



US00D964571S

(12) **United States Design Patent**
Bierman

(10) **Patent No.:** **US D964,571 S**
(45) **Date of Patent:** **** Sep. 20, 2022**

- (54) **CATHETER SECUREMENT PAD**
- (71) Applicant: **Maddoc Medical Products, Inc.**, Los Angeles, CA (US)
- (72) Inventor: **Steven Bierman**, Del Mar, CA (US)
- (73) Assignee: **Maddoc Medical Products, Inc.**, Los Angeles, CA (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/692,603**
- (22) Filed: **May 28, 2019**
- (51) **LOC (13) Cl.** **24-04**
- (52) **U.S. Cl.**
USPC **D24/189**
- (58) **Field of Classification Search**
USPC D24/127–130, 132, 188–189; 604/187, 604/227, 180, 174; 602/58–59, 46, 41, 602/52; 128/DIG. 26
CPC A61M 25/02; A61M 2025/0206; A61M 2025/024; A61M 2025/0266; A61M 2025/028; A61M 2025/0246; Y10S 128/26
See application file for complete search history.

- D409,754 S * 5/1999 Dunshee D24/189
- D410,087 S * 5/1999 Dunshee D24/189
- 5,981,822 A * 11/1999 Addison A61F 13/0203 602/56
- 6,011,194 A * 1/2000 Buglino A61F 13/0209 428/326

(Continued)

OTHER PUBLICATIONS

Bard Securis stabilization device web page screen shots, taken from <https://www.bardaccess.com/products/procedural/securis> on Jun. 12, 2020.

Primary Examiner — Nathan M Johnston
(74) *Attorney, Agent, or Firm* — Master Key IP, LLP; Jeromye V. Sartain

(57) **CLAIM**

The ornamental design for a catheter securement pad, as shown and described.

DESCRIPTION


FIG. 1 is an exploded perspective view showing an exemplary embodiment of my new catheter securement pad design; FIG. 2 is a top view of the catheter securement pad with the peel-off layers removed for ease of illustration; FIG. 3 is a bottom view of the catheter securement pad with the peel-off layers removed for ease of illustration; FIG. 4 is a left side view of the catheter securement pad with the peel-off layers removed for ease of illustration; FIG. 5 is a right side view of the catheter securement pad with the peel-off layers removed for ease of illustration; FIG. 6 is a front view of the catheter securement pad with the peel-off layers removed for ease of illustration; and, FIG. 7 is a rear view of the catheter securement pad with the peel-off layers removed for ease of illustration. The broken lines show portions of the catheter securement pad that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 4,126,130 A * 11/1978 Cowden A61F 13/04 602/8
- D267,510 S * 1/1983 Golub D24/189
- 4,627,842 A 12/1986 Katz
- 4,997,421 A 3/1991 Palsrok et al.
- 5,056,510 A * 10/1991 Gilman A61F 13/0246 D24/189
- 5,533,962 A * 7/1996 Peterman A61F 13/0203 602/44
- 5,702,356 A * 12/1997 Hathman A61F 13/0206 602/41
- 5,855,591 A 1/1999 Bierman
- D408,541 S * 4/1999 Dunshee D24/189

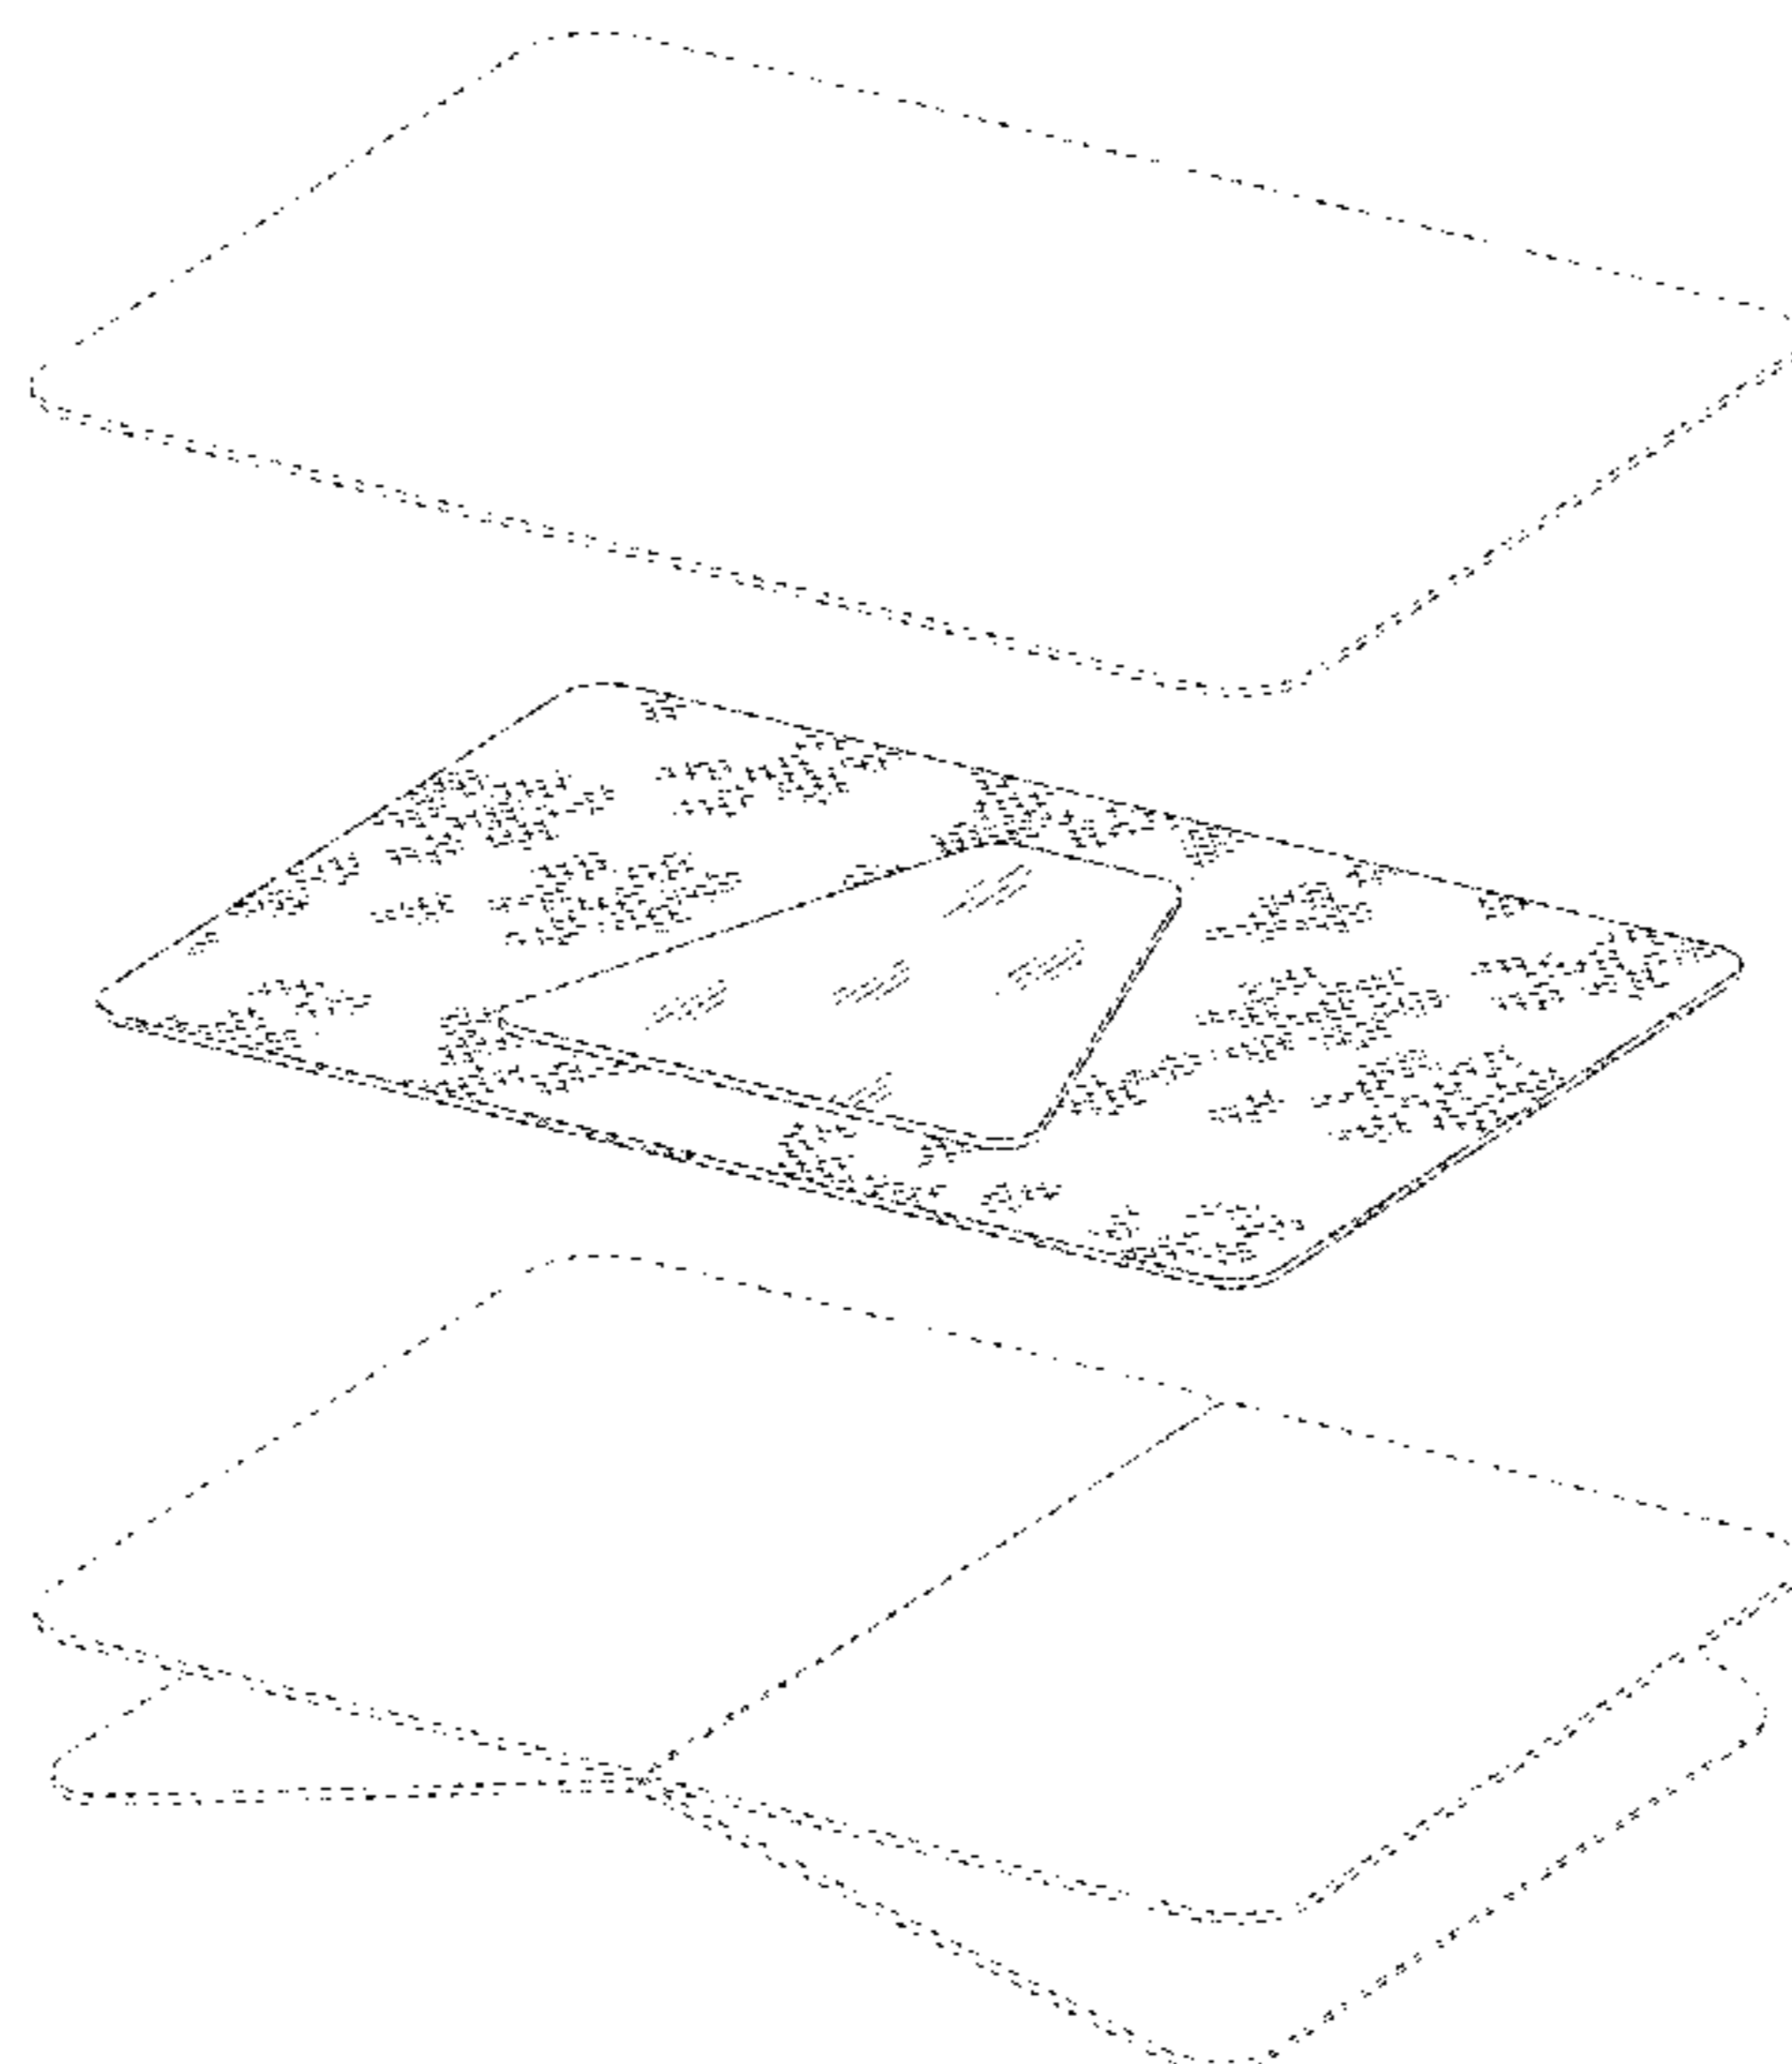

(56)

References Cited

U.S. PATENT DOCUMENTS

D424,699 S *	5/2000	Allen	D24/189	D604,423 S *	11/2009	Dunshee	D24/189
6,099,509 A *	8/2000	Brown, Jr.	A61M 25/02 602/41	8,394,067 B2	3/2013	Bracken et al.		
6,224,571 B1	5/2001	Bierman			8,486,004 B1	7/2013	Propp		
6,284,941 B1 *	9/2001	Cox	A61K 9/7084 602/41	8,608,704 B2	12/2013	Bierman		
6,413,240 B1	7/2002	Bierman et al.			8,608,705 B2	12/2013	Peters et al.		
D492,786 S *	7/2004	Saim	D24/189	9,017,290 B2	4/2015	Peters et al.		
6,786,892 B2	9/2004	Bierman			D746,996 S *	1/2016	Karlsson	D24/189
D513,639 S *	1/2006	Saim	D24/189	9,895,514 B2	2/2018	Bierman et al.		
D515,701 S *	2/2006	Horhota	D24/189	10,232,145 B2	3/2019	Bierman et al.		
7,153,291 B2	12/2006	Bierman			10,463,837 B2	11/2019	Bierman et al.		
D573,260 S *	7/2008	Dunshee	D24/189	10,561,825 B2	2/2020	Bierman et al.		
D574,962 S *	8/2008	Atkins	D24/189	D898,924 S *	10/2020	Hinds	D24/189
D578,651 S *	10/2008	Dunshee	D24/189	D943,751 S *	2/2022	Caneppele	D24/189
D582,560 S *	12/2008	Sachi	D24/189	2006/0247577 A1	11/2006	Wright		
7,531,711 B2 *	5/2009	Sigurjonsson	A61L 15/58 602/41	2010/0298778 A1 *	11/2010	Bracken	A61M 25/02 604/180
					2011/0319830 A1	12/2011	Peters et al.		
					2013/0204190 A1	8/2013	Wilborn et al.		
					2020/0179655 A1	6/2020	Bierman et al.		

* cited by examiner

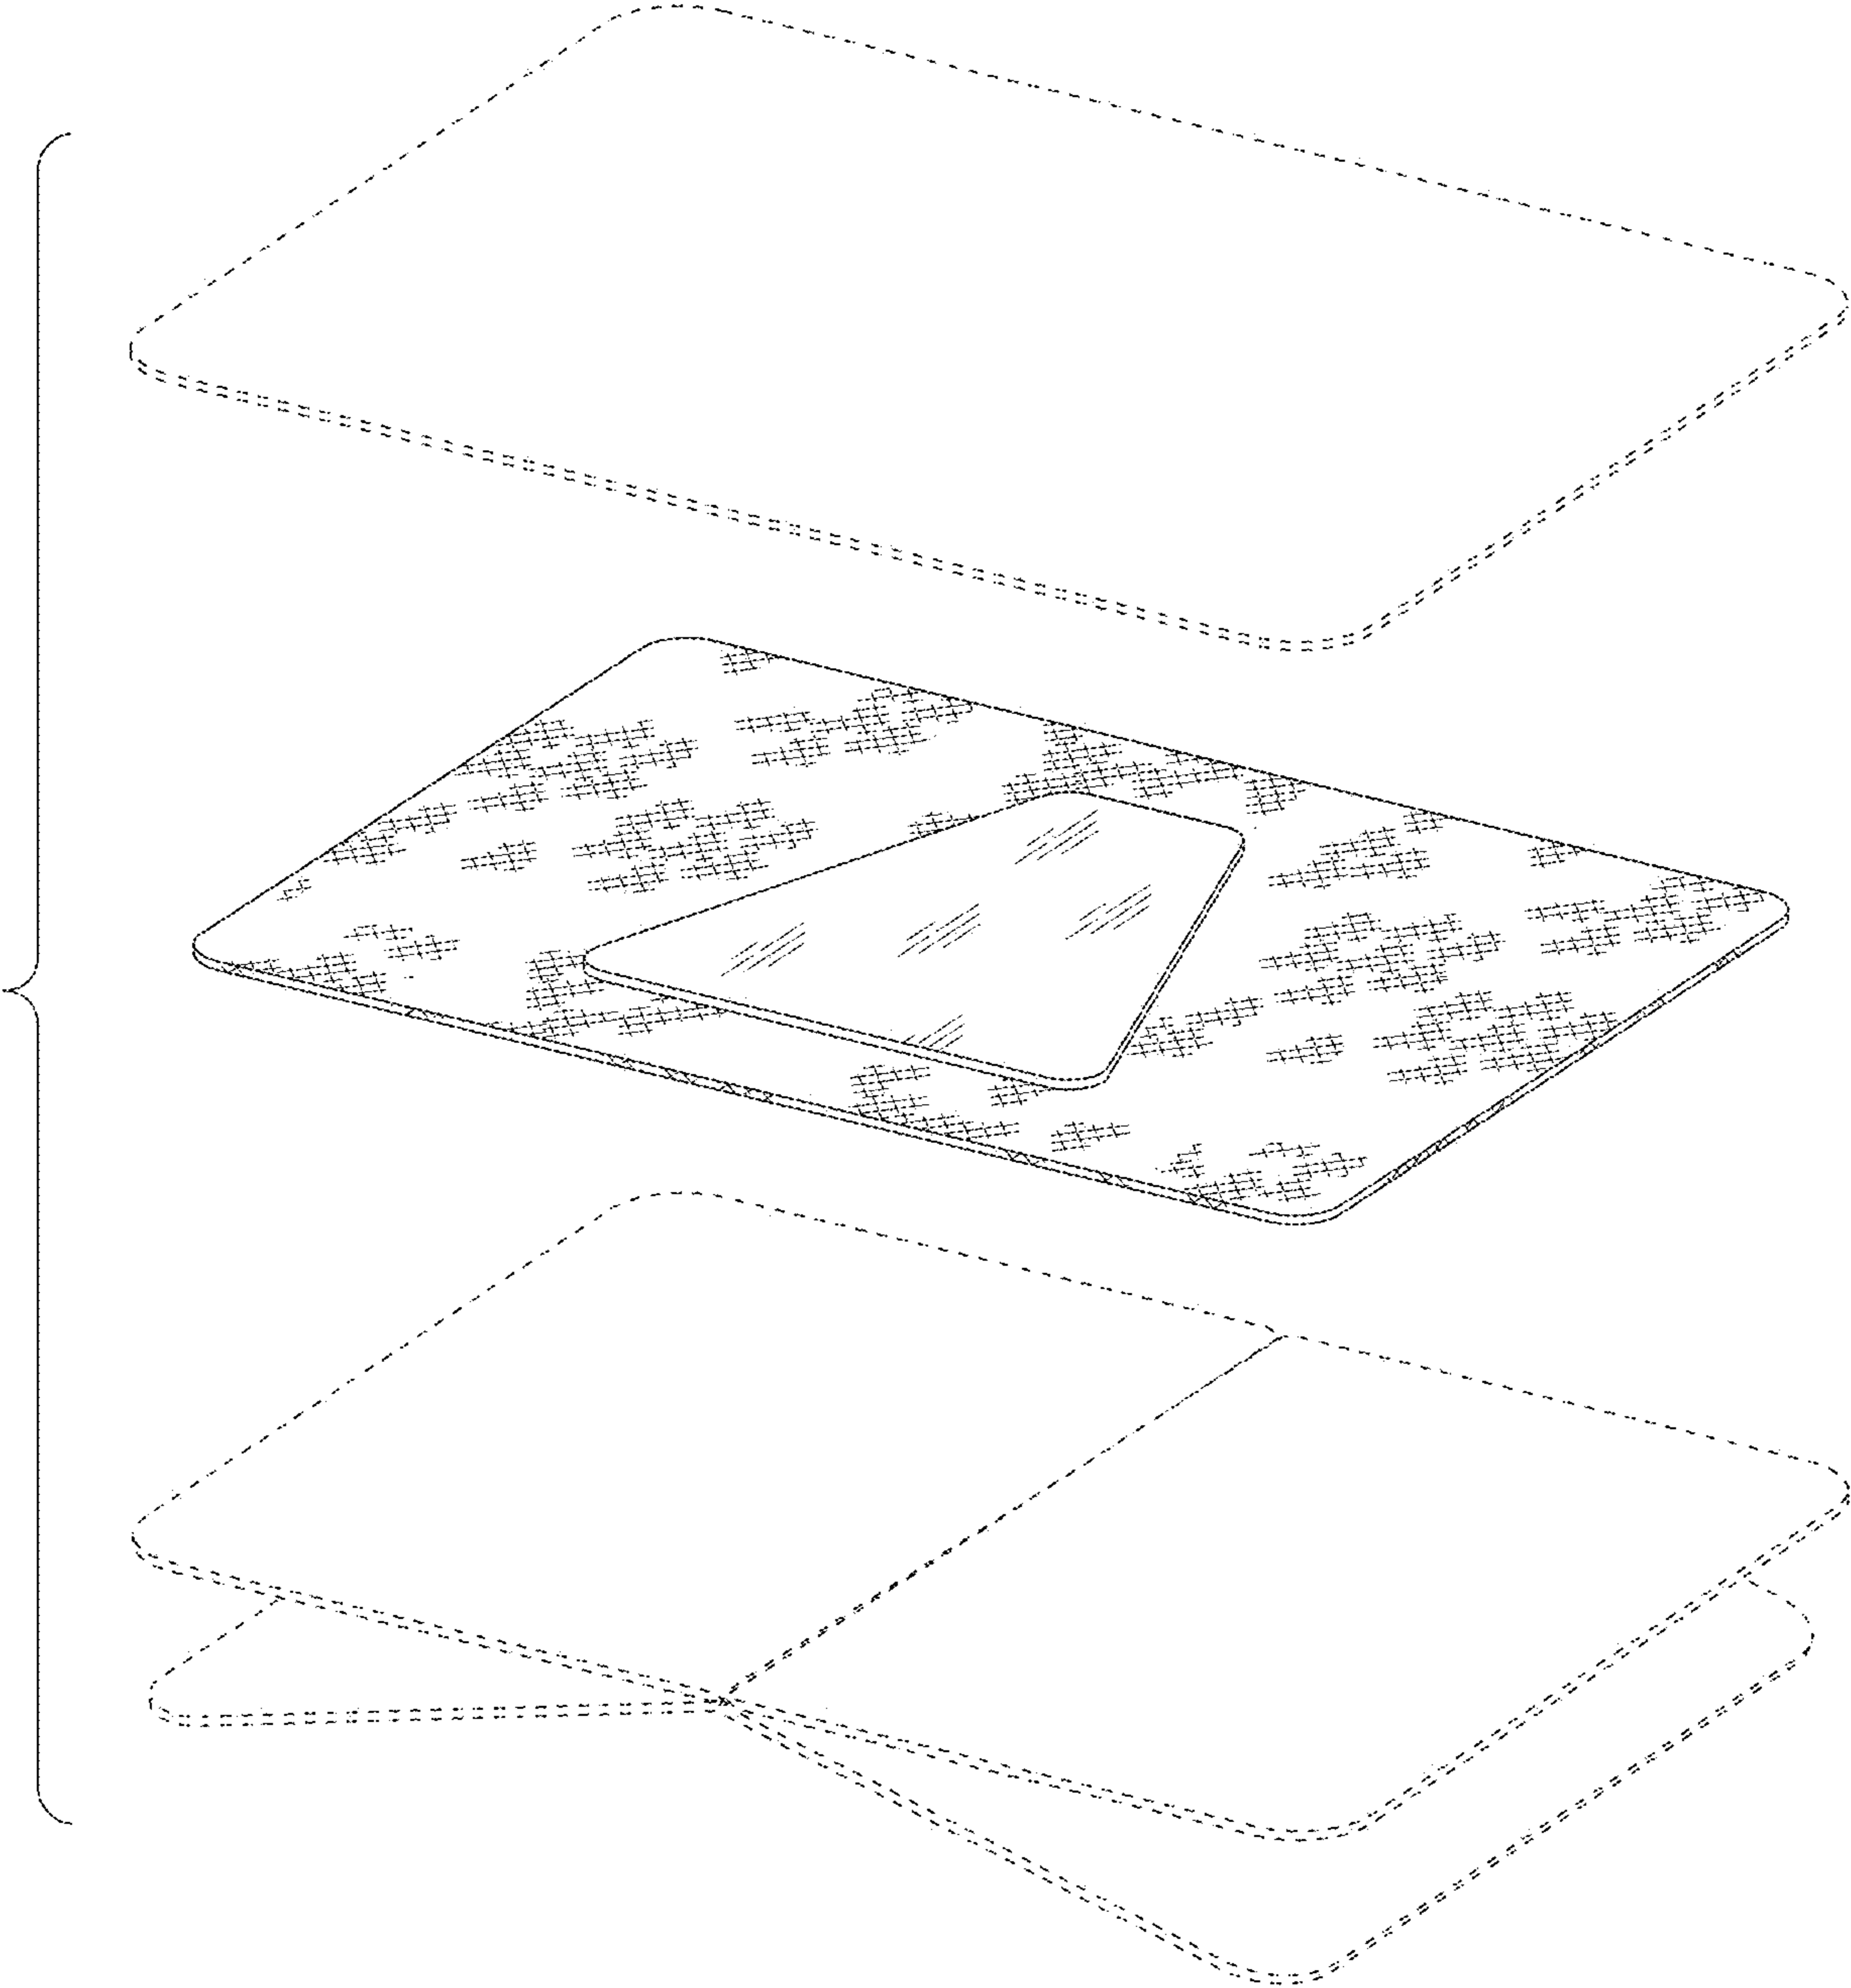


Fig. 1

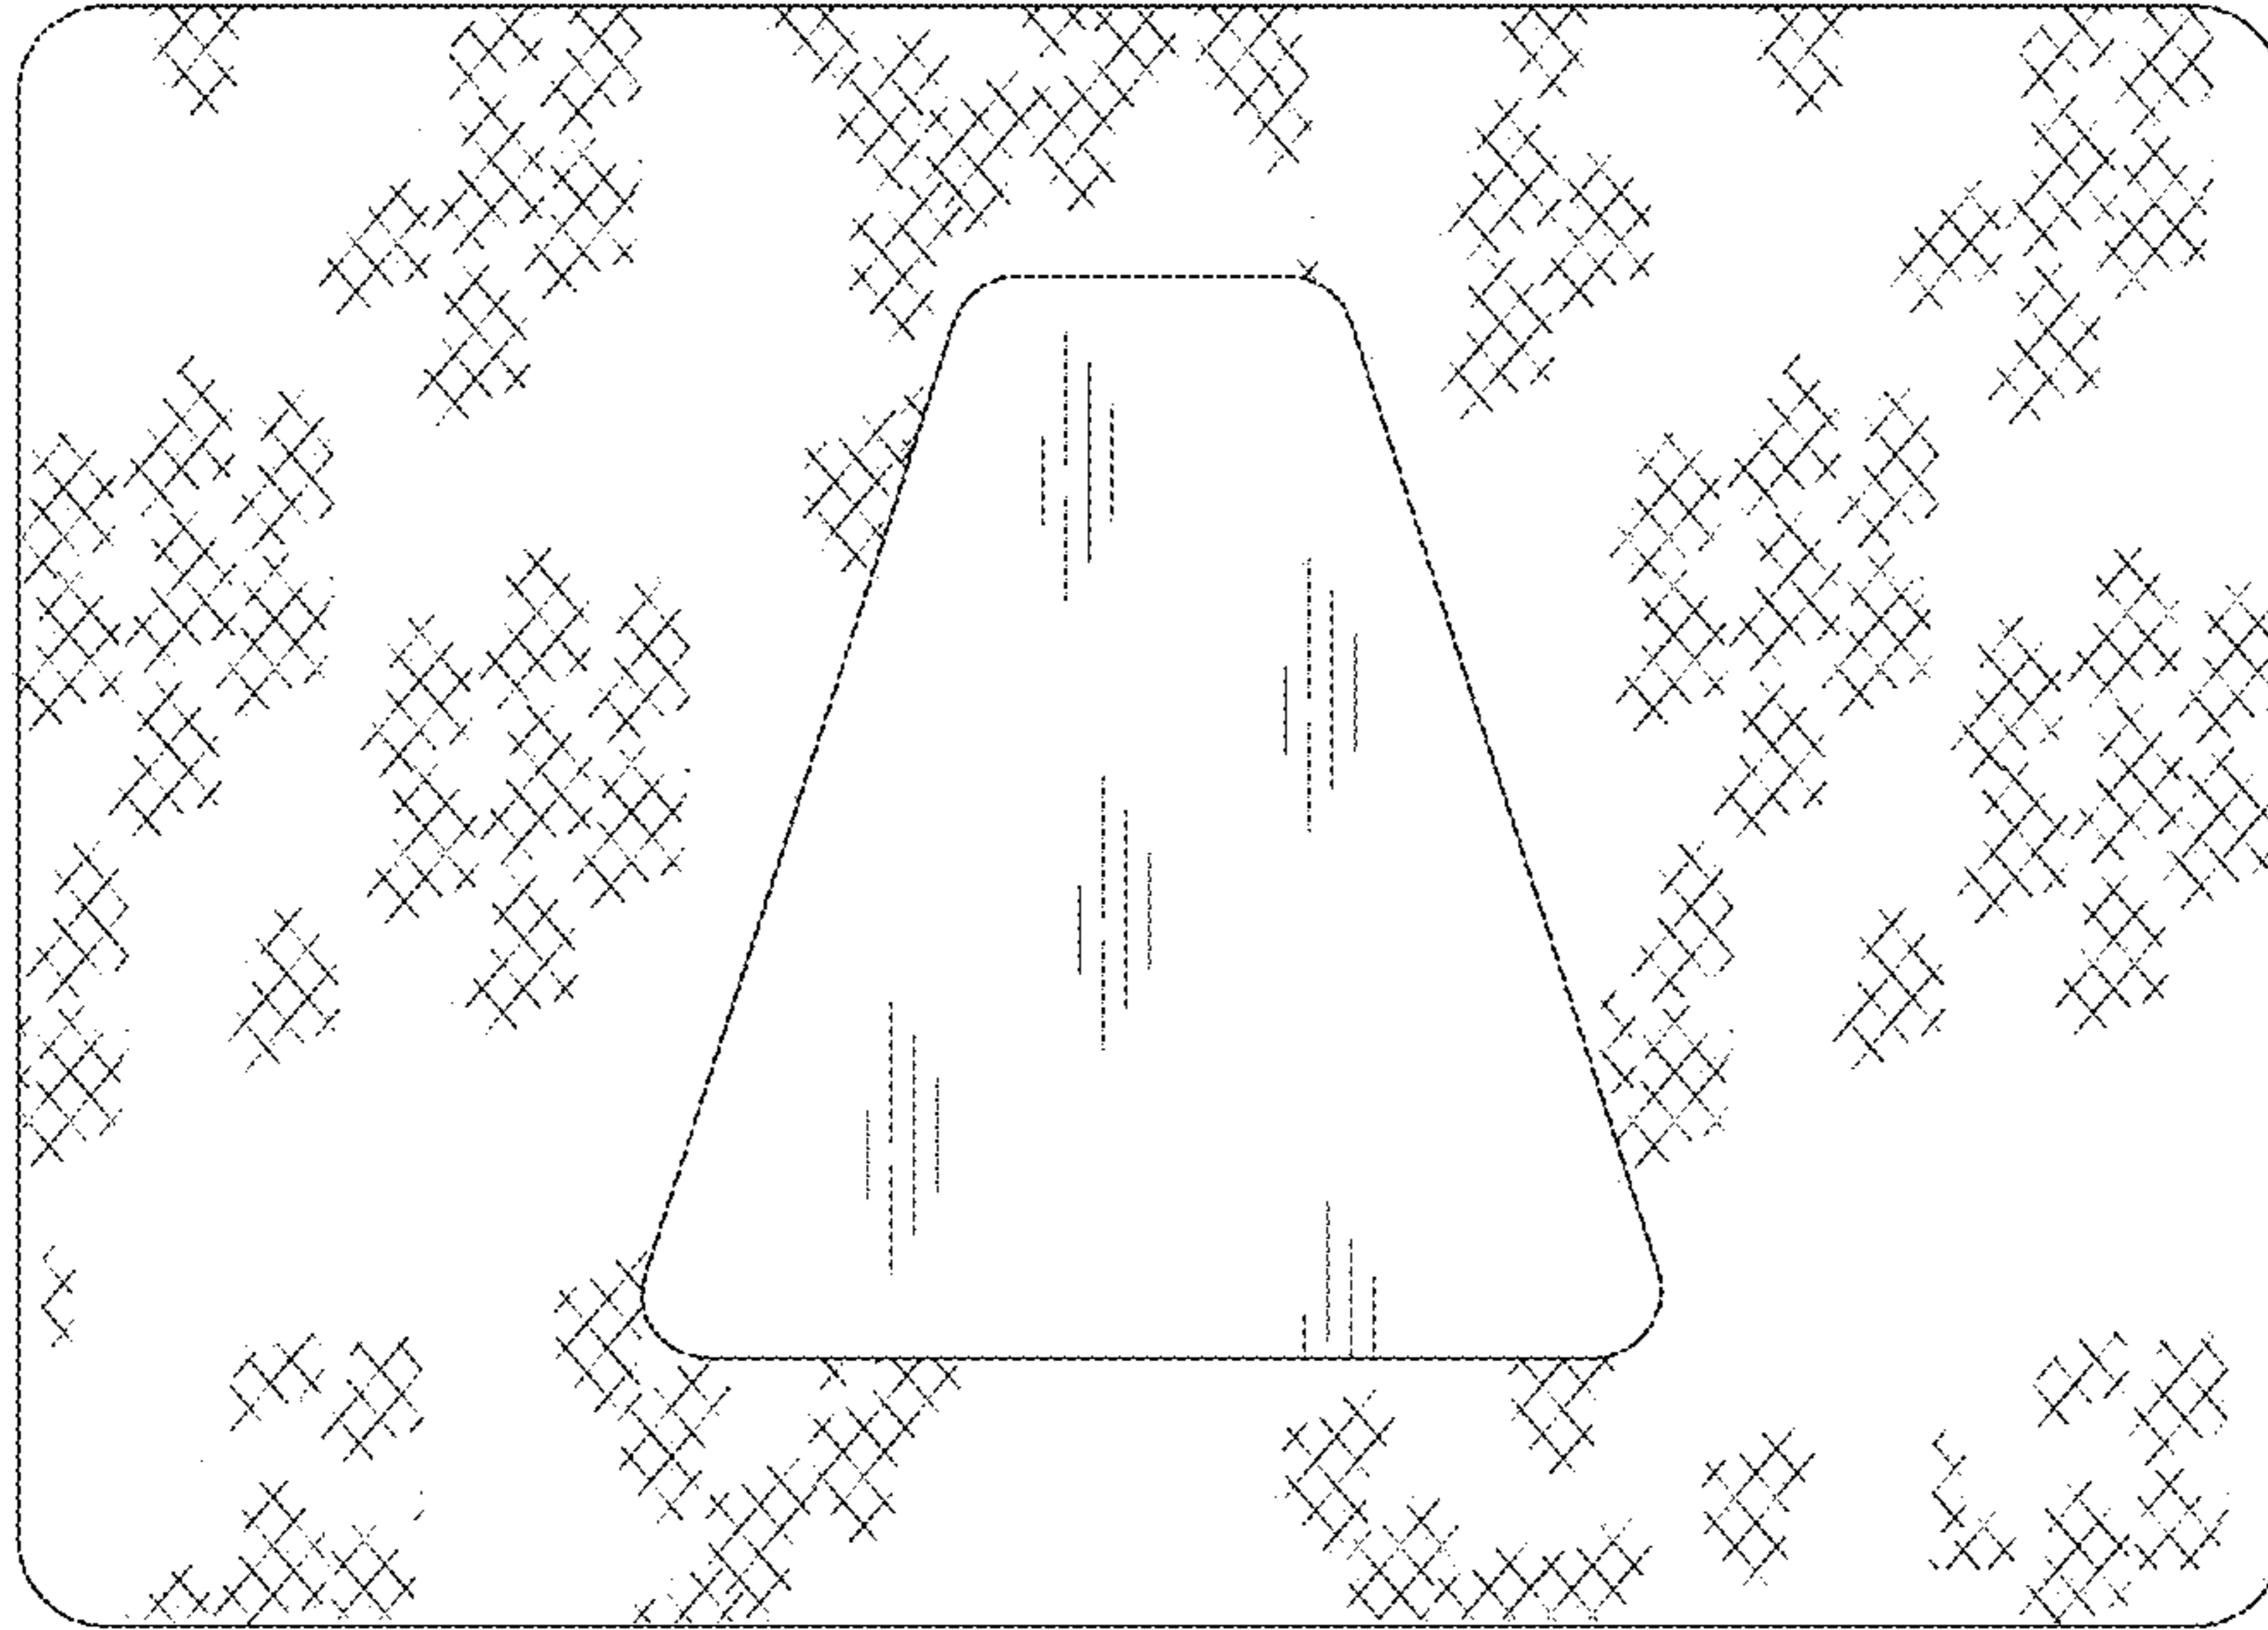


Fig. 2

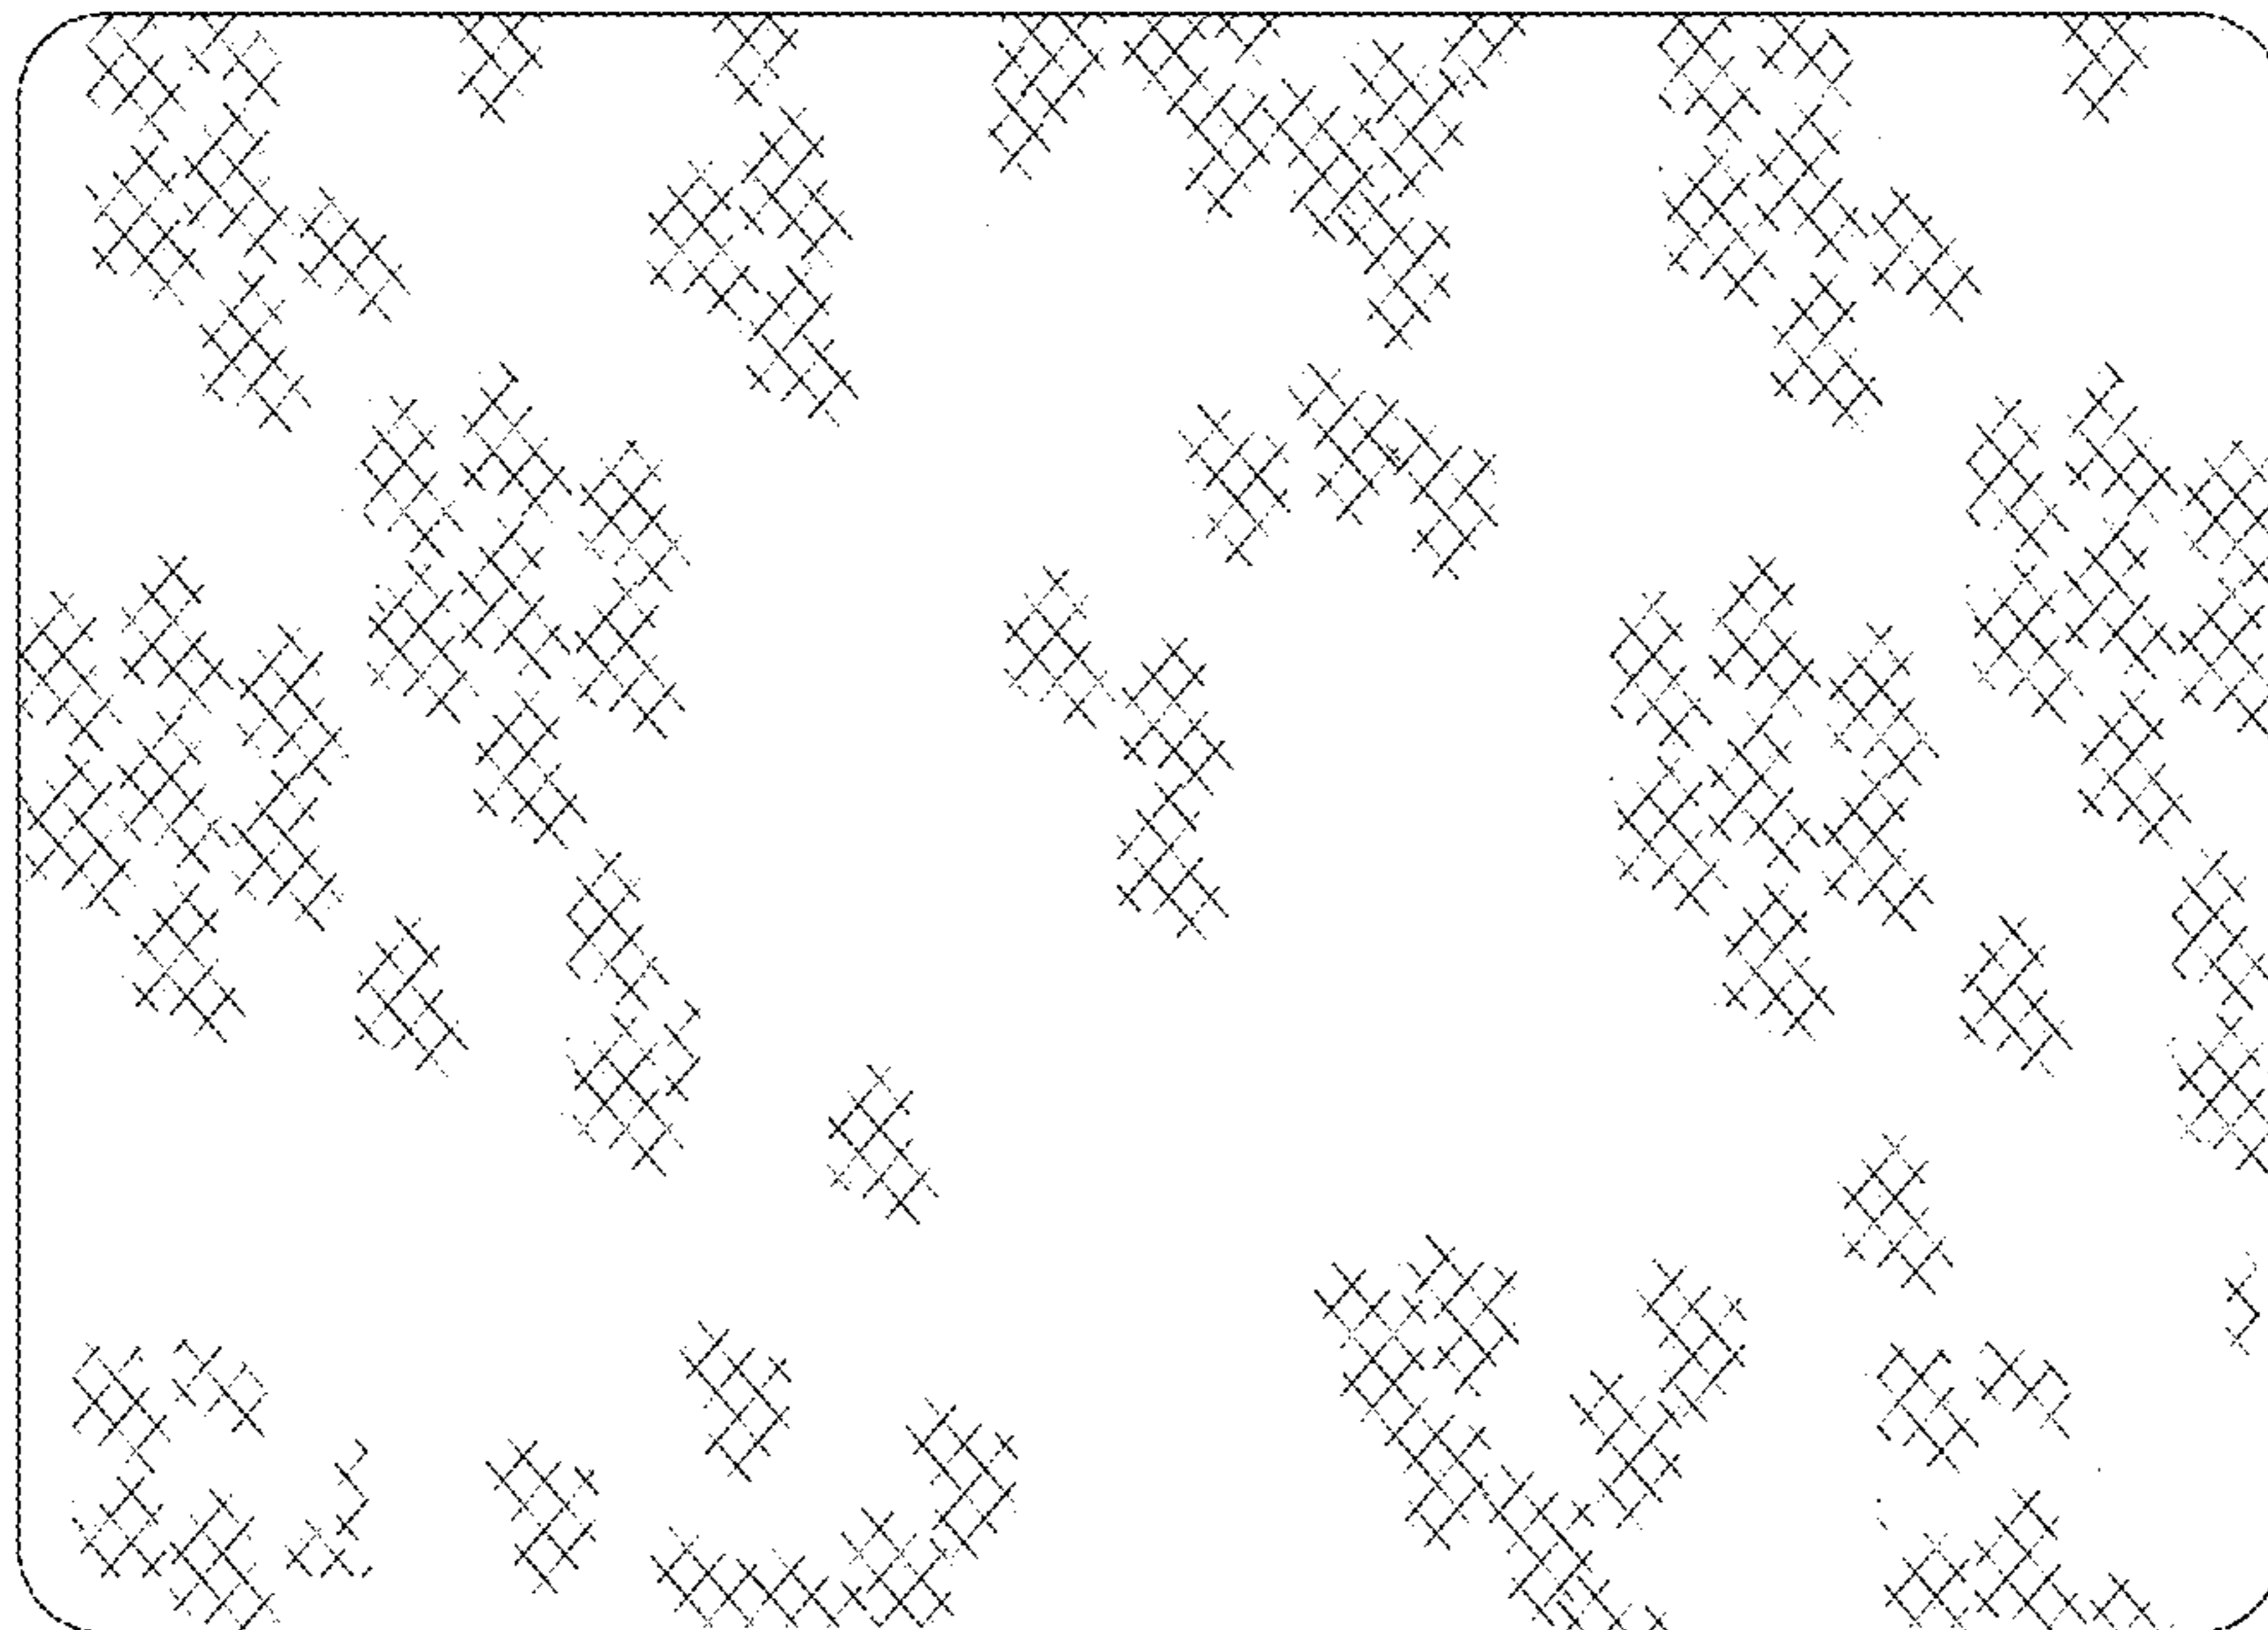


Fig. 3



Fig. 4

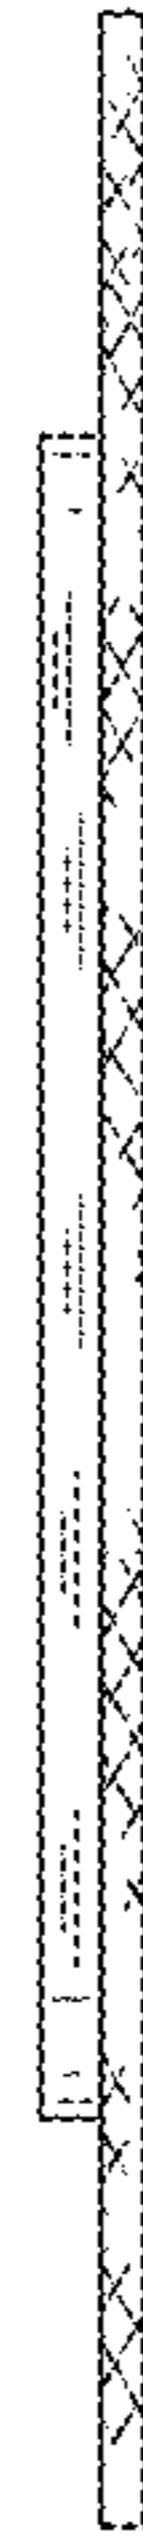


Fig. 5

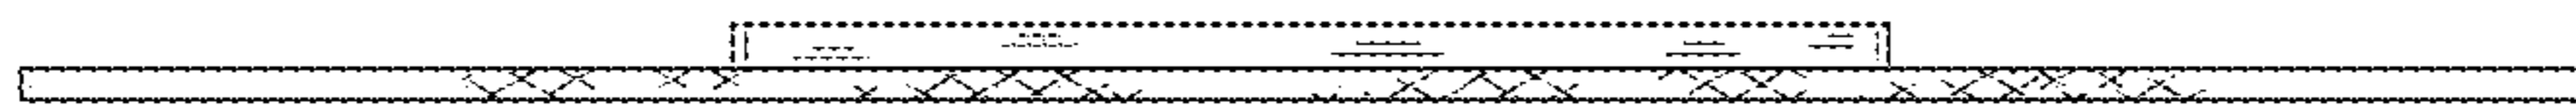


Fig. 6

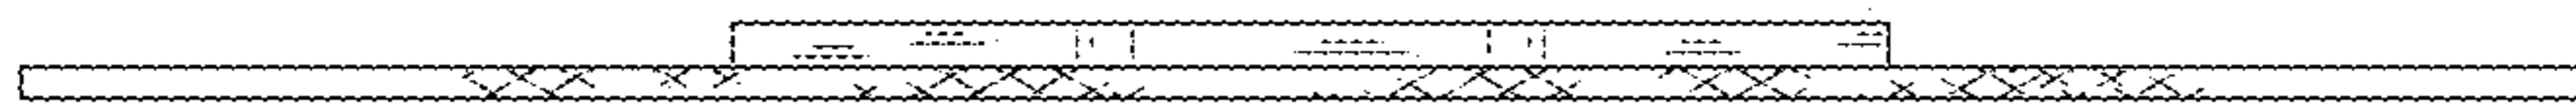


Fig. 7