

US00D966307S

(12) **United States Design Patent** (10) **Patent No.:** **US D966,307 S**
McIver et al. (45) **Date of Patent:** **** Oct. 11, 2022**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH A GRAPHICAL USER INTERFACE**

(71) Applicant: **INSPIRE MEDICAL SYSTEMS, INC.**, Golden Valley, MN (US)
(72) Inventors: **Jordan McIver**, Blaine, MN (US); **Michael Coleman**, Shoreview, MN (US); **John Rondoni**, Plymouth, MN (US); **Isabel Ancona**, Boston, MA (US)

(73) Assignee: **INSPIRE MEDICAL SYSTEMS, INC.**, Golden Valley, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/772,824**

(22) Filed: **Mar. 4, 2021**

(51) **LOC (13) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495
CPC A61B 5/02; G16H 10/60; G16H 50/00; G16H 10/00; G16H 20/00; G16H 20/30
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D573,599	S	*	7/2008	Williams	D14/486
D600,248	S	*	9/2009	Scalisi	D14/485
D634,749	S	*	3/2011	Brown	D14/486
D635,579	S	*	4/2011	Scalisi	D14/486
D637,603	S	*	5/2011	Godgart	D14/486
D640,265	S	*	6/2011	Brouwers	D14/486
D667,837	S	*	9/2012	Magee	D14/486
D667,838	S	*	9/2012	Magee	D14/486
D674,810	S	*	1/2013	Goodspeed	D14/486
D685,812	S	*	7/2013	Bork	D14/486
D689,065	S	*	9/2013	Glaeske	D14/486

D689,081	S	*	9/2013	Rhee	D14/486
D714,339	S	*	9/2014	Hendrickson	D14/487
D760,248	S	*	6/2016	Suarez	D14/485
9,452,293	B2		9/2016	Rondoni et al.		
D774,527	S	*	12/2016	Klein	D14/490
D774,528	S	*	12/2016	Klein	D14/490
D774,529	S	*	12/2016	Klein	D14/490
9,839,786	B2		12/2017	Rondoni et al.		
D832,865	S		11/2018	Dieken et al.		
D833,461	S		11/2018	Dieken et al.		
D840,426	S		2/2019	Dieken et al.		
D869,490	S		12/2019	Rondoni et al.		
D871,433	S		12/2019	Rondoni et al.		
D871,434	S		12/2019	Rondoni et al.		
D890,775	S	*	7/2020	Clay	D14/485
2006/0271480	A1	*	11/2006	Allin	G06Q 20/14 705/40

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2021016558 A1 1/2021

Primary Examiner — Rachel A. Voorhies
(74) *Attorney, Agent, or Firm* — Dicke, Billig & Czaja, PLLC

(57) **CLAIM**


The ornamental design for a display screen or portion thereof with a graphical user interface, as shown and described.

DESCRIPTION

The sole FIGURE is a front view of a display screen or portion thereof with a graphical user interface showing our new design.

In the FIGURE, the outermost broken lines show a display screen or portion thereof and form no part of the claimed design. The remaining broken lines show elements of the graphical user interface that form no part of the claimed design.

1 Claim, 1 Drawing Sheet

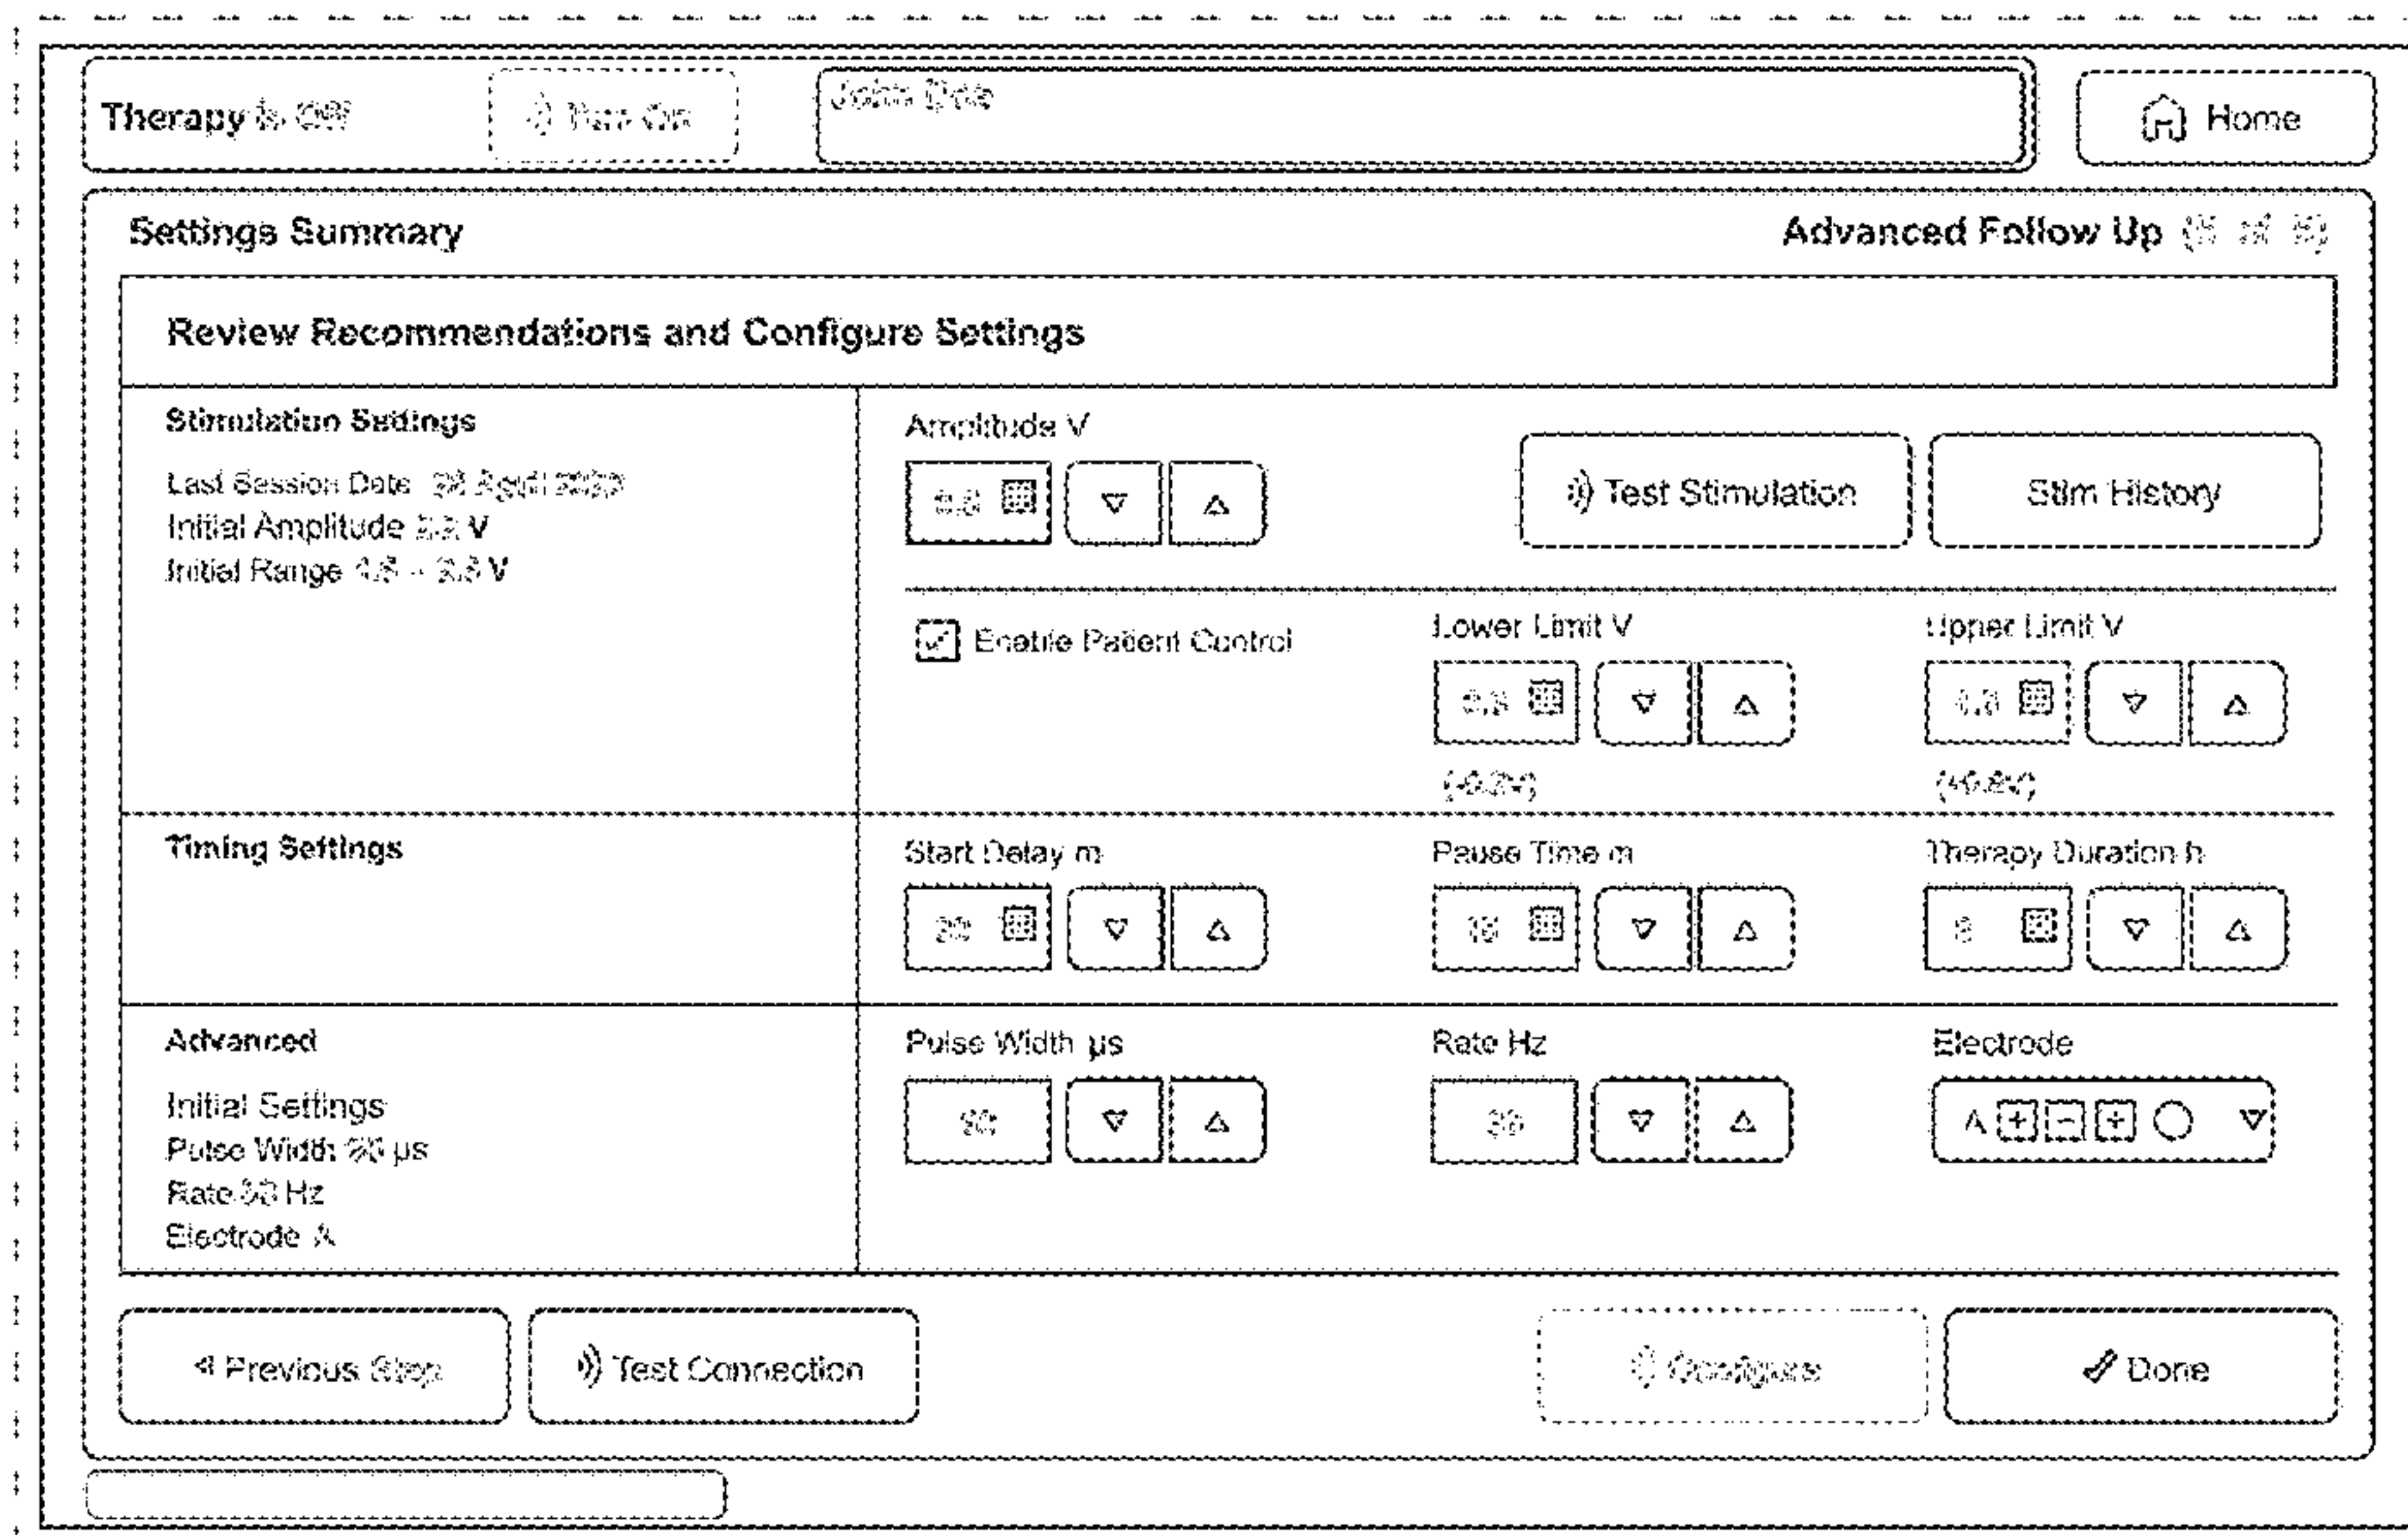

(56)

References Cited

U.S. PATENT DOCUMENTS

2009/0164249 A1* 6/2009 Hunt G06Q 10/00
705/3
2010/0185183 A1* 7/2010 Aime A61M 5/14276
604/891.1
2016/0367184 A1* 12/2016 Lim G16H 50/30
2017/0263144 A1* 9/2017 Horan G09B 5/065
2019/0175026 A1 6/2019 Verzal et al.
2019/0365228 A1 12/2019 Rondoni et al.
2019/0371478 A1 12/2019 Rondoni et al.
2019/0371479 A1 12/2019 Rondoni et al.

* cited by examiner

Therapy

Test Connection

System Diagnostics

Home

Advanced Follow Up (5 of 6)

Review Recommendations and Configure Settings

<p>Stimulation Settings</p> <p>Last Session Date 28 Sept 2020</p> <p>Initial Amplitude 30.2 V</p> <p>Initial Range 1.8 - 2.5 V</p>	<p style="text-align: center;">Amplitude V</p> <div style="display: flex; justify-content: space-around;"> <div> 30.2</div> <div><input type="text"/></div> <div><input type="button" value="v"/></div> <div><input type="button" value="Δ"/></div> </div> <p><input checked="" type="checkbox"/> Enable Patient Control</p> <div style="display: flex; justify-content: space-between;"> <div style="text-align: center;"> <p>Lower Limit V</p> <div style="display: flex; justify-content: space-around;"> <div> 0.0</div> <div><input type="text"/></div> <div><input type="button" value="v"/></div> <div><input type="button" value="Δ"/></div> </div> <p>(-0.2V)</p> </div> <div style="text-align: center;"> <p>Upper Limit V</p> <div style="display: flex; justify-content: space-around;"> <div> 1.0</div> <div><input type="text"/></div> <div><input type="button" value="v"/></div> <div><input type="button" value="Δ"/></div> </div> <p>(+0.8V)</p> </div> </div>
<p>Timing Settings</p>	<p style="text-align: center;">Test Stimulation</p> <p style="text-align: center;"> Stim History</p>
<p>Advanced</p> <p>Initial Settings</p> <p>Pulse Width 300 μs</p> <p>Rate 30 Hz</p> <p>Electrode A</p>	<p style="text-align: center;">Timing</p> <div style="display: flex; justify-content: space-between;"> <div style="text-align: center;"> <p>Start Delay m</p> <div style="display: flex; justify-content: space-around;"> <div> 300</div> <div><input type="text"/></div> <div><input type="button" value="m"/></div> <div><input type="button" value="Δ"/></div> </div> </div> <div style="text-align: center;"> <p>Pause Time m</p> <div style="display: flex; justify-content: space-around;"> <div> 100</div> <div><input type="text"/></div> <div><input type="button" value="m"/></div> <div><input type="button" value="Δ"/></div> </div> </div> <div style="text-align: center;"> <p>Therapy Duration h</p> <div style="display: flex; justify-content: space-around;"> <div> 0</div> <div><input type="text"/></div> <div><input type="button" value="h"/></div> <div><input type="button" value="Δ"/></div> </div> </div> </div>
<p>Advanced</p> <p>Initial Settings</p> <p>Pulse Width 300 μs</p> <p>Rate 30 Hz</p> <p>Electrode A</p>	<p style="text-align: center;">Advanced</p> <div style="display: flex; justify-content: space-between;"> <div style="text-align: center;"> <p>Pulse Width μs</p> <div style="display: flex; justify-content: space-around;"> <div> 300</div> <div><input type="text"/></div> <div><input type="button" value="μs"/></div> <div><input type="button" value="Δ"/></div> </div> </div> <div style="text-align: center;"> <p>Rate Hz</p> <div style="display: flex; justify-content: space-around;"> <div> 30</div> <div><input type="text"/></div> <div><input type="button" value="Hz"/></div> <div><input type="button" value="Δ"/></div> </div> </div> <div style="text-align: center;"> <p>Electrode</p> <div style="display: flex; justify-content: space-around;"> <div> A</div> <div><input type="text"/></div> <div><input type="button" value="A"/></div> <div><input type="button" value="Δ"/></div> </div> </div> </div>

Previous Step

Test Connection

Configure

Done