



US00D967181S

(12) **United States Design Patent**
Lin et al.(10) **Patent No.:** US D967,181 S
(45) **Date of Patent:** ** Oct. 18, 2022(54) **HEALTH MANAGEMENT TERMINAL DISPLAY SCREEN WITH TRANSITIONAL GRAPHICAL USER INTERFACE**(71) Applicant: **Jiangyu Kangjian Innovation Medical Technology(Chengdu) Co., Ltd,** Chengdu (CN)(72) Inventors: **Chi-Fan Lin**, New Taipei (TW); **Ying-Wei Sheng**, New Taipei (TW)(73) Assignee: **Jiangyu Kangjian Innovation Medical Technology(Chengdu) Co., Ltd,** Chengdu (CN)(**) Term: **15 Years**(21) Appl. No.: **29/731,577**(22) Filed: **Apr. 16, 2020**(30) **Foreign Application Priority Data**

Oct. 21, 2019 (CN) 201930573063.X

(51) LOC (13) Cl. **14-04**

(52) U.S. Cl.

USPC **D14/488**(58) **Field of Classification Search**USPC D14/485-95
CPC G06F 3/48; G06F 3/0481; G06F 3/04812;
G06F 3/04815; G06F 3/04817; G06F
3/0482; G06F 3/0483; G06F 3/0484;
G06F 3/04842; G06F 3/04845; G06F
3/04847; G06F 3/0485; G06F 3/0486;
G06F 3/0487; G06F 3/0488; G06F
3/04883; G06F 3/04886

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D390,548 S * 2/1998 Maekawa D14/488
D425,499 S * 5/2000 Millington D14/488D441,763 S * 5/2001 Kahn D14/488
6,232,970 B1 * 5/2001 Bodnar G06F 3/0236
715/708
D523,868 S * 6/2006 Kuroda D14/485
D549,712 S * 8/2007 Kim D14/485
D573,152 S * 7/2008 Jasinski D14/485
(Continued)

OTHER PUBLICATIONS

Diatron Aquila Training Video Basic—Diatron, <https://www.youtube.com/watch?v=dg07zN-JPXg> (Year: 2017).*

(Continued)

Primary Examiner — Melanie H Tung*Assistant Examiner* — Darmawan Truong(74) *Attorney, Agent, or Firm* — ScienBiziP, P.C.

(57)

CLAIM


The ornamental design for a health management terminal display screen with transitional graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a first image of the health management terminal display screen with transitional graphical user interface; FIG. 2 is a second image thereof; FIG. 3 is a third image thereof; FIG. 4 is a fourth image thereof; FIG. 5 is a fifth image thereof; and, FIG. 6 is a sixth image thereof.

The appearance of the transitional image sequentially transitions between the images shown in FIGS. 1-6. The process or period in which one image transitions to another image forms no part of the claimed design.

The broken lines showing the health management terminal display screen form no part of the claim design. The remaining broken lines showing text and portions of the graphical user interface form no part of the claimed design.

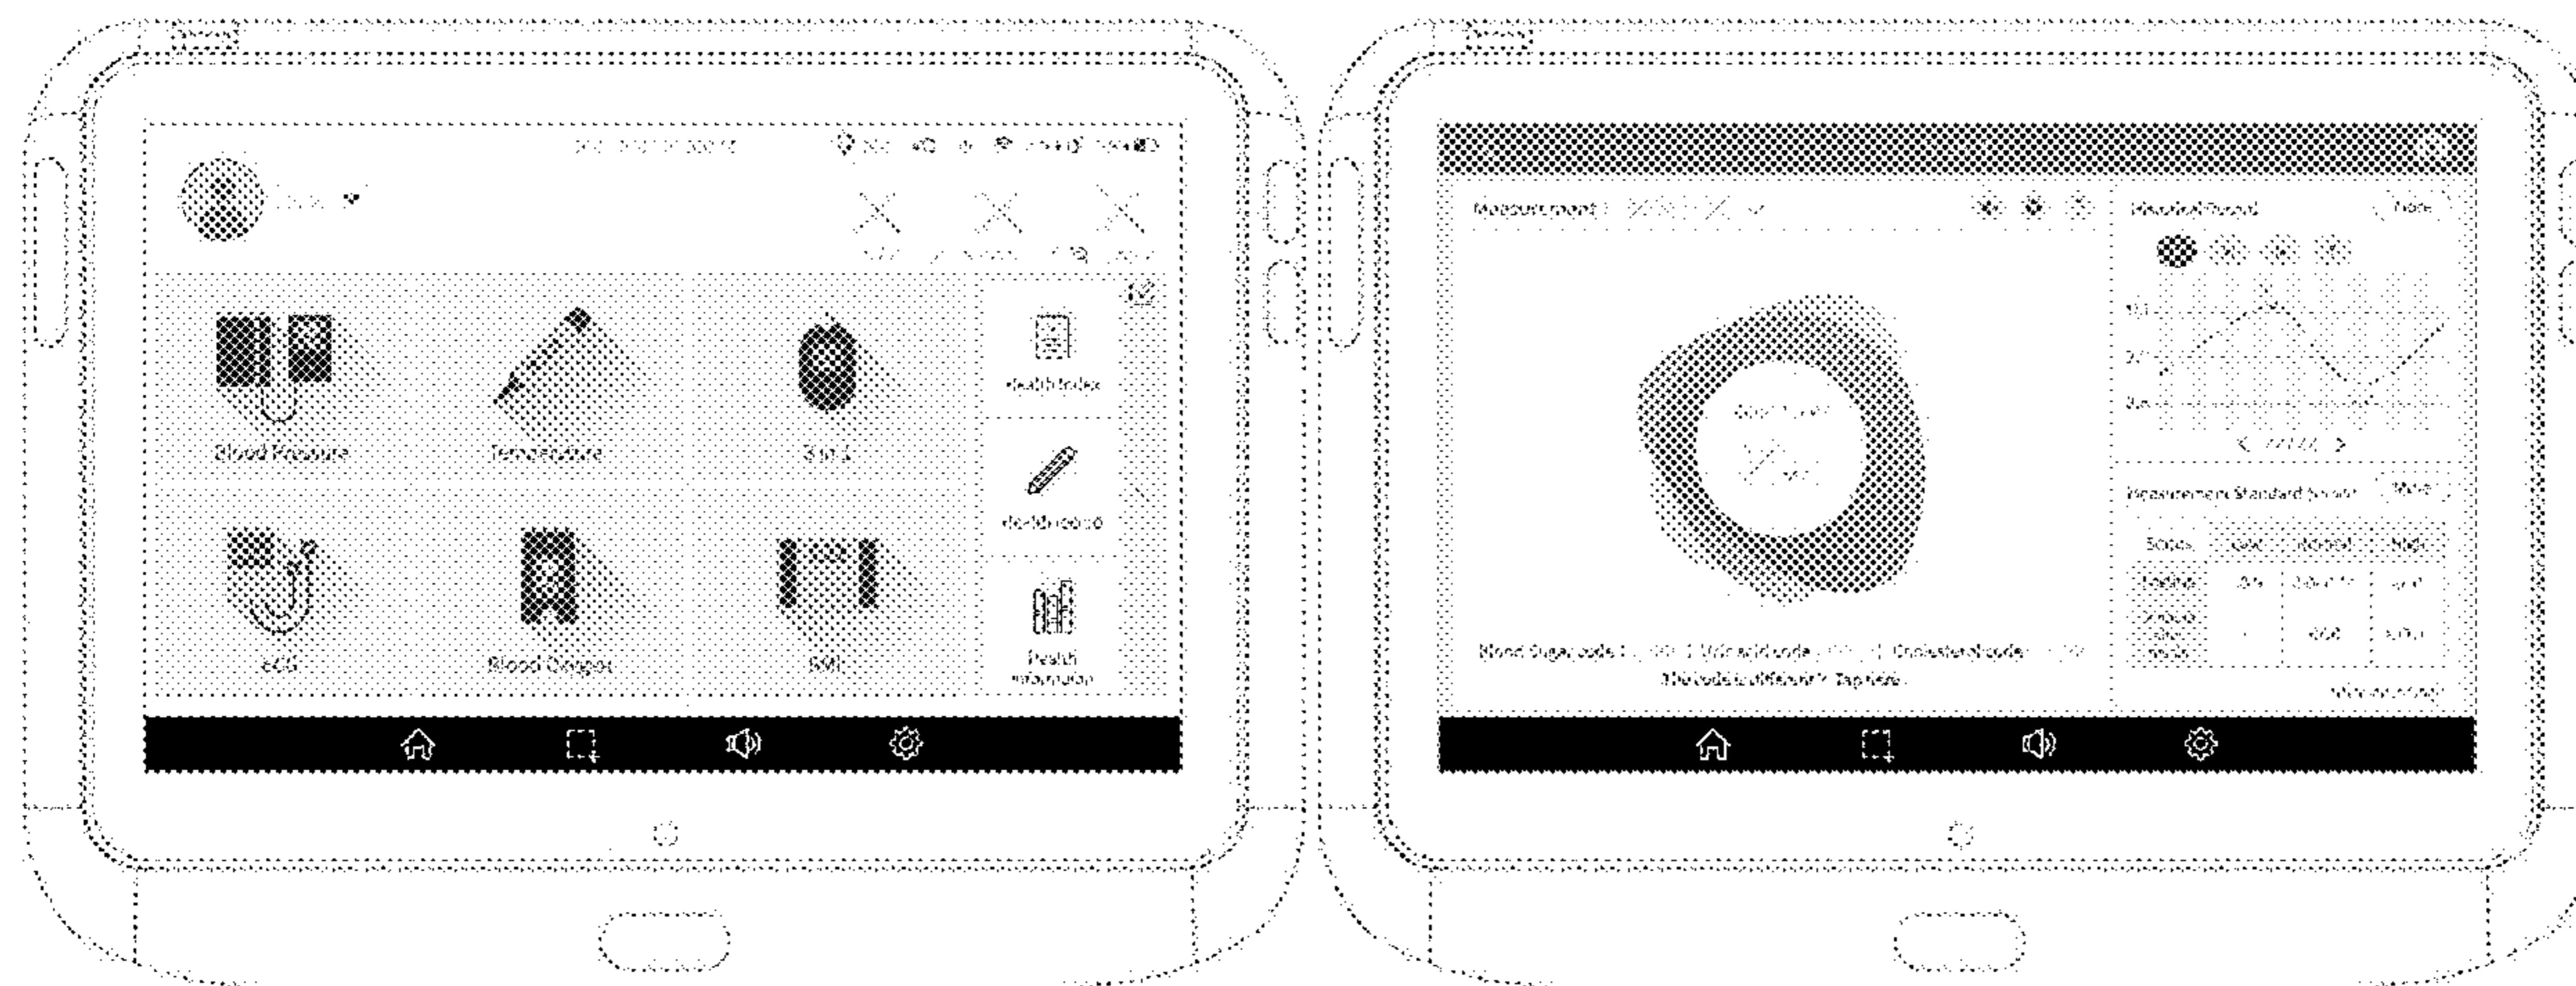1 Claim, 6 Drawing Sheets

(56)

References Cited

U.S. PATENT DOCUMENTS

D591,304 S * 4/2009 Banks D14/485
D597,098 S * 7/2009 Su D14/492
D605,652 S * 12/2009 Plaisted D14/485
D607,464 S * 1/2010 Tang D14/492
D636,779 S * 4/2011 Boush D14/486
D781,339 S * 3/2017 Li D14/487
D927,507 S * 8/2021 Norman D14/485
D927,523 S * 8/2021 Mukaty D14/486
D928,815 S * 8/2021 Esteve Velázquez D14/486
D941,849 S * 1/2022 Knowles D14/492
2002/0002453 A1 * 1/2002 Lazaridis G06F 40/279
707/999.005
2015/0039176 A1 * 2/2015 Fish G07C 5/008
701/31.6

OTHER PUBLICATIONS

Bonacea Medical Diary—Ideamotive, <https://dribbble.com/shots/5043123-Bonacea-Medical-Diary> (Year: 2018).*

* cited by examiner

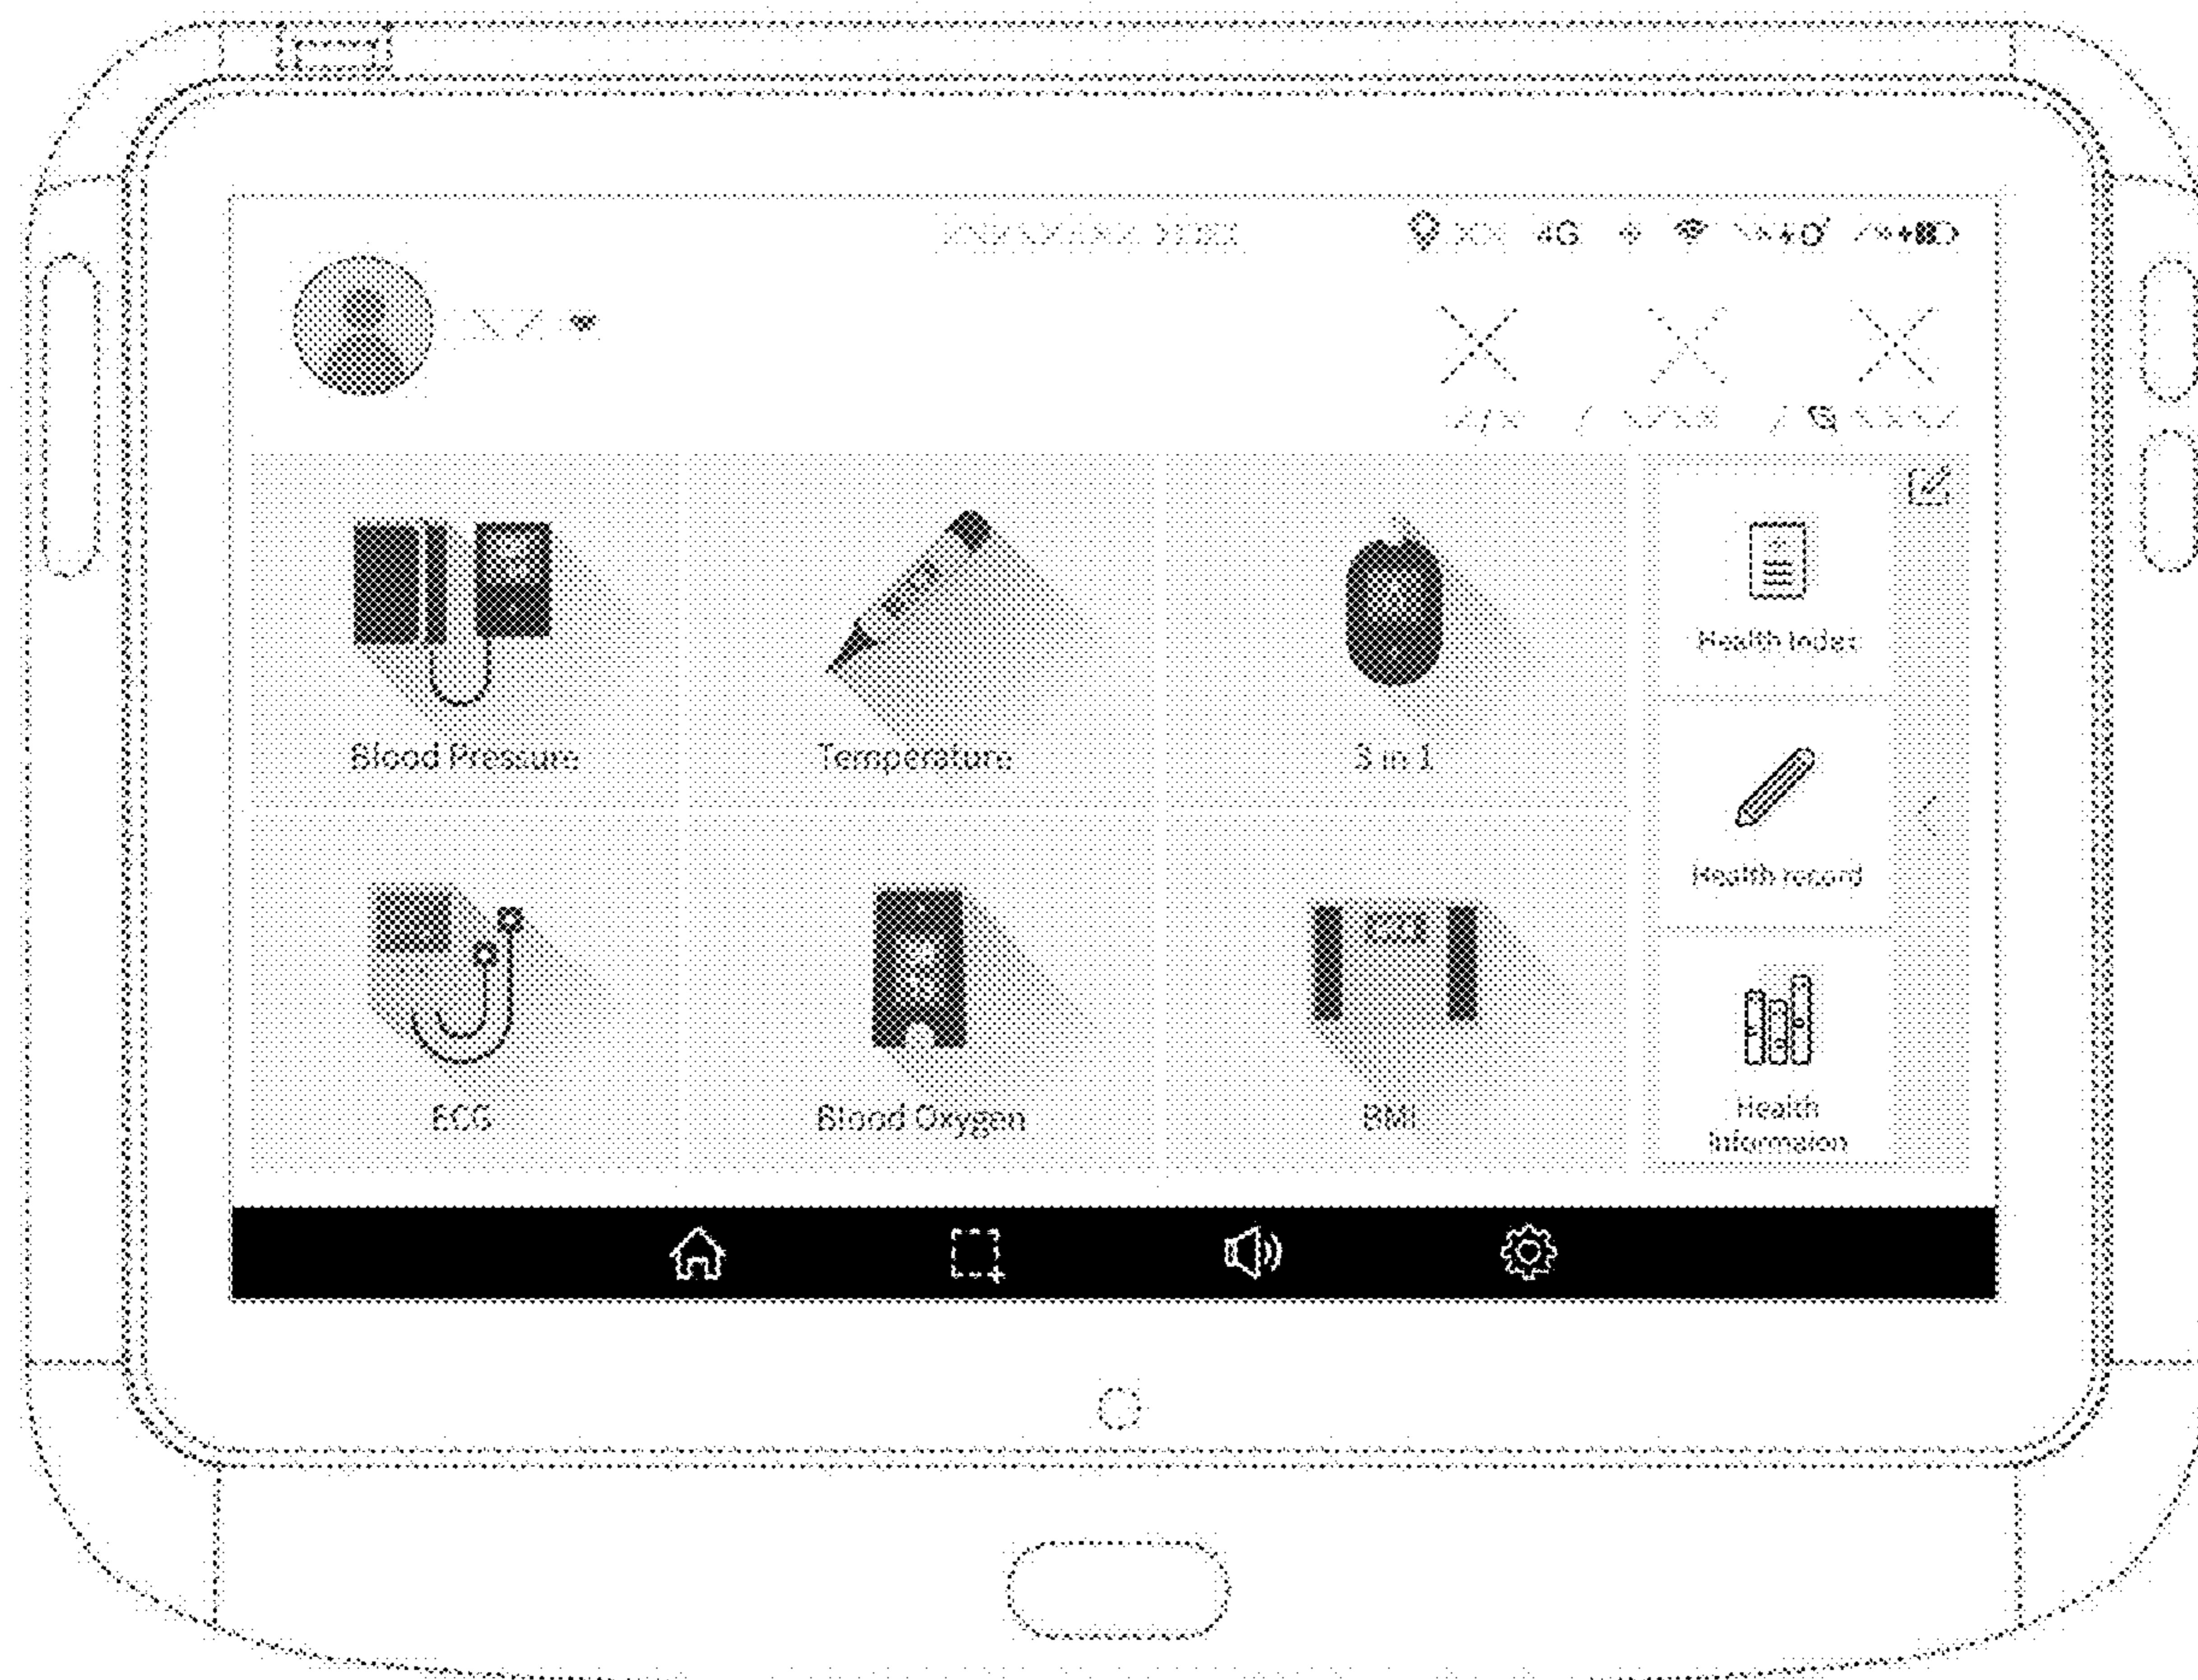


FIG. 1

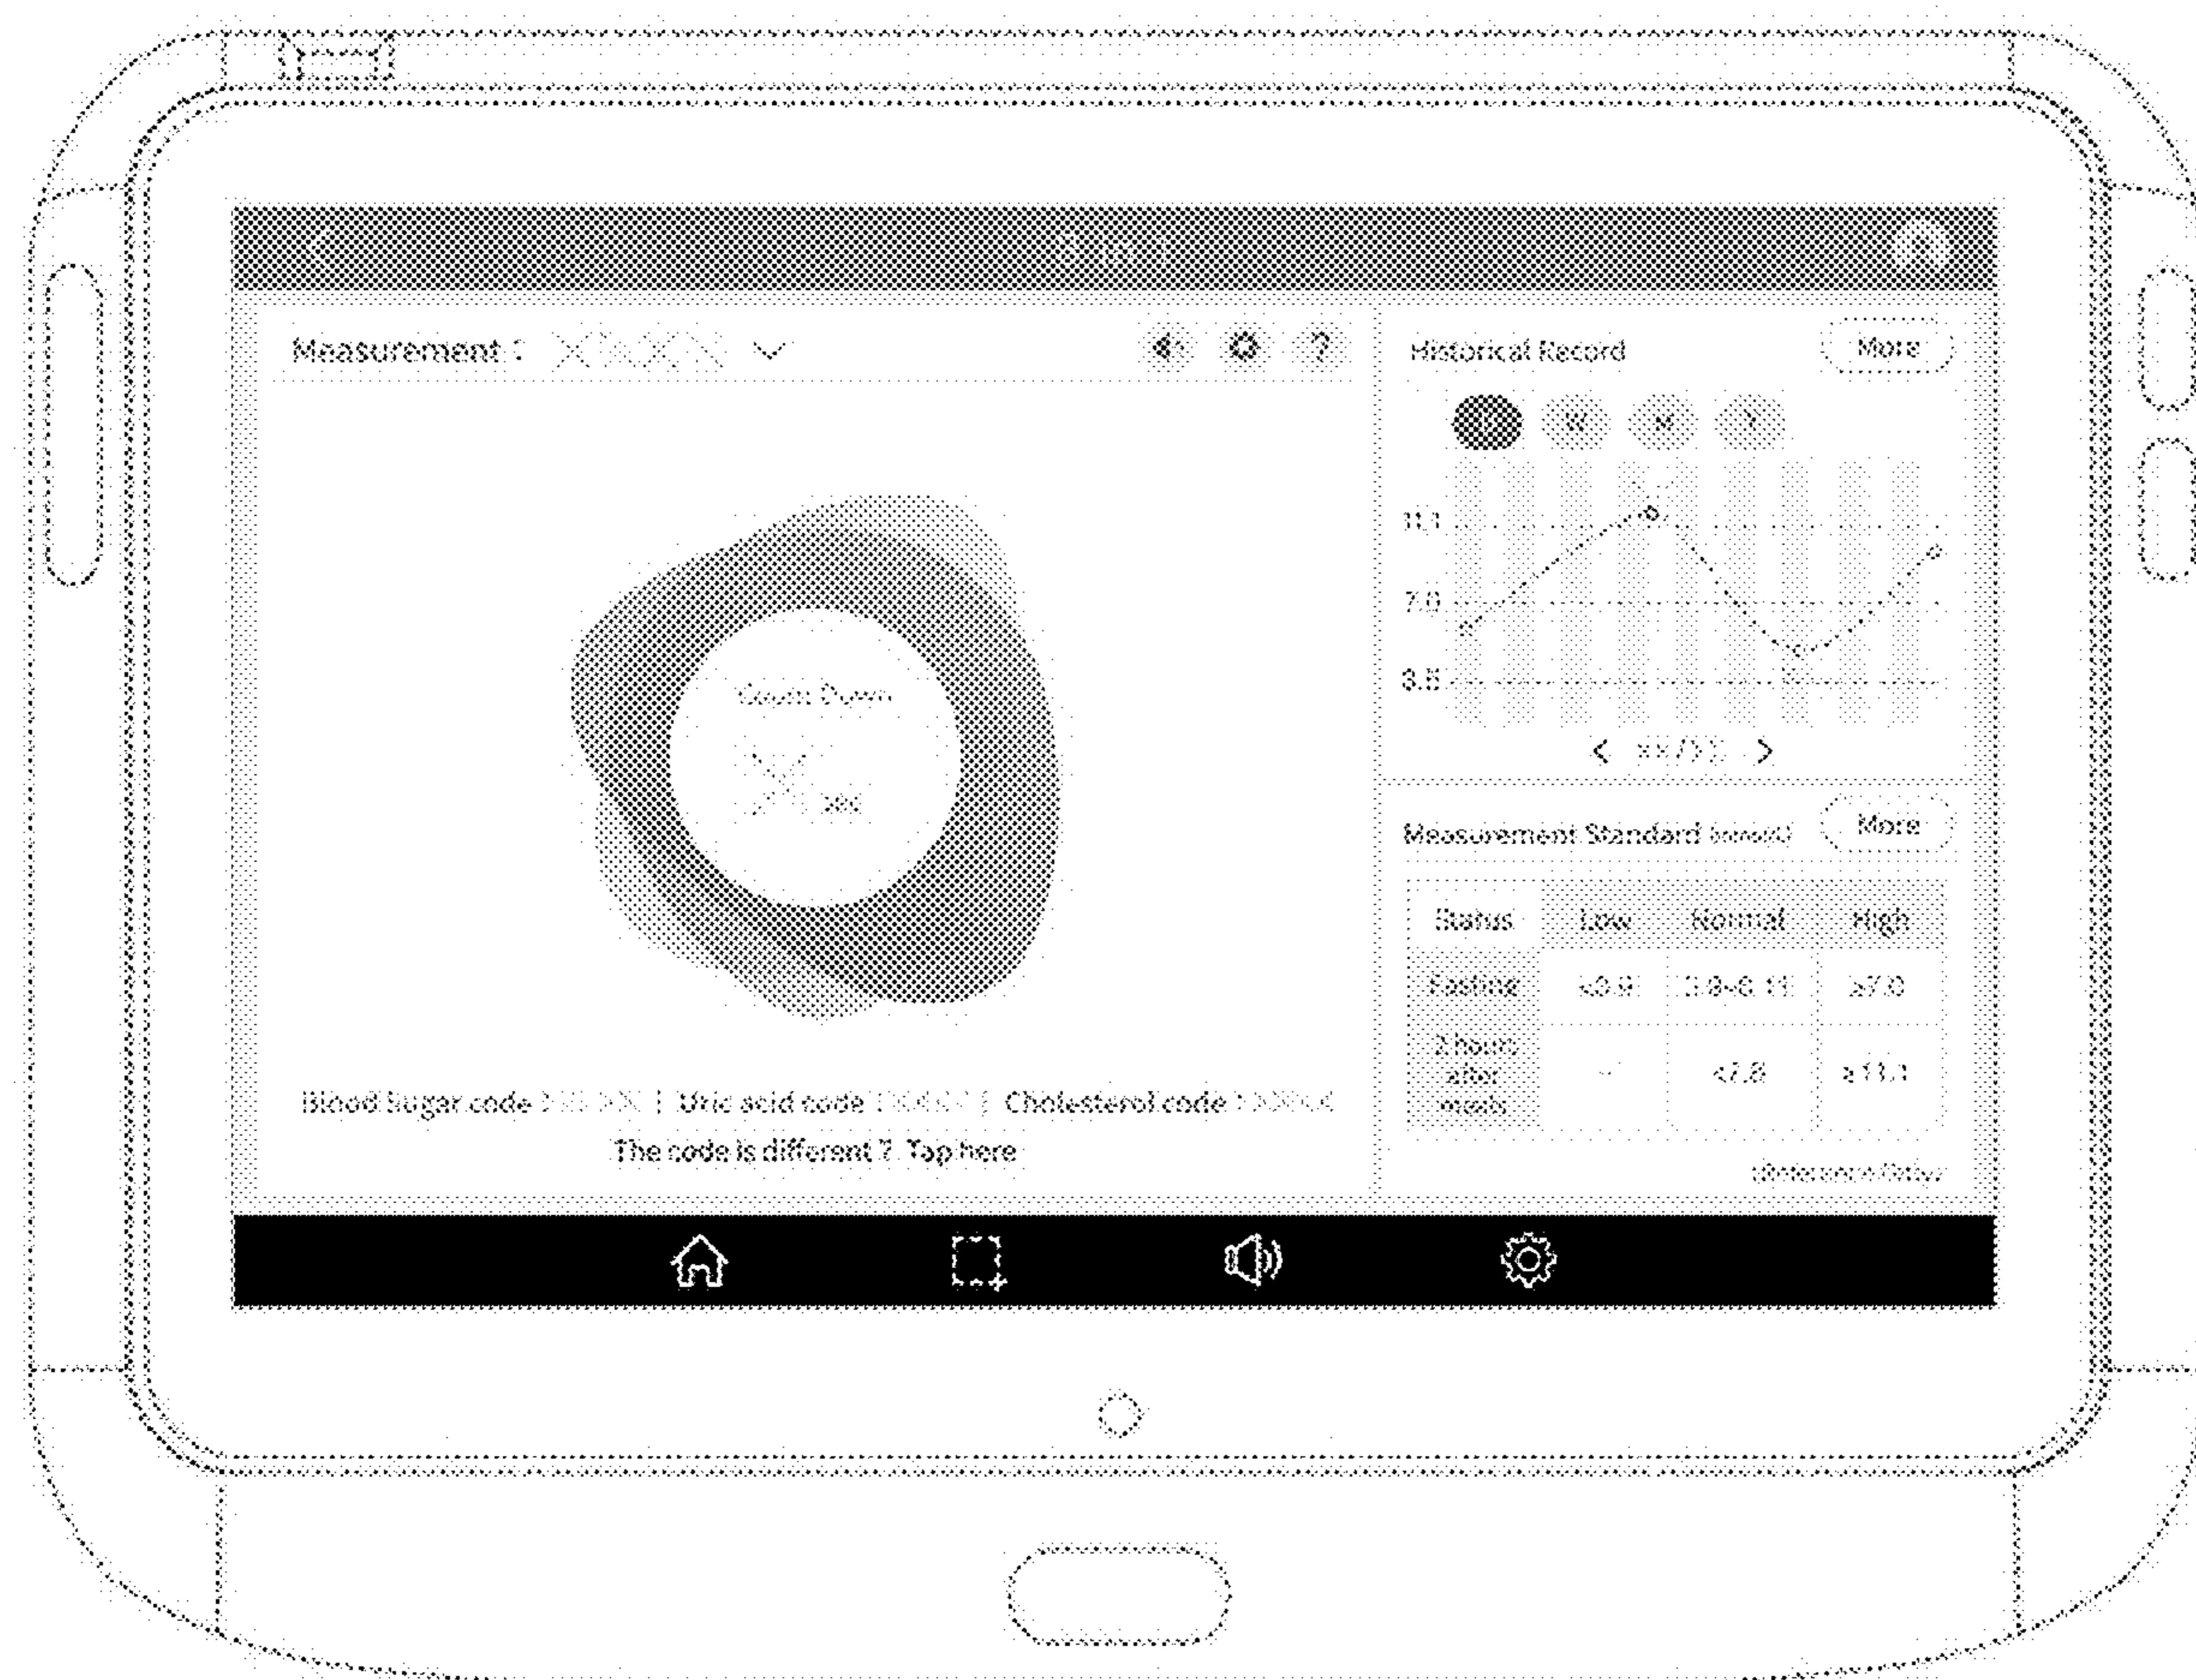


FIG. 2

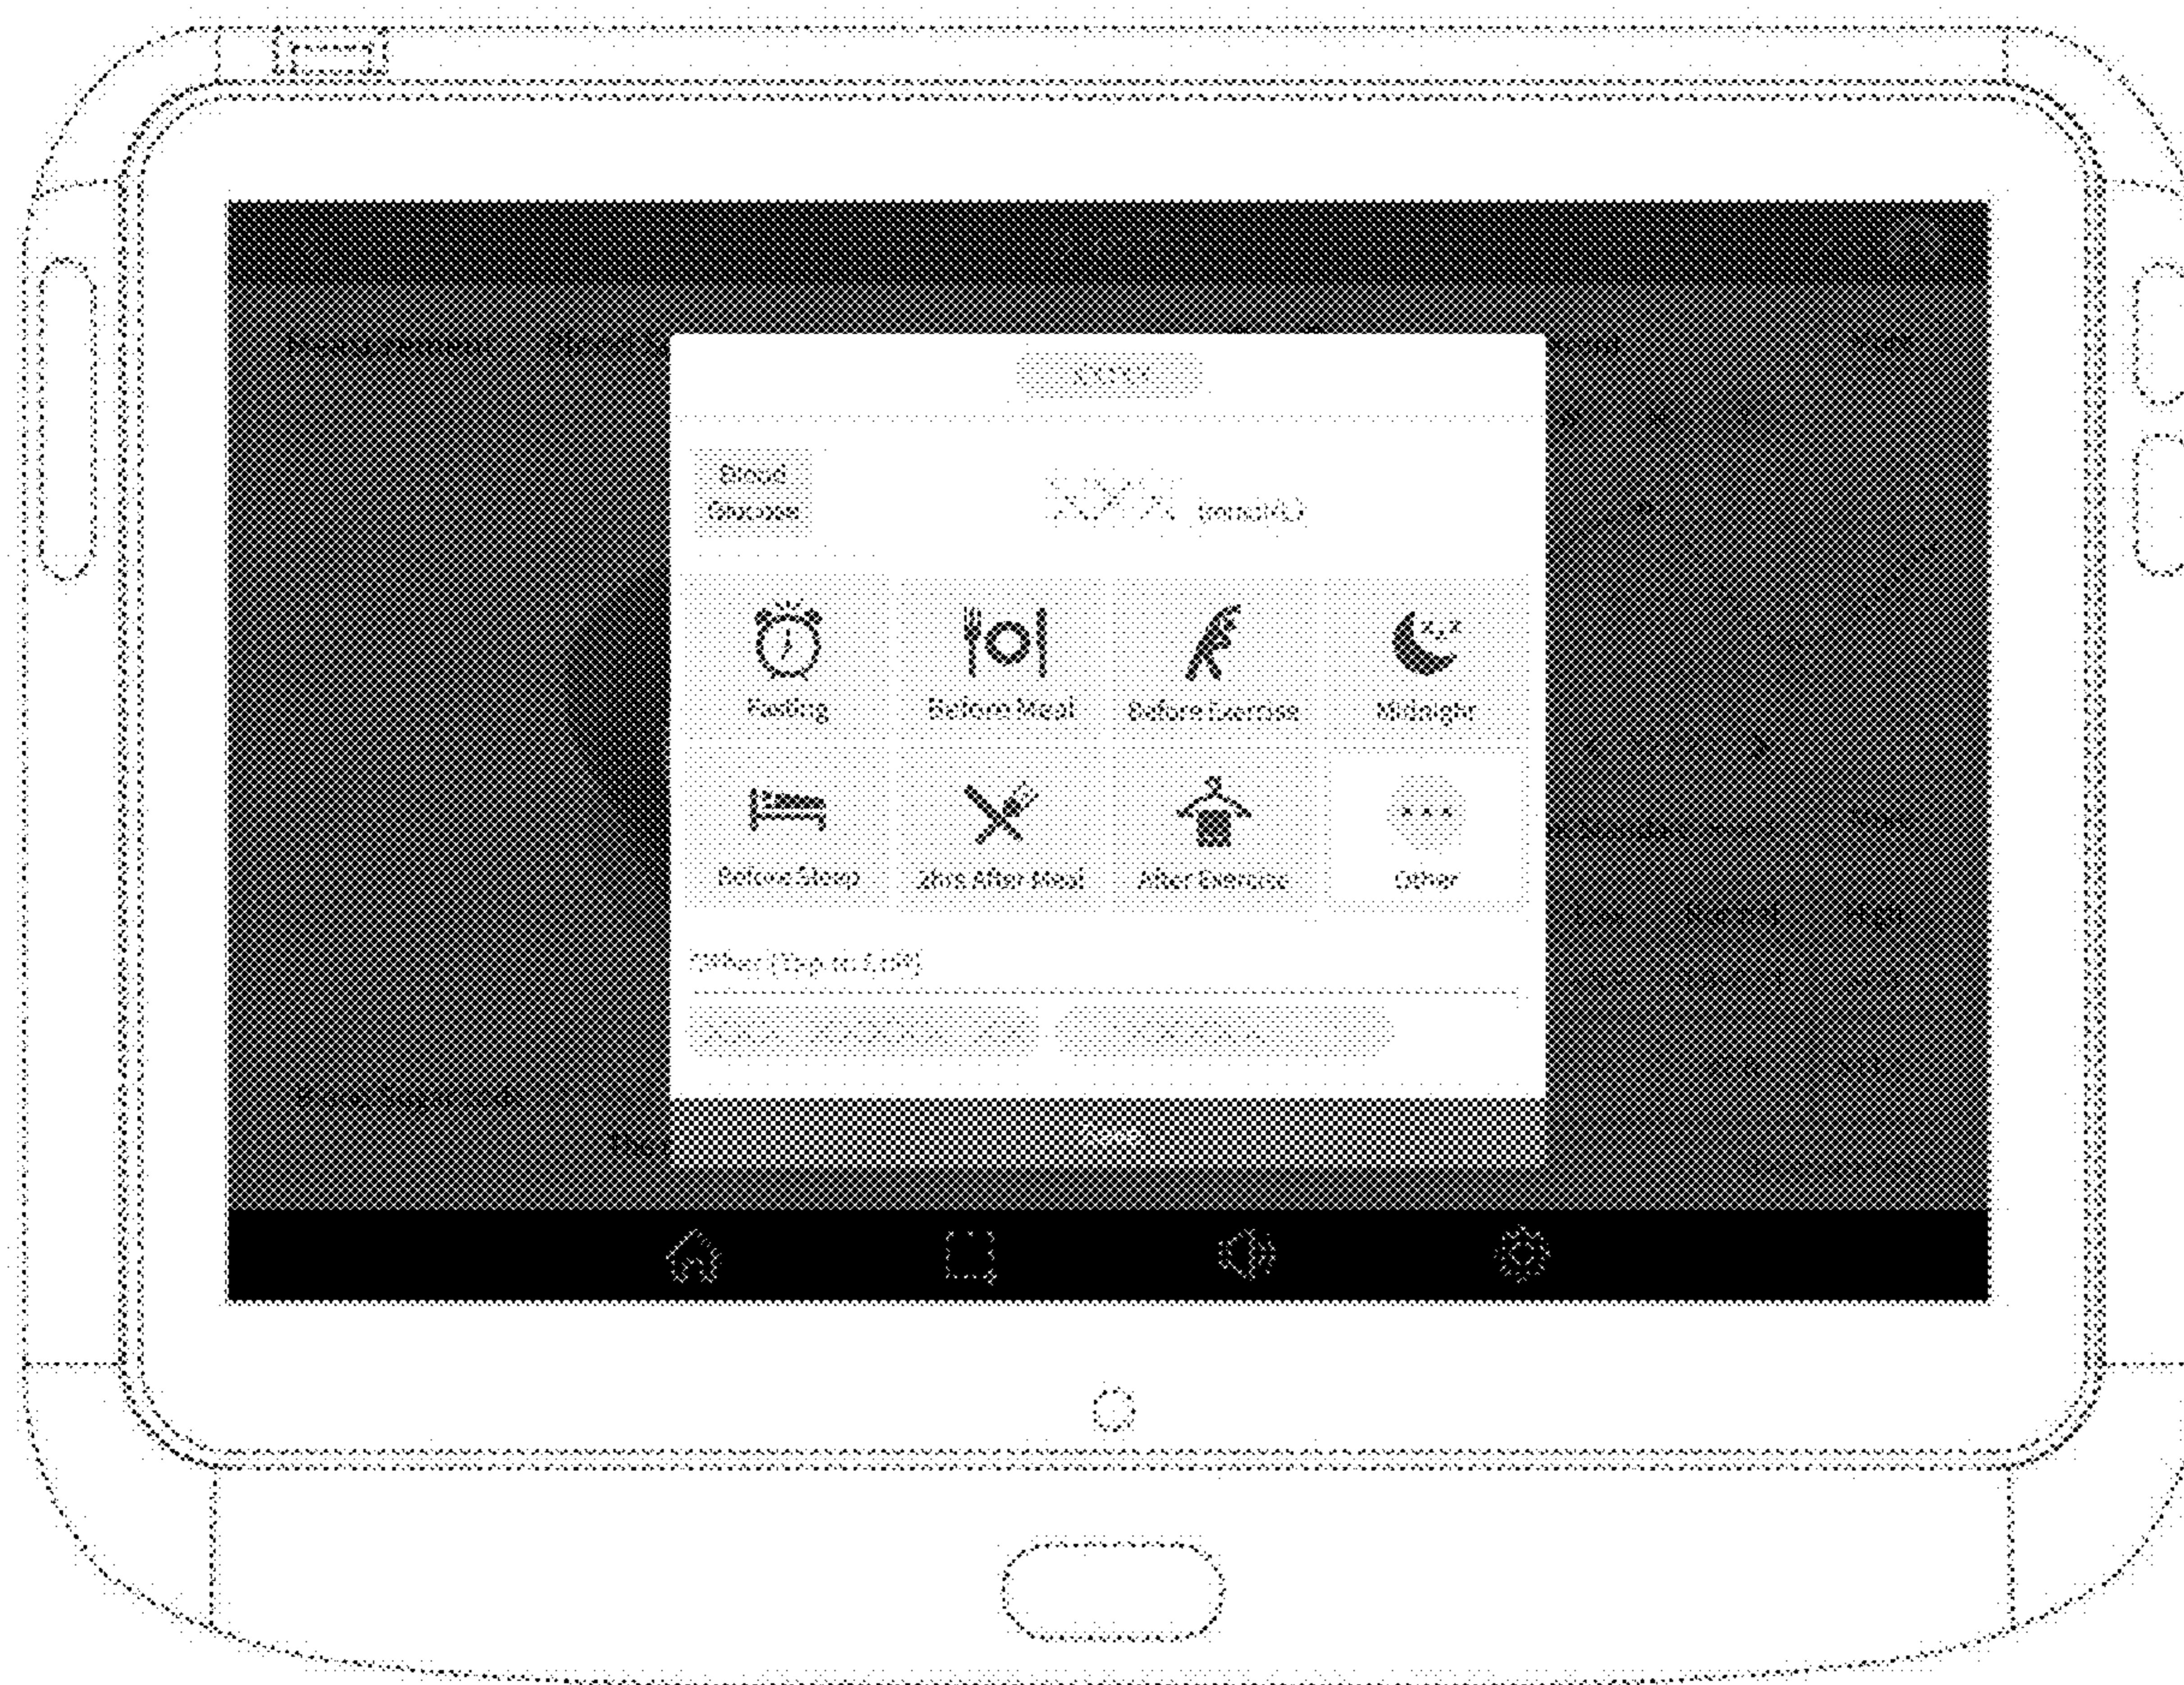


FIG. 3



FIG. 4



FIG. 5



FIG. 6