



US00D967458S

(12) **United States Design Patent**  
**Palthur et al.**

(10) **Patent No.:** **US D967,458 S**

(45) **Date of Patent:** **\*\* Oct. 18, 2022**

(54) **KIOSK**

(71) Applicant: **INNONEO HEALTH TECHNOLOGIES, INC.**, Boston, MA (US)

(72) Inventors: **Maruthi Prasad Palthur**, Westborough, MA (US); **Mary Elizabathe Joseph**, Hopkinton, MA (US)

(73) Assignee: **INNONEO HEALTH TECHNOLOGIES, INC.**, Boston, MA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/751,839**

(22) Filed: **Sep. 23, 2020**

(51) **LOC (13) Cl.** ..... **25-03**

(52) **U.S. Cl.**  
USPC ..... **D25/33**

(58) **Field of Classification Search**  
USPC ..... D25/1-35, 48.1

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

2,090,827 A \* 8/1937 Bak ..... E04H 1/1222  
126/190  
2,707,426 A \* 5/1955 Cooper ..... E04B 1/24  
52/270

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 201430016890 \* 8/2014  
CN 201730415458 \* 4/2018  
CN 201730438588 \* 4/2018

**OTHER PUBLICATIONS**

Isolation Rooms, available in tgh.org, announced Year 2020 [online], [site visited Feb. 25, 2022], Internet URL: <https://www.tgh.org/>

news/tgh-health-news/2020/may/how-isolation-rooms-help-keep-patients-safe (Year: 2020).\*

(Continued)

*Primary Examiner* — Brett Miller  
*Assistant Examiner* — Jasmine L. Comedy


(57) **CLAIM**

The ornamental design for a kiosk, as shown and described.

**DESCRIPTION**

FIG. 1 is a front-top perspective view of a kiosk showing my new design;  
FIG. 2 is a front-bottom perspective view thereof;  
FIG. 3 is a rear-top perspective view thereof;  
FIG. 4 is a rear-bottom perspective view thereof;  
FIG. 5 is a rear elevational view thereof;  
FIG. 6 is a front elevational view thereof;  
FIG. 7 is a left elevational view thereof;  
FIG. 8 is a right elevational view thereof;  
FIG. 9 is a top plan view thereof;  
FIG. 10 is a bottom plan view thereof;  
FIG. 11 is a left cross-sectional view taken along cutting line 11-11 in FIG. 9;  
FIG. 12 is a front-top perspective cross-sectional view taken along cutting line 11-11 in FIG. 9;  
FIG. 13 is a rear-top perspective cross-sectional view taken along cutting line 11-11 in FIG. 9;  
FIG. 14 is a left cross-sectional view taken along cutting line 14-14 in FIG. 9;  
FIG. 15 is a front-top perspective cross-sectional view taken along cutting line 14-14 in FIG. 9;  
FIG. 16 is a rear-top perspective cross-sectional view taken along cutting line 14-14 in FIG. 9; and,  
FIG. 17 is a supplemental front-top perspective view of the kiosk with a logo.  
The broken lines shown are for illustrative purposes only and form no part of the claimed design.

**1 Claim, 17 Drawing Sheets**

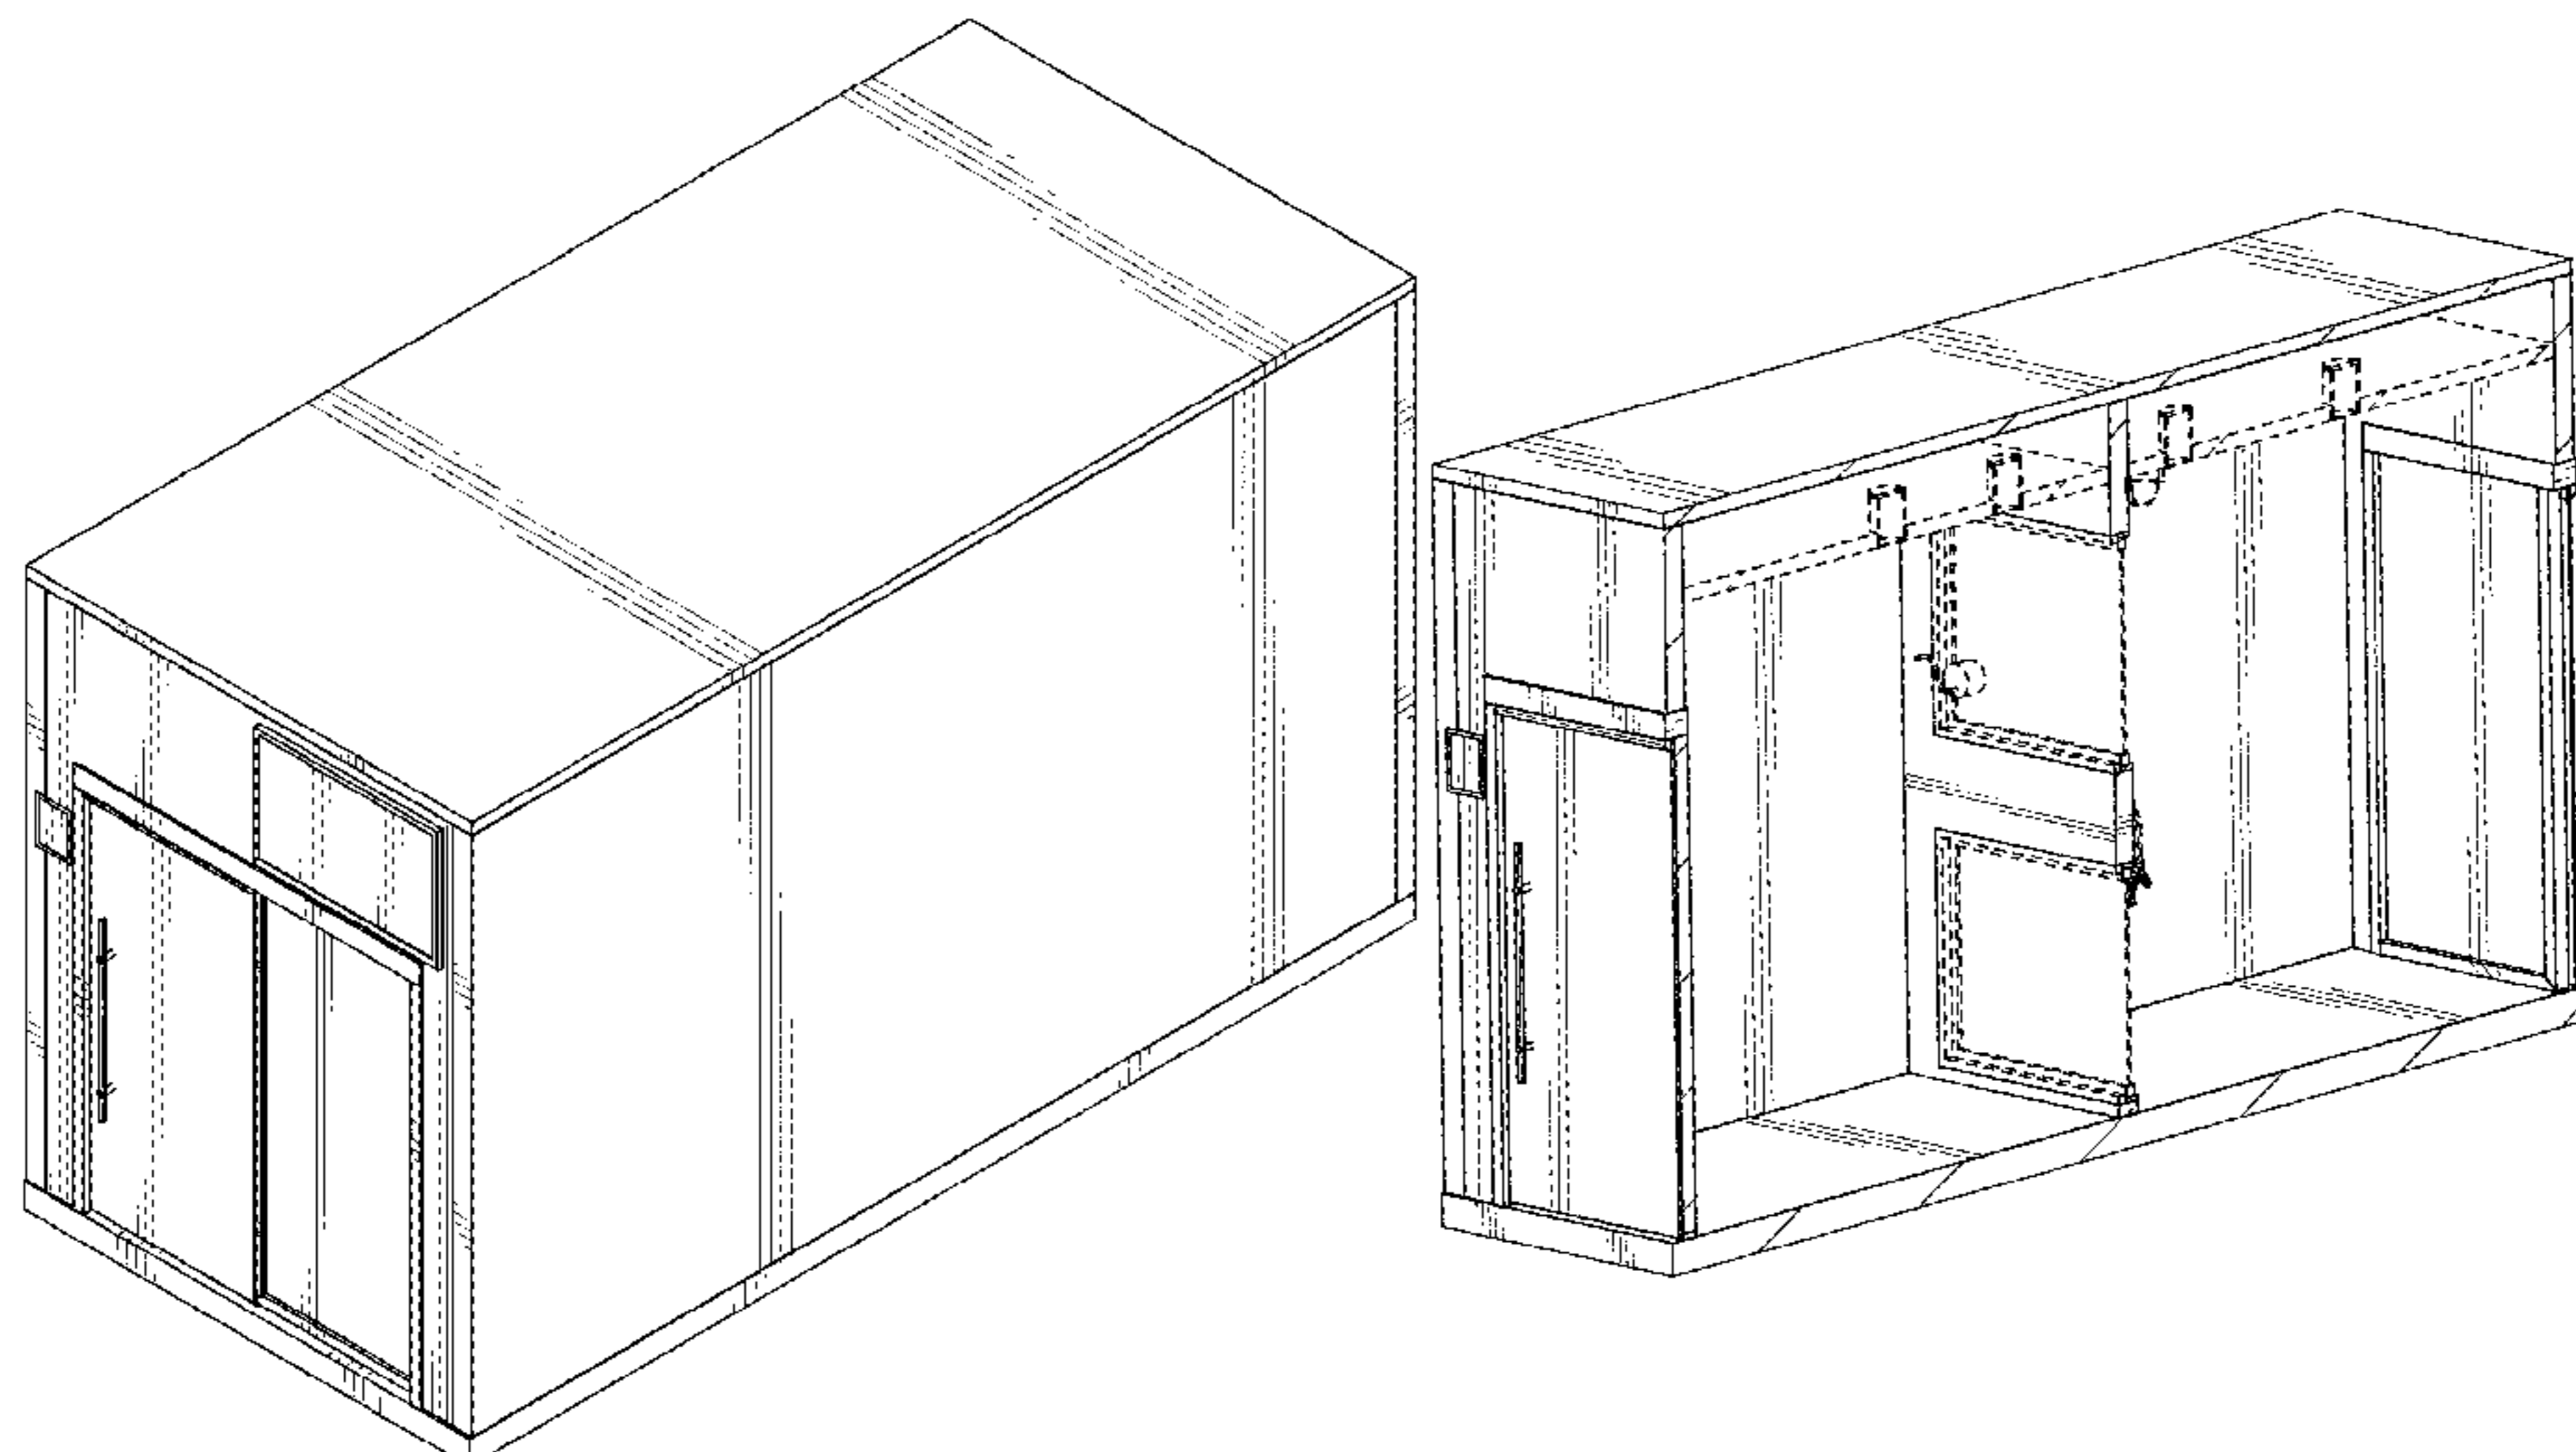

(58) **Field of Classification Search**

CPC ... E04H 1/1222; E04H 1/1272; E04H 12/182;  
 E04H 1/1205; E04H 1/125; E04H 3/08;  
 E04B 1/24

See application file for complete search history.

D828,927	S *	9/2018	Solie	.....	D25/33
D829,343	S *	9/2018	Solie	.....	D25/33
D846,147	S *	4/2019	Zhu	.....	D25/16
10,376,604	B2	8/2019	Romo et al.		
D885,812	S *	6/2020	Kahn	.....	D6/700
2014/0251401	A1 *	9/2014	Barber	.....	E04H 1/1205 135/121
2015/0199783	A1	7/2015	Cashman et al.		

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,110,907	A *	11/1963	King	.....	E04B 1/34869 4/300
3,383,812	A *	5/1968	Starr	.....	E04H 1/1205 52/36.2
3,611,907	A *	10/1971	Wasserman	.....	E04B 1/8218 D25/16
D344,140	S *	2/1994	Webster	.....	D25/33
5,285,604	A *	2/1994	Carlin	.....	E04H 1/1205 52/36.2
D655,019	S *	2/2012	Colless	.....	D25/15
D694,909	S	12/2013	Cashman et al.		
9,103,134	B1 *	8/2015	Murray	.....	E04H 1/125
D745,188	S *	12/2015	Hart	.....	D25/16
D771,835	S *	11/2016	Bottin	.....	D25/33
D791,967	S *	7/2017	Goldberg	.....	D25/16
D812,247	S *	3/2018	Price	.....	D25/16

OTHER PUBLICATIONS

Critical Isolation Rooms, available in [starcsystems.com](http://starcsystems.com), announced Year 2020 [online], [site visited Feb. 25, 2022], Internet URL: <https://blog.starcsystems.com/blog/starc-systems-refocuses-production-to-provide-critical-isolation-rooms-for-healthcare-facilities> (Year: 2020).\*

Shim Hyun-Tai, Korea's evolving virus tests—from drive-through to walk-through, <<http://www.koreabiomed.com/news/articleView.html?idxno=7767>>.

The 'phone booths' that are making Covid tests in India easier, quicker and safer, <<https://economictimes.indiatimes.com/industry/healthcare/biotech/healthcare/the-phone-booths-that-are-making-covid-tests-in-india-easier-quicker-and-safer/articleshow/75040280.cms?from=mdr>>.

\* cited by examiner

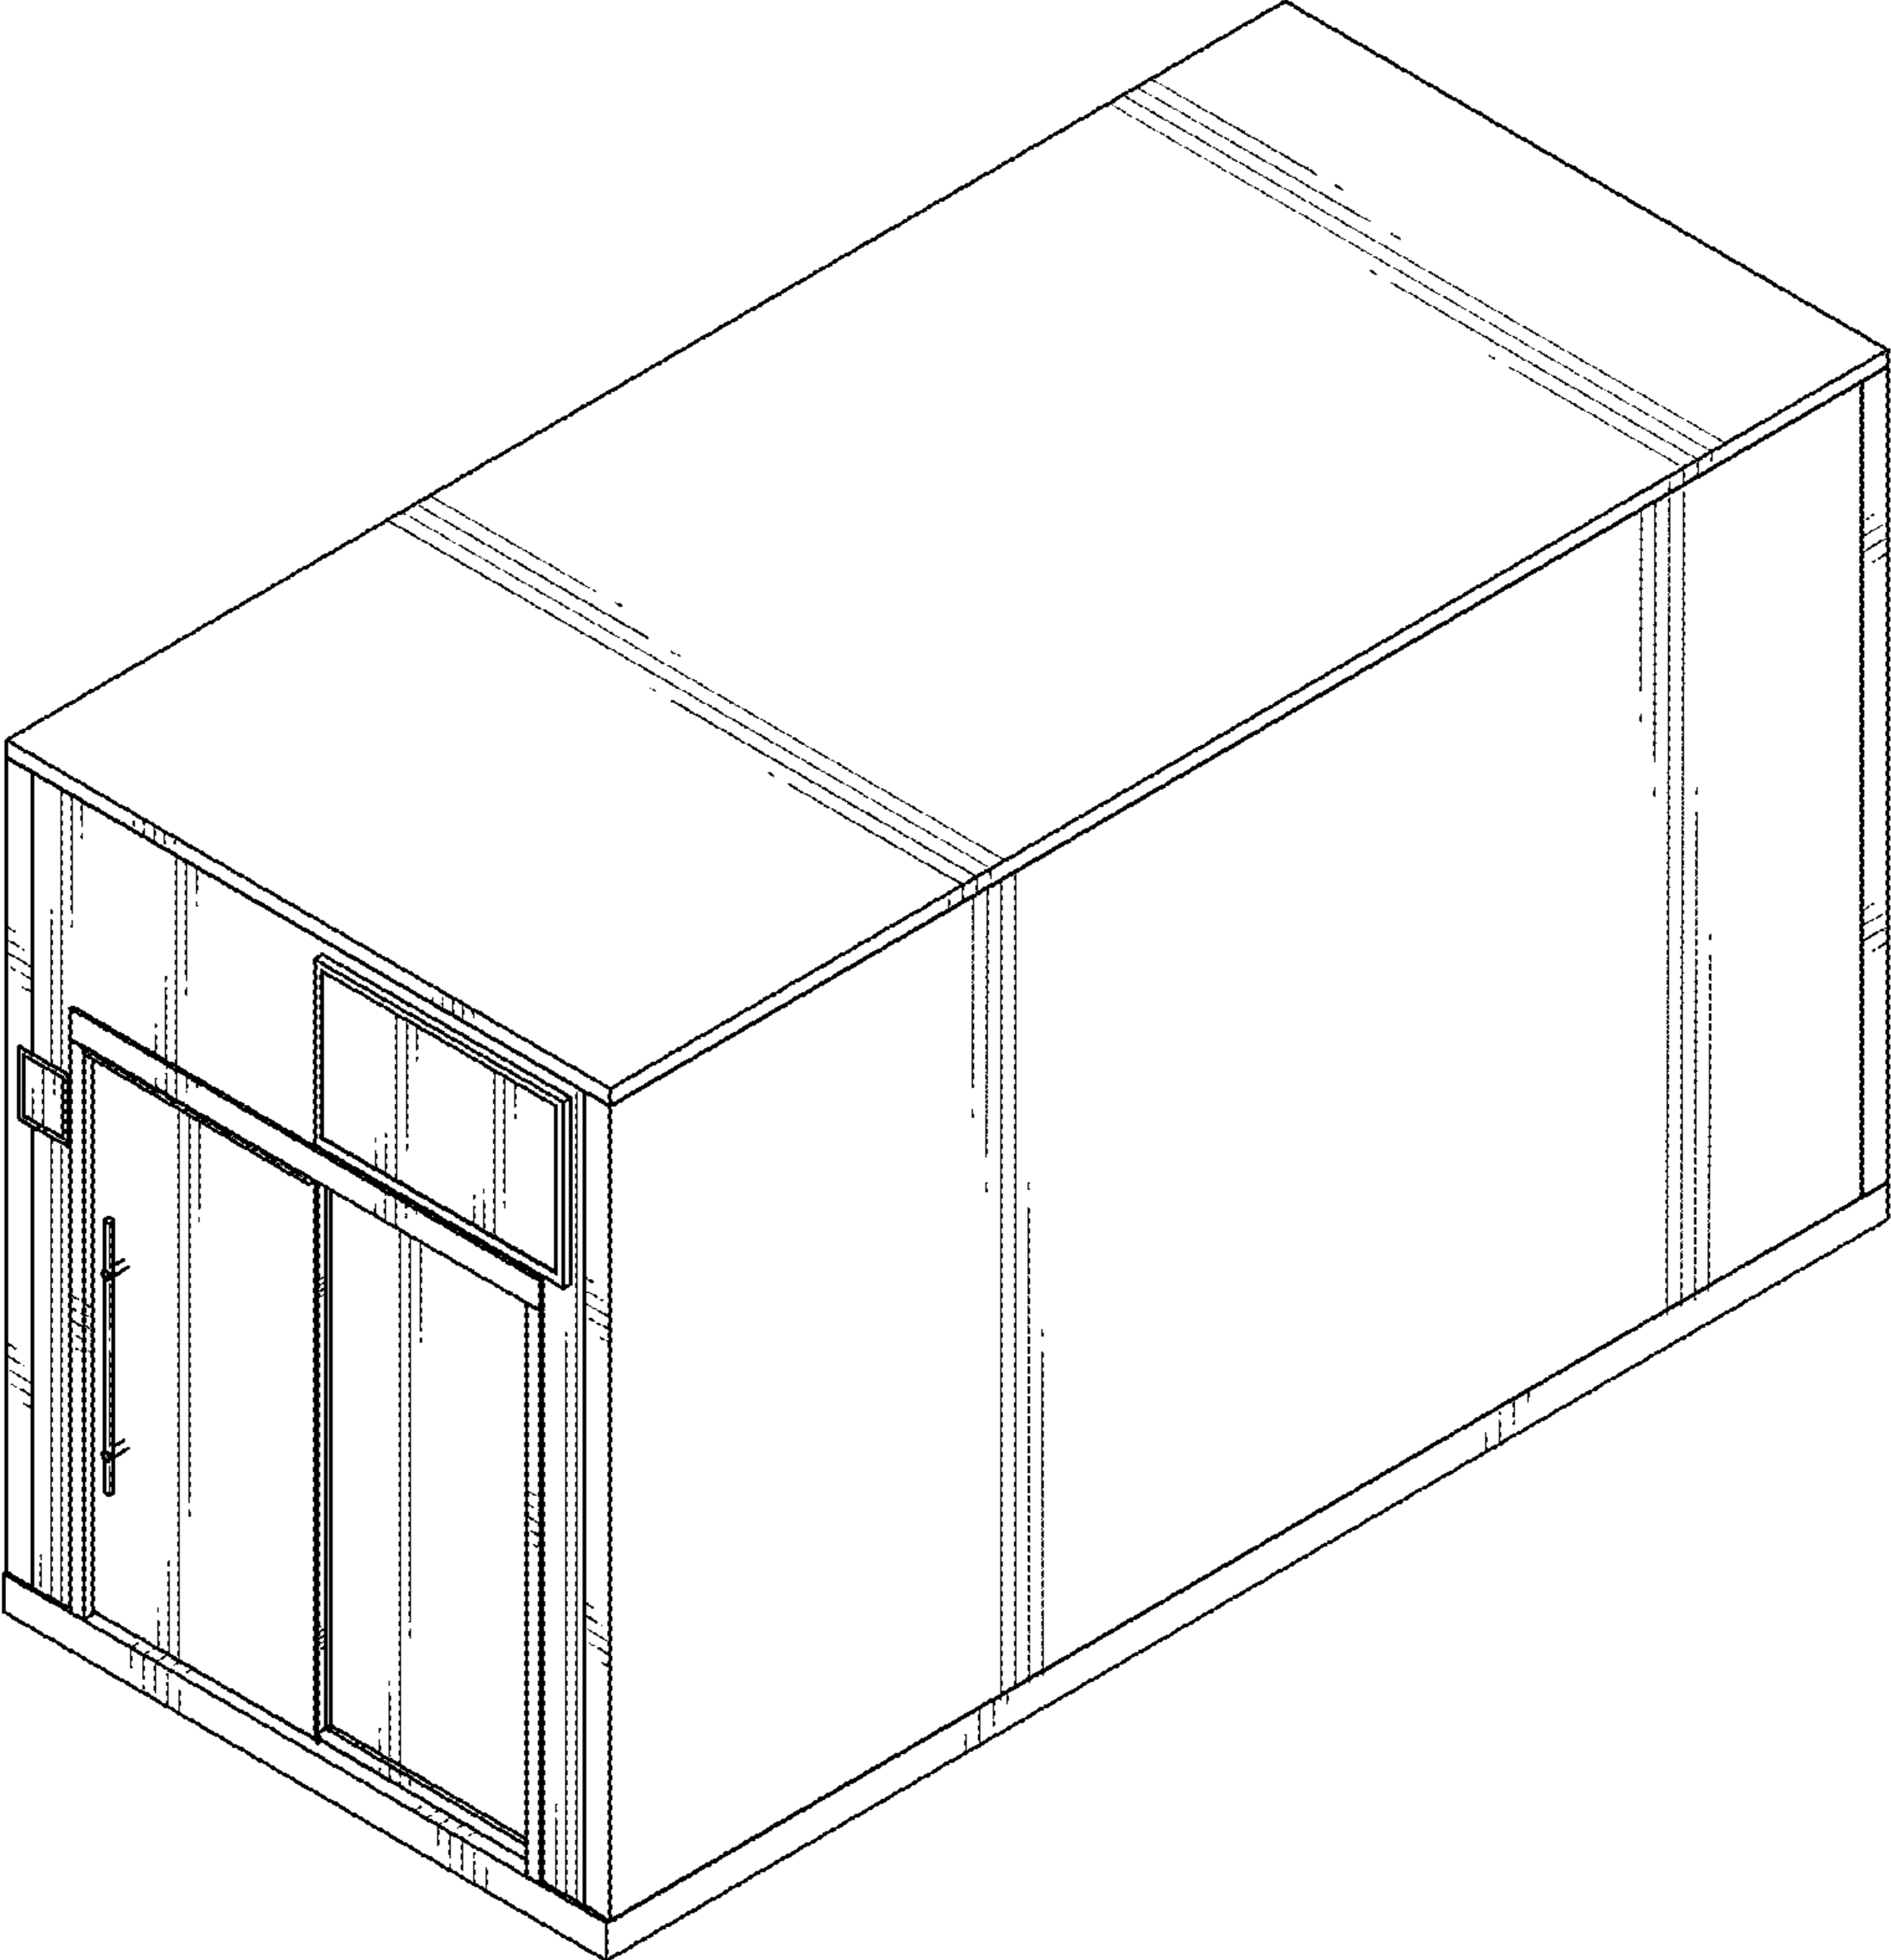


FIG. 1

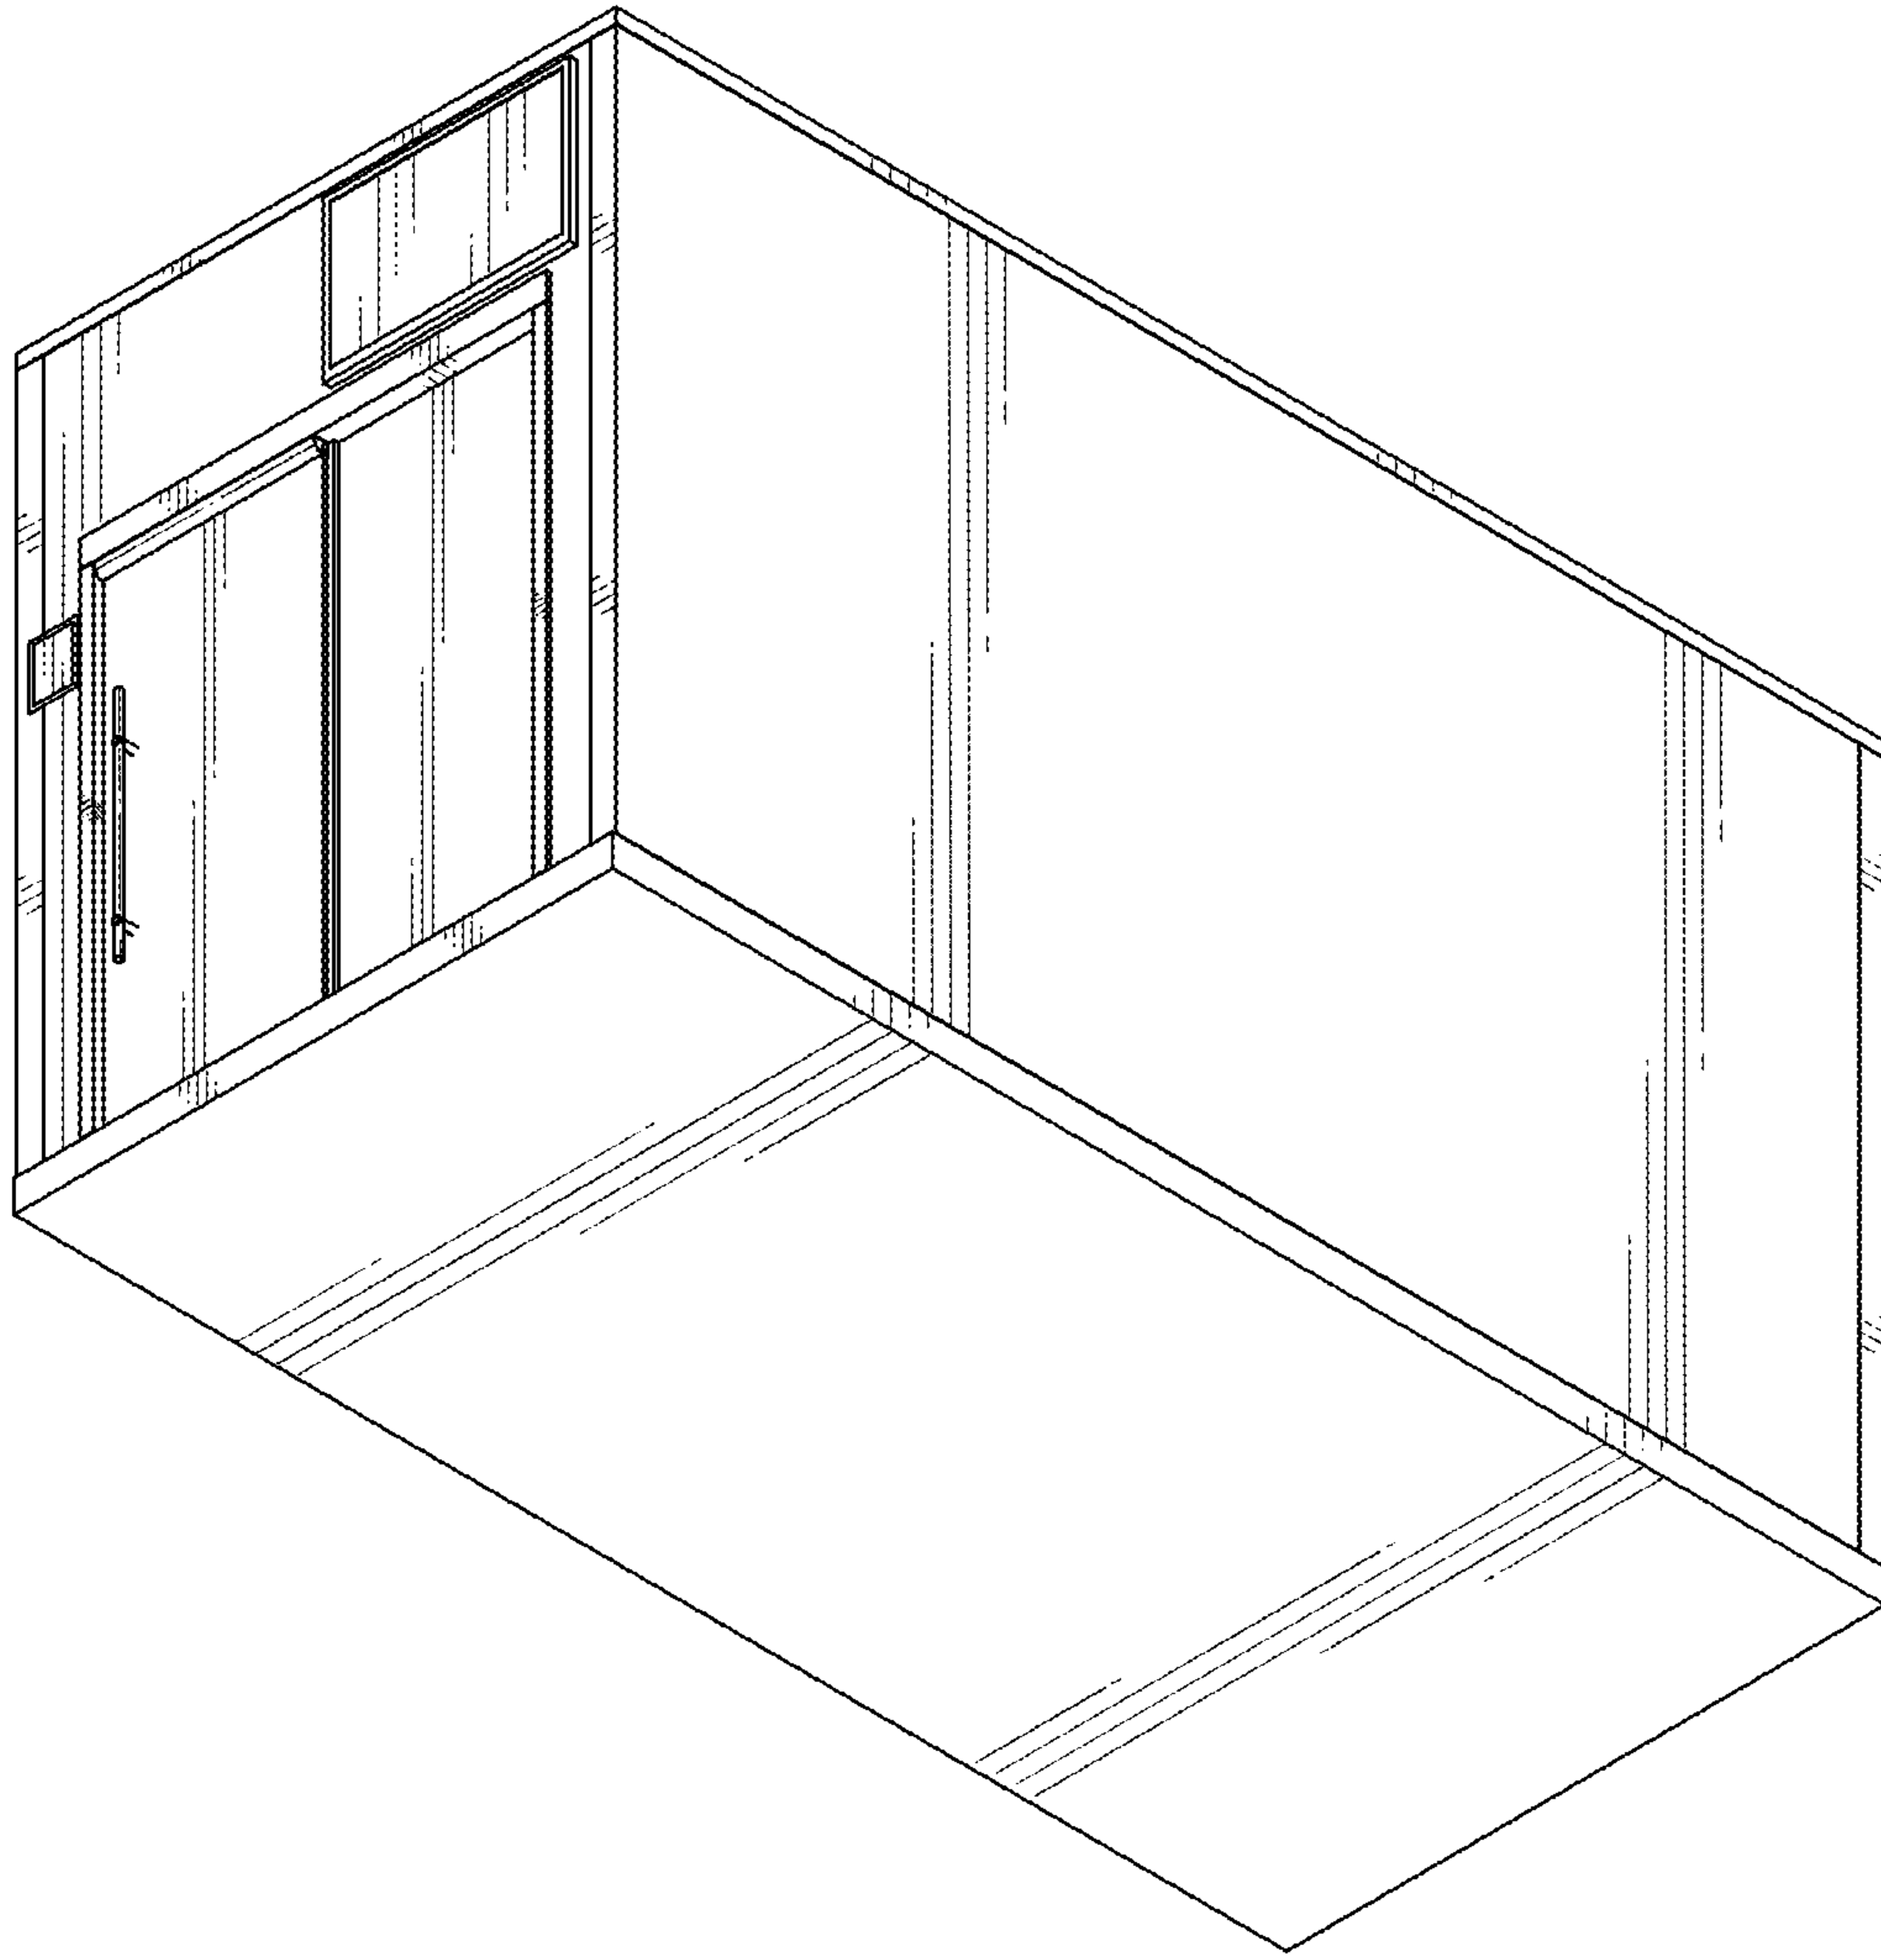


FIG. 2

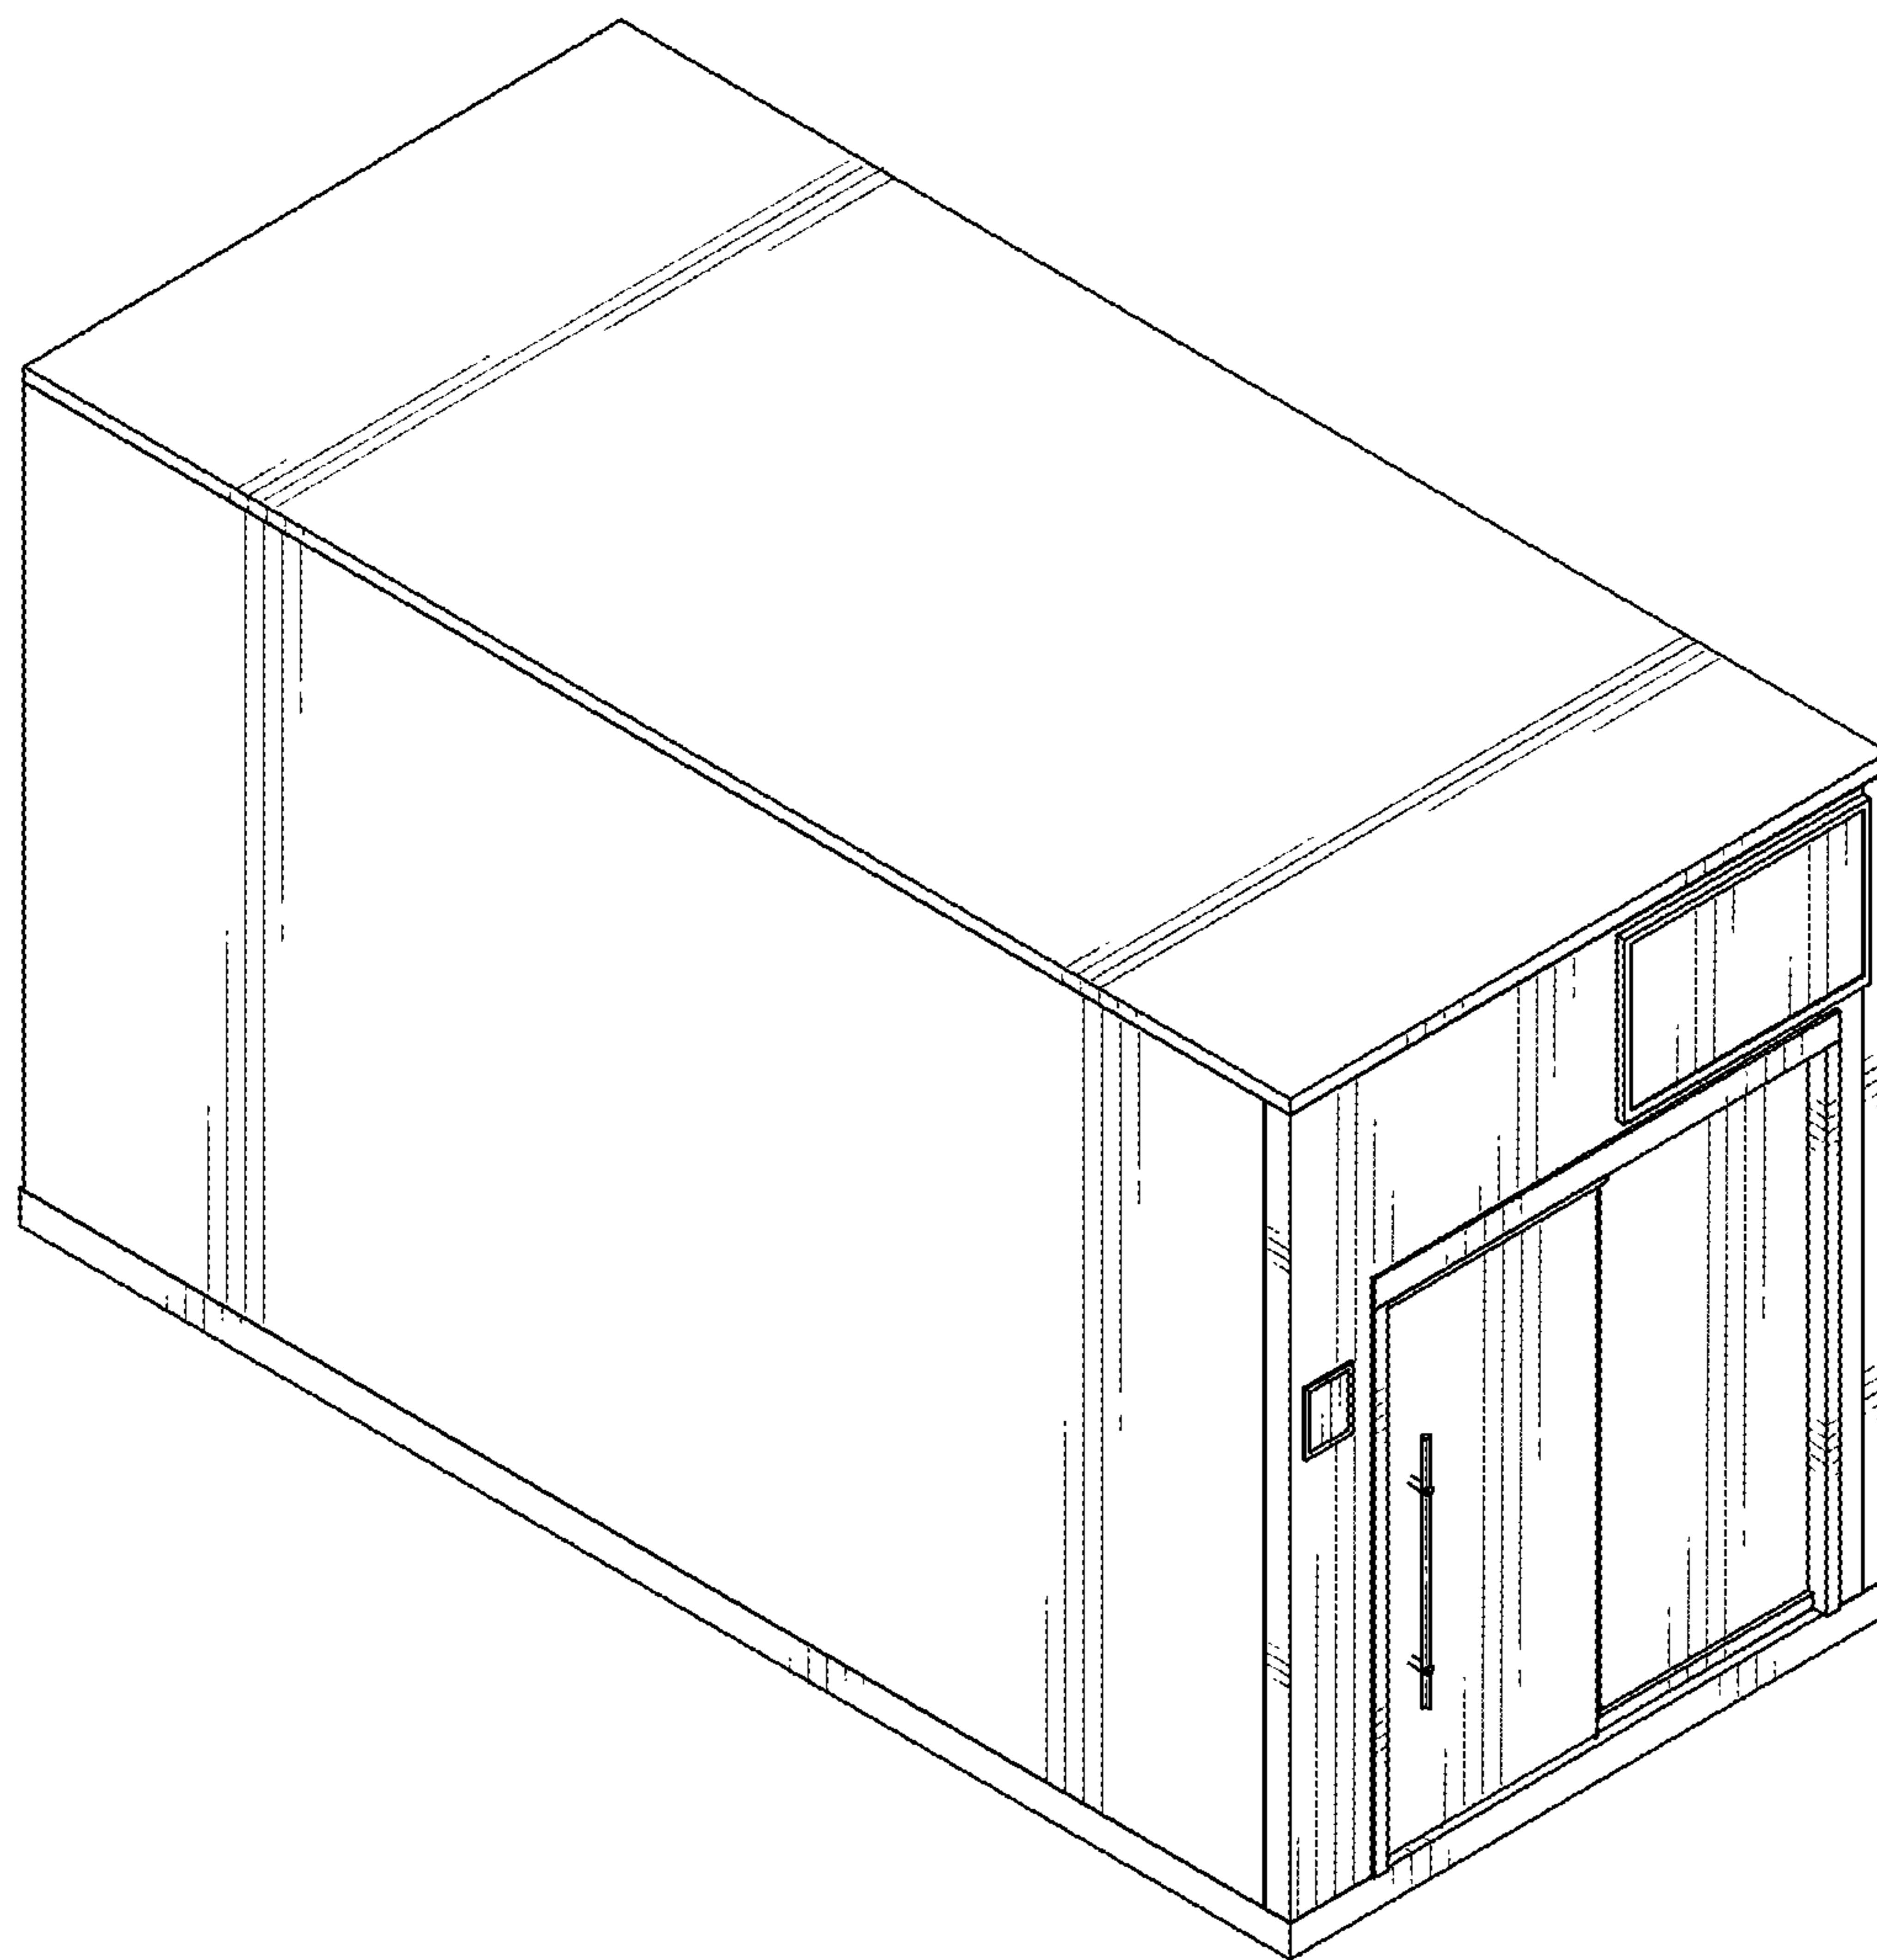


FIG. 3

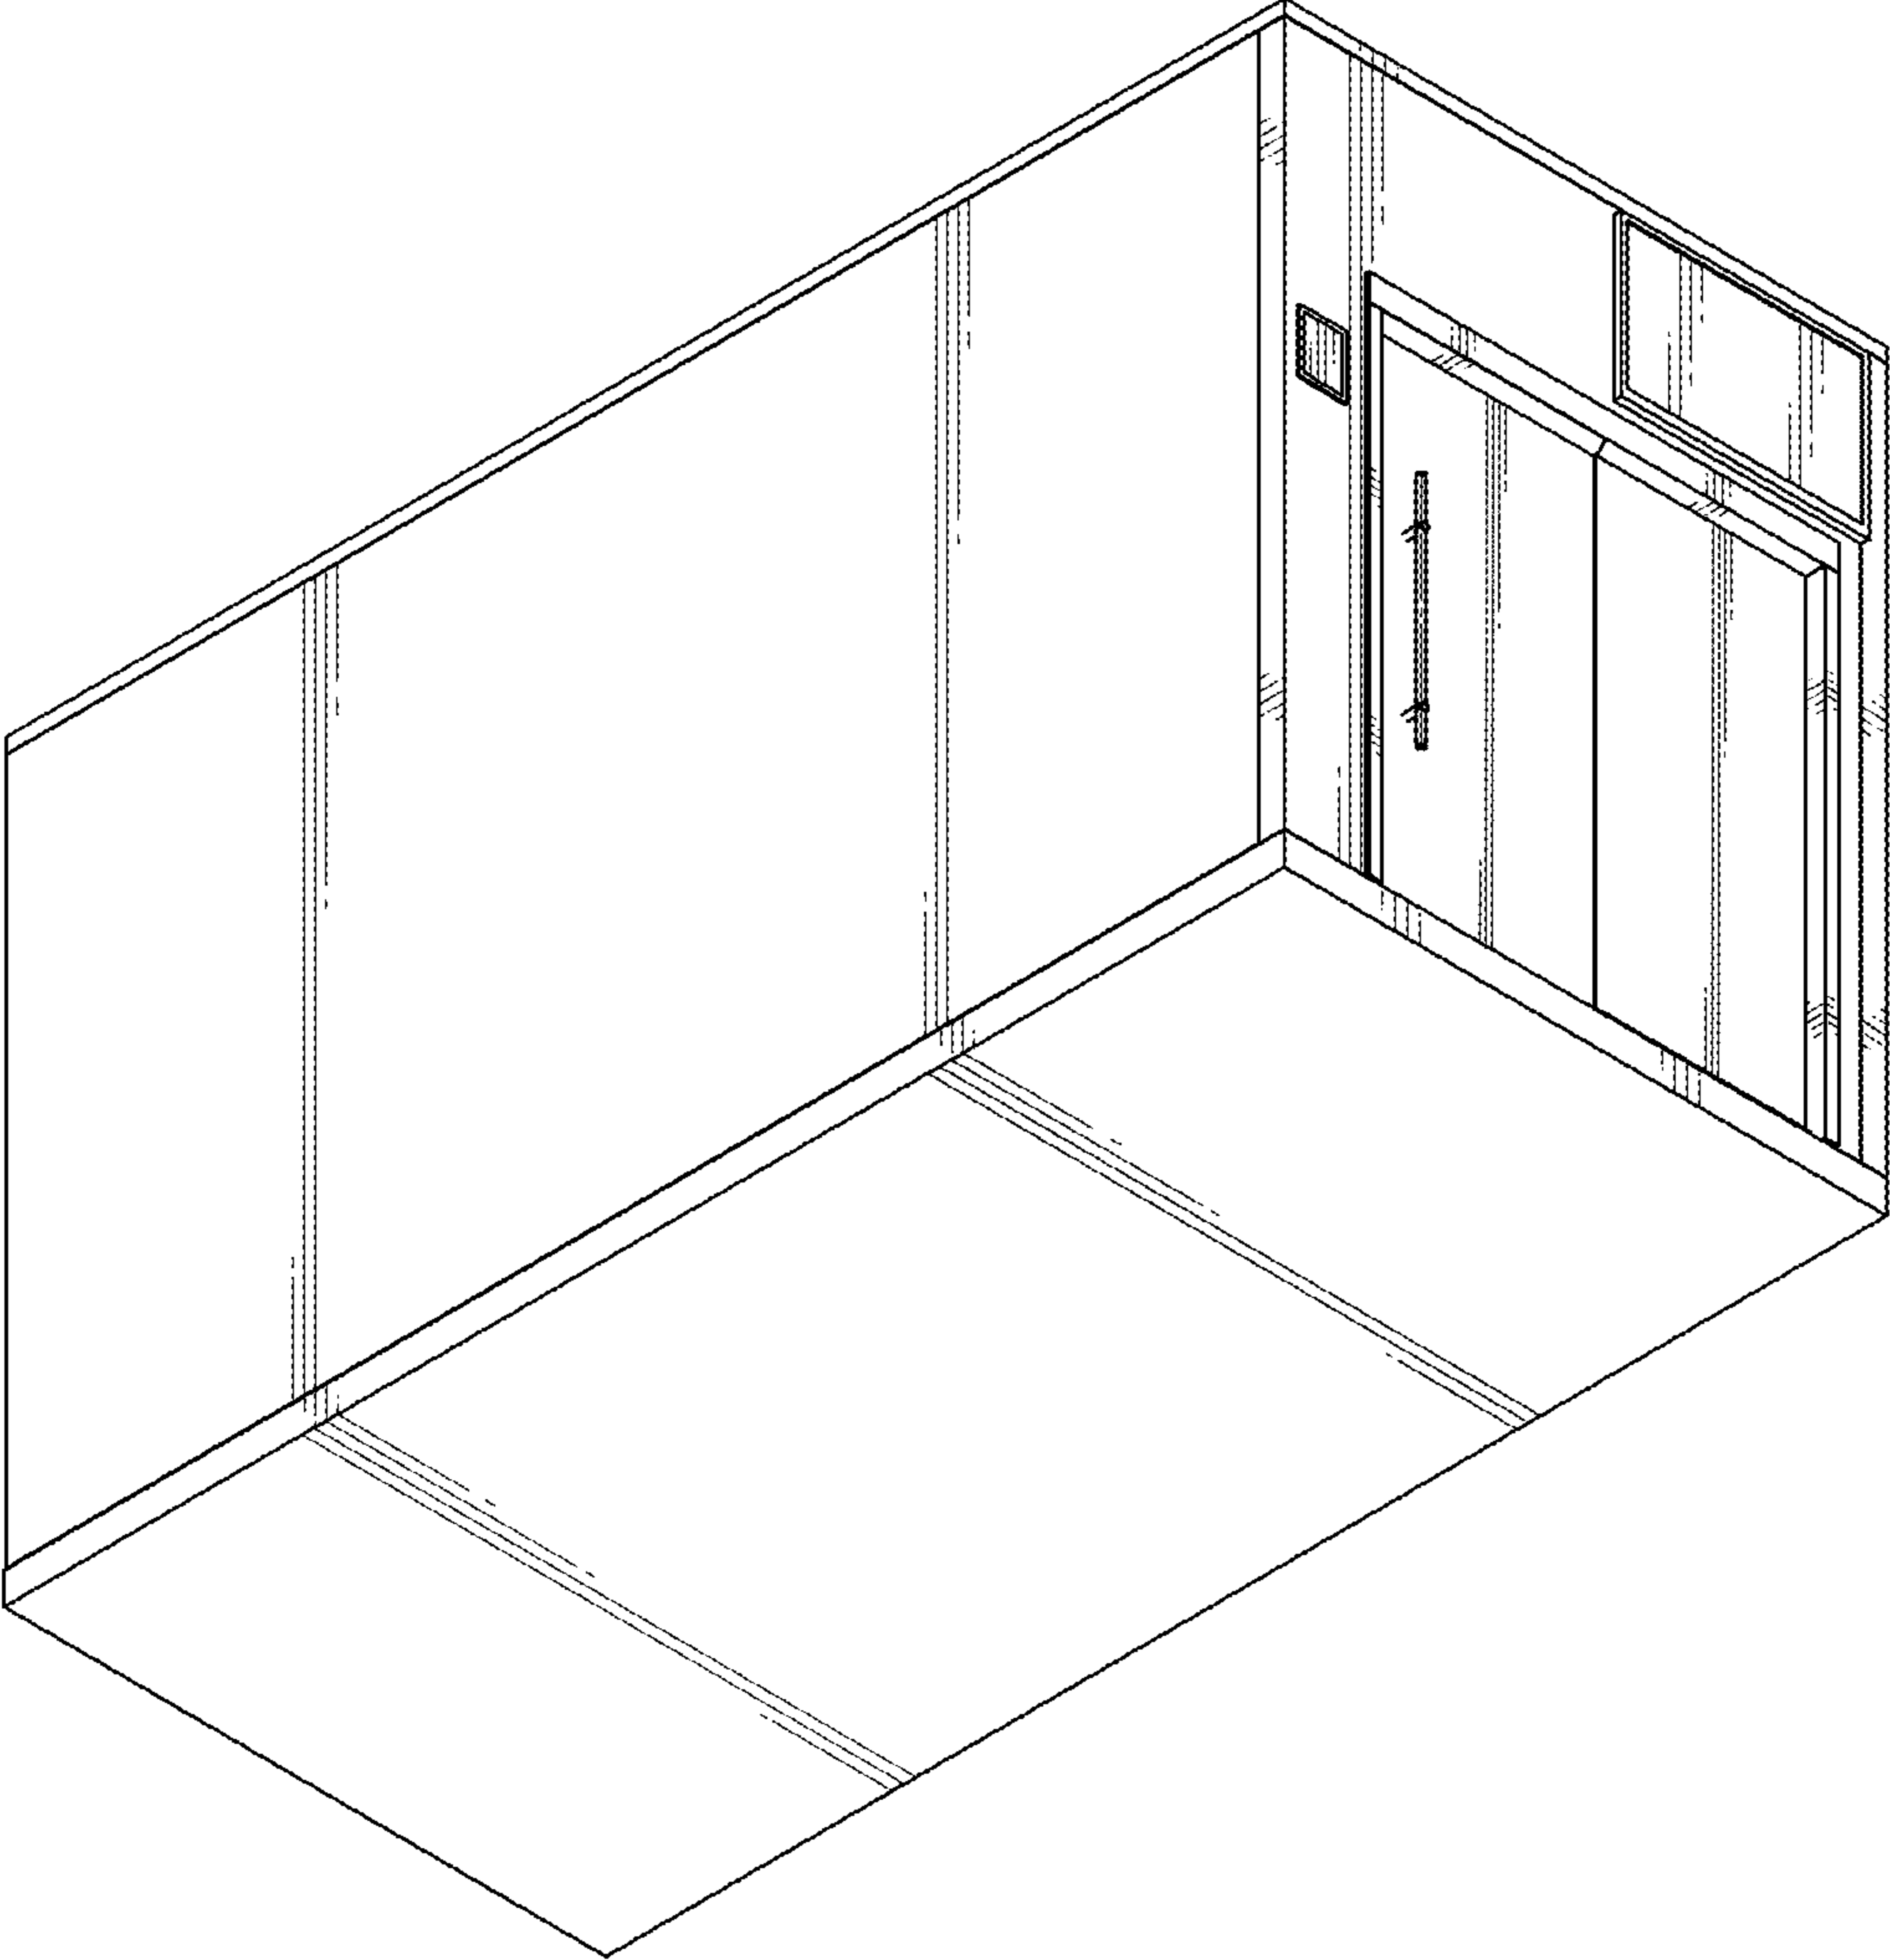


FIG. 4

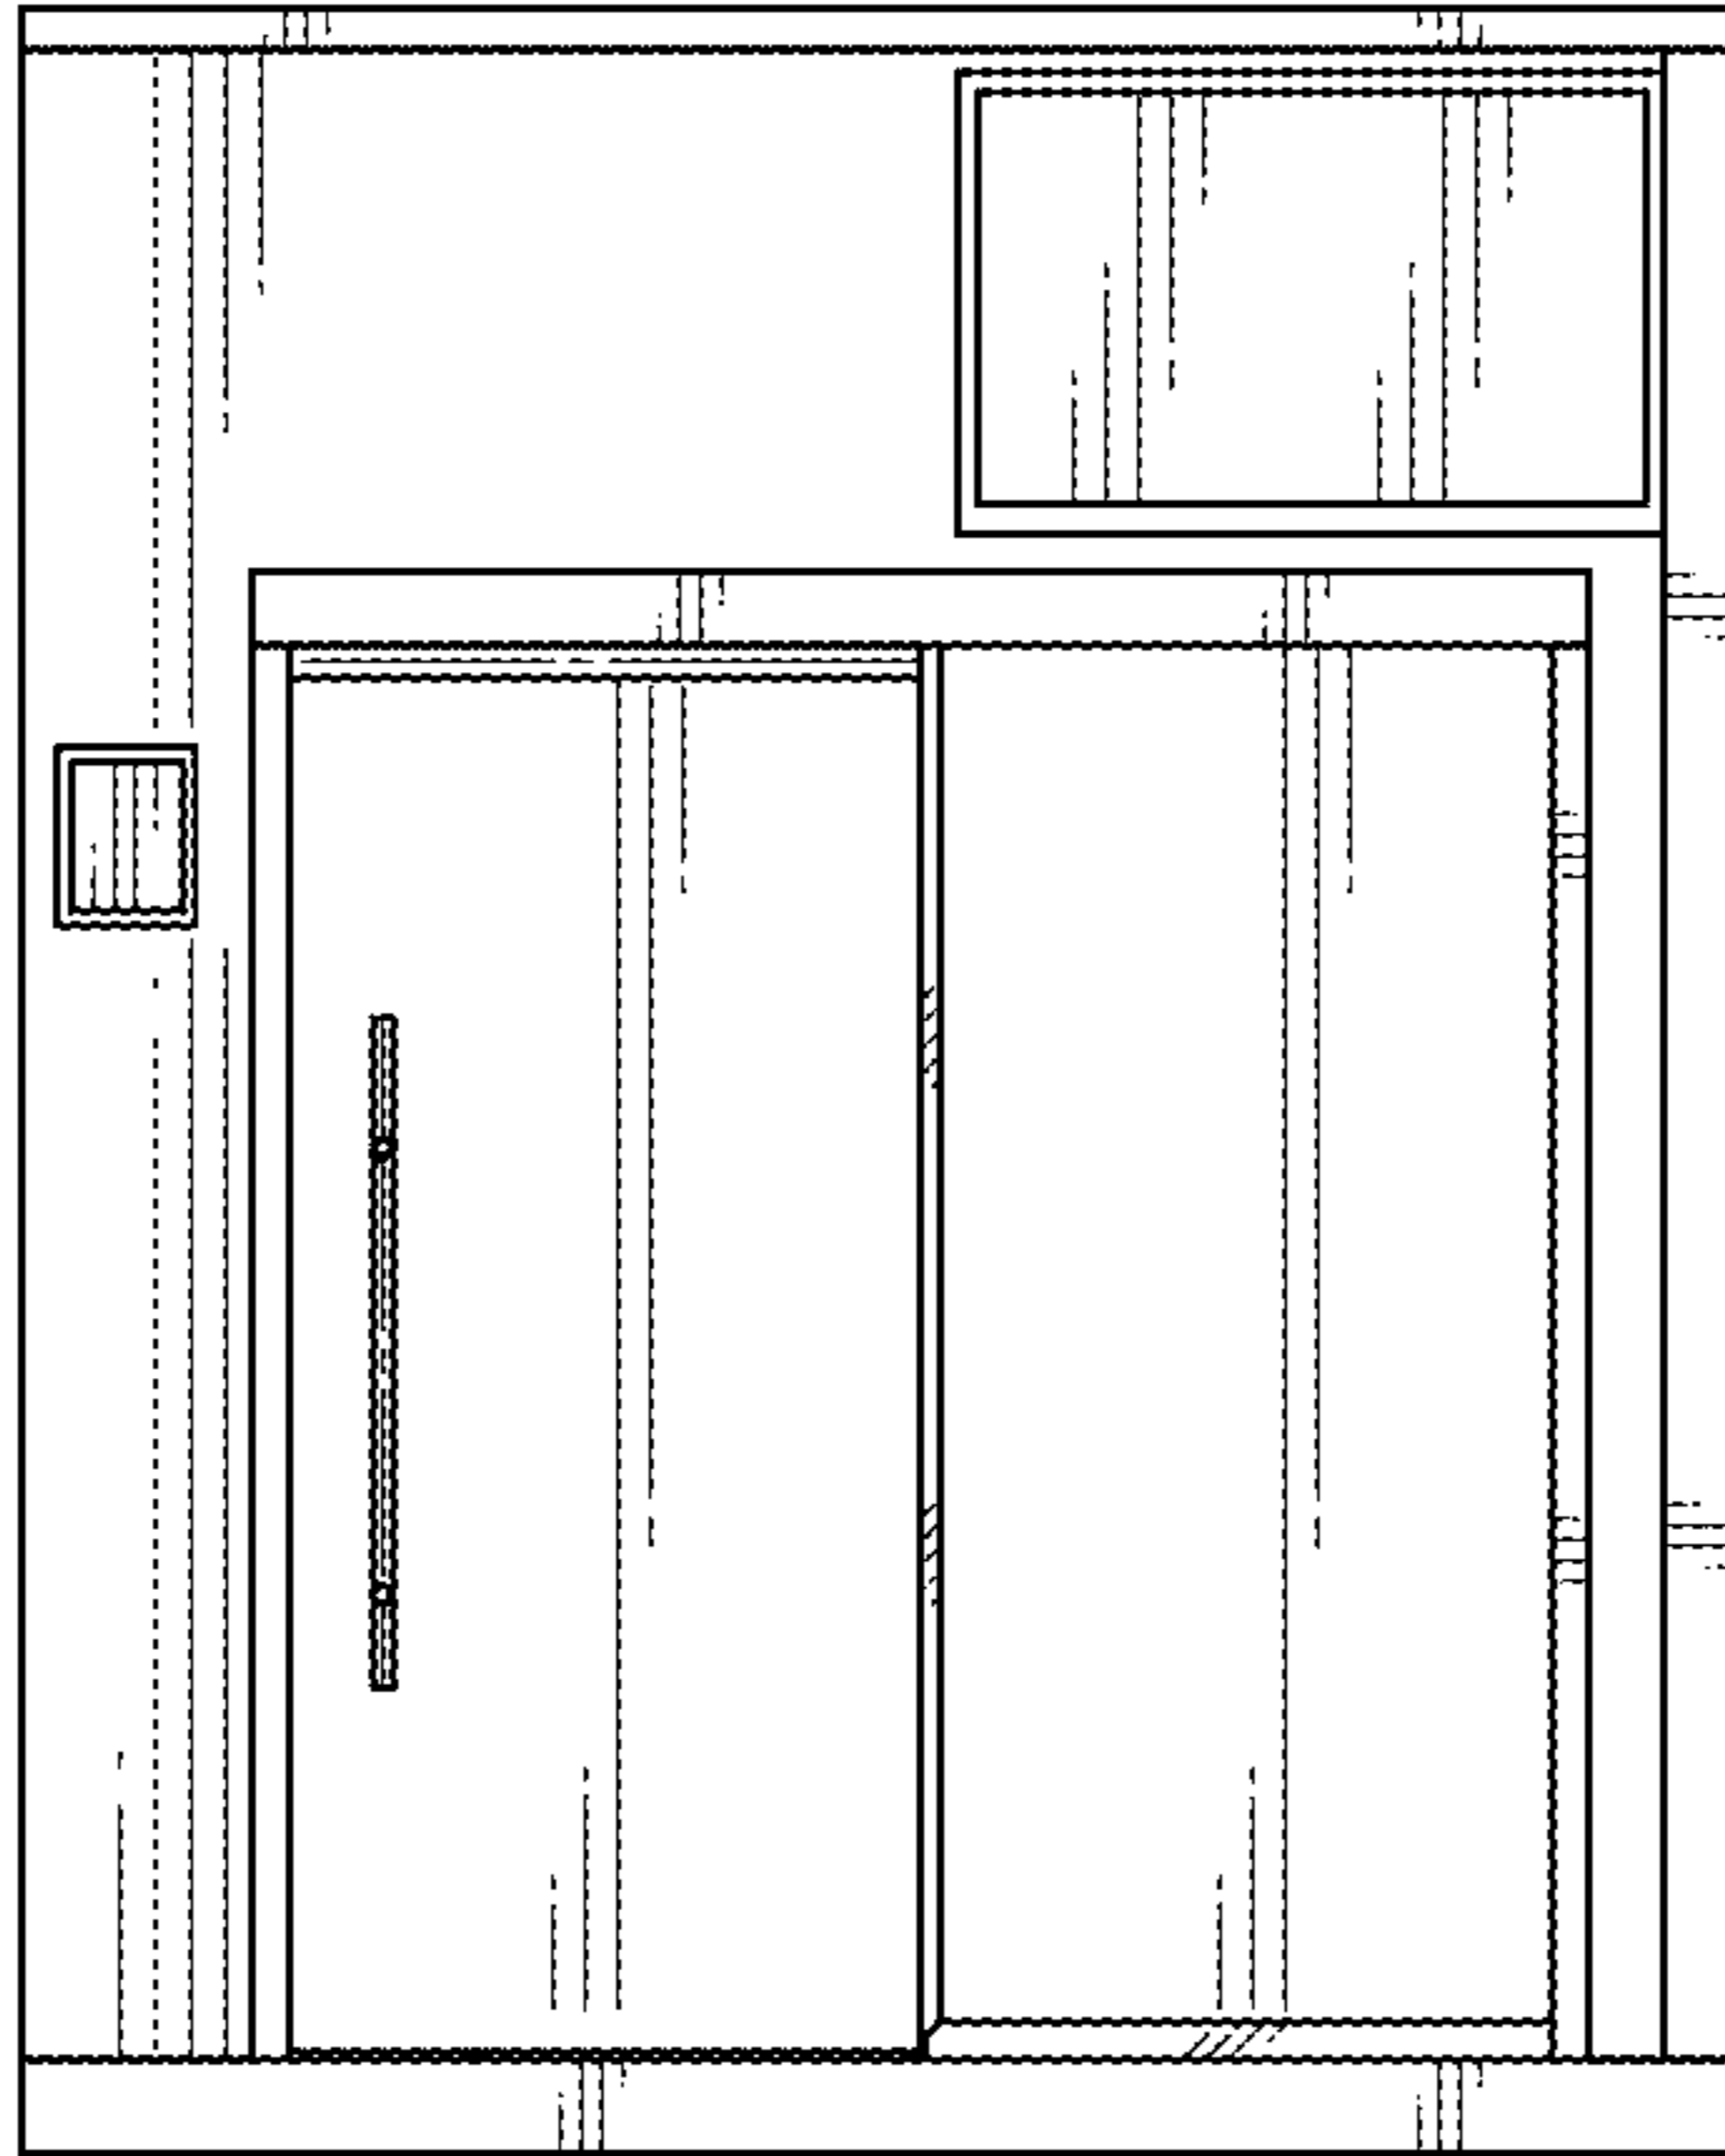


FIG. 5

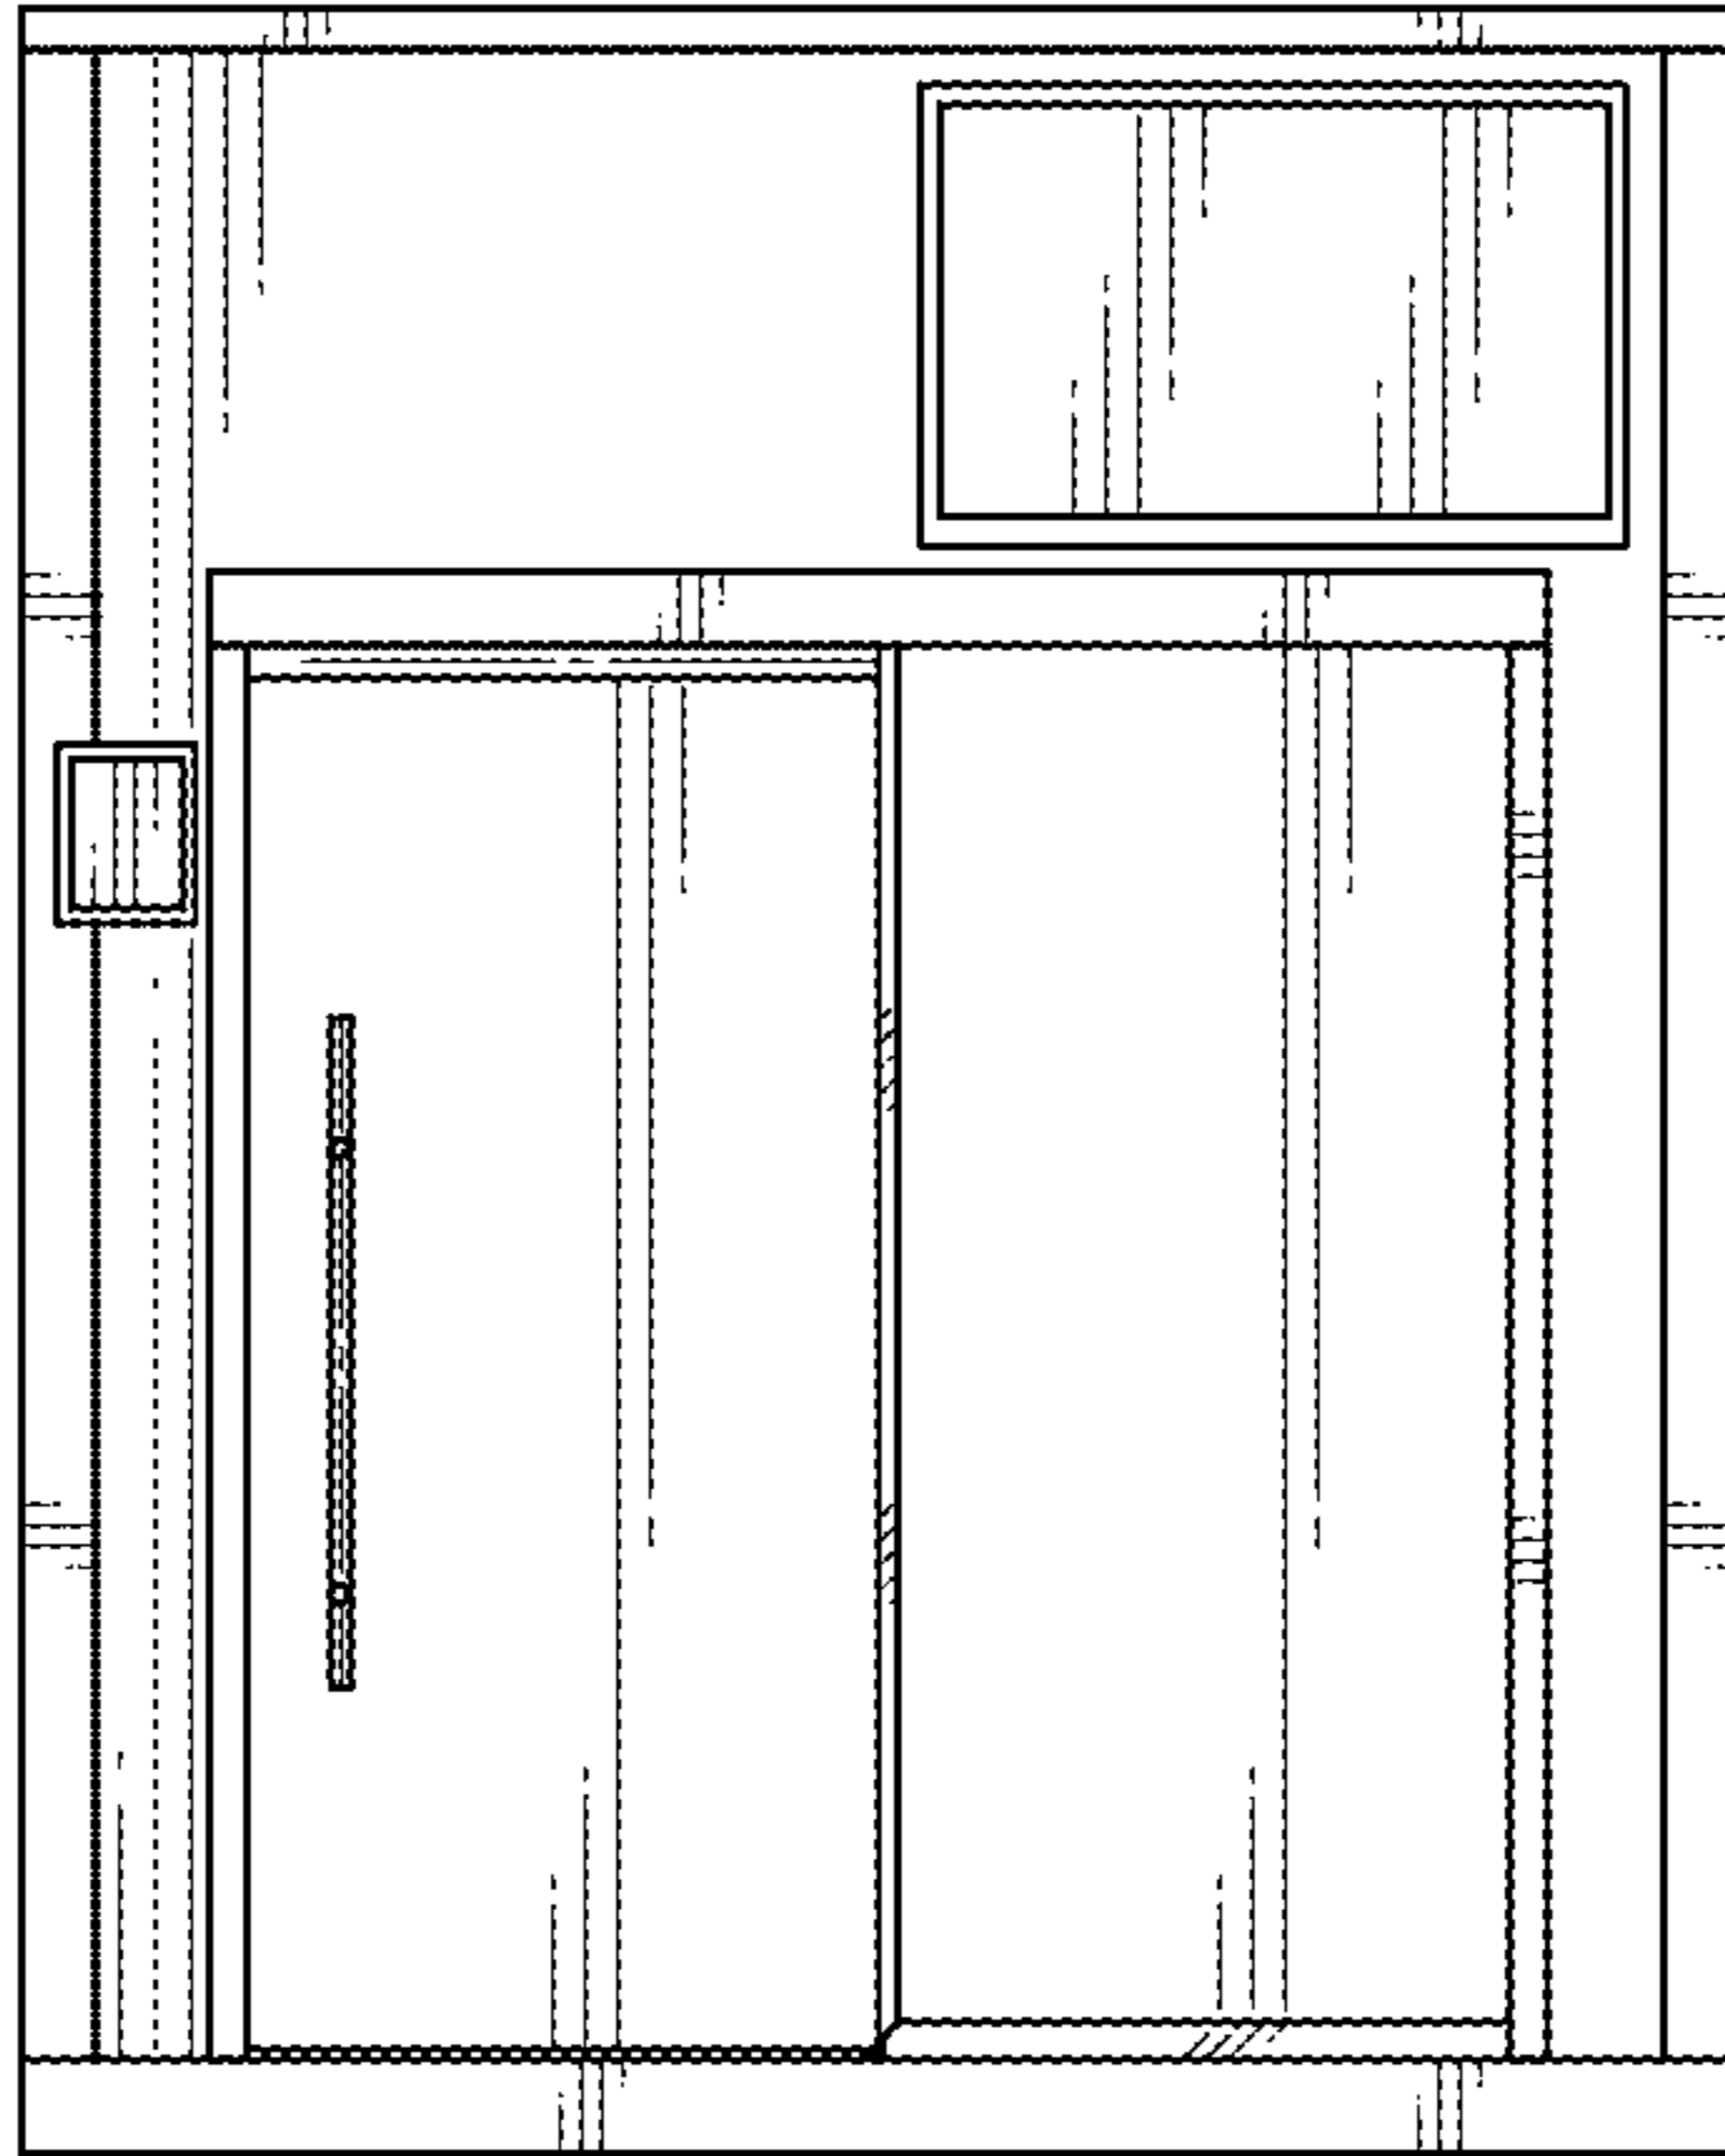


FIG. 6



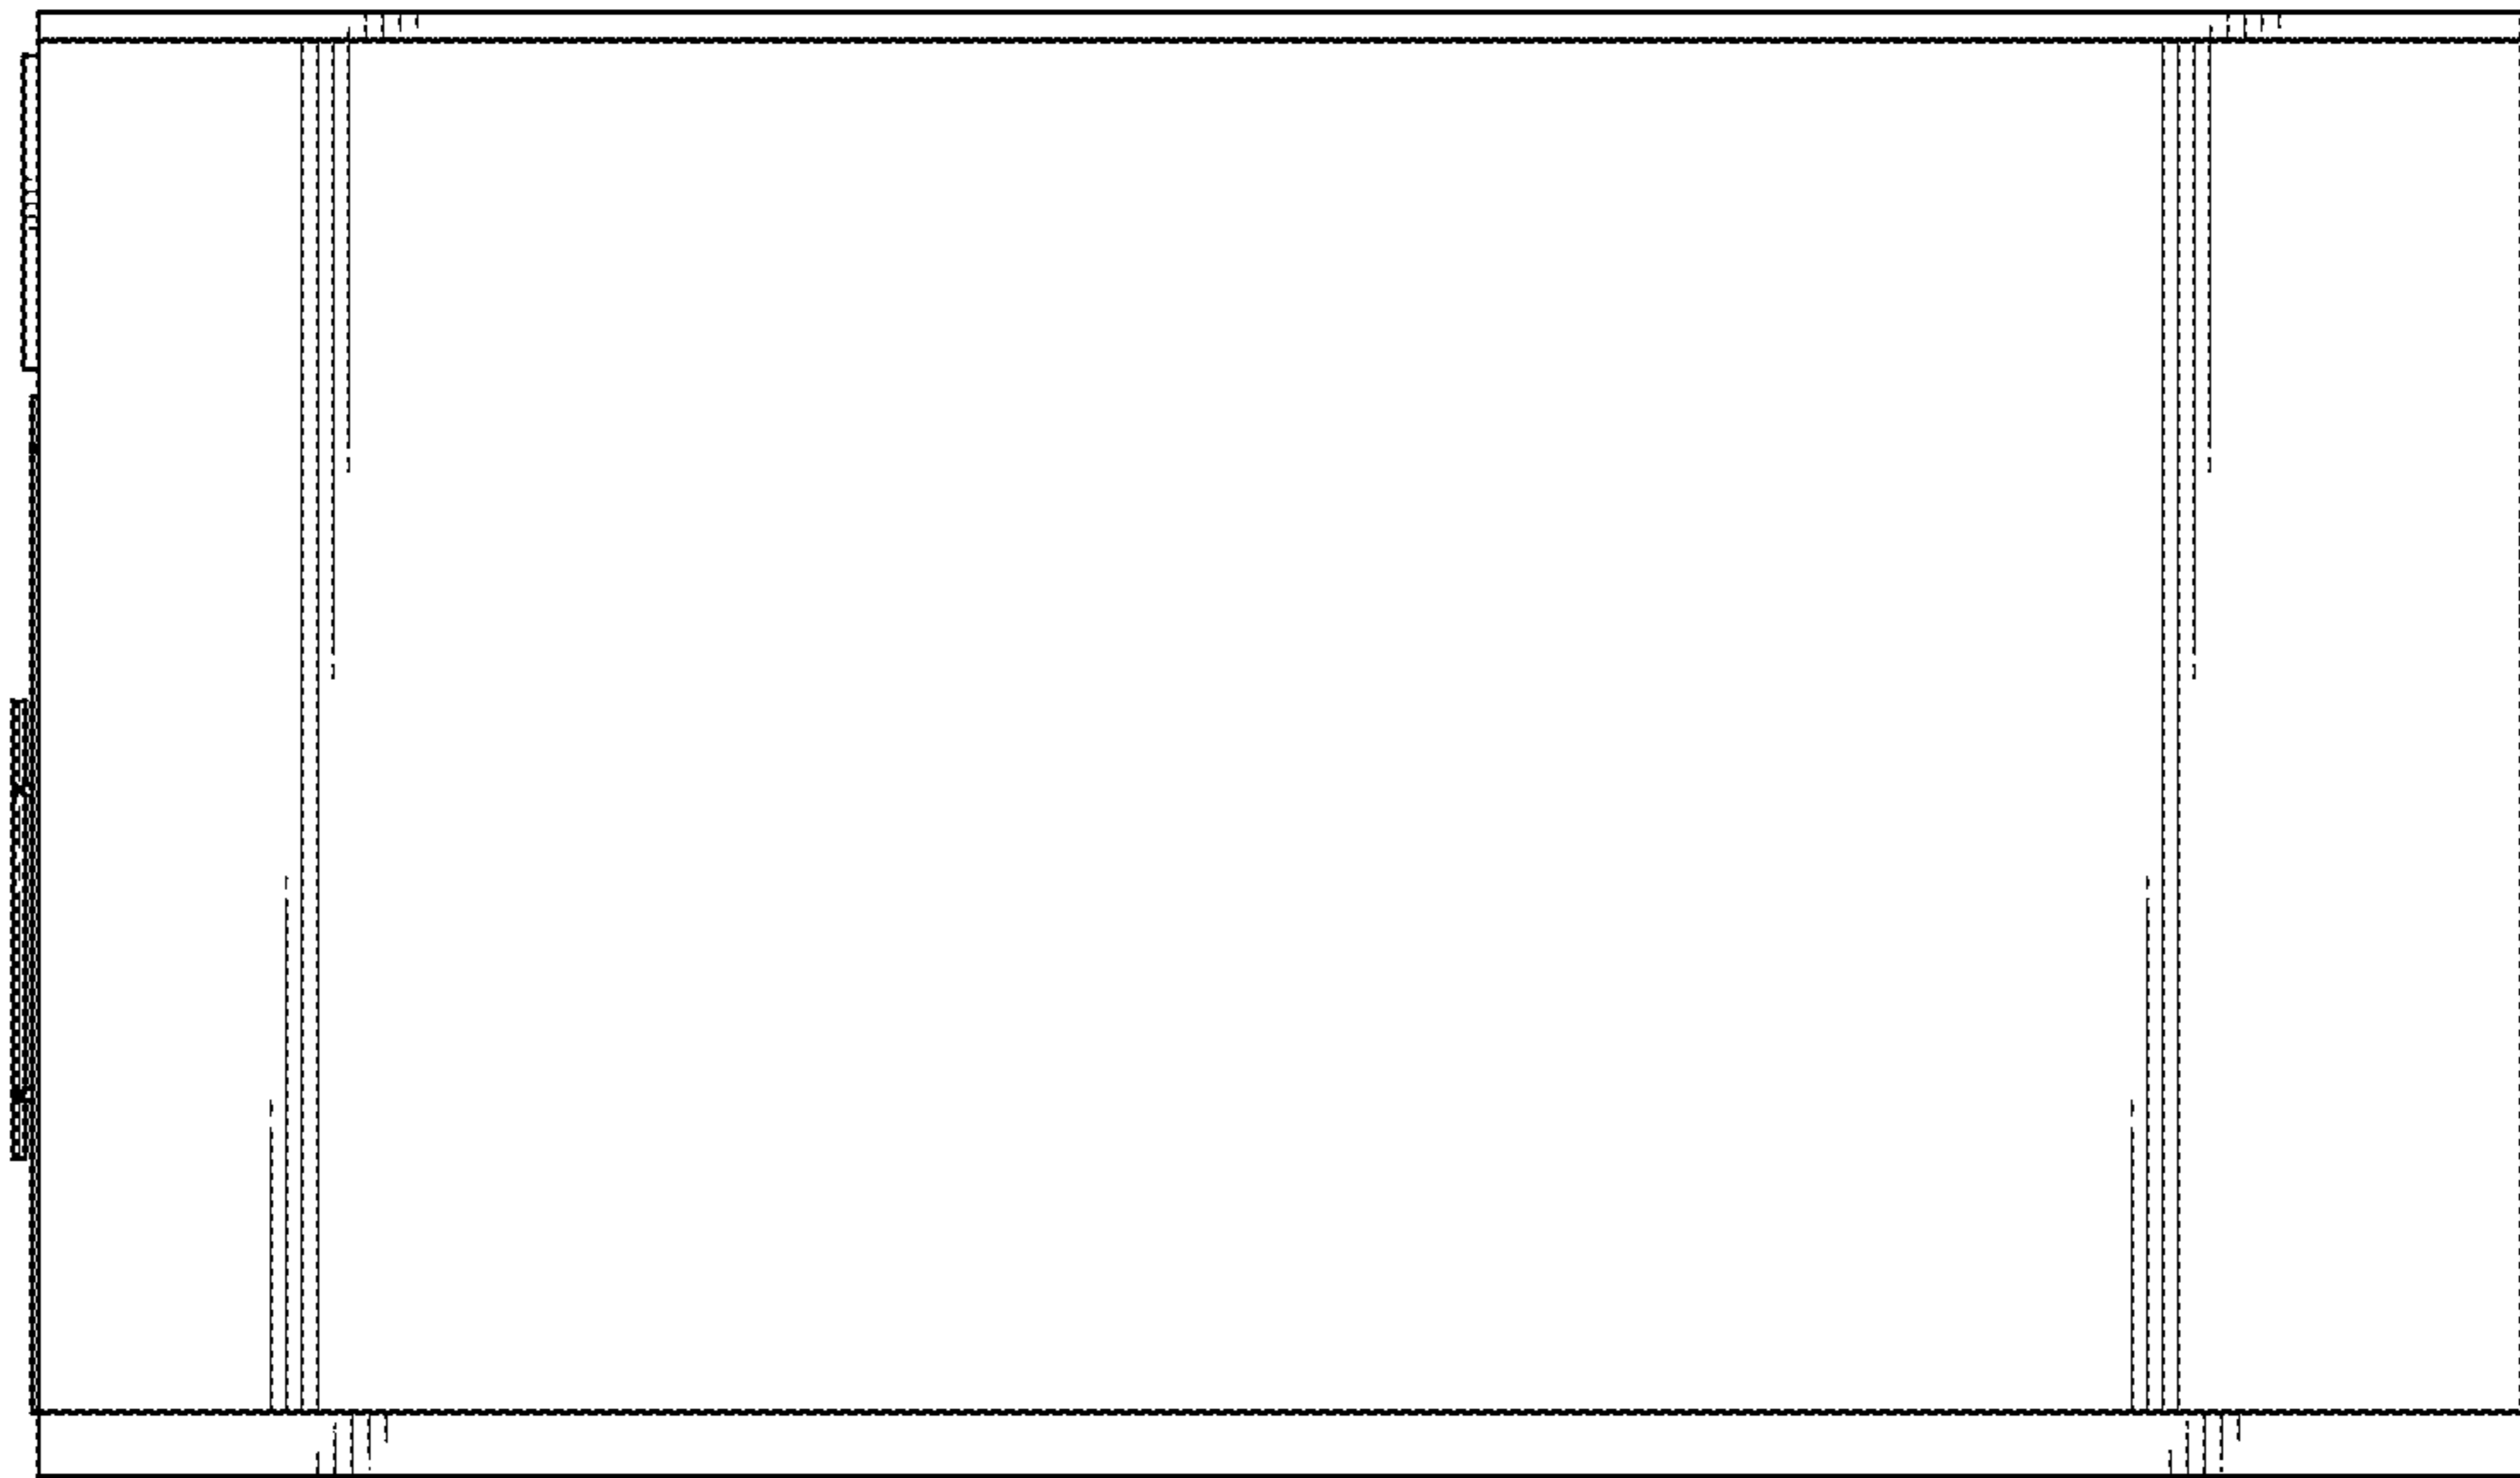


FIG. 7

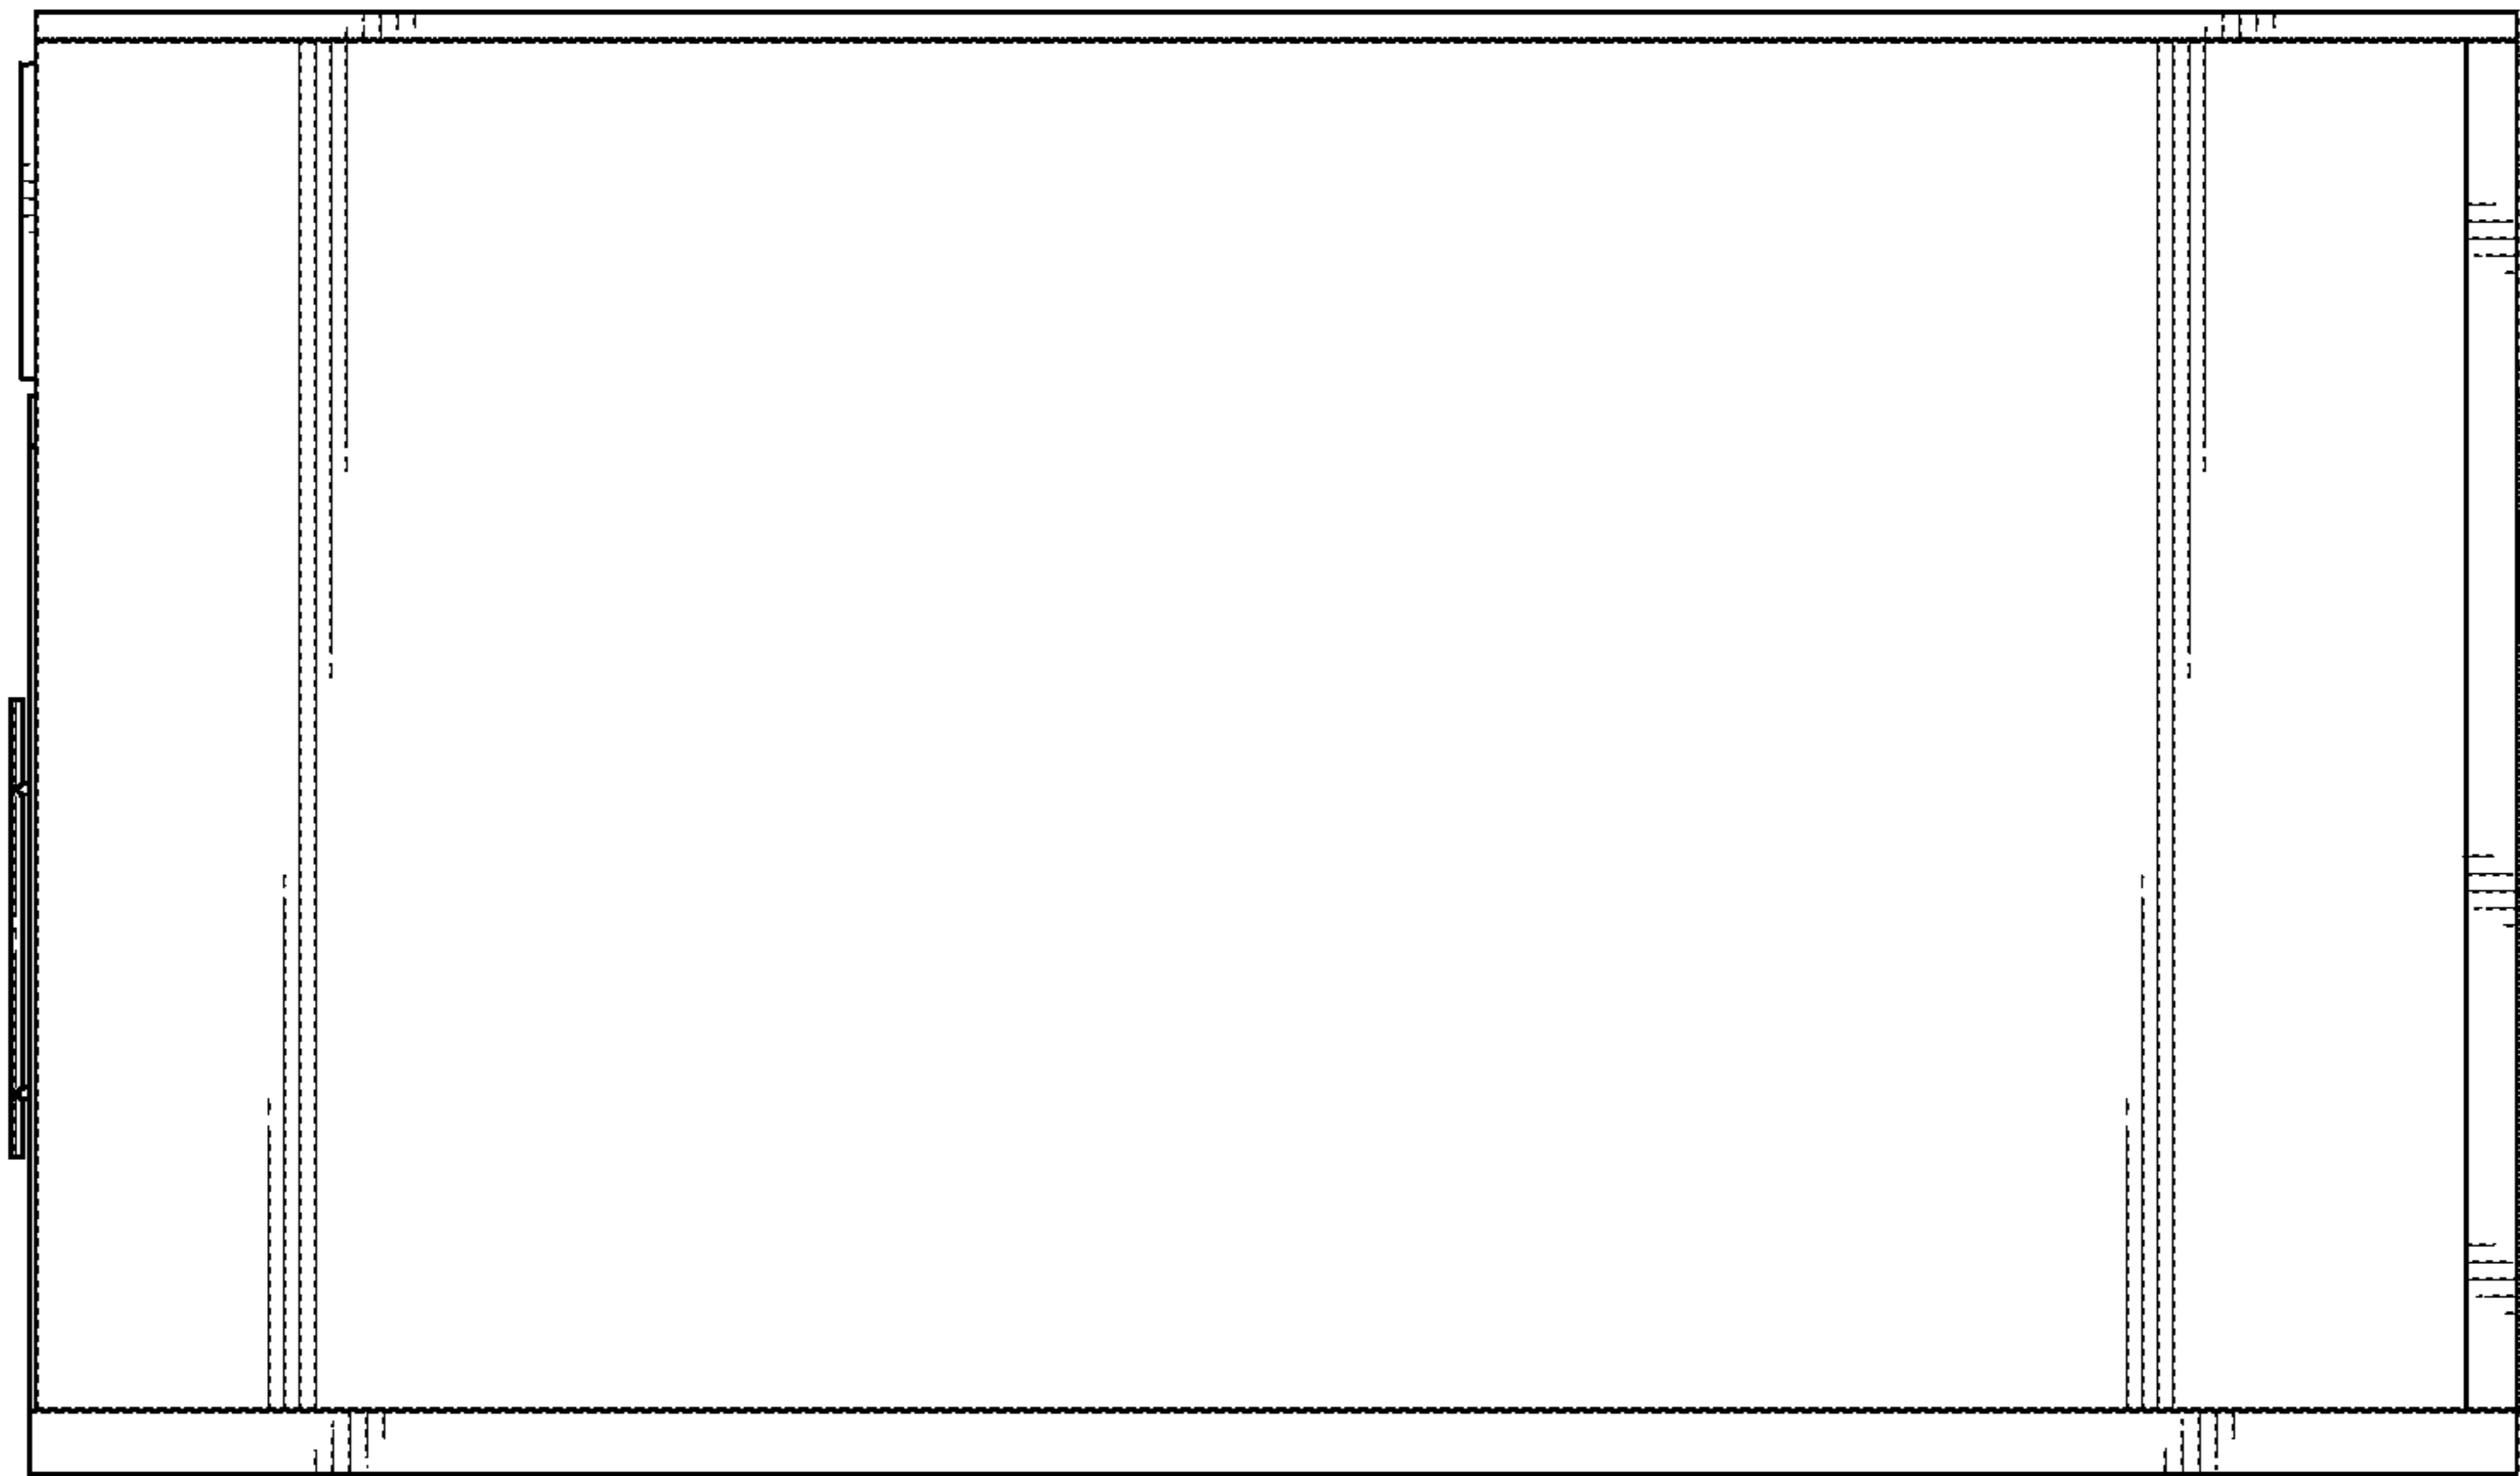


FIG. 8

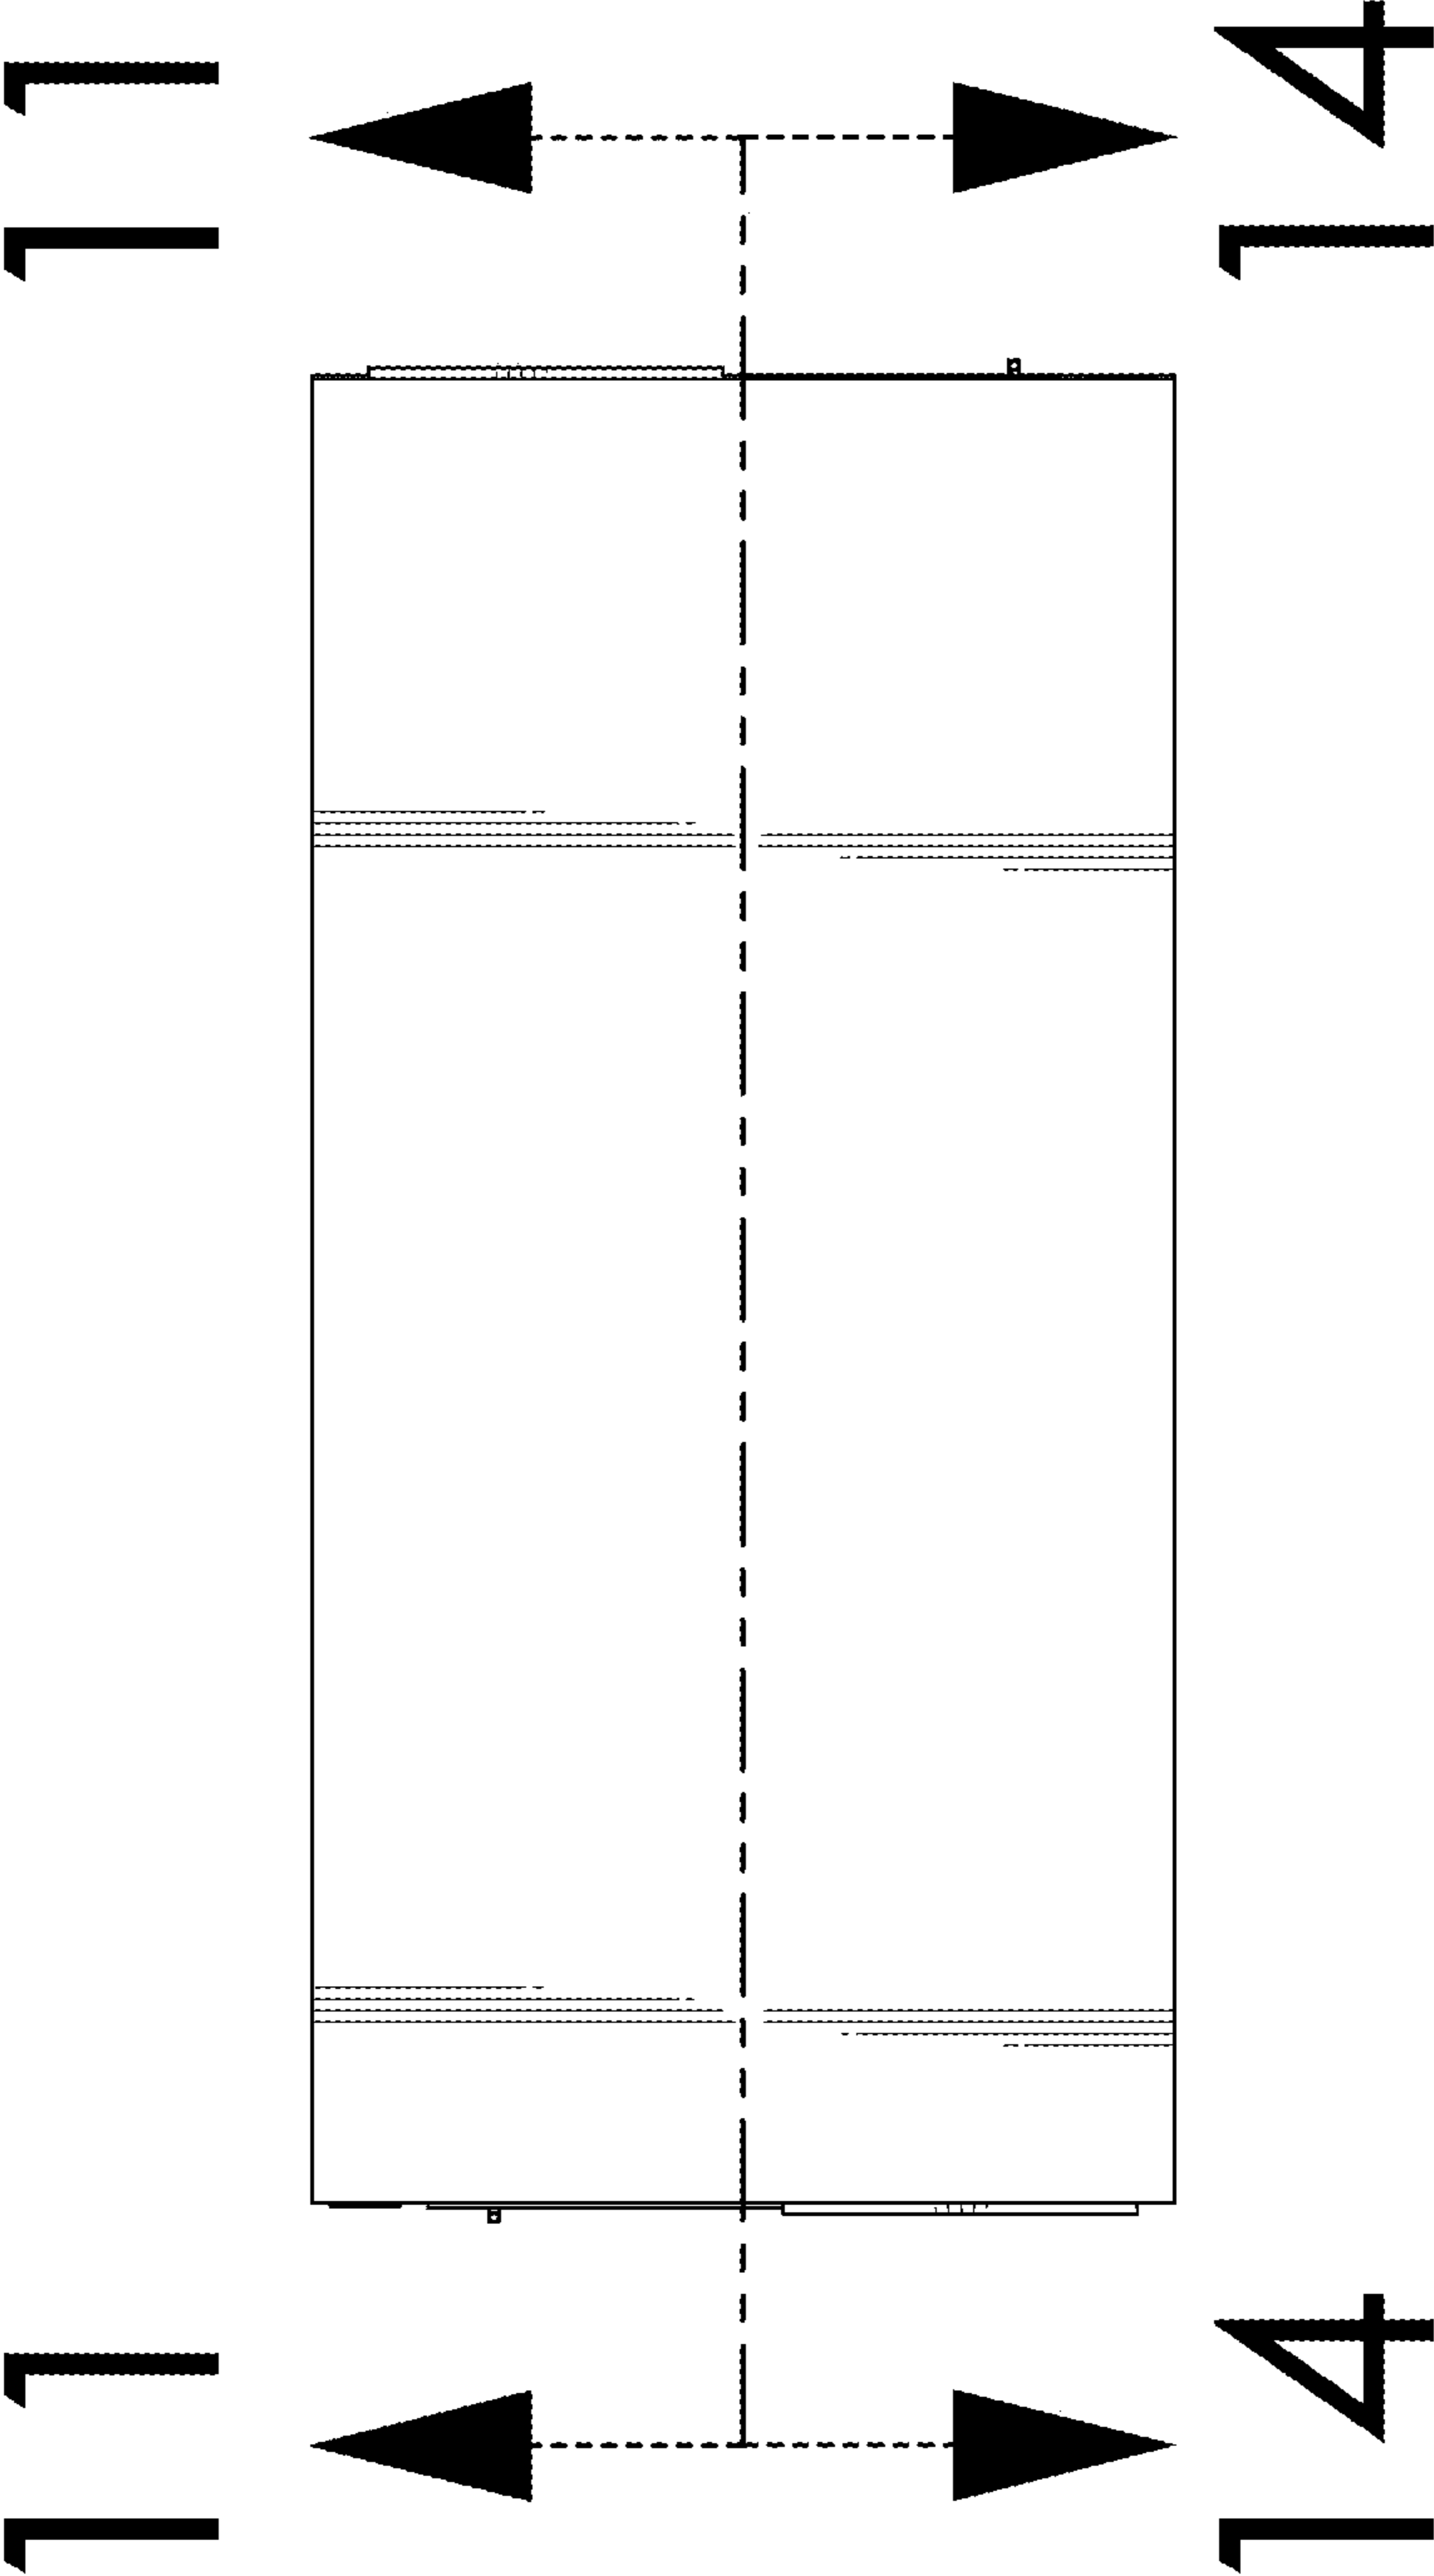


FIG. 9

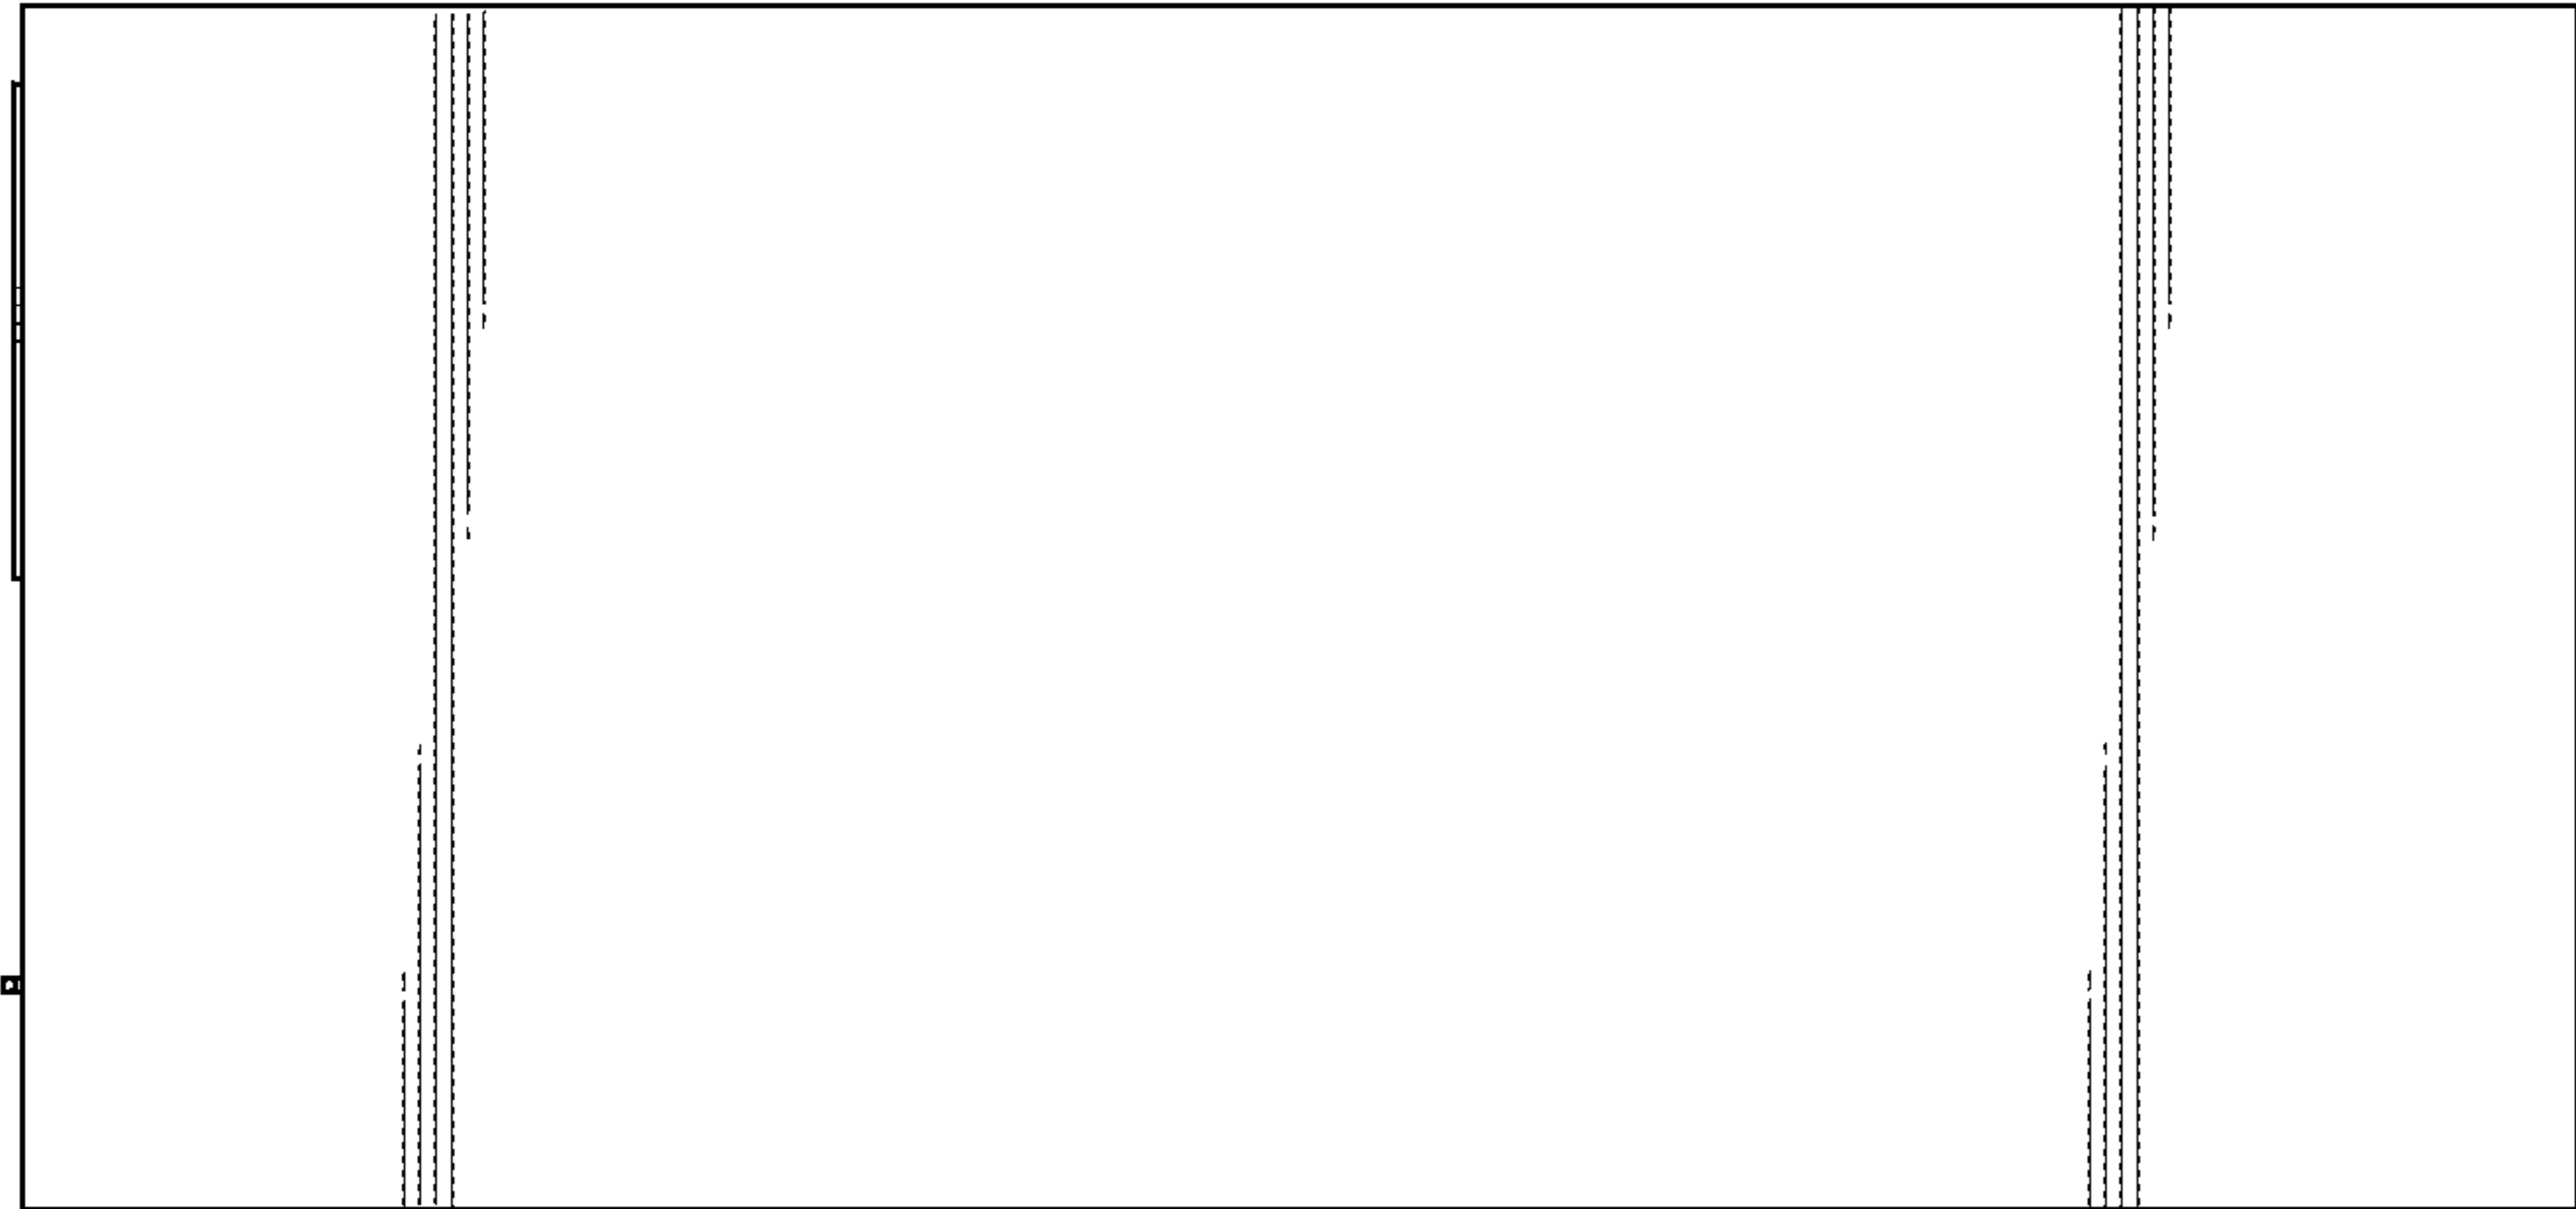


FIG. 10

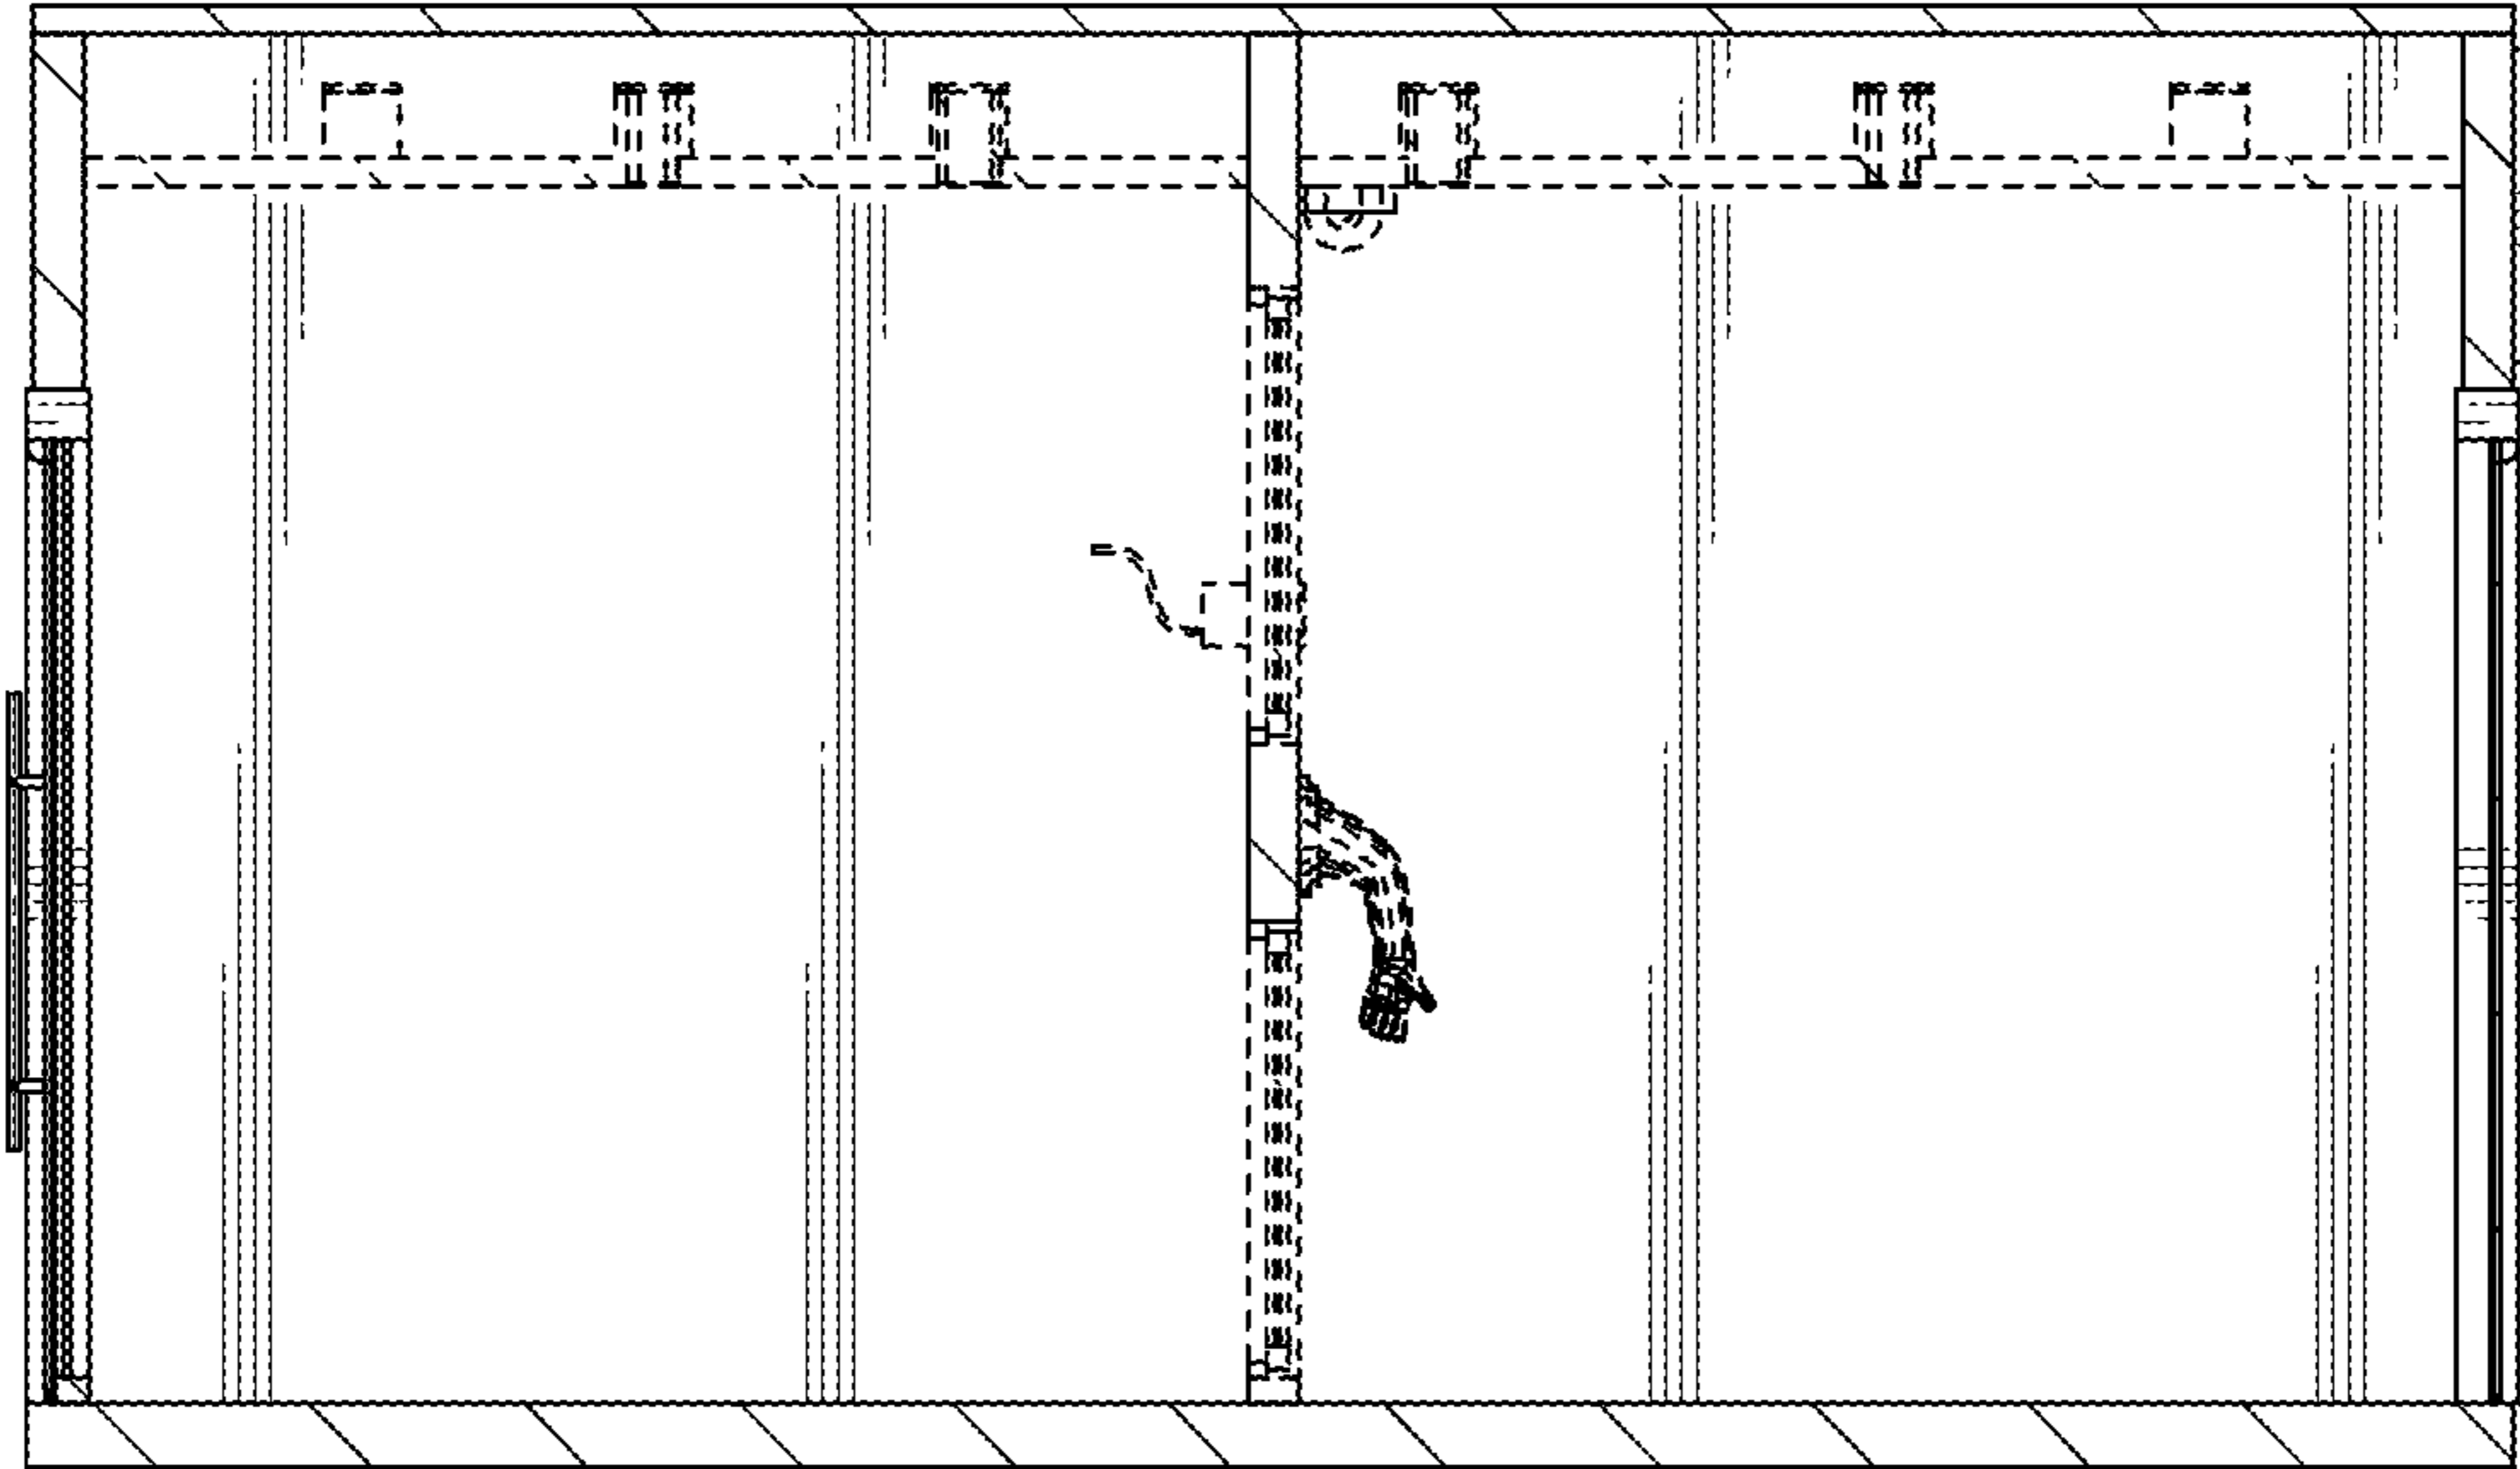


FIG. 11

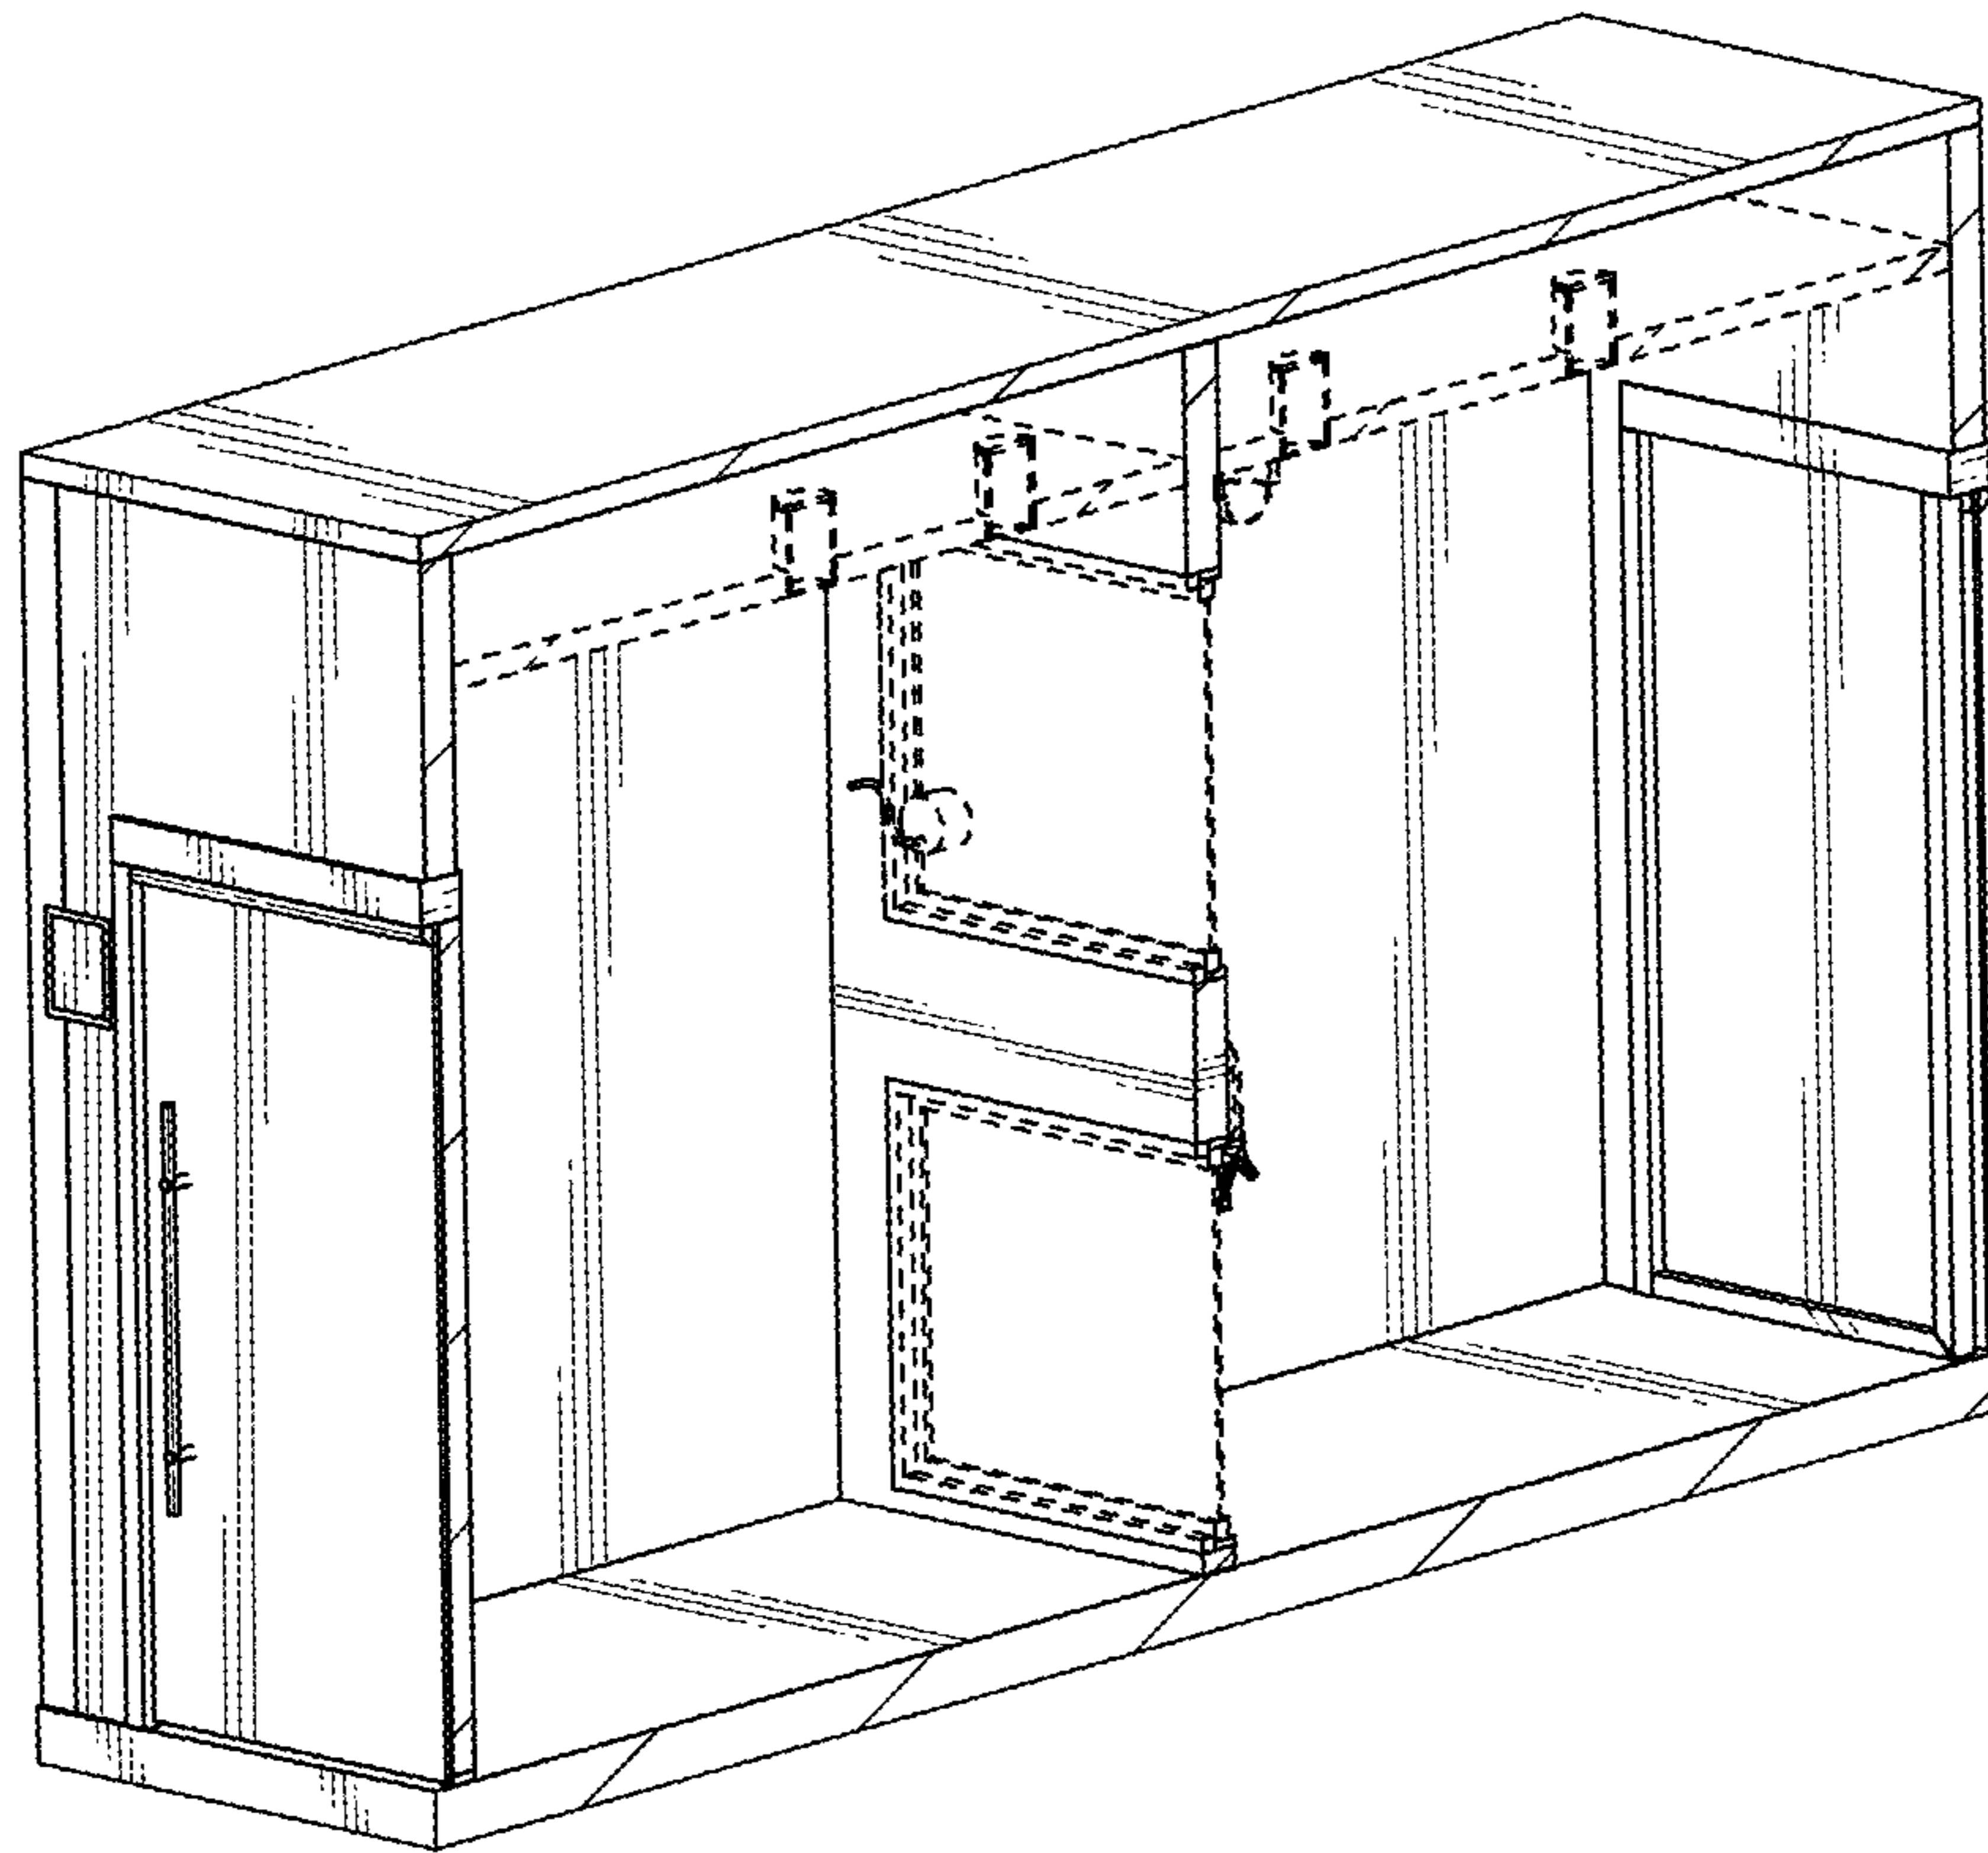


FIG. 12

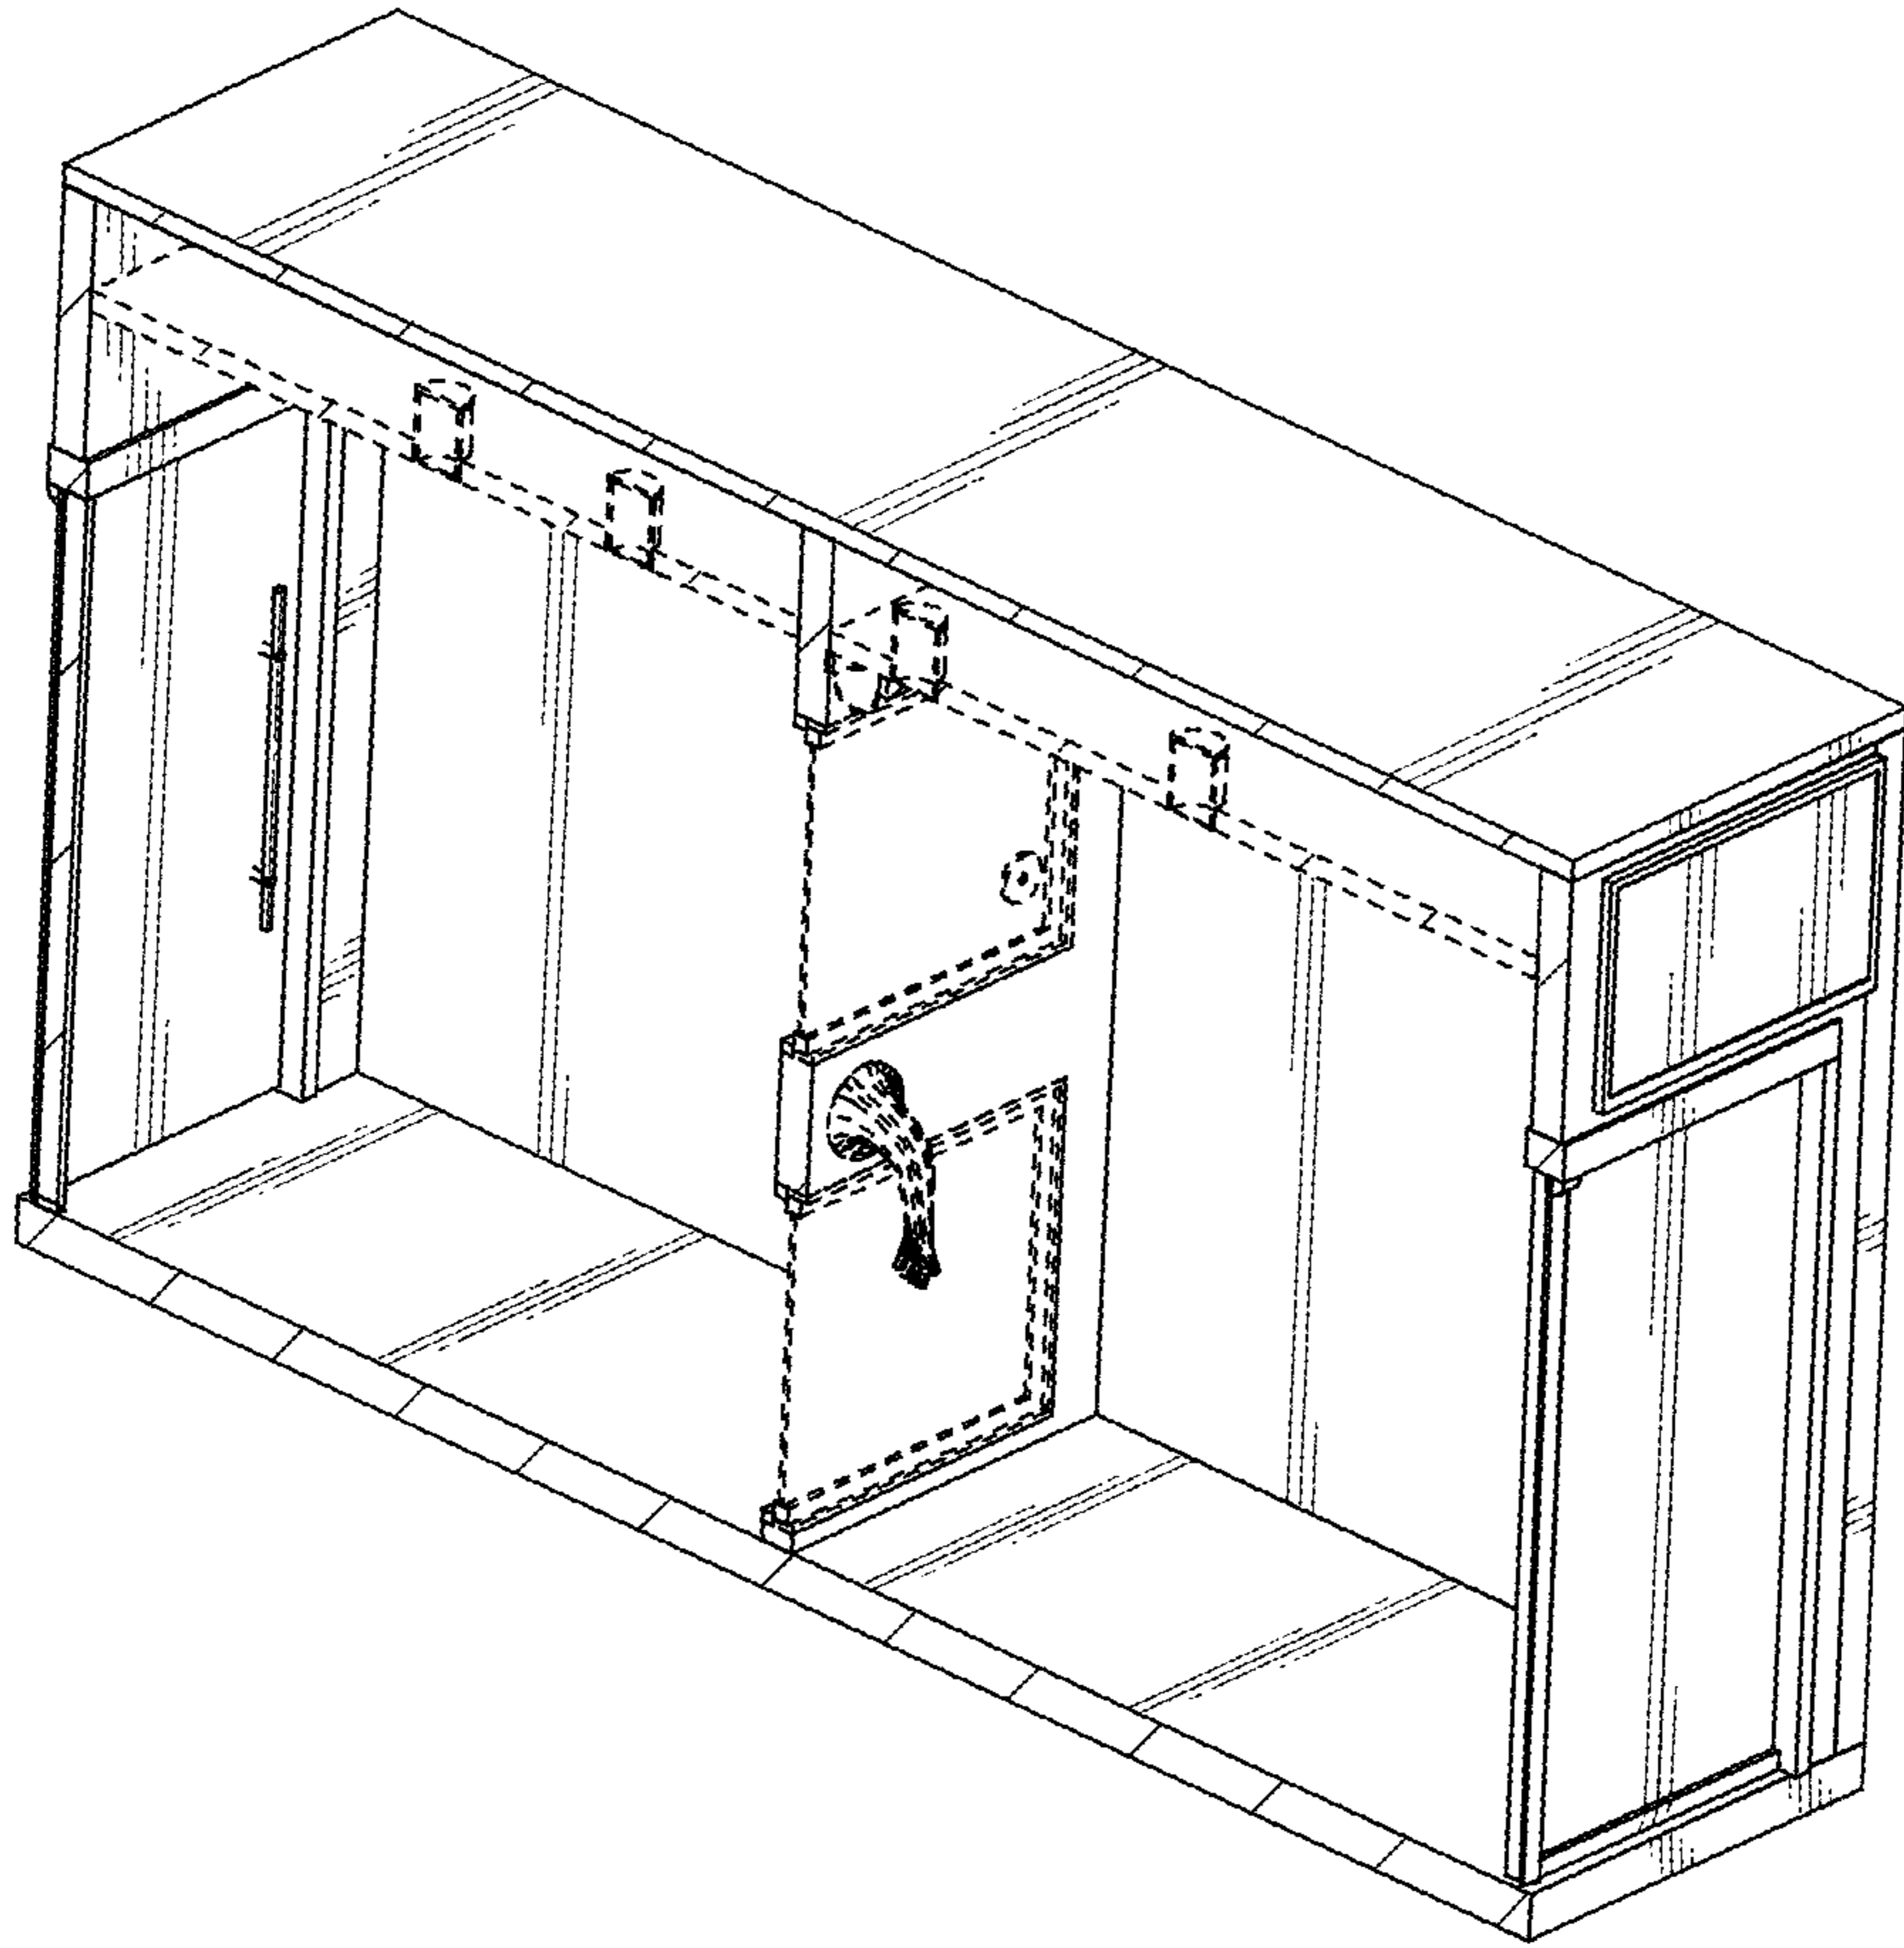


FIG. 13

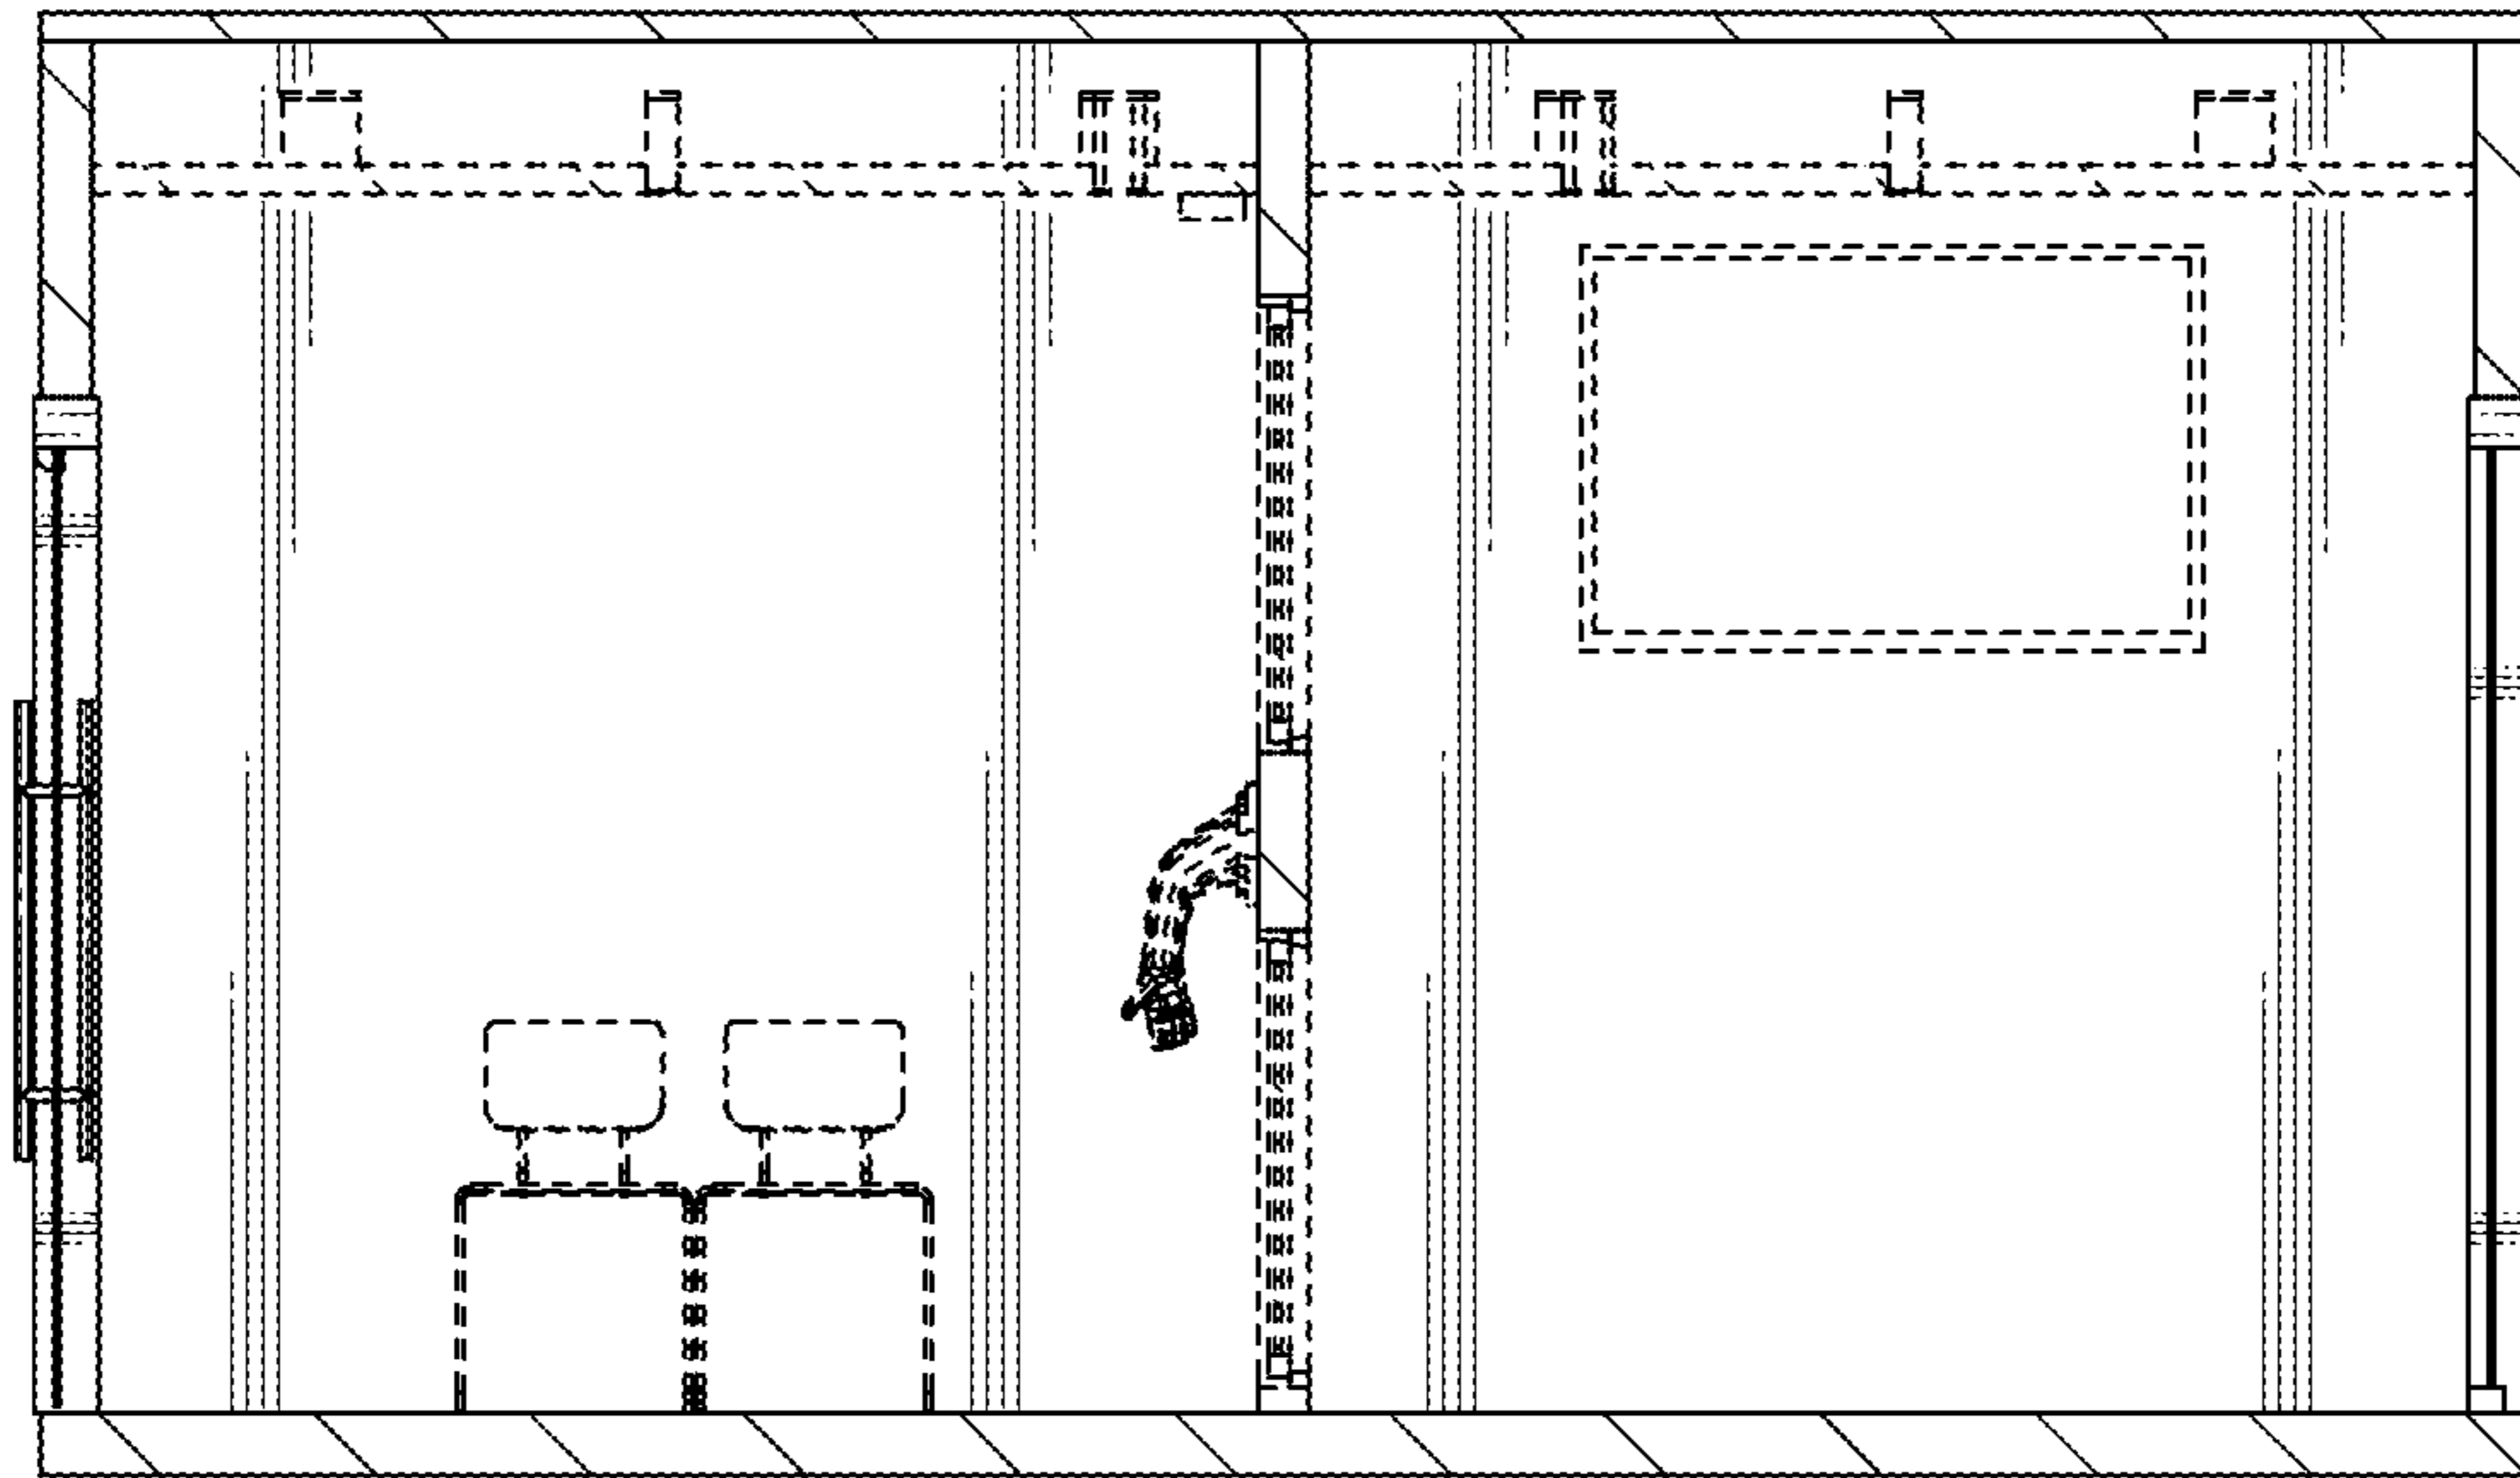


FIG. 14



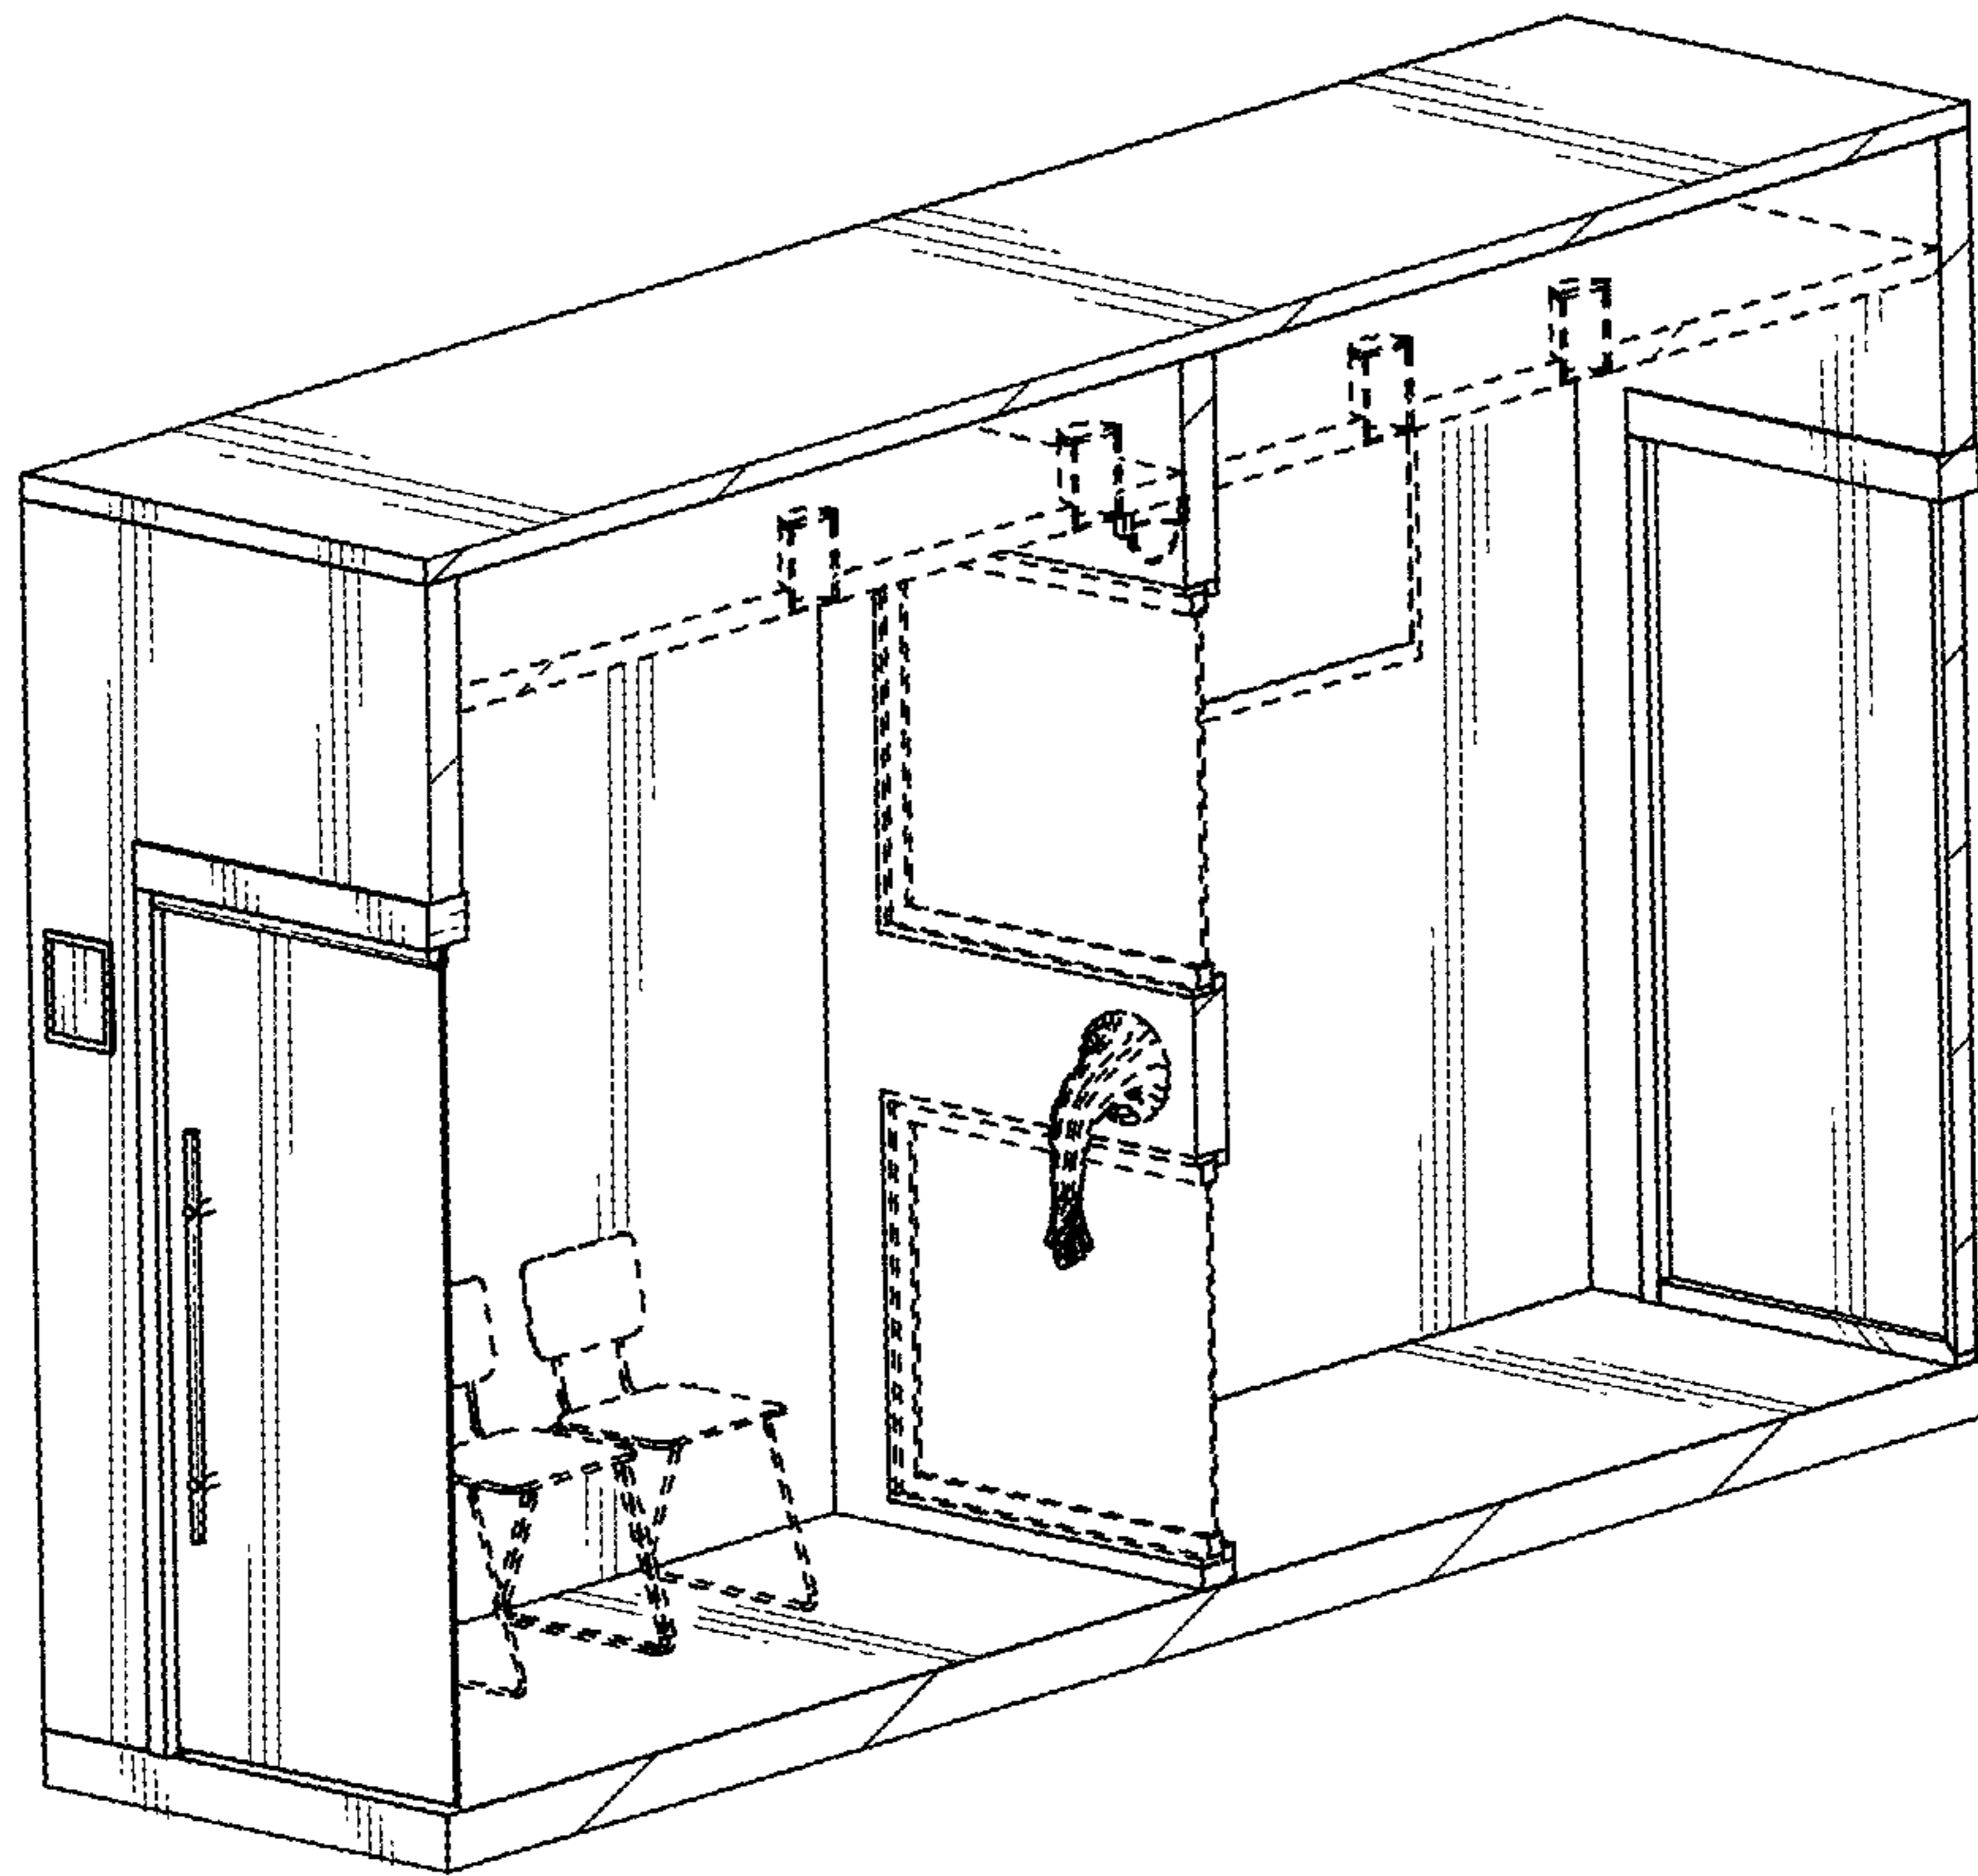


FIG. 15

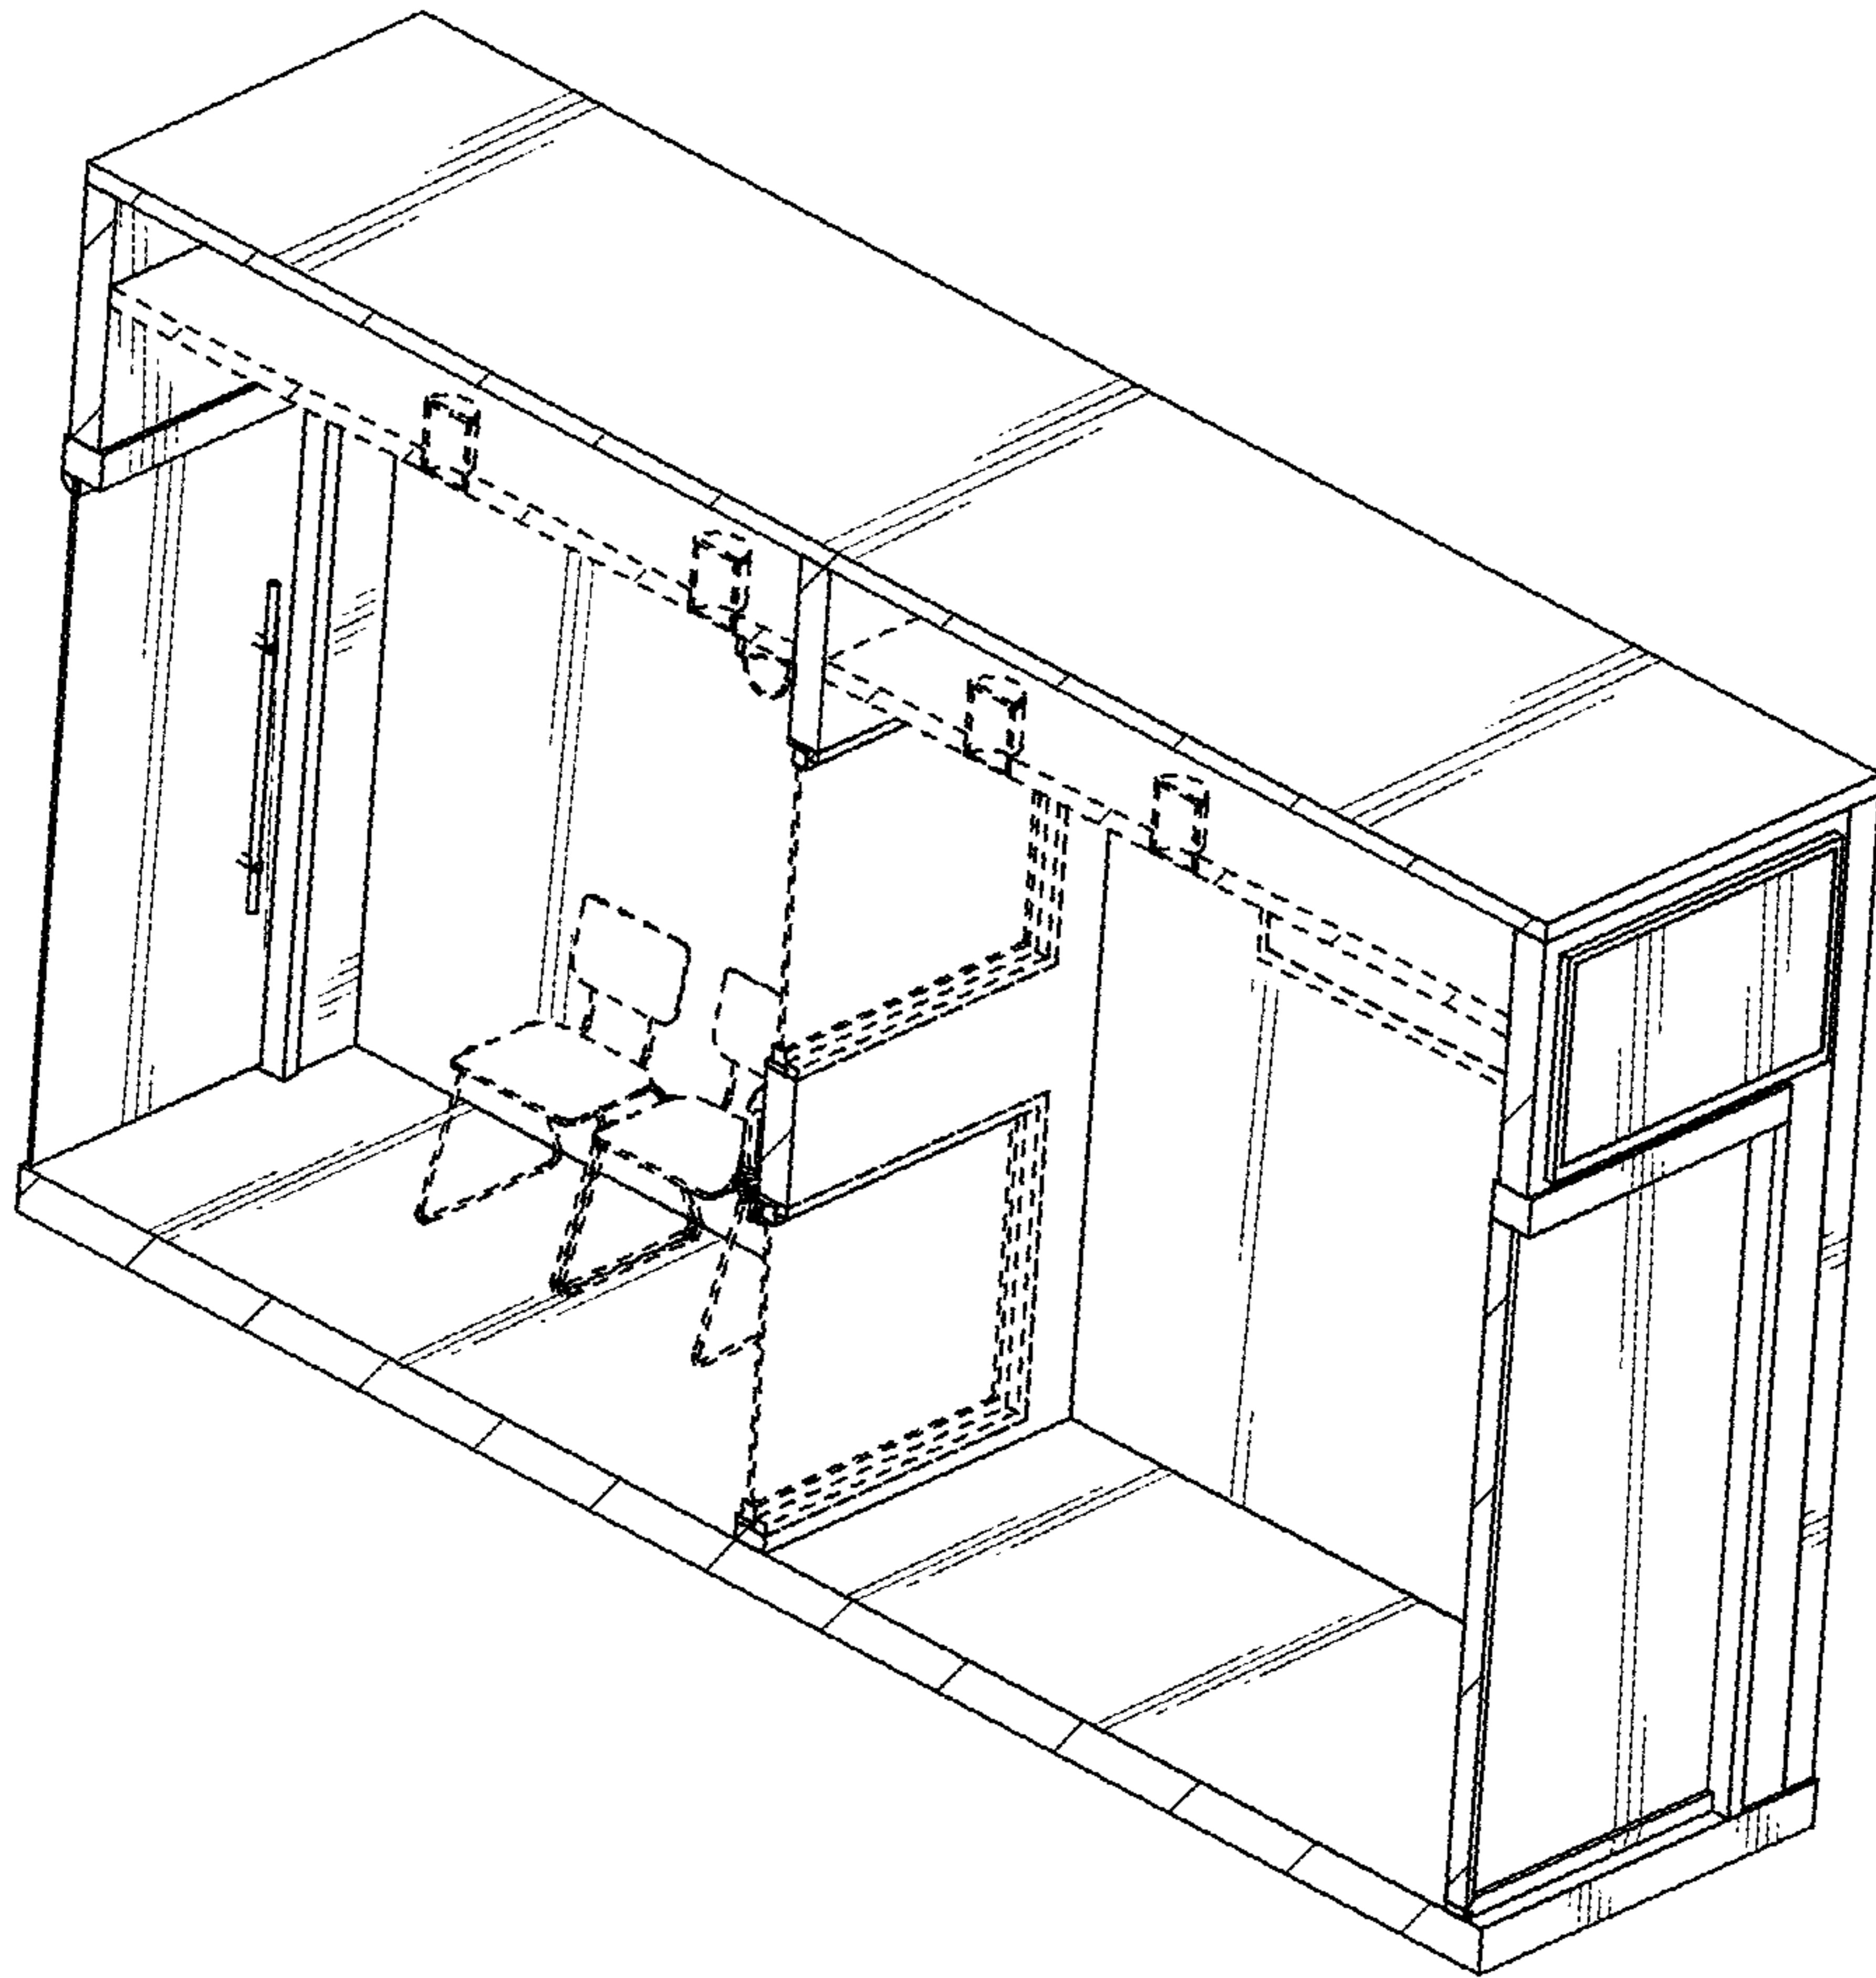


FIG. 16

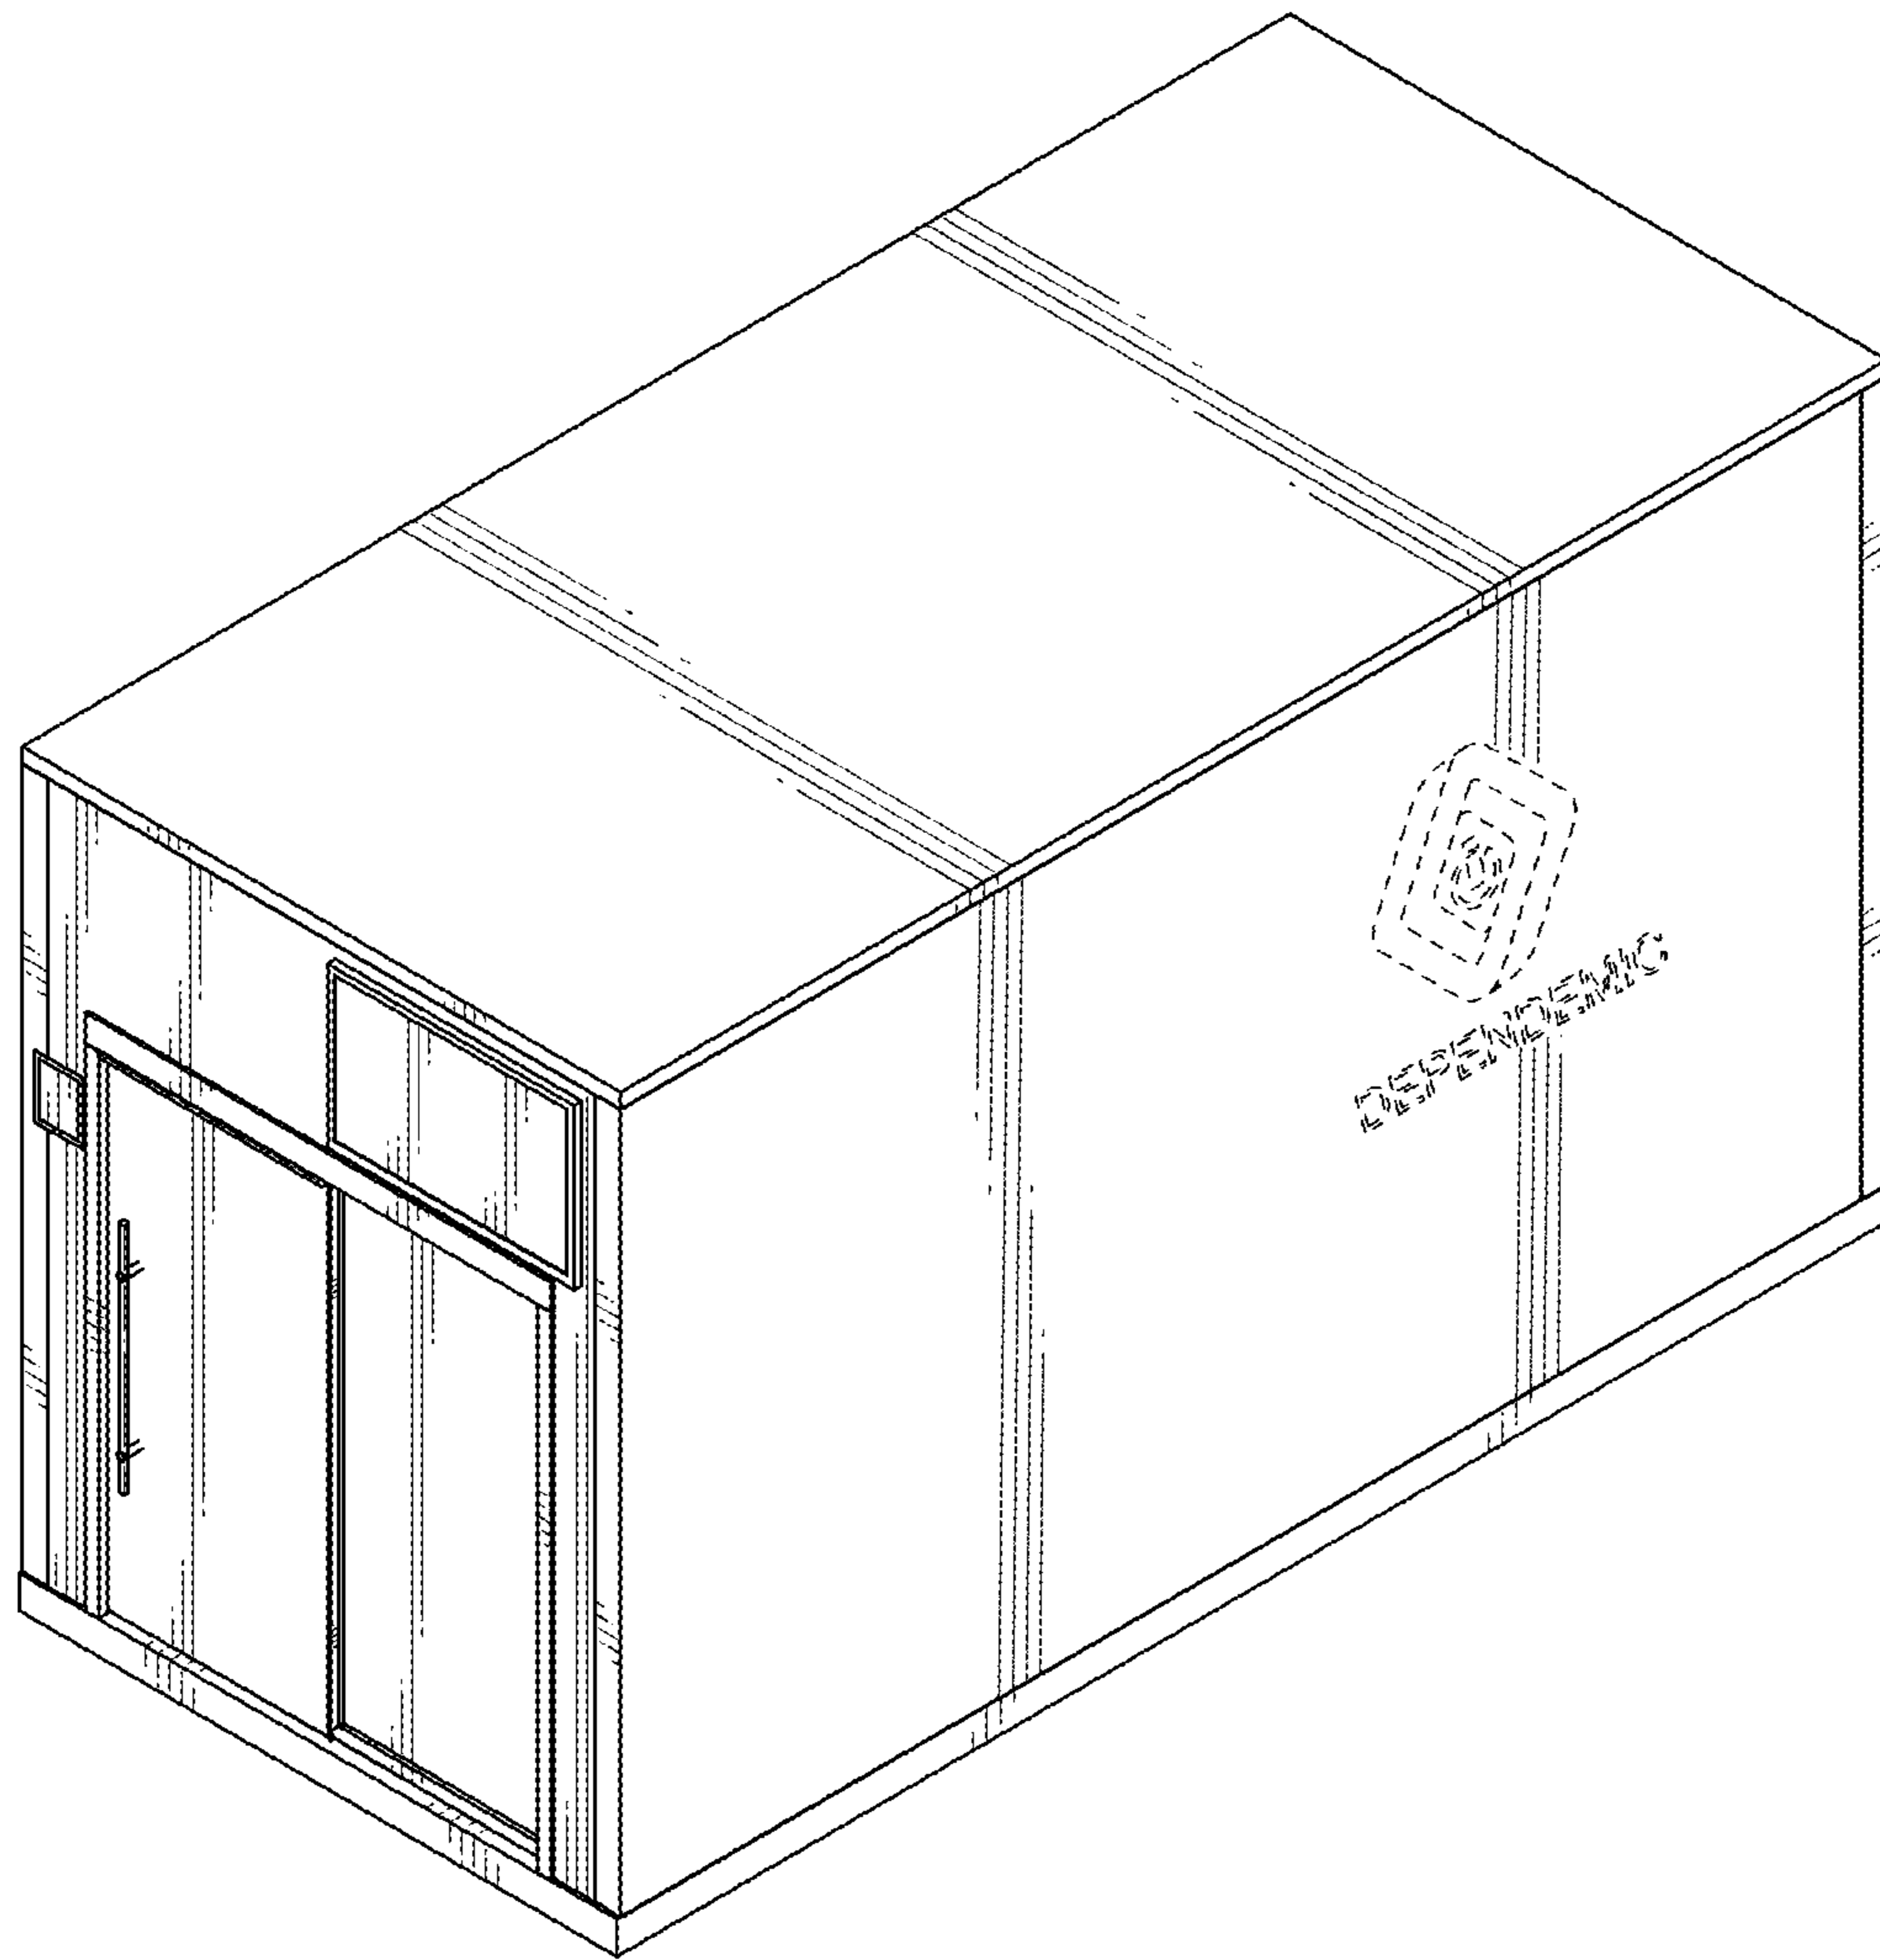


FIG. 17