



US00D971937S

(12) **United States Design Patent** (10) **Patent No.:** **US D971,937 S**  
**Mairs et al.** (45) **Date of Patent:** **\*\* Dec. 6, 2022**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH A GRAPHICAL USER INTERFACE**

(71) Applicant: **INSPIRE MEDICAL SYSTEMS, INC.**, Golden Valley, MN (US)

(72) Inventors: **Nicholas Mairs**, Minneapolis, MN (US); **Aaron Veicht**, Vadnais Heights, MN (US); **John Rondoni**, Plymouth, MN (US); **Donovan Fellows**, Lake Elmo, MN (US); **Brody Belland**, St. Louis Park, MN (US)

(73) Assignee: **INSPIRE MEDICAL SYSTEMS, INC.**, Golden Valley, MN (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/770,214**

(22) Filed: **Feb. 10, 2021**

(51) **LOC (13) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/485**

(58) **Field of Classification Search**  
USPC ..... D14/485–495  
CPC .... G06F 3/048; G06F 3/0481; G06F 3/04817; G06F 3/0482; G06F 3/0483; G06F 3/04842; G06F 3/0485; G06F 3/04855; G06F 3/0486; G06F 3/0488; G06F 3/04886; G06F 9/451; G06F 40/103; G06F 40/106; G06F 40/189; G06F 40/191

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D720,765 S \* 1/2015 Xie ..... D14/486  
D783,649 S \* 4/2017 Wu ..... D14/492  
D797,118 S \* 9/2017 Van Every ..... D14/485  
D817,339 S \* 5/2018 Nanjappan ..... D14/492

D819,056 S \* 5/2018 Nanjappan ..... D14/485  
D822,050 S \* 7/2018 Gandhi ..... D14/486  
D822,702 S \* 7/2018 Gandhi ..... D14/486  
D843,406 S \* 3/2019 Heckerman ..... D14/486  
D870,144 S \* 12/2019 Mensinger ..... D14/488  
D890,792 S \* 7/2020 Valladares ..... D14/486  
D903,700 S \* 12/2020 Valladares ..... D14/486  
D914,032 S \* 3/2021 Einspahr ..... D14/485  
D916,108 S \* 4/2021 Stoeckle ..... D14/486  
D916,117 S \* 4/2021 Downie ..... D14/486  
D919,644 S \* 5/2021 Jang ..... D14/486  
D923,638 S \* 6/2021 Vautrin ..... H04R 3/04  
D14/485  
D928,176 S \* 8/2021 Hamre ..... D14/485  
D928,805 S \* 8/2021 Yore ..... D14/485  
D931,302 S \* 9/2021 Rhyu ..... D14/485  
D938,469 S \* 12/2021 Varga ..... D14/486  
D942,994 S \* 2/2022 Dalonzo ..... D14/486  
2010/0023865 A1 \* 1/2010 Fulker ..... G08B 25/14  
700/286  
2019/0365228 A1 12/2019 Rondoni et al.

\* cited by examiner

Primary Examiner — Nicole C Shiflet

(74) Attorney, Agent, or Firm — Dicke, Billig & Czaja, PLLC


(57) **CLAIM**

The ornamental design for a display screen or portion thereof with a graphical user interface, as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of a display screen or portion thereof with a graphical user interface showing our new design; and, FIG. 2 is a front view of a second embodiment thereof. In the FIGURES, the outermost broken lines show a display screen or portion thereof and form no part of the claimed design. The remaining broken lines show elements of the graphical user interface that form no part of the claimed design.

**1 Claim, 2 Drawing Sheets**

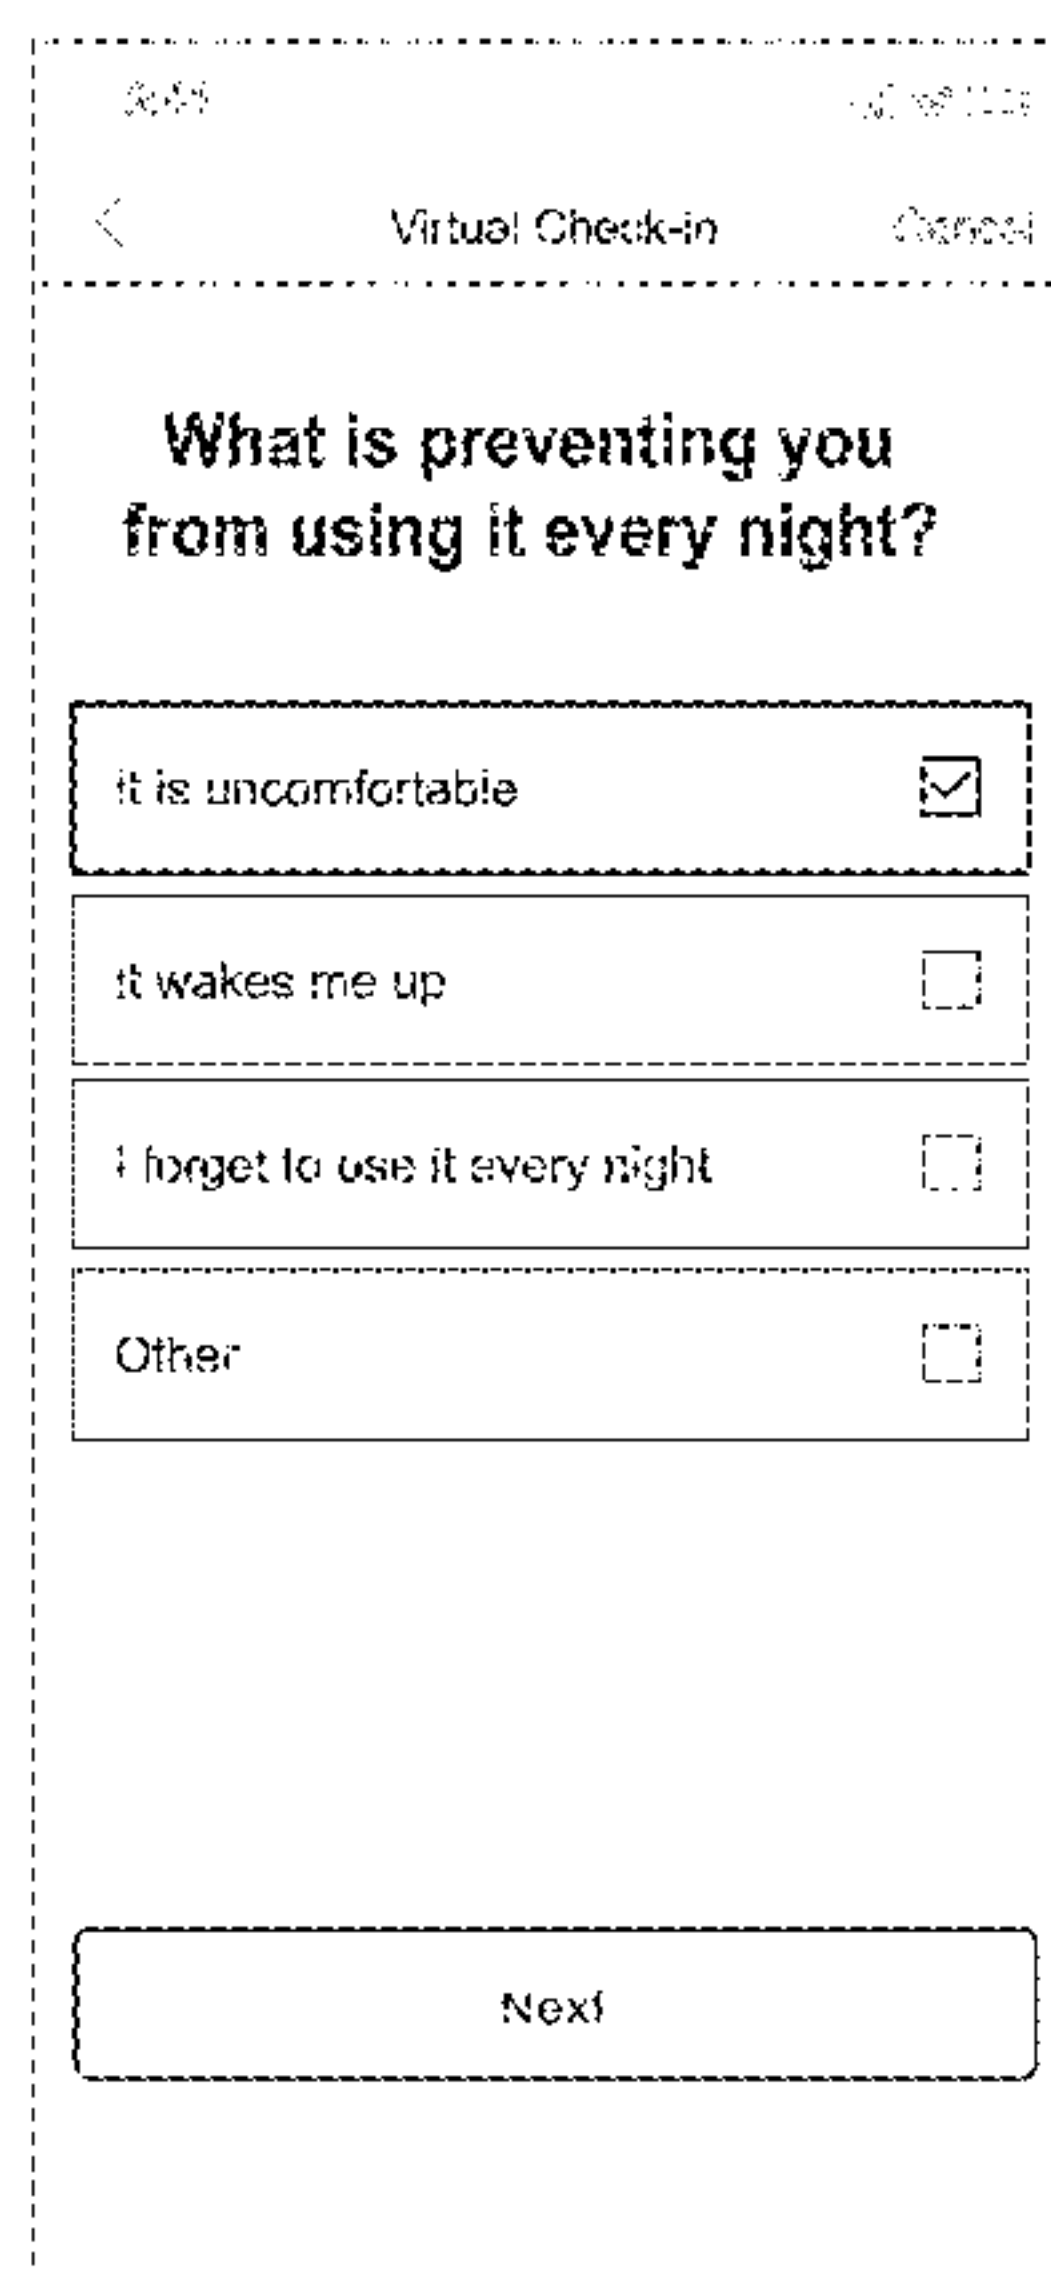

9:41 📶 🔋

< Virtual Check-in Cancel

**What is preventing you from using it every night?**

It is uncomfortable	<input checked="" type="checkbox"/>
It wakes me up	<input type="checkbox"/>
I forget to use it every night	<input type="checkbox"/>
Other	<input type="checkbox"/>

Next

FIG. 1

The image shows a mobile application interface for a "Virtual Check-in" survey. At the top, there is a status bar with the time 9:41 and icons for cellular signal, Wi-Fi, and battery. Below the status bar is a navigation bar with a back arrow on the left, the title "Virtual Check-in" in the center, and a "Cancel" button on the right. The main content area contains the question "Has your snoring improved?" in bold text. Below the question are three radio button options: "Yes" (which is selected), "No", and "Not sure". At the bottom of the screen is a "Next" button.

FIG. 2