



US00D972734S

(12) **United States Design Patent**
Farnsworth et al.

(10) **Patent No.:** **US D972,734 S**
(45) **Date of Patent:** **** Dec. 13, 2022**

(54) **MEDICAL EVALUATION GATEWAY HOUSING**

(71) Applicant: **SYMPTOMSENSE, LLC**

(72) Inventors: **Hilary Farnsworth**, New Rochelle, NY (US); **Bilal Muhammad**, West Babylon, NY (US); **Lenworth Anderson**, Bayside, NY (US); **Asheik Hussain**, Ozone Park, NY (US); **Mohammed Elbadry**, East Setauket, NY (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/744,289**

(22) Filed: **Jul. 28, 2020**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186**

(58) **Field of Classification Search**
USPC D10/46, 57, 104.1, 106.1; D14/420;
D24/107, 158, 185, 186, 217, 231;
D25/16
CPC A61B 5/01; A61B 5/02; A61B 5/05; A61B
5/015

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,818,472 A * 6/1974 Mauk G08B 13/2471
340/572.5
- 4,012,690 A * 3/1977 Heytow G01V 3/105
340/552
- D276,296 S * 11/1984 Cooper D25/16
- D297,221 S * 8/1988 Podhrasky D10/106.1
- D319,195 S * 8/1991 Belletire D10/106.1
- D330,684 S * 11/1992 Joseph D10/106.1
- D346,341 S * 4/1994 Westerberg D10/106.1
- D351,804 S * 10/1994 Kellstedt, Jr. D10/46
- D464,280 S * 10/2002 Kim D10/106.1

- D483,282 S * 12/2003 Niemi D10/106.1
- D657,058 S * 4/2012 Awad D24/158
- D667,555 S * 9/2012 Boudier G01V 5/0016
D24/158
- D718,156 S * 11/2014 Demetrescu D10/104.1
- D746,472 S * 12/2015 Morgan G16H 30/40
D24/186

(Continued)

OTHER PUBLICATIONS

Matt Hamblen, "ThermalPass fever detection device relies on multiple thermal sensors", Fierce Electronics, Jun. 3, 2020, <https://www.fierceelectronics.com/electronics/thermalpass-fever-detection-device-relies-multiple-thermal-sensors>

(Continued)

Primary Examiner — George D. Kirschbaum

Assistant Examiner — Lillian Windham

(74) *Attorney, Agent, or Firm* — Carter, DeLuca & Farrell LLP; George Likourezos


(57) **CLAIM**

The ornamental design for a medical evaluation gateway housing, as shown and described.

DESCRIPTION

FIG. 1 is a perspective right view of a medical evaluation gateway housing in accordance with the present design; FIG. 2 is a perspective left view in accordance with the present design; FIG. 3 is a front view thereof; FIG. 4 is a back view thereof; FIG. 5 is a right-side view thereof; FIG. 6 is a left-side view thereof; FIG. 7 is a top plan view thereof; and, FIG. 8 is a bottom plan view thereof. The broken lines shown in the drawings illustrate portions of the medical evaluation gateway housing that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

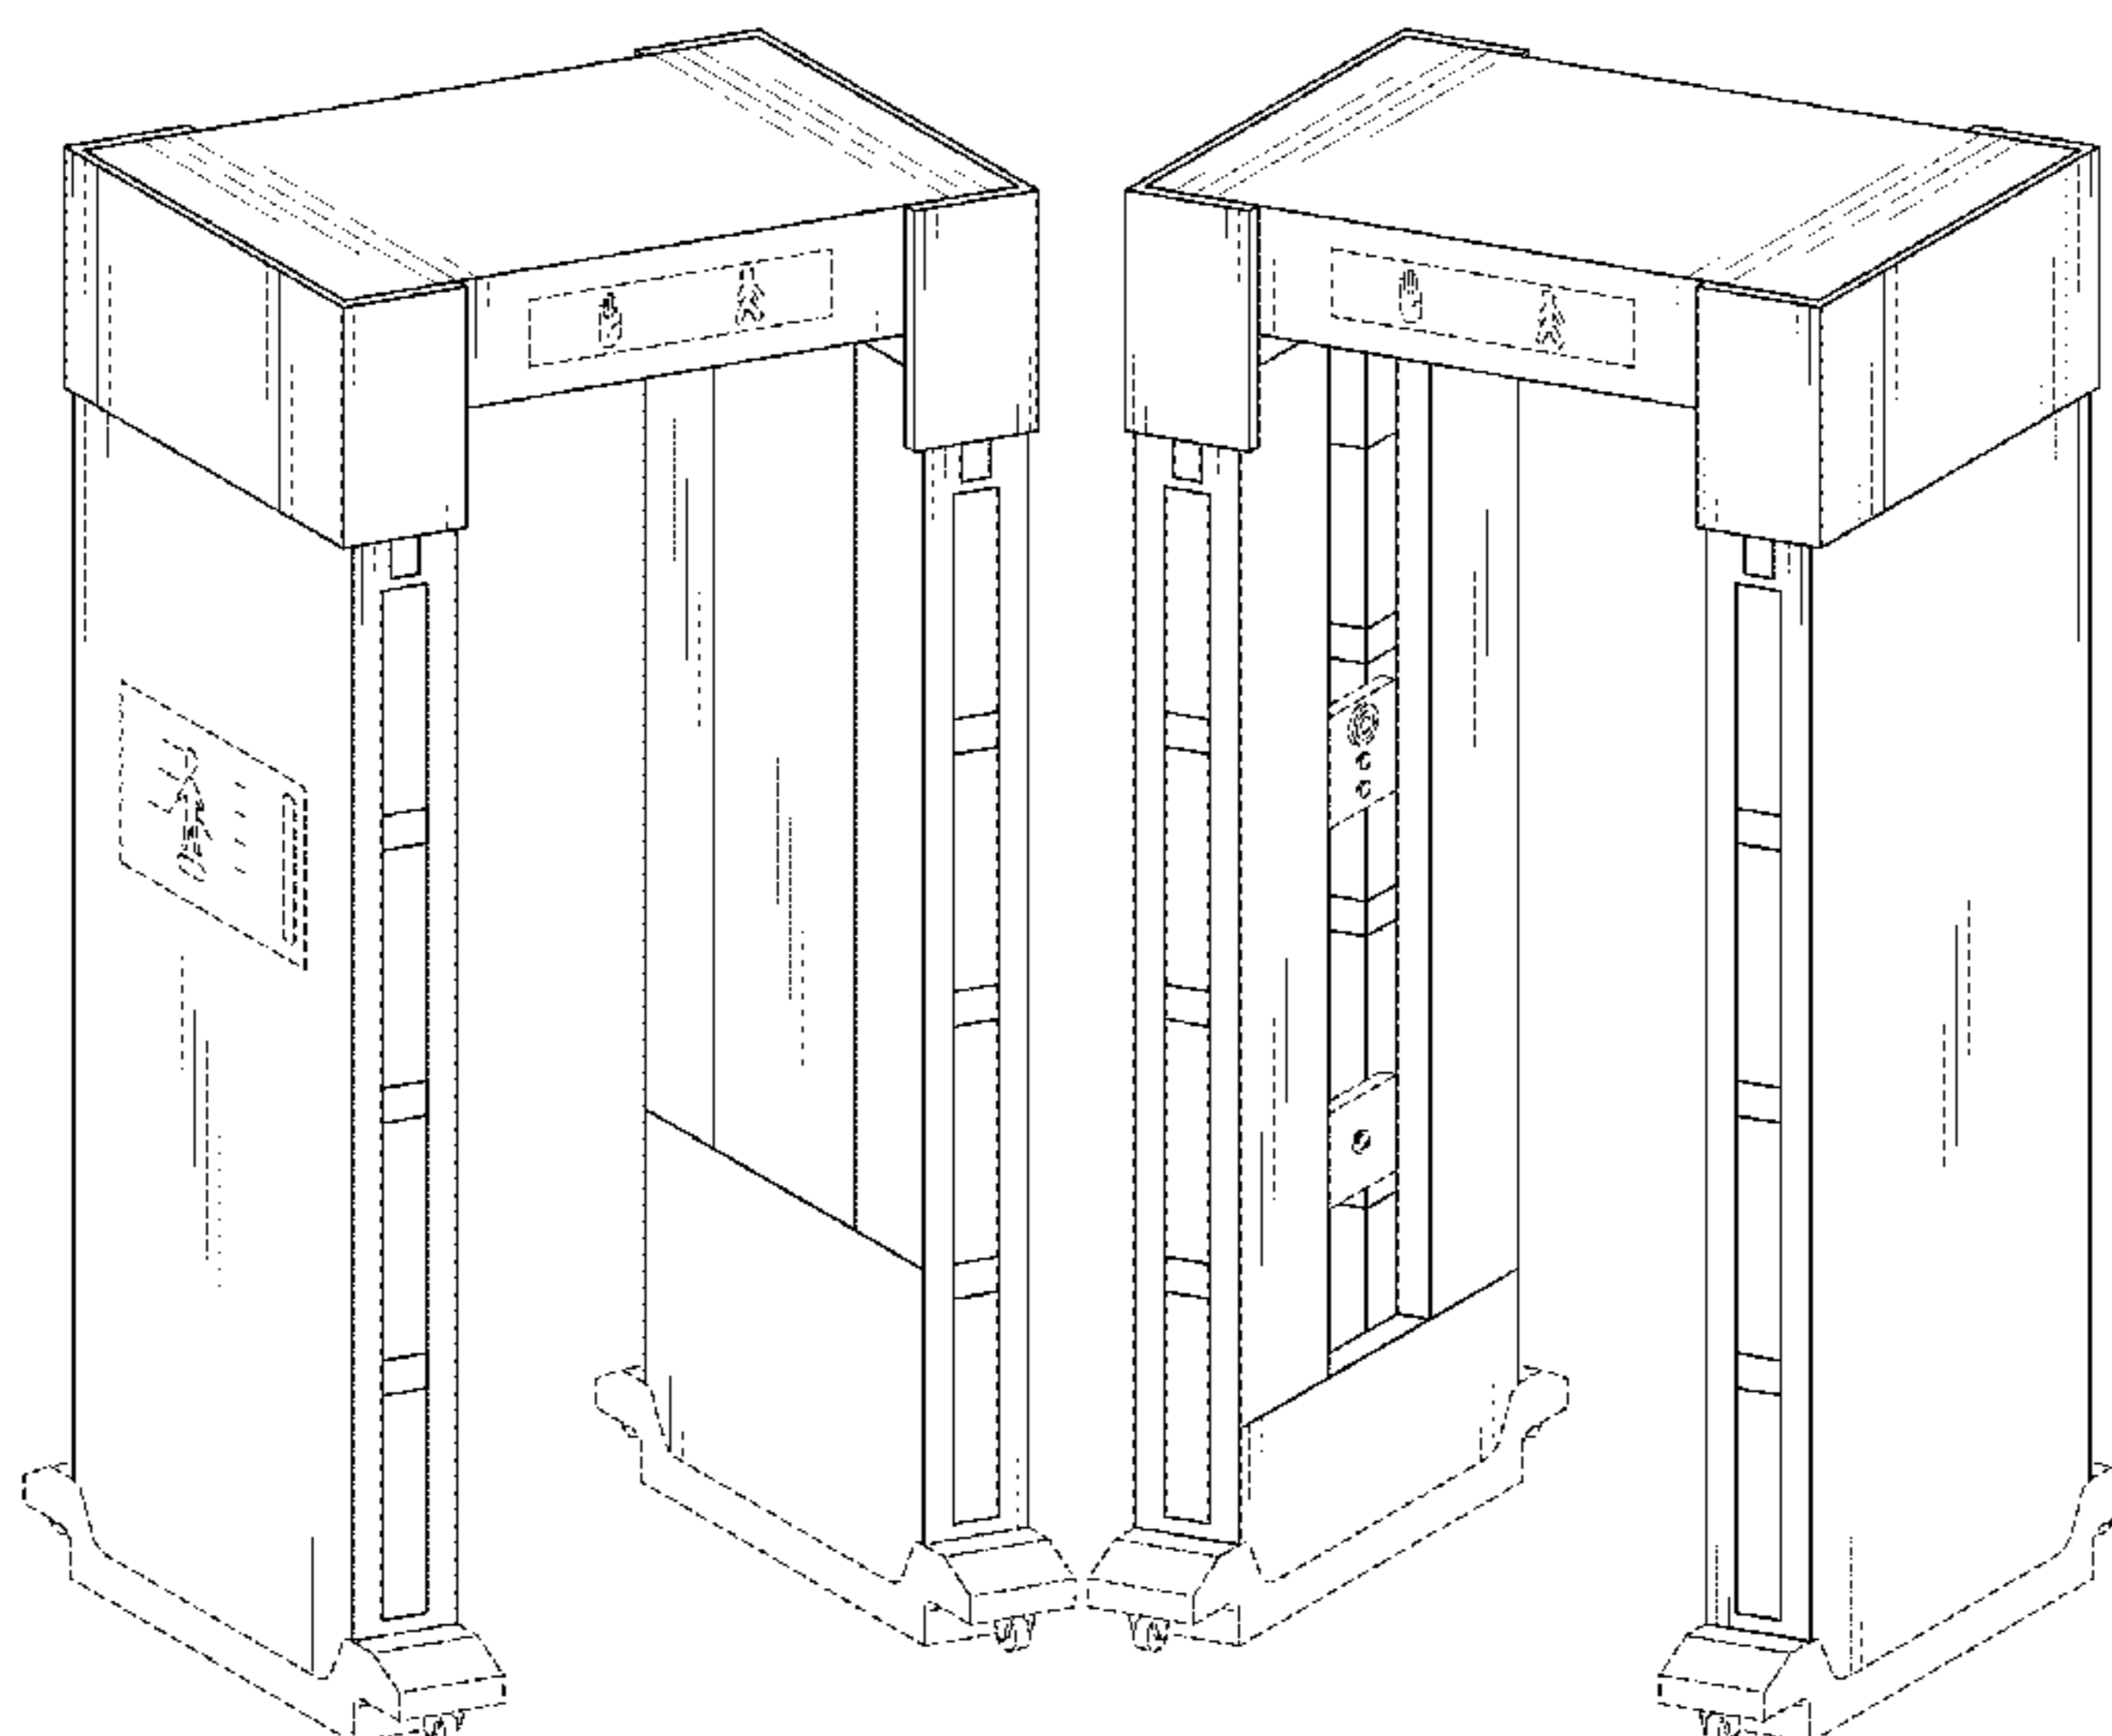

(56)

References Cited

U.S. PATENT DOCUMENTS

D823,145 S * 7/2018 Xia G01T 1/167
 D10/47
 10,473,811 B1 * 11/2019 Bairashewski G01V 5/0016
 10,976,467 B2 * 4/2021 Griffin G01V 13/00
 D937,697 S * 12/2021 Manneschi D10/106.1
 D944,994 S * 3/2022 Salillas D24/186
 D952,635 S * 5/2022 Wertel D24/158
 D952,636 S * 5/2022 Wertel A61L 2/0047
 D24/158
 D956,262 S * 6/2022 Ramos G01V 13/00
 D24/217
 2012/0128124 A1 * 5/2012 Sabol G01T 1/167
 378/22
 2012/0130145 A1 * 5/2012 Sabol G16H 30/40
 600/1
 2020/0408949 A1 * 12/2020 Griffin G01V 13/00
 2021/0393139 A1 * 12/2021 Manneschi A61B 5/01
 2022/0062453 A1 * 3/2022 Willis A61L 2/0047

OTHER PUBLICATIONS

Zorpro, "IR Body Temperature Scanner", ZORTEMP 1000, pp. 1-5, <https://zorpro.com/ir-body-temperature-scanner/>.
 Health Detector Metal Detector SymptomSense New York published on the website <https://web.archive.org/web/20200626081915/https://www.symptomsense.com/> "Early Detection, Less Infection," Jun. 26, 2020 (1 page).
 SymptomSense symptomsense Twitter published on the website <https://twitter.com/symptomsense/status/1276231271954423810/photo/2> Jun. 26, 2020 (1 page).
 20+ Facebook published on the website <https://www.facebook.com/sotertech/videos/647631889171318> Fever Elevated Heart Rate Hypoxemia Shortness of Breath Cough Congestion, Jul. 21, 2020 (1 page).
 Soter Technologies soter_tech Instagram photos and videos published on the website <https://www.instagram.com/p/CC4MocFA1bU/> Jul. 21, 2020 (1 page).
 Examination Report for Corresponding Australian Design application No. 202110355 dated Jul. 15, 2021 (6 pages).

* cited by examiner

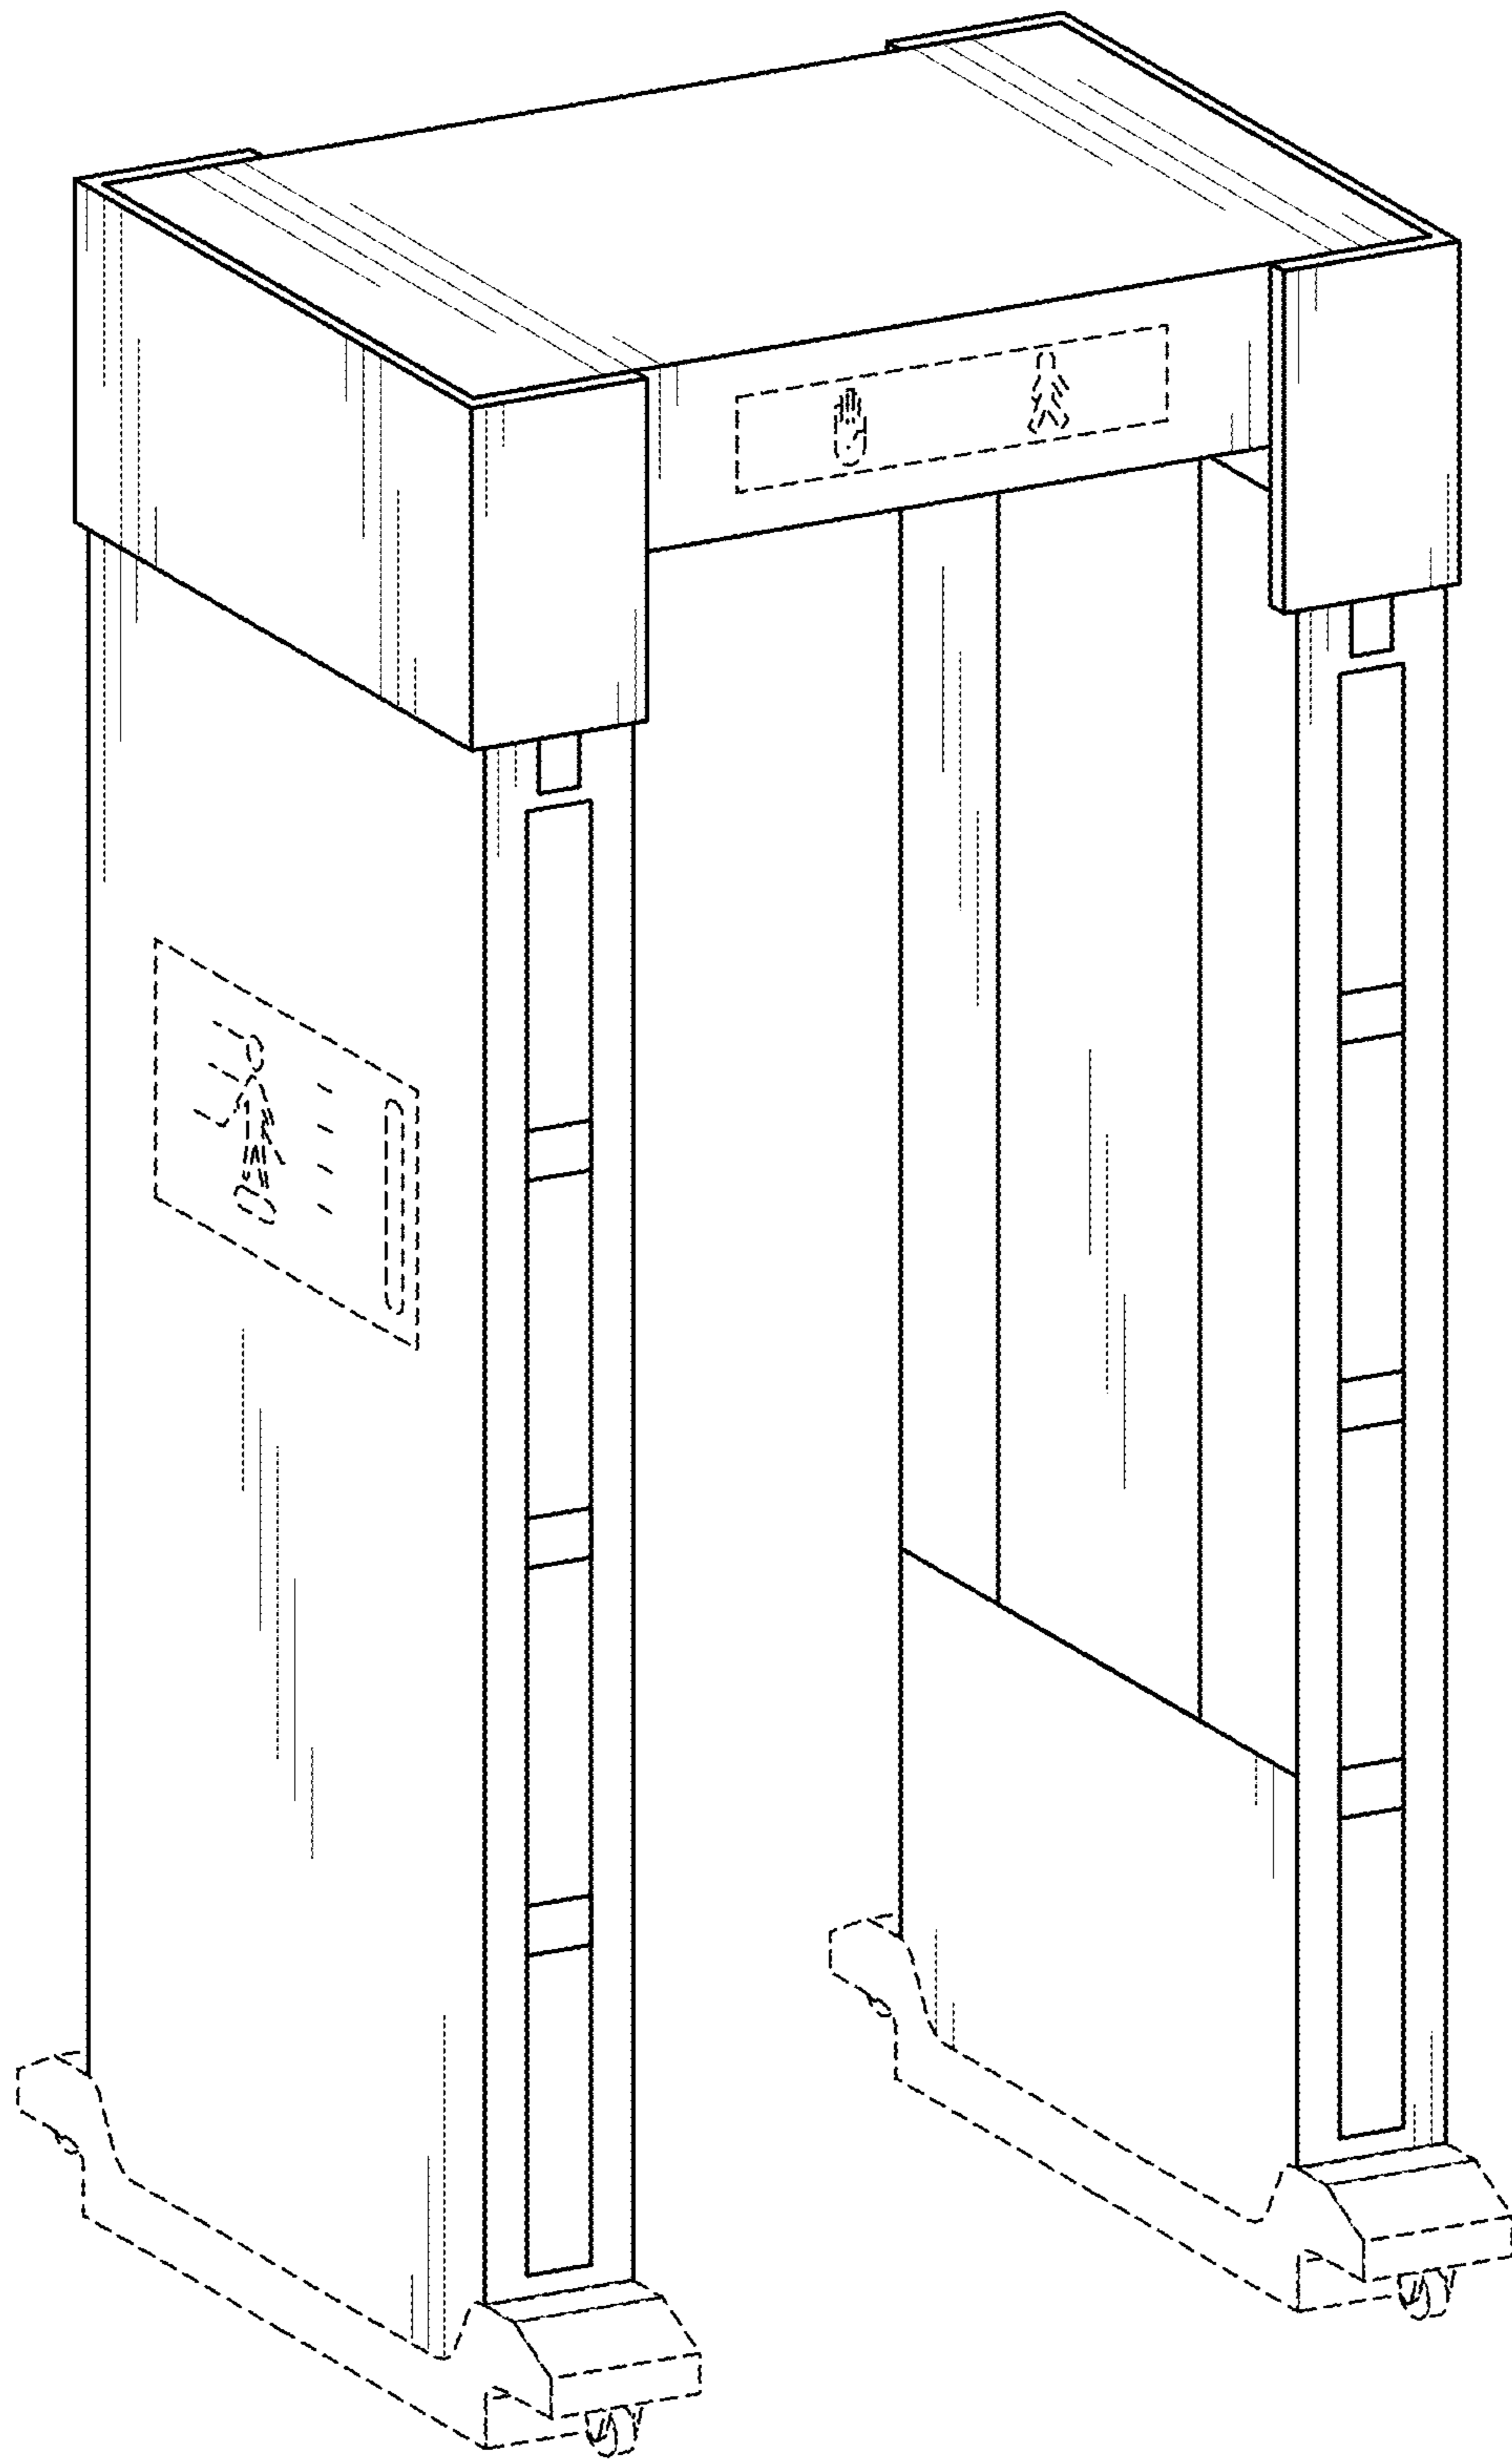


FIG. 1

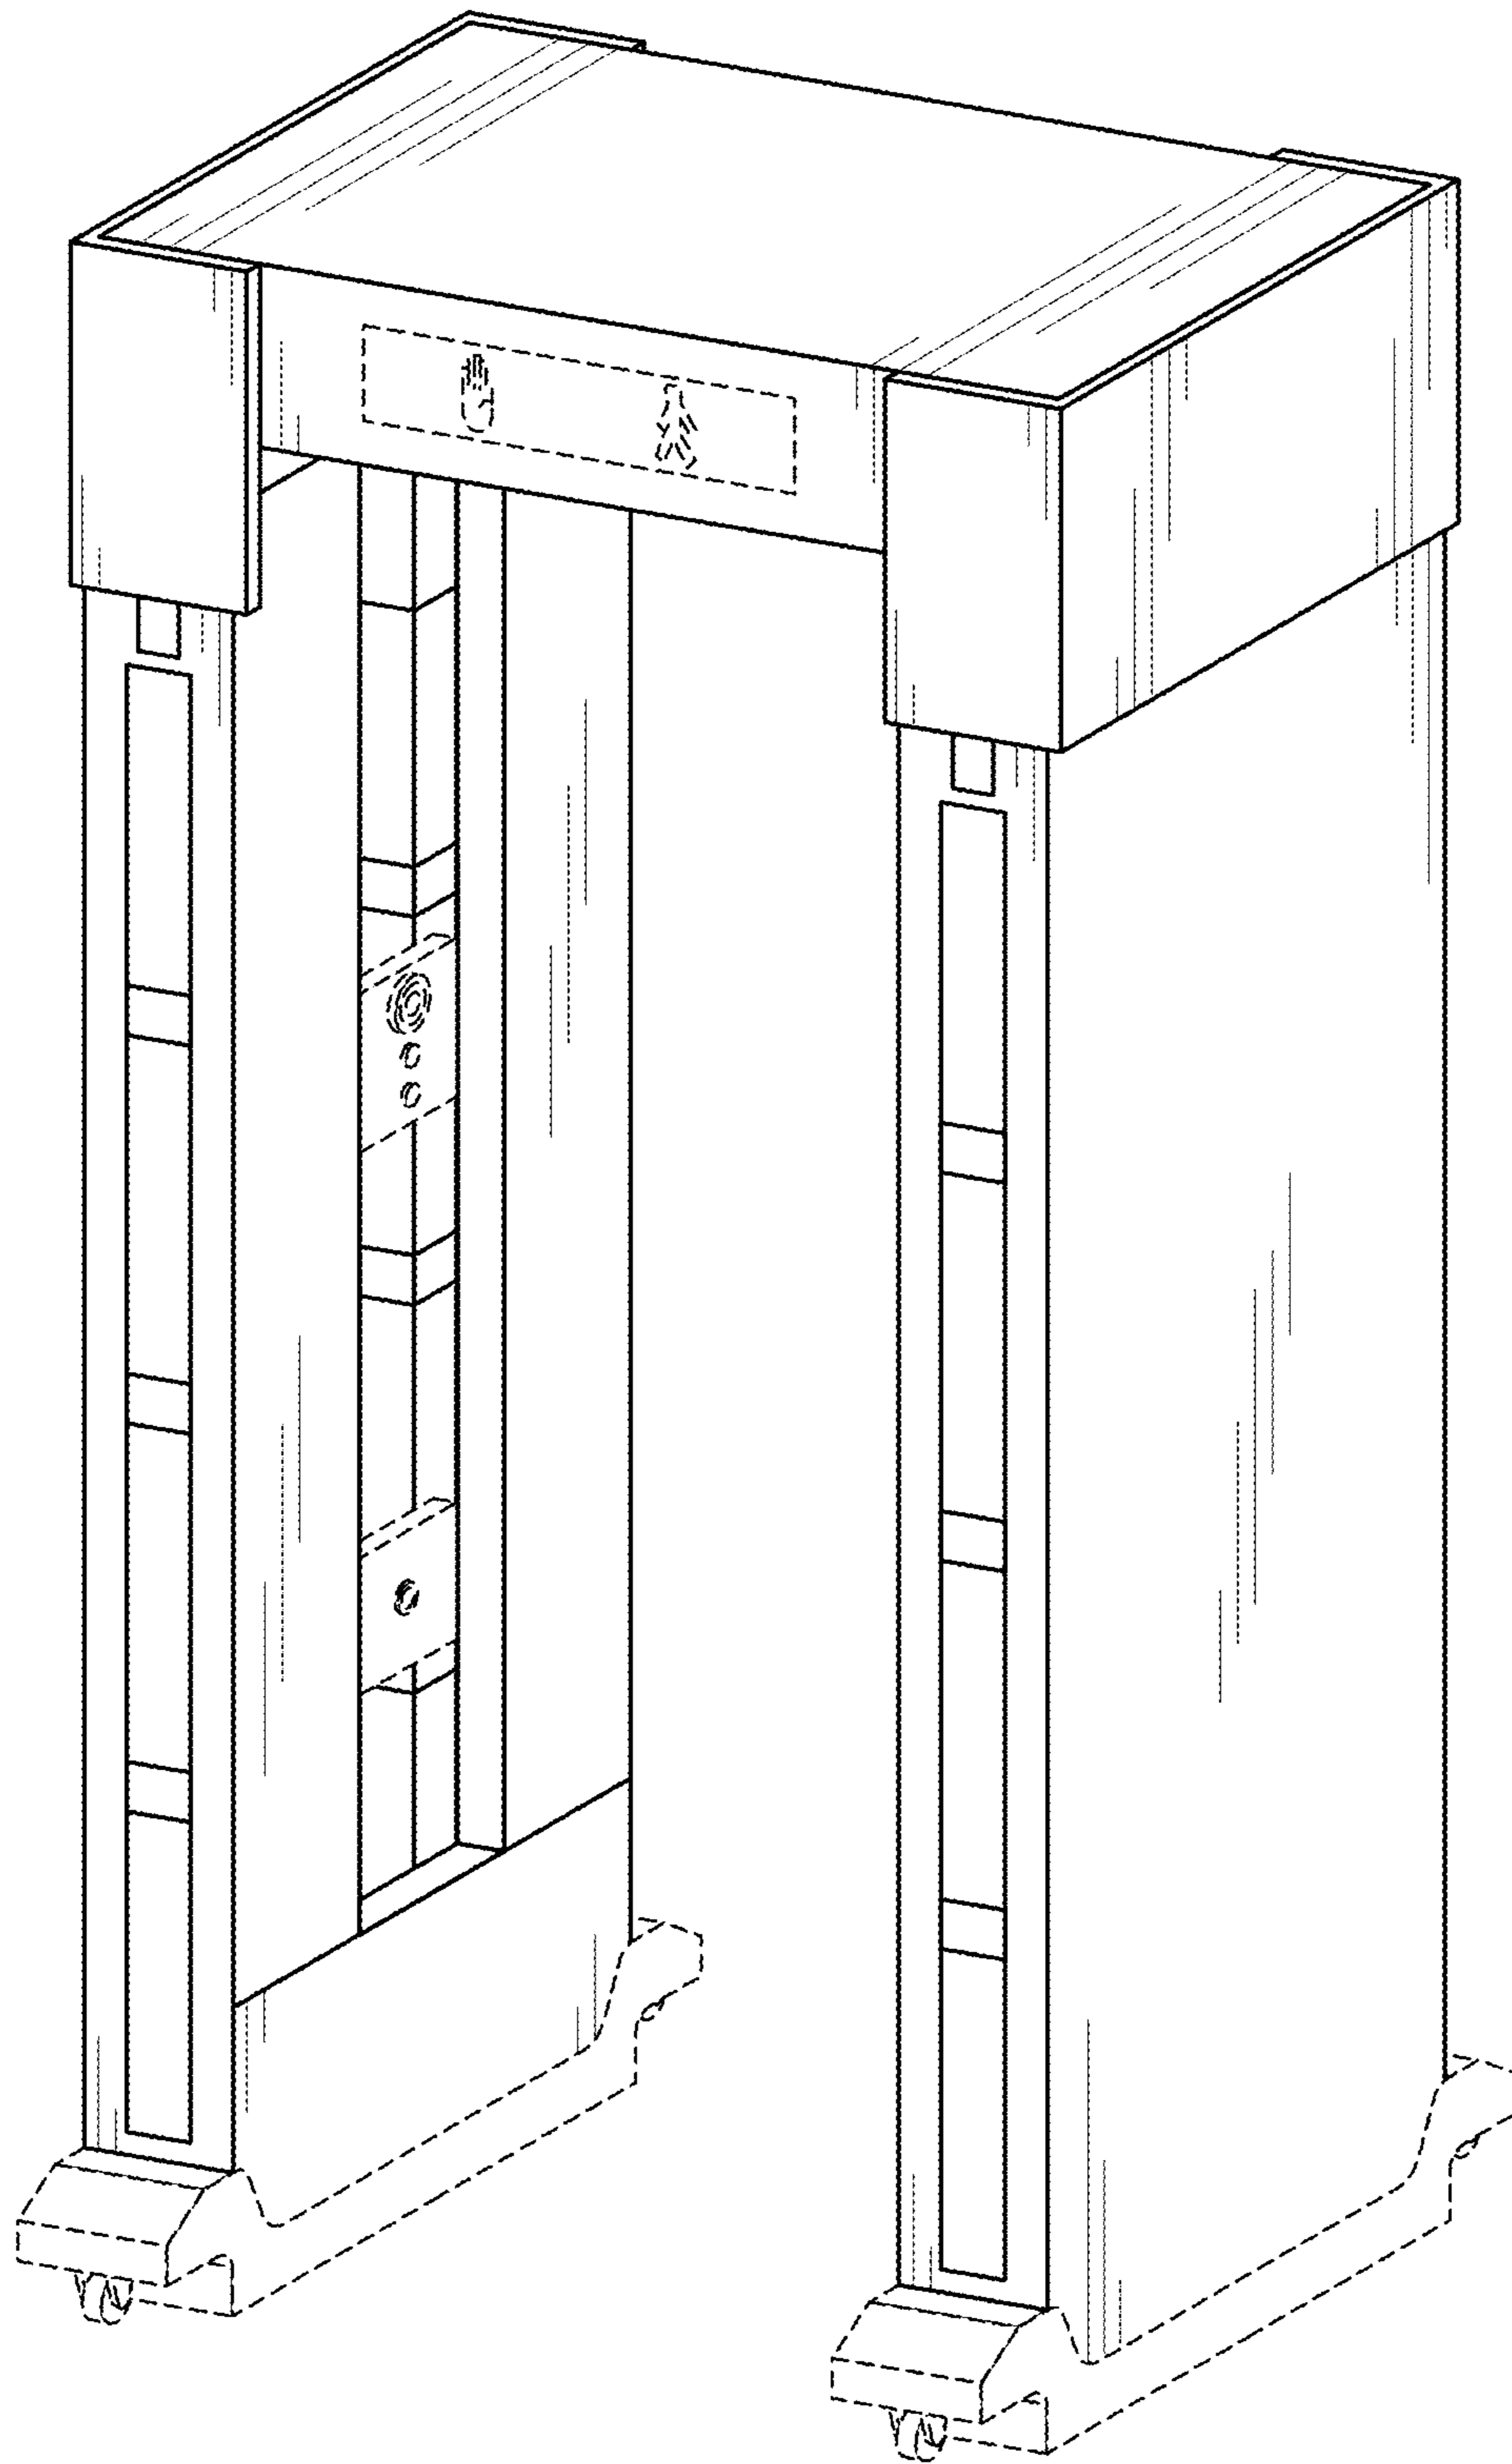


FIG. 2

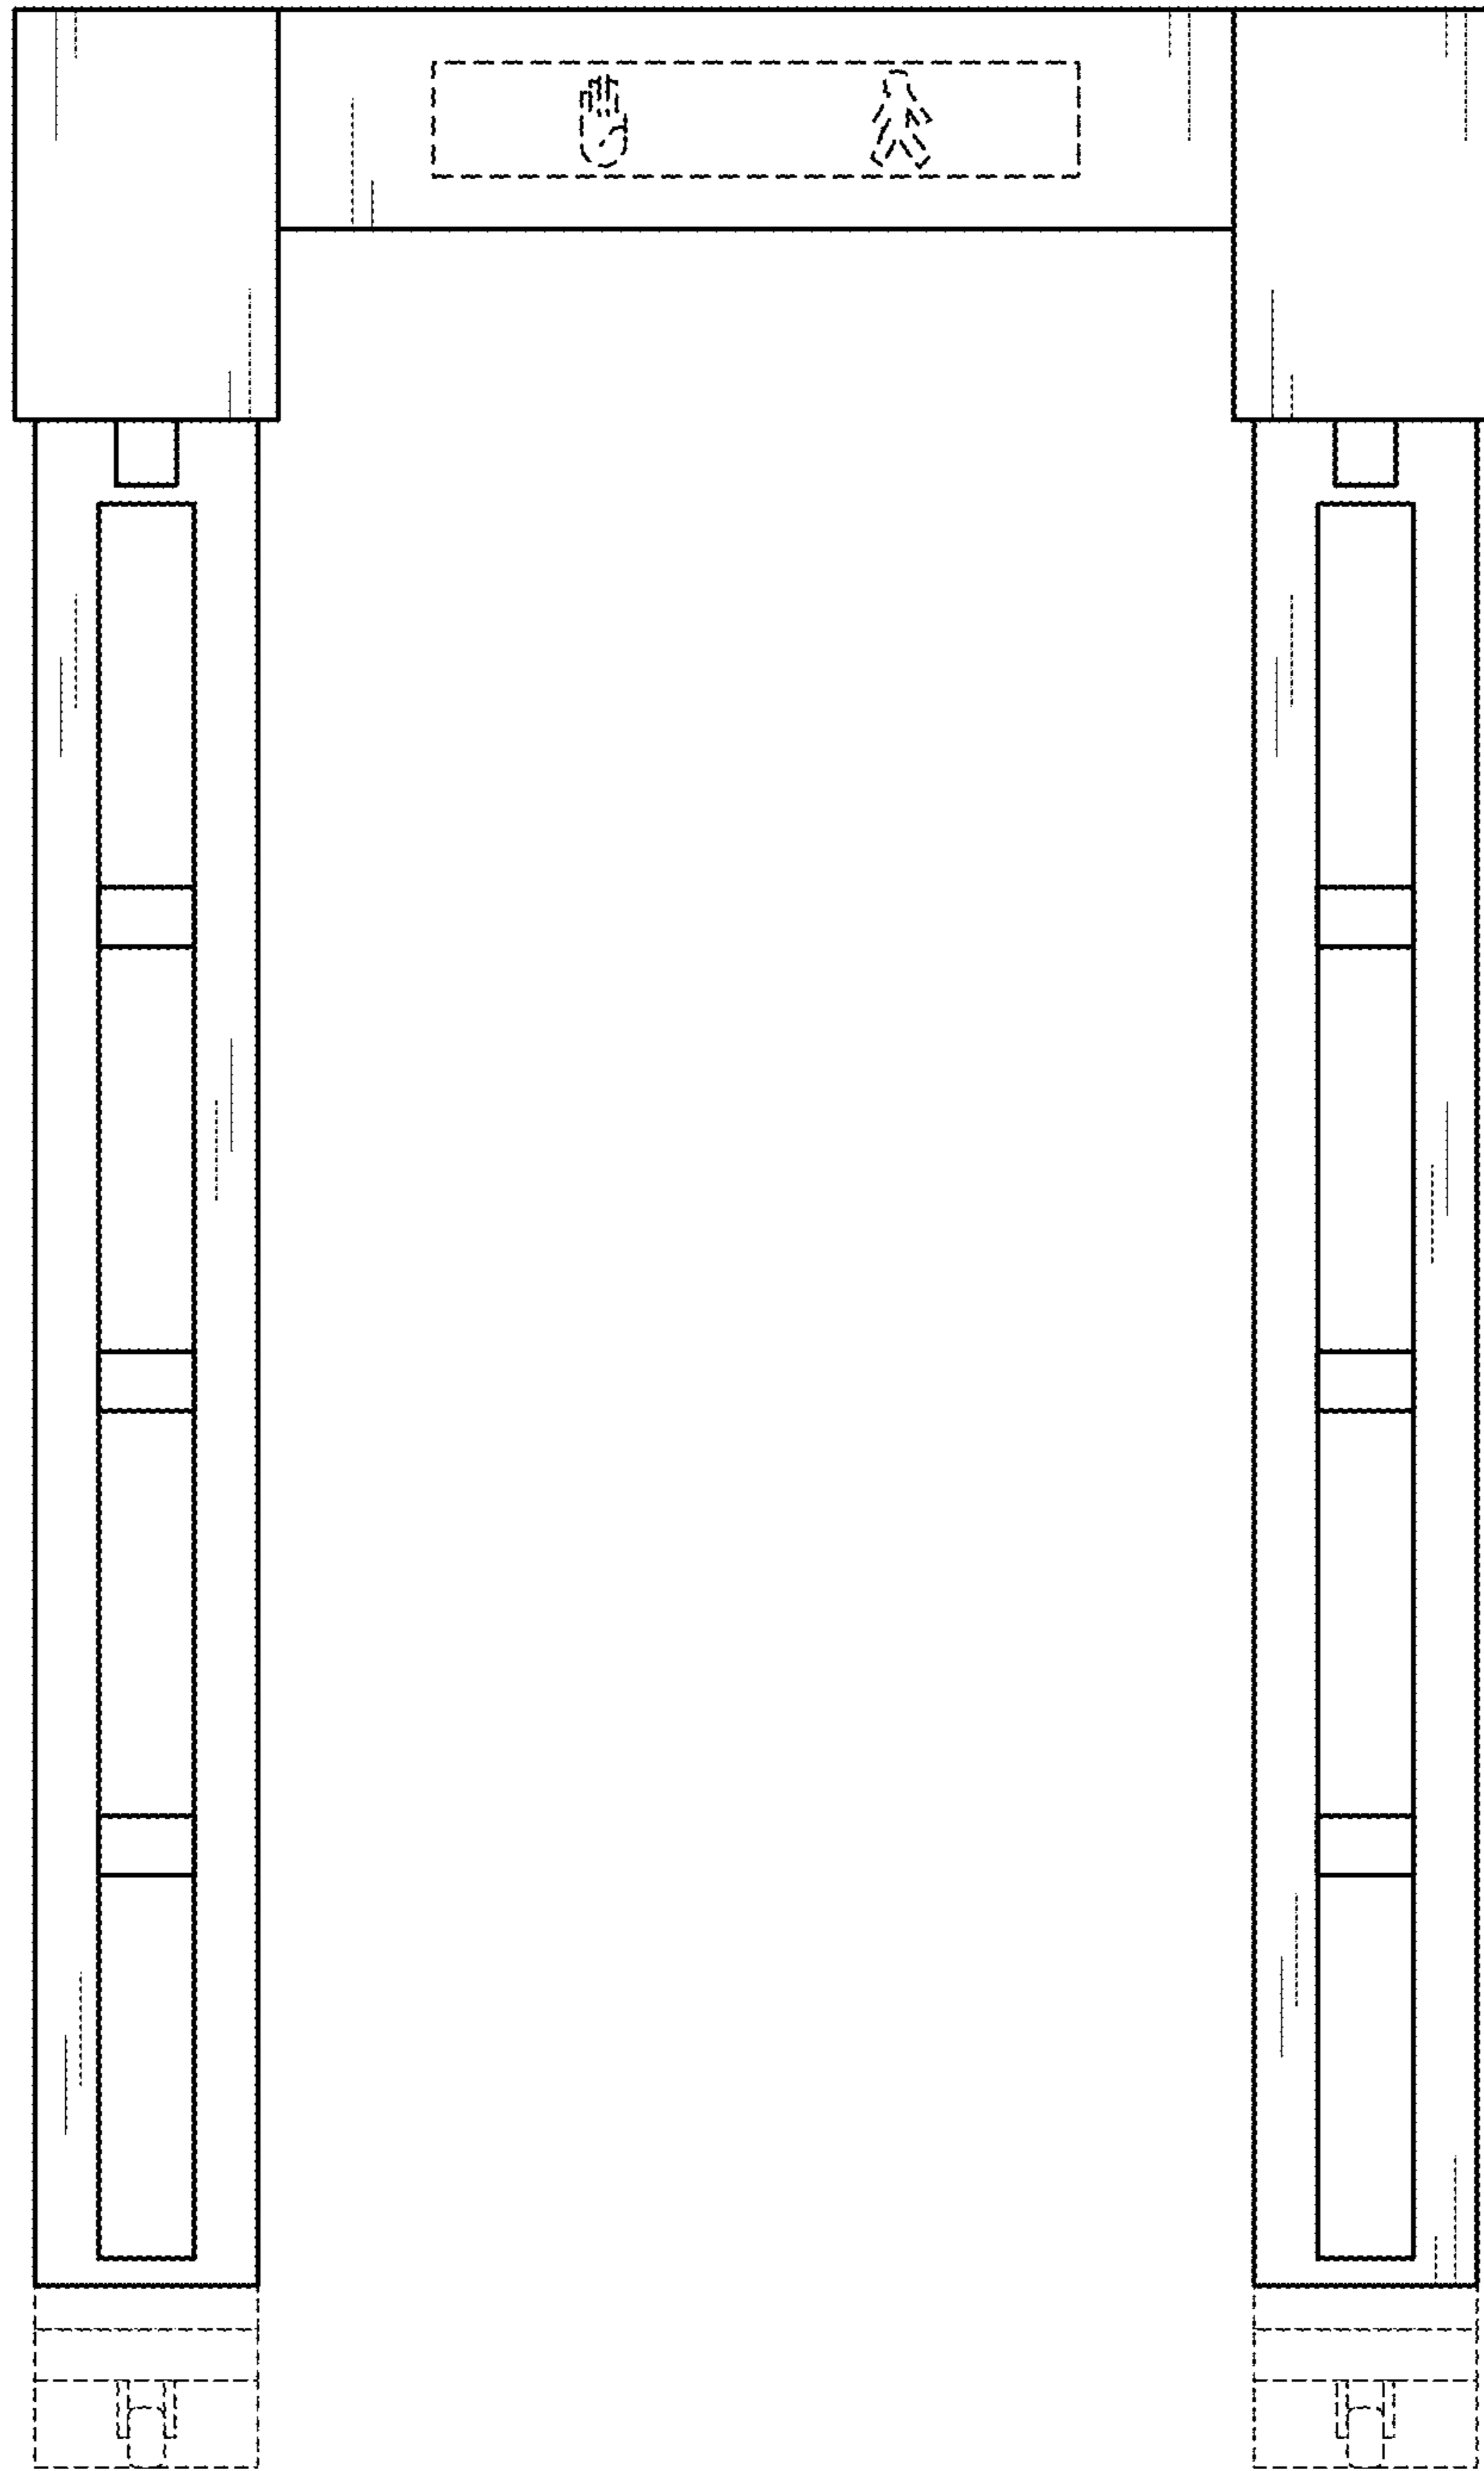


FIG. 3

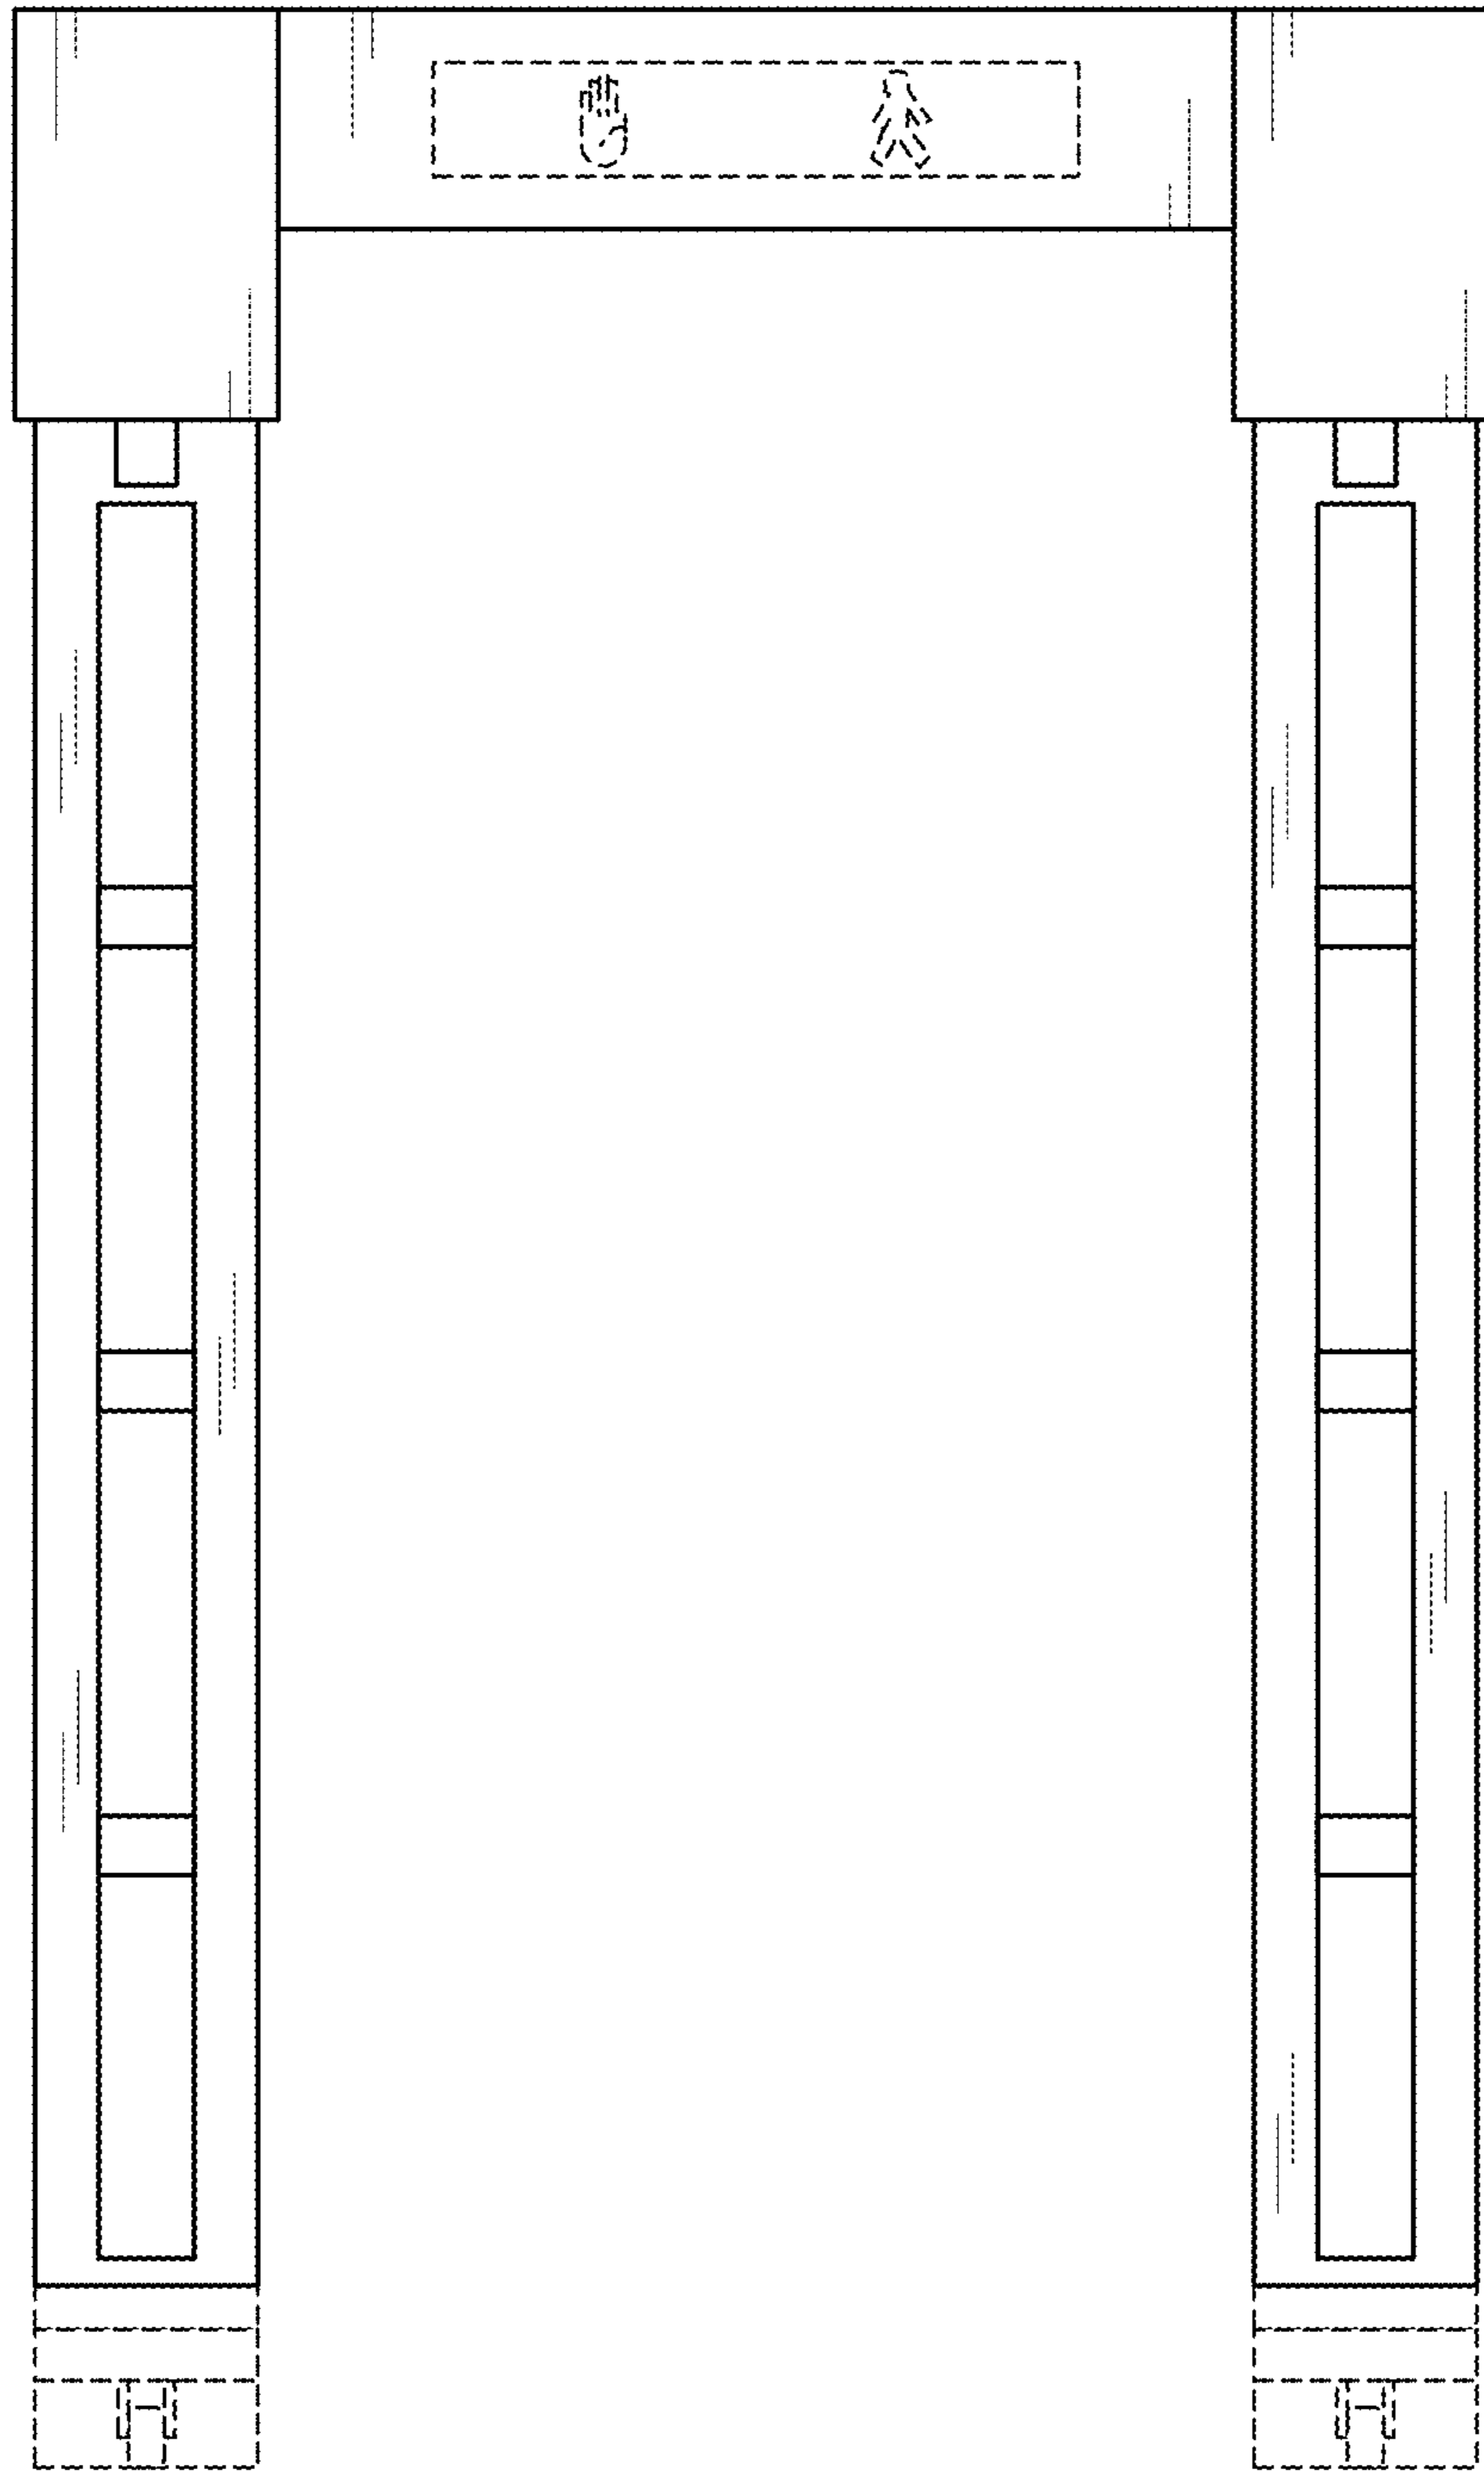


FIG. 4

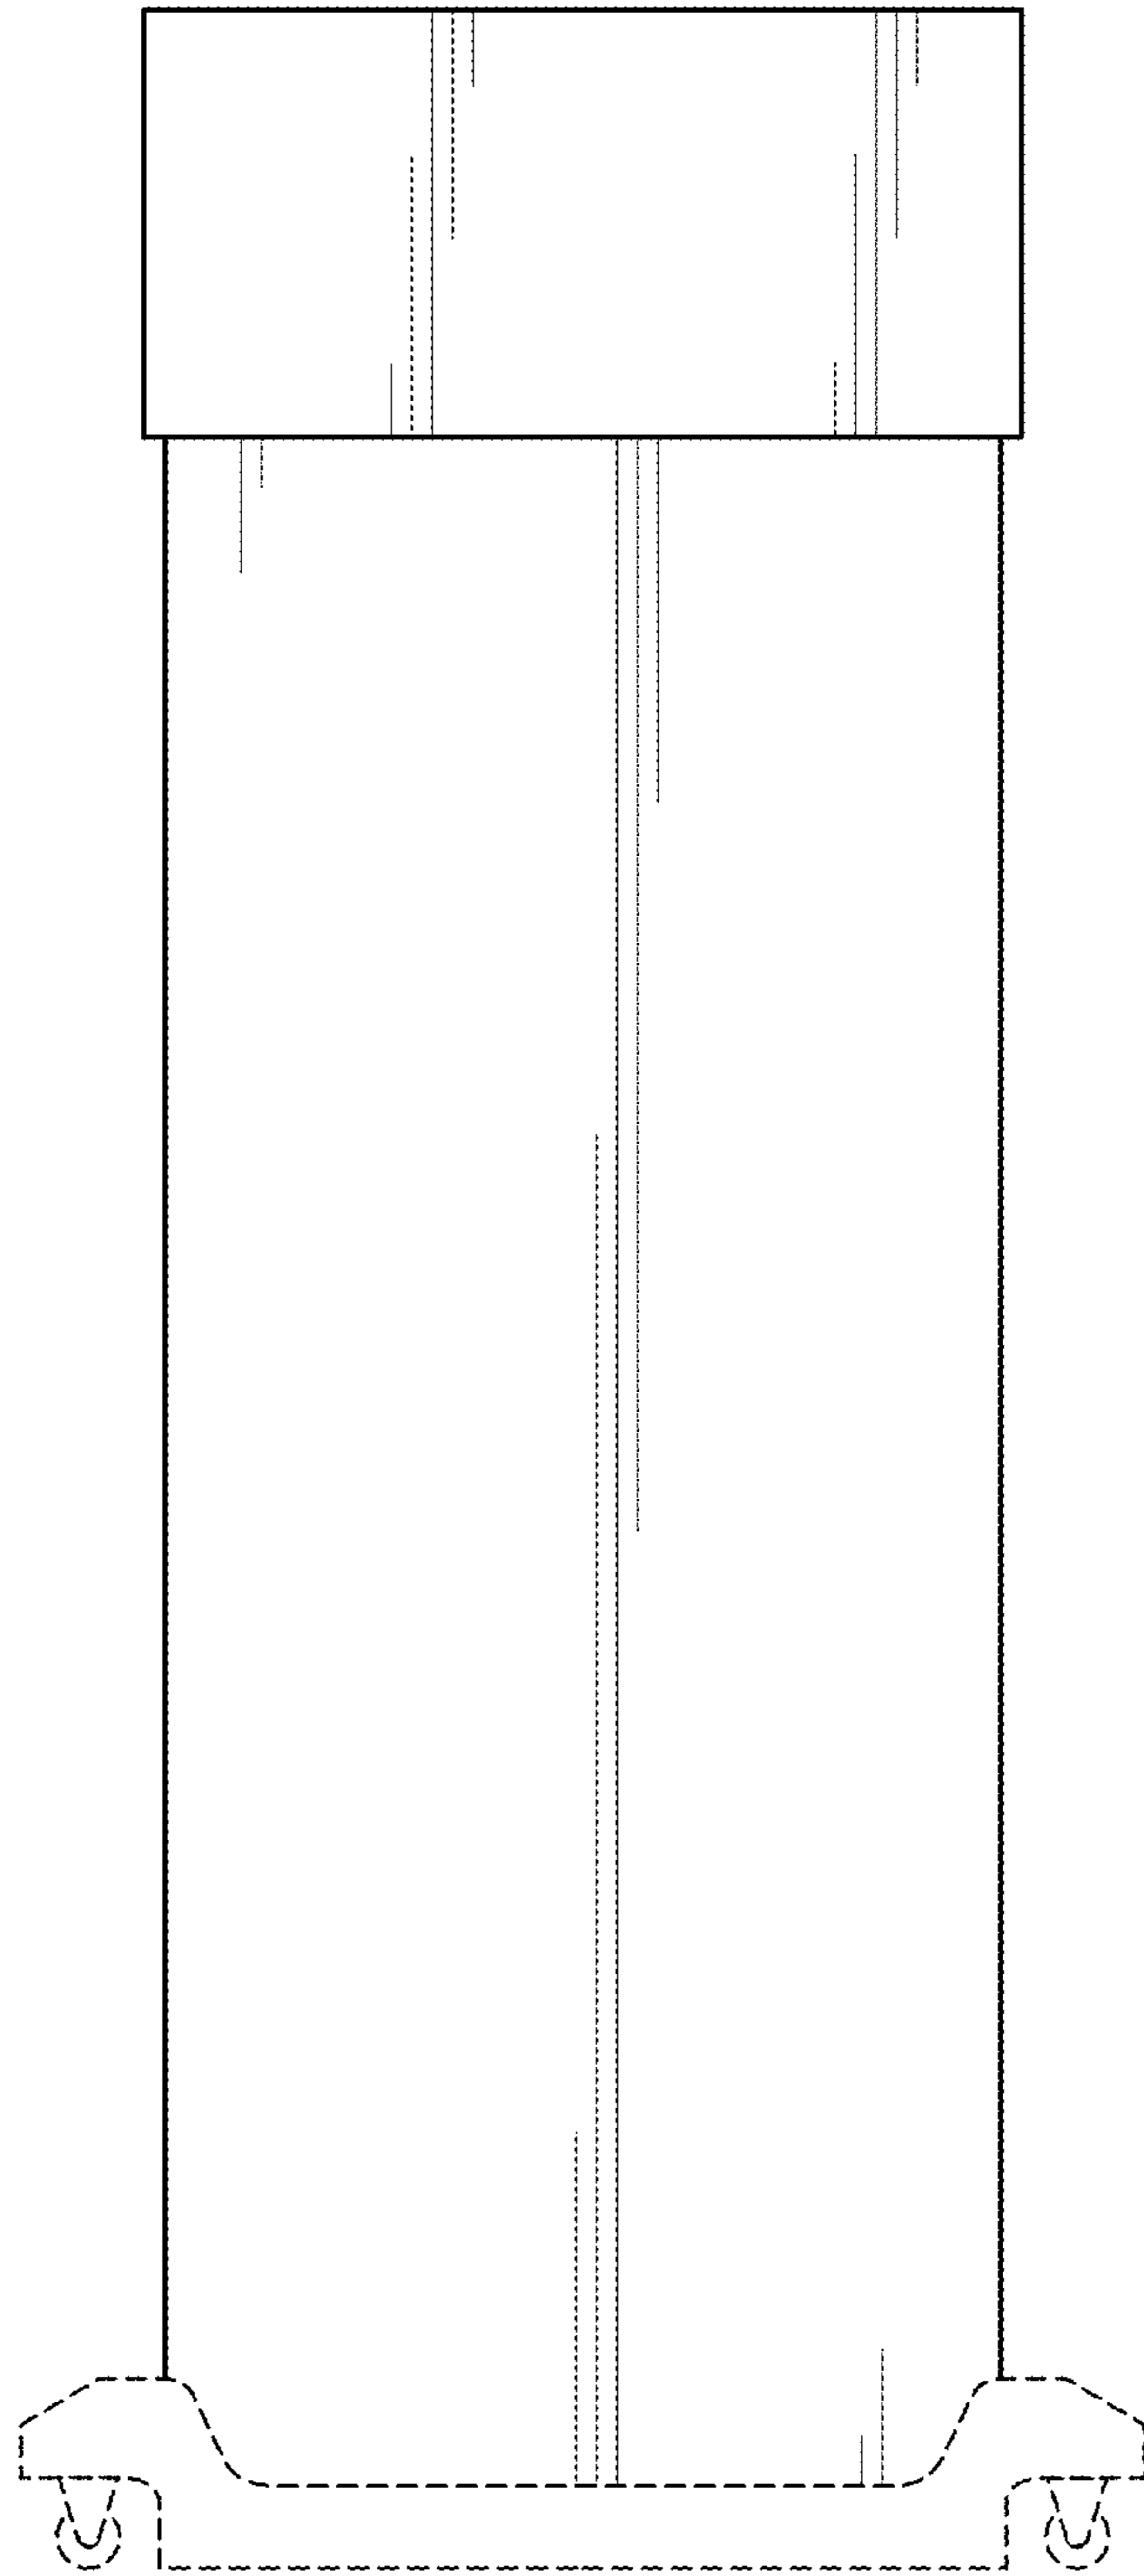


FIG. 5

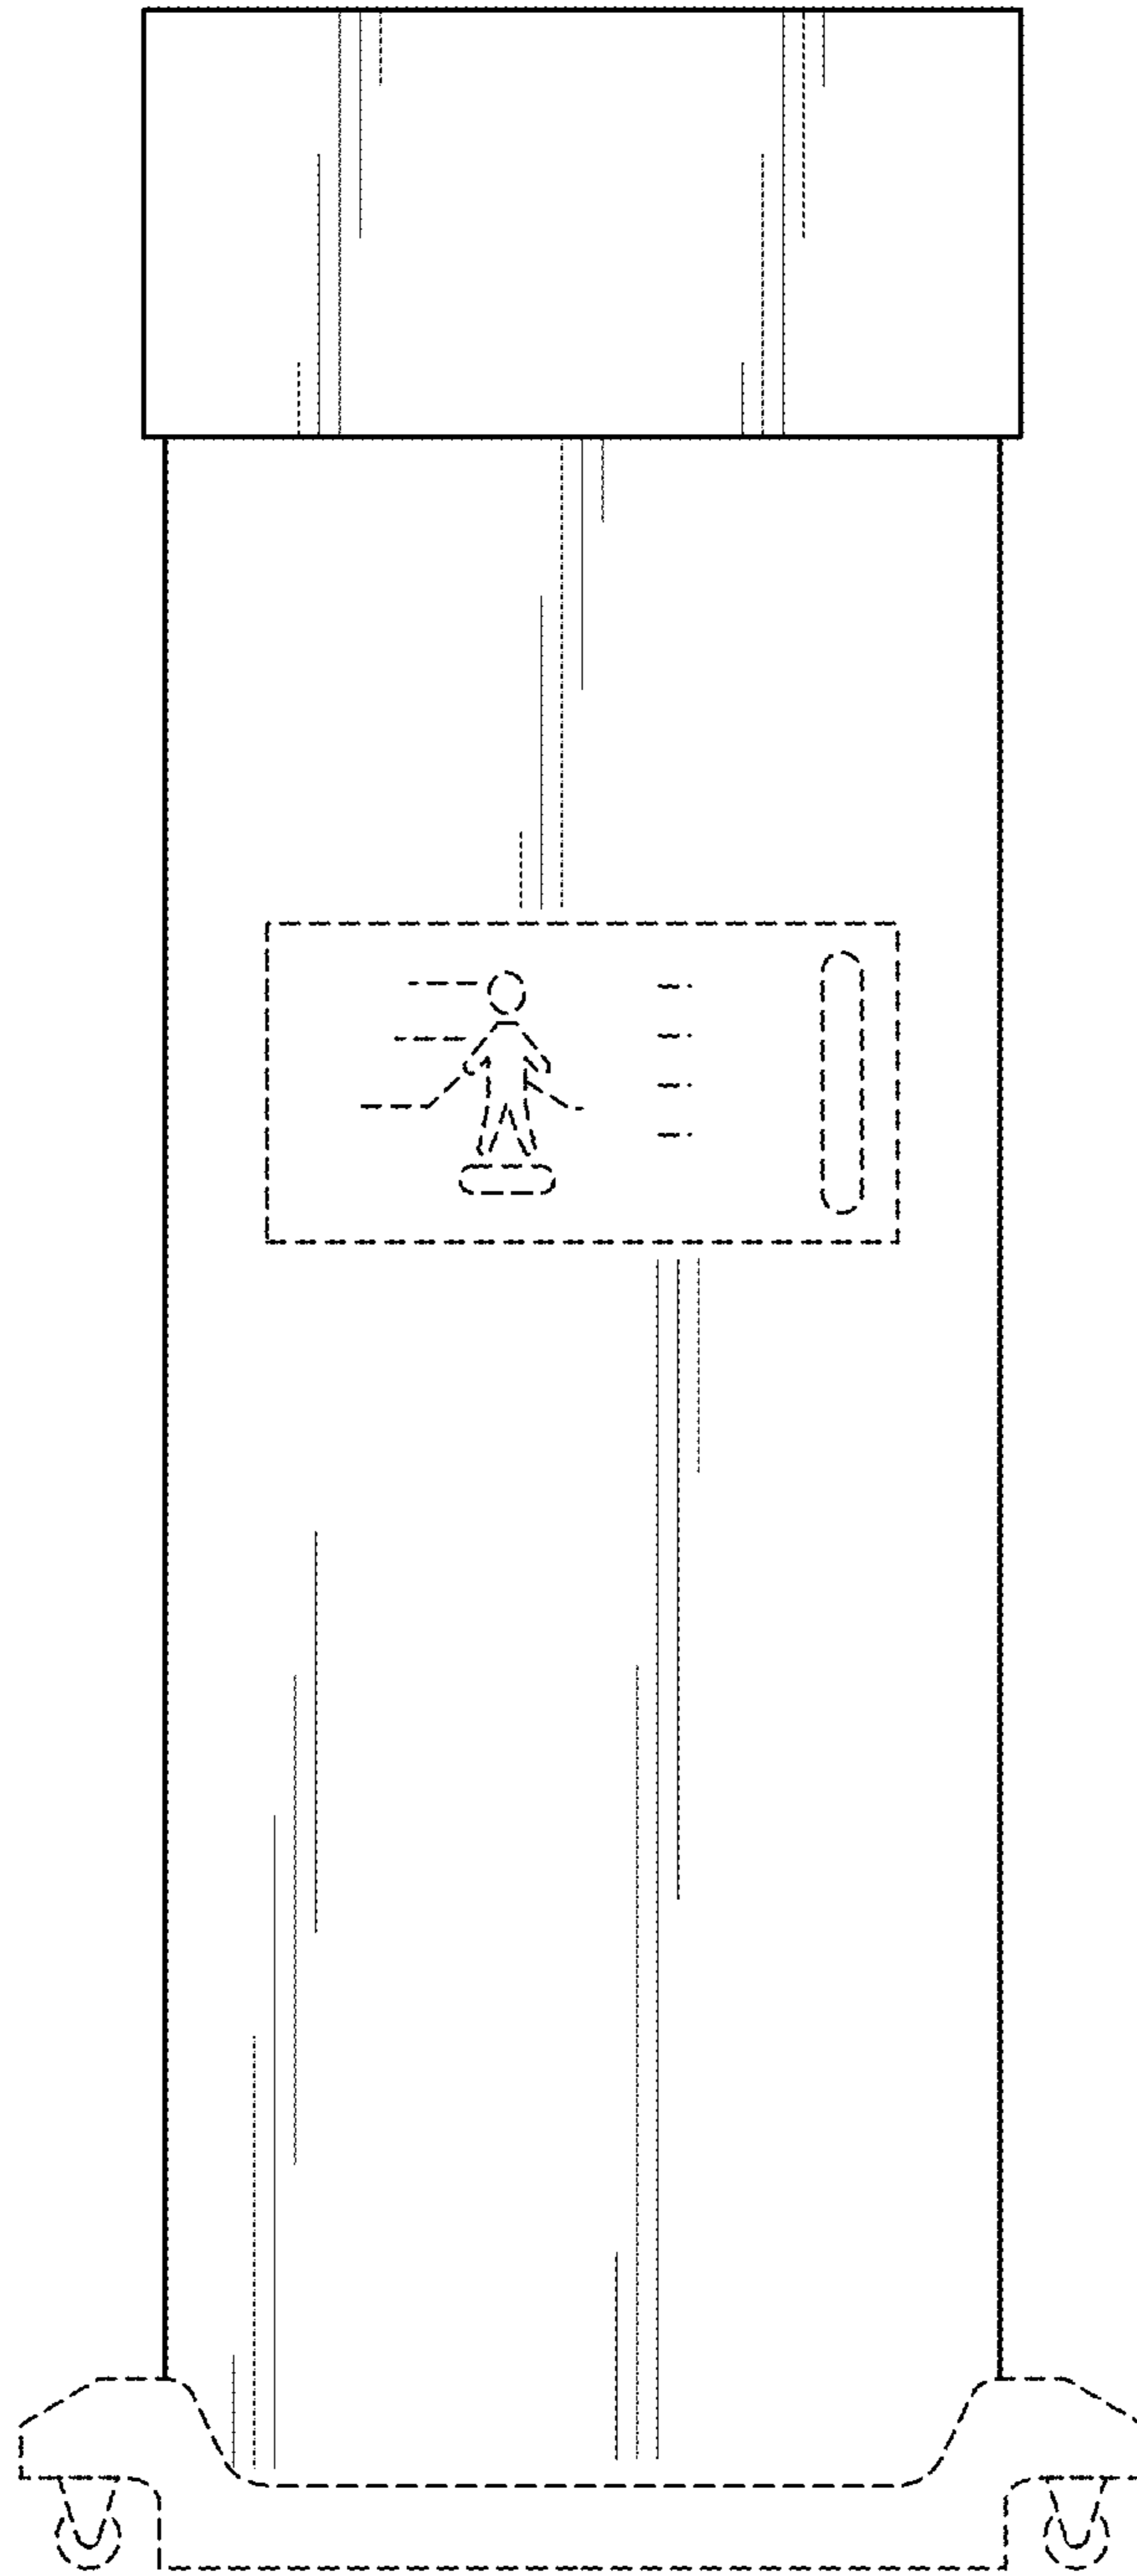


FIG. 6

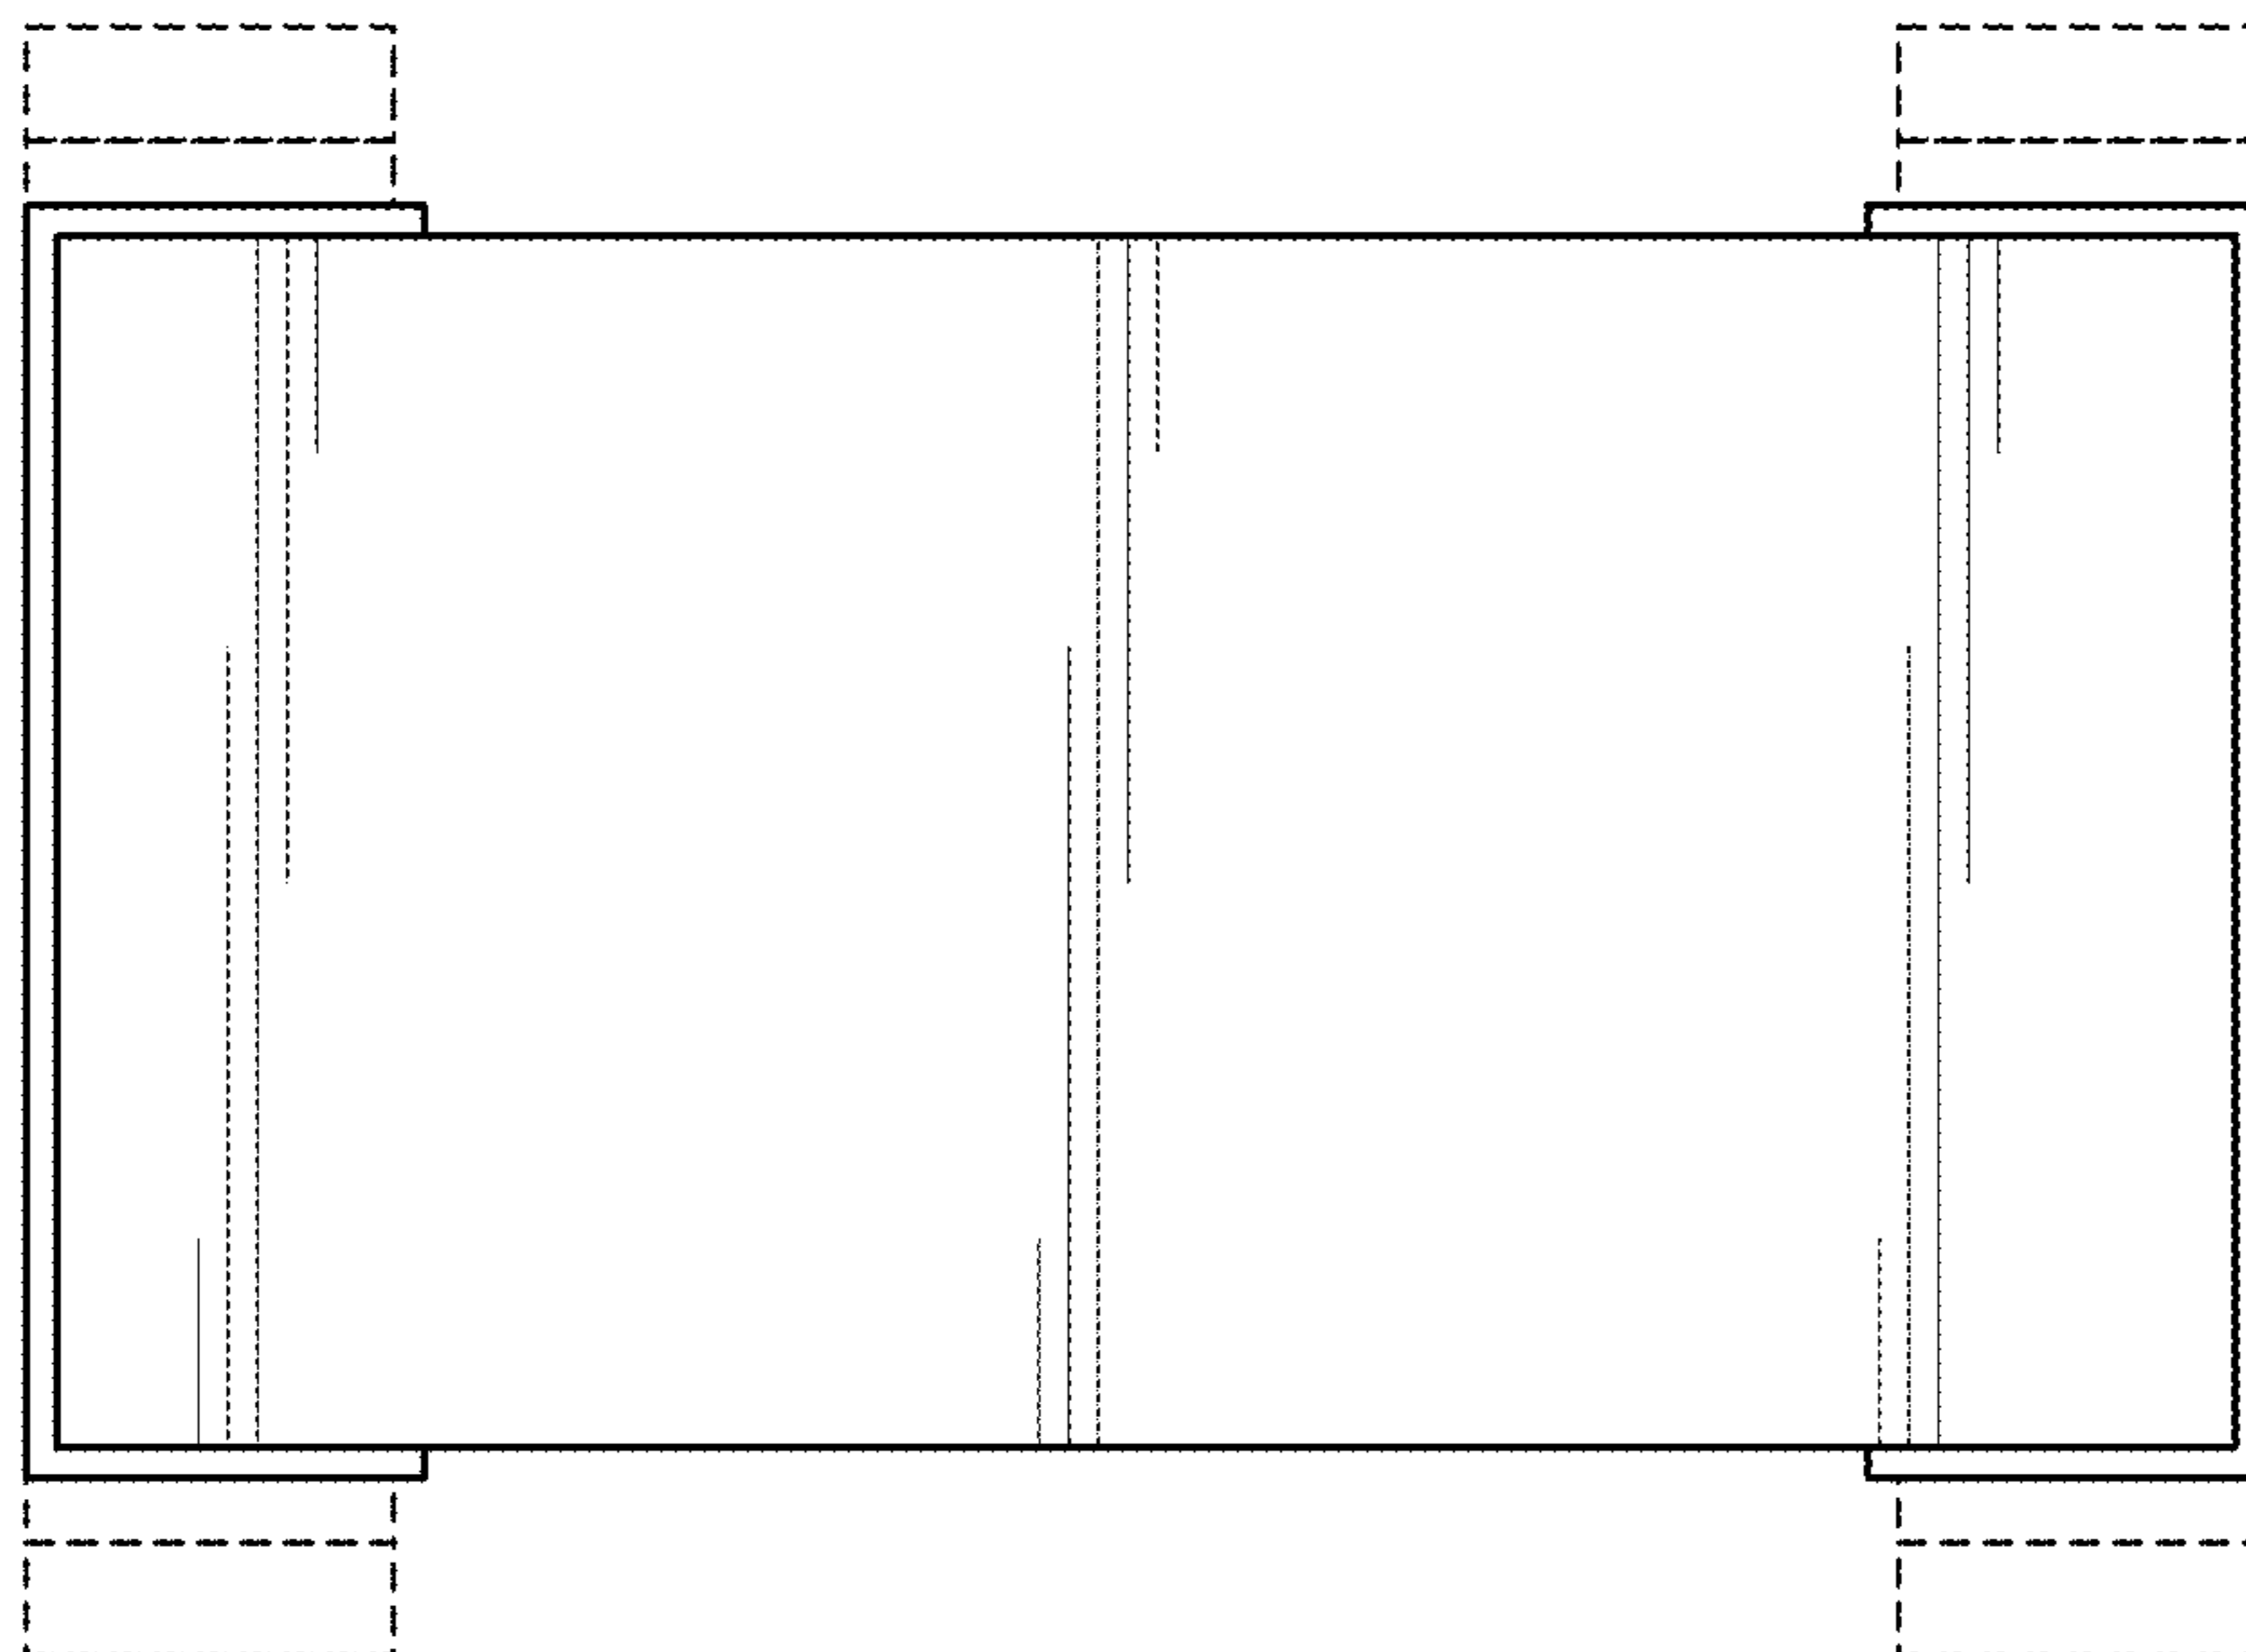


FIG. 7

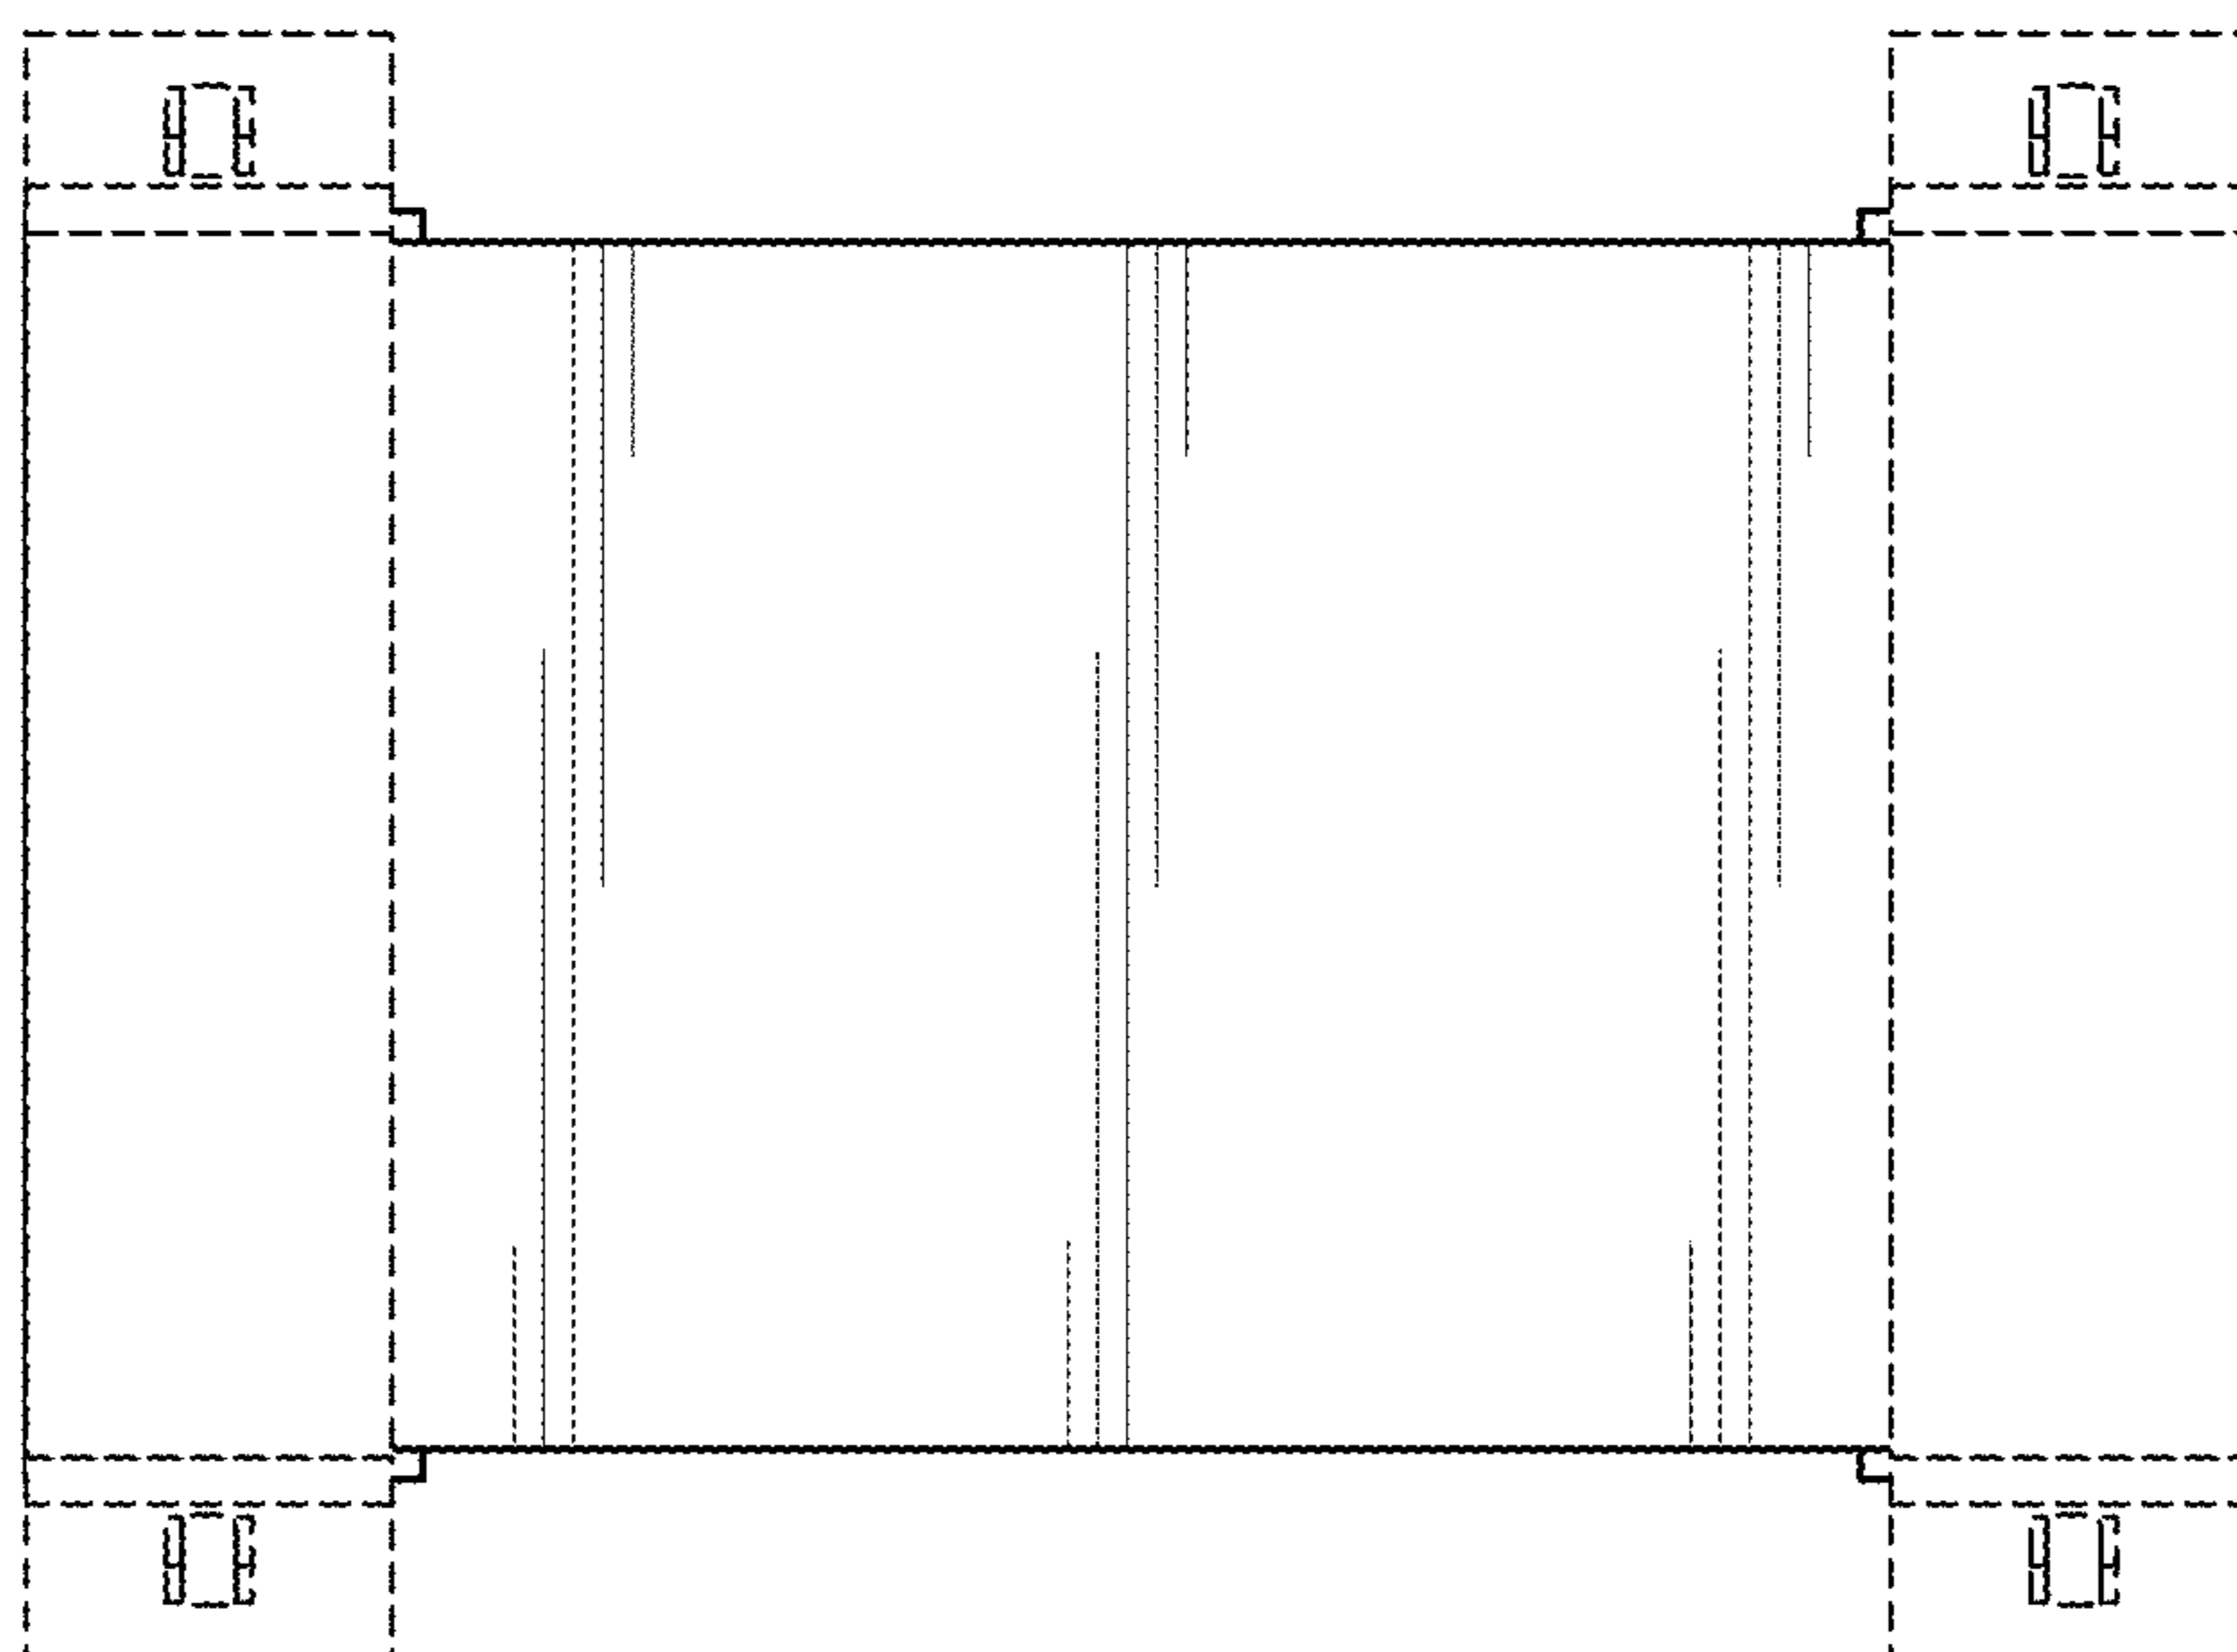


FIG. 8