



US00D973208S

(12) **United States Design Patent** (10) **Patent No.:** **US D973,208 S**  
**Amari** (45) **Date of Patent:** **\*\* \*Dec. 20, 2022**

(54) **KEYBOARD FOR A MEDICAL ULTRASONIC OBSERVATION DEVICE**

(71) Applicant: **OLYMPUS CORPORATION**, Tokyo (JP)

(72) Inventor: **Ryota Amari**, Machida (JP)

(73) Assignee: **OLYMPUS CORPORATION**, Tokyo (JP)

(\*) Notice: This patent is subject to a terminal disclaimer.

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/757,077**

(22) Filed: **Nov. 3, 2020**

(30) **Foreign Application Priority Data**

Jun. 24, 2020 (JP) ..... 2020-012631 D

(51) **LOC (13) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/186**

(58) **Field of Classification Search**  
USPC ..... D24/107, 158, 160, 185, 186, 187, 231, D24/232, 137, 138; D14/391, 392, 397, D14/455, 456, 315, 318; D18/1, 2, 7, 52, D18/53  
CPC ..... A61B 8/4405; A61B 8/4416; A61B 8/462; A61B 8/467; A61B 50/13; A61B 5/338; A61G 12/001  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D398,059 S \* 9/1998 Kwak ..... D24/160  
5,872,527 A \* 2/1999 Yanagisawa ..... A61B 1/00039  
341/22

D509,900 S \* 9/2005 Barnes ..... D24/160  
D604,845 S \* 11/2009 Hibi ..... D24/138  
D666,159 S \* 8/2012 Adenau ..... D13/164  
D719,260 S \* 12/2014 Shimobayashi ..... D24/138  
D789,532 S \* 6/2017 Tanaka ..... D24/138  
D936,842 S \* 11/2021 Wu ..... D24/186  
D940,882 S \* 1/2022 Nally ..... D24/186  
D950,571 S \* 5/2022 Amari ..... D14/455  
2011/0152685 A1 \* 6/2011 Misono ..... A61B 8/467  
600/443  
2019/0290245 A1 \* 9/2019 Yoshimura ..... A61B 8/4427  
2019/0336105 A1 \* 11/2019 Yoshimura ..... A61B 8/469

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Scully, Scott, Murphy & Presser, P.C.

(57) **CLAIM**

The ornamental design for a keyboard for a medical ultrasonic observation device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a keyboard for a medical ultrasonic observation device showing my new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left-side elevational view thereof, the right-side elevational view being a mirror image thereof;

FIG. 5 is a top plan view thereof;

FIG. 6 is a bottom plan view thereof; and,

FIG. 7 is an enlarged view of area "7" identified by the dot-dash chain broken line in FIG. 2.

The broken lines illustrate portions of the keyboard for a medical ultrasonic observation device that form no part of the claimed design. The dot-dash chain broken line in FIG. 2 identifies area "7" of the keyboard for a medical ultrasonic observation device that is shown in enlarged view in FIG. 7 and forms no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

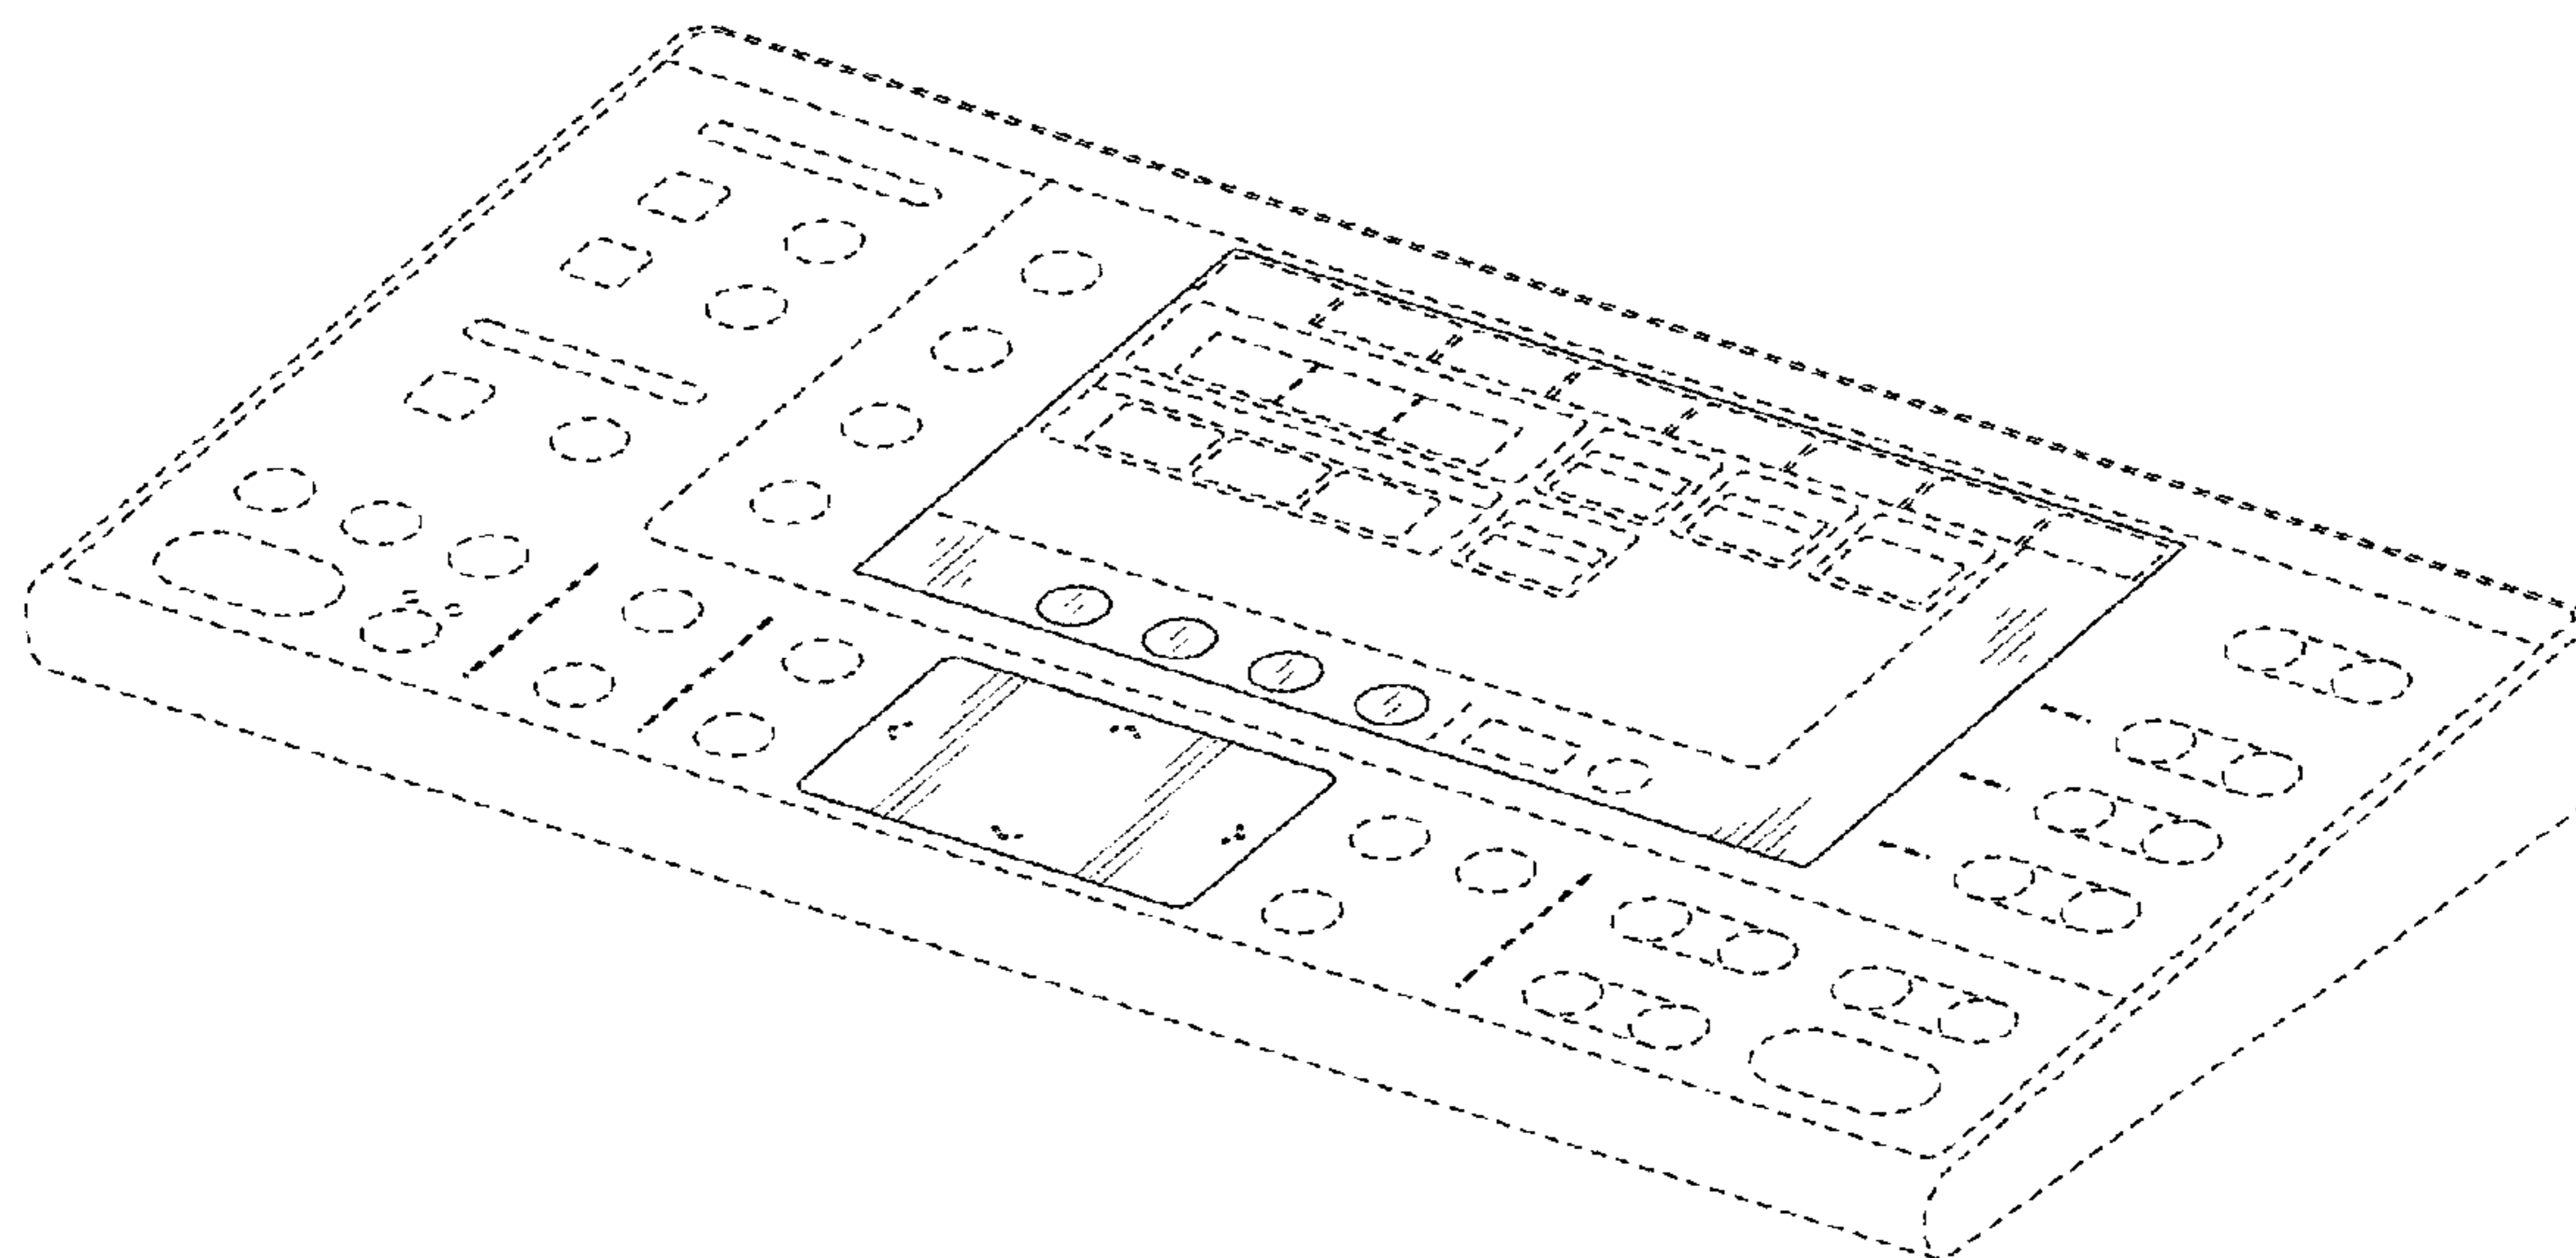


FIG. 1

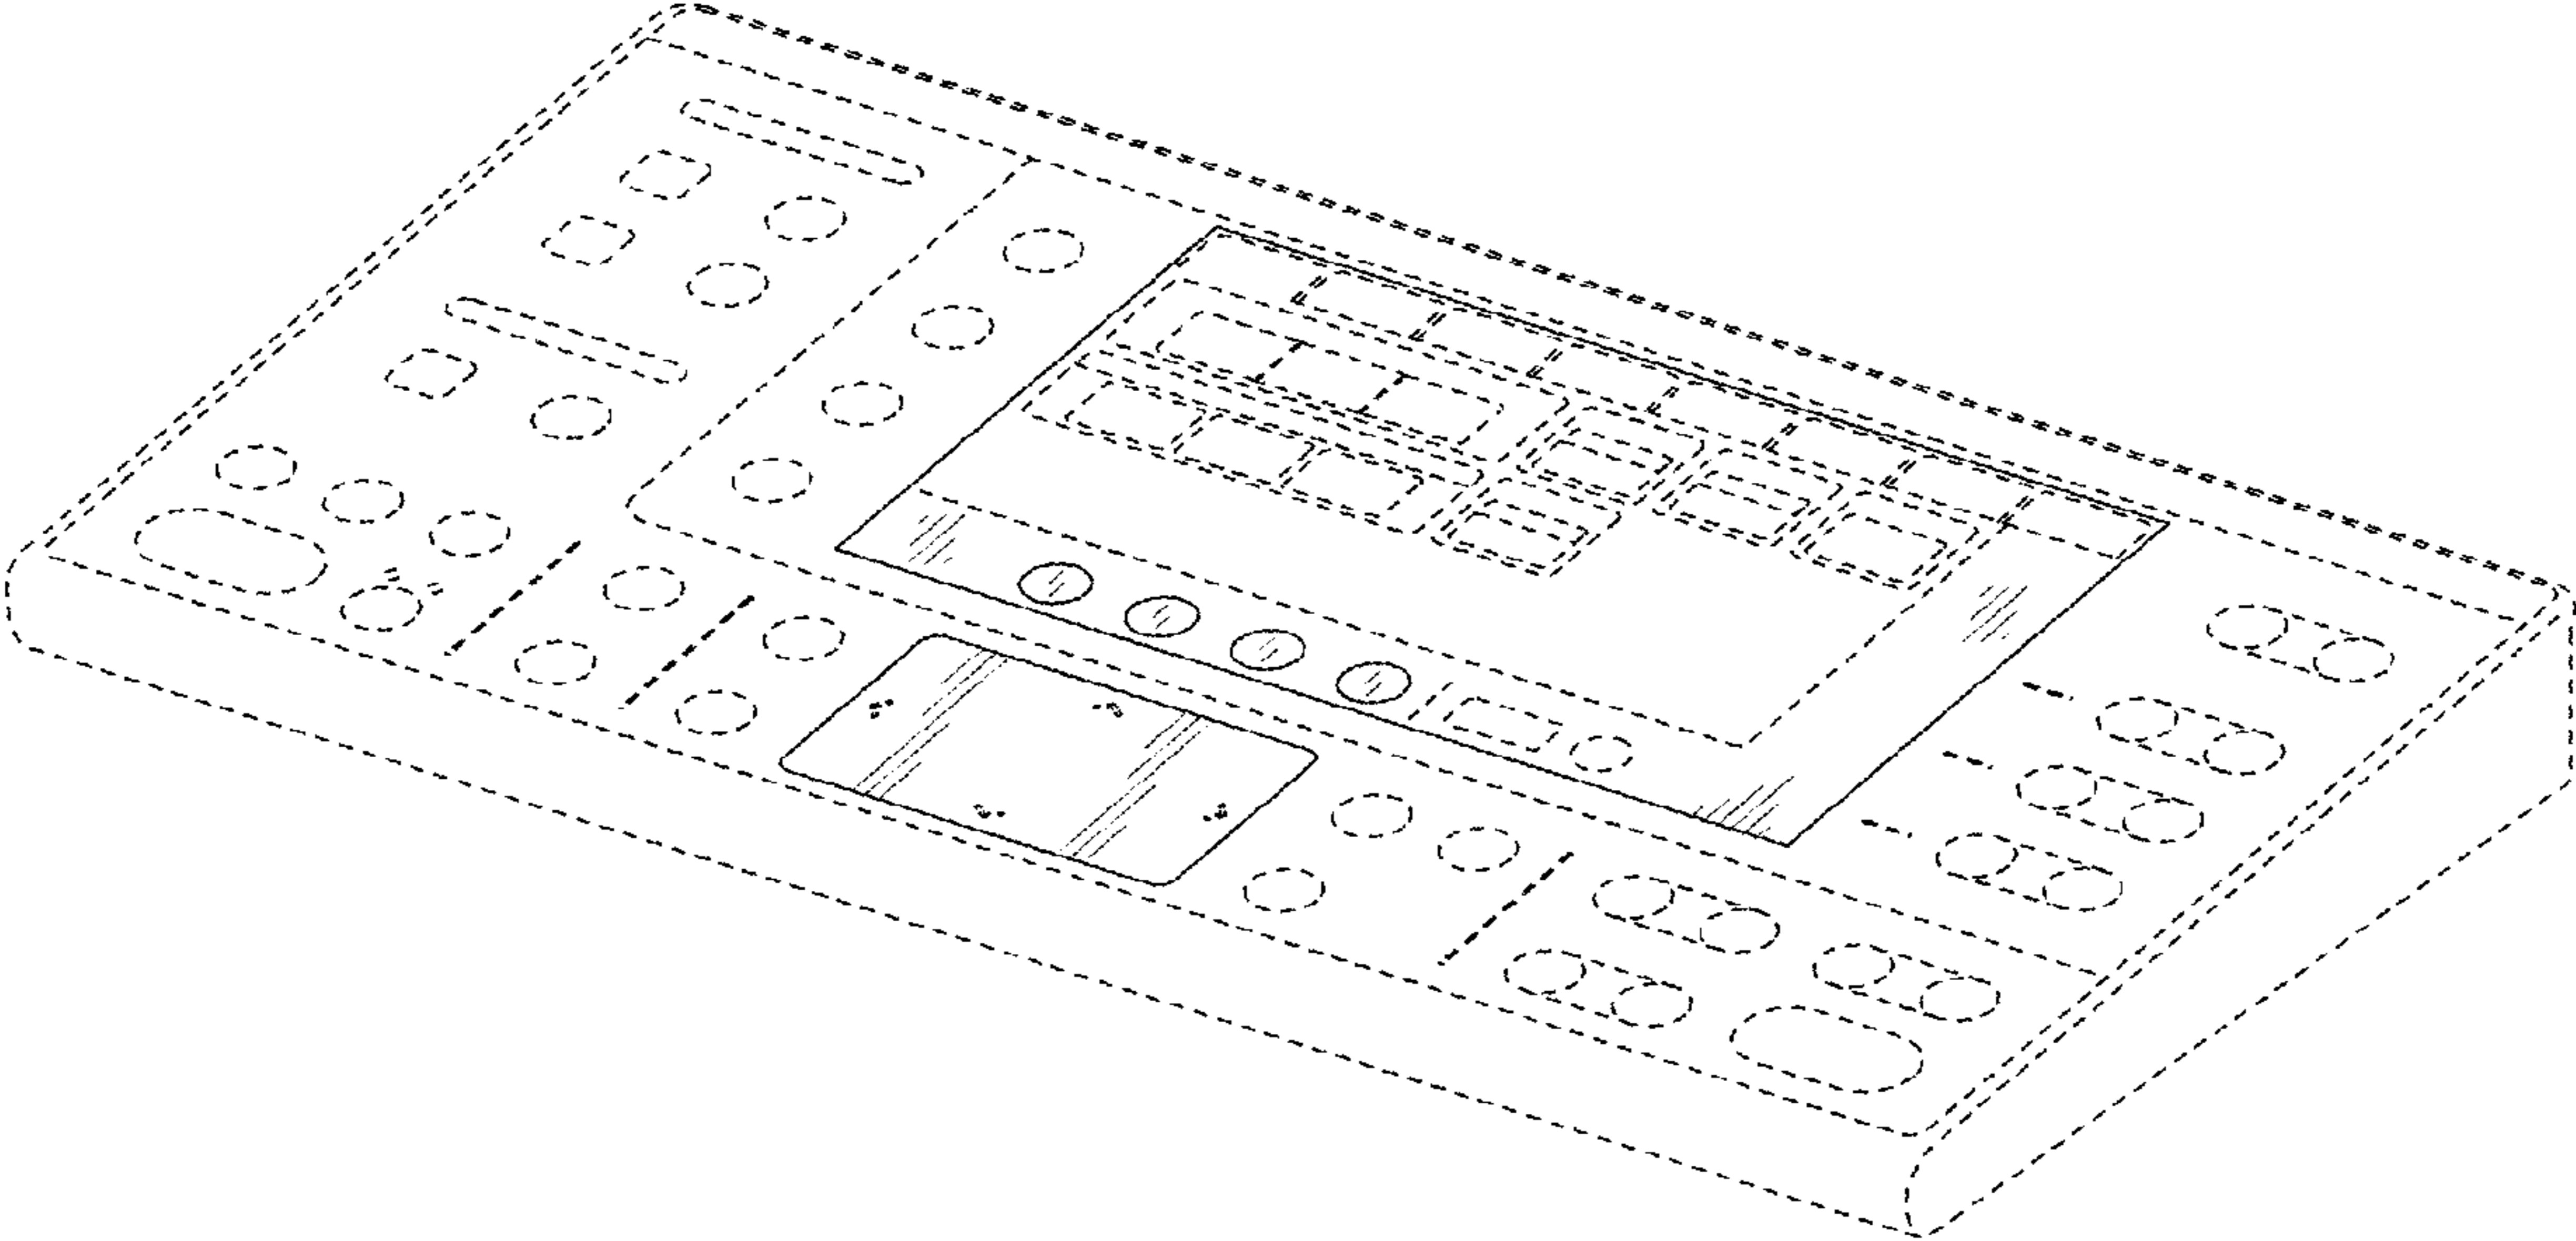


FIG. 2

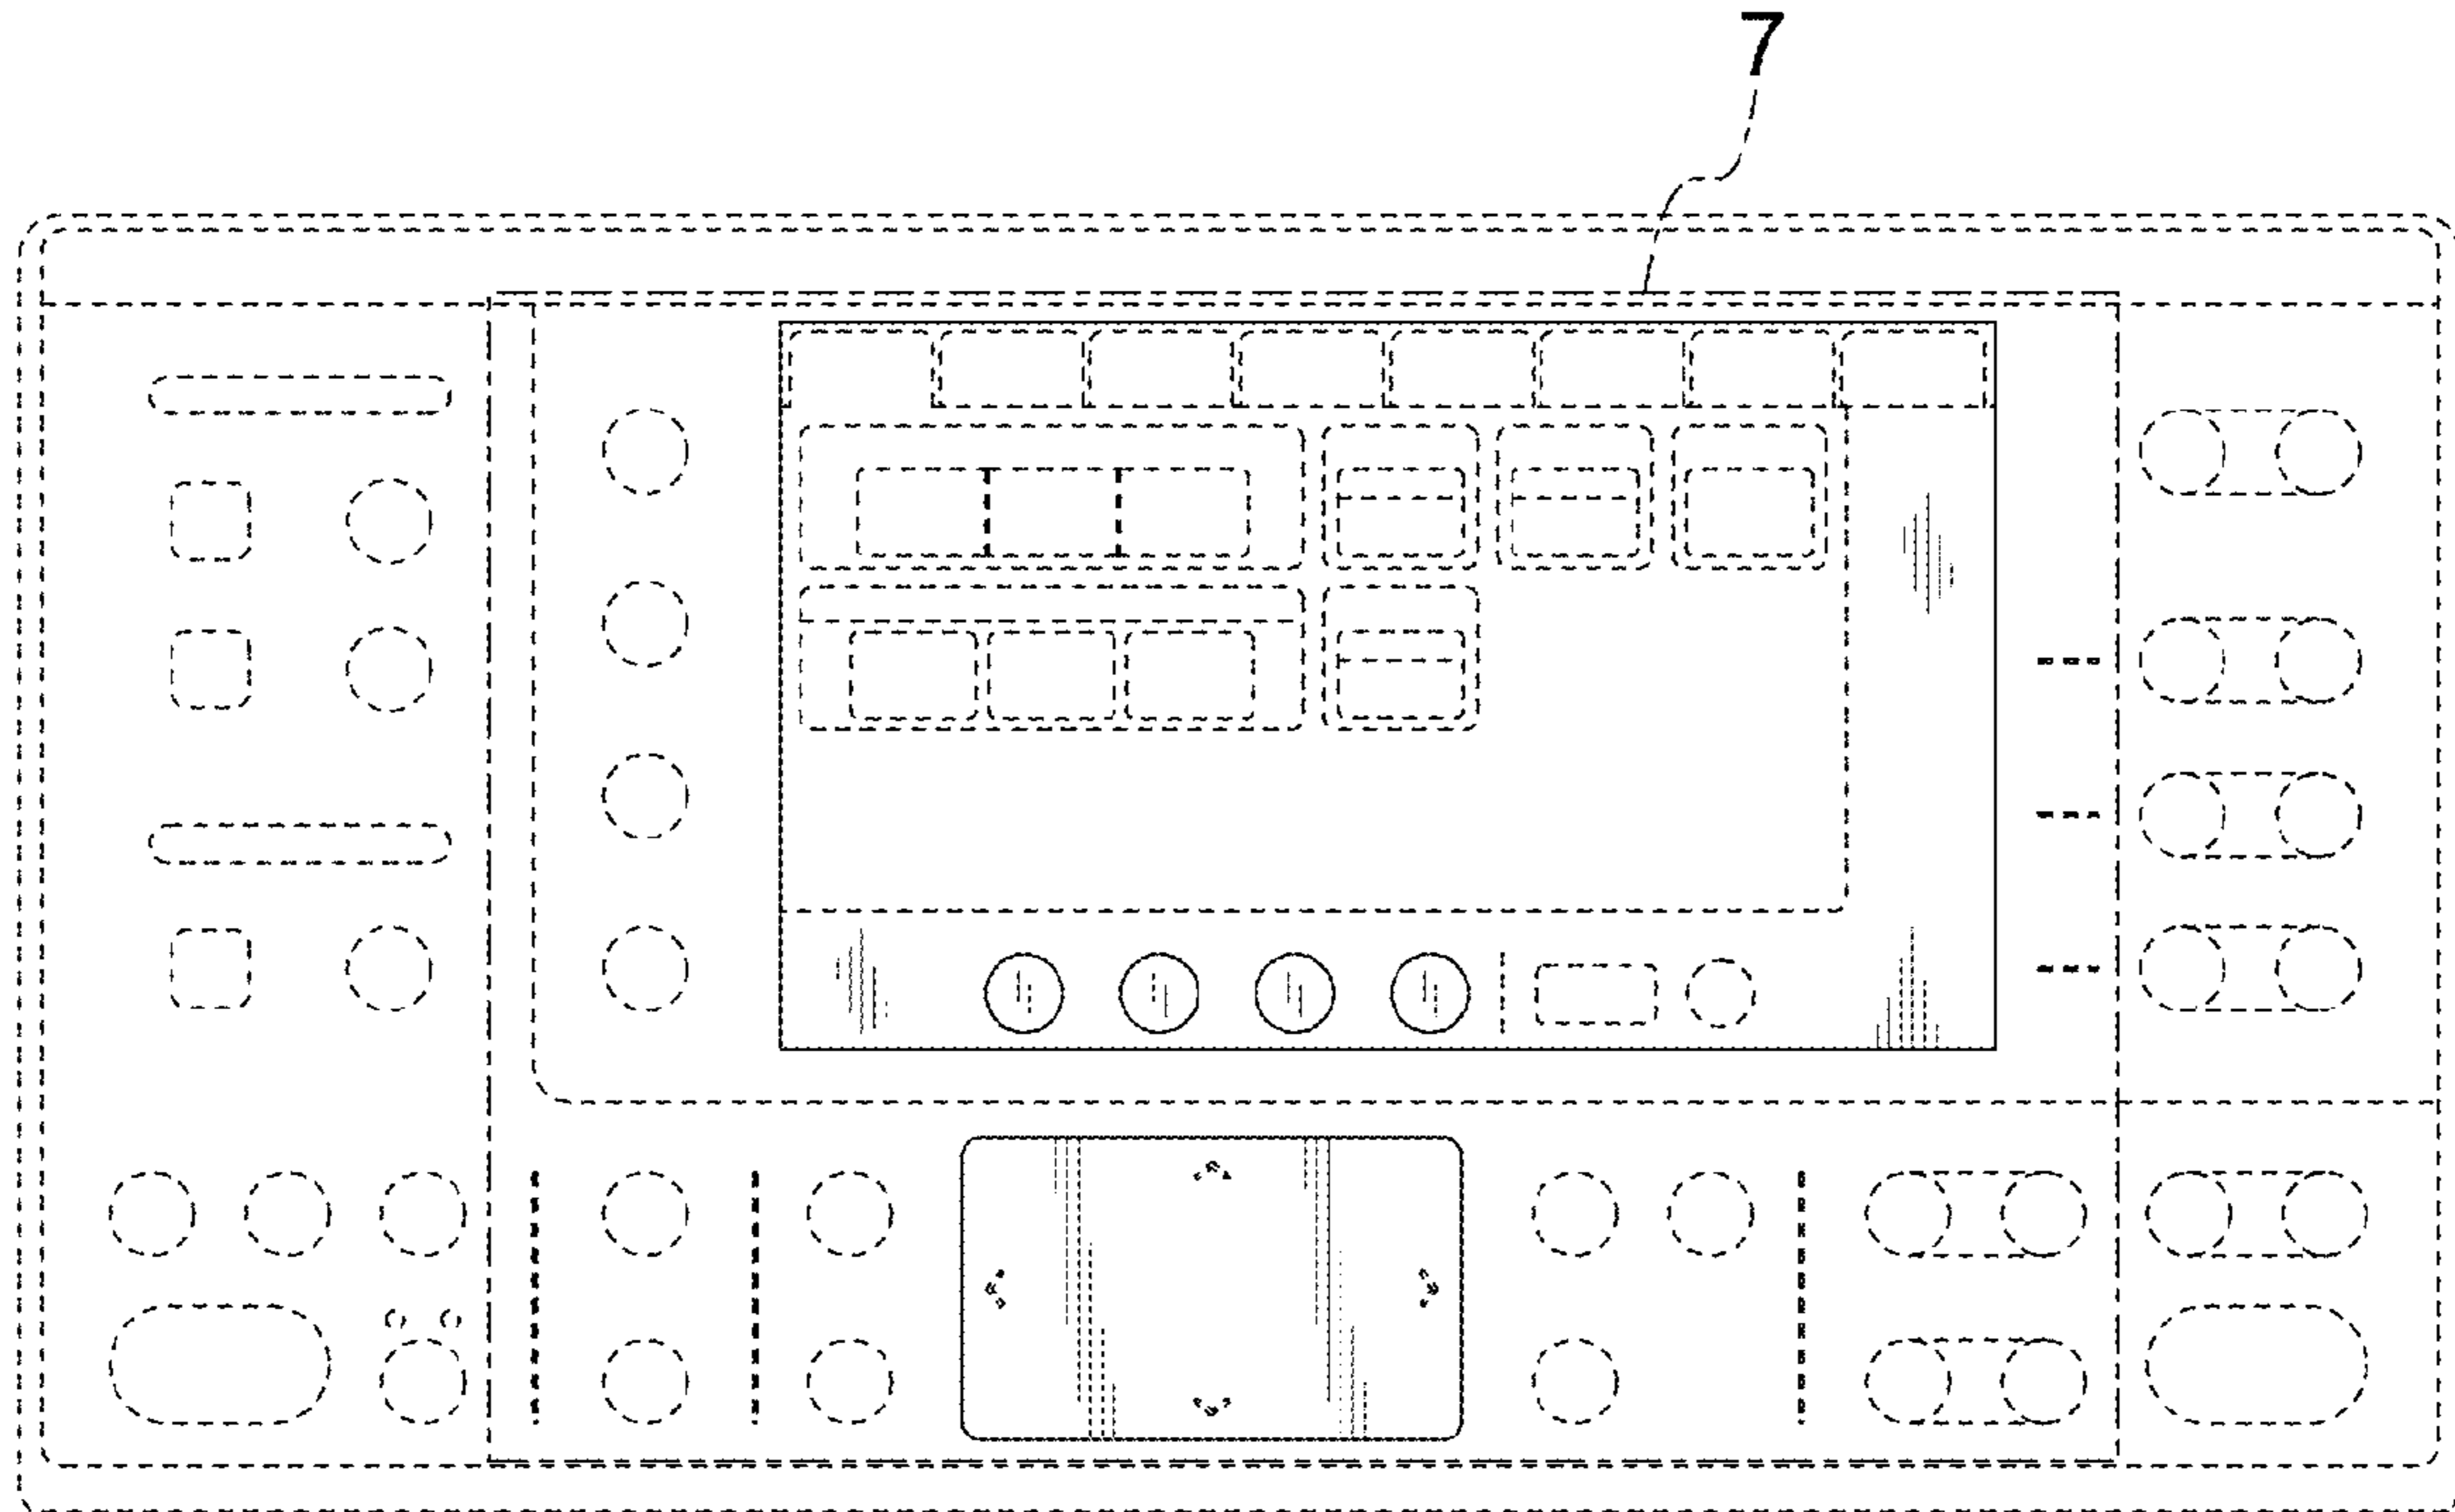
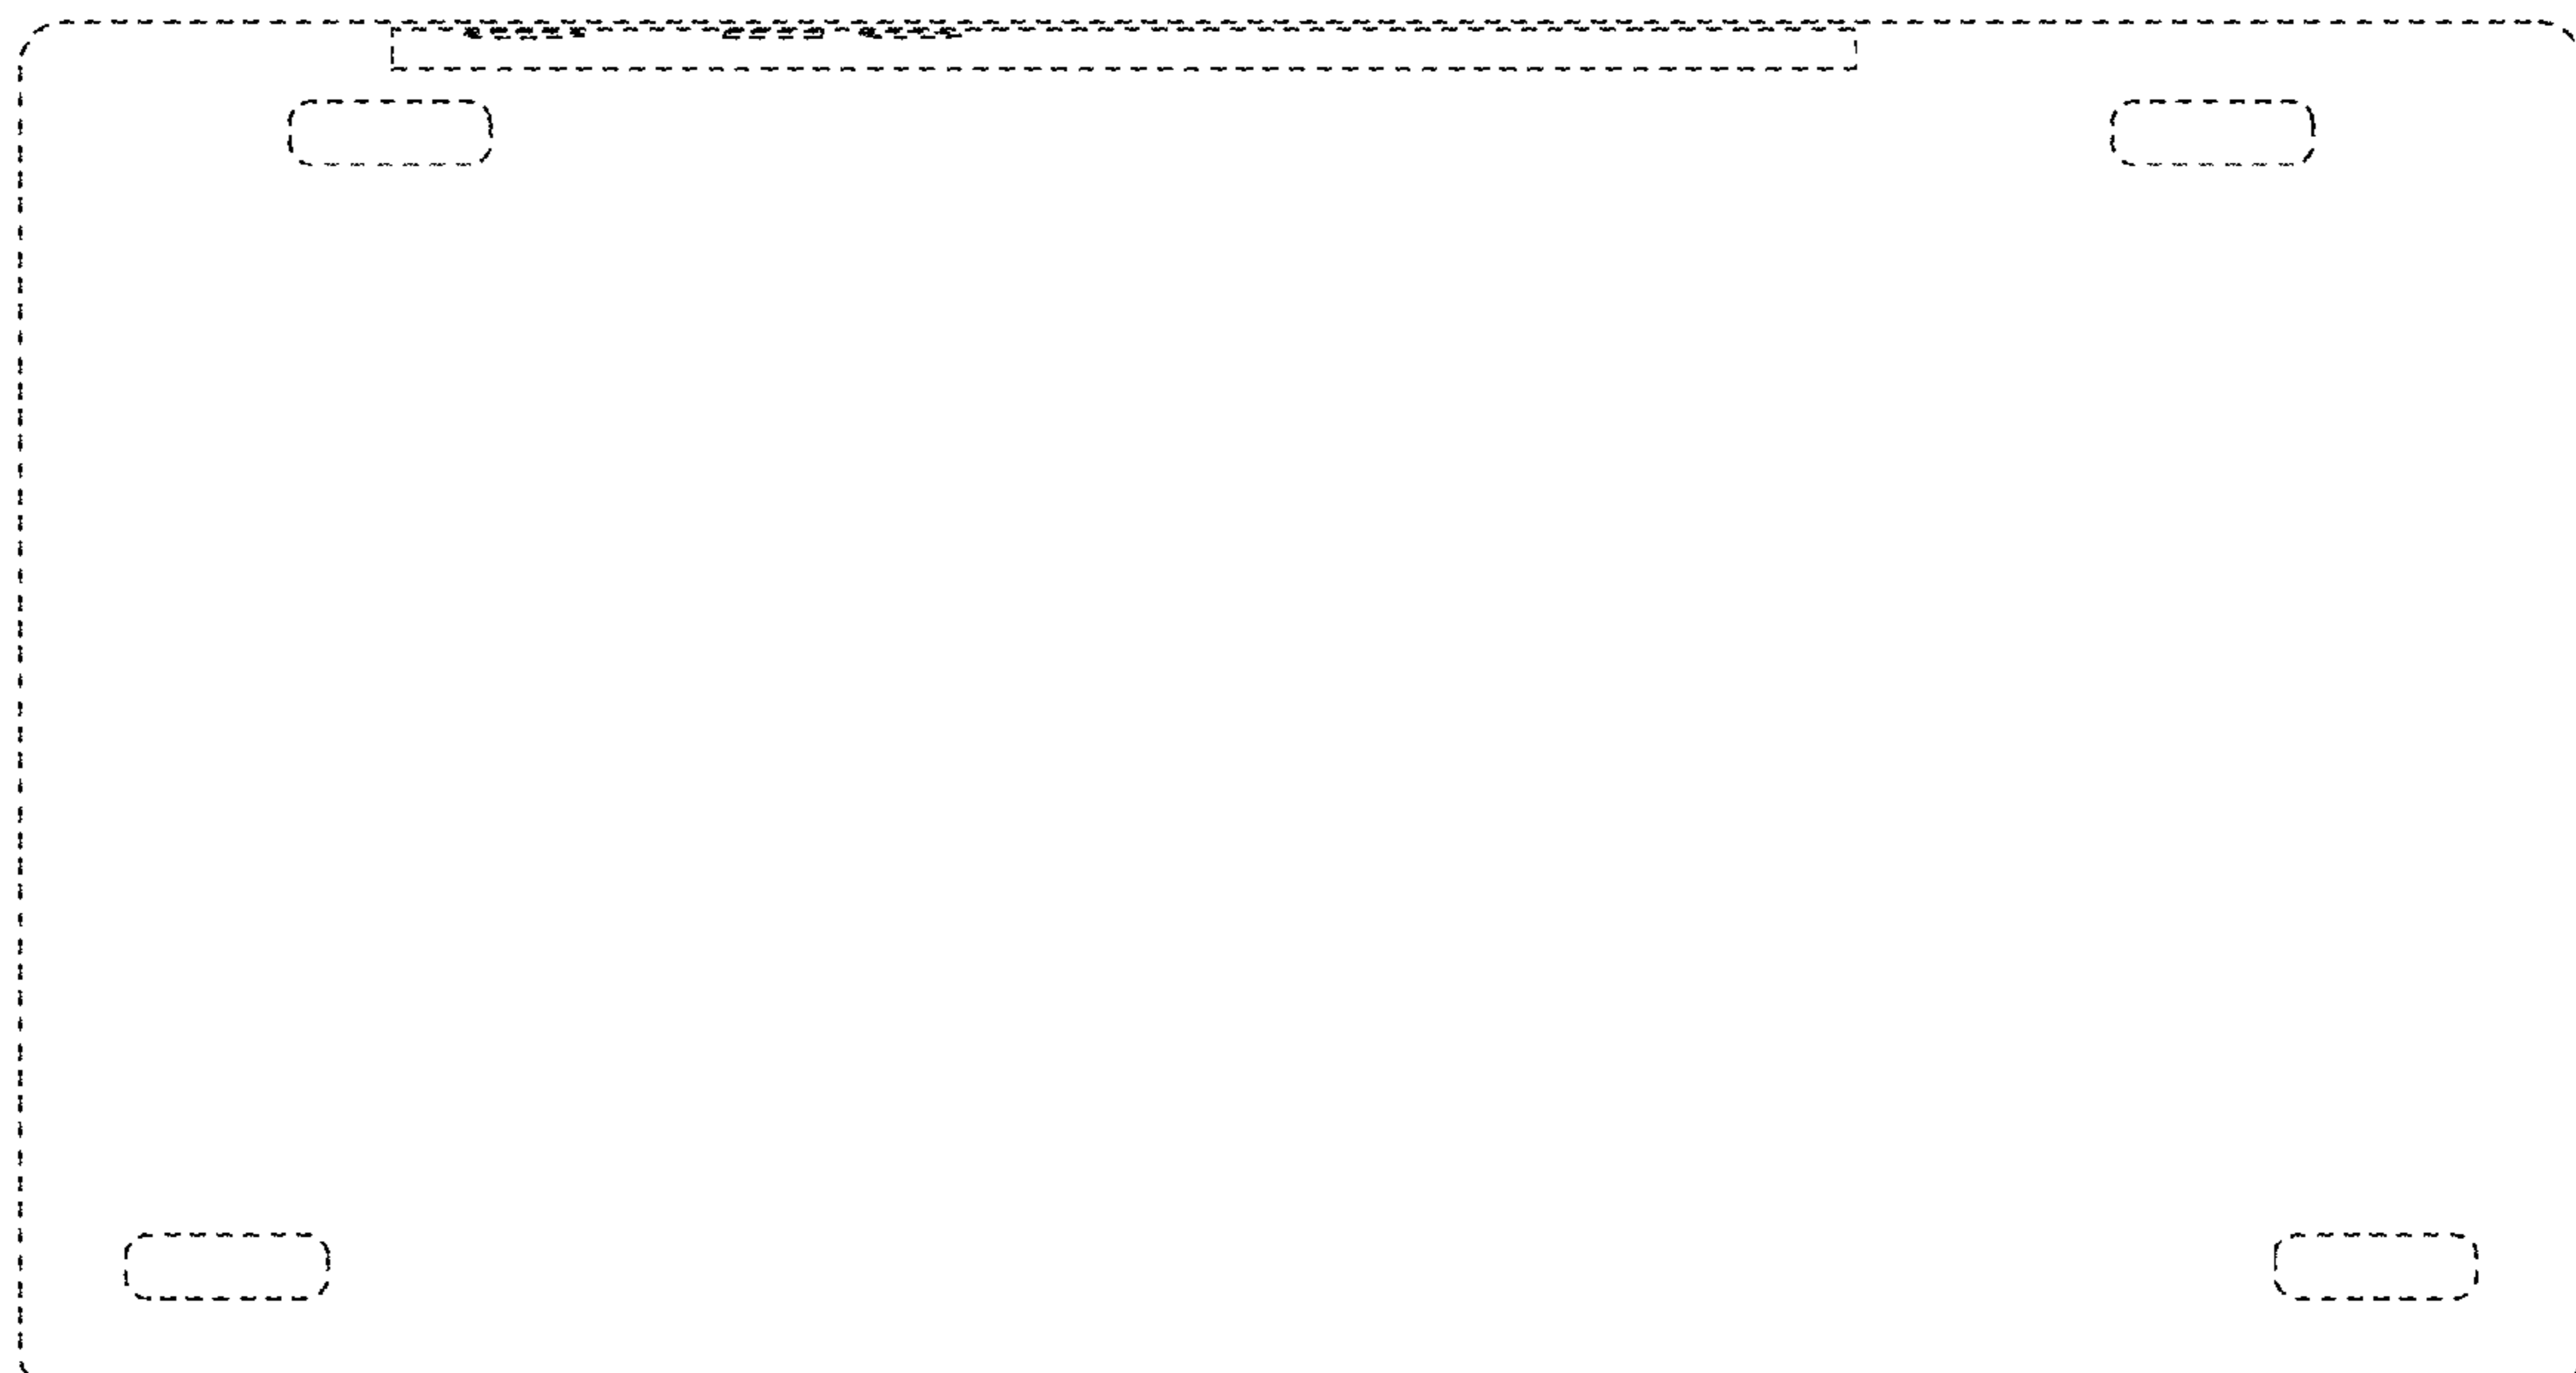
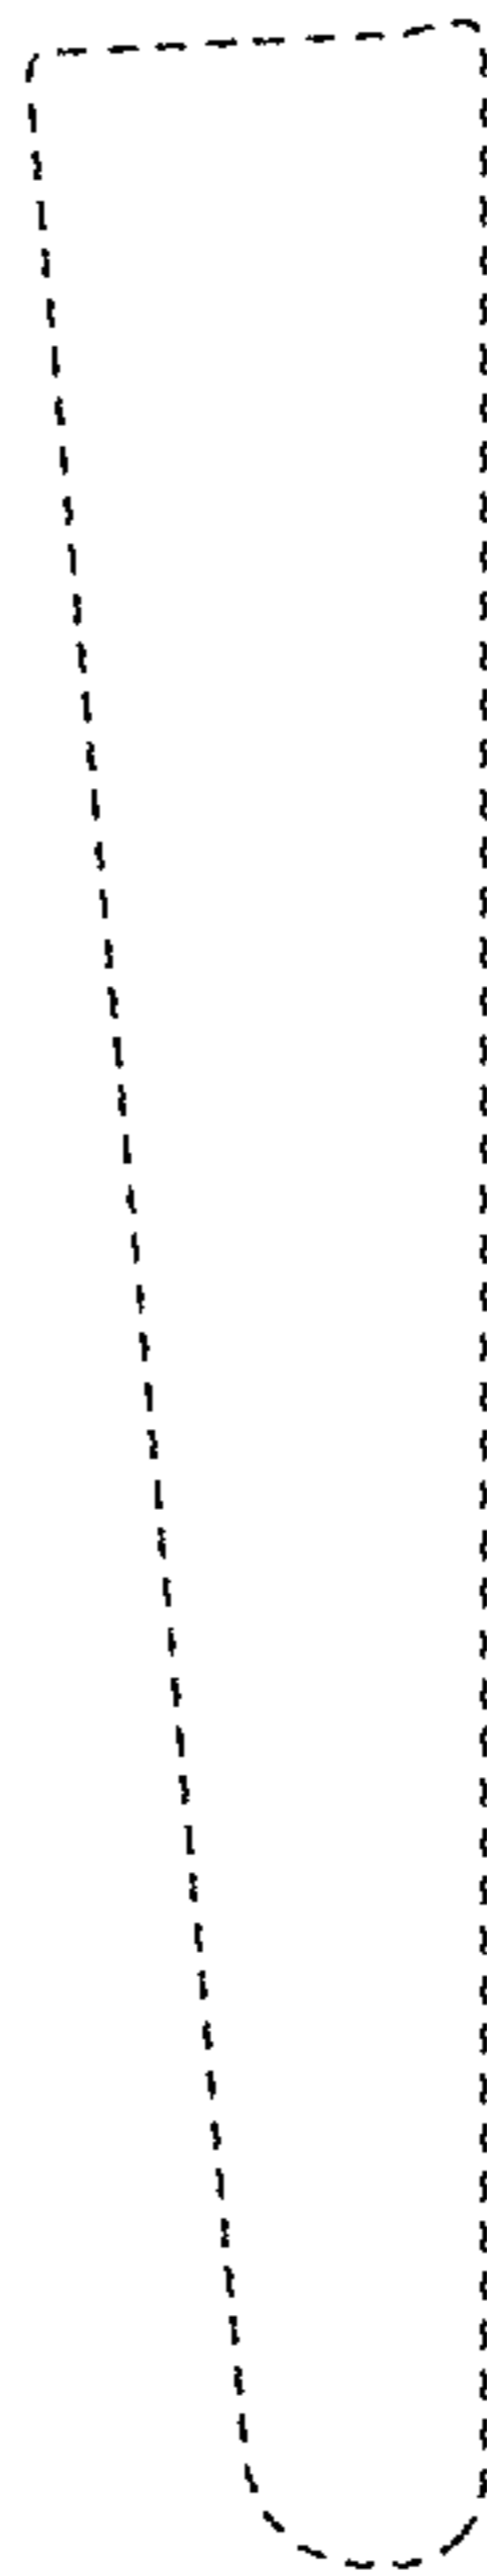


FIG. 3



*FIG. 4*



*FIG. 5*



*FIG. 6*



FIG. 7

