



US00D973876S

(12) **United States Design Patent** (10) **Patent No.:** **US D973,876 S**
Young (45) **Date of Patent:** **** Dec. 27, 2022**

(54) **BLOOD SAMPLING DEVICE**
(71) Applicant: **Stephen A. Young**, Albemarle, NC (US)
(72) Inventor: **Stephen A. Young**, Albemarle, NC (US)
(**) Term: **15 Years**
(21) Appl. No.: **29/728,375**
(22) Filed: **Mar. 18, 2020**
(51) **LOC (13) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/146**
(58) **Field of Classification Search**
USPC D24/112-114, 117-119, 127, 130, 133, D24/186, 104, 165, 167, 169; D21/385, D21/386, 388, 403, 404; D11/121, 122, D11/123, 124, 132, 133; D10/46, 104.1, D10/106.1, 106.5, 106.6, 116.1, 118, D10/118.1, 118.2, 119.1, 120, 121, 124, D10/126; D13/171
CPC .. A61M 2005/14268; A61M 2005/341; A61M 2009/045; A61M 5/1413; A61M 5/14244; A61M 5/14248; A61M 5/165; A61M 5/36; A61M 5/38; A61B 5/150022; A61B 5/14532; A61B 5/157
See application file for complete search history.

6,749,618 B2 6/2004 Levaughn et al.
D531,725 S 11/2006 Loerwald et al.
7,303,726 B2 * 12/2007 McAllister A61B 5/1518
436/166
8,372,015 B2 2/2013 Escutia et al.
8,545,693 B2 * 10/2013 McColl G01N 27/3271
204/403.01
D707,826 S * 6/2014 Young D24/169
8,828,038 B2 9/2014 Brown et al.
D736,111 S * 8/2015 Klein D24/169
D757,273 S * 5/2016 Nelson D24/169
D783,170 S * 4/2017 Carreon D24/167
D788,061 S * 5/2017 Siminoff D10/118.2
D788,603 S * 6/2017 Liu D10/49
D789,820 S * 6/2017 Siminoff D10/118.2
D798,177 S * 9/2017 Siminoff D10/118.2
D800,313 S * 10/2017 Chang D24/167

(Continued)

Primary Examiner — Samantha Q Lawrence
(74) *Attorney, Agent, or Firm* — Ashley Law Firm P.C.;
Stephen S. Ashley, Jr.

(57) **CLAIM**


I claim the ornamental design for a blood sampling device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the blood sampling device according to the invention;
FIG. 2 is a left side view of the blood sampling device;
FIG. 3 is an inverted right side view of the blood sampling device;
FIG. 4 is a front elevation of the blood sampling device;
FIG. 5 is a top plan view of the blood sampling device;
FIG. 6 is a rear elevation of the blood sampling device; and,
FIG. 7 is a bottom plan view of the blood sampling device.
The broken lines shown in FIGS. 1-3 illustrate portions of the blood sampling device that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

(56) **References Cited**
U.S. PATENT DOCUMENTS
4,554,353 A * 11/1985 Chorvat C07D 207/40
546/208
D318,695 S * 7/1991 Rosa D21/406
D339,760 S * 9/1993 Lucero D10/118
6,071,294 A 6/2000 Simons et al.
D444,557 S 7/2001 Levaughn et al.
6,706,159 B2 3/2004 Moerman et al.

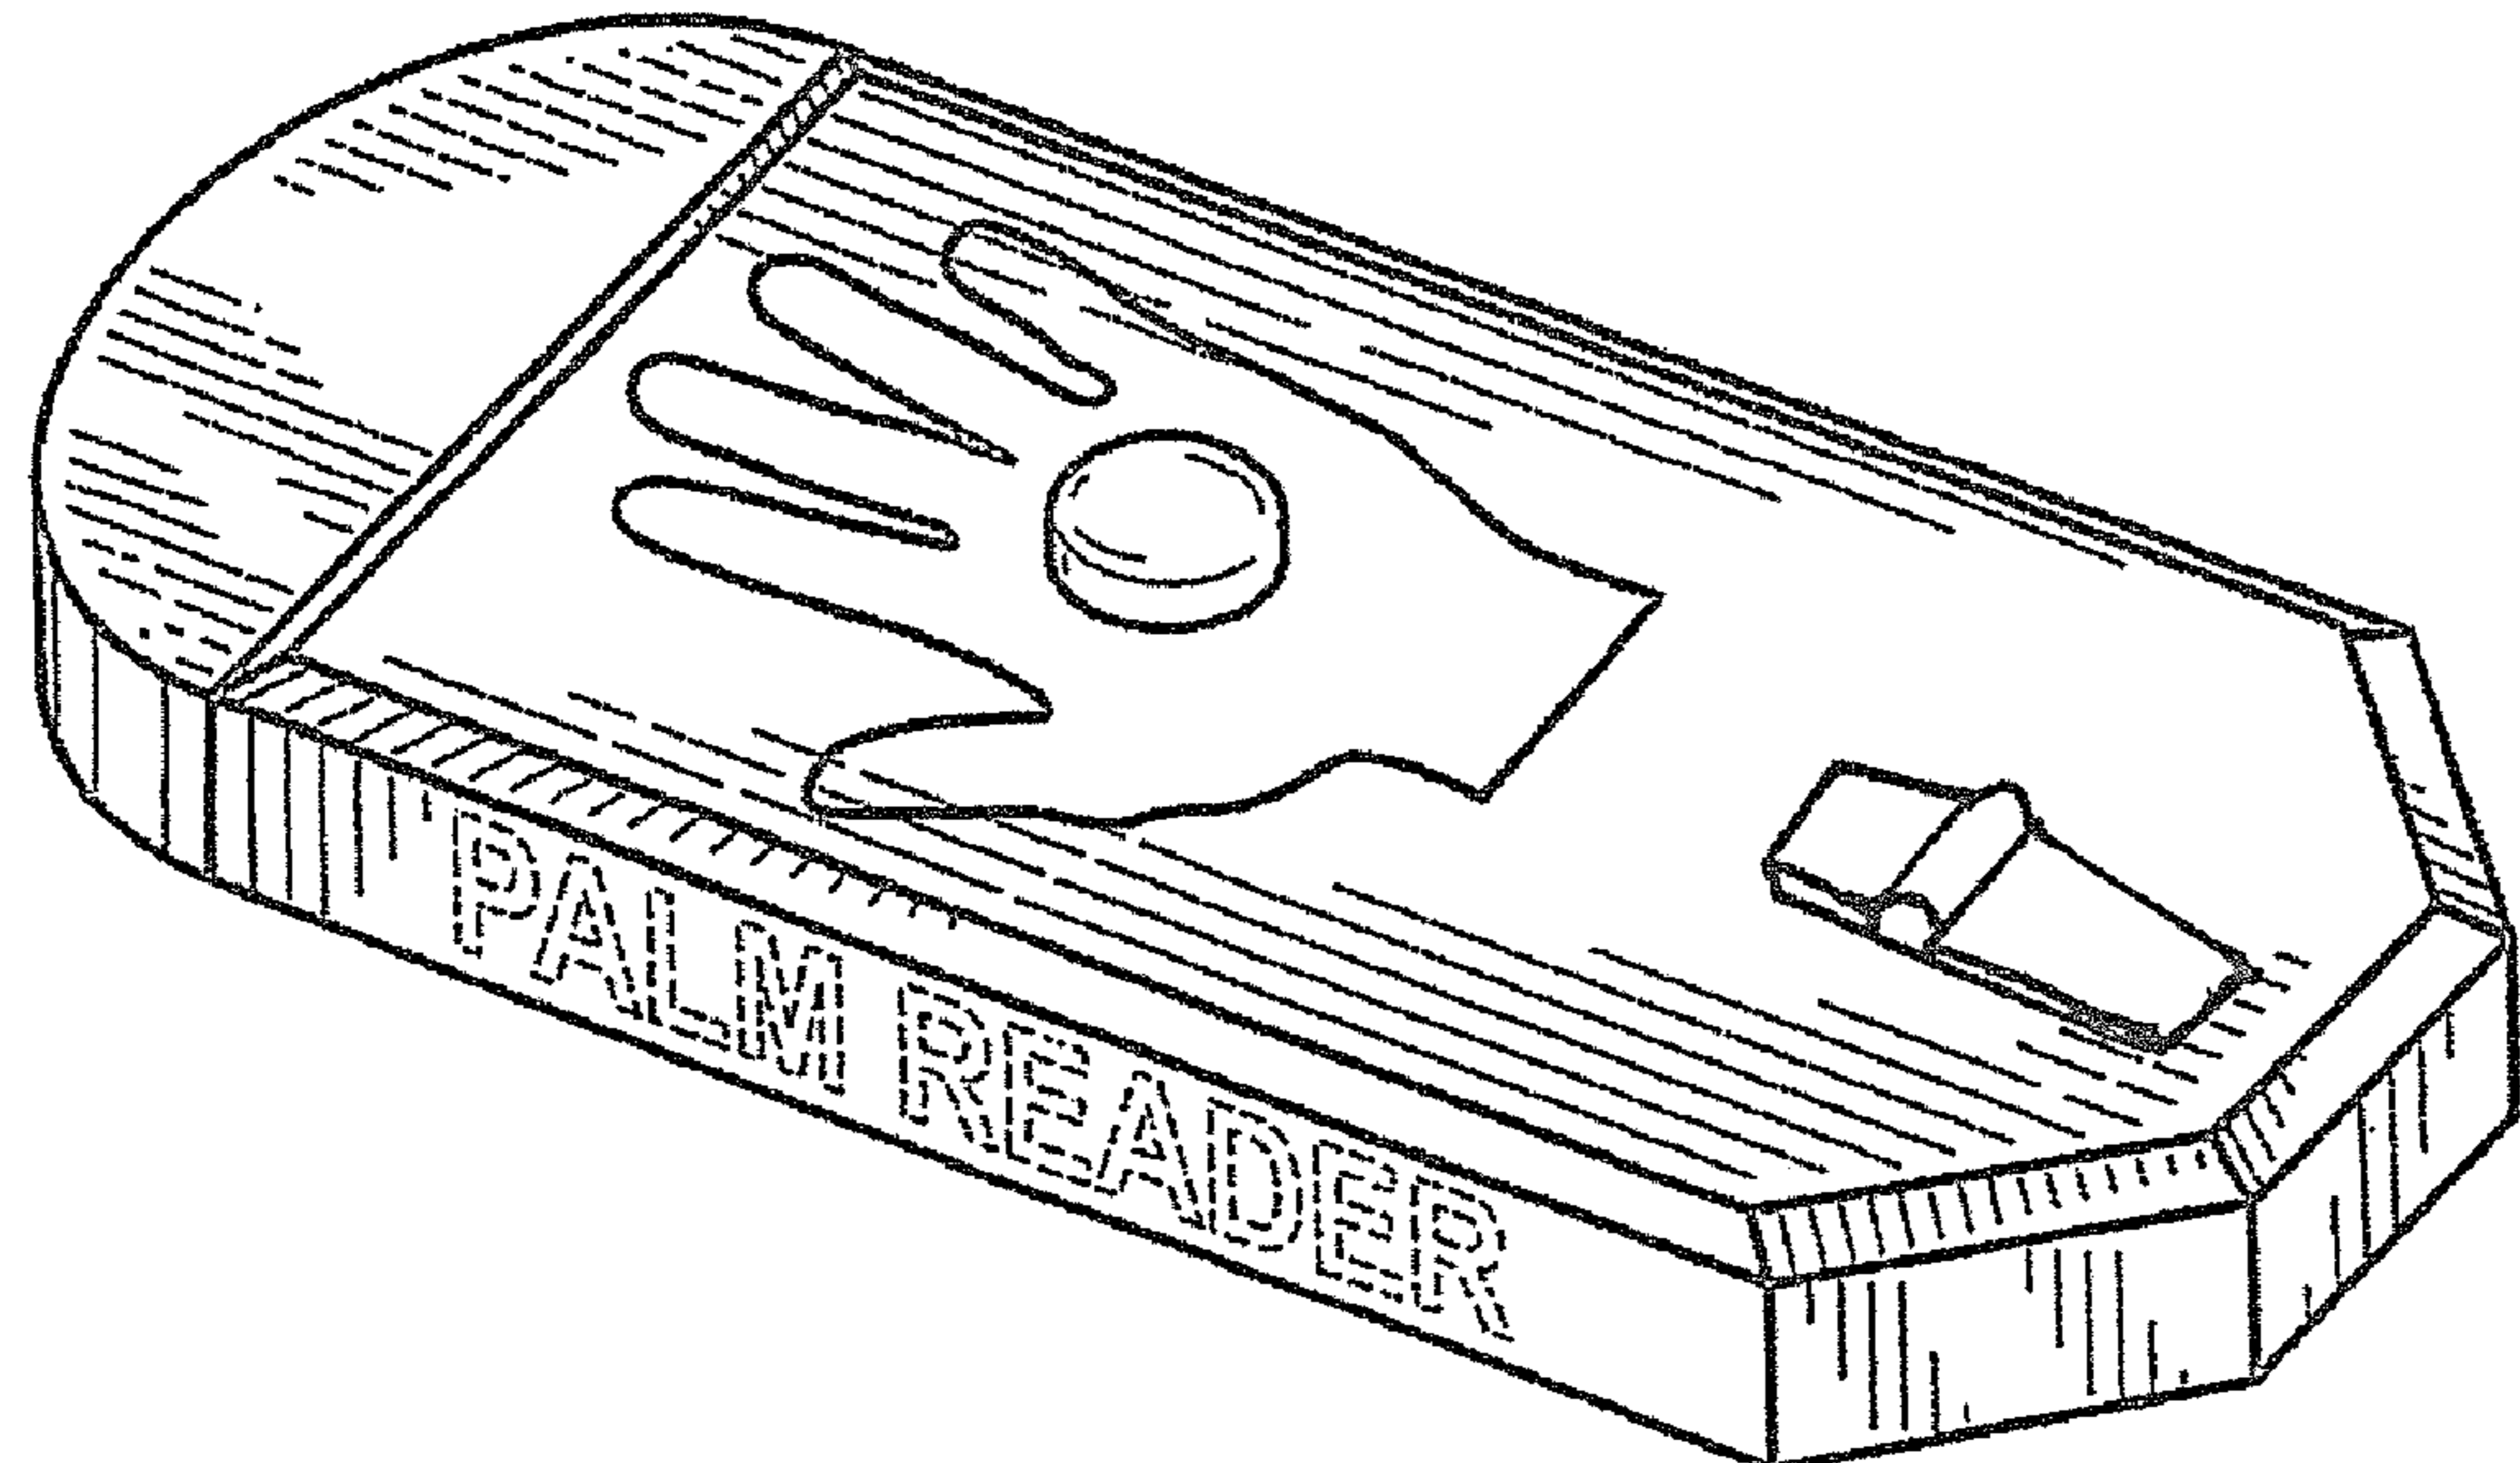

(56)

References Cited

U.S. PATENT DOCUMENTS

D812,229	S	*	3/2018	Al-Siddiq	D24/167
D824,517	S		7/2018	Young		
D825,356	S	*	8/2018	Yu	D10/70
D831,580	S	*	10/2018	Amano	D13/158
D835,589	S	*	12/2018	Zhang	D13/171
D837,079	S	*	1/2019	Mansen	D10/106.1
D852,956	S		7/2019	Young		
2003/0212345	A1	*	11/2003	McAllister	A61B 5/150427 600/584
2009/0237262	A1	*	9/2009	Smith	A61B 5/7435 435/14

* cited by examiner

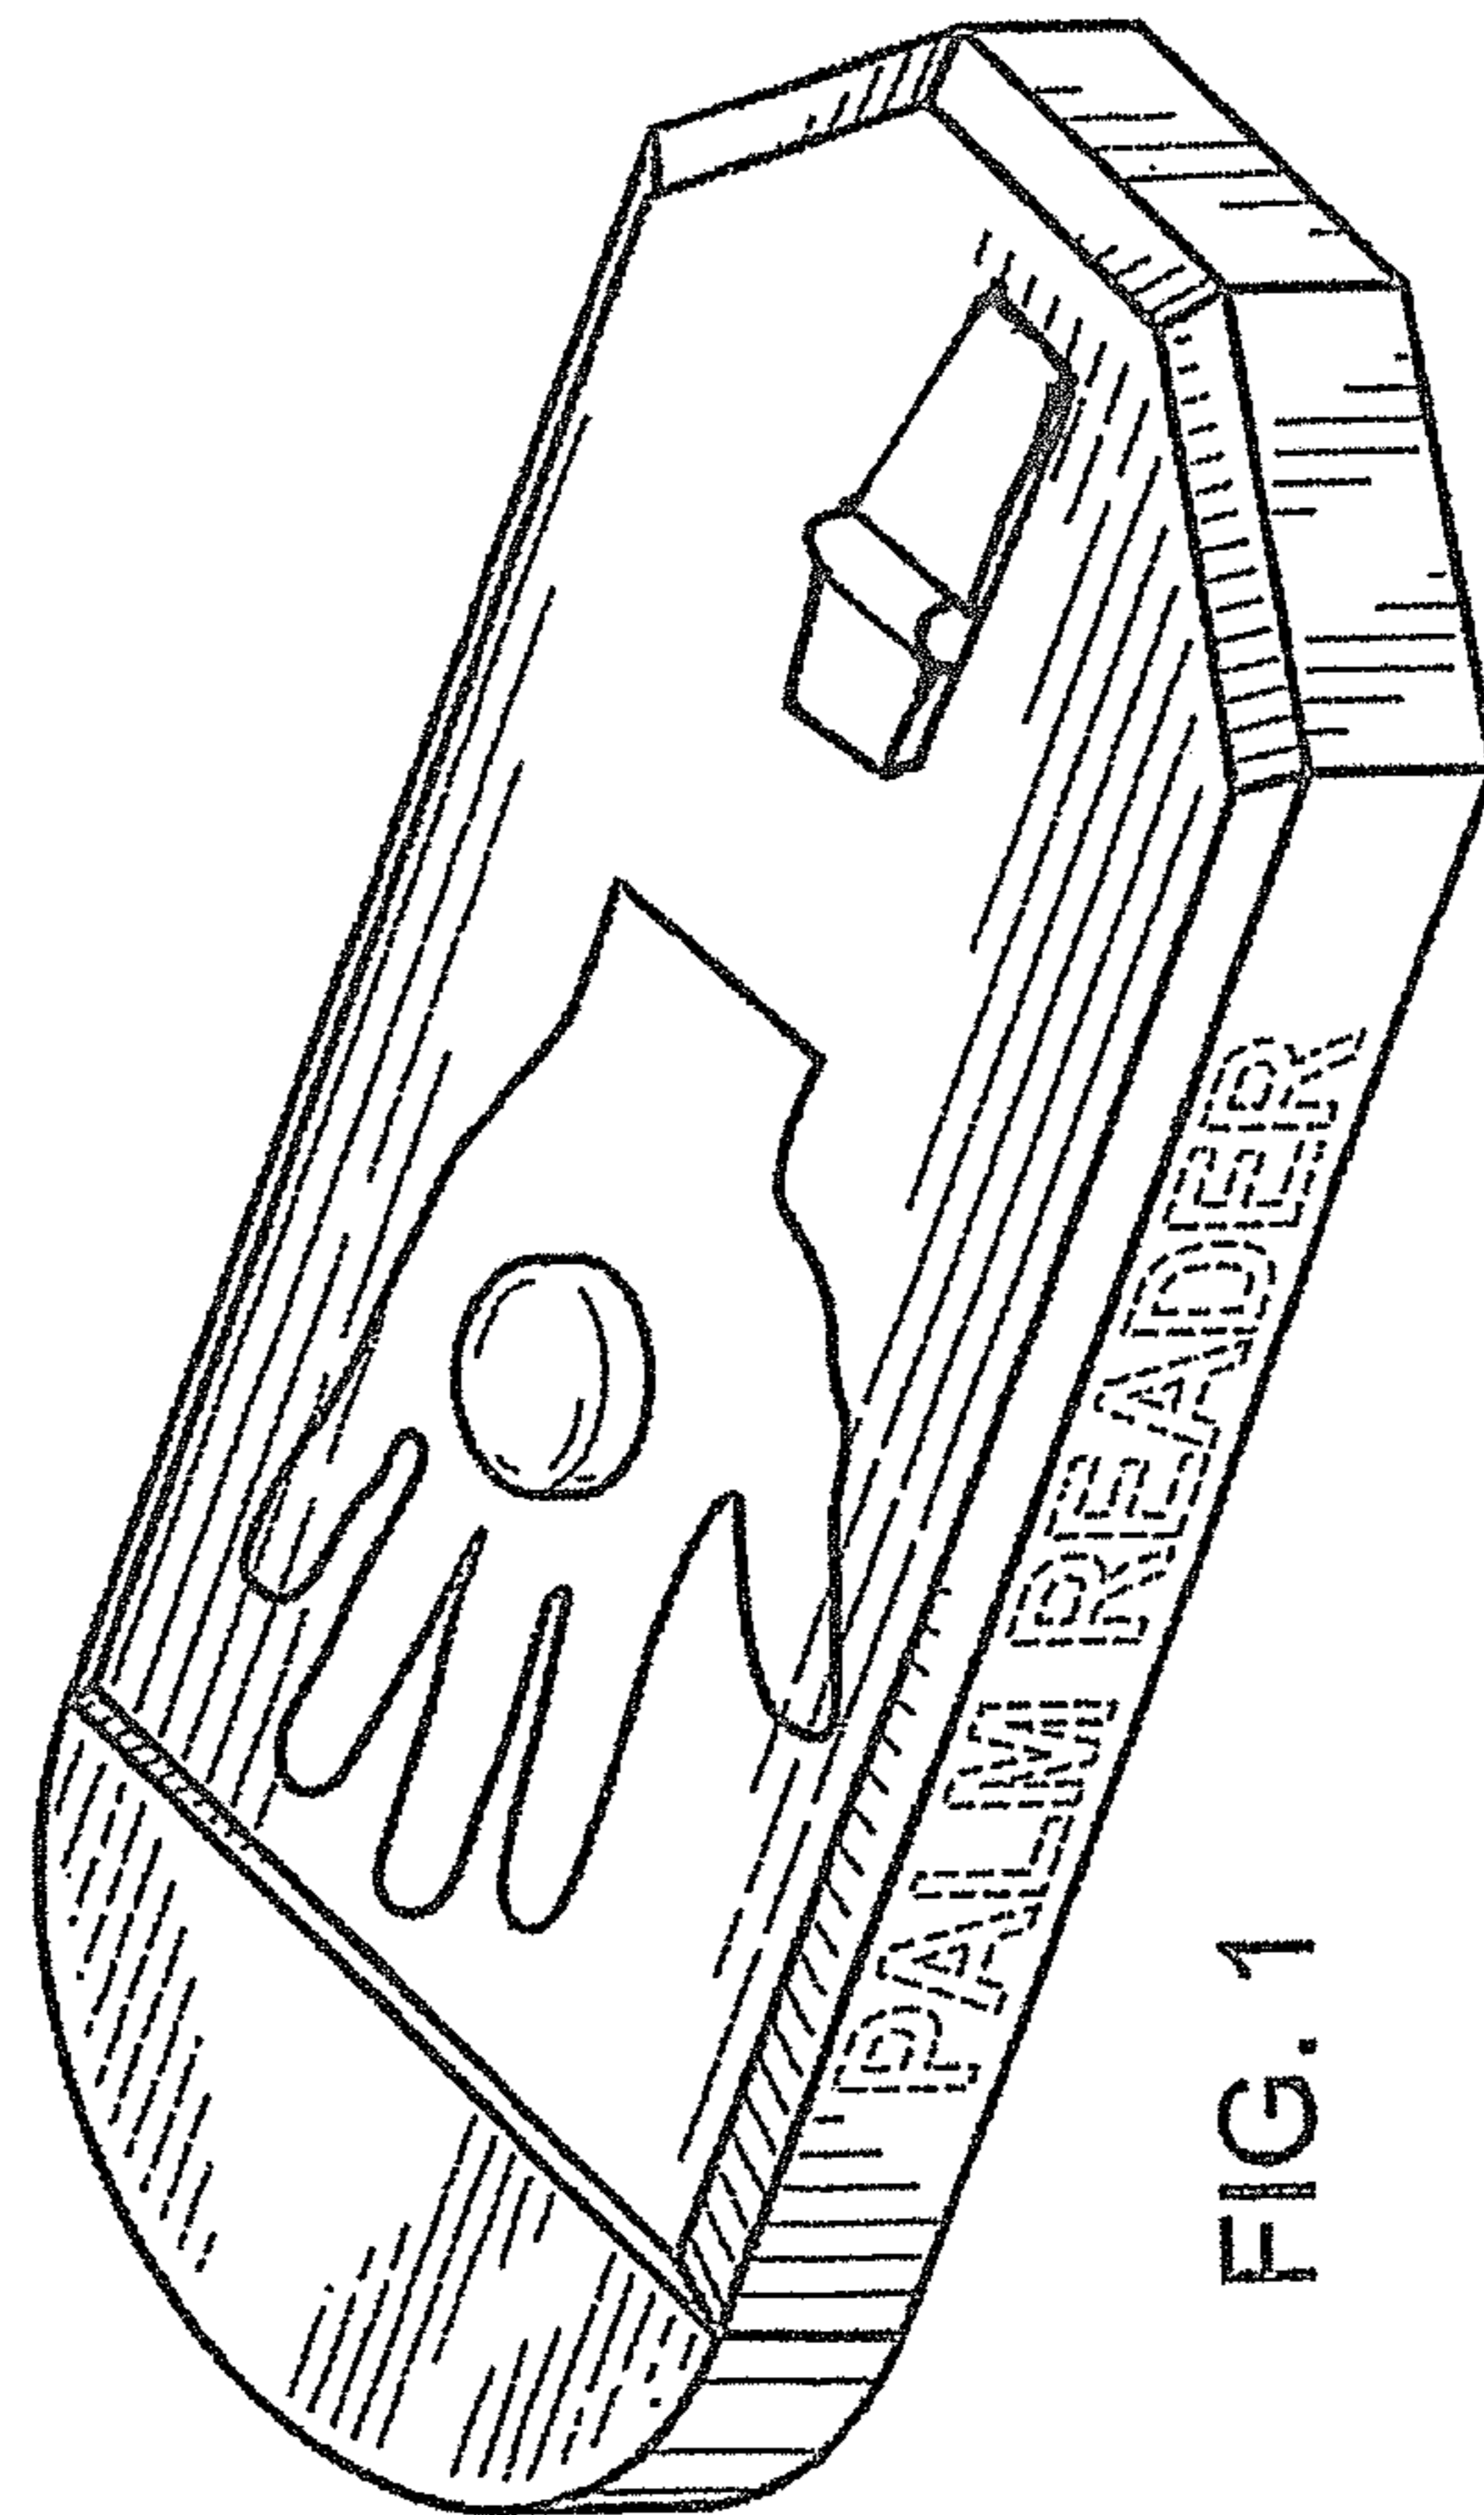


FIG. 1

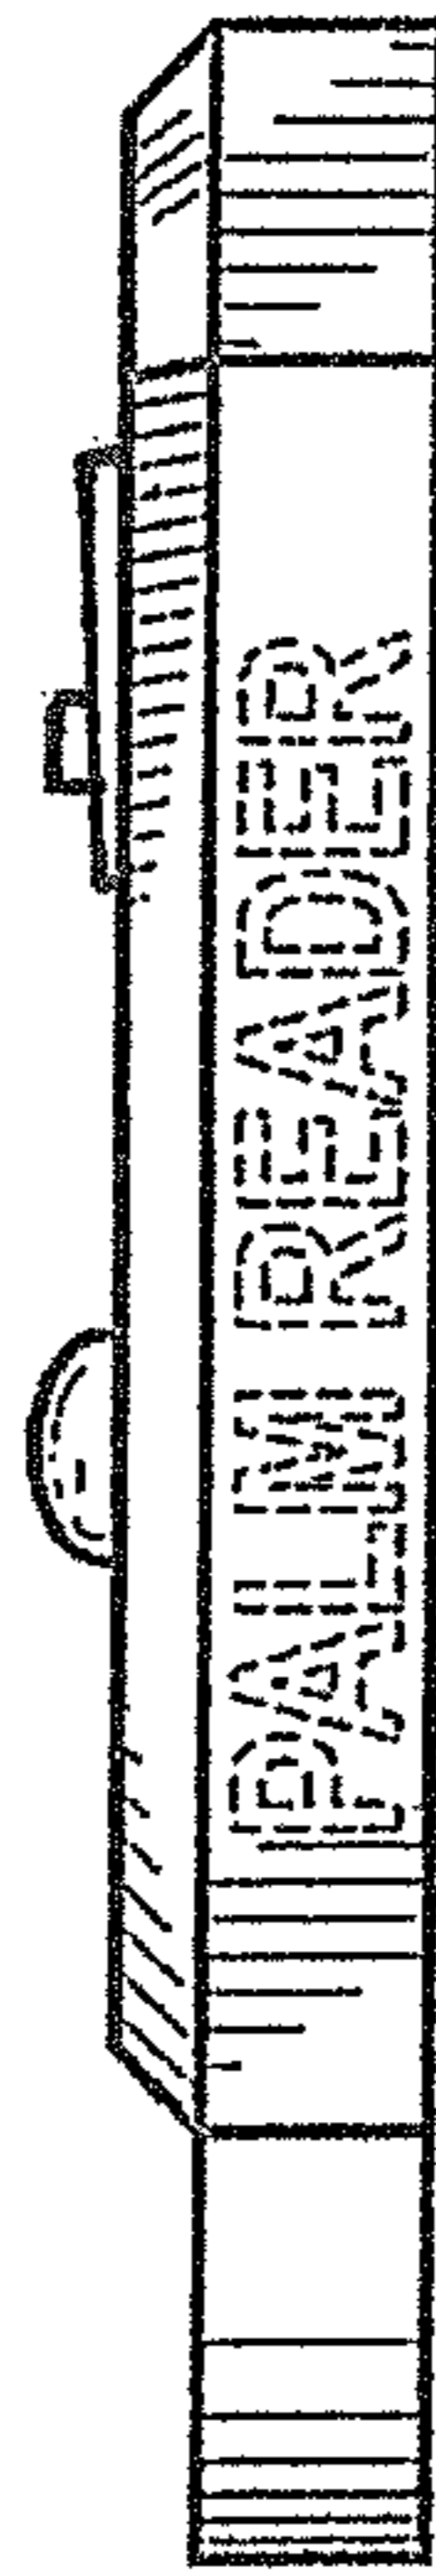


FIG. 2

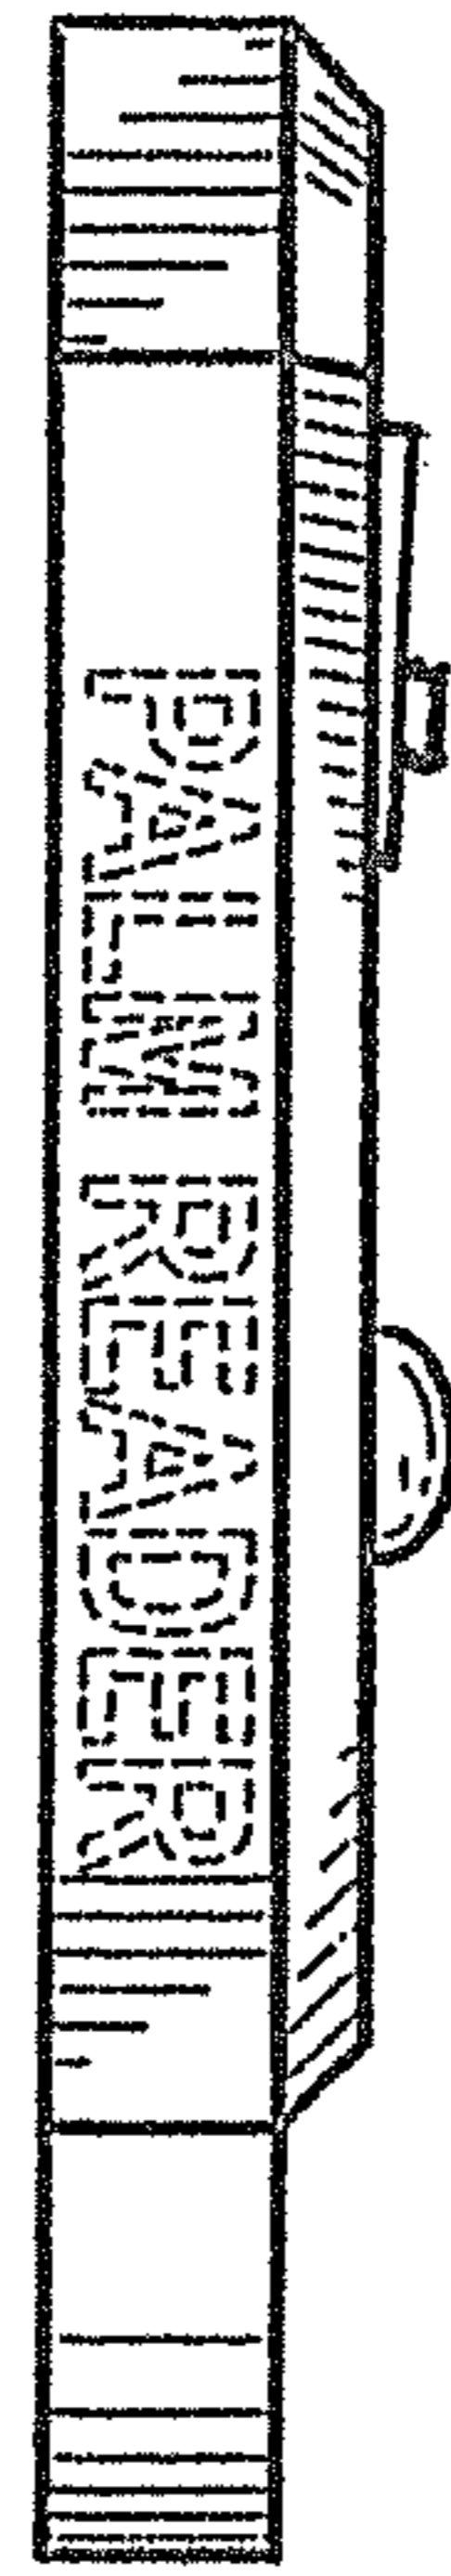


FIG. 3

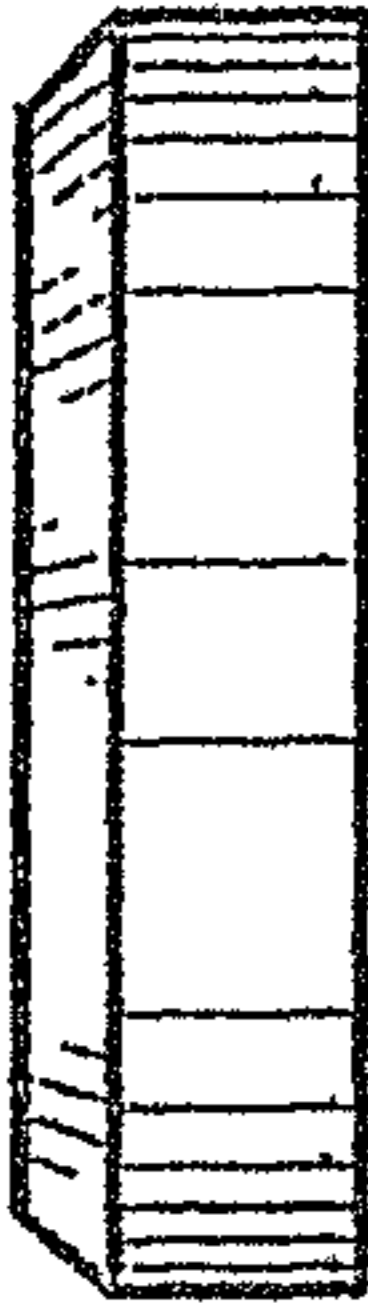


FIG. 4

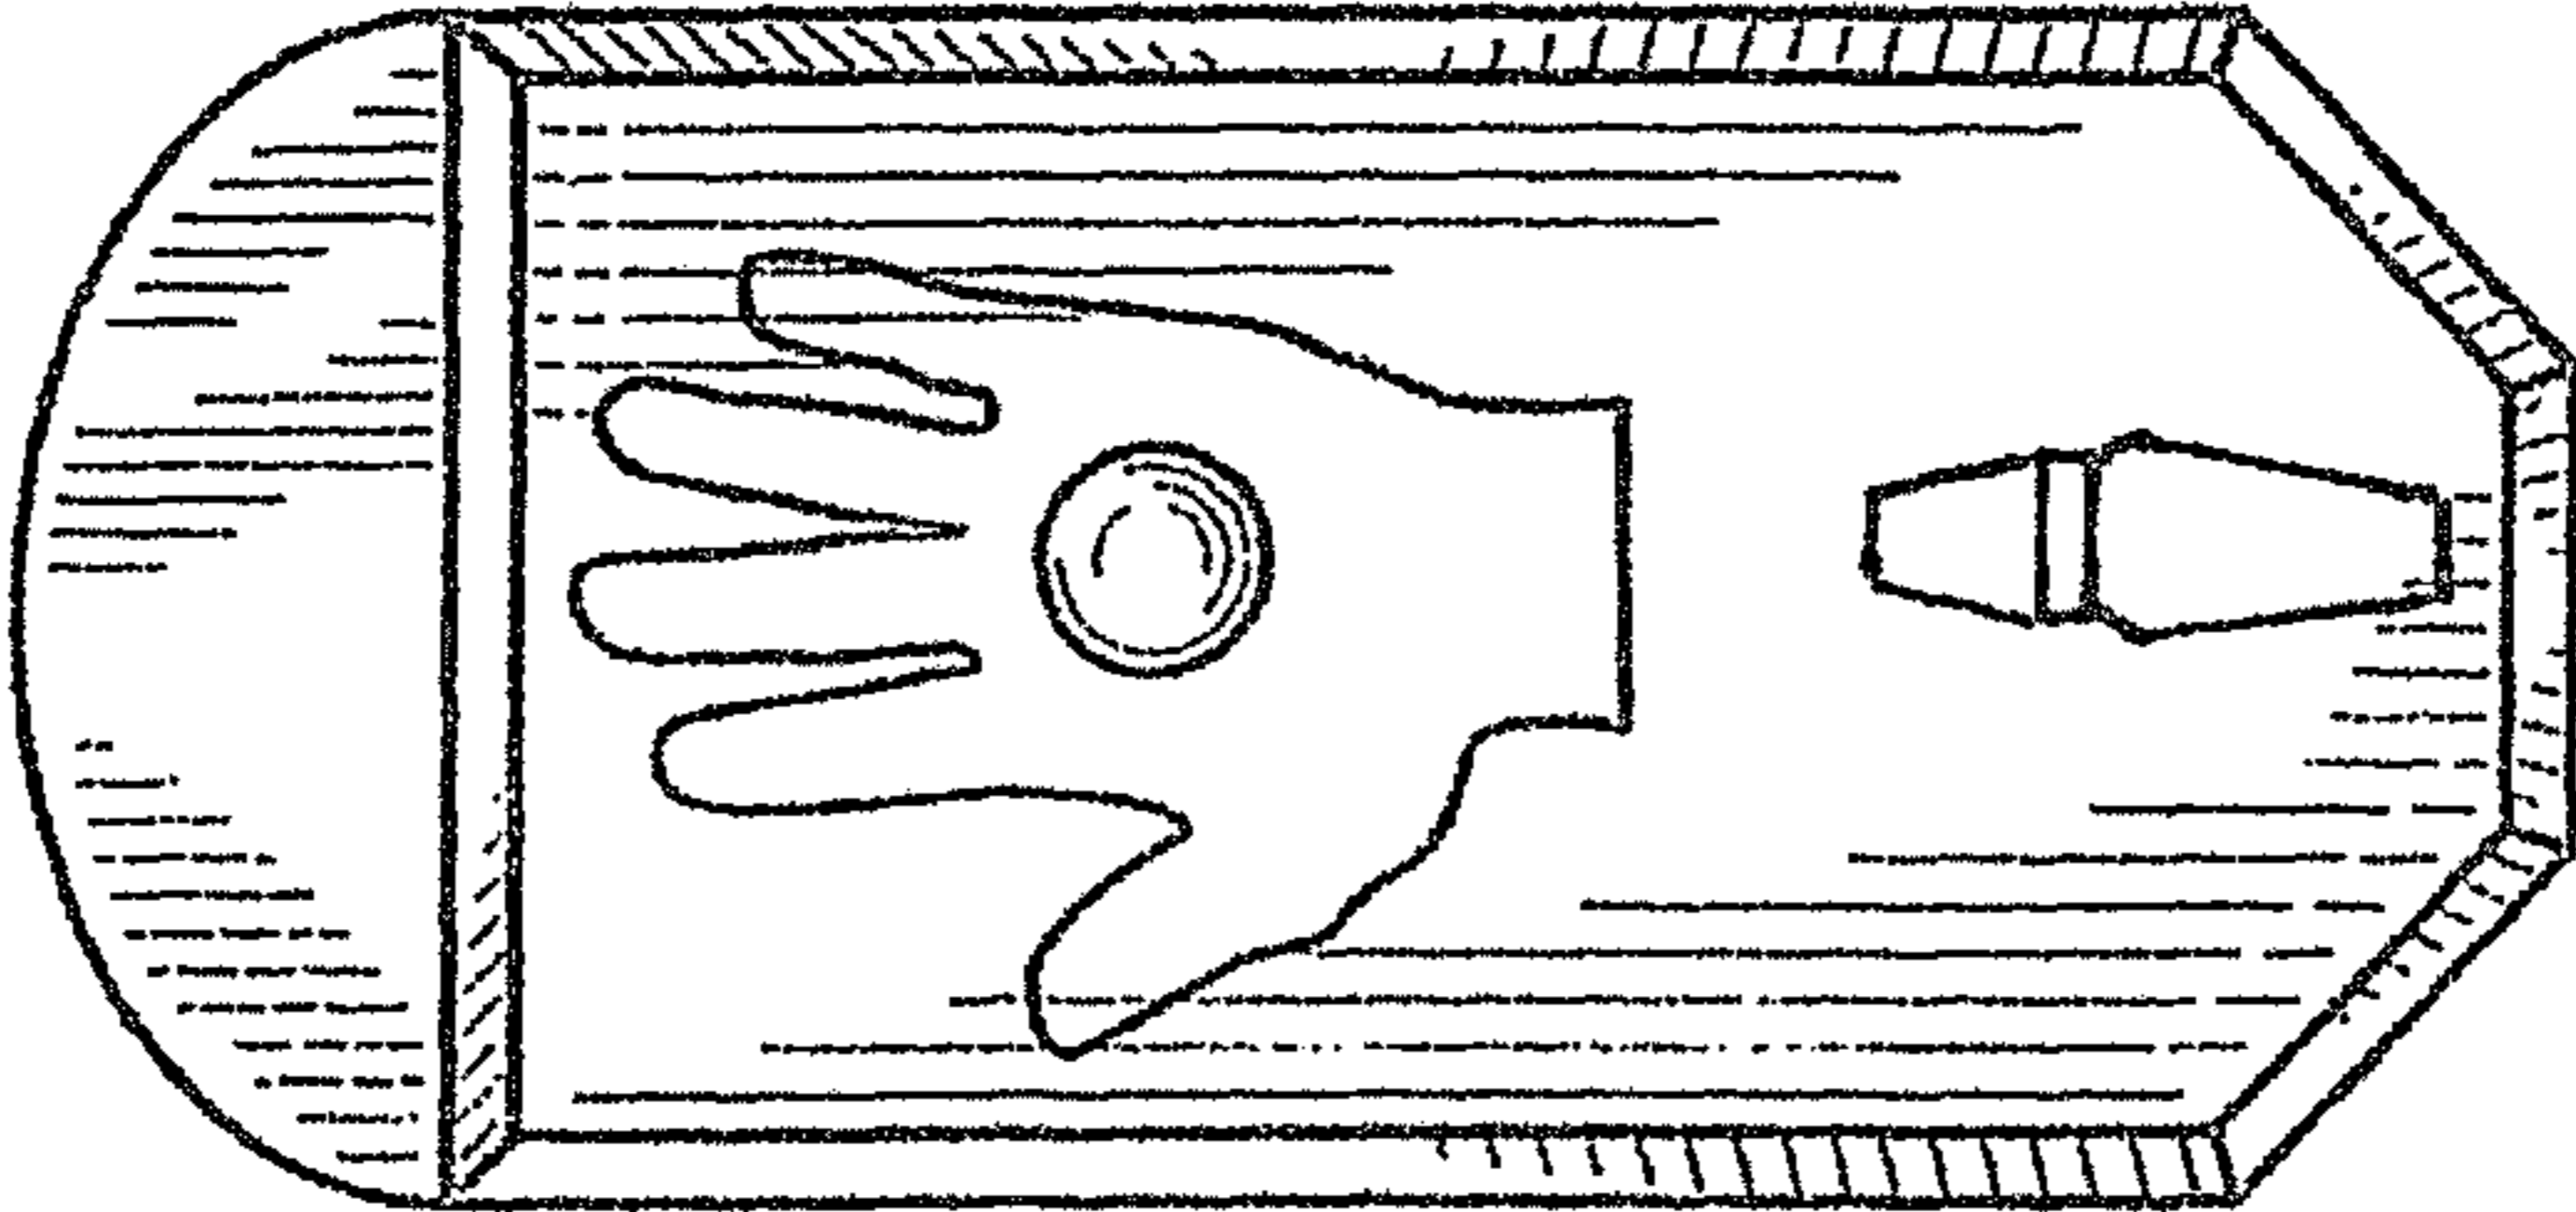


FIG. 5



FIG. 6

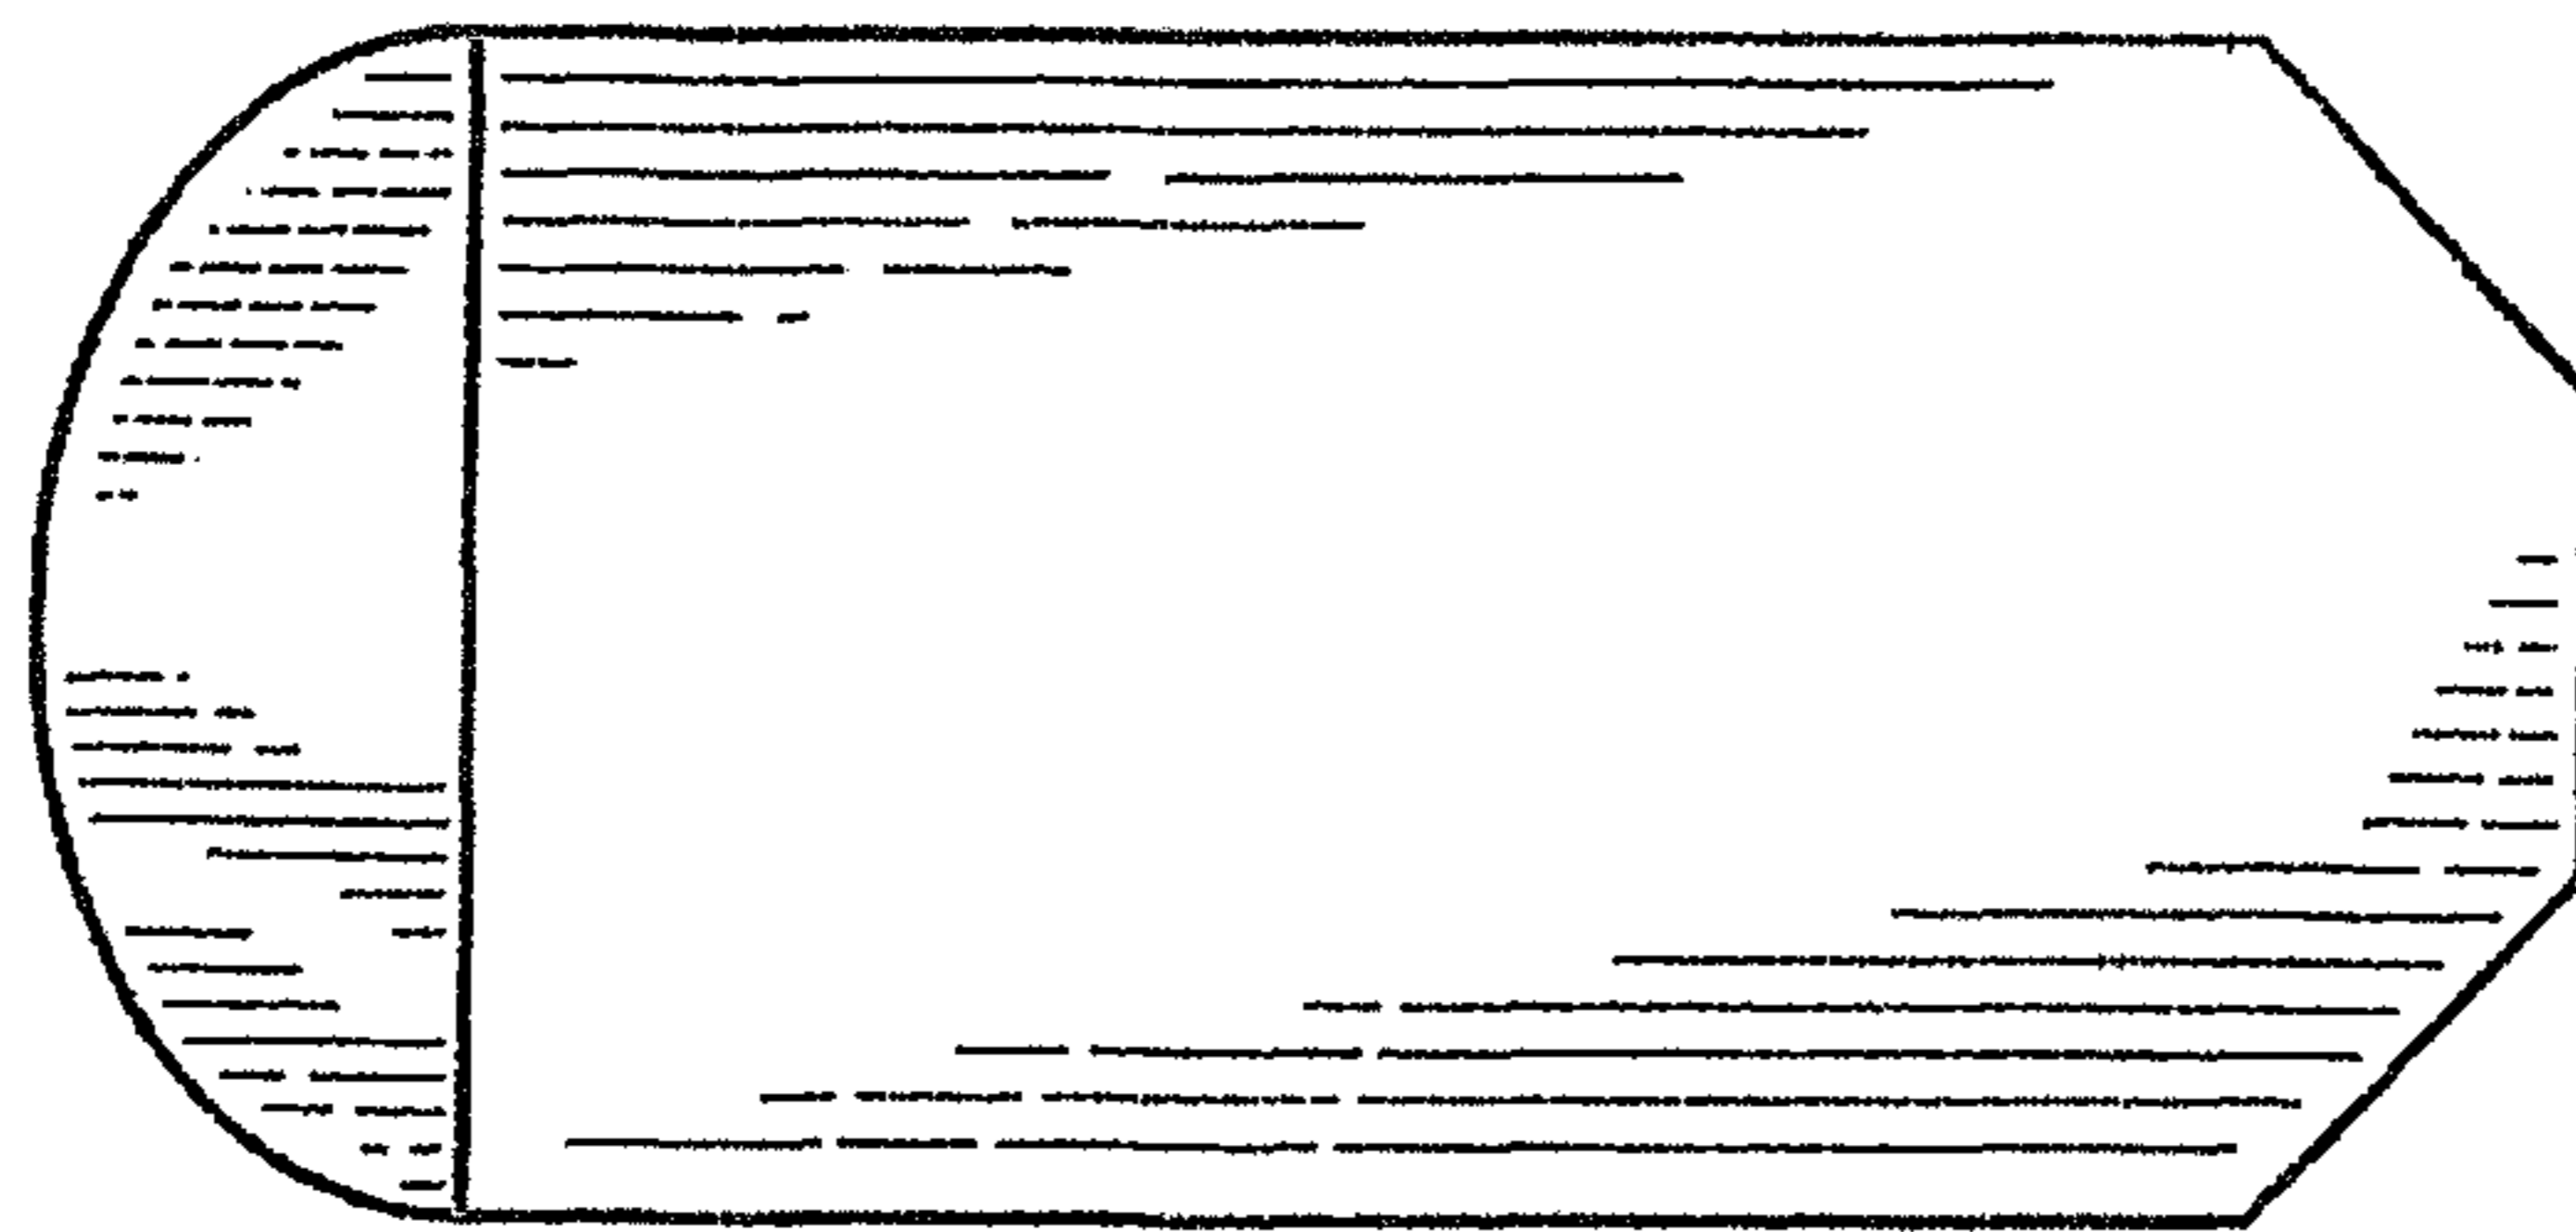


FIG. 7