



US00D974565S

(12) **United States Design Patent** (10) **Patent No.:** **US D974,565 S**
Li (45) **Date of Patent:** **** Jan. 3, 2023**

(54) **PULSE OXIMETER**

(71) Applicant: **Guangdong Health Tree Medical Technology Co., Ltd., Guangdong (CN)**

(72) Inventor: **Dong Li, Guangdong (CN)**

(**) Term: **15 Years**

(21) Appl. No.: **29/824,514**

(22) Filed: **Jan. 25, 2022**

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/169; D24/167**

(58) **Field of Classification Search**
USPC D24/186, 188–191, 169, 200, 214, 215, D24/107, 164–168, 185, 187; D14/218
CPC A61N 1/04; A61N 1/0404; A61N 1/06; A61N 1/36; A61N 1/36003; A61N 1/36014; A61N 1/36021; A61N 1/36057; A61N 1/36071; A61N 5/0616; A61N 5/062; A61N 5/0613; A61N 1/36017; A61N 1/36128; A61N 1/37247; A61N 1/0456
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D281,724 S	*	12/1985	Michiels	D13/110
D352,463 S	*	11/1994	Kubo	D10/2
D393,313 S	*	4/1998	Meisner	D24/169
D401,696 S	*	11/1998	Kuo	D24/200
D412,364 S	*	7/1999	Agarwala	D24/200
D414,870 S	*	10/1999	Saltzstein	D24/186
D484,600 S	*	12/2003	Kaar	D24/169
D502,655 S	*	3/2005	Huang	D10/81
D503,641 S	*	4/2005	Huang	D10/81
D535,031 S	*	1/2007	Barrett	D24/186
D547,454 S	*	7/2007	Hsieh	D24/186
D582,043 S	*	12/2008	Koike	D24/165
D601,256 S	*	9/2009	Takano	D24/169
D621,048 S	*	8/2010	Severe	D24/167

D621,515 S	*	8/2010	Chua	D24/186
D634,430 S	*	3/2011	Osiecki	D24/165
D634,431 S	*	3/2011	Severe	D24/167
D641,880 S	*	7/2011	Noguchi	D24/165
D659,836 S	*	5/2012	Bensch	D24/167
D670,810 S	*	11/2012	Fukuzawa	D24/169
D670,811 S	*	11/2012	Fukuzawa	D24/169

(Continued)

FOREIGN PATENT DOCUMENTS

CN 304876080 * 11/2018

OTHER PUBLICATIONS

Lepu Overnight Pulse Oximeter, [site visited Aug. 11, 2022]. Available from Internet. URL: <https://www.lepucreative.com/products/lepu-digital-portable-handheld-overnight-pulse-oximeter-sp-20-for-infant-kid-toddler-adult-android-iphone-with-...> (Year: 2022).*

Primary Examiner — T Chase Nelson
Assistant Examiner — Kelly L Gross
(74) *Attorney, Agent, or Firm* — Che-Yang Chen; Law Office of Michael Chen


(57) **CLAIM**

The ornamental design for a pulse oximeter, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the pulse oximeter showing my new design;
FIG. 2 is a perspective view thereof from another angle;
FIG. 3 is a front elevational view thereof;
FIG. 4 is a rear elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a right side elevational view thereof;
FIG. 7 is a top plan view thereof; and,
FIG. 8 is a bottom plan view thereof.
The broken lines in the drawings show portions of the pulse oximeter that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

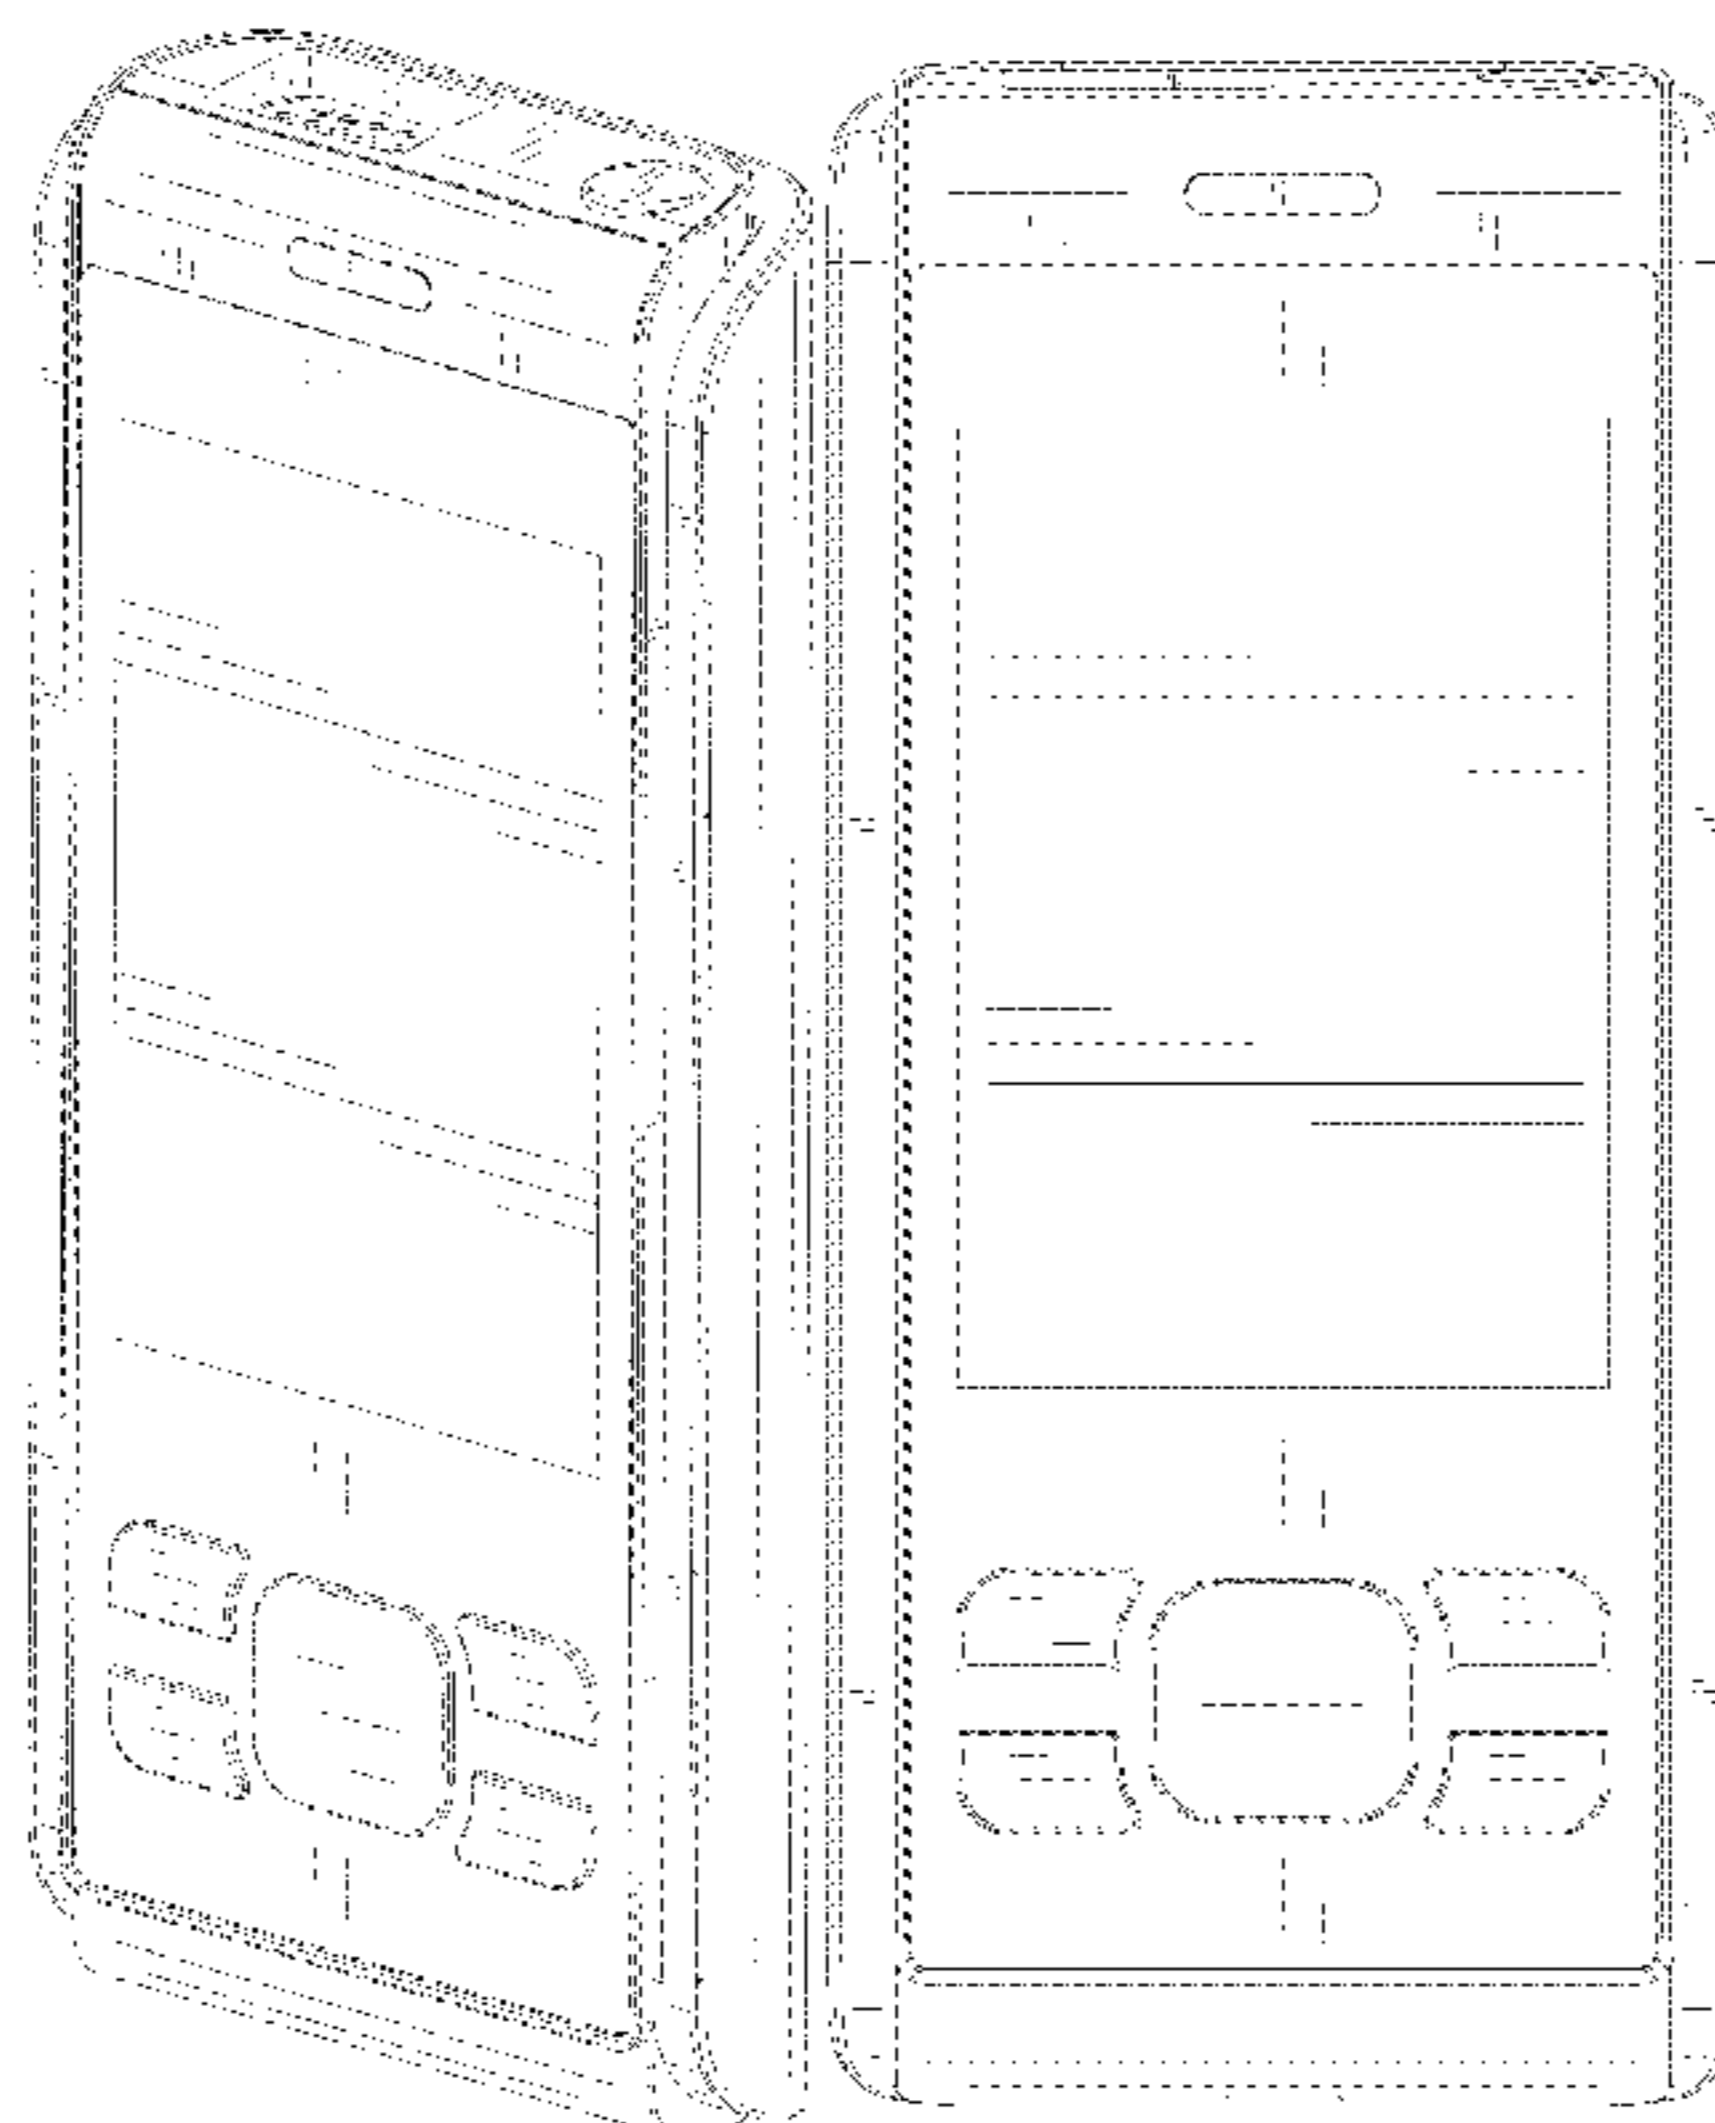

(56)

References Cited

U.S. PATENT DOCUMENTS

D686,731 S *	7/2013	Oka	D24/169	D794,802 S *	8/2017	Binier	D24/169
D690,422 S *	9/2013	Oka	D24/169	D800,313 S *	10/2017	Chang	D24/167
D696,404 S *	12/2013	Golnik	D24/169	D802,780 S *	11/2017	Hsu	D24/200
D696,405 S *	12/2013	Koski	D24/169	D811,597 S *	2/2018	Verbrugge	D24/165
D713,963 S *	9/2014	Liedtke	D24/169	D812,229 S *	3/2018	Al-Siddiq	D24/167
D719,263 S *	12/2014	Shibata	D24/165	D815,743 S *	4/2018	Liao	D24/165
D721,177 S *	1/2015	Ahlstrom	D24/169	D836,789 S *	12/2018	Jiang	D24/200
D731,067 S *	6/2015	Huang	D24/169	D849,950 S *	5/2019	Nishiyama	D24/165
D739,945 S *	9/2015	Cadio	D24/169	D851,253 S *	6/2019	Goolkasian	D24/167
D741,497 S *	10/2015	Aber	D24/186	D858,464 S *	9/2019	Li	D13/168
D747,489 S *	1/2016	Ahlstrom	D24/169	D874,007 S *	1/2020	Chang	D24/169
D752,229 S *	3/2016	Chen	D24/165	D884,903 S *	5/2020	Cadio	D24/169
D757,273 S *	5/2016	Nelson	D24/169	D890,346 S *	7/2020	Lam	D24/167
D758,606 S *	6/2016	Chen	D24/215	D893,728 S *	8/2020	Zhao et al.	D24/200
D759,262 S *	6/2016	Chen	D24/215	D893,735 S *	8/2020	Yin	D24/200
D759,263 S *	6/2016	Chen	D24/215	D893,736 S *	8/2020	Yin	D24/200
D762,872 S *	8/2016	Chen	D24/215	D922,582 S *	6/2021	Peng	D24/200
D778,445 S *	2/2017	Cadio	D24/169	D932,637 S *	10/2021	Hsu	D24/200
D779,677 S *	2/2017	Chen	D24/215	D933,234 S *	10/2021	Al-Ali	D24/165
					D936,850 S *	11/2021	Chen	D24/200
					D954,281 S *	6/2022	Hsu	D24/200

* cited by examiner

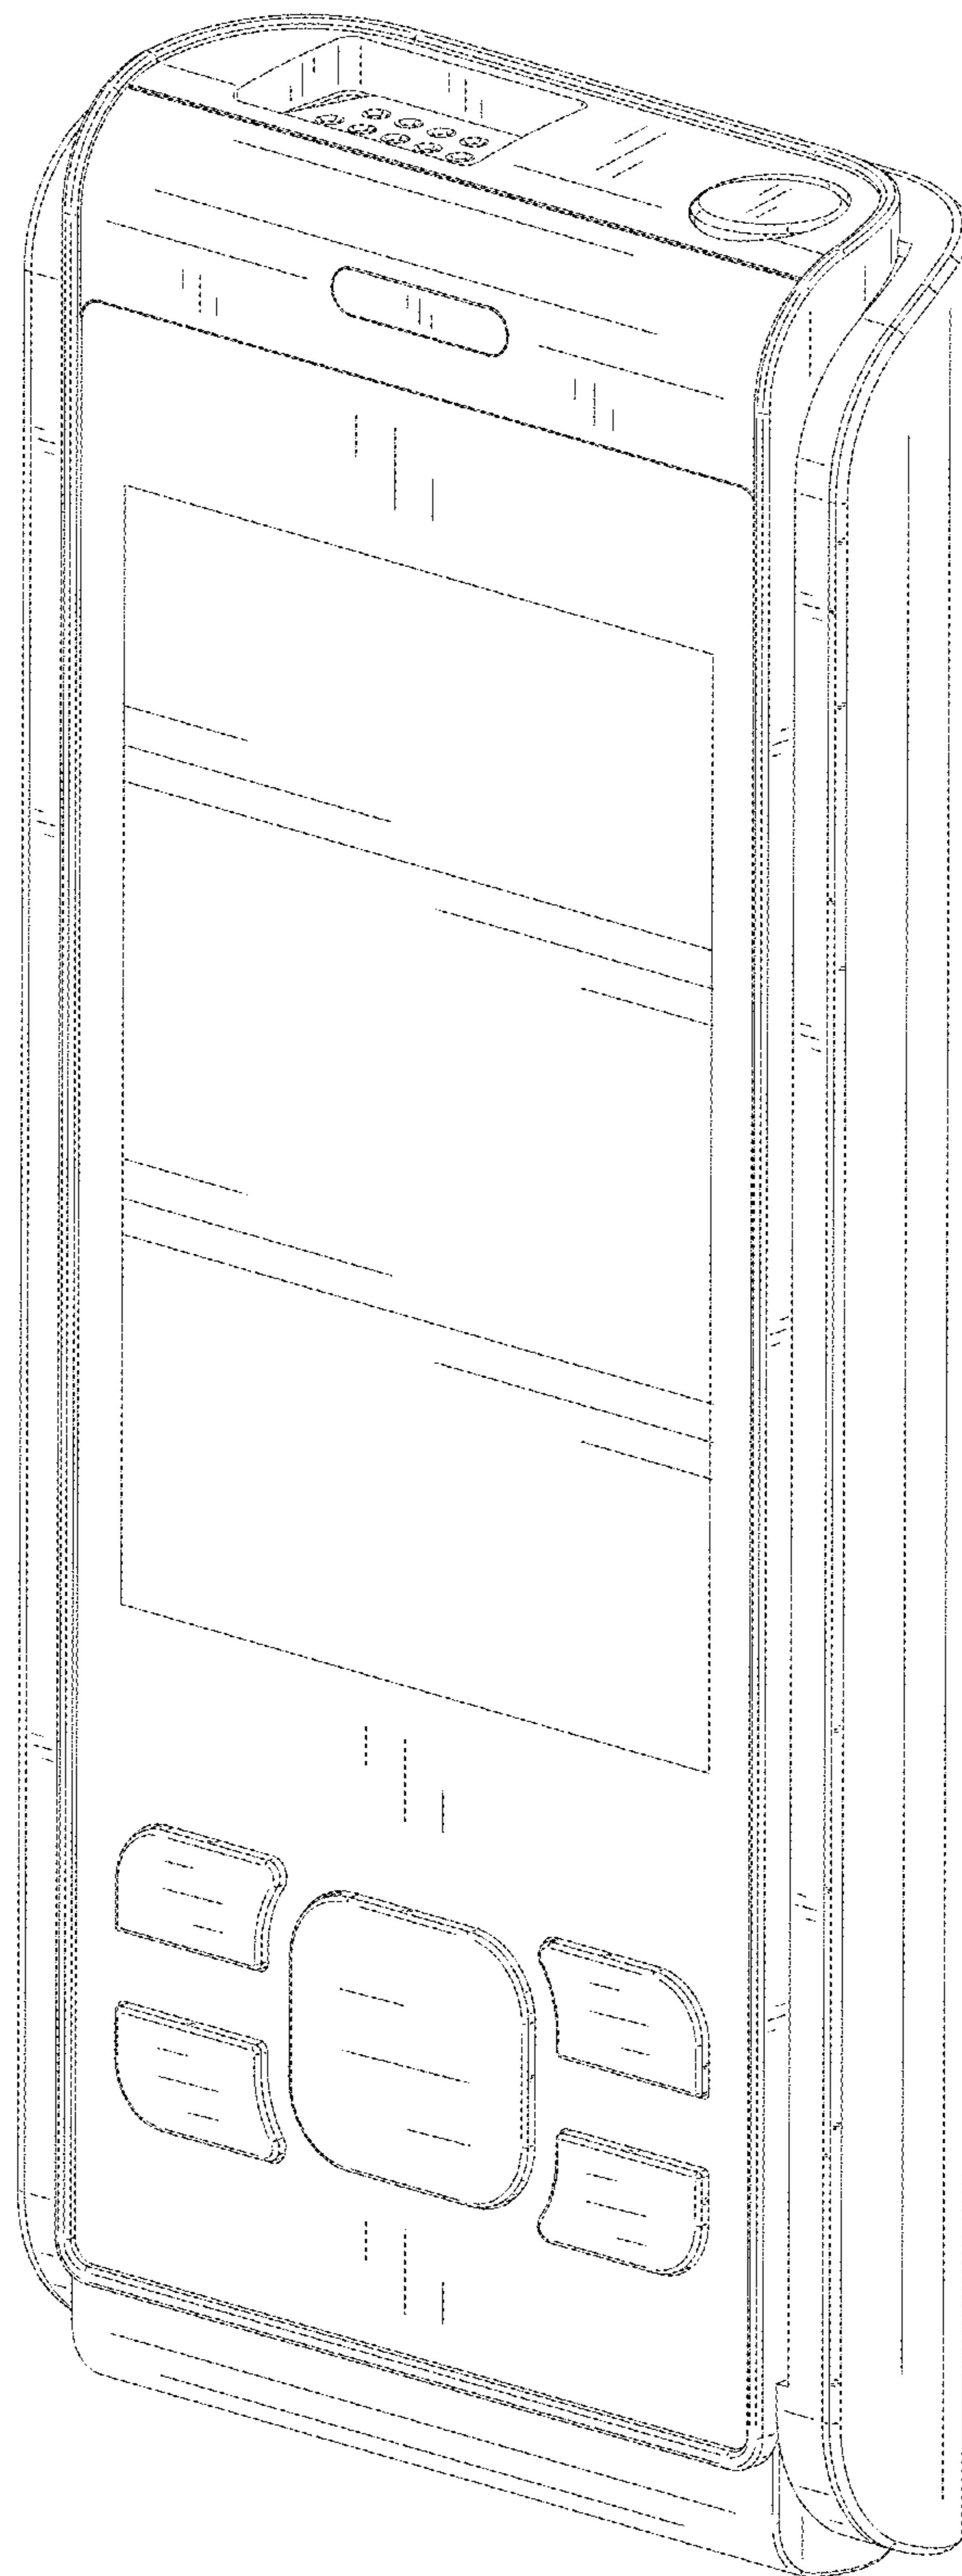


FIG. 1

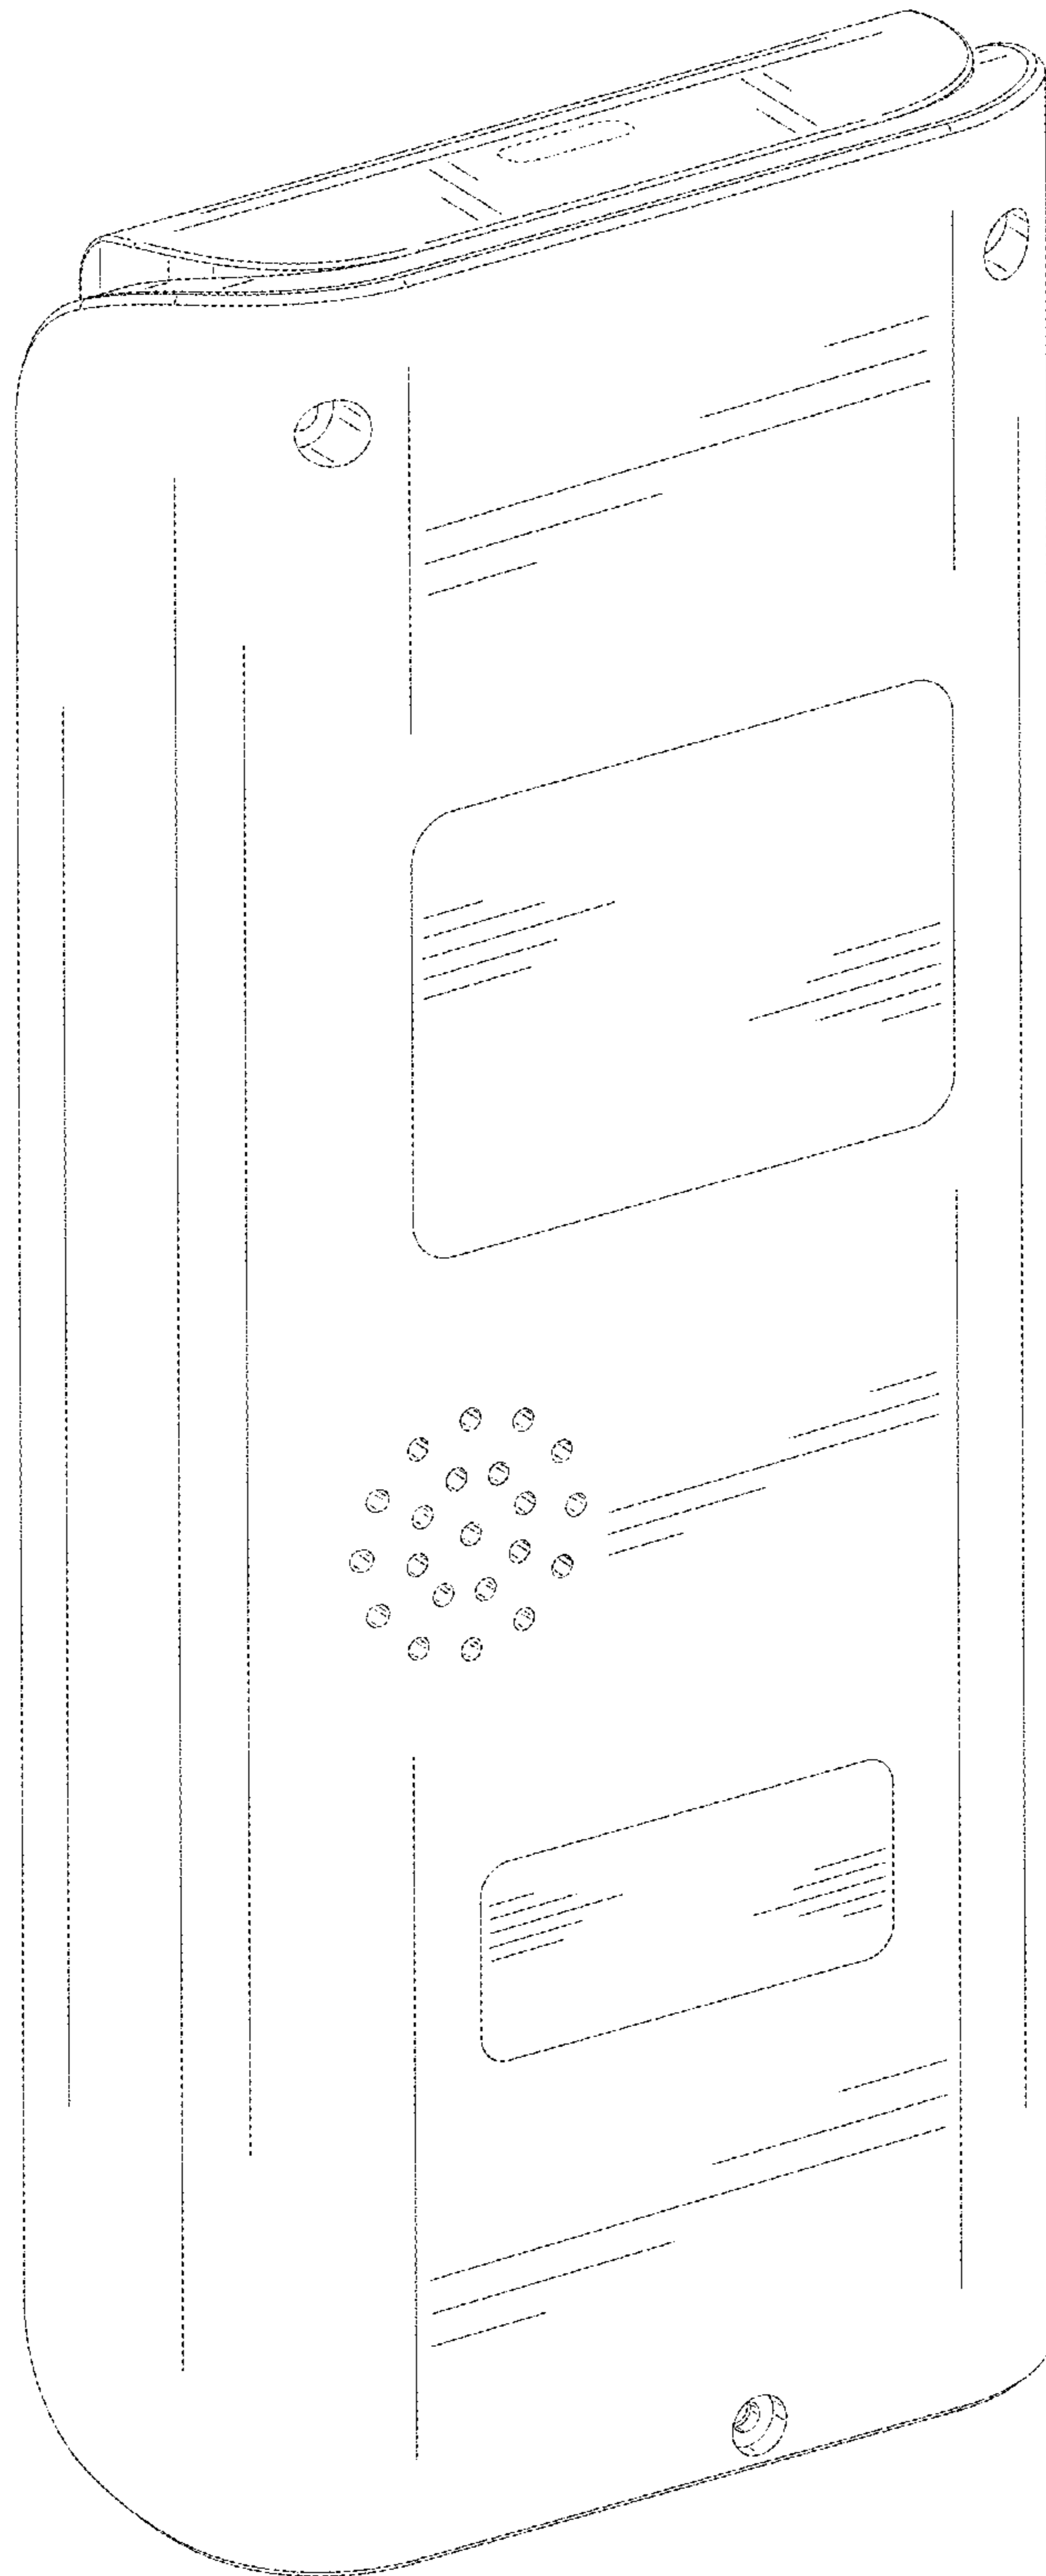


FIG. 2

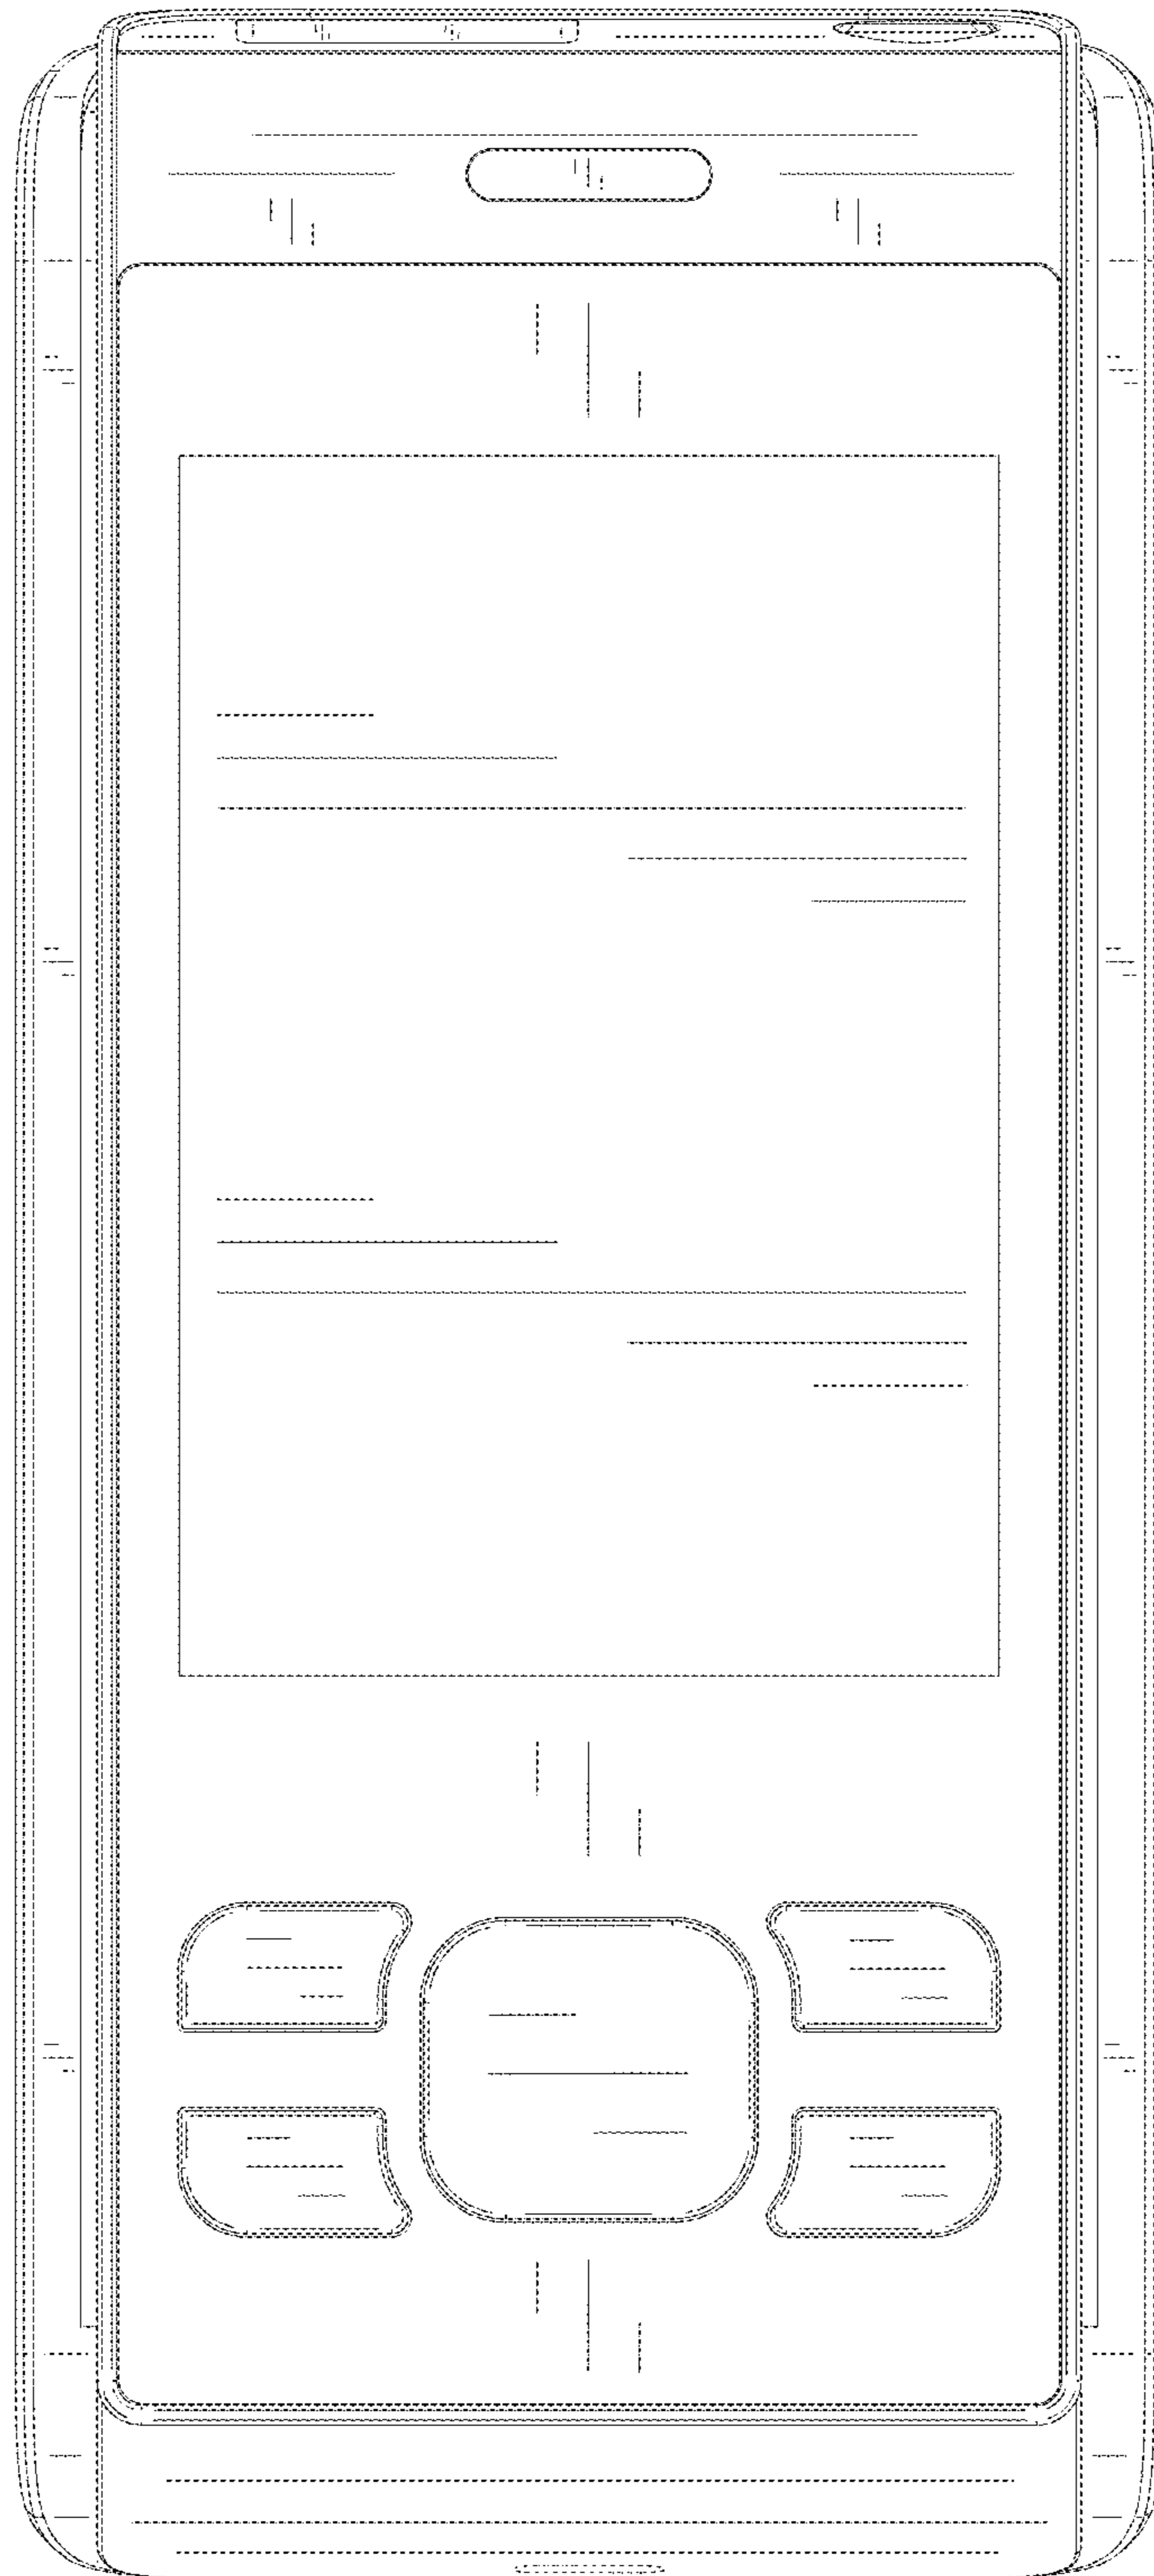


FIG. 3

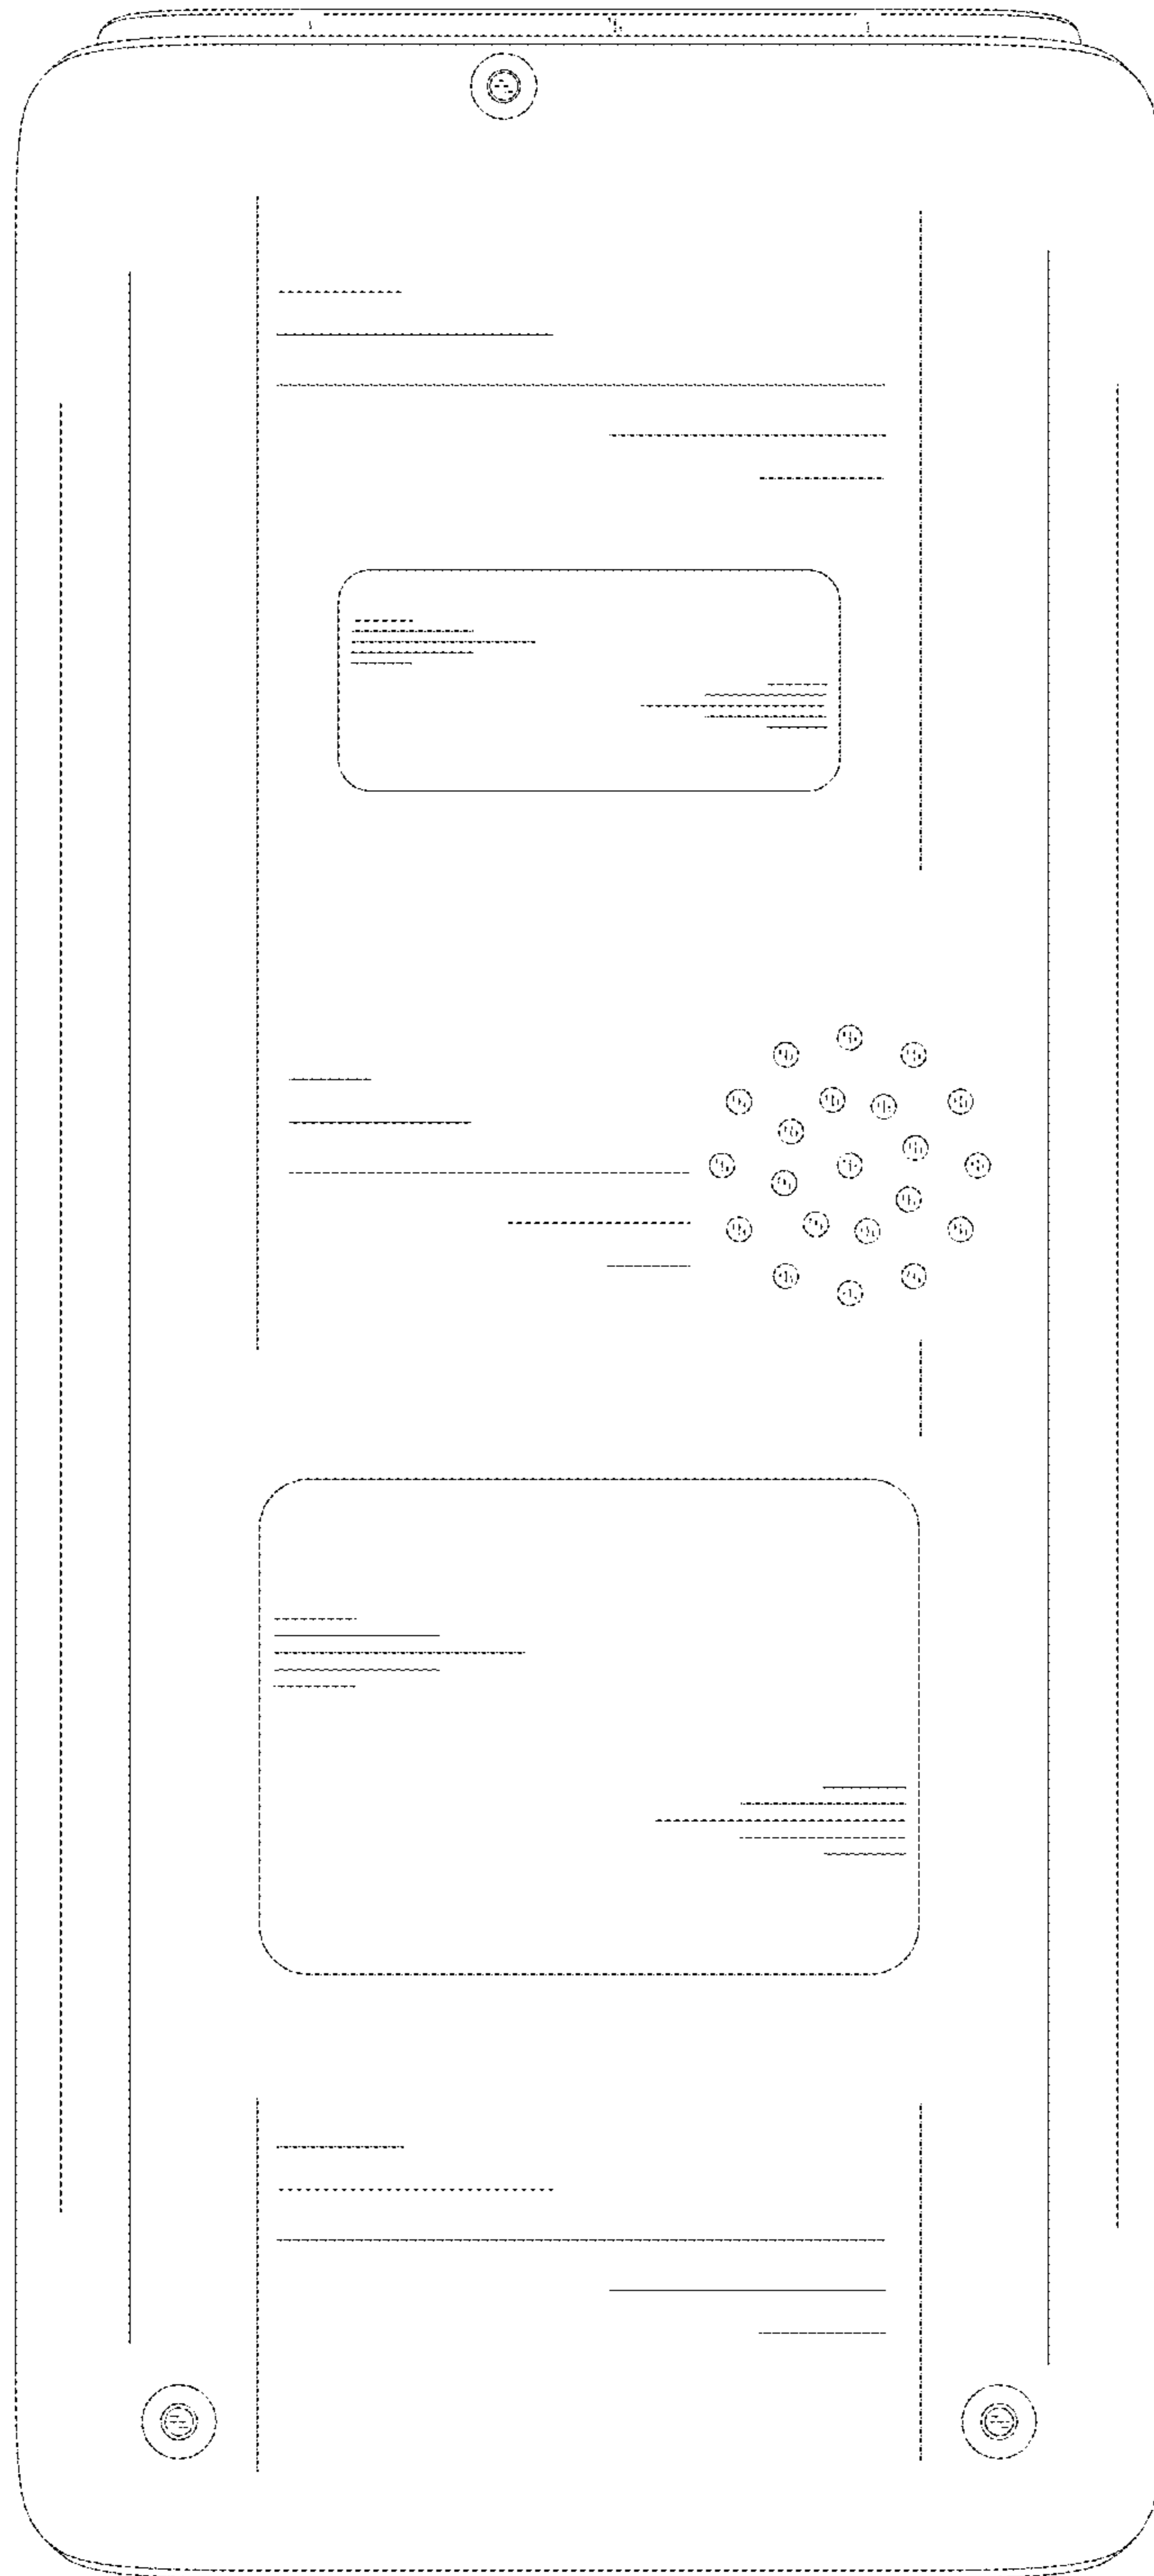


FIG. 4

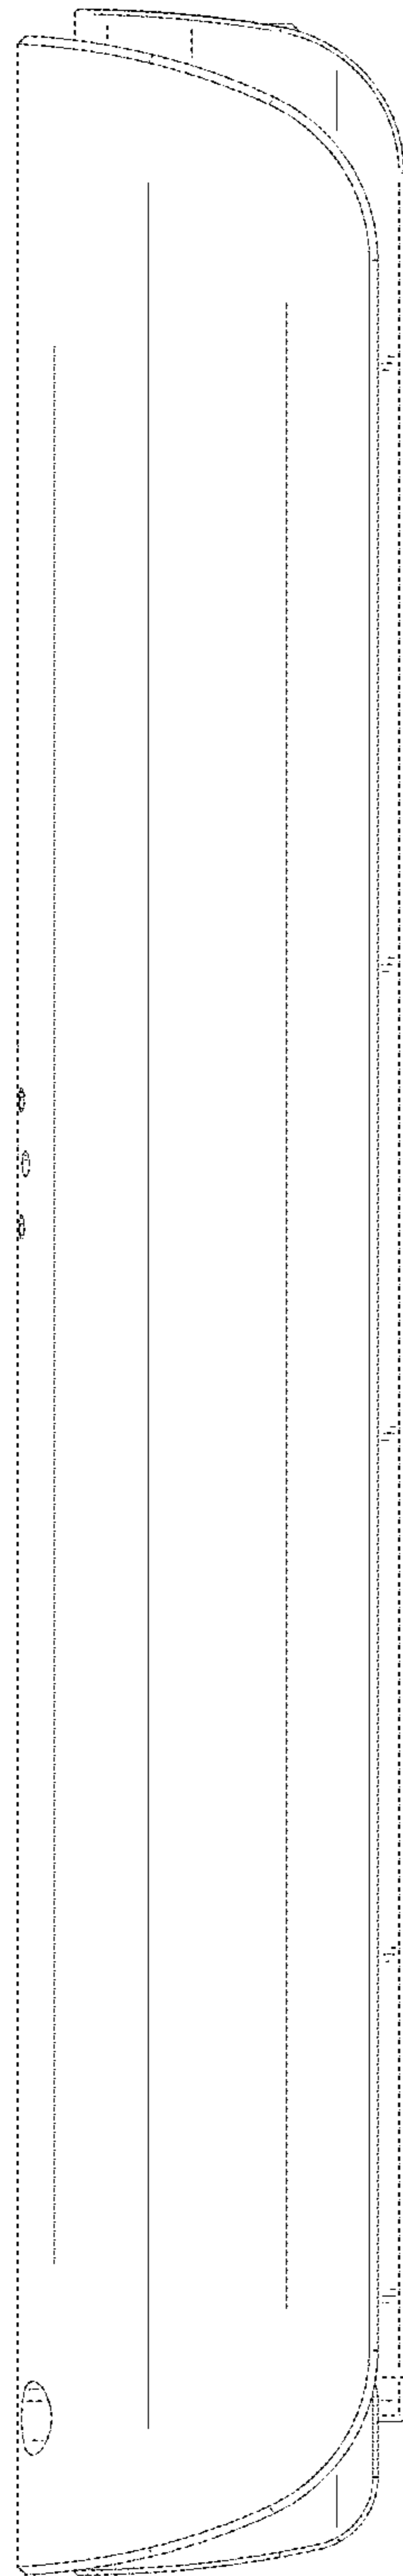


FIG. 5

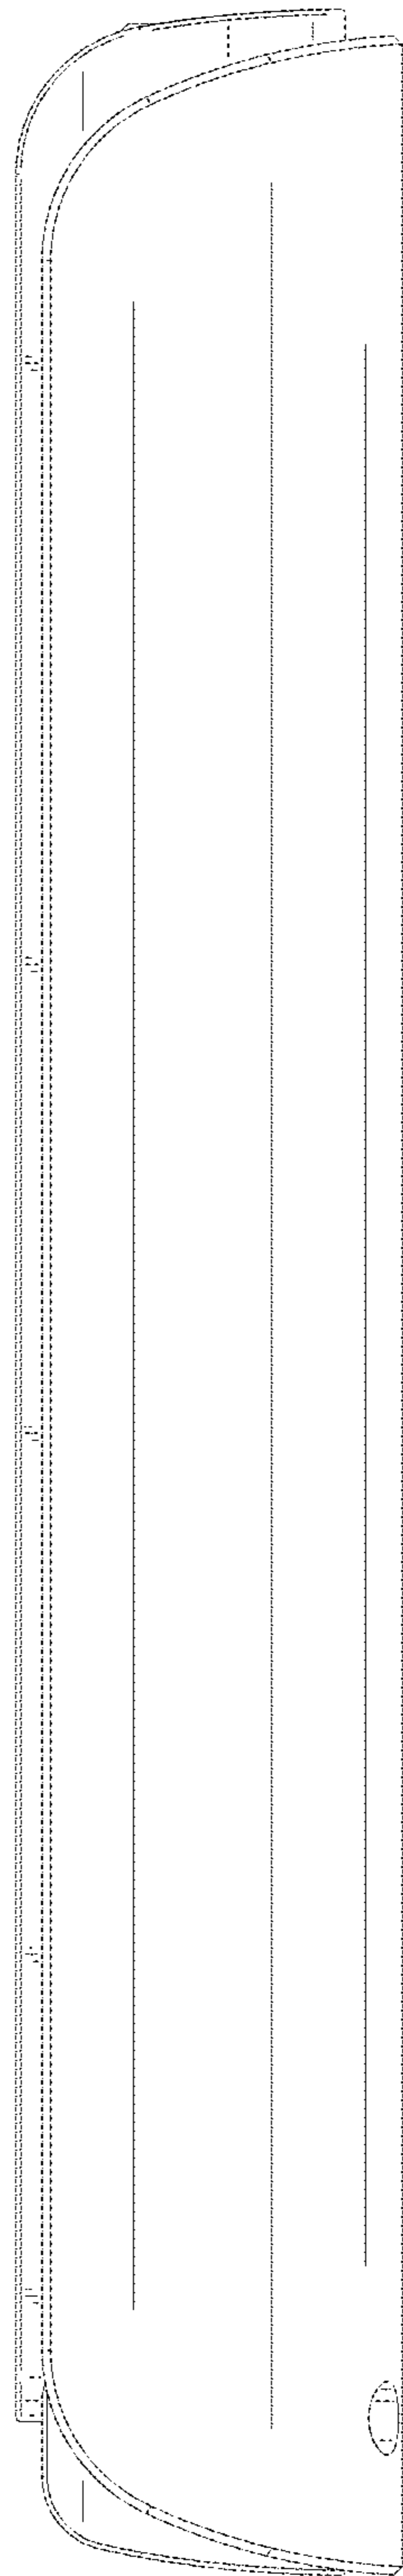


FIG. 6

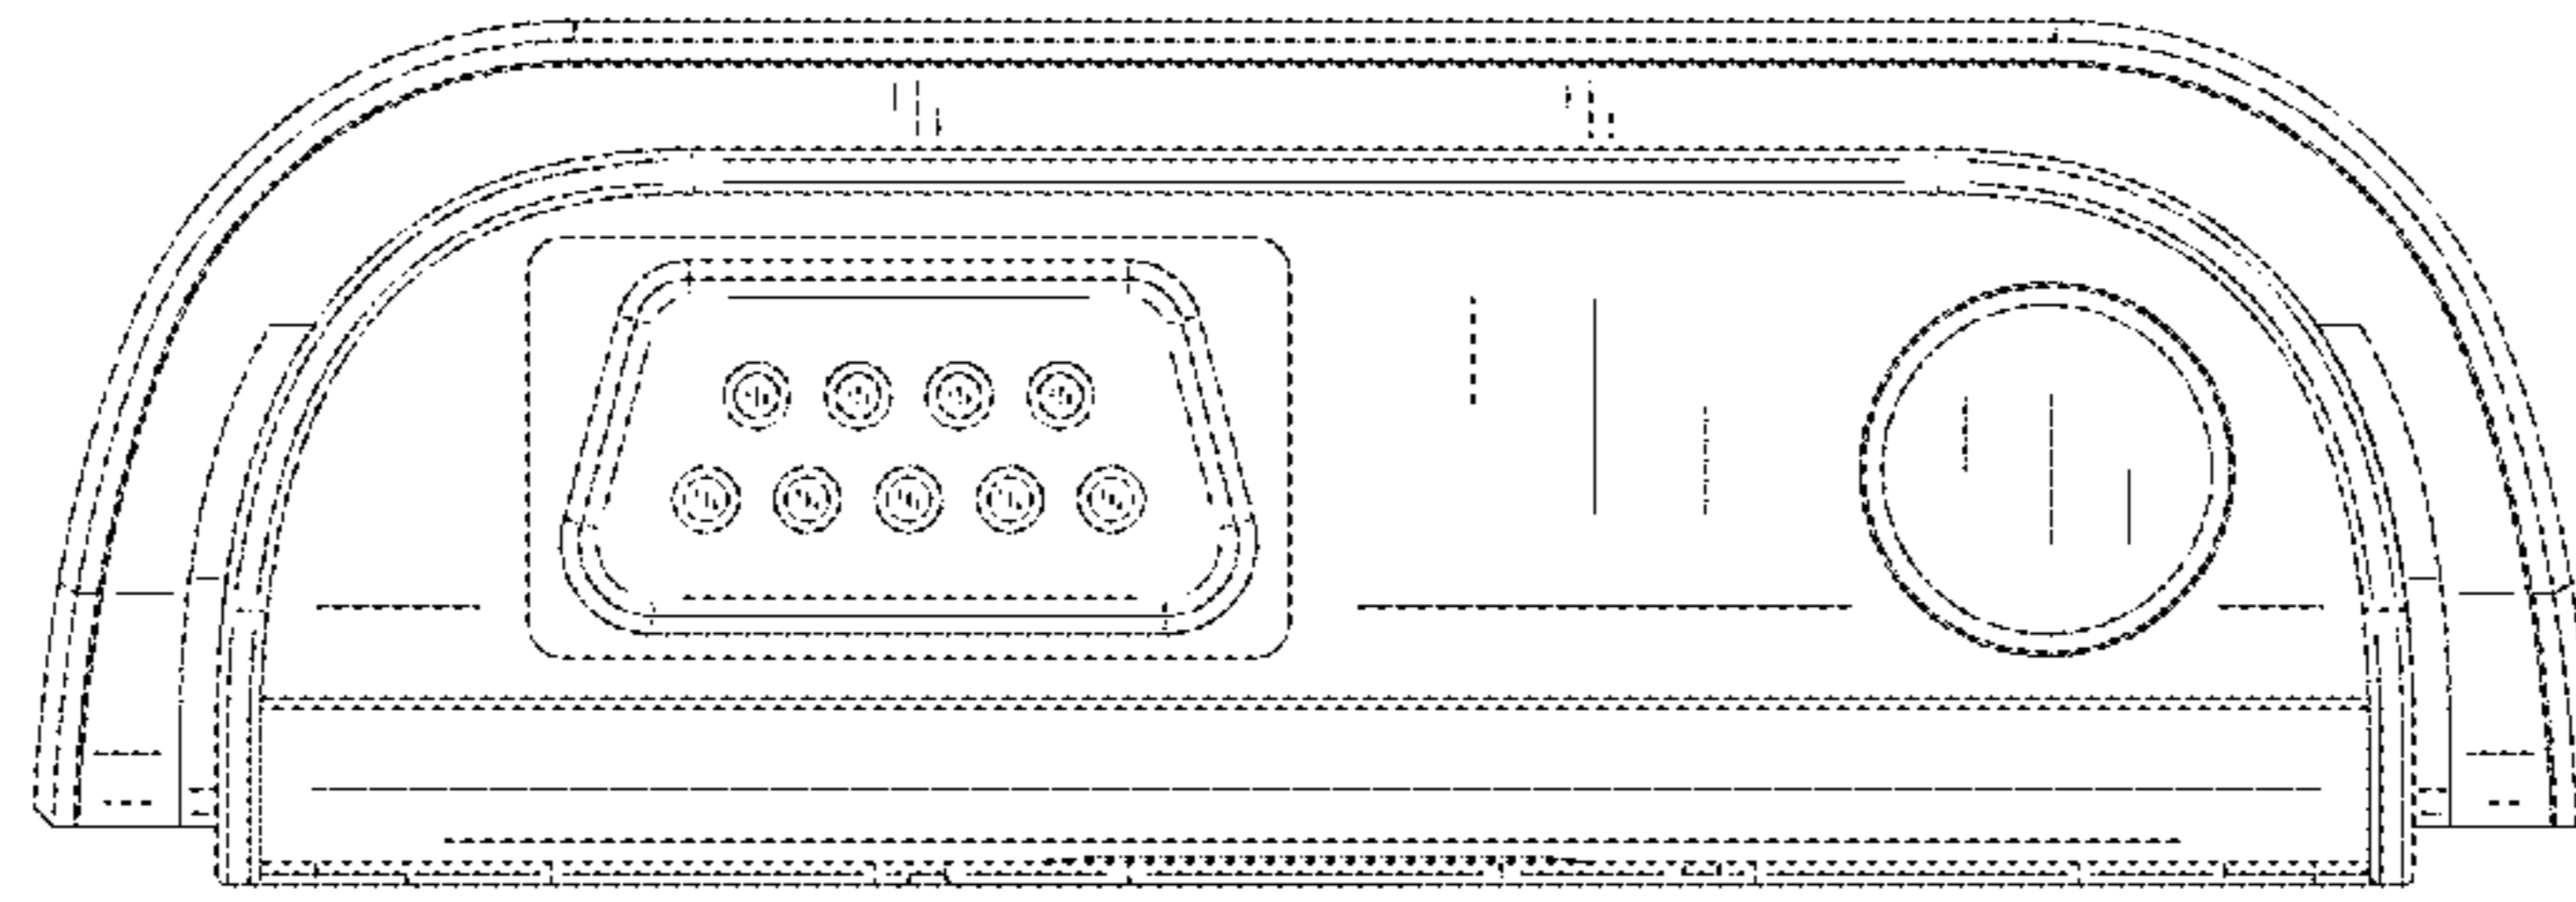


FIG. 7

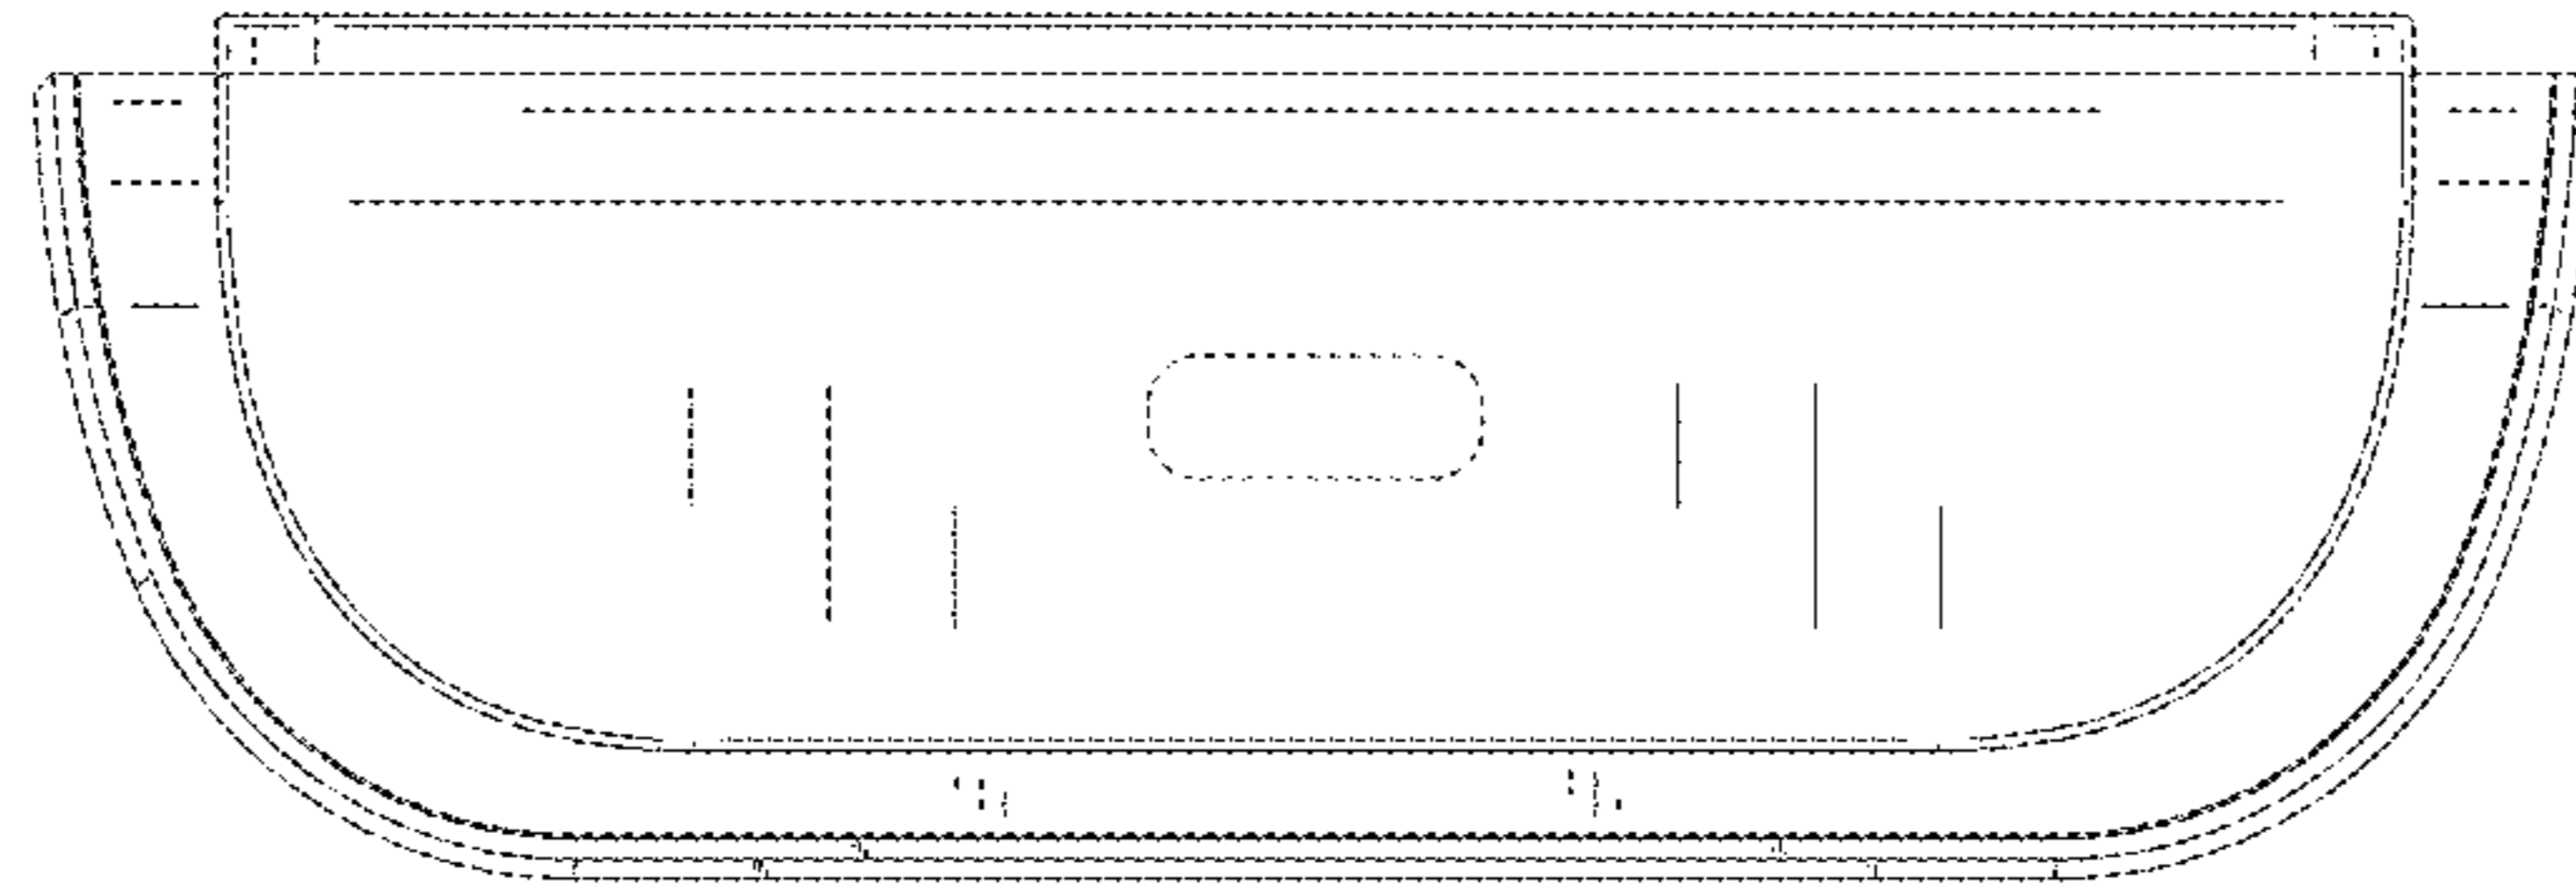


FIG. 8