



US00D975288S

(12) **United States Design Patent**
Zimmermann

(10) **Patent No.:** **US D975,288 S**

(45) **Date of Patent:** **** Jan. 10, 2023**

(54) **MEDICAL DEVICE FOR FETAL MONITORING**

(71) Applicant: **VIEWCARE TECHNOLOGIES 1 APS, Soborg (DK)**

(72) Inventor: **Henrik Zimmermann, Aarhus (DK)**

(73) Assignee: **VIEWCARE TECHNOLOGIES 1 APS, Soborg (DK)**

(**) Term: **15 Years**

(21) Appl. No.: **29/836,375**

(22) Filed: **Apr. 26, 2022**

Related U.S. Application Data

(62) Division of application No. 35/509,946, filed on Jan. 27, 2020 (U.S. filing date under 35 U.S.C. 384), and having an international filing date of Jan. 27, 2020, now Pat. No. Des. 953,543.

(51) **LOC (14) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/130, 200, 206, 215, 133, 186, 193, D24/107, 158, 187, 188–192; D29/100, D29/108, 120.1, 121.1, 121.2; D30/146
CPC .. A61B 5/02438; A61B 5/6823; A61B 5/0006
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D418,606 S	1/2000	Davis
D442,269 S	5/2001	Pinchuk
D455,481 S	4/2002	Christianson
D578,221 S	10/2008	Sakurai
D600,352 S	9/2009	Cryan

D690,019 S	9/2013	Nichola	
D699,858 S *	2/2014	Neumann D24/215
D717,956 S	11/2014	Alexander	
D771,820 S	11/2016	Haye	
D775,361 S *	12/2016	Vosch D24/187

(Continued)

OTHER PUBLICATIONS

Jordemoder Foreningen. The sound of a good invention by Connie Mikkelsen. 2021. <https://jordemoderforeningen.dk/nyhed/artikel/lyden-af-en-god-opfindelse/> (Year: 2021).*

(Continued)

Primary Examiner — Darcey E Gottschalk
(74) *Attorney, Agent, or Firm* — Moser Taboada


(57) **CLAIM**

The ornamental design for a medical device for fetal monitoring, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical device for fetal monitoring.
FIG. 2 is a front view of the medical device for fetal monitoring.
FIG. 3 is a rear view of the medical device for fetal monitoring.
FIG. 4 is top view of the medical device for fetal monitoring.
FIG. 5 is a bottom view of the medical device for fetal monitoring.
FIG. 6 is a right side view of the medical device for fetal monitoring; and,
FIG. 7 is a left side view of the medical device for fetal monitoring.
The broken lines shown in one or more of the figures are for the purpose of illustrating portions of the medical device for fetal monitoring and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

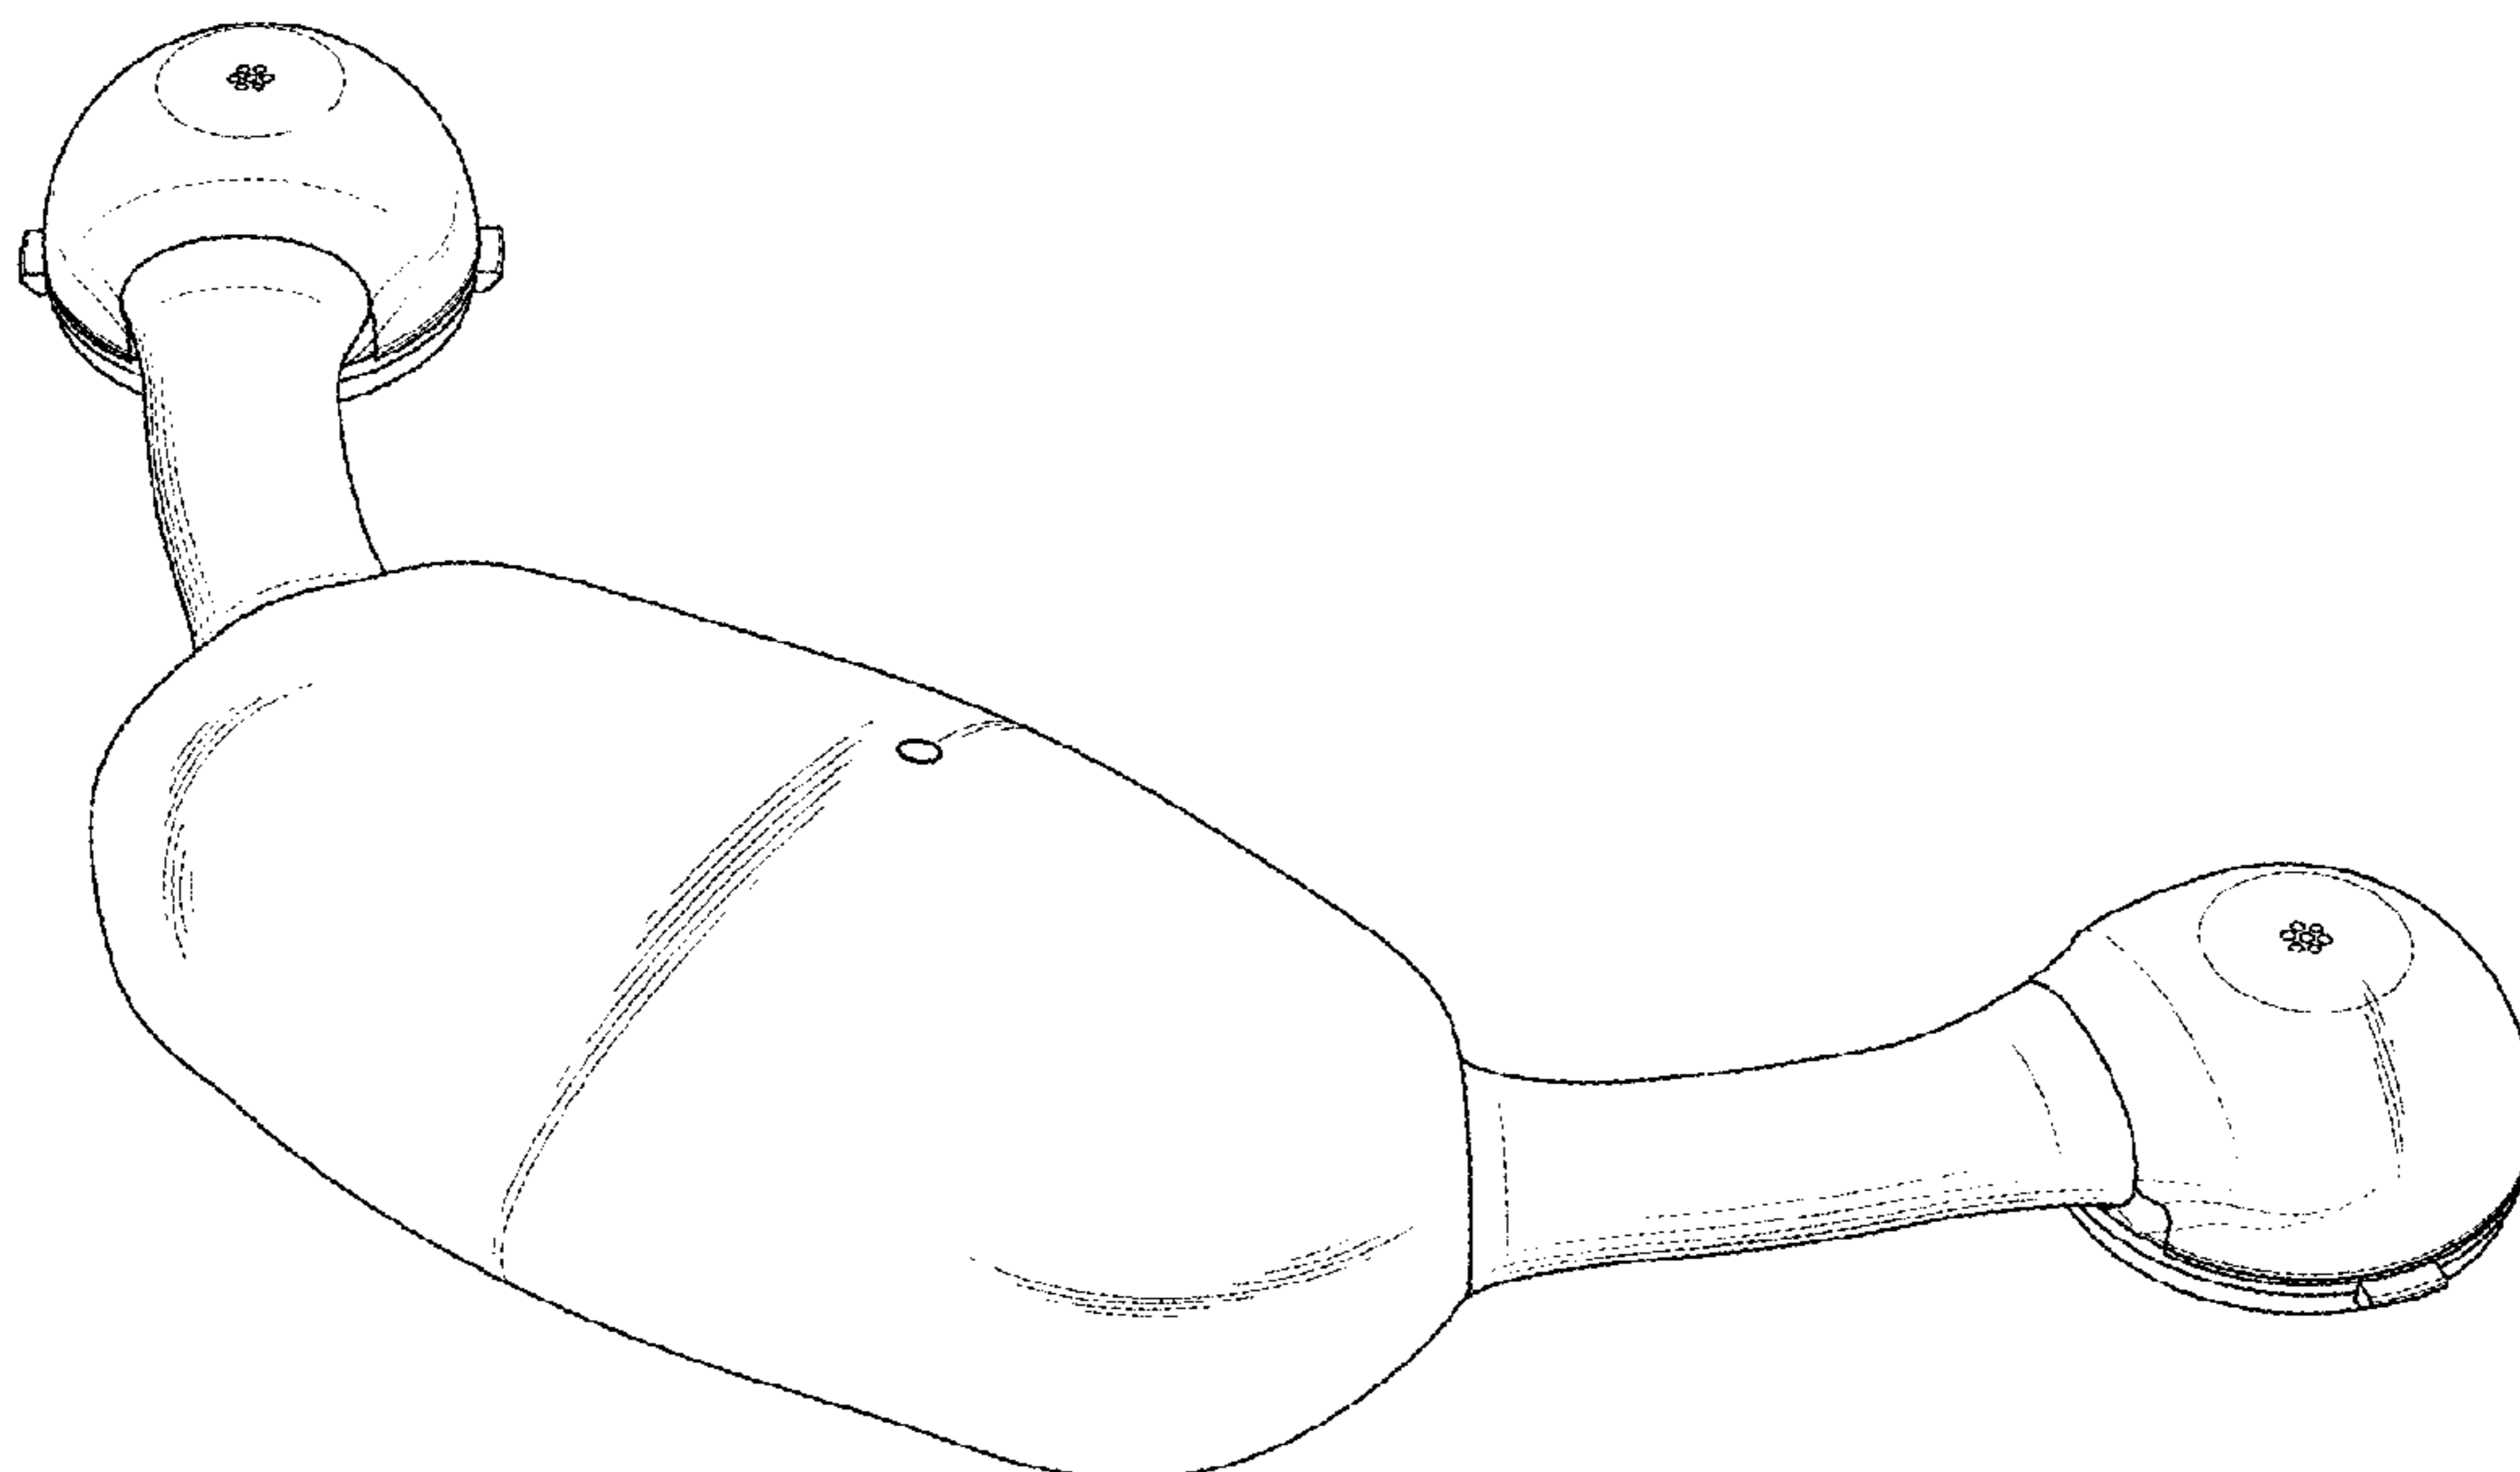

(56)

References Cited

U.S. PATENT DOCUMENTS

D796,683 S 9/2017 Smeros
D823,470 S 7/2018 Neubauer
D925,744 S 7/2021 Yeip
D932,639 S * 10/2021 McDonough D24/187
D953,543 S * 5/2022 Zimmermann D24/187
D961,789 S * 8/2022 Ding D23/370
2018/0199883 A1 7/2018 Banet

OTHER PUBLICATIONS

Aalborg University. Biosensor Creates a Breakthrough in Pregnancy and Birth Monitoring. Feb. 2, 2021. <https://www.en.aau.dk/cooperation/how-to-cooperate/inventions-technology/examples/Successful+inventions/biosensor-creates-a-breakthrough-in-pregnancy-and-birth-monitoring.cid499500> (Year: 2021).*

Japan Gov. Handy Fetal Monitor Brings Peace of Mind to Mothers, 2020, https://www.japan.go.jp/tomodachi/2020/summer2020/handy_fetal_monitor.htm (Year: 2020).

* cited by examiner

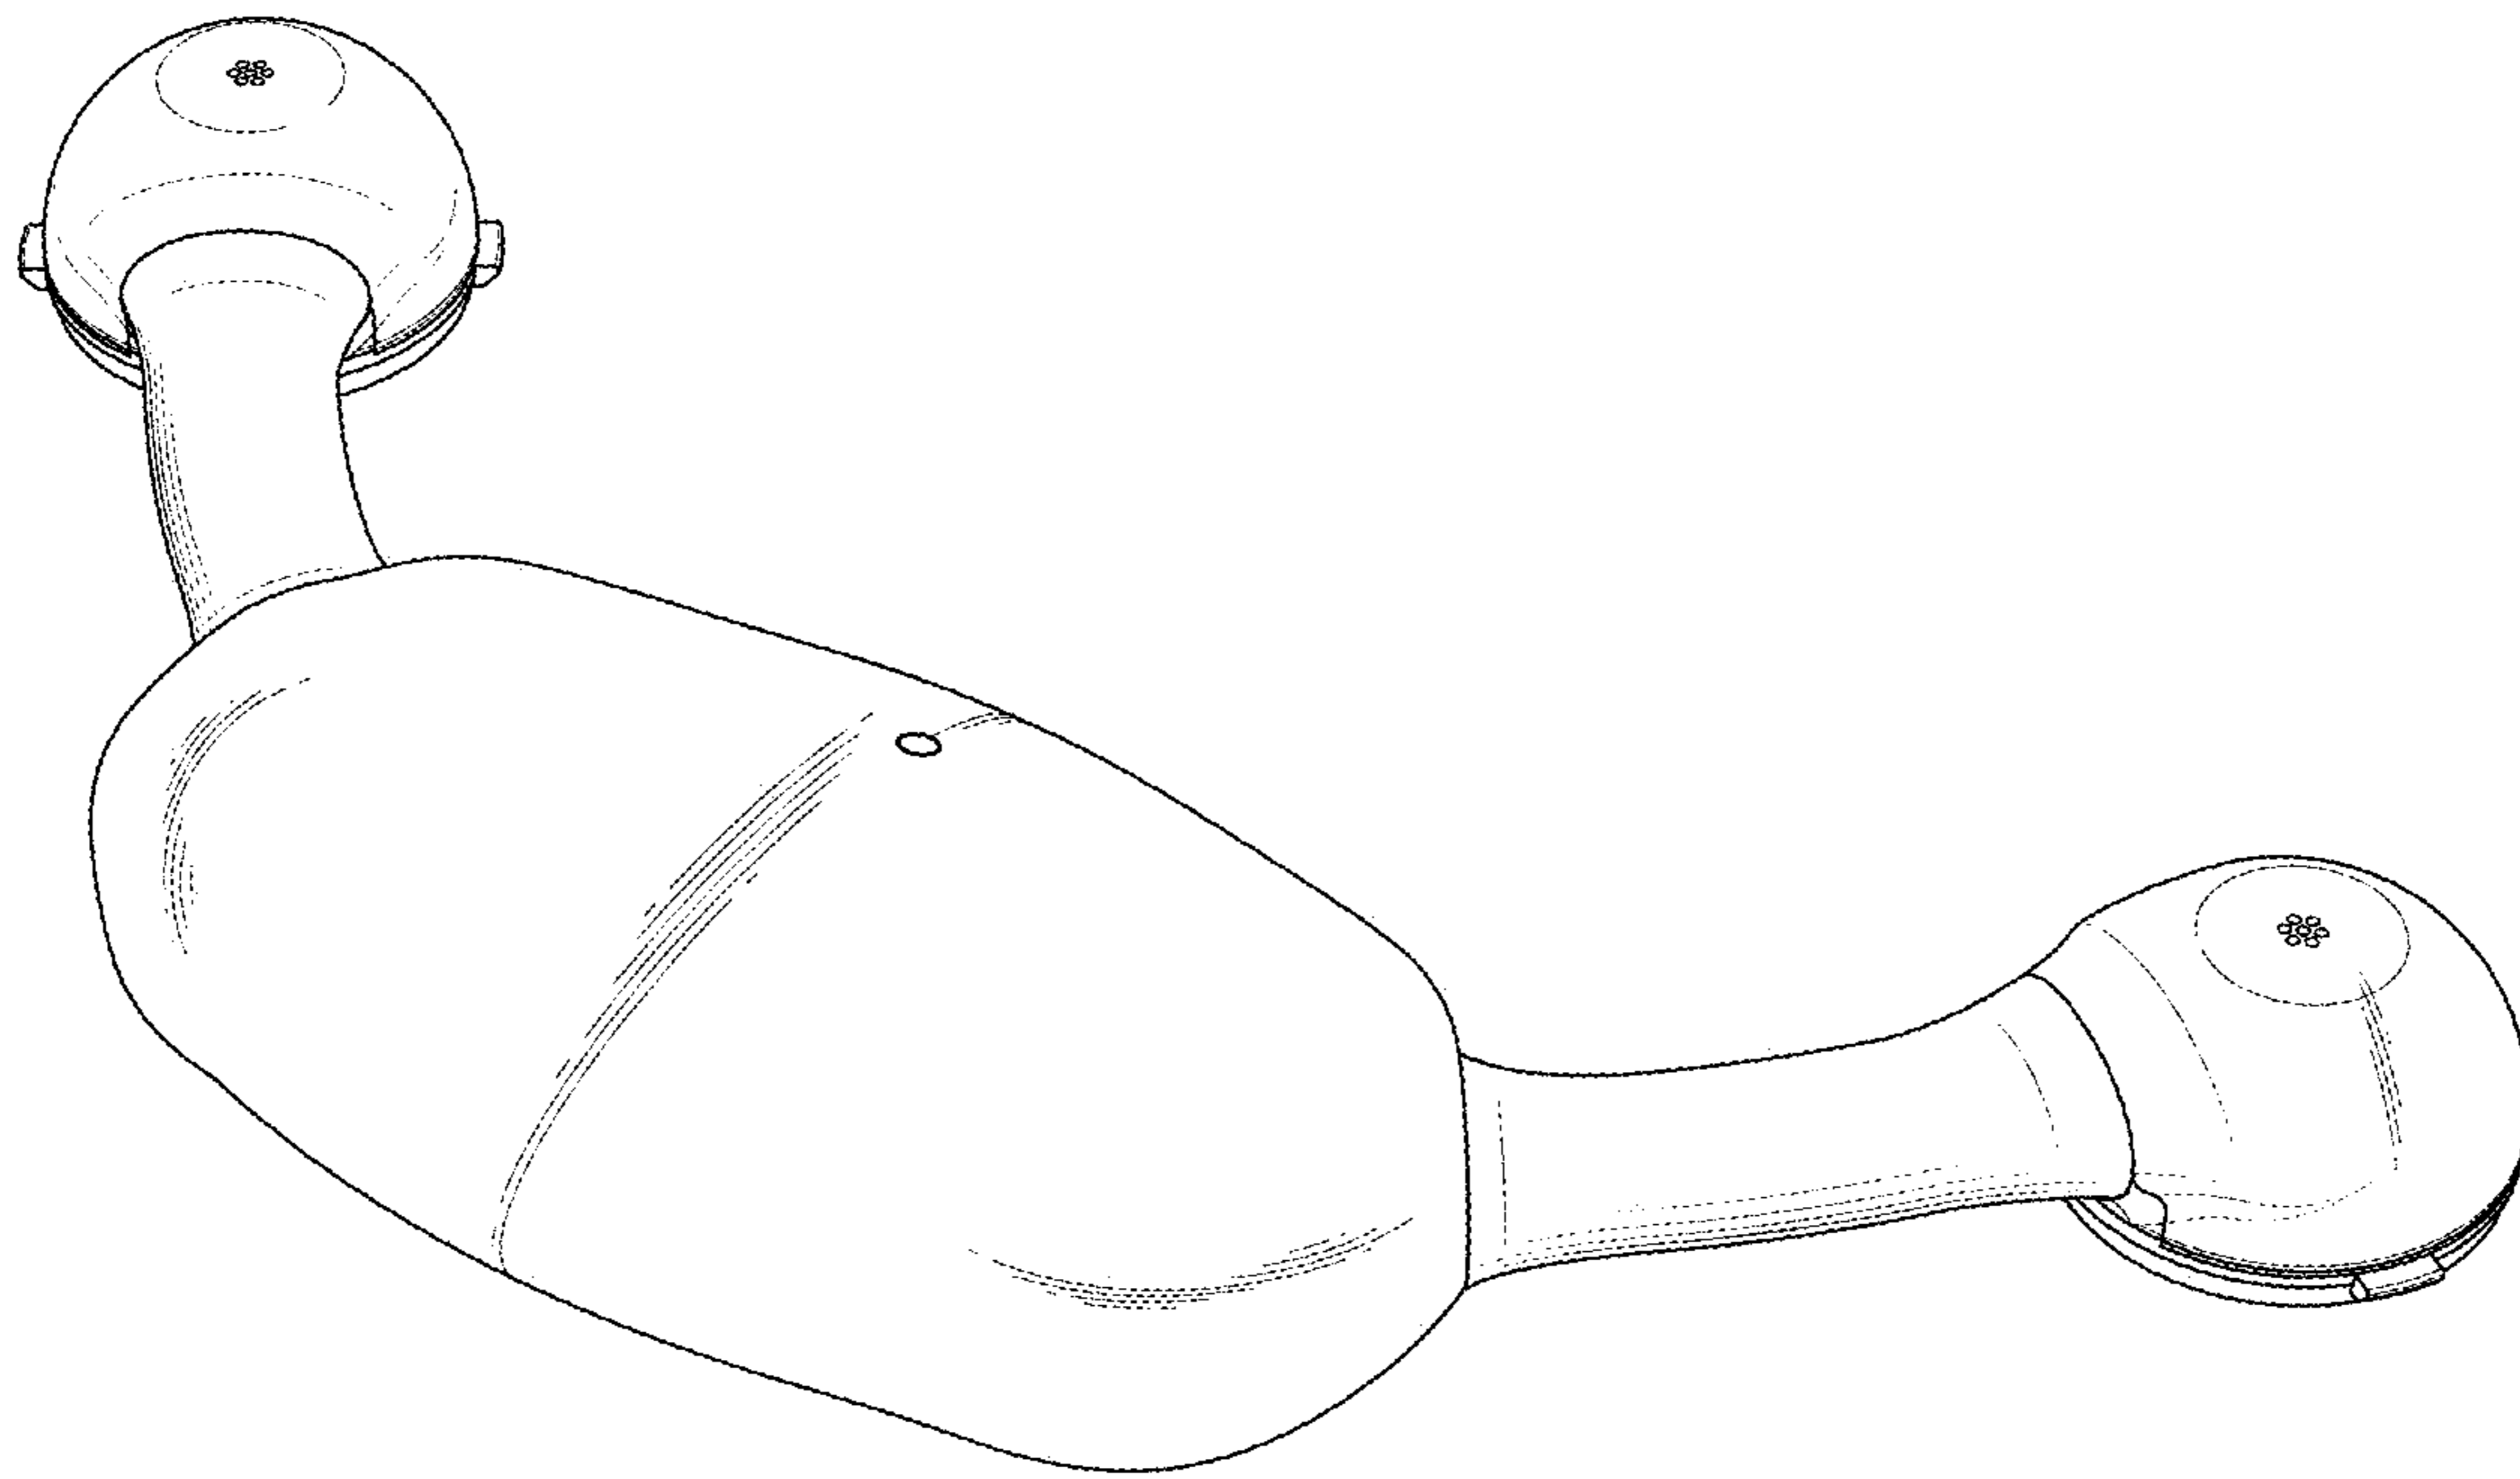


FIG. 1

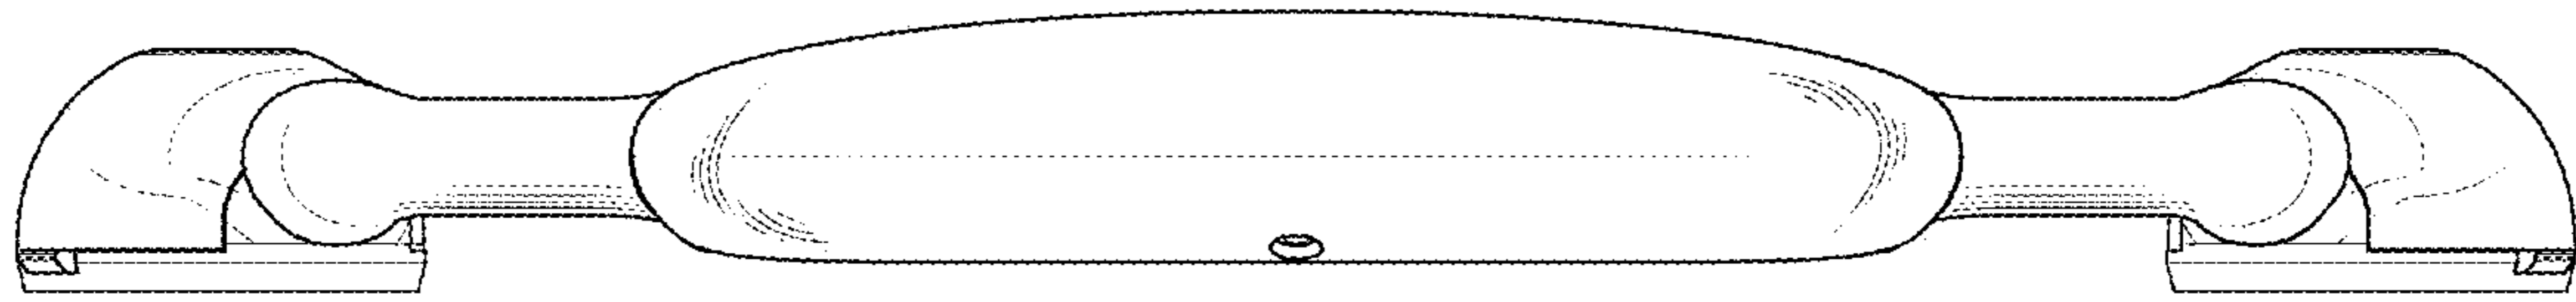


FIG. 2

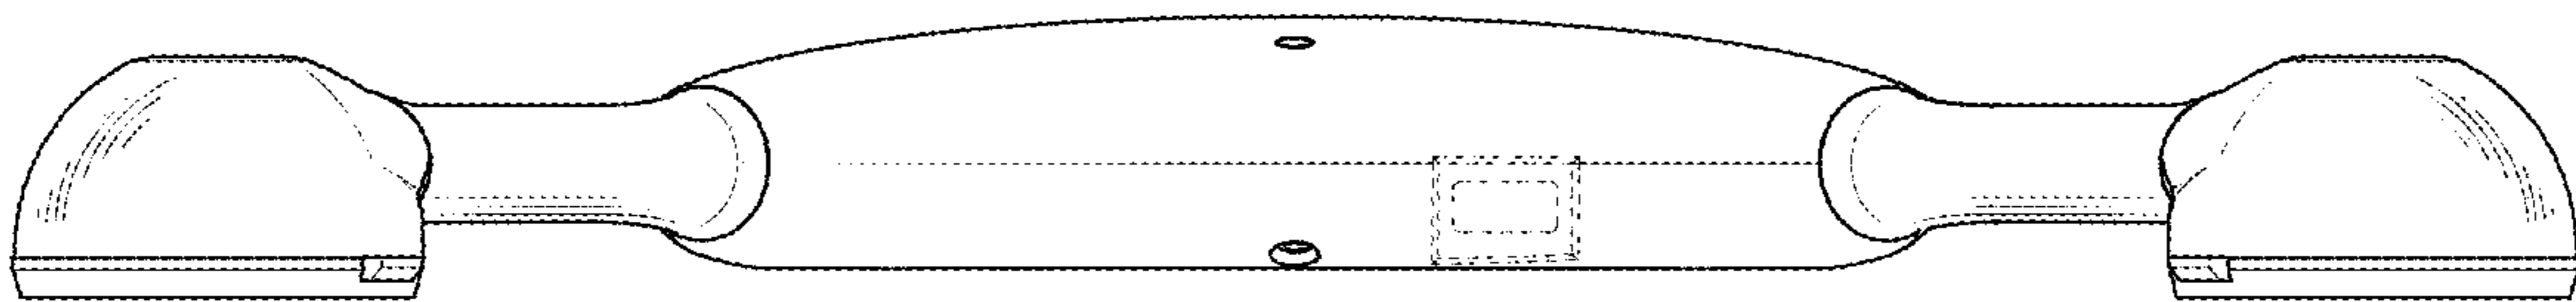


FIG. 3

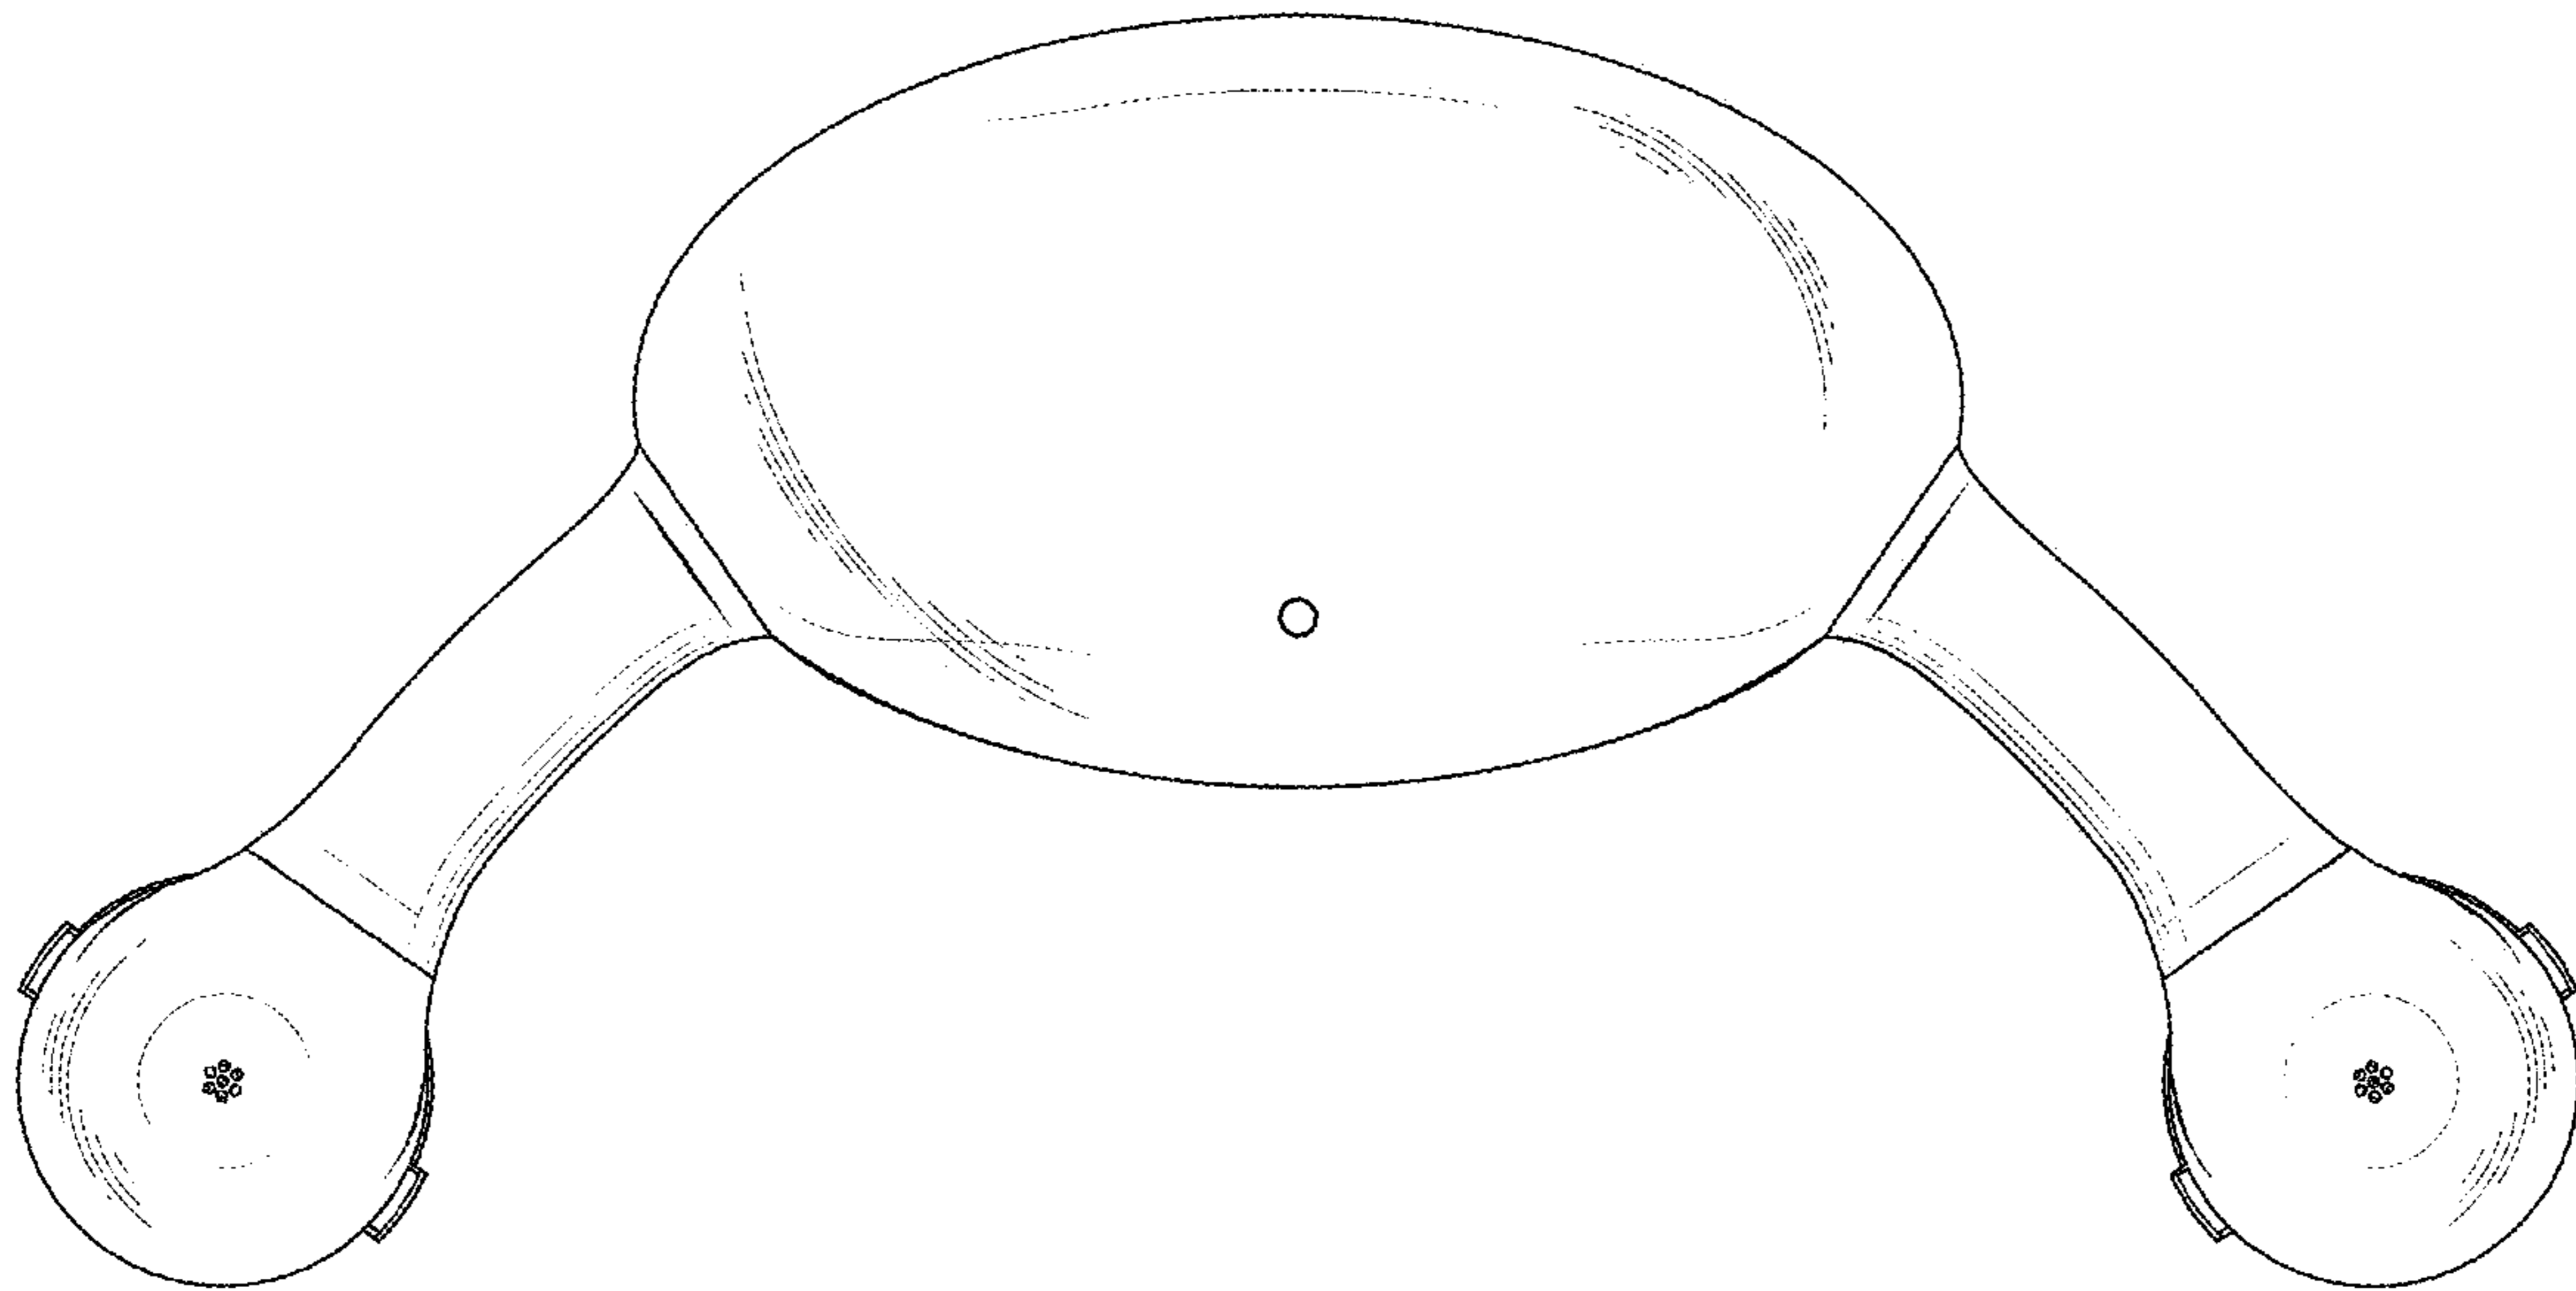


FIG. 4

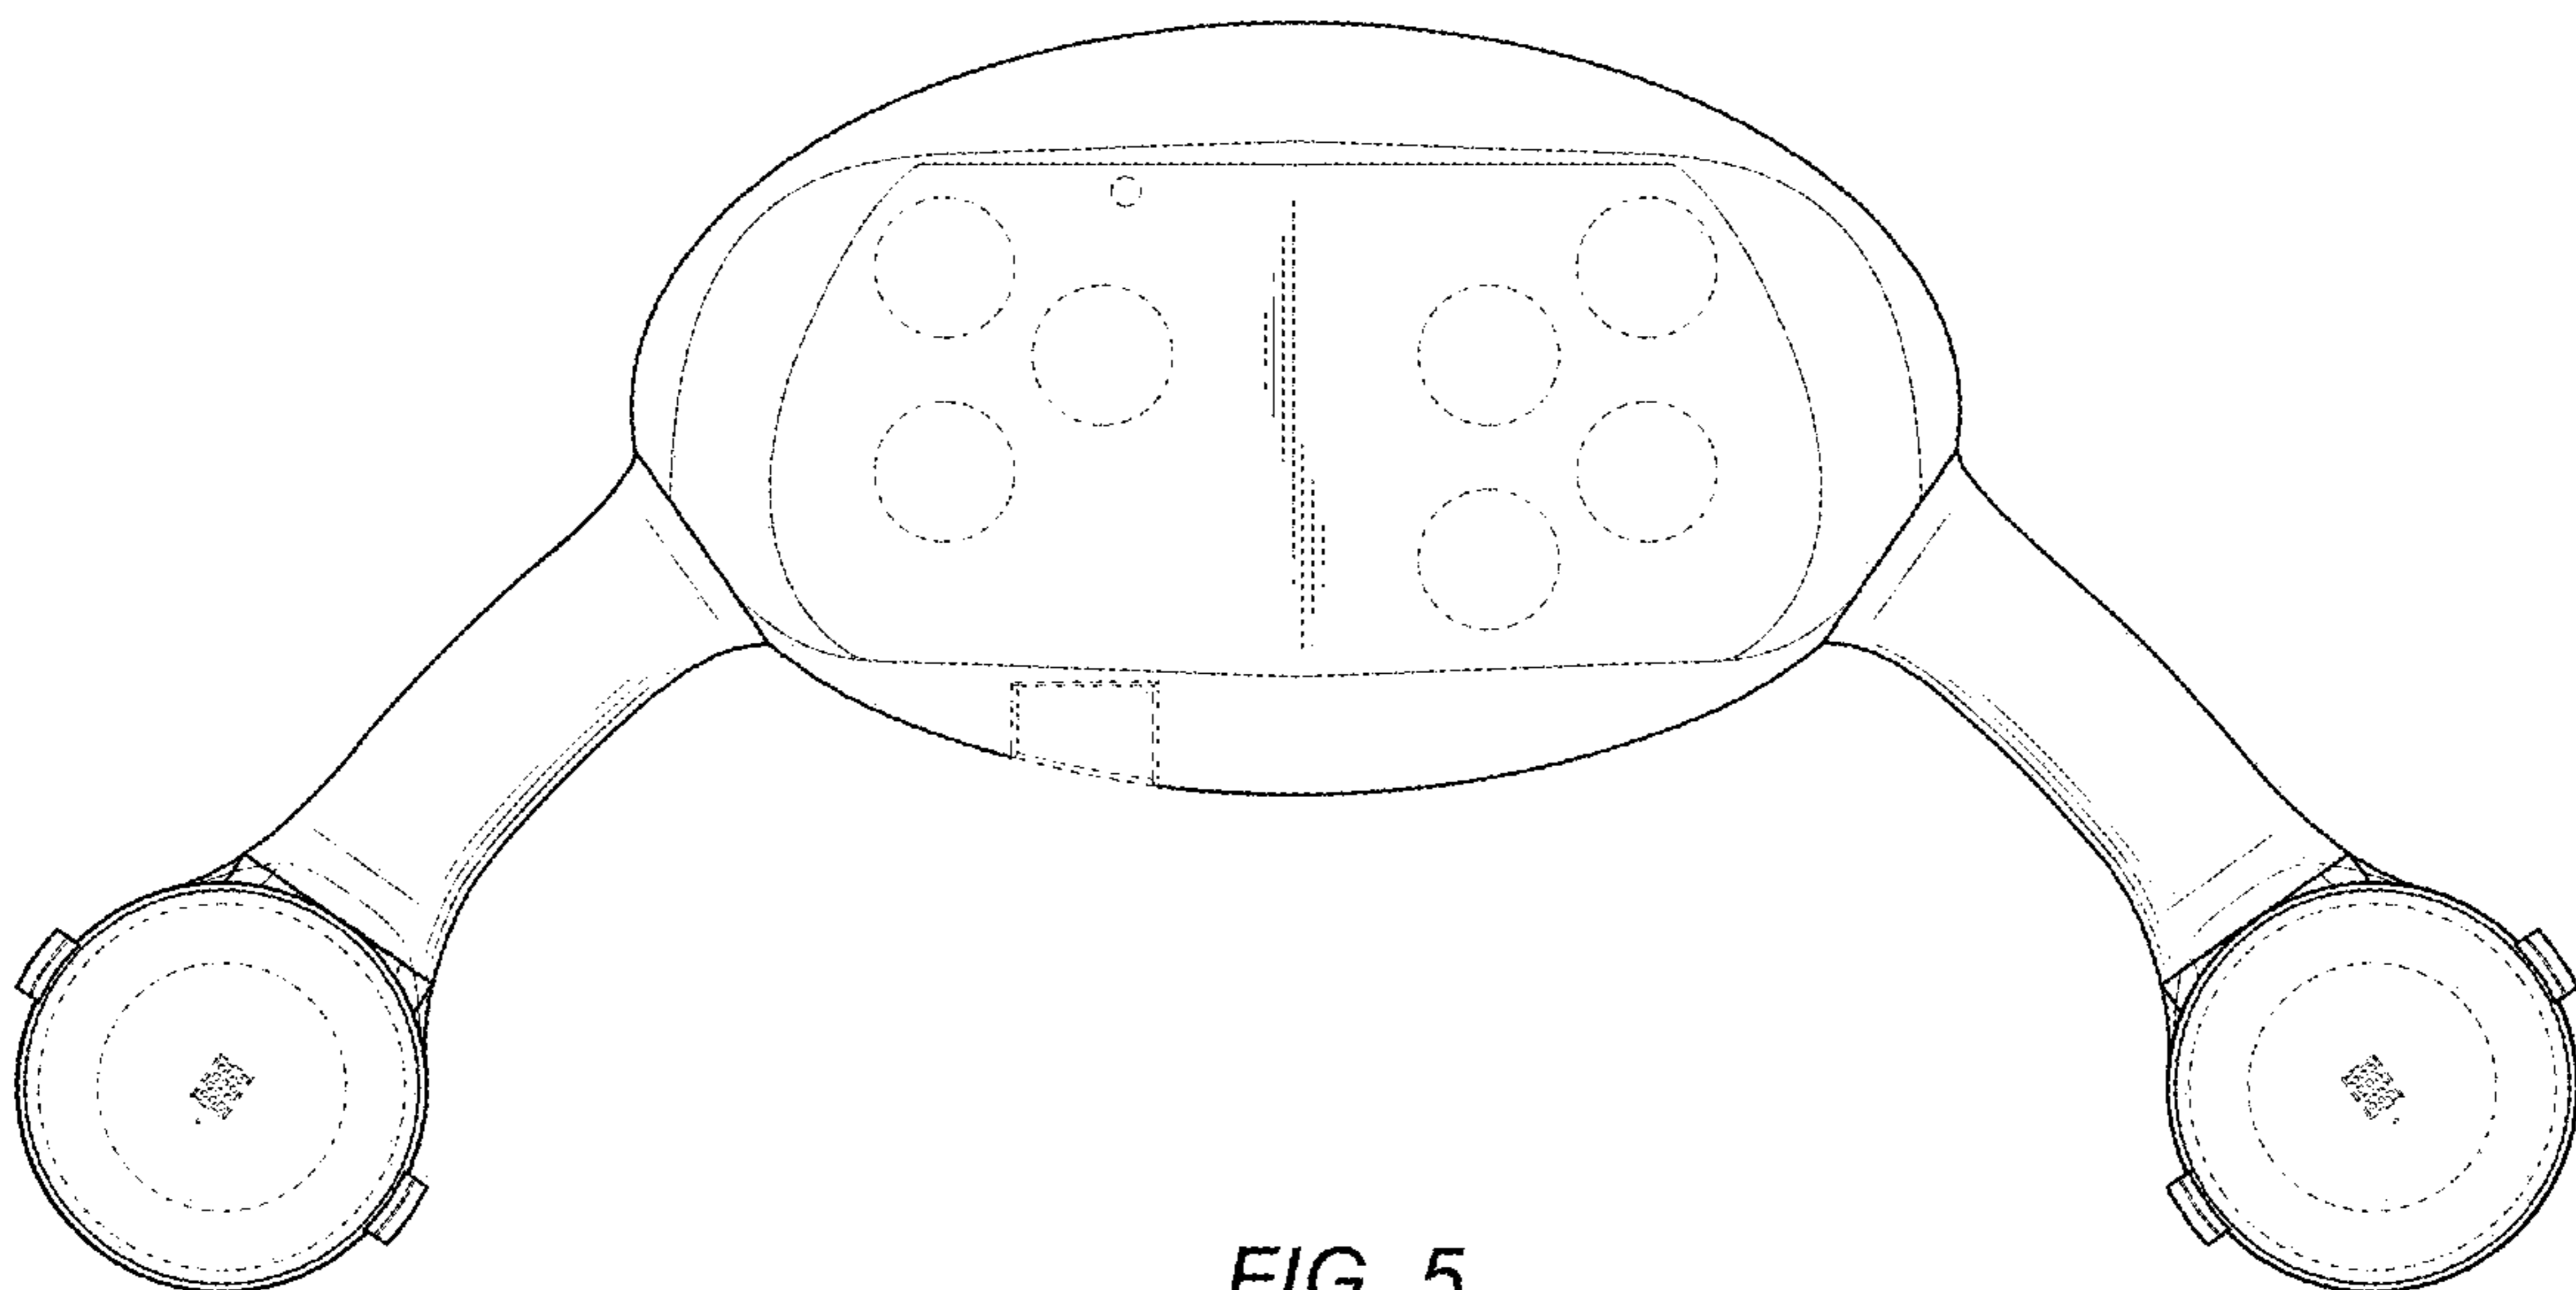


FIG. 5

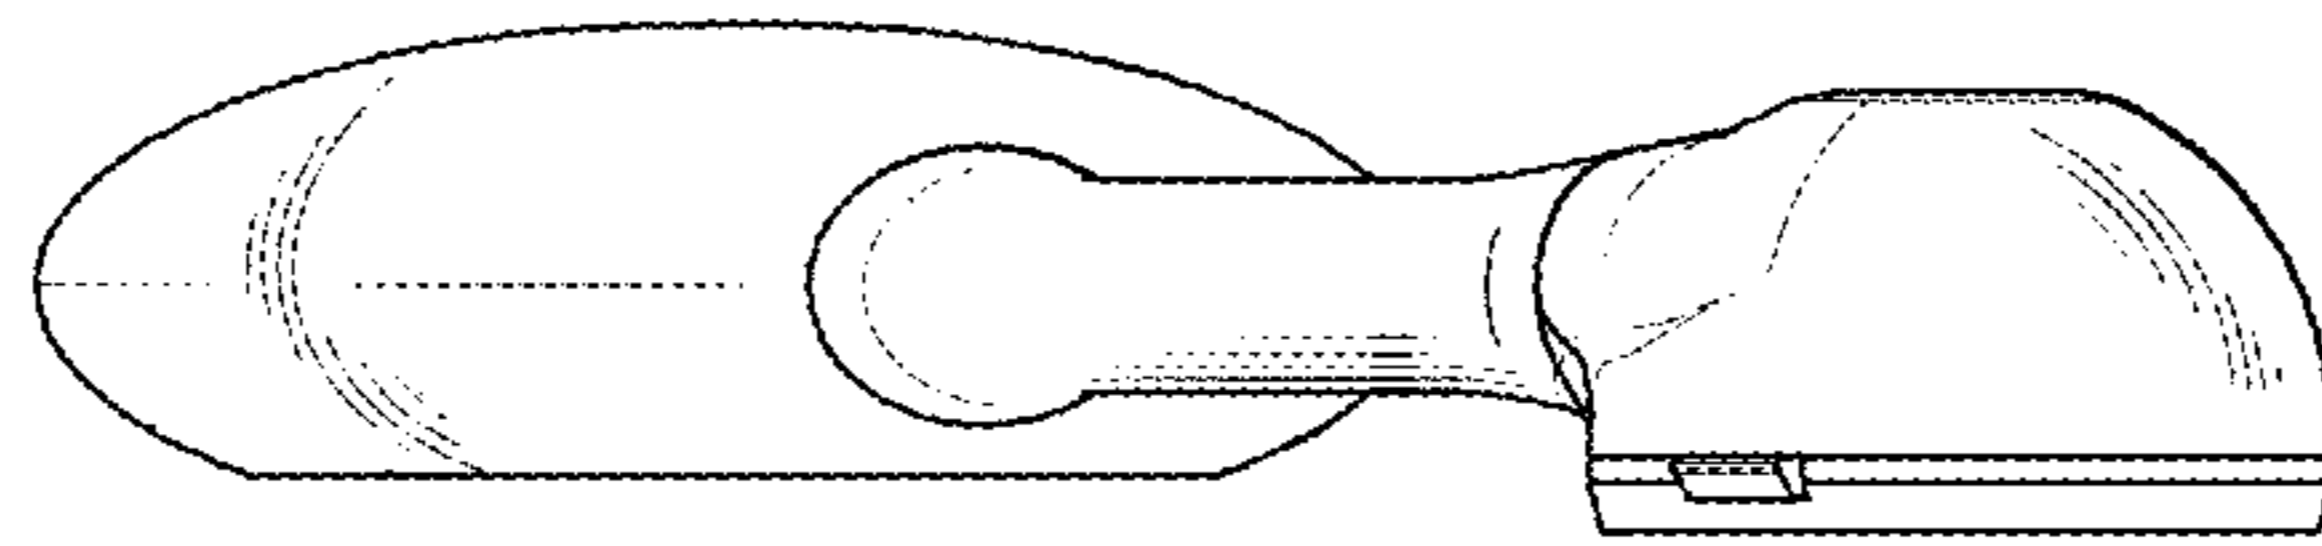


FIG. 6

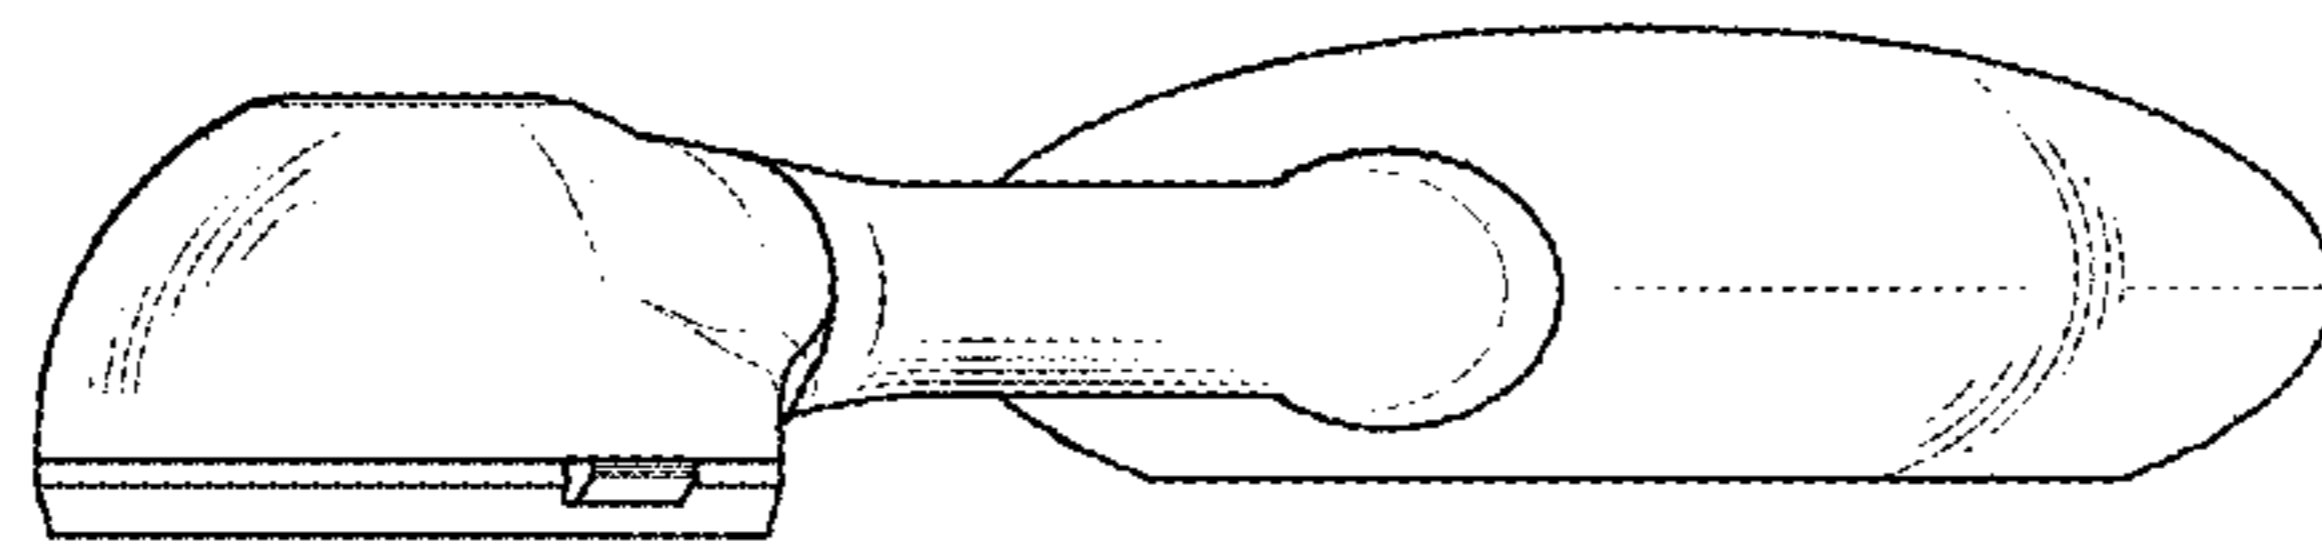


FIG. 7