

US00D975309S

(12) **United States Design Patent** (10) **Patent No.:** **US D975,309 S**  
**Gronewold et al.** (45) **Date of Patent:** **\*\* Jan. 10, 2023**

(54) **MEDICAL DIAGNOSTIC KIT**  
(71) Applicant: **T-Mobile Innovations LLC**, Overland Park, KS (US)  
(72) Inventors: **Julia Lea Gronewold**, Wichita, KS (US); **Joao Teixeira**, Shawnee, KS (US)  
(73) Assignee: **SPRINT COMMUNICATIONS COMPANY LP**, Overland Park, KS (US)

D838,379 S \* 1/2019 Trump ..... D24/216  
D942,035 S \* 1/2022 Suarez del Real Pena . D24/216  
2005/0084842 A1\* 4/2005 O'Connor ..... A61B 10/0045  
435/287.7

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(57) **CLAIM**

The ornamental design for a medical diagnostic kit, as shown and described.

**DESCRIPTION**


(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/779,226**  
(22) Filed: **Apr. 16, 2021**  
(51) **LOC (14) Cl.** ..... **24-01**  
(52) **U.S. Cl.**  
USPC ..... **D24/216**  
(58) **Field of Classification Search**  
USPC ..... D24/107, 186, 216, 232, 233, 234, 121,  
D24/122, 223, 224, 225, 227, 231, 119;  
D10/81  
CPC ..... A61B 10/0051; A61B 10/0096; C12Q  
1/6883; C12Q 1/6806; B01L 3/5023;  
B01L 3/523; B01L 3/565; B01L  
2300/0809; B01L 2300/0832  
See application file for complete search history.

FIG. 1 is a front perspective view of a medical diagnostic kit in accordance with our new design;  
FIG. 2 is a front elevation view thereof;  
FIG. 3 is a rear elevation view thereof;  
FIG. 4 is a side view thereof;  
FIG. 5 is a side view thereof, for the side opposite that of FIG. 4;  
FIG. 6 is a top view thereof;  
FIG. 7 is a bottom view thereof;  
FIG. 8 is a rear perspective view thereof;  
FIG. 9 is a front perspective view of another medical diagnostic kit in accordance with my new design;  
FIG. 10 is a front elevation view thereof;  
FIG. 11 is a rear elevation view thereof;  
FIG. 12 is a side view thereof;  
FIG. 13 is another side view thereof;  
FIG. 14 is a top view thereof;  
FIG. 15 is a bottom view thereof;  
FIG. 16 is a rear perspective view thereof; and,  
FIG. 17 is an exploded view thereof.  
The stippled shading in the drawings represents surfaces having the contrast in appearance shown.  
The broken lines in FIG. 17 illustrate portions of the medical diagnostic kit that form no part of the claimed design.

(56) **References Cited**  
U.S. PATENT DOCUMENTS

D287,570 S \* 1/1987 Olsen ..... D24/224  
D477,669 S \* 7/2003 Zhou ..... D24/224  
D743,571 S \* 11/2015 Jackson ..... D24/224  
D748,813 S \* 2/2016 Ishiguro ..... D24/224  
D760,490 S \* 7/2016 Johnson ..... D3/203.1

**1 Claim, 11 Drawing Sheets**

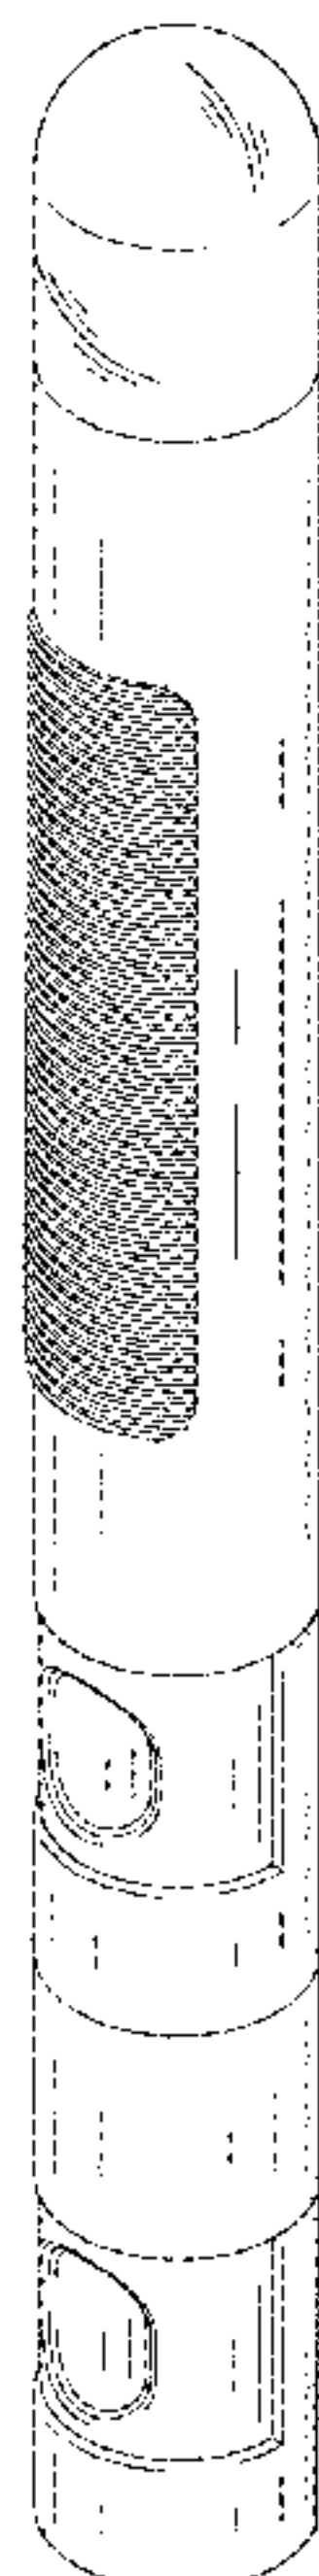

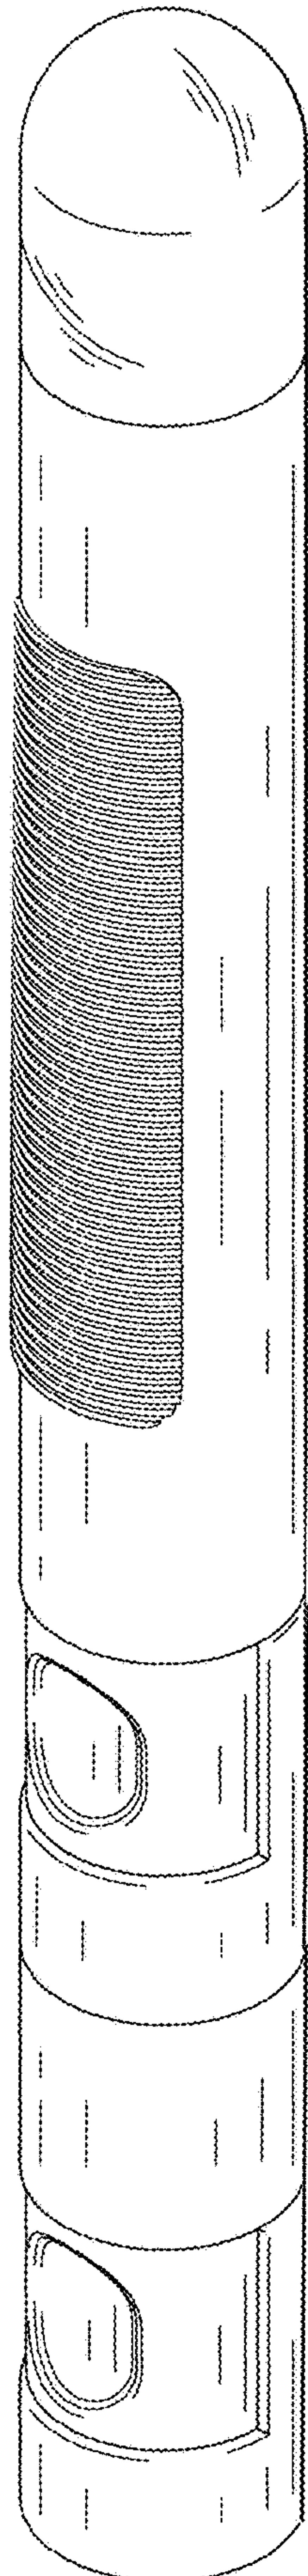


FIG. 1

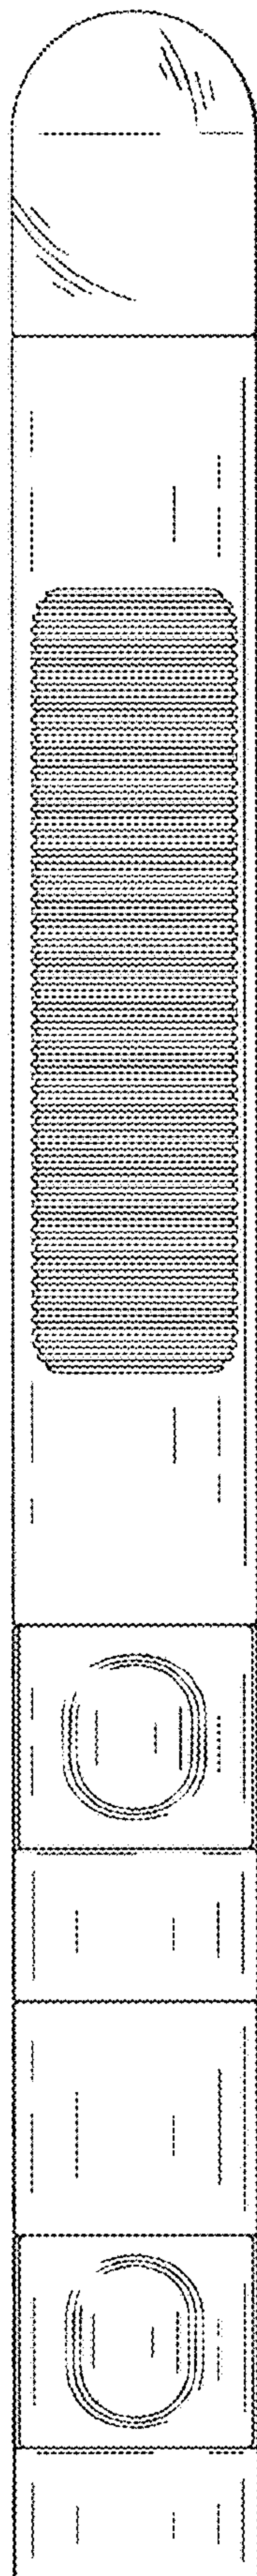


FIG. 2

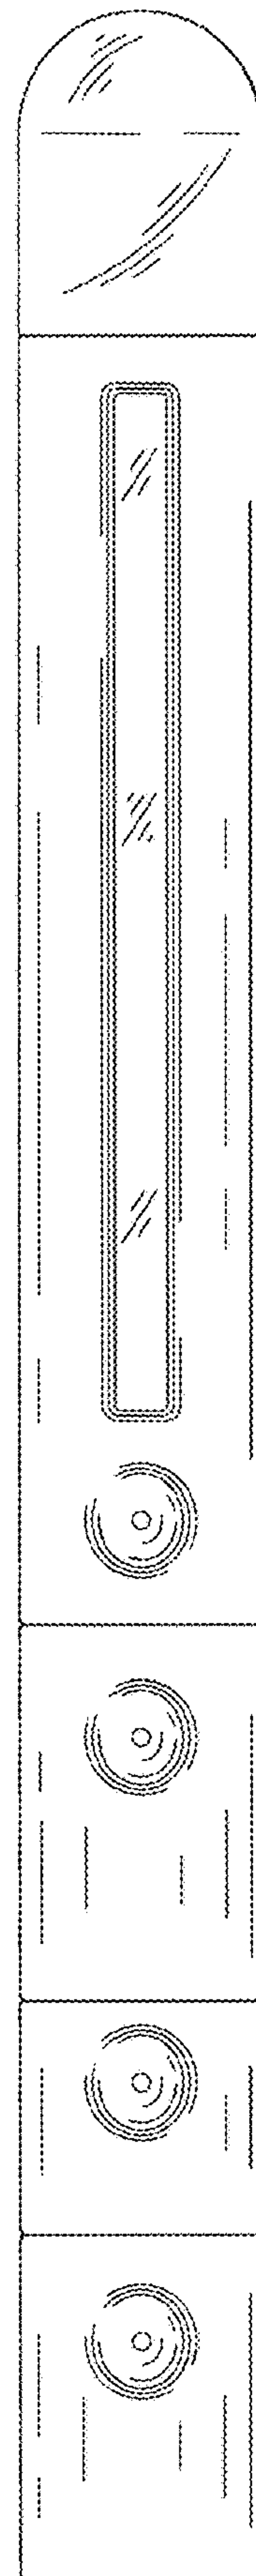


FIG. 3



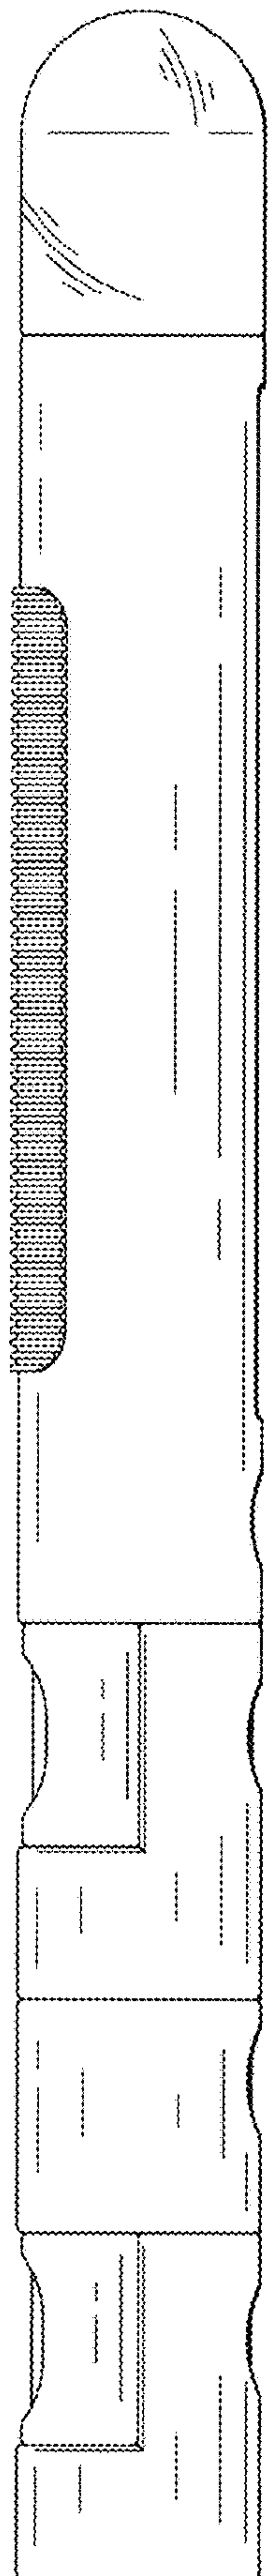


FIG. 4

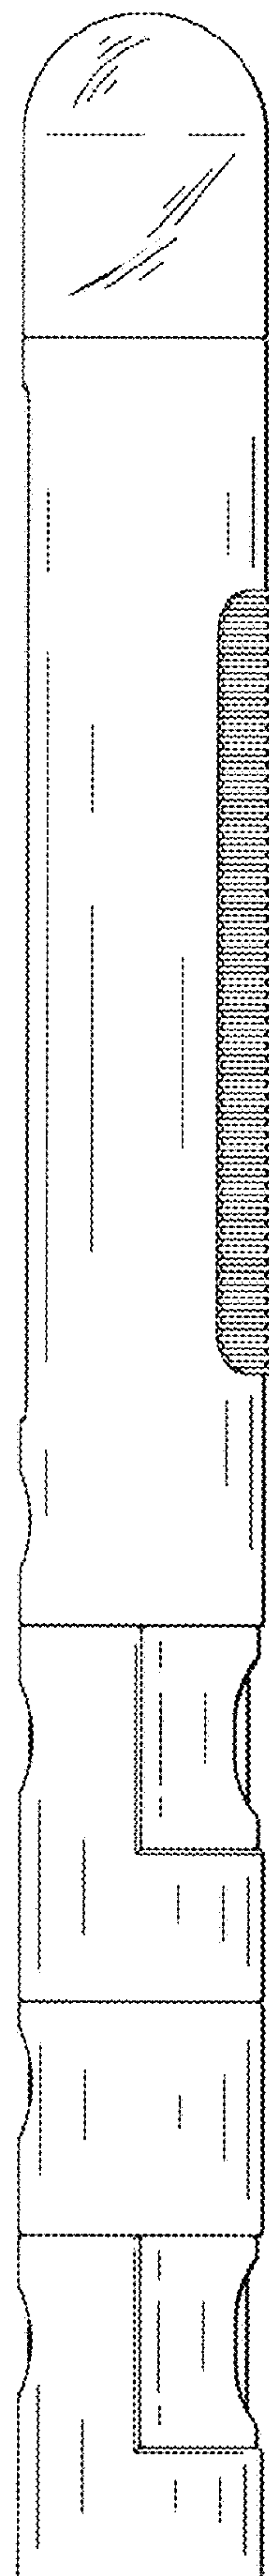


FIG. 5

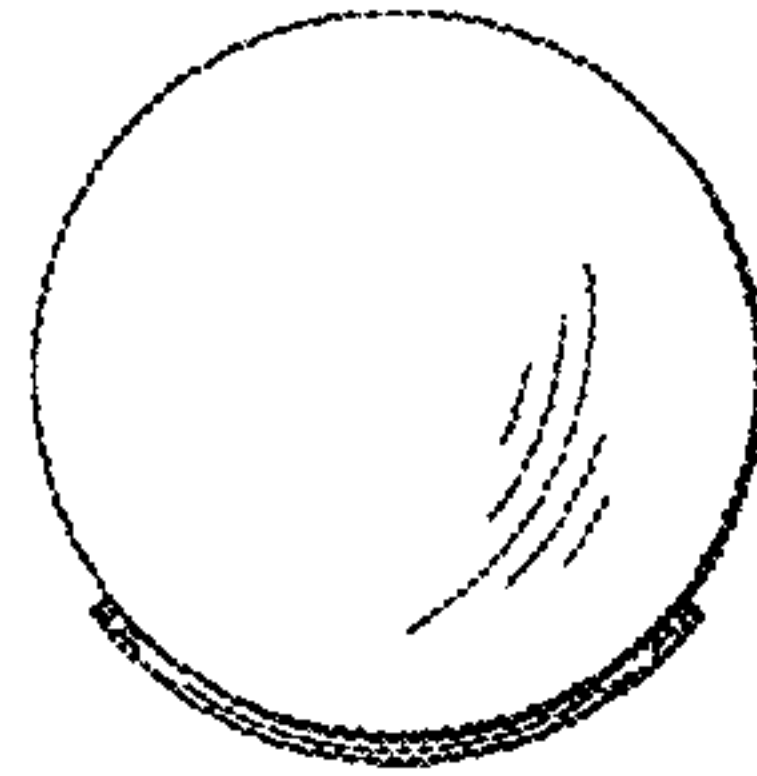


FIG. 6

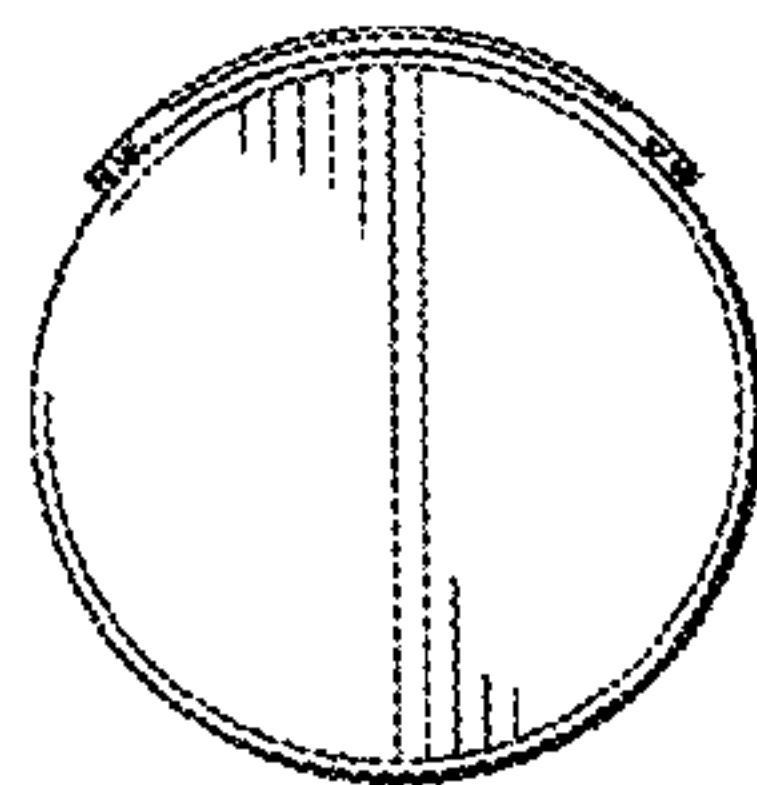


FIG. 7

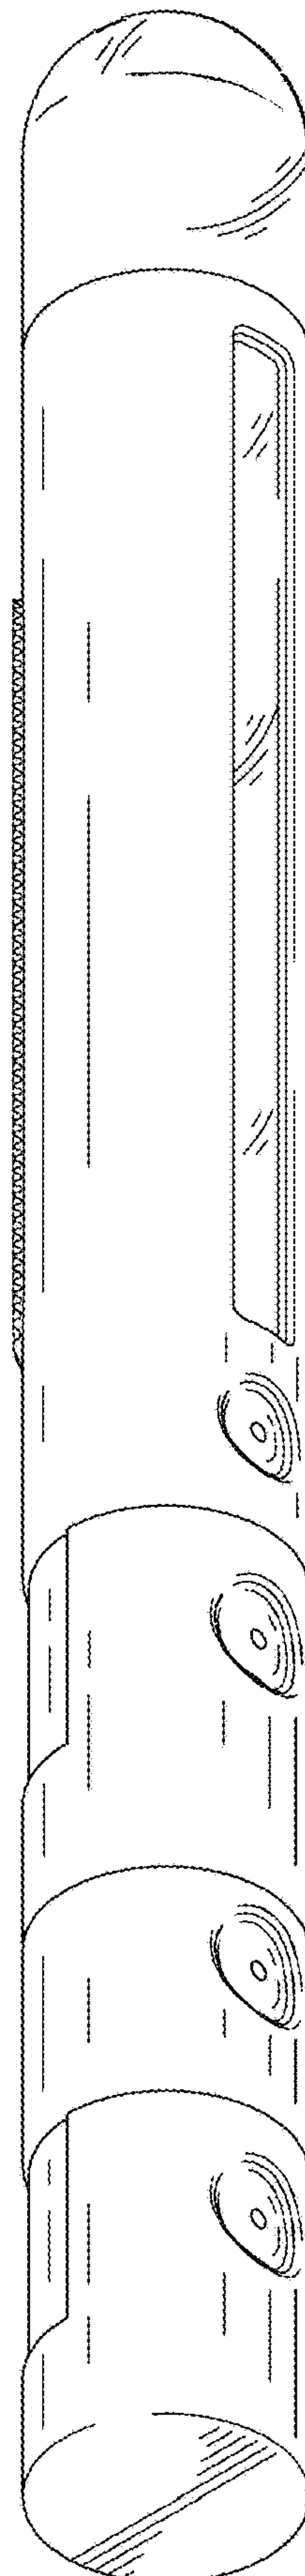


FIG. 8

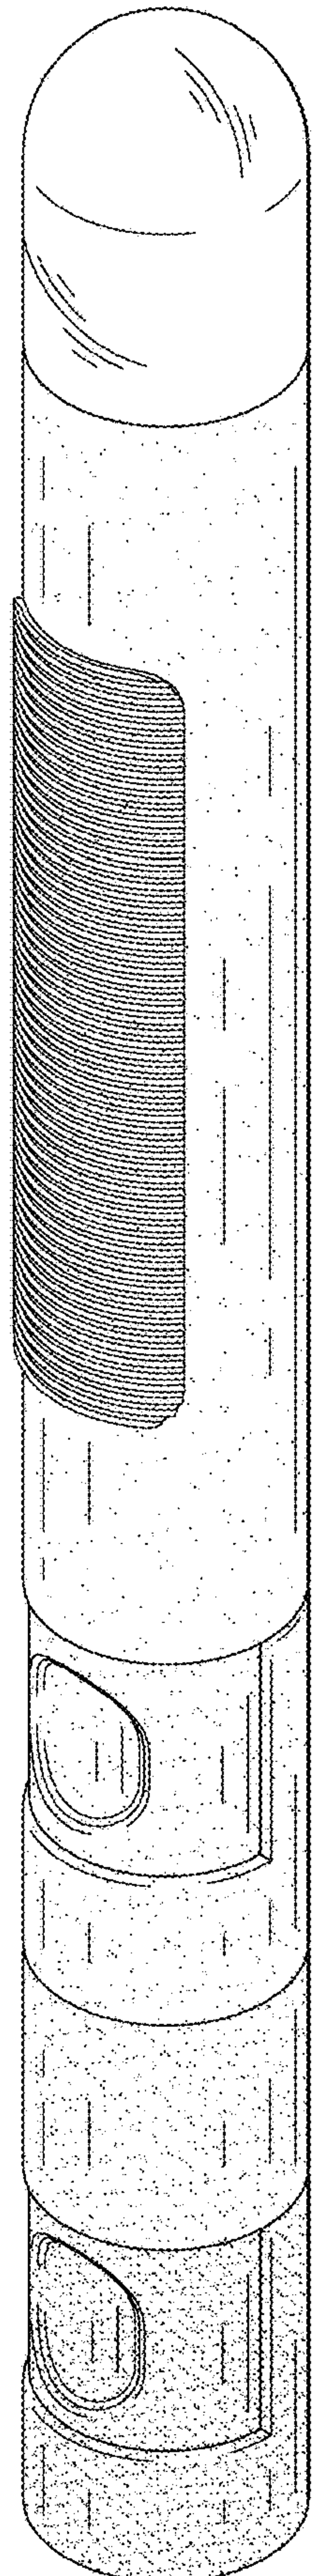


FIG. 9



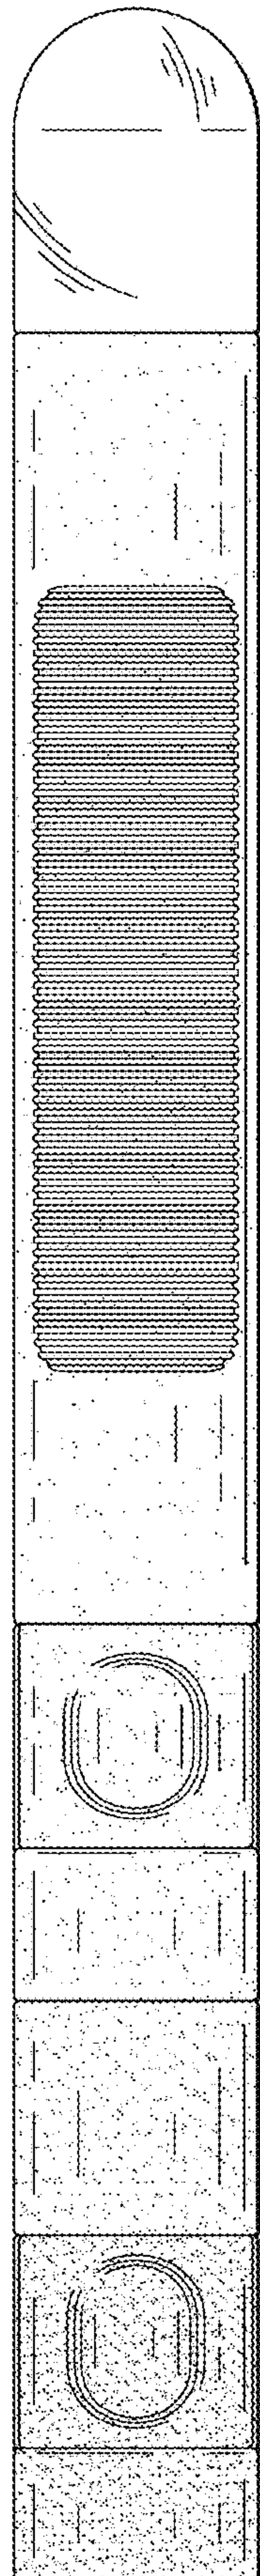


FIG. 10

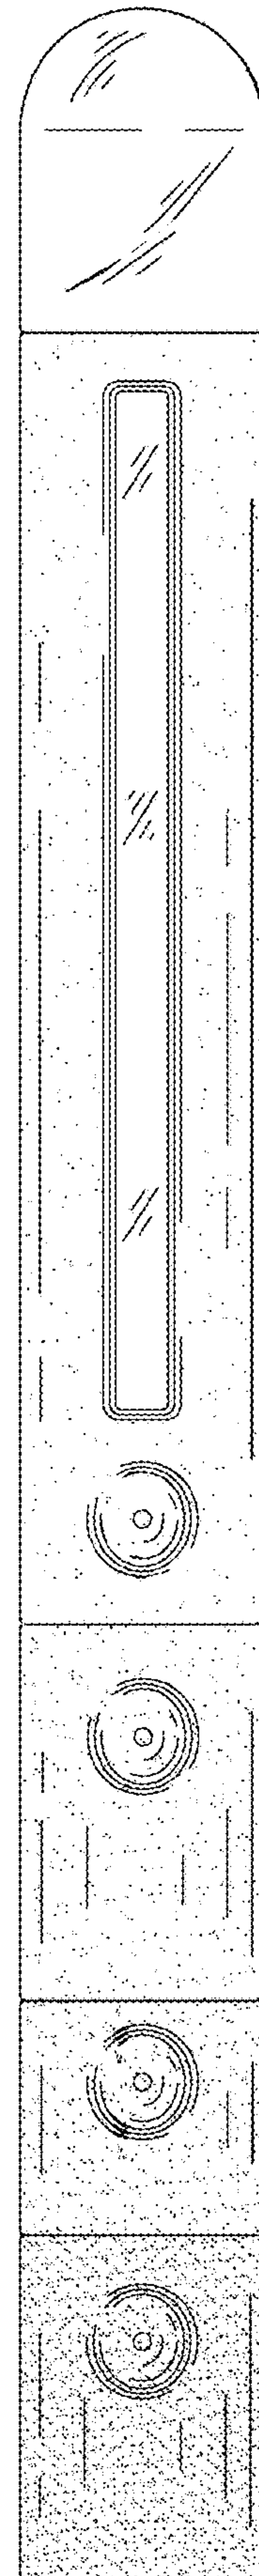


FIG. 11



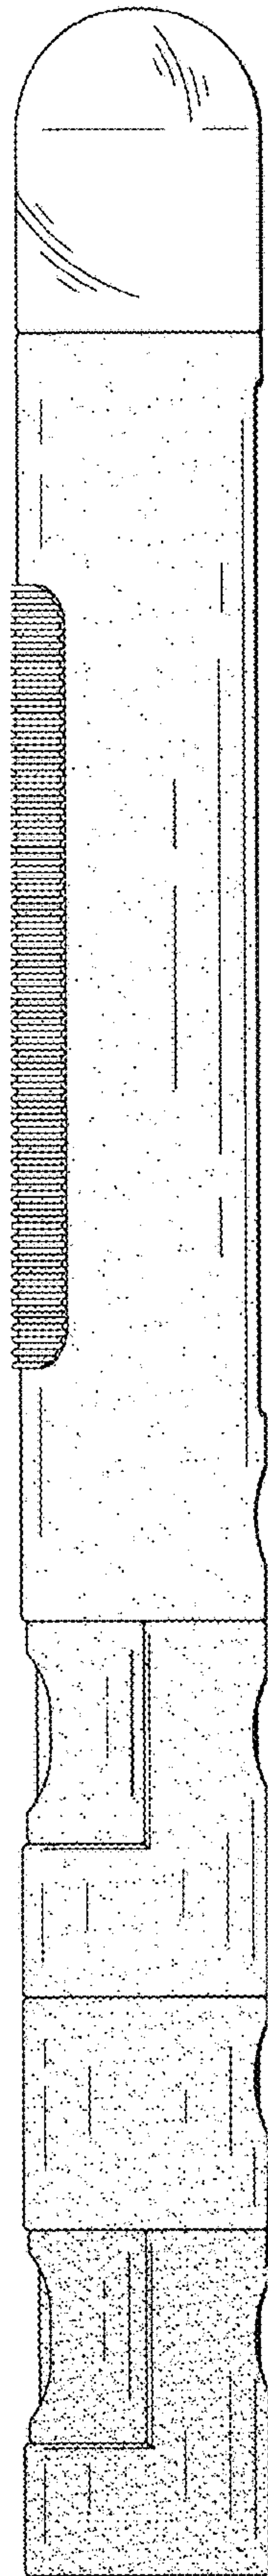


FIG. 12



FIG. 13

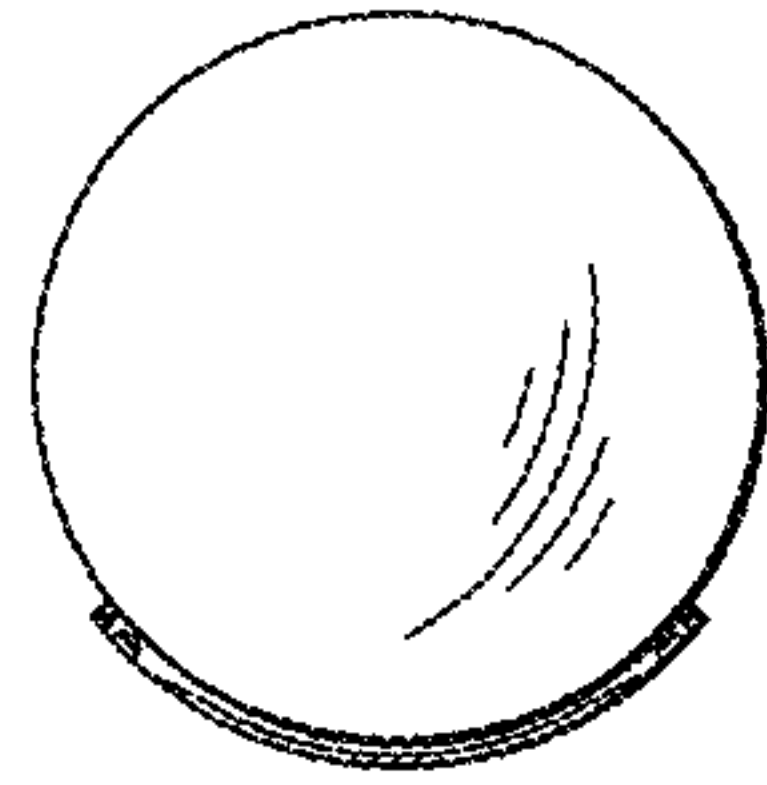


FIG. 14

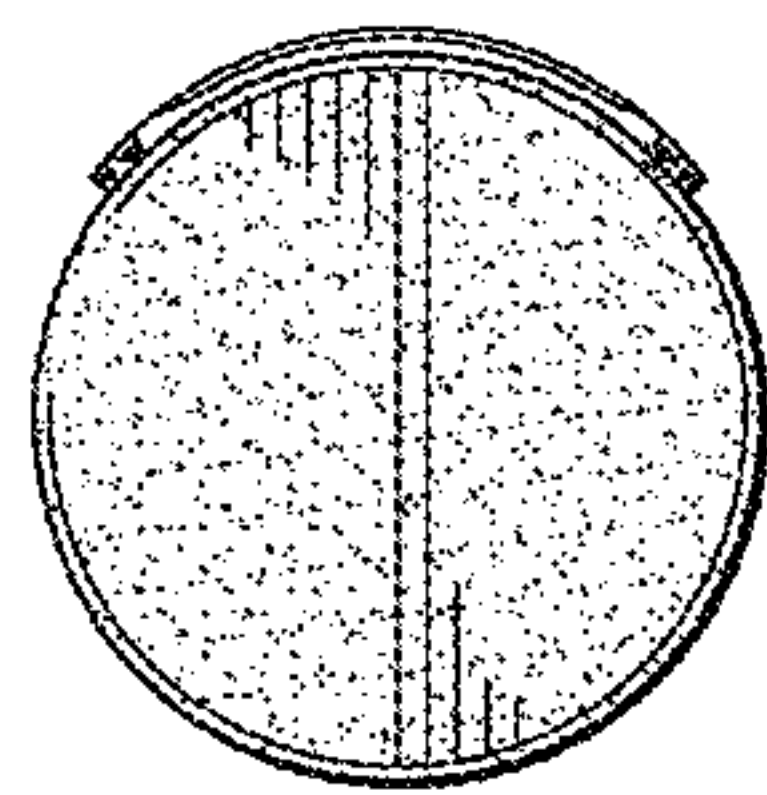


FIG. 15

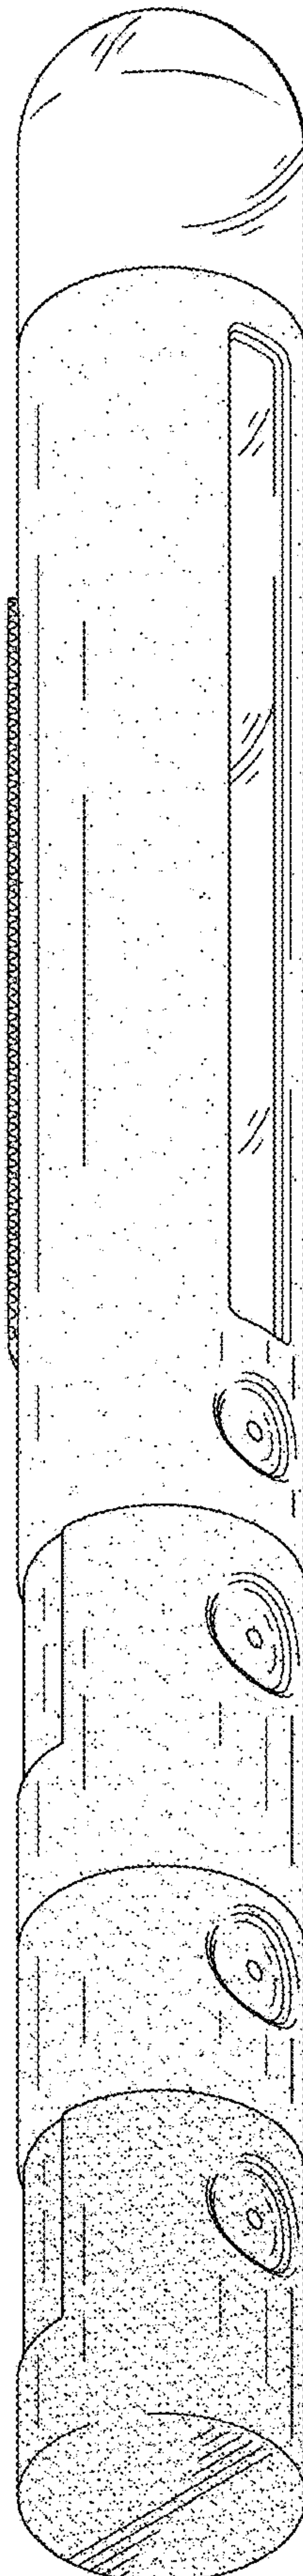


FIG. 16

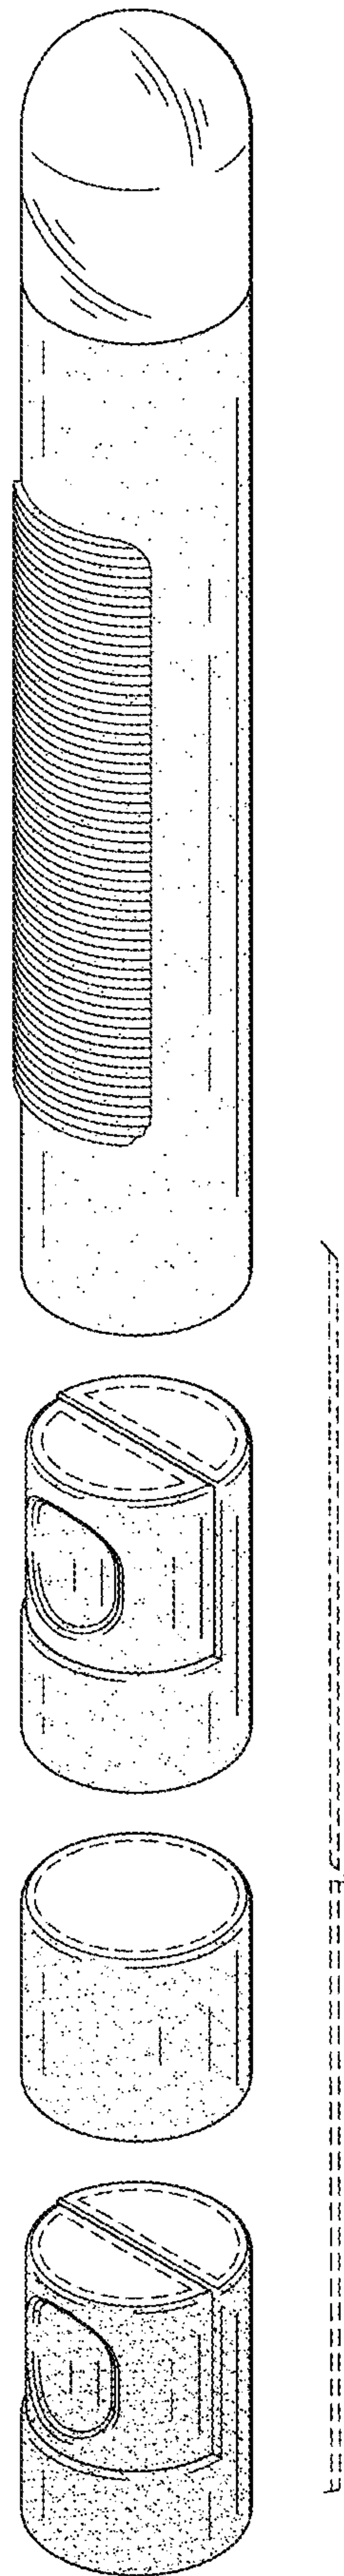


FIG. 17