



US00D975855S

(12) **United States Design Patent**
Bierman

(10) **Patent No.:** **US D975,855 S**

(45) **Date of Patent:** **** Jan. 17, 2023**

- (54) **CATHETER SECUREMENT PAD**
- (71) Applicant: **Maddoc Medical Products, Inc.**, Los Angeles, CA (US)
- (72) Inventor: **Steven Bierman**, Del Mar, CA (US)
- (73) Assignee: **Maddoc Medical Products, Inc.**, Los Angeles, CA (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/775,815**
- (22) Filed: **Mar. 25, 2021**
- (51) **LOC (14) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/189**; D24/128
- (58) **Field of Classification Search**
USPC D24/127-130, 188-190
CPC A61M 25/02; A61M 2025/0206; A61M 2025/024; A61M 2025/0266; A61M 2025/028; A61M 2025/0246; Y10S 128/26
See application file for complete search history.

9,017,290 B2 4/2015 Peters et al.
 D745,973 S * 12/2015 Russo D24/189
 9,895,514 B2 2/2018 Bierman et al.
 (Continued)

OTHER PUBLICATIONS

Merit Medical StayFIX Catheter Fixation Device, Merit Medical Systems, healthproductsforyou.com, [Post date unknown], [Sitem seen Nov. 14, 2022], Seen at URL: <https://www.healthproductsforyou.com/p-merit-medical-stayfix-catheter-fixation-device.html> (Year: 2022).*

(Continued)

Primary Examiner — Natasha Vujcic
Assistant Examiner — Gilbert B Ford
 (74) *Attorney, Agent, or Firm* — Master Key IP, LLP;
 Jeromye V. Sartain

(57) **CLAIM**

The ornamental design for a catheter securement pad, as shown and described.

DESCRIPTION


FIG. 1 is an exploded perspective view showing a catheter securement pad;
 FIG. 2 is a top view of the catheter securement pad with the peel-off layers removed for ease of illustration;
 FIG. 3 is a bottom view of the catheter securement pad with the peel-off layers removed for ease of illustration;
 FIG. 4 is a left side view of the catheter securement pad with the peel-off layers removed for ease of illustration;
 FIG. 5 is a right side view of the catheter securement pad with the peel-off layers removed for ease of illustration;
 FIG. 6 is a front view of the catheter securement pad with the peel-off layers removed for ease of illustration; and,
 FIG. 7 is a rear view of the catheter securement pad with the peel-off layers removed for ease of illustration.
 The broken lines show portions of the catheter securement pad that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,627,842	A	12/1986	Katz	
4,997,421	A	3/1991	Palsrok et al.	
5,855,591	A	1/1999	Bierman	
6,224,571	B1	5/2001	Bierman	
6,413,240	B1	7/2002	Bierman et al.	
6,786,892	B2	9/2004	Bierman	
7,153,291	B2	12/2006	Bierman	
7,204,827	B2 *	4/2007	Kessler A61M 25/02 128/DIG. 26
D577,437	S *	9/2008	Bierman D24/128
8,394,067	B2	3/2013	Bracken et al.	
8,486,004	B1	7/2013	Propp	
8,608,704	B2	12/2013	Bierman	
8,608,705	B2	12/2013	Peters et al.	

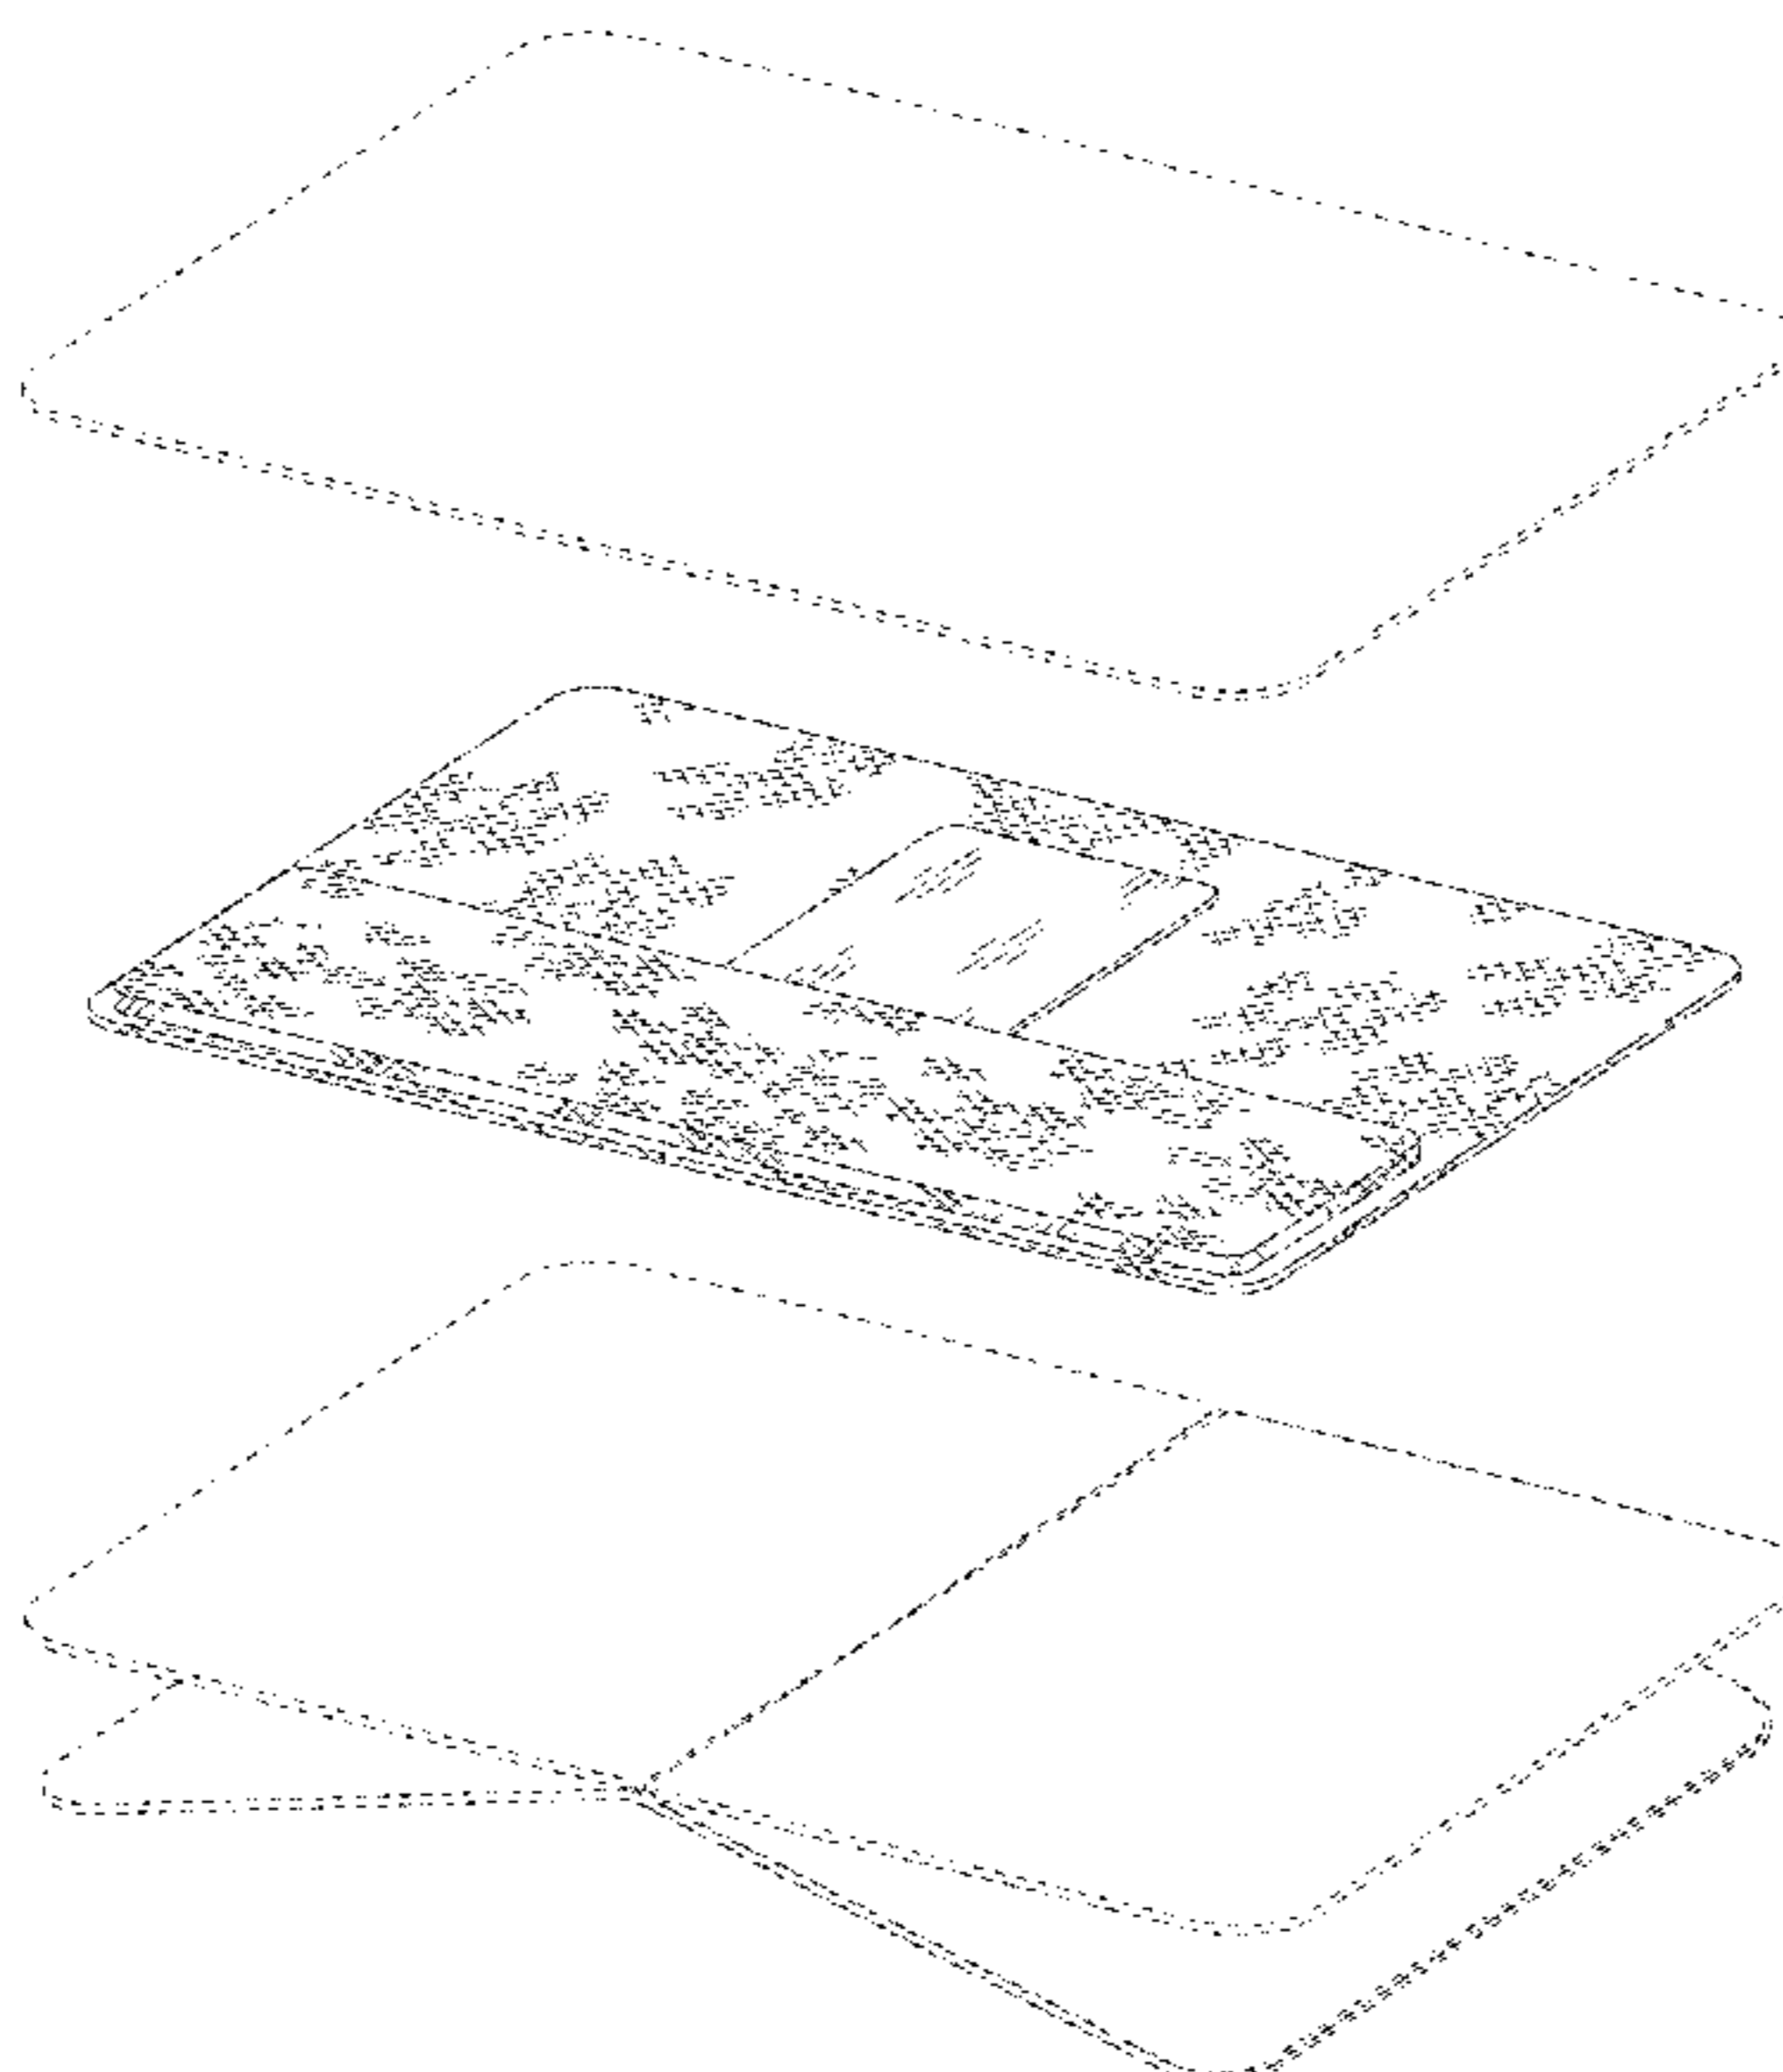

(56)

References Cited

U.S. PATENT DOCUMENTS

D818,121 S * 5/2018 Park D24/128
D834,711 S * 11/2018 Kyvik D24/128
10,188,835 B1 * 1/2019 McClarren A61M 25/02
10,232,145 B2 3/2019 Bierman et al.
D848,614 S * 5/2019 Wilson D24/128
10,463,837 B2 11/2019 Bierman et al.
10,561,825 B2 2/2020 Bierman et al.
D877,306 S * 3/2020 Liu D24/189
D877,326 S * 3/2020 Coleman D24/128
D898,925 S * 10/2020 Kelbie D24/189
11,020,564 B2 * 6/2021 Madlung A61M 25/0113
D946,767 S * 3/2022 Kemper D24/189
D964,571 S * 9/2022 Bierman D24/189
2006/0247577 A1 11/2006 Wright
2011/0319830 A1 12/2011 Peters et al.
2013/0204190 A1 8/2013 Wilborn et al.
2020/0179655 A1 6/2020 Bierman et al.

OTHER PUBLICATIONS

Bard Securis stabilization device web page screen shots, taken from <https://www.bardaccess.com/products/procedural/securis> on Jun. 12, 2020.

* cited by examiner

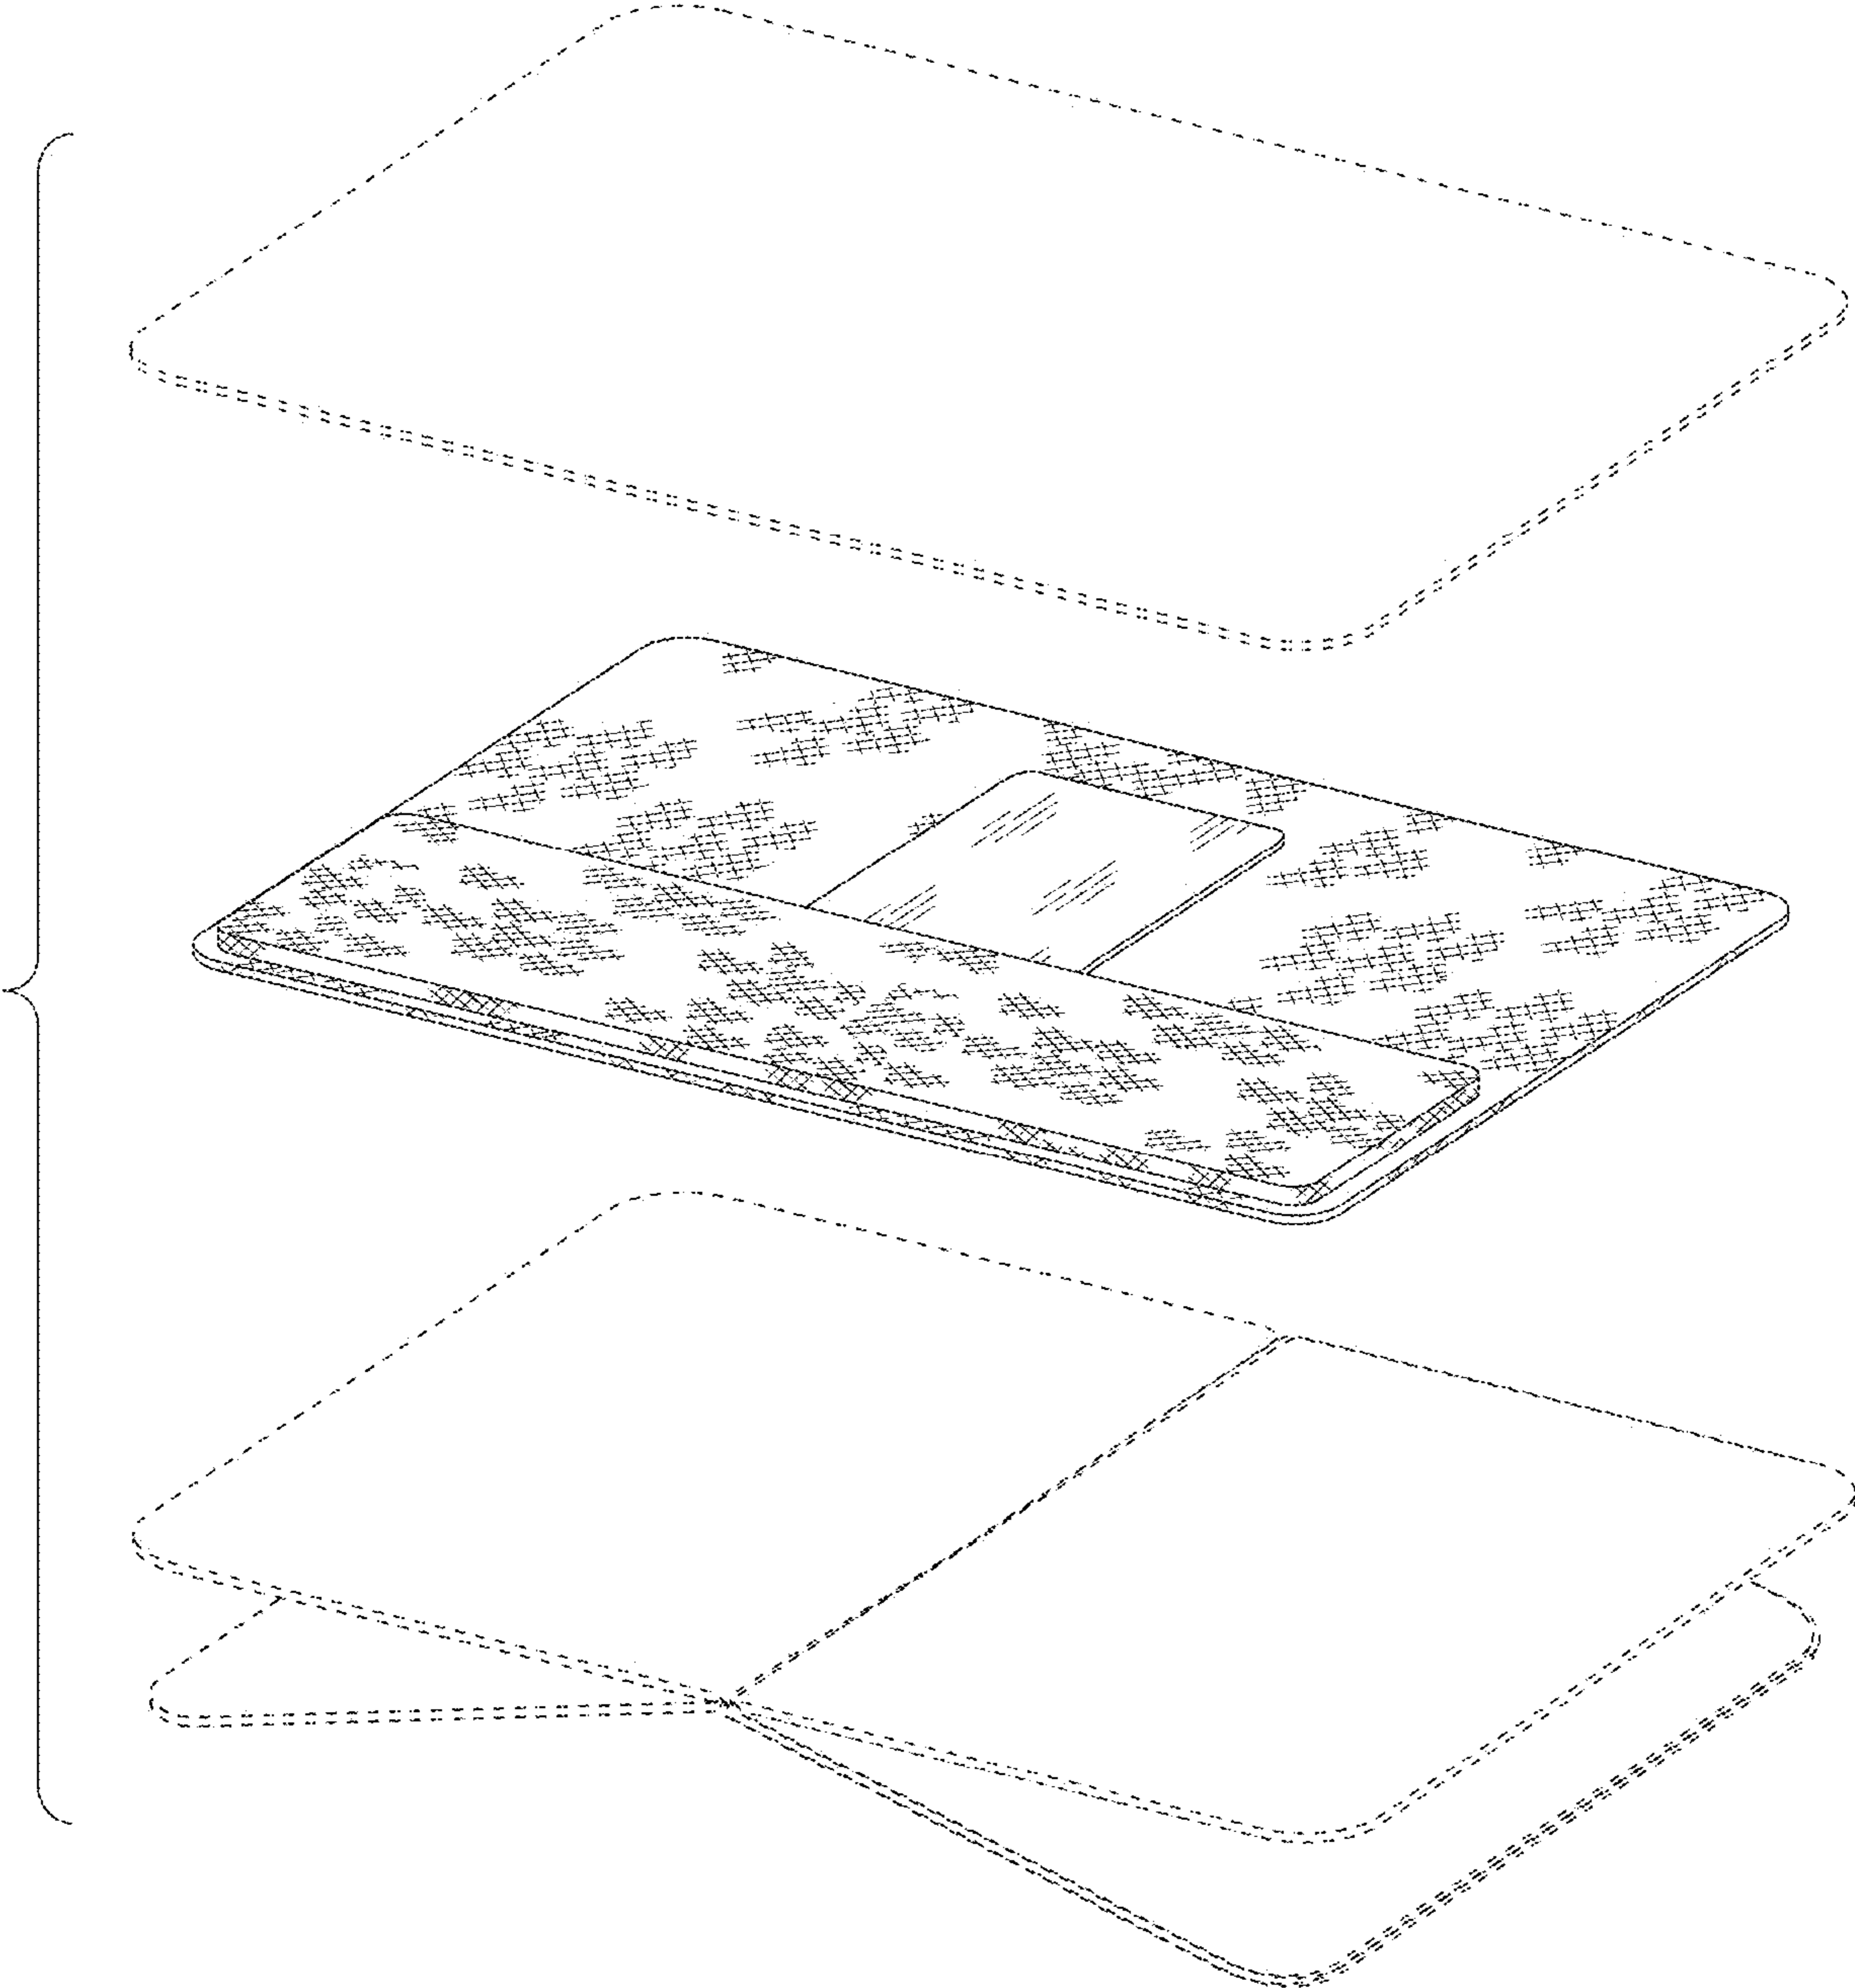


Fig. 1

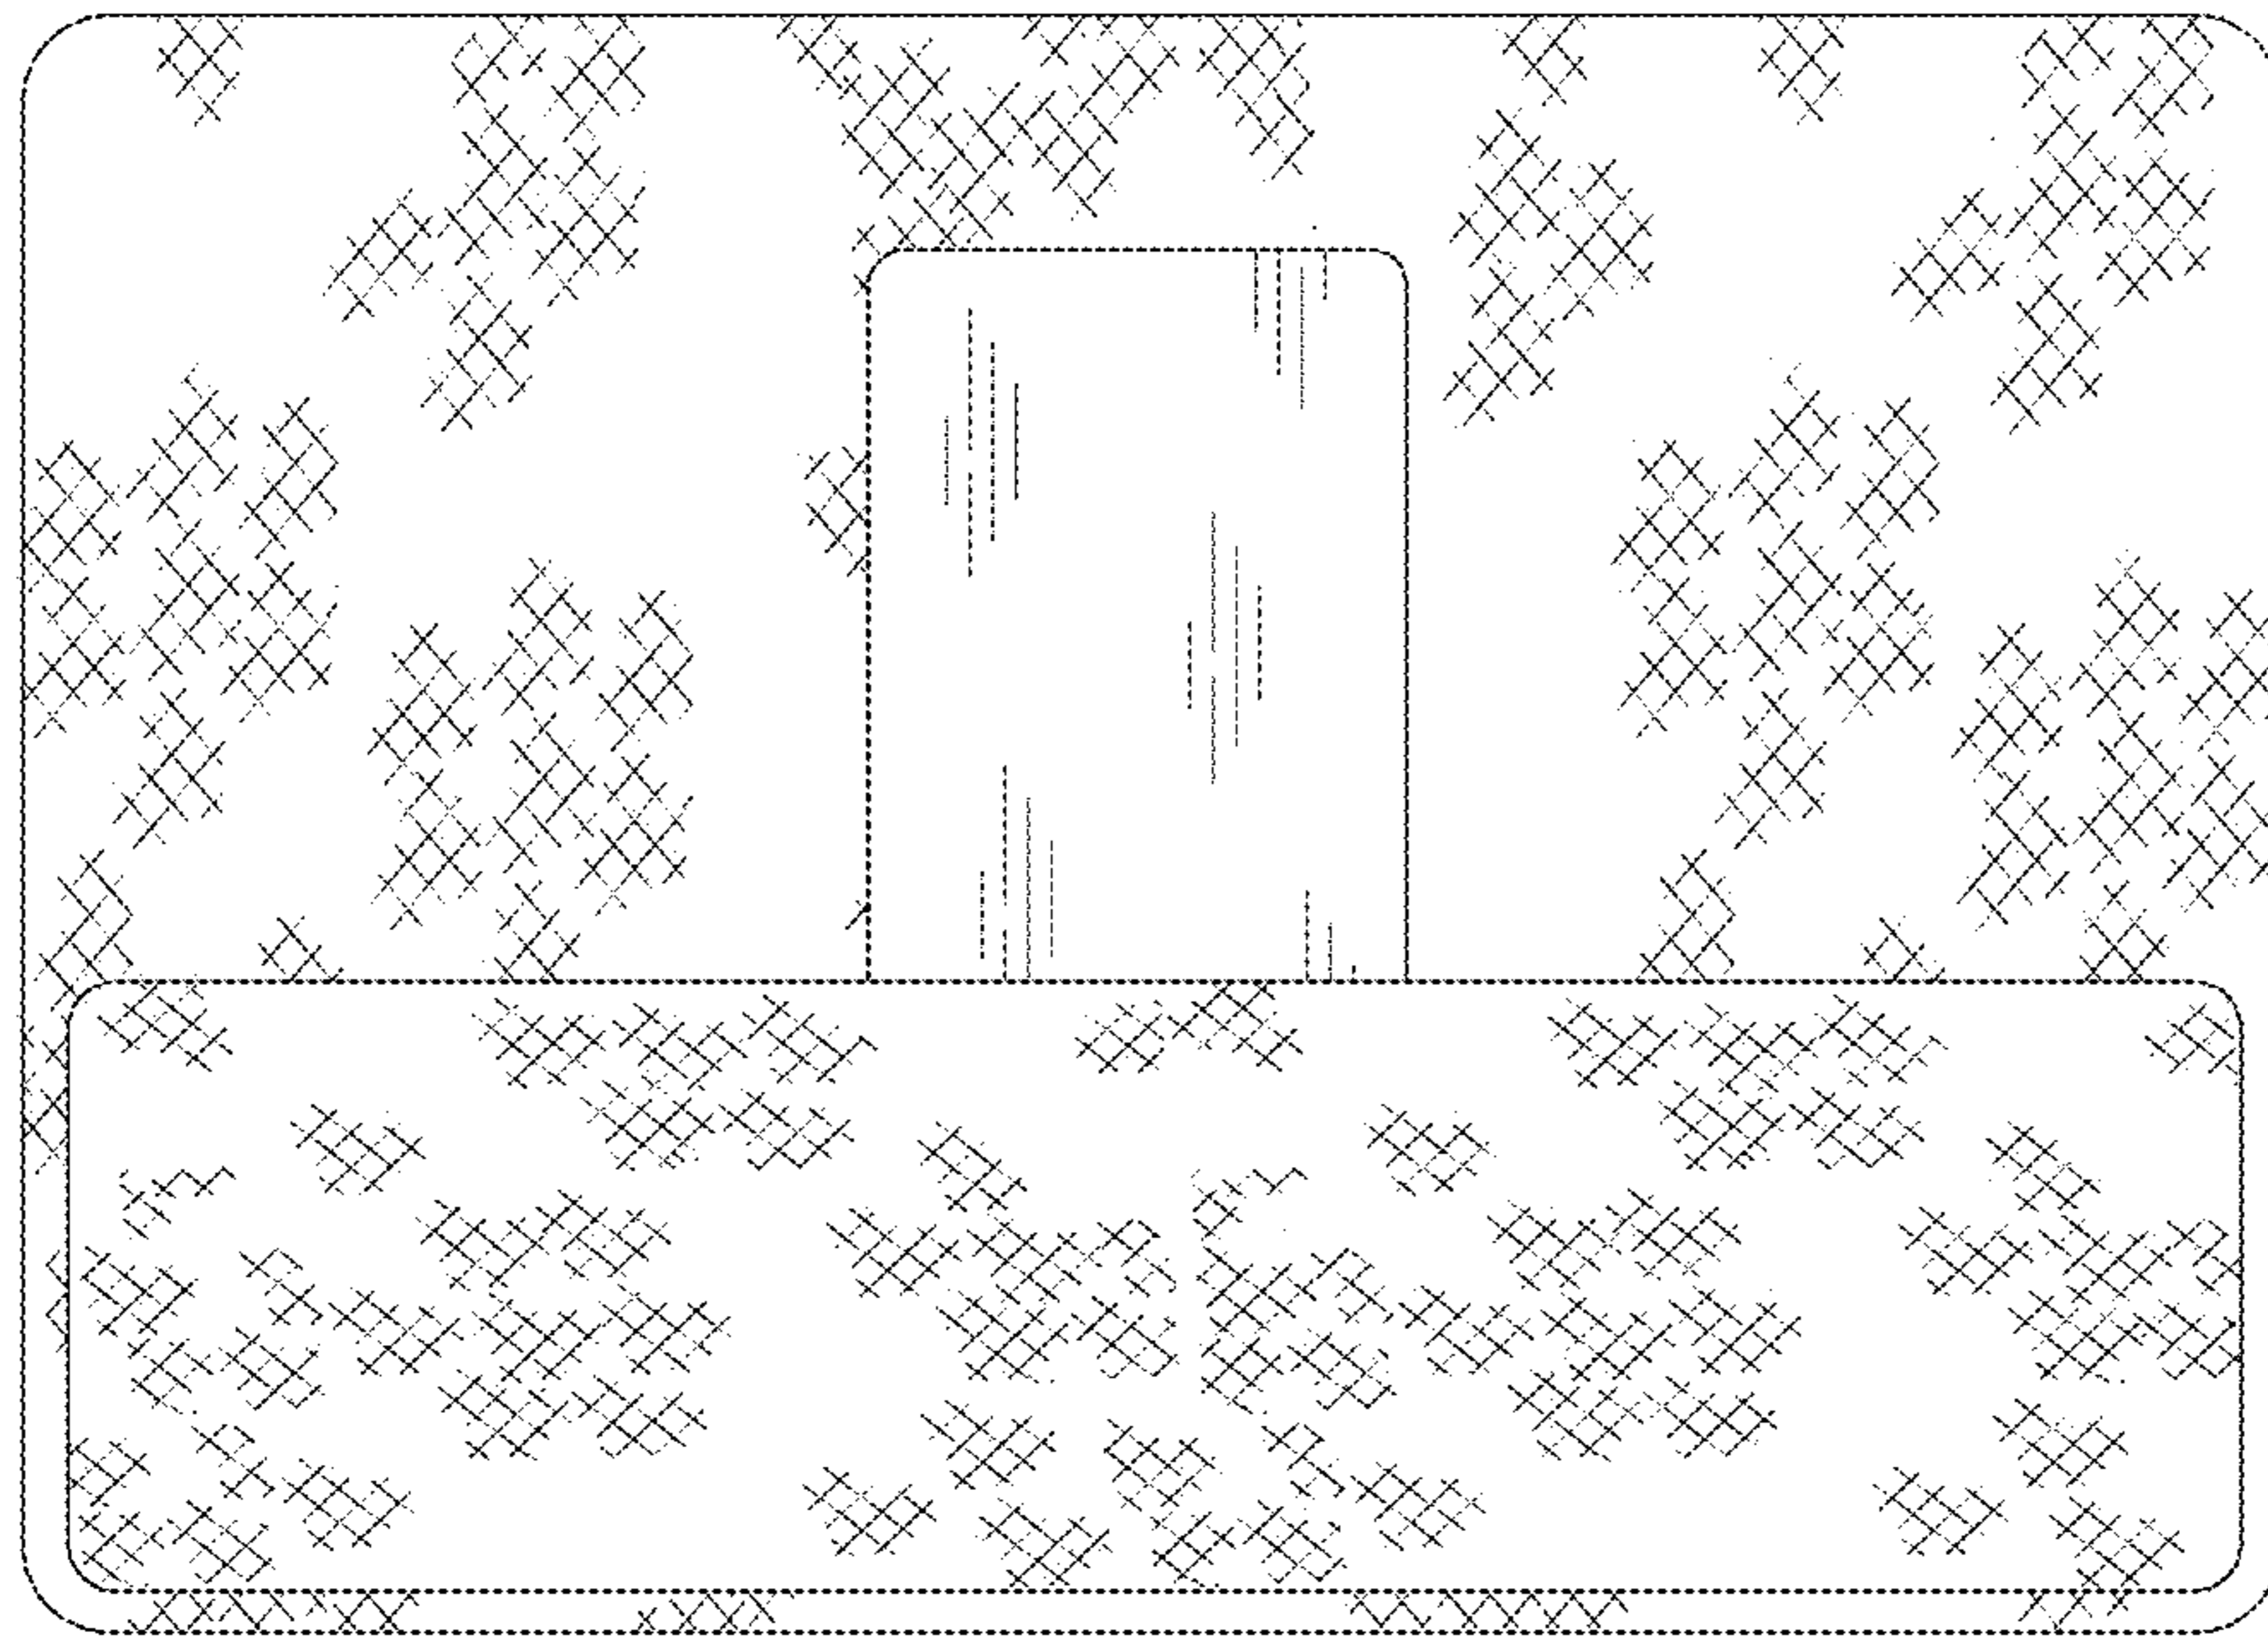


Fig. 2

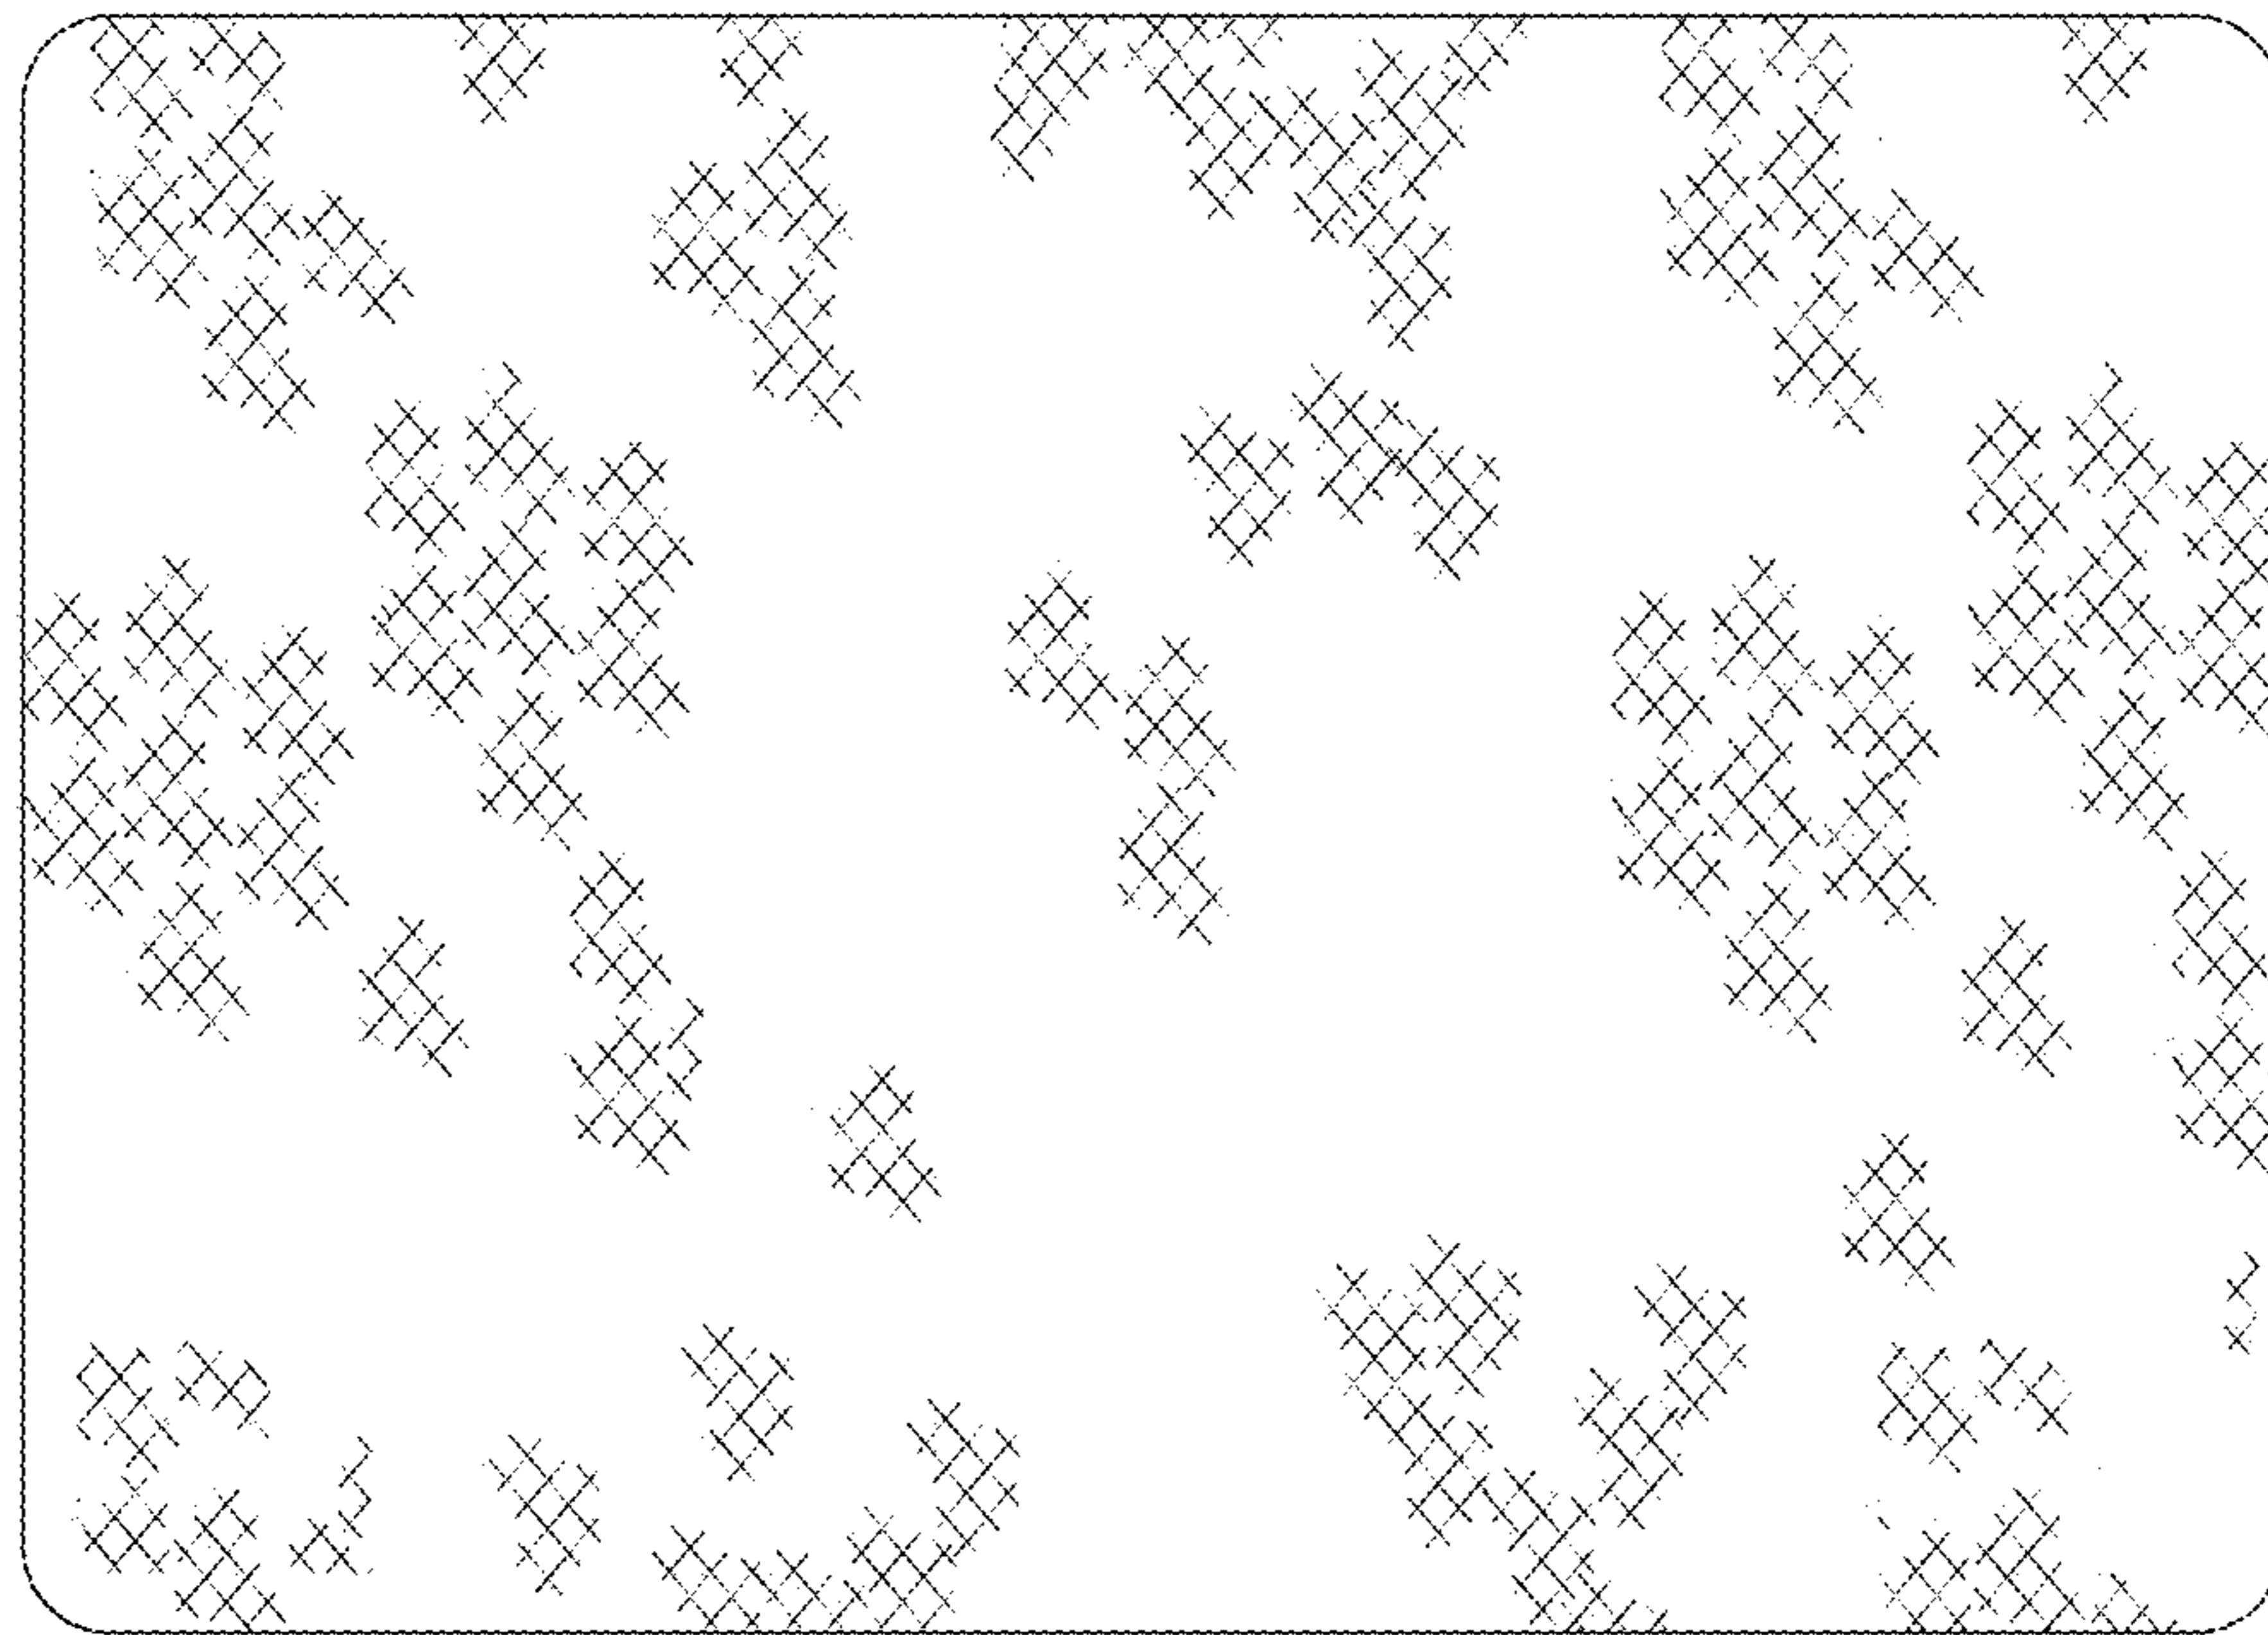


Fig. 3

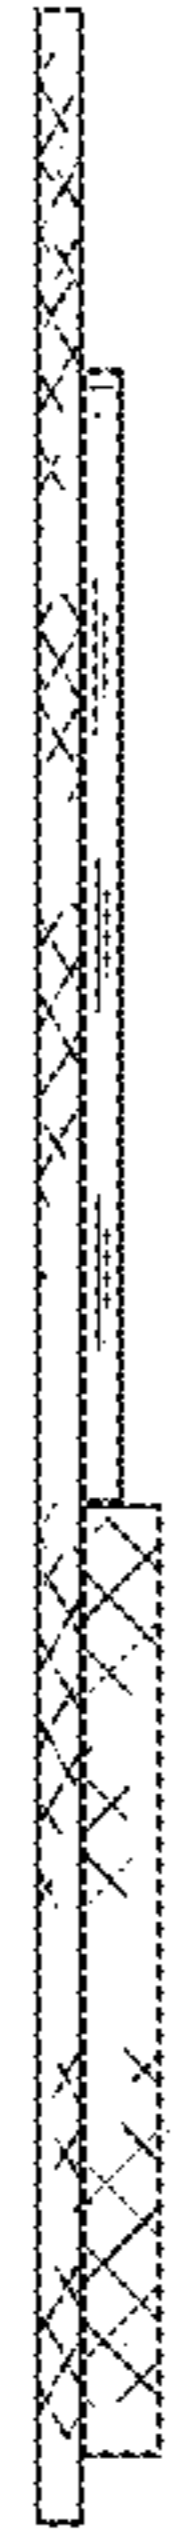


Fig. 4

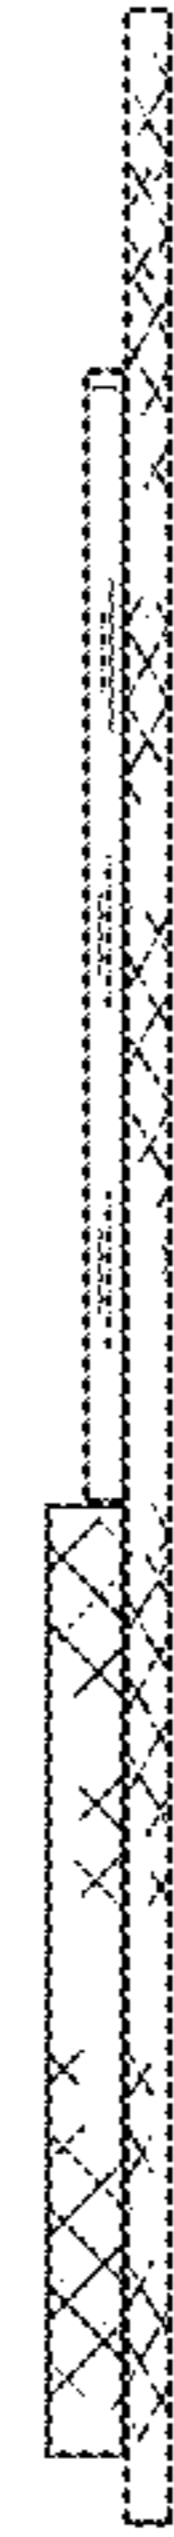


Fig. 5

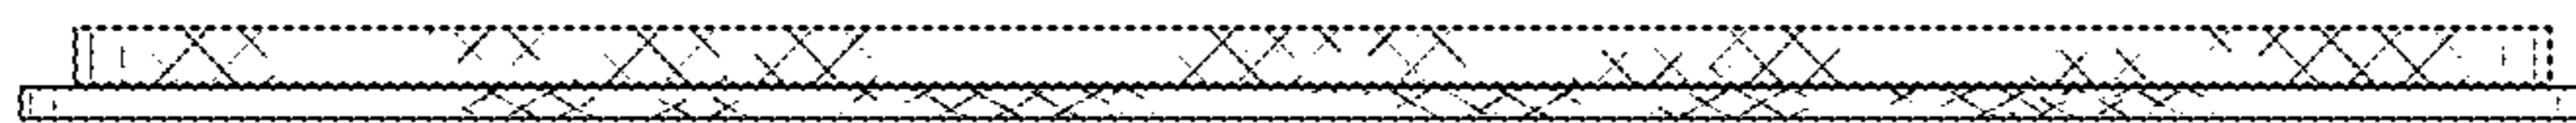


Fig. 6

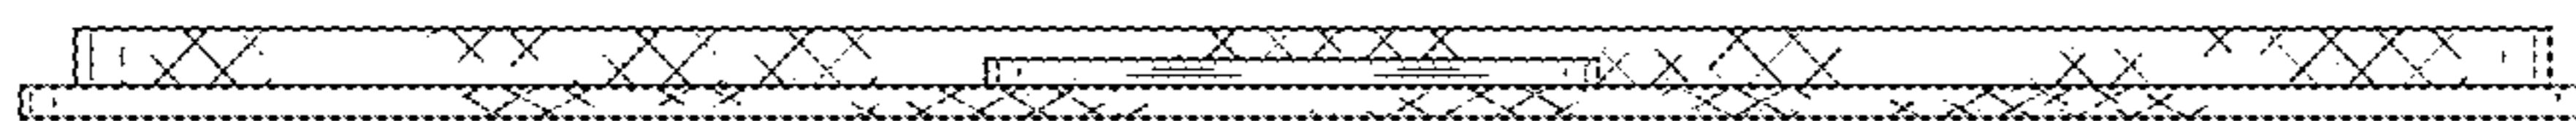


Fig. 7