



US00D977116S

(12) **United States Design Patent** (10) **Patent No.:** **US D977,116 S**  
**Gennaco et al.** (45) **Date of Patent:** **\*\* Jan. 31, 2023**

(54) **PHYSIOLOGICAL MONITOR RECEPTACLE**

(71) Applicant: **Whoop, Inc.**, Boston, MA (US)

(72) Inventors: **Jillian Gennaco**, Wakefield, MA (US);  
**Stacey K. Keetell**, Watertown, MA (US); **Stephen Ronald Gambie**,  
Brighton (GB); **Daniel Philip Wiese**,  
Cambridge, MA (US)

(73) Assignee: **Whoop, Inc.**, Boston, MA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/794,724**

(22) Filed: **Jun. 15, 2021**

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/186**

(58) **Field of Classification Search**  
USPC ..... D24/164, 165, 167, 168, 169, 186, 187,  
D24/107; D10/70; D14/344  
CPC ... A61B 5/0022; A61B 5/02055; A61B 5/282;  
A61B 5/6898; A61B 5/1112; A61B  
5/1117; A61B 5/1118; A61B 5/14532;  
A61B 5/6824; A61B 5/6829; A61B  
5/6831; A61B 5/6802; A61B 5/6803;  
A61B 5/6804; A61B 5/6807

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D567,950 S	*	4/2008	Savage, Jr.	.....	D24/186
D875,264 S	*	2/2020	Katz	.....	D24/200
D898,924 S	*	10/2020	Hinds	.....	D24/189
D927,699 S	*	8/2021	Al-Ali	.....	D24/187
D928,330 S	*	8/2021	Itagaki	.....	D24/187
D939,699 S	*	12/2021	Lam	.....	D24/134
D952,863 S	*	5/2022	Rodriguez	.....	D24/186

2014/0189928	A1*	7/2014	Oleson	.....	A61B 5/6804 600/388
2018/0235526	A1*	8/2018	Jones	.....	A61B 5/6833
2018/0295897	A1*	10/2018	Donohoe	.....	A61B 5/681
2022/0117504	A1*	4/2022	Gennaco	.....	A61B 5/0205

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Strategic Patents, P.C.


(57) **CLAIM**

The ornamental design for a physiological monitor receptacle, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a design for a physiological monitor receptacle;  
 FIG. 2 is a front view thereof;  
 FIG. 3 is a rear view thereof;  
 FIG. 4 is a left side view thereof;  
 FIG. 5 is a right side view thereof;  
 FIG. 6 is a top view thereof;  
 FIG. 7 is a bottom view thereof;  
 FIG. 8 is a rear perspective view thereof showing a movable flap in a first open position to demonstrate movement of the movable flap;  
 FIG. 9 is a rear perspective view thereof showing a movable flap in a second open position to demonstrate movement of the movable flap;  
 FIG. 10 is a rear perspective view thereof engaged with unclaimed apparel; and,  
 FIG. 11 is a front perspective view thereof engaged with unclaimed apparel.  
 The broken lines showing the apparel in FIGS. 10 and 11 represent environmental subject matter and form no part of the claimed design; the remaining broken lines depict portions of the physiological monitor receptacle that form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

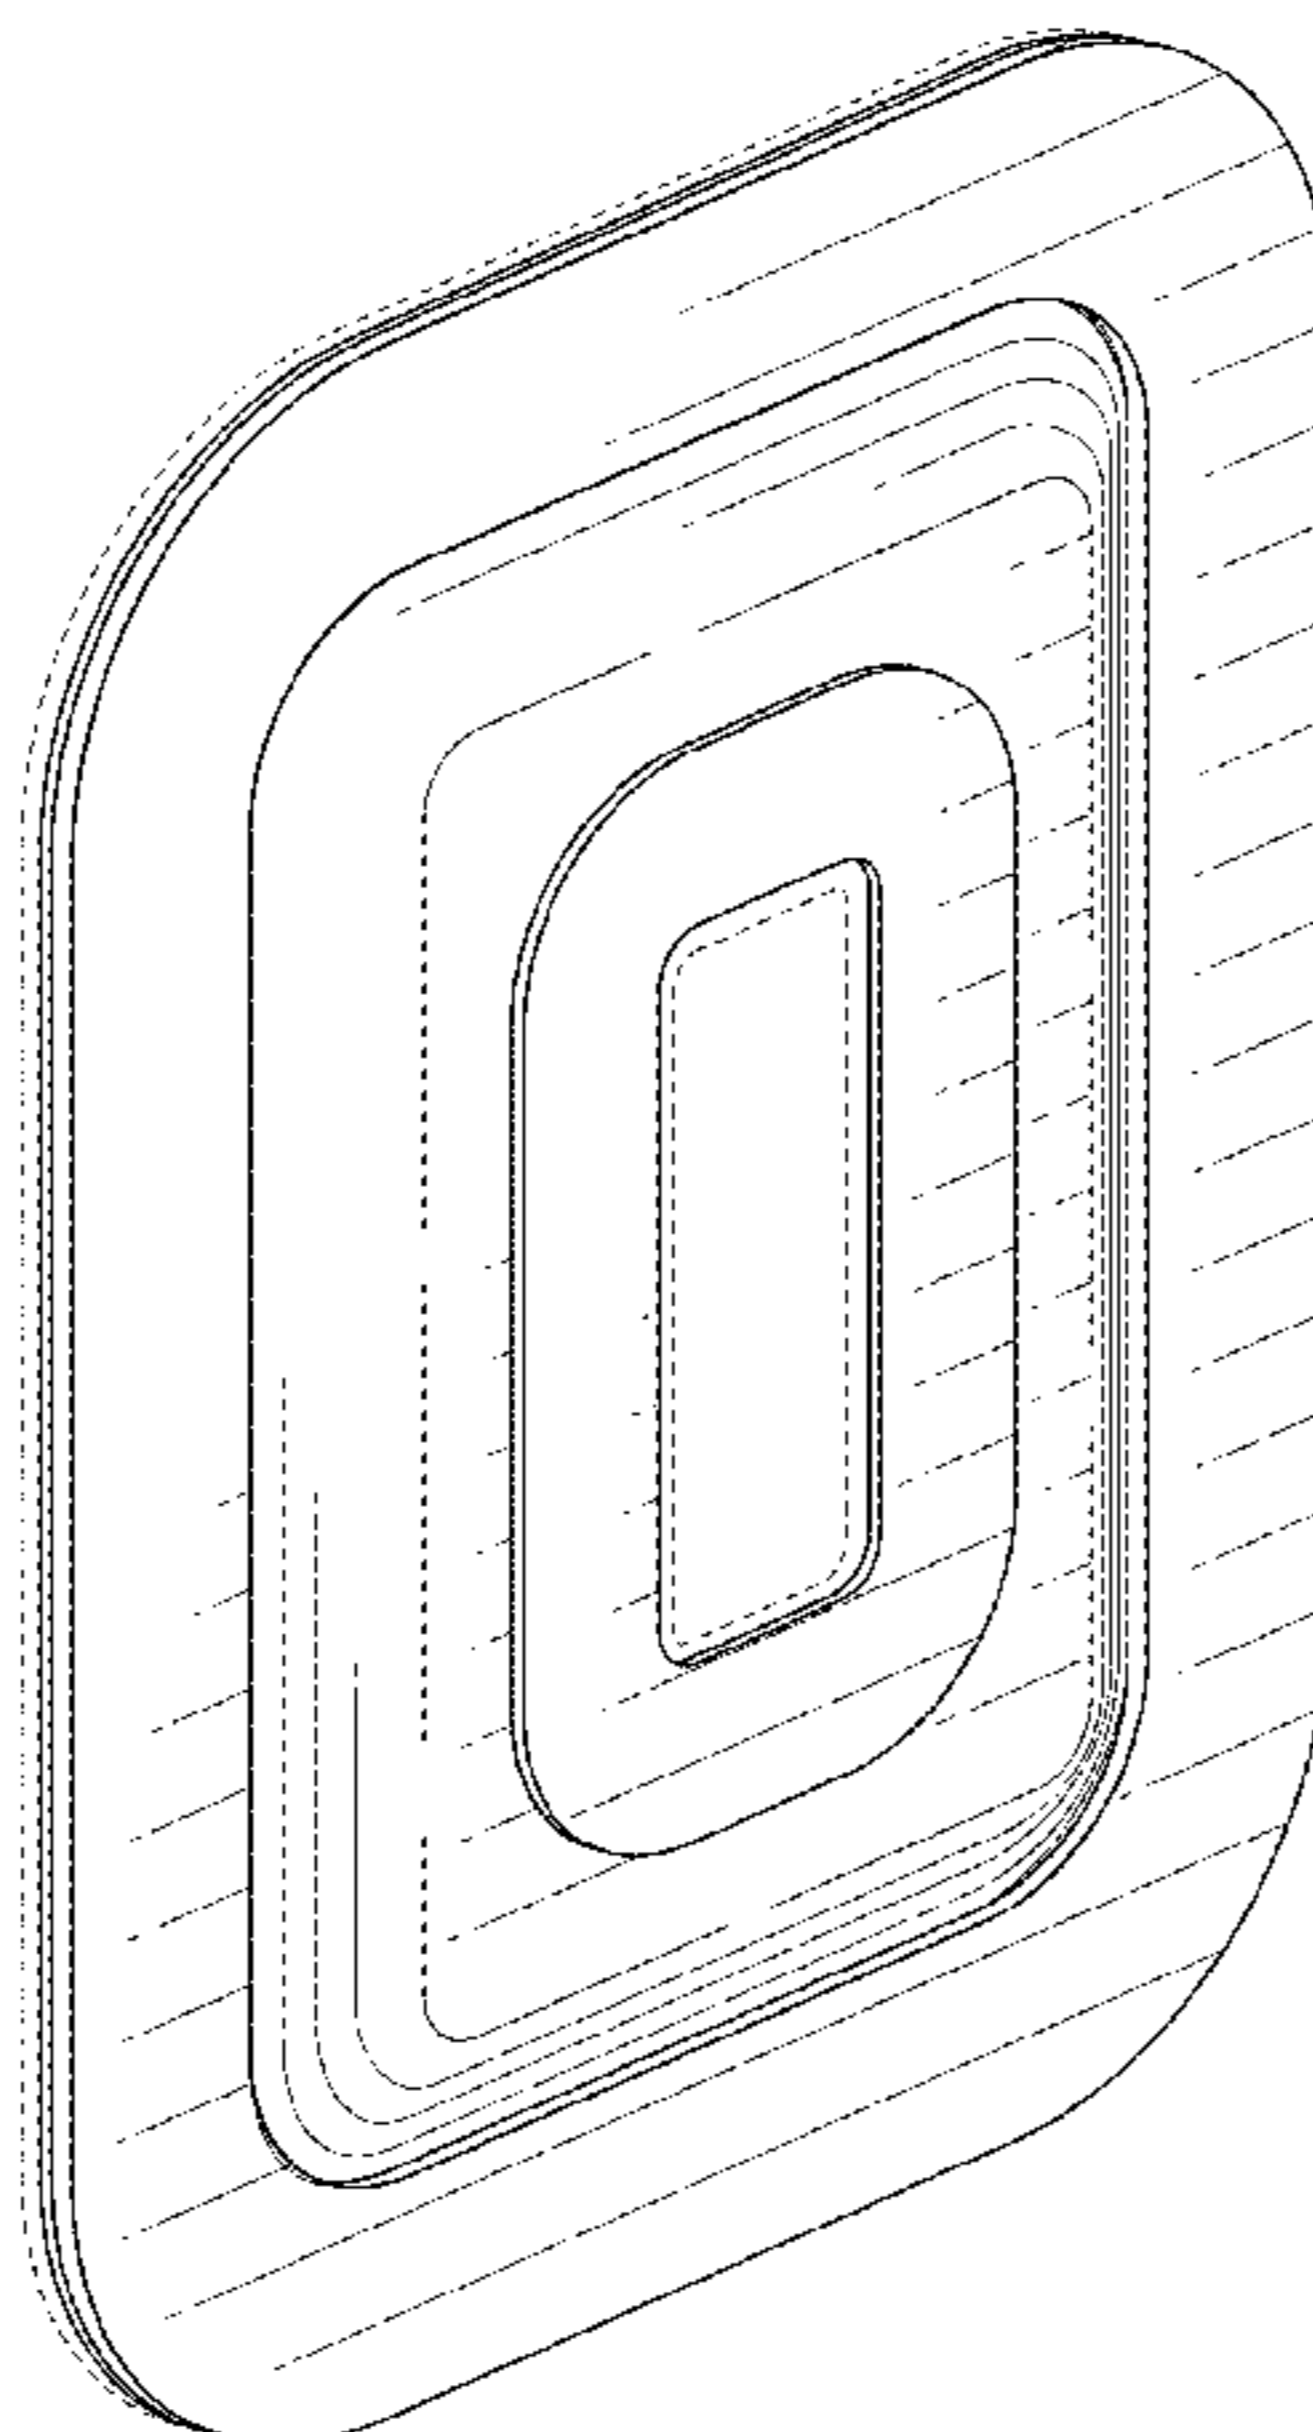

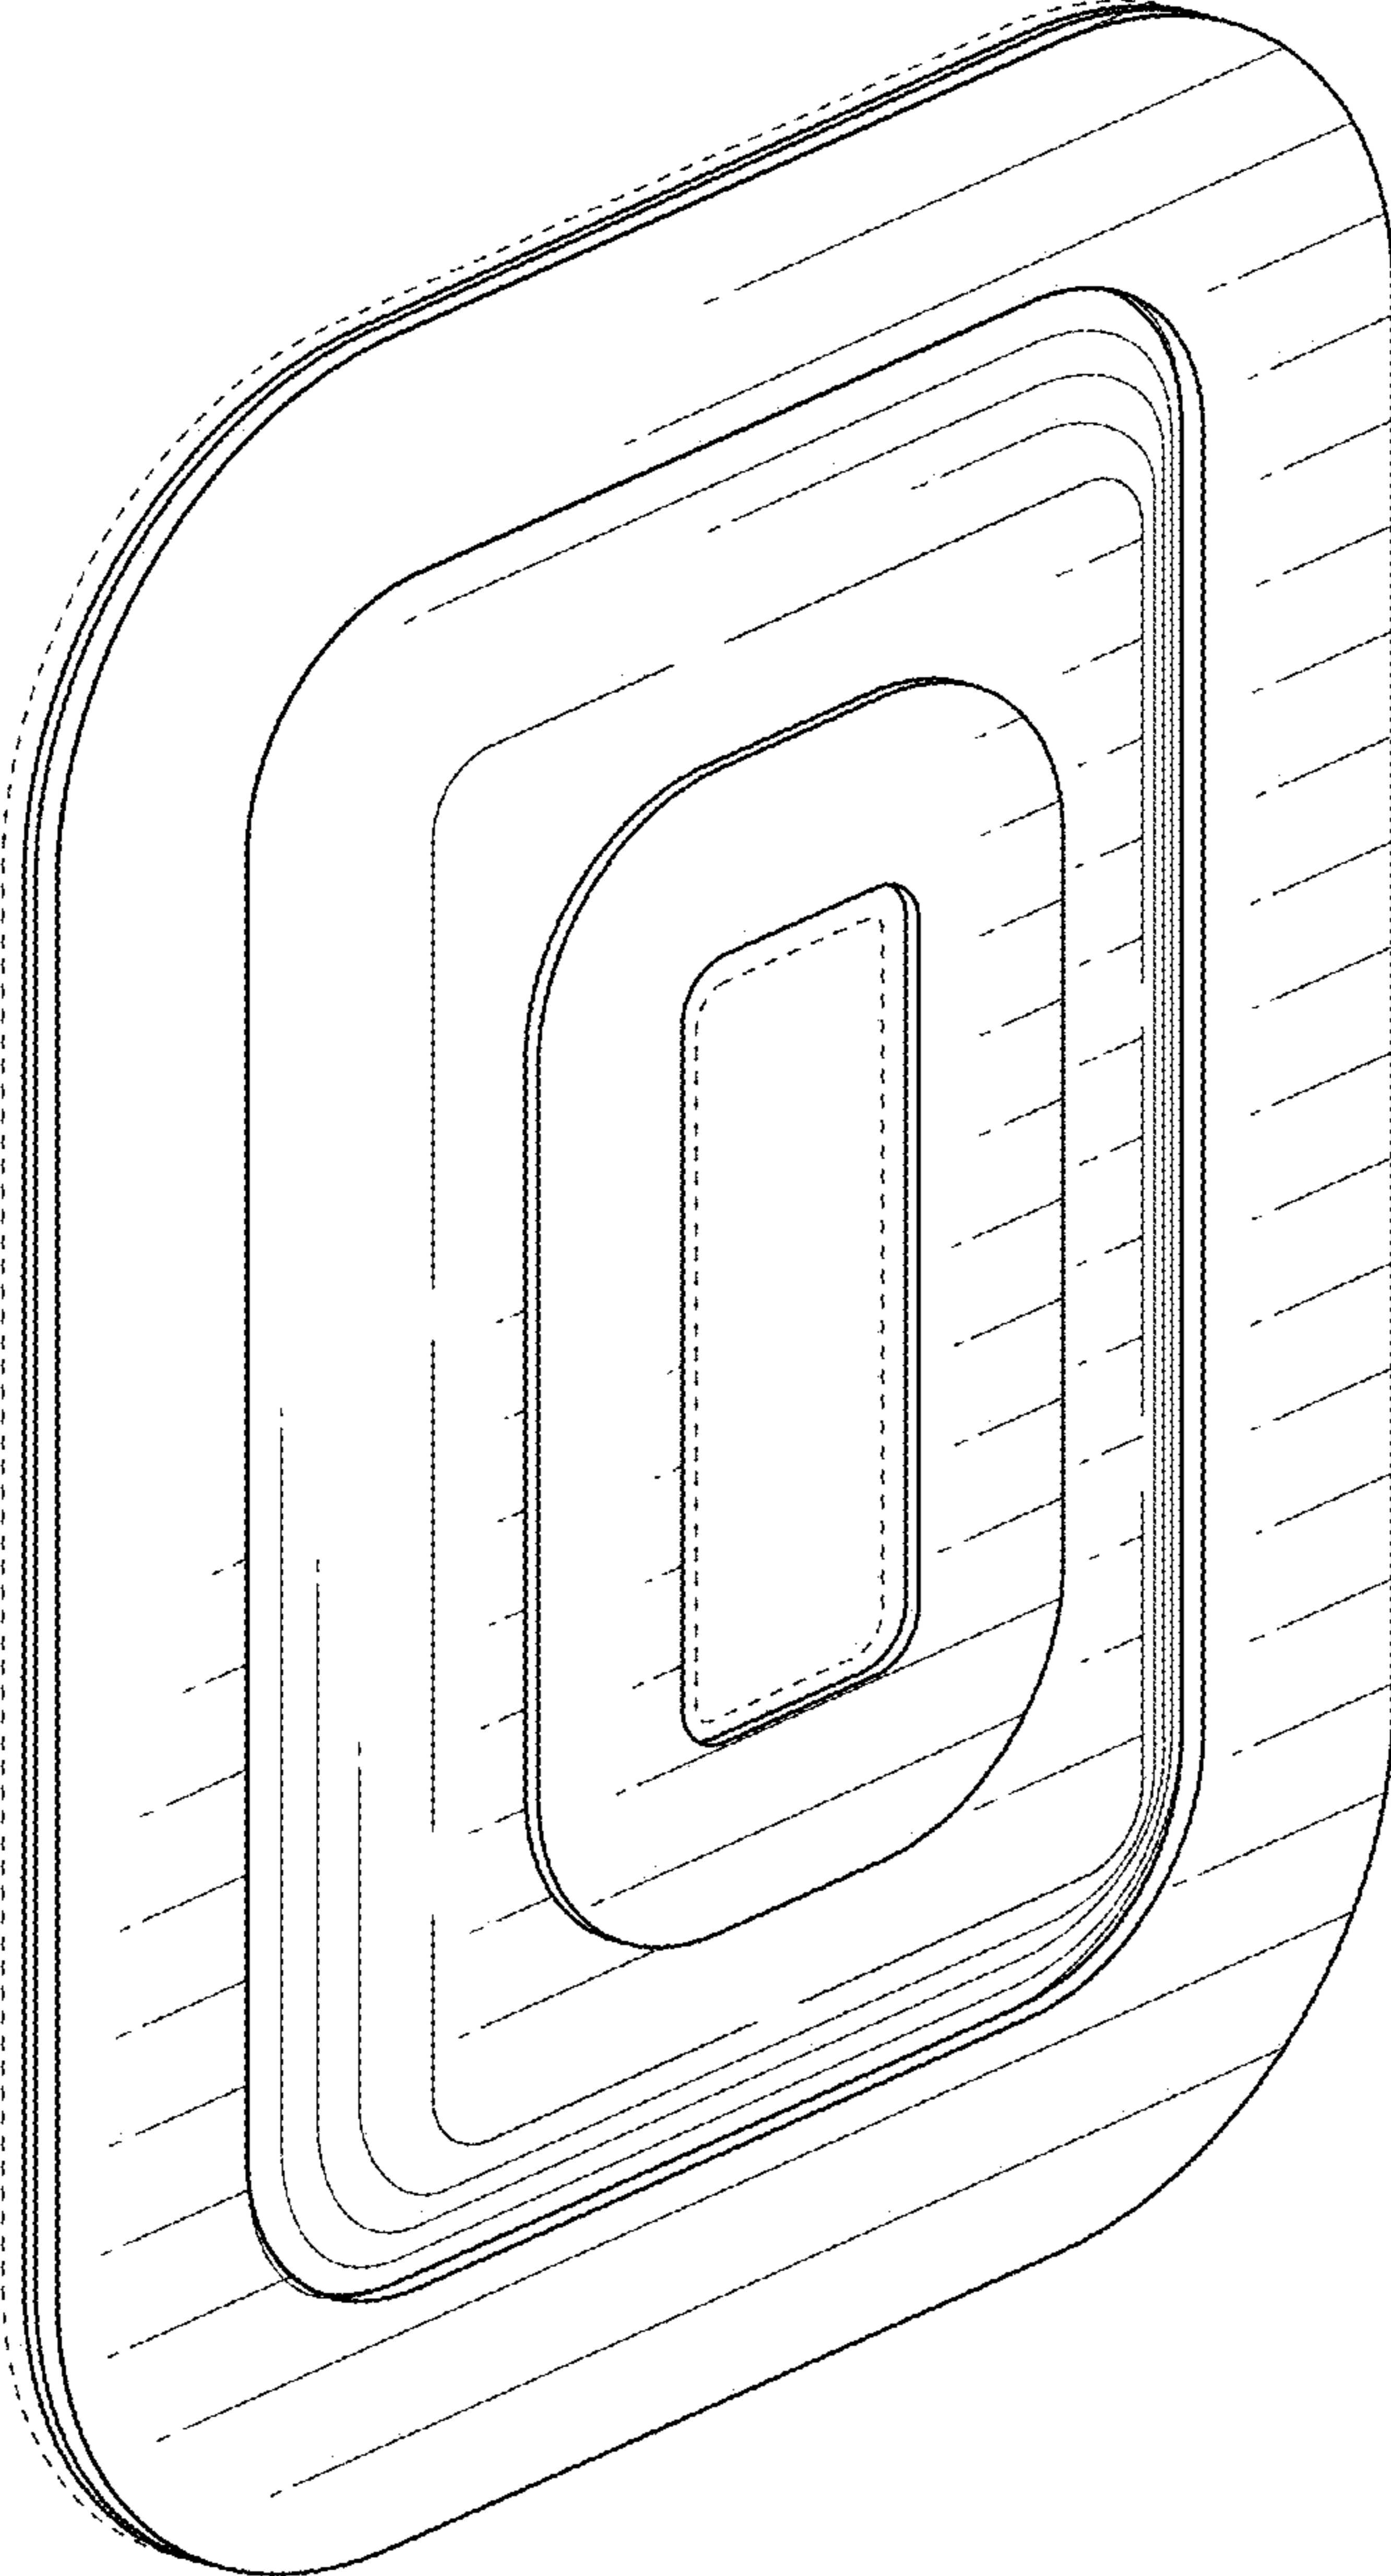


FIG. 1

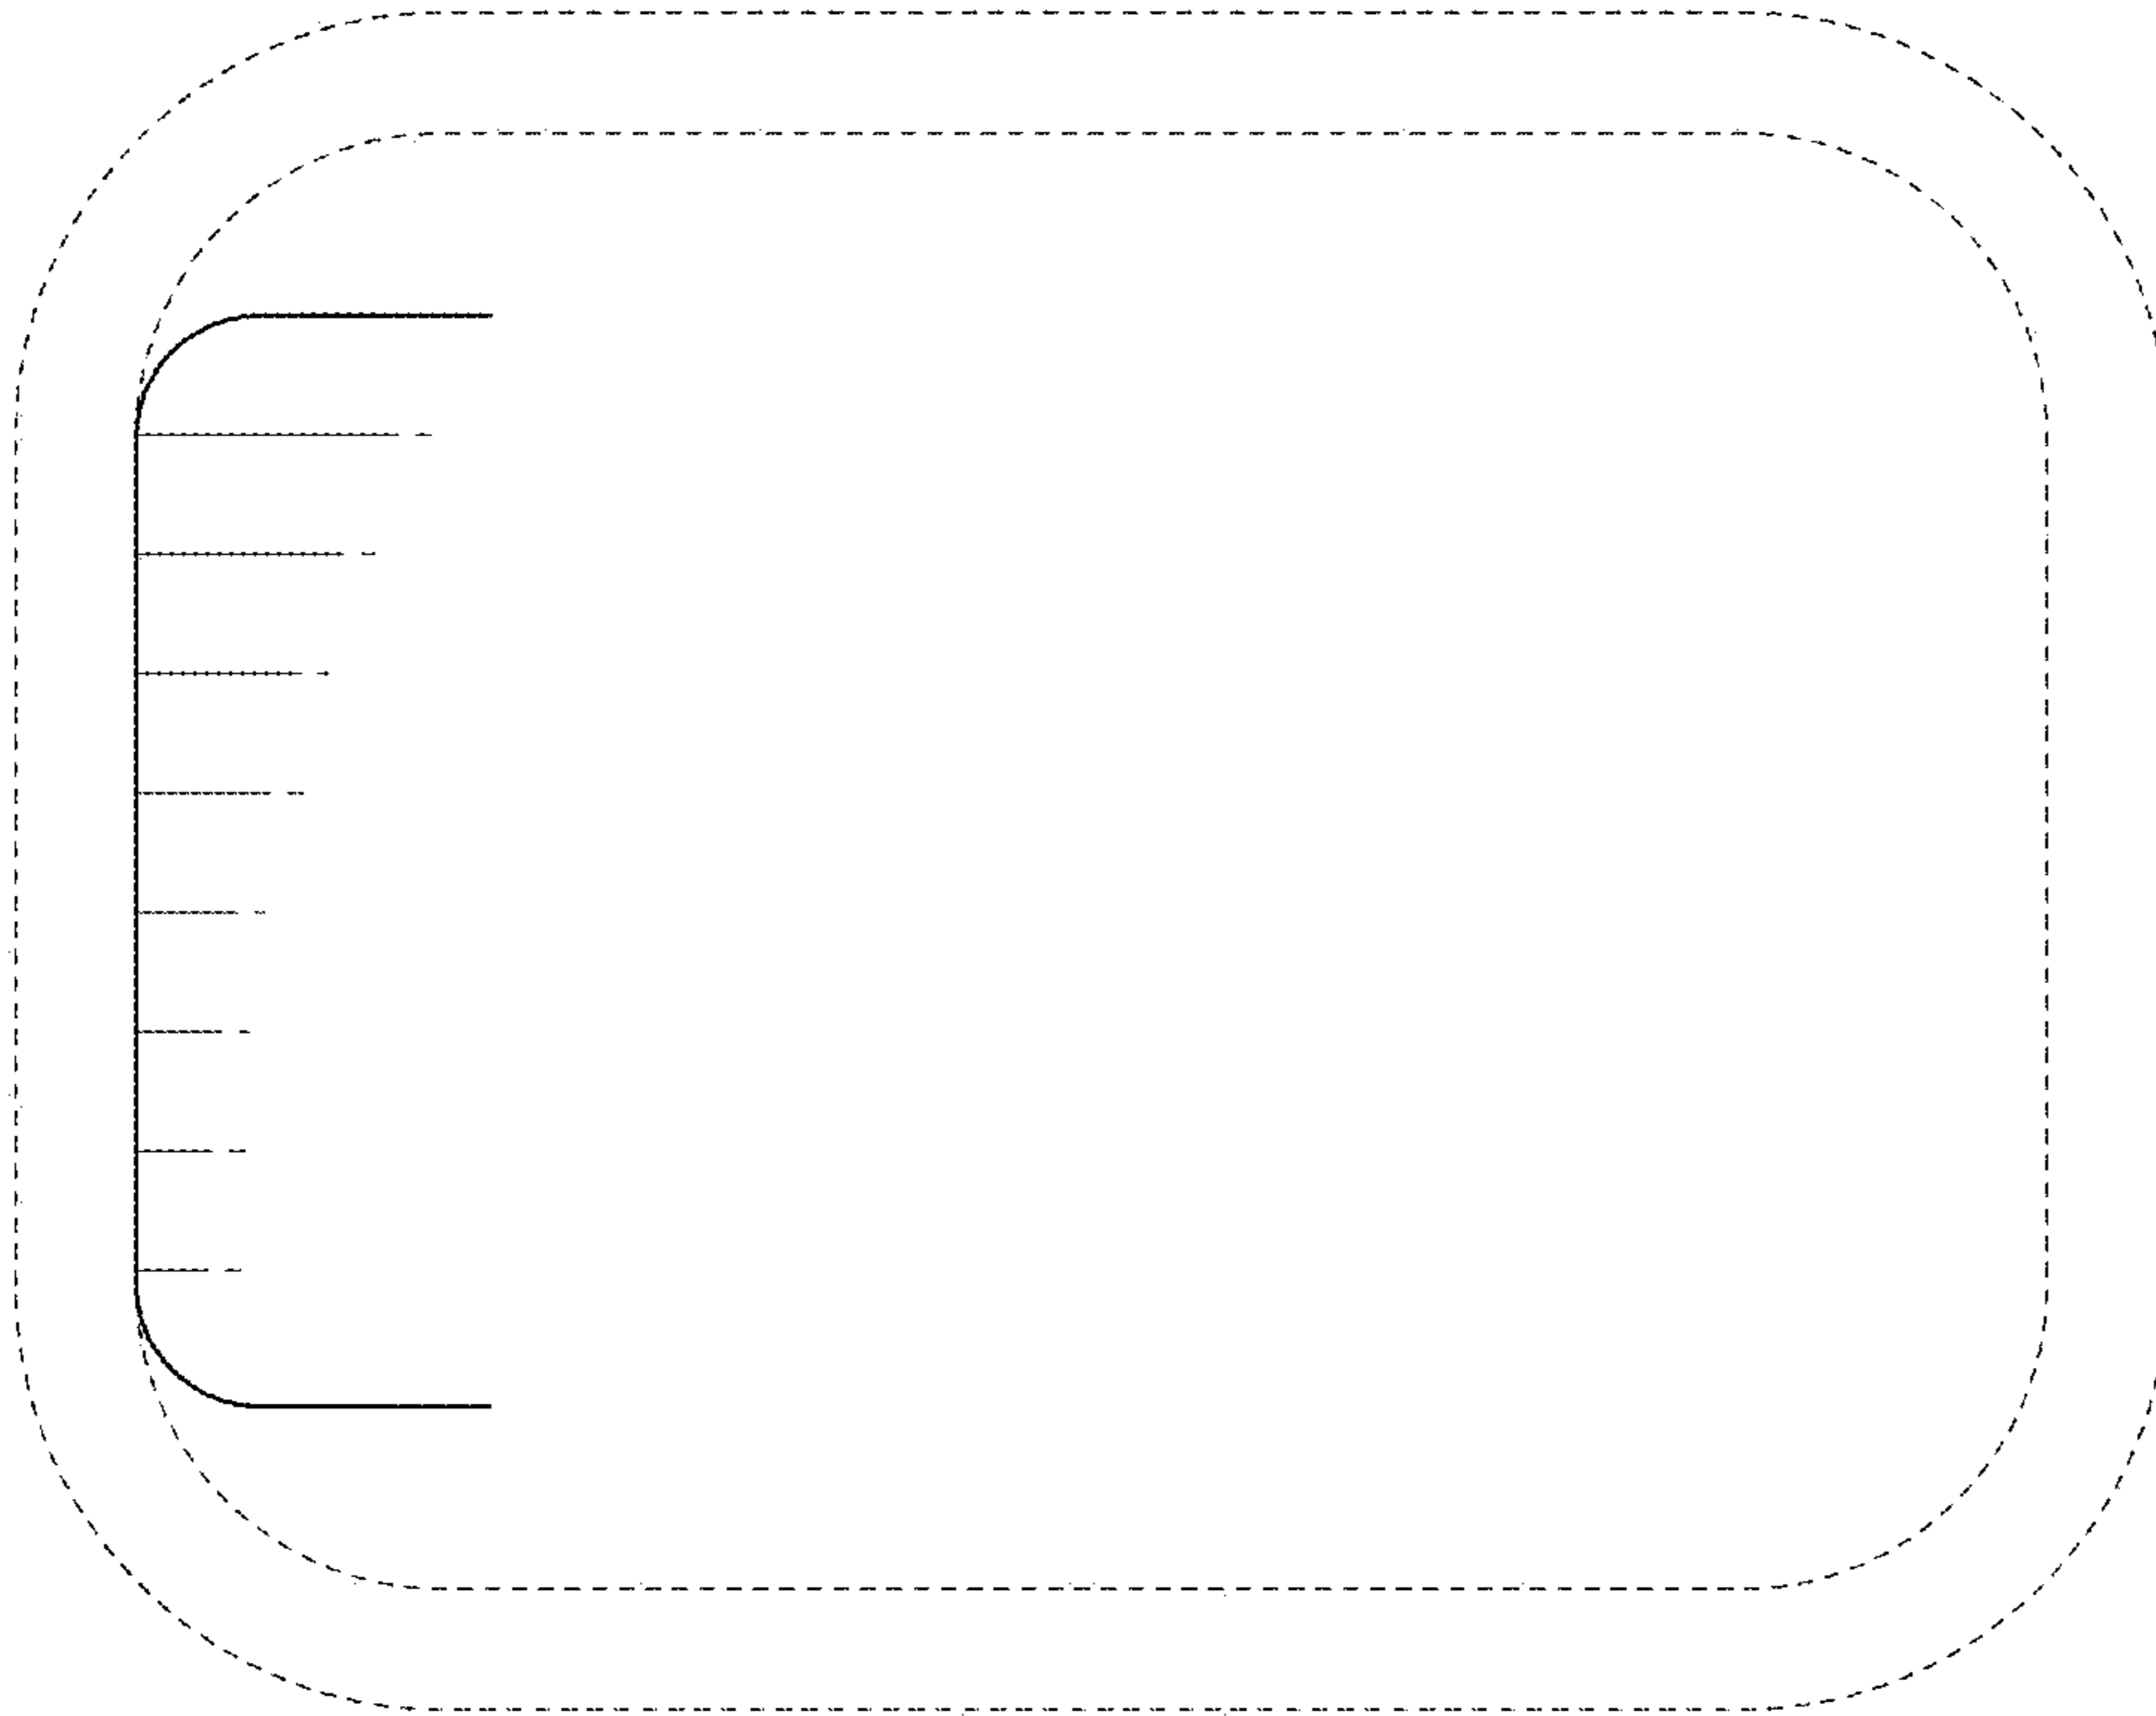


FIG. 3

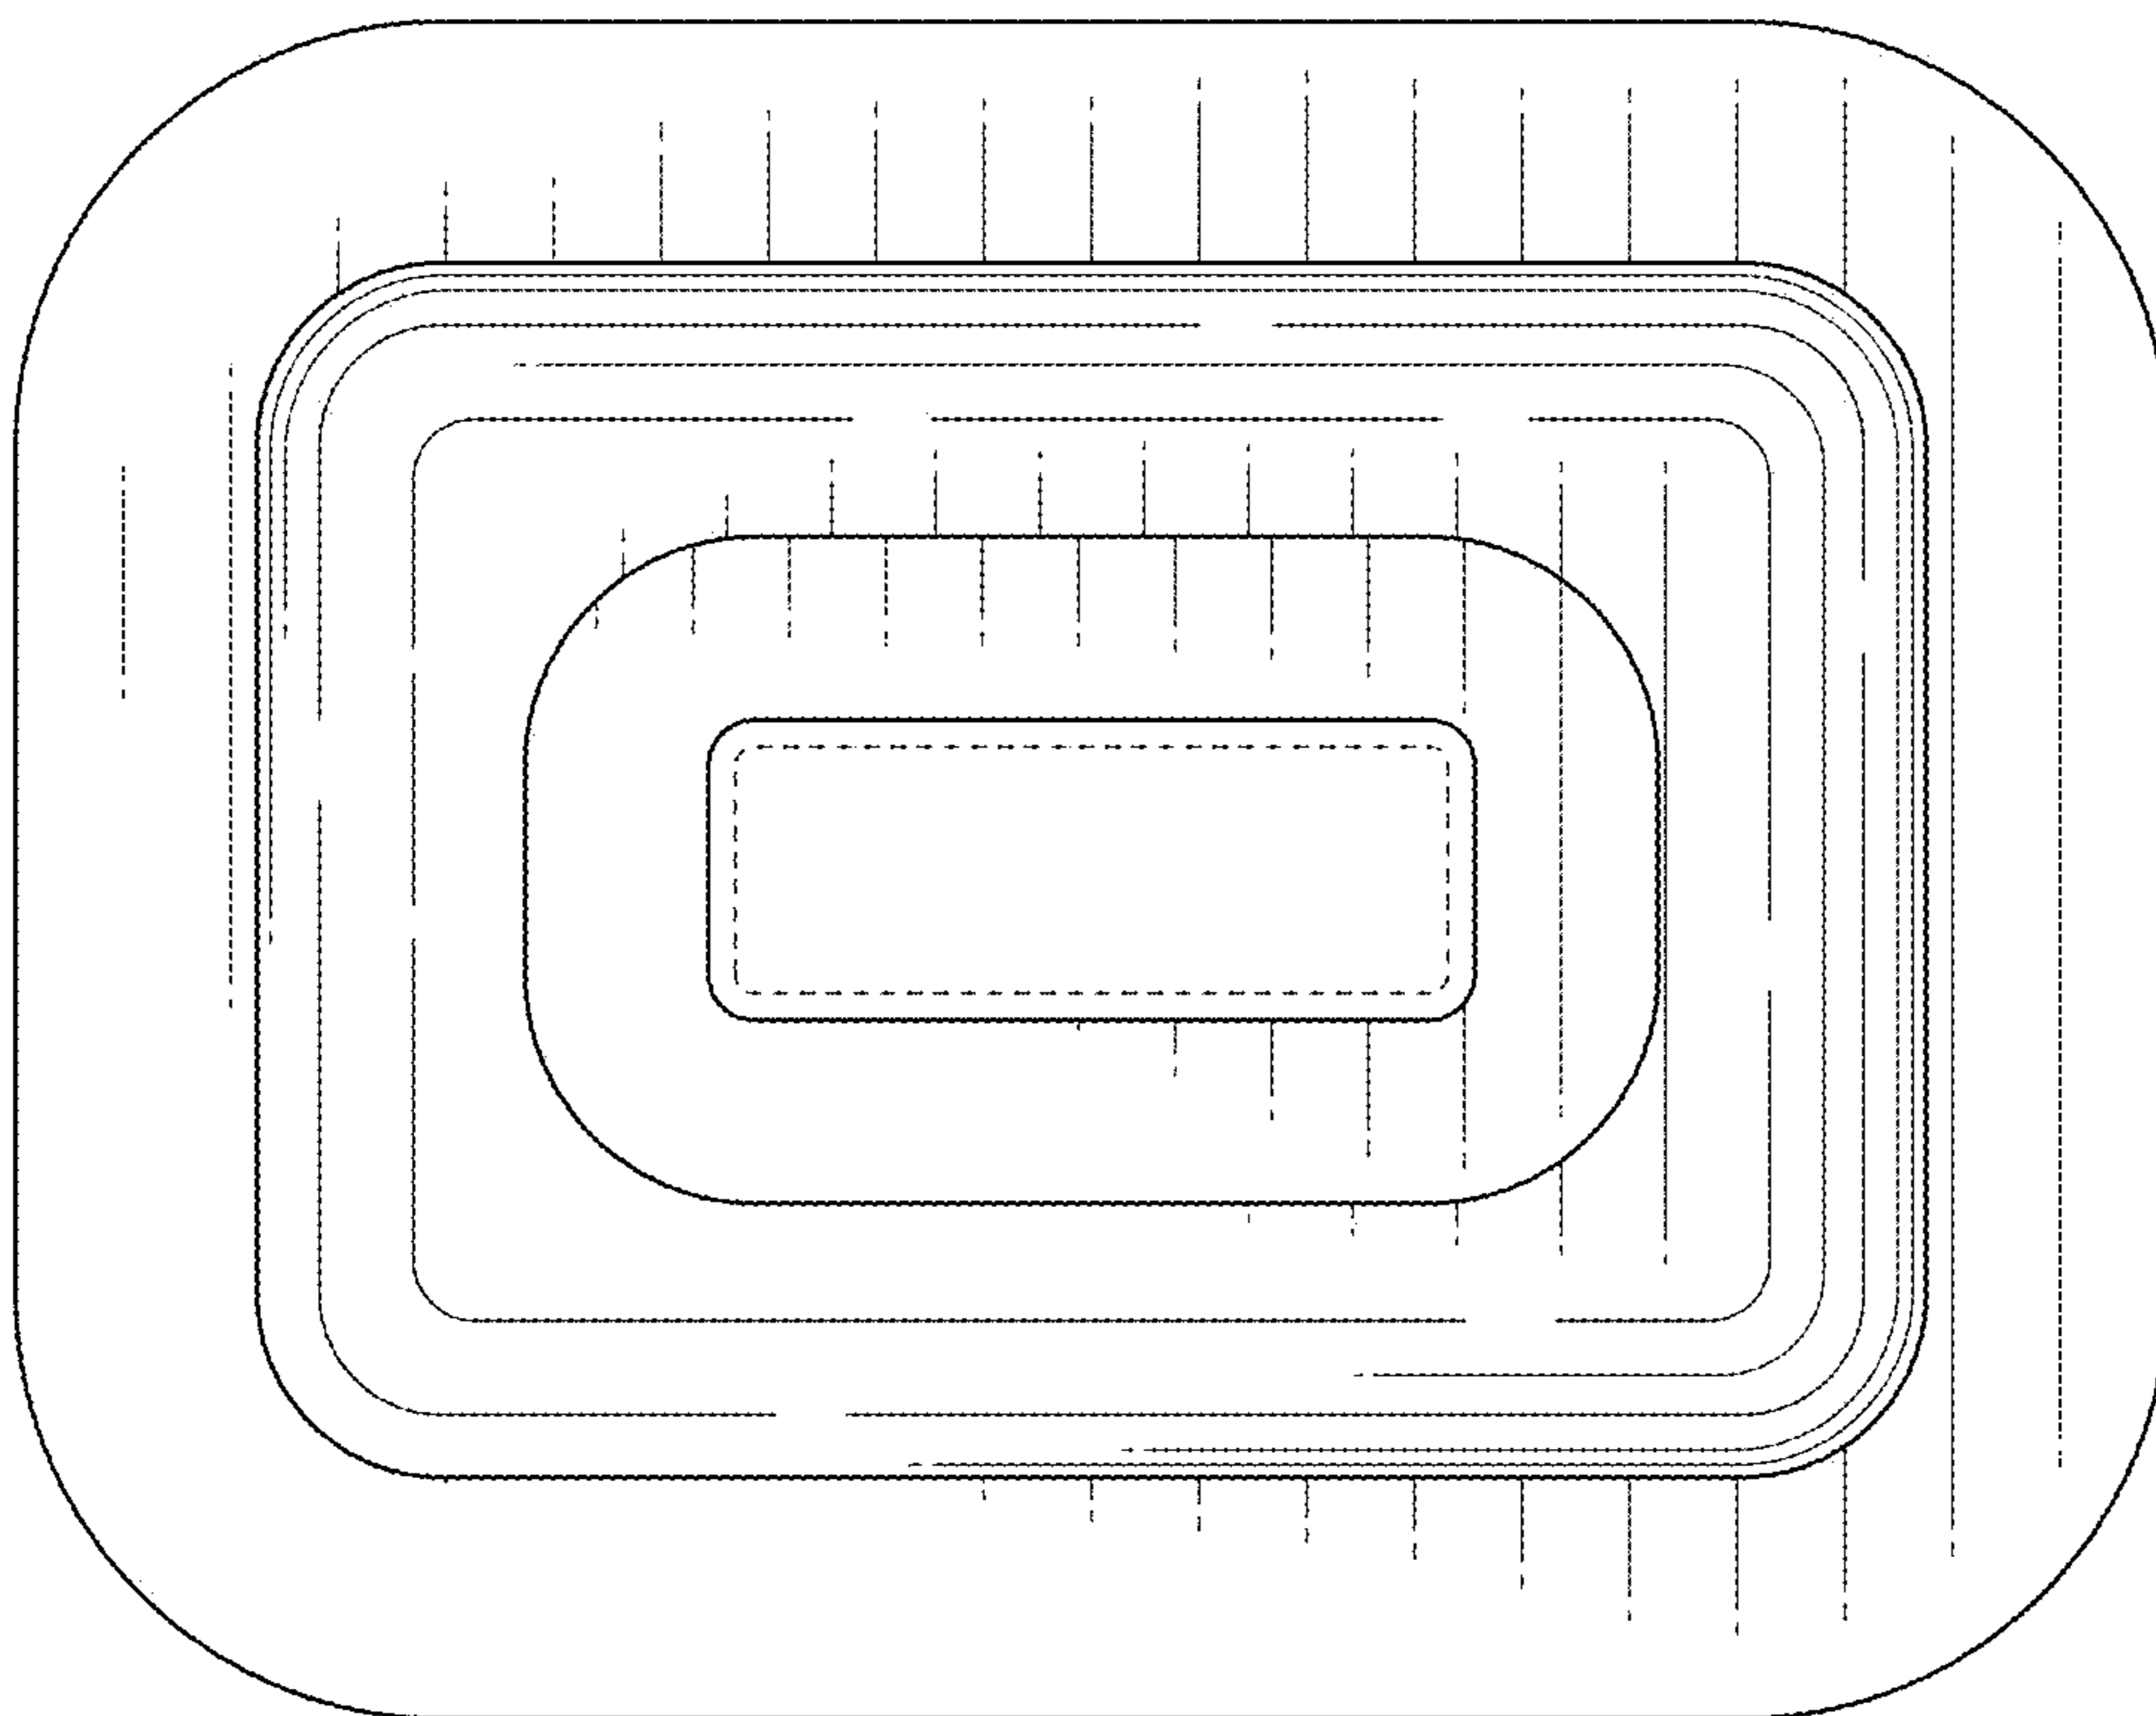


FIG. 2



FIG. 4

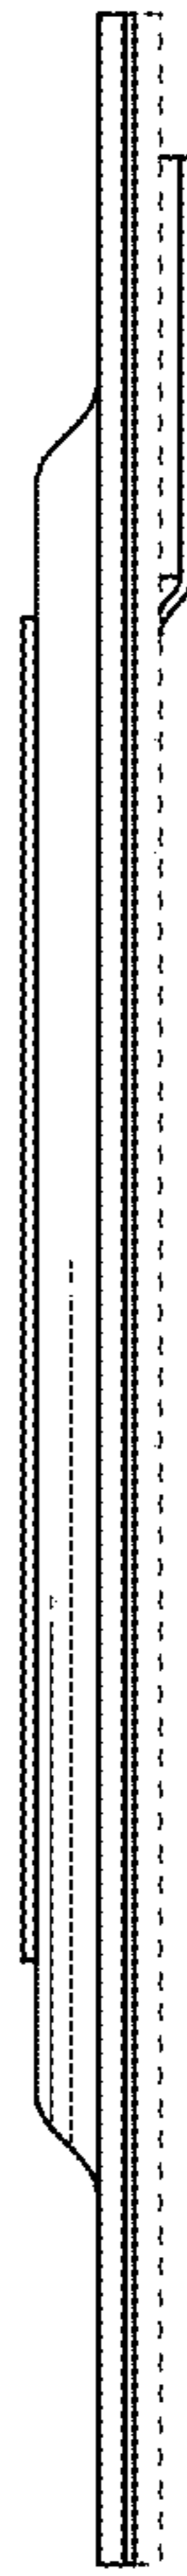


FIG. 5

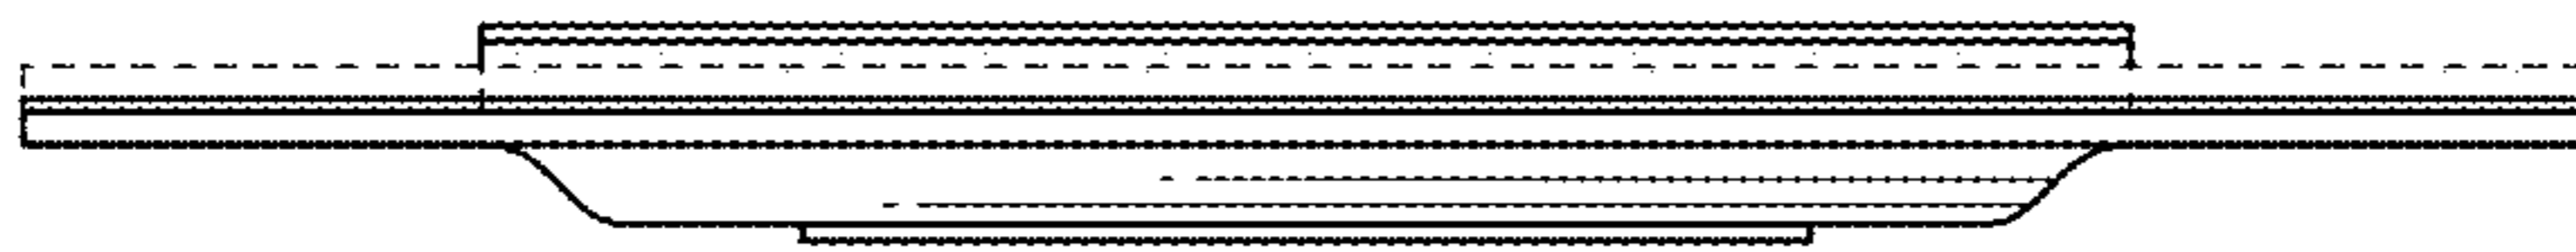


FIG. 6



FIG. 7

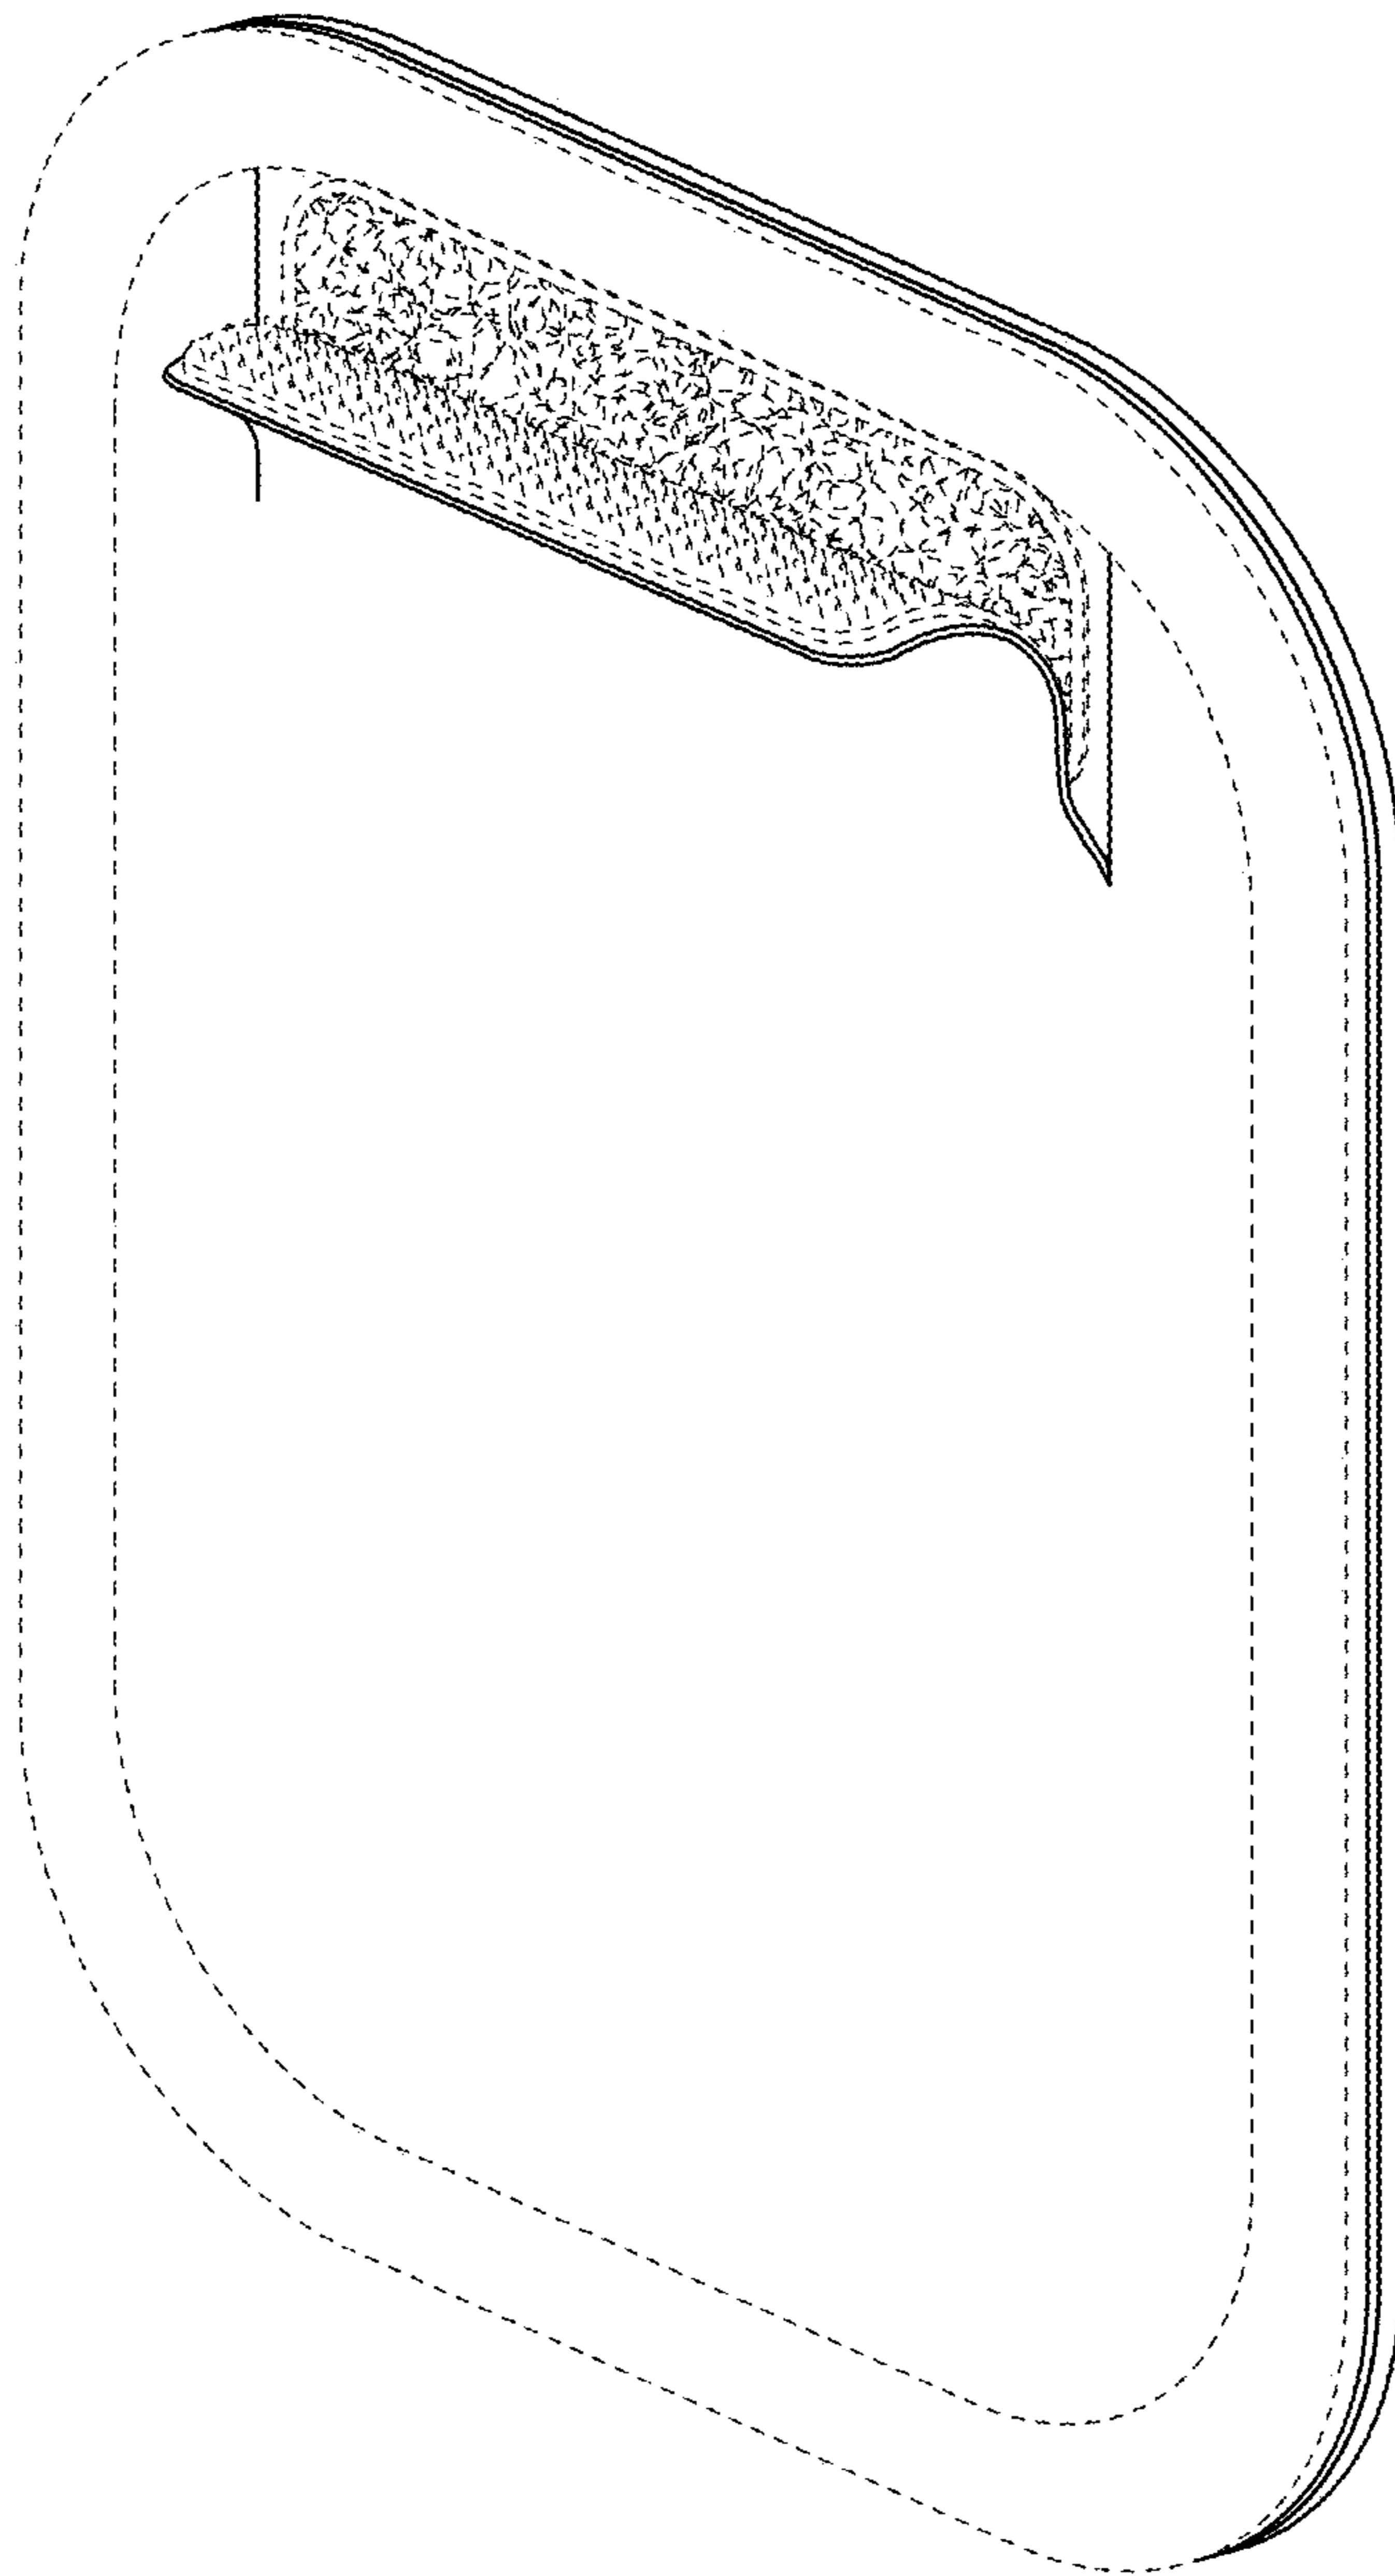


FIG. 8

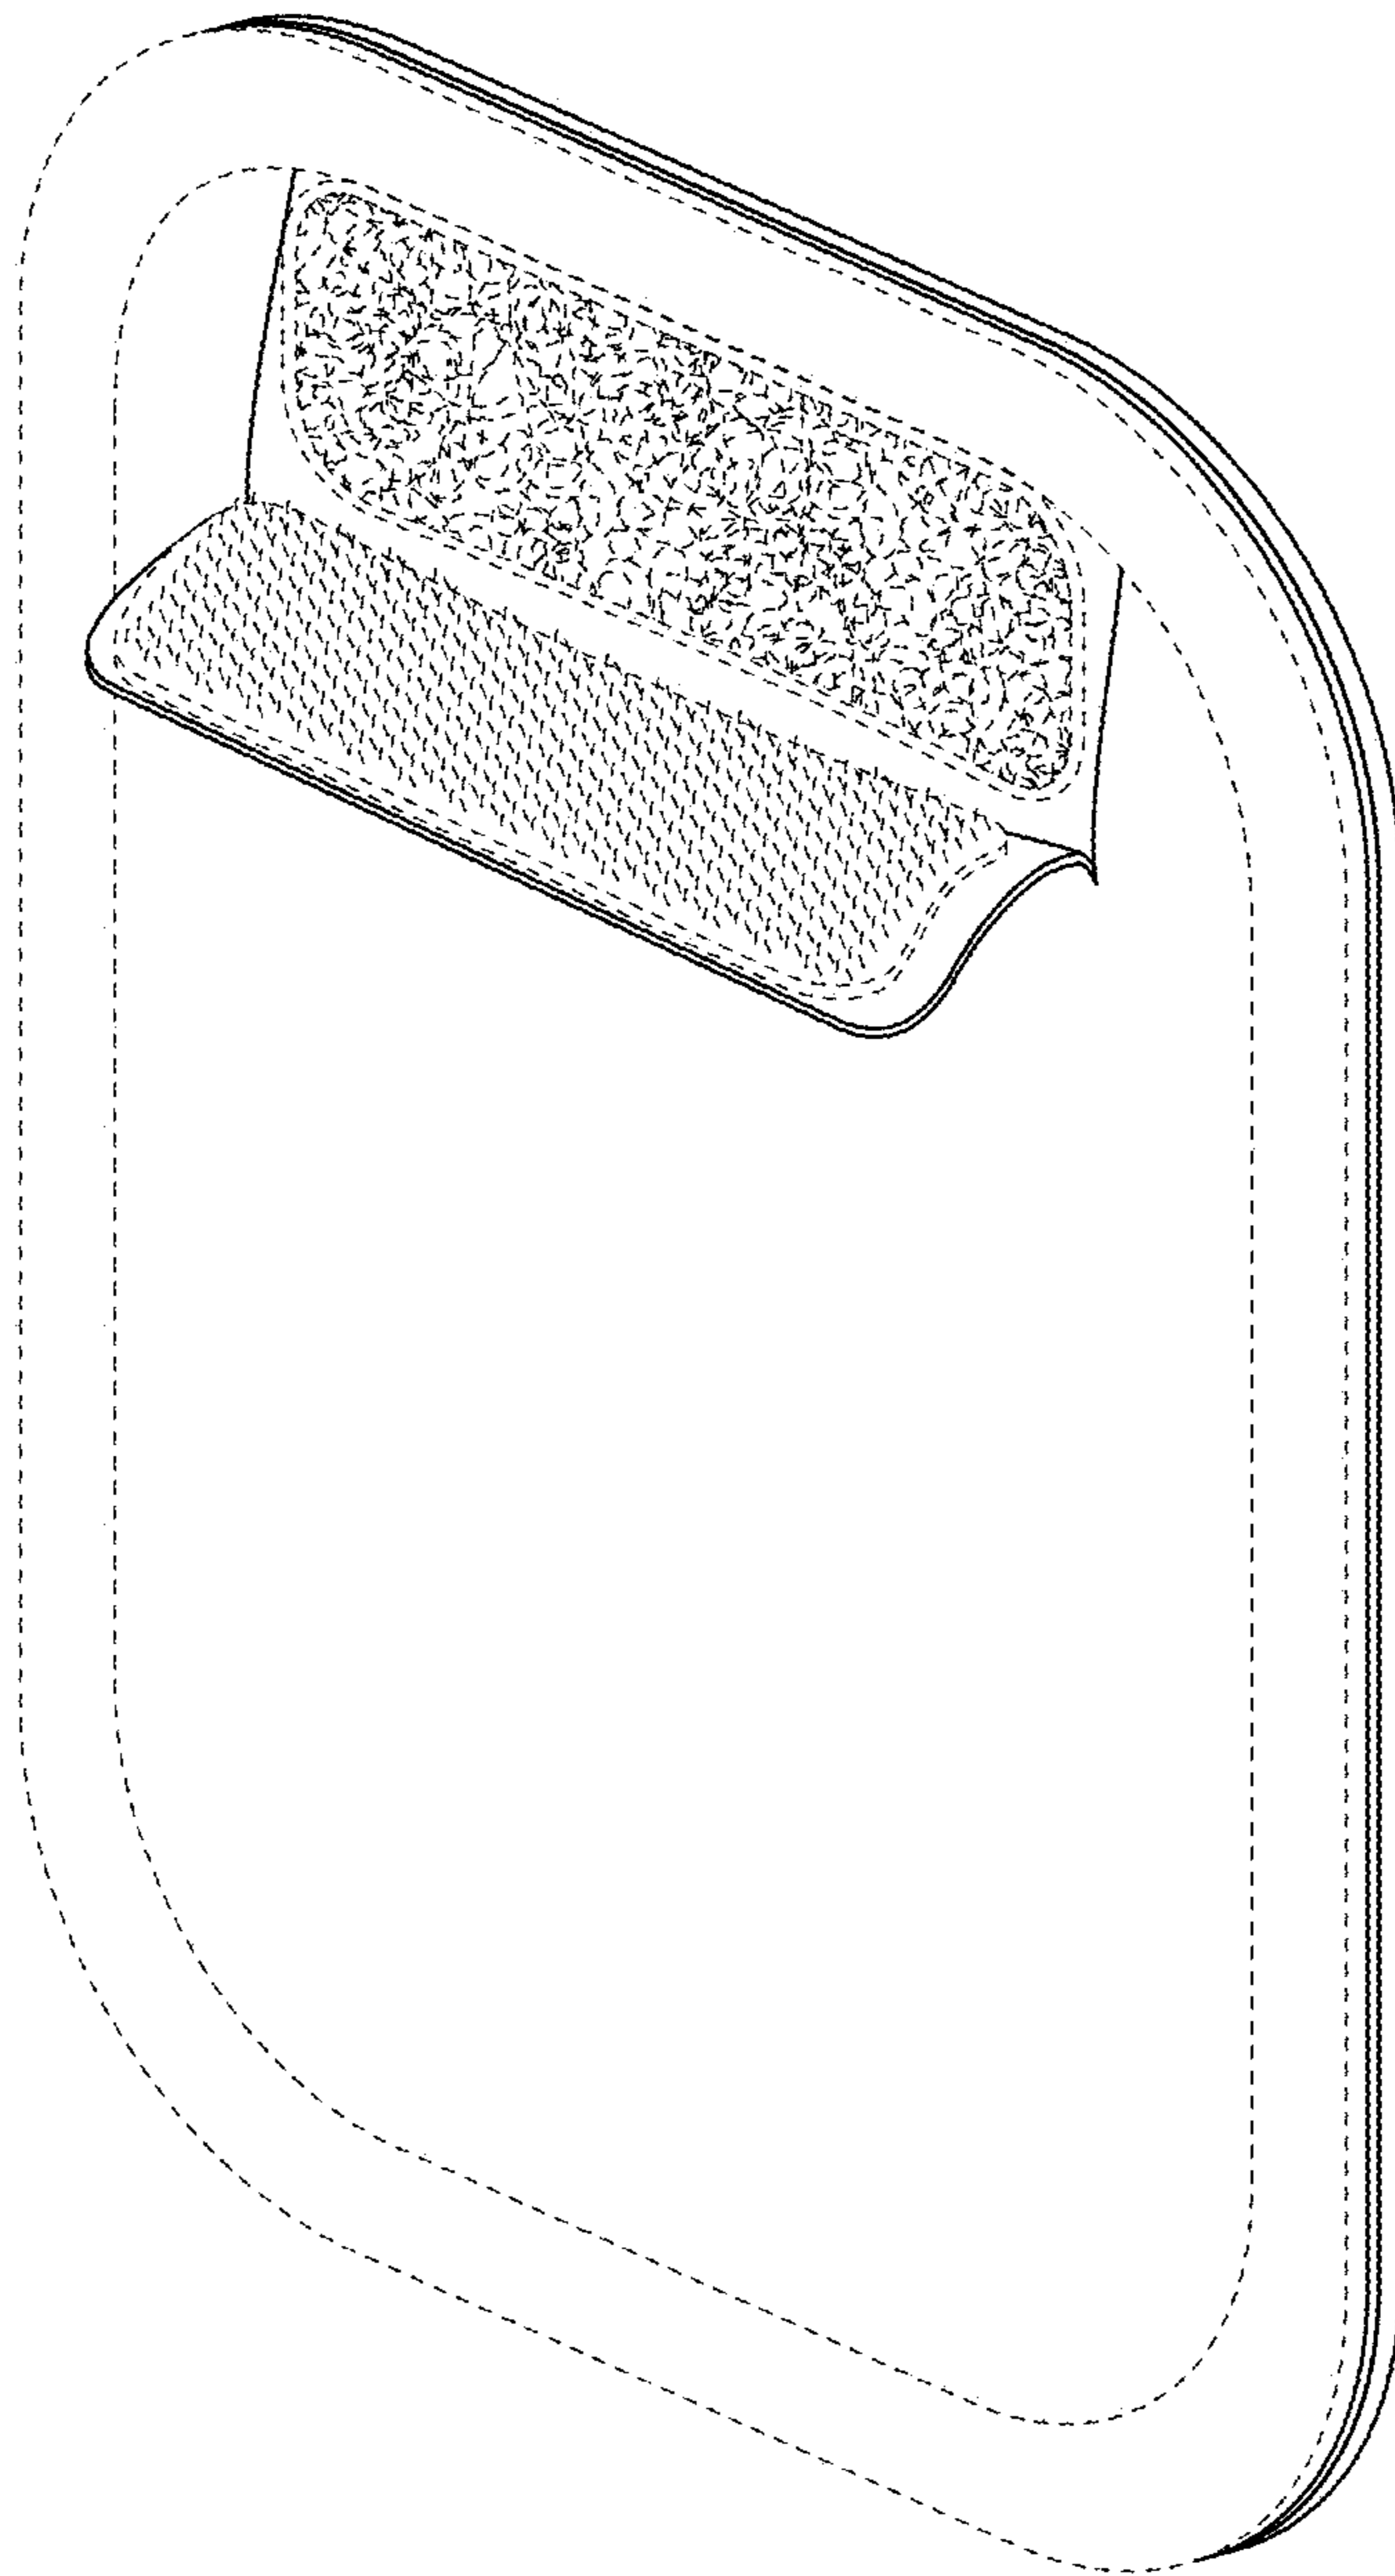


FIG. 9

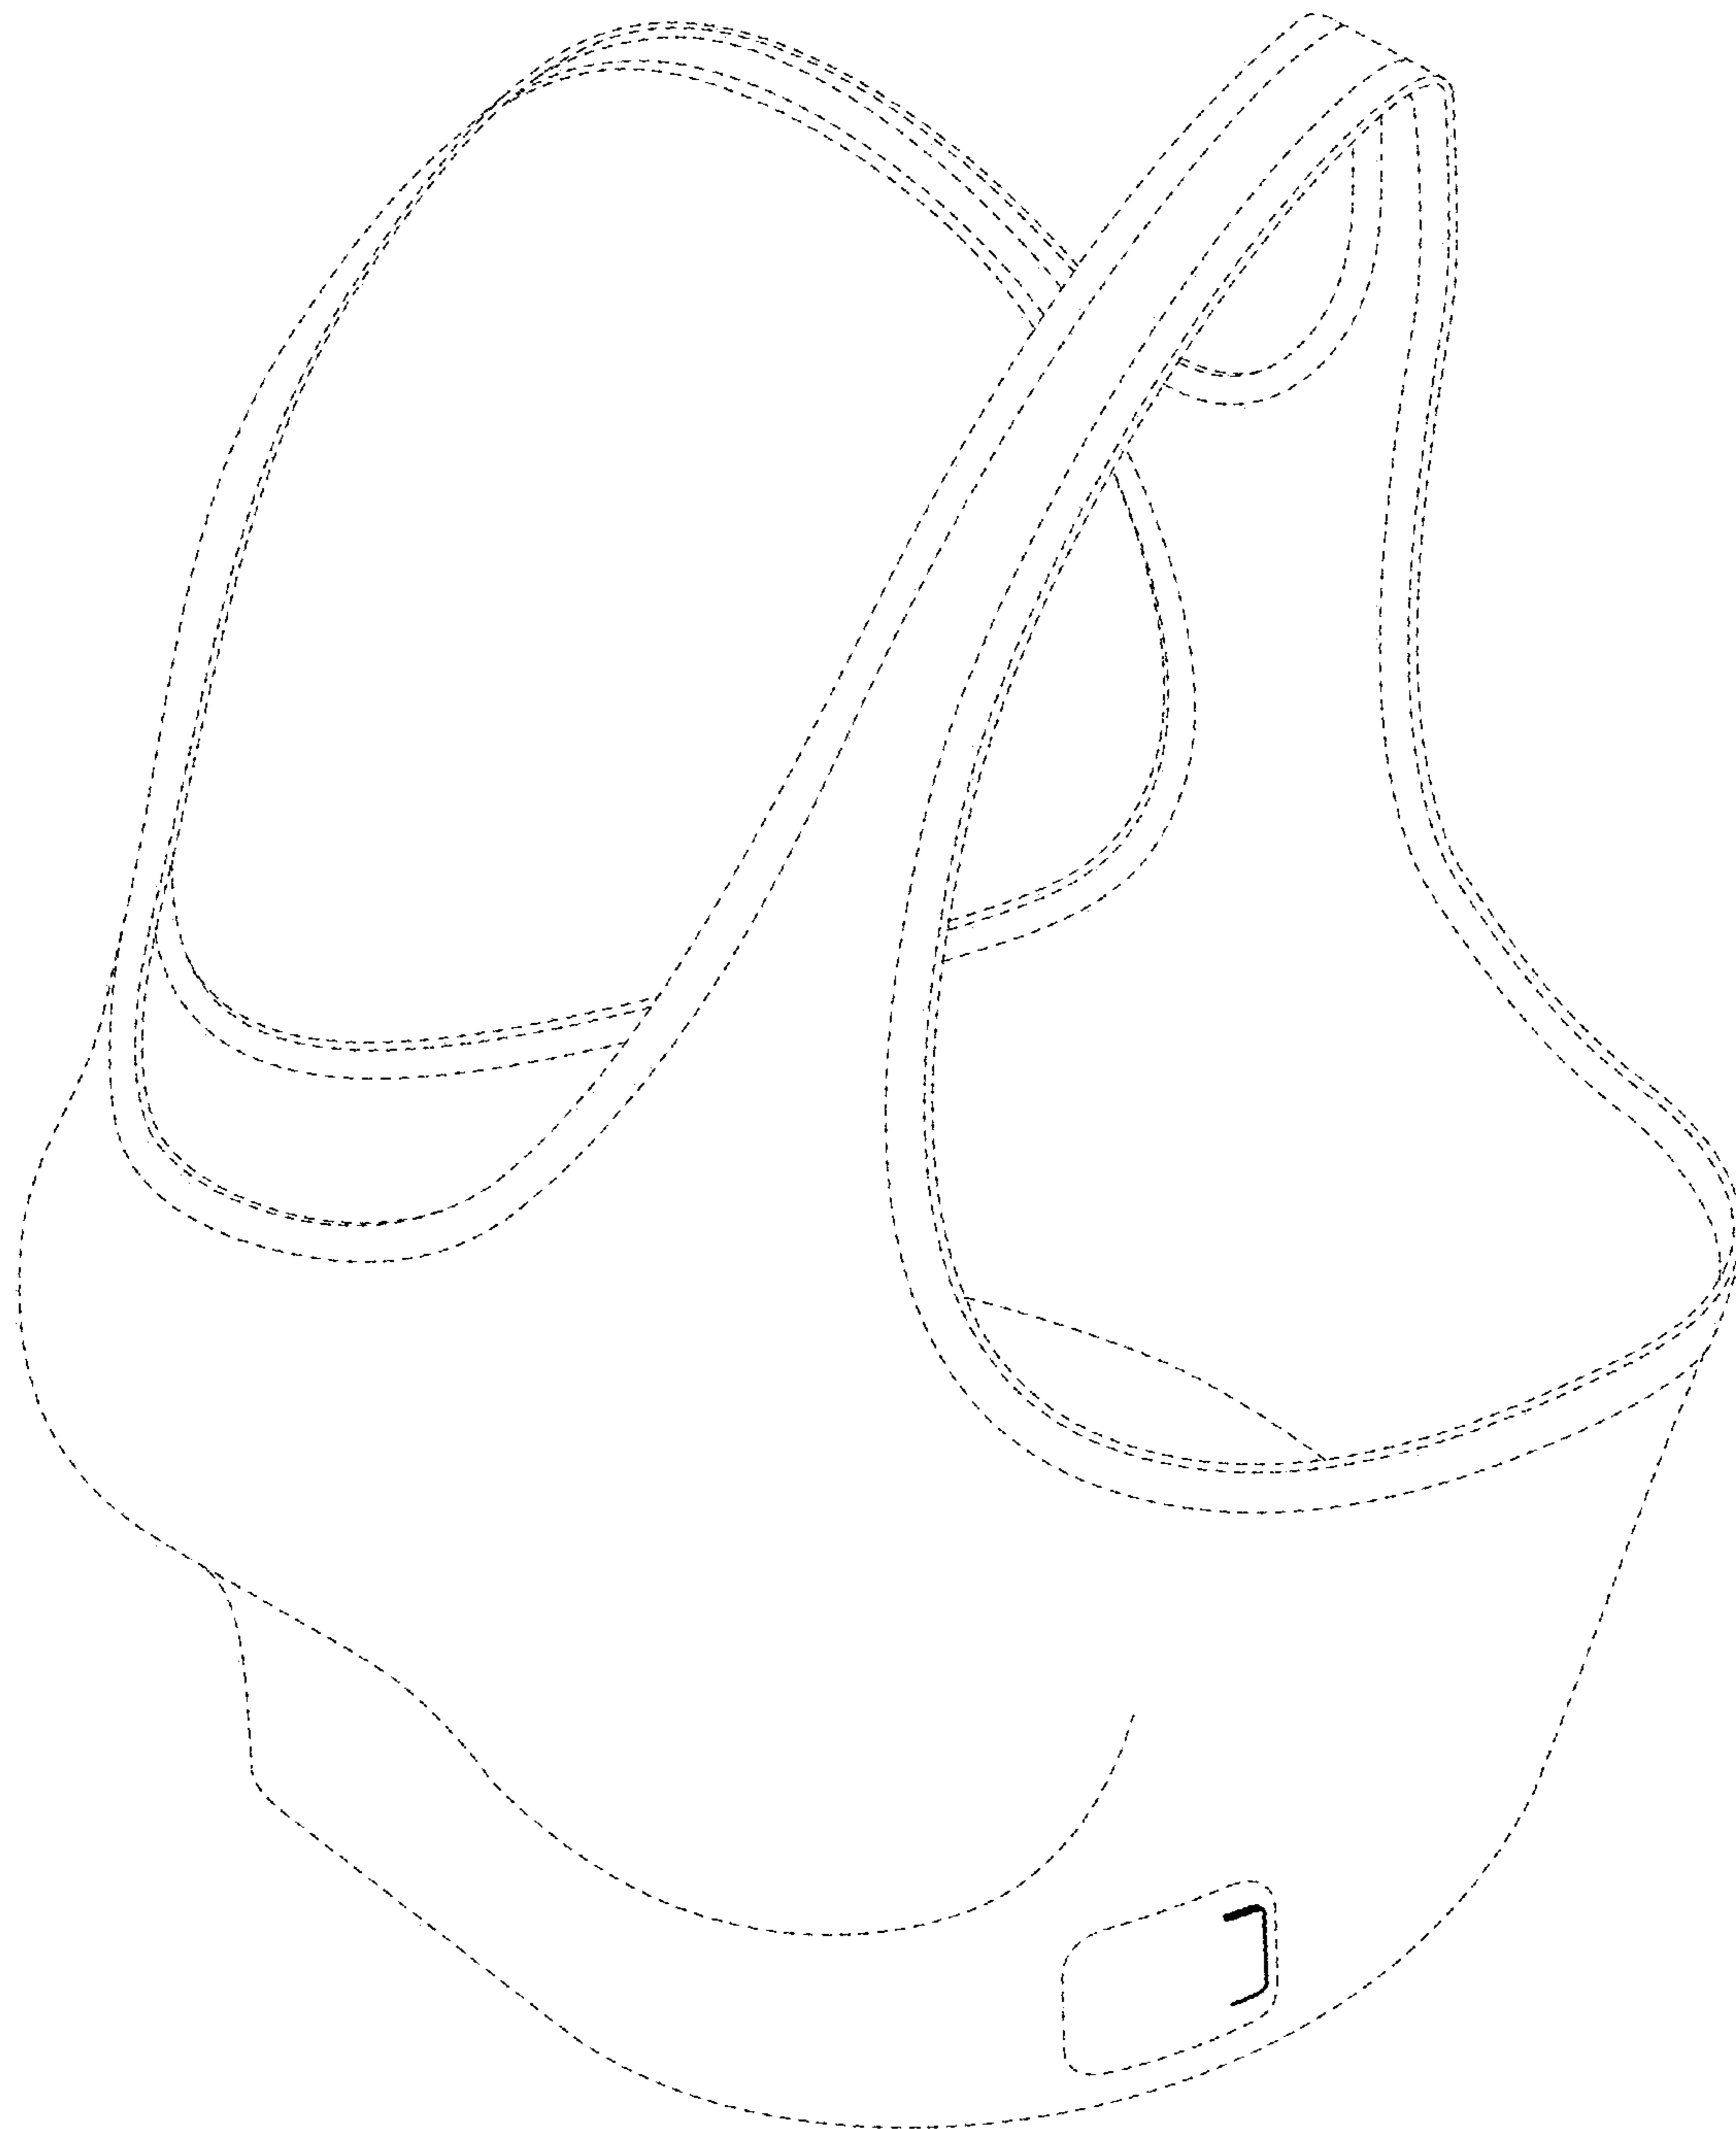


FIG. 10

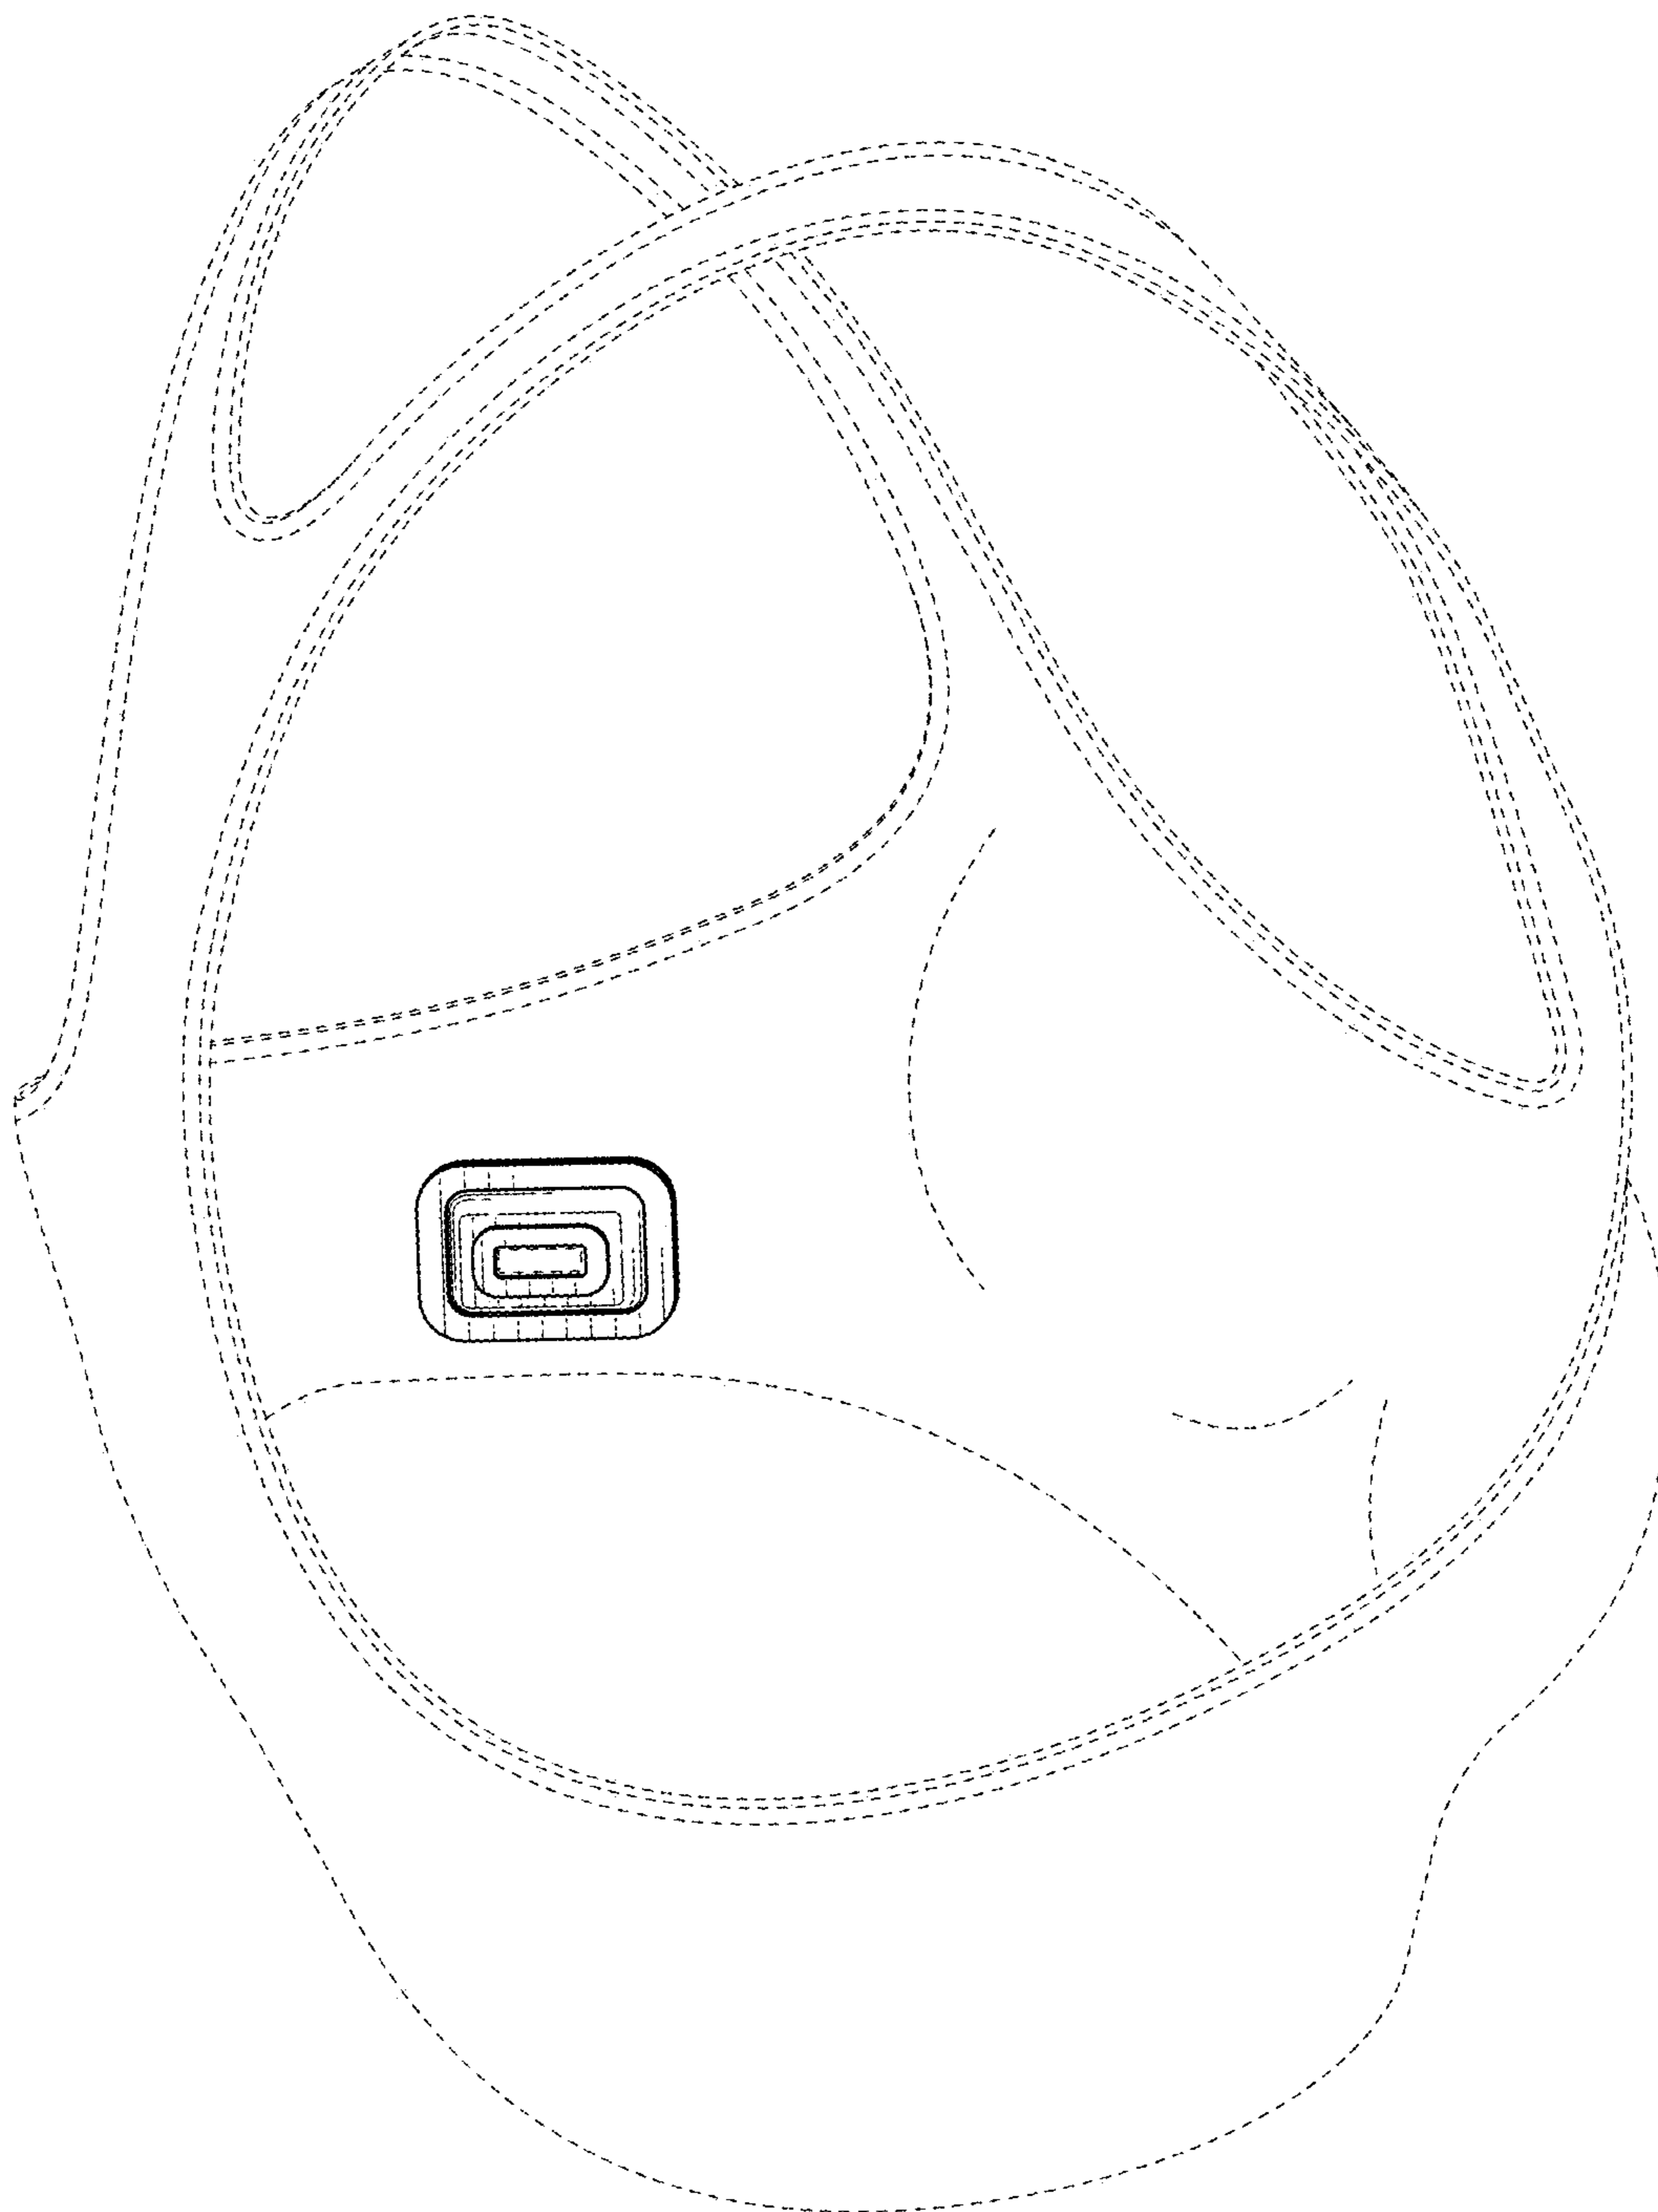


FIG. 11