



US00D977674S

(12) **United States Design Patent**
Allegoren et al.

(10) **Patent No.:** **US D977,674 S**
(45) **Date of Patent:** **** Feb. 7, 2023**

(54) **LIGHT VISOR FOR SEQUENCING INSTRUMENT**

(71) Applicant: **Illumina, Inc.**, San Diego, CA (US)

(72) Inventors: **Erik Allegoren**, San Diego, CA (US);
Erik Williamson, San Diego, CA (US);
Jack Godfrey Wood, San Diego, CA (US)

(73) Assignee: **Illumina, Inc.**, San Diego, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/796,923**

(22) Filed: **Jun. 28, 2021**

Related U.S. Application Data

(62) Division of application No. 29/717,775, filed on Dec. 19, 2019, now Pat. No. Des. 925,768.

(51) **LOC (14) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/232**

(58) **Field of Classification Search**
USPC D24/107, 169, 186, 216, 224, 231, 232,
D24/185, 223; D10/81
CPC G01N 35/00306; G01N 35/00326; G01N
35/00336; G01N 35/025; G01N 35/1085;
G01N 2030/027; G01N 21/6458; G01N
21/6484; G01N 21/6486; G01N 21/76;
G01N 2021/6432; C12Q 1/6898; C12Q
1/68

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D621,523 S 8/2010 Onuma
D646,189 S 10/2011 Dinter
D649,075 S 11/2011 Chan

D661,607 S 6/2012 Dinter
D662,431 S 6/2012 Kimura
D689,196 S 9/2013 Marmier
D729,405 S 5/2015 Ramstad
D735,883 S 8/2015 Bauer
D737,459 S 8/2015 Kurihara

(Continued)

FOREIGN PATENT DOCUMENTS

JP D2017501683 10/2018

OTHER PUBLICATIONS

MGI launches first “benchtop” sequencing laboratory and automation products. MGI. Oct. 25, 2019.

(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Heslin Rothenberg Farley & Mesiti, P.C.

(57) **CLAIM**


We claim the ornamental design for a light visor for sequencing instrument, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of the light visor for sequencing instrument comprising our new design; FIG. 2 is a front elevational view of the design of FIG. 1; FIG. 3 is a right side elevational view of the design of FIG. 1; FIG. 4 is a top plan view of the design in FIG. 1; FIG. 5 is a bottom plan view of the design of FIG. 1; and, FIG. 6 is a rear elevational view of the design in FIG. 1. The left side elevational view of the design shown in FIG. 1 is identical to FIG. 3.

The broken lines shown in the drawings illustrate portions of the light visor for sequencing instrument that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

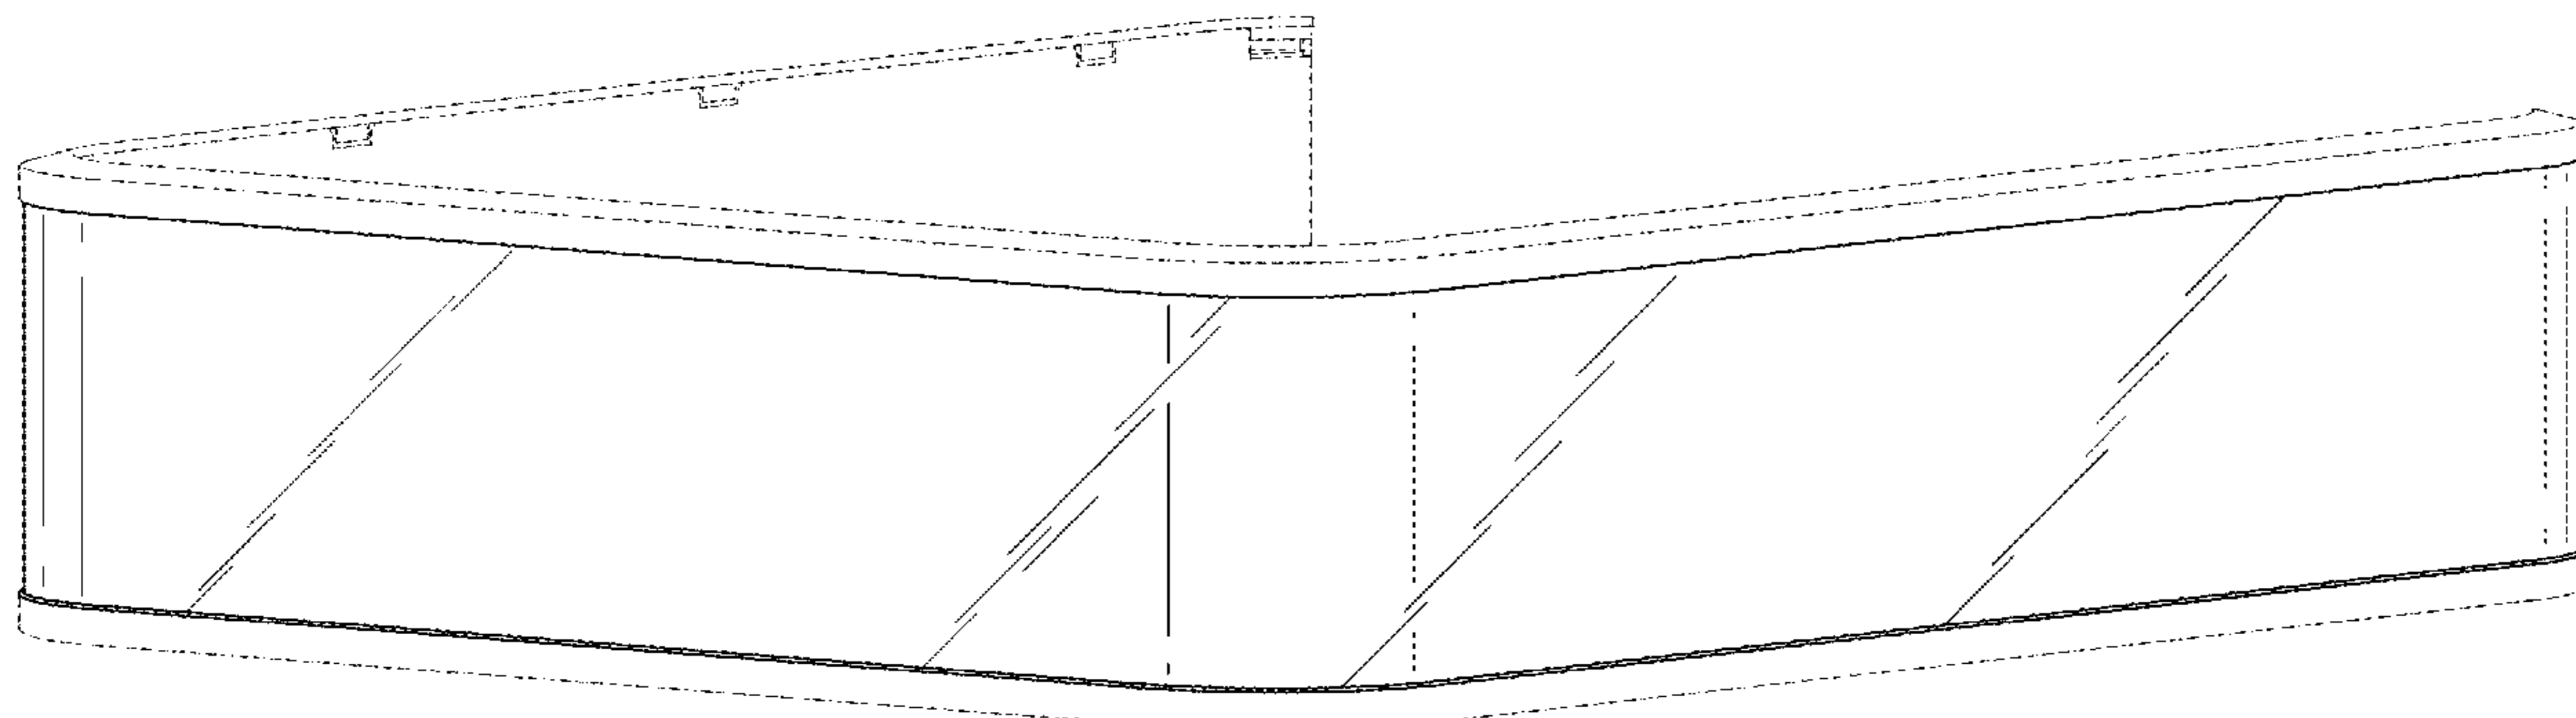

(56)

References Cited

U.S. PATENT DOCUMENTS

D774,659	S	12/2016	Quackenbush	
D782,690	S	3/2017	Kurihara	
D794,211	S	8/2017	Ang	
D800,000	S	10/2017	Barton	
D841,478	S	2/2019	Smith	
D843,005	S	3/2019	Kobeli	
D848,020	S	5/2019	Kobeli	
D855,823	S	8/2019	Williamson	
D865,998	S	11/2019	Mellett	
10,626,440	B2 *	4/2020	Tajima	G01N 35/1065
D923,197	S	6/2021	Allegoren	
D923,198	S	6/2021	Allegoren	
D925,768	S *	7/2021	Allegoren	D24/232
D952,901	S *	5/2022	Dye	D24/232
2020/0110108	A1	4/2020	Cox-Muranami	
2020/0171502	A1	6/2020	Kumar	

OTHER PUBLICATIONS

Dye et al., "Sequencing Instrument Light Visor", U.S. Appl. No. 29/720,284, filed Jan. 10, 2020.

* cited by examiner

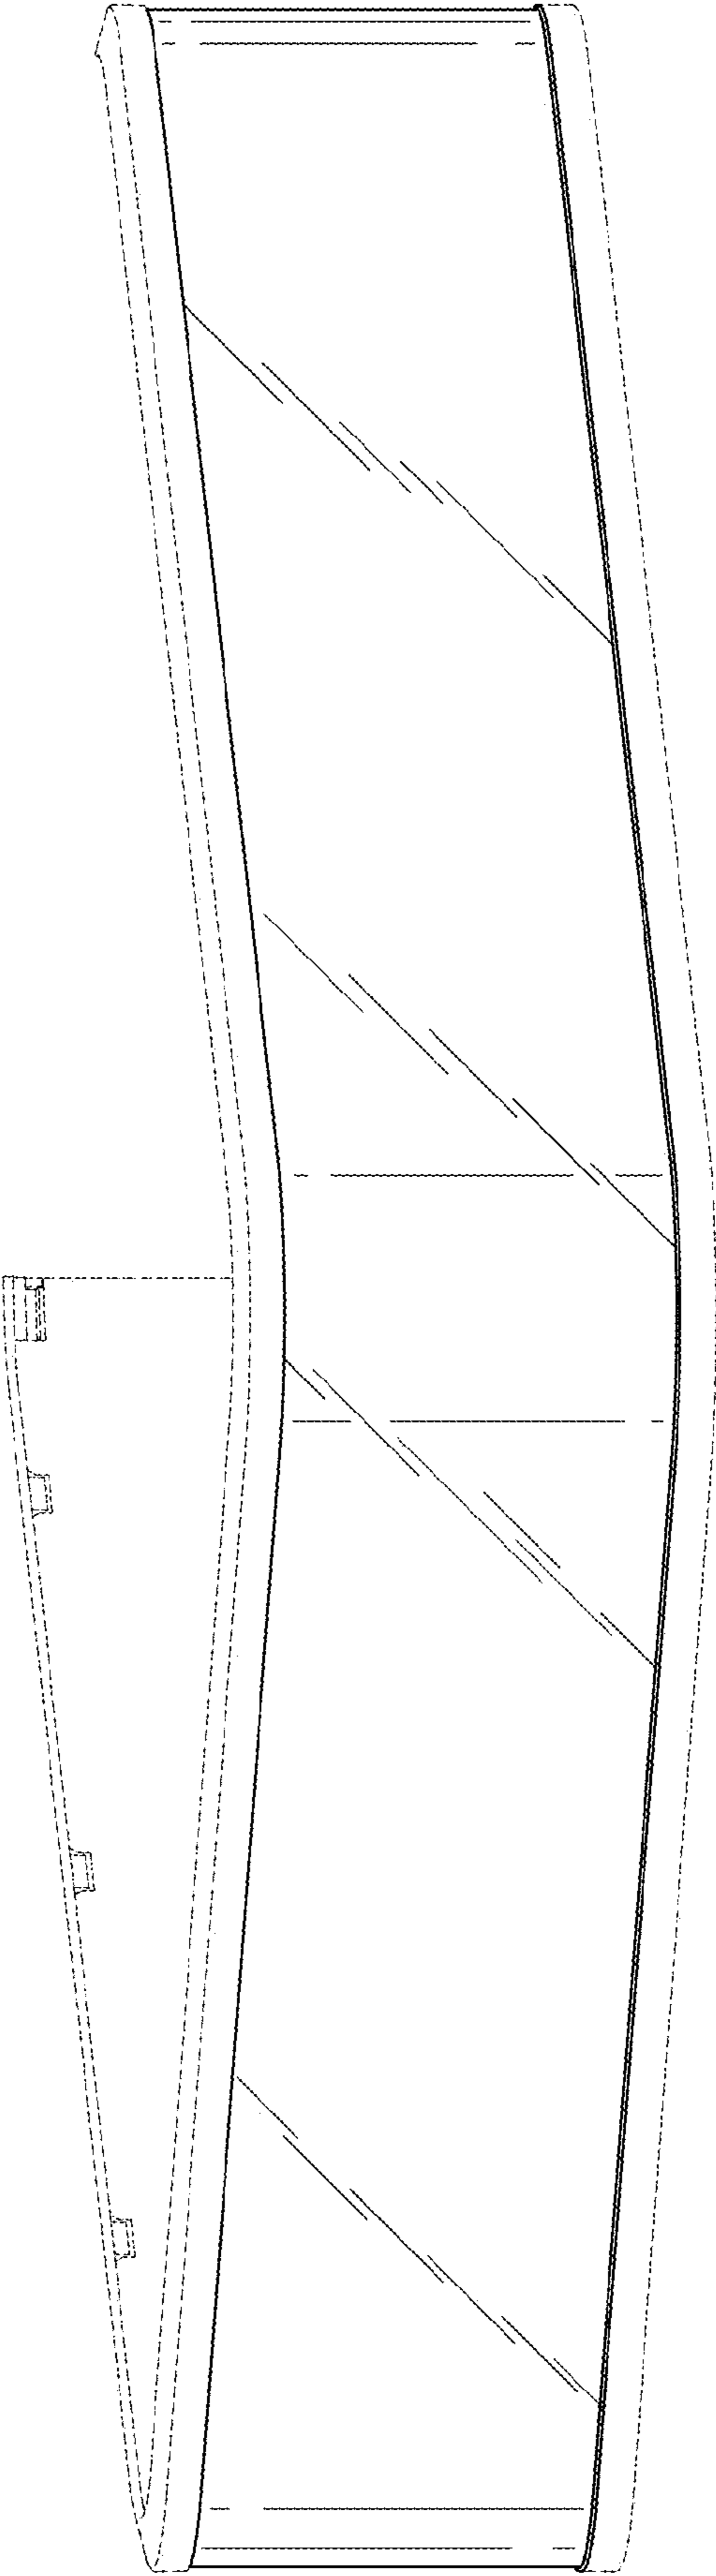


FIG. 1

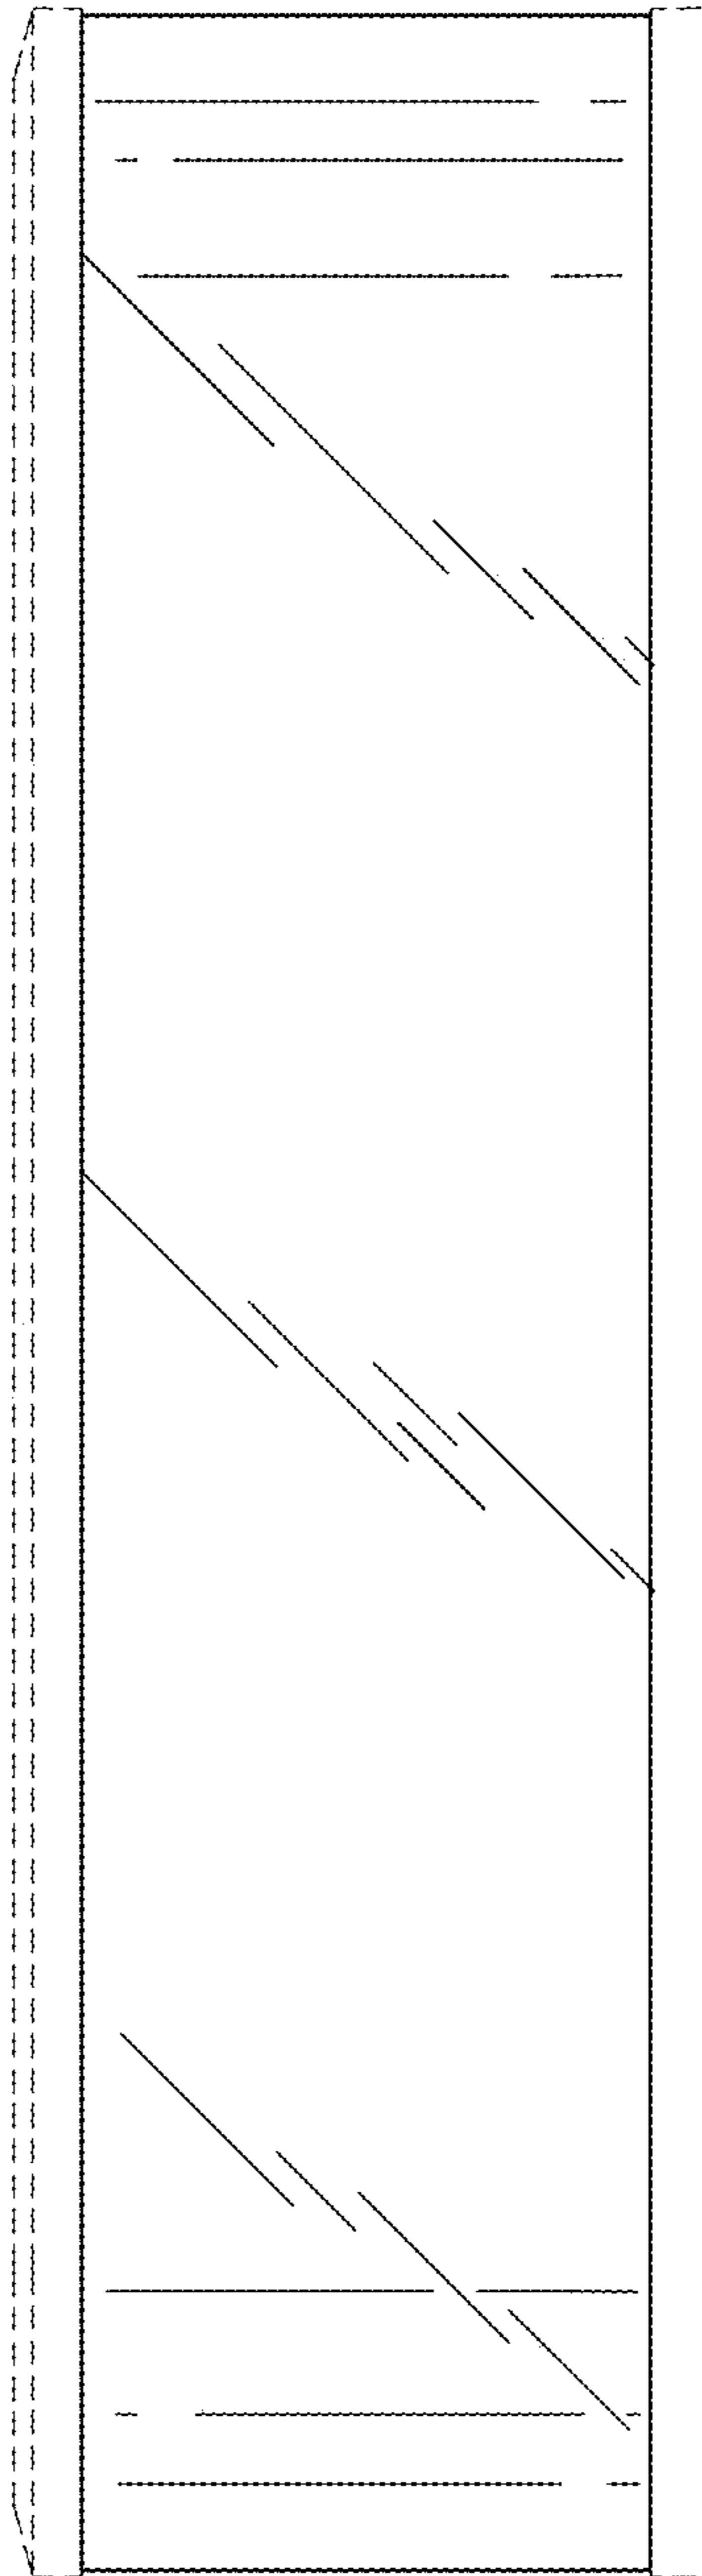


FIG. 2

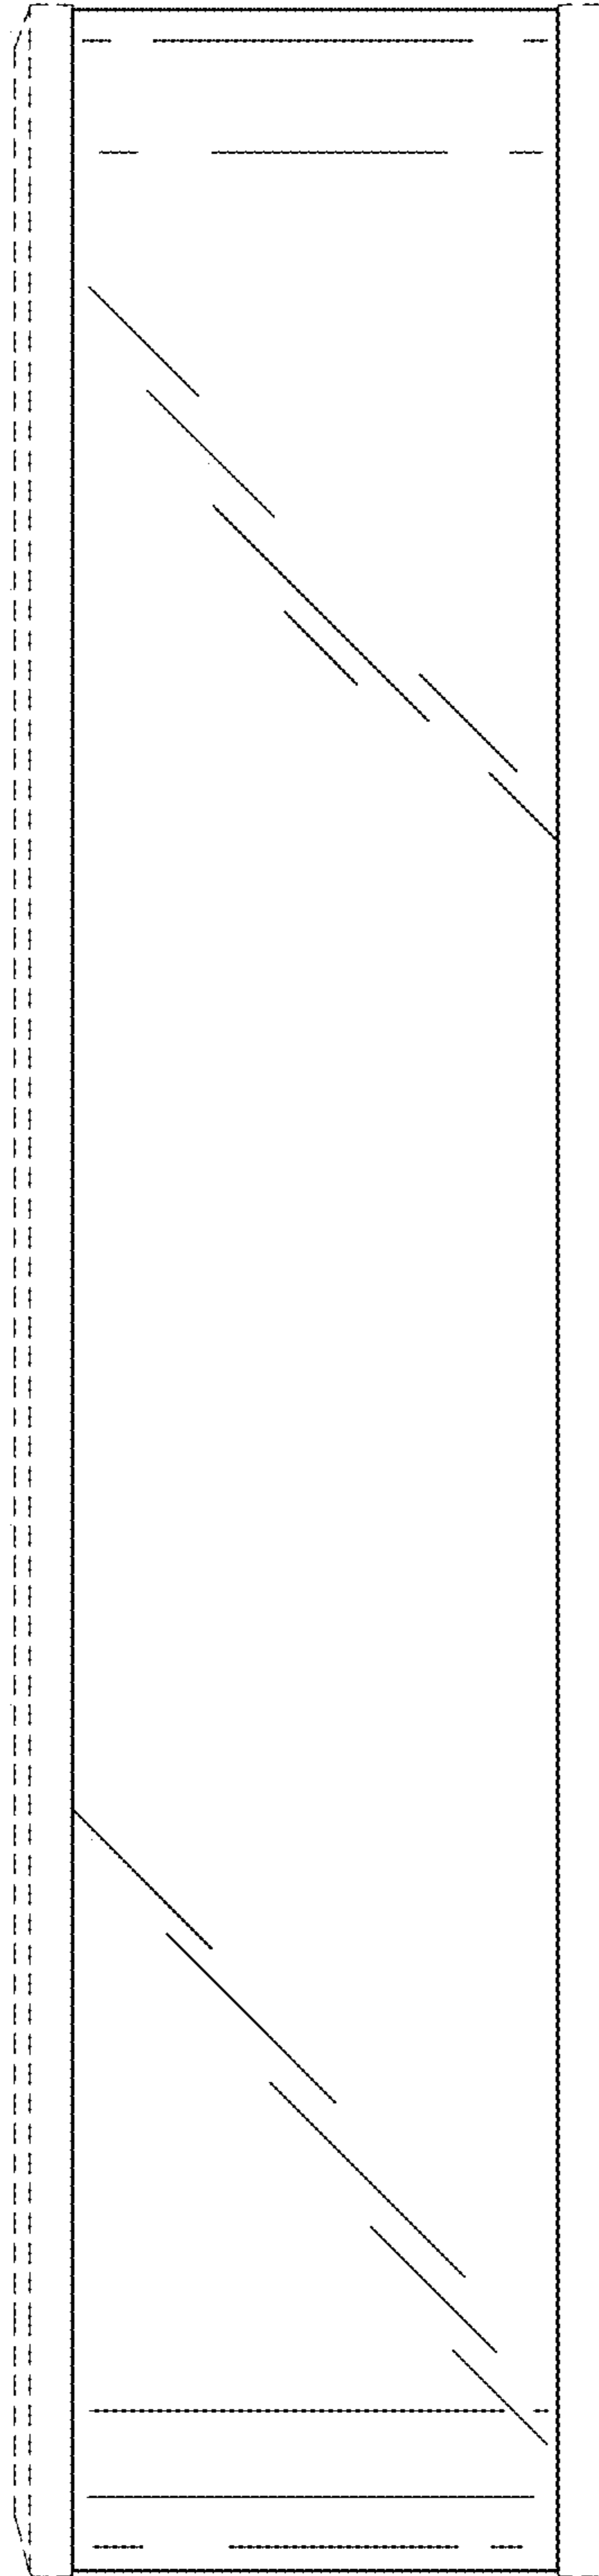


FIG. 3

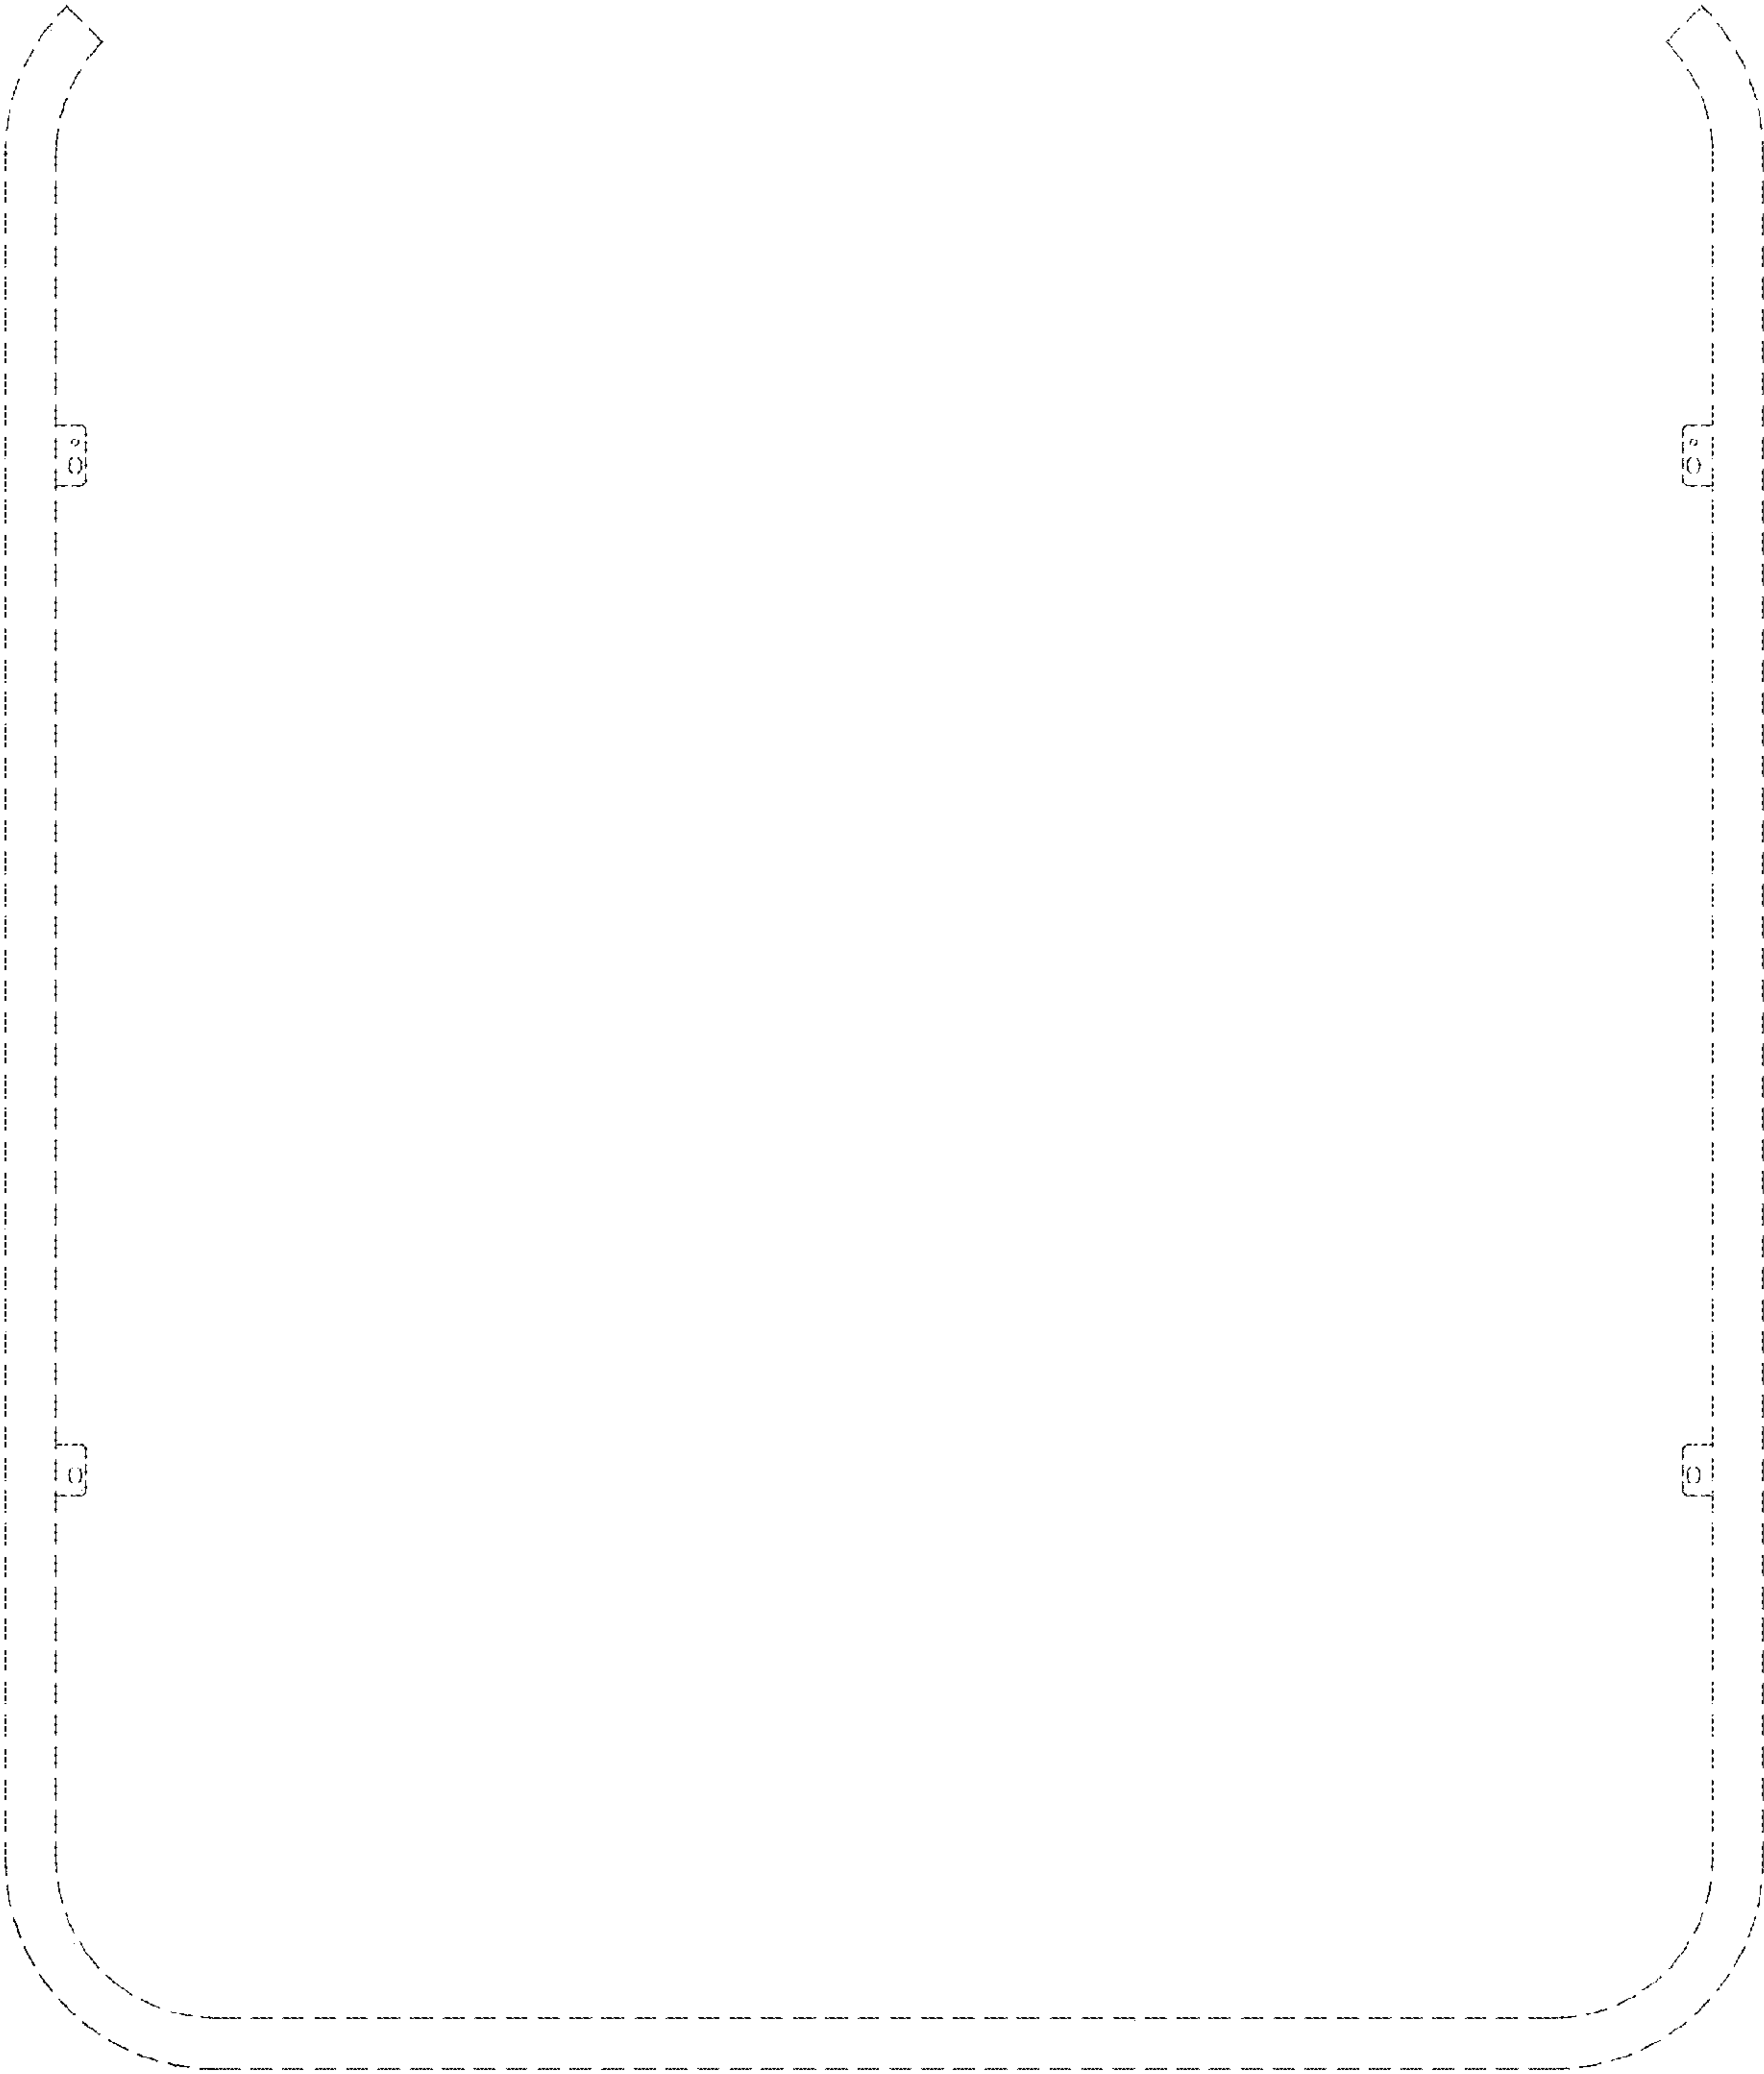


FIG. 4

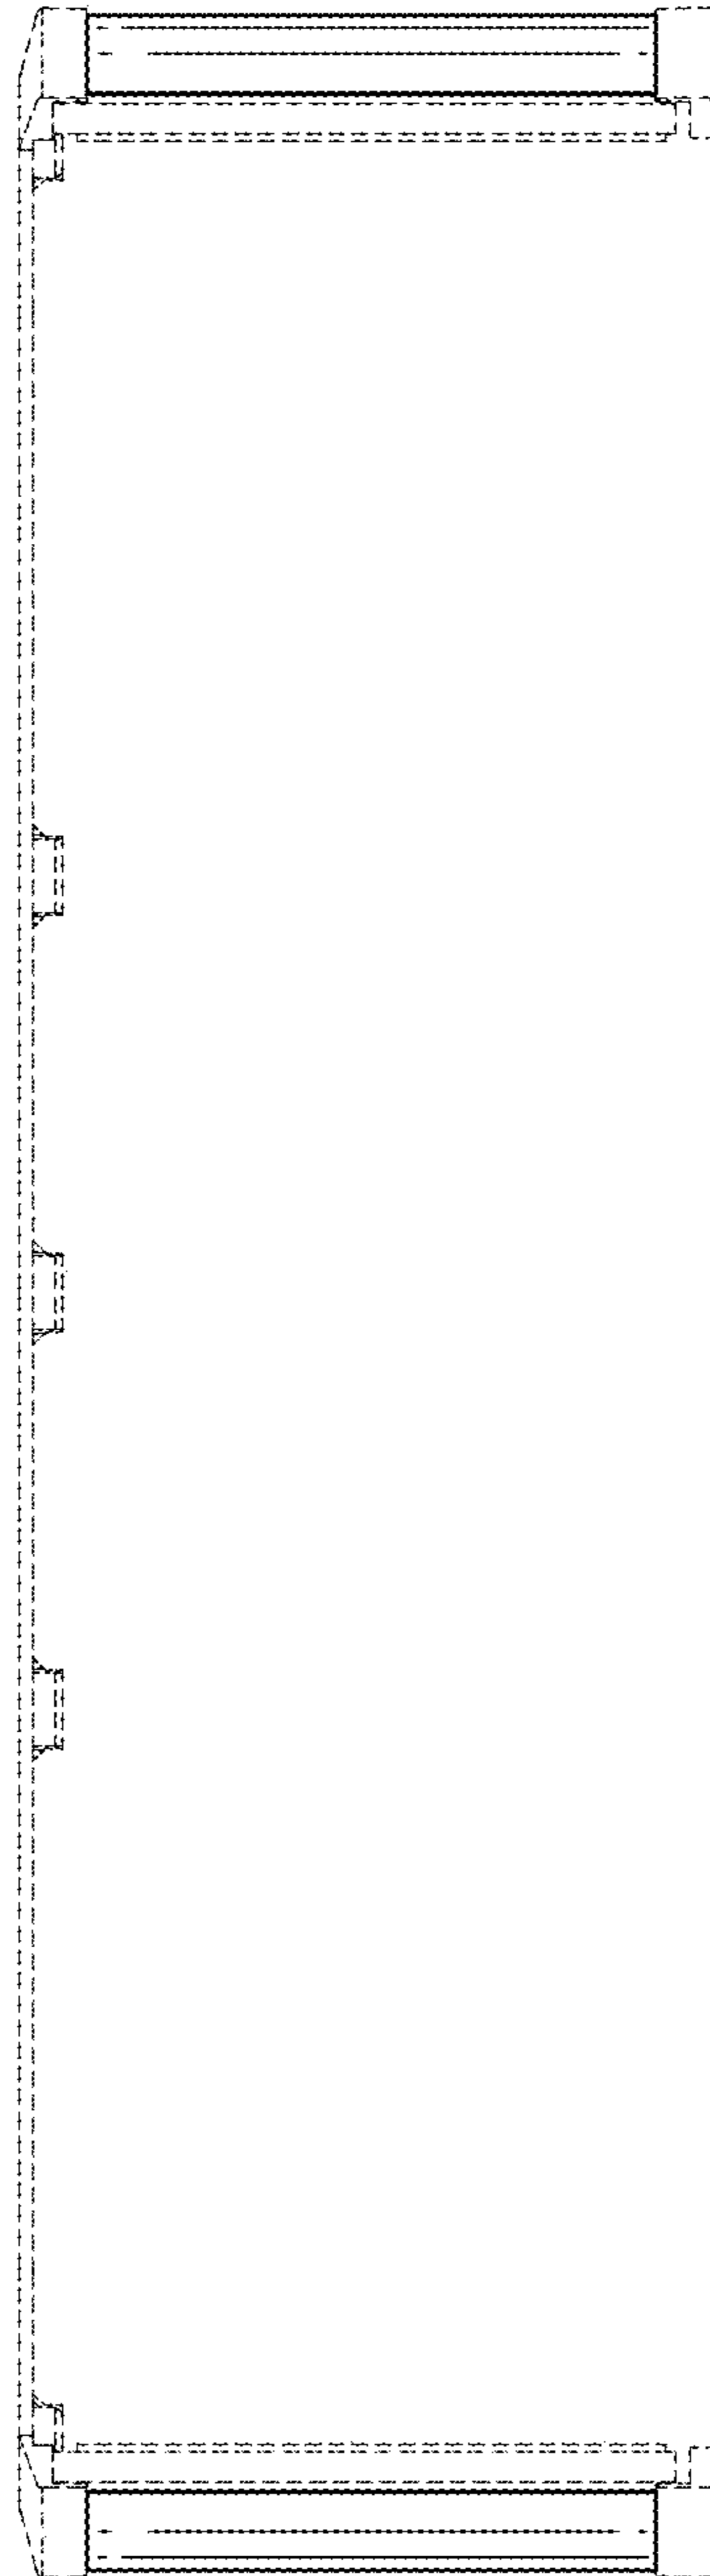


FIG. 5

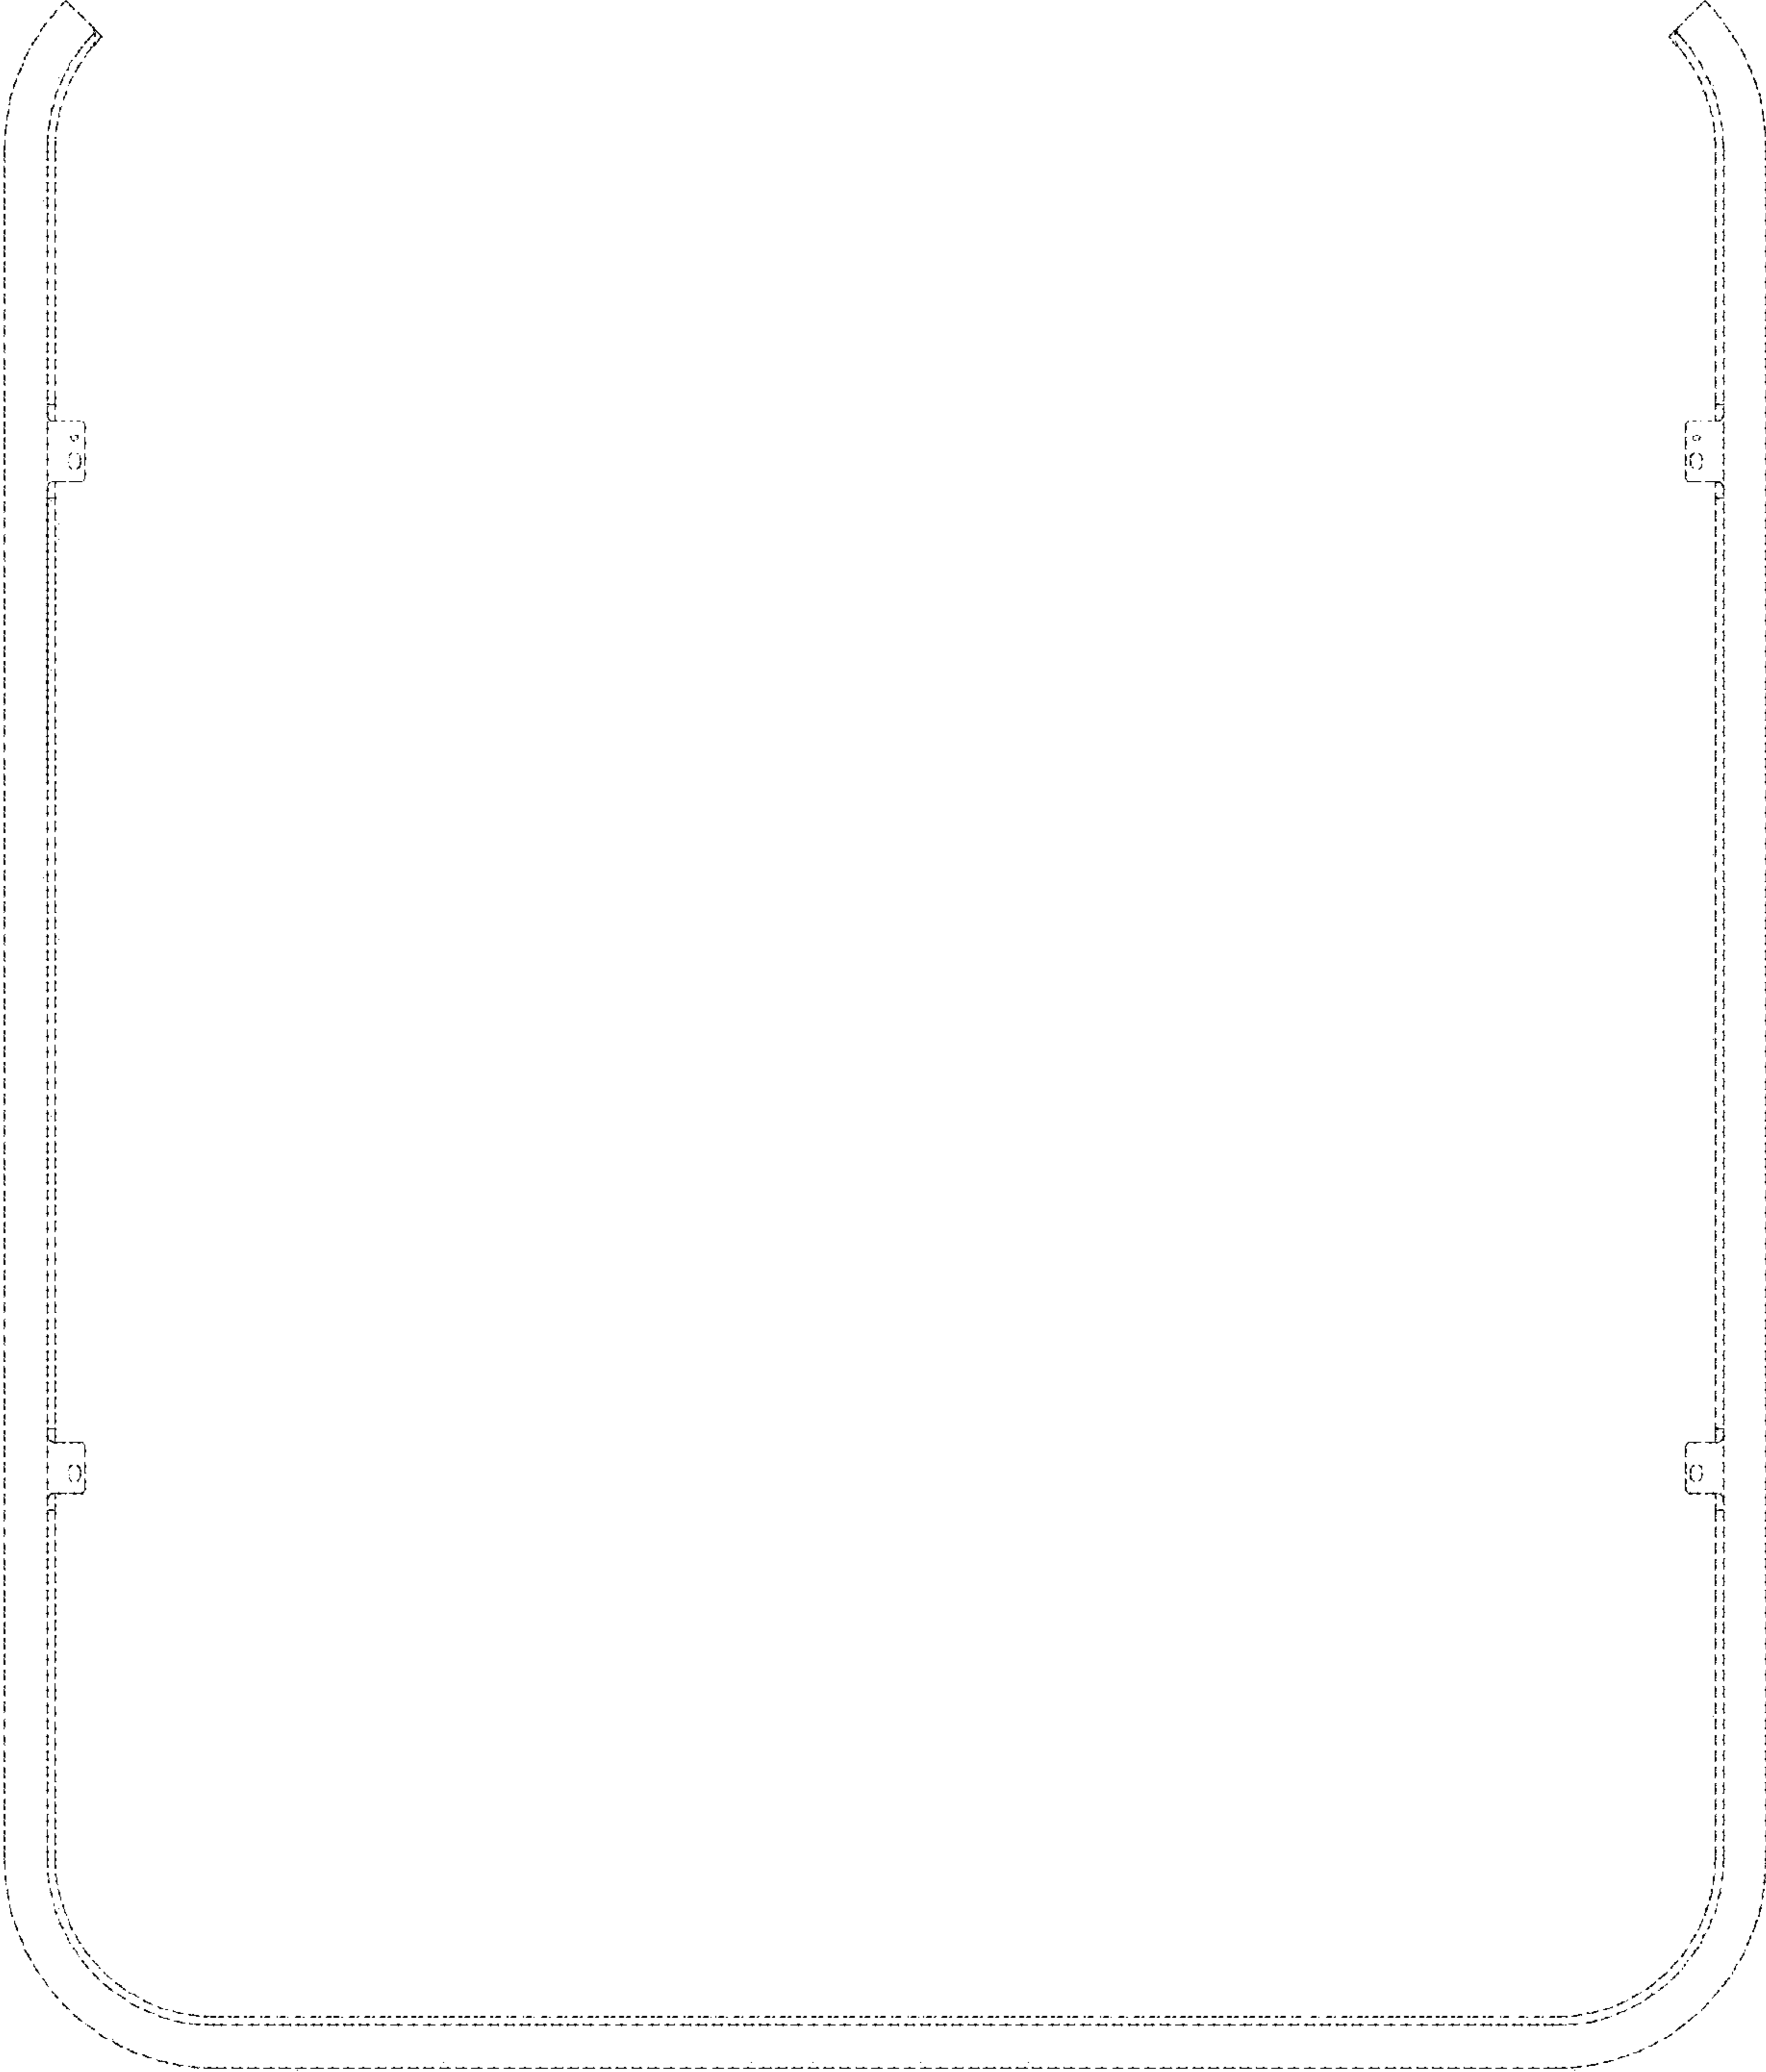


FIG. 6