



US00D978332S

(12) **United States Design Patent** (10) **Patent No.:** **US D978,332 S**  
**Rothermel et al.** (45) **Date of Patent:** **\*\* Feb. 14, 2023**

(54) **MEDICAL DEVICE**  
(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,  
Eindhoven (NL)  
(72) Inventors: **Justin Rothermel**, Monroeville, PA  
(US); **Joshua Greenberg**, Aspinwall,  
PA (US); **Robert O’Grady**, Pittsburgh,  
PA (US)

2008/0060649 A1\* 3/2008 Veliss ..... A61M 16/0825  
128/205.25  
2015/0182719 A1\* 7/2015 Grashow ..... A61M 16/0666  
128/205.25  
2018/0147382 A1\* 5/2018 Hlopick ..... A61M 16/06  
2019/0298954 A1\* 10/2019 Rothermel ..... A61M 16/0616  
2019/0388639 A1\* 12/2019 Grashow ..... A61M 16/0622  
2020/0384229 A1\* 12/2020 Lashinsky ..... A61M 16/06  
2021/0030990 A1\* 2/2021 Klinkenberg ..... A61M 16/0683  
2021/0093236 A1\* 4/2021 Margaria ..... A61B 5/0002  
(Continued)

(73) Assignee: **KONINKLIJKE PHILIPS N.V.**,  
Eindhoven (NL)

**FOREIGN PATENT DOCUMENTS**

(\*\*) Term: **15 Years**

WO WO D203125-003 \* 8/2019

(21) Appl. No.: **29/682,038**

**OTHER PUBLICATIONS**

(22) Filed: **Mar. 1, 2019**

“Philips Respironics DreamWisp Nasal CPAP Mask” posted by user  
The CPAP Shop. Youtube. Date posted: Mar. 19, 2019. Date  
retrieved: Jan. 26, 2022. Retrieved from internet: <https://www.youtube.com/watch?v=xp8686rD17Y> (Year: 2019).\*

(51) **LOC (14) Cl.** ..... **29-02**

(52) **U.S. Cl.**  
USPC ..... **D24/110.4**

(58) **Field of Classification Search**  
USPC ..... D24/110, 110.1–110.4, 110.6, 127;  
D29/108, 122  
CPC ..... A61M 16/06; A61M 16/0605; A61M  
16/0616; A61M 16/0622; A61M 16/0633;  
A61M 16/0644; A61M 16/0666; A61M  
16/0672; A61M 16/0683

*Primary Examiner* — Mary Shannon Malley  
*Assistant Examiner* — Lee D. Starr

See application file for complete search history.

(57) **CLAIM**

The ornamental design for a medical device, as shown and  
described.

(56) **References Cited**


**U.S. PATENT DOCUMENTS**

D717,942 S \* 11/2014 Neff ..... D24/127  
D799,699 S \* 10/2017 Higgins ..... D24/110.4  
D829,322 S \* 9/2018 Eury ..... D24/110.4  
D869,637 S \* 12/2019 Higgins ..... D24/110  
D869,642 S \* 12/2019 Andrews ..... D24/110.4  
D893,013 S \* 8/2020 Higgins ..... D24/110.4  
D924,388 S \* 7/2021 Blanch ..... D24/110.4  
D933,814 S \* 10/2021 Eves ..... D24/110.4  
D954,938 S \* 6/2022 Rothermel ..... D24/110.4  
D955,561 S \* 6/2022 Rothermel ..... D24/110.4

**DESCRIPTION**

FIG. 1 is a top, front, right perspective view of a medical  
device, showing the new design;  
FIG. 2 is a bottom, rear, left perspective view thereof;  
FIG. 3 is a front elevation view thereof;  
FIG. 4 is a rear elevation view thereof;  
FIG. 5 is a right side view thereof;  
FIG. 6 is a left side view thereof;  
FIG. 7 is a top plan view thereof; and,  
FIG. 8 is a bottom plan view thereof.  
The broken lines of even length illustrate portions of the  
medical device that form no part of the claimed design.

**1 Claim, 8 Drawing Sheets**

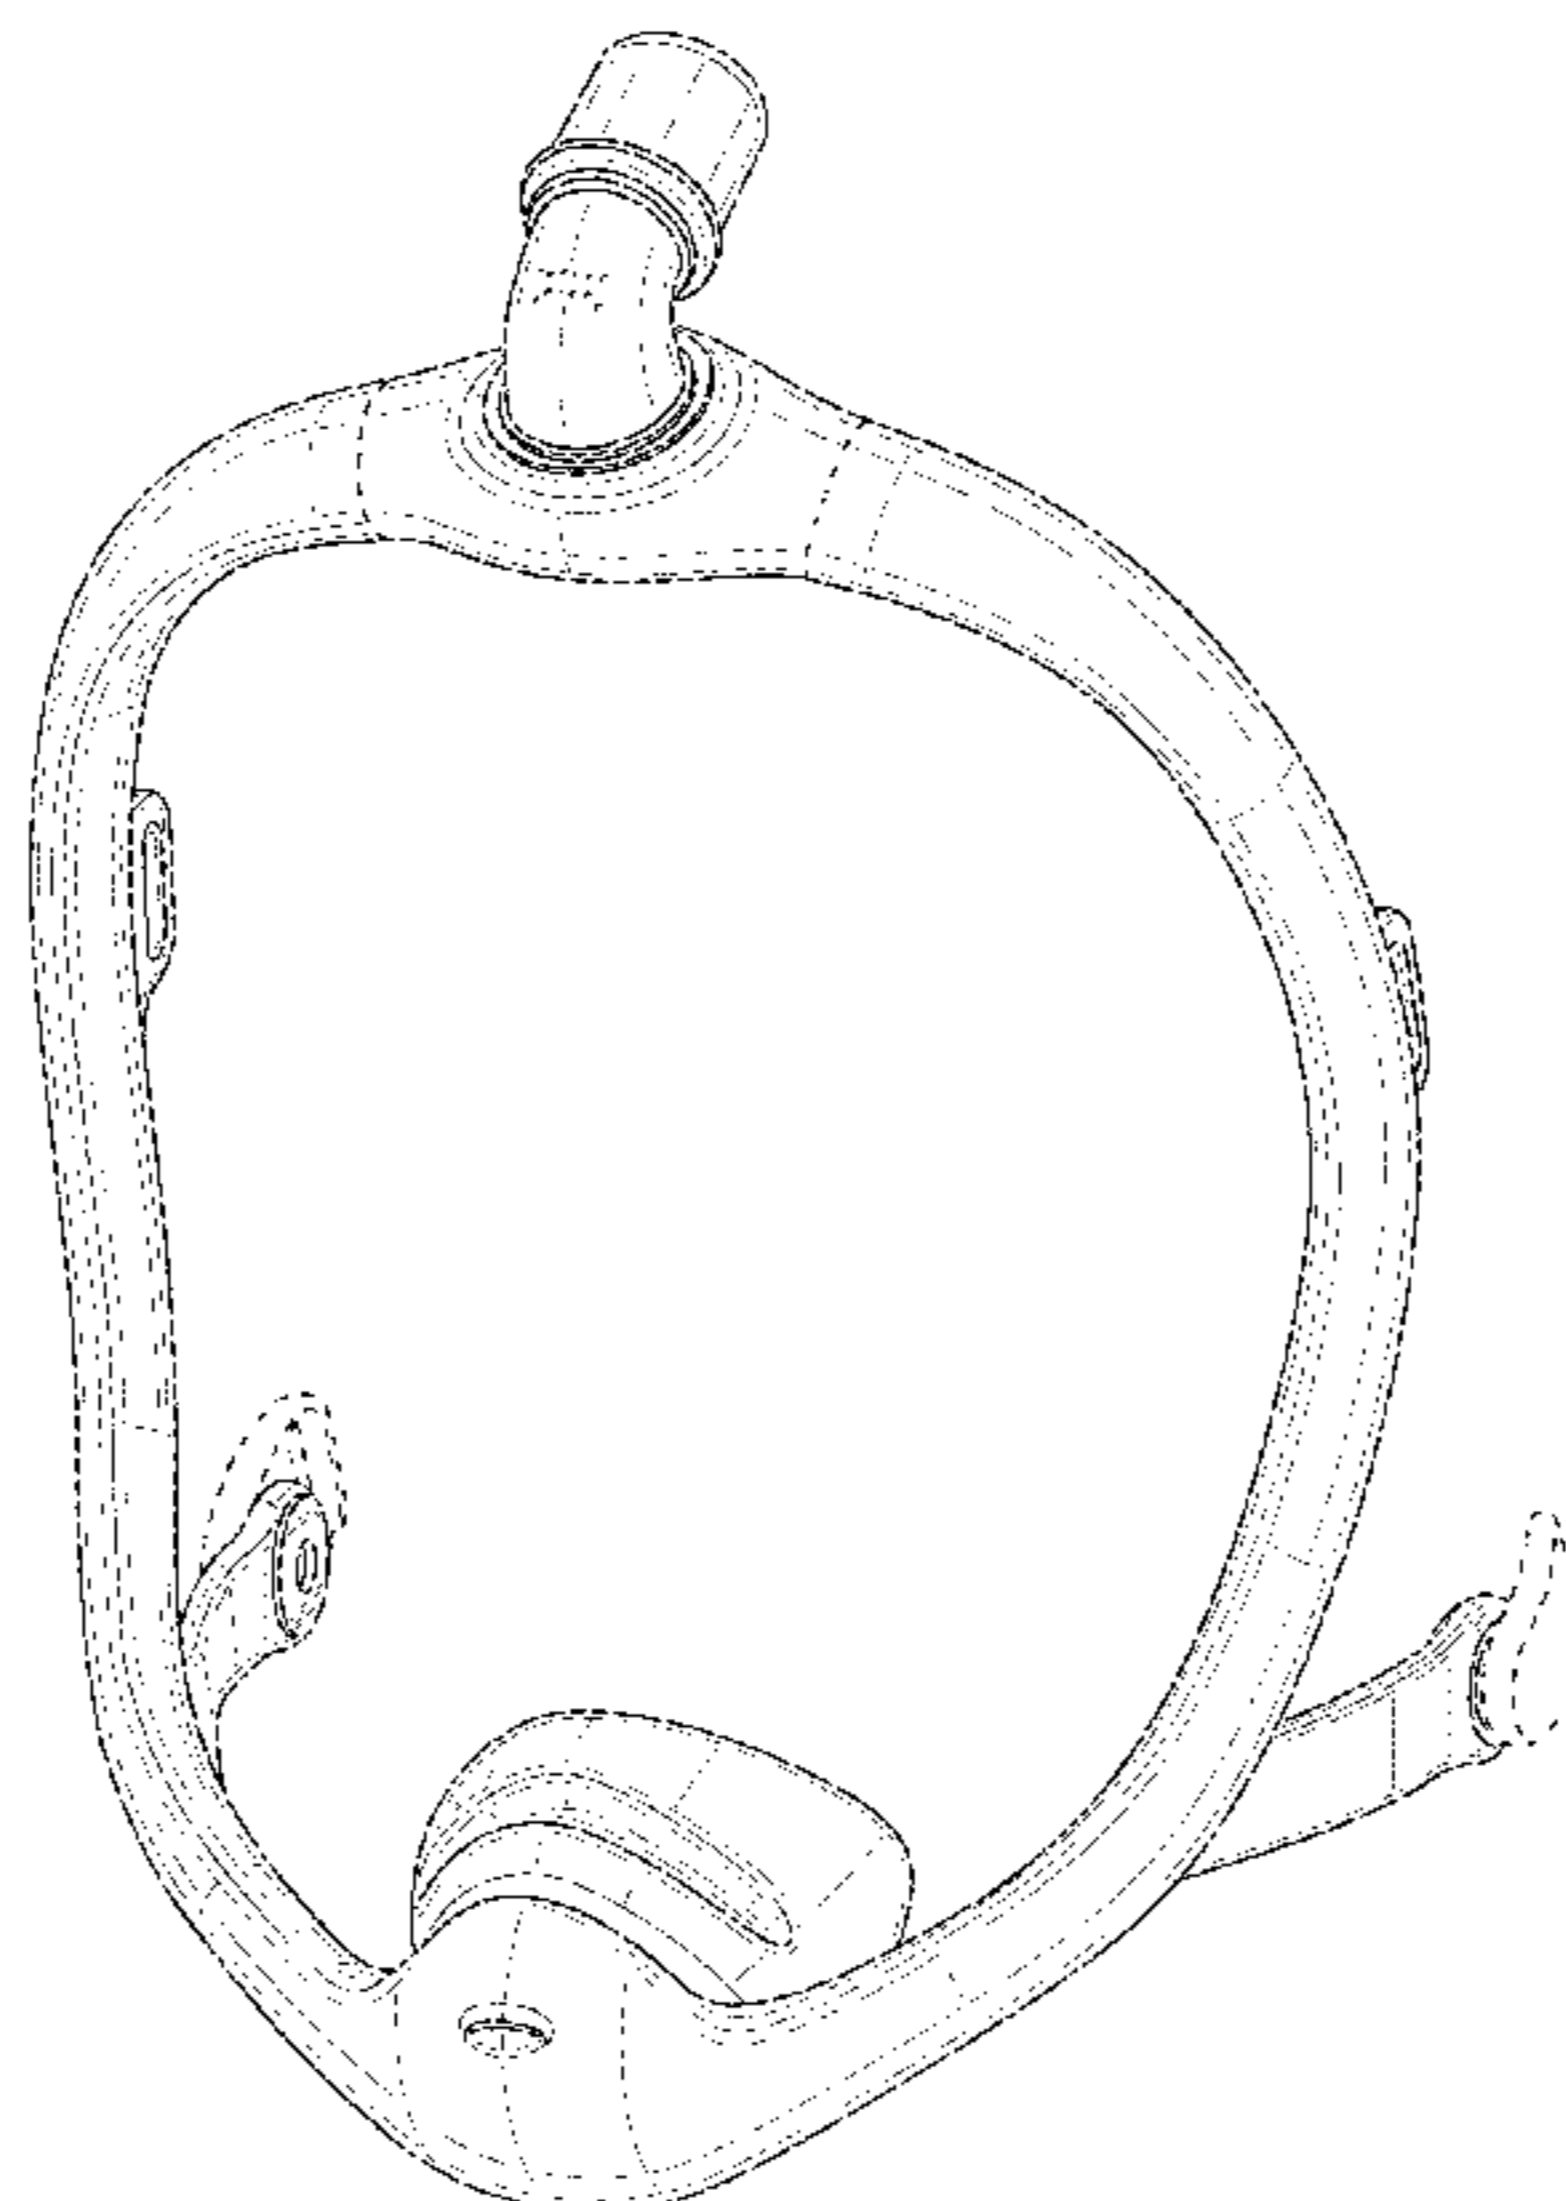

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2021/0093820 A1\* 4/2021 Grashow ..... A61M 16/0616  
2021/0252243 A1\* 8/2021 Barlow ..... A61M 16/0833  
2022/0241534 A1\* 8/2022 Rothermel ..... A61M 16/0683  
2022/0265949 A1\* 8/2022 Davidson ..... A61M 16/0816

\* cited by examiner

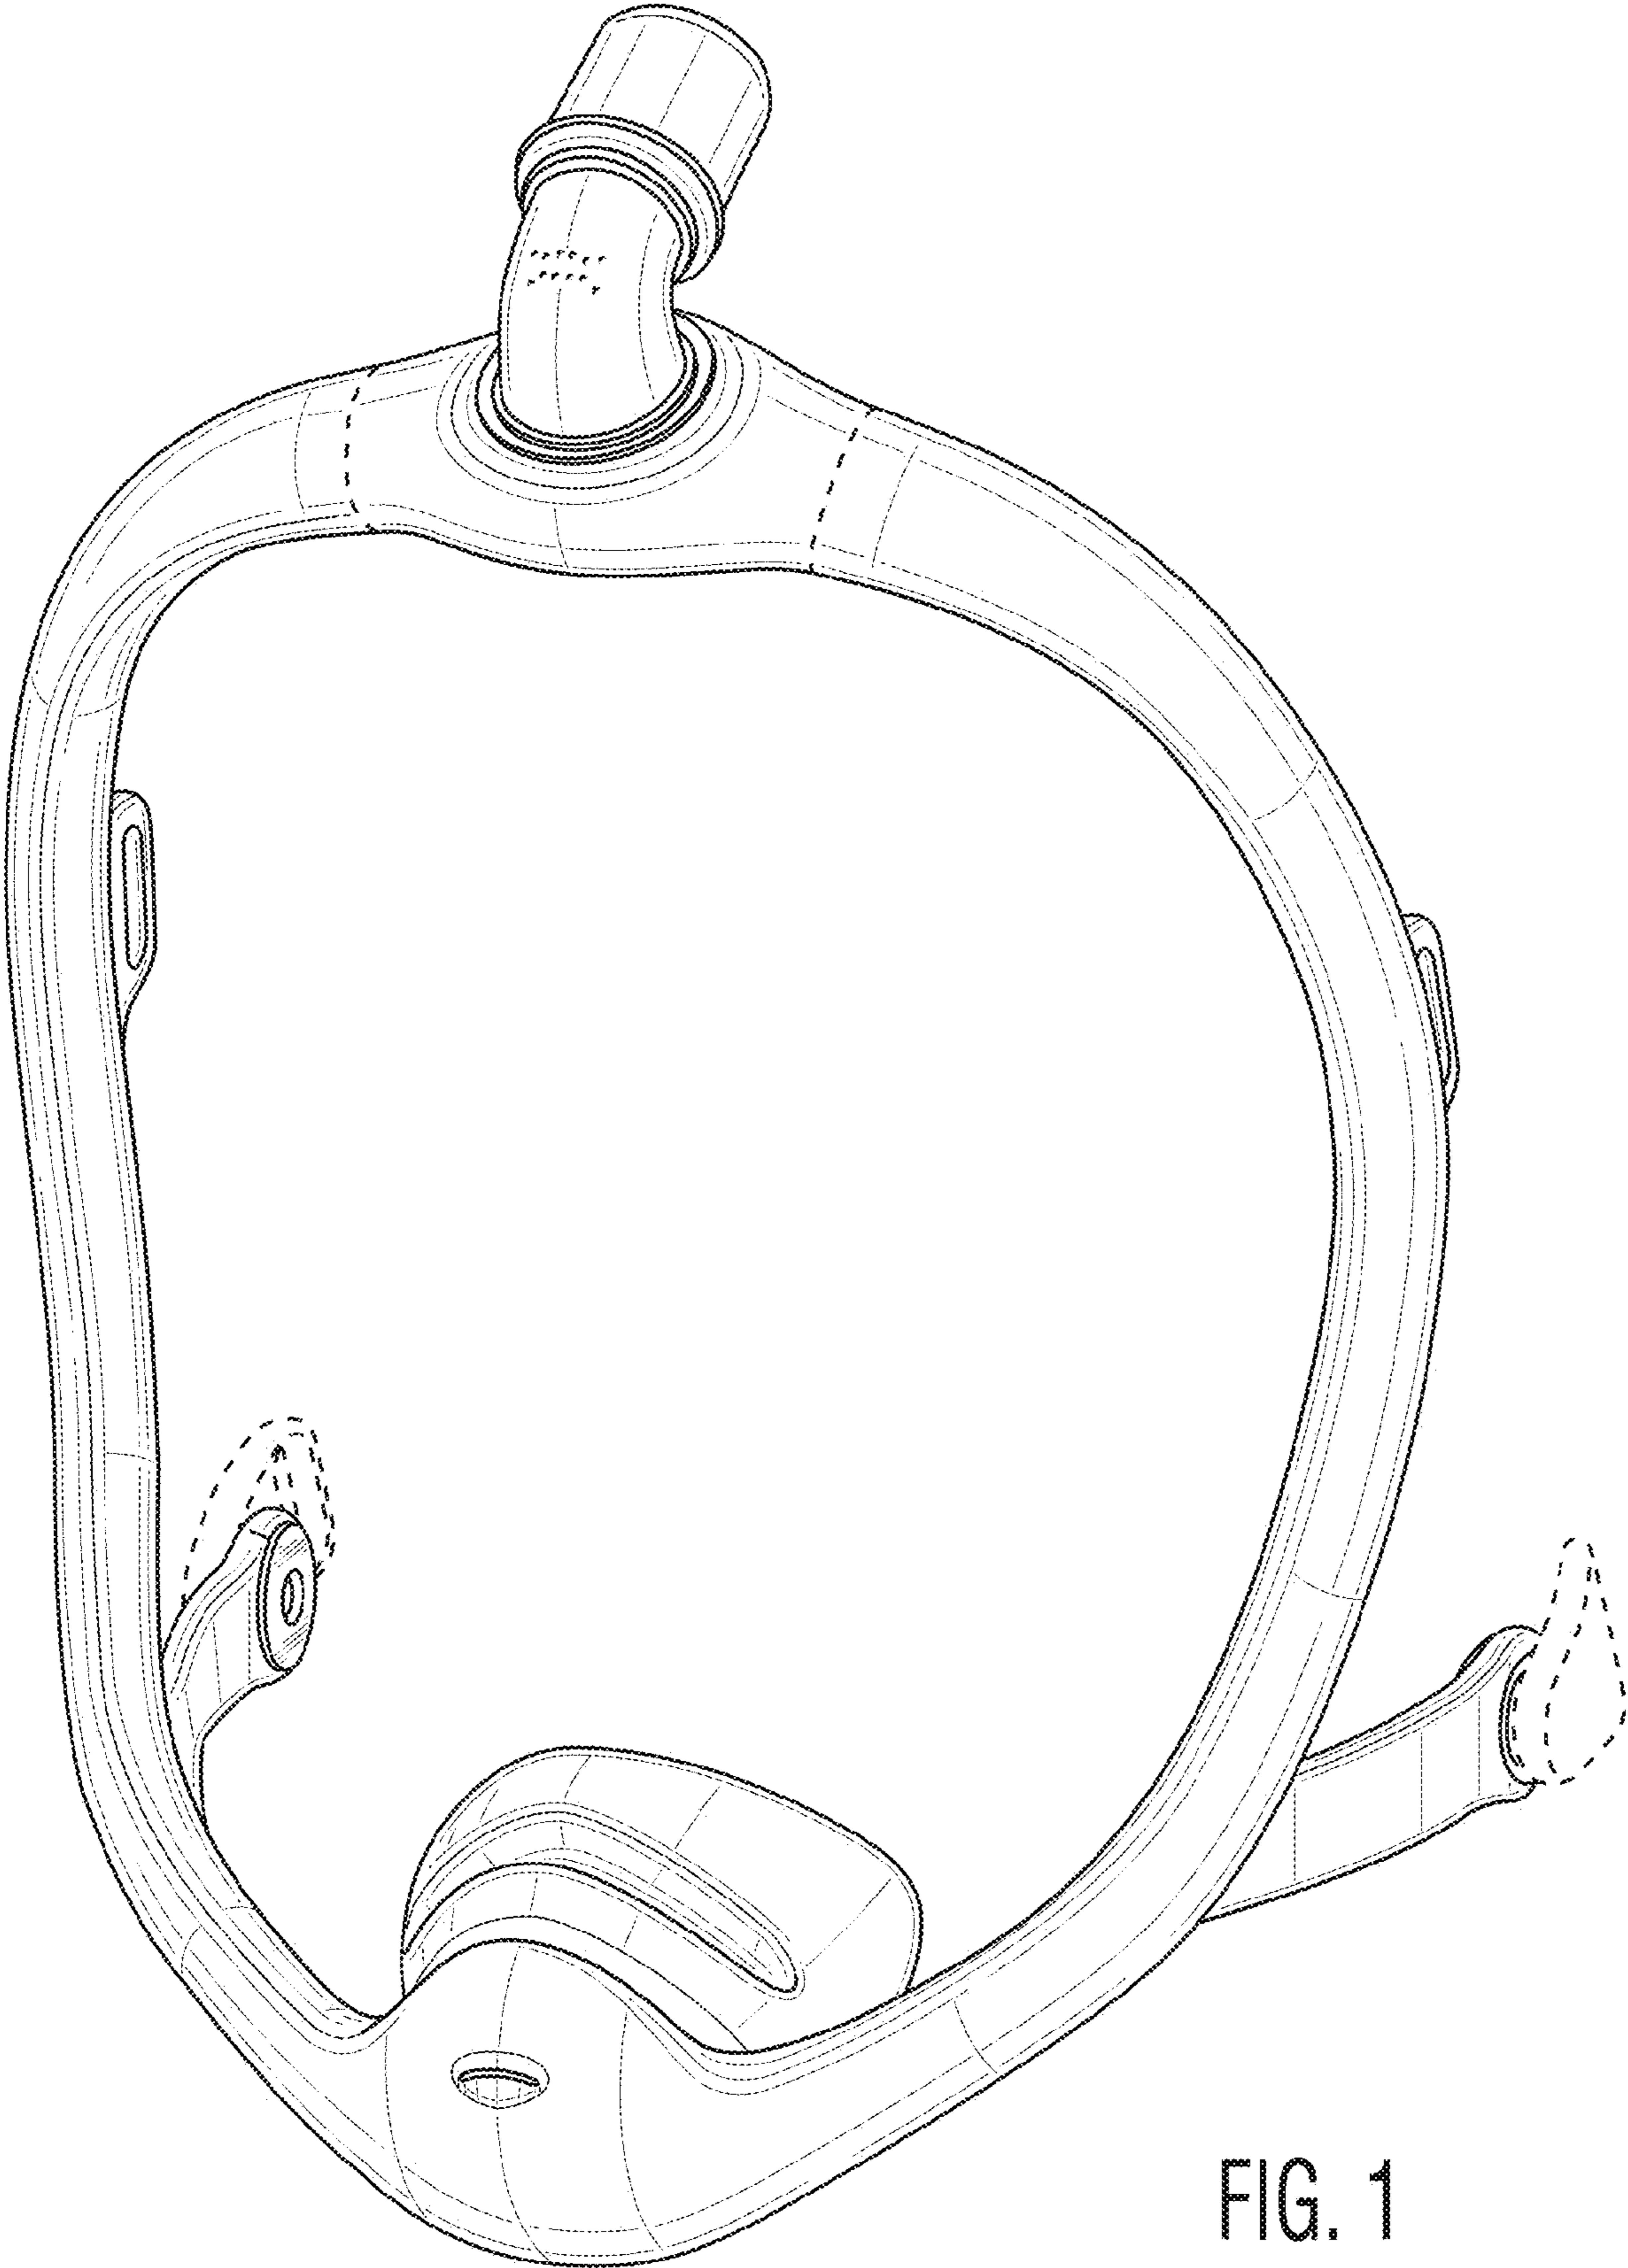


FIG. 1

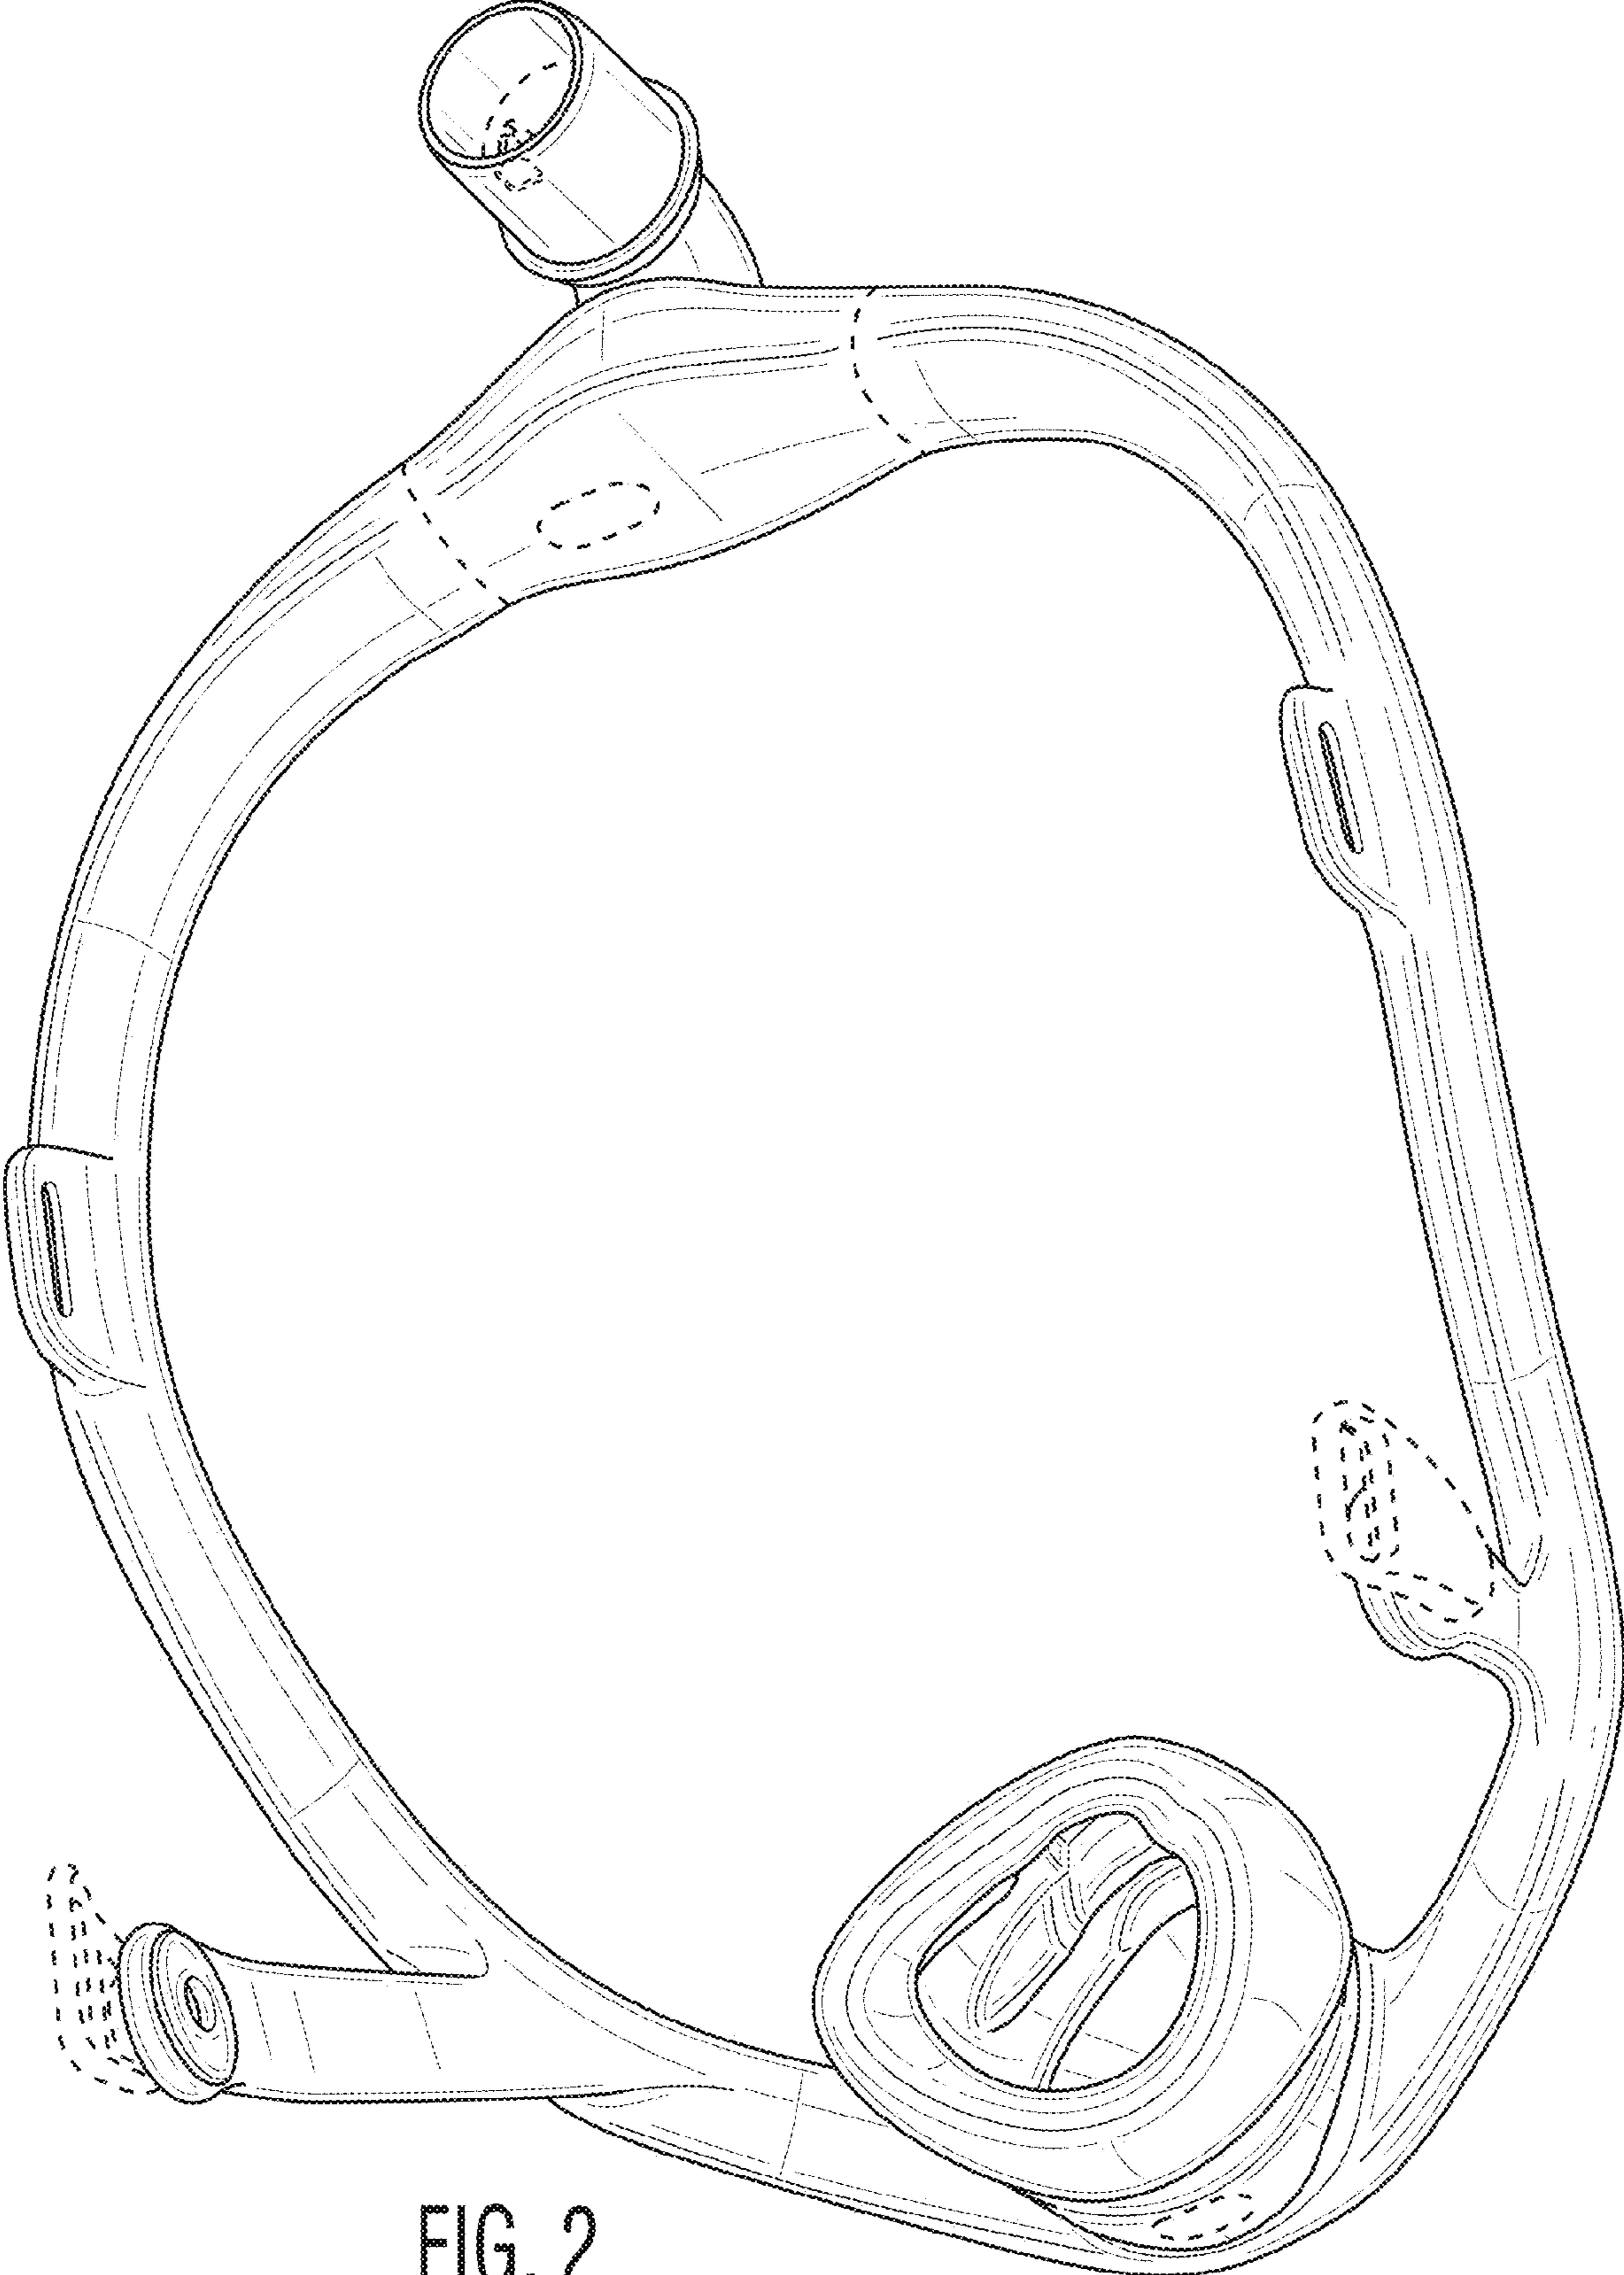


FIG. 2

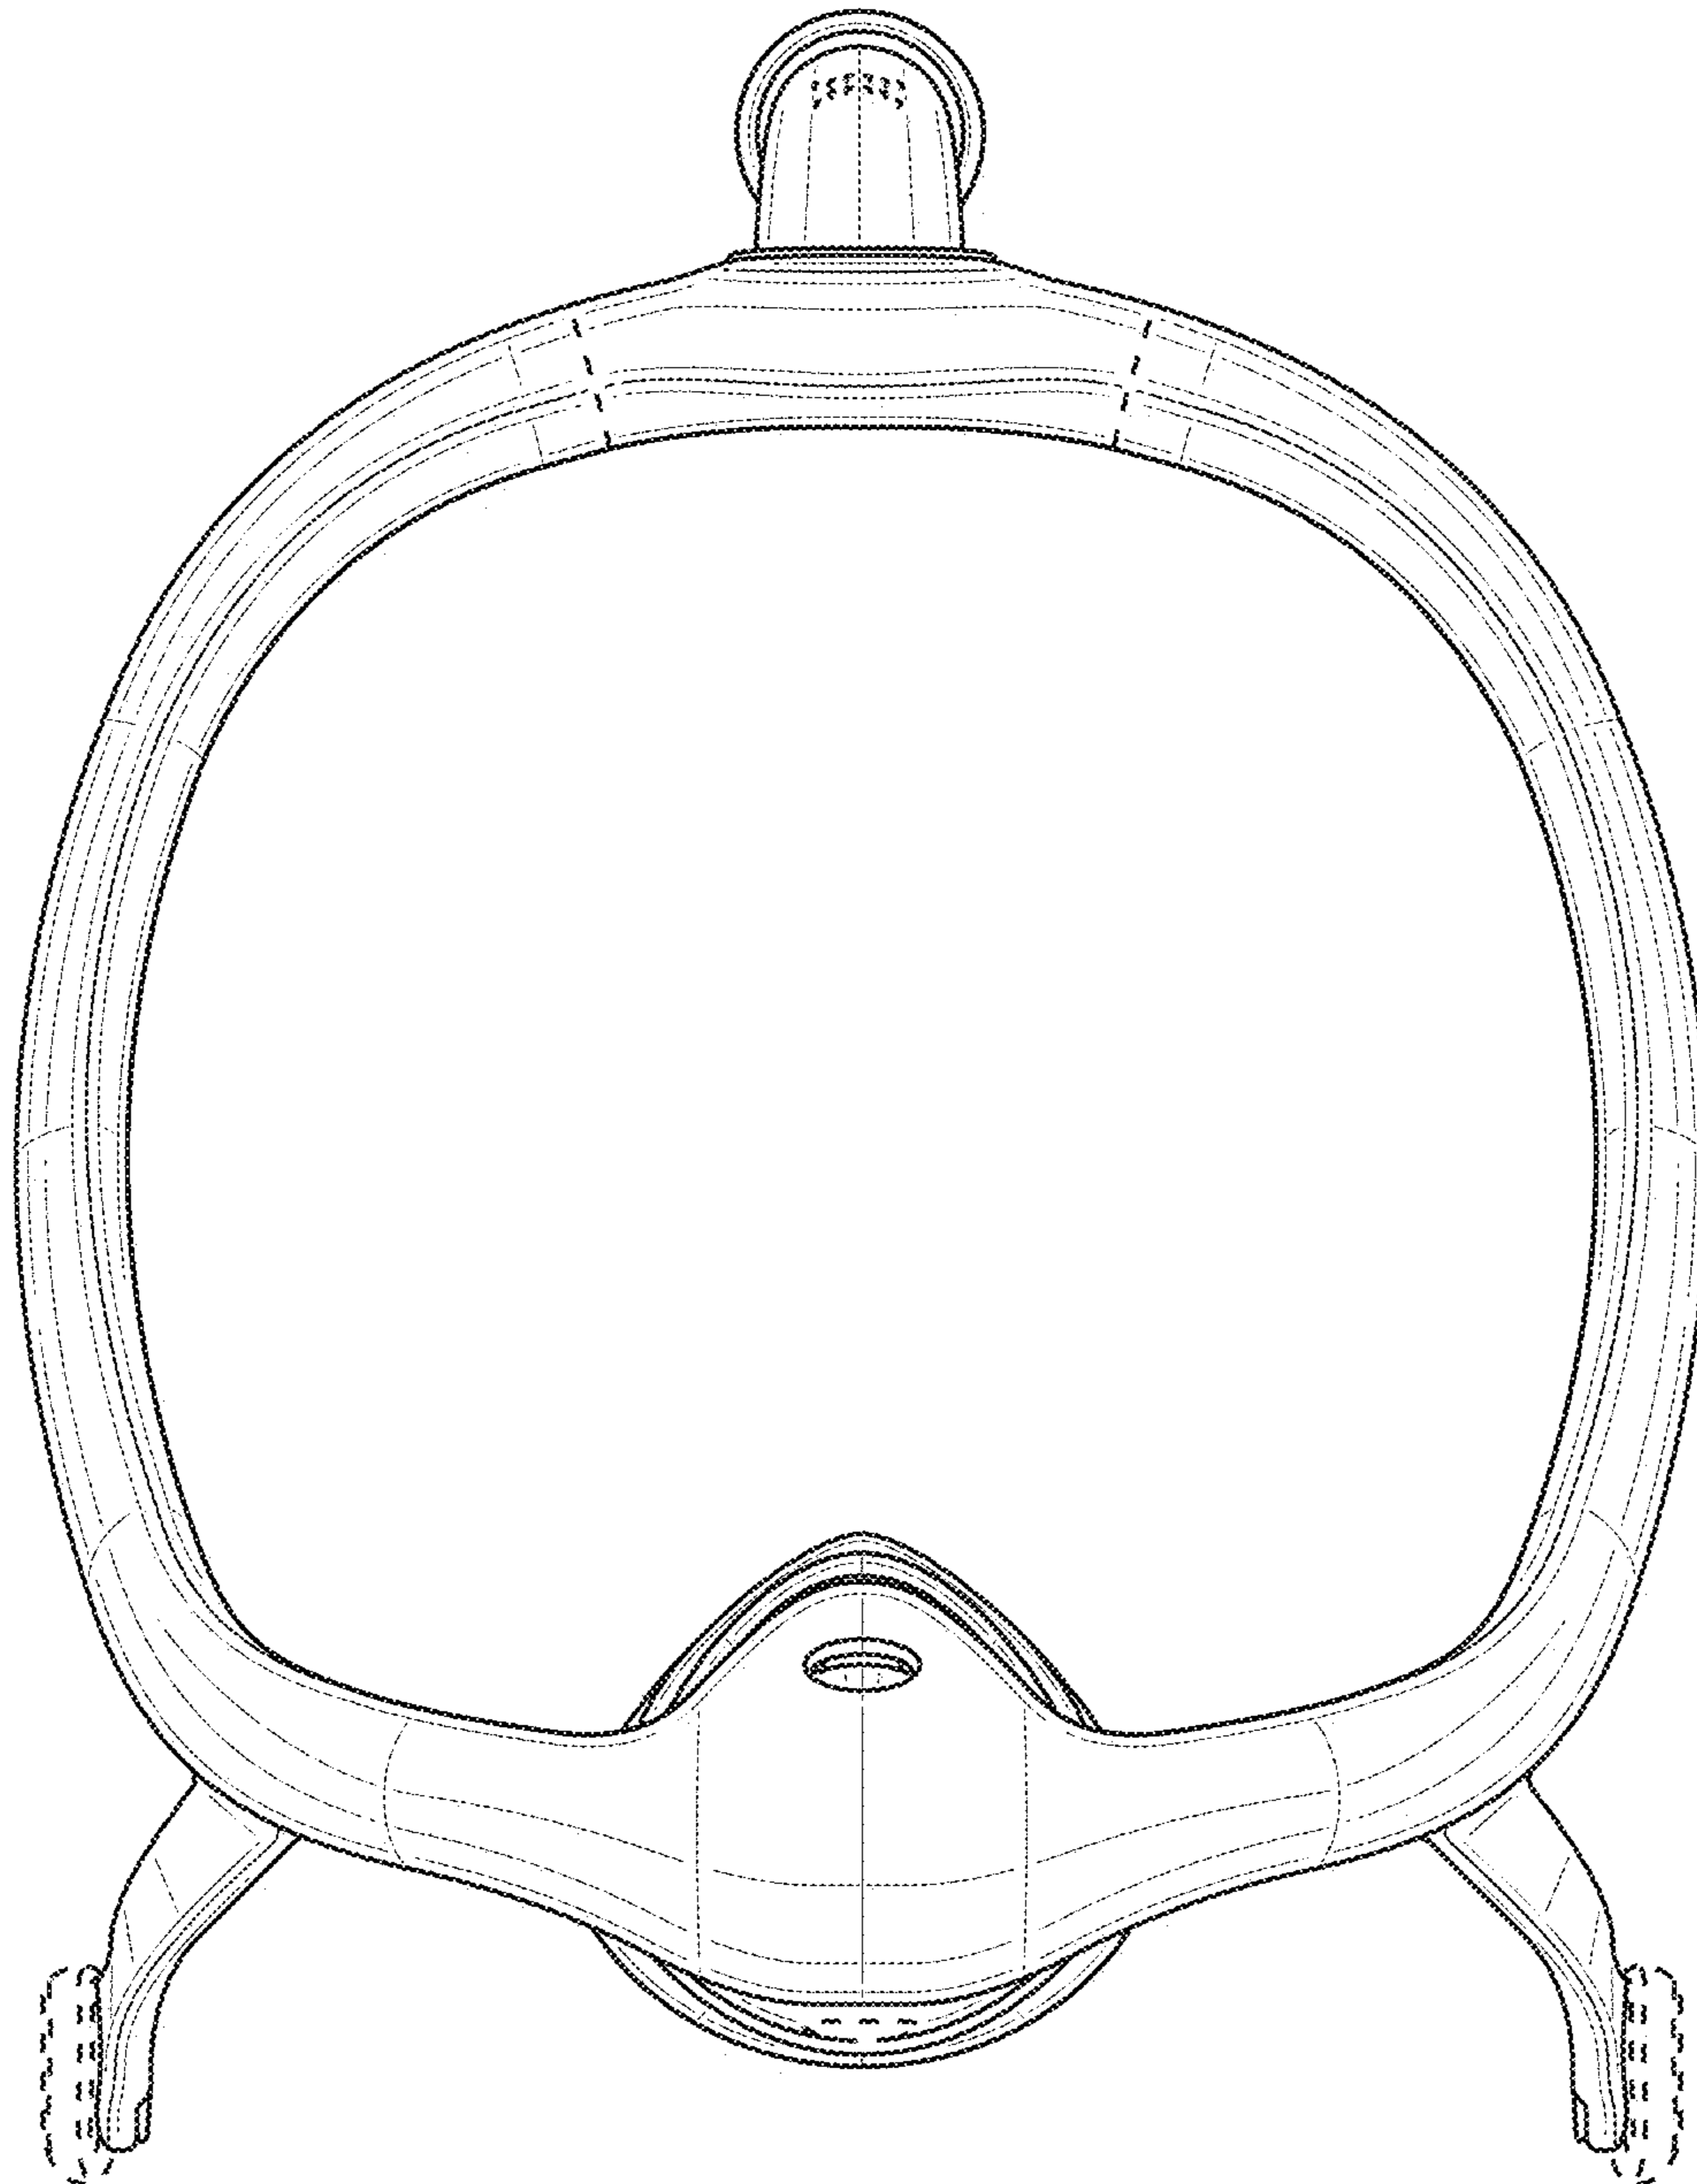


FIG. 3

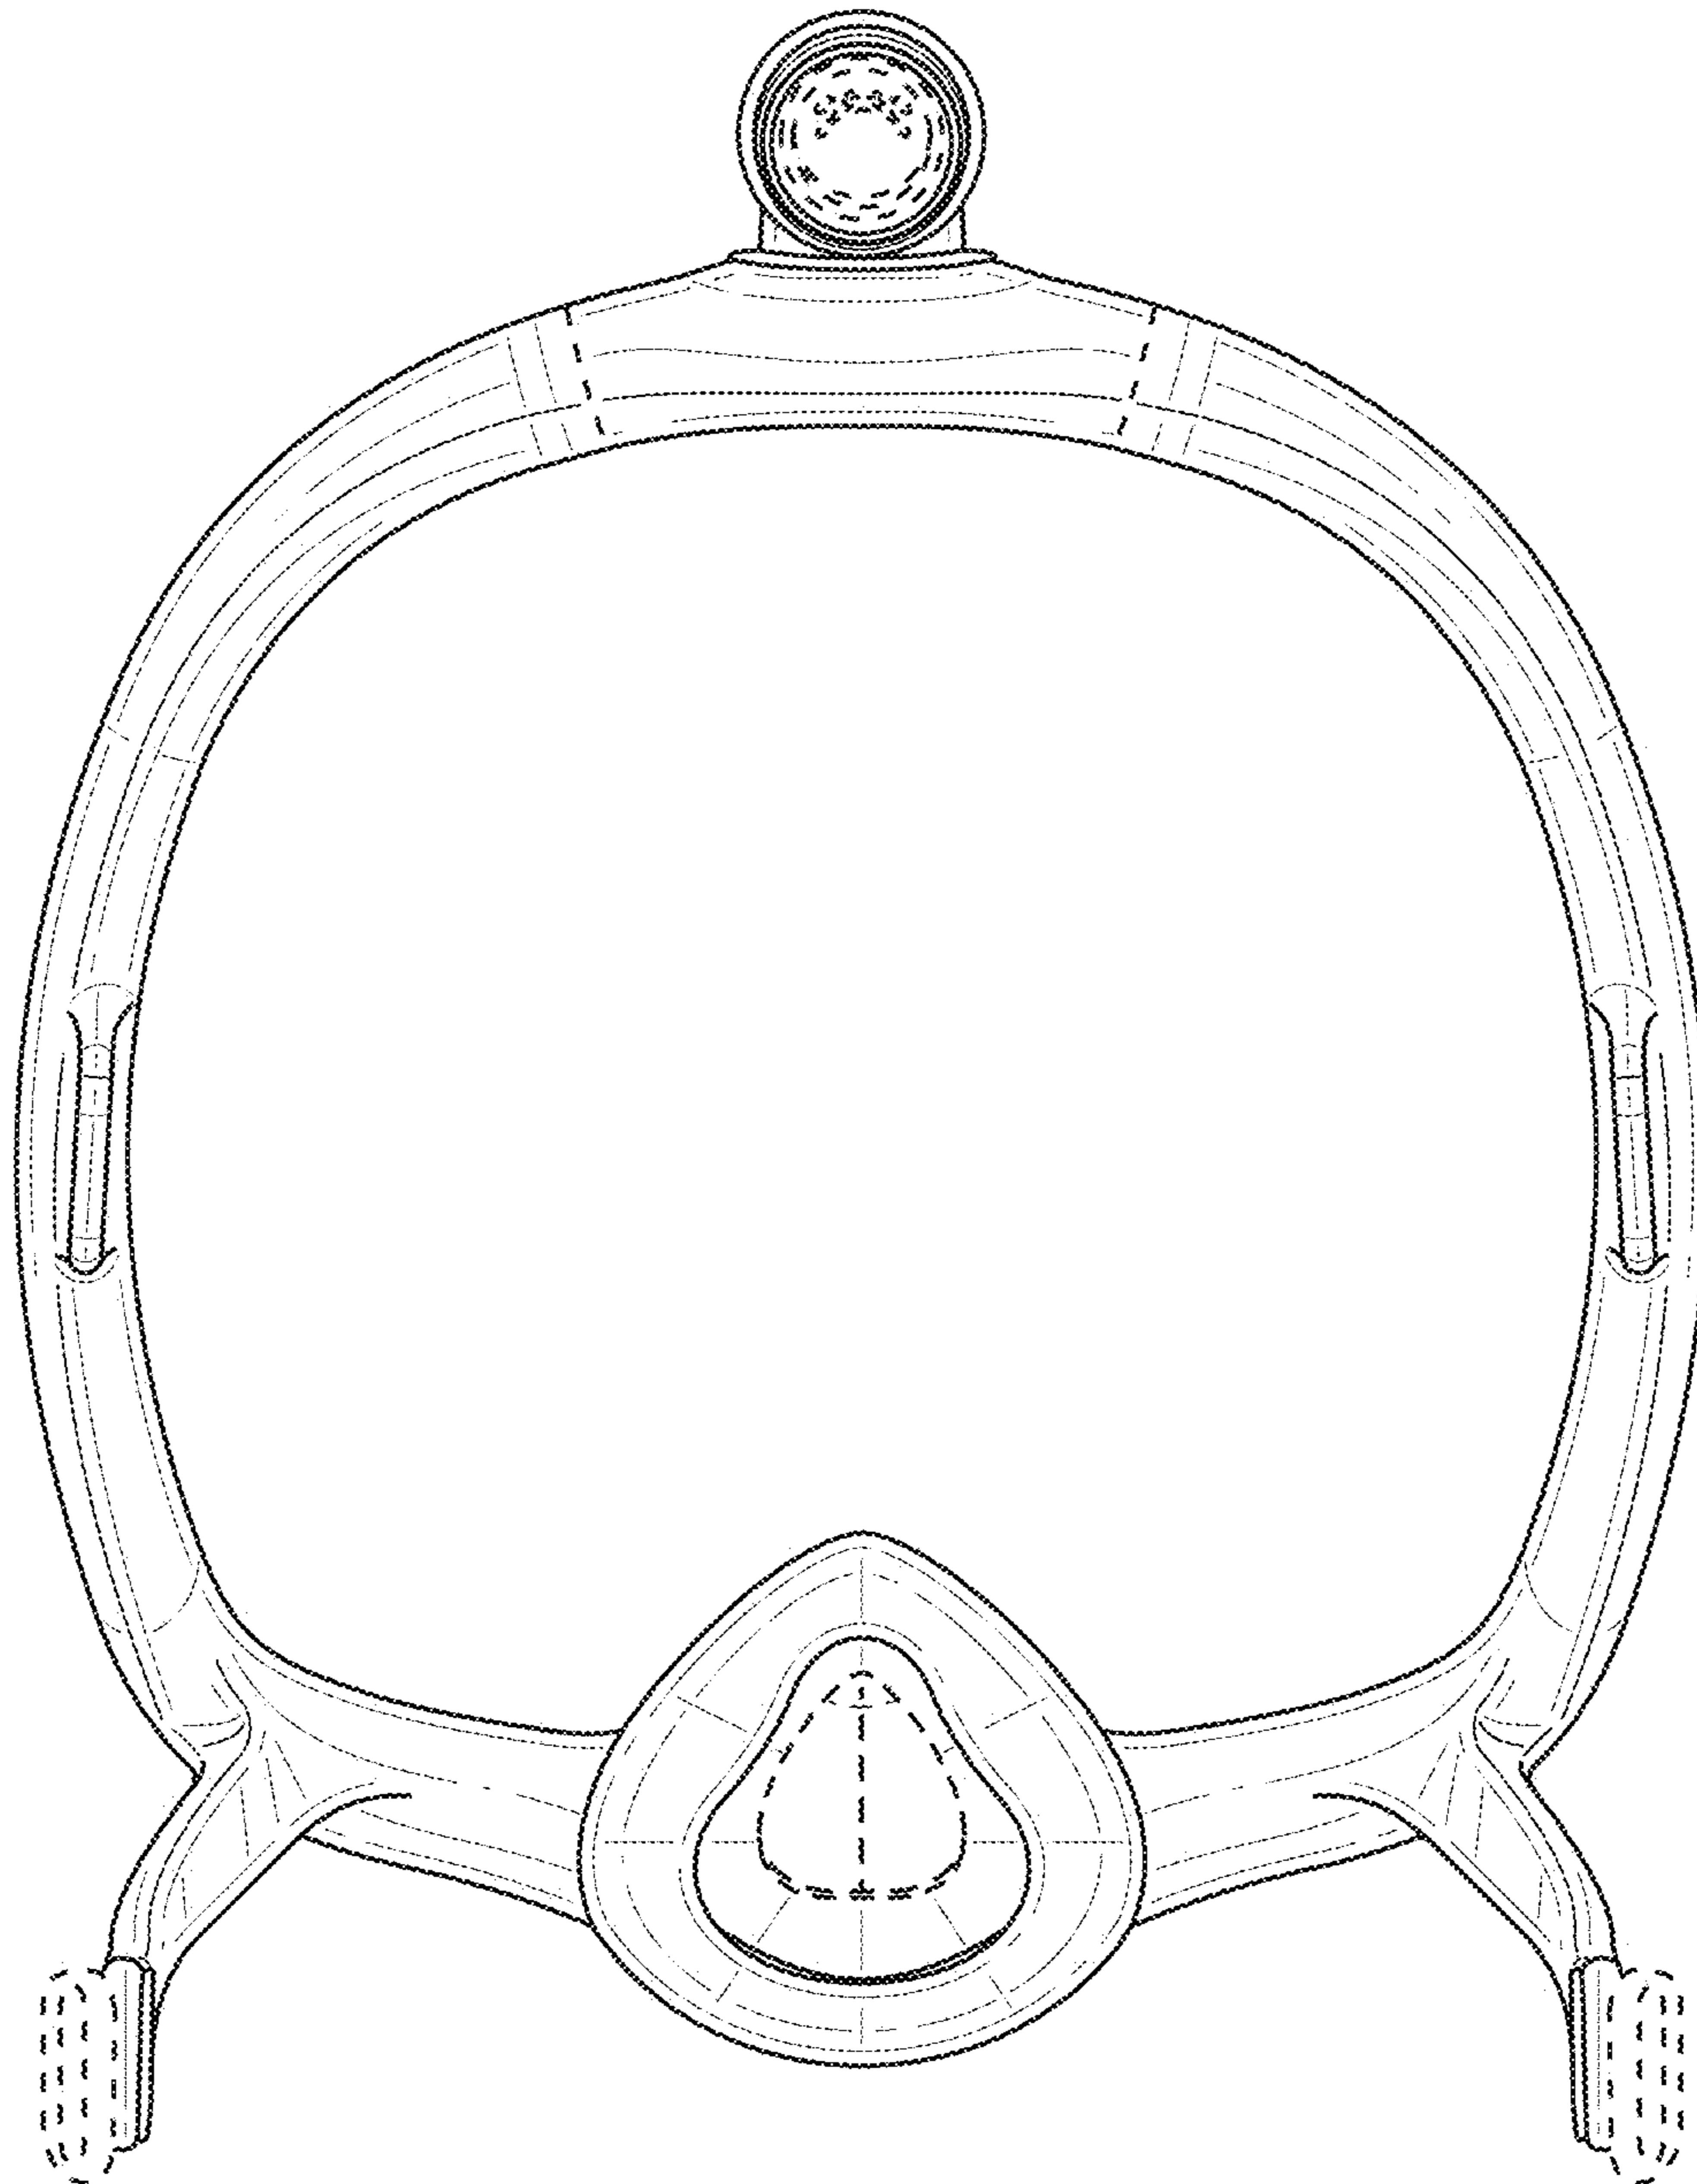


FIG. 4

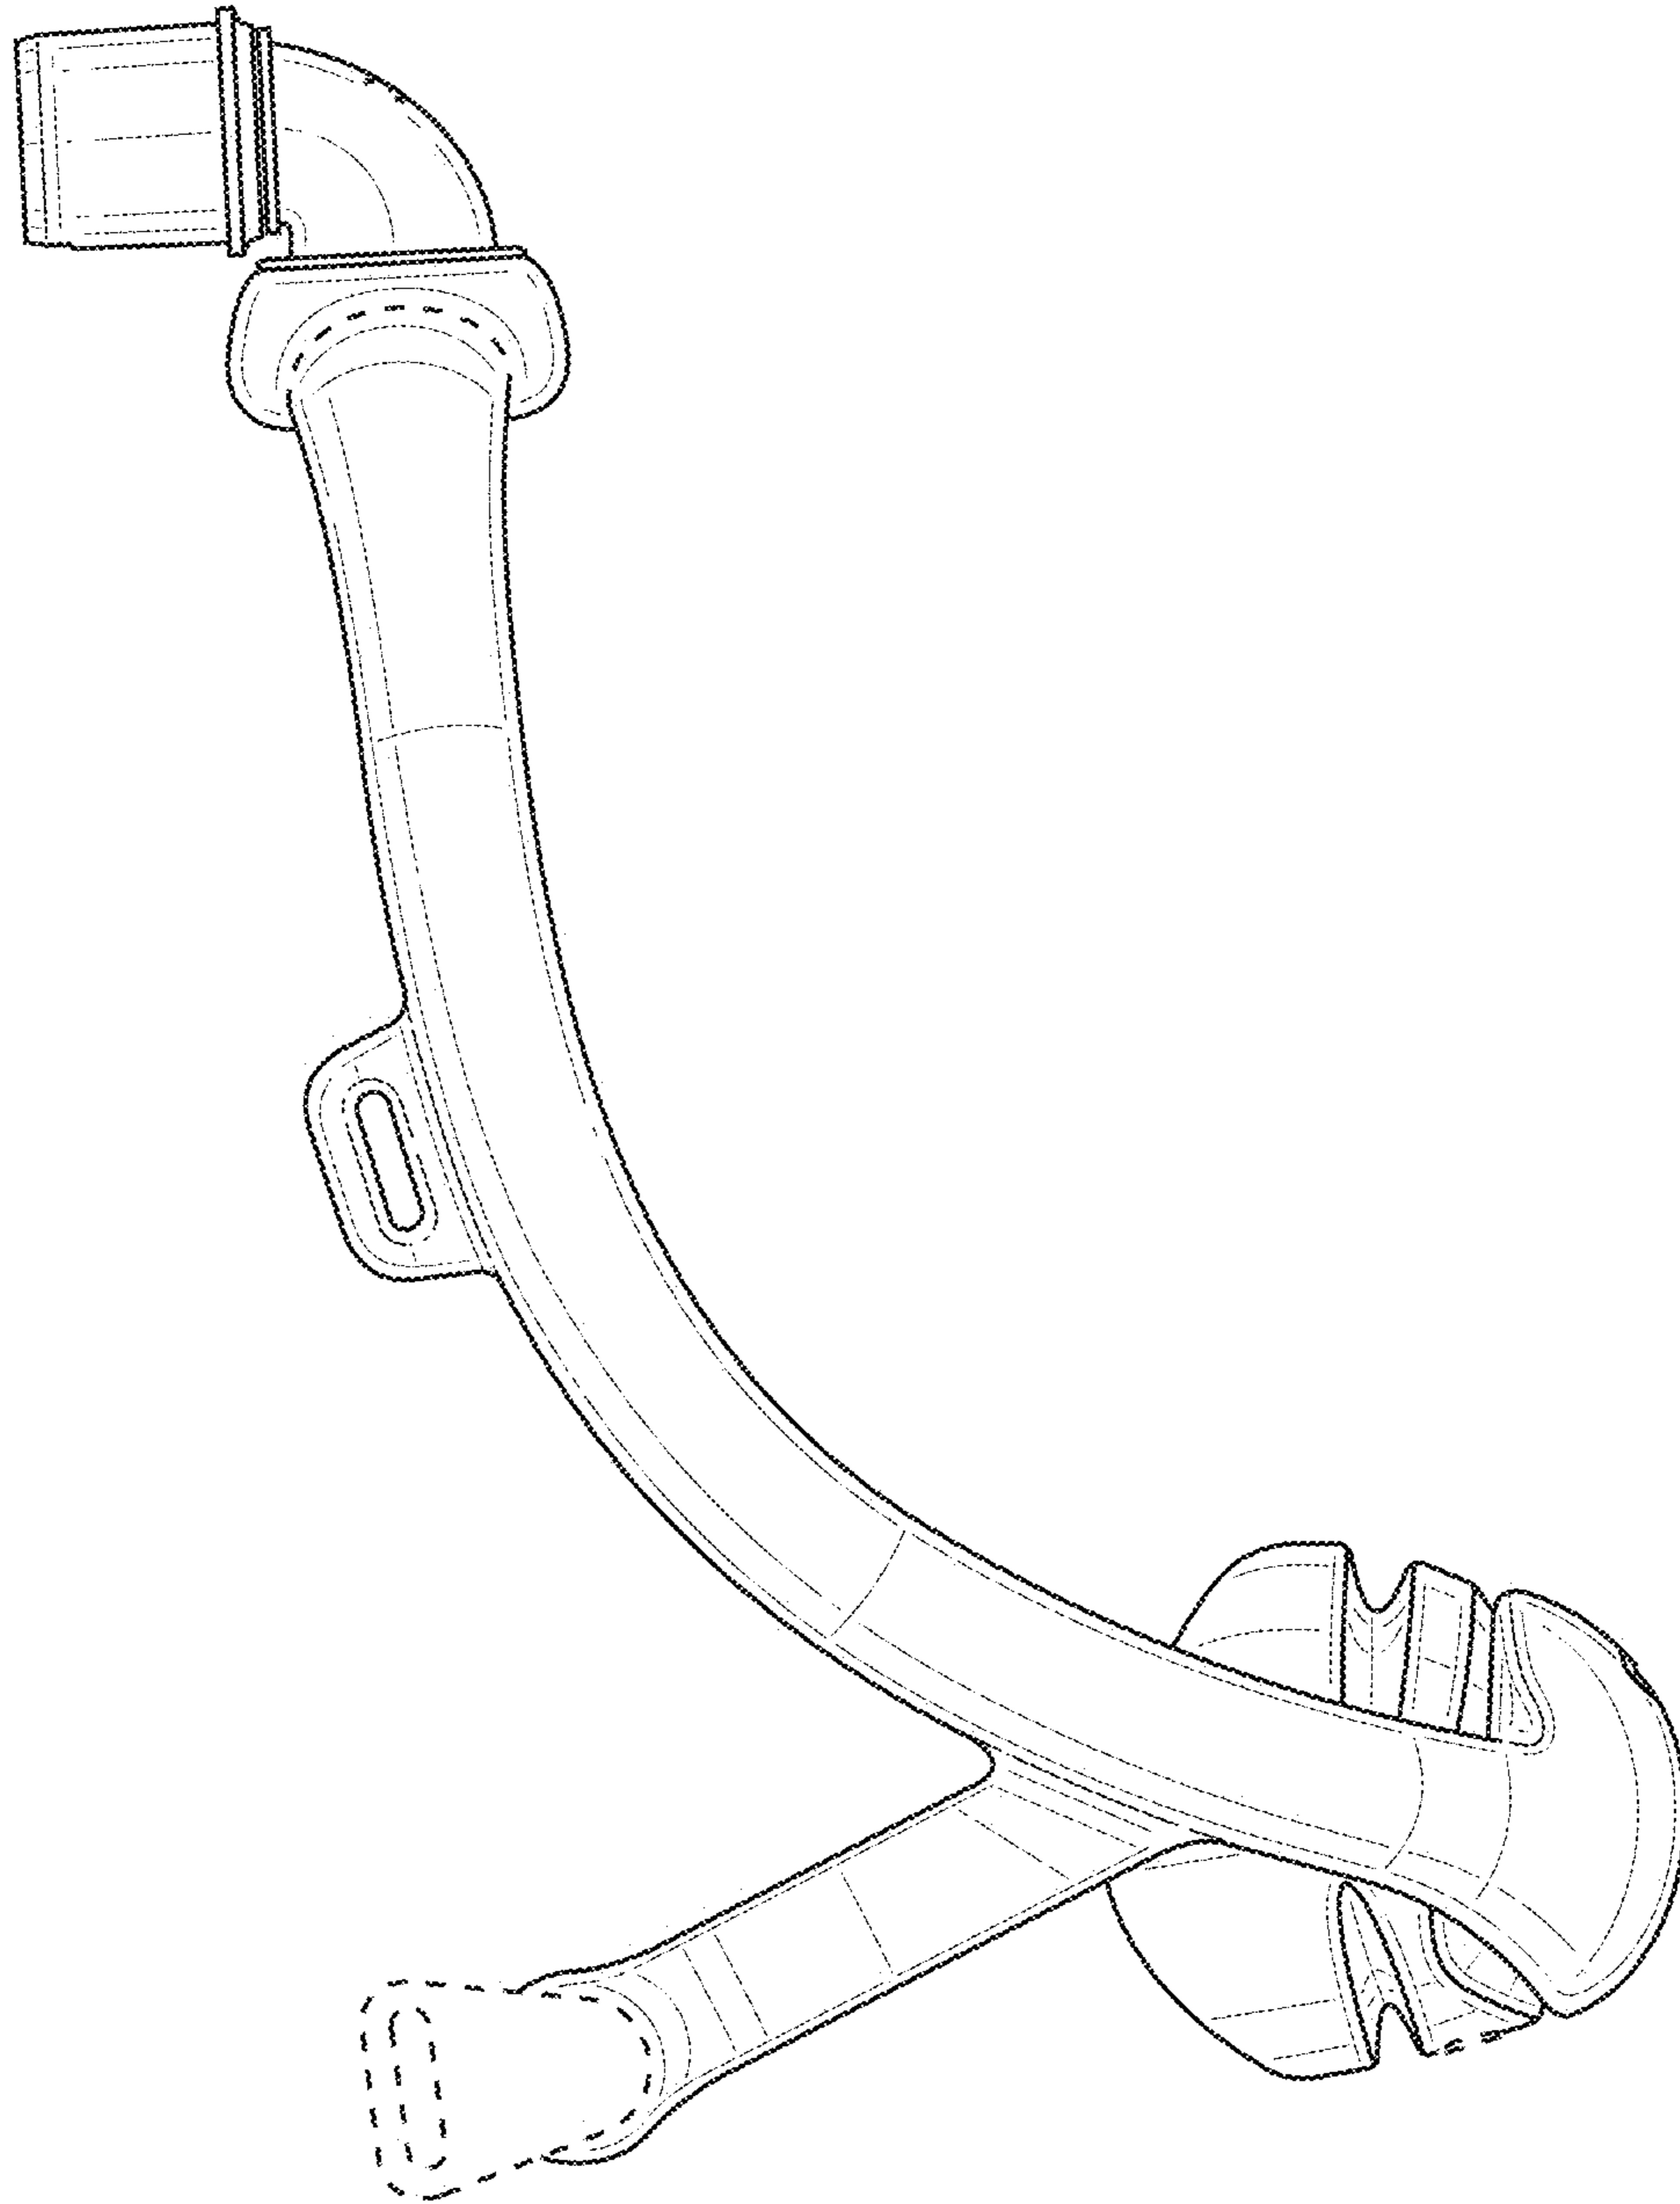


FIG. 5

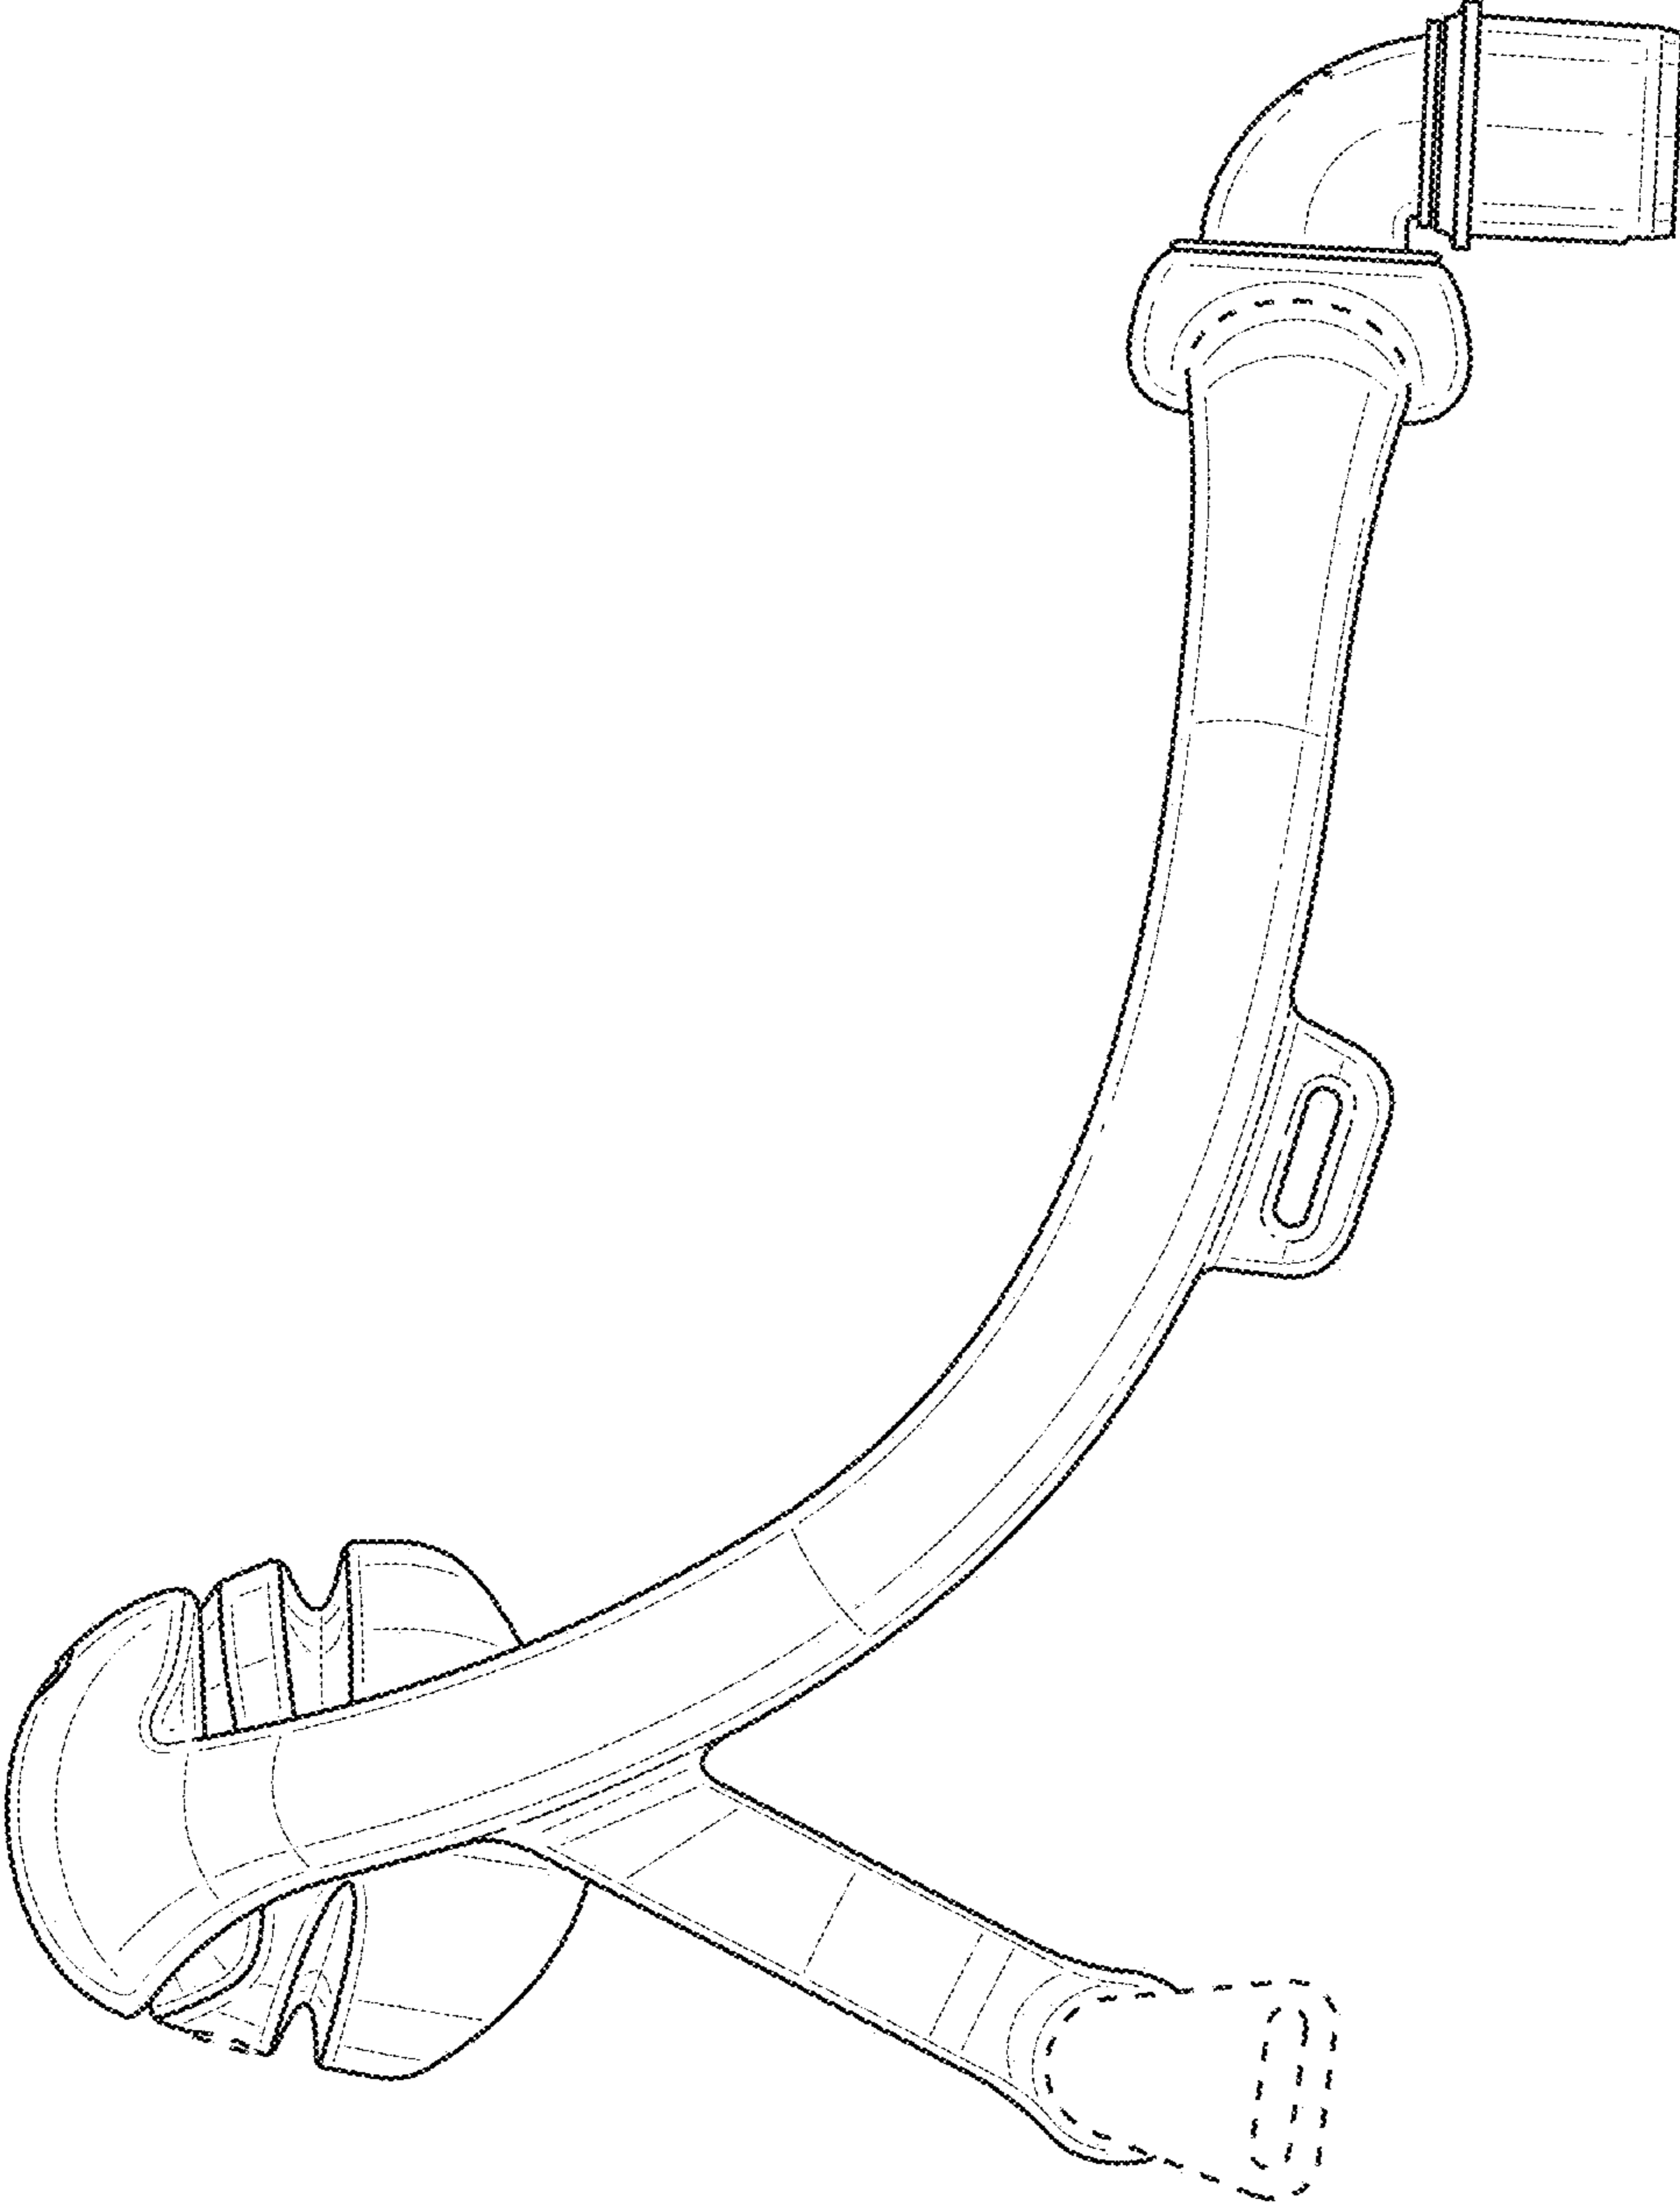


FIG. 6



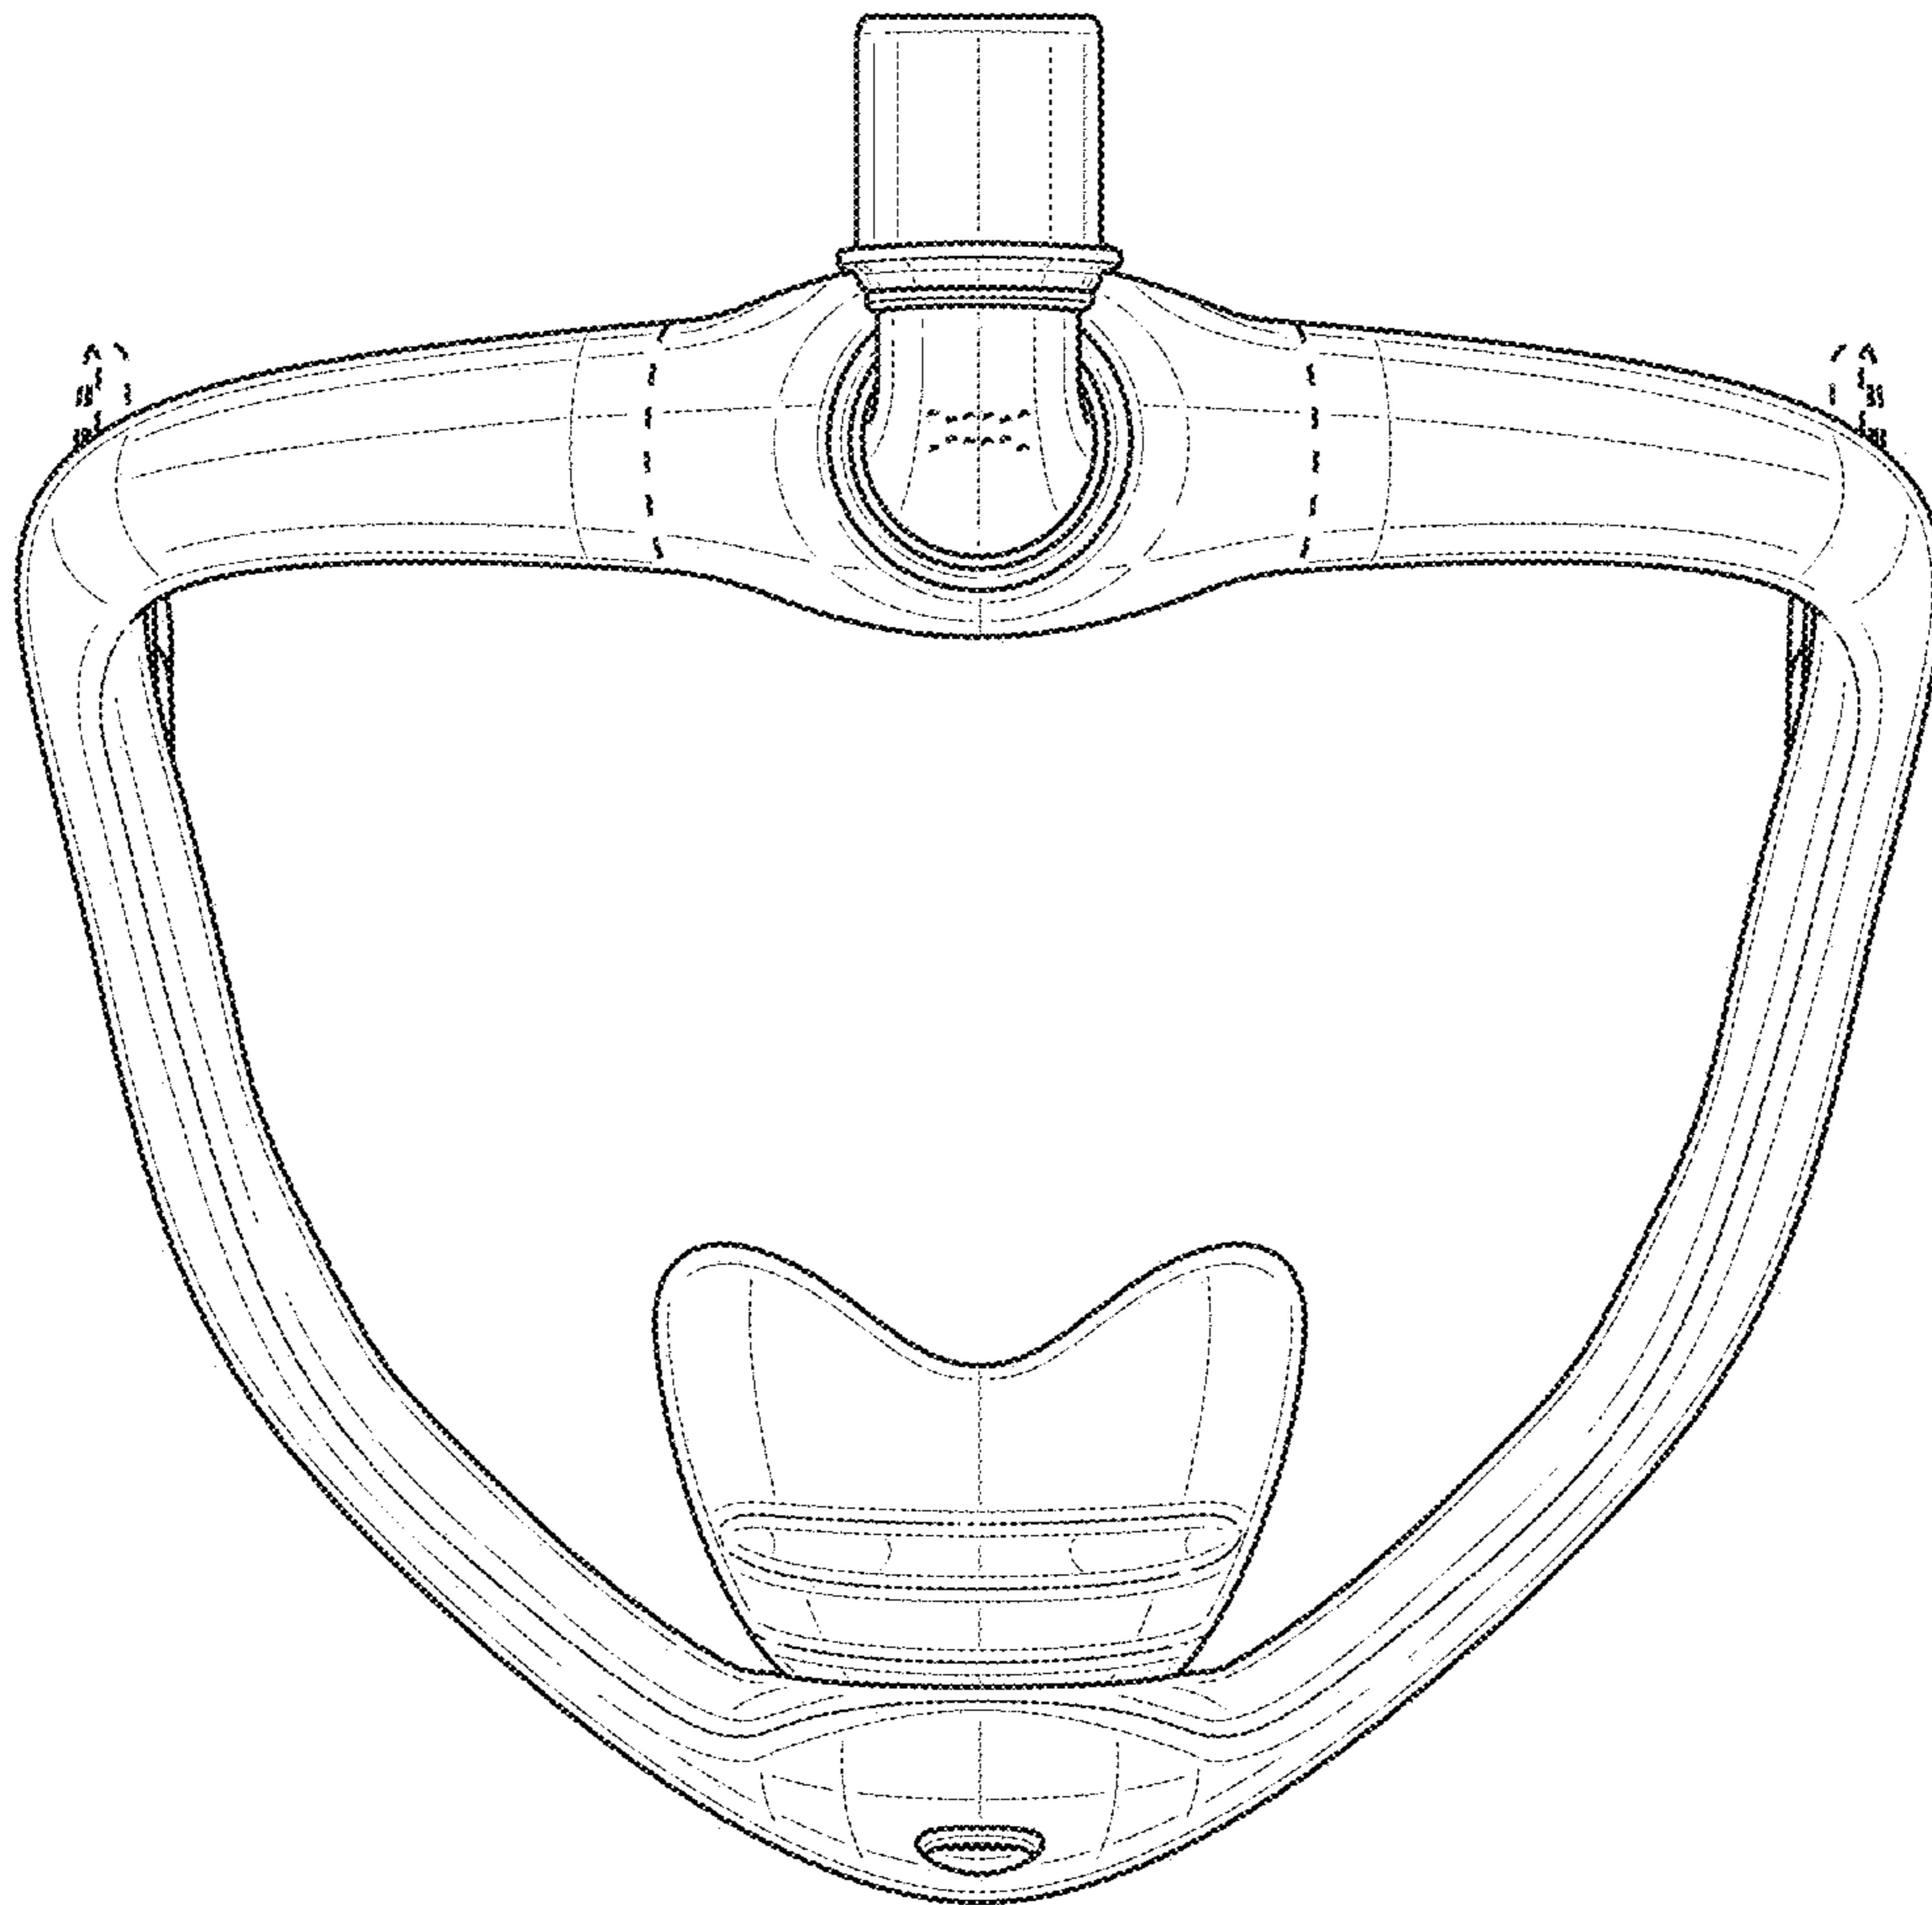


FIG. 7

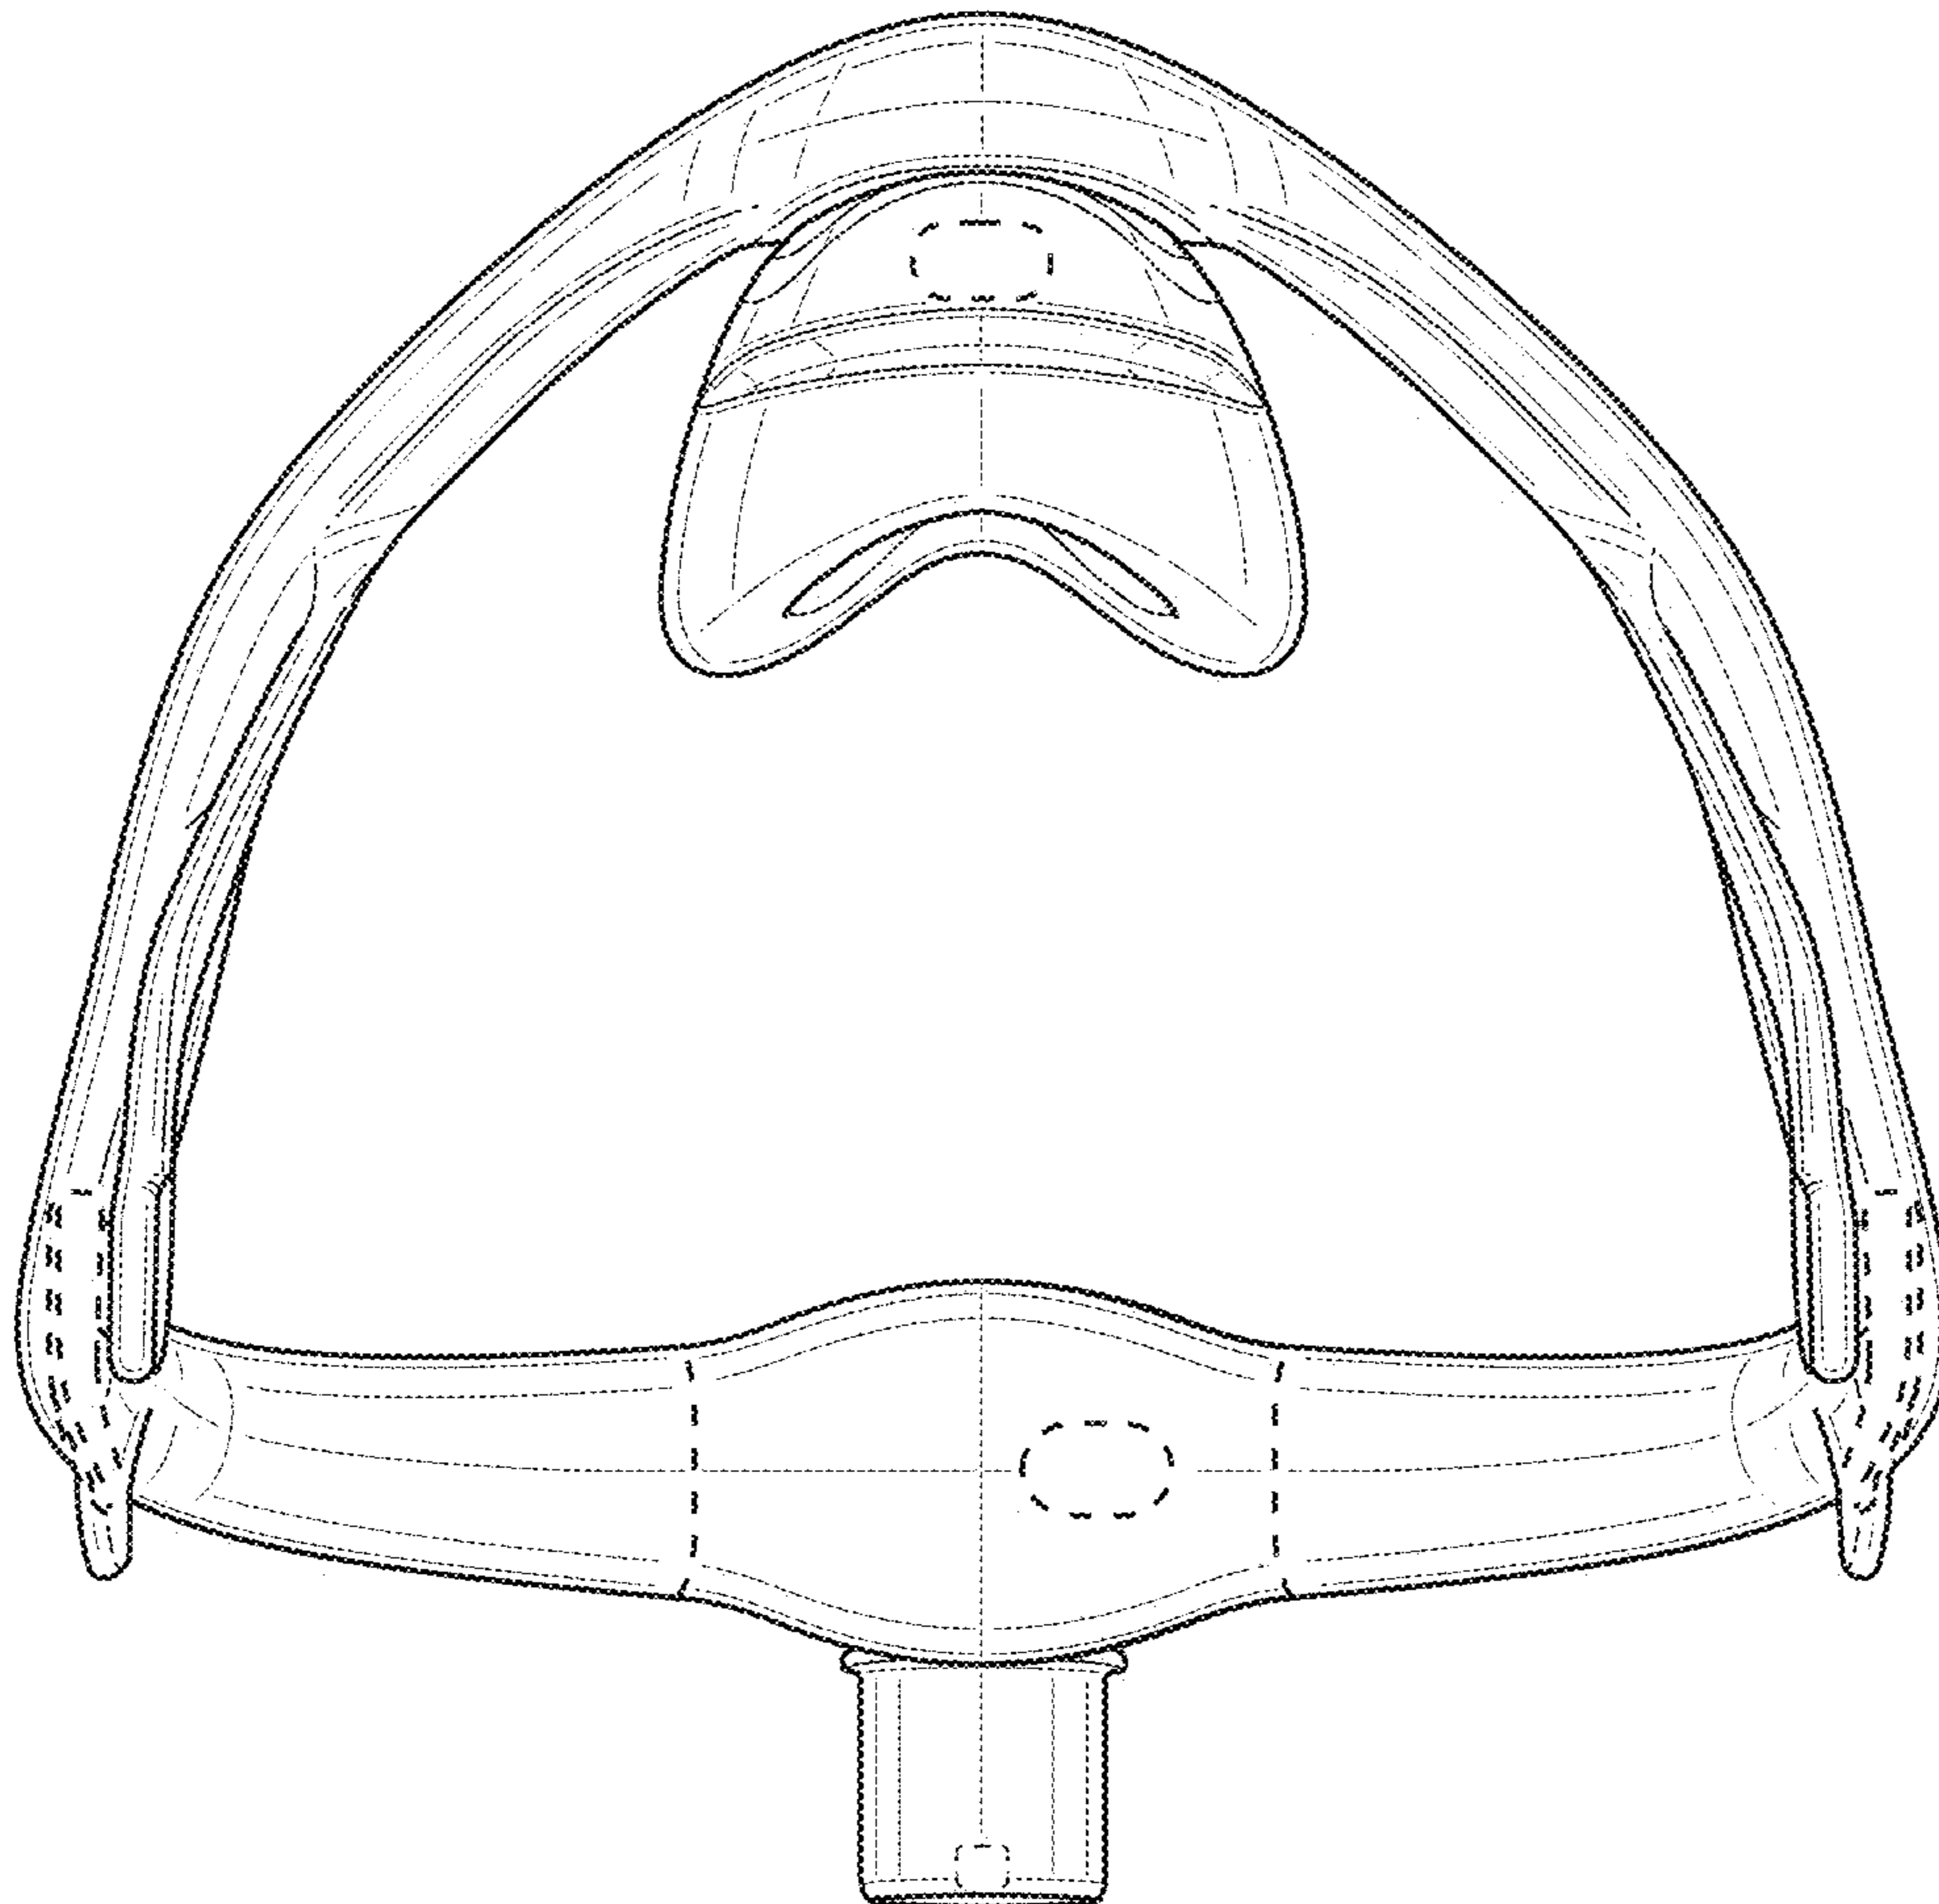


FIG. 8