



US00D978358S

(12) **United States Design Patent**
Laing et al.

(10) **Patent No.:** **US D978,358 S**

(45) **Date of Patent:** **** Feb. 14, 2023**

(54) **UROFLOWMETER**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **CLEARTRAC TECHNOLOGIES, LLC**, Elizabethton, TN (US)

CN 2221776 Y 3/1996
CN 105769223 A 7/2016

(Continued)

(72) Inventors: **Brent Laing**, Greenwood Village, CO (US); **John Green**, Elizabethton, TN (US); **Paul R. Johnson**, Boulder, CO (US); **Robert John Smith**, Louisville, CO (US); **Robert Edwin Schneider**, Erie, CO (US); **Magnus Hargis**, Hudson, CO (US); **Elise Geolat Edson**, Boulder, CO (US); **Elizabeth A. O'Brien**, Louisville, CO (US)

OTHER PUBLICATIONS

Drive Medical. "Drive Medical Folding Steel Bedside Commode, Grey." obtained Nov. 12, 2018 from <https://www.amazon.com/Drive-Medical-Folding-Bedside-Commode/dp/B001HP7AQE/ref=sr_1_3?s=industrial&ie=UTF8&qid=1539732631&sr=1-3&keywords=commode>, 8 pages.

(Continued)

(73) Assignee: **CLEARTRAC TECHNOLOGIES, LLC**, Elizabethton, TN (US)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Dorsey & Whitney LLP

(**) Term: **15 Years**

(57) **CLAIM**

(21) Appl. No.: **29/810,290**

The ornamental design for a uroflowmeter, as shown and described.

(22) Filed: **Oct. 4, 2021**

DESCRIPTION

Related U.S. Application Data

(63) Continuation of application No. 29/656,567, filed on Jul. 13, 2018, now Pat. No. Des. 932,632.

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/186**; D24/122

(58) **Field of Classification Search**
USPC D24/107, 121, 122, 129, 130, 186, 216, D24/217, 223–227, 231, 232, 133; D10/81, 96, 102; D7/691

(Continued)

FIG. 1 shows a front perspective view of a uroflowmeter; FIG. 2 shows a rear perspective view of the uroflowmeter of FIG. 1; FIG. 3 shows a right elevation view of the uroflowmeter of FIG. 1; FIG. 4 shows a left elevation view of the uroflowmeter of FIG. 1; FIG. 5 shows a front elevation view of the uroflowmeter of FIG. 1; FIG. 6 shows a rear elevation view of the uroflowmeter of FIG. 1; FIG. 7 shows a top view of the piece of the uroflowmeter of FIG. 1; and, FIG. 8 shows a bottom view of the uroflowmeter of FIG. 1. The broken lines in FIGS. 1-8 illustrate portions of the uroflowmeter and form no part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

2,648,981 A 8/1953 Drake
3,172,130 A 3/1965 Lange

(Continued)

1 Claim, 4 Drawing Sheets

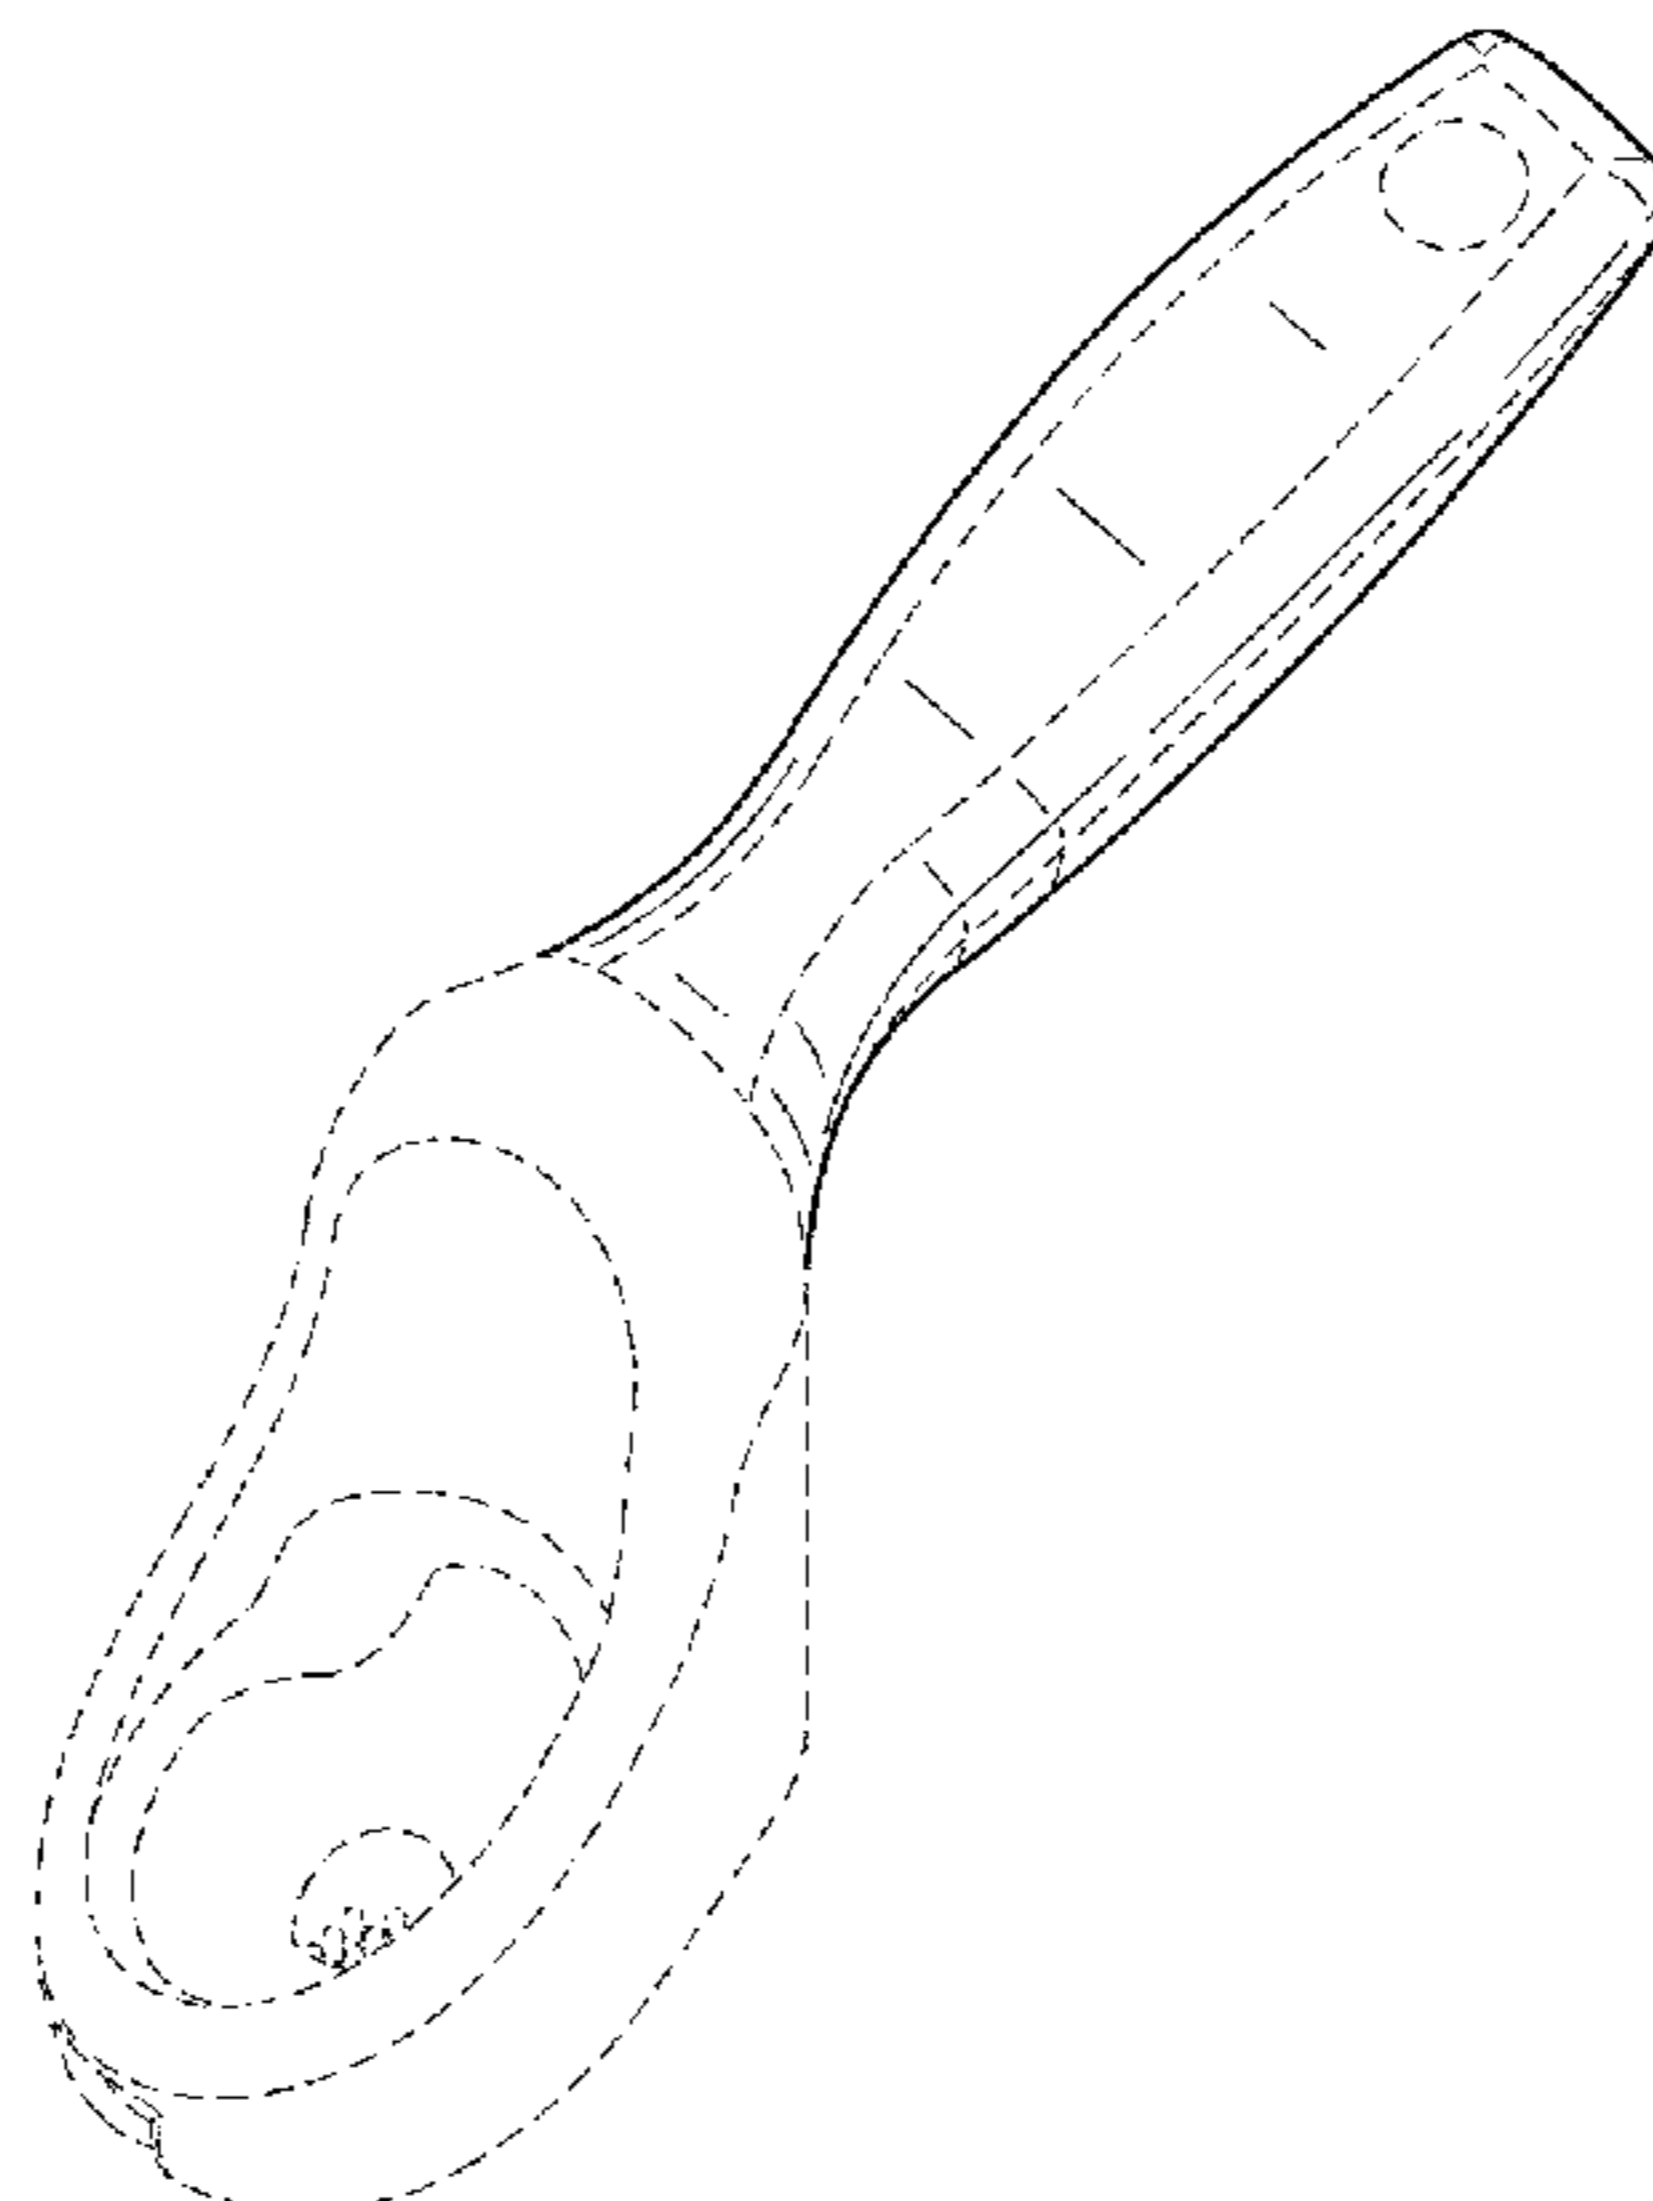

(58) **Field of Classification Search**
 CPC A61B 10/007; A61B 5/205; A61B 5/207;
 A61B 5/208
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|-----------|------|---------|-------------------------------------|--|
| 3,219,276 | A | 11/1965 | Norris | |
| 3,859,854 | A | 1/1975 | Dye et al. | |
| 3,871,230 | A | 3/1975 | Dye et al. | |
| 3,884,072 | A | 5/1975 | Cheng | |
| 3,929,412 | A | 12/1975 | Villari | |
| 3,931,972 | A | 1/1976 | Fabian | |
| 4,051,431 | A | 9/1977 | Wurster | |
| 4,085,616 | A | 4/1978 | Patel et al. | |
| 4,131,016 | A | 12/1978 | Layton | |
| 4,238,448 | A | 12/1980 | Layton et al. | |
| 4,343,316 | A | 8/1982 | Jespersen | |
| 4,554,687 | A | 11/1985 | Carter et al. | |
| 4,569,090 | A | 2/1986 | Muller | |
| 4,576,076 | A | 3/1986 | Pyle | |
| 4,619,273 | A | 10/1986 | Iosif | |
| D296,360 | S | 6/1988 | Oelberg | |
| 4,832,046 | A | 5/1989 | Parrish | |
| 4,891,993 | A | 1/1990 | Barker | |
| 5,046,510 | A | 9/1991 | Ams et al. | |
| 5,062,304 | A | 11/1991 | Van et al. | |
| 5,176,148 | A | 1/1993 | Wiest et al. | |
| 5,186,394 | A | 2/1993 | Tsuji | |
| D340,768 | S | 10/1993 | Jabour | |
| 5,377,101 | A | 12/1994 | Rollema | |
| 5,422,076 | A | 6/1995 | Jones | |
| D378,129 | S | 2/1997 | Wexler et al. | |
| 5,794,541 | A | 8/1998 | Hirose | |
| D422,851 | S | 4/2000 | Joergensen | |
| D425,365 | S | 5/2000 | Chien | |
| D436,801 | S | 1/2001 | Wonderley | |
| 6,398,742 | B1 | 6/2002 | Kim | |
| D460,328 | S | 7/2002 | De Groote et al. | |
| D461,105 | S | 8/2002 | Law | |
| 6,651,259 | B1 | 11/2003 | Hartman et al. | |
| D492,995 | S | 7/2004 | Rue et al. | |
| D494,279 | S | 8/2004 | Cogan et al. | |
| 6,889,563 | B2 | 5/2005 | Tomita et al. | |
| 6,904,809 | B1 | 6/2005 | Aundal | |
| 6,931,943 | B1 | 8/2005 | Aundal | |
| D545,621 | S | 7/2007 | Hood | |
| D551,032 | S | 9/2007 | Lion et al. | |
| D552,431 | S | 10/2007 | Chou | |
| D572,089 | S | 7/2008 | Tey et al. | |
| 7,416,542 | B2 | 8/2008 | Aundal | |
| D598,251 | S | 8/2009 | Ikoma et al. | |
| 7,606,617 | B2 | 10/2009 | Wariar | |
| 7,739,907 | B2 | 6/2010 | Boiarski | |
| D619,246 | S | 7/2010 | Hazeres | |
| 7,762,596 | B1 * | 7/2010 | Gaydos A01K 23/005 600/573 | |
| 7,819,020 | B2 | 10/2010 | Jacobi et al. | |
| 7,892,217 | B2 | 2/2011 | Boiarski | |
| 8,141,420 | B2 | 3/2012 | Hirao | |
| D659,558 | S | 5/2012 | Johnson et al. | |
| 8,231,552 | B2 | 7/2012 | Shahar et al. | |
| 8,424,376 | B2 | 4/2013 | Boiarski | |
| D681,392 | S | 5/2013 | Dichraff et al. | |
| D688,370 | S | 8/2013 | Desai | |
| 8,500,705 | B2 | 8/2013 | Kim | |
| 8,544,341 | B2 | 10/2013 | Grumbles et al. | |
| 8,574,492 | B2 | 11/2013 | Morita et al. | |
| D709,185 | S * | 7/2014 | Queiroli D24/122 | |
| 8,813,551 | B2 | 8/2014 | Boiarski | |
| 9,021,878 | B2 | 5/2015 | Grinstein et al. | |
| D736,043 | S | 8/2015 | Lee et al. | |
| D770,613 | S | 11/2016 | Roberts | |
| 9,642,737 | B2 | 5/2017 | Seres et al. | |
| 9,775,556 | B2 | 10/2017 | Dimino et al. | |
| 9,885,598 | B2 | 2/2018 | Tesar et al. | |

| | | | | |
|--------------|-----|---------|------------------------|--|
| D823,652 | S | 7/2018 | Dooley et al. | |
| 10,034,659 | B2 | 7/2018 | Siller Gonzalez et al. | |
| D842,985 | S | 3/2019 | Heckerman | |
| D862,999 | S | 10/2019 | Riedel et al. | |
| D871,137 | S | 12/2019 | Brouillac | |
| D873,995 | S * | 1/2020 | Laing D24/122 | |
| D876,183 | S | 2/2020 | Yee | |
| 10,578,196 | B2 | 3/2020 | Haremaki et al. | |
| D889,918 | S | 7/2020 | Hubert | |
| D893,947 | S | 8/2020 | Pulk | |
| D914,204 | S * | 3/2021 | Roberts D24/122 | |
| D919,798 | S * | 5/2021 | Laing D24/122 | |
| D920,502 | S * | 5/2021 | Laing D24/122 | |
| 11,029,239 | B2 | 6/2021 | Littley et al. | |
| D932,632 | S * | 10/2021 | Laing D24/186 | |
| D932,633 | S * | 10/2021 | Laing D24/186 | |
| D932,648 | S * | 10/2021 | Laing D24/216 | |
| D933,238 | S * | 10/2021 | Laing D24/186 | |
| D933,239 | S * | 10/2021 | Laing D24/186 | |
| D933,240 | S * | 10/2021 | Laing D24/186 | |
| D933,241 | S * | 10/2021 | Liang D24/186 | |
| 2005/0261605 | A1 | 11/2005 | Shemer et al. | |
| 2008/0312556 | A1 | 12/2008 | Dijkman | |
| 2008/0312557 | A1 | 12/2008 | Cho et al. | |
| 2011/0000309 | A1 | 1/2011 | Griffiths et al. | |
| 2012/0109008 | A1 | 5/2012 | Charlez et al. | |
| 2016/0029942 | A1 | 2/2016 | Paulsen et al. | |
| 2016/0051176 | A1 | 2/2016 | Ramos et al. | |
| 2017/0020433 | A1 | 1/2017 | Hotaling et al. | |
| 2017/0086728 | A1 | 3/2017 | Hidas | |
| 2017/0105670 | A1 | 4/2017 | Holt et al. | |
| 2017/0135622 | A1 | 5/2017 | Shimokawa et al. | |
| 2017/0307423 | A1 | 10/2017 | Pahwa et al. | |
| 2018/0085008 | A1 | 3/2018 | Hall et al. | |
| 2018/0303465 | A1 | 10/2018 | Lyon et al. | |
| 2019/0039201 | A1 | 2/2019 | Müller | |
| 2019/0365306 | A1 | 12/2019 | Laing et al. | |
| 2019/0365307 | A1 | 12/2019 | Laing et al. | |
| 2019/0365308 | A1 | 12/2019 | Laing et al. | |
| 2020/0209044 | A1 | 7/2020 | Holt et al. | |
| 2020/0268303 | A1 | 8/2020 | Oliva | |

FOREIGN PATENT DOCUMENTS

| | | | |
|----|----------------|----|---------|
| CN | 106037766 | A | 10/2016 |
| DE | 3007855 | A1 | 9/1981 |
| DE | 19733630 | A1 | 2/1999 |
| DE | 102014008760 | A1 | 1/2015 |
| EM | 005840378-0001 | | 3/2019 |
| EM | 005840378-0002 | | 3/2019 |
| EM | 005840378-0003 | | 3/2019 |
| EM | 006821633-001 | | 10/2019 |
| EM | 006821633-0002 | | 10/2019 |
| EM | 006821633-0003 | | 10/2019 |
| EM | 006821633-0004 | | 10/2019 |
| EP | 2303124 | B1 | 8/2012 |
| EP | 2741671 | B1 | 1/2016 |
| EP | 2716219 | B1 | 3/2017 |
| EP | 2564778 | B1 | 4/2018 |
| JP | 3729732 | B2 | 10/2005 |
| KR | 20110030826 | A | 3/2011 |
| RU | 2034516 | C1 | 5/1995 |
| RU | 2071724 | C1 | 1/1997 |
| RU | 2643110 | C1 | 1/2018 |
| WO | 9925246 | A1 | 5/1999 |
| WO | 2009035599 | A1 | 3/2009 |
| WO | 2009142508 | A1 | 11/2009 |
| WO | 2014141234 | A1 | 9/2014 |
| WO | 2016056571 | A1 | 4/2016 |
| WO | 2017036952 | A1 | 3/2017 |
| WO | 2017149272 | A1 | 9/2017 |
| WO | 2018036664 | A1 | 3/2018 |
| WO | 2018051244 | A1 | 3/2018 |

OTHER PUBLICATIONS

Specimen Collection Unit. "Specimen Collection Unit, QTY of 1." obtained Nov. 12, 2018 from <<https://www.amazon.com/Specimen->

(56)

References Cited

OTHER PUBLICATIONS

Collection-Unit-QTY-1/dp/B002ZUCVP0#feature-bullets-btf>, 6 pages.

Bestmedical. "Uroflowmeter: Portable & wireless." obtained Nov. 12, 2018 from <<http://www.best-medical.nl/uroflowmeter/>>, 6 pages.

MDTI. "Uflow meter Male Urine Peak Flow Device." obtained Nov. 12, 2018 from <<https://www.mdti.co.uk/uflow->>, 2 pages.

Albyn Medical Product Detail. "SmartFlow: SmartFlow brings together high specifications and ease-of-use." Obtained Nov. 12, 2018 from <<http://www.albynmedical.com/products/ProductDetail.aspx?ID=8>>, 2 pages.

Laborie: "Uroflometry: Uroflowmeters designed for practical, every-day studies, available in a range of configurations to meet different demands." obtained Nov. 12, 2018 from <<https://www.laborie.com/category/urology-urogynecology/uroflowmetry/>>, 6 pages.

Minze Health. "Homeflow." obtained Nov. 12, 2018 from <<https://minzehealth.com/products/homeflow/>>, 8 pages.

Chun, Kwonsoo et al., "Noninvasive Medical Tools for Evaluating Voiding Pattern in Real Life." International Neurology Journal, 2017, S10-16.

Do It Yourself, "Urinal Repair: Troubleshoot Urinal Plumbing Problems", <https://web.archive.org/web/20171015111849/http://www.doityourself.com/urinal-repair-troubleshoot-urinal-plumbing-problems>; accessed on May 13, 2019, Oct. 15, 2017, 3 pages.

PCT, "International Search Report and Written Opinion", Application No. PCT/US2019/021292, dated May 8, 2019, 11 pages.

PCT, "International Search Report and Written Opinion", Application No. PCT/US19/21421, dated May 31, 2019, 16 pages.

* cited by examiner

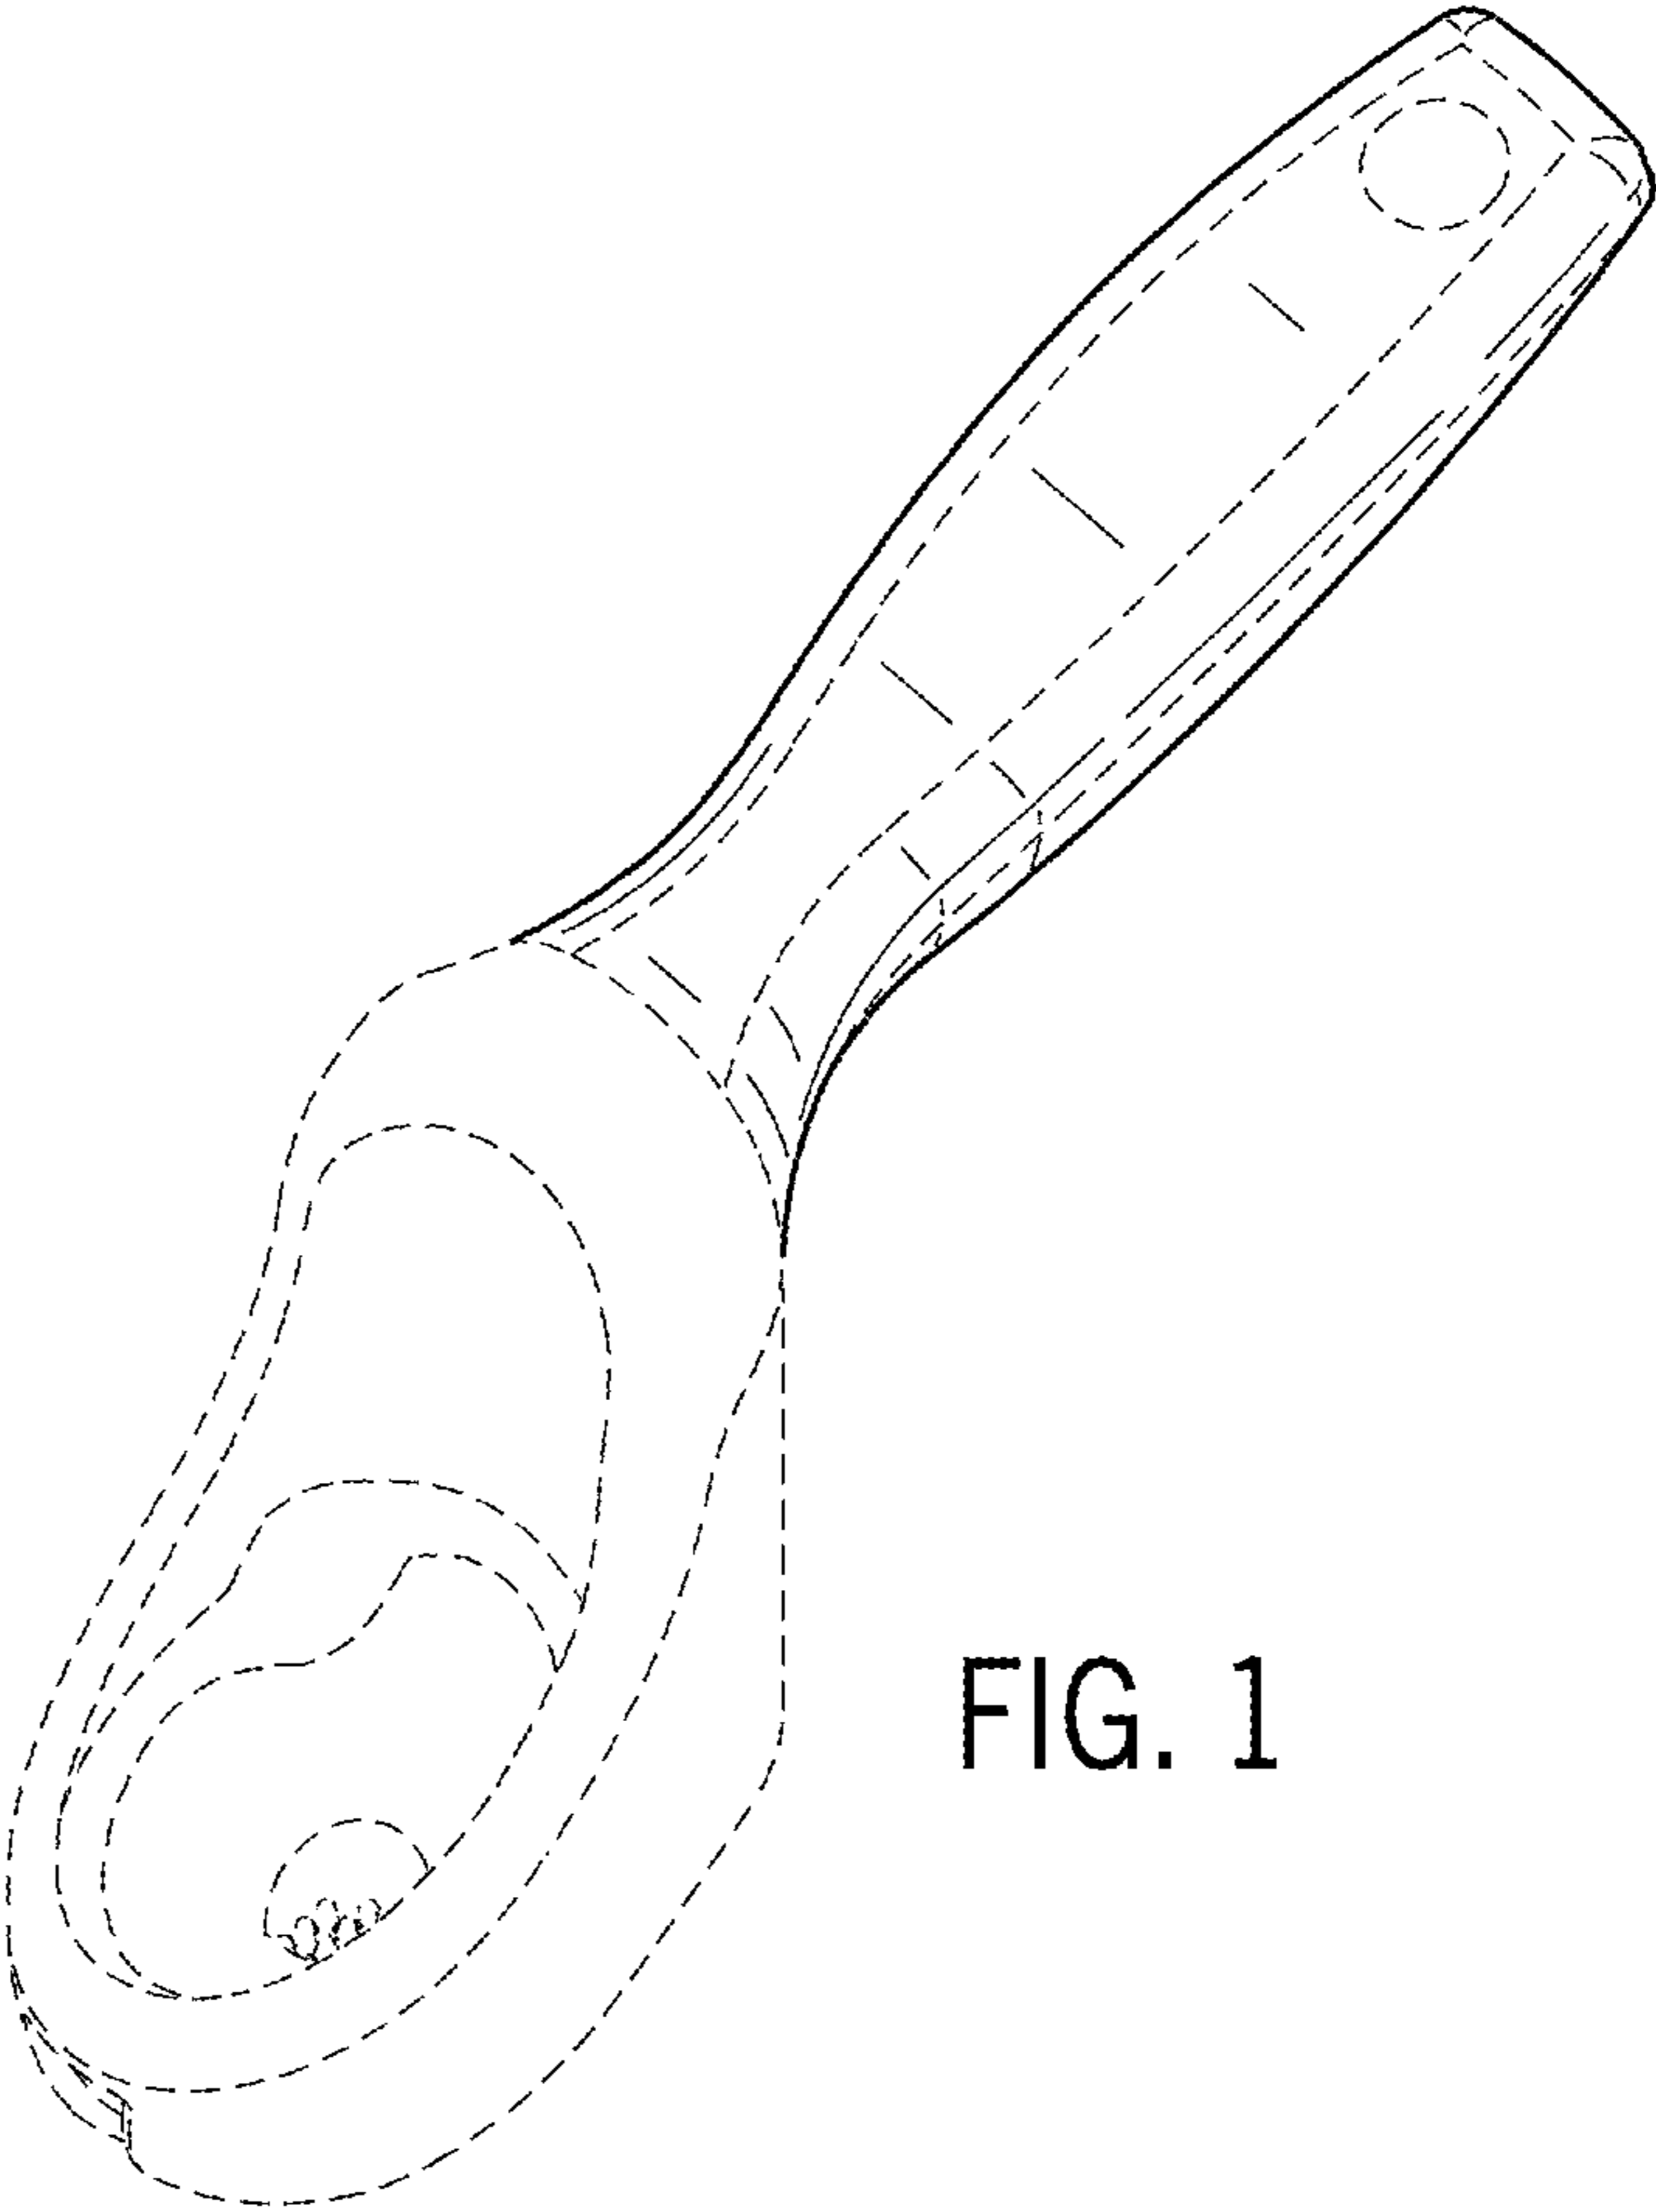


FIG. 1

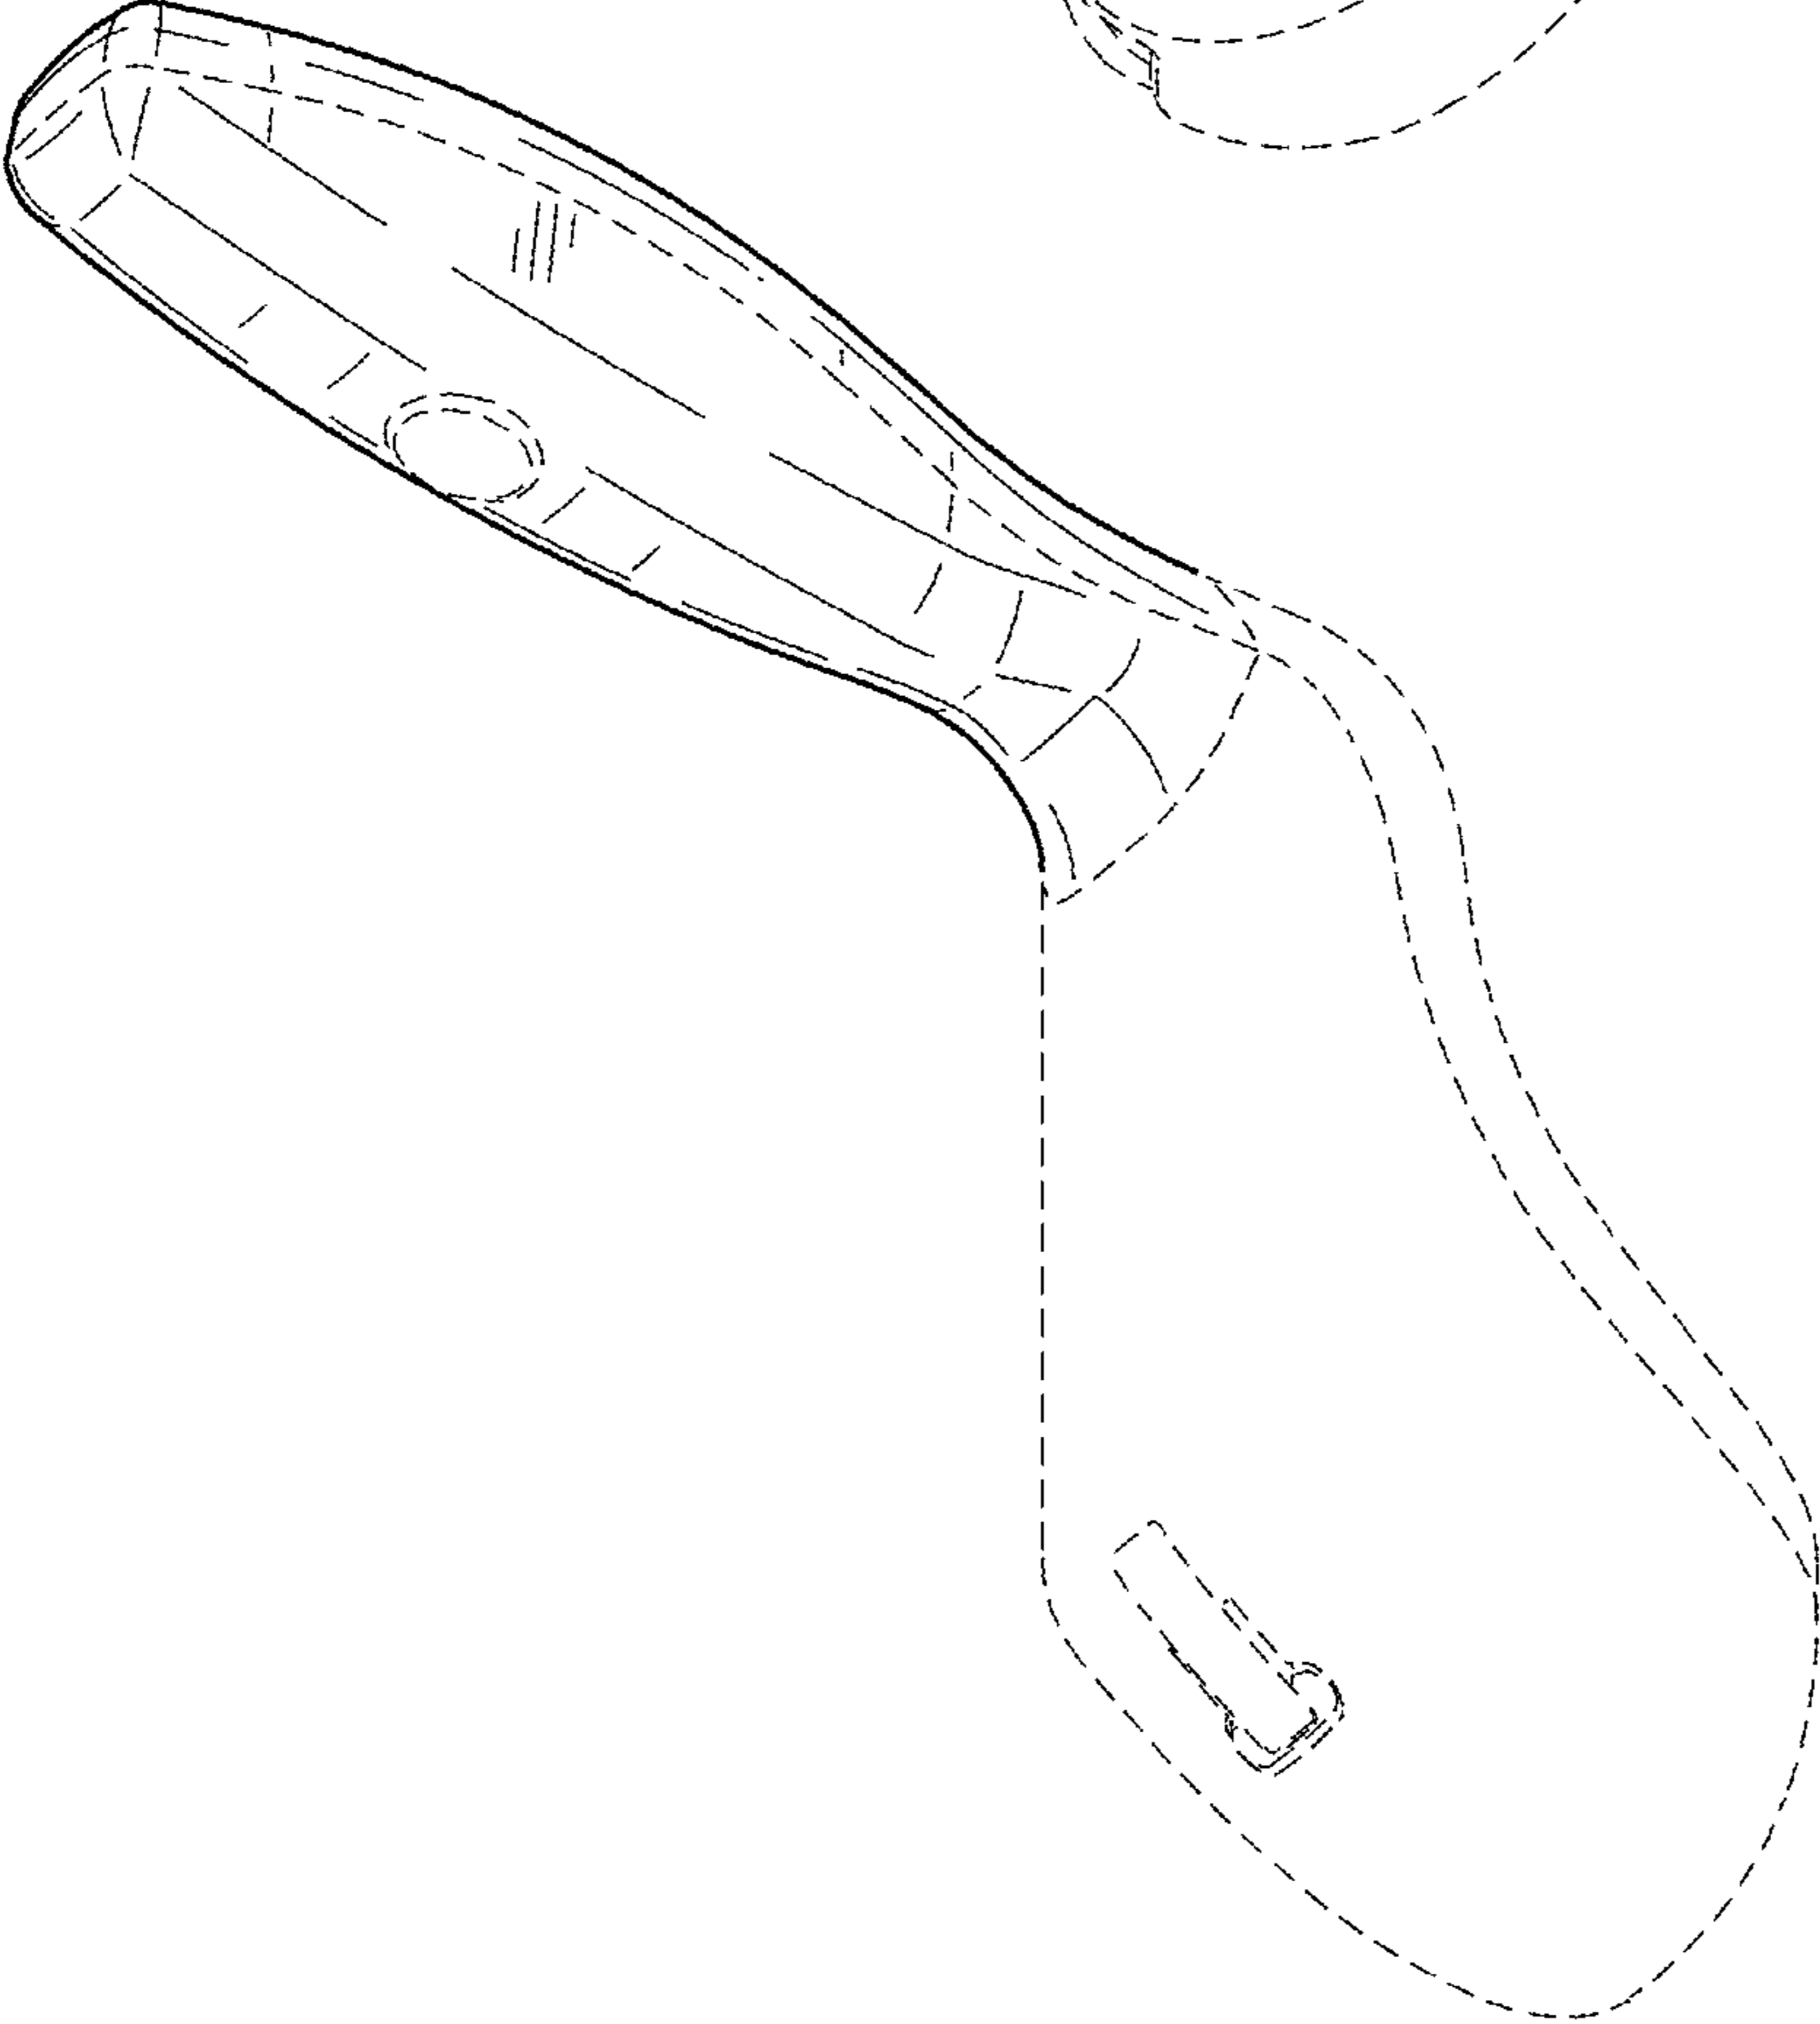


FIG. 2

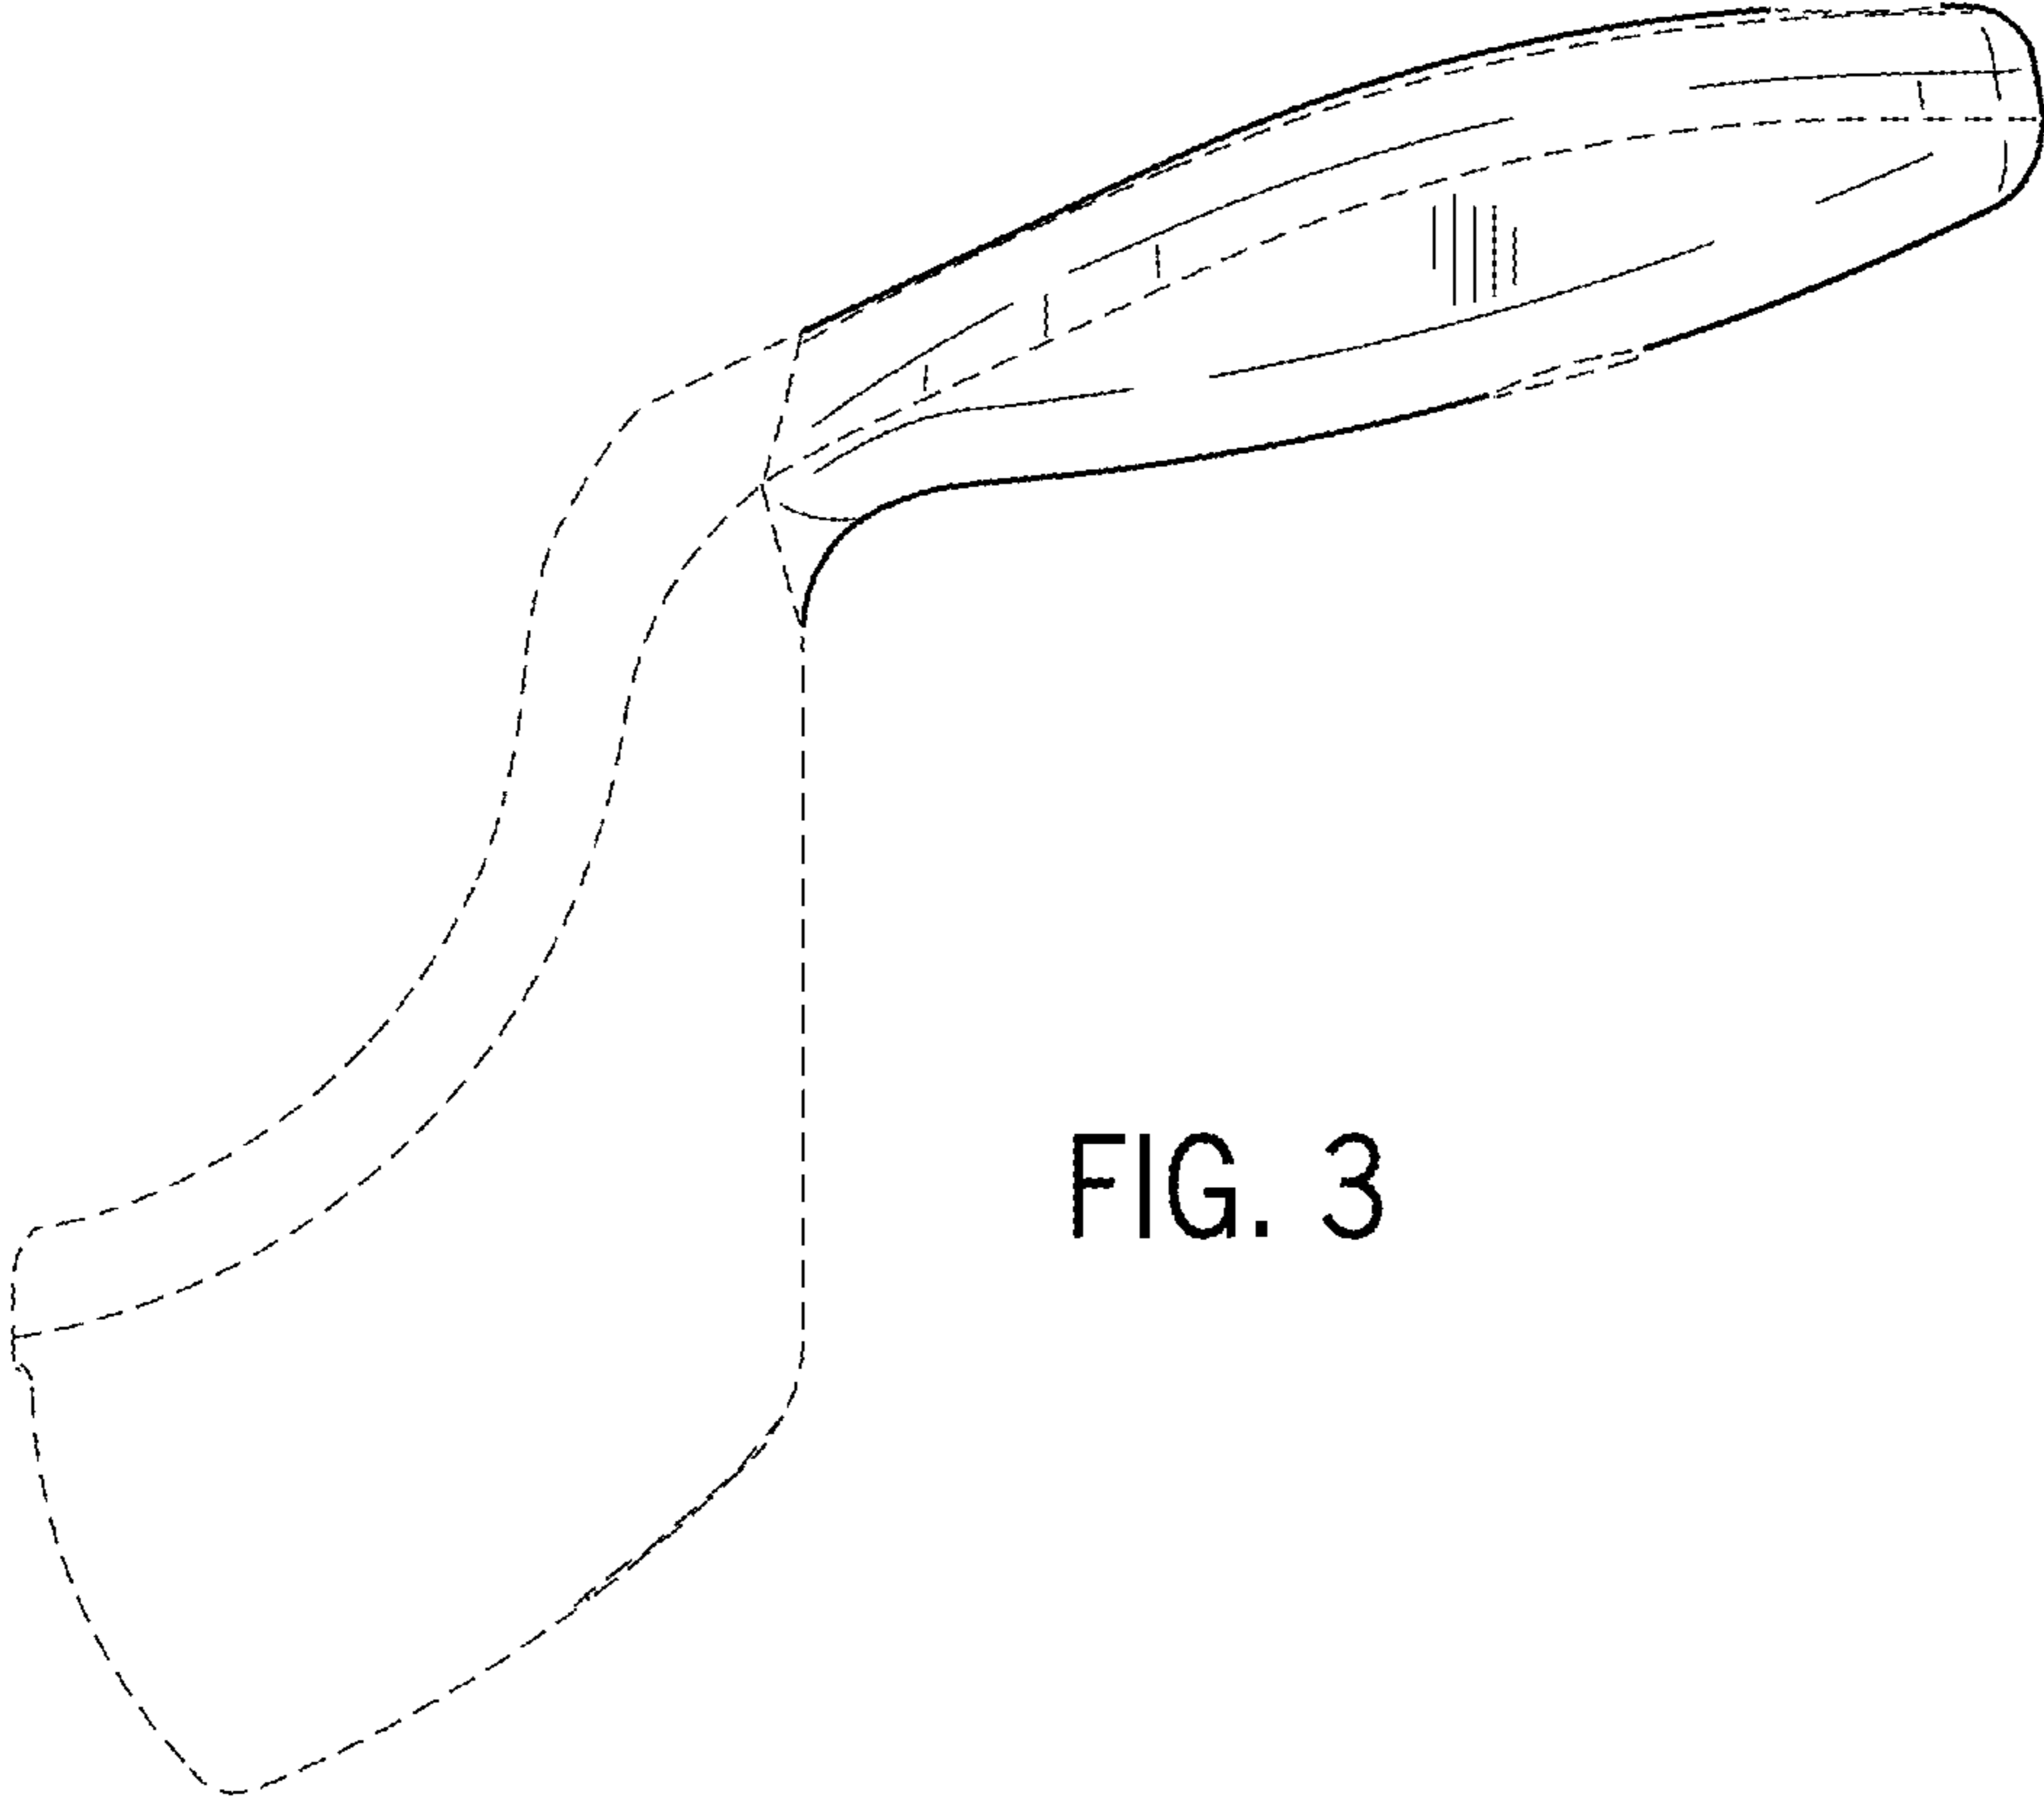


FIG. 3

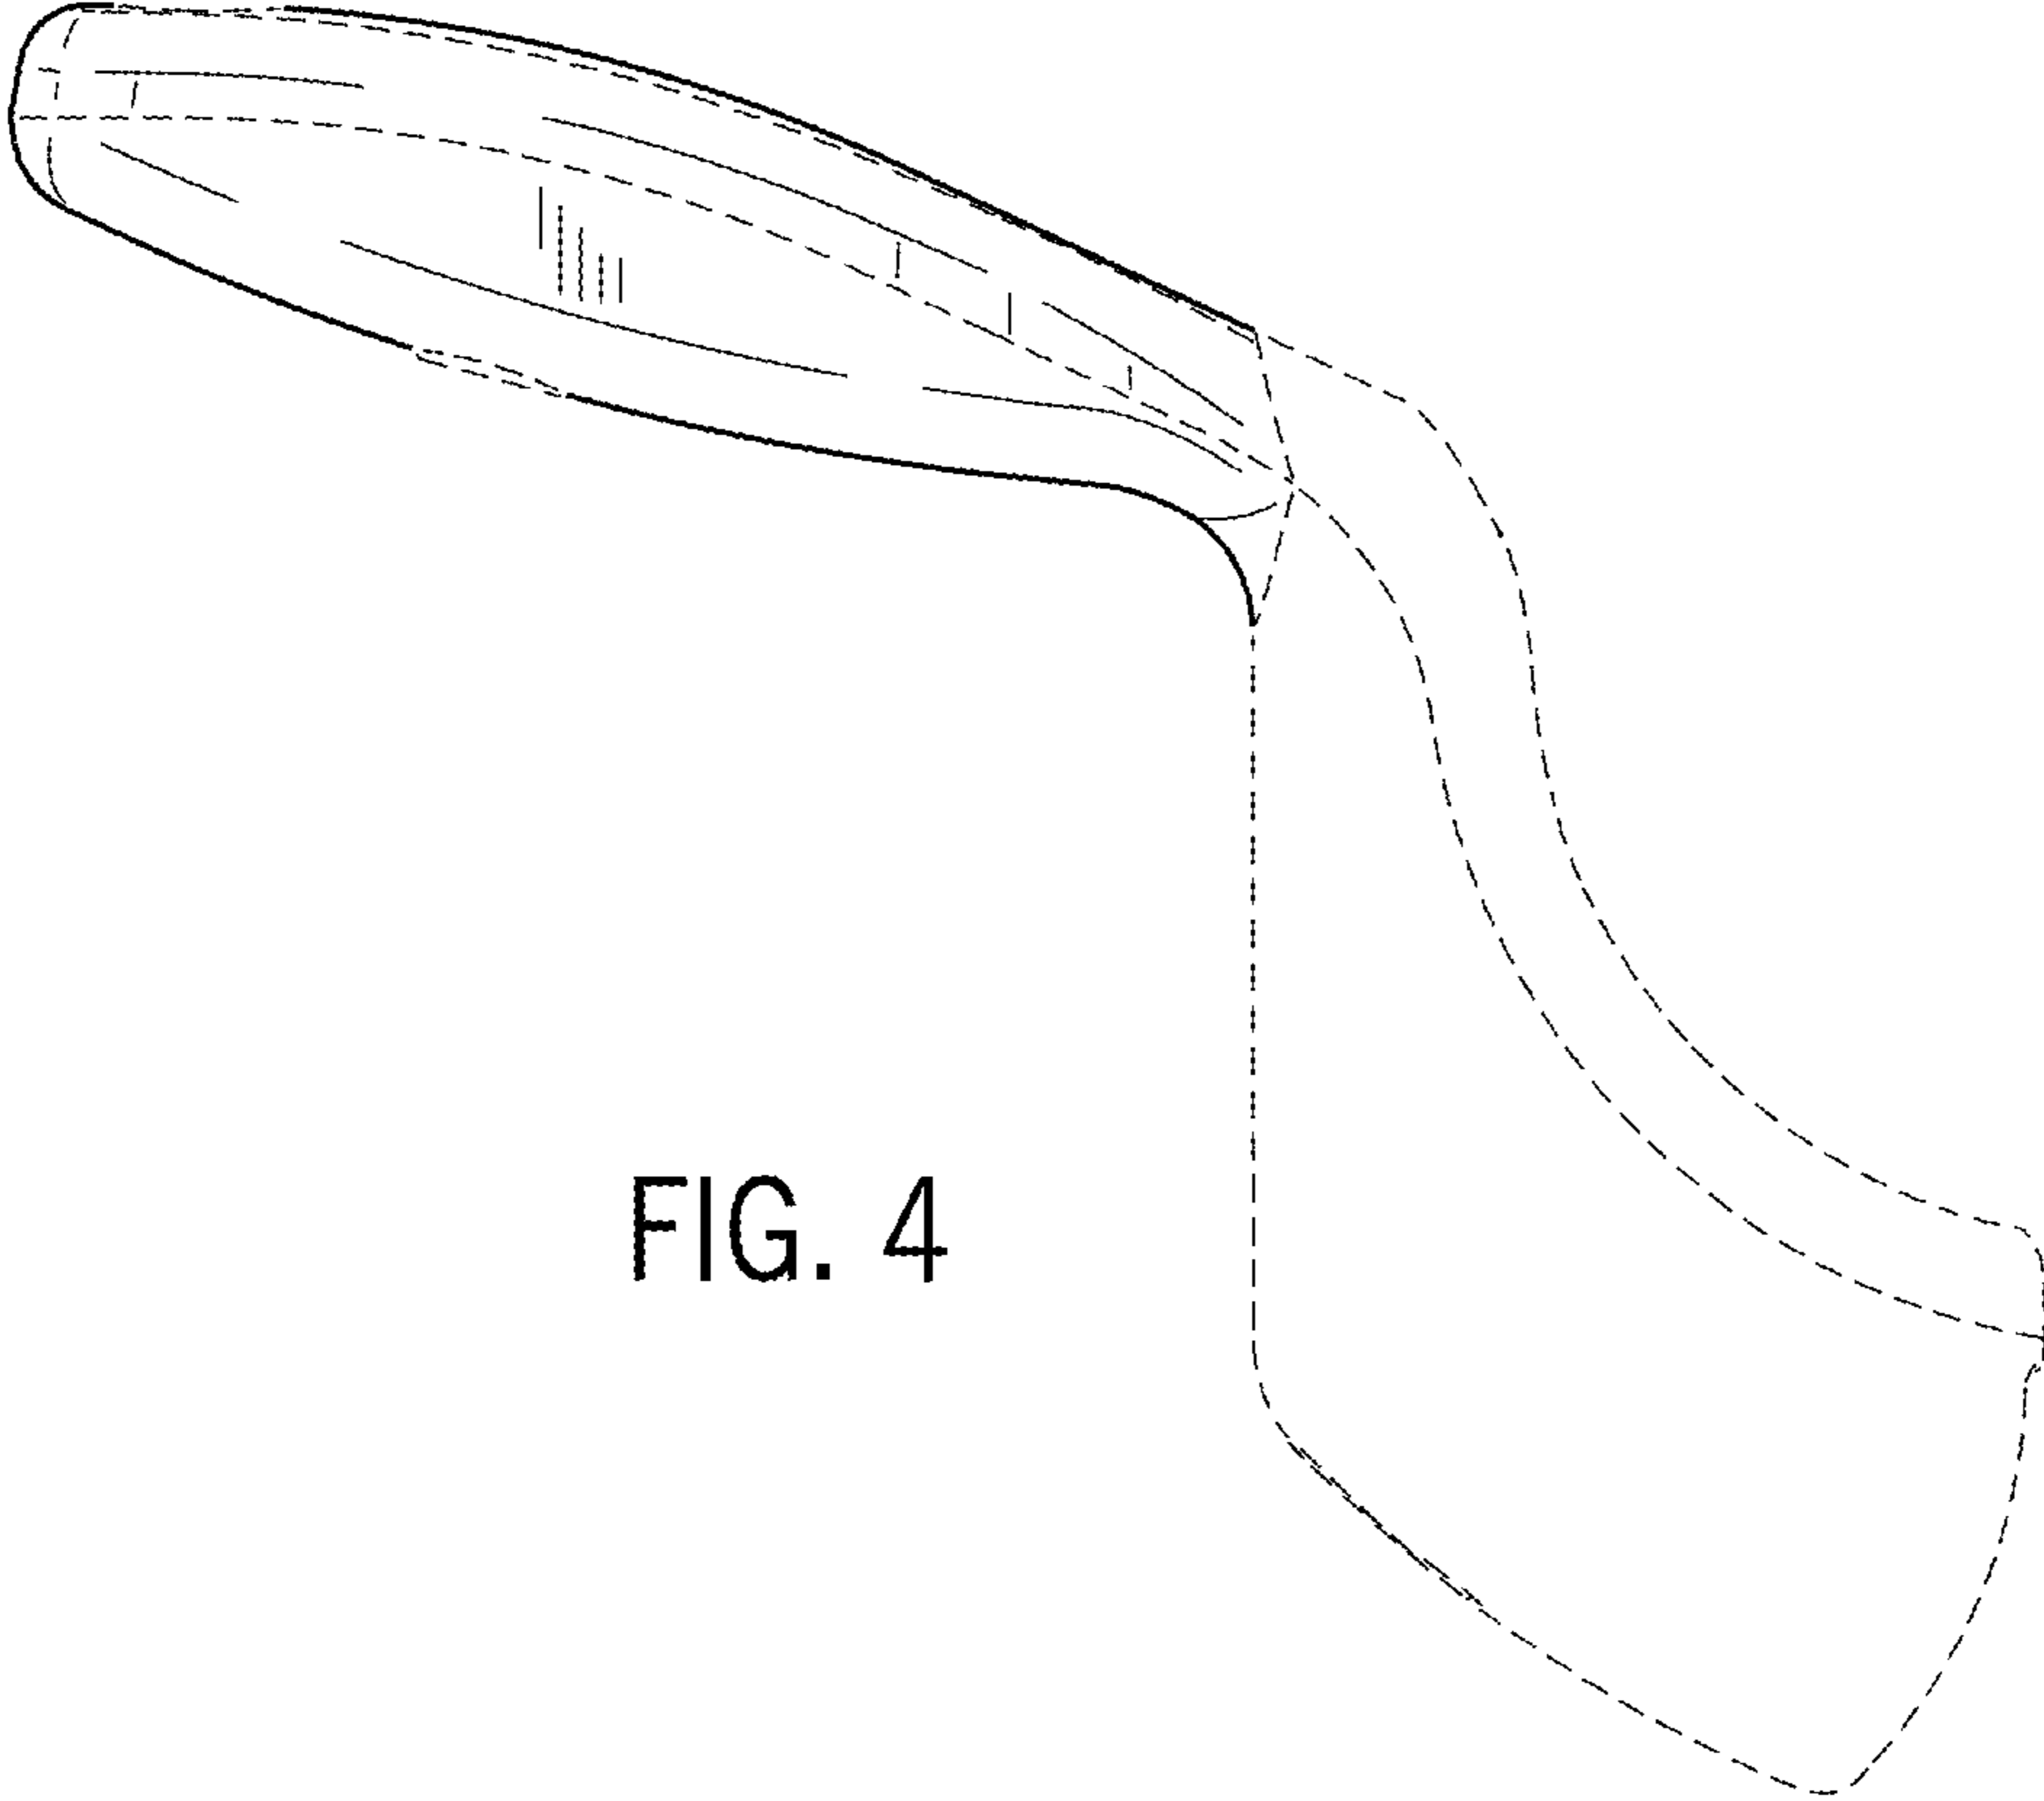


FIG. 4

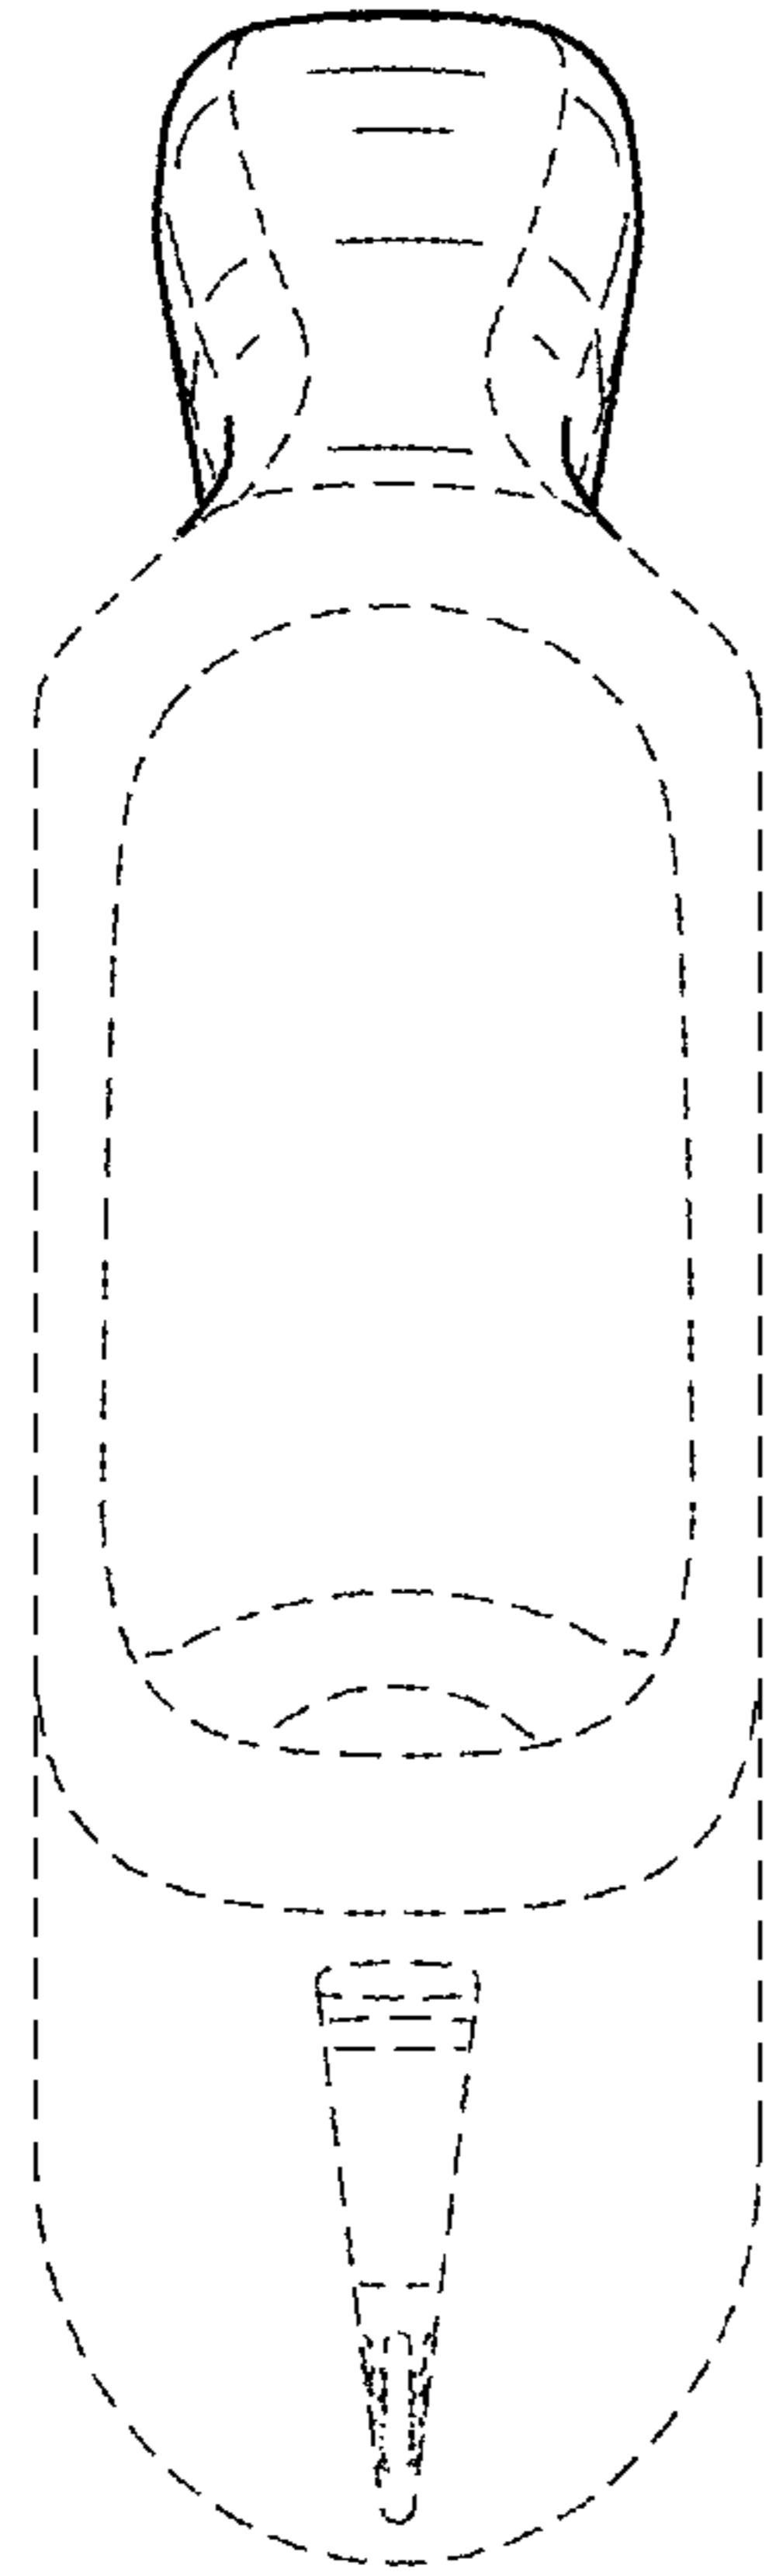


FIG. 5

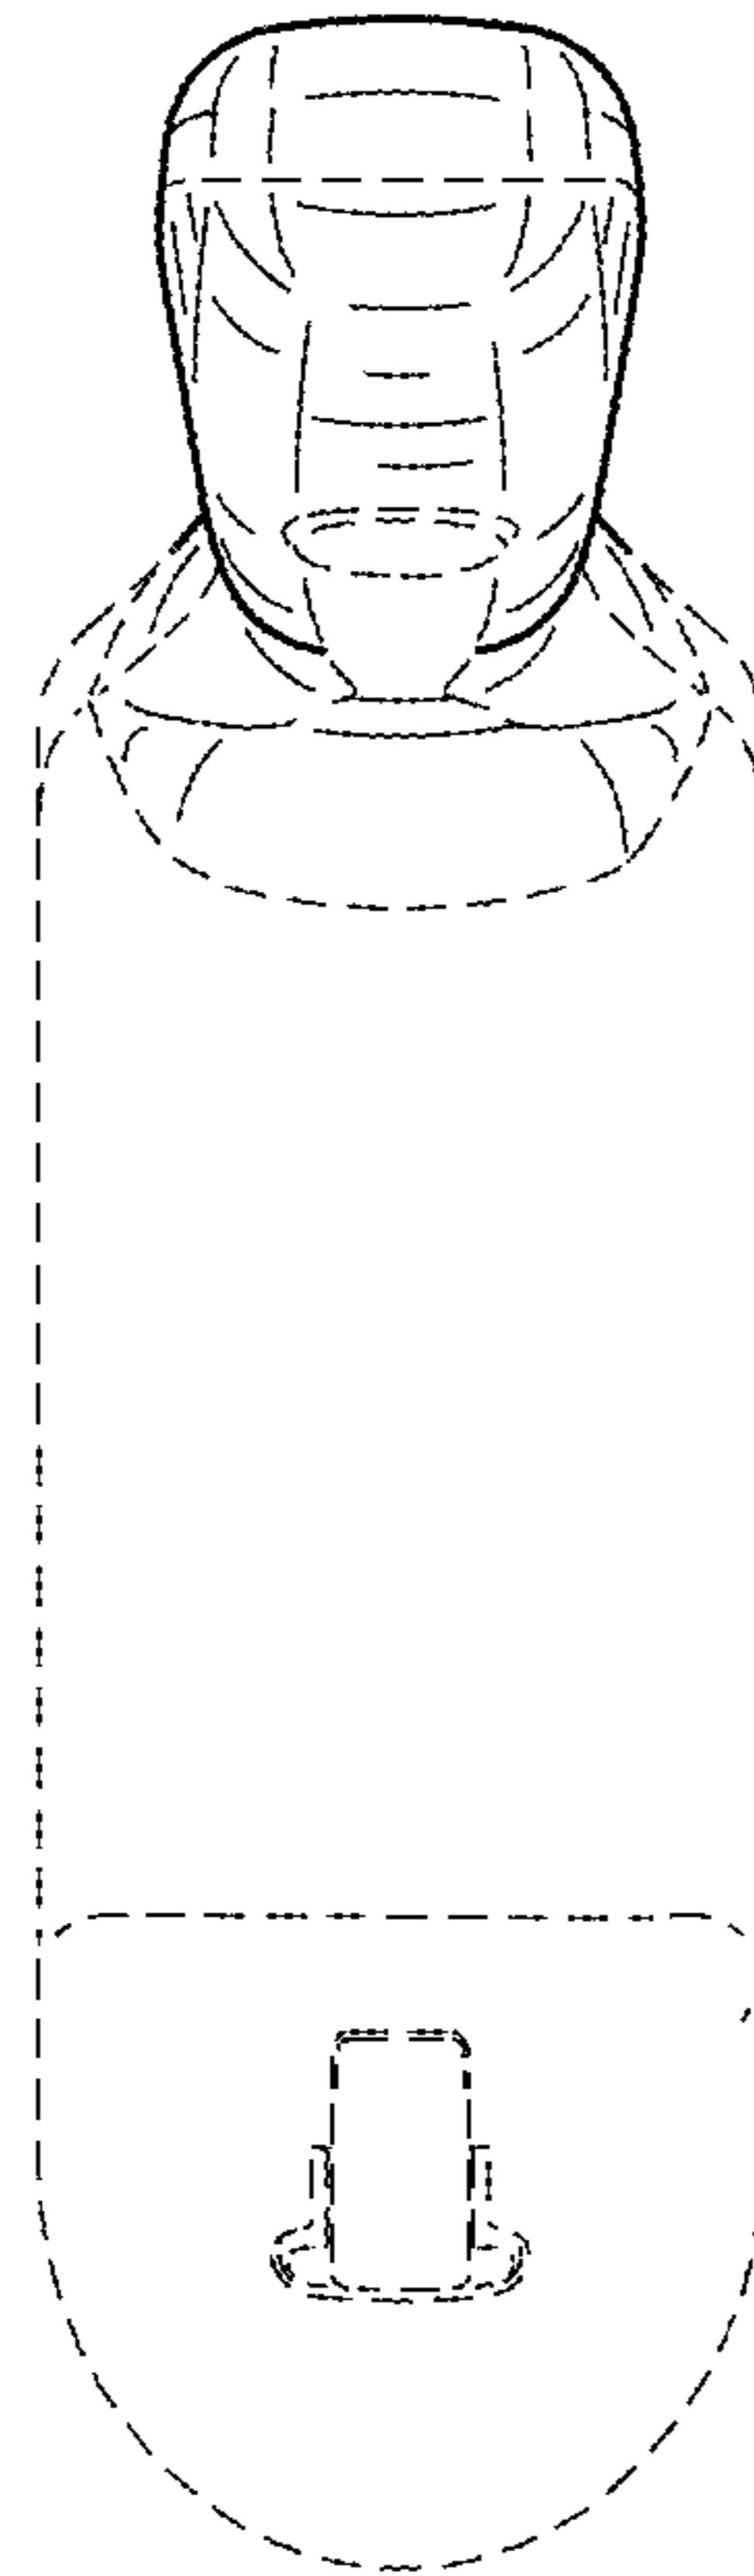


FIG. 6

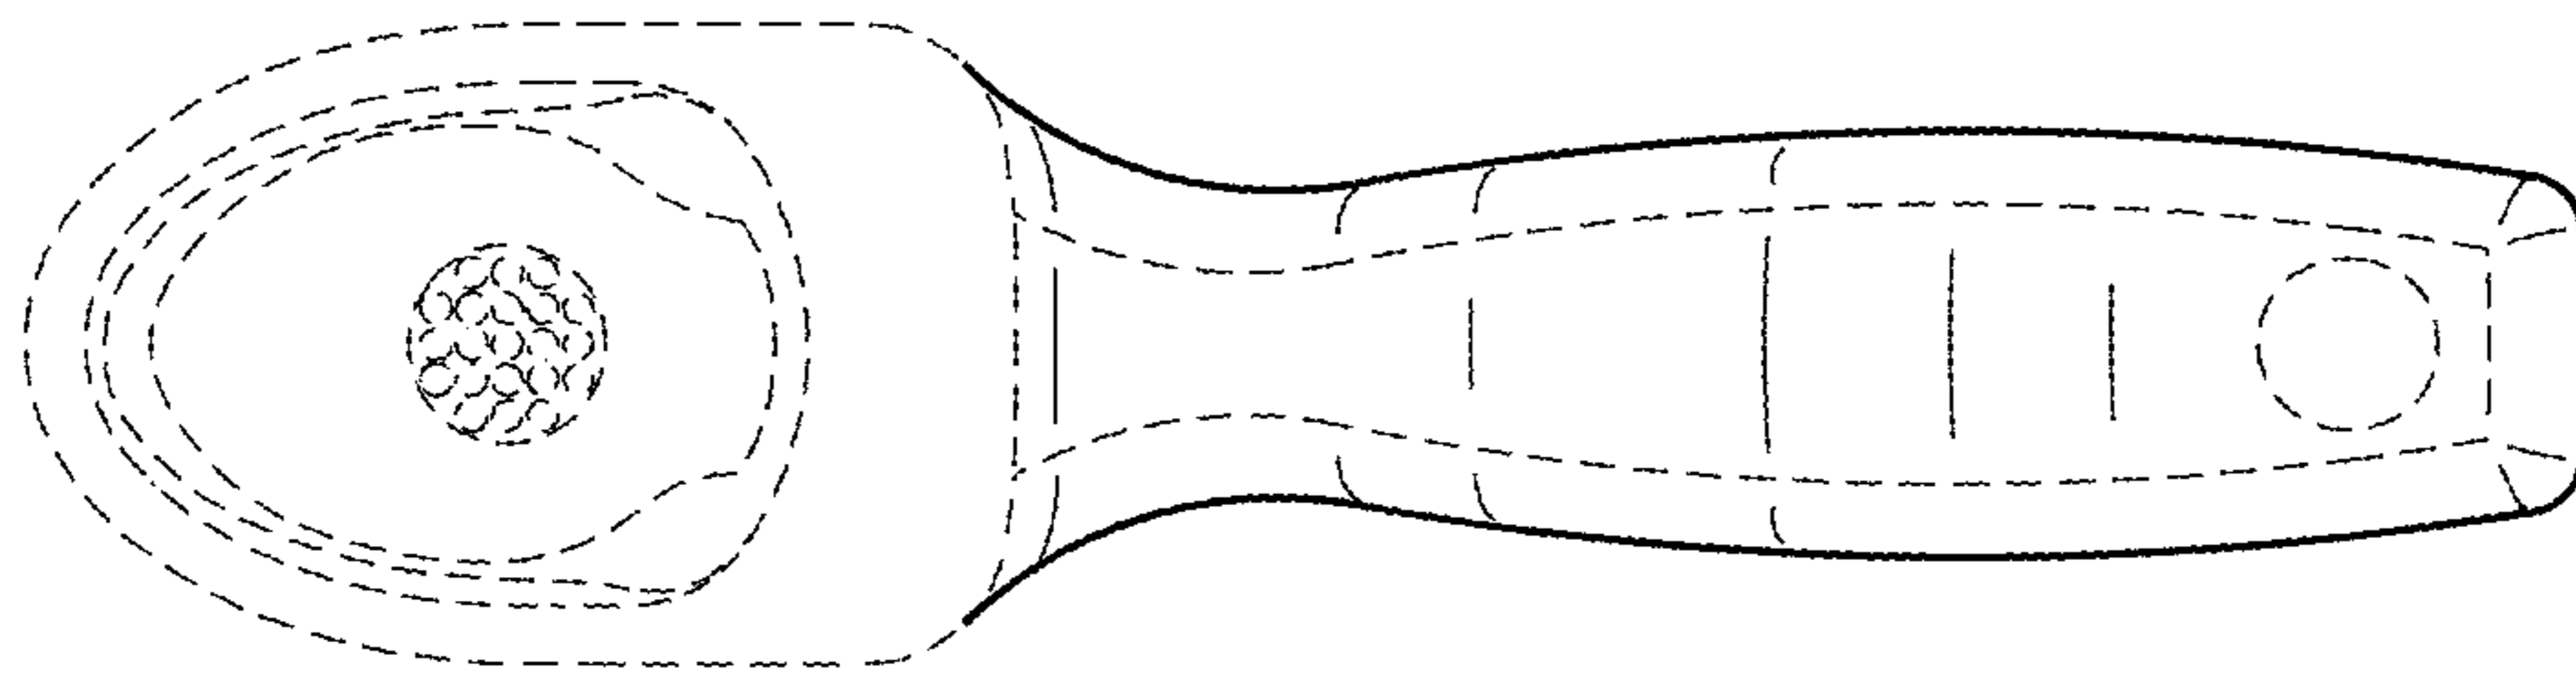


FIG. 7

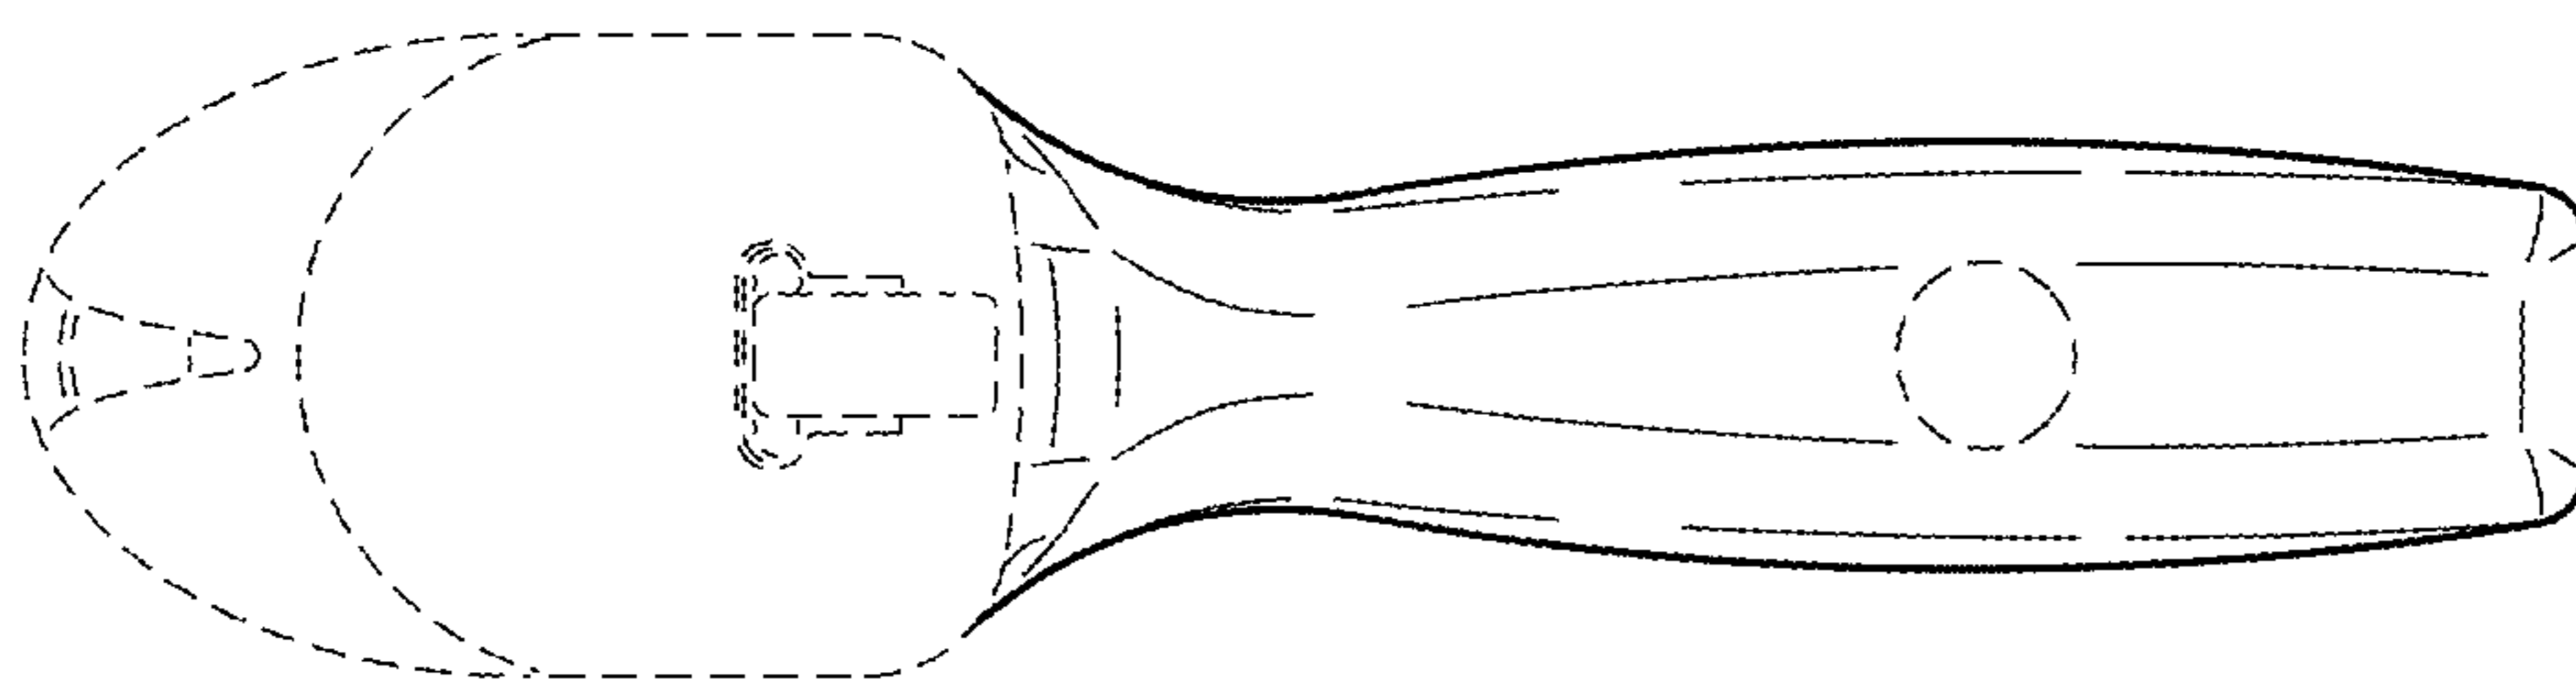


FIG. 8