

US00D978370S

(12) **United States Design Patent**
Gut et al.

(10) **Patent No.:** **US D978,370 S**

(45) **Date of Patent:** **** Feb. 14, 2023**

(54) **LABORATORY DIAGNOSIS APPARATUS**

(71) Applicant: **Roche Molecular Systems, Inc.**,
Pleasanton, CA (US)

(72) Inventors: **Raphael Gut**, Rotkreuz (CH); **Sofia E. Galbraith**, Rotkreuz (CH); **Tobias Nuesch**, Zurich (CH); **Christian Rogge**, Munich (DE)

(73) Assignee: **Roche Molecular Systems, Inc.**,
Pleasanton, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/762,428**

(22) Filed: **Dec. 16, 2020**

(30) **Foreign Application Priority Data**

Jun. 30, 2020 (EP) 008026132

(51) **LOC (14) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/107, 185, 186, 216, 219, 231–234;
D10/81
CPC G01N 2035/00306; G01N 2035/00326;
G01N 2035/00336; G01N 2030/027;
G01N 21/76

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D598,129 S * 8/2009 Tsukuda D24/234
D662,431 S * 6/2012 Kimura D10/81
D799,999 S * 10/2017 Barton D24/216
D802,156 S * 11/2017 Barton D24/216
D843,597 S * 3/2019 Kurz-Ottenwaelder D24/232
D887,296 S * 6/2020 Stone D24/216
D887,545 S * 6/2020 Heintze D24/107

D896,981 S * 9/2020 Gruen D24/232
D920,145 S * 5/2021 Livingston D24/216
2013/0288355 A1* 10/2013 DeWitte G01N 35/026
435/288.6
2017/0269114 A1* 9/2017 Bryant G01N 35/04
2017/0341873 A1* 11/2017 Vivet G01N 35/04

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Bose McKinney & Evans LLP

(57) **CLAIM**

The ornamental design for a laboratory diagnosis apparatus, as shown and described.

DESCRIPTION

A portion of the disclosure of this patent document contains material to which a claim for copyright and trademark is made. The copyright and trademark owner has no objection to the reproduction of the patent document or the patent disclosure, as it appears in the U.S. Patent Office records, but reserves all other copyright and trademark rights whatsoever.

FIG. 1 is a front view of a laboratory diagnosis apparatus. FIG. 2 is a back view of the laboratory diagnosis apparatus of FIG. 1.

FIG. 3 is a side view of the laboratory diagnosis apparatus of FIG. 1.

FIG. 4 is a side view of the laboratory diagnosis apparatus of FIG. 1.


FIG. 5 is a top view of the laboratory diagnosis apparatus of FIG. 1.

FIG. 6 is a bottom view of the laboratory diagnosis apparatus of FIG. 1; and,

FIG. 7 is a perspective view of the laboratory diagnosis apparatus of FIG. 1.

The broken lines illustrate portions of the laboratory diagnosis apparatus that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

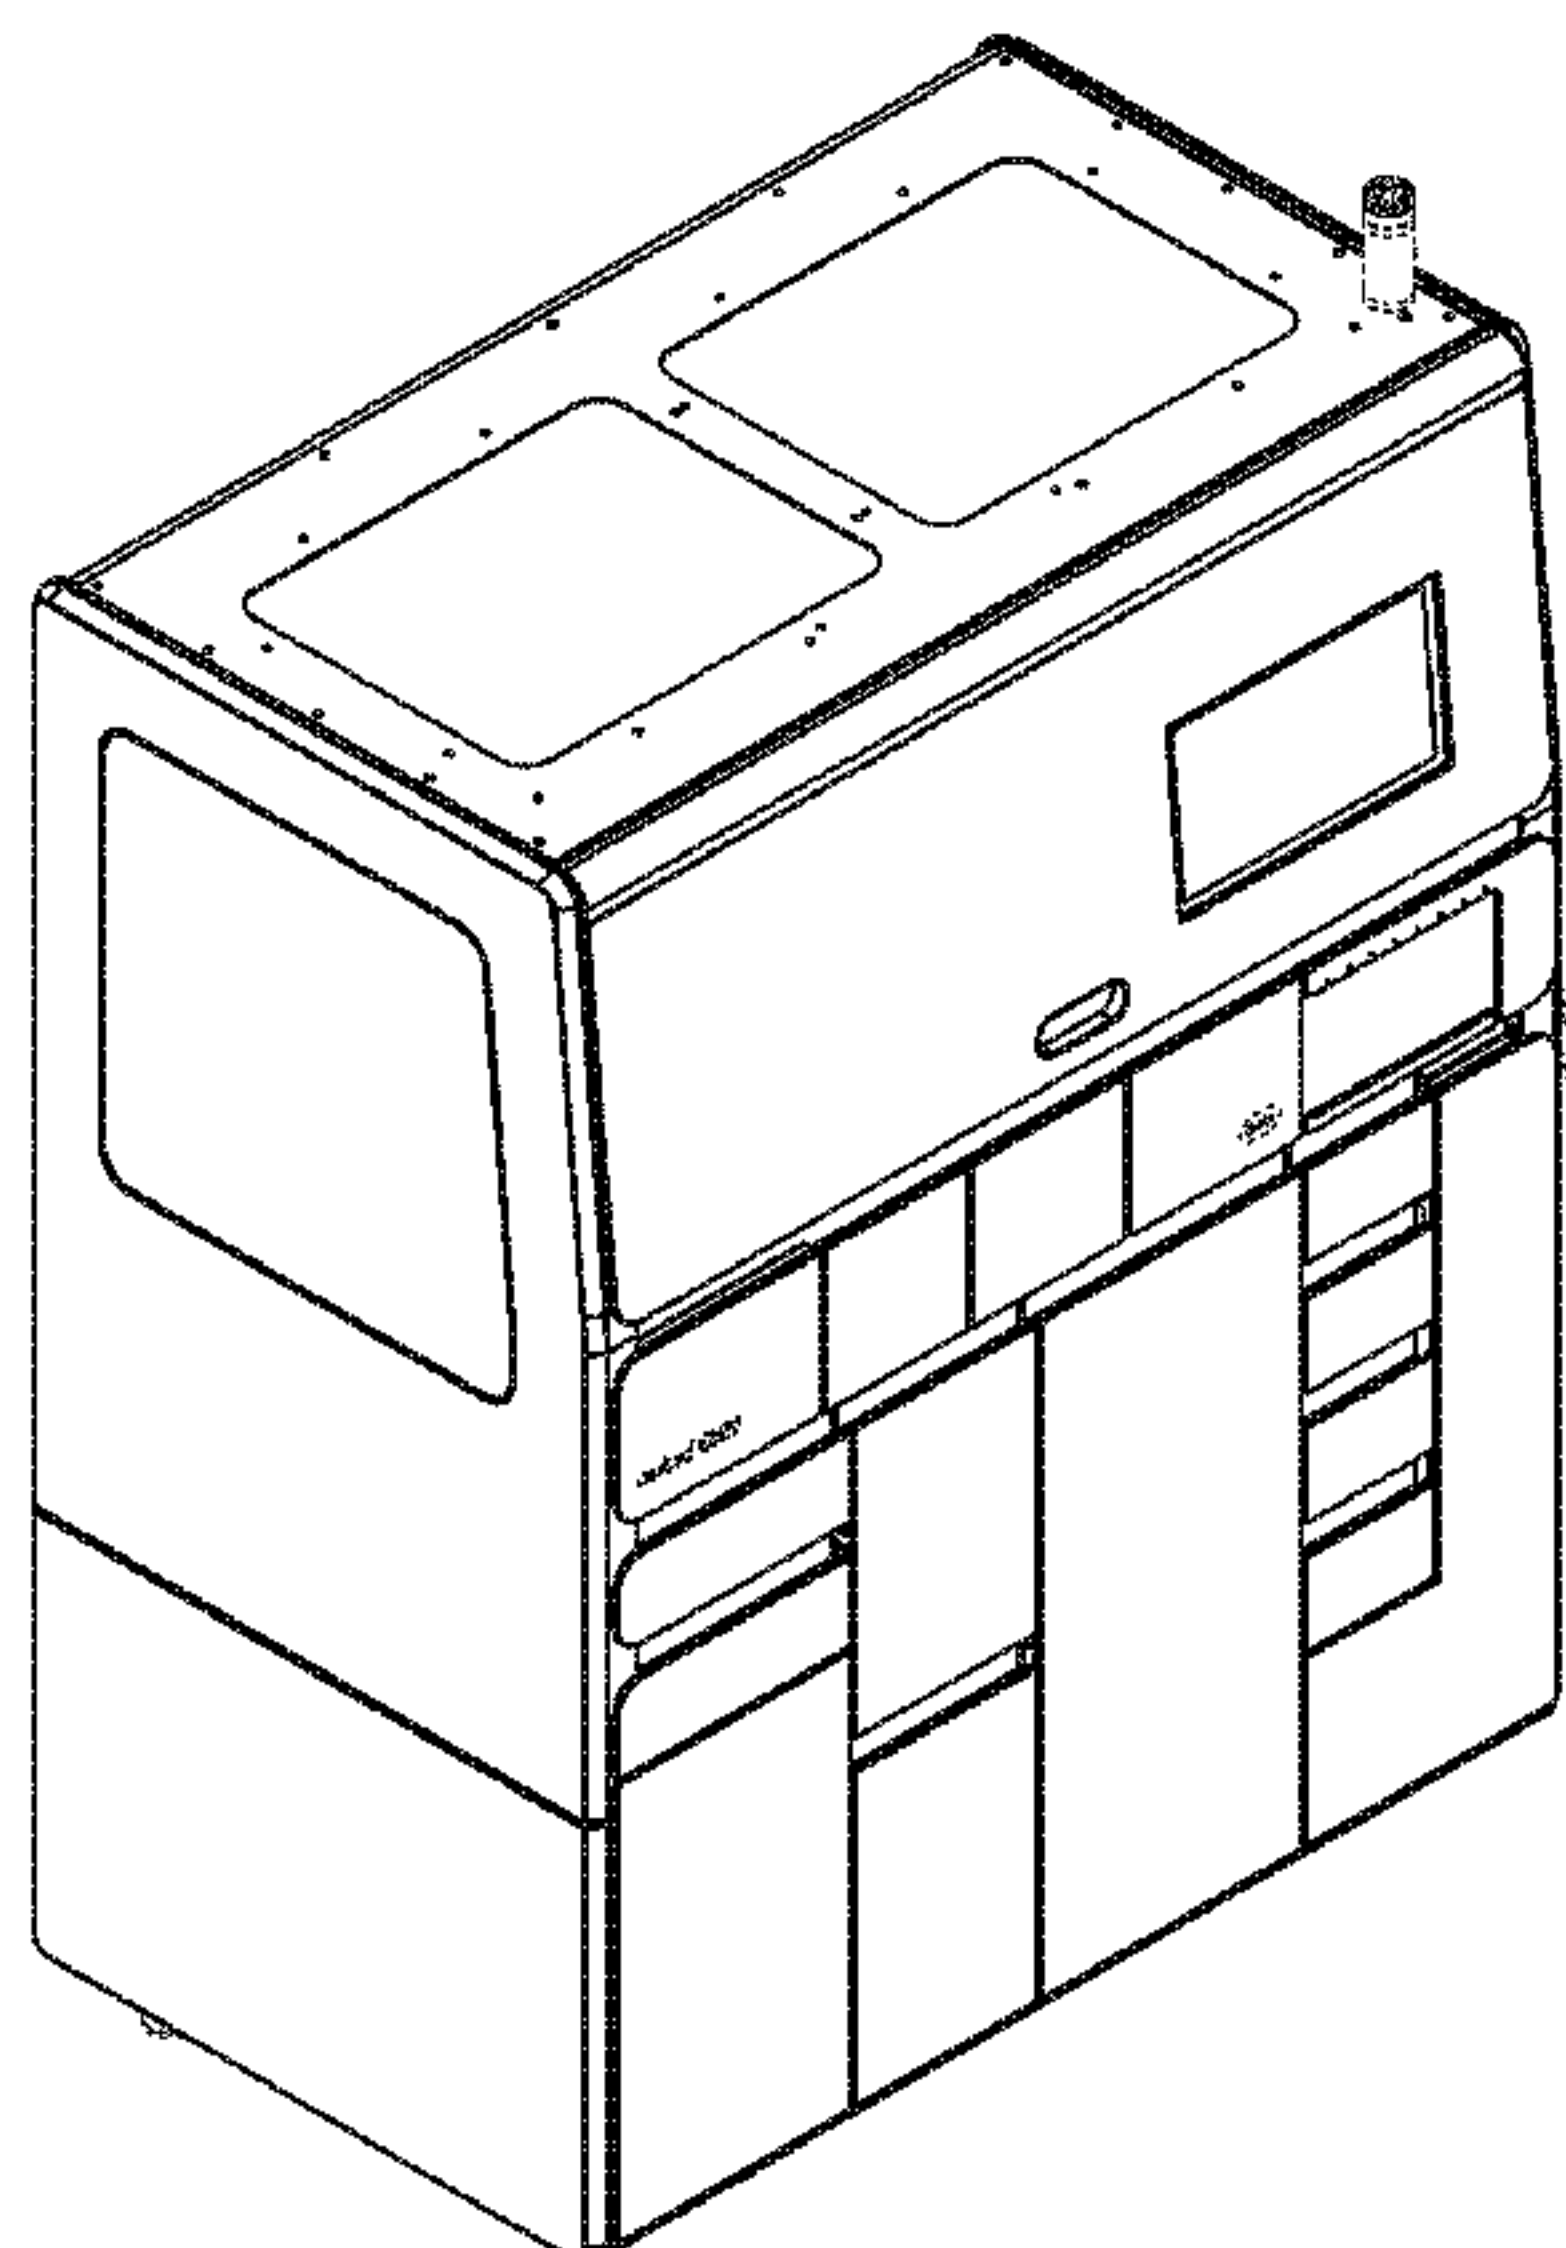

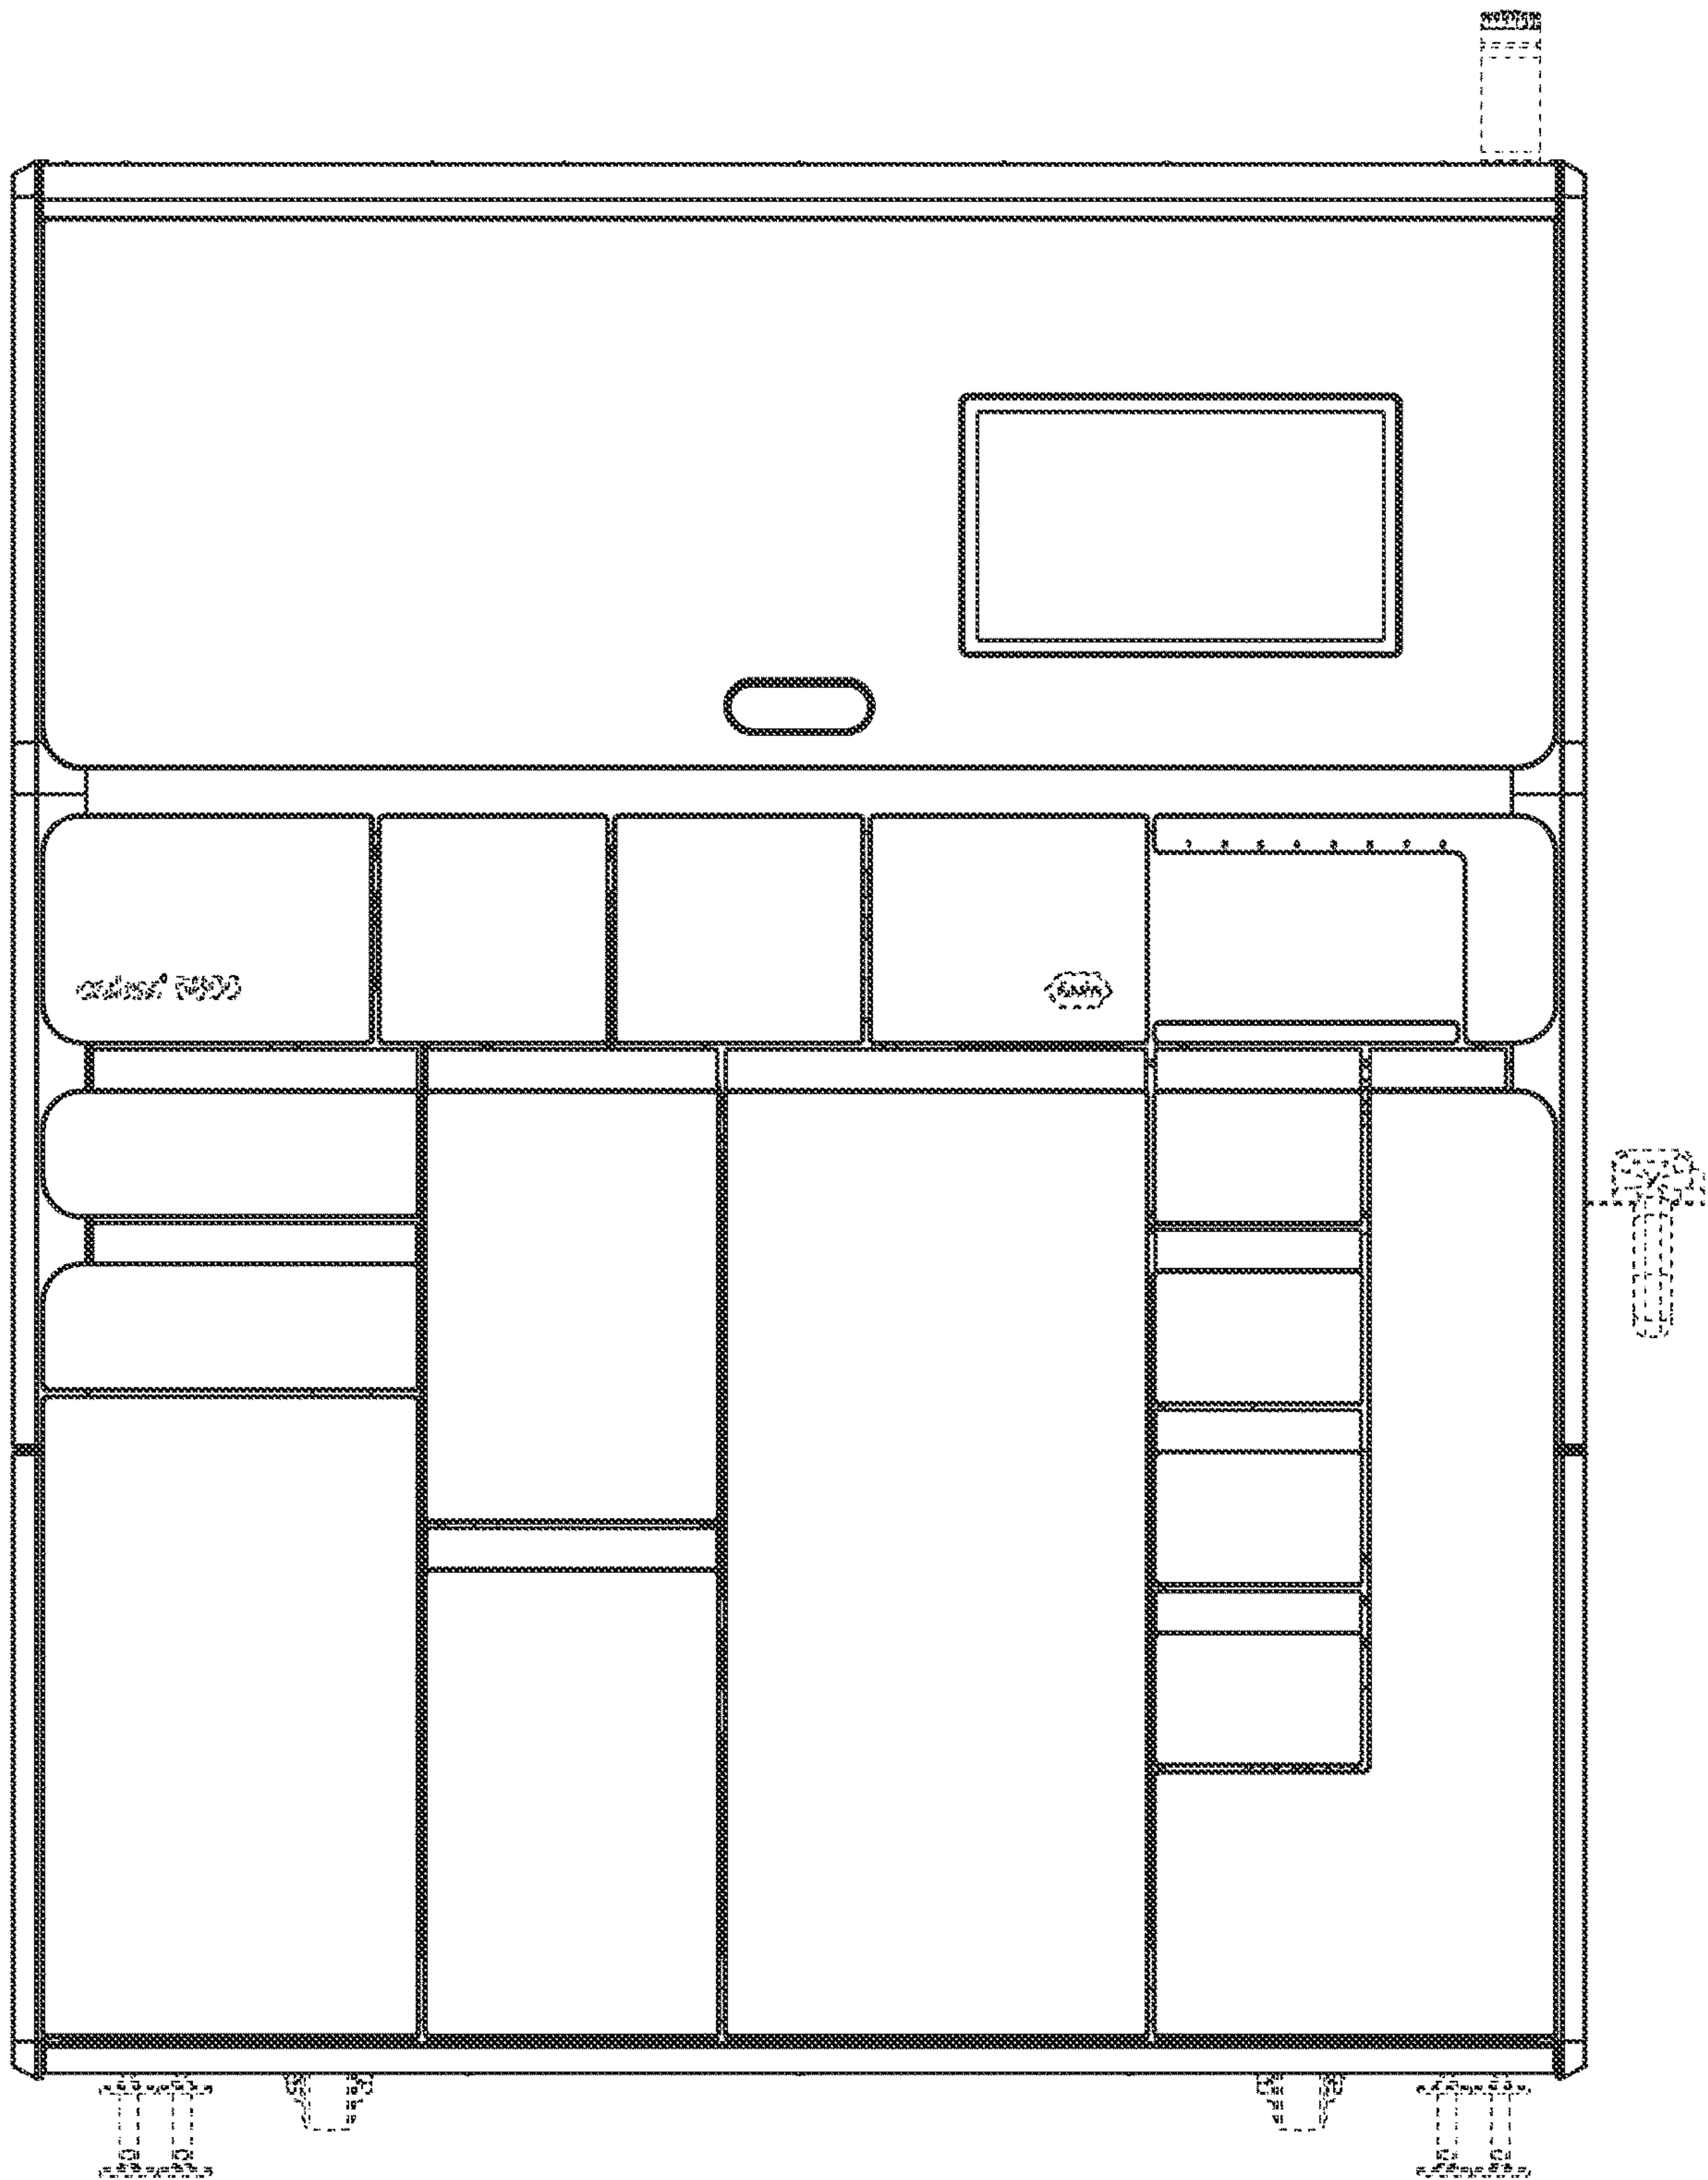


Fig. 1

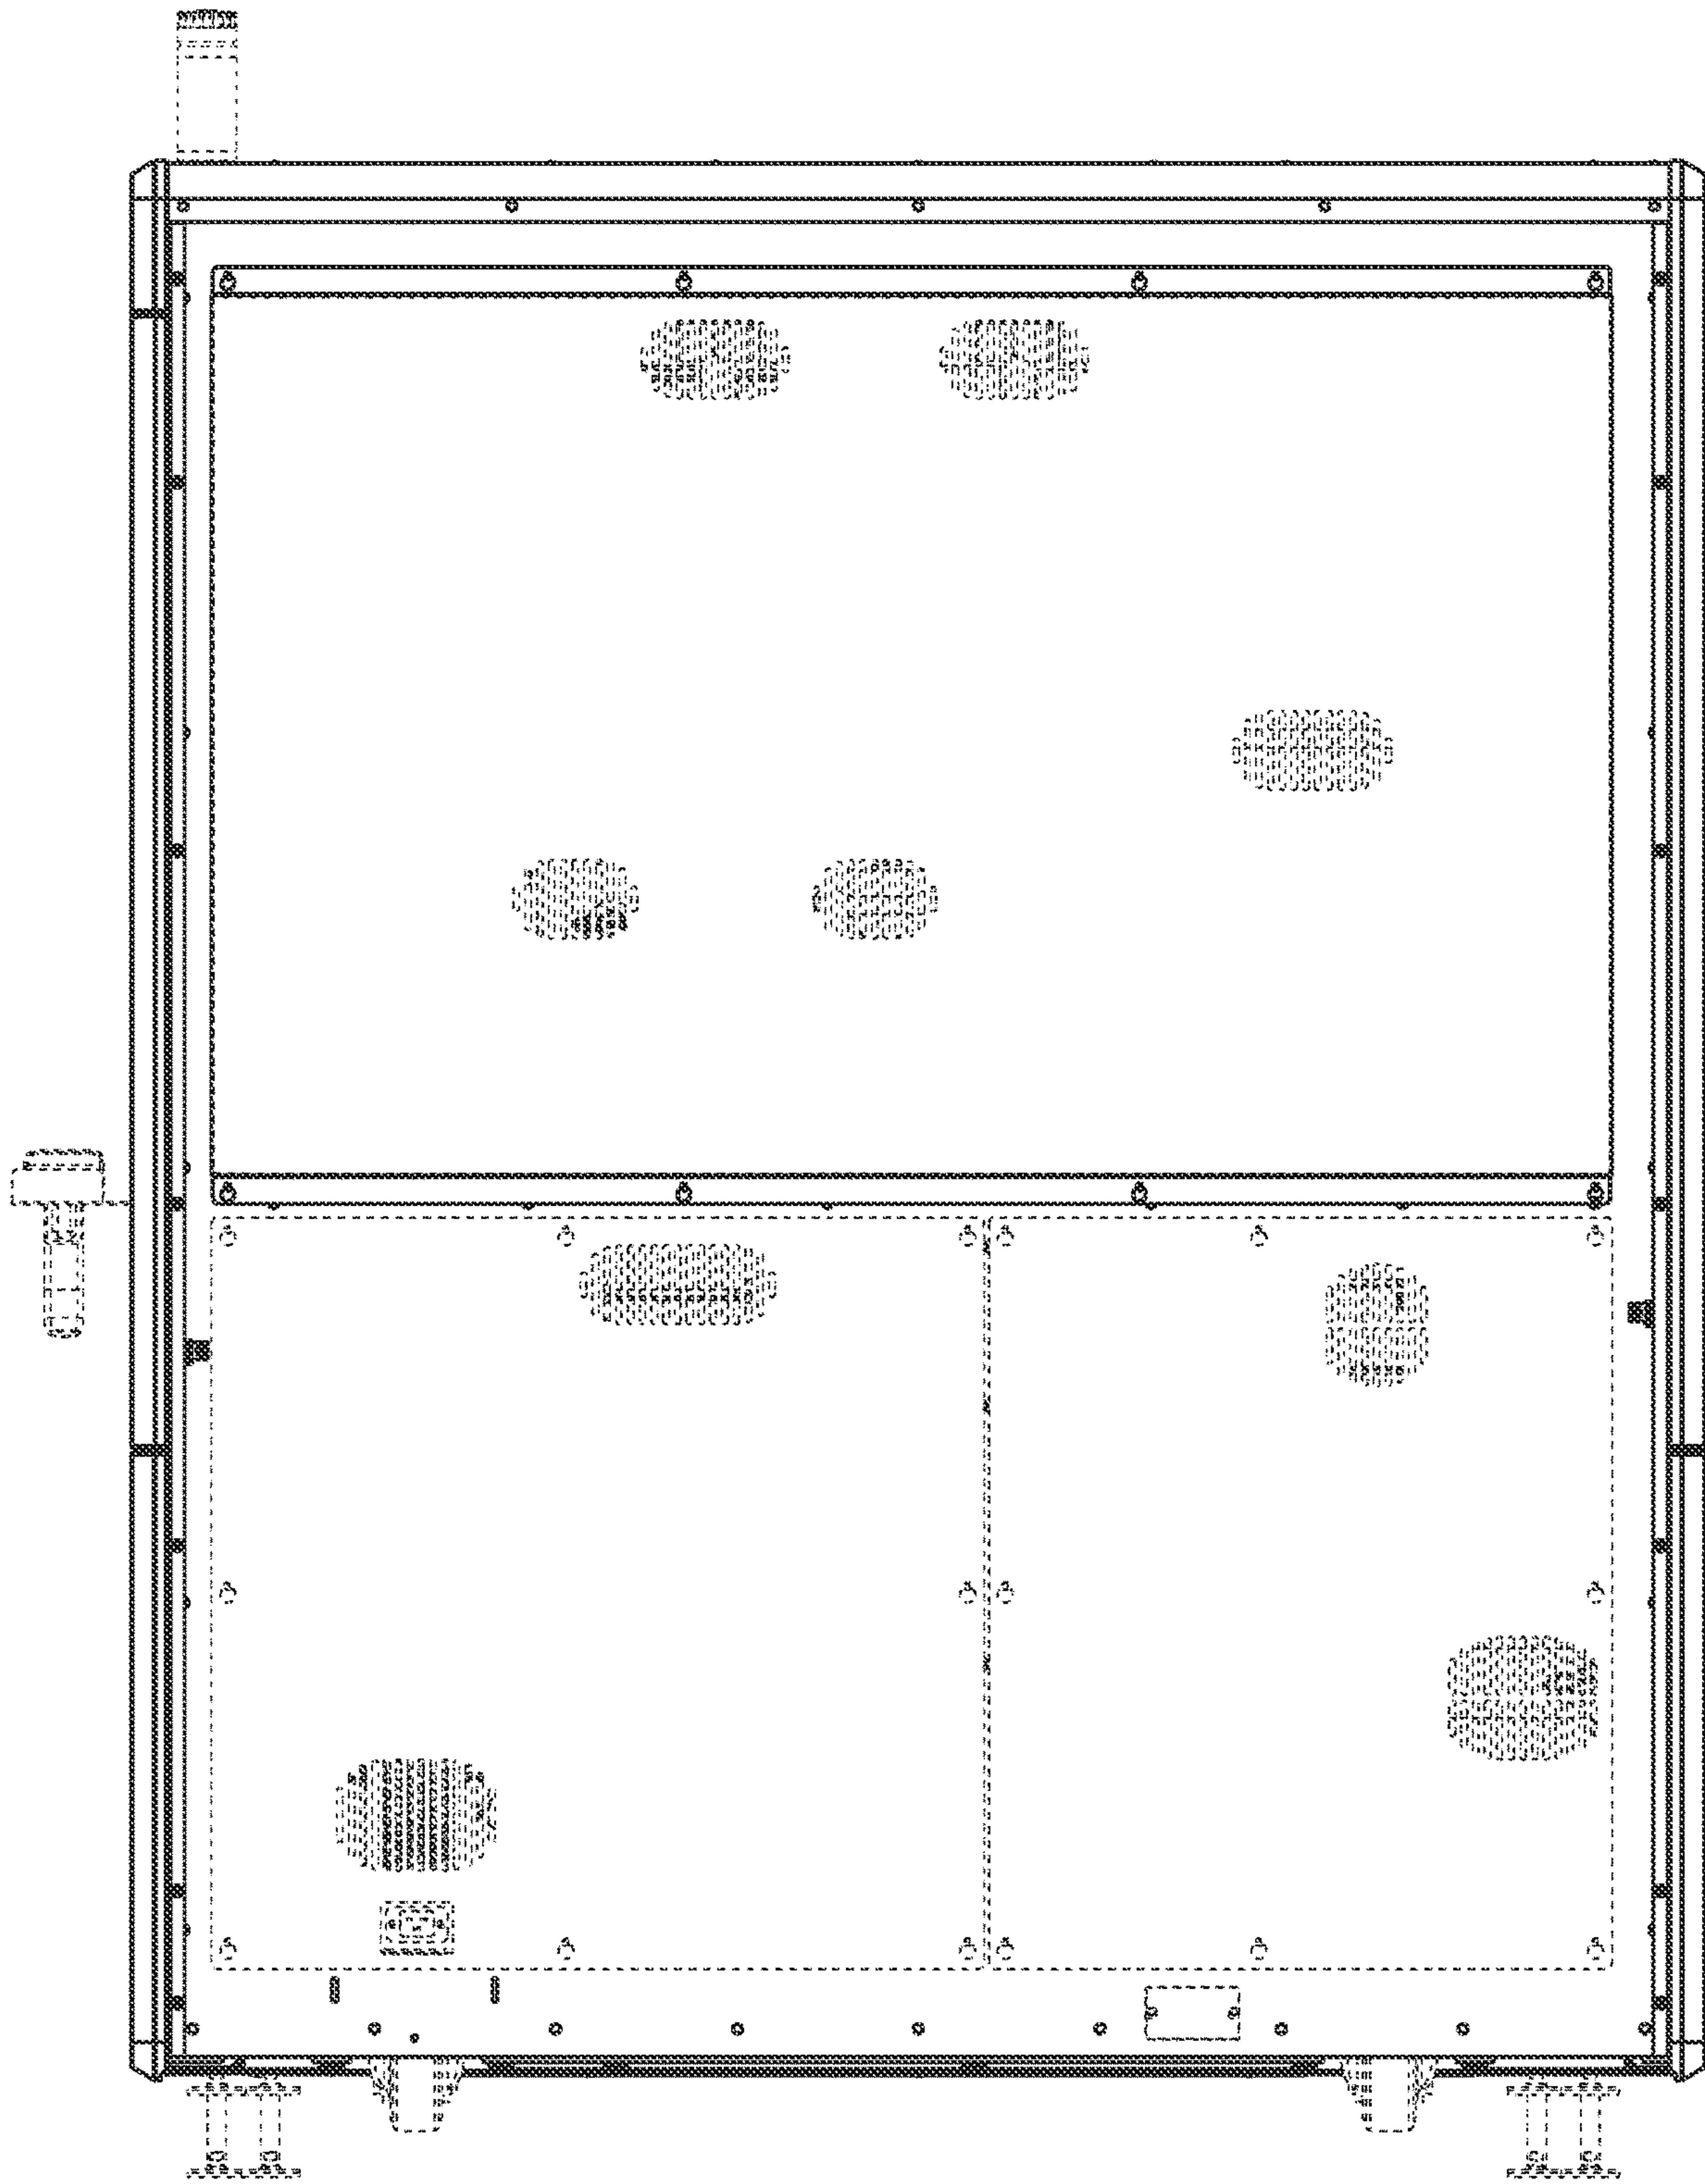


Fig. 2

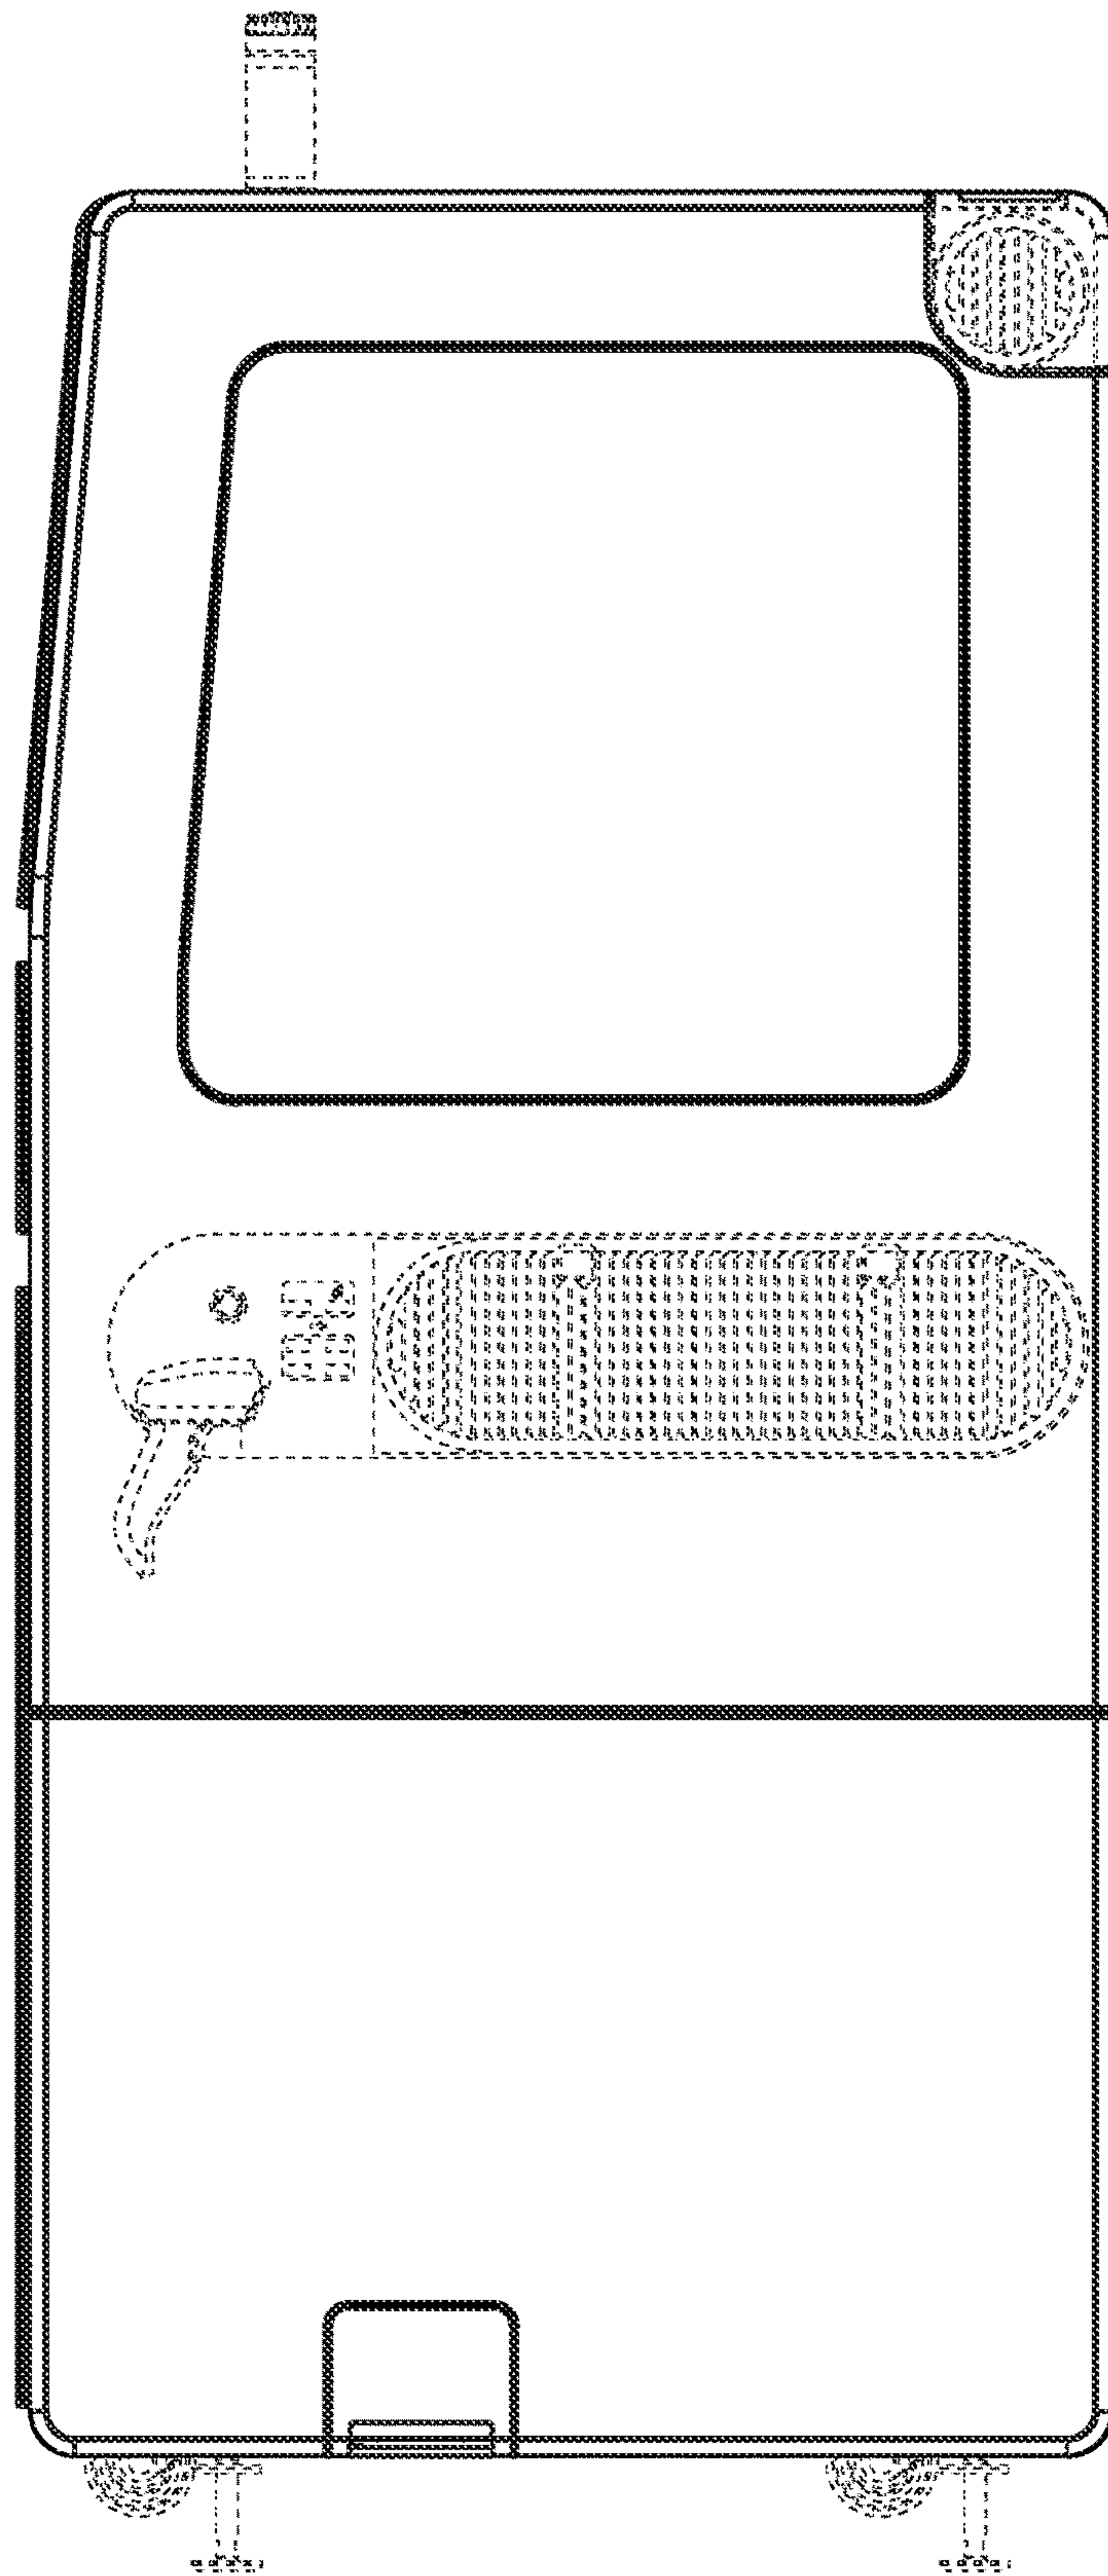


Fig. 3

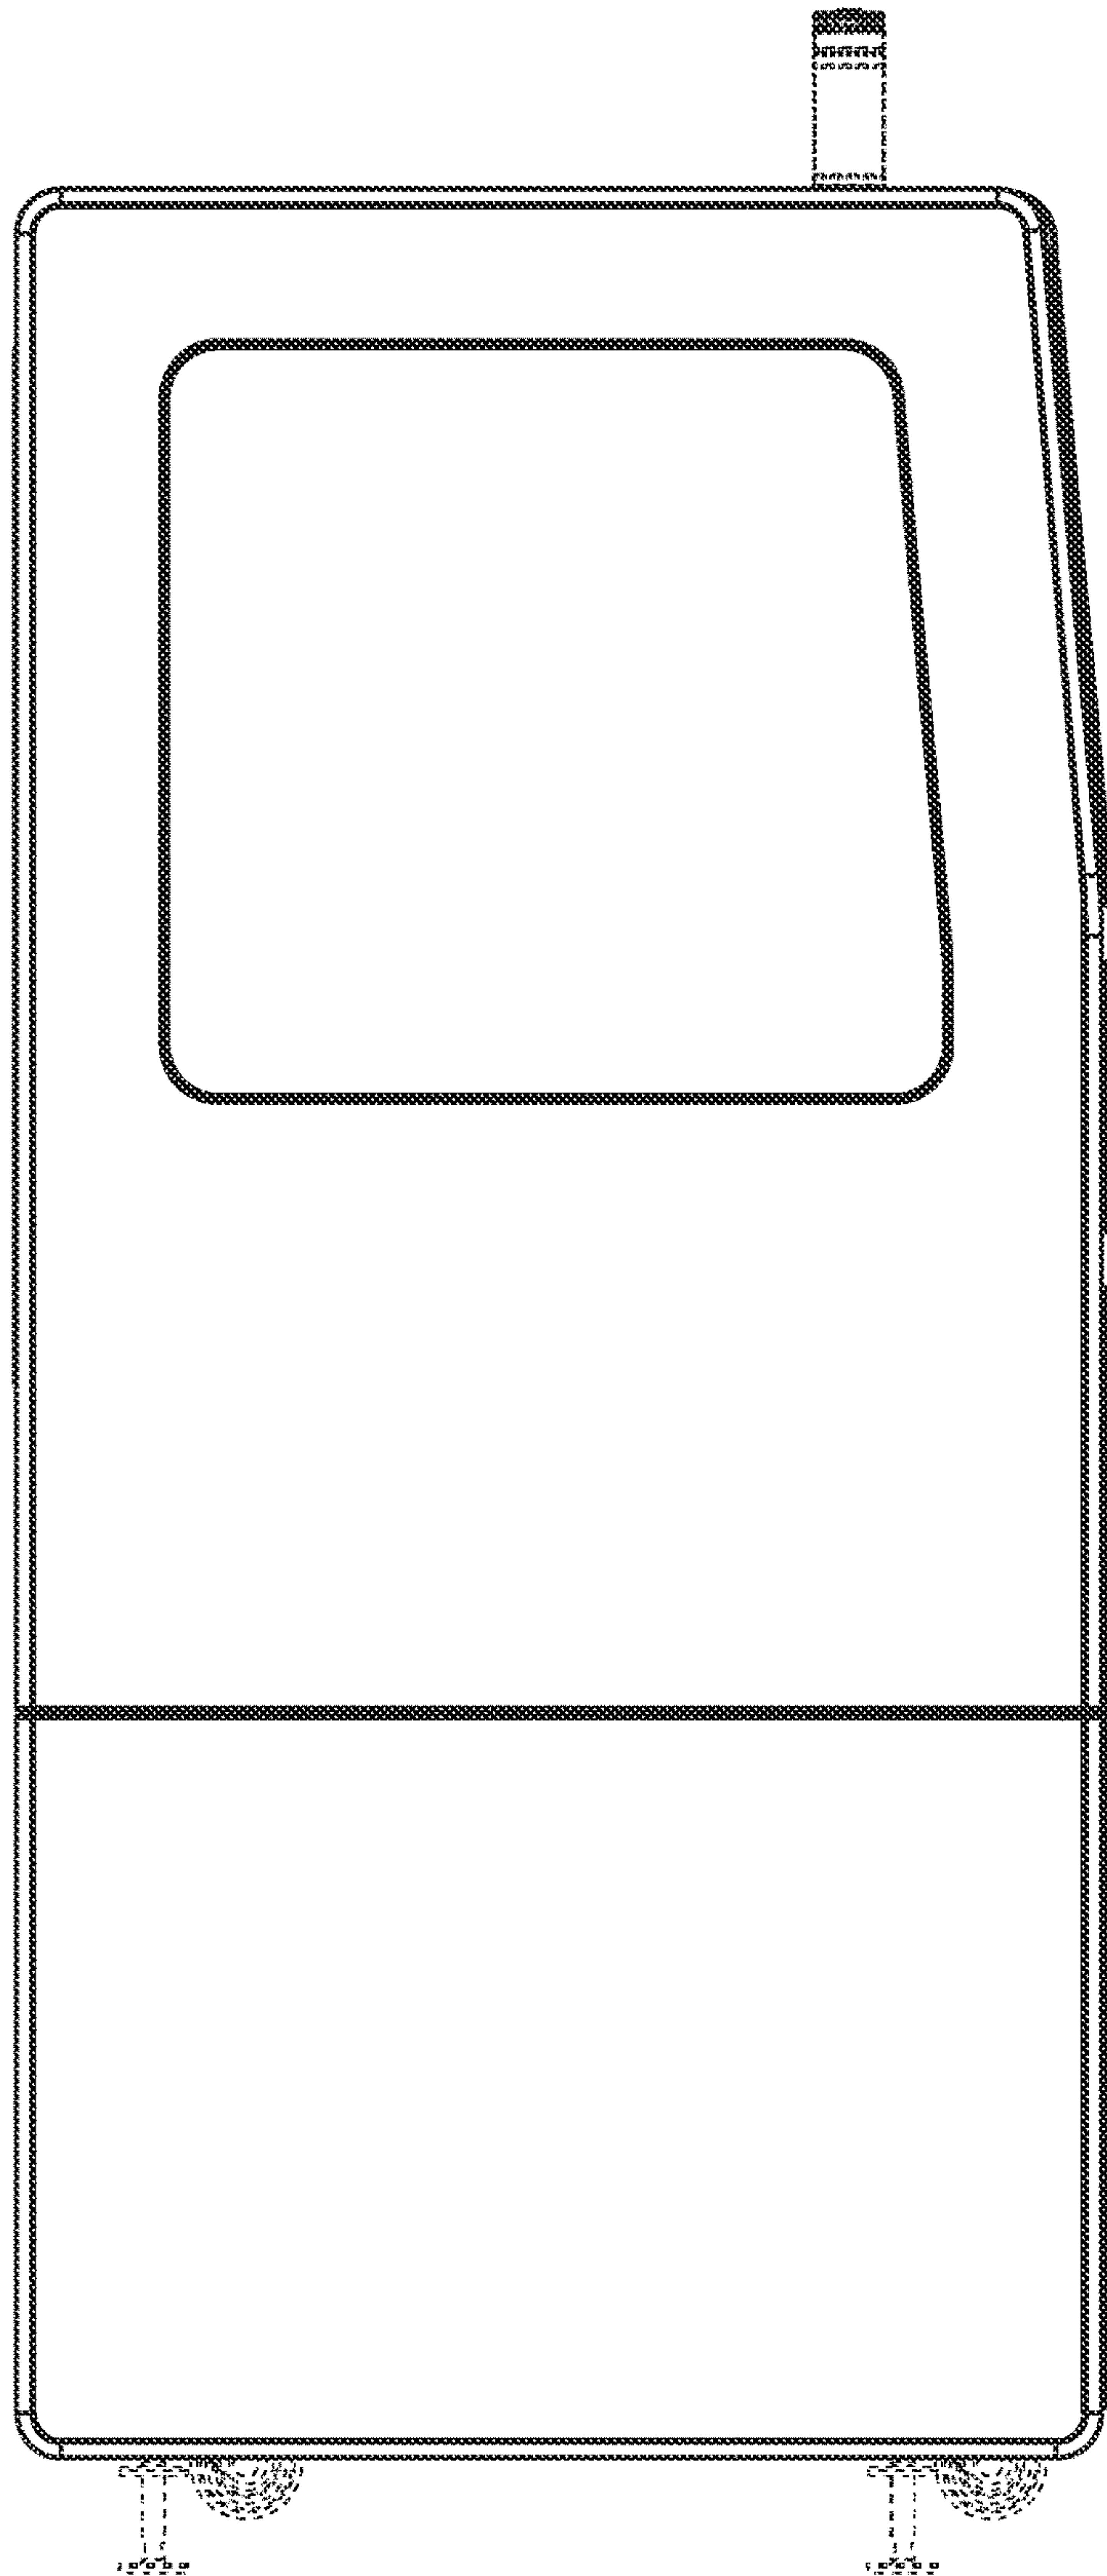


Fig. 4

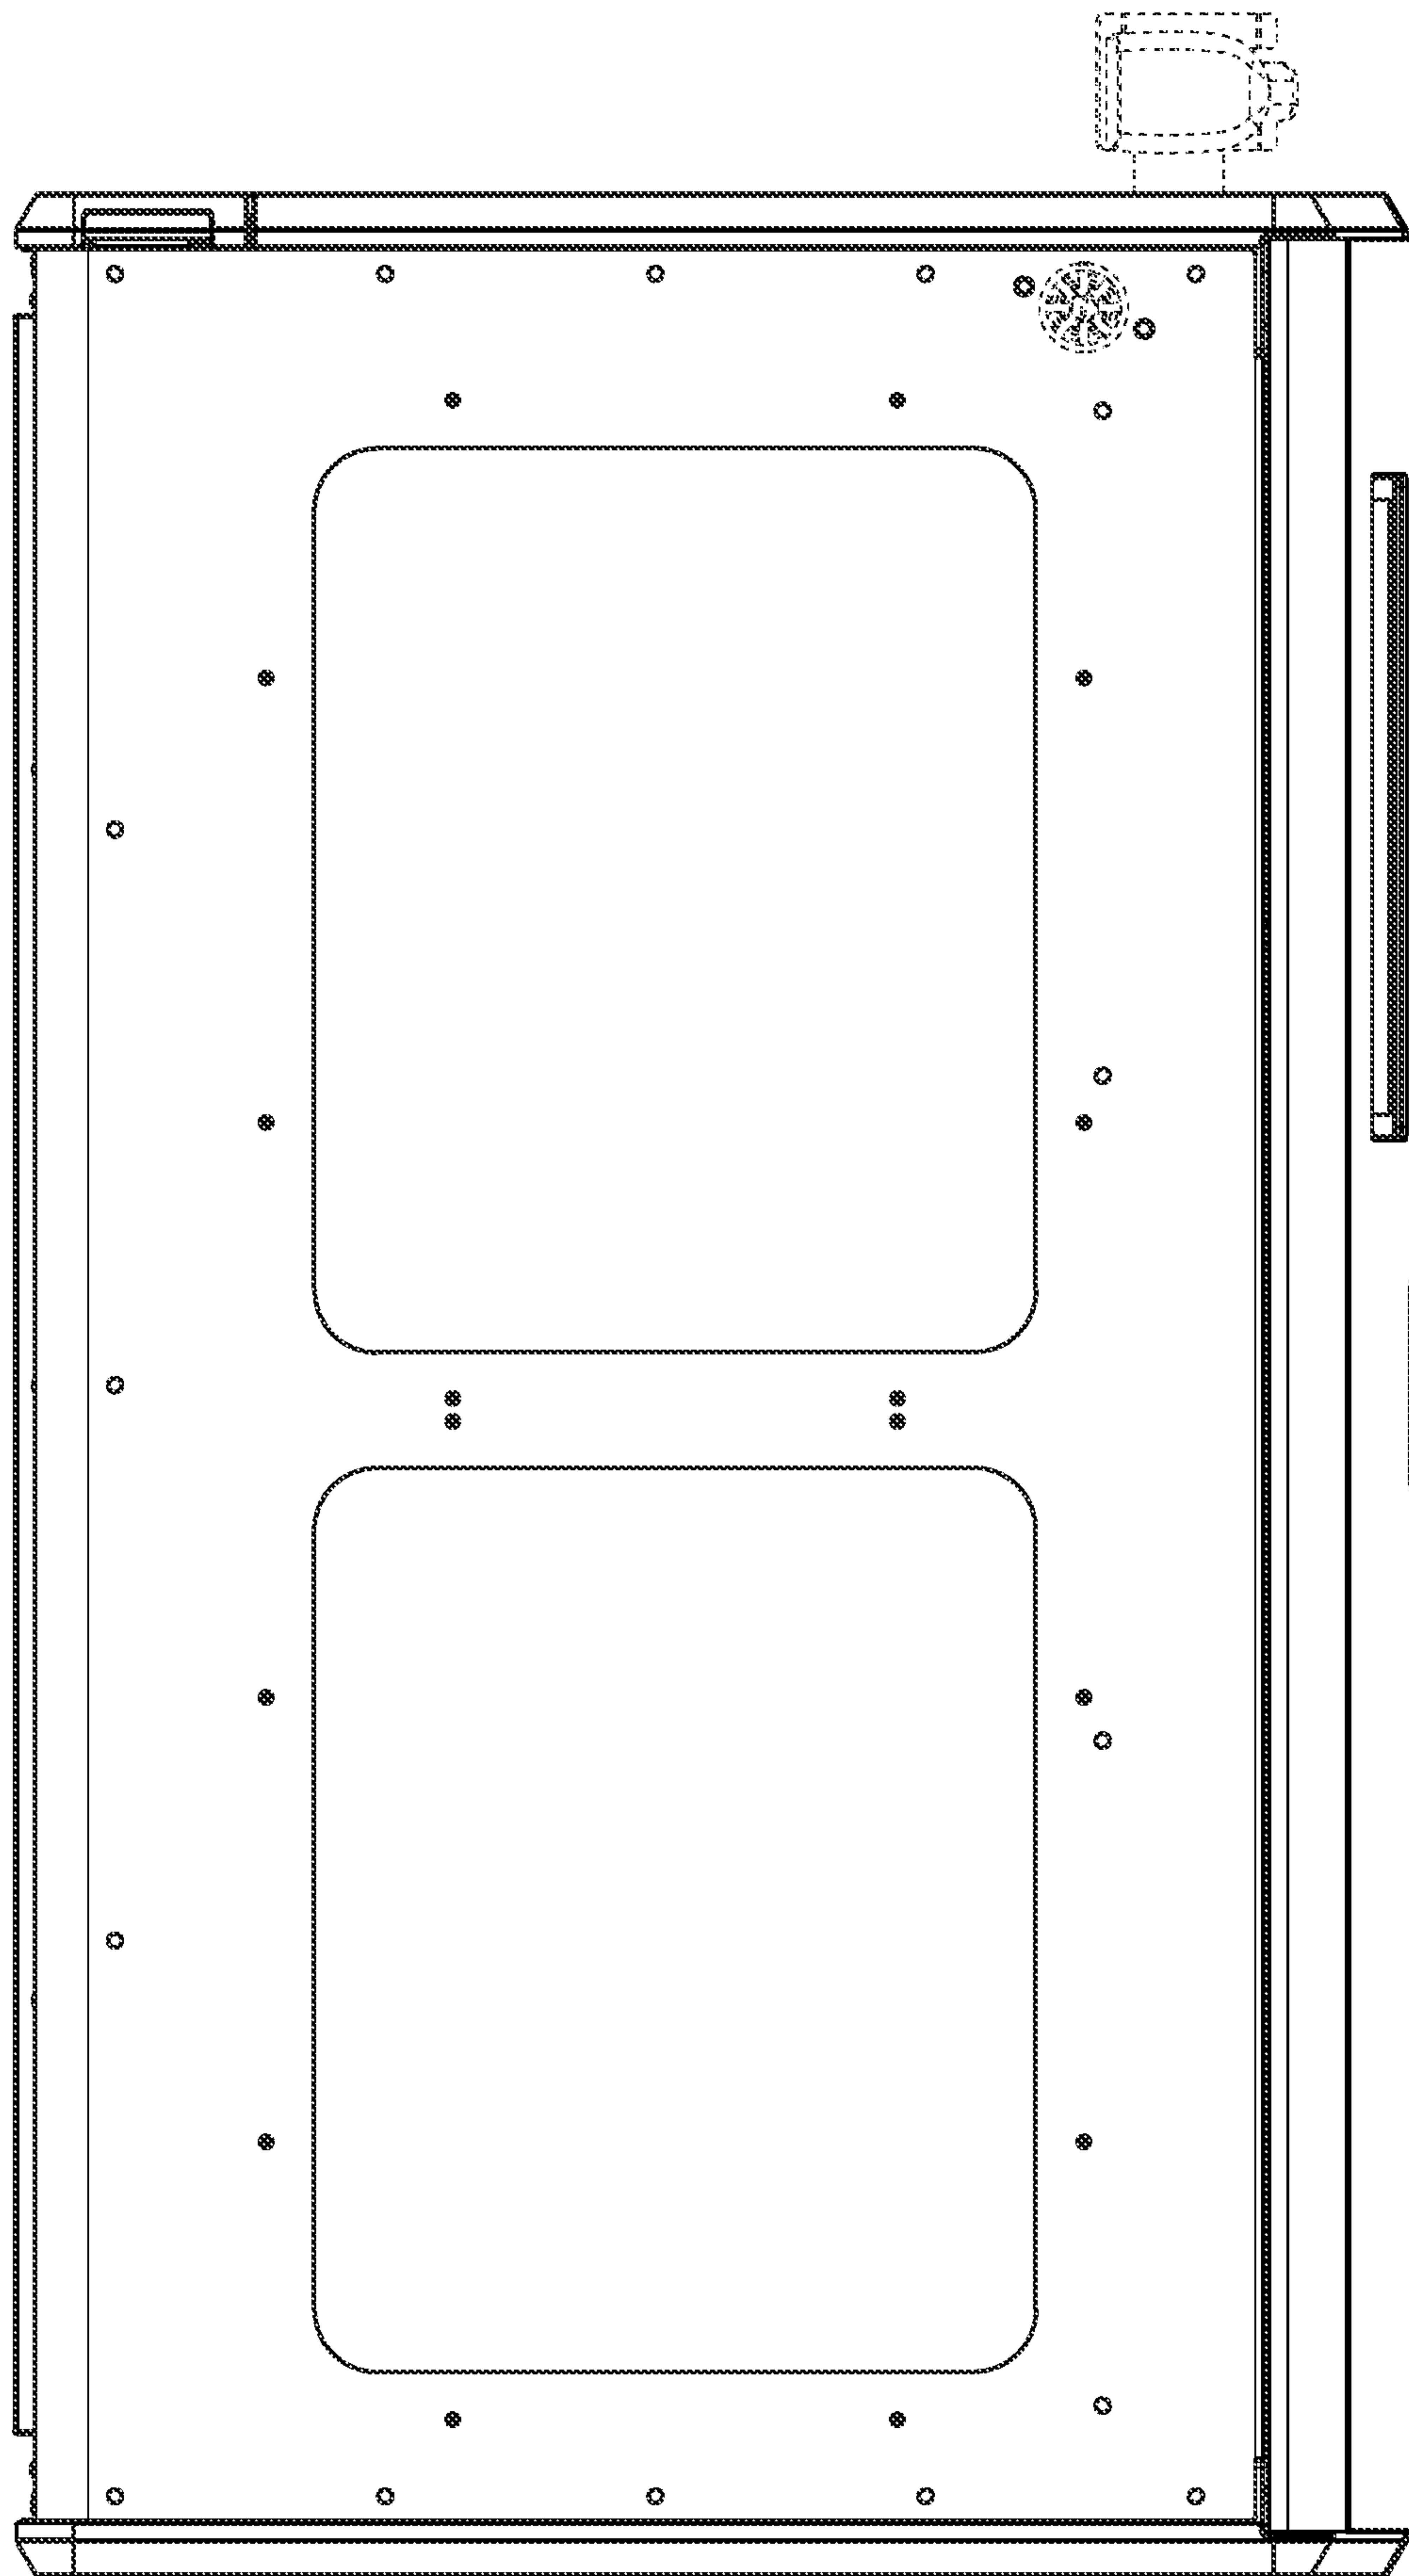


Fig. 5

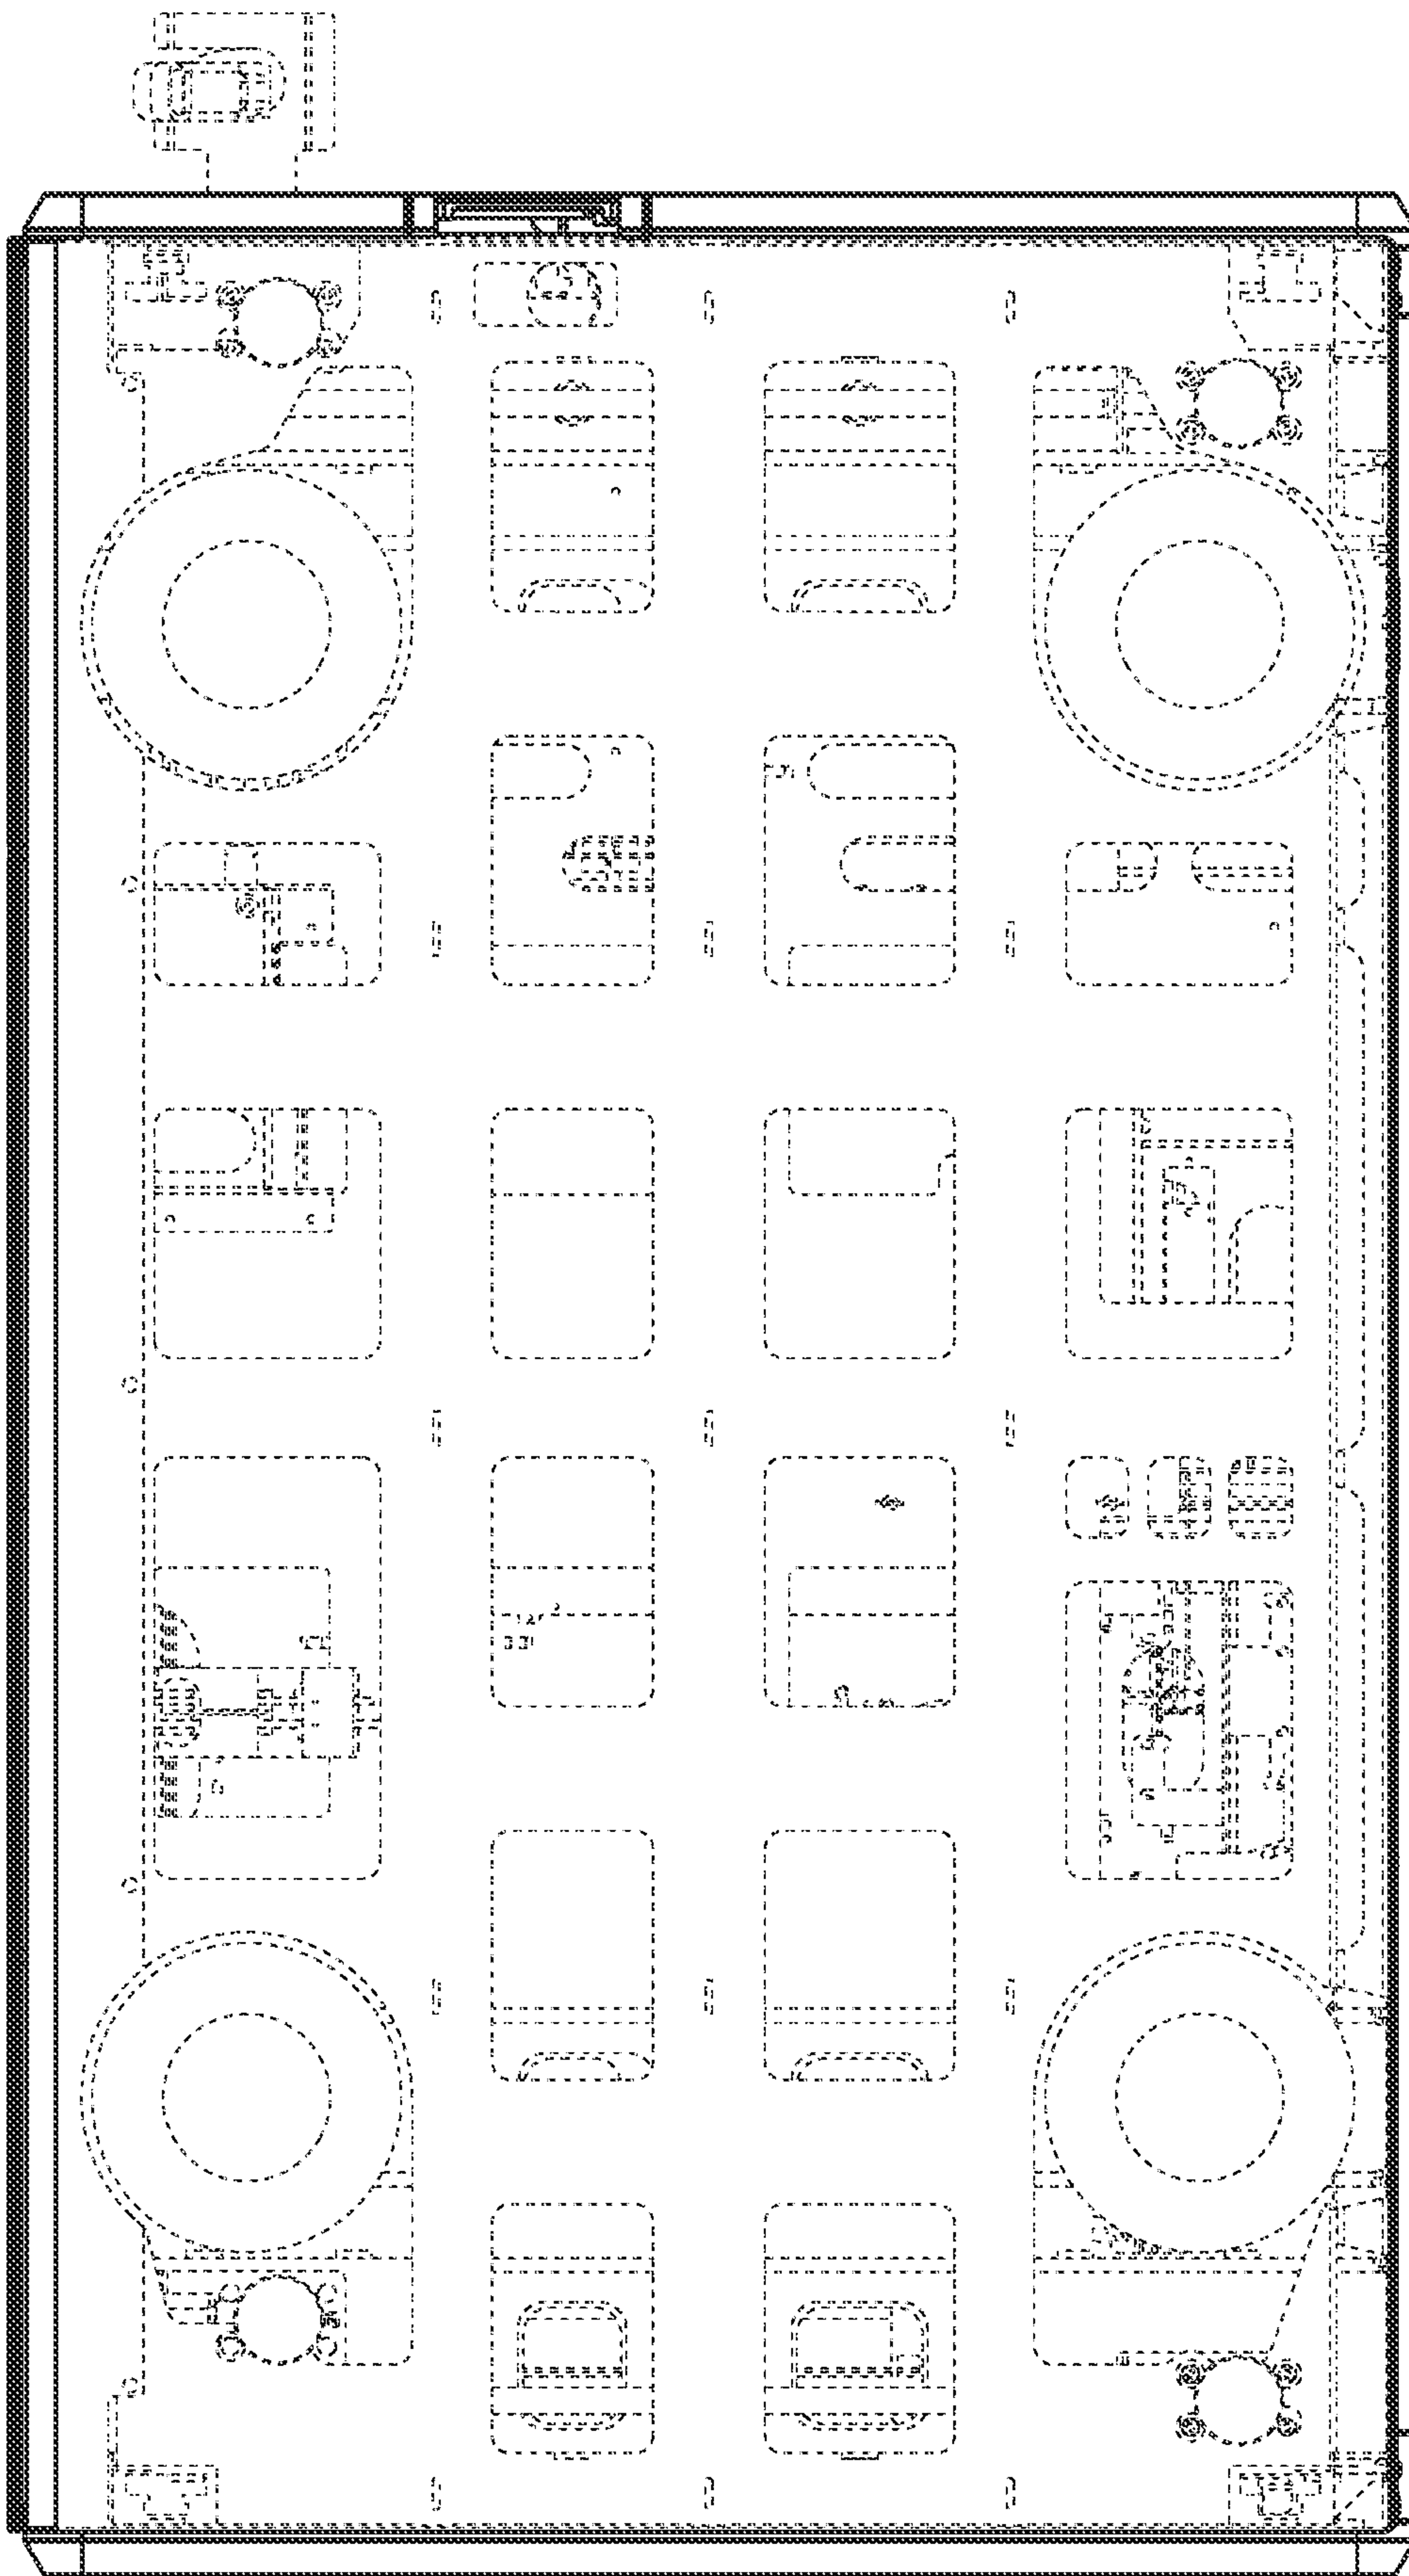


Fig. 6

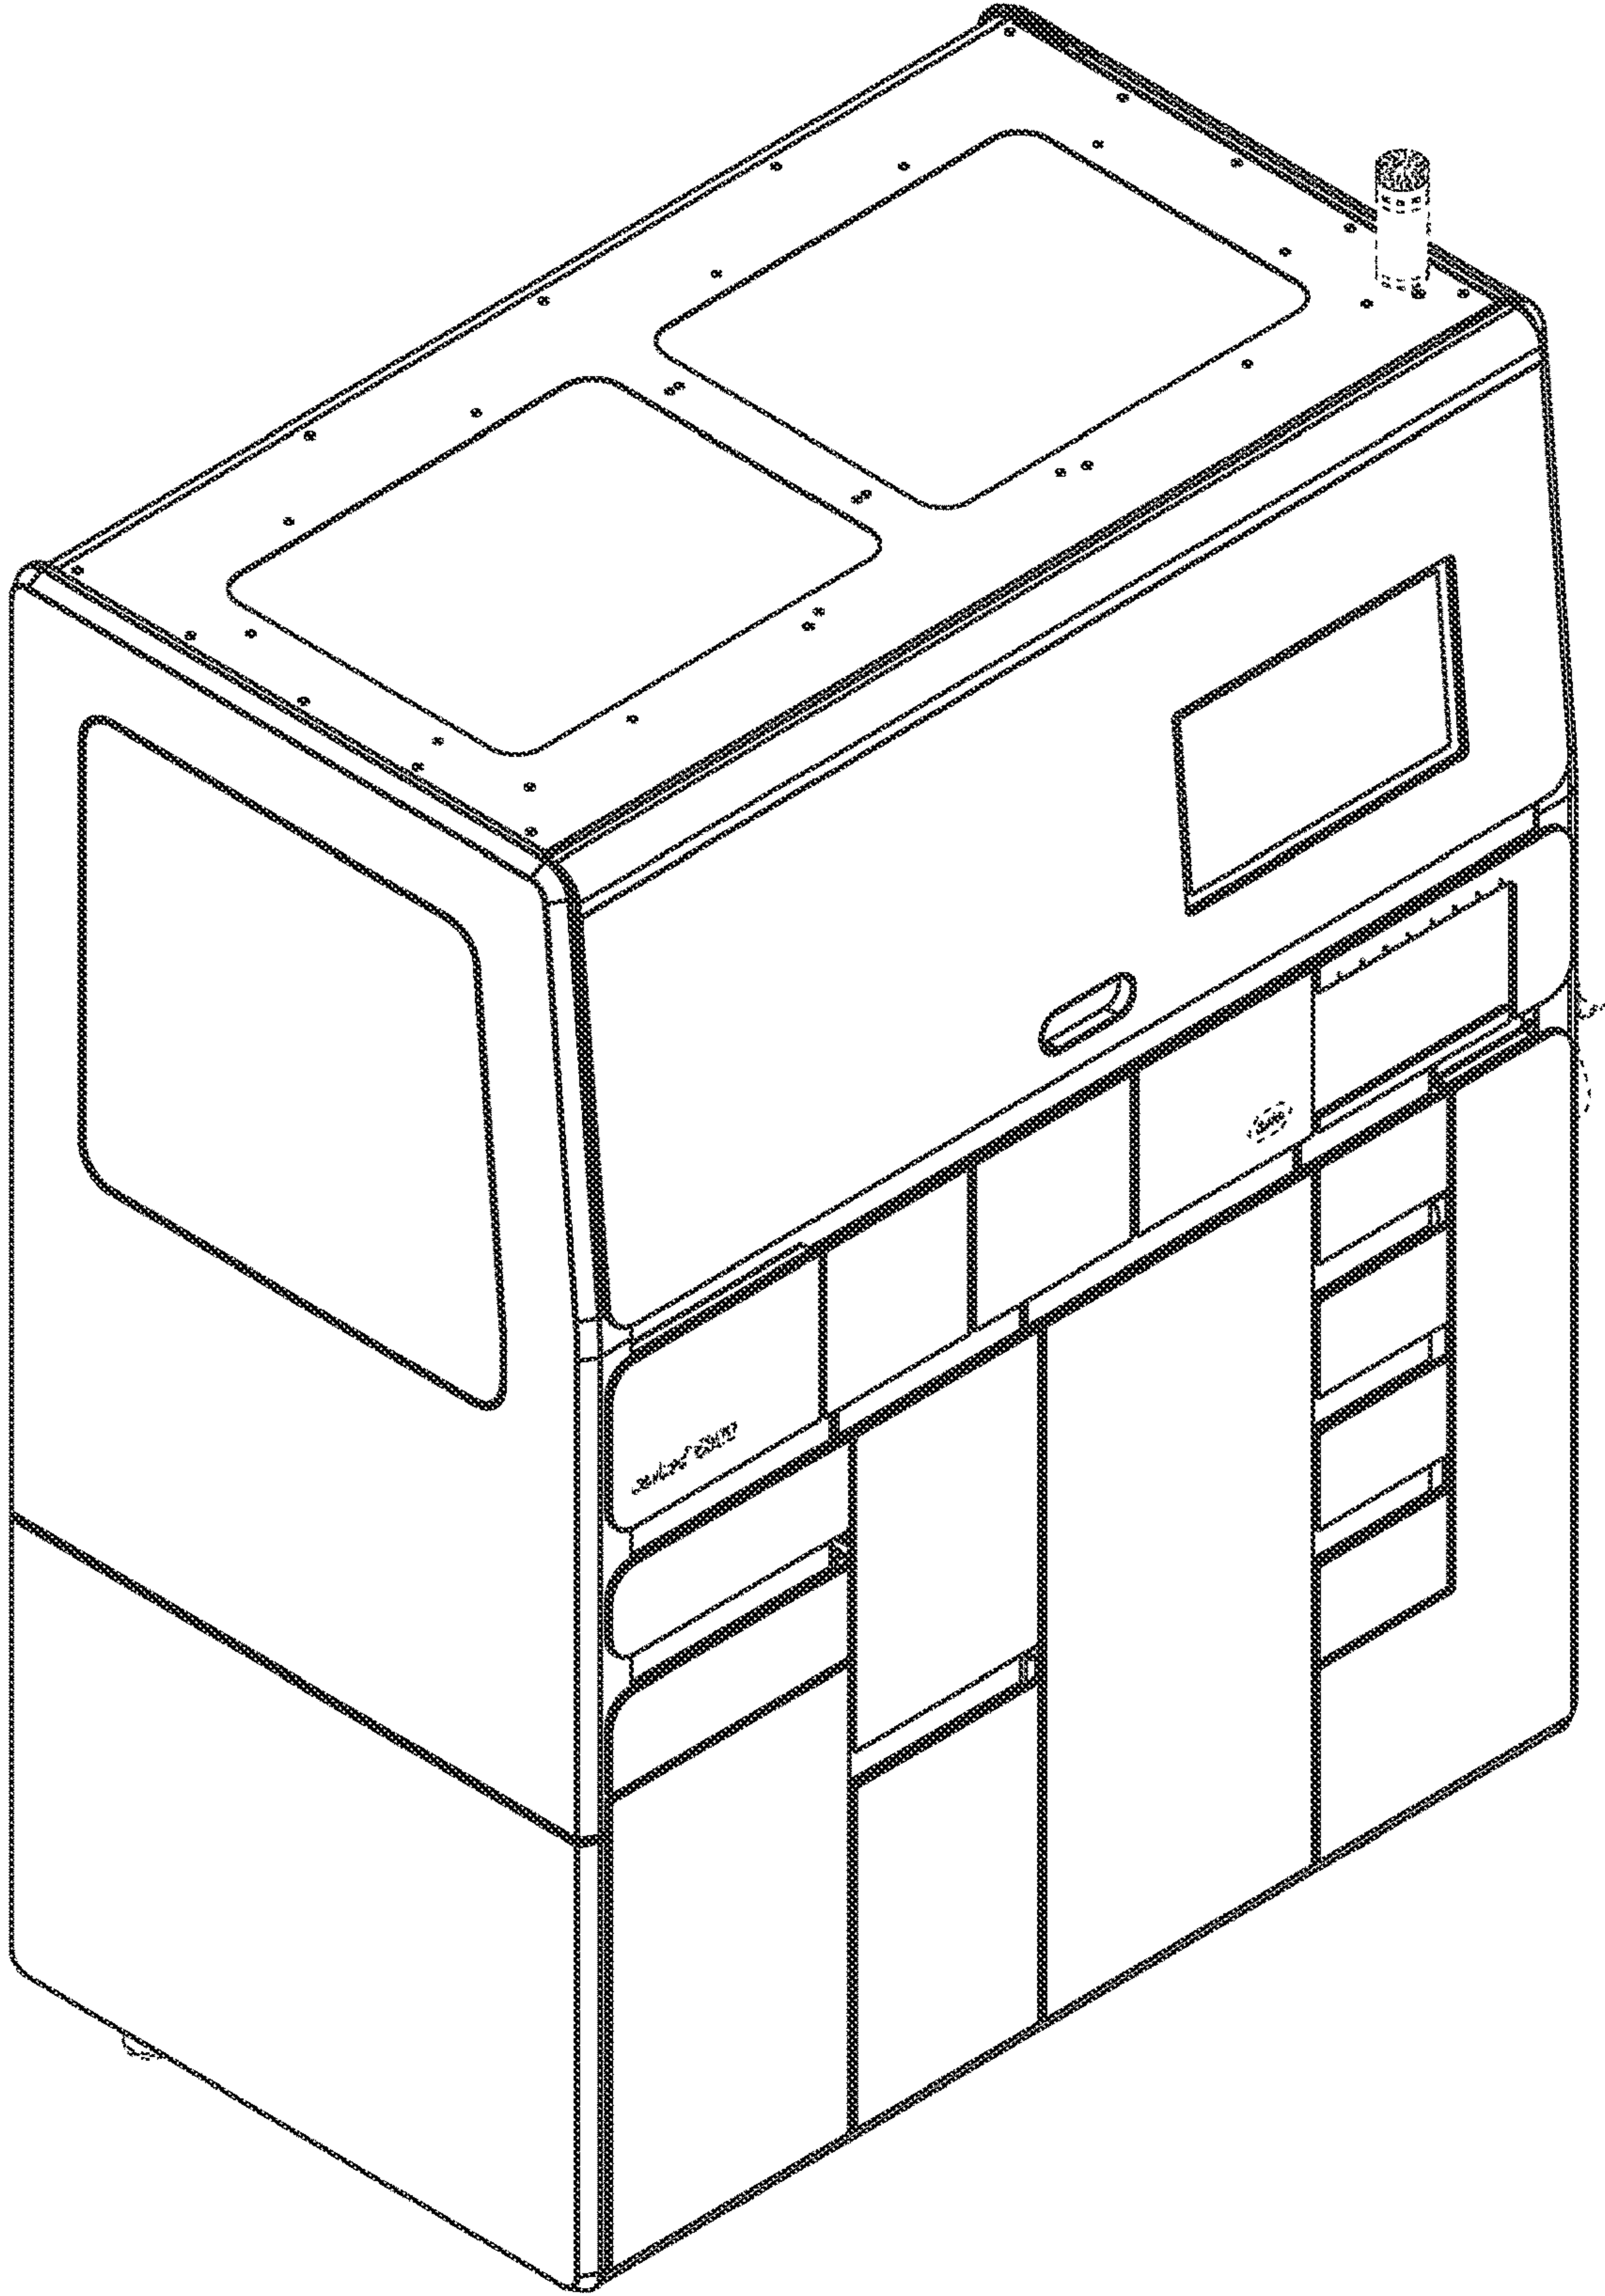


Fig. 7