



US00D979077S

(12) **United States Design Patent** (10) **Patent No.:** **US D979,077 S**  
**Russomanno et al.** (45) **Date of Patent:** **\*\* Feb. 21, 2023**

- (54) **ELECTRODE**
- (71) Applicant: **OpenBCI, Inc.**, Brooklyn, NY (US)
- (72) Inventors: **Conor Russomanno**, Brooklyn, NY (US); **Aaron Trocola**, Brooklyn, NY (US); **Sean Montgomery**, Reno, NV (US)
- (73) Assignee: **OpenBCI, Inc.**, Brooklyn, NY (US)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/773,414**
- (22) Filed: **Mar. 9, 2021**

**Related U.S. Application Data**

- (63) Continuation of application No. PCT/US2021/015470, filed on Jan. 28, 2021.
- (51) **LOC (14) Cl.** ..... **24-02**
- (52) **U.S. Cl.**  
USPC ..... **D24/187**
- (58) **Field of Classification Search**  
USPC ..... D24/107, 168, 186, 187, 189, 200, D24/211–215; D28/63, 74, 77; D30/158  
CPC ..... A61B 5/042; A61B 5/0404; A61B 5/0416; A61N 1/046; A61N 1/0472  
See application file for complete search history.

**References Cited**

**U.S. PATENT DOCUMENTS**

D315,038 S *	2/1991	Strickler	.....	D30/158
D321,434 S *	11/1991	Strickler	.....	D30/158
D333,730 S *	3/1993	Martin	.....	D30/158
D375,588 S *	11/1996	Bzoch	.....	D4/114
D438,975 S *	3/2001	Chen	.....	D24/214
D698,454 S *	1/2014	DiStefano	.....	D24/215
D699,903 S *	2/2014	Singer	.....	D4/124
D712,470 S *	9/2014	Riddle	.....	D19/59
D763,939 S *	8/2016	Khanicheh	.....	D16/130
D797,297 S *	9/2017	Martin	.....	D24/187

D826,412 S *	8/2018	Martin	.....	D24/187
D835,363 S *	12/2018	Hebert	.....	D30/158
D852,367 S *	6/2019	Sargent	.....	D24/187
D869,662 S *	12/2019	Sargent	.....	D24/187

(Continued)

**OTHER PUBLICATIONS**

3D Printed Dry EEG Electrodes. Online, published date Feb. 10, 2016 from URL: <https://www.mdpi.com/1424-8220/16/10/1635/htm>.\*

(Continued)

*Primary Examiner* — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Zhong Law, LLC

(57) **CLAIM**

The ornamental design for an electrode, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a first embodiment of an electrode in accordance with the claimed design.

FIG. 2 is a top view of the electrode in FIG. 1.

FIG. 3 is a front view of the electrode in FIG. 1. The rear view, left side view, and right side view of the electrode in FIG. 1 are substantially similar to the front view of the electrode shown in FIG. 3.

FIG. 4 is a bottom view of the electrode in FIG. 1.

FIG. 5 is a perspective view of a second embodiment of the electrode in accordance with the claimed design.


FIG. 6 is a top view of the electrode in FIG. 5.

FIG. 7 is a front view of the electrode in FIG. 5. The rear view, left side view, and right side view of the electrode in FIG. 5 are substantially similar to the front view of the electrode shown in FIG. 7; and,

FIG. 8 is a bottom view of the electrode in FIG. 5.

The broken lines, the areas within them, and the areas bounded by broken lines and solid lines depict portions of the electrode that form no part of the claimed design.

**1 Claim, 8 Drawing Sheets**

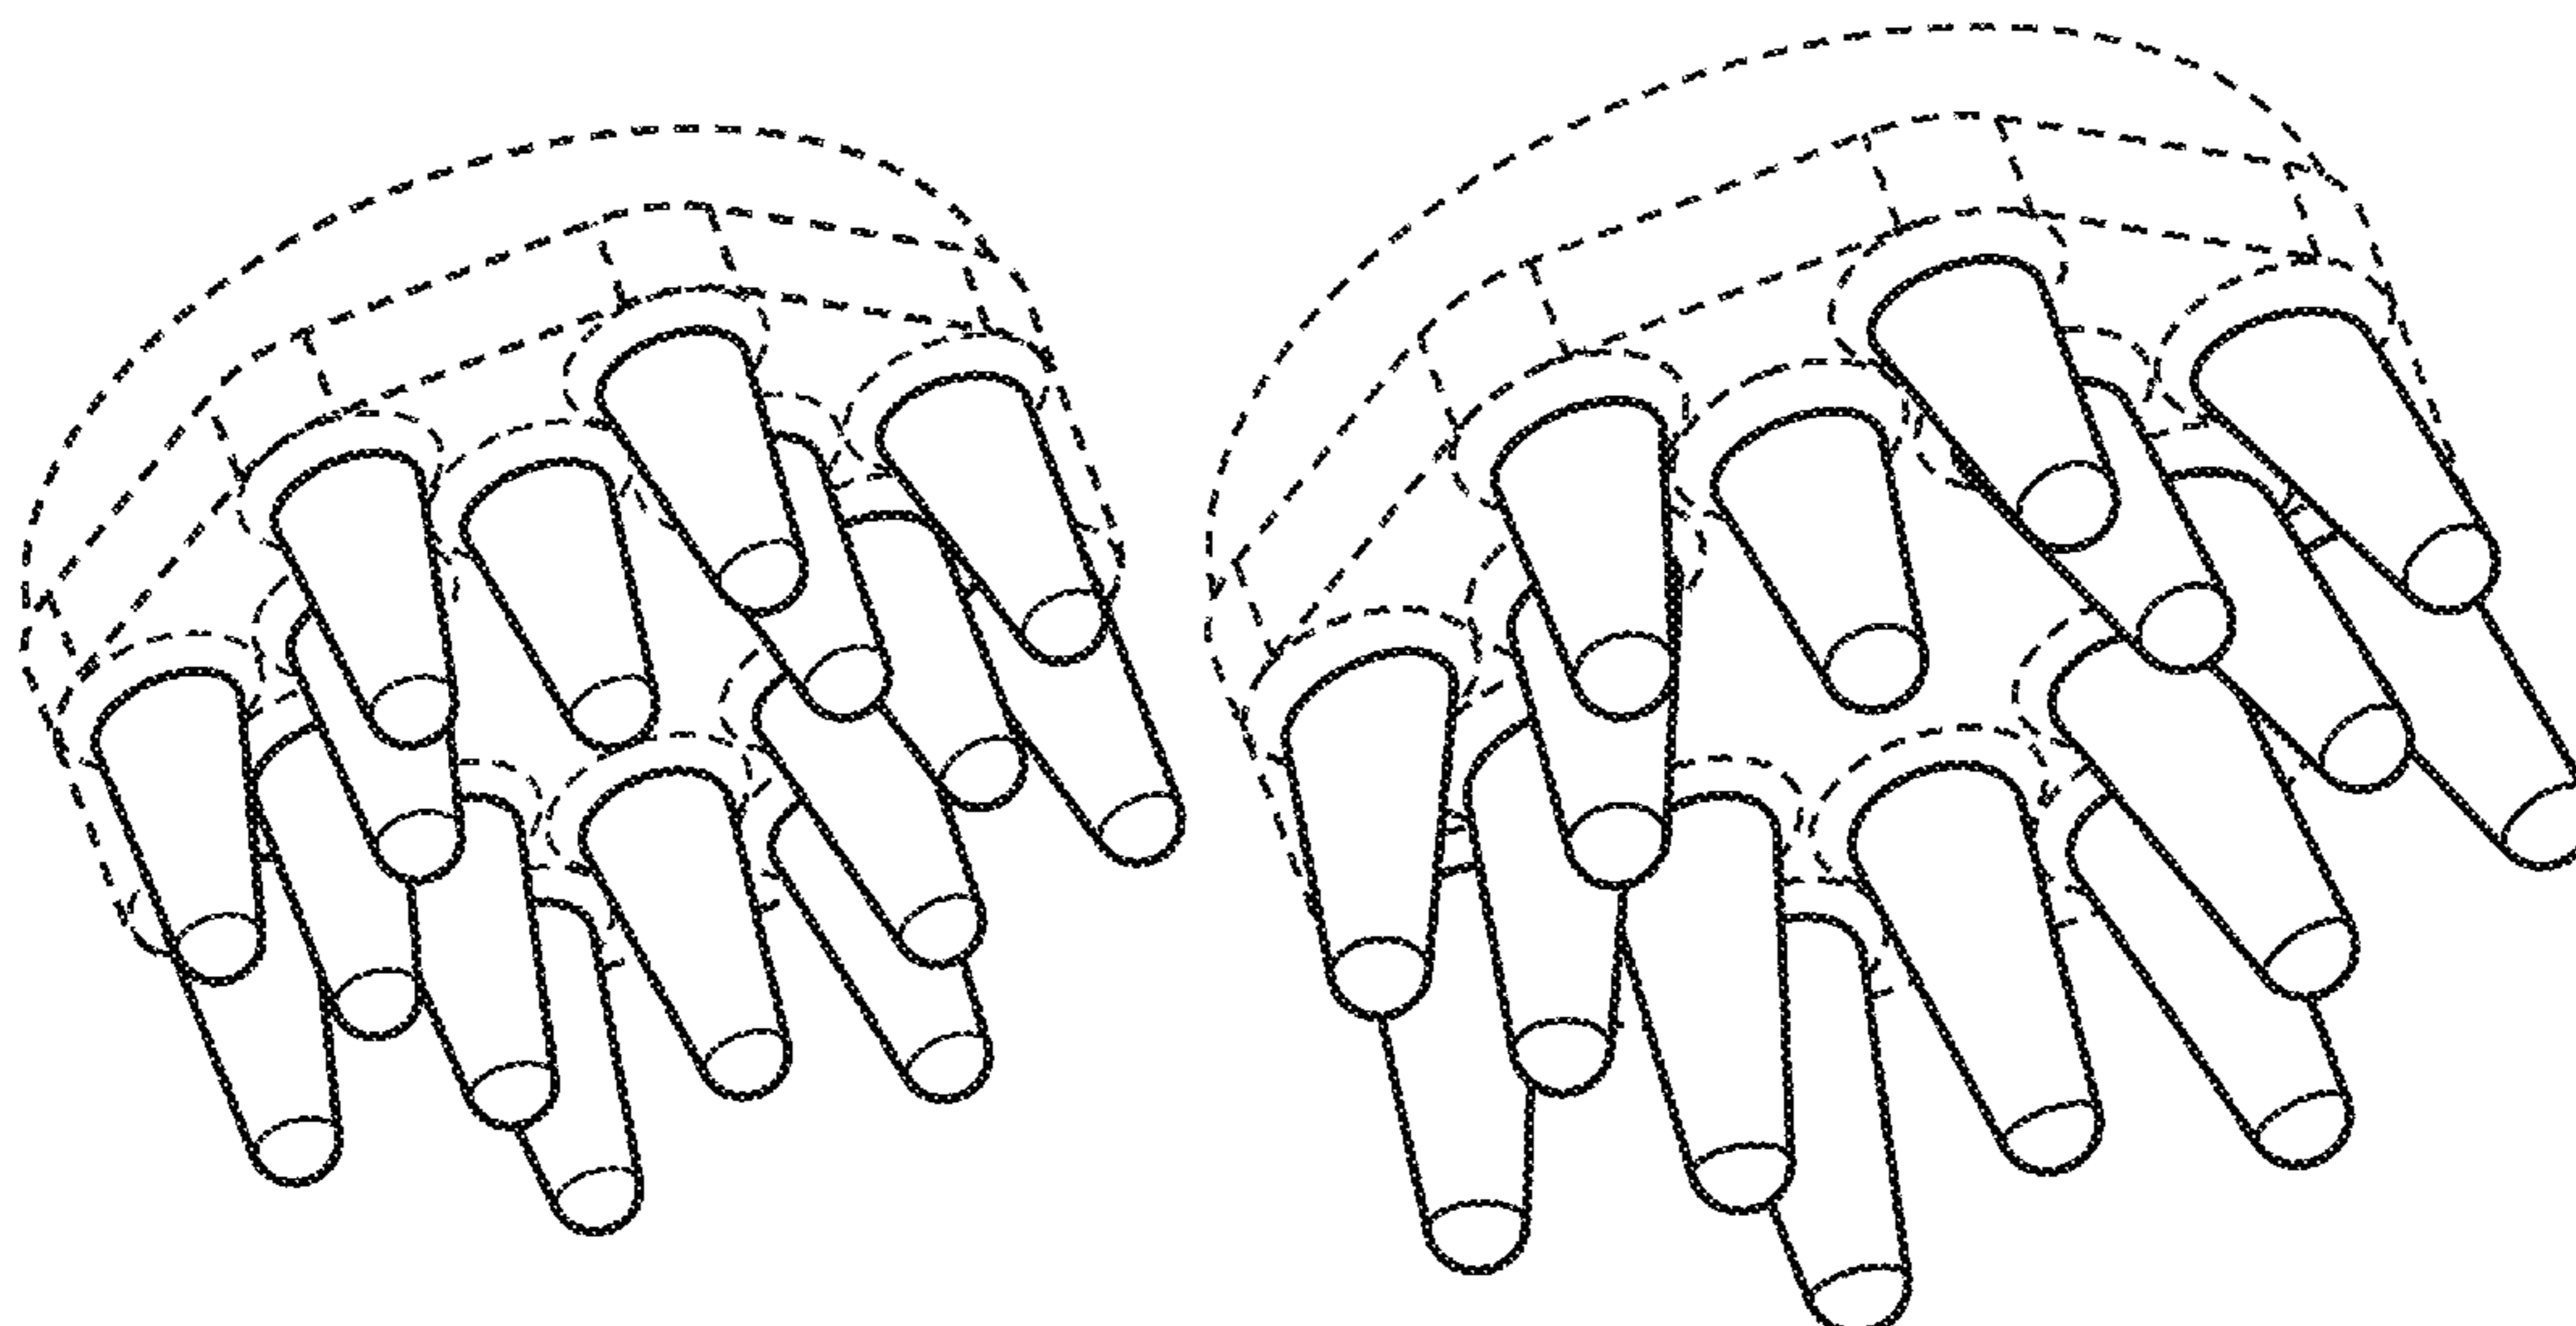

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D898,376 S \* 10/2020 Johnson ..... D4/134  
D917,714 S \* 4/2021 Chen ..... D24/187  
D935,624 S \* 11/2021 Soulet De Brugiere .... D24/187  
2015/0182165 A1\* 7/2015 Miller ..... A61B 5/6814  
600/544

OTHER PUBLICATIONS

Dry EEG Comb Electrodes. Online, published date unknown.  
Retrieved on Jun. 13, 2022 from URL: <https://shop.openbci.com/products/5-mm-spike-electrode-pack-of-30>.\*

Buying Dry / Active Electrodes. Online, published date Jan. 2015.  
Retrieved on Jun. 13, 2022 from URL: <https://openbci.com/forum/index.php?p=/discussion/138/buying-dry-active-electrodes>.\*

\* cited by examiner

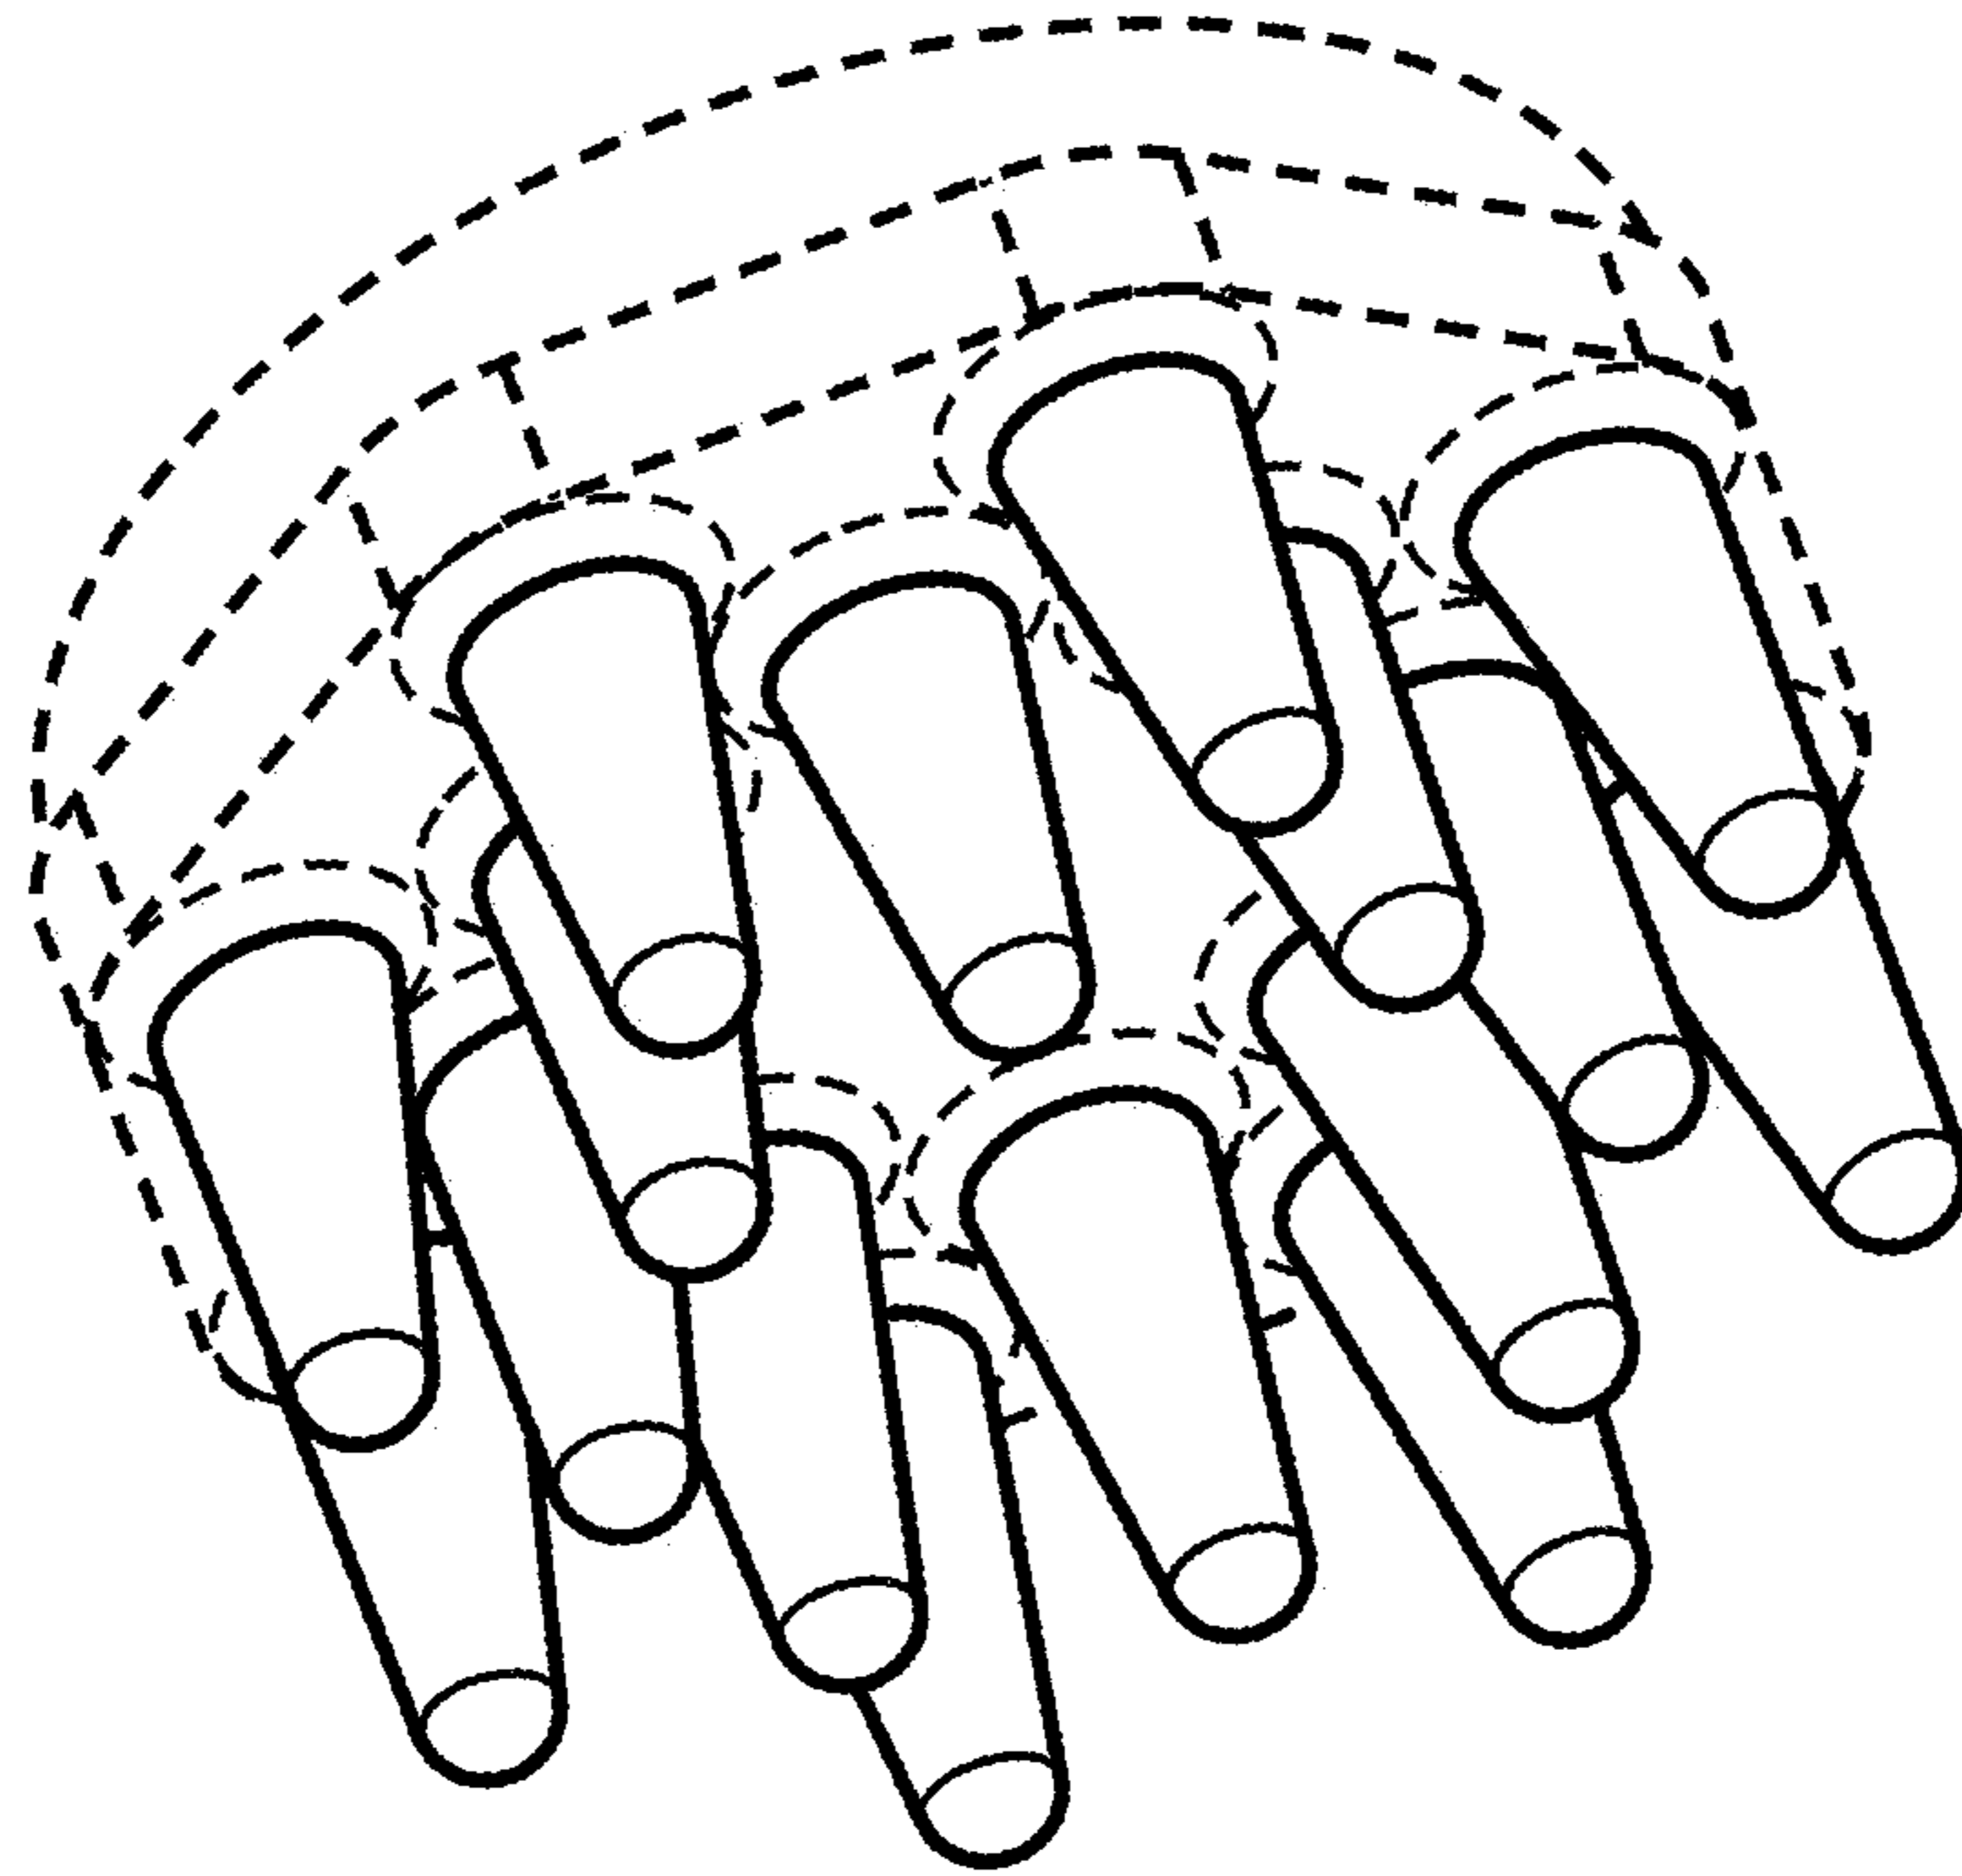


FIG. 1

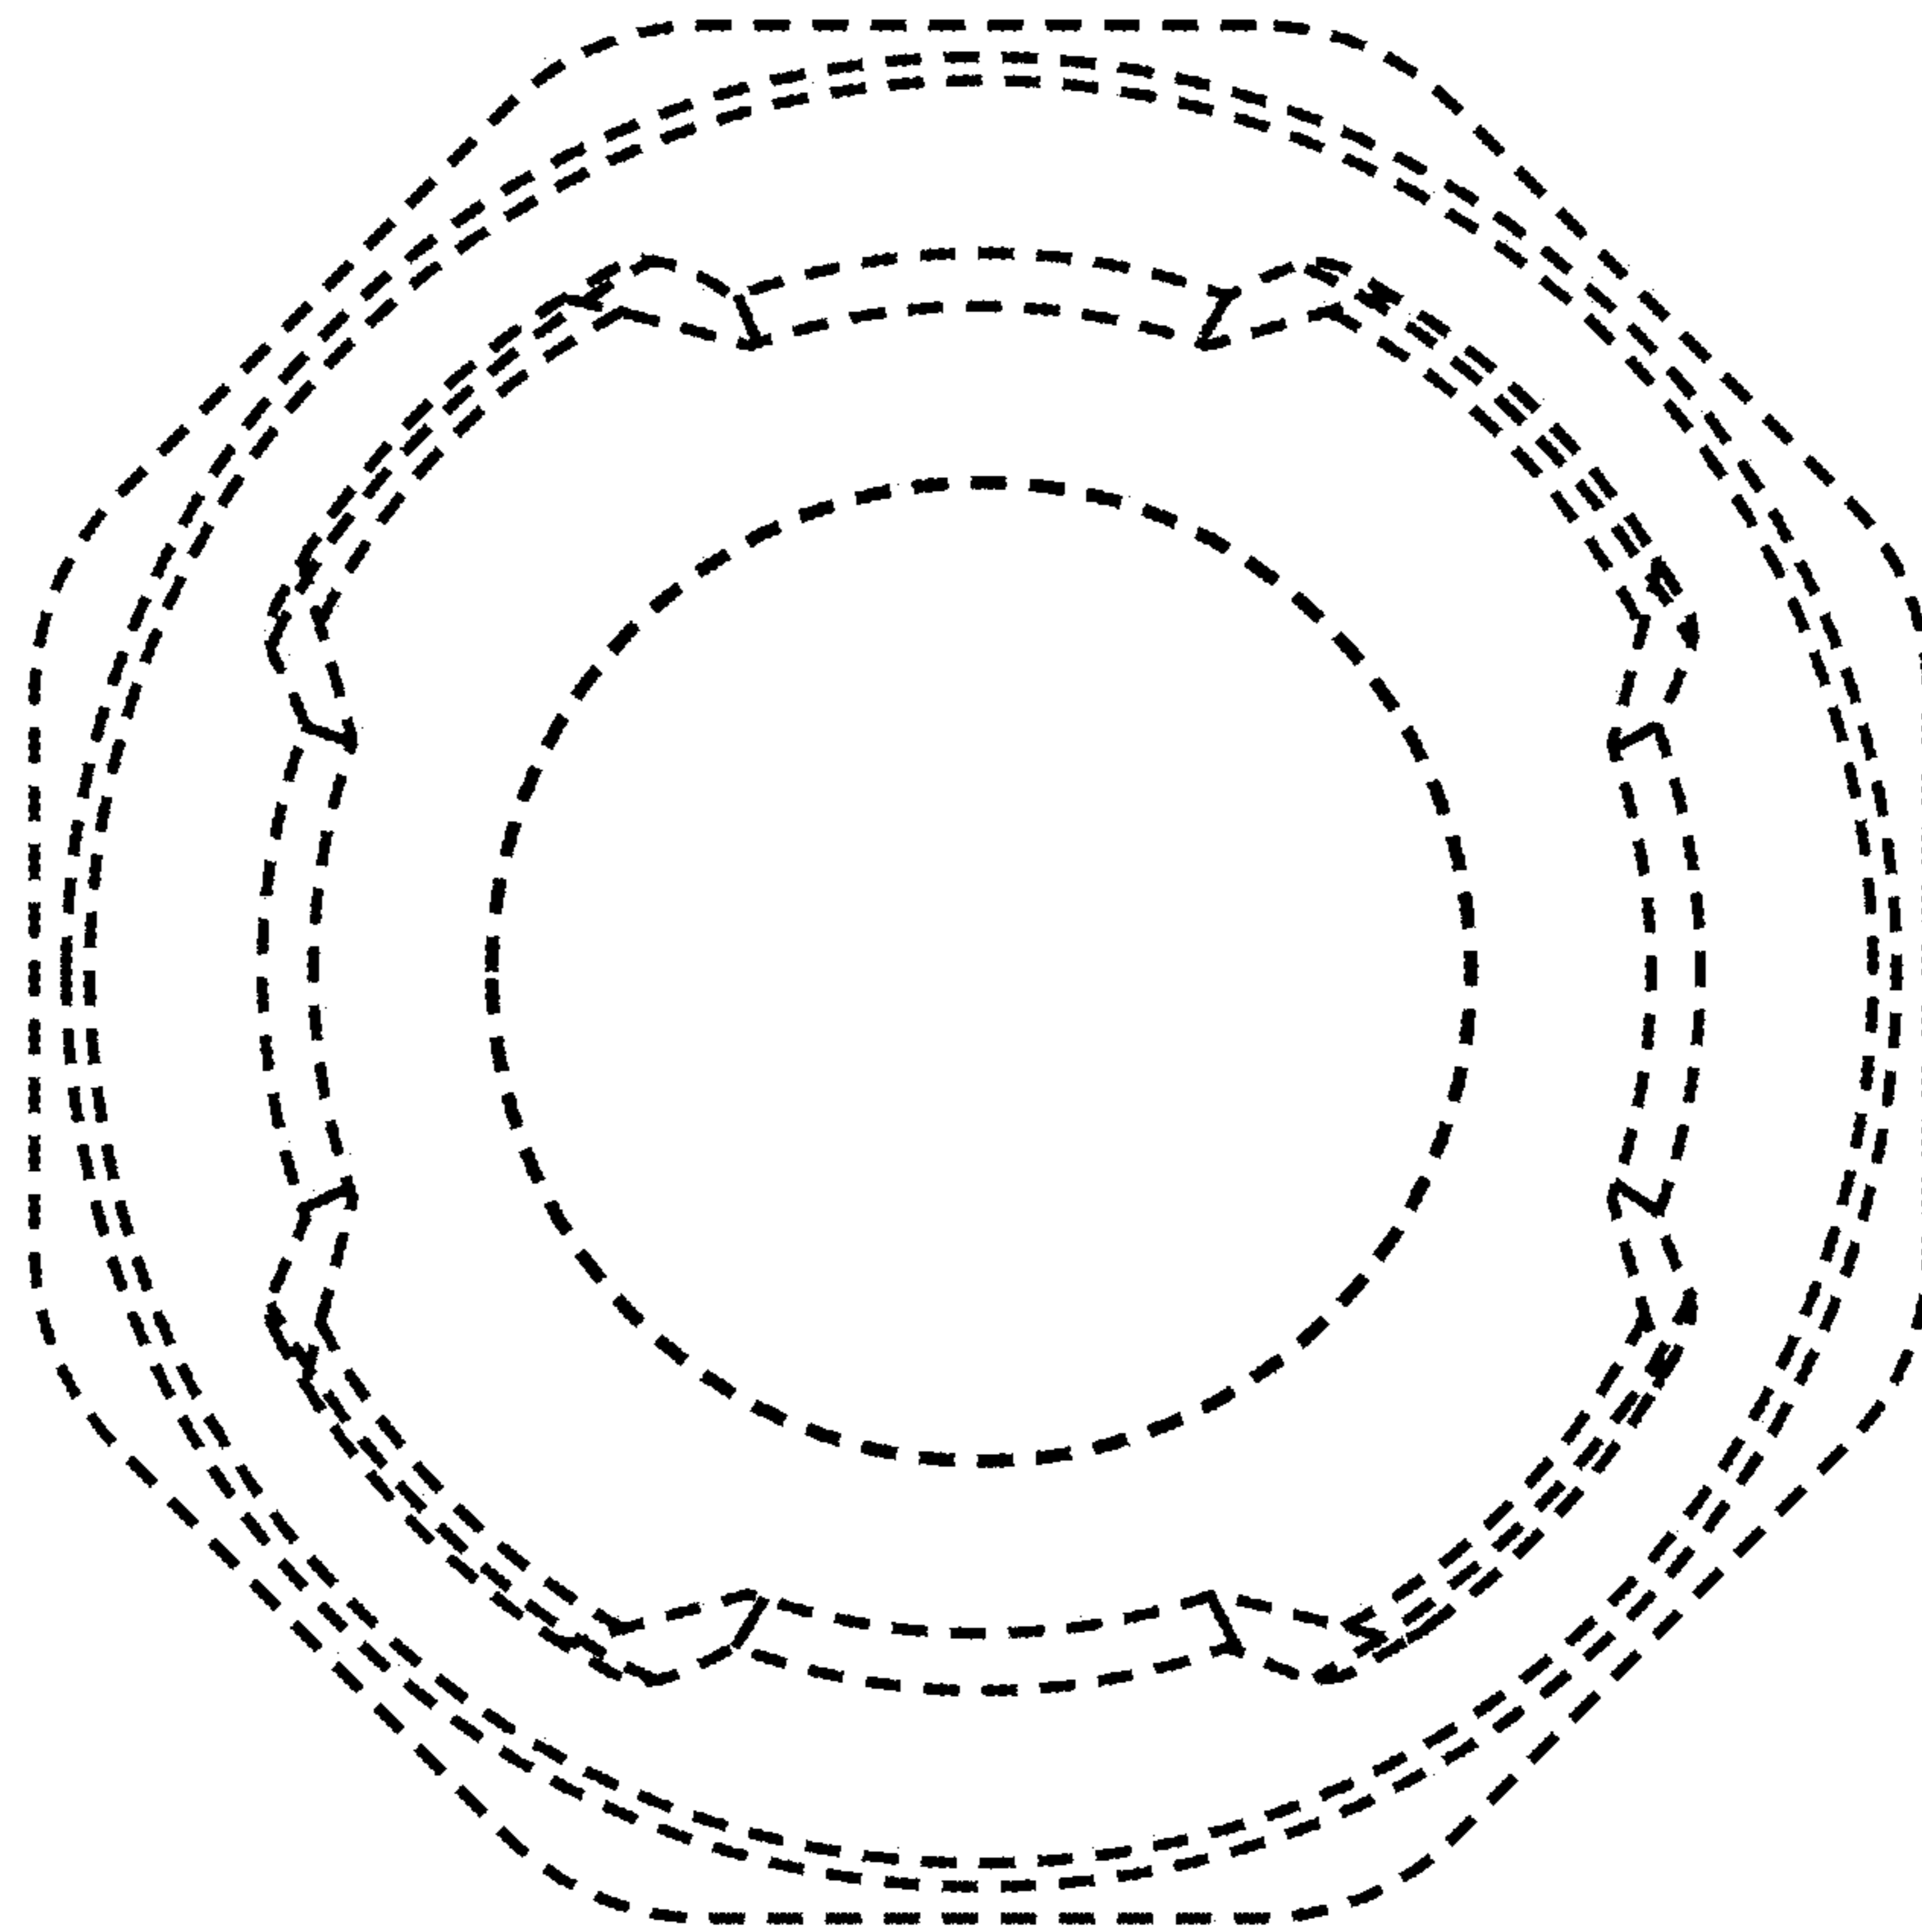


FIG. 2

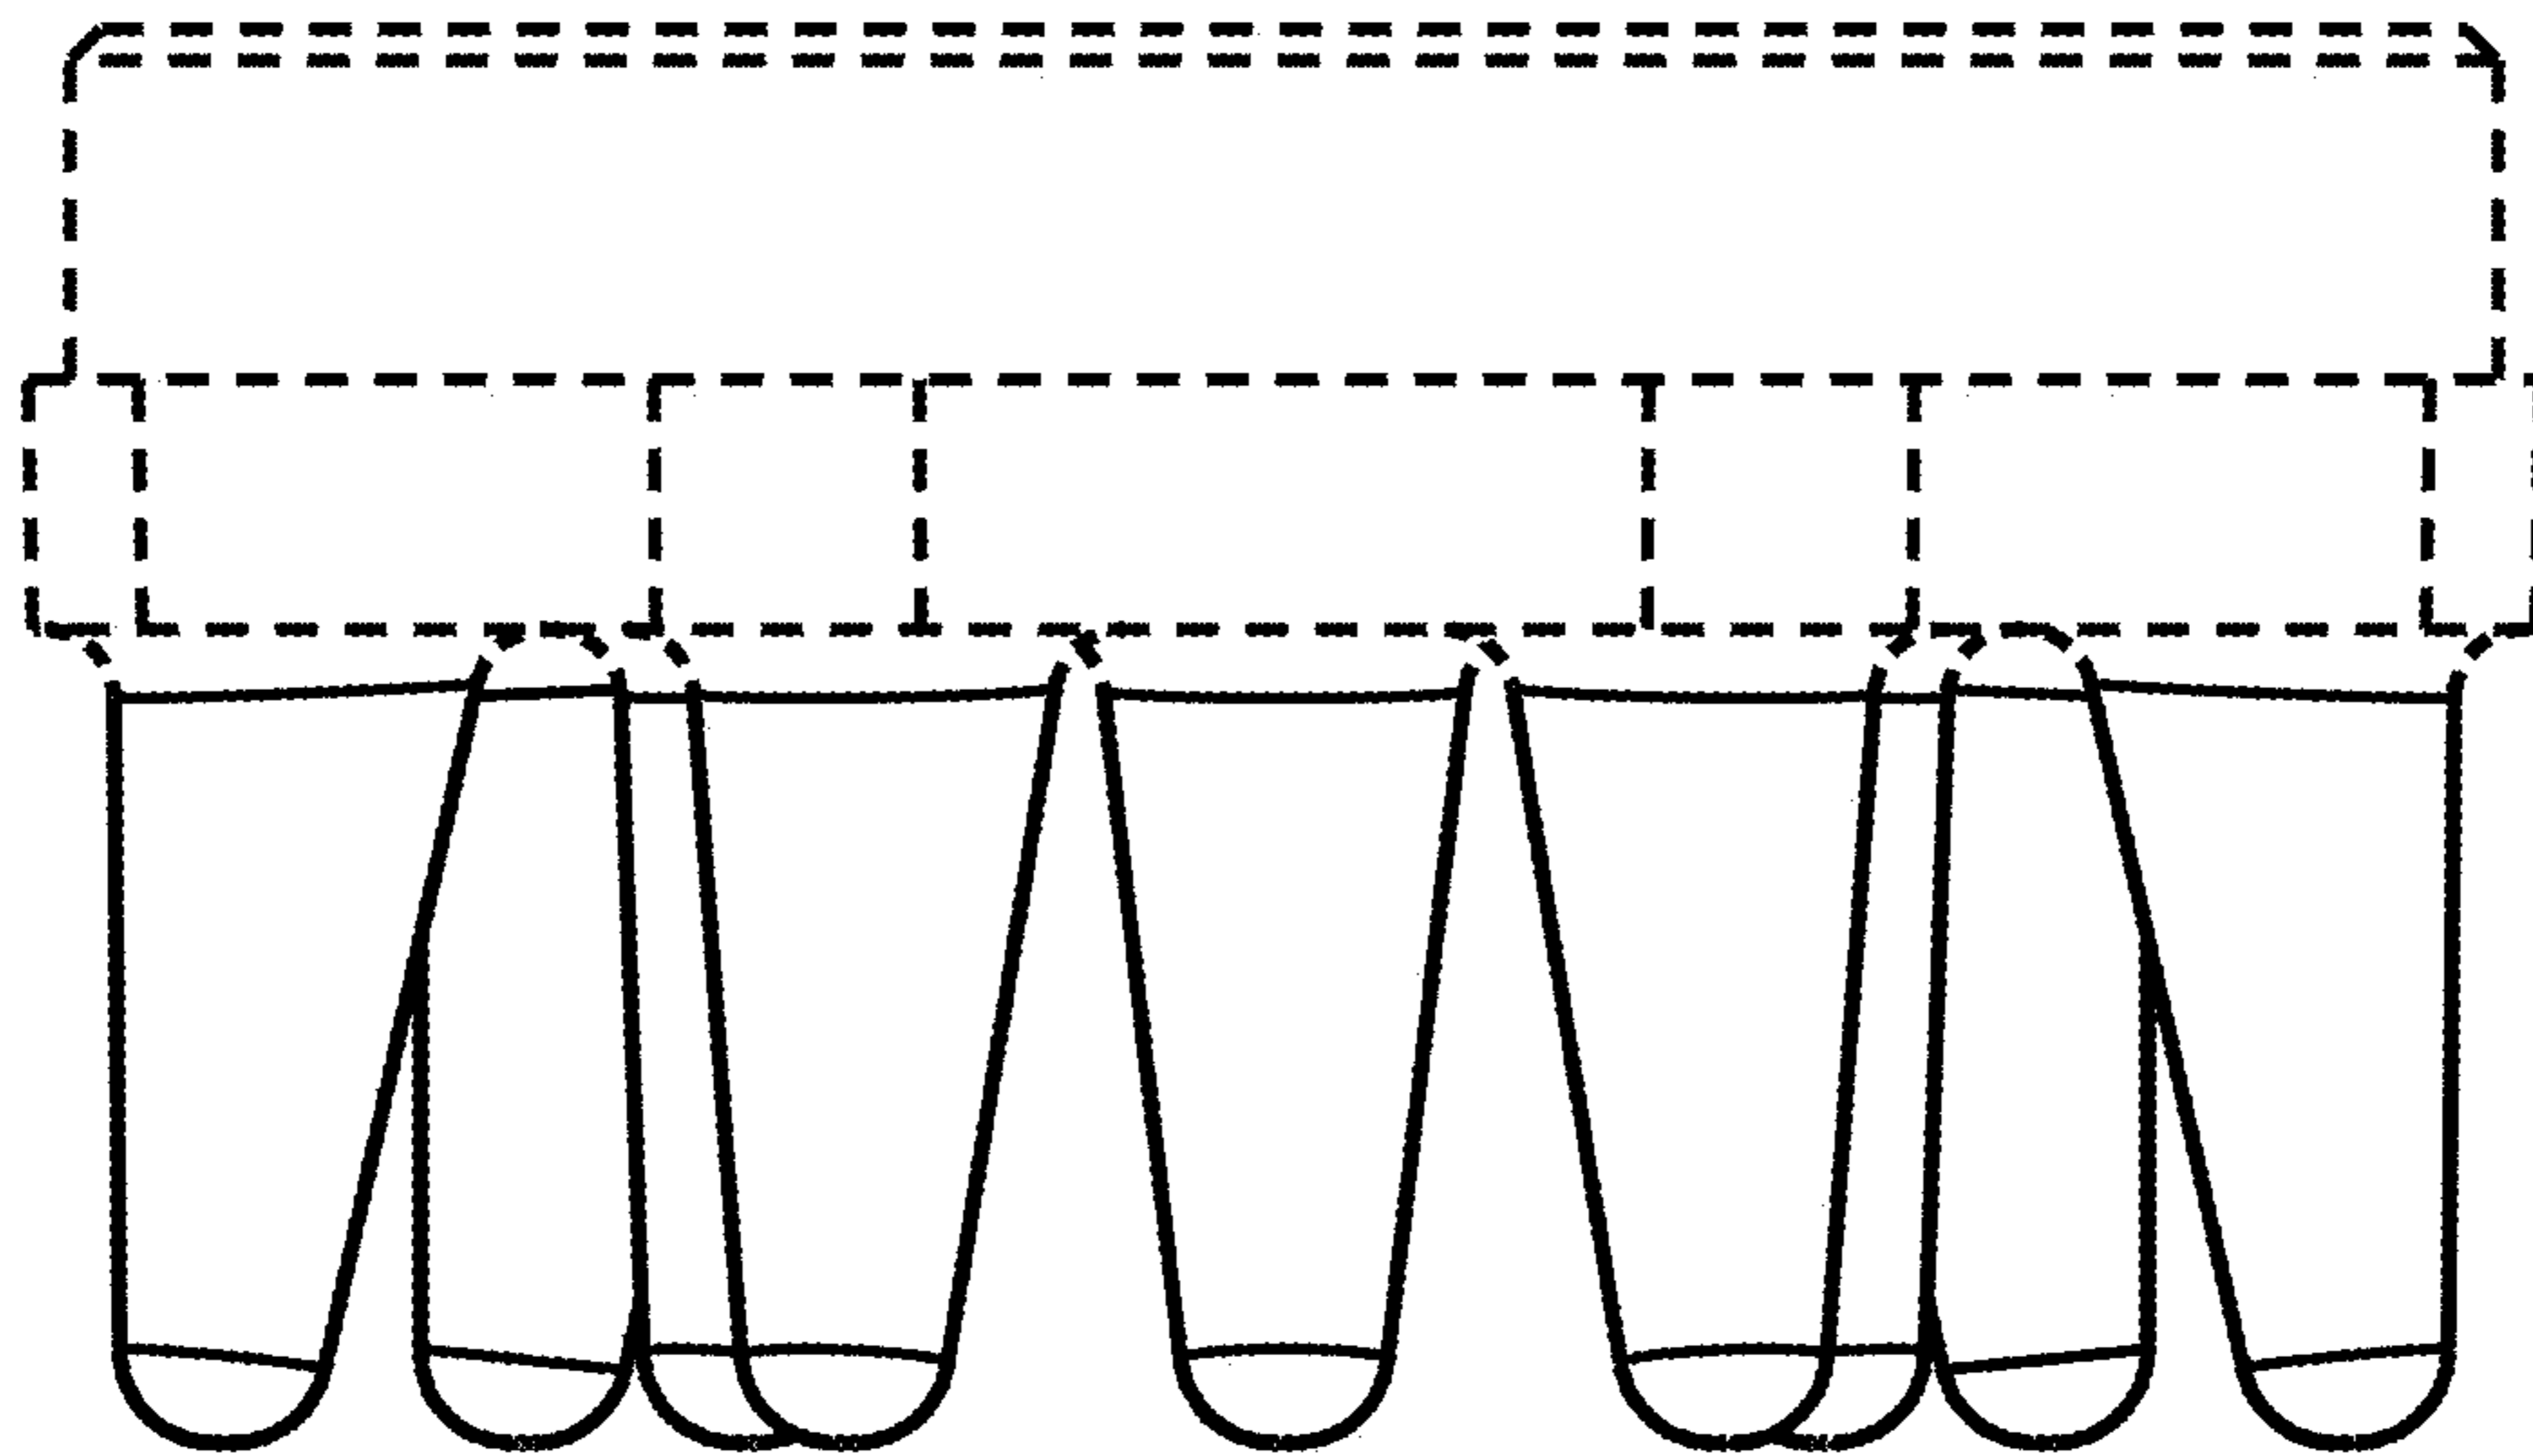


FIG. 3

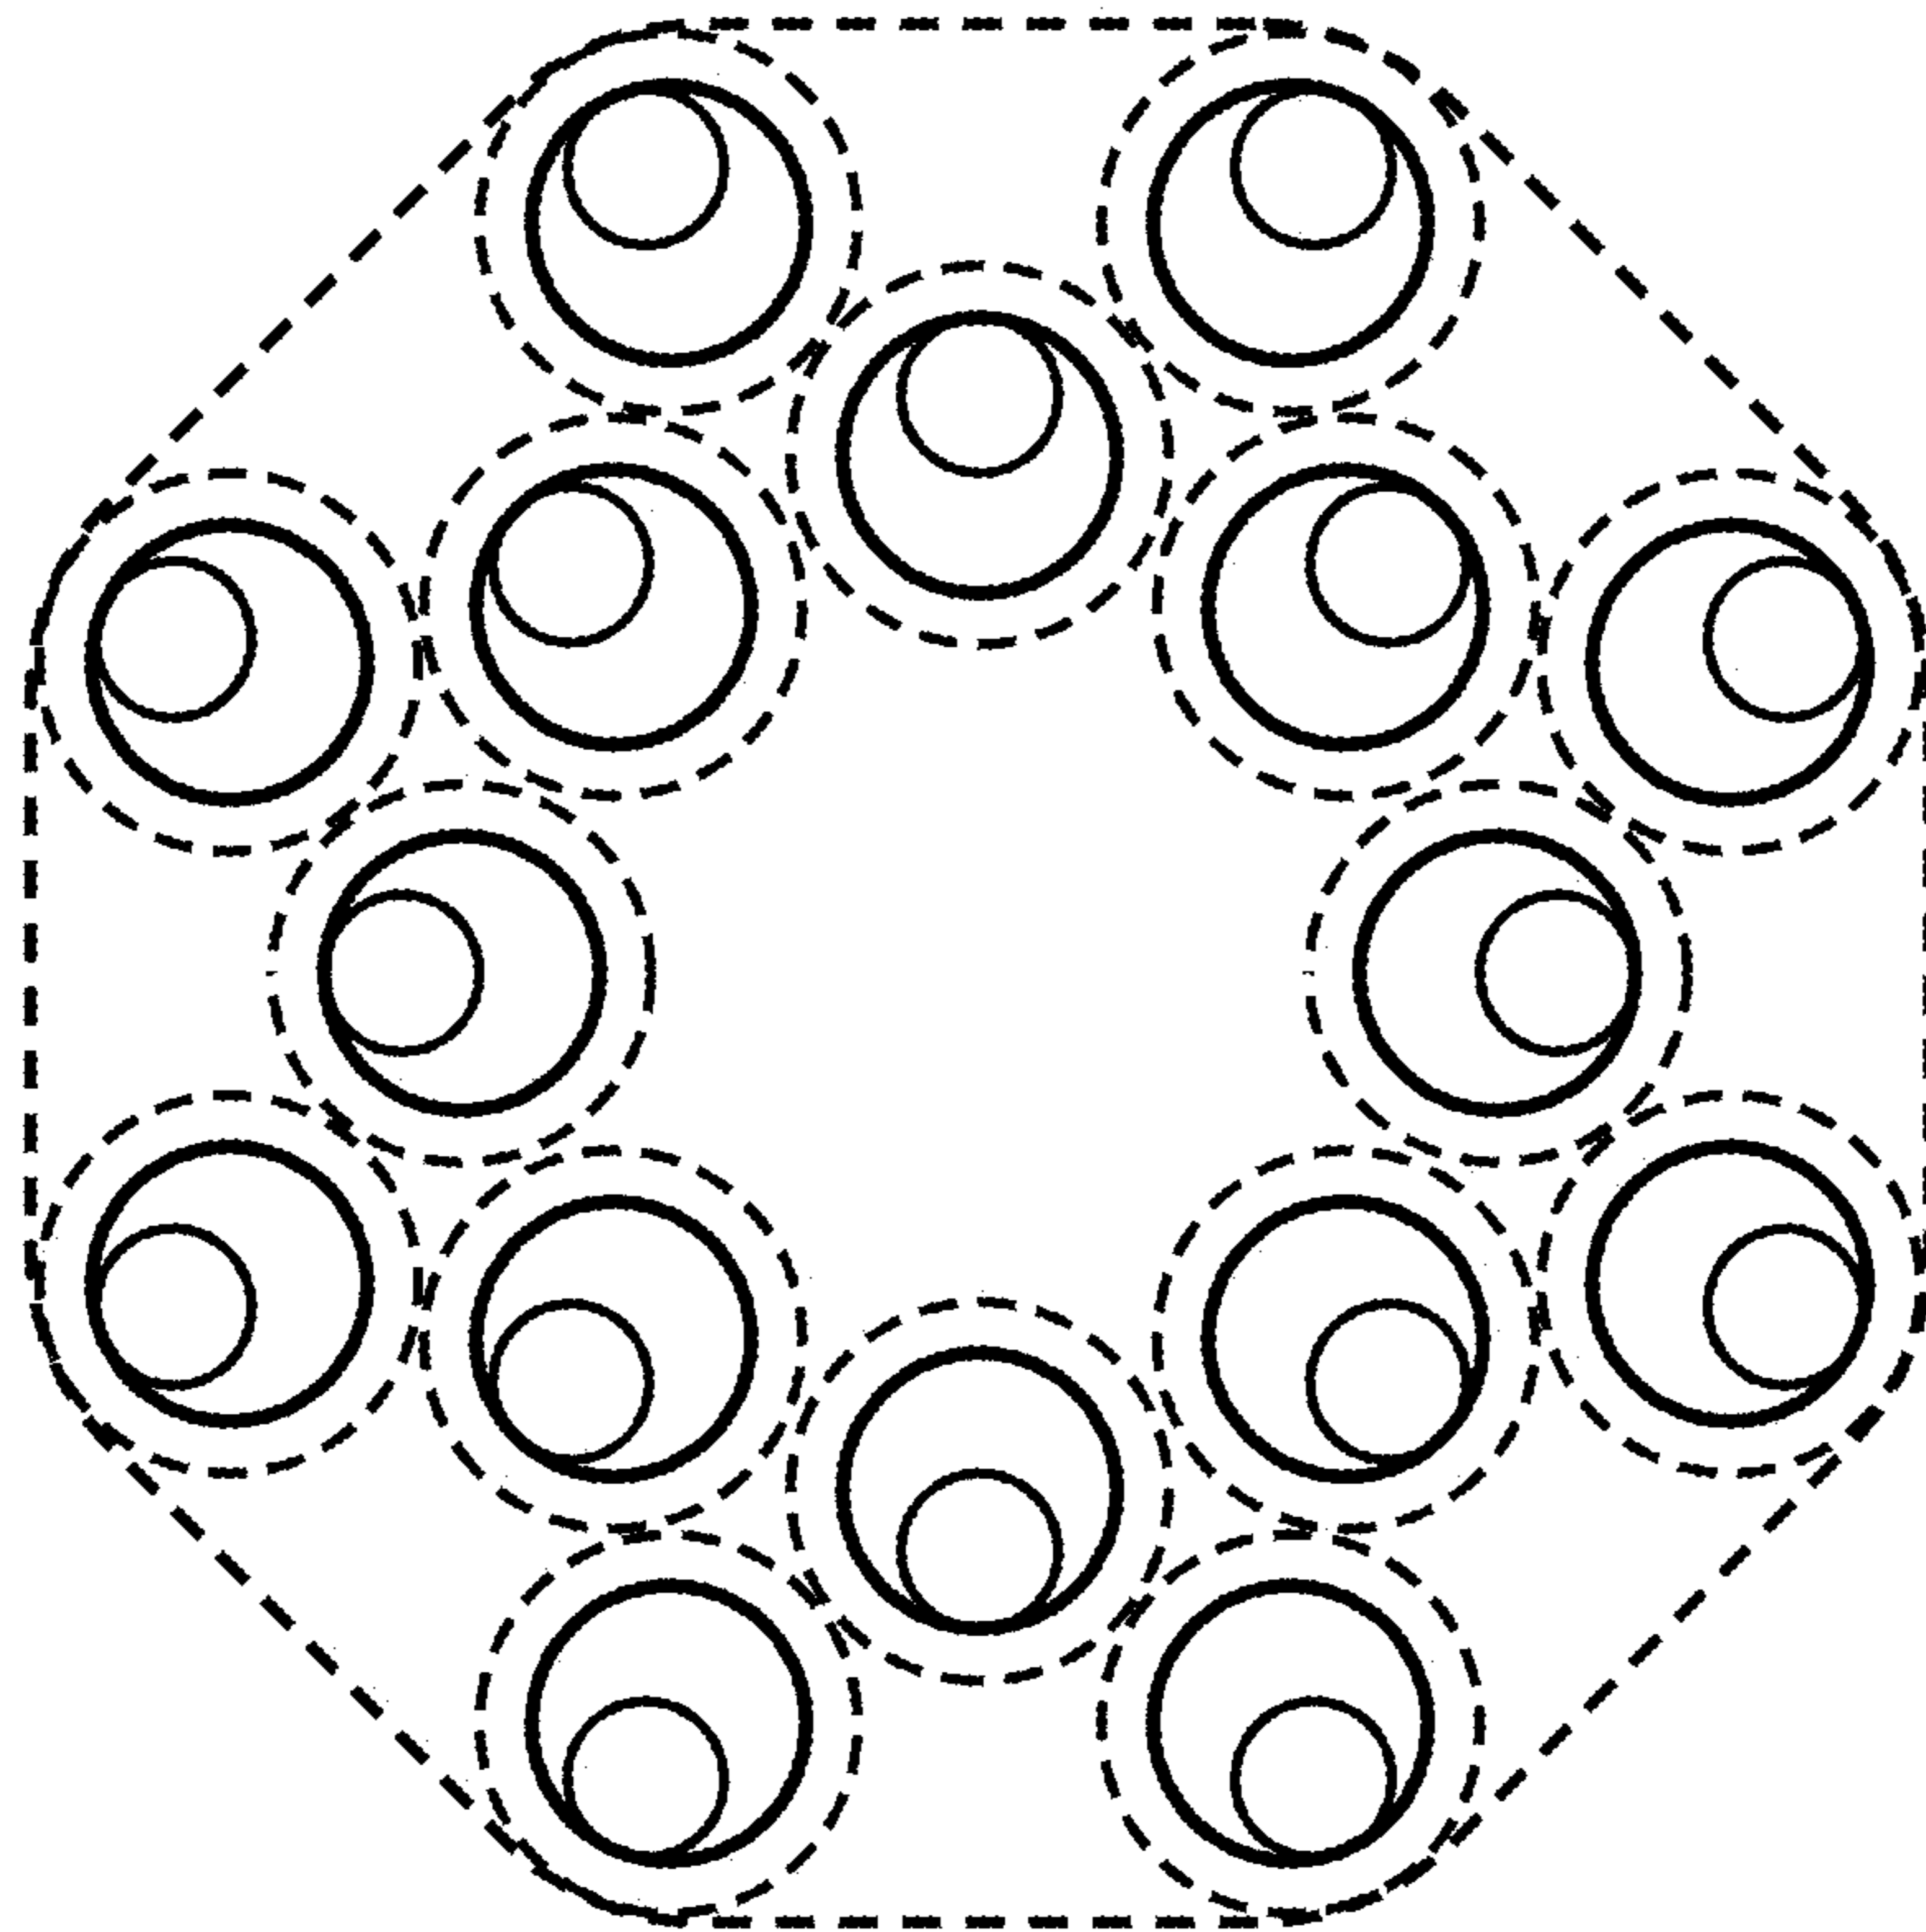


FIG. 4

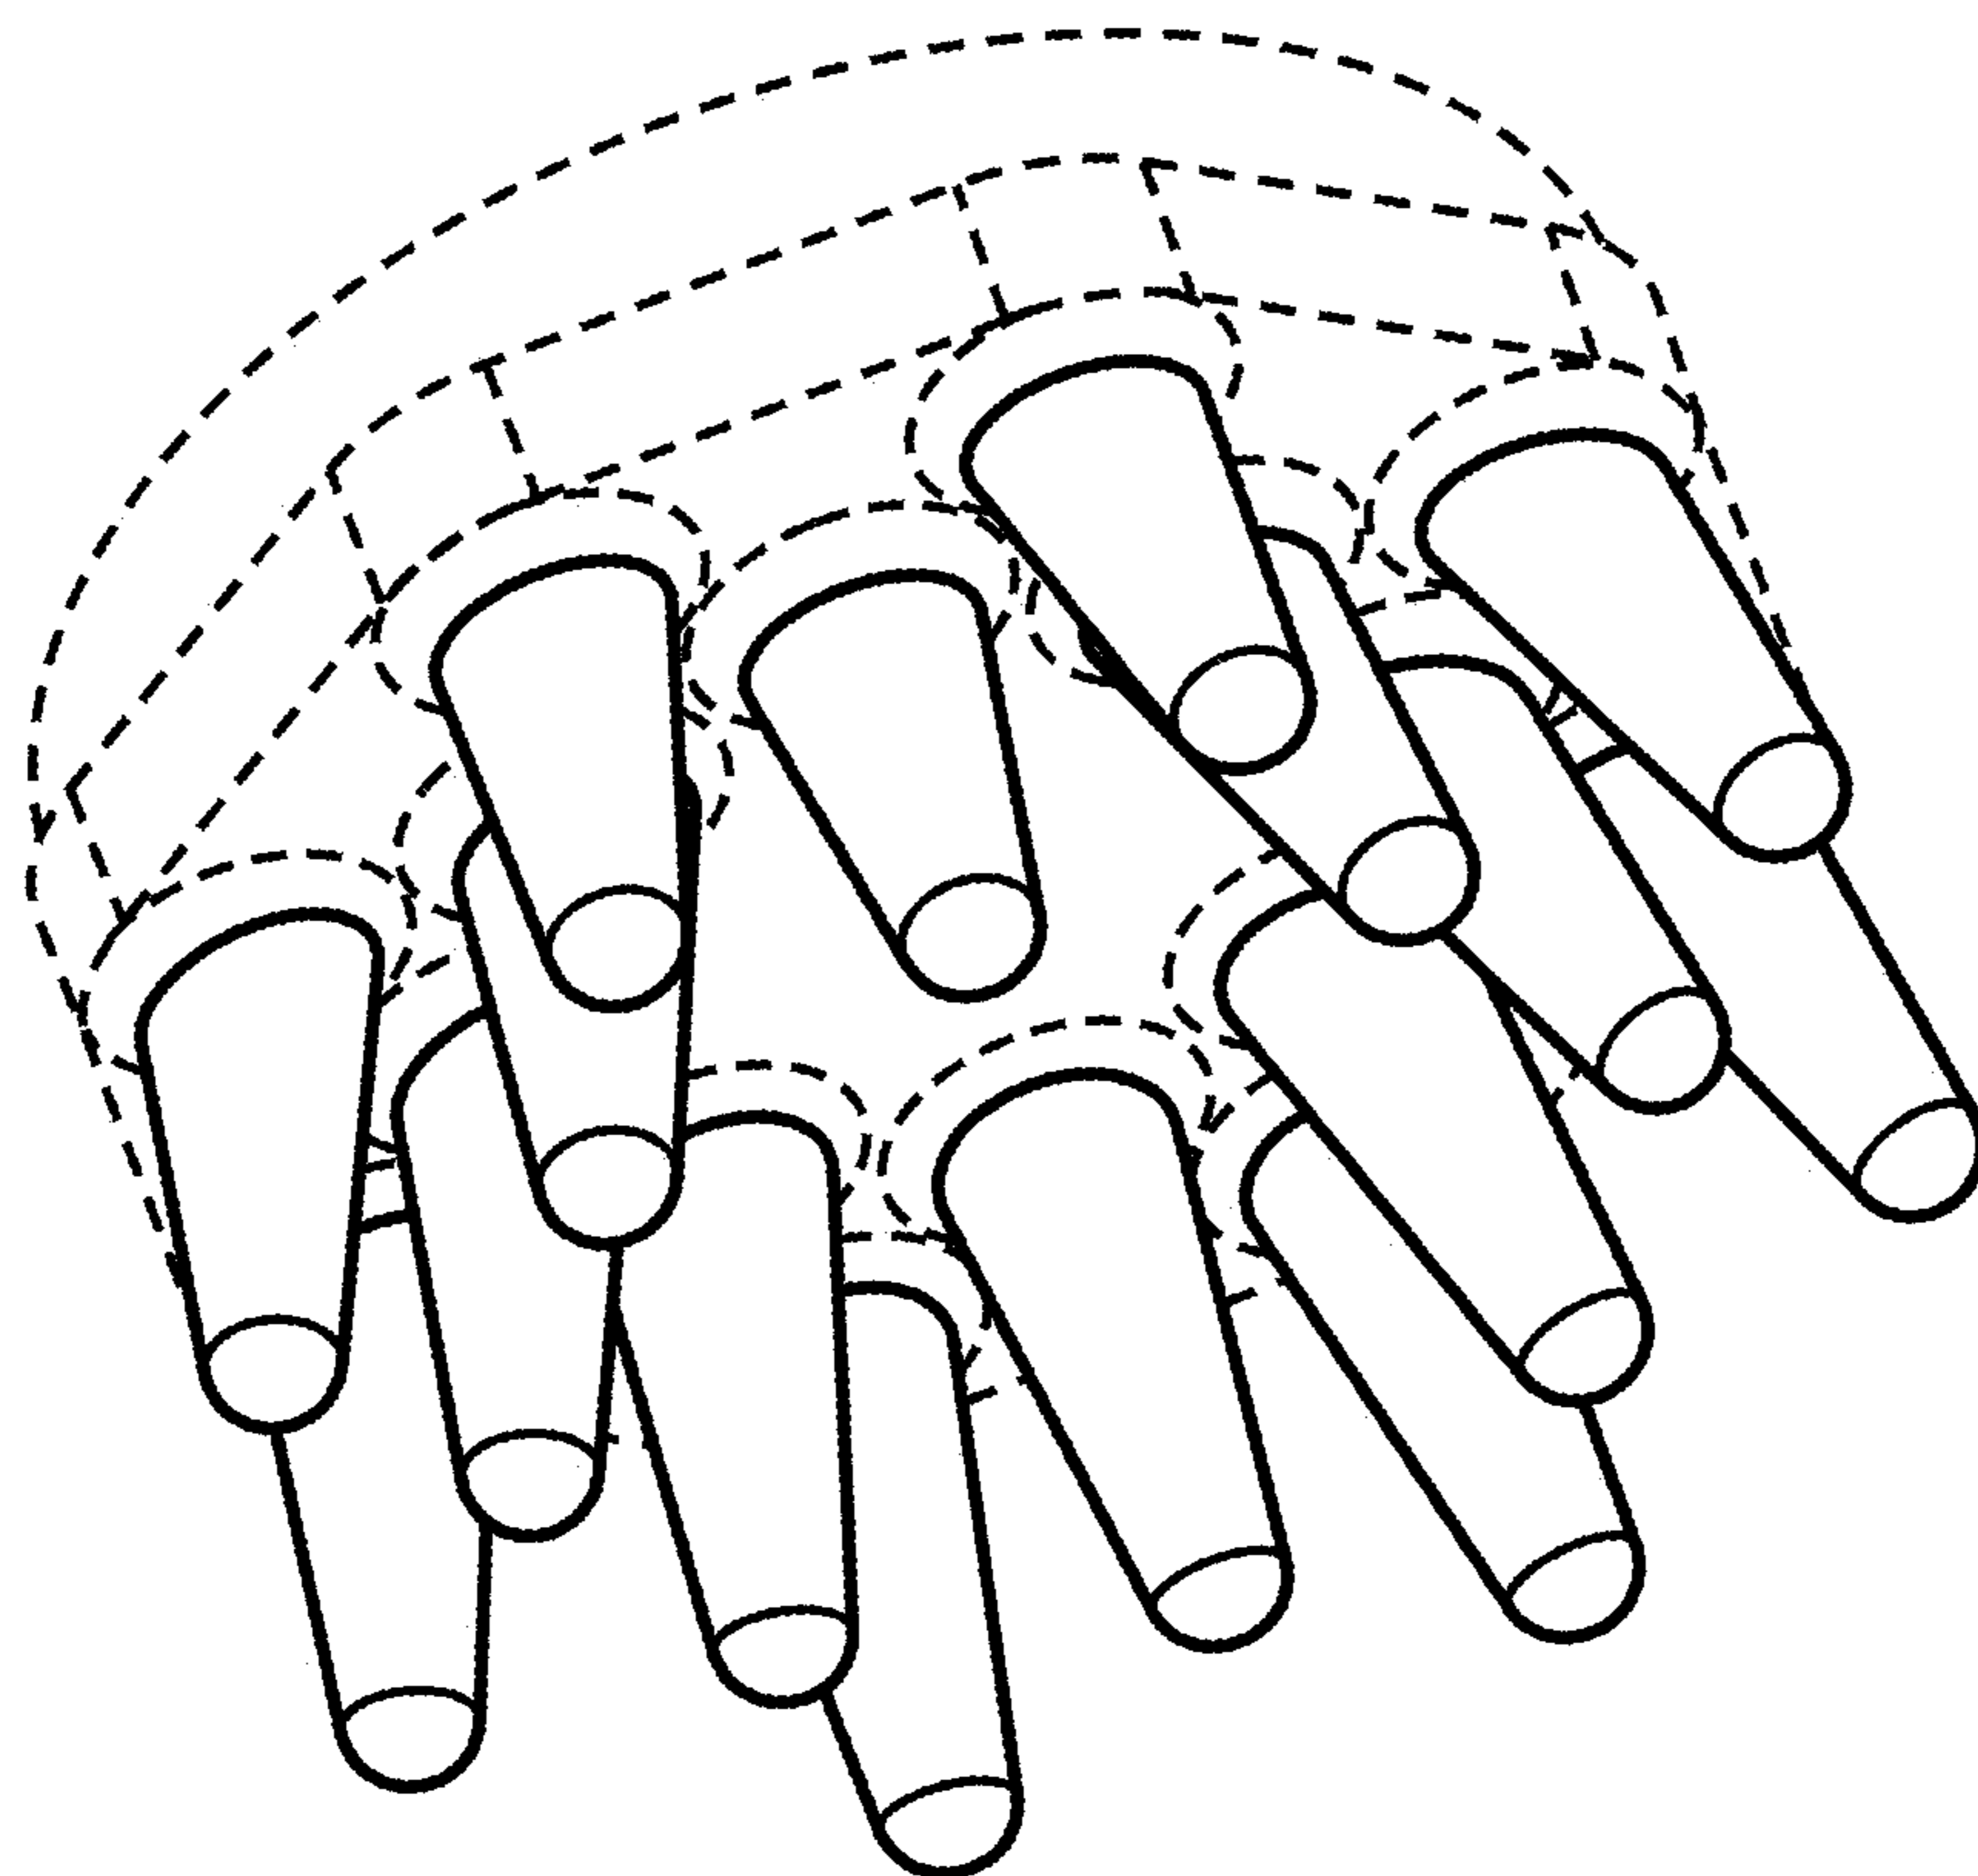


FIG. 5

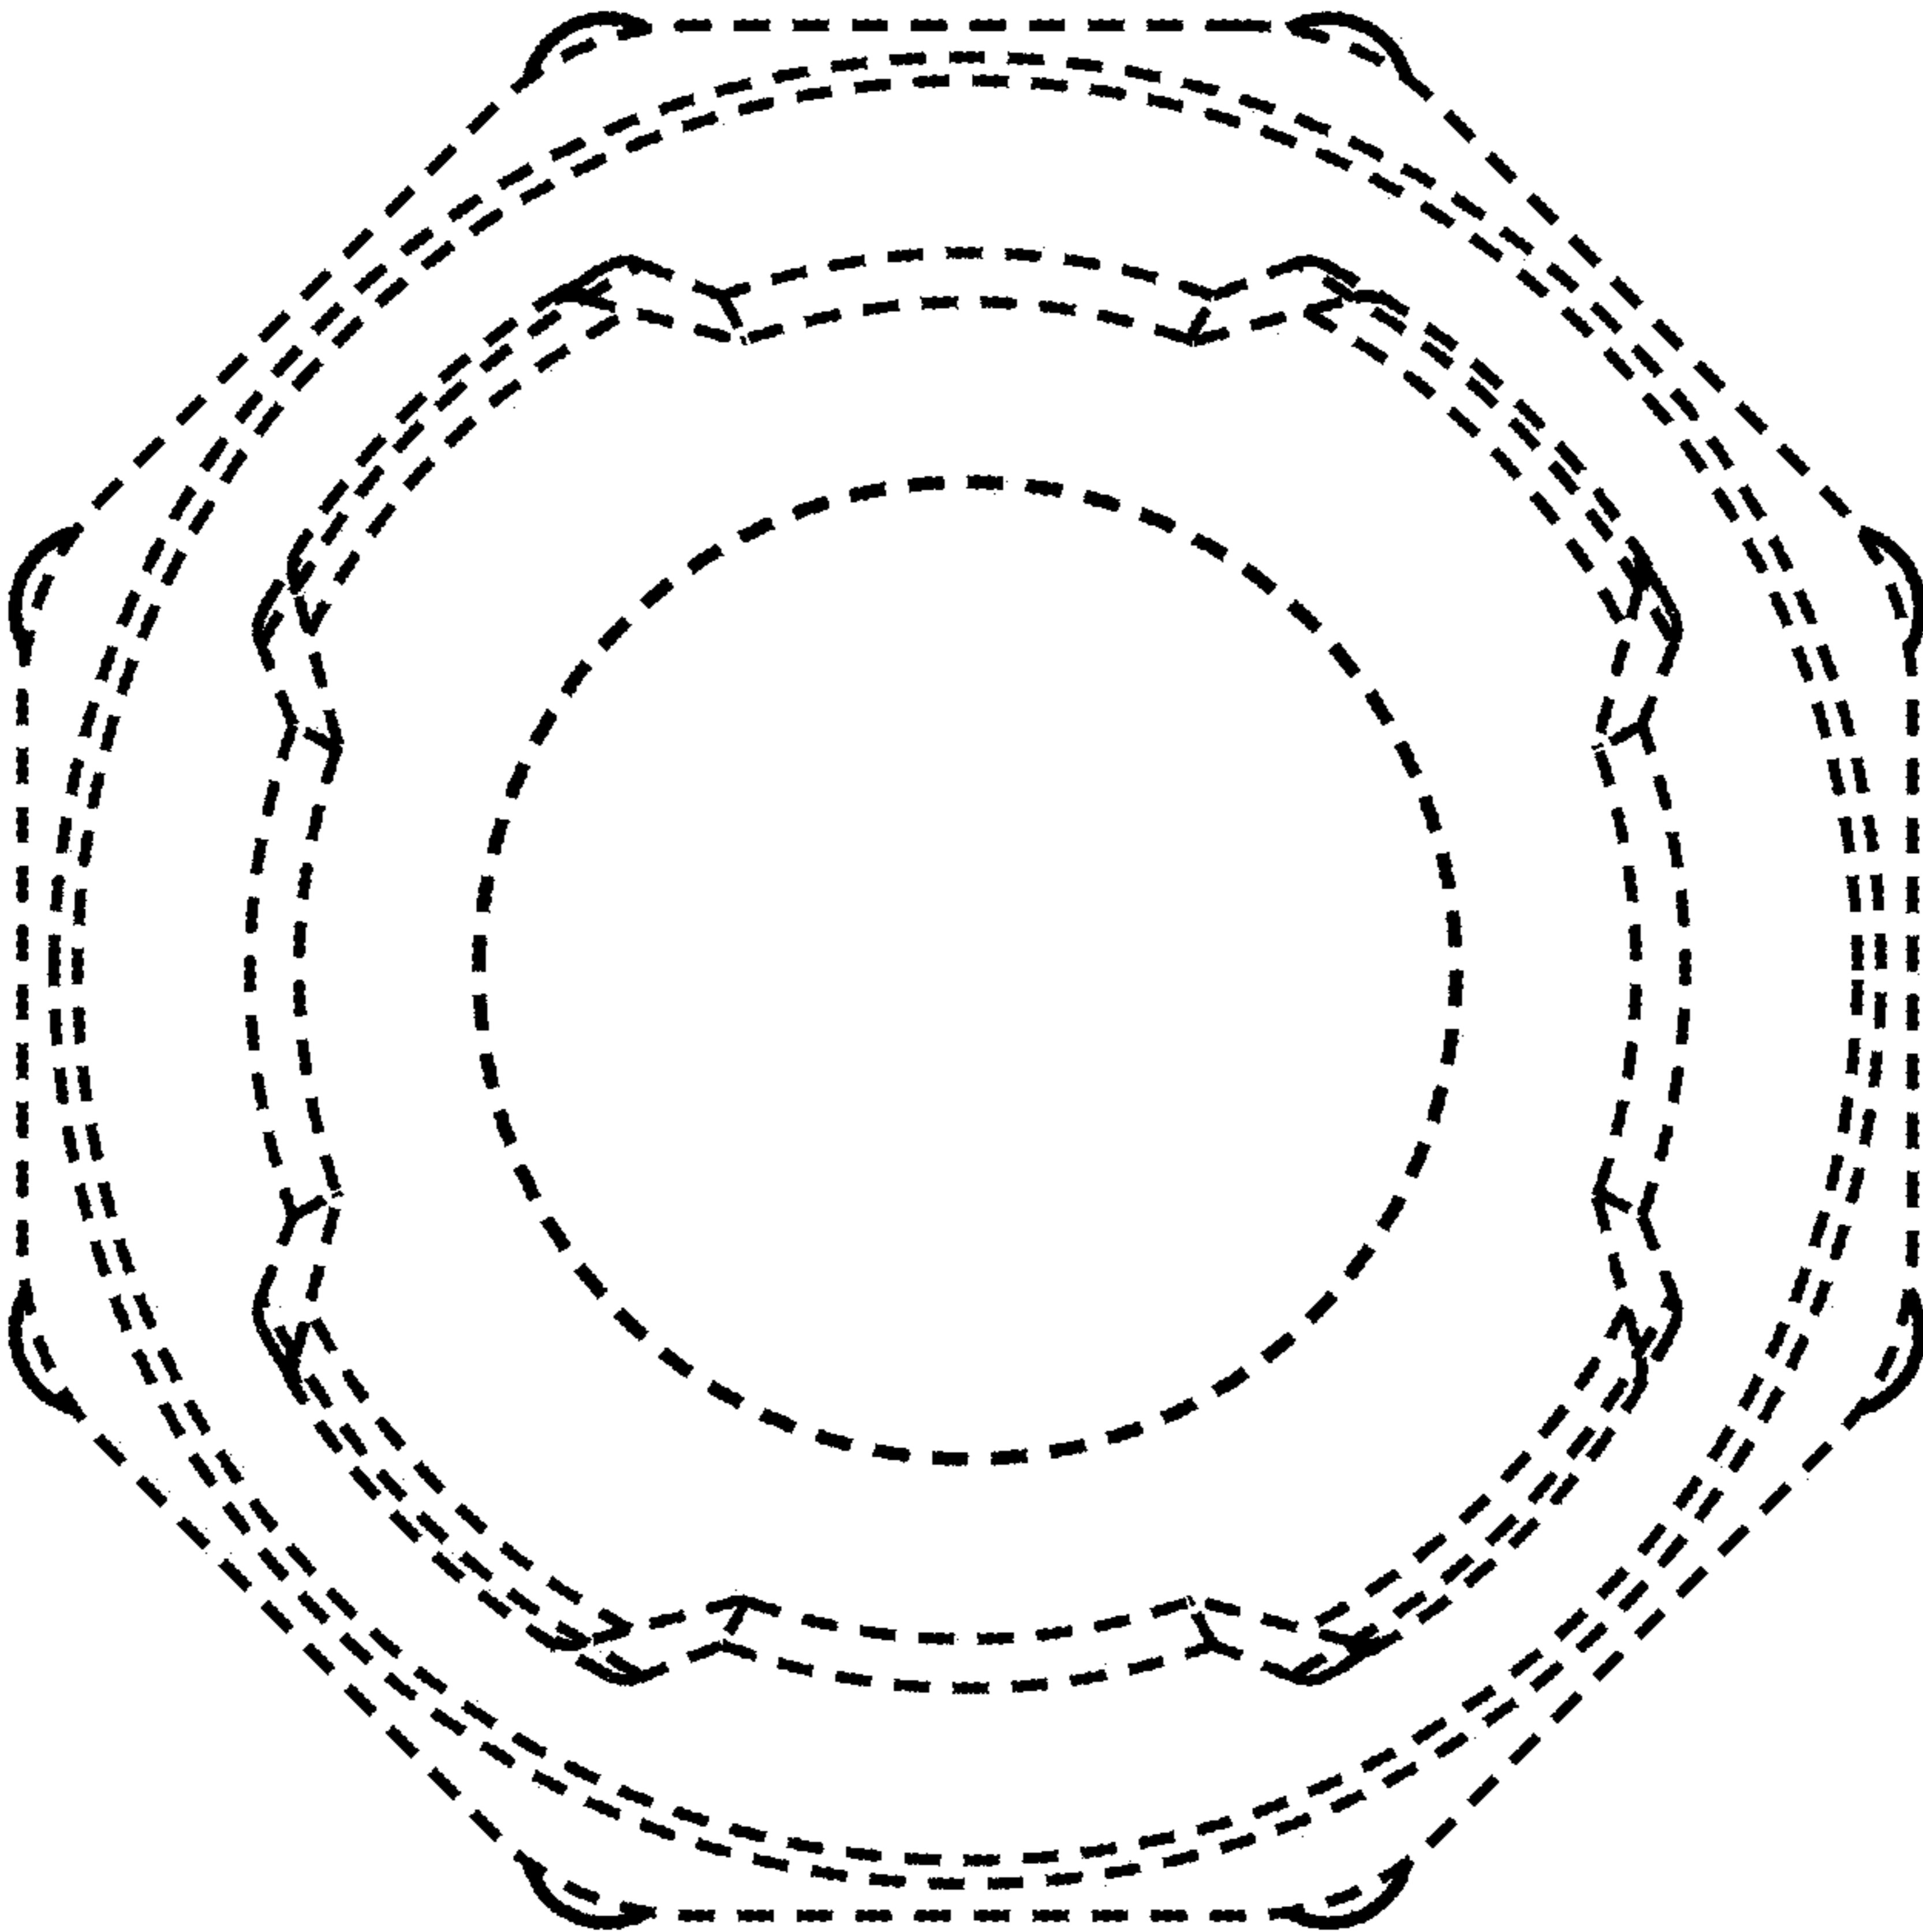


FIG. 6



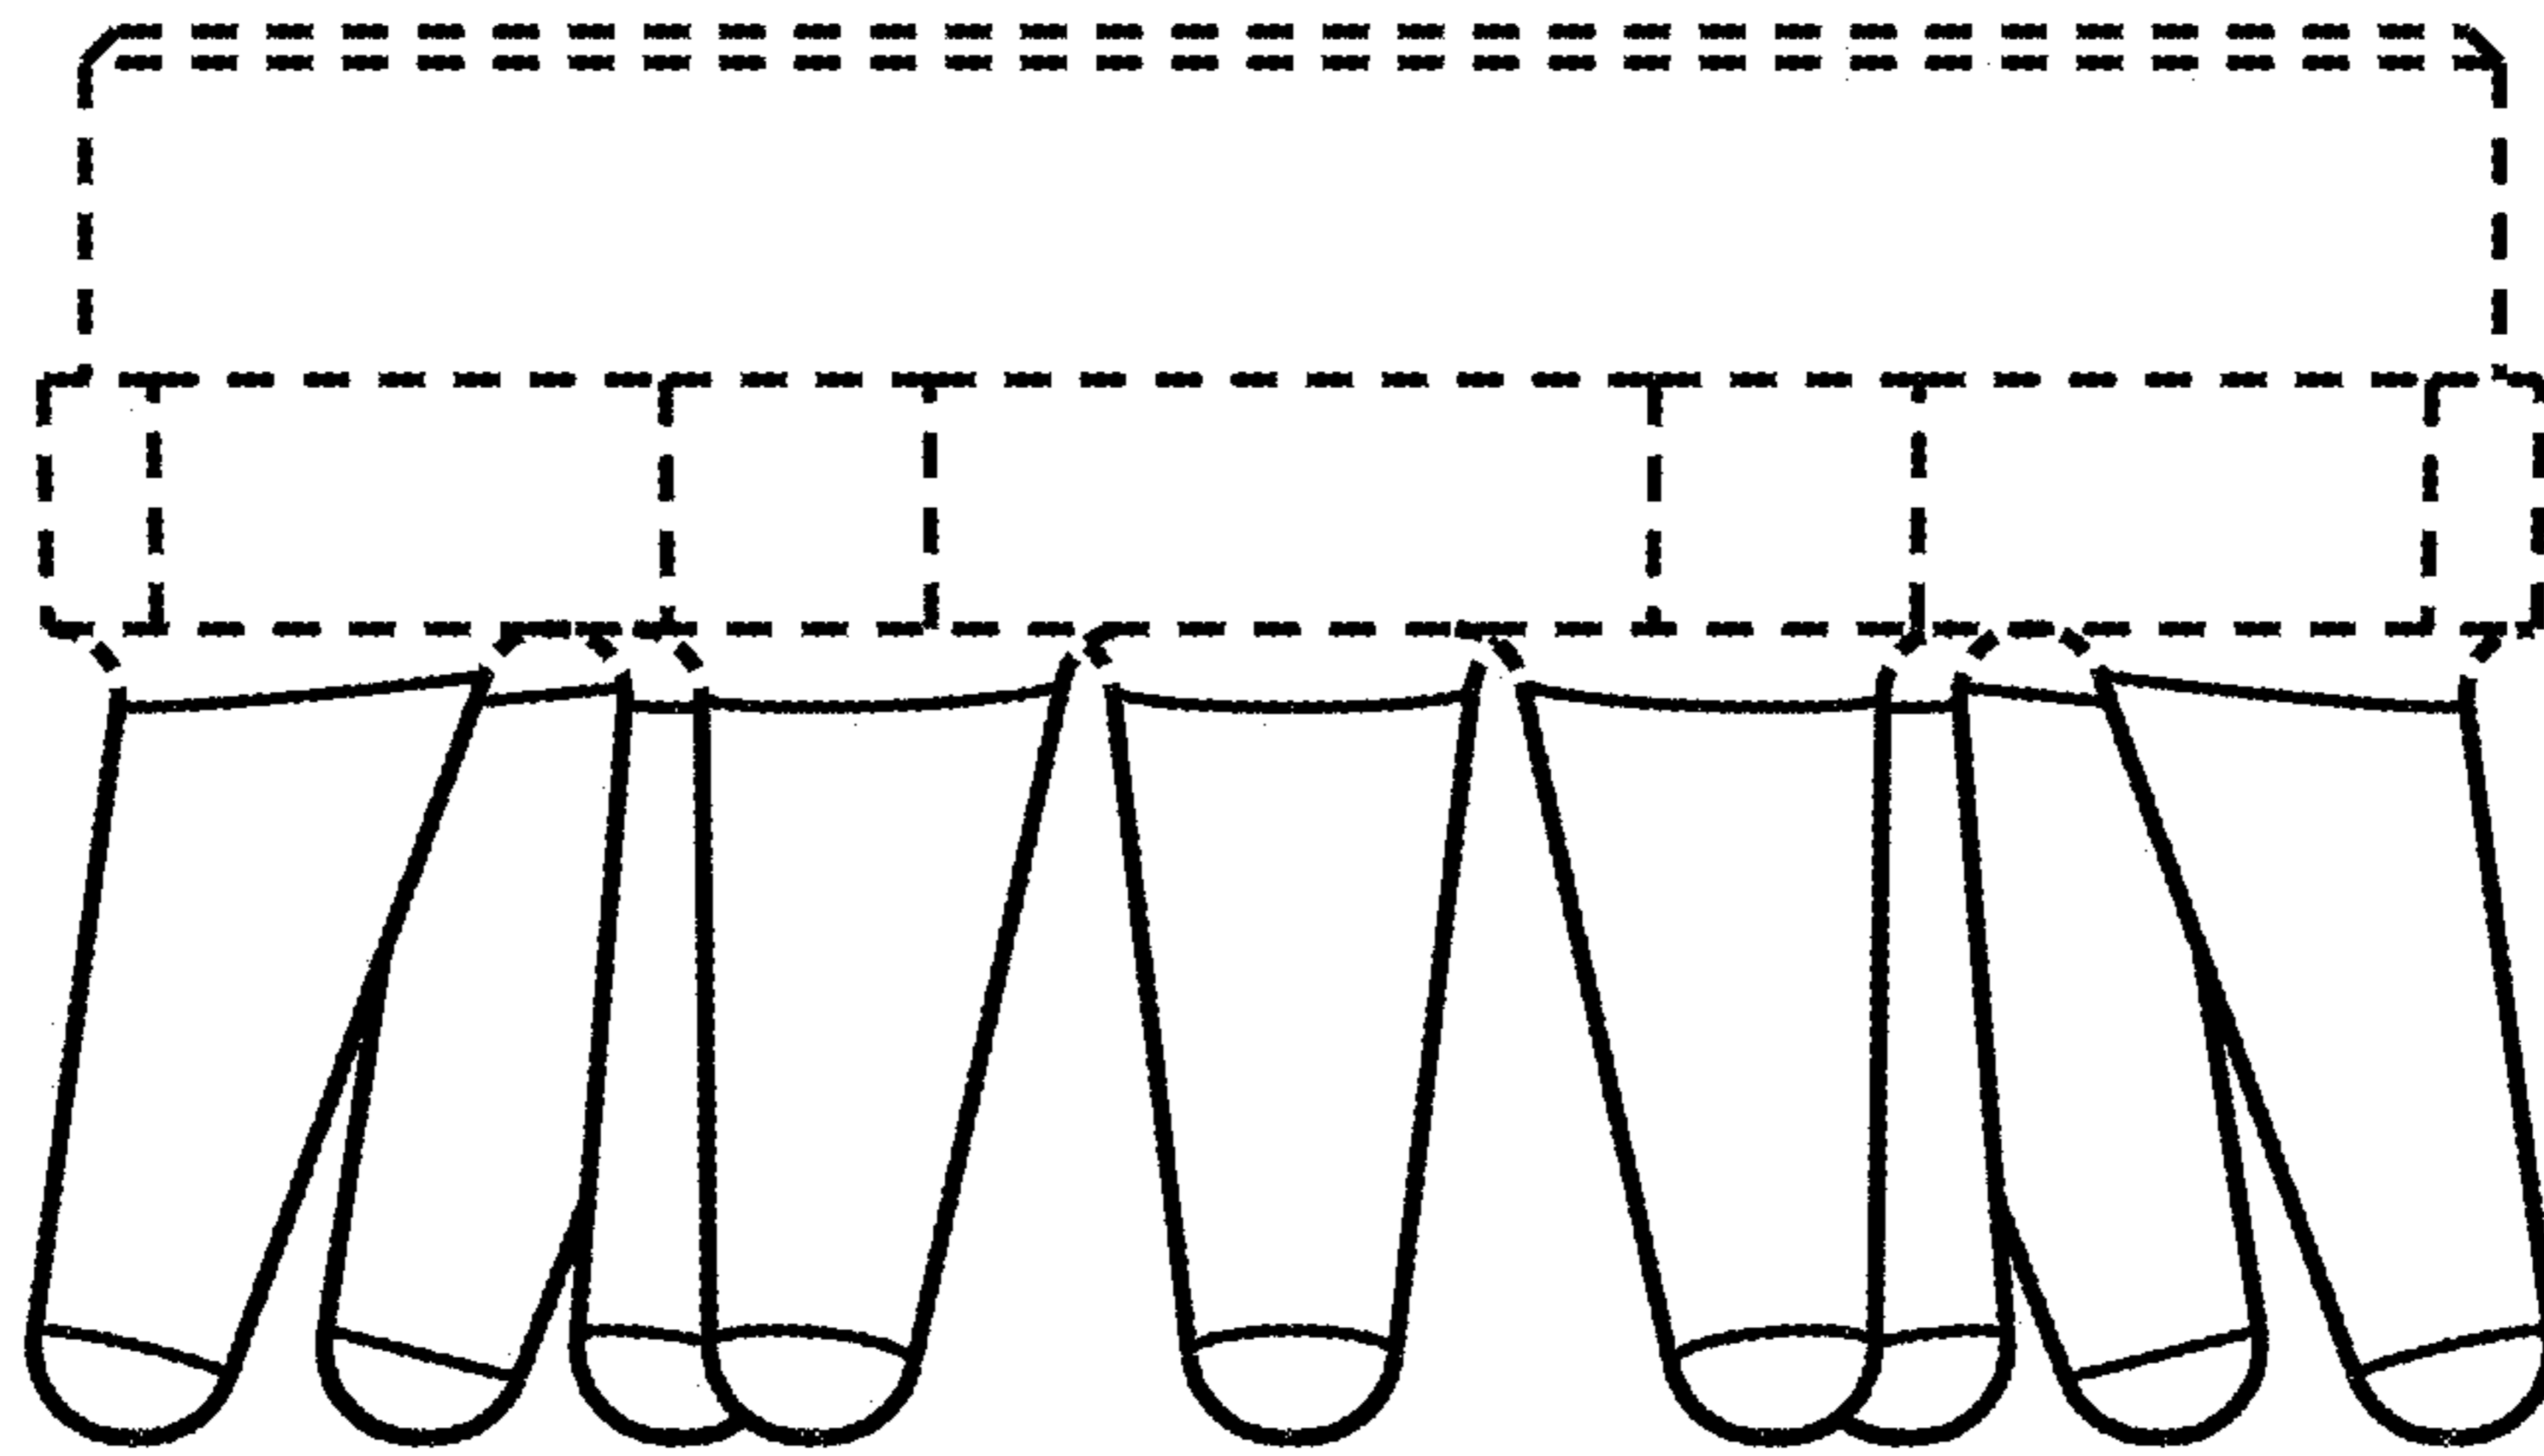


FIG. 7

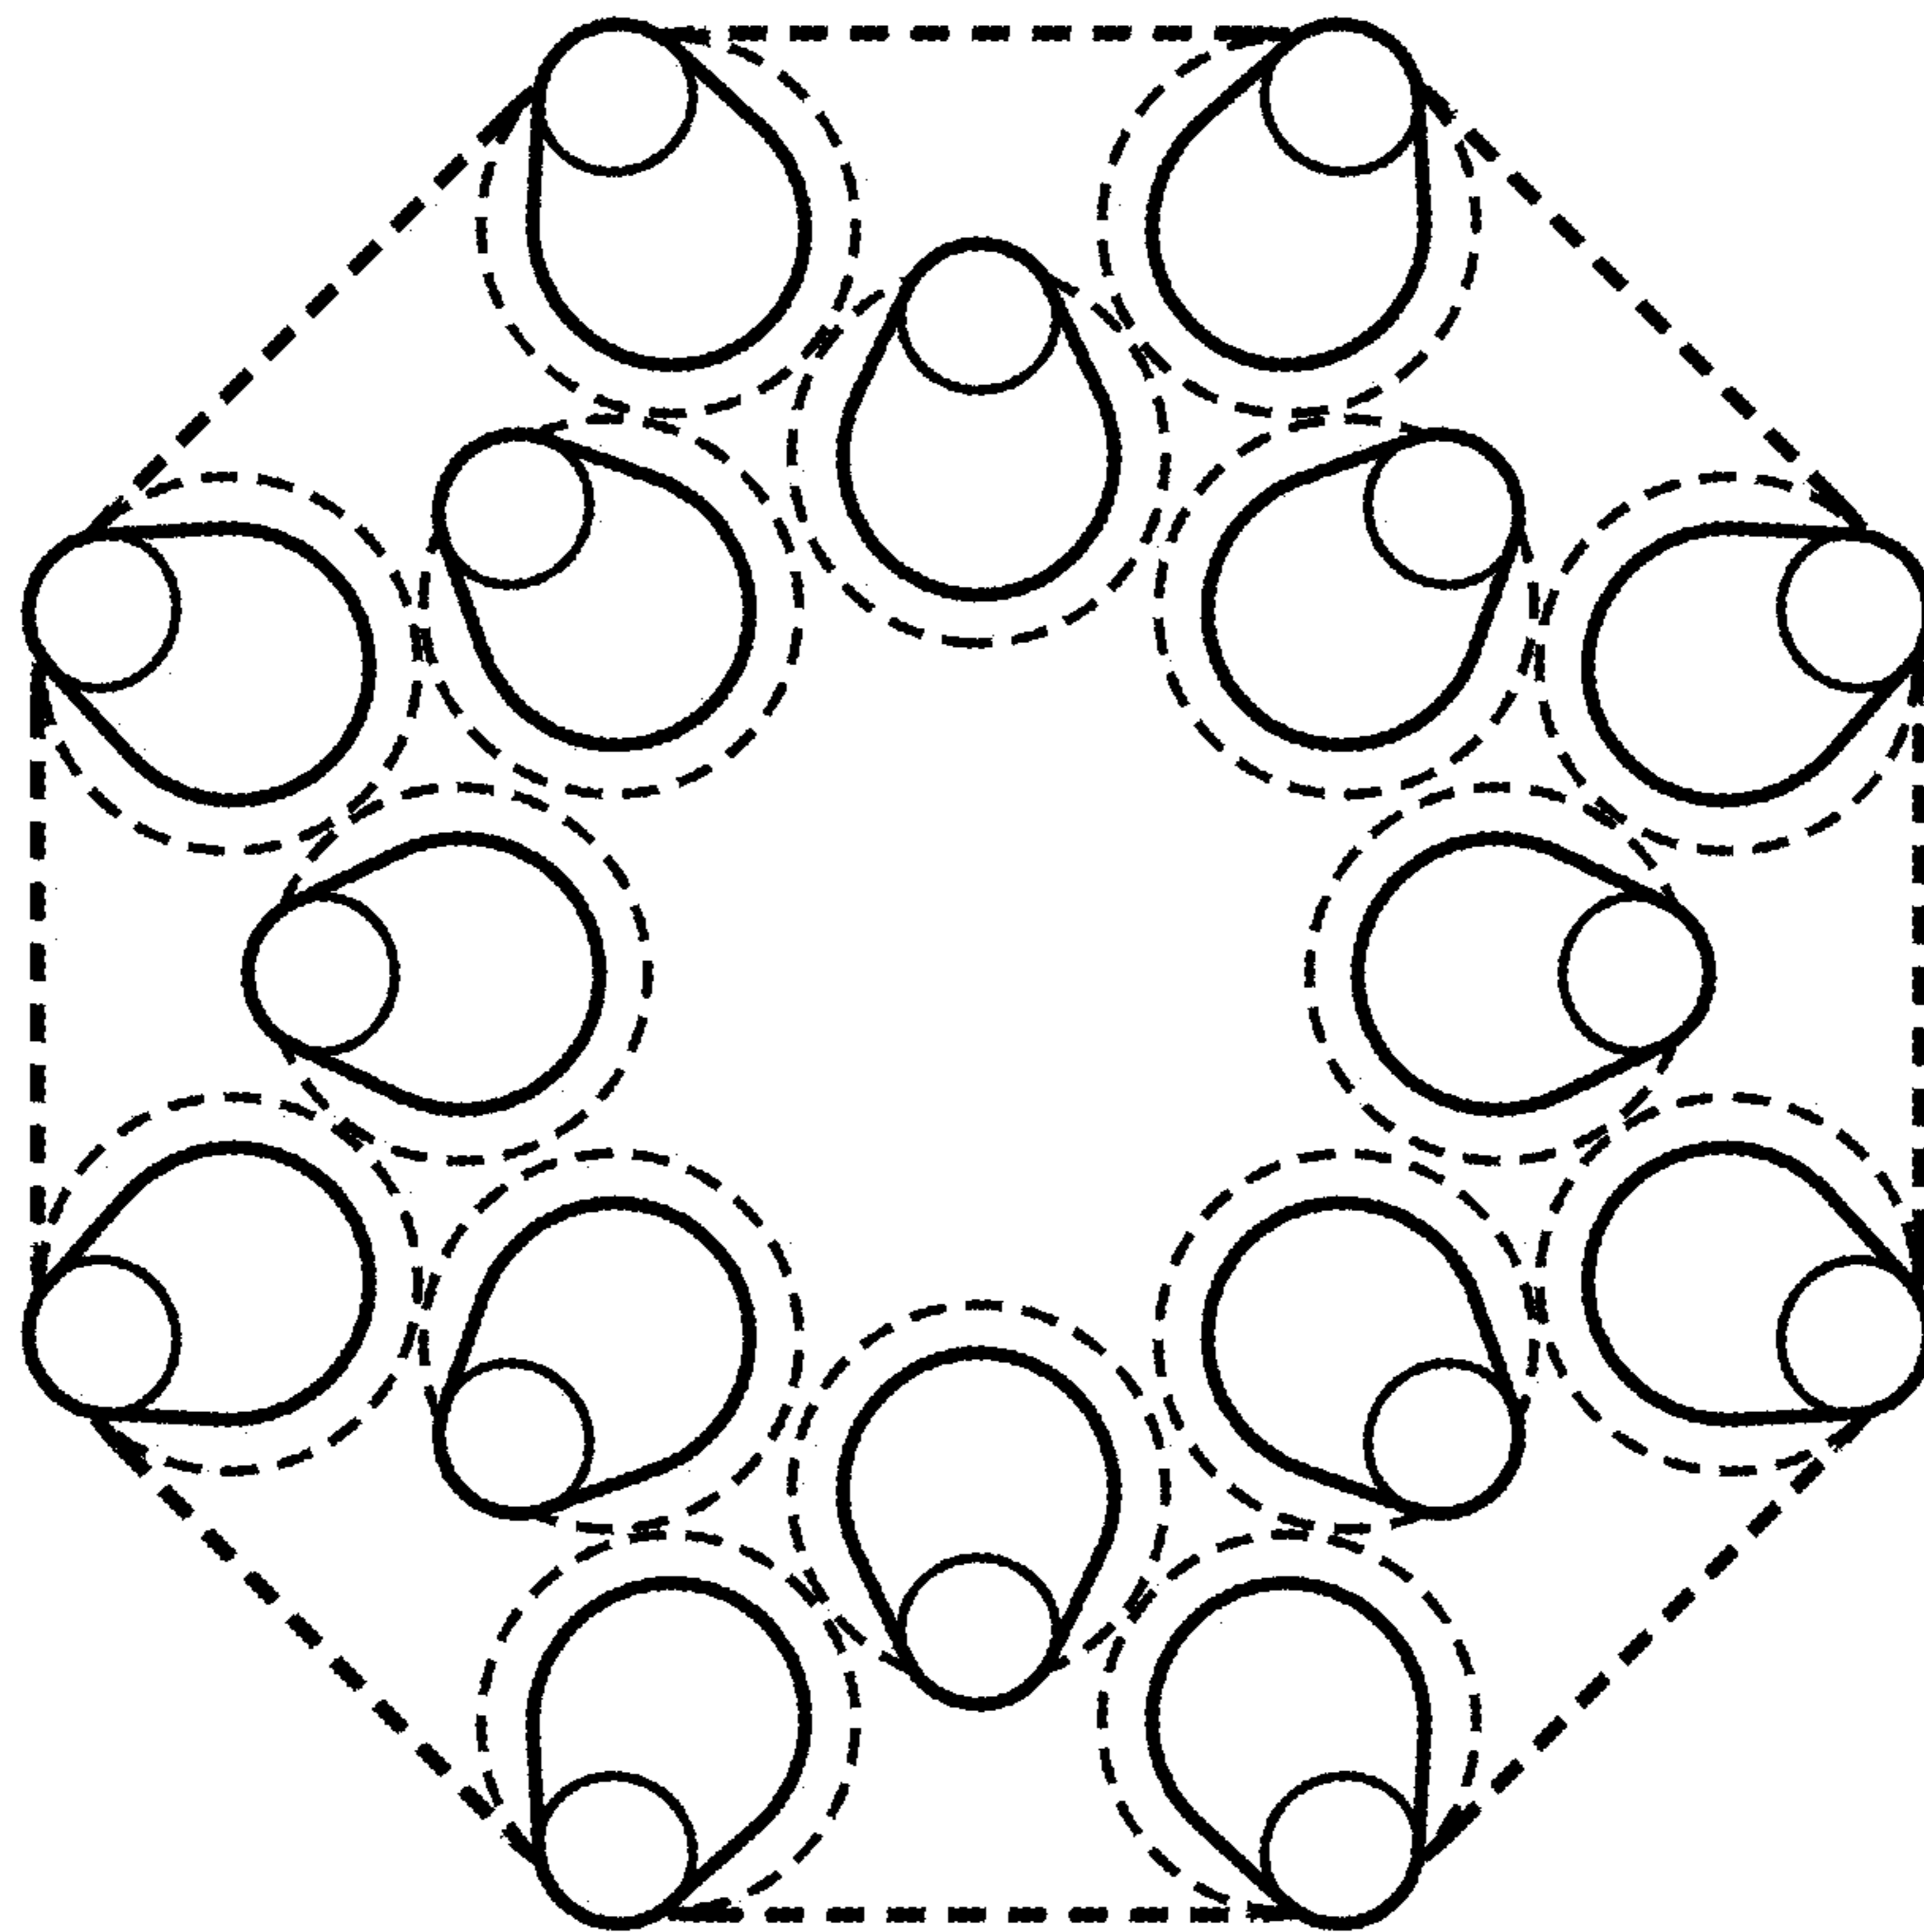


FIG. 8