



US00D979093S

(12) **United States Design Patent** (10) **Patent No.:** **US D979,093 S**  
**Jeffrey-Coker et al.** (45) **Date of Patent:** **\*\* Feb. 21, 2023**

(54) **REAGENT CARTRIDGE**  
(71) Applicant: **Singular Genomics Systems, Inc.**, La Jolla, CA (US)  
(72) Inventors: **Bande Jeffrey-Coker**, Darnestown, MD (US); **Eli N. Glezer**, Del Mar, CA (US); **Anson Hsu**, San Diego, CA (US); **Cory Spivey**, San Diego, CA (US)  
(73) Assignee: **Singular Genomics Systems, Inc.**, La Jolla, CA (US)

D632,803 S 2/2011 Motadel et al.  
8,182,763 B2 5/2012 Duffy et al.  
D673,293 S 12/2012 Demas et al.  
D674,112 S \* 1/2013 Demas ..... D24/226  
(Continued)

**FOREIGN PATENT DOCUMENTS**

GB 2560161 A 9/2018  
KR 3020190032223 \* 7/2019  
WO WO-01/60519 A1 8/2001  
WO WO-2020/183195 A1 9/2020  
WO WO-2021/126420 A1 6/2021

(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/837,498**  
(22) Filed: **May 5, 2022**  
(51) **LOC (14) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/226**  
(58) **Field of Classification Search**  
USPC ..... D24/128, 216, 223-230; D3/203.1,  
D3/203.3; D19/75, 85, 90  
CPC ..... A61B 5/150343; B01D 9/00; B01L 3/06;  
B01L 3/502; B01L 3/5025; B01L 3/5082;  
B01L 3/5085  
See application file for complete search history.

**OTHER PUBLICATIONS**

Preparing DNA Libraries for Sequencing on the MiSeq®. Online, published date Jan. 2013. Retrieved on Aug. 23, 2022 from URL: <https://content.ilabsolutions.com/wp-content/uploads/2013/04/MiSeq-Preparing-DNA-libraries.pdf>.\*

(Continued)

*Primary Examiner* — Omeed Agilee  
(74) *Attorney, Agent, or Firm* — Mintz, Levin, Cohn, Ferris, Glovsky and Popeo, P.C.

(57) **CLAIM**


The ornamental design for a reagent cartridge, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, top, and right side perspective view of a reagent cartridge of our design;  
FIG. 2 is a front view thereof;  
FIG. 3 is a rear view thereof;  
FIG. 4 is a right side view thereof;  
FIG. 5 is a left side view thereof;  
FIG. 6 is a top view thereof; and,  
FIG. 7 is a bottom view thereof.  
The dash-dash broken lines illustrate portions of the reagent cartridge that form no part of the claimed design.

(56) **References Cited**  
U.S. PATENT DOCUMENTS  
D242,654 S \* 12/1976 Rawls ..... 206/561  
4,090,850 A \* 5/1978 Chen ..... B01L 3/5025  
422/535  
D338,965 S \* 8/1993 Glanz ..... D24/227  
D359,126 S 6/1995 Hovatter  
6,096,562 A 8/2000 Bunn et al.  
6,190,300 B1 2/2001 Demsia et al.  
6,190,878 B1 2/2001 Pierson et al.  
D438,633 S \* 3/2001 Miller ..... D24/224  
D453,573 S 2/2002 Lafond et al.  
D628,306 S \* 11/2010 Blanc ..... D24/230  
7,854,896 B2 12/2010 Tyndorf et al.

**1 Claim, 4 Drawing Sheets**

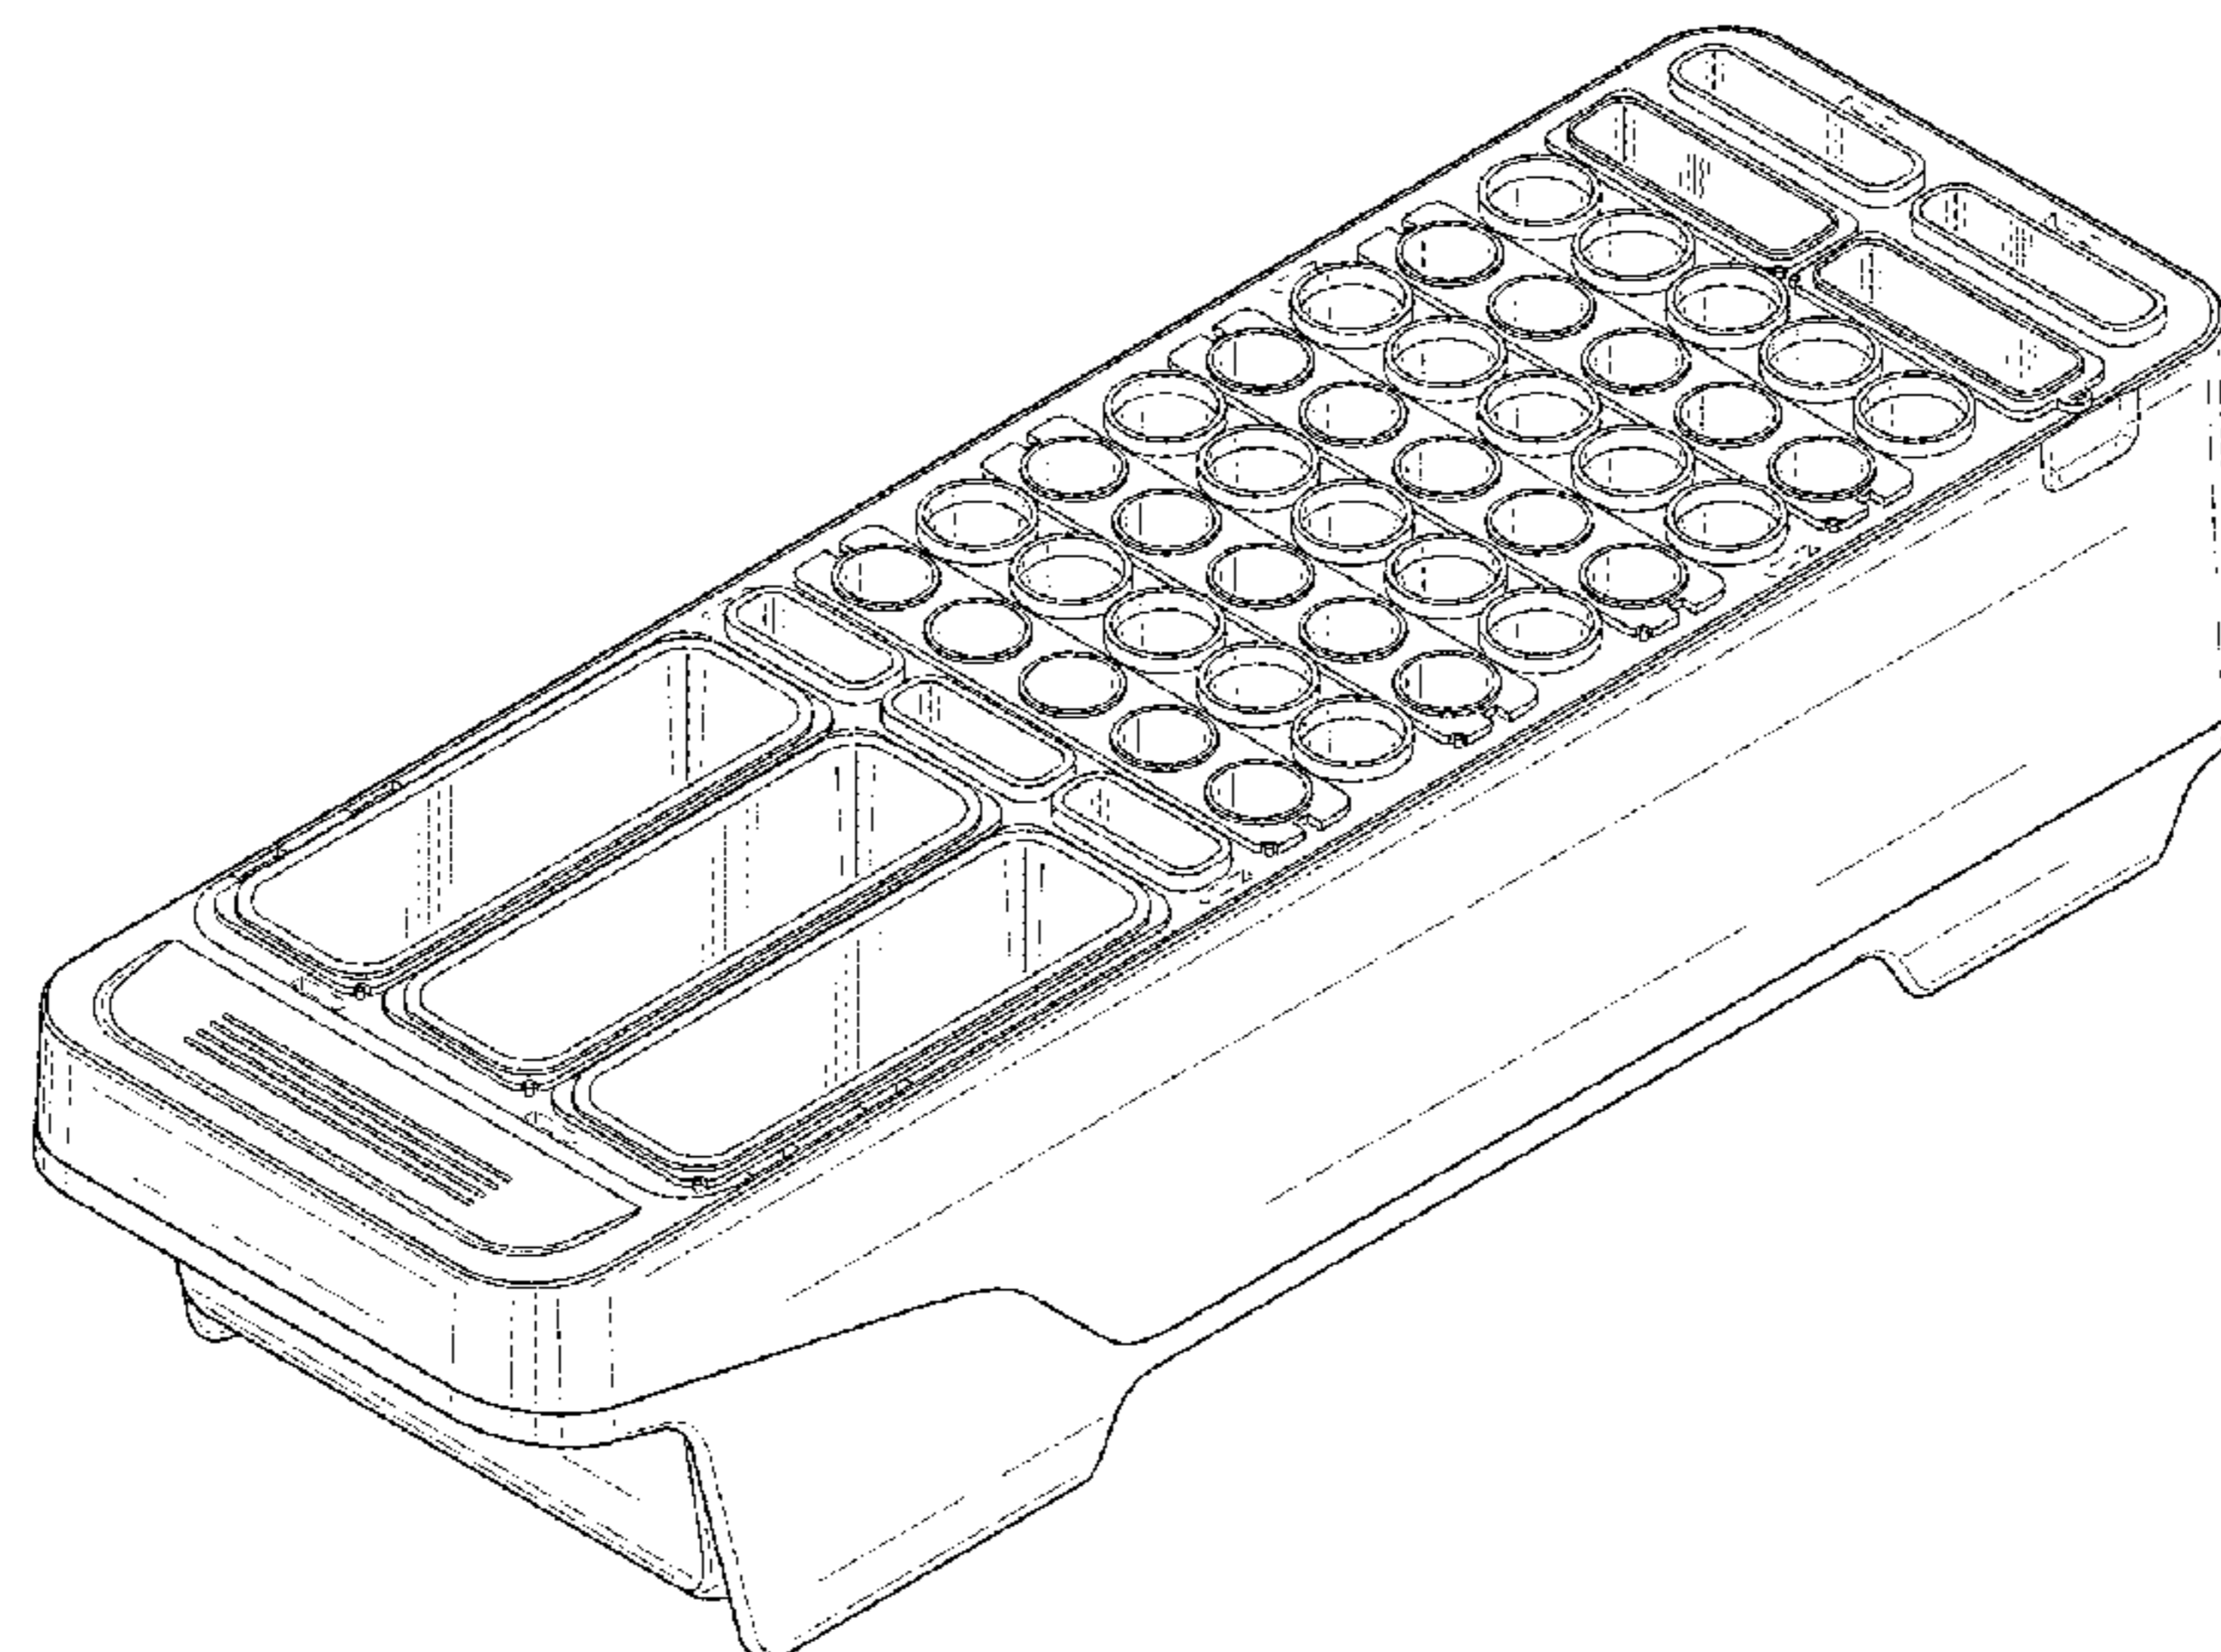

(56)

References Cited

U.S. PATENT DOCUMENTS

8,361,385 B2 1/2013 Glezer et al.  
 D687,567 S 8/2013 Jungheim et al.  
 D691,733 S 10/2013 Demas et al.  
 D699,370 S 2/2014 Motadel et al.  
 8,701,913 B2 4/2014 Pack et al.  
 D709,625 S 7/2014 Baum et al.  
 9,080,207 B2 7/2015 Handique et al.  
 D735,881 S 8/2015 Thomas  
 9,180,461 B2 11/2015 Edens et al.  
 9,260,763 B2 2/2016 Thomas et al.  
 9,267,890 B2 2/2016 Kawata et al.  
 D759,835 S 6/2016 Baum et al.  
 9,488,648 B2 11/2016 Neely et al.  
 9,519,000 B2 12/2016 Wilson et al.  
 D776,297 S \* 1/2017 Demas ..... D24/230  
 9,702,852 B2 7/2017 Lowery, Jr. et al.  
 D808,540 S \* 1/2018 Johns ..... D24/227  
 D812,243 S \* 3/2018 Johns ..... D24/227  
 9,931,635 B1 4/2018 Ho  
 10,071,381 B2 9/2018 Welch et al.  
 D840,049 S 2/2019 Schulz et al.  
 D840,050 S 2/2019 Schulz et al.  
 D840,051 S 2/2019 Schulz et al.  
 D843,007 S 3/2019 Schulz et al.  
 10,220,392 B2 3/2019 Baum et al.  
 10,241,054 B2 3/2019 Williams et al.  
 D848,637 S 5/2019 Schulz et al.  
 D852,977 S 7/2019 Suchocki et al.  
 D854,707 S 7/2019 Jakobsen et al.  
 10,335,787 B2 7/2019 Haghgooie et al.  
 10,351,843 B2 7/2019 Belz et al.  
 D856,527 S 8/2019 Kaplan et al.  
 D857,228 S 8/2019 Kaplan et al.  
 D857,229 S 8/2019 Kaplan et al.  
 10,377,538 B2 8/2019 Crivelli et al.  
 D861,914 S 10/2019 Blake et al.  
 D864,412 S 10/2019 Dangelo et al.  
 D865,213 S 10/2019 Dangelo et al.  
 D865,215 S 10/2019 Dangelo et al.  
 D902,431 S 11/2020 Sims et al.  
 10,921,336 B2 2/2021 Hansen et al.  
 D918,417 S \* 5/2021 O'Mahony ..... D24/229  
 D919,115 S 5/2021 Kaplan et al.  
 11,000,851 B2 5/2021 Knight  
 D932,052 S \* 9/2021 Zergiebel ..... D24/227  
 11,199,538 B2 12/2021 Burd et al.  
 11,254,942 B2 2/2022 Tian et al.  
 11,293,021 B1 4/2022 Bemate et al.  
 D959,018 S \* 7/2022 Livingston ..... D24/226  
 2004/0238401 A1 12/2004 Greenstein et al.  
 2008/0257882 A1 10/2008 Turner  
 2013/0309147 A1 11/2013 Yu et al.  
 2014/0234182 A1 8/2014 Motadel et al.  
 2017/0036207 A1 2/2017 Wright et al.  
 2017/0043346 A1 \* 2/2017 Welch ..... A61B 5/15  
 2017/0136467 A1 \* 5/2017 Johns ..... G01N 35/00732  
 2017/0197213 A1 7/2017 Nielsen et al.  
 2020/0122141 A1 4/2020 Haghgooie et al.  
 2020/0290037 A1 9/2020 Salomon et al.  
 2021/0324445 A1 10/2021 Buse et al.  
 2022/0080425 A1 3/2022 Bashar et al.  
 2022/0112452 A1 4/2022 Garst et al.  
 2022/0112508 A1 4/2022 Garst et al.

OTHER PUBLICATIONS

Qiagen—QIAAsymphony® DNA Maxi Handbook located at <<https://www.google.com/imgres?imgurl=x-raw-image%3A%2F%2Ffae>

1930bd2bc06f496a635e47dff671c1818eff4edfb5a5123e3a71ff012524a&imgrefurl=https%3A%2F%2Fwww.qiagen.com%2Fde%2Fresources%2Fdownload.aspx%3Fid%3D71390d4f-115f-4368-ba2e-5f6cf7936b21%26lang%3Den&tbnid=9Aa80guT4fqjvM&vet=10CAoQMjyUAWoXChMI8LLzioel9wVAAAAAB0AAAAAEAQ..i&docid=7suzloSWWcuBtM&w=1109&h=439&q=DNA%20sequencer%20reagent%20cartridges&ved=0CAoQMviUAWoXChMI8LLzioel9wVAAAAAB0AAAAAEAQ, last accessed May 5, 2022.

Qiagen—RNA kit located at <<https://www.qiagen.com/us/products/discovery-and-translational-research/dna-rna-purification/rna-purification/total-rna/qiasymphony-rna-kit/>> last accessed May 5, 2022.

Removable 8 Well PCR Tube Strip located at <<https://www.azenta.com/products/removable-8-well-pcr-tube-strip>> last accessed May 5, 2022.

Axygen® PCR-strips of 8 tubes located at <<https://www.mls.be/en/p/tubes-racks-pcr/analyser-cups-microtubes-pcr-disposables/axygen-microtubes-pcr-range/axygen-pcr-range/>> last accessed May 5, 2022.

NovaSeq Reagent Kits, Illumina, located at <<https://www.illumina.com/products/by-type/sequencing-kits/cluster-gen-sequencing-reagents/novaseq-reagent-kits.html>> last accessed May 5, 2022.

The Illumina Sequencing Protocol and the NovaSeq 6000 System | SpringerLink, located at <<https://www.google.com/imgres?imgurl=x-raw-image%3A%2F%2F%2F2F288cbe228cbff5322455626b5c915345d4afdb>> last accessed May 5, 2022.

NextSeq 500/550 v2.5 Kits located at <<https://www.illumina.com/products/by-type/sequencing-kits/cluster-gen-sequencing-reagents>> last accessed May 5, 2022.

MiSeq Reagent Kit v3 located at <<https://www.illumina.com/systems/sequencing-platforms/miseq/products-services.html>> last accessed May 5, 2022.

Hitachi—Compact CE Sequencer DS3000 located at <<https://www.hitachi-hightech.com/global/science/products/bio-systems/sequencer/ds3000.html>> last accessed May 5, 2022.

Ion 540™ Kit-Chef (2 sequencing runs per initialization) located at <<https://www.thermofisher.com/order/catalog/product/A30011>> last accessed May 5, 2022.

LabX Ion S5 Semiconductor Sequencer + Ion Chef System | For Sale | Labx Ad 14035113, located at <[Stellar Scientific—SeeMore 0.2ml Optically Clear PCR Strip Tube with Separate Dome Caps, located at <<https://www.stellarscientific.com/seemore-0-2ml-optically-clear-pcr-strip-tube-with-separate-dome-caps-sterile-125-pack/#&gid=1&pid=1>> last accessed May 5, 2022.](https://www.google.com/imgres?imgurl=https%3A%2F%2Fcheckout.labx.com%2Fpub%2Fmedia%2Fcatalog%2Fproduct%2Fi%2Fm%2Fimg-20220202-092431058.jpg&imgrefurl=https%3A%2F%2Fwww.labx.com%2Fitem%2Fion-s5-semiconductor-sequencer-ion-chef-system%2F14035113&tbnid=CtQy2sSs_zECkM&vet=10CK0BEDMotgFqFwoTCPCy84qHpfcCFQAAAAAdAAAAABAD..i&docid=18bcwsY5Nbi5hM&w=1600&h=1200&q=DNA%20sequencer%20reagent%20cartridges&ved=0CK0BEDMotgFqFwoTCPCy84qHpfcCFQAAAAAdAAAAABAD> last accessed May 5, 2022.</p>
</div>
<div data-bbox=)

CAPP 0.1 and 0.2 ML PCR Strip Tubes, located at <<https://www.capp.dk/product/expell-pcr-strip-tubes>> last accessed May 5, 2022.  
 T320-2 & T320-3 Amplitube™ 8 Tube Strips With Individually Attached Caps, located at <<https://www.simport.com/en/products/224-t320-2.html>> last accessed May 5, 2022.

Fischer Scientific—Eppendorf™ PCR Tube Strips and Domed Cap Strips, 0.1 mL, located at <<https://www.fishersci.se/shop/products/eppendorf-0-1ml-pcr-tubes-cap-strips/10146704>> last accessed May 5, 2022.

\* cited by examiner



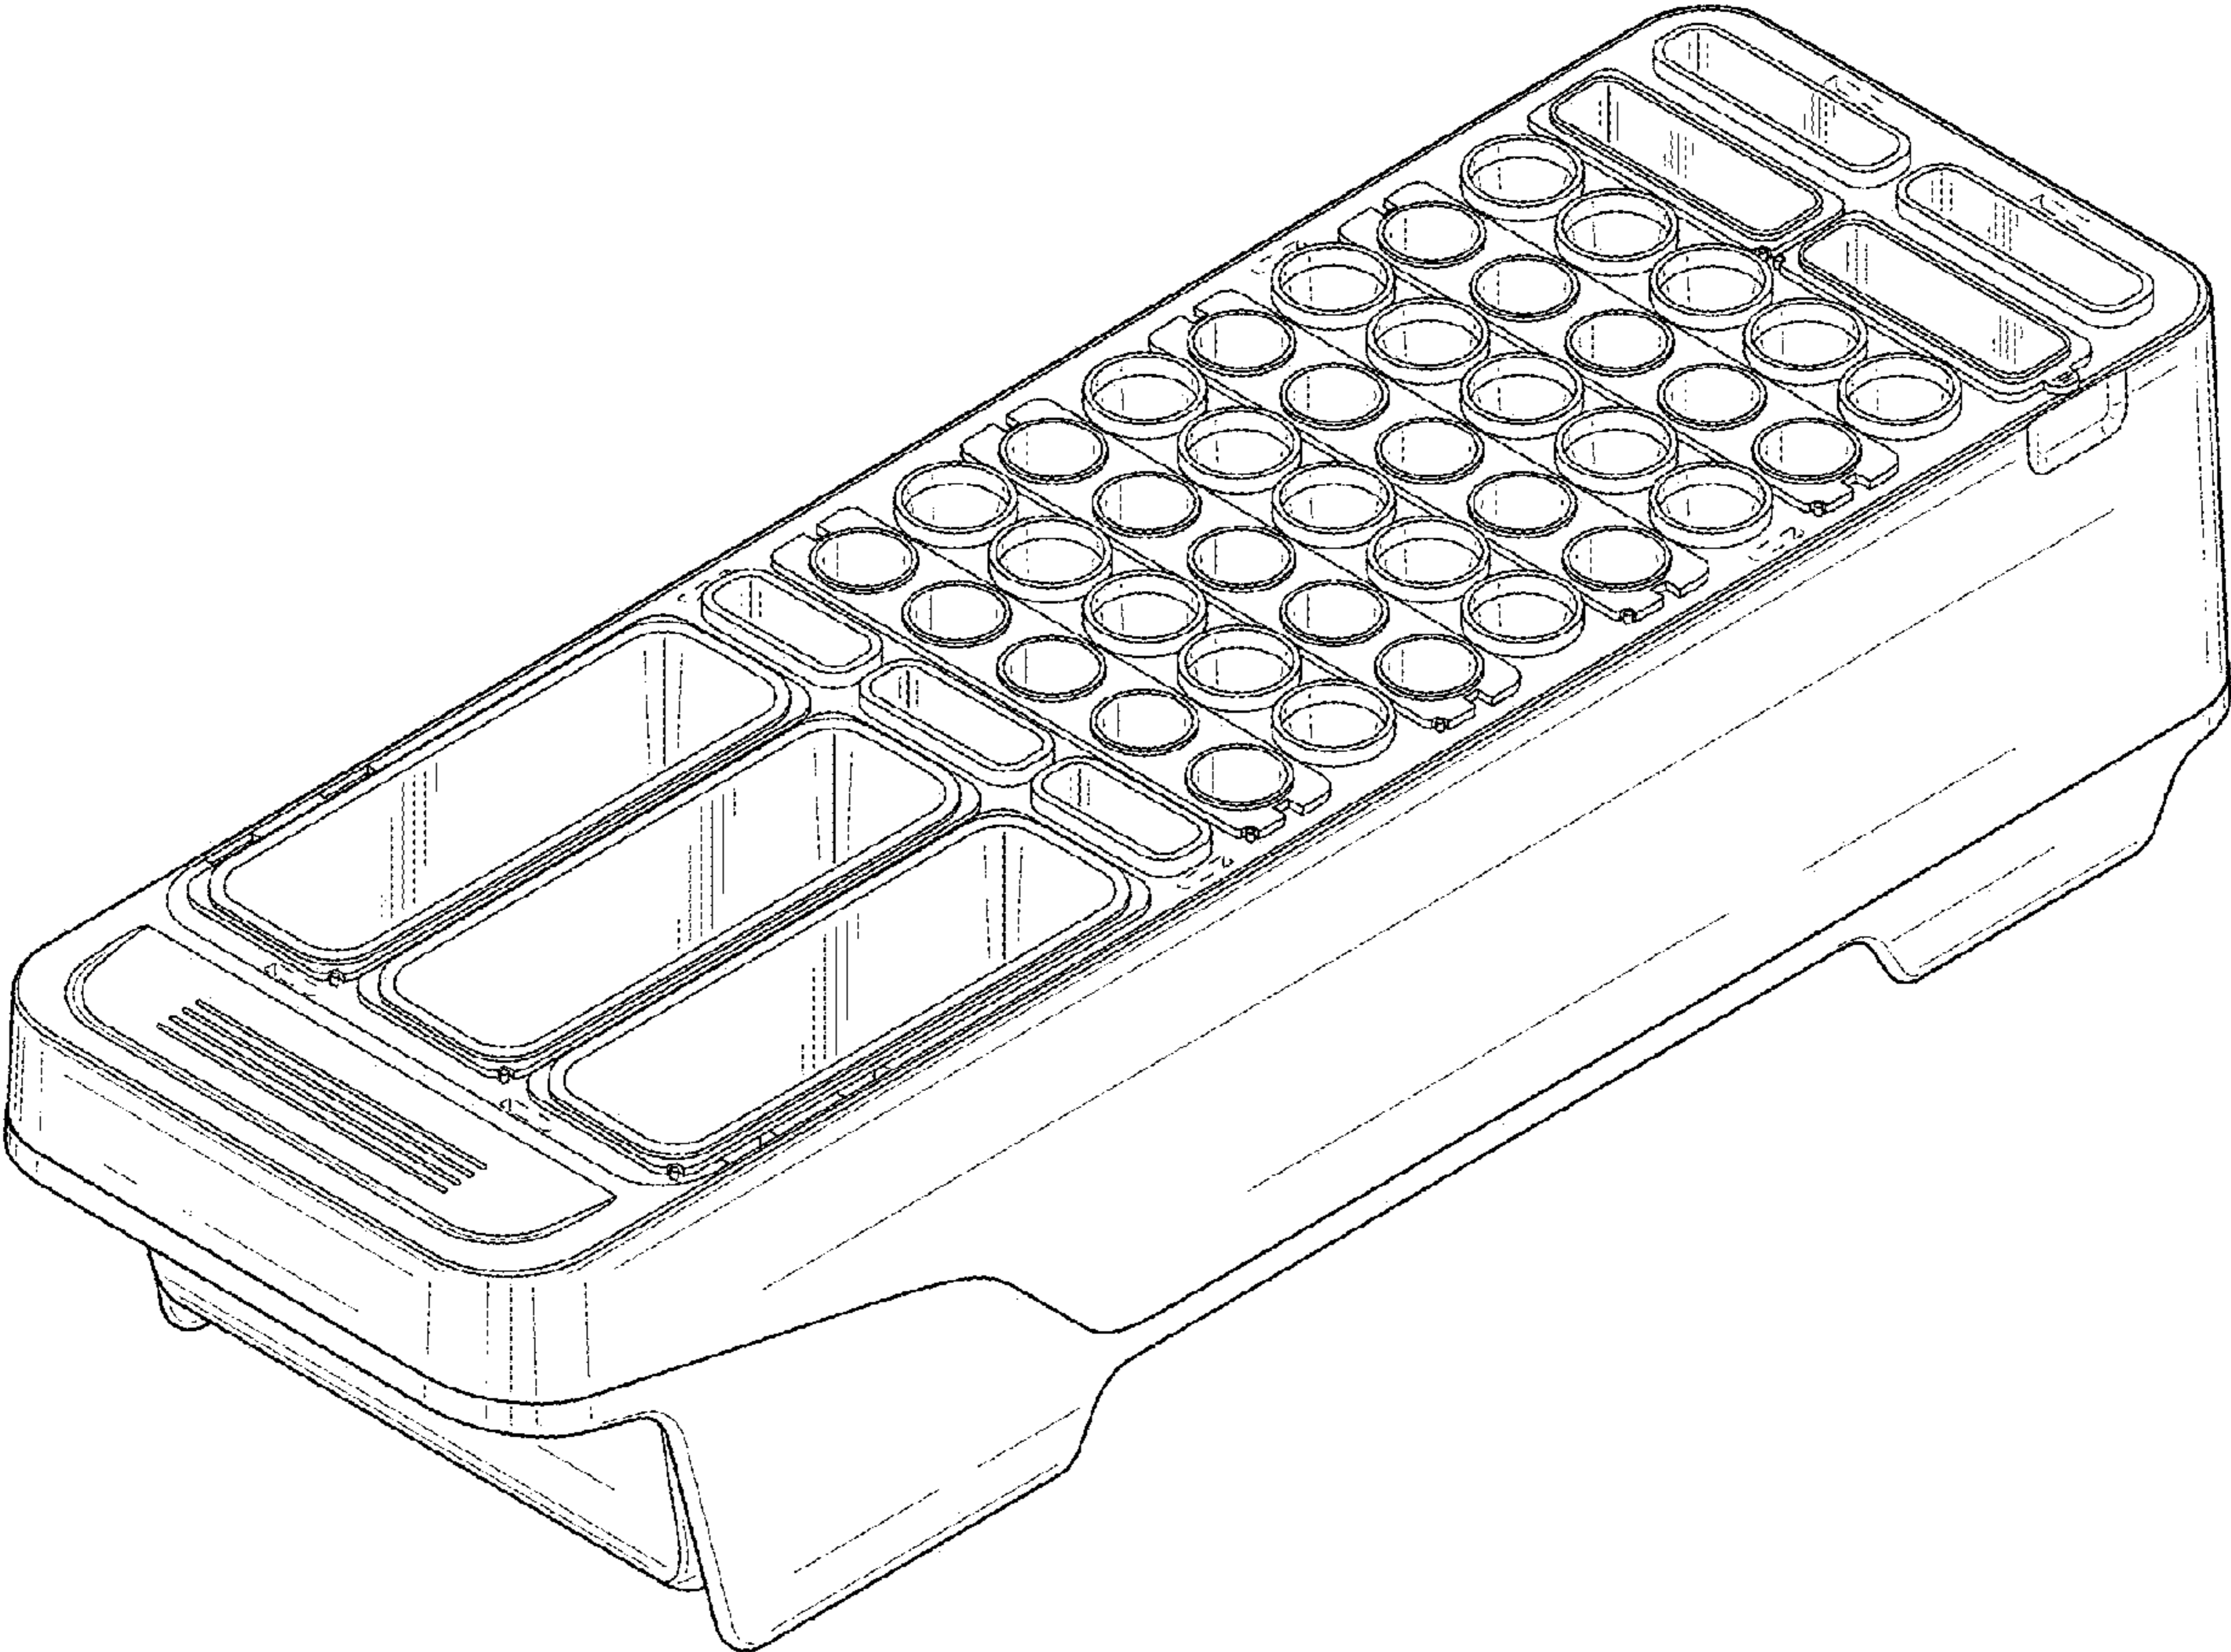



FIG. 1

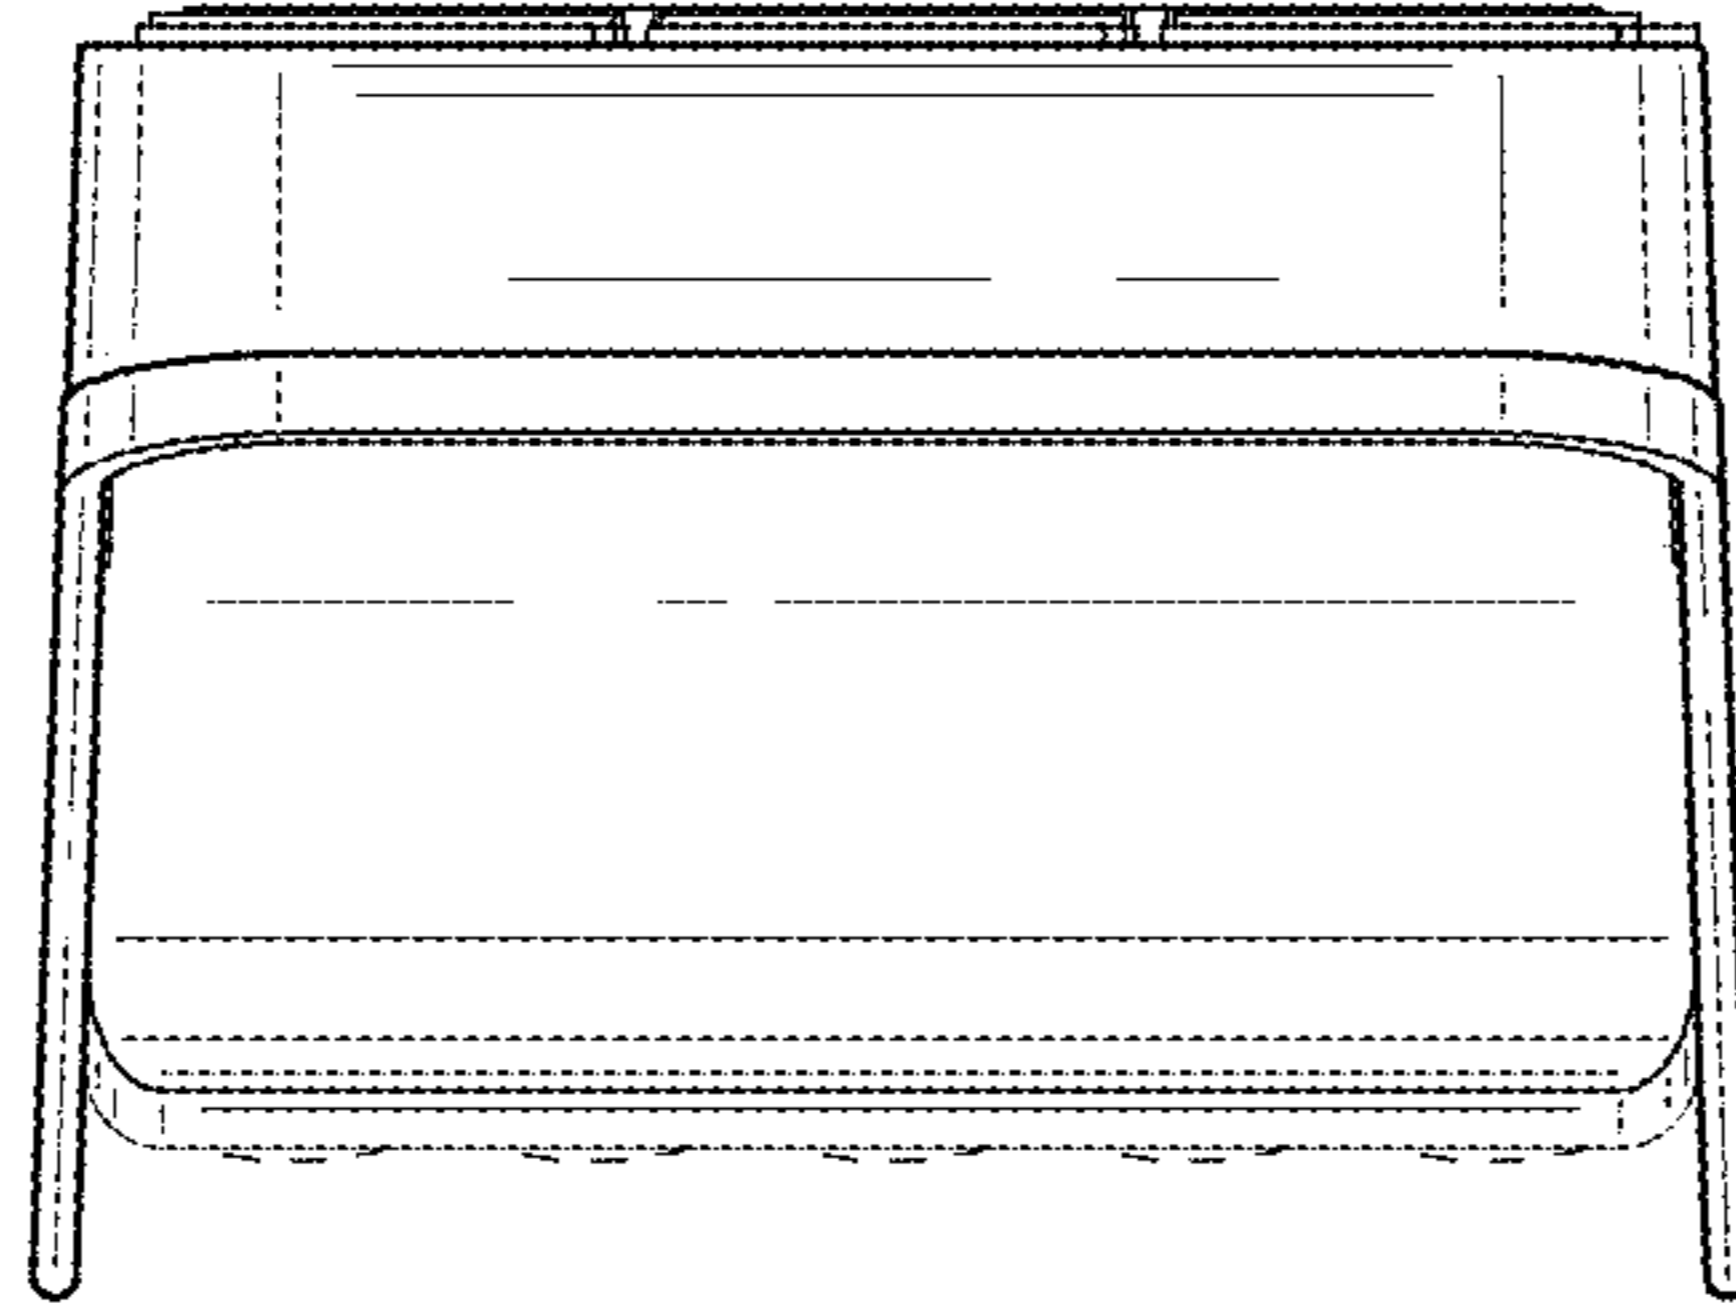


**FIG. 2**

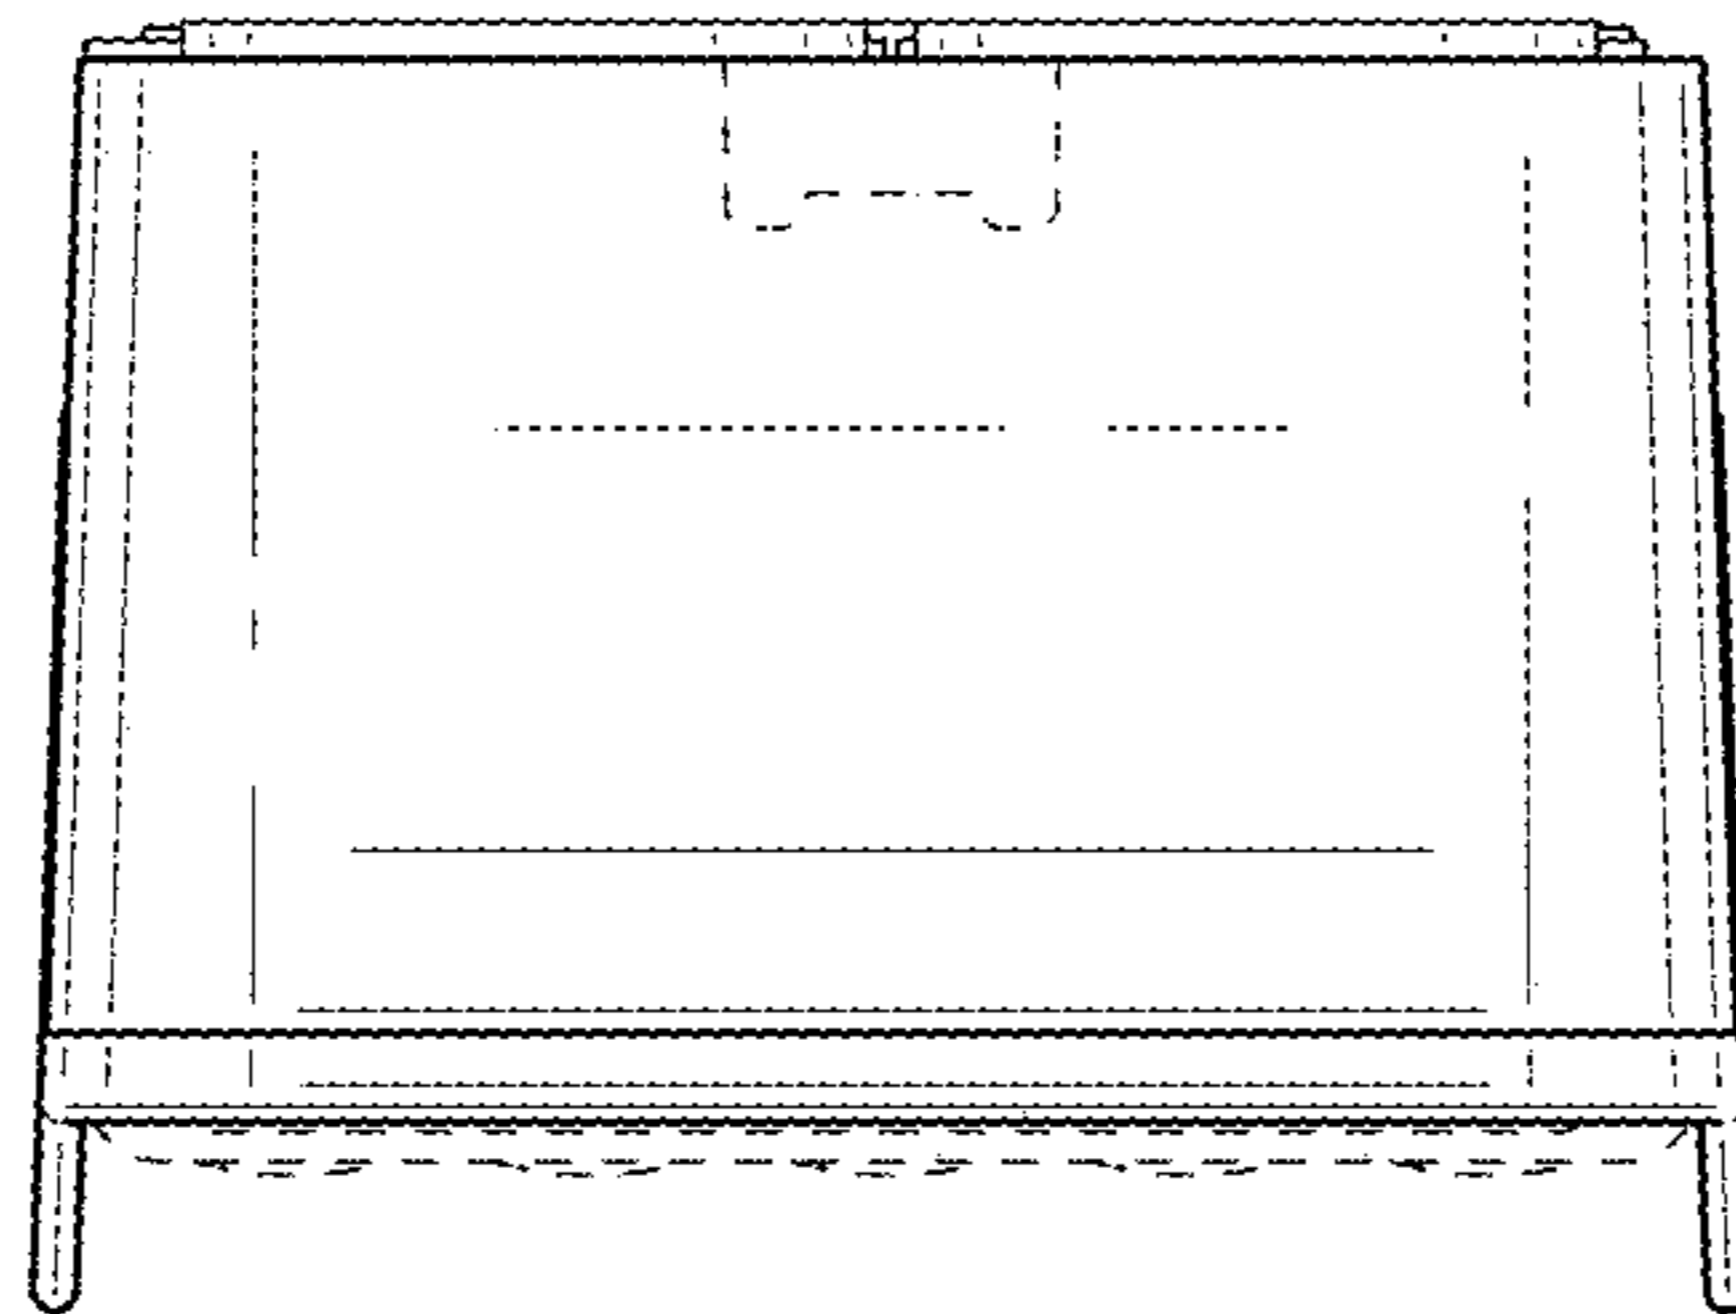


**FIG. 3**

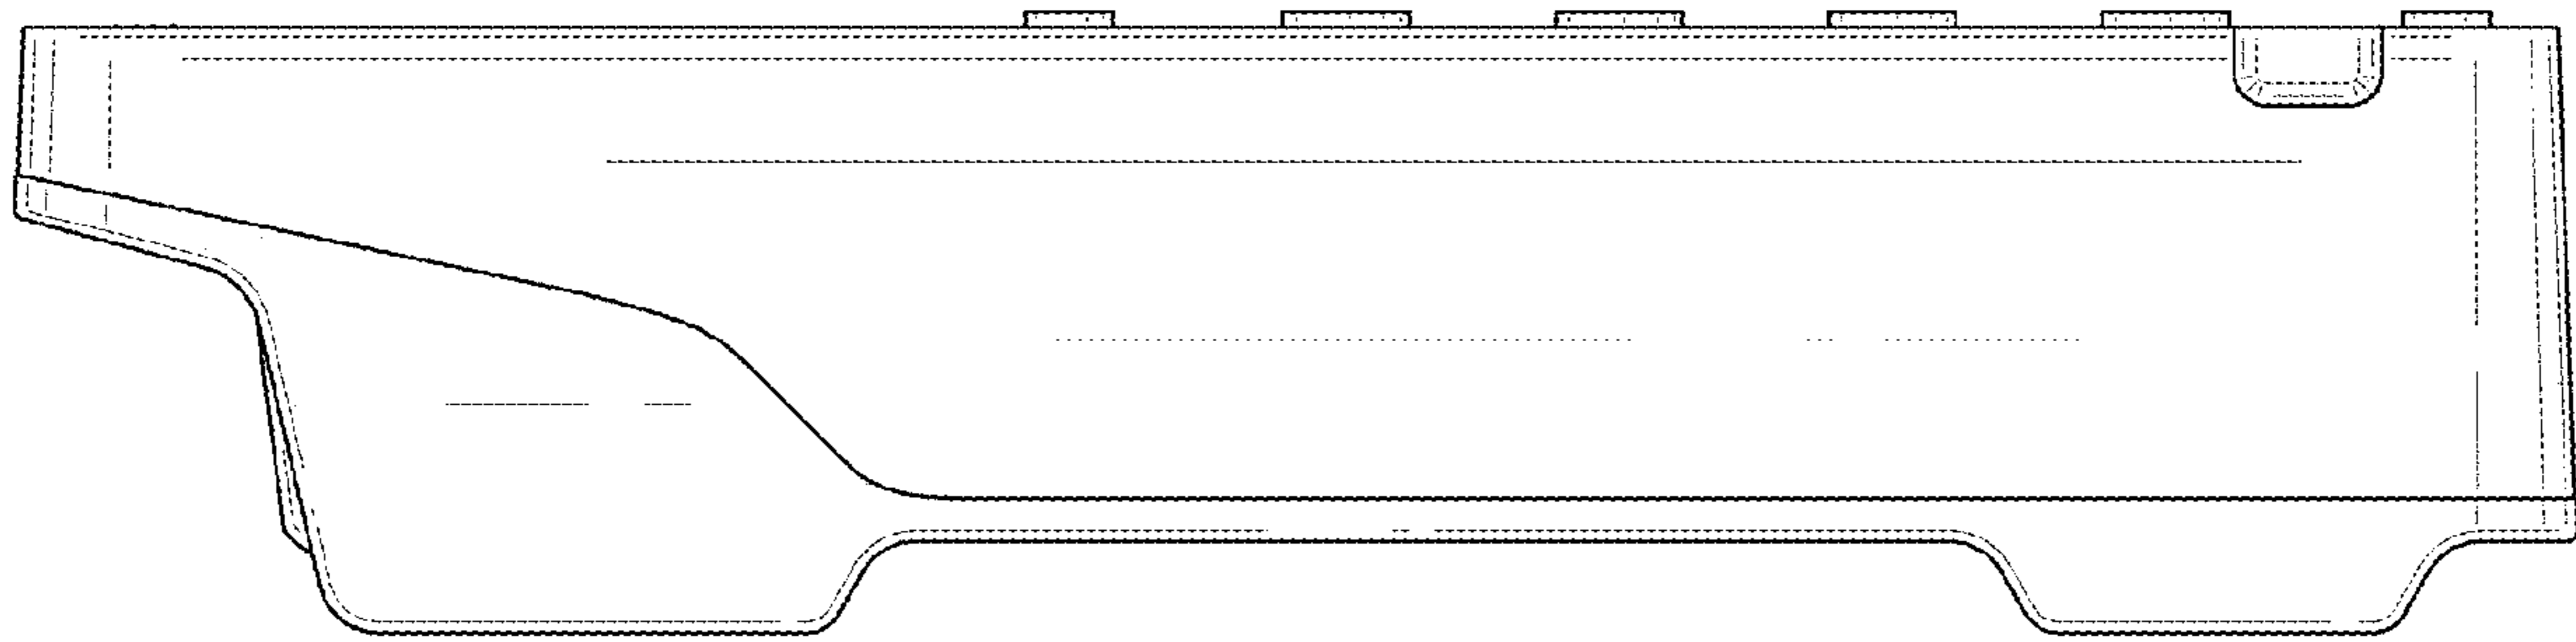


**FIG. 4**

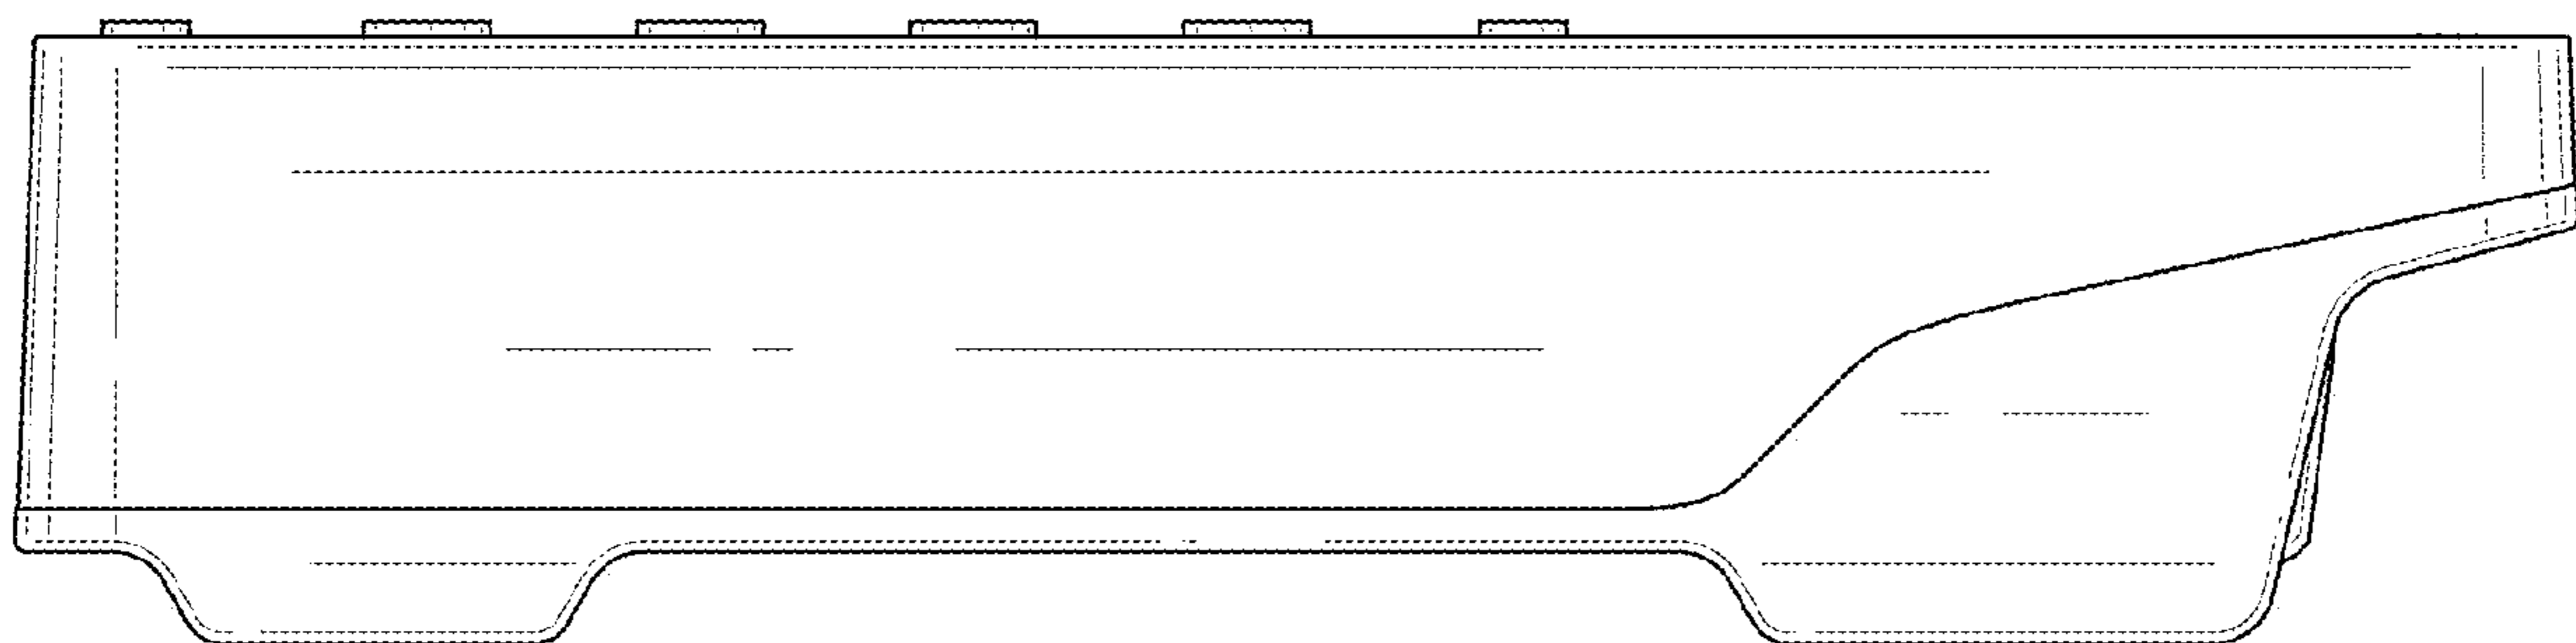

**FIG. 5**

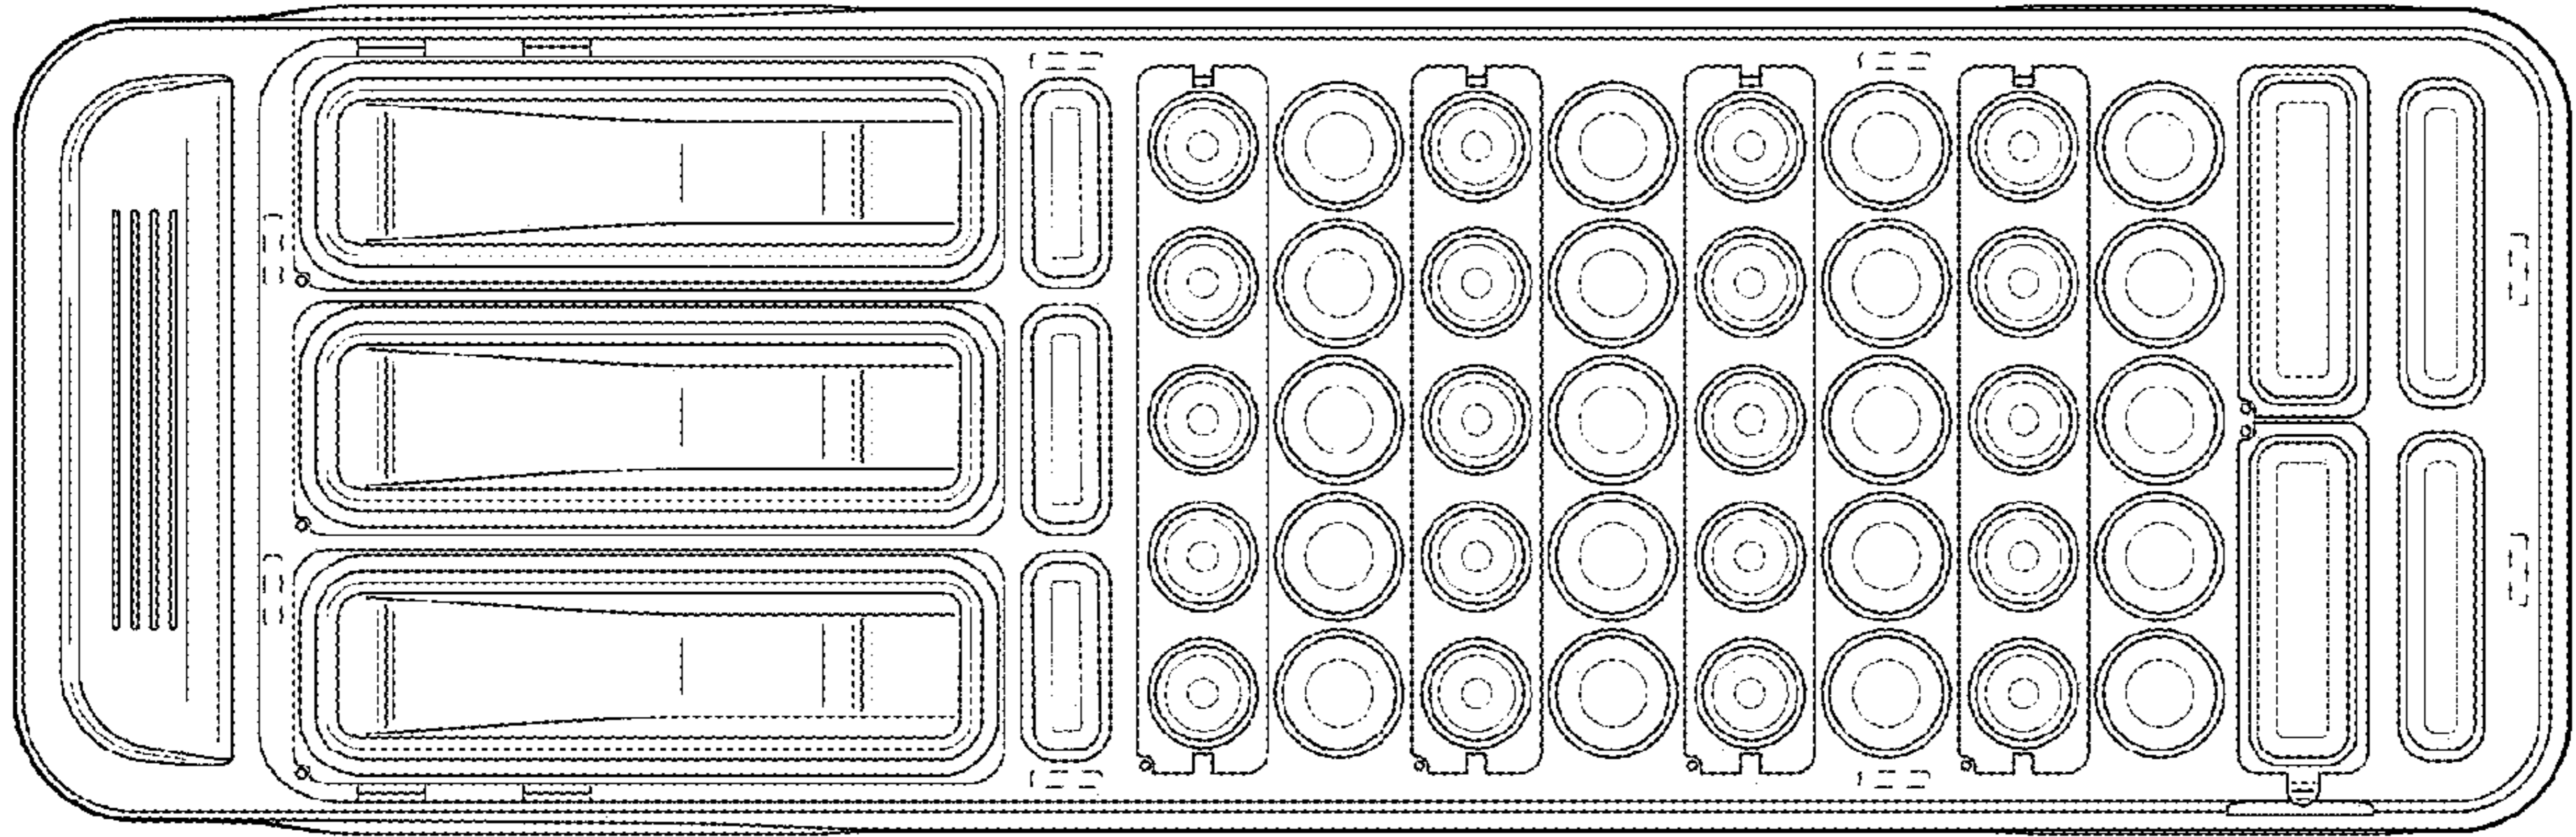

**FIG. 6**

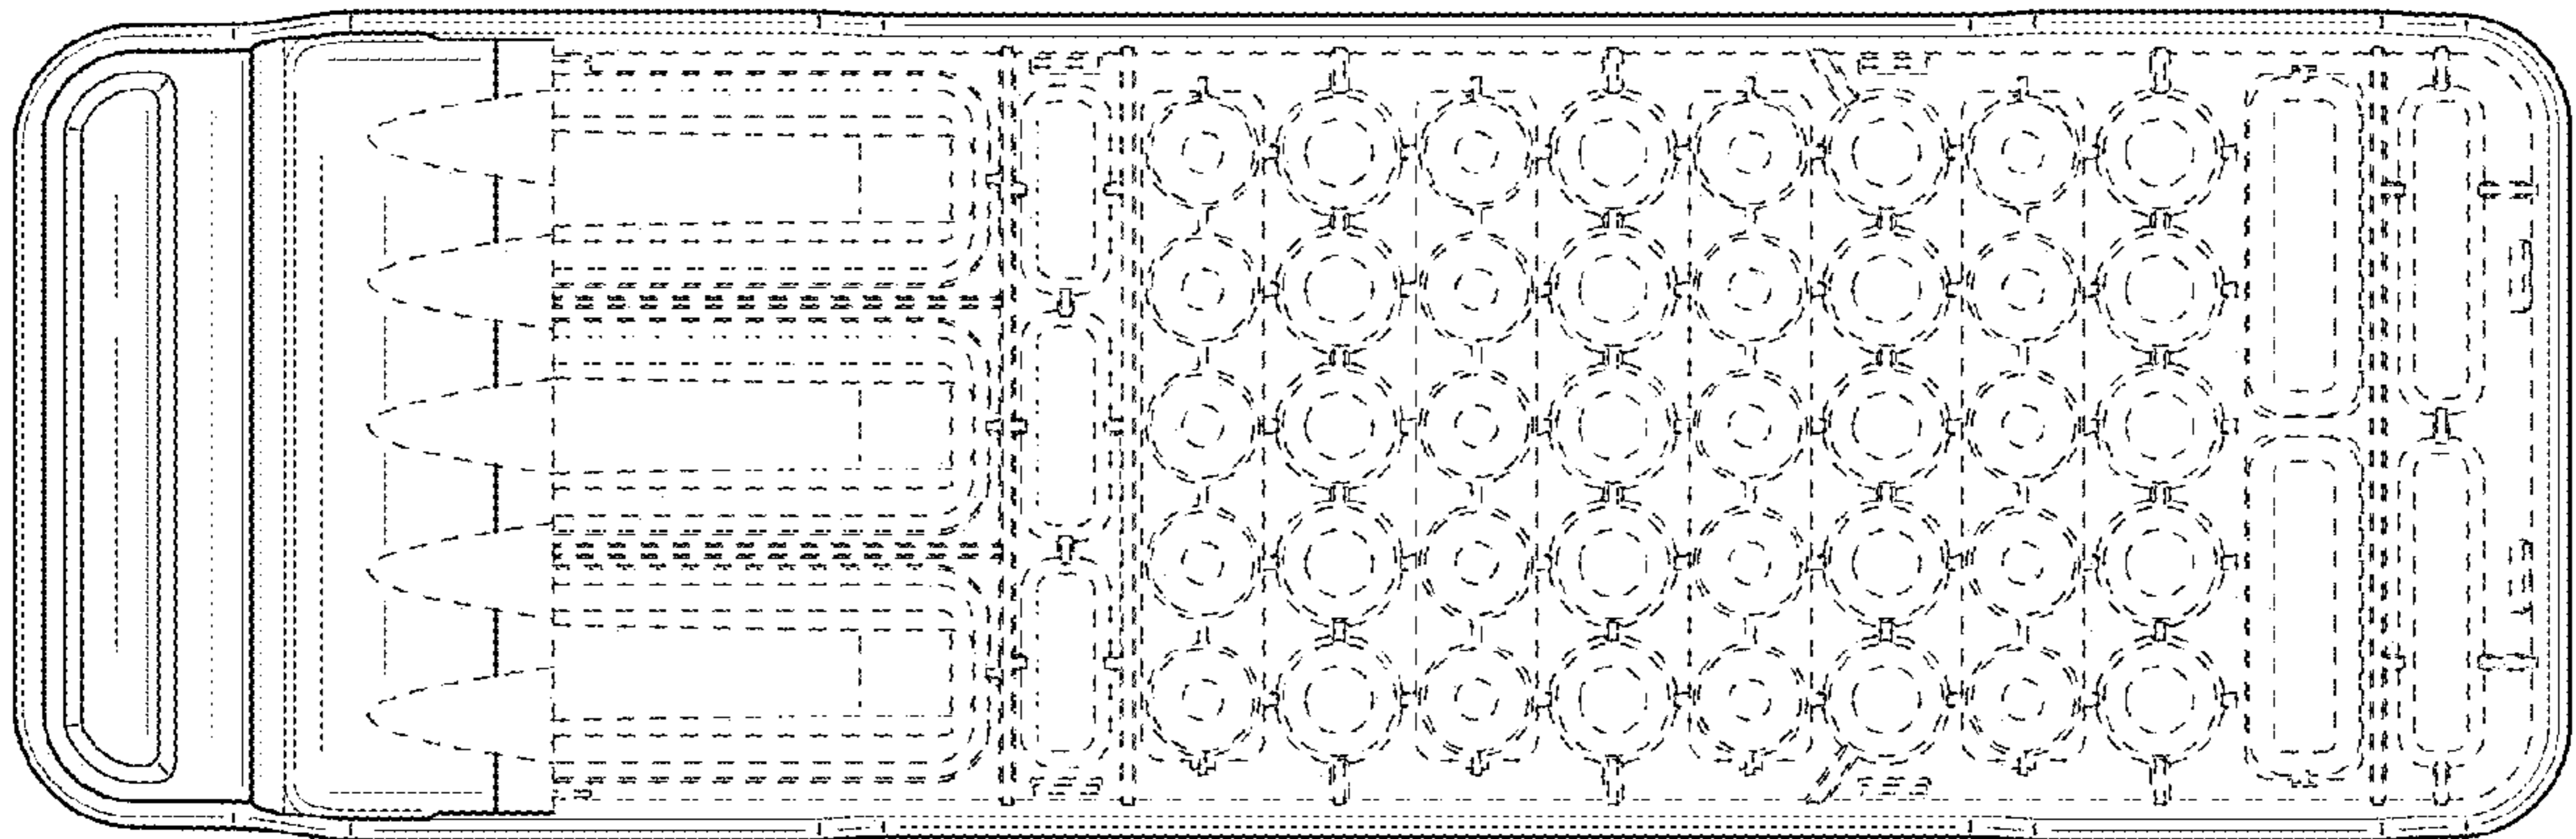

**FIG. 7**