

US00D979145S

(12) **United States Design Patent**
Van Nortwick et al.

(10) **Patent No.:** **US D979,145 S**
(45) **Date of Patent:** **** Feb. 21, 2023**

(54) **SURGICAL HELMET**

(71) Applicant: **Stryker Corporation**, Kalamazoo, MI (US)

(72) Inventors: **Matthew Van Nortwick**, Kalamazoo, MI (US); **Benjamin Edinger**, Grand Haven, MI (US)

(73) Assignee: **Stryker Corporation**, Kalamazoo, MI (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/700,254**

(22) Filed: **Jul. 31, 2019**

(51) **LOC (14) Cl.** **29-02**

(52) **U.S. Cl.**
USPC **D29/102**

(58) **Field of Classification Search**

USPC D2/865, 866, 867, 869, 870, 872, 873, D2/874, 878, 886, 887, 888, 891, 892, D2/893; D21/698, 788; D24/108, 110, D24/110.1, 110.2, 110.3, 110.4; D29/100, 102, 103, 104, 105, 106, 107, D29/108, 109, 110, 112, 122

CPC A41D 13/00; A41D 13/012; A41D 13/05; A41D 13/11; A41D 13/1107; A41D 13/1138; A41D 13/1161; A41D 13/1176; A42B 1/00; A42B 1/002; A42B 1/0181; A42B 1/0184; A42B 1/02; A42B 3/00; A42B 3/04; A42B 3/0406; A42B 3/06; A42B 3/066; A42B 3/16; A42B 3/18; A42B 3/20; A42B 3/22; A42B 3/221; A42B 3/222; A42B 3/226; A42B 3/227; A42B 3/28; A42B 3/32; A42B 3/322; A42B 3/324; A42B 1/012; A42B 3/225; F41H

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,758,307 A * 8/1956 Treiber A61F 9/025
2/9

5,301,372 A 4/1994 Matoba
5,630,412 A 5/1997 Dubruille et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2017112485 A1 6/2017

OTHER PUBLICATIONS

Stryker, "T5 Personal Protection System", first available 2015. (<https://www.strykermeded.com/media/1081/t5-personal-protection-brochure.pdf>) (Year: 2015).*

(Continued)

Primary Examiner — Lauren D McVey

Assistant Examiner — Justin A Johnson

(74) *Attorney, Agent, or Firm* — Howard & Howard Attorneys PLLC

(57) **CLAIM**

The ornamental design for a surgical helmet, as shown and described.

DESCRIPTION

FIG. 1 is a top, front left-side perspective view of a surgical helmet;

FIG. 2 is a bottom left-side perspective view thereof;

FIG. 3 is a front right-side perspective view thereof;

FIG. 4 is a front-side view thereof;

FIG. 5 is a right-side view thereof;

FIG. 6 is a left-side view thereof;


FIG. 7 is a top-side view thereof;

FIG. 8 is a bottom-side view thereof; and,

FIG. 9 is a rear-side view thereof.

The broken lines immediately adjacent to the shaded areas depict the bounds of the claimed design, while all other broken lines are directed to environment. The broken lines form no part of the claimed design.

1 Claim, 9 Drawing Sheets

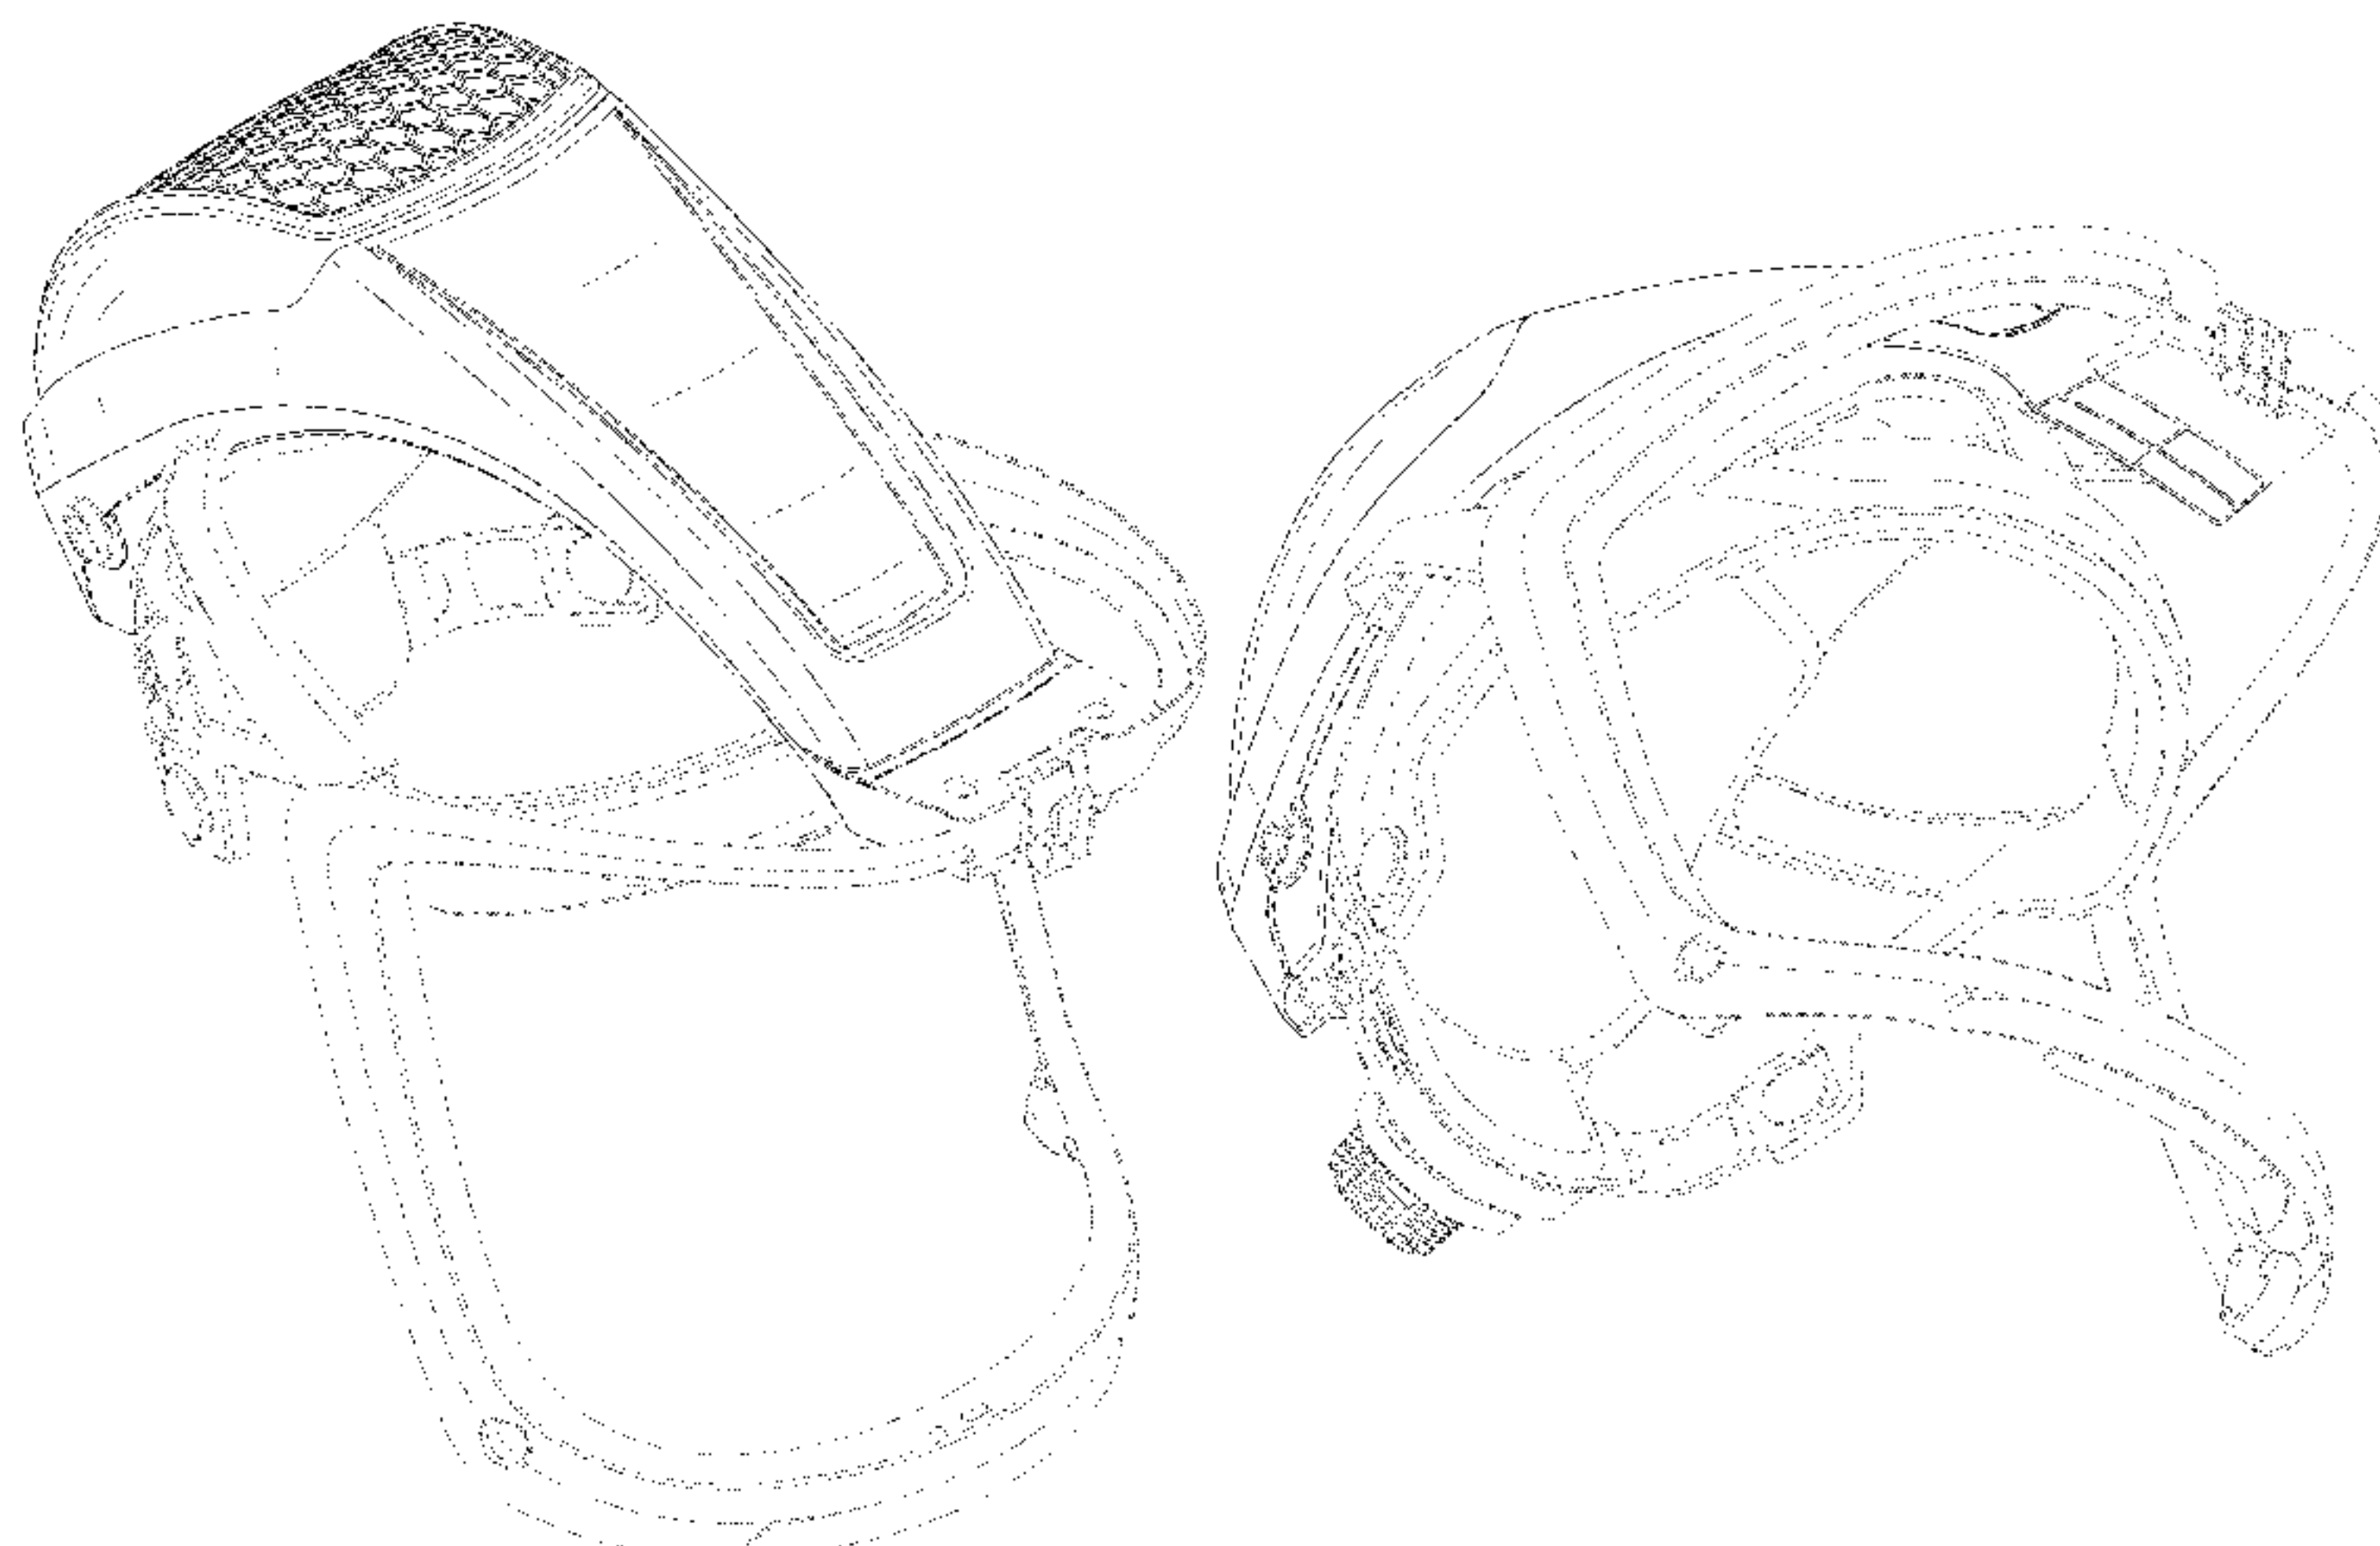

US D979,145 S

(58) **Field of Classification Search**
 CPC 1/00; F41H 1/04; F41H 1/06; F41H 1/08;
 A63B 2243/007
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D384,441	S *	9/1997	Badger	D29/110
5,711,033	A	1/1998	Green et al.		
6,170,084	B1	1/2001	Gordon et al.		
6,481,019	B2	11/2002	Diaz et al.		
6,622,311	B2	9/2003	Diaz et al.		
6,792,944	B1	9/2004	Green et al.		
D499,214	S *	11/2004	Cheng	D29/110
6,918,141	B2	7/2005	Green et al.		
6,928,662	B2	8/2005	Fournier		
6,954,968	B1	10/2005	Sitbon		
6,973,677	B2	12/2005	Diaz et al.		
7,093,302	B1	8/2006	Burns		
D539,485	S *	3/2007	Huh	D29/110
7,200,873	B2	4/2007	Klotz et al.		
7,225,471	B2	6/2007	Sutter et al.		
7,735,156	B2	6/2010	VanDerWoude et al.		
7,752,682	B2	7/2010	VanDerWoude et al.		
7,937,775	B2	5/2011	Manzella, Jr. et al.		
8,225,421	B1	7/2012	Froissard		
8,234,722	B2	8/2012	VanDerWoude et al.		
8,261,375	B1	9/2012	Reaux		
D670,036	S *	10/2012	Folkesson	A61F 9/025 D29/108
8,282,234	B2	10/2012	VanDerWoude et al.		
8,302,599	B2	11/2012	Green		
8,407,818	B2	4/2013	VanDerWoude et al.		
8,453,262	B2	6/2013	Green		
8,621,375	B2	12/2013	Berger et al.		
8,621,664	B2	1/2014	Peebles		
8,745,763	B2	6/2014	Cho		
8,819,869	B2	9/2014	VanDerWoude et al.		
9,173,437	B2	11/2015	VanDerWoude et al.		
9,833,032	B2	12/2017	Jacobsen		
10,420,386	B1 *	9/2019	Jefferis	A41D 13/1153

D888,228	S *	6/2020	Hare	A42B 3/225 D24/110.3
D895,213	S *	9/2020	Sanders	A41D 13/1153 D29/110
2001/0032348	A1 *	10/2001	Diaz	A41D 13/1153 2/171.3
2006/0213523	A1 *	9/2006	VanDerWoude	A42B 3/286 128/863
2007/0060011	A1	3/2007	Daftari et al.		
2009/0151054	A1	6/2009	VanDerWoude et al.		
2013/0283508	A1	10/2013	Durham et al.		
2015/0090254	A1	4/2015	Pavalarajan et al.		
2015/0375019	A1	12/2015	VanDerWoude et al.		
2017/0112224	A1 *	4/2017	Gotti	A42B 3/225
2017/0196281	A1	7/2017	Rosati et al.		
2020/0178622	A1	6/2020	Jascomb et al.		
2020/0375272	A1 *	12/2020	Ulmer	A41D 13/1153
2020/0375281	A1 *	12/2020	Prevot	A62B 23/02

OTHER PUBLICATIONS

Vivi, "Protection you barely notice.", first available Jul. 2017. (<http://www.surgicalspecialties.com.au/system/resources/W1siZils1j1wMjAvMDMvMTcvMjNfMjhfMjBfMjk2X1NTMDAyMV9WaVZpX1Byb3RlY3Rpb25fWW91X0JhcmVseV9Ob3RyY2UucGRml1d/SS0021—ViVi Protection You Barely Notice.pdf>) (Year: 2017).*

Vimeo, "Stryker—Surgical Helmet Teaser", first available Dec. 5, 2019. (<https://vimeo.com/377677640>) (Year: 2019).*

Kaiser, "Surgical Helmet", first accessed Apr. 1, 2021. (<https://www.kaiser-tech.com.tw/5-01-surgical-helmet>) (Year: 2021).*

Bio-Medical Devices Intl, "MaxAir Systems 2270-01 Pre-Filter DLC Hood Instructions for Use", Available on or before Apr. 2017, 3 pages.

International Search Report for Application No. PCT/US2019/015128 dated Jun. 21, 2019, 5 pages.

Non-Final Office Action for U.S. Appl. No. 16/223,523, dated Jul. 11, 2019, 14 pages.

United States Non-Provisional U.S. Appl. No. 16/257,668, filed Jan. 25, 2019.

* cited by examiner

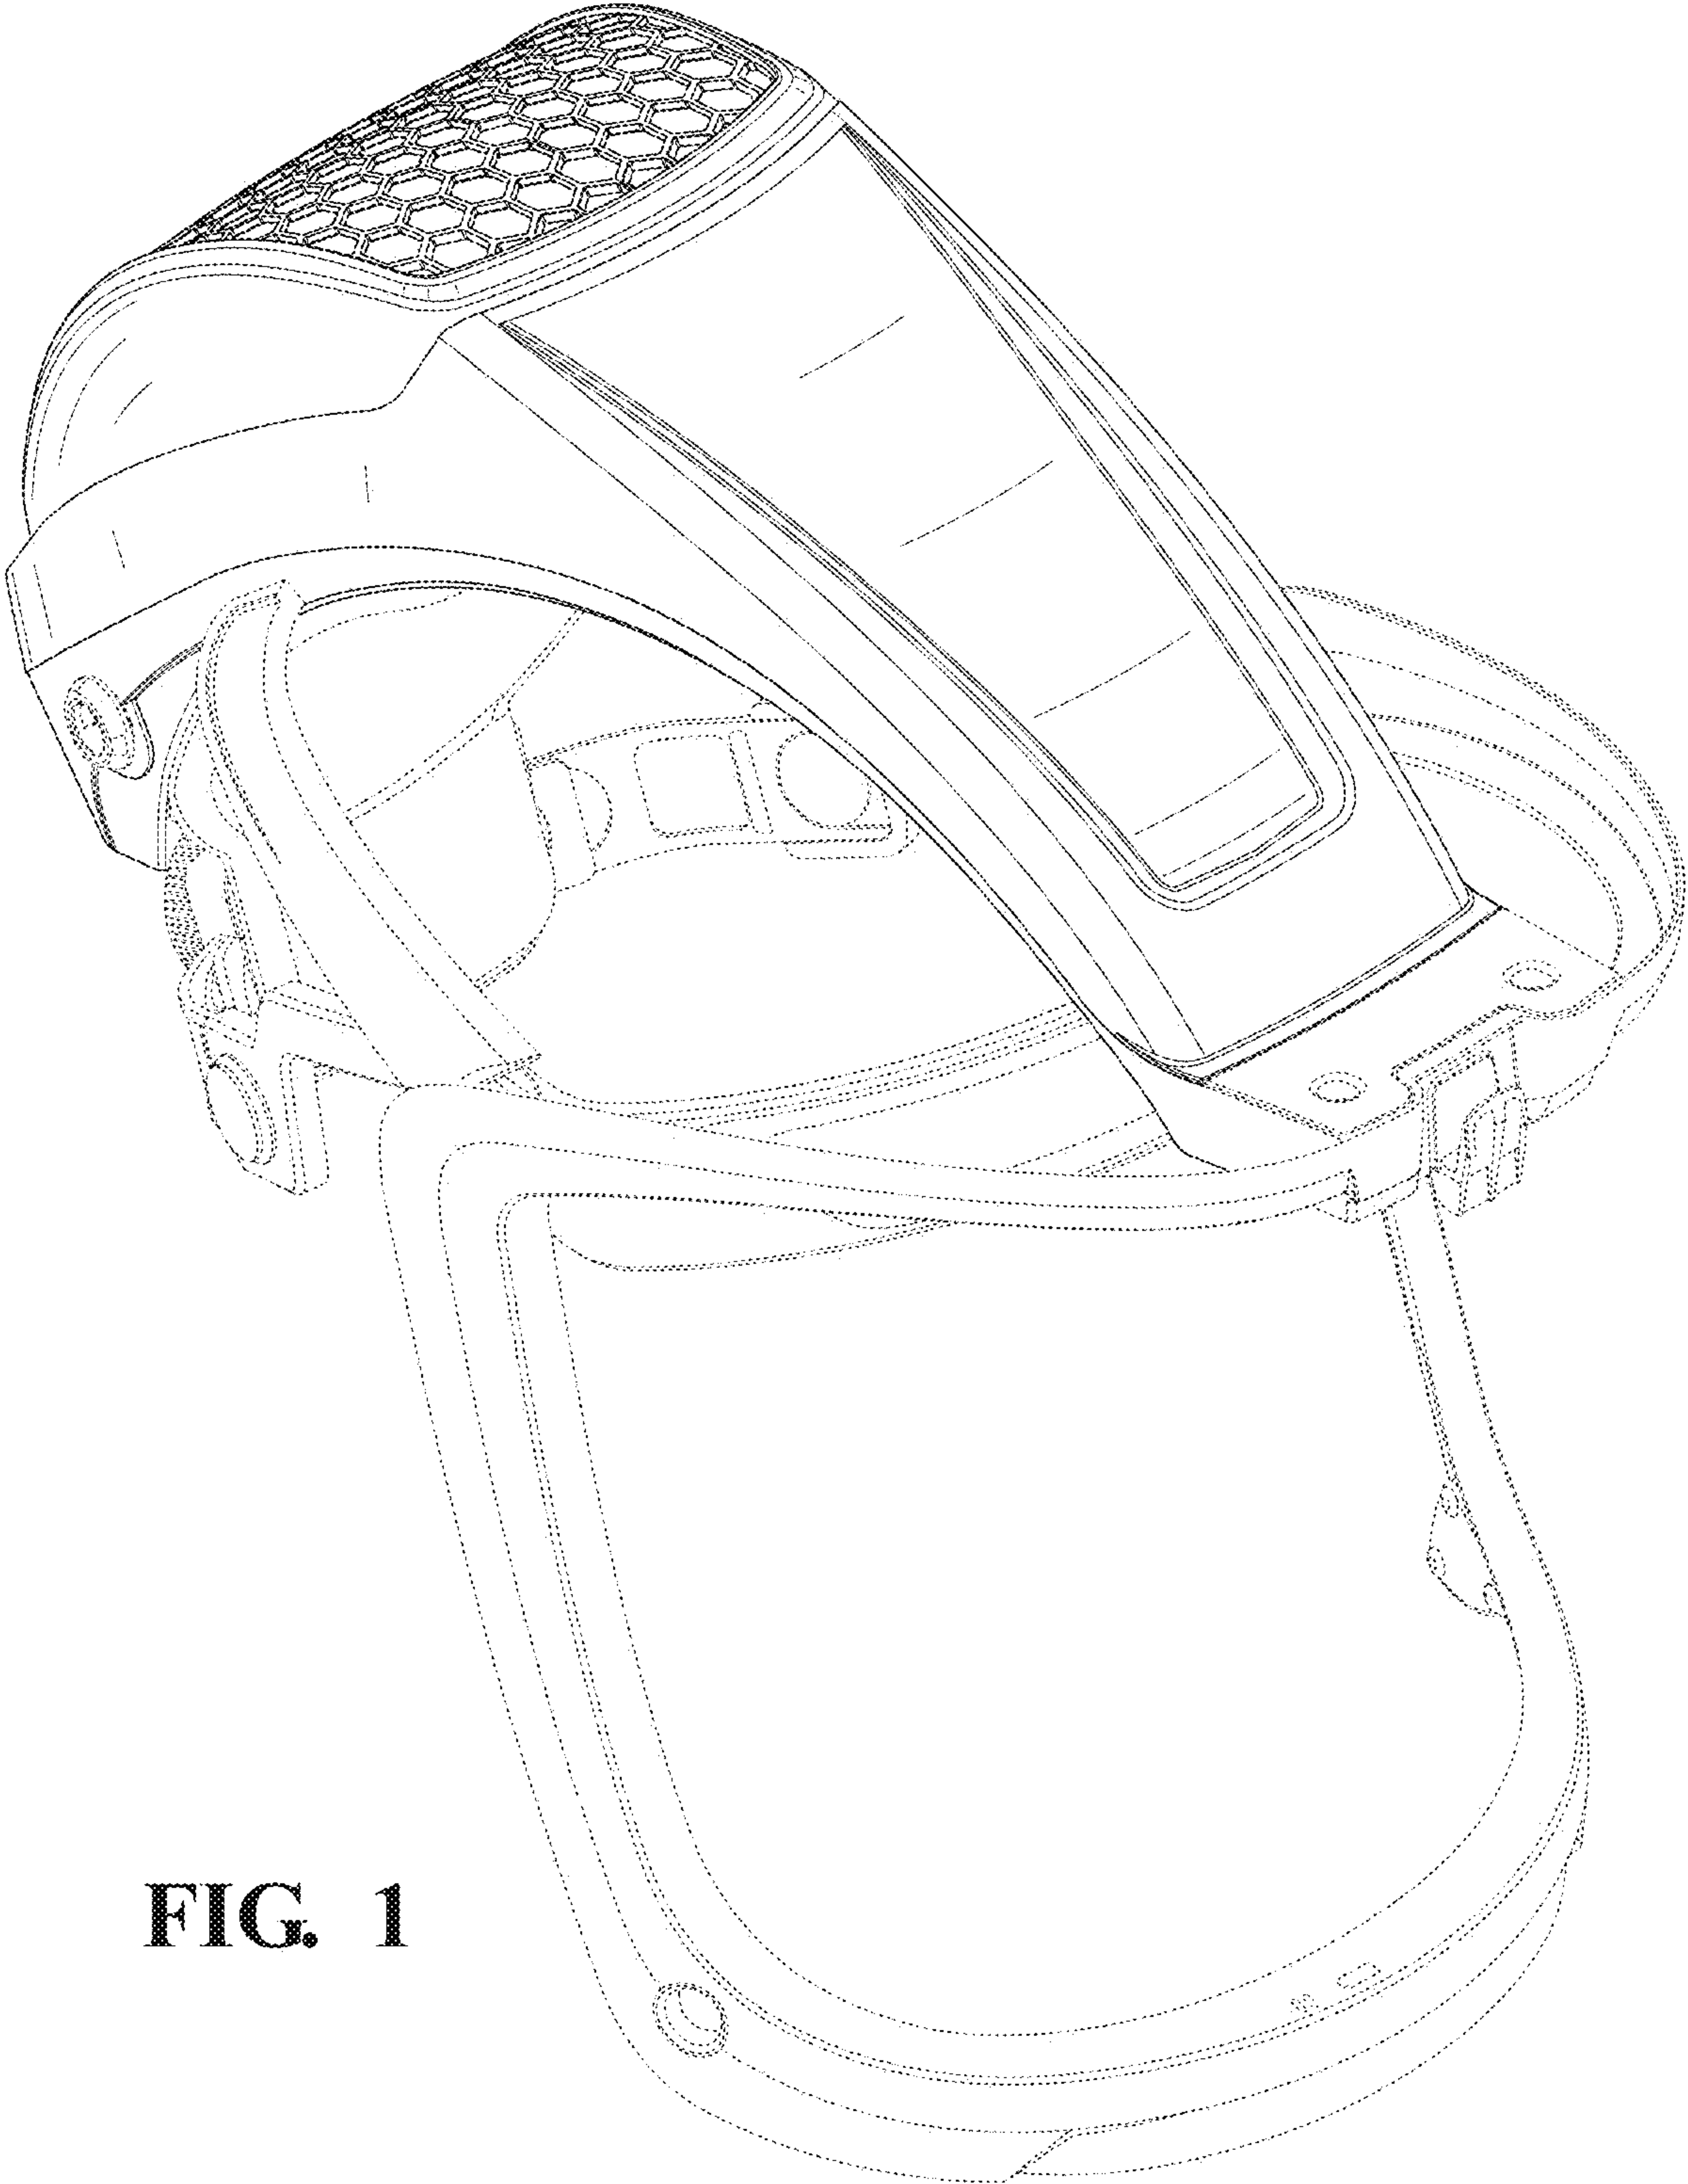


FIG. 1

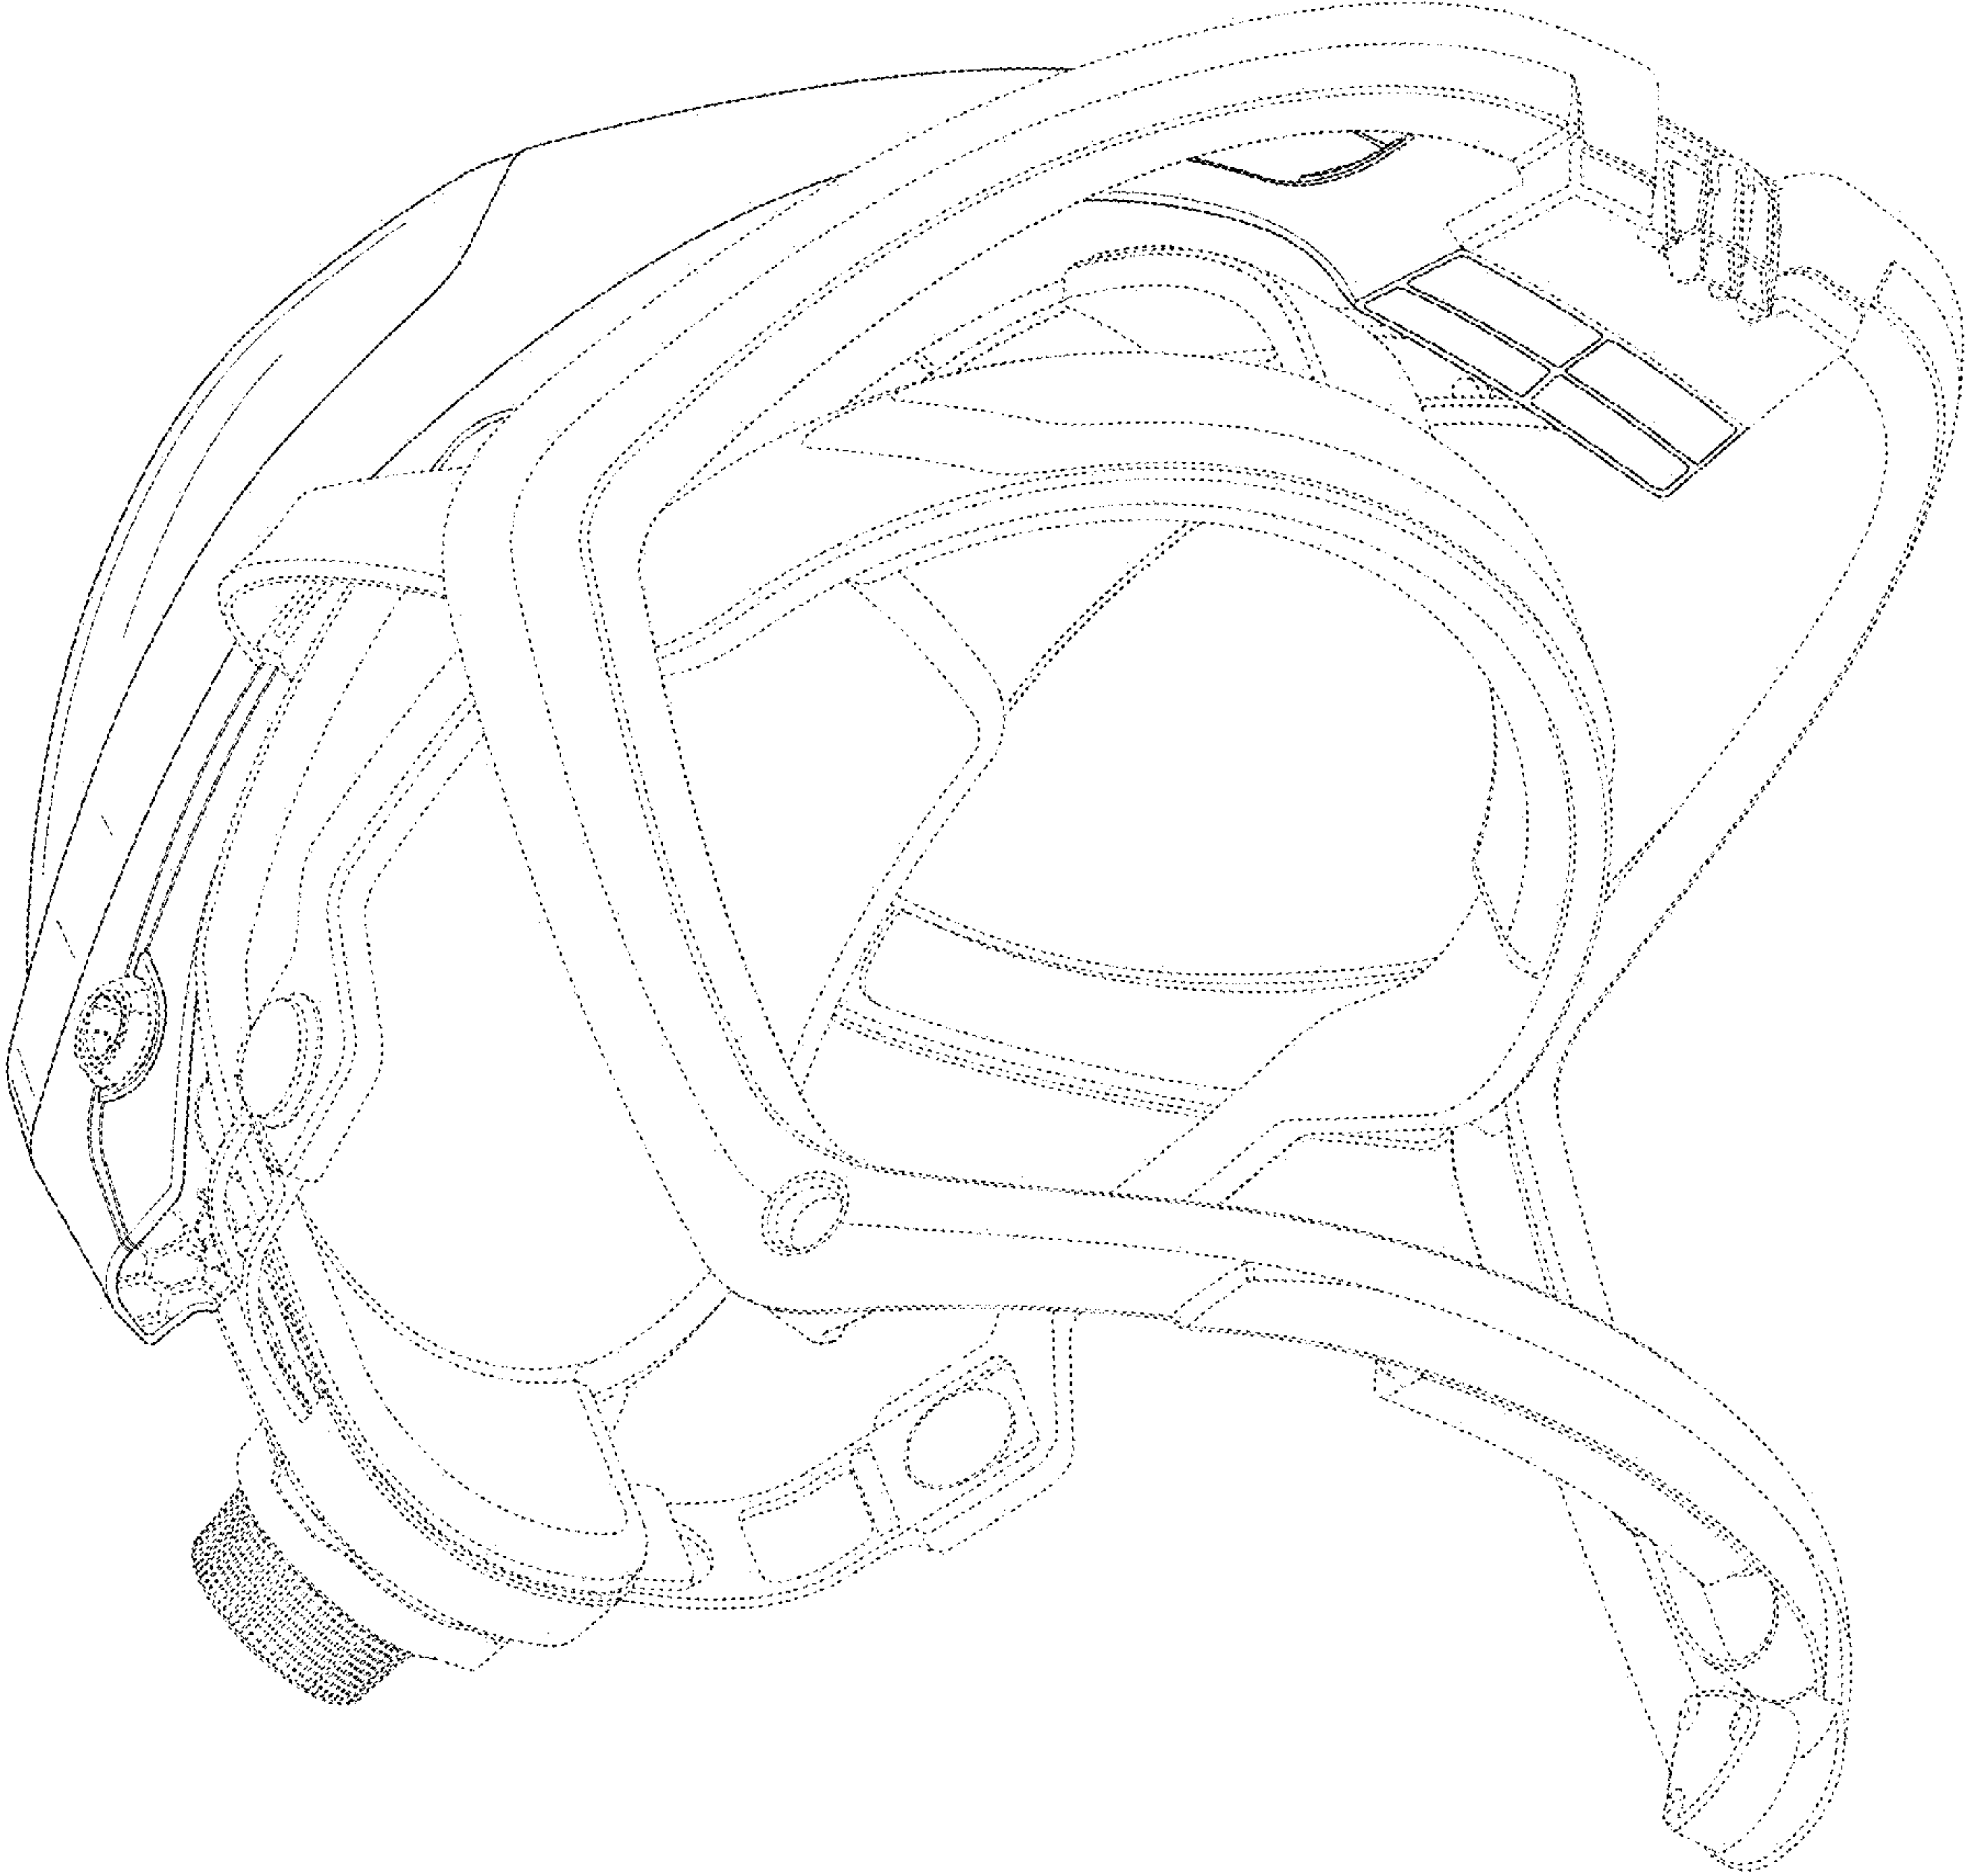


FIG. 2

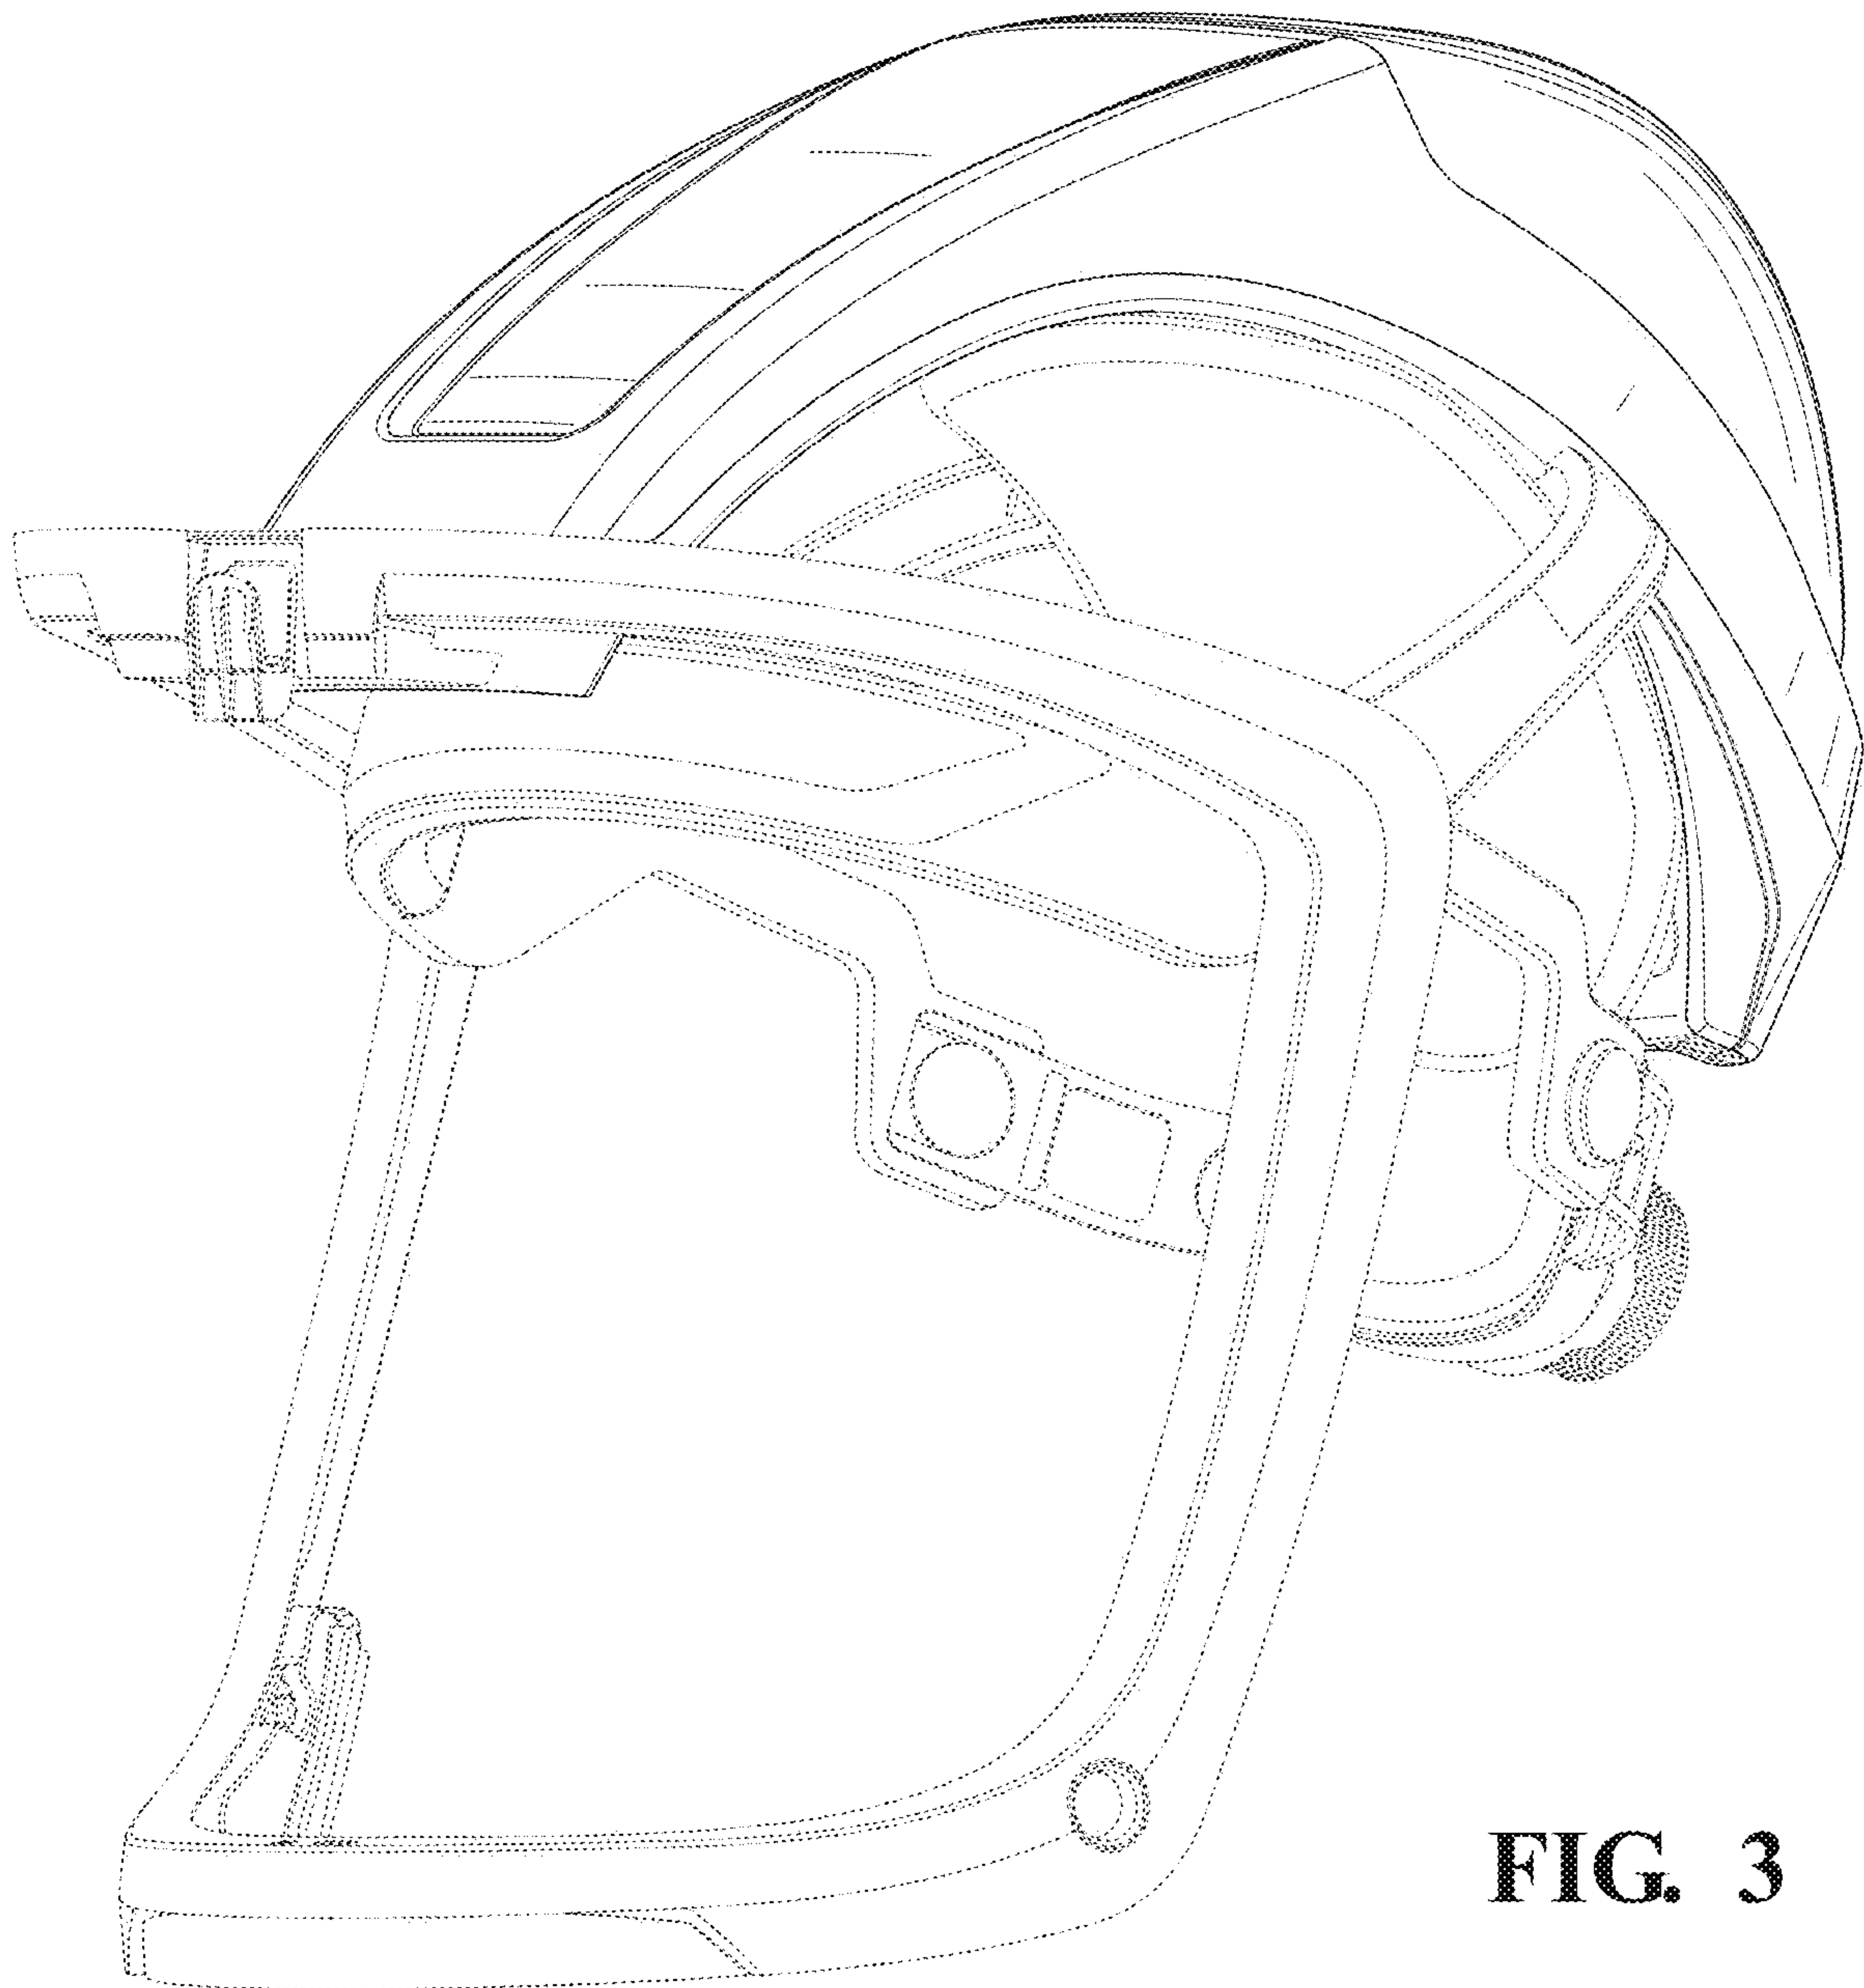


FIG. 3

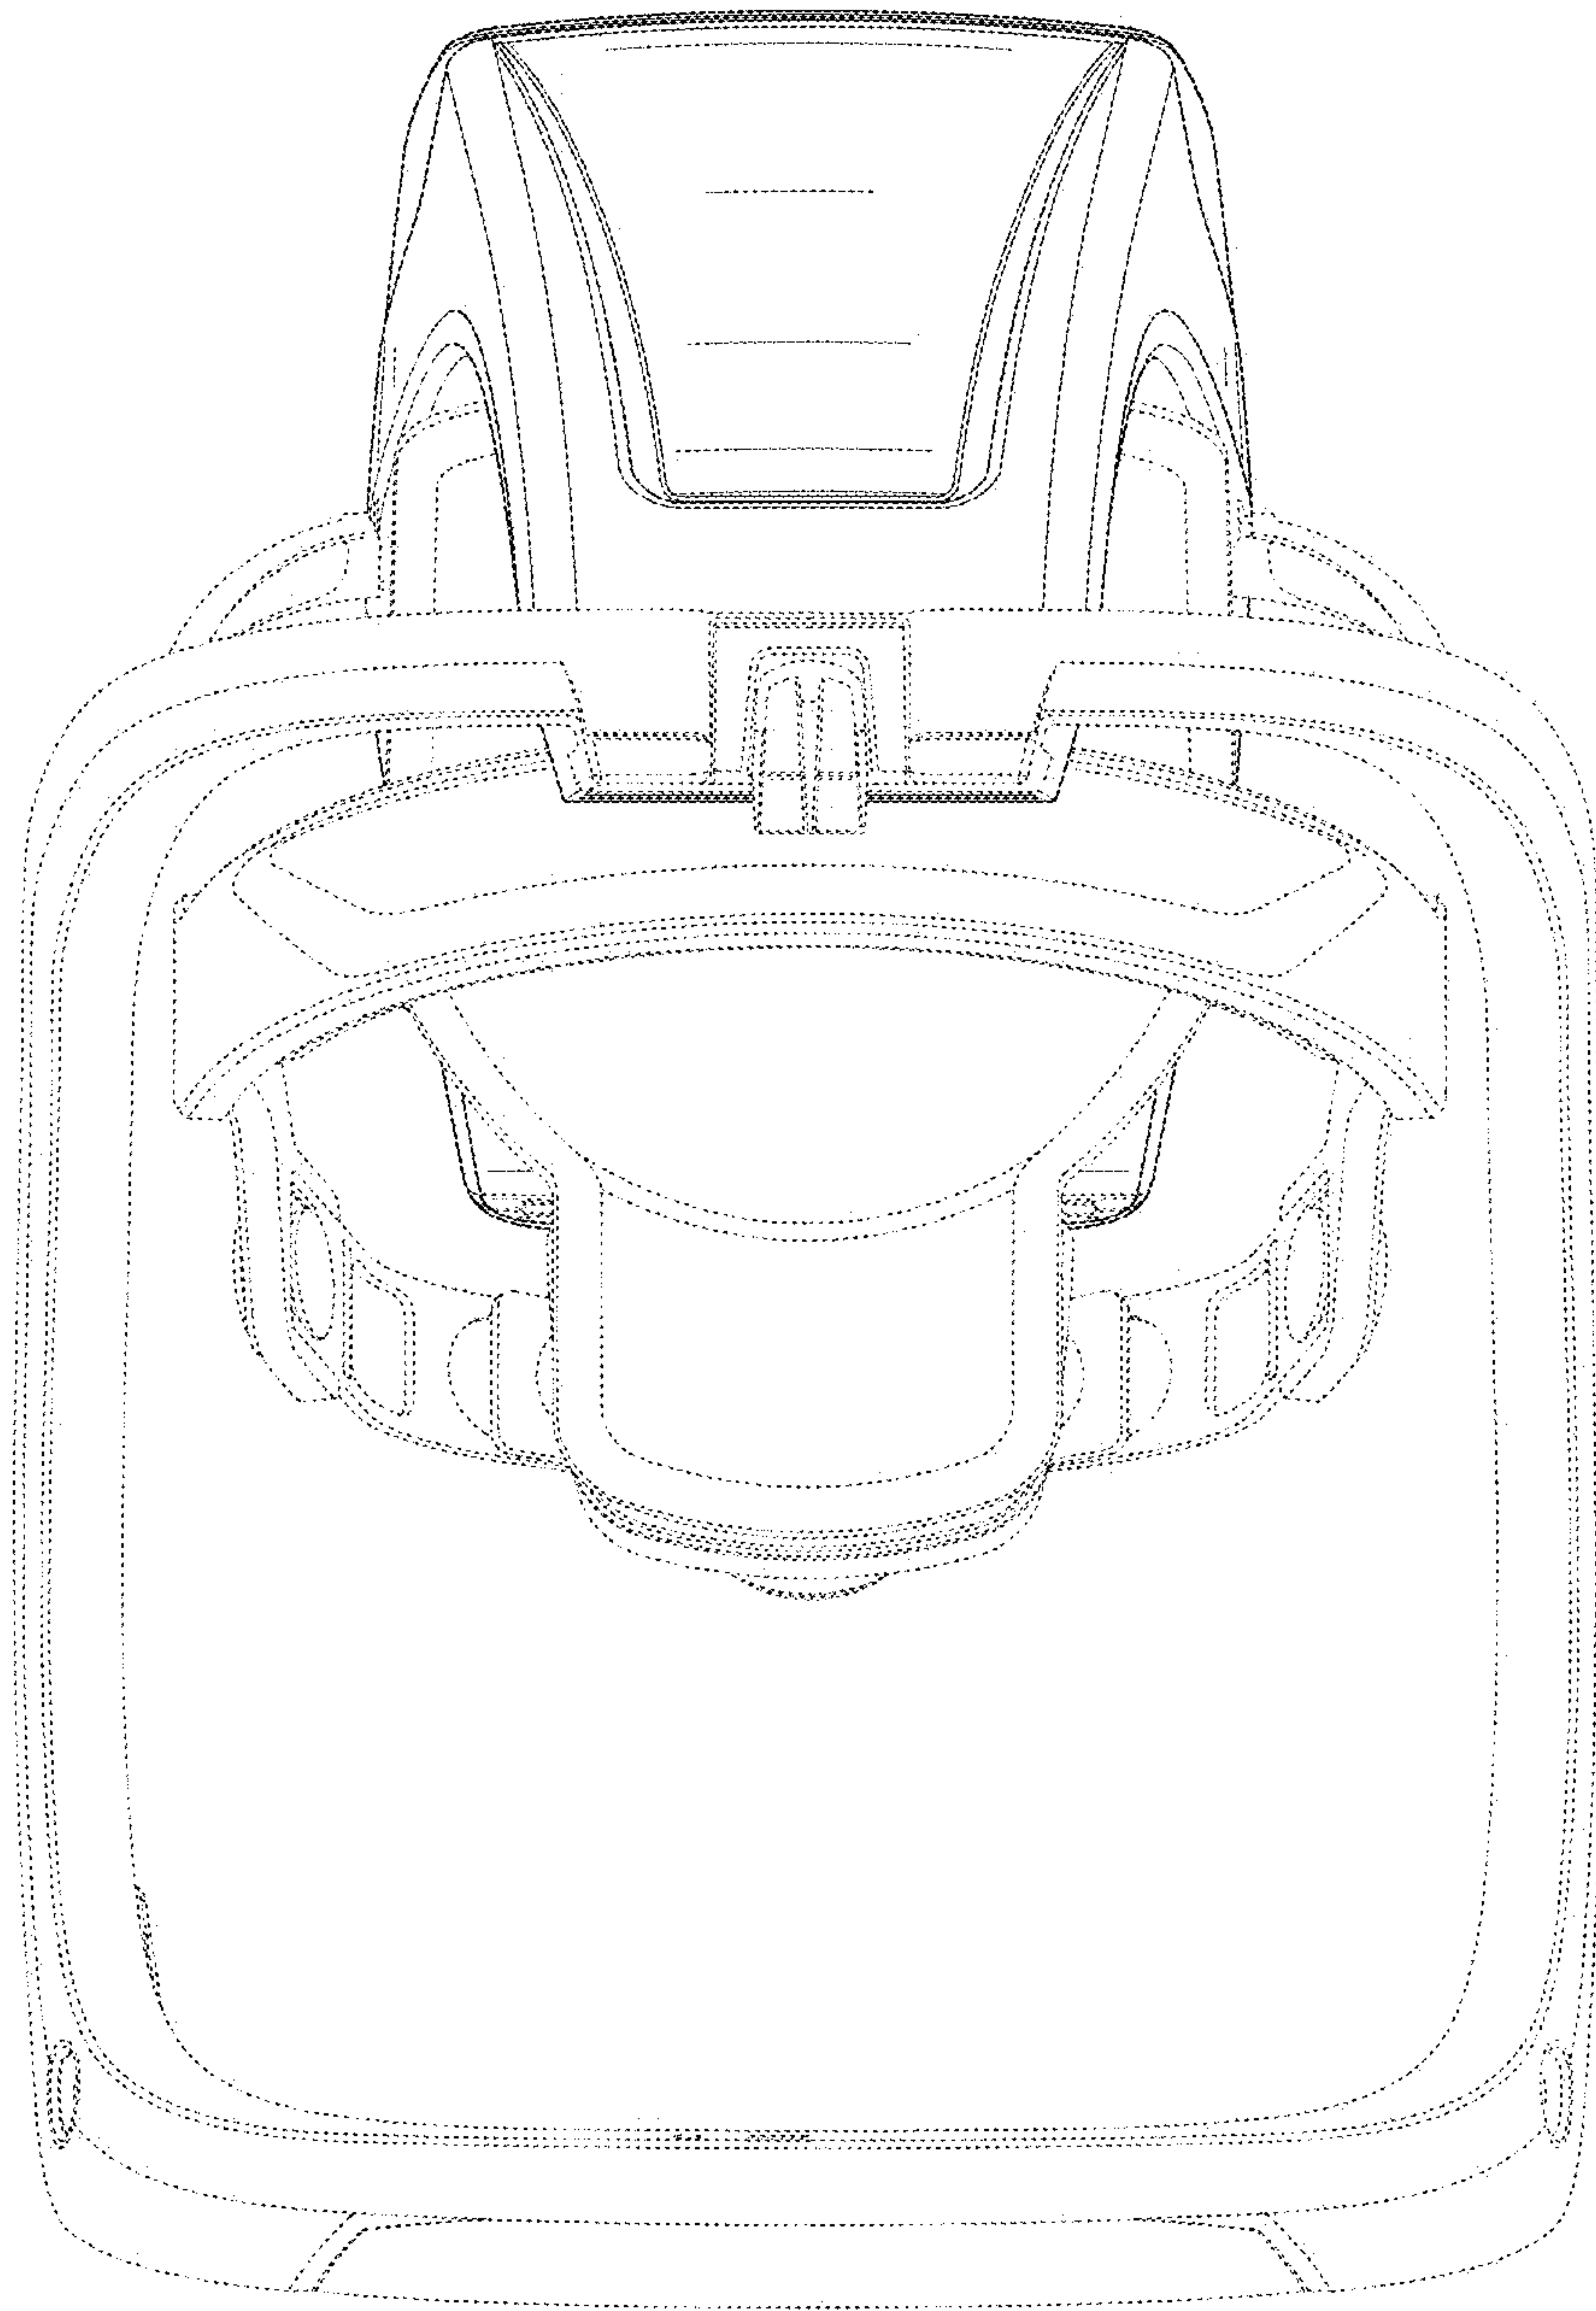


FIG. 4

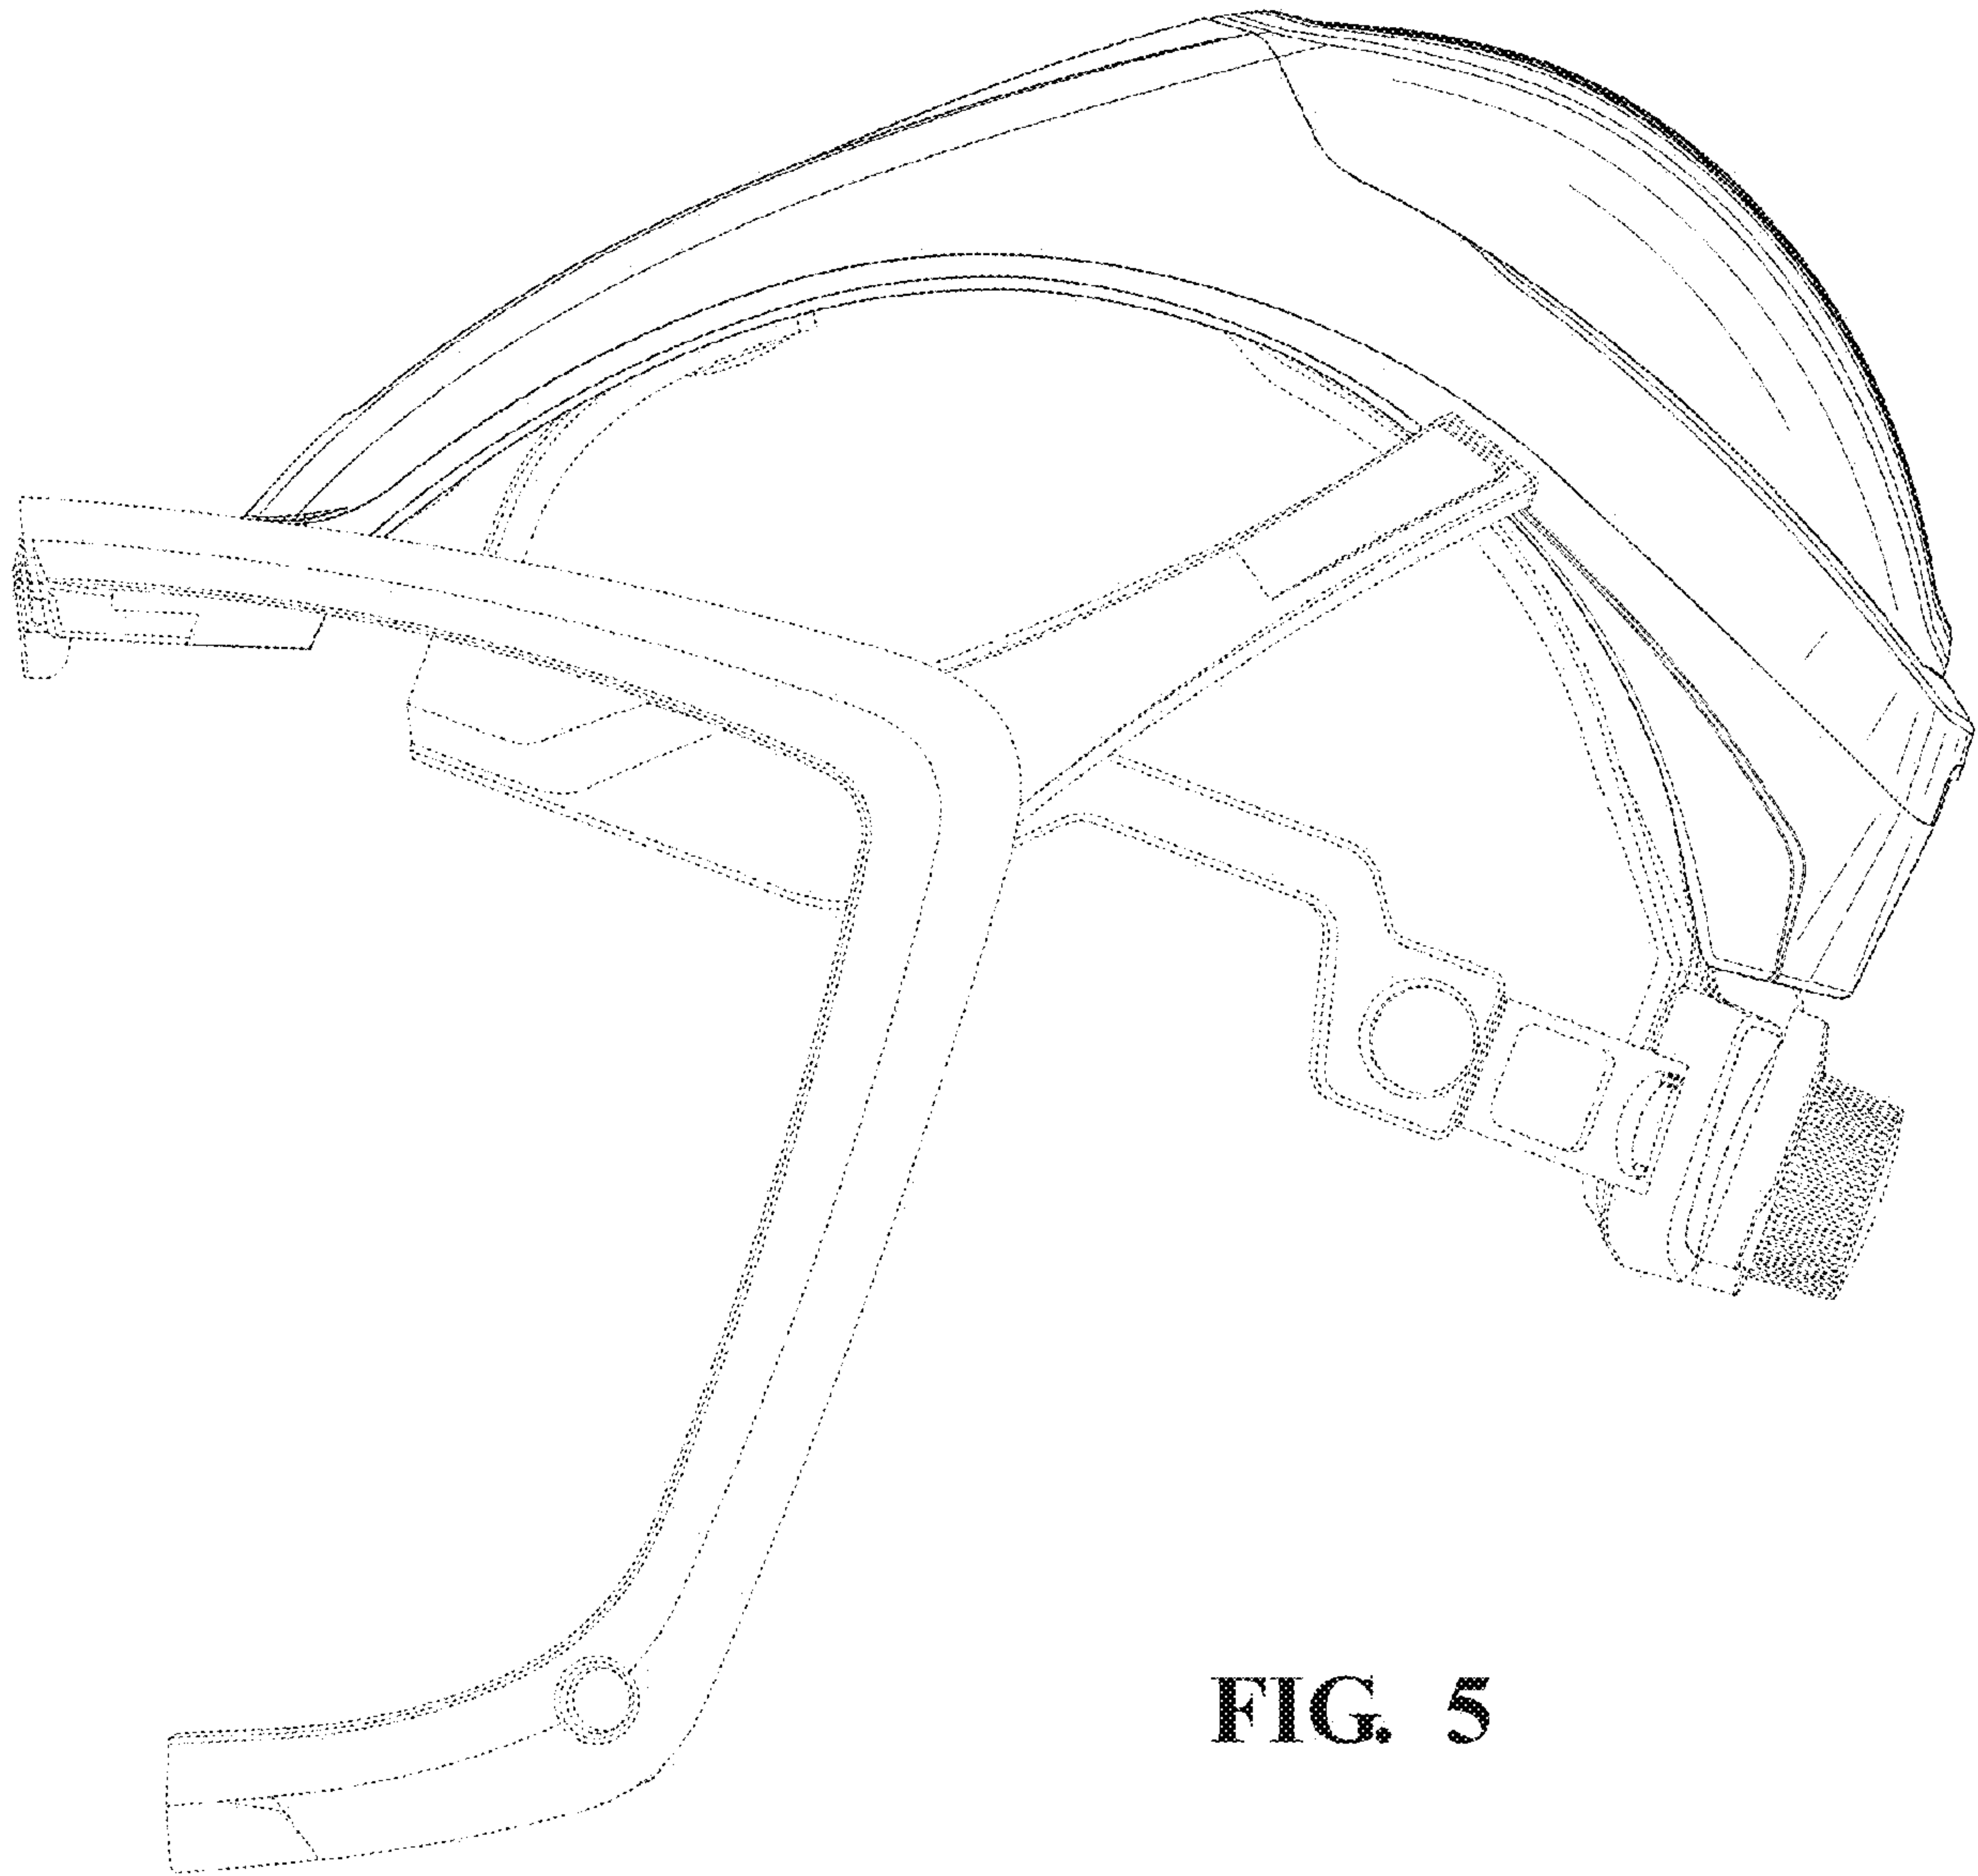


FIG. 5

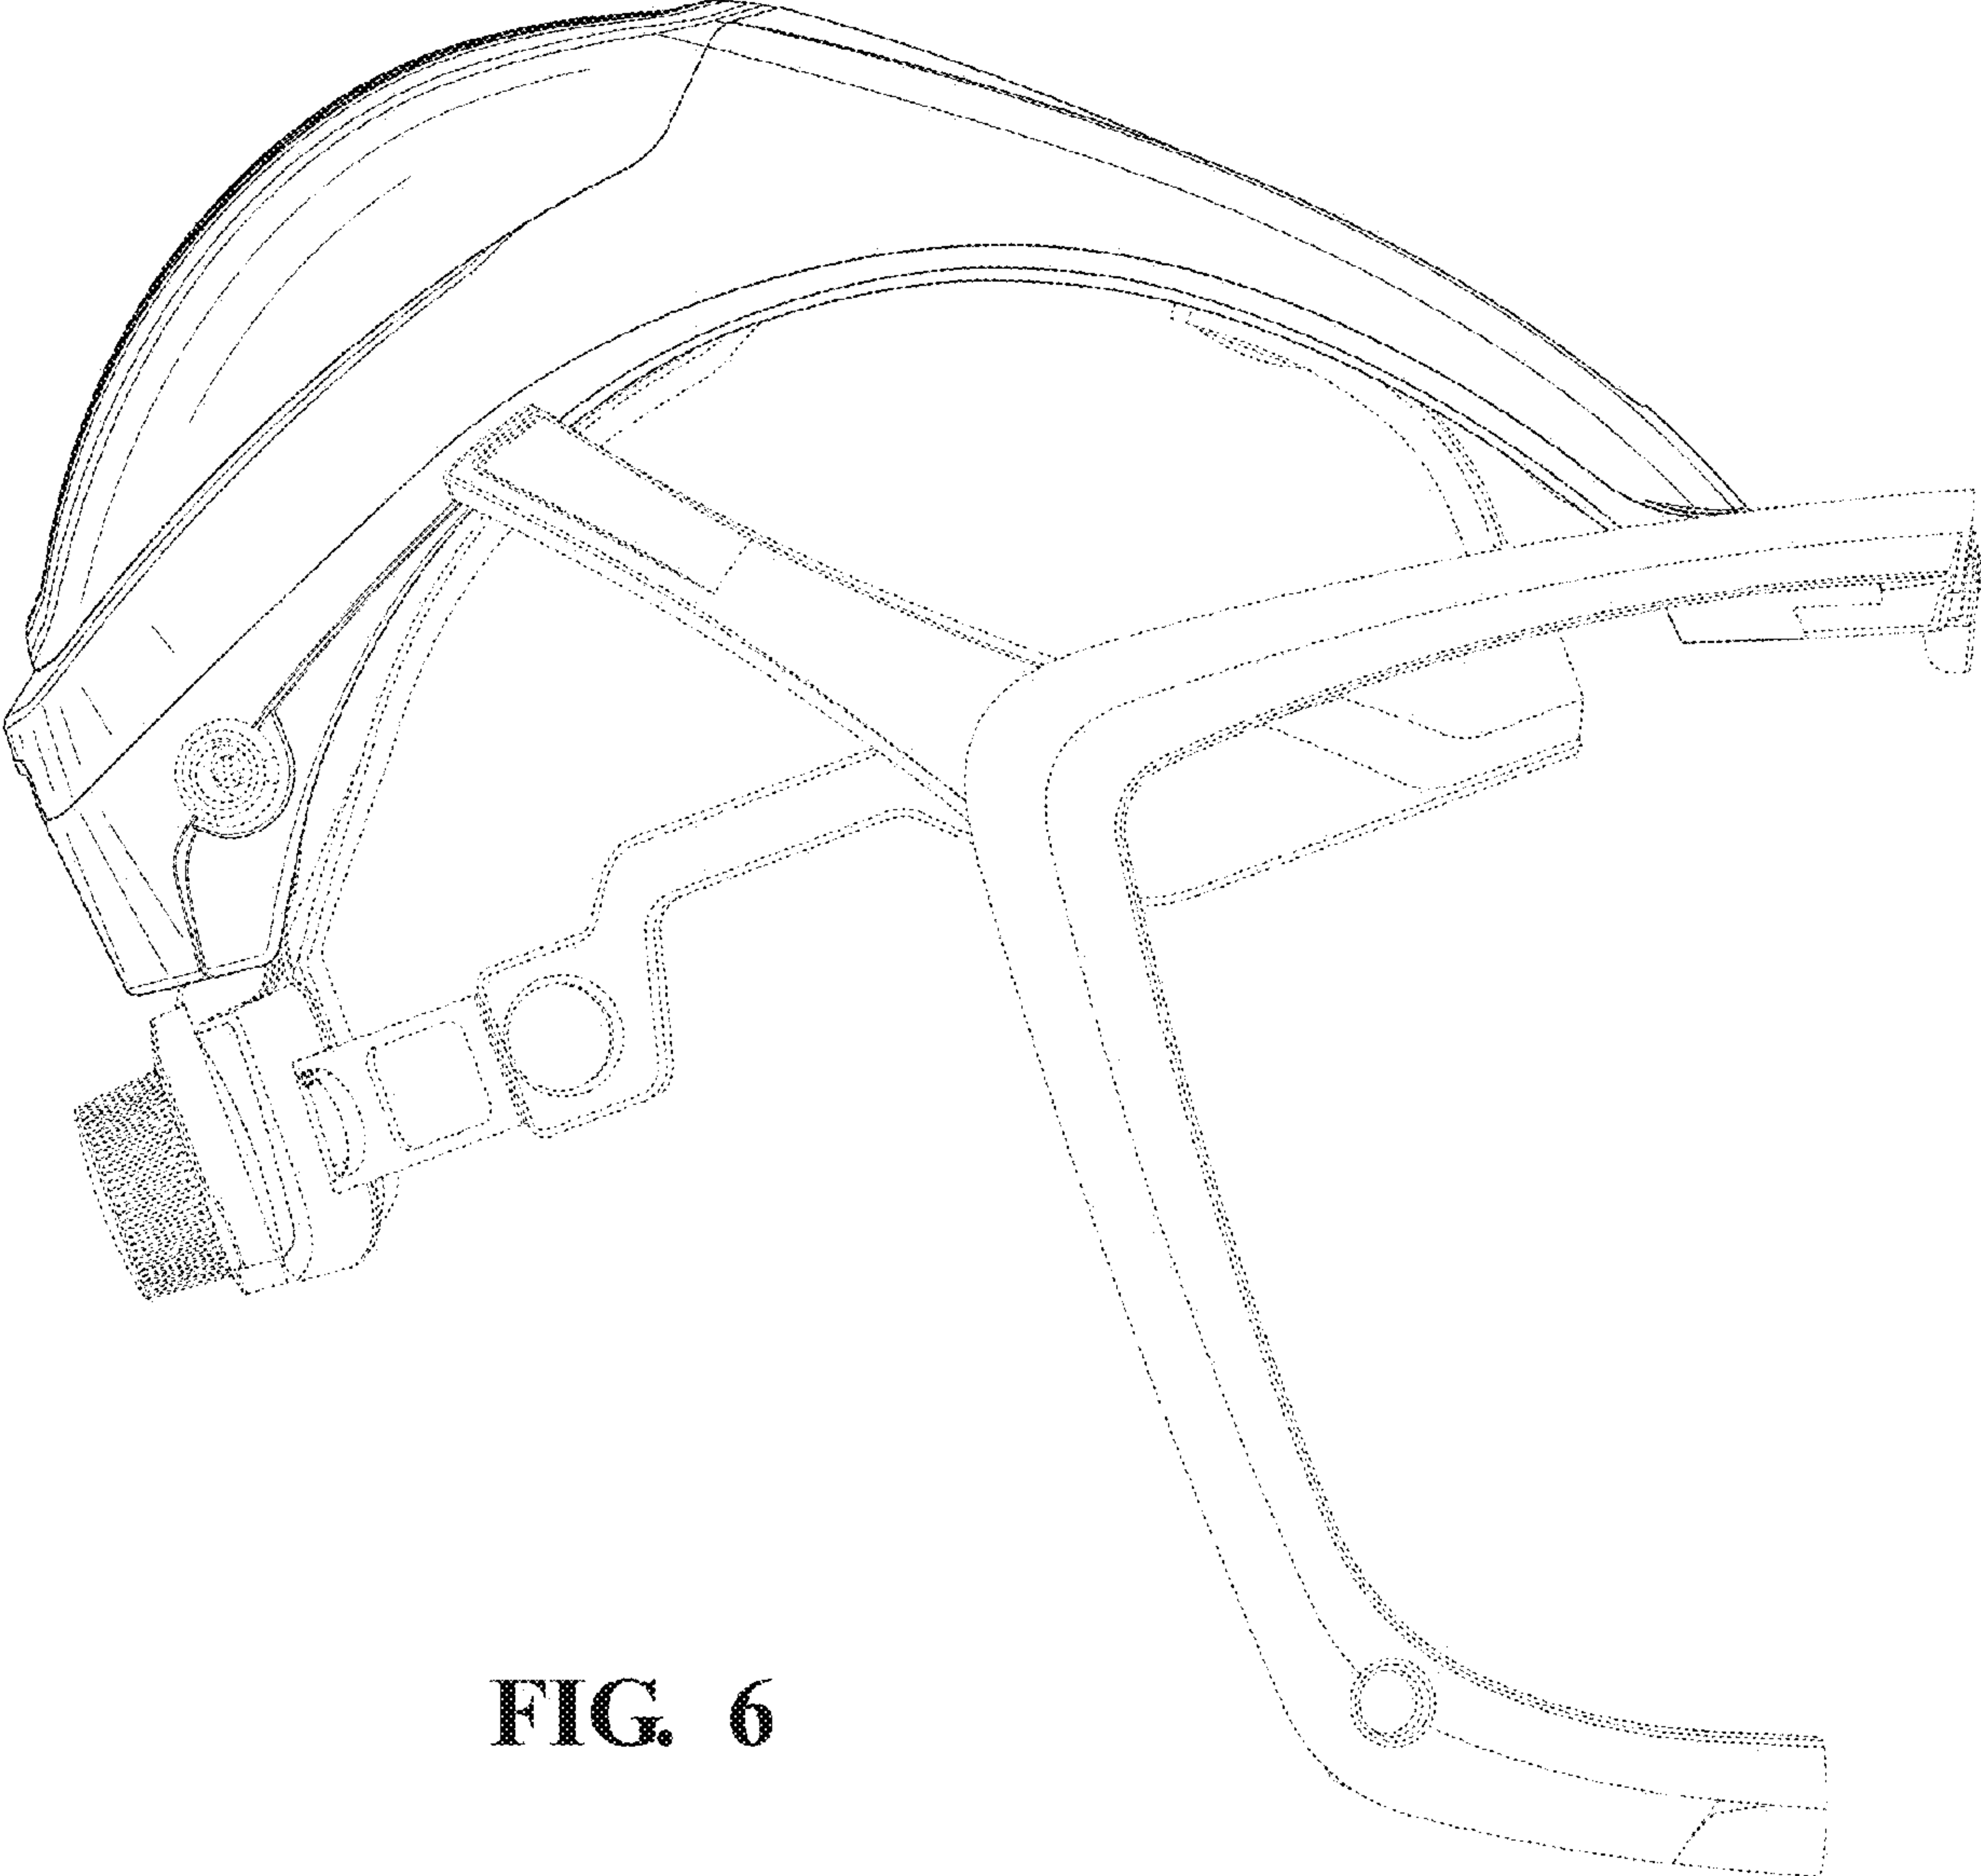


FIG. 6

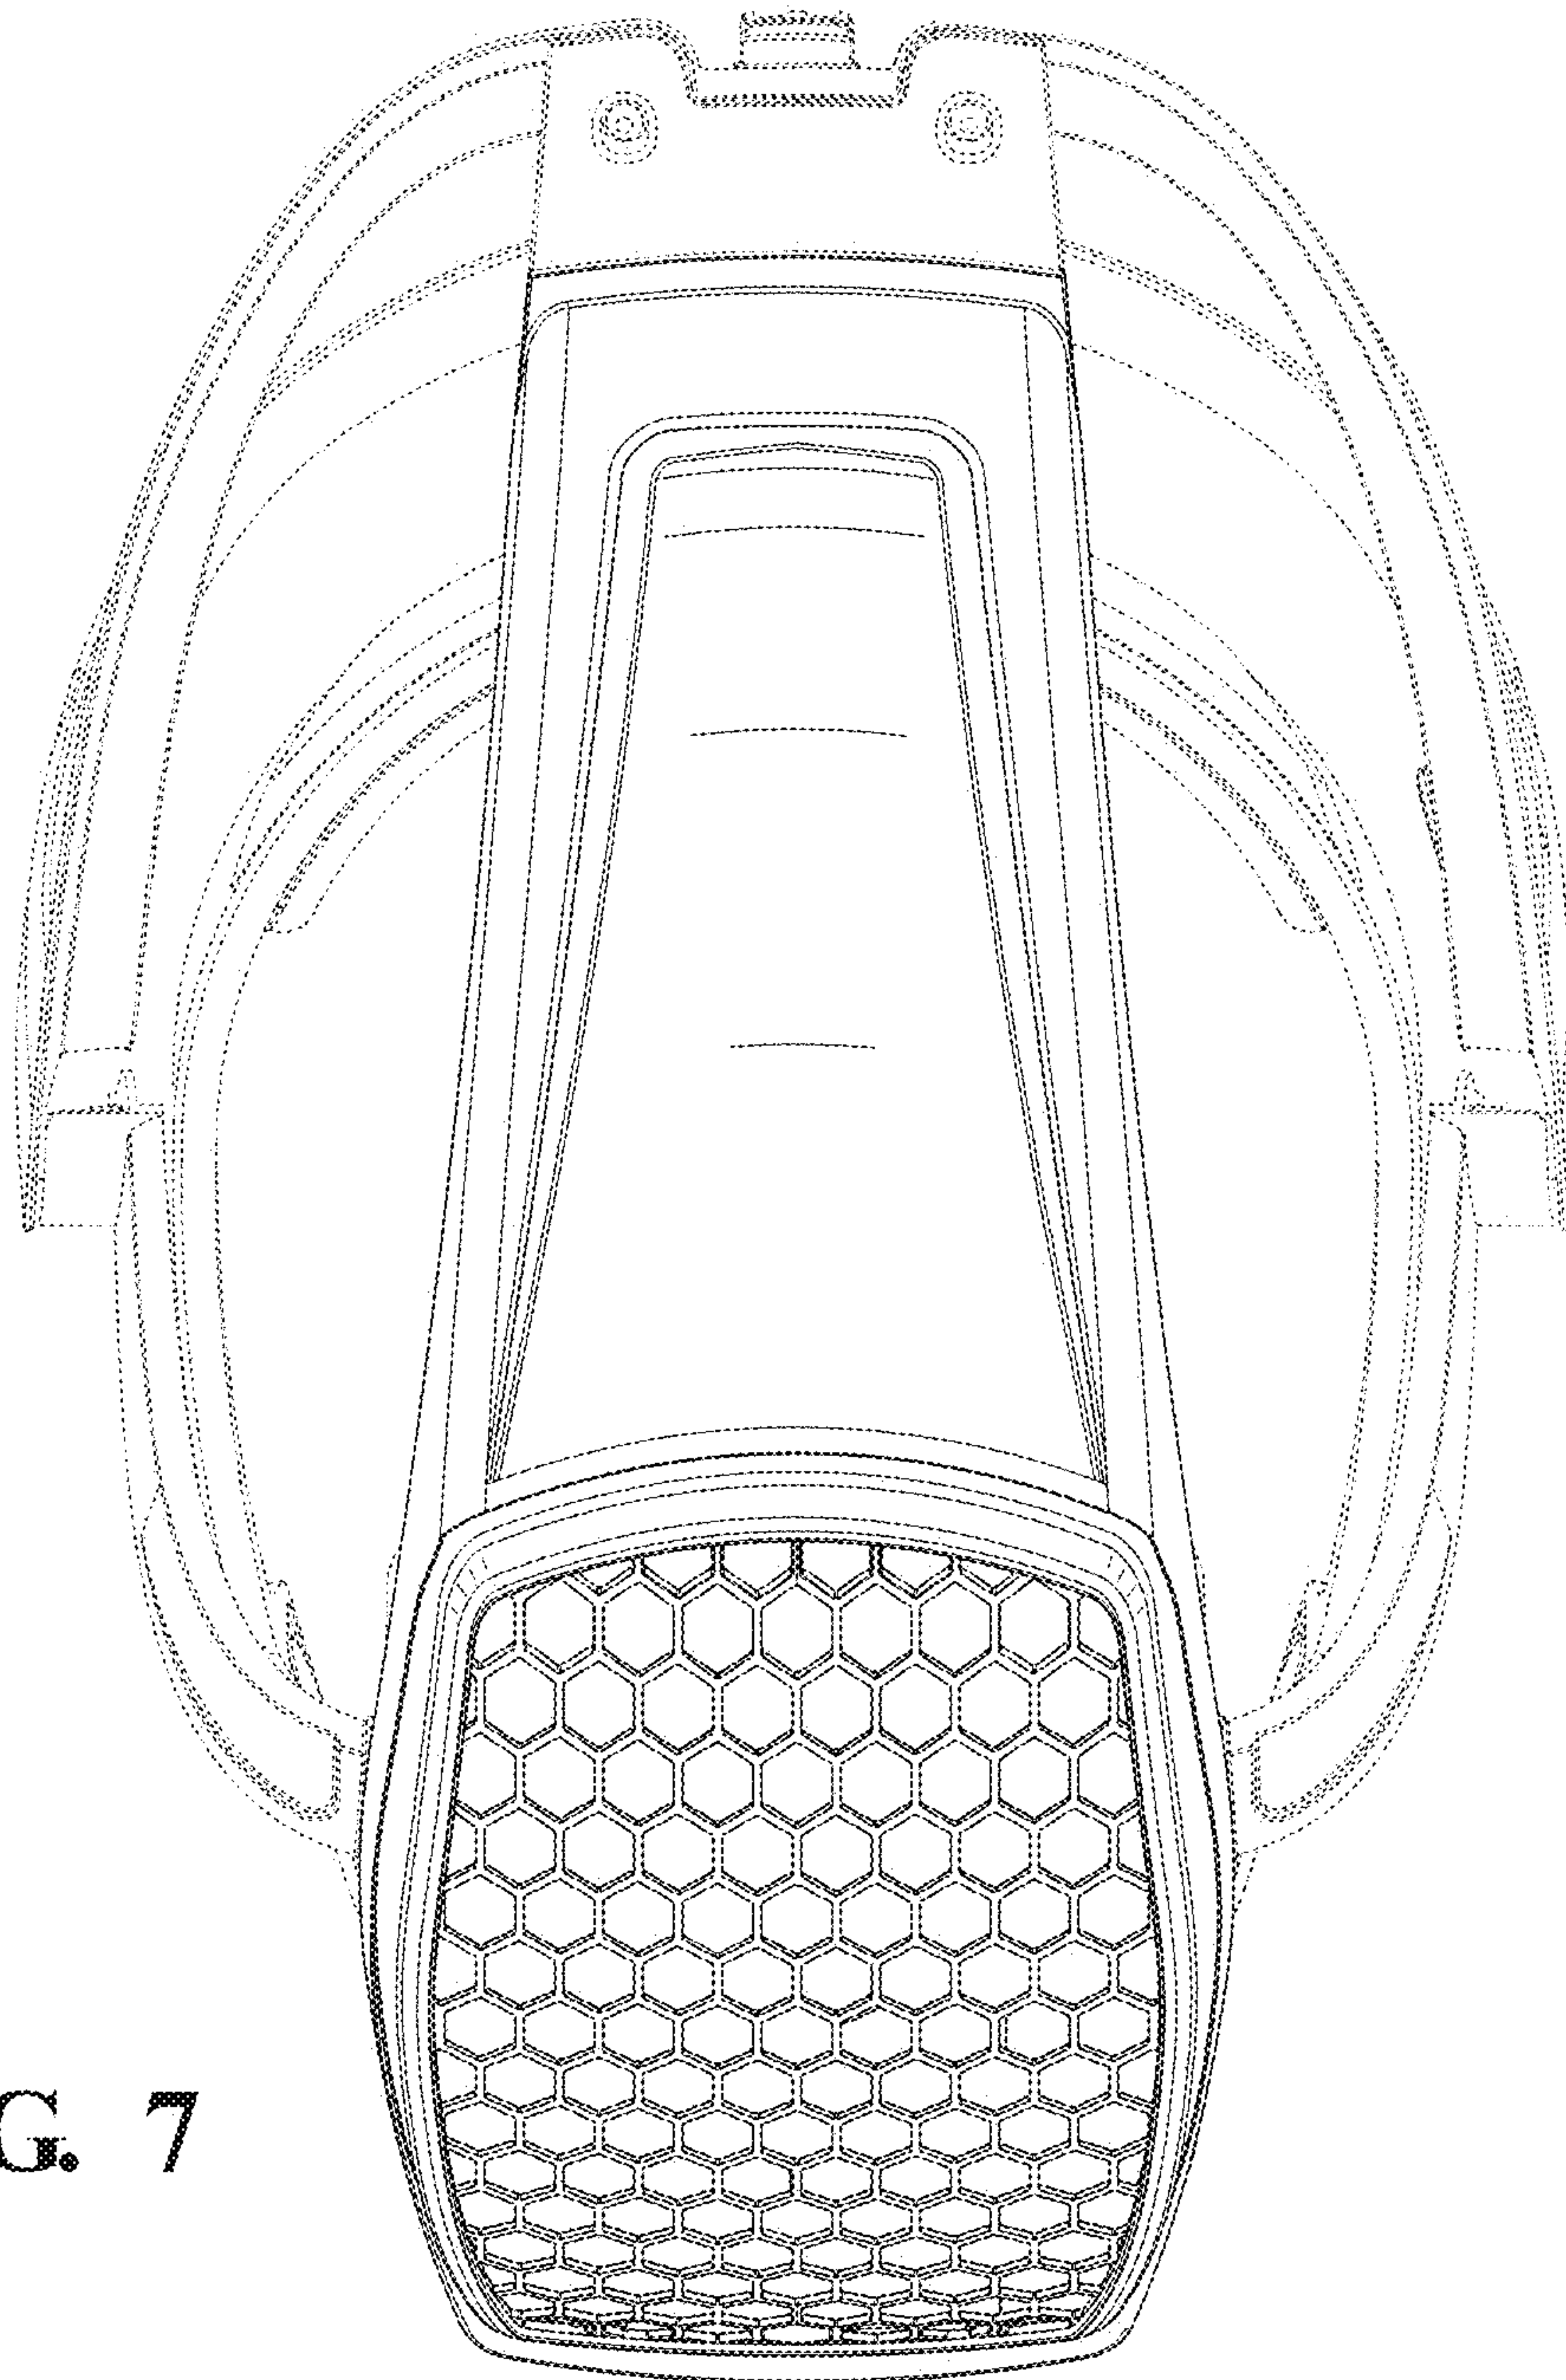


FIG. 7

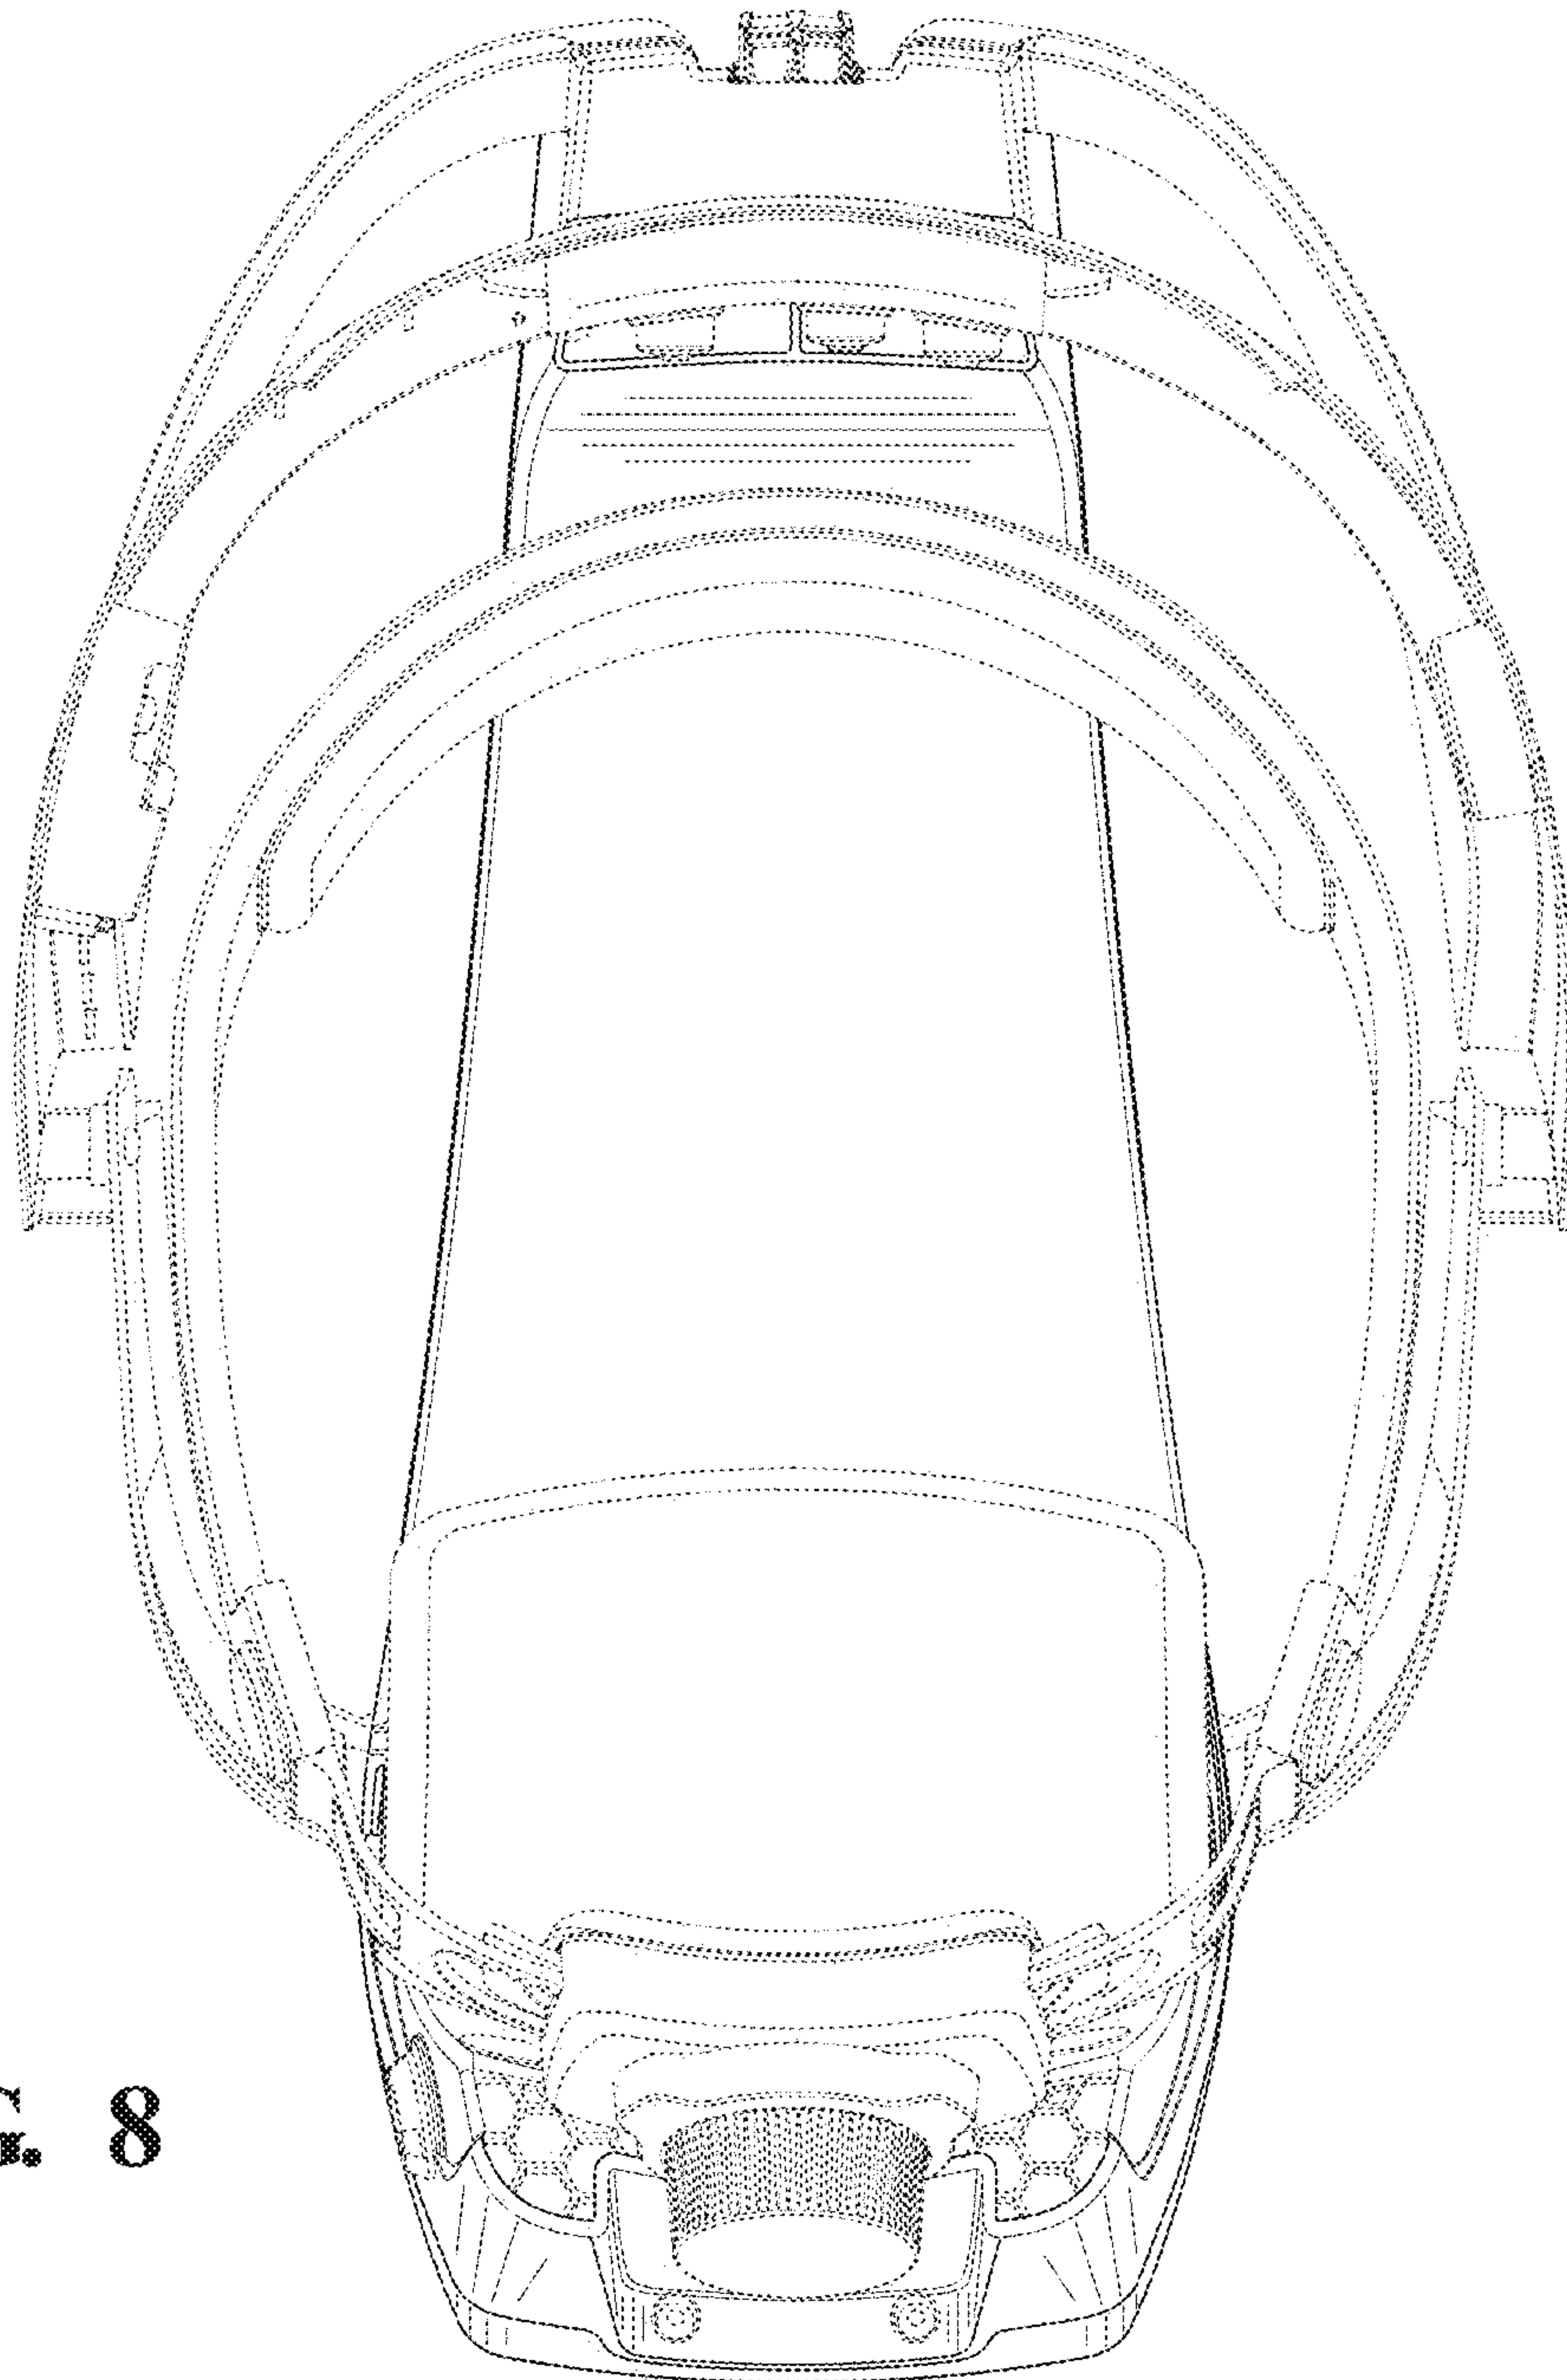


FIG. 8

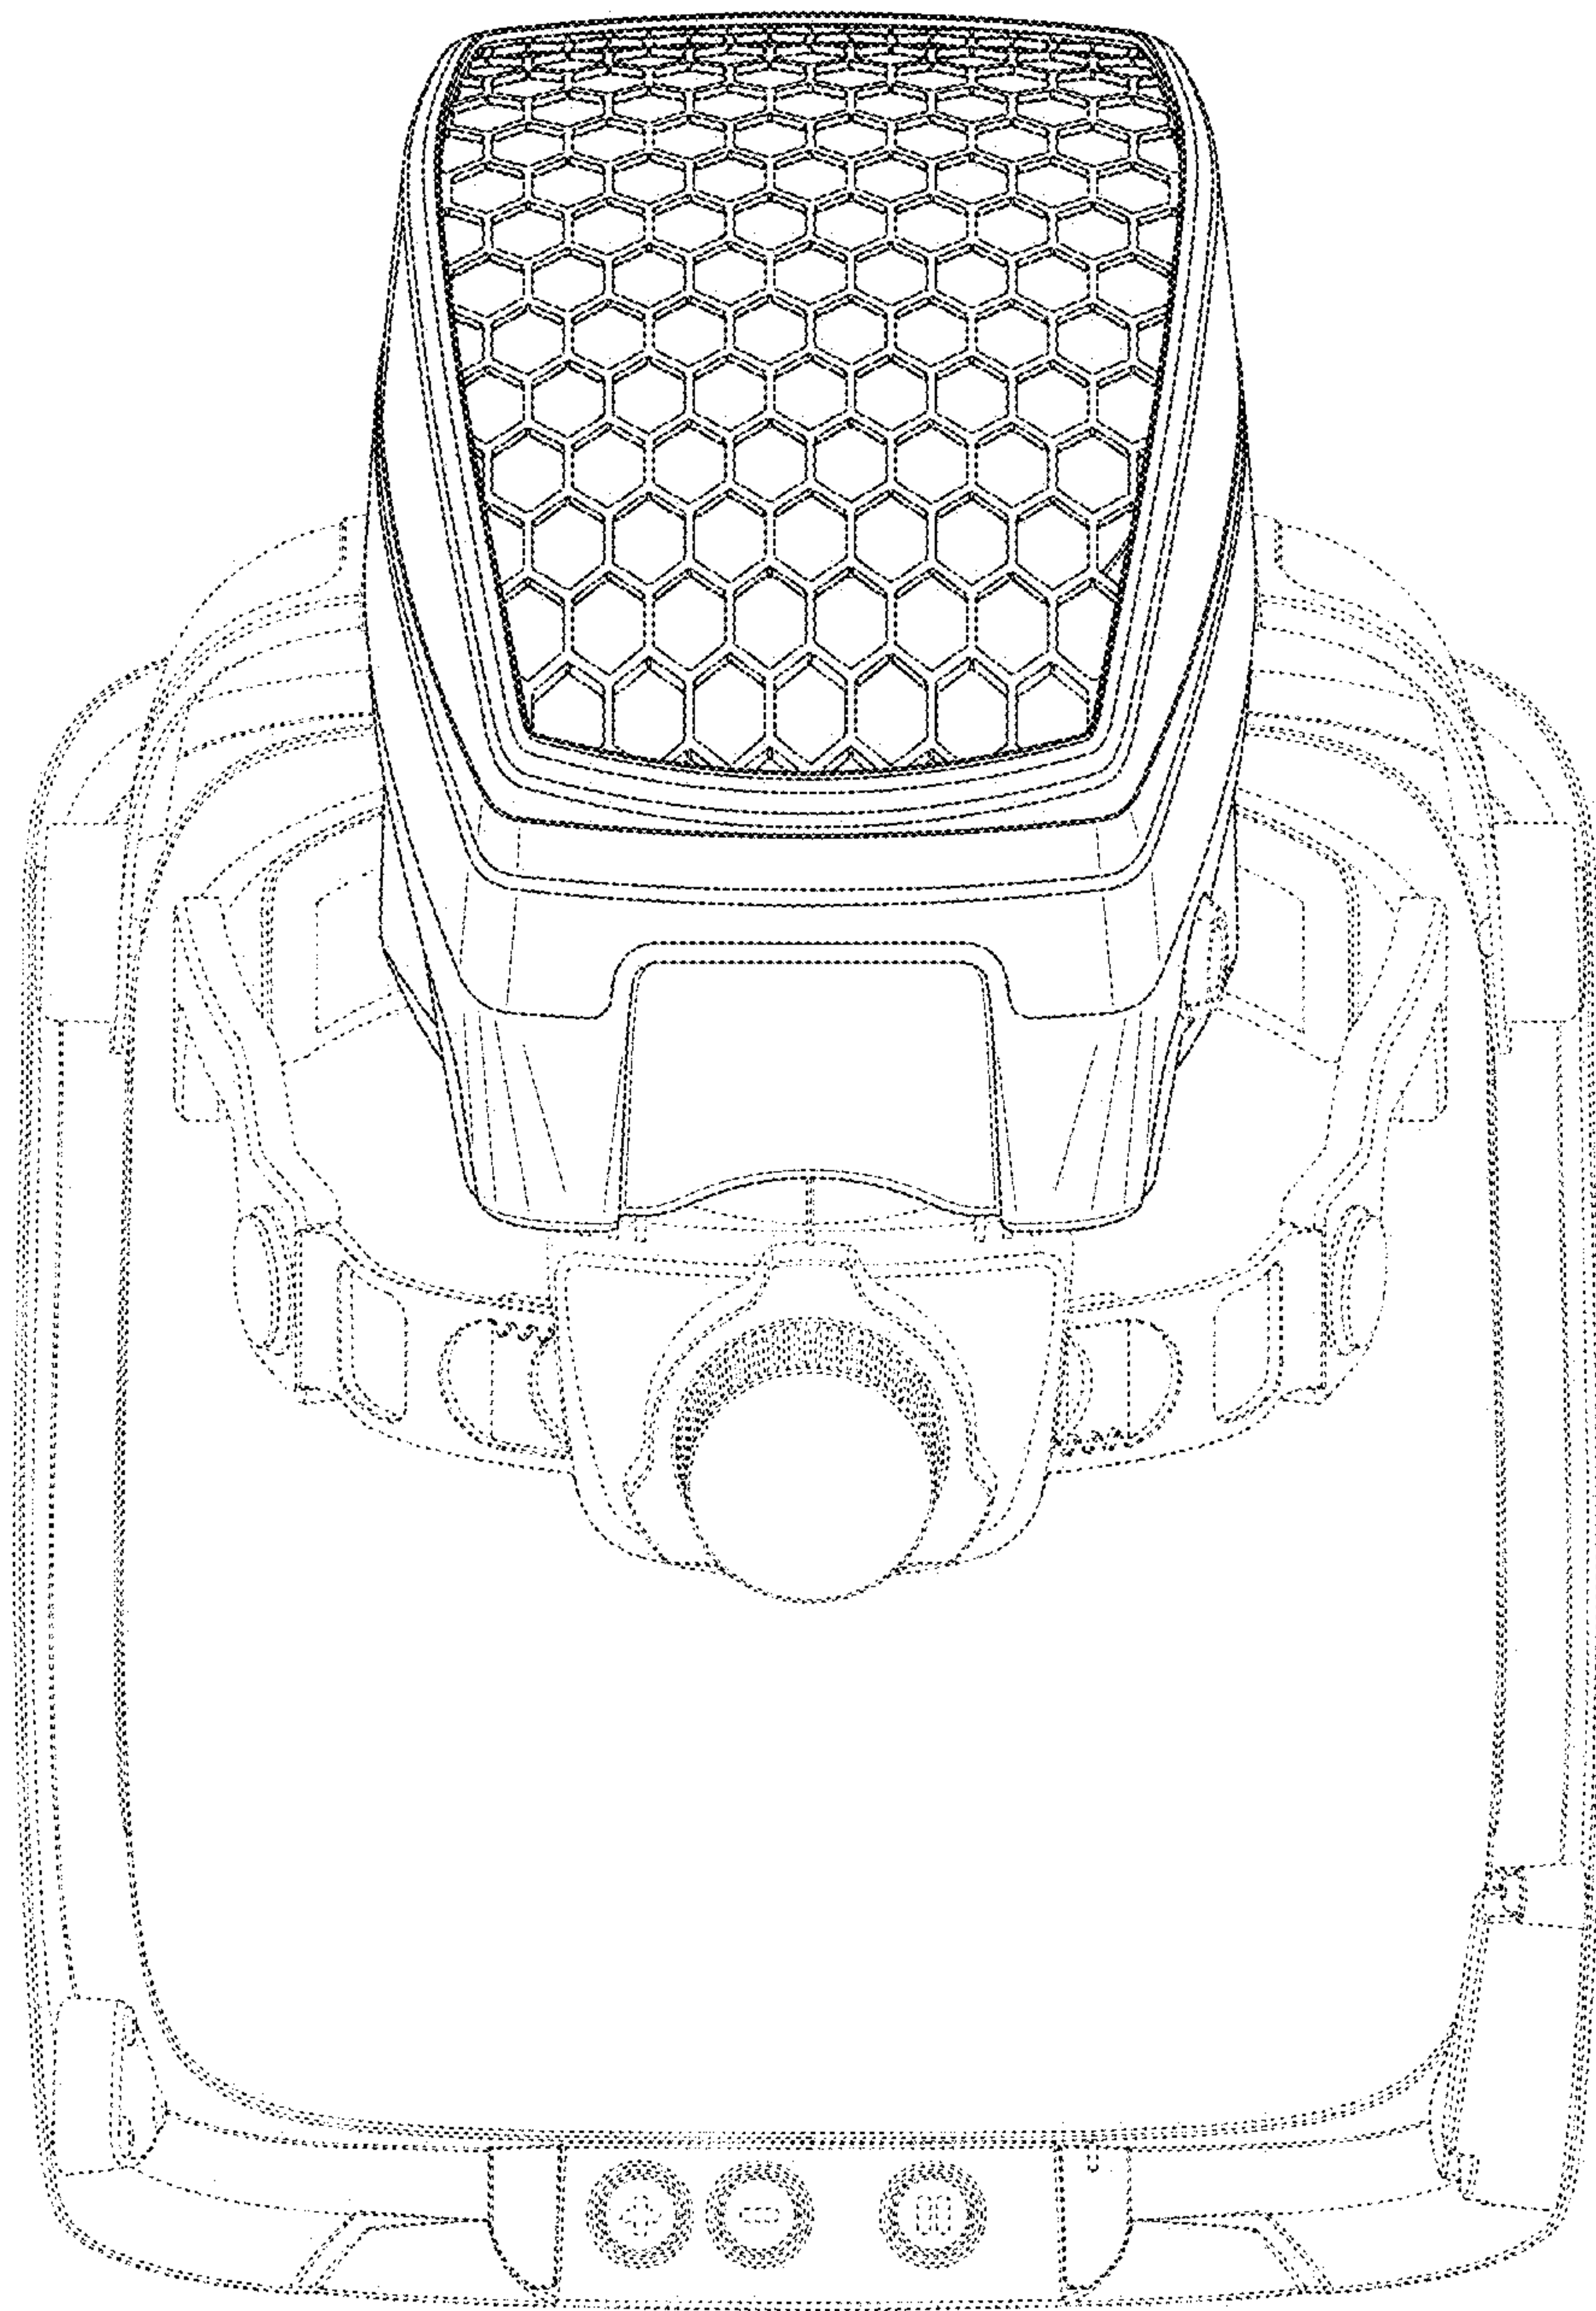


FIG. 9