



US00D979758S

(12) **United States Design Patent**  
**Hirasawa et al.**

(10) **Patent No.:** **US D979,758 S**

(45) **Date of Patent:** **\*\* Feb. 28, 2023**

(54) **SPHYGMOMANOMETER**

(71) Applicant: **OMRON HEALTHCARE Co., Ltd.**,  
Kyoto (JP)

(72) Inventors: **Asa Hirasawa**, Kyoto (JP); **Shasha Liu**, Shanghai (CN); **Wangxin Xie**, Shanghai (CN)

(73) Assignee: **OMRON HEALTHCARE Co., Ltd.**,  
Kyoto (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/809,430**

(22) Filed: **Sep. 28, 2021**

(30) **Foreign Application Priority Data**

Mar. 31, 2021 (CN) ..... 202130178811.1

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/165**

(58) **Field of Classification Search**  
USPC ..... D24/107, 164–169, 185–187; D10/98;  
D14/344  
CPC ..... A61B 5/0404; A61B 5/021; A61B 5/024;  
A61B 5/02438; A61B 5/681; A61B  
5/0402; A61B 2560/0462  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D583,474 S \* 12/2008 Mitsunami ..... D24/165  
D722,165 S \* 2/2015 Pukall ..... D24/165  
D739,938 S \* 9/2015 Schempp ..... D24/165  
D743,035 S \* 11/2015 Uozumi ..... D24/165  
D802,768 S \* 11/2017 Rider ..... D24/165

D850,622 S \* 6/2019 Noguchi ..... D24/165  
D862,702 S \* 10/2019 Nishiyama ..... D24/165  
D922,581 S \* 6/2021 Wang ..... D24/165  
D942,628 S \* 2/2022 Dai ..... D24/165  
2015/0190064 A1\* 7/2015 Kinoshita ..... A61B 5/024  
600/490

**OTHER PUBLICATIONS**

The design of sphygmomanometer on p. 69 of “Croissant (magazine)”, vol. 16, issued on Aug. 25, 2010, furnished in the National Center for Industrial Property Information and Training on Aug. 16, 2010.

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Capitol City TechLaw

(57) **CLAIM**

The ornamental design for a sphygmomanometer, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, bottom, and right side perspective view of a sphygmomanometer, showing our new design; FIG. 2 is a front view thereof; FIG. 3 is a rear view thereof; FIG. 4 is a top view thereof; FIG. 5 is a bottom view thereof; FIG. 6 is a left side view thereof; and, FIG. 7 is a right side view thereof.

The broken lines shown in the figures illustrate portions of the sphygmomanometer that form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

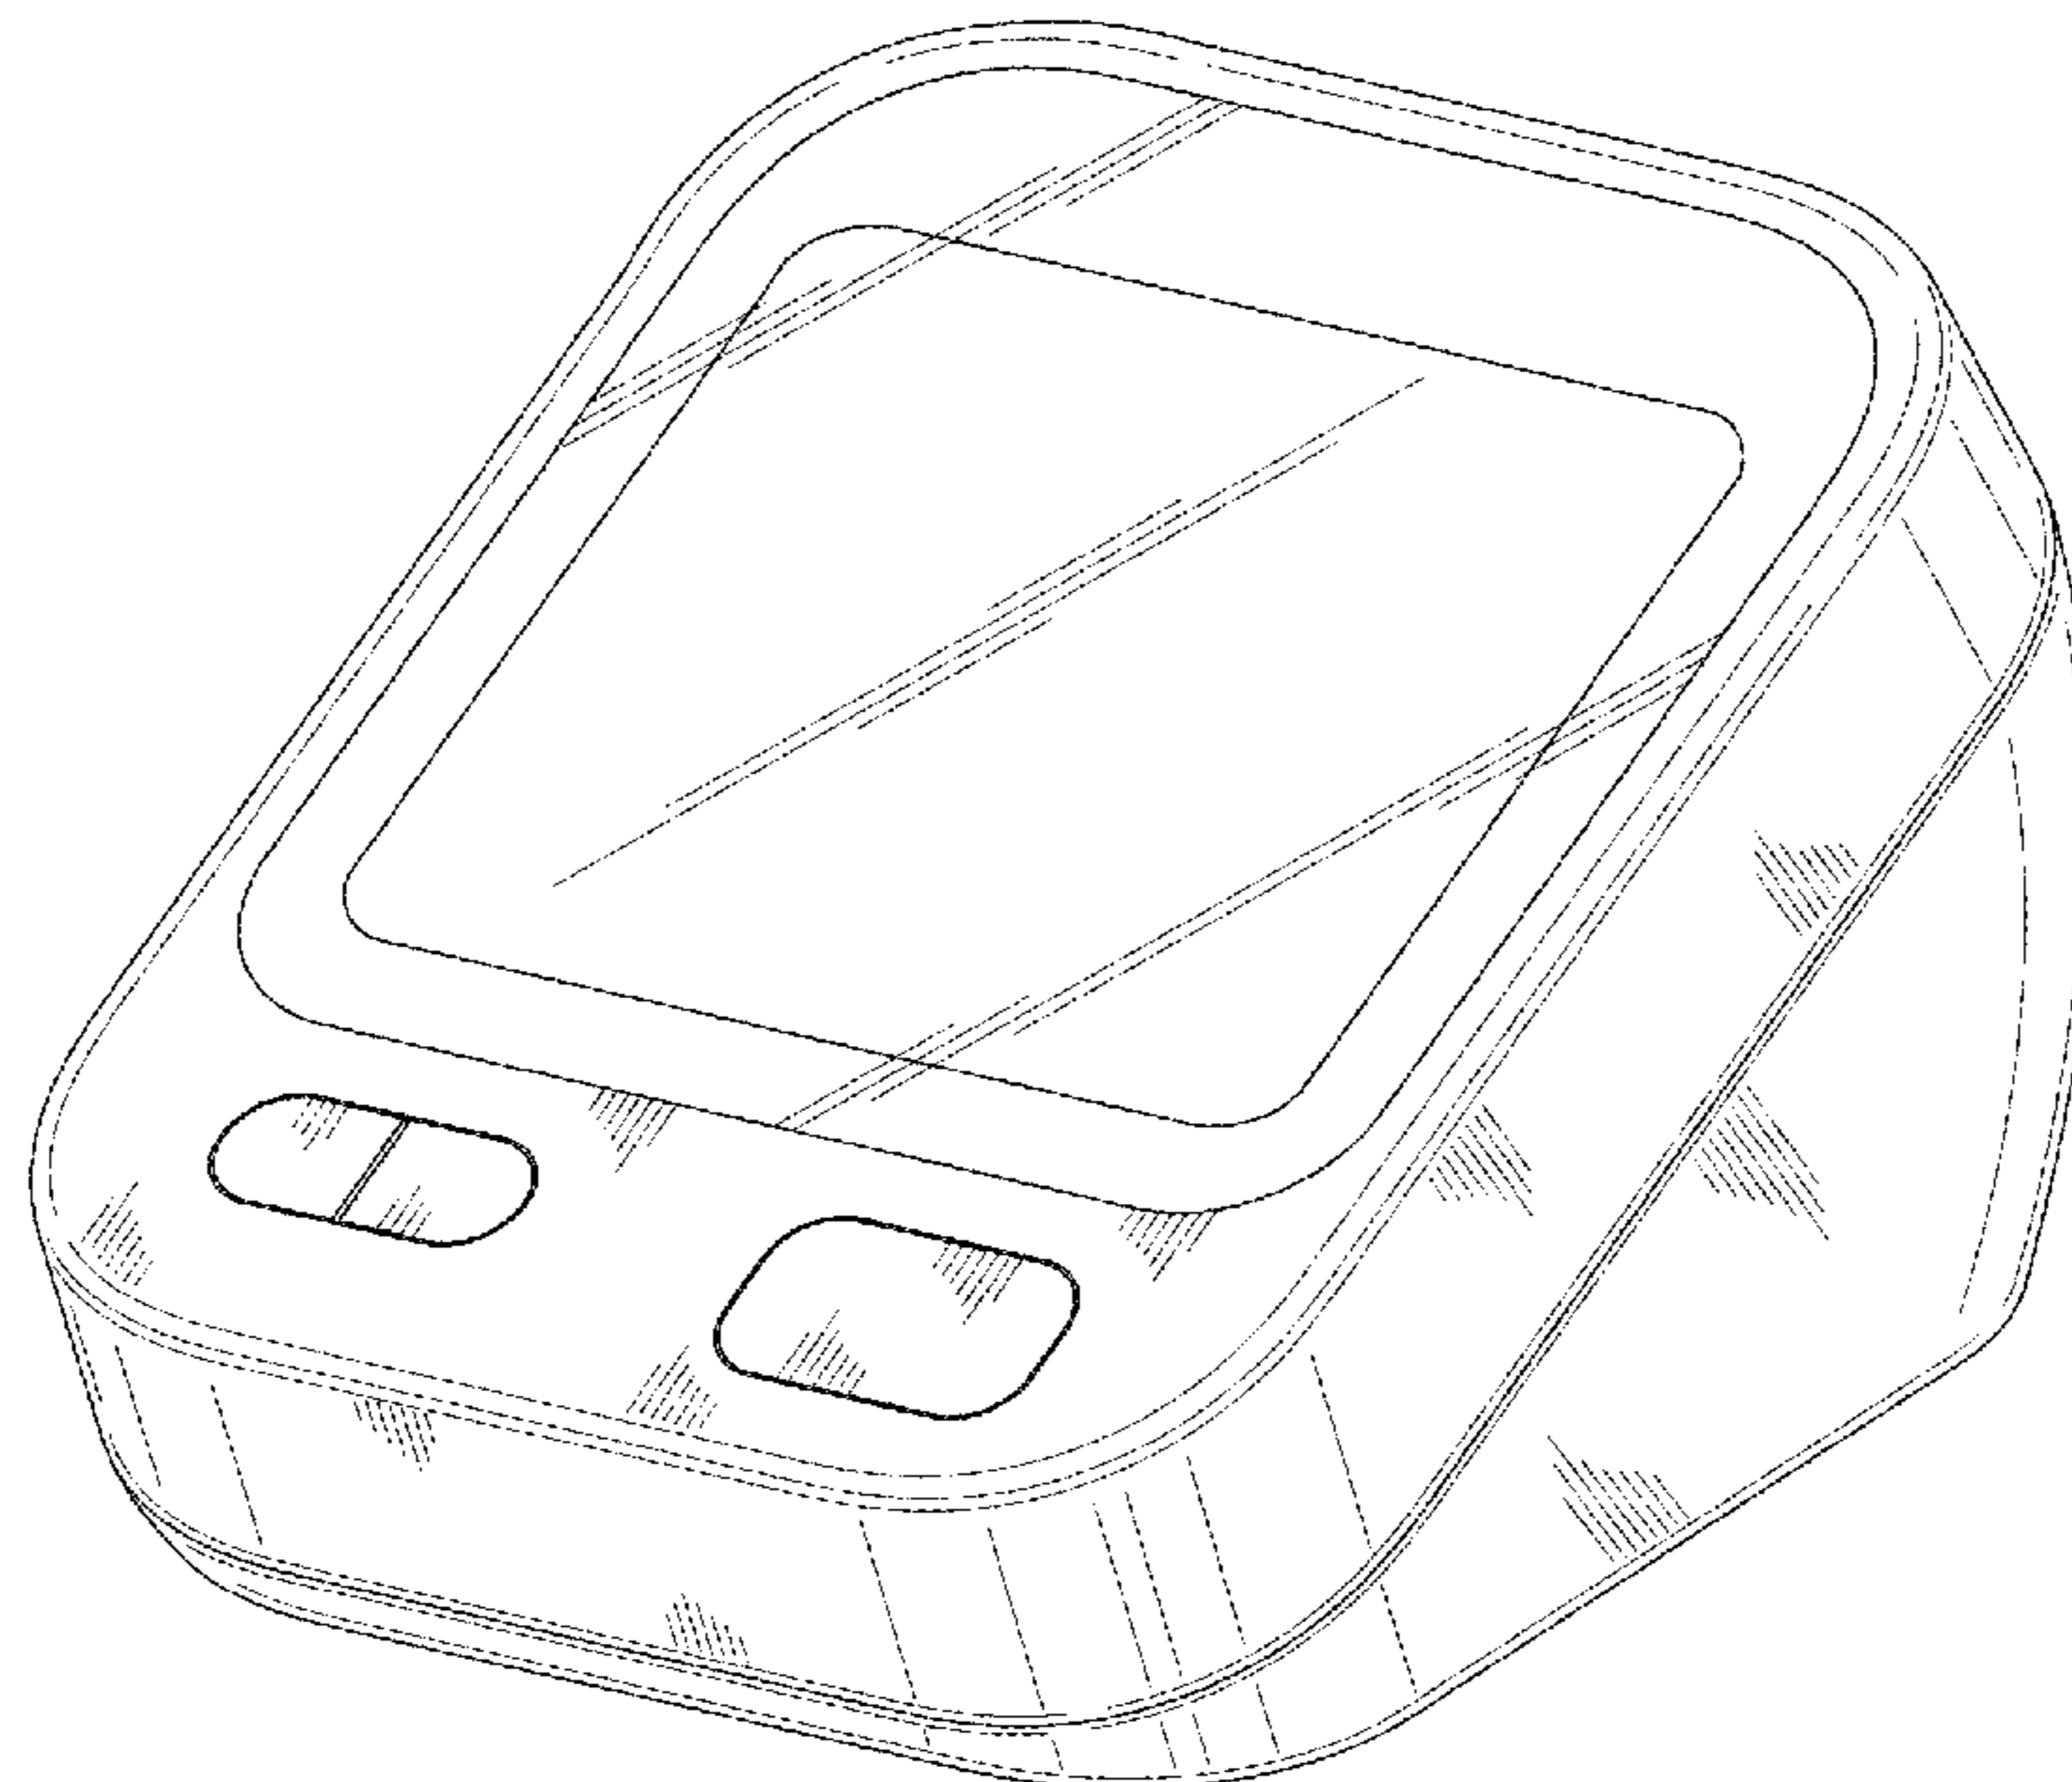


FIG. 1

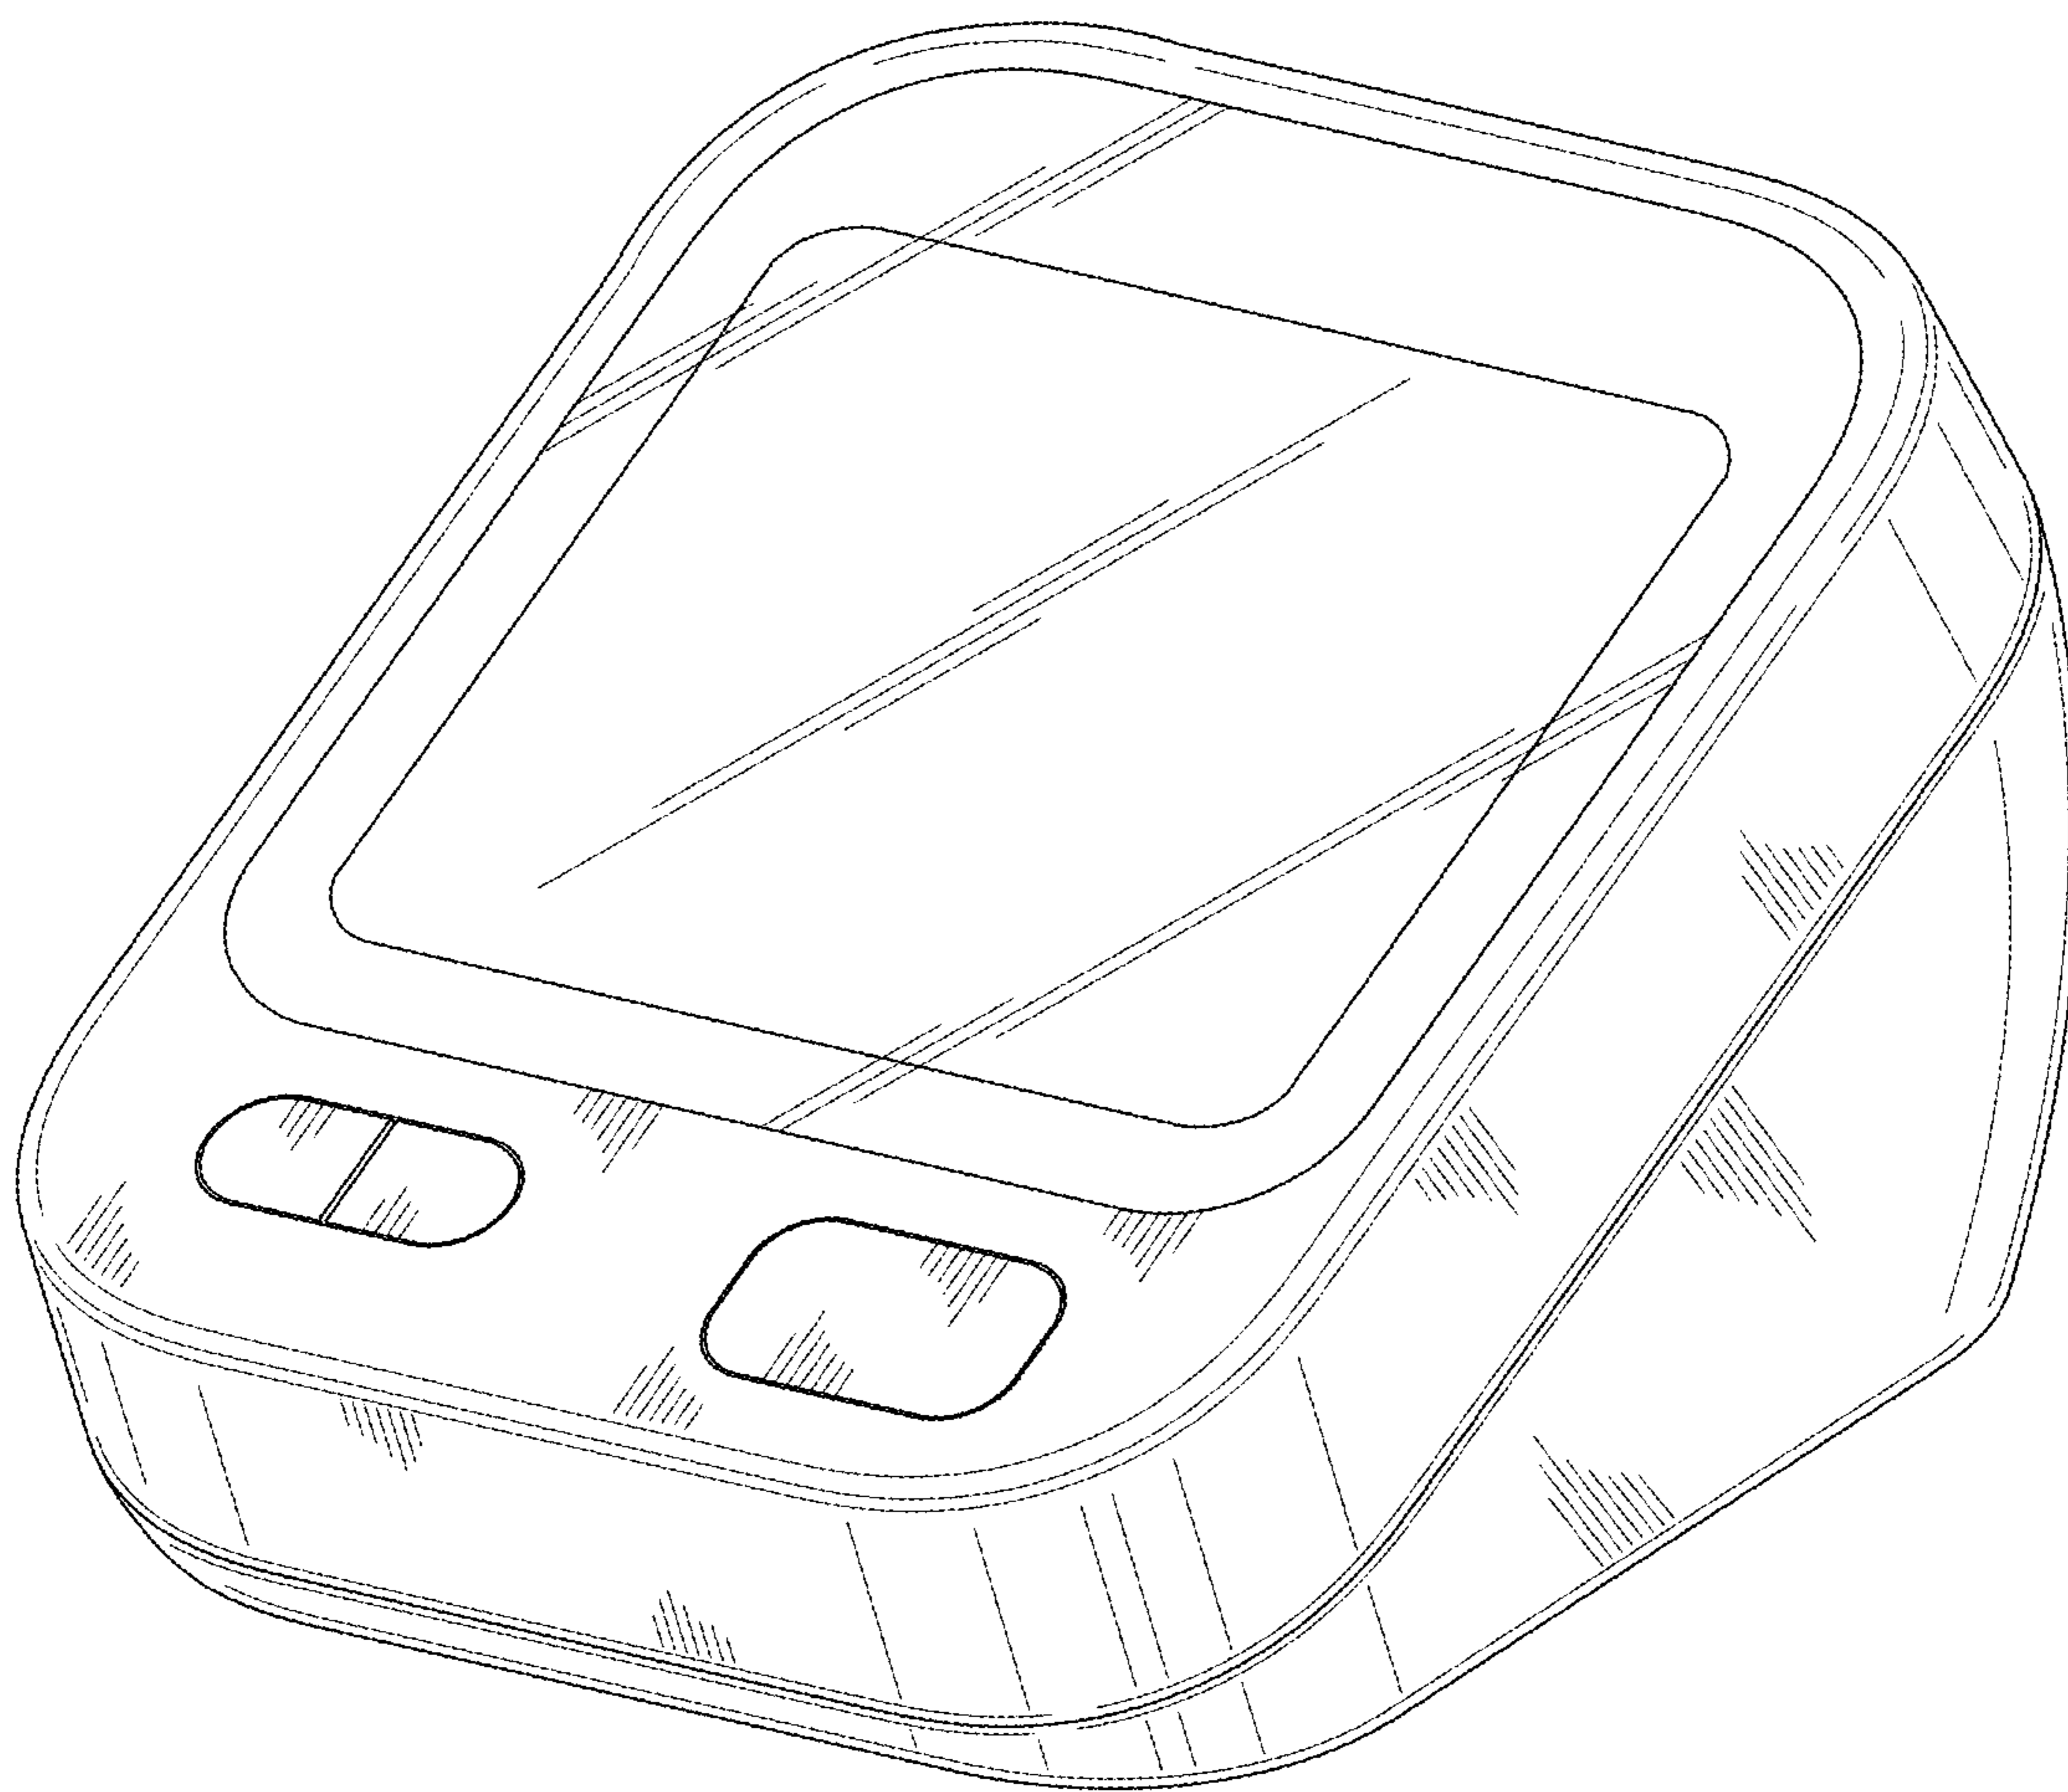


FIG. 2

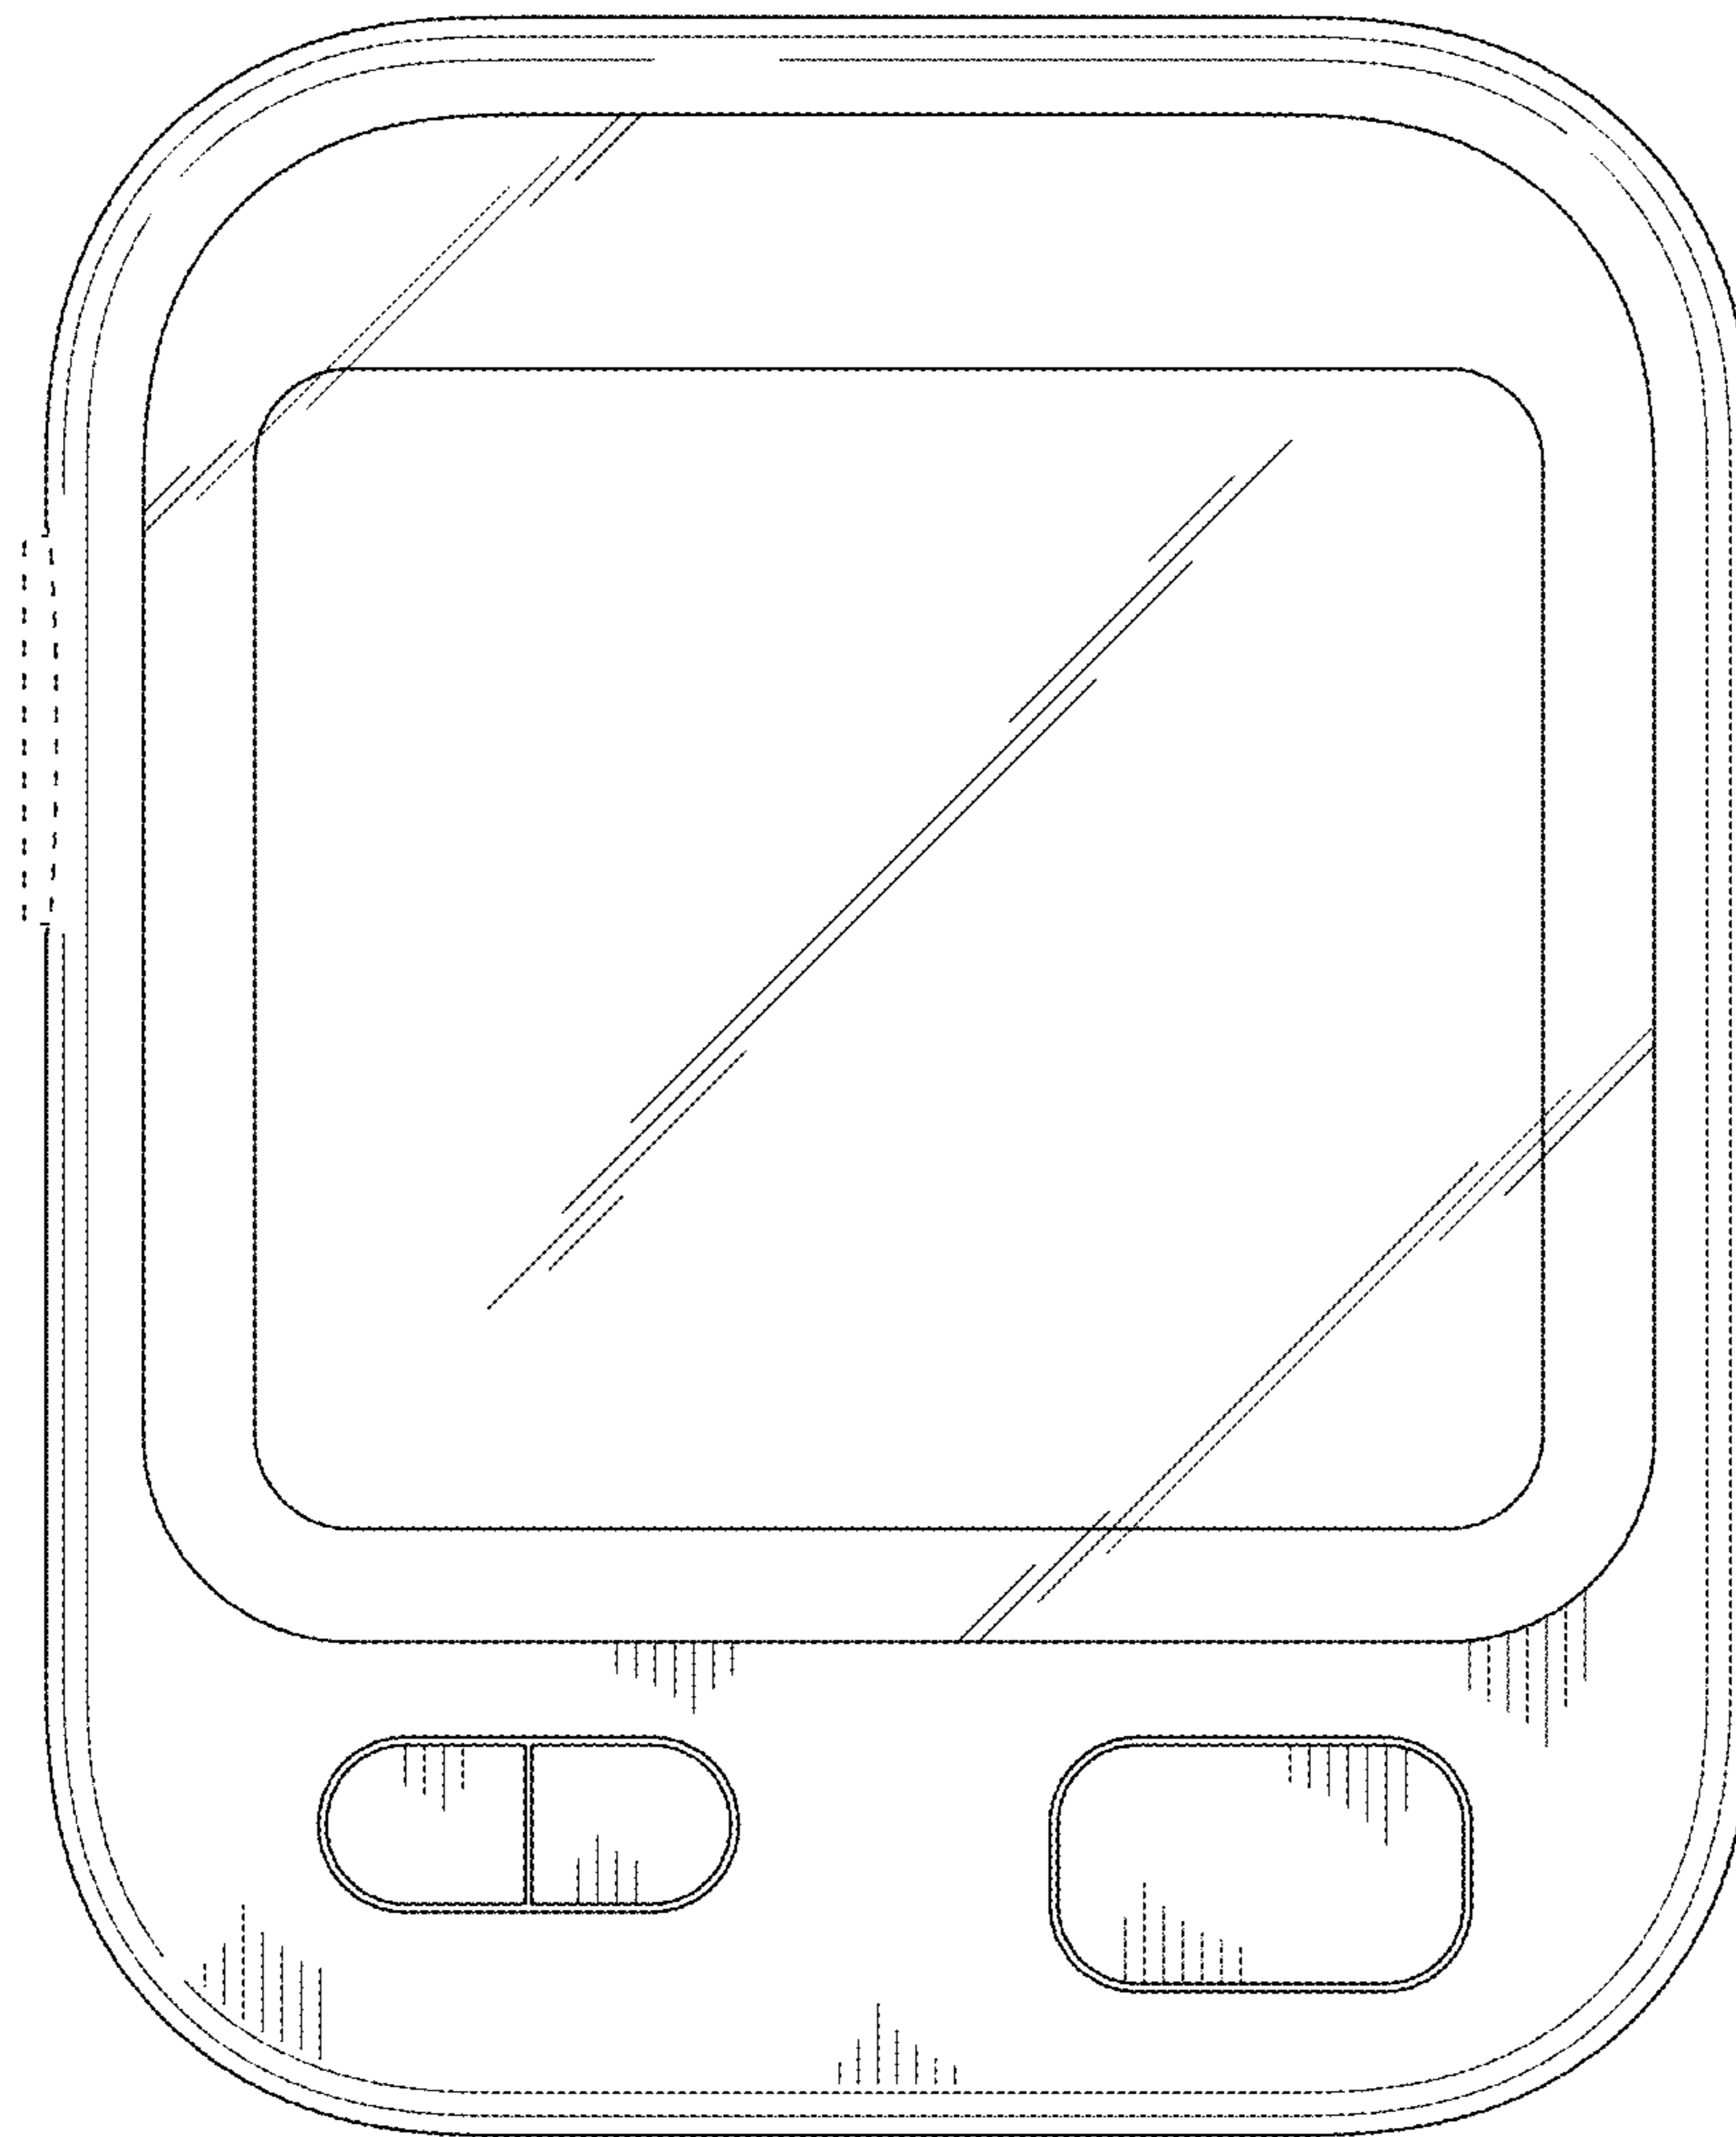


FIG. 3

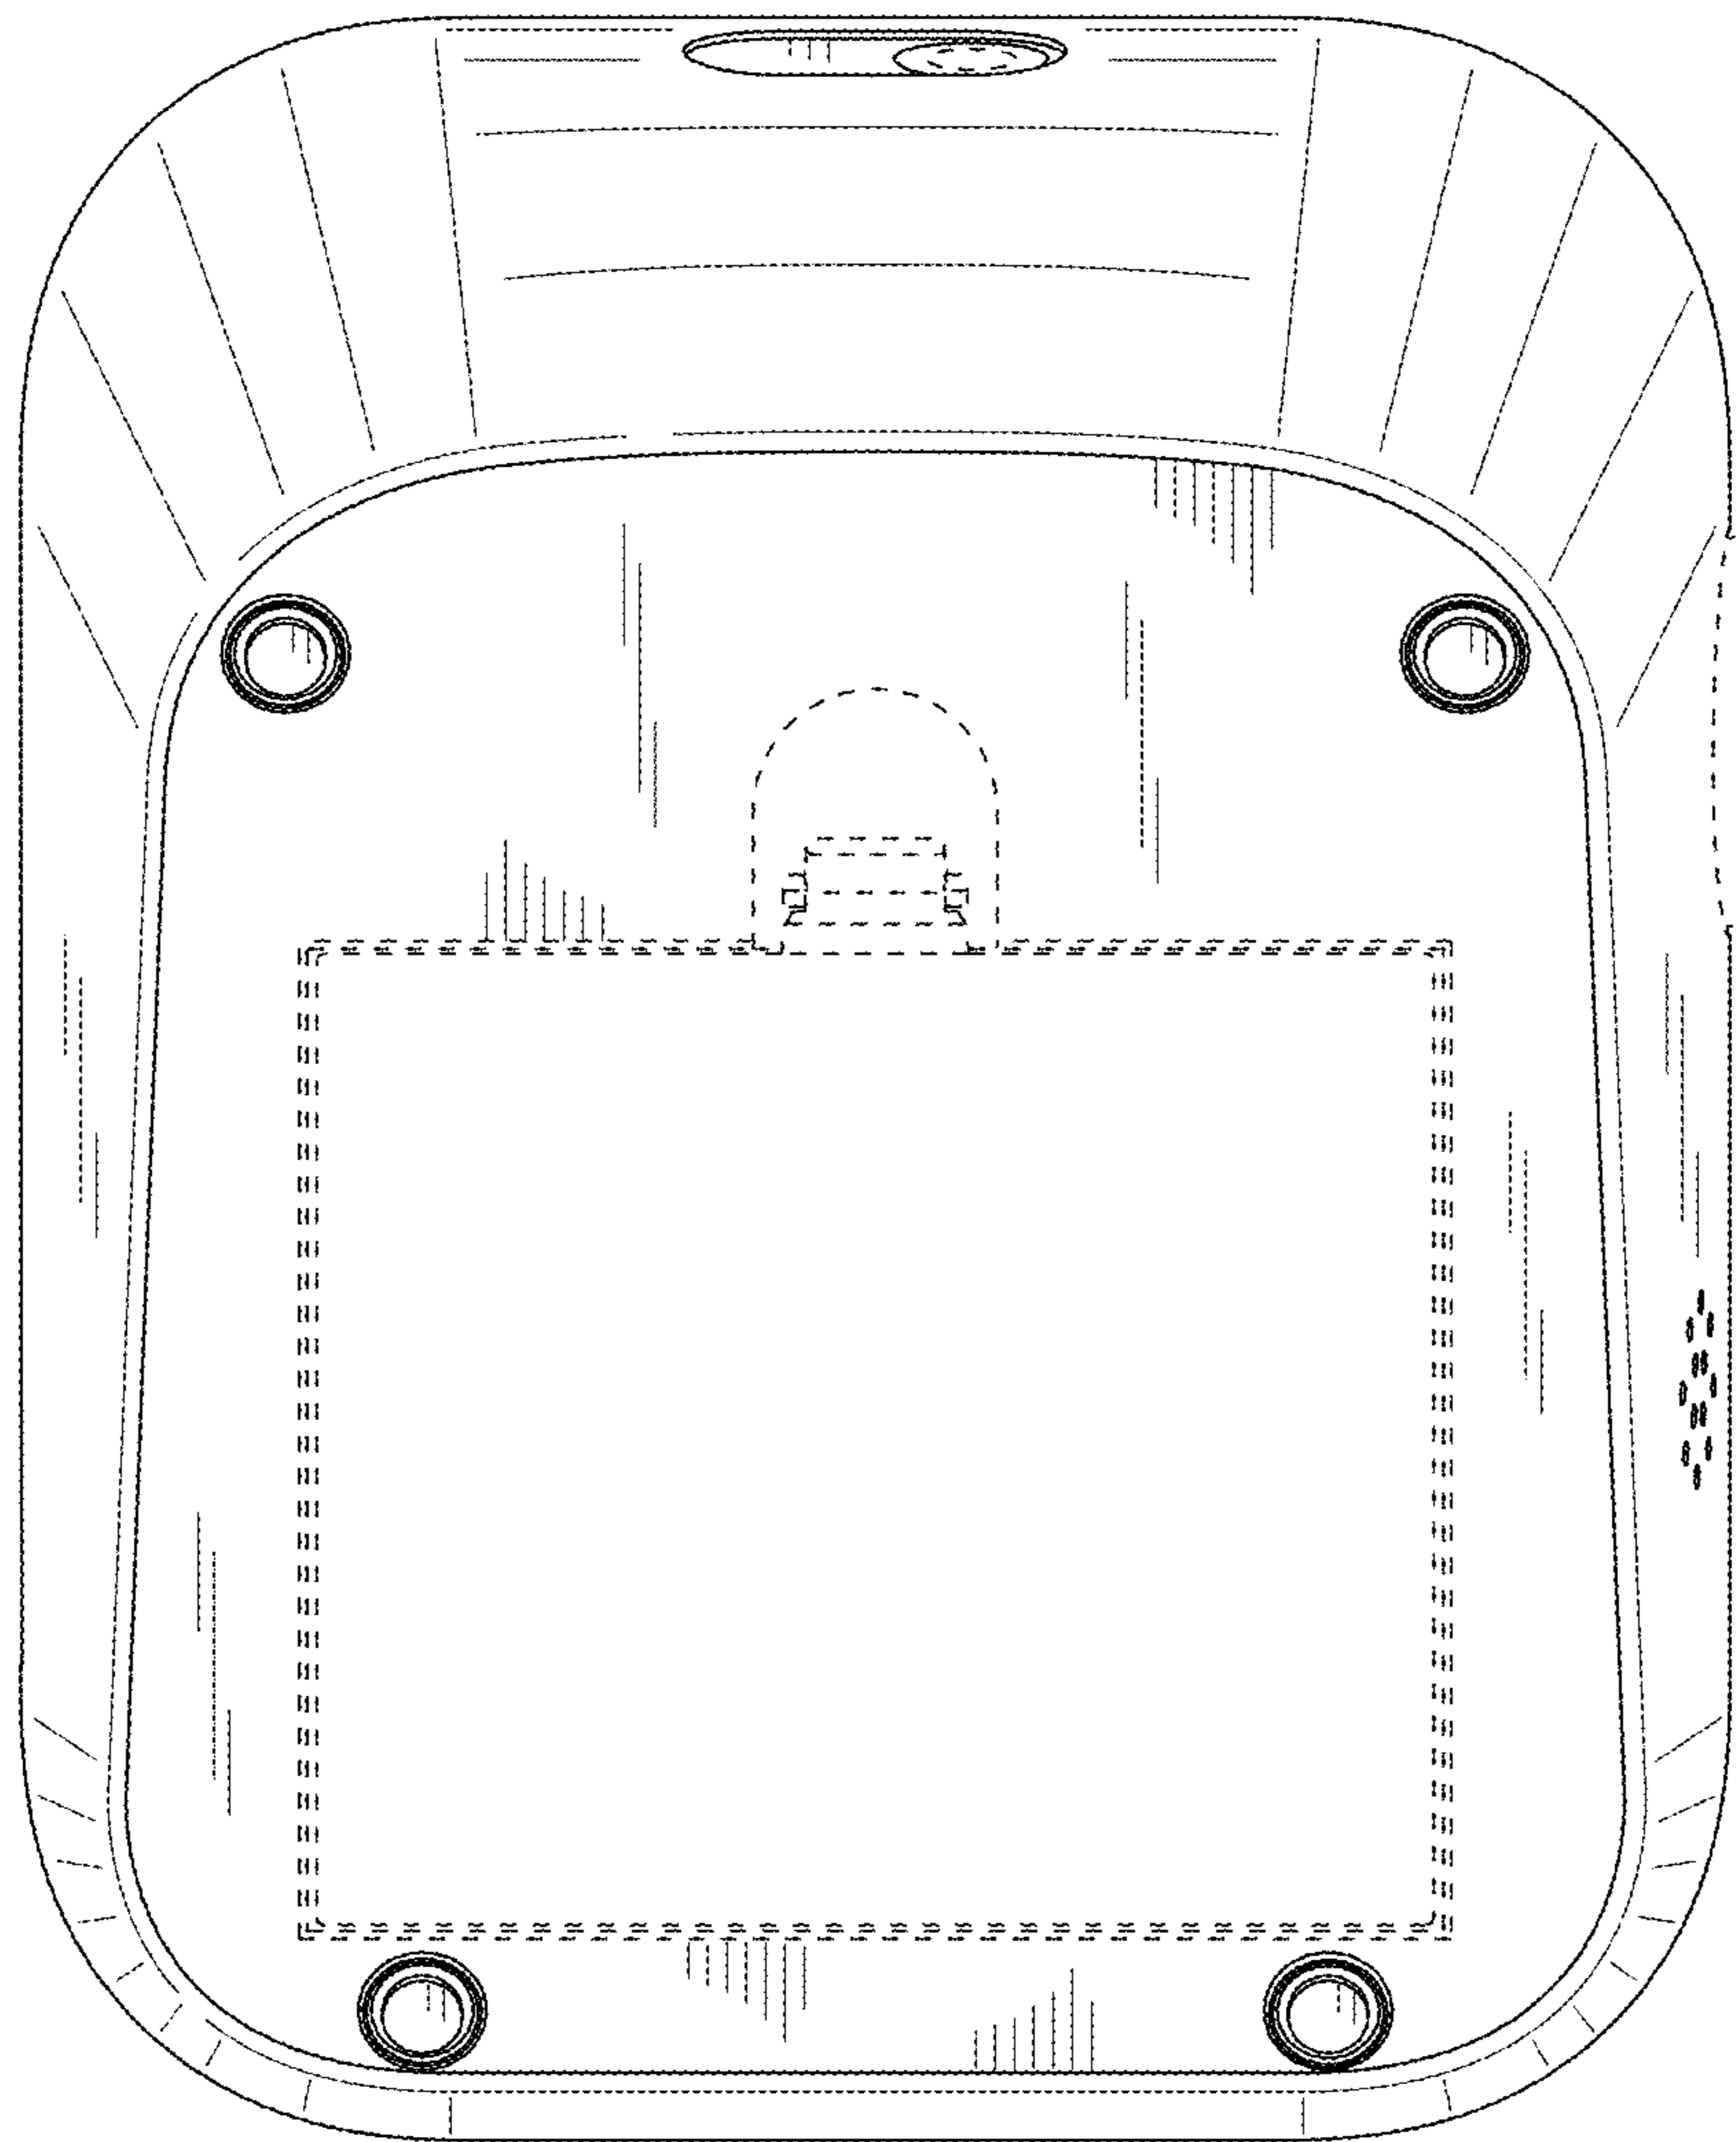


FIG. 4

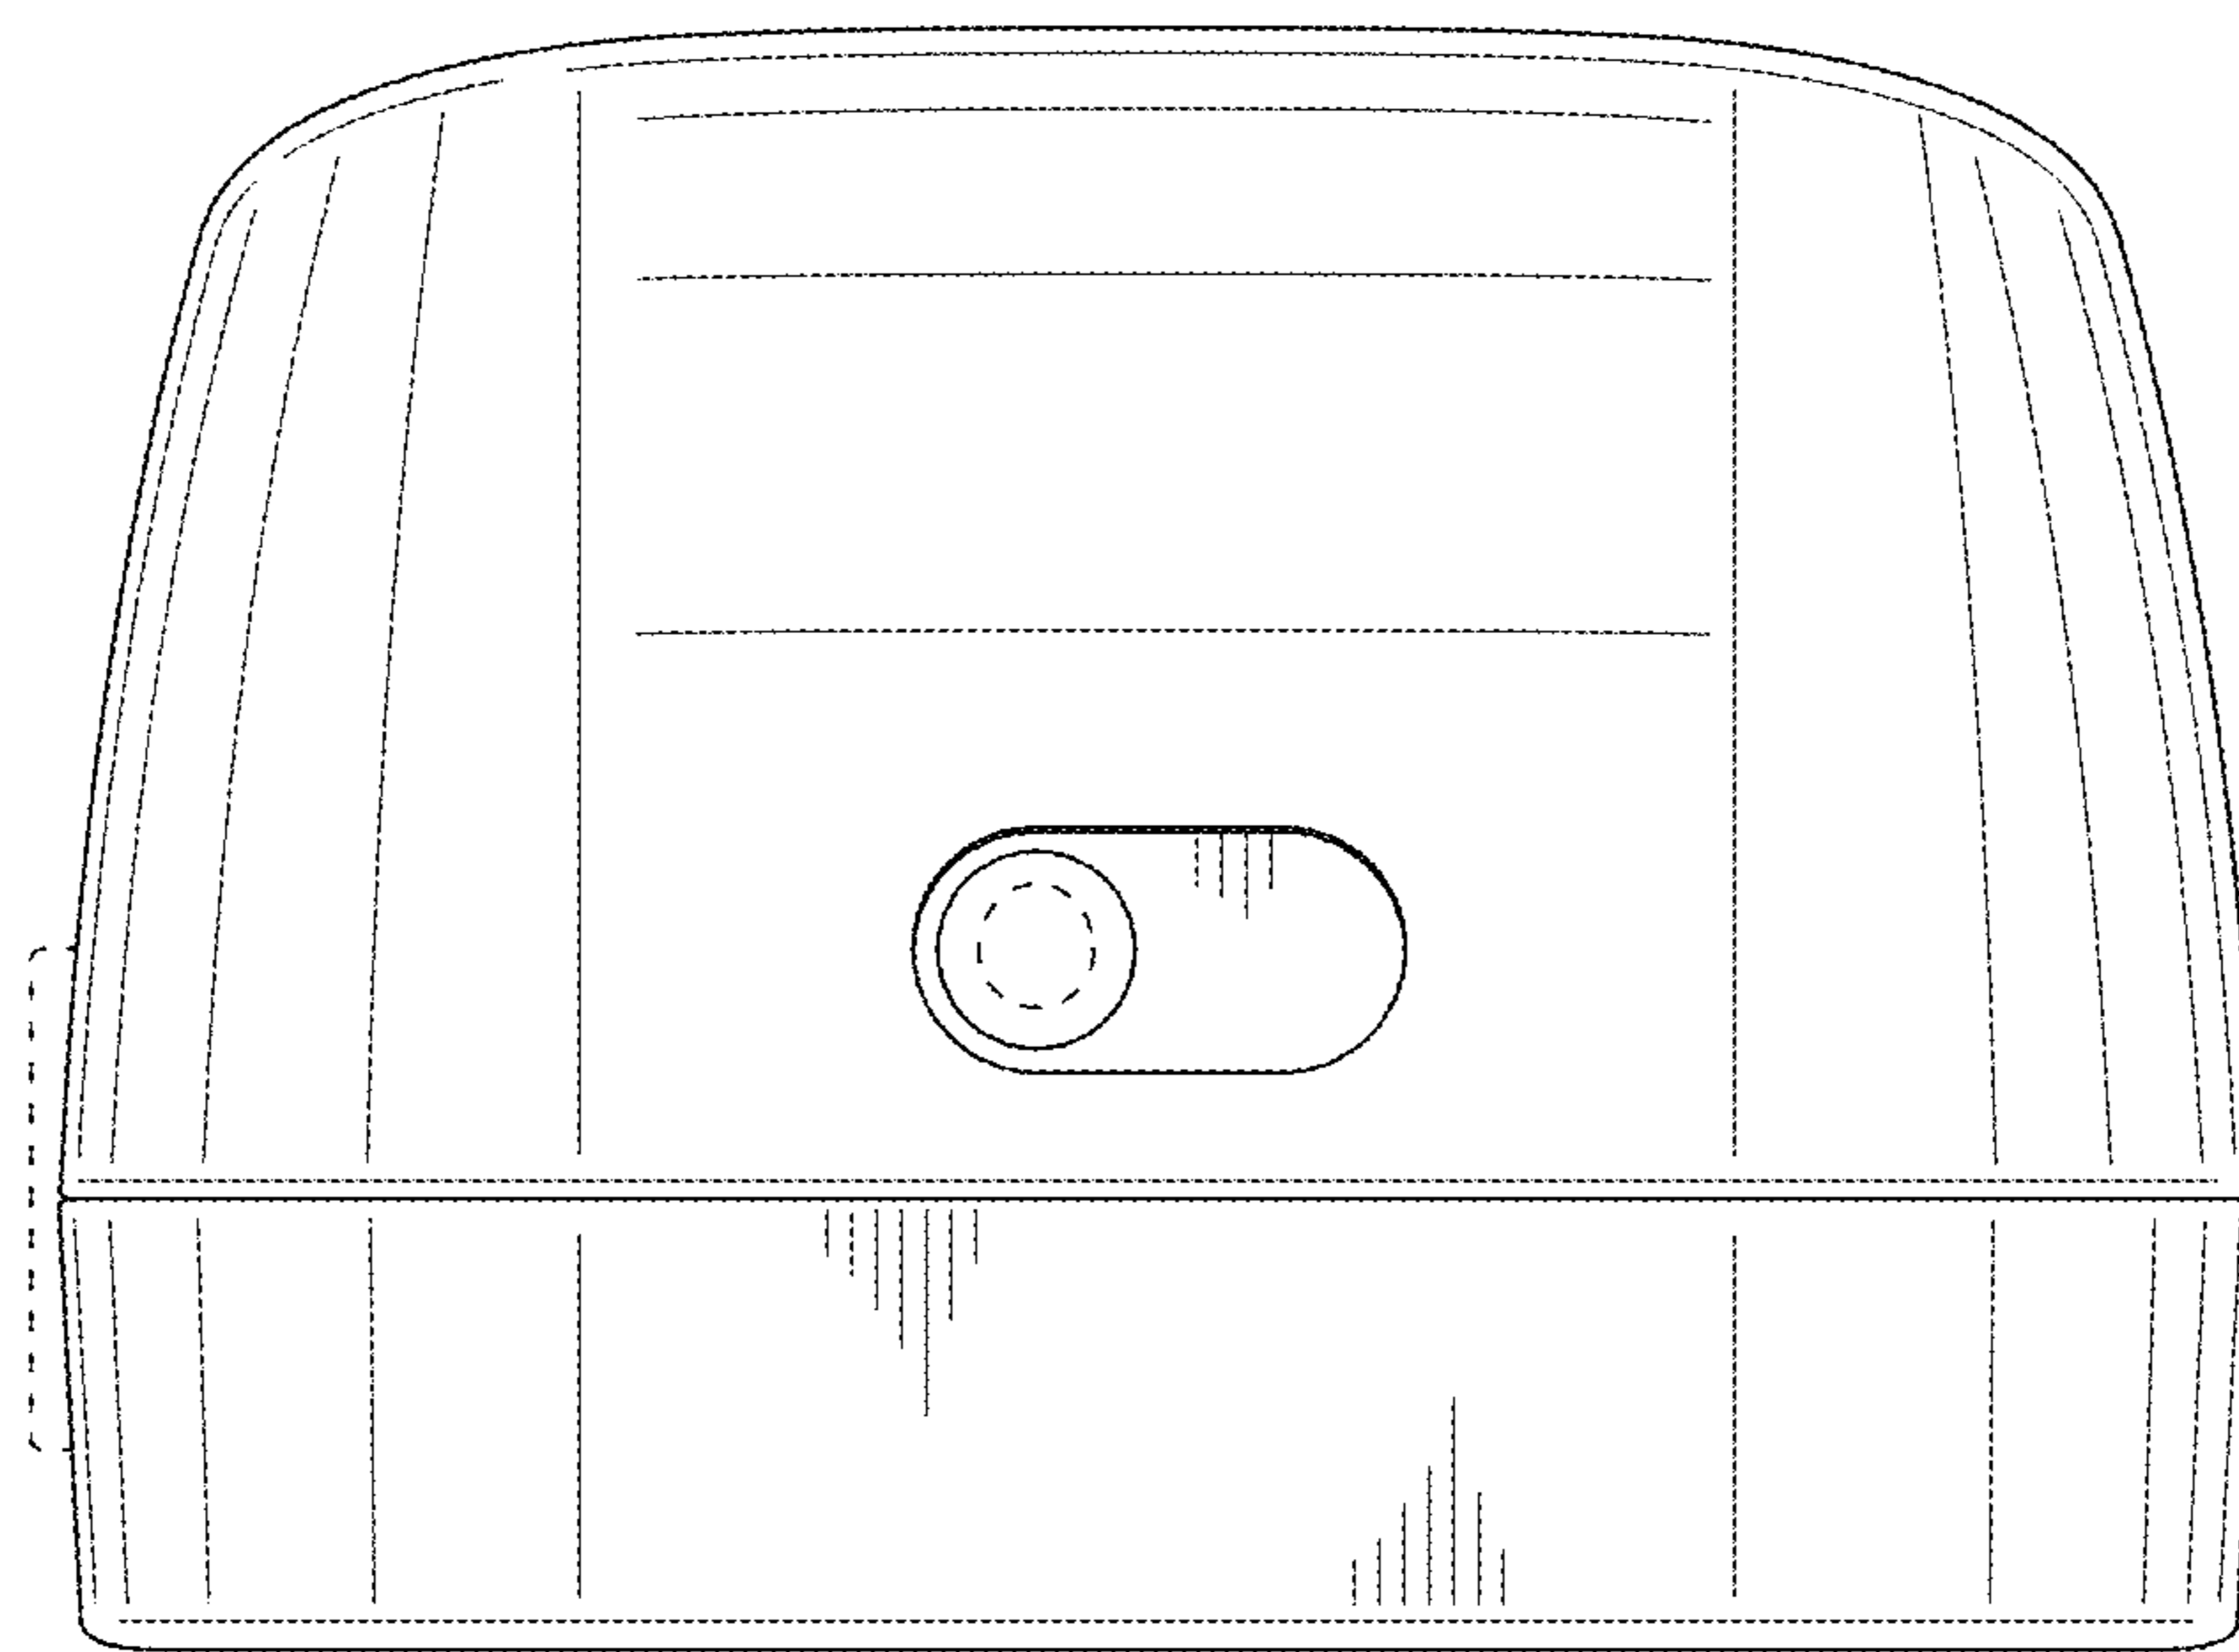


FIG. 5

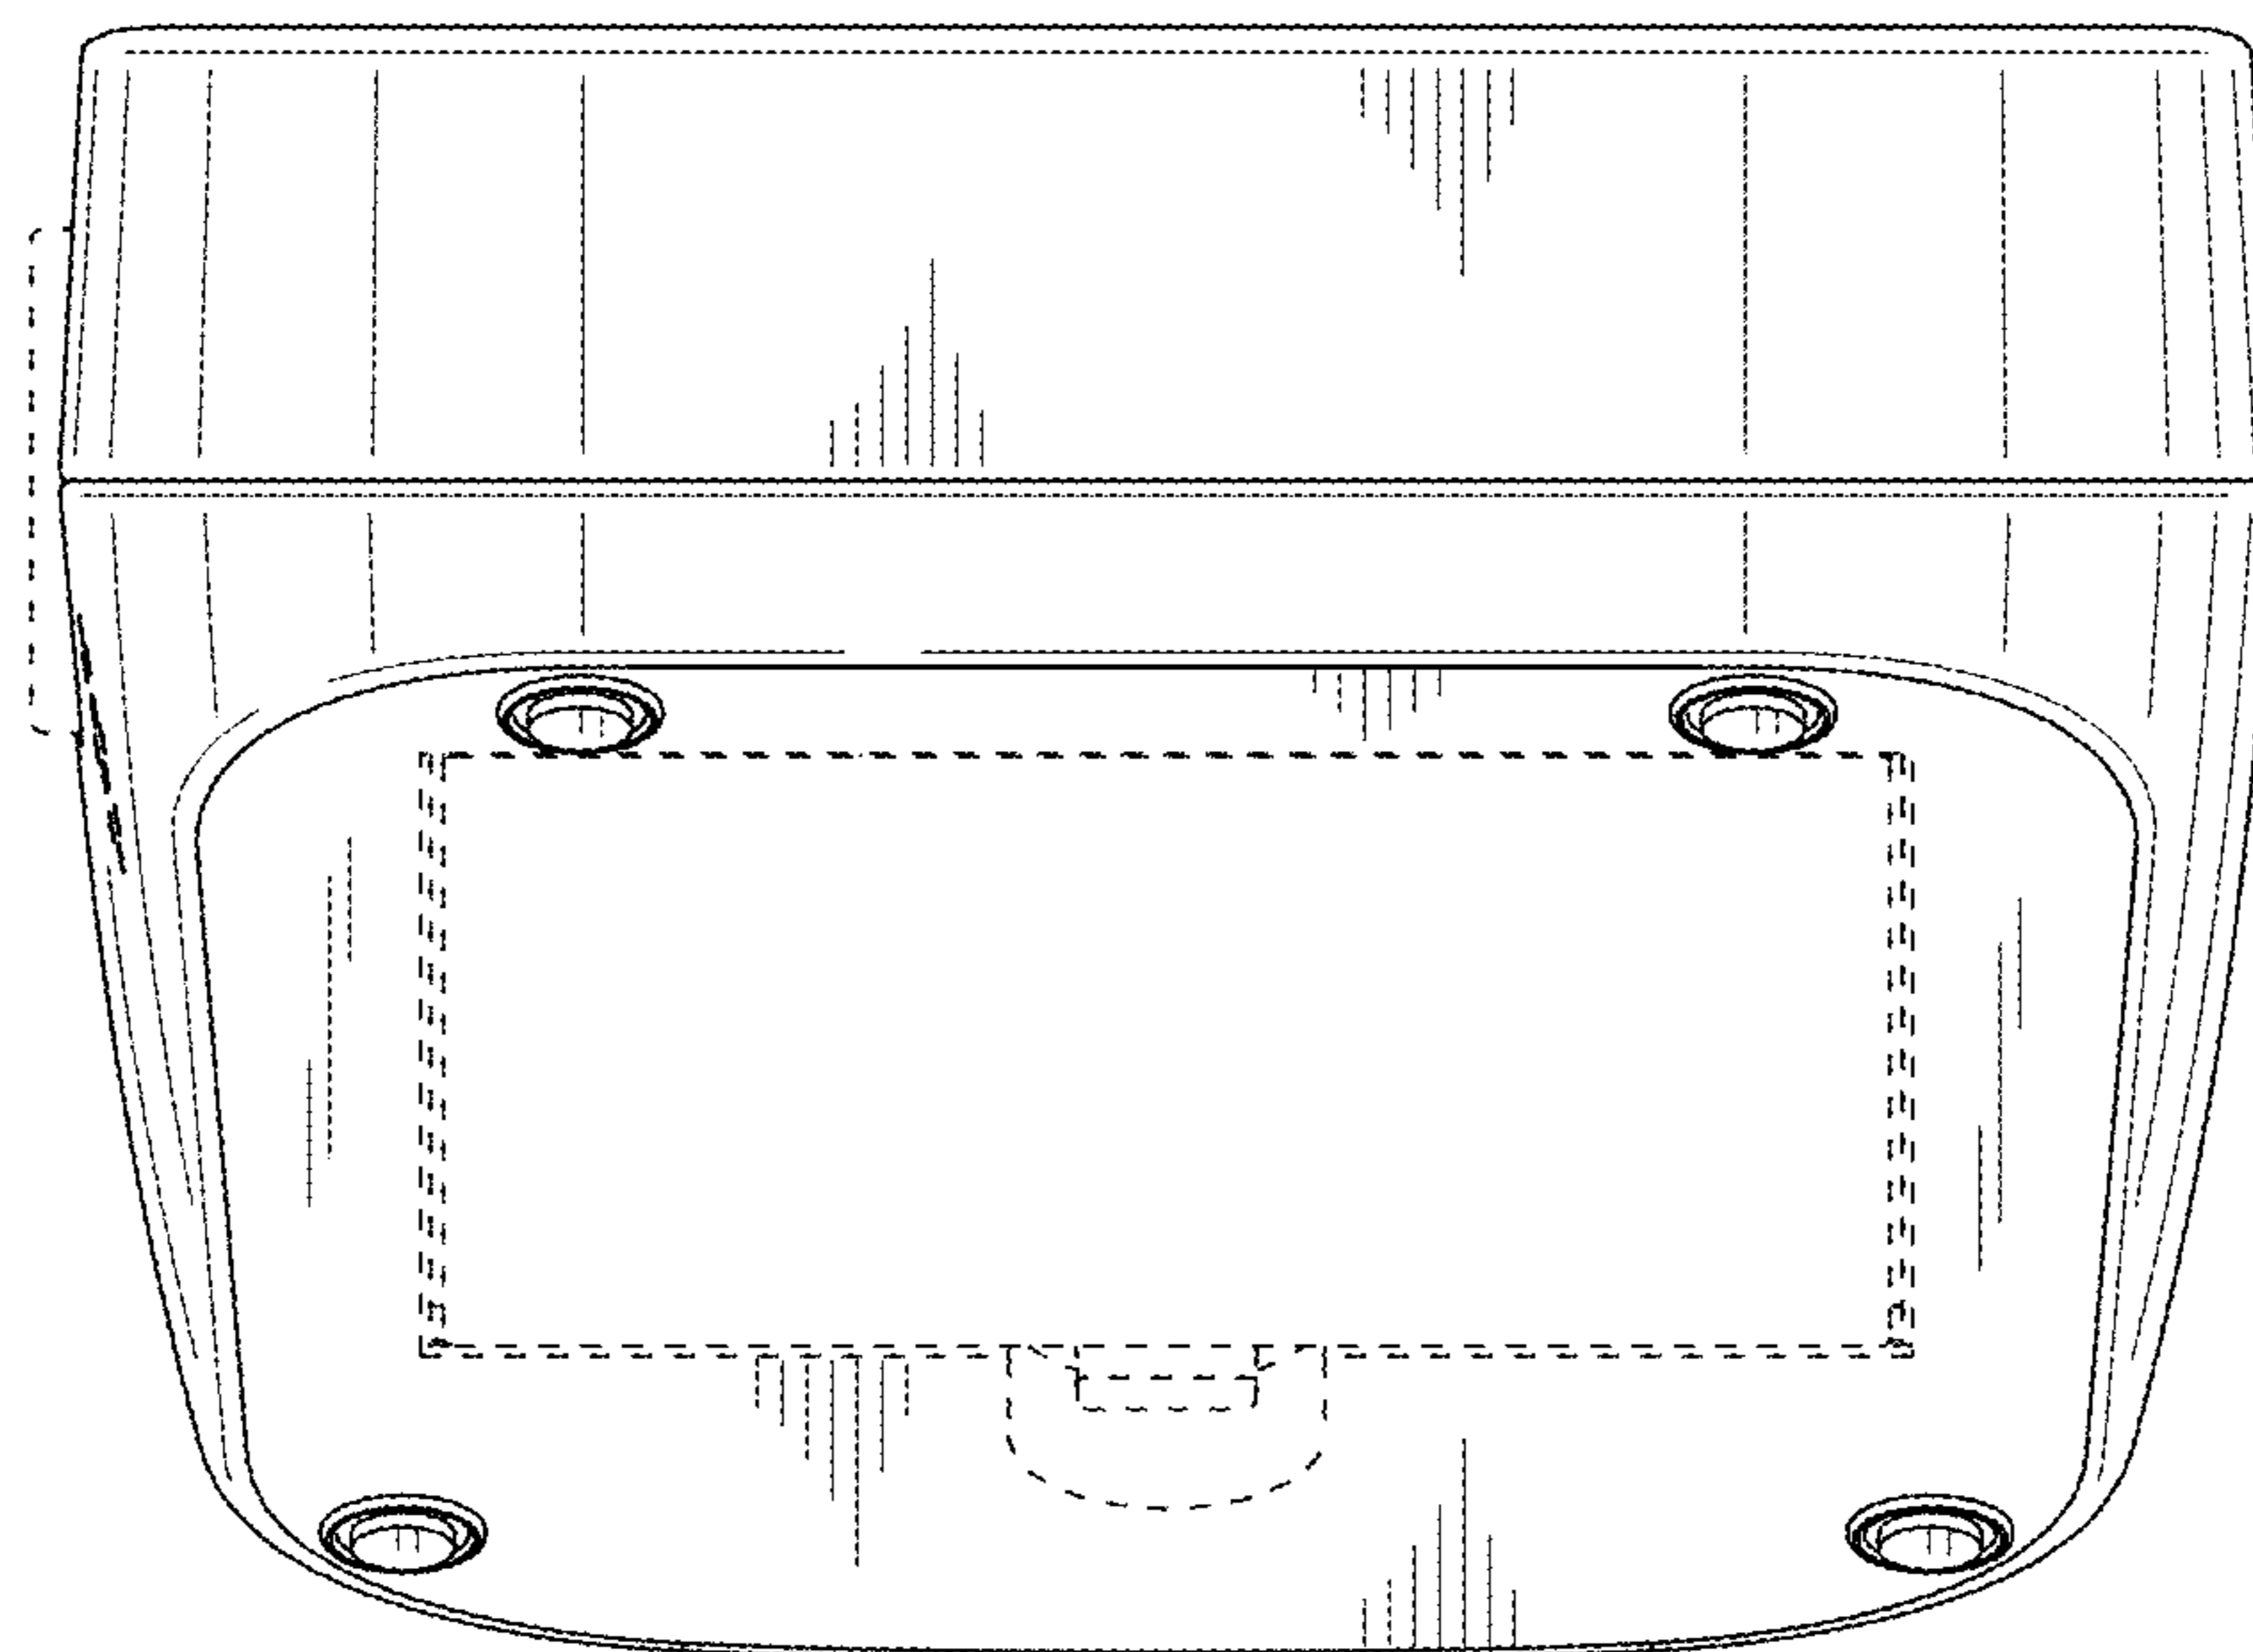


FIG. 6

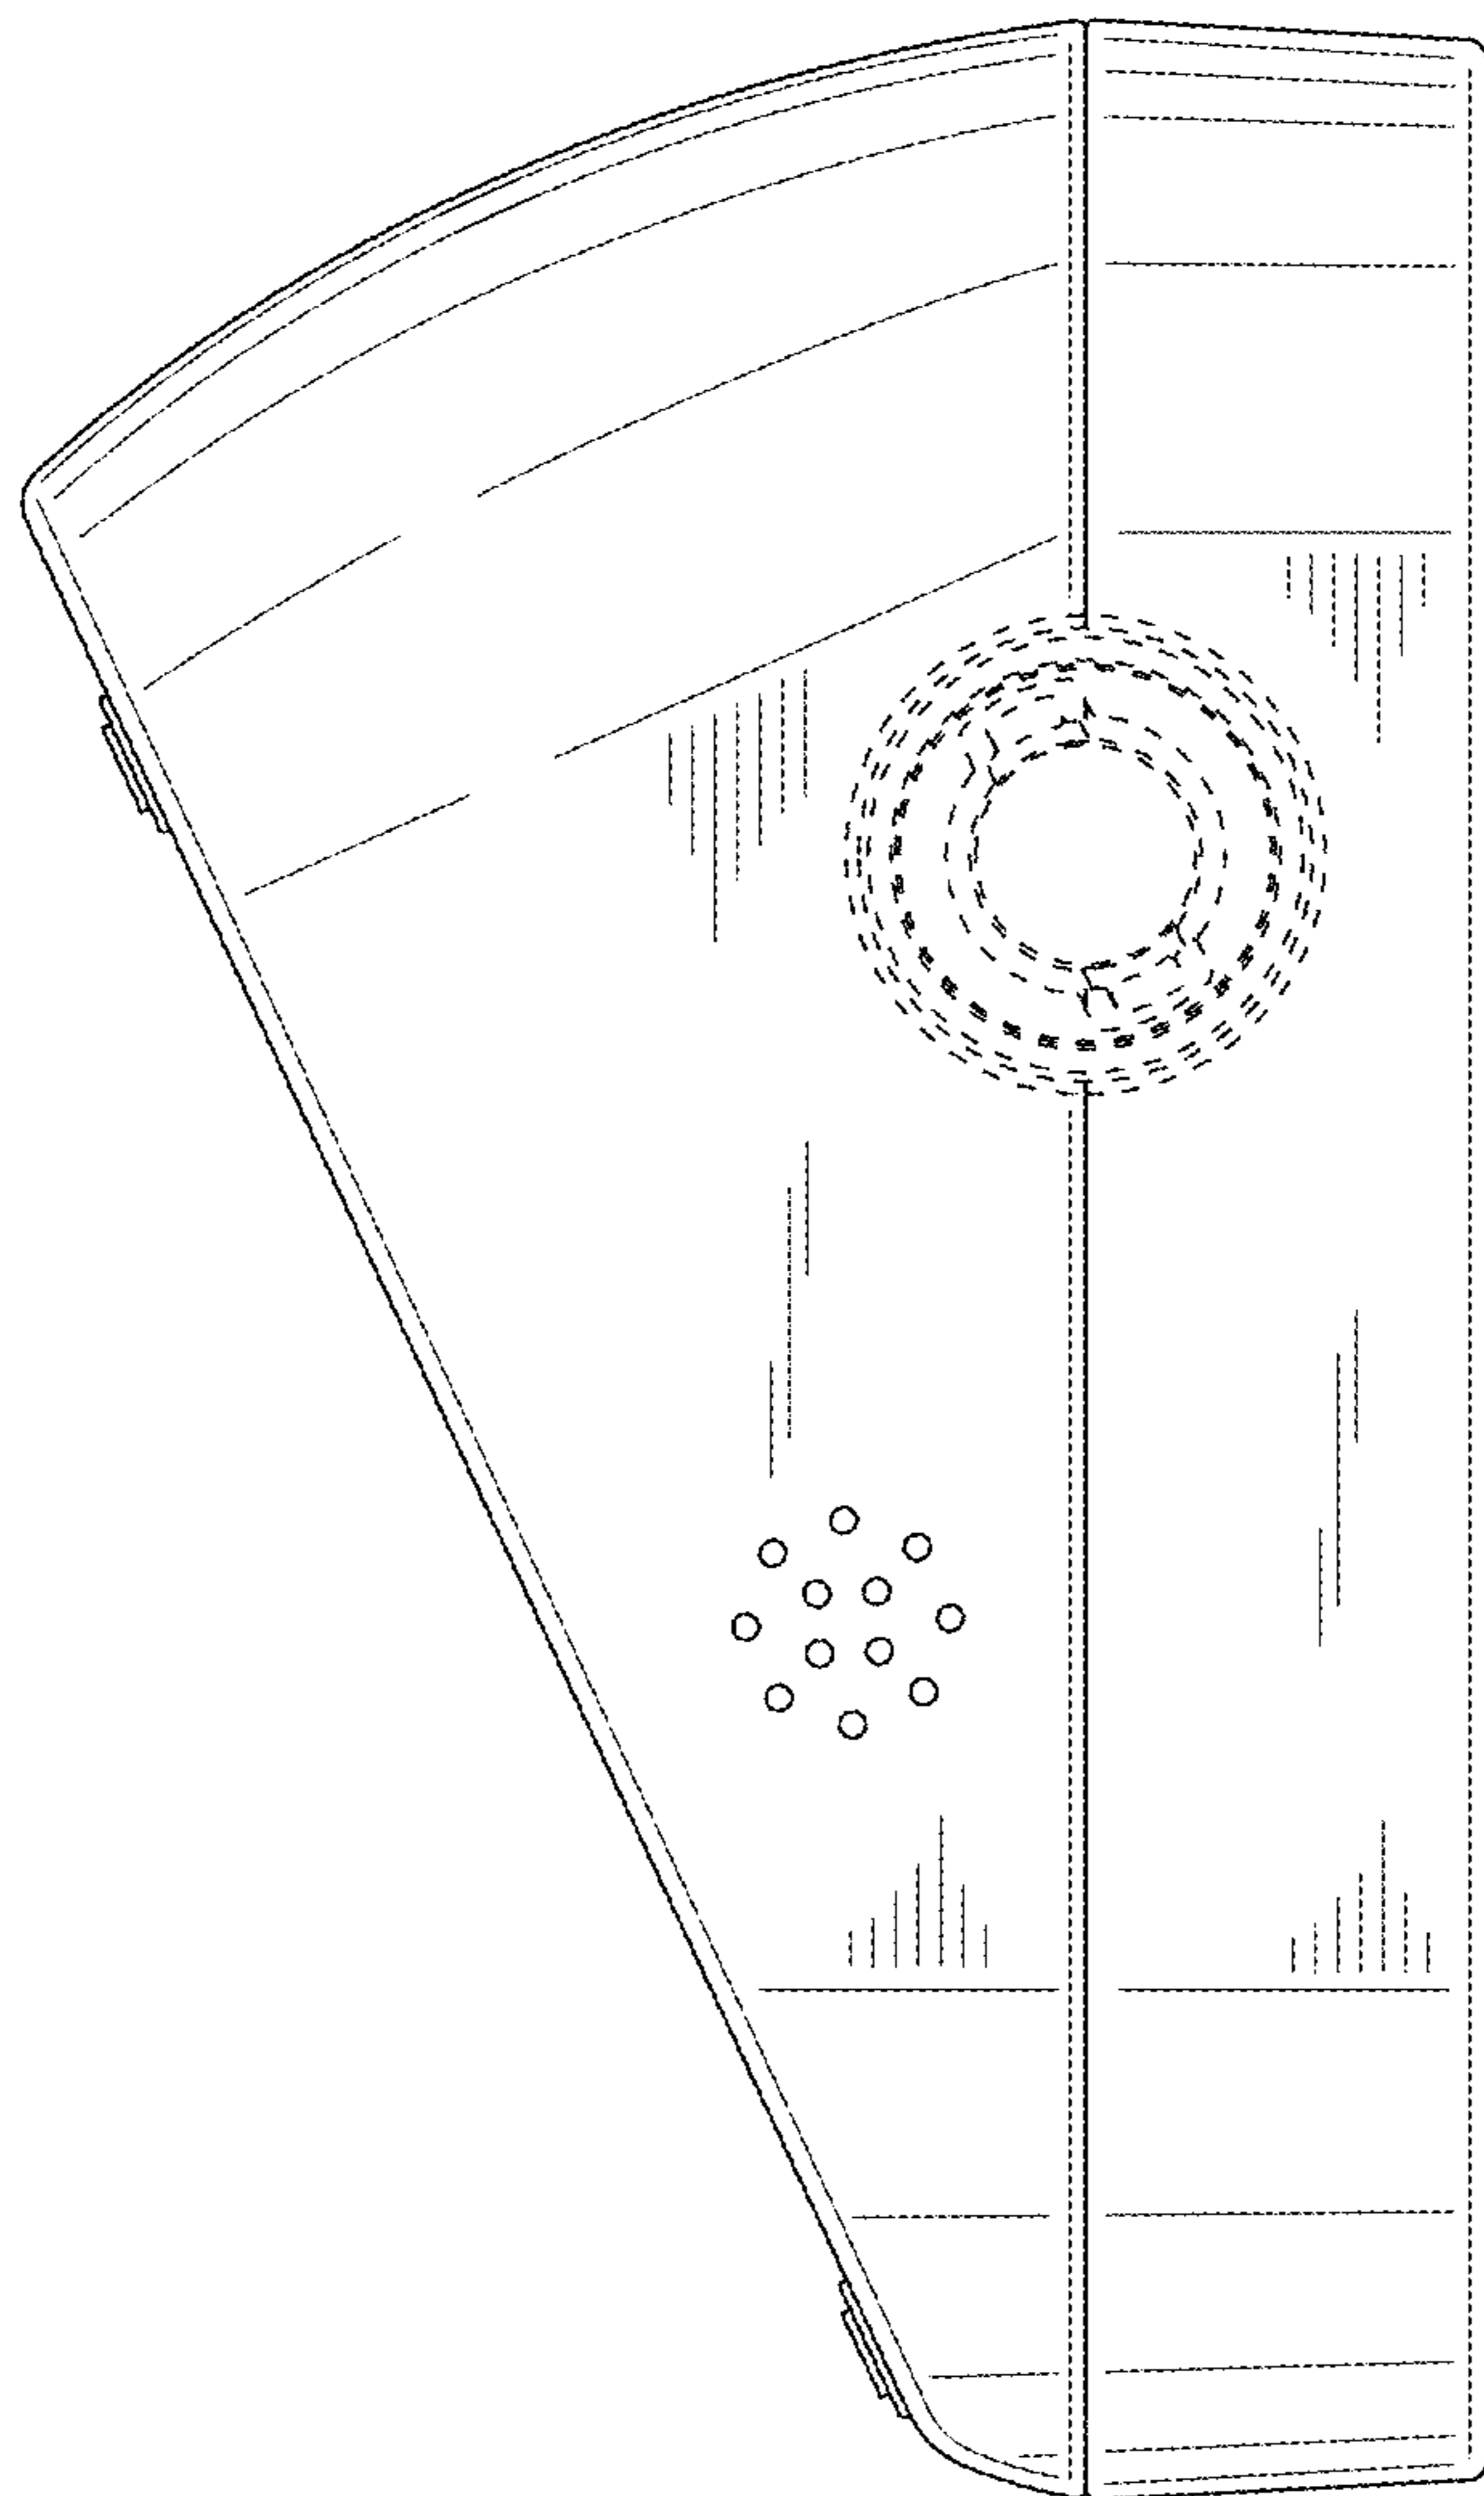


FIG. 7

