



US00D979787S

(12) **United States Design Patent** (10) **Patent No.:** **US D979,787 S**  
**Gruen et al.** (45) **Date of Patent:** **\*\* Feb. 28, 2023**

(54) **DIAGNOSTIC APPARATUS FOR MEDICAL OR LABORATORY PURPOSES**

- (71) Applicant: **EUROIMMUN Medizinische Labordiagnostika AG**, Luebeck (DE)
- (72) Inventors: **Torsten Gruen**, Hamburg (DE); **Frank Mollenhauer**, Ziethen (DE)
- (73) Assignee: **EUROIMMUN Medizinische Labordiagnostika AG**, Luebeck (DE)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/746,924**
- (22) Filed: **Aug. 18, 2020**

**Related U.S. Application Data**

- (62) Division of application No. 29/676,801, filed on Jan. 15, 2019, now Pat. No. Des. 896,981.

(30) **Foreign Application Priority Data**

- Jul. 20, 2018 (EM) ..... 005508876.0001
  - Jul. 20, 2018 (EM) ..... 005508876.0002
- (Continued)

- (51) **LOC (14) Cl.** ..... **24-01**
- (52) **U.S. Cl.**  
USPC ..... **D24/216**

- (58) **Field of Classification Search**  
USPC ..... D24/107, 185, 186, 216, 219, 231-234;  
D10/81
- (Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- D515,707 S 2/2006 Shinohara et al.
  - D646,189 S 10/2011 Dinter et al.
- (Continued)

**OTHER PUBLICATIONS**

Examination Report dated Nov. 9, 2020 in Canadian Application No. 185723, 2 pages.

(Continued)

*Primary Examiner* — Anhdao Doan  
(74) *Attorney, Agent, or Firm* — Grüneberg and Myers PLLC

(57) **CLAIM**

The ornamental design for a diagnostic apparatus for medical or laboratory purposes, as shown and described.

**DESCRIPTION**

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a left side elevational view of a first embodiment of a diagnostic apparatus for medical or laboratory purposes. FIG. 2 is a right side elevational view thereof.

FIG. 3 is a front elevational view thereof

FIG. 4 is a top front perspective view thereof.

FIG. 5 is a top front perspective view thereof.

FIG. 6 is a right side elevational view of a second embodiment of a diagnostic apparatus for medical or laboratory purposes.

FIG. 7 is a front elevational view thereof

FIG. 8 is a left side elevational view thereof.

FIG. 9 is a top front perspective view thereof.

FIG. 10 is a top front perspective view thereof.

FIG. 11 is a left side elevational view of a third embodiment of a diagnostic apparatus for medical or laboratory purposes.

FIG. 12 is a top front perspective view thereof.

FIG. 13 is a right side elevational view thereof.

FIG. 14 is a front elevational view thereof.

FIG. 15 is a top front perspective view thereof.

FIG. 16 is a left side elevational view of a fourth embodiment of a diagnostic apparatus for medical or laboratory purposes.

FIG. 17 is a front elevational view thereof.

FIG. 18 is a right side elevational view thereof.

(Continued)

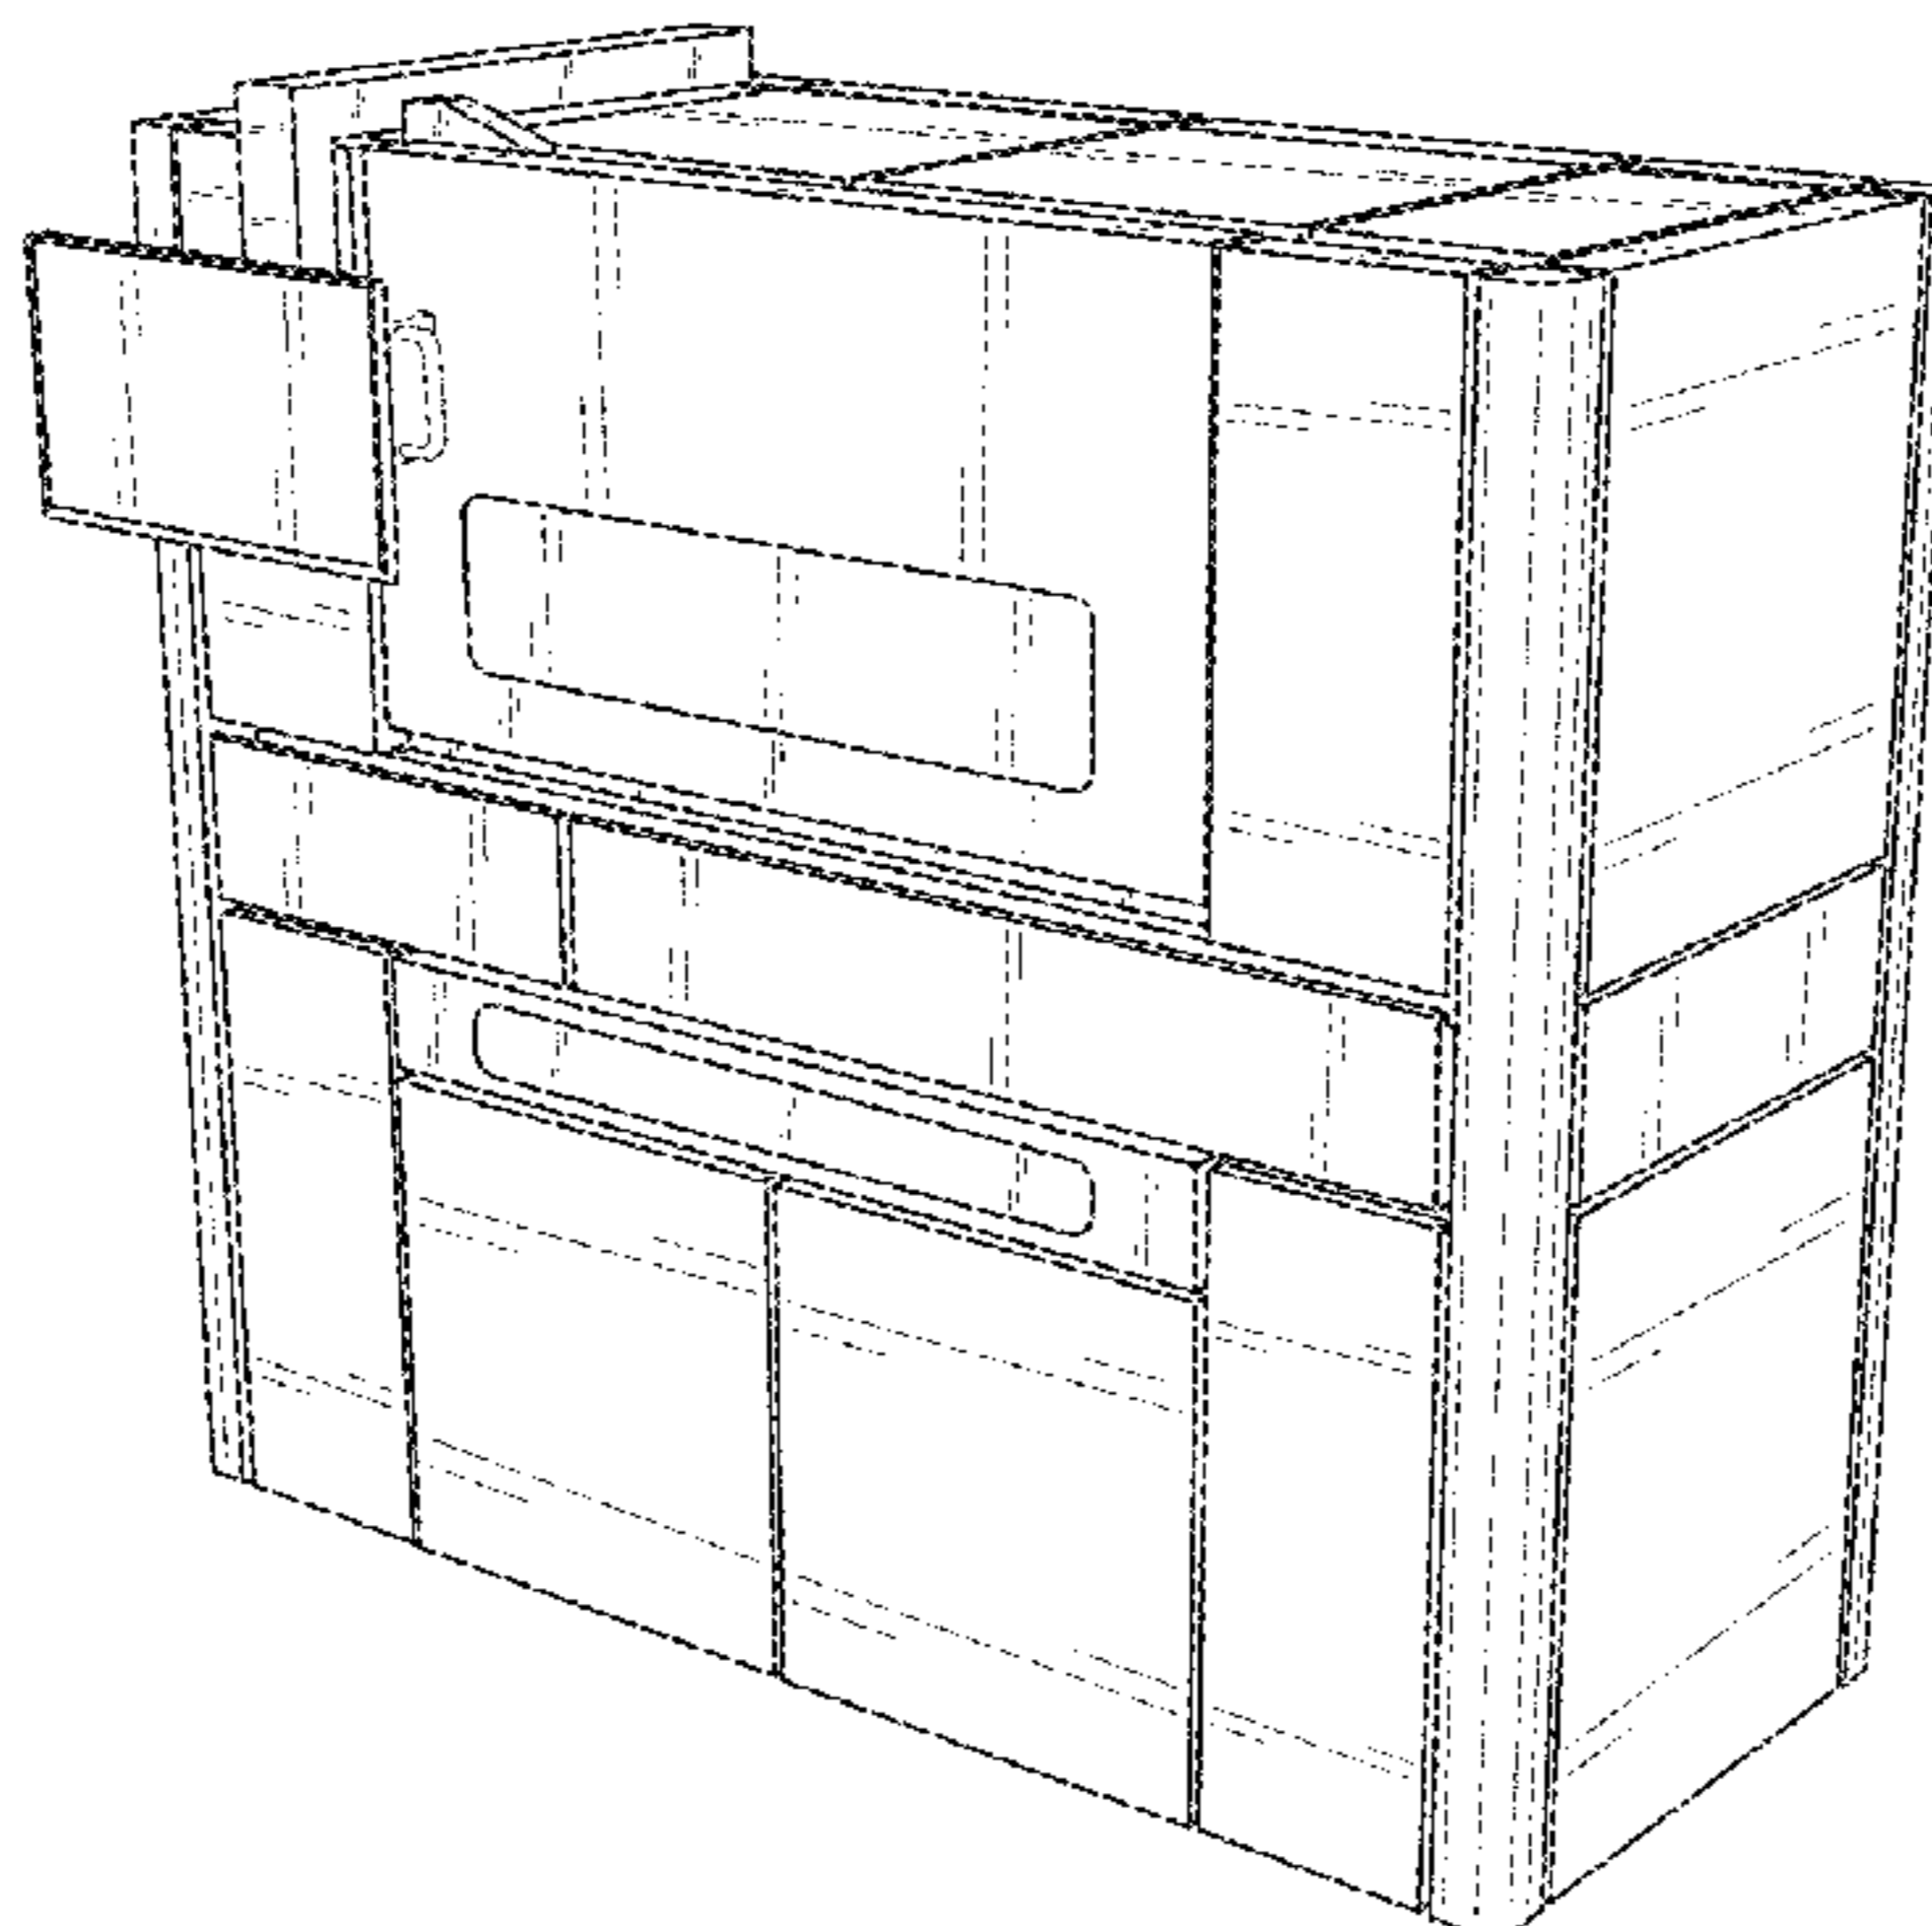


FIG. 19 is a top front perspective view thereof.  
 FIG. 20 is a top front perspective view thereof.  
 FIG. 21 is a front elevational view of a fifth embodiment of a diagnostic apparatus for medical or laboratory purposes.  
 FIG. 22 is a right side elevational view thereof.  
 FIG. 23 is a left side elevational view thereof.  
 FIG. 24 is a top front perspective view thereof; and,  
 FIG. 25 is a top front perspective view thereof.  
 The broken lines illustrate portions of the diagnostic apparatus that form no part of the claimed design.

**1 Claim, 25 Drawing Sheets  
 (6 of 25 Drawing Sheet(s) Filed in Color)**

(30) **Foreign Application Priority Data**

Jul. 20, 2018 (EM) ..... 005508876.0003  
 Jul. 20, 2018 (EM) ..... 005508876.0004  
 Jul. 20, 2018 (EM) ..... 005508876.0005  
 Jul. 20, 2018 (EM) ..... 005508876.0006  
 Jul. 20, 2018 (EM) ..... 005508876.0007  
 Jul. 20, 2018 (EM) ..... 005508876.0008  
 Jul. 20, 2018 (EM) ..... 005508876.0009  
 Jul. 20, 2018 (EM) ..... 005508876.0010

(58) **Field of Classification Search**

CPC ..... G01N 2035/00306; G01N 2035/00326;  
 G01N 2035/00336; G01N 2030/027;  
 G01N 21/76

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D662,431 S 6/2012 Kimura  
 D690,023 S \* 9/2013 Chang ..... D24/216  
 D698,038 S 1/2014 Davis et al.

D705,944 S 5/2014 Chang et al.  
 D716,966 S 11/2014 Lizari Illarramendi  
 D774,659 S 12/2016 Quackenbush et al.  
 D777,049 S 1/2017 Barton et al.  
 D780,935 S 3/2017 Goos et al.  
 D791,338 S 7/2017 Morkos et al.  
 D799,999 S 10/2017 Barton et al.  
 D802,156 S 11/2017 Barton et al.  
 D802,785 S 11/2017 Barton et al.  
 D808,038 S 1/2018 Böhm et al.  
 D843,005 S 3/2019 Kobeli et al.  
 D875,963 S 2/2020 Gruen  
 D883,510 S 5/2020 Neuman  
 D888,985 S 6/2020 Hsieh  
 D896,981 S \* 9/2020 Gruen ..... D24/232  
 D907,245 S 1/2021 Rateike et al.  
 D914,230 S \* 3/2021 Kaffka ..... D24/216  
 2013/0288355 A1 10/2013 DeWitte et al.  
 2016/0161428 A1 6/2016 Takahara et al.  
 2017/0269114 A1 9/2017 Bryant et al.

OTHER PUBLICATIONS

Hüwelmann et al., "Apparatus and equipment for doctors, hospitals and laboratories", EUROIMMUN Medizinische Labordiagnostika AG, Germany, filed Aug. 25, 2021, European Union Intellectual Property Organization design Nos. 008661094-0001, 008661094-0002, 008661094-0003, 008661094-0004, 008661094-0005, 008661094-0006.

Official Gazette Publication 2545 published Oct. 15, 2019 in Brazilian Design Application No. BR 30 2019 004439-0 dated Sep. 19, 2019; p. 72/320.

Official Gazette Publication 2560 published Jan. 28, 2020 in Brazilian Design Application No. BR 30 2019 004439-0 dated Sep. 19, 2019; p. 63/203.

Rateike et al., "Apparatus and equipment for doctors, hospitals and laboratories", EUROIMMUN Medizinische Labordiagnostika AG, Germany, filed Mar. 22, 2019, European Union Intellectual Property Organization design Nos. 006319323-0001, 006319323-0002, 006319323-0003, 006319323-0004.

U.S. Appl. No. 29/791,970, filed Feb. 23, 2022, Christian Hüwelmann.

\* cited by examiner

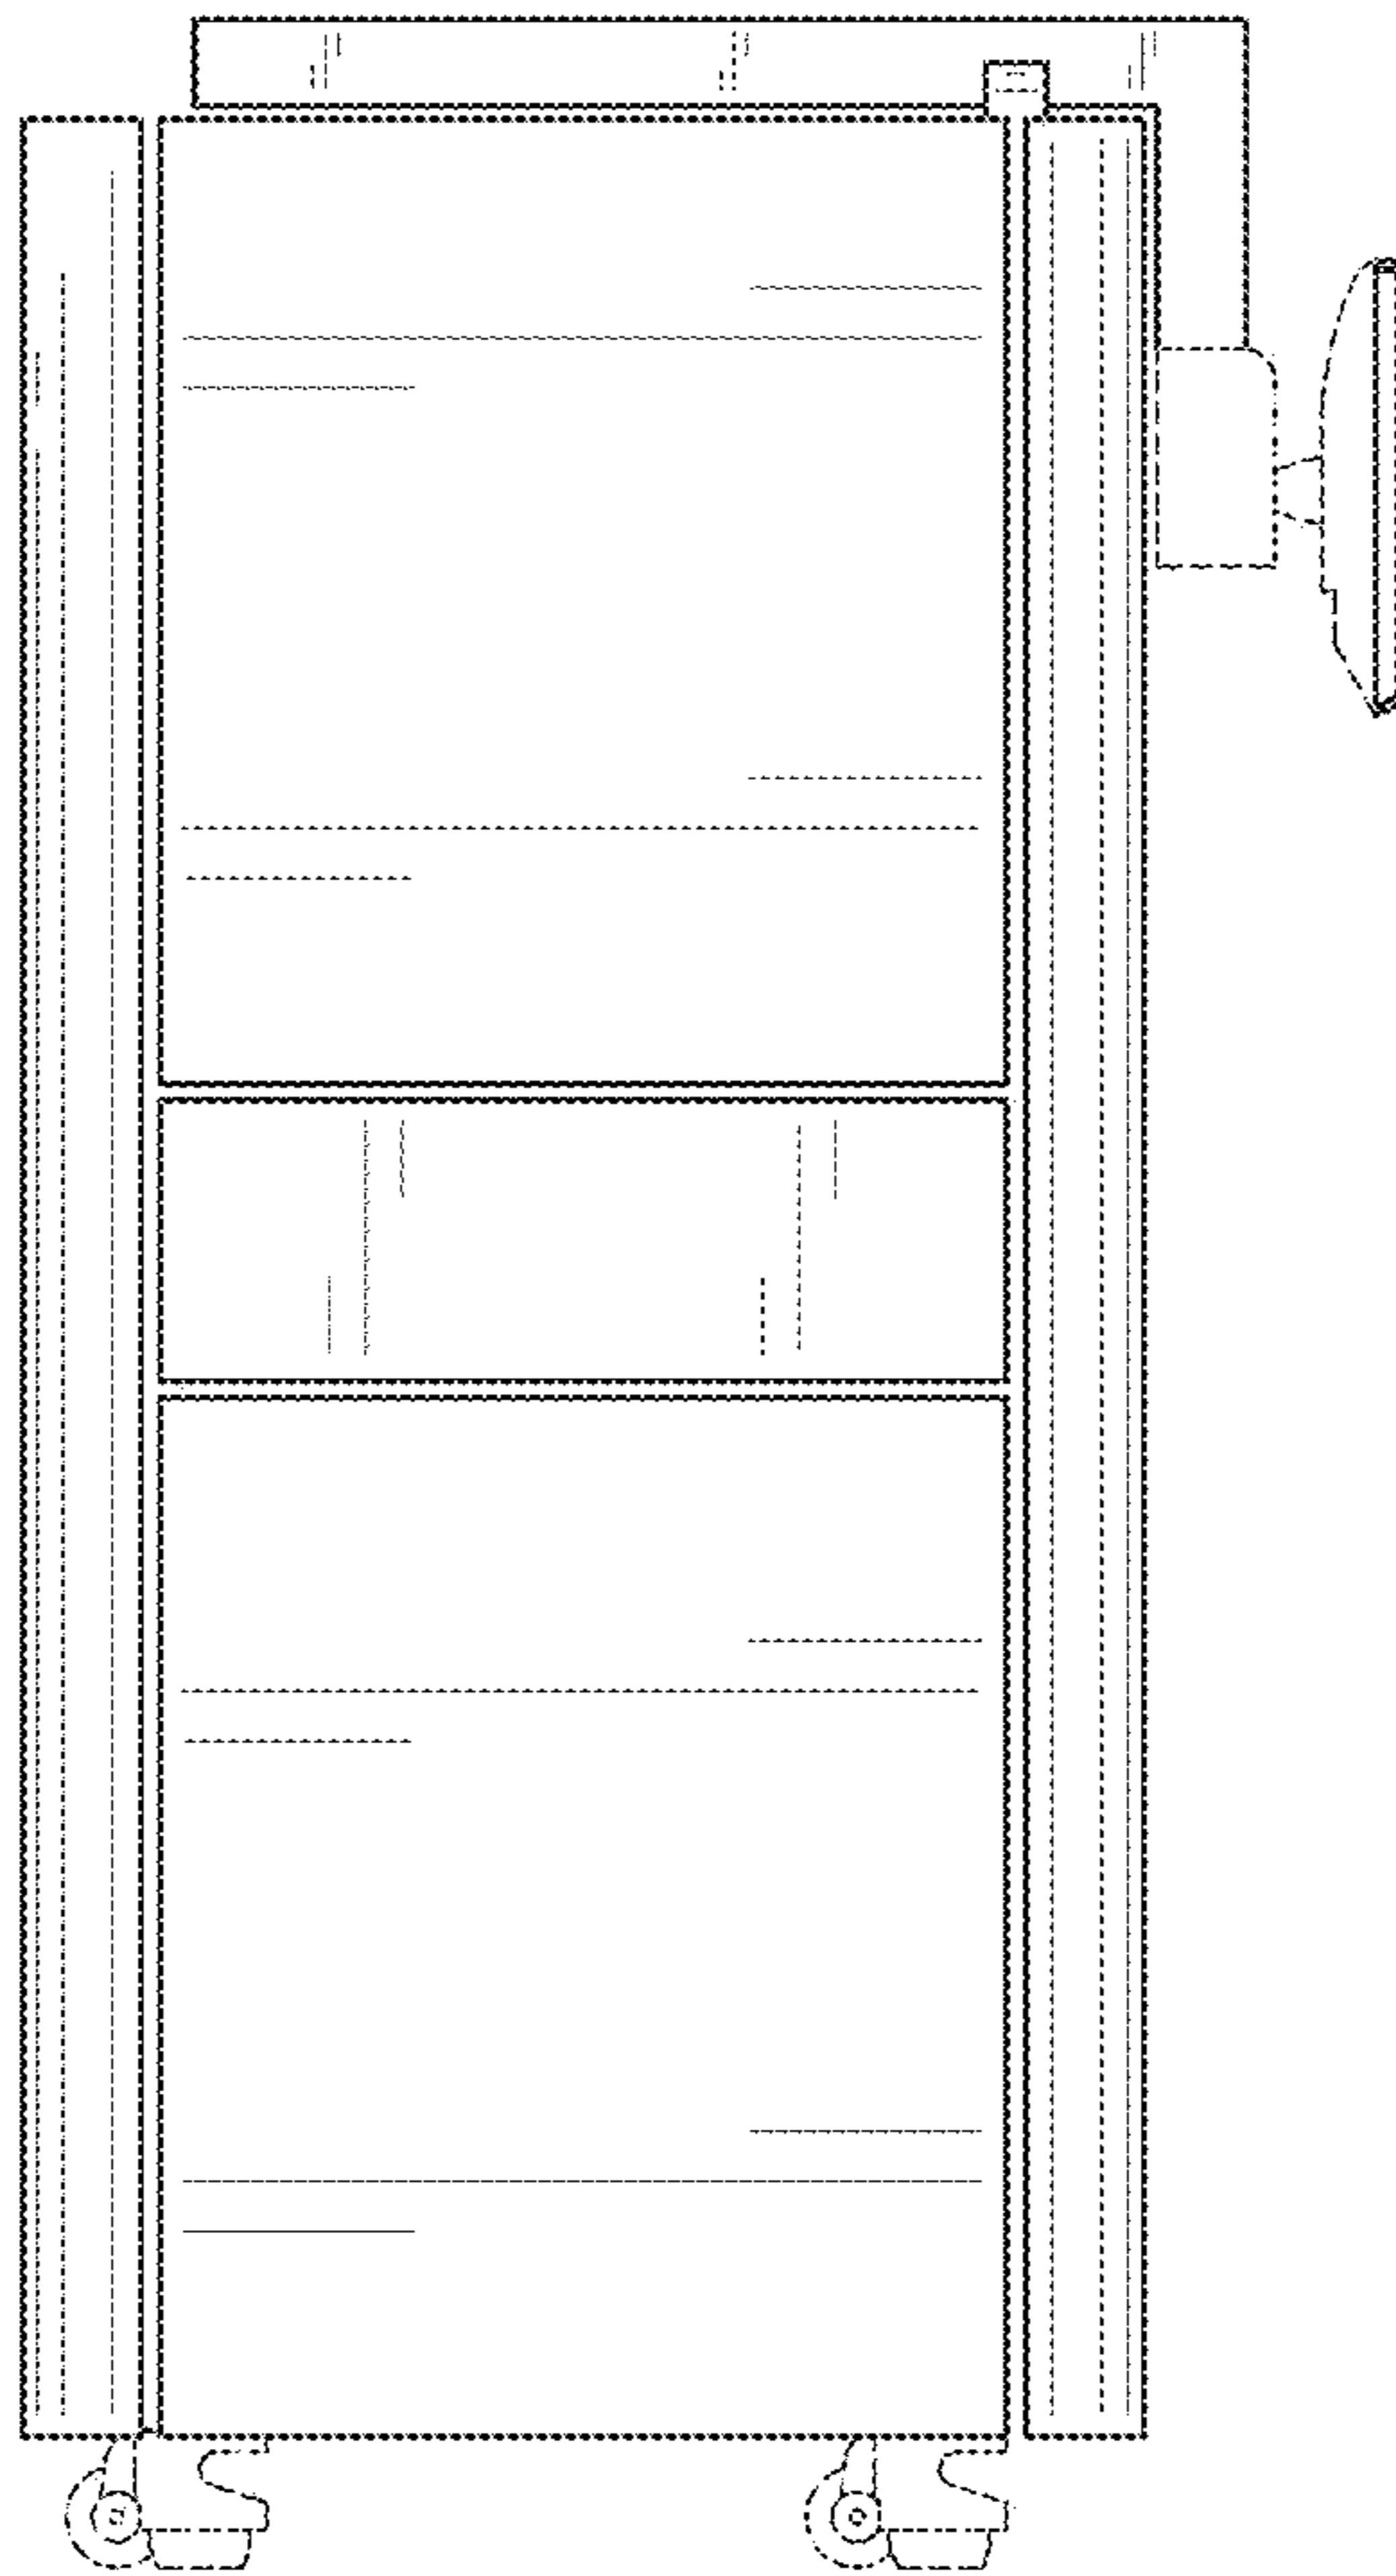


FIG. 1

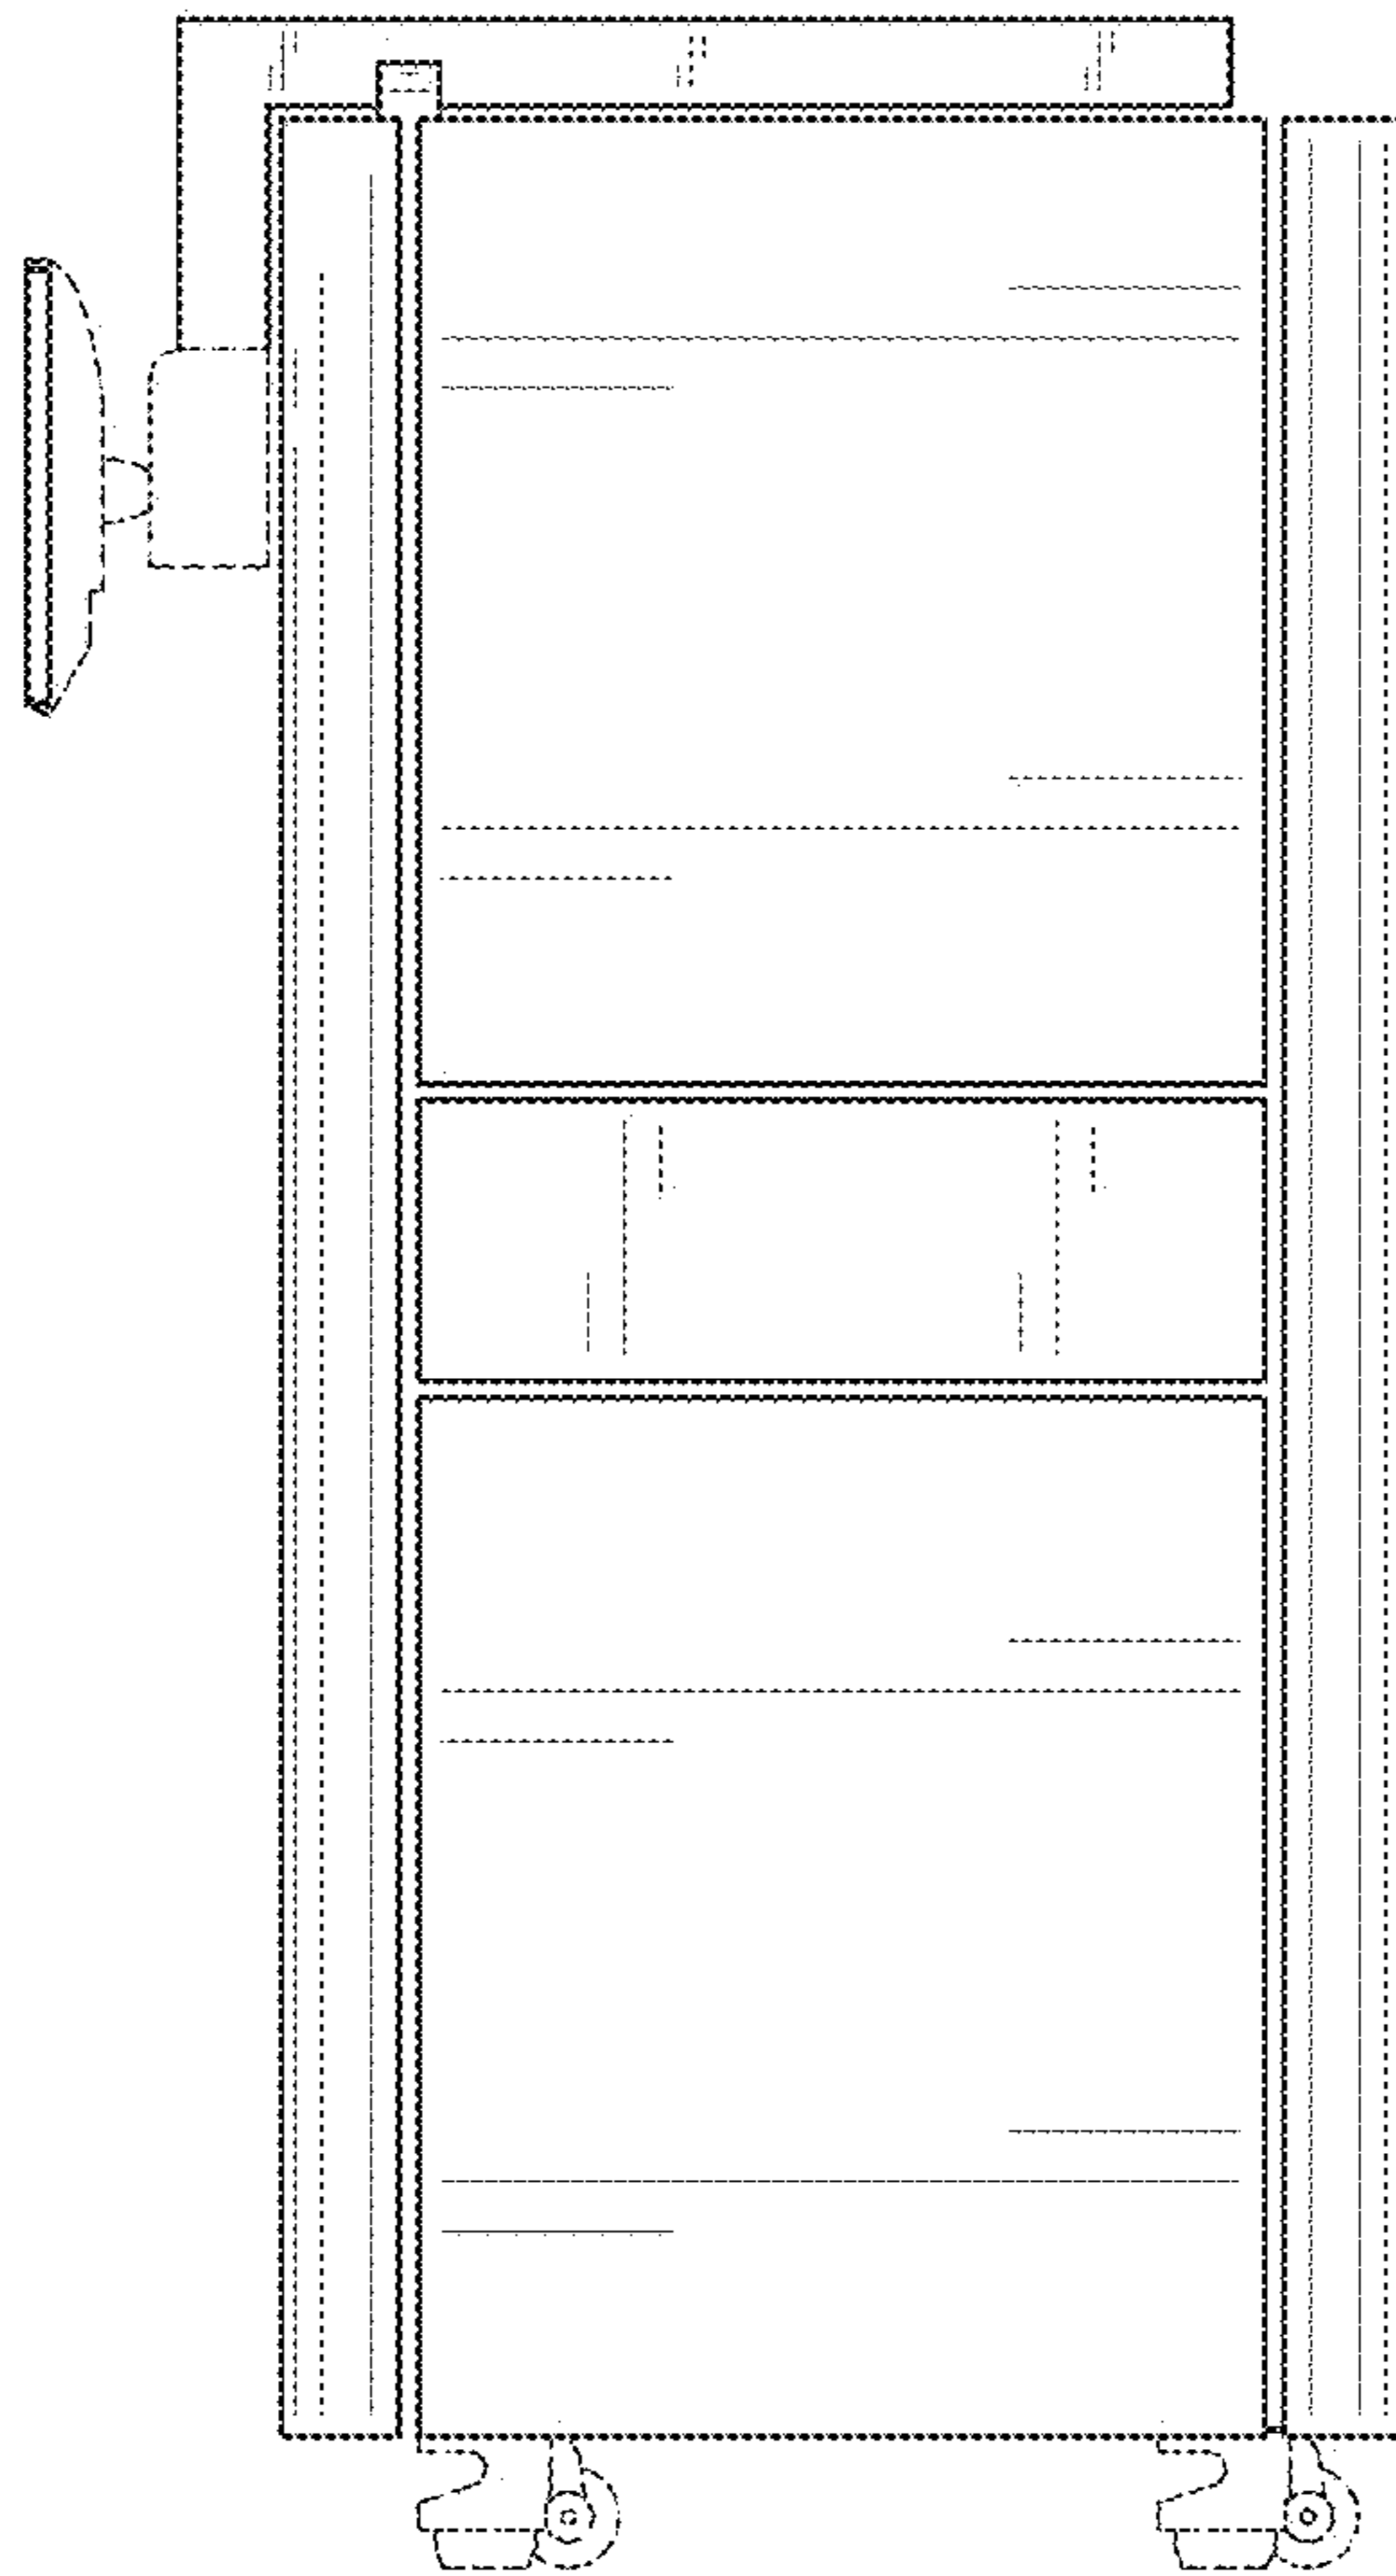


FIG. 2

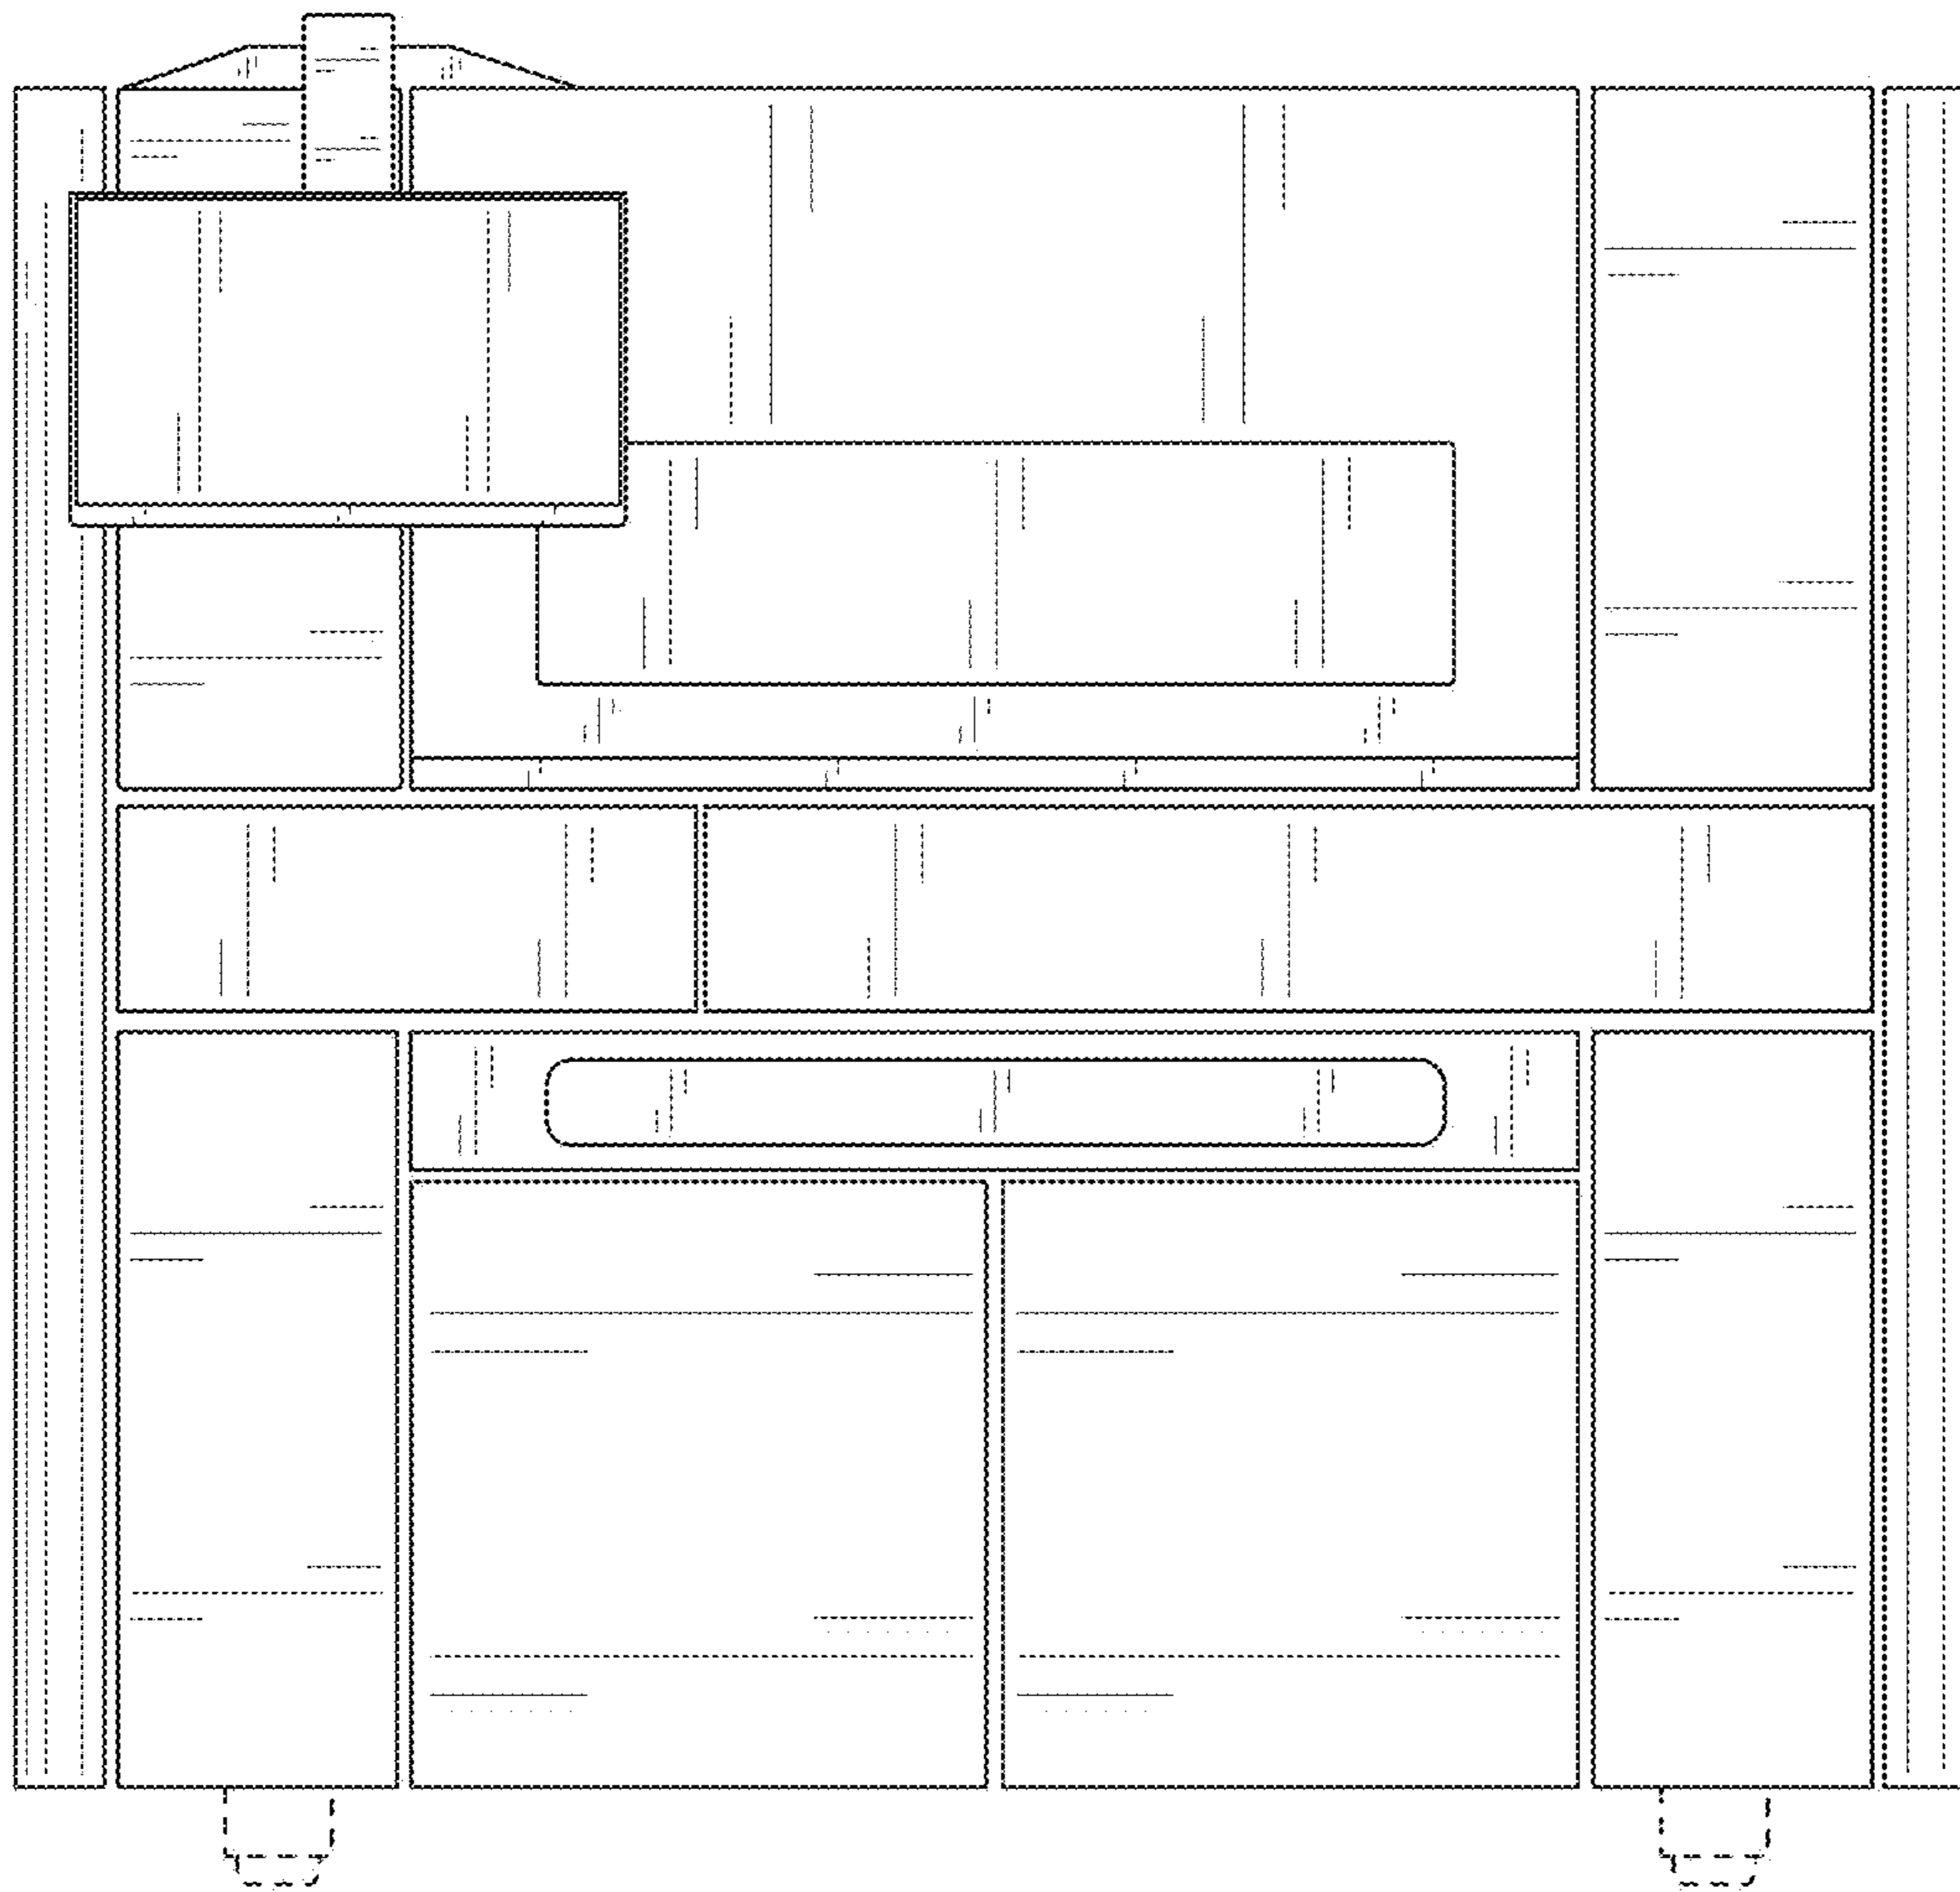


Fig. 3

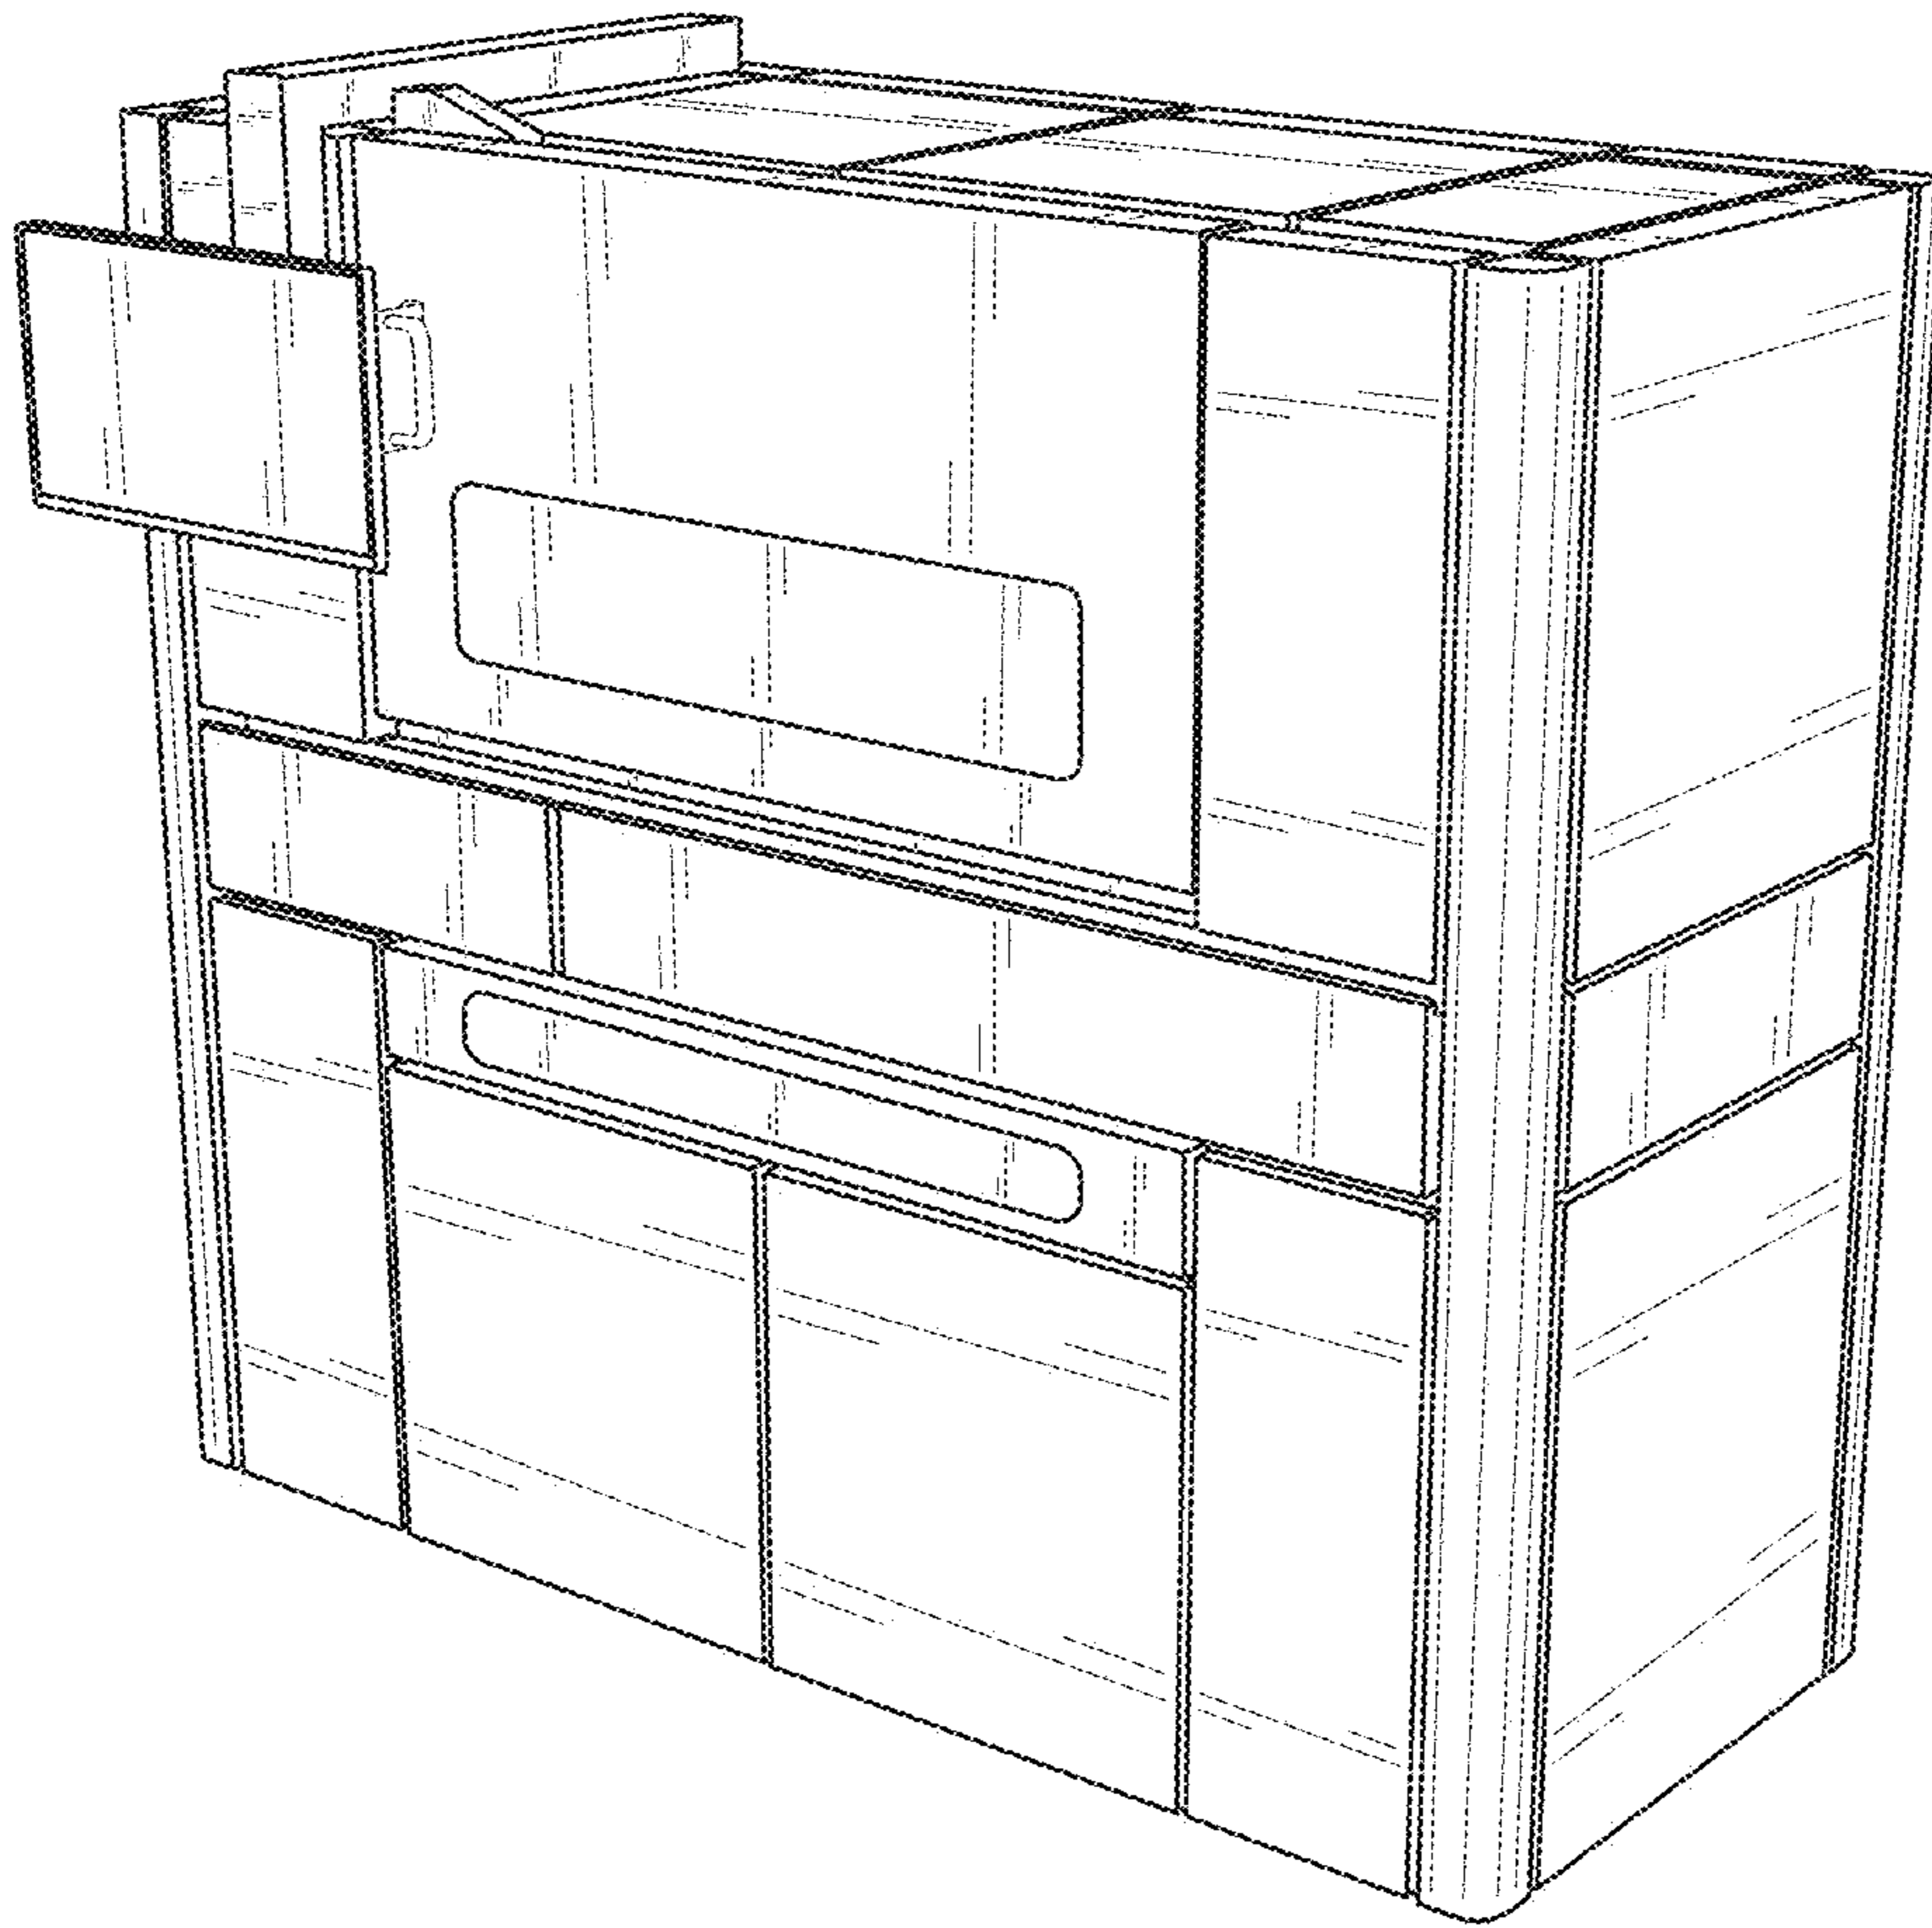


FIG. 4

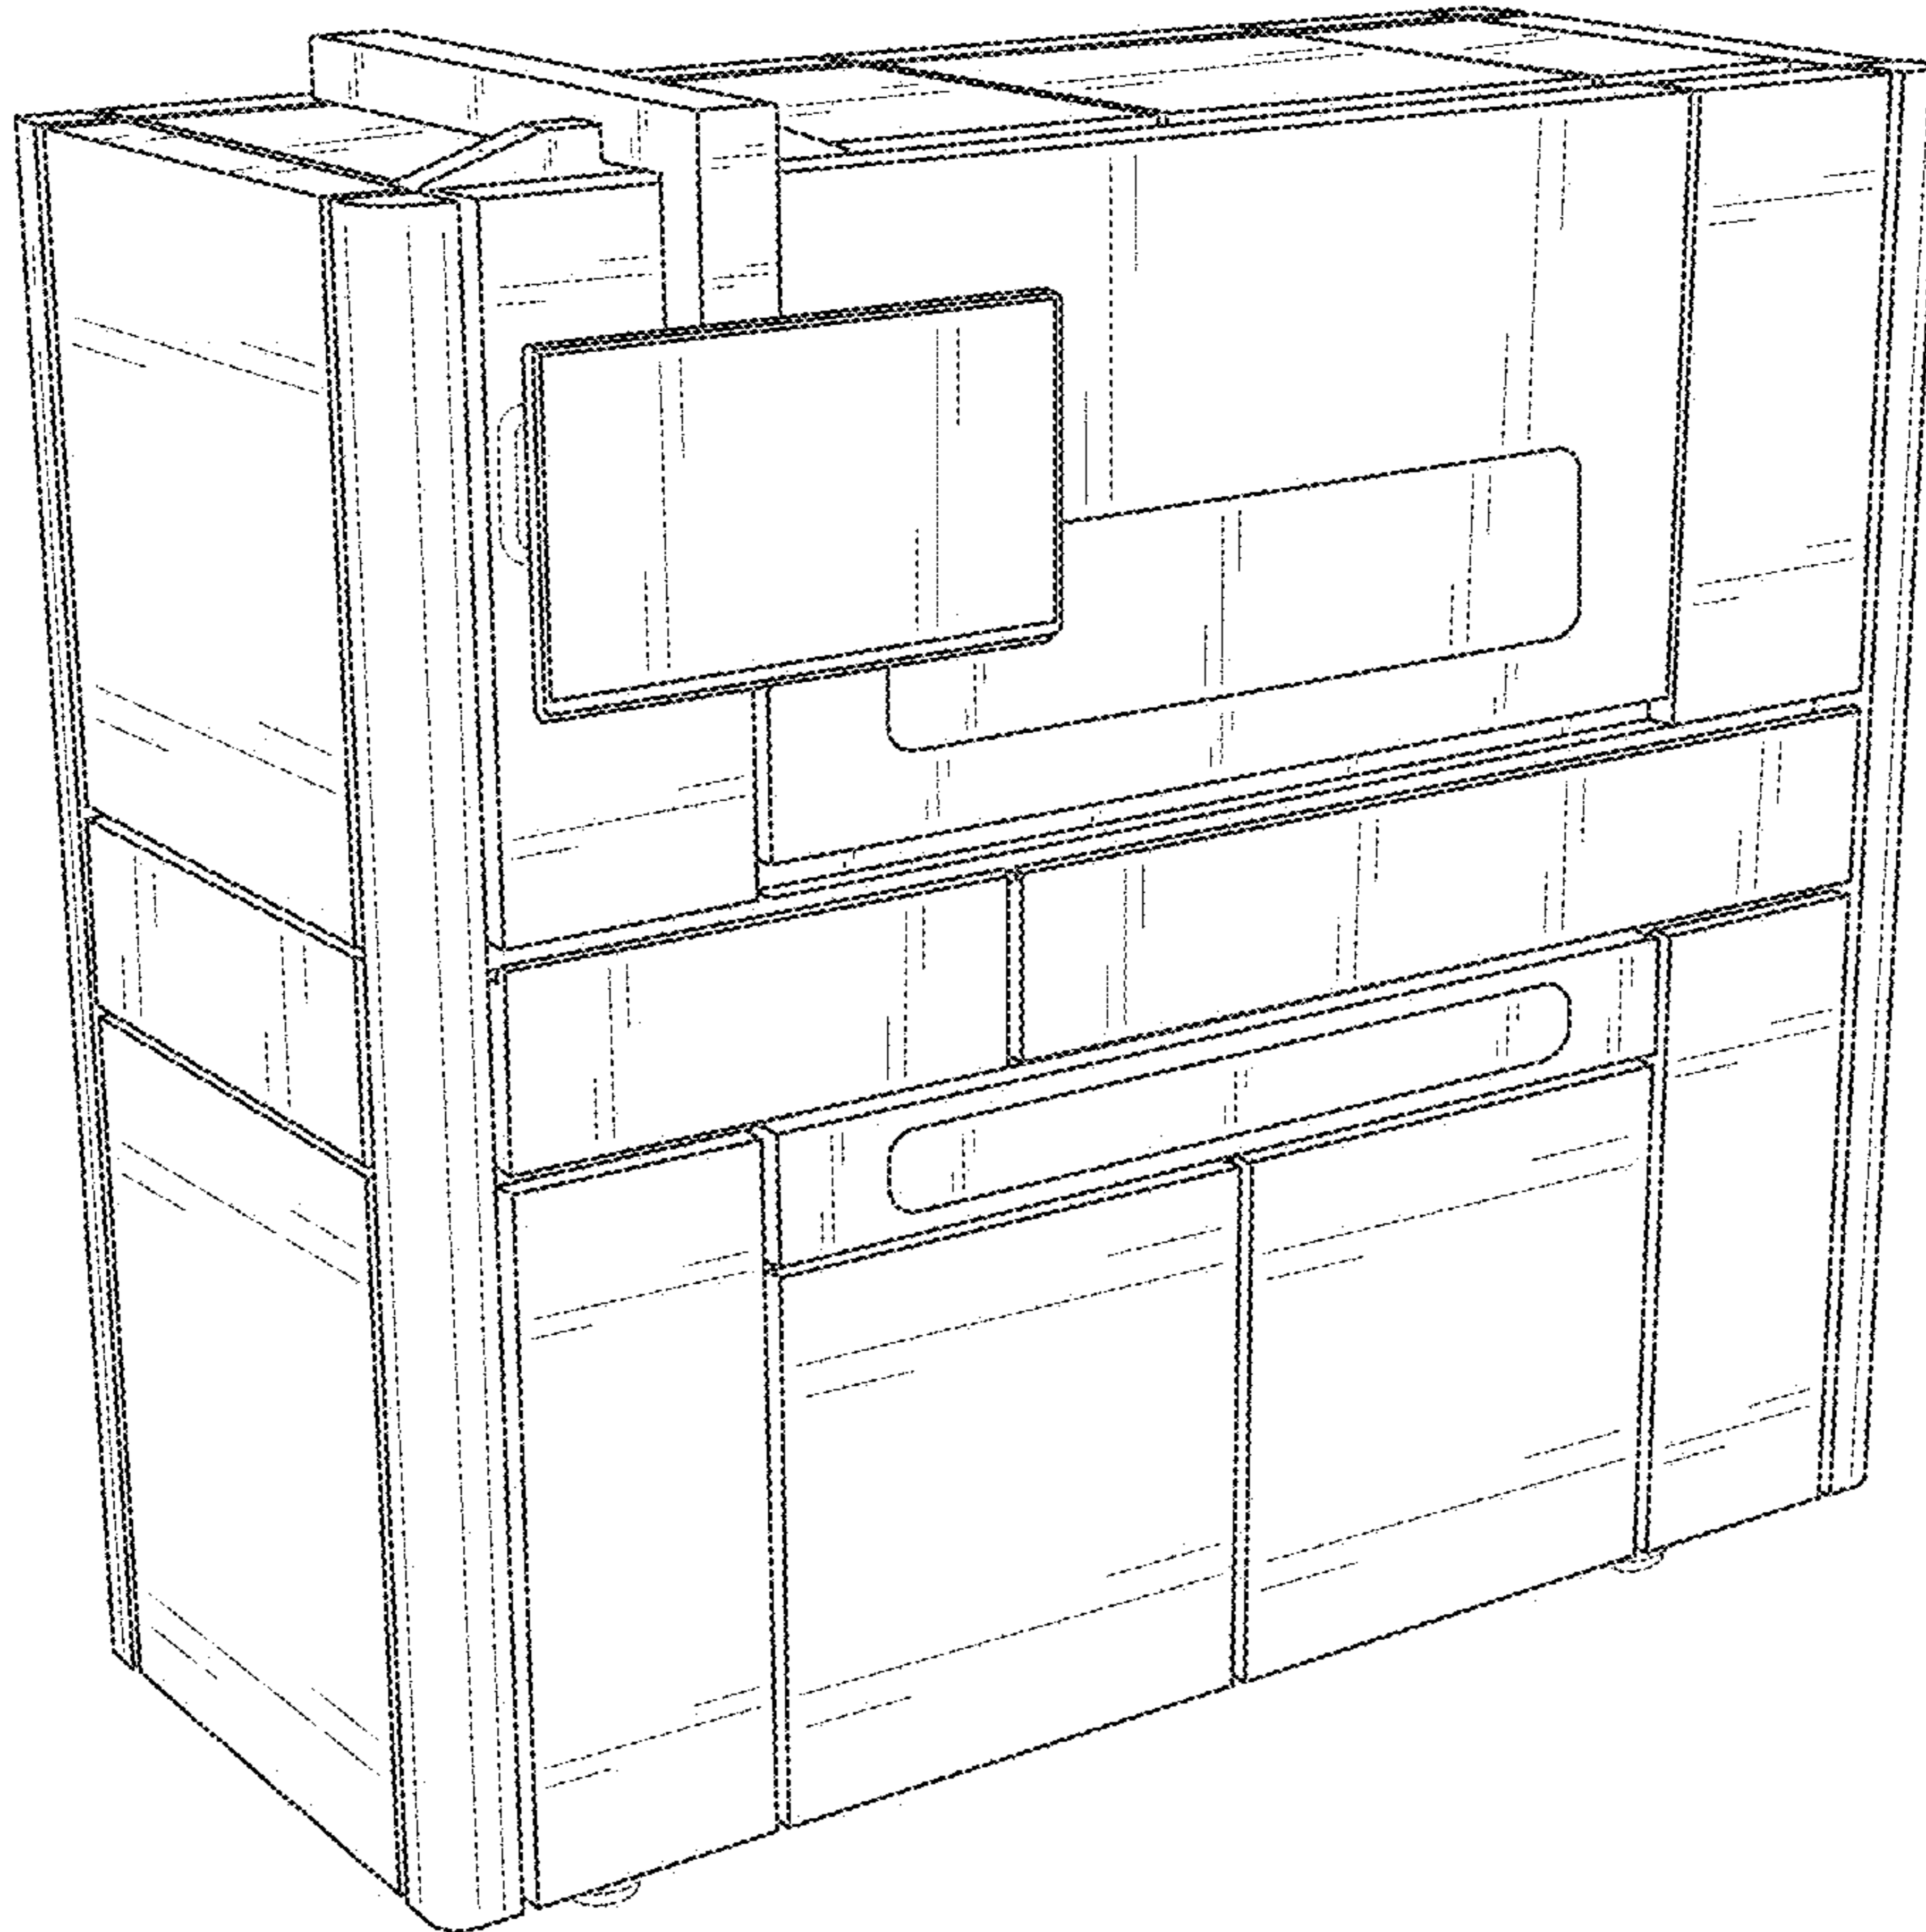


FIG. 5

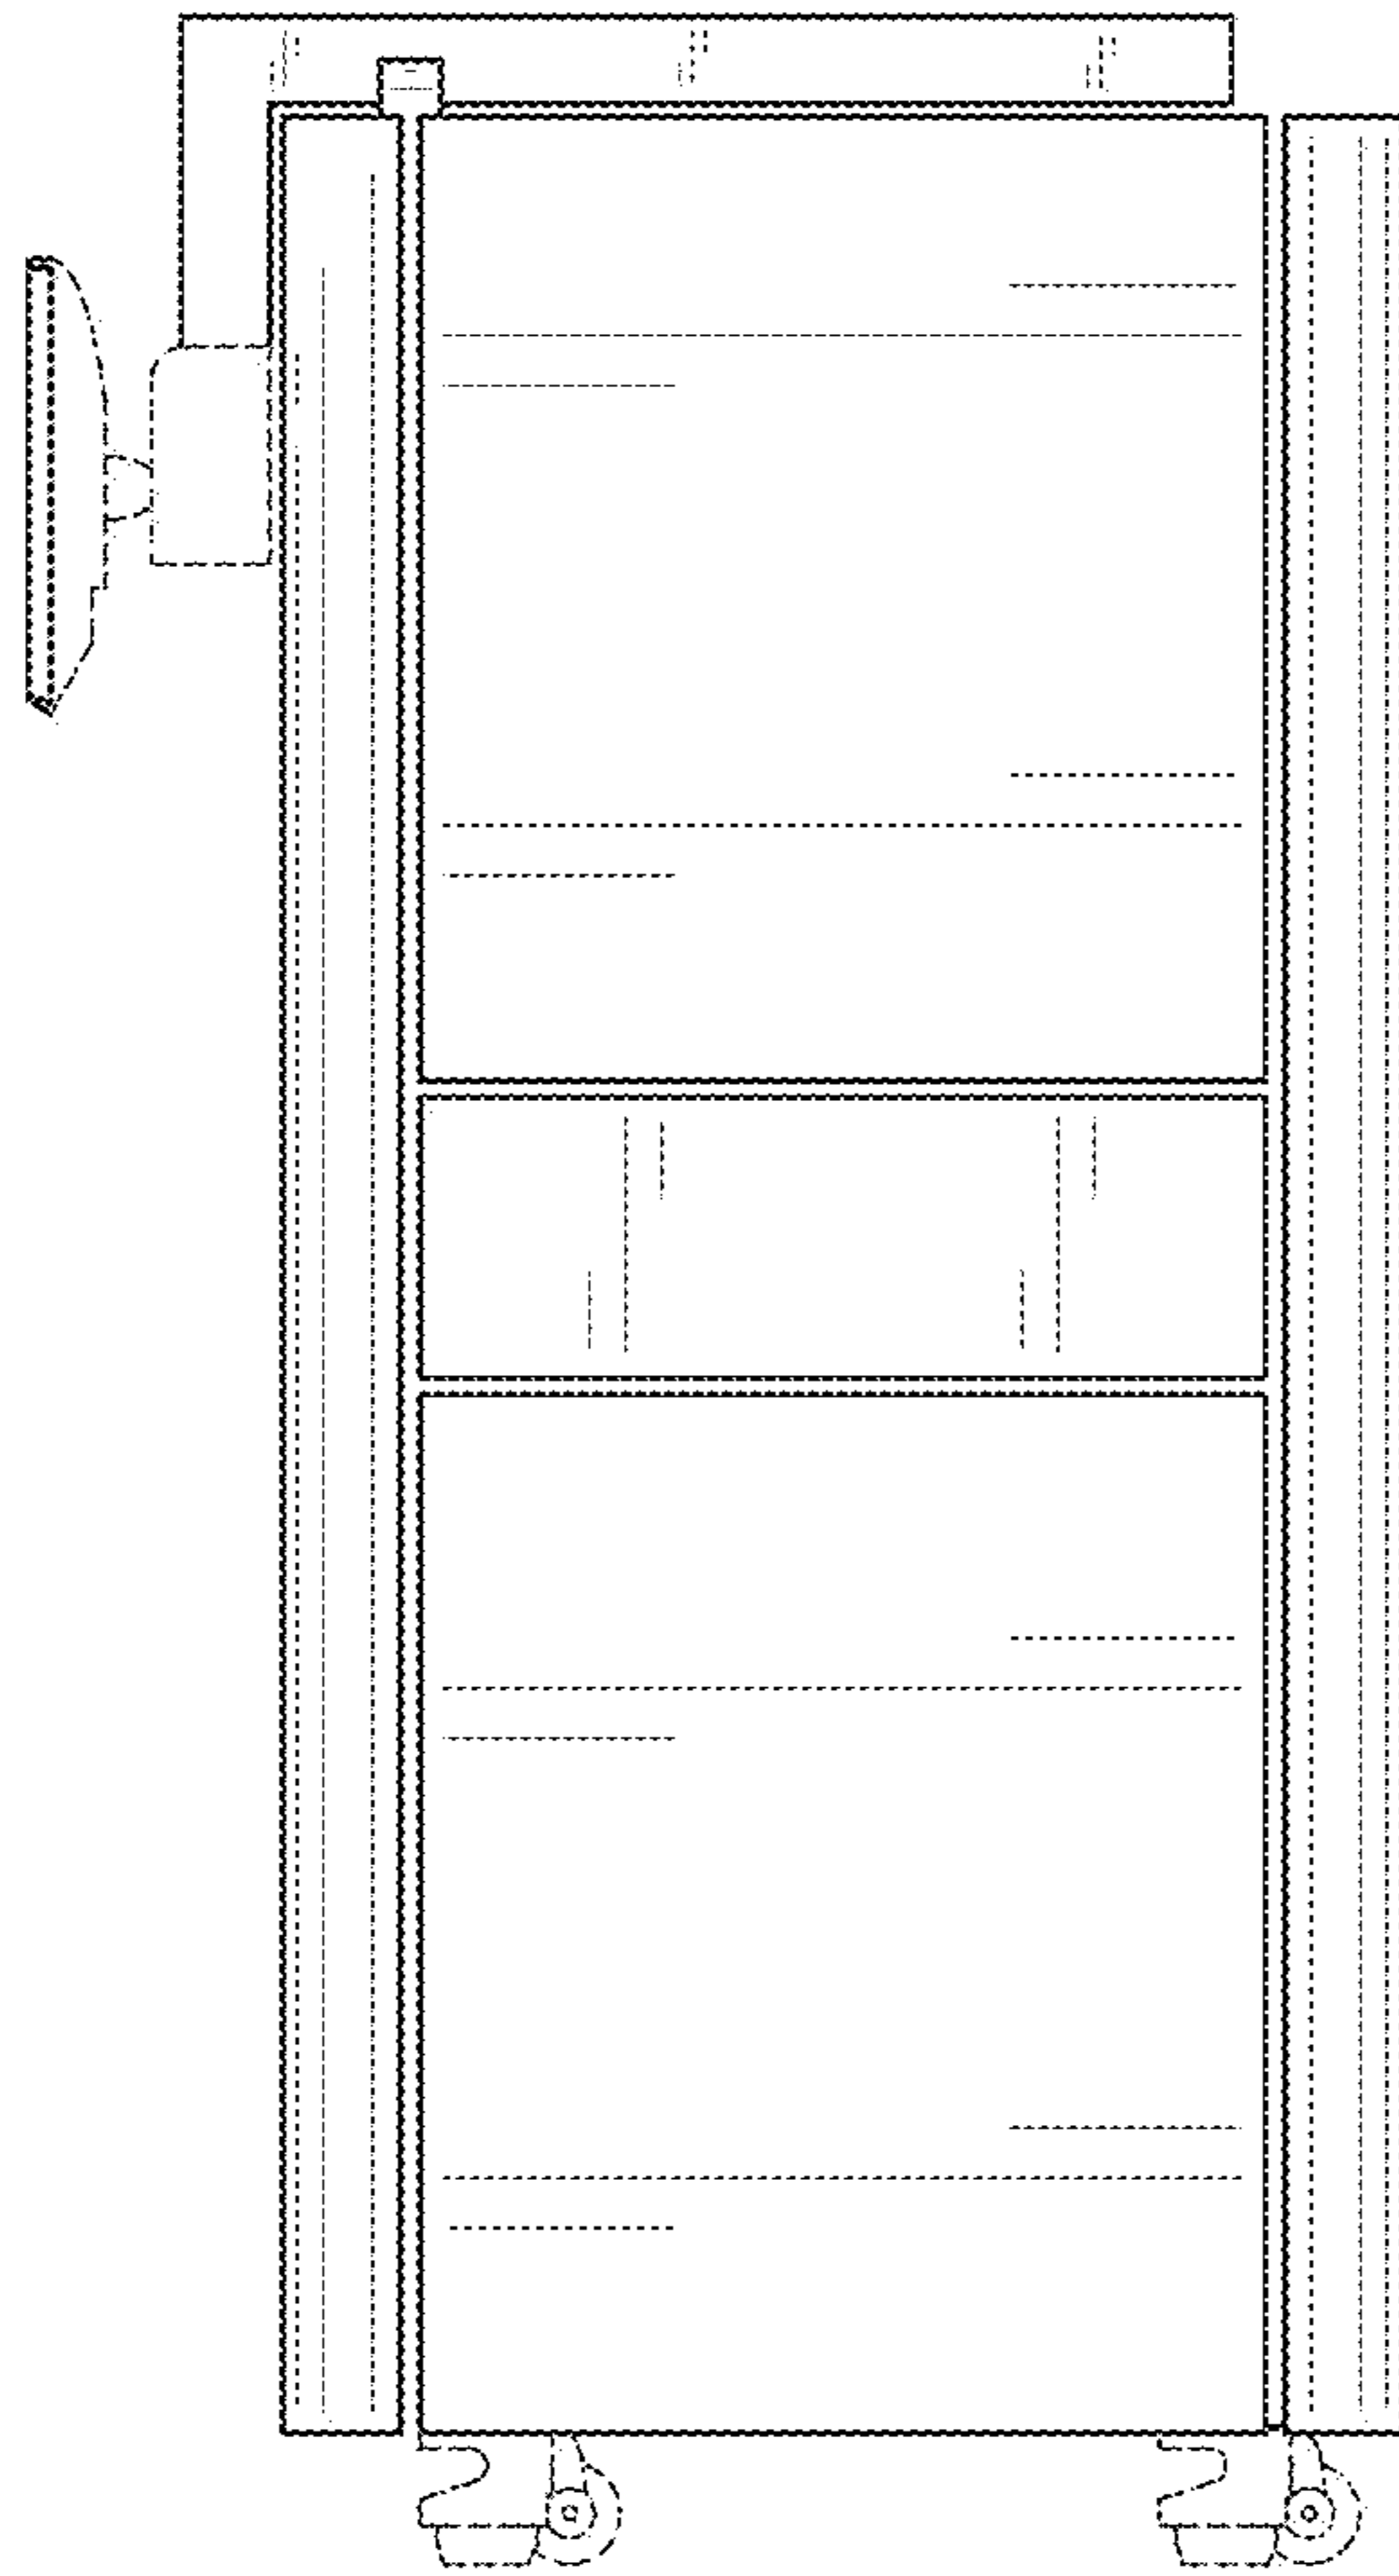


FIG. 6



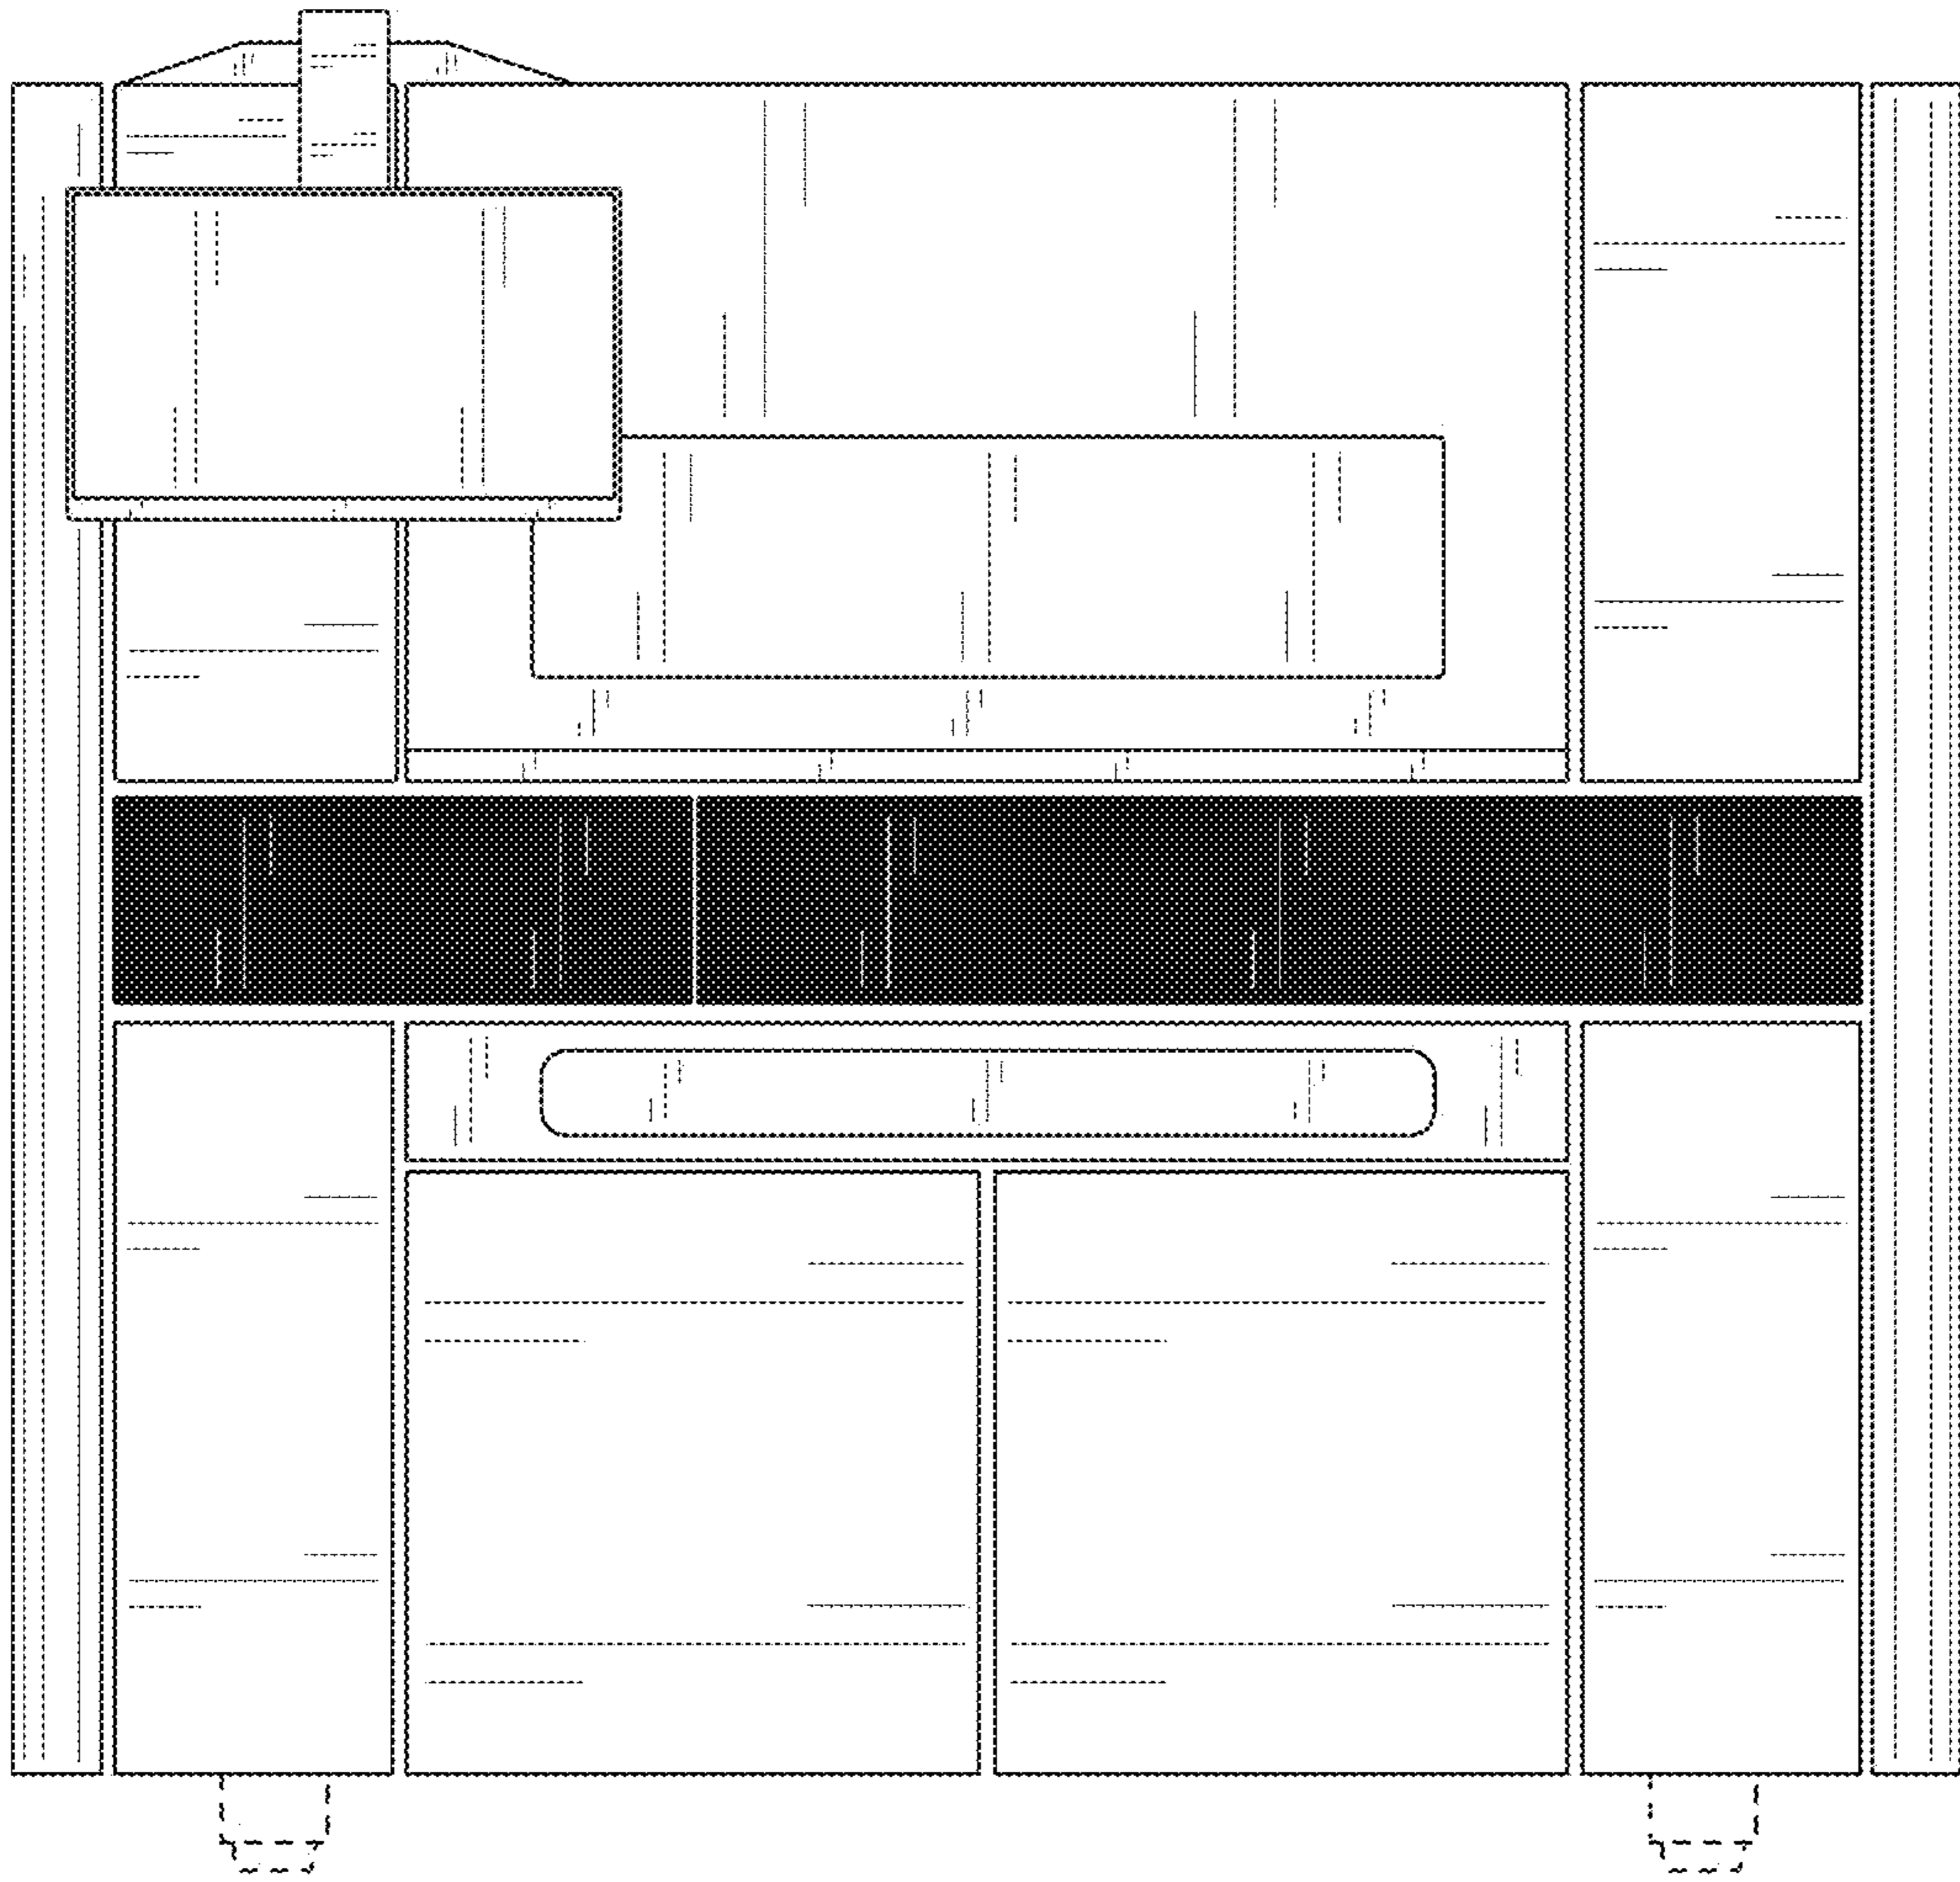


Fig. 7

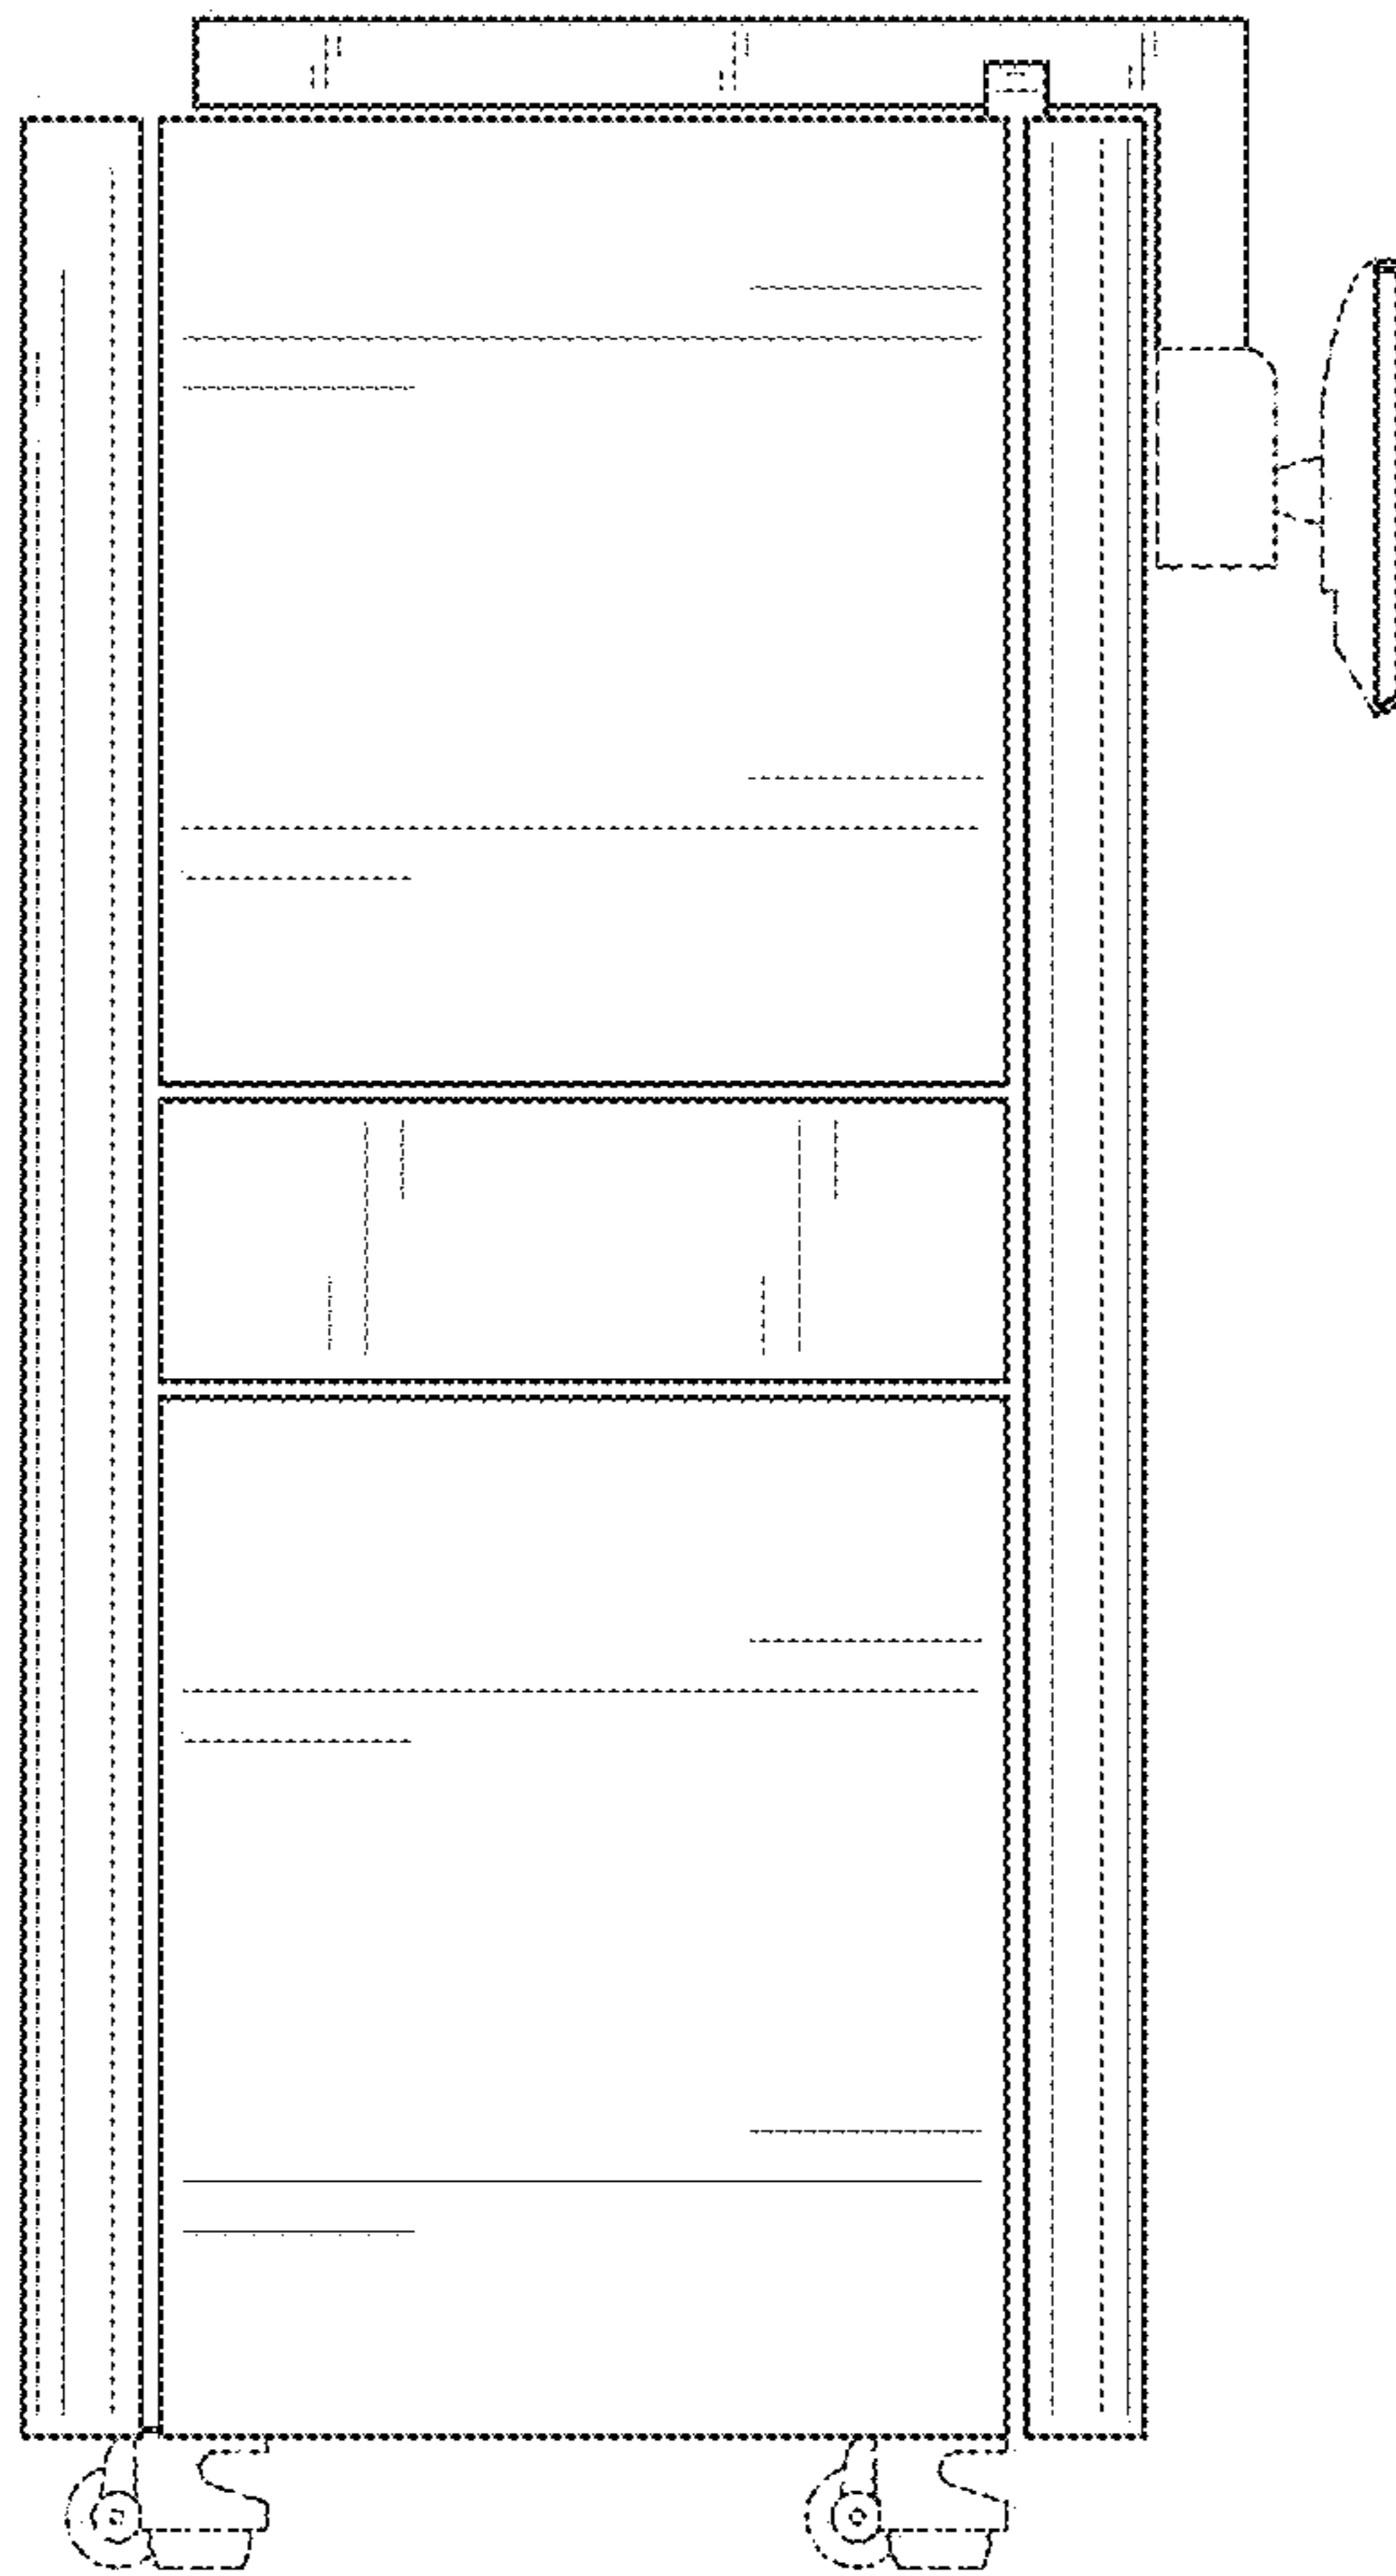


FIG. 8

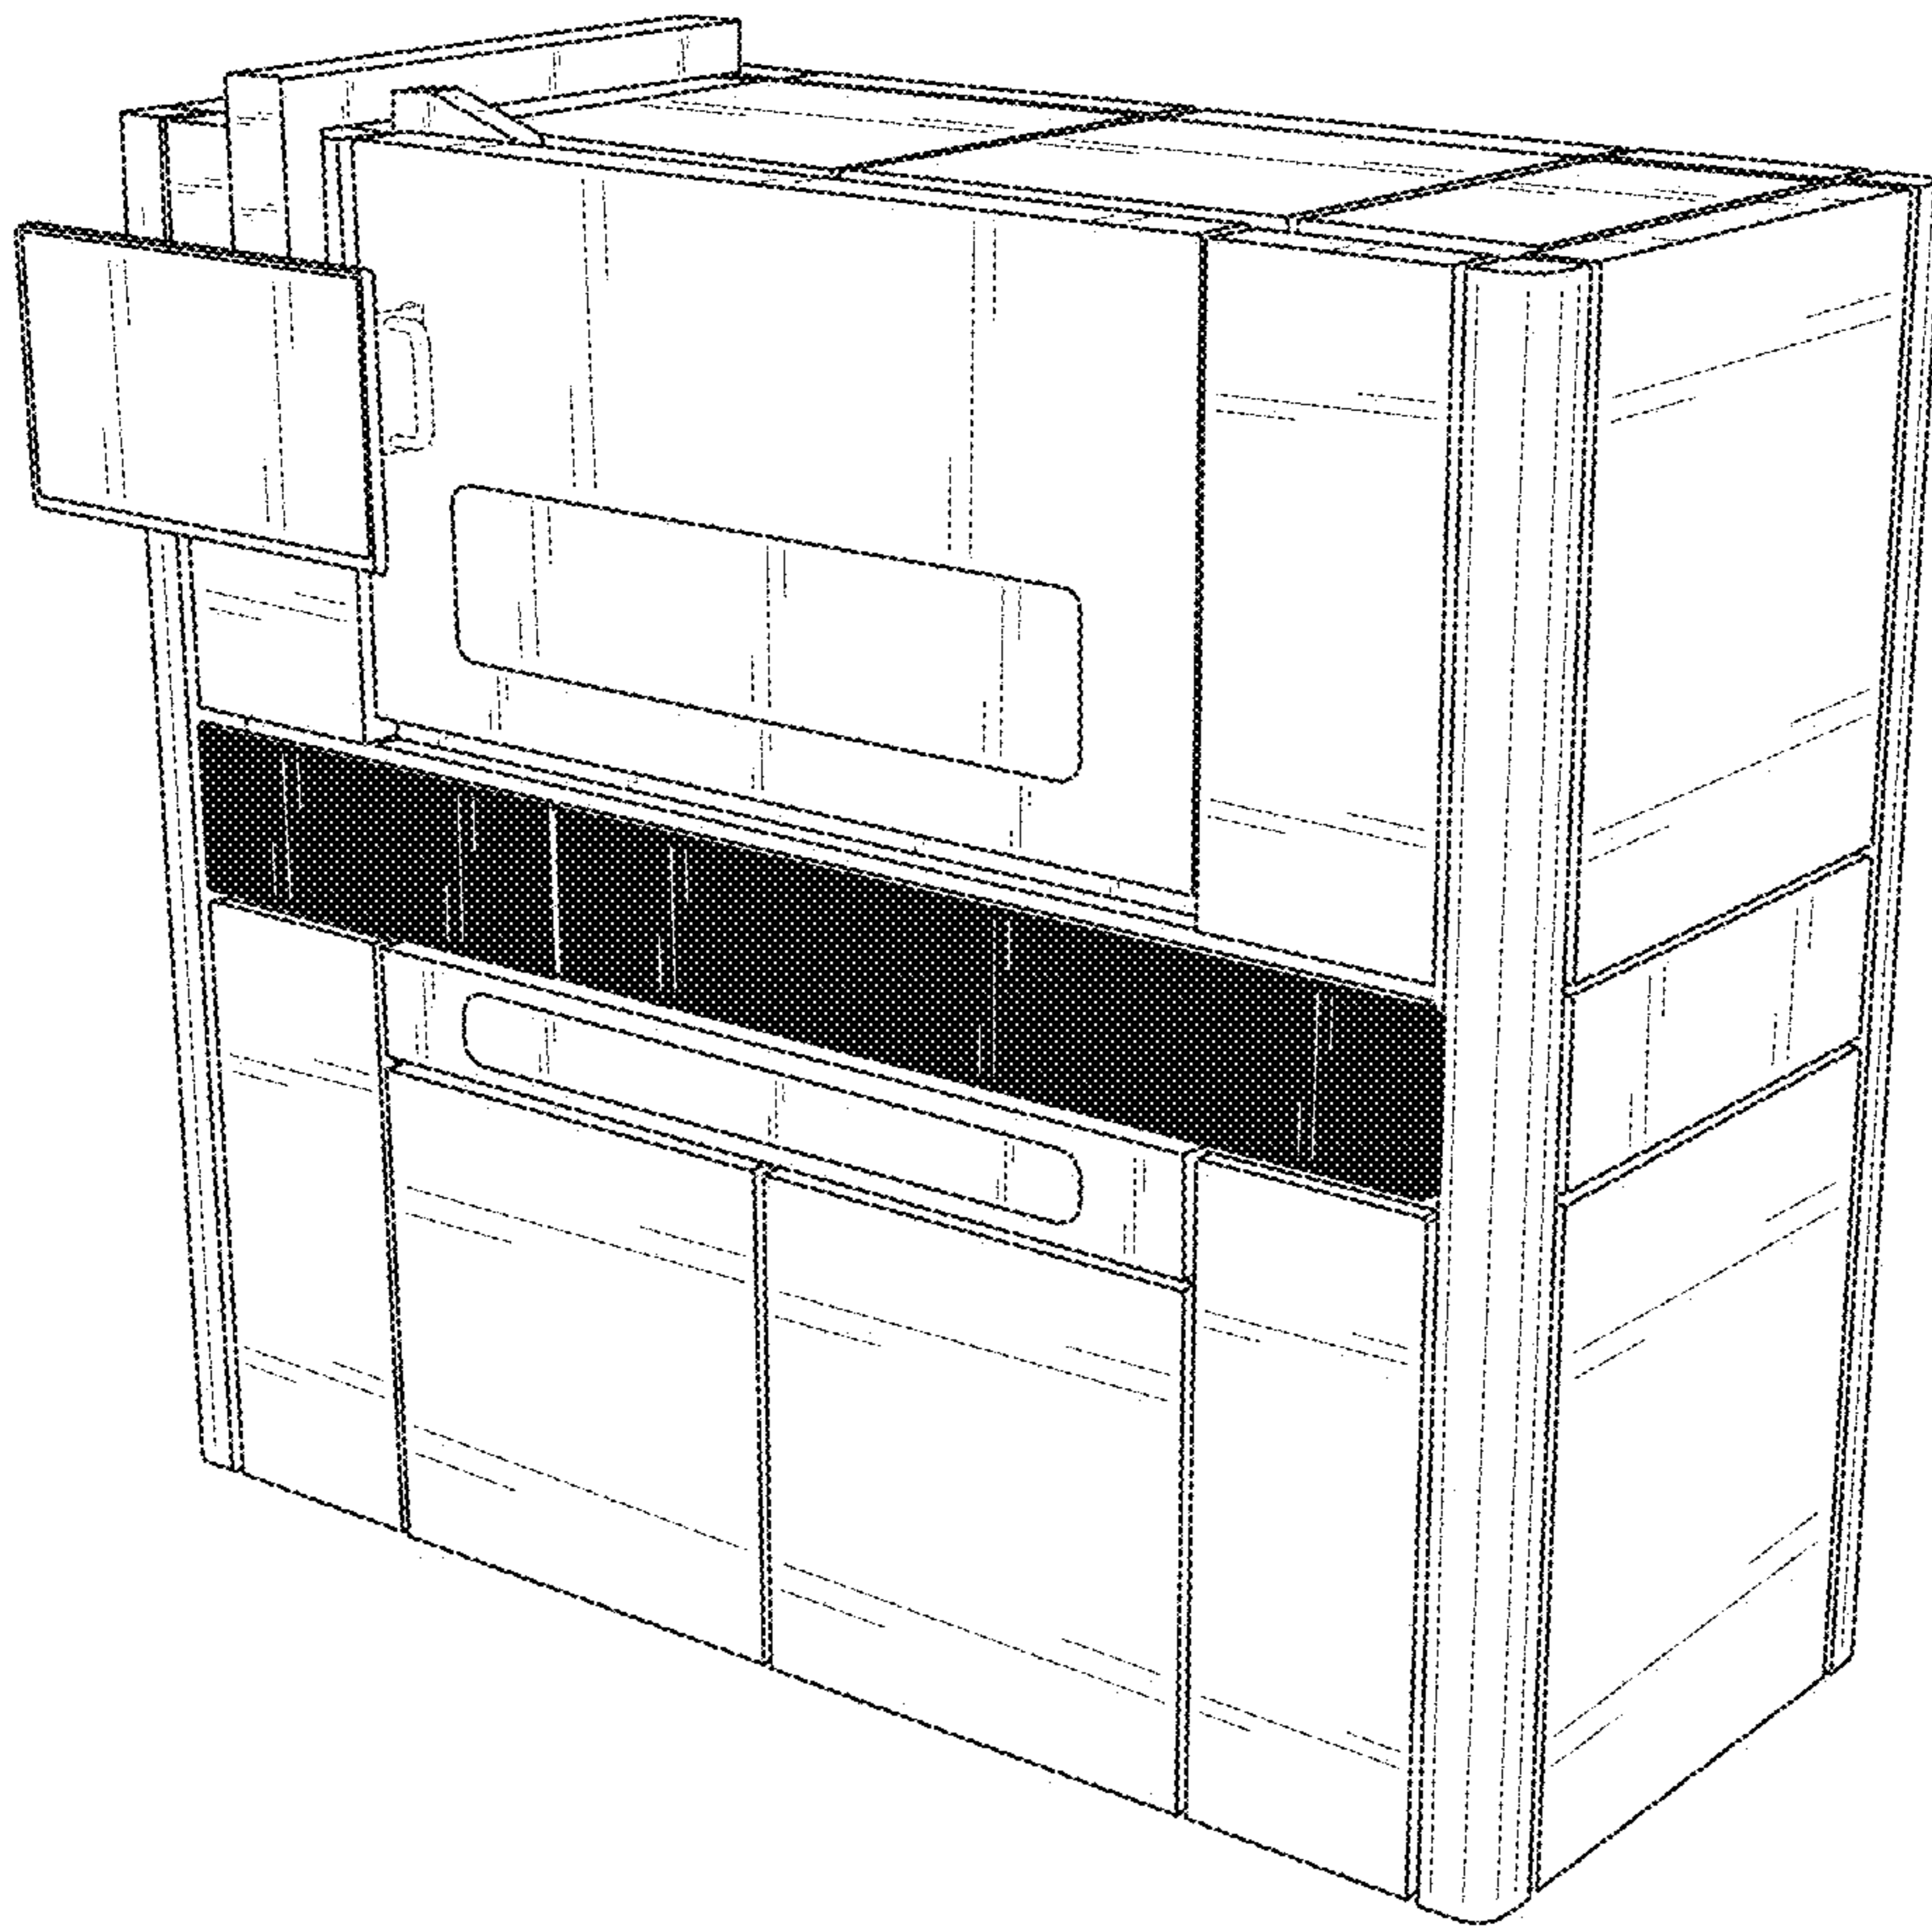


FIG. 9

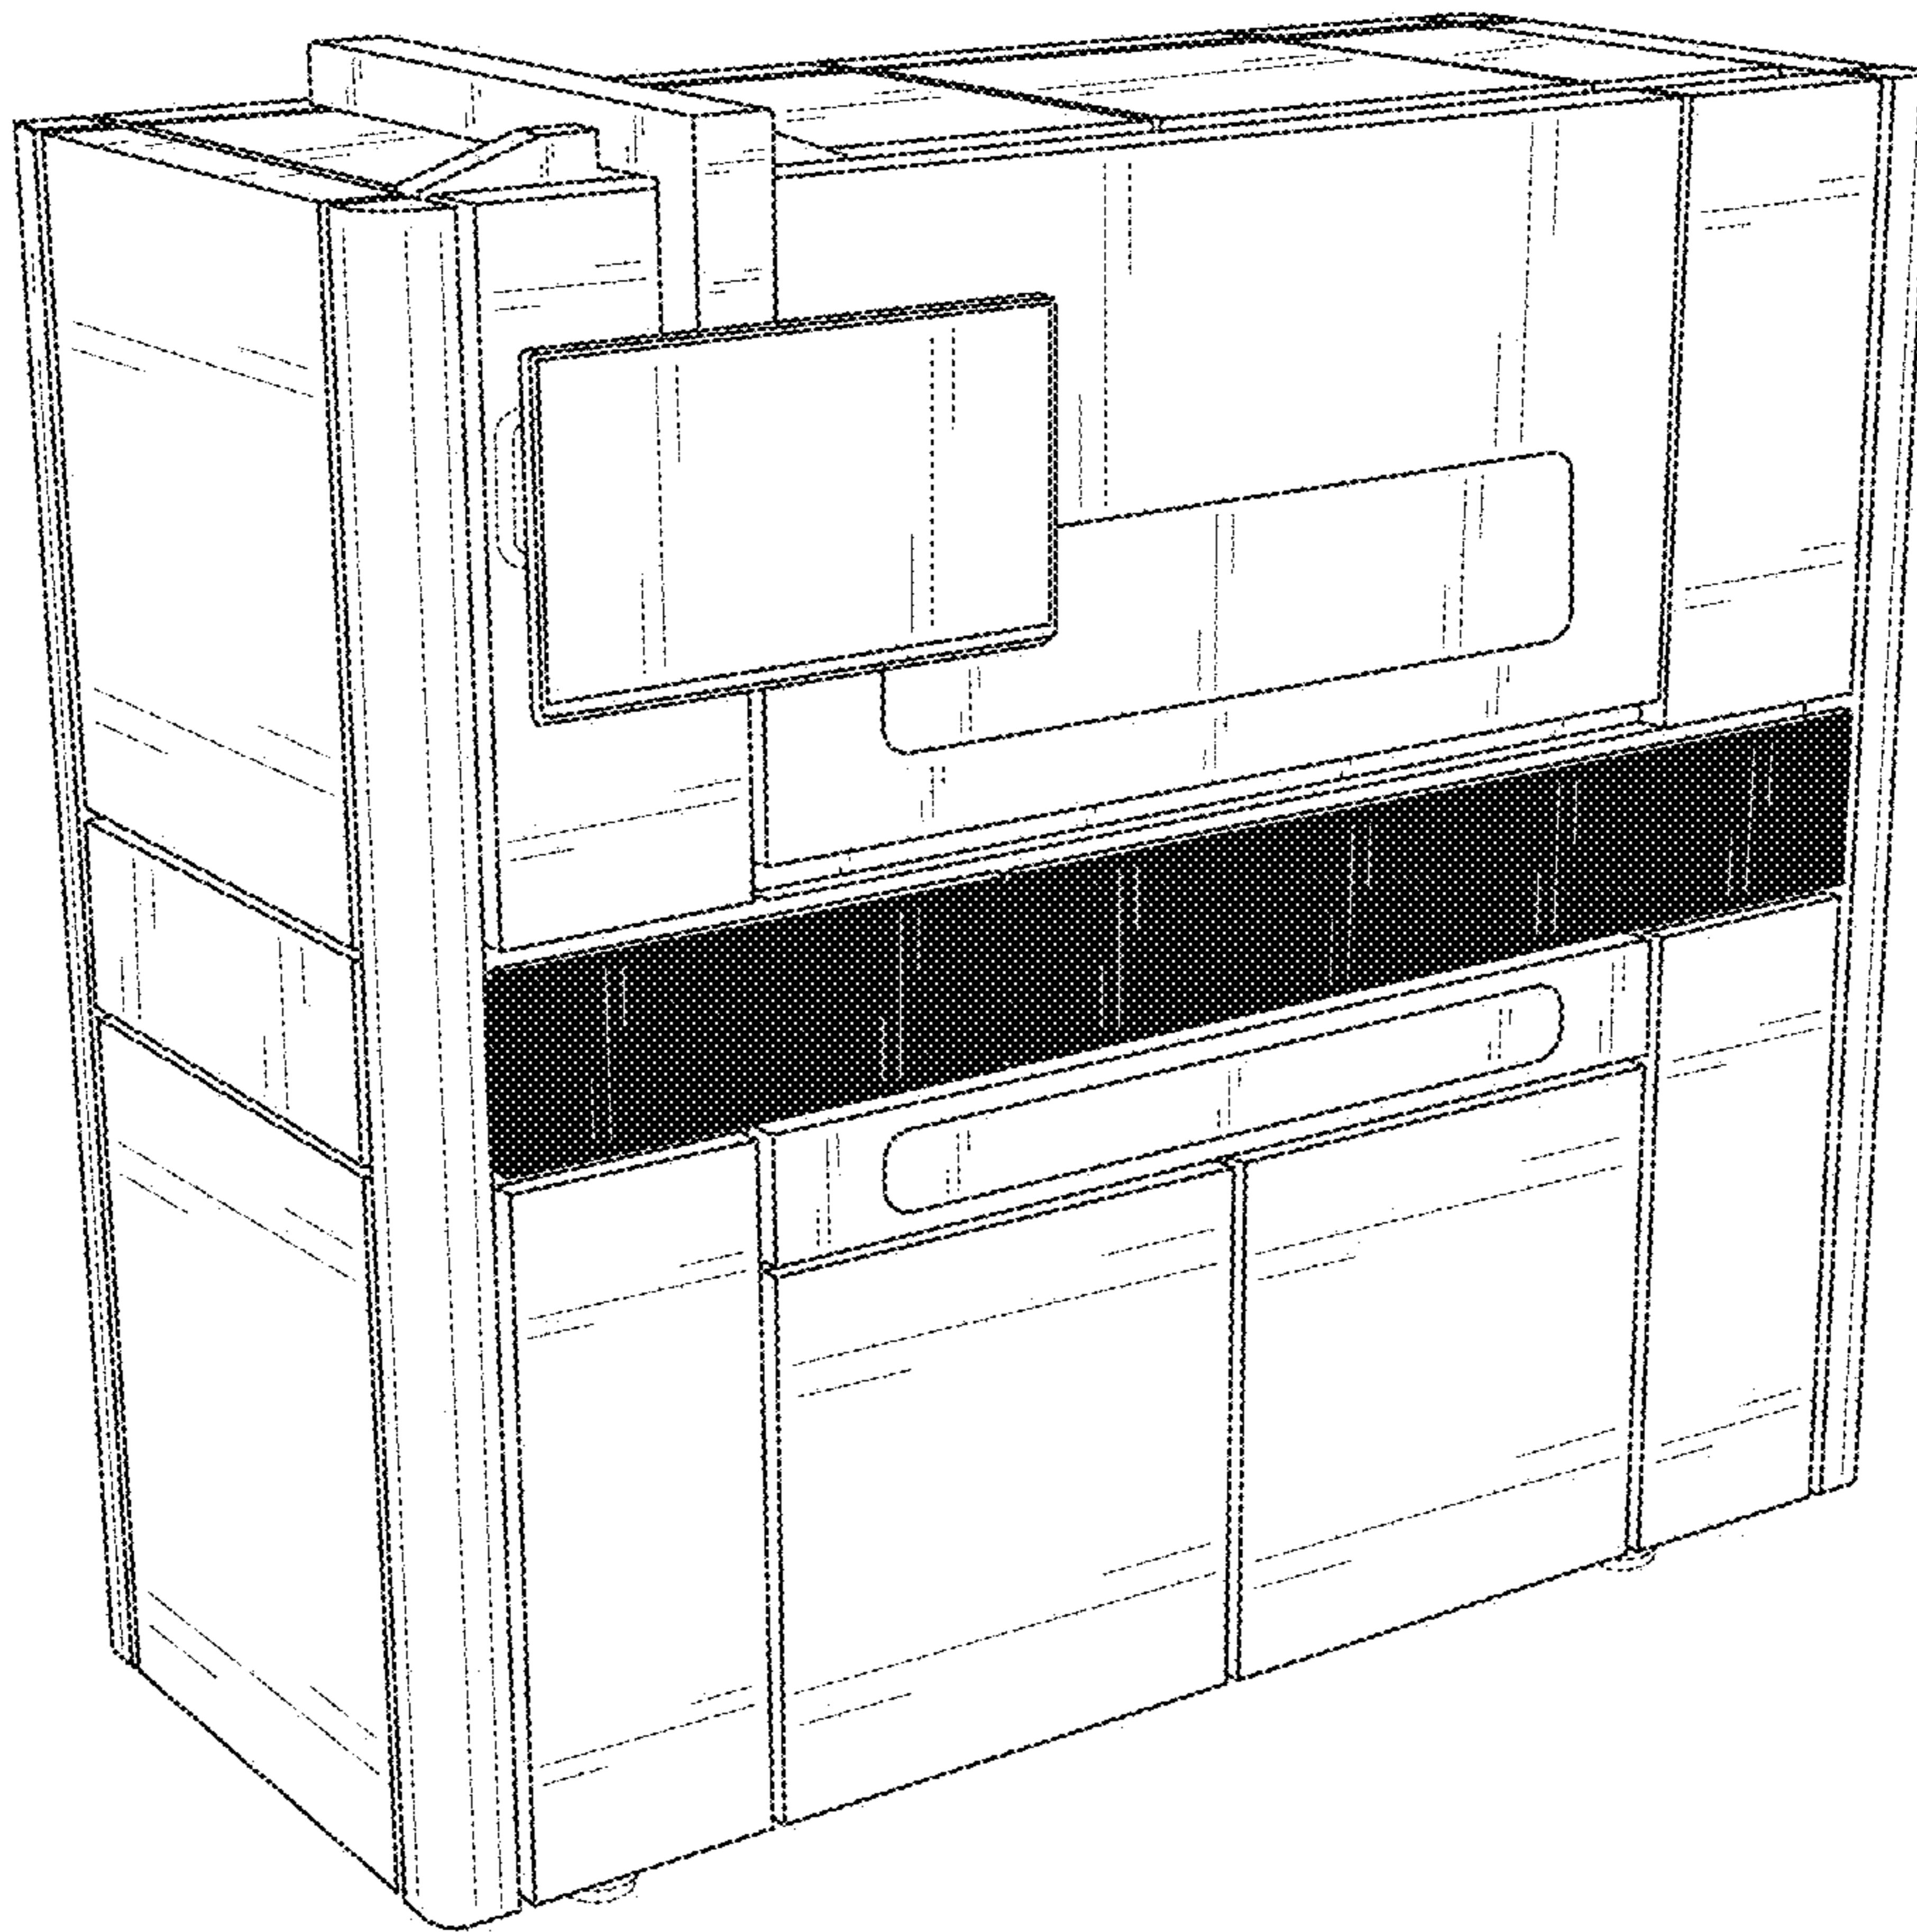


FIG. 10

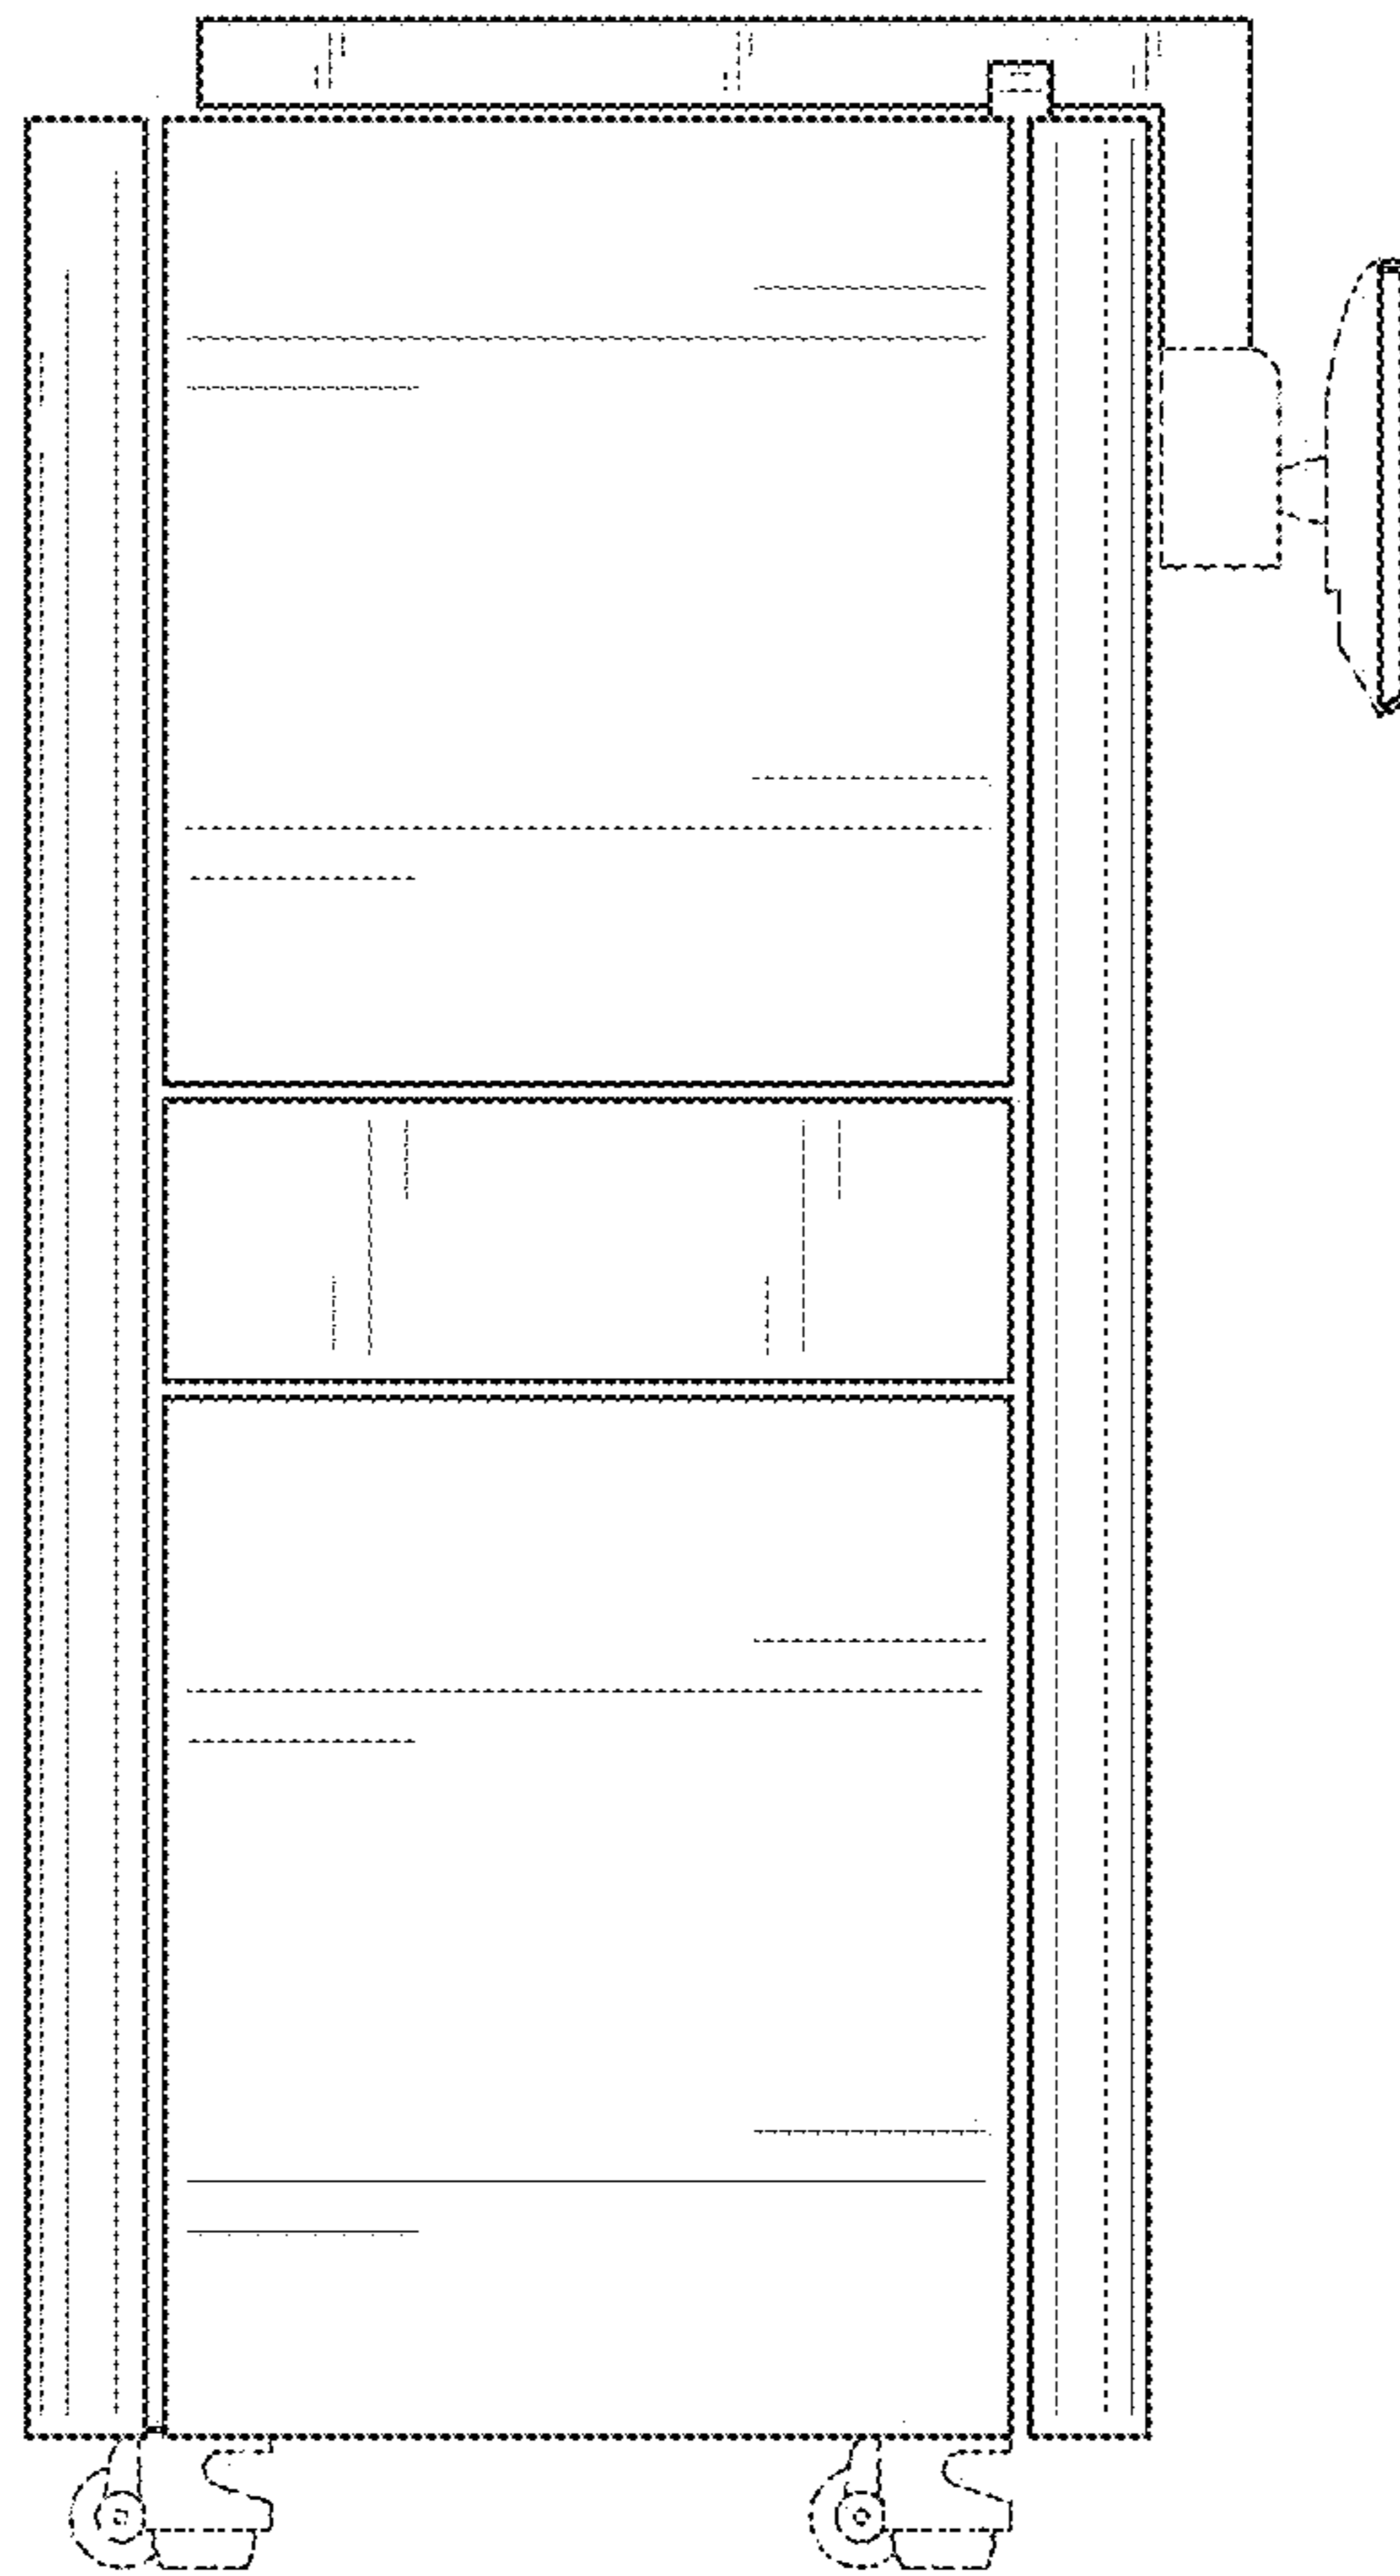


FIG. 11

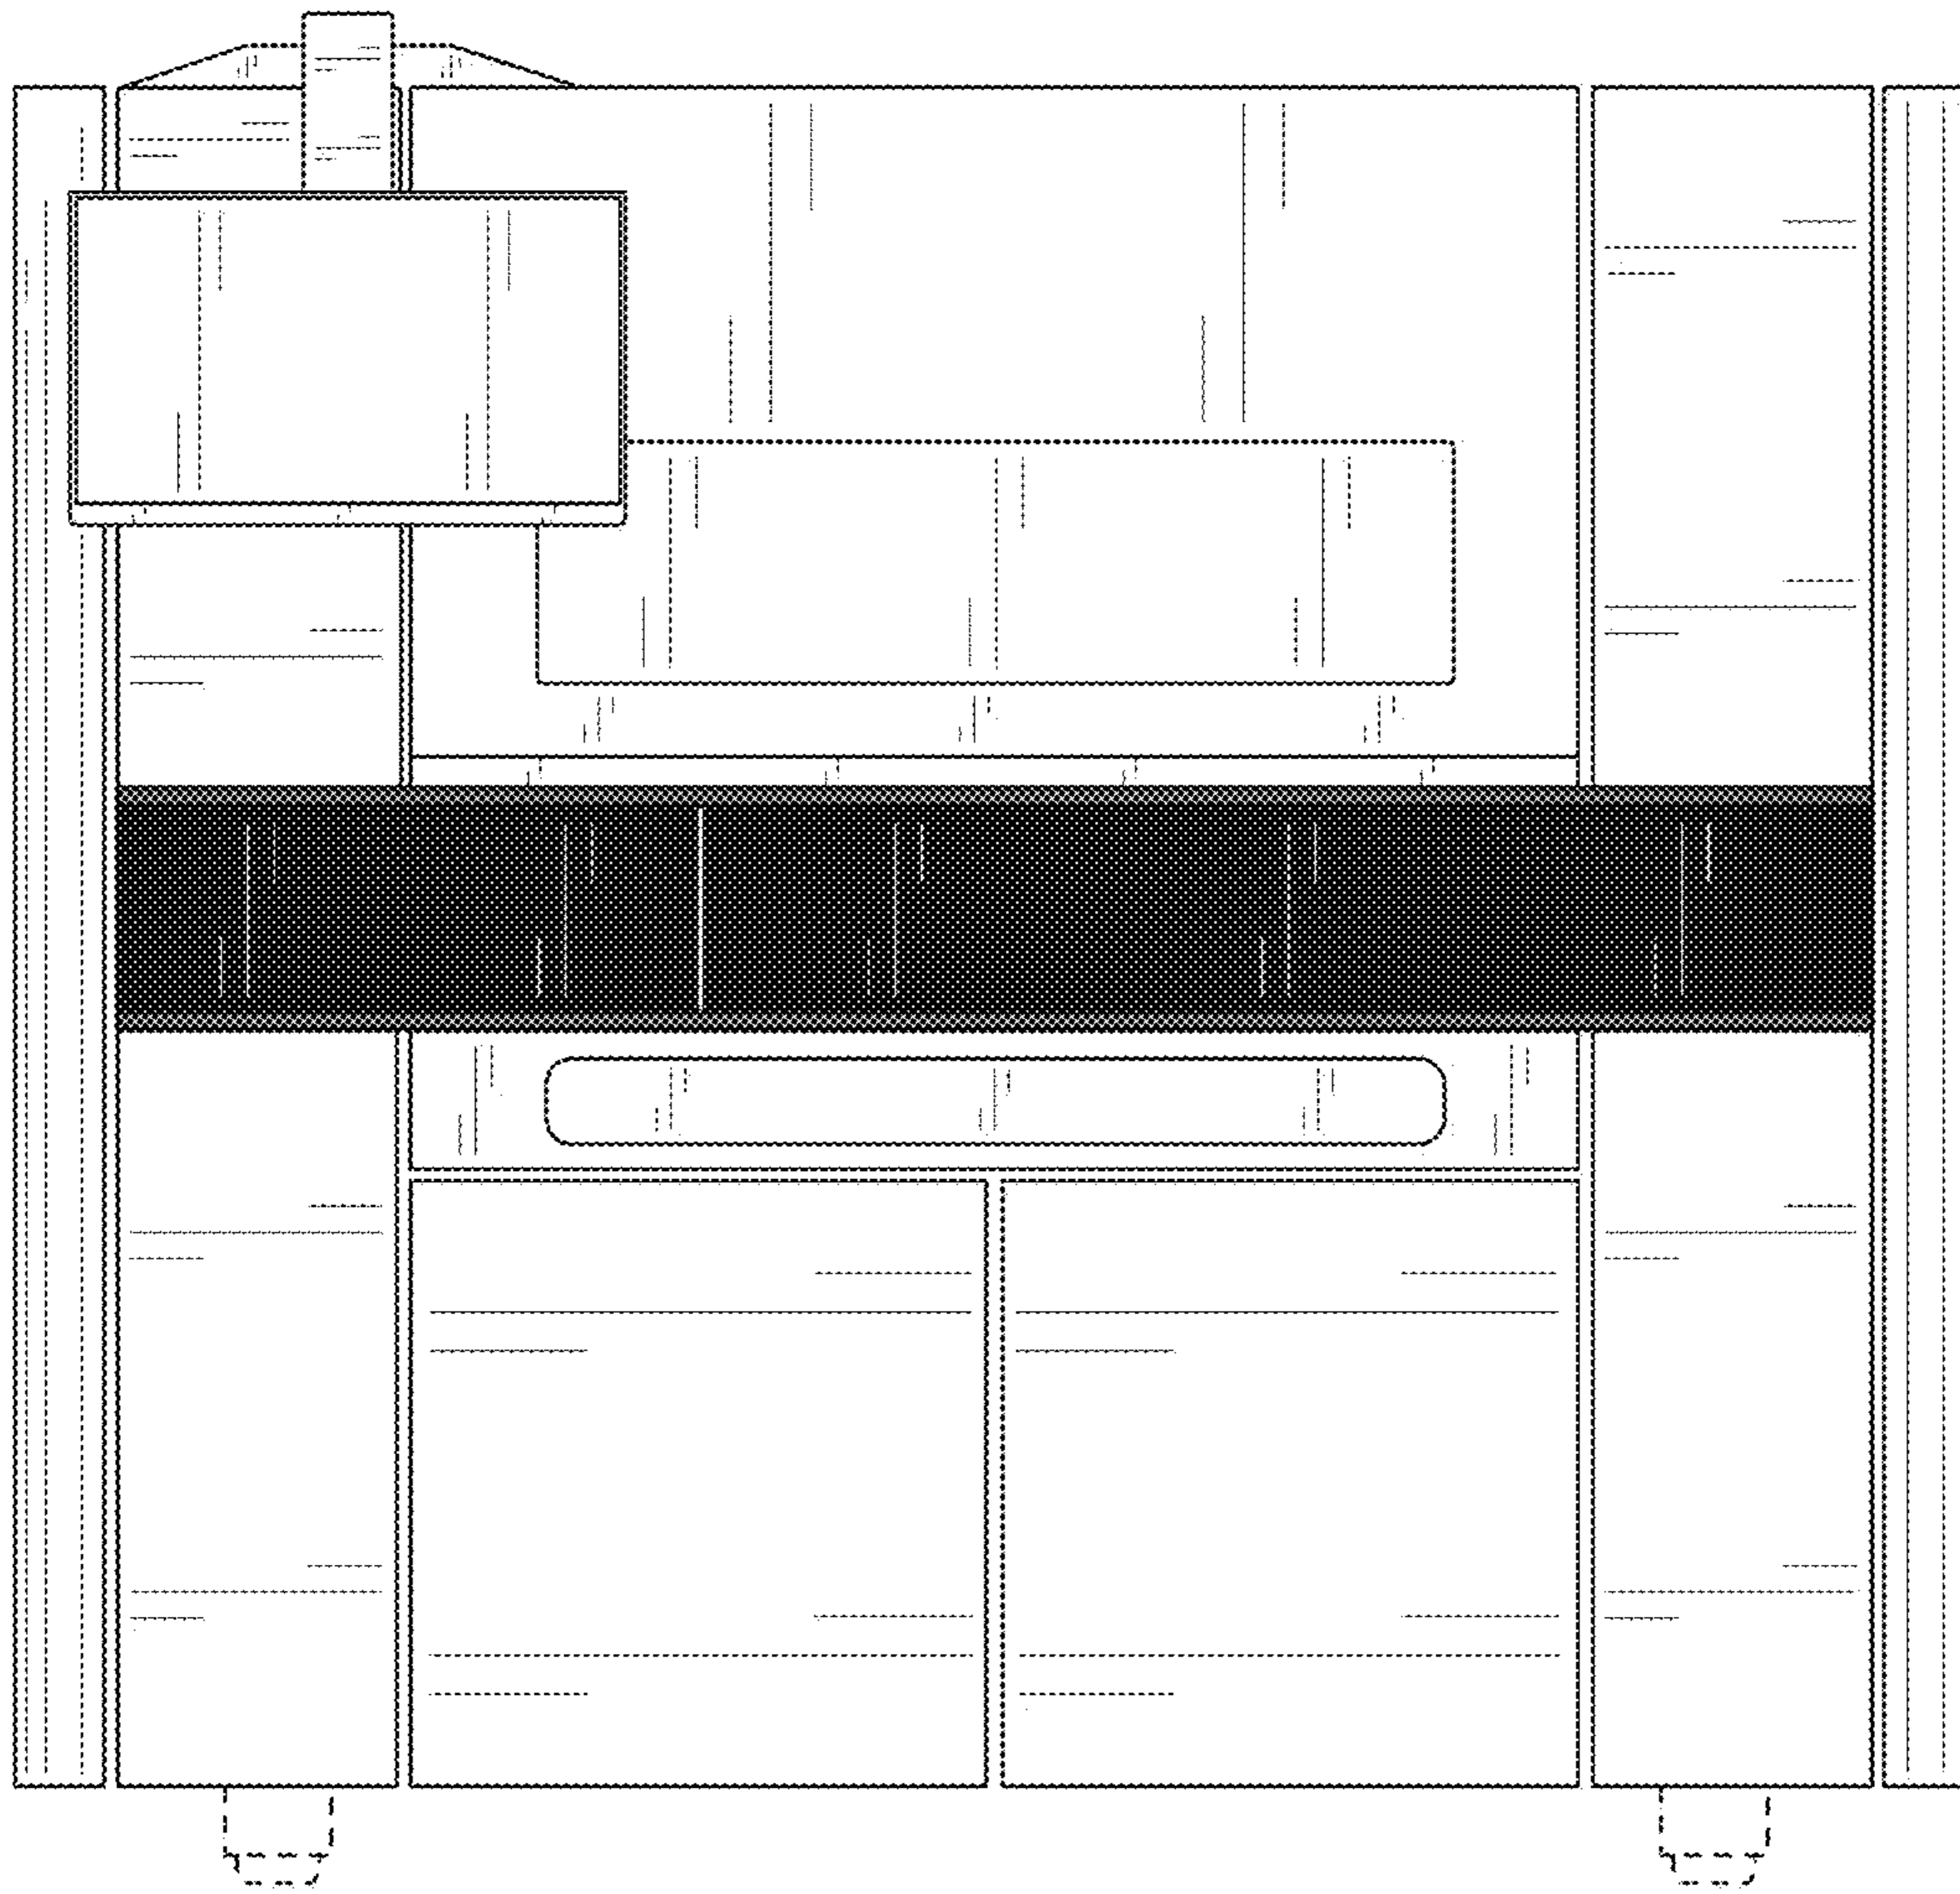


Fig. 12

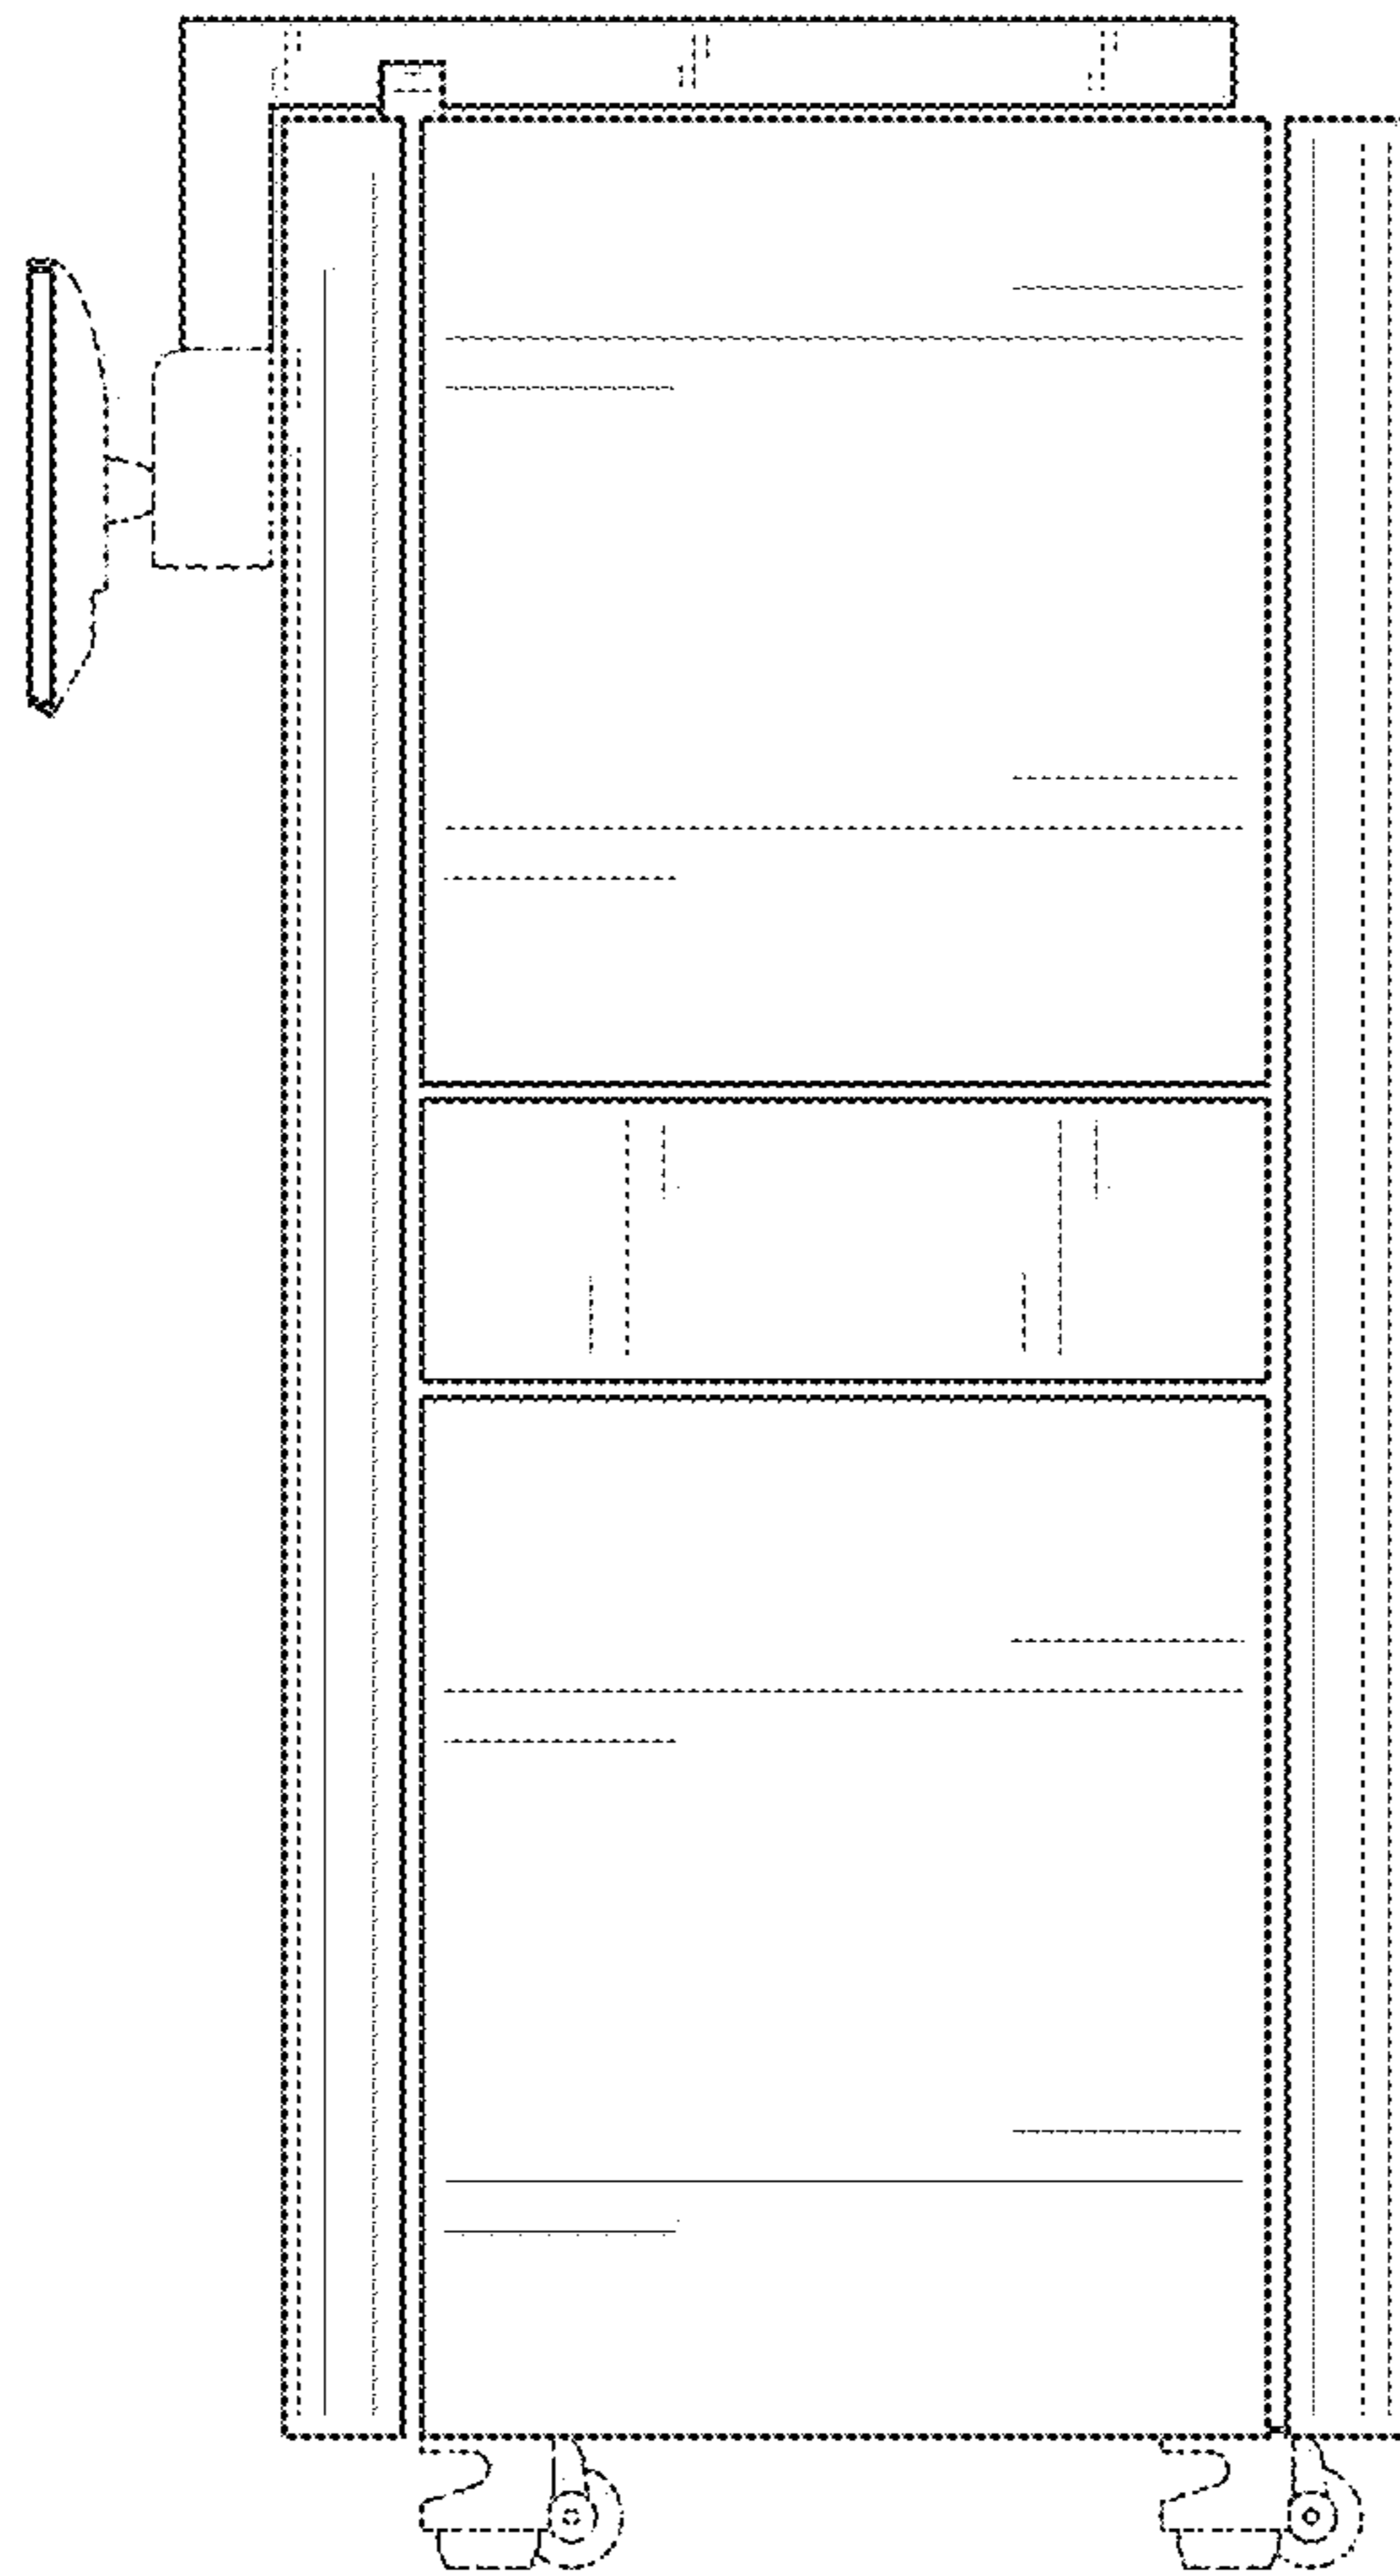


FIG. 13

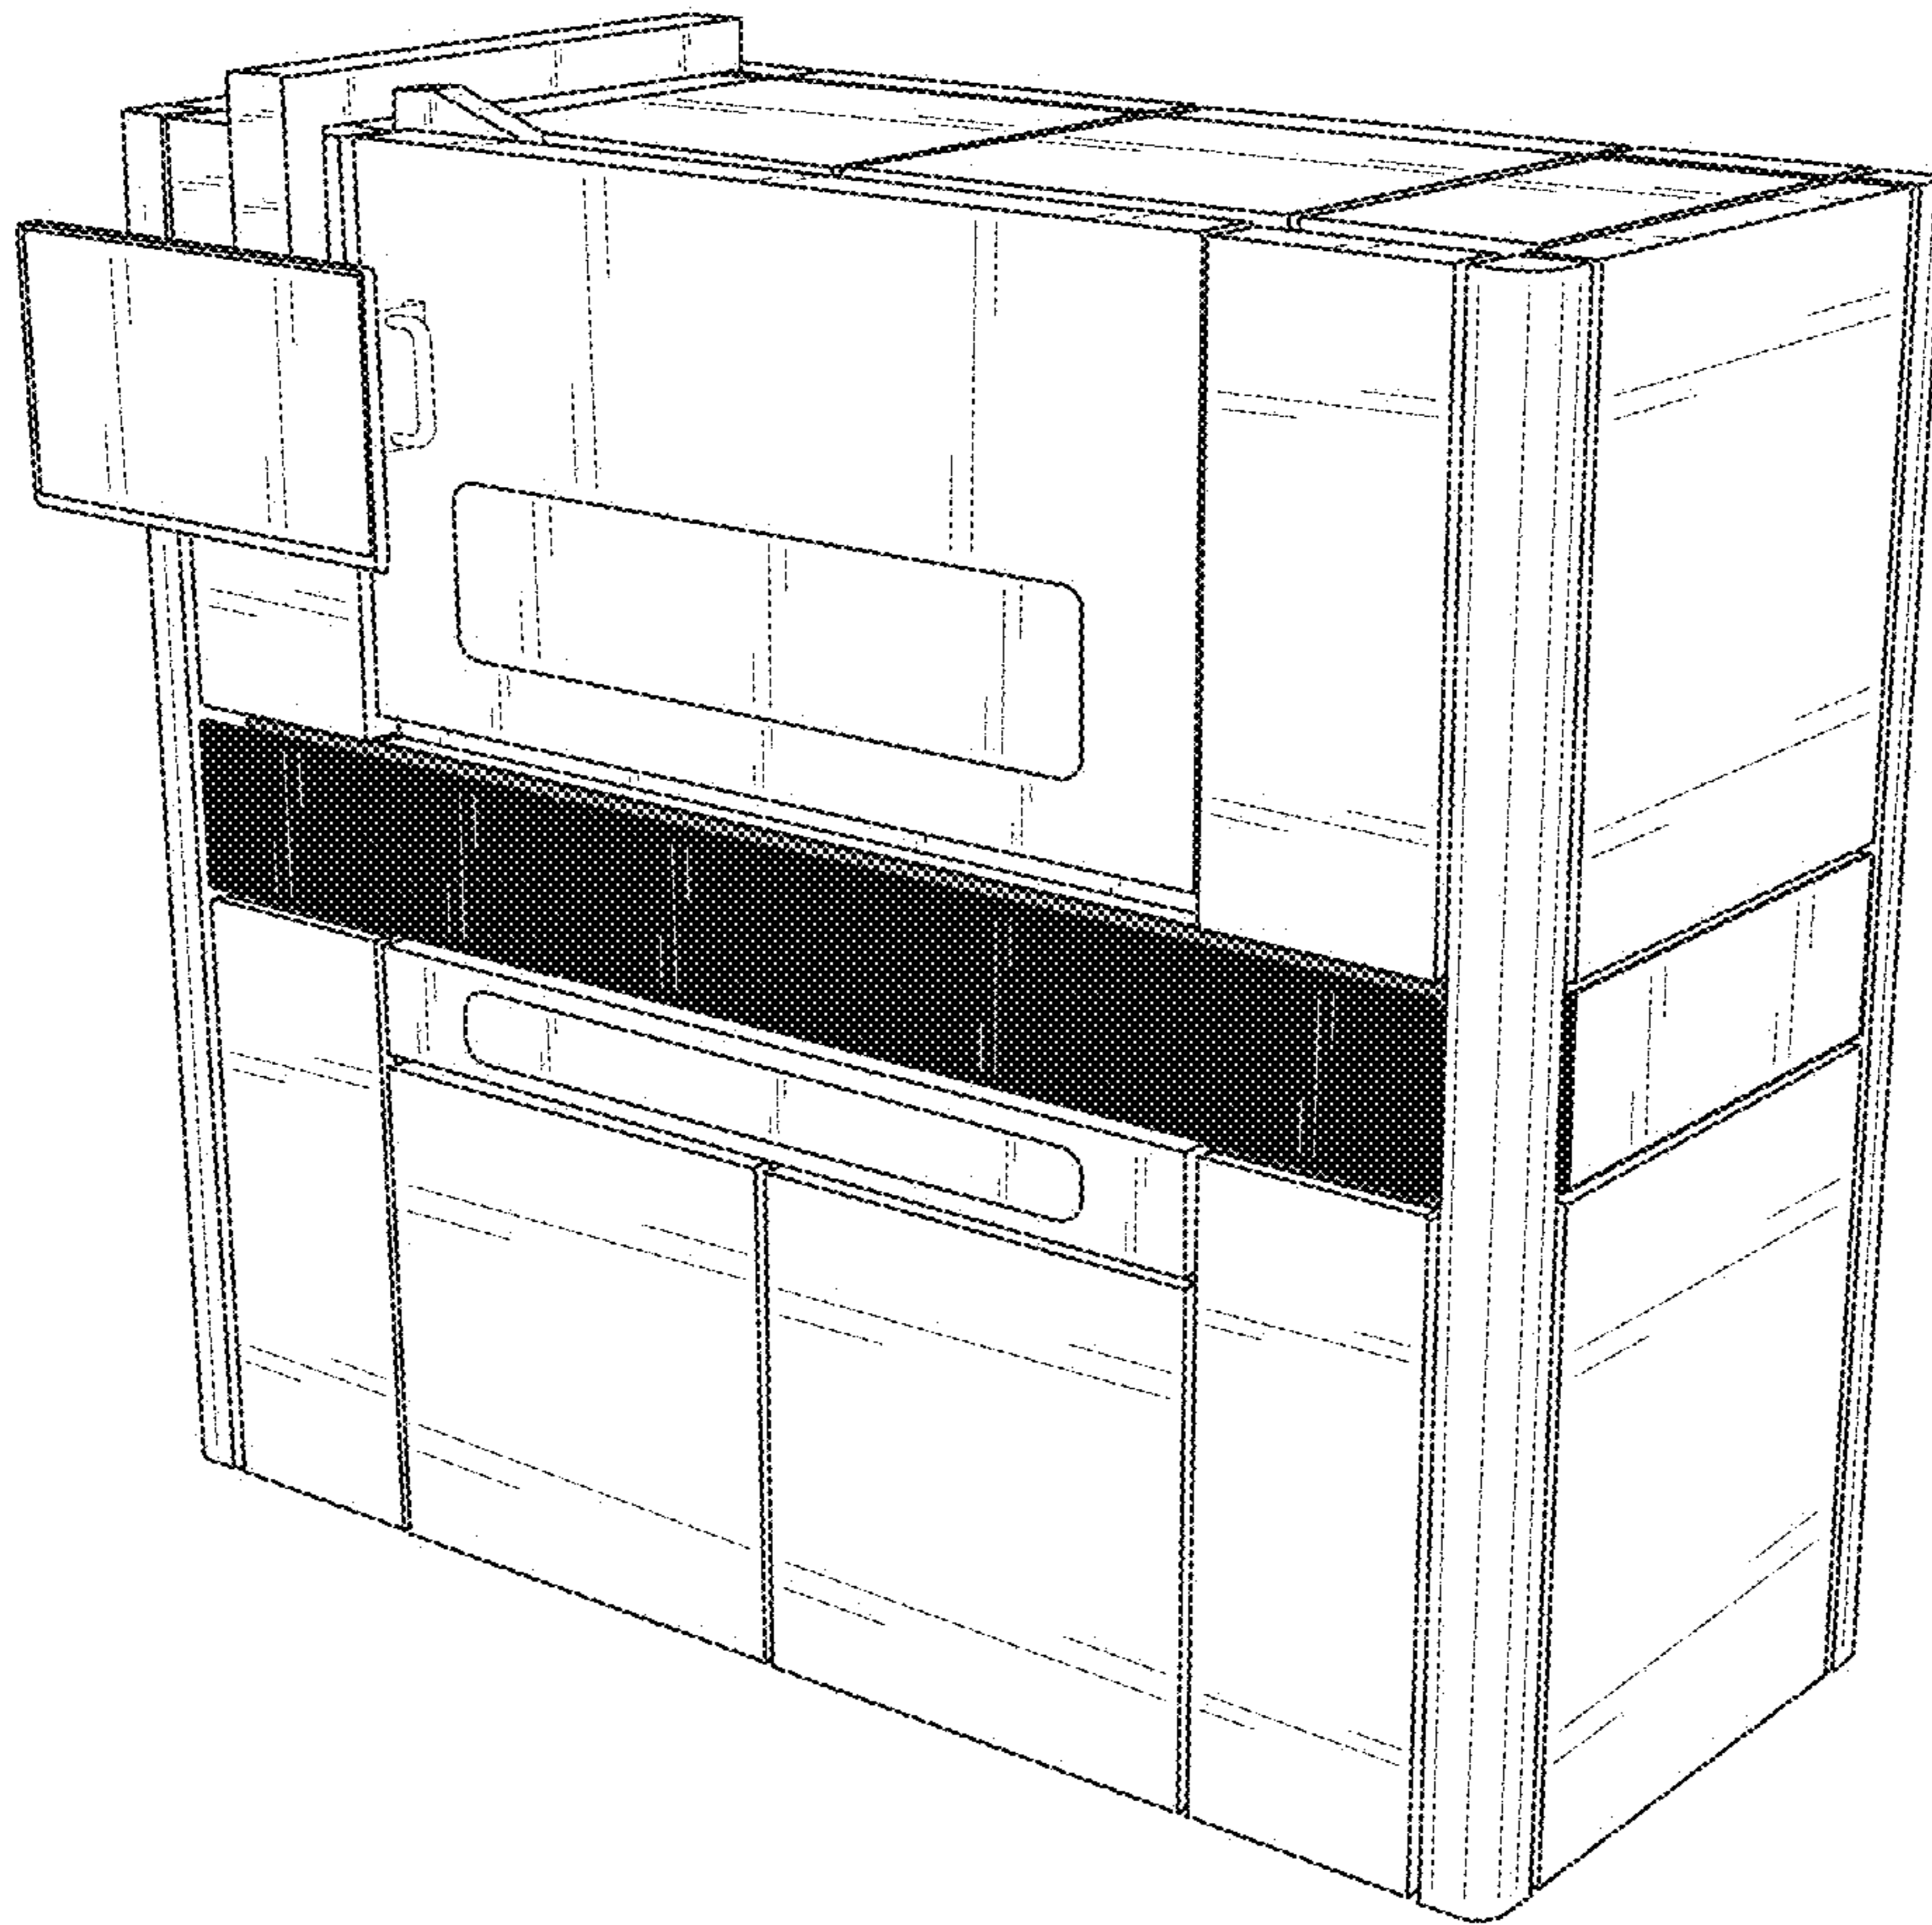


FIG. 14



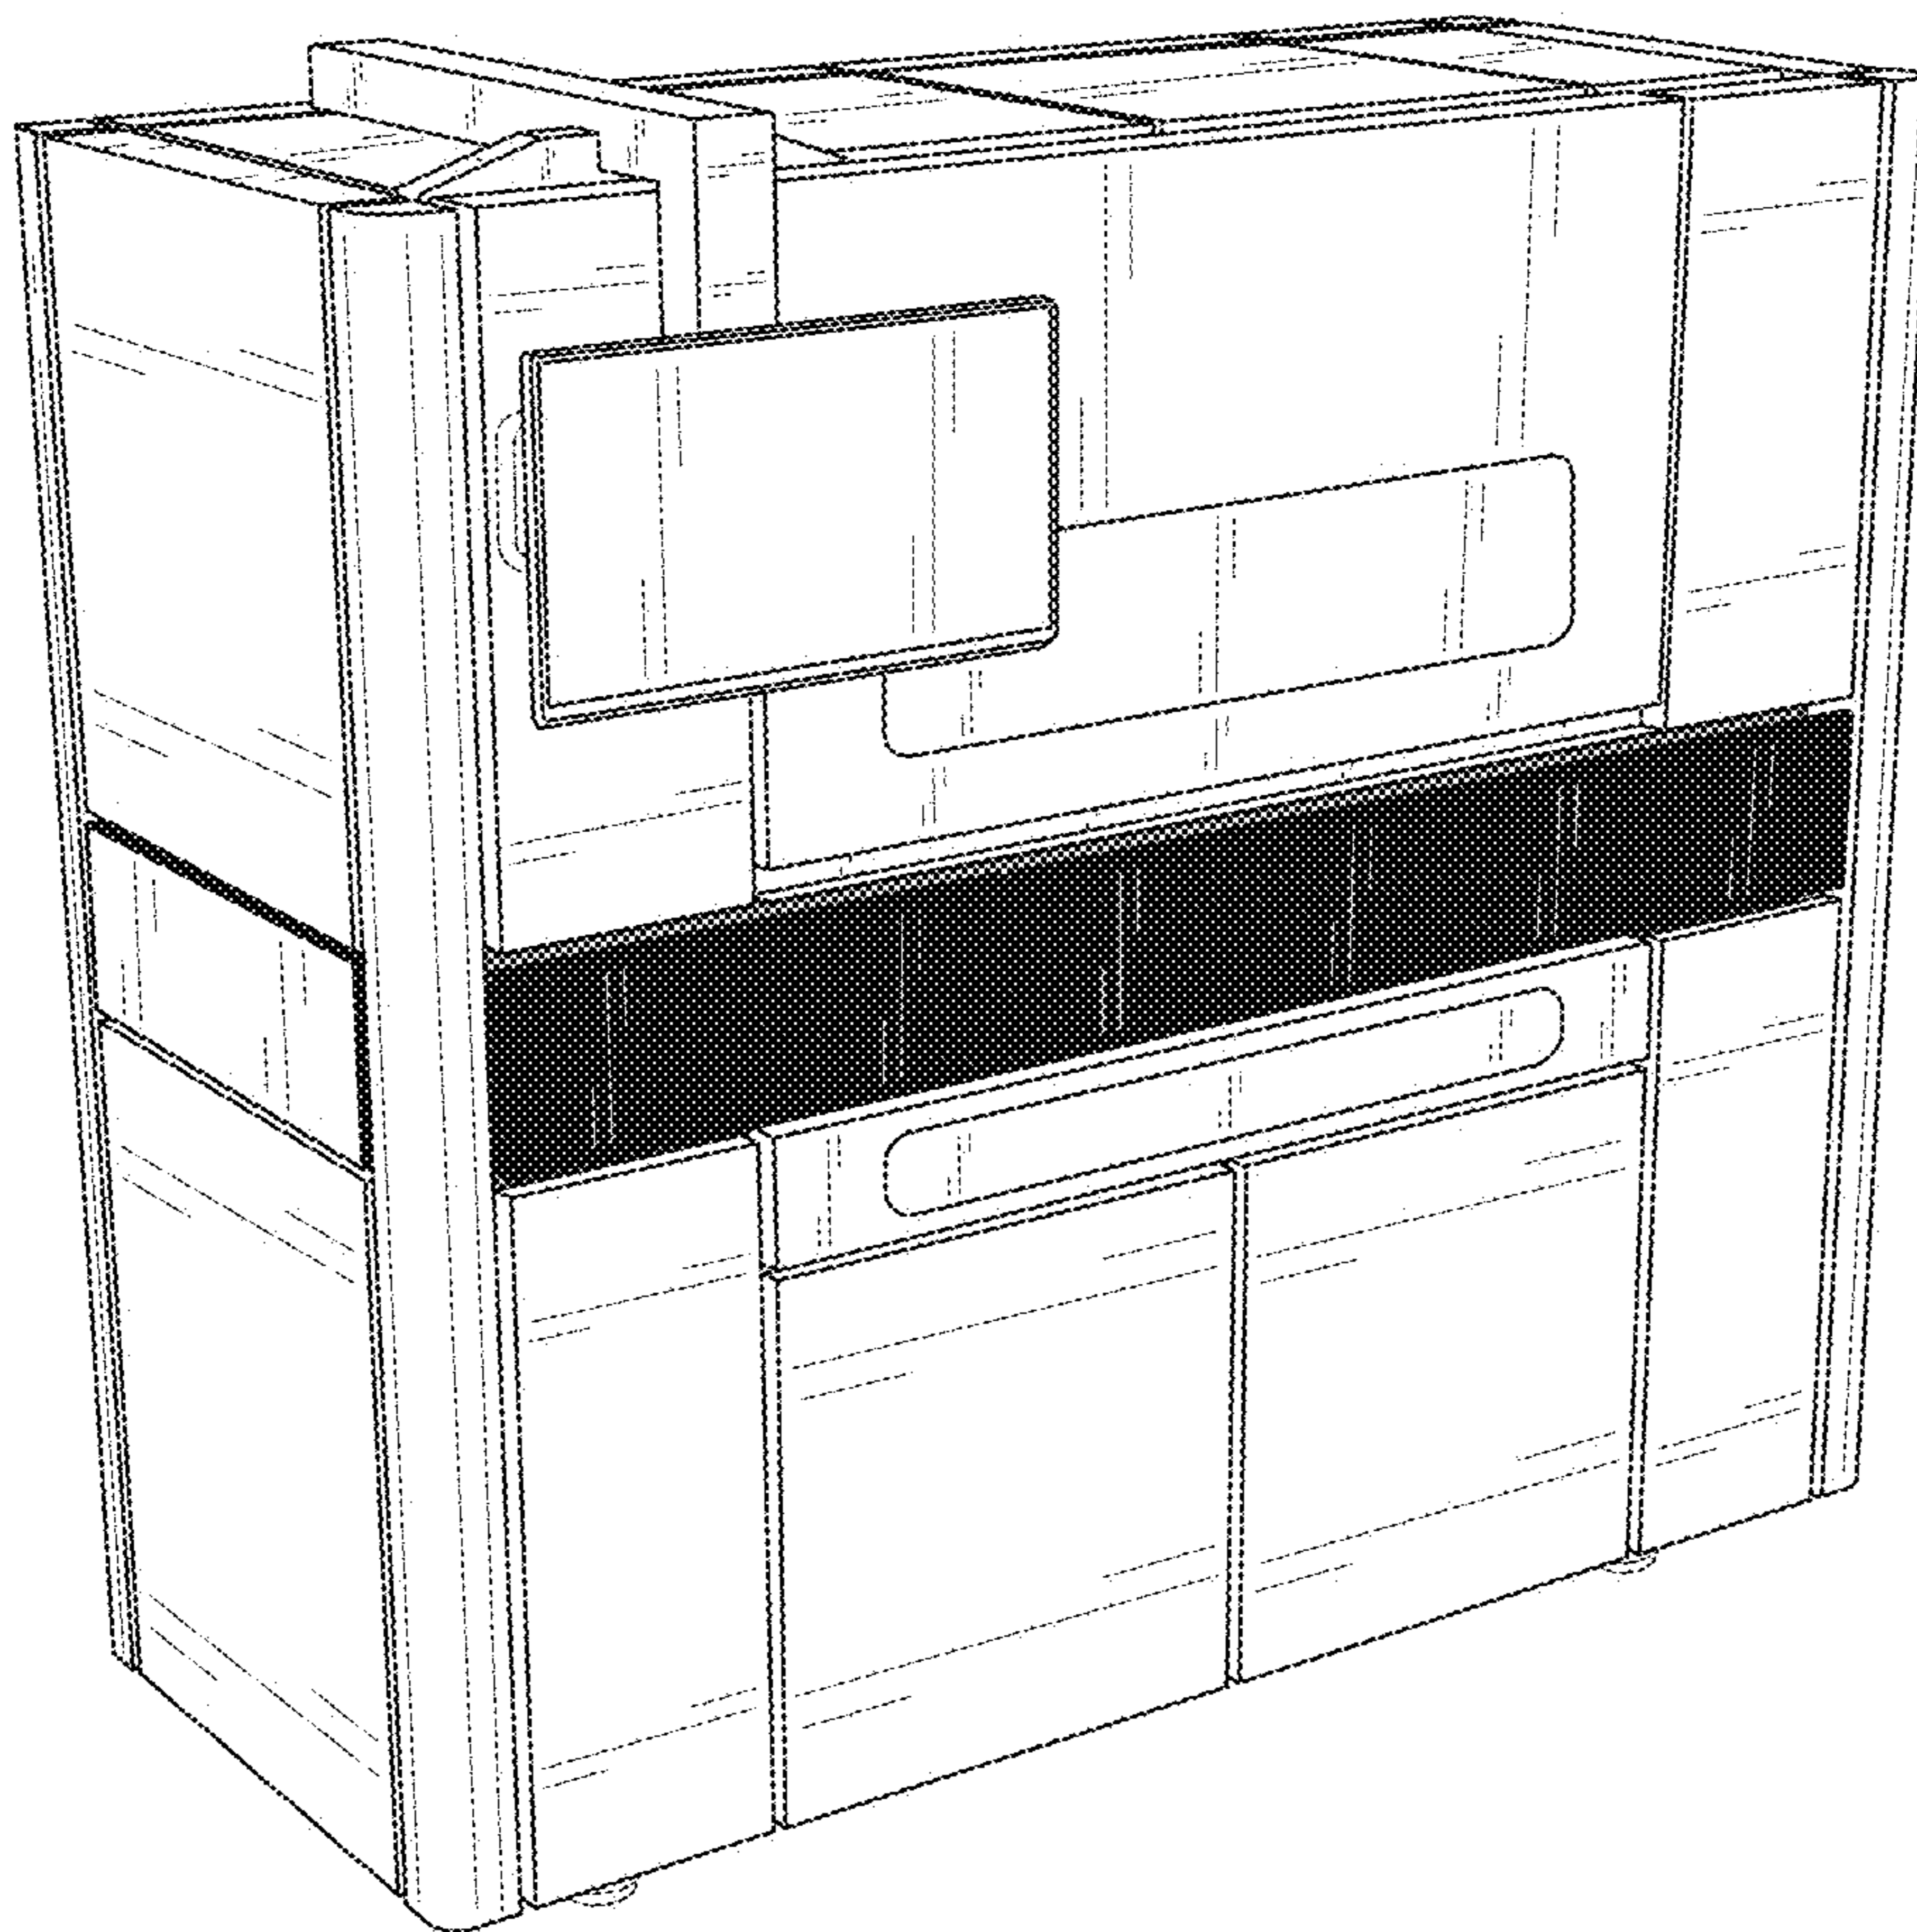


FIG. 15

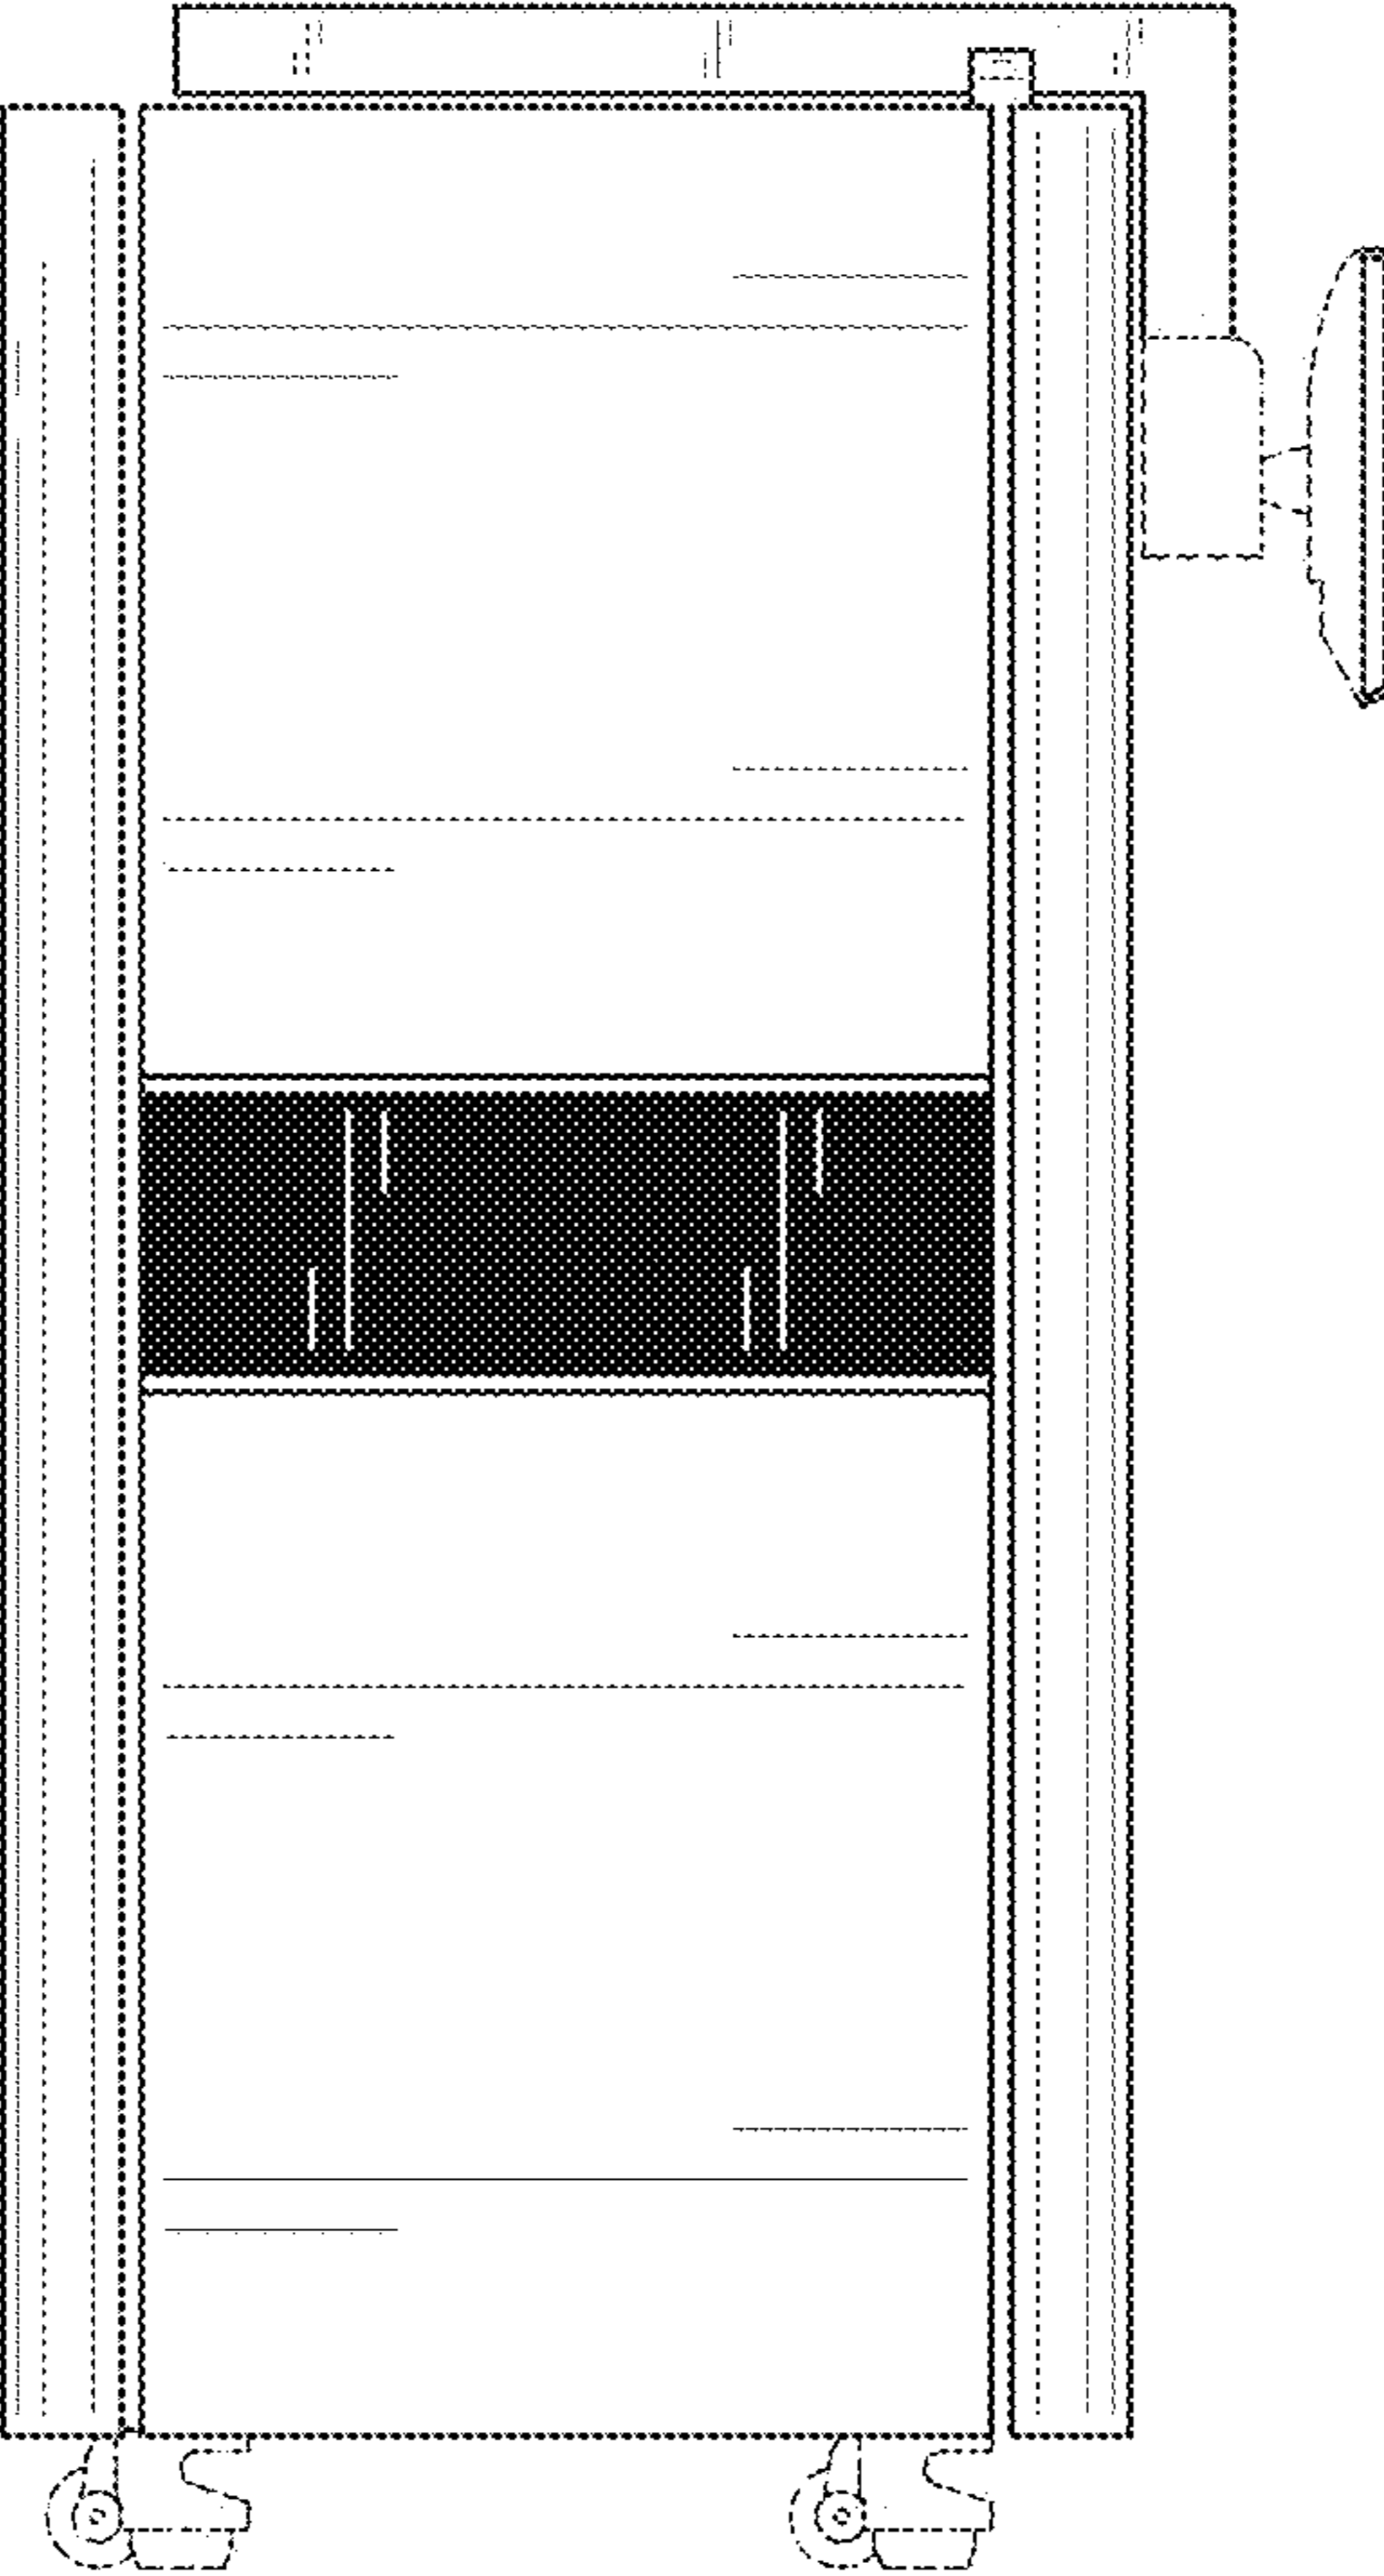


FIG. 16

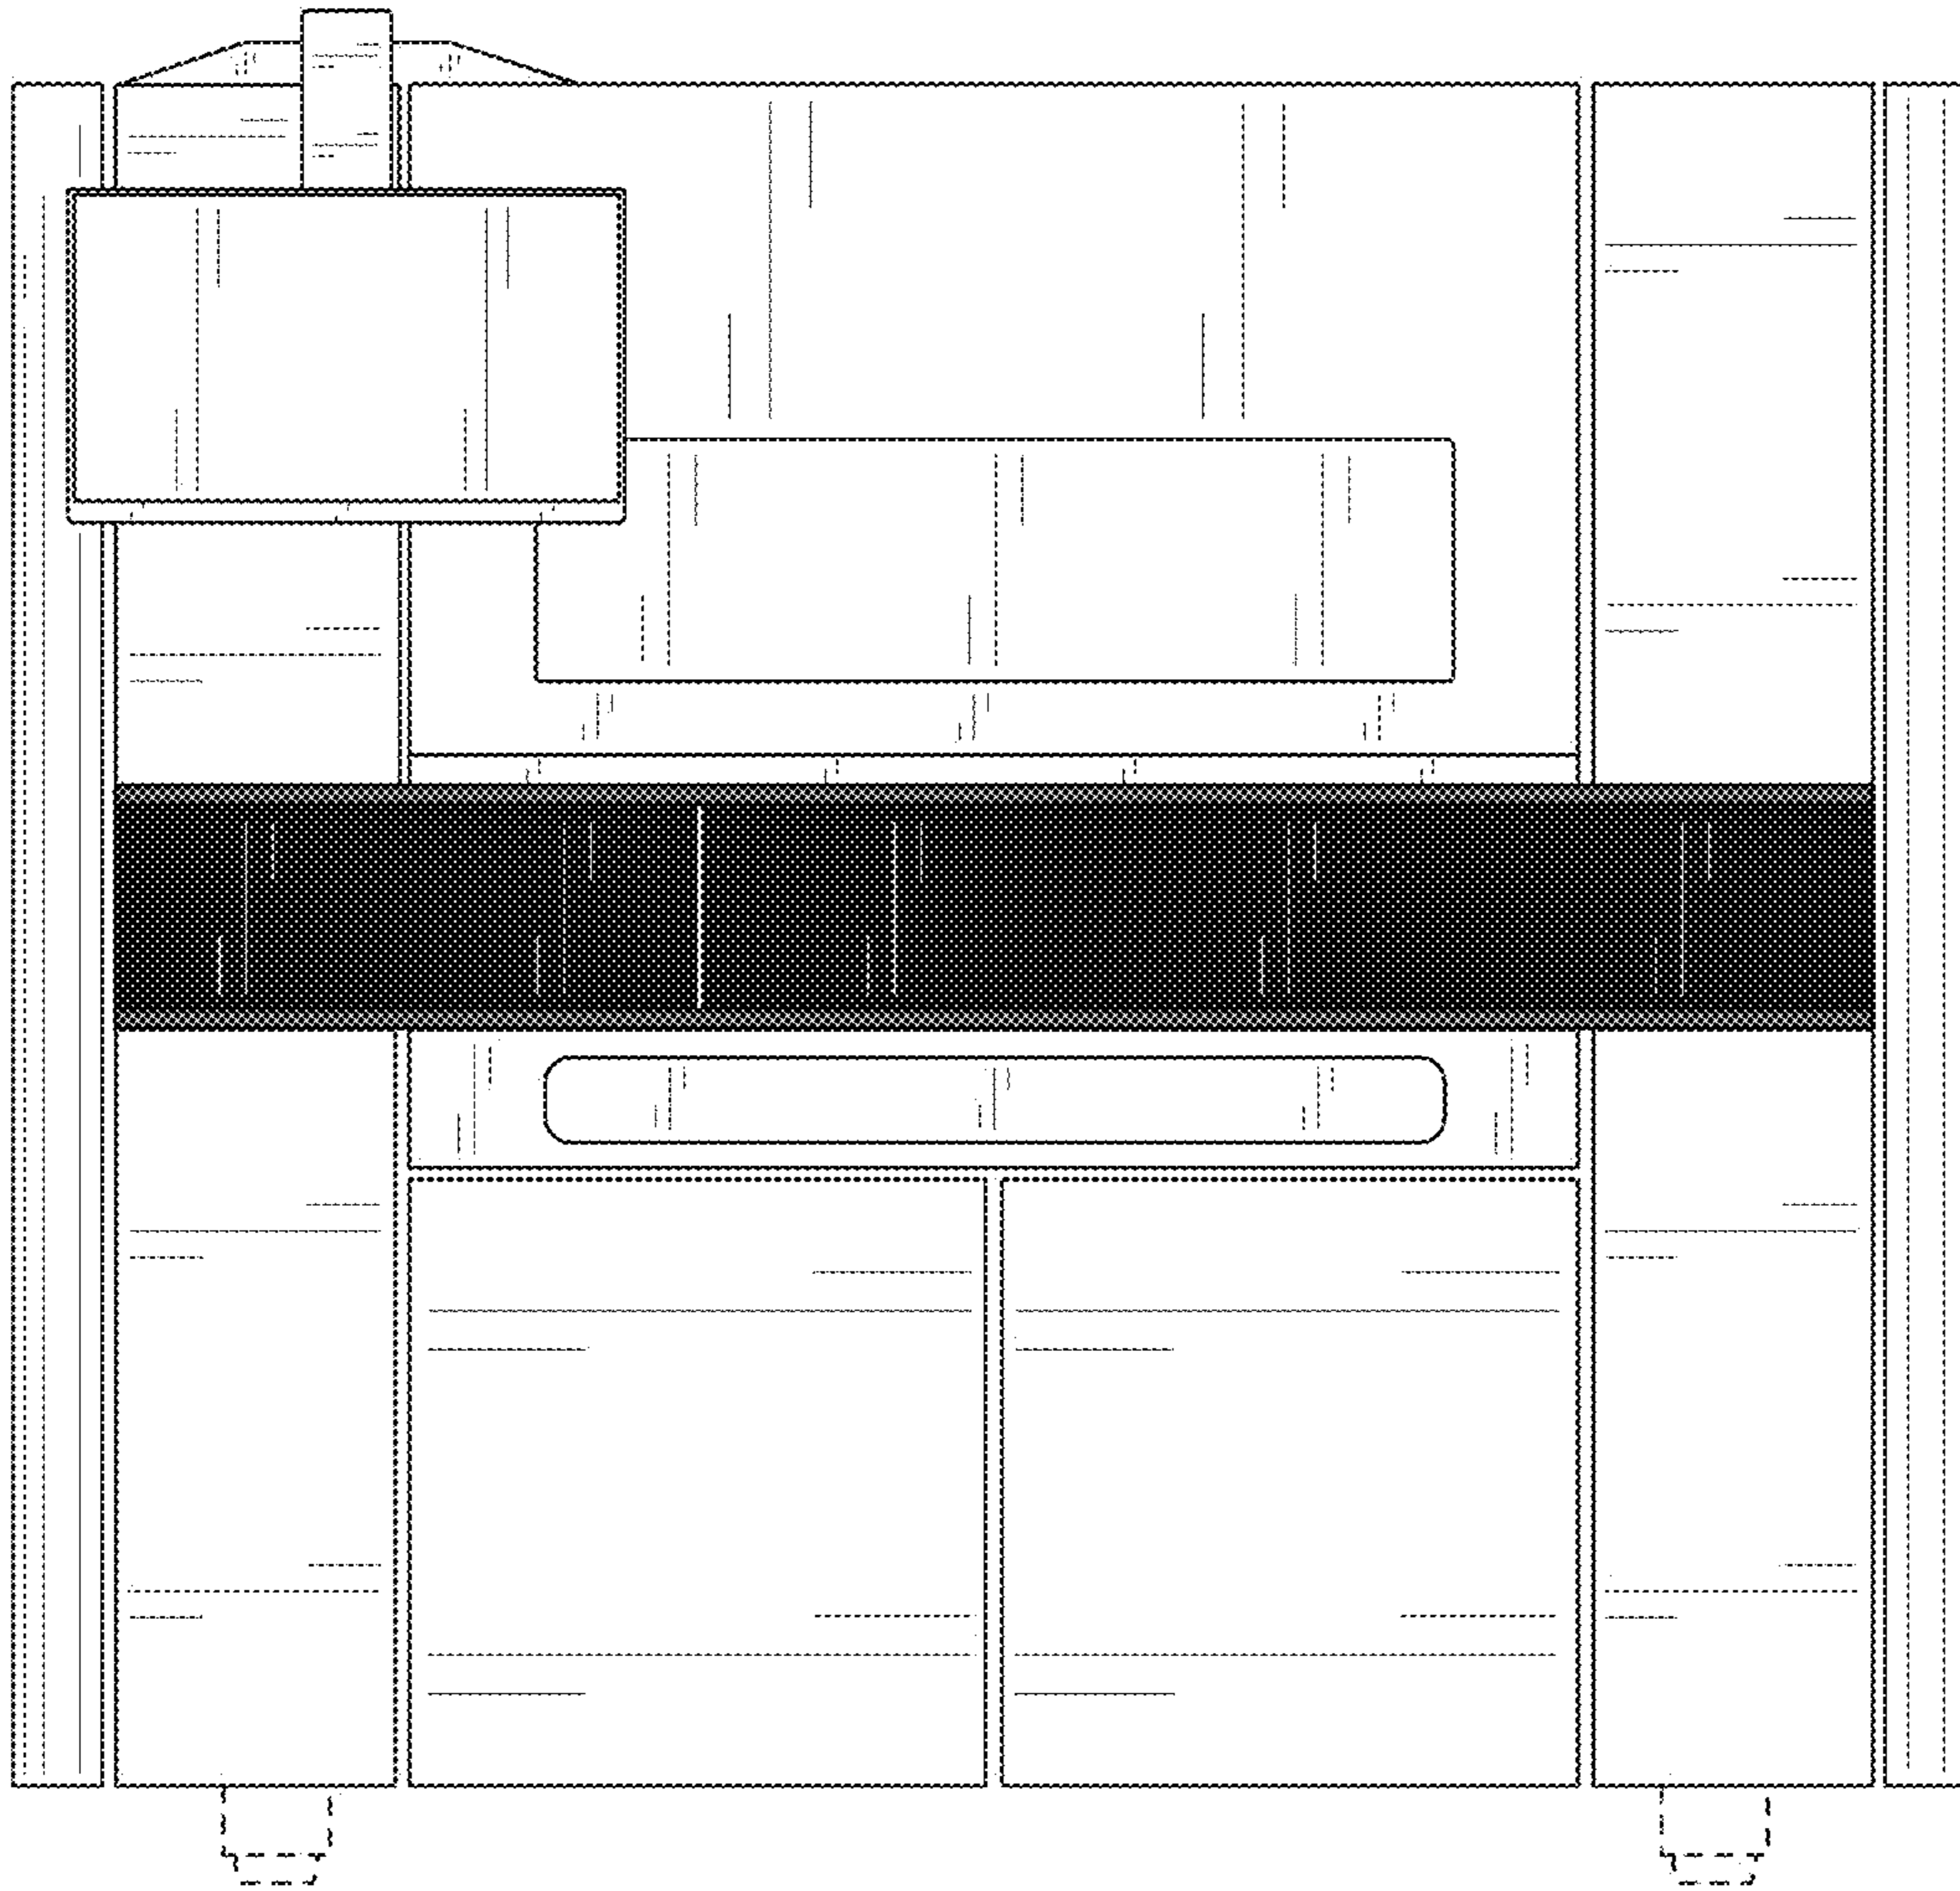


Fig. 17

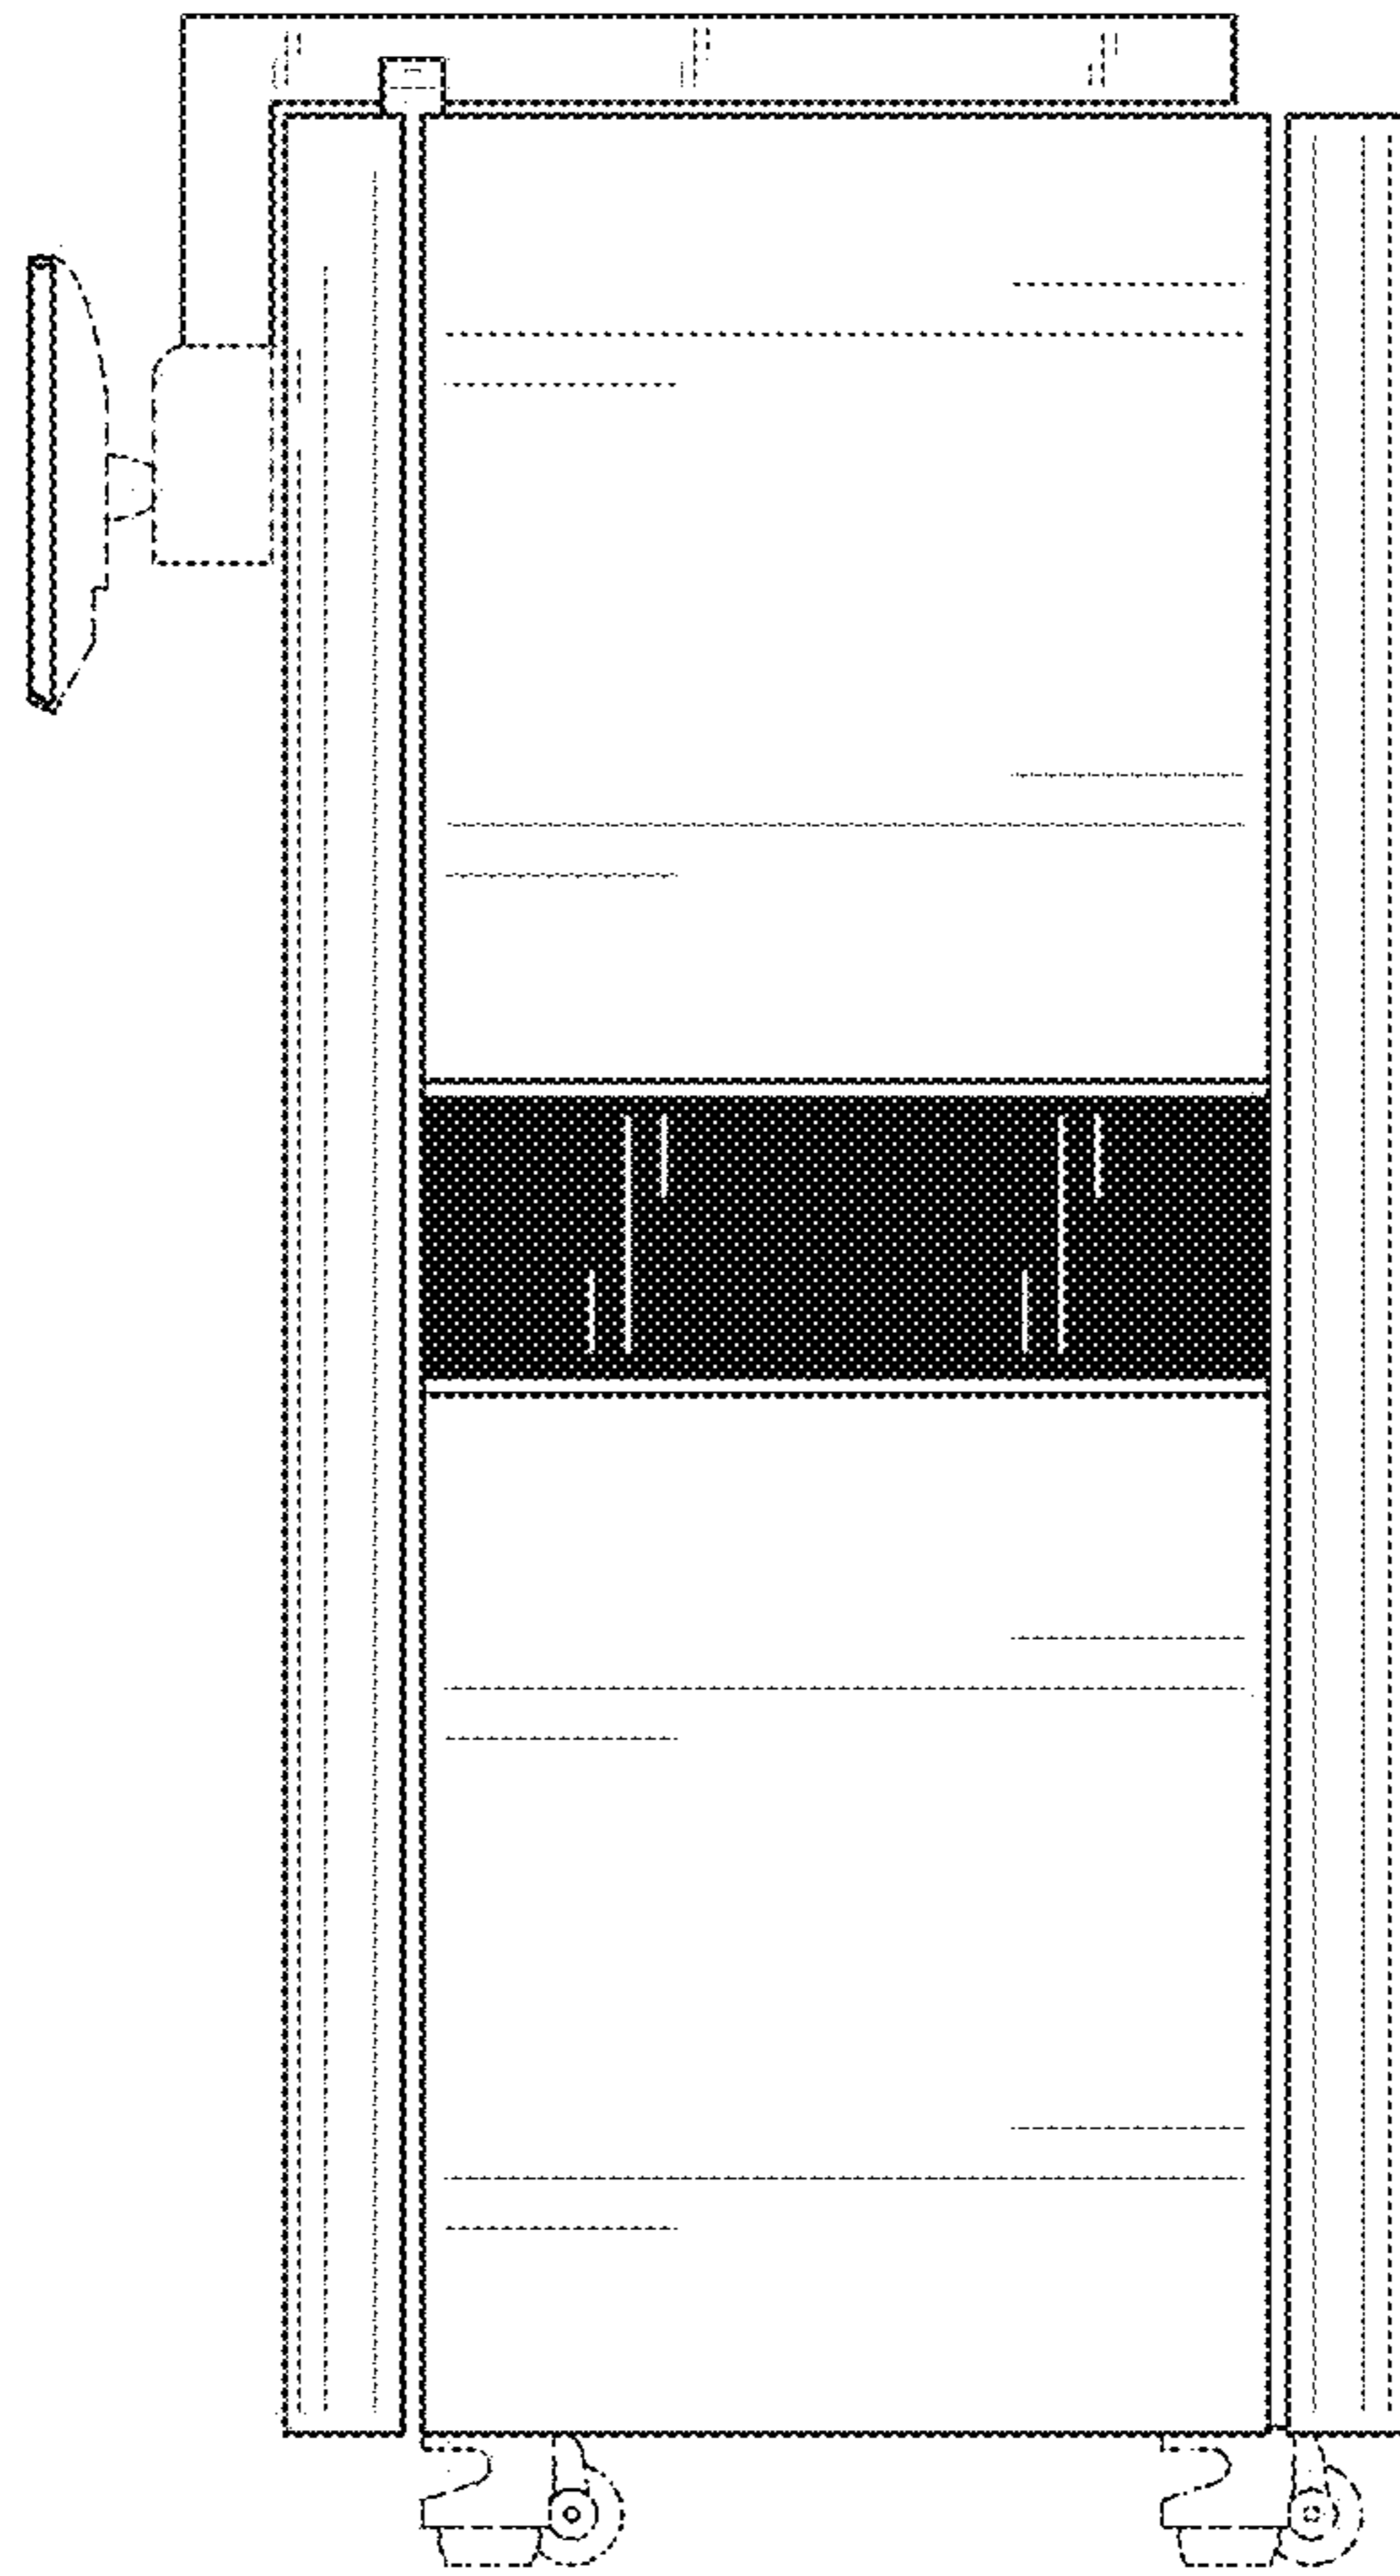


FIG. 18

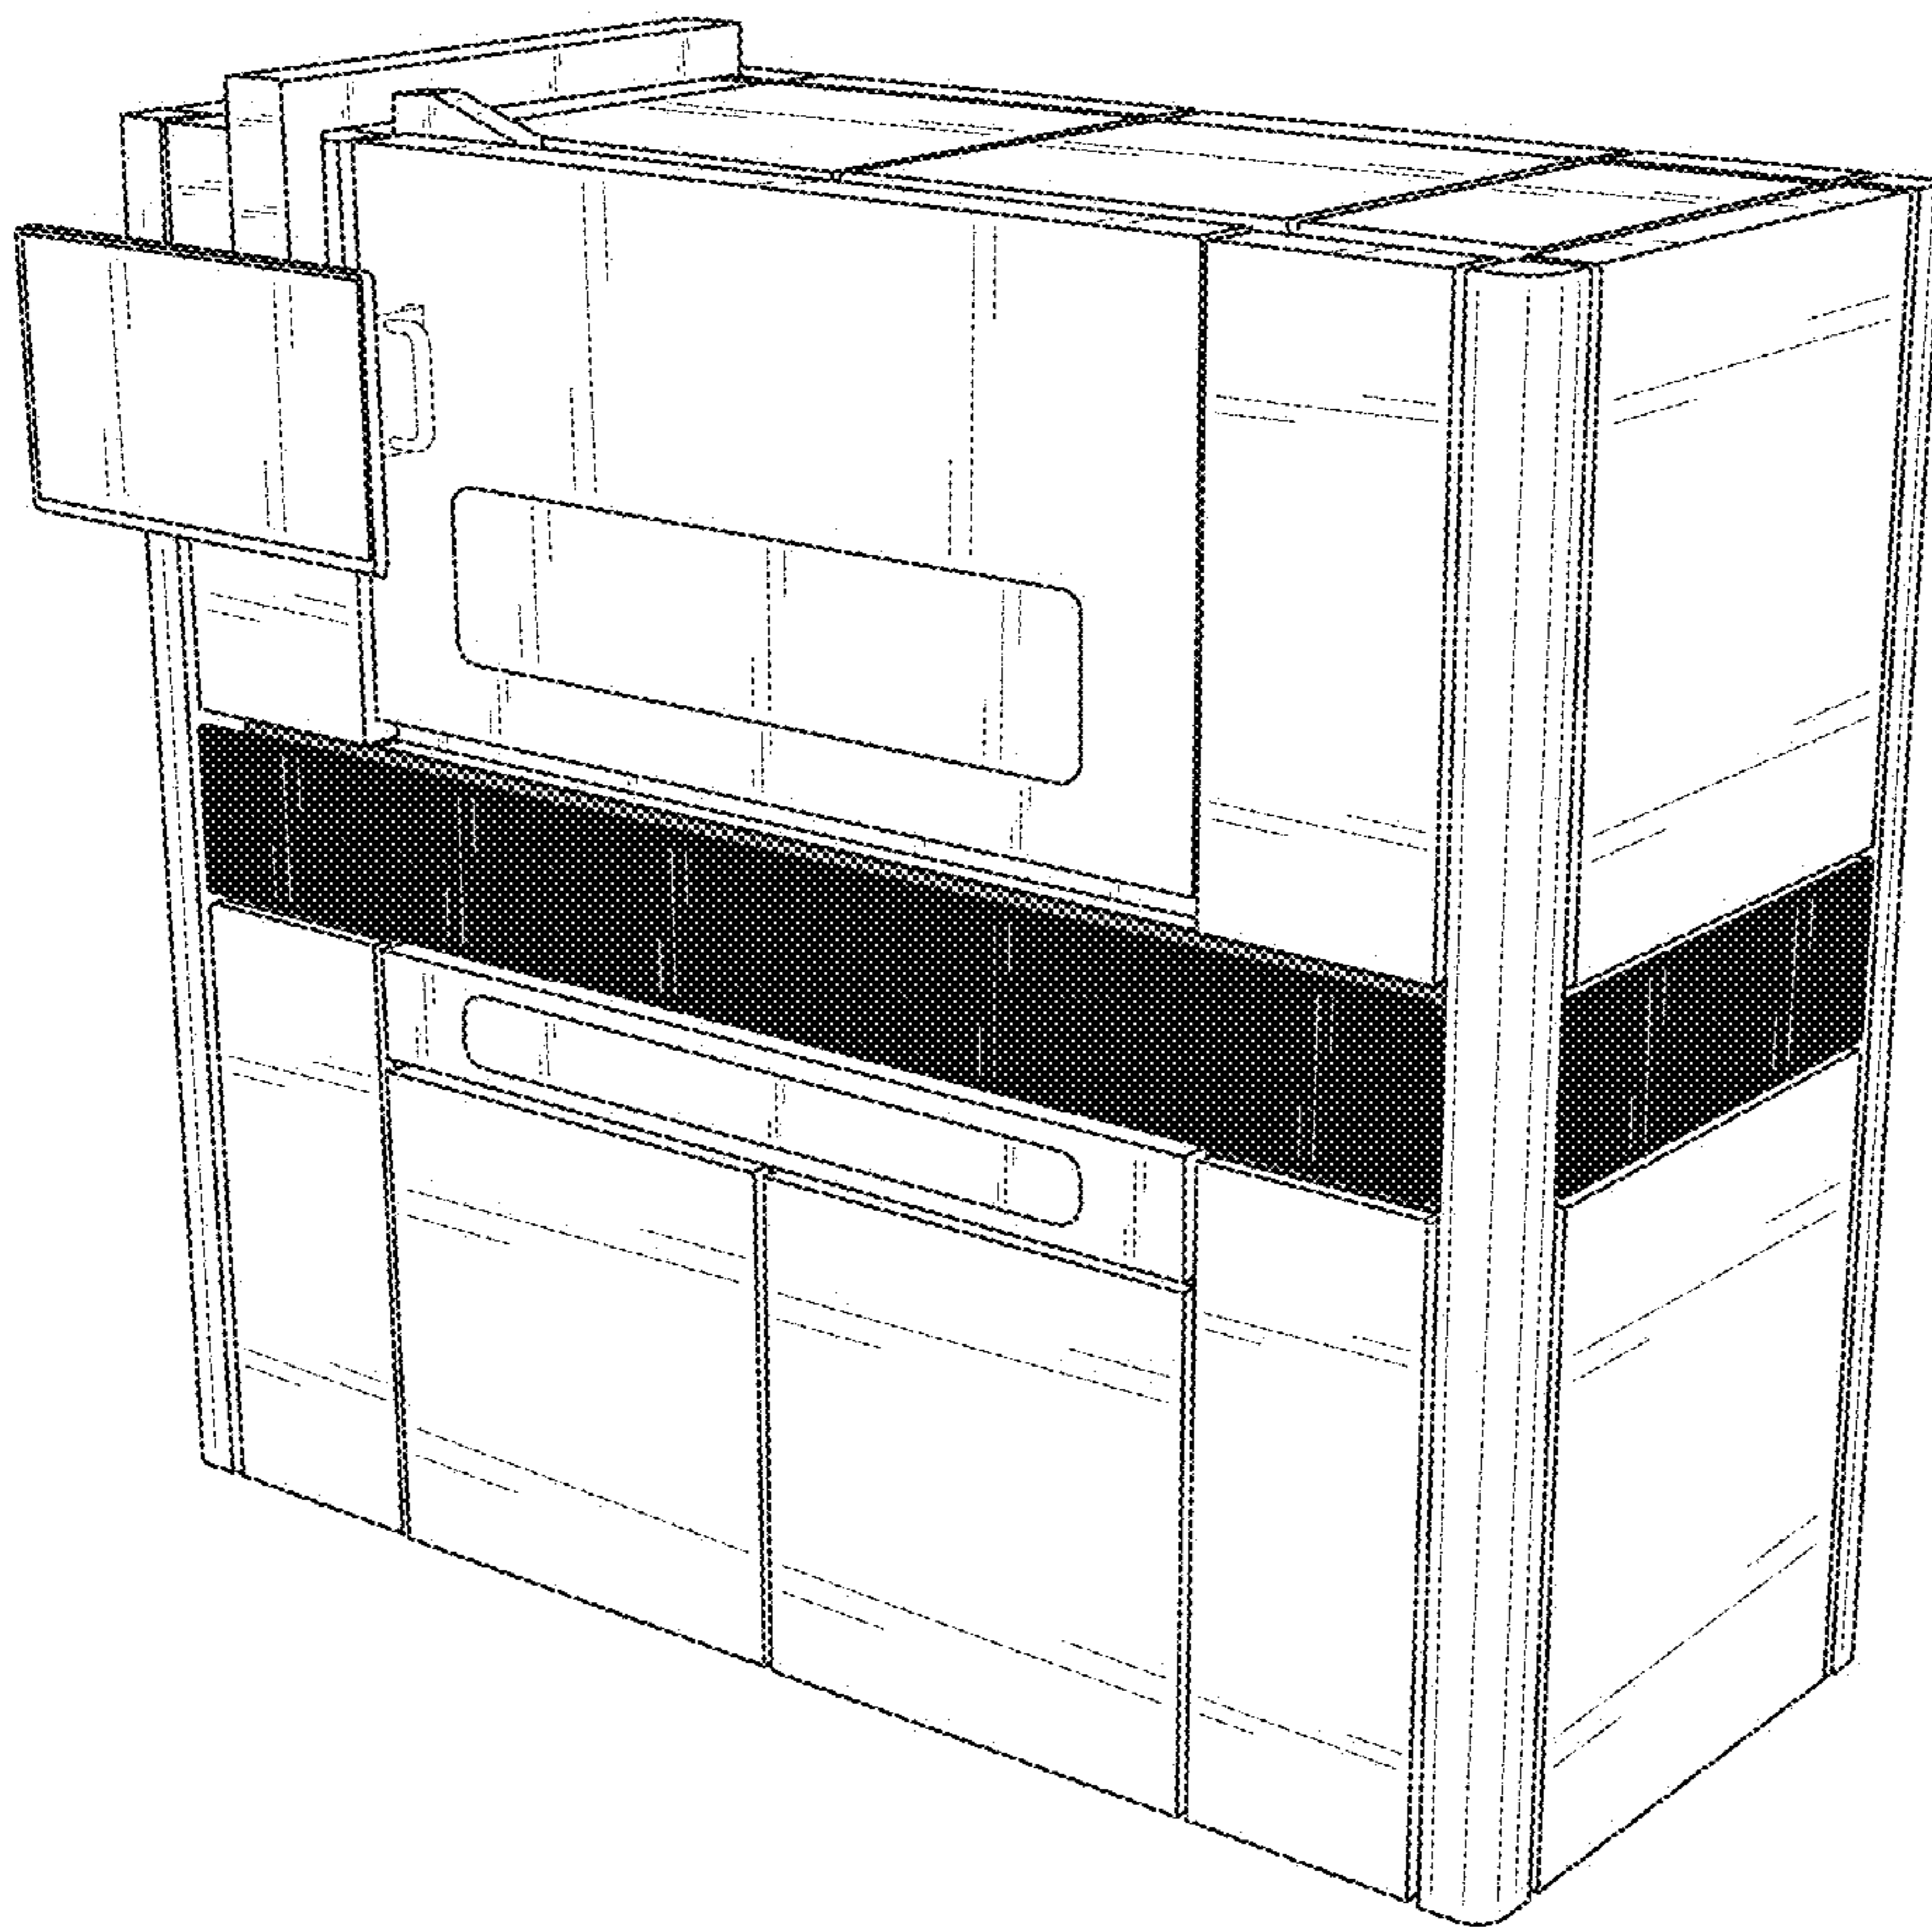


FIG. 19

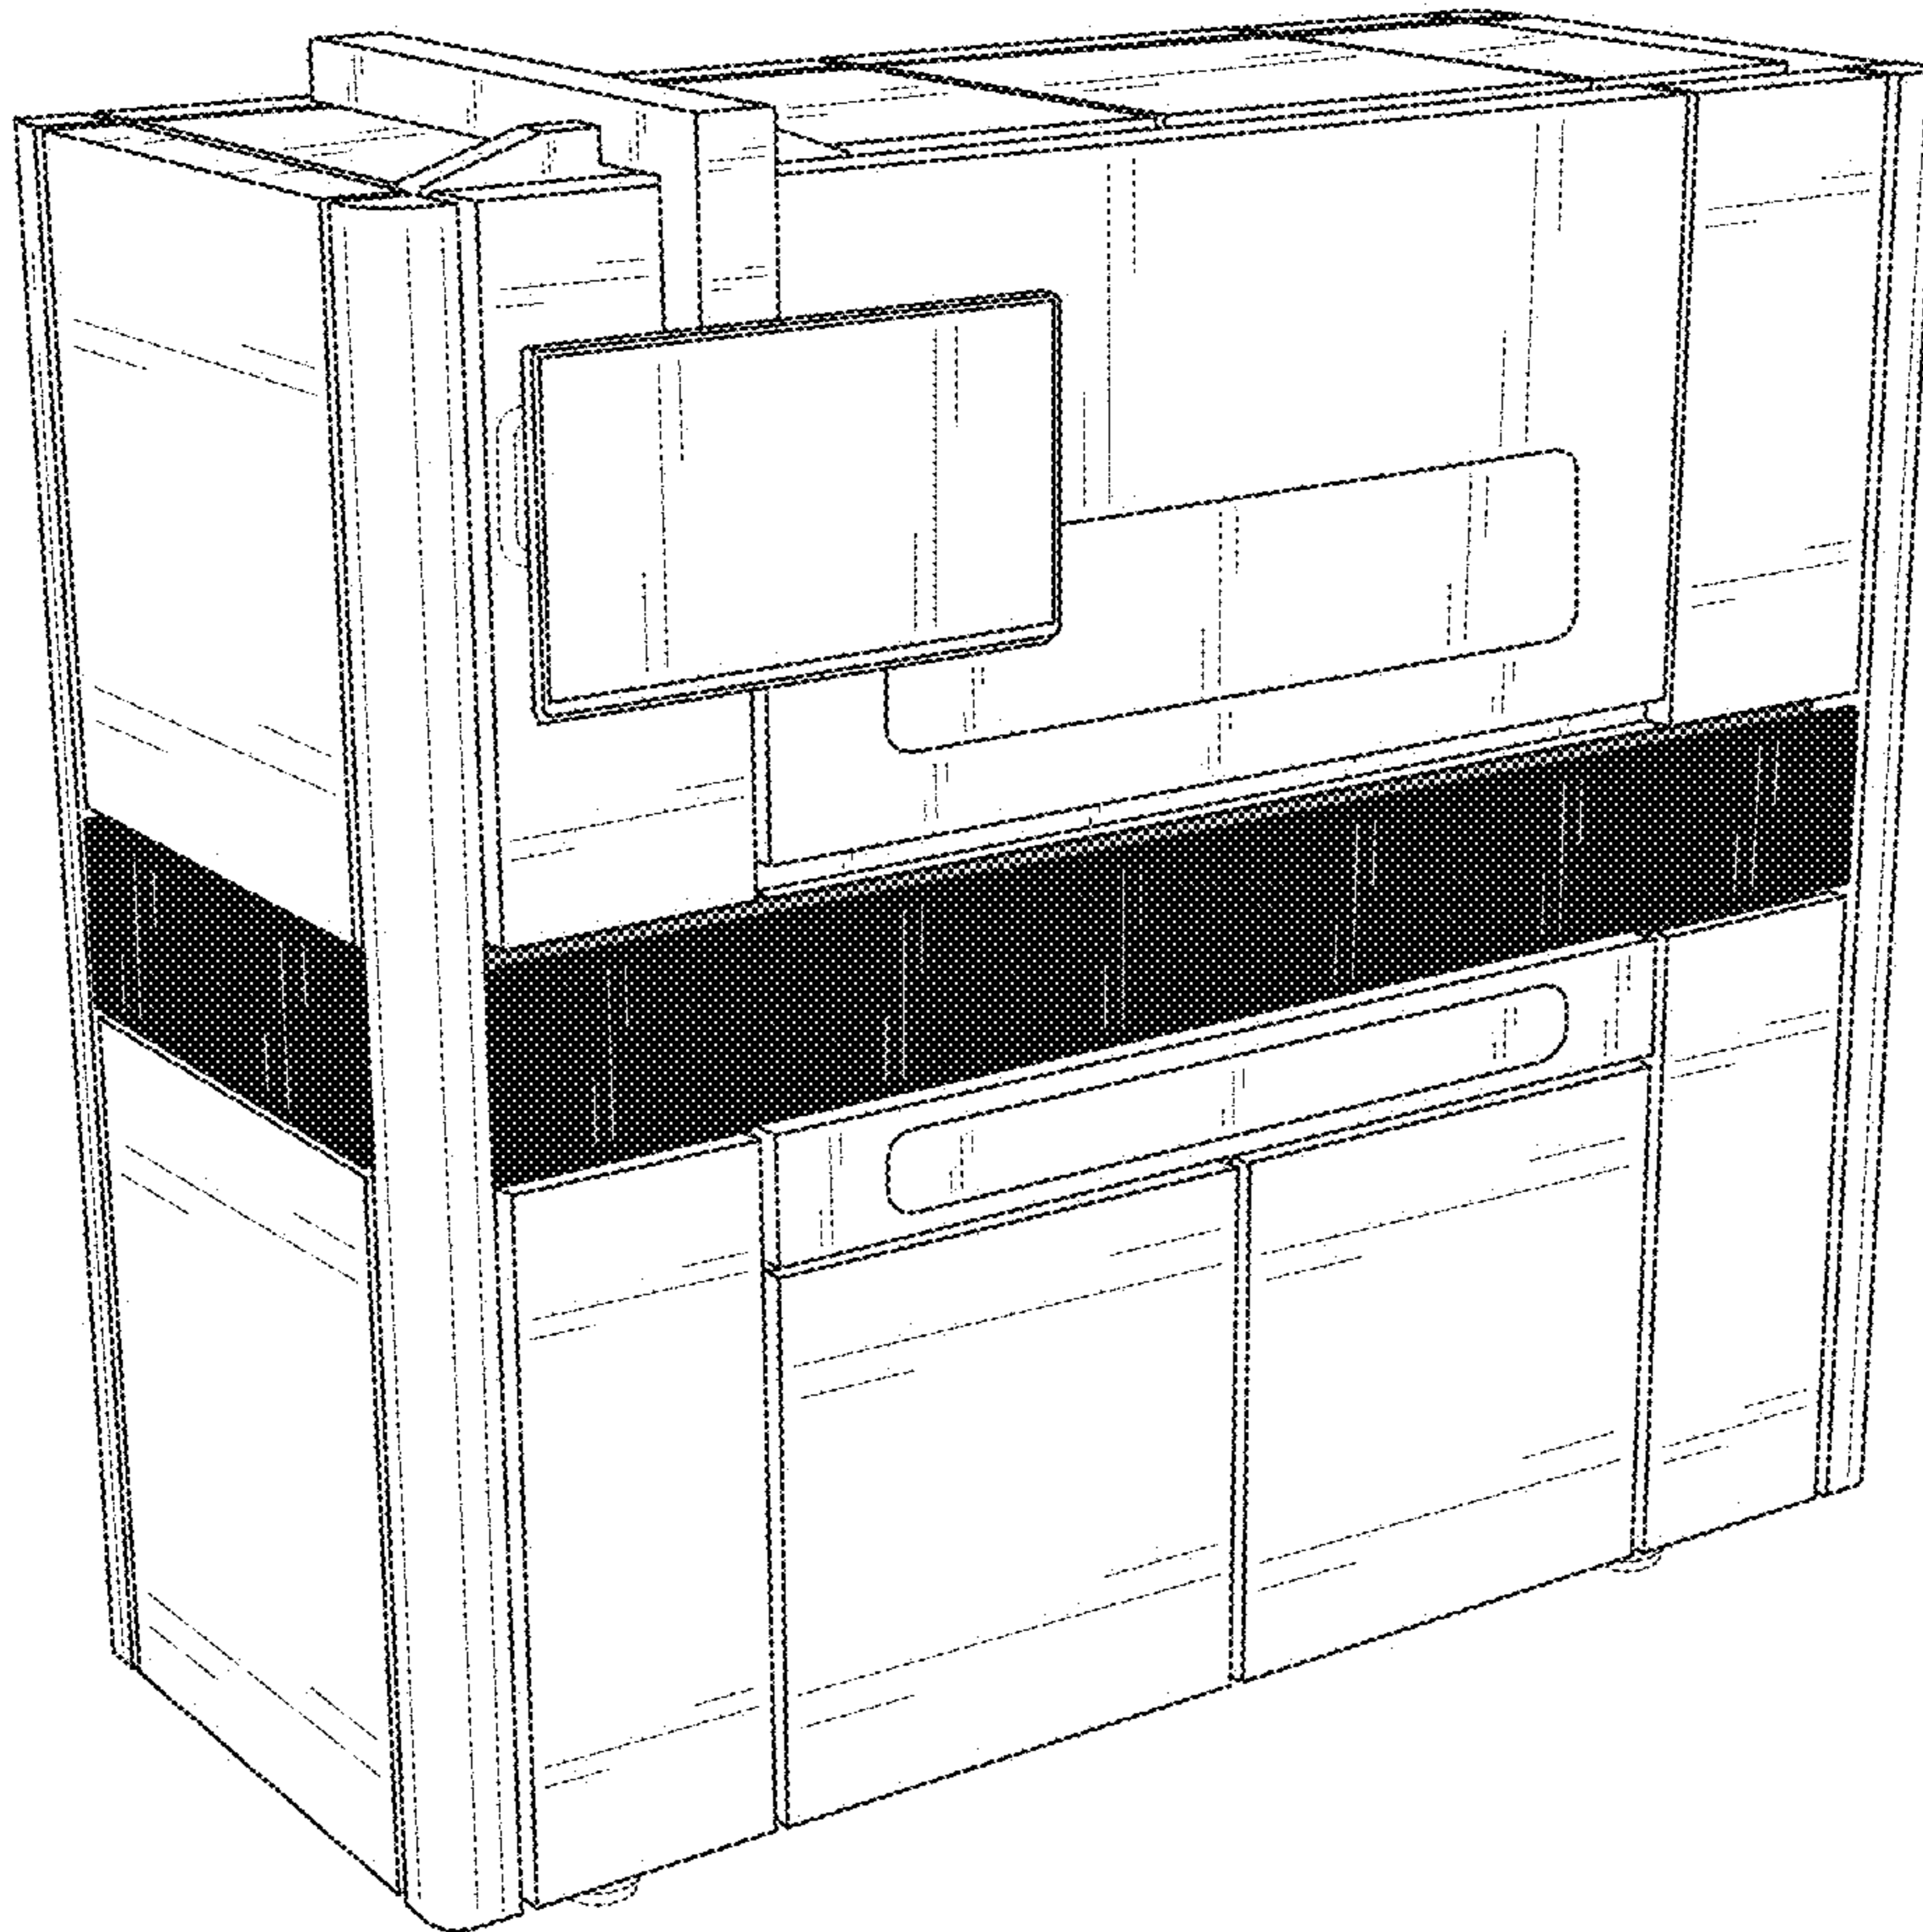


FIG. 20

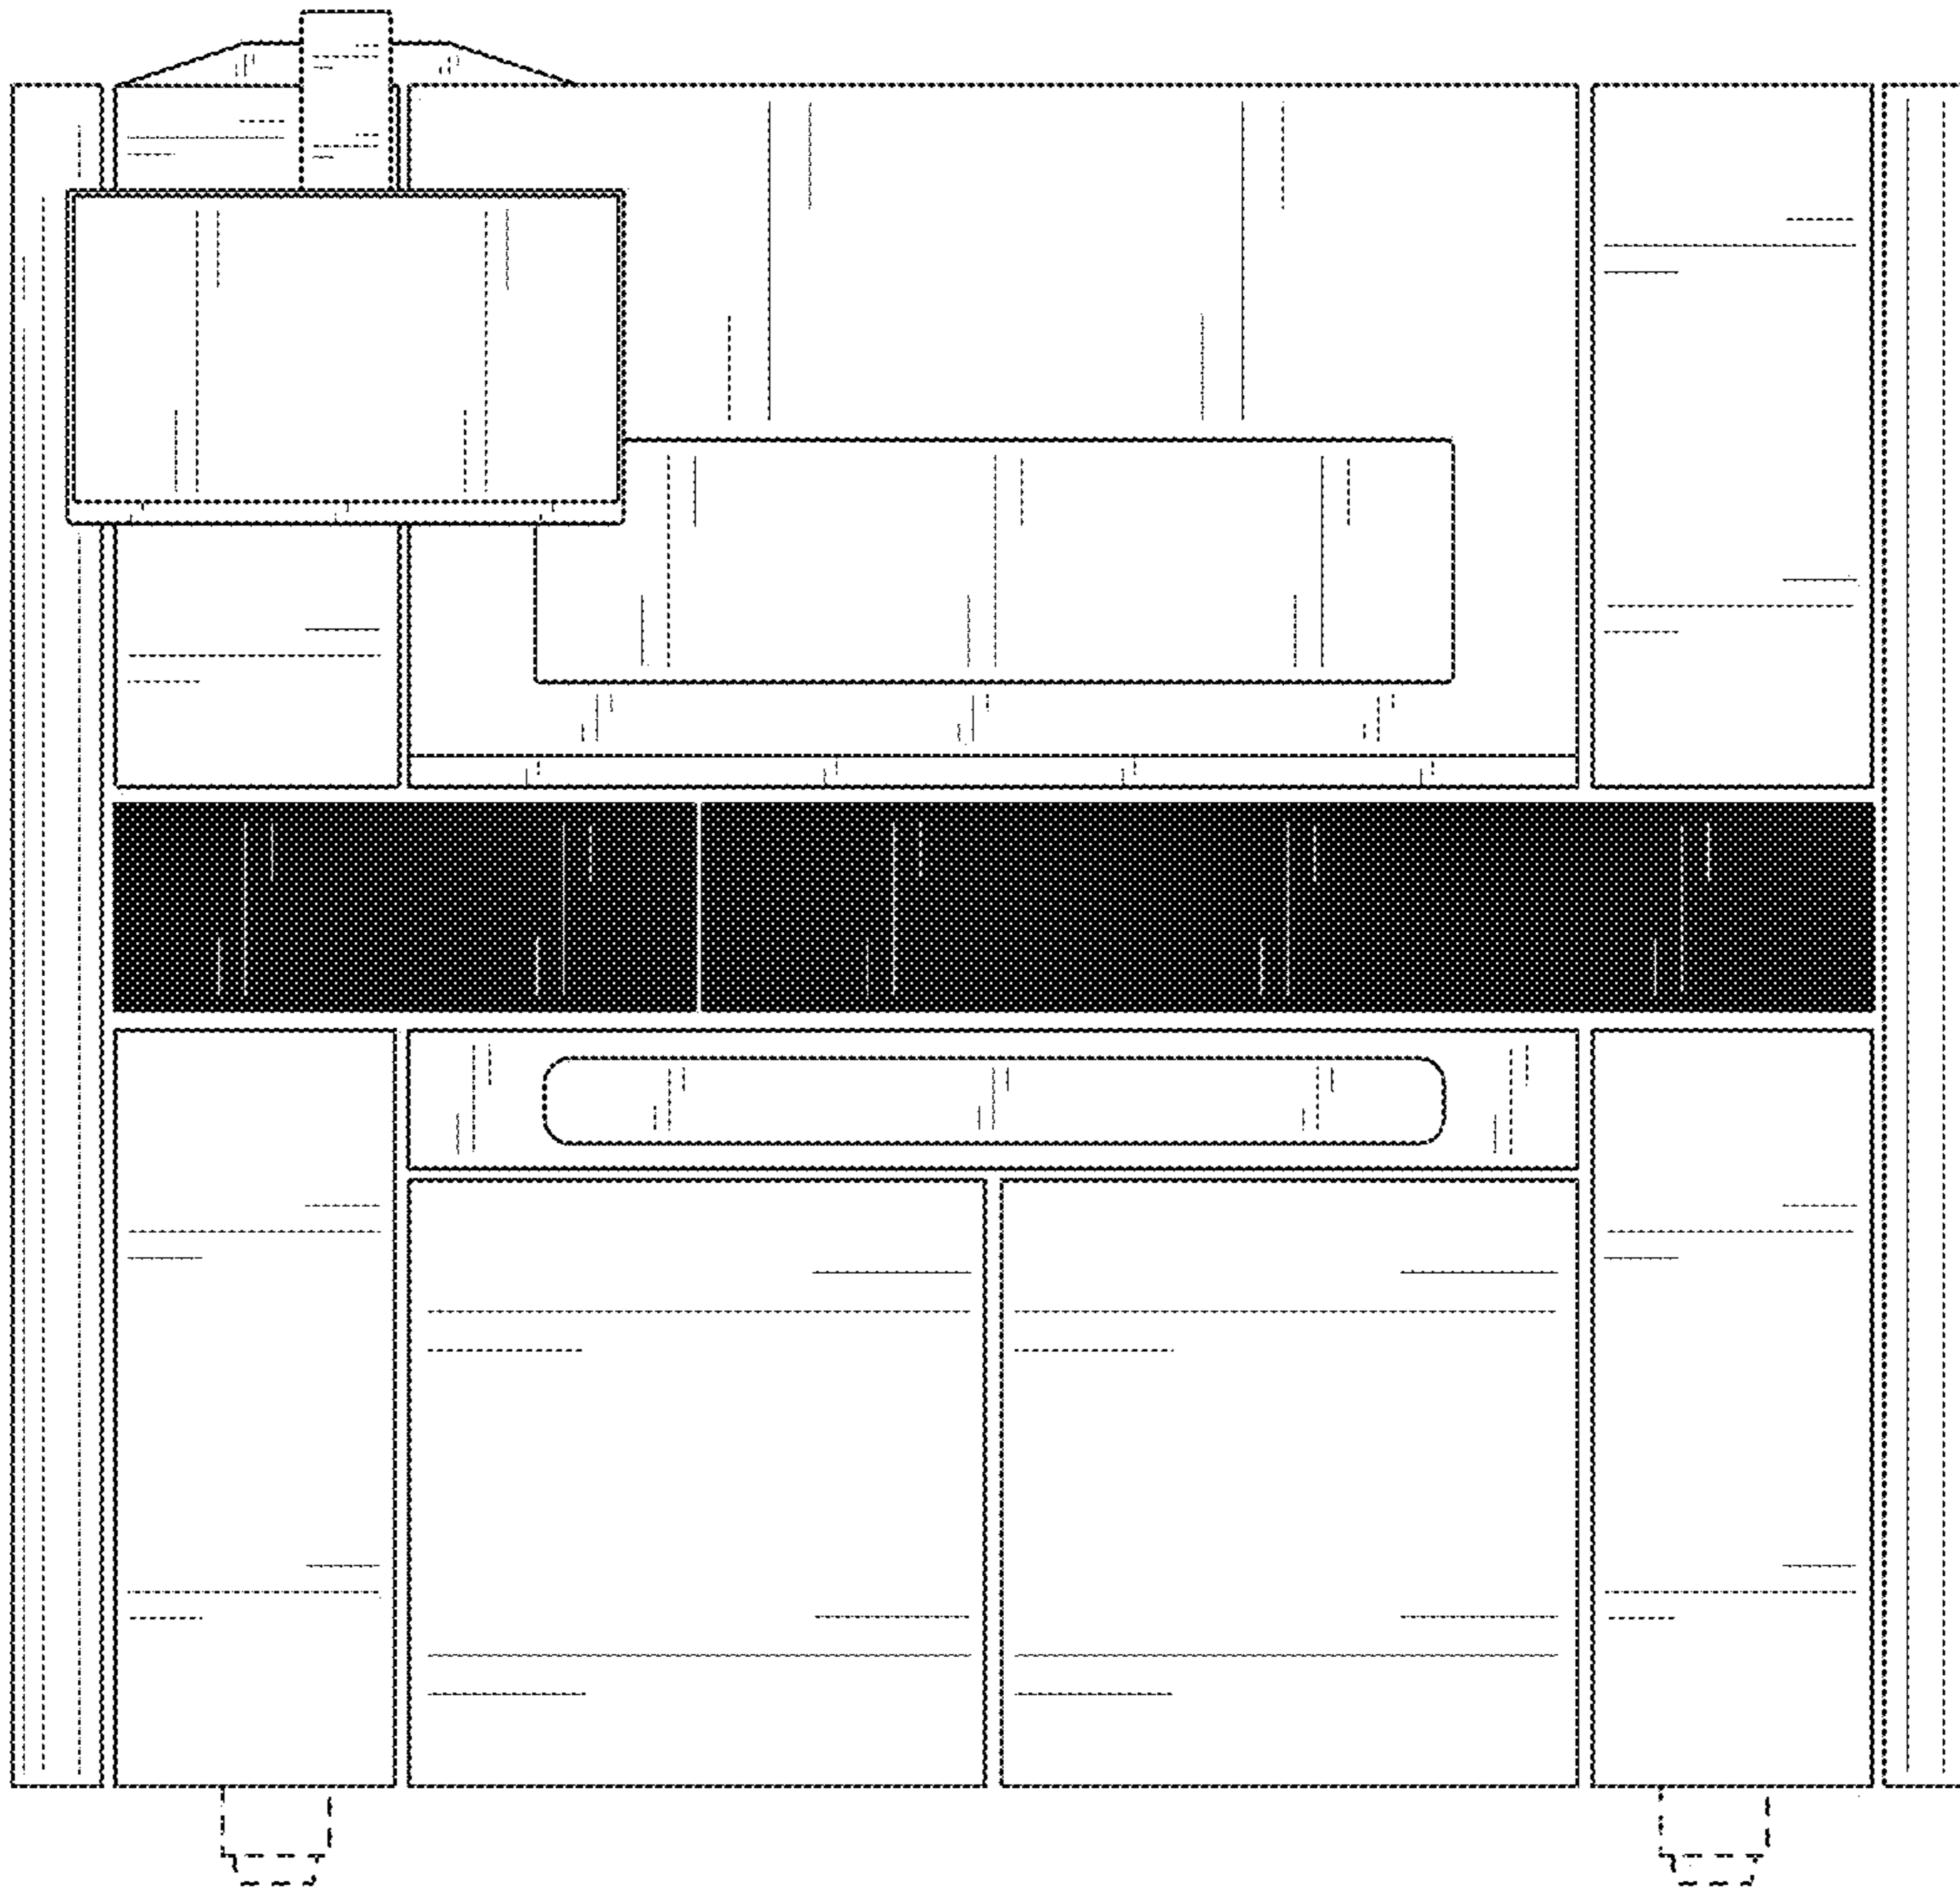


Fig. 21

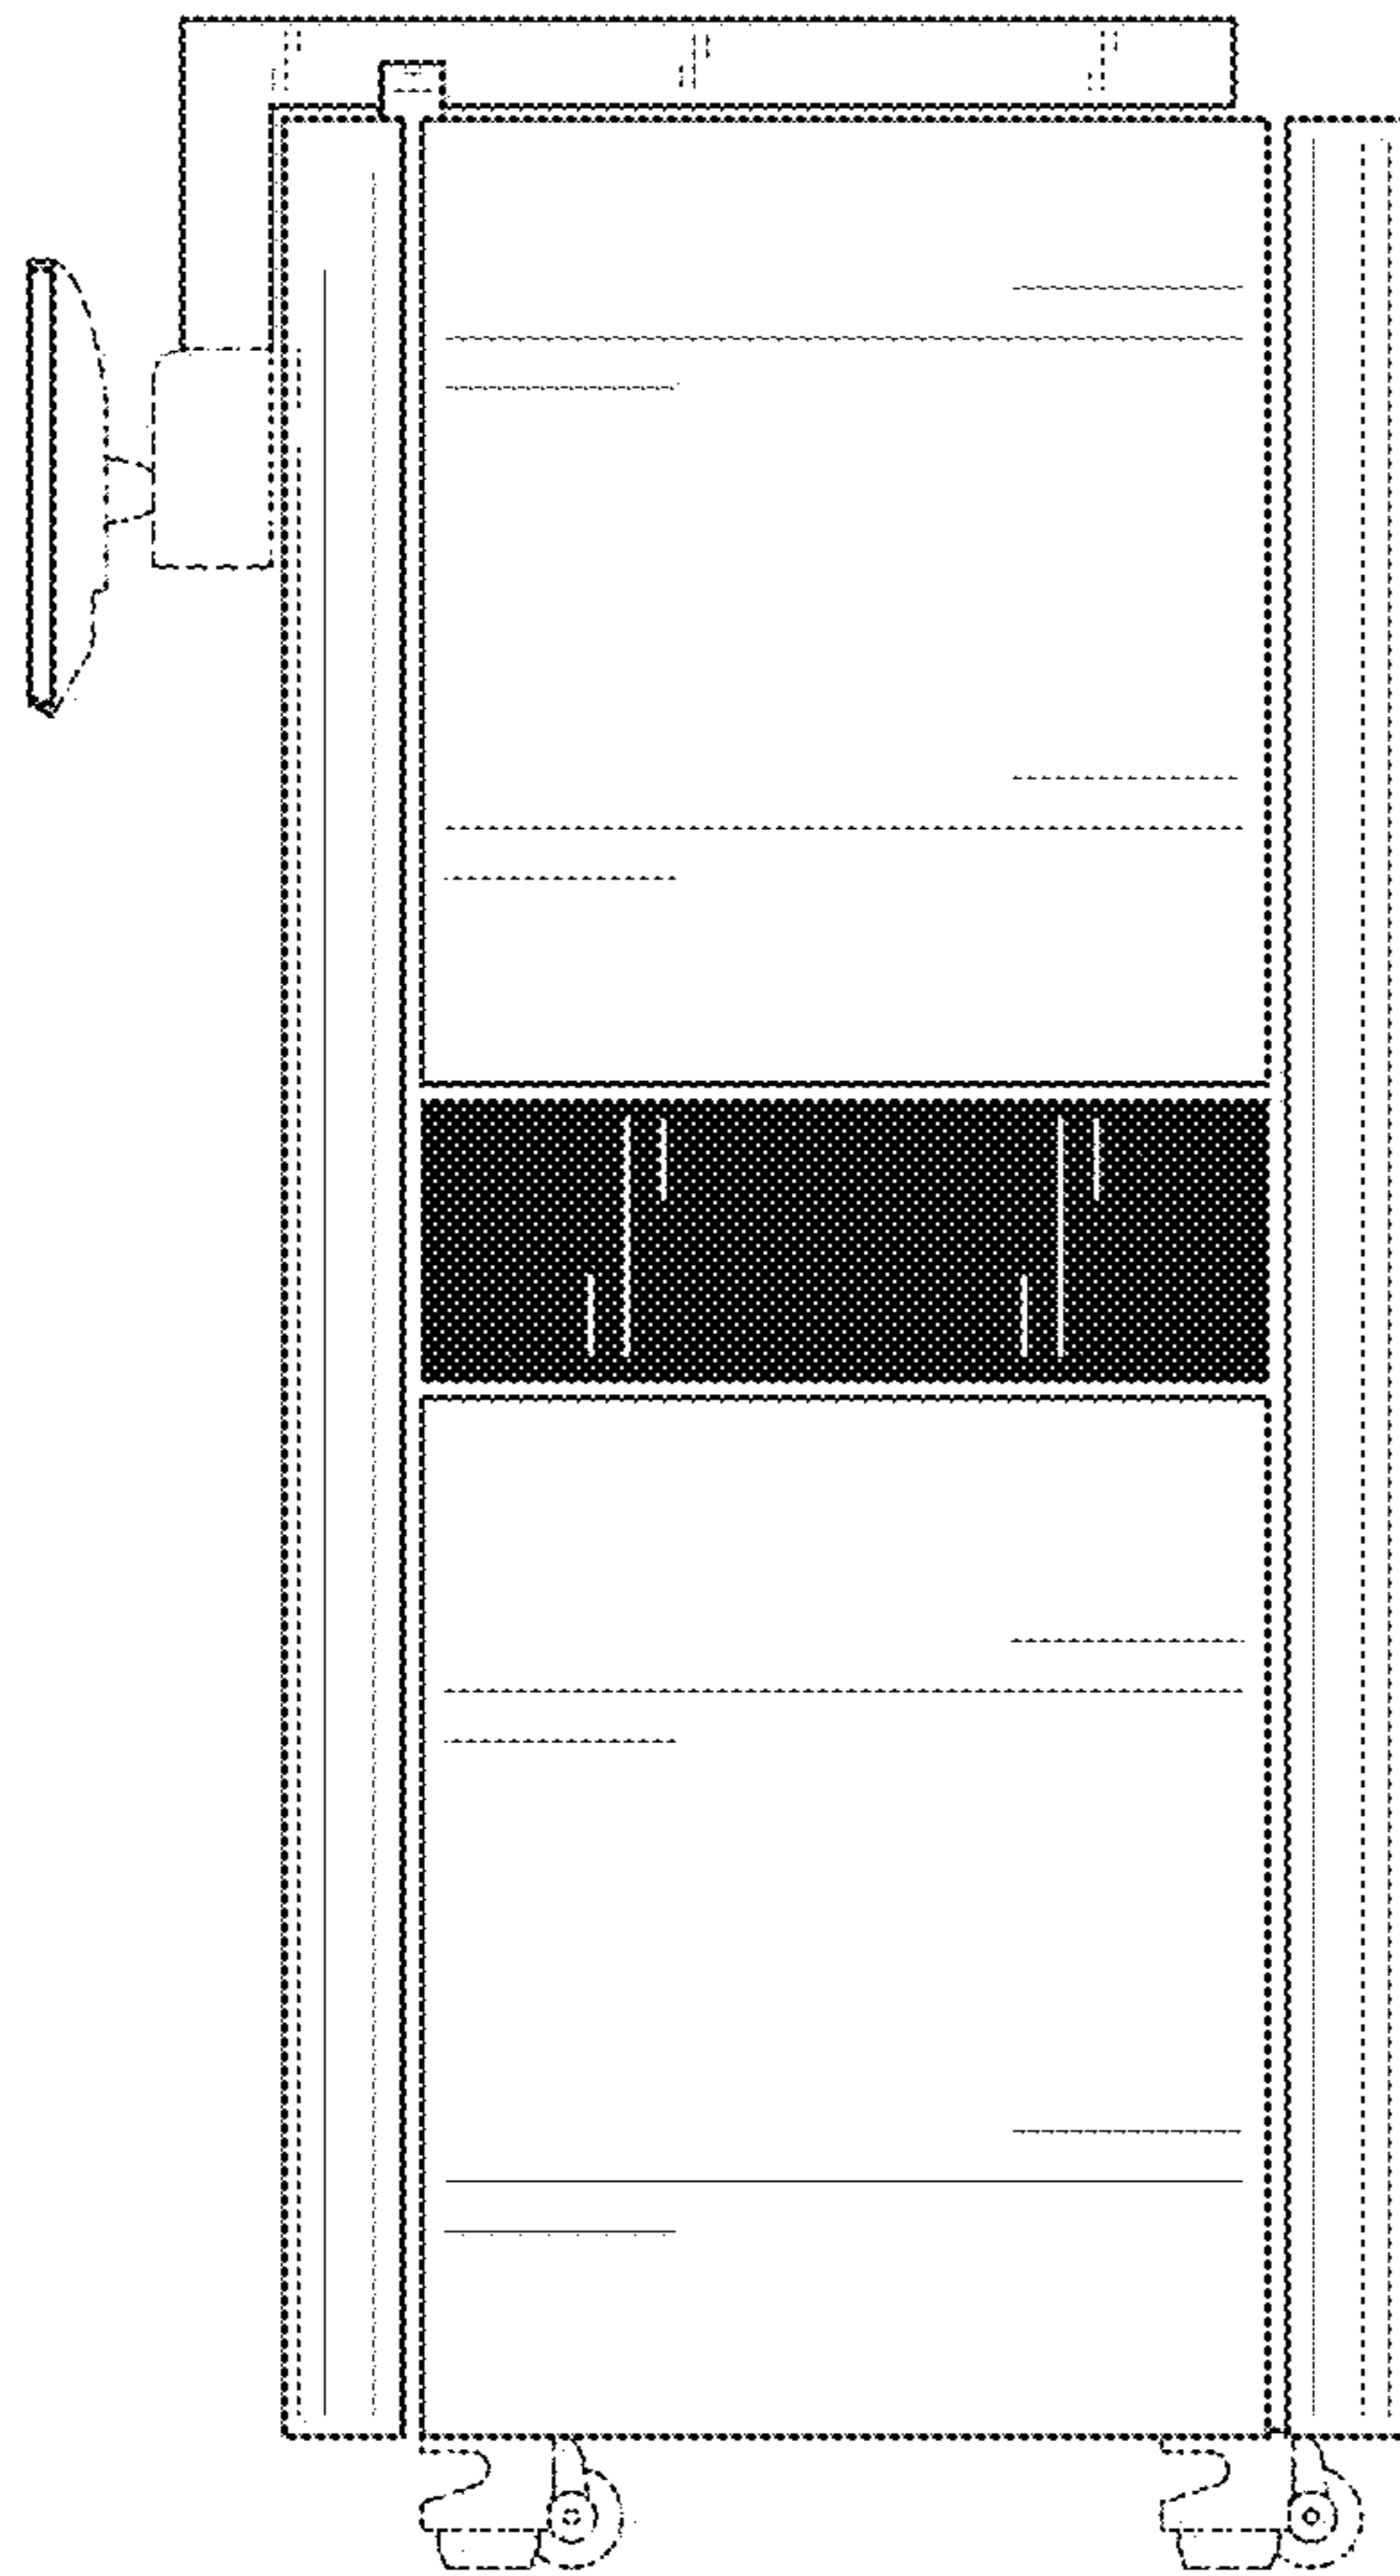


FIG. 22



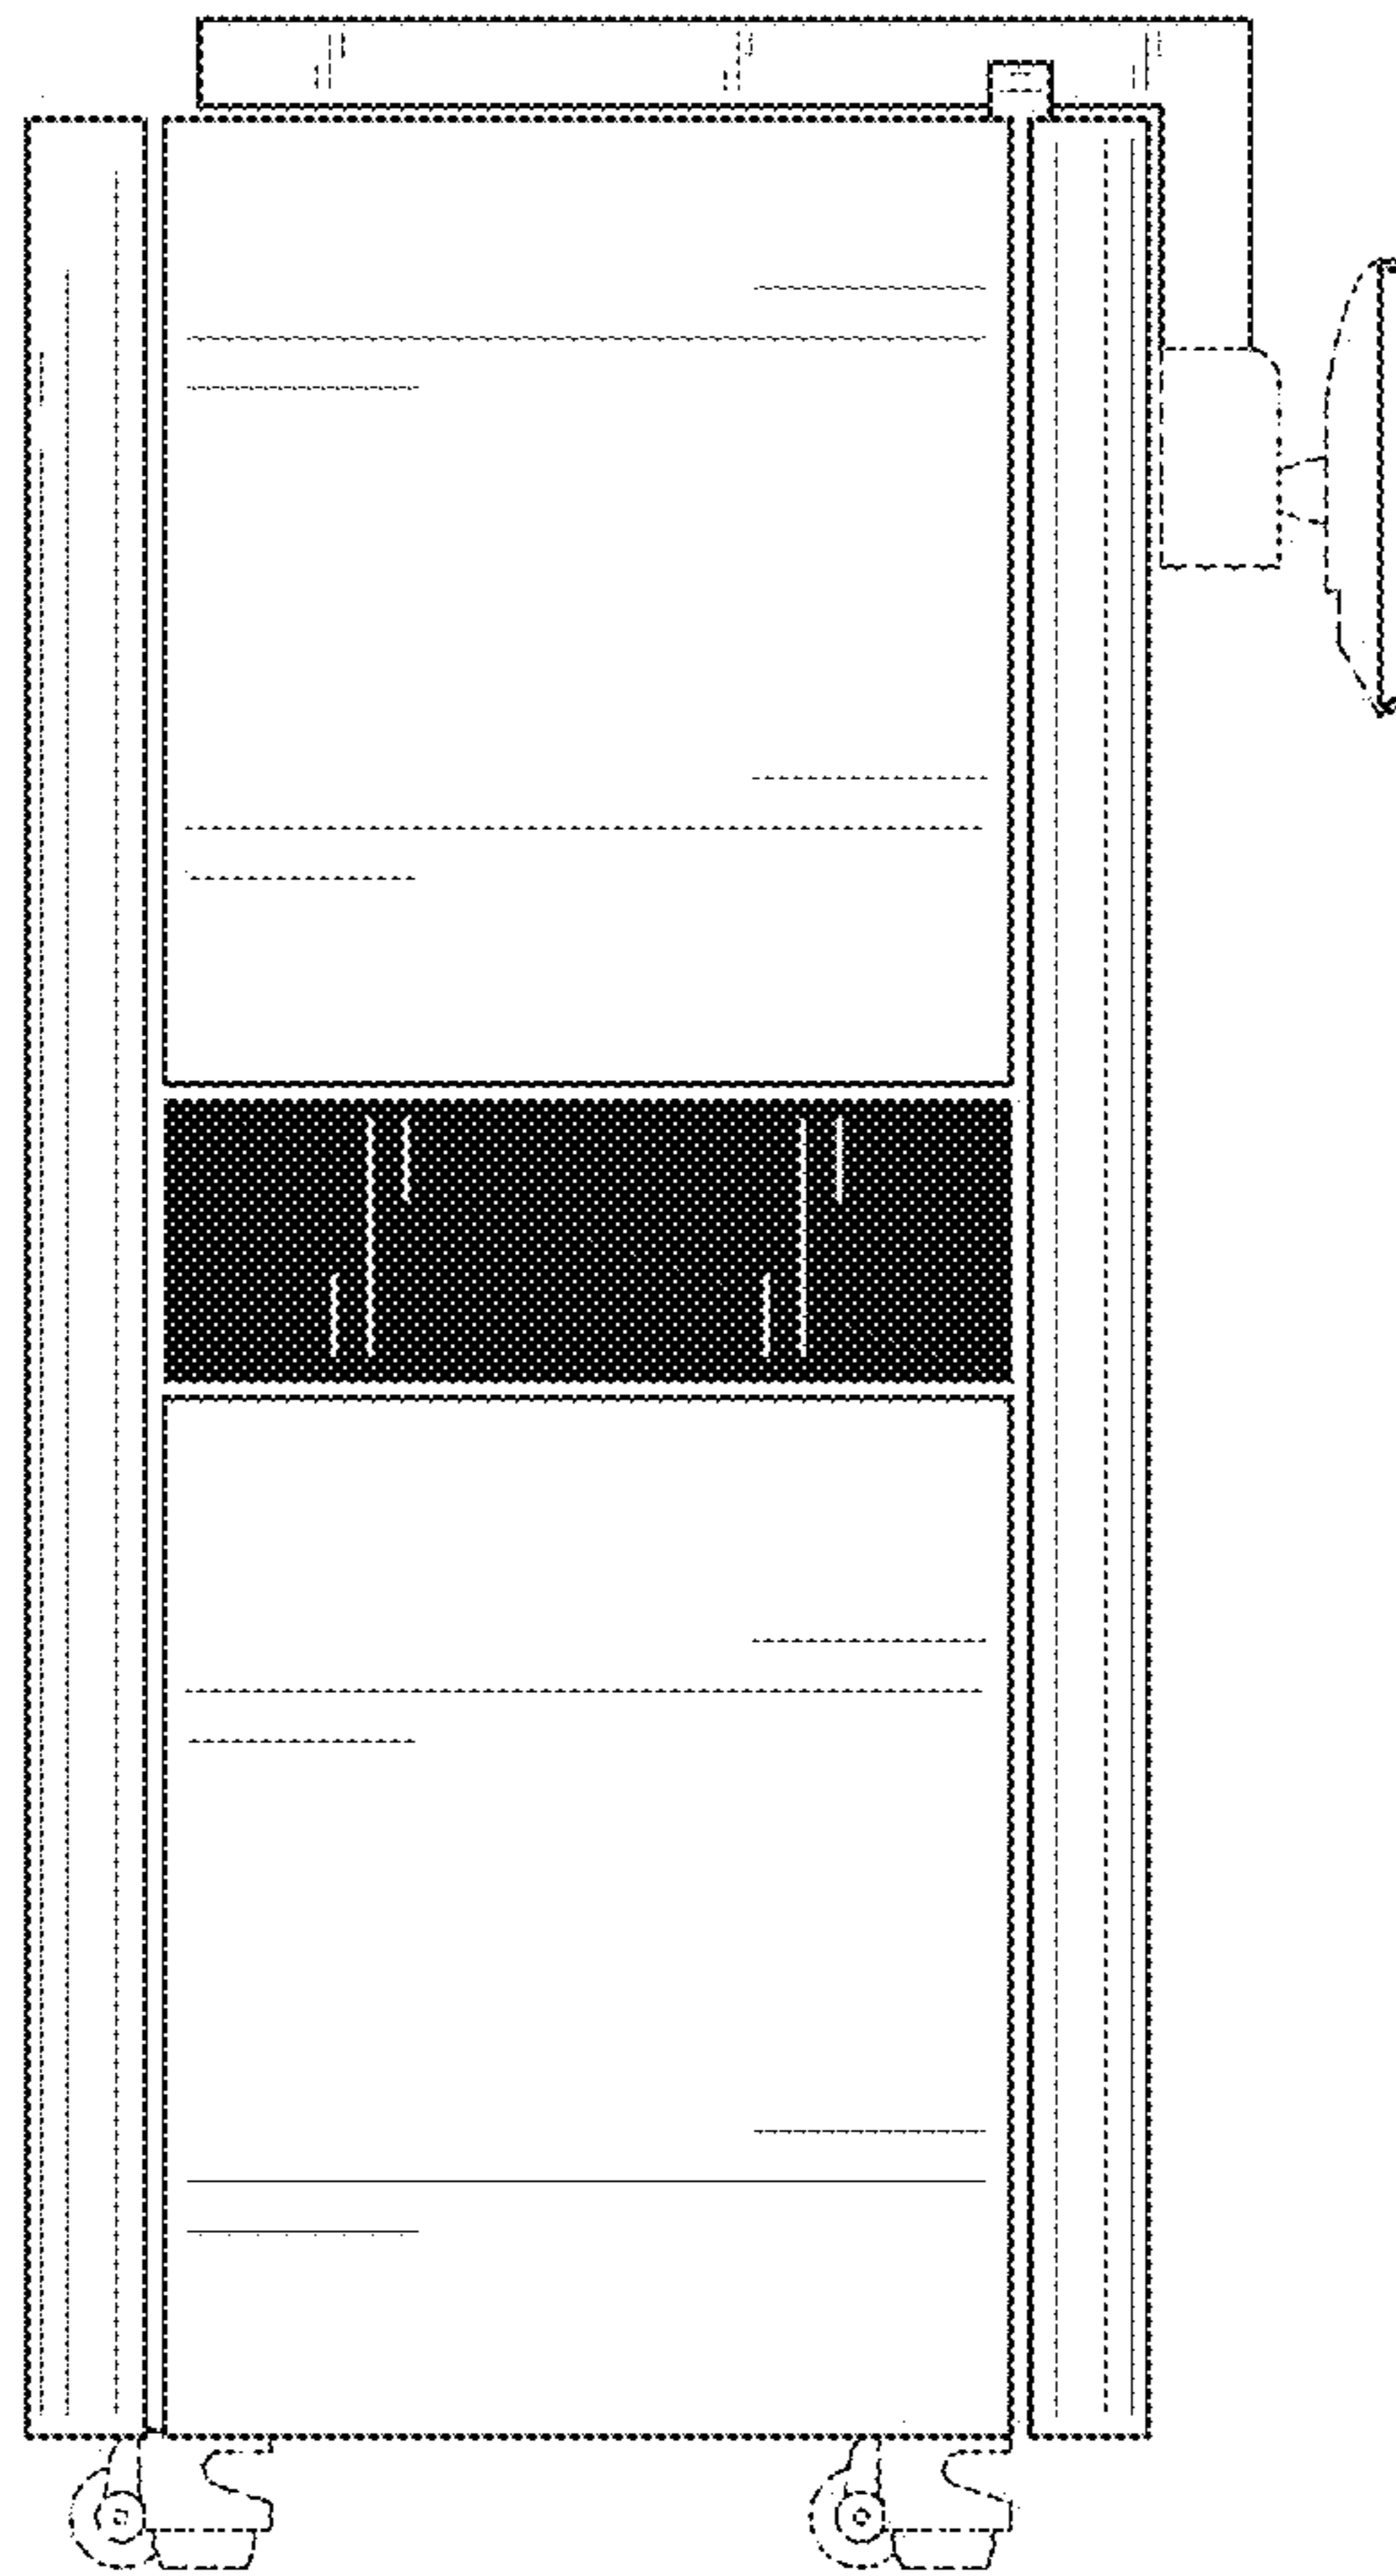


FIG. 23

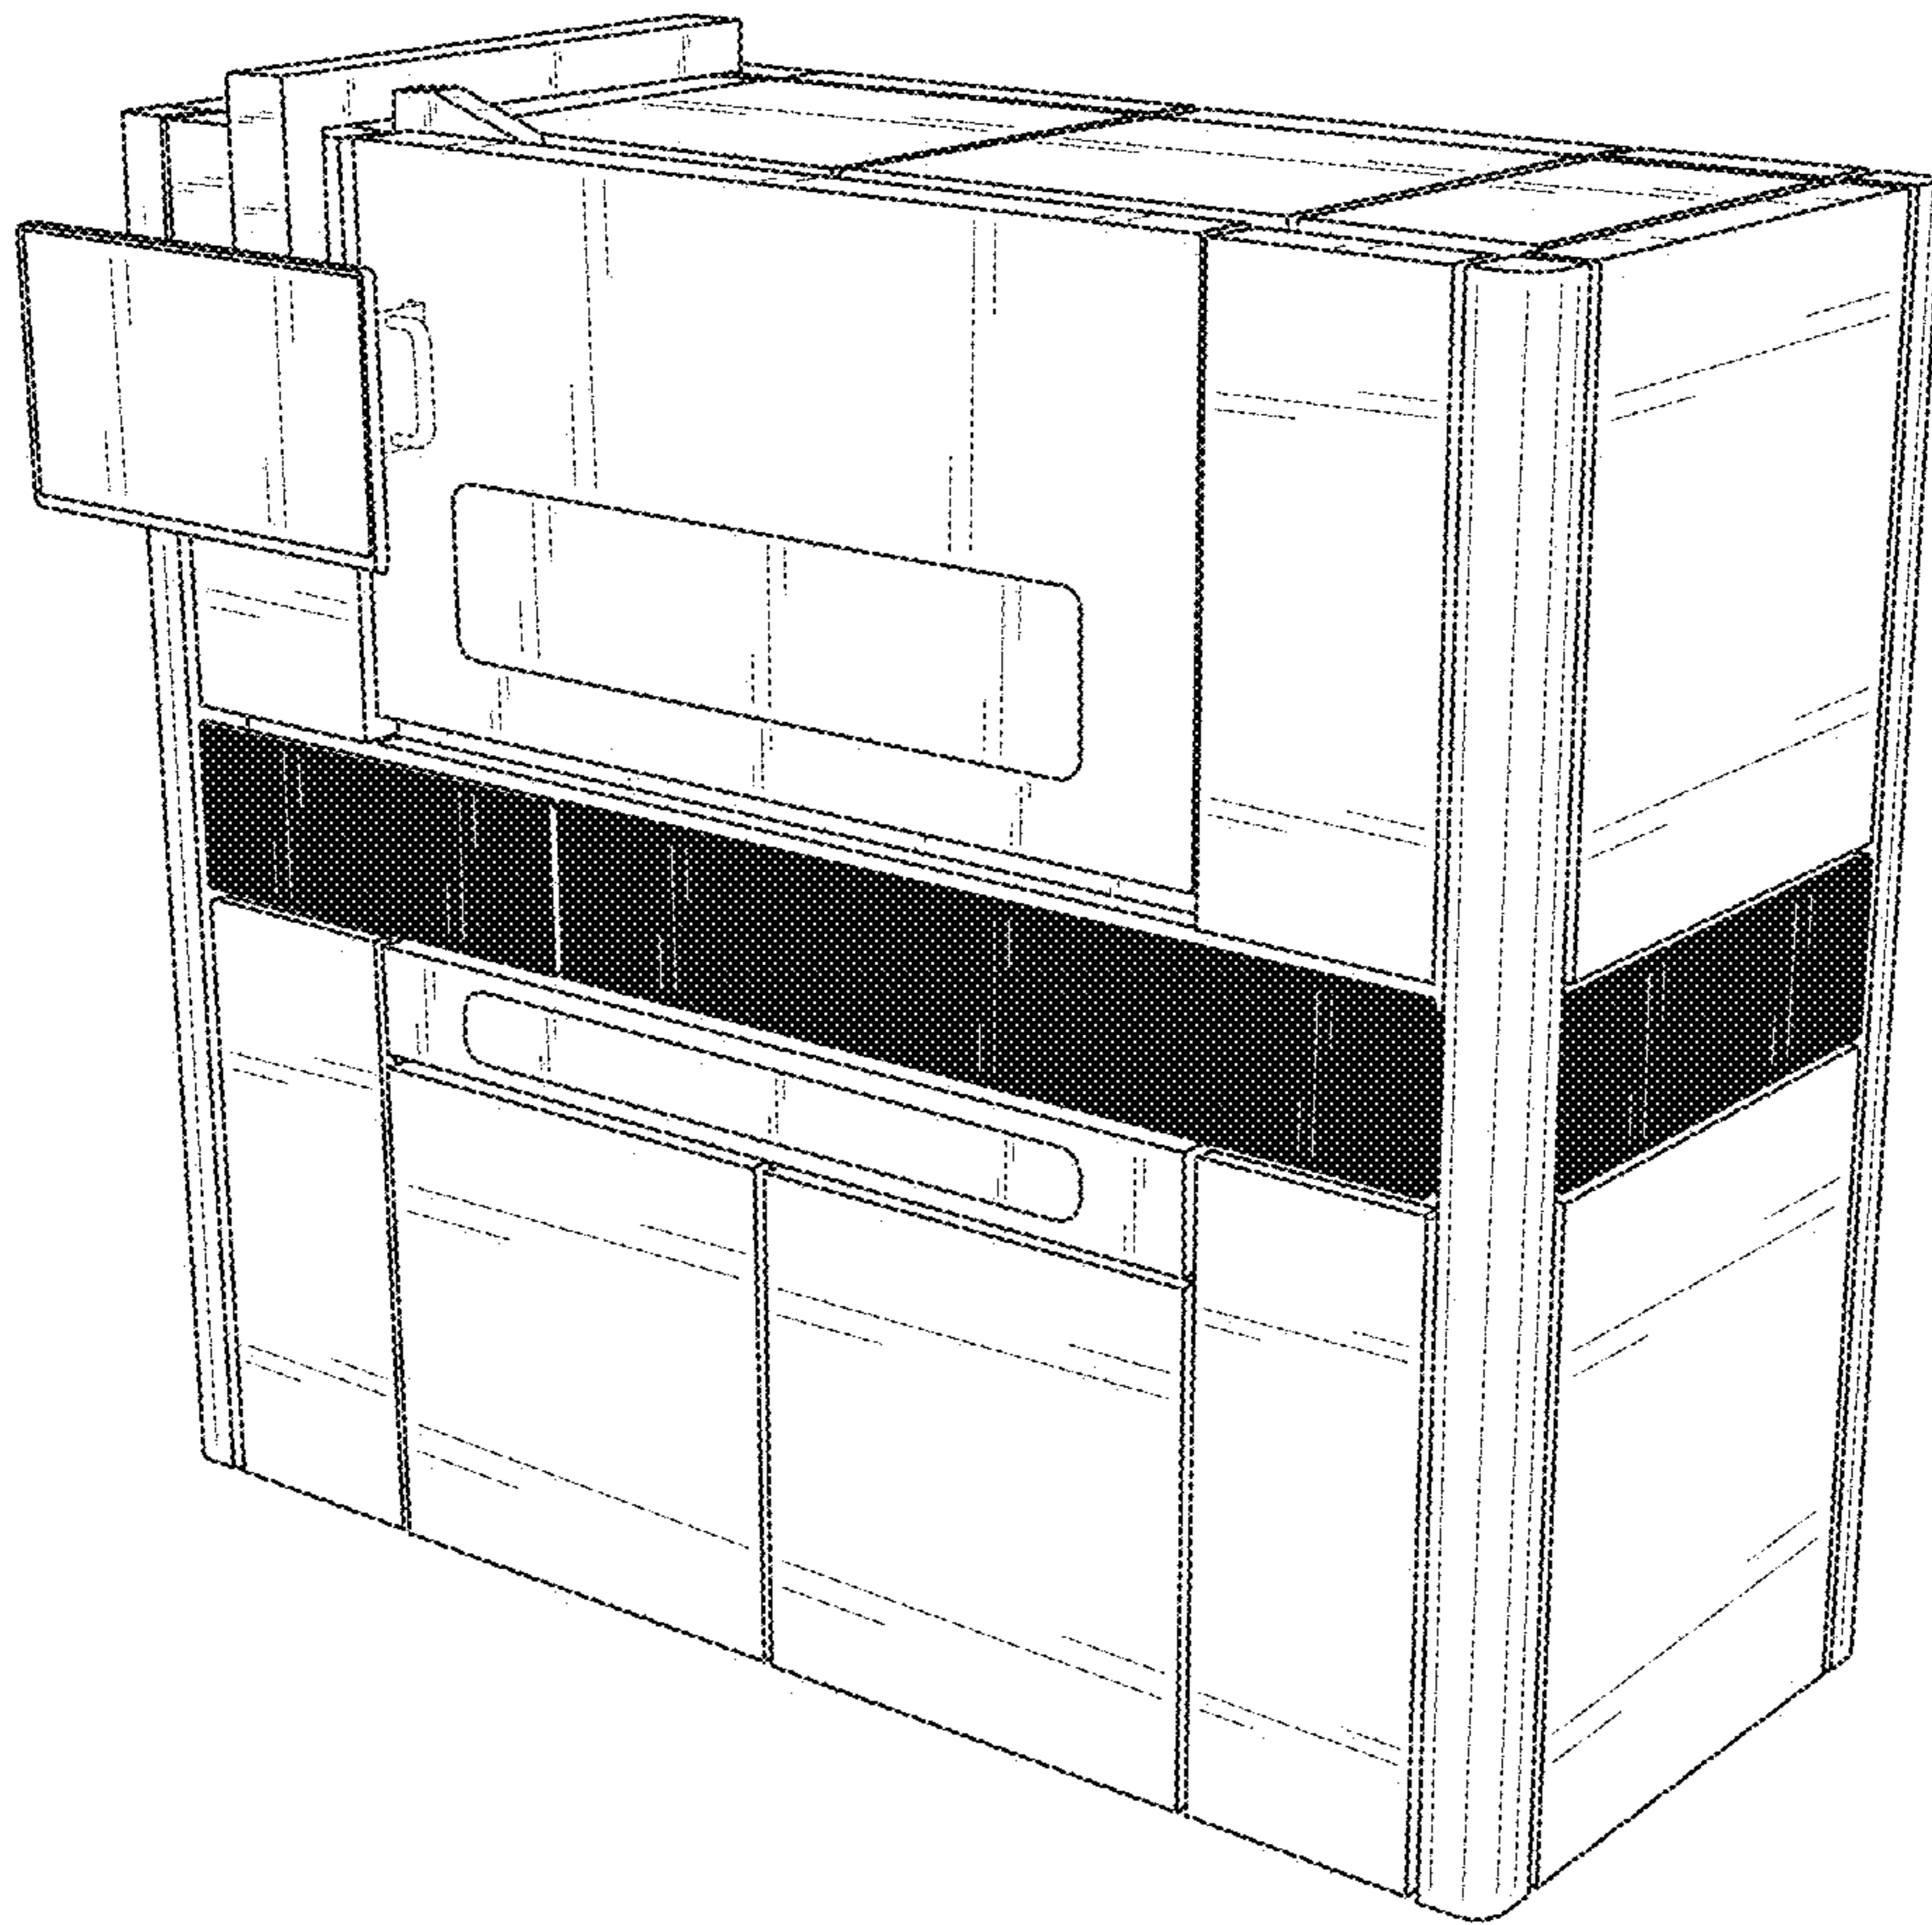


FIG. 24

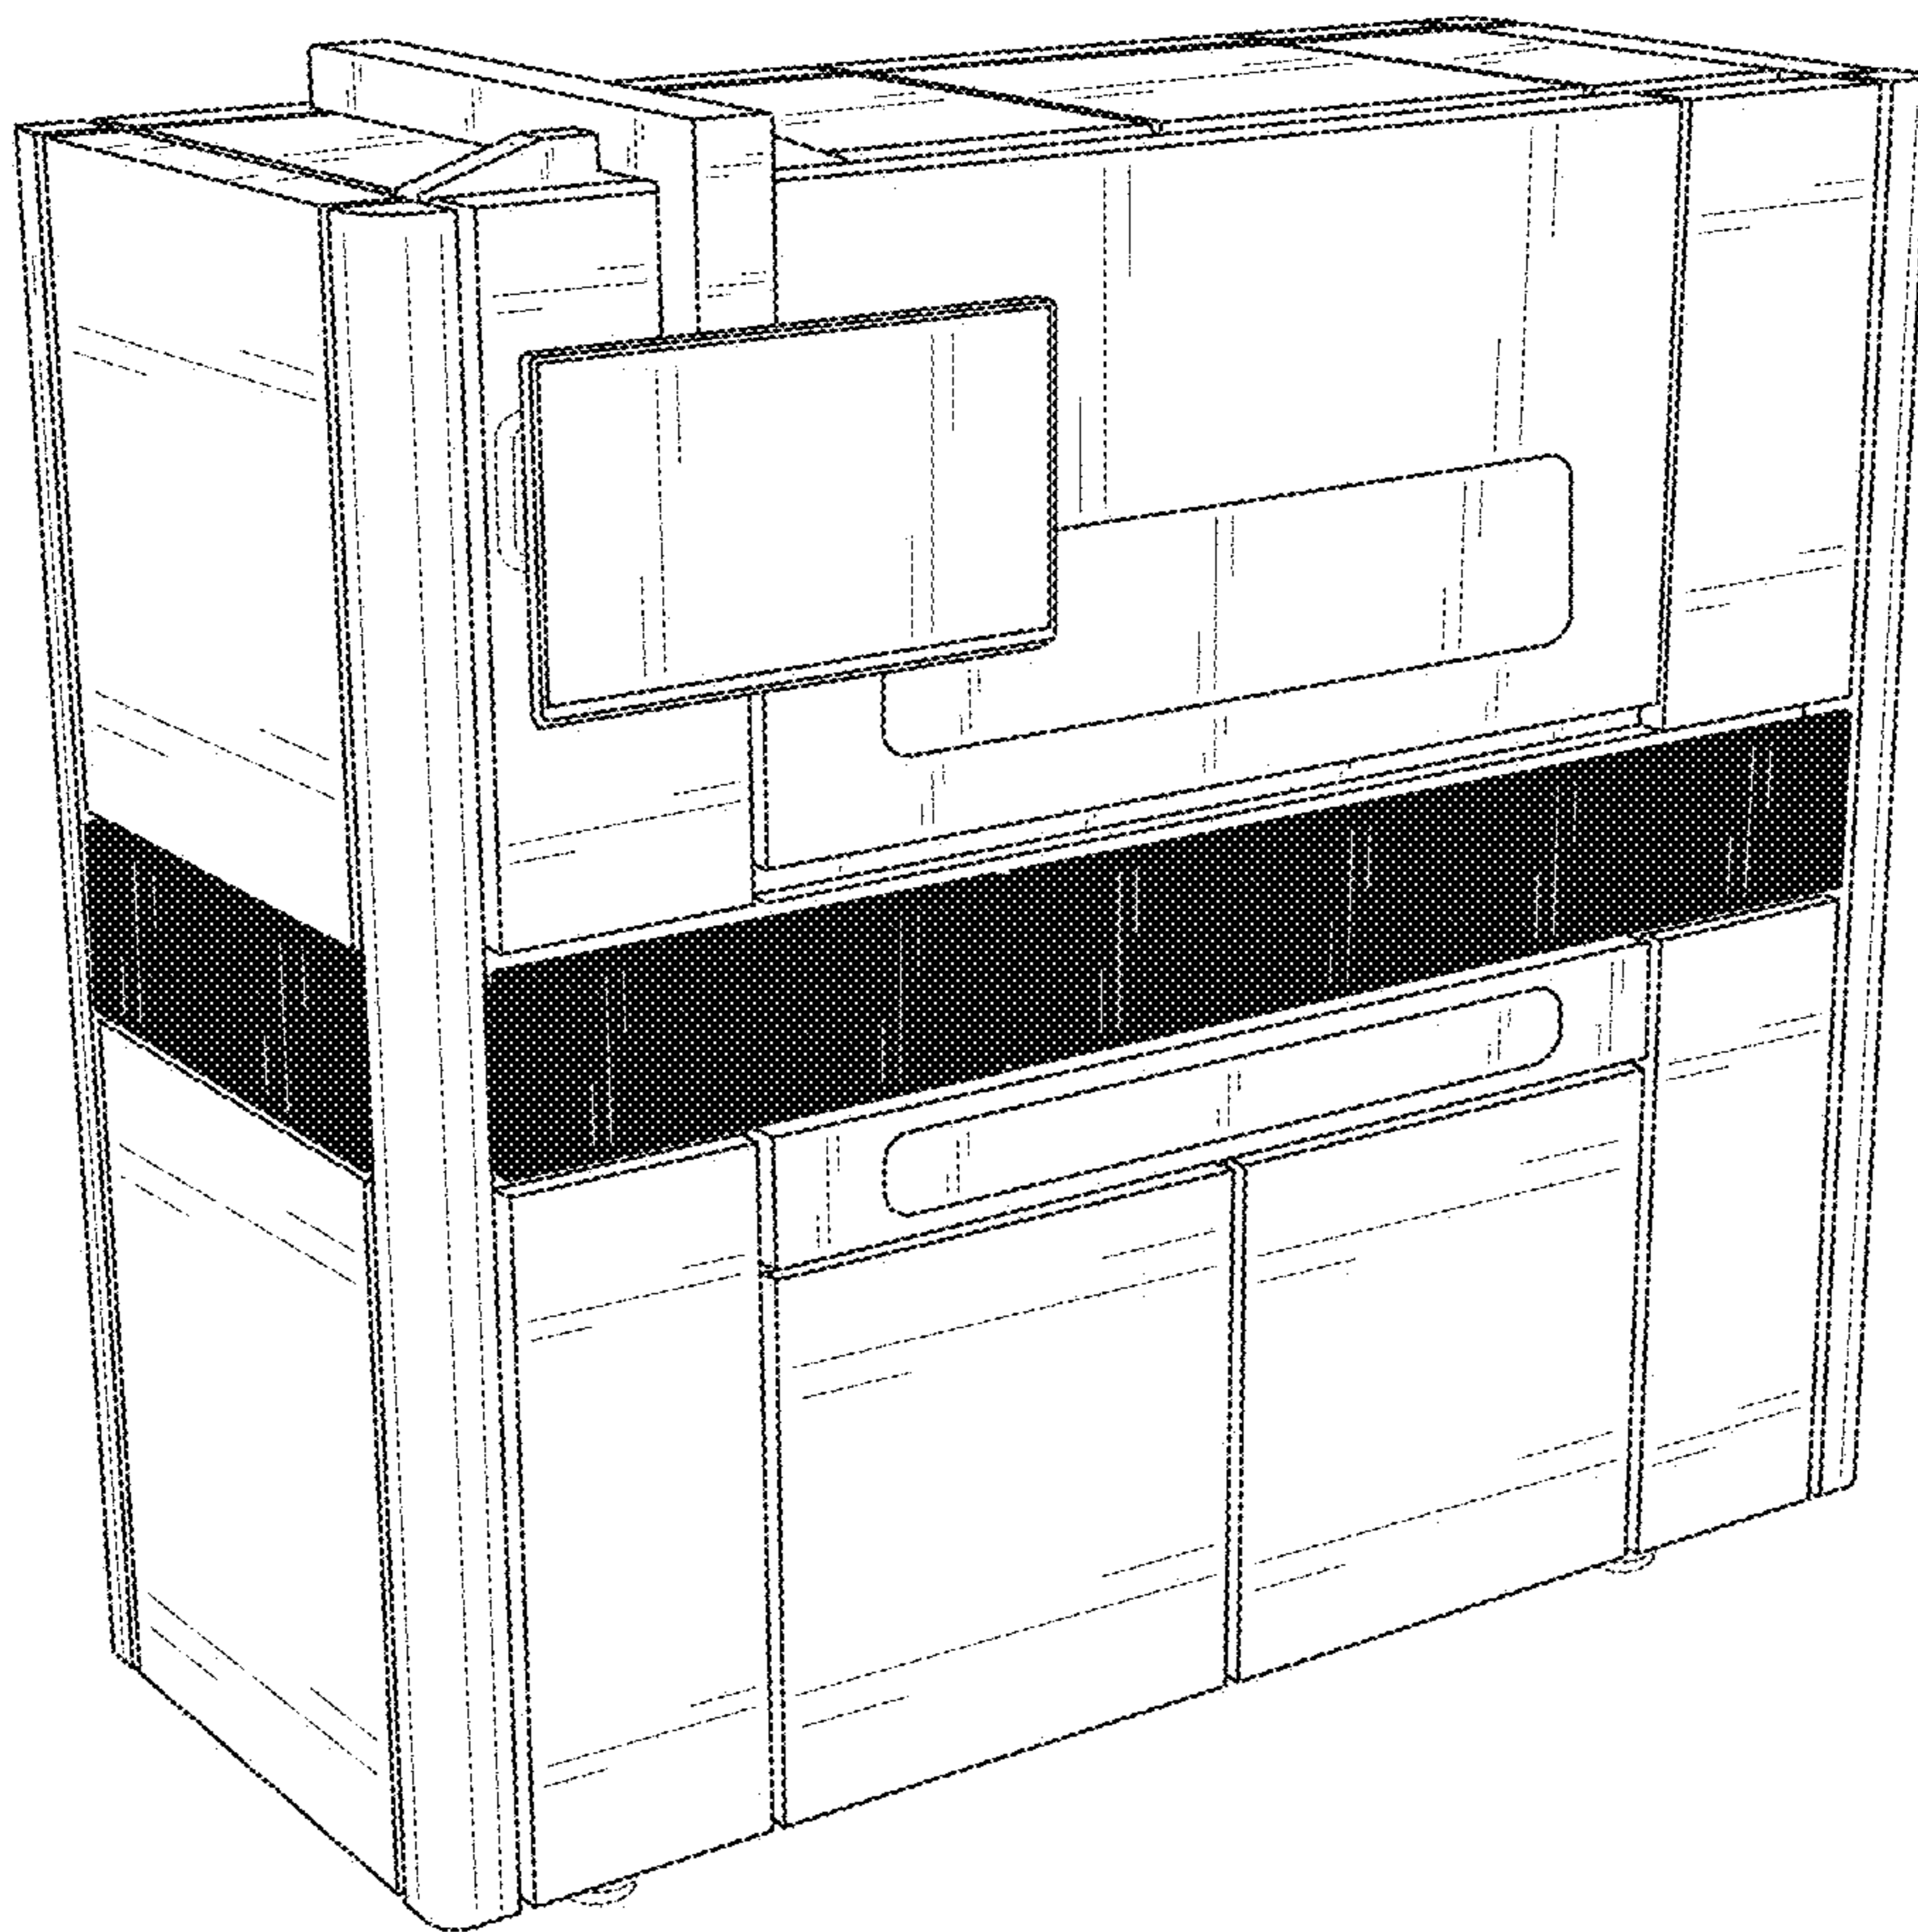


FIG. 25