



US00D981569S

(12) **United States Design Patent** (10) **Patent No.:** **US D981,569 S**  
**Burgess et al.** (45) **Date of Patent:** **\*\* Mar. 21, 2023**

(54) **HOSPITAL POLE, BRACKET ARM AND CONNECTOR ASSEMBLY**

(71) Applicant: **Fisher & Paykel Healthcare Limited**, Auckland (NZ)

(72) Inventors: **Aidan Robert Burgess**, Auckland (NZ); **Shane Terry Massey**, Auckland (NZ); **Taylor James Edwards**, Auckland (NZ); **Craig Karl White**, Auckland (NZ)

(73) Assignee: **Fisher & Paykel Healthcare Limited**, Auckland (NZ)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/736,383**

(22) Filed: **May 29, 2020**

**Related U.S. Application Data**

(62) Division of application No. 29/697,966, filed on Jul. 12, 2019, now Pat. No. Des. 889,643, which is a division of application No. 29/605,819, filed on May 30, 2017, now Pat. No. Des. 860,438.

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/185**

(58) **Field of Classification Search**  
USPC ..... D8/355, 353, 356, 366, 371, 373, 380, D8/381; D13/154; D14/140.6, 452, 239; D24/127, 128, 234, 231, 186, 185  
CPC ..... B62B 3/1476; B62B 3/16; B62B 3/1472; B62B 3/12; B62B 3/005; B62B 2202/30; B62B 2203/07; B62B 5/067; B62B 5/002

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D255,718 S 7/1980 Hunt  
D357,406 S 4/1995 Whitaker  
D357,922 S 5/1995 Nysether et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO 2018/195154 10/2018

OTHER PUBLICATIONS

PSY121—Flat Screen Monitor Support Bracket with Articulating Arm , Thorlabs.com, [Post Date: unknown], [Site seen Mar. 7, 2022], Seen at URL: <https://www.thorlabs.com/thorproduct.cfm?partnumber=PSY121> (Year: 2022).\*

(Continued)

*Primary Examiner* — Natasha Vujcic  
*Assistant Examiner* — Gilbert B Ford

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **CLAIM**

The ornamental design for a hospital pole, bracket arm and connector assembly, as shown and described.

**DESCRIPTION**


FIG. 1 is a perspective view of the hospital pole, bracket arm and connector assembly showing a first embodiment of our design.

FIG. 2 is a perspective view of the hospital pole, bracket arm and connector assembly showing a second embodiment of our design; and,

FIG. 3 is a perspective view of the hospital pole, bracket arm and connector assembly showing a third embodiment of our design.

The broken lines in the drawings illustrate the environment of the hospital pole bracket arm, and connector assembly which forms no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

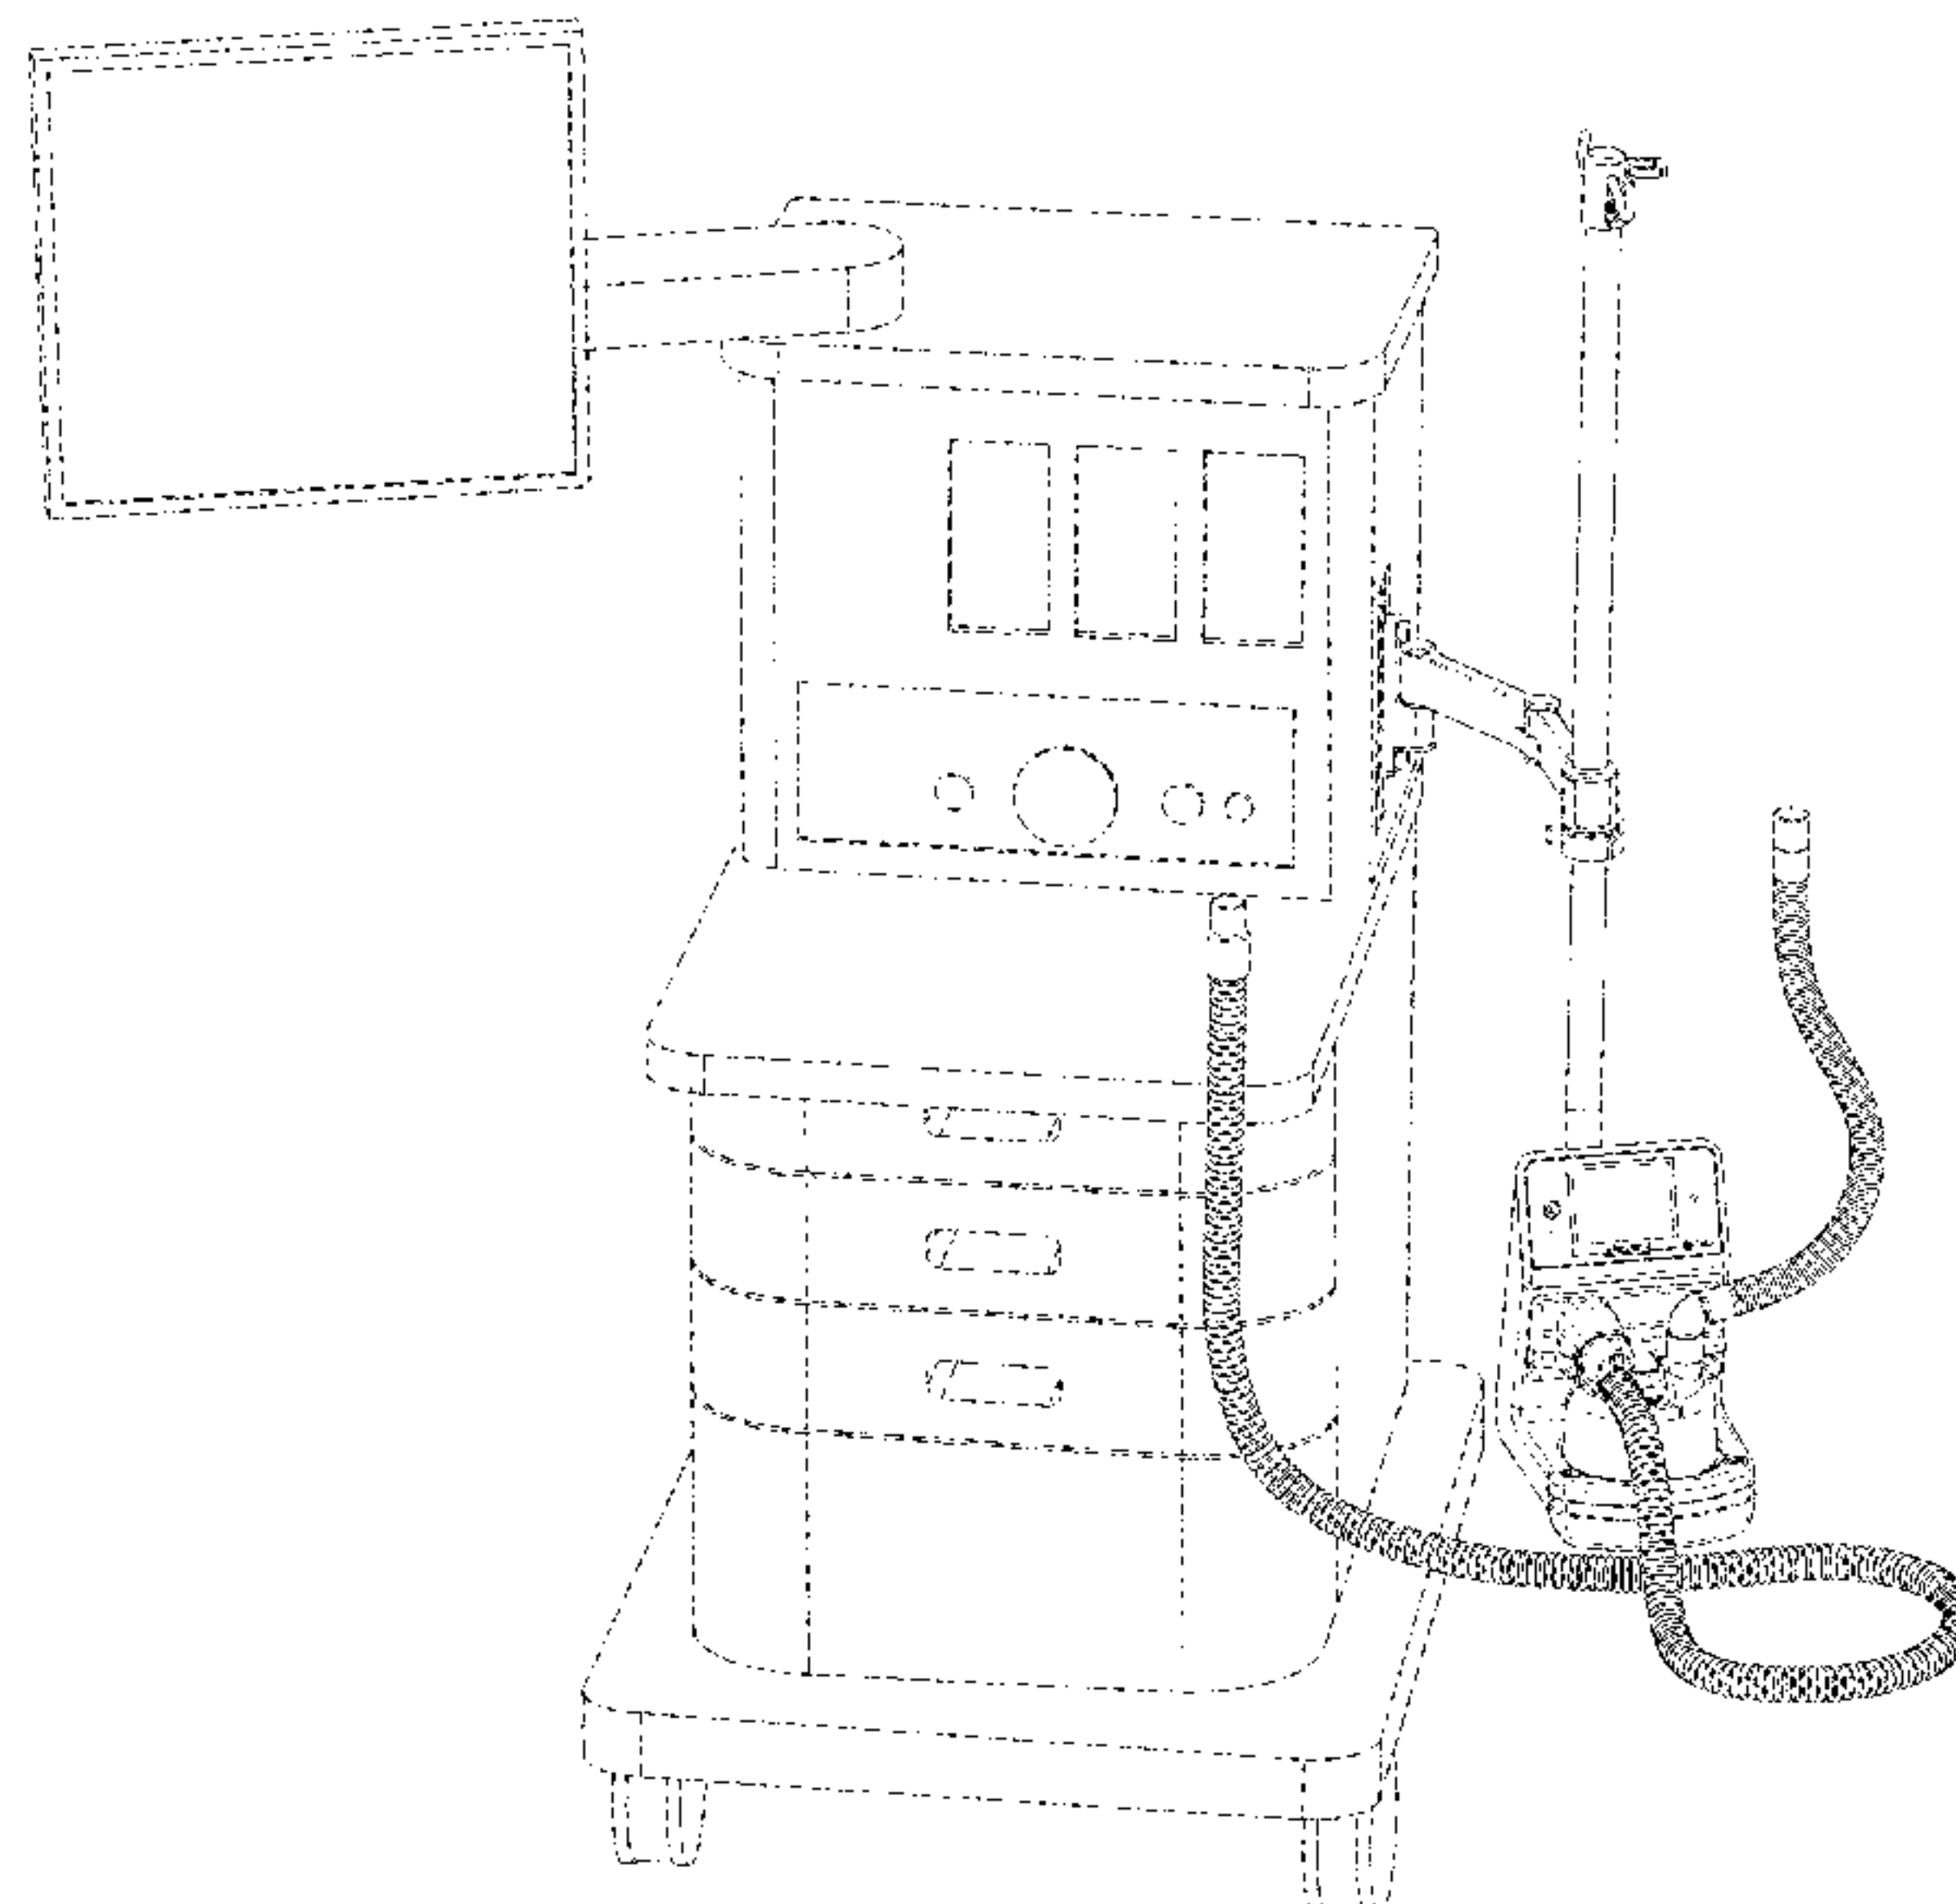

(56)

References Cited

U.S. PATENT DOCUMENTS

D462,893 S 9/2002 Sung  
 D491,574 S 6/2004 Hung  
 D496,367 S \* 9/2004 Pfister ..... D14/451  
 D507,477 S \* 7/2005 Pfister ..... D14/451  
 D537,014 S \* 2/2007 Tait ..... D11/183  
 D537,323 S \* 2/2007 Saez ..... D14/452  
 D540,658 S \* 4/2007 Worrall ..... D8/363  
 7,364,127 B2 4/2008 Huang  
 D611,802 S \* 3/2010 Li ..... D8/363  
 D632,301 S 2/2011 Kasuga et al.  
 D634,016 S \* 3/2011 Schon ..... D24/186  
 D649,535 S 11/2011 Lau et al.  
 D652,521 S \* 1/2012 Ross ..... D24/185  
 D657,469 S \* 4/2012 Vilas ..... D24/185  
 D671,820 S \* 12/2012 Henderson ..... D8/373  
 8,459,602 B2 6/2013 Herskovic  
 D707,360 S \* 6/2014 Kim ..... D24/185  
 D708,334 S \* 7/2014 Kim ..... D24/185  
 D724,736 S \* 3/2015 Kim ..... D24/185  
 D742,206 S 11/2015 Bowman et al.  
 D743,558 S \* 11/2015 Kim ..... D24/186  
 D744,321 S \* 12/2015 Boynton ..... D8/363  
 9,278,040 B2 \* 3/2016 Hung ..... G06F 3/01  
 9,746,130 B2 8/2017 Hung  
 9,755,375 B2 9/2017 Xiang et al.  
 9,890,899 B2 2/2018 Theis et al.  
 D837,039 S \* 1/2019 Angus ..... D8/356  
 D860,438 S 9/2019 Burgess et al.  
 D870,548 S 12/2019 Modracek  
 D874,449 S \* 2/2020 Ahrens ..... D14/239  
 D875,951 S \* 2/2020 Kent ..... D24/185  
 D889,643 S \* 7/2020 Burgess ..... D24/128  
 D917,701 S \* 4/2021 Chai ..... D24/186  
 D920,988 S \* 6/2021 Shu ..... D14/452  
 D922,332 S \* 6/2021 Medhin ..... D13/154

D922,394 S \* 6/2021 Lu ..... D14/452  
 D930,633 S \* 9/2021 Xu ..... D14/239  
 D932,629 S \* 10/2021 Ruff ..... D24/185  
 D932,630 S \* 10/2021 Ruff ..... D24/185  
 D932,631 S \* 10/2021 Ruff ..... D24/185  
 D933,460 S \* 10/2021 Jin ..... D8/363  
 D940,879 S \* 1/2022 Ryu ..... D24/185  
 11,230,312 B2 \* 1/2022 Kaushansky ..... B62B 3/02

OTHER PUBLICATIONS

Pole/Pipe Mounting Bracket ( PA-32 ), Modernsolid.com, [Post date: Jan. 28, 2019], [Site seen Mar. 7, 2022], Seen at URL: <https://www.modernsolid.com/PA-32-Pole-Pipe-Mounting-Bracket.htm> (Year: 2019).\*

Fisher & Paykel 900MR303 Mounting Bracket, Fisher & Paykel, [Post Date Unknown], [Site seen Mar. 7, 2022], Seen at URL: <https://www.estatedmedical.com/products/fisher-paykel-900mr303-mounting-bracket-1-ea.html> (Year: 2022).\*

CH-1003, posted unknown, [retrieved May 17, 2018]. Retrieved from Internet, <URL: <https://www.hatchmed.com/ivtow-1/>>.

Home > Ergonomic Products > Monitor Arms > Glide Monitor Arm, posted unknown, [retrieved May 17, 2018]. Retrieved from Internet, <URL: [https://www.genesys-uk.com/Glide-Monitor-Arm.Html?cPath-9\\_13](https://www.genesys-uk.com/Glide-Monitor-Arm.Html?cPath-9_13)>.

Humanscale M/Flex Monitor Arm—One Monitor Solution, posted Feb. 18, 2016, [retrieved May 17, 2018]. Retrieved from Internet, <URL: <https://www.thehumansolution.com/humanscale-mflex-monitor-arm.html>>.

Wali Single LCD Monitor Desk Mount Fully Adjustable Stand Fits One Screen up to 27", 22 lbs. Weight Capacity (M001), Black, posted Nov. 27, 2015, [retrieved May 17, 2018]. Retrieved from Internet, <URL: <https://www.amazon.com/WALK-Single-Monitor-Adjustable-Capacity/dp/B018MT6ZEK>>.

\* cited by examiner

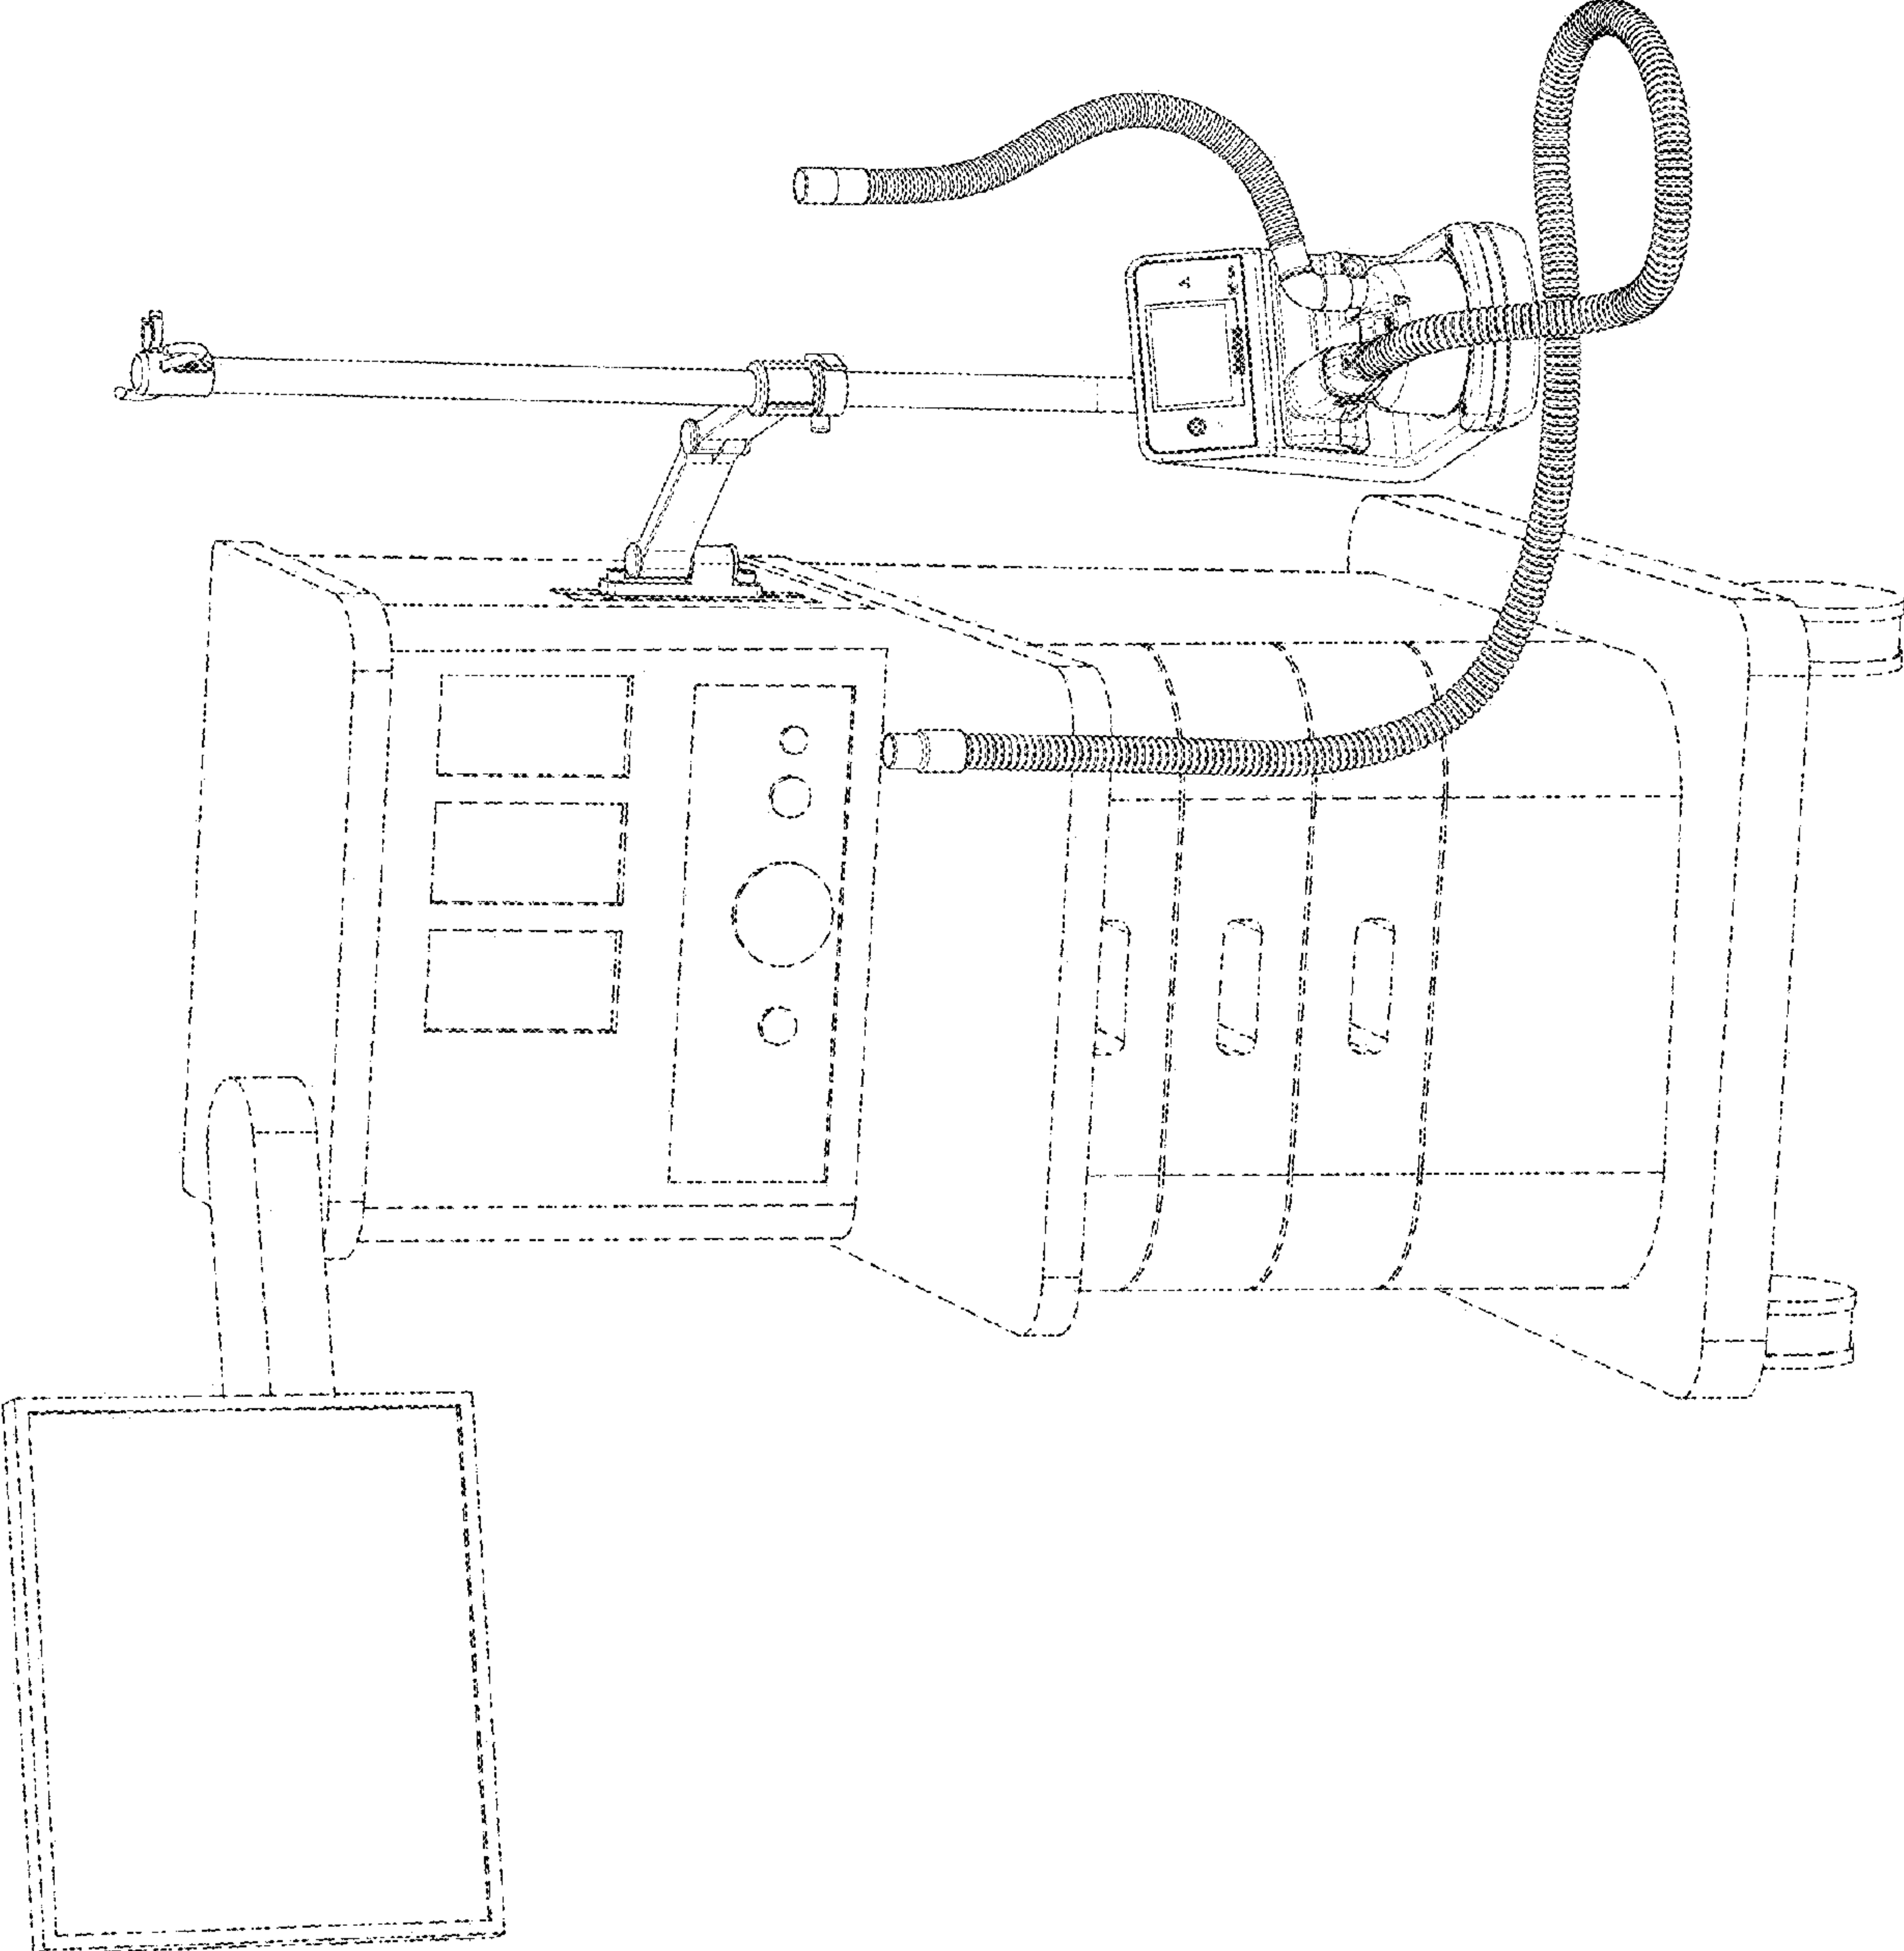


FIG. 1



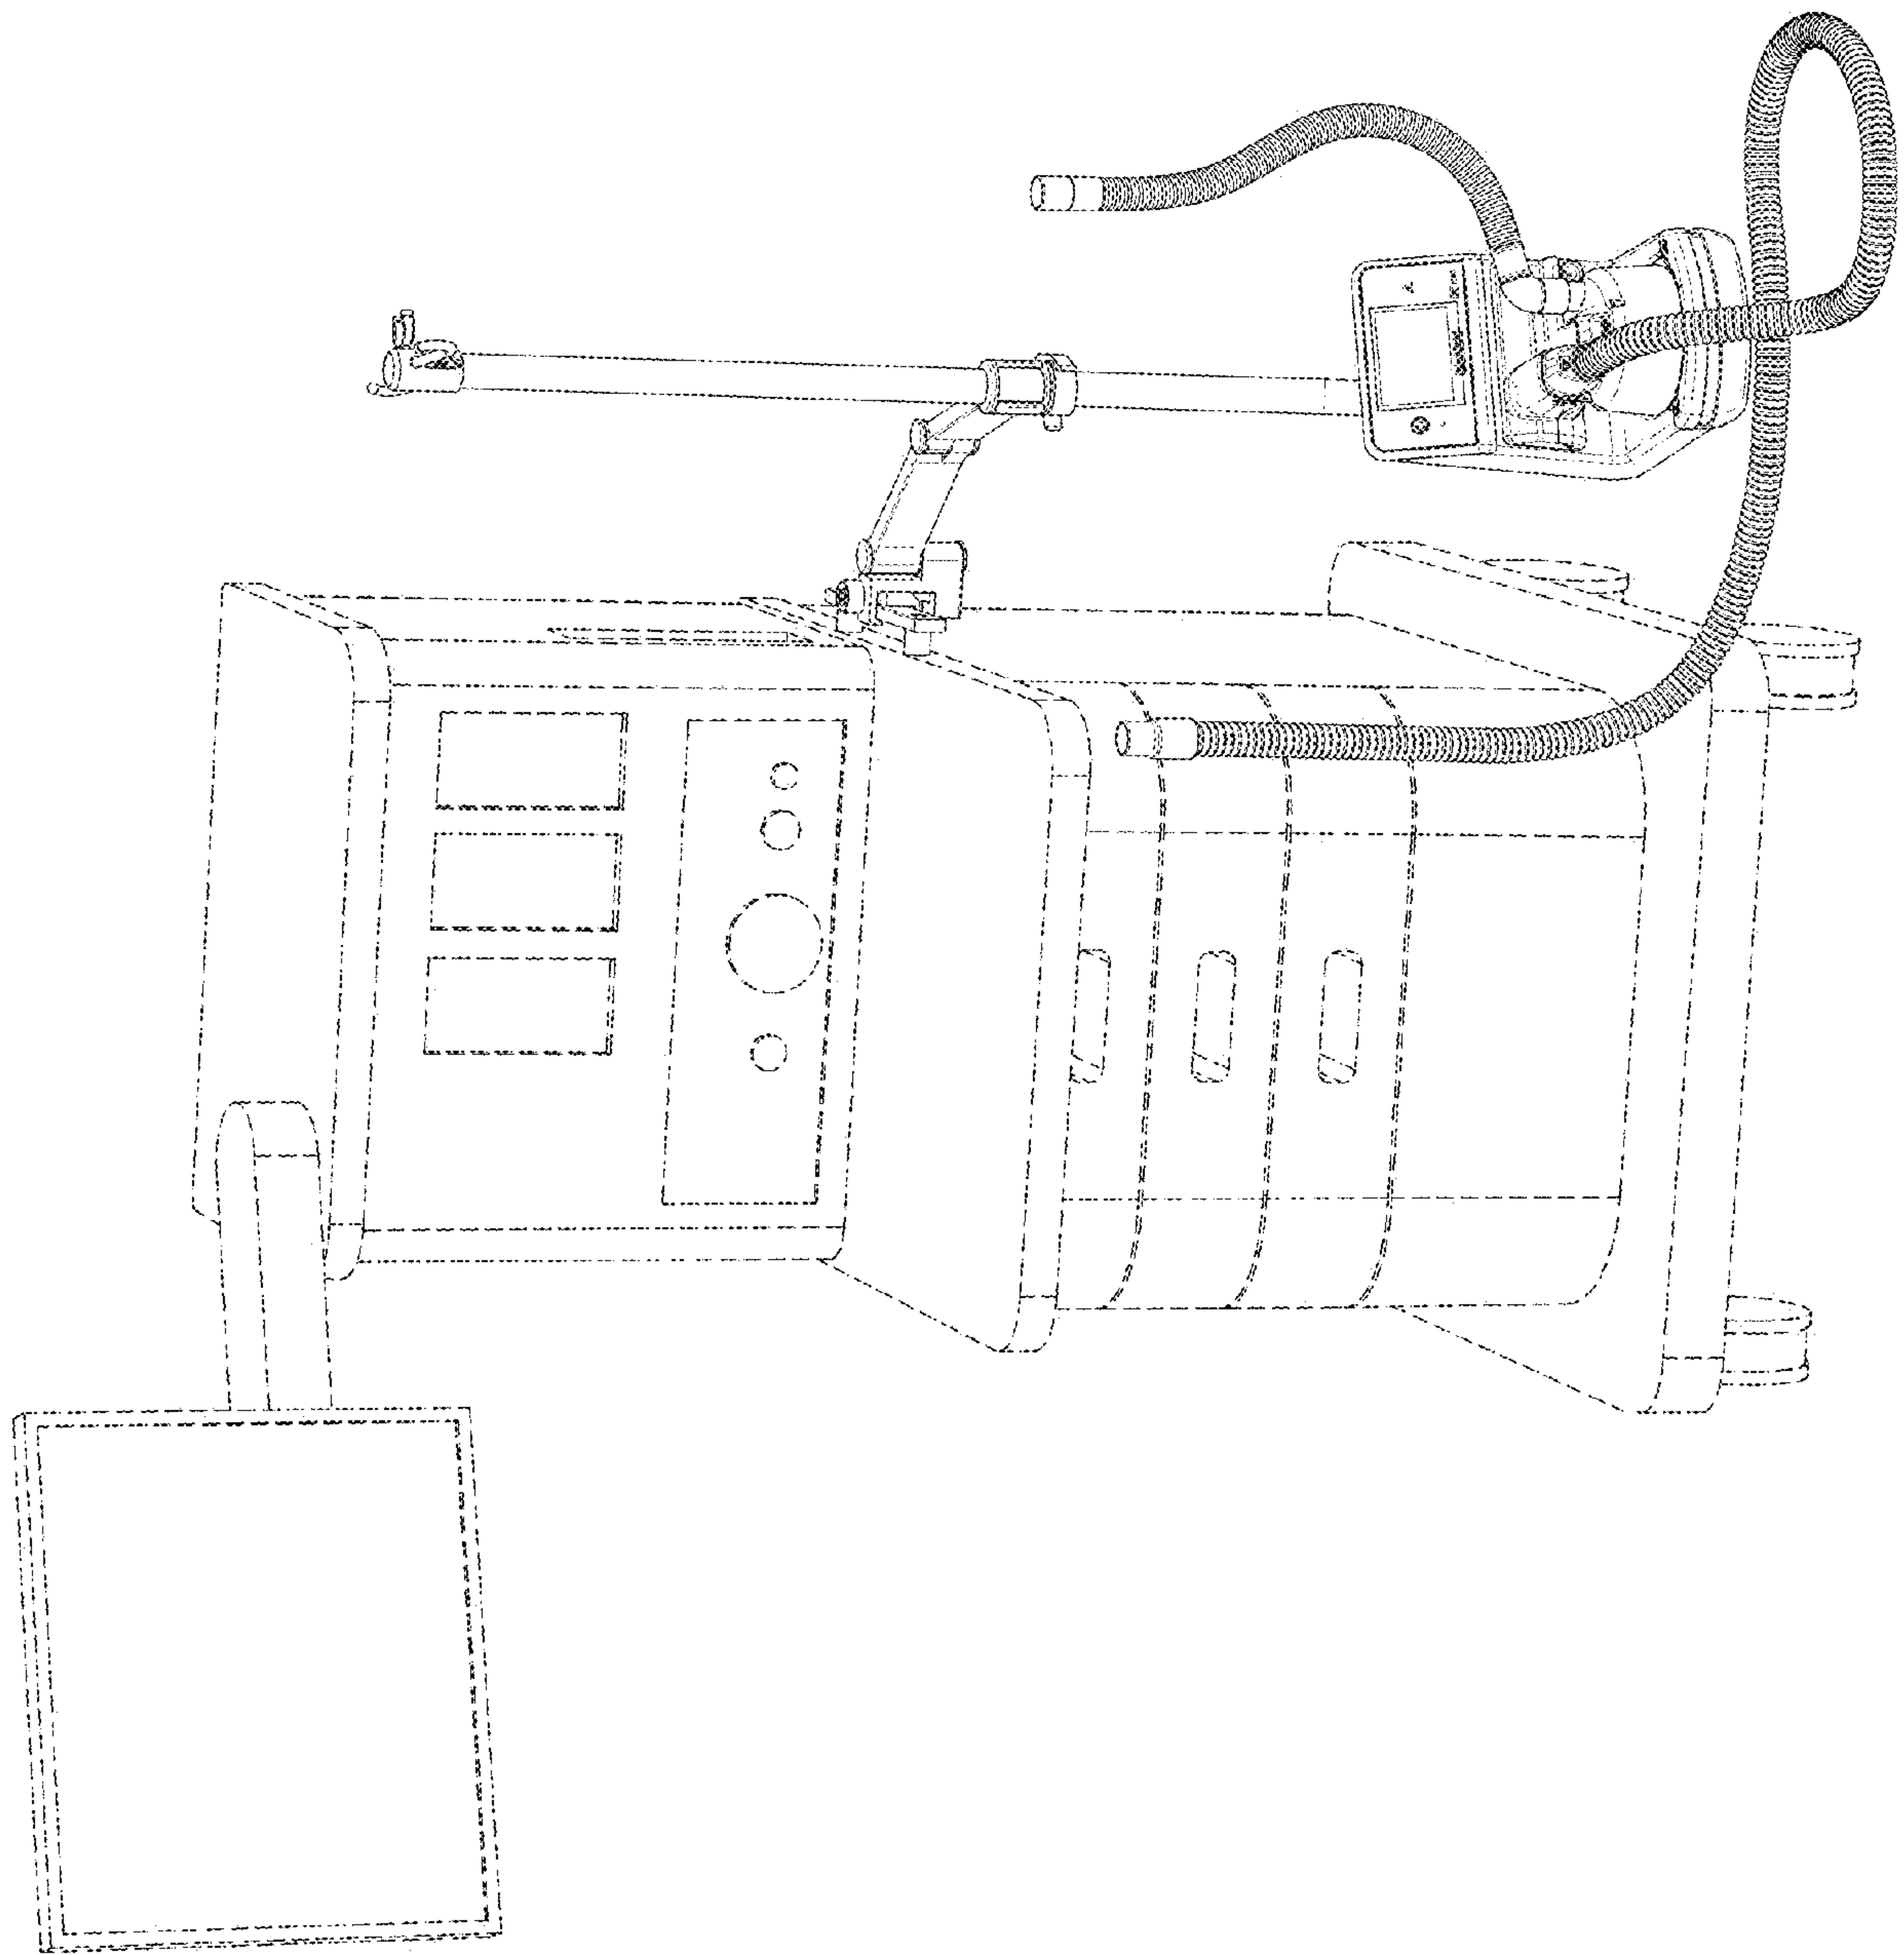


FIG. 2

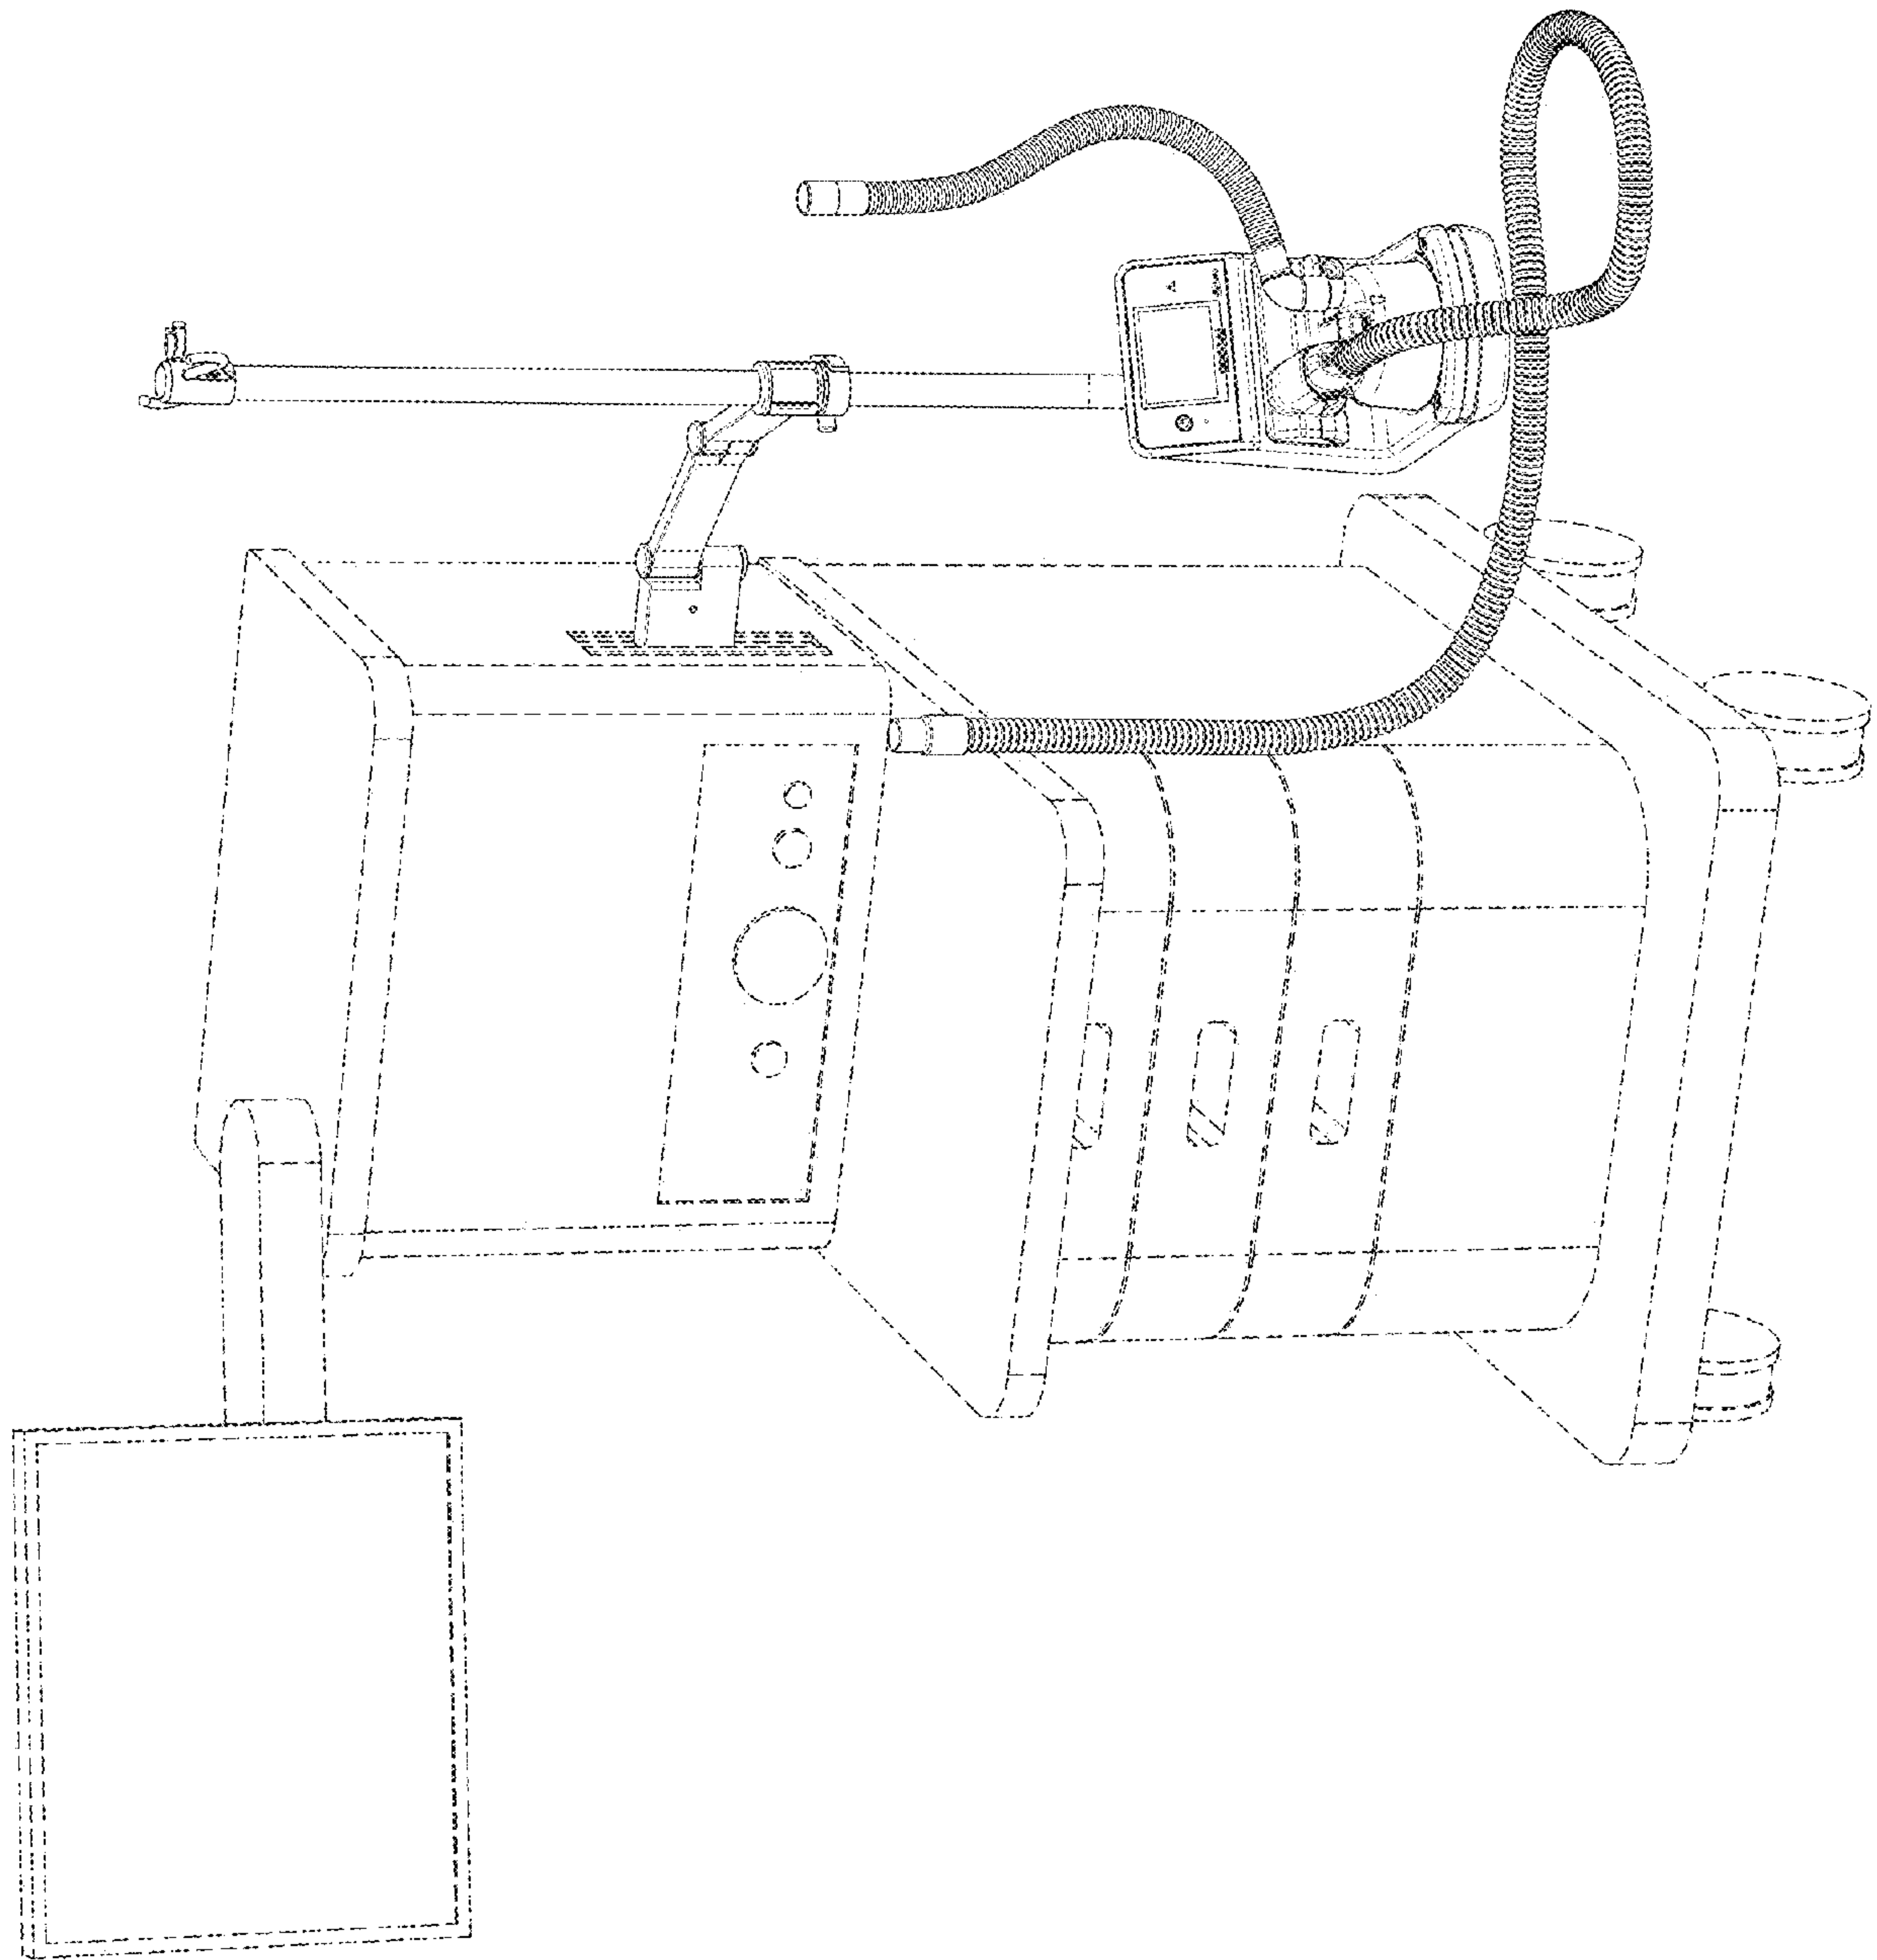


FIG. 3