



US00D982181S

(12) **United States Design Patent** (10) **Patent No.:** **US D982,181 S**
Tanaka (45) **Date of Patent:** **** Mar. 28, 2023**

(54) **MEDICAL BIOCHEMICAL ANALYZER**

(71) Applicant: **FUJIFILM Corporation**, Tokyo (JP)

(72) Inventor: **Kunihiko Tanaka**, Kanagawa (JP)

(73) Assignee: **FUJIFILM Corporation**, Tokyo (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/759,417**

(22) Filed: **Nov. 23, 2020**

(30) **Foreign Application Priority Data**

May 29, 2020 (JP) 2020-010733 D

(51) **LOC (14) Cl.** **24-01**

(52) **U.S. Cl.**

USPC **D24/232**

(58) **Field of Classification Search**

USPC D24/107, 185, 186, 216, 219, 231–234;
D10/81

CPC G01N 2035/00306; G01N 2035/00326;
G01N 2035/00336; G01N 2030/027;
G01N 21/76; G01N 2035/00039; G01N
2035/00049; G01N 35/00029

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,855,847 A * 1/1999 Oonuma G01N 35/02
422/65

D523,153 S * 6/2006 Akashi D10/81

D588,276 S * 3/2009 Isozaki D24/232

D638,545 S * 5/2011 Okawa D24/186

D818,146 S * 5/2018 Tanaka

D874,017 S * 1/2020 Jenoski D24/216

D889,668 S * 7/2020 Chiu D24/185

D890,361 S * 7/2020 Nüesch D24/232

D906,536 S * 12/2020 Kozono D24/216

2008/0216590 A1 * 9/2008 Blanton G01N 35/00029
73/863.11

2008/0268529 A1 * 10/2008 Furusato B01L 3/50851
435/289.1

2013/0288259 A1 * 10/2013 Tajima G01N 35/00732
435/6.12

2014/0073517 A1 * 3/2014 Zhou G01N 35/1002
435/6.12

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC

(57) **CLAIM**

The ornamental design for a medical biochemical analyzer,
as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of a medical biochemical
analyzer, showing the new design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a top view thereof;

FIG. 5 is a bottom view thereof.

FIG. 6 is a right side view thereof;


FIG. 7 is a left side view thereof;

FIG. 8 is a perspective view showing a state thereof in which
a lid is open; and,

FIG. 9 is a left side view showing the state thereof in which
the lid is open.

The broken lines in the drawings depict portions of the
medical biochemical analyzer that form no part of the
claimed design.

1 Claim, 9 Drawing Sheets

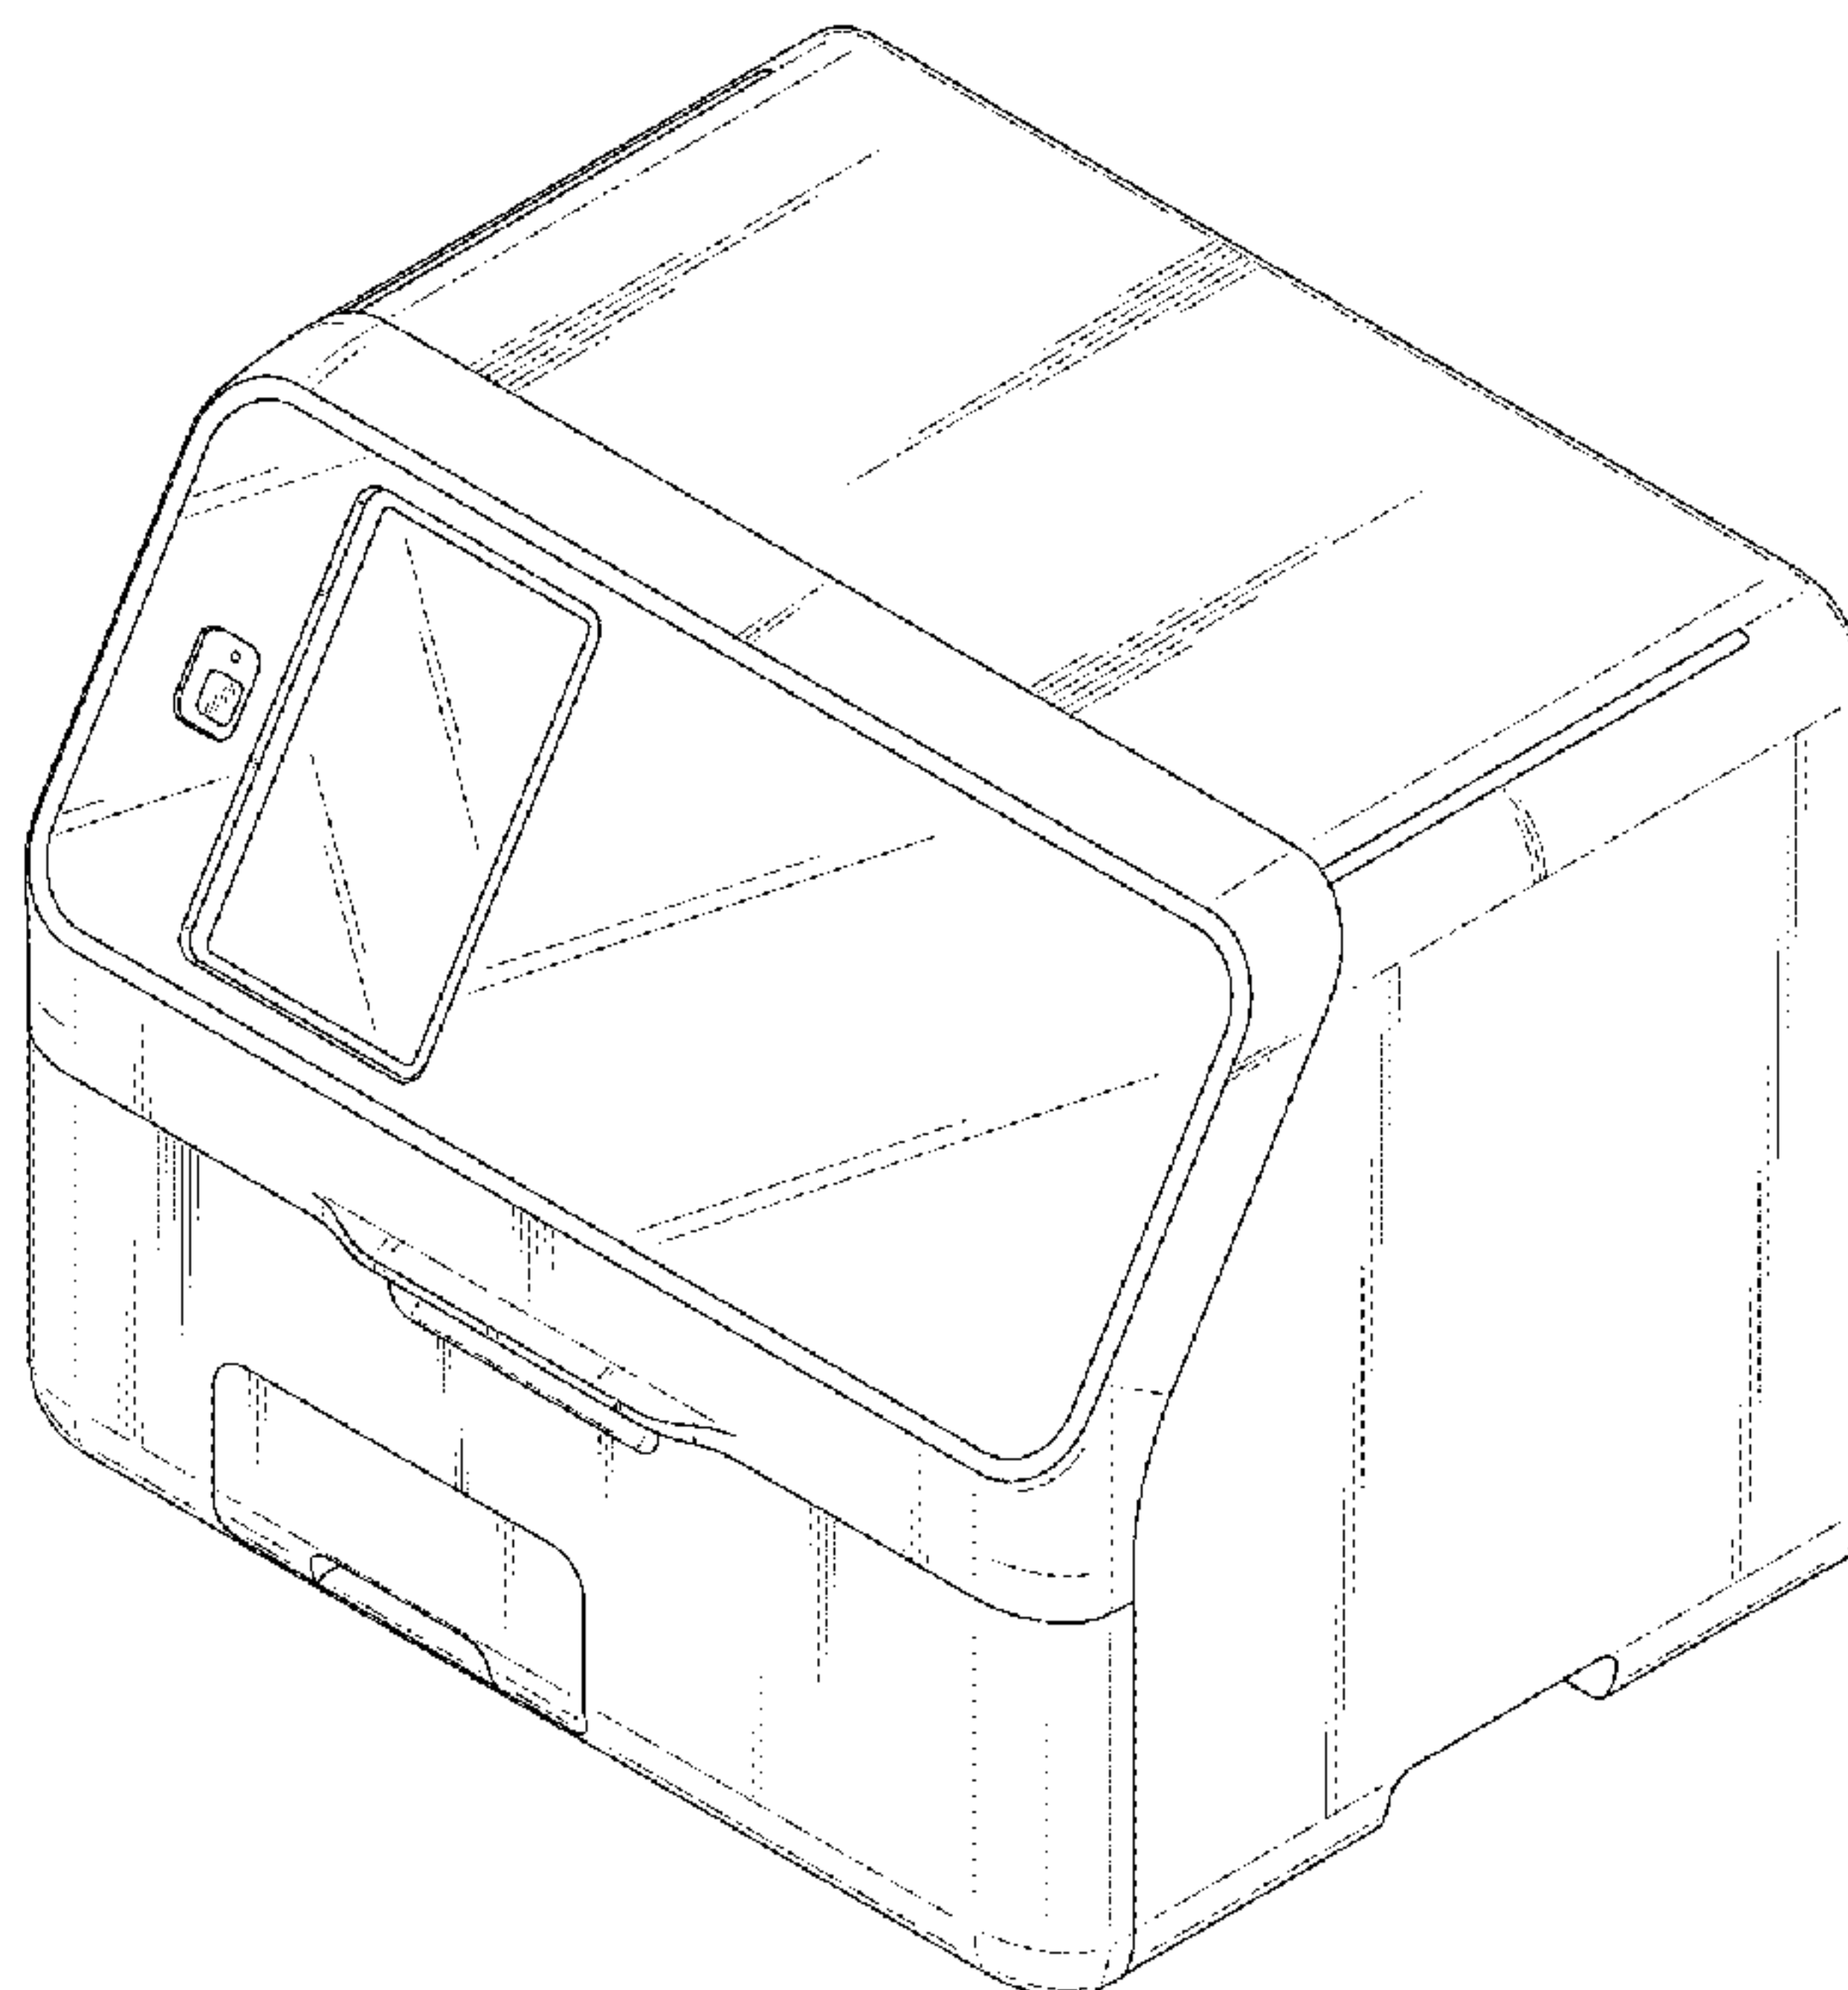

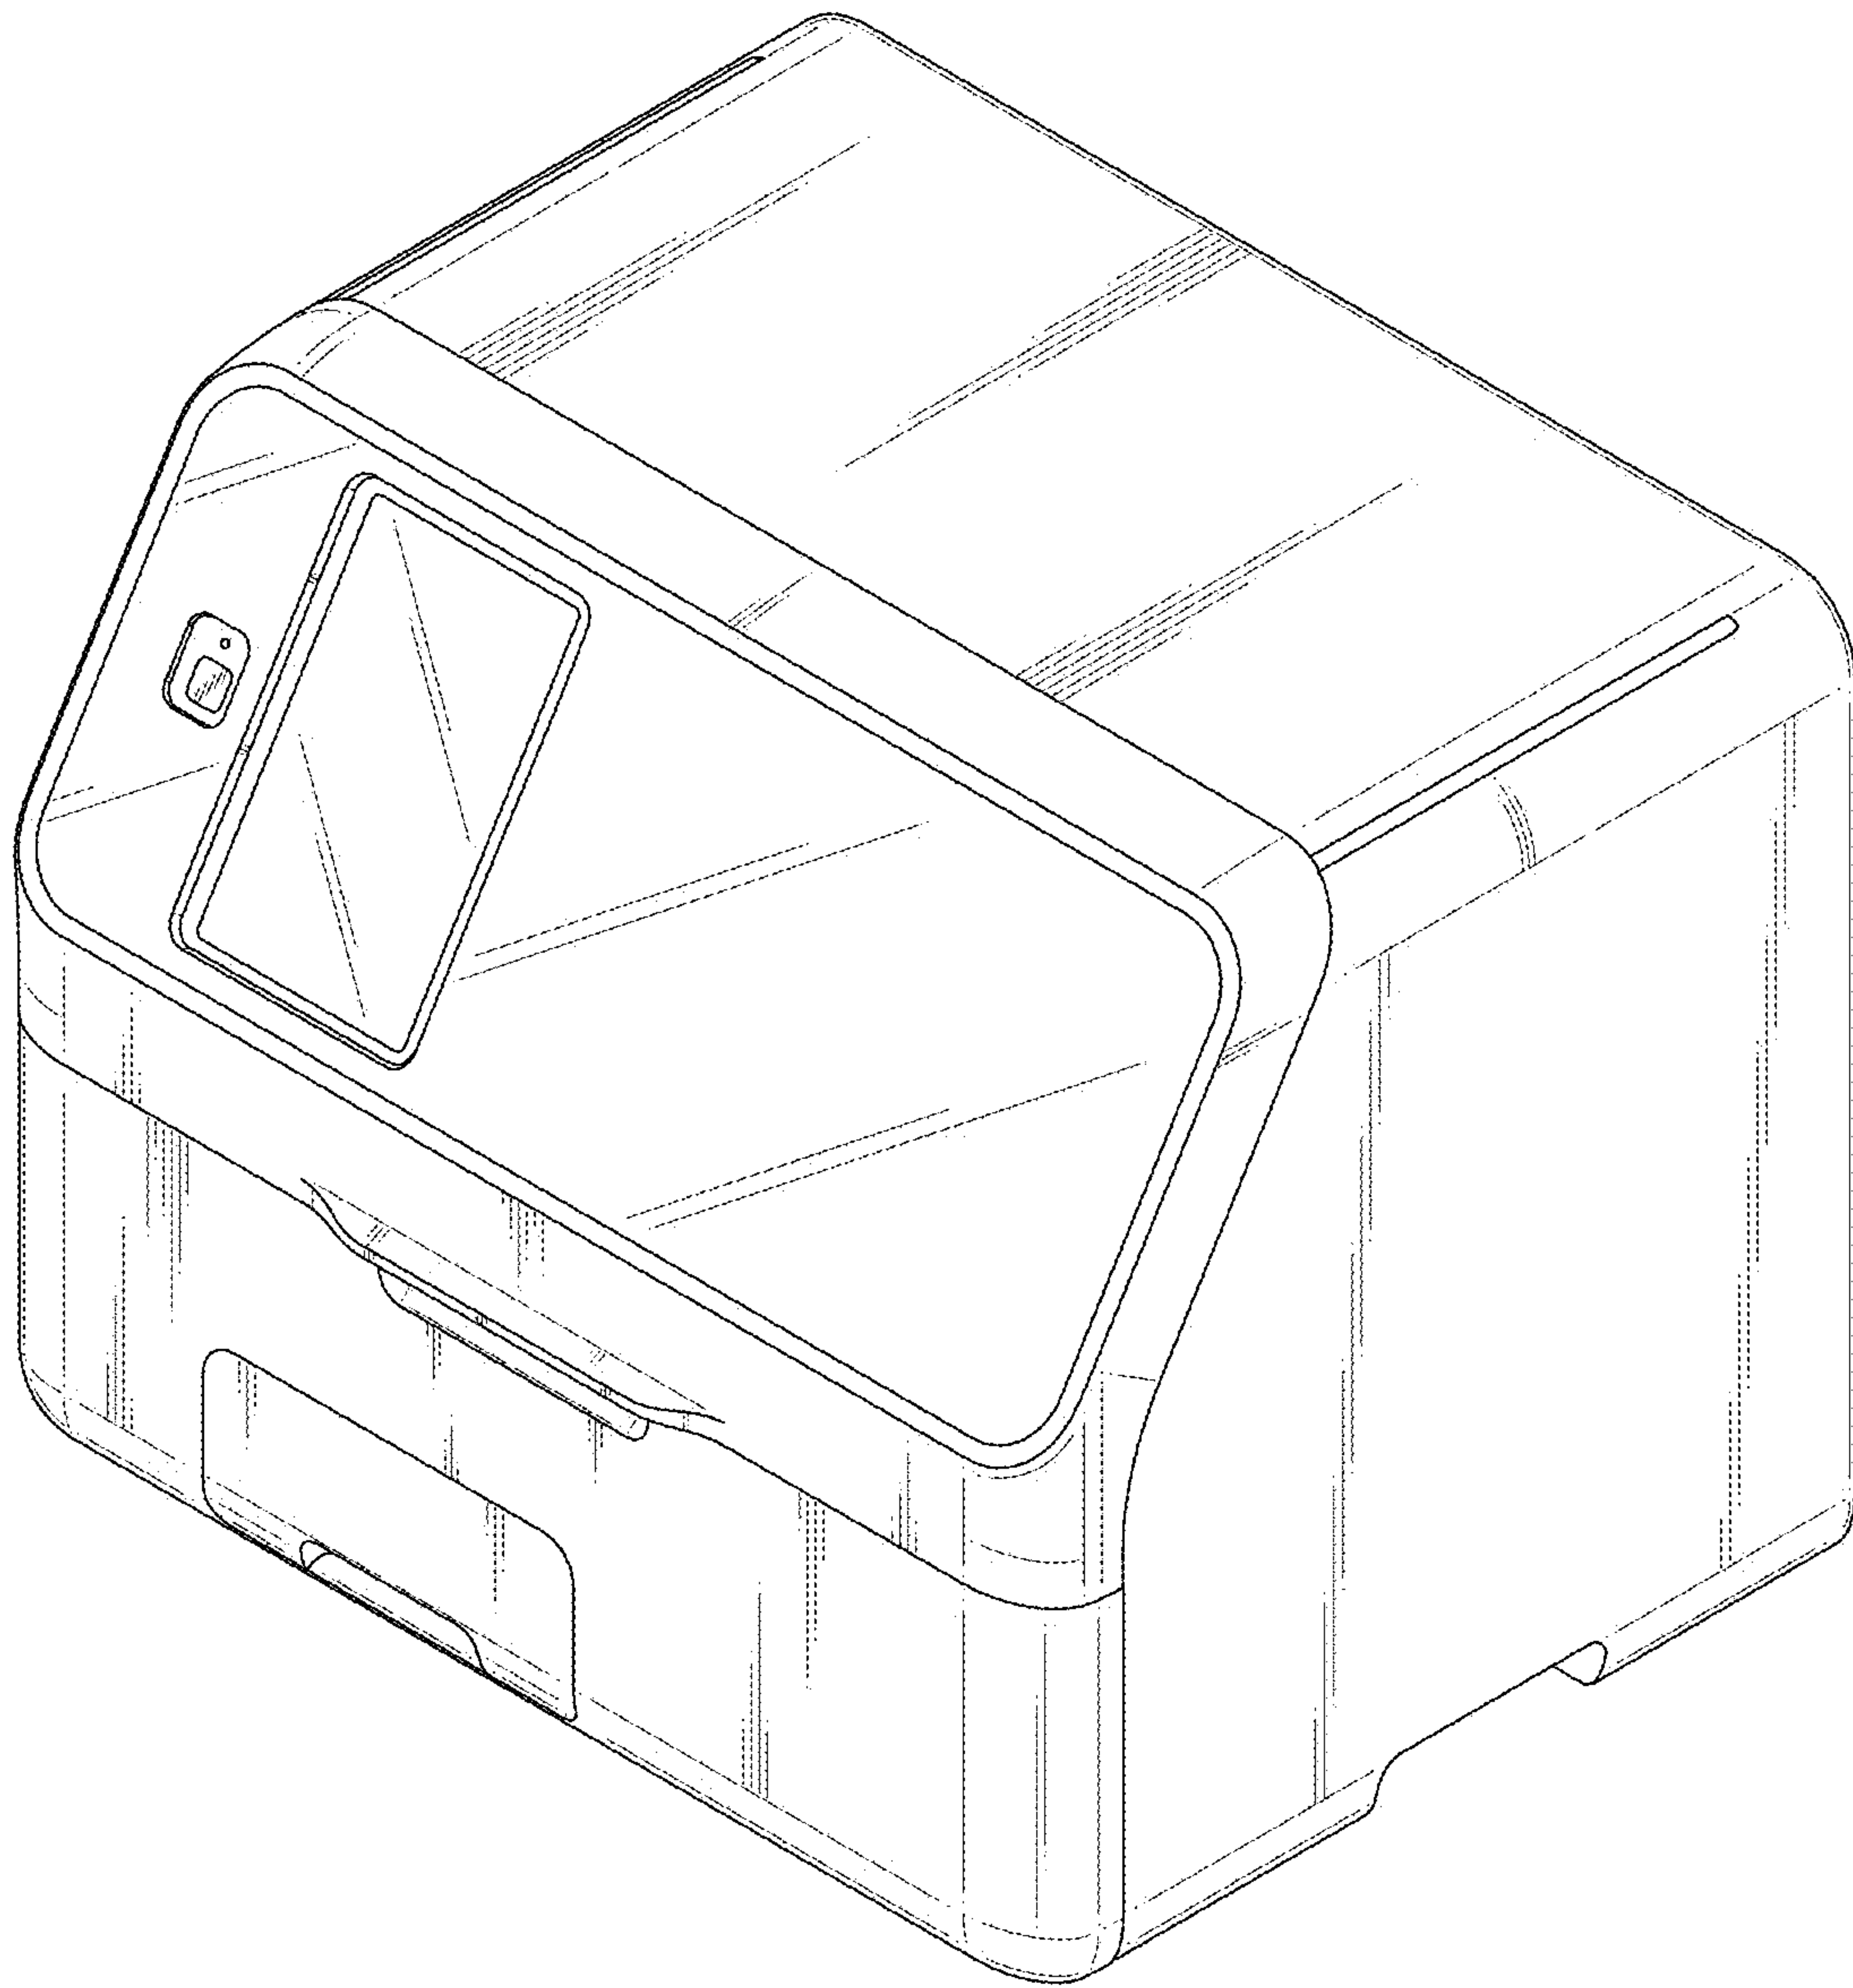


FIG.1

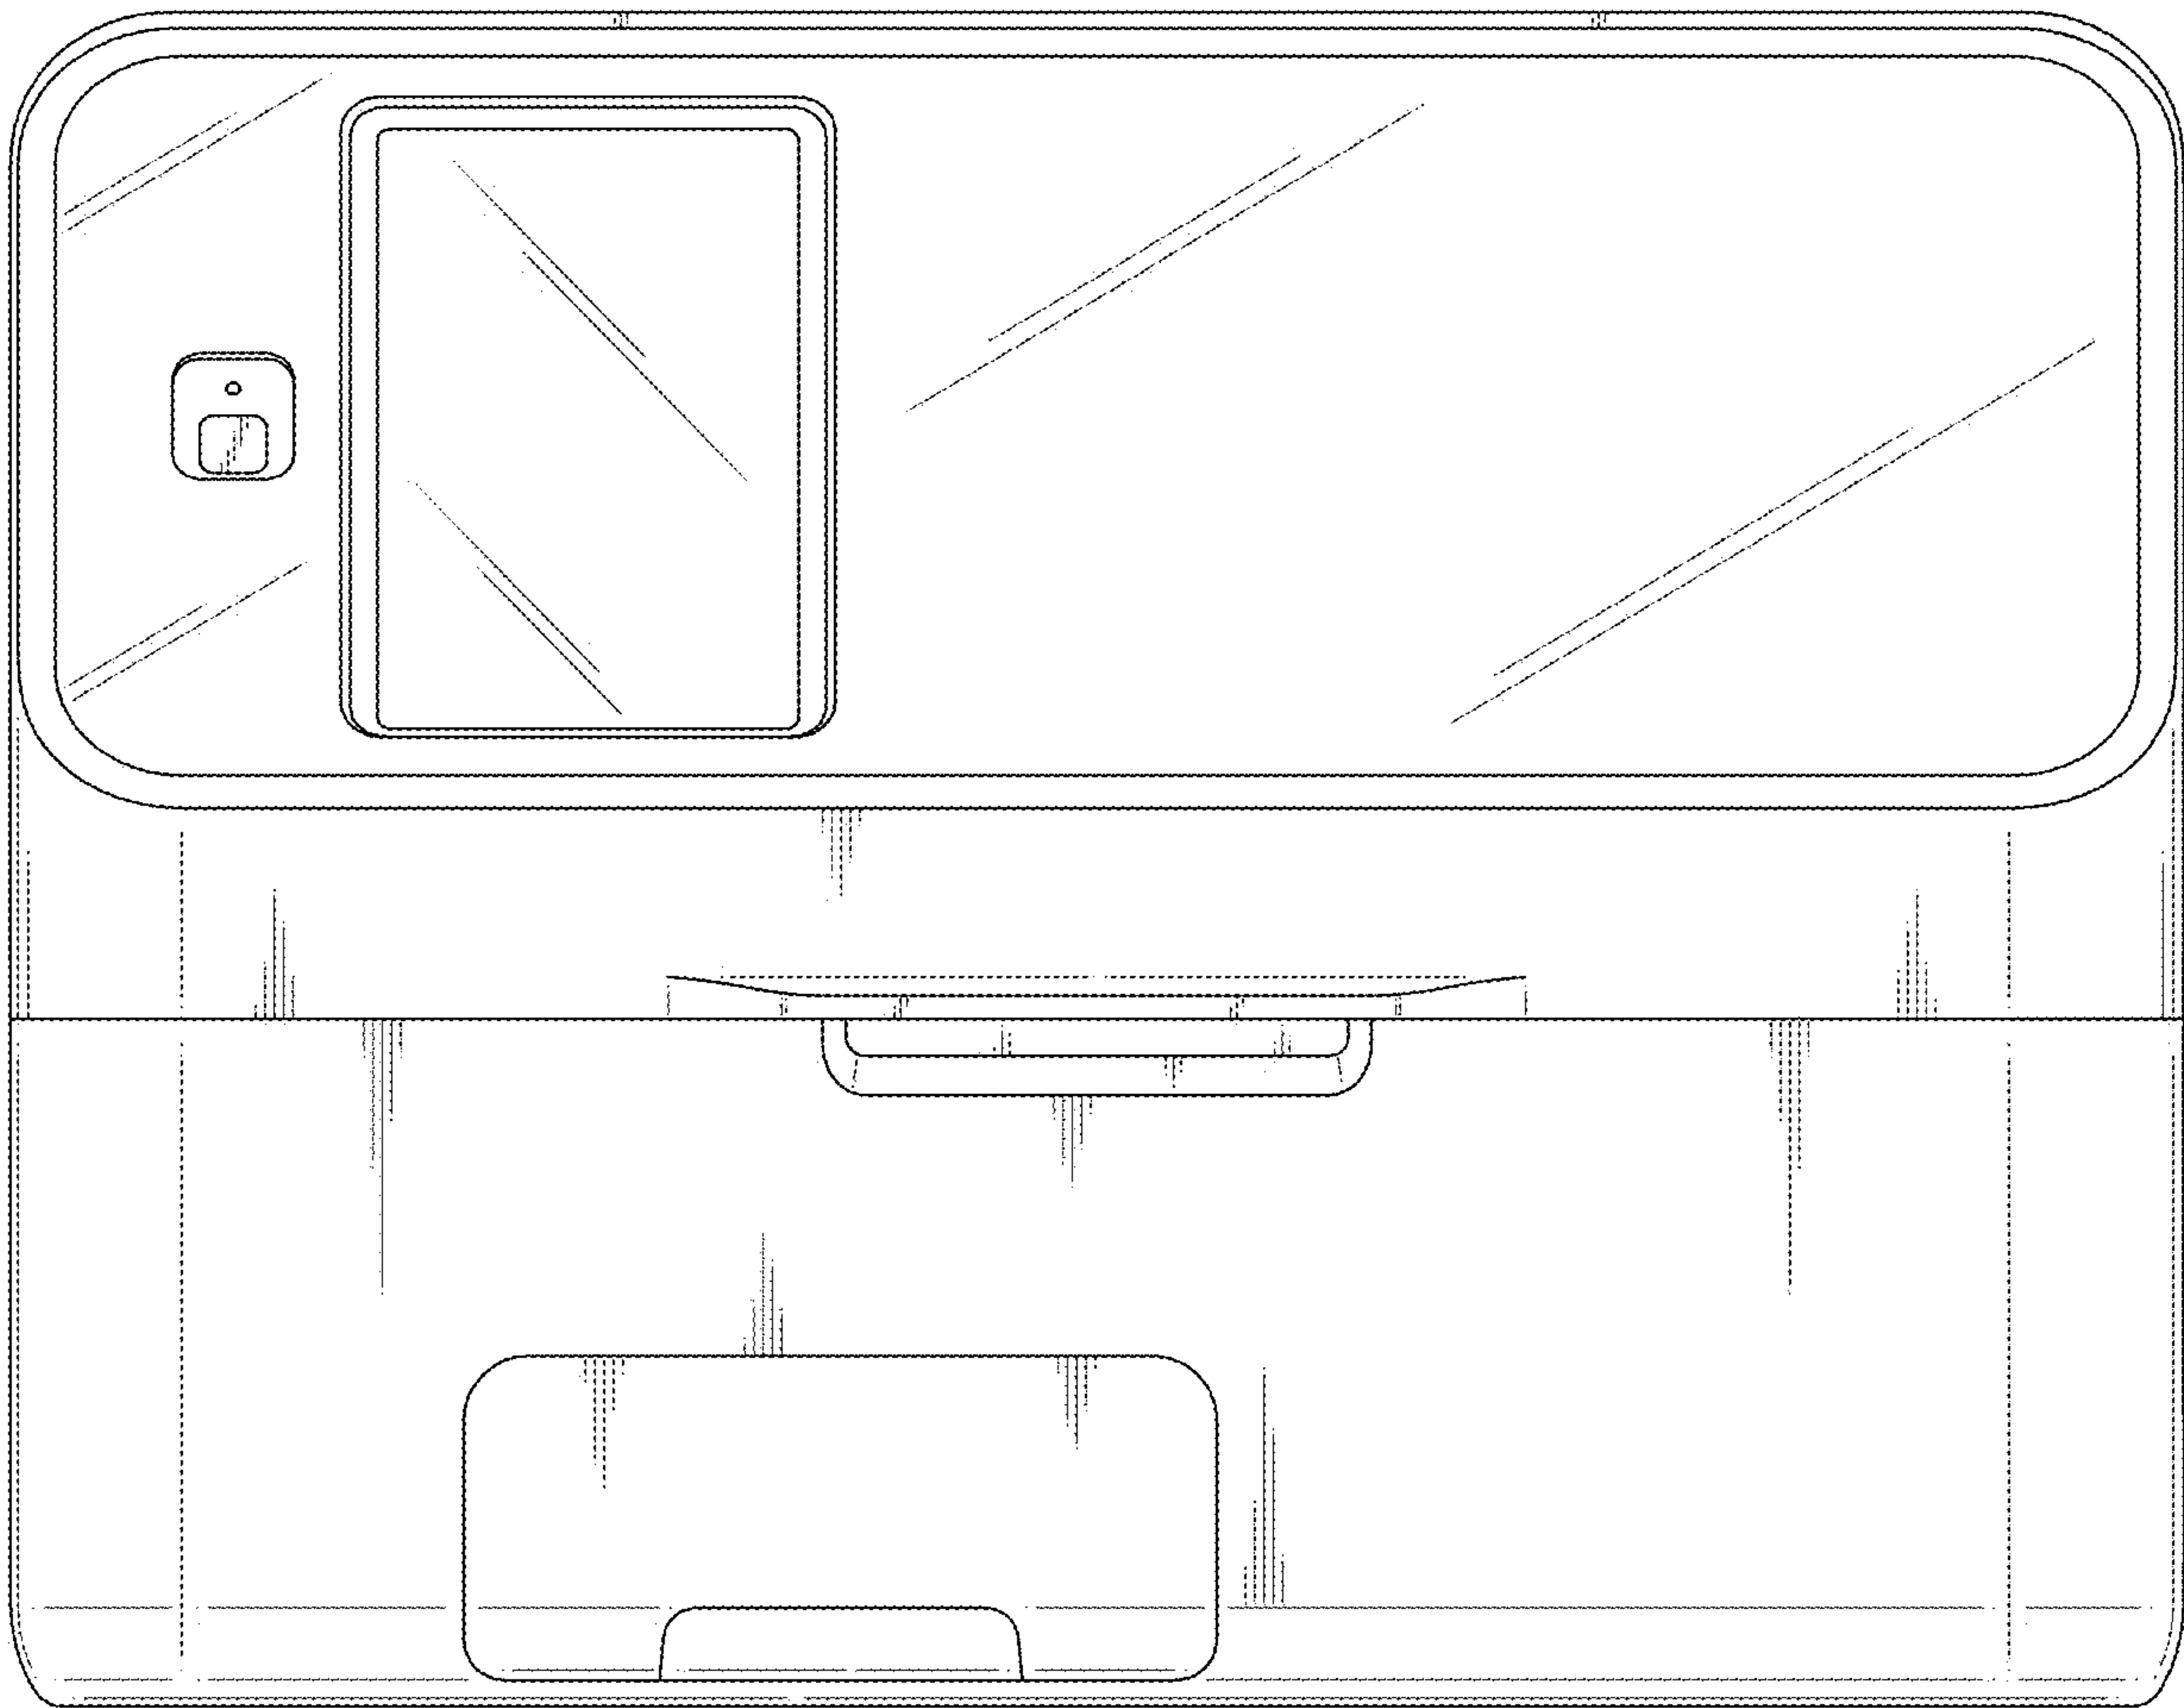


FIG.2

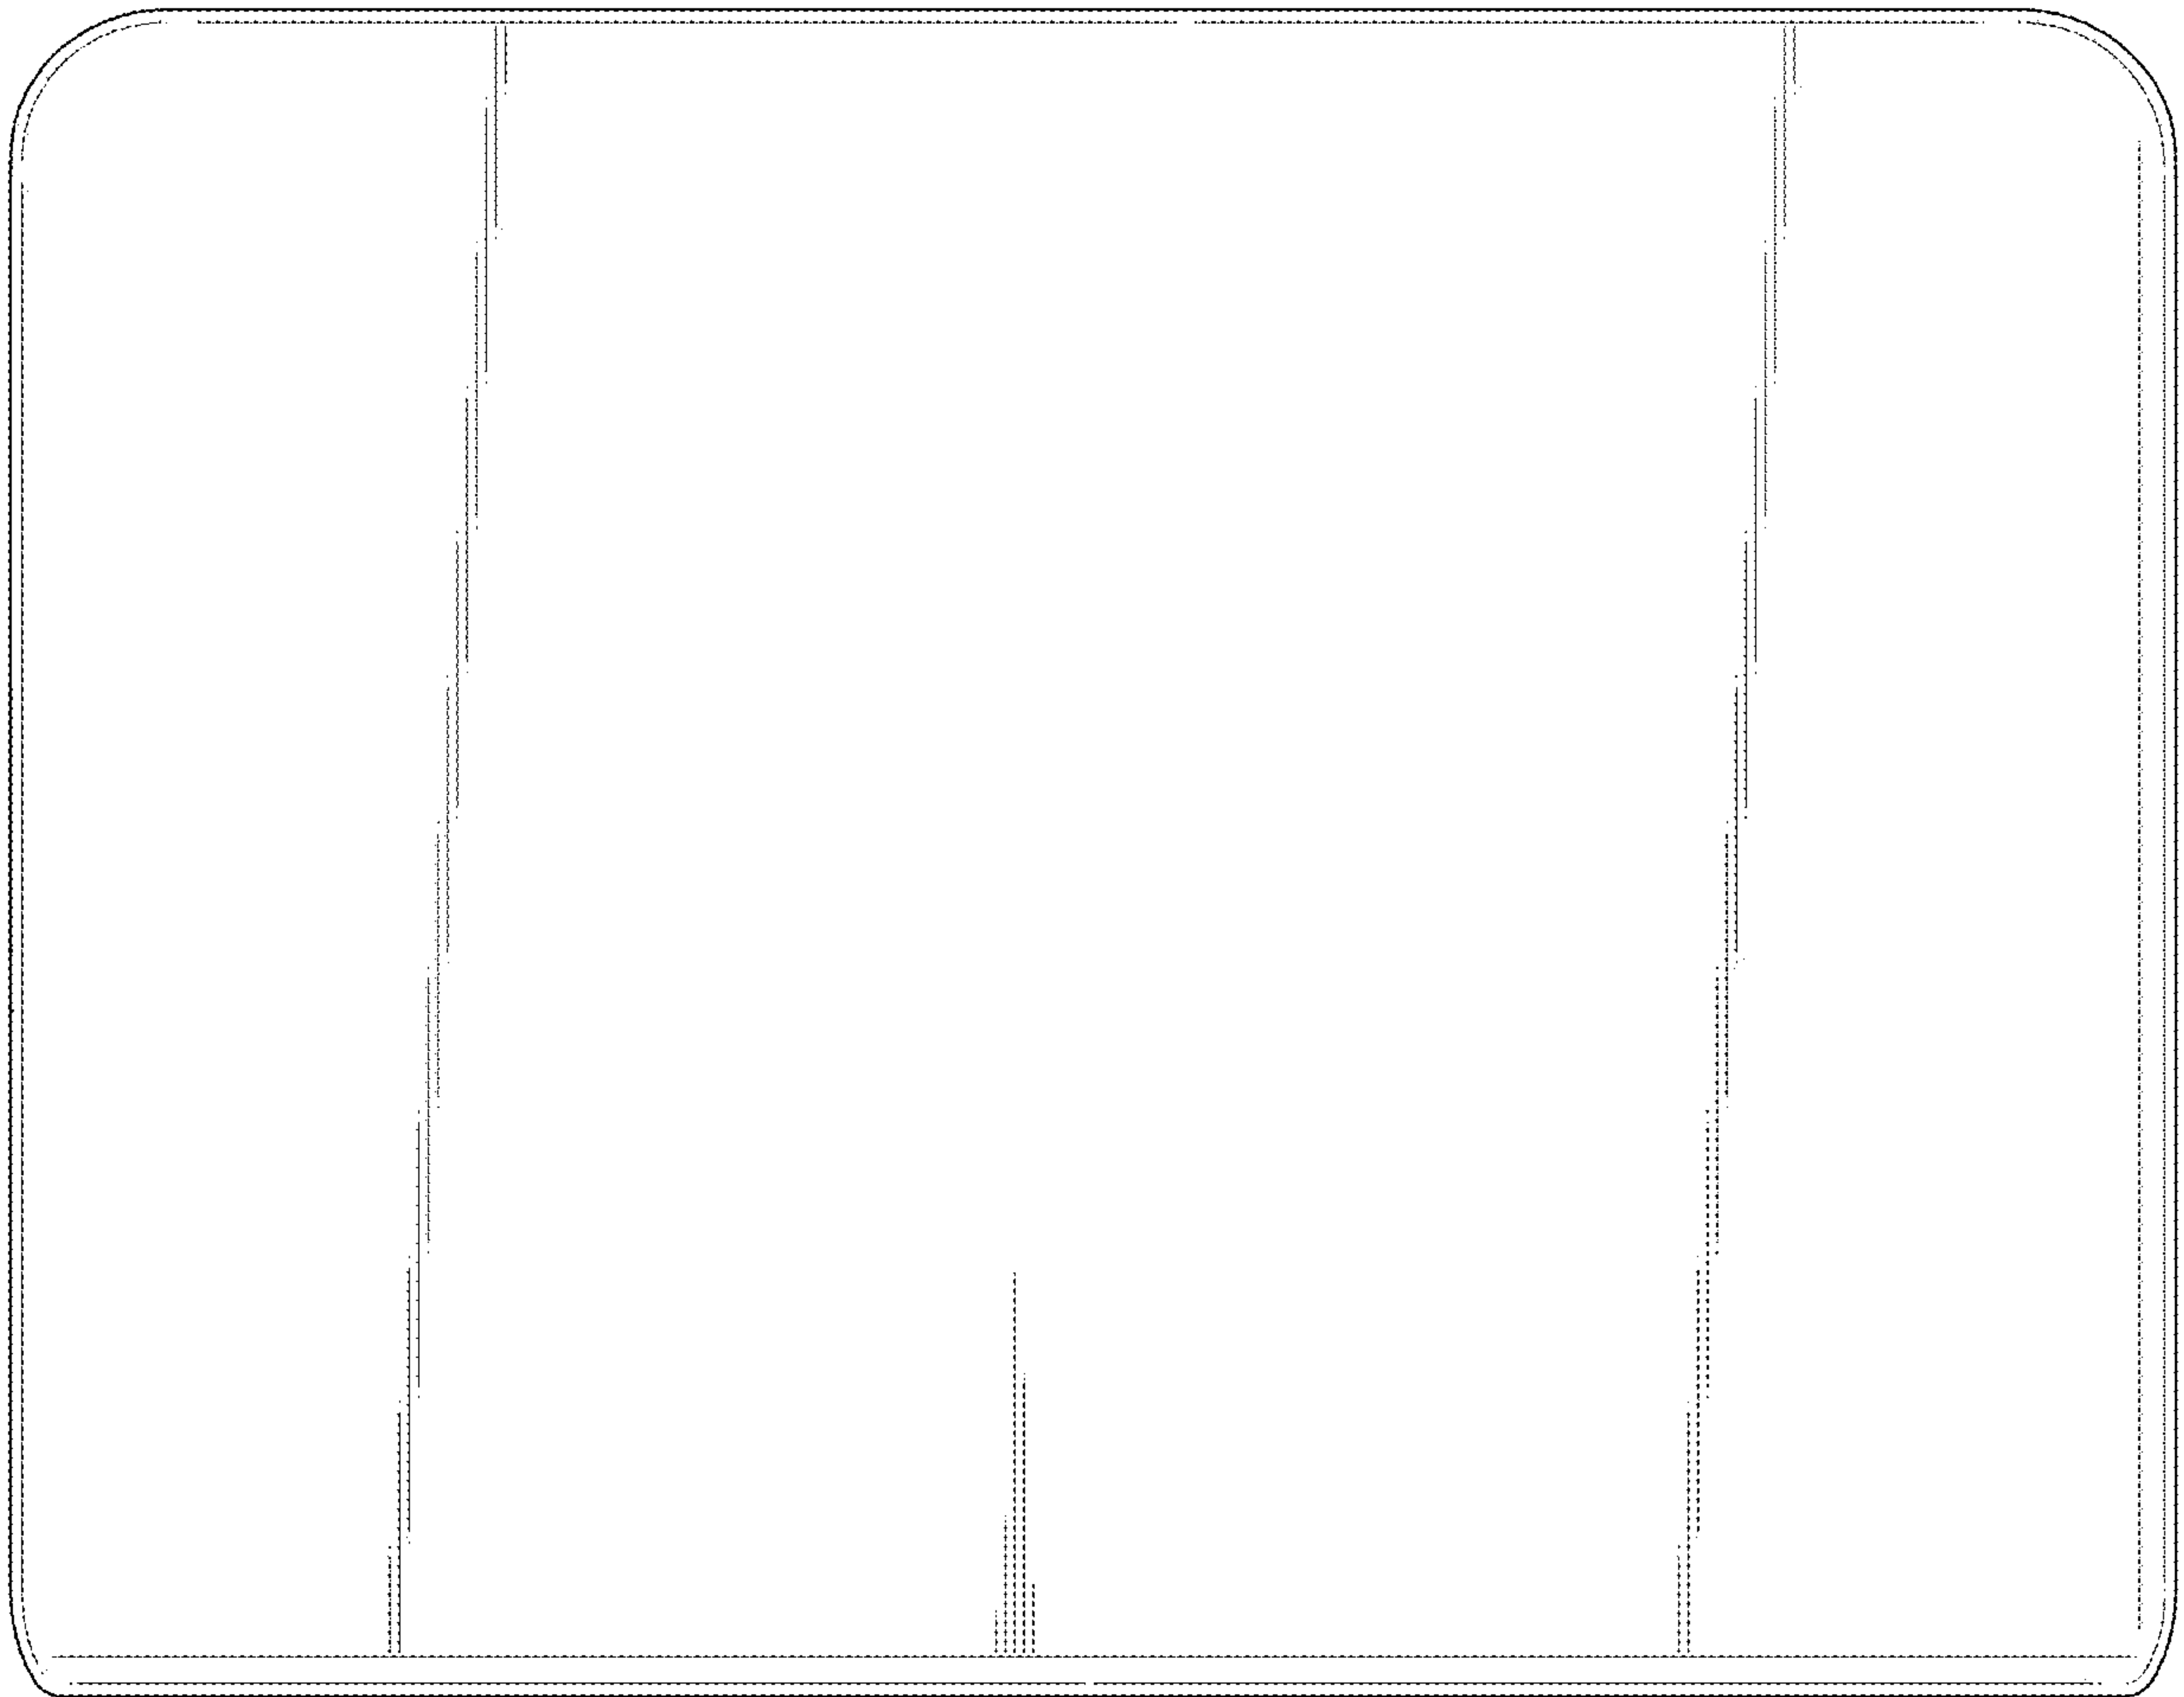


FIG.3

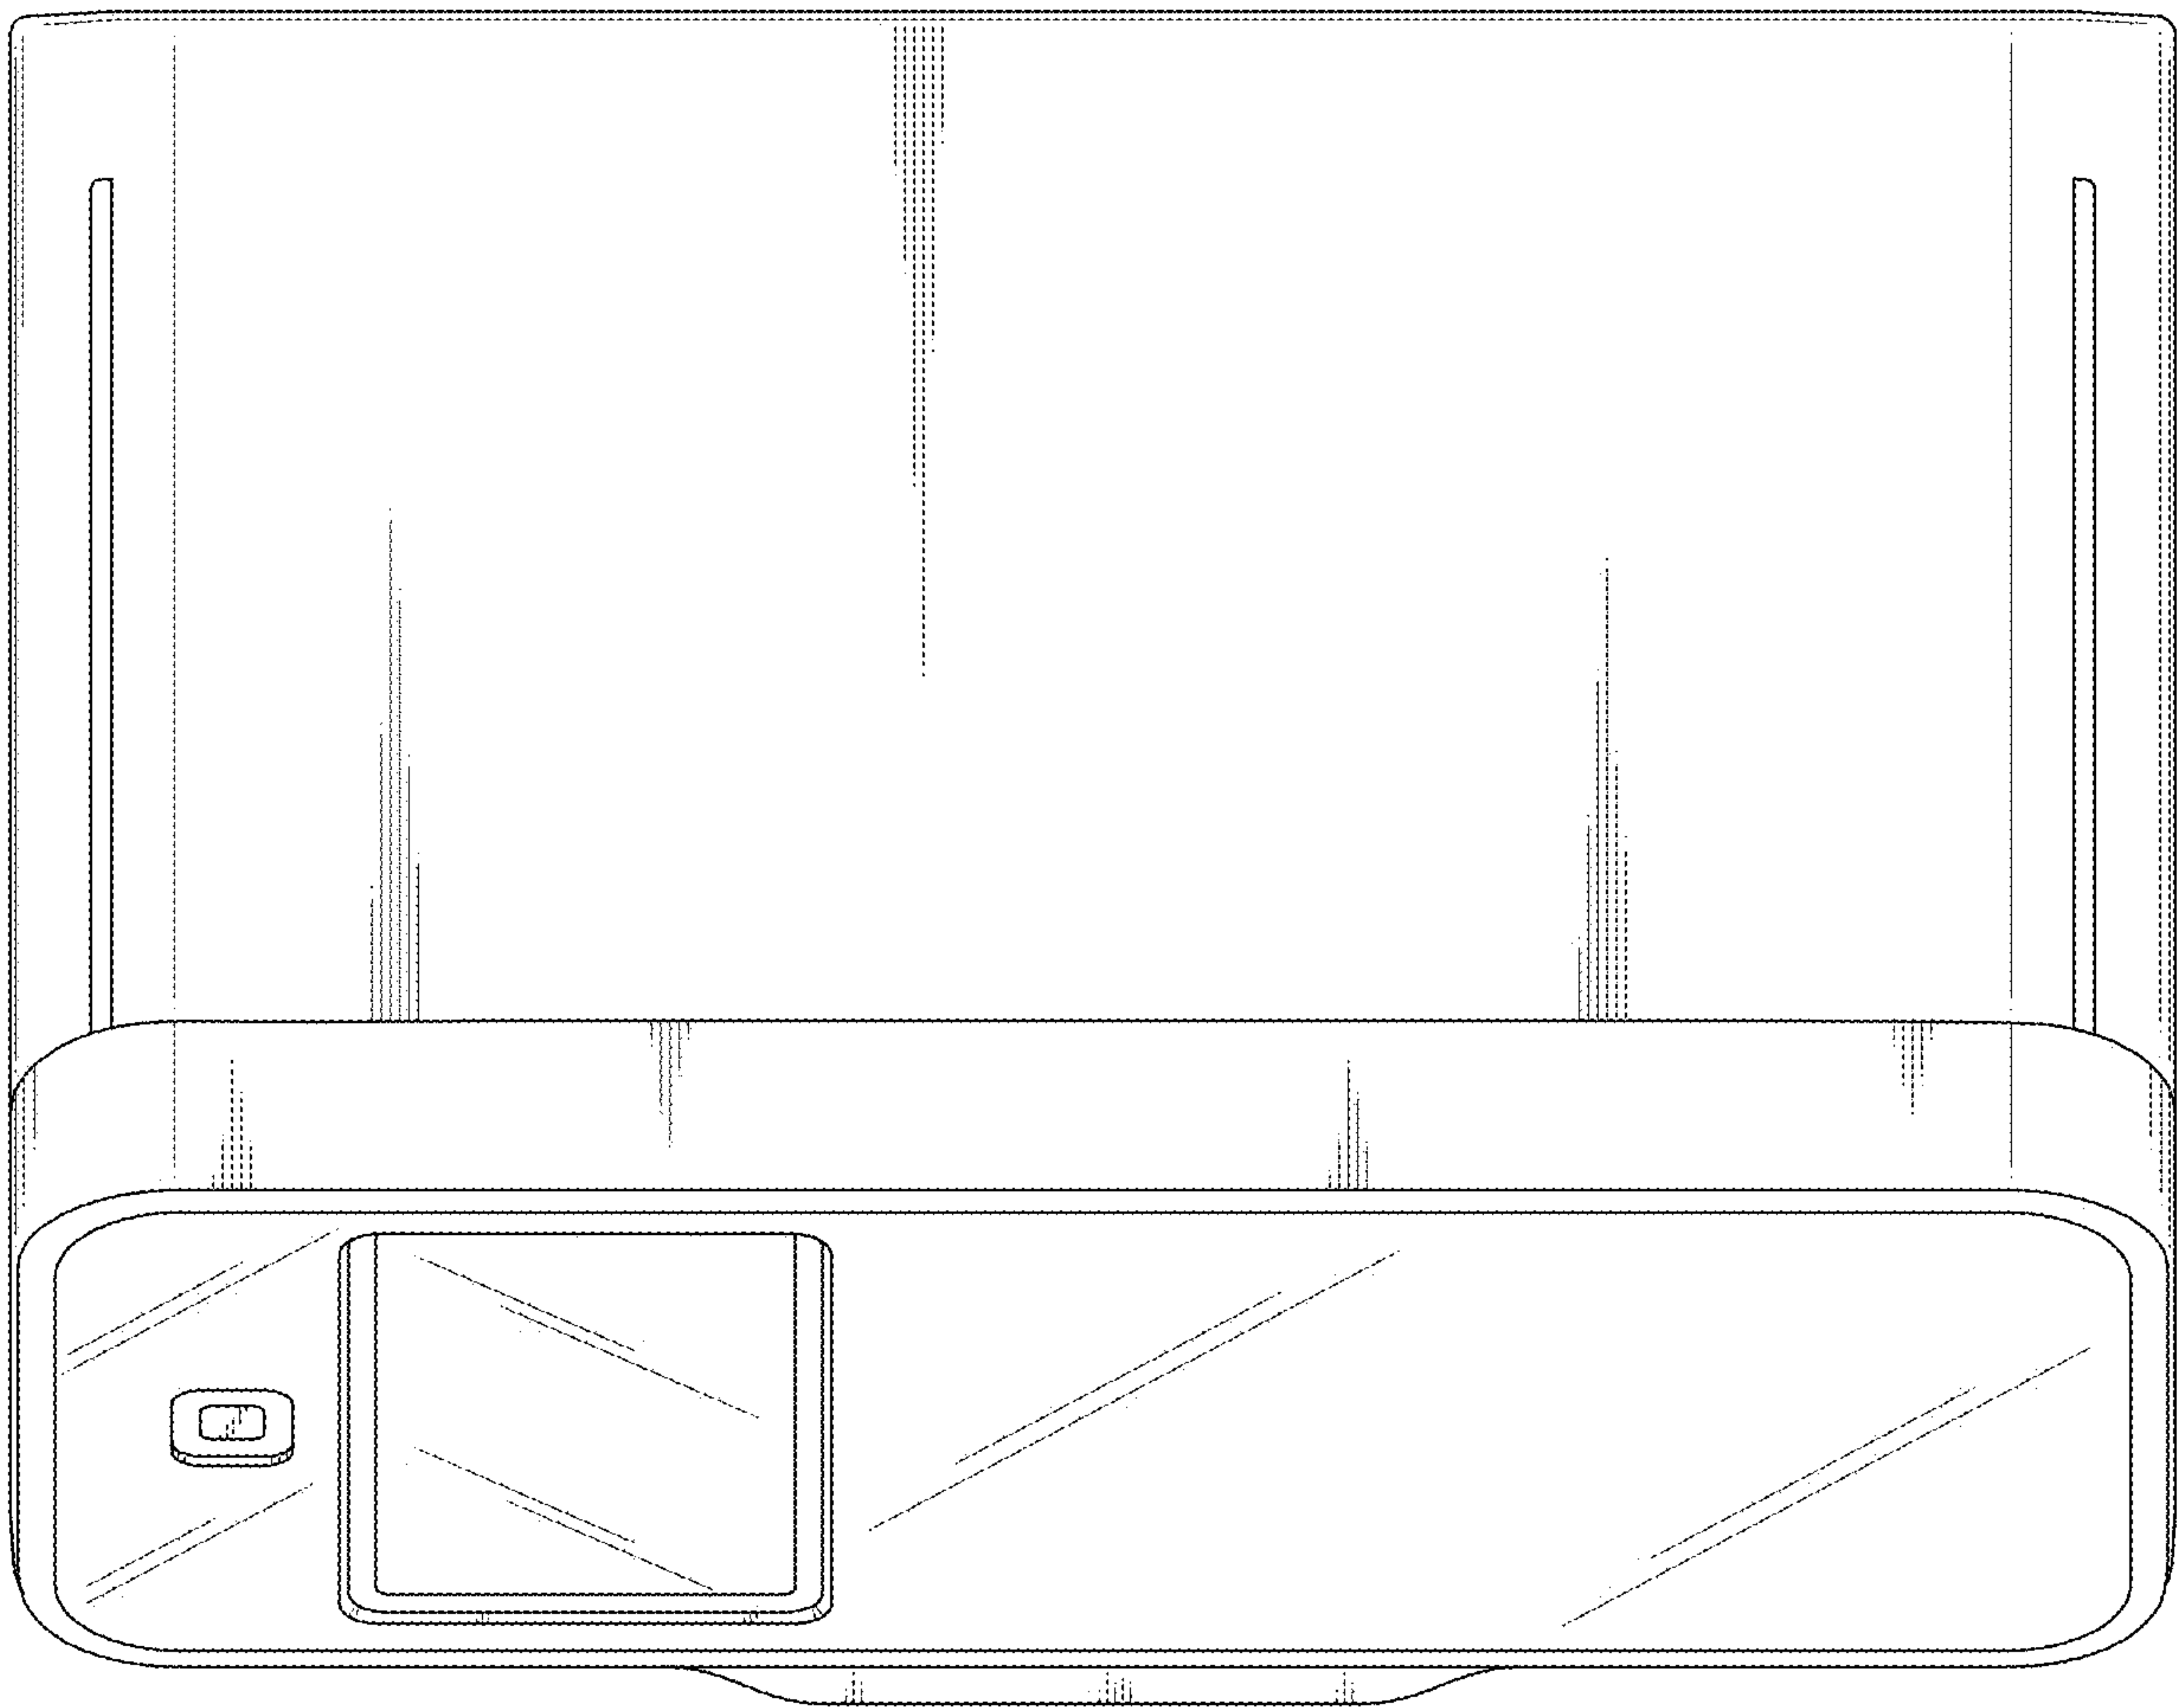


FIG.4

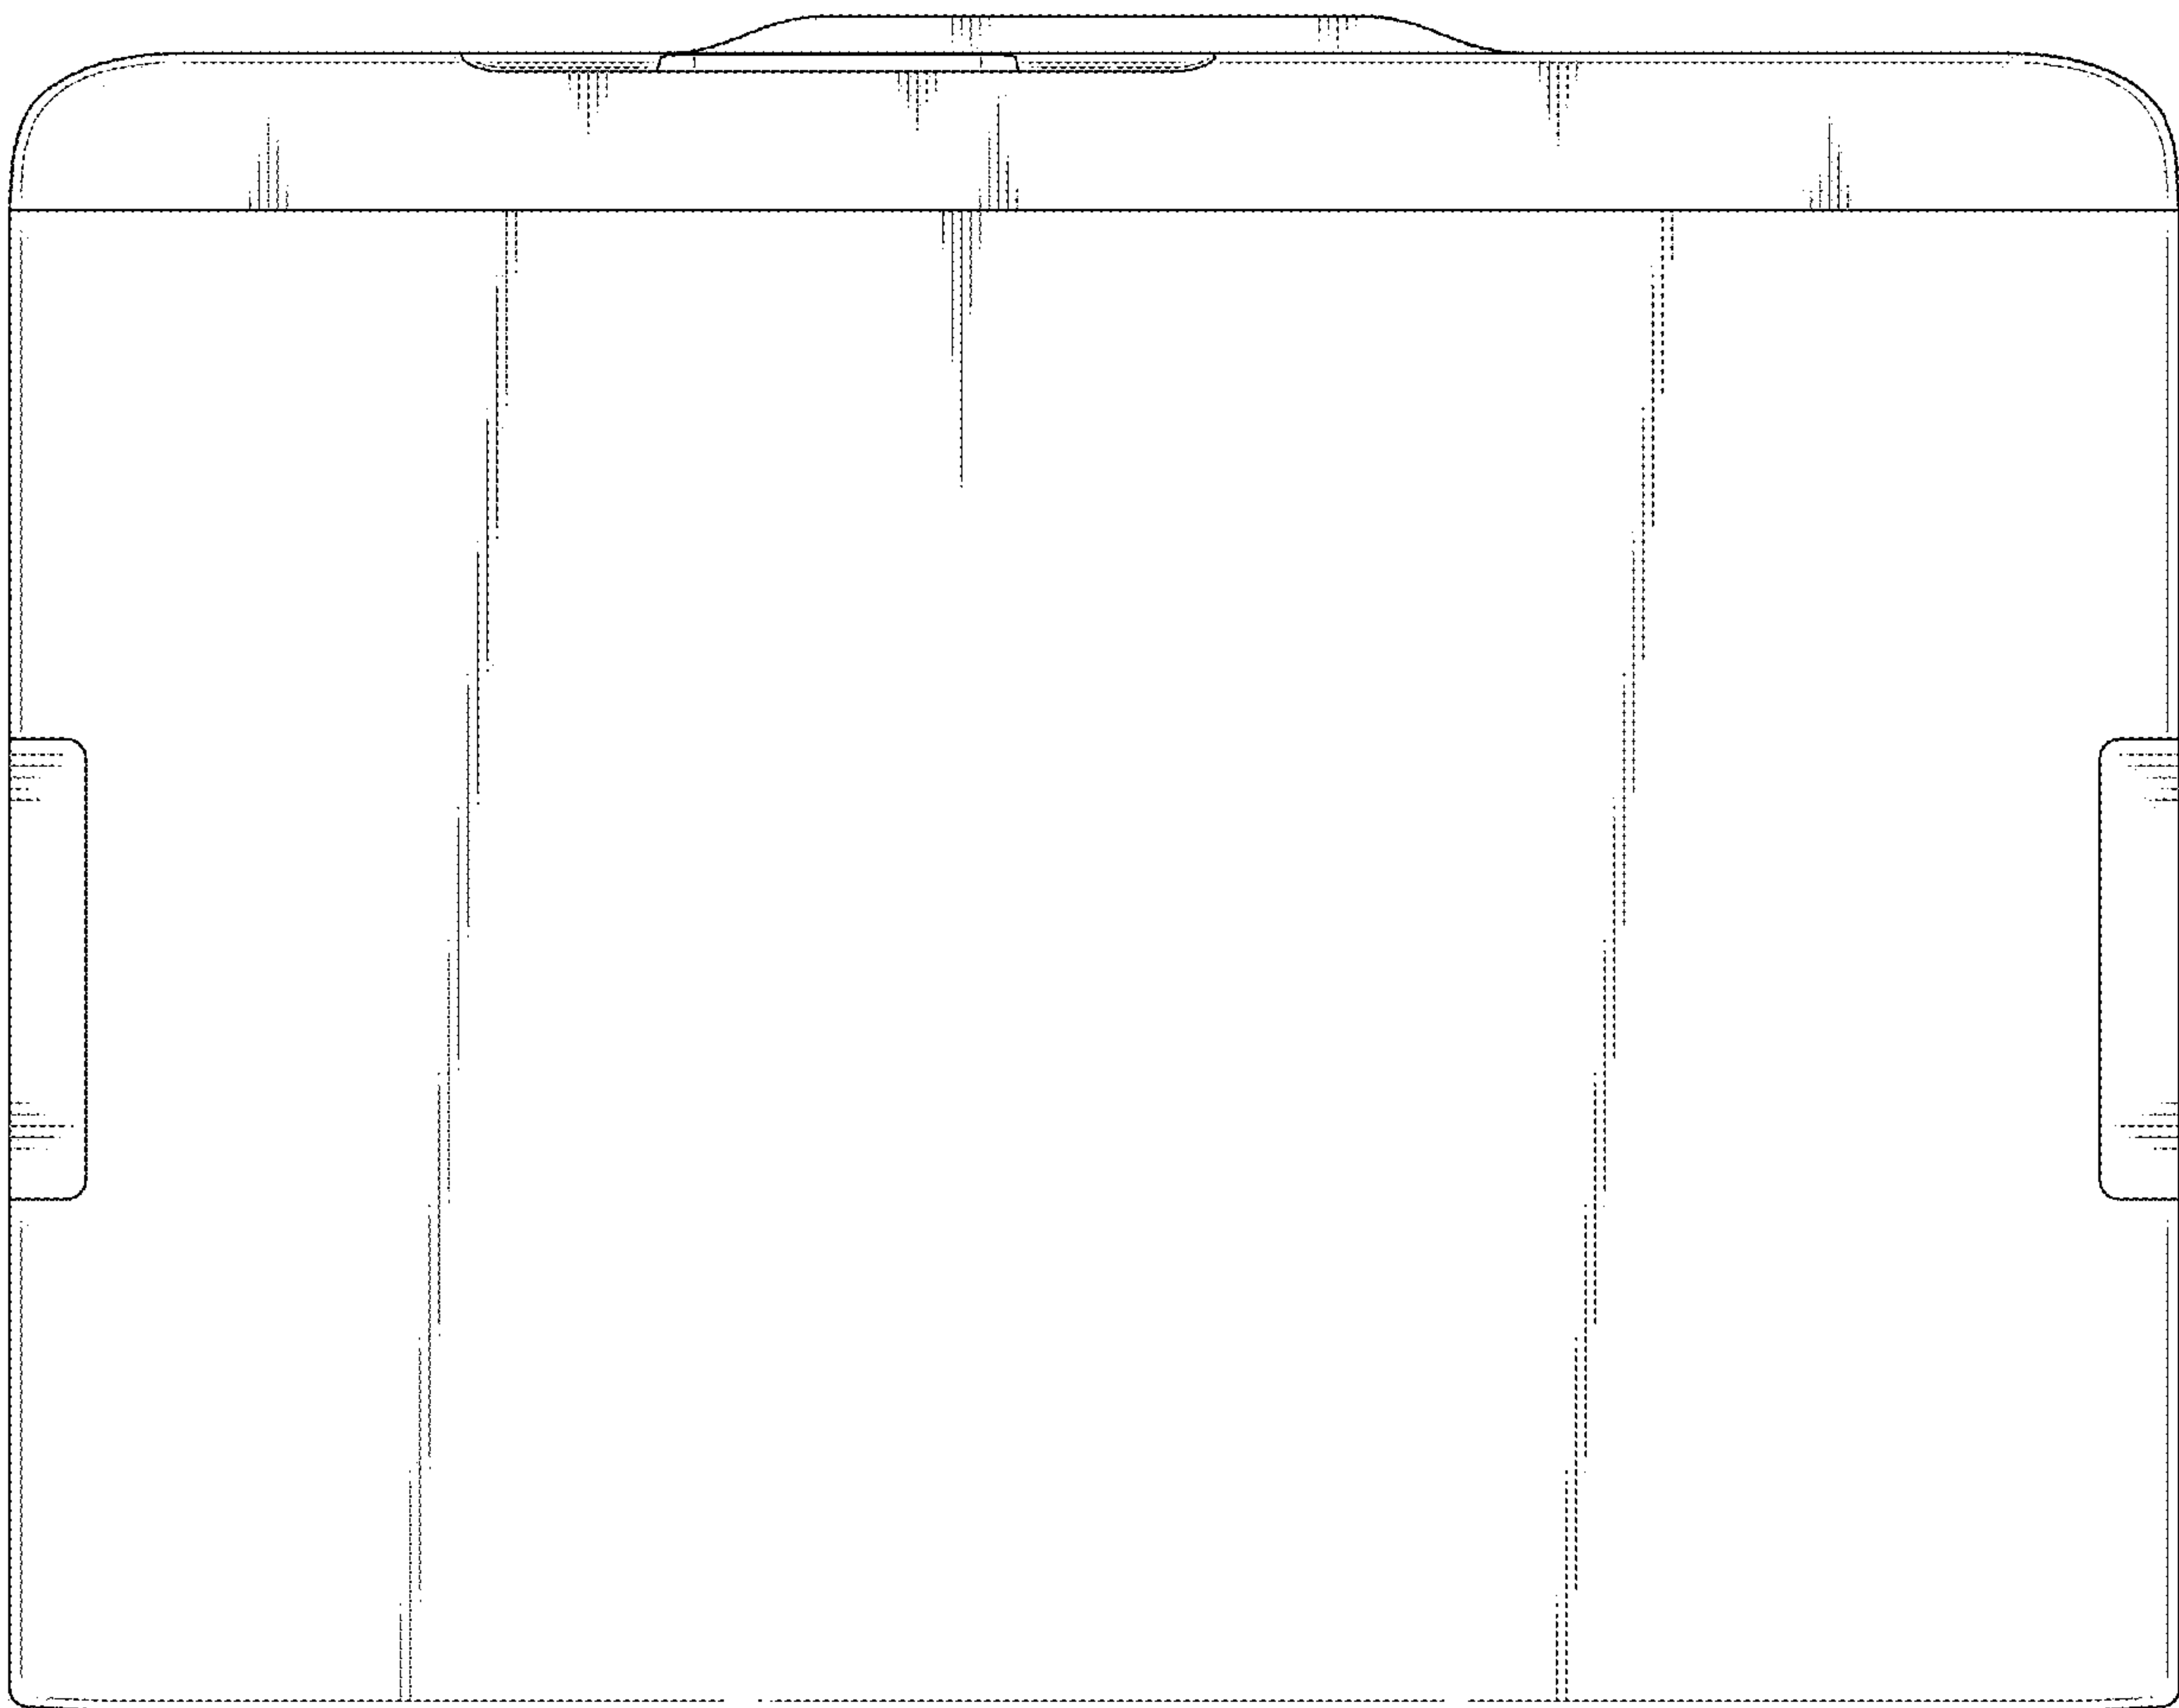


FIG.5

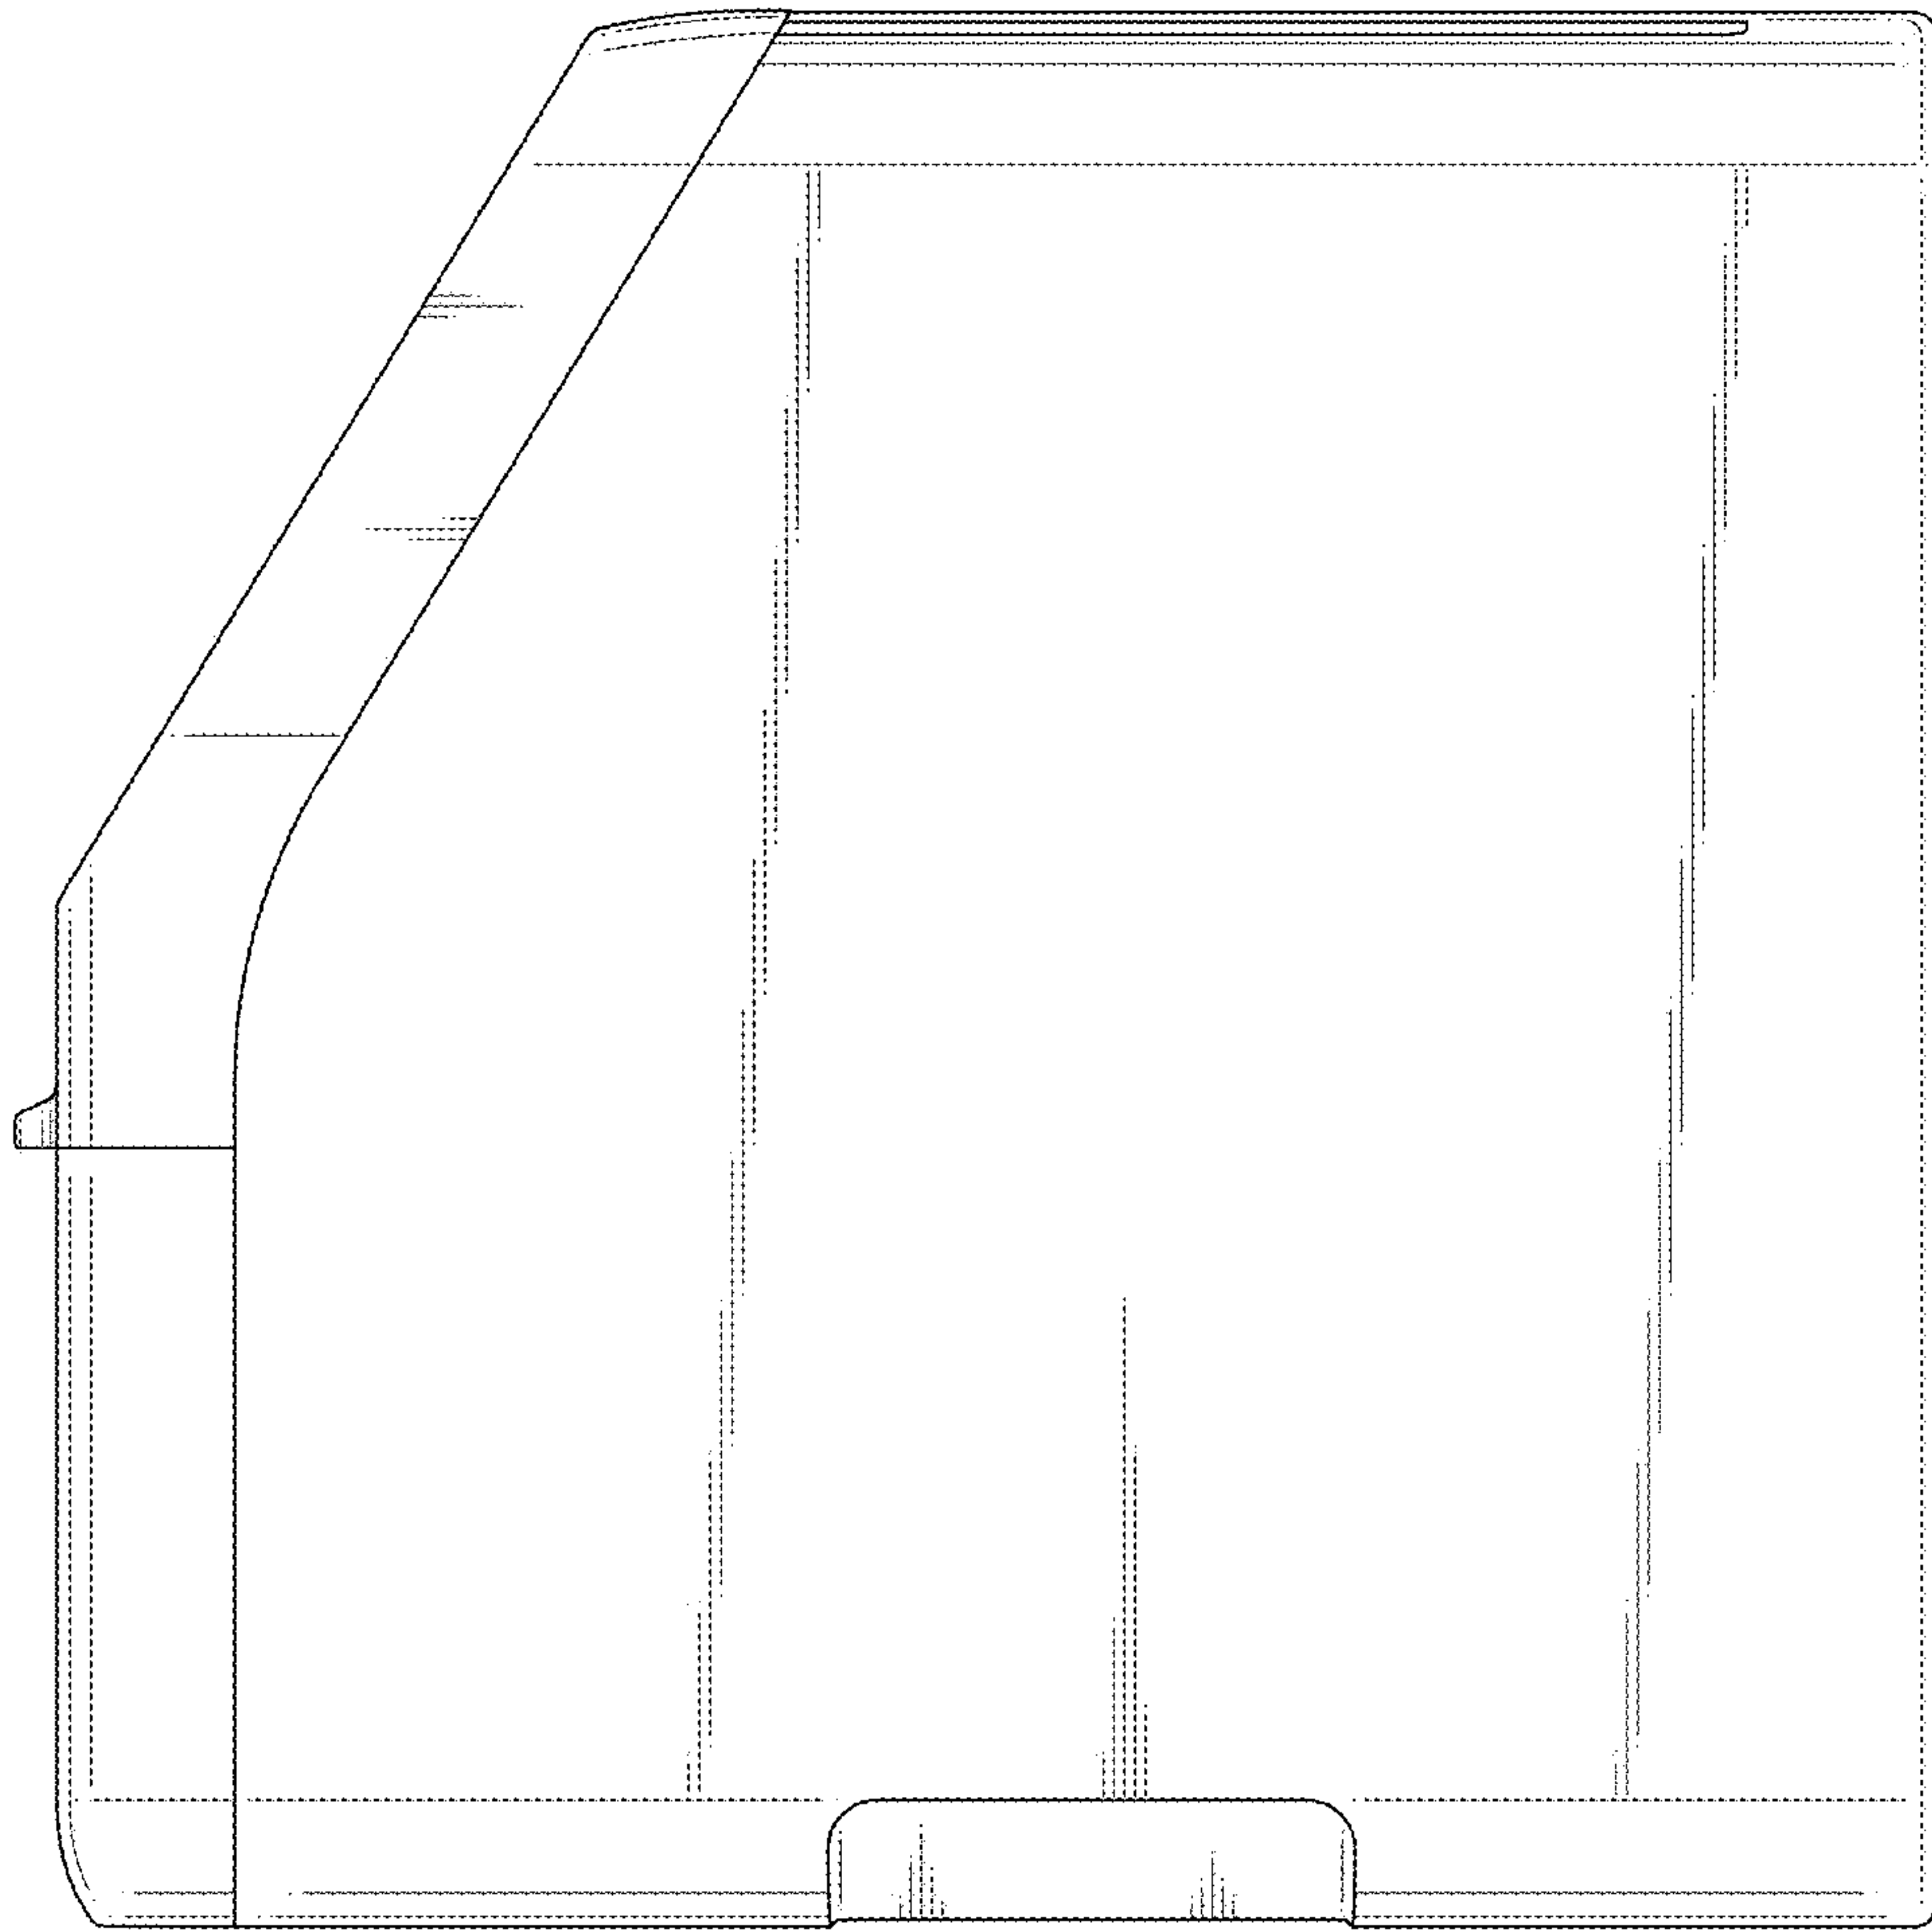


FIG.6

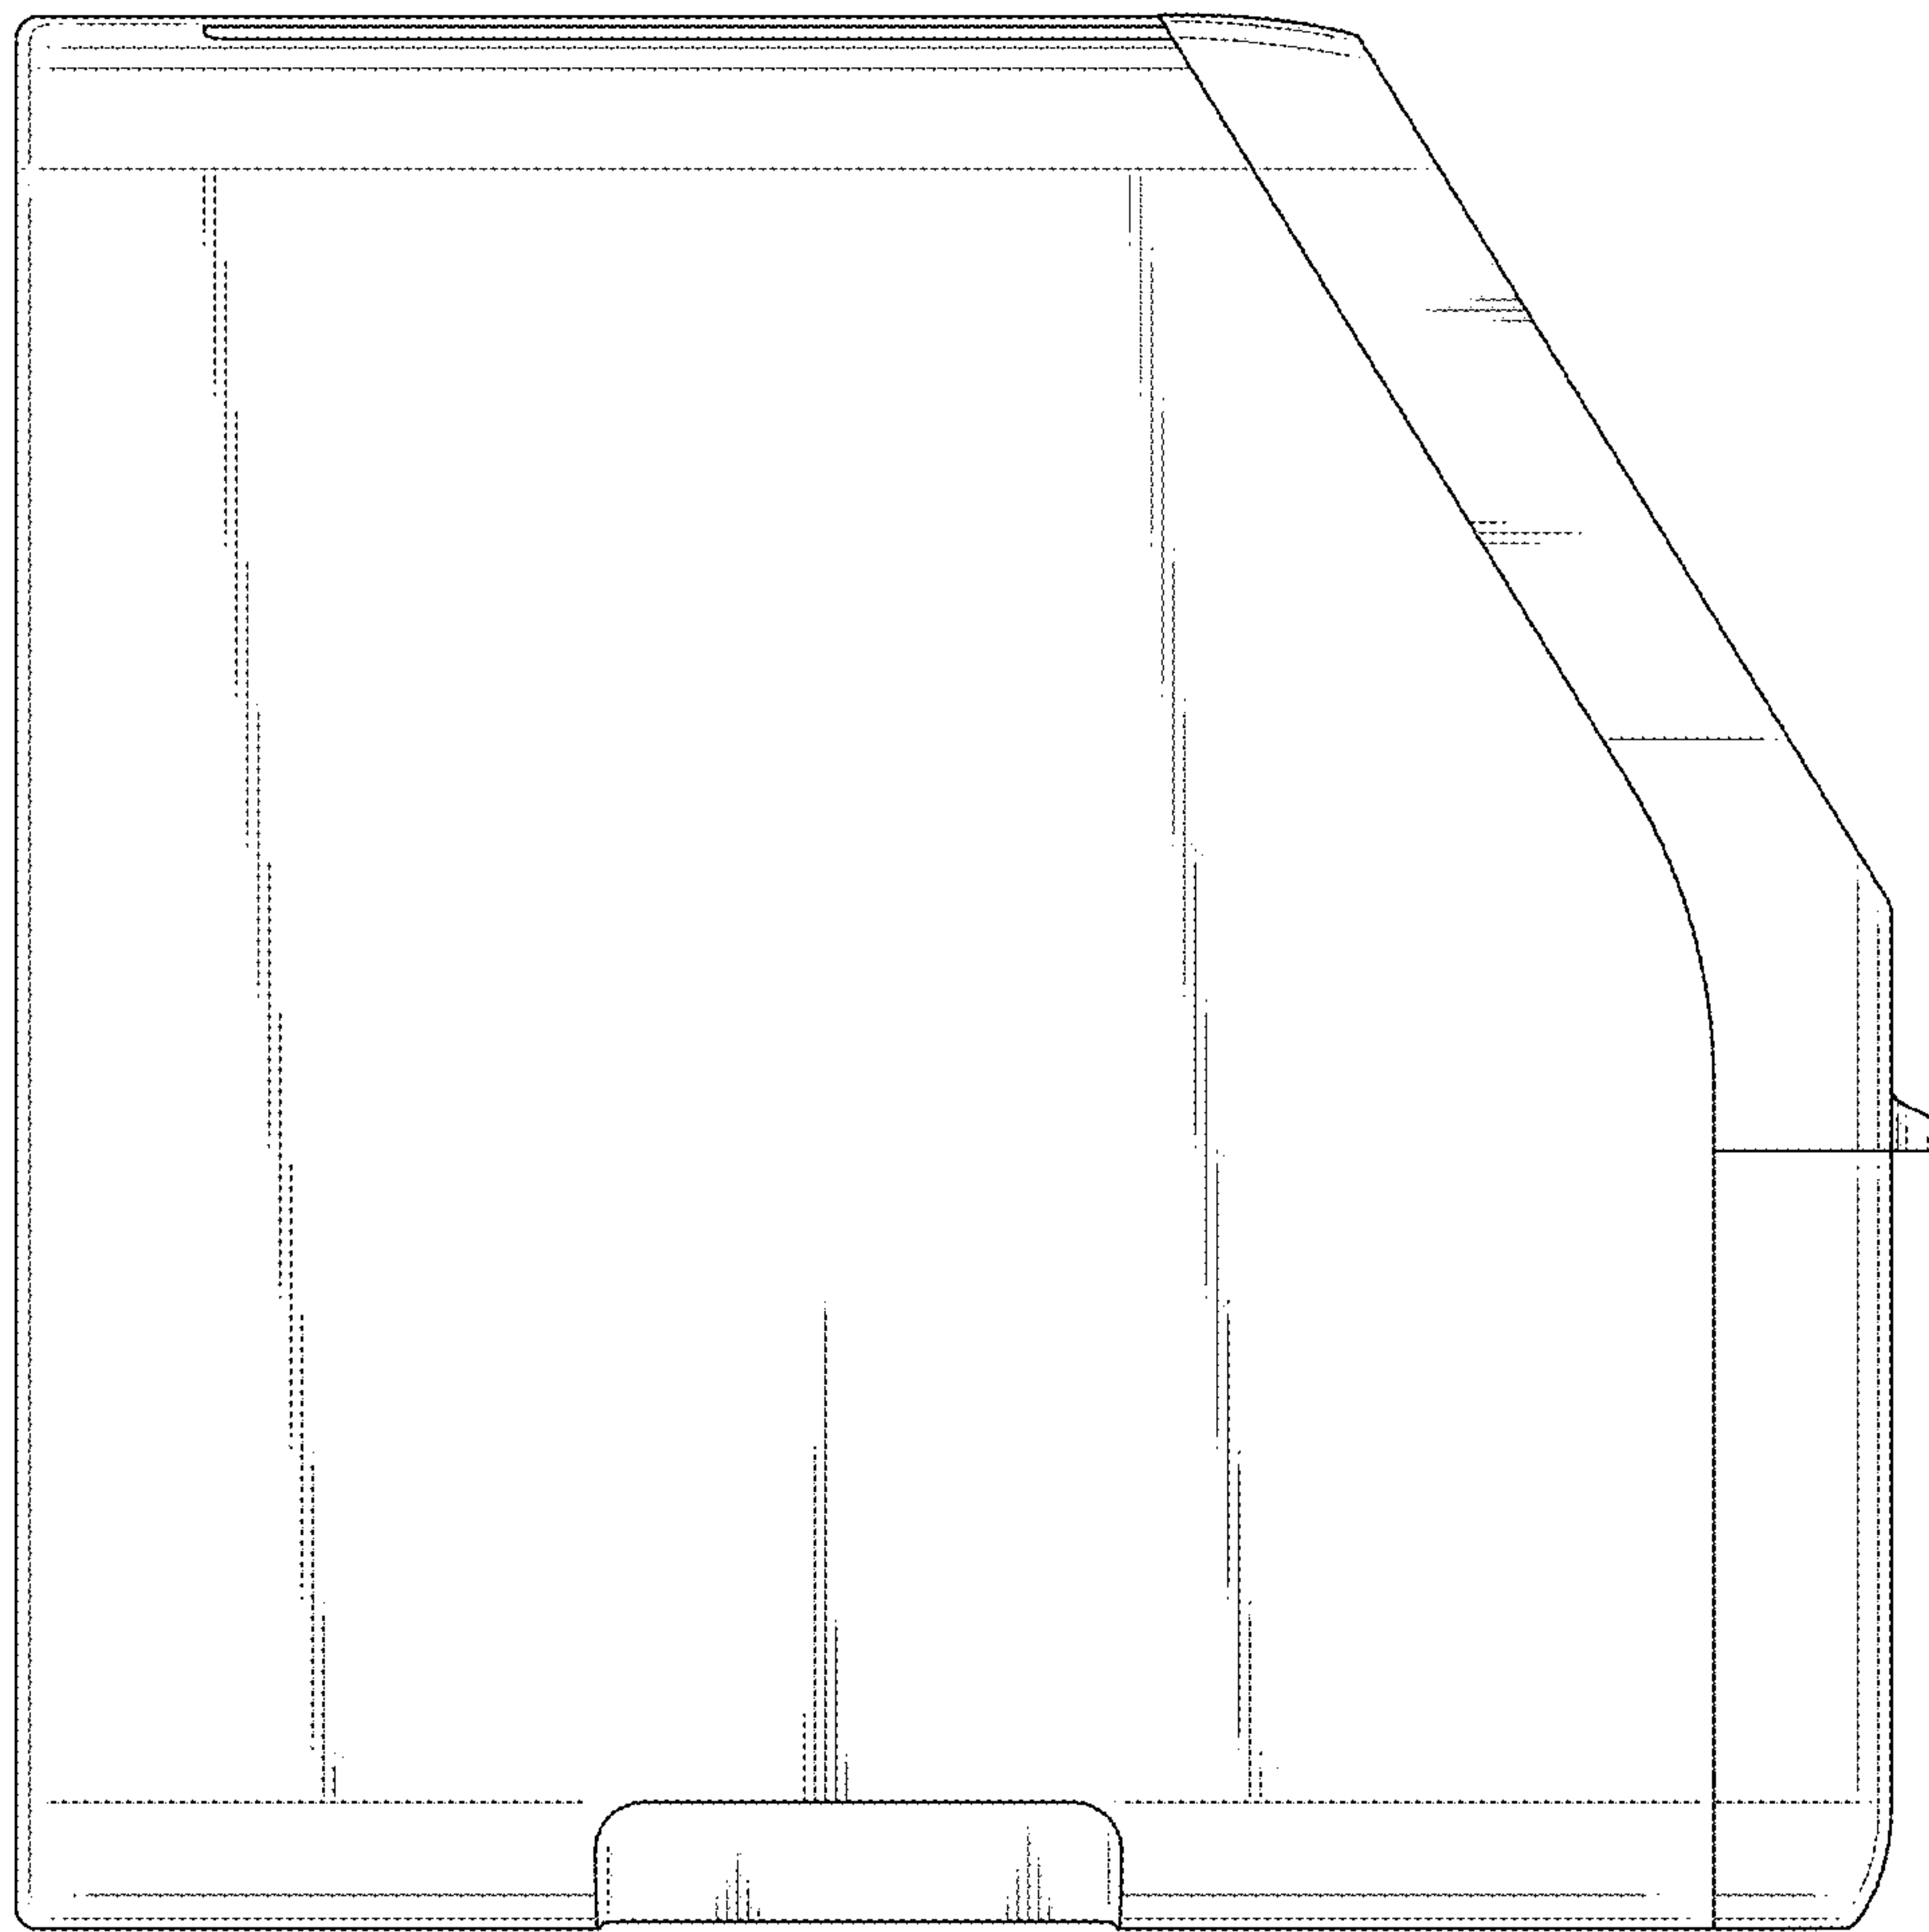


FIG.7

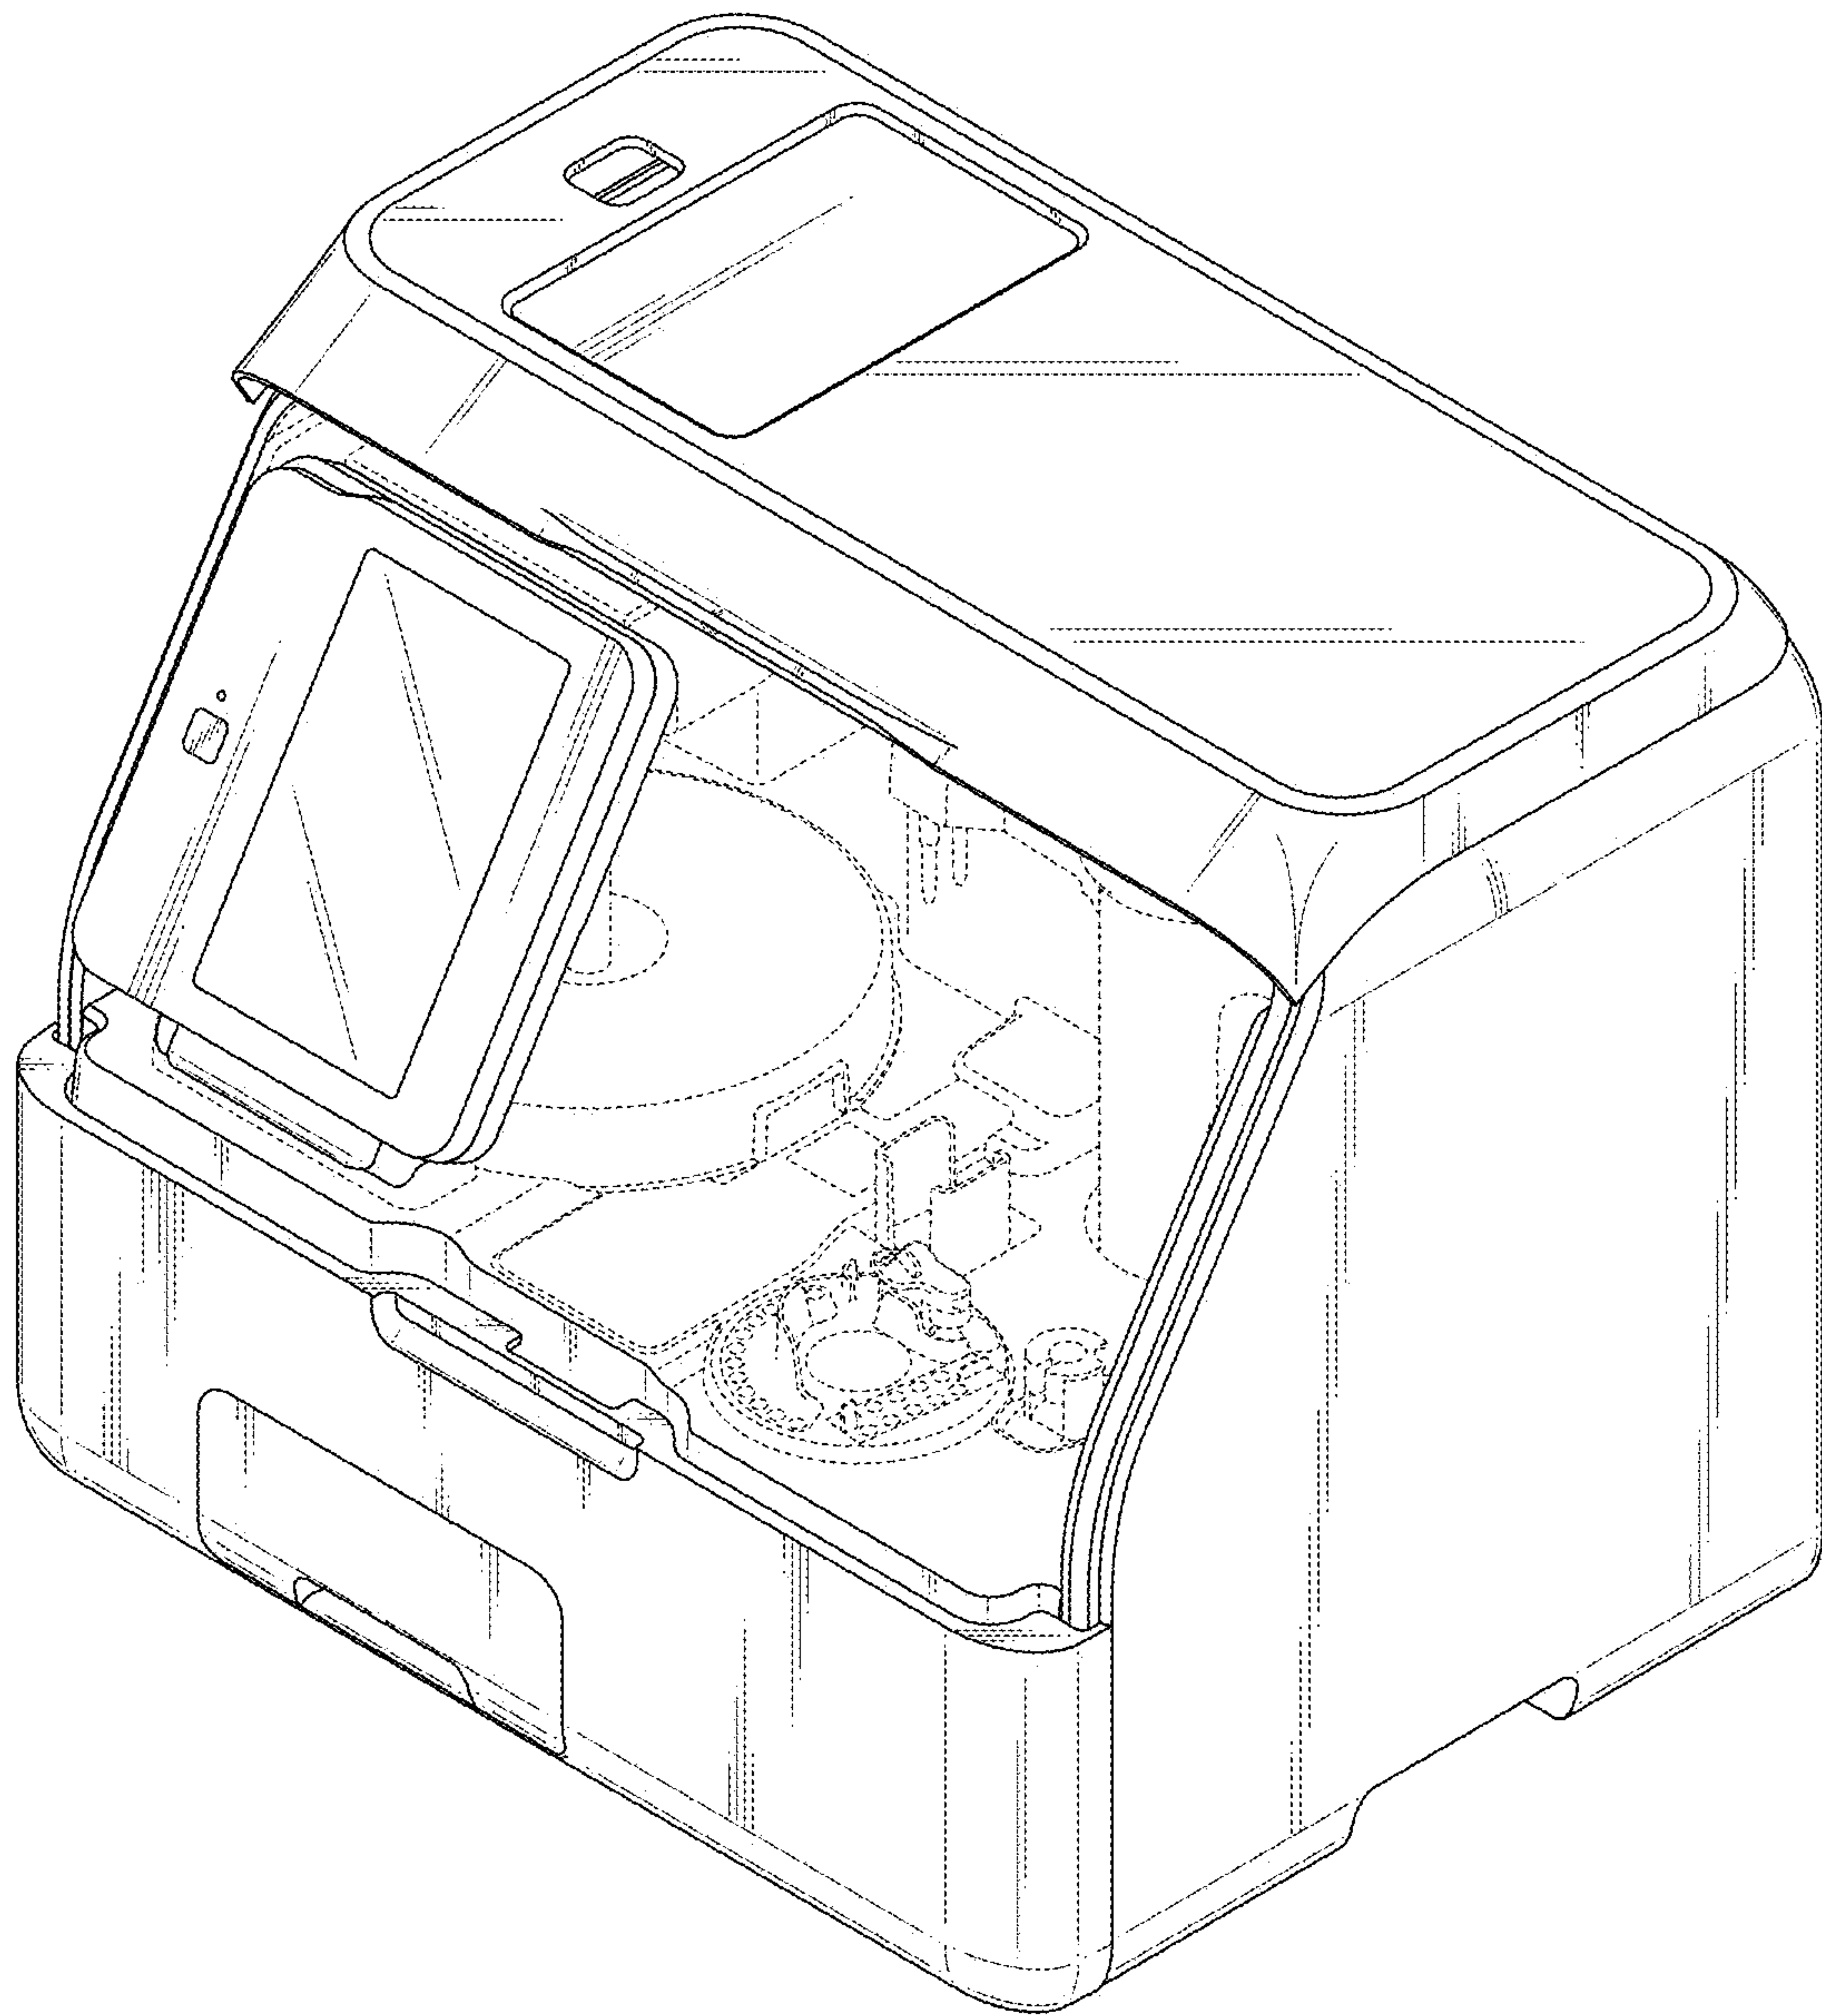


FIG.8

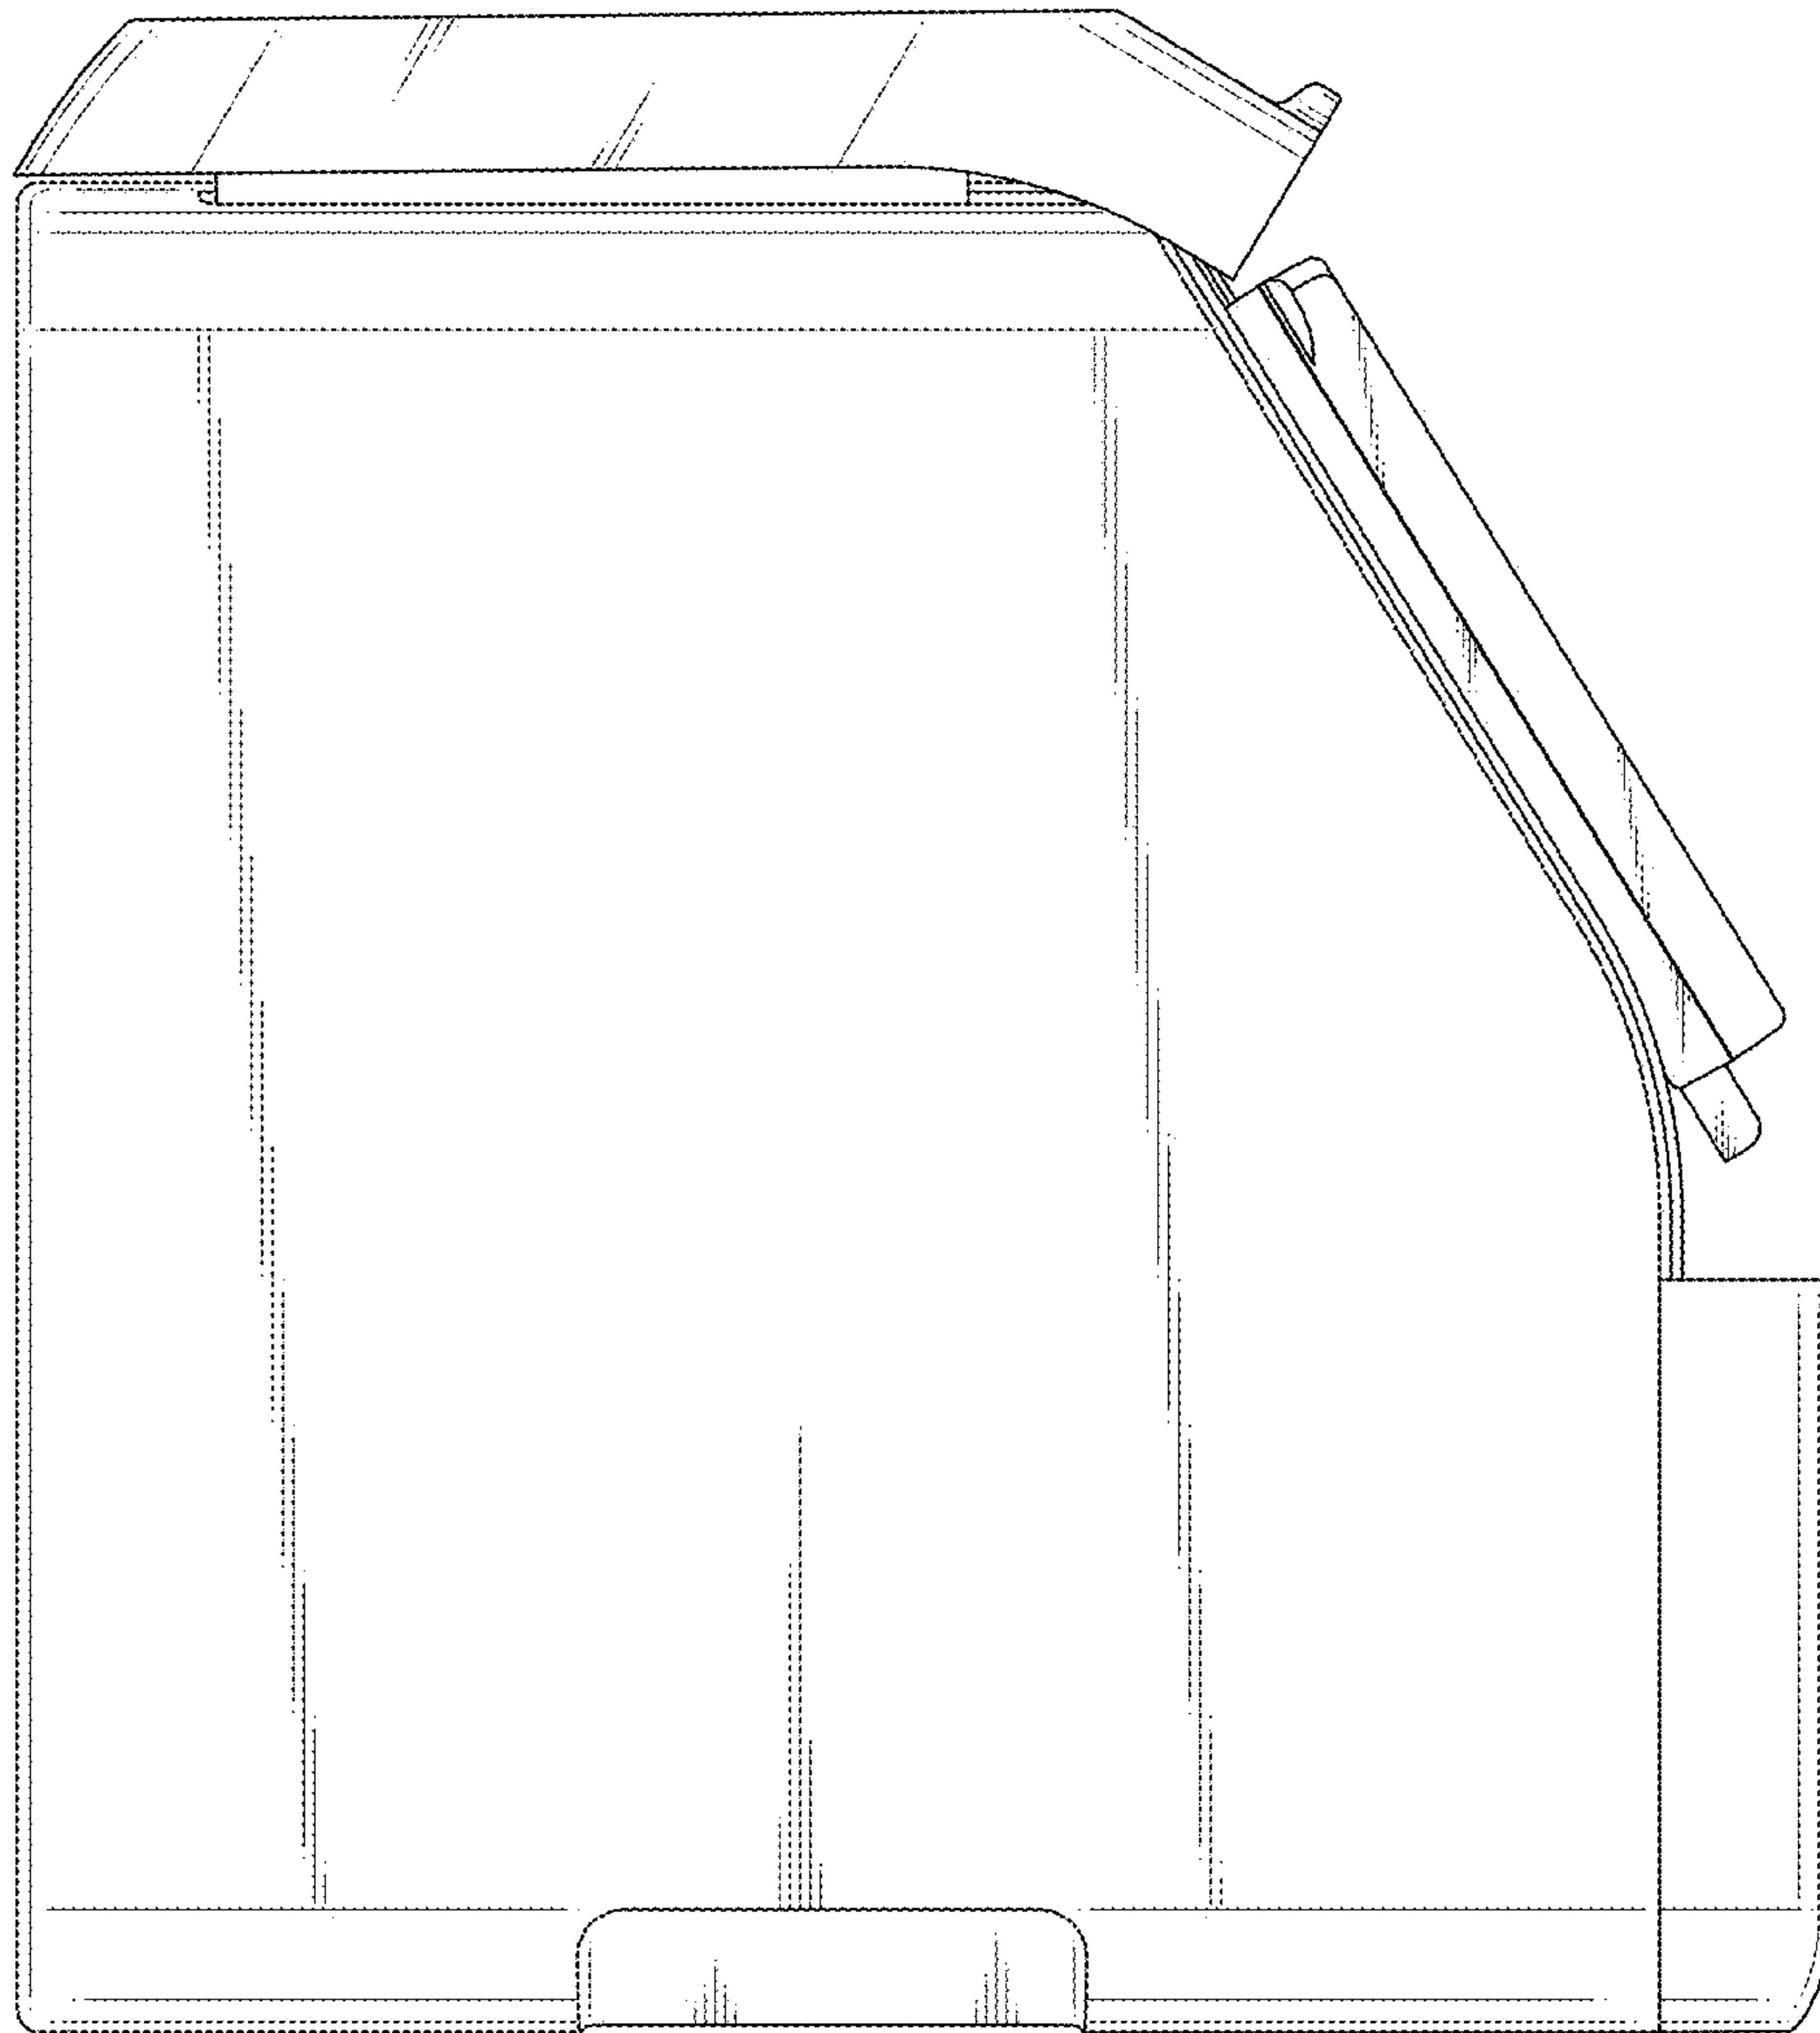


FIG.9