



US00D982744S

(12) **United States Design Patent** (10) **Patent No.:** **US D982,744 S**  
**Ryan et al.** (45) **Date of Patent:** **\*\* Apr. 4, 2023**

(54) **DRUG DELIVERY DEVICE**  
(71) Applicant: **Enesi Pharma Limited**, Abingdon (GB)

D776,261 S \* 1/2017 Jones ..... D24/113  
D786,423 S \* 5/2017 Jones ..... D24/113  
D790,687 S \* 6/2017 Jones ..... D24/113  
(Continued)

(72) Inventors: **Owen Ryan**, County Wicklow (IE);  
**David Andrew Grant**, Faringdon (GB);  
**Ritwik**, Oxfordshire (GB)

**OTHER PUBLICATIONS**

Kutepatil, O., Enesi Pharma form an R&D collaboration with Public Health England, Oct. 2018, news release, retrieved Oct. 4, 2021 from <URL:http://exsoft.org/enesi-pharma-forms-rd-public-health-england/> (Year: 2018).\*

(73) Assignee: **AVAXZIPEN LIMITED**, Abingdon (GB)

*Primary Examiner* — Calvin E Vansant  
(74) *Attorney, Agent, or Firm* — Bochner IP, PLLC;  
Andrew D. Bochner

(\*\*) Term: **15 Years**

(21) Appl. No.: **35/510,287**

(22) Filed: **Mar. 10, 2020**

(57) **CLAIM**

The ornamental design for a drug delivery device, as shown and described.

(80) **Hague Agreement Data**

Int. Filing Date: **Mar. 10, 2020**  
Int. Reg. No.: **DM/207563**  
Int. Reg. Date: **Mar. 10, 2020**  
Int. Reg. Pub. Date: **Sep. 11, 2020**

**DESCRIPTION**

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/114**

(58) **Field of Classification Search**  
USPC ..... D24/216, 222, 114, 112, 130, 113, 108  
CPC ..... A61M 2205/19; A61M 2250/00; A61M  
37/0069

See application file for complete search history.


1.1 is a front left perspective view;  
1.2 is a front right perspective view;  
1.3 is a front perspective view with a portion of the device rotated;  
1.4 is a front left perspective view with a portion of the device rotated;  
1.5 is a front right perspective view with a portion of the device rotated;  
1.6 is a front perspective view;  
2.1 is a front left perspective view;  
2.2 is a front right perspective view;  
2.3 is a front perspective view with a portion of the device rotated;  
2.4 is a front left perspective view with a portion of the device rotated;  
2.5 is a front right perspective view with a portion of the device rotated; and  
2.6 is a front perspective view.  
The broken lines depict portions of the drug delivery device that form no part of the claim.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D428,650 S \* 7/2000 Bellhouse ..... D24/112  
D479,748 S \* 9/2003 Tyce ..... D19/164  
D481,120 S \* 10/2003 Hawley ..... D19/177  
D555,609 S \* 11/2007 Galbraith ..... D24/114  
D567,939 S \* 4/2008 Mattigka ..... D24/114  
D619,244 S \* 7/2010 Van der Stappen ..... D24/113  
D676,547 S \* 2/2013 Quinn ..... D24/113  
D749,719 S \* 2/2016 Sanders ..... D24/114  
D770,611 S \* 11/2016 Saussaye ..... D24/114

**1 Claim, 12 Drawing Sheets**

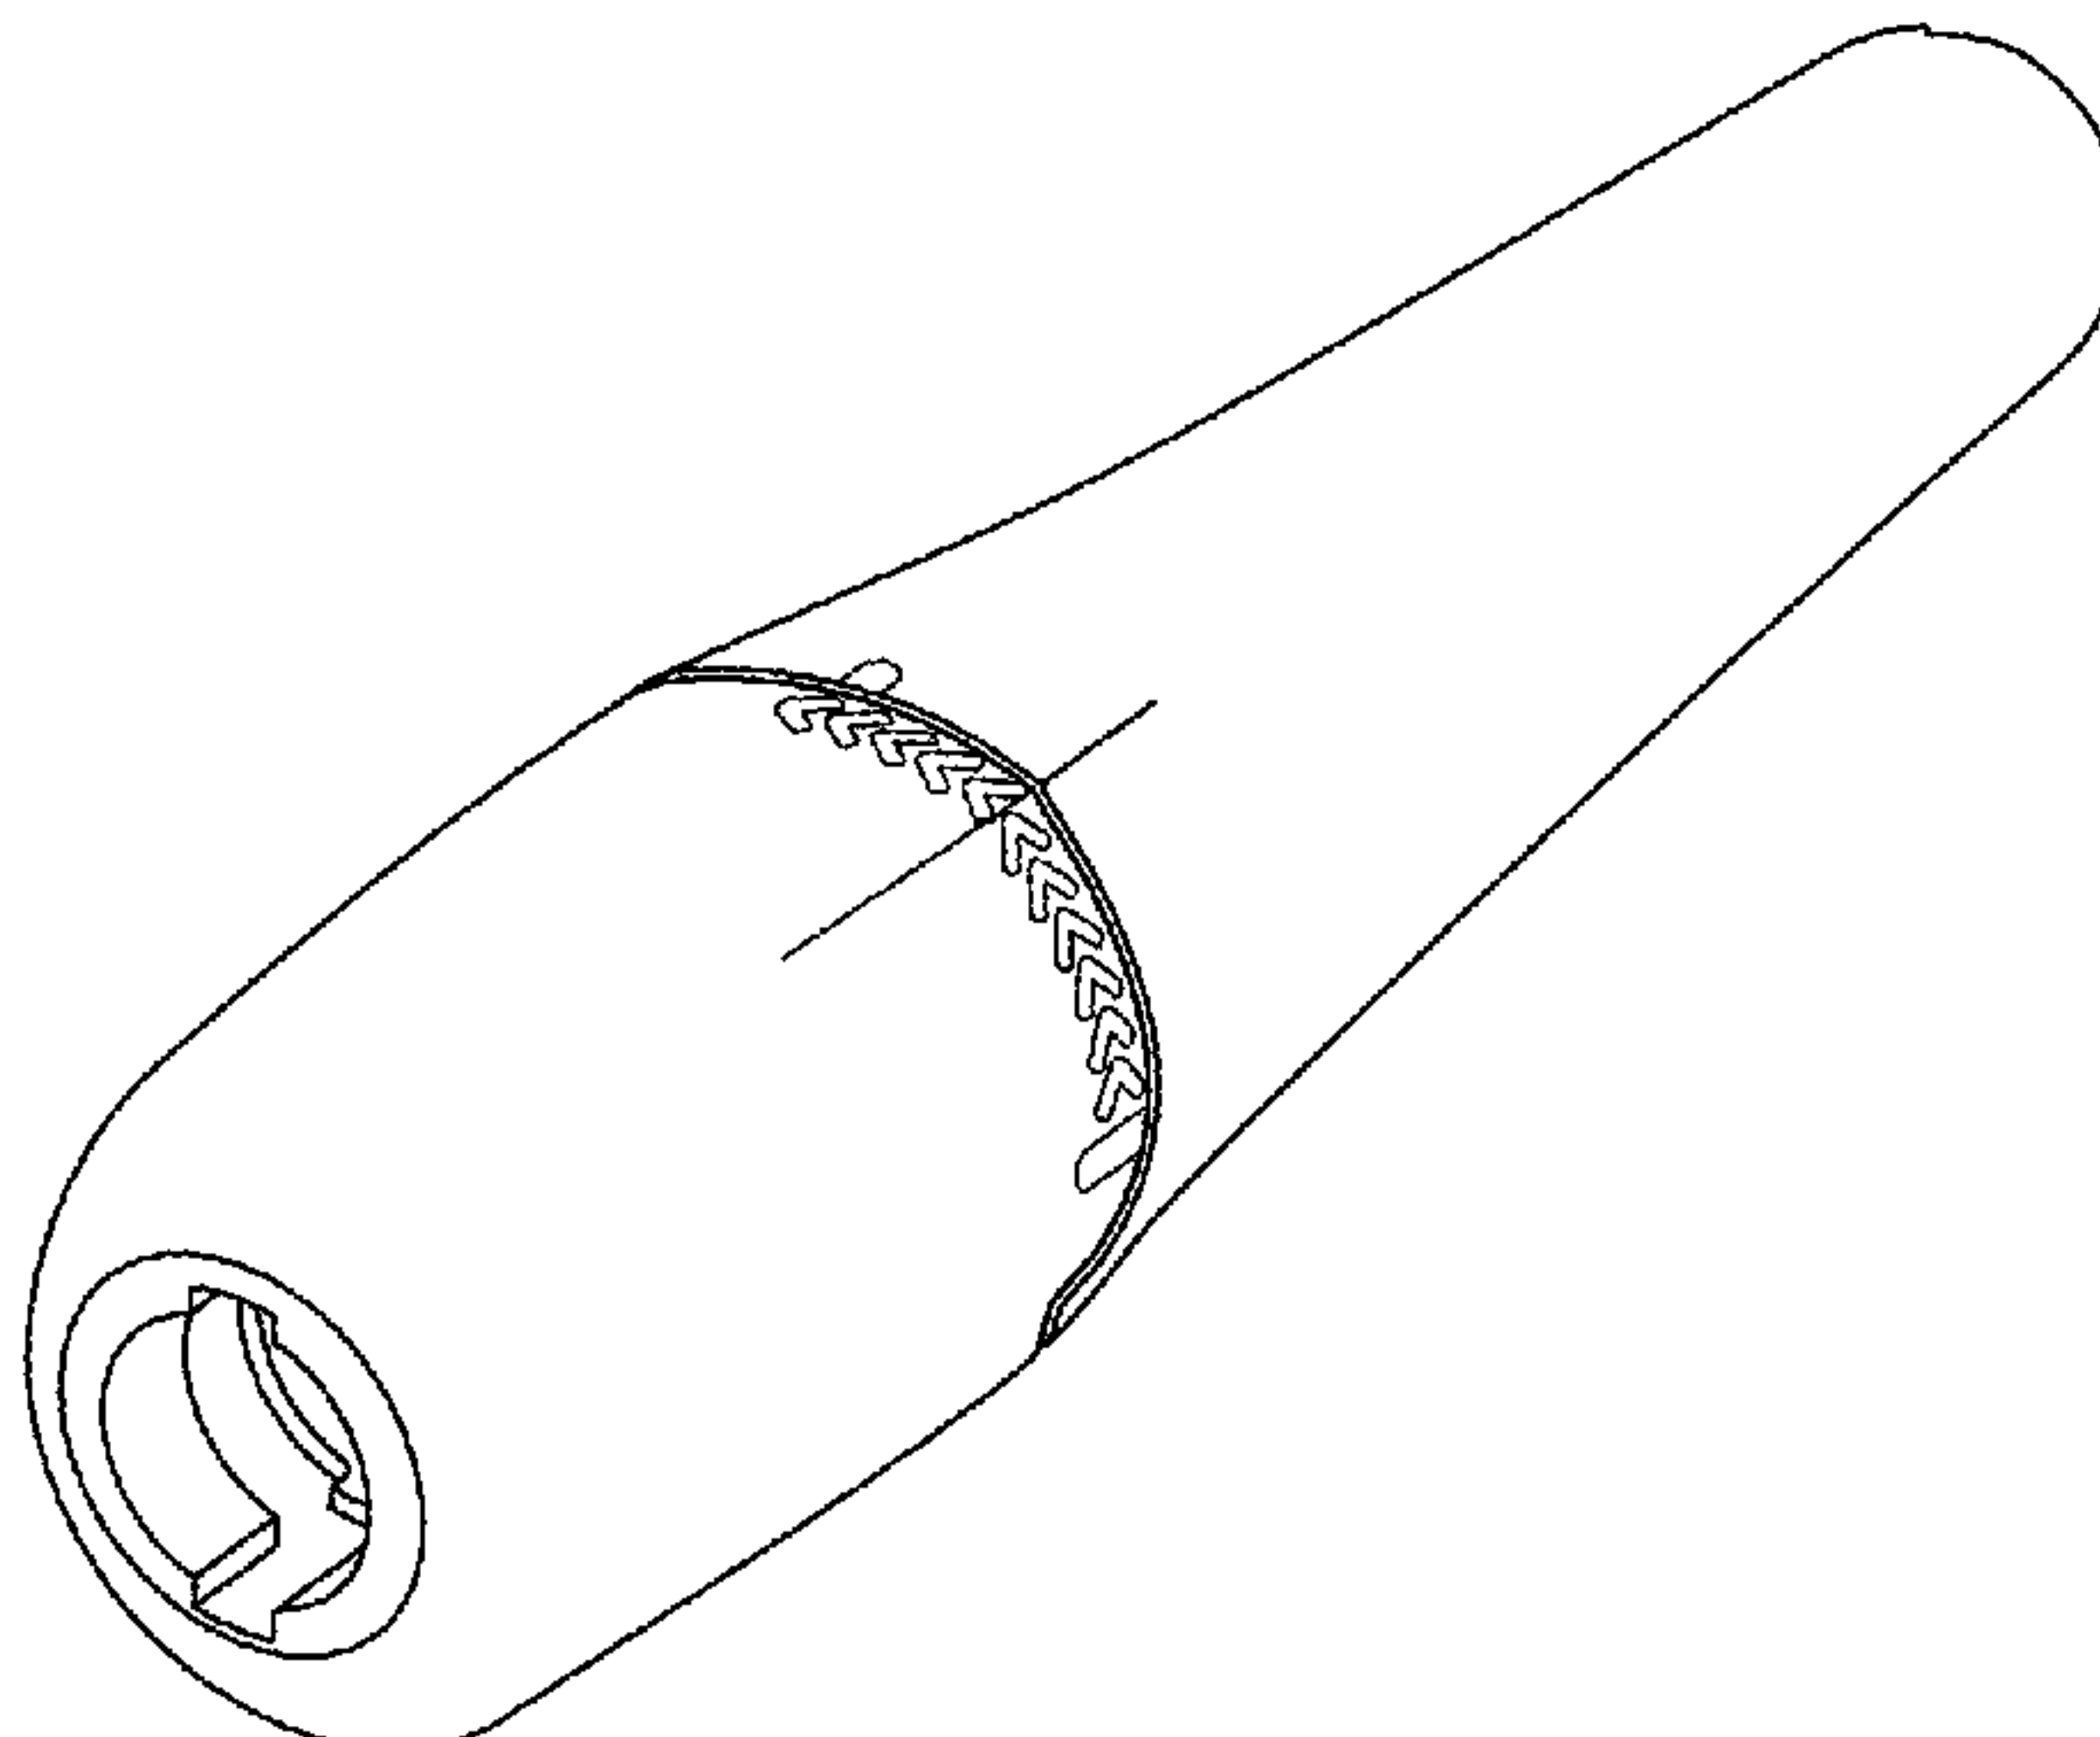


(56)

**References Cited**


U.S. PATENT DOCUMENTS

D792,578 S *	7/2017	Jones .....	D24/113
D800,898 S *	10/2017	Sanders .....	D24/114
D862,690 S *	10/2019	Jansen .....	D24/113
D878,563 S *	3/2020	Clawson .....	D24/113
D886,281 S *	6/2020	Boyaval .....	D24/113
D888,942 S *	6/2020	Cannamela .....	D24/114
D890,918 S *	7/2020	Fritz .....	D24/112
D915,584 S *	4/2021	Eisenkrein .....	D24/130
D926,967 S *	8/2021	Rogge .....	D24/113
D926,973 S *	8/2021	Andersen .....	D24/114
2018/0028798 A1 *	2/2018	Conlon .....	A61M 37/0069


\* cited by examiner

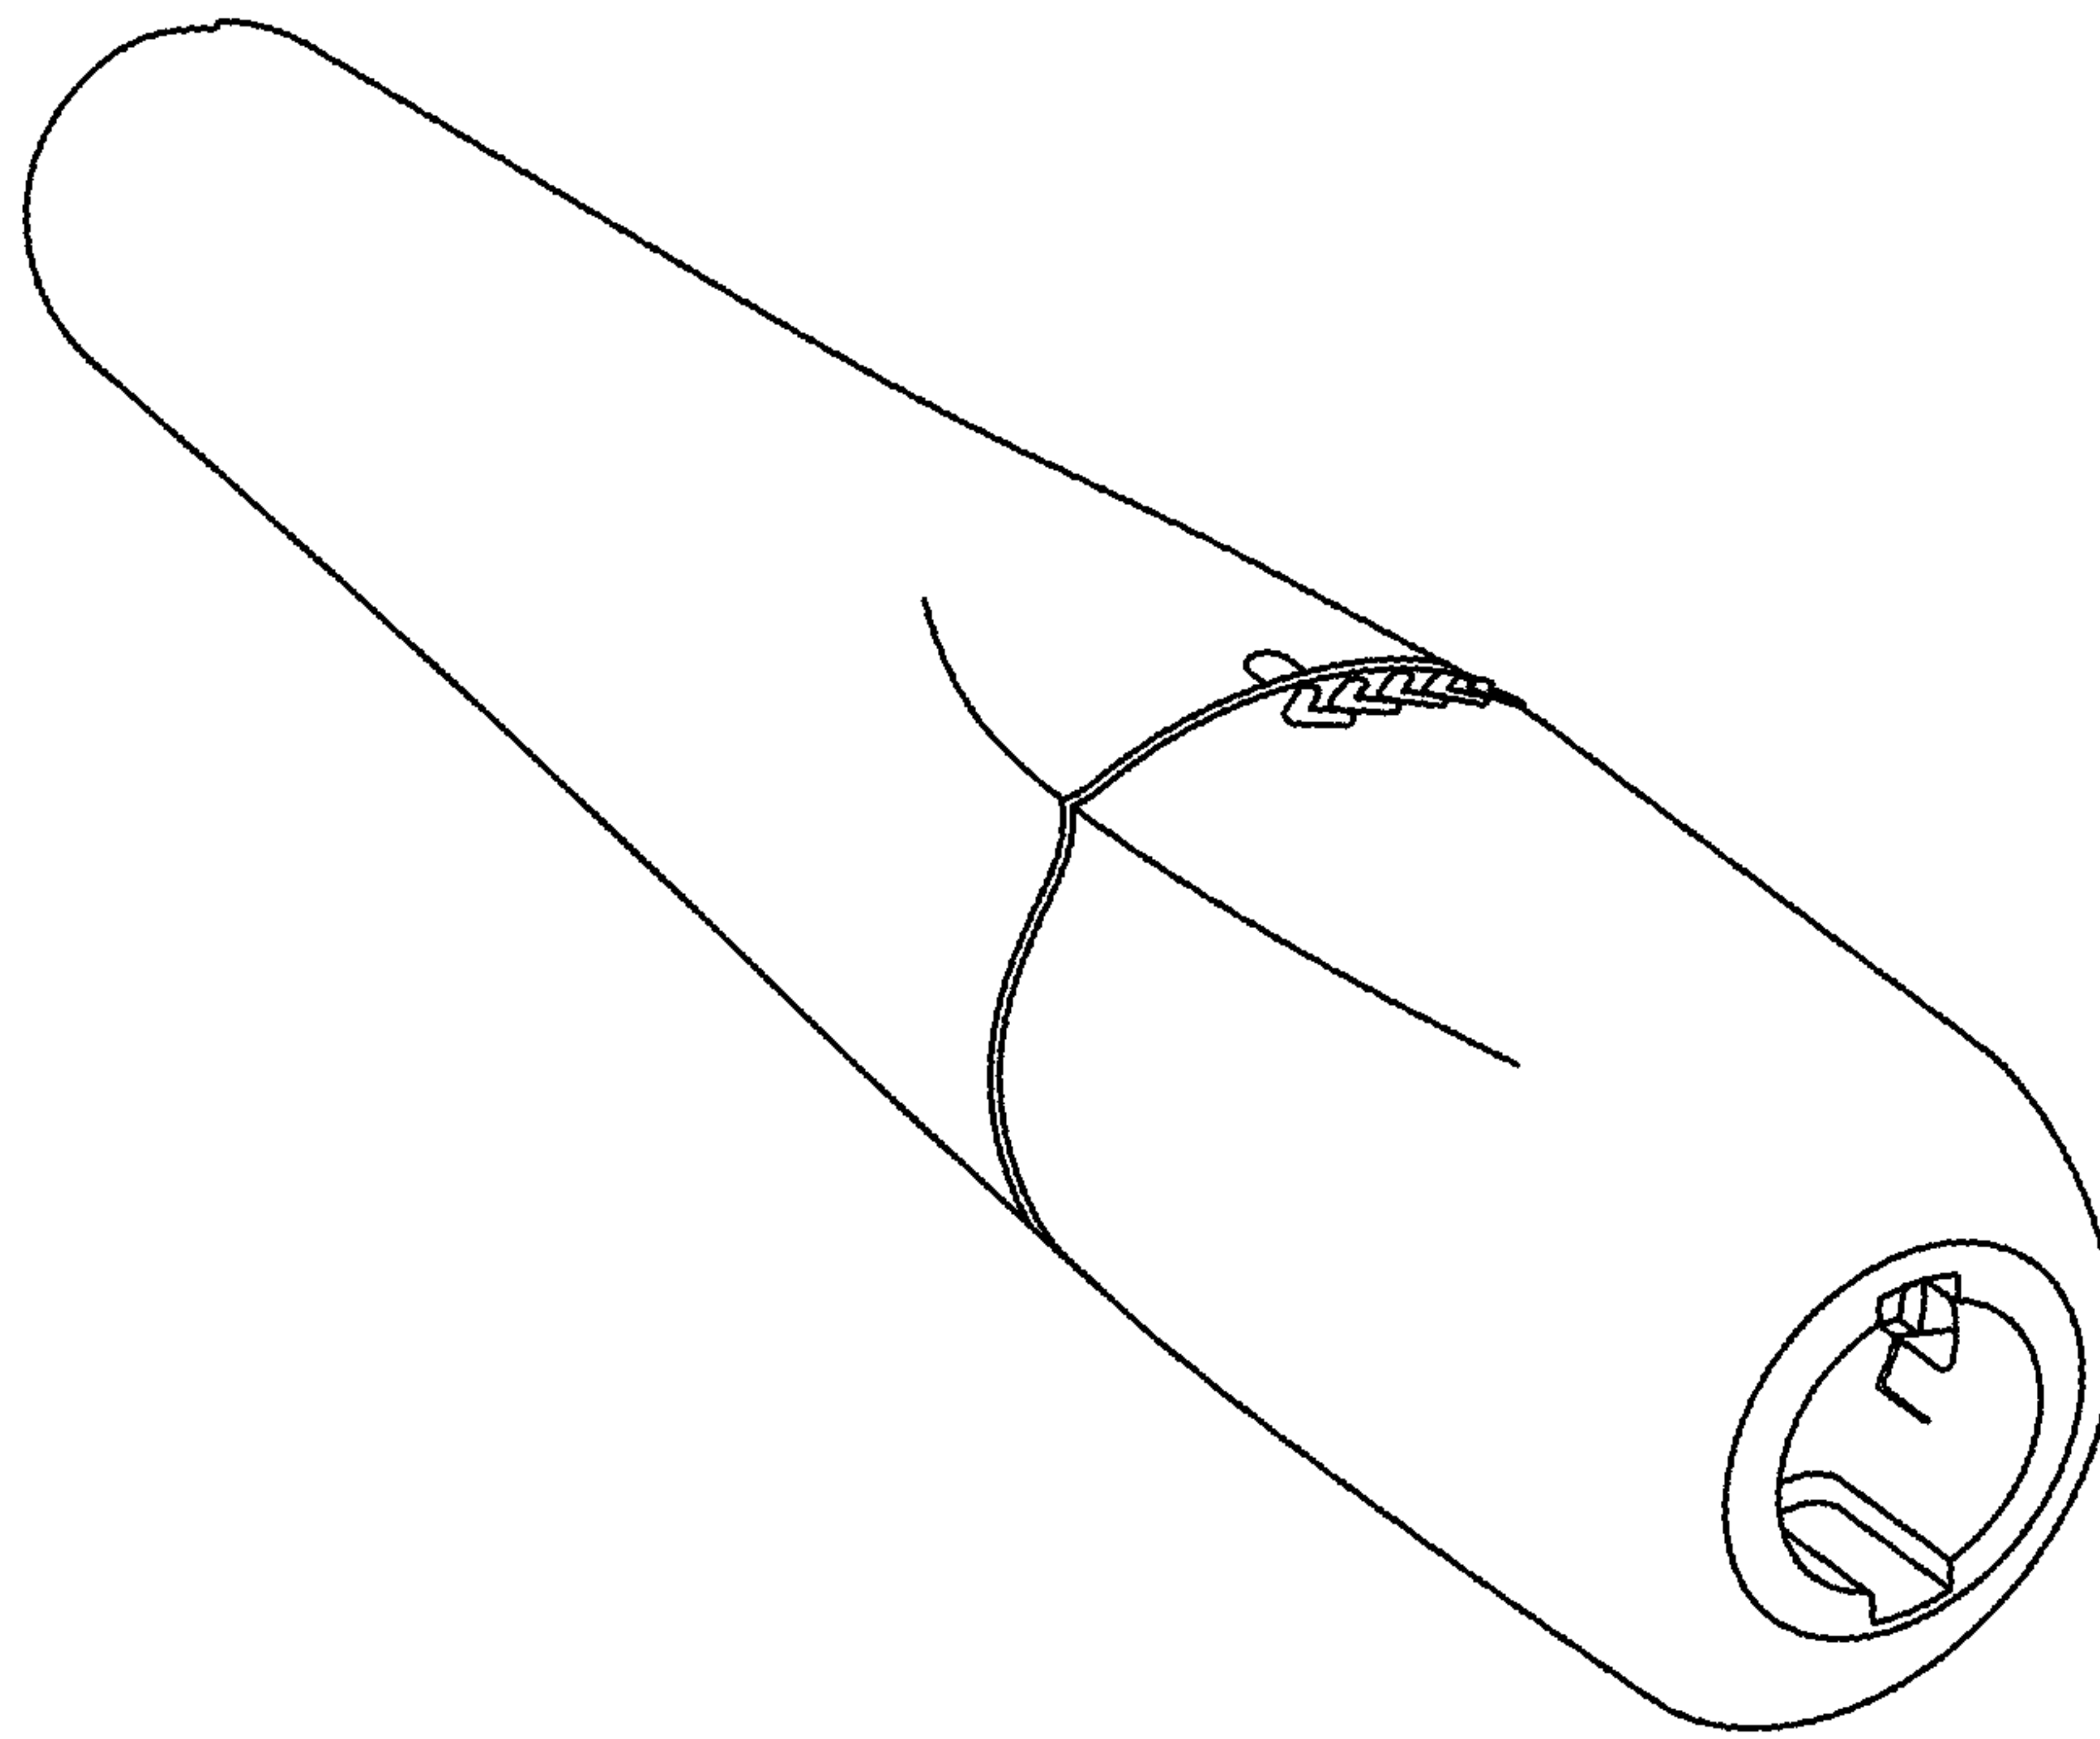


1.1

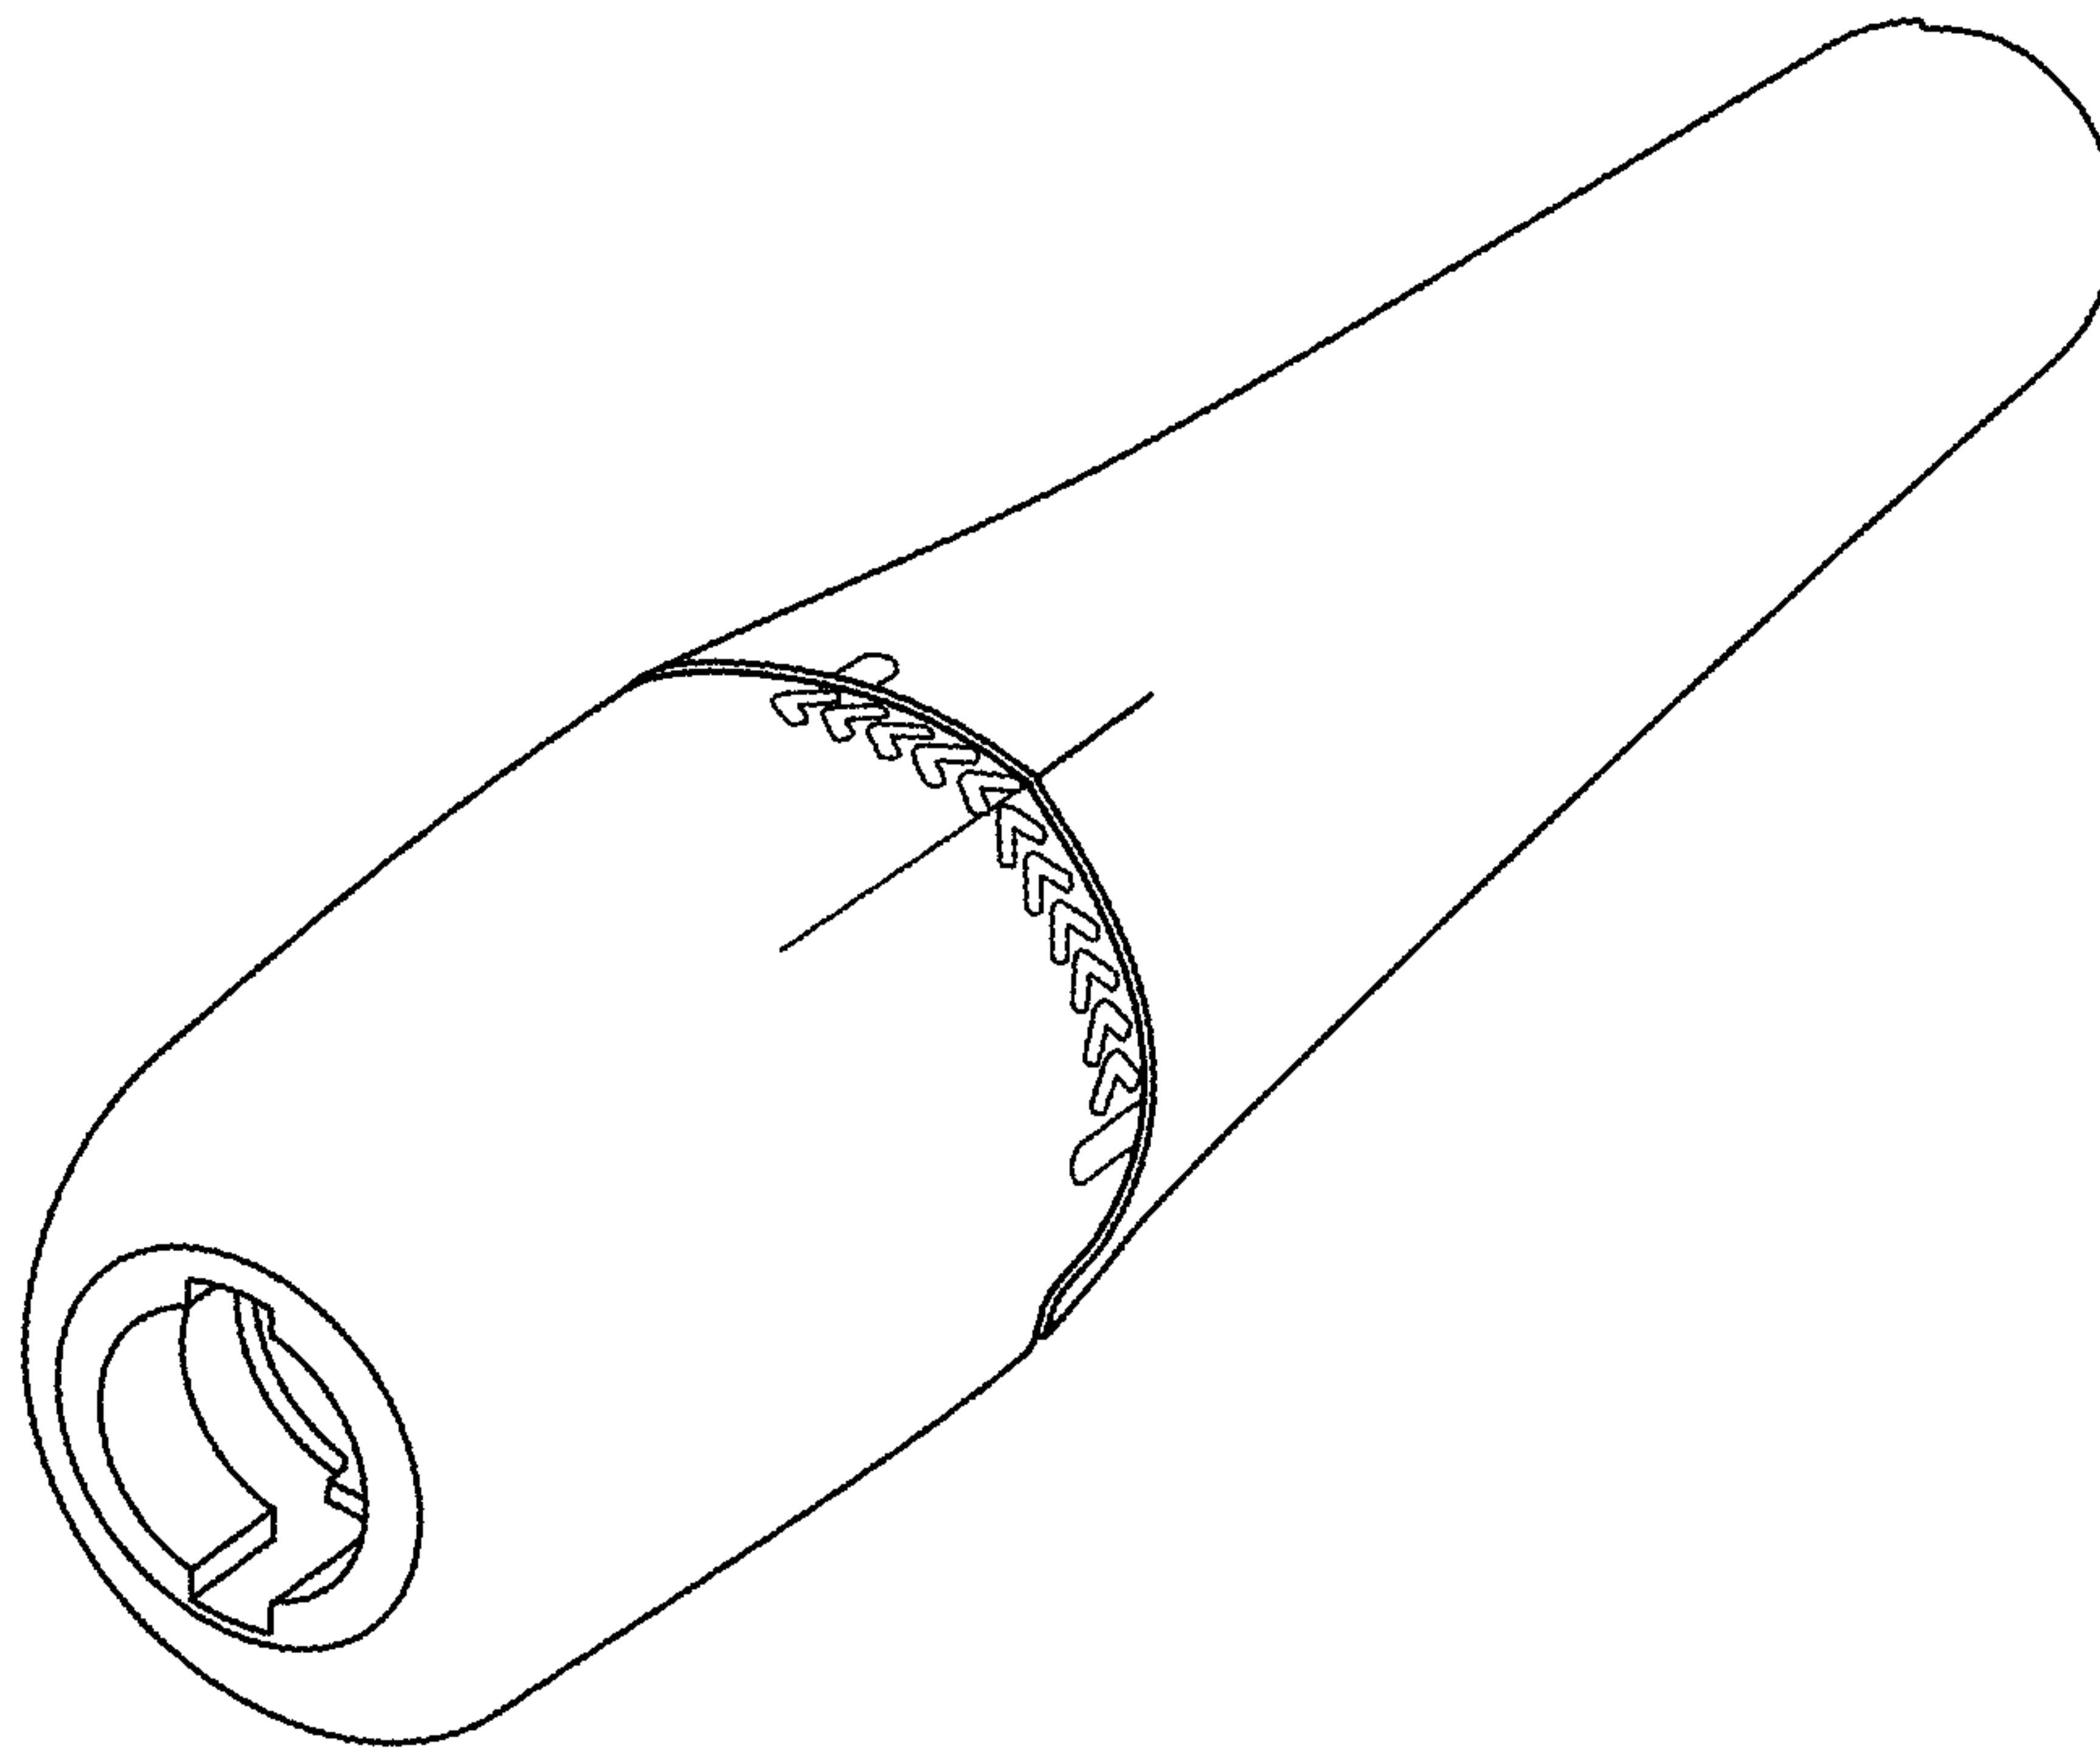


1.2

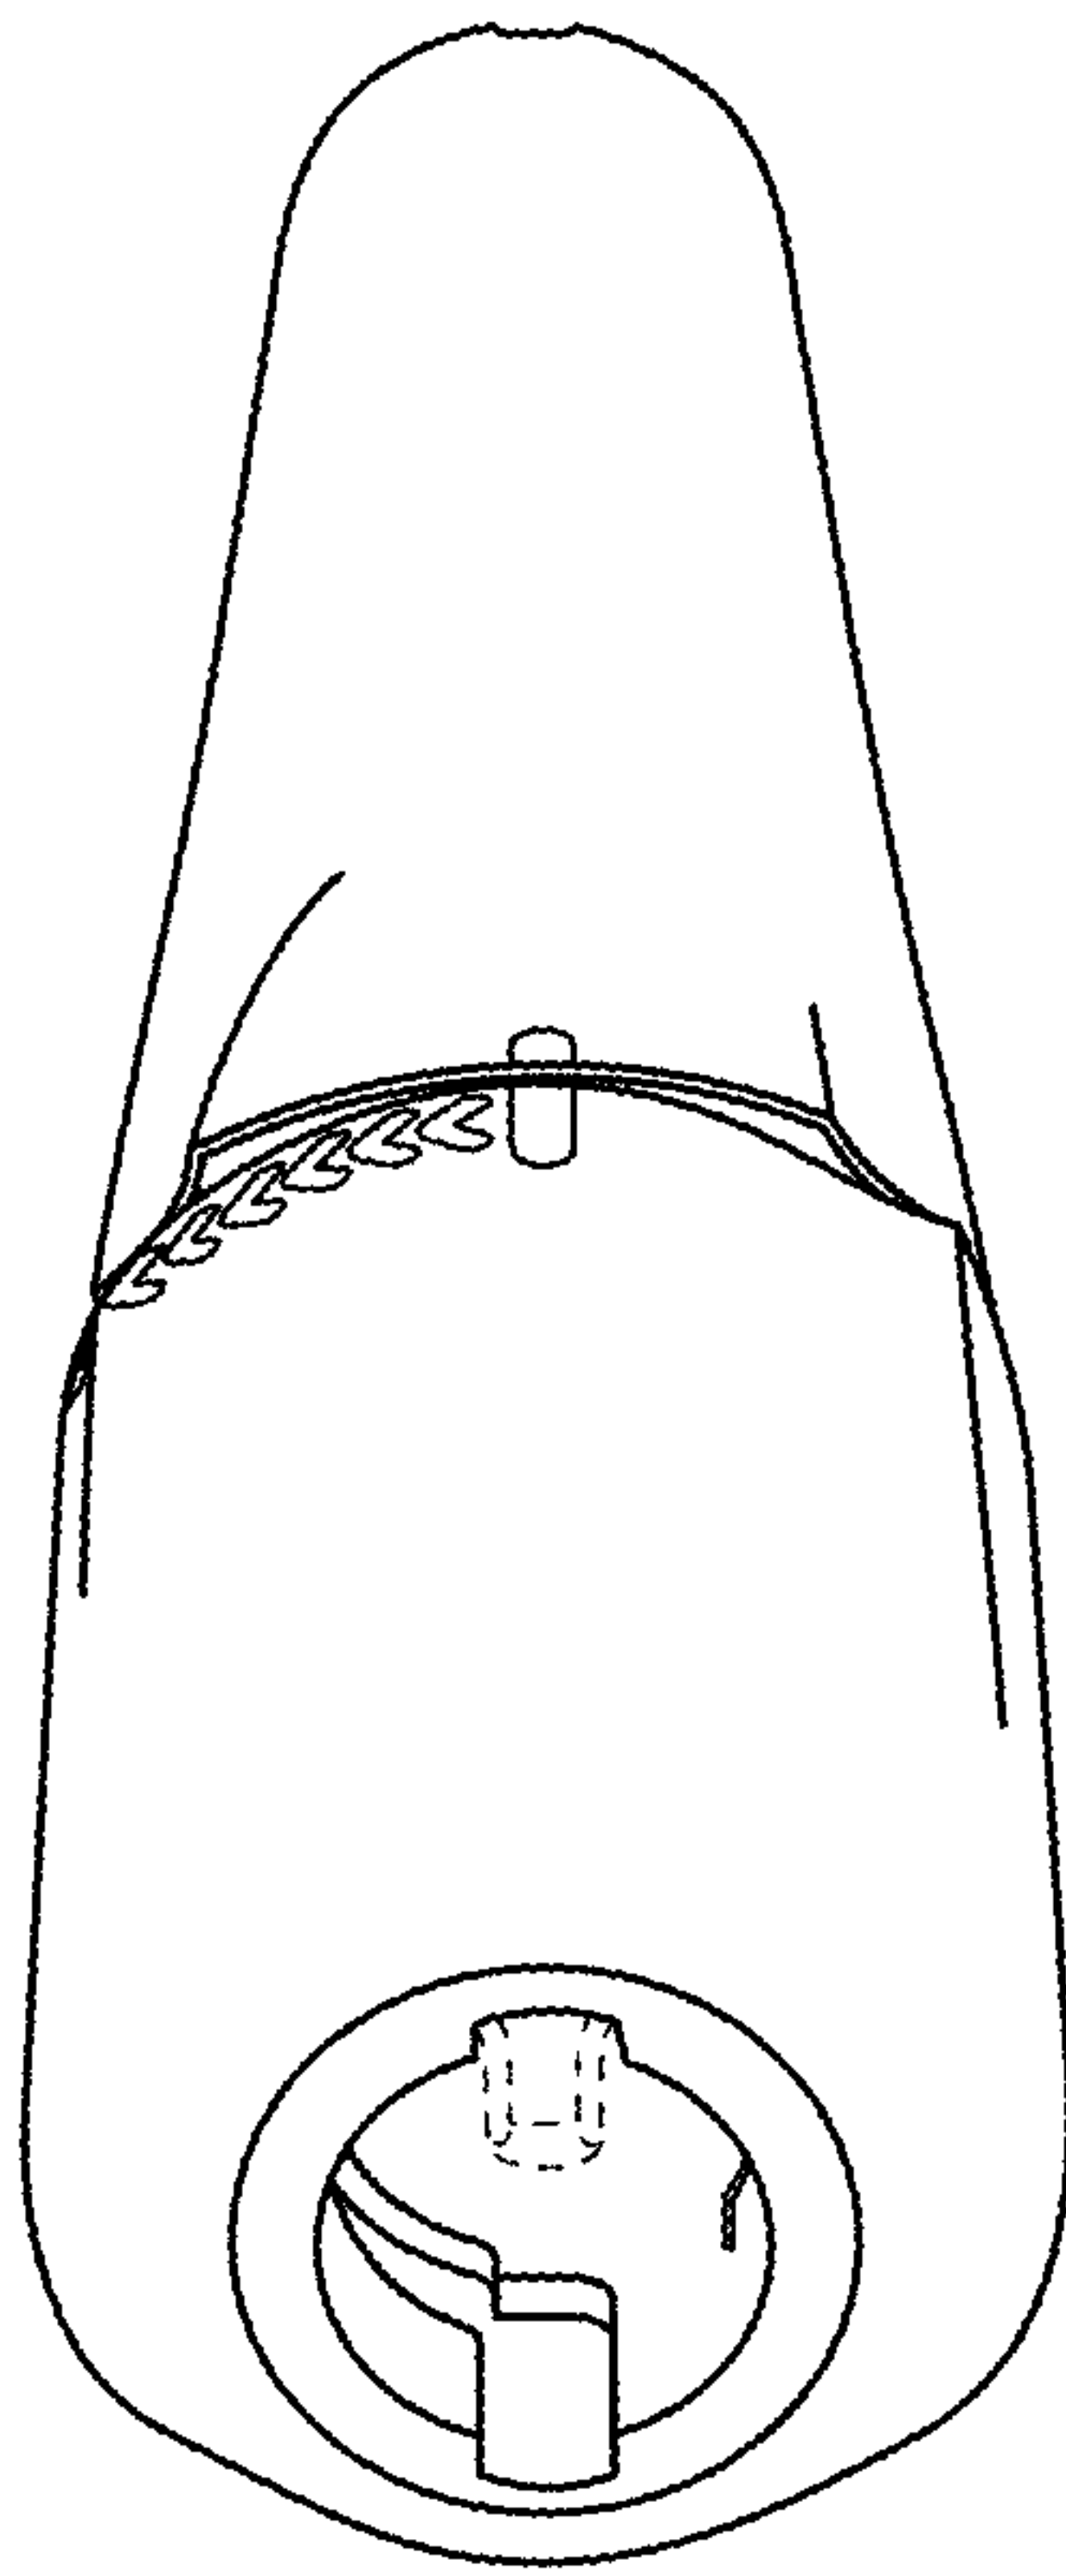


1.3

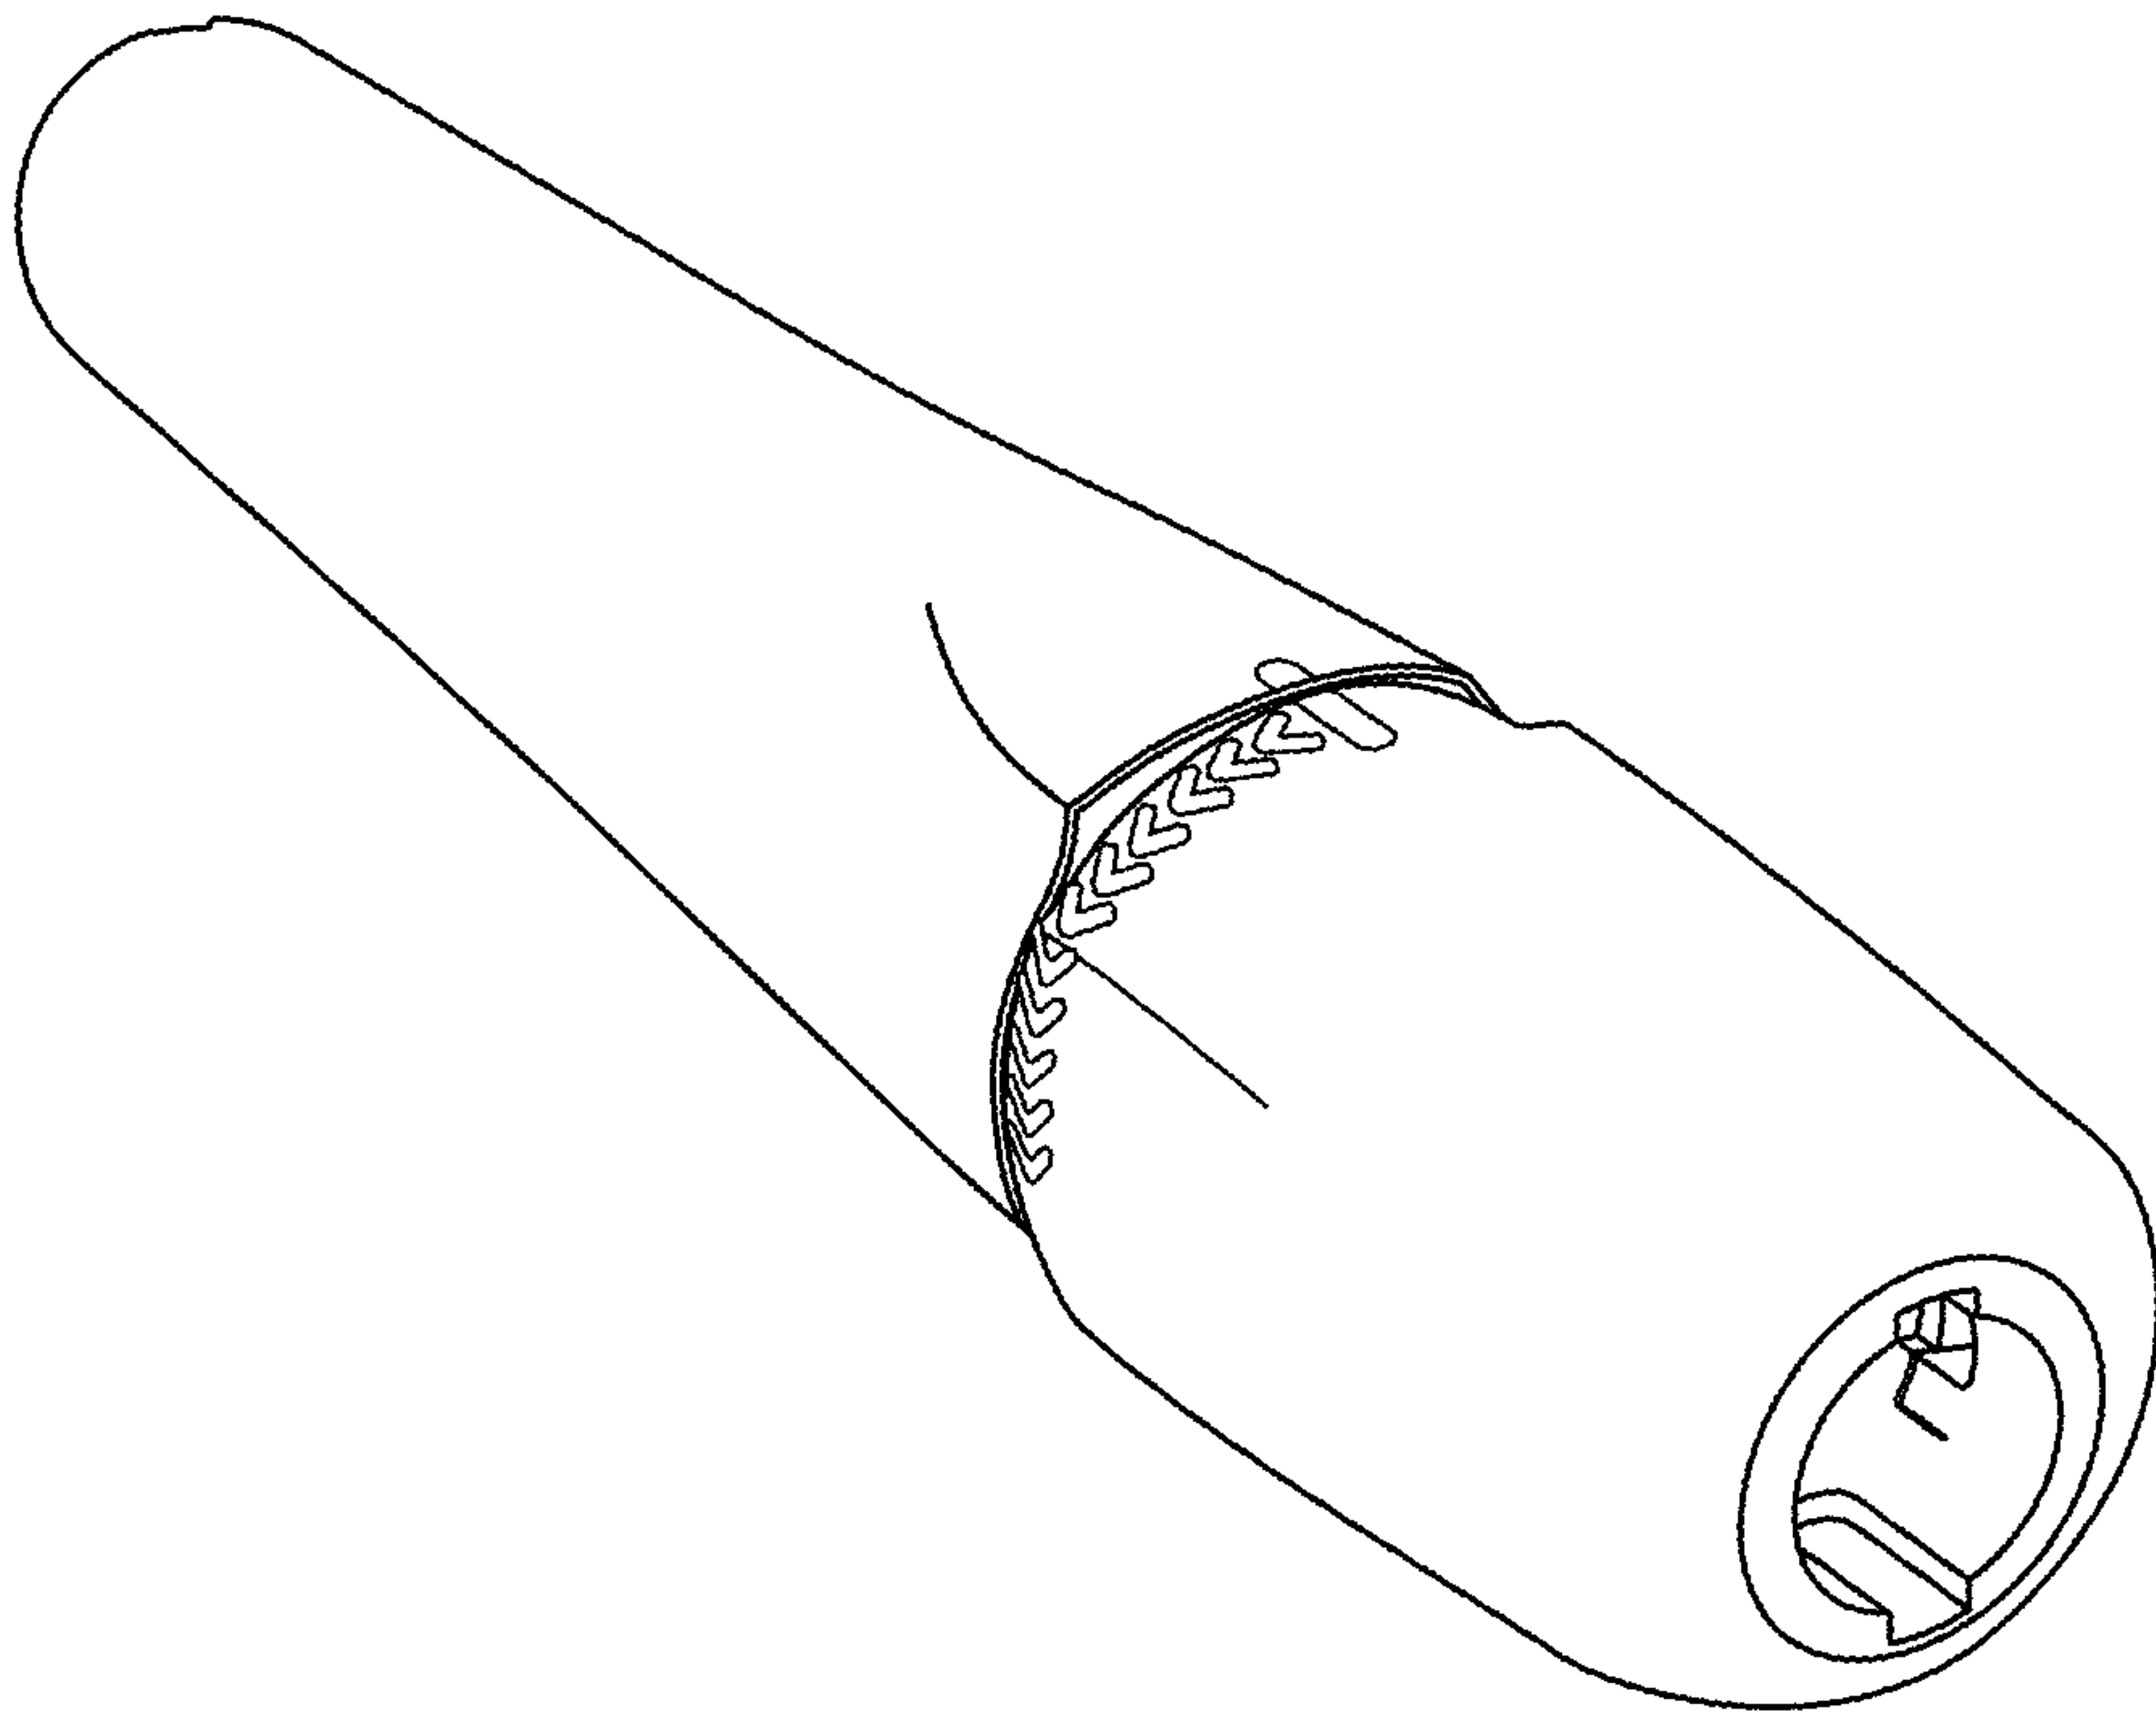

1.4

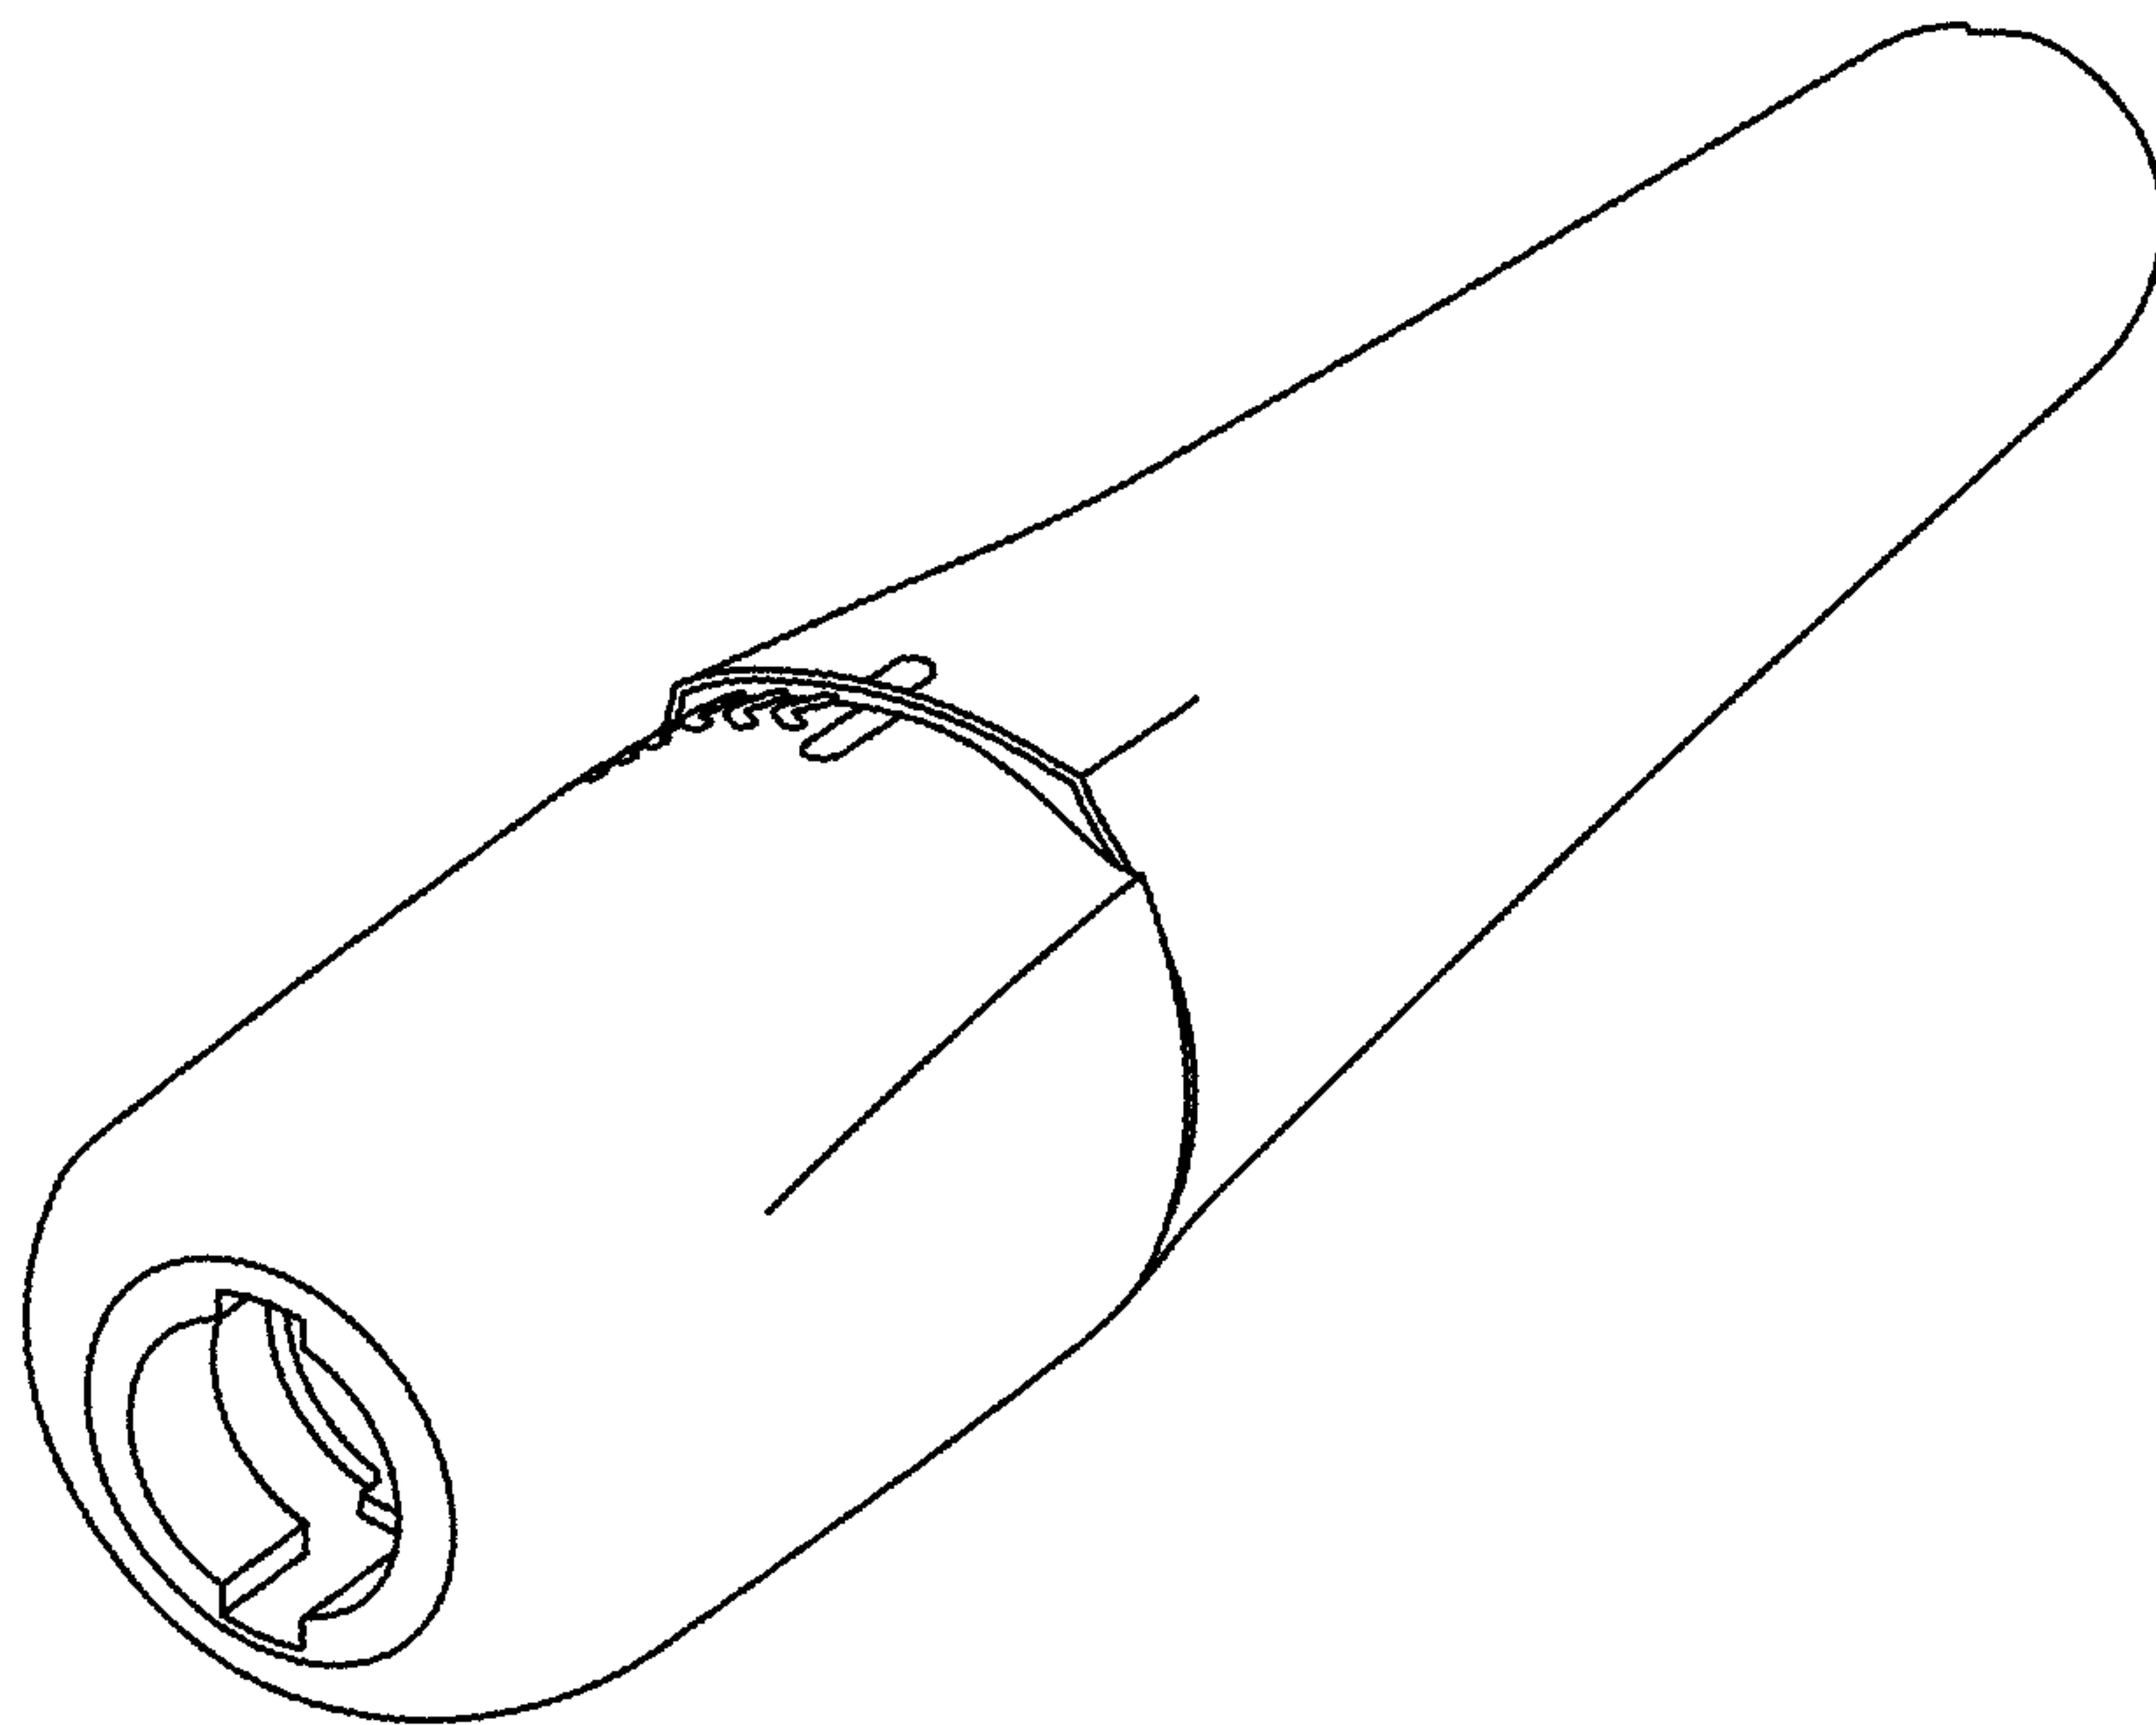


1.5

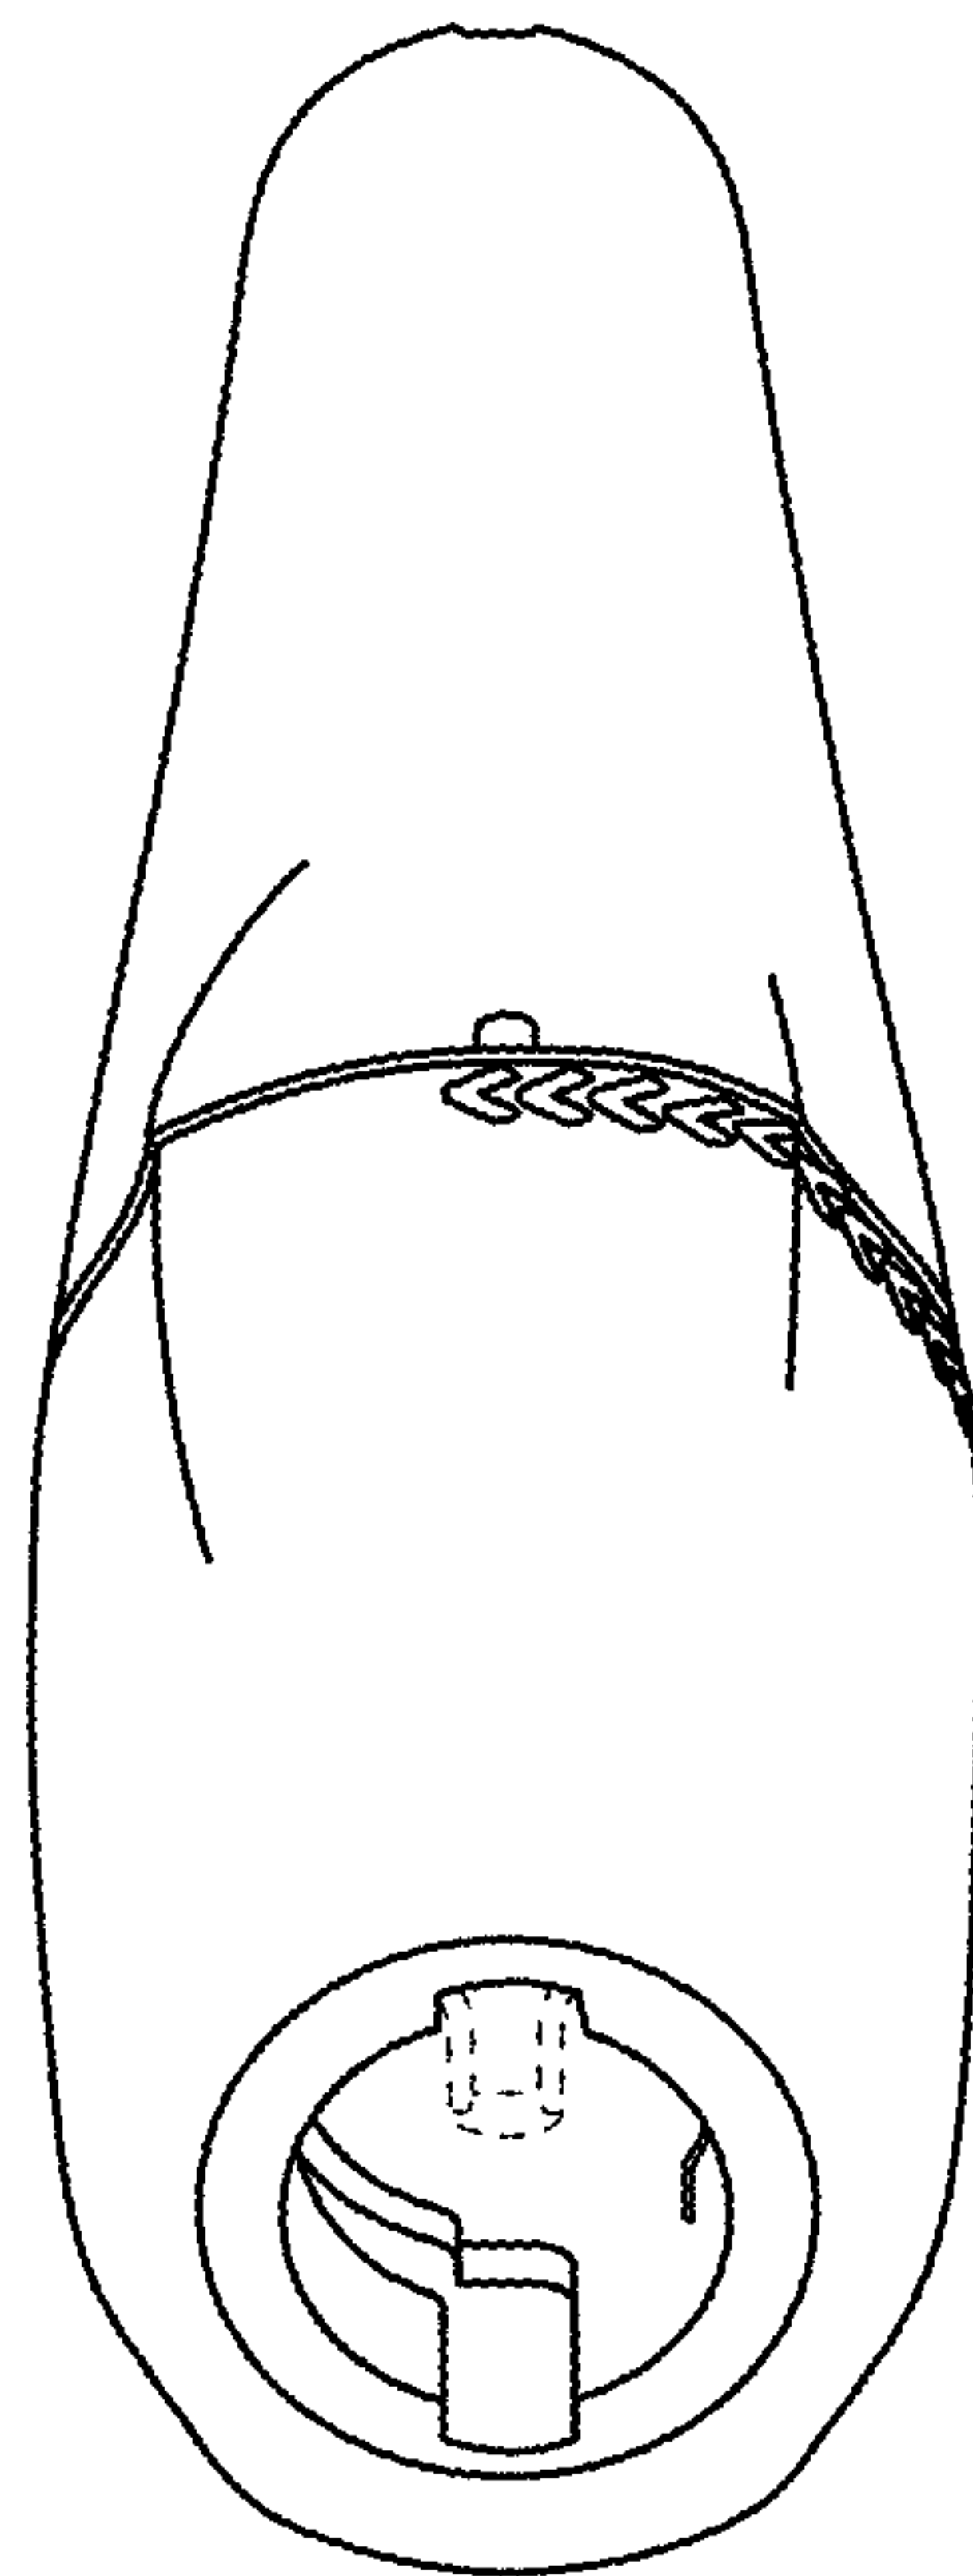


1.6




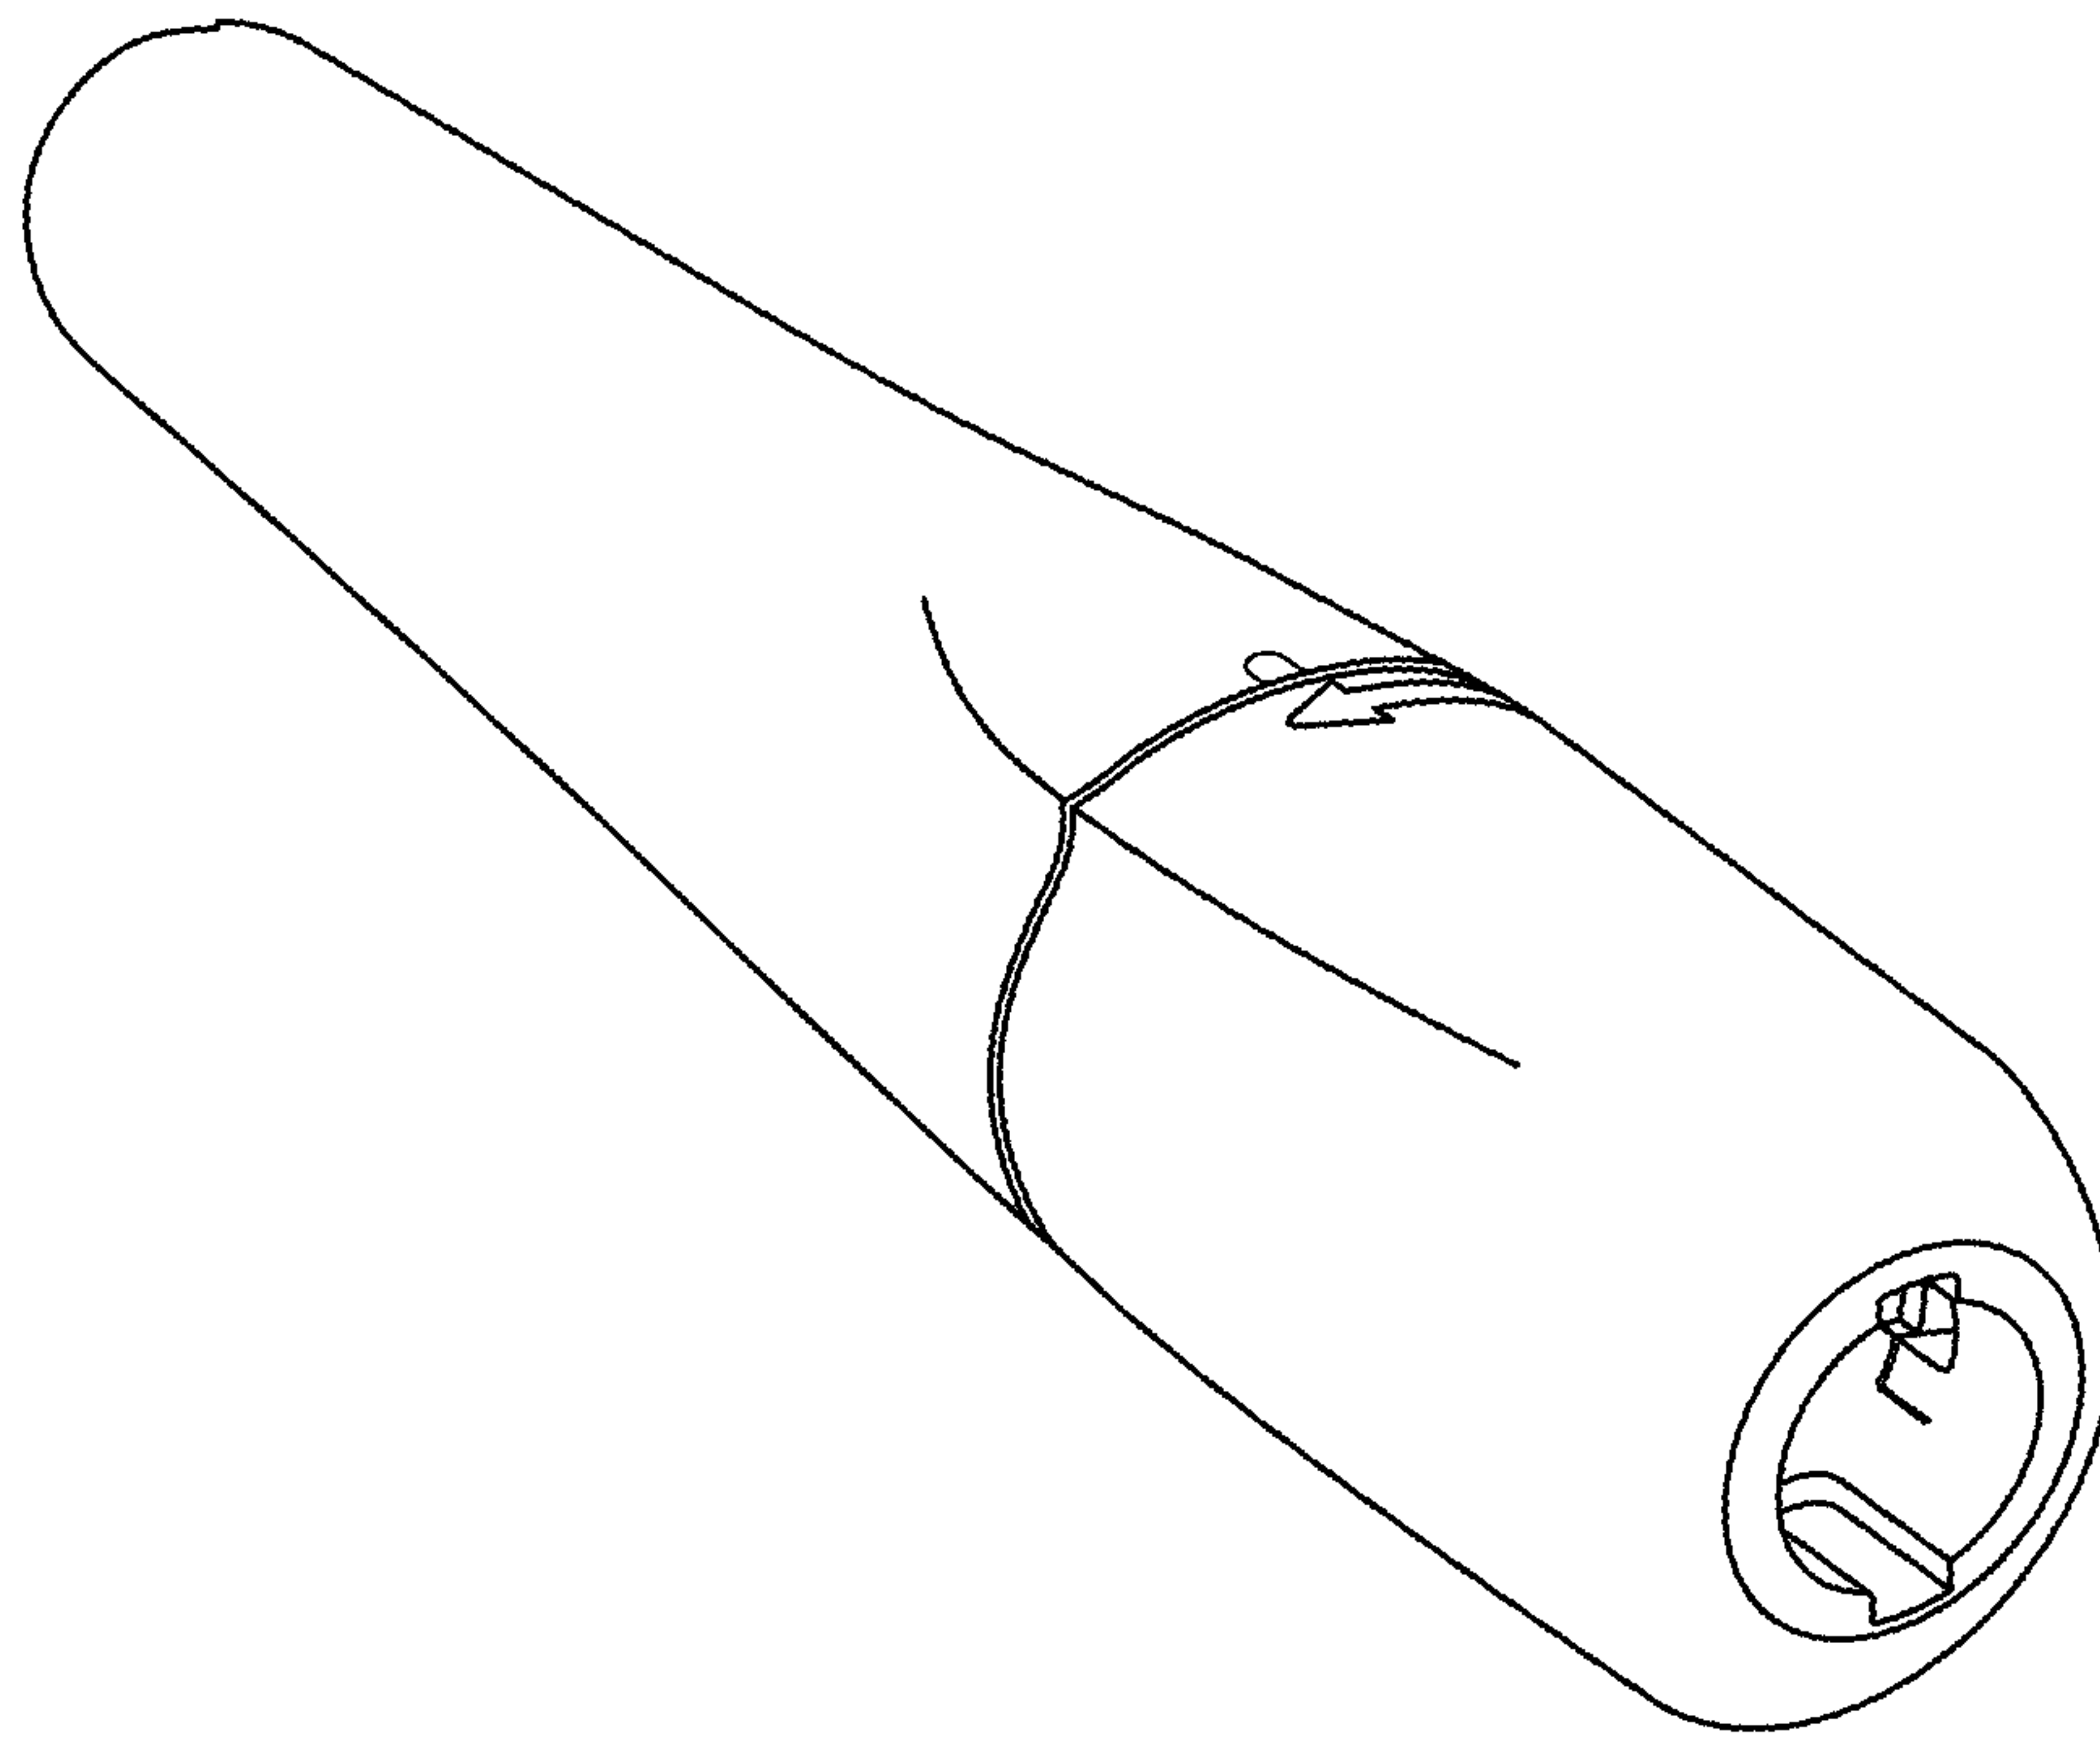


2.1

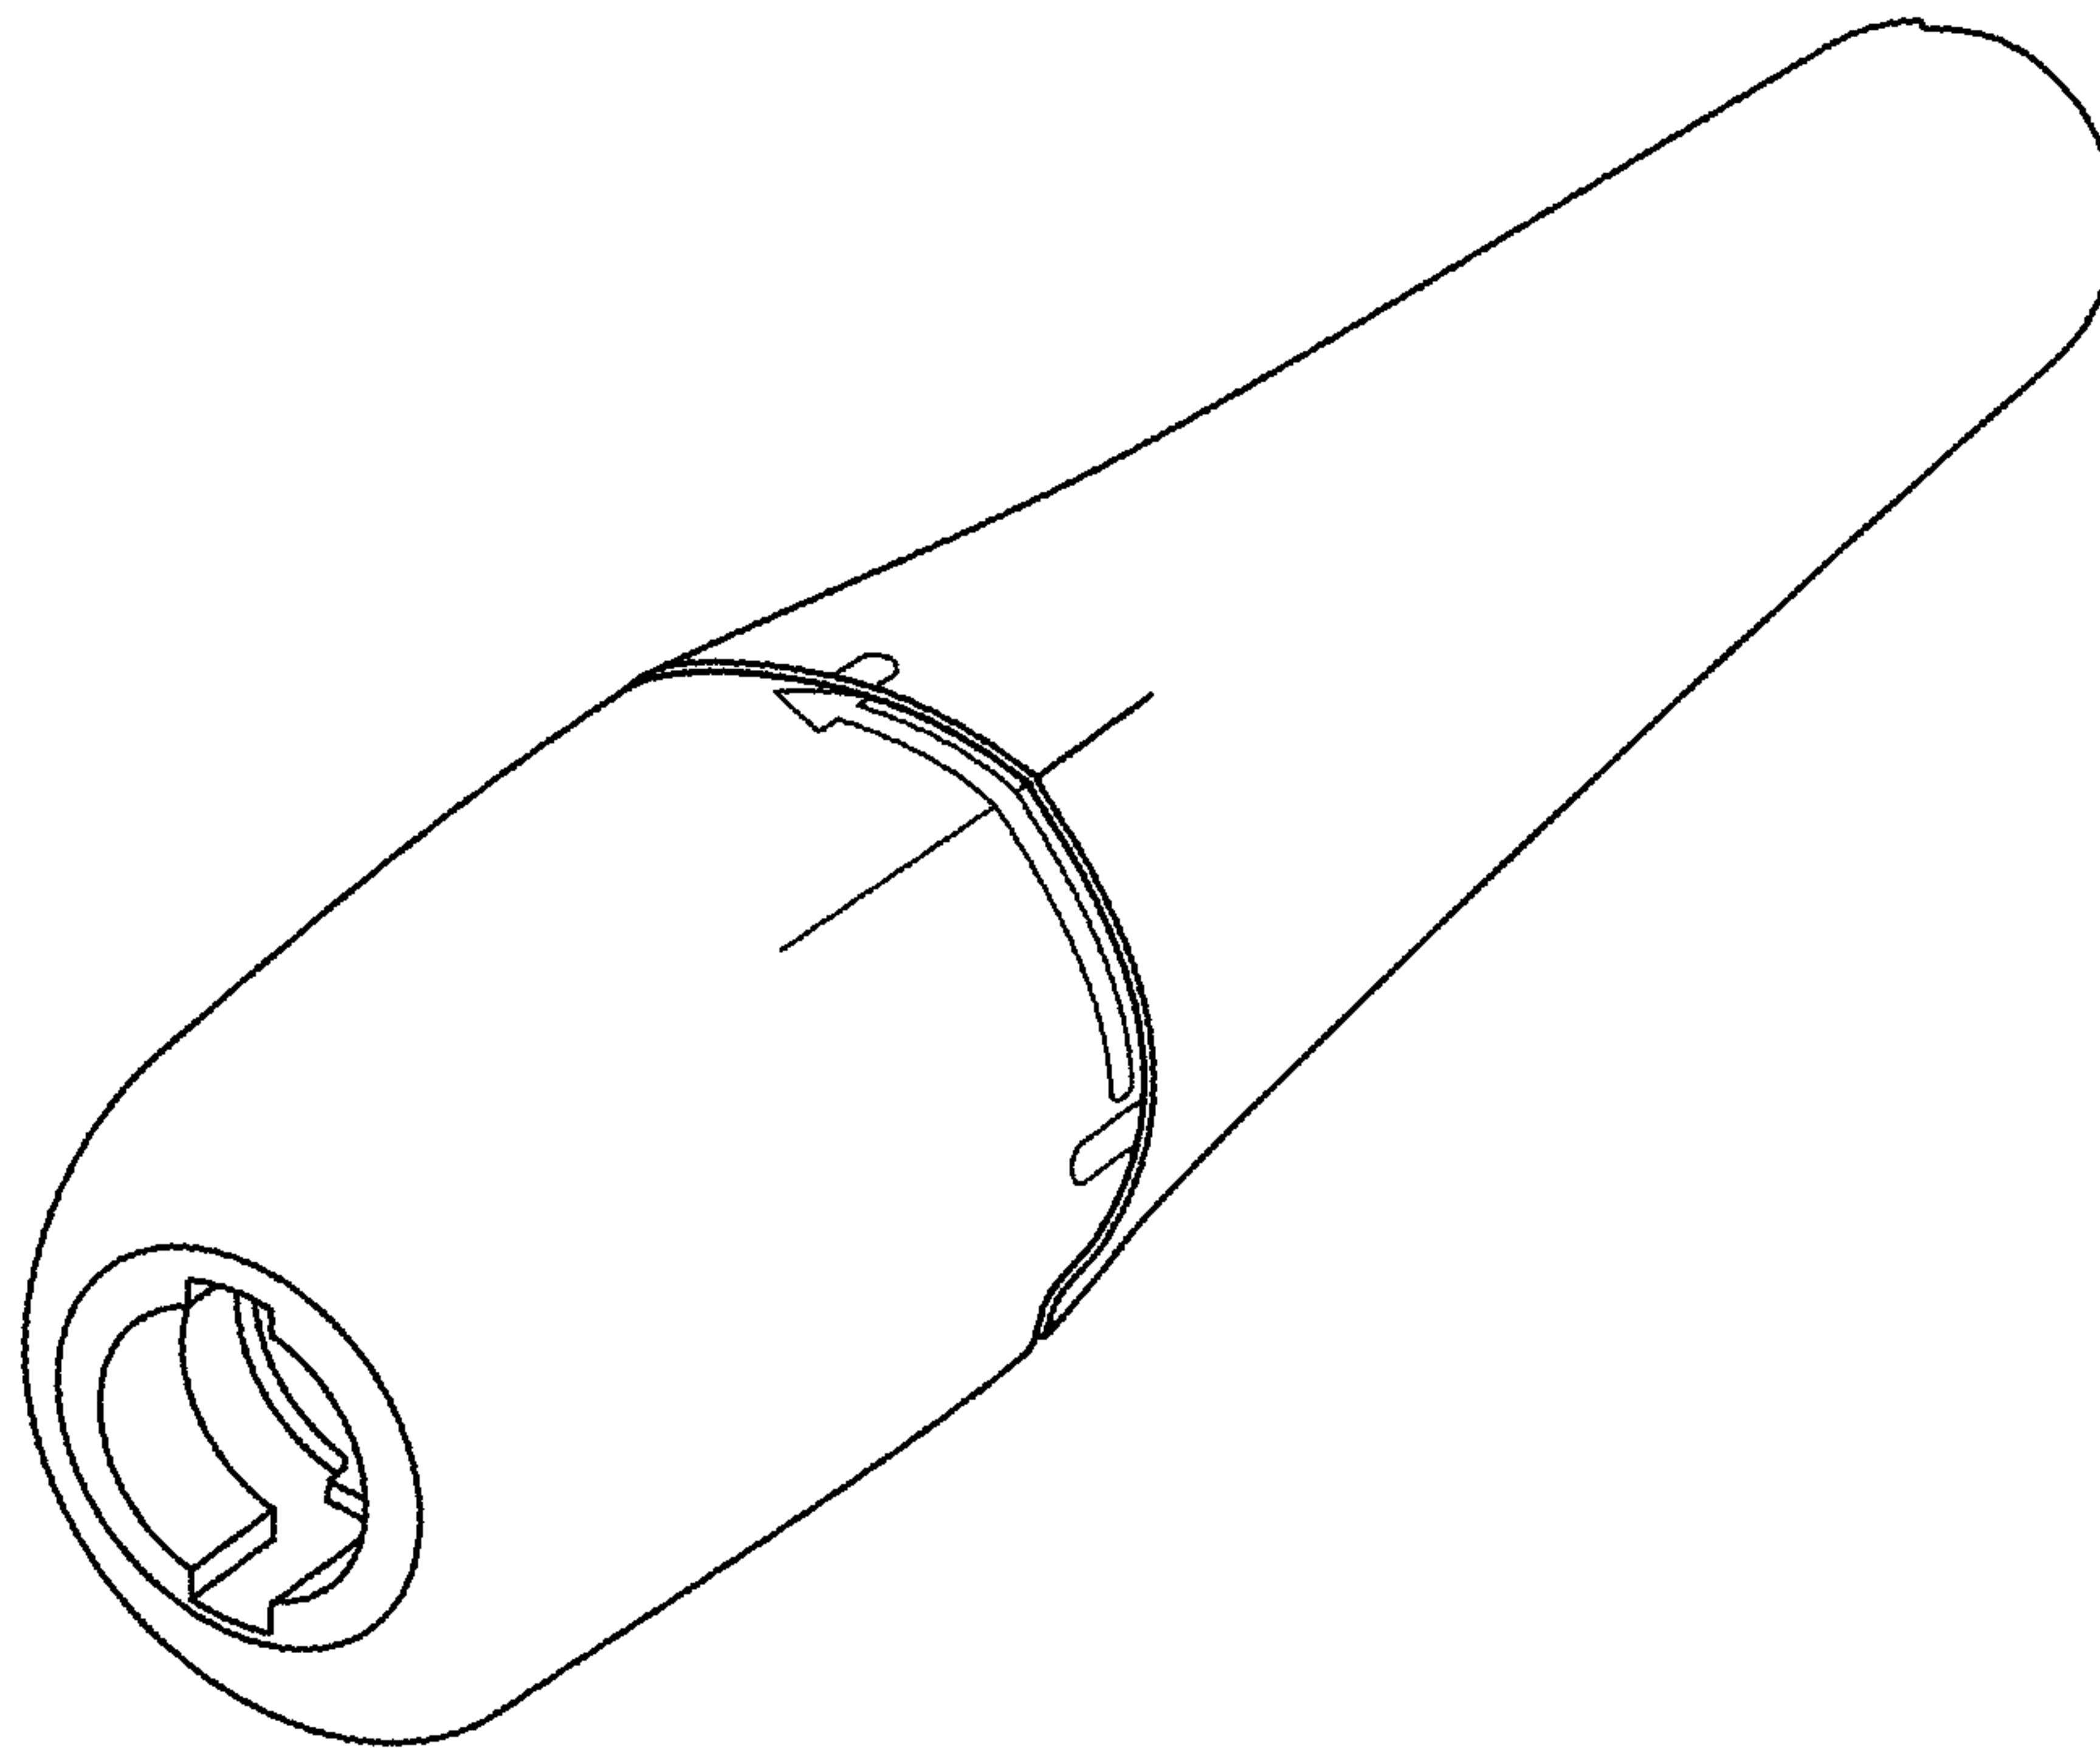


2.2

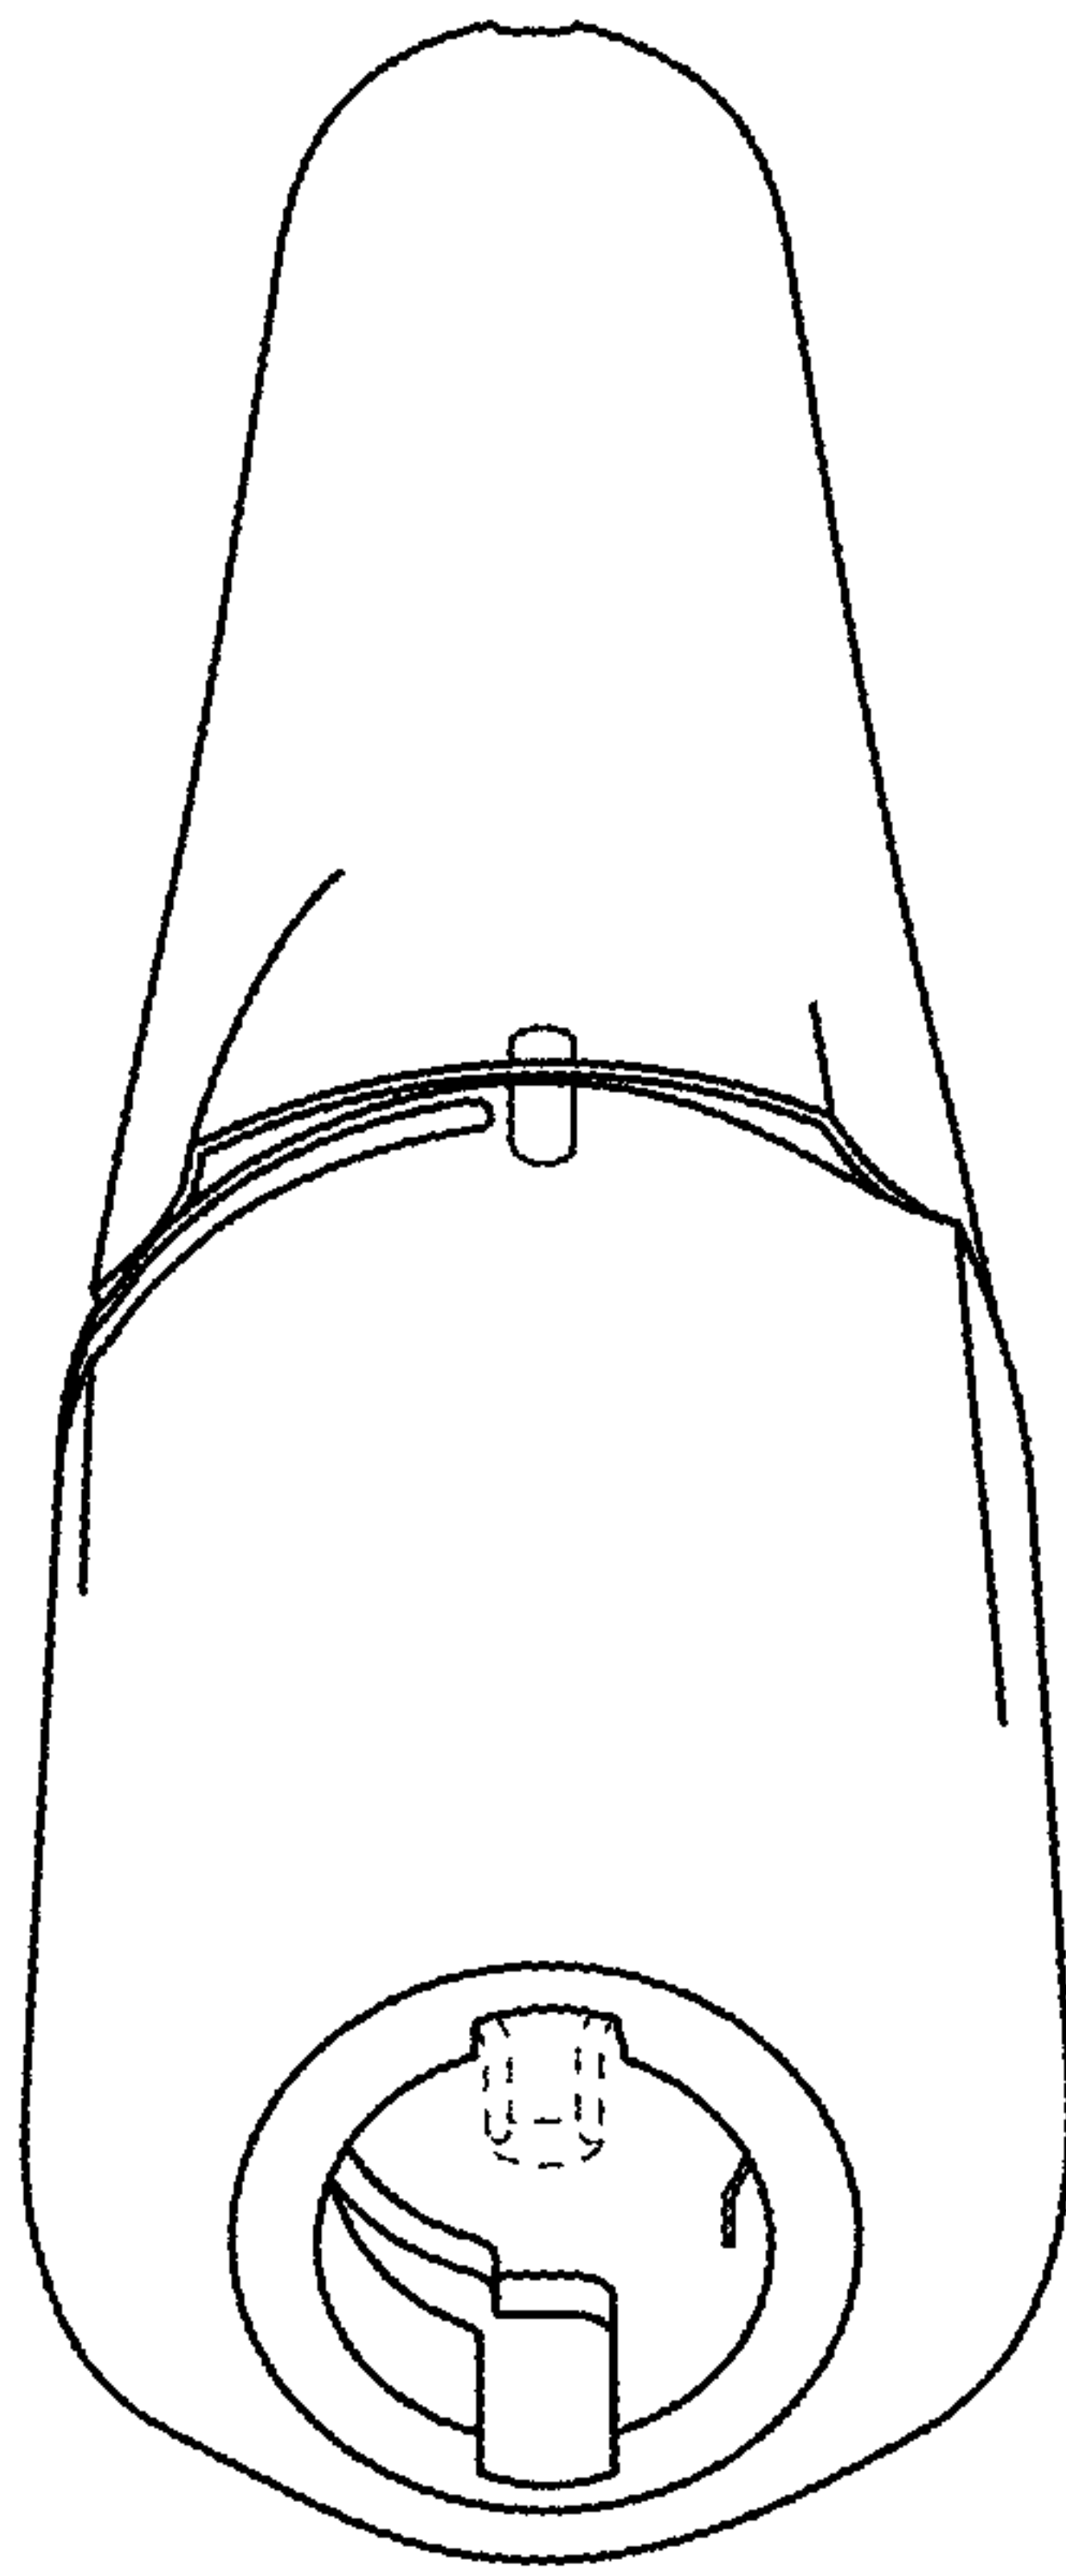


2.3

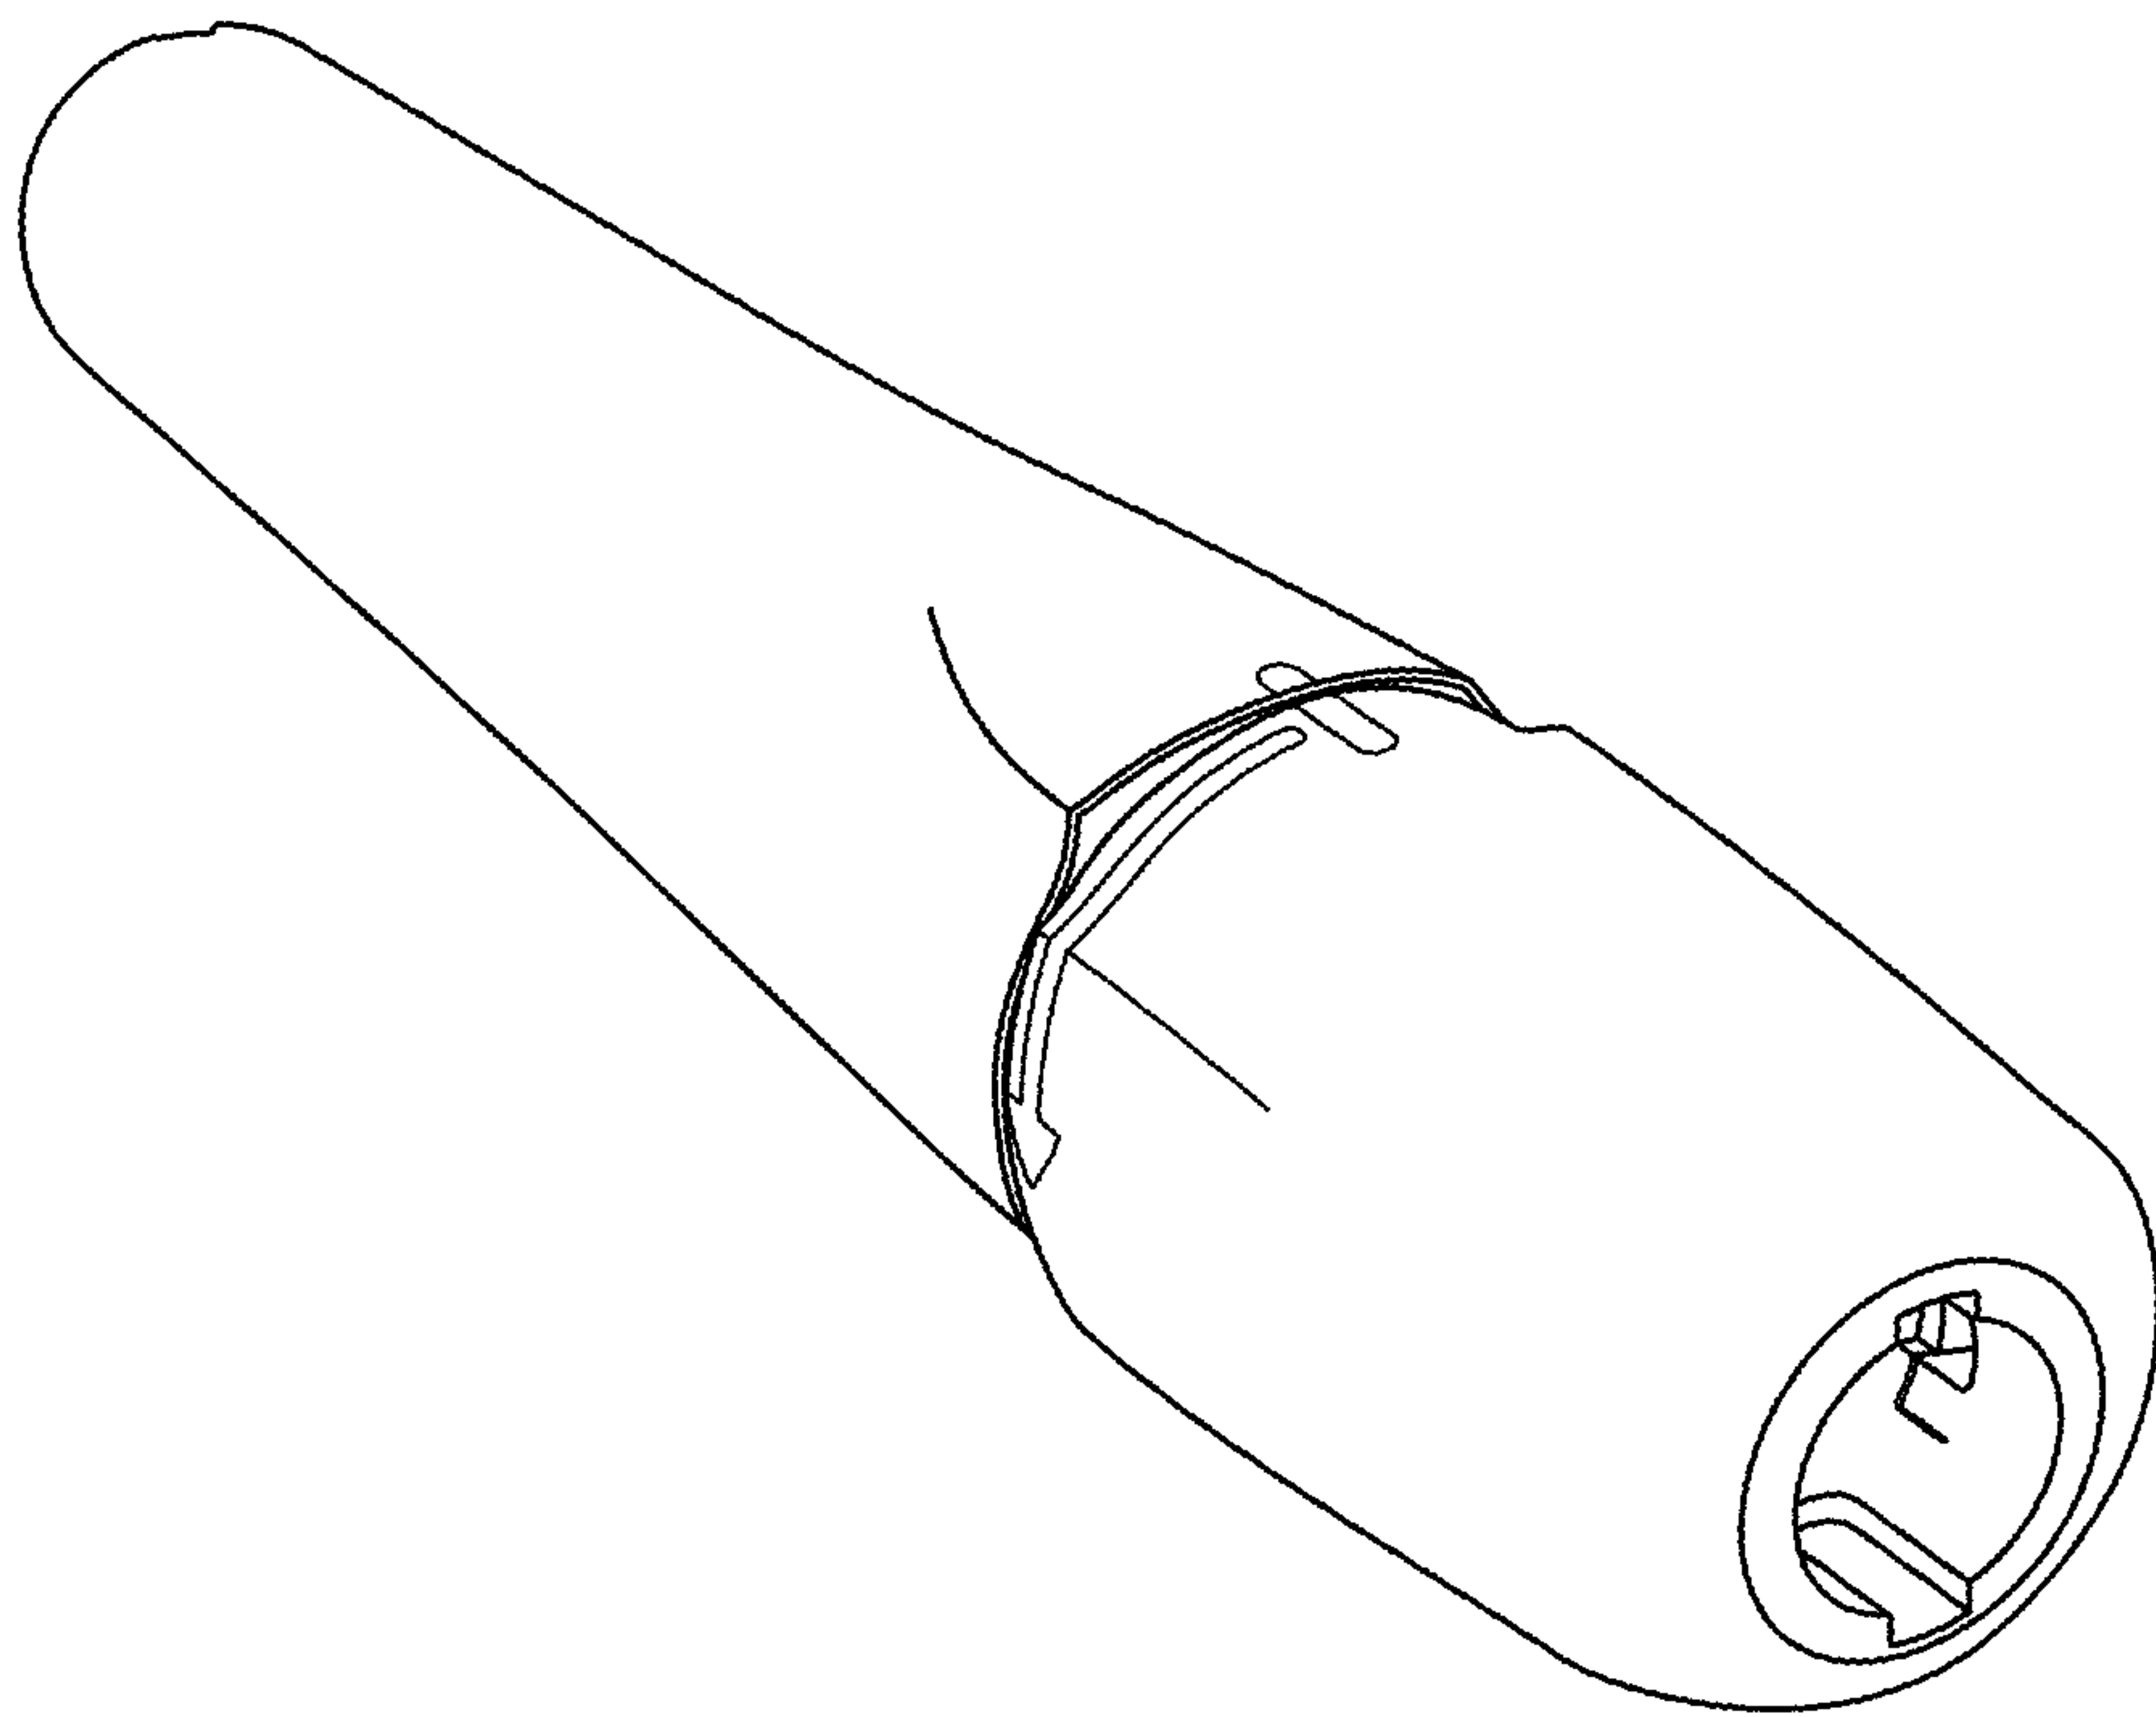

2.4

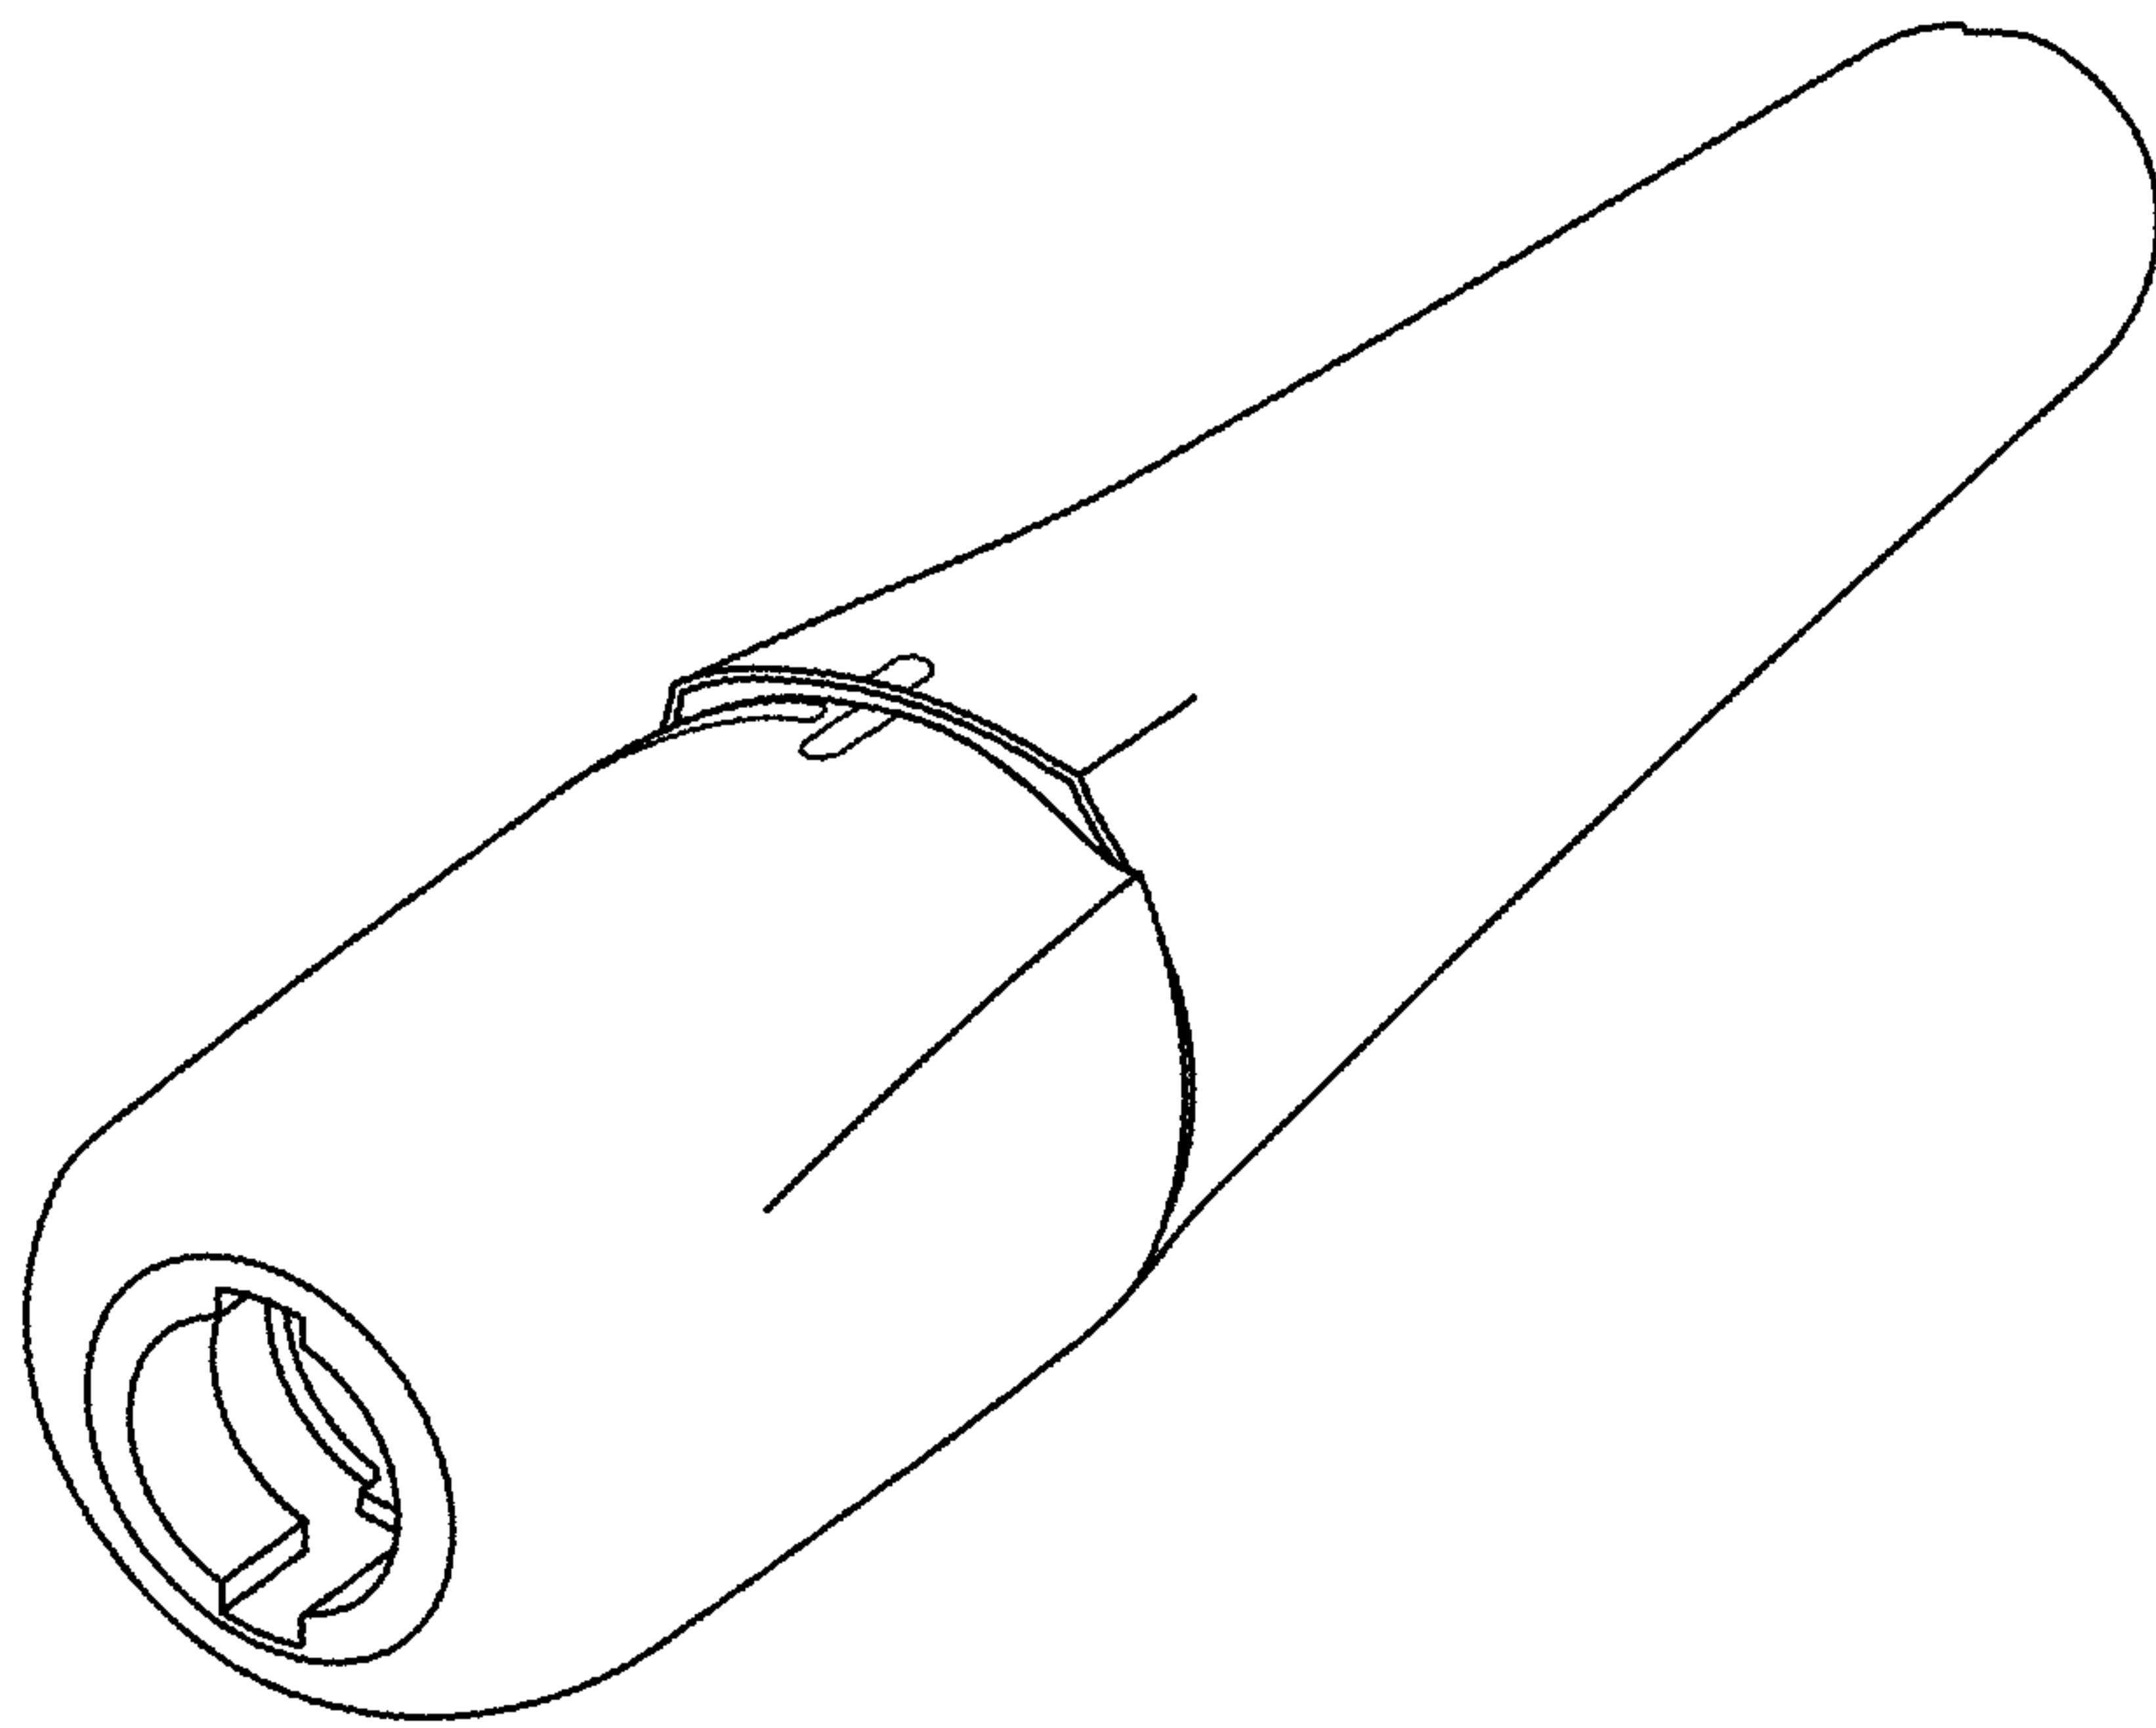

2.5

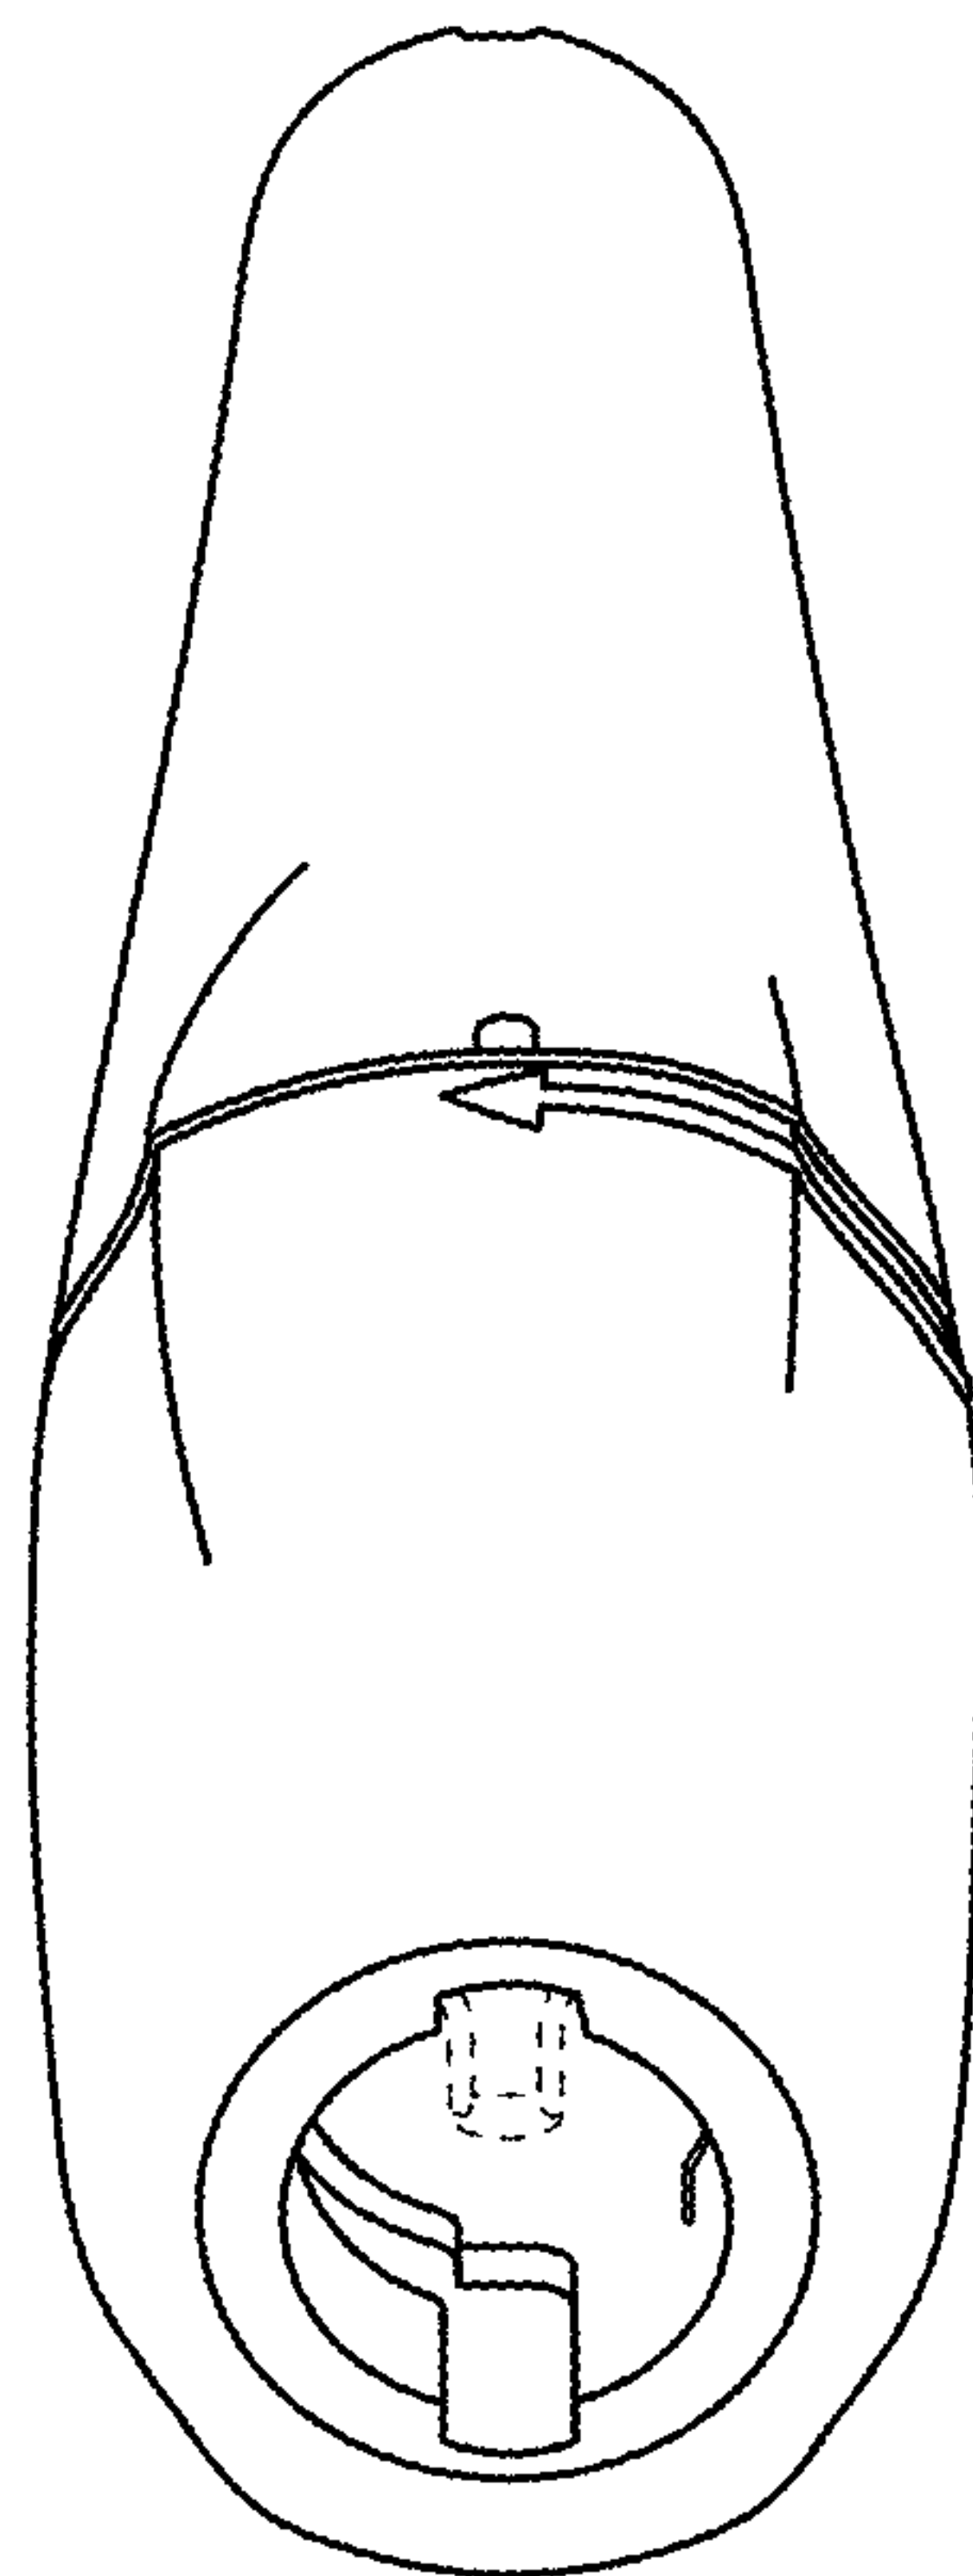

2.6