



US00D982746S

(12) **United States Design Patent**
Woo et al.

(10) **Patent No.:** **US D982,746 S**

(45) **Date of Patent:** **** Apr. 4, 2023**

(54) **MEDICAL DEVICE HOLDER**

(71) Applicant: **CUREXO, INC.**, Seoul (KR)

(72) Inventors: **Dong Gi Woo**, Seoul (KR); **Hong Ho Kim**, Daejeon (KR)

(73) Assignee: **CUREXO, INC.**, Seoul (KR)

(**) Term: **15 Years**

(21) Appl. No.: **29/701,626**

(22) Filed: **Aug. 13, 2019**

(30) **Foreign Application Priority Data**

Feb. 13, 2019 (KR) 30-2019-0006478

(51) **LOC (14) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/128**

(58) **Field of Classification Search**
USPC D24/158-161, 185, 186, 128; D14/452;
D8/355, 363

CPC .. A61B 1/00188; A61B 1/00149; A61B 1/042
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,863,133	A *	9/1989	Bonnell	F16M 11/2021
					403/56
D435,852	S *	1/2001	Oddsens, Jr.	D14/452
D495,240	S *	8/2004	Mnich	D8/355
D507,477	S *	7/2005	Pfister	D14/451
D537,323	S *	2/2007	Saez	D14/452
D584,734	S *	1/2009	Chu	D14/452
D611,802	S *	3/2010	Li	D8/363
D631,052	S *	1/2011	Hung	D14/452
D679,282	S *	4/2013	Liu	D14/452
D745,873	S *	12/2015	Xiang	D14/452
D746,474	S *	12/2015	Koros	D24/128

D796,519	S *	9/2017	Hung	D14/452
D822,671	S *	7/2018	Chu	D14/452
D830,371	S *	10/2018	Lau	D14/452
D837,387	S *	1/2019	Vollum	D24/185
D843,379	S *	3/2019	Lindo	D14/452
D848,444	S *	5/2019	Jung	D14/452
D871,588	S *	12/2019	Schultz	D24/185
D922,394	S *	6/2021	Lu	D14/452
D926,196	S *	7/2021	Lyu	D14/452
D931,292	S *	9/2021	Kleist	D14/452
D936,069	S *	11/2021	You	D14/452
D936,070	S *	11/2021	You	D14/452
D936,071	S *	11/2021	You	D14/452
D951,962	S *	5/2022	You	D14/452
2018/0071049	A1 *	3/2018	Nowatschin	A61B 1/00149

* cited by examiner

Primary Examiner — Nathan M Johnston

(74) *Attorney, Agent, or Firm* — Bridgeway IP Law Group, PLLC; Jihun Kim

(57) **CLAIM**

We claim the ornamental design for a medical device holder, as shown and described.

DESCRIPTION

FIG. 1 is perspective view of a medical device holder, showing our new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left side elevational view thereof;

FIG. 5 is a right side elevational view thereof;

FIG. 6 is a top plan view thereof;


FIG. 7 is a bottom plan view thereof;

FIG. 8 is an enlarged view of FIG. 1; and,

FIG. 9 is a reference view thereof showing a configuration of use.

The broken lines in the drawings show portions of the medical device holder or show environmental structure which form no part of the claimed design.

1 Claim, 8 Drawing Sheets

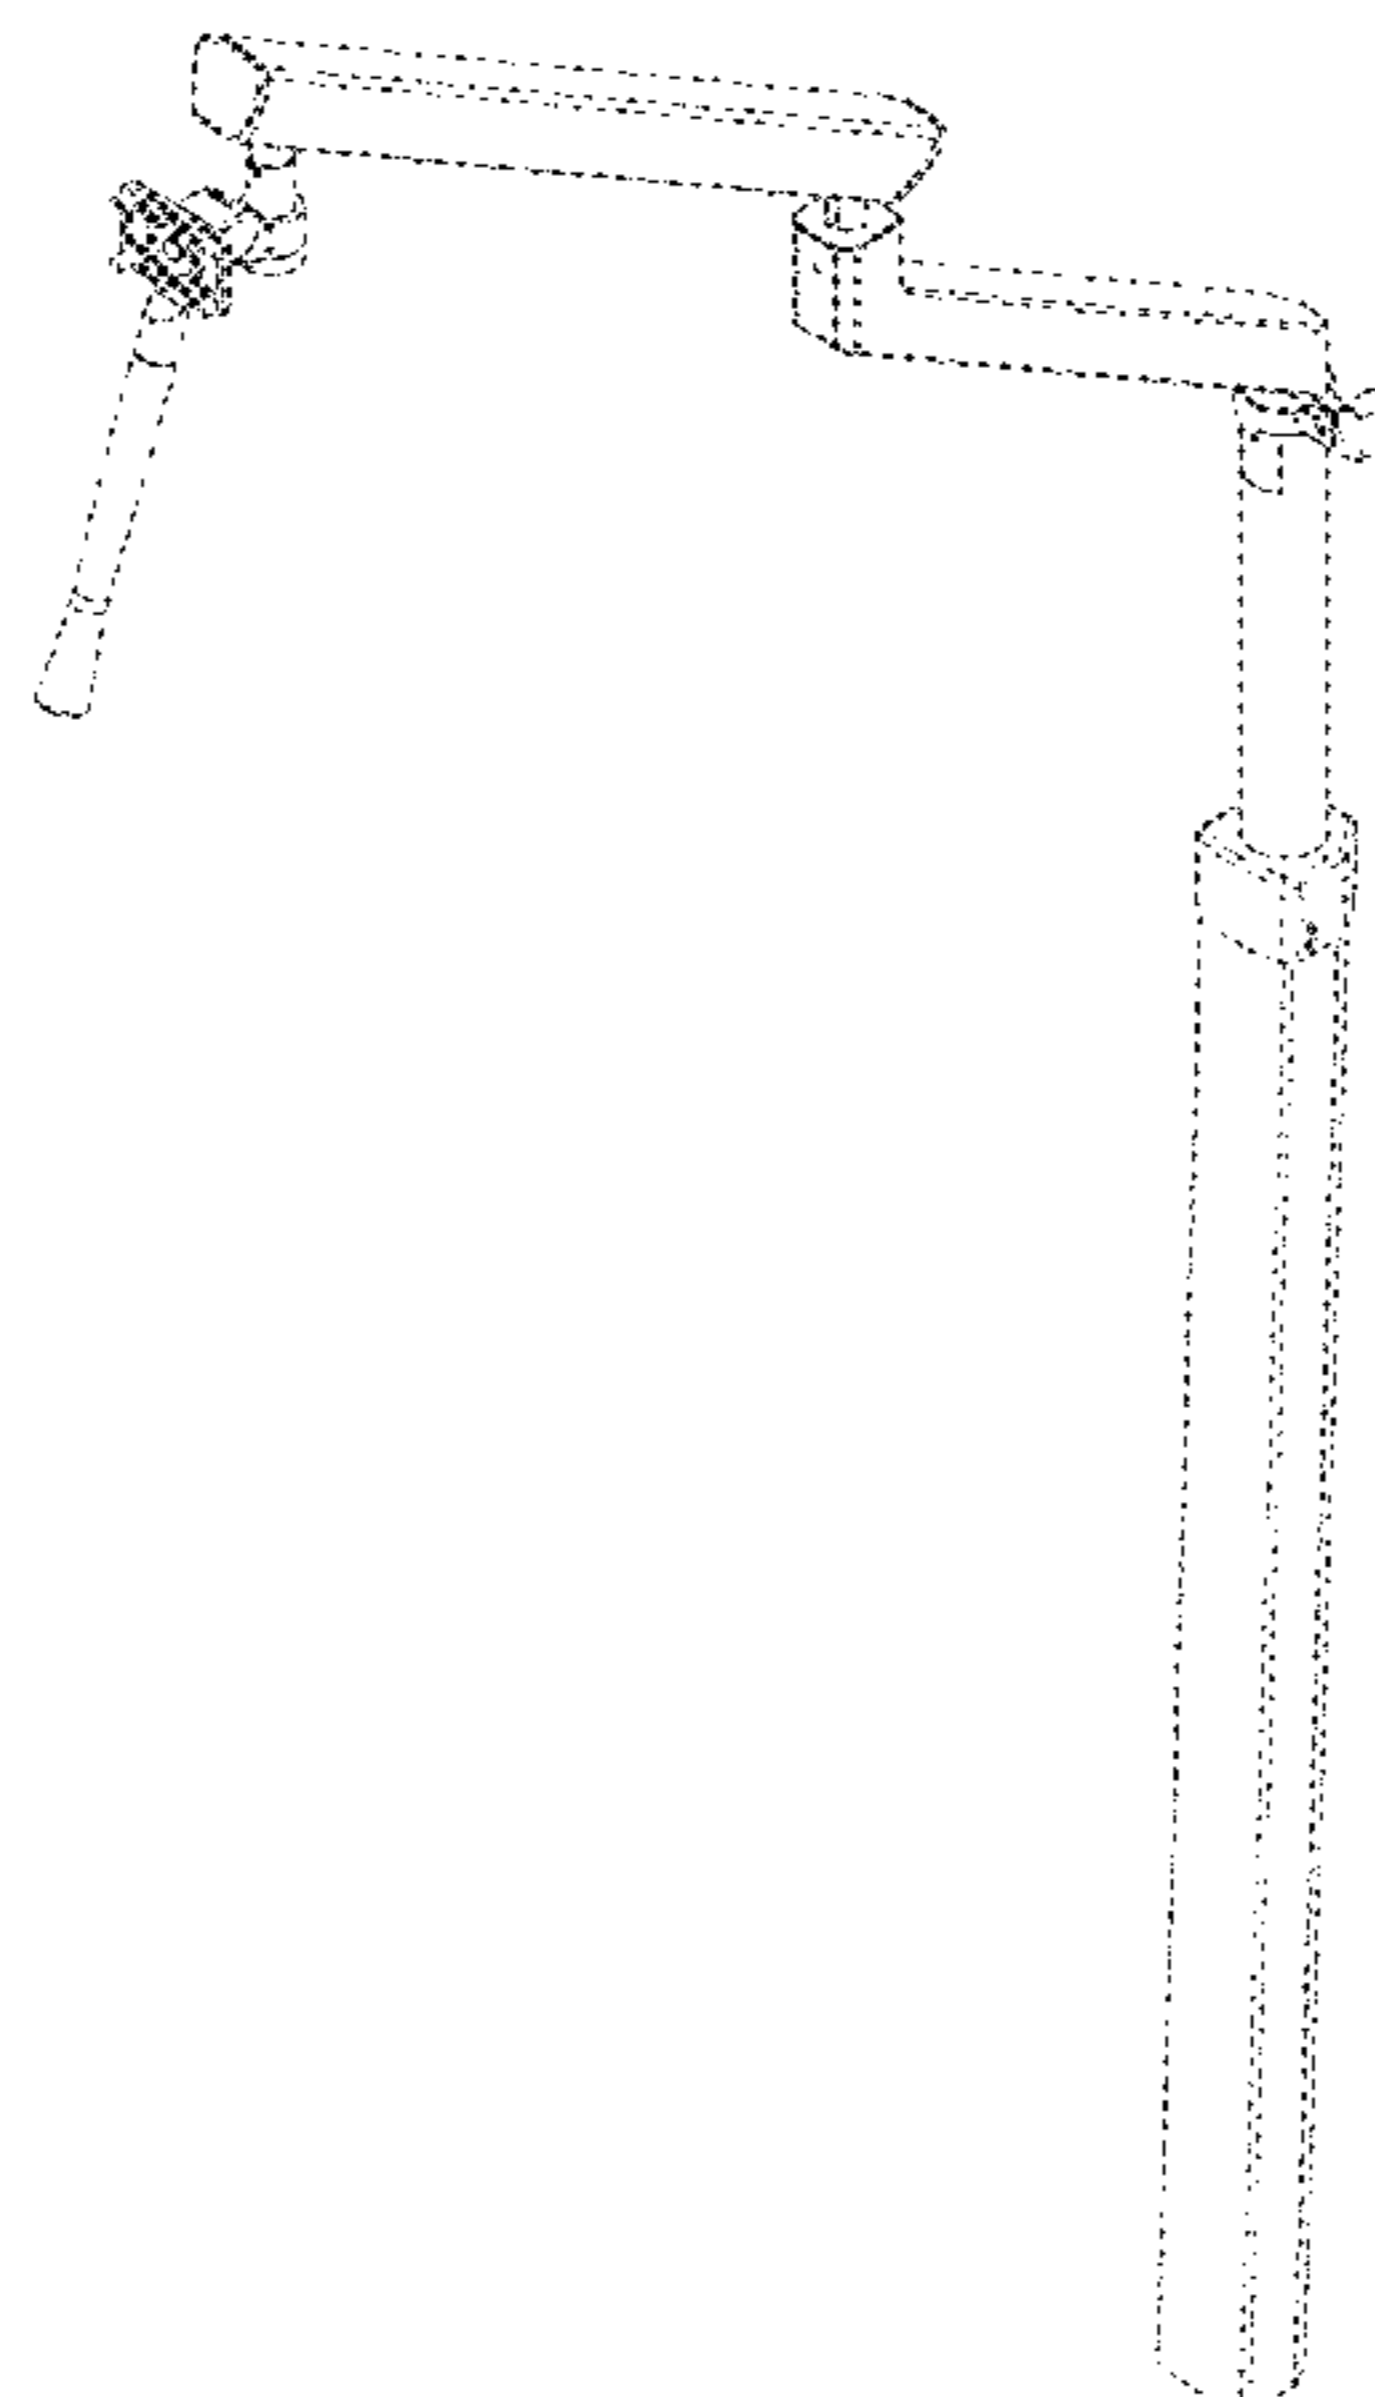

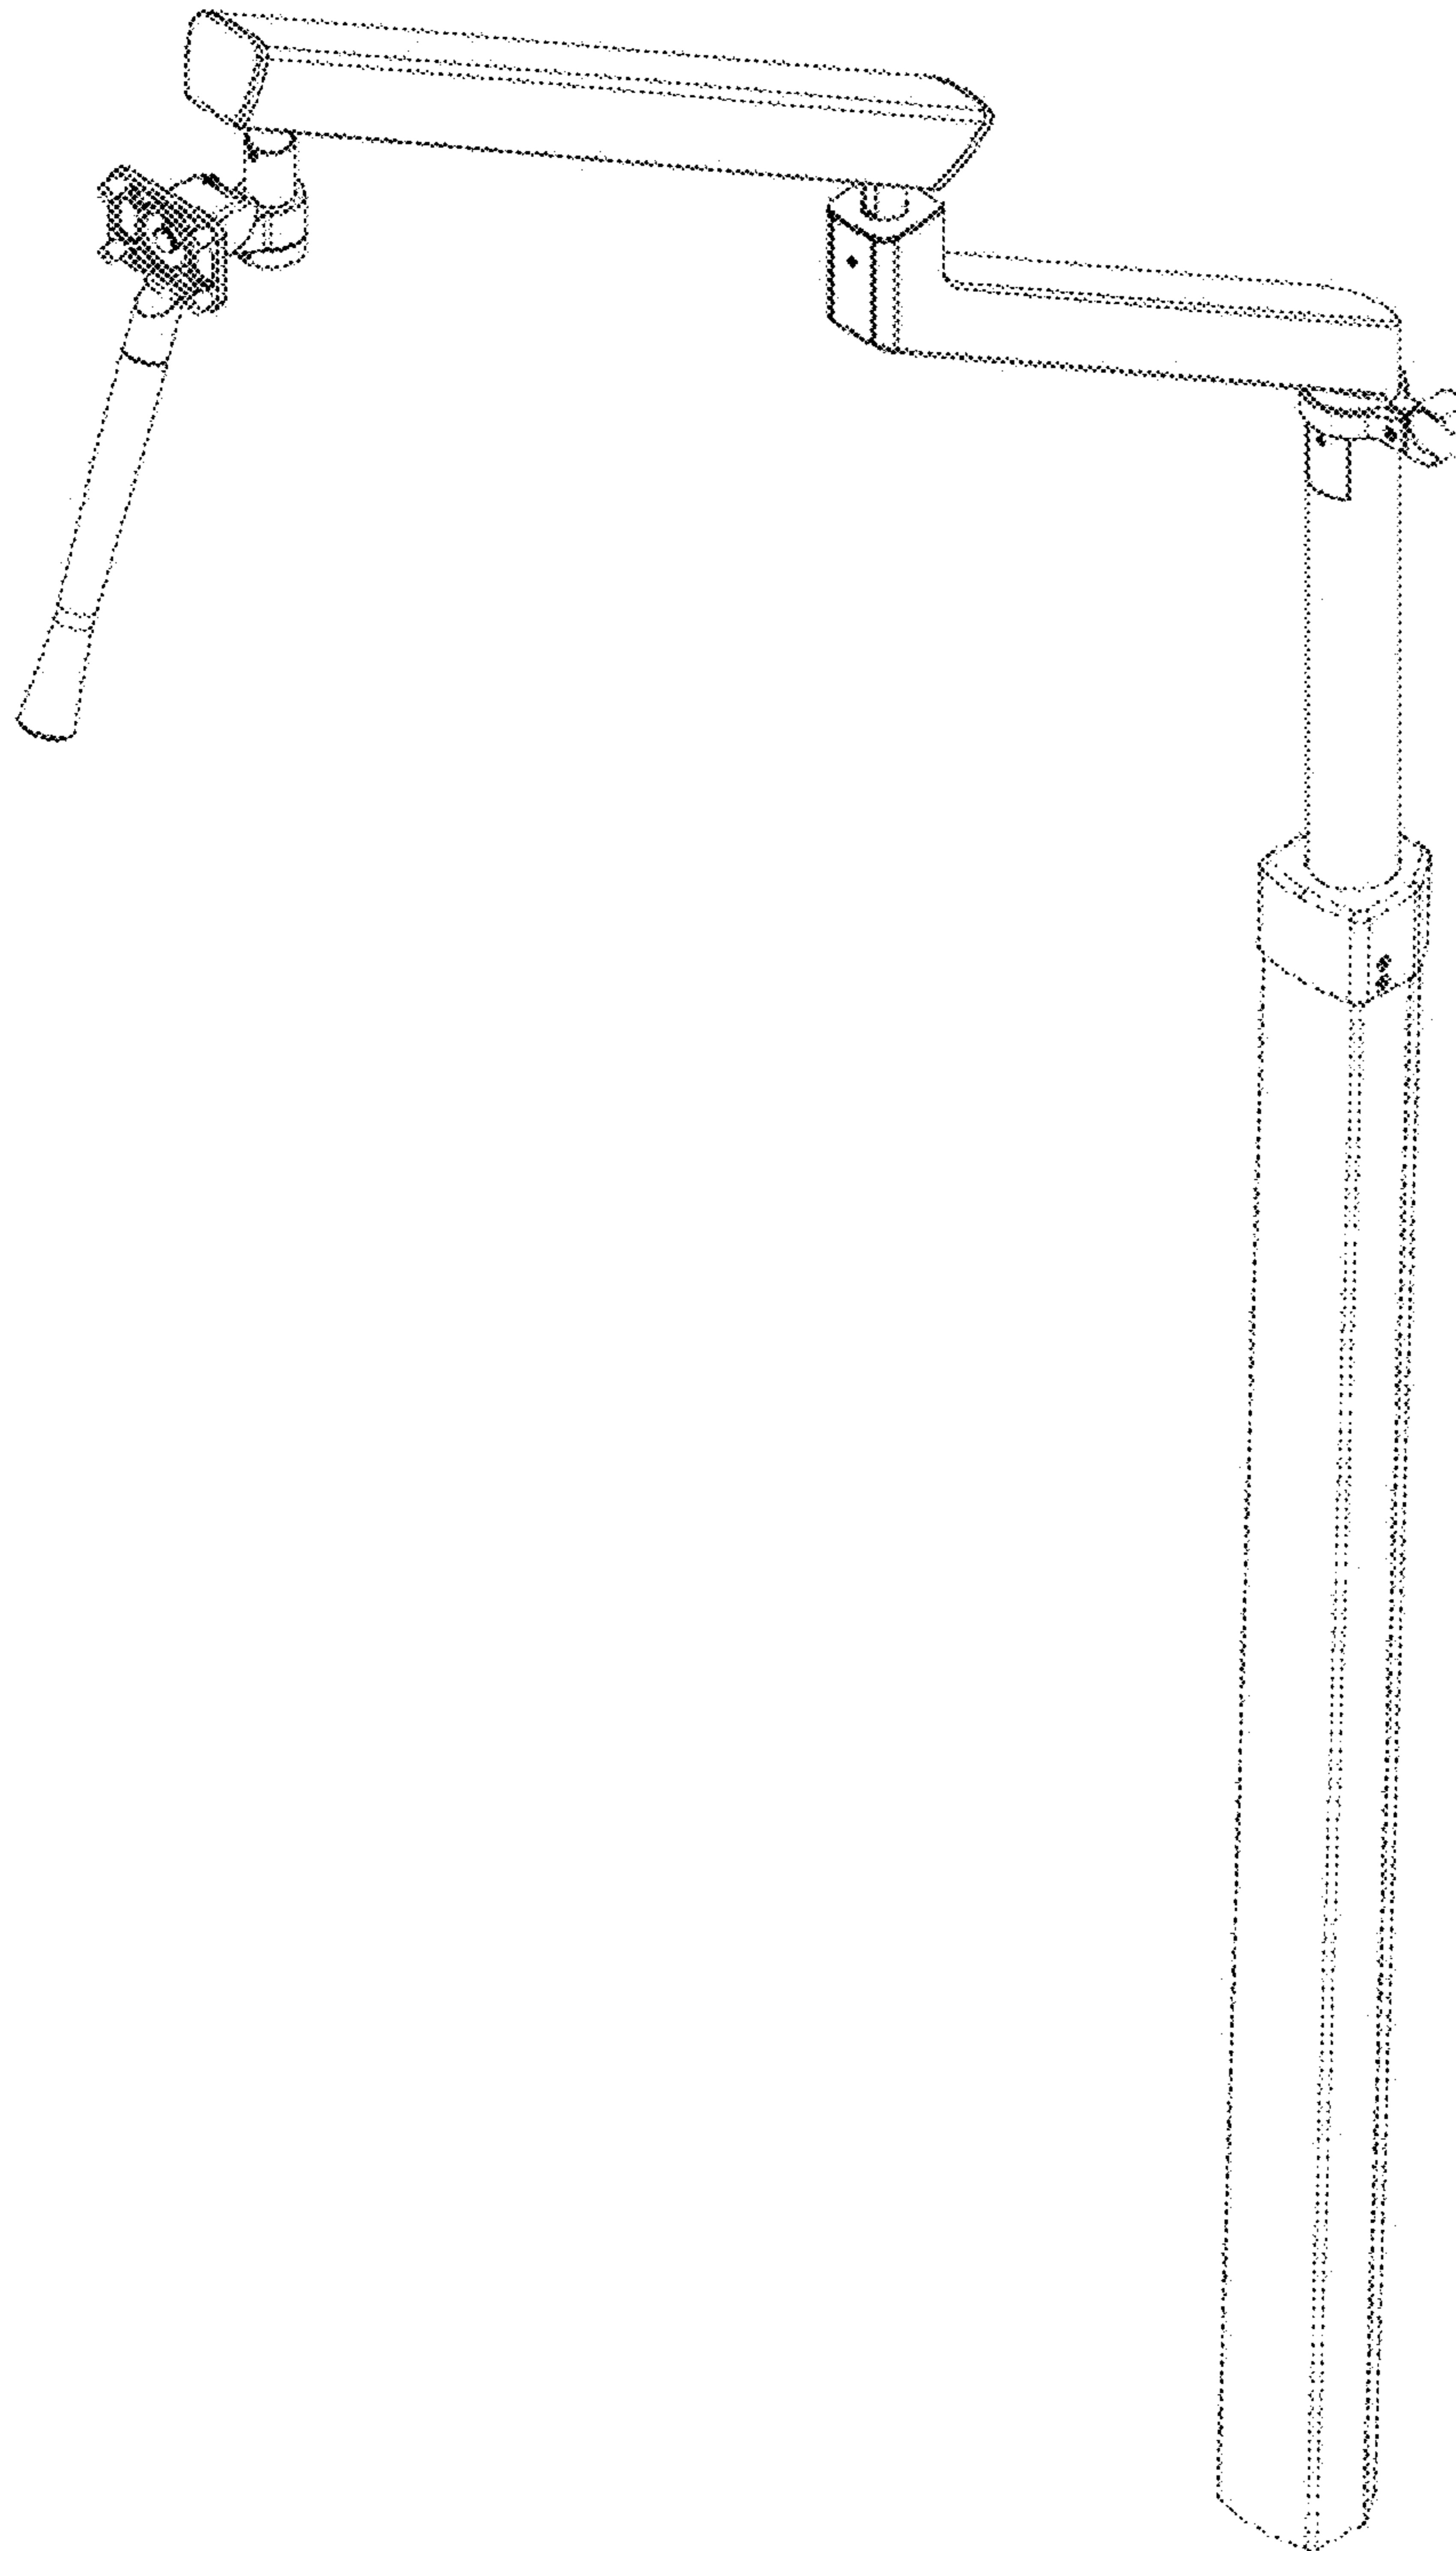


FIG. 1

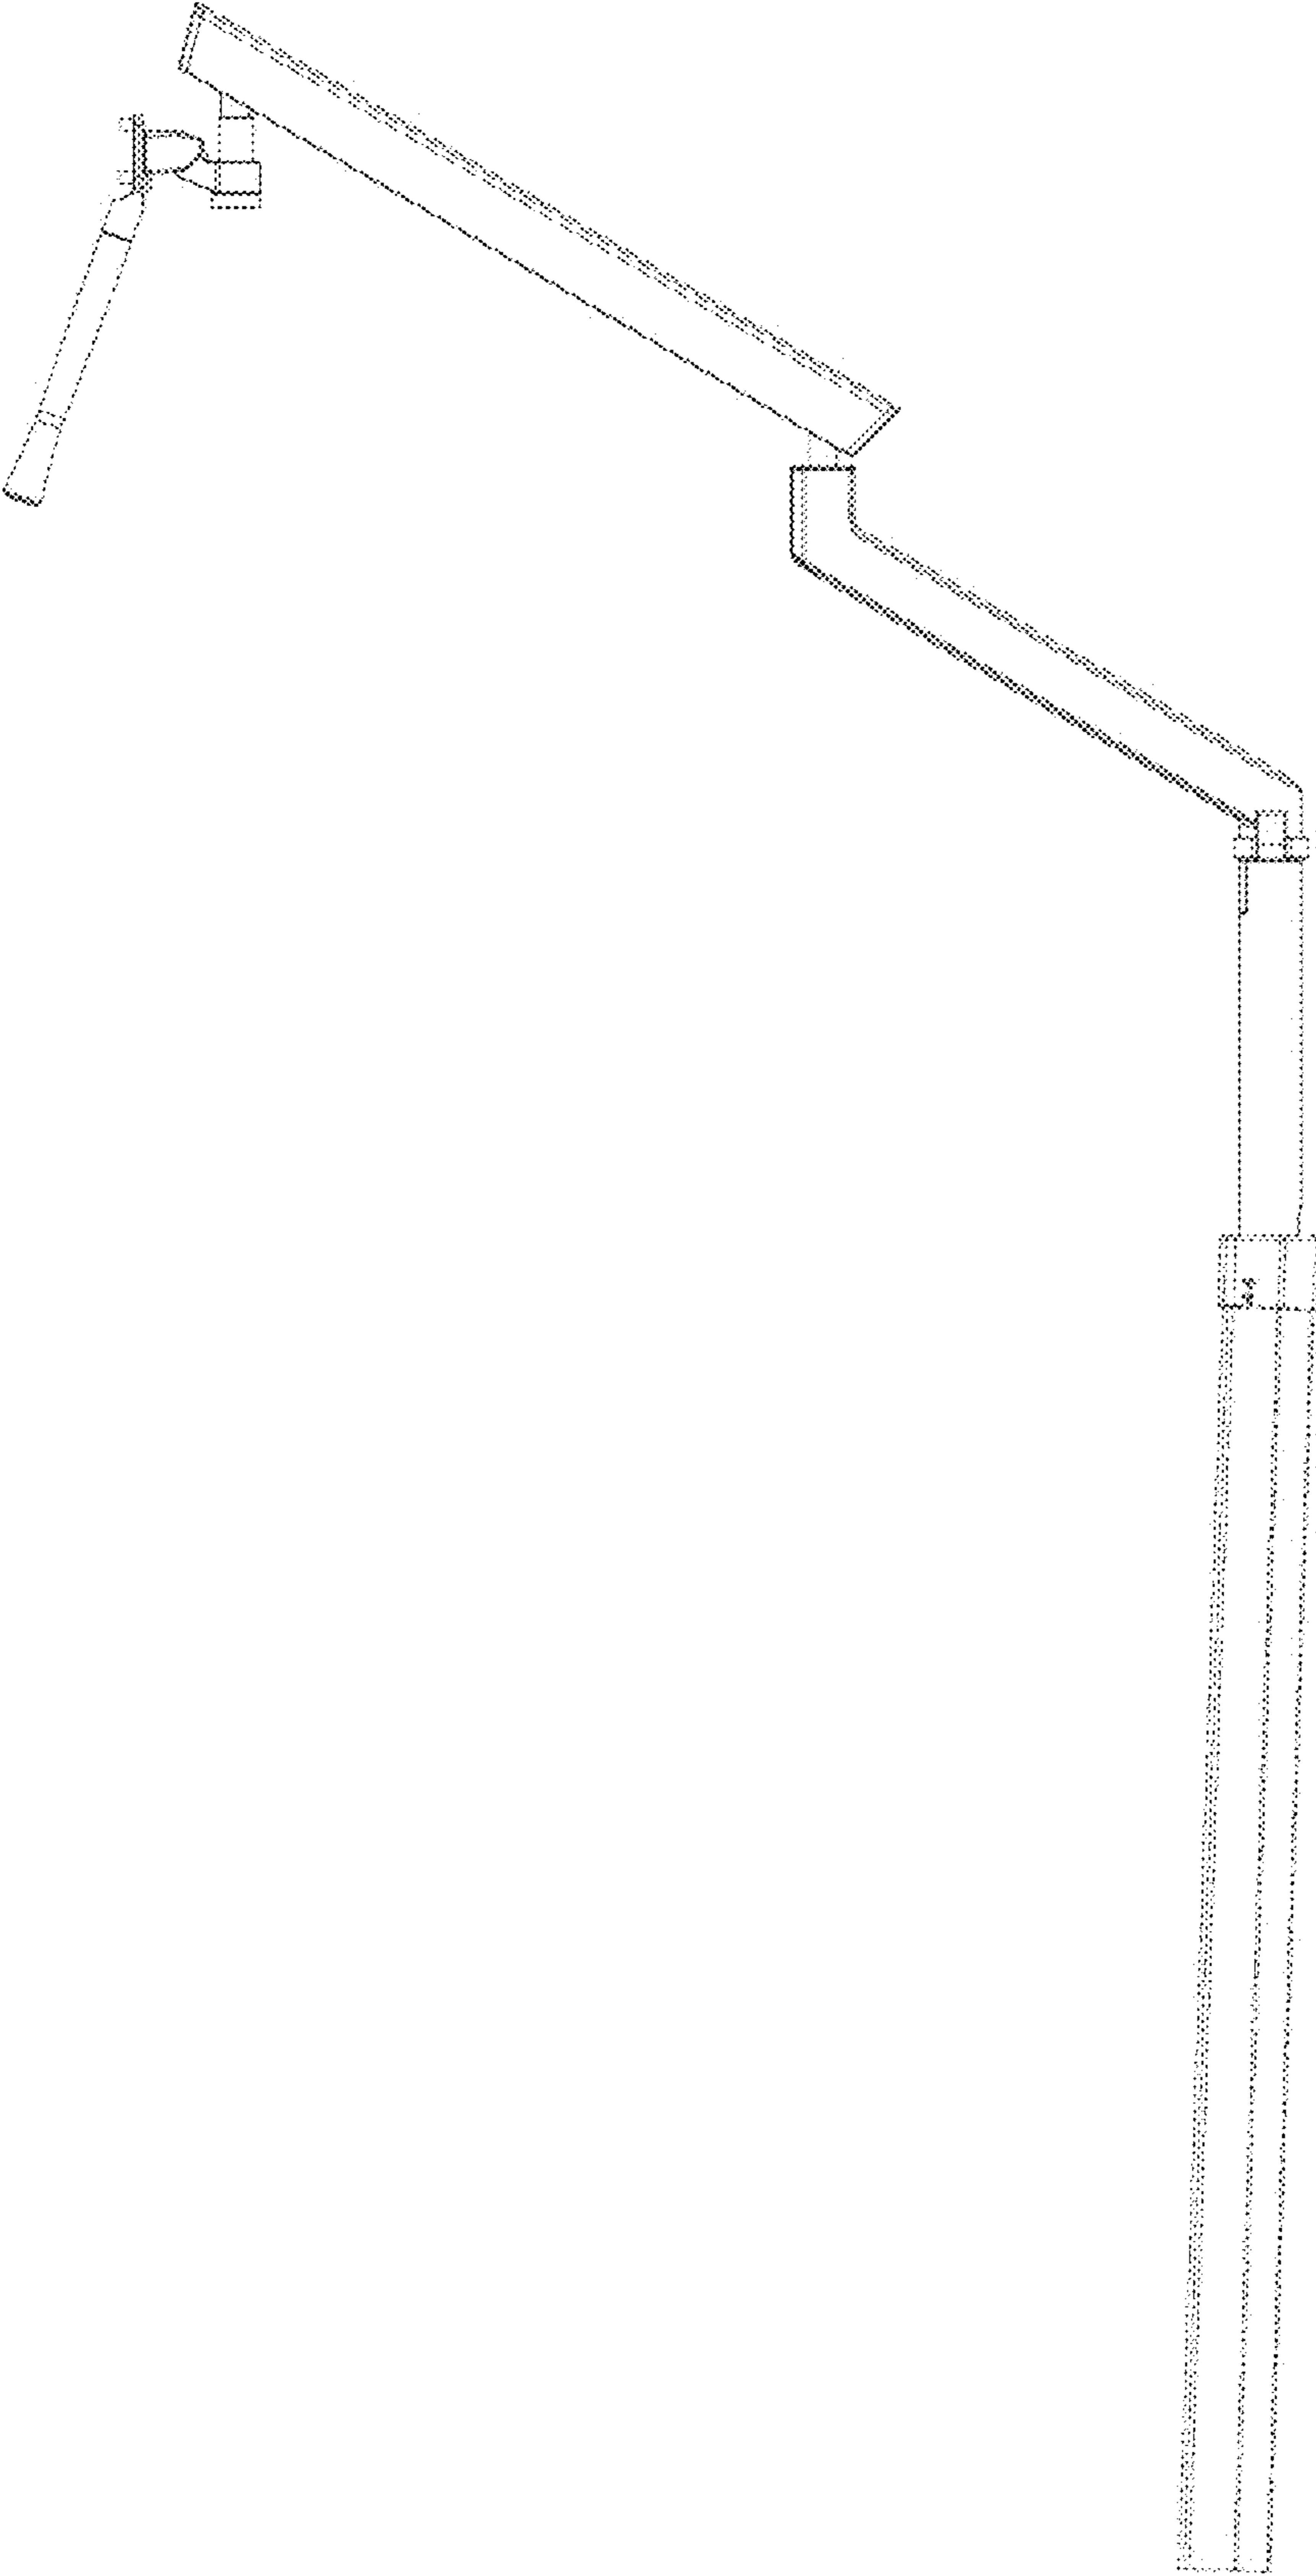


FIG. 2

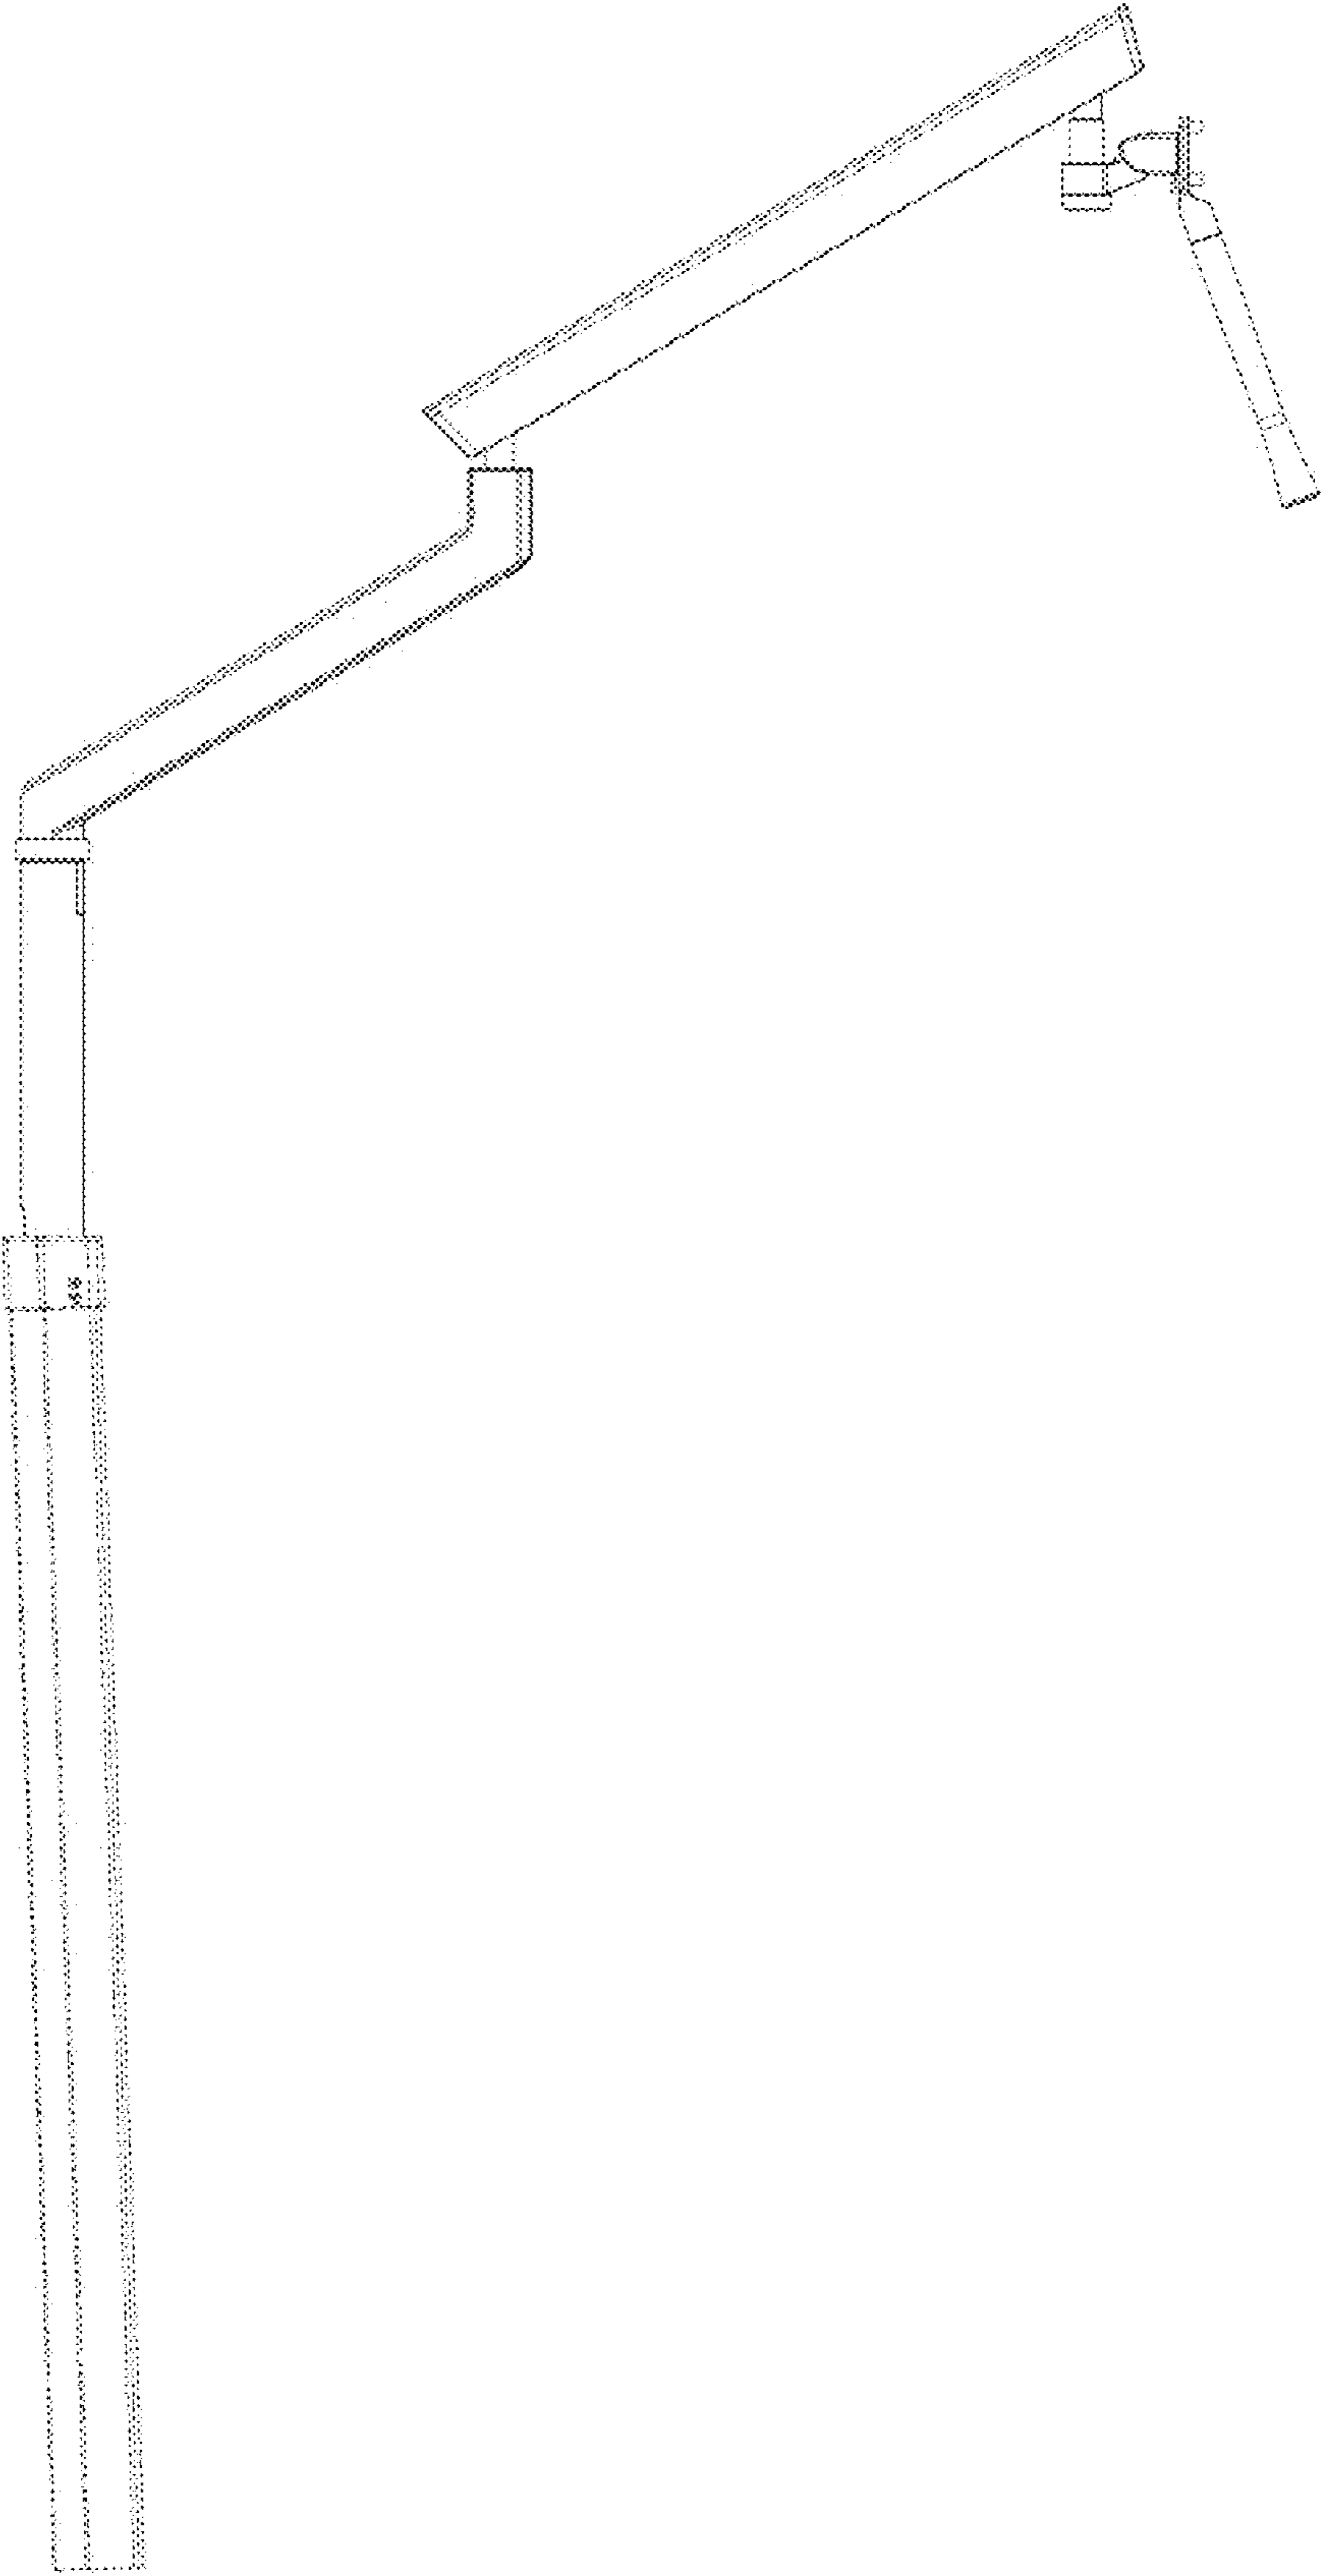


FIG. 3

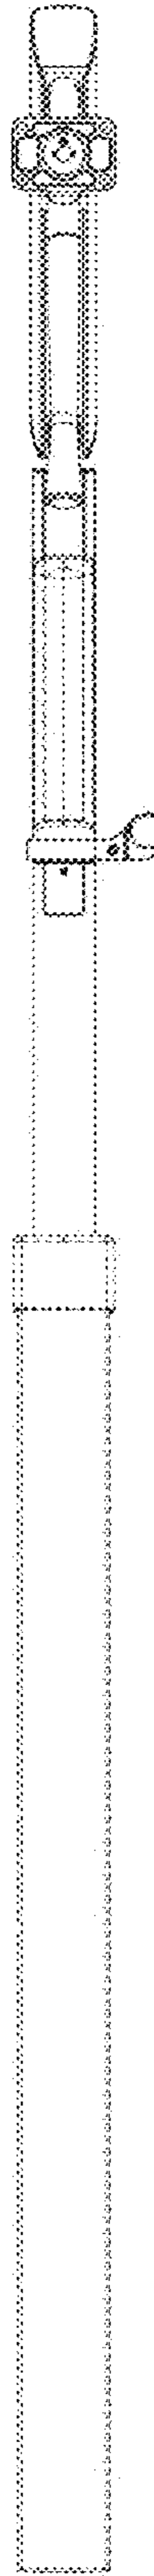


FIG. 4



FIG. 5

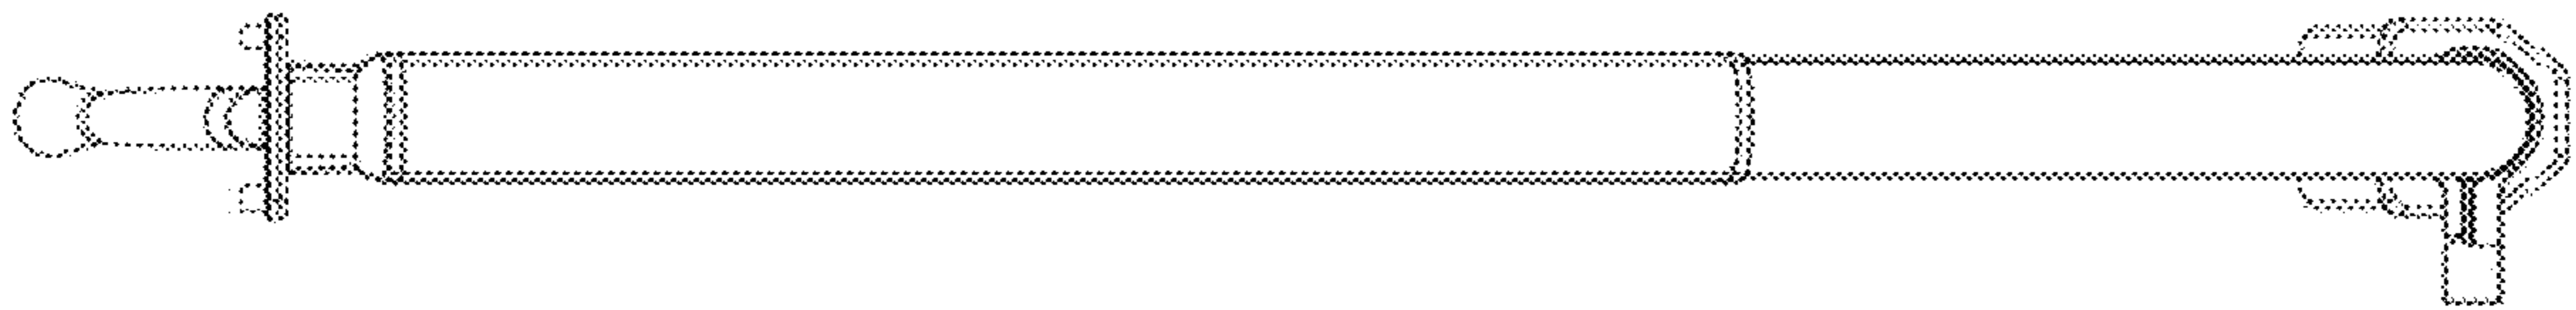


FIG. 6

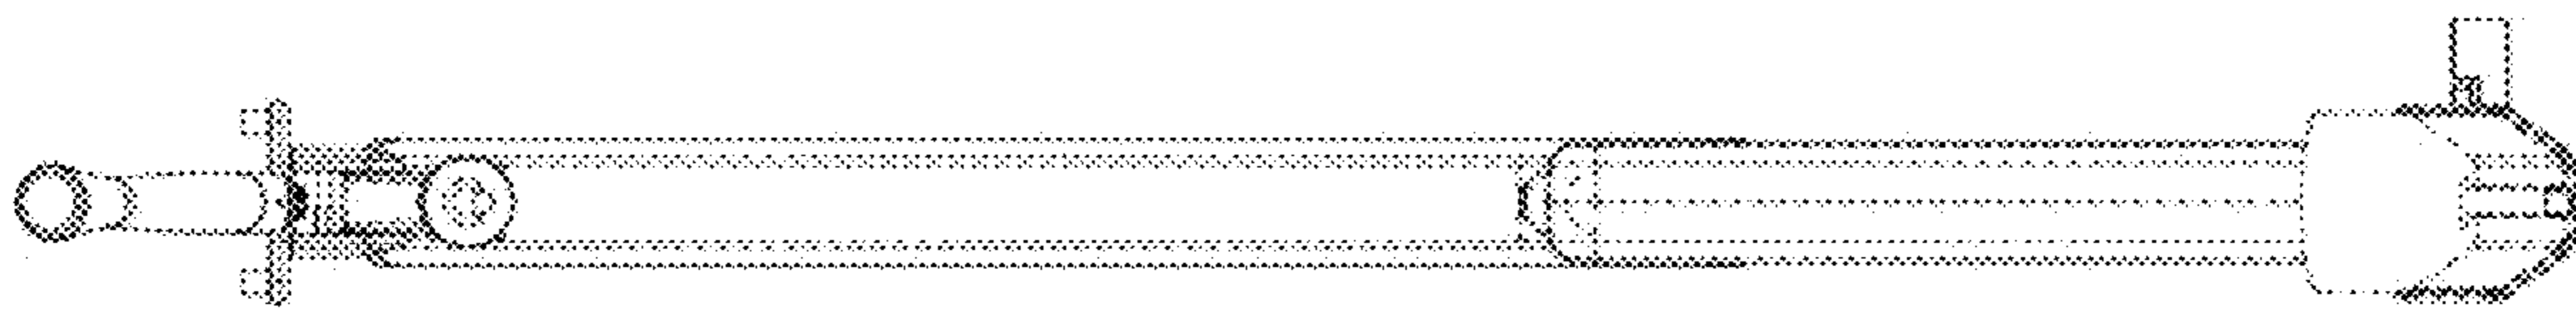


FIG. 7

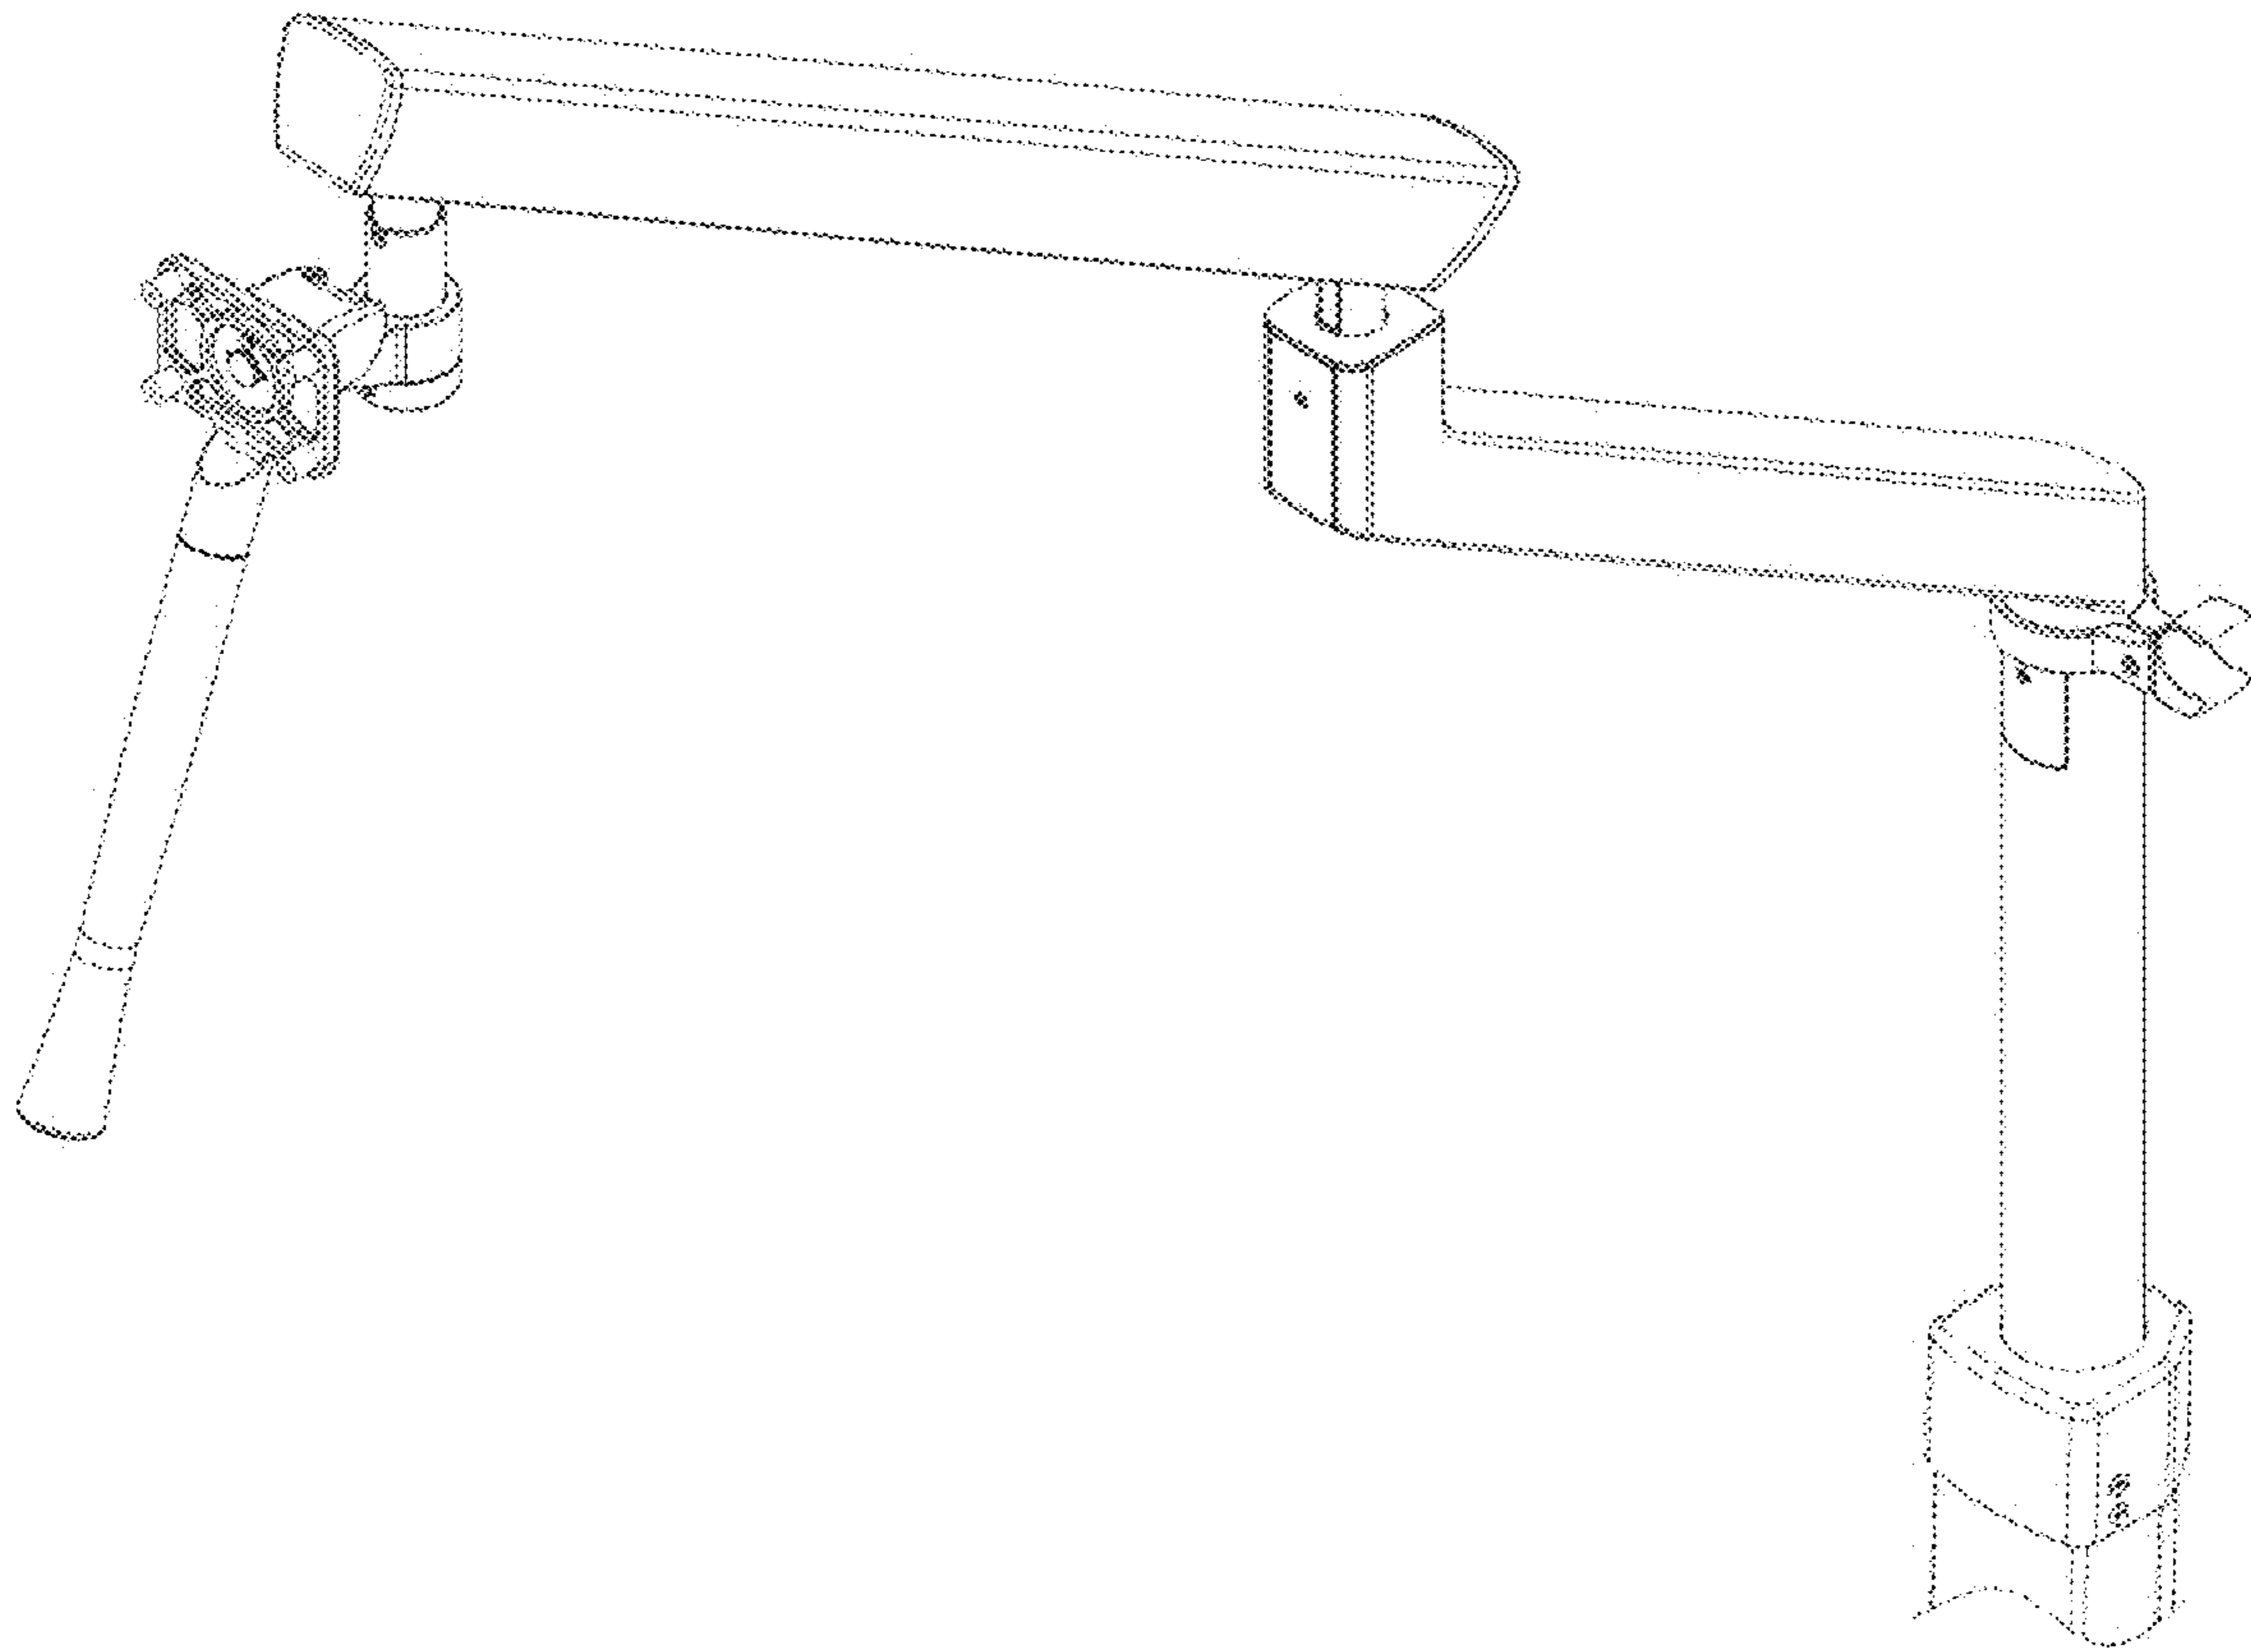


FIG. 8

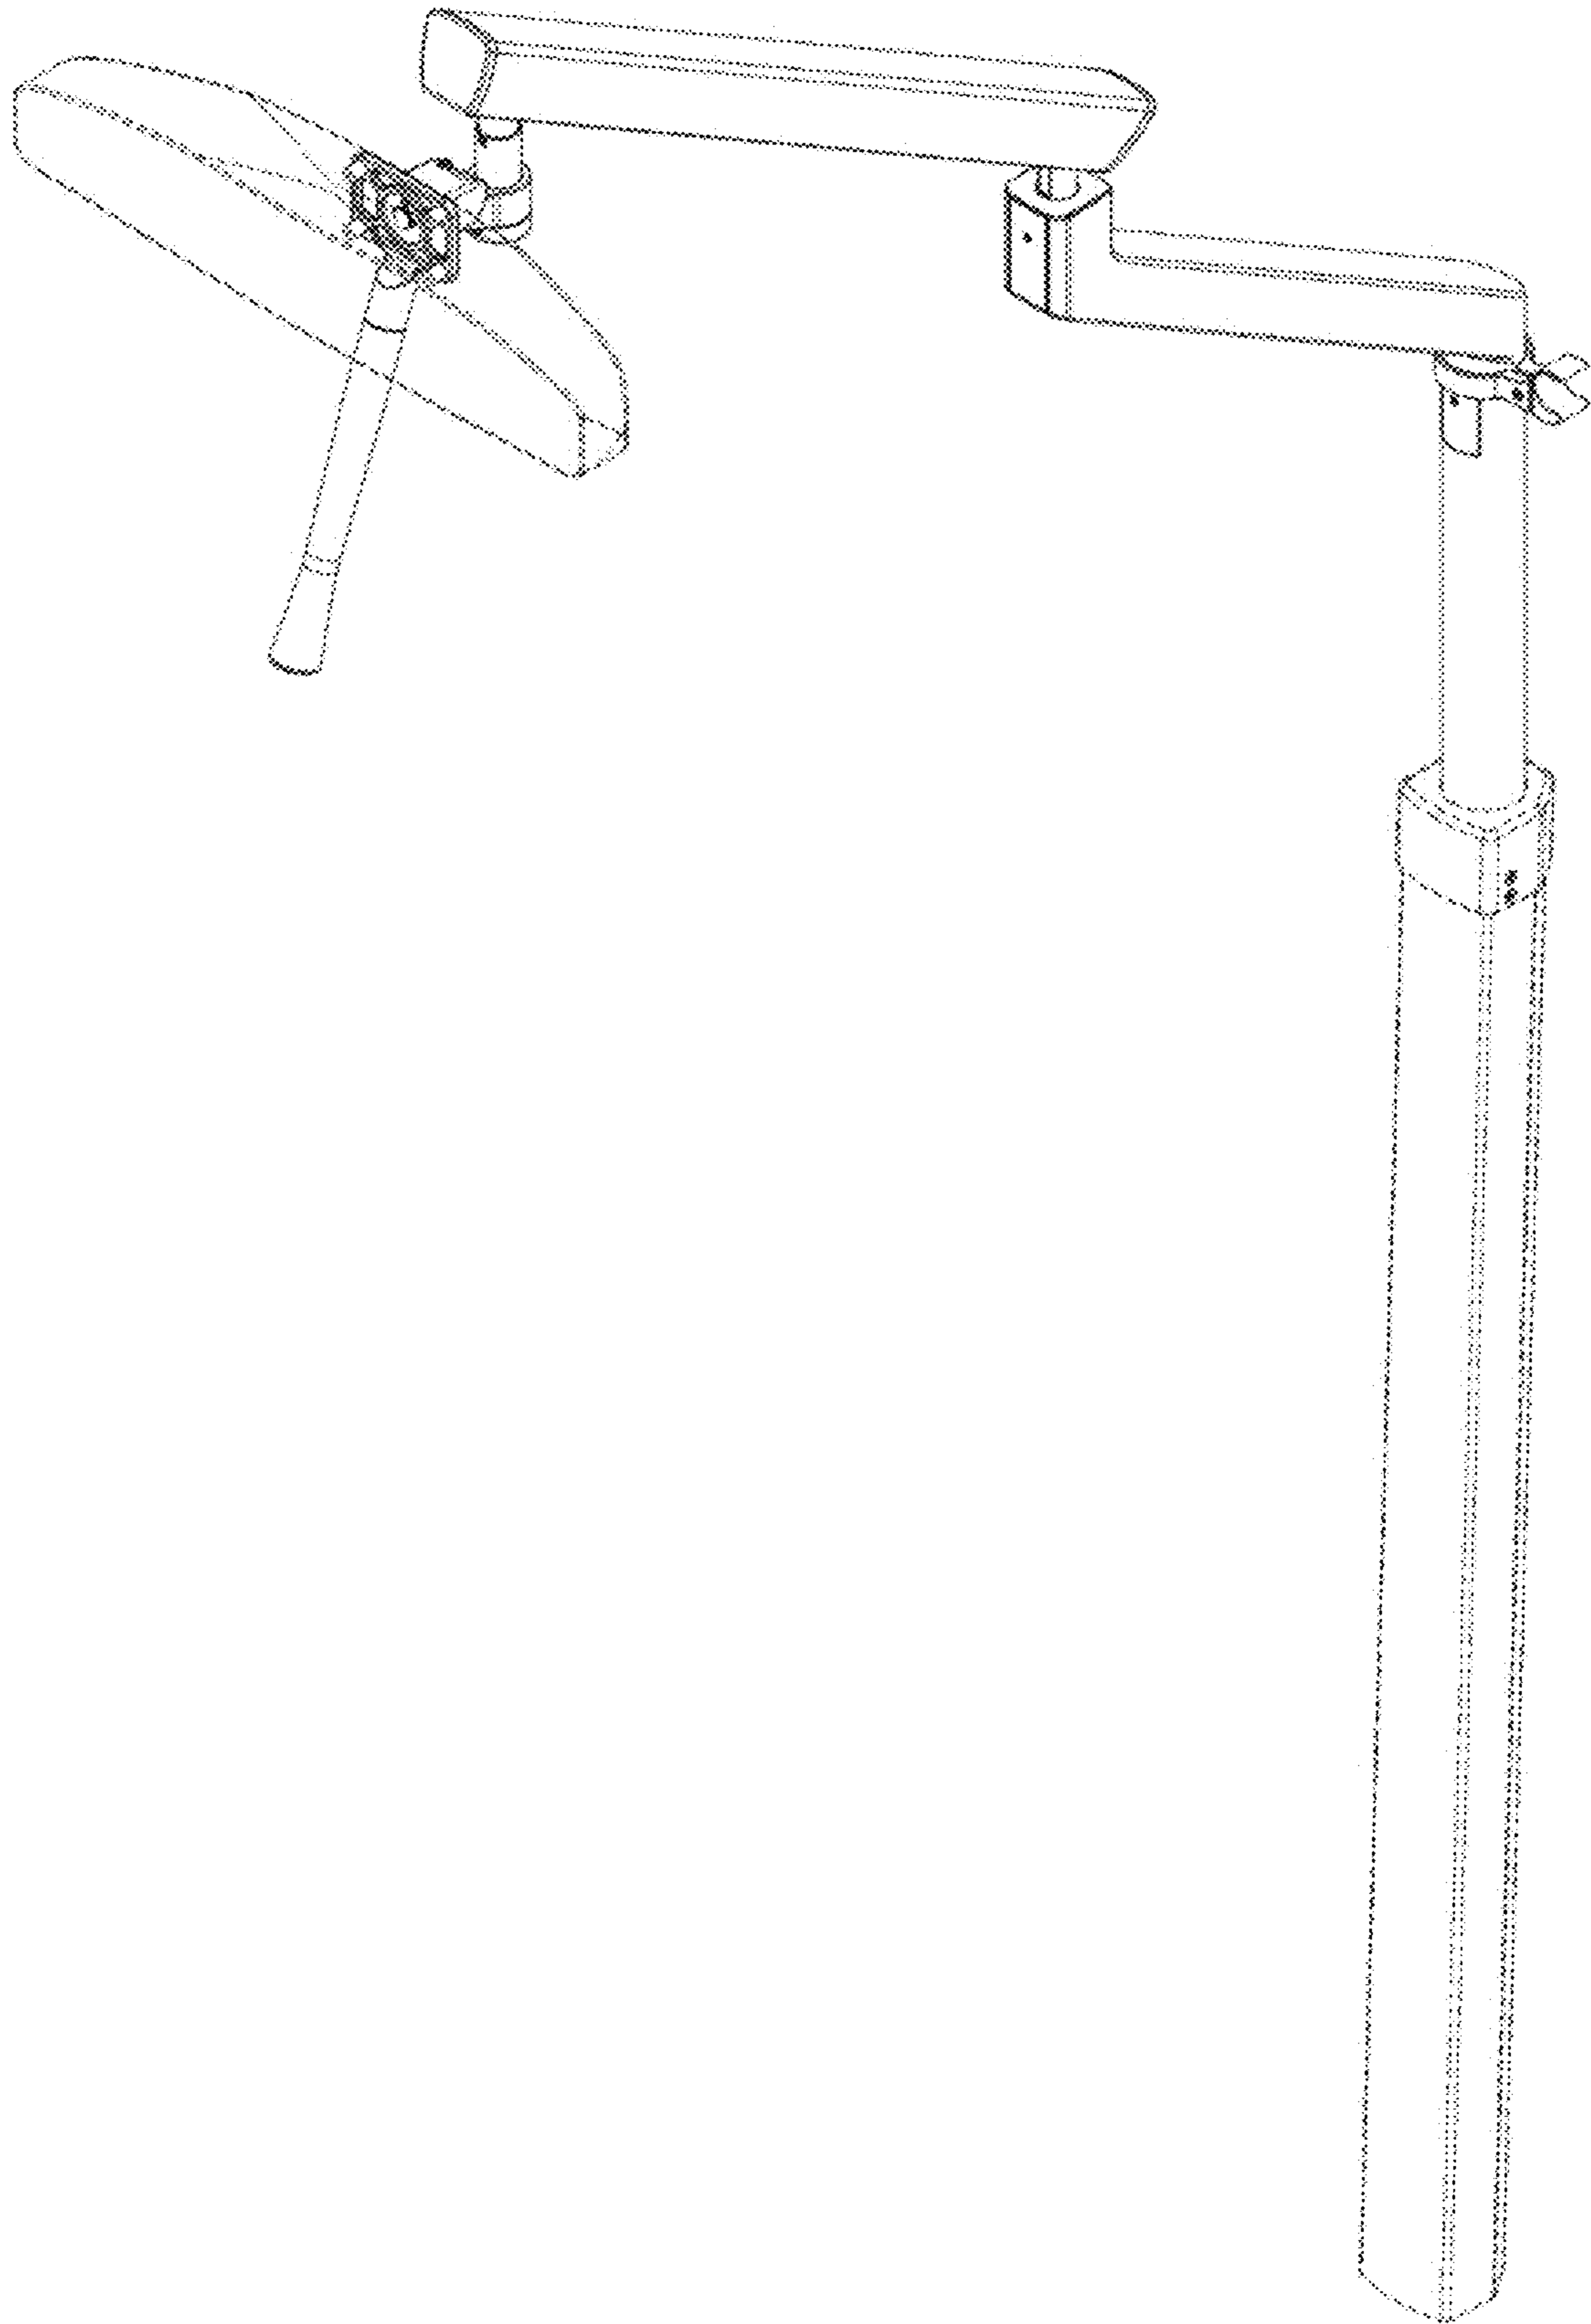


FIG. 9