



US00D982759S

(12) **United States Design Patent**  
**Qian et al.**

(10) **Patent No.:** **US D982,759 S**  
(45) **Date of Patent:** **\*\* Apr. 4, 2023**

(54) **MULTI-PARAMETER DETECTOR FOR MEDICAL USE**

(71) Applicant: **BEIJING CHOICE ELECTRONIC TECHNOLOGY CO., LTD.**, Beijing (CN)

(72) Inventors: **Xiaolun Qian**, Beijing (CN); **Chuanlong Ma**, Beijing (CN); **Zesheng Xi**, Beijing (CN)

(\*\*) Term: **15 Years**

(21) Appl. No.: **35/515,143**

(22) Filed: **Aug. 9, 2022**

(80) **Hague Agreement Data**

Int. Filing Date: **Aug. 9, 2022**

Int. Reg. No.: **DM/223169**

Int. Reg. Date: **Aug. 9, 2022**

Int. Reg. Pub. Date: **Sep. 16, 2022**

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/167**  
CPC ..... **A61B 5/7203** (2013.01)

(58) **Field of Classification Search**  
USPC ..... D24/107, 167, 186, 187, 158, 216, 218, D24/224, 225; D10/70, 75, 97, 98, 46; D14/344, 138 C, 138 R  
CPC ... A61B 5/7203; A61B 5/308; A61B 5/02055; A61B 5/316; A61B 5/681; A61B 5/282; A61B 5/002; A61B 5/332; A61B 5/30; A61B 5/7225; A61B 2562/0209; A61B 2560/0214; A61B 5/14546; A61B 5/6838; A61B 2560/0209; A61B 5/0006; A61B 5/6826; A61B 5/14532; A61B 2562/043  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,619,039 A \* 4/1997 Montanari ..... H01L 31/024  
250/352  
D420,452 S \* 2/2000 Cardy ..... D24/224

D566,280 S \* 4/2008 Baba ..... D10/46  
D599,909 S \* 9/2009 Rinott ..... D24/186  
D683,459 S \* 5/2013 Haltof ..... D24/161  
D751,715 S \* 3/2016 Bostley ..... D24/161  
D753,827 S \* 4/2016 Sul ..... D24/158  
D763,939 S \* 8/2016 Khanicheh ..... D16/130  
D770,042 S \* 10/2016 Christensen ..... D24/128  
D771,821 S \* 11/2016 Hilbig ..... D24/186  
D776,821 S \* 1/2017 Chou ..... D24/186  
D786,441 S \* 5/2017 Sul ..... D24/158  
D787,679 S \* 5/2017 Sul ..... D24/158  
D794,207 S \* 8/2017 Flanagan ..... D24/186  
D818,591 S \* 5/2018 Asai ..... D24/158  
D821,582 S \* 6/2018 Onishi ..... D24/158  
D837,402 S \* 1/2019 Kim ..... D24/232  
D854,690 S \* 7/2019 Sun ..... D24/158  
D868,974 S \* 12/2019 Albert ..... D24/167  
D888,246 S \* 6/2020 Kim ..... D24/158  
D895,118 S \* 9/2020 Hwang ..... D24/167  
D895,119 S \* 9/2020 Hwang ..... D24/167  
D895,120 S \* 9/2020 Hwang ..... D24/167

(Continued)

**OTHER PUBLICATIONS**

ChoiceMMed.com HeartPal (Year: 2019).\*

*Primary Examiner* — Richard E Chilcot


(57) **CLAIM**

The ornamental design for multi-parameter detector for medical use, as shown and described.

**DESCRIPTION**

- 1. Multi-parameter detector for medical use
- 1.1 Front
- 1.2 Back
- 1.3 Left
- 1.4 Right
- 1.5 Top
- 1.6 Bottom
- 1.7 Perspective

**1 Claim, 7 Drawing Sheets**

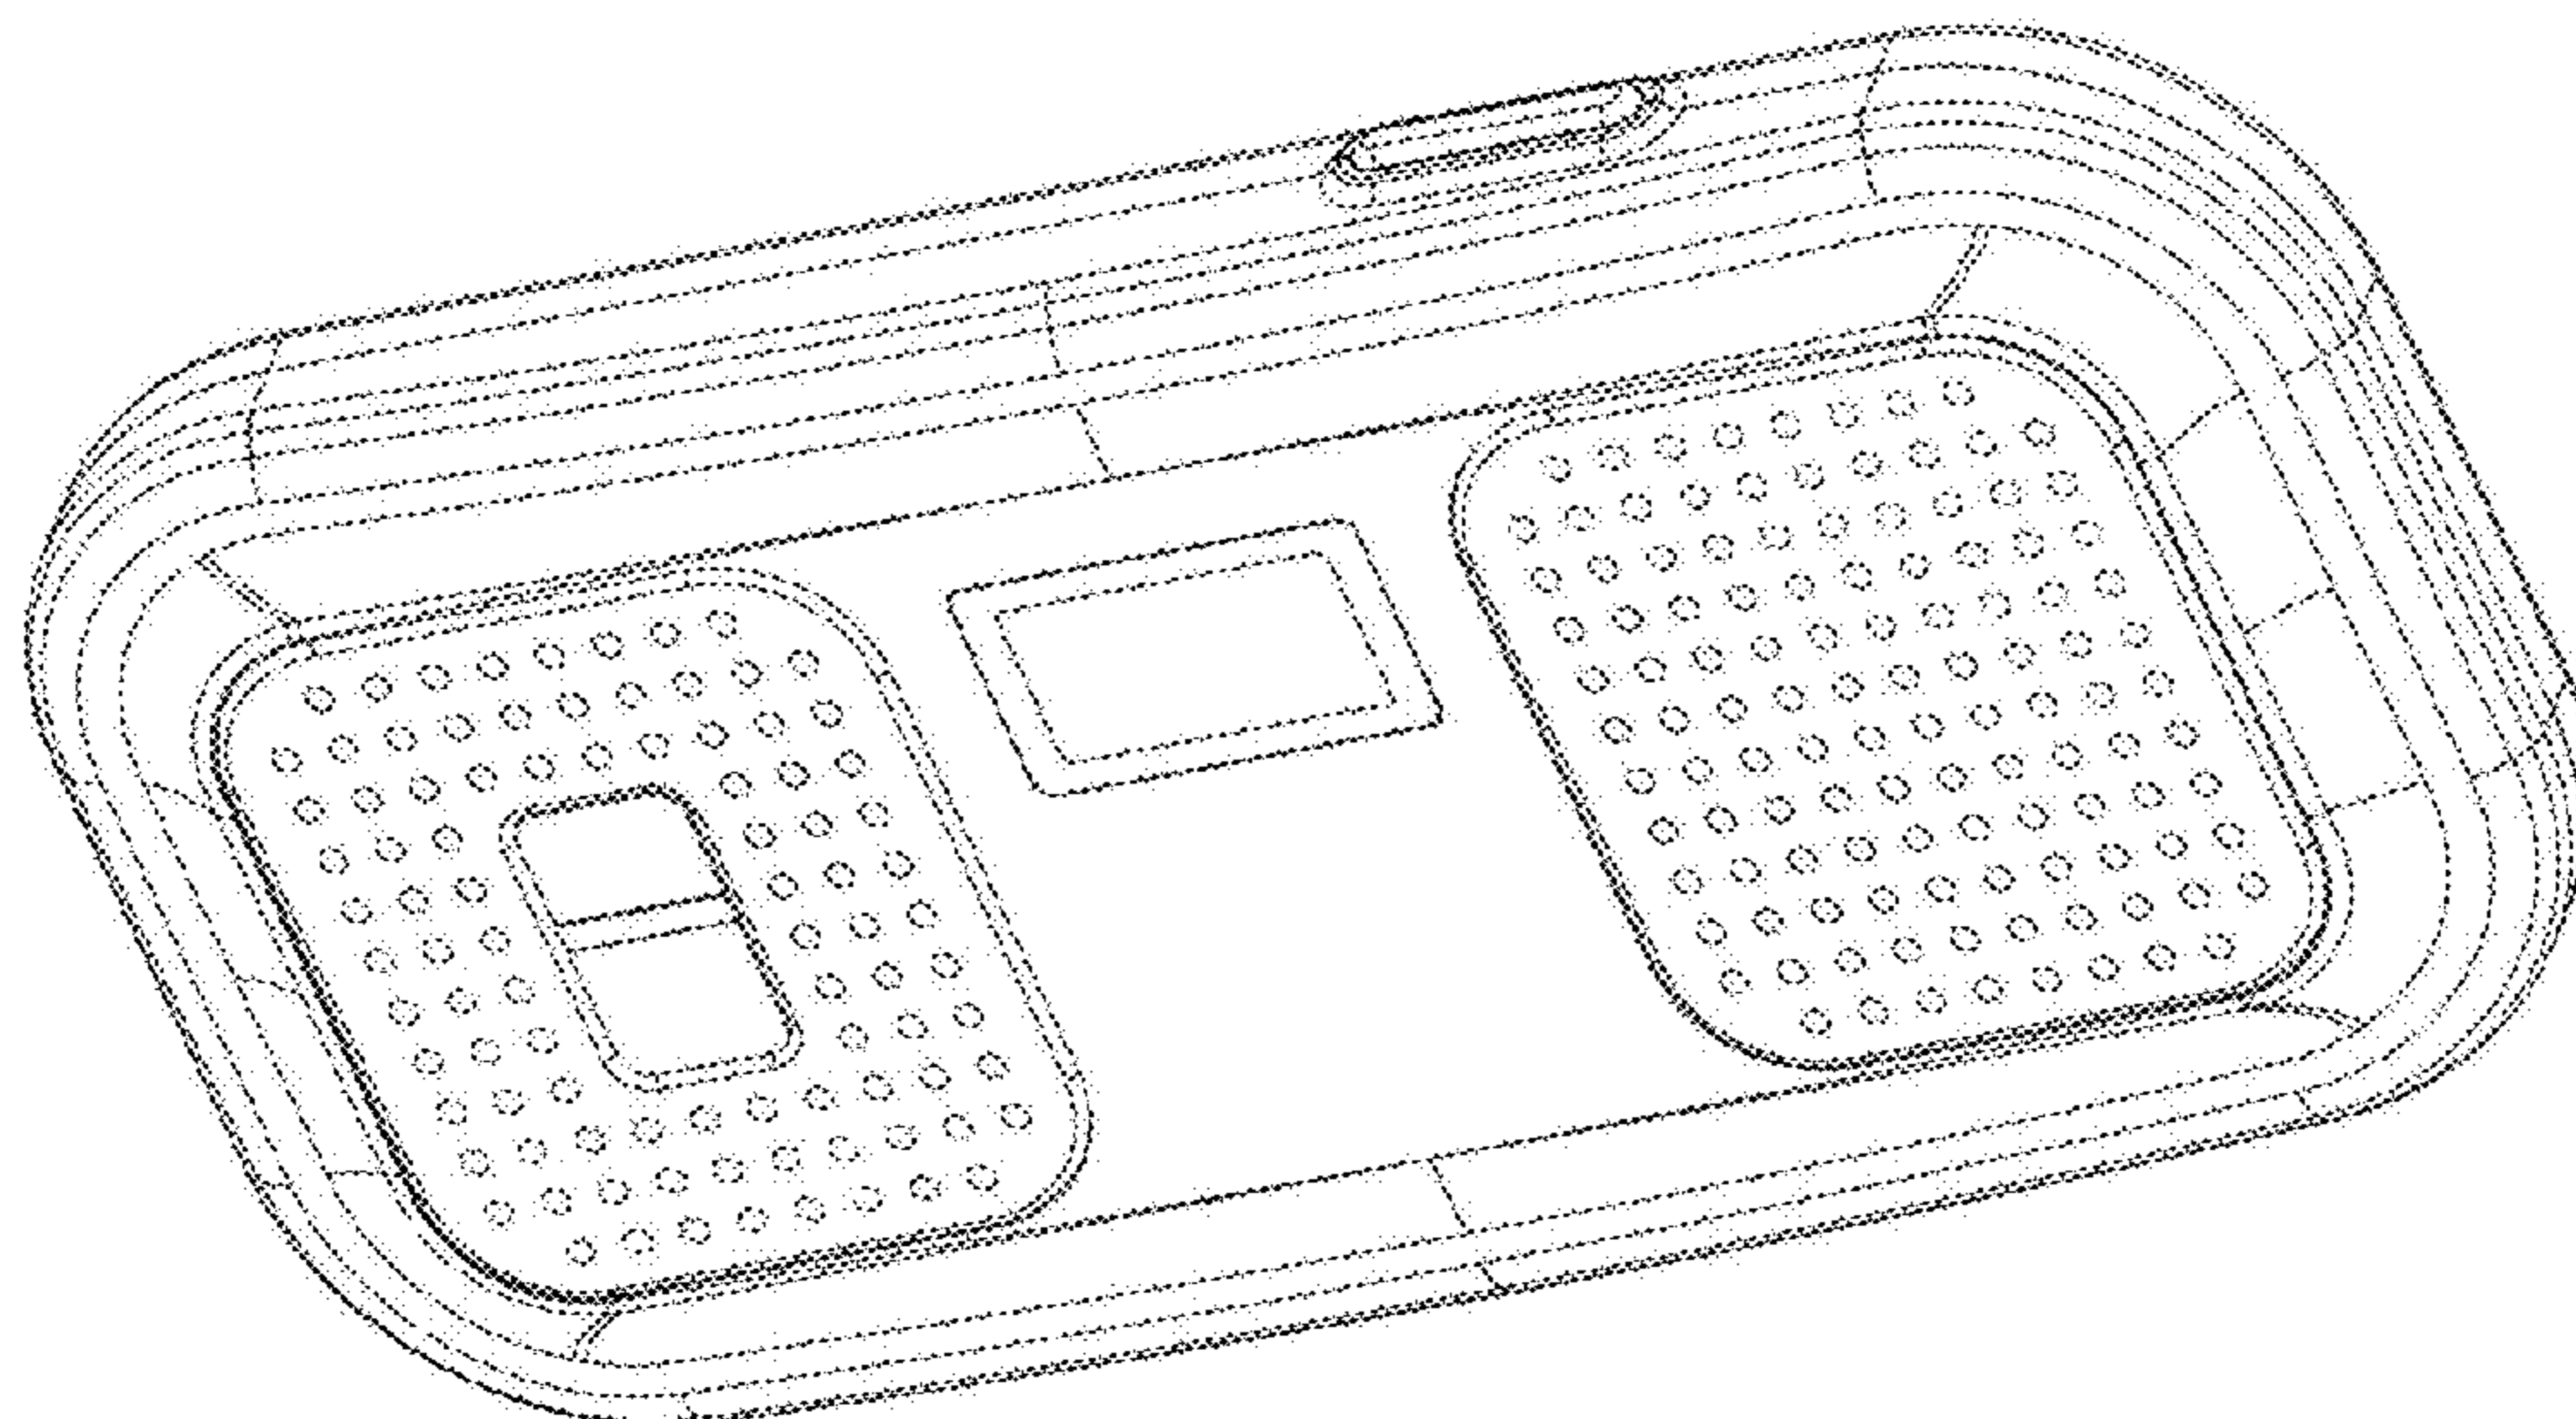


(56)

**References Cited**


U.S. PATENT DOCUMENTS

D912,823	S	*	3/2021	Hwang	.....	D24/167
D913,499	S	*	3/2021	Hwang	.....	D24/167
D913,500	S	*	3/2021	Hwang	.....	D24/167
D940,881	S	*	1/2022	Hadley	.....	D24/186
D950,061	S	*	4/2022	Riggs	.....	D24/224
D956,982	S	*	7/2022	Hellman	.....	D24/186
D962,467	S	*	8/2022	Taylor	.....	D24/224
11,486,825	B1	*	11/2022	Mozneb	.....	G01N 21/41
2020/0315480	A1	*	10/2020	Hwang	.....	A61B 5/7203


\* cited by examiner

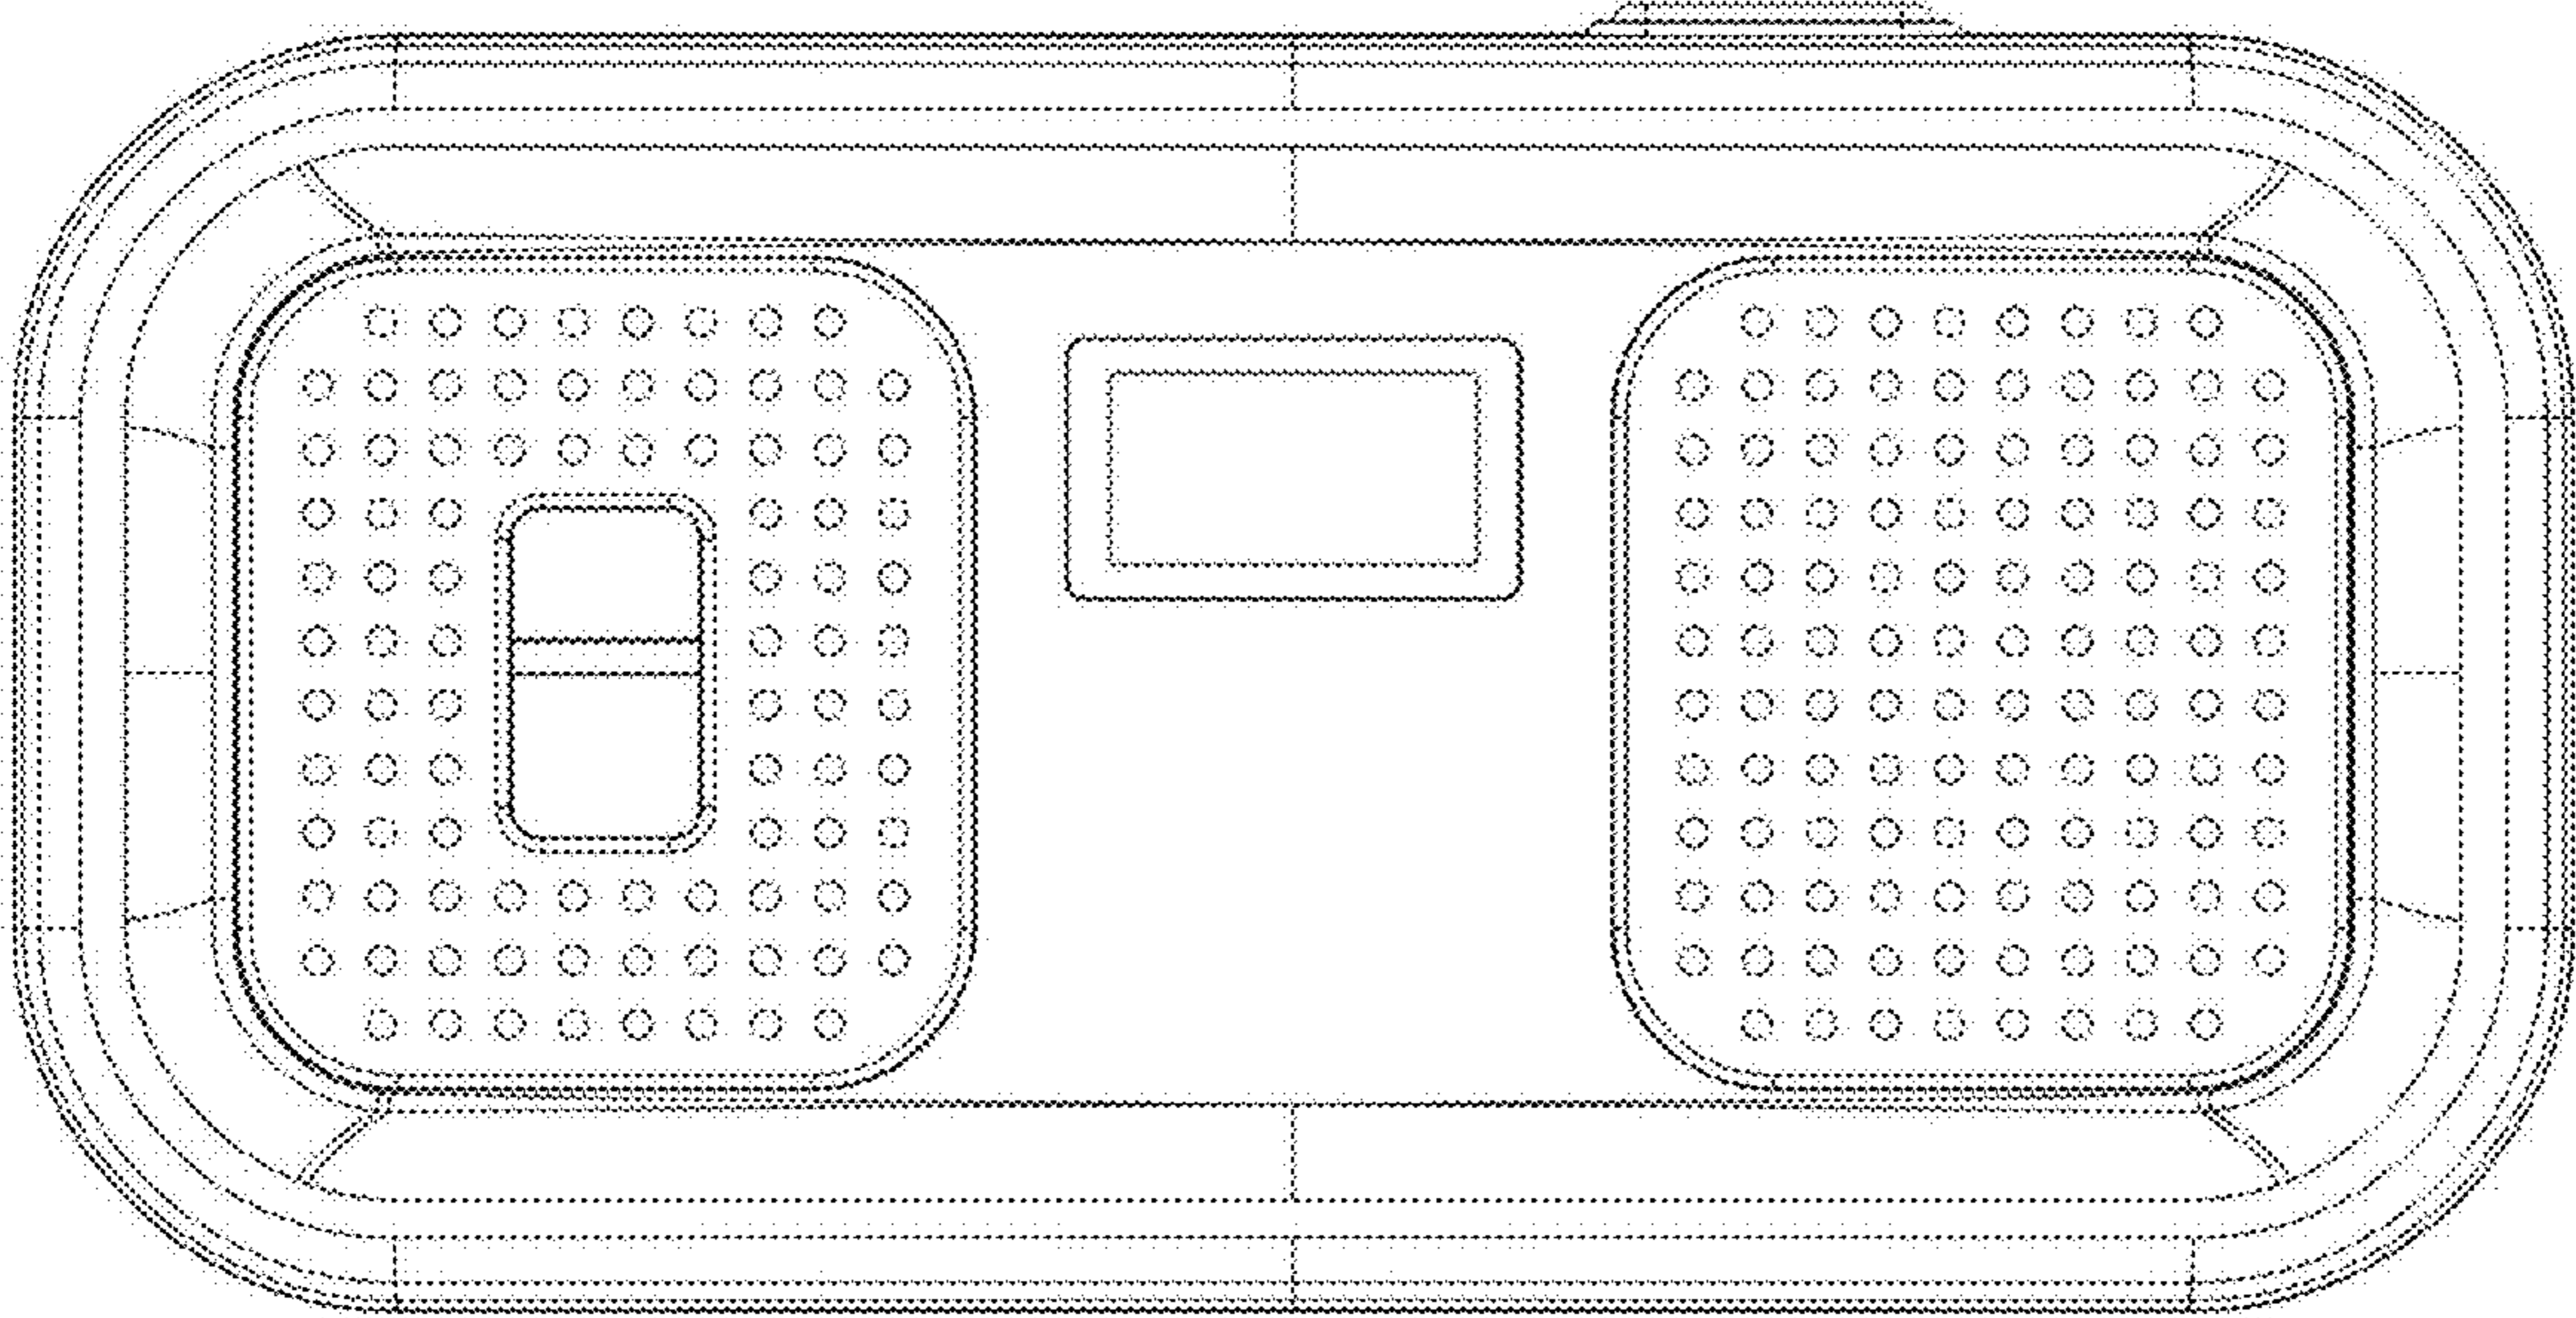


1.1

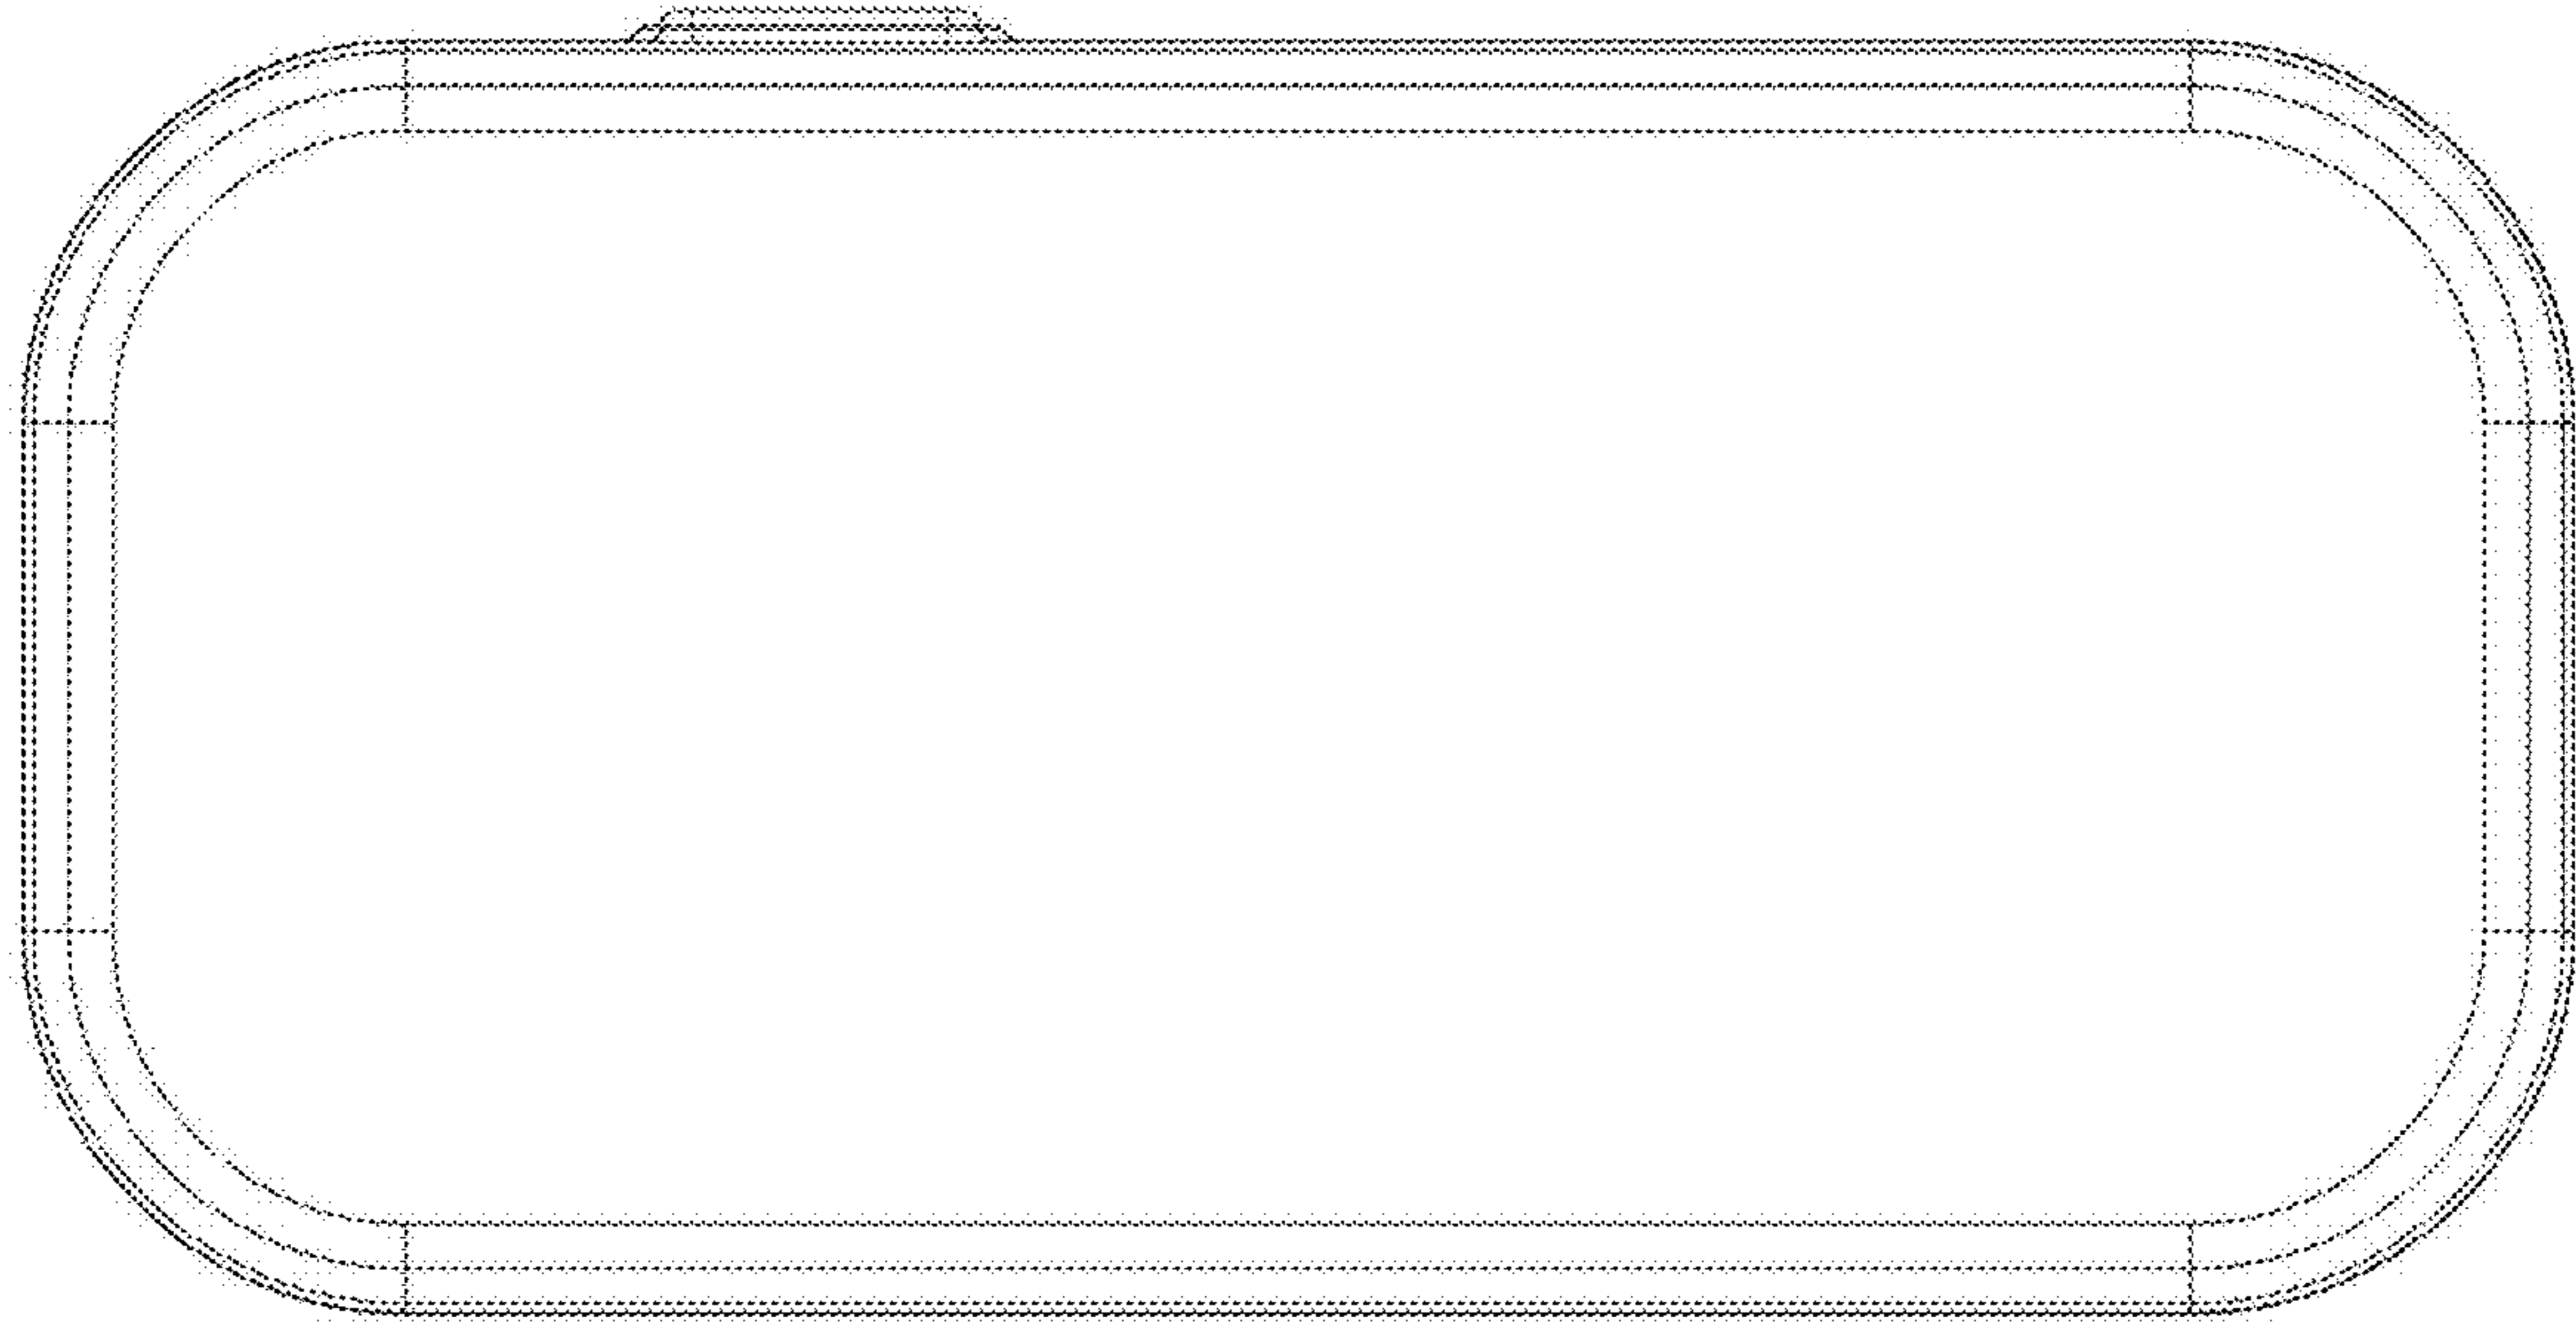


1.2

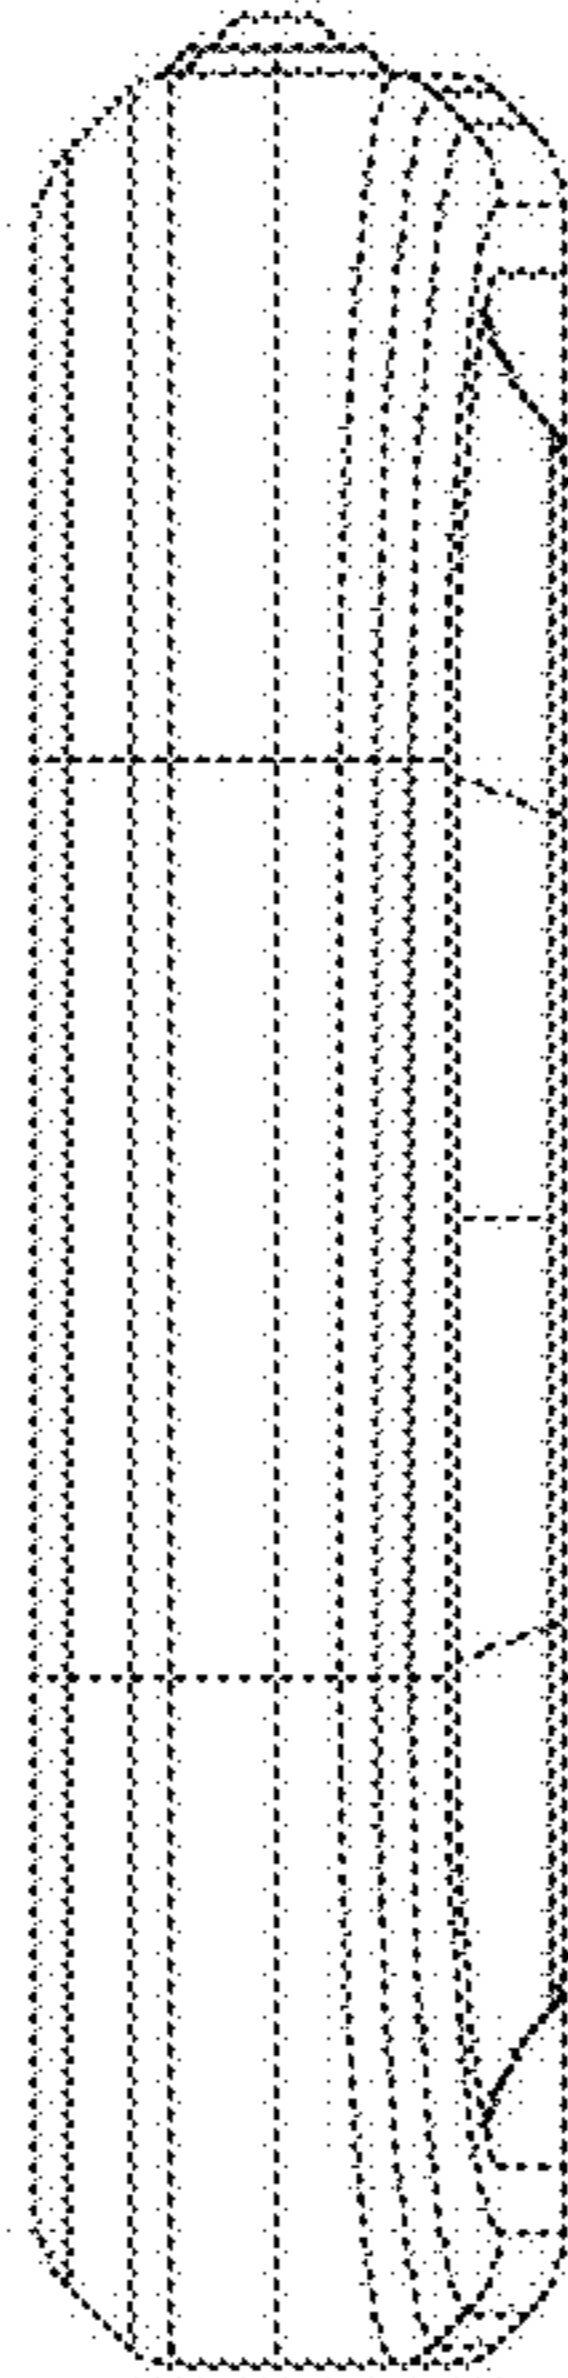


1.3

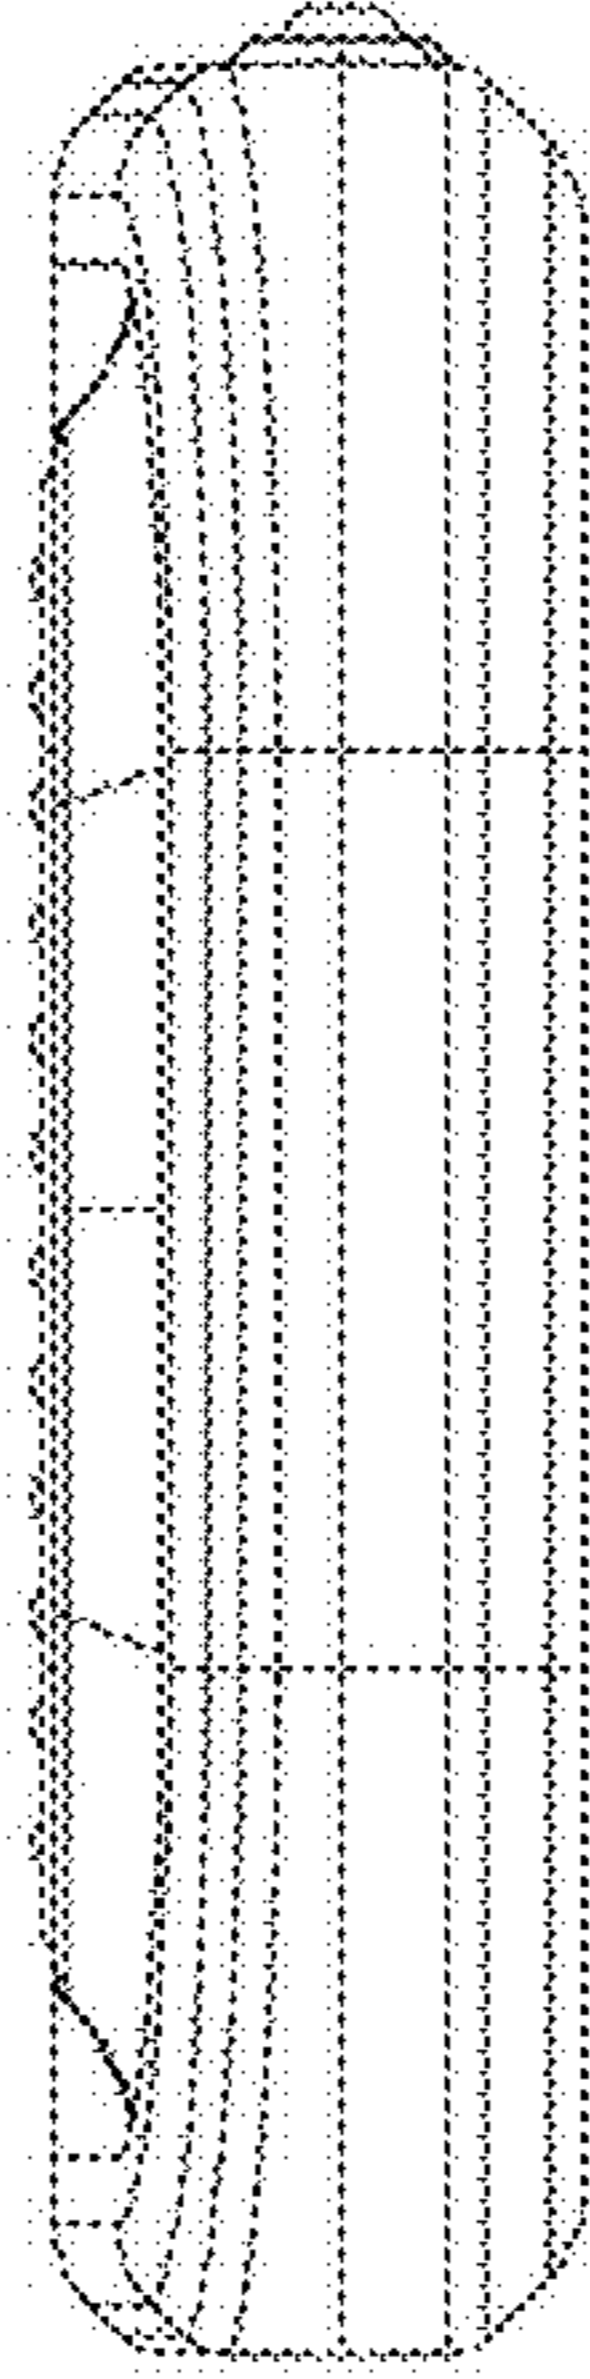

1.4

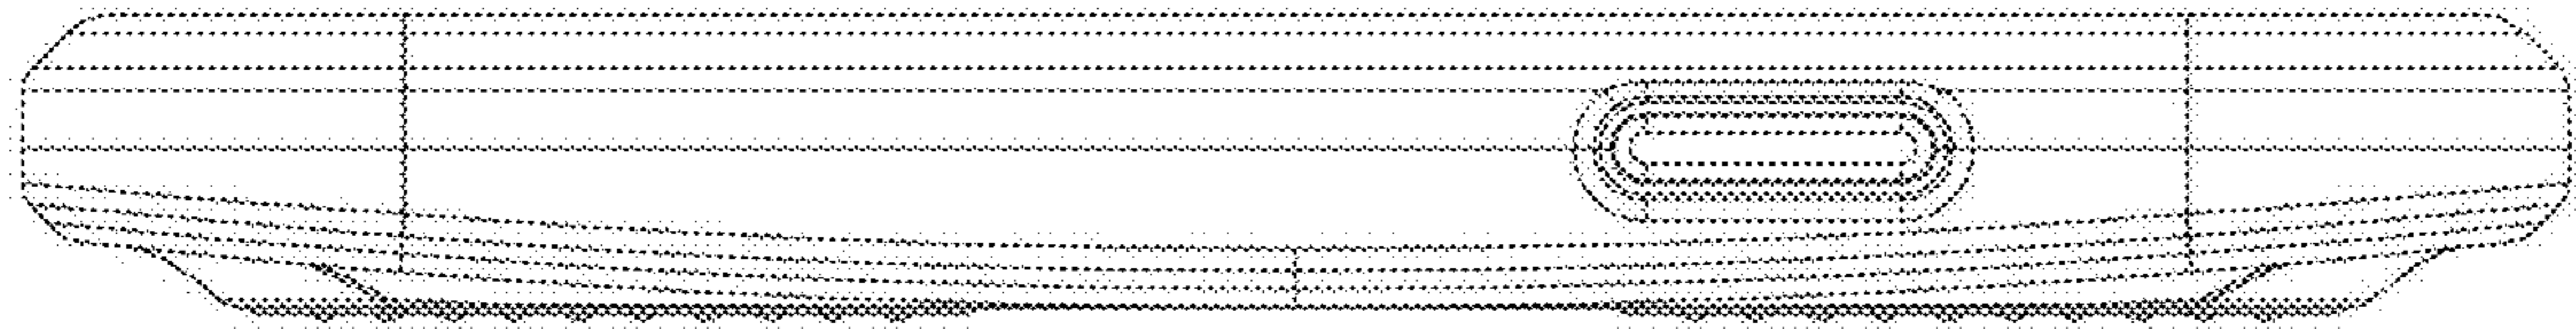

1.5

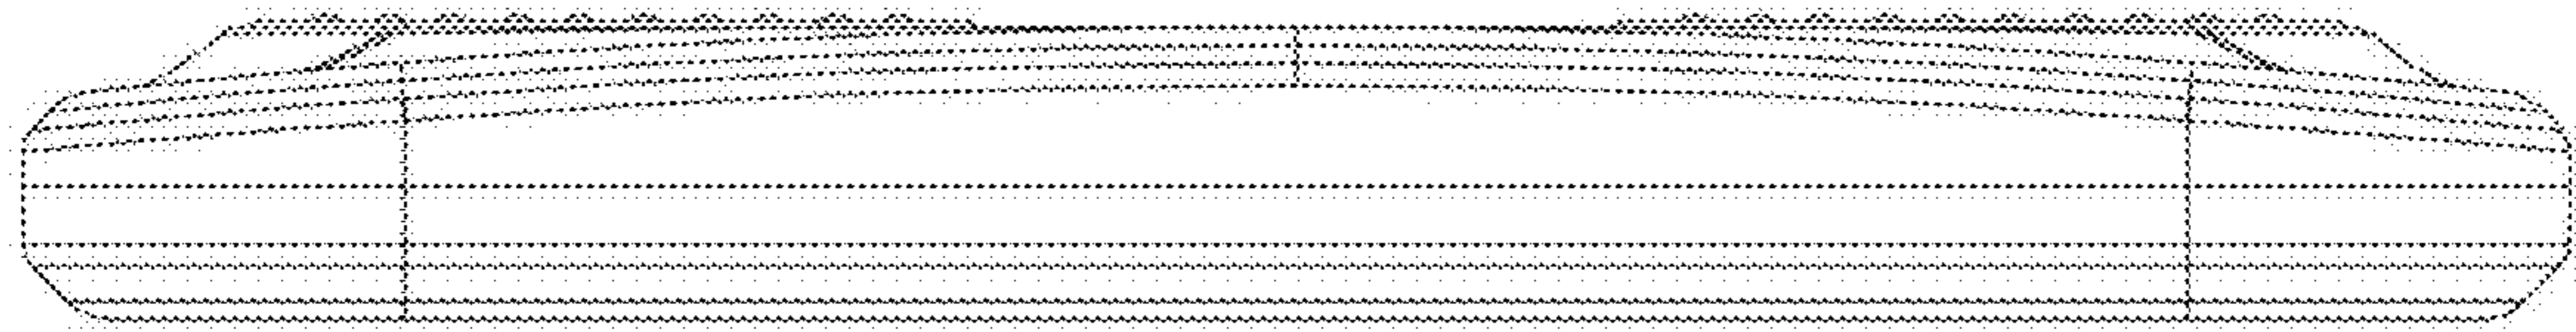

1.6



