

(12)

United States Design Patent

Cao

(10)

Patent No.:

US D982,767 S

(45)

Date of Patent:

** Apr. 4, 2023

(54) LOW-FREQUENCY MASSAGE DEVICE

(71) Applicant: FAMIDOC TECHNOLOGY CO., LTD., Dongguan (CN)

(72) Inventor: Liang Cao, Dongguan (CN)

(73) Assignee: FAMIDOC TECHNOLOGY CO., LTD., Dongguan (CN)

(**) Term: 15 Years

(21) Appl. No.: 29/779,052

(22) Filed: Apr. 16, 2021

(30) Foreign Application Priority Data

Apr. 13, 2021 (EM) 008500292

(51) LOC (14) Cl. 24-01

(52) U.S. Cl. USPC D24/215; D24/200

(58) Field of Classification Search
USPC D24/177, 186, 200, 211, 212, 213, 214, D24/215, 232; D10/57; D14/138 AA, D14/138 AD, 138 R, 140, 142
CPC H04M 1/0266; A61N 1/0456; A61N 1/37247; A61N 1/36171; A61N 1/3603; A61N 1/40; A61N 2007/0026; A61H 39/002; A61H 2201/5043; A61H 2201/5046; A61H 2230/085; A61H 2230/045; A61H 39/007; A61H 2230/10
See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

D750,263 S	*	2/2016	Shigeno	D24/200
D757,292 S	*	5/2016	Chen	D24/215
D758,605 S	*	6/2016	Chen	D24/215
D758,606 S	*	6/2016	Chen	D24/215
D759,263 S	*	6/2016	Chen	D24/215

D762,872 S	*	8/2016	Chen	D24/215
D813,407 S	*	3/2018	Chen	D24/215
D813,408 S	*	3/2018	Chen	D24/215
D822,216 S	*	7/2018	Barker	D24/186
D836,788 S	*	12/2018	Peng	D24/200
D879,983 S	*	3/2020	Wang	D24/200
D893,735 S	*	8/2020	Yin	D24/200
D893,736 S	*	8/2020	Yin	D24/200
D898,692 S	*	10/2020	Lee	D14/138 AD
D910,868 S	*	2/2021	Stewart	D24/215
D928,774 S	*	8/2021	Seo	D14/138 AA
D945,385 S	*	3/2022	Takahashi	D14/138 R

(Continued)

OTHER PUBLICATIONS

Amazon, "Famidoc TENS EMS_Muscle Stimulator", Date First Available: Nov. 11, 2021. <https://www.amazon.com/Stimulator-Channels-Intensity-Shoulder-Electronic/dp/B09LLC915H> (Year: 2021).*

(Continued)

Primary Examiner — Michael A Maharajh


(57) CLAIM

The ornamental design for a low-frequency massage device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a low-frequency massage device showing my new design;
FIG. 2 is another perspective view thereof;
FIG. 3 is a front elevational view thereof;
FIG. 4 is a rear elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a right side elevational view thereof;
FIG. 7 is a top plan view thereof; and,
FIG. 8 is a bottom plan view thereof.
The broken lines in the drawings depict portions of the low-frequency massage device that form no part of the claimed design.

1 Claim, 8 Drawing Sheets

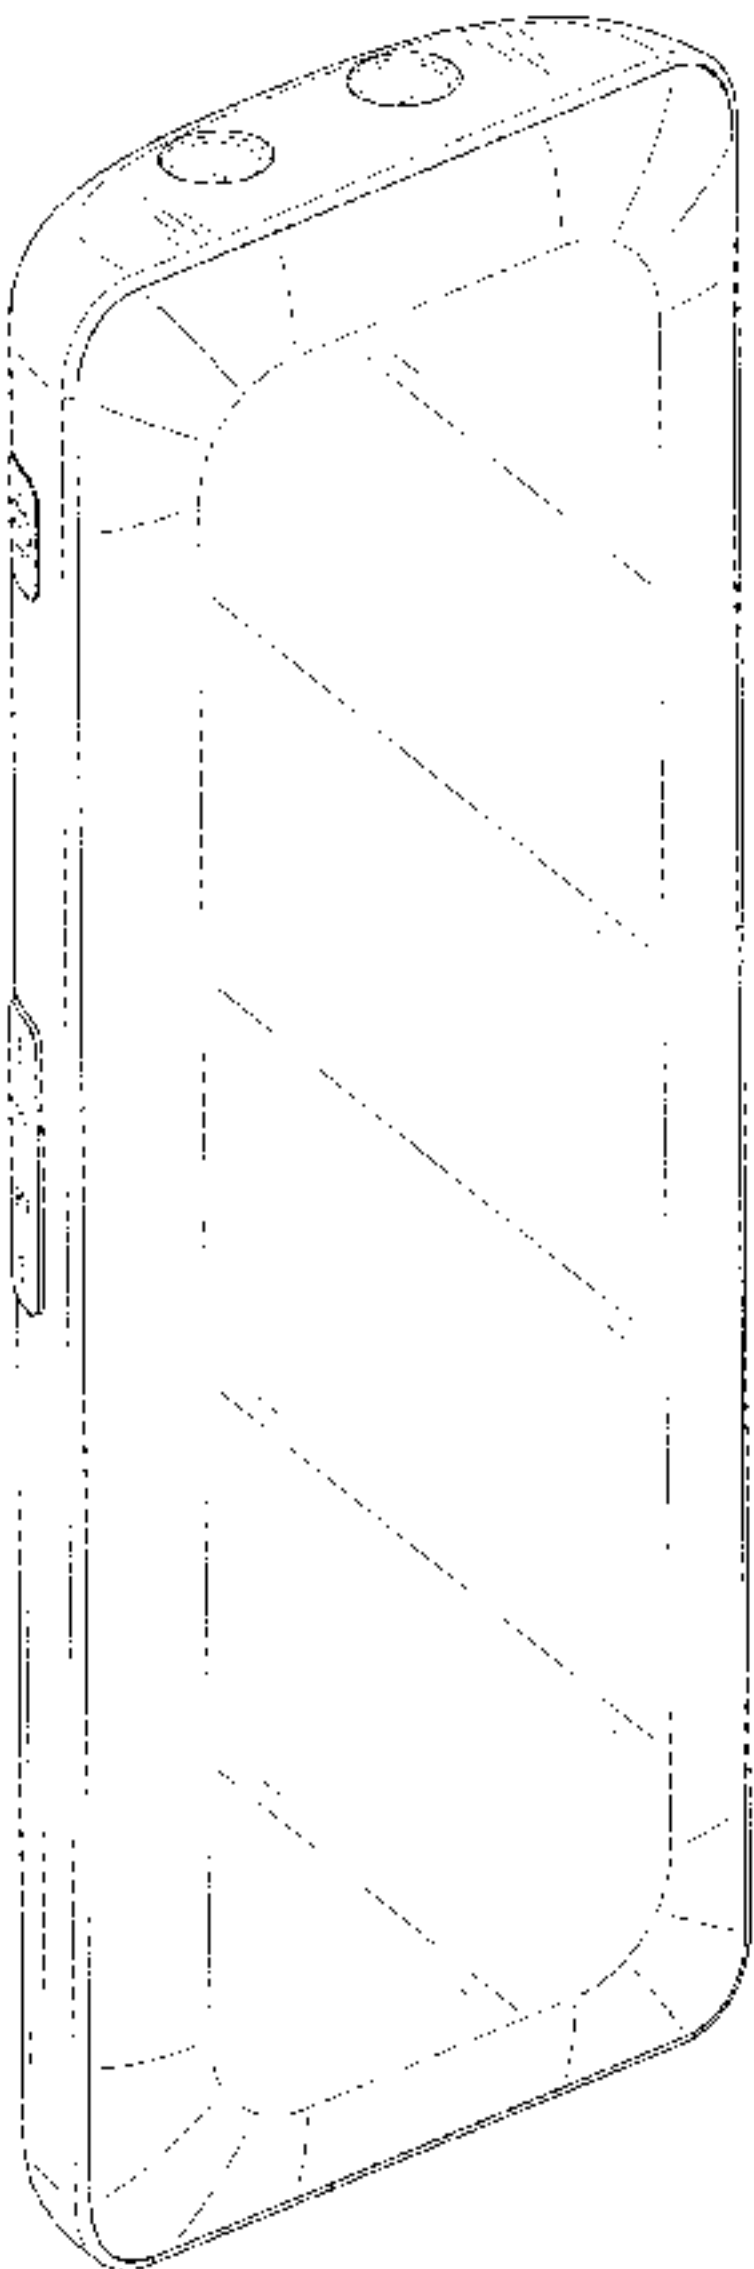

(56) **References Cited**

U.S. PATENT DOCUMENTS

D947,804 S * 4/2022 McPhail D14/138 AA
D948,741 S * 4/2022 Jin D24/215
D955,357 S * 6/2022 Sun D14/138 AD
D961,786 S * 8/2022 Chen D24/200

OTHER PUBLICATIONS

Amazon, “Belifu_TENS EMS Muscle Stimulator”, Feb. 12, 2022.
https://www.amazon.com/Belifu-Stimulator-Independent-Temperature-Intensities/dp/B09KNLJDHY?ref_=ast_sto_dp&th=1&psc=1 (Year: 2022).*

* cited by examiner

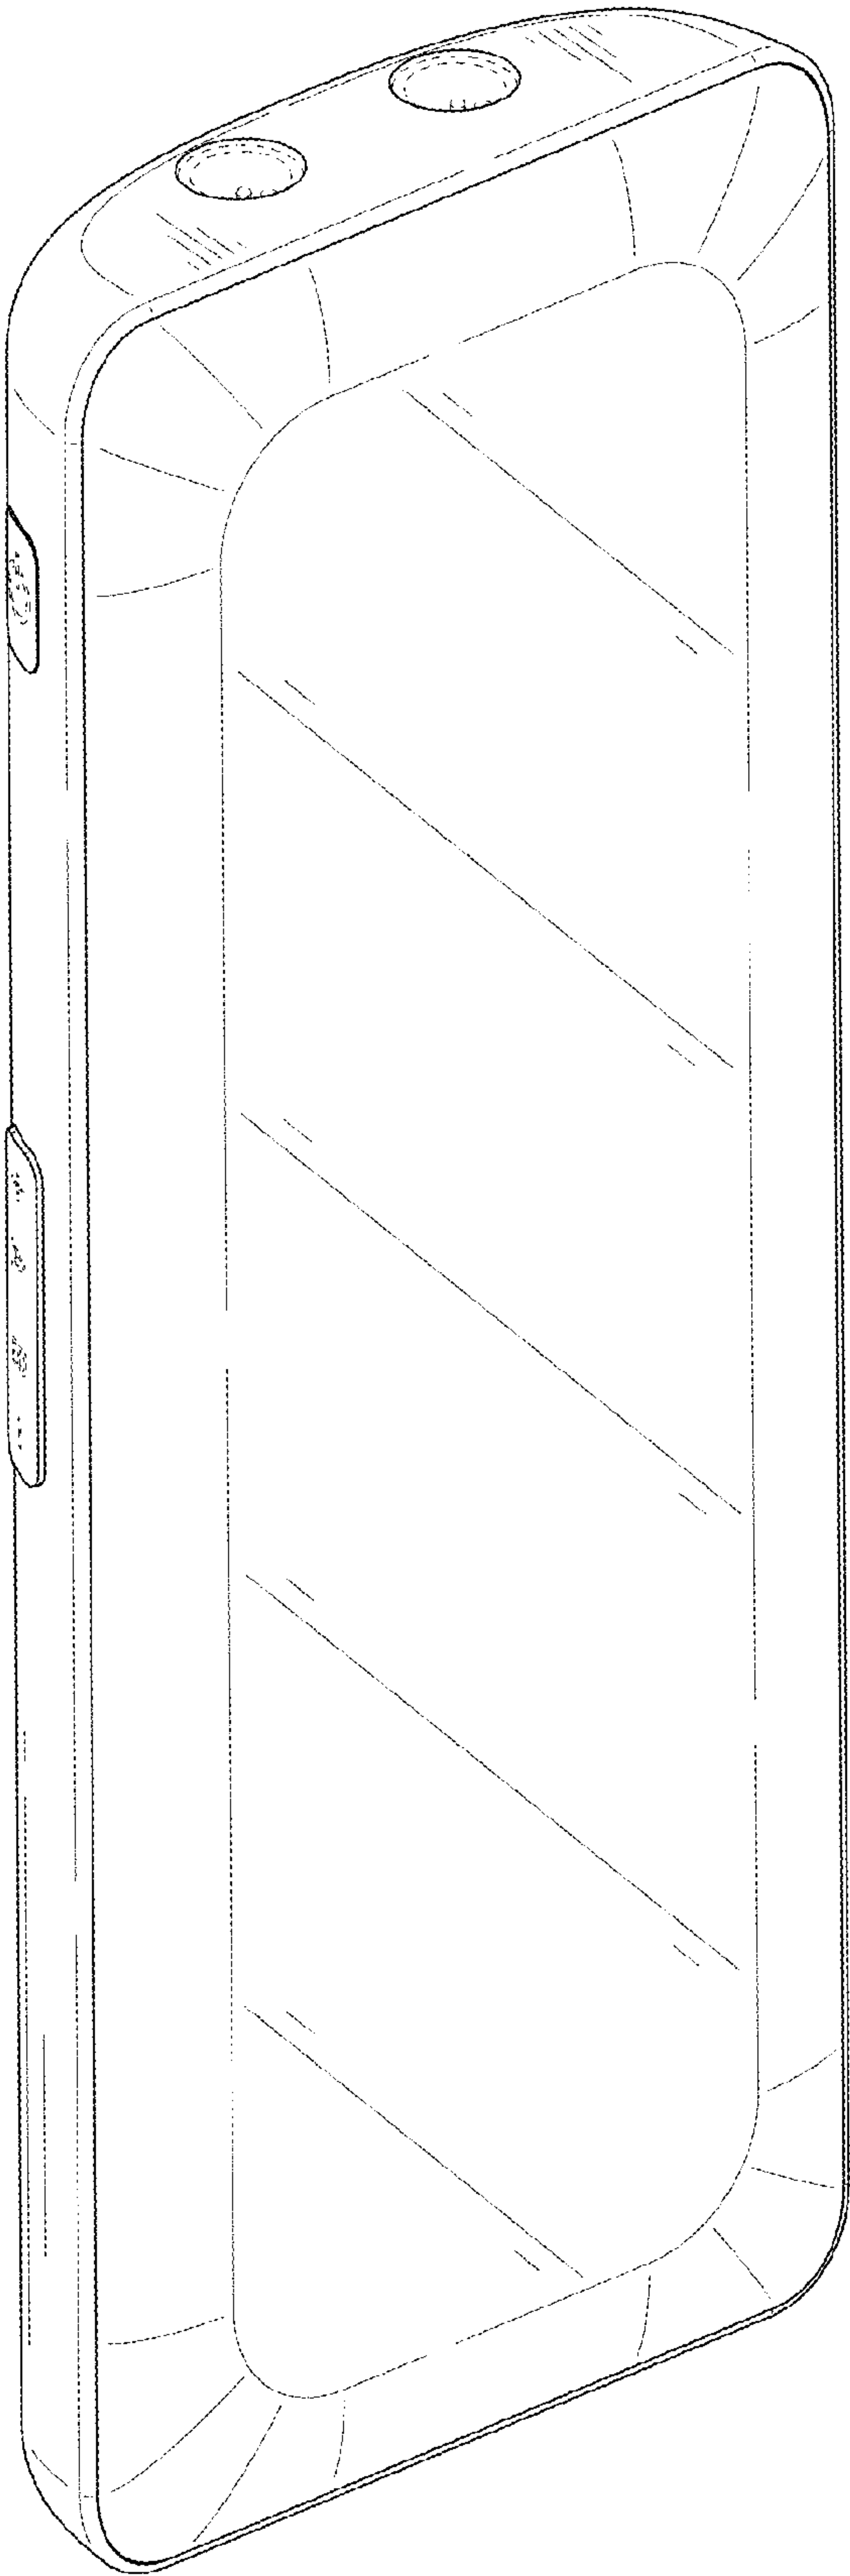


FIG. 1

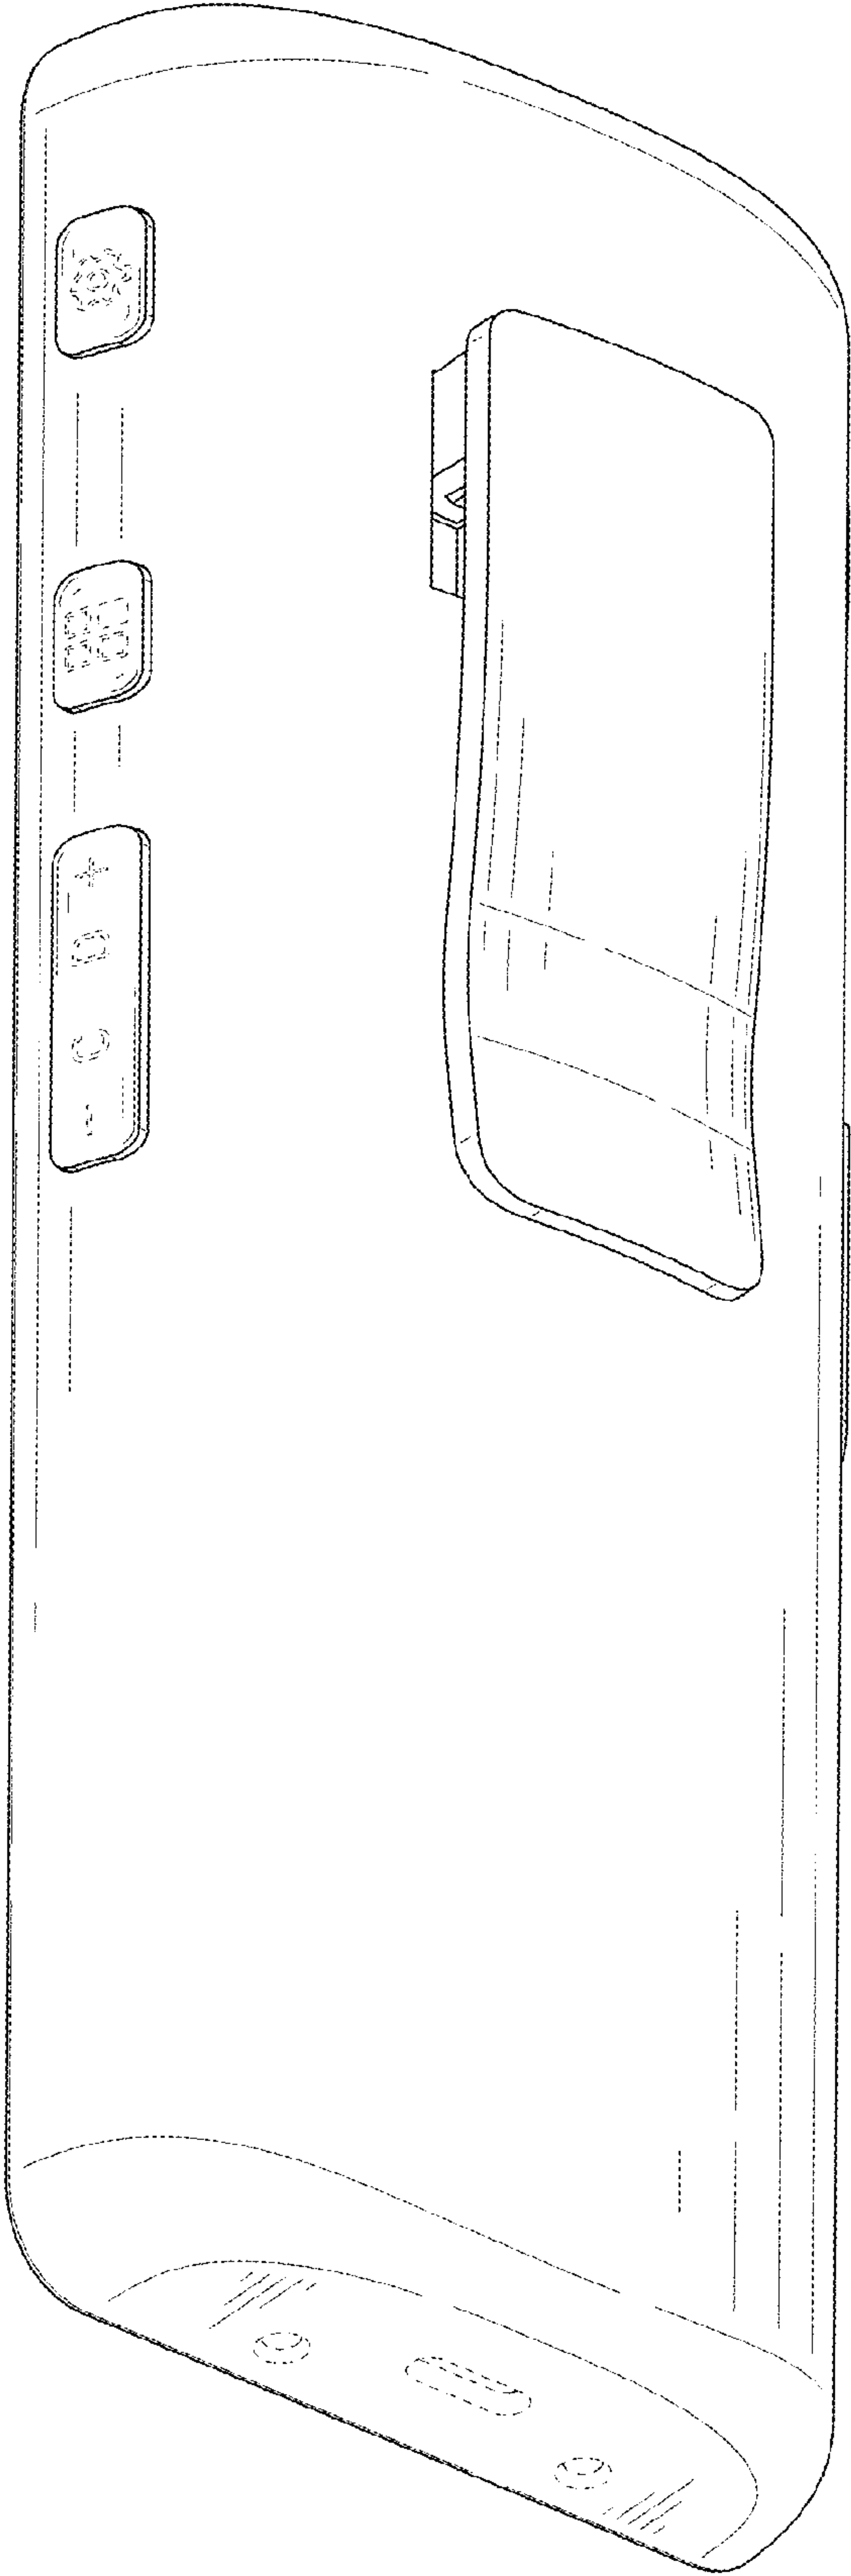


FIG. 2

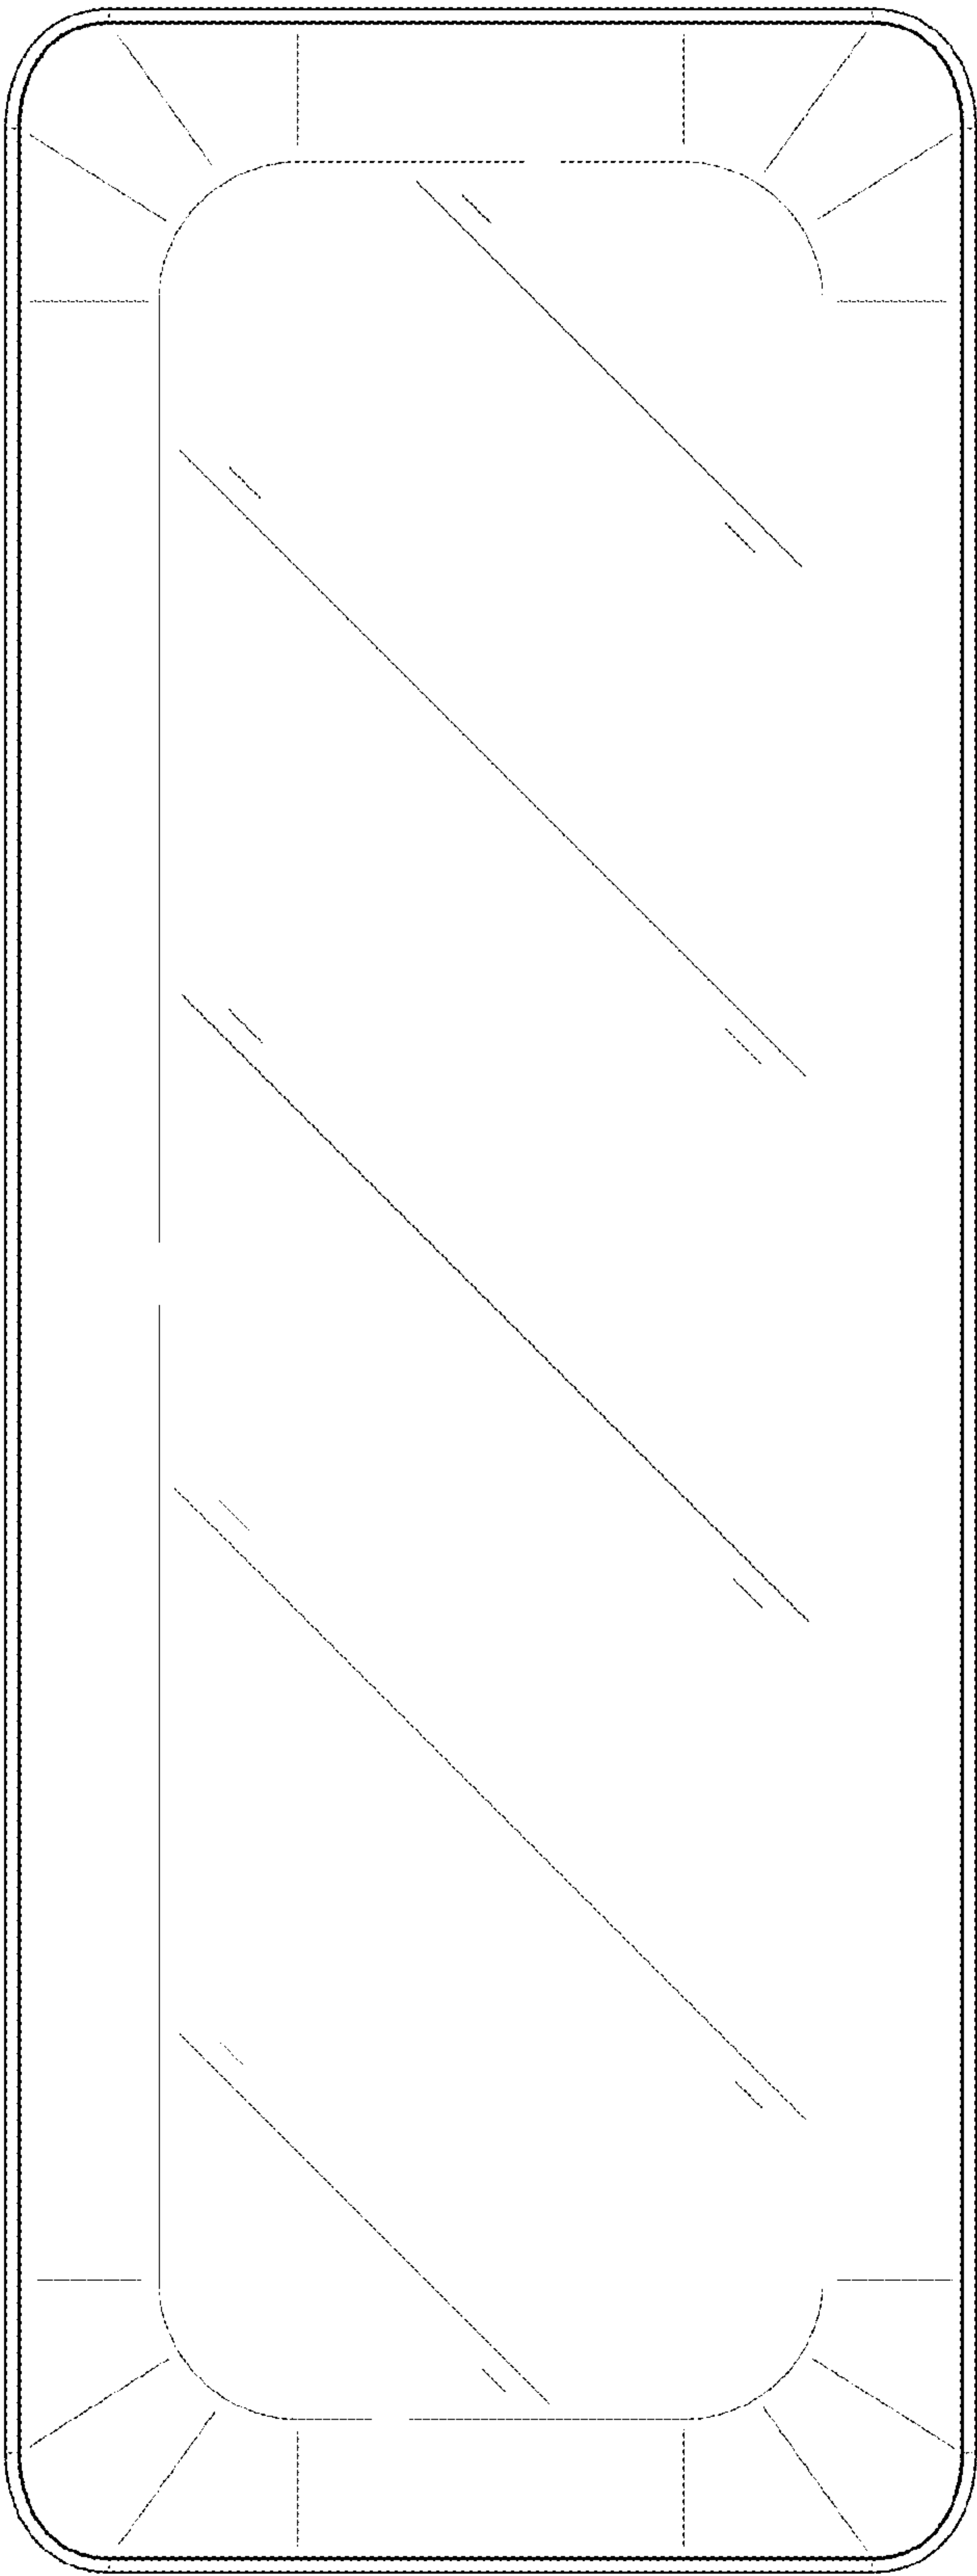


FIG. 3

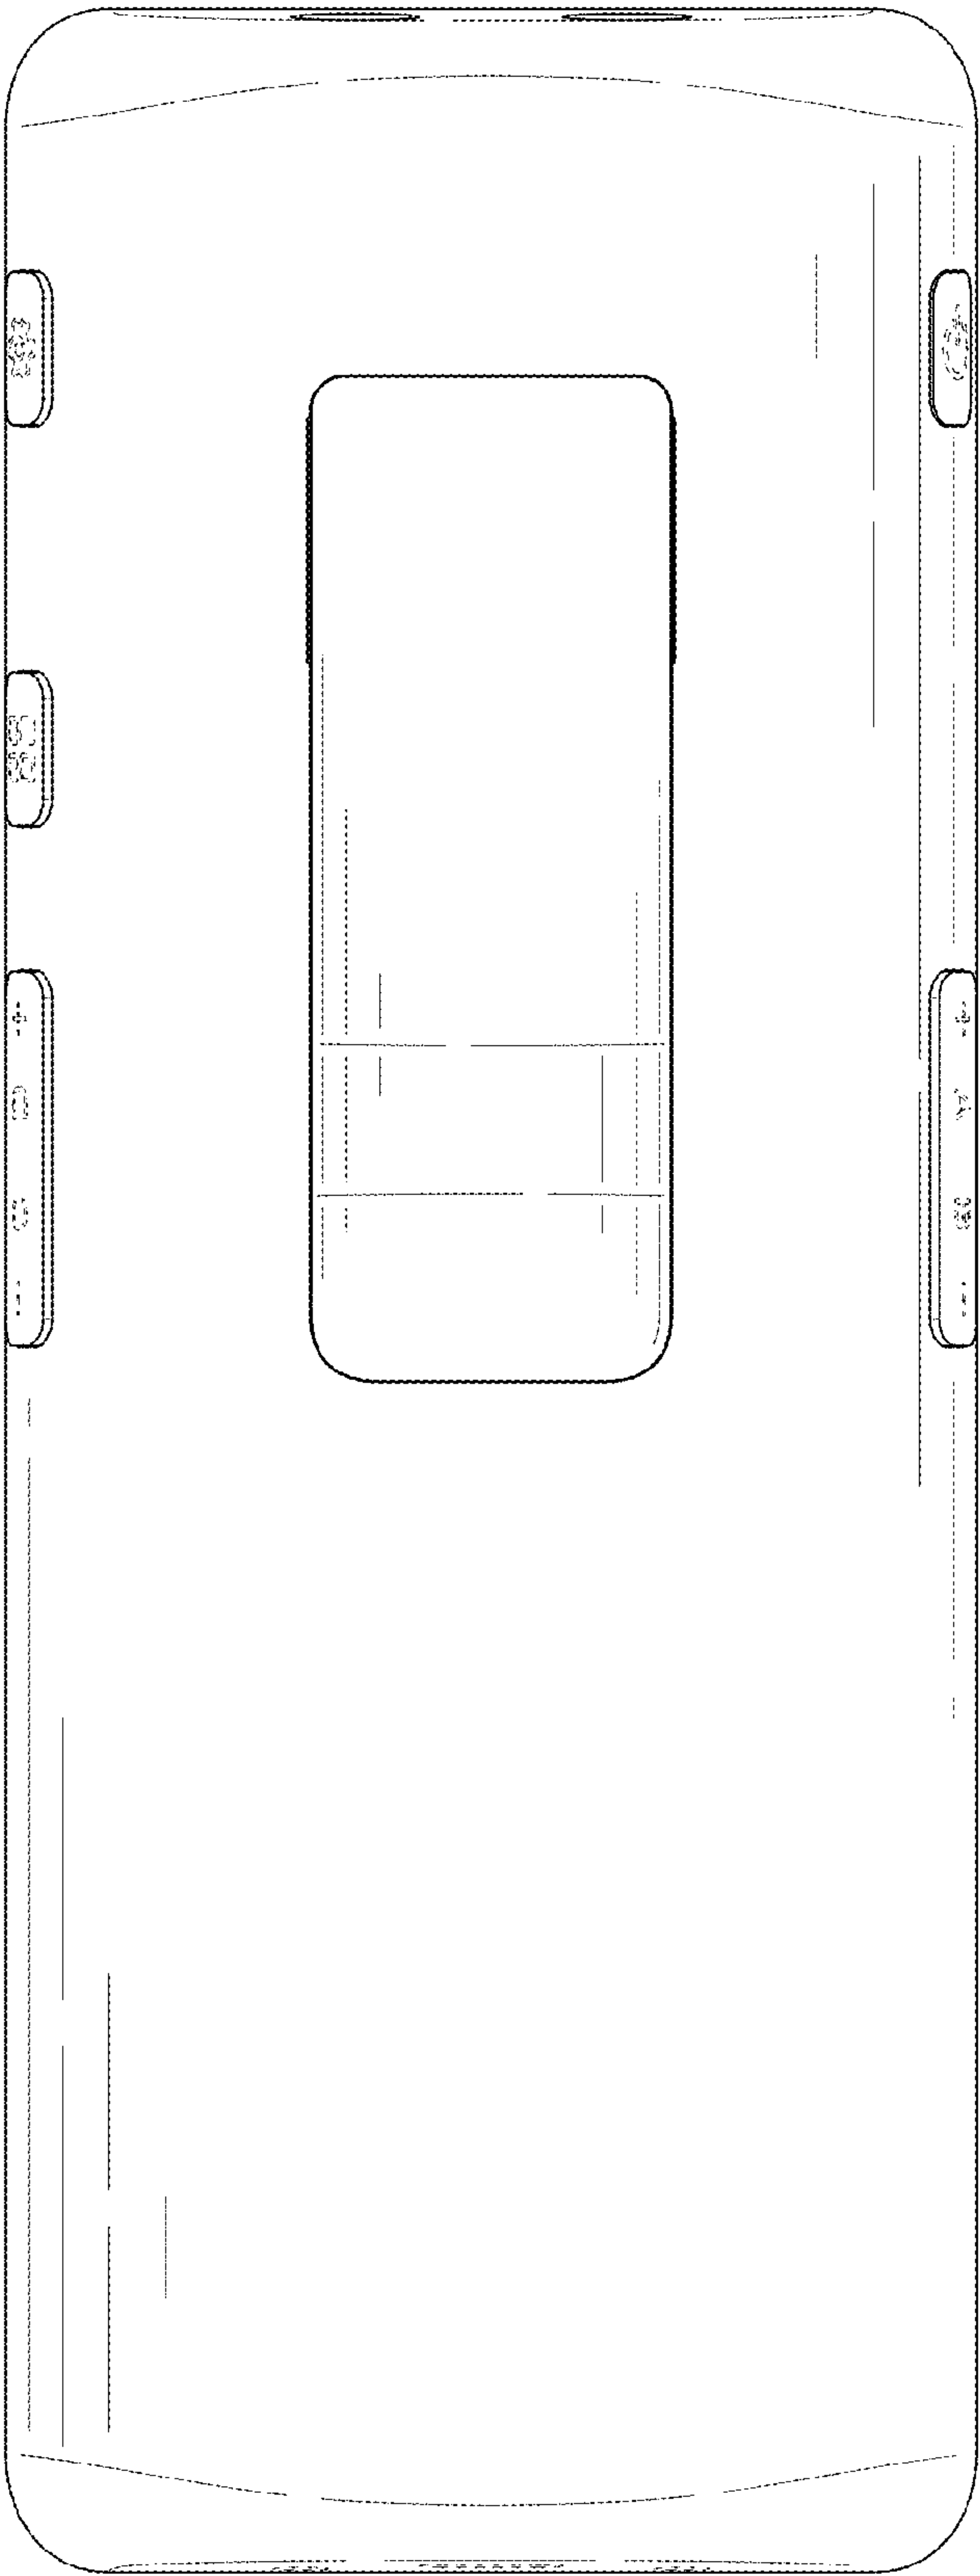


FIG. 4

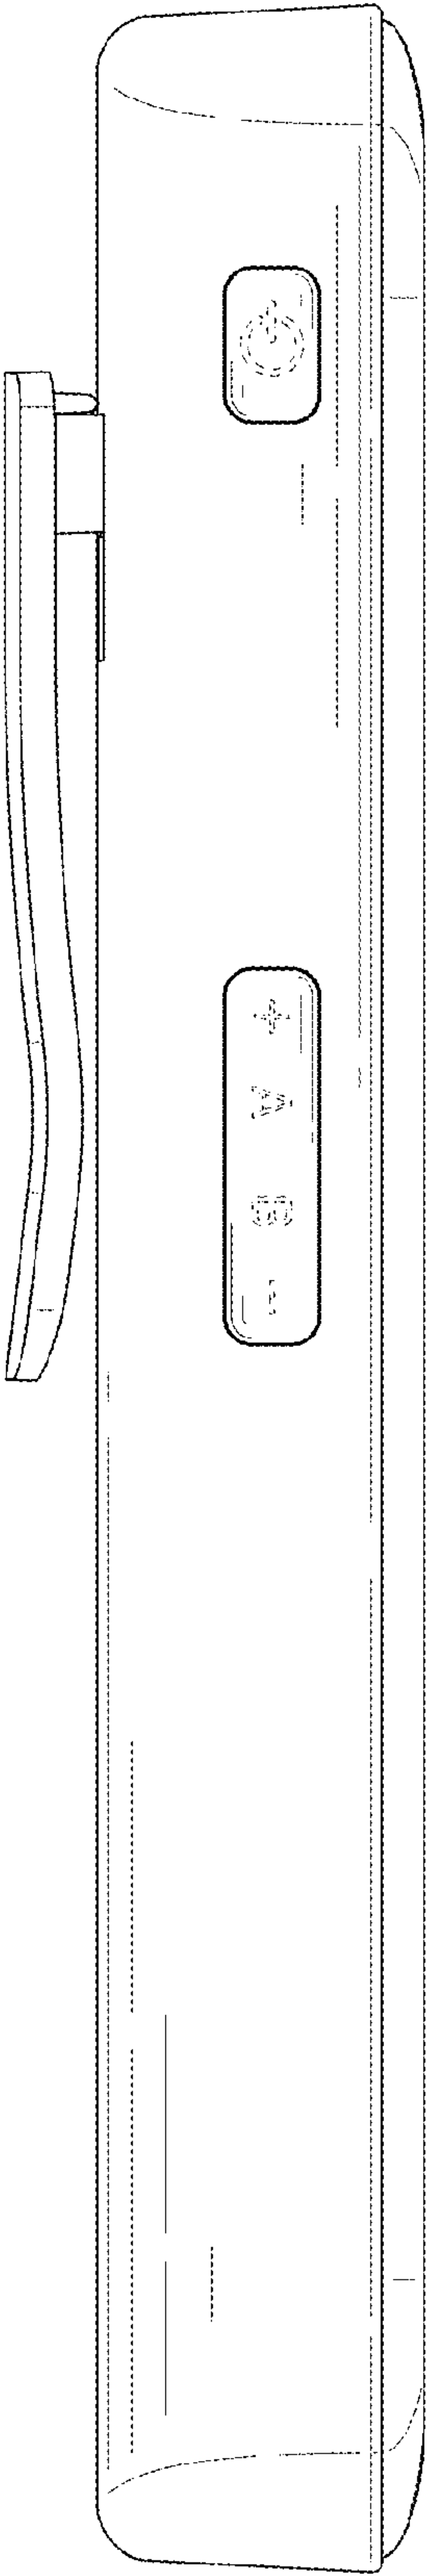


FIG. 5

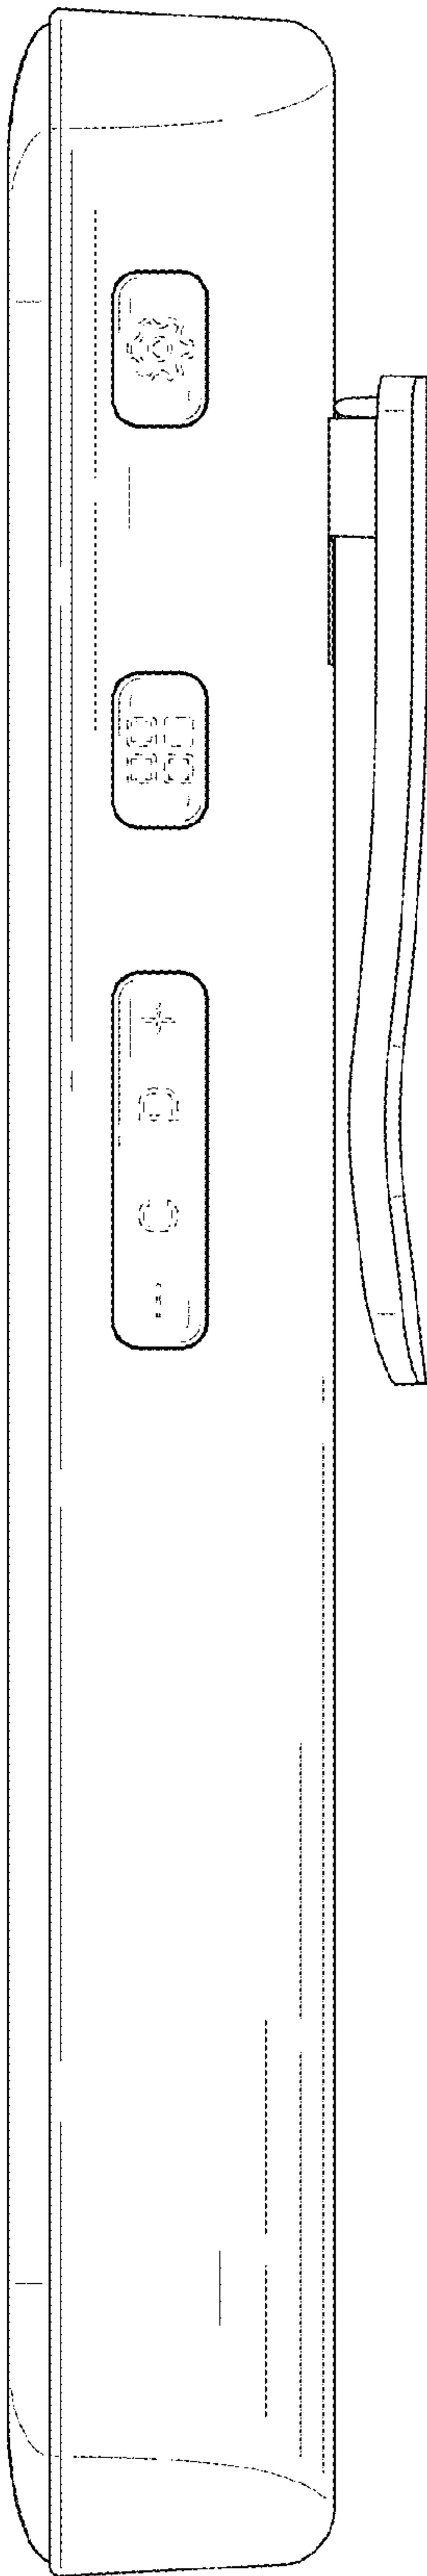


FIG. 6

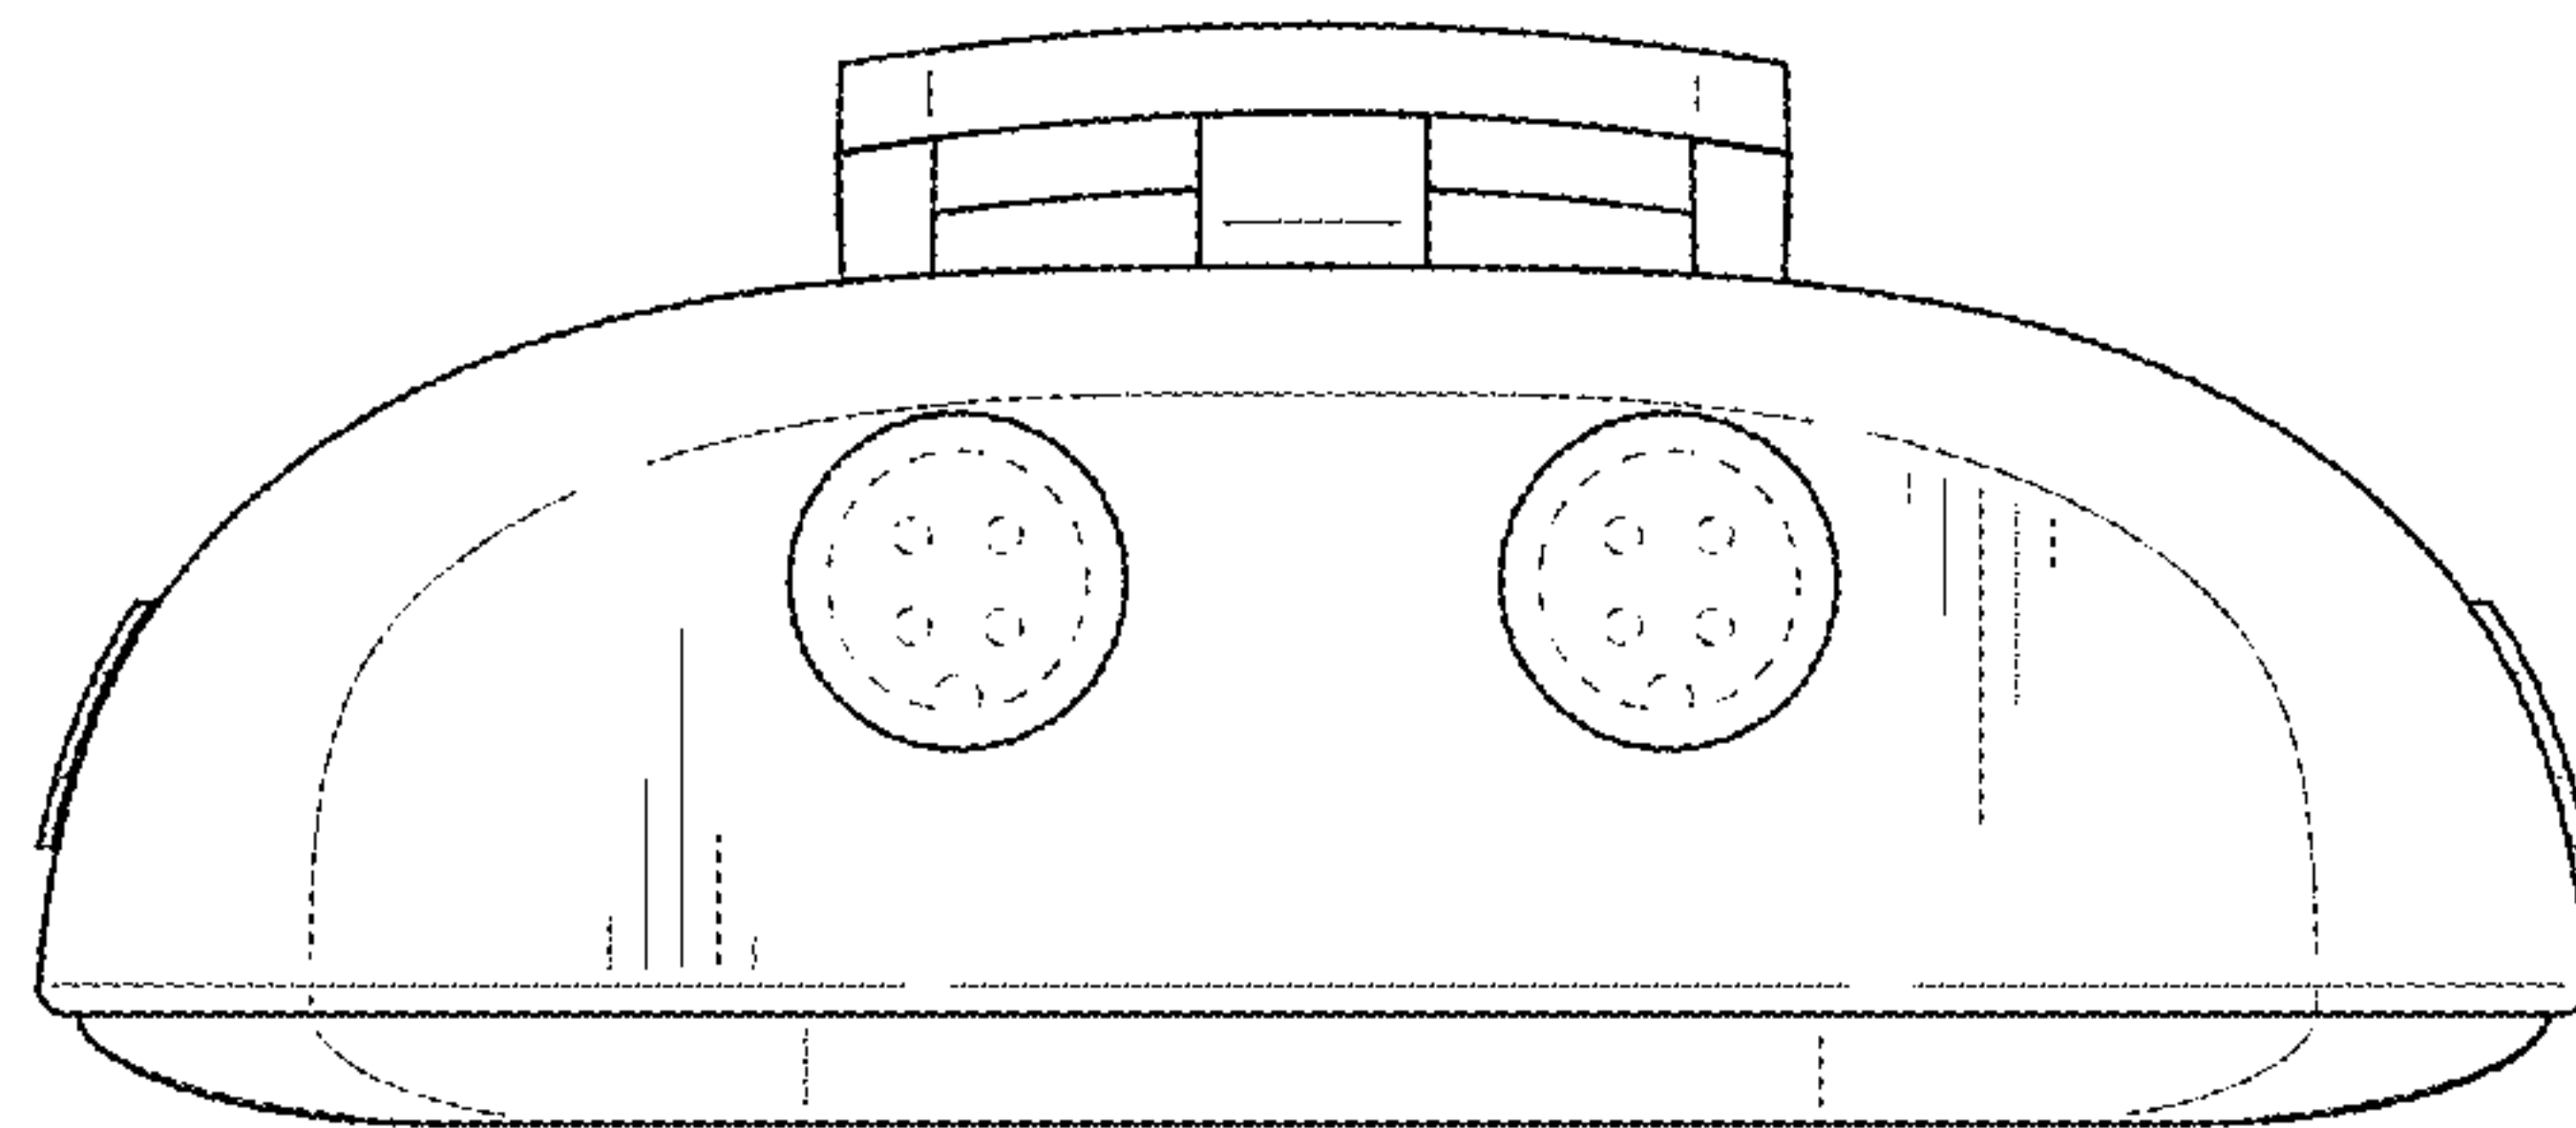


FIG. 7

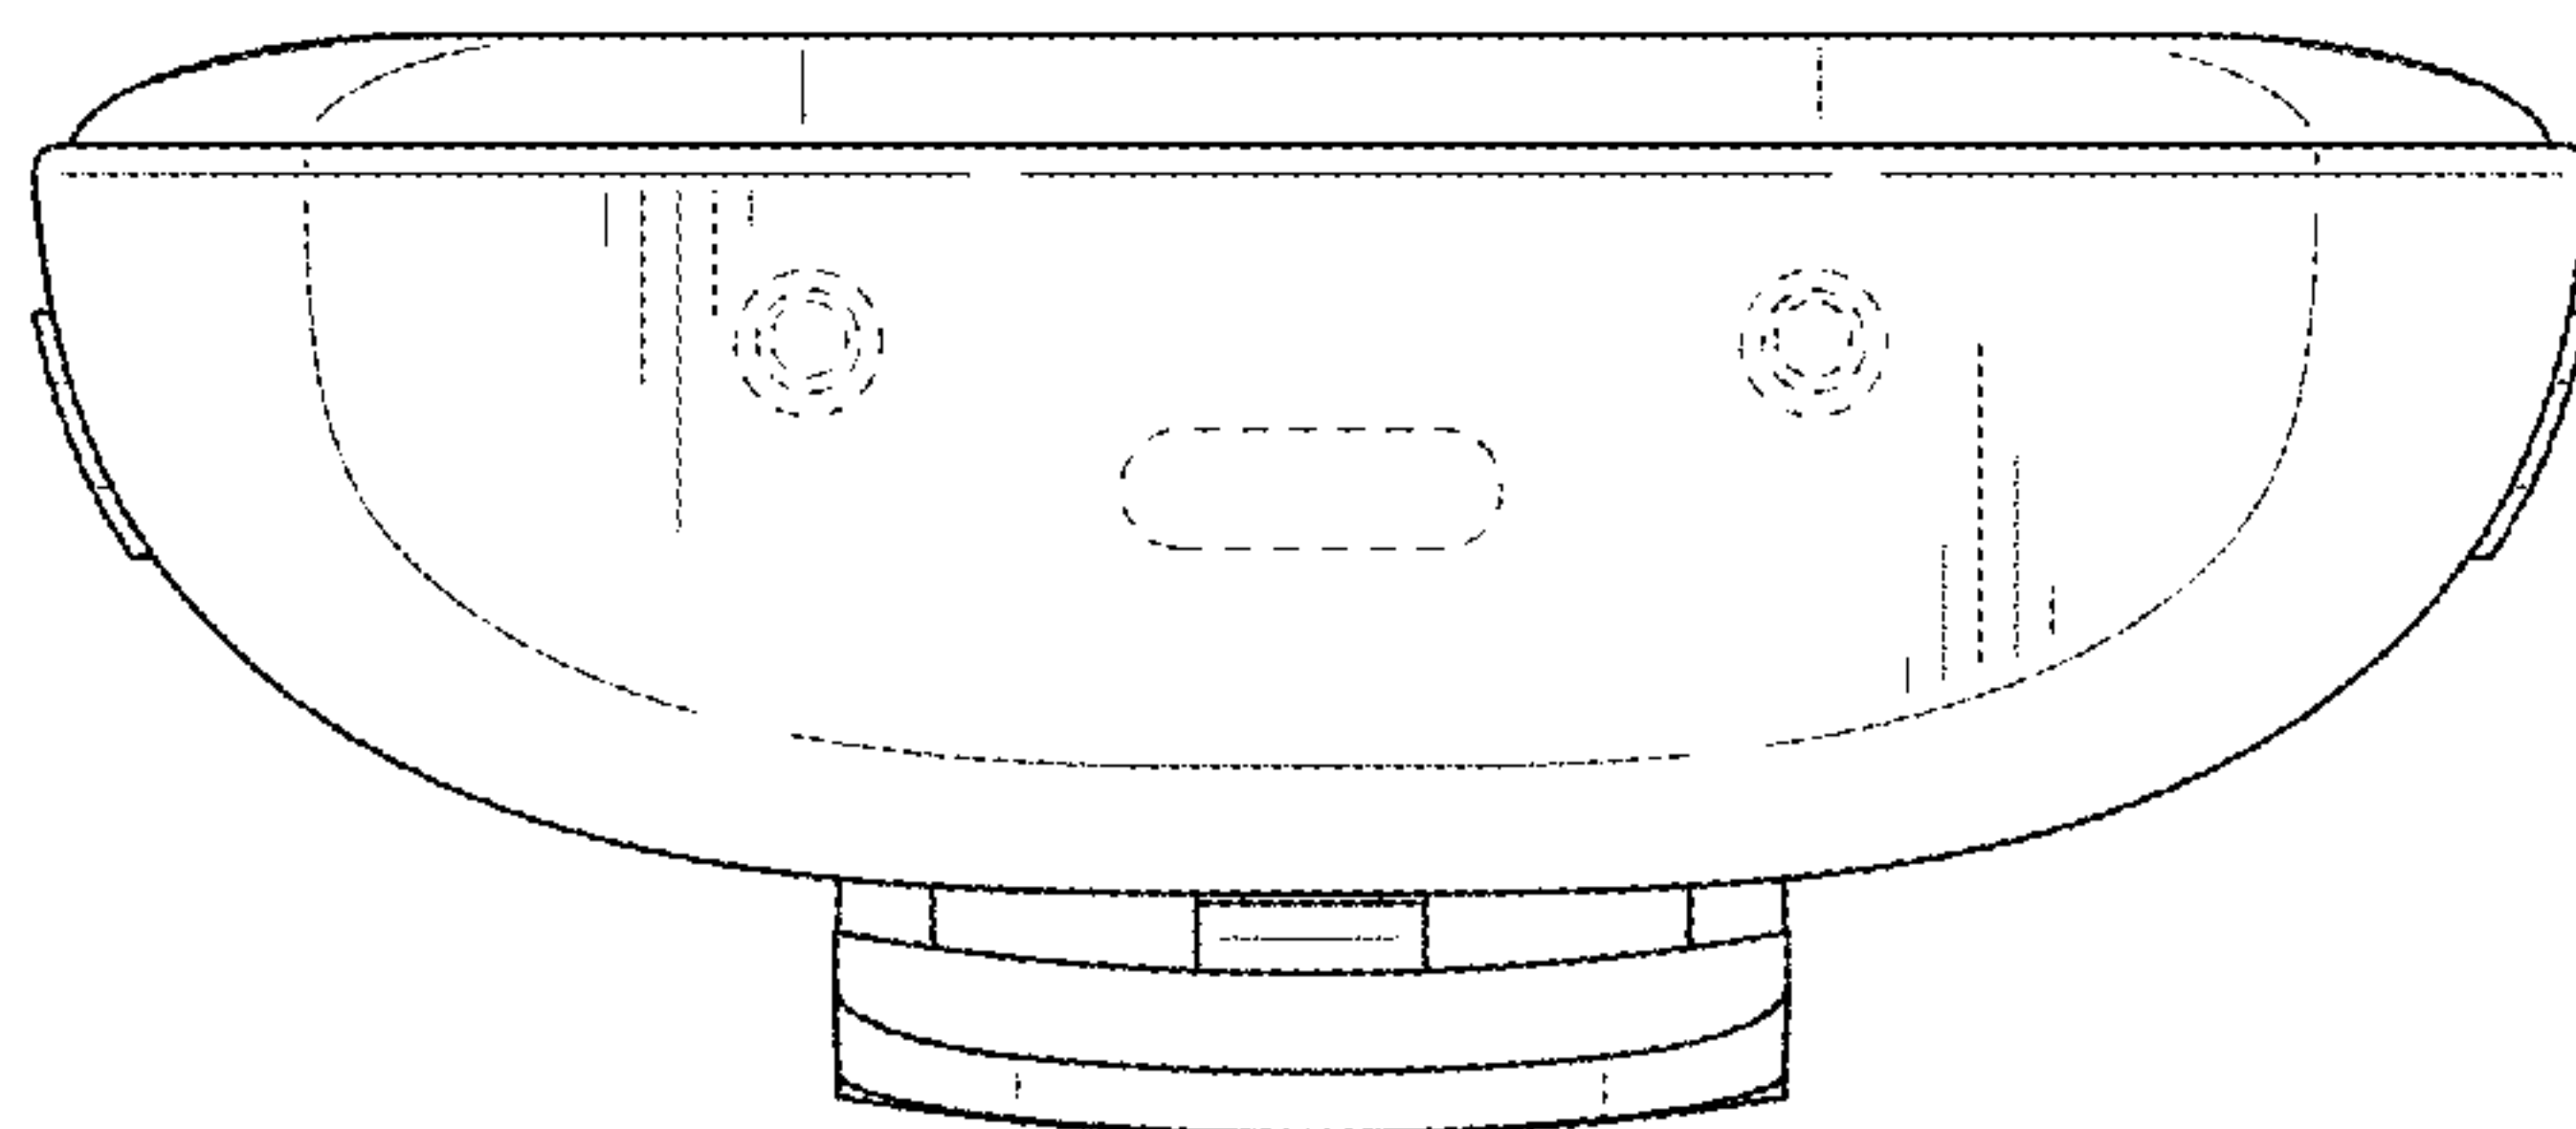


FIG. 8