



US00D983682S

(12) **United States Design Patent**  
**Lubjenka et al.**

(10) **Patent No.:** **US D983,682 S**  
(45) **Date of Patent:** **\*\* Apr. 18, 2023**

(54) **CHEMICAL ANALYSIS INSTRUMENT**

- (71) Applicant: **NICOYA LIFESCIENCES, INC.**,  
Kitchener (CA)
- (72) Inventors: **Mandy Lubjenka**, Durham (CA);  
**Trang Tina Thi Thuy Nguyen**,  
Waterloo (CA); **Ryan Denomme**,  
Kitchener (CA); **Patrick Sterlina**,  
Apex, NC (US); **Arjun Sudarsan**,  
Carlsbad, CA (US); **Jason Garr**,  
Hamilton (CA); **Krishna Iyer**, Waterloo  
(CA); **Charles Curbbun**, Solana Beach,  
CA (US); **Lee-Anne Stossell**, San  
Marcos, CA (US)
- (73) Assignee: **Nicoya Lifesciences, Inc.**, Kitchener  
(CA)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/721,168**

(22) Filed: **Jan. 17, 2020**

(51) **LOC (14) Cl.** ..... **10-04**

(52) **U.S. Cl.**  
USPC ..... **D10/81; D24/232**

(58) **Field of Classification Search**  
USPC ..... **D10/81-86, 94-103; D24/216, 185, 232**

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D750,989 S \* 3/2016 Shimizu ..... D10/81  
D848,880 S \* 5/2019 Smith ..... D10/81

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 303030578 \* 6/2014  
CN 305491051 \* 3/2019

(Continued)

**OTHER PUBLICATIONS**

Kitchener, On, ,the World's First Digital Benchtop SPR System, Nicoya Launches Alto, Date first available Jan. 23, 2020, [online]retrieved Nov. 10, 2021 ,available from <https://nicoyalife.com/blog/press-releases/alto-digital-spr-nicoya-press-release/> (Year: 202).\*

(Continued)

*Primary Examiner* — Keli L Hill

*Assistant Examiner* — Sara S Sahneh

(74) *Attorney, Agent, or Firm* — Wilson Sonsini Goodrich & Rosati

(57) **CLAIM**

The ornamental design for a chemical analysis instrument, as shown and described.

**DESCRIPTION**

FIG. 1 is a front left top perspective view of a chemical analysis instrument;

FIG. 2 is a front right top perspective view of the chemical analysis instrument of FIG. 1;

FIG. 3 is a back right bottom perspective view of the chemical analysis instrument of FIG. 1;

FIG. 4 is a front elevation view of the chemical analysis instrument of FIG. 1;

FIG. 5 is a back elevation view of the chemical analysis instrument of FIG. 1;

FIG. 6 is a left elevation view of the chemical analysis instrument of FIG. 1;



FIG. 7 is a right elevation view of the chemical analysis instrument of FIG. 1;

FIG. 8 is a top elevation view of the chemical analysis instrument of FIG. 1; and,

FIG. 9 is a bottom elevation view of the chemical analysis instrument of FIG. 1.

The broken lines shown are included for the purpose of illustrating portions of the chemical analysis instrument that form no part of the claims.

**1 Claim, 9 Drawing Sheets**

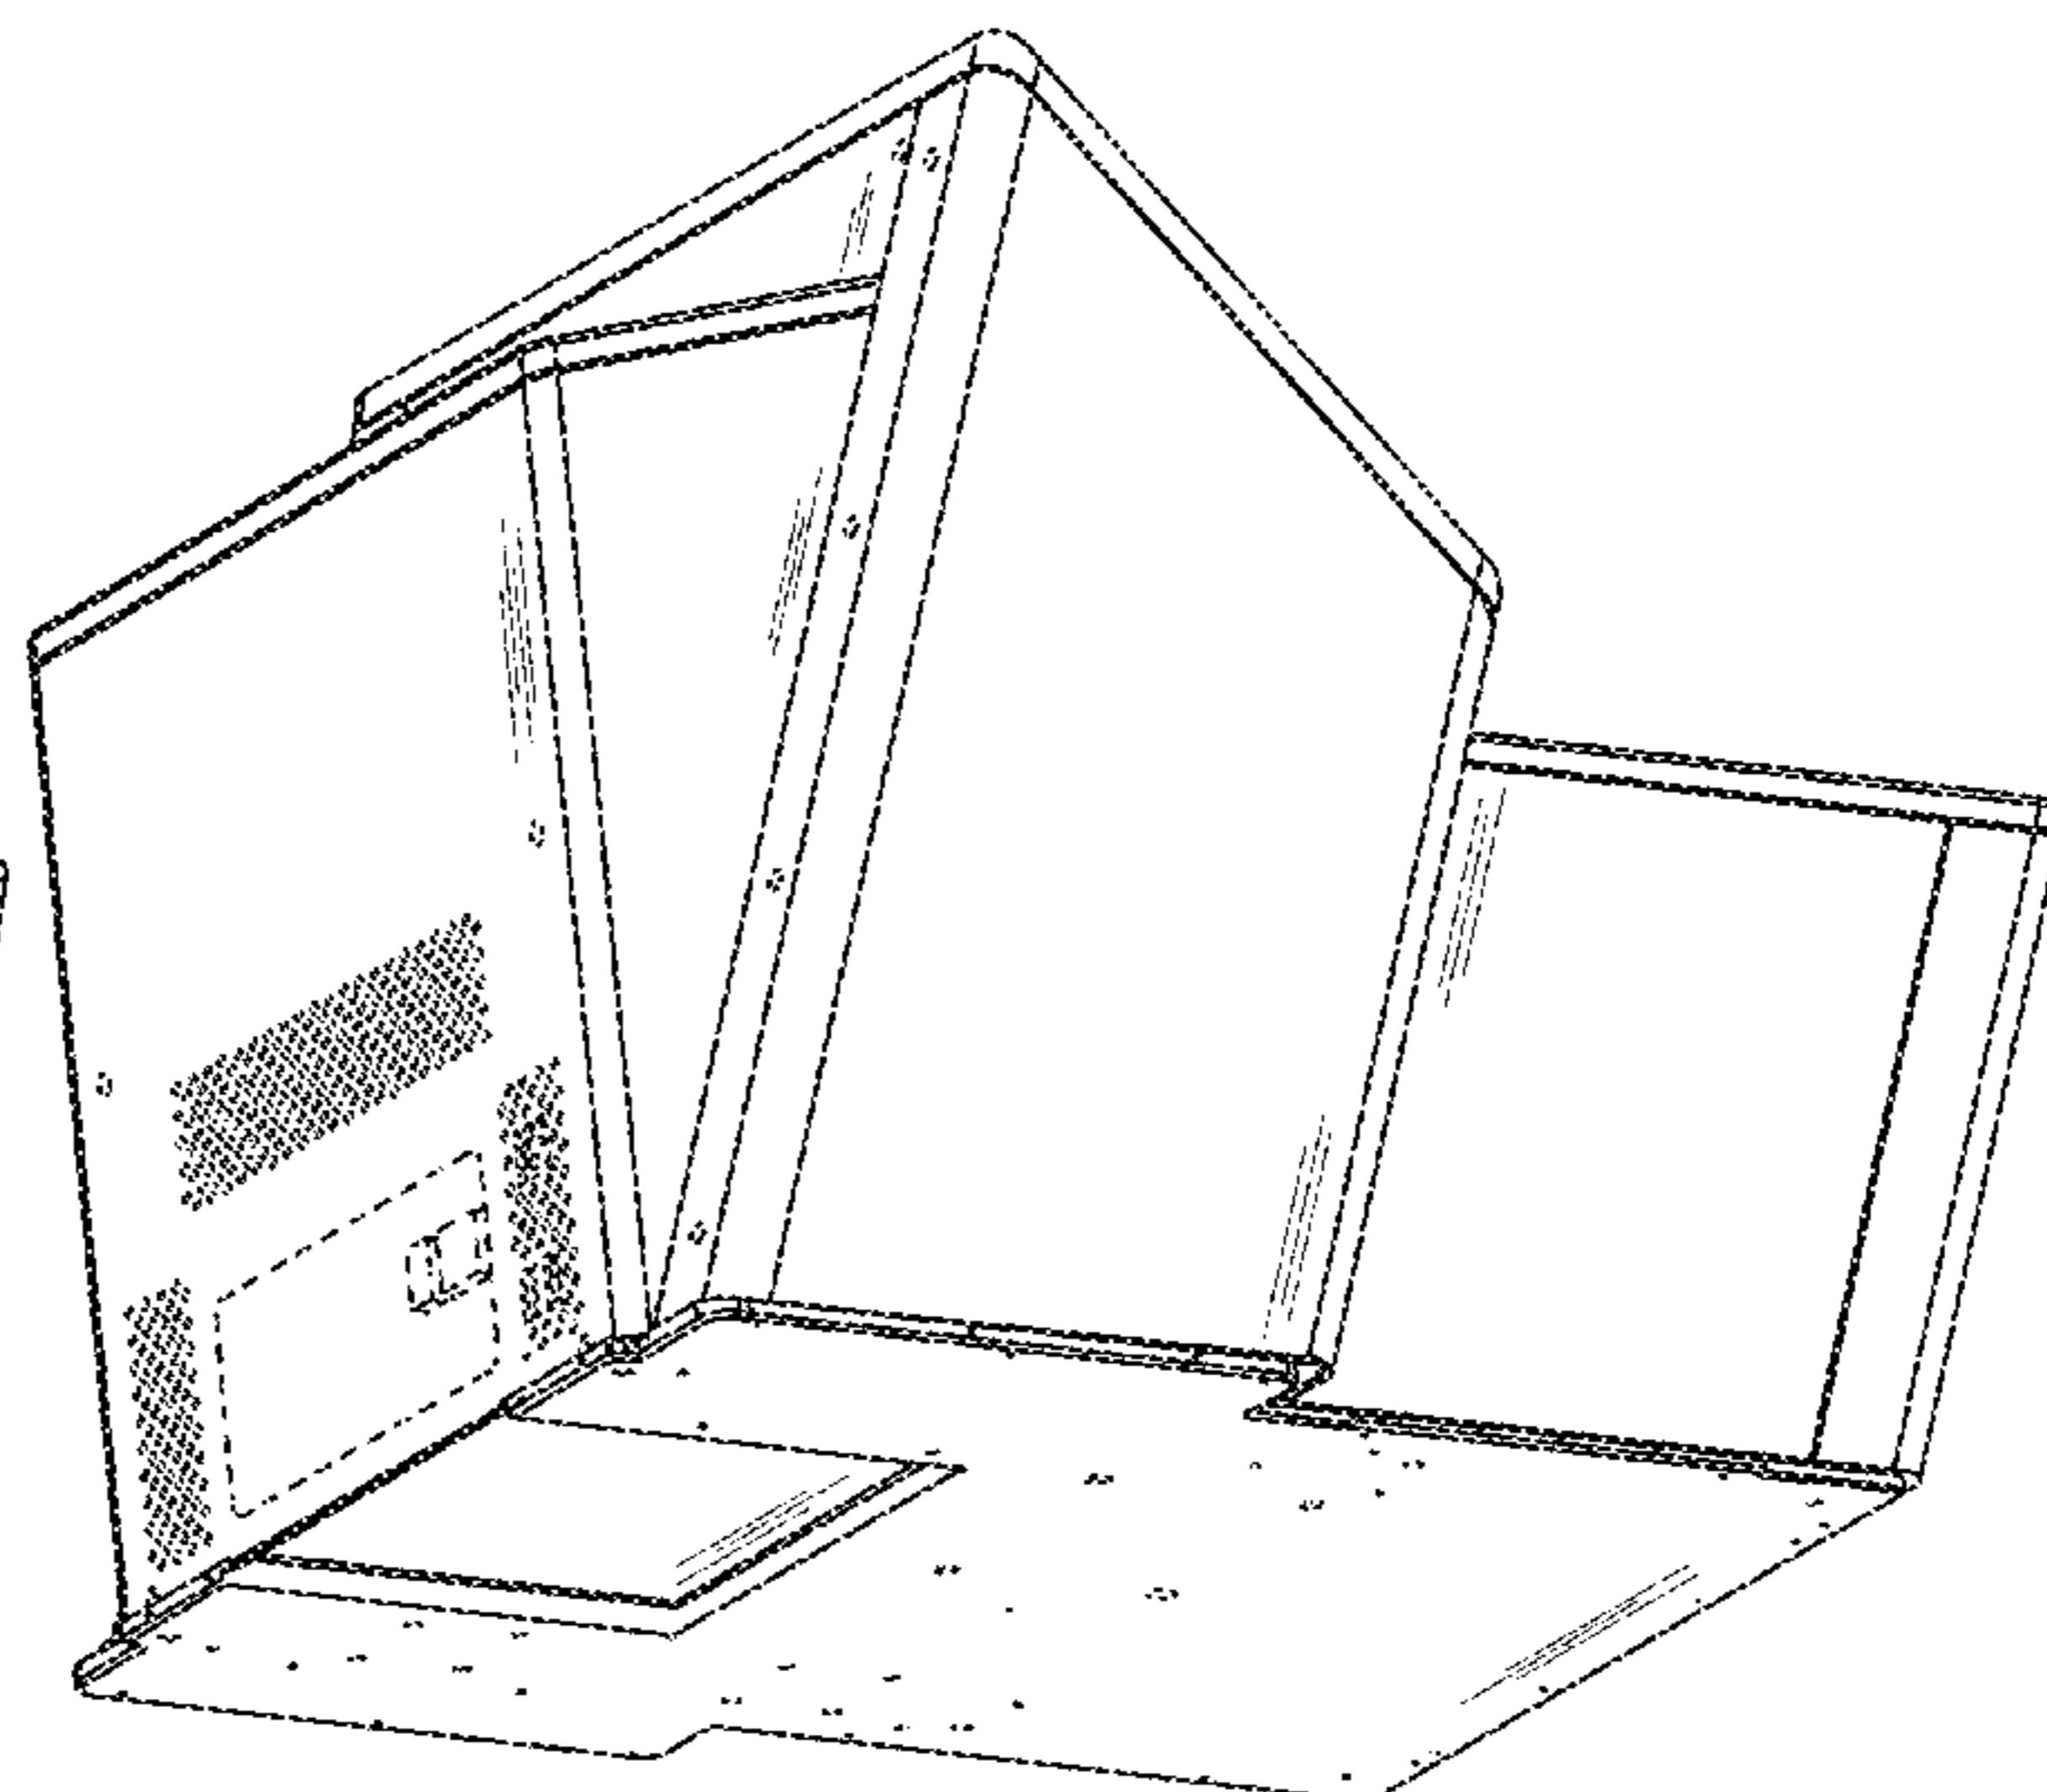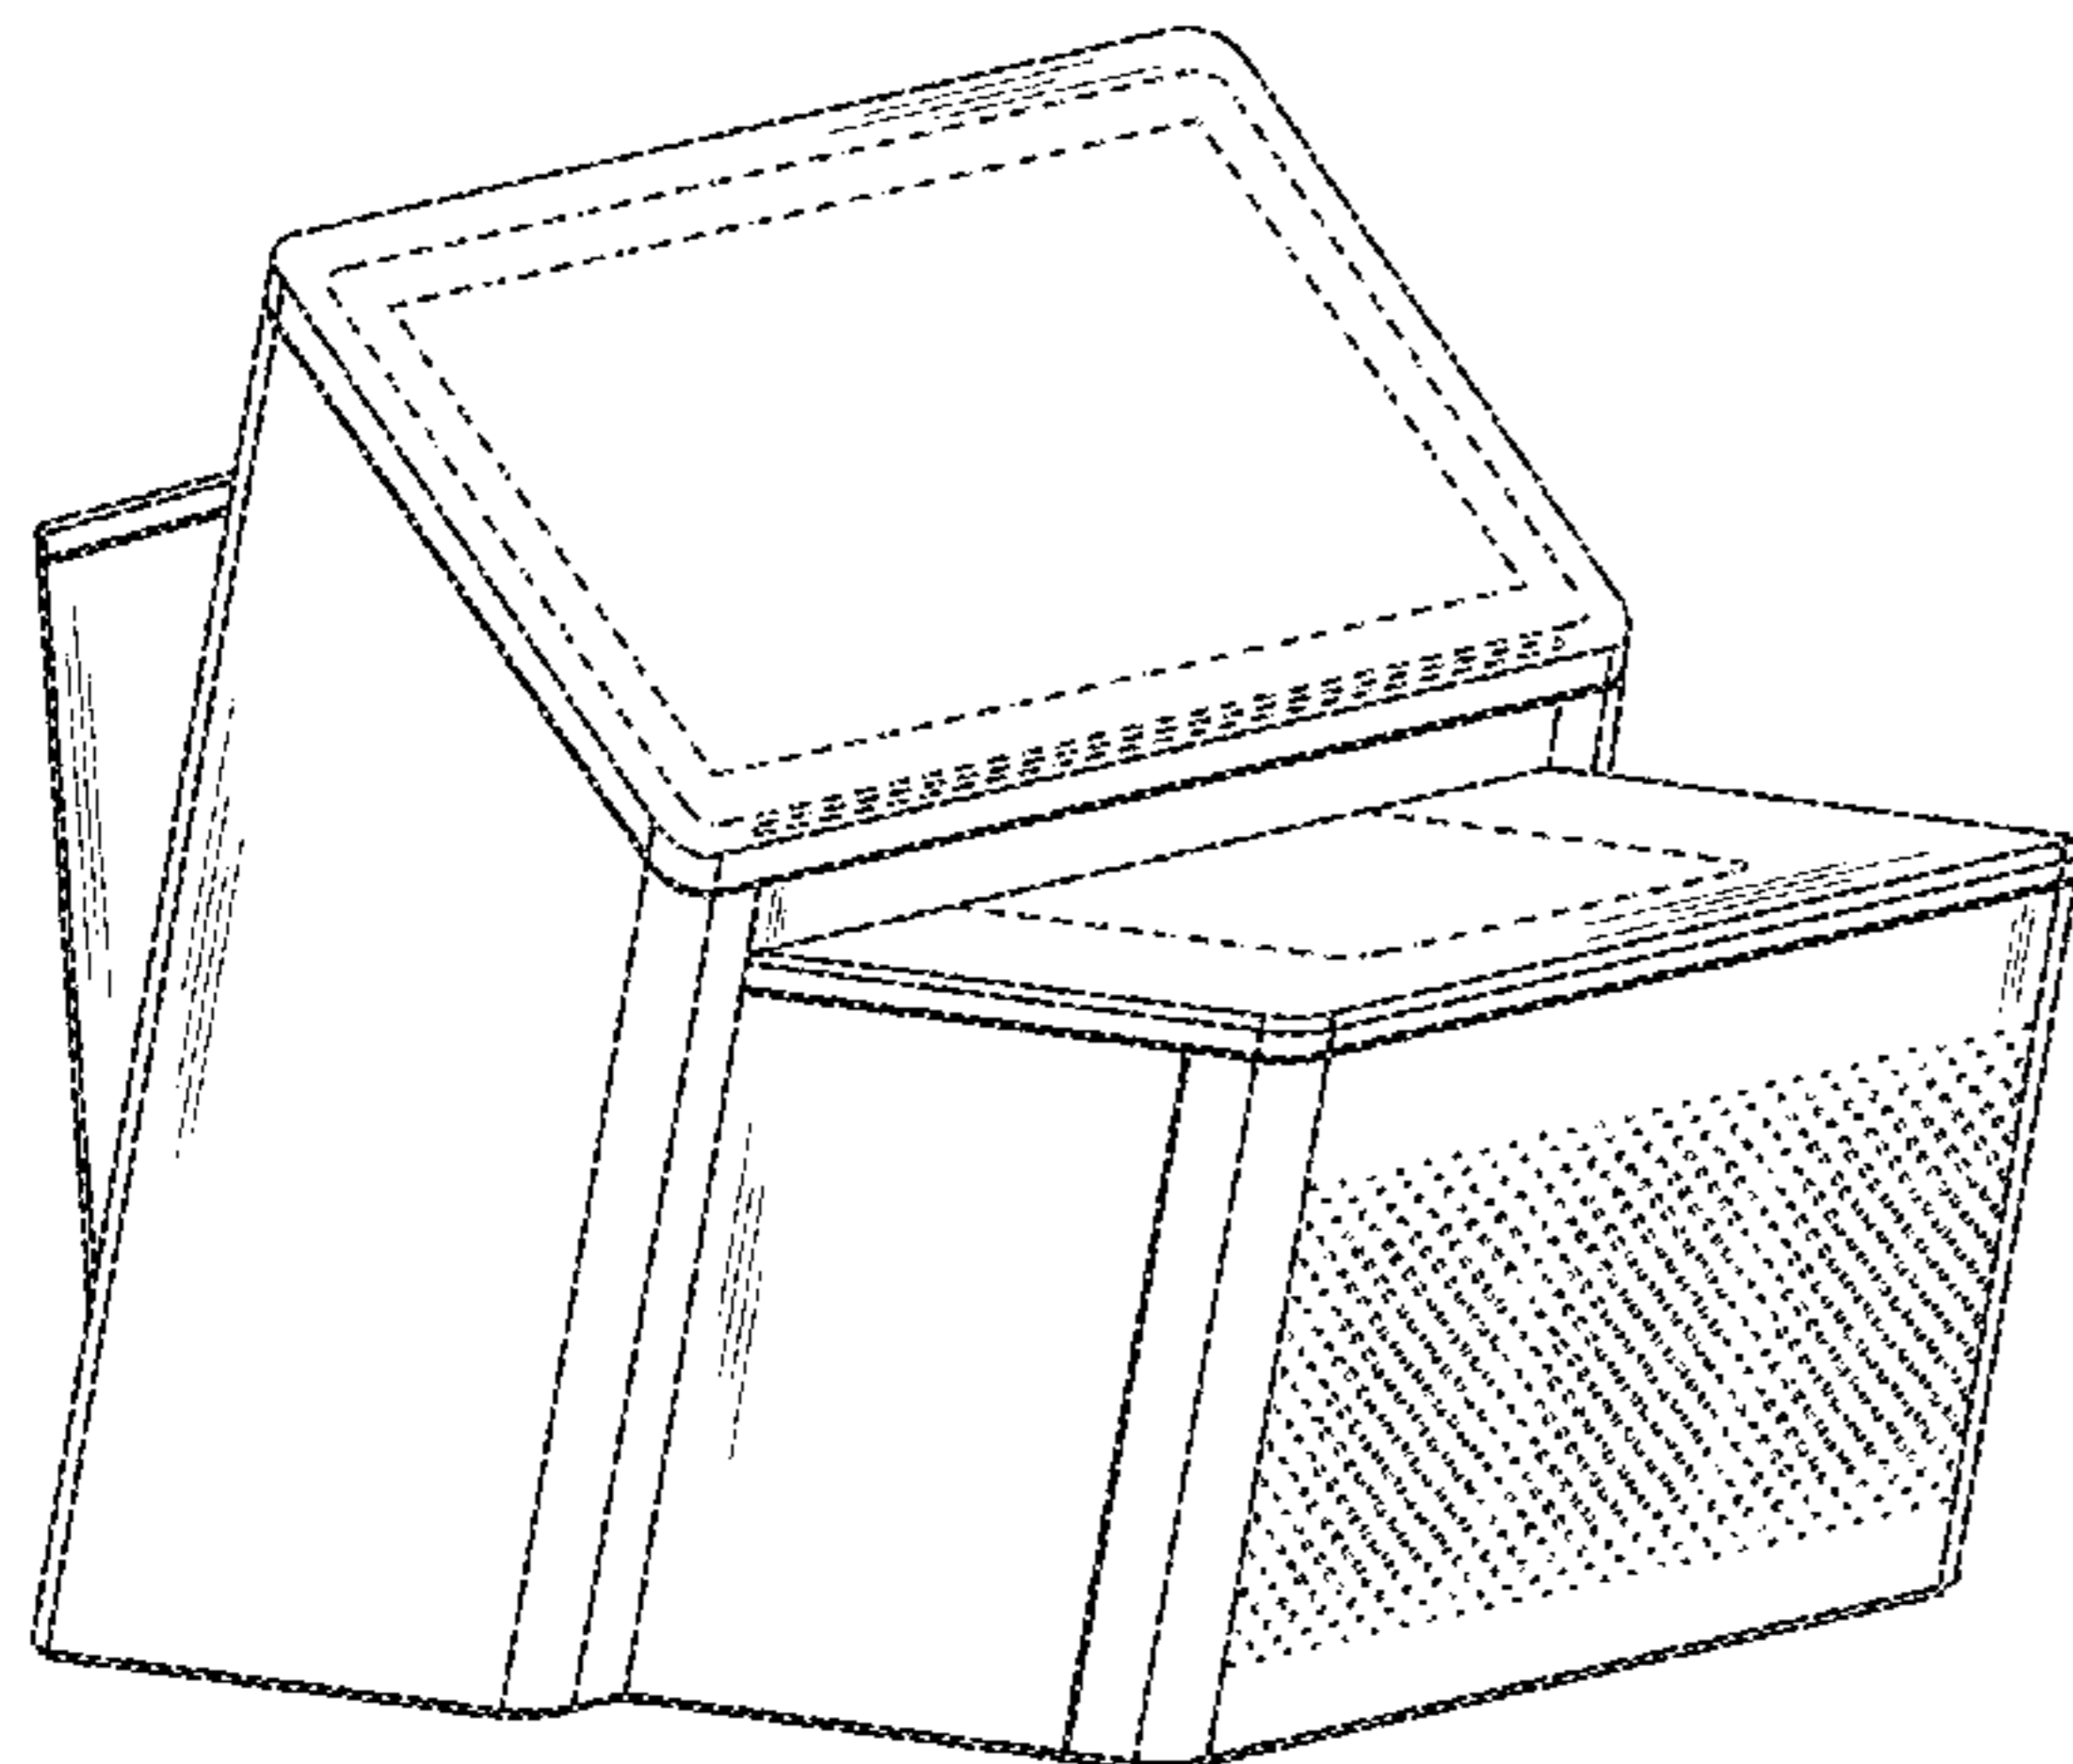

(58) **Field of Classification Search**

CPC .. G01N 21/00; G01N 21/01; G01N 2201/022;  
 G01N 2201/0221; G01N 2201/0222;  
 G01N 2201/0224; G01N 2201/0225;  
 G01N 2201/0227; G01N 25/08; G01N  
 25/085; G01N 25/10; G01N 25/12; G01N  
 25/14; G01N 25/142; G01N 25/145;  
 G01N 25/147; G01N 25/16; G01N 25/18;  
 G01N 25/20; G01N 25/22; G01N 30/06;  
 G01N 35/026; G01N 27/62; G01N 35/08;  
 G01N 30/72; G01N 35/0092; G01N  
 30/88; G01N 33/53; G01N 33/50; G01N  
 35/025; G01N 35/00603; G01N  
 35/00584; H01J 49/0413

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D854,703 S \* 7/2019 Juhlin ..... D24/216  
 D857,903 S \* 8/2019 Esfandiari ..... D24/185  
 D888,267 S \* 6/2020 Salomon ..... D24/216  
 D888,985 S \* 6/2020 Hsieh ..... D24/232  
 D909,605 S \* 2/2021 Mathers ..... D24/232  
 D911,859 S \* 3/2021 Morgan, III ..... D10/81  
 D914,905 S \* 3/2021 Wade ..... D24/216  
 D932,929 S \* 10/2021 Stone ..... D10/81  
 D937,694 S \* 12/2021 VanDyke ..... D10/81

D944,105 S \* 2/2022 Barton ..... D24/216  
 D946,431 S \* 3/2022 Blake ..... D24/232  
 D953,563 S \* 5/2022 Matakai ..... D24/186  
 D954,574 S \* 6/2022 Blake ..... D24/232  
 D963,499 S \* 9/2022 Blake ..... D24/232  
 D965,171 S \* 9/2022 Ui ..... D24/216  
 D965,816 S \* 10/2022 Luther ..... D24/233  
 2015/0130463 A1 \* 5/2015 Wellman ..... G01R 33/30  
 324/321  
 2018/0149600 A1 \* 5/2018 Farrell ..... G01N 33/48785  
 2021/0151313 A1 \* 5/2021 Ueda ..... H01J 49/4225  
 2021/0384024 A1 \* 12/2021 Carney ..... H01J 49/025

FOREIGN PATENT DOCUMENTS

GB 6036377 \* 5/2018  
 GB 6036378 \* 5/2018  
 JP D1094655 \* 3/2000  
 JP D1096237 \* 11/2000  
 KR 301085998.0000 \* 3/2020

OTHER PUBLICATIONS

7 Top Mass Spectrometry Innovations from ASMS 2019, SelectScience  
 editors, Date first available Jun. 11, 2019, [online]retrieved Nov. 10,  
 2021, available from <https://www.selectscience.net/top-lists/7-top-mass-spectrometry-innovations-from-asms-2019/?artID=49069> (Year:  
 2019).\*

\* cited by examiner

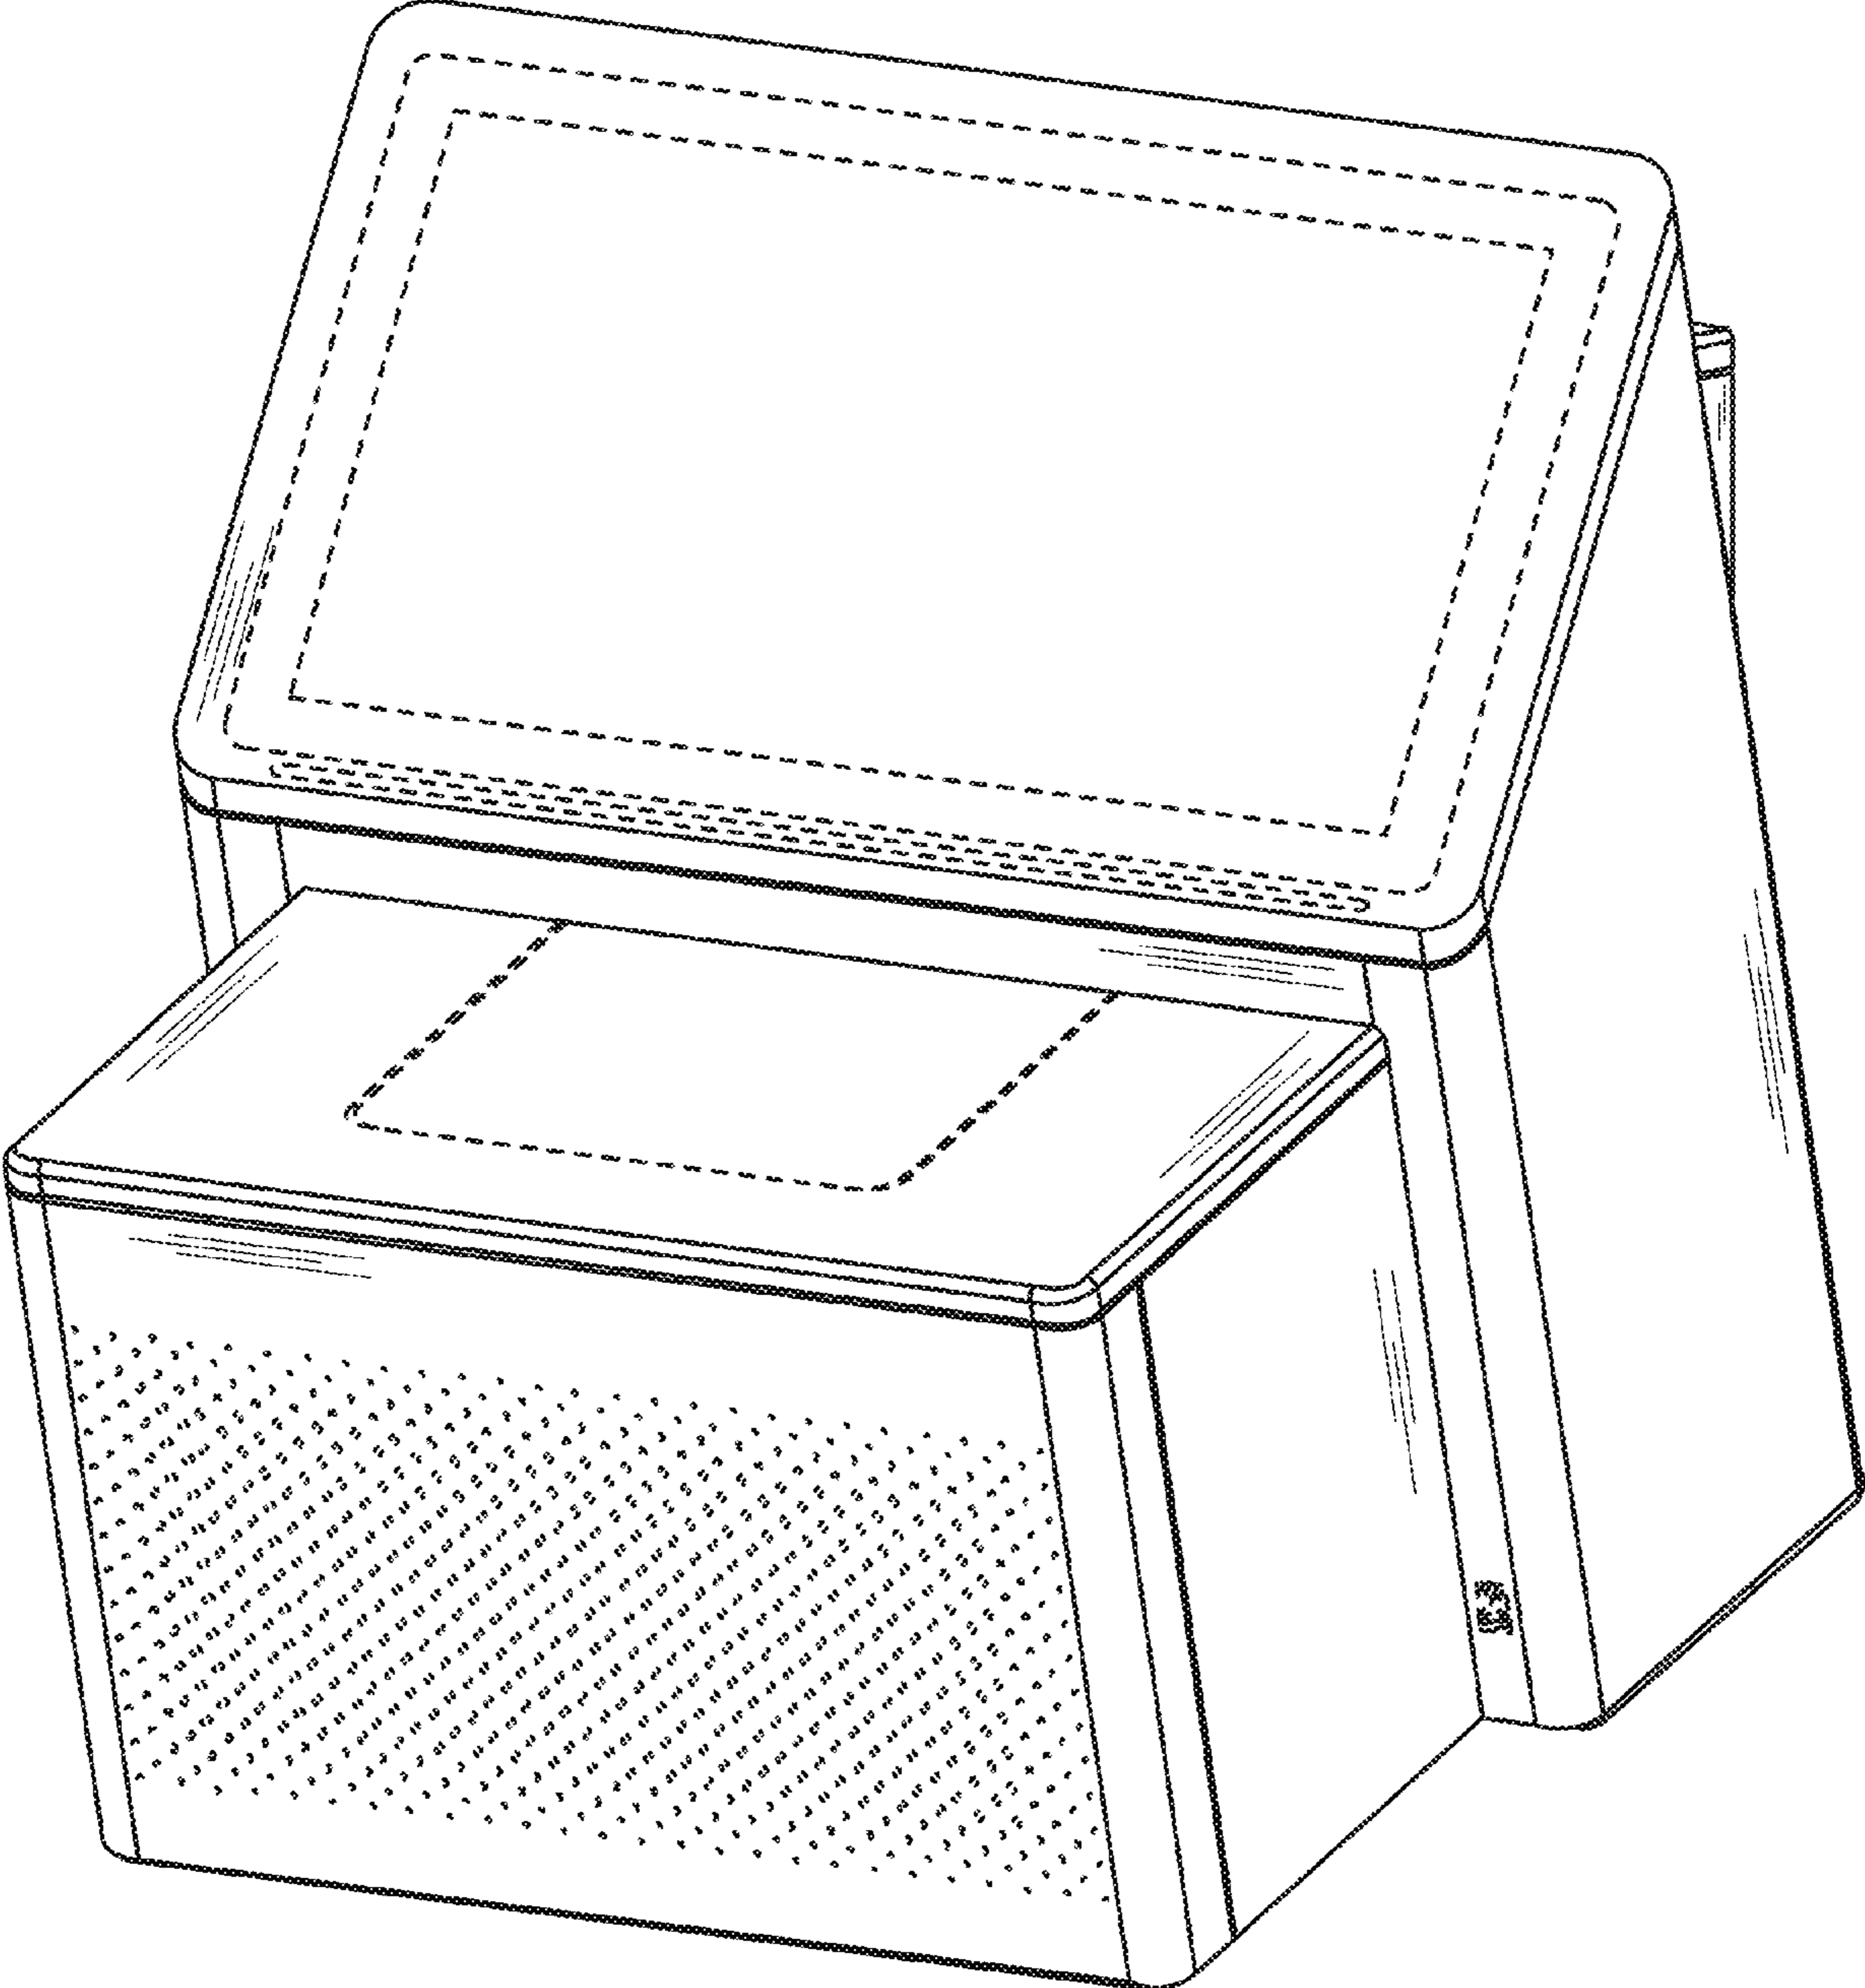


FIG. 1

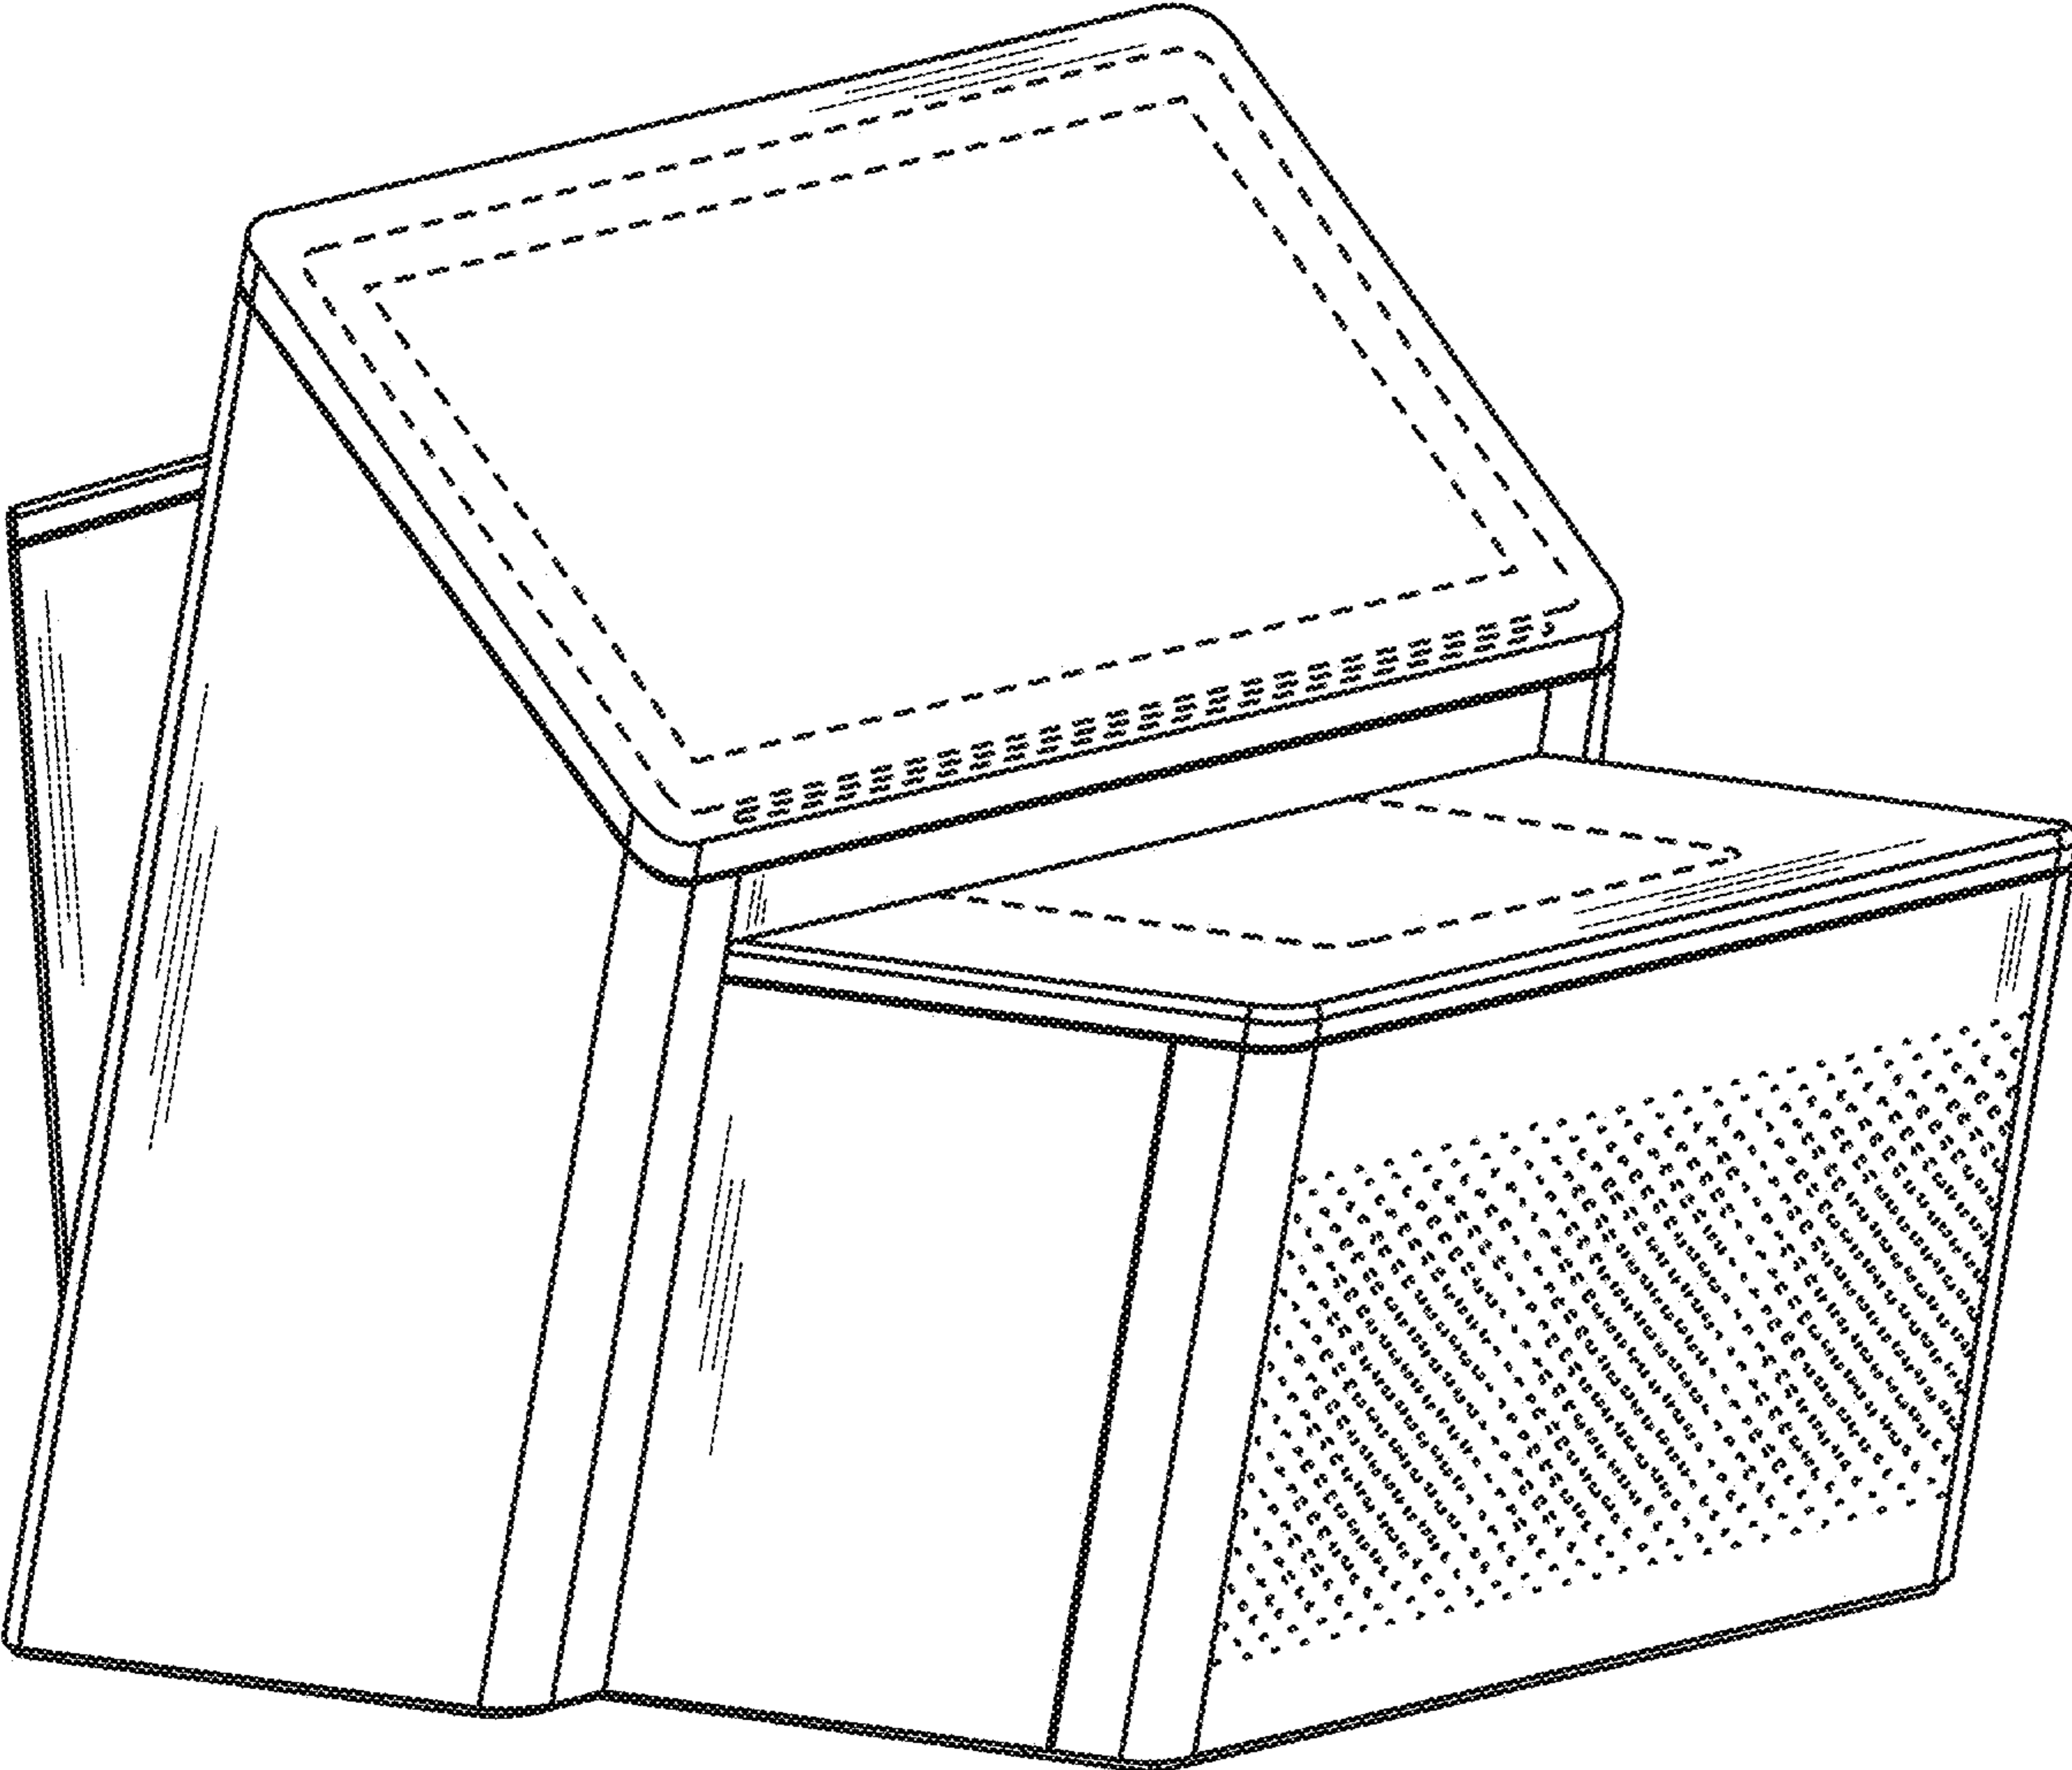


FIG. 2

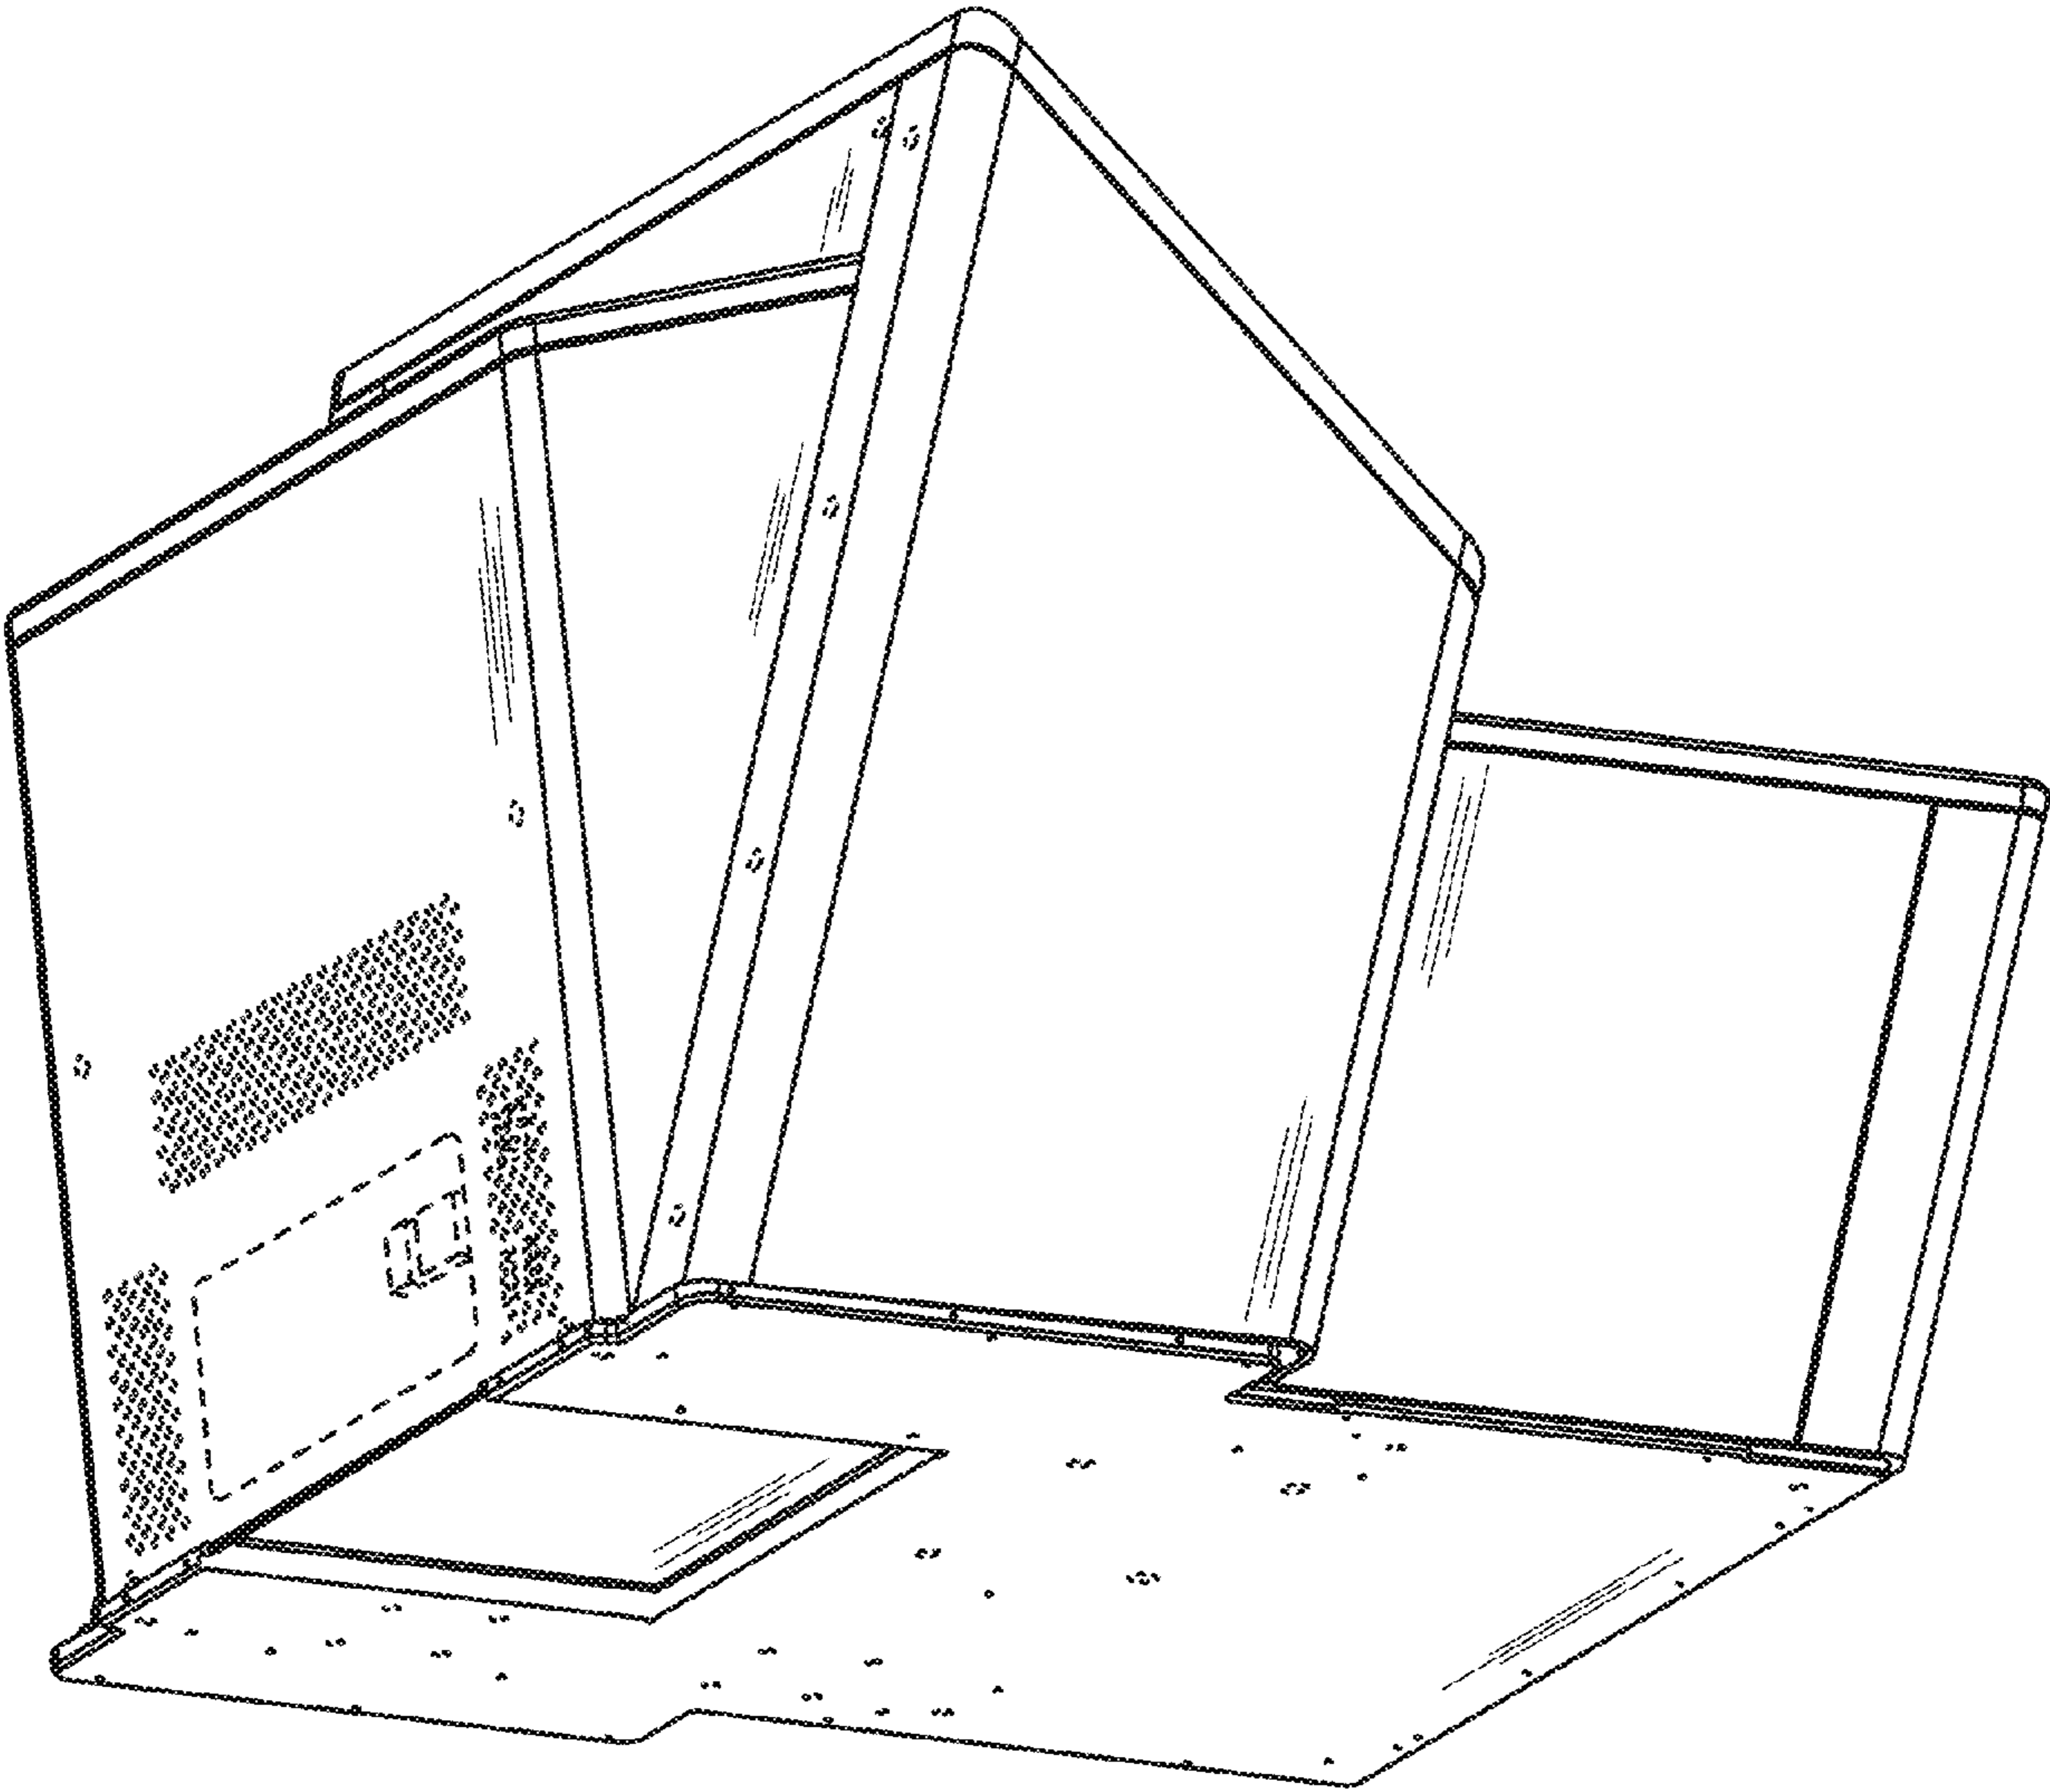


FIG. 3

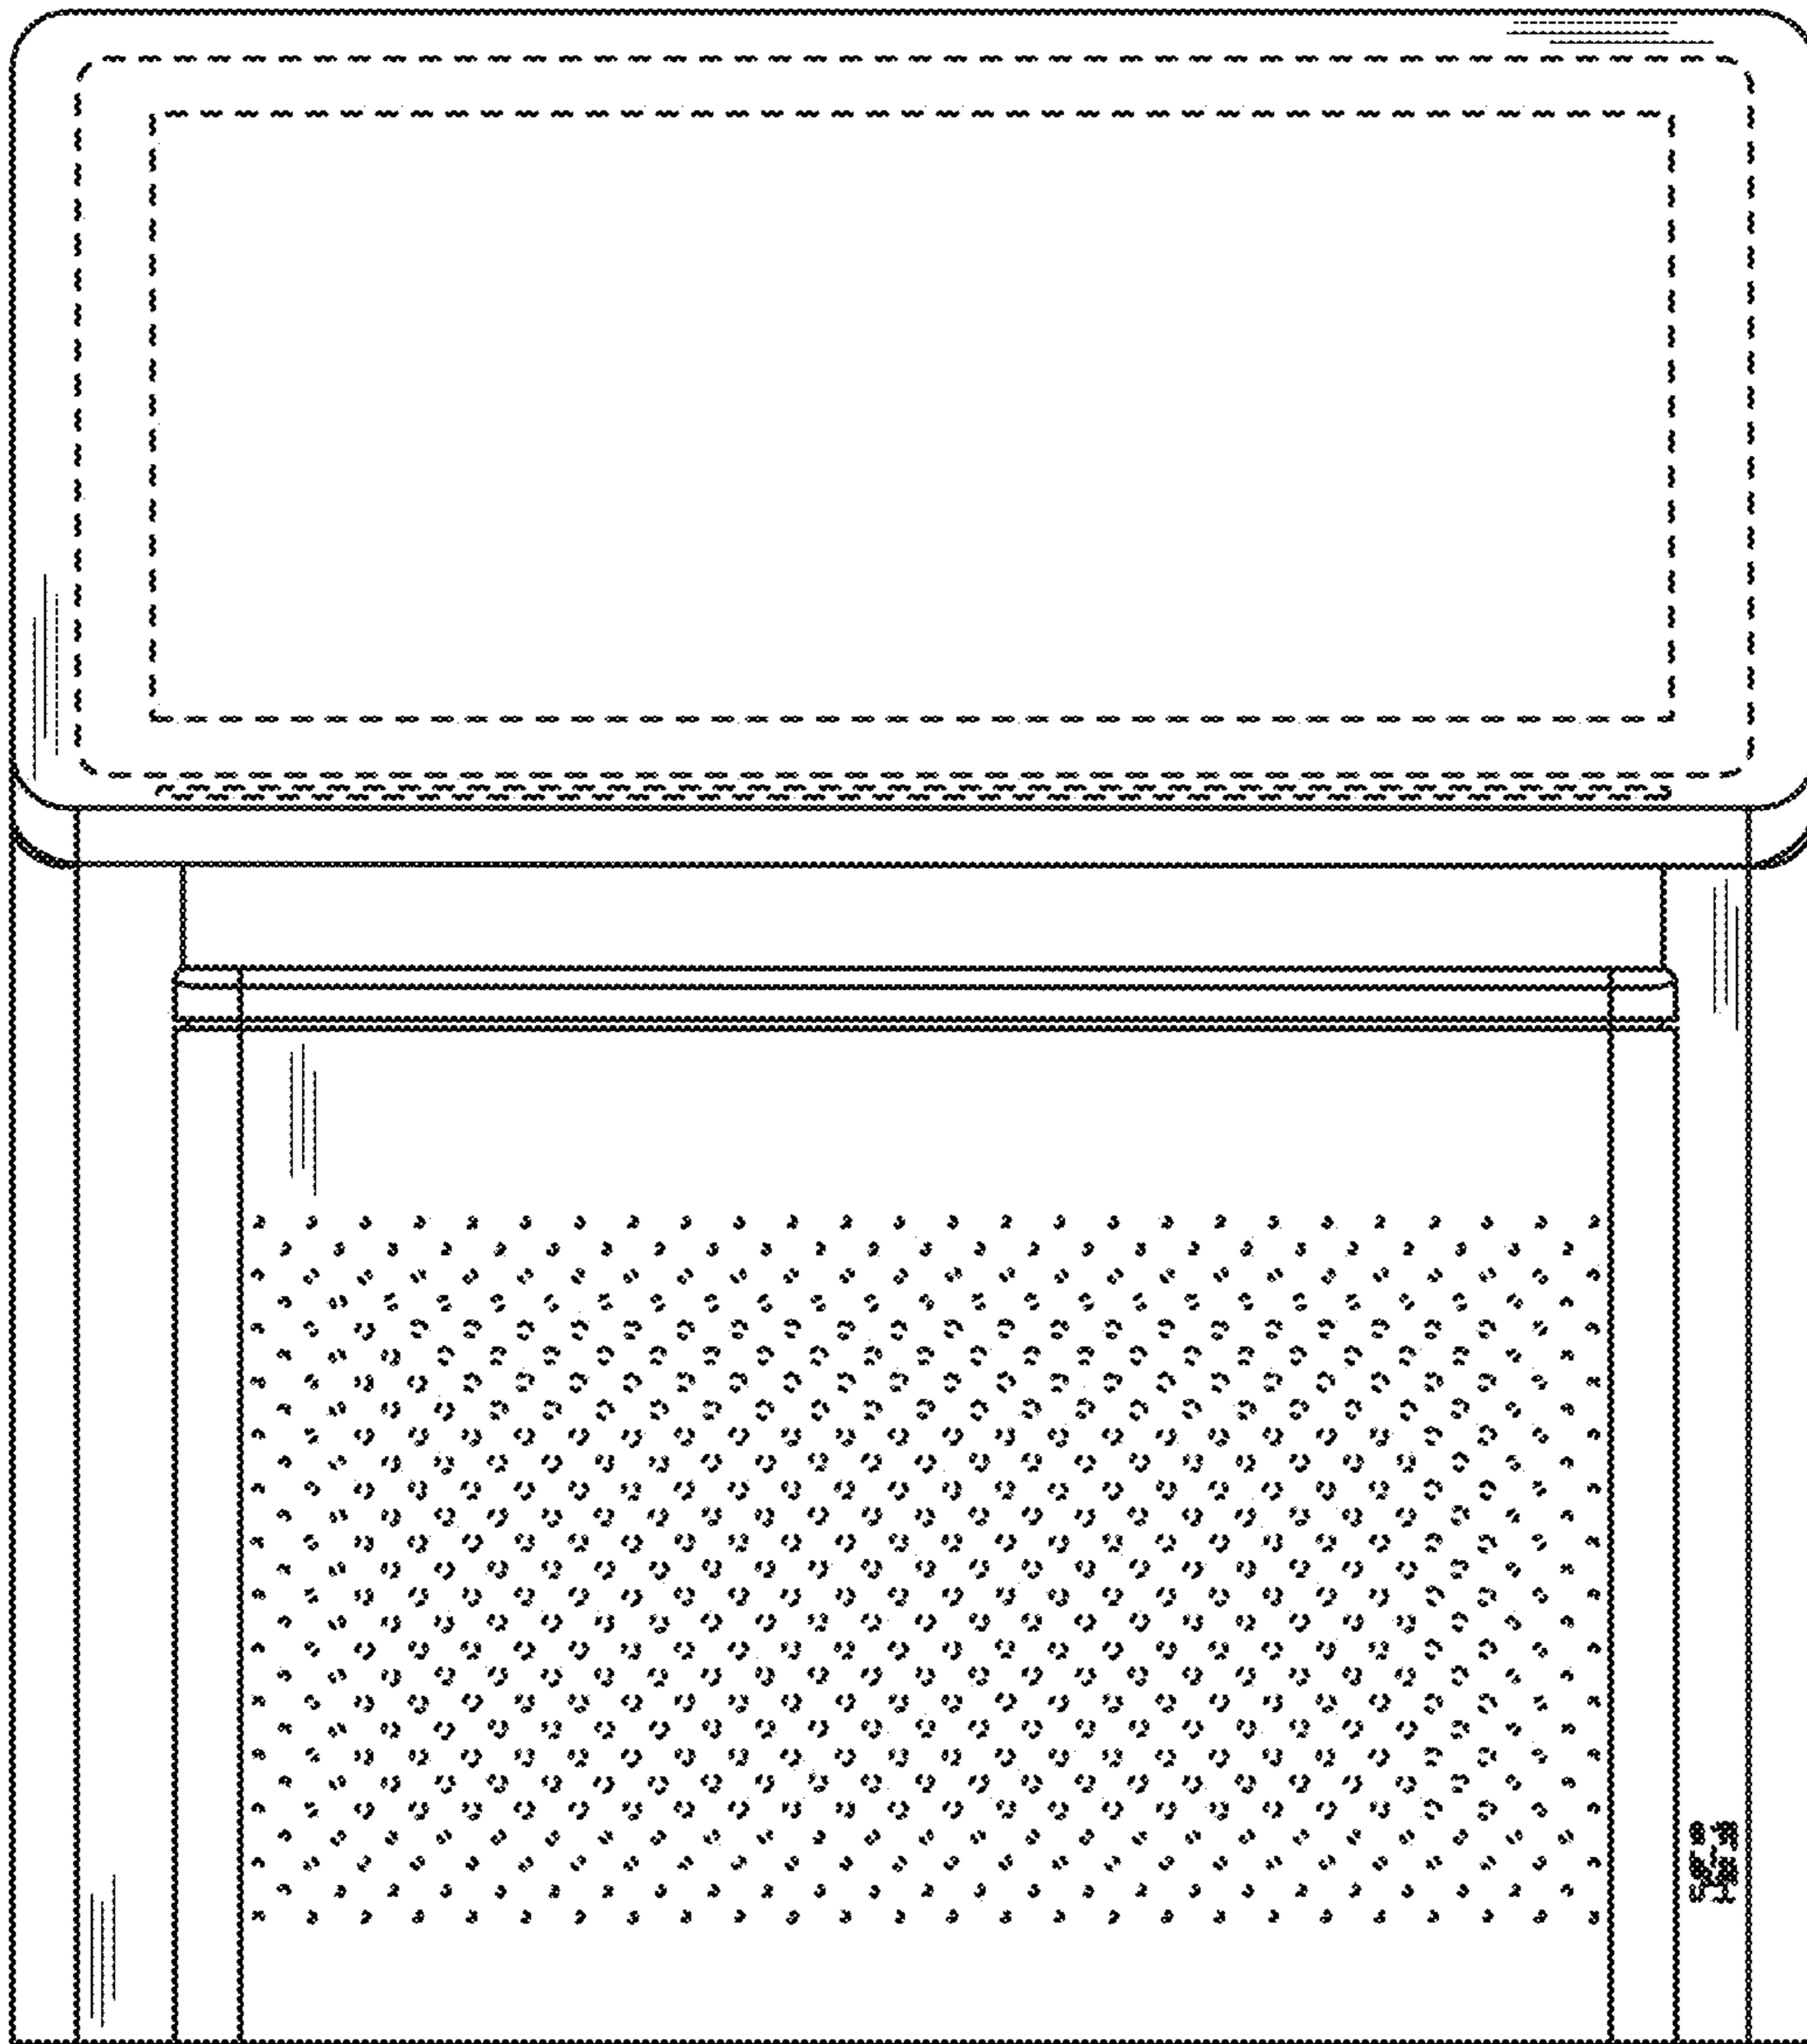


FIG. 4

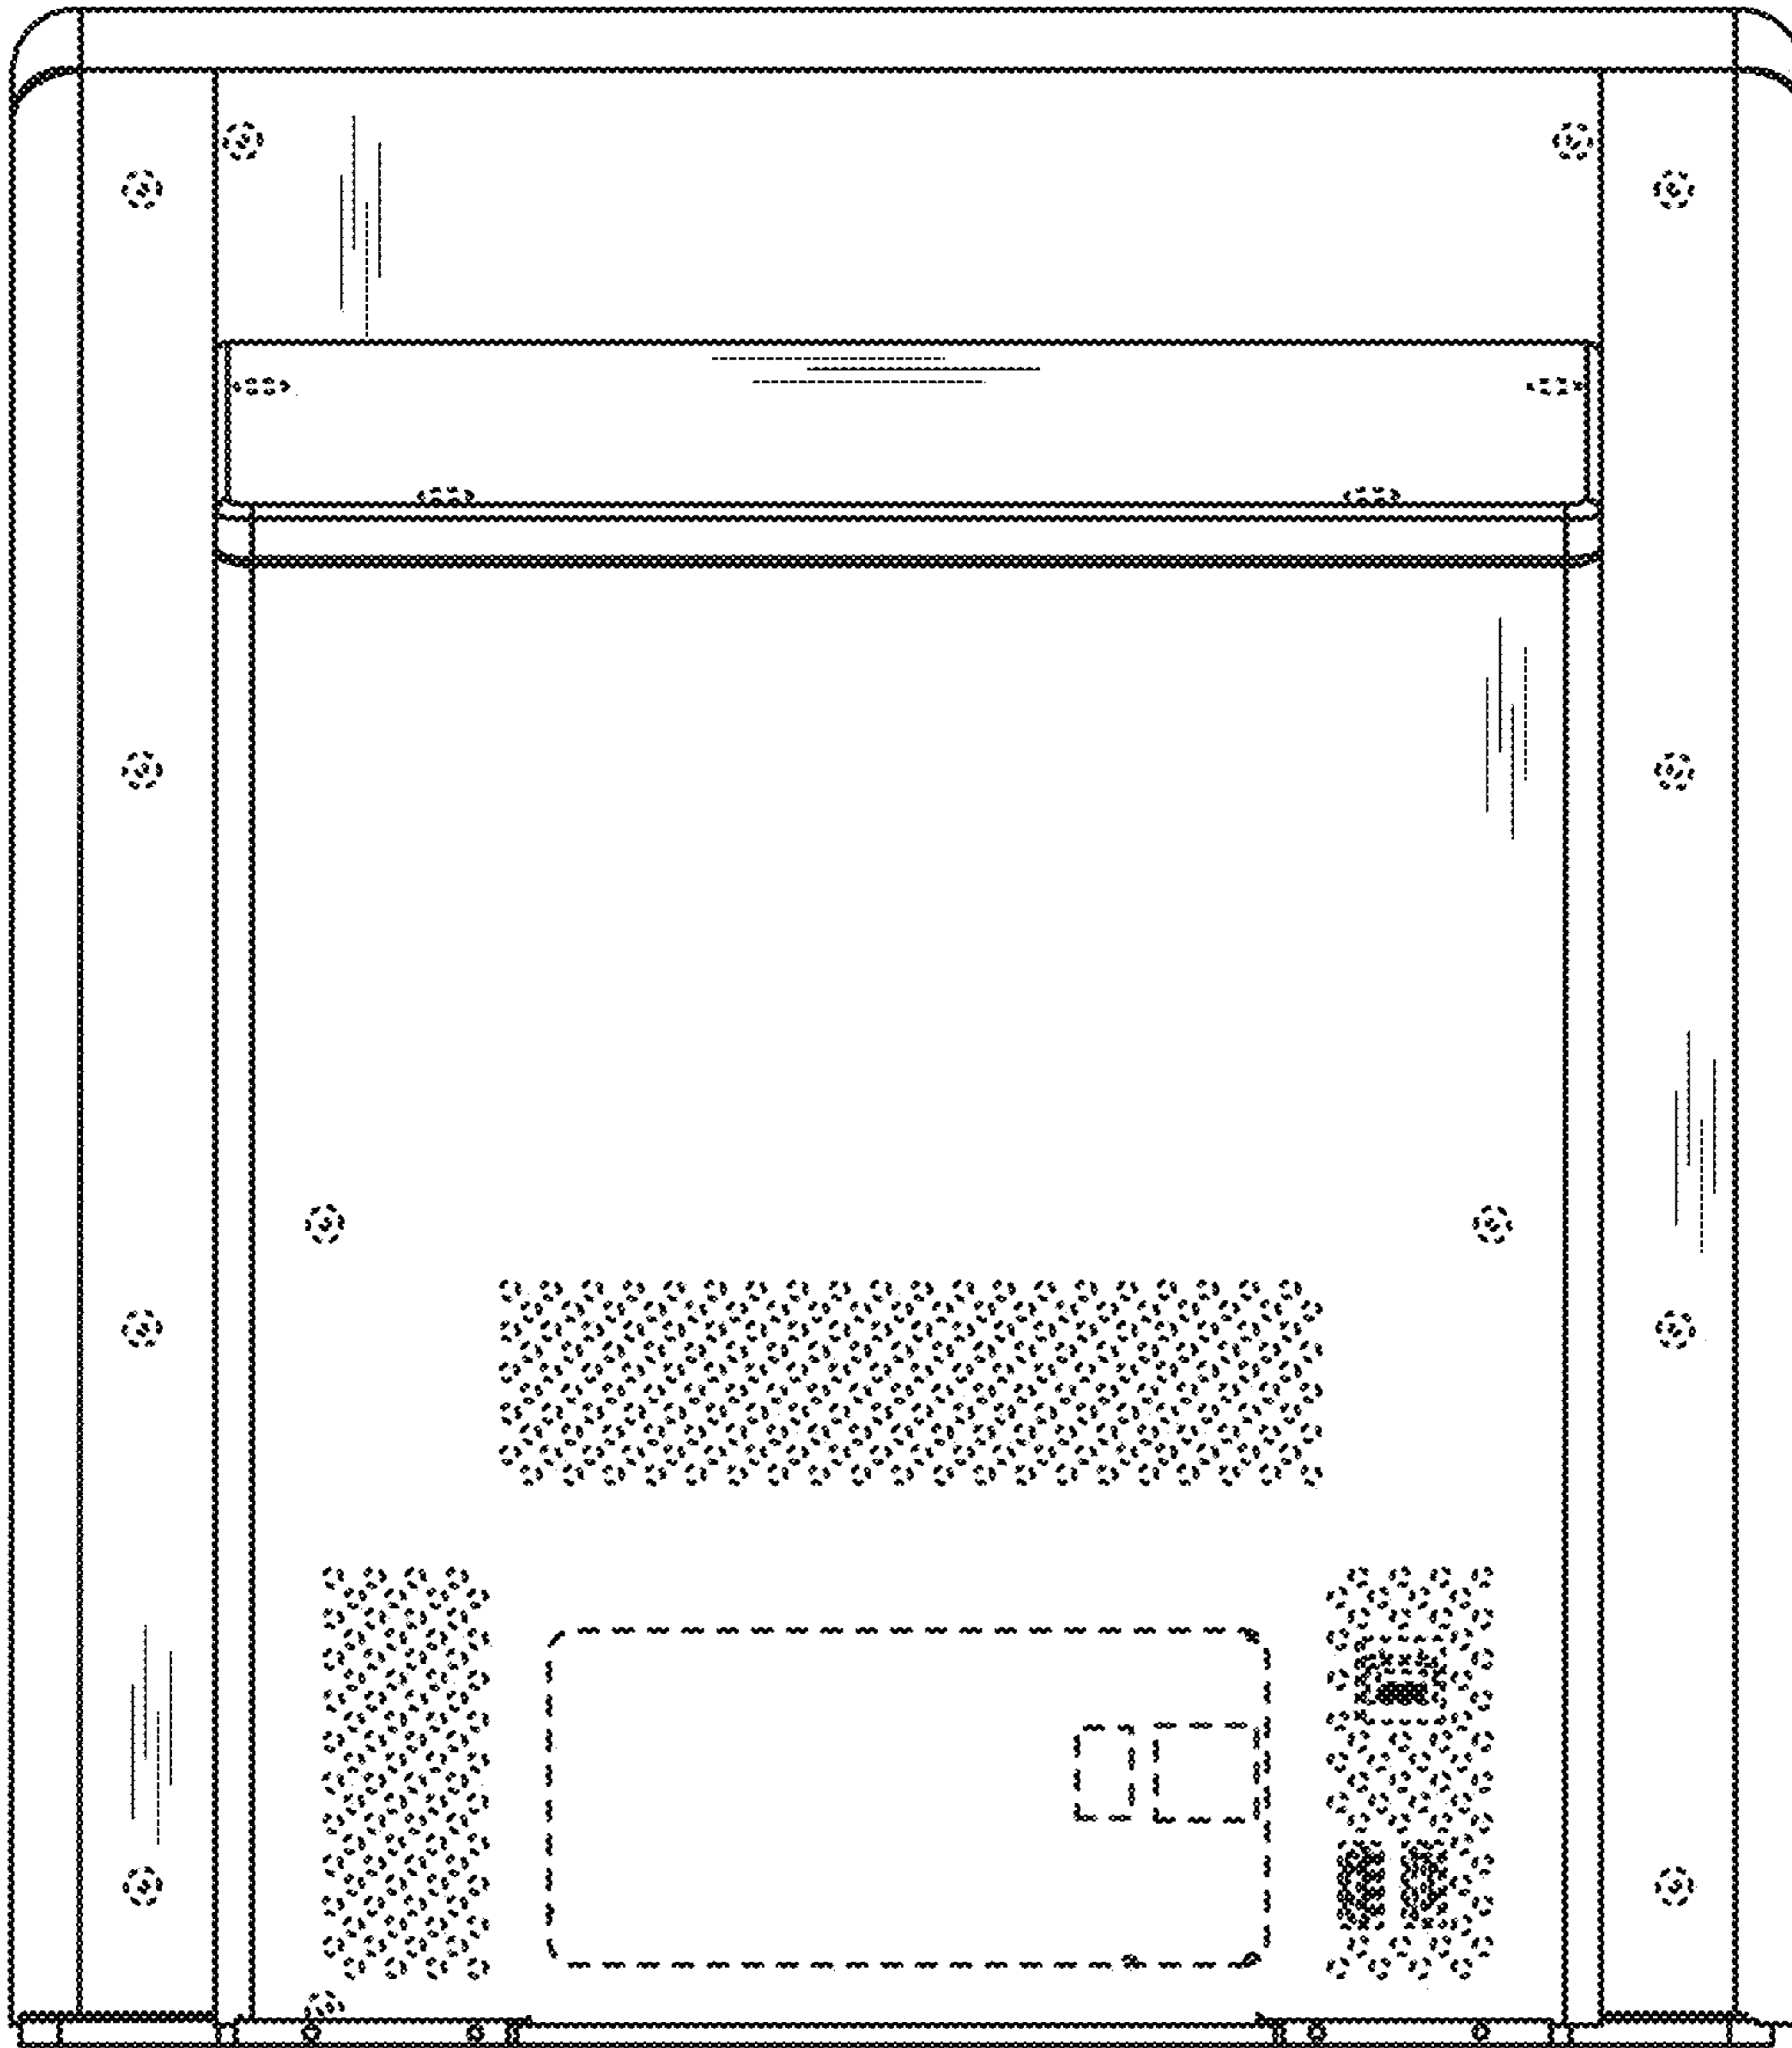


FIG. 5

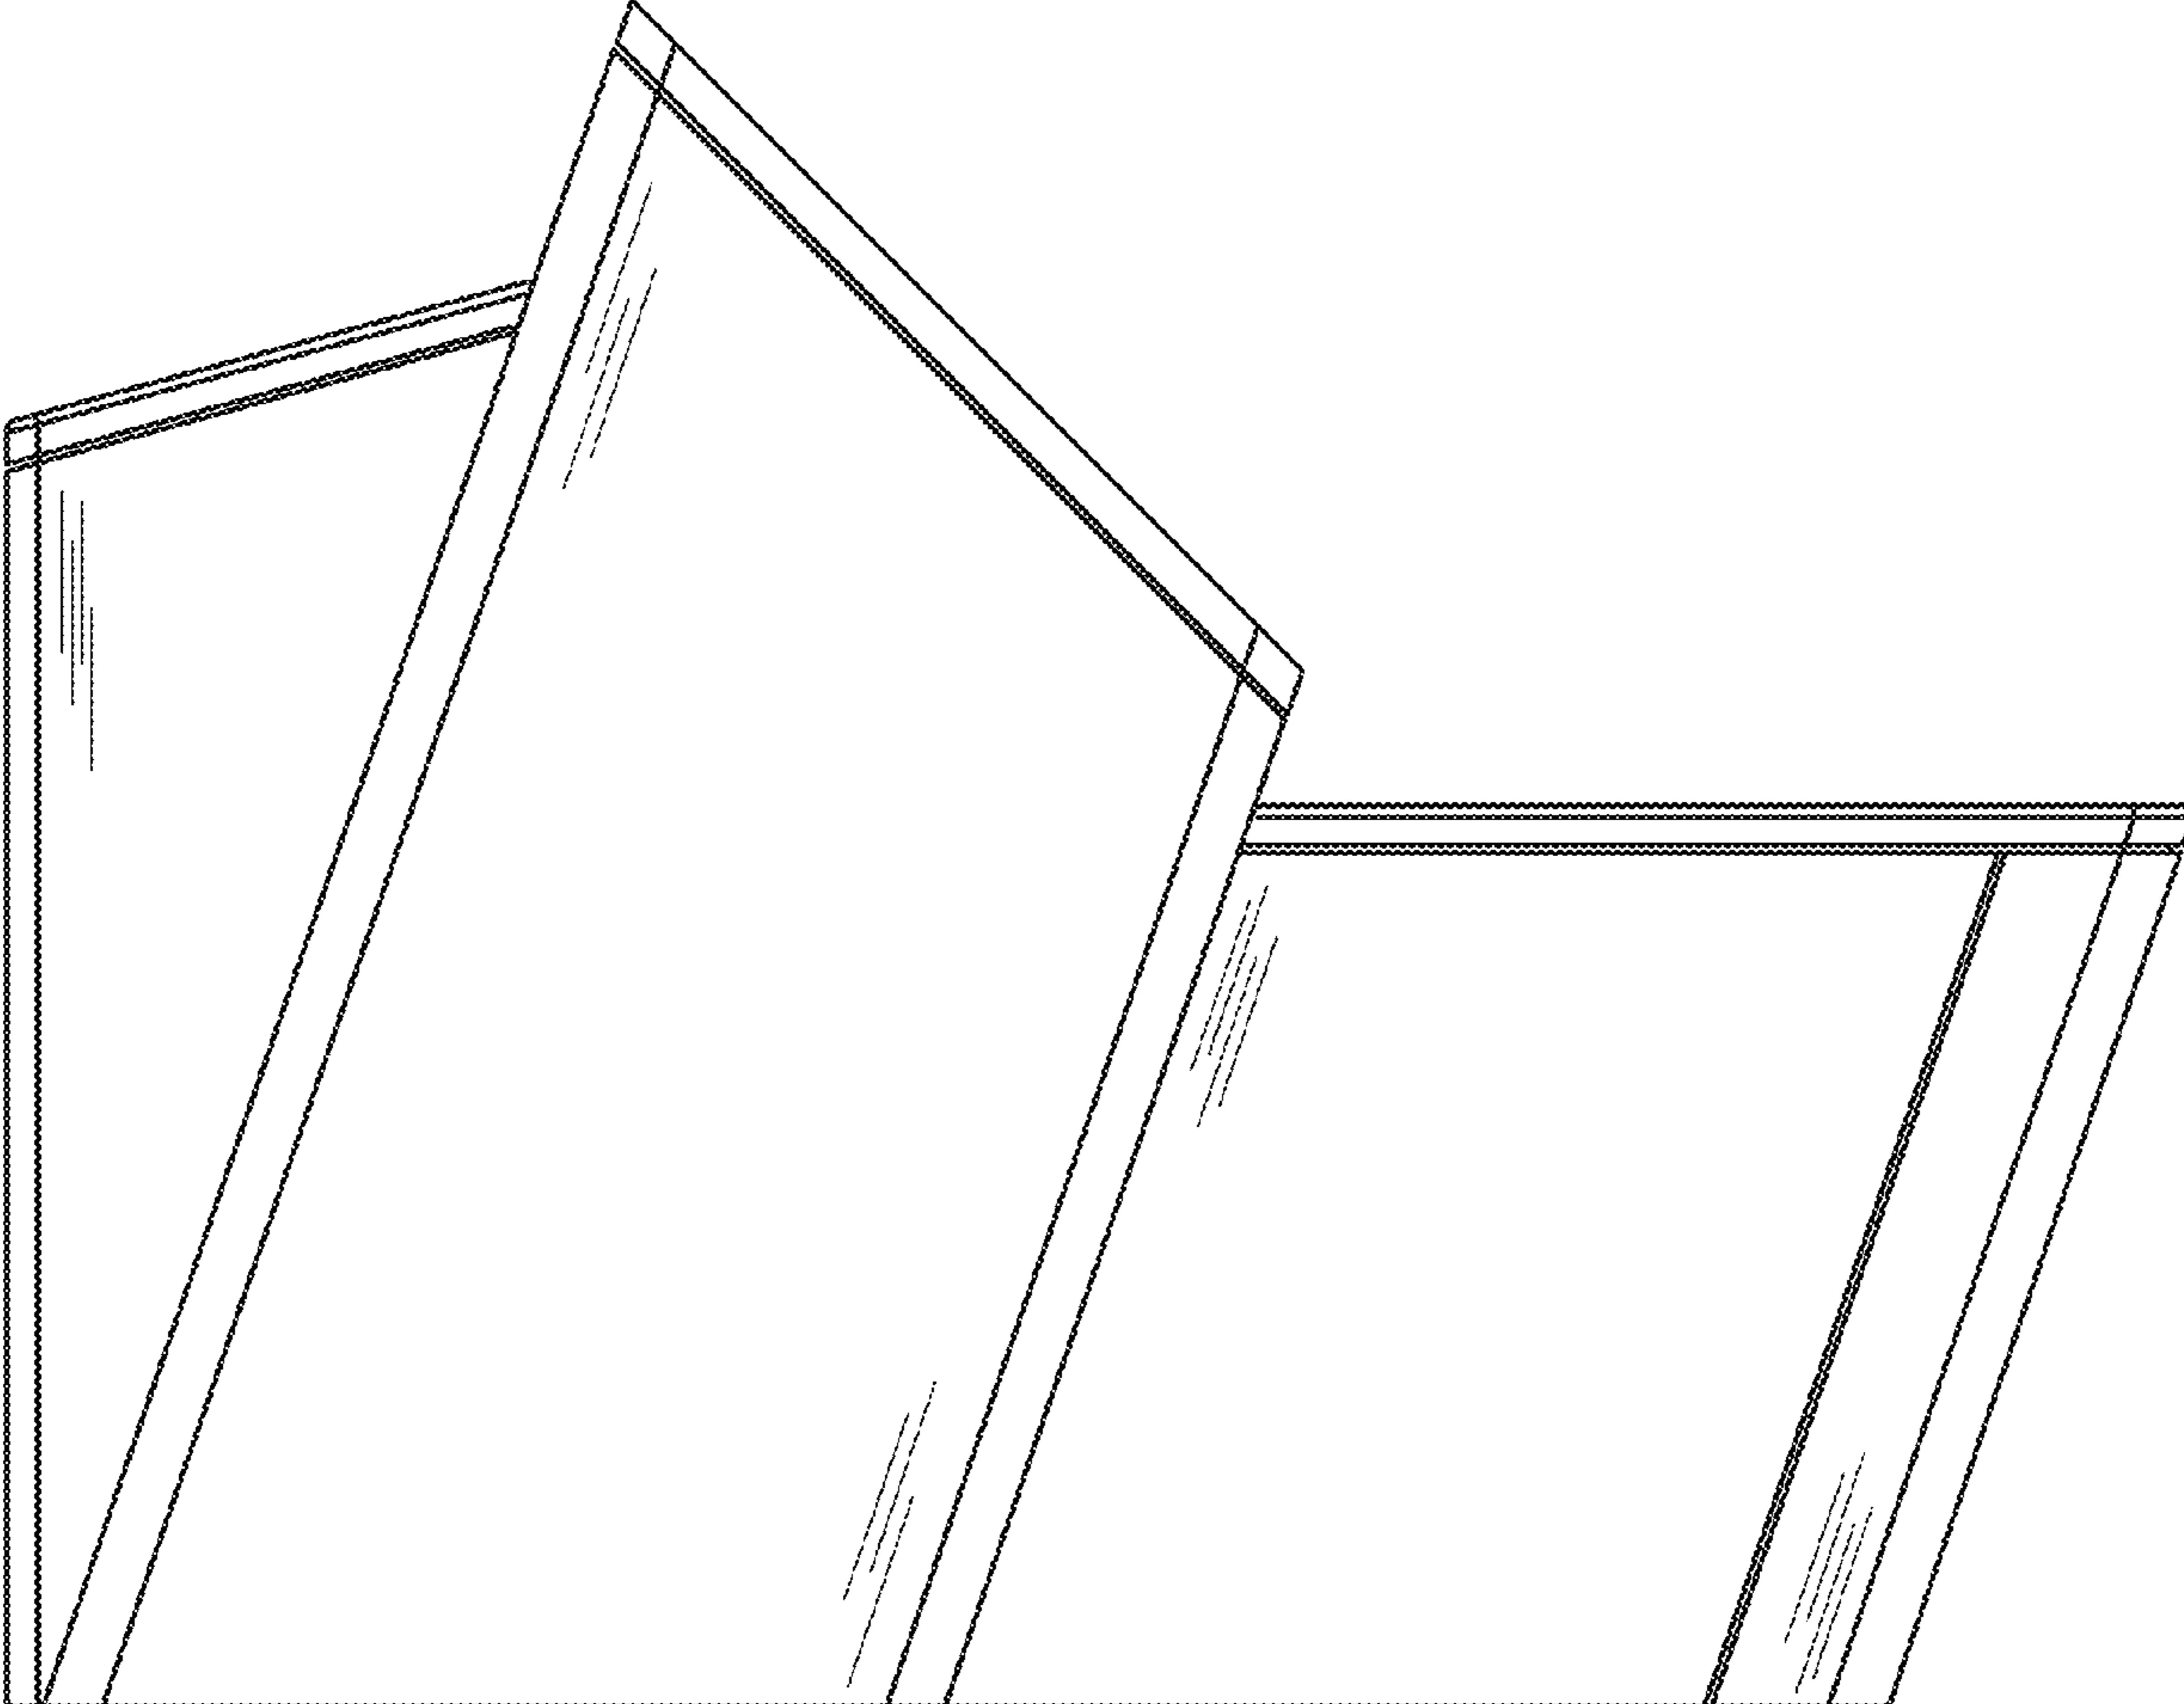


FIG. 6



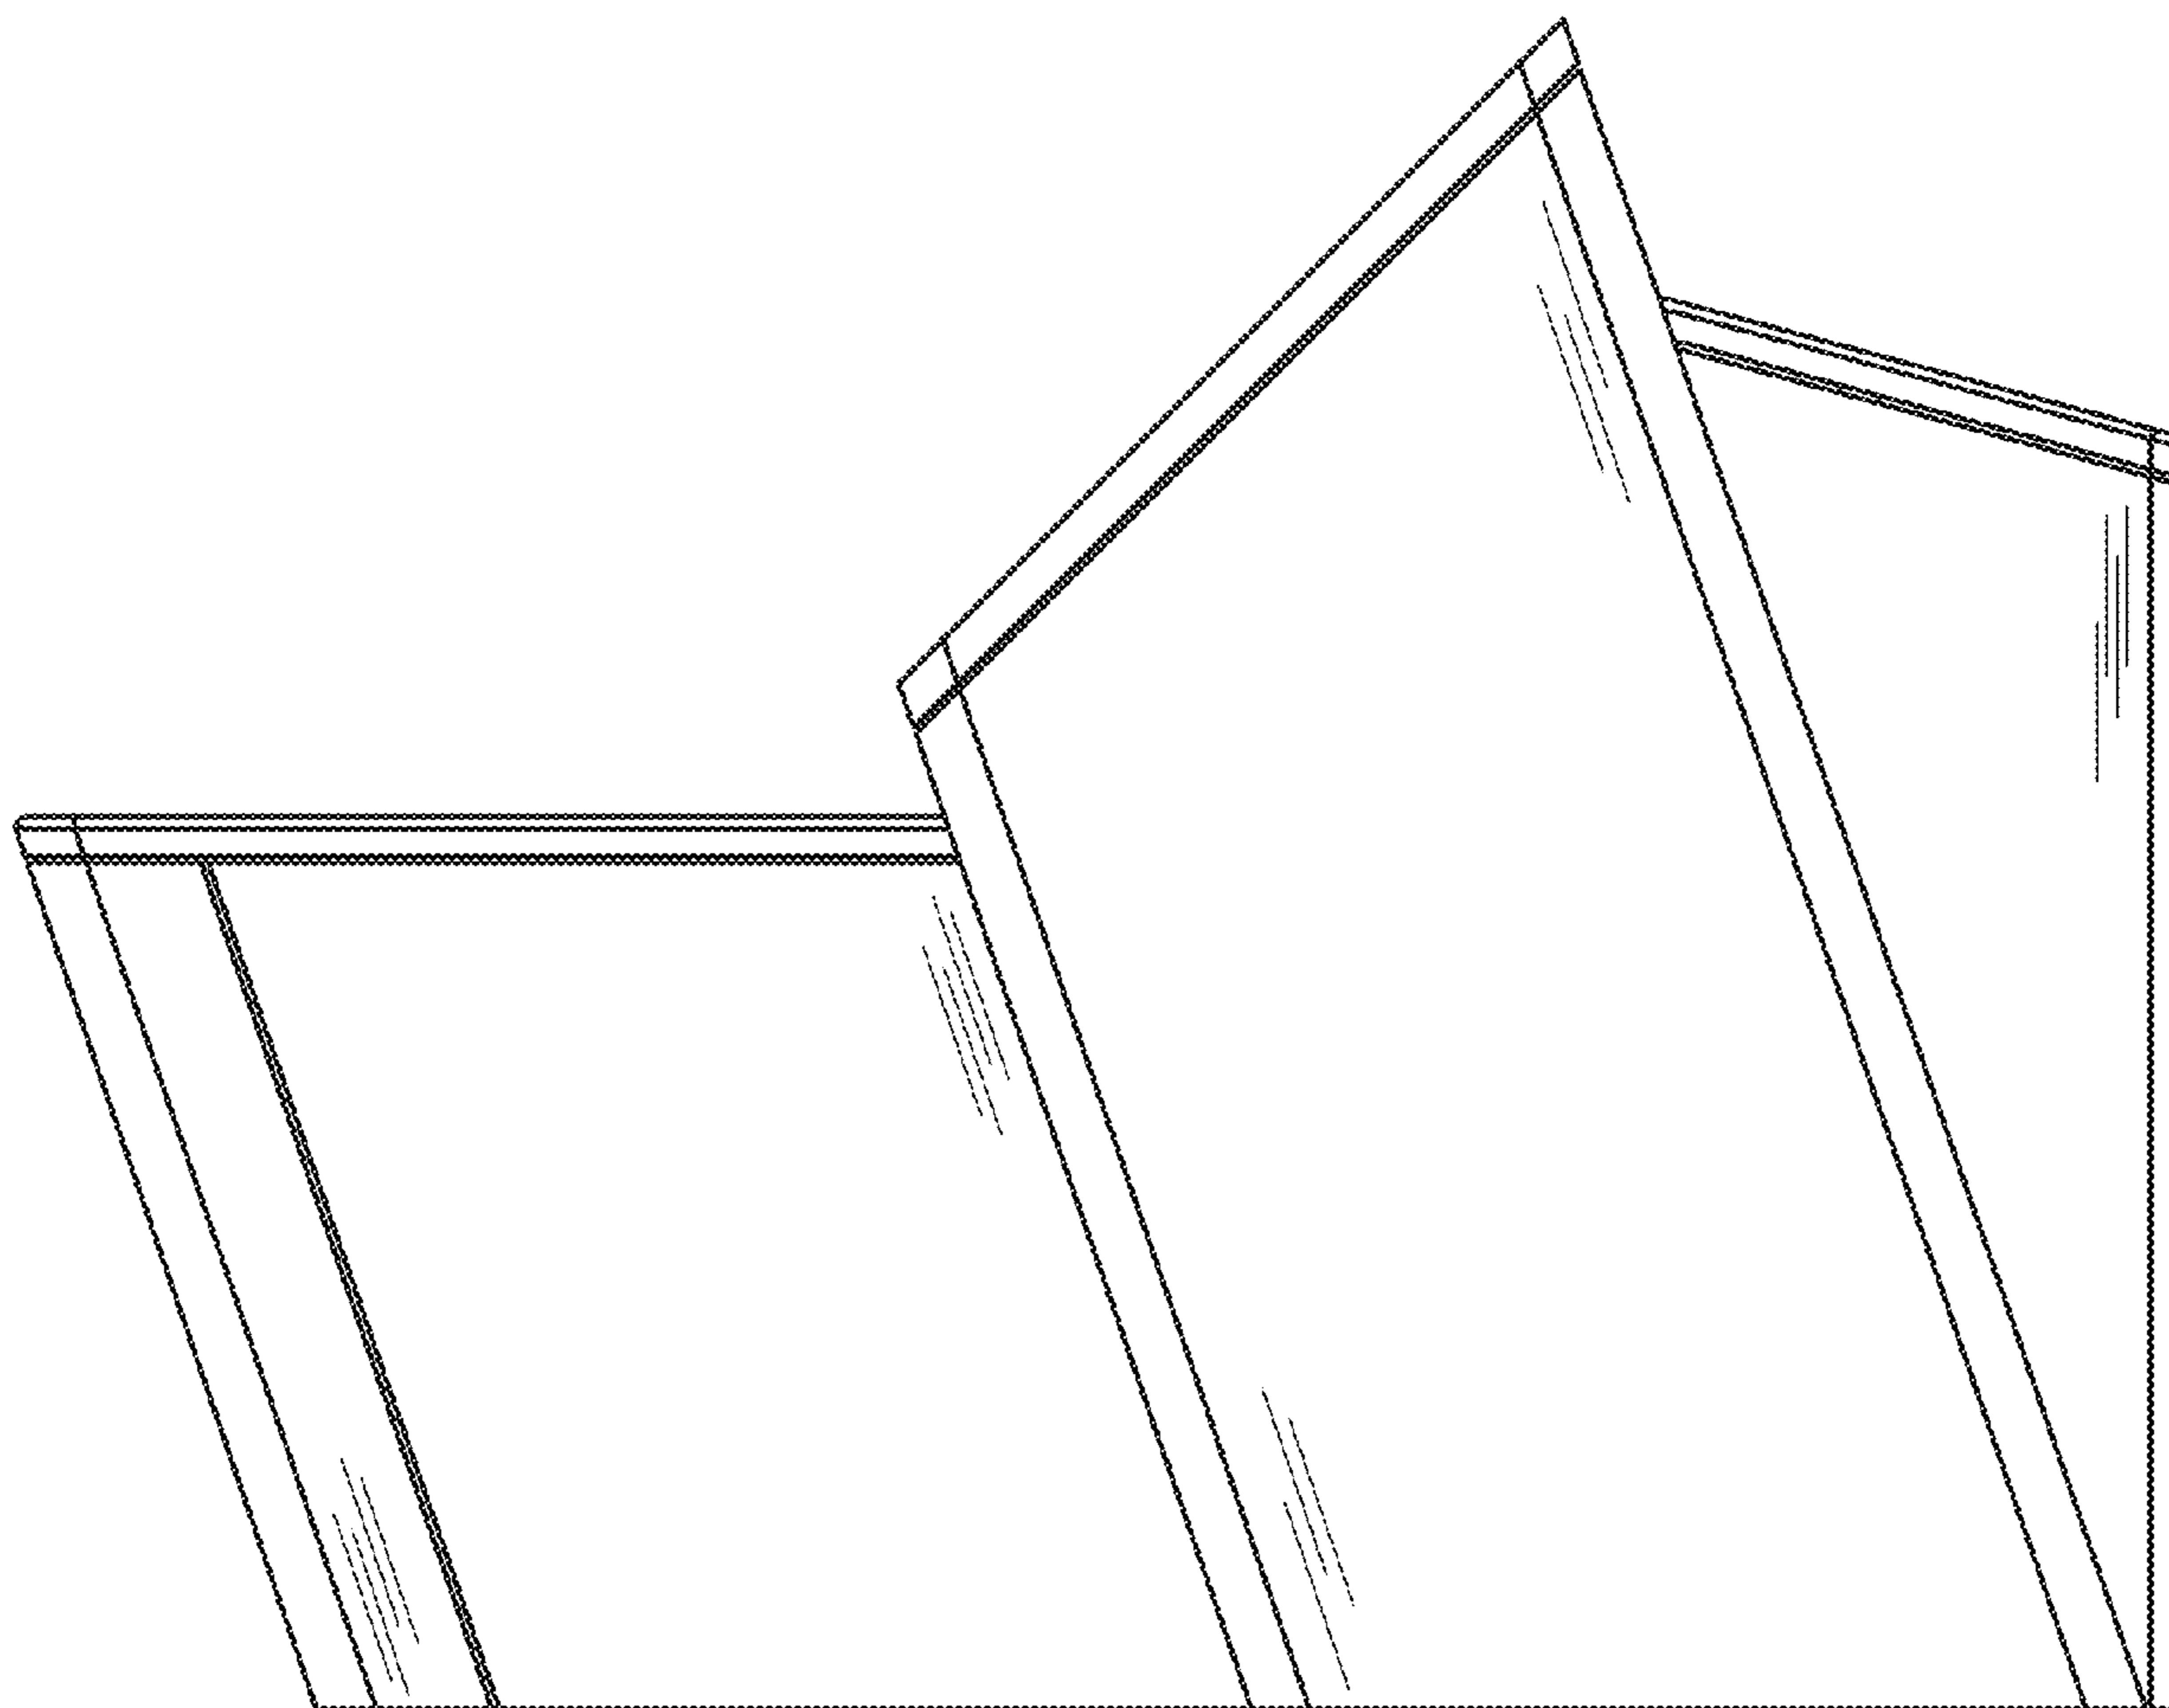


FIG. 7

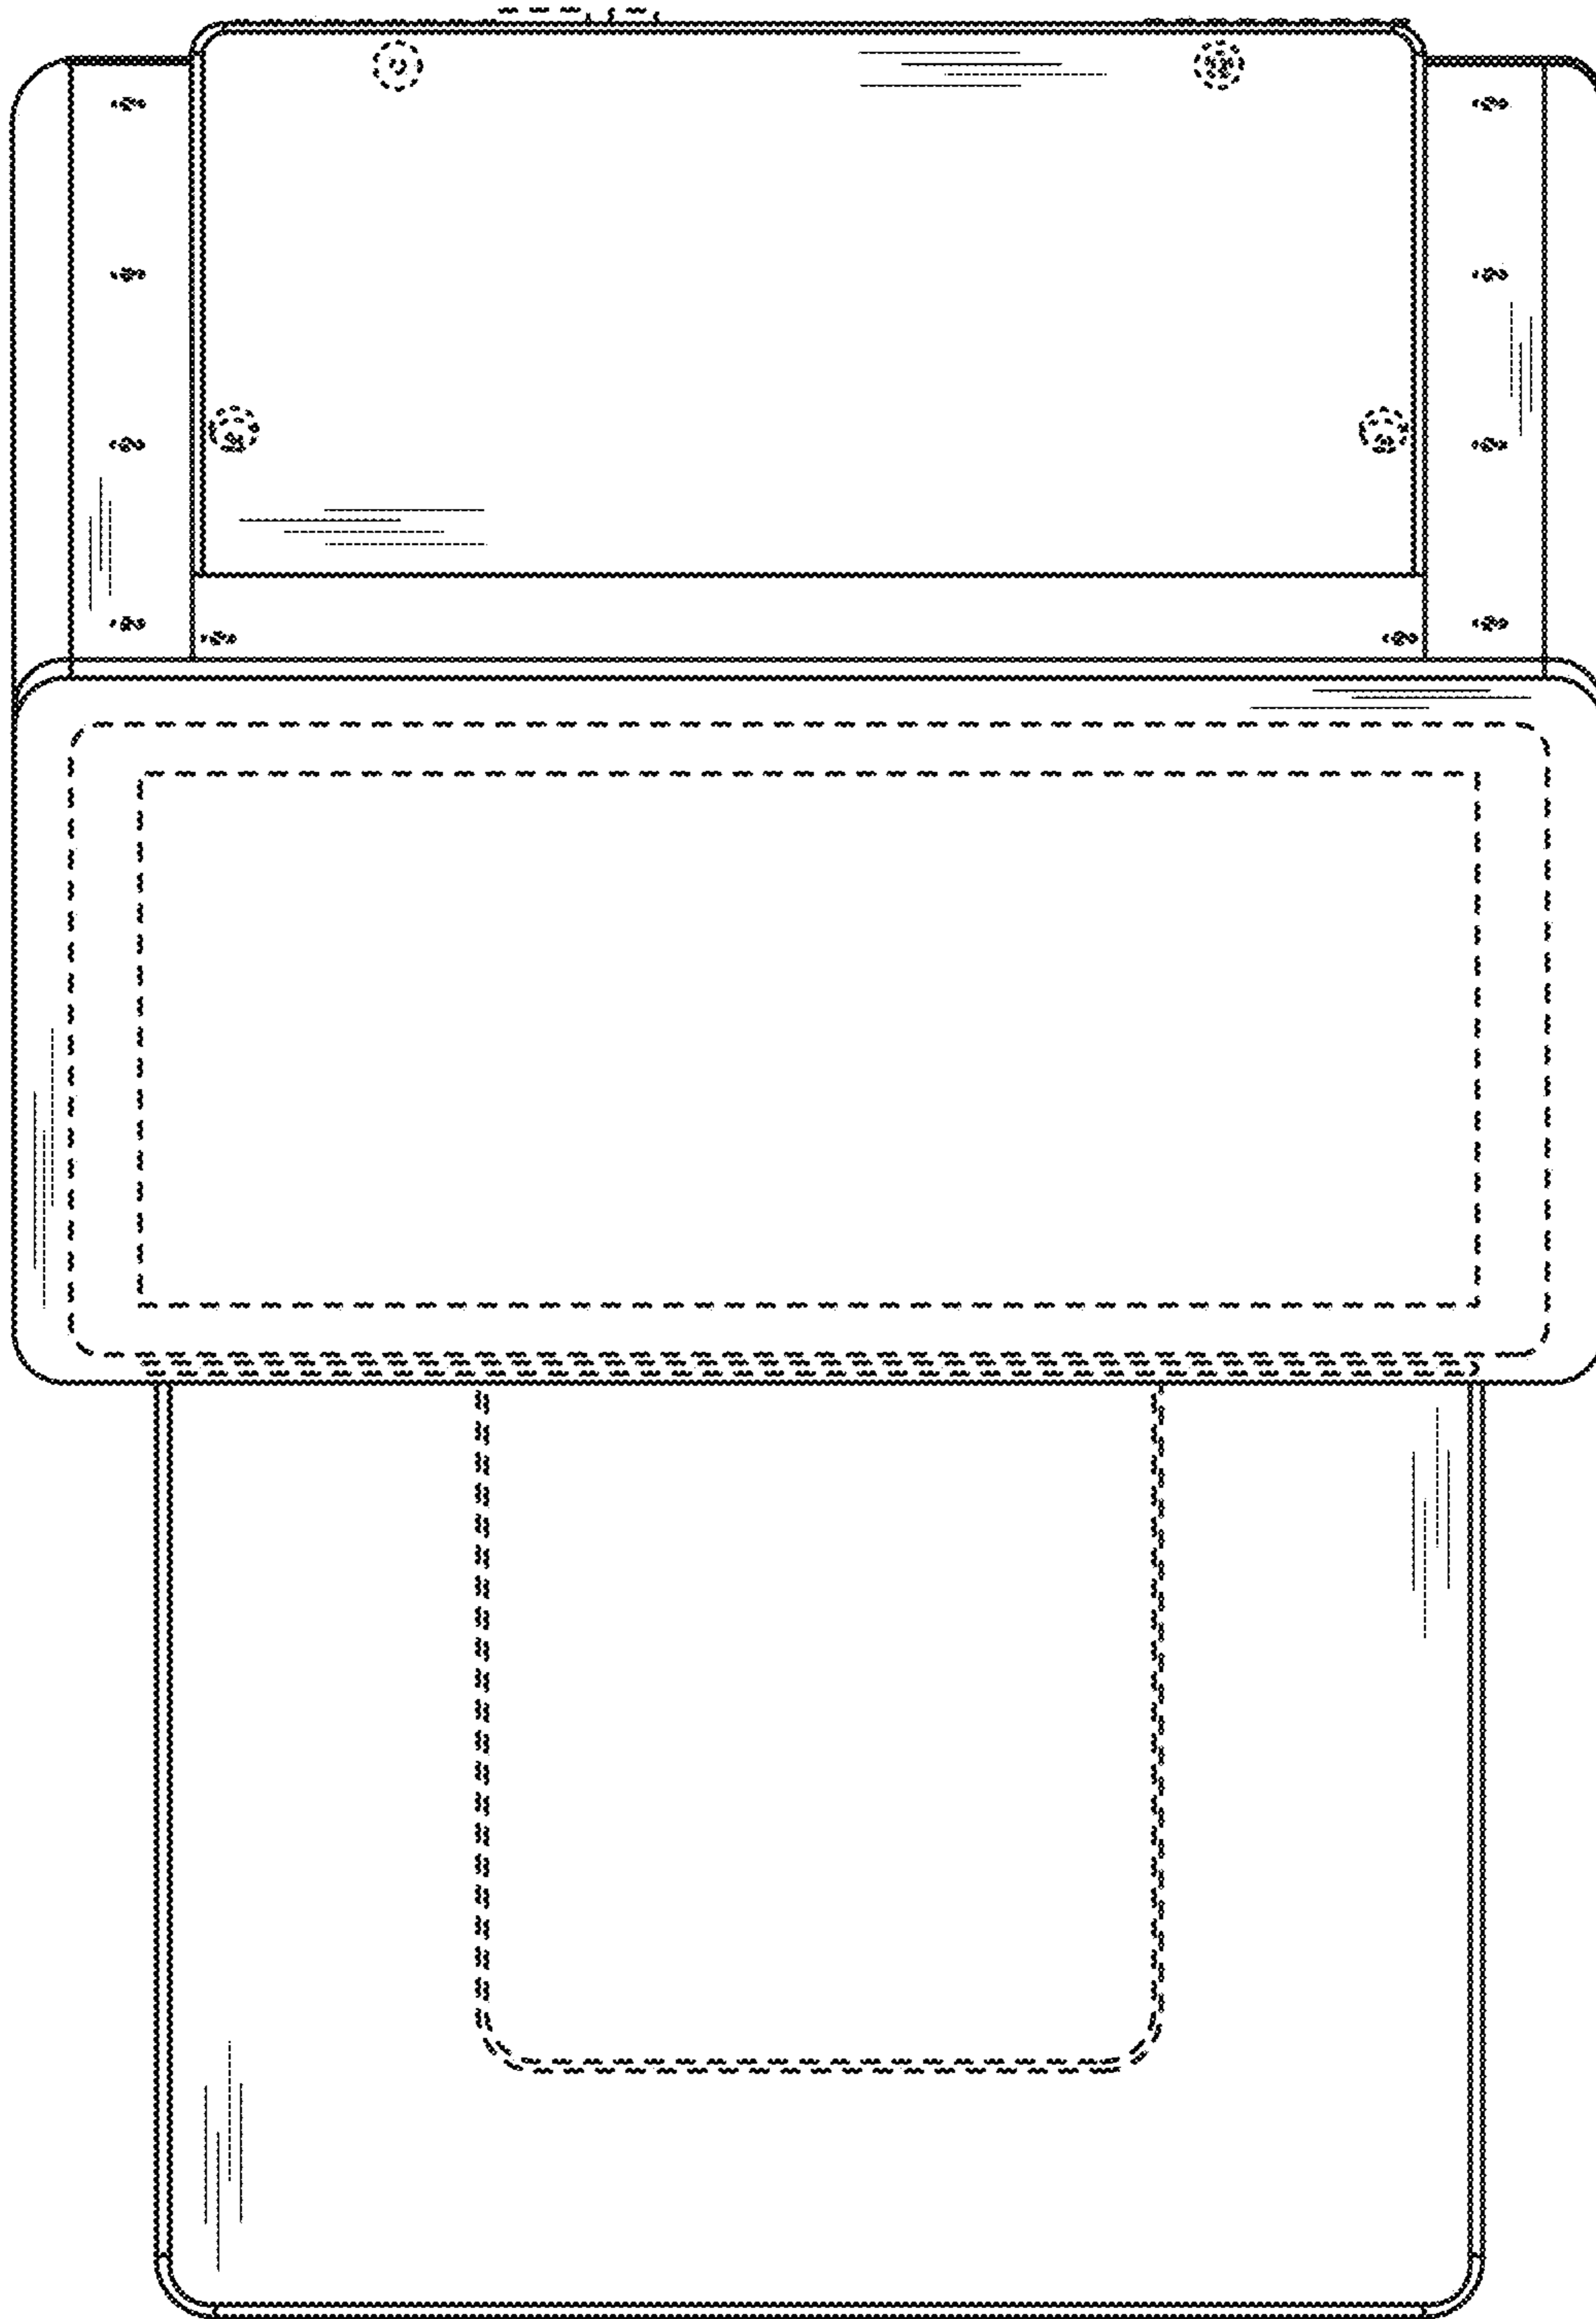


FIG. 8

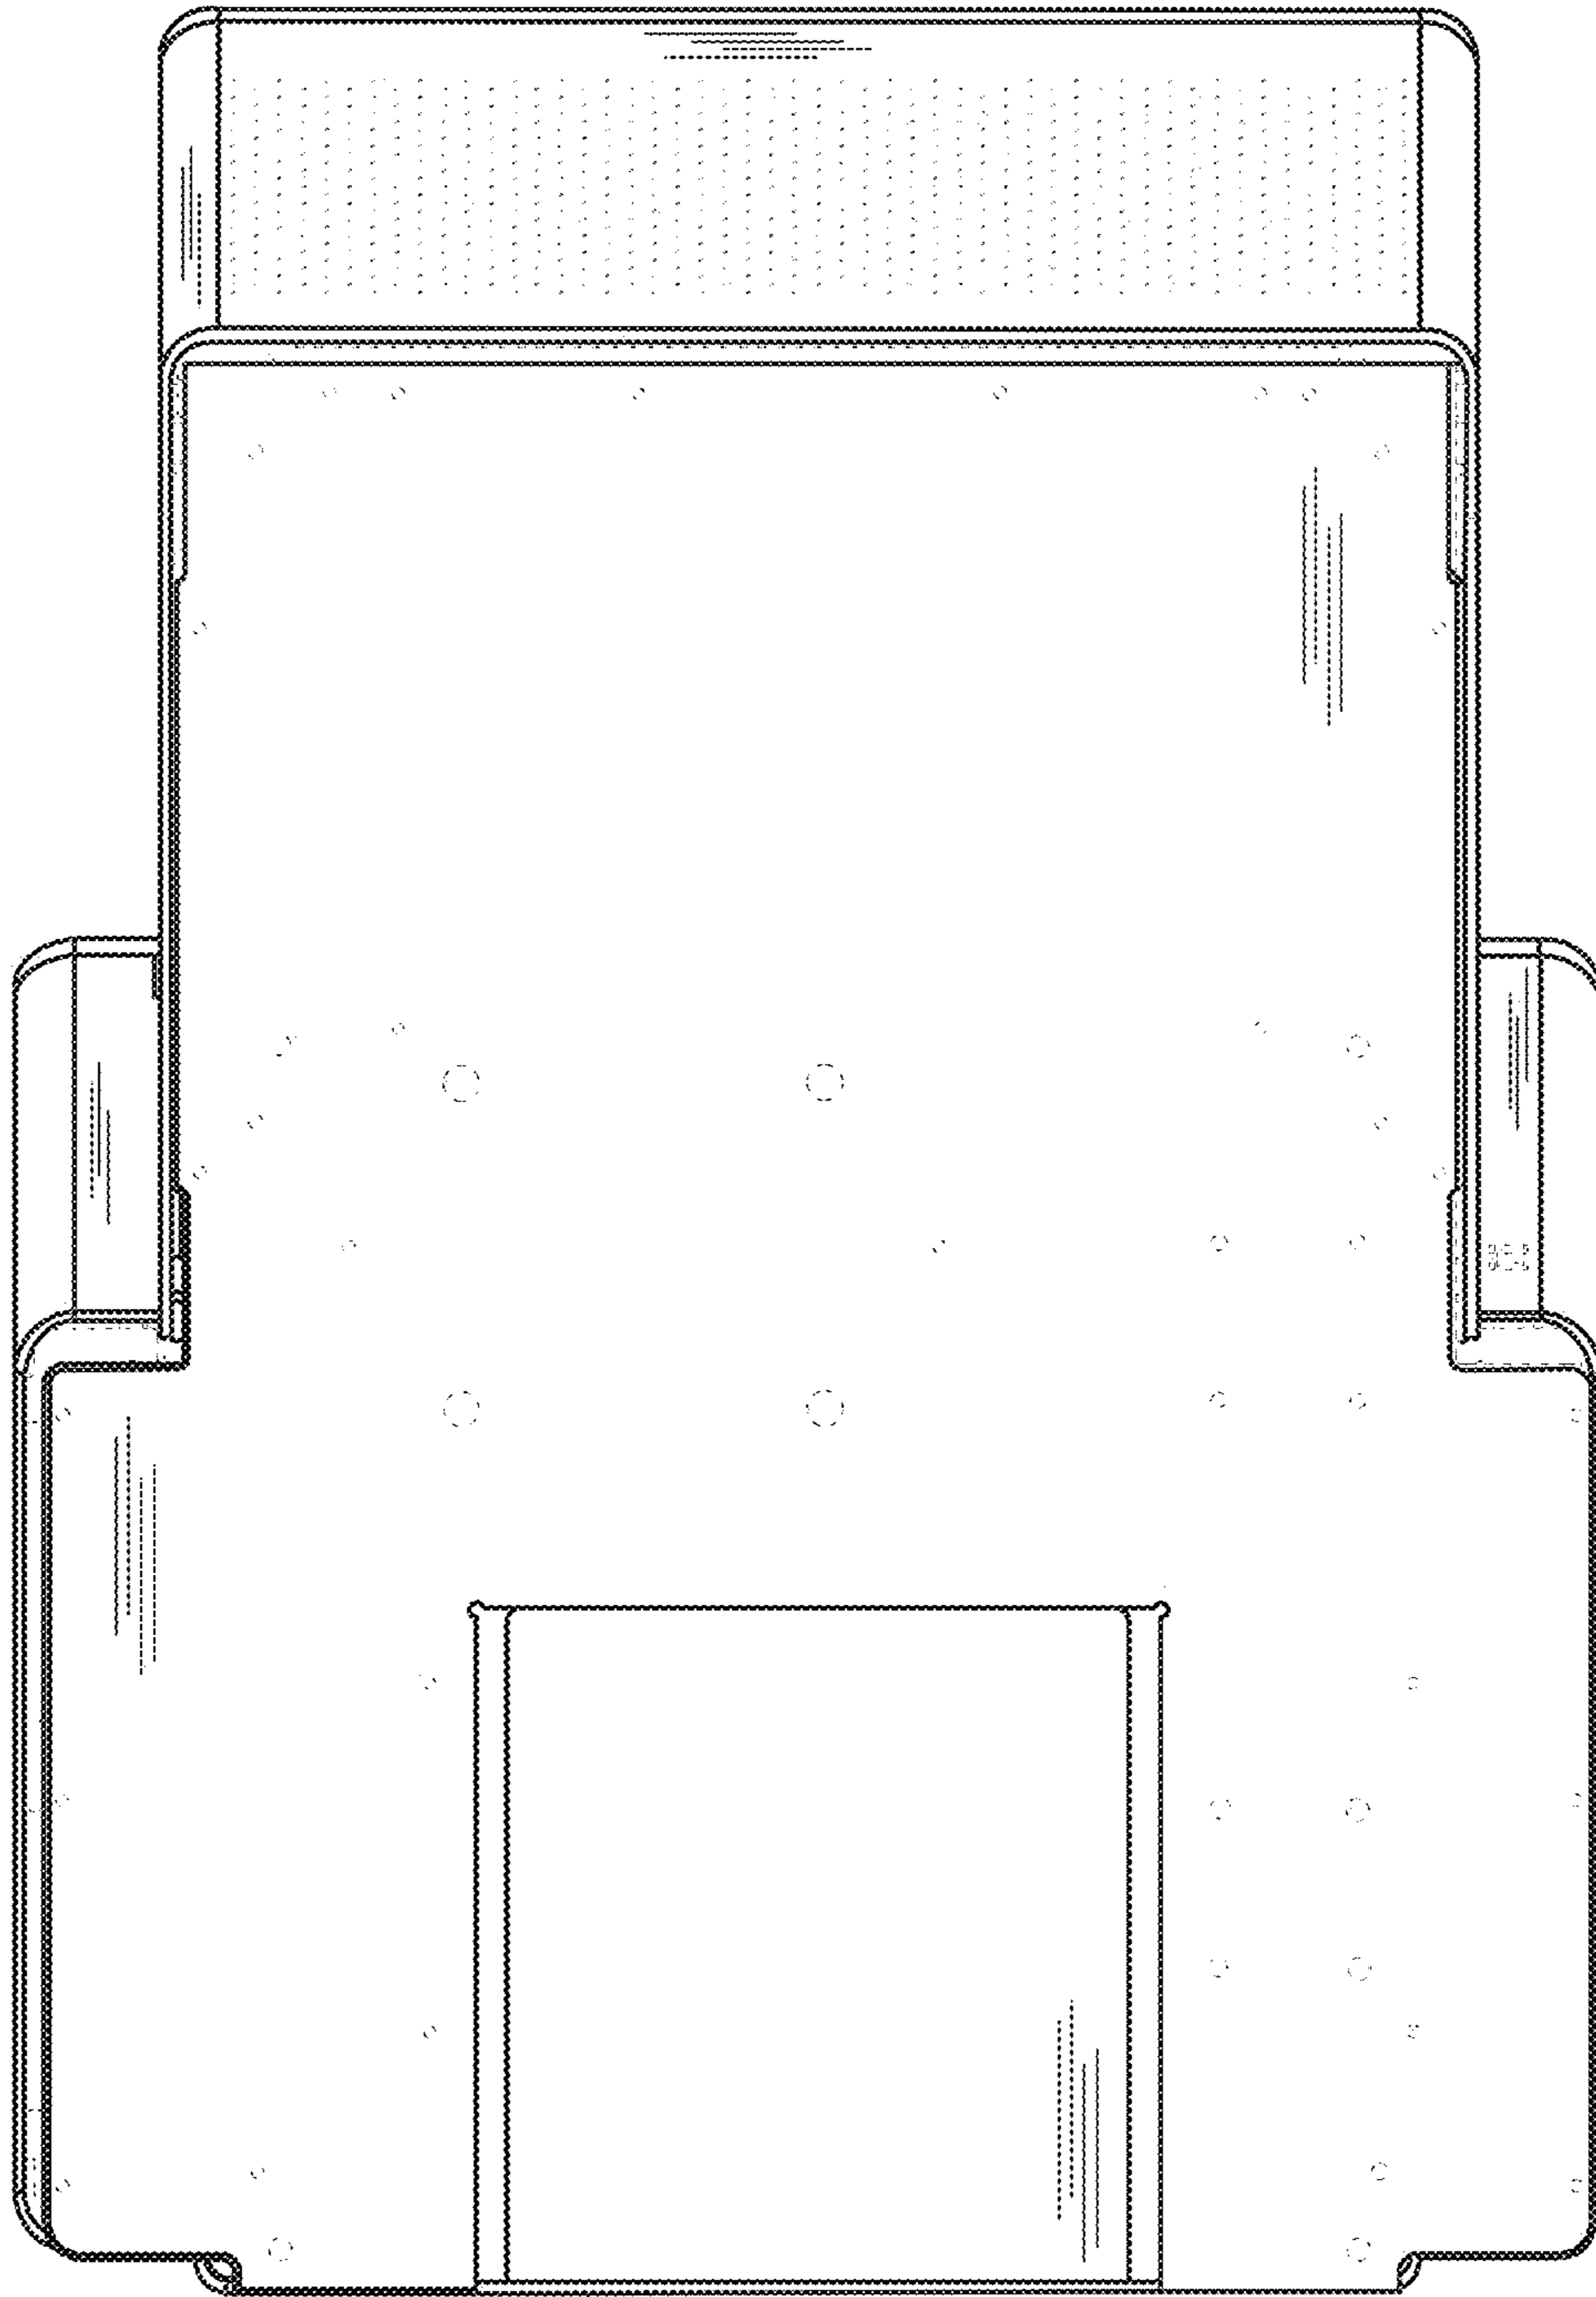


FIG. 9