



US00D984460S

(12) **United States Design Patent** (10) **Patent No.:** **US D984,460 S**
Ben-Haim et al. (45) **Date of Patent:** **** Apr. 25, 2023**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH ICON**

(71) Applicant: **Navix International Limited**, Road Town (VG)

(72) Inventors: **Shlomo Ben-Haim**, Marlow (GB); **Yitzhack Schwartz**, Haifa (IL); **Leonid Gluhovsky**, Gilon (IL); **Yaara Yarden**, Givat Shmuel (IL)

(73) Assignee: **Navix International Limited**, Road Town (VG)

(**) Term: **15 Years**

(21) Appl. No.: **29/774,343**

(22) Filed: **Mar. 16, 2021**

Related U.S. Application Data

(62) Division of application No. 29/619,342, filed on Sep. 28, 2017, now Pat. No. Des. 918,929.

(51) **LOC (14) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485-495

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D526,326 S 8/2006 Matsumoto
D614,634 S 4/2010 Nilsen

(Continued)

FOREIGN PATENT DOCUMENTS

JP 2017-162476 9/2017

OTHER PUBLICATIONS

Masayoshi Takashima, published Jul. 4, 2014 [online] by sinuswellbeing.com. Site accessed Sep. 22, 2022. Available at URL: <<http://www.sinuswellbeing.com/blog/2014/7/4/why-are-doctors-still-using-2d-imaging-ct-an-mri-scans-when-3d-is-readily-available>>.*

(Continued)

Primary Examiner — Daniel J Domino

(57) **CLAIM**

We claim the ornamental design for a display screen or portion thereof with icon, as shown and described.

DESCRIPTION

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a front view of a display screen or portion thereof with icon in accordance with a first embodiment;

FIG. 2 is a front view of a display screen or portion thereof with icon in accordance with a second embodiment;

FIG. 3 is a front view of a display screen or portion thereof with icon in accordance with a third embodiment;


FIG. 4 is a front view of a display screen or portion thereof with icon in accordance with a fourth embodiment; and,

FIG. 5 is a front view of a display screen or portion thereof with icon in accordance with a fifth embodiment.

The broken line in each FIGURE shows portions of the display screen or portion thereof for the purpose of illustrating environmental structure and forms no part of the claimed design.

This patent application contains at least one drawing executed in grayscale or color and is being filed by EFS.

1 Claim, 5 Drawing Sheets
(5 of 5 Drawing Sheet(s) Filed in Color)

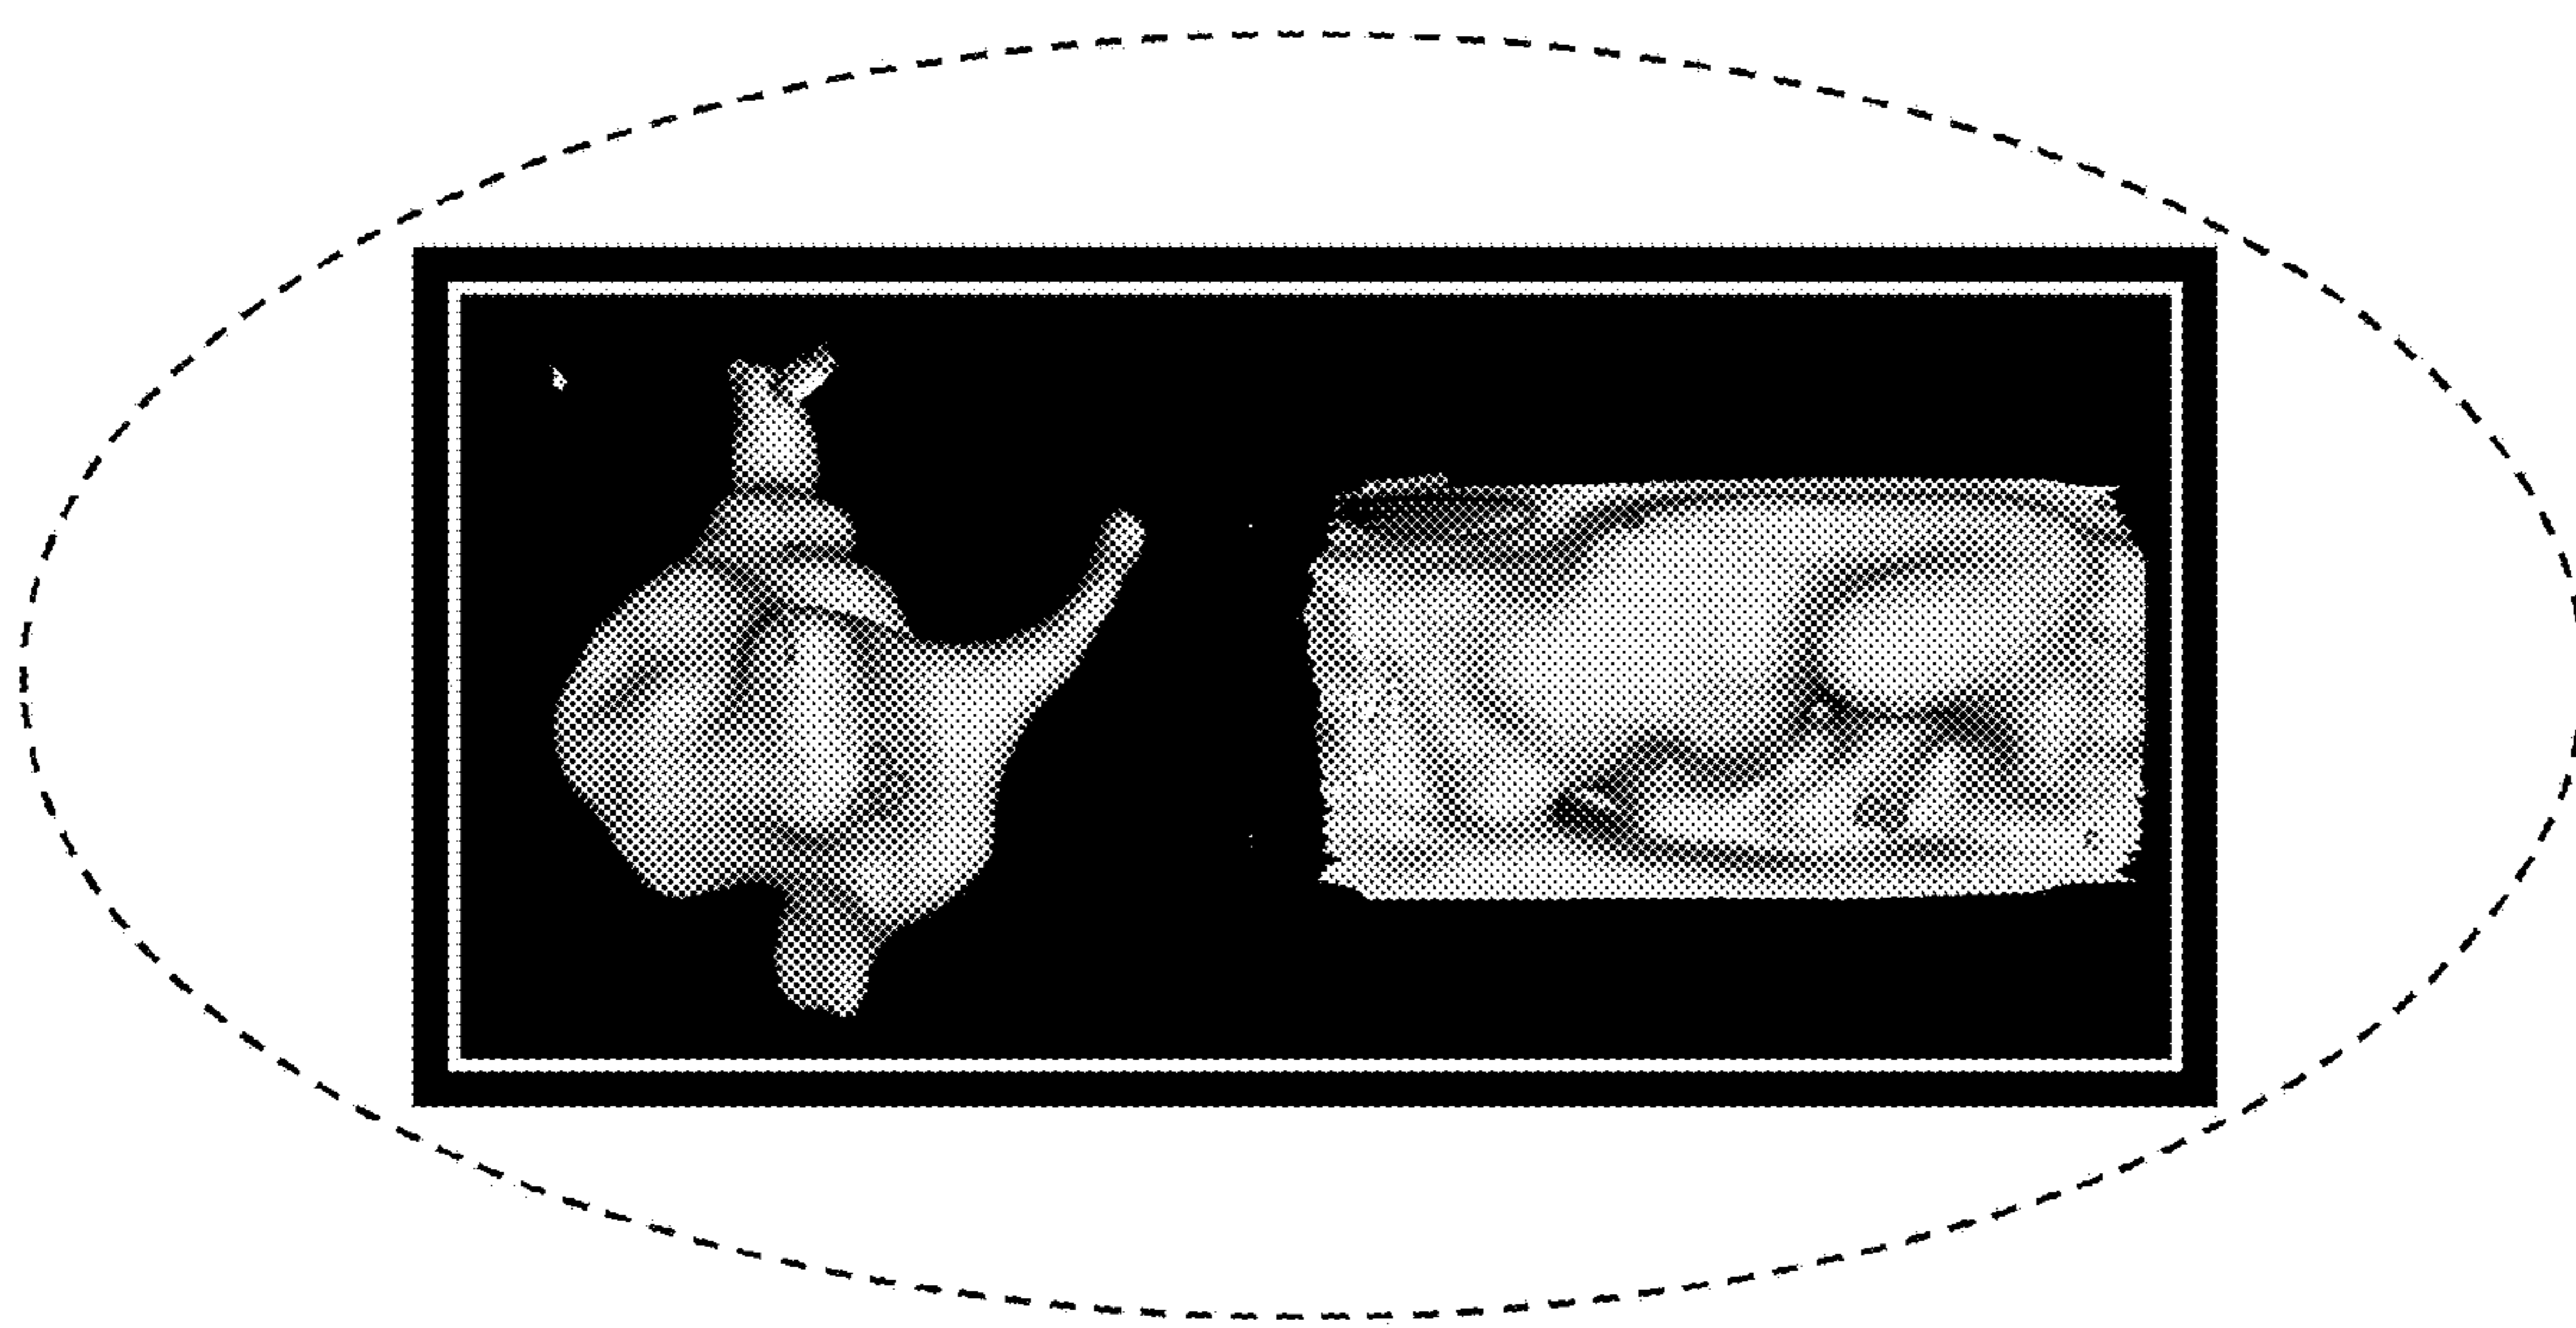

(58) **Field of Classification Search**

CPC G06F 3/048; G06F 3/0481; G06F 3/04812;
 G06F 3/04815; G06F 3/04817; G06F
 3/0482; G06F 3/0483; G06F 3/0484;
 G06F 3/04842; G06F 3/04845; G06F
 3/04847; G06F 3/0485; G06F 3/04855;
 G06F 3/0486; G06F 3/0487; G06F
 3/0488; G06F 3/04883; G06F 3/04886
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D714,818	S	10/2014	Wang	
D722,609	S	2/2015	Lee	
D741,884	S	10/2015	Lee	
D843,382	S	3/2019	Shadforth	
D843,385	S	3/2019	Ben-Haim	
D847,198	S	4/2019	Taylor	
D858,532	S *	9/2019	Lei	D14/485
D864,235	S	10/2019	Ben-Haim	
D867,392	S *	11/2019	Wassborn	D14/489
D868,095	S *	11/2019	Morris	D14/486
D874,482	S *	2/2020	Ishigaki	D14/485
D874,515	S *	2/2020	Ishigaki	D14/489
D878,413	S *	3/2020	Ben-Haim	D14/485
D878,414	S *	3/2020	Ben-Haim	D14/485
D905,741	S *	12/2020	Dye	D14/489
D918,929	S *	5/2021	Ben-Haim	D14/485
D918,957	S *	5/2021	Ben-Haim	D14/489
D918,958	S *	5/2021	Ben-Haim	D14/489
D919,648	S *	5/2021	Gilboa	D14/489
D944,853	S *	3/2022	Ben-Haim	D14/489
2004/0009459	A1 *	1/2004	Anderson	G06T 19/00 703/11
2009/0125840	A1	5/2009	Squilla	
2013/0179162	A1	7/2013	Merschon	
2014/0176538	A1	6/2014	Lynn	
2015/0305646	A1	10/2015	Schwartz	
2015/0366523	A1	12/2015	Ben-Haim	
2016/0129349	A1 *	5/2016	Zhao	A63F 13/80 463/31
2017/0084029	A1 *	3/2017	Piazza	G06T 7/60

OTHER PUBLICATIONS

Hamza Mousa, published Jun. 27, 2019 [online] by medevel.com. Site accessed Sep. 22, 2022. Available at URL: <<https://medevel.com/ami-medical-imaging/>>.*

G. Sakas, published Aug. 1, 2002 [online] by semanticscholar.org. Site accessed Sep. 22, 2022. Available at URL: <<https://www.semanticscholar.org/paper/Trends-in-medical-imaging%3A-from-2D-to-3D-Sakas/9f01f98a9b8235dc38c751f74b93d976dbd8a5e2>>.*

Publication entitled GE Healthcare, CardEP dated 2016 (2 pages). Accepted Manuscript for publication in *HearthRhythm* entitled on the Accuracy of CartoMerge for Guiding Posterior Left Atrial Ablation in Man, by Zhong, H. et al. Acceptance date Jan. 29, 2007 (31 pages).

Presentation entitled EPD What's Next dated May 2017.

Presentation entitled Real-Time Lesion Formation and Gap Detection During Ablation of AF using Novel Electro-Magnetic Imaging System: 12-Month Follow-Up dated Jan. 2018.

Presentation entitled Durable-I Real-time gap detection during AF ablation using Dielectric Sensing dated Jan. 2017.

Presentation entitled Europace EHRA2017 Cardiostim EDP—Real Time Tissue Characterization During Ablation dated Jun. 2017.

Presentation entitled HD 3D Dielectric Anatomical Mapping depicting detailed and clinically useful RA, LA and LV anatomy dated May 2017.

Presentation entitled Europace EHRA2017 Cardiostim EDP EP Dynamics—KOL Meeting dated Jun. 2017.

Presentation entitled EP Dynamics—KOL Meeting dated May 2017.

Article entitled Real-Time Lesion Formation and Gap Detection During Ablation of AF Using Novel Electro-Anatomical Dielectric Mapping System: 12-Month Follow-Up dated Jan. 2018.

Presentation entitled Novel Electro Magnetic Imaging, Vivek Reddy dated Jan. 2018.

Presentation entitled Novosibirsk EDP Experience dated May 2017.

* cited by examiner

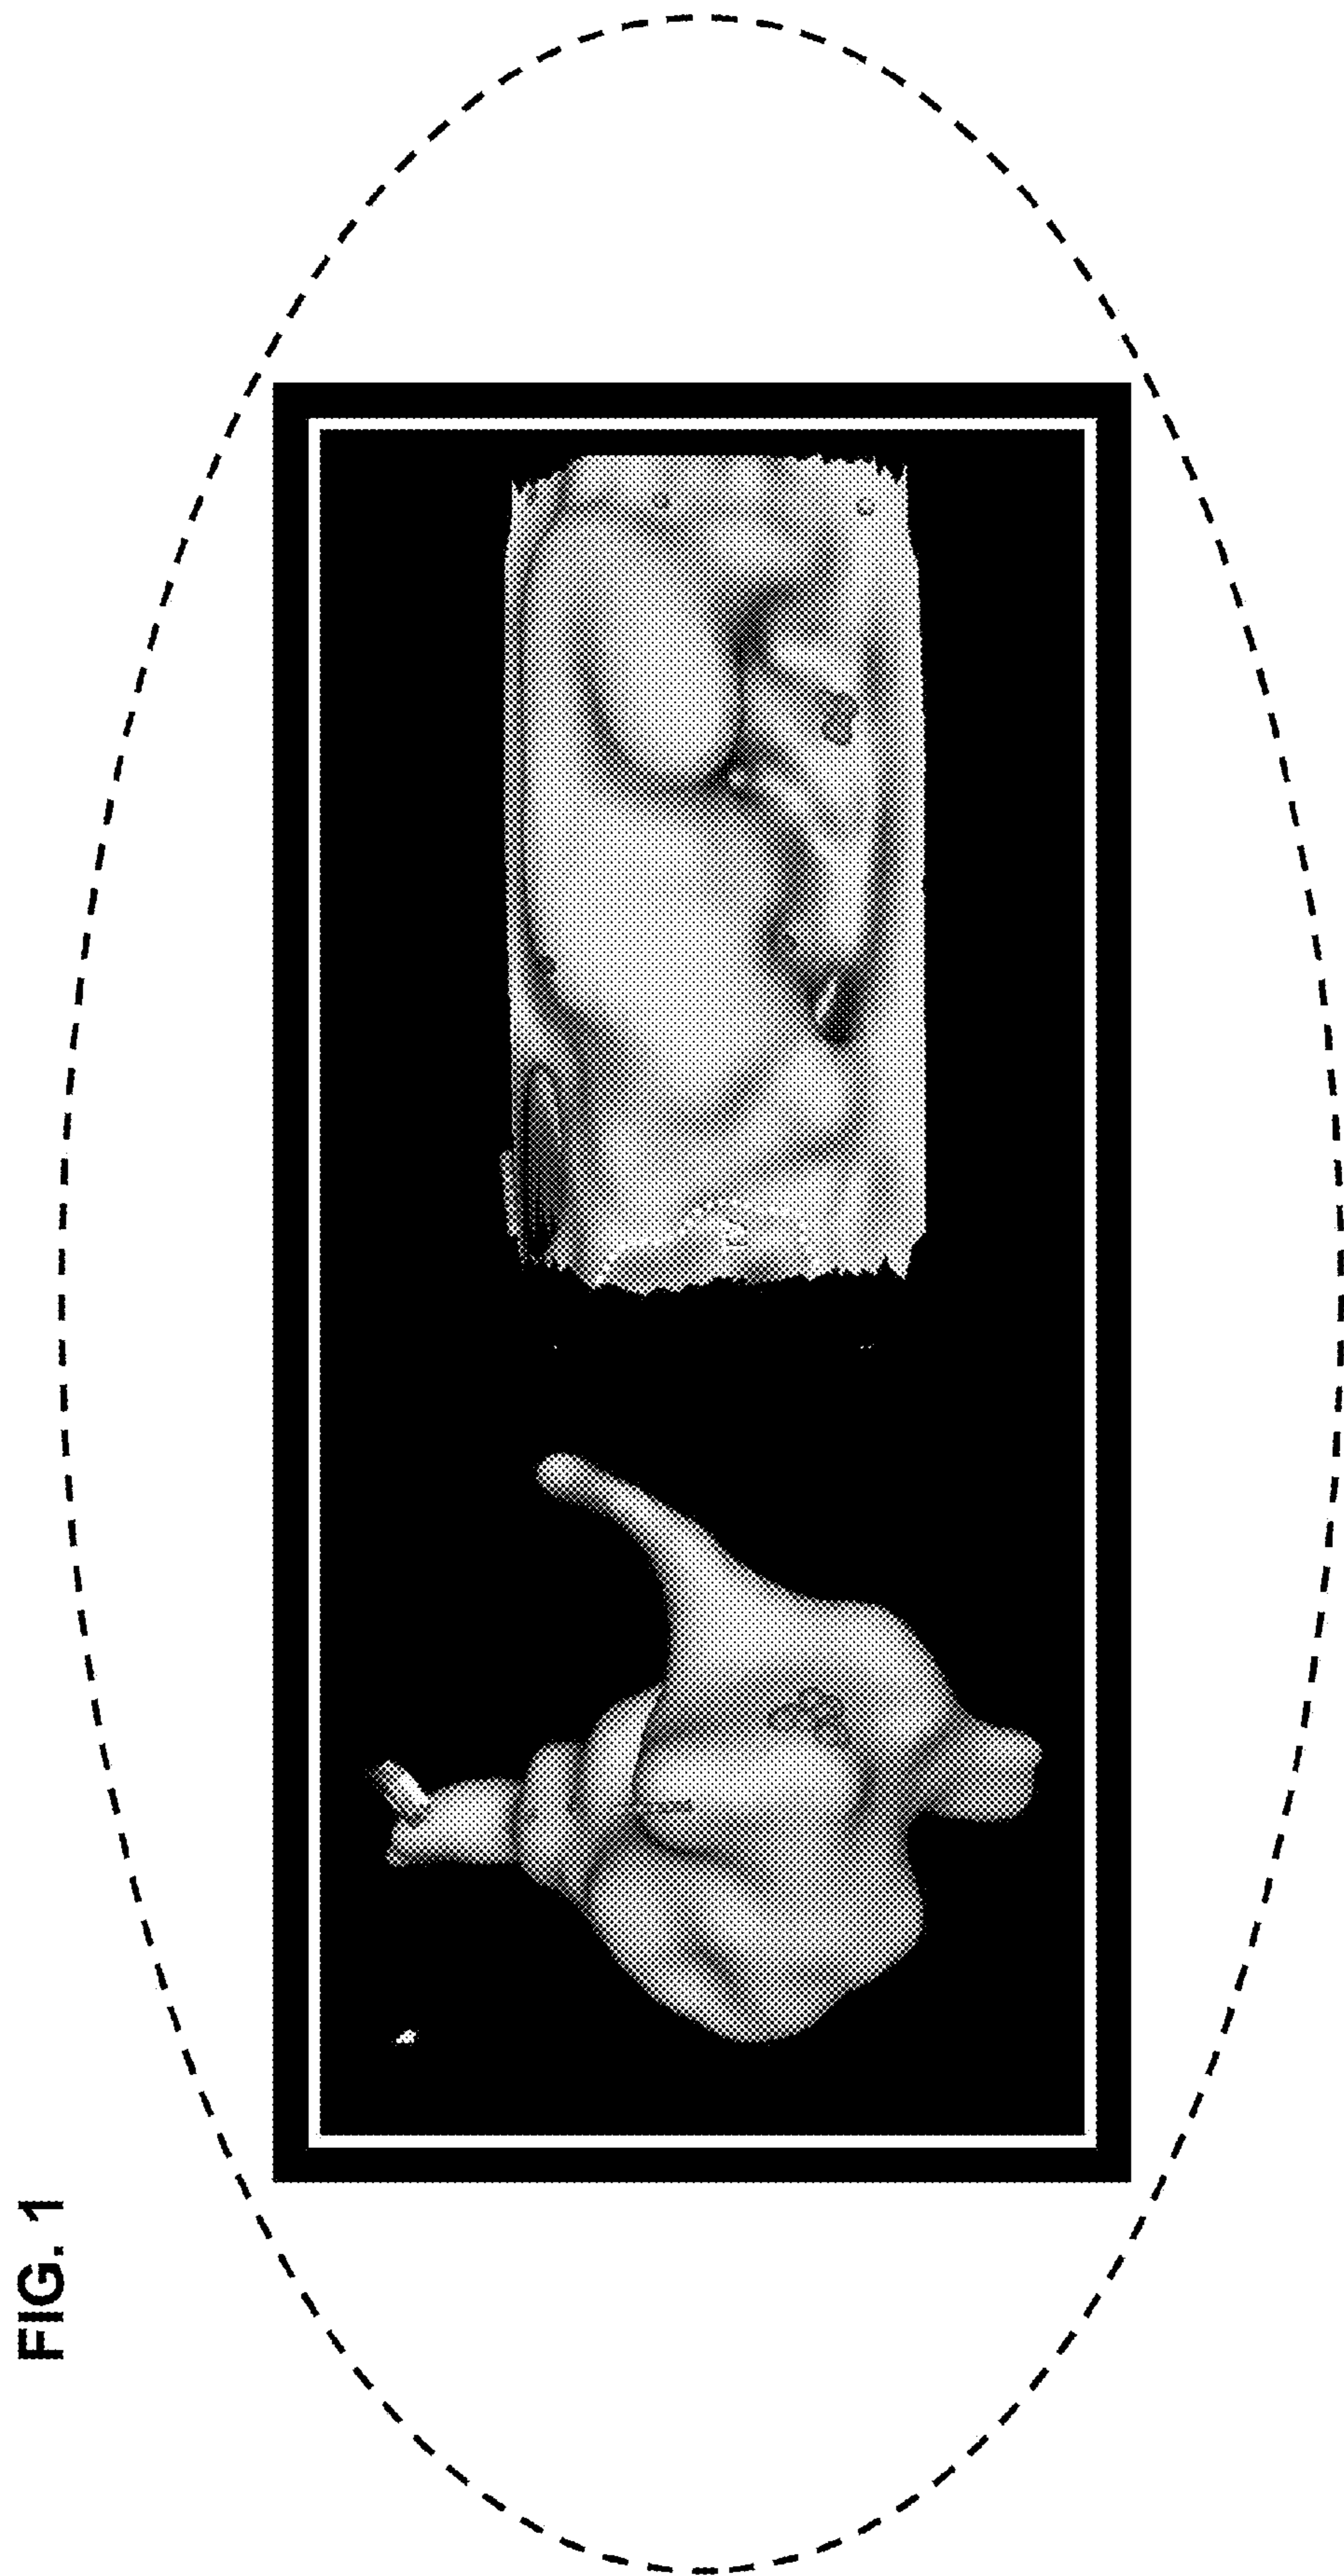
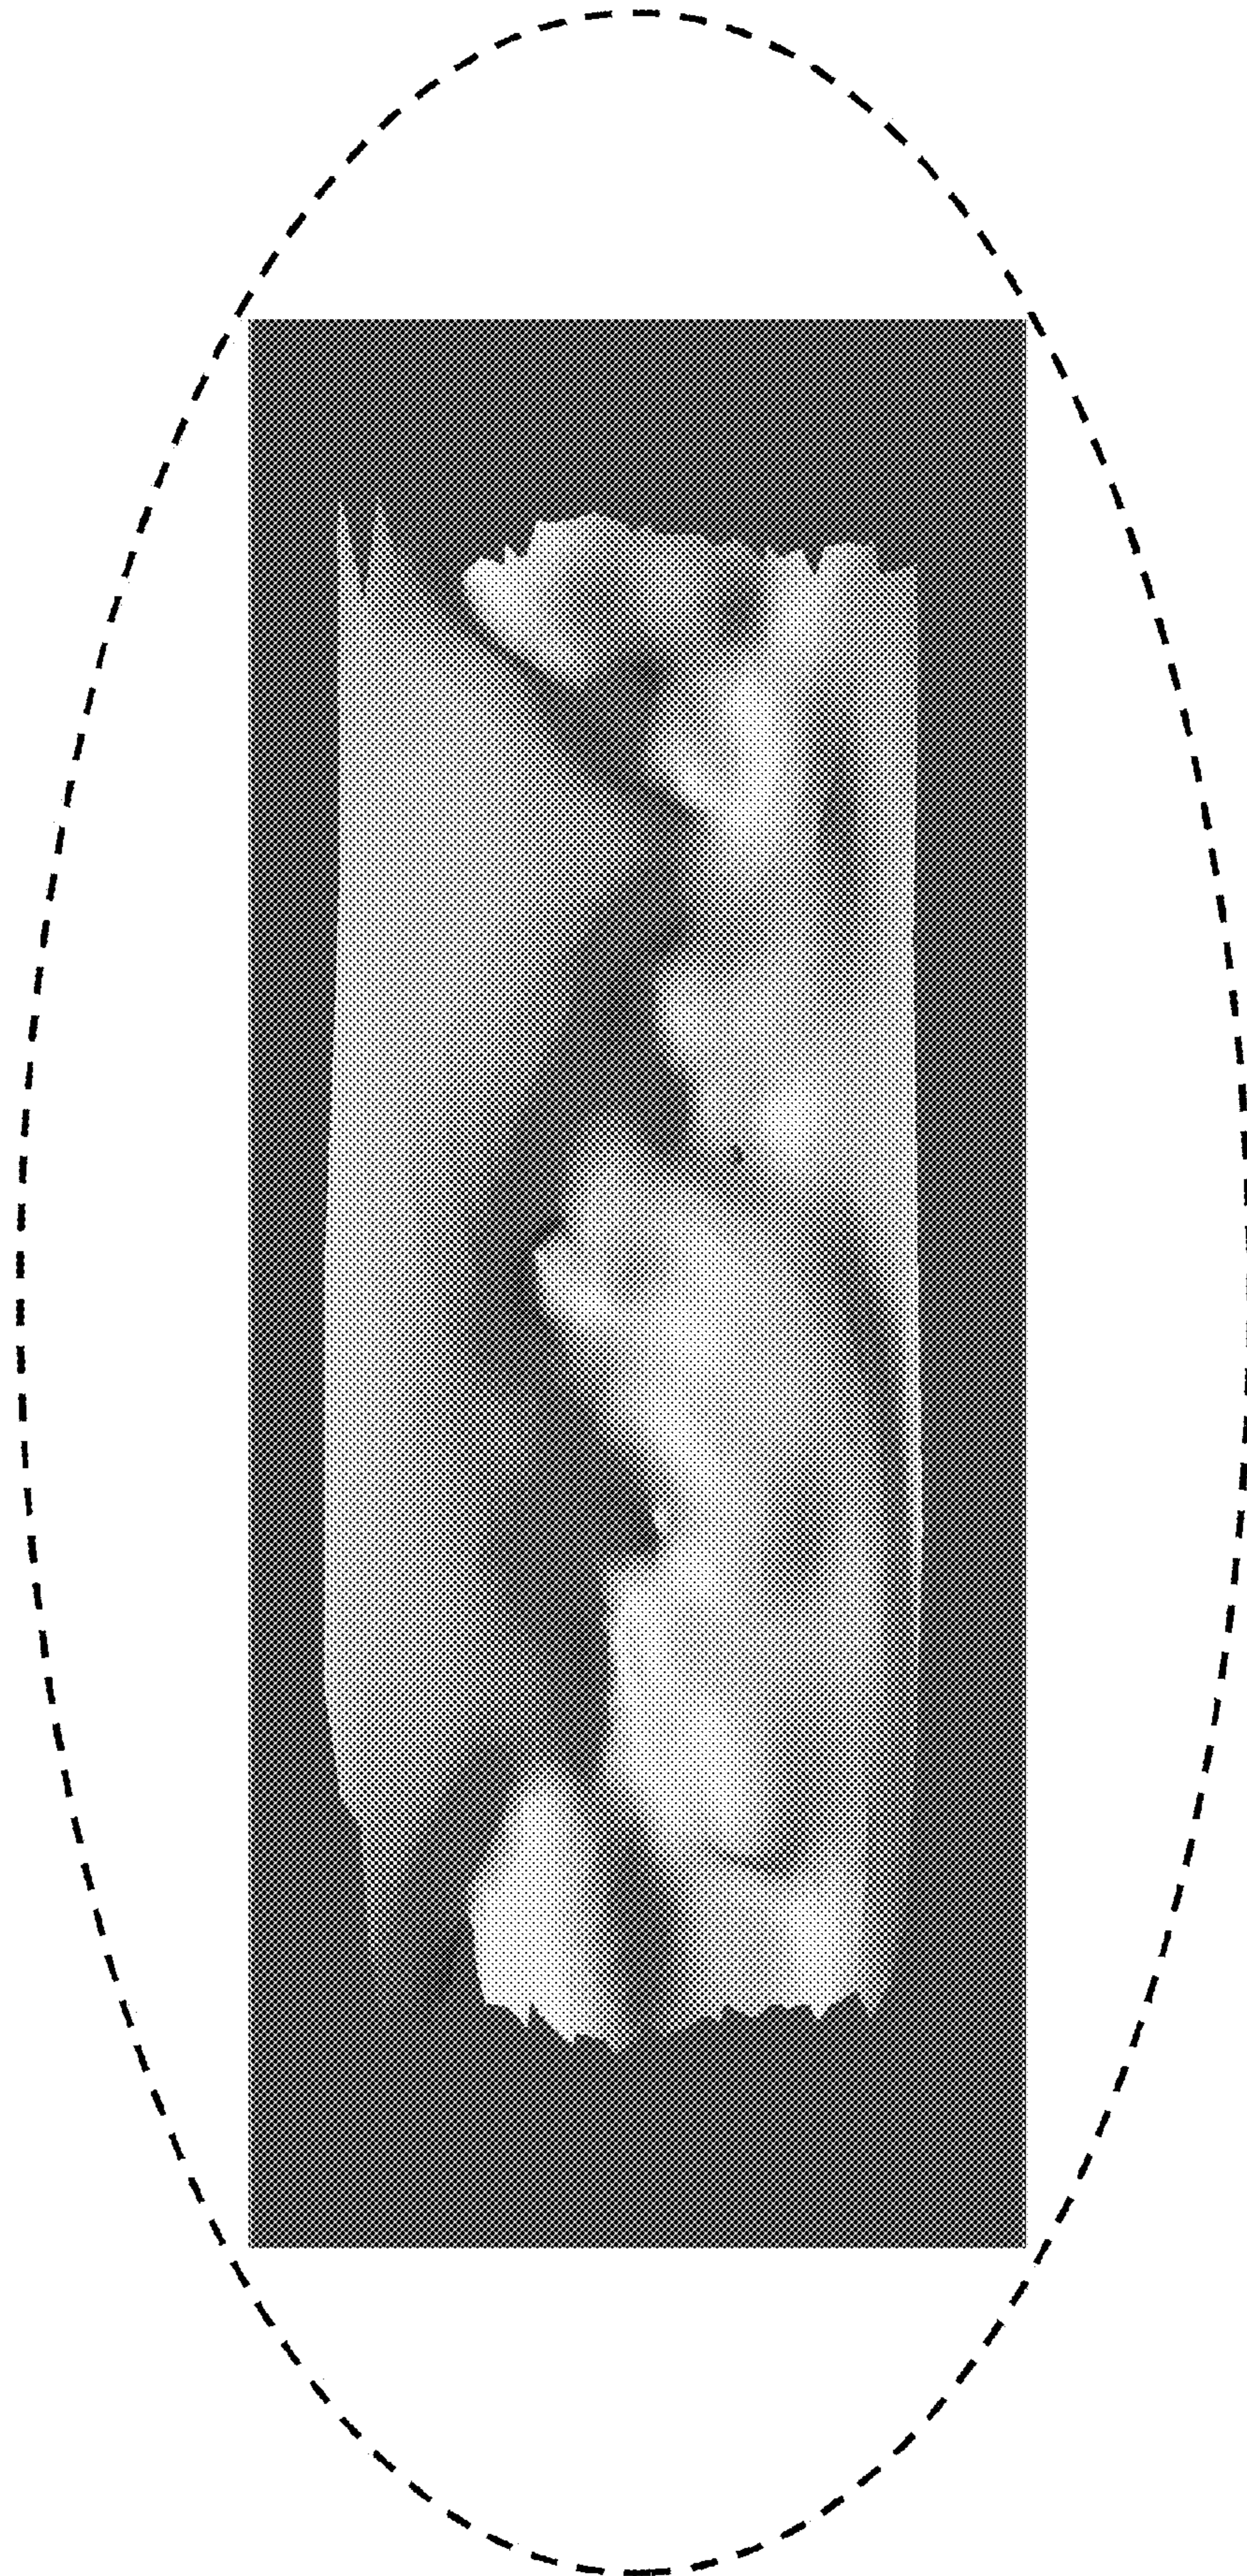


FIG. 1

FIG. 2



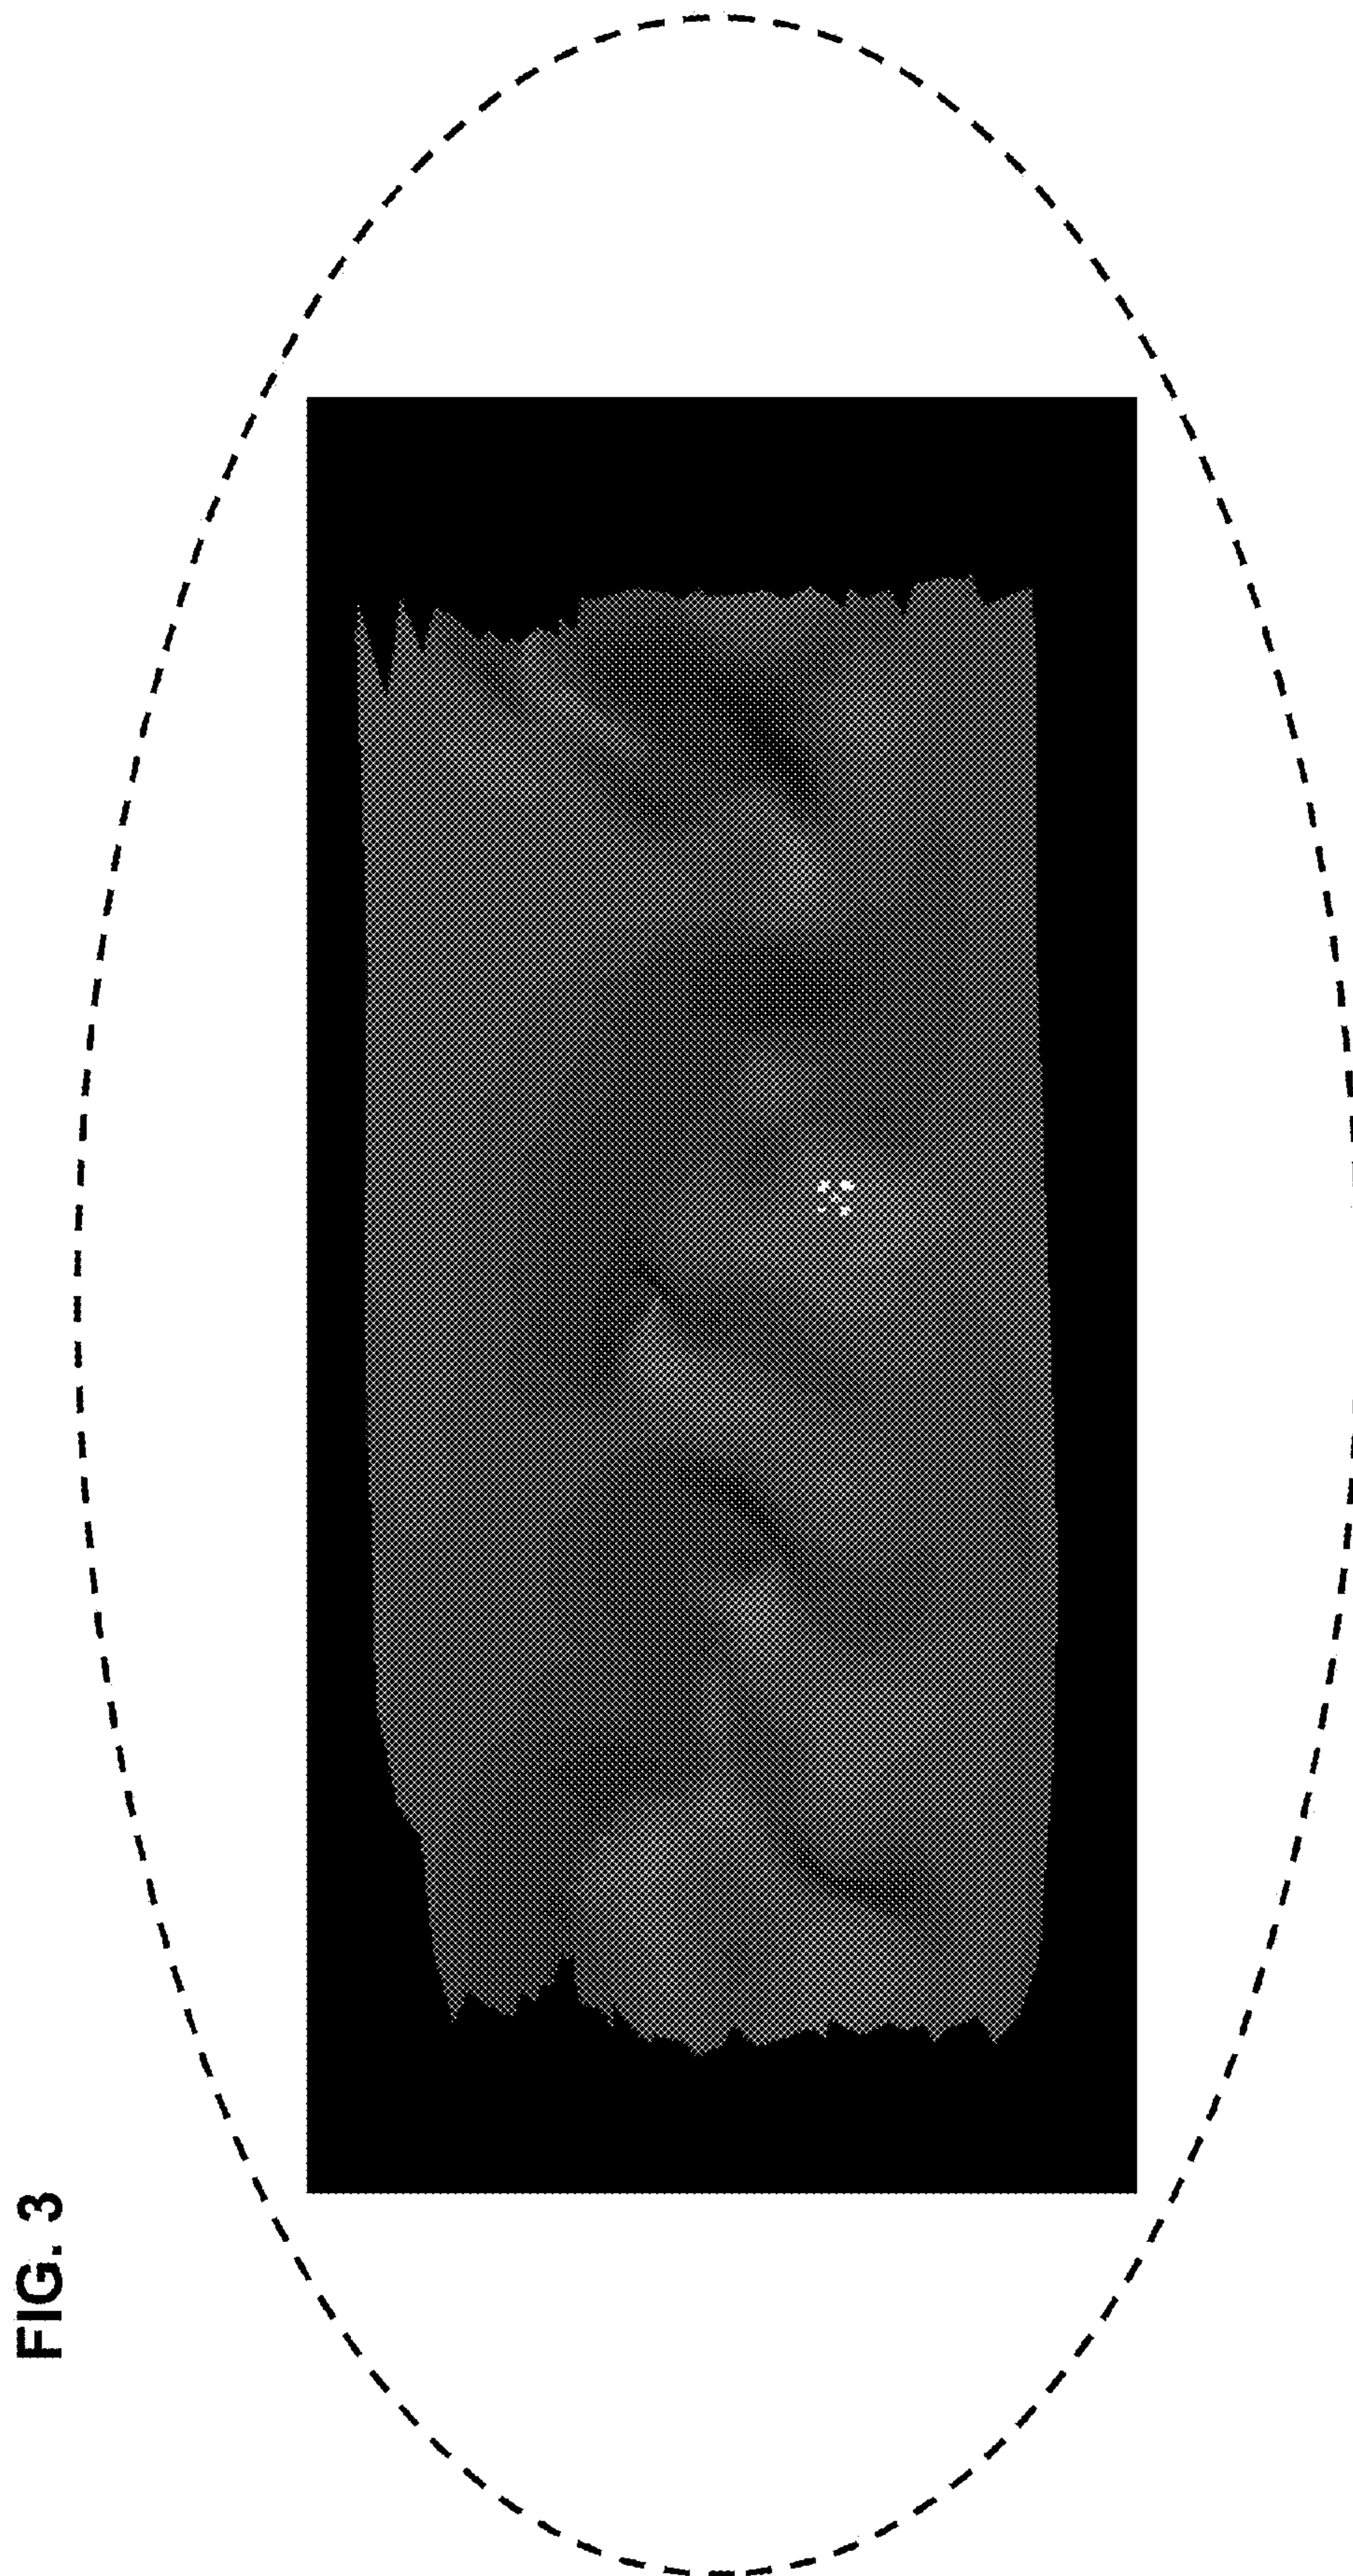


FIG. 3

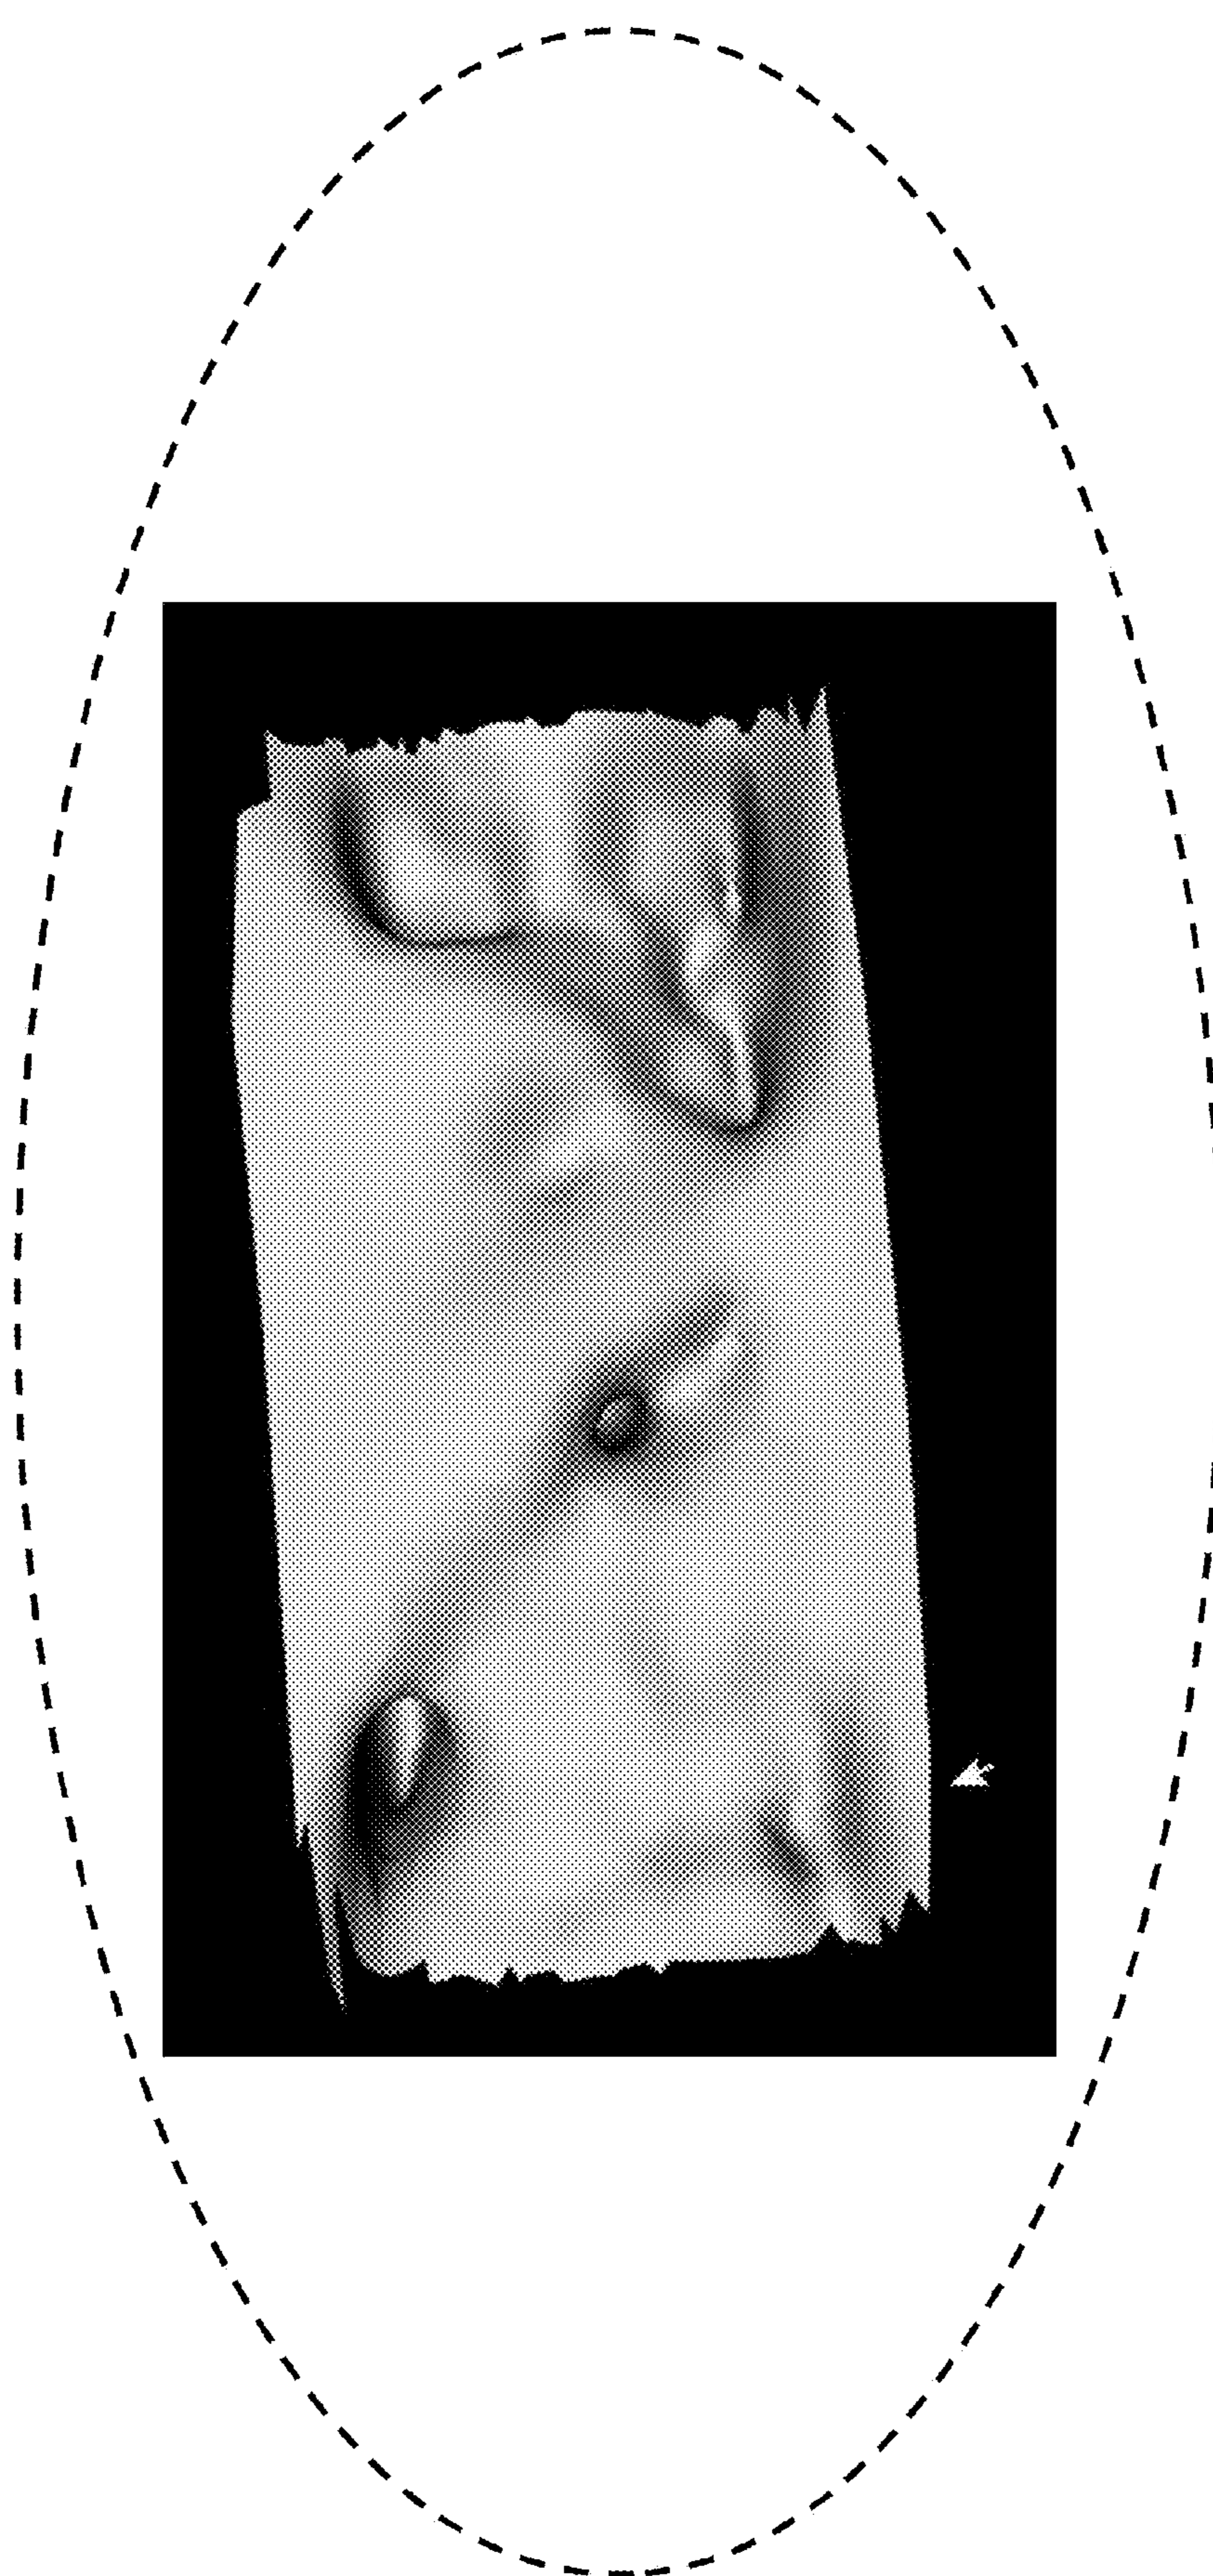


FIG. 4

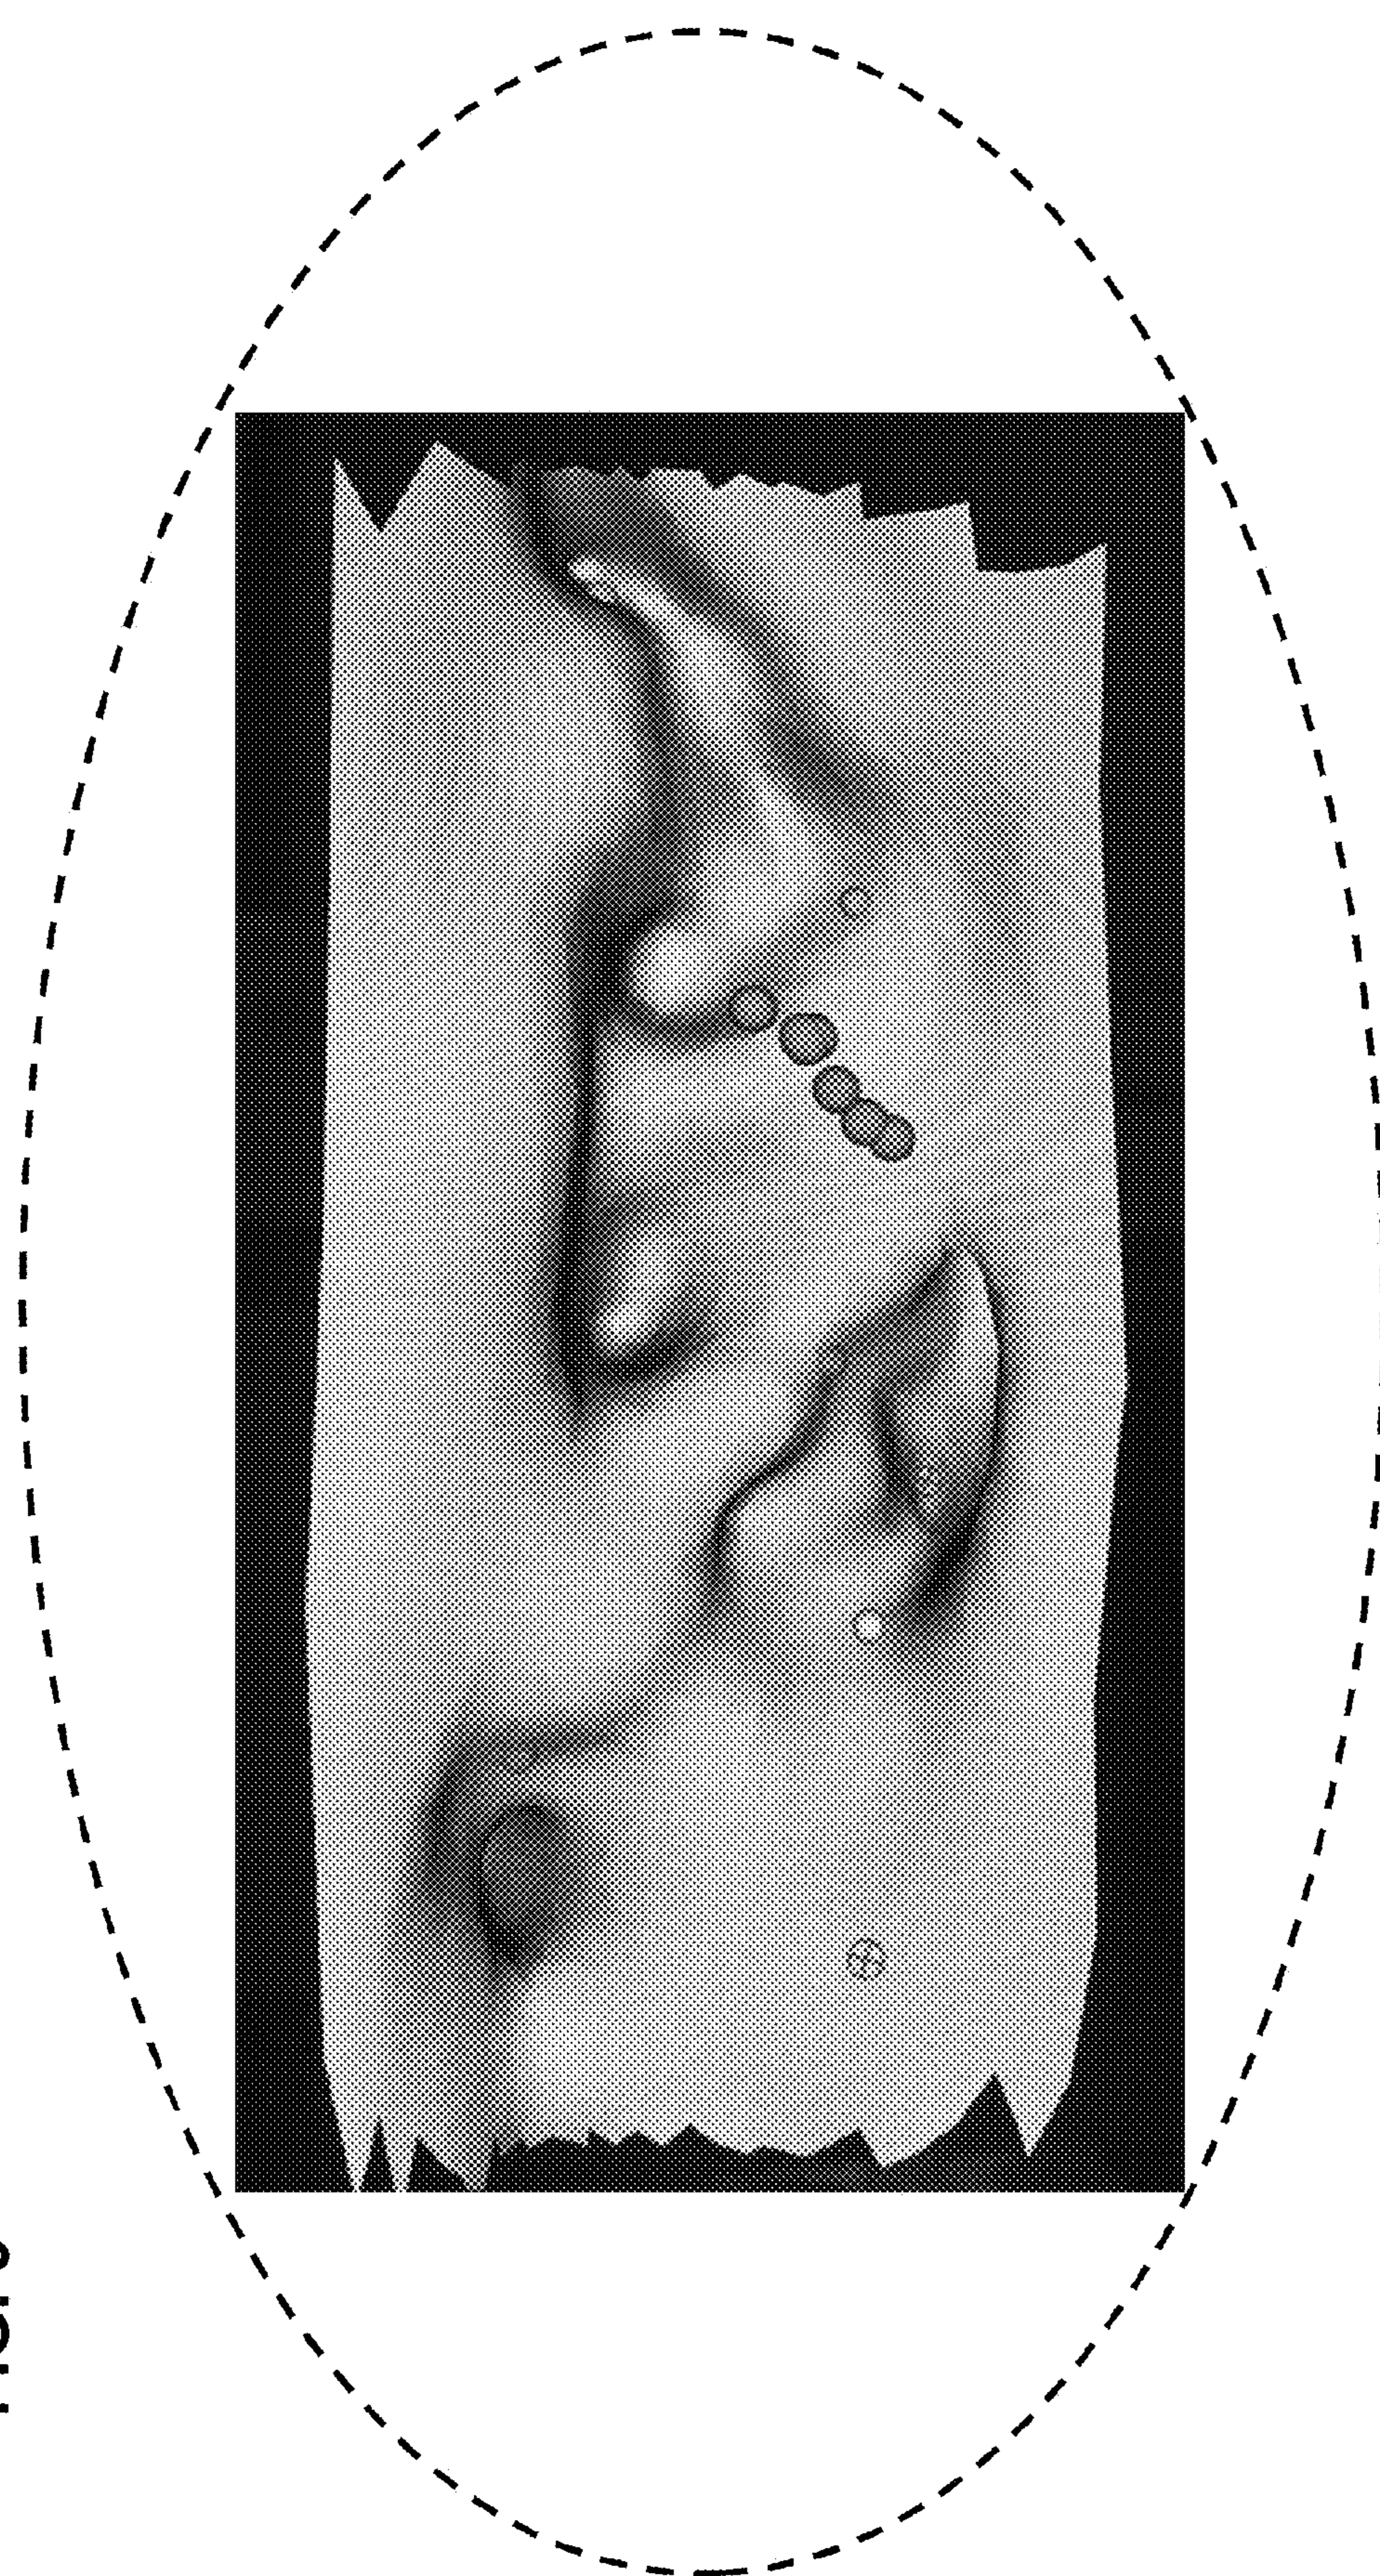


FIG. 5