US00D985115S

# (12) United States Design Patent

Wood

(10) Patent No.: US D985,115 S
(45) Date of Patent: ** May 2, 2023

(54) **SLEEP APNEA NASAL PILLOWS DEVICE**

(71) Applicant: **REMSleep Holdings Inc**, Tampa, FL (US)

(72) Inventor: **Thomas Jackson Wood**, Waycross, GA (US)

(73) Assignee: **REMSleep Holdings Inc.**, Tampa, FL (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/763,547**

(22) Filed: **Dec. 23, 2020**

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 15/595,990, filed on May 16, 2017, now Pat. No. 10,987,481.

(51) **LOC (14) Cl.** ..... **29-02**

(52) **U.S. Cl.**
USPC ..... **D24/110.4**; D24/110.1

(58) **Field of Classification Search**
USPC ..... D24/106, 108, 110, 110.1, 110.4, 110.5, D24/121, 127–129, 164, 184, 231
CPC ..... A61M 16/0683; A61M 16/0875; A61M 16/0666; A61M 16/0605; A61M 16/0611; A61M 16/208; A61M 2205/42; A62B 23/06
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|---|---|---|---|---|
| D612,933 | S * | 3/2010 | Prentice | D24/110.4 |
| D664,639 | S * | 7/2012 | Hoke | D24/108 |
| D674,480 | S * | 1/2013 | Prentice | D24/110.4 |
| D687,539 | S * | 8/2013 | Matula, Jr. | D24/110.1 |
| D746,468 | S * | 12/2015 | Meadows | D24/106 |
| 9,901,700 | B2 * | 2/2018 | McAuley | A61M 16/0611 |
| D863,540 | S * | 10/2019 | Collazo | D24/110.1 |
| D868,240 | S * | 11/2019 | Collazo | D24/110.1 |
| D878,545 | S * | 3/2020 | Scheiner | D24/110 |
| 10,987,481 | B2 * | 4/2021 | Wood | A61M 16/0683 |
| 2006/0283461 | A1 | 12/2006 | Lubke et al. | |

(Continued)

FOREIGN PATENT DOCUMENTS

| | | | |
|---|---|---|---|
| EM | 000683396-0001 | * | 5/2007 |
| JP | D1430470 | * | 12/2011 |

OTHER PUBLICATIONS

ResMed Nasal Pillow. Jun. 6, 2017. Site visited Dec. 3, 2022. [https://www.amazon.com/ResMed-AirFit-Nasal-Pillows-Cushions/dp/B01N0SXUC4/ref=sr_1_2?keywords=sleep+apnea+nasal+pillow&qid=1670122899&sprefix=sleep+apnea+nasal%2Caps%2C152&sr=8-2] (Year: 2017).*

(Continued)

*Primary Examiner* — Wendy L Arminio
*Assistant Examiner* — Maheen Khurshid
(74) *Attorney, Agent, or Firm* — Larson & Larson, P.A.; Frank Liebenow; Justin P. Miller

(57) **CLAIM**


The ornamental design for a sleep apnea nasal pillows device, as shown and described.

**DESCRIPTION**

FIG. **1** is a perspective view of a sleep apnea nasal pillows device showing my new design;
FIG. **2** is a top plan view thereof;
FIG. **3** is a bottom plan elevation view thereof;
FIG. **4** is a right-side elevation view thereof;
FIG. **5** is a left-side elevation view thereof;
FIG. **6** is a front elevation view thereof; and,
FIG. **7** is a rear elevation view thereof.

The dash-dash broken lines in the drawings depict portions of the sleep apnea nasal pillows device that form no part of the claimed design. The dot-dash broken lines in the drawings depict boundaries of the claimed design and form no part thereof.

**1 Claim, 6 Drawing Sheets**

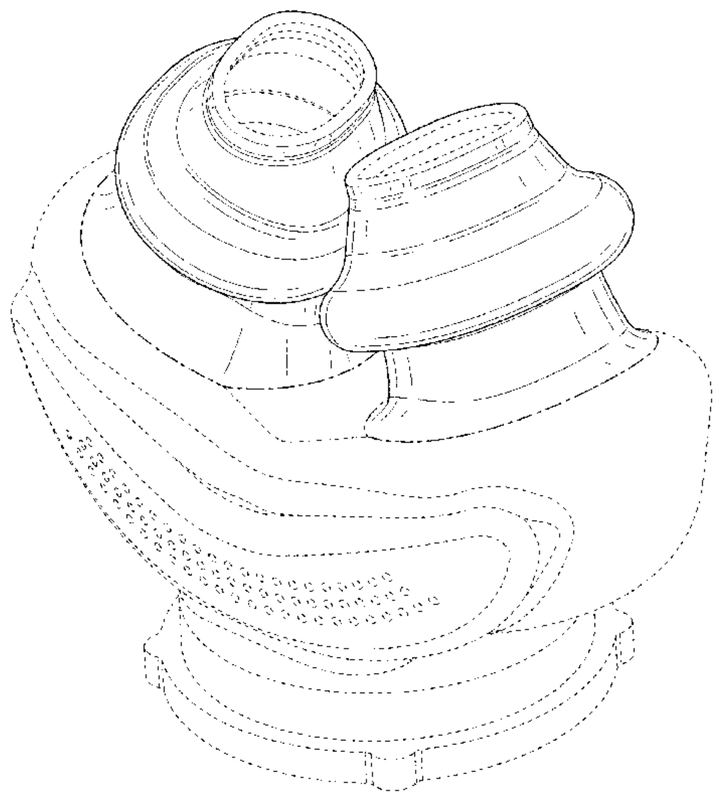

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|---|---|---|---|---|
| 2016/0015921 | A1 | 1/2016 | Harrison et al. | |
| 2017/0143926 | A1* | 5/2017 | Allum | A61M 16/0816 |
| 2017/0368285 | A1* | 12/2017 | Wood | A61M 16/0683 |
| 2018/0078725 | A1 | 3/2018 | Richardson et al. | |
| 2021/0213229 | A1* | 7/2021 | Wood | A61M 16/0666 |

OTHER PUBLICATIONS

Swift FX Pillow—Small by ResMed. Sep. 5, 2011. Site visited Dec. 3, 2022. [https://www.amazon.com/Swift-FX-Nasal-Pillow-Small/dp/B005LAPE0K/ref=sr_1_69?keywords=sleep+apnea+nasal+pillow&qid=1670123402&sprefix=sleep+apnea+nasal%2Caps%2C152&sr=8-69] (Year: 2011).*

Philips Respironics. Sep. 19, 2018. Site visited Dec. 3, 2022. [https://www.amazon.com/Philips-Respironics-Nuance-Replacement-Pillows/dp/B07DGFH9MD/ref=sr_1_4?crid=2YHXIHO3Y7Q2E&keywords=nasal+pillow&qid=1670123733&sprefix=nasal+pillow%2Caps%2C85&sr=8-4] (Year: 2018).*

* cited by examiner

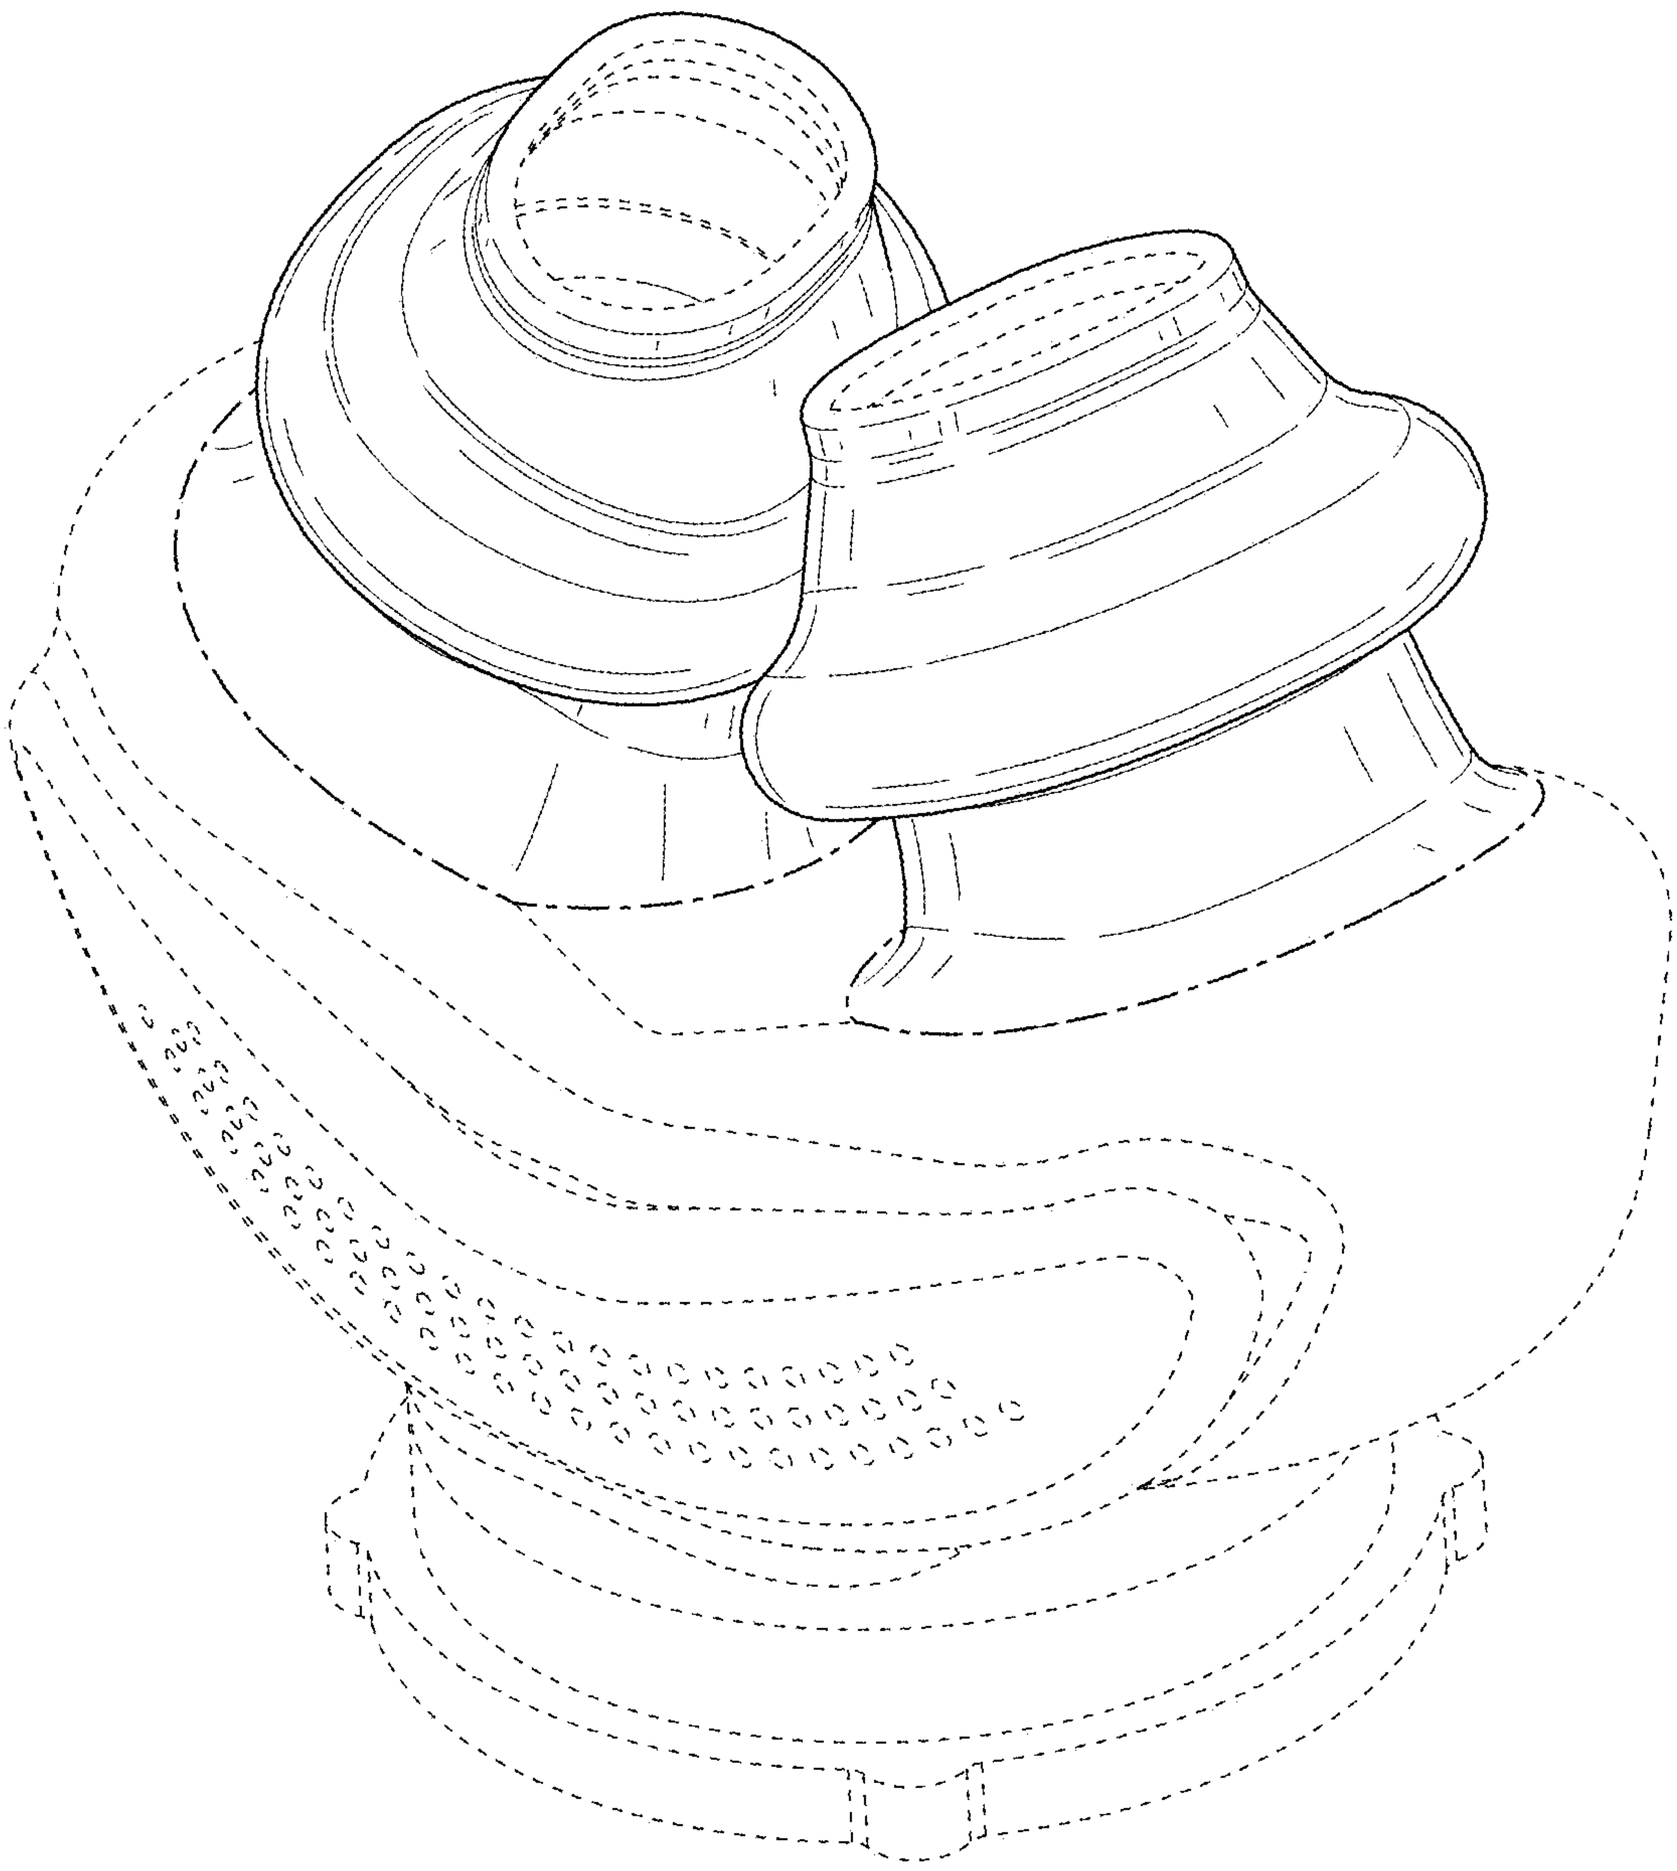


FIG. 1

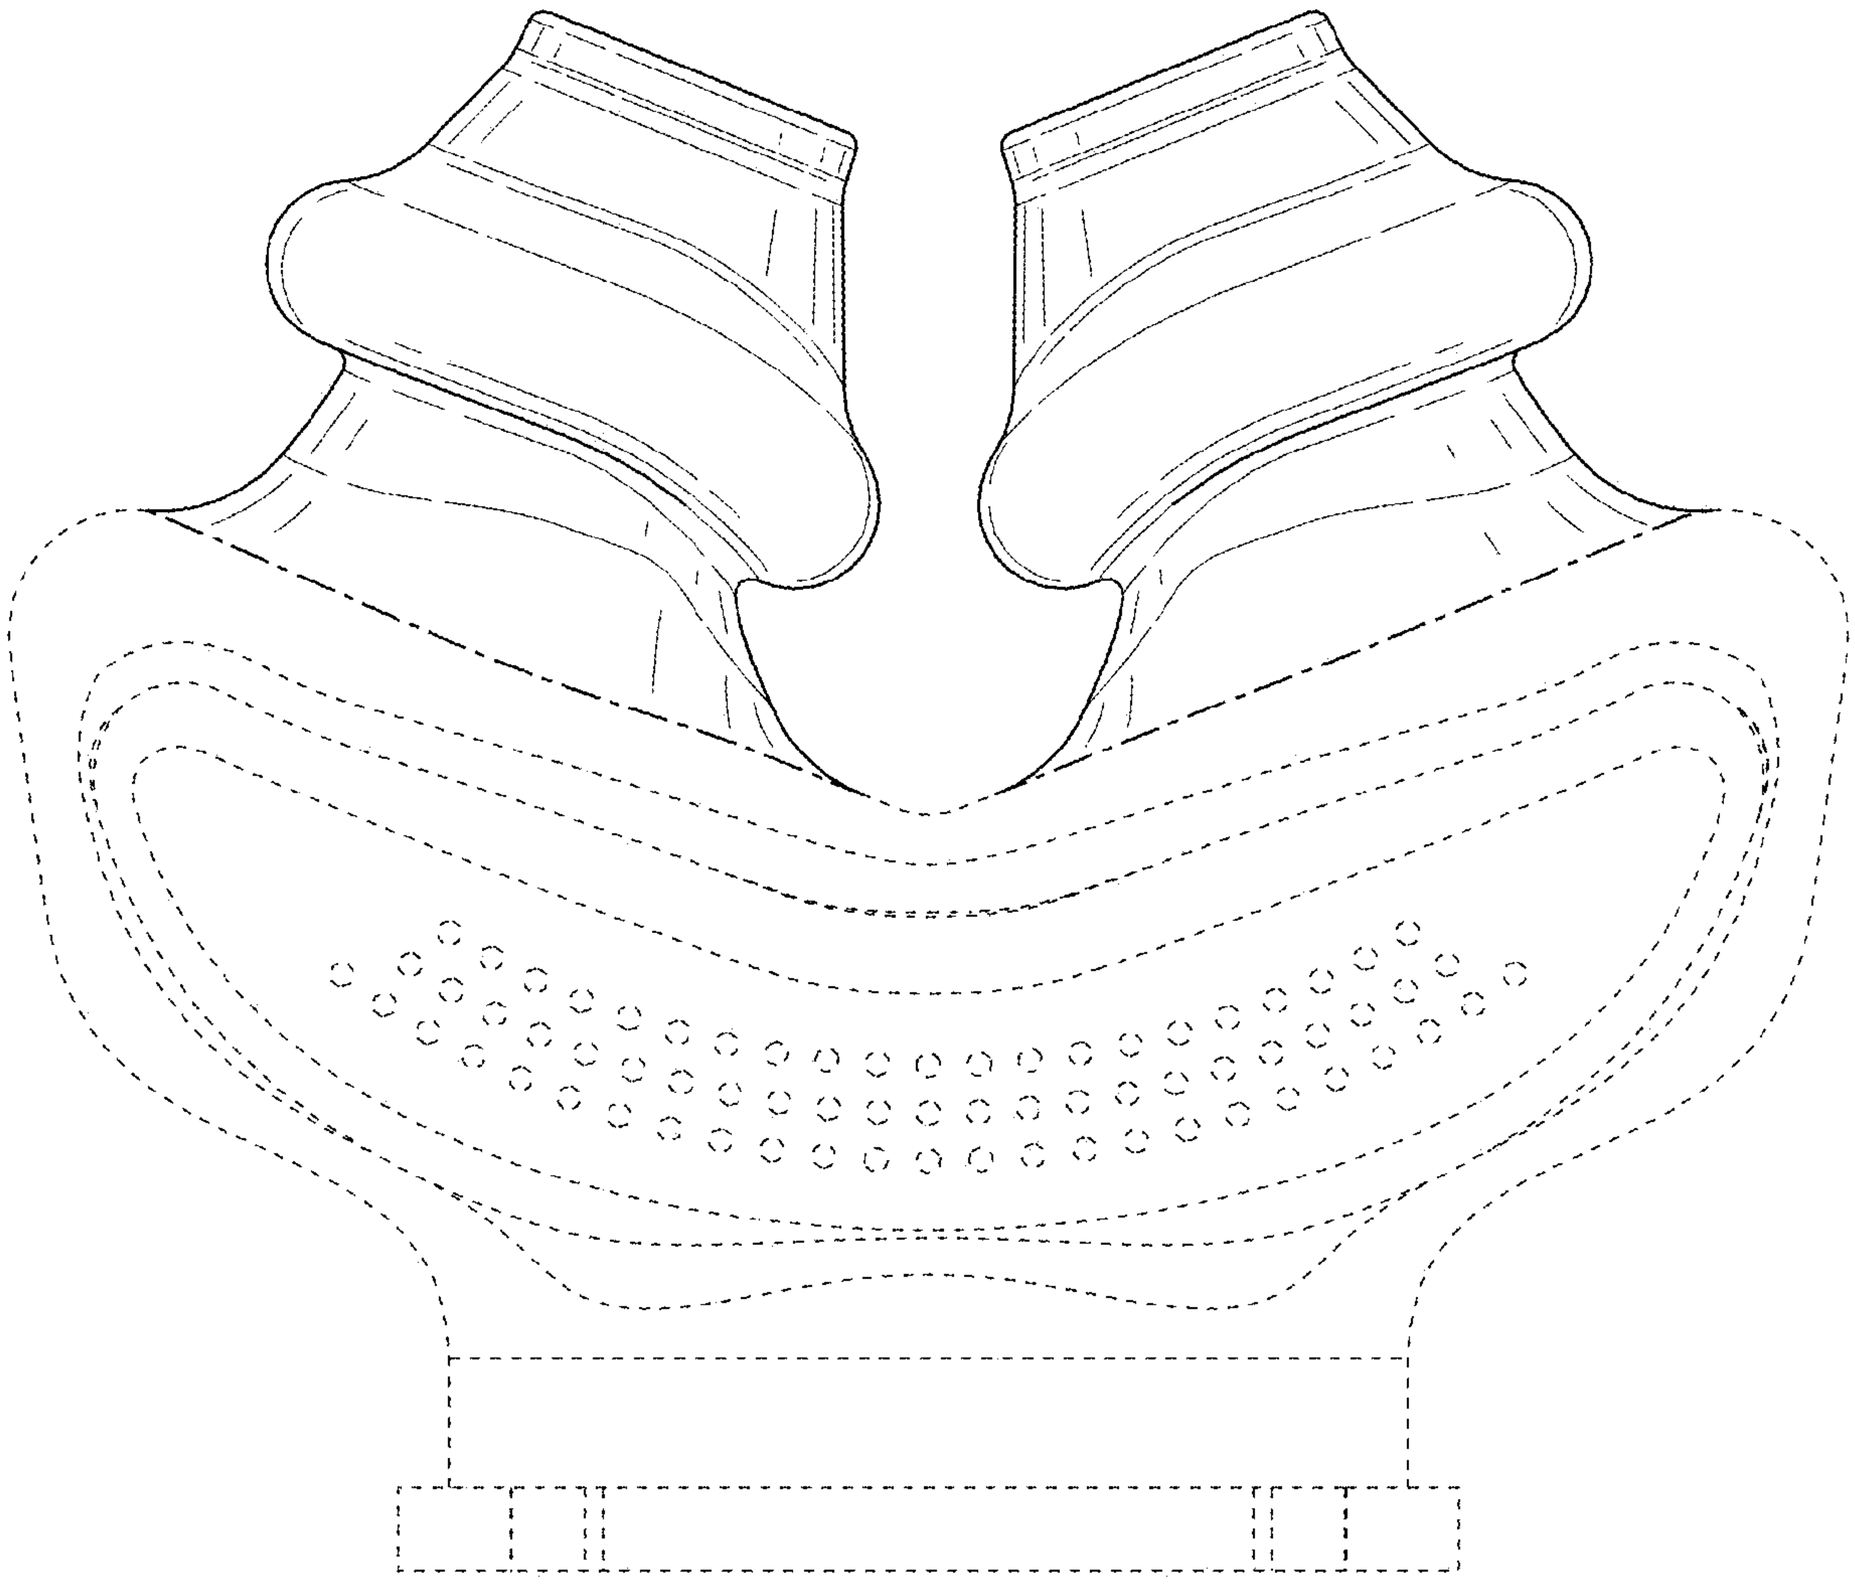


FIG. 2

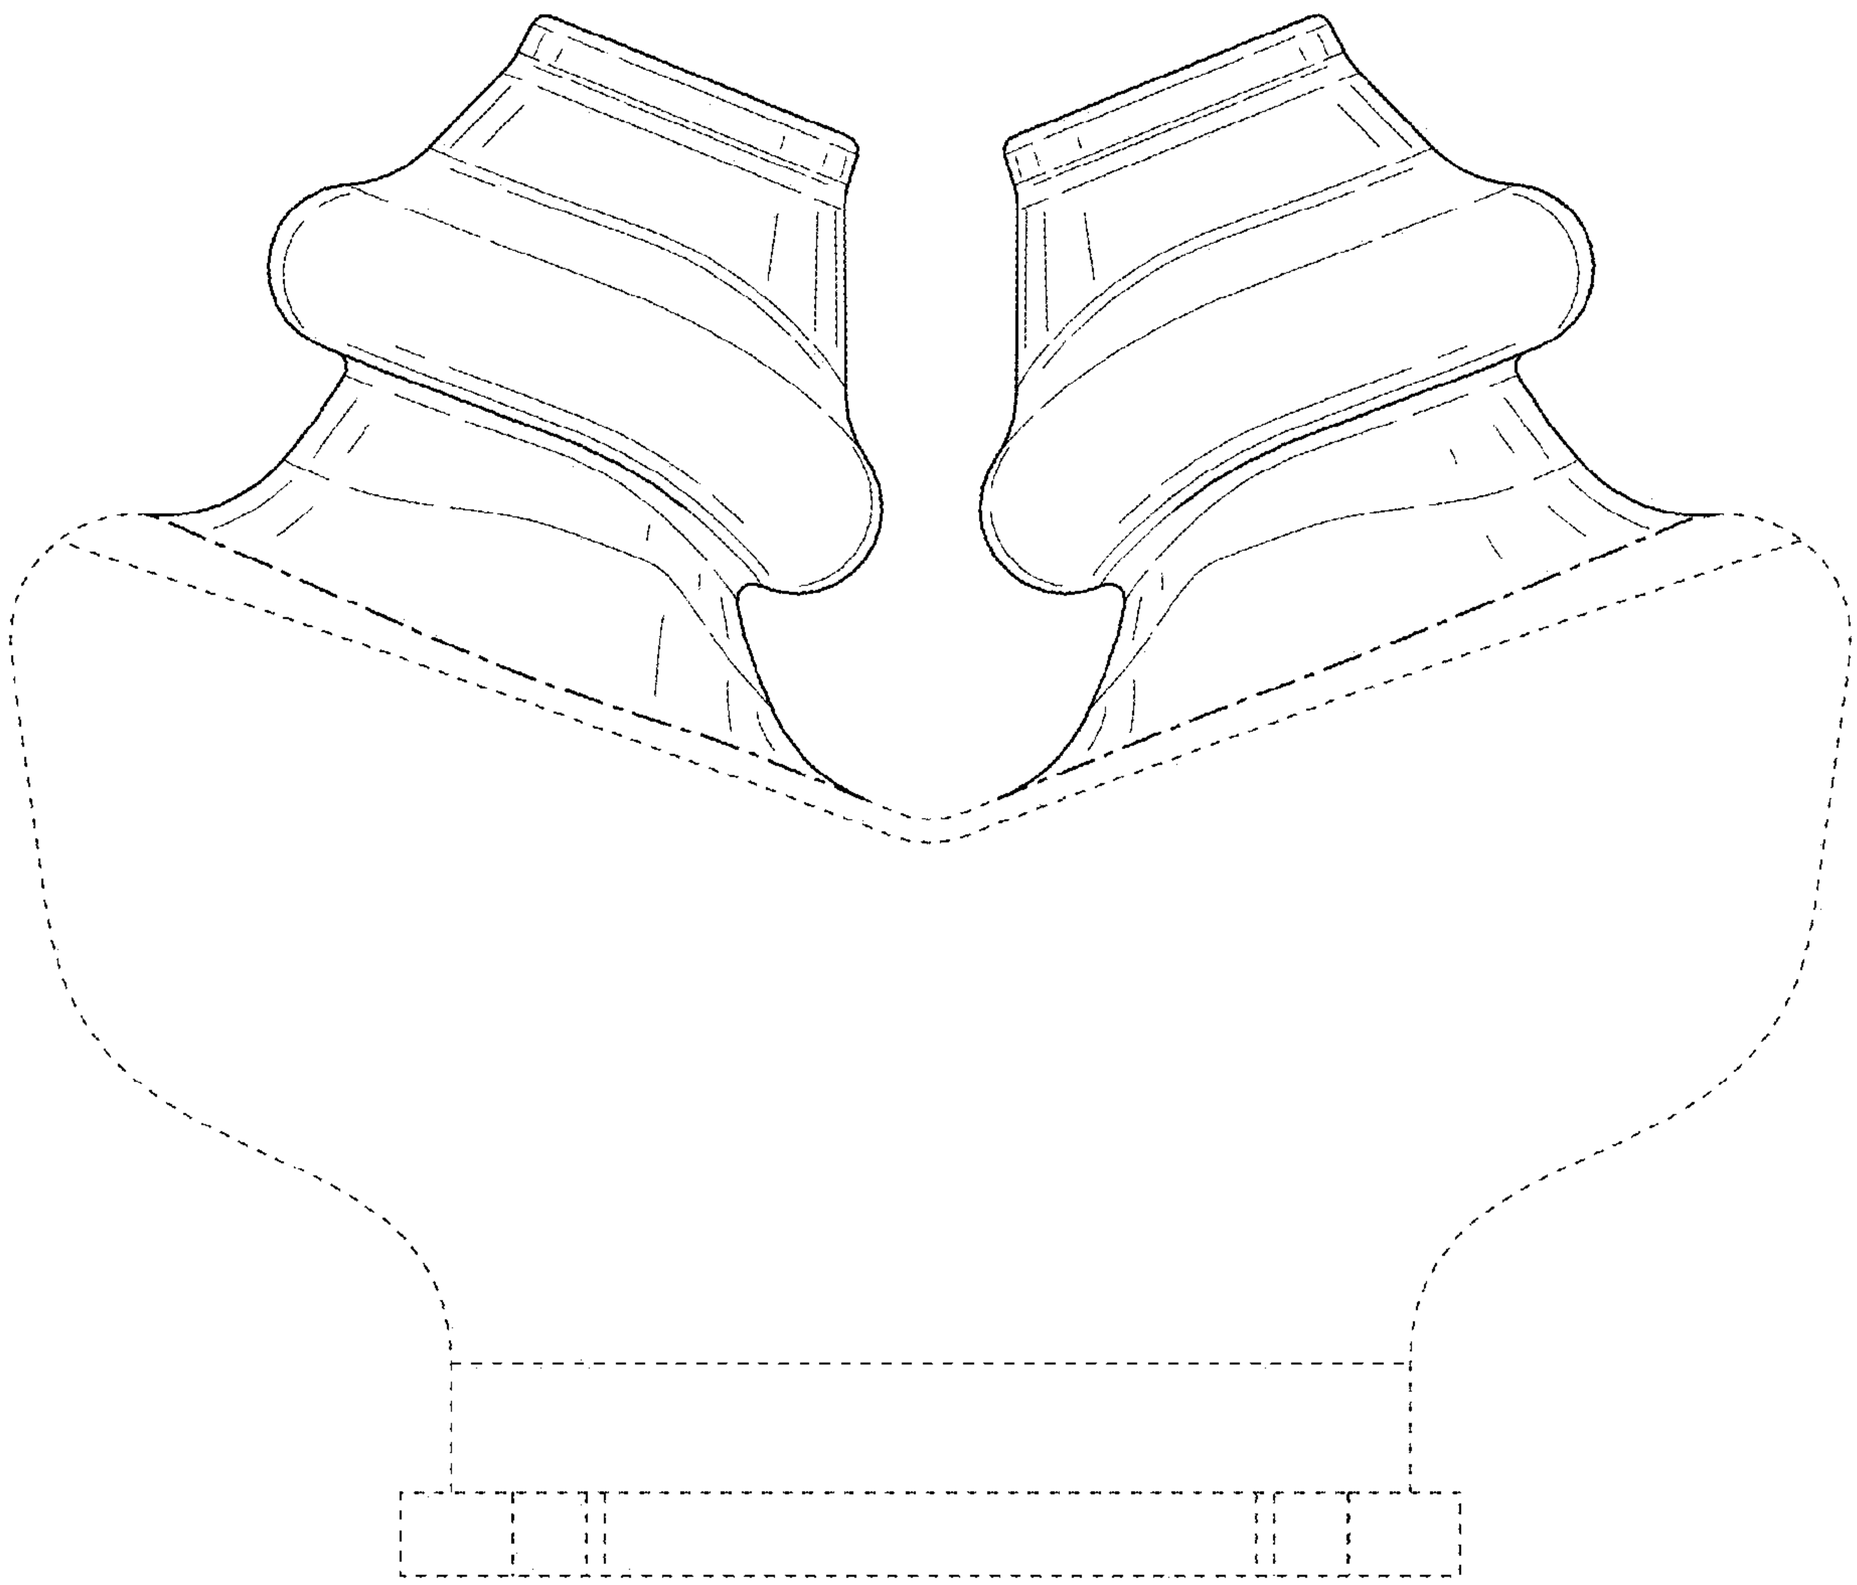


FIG. 3

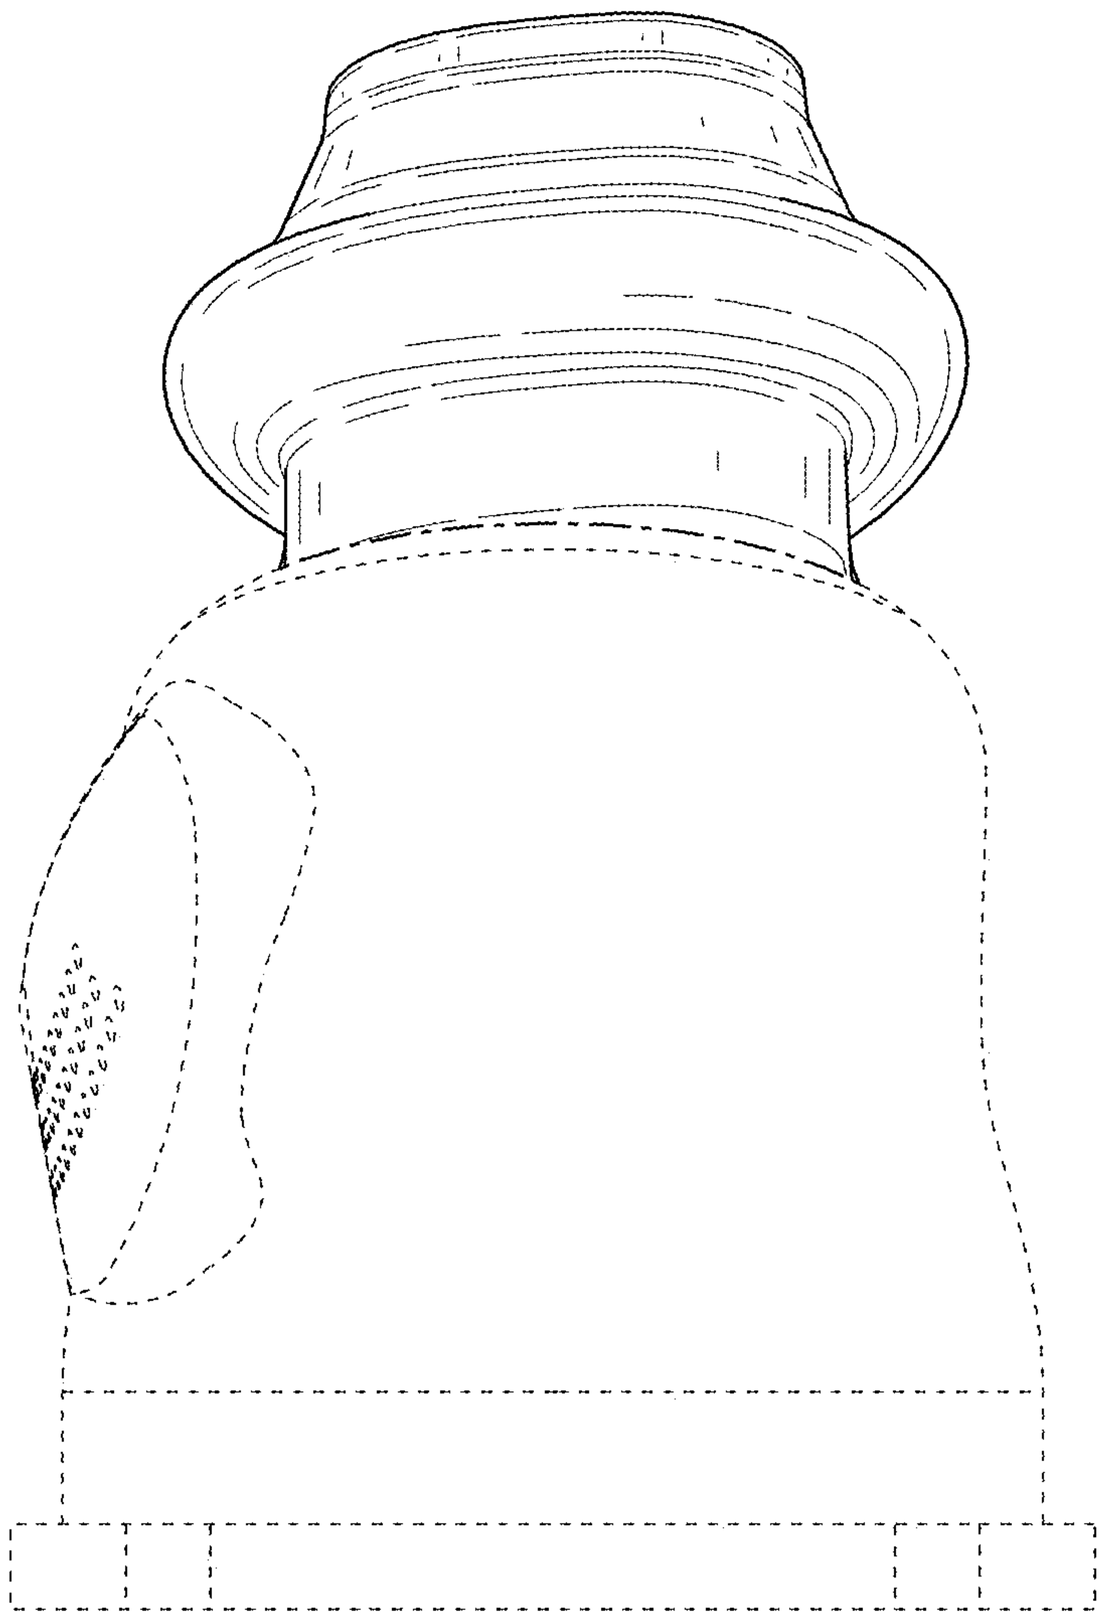


FIG. 4

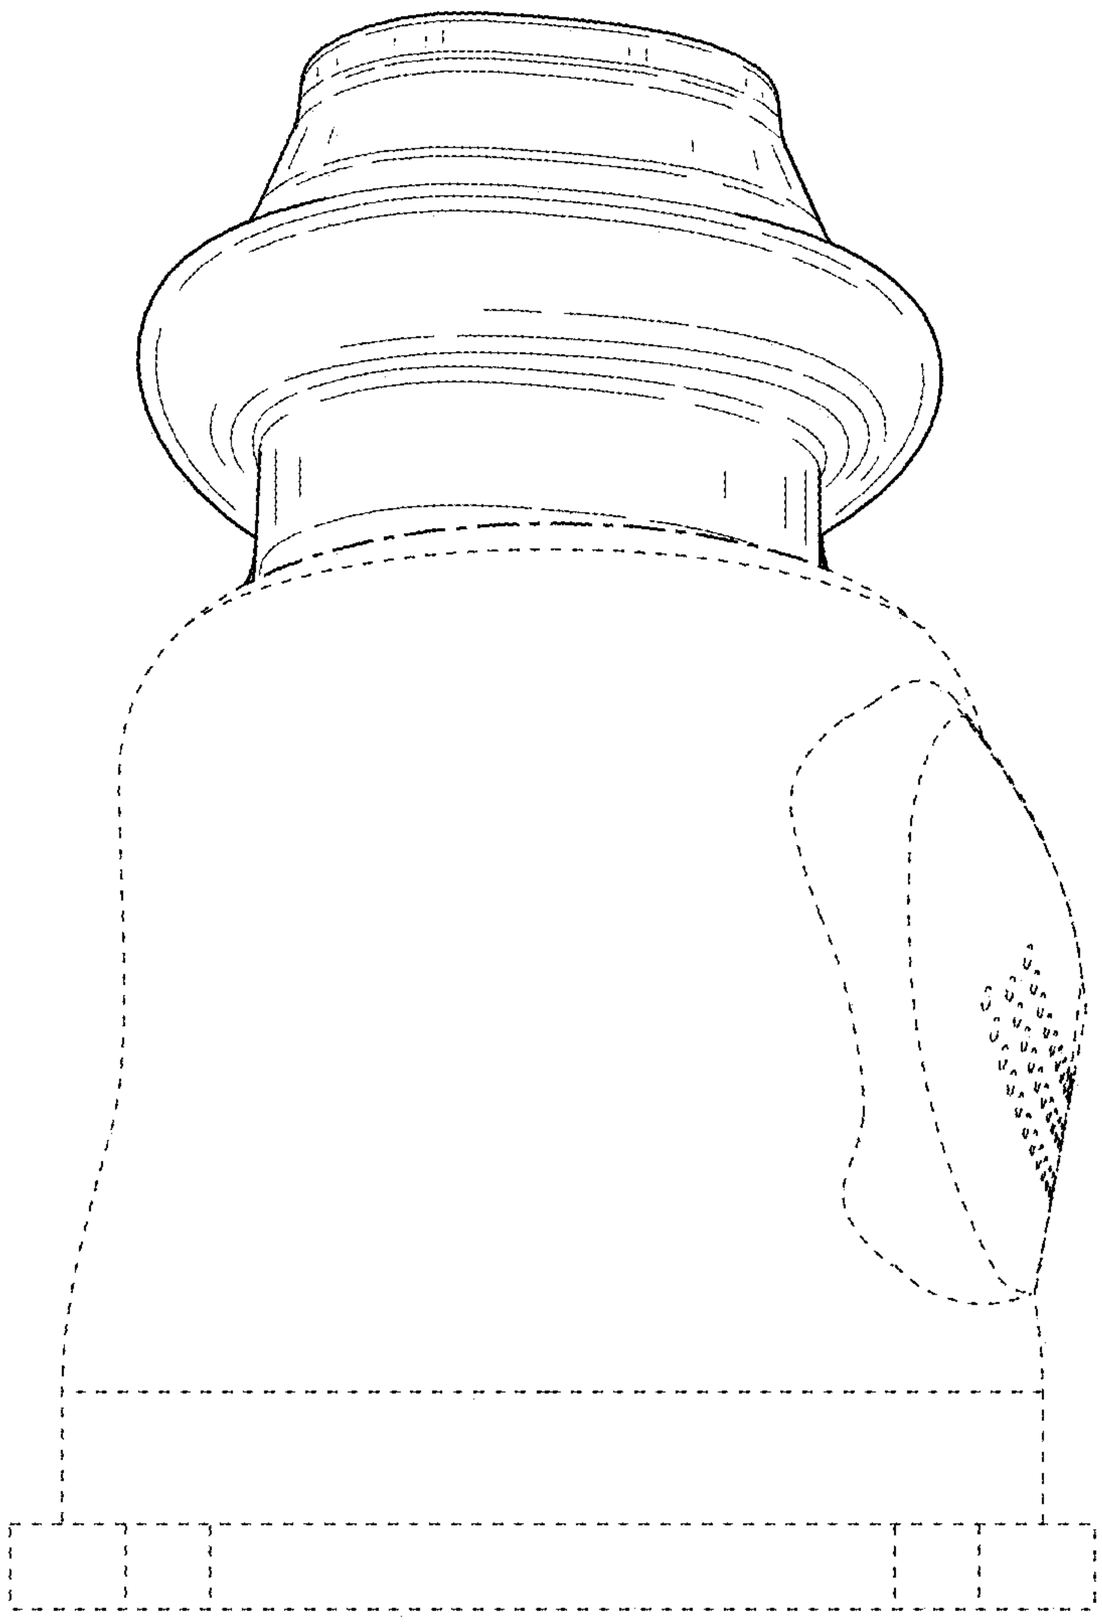


FIG. 5

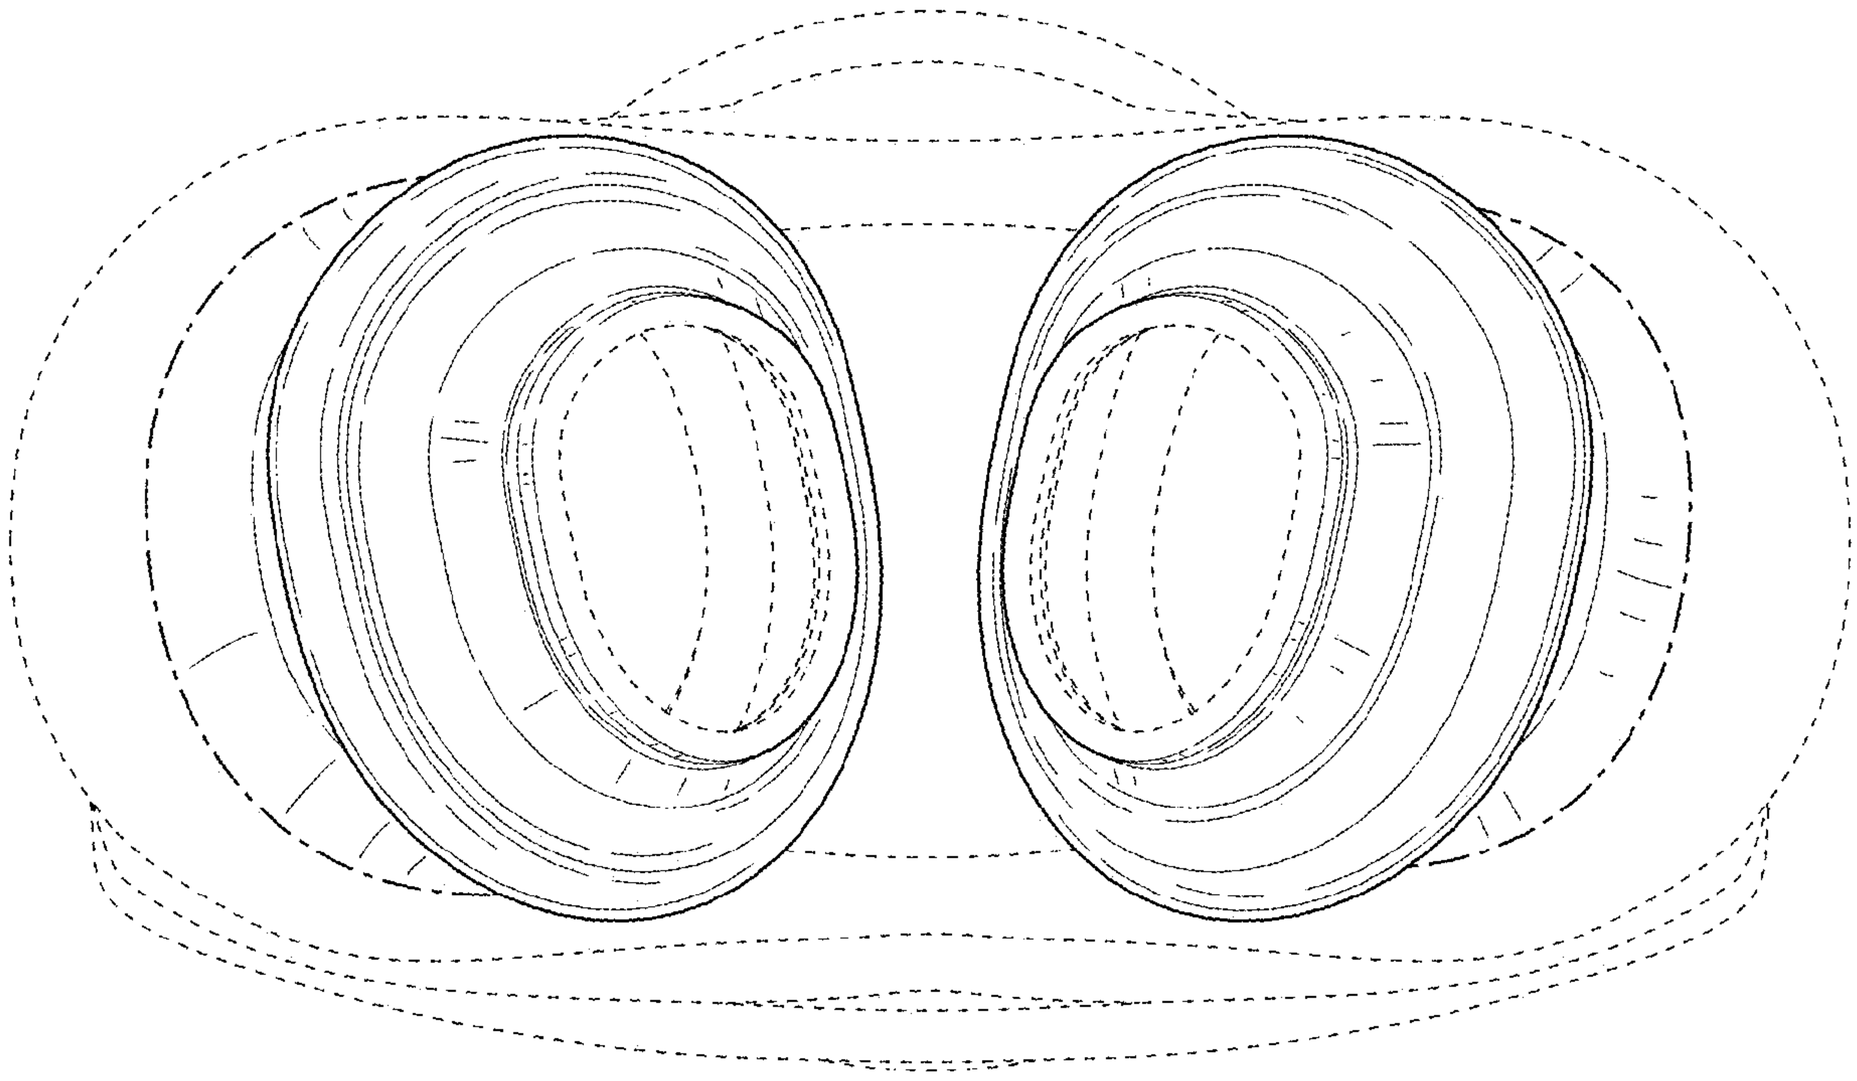


FIG. 6

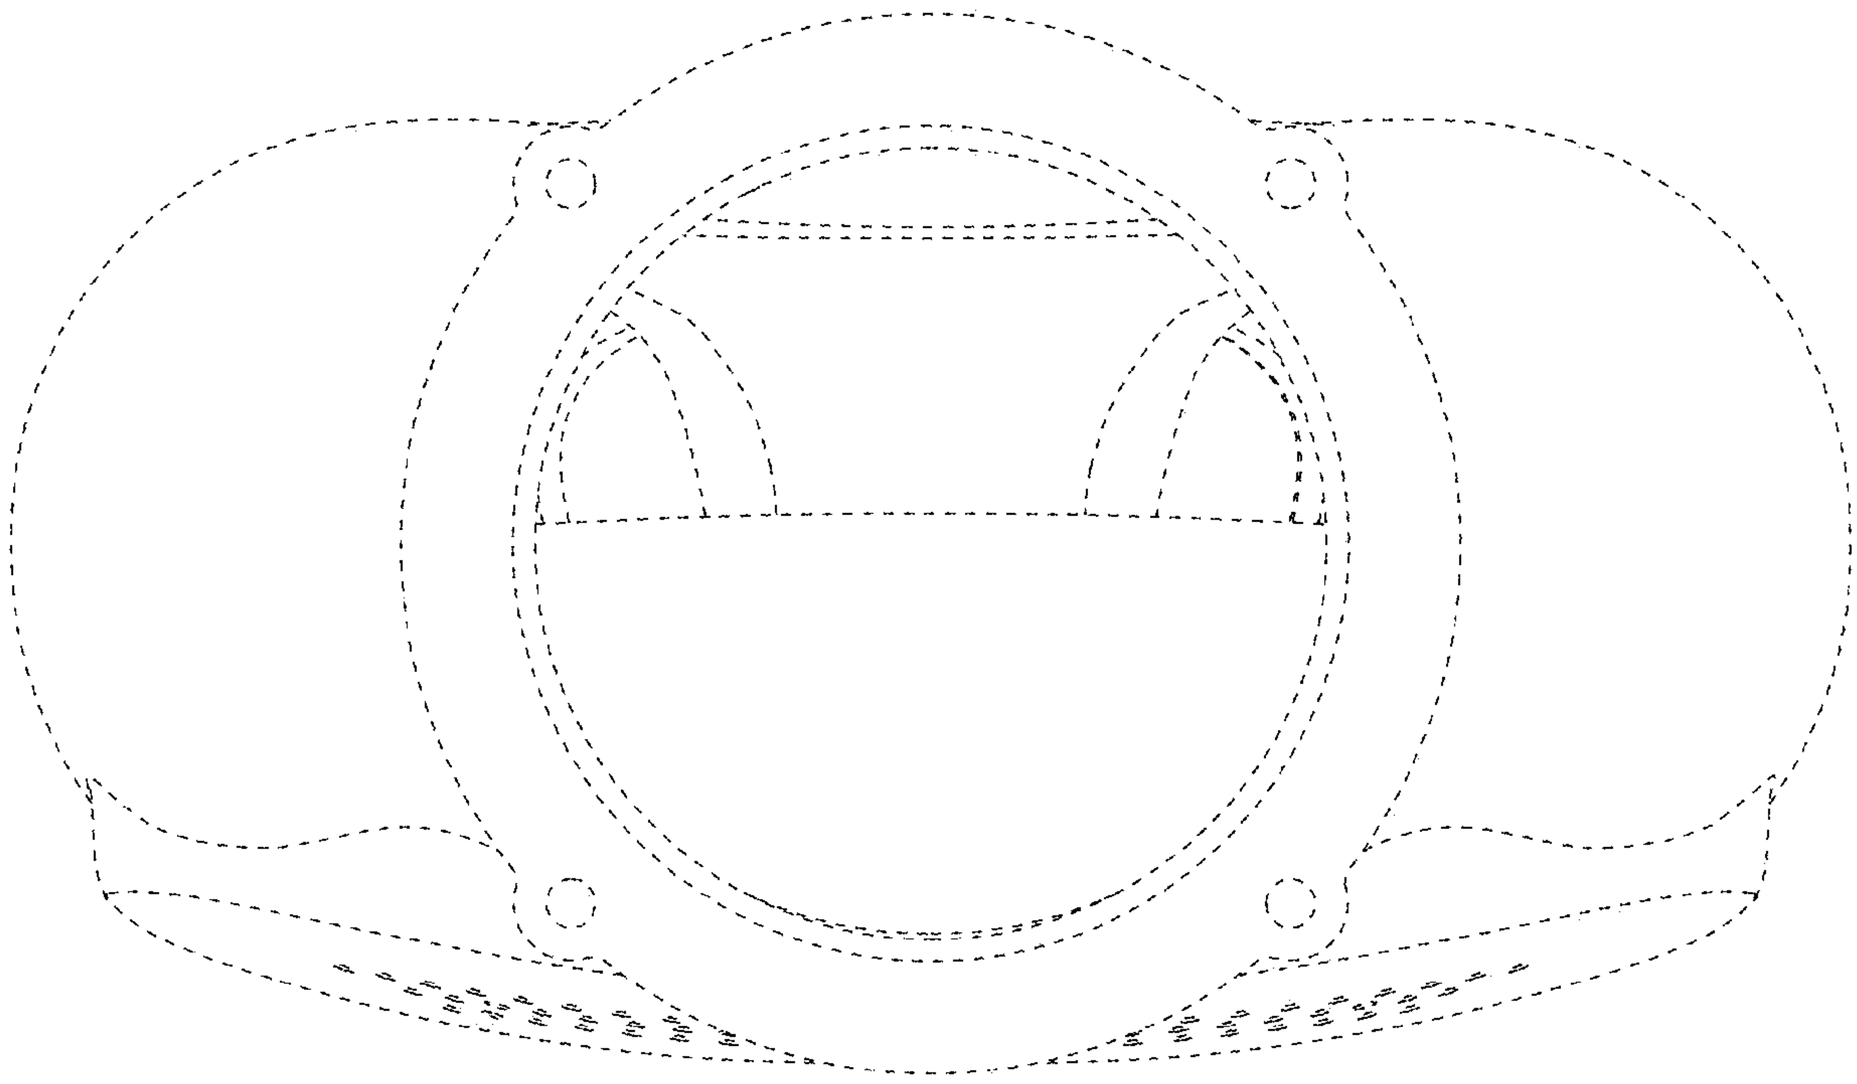


FIG. 7