



US00D985588S

(12) **United States Design Patent** (10) **Patent No.:** **US D985,588 S**
Farlow et al. (45) **Date of Patent:** **** May 9, 2023**

(54) **DISPLAY SCREEN WITH A GRAPHICAL USER INTERFACE FOR AN ENDOSCOPE PITCH INDICATOR**

(71) Applicant: **Covidien LP**, Mansfield, MA (US)
(72) Inventors: **Jared N. Farlow**, Los Angeles, CA (US); **Robert J. Stephens**, Superior, CO (US); **Elizabeth Lauren Lu**, Somerville, MA (US); **Edbert C. Wang**, Long Island City, NY (US); **Margaret A. Jacobi**, Waban, MA (US); **Sonya H. Mead**, Newton, MA (US); **Tara M. Kovalik**, Arlington, MA (US); **Leslie Johnston**, Hyde Park, MA (US)

(73) Assignee: **Covidien LP**, Mansfield, MA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/804,274**

(22) Filed: **Aug. 19, 2021**

Related U.S. Application Data

(63) Continuation of application No. 17/427,679, filed as application No. PCT/US2021/034125 on May 26, 2021.

(51) **LOC (14) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485-95
CPC G06F 3/048; G06F 3/0481; G06F 3/04812; G06F 3/04815; G06F 3/04817; G06F 3/0482; G06F 3/0483; G06F 3/0484; G06F 3/04842; G06F 3/04845; G06F 3/04847; G06F 3/0485; G06F 3/0486; G06F 3/0487;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D428,399 S * 7/2000 Kahn D14/488
D492,696 S * 7/2004 Minagawa D14/491
D496,667 S * 9/2004 Høglund D14/491

(Continued)

FOREIGN PATENT DOCUMENTS

WO 2019204013 A1 10/2019
WO 2020214193 A1 10/2020
WO 2021030651 A1 2/2021

OTHER PUBLICATIONS

Custom Arrow Button—Kloep, <https://www.codeproject.com/Articles/11625/Custom-Arrow-Button> (Year: 2005).*

(Continued)

Primary Examiner — Melanie H Tung
Assistant Examiner — Darmawan Truong

(74) *Attorney, Agent, or Firm* — Carter, DeLuca & Farrell LLP

(57) **CLAIM**

The ornamental design for a display screen with a graphical user interface of an endoscope pitch indicator, substantially as shown and described.

DESCRIPTION

FIG. 1 is a front view of a first embodiment of a display screen with a graphical user interface for an endoscope pitch indicator;


FIG. 2 is a second embodiment thereof;

FIG. 3 is a third embodiment thereof; and,

FIG. 4 is a fourth embodiment thereof.

The broken lines showing the display screen form no part of the claimed design. The remaining broken lines showing portions of the graphical user interface form no part of the claimed design.

1 Claim, 4 Drawing Sheets

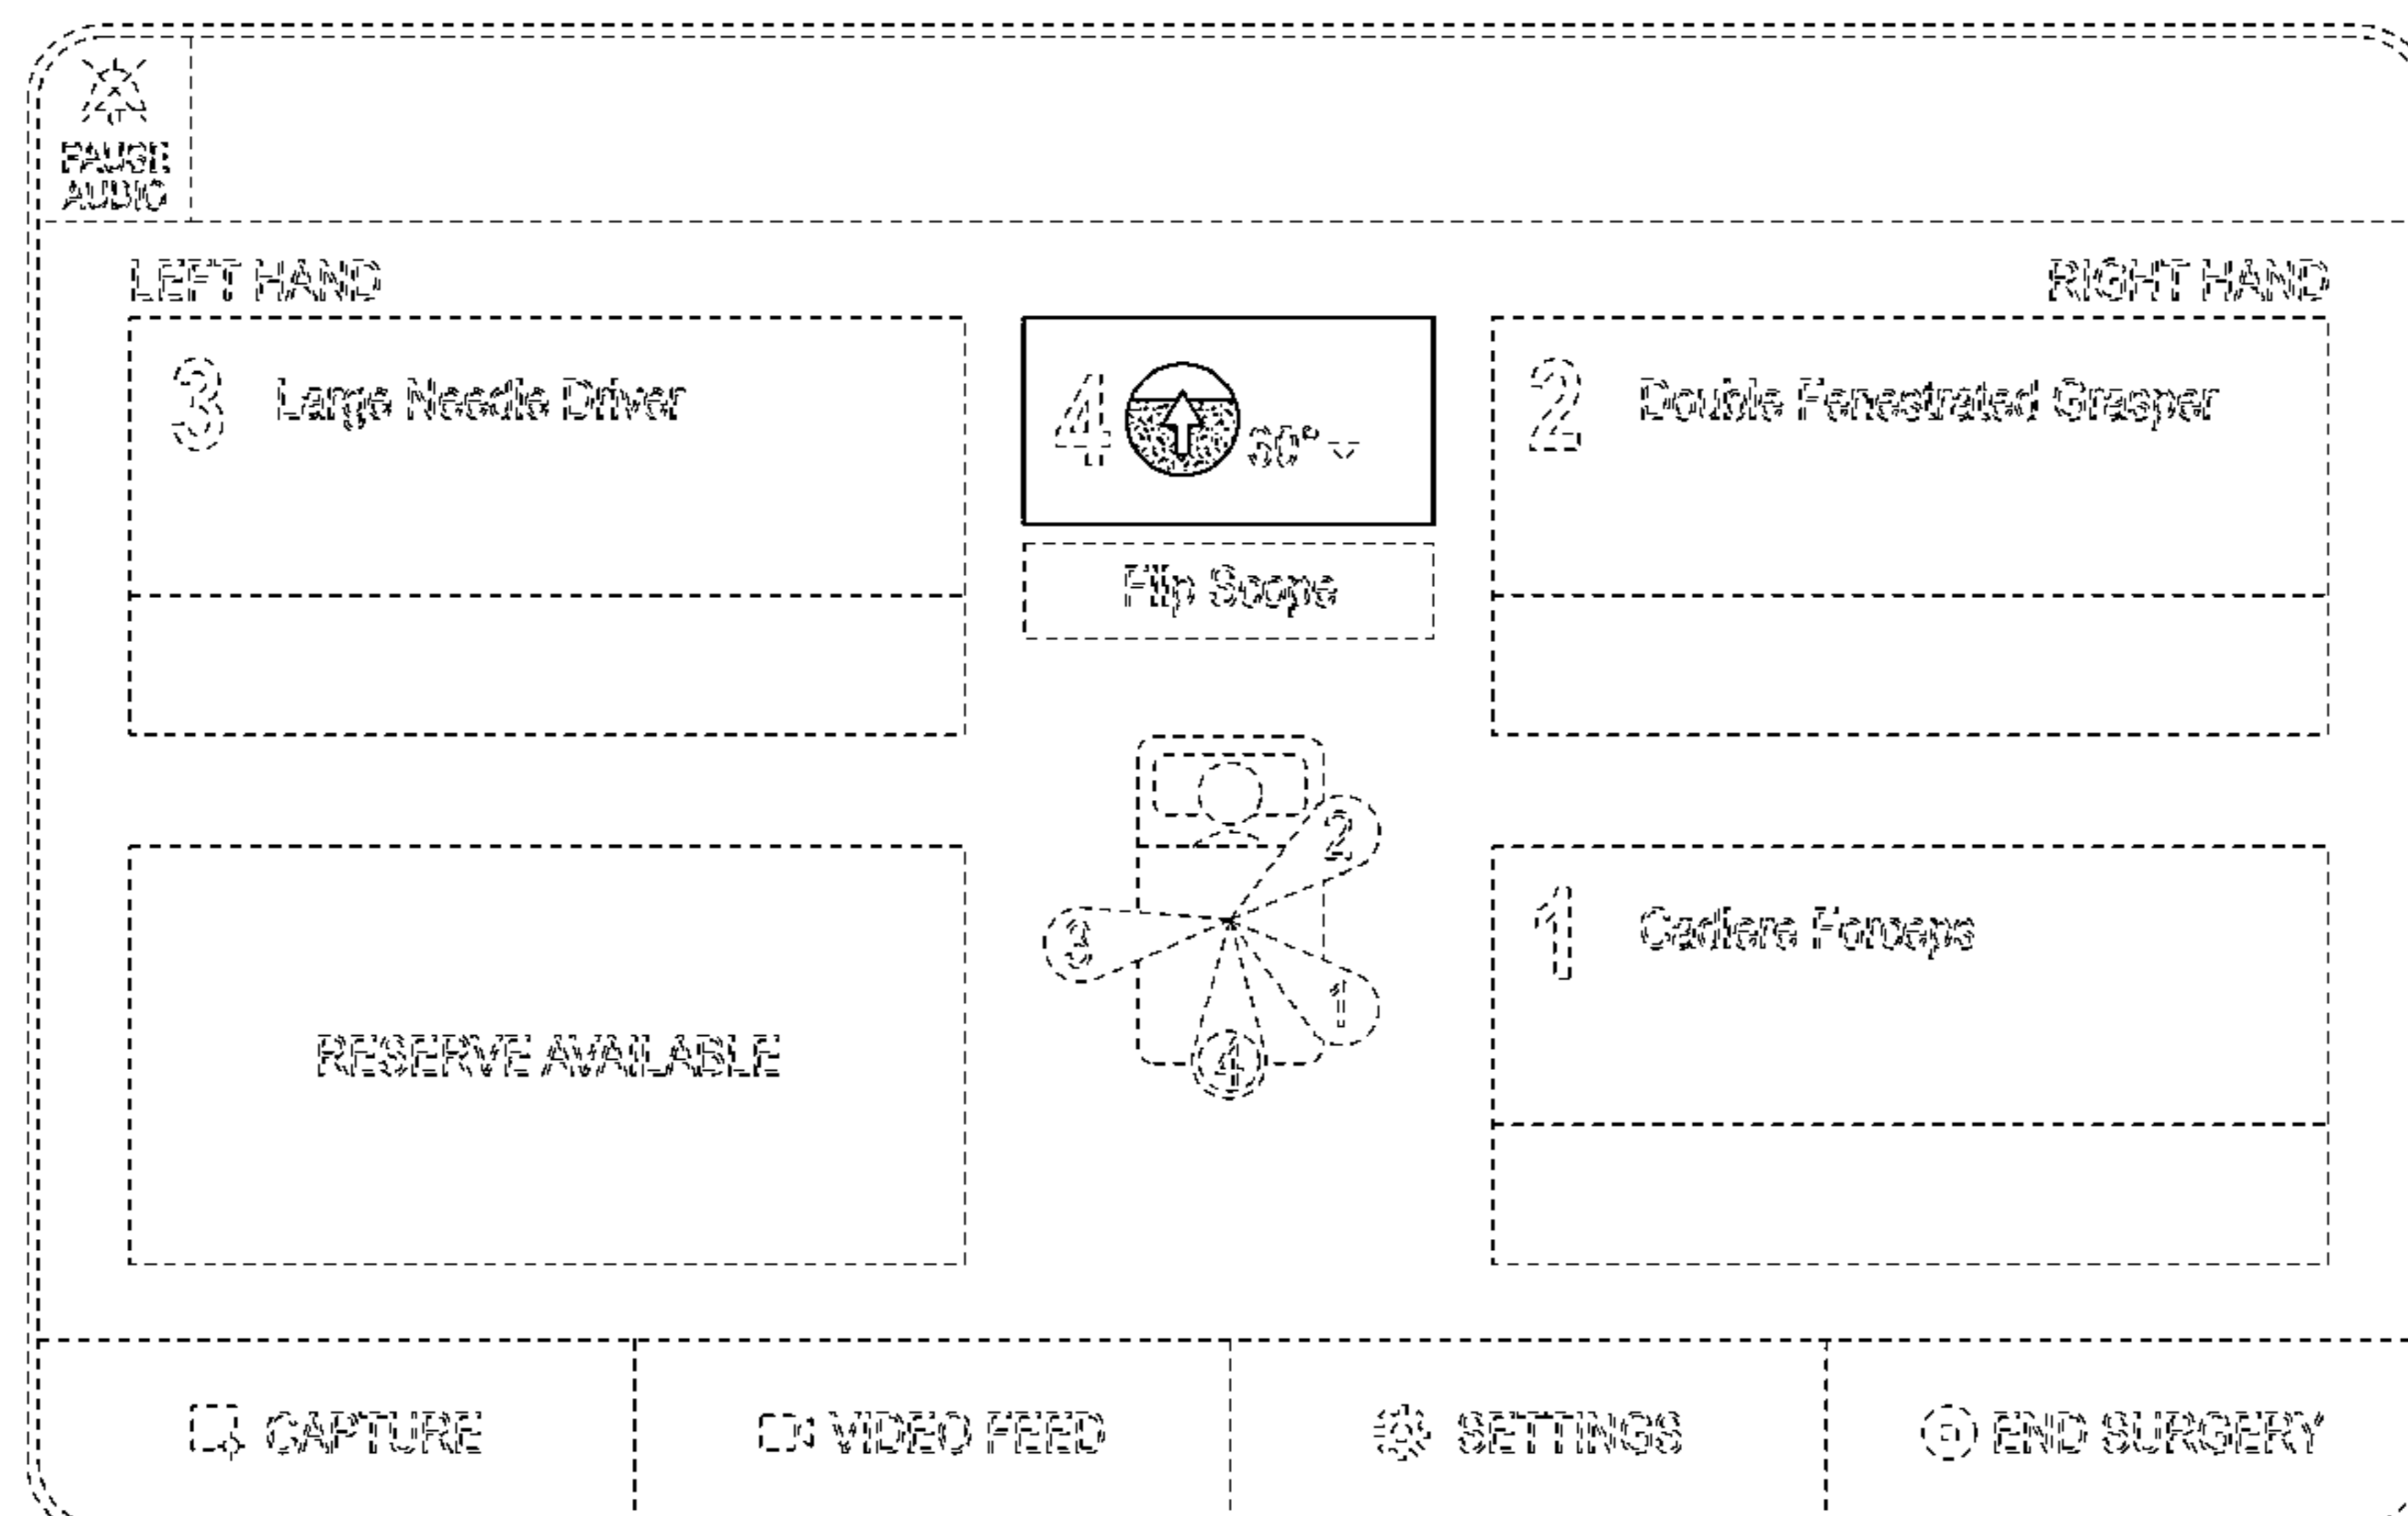

(58) **Field of Classification Search**

CPC G06F 3/0488; G06F 3/04883; G06F
3/04886

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D612,398	S	*	3/2010	Lemay	D14/491
D683,755	S	*	6/2013	Phelan	D14/489
D686,245	S	*	7/2013	Gardner	D14/491
D709,914	S	*	7/2014	Berdan	D14/491
D710,371	S	*	8/2014	van Os	D14/486
D711,910	S	*	8/2014	Inose	D14/489
D712,925	S	*	9/2014	Meegan	D14/489
D720,364	S	*	12/2014	Park	D14/486
D741,370	S	*	10/2015	Torres	D14/492
D751,579	S	*	3/2016	Hansing	D14/485
D757,043	S	*	5/2016	Zankowski	D14/485
D790,593	S	*	6/2017	Zhong	D14/491
D852,811	S	*	7/2019	Babion	D14/485
D876,456	S	*	2/2020	Broughton	D14/491
D888,097	S	*	6/2020	Butcher	D14/491
2002/0109737	A1	*	8/2002	Jaeger	G06F 3/0481 715/863
2003/0126166	A1	*	7/2003	Good	G06F 3/04892 708/520
2017/0079730	A1		3/2017	Azizian et al.		

OTHER PUBLICATIONS

Font Awesome 5 solid arrow circle right—Wikimedia, https://commons.wikimedia.org/wiki/File:Font_Awesome_5_solid_arrow-circle-right.svg (Year: 2018).*

International Search Report dated Nov. 5, 2021 issued in corresponding PCT Appln. No. PCT/US2021/034125.

* cited by examiner

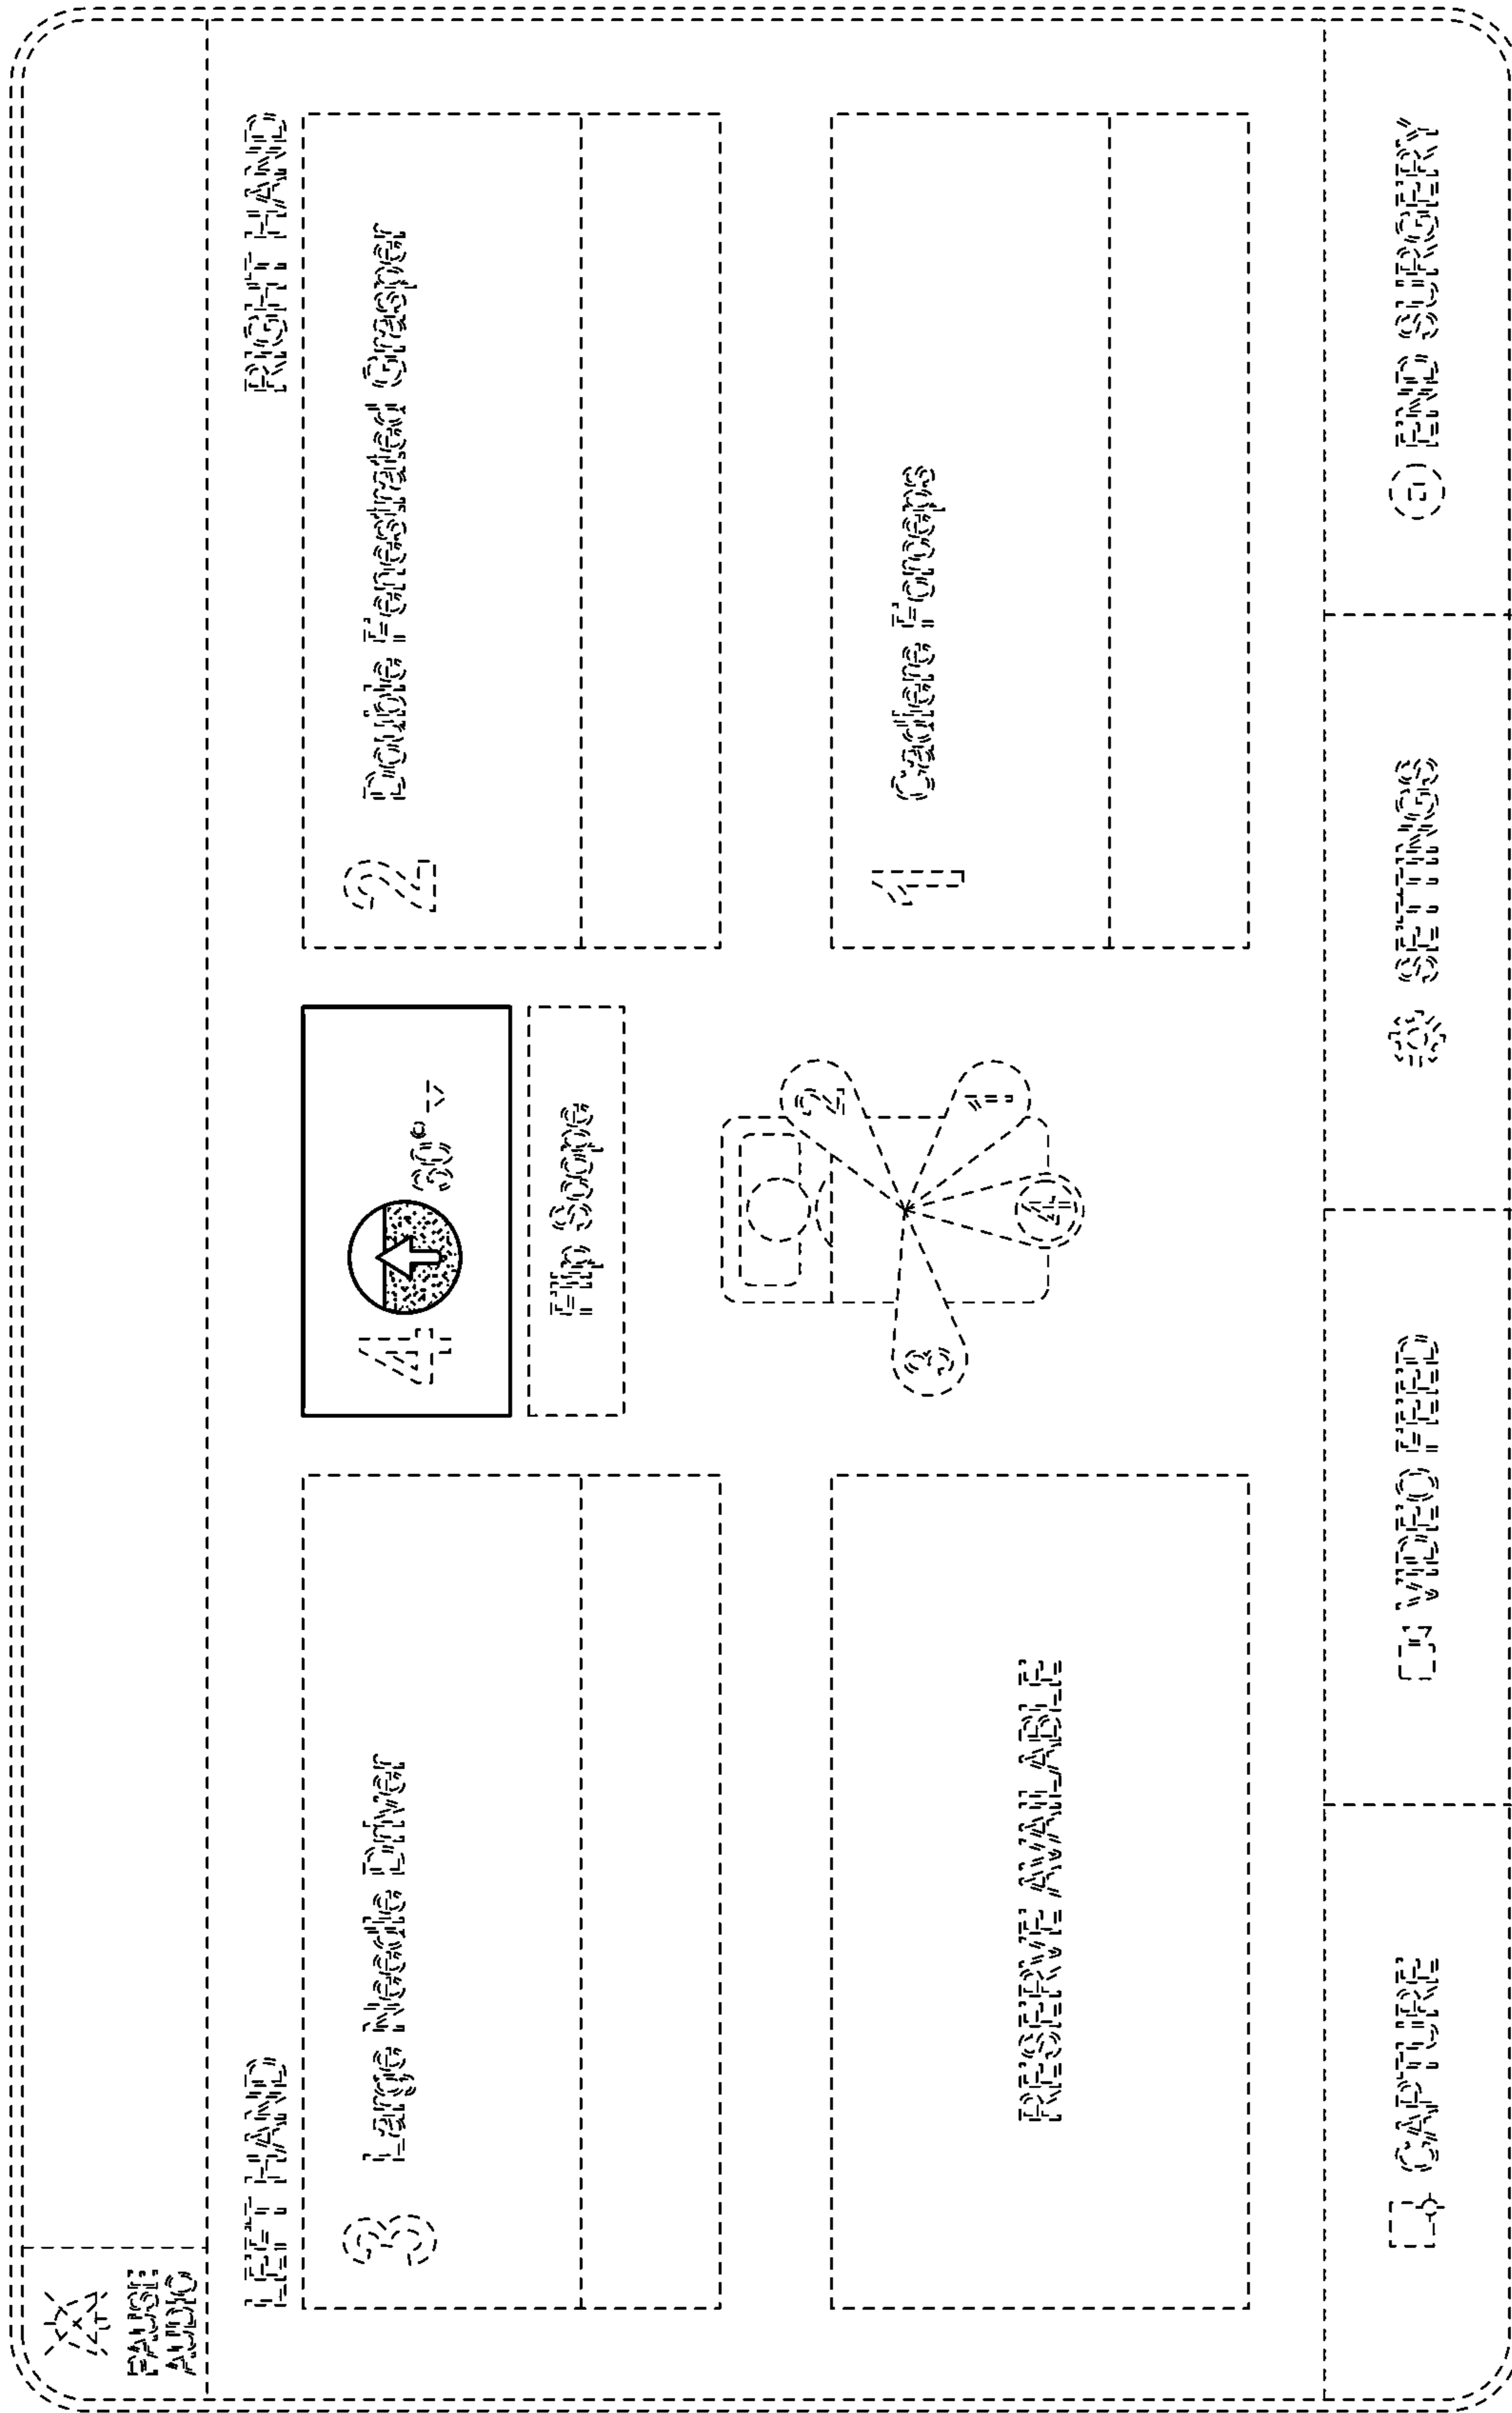


FIG. 1

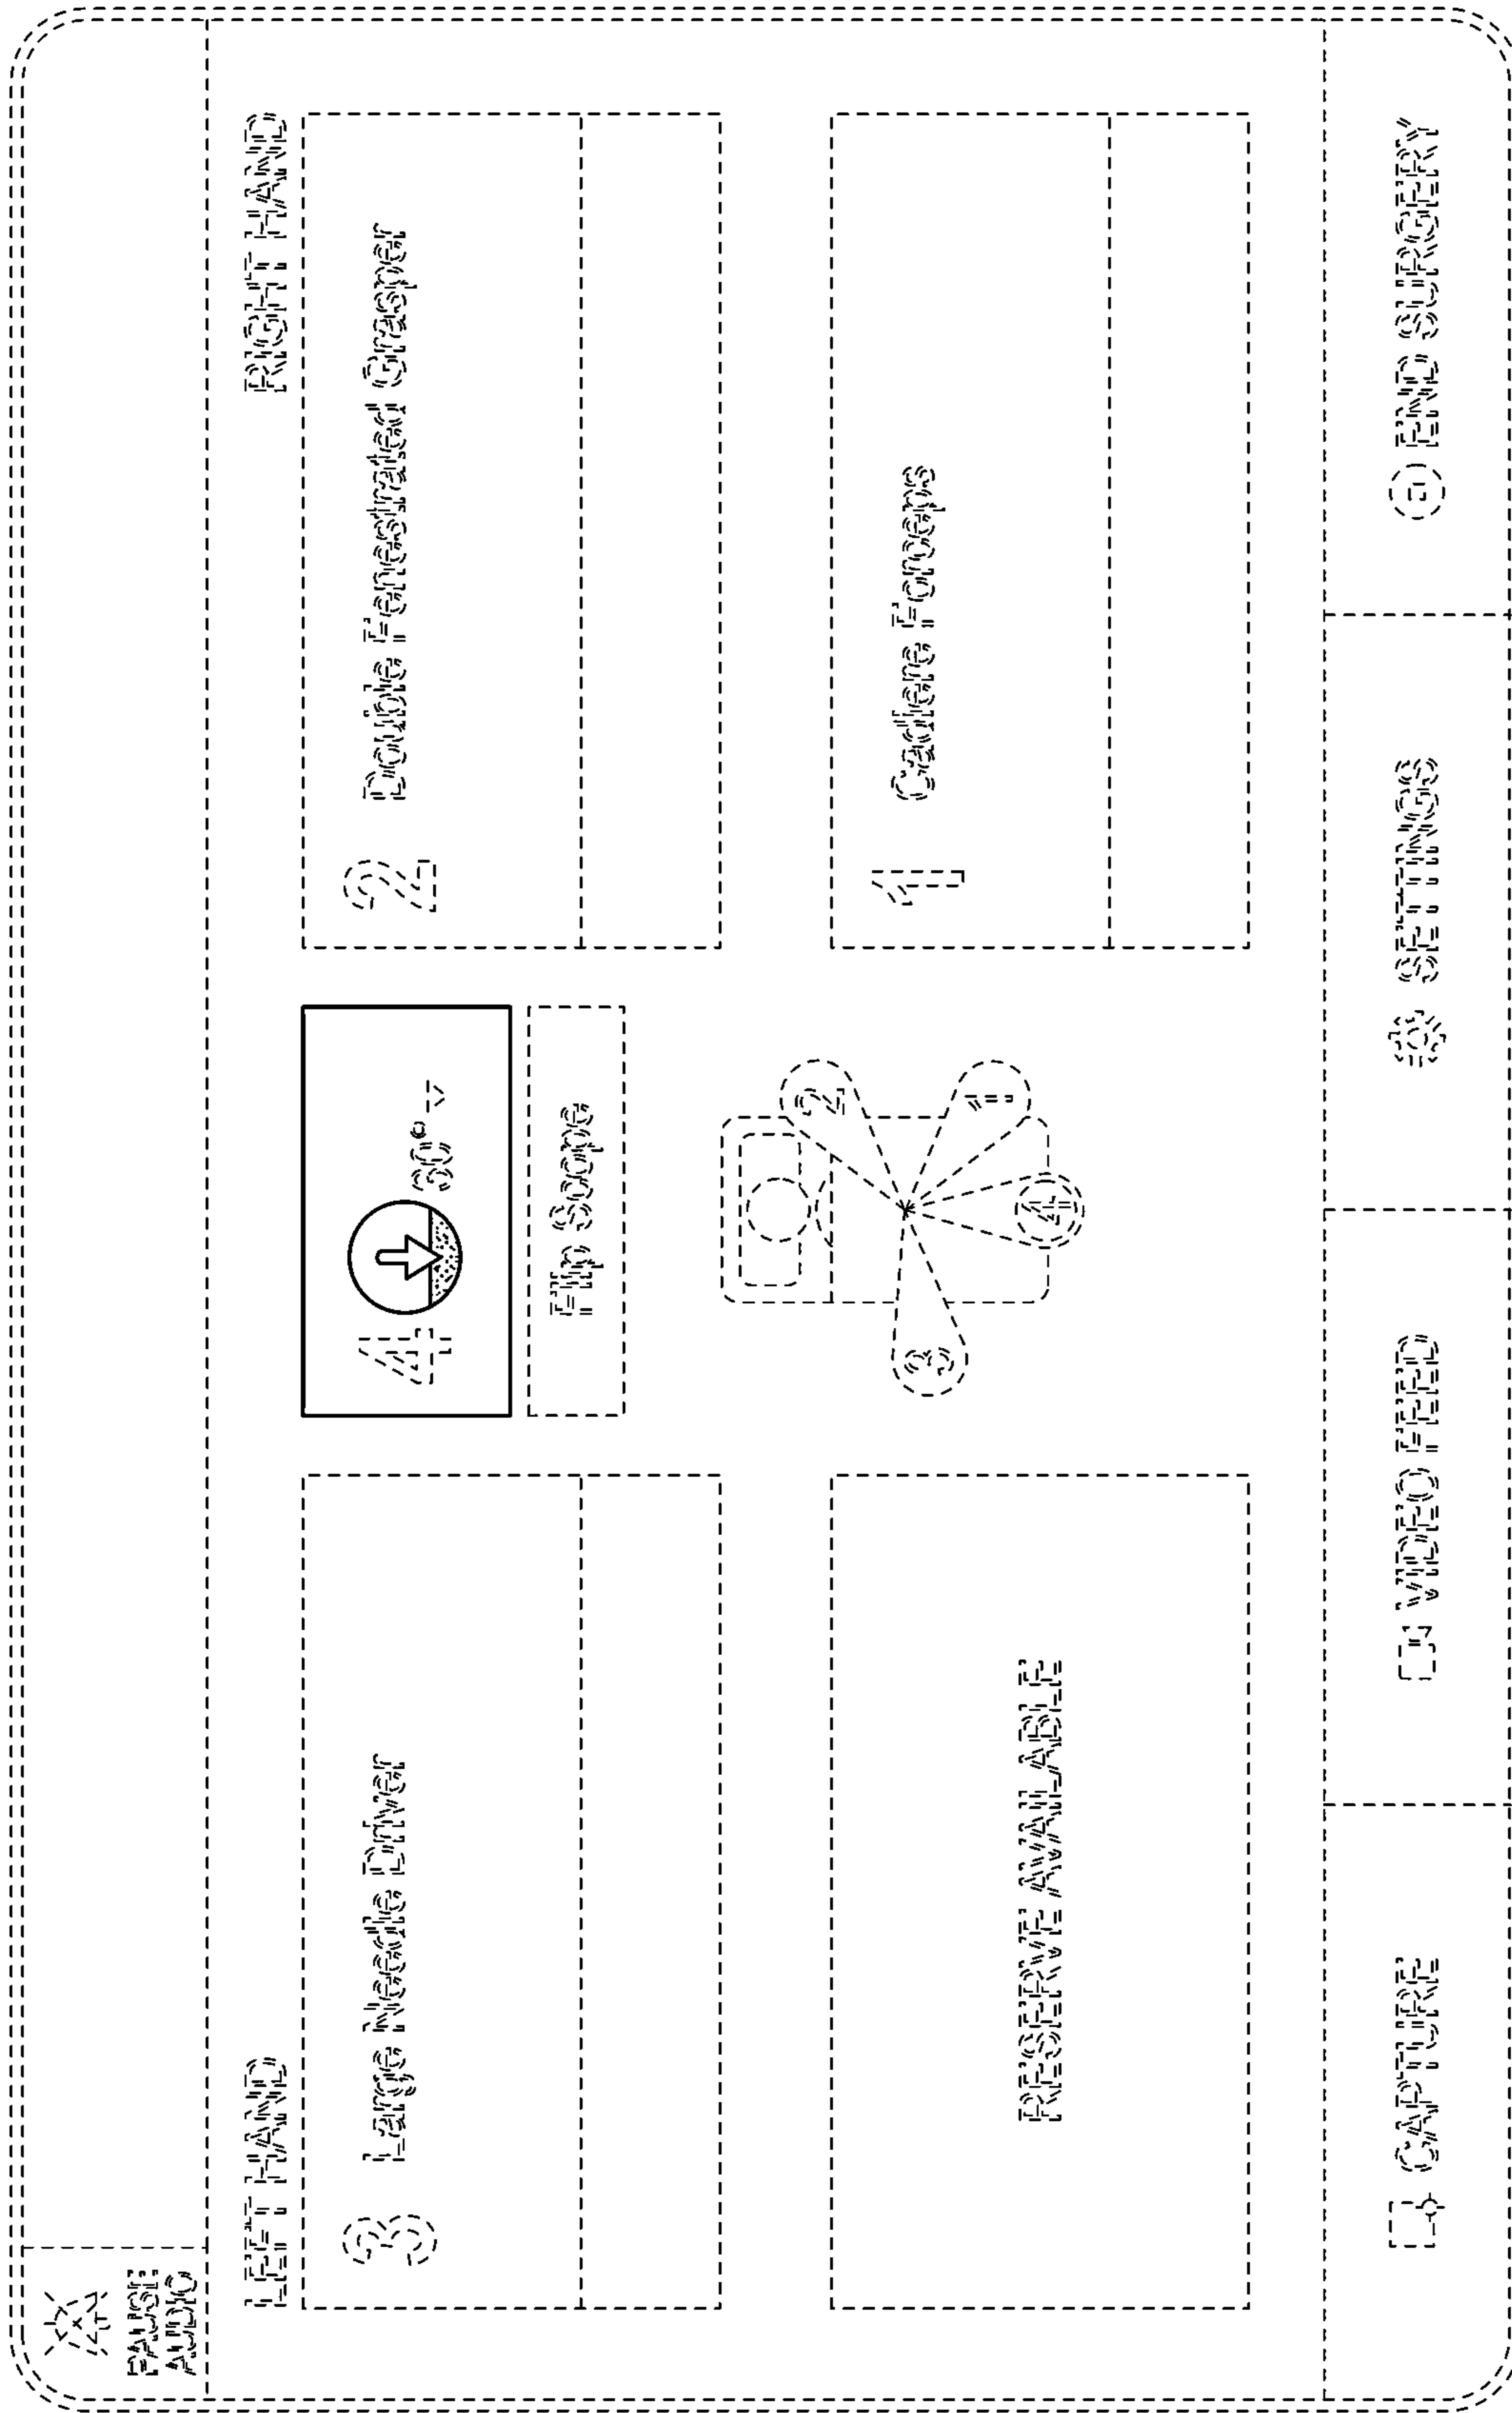


FIG. 2

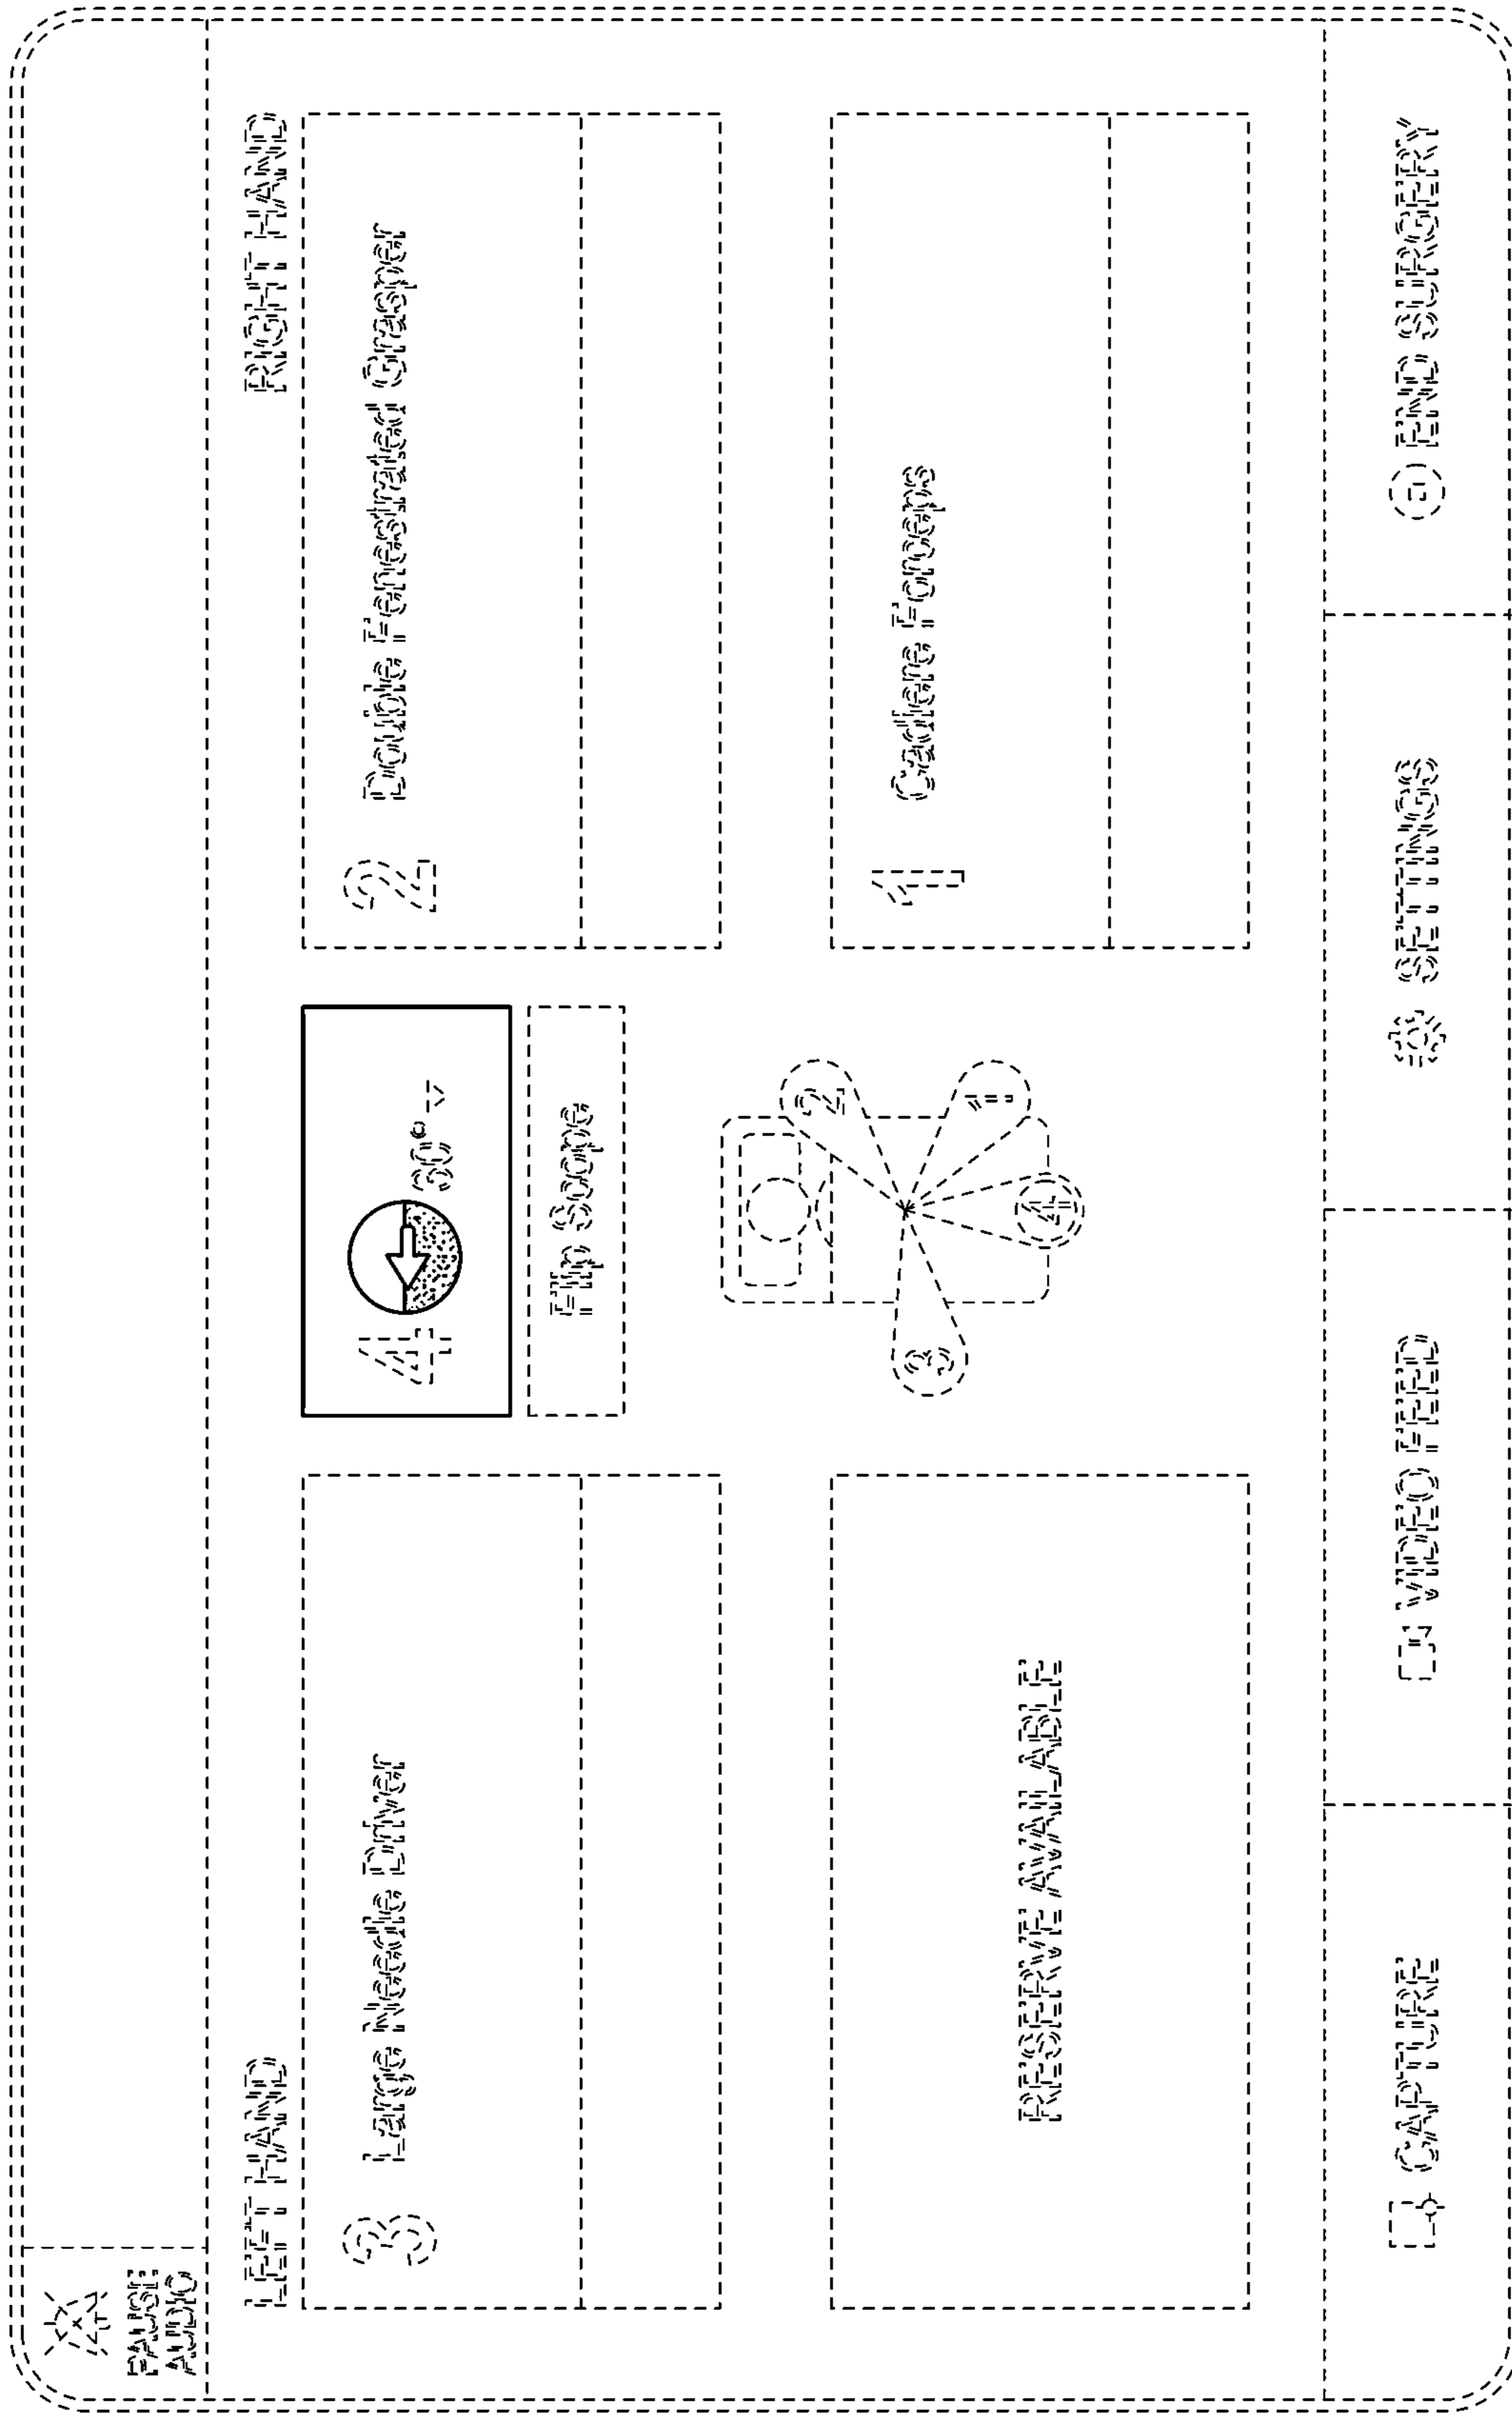


FIG. 3

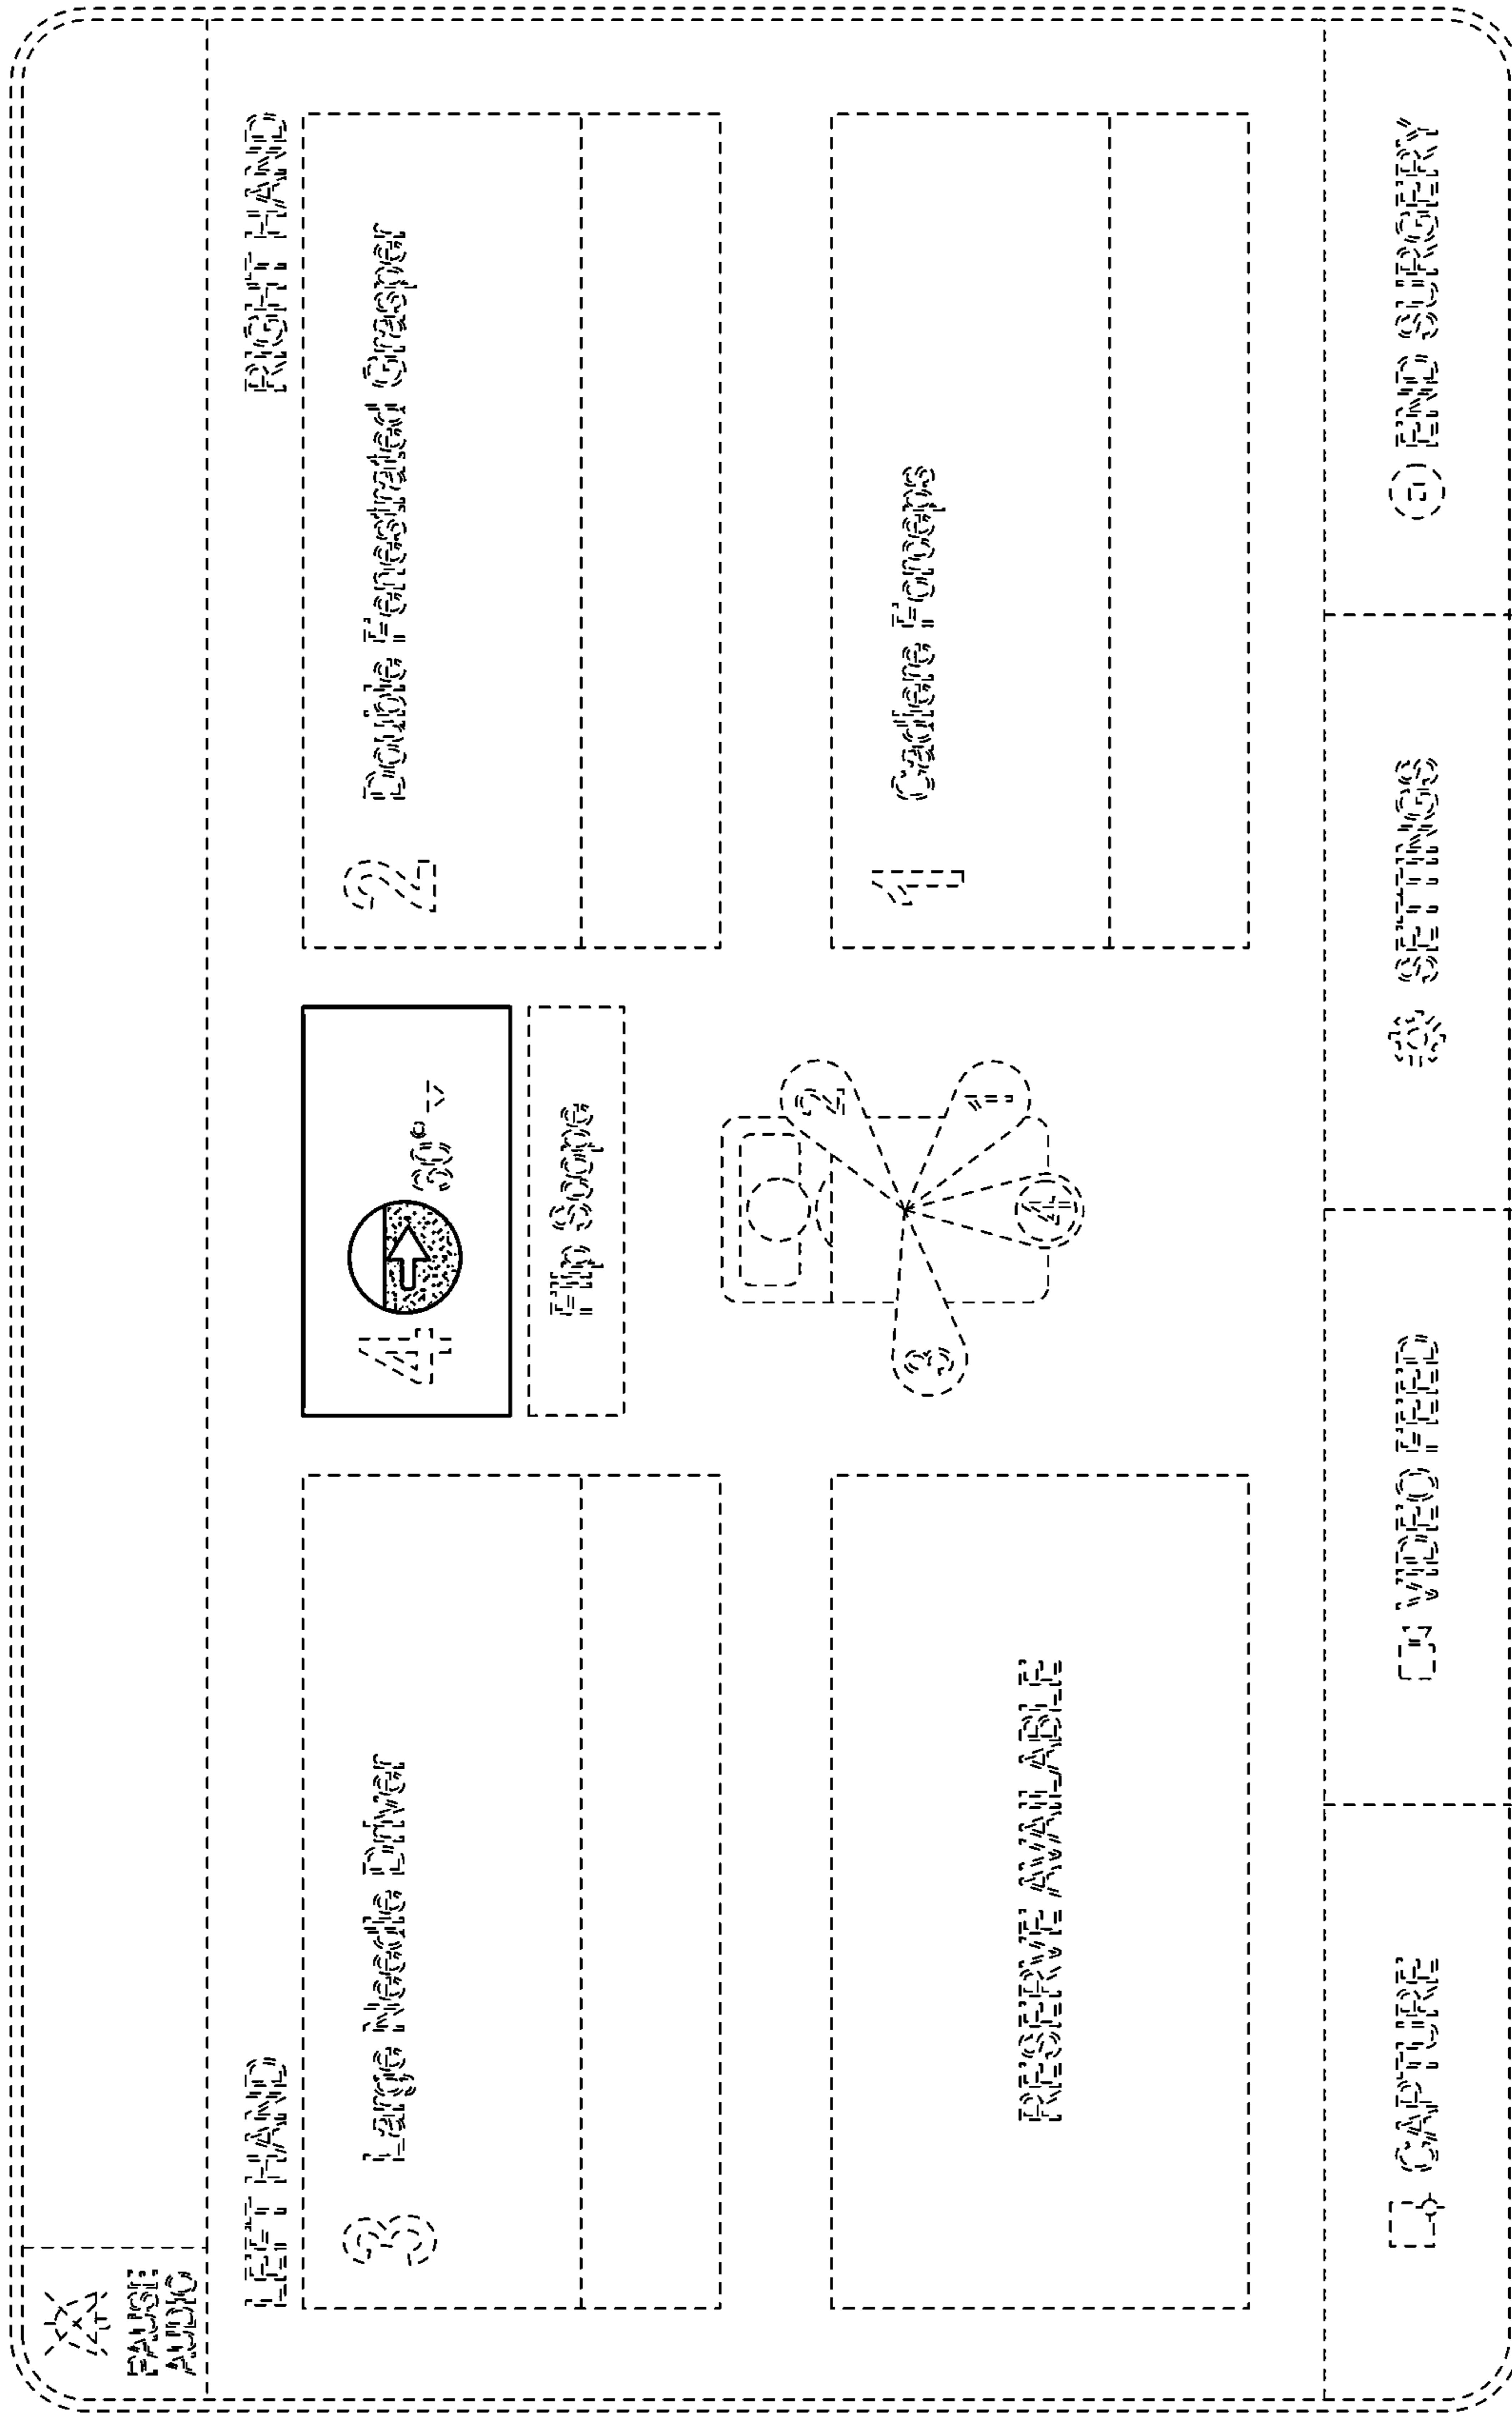


FIG. 4