



US00D986262S

(12) **United States Design Patent** (10) **Patent No.:** **US D986,262 S**  
**Amari et al.** (45) **Date of Patent:** **\*\* May 16, 2023**

(54) **DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE**

9,572,492 B2 \* 2/2017 Simpson ..... A61B 5/6852  
9,763,596 B2 \* 9/2017 Tonar ..... A61B 5/7278  
10,102,348 B2 \* 10/2018 Vendrell ..... G06F 3/04817

(Continued)

(71) Applicant: **OLYMPUS MEDICAL SYSTEMS CORPORATION**, Tokyo (JP)

FOREIGN PATENT DOCUMENTS

(72) Inventors: **Ryota Amari**, Machida (JP); **Shiho Miyauchi**, Tokyo (JP); **Takashi Nagata**, Shiki (JP)

CN 305286160 \* 8/2019  
CN 305391772 \* 10/2019

(Continued)

(73) Assignee: **OLYMPUS MEDICAL SYSTEMS CORPORATION**, Hachioji (JP)

OTHER PUBLICATIONS

(\*\*) Term: **15 Years**

Gastone Ciut, et al., *Frontiers of Robotic Colonoscopy: A Comprehensive Review of Robotic Colonoscopes and Technologies*, Publication Date May 31, 2020, Retrieved Date Oct. 11, 2022, Retrieved from Internet, < <https://www.mdpi.com/2077-0383/9/6/1648/htm> > (Year: 2020).\*

(Continued)

(21) Appl. No.: **29/797,521**

(22) Filed: **Jul. 1, 2021**

(51) **LOC (14) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/485**

(58) **Field of Classification Search**  
USPC ..... D14/485-488, 489-495  
CPC ..... A61B 5/02; G06F 3/048; G06F 3/04842; G06F 3/04845; G06F 3/0481; H04M 1/724-72484  
See application file for complete search history.

*Primary Examiner* — Rachel A. Voorhies

*Assistant Examiner* — Ana M. Vine

(74) *Attorney, Agent, or Firm* — Kenja IP Law PC

(57) **CLAIM**

The ornamental design for a display screen with graphical user interface, as shown and described.

**DESCRIPTION**

(56) **References Cited**


U.S. PATENT DOCUMENTS

- D397,687 S \* 9/1998 Arora ..... A61B 1/00055 D14/489
- D593,575 S \* 6/2009 Ball ..... D14/486
- 8,038,608 B2 \* 10/2011 Shigemori ..... A61B 1/00055 600/160
- D689,893 S \* 9/2013 Perry ..... G16H 20/40 D14/486
- 8,537,209 B2 \* 9/2013 Iwasaki ..... A61B 1/0004 715/767
- D771,648 S \* 11/2016 Rodriguez ..... G06T 19/20 D14/485

FIG. 1 is a front view of a display screen with graphical user interface of our new design; and, FIG. 2 is an enlarged view of the portion surrounded by the dashed-dotted line in FIG.1.

The broken line showing of the display screen and the interior dash-dash broken lines showing graphical user interface elements are included for illustrating portions of the article and form no part of the claimed design. The dot-dash broken line circle and the dot-dash lead line labeled 2 indicates the area from which the enlargement is taken and forms no part of the claimed design.

**1 Claim, 2 Drawing Sheets**

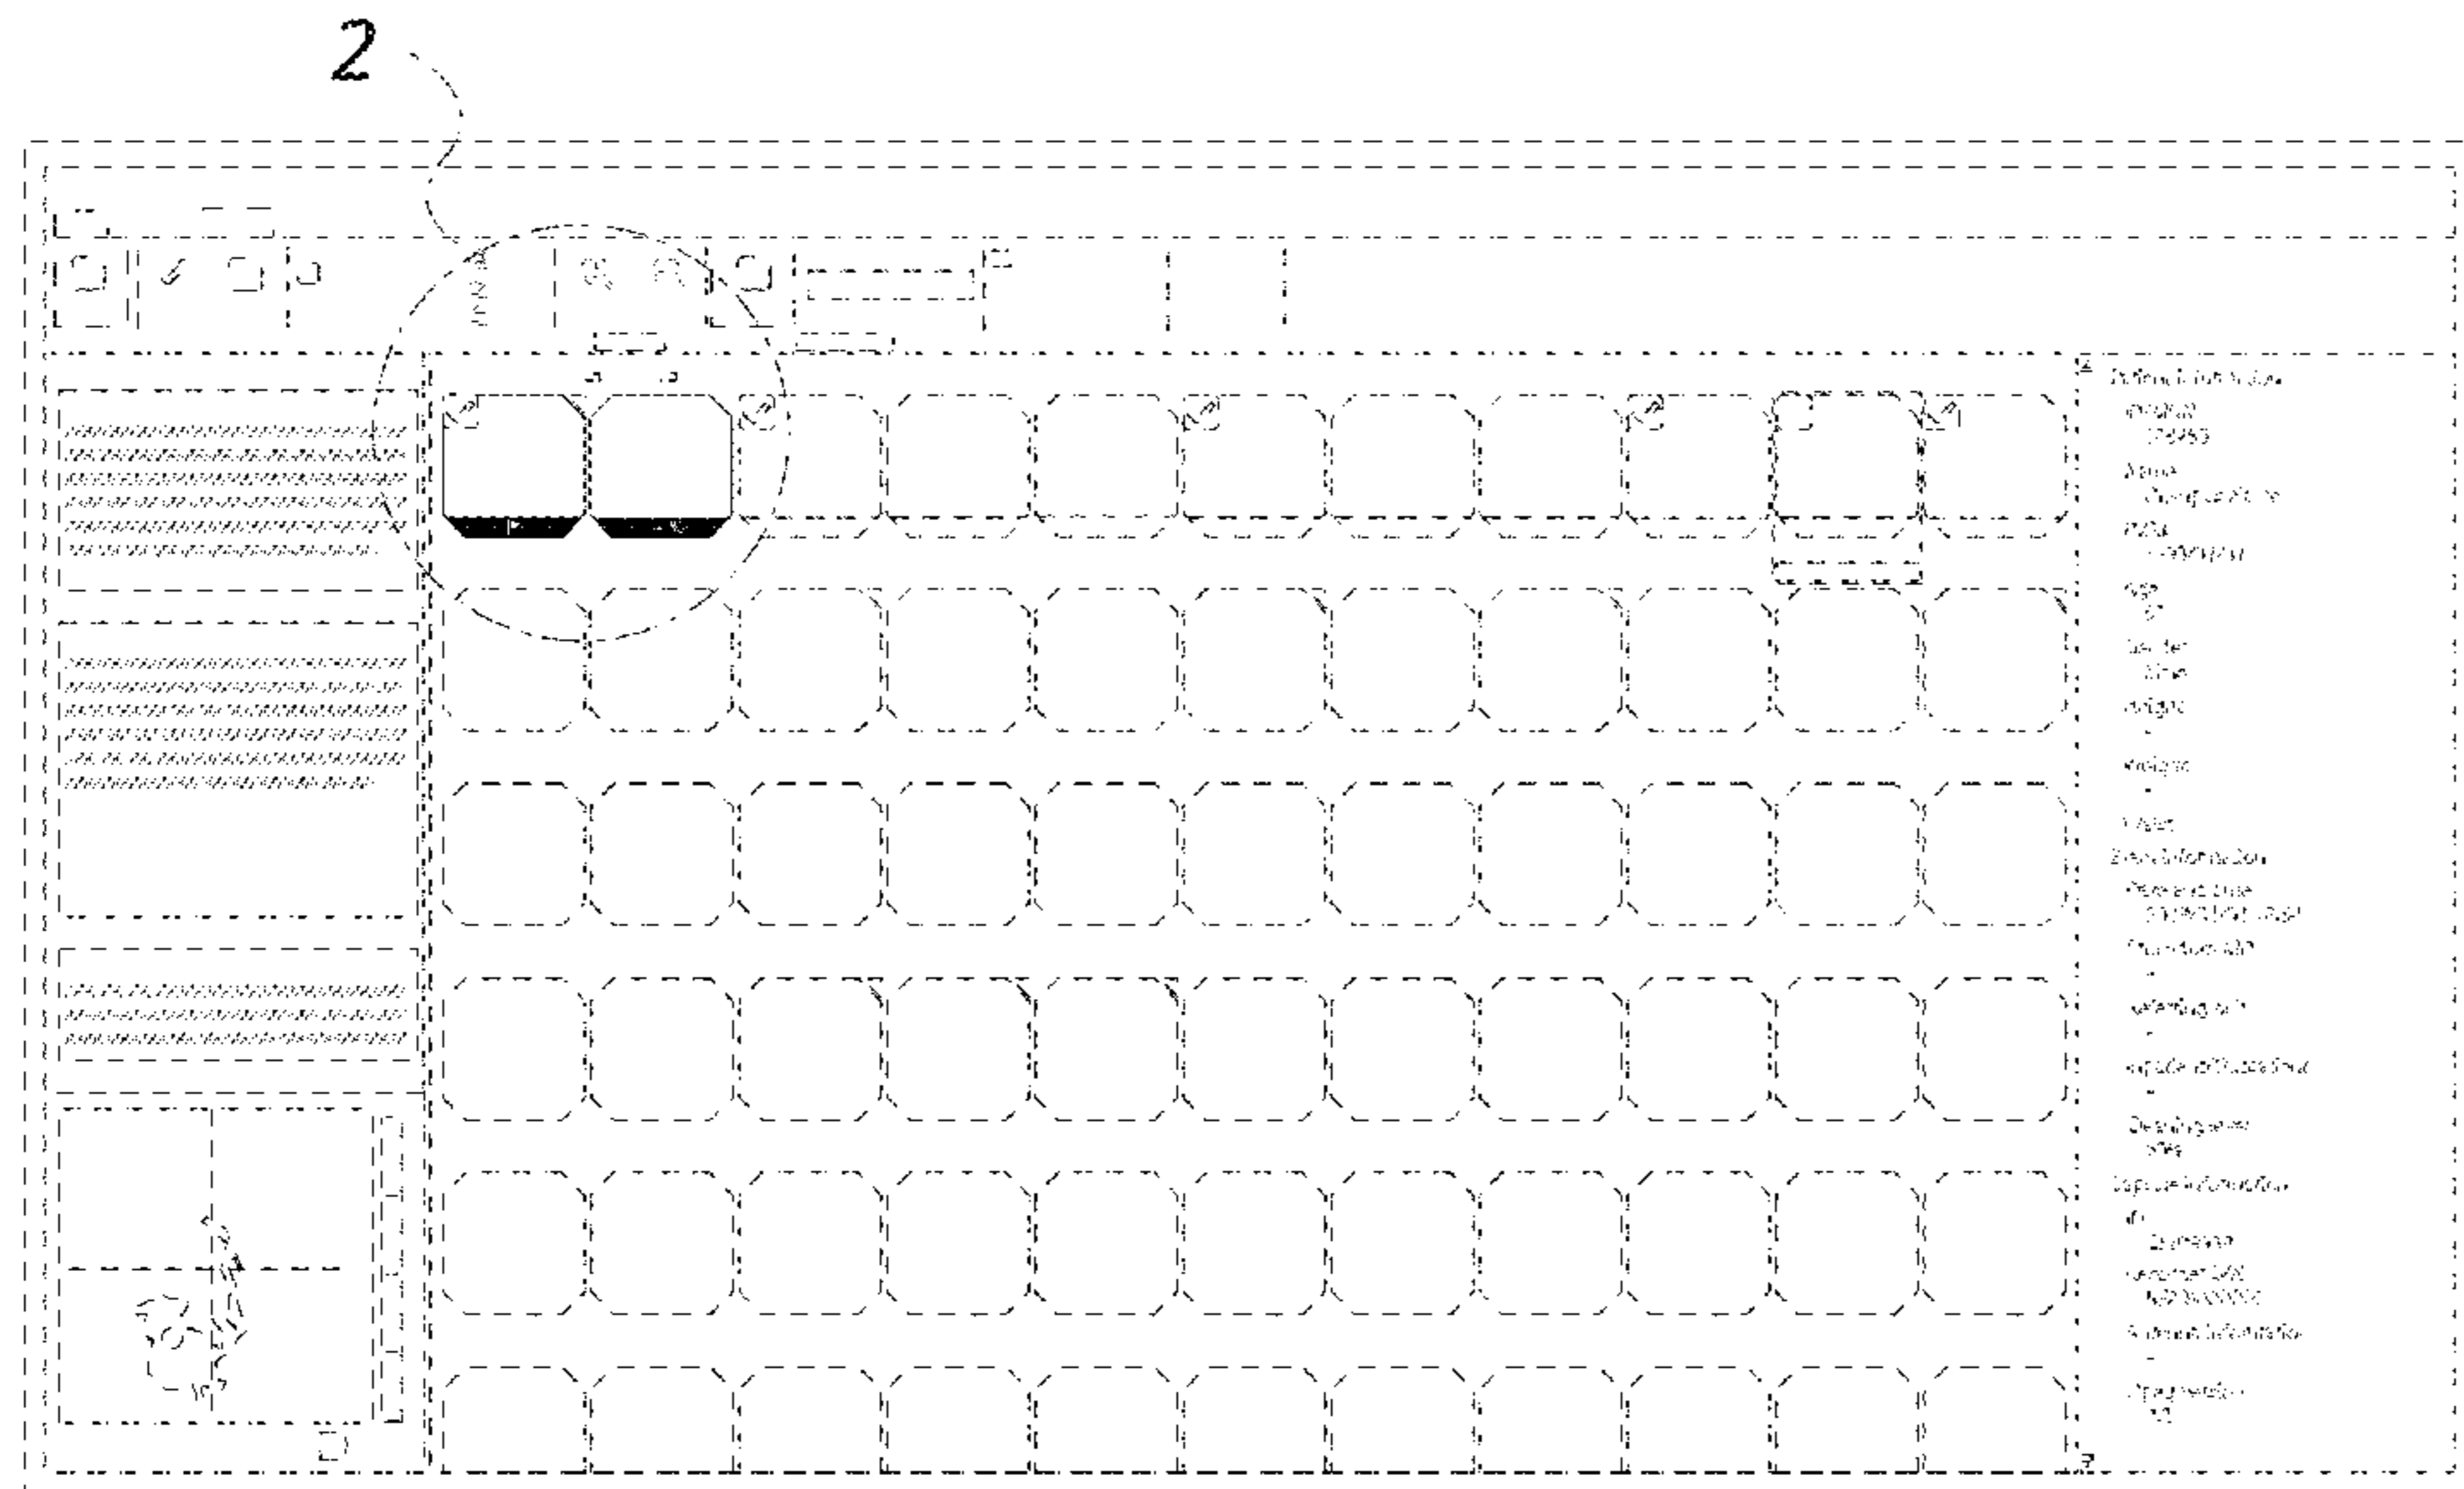

(56)

References Cited

U.S. PATENT DOCUMENTS

10,957,441 B2 \* 3/2021 Hermans ..... G16H 15/00  
 2009/0300540 A1 \* 12/2009 Russell ..... G06T 19/00  
 345/473  
 2012/0296957 A1 \* 11/2012 Stinson ..... G06F 3/04883  
 709/203  
 2014/0112564 A1 \* 4/2014 Hsiao ..... G06T 11/60  
 382/131  
 2015/0031954 A1 1/2015 Kimoto et al.  
 2015/0281564 A1 \* 10/2015 Shin ..... H04N 5/32  
 715/771  
 2015/0301732 A1 \* 10/2015 Henderson ..... G06T 7/0012  
 715/781  
 2015/0310652 A1 \* 10/2015 Dobson ..... G06T 7/0012  
 345/629  
 2015/0356271 A1 \* 12/2015 Kozuka ..... H04N 21/4725  
 705/2  
 2016/0202875 A1 \* 7/2016 Lee ..... G06T 19/20  
 345/419  
 2016/0203286 A1 \* 7/2016 Okabe ..... G16H 30/20  
 705/2  
 2020/0015927 A1 \* 1/2020 Ichiki ..... A61B 1/0661  
 2020/0030044 A1 \* 1/2020 Wang ..... G16H 20/40

FOREIGN PATENT DOCUMENTS

CN 306168483 \* 11/2020  
 CN 306189962 \* 11/2020

CN 306210541 \* 12/2020  
 CN 306236667 \* 12/2020  
 CN 306460996 \* 4/2021  
 CN 306512212 \* 5/2021  
 JP 1489661 S 2/2014  
 JP 1489662 S 2/2014

OTHER PUBLICATIONS


Hanna Borgli et al., HyperKvasir, a comprehensive multi-class image and video dataset for gastrointestinal endoscopy, Publication Date Aug. 28, 2020, Retrieved Date Oct. 11, 2022, Retrieved from Internet, < <https://www.nature.com/articles/s41597-020-00622-y> > (Year: 2020).\*

Maarten R. Struyvenberg, MD, et al., A computer-assisted algorithm for narrow-band imaging-based tissue characterization . . . , Publication Date Jun. 3, 2020, Retrieved Date Oct. 11, 2021, Retrieved from Internet, < [https://www.giejournal.org/article/S0016-5107\(20\)34400-X/fulltext#relatedArticles](https://www.giejournal.org/article/S0016-5107(20)34400-X/fulltext#relatedArticles) > (Year: 2020).\*

PillCam™ Capsule Endoscopy User Manual, PillCam™ Desktop Software Version 9.0, Nov. 2016, p. 176.

\* cited by examiner

FIG. 1

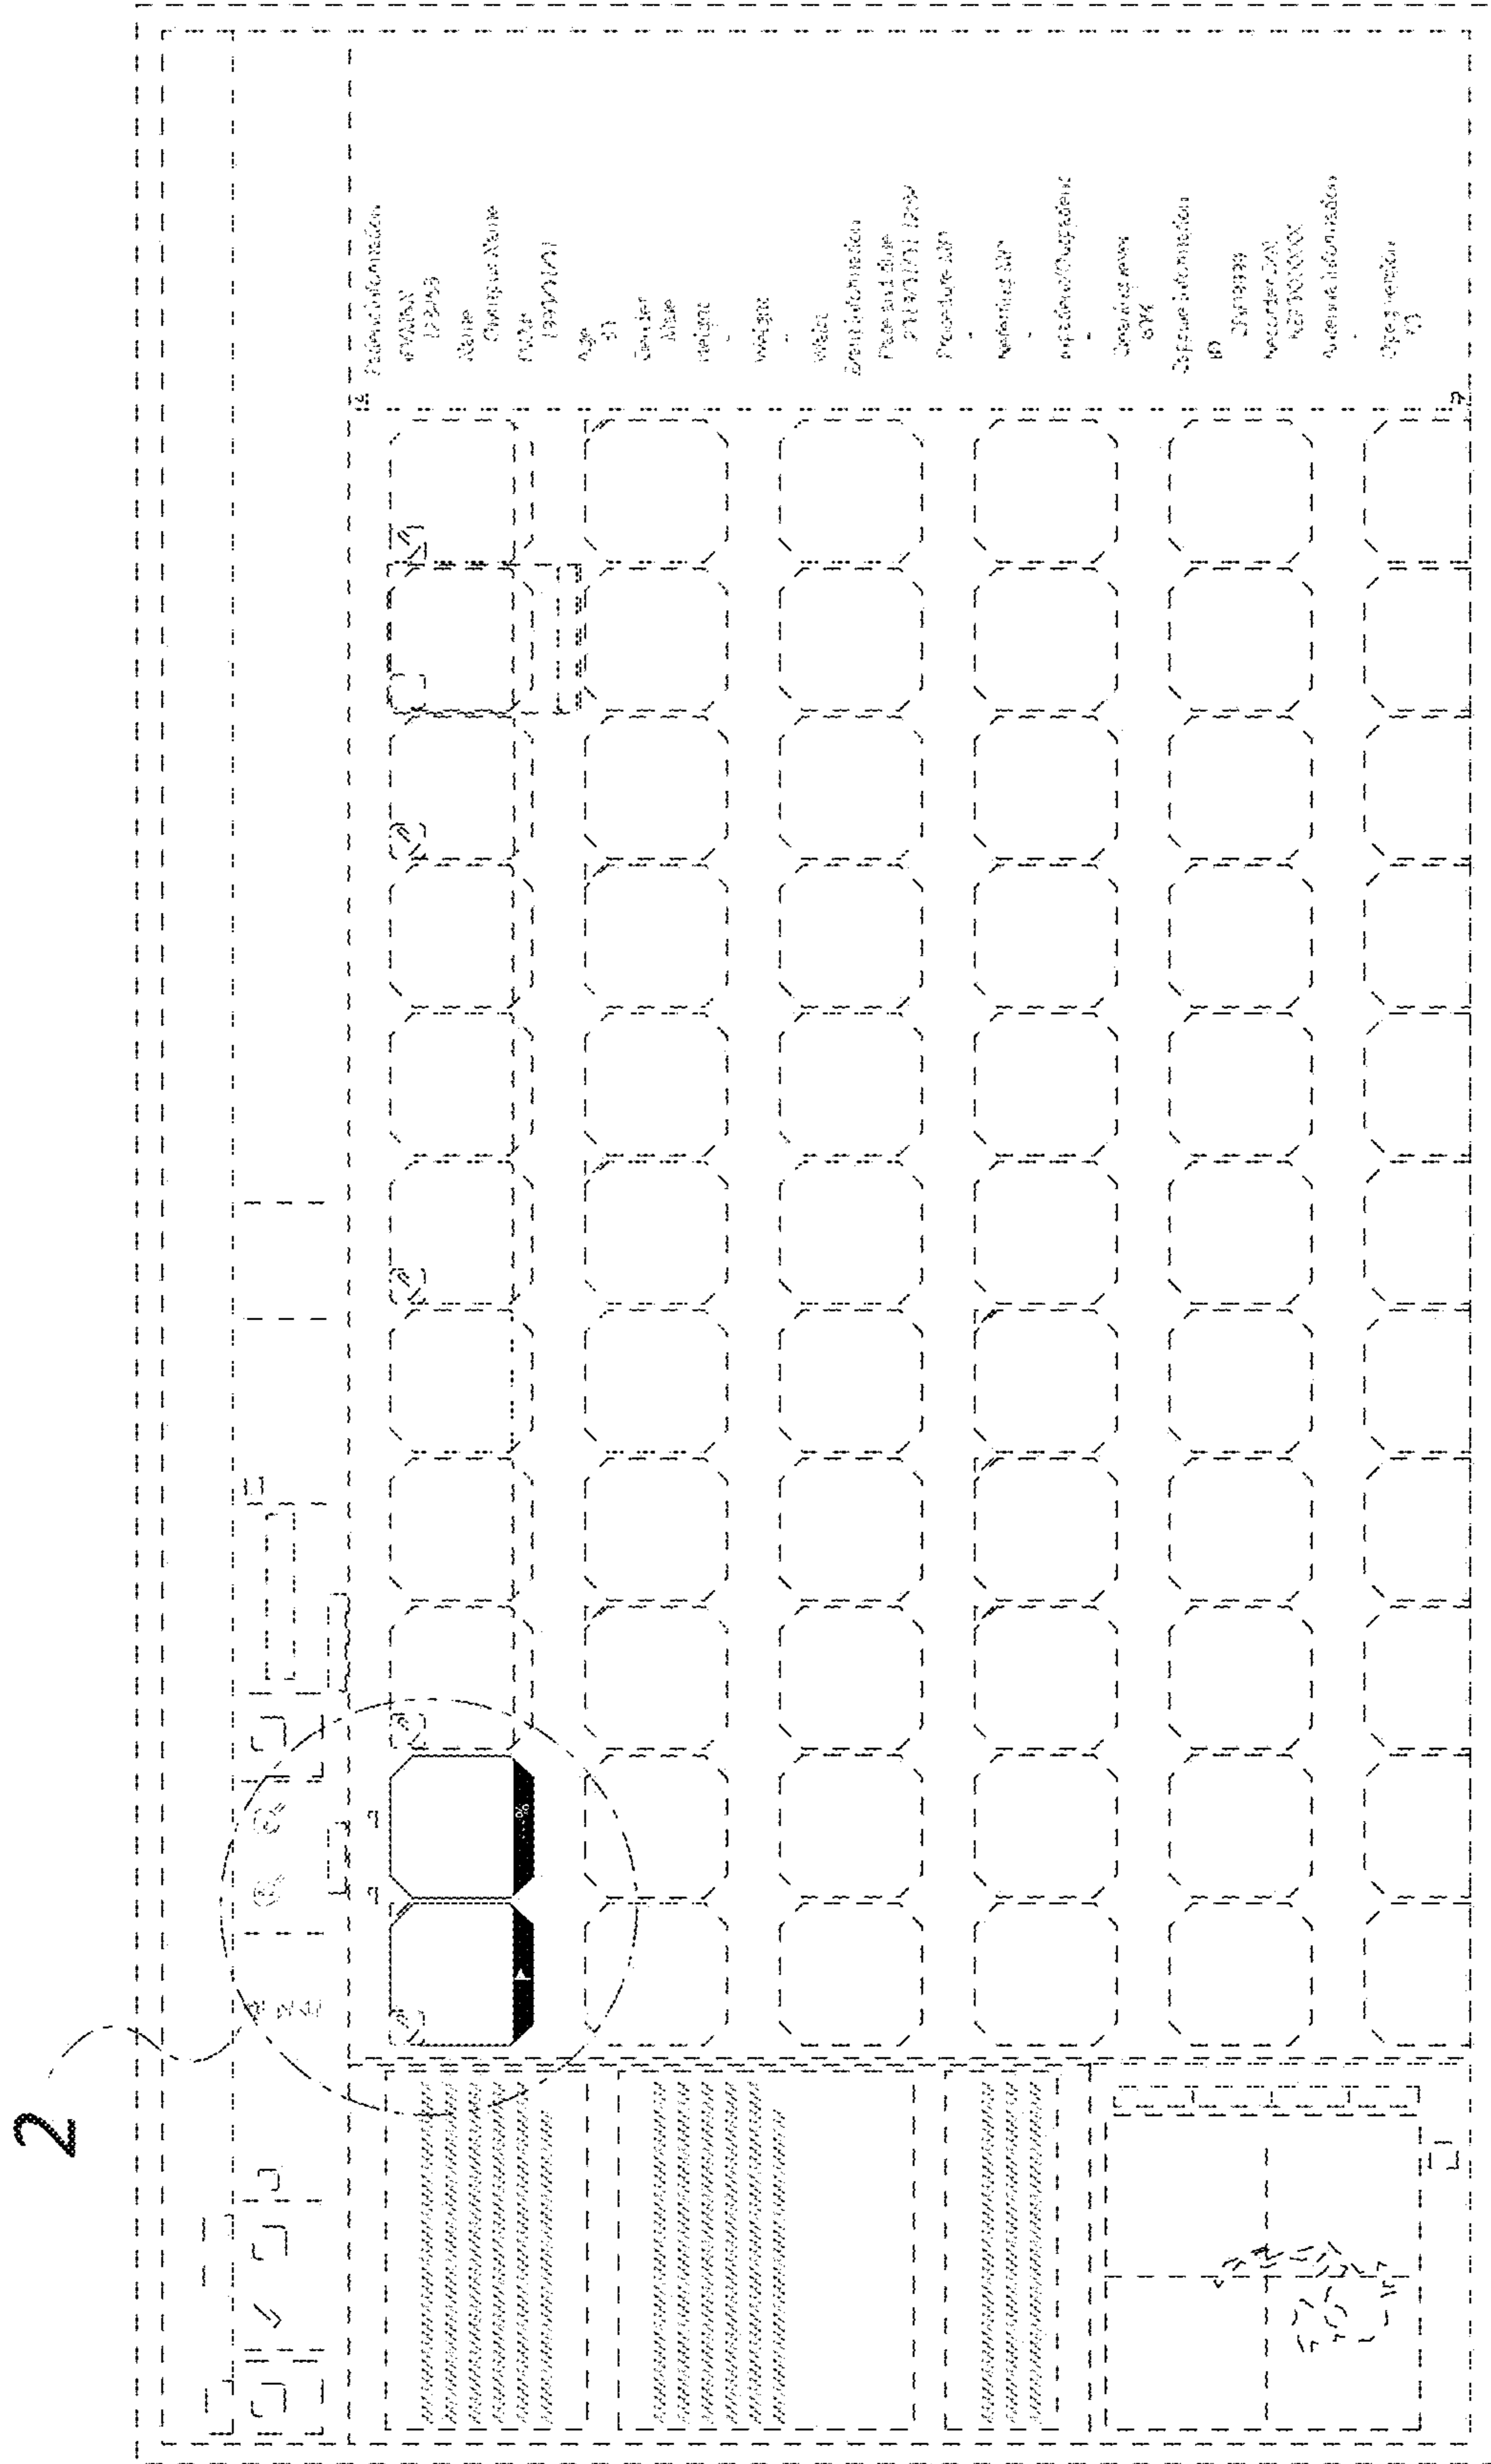

*FIG. 2*

