



US00D987109S

(12) **United States Design Patent** (10) **Patent No.:** **US D987,109 S**
Kovacs (45) **Date of Patent:** **** May 23, 2023**

(54) **EXTRUDED BASE PLATE FOR AN OPERATING ROOM TABLE**

(71) Applicant: **INNOVATIVE MEDICAL PRODUCTS, INC.**, Plainville, CT (US)

(72) Inventor: **Tamas Kovacs**, Burlington, CT (US)

(73) Assignee: **INDUSTRIAL FLOW SOLUTIONS, INC.**, Plainville, CT (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/799,669**

(22) Filed: **Jul. 15, 2021**

(51) **LOC (14) Cl.** **24-99**

(52) **U.S. Cl.**
USPC **D24/231**; D24/183; D24/184

(58) **Field of Classification Search**
USPC D24/127, 128, 171, 172, 183, 184, 227, D24/231, 234; D8/20, 377

CPC A61B 6/0407; A61B 5/704; A61B 90/50; A61B 2090/571; A61B 2034/2055

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 2,829,640 A * 4/1958 Moorman A61G 13/12 378/208
- D240,707 S * 7/1976 Rudinski D8/377
- D252,668 S * 8/1979 Rudinski D25/119
- 4,232,681 A 11/1980 Tulaszewski
- 4,653,482 A * 3/1987 Kurland A61G 13/12 5/601
- 5,826,286 A * 10/1998 Cranston A61G 13/04 5/942
- 6,058,534 A 5/2000 Navarro et al.
- D439,670 S * 3/2001 Sommer D24/183
- D502,090 S * 2/2005 Castellanos D8/377
- D543,094 S * 5/2007 Remmers D8/377

- D585,267 S * 1/2009 Di Vinadio D8/377
- D611,743 S * 3/2010 Mitten D8/377
- 7,971,298 B2 * 7/2011 Kobuß A61B 6/0442 5/621
- 8,146,874 B2 * 4/2012 Yu A61G 7/0503 248/316.4
- D731,068 S * 6/2015 Moon D24/183

(Continued)

FOREIGN PATENT DOCUMENTS

JP D1724704 * 9/2022

OTHER PUBLICATIONS

IFU-IMP-0003 Quad® Clamp. Feb. 3, 2021. Site visited Dec. 16, 2022. [<https://www.impmedical.com/surgical-positioning/knee-positioner/De-Mayo-Adapt2Fit-surgical-knee-positioning-leg-holder>] (Year: 2021).*

(Continued)

Primary Examiner — Wendy L Arminio
Assistant Examiner — Maheen Khurshid
(74) *Attorney, Agent, or Firm* — Damian Wasserbauer, Esq.; Nicholas E. Blanton; Wasserbauer Law LLC


(57) **CLAIM**

The ornamental design for an extruded base plate for an operating room table, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right side perspective view of the extruded base plate for an operating room table in accordance with the present invention;
FIG. 2 is a front view thereof;
FIG. 3 is a rear view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a bottom view thereof; and,
FIG. 6 is a right side view thereof, wherein the left side view is a mirror image thereof.

1 Claim, 6 Drawing Sheets

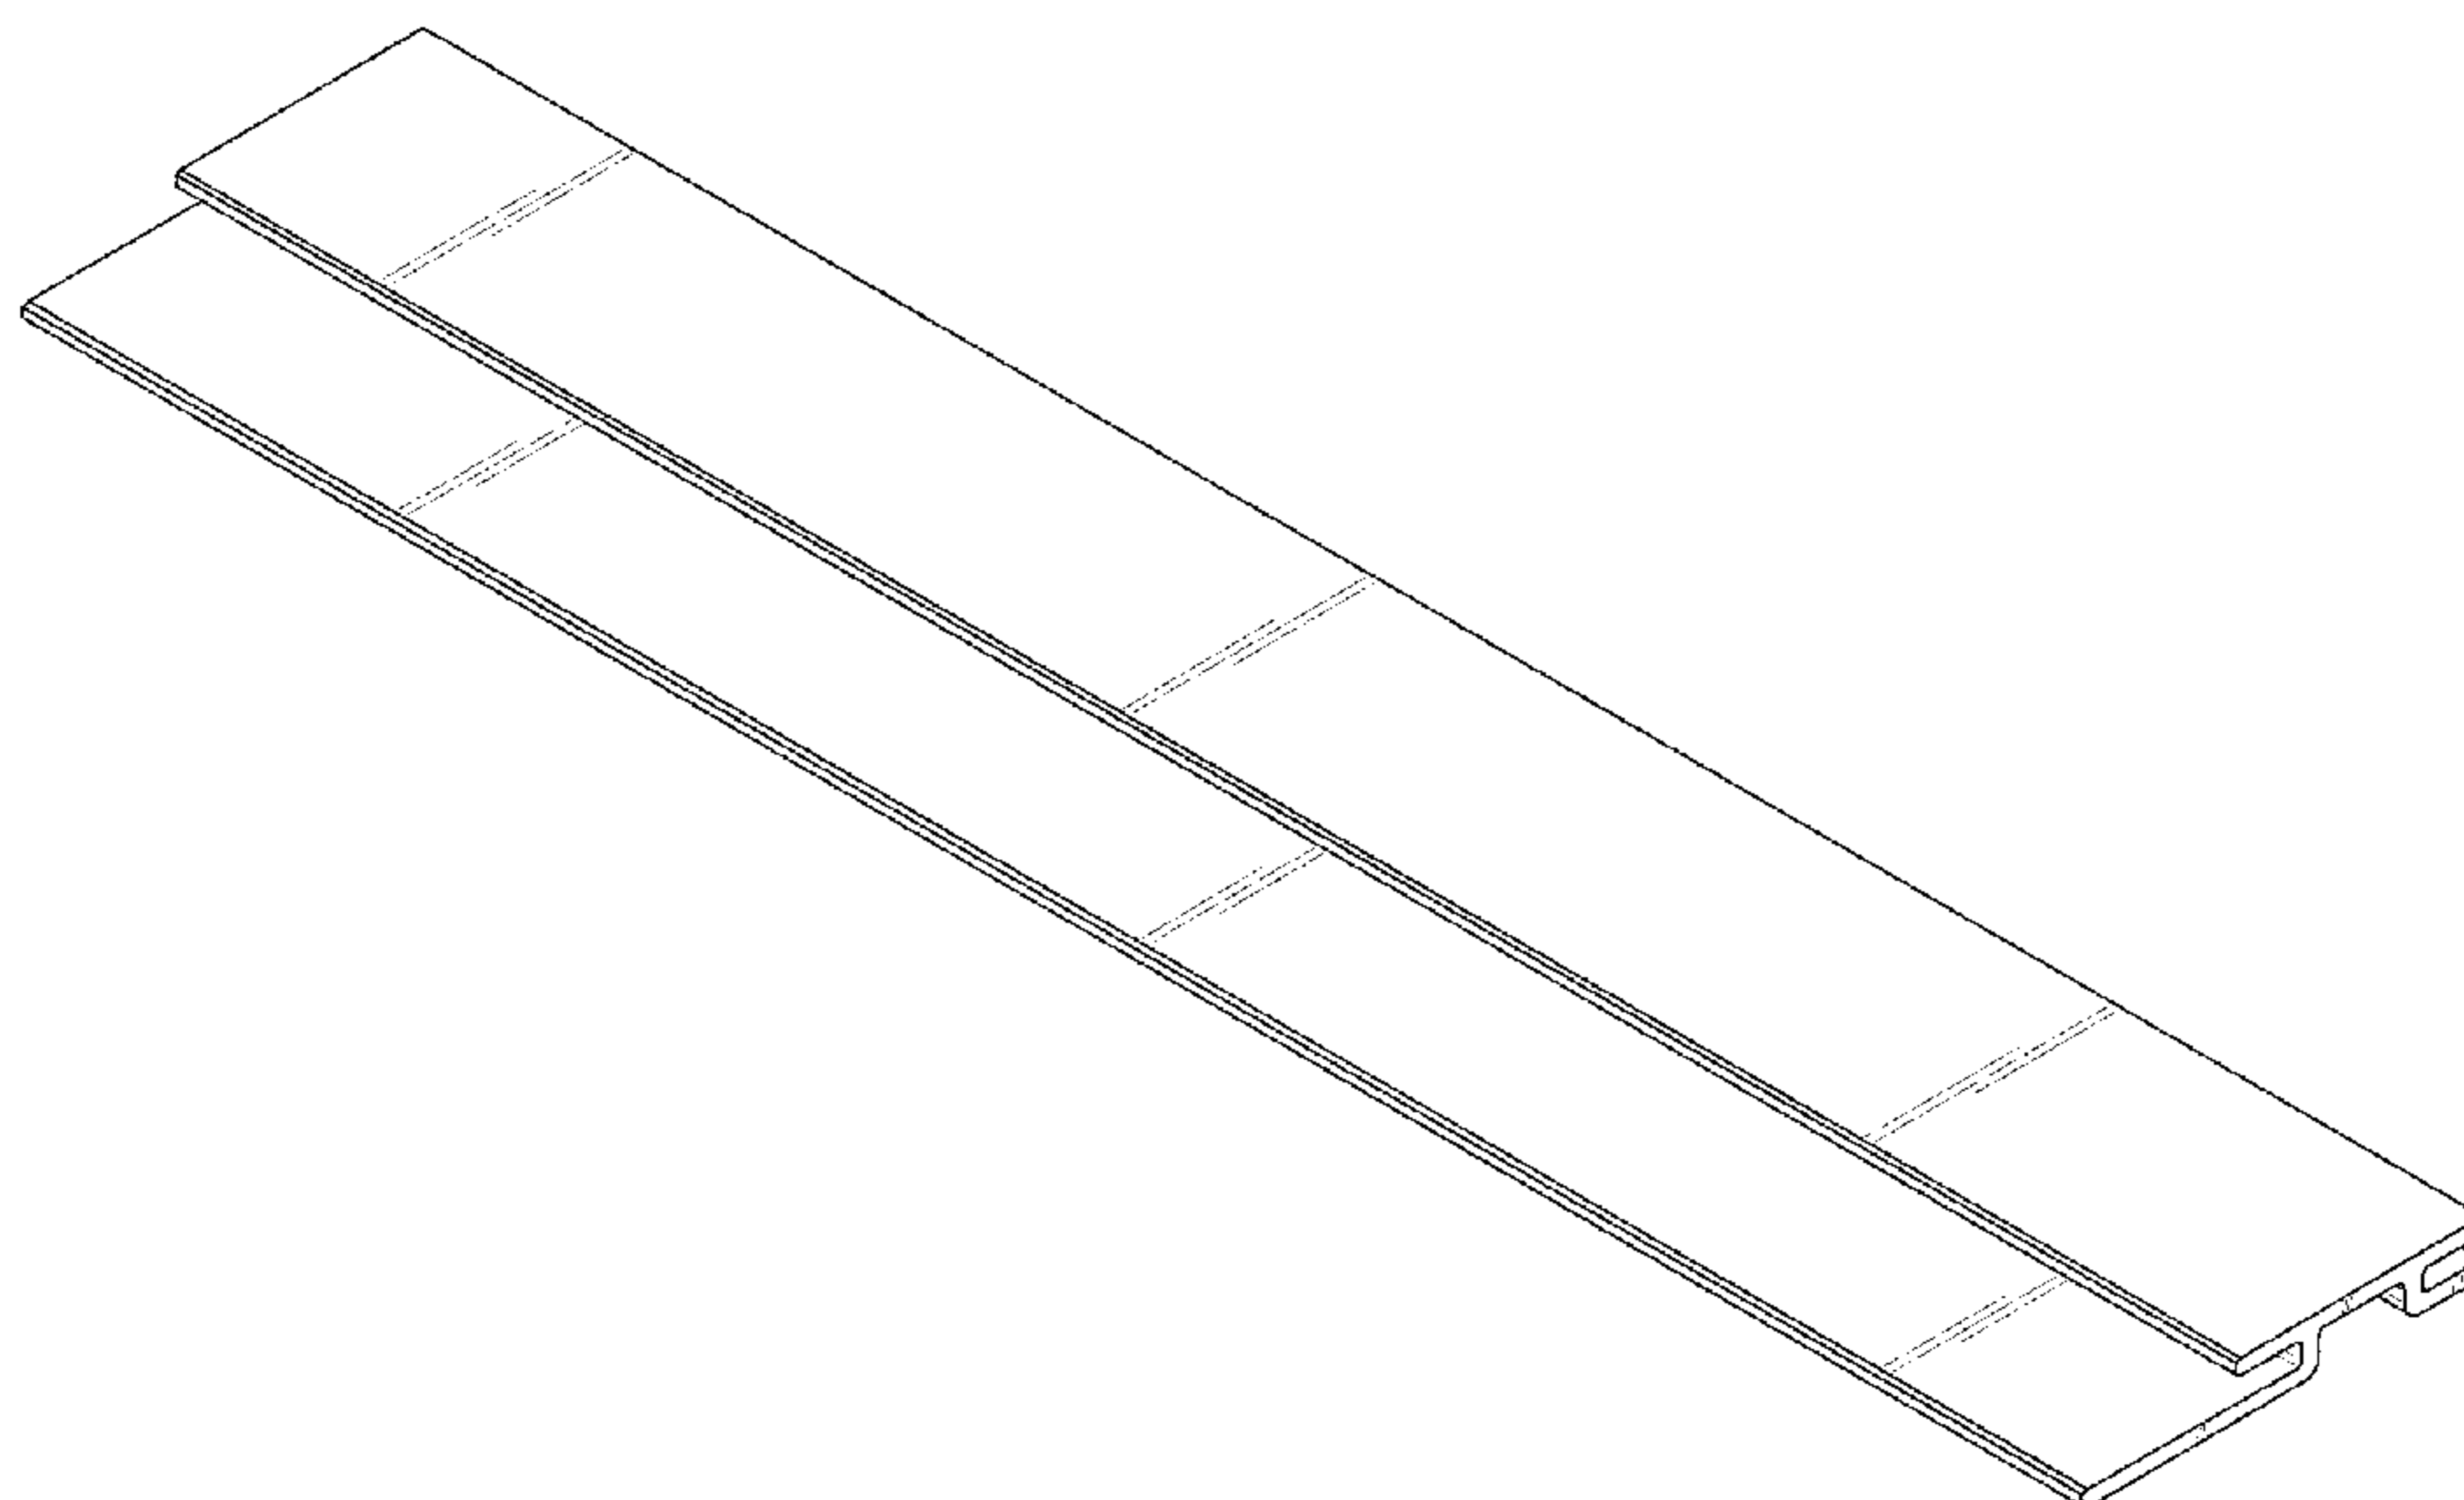

(56)

References Cited

U.S. PATENT DOCUMENTS

D755,041	S *	5/2016	Weldon	D8/377
9,603,765	B2	3/2017	Kreuzer et al.		
9,615,987	B2	4/2017	Worm et al.		
9,642,762	B2 *	5/2017	Frueh	A61G 7/08
D791,348	S *	7/2017	Singh	D25/119
D791,354	S *	7/2017	Singh	D25/119
D813,636	S *	3/2018	Hsieh	D8/71
D834,928	S *	12/2018	Lu	D8/381
D838,857	S *	1/2019	Blackwell	D24/184
D844,807	S *	4/2019	Blackwell	D24/231
D872,884	S *	1/2020	Carter	D25/119
D909,179	S *	2/2021	Kovacs	D8/349
10,912,697	B2 *	2/2021	Staudinger	A61G 13/02
D920,769	S *	6/2021	Kovacs	D25/164
11,083,420	B2 *	8/2021	Suga	A61B 6/0407
D948,998	S *	4/2022	Noe	D25/119
2016/0151223	A1 *	6/2016	Ferro	A61G 13/129 128/845

OTHER PUBLICATIONS

SchureMed TKR Positioner. 2009. Site visited Dec. 16, 2022. [https://www.universalmedicalinc.com/tkr-positioner-for-total-knee-replacement.html?campaignid=1821462889&adgroupid=70633908718&adid=345215573729&gclid=EA1a1QobChMlrZDKIqH--wIVGpflCh3EygSNEAAYASABEgK2bPD_BwE] (Year: 2009).*

TKR Positioner. Apr. 7, 2021. Site visited Dec. 16, 2022. [https://www.youtube.com/watch?v=_ZduRUDweUA] (Year: 2021).*

* cited by examiner

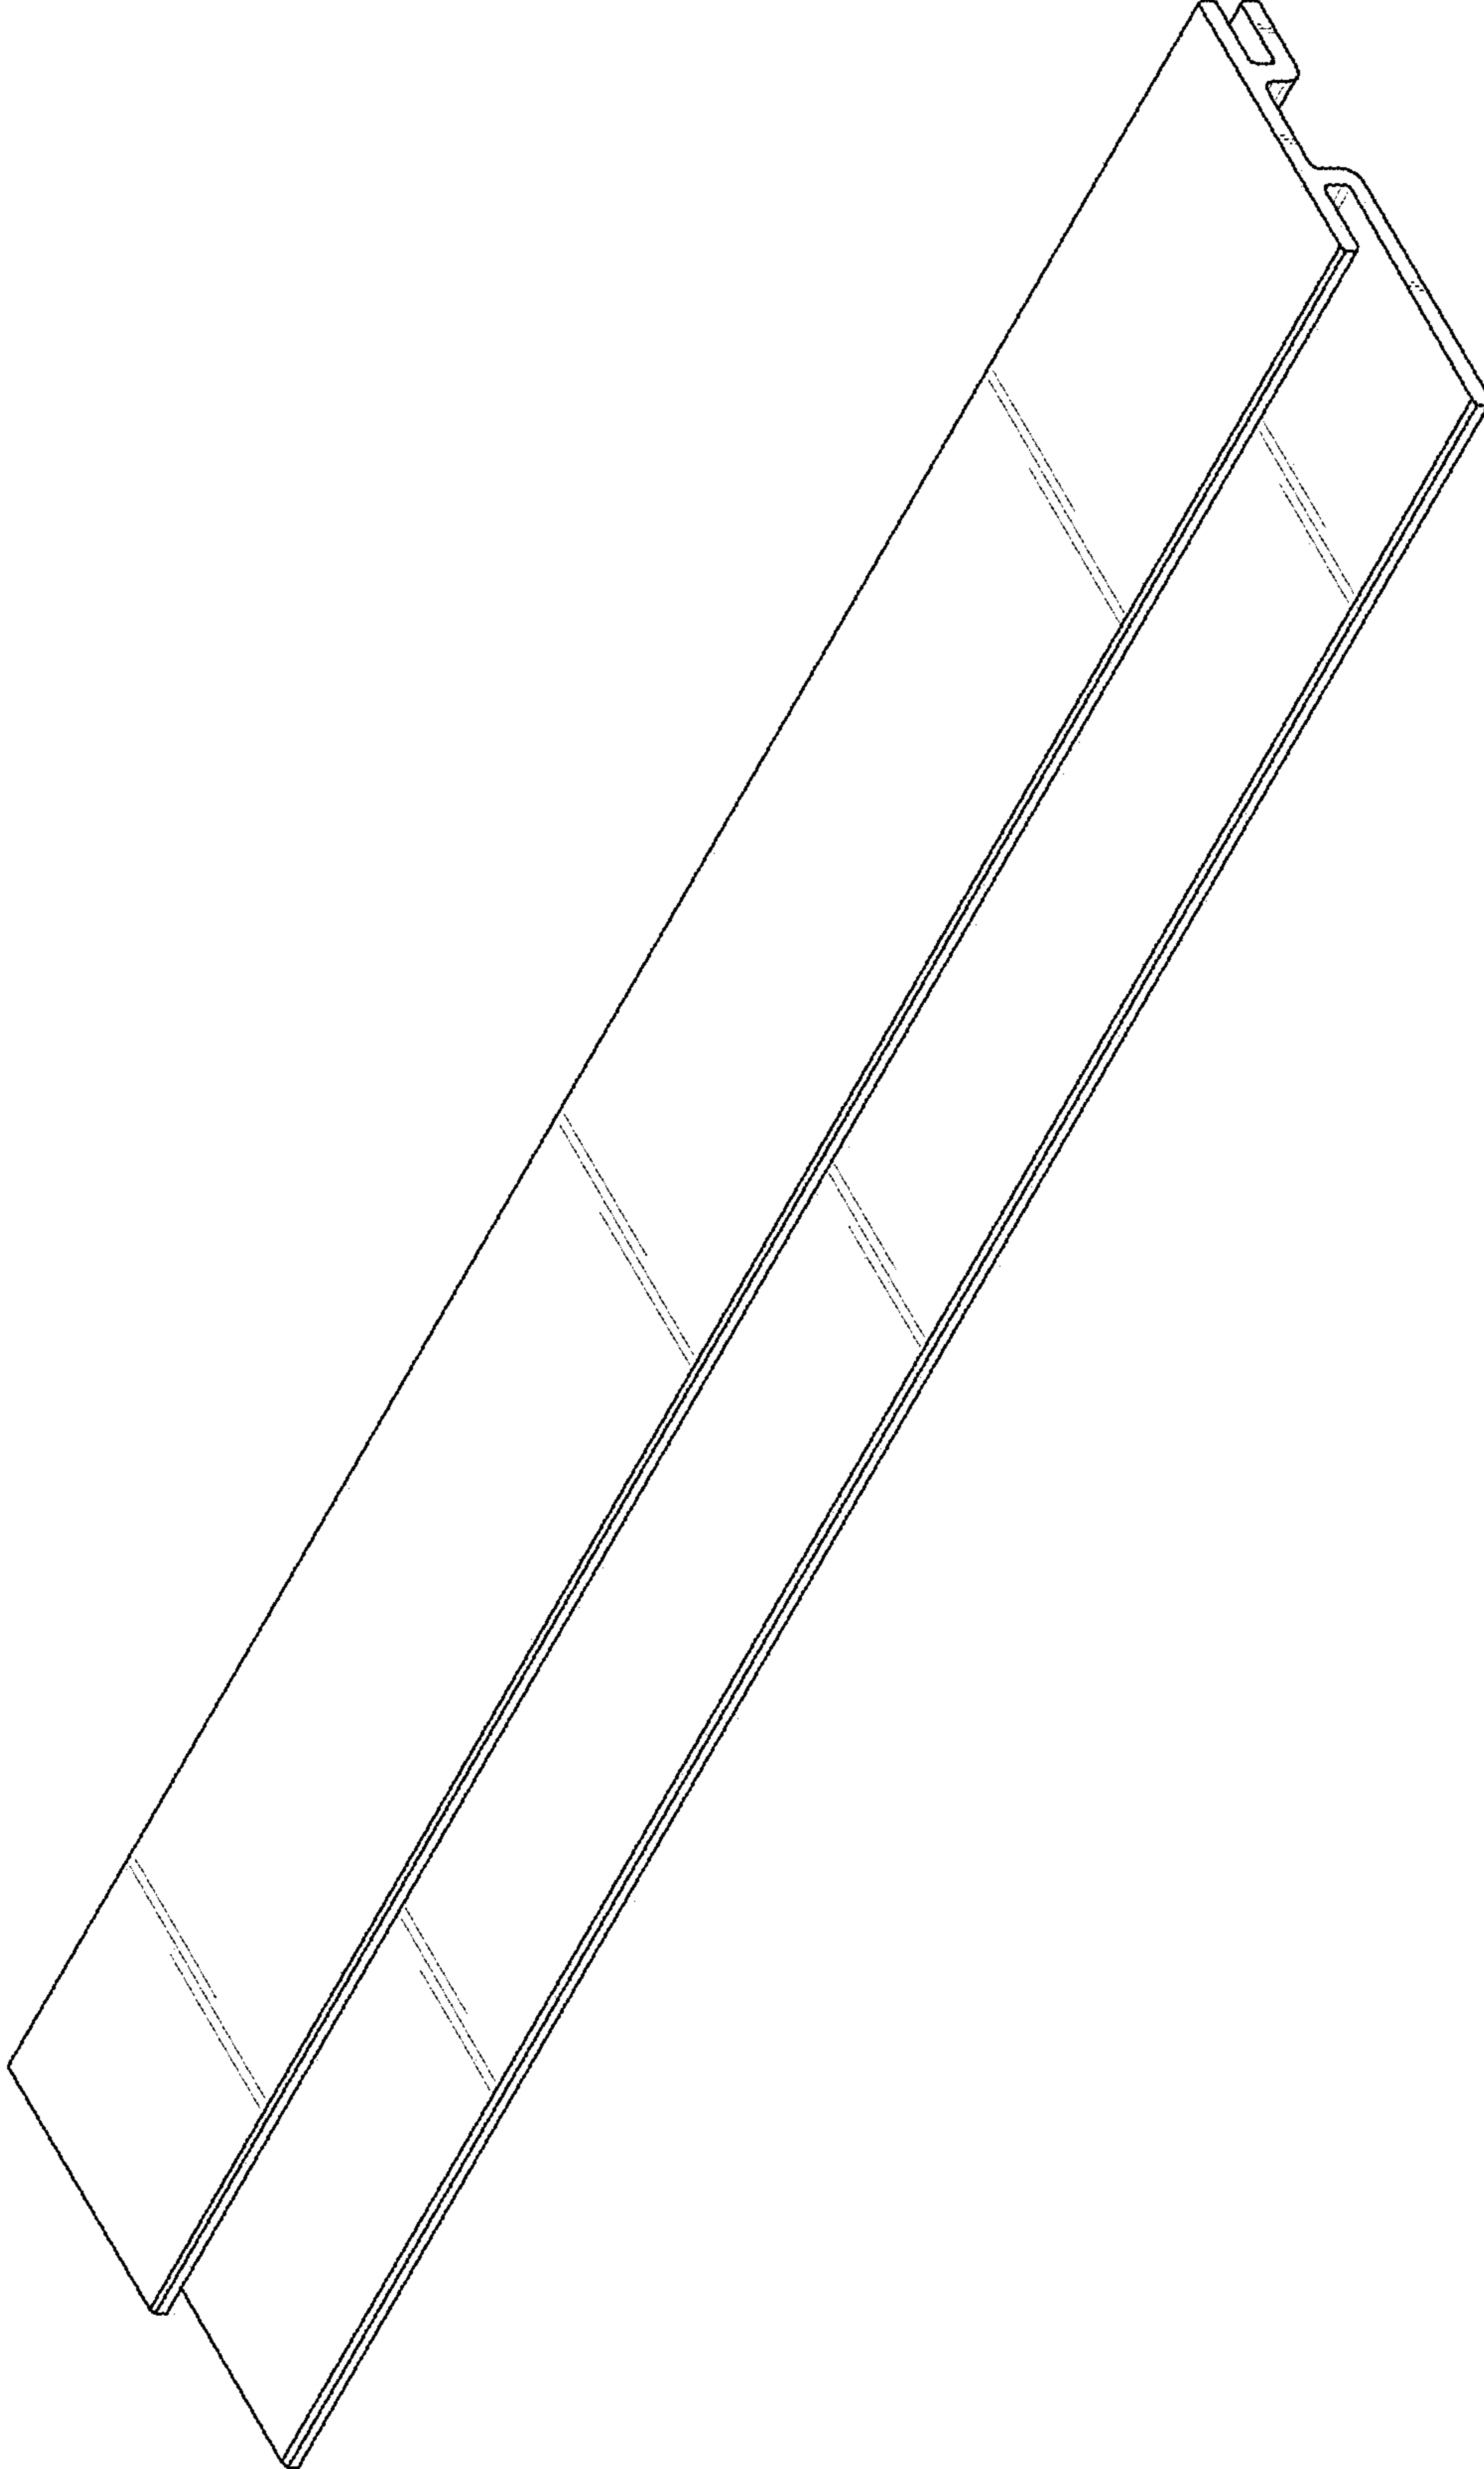


FIG. 1



FIG. 2



FIG. 3

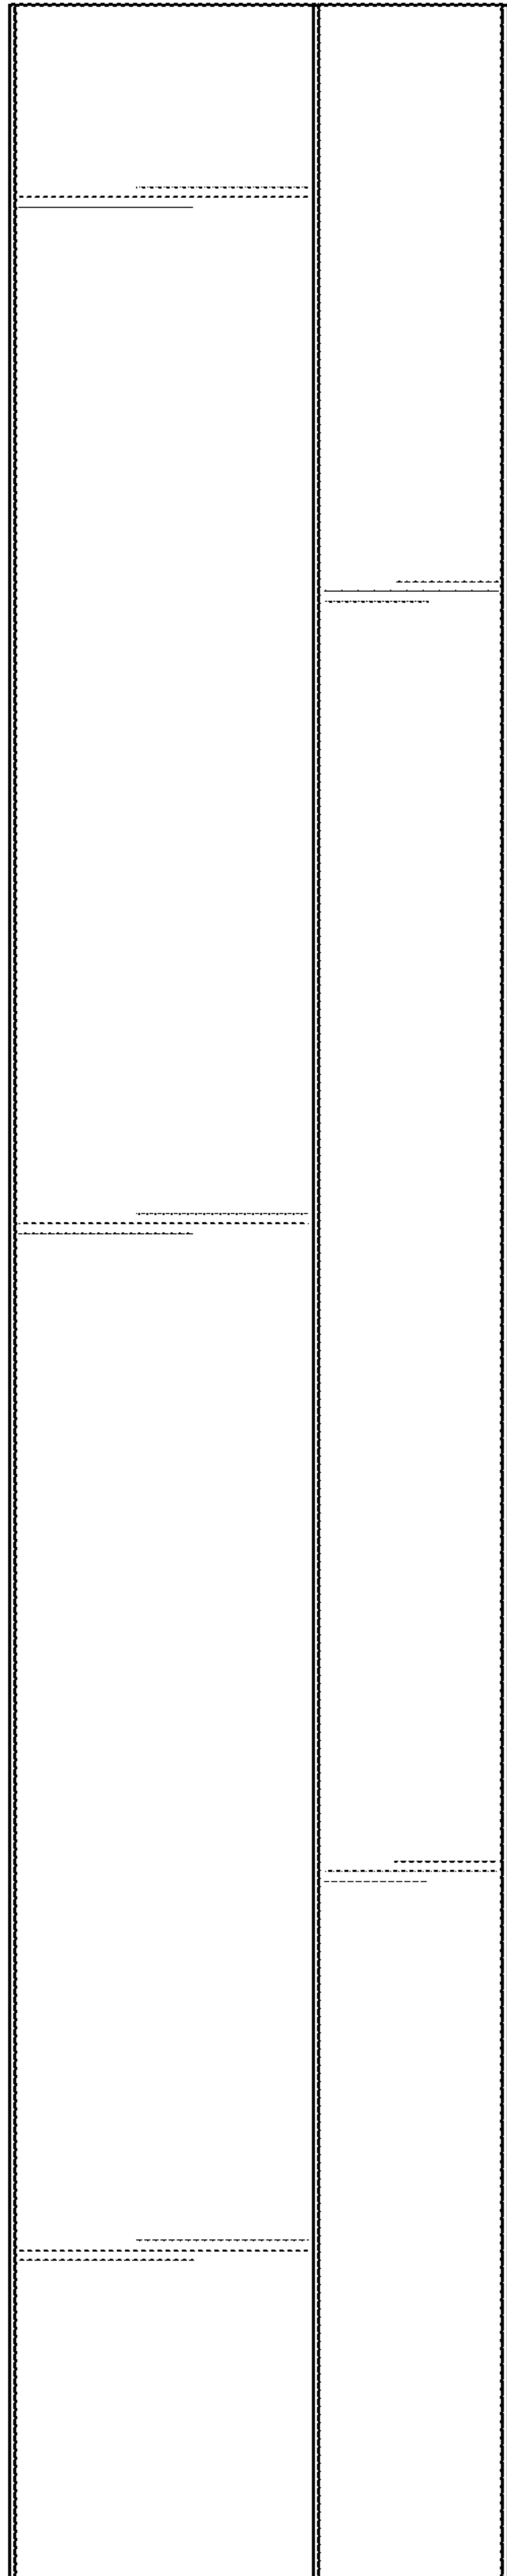


FIG. 4

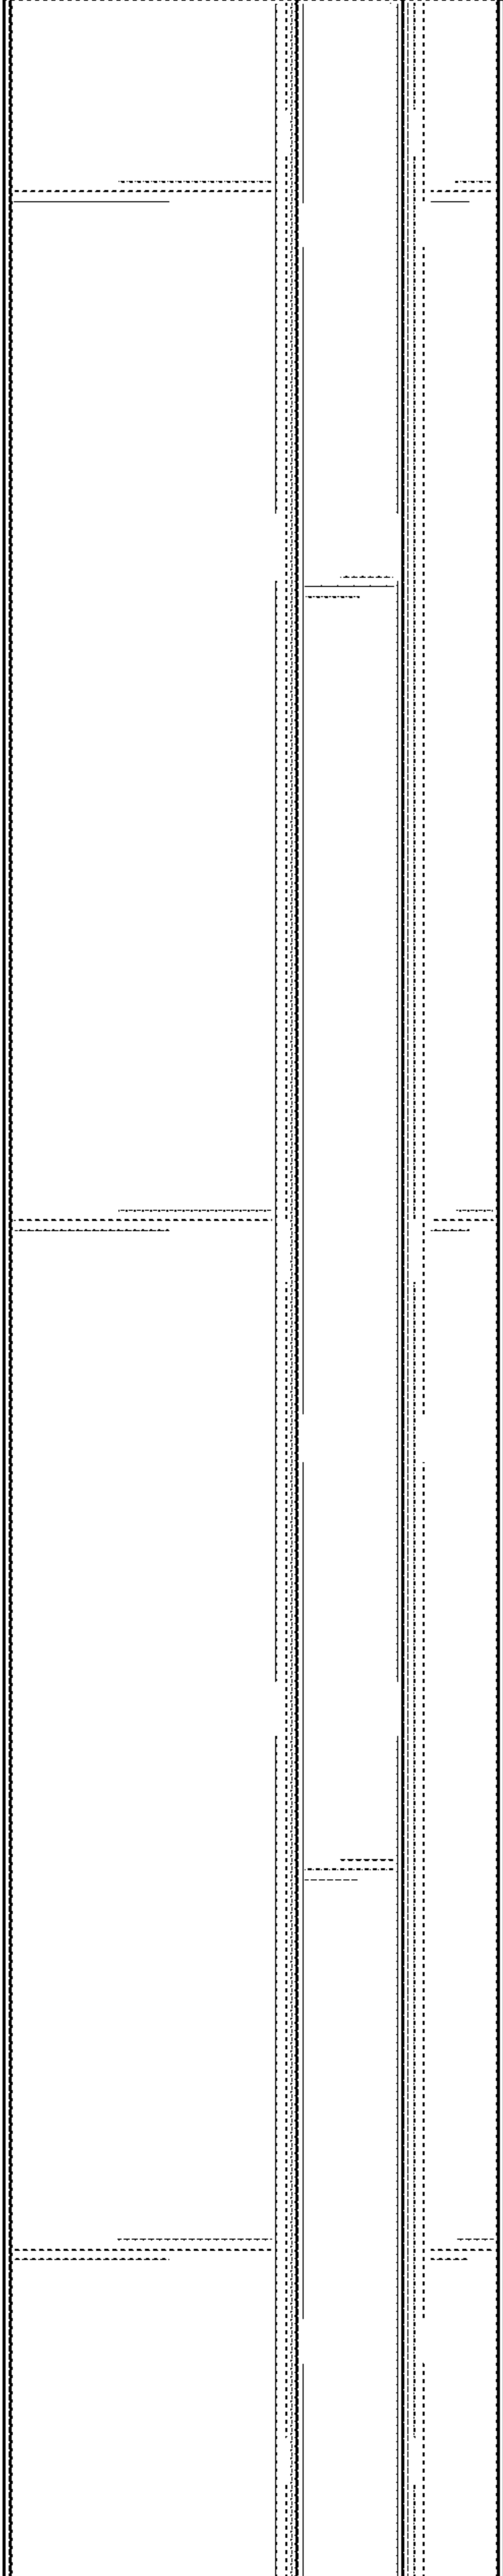


FIG. 5



FIG. 6