



US00D987109S

(12) **United States Design Patent** (10) **Patent No.:** **US D987,109 S**  
**Kovacs** (45) **Date of Patent:** **\*\* May 23, 2023**

(54) **EXTRUDED BASE PLATE FOR AN OPERATING ROOM TABLE**

(71) Applicant: **INNOVATIVE MEDICAL PRODUCTS, INC.**, Plainville, CT (US)

(72) Inventor: **Tamas Kovacs**, Burlington, CT (US)

(73) Assignee: **INDUSTRIAL FLOW SOLUTIONS, INC.**, Plainville, CT (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/799,669**

(22) Filed: **Jul. 15, 2021**

(51) **LOC (14) Cl.** ..... **24-99**

(52) **U.S. Cl.**  
USPC ..... **D24/231**; D24/183; D24/184

(58) **Field of Classification Search**  
USPC ..... D24/127, 128, 171, 172, 183, 184, 227, D24/231, 234; D8/20, 377  
CPC ..... A61B 6/0407; A61B 5/704; A61B 90/50; A61B 2090/571; A61B 2034/2055  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 2,829,640 A \* 4/1958 Moorman ..... A61G 13/12 378/208
- D240,707 S \* 7/1976 Rudinski ..... D8/377
- D252,668 S \* 8/1979 Rudinski ..... D25/119
- 4,232,681 A 11/1980 Tulaszewski
- 4,653,482 A \* 3/1987 Kurland ..... A61G 13/12 5/601
- 5,826,286 A \* 10/1998 Cranston ..... A61G 13/04 5/942
- 6,058,534 A 5/2000 Navarro et al.
- D439,670 S \* 3/2001 Sommer ..... D24/183
- D502,090 S \* 2/2005 Castellanos ..... D8/377
- D543,094 S \* 5/2007 Remmers ..... D8/377

- D585,267 S \* 1/2009 Di Vinadio ..... D8/377
  - D611,743 S \* 3/2010 Mitten ..... D8/377
  - 7,971,298 B2 \* 7/2011 Kobuß ..... A61B 6/0442 5/621
  - 8,146,874 B2 \* 4/2012 Yu ..... A61G 7/0503 248/316.4
  - D731,068 S \* 6/2015 Moon ..... D24/183
- (Continued)

FOREIGN PATENT DOCUMENTS

JP D1724704 \* 9/2022

OTHER PUBLICATIONS

IFU-IMP-0003 Quad® Clamp. Feb. 3, 2021. Site visited Dec. 16, 2022. [<https://www.impmedical.com/surgical-positioning/knee-positioner/De-Mayo-Adapt2Fit-surgical-knee-positioning-leg-holder>] (Year: 2021).\*

(Continued)

*Primary Examiner* — Wendy L Arminio  
*Assistant Examiner* — Maheen Khurshid  
(74) *Attorney, Agent, or Firm* — Damian Wasserbauer, Esq.; Nicholas E. Blanton; Wasserbauer Law LLC


(57) **CLAIM**

The ornamental design for an extruded base plate for an operating room table, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, top, right side perspective view of the extruded base plate for an operating room table in accordance with the present invention;  
FIG. 2 is a front view thereof;  
FIG. 3 is a rear view thereof;  
FIG. 4 is a top view thereof;  
FIG. 5 is a bottom view thereof; and,  
FIG. 6 is a right side view thereof, wherein the left side view is a mirror image thereof.

**1 Claim, 6 Drawing Sheets**

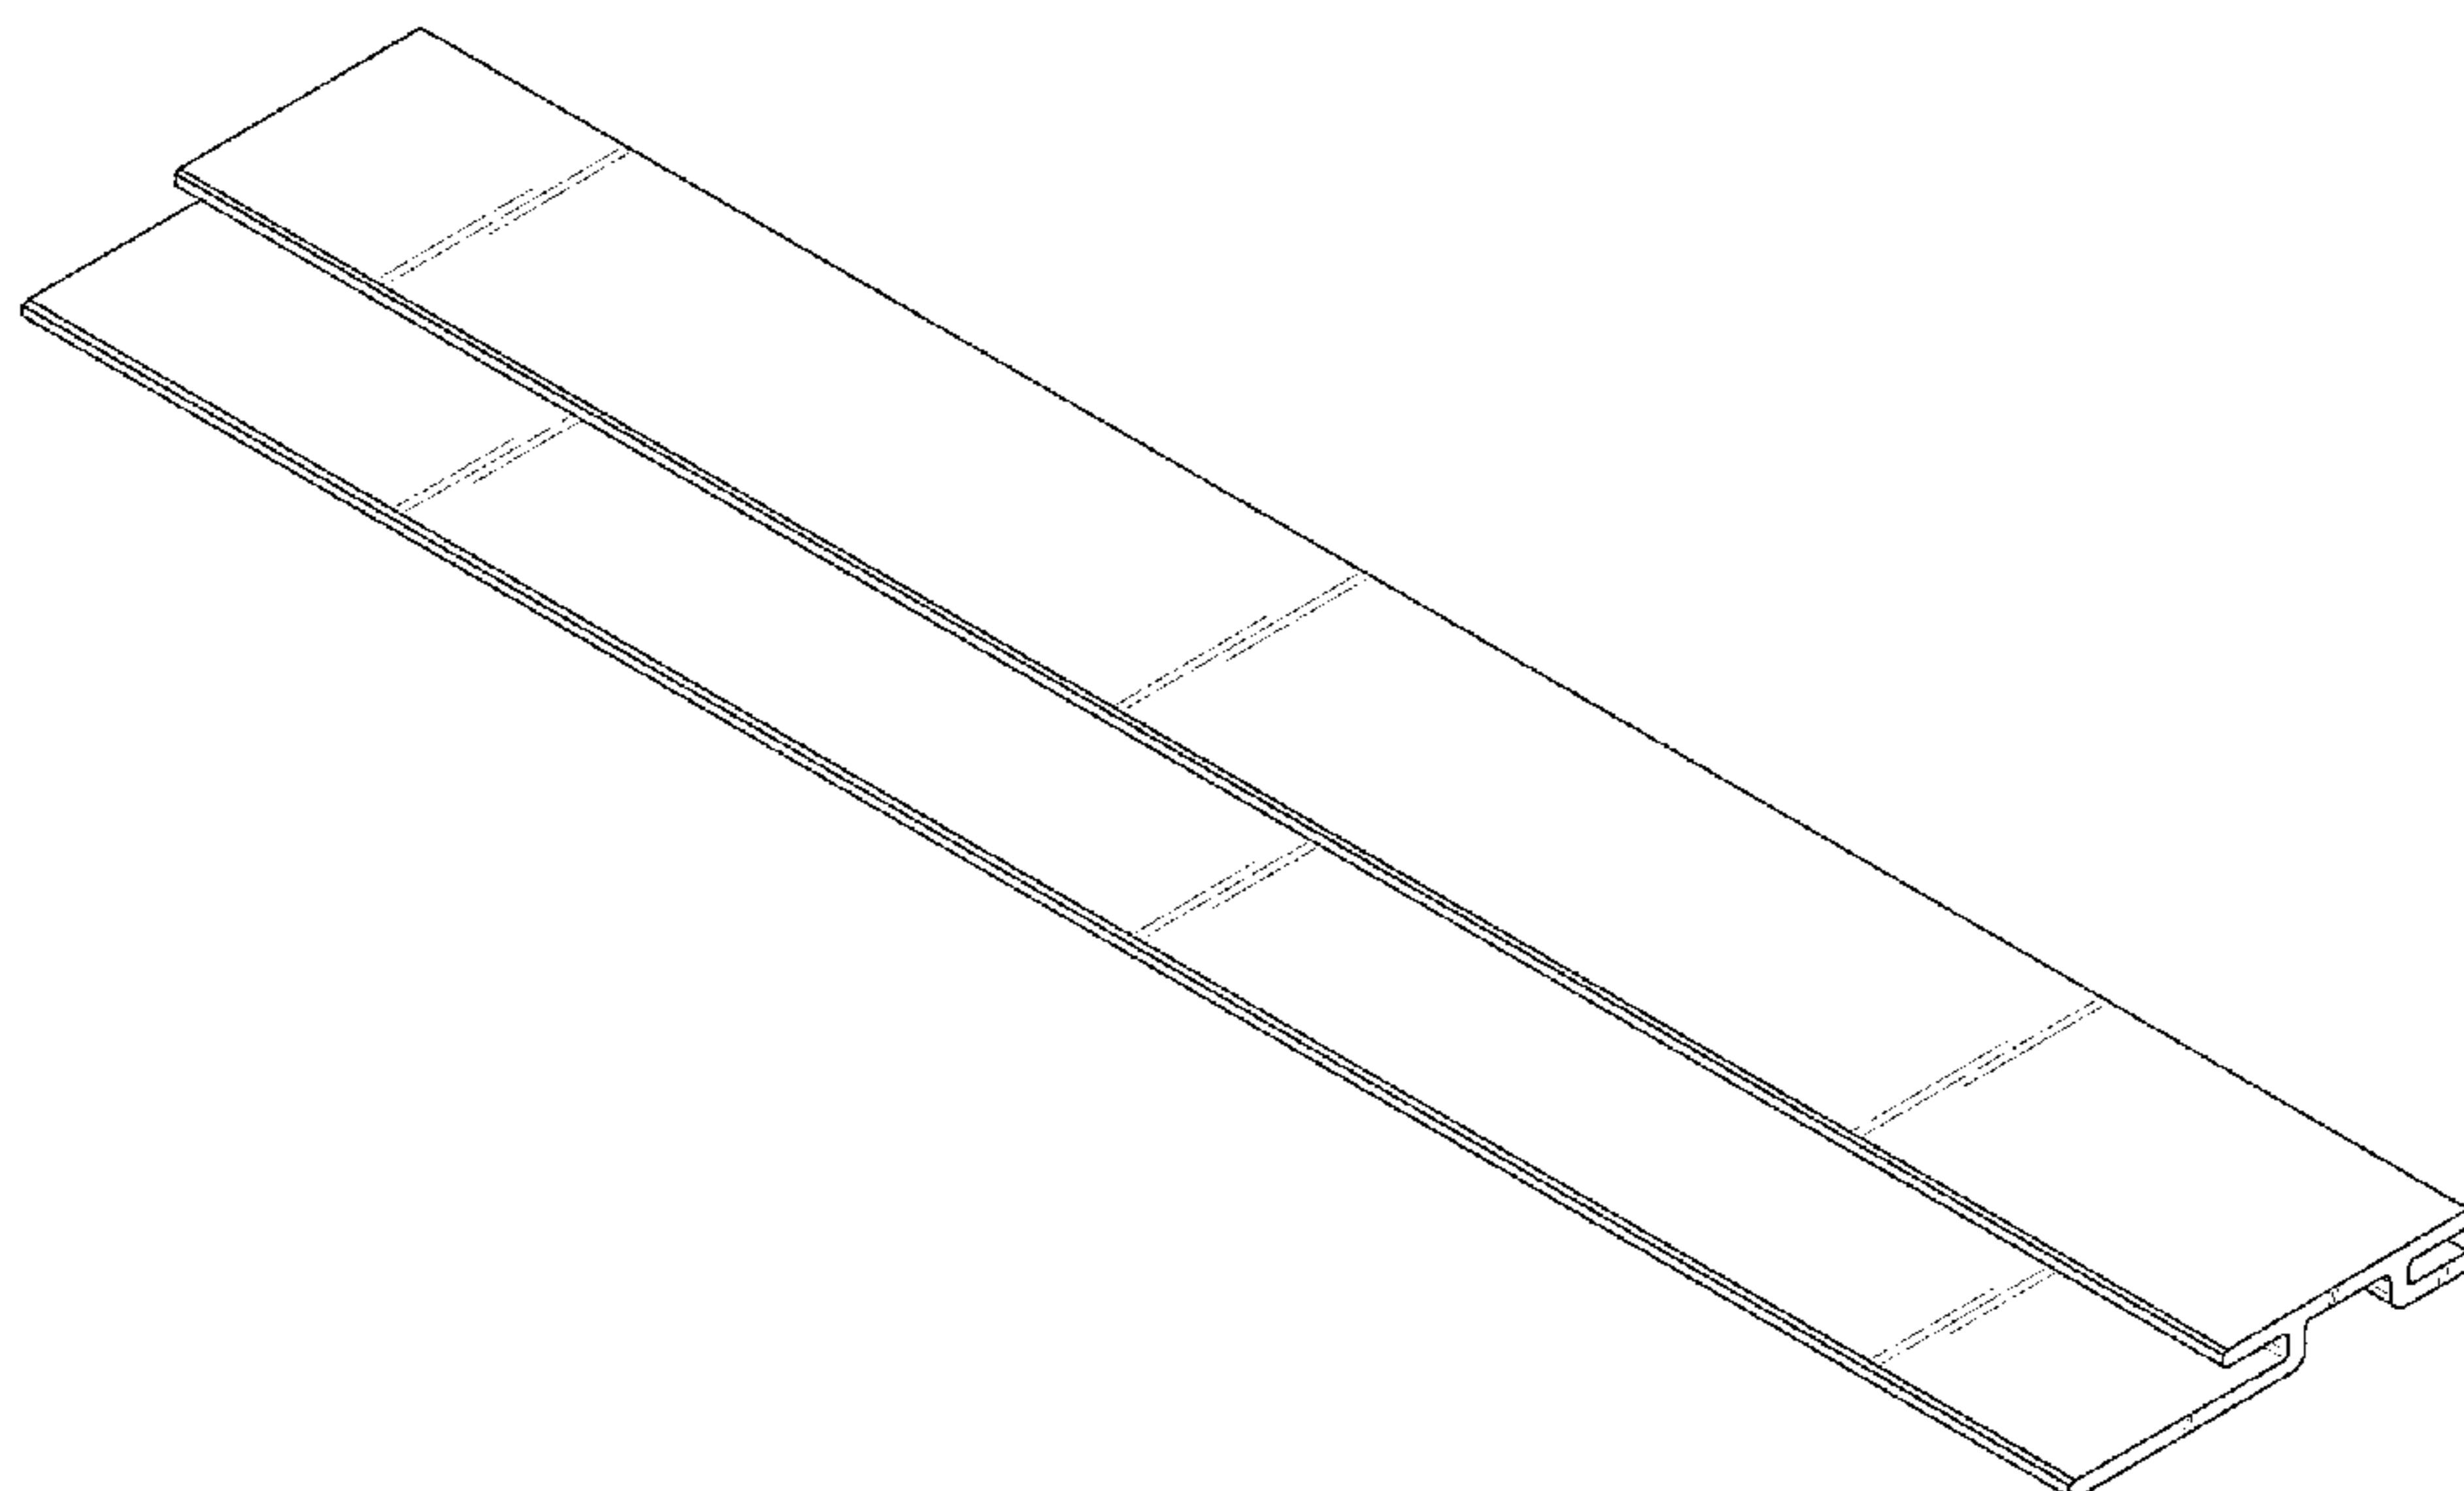

(56)

**References Cited**

U.S. PATENT DOCUMENTS

|              |      |         |                |       |                        |
|--------------|------|---------|----------------|-------|------------------------|
| D755,041     | S *  | 5/2016  | Weldon         | ..... | D8/377                 |
| 9,603,765    | B2   | 3/2017  | Kreuzer et al. |       |                        |
| 9,615,987    | B2   | 4/2017  | Worm et al.    |       |                        |
| 9,642,762    | B2 * | 5/2017  | Frueh          | ..... | A61G 7/08              |
| D791,348     | S *  | 7/2017  | Singh          | ..... | D25/119                |
| D791,354     | S *  | 7/2017  | Singh          | ..... | D25/119                |
| D813,636     | S *  | 3/2018  | Hsieh          | ..... | D8/71                  |
| D834,928     | S *  | 12/2018 | Lu             | ..... | D8/381                 |
| D838,857     | S *  | 1/2019  | Blackwell      | ..... | D24/184                |
| D844,807     | S *  | 4/2019  | Blackwell      | ..... | D24/231                |
| D872,884     | S *  | 1/2020  | Carter         | ..... | D25/119                |
| D909,179     | S *  | 2/2021  | Kovacs         | ..... | D8/349                 |
| 10,912,697   | B2 * | 2/2021  | Staudinger     | ..... | A61G 13/02             |
| D920,769     | S *  | 6/2021  | Kovacs         | ..... | D25/164                |
| 11,083,420   | B2 * | 8/2021  | Suga           | ..... | A61B 6/0407            |
| D948,998     | S *  | 4/2022  | Noe            | ..... | D25/119                |
| 2016/0151223 | A1 * | 6/2016  | Ferro          | ..... | A61G 13/129<br>128/845 |

OTHER PUBLICATIONS

SchureMed TKR Positioner. 2009. Site visited Dec. 16, 2022. [[https://www.universalmedicalinc.com/tkr-positioner-for-total-knee-replacement.html?campaignid=1821462889&adgroupid=70633908718&adid=345215573729&gclid=EA1a1QobChMlrZDKIqH--wIVGpflCh3EygSNEAAYASABEgK2bPD\\_BwE](https://www.universalmedicalinc.com/tkr-positioner-for-total-knee-replacement.html?campaignid=1821462889&adgroupid=70633908718&adid=345215573729&gclid=EA1a1QobChMlrZDKIqH--wIVGpflCh3EygSNEAAYASABEgK2bPD_BwE)] (Year: 2009).\*

TKR Positioner. Apr. 7, 2021. Site visited Dec. 16, 2022. [[https://www.youtube.com/watch?v=\\_ZduRUDweUA](https://www.youtube.com/watch?v=_ZduRUDweUA)] (Year: 2021).\*

\* cited by examiner

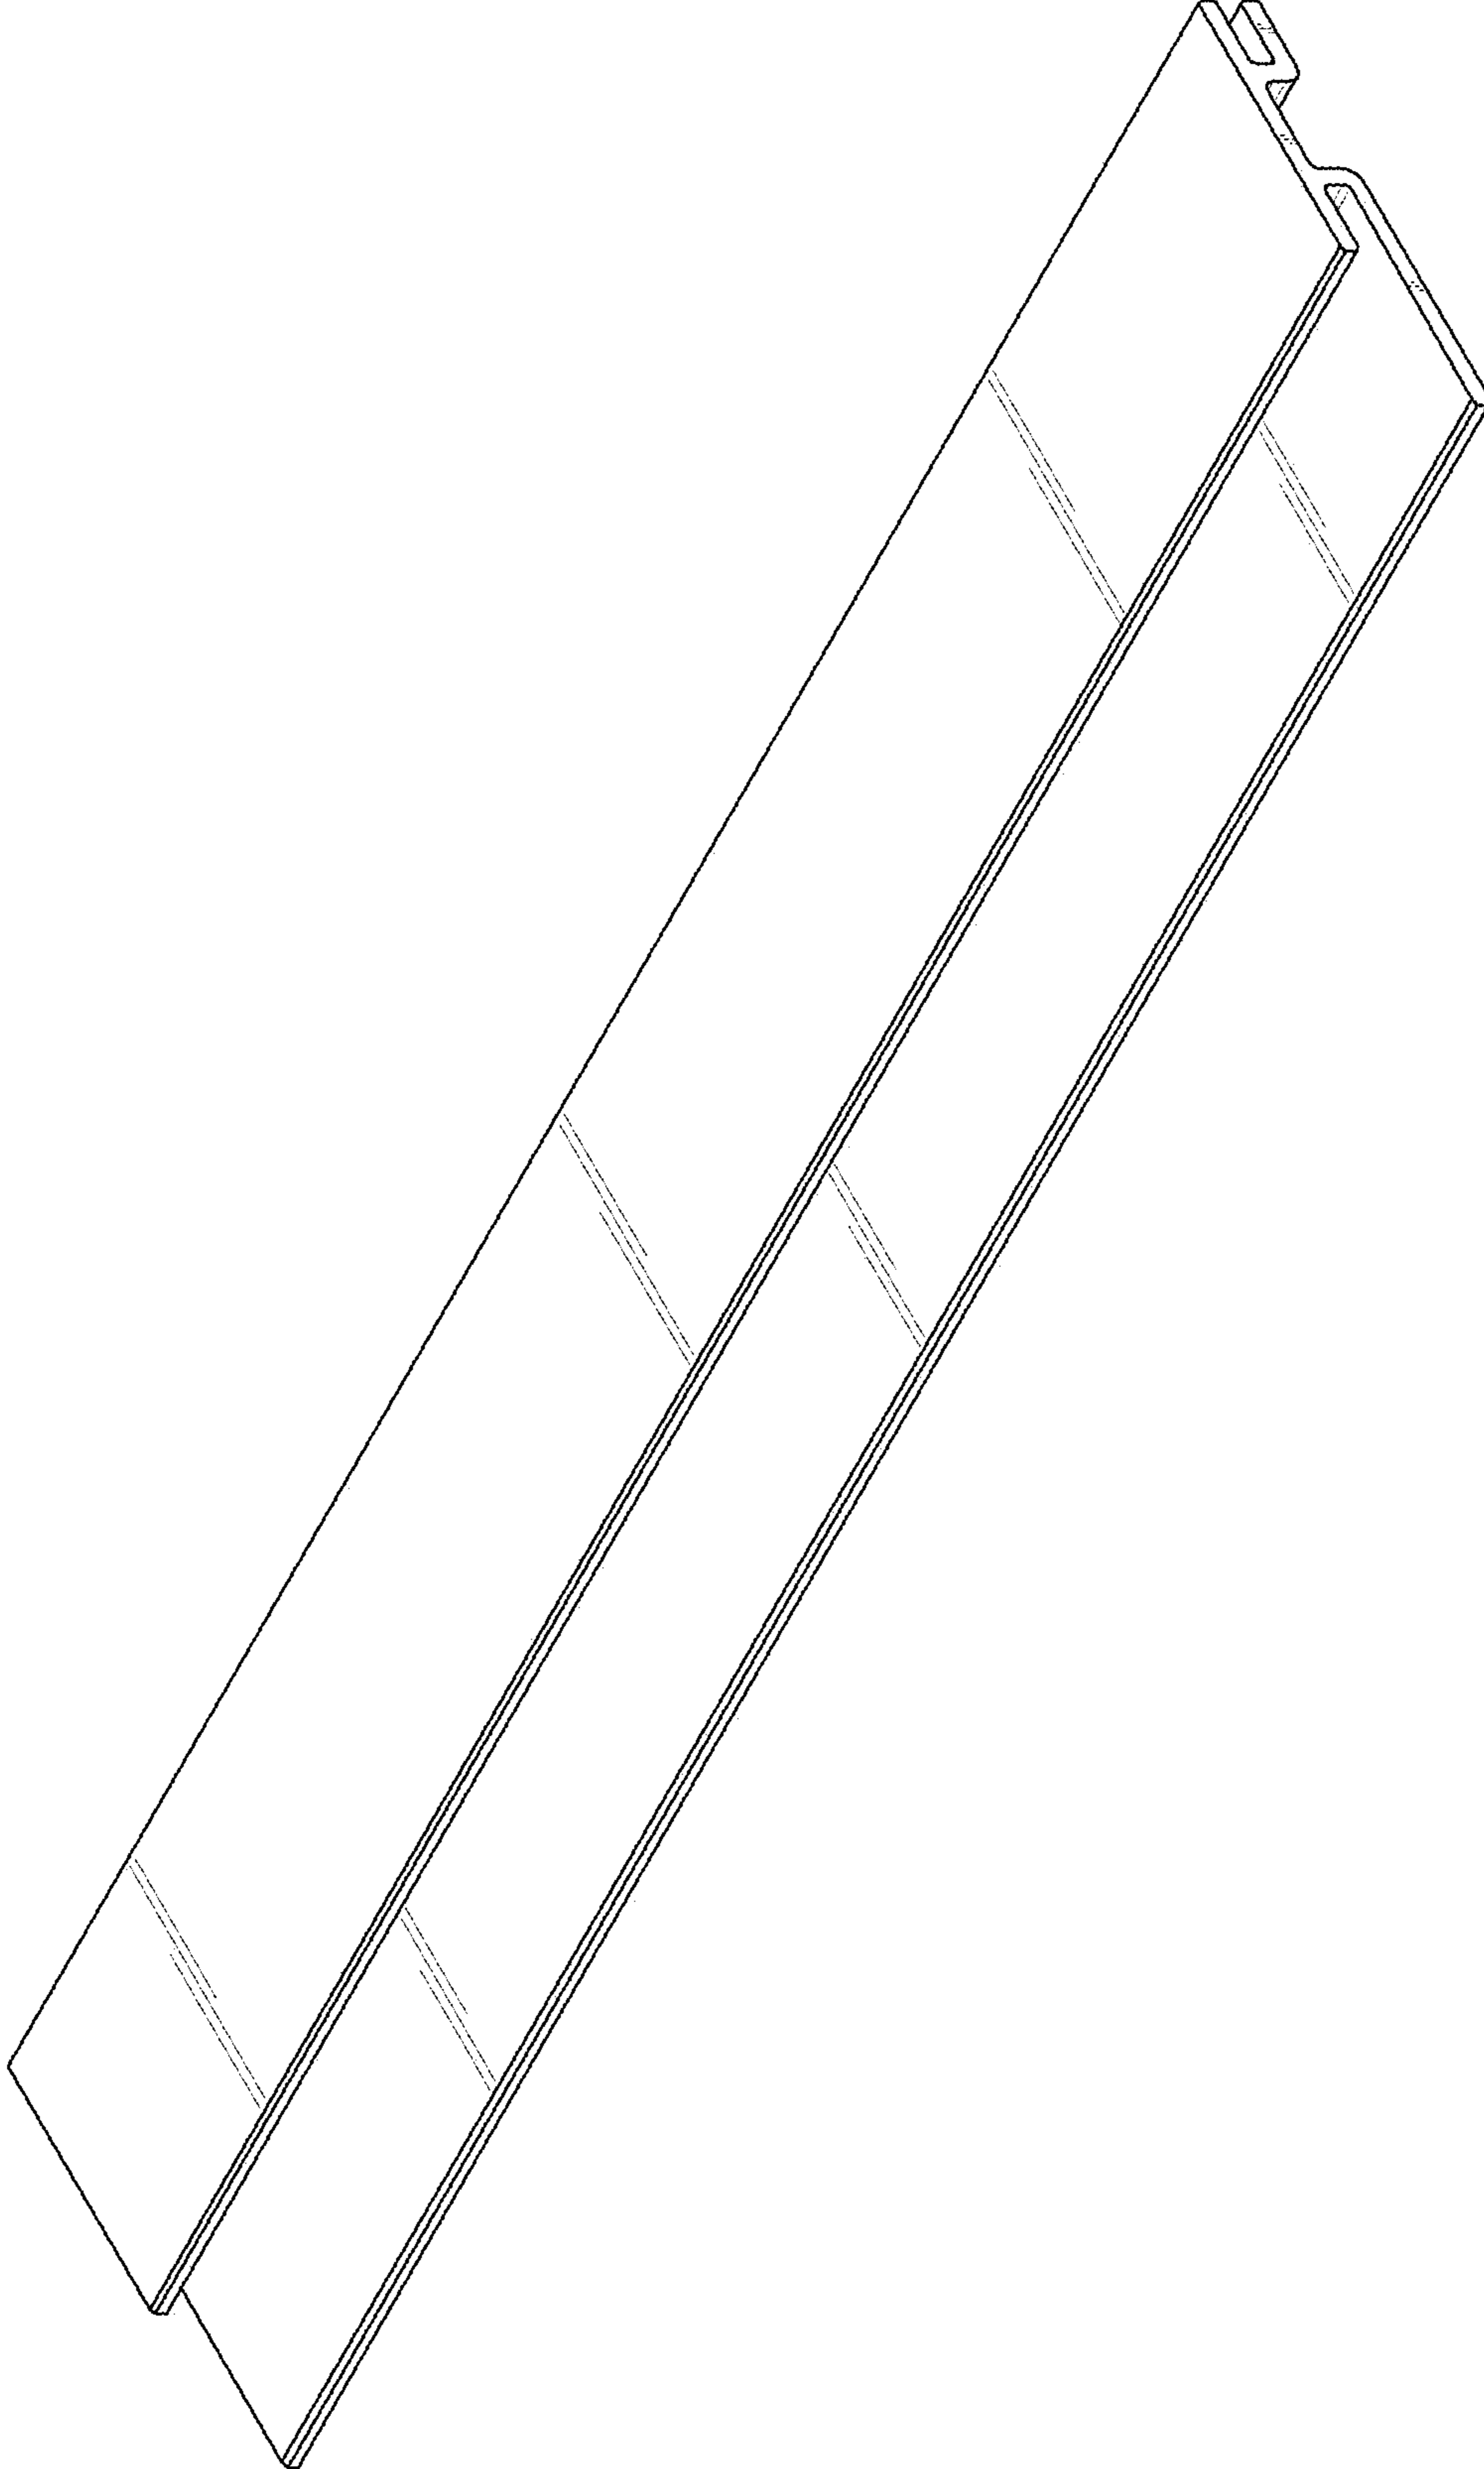


FIG. 1



FIG. 2



FIG. 3

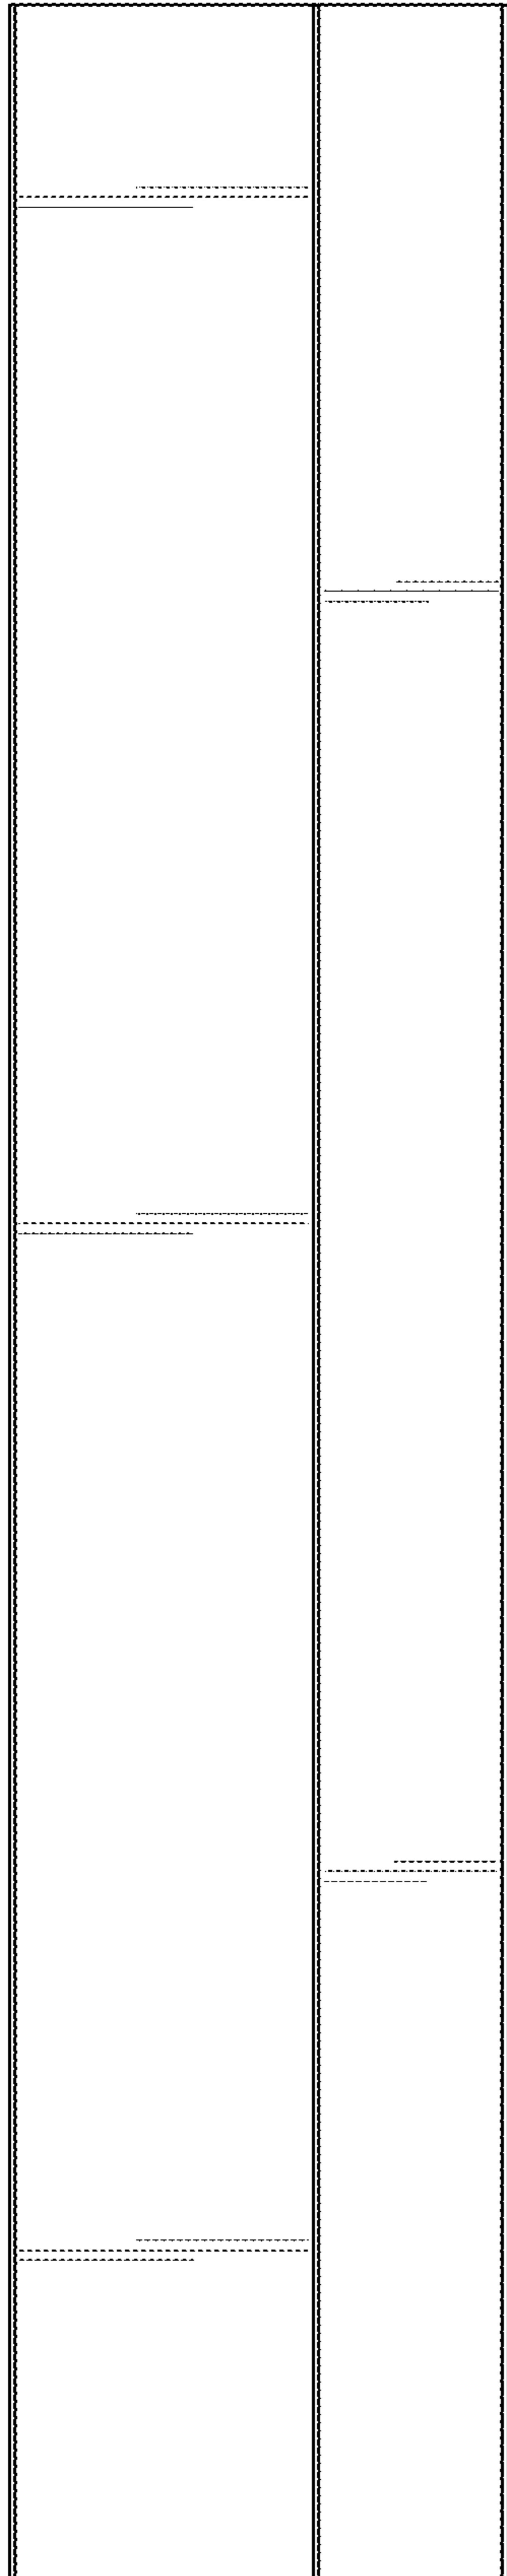


FIG. 4

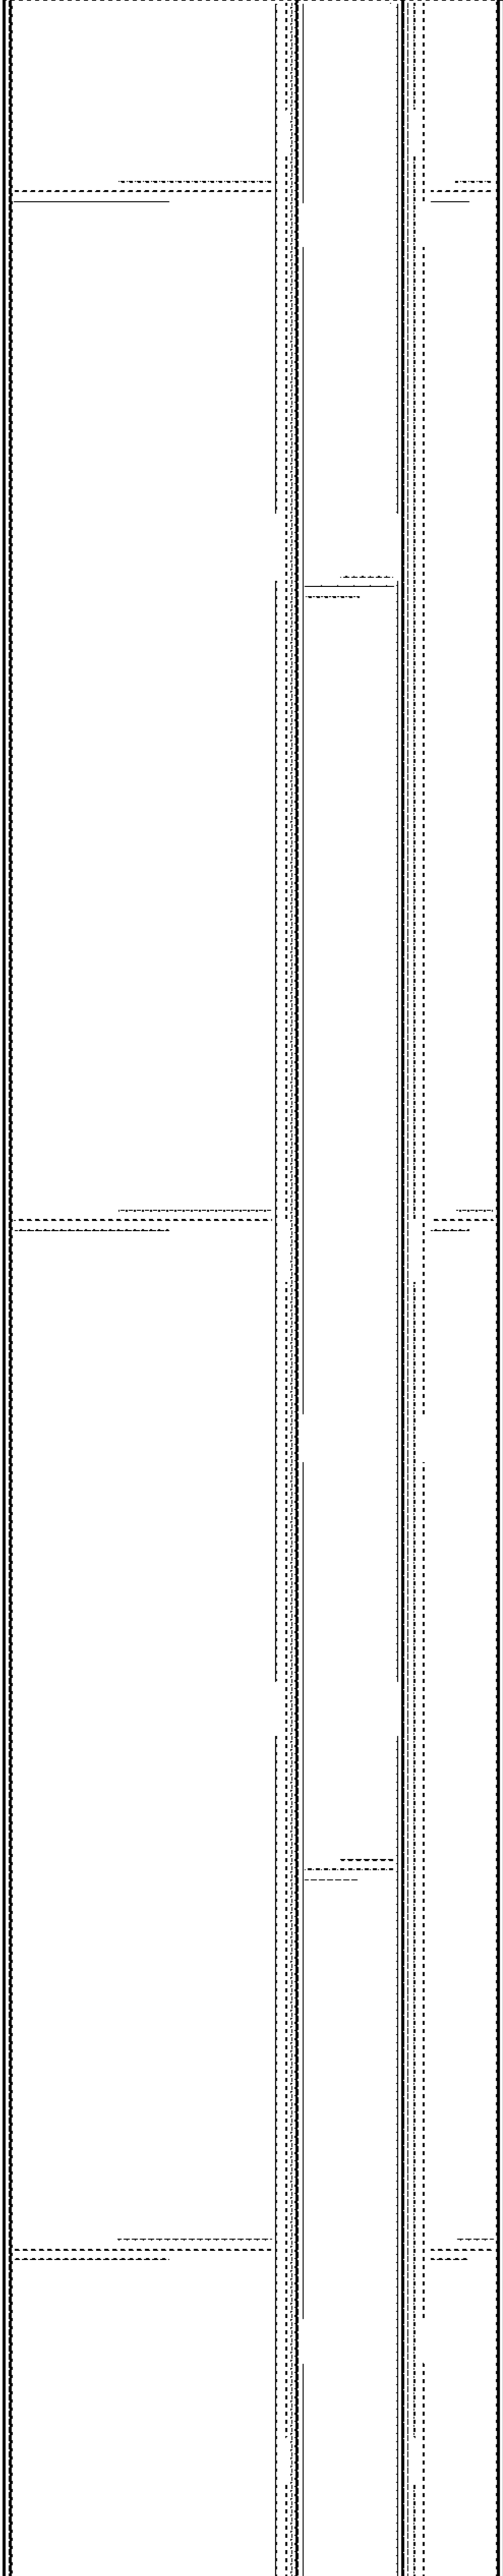


FIG. 5



FIG. 6