



US00D989298S

(12) **United States Design Patent** (10) **Patent No.:** **US D989,298 S**  
**Slaby et al.** (45) **Date of Patent:** **\*\* Jun. 13, 2023**

(54) **INFUSION PUMP RACK**

(71) Applicants: **BAXTER INTERNATIONAL INC.**,  
Deerfield, IL (US); **BAXTER**  
**HEALTHCARE SA**, Glattpark (CH)  
(72) Inventors: **Jiri Slaby**, Buffalo Grove, IL (US);  
**Troy David Heavelyn**, Grayslake, NY  
(US); **Jing Li**, Libertyville, IL (US);  
**Aaron Hexamer**, Grayslake, IL (US);  
**Mark Andrew Luzbetak**, Kildeer, IL  
(US); **Ken Powers**, Evanston, IL (US);  
**Andrew Kellock**, Mitcham Victoria  
(AU); **Ulf Quensel**, Ystad (SE); **Robert**  
**Cuevas**, Twin Lakes, WI (US); **David**  
**Gorgi**, Schaumburg, IL (US)

(73) Assignees: **BAXTER INTERNATIONAL INC.**,  
Deerfield, IL (US); **BAXTER**  
**HEALTHCARE SA**, Glattpark (CH)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/769,501**

(22) Filed: **Feb. 5, 2021**

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/185**

(58) **Field of Classification Search**  
USPC ..... D24/108, 111, 127-129, 227-229, 231,  
D24/234; D6/672, 673, 677, 677.1, 702,  
D6/705, 705.1

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D426,092 S \* 6/2000 Neustadt ..... D6/705  
D459,137 S \* 6/2002 Poirier ..... D6/677.1

(Continued)

**FOREIGN PATENT DOCUMENTS**

GB 6152738 \* 8/2021  
NZ 429275-0001 \* 2/2021

**OTHER PUBLICATIONS**

DI-4000 Standalone rack, Trade Korea, [Post date: Mar. 16, 2017],  
[Site seen Aug. 9, 2022], Seen at URL: <https://www.tradekorea.com/product/detail/P475265/Volumetric-Infusion-Pump.html> (Year:  
2017).\*

(Continued)

*Primary Examiner* — Natasha Vujcic  
*Assistant Examiner* — Gilbert B Ford  
(74) *Attorney, Agent, or Firm* — K&L Gates LLP


(57) **CLAIM**

We claim, the ornamental design for an infusion pump rack,  
as shown and described herein.

**DESCRIPTION**

FIG. 1 illustrates a perspective view of an infusion pump rack, according to one embodiment of the invention.  
FIG. 2 illustrates a front view of the infusion pump rack shown in FIG. 1.  
FIG. 3 illustrates a rear side view of the infusion pump rack shown in FIG. 1.  
FIG. 4 illustrates a left side view of the infusion pump rack shown in FIG. 1.  
FIG. 5 illustrates a right-side view of the infusion pump rack shown in FIG. 1.  
FIG. 6 illustrates a top view of the infusion pump rack shown in FIG. 1.  
FIG. 7 illustrates a bottom view of the infusion pump rack shown in FIG. 1.  
FIG. 8 illustrates a perspective view of an infusion pump rack, according to a second embodiment of the invention.  
FIG. 9 illustrates a front view of the infusion pump rack shown in FIG. 8.  
FIG. 10 illustrates a rear view of the infusion pump rack shown in FIG. 8.  
FIG. 11 illustrates a left side view of the infusion pump rack shown in FIG. 8.  
FIG. 12 illustrates a right-side view of the infusion pump rack shown in FIG. 8.  
FIG. 13 illustrates a top view of the infusion pump rack shown in FIG. 8; and,  
FIG. 14 illustrates a bottom view of the infusion pump rack shown in FIG. 8.

(Continued)

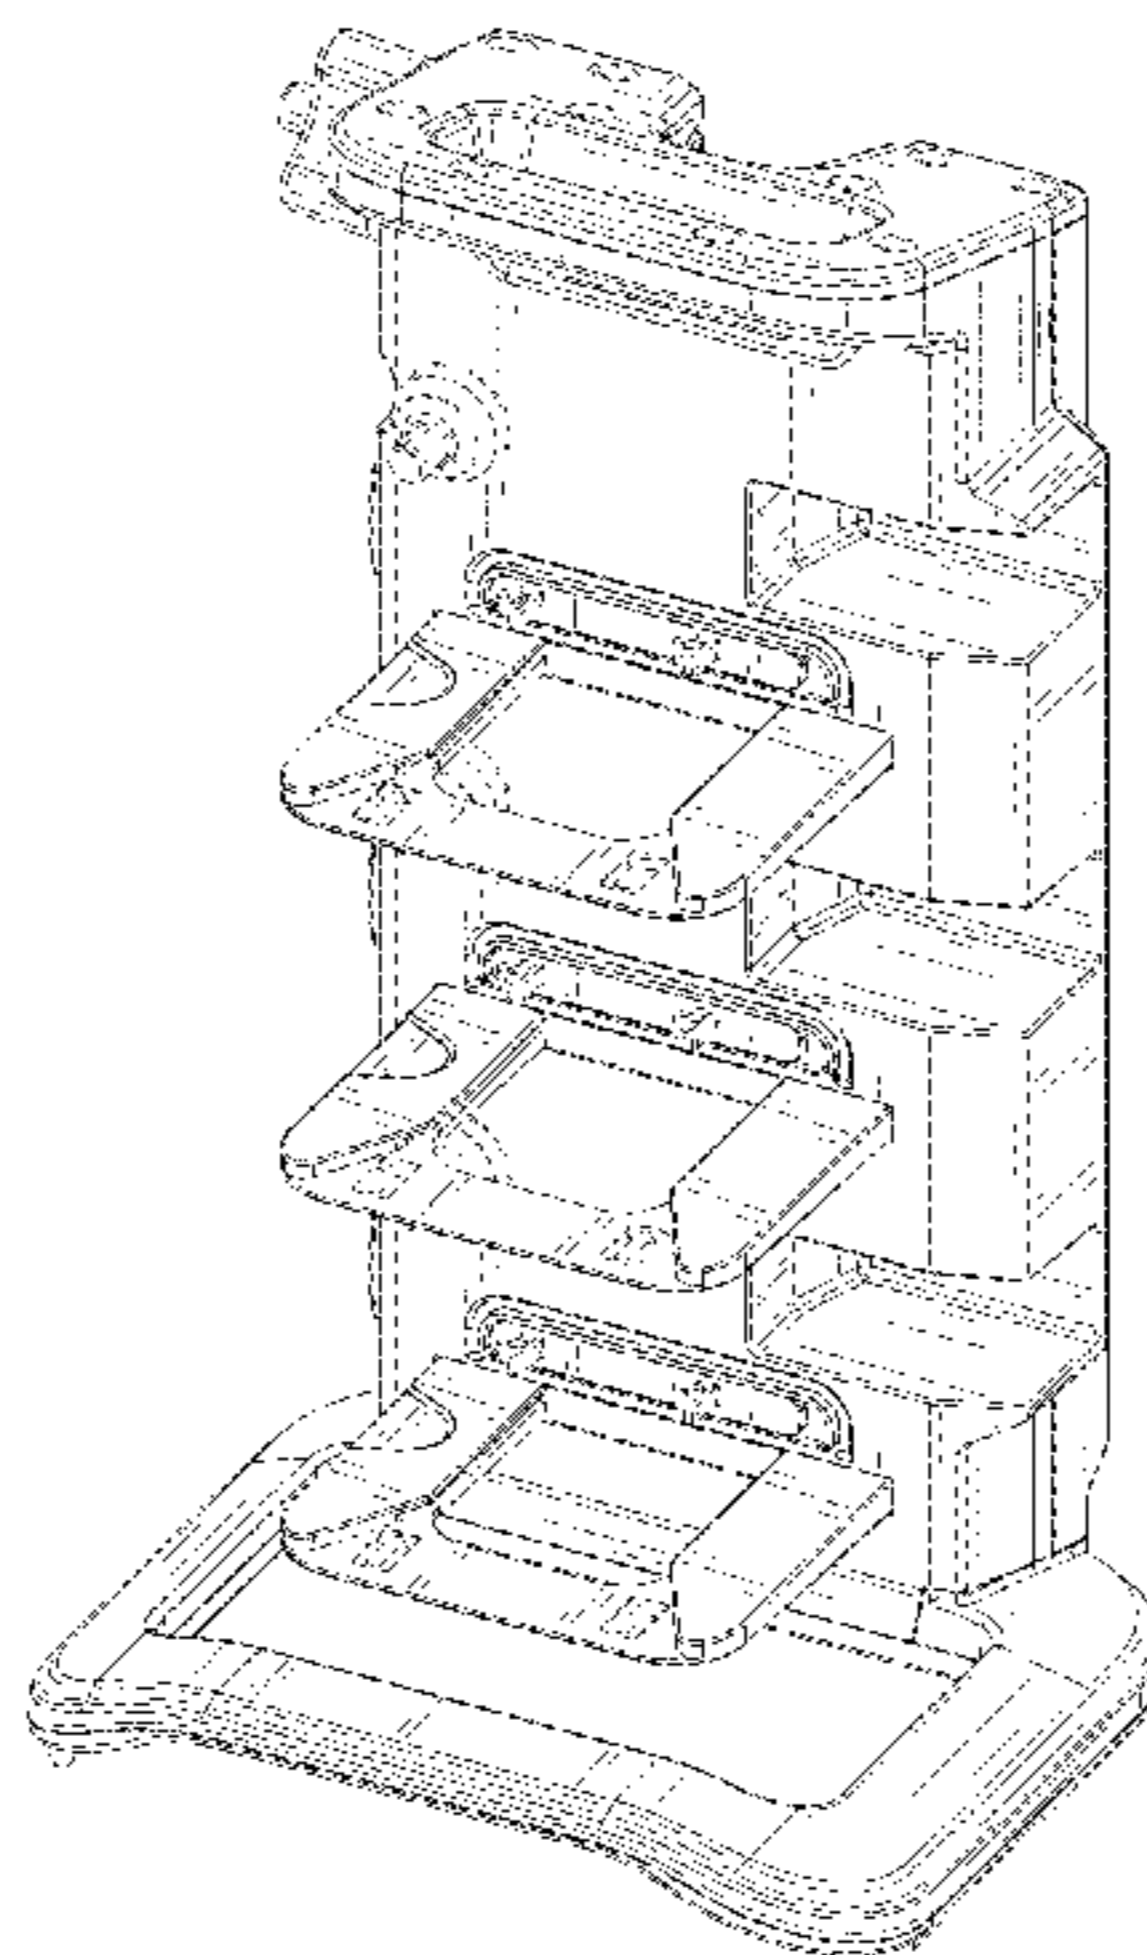

The broken lines in the drawings illustrate portions of the infusion pump rack and form no part of the claimed design. Additionally, the infusion pump rack is not limited to the scale shown herein.

**1 Claim, 14 Drawing Sheets**

**(58) Field of Classification Search**

CPC . A61M 5/1413; H05K 5/0021; H05K 7/1435;  
F16M 11/24; F16M 2200/027; A61B  
19/0256; G06F 19/3412; G06F 19/3468  
See application file for complete search history.

**(56) References Cited**

**U.S. PATENT DOCUMENTS**

6,407,335 B1 \* 6/2002 Franklin-Lees ..... F16M 13/02  
174/58  
D564,796 S \* 3/2008 Zambelli ..... D6/677.1

D700,704 S \* 3/2014 Kitt ..... D24/185  
D777,933 S \* 1/2017 Hrenchir ..... D24/185  
D810,958 S \* 2/2018 Lacy ..... D24/227  
9,987,415 B2 \* 6/2018 Asama ..... A61M 5/1417  
D860,464 S \* 9/2019 Caywood ..... D24/185  
D935,246 S \* 11/2021 Peng ..... D6/677.1  
D953,540 S \* 5/2022 Behrendt ..... D24/185  
2014/0321096 A1 \* 10/2014 Kajackas ..... A61G 12/00  
361/807  
2015/0041419 A1 \* 2/2015 Hasegawa ..... F16M 11/041  
248/676

**OTHER PUBLICATIONS**

MP-80 docking station with 6 channels, Medcaptain Medical Technology Co., Ltd, facebook, [Post date: Jun. 12, 2015], [Site seen Aug. 9, 2022], Seen at URL: <https://m.facebook.com/MedcaptainMedTech/photos/mp-80-docking-station-with-6-channels/1382577882043695/> (Year: 2015).\*

\* cited by examiner



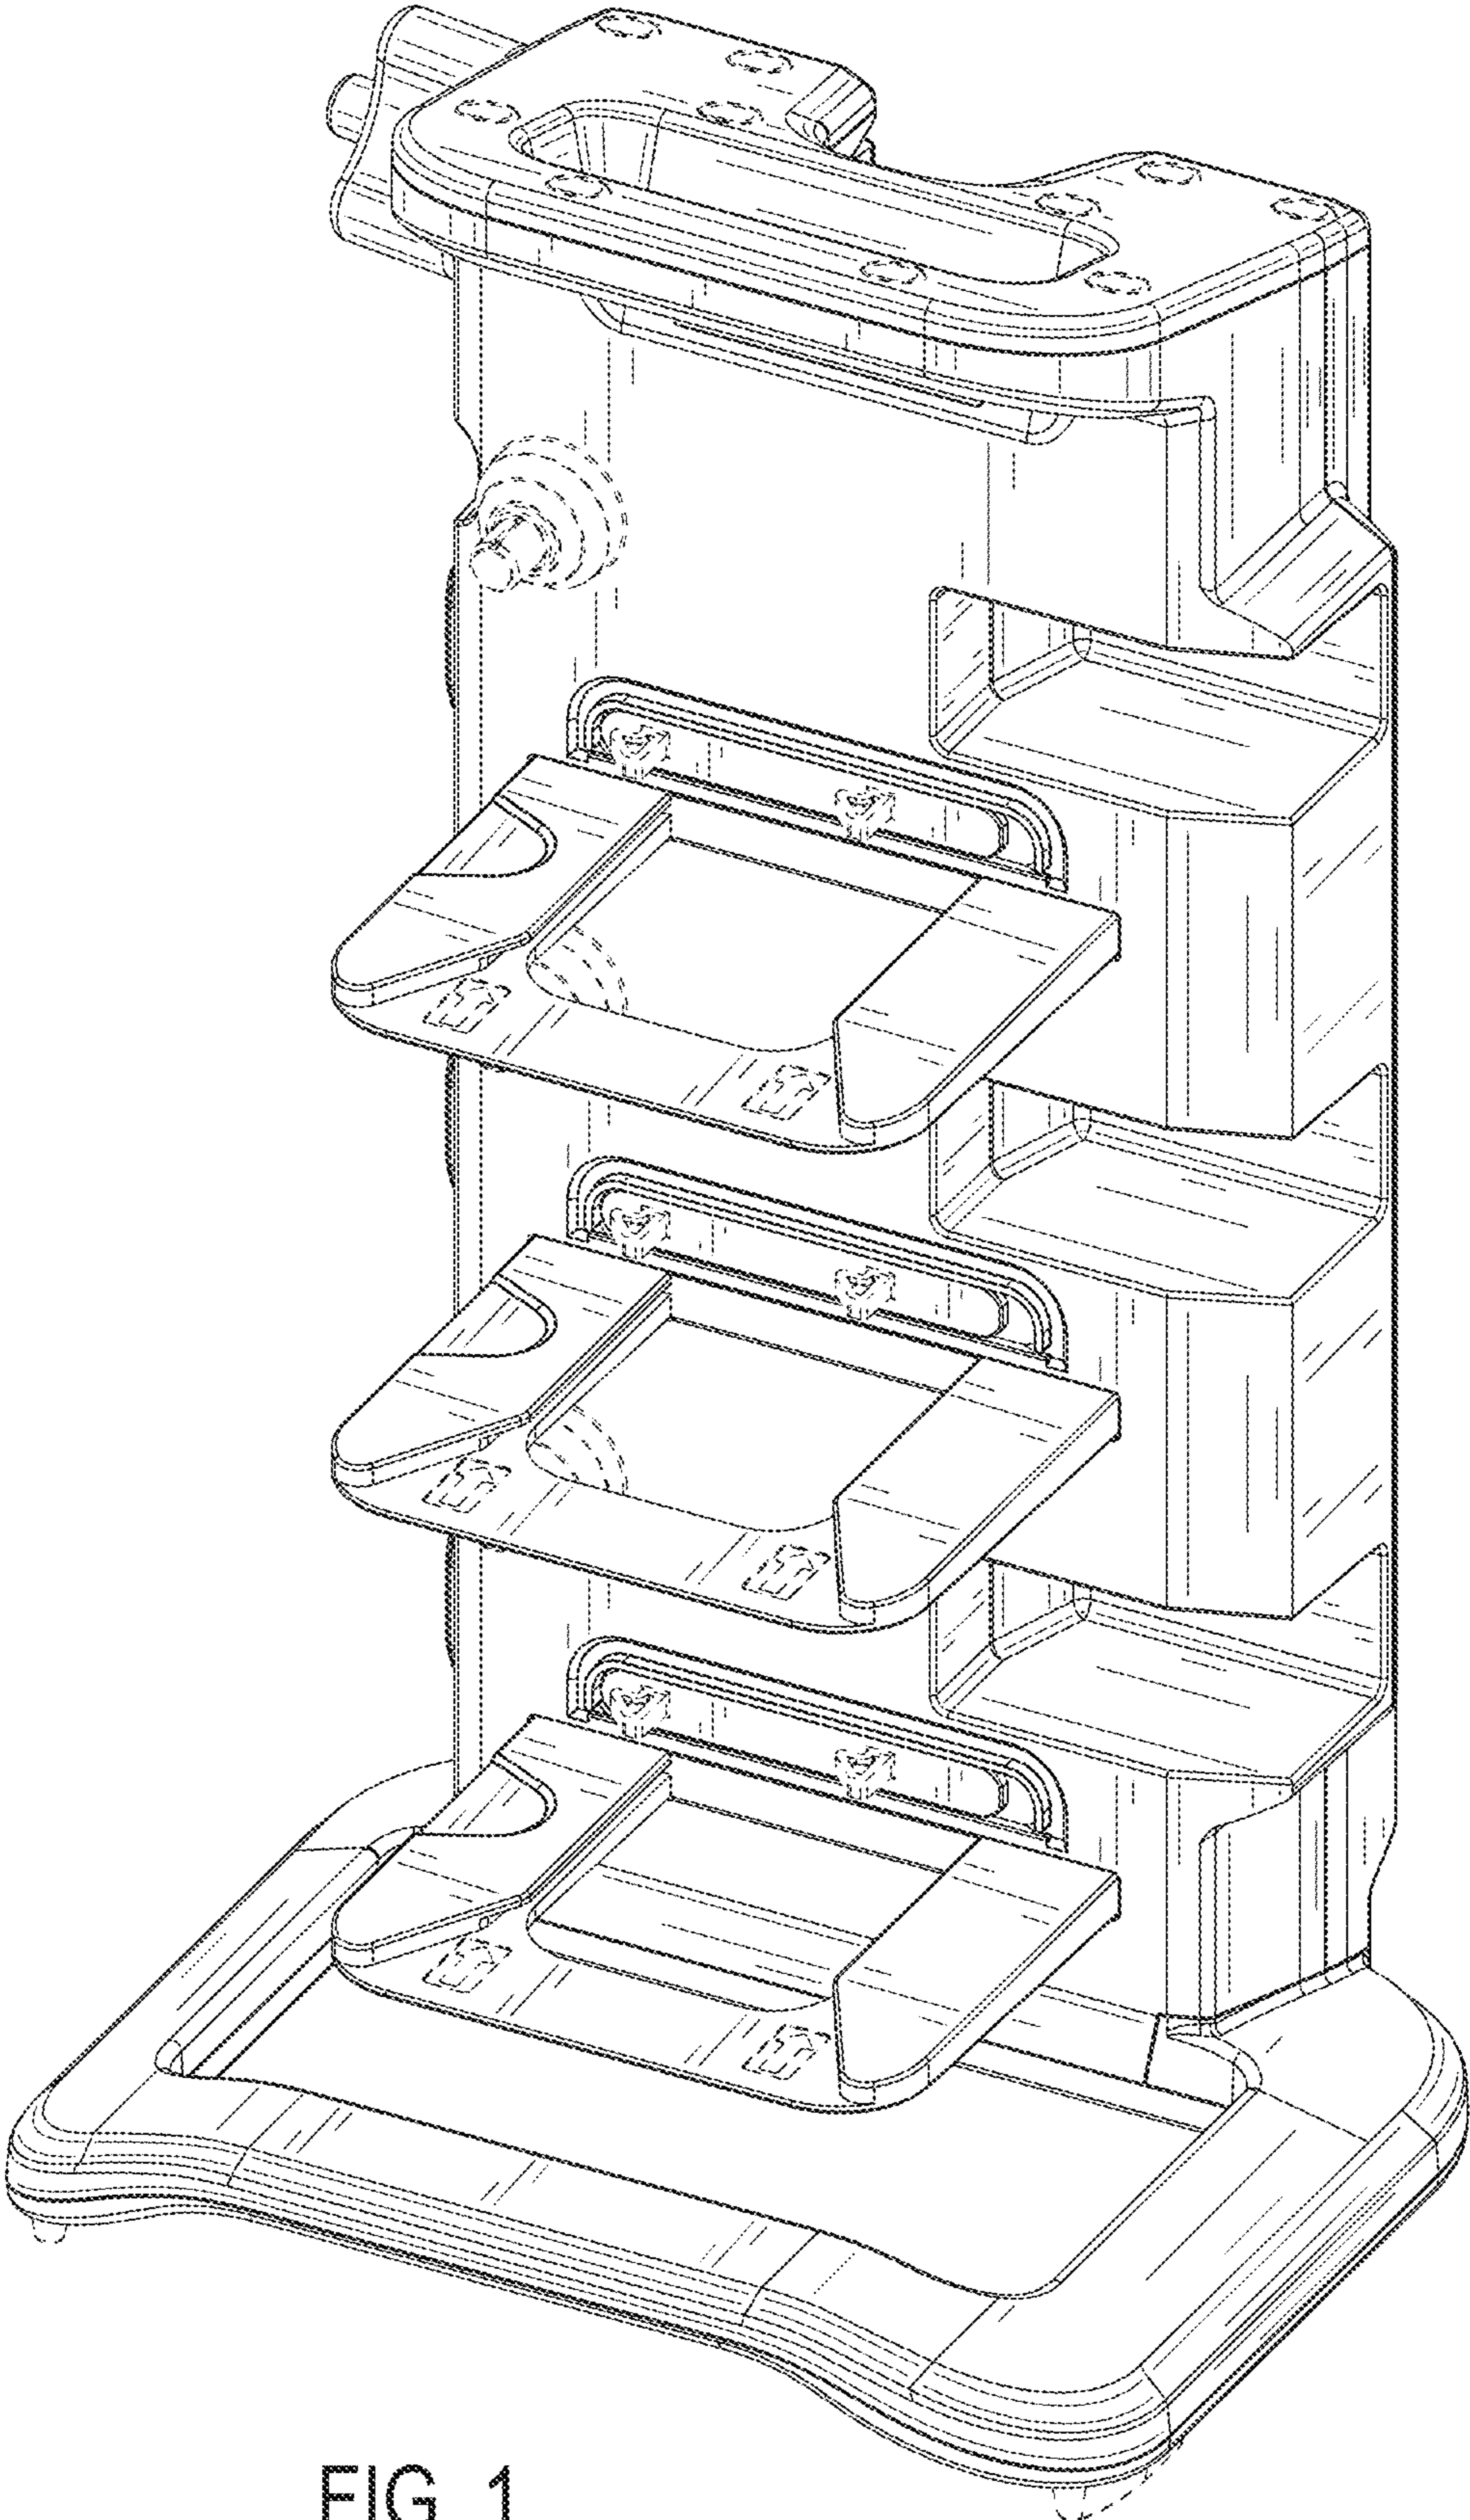


FIG. 1

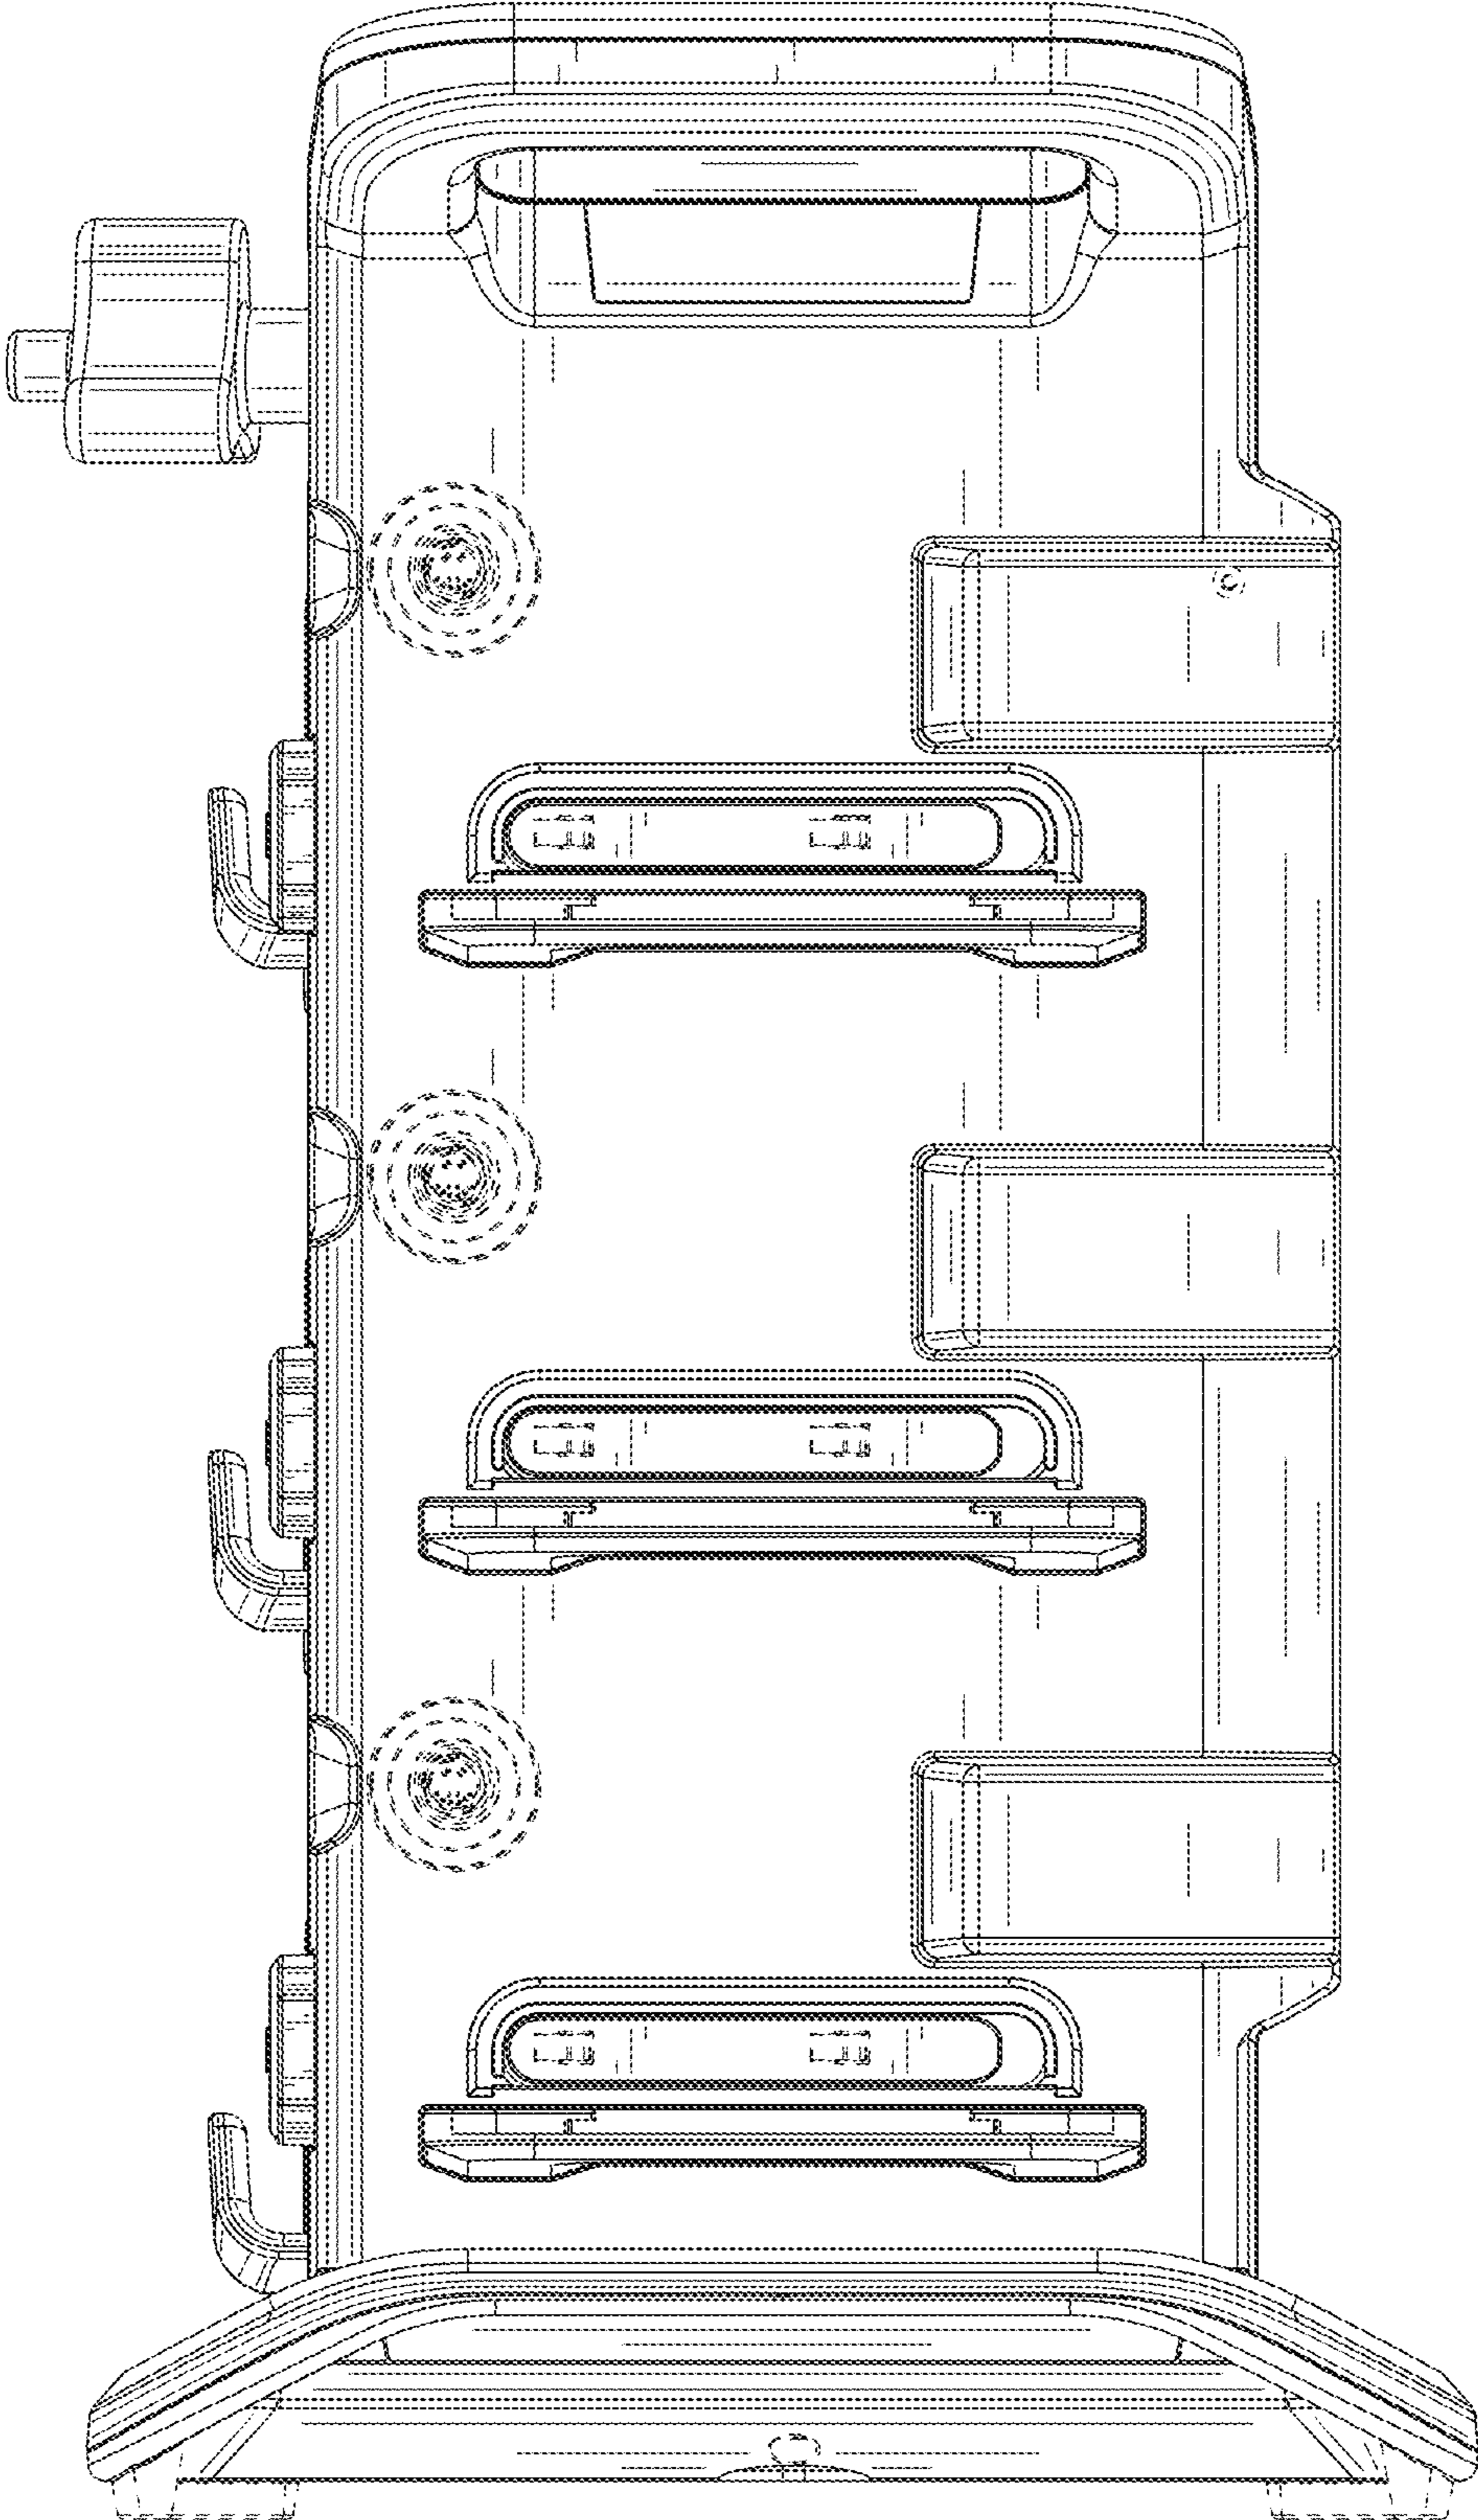


FIG. 2



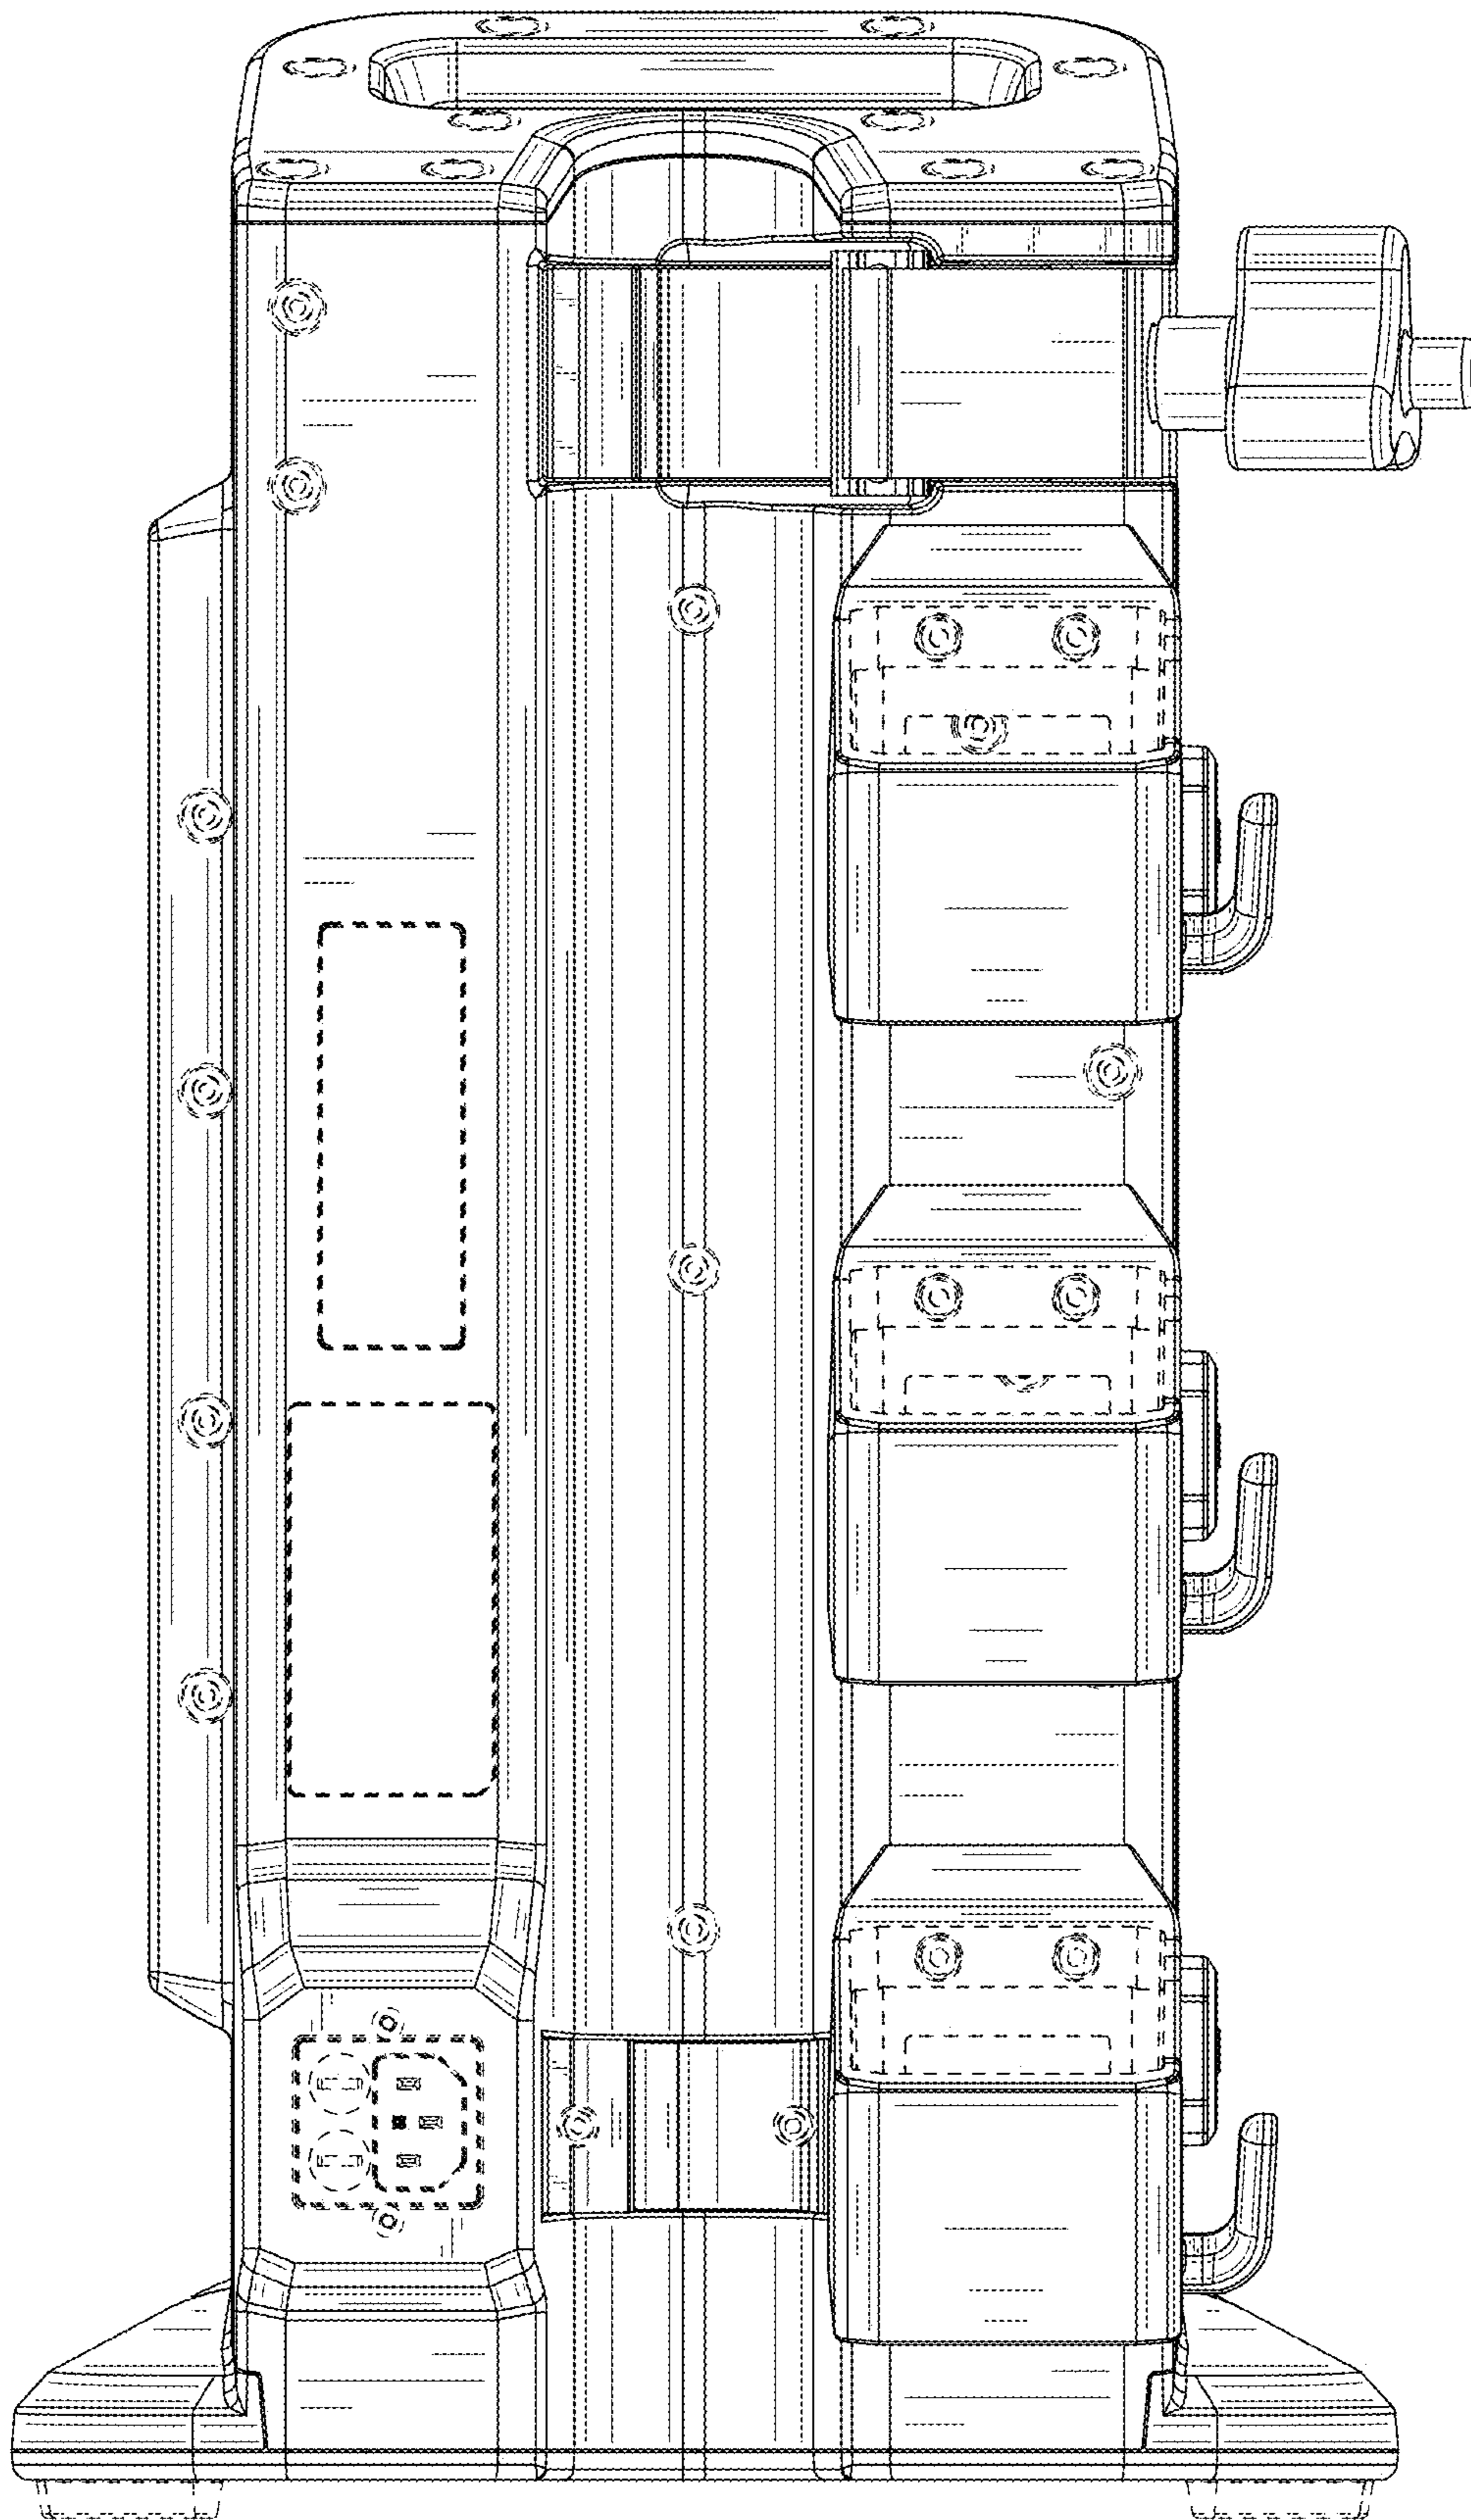


FIG. 3

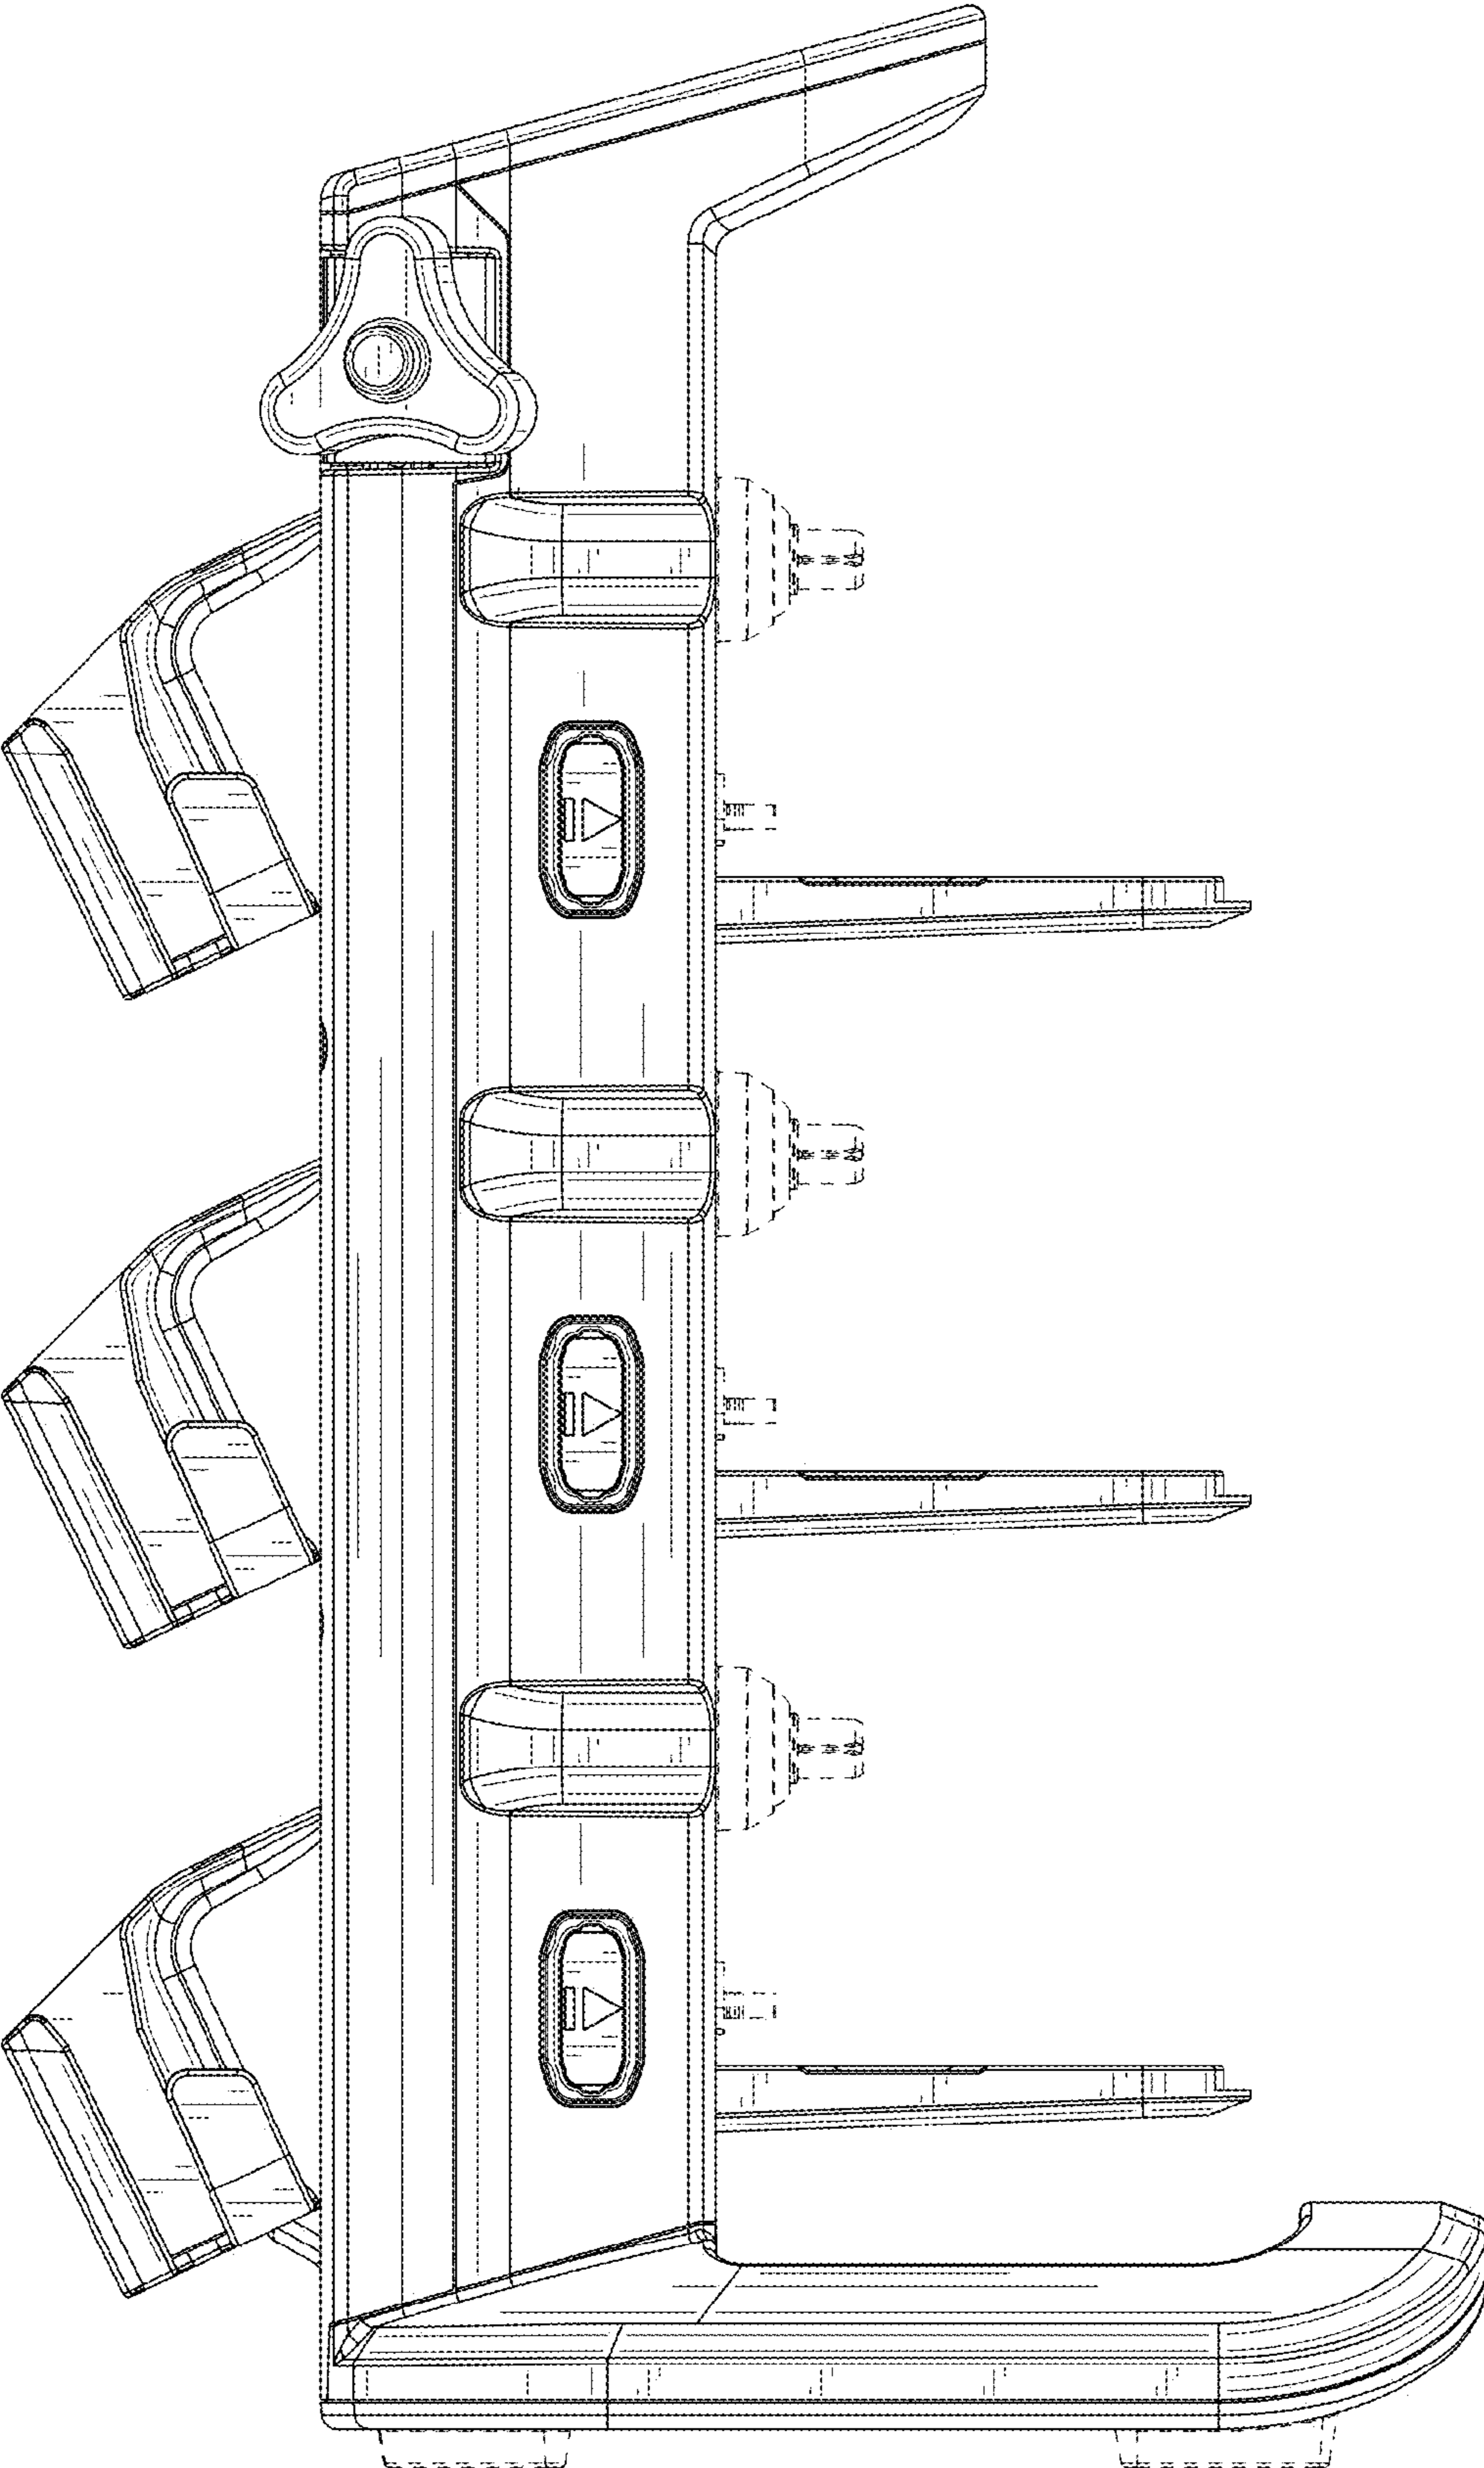


FIG. 4



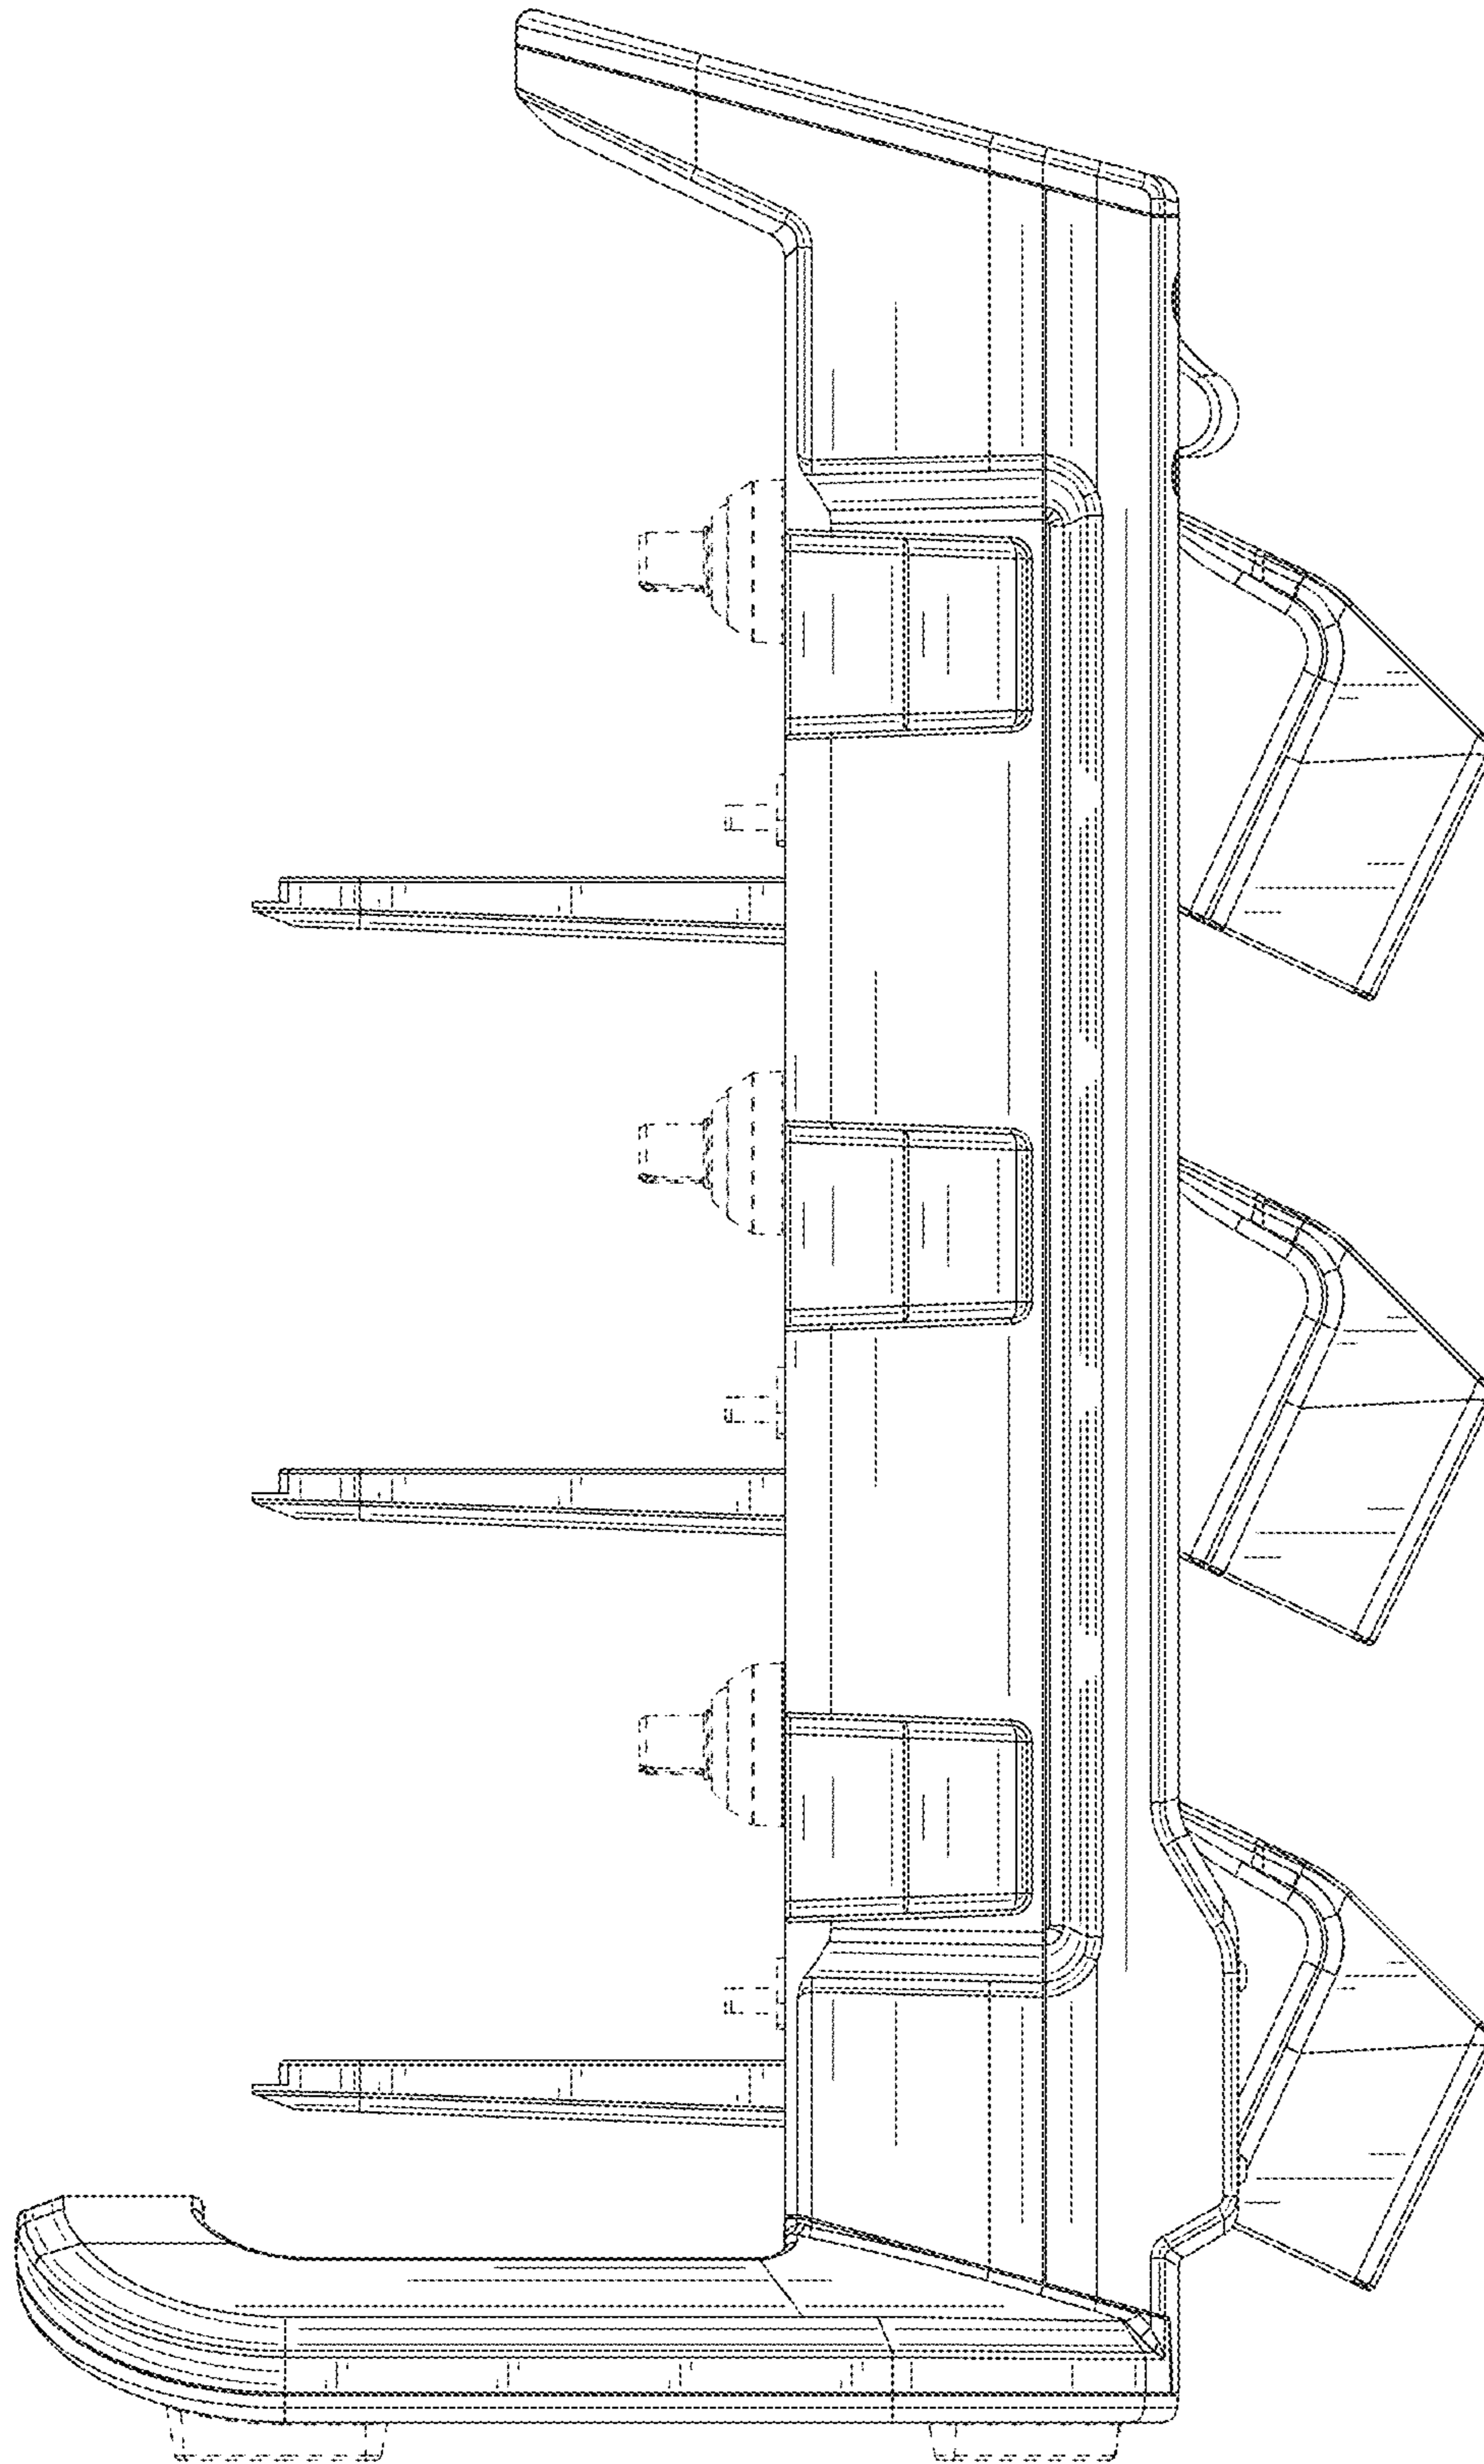


FIG. 5

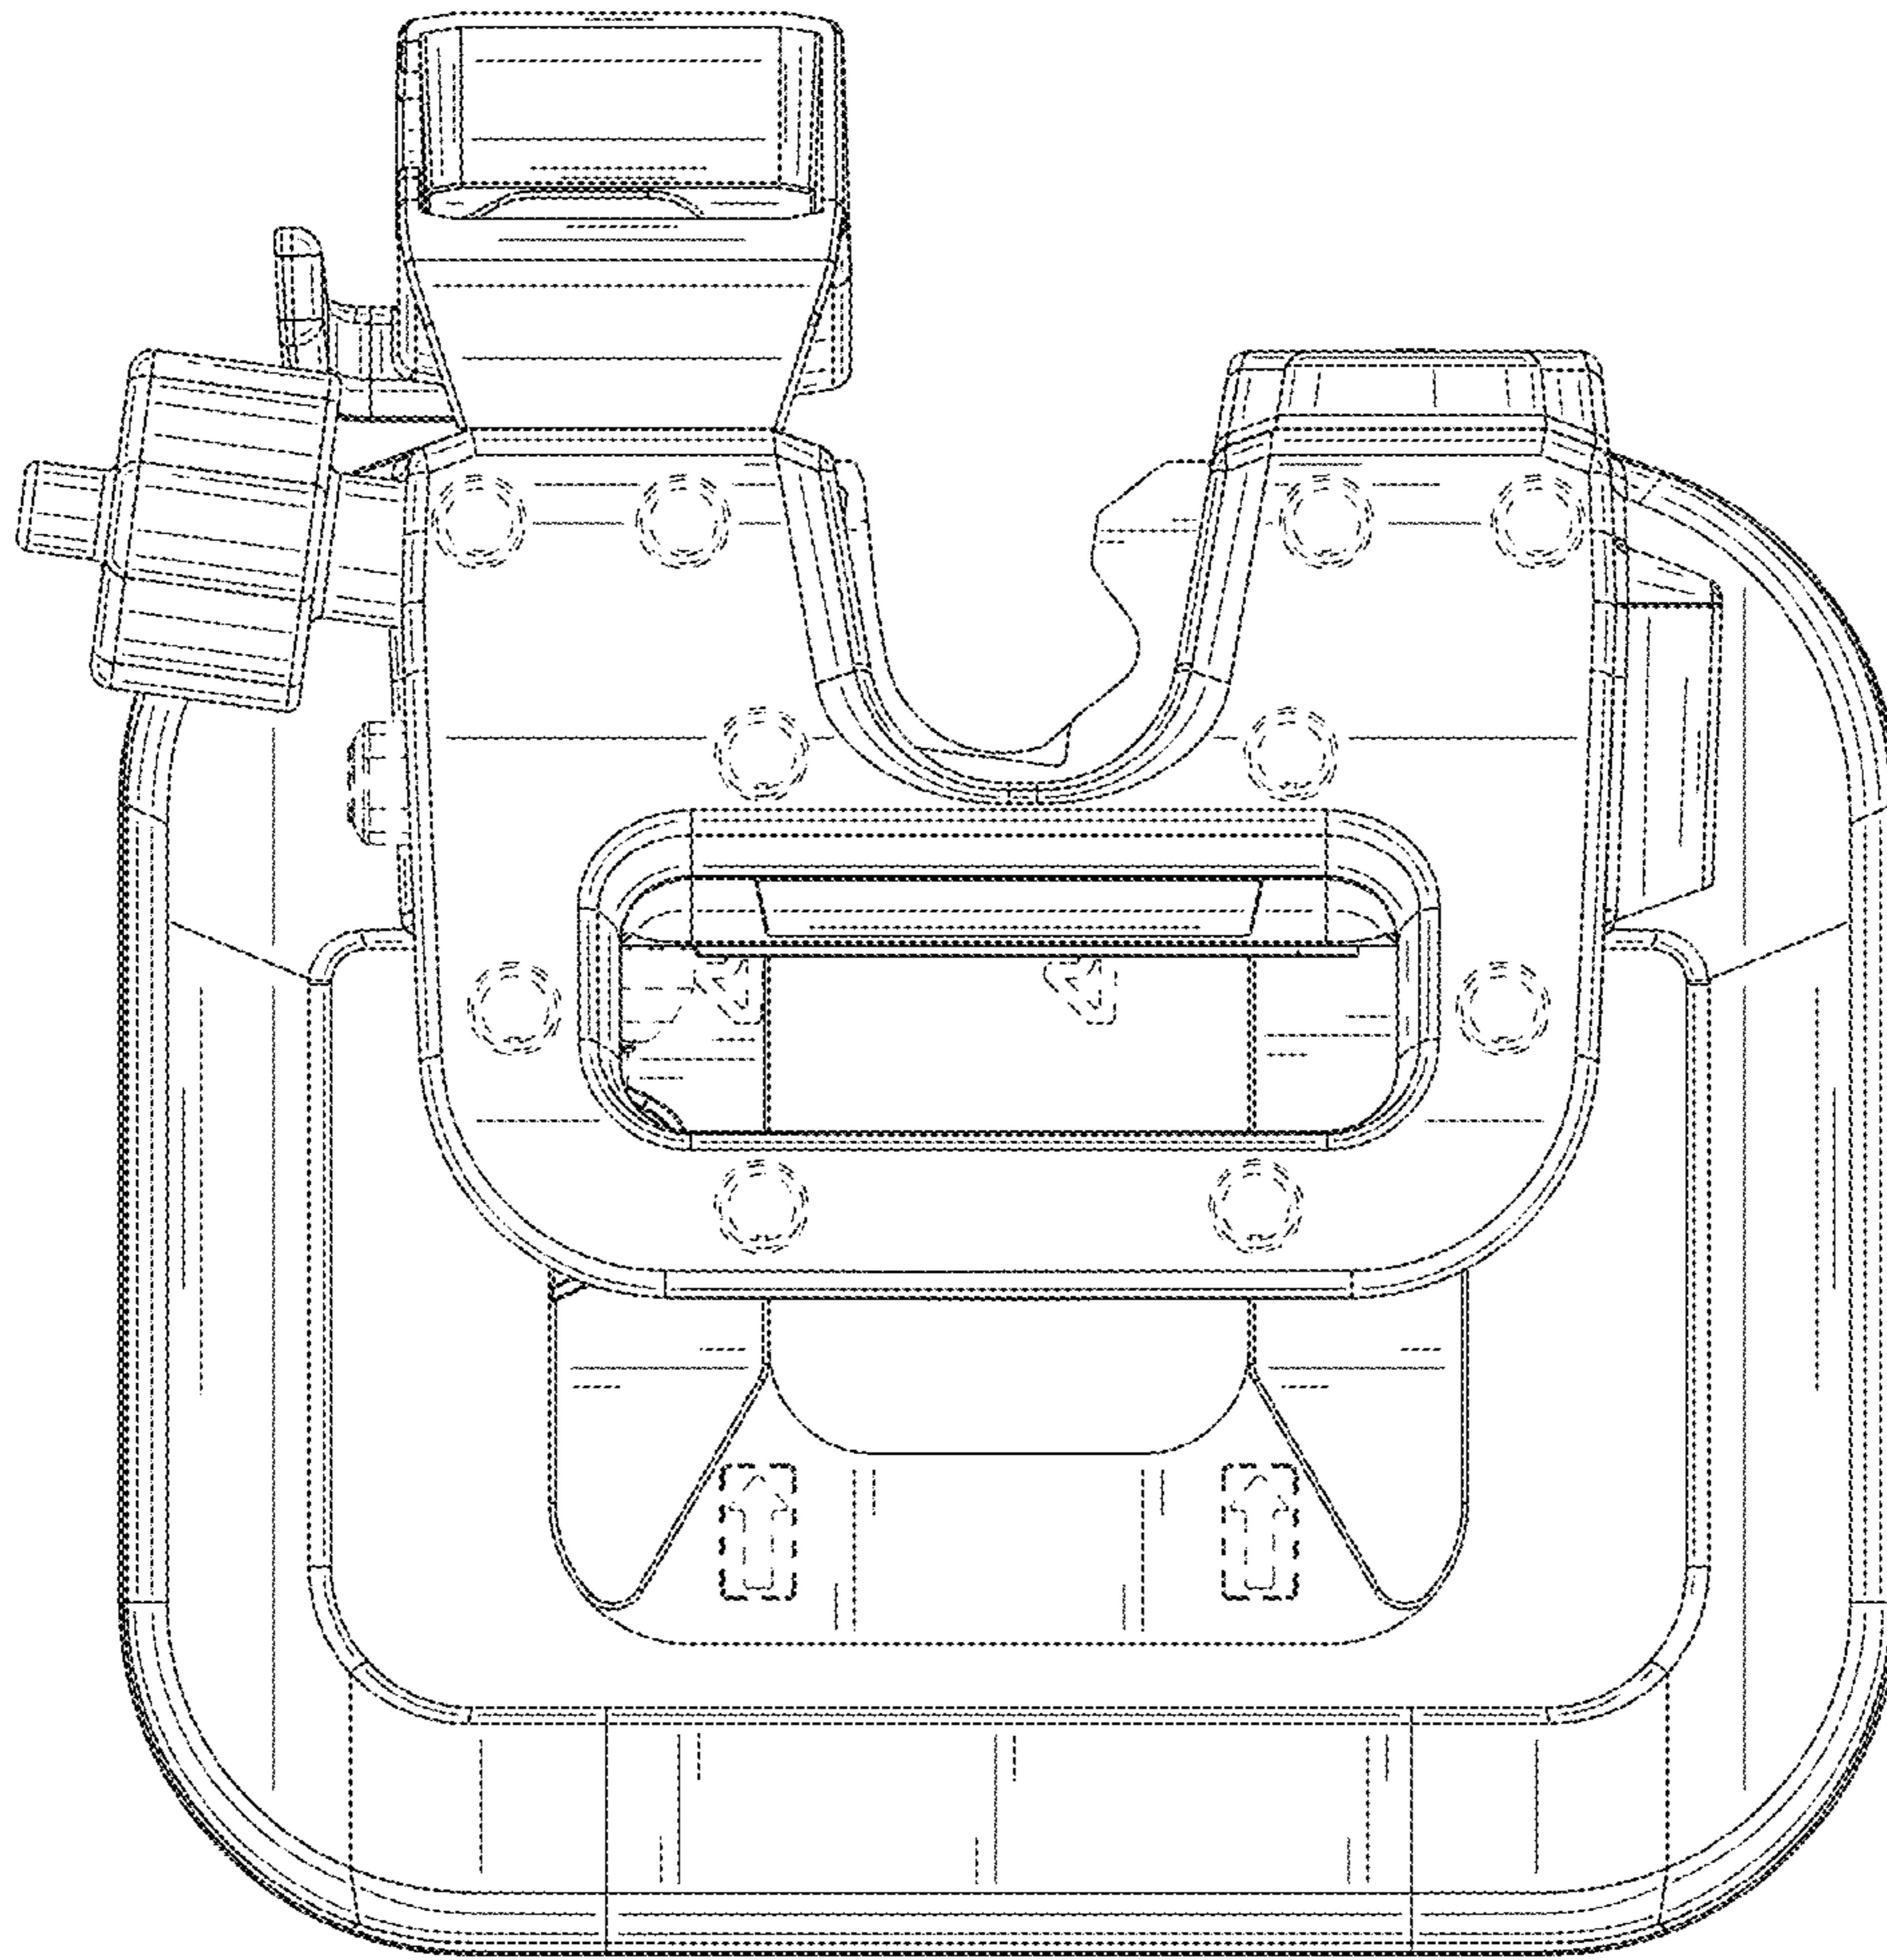


FIG. 6



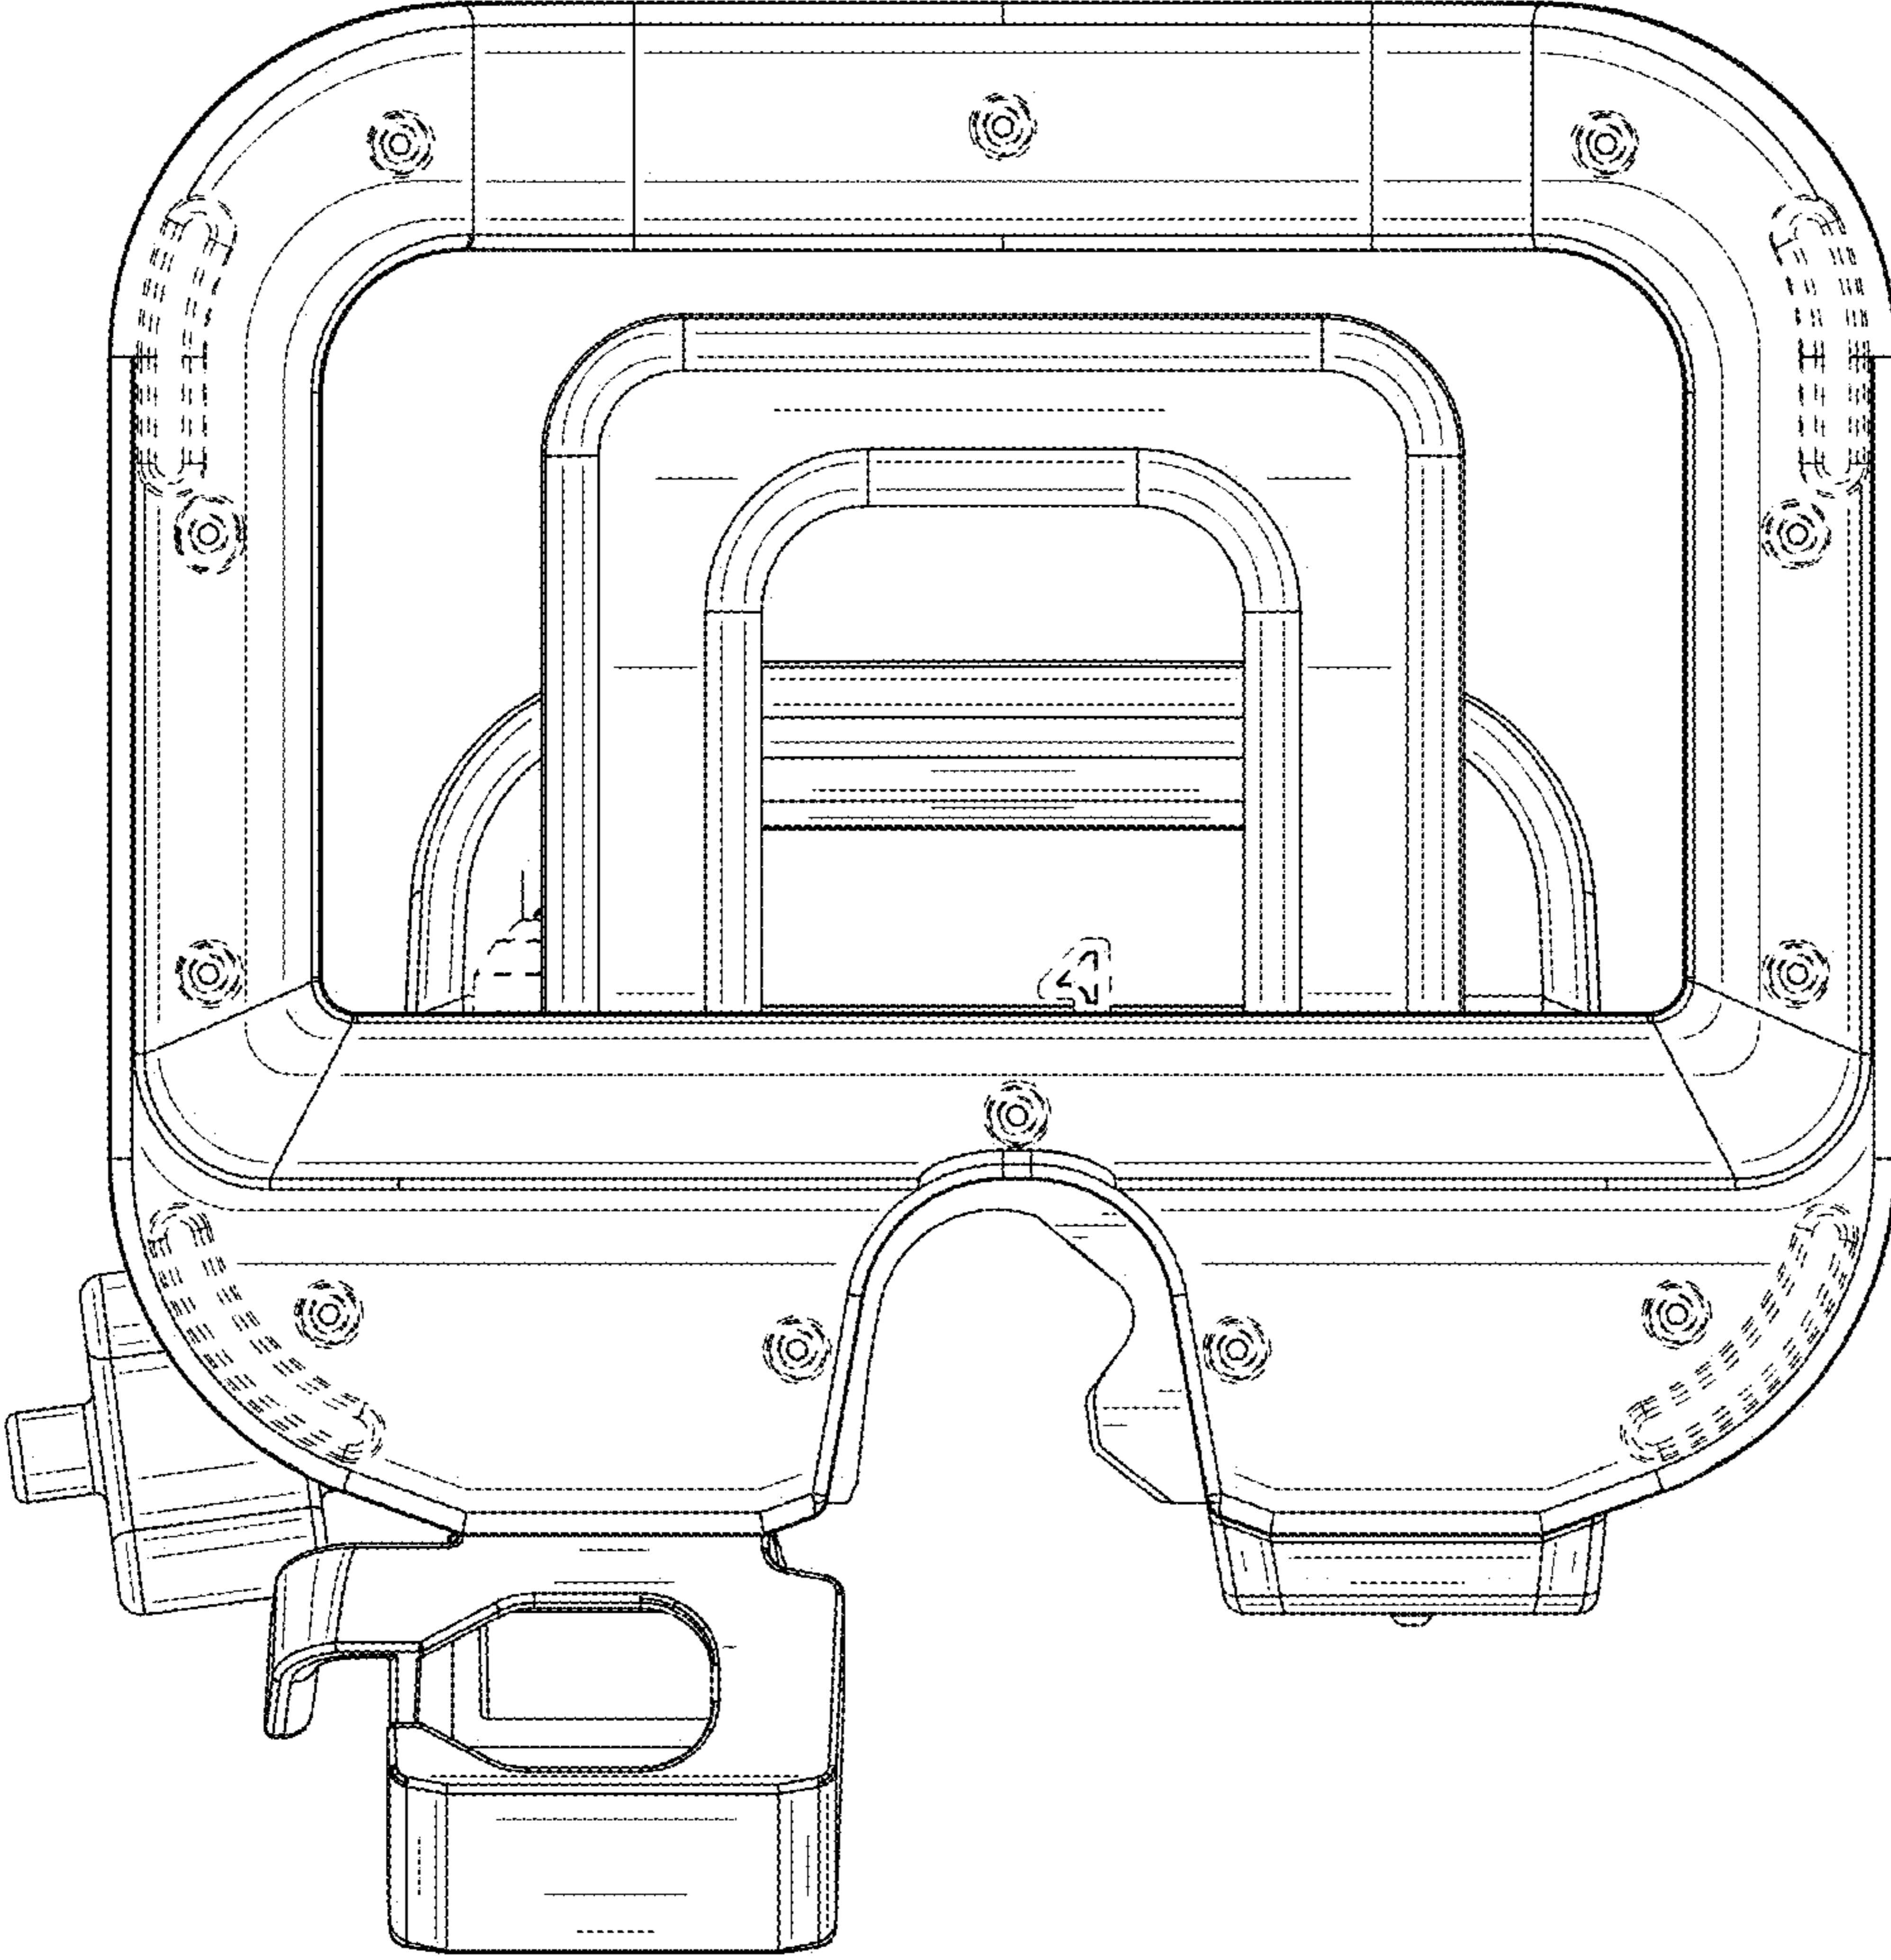


FIG. 7

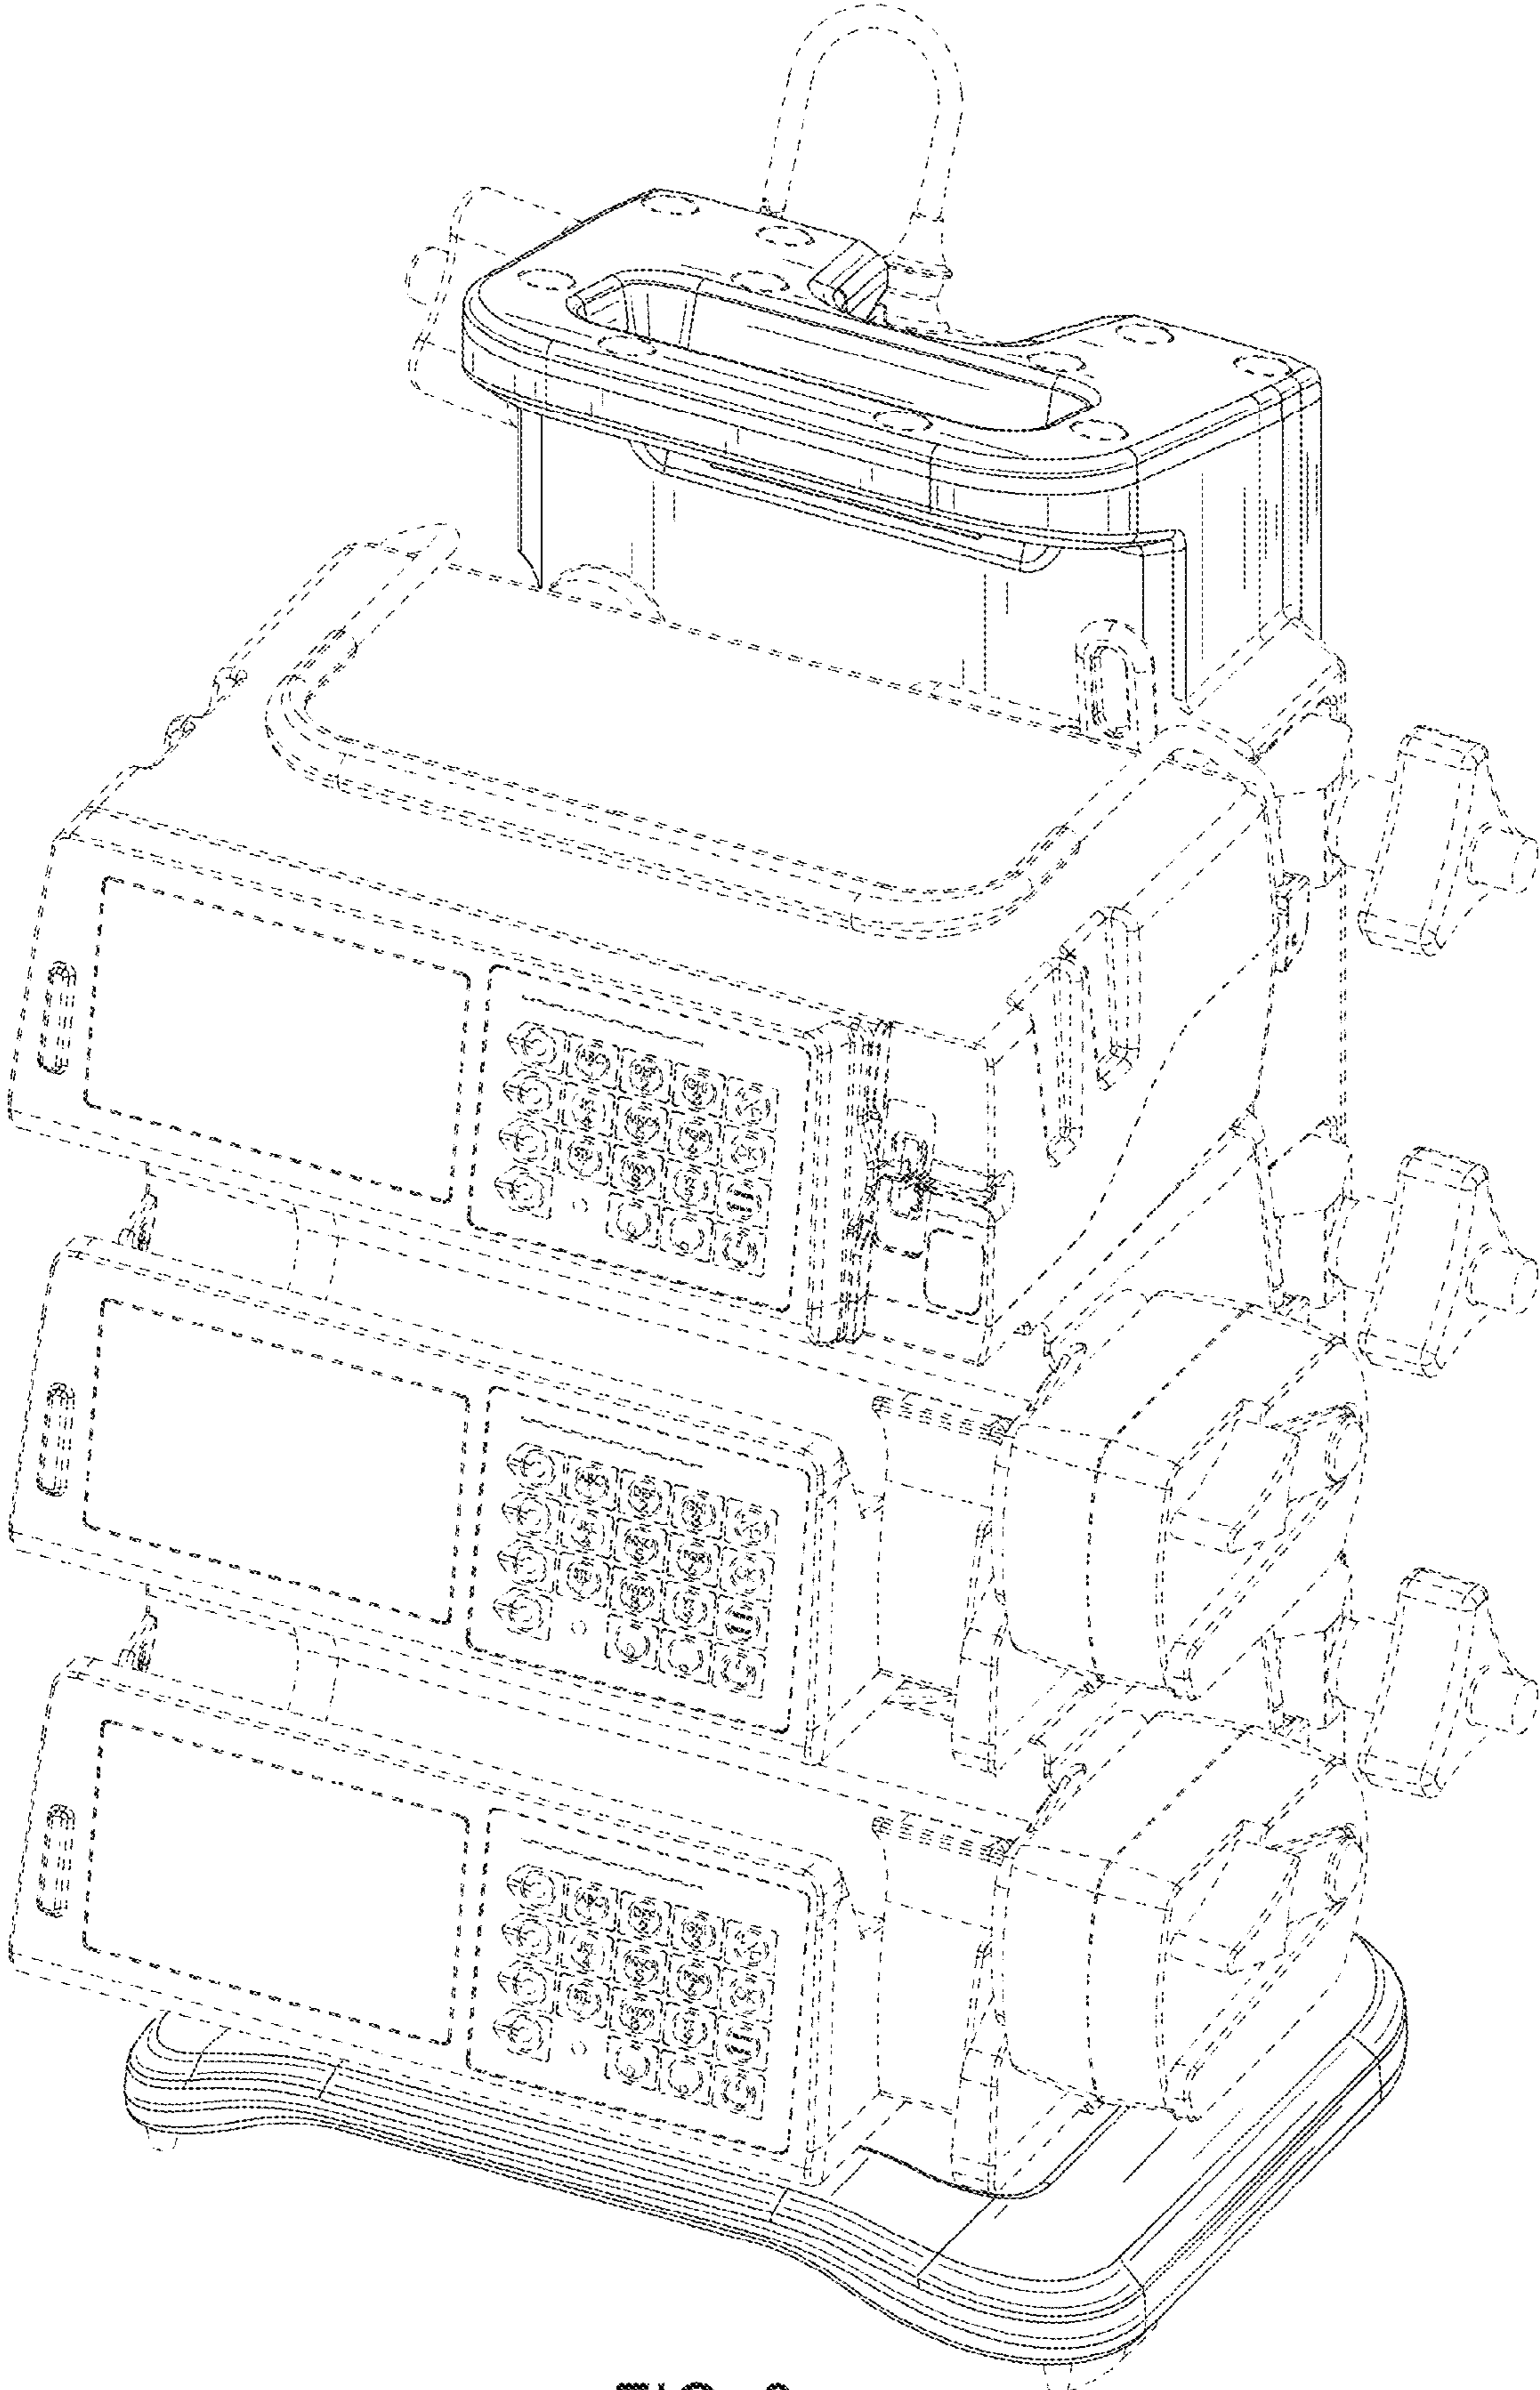


FIG. 8



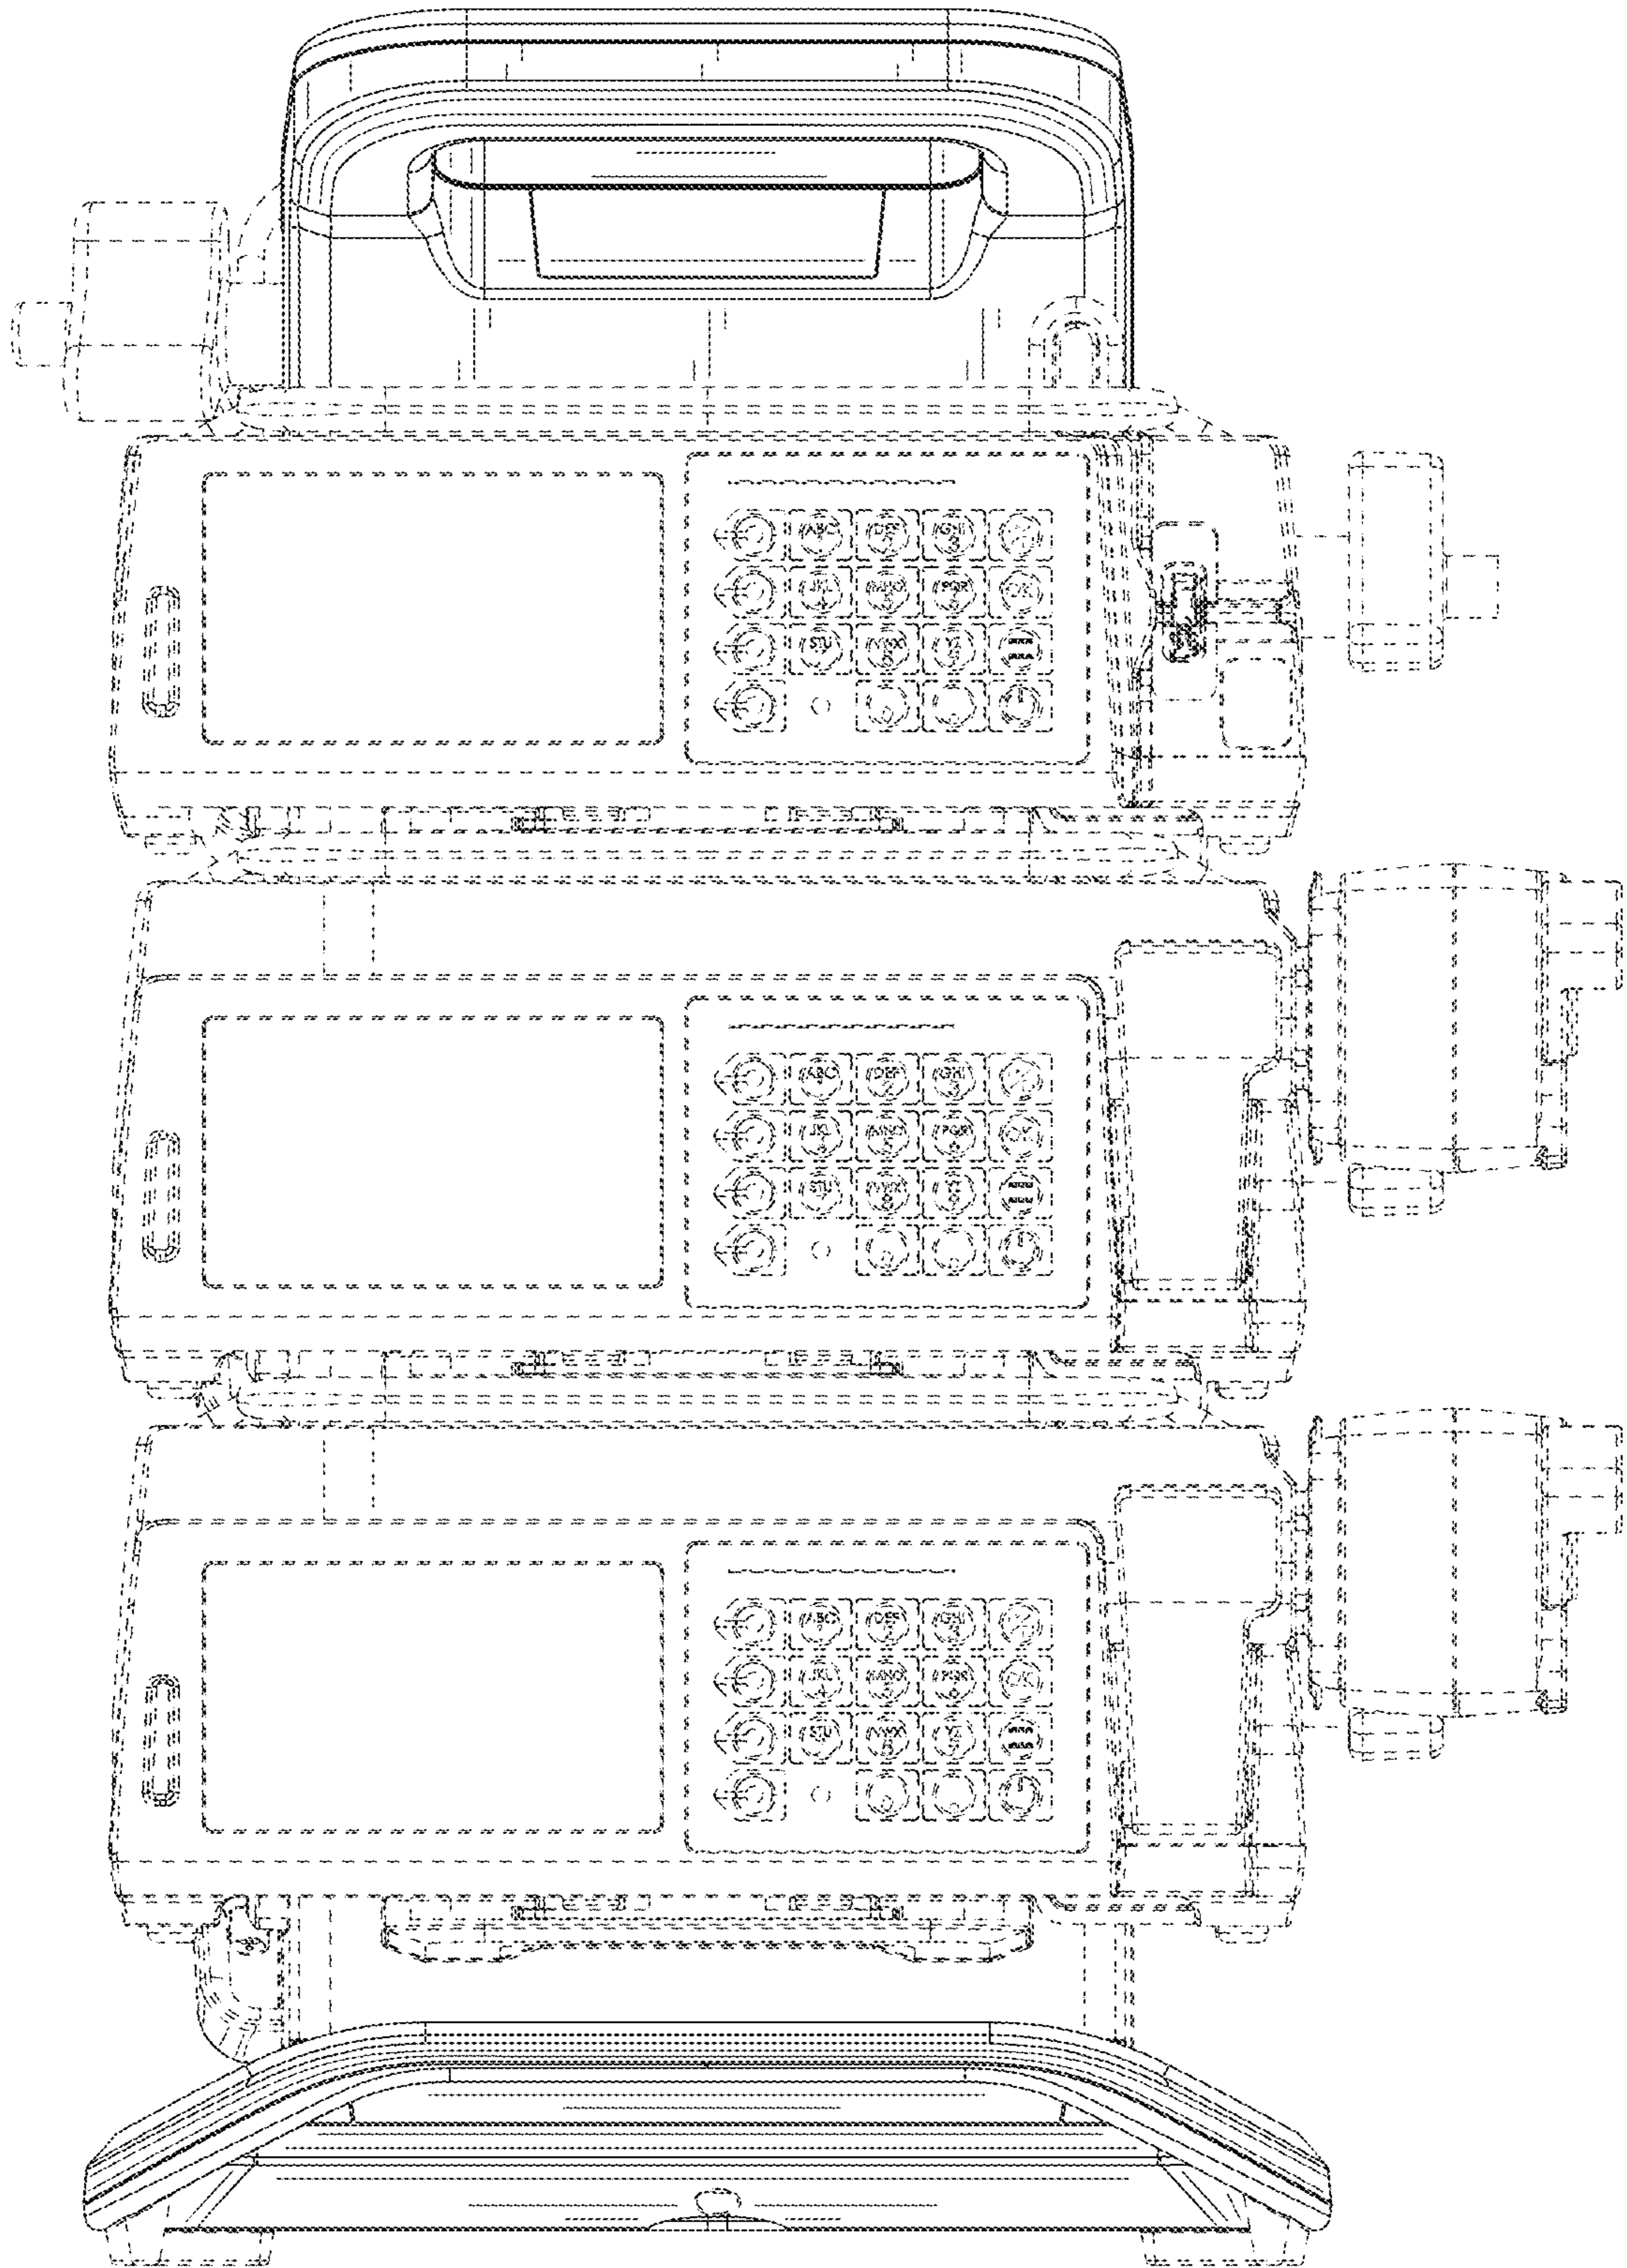


FIG. 9

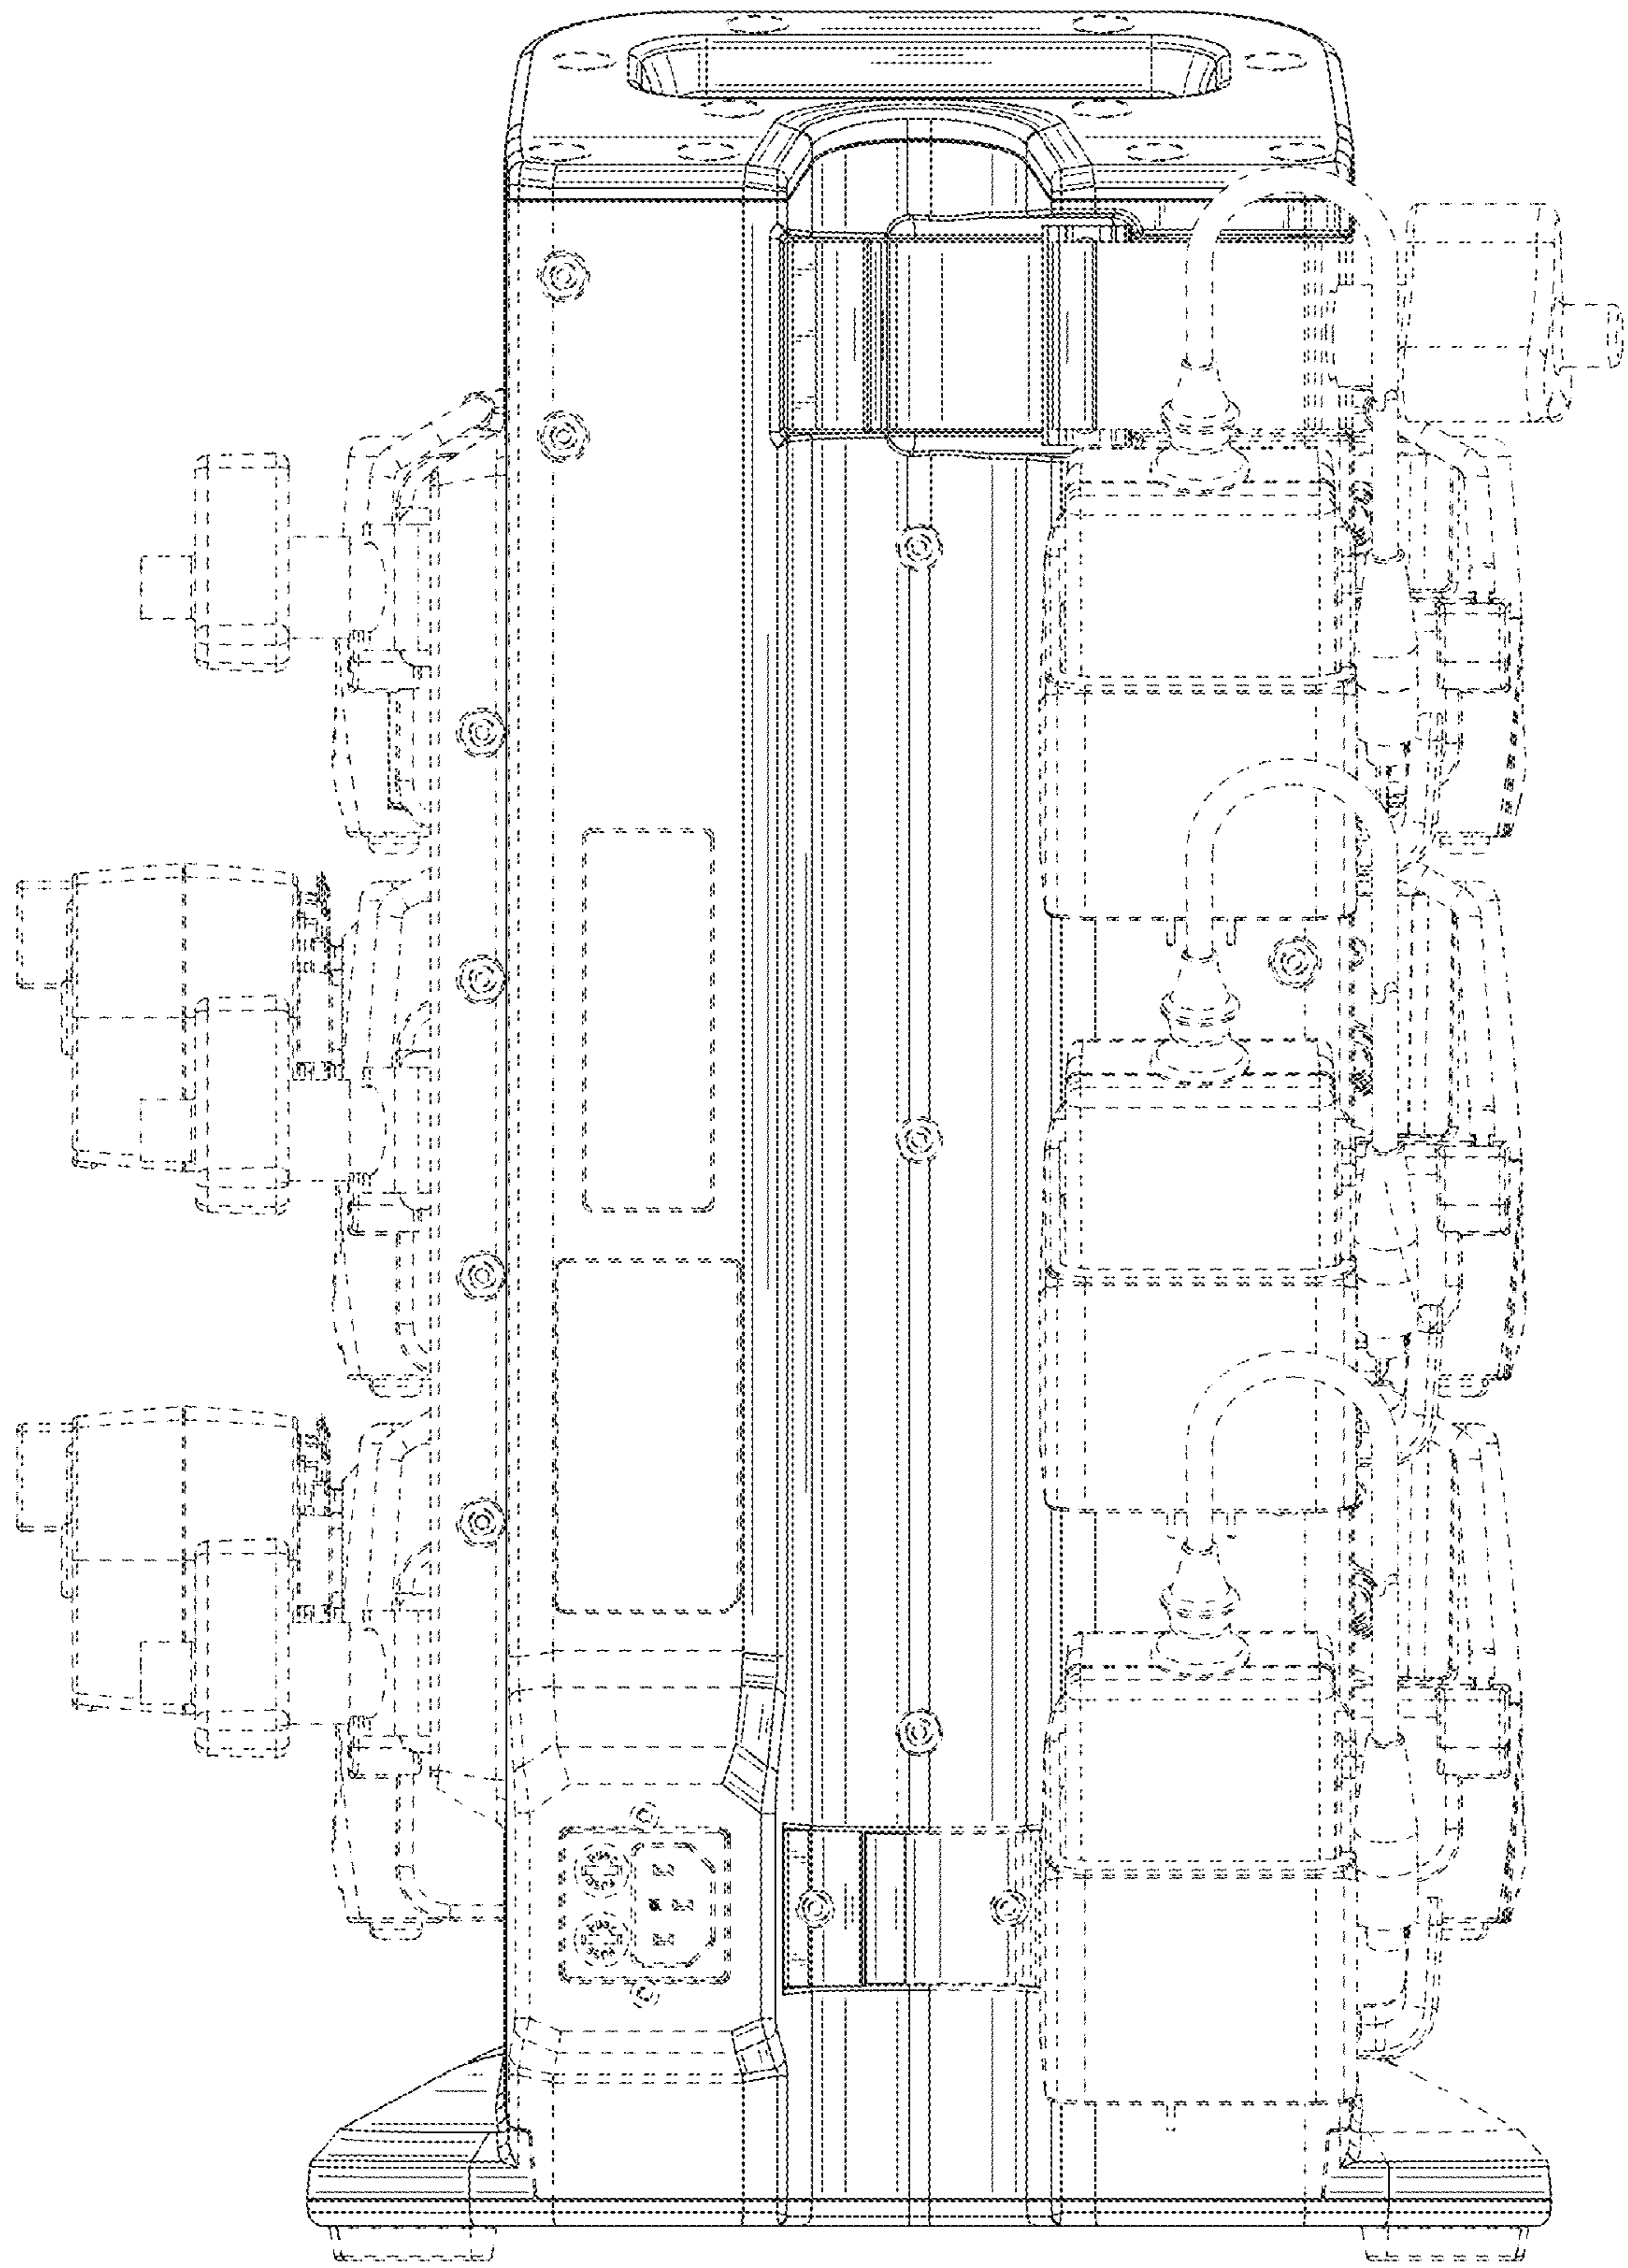


FIG. 10





FIG. 11

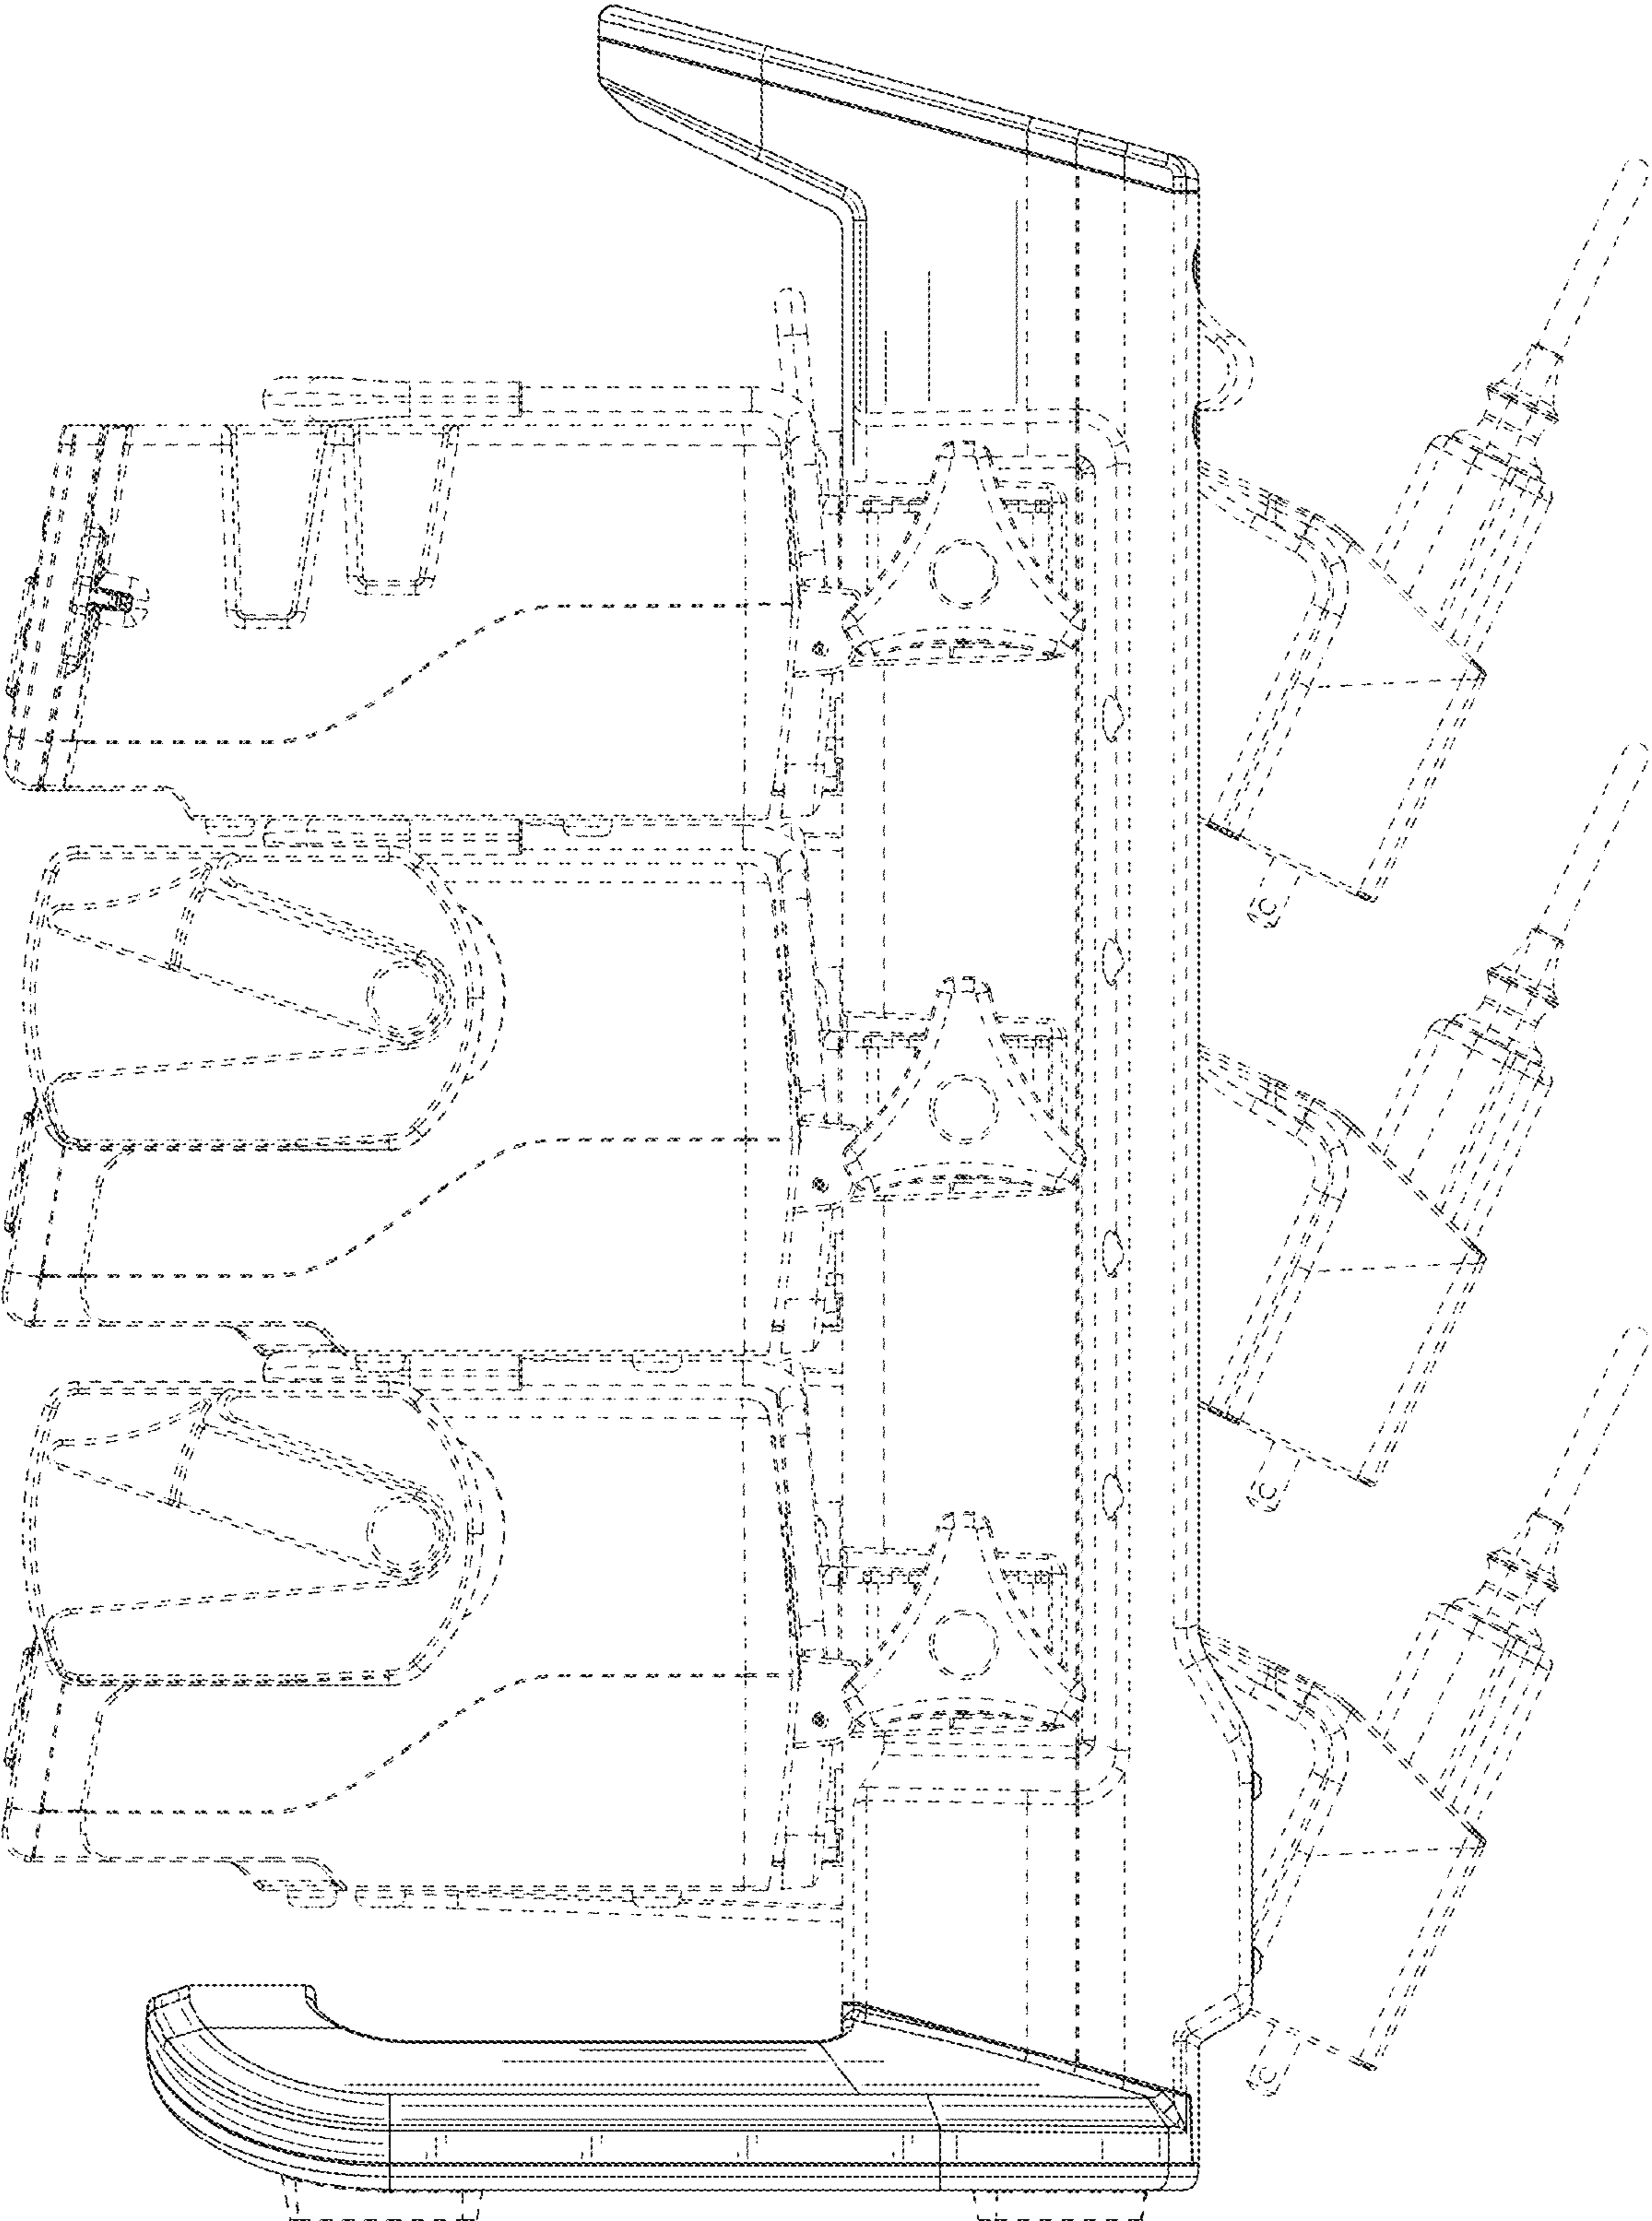


FIG. 12



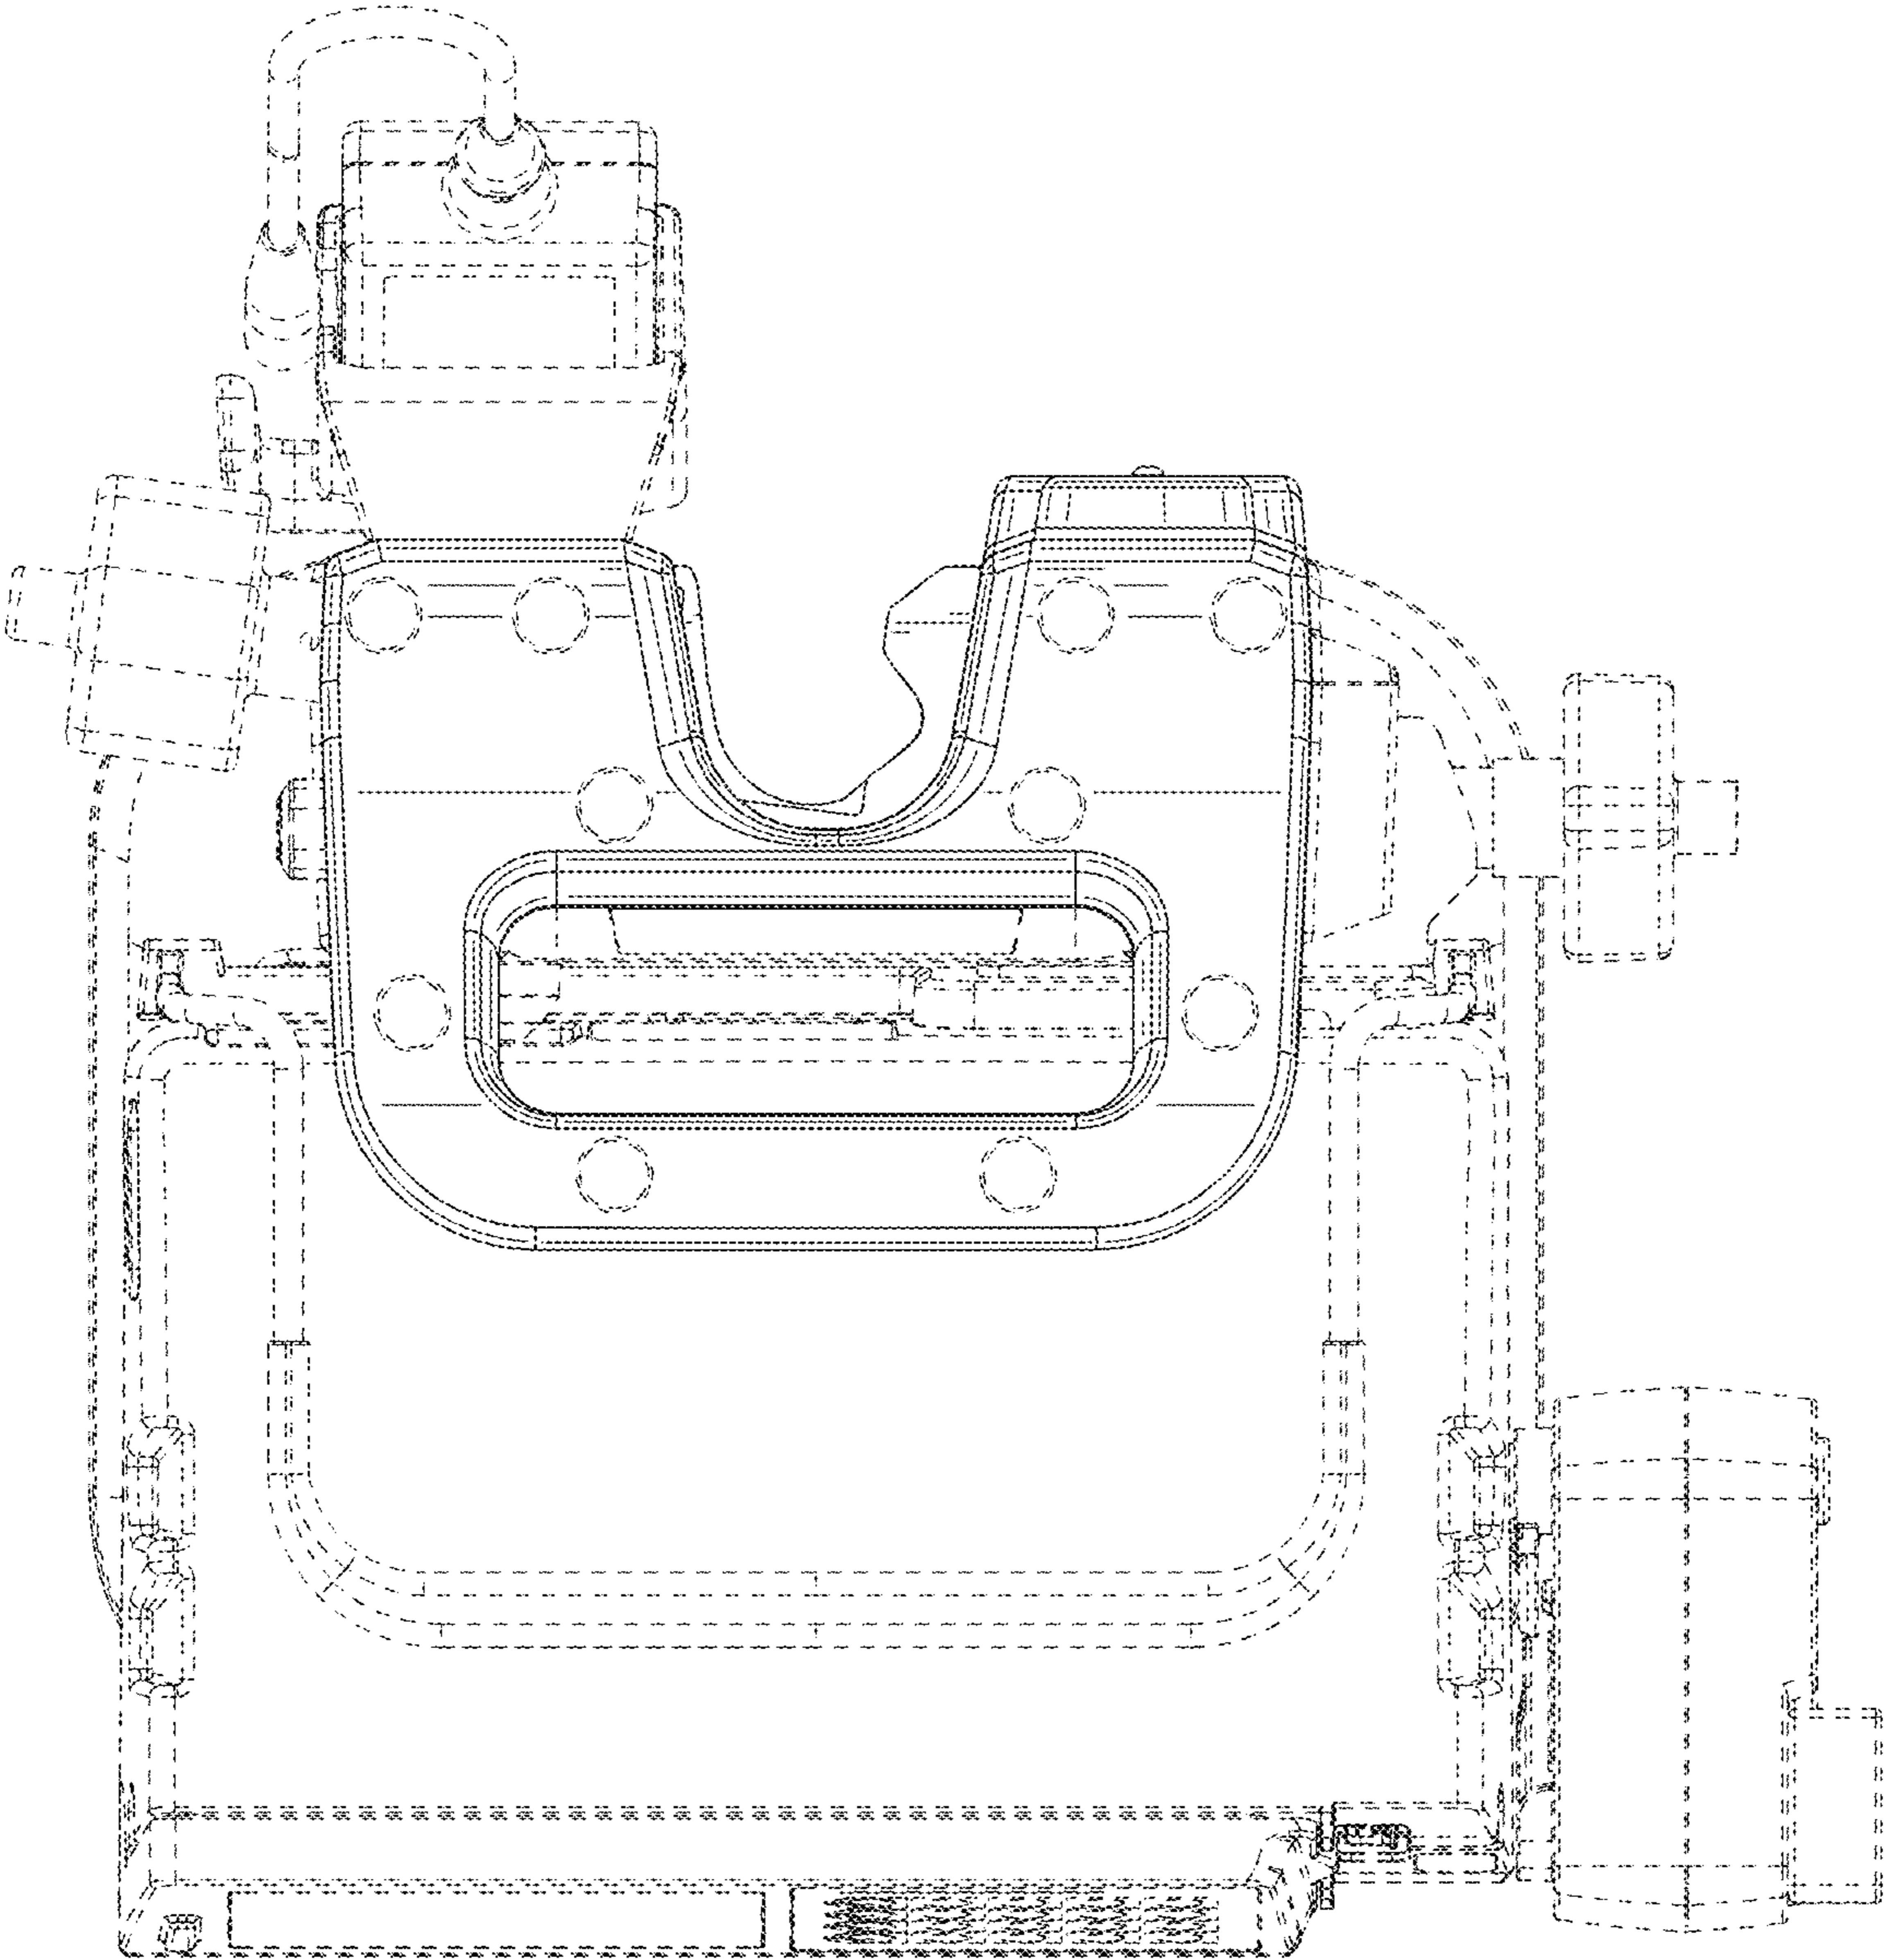


FIG. 13

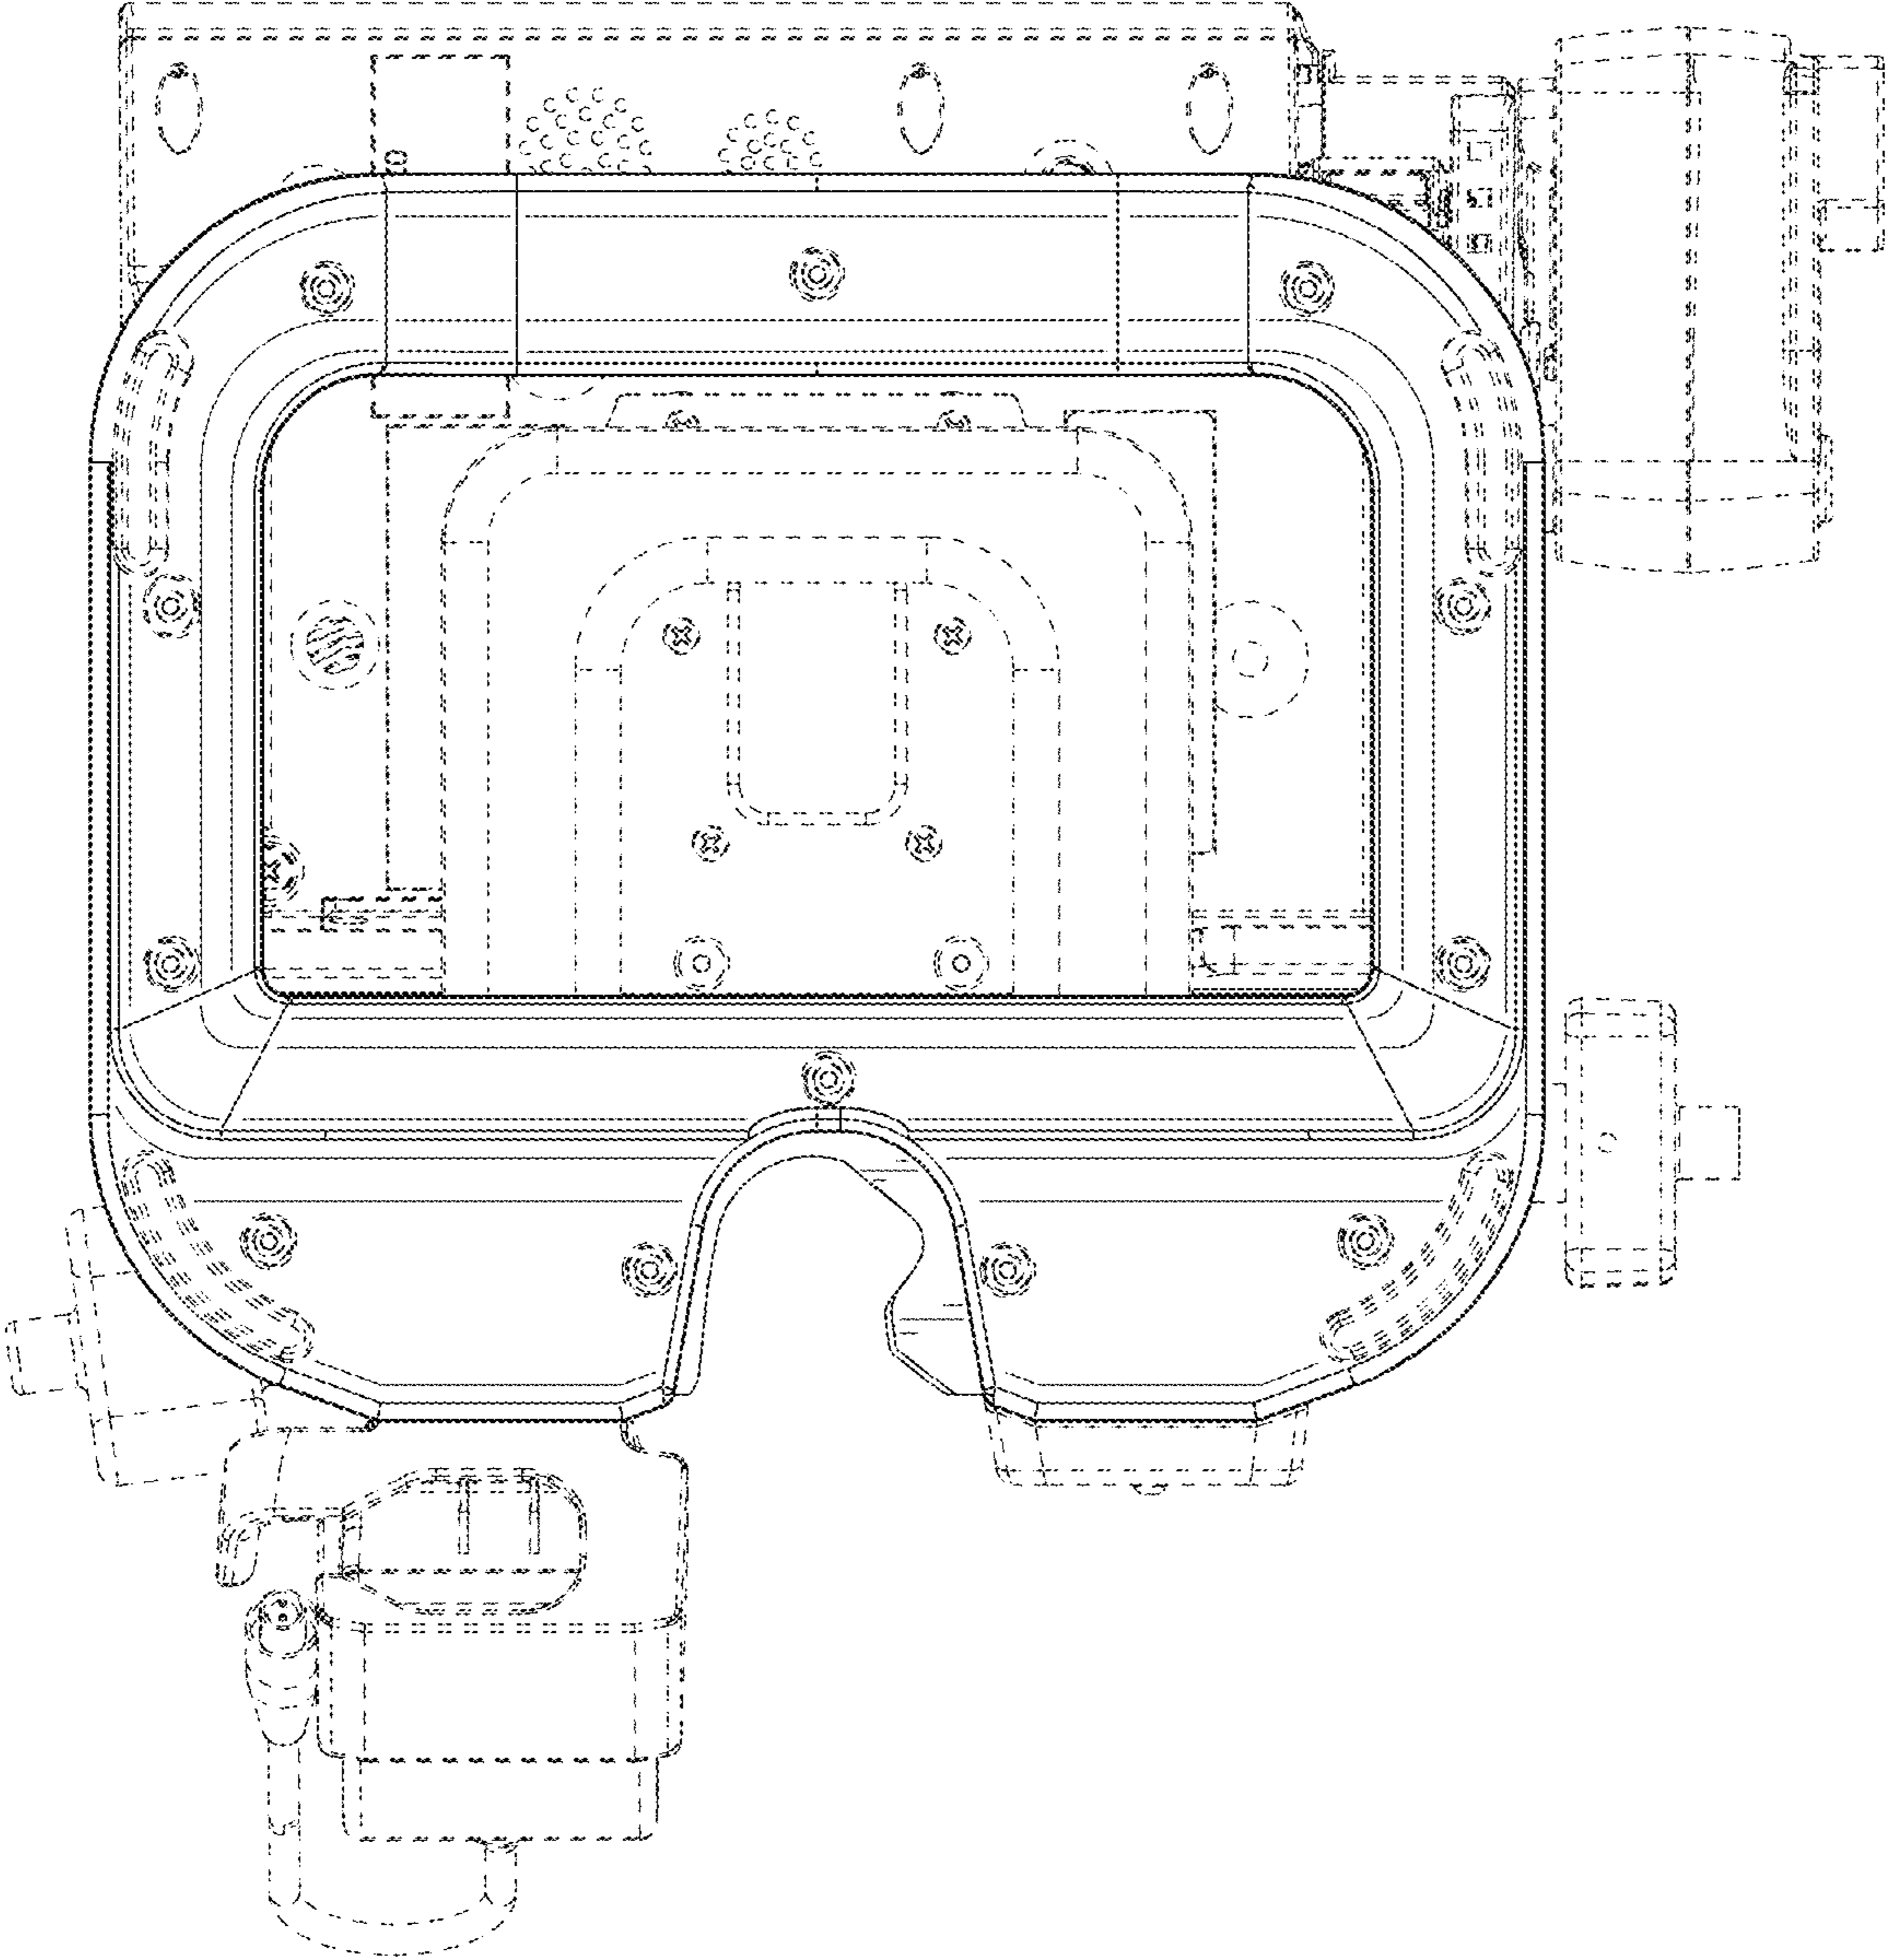


FIG. 14