

(12)

United States Design Patent

Wolf et al.

(10)

Patent No.:

US D998,172 S

(45)

Date of Patent:

** Sep. 5, 2023

(54) **SAMPLE RACK**

(71) Applicant: **Ultima Genomics, Inc.**, Newark, CA (US)

(72) Inventors: **Jacob Wolf**, Oakland, CA (US);
Nathan Beckett, Oakland, CA (US)

(73) Assignee: **ULTIMA GENOMICS, INC.**, Newark, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/774,033**

(22) Filed: **Mar. 12, 2021**

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/229**

(58) **Field of Classification Search**
USPC D24/107, 121, 169, 186, 216, 217,
D24/223–230; D9/756–758; D3/294,
D3/295
CPC .. B01L 3/502; B01L 9/06; B01L 3/545; B01L
3/50851; B01L 3/527
See application file for complete search history.

D669,597 S * 10/2012 Cavada D24/224
D672,881 S * 12/2012 Kraihanzel D24/224
D675,338 S * 1/2013 Suzuki D24/229
(Continued)

FOREIGN PATENT DOCUMENTS

JP D2008-6213 * 11/2009
KR 3010631580005 12/2020

OTHER PUBLICATIONS

Axygen™ 8-Strip PCR Tubes, 0.2mL. Available at <https://www.fishersci.com/shop/products/axygen-8-strip-pcr-tubes-flat-cap-0-2ml-color-maxyclear/14222252>. Accessed on Jun. 25, 2020 (2 pages).
(Continued)

Primary Examiner — Omeed Agilee
(74) *Attorney, Agent, or Firm* — Wilson Sonsini Goodrich & Rosati

(57) **CLAIM**

The ornamental design for a sample rack, as shown and described.

DESCRIPTION


FIG. 1 is a top perspective view of a sample rack showing a sample tube out of its place in the sample rack;
FIG. 2 is a top perspective view of the sample rack showing the sample tube in its place in the sample rack;
FIG. 3 is a bottom perspective view thereof;
FIG. 4 is a top view thereof;
FIG. 5 is a right side view thereof;
FIG. 6 is a bottom view thereof;
FIG. 7 is a left side view thereof;
FIG. 8 is a front view thereof; and,
FIG. 9 is a back view thereof.
Broken lines shown in the drawings are included for illustrating portions of the sample rack that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

(56) **References Cited**

U.S. PATENT DOCUMENTS

D249,706 S * 9/1978 Adamski D24/230
4,675,299 A * 6/1987 Witty G01N 33/5304
D24/223
D413,391 S * 8/1999 Lapeus D24/227
D414,271 S 9/1999 Mendoza
D421,130 S * 2/2000 Cohen D24/229
6,123,205 A * 9/2000 Dumitrescu B01L 9/06
211/74
D461,554 S 8/2002 Lafond et al.
6,602,474 B1 * 8/2003 Tajima B01L 3/50855
435/303.1
7,704,735 B2 4/2010 Facer et al.
D618,820 S * 6/2010 Wilson D24/227
D631,557 S 1/2011 Tajima et al.

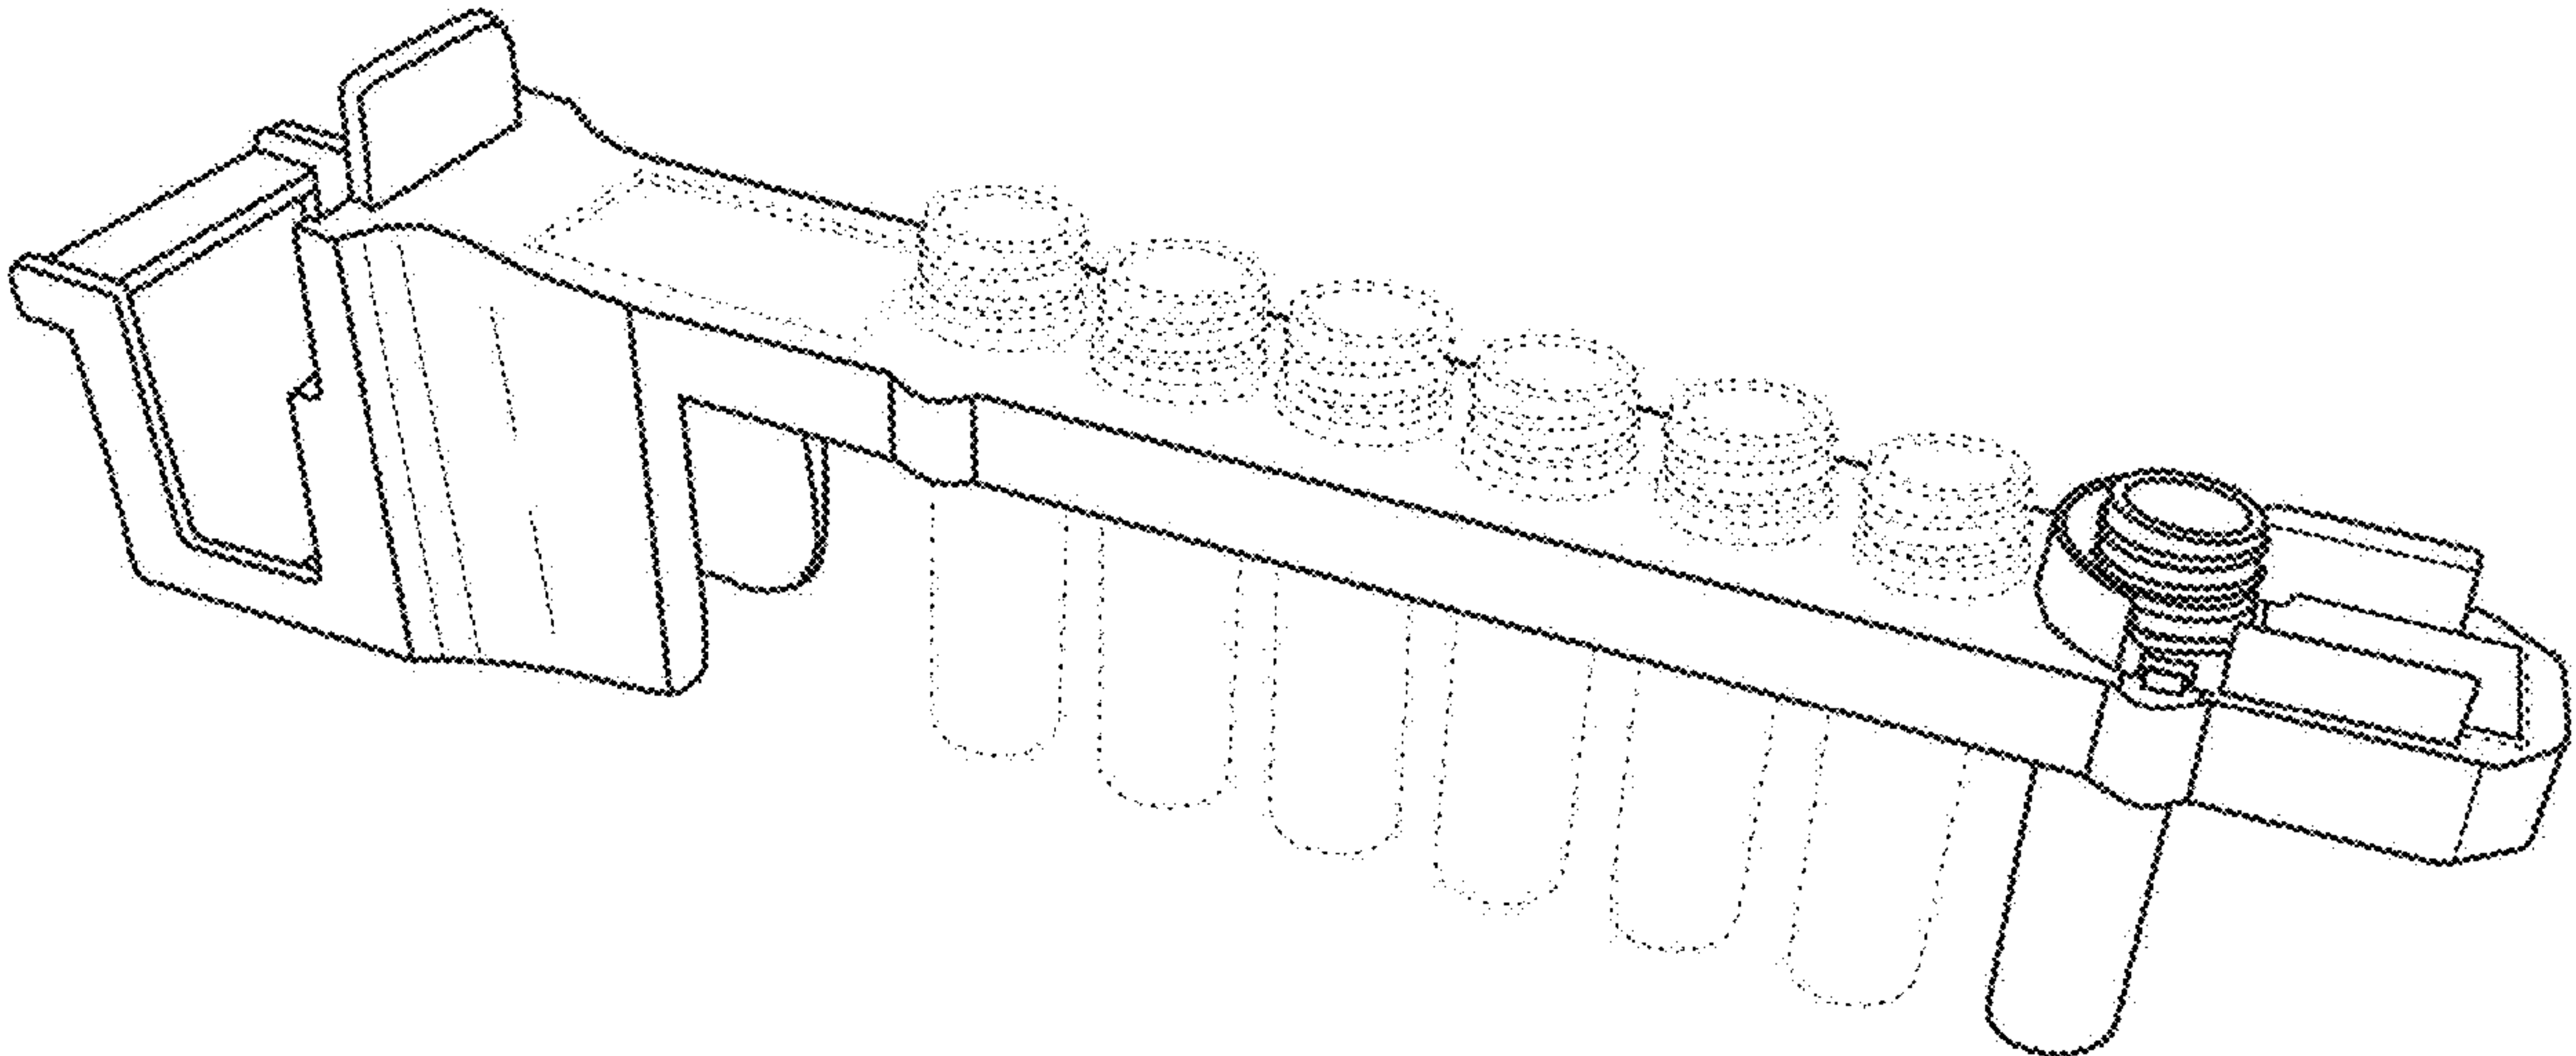

(56)

References Cited

U.S. PATENT DOCUMENTS

9,144,801 B2 * 9/2015 Johnson B01L 9/06

9,222,954 B2 * 12/2015 Lentz G01N 35/1011

D792,981 S * 7/2017 Tajima D24/224

D848,638 S 5/2019 Sims et al.

D849,961 S 5/2019 Muller et al.

D854,707 S 7/2019 Jakobsen et al.

D902,433 S 11/2020 Livingston et al.

D918,417 S 5/2021 O'Mahony et al.

D922,212 S 6/2021 Suchsland

D928,952 S * 8/2021 Verschoor D24/186

D938,612 S * 12/2021 Liu D24/229

2005/0170498 A1 8/2005 Dolley et al.

2009/0129978 A1 * 5/2009 Wilson C08G 83/003

422/400

2010/0203643 A1 8/2010 Self et al.

2011/0286897 A1 11/2011 Uschkureit et al.

2012/0051987 A1 * 3/2012 Johnson B01L 9/06

422/562

2014/0206088 A1 * 7/2014 Lentz B01L 3/527

422/549

2016/0319329 A1 11/2016 Natale et al.

OTHER PUBLICATIONS

Co-pending U.S. Appl. No. 29/740,346, inventors Beckett; Nathan et al., filed Jul. 2, 2020.

Dropix Sample Tray Holder. Online, published date unknown. Retrieved on Oct. 28, 2021 from <https://www.dolomite-microfluidics.com/product/dropix-sample-strip-holder/>.

Oilfield-Wiki. Electrostatic treater. Available at http://www.oilfieldwiki.com/wiki/Electrostatic_treater. Accessed on Mar. 13, 2020.

U.S. Appl. No. 29/740,346 Office Action dated Nov. 2, 2021.

* cited by examiner

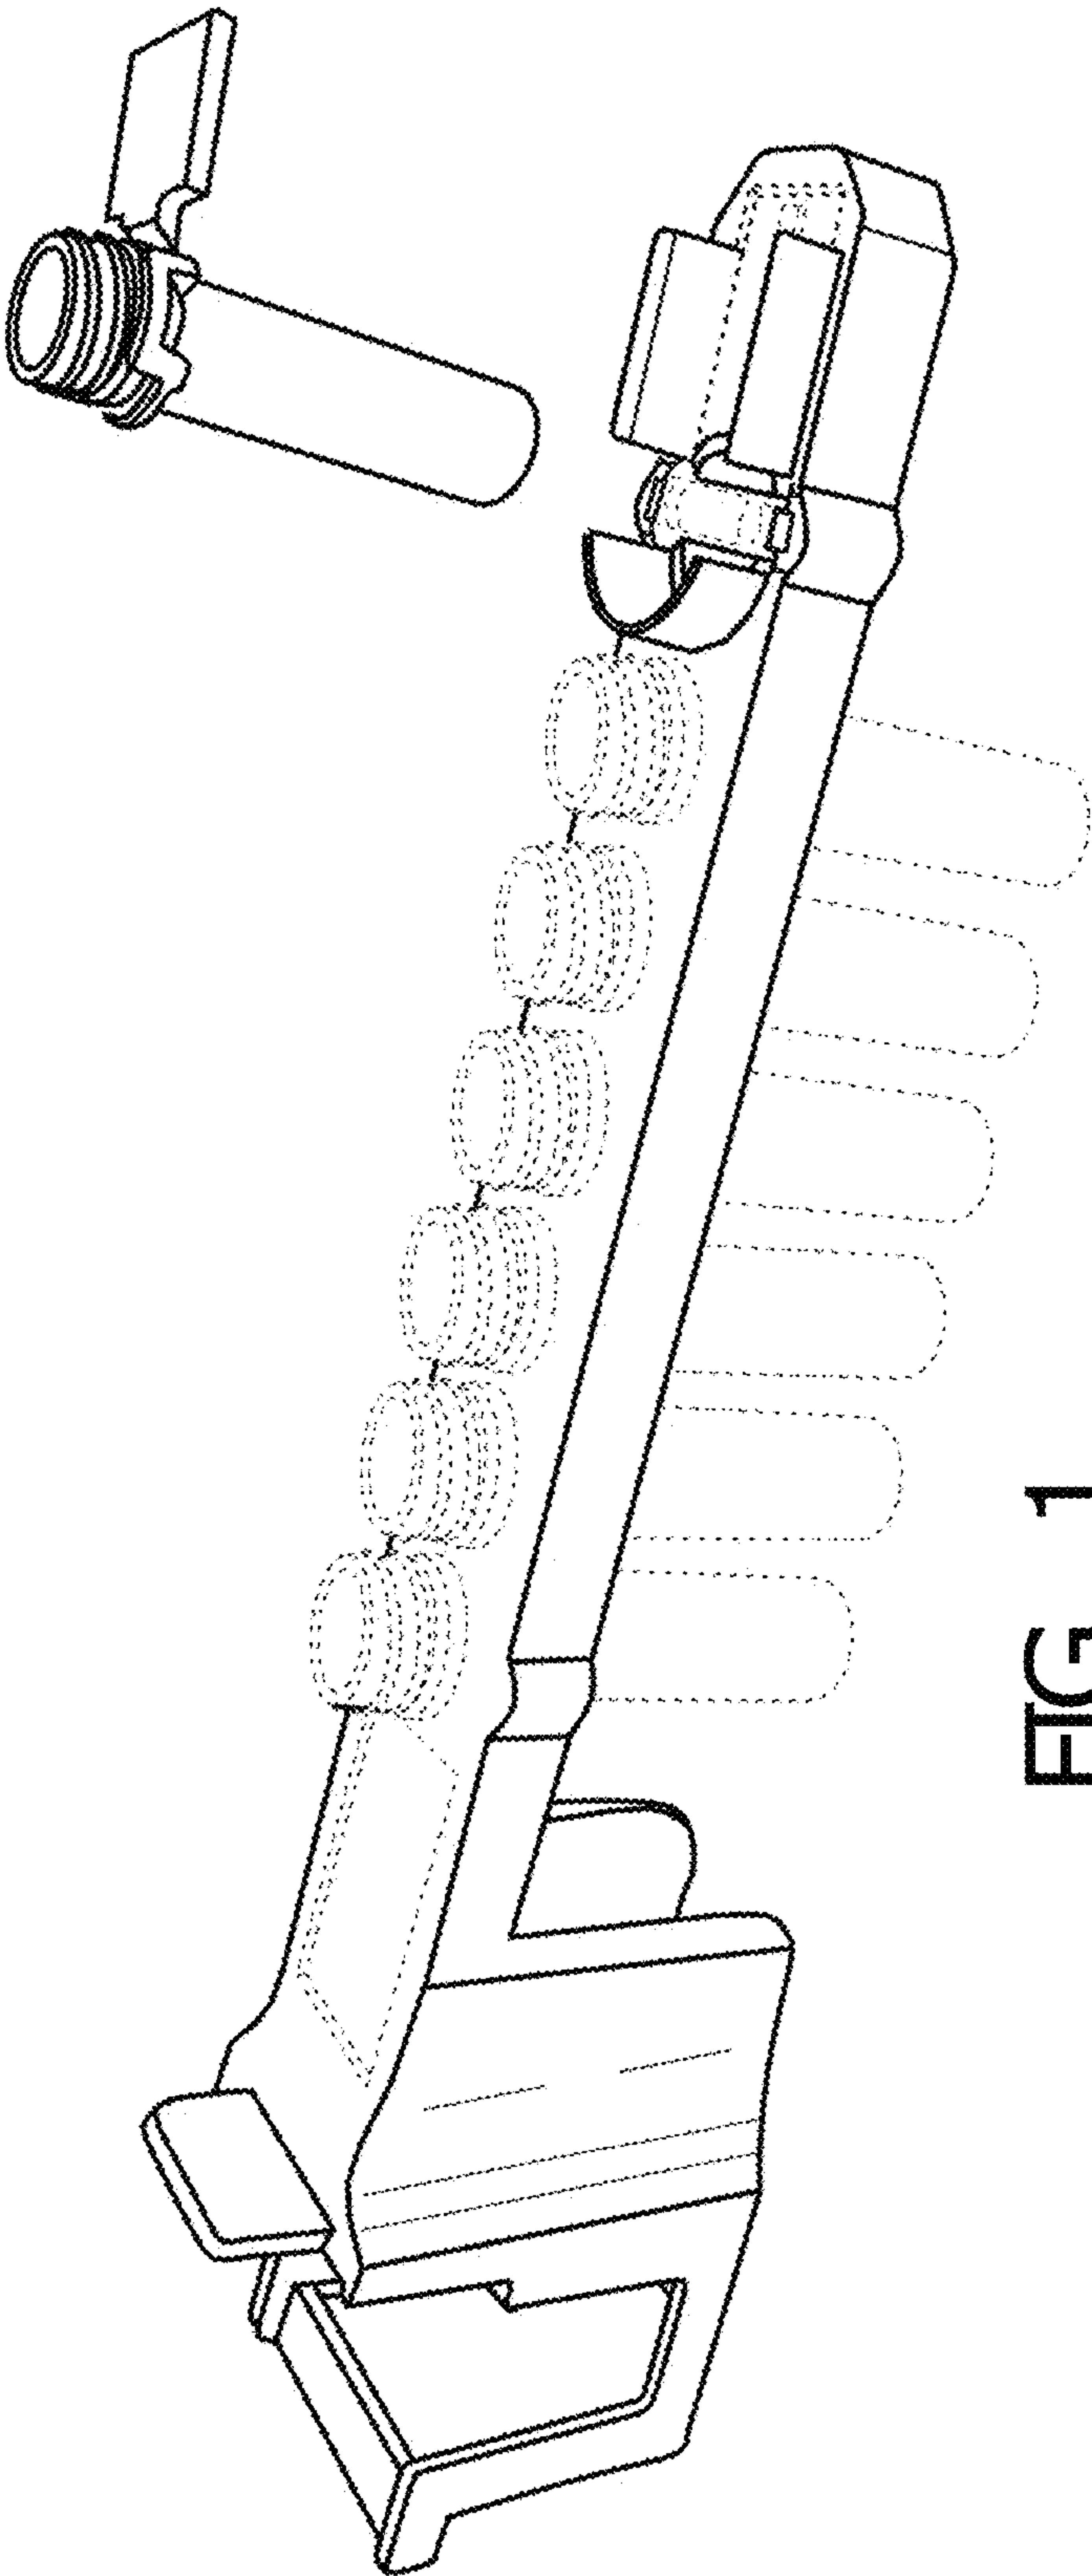


FIG. 1

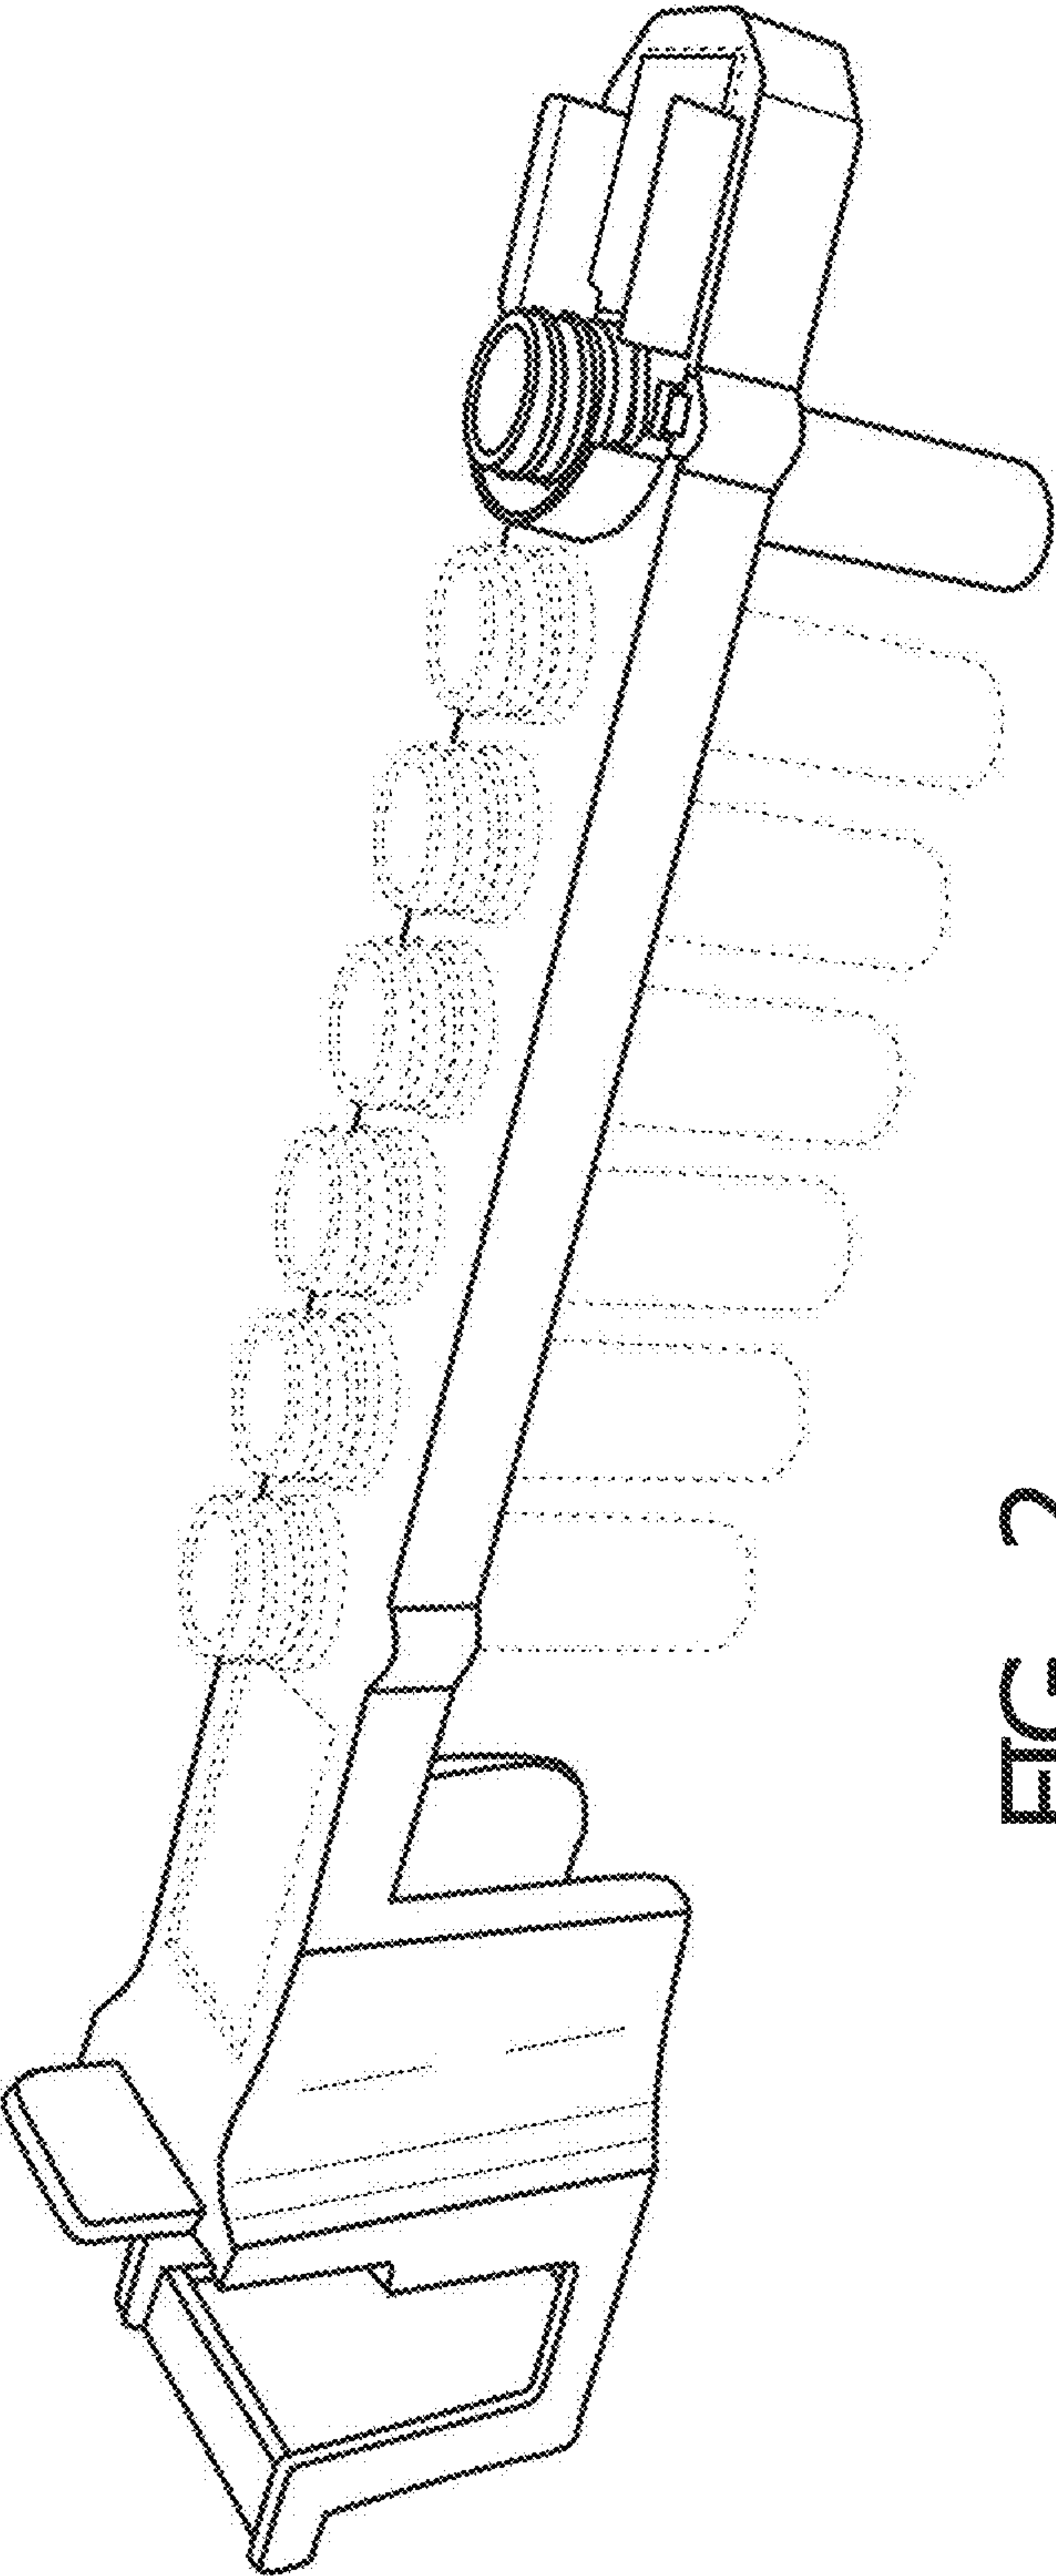


FIG. 2

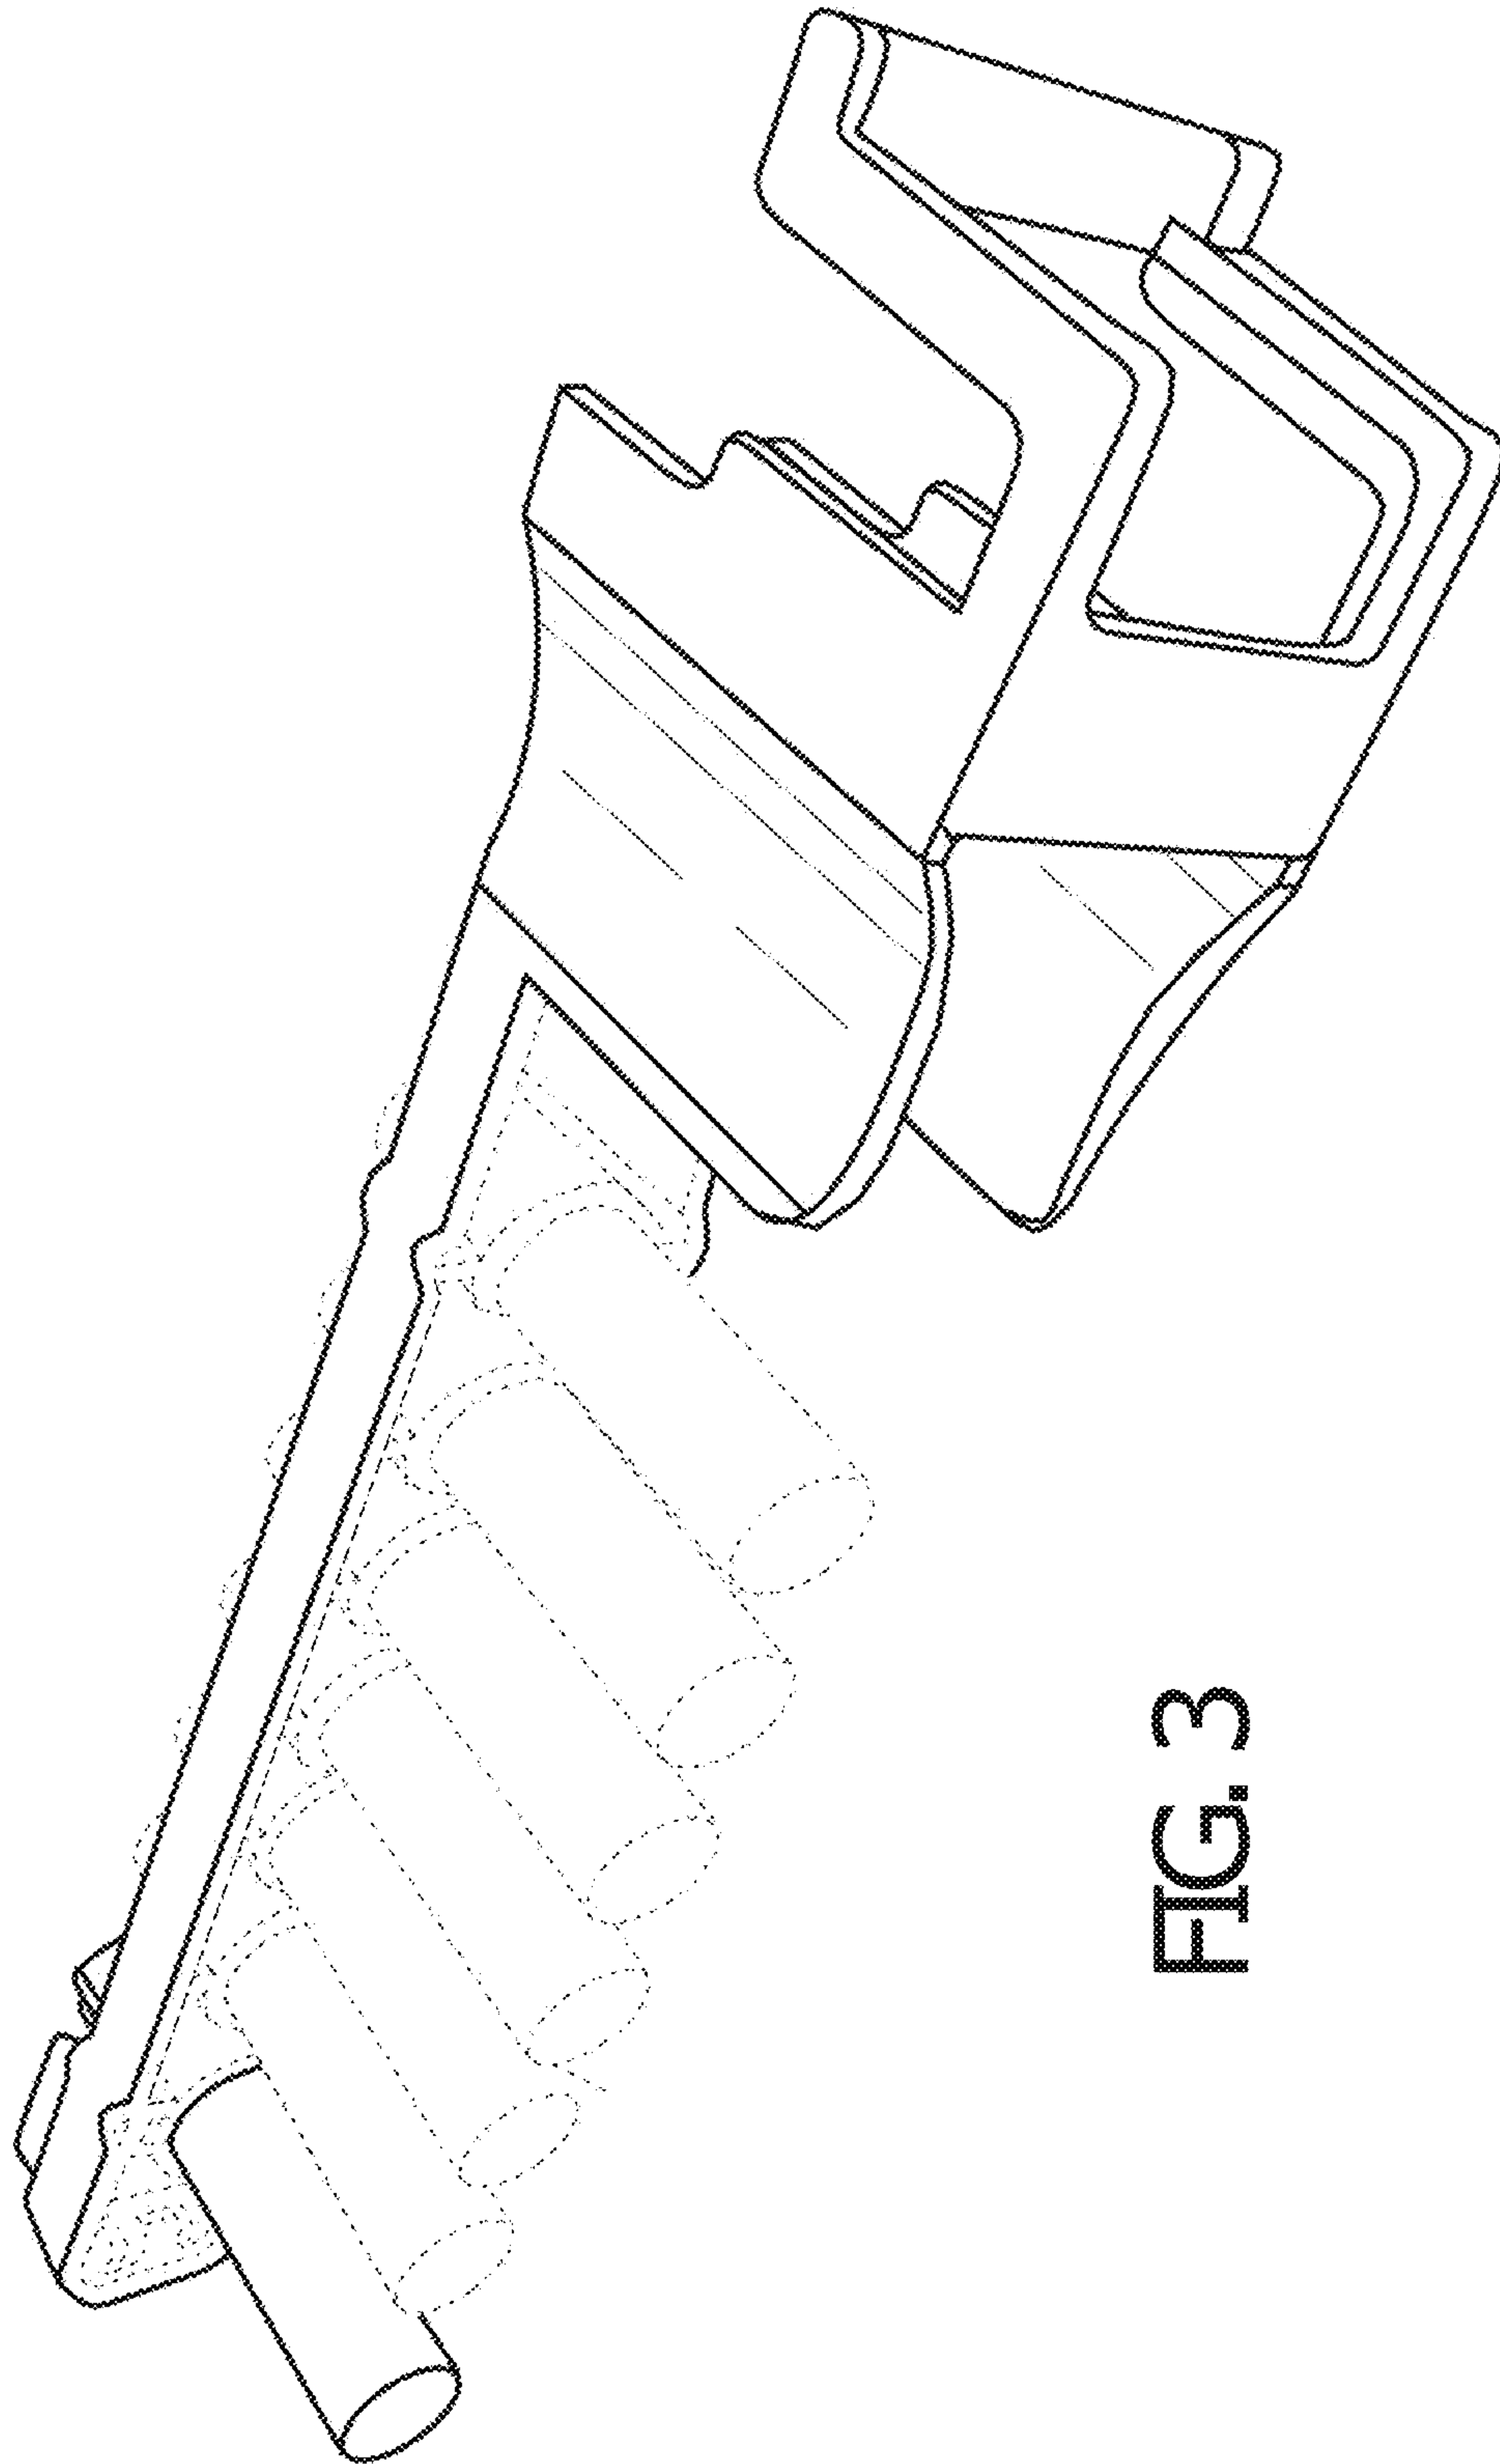


FIG. 3

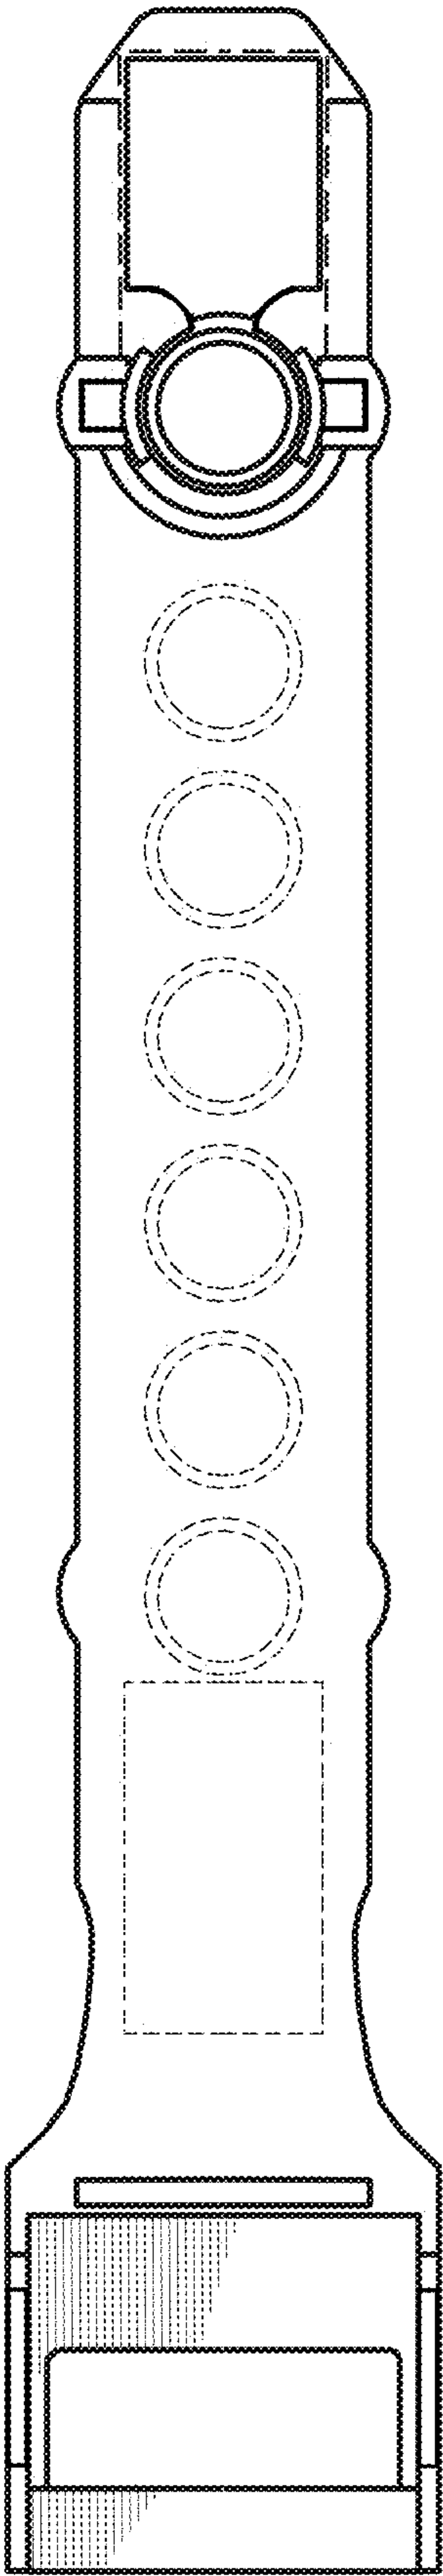


FIG. 4

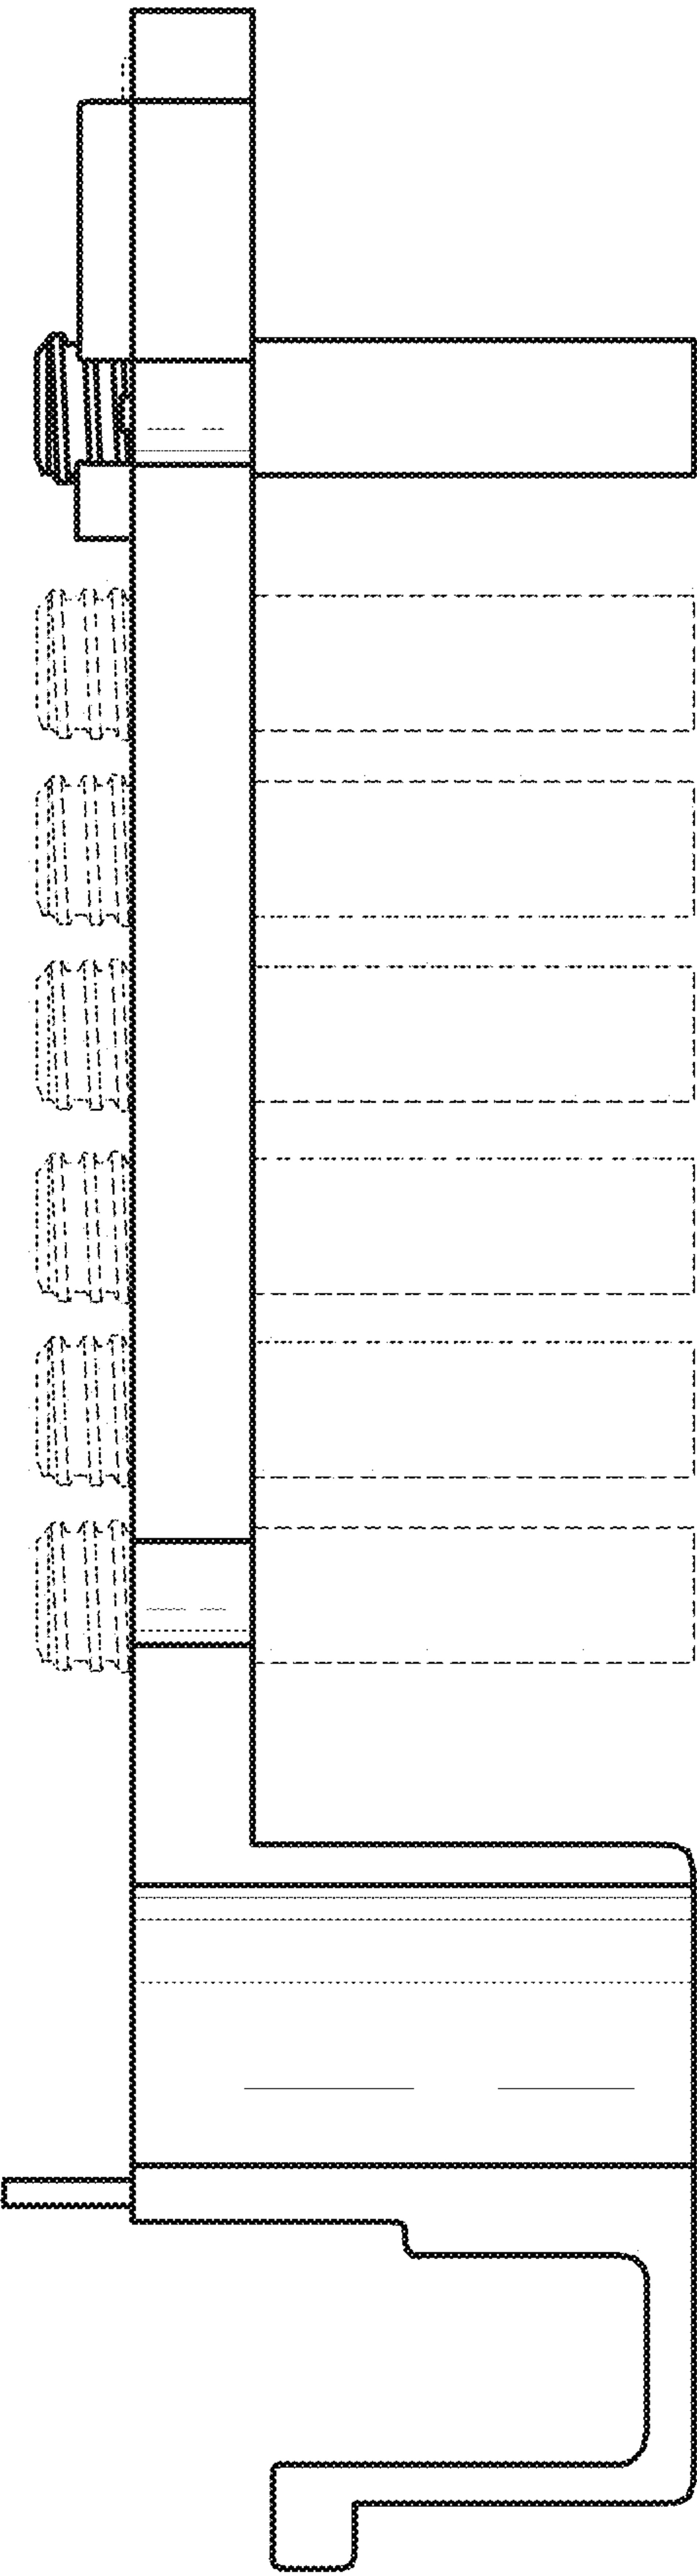


FIG. 5

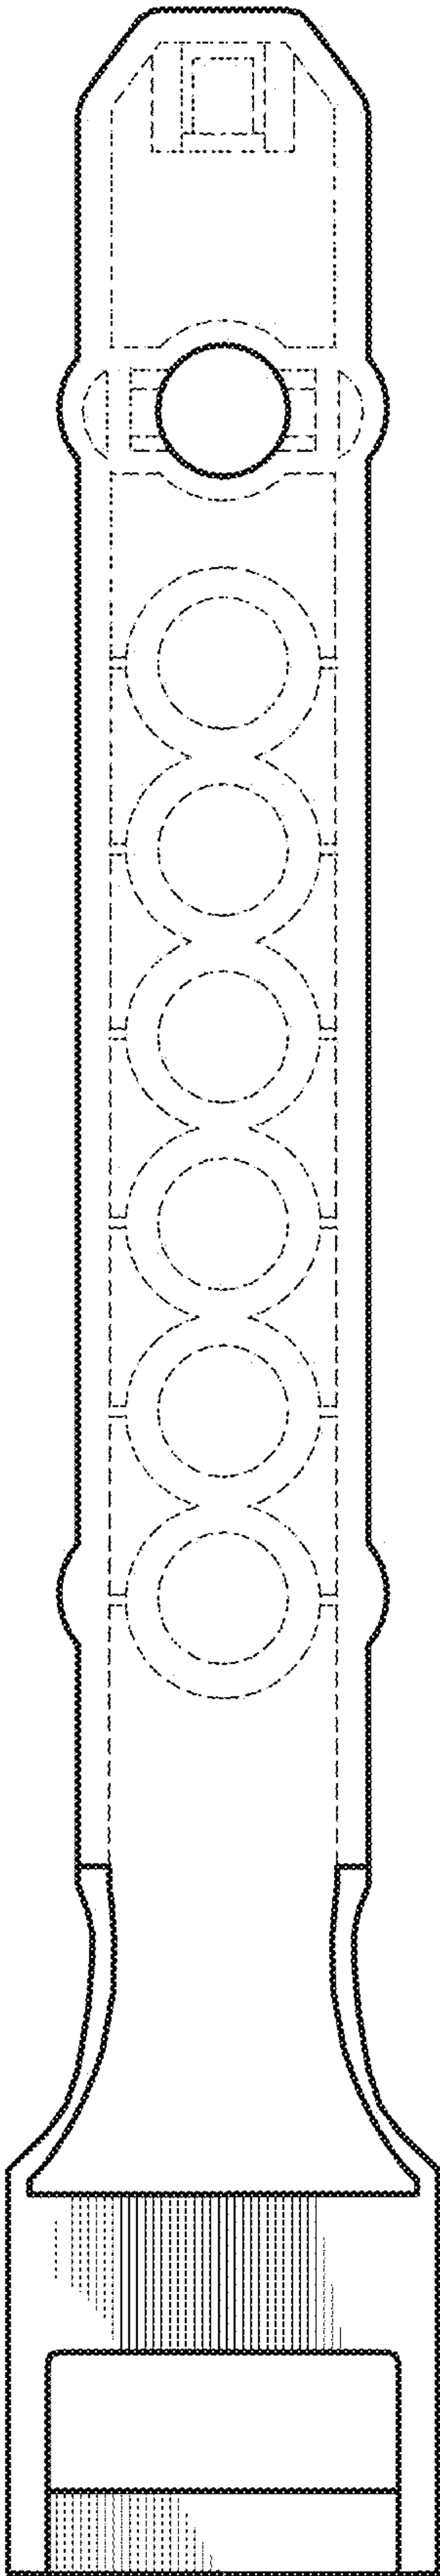


FIG. 6

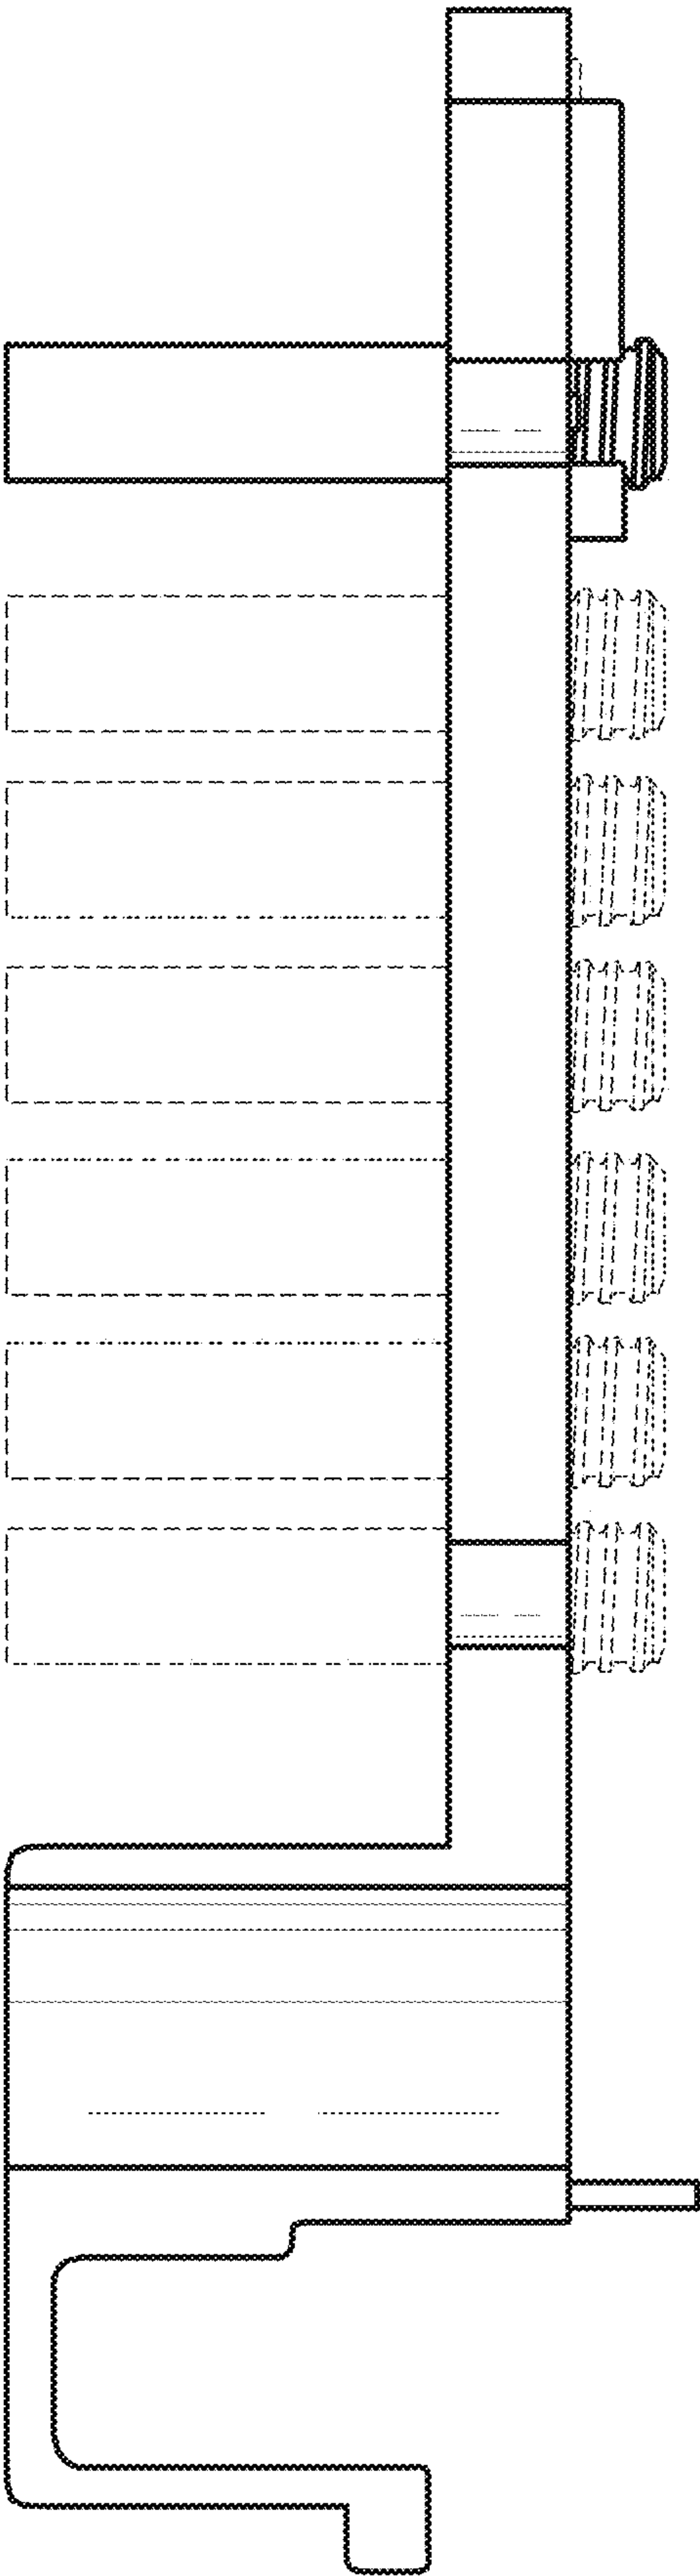


FIG. 7

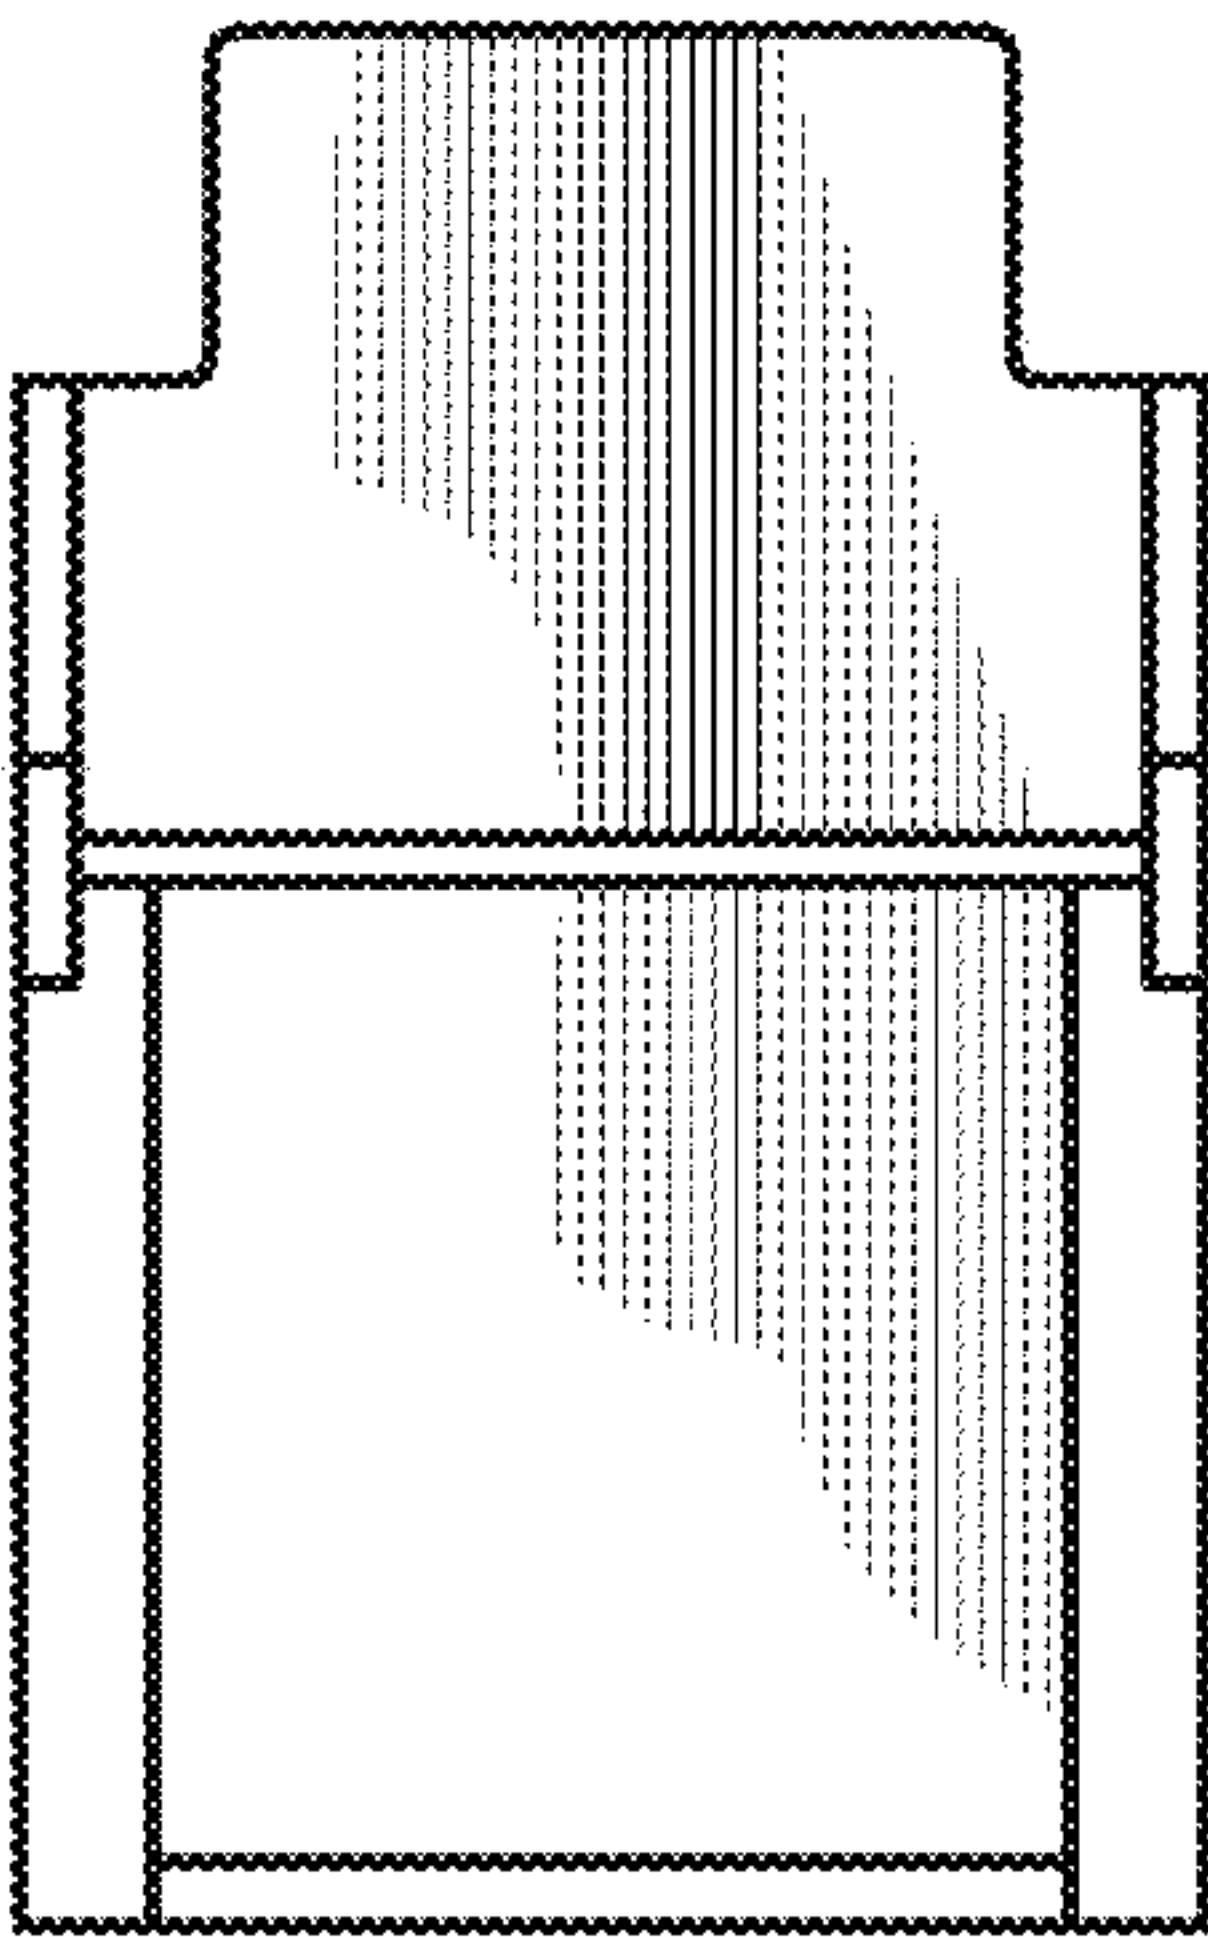


FIG. 8

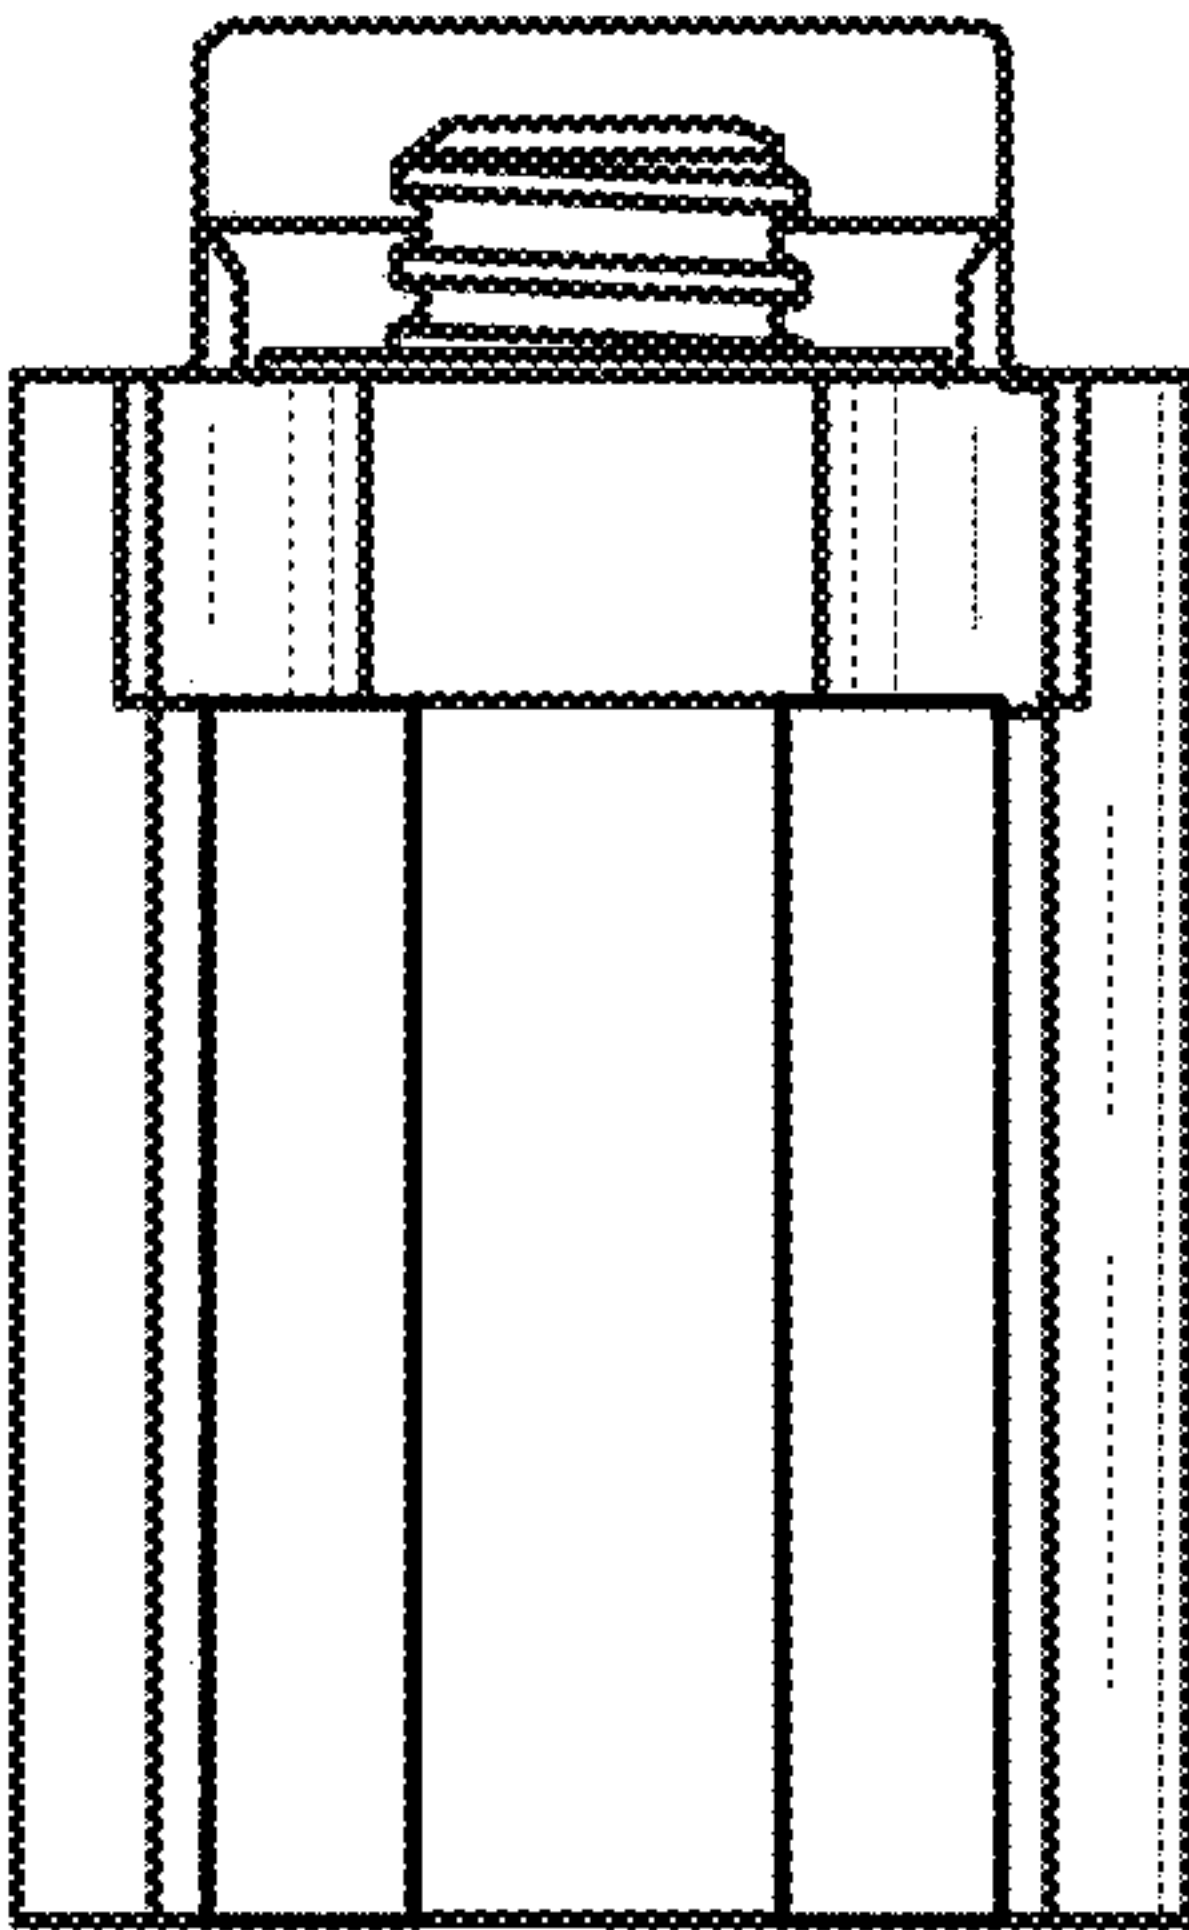


FIG. 9