



US00RE33834E

United States Patent [19]

[11] E

Patent Number: **Re. 33,834**

Warner

[45] Reissued Date of Patent: **Mar. 3, 1992**

[54] **HEART-RELATED PARAMETERS MONITORING APPARATUS**

[75] Inventor: **Glenfield Warner, St. Laurent, Canada**

[73] Assignees: **Sylvia Warner, St. Laurent; Priyamvada Sankar, Brossard, both of Canada**

[21] Appl. No.: **556,101**

[22] Filed: **Jul. 20, 1990**

Related U.S. Patent Documents

Reissue of:

[64] Patent No.: **4,834,107**
Issued: **May 30, 1989**
Appl. No.: **105,803**
Filed: **Oct. 8, 1987**

U.S. Applications:

[63] Continuation-in-part of Ser. No. 59,520, Jun. 8, 1987, abandoned, which is a continuation-in-part of Ser. No. 807,693, Dec. 11, 1985, abandoned, which is a continuation-in-part of Ser. No. 608,955, May 10, 1984, abandoned.

[51] Int. Cl.⁵ **A61B 5/02**

[52] U.S. Cl. **128/668; 128/666; 128/691; 128/694; 128/713**

[58] Field of Search **128/666, 668, 691, 694, 128/713**

[56] References Cited

U.S. PATENT DOCUMENTS

4,030,485 6/1977 Warner 128/2.05 A
4,425,920 1/1984 Bowland 128/672

FOREIGN PATENT DOCUMENTS

2092309 8/1982 United Kingdom 128/672

Primary Examiner—Asok Pal

Attorney, Agent, or Firm—Chilton, Alix & Van Kirk

[57] ABSTRACT

A non-invasive method, and an apparatus, for determining heart-related parameters in patients. The method and apparatus determine pulse pressure, time constant of the arterial system, systolic and diastolic pressure, peripheral resistance, cardiac output and mean arterial blood pressure.

18 Claims, 6 Drawing Sheets

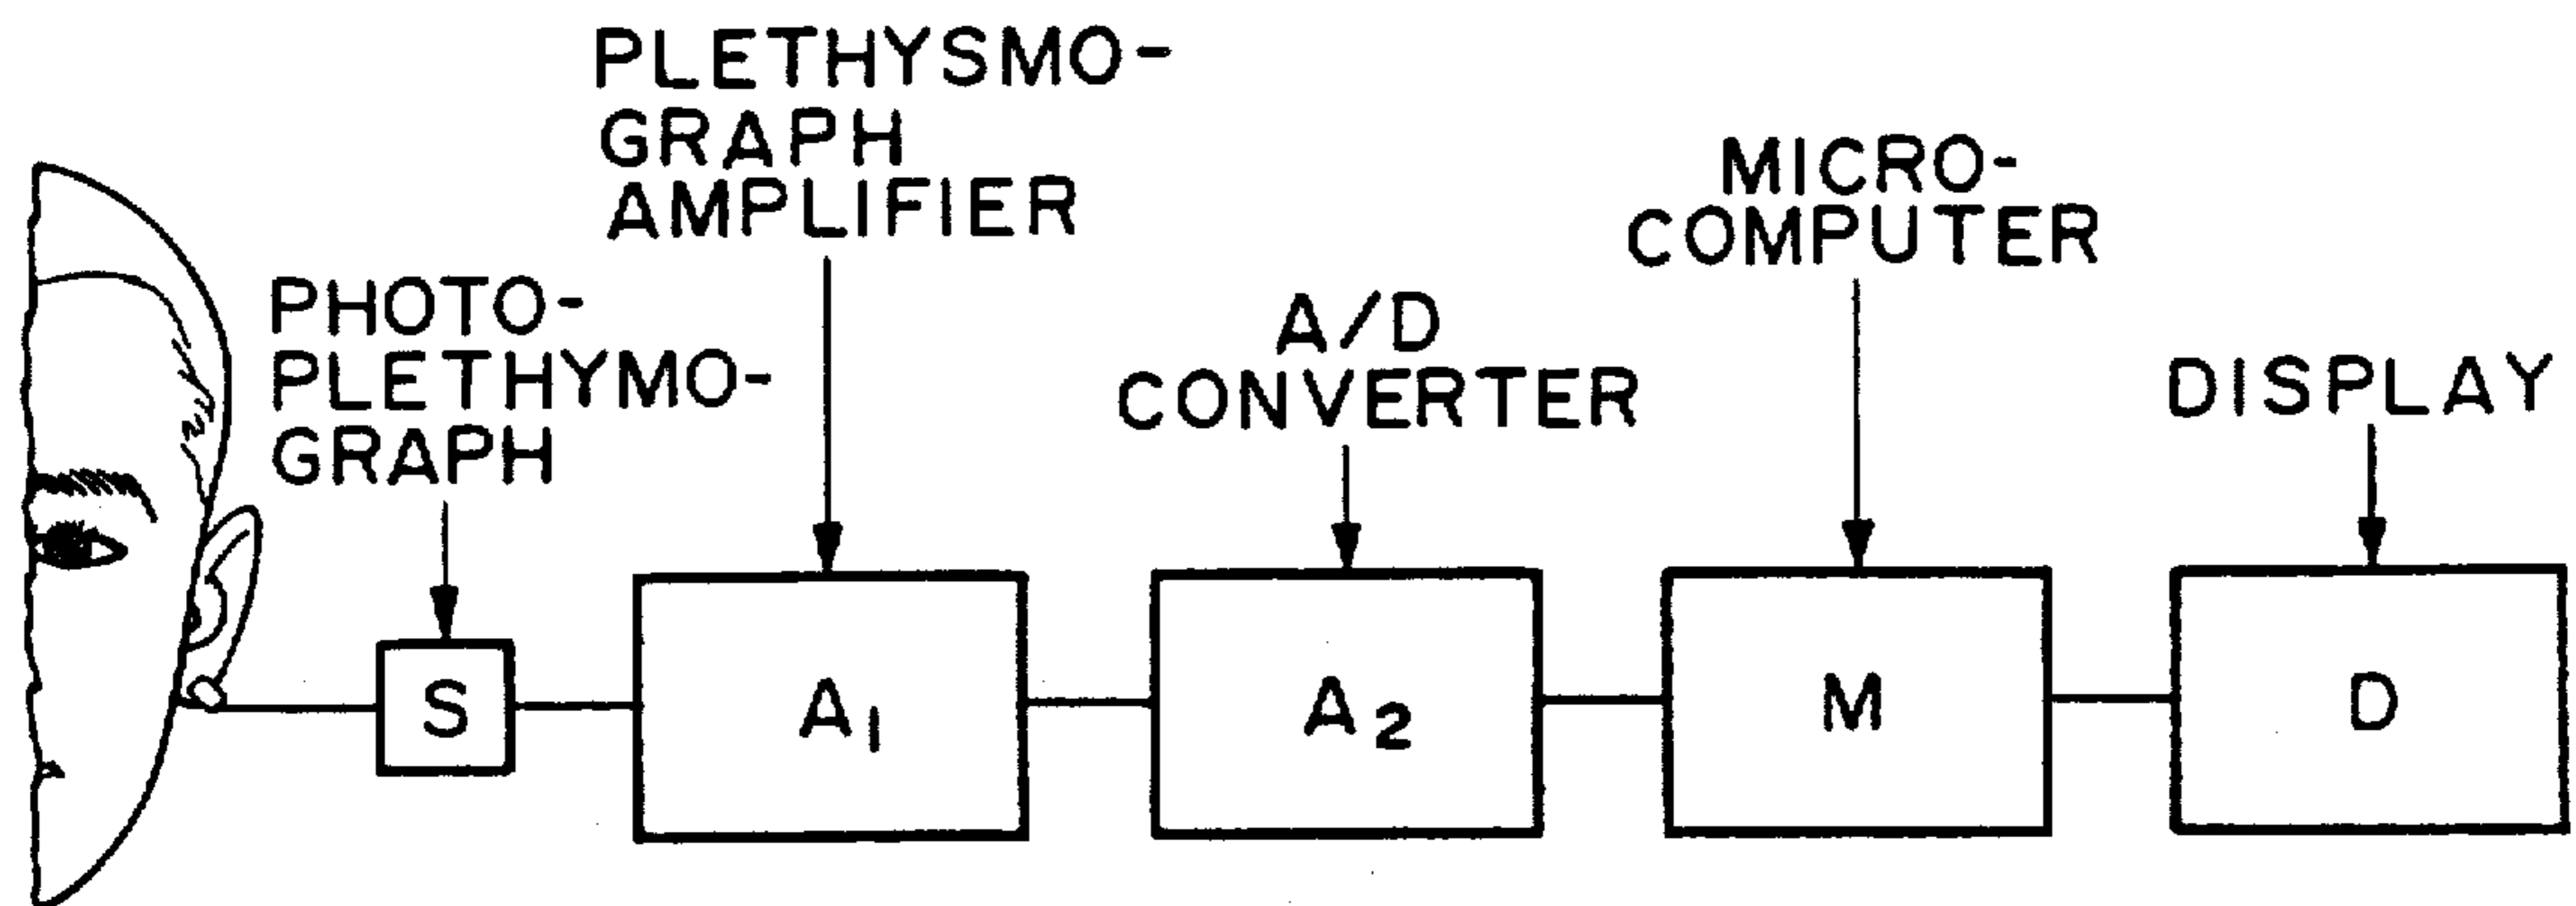


FIG. 1

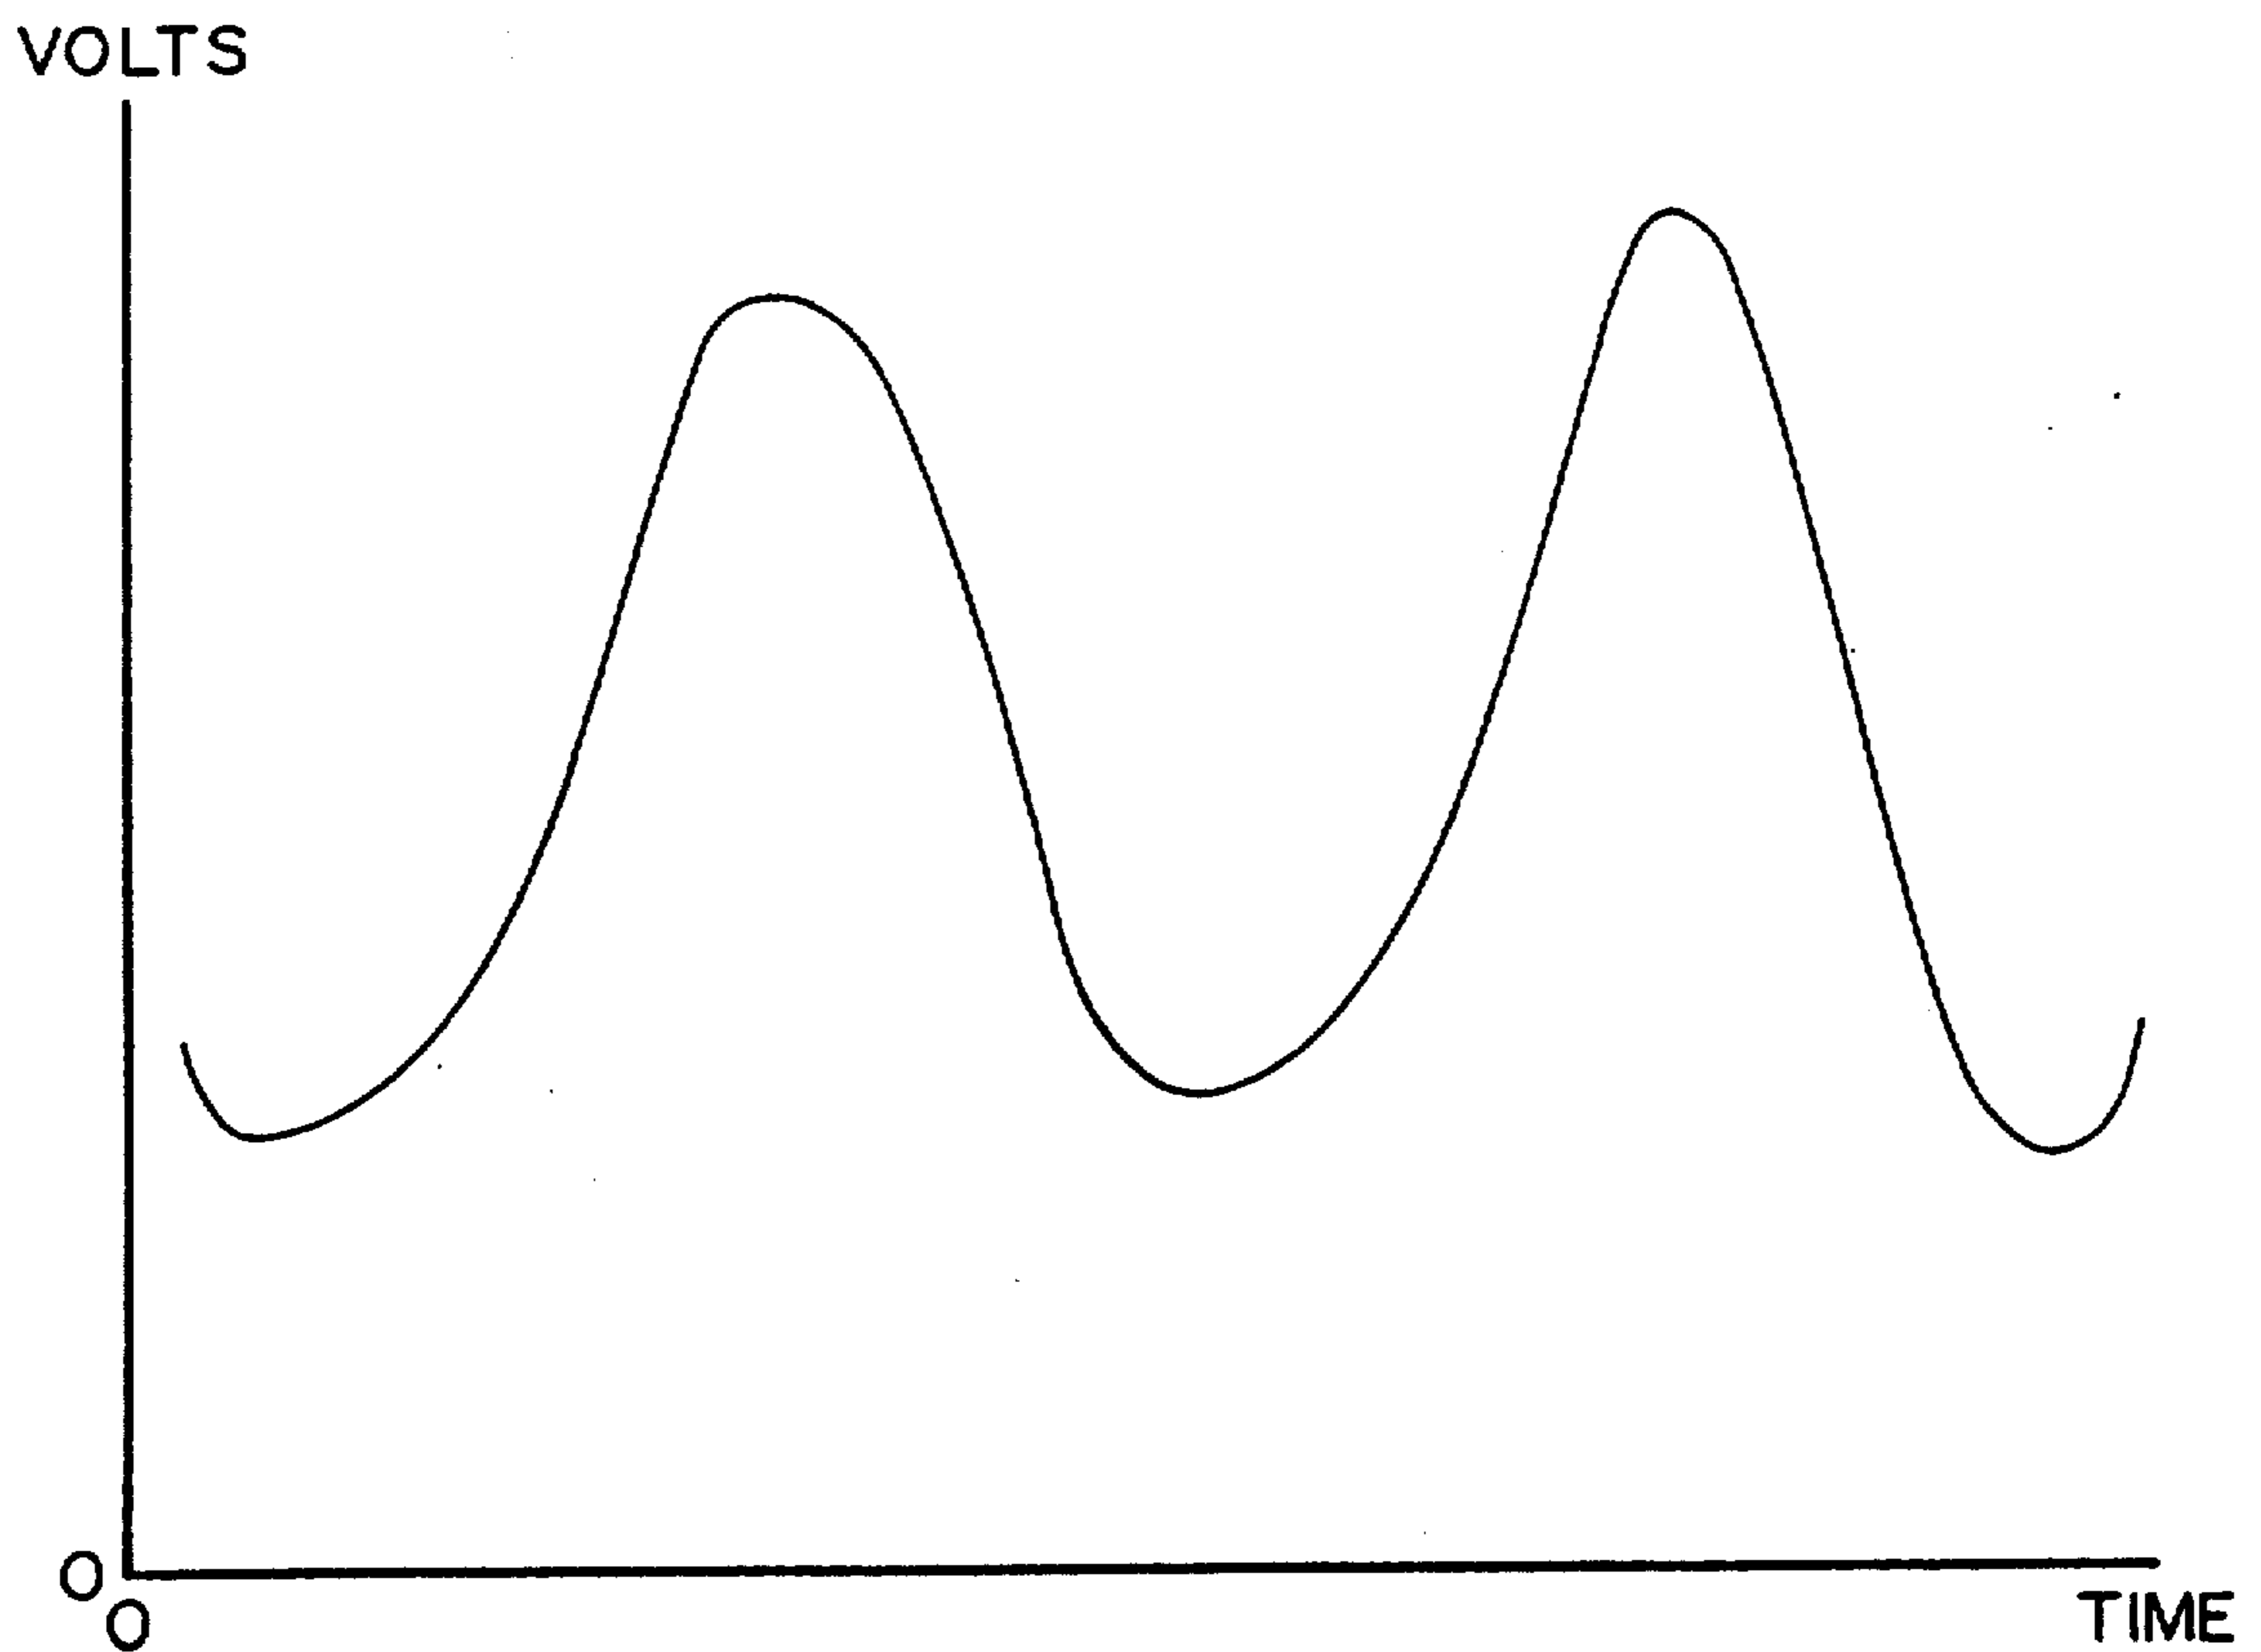


FIG. 2

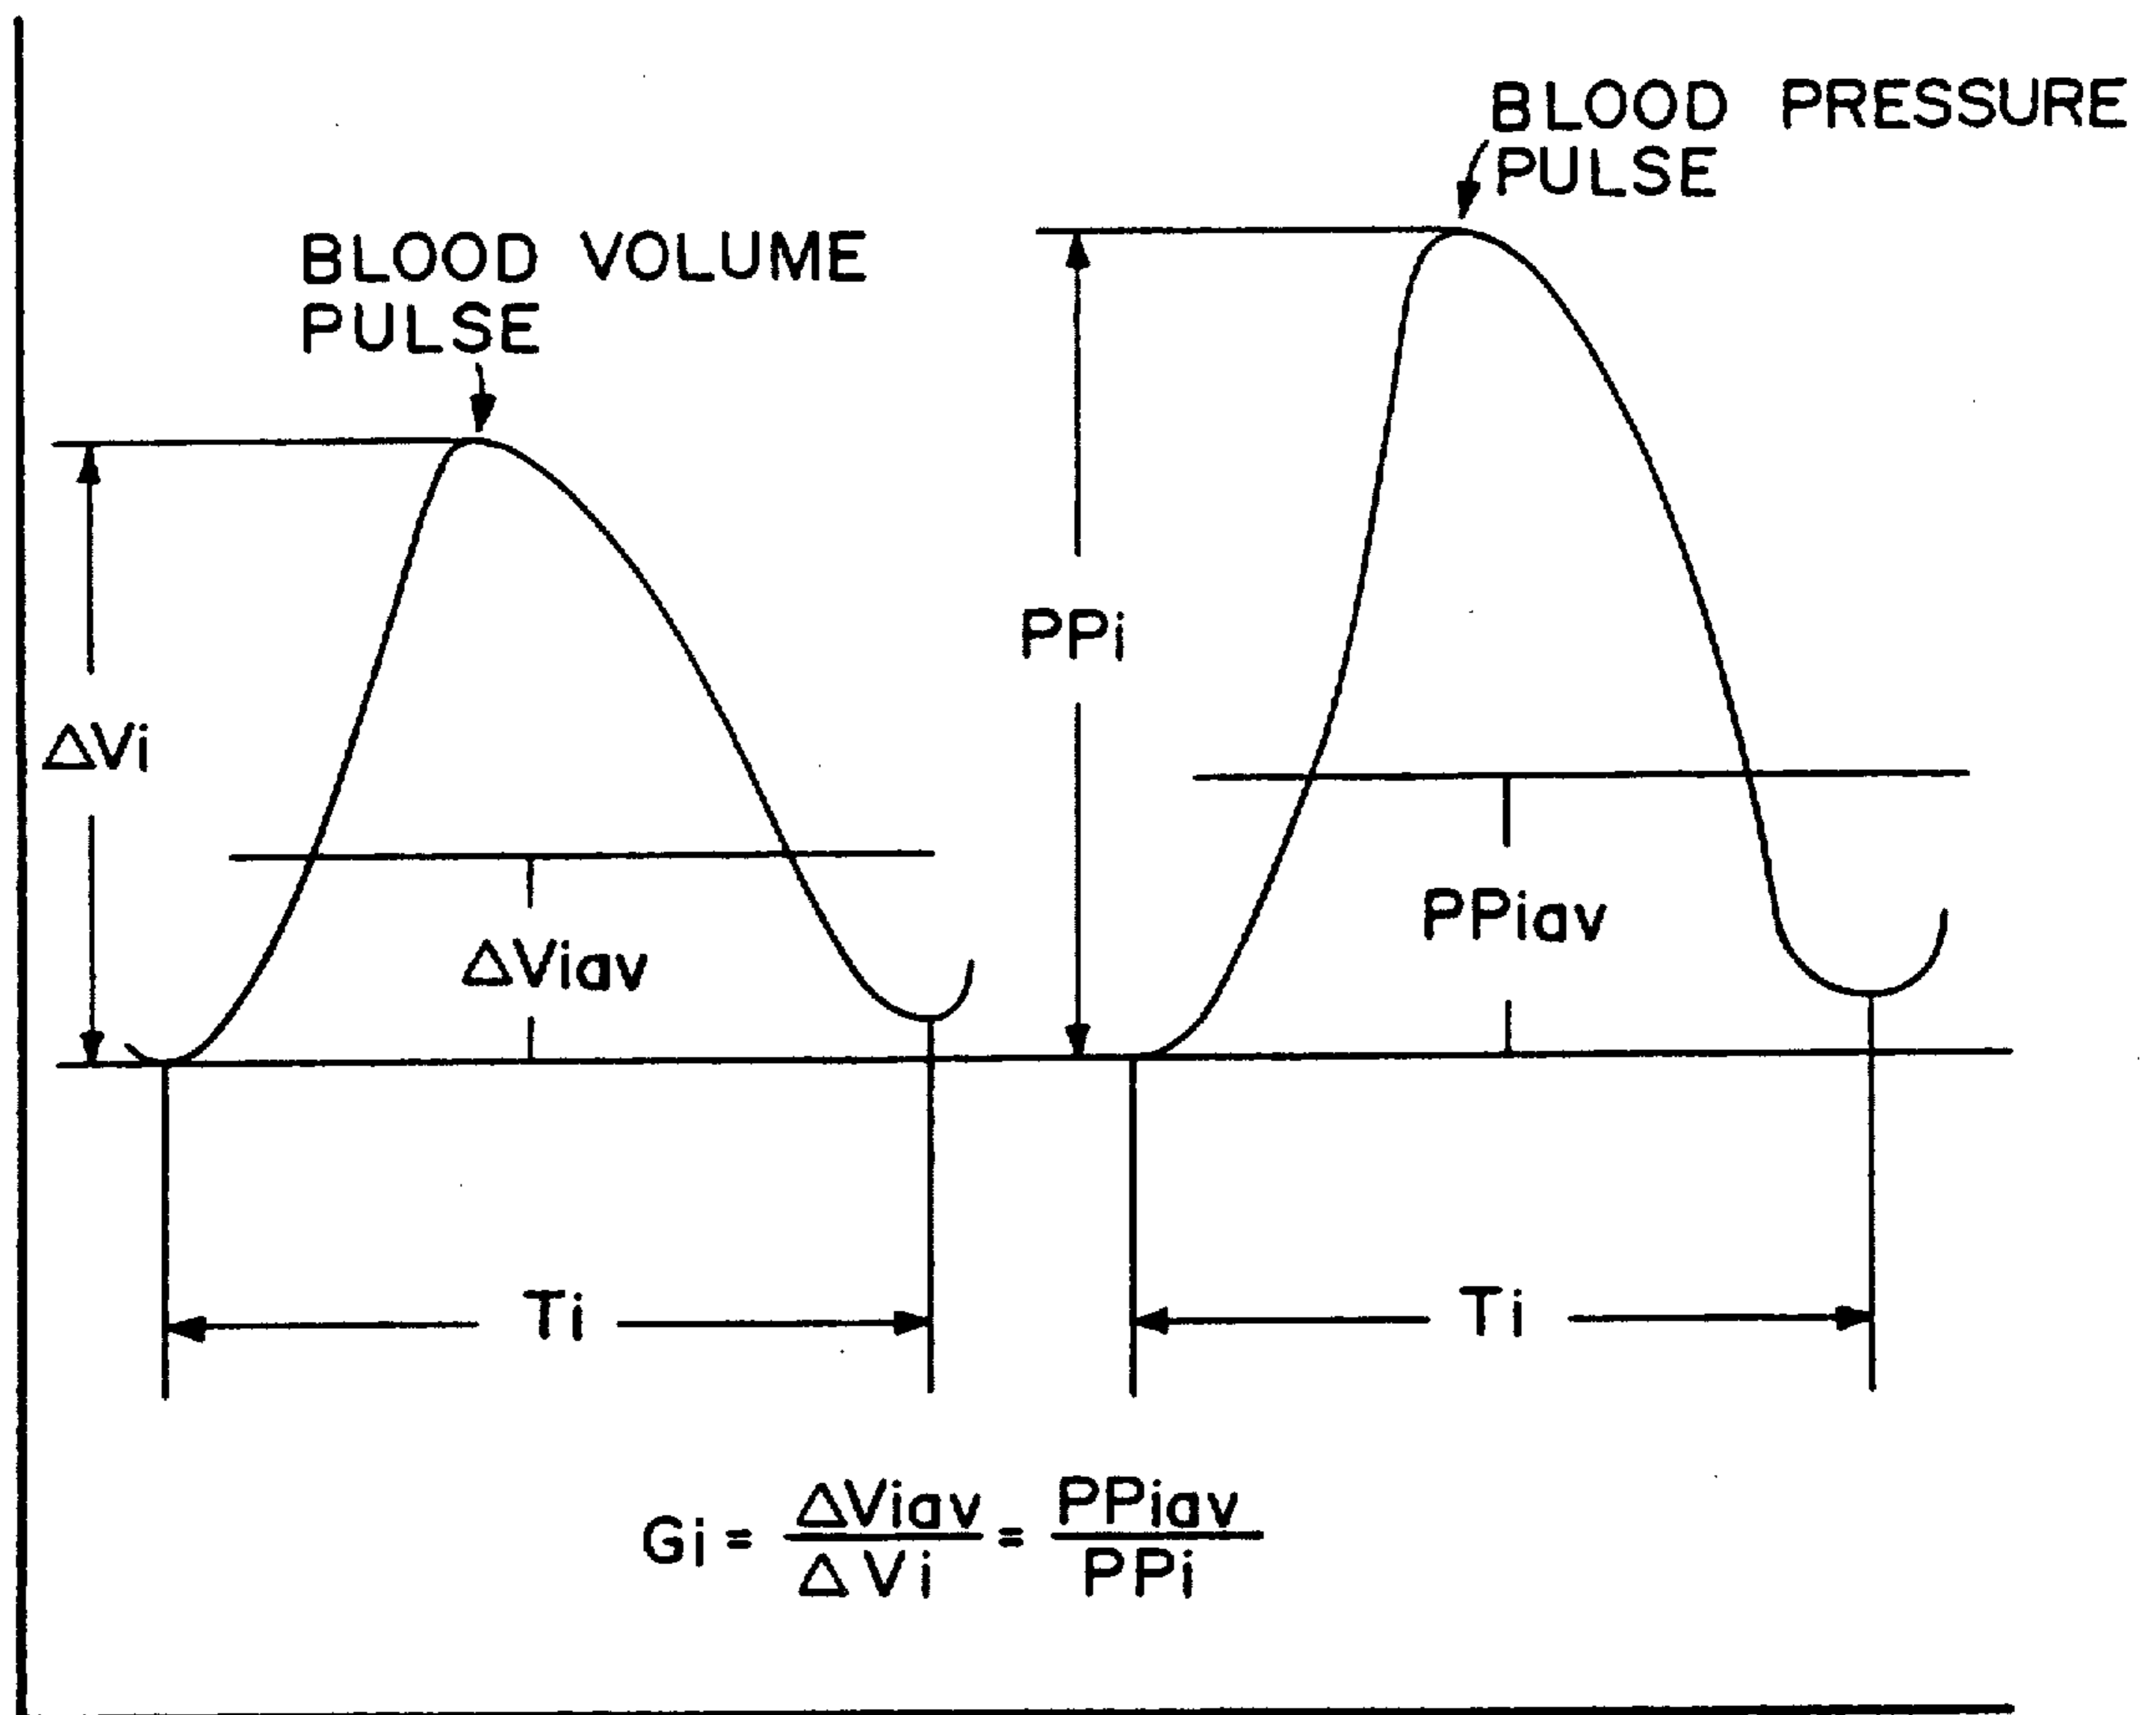
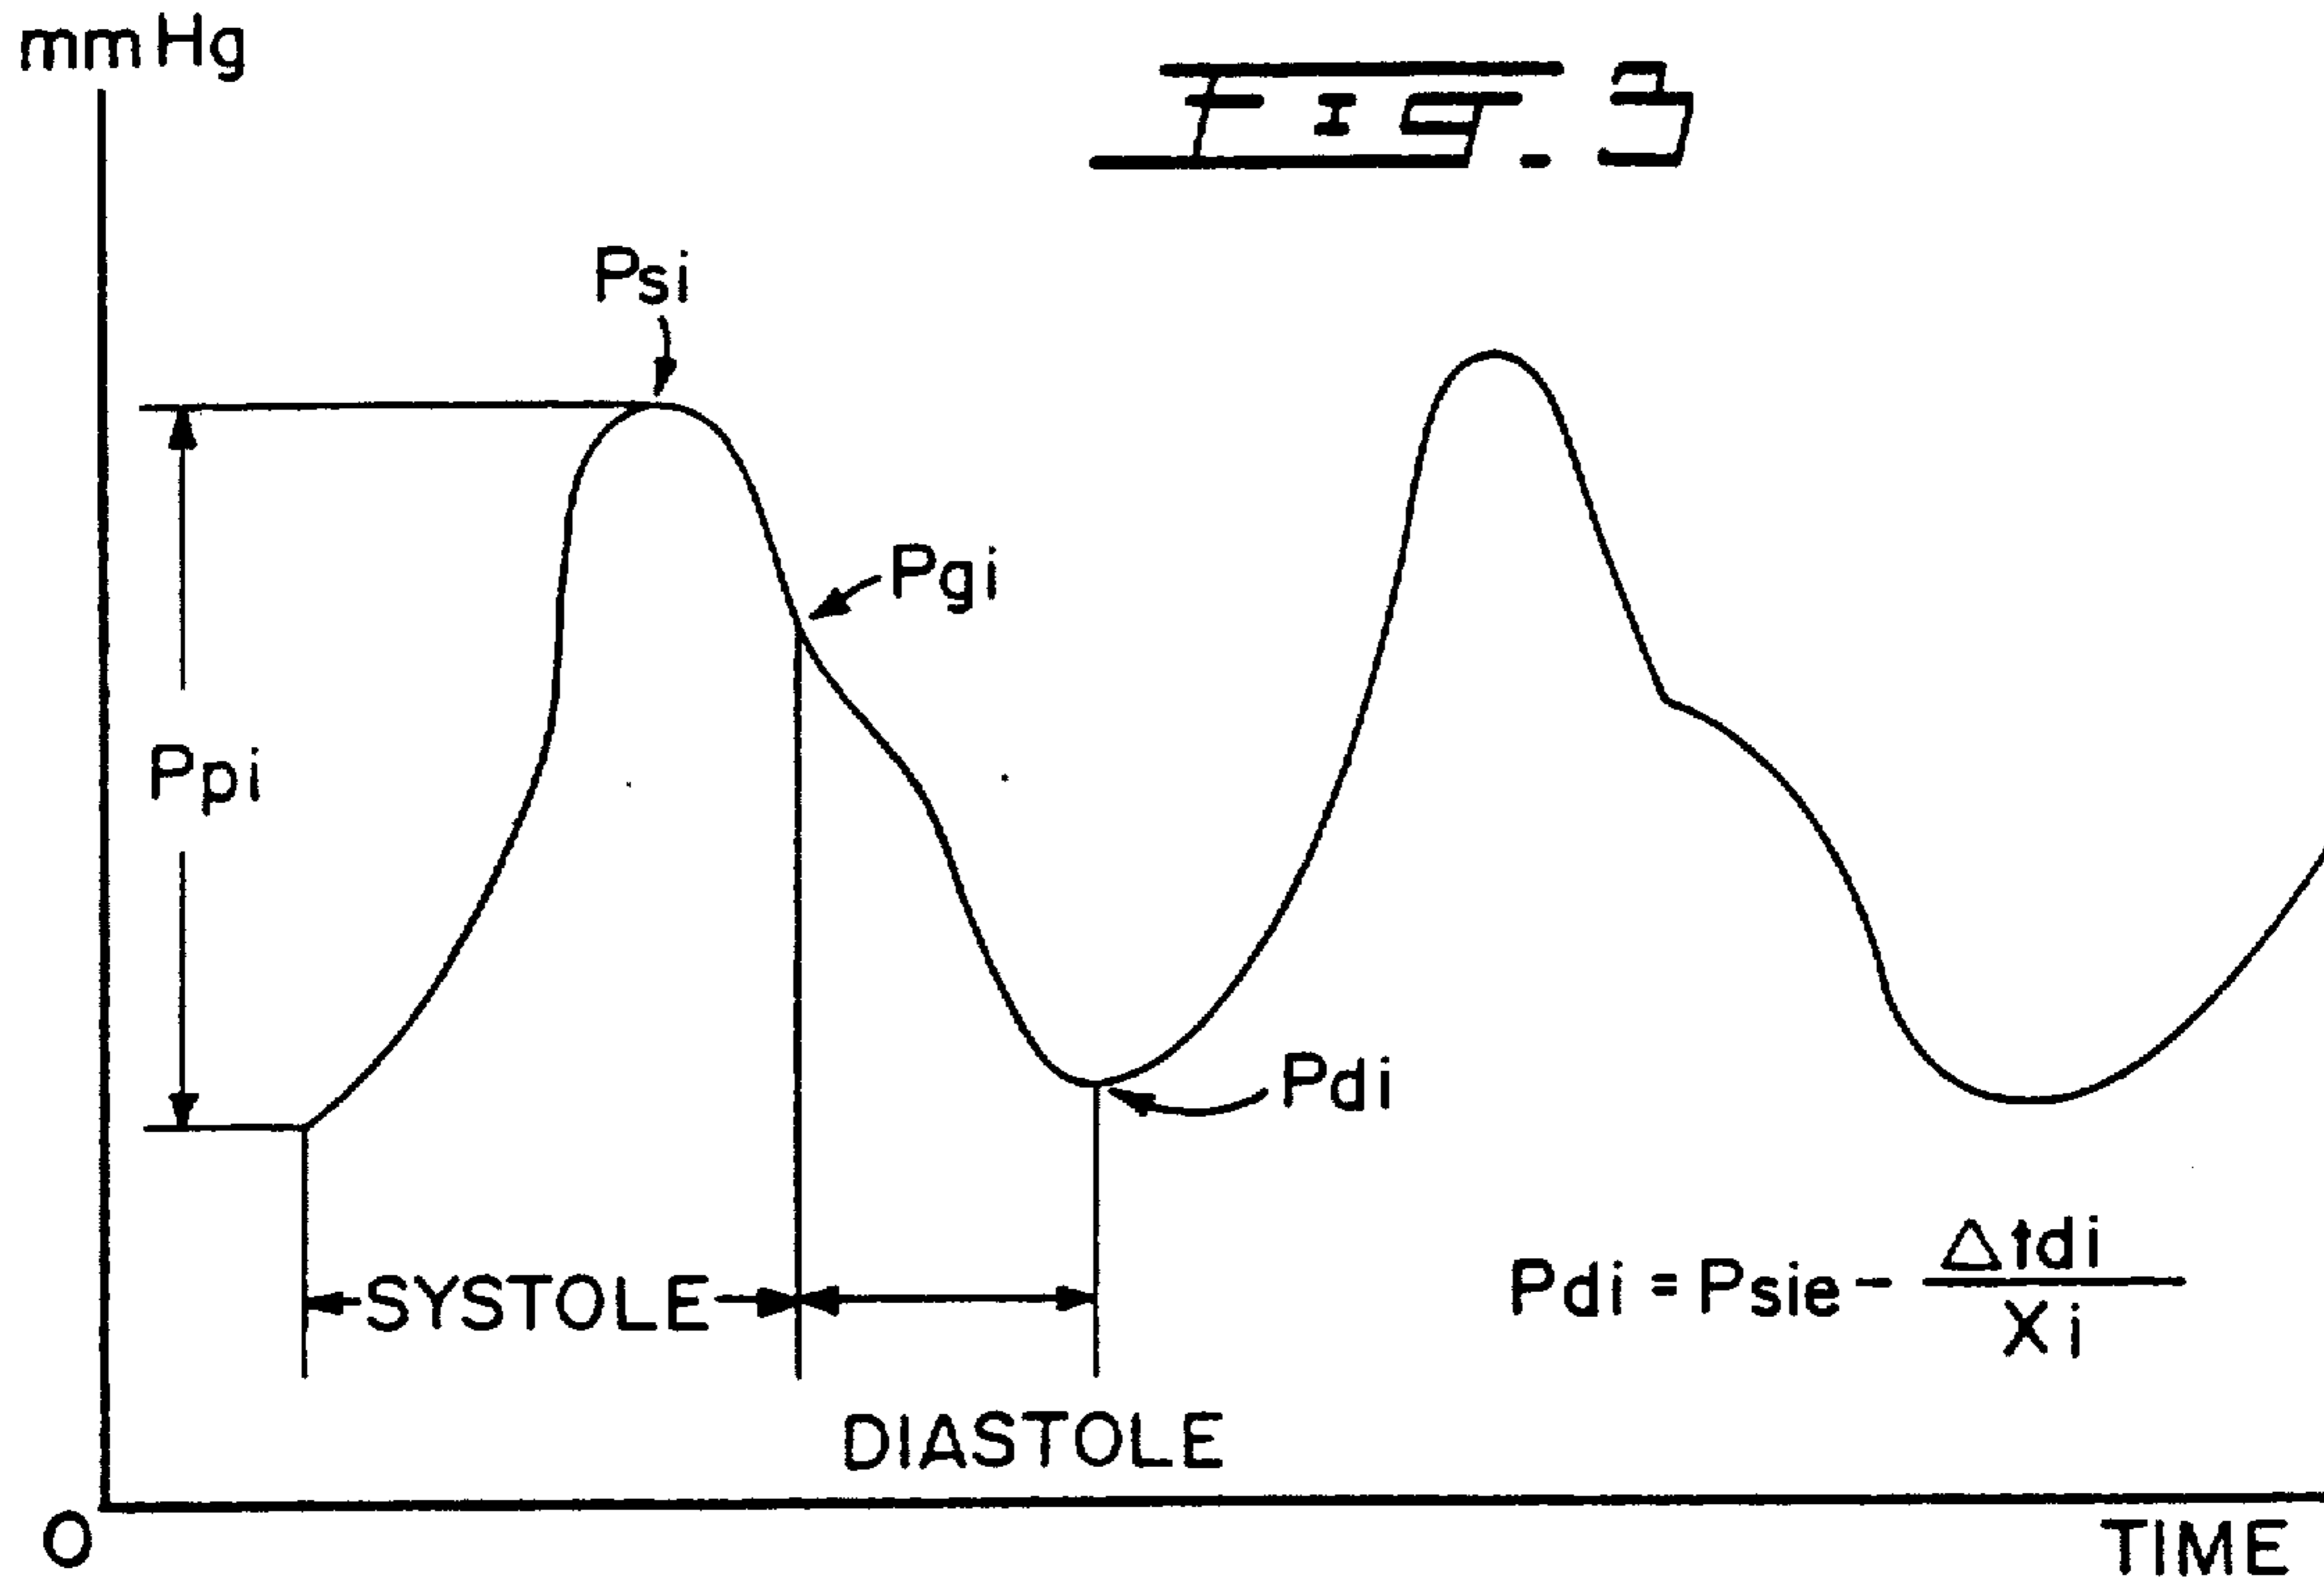


FIG. 5

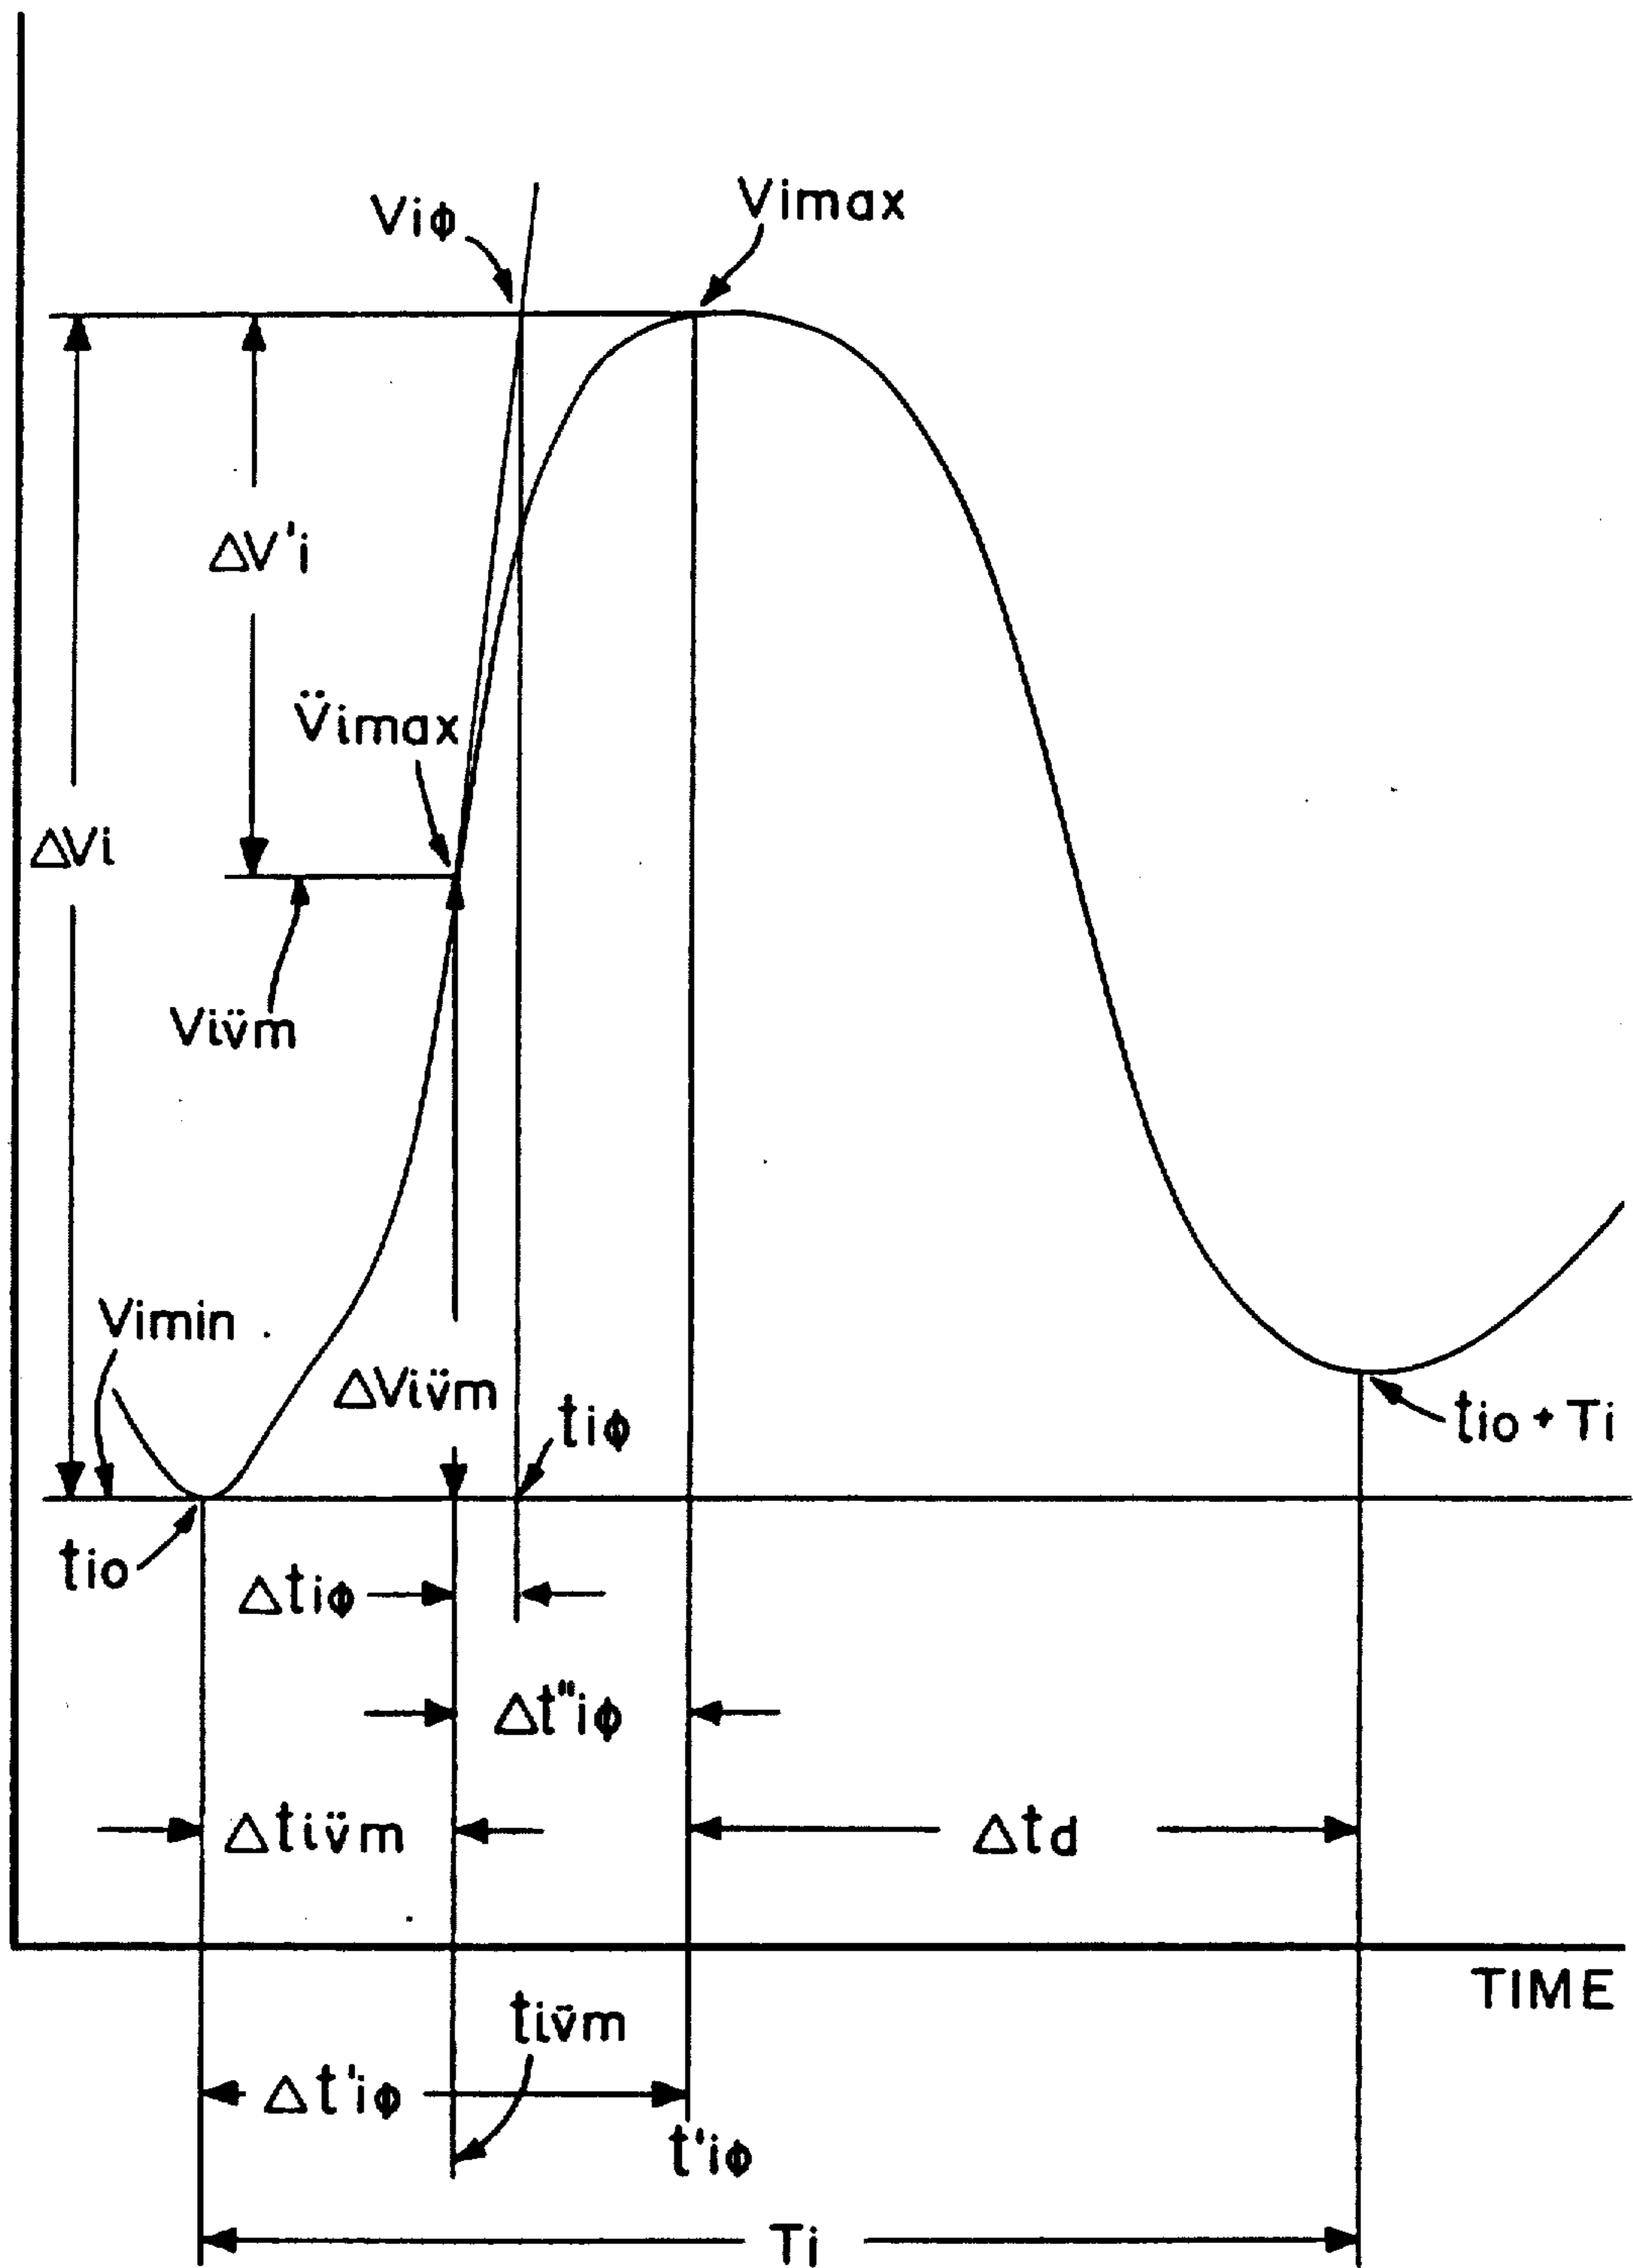


FIG. 4A

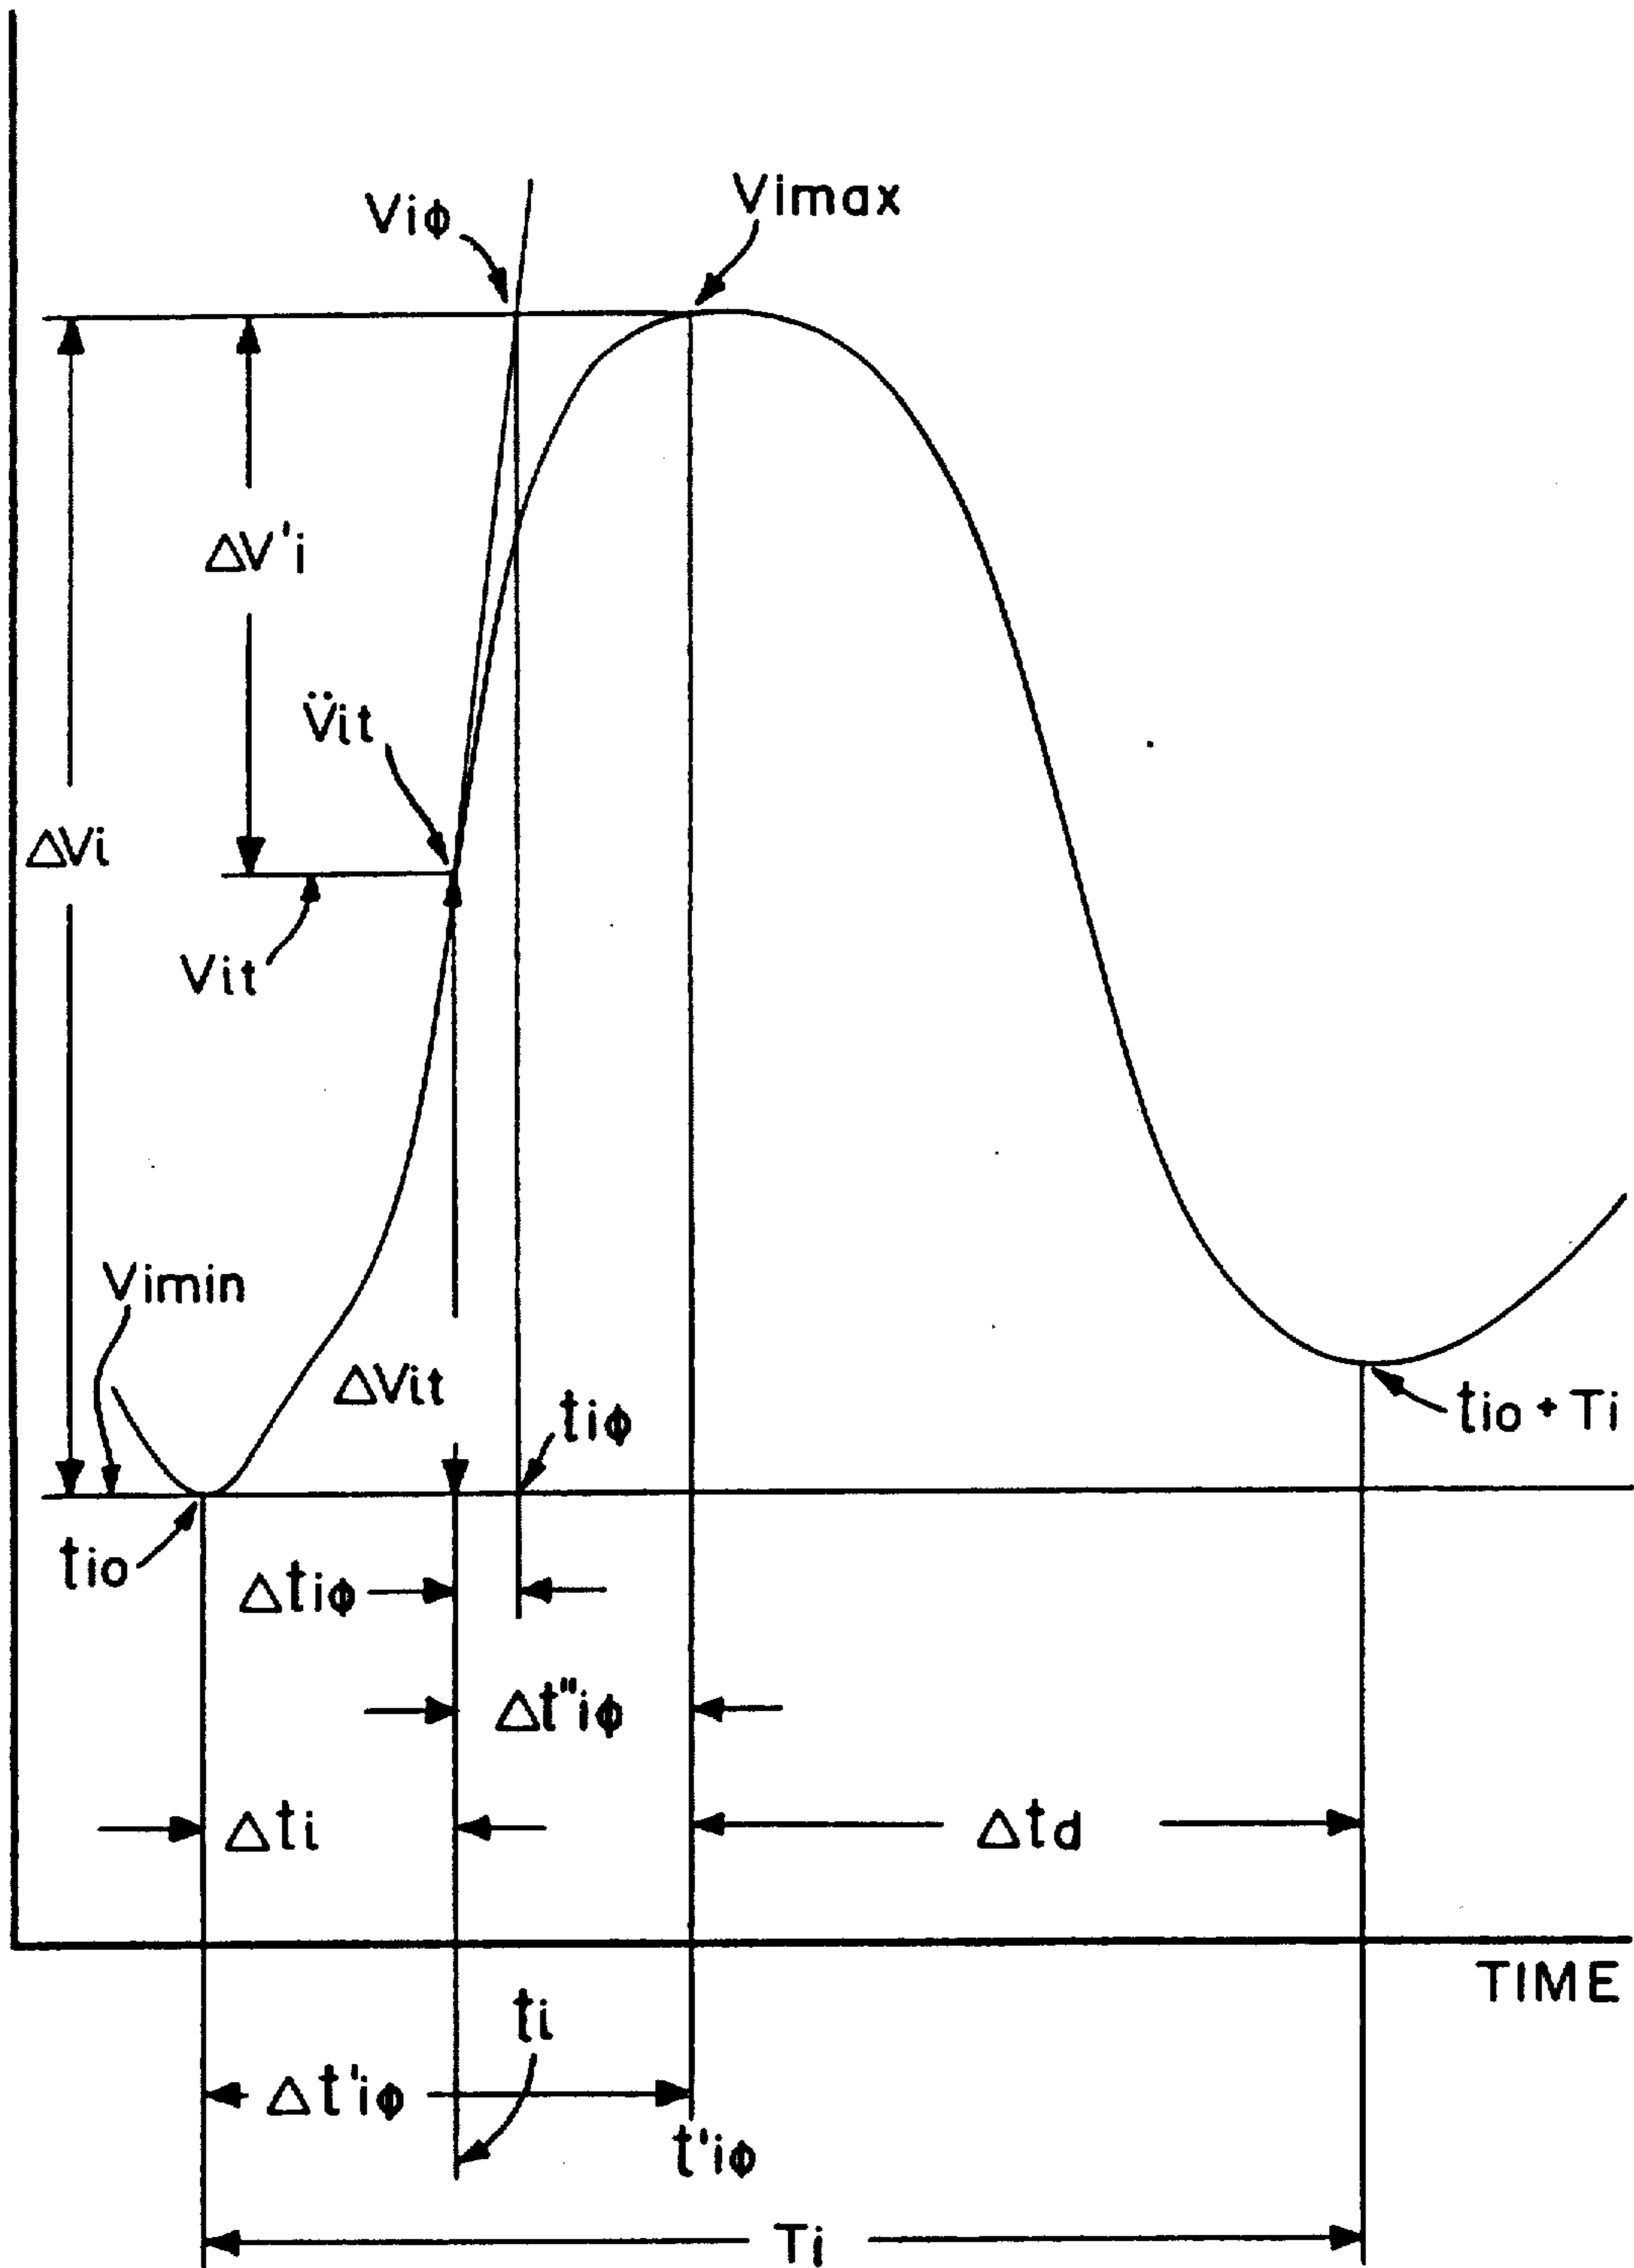


FIG. 4B

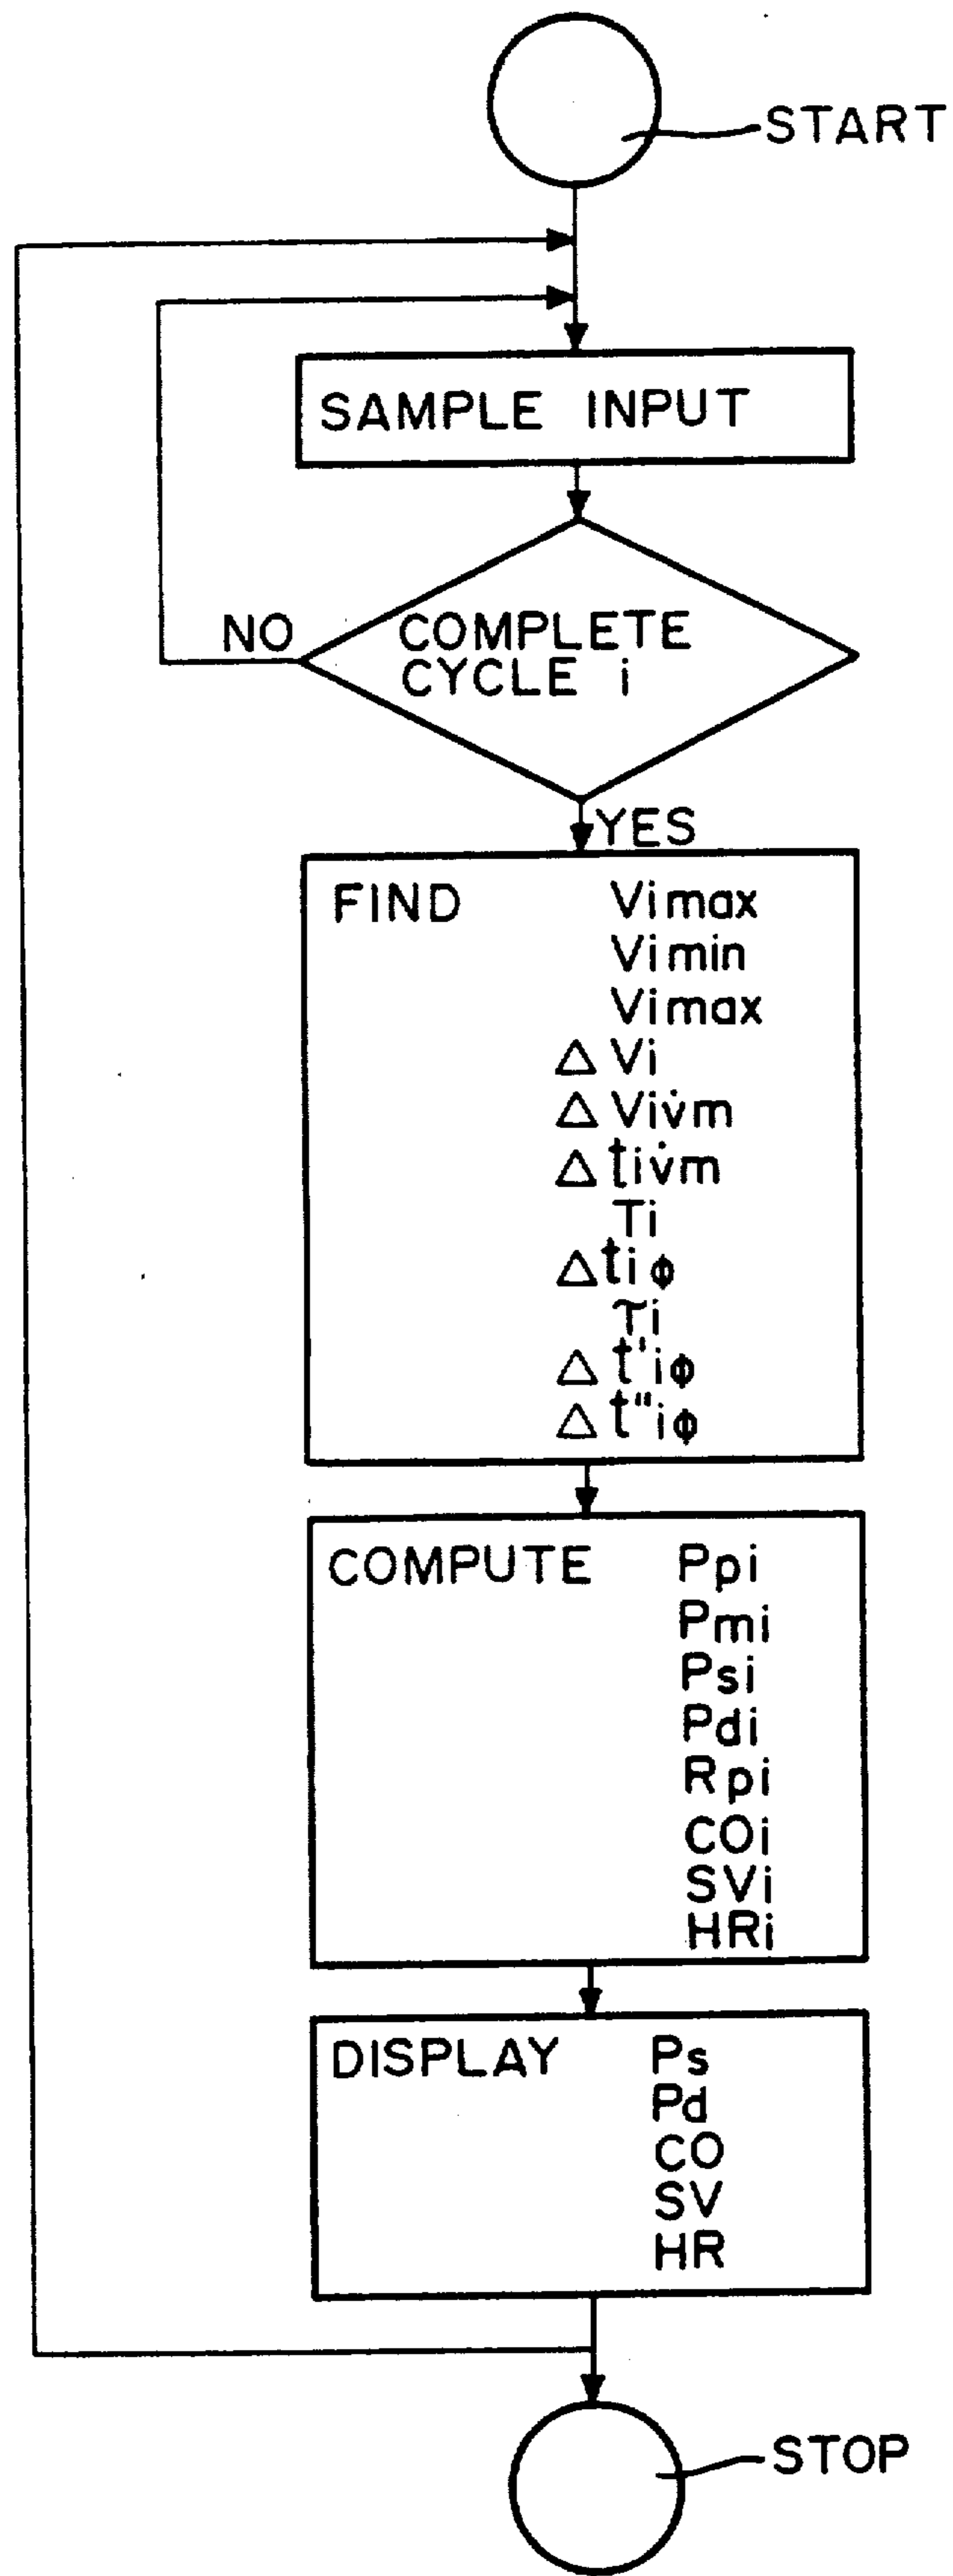


FIG. 6

HEART-RELATED PARAMETERS MONITORING APPARATUS

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue.

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a reissue of application Ser. No. 105,803, filed Oct. 8, 1987, now U.S. Pat. No. 4,834,107, which application is a continuation-in-part application Ser. No. 059,520, filed June 8, now abandoned which is a continuation-in-part application Ser. No. 807,693, filed Dec. 11, 1985, now abandoned which is a continuation-in-part of parent application Ser. No. 608,955, filed May 10, 1984, now all abandoned.

BACKGROUND OF INVENTION

1. Field of the Invention

The invention relates to a non-invasive method of measuring arterial blood pressure and cardiac output. The invention also relates to an apparatus for carrying out the method.

2. Description of Prior Art

Non-invasive methods and apparatus for measuring arterial blood pressure and cardiac output are known in the art. Once such method and apparatus is illustrated in U.S. Pat. No. 4,030,485, Warner, issued June 21, 1977. A second such method and apparatus is taught in U.S. Pat. No. 4,418,700, Warner, issued Dec. 6, 1983. The present invention constitutes an improvement and refinement of the method and apparatus as taught in the latter patent.

SUMMARY OF INVENTION

The invention relates to a non-invasive method, and an apparatus for determining heart-related parameters in patients. The method and apparatus determine pulse pressure, time constant of the arterial system, systolic and diastolic pressure, peripheral resistance, and cardiac output and means arterial blood pressure.

BRIEF DESCRIPTION OF DRAWINGS

The invention will be better understood by an examination of the following description together with the accompanying drawings in which:

FIG. 1 is a block diagram of the apparatus for carrying out the inventive method;

FIG. 2 is a typical sensor output of the system as illustrated in FIG. 1;

FIG. 3 illustrates arterial blood pressure pulses;

FIGS. 4, 4a and 4b illustrate a blood volume pulse;

FIG. 5 illustrates a blood volume pulse and a blood pressure pulse to illustrate the ratio g ; and

FIG. 6 is a simplified flowchart for a computer program for performing calculations in accordance with the invention.

DESCRIPTION OF PREFERRED EMBODIMENTS

As seen in FIG. 1, an apparatus in accordance with the invention comprises a volume sensor such as a photo-electric plethysmograph S, an amplifier A₁, an analog to digital converter A₂, a microcomputer M and a display device D. The plethysmograph sensor S is

attached to, for example, the earlobe of a subject. The sensor could also be attached to other suitable parts of the body such as the forehead, fingertips or toes.

As is known, the plethysmograph, detects changes in blood volume of the region to which it is attached. A typical sensor output signal is shown in FIG. 2. As seen in FIG. 2, the output signal has a pulsating component and a DC component.

The output of the sensor is applied to the plethysmograph amplifier A₁ where it is amplified and filtered and the DC component is discarded. The output of A₁ has a DC component, but this is not directly related to the sensor DC component.

The output of A₁ is fed to the analog to digital (A/D) converter A₂ which digitizes the signal. In a preferred embodiment, the sampling rate is 100 per second.

Microcomputer M accepts signals from A₂ and processes them according to the instructions it contains. These instructions are schematically represented in the simplified flowchart of FIG. 6.

The computer quantities are then displayed on a CRT monitor D or other suitable display means.

THEORY

Arterial blood pressure pulses are shown in FIG. 3. The shape of these curves vary according to the site where they are measured. The highest pressure reached during a cycle i is called the arterial systolic blood pressure, P_{si}. The lowest pressure reached during the same cycle is called the arterial diastolic blood pressure, P_{di}. The pressure rise from P_{di} to P_{si} in the same cycle is the pulse pressure, P_{pi}.

By definition

$$P_{si} - P_{di} = P_{pi} \tag{1}$$

To find P_{pi}

A plethysmographic pulse is shown in FIG. 4. The minimum value at the beginning of the pulse is V_{imin}. The maximum value of the pulse is V_{imax}. As the pulse volume rises from V_{imin} to V_{imax}, the time rate of volume change reaches a maximum \dot{V}_{imax} at time $t_i \dot{V}_m$. The pulse volume at time $t_i \dot{V}_m$ is V_i \dot{V}_m . let

$$\frac{V_{i\dot{V}_m} - V_{imin}}{V_{imax} - V_{imin}} = \frac{\Delta V_{i\dot{V}_m}}{\Delta V_i} = R_i \tag{2}$$

In addition to finding the values of $\dot{V}_{i\dot{V}_m}$ corresponding to \dot{V}_{imax} , see U.S. Pat. No. 4,418,700, Warner, values of V_i \dot{V}_m are also found corresponding to \dot{V}_{imax}^{-1} , \dot{V}_{imax}^{-2} , . . . \dot{V}_{imax}^{-k} , where k is a function of \dot{V}_{imax} .

All of the values of $\dot{V}_{i\dot{V}_m}$ corresponding to the time rates of volume change lying between and including \dot{V}_{imax} and \dot{V}_{imax}^{-k} are averaged and used to compute $\Delta V_{i\dot{V}_m}$.

The average value of V_i \dot{V}_m is

$$\bar{V}_{i\dot{V}_m} = \frac{\sum_1^{n_0} V_{i0m n_0} + \sum_1^{n_1} V_{i1m n_1} + \dots + \sum_1^{n_k} V_{ikm n_k}}{n_0 + n_1 + \dots + n_k}$$

where

n_0 = number of values of V_i \dot{V}_m corresponding to \dot{V}_{imax}

n_l = number of values of V_{iVlm} corresponding to $V_{imax} - 1$
 ... = ...

n_k = number of values of V_{iVkm} corresponding to $V_{imax} - k$
 $k = (V_{imax}/m)$ (integral values only) + 1
 m = constant ... a preferred value of $m = 20$
 l = constant ... a preferred value of $l = 1$

$$P_{pi} = K_{pp} \left(\frac{R_i - r_1}{(1 + r_2 - R_i)^\alpha} \right) \quad (4a)$$

K_{pp} = constant determined by a first calibration
 r_1 = constant ... preferably equal to 0
 r_2 = constant ... preferably equal to 0
 $0 \leq \alpha \leq 1$

R_{i1} can now be defined, as per equation (2) above, but using the average value of V_{iVlm} so that equation (2) can be rewritten

$$\text{let } \frac{\bar{V}_{iVm} - V_{imin}}{V_{imax} - V_{imin}} = \frac{\Delta V_{iVm}}{\Delta V_i} = R_i \quad (2)$$

From FIG. 4

$$\Delta V'_i = \Delta V_i - \Delta V_{iVm}$$

$$\frac{\Delta V'_i}{\Delta V_i} = R' = \frac{\Delta V_i - \Delta V_{iVm}}{\Delta V_i} = 1 - \frac{\Delta V_{iVm}}{\Delta V_i} = 1 - R_i$$

wherein

$$R'_i = 1 - R_i$$

or

$$R_i = 1 - R'_i$$

No other calibration should be required with different subjects. However, if desired, K_{pp} can be determined for each subject.

To find mean blood pressure

The mean blood pressure P_{mi} during a cycle i is given by

$$P_{mmi} = K_4 \left[\frac{\Delta V_i}{\Delta \dot{V}_{imax}} \right]^{-b_3} \quad (5)$$

$$P_{mi} = P_{mmi} + P_0 \quad (6)$$

b_3 = exponent ... the preferred value of b_3 is equal to 0.5

K_4 = constant determined at calibration for each subject. It is only necessary to find this constant once for each subject. The measurements carried out at different times on the same subject do not require separate calibration

P_0 = constant ... preferred 25 mmHg

$$\Delta \dot{V}_{imax} = \text{maximum time rate of change of } \Delta V_i = \dot{V}_{imax}$$

-continued

$$P_{si} = P_{mi} + (1 - g_i)P_{pi} \quad (7)$$

where

$$g_i = (\Delta V_{iAV} / \Delta V_i) \quad (5)$$

ΔV_{iAV} = average value of ΔV_i over the time interval T_i

$$P_{di} = P_{si} - P_{pi} \quad (8)$$

The variable g_i can take on a constant value g_0 whose preferred value is 0.333.

Alternatively, mean blood pressure can be determined using the following expression:

$$P_{mmi} = K_4 \left[\frac{\Delta V_i}{\Delta V_{imax} [G(t)]} \right]^{-b_3} \quad (5')$$

$$= K_4 \left(\frac{1}{r_i} \right)^{-b_3}$$

(for definition of r_i see Equation 10 below);

where

$G(t)$ = a function of t , in a particular case,

$$G(t) = (\phi_c / \phi_i)$$

$$\phi_c = \left[\left(\frac{1}{\Delta t_c} \right) \right]^y$$

$$\phi_i = \left[\left(\frac{1}{\Delta t_i} \right) \right]^y$$

$$\Delta t_c = (\Delta t'_{i\phi_c})$$

$$\Delta t_i = \Delta t'_{i\phi}$$

where

$[T_c = T \text{ at calibration}] \Delta t_c = \Delta t \text{ at calibration } \Delta t'_{i\phi}$ (- see FIG. 4B)

$[t_c = t \text{ at calibration } \Delta t'_{i\phi_c}$ (see FIG. 4B)]

$[\phi_c = (T_c/t_c) = (T/t) \text{ at calibration}] \phi_c = (1/\Delta t)^y \text{ at calibration}$

y = constant

The remainder of the terms in equation 5' are the same as similar terms in equation 5.

Determination of ratio R (FIG. 4b)

From FIG. 4b, the ratio R is

$$R_i = (\Delta V_{ii} / \Delta V_i)$$

where

ΔV_{ii} = change in volume at predetermined time t_i

ΔV_i = total volume change during cycle i

t_i = time such that $\Delta t_i = K_T \Delta t'_{i\phi}$

K_T = constant

Estimation of pulse pressure, PP

$$\frac{1 - e^{K'TkPPI}}{1 - e^{-kPPI}} = R_i$$

where

PP_i = pulse pressure = $p_s - P_d$

P_s = systolic blood pressure

P_d = diastolic blood pressure

k = constant

$K'T$ = constant $\approx K_T$

In FIG. 4B

$$\Delta V'_i = \Delta V_i - \Delta V_{ii}$$

65

$$\Delta V'_i = \Delta V_i - \Delta V_{ii}$$

$$\frac{\Delta V'_i}{\Delta V_i} = \frac{\Delta V_i - \Delta V_{ii}}{\Delta V_i} = 1 - \frac{\Delta V_{ii}}{\Delta V_i} = 1 - R_i = R'_i$$

-continued

$$\left[\frac{\Delta V'_i}{\Delta V_i} = \frac{\Delta V_i - \Delta V_{it}}{\Delta V_i} = 1 - \frac{\Delta V_{it}}{\Delta V_i} = 1 - R_i = R'_i \right]$$

wherein from the above equation:

$$1 - \frac{1 - e^{-KTkPP_i}}{1 - e^{-kPP_i}} = 1 - R_i$$

$$\frac{1 - e^{-kPP_i} - (1 - e^{-KTkPP_i})}{1 - e^{-kPP_i}} = 1 - R_i$$

$$\frac{-e^{-kPP_i} + e^{-KTkPP_i}}{1 - e^{-kPP_i}} = 1 - R_i$$

multiply numerator and denominator by e^{kPP_i}

$$\frac{-1 + e^{kPP_i} e^{-KTkPP_i}}{e^{kPP_i} - 1} = 1 - R_i$$

$$\frac{e^{kPP_i(1-KT)} - 1}{e^{kPP_i} - 1} = 1 - R_i = R'_i$$

Determination of r
From FIG. 4

$$r_i = (\dot{V}_{imax} / \Delta V_i) G(t)$$

where

V_{imax} = maximum time rate of volume increase in cycle i

ΔV_i = total volume increase during cycle i

From FIG. 4b

$$\left[r_i = (\dot{V}_{it} / \Delta V_i) G(t) \right]$$

$$r_i = (V_{it} / V_i) G(t)$$

V_{it} = time rate of increase of volume $V_{i(t)}$ at time t_i

ΔV_i = total volume increase of volume during

ΔV_i = total increase of volume during time interval

$\Delta t_{i\phi}$

Estimation of Mean Blood Pressure

(1) $P_{mi}' = K_1 r_{ic}^a$

K_1 = calibration constant

$P_{mi}' = (P_s + P_d) / 2 - P_o$

P_{si} = systolic blood pressure, in cycle i

$P_{mi} = (P_s + P_d) / 2$

P_{di} = diastolic blood pressure, in cycle i

a = constant

P_o = constant

[(2) $e^{kP_{mi}} = K_2 R_{ic}^b$] (2) $e^{kP_{mi}} = K_2 r_{ic}^b$

where

K_2 = constant (calibration)

b = constant

$$(K_3) \frac{e^{-k(P_{mo} - j\phi_{1i})} - e^{-k(P_{mo} + \phi_{2i})}}{e^{-k(P_{mo} - \phi_{1i})} - e^{-k(P_{mo} + \phi_{2i})}} = r_i$$

where

P_{mo} = constant at calibration

$\phi_{1i} + \phi_{2i} = PP_i$ = pulse pressure during cycle i

k = constant

j = constant

solve equation by making LHS=RHS by varying ϕ_{1i} and ϕ_{2i} ($\phi_{2i} = PP_i - \phi_{1i}$)

then

$P_{si} = P_{mo} + \phi_{2i} + P_o$

5 $P_{di} = P_{mo} - \phi_{1i} + P_o$

$P_{mi} = (P_{si} + P_{di}) / 2$

P_o = constant

r_i = ratio of exponentials

K_3 = coefficient (variable or constant)

10 Correction for r_i

r_i (corrected) = $r_{ic} = r_i e^{m(\phi_o - \phi_i)}$

m = constant

$\phi_o = PP_i$ at calibration

ϕ_i = current value of PP_i .

15 Equation (9) above is only one form which this particular equation can take. By simple mathematical manipulations, the invention may take two other forms as per (10) and (11) below. What follows is the manipulations as well as the two other forms of the equation:

20 As above noted

$$\phi_{2i} + \phi_{1i} = PP_i = P_{si} - P_{di}$$

$$\phi_{2i} + \phi_{1i} = (P_{si} - P_o) - (P_{di} - P_o)$$

25

Let

$P'_{si} = P_{si} - P_o$

30 $P'_{di} = P_{di} - P_o$

30

$\phi_{2i} + \phi_{1i} = P'_{si} - P'_{di}$

add and subtract P_{mo} on RHS above

$$\phi_{2i} + \phi_{1i} = P'_{si} - P_{mo} + P_{mo} - P'_{di} \tag{A}$$

35

ϕ_{2i} and ϕ_{1i} can take on any values in satisfying the above equation (A)

Put $\phi_{2i} = P'_{si} - P_{mo}$

and $\phi_{1i} = P_{mo} - P'_{di}$ in equation (9)

40 then

$$K_3 \left[\frac{e^{-k(P_{mo} - j(P_{mo} - P_{di}))} - e^{-k(P_{mo} + j(P_{si} - P_{di}))}}{e^{-k(P_{mo} - (P_{mo} - P_{di}))} - e^{-k(P_{mo} + (P_{si} - P_{di}))}} \right] = r_i \tag{10}$$

45

simplifying the denominator

$$50 K_3 \left[\frac{e^{-k(P_{mo} - j(P_{mo} - P_{di}))} - e^{-k(P_{mo} + j(P_{si} - P_{di}))}}{e^{-kP_{di}} - e^{-kP_{si}}} \right] = r_i \tag{11}$$

To solve equation 11:

(1) Set $P'_{di} = P'_{si} - PP_i$ and solve for P'_{si}

$P'_{mi} = (P_{si} + P_{di}) / 2 - P_o$

55

(2) Set $P'_{si} = P'_{di} - PP_i$ and solve for P'_{di}

Although particular embodiments have been illustrated, this was for the purpose of describing, but not limiting, the invention. Various modifications, which will come readily to the mind of one skilled in the art, are within the scope of the invention as defined in the appended claims.

$$P_{mi} = (P_{si} + P_{di}) / 2$$

I claim:

65 1. Apparatus for determining the magnitude of heart-related parameters in a patient; comprising;

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein means for calculating calculates the magnitude of the pulse pressure parameter in accordance with the following expression;

$$P_{pi} = K_{pp} \left[\frac{R_{il} - r_1}{(1 + r_2 - R_{il})} \right]$$

wherein

P_{pi} = pulse pressure during cycle i

K_{pp} = constant determined by a first calibration

r_1 = constant

r_2 = constant

$R_{il} = (\Delta \dot{V}_i V_m / \Delta V_i)$

where $\Delta V_i V_m$ = volume change at time $t_i V_m$ during cycle i corresponding to maximum rate of volume change, V_{imax}

ΔV_i = maximum volume change during cycle i

$\Delta t_i V_m$ = time interval from start of cycle i to time of maximum rate of volume change V_{imax} .

2. Apparatus for determining the magnitude of heart-related parameters in a patient;

comprising;

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood

volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum [amplitude,] *amplitude*, said maximum rate of change of said signal, said first difference, said second [different,] *difference*, said first time interval, and said second time interval; and

means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein means for calculating [calculates] *calculates* the magnitude of the mean arterial blood pressure, P_{mi} parameter in accordance with the following expression:

$$P_{mi} = P_o + P_{mmi}$$

$$P_{mmi} = \left[K_4 \frac{\Delta V_i}{\Delta V_{imax} [G(t)]} \right]^{-b_3}$$

$$[P_{mmi} = K_4 \left[\frac{\Delta V_i}{\Delta V_{imax} [G(t)]} \right]^{-b_3}]$$

where

K_4 = constant determined for each subject

b_3 = constant

P_{mmi} = pseudo mean arterial blood pressure during cycle i

$[\Delta_i] \Delta V_i$ = maximum volume change during cycle i

$\Delta \dot{V}_{imax}$ = maximum time rate of change of ΔV_i
 = \dot{V}_{imax}

where

$$G(t) = \frac{\phi_c}{\phi_l}$$

5

10

15

20

25

30

35

40

45

50

55

60

65

-continued

$$\phi_c = \left[\frac{1}{\Delta t_c} \right]^y$$

$$\phi_l = \left[\frac{1}{\Delta t_l} \right]^y$$

where

$$\Delta t_c = \Delta t \text{ at calibration} = \Delta t_{i\phi c}$$

$$\Delta t_l = \Delta t_{i\phi}$$

$$y = \text{constant.}$$

3. Apparatus for determining the magnitude of heart-related parameters in a patient;

comprising;

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum [amplitude,] *amplitude*, said maximum rate of change of said signal, said first difference, said second [different,] *difference*, said first time interval, and said second time interval; and means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein means for calculating calculates the magnitude of the systolic pressure (P_{si}) parameter in accordance with the following expression:

$$P_{si} = P_{mi} + (1 - g_0)P_{pi}$$

wherein

$$g_0 = \text{constant.}$$

4. Apparatus for determining the magnitude of heart-related parameters in a patient;

comprising:

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum [amplitude,] *amplitude*, said maximum rate of change of said signal, said first difference, said second [different,] *difference*, said first time interval, and said second time interval; and

means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein means for calculating calculates the magnitude of the systolic pressure (P_{si}) parameter in accordance with the following expression:

$$P_{si} = P_{mi} + (1 - g_i)P_{pi}$$

wherein:

$$g_i = (\Delta V_{iAV} / \Delta V_i)$$

P_{pi} = pulse pressure during cycle i

ΔV_i = represented by said first difference

ΔV_{iAV} = represented by the difference between said minimum amplitude and an amplitude equal to the average value of a pulse in a cycle i .

5. Apparatus for determining the magnitude of heart-related parameters in a patient;

comprising;

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood volume variation being [cycle] cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum [amplitude,] amplitude, said maximum rate of change of said signal, said first difference, said second [different,] difference, said first time interval, and said second time interval; and means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein means for calculating calculates the magnitude of the arterial blood pressure, P_{mi} parameter in accordance with the following expression:

$$P_{mi} = P_o + P_{mmi}$$

$$P_{mmi} = \left[K_4 \frac{\Delta V_i}{\Delta V_{imax}[G(t)]} \right]^{-b_3}$$

$$[P_{mmi} = K_4 \left[\frac{\Delta V_i}{\Delta V_{imax}[G(t)]} \right]^{-b_3}]$$

where

- K_4 =constant determined for each subject
- b_3 =constant
- P_{mmi} =pseudo mean arterial blood pressure during cycle i
- ΔV_i =maximum volume change during cycle i

$$\hat{V}_{imax} = \text{maximum time rate of change of } V_i$$

$$= \dot{V}_{imax}$$

P_o =constant

where

$G(t)$ =a function of t.

6. A method for determining the magnitude of heart-related parameters in a patient;

comprising:

detecting blood volume, and thereby blood volume variation, in said patient and providing a signal representative of said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said maximum amplitude and said minimum amplitude, a maximum rate of change of said signal being representative of the maximum rate of change of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum change of rate of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and calculating the magnitude of the pulse pressure parameter in accordance with the following expression:

$$P_{pi} = K_{pp} \left[\frac{R_{i1} - r_1}{(1 + r_2 - R_{i1})} \right]$$

wherein

- P_{pi} =pulse pressure during cycle i
- K_{pp} =constant determined by a first calibration
- r_1 =constant
- r_2 =constant
- $R_{i1}=(\Delta V_i \hat{V}_m / \Delta V_i)$

where

$[\Delta V_i \hat{V}_m$ =volume change at time $t_i \hat{V}_m$ during cycle i corresponding to maximum rate of volume change, V_{imax}]

$\Delta V_i \hat{V}_m$ =volume change at time $t_i \hat{V}_m$ during cycle i corresponding to maximum rate of volume change, V_{imax}

ΔV_i =maximum volume change during cycle i
 $\Delta t_i \hat{V}_m$ =time interval from start of cycle i to time of maximum rate of volume change V_{imax} .

7. A method for determining the magnitude of heart-related parameters in a patient;

comprising:

detecting blood volume, and thereby blood volume variation, in said patient and providing a signal representative of said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said maximum amplitude and said mini-

mum amplitude, a maximum rate of change of
 said signal being representative of the maximum
 rate of change of blood volume, a second time
 interval between the minimum amplitude and the
 time of the maximum rate of change of said sig- 5
 nal, a first difference in amplitude between said
 maximum amplitude and said minimum ampli-
 tude, a second difference in amplitude between
 the maximum amplitude and the amplitude at the
 time of maximum change of rate of said signal 10
 being representative of the difference in volume
 between the maximum amount of blood volume
 and the volume at the time of maximum rate of
 change of said blood volume, and a pulse repeti-
 tion period;
 measuring said maximum amplitude, said minimum
 amplitude, said maximum rate of change of said
 signal, said first difference, said second differ-
 ence, said first time interval, and said second
 time interval; and
 calculating the magnitude of the mean [artial]
 arterial pressure P_{mi} in accordance with the fol-
 lowing expression:

$$P_{mi} = P_o + P_{mmi}$$

$$P_{mmi} = \left[K_4 \frac{\Delta V_i}{\dot{\Delta V}_{imax}[G(t)]} \right]^{-b_3}$$

$$[P_{mmi} = K_4 \left[\frac{\Delta V_i}{\dot{\Delta V}_{imax}[G(t)]} \right]^{-b_3}]$$

where
 K_4 = constant determined for each subject
 b_3 = constant
 P_{mmi} = pseudo mean arterial blood pressure dur-
 ing cycle i
 ΔV_i = maximum volume change during cycle i
 $\dot{\Delta V}_{imax}$ = maximum time rate of change of
 $\Delta V_i = \dot{\Delta V}_{imax}$

$$G(t) = \frac{\phi_c}{\phi_i}$$

$$\phi_c = \left[\frac{1}{\Delta t_c} \right]^y$$

$$\phi_i = \left[\frac{1}{\Delta t_i} \right]^y$$

where

$$\Delta t_c = \Delta t \text{ at calibration} = \Delta t_{i\phi_c}$$

$$\Delta t_i = \Delta t_{i\phi}$$

y = constant.

8. A method for determining the magnitude of heart-
 related parameters in a patient;

comprising:

detecting blood volume, and thereby blood volume
 variation, in said patient and providing a signal
 representative of said blood volume, and thereby
 said blood volume variation;

said blood volume variation being cyclic in nature
 whereby said signal comprises a cyclic curve
 having, in each cycle of variation, a variable

slope, a maximum amplitude representative of
 the maximum amount of blood volume, a mini-
 mum amplitude representative of the minimum
 amount of blood volume, a first time interval
 between said maximum amplitude and said mini-
 mum amplitude, a maximum rate of change of
 said signal being representative of the maximum
 rate of change of blood volume, a second time
 interval between the minimum amplitude and the
 time of the maximum rate of change of said sig-
 nal, a first difference in amplitude between said
 maximum amplitude and said minimum ampli-
 tude, a second difference in amplitude between
 the maximum amplitude and the amplitude at the
 time of maximum change of rate of said signal
 being representative of the difference in volume
 between the maximum amount of blood volume
 and the volume at the time of maximum rate of
 change of said blood volume, and a pulse repeti-
 tion period;
 measuring said maximum amplitude, said minimum
 amplitude, said maximum rate of change of said
 signal, said first difference, said second differ-
 ence, said first time interval, and said second
 time interval; and
 calculating the magnitude of the systolic pressure
 (P_{si} parameter in accordance with the following
 expression:

$$P_{si} = P_{mi} + (1 - g_0)P_{pi}$$

wherein

g_0 = constant.

9. A method for determining the magnitude of heart-
 related parameters in a patient;

comprising:

detecting blood volume, and thereby blood volume
 variation, in said patient and providing a signal
 representative of said blood volume, and thereby
 said blood volume variation;

said blood volume variation being cyclic in nature
 whereby said signal comprises a cyclic curve
 having, in each cycle of variation, a variable
 slope, a maximum amplitude representative of
 the maximum amount of blood volume, a mini-
 mum amplitude representative of the minimum
 amount of blood volume, a first time interval
 between said maximum amplitude and said mini-
 mum amplitude, a maximum rate of change of
 said signal being representative of the maximum
 rate of change of blood volume, a second time
 interval between the minimum amplitude and the
 time of the maximum rate of change of said sig-
 nal, a first difference in amplitude between said
 maximum amplitude and said minimum ampli-
 tude, a second difference in amplitude between
 the maximum amplitude and the amplitude at the
 time of maximum change of rate of said signal
 being representative of the difference in volume
 between the maximum amount of blood volume
 and the volume at the time of maximum rate of
 change of said blood volume, and a pulse repeti-
 tion period;

measuring said maximum amplitude, said minimum
 amplitude, said maximum rate of change of said
 signal, said first difference, said second differ-

ence, said first time interval, and said second time interval; and calculating the magnitude of the systolic pressure (P_{si}) parameter in accordance with the following expression:

$$P_{si} = P_{mi} + (1 - g_i)P_{pi}$$

wherein:

$$g_i = (\Delta V_{iAV} / \Delta V_i)$$

P_{pi} = pulse pressure during cycle i

ΔV_i = represented by said first difference

ΔV_{iAV} = represented by the difference between said minimum amplitude and an amplitude equal to the average value of a pulse in a cycle i .

10. A method for determining the magnitude of heart-related parameters in a patient; comprising:

detecting blood volume, and thereby blood volume variation, in said patient and providing a signal representative of said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said maximum amplitude and said minimum amplitude, a maximum rate of change of said signal being representative of the maximum rate of change of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum change of rate of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

calculating the magnitude of the arterial blood pressure, P_{mi} parameter in accordance with the following expression:

$$P_{mi} = P_o + P_{mmi}$$

$$P_{mmi} = \left[K_4 \frac{\Delta V_i}{\Delta V_{imax} [G(t)]} \right]^{-b_3}$$

$$K_{P_{mmi}} = K_4 \left[\frac{\Delta V_i}{\Delta V_{imax} [G(t)]} \right]^{-b_3}$$

where

K_4 = constant determined for each subject

b_3 = constant

P_{mmi} = pseudo mean arterial blood pressure during cycle i

ΔV_i = maximum volume change during cycle i

$\Delta \dot{V}_{imax}$ = maximum time rate of change of V_i = $\frac{V_{imax}}{V_{imax}}$

P_o = constant

$G(t)$ = a function of t and T .

11. Apparatus for determining the magnitude of heart-related parameters in a patient; comprising:

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum [amplitude,] amplitude, said maximum rate of change of said signal, said first difference, said second [different,] difference, said first time interval, and said second time interval; and

means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein means for calculating calculates the magnitude of the pulse pressure parameter in accordance with the following expression:

$$P_{pi} = K_{pp} \left[\frac{R_{i1} - r_1}{(1 + r_2 - R_{i1})} \right]$$

wherein

P_{pi} = pulse pressure during cycle i

K_{pp} = constant determined by a first calibration

r_1 = constant

r_2 = constant

$R_{i1} = \Delta V_i \dot{V}_m / \Delta V_i$

where

ΔV_{iV_m} = volume change at preselected time t_{iV_m} during cycle i

ΔV_i = maximum volume change during cycle i

Δt_{iV_m} = time interval from start of cycle i to preselected time of t_{iV_m} .

12. A method for determining the magnitude of heart-related parameters in a patient; comprising:

detecting blood volume, and thereby blood volume variation, in said patient and providing a signal representative of said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said maximum amplitude and said minimum amplitude, a maximum rate of change of said signal being representative of the maximum rate of change of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum change of rate of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

calculating the magnitude of the pulse pressure parameter in accordance with the following expression:

$$P_{pi} = K_{pp} \left[\frac{R_{i1} - r_1}{(1 + r_2 - R_{i1})} \right]$$

wherein

P_{pi} = pulse pressure during cycle i

K_{pp} = constant determined by a first calibration

r_1 = constant

r_2 = constant

$R_{i1} = (\Delta V_{iV_m} / V_i)$

where

ΔV_{iV_m} = volume change at preselected time t_{iV_m} during cycle i

ΔV_i = maximum volume change during cycle i

Δt_{iV_m} = time interval from start of cycle i to predetermined time of t_{iV_m} .

13. Apparatus for determining the magnitude of heart-related parameters in a patient; comprising;

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood

volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein the means for calculating calculates the magnitude of the mean pressure parameter in accordance with the following expression:

$$(1) P'_{mi} = K_1 r_{ic}^a$$

where

K_1 = calibration constant

$[P'_{mi} = (P_s + P_d)/2 - P_o]$

P_{si} = systolic blood pressure, in cycle i

$[P_{mi} = (P_s + P_d)/2]$

P_{di} = diastolic blood pressure, in cycle i

a = constant

P_o = constant.

14. A method for determining the magnitude of heart-related parameters in a patient; comprising:

detecting blood volume, and thereby blood volume variation, in said patient and providing a signal [representation] representative of said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said maximum amplitude and said minimum amplitude, a maximum rate of change of said signal being representative of the maximum rate of change of blood volume, a second time

interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum change of rate of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

calculating the magnitude of mean pulse pressure in accordance with the following expression:

$$[(1) P_{mi} = K_1 r_i^a]$$

$$(1) P_{mi} = K_1 r_i^a$$

where

K_1 = calibration constant

$$[P'_{mi} = (P_s + P_d)/2 - P_o]$$

$$P_{mi} = (P_{si} + P_{di})/2 - P_o$$

P_{si} = systolic blood pressure, in cycle i

$$[P_{mi} = (P_s + P_d)/2]$$

$$P_{mi} = (P_{si} + P_{di})/2$$

P_{di} = diastolic blood pressure, in cycle i

a = constant

P_o = constant.

15. Apparatus for determining the magnitude of heart-related parameters in a patient; comprising;

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said

second [different,] difference, said first time interval, and said second time interval; and means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring; wherein the means for calculating calculates implicitly the magnitude of the mean pulse pressure in accordance with the following expression:

$$(K_3) \frac{e^{-k(P_{mo} - j\phi_{1i})} - e^{-k(P_{mo} + \phi_{2i})}}{e^{-k(P_{mo} - \phi_{1i})} - e^{-k(P_{mo} + \phi_{2i})}} = r_i \quad (3)$$

$$[K_3] \frac{-k(P_{mo} - j\phi_{1i}) - e^{-k(P_{mo} + \phi_{2i})}}{e^{-k(P_{mo} - \phi_{1i})} - e^{-k(P_{mo} + \phi_{2i})}} = r_i]$$

where

P_{mo} = constant at calibration

$\phi_{1i} + \phi_{2i} = PP_i$ = pulse pressure during cycle i

k = constant

j = constant

$$P_{si} = P_{mo} + \phi_{2i} + P_o$$

$$P_{di} = P_{mo} - \phi_{1i} + P_o$$

$$P_{mi} = (P_{si} + P_{di})/2$$

P_o = constant

r_i = ratio of exponentials

K_3 = coefficient (variable or constant).

16. A method for determining the magnitude of heart-related parameters in a patient; comprising:

detecting blood volume, and thereby blood volume variation, in said patient and providing a signal representative of said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said maximum amplitude and the said minimum amplitude, a maximum rate of change of said signal being representative of the maximum rate of change of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum change of rate of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

wherein the means for calculating calculates implicitly the magnitude of mean pulse pressure in accordance with the following [expression] expression:

$$(K_3) \frac{e^{-k(P_{mo}-j\phi_{1i})} - e^{-k(P_{mo}+\phi_{2i})}}{e^{-k(P_{mo}-\phi_{1i})} - e^{-k(P_{mo}+\phi_{2i})}} = r_i \quad (3)$$

$$\left[K_3 \frac{e^{-k(P_{mo}-j\phi_{1i})} - e^{-k(P_{mo}+\phi_{2i})}}{e^{-k(P_{mo}-\phi_{1i})} - e^{-k(P_{mo}+\phi_{2i})}} = r_i \right]$$

where

P_{mo} = constant at calibration

$\phi_{1i} + \phi_{2i} = PP_i$ = pulse pressure during cycle i

k = constant

j = constant

$[P_{2i} = P_{mo} + \phi_{2i} + P_o]$

$P_{si} = P_{mo} + \phi_{2i} + P_o$

$P_{di} = P_{mo} - \phi_{1i} + P_o$

$P_{mi} = (P_{si} + P_{di})/2$

P_o = constant

r_i = ratio of exponentials

K_3 = coefficient (variable or constant).

17. Apparatus for determining the magnitude of heart-related parameters in a patient;

comprising:

means for detecting blood volume, and thereby blood volume variation, in said patient, and for providing a signal representative of said blood volume, and thereby said blood volume variation;

said means for detecting being attachable to said patient to thereby detect said blood volume, and thereby said blood volume variation;

said blood variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said minimum amplitude and said maximum amplitude, a maximum rate of change of said signal being representative of the maximum rate of increase of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum rate of change of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

means for measuring said maximum amplitude; said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

means for calculating the magnitude of selected ones of said parameters, said means for calculating being connected to both said means for detecting and means for measuring;

wherein means for calculating calculates the magnitude of the pulse pressure parameter in accordance with the following expression;

$$\frac{1 - e^{-KT'PP_i}}{1 - e^{kPP_i}} = R_i$$

where

PP_i = Pulse Pressure = $P_s - P_d$

P_s = Systolic blood pressure

P_d = diastolic blood pressure

k = constant

K' = constant.

18. A method for determining the magnitude of heart-related parameters in a patient;

comprising:

detecting blood volume, and thereby blood volume variation, in said patient and providing a signal representative of said blood volume, and thereby said blood volume variation;

said blood volume variation being cyclic in nature whereby said signal comprises a cyclic curve having, in each cycle of variation, a variable slope, a maximum amplitude representative of the maximum amount of blood volume, a minimum amplitude representative of the minimum amount of blood volume, a first time interval between said maximum amplitude and said minimum amplitude, a maximum rate of change of said signal being representative of the maximum rate of change of blood volume, a second time interval between the minimum amplitude and the time of the maximum rate of change of said signal, a first difference in amplitude between said maximum amplitude and said minimum amplitude, a second difference in amplitude between the maximum amplitude and the amplitude at the time of maximum change of rate of said signal being representative of the difference in volume between the maximum amount of blood volume and the volume at the time of maximum rate of change of said blood volume, and a pulse repetition period;

measuring said maximum amplitude, said minimum amplitude, said maximum rate of change of said signal, said first difference, said second difference, said first time interval, and said second time interval; and

calculating the magnitude of the mean arterial pressure P_{mi} in accordance with the following expression:

$$\frac{1 - e^{-KT'PP_i}}{1 - e^{kPP_i}} = R_i$$

where

PP_i = Pulse Pressure = $P_s - P_d$

P_s = Systolic blood pressure

P_d = Diastolic blood pressure

k = constant

K' = constant.

* * * * *