



US00RE39772E

(19) **United States**
(12) **Reissued Patent**
Herron et al.

(10) **Patent Number: US RE39,772 E**
(45) **Date of Reissued Patent: Aug. 14, 2007**

- (54) **LENS AND ASSOCIATABLE FLOW CELL**
- (75) Inventors: **James N. Herron**, Salt Lake City, UT (US); **Douglas A. Christensen**, Salt Lake City, UT (US); **Victor A. Pollack**, Salt Lake City, UT (US); **Richard D. McEachern**, Ann Arbor, MI (US); **Eric M. Simon**, Salt Lake City, UT (US)
- (73) Assignee: **University of Utah Research Foundation**, Salt Lake City, UT (US)
- (21) Appl. No.: **10/225,687**
- (22) PCT Filed: **Mar. 19, 1997**
- (86) PCT No.: **PCT/US97/04398**
§ 371 (c)(1),
(2), (4) Date: **Sep. 18, 1997**
- (87) PCT Pub. No.: **WO97/35176**
PCT Pub. Date: **Sep. 25, 1997**

Related U.S. Patent Documents

Reissue of:

- (64) Patent No.: **6,108,463**
- Issued: **Aug. 22, 2000**
- Appl. No.: **09/142,948**
- Filed: **Sep. 18, 1998**

U.S. Applications:

- (60) Provisional application No. 60/022,434, filed on Aug. 8, 1996, and provisional application No. 60/013,695, filed on Mar. 19, 1996.
- (51) **Int. Cl.**
G02B 6/26 (2006.01)
G02B 6/10 (2006.01)
G01N 21/00 (2006.01)
G01N 33/552 (2006.01)
G01N 33/72 (2006.01)
- (52) **U.S. Cl.** **385/12; 385/15; 385/33; 385/37; 385/130; 385/146; 422/82.11**
- (58) **Field of Classification Search** **385/12, 385/15, 33, 37, 129, 130, 141, 146; 422/82.4, 422/82.05; 436/63**

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,490,847 A * 1/1970 Beale et al. 356/326

(Continued)

FOREIGN PATENT DOCUMENTS

DE 4412893 A1 10/1995 385/12 X

(Continued)

OTHER PUBLICATIONS

Supplementary Partial European Search Report, EP 97 91 6086, dated Oct. 26, 1999.


(Continued)

Primary Examiner—Brian M. Healy
(74) *Attorney, Agent, or Firm*—TraskBritt

(57) **ABSTRACT**

Improvements in a biosensor of the type having reservoirs or wells for analyzing a biological liquid are disclosed. A biosensor (190) includes a waveguide (164) placed between a plurality of members such as plates (100, 186), at least one of the members (100) being formed to define the walls (132, 134, 136) of the reservoirs where the liquid is biologically analyzed. The walls of the reservoirs are made of an inert, opaque material such as a metal. Although the biosensor may include a gasket (162), the gasket is associated with the members and waveguide in such a way (e.g. by recessing the gasket into a channel formed into a metal plate) so that the gasket does not form any significant portion of the reservoir wall. Waveguides of varying composition (e.g. plastic, quartz or glass) may be associated with the members to form the biosensor. The metal plate of the biosensor has input and output ports for infusing, draining, or oscillating the liquid to be analyzed in the reaction reservoir. Also disclosed is a sled-shaped waveguide associated with a rear lens to couple light out of the waveguide to serve as a quality control measure thus insuring that the biosensor is properly placed and that the light is working.

18 Claims, 13 Drawing Sheets

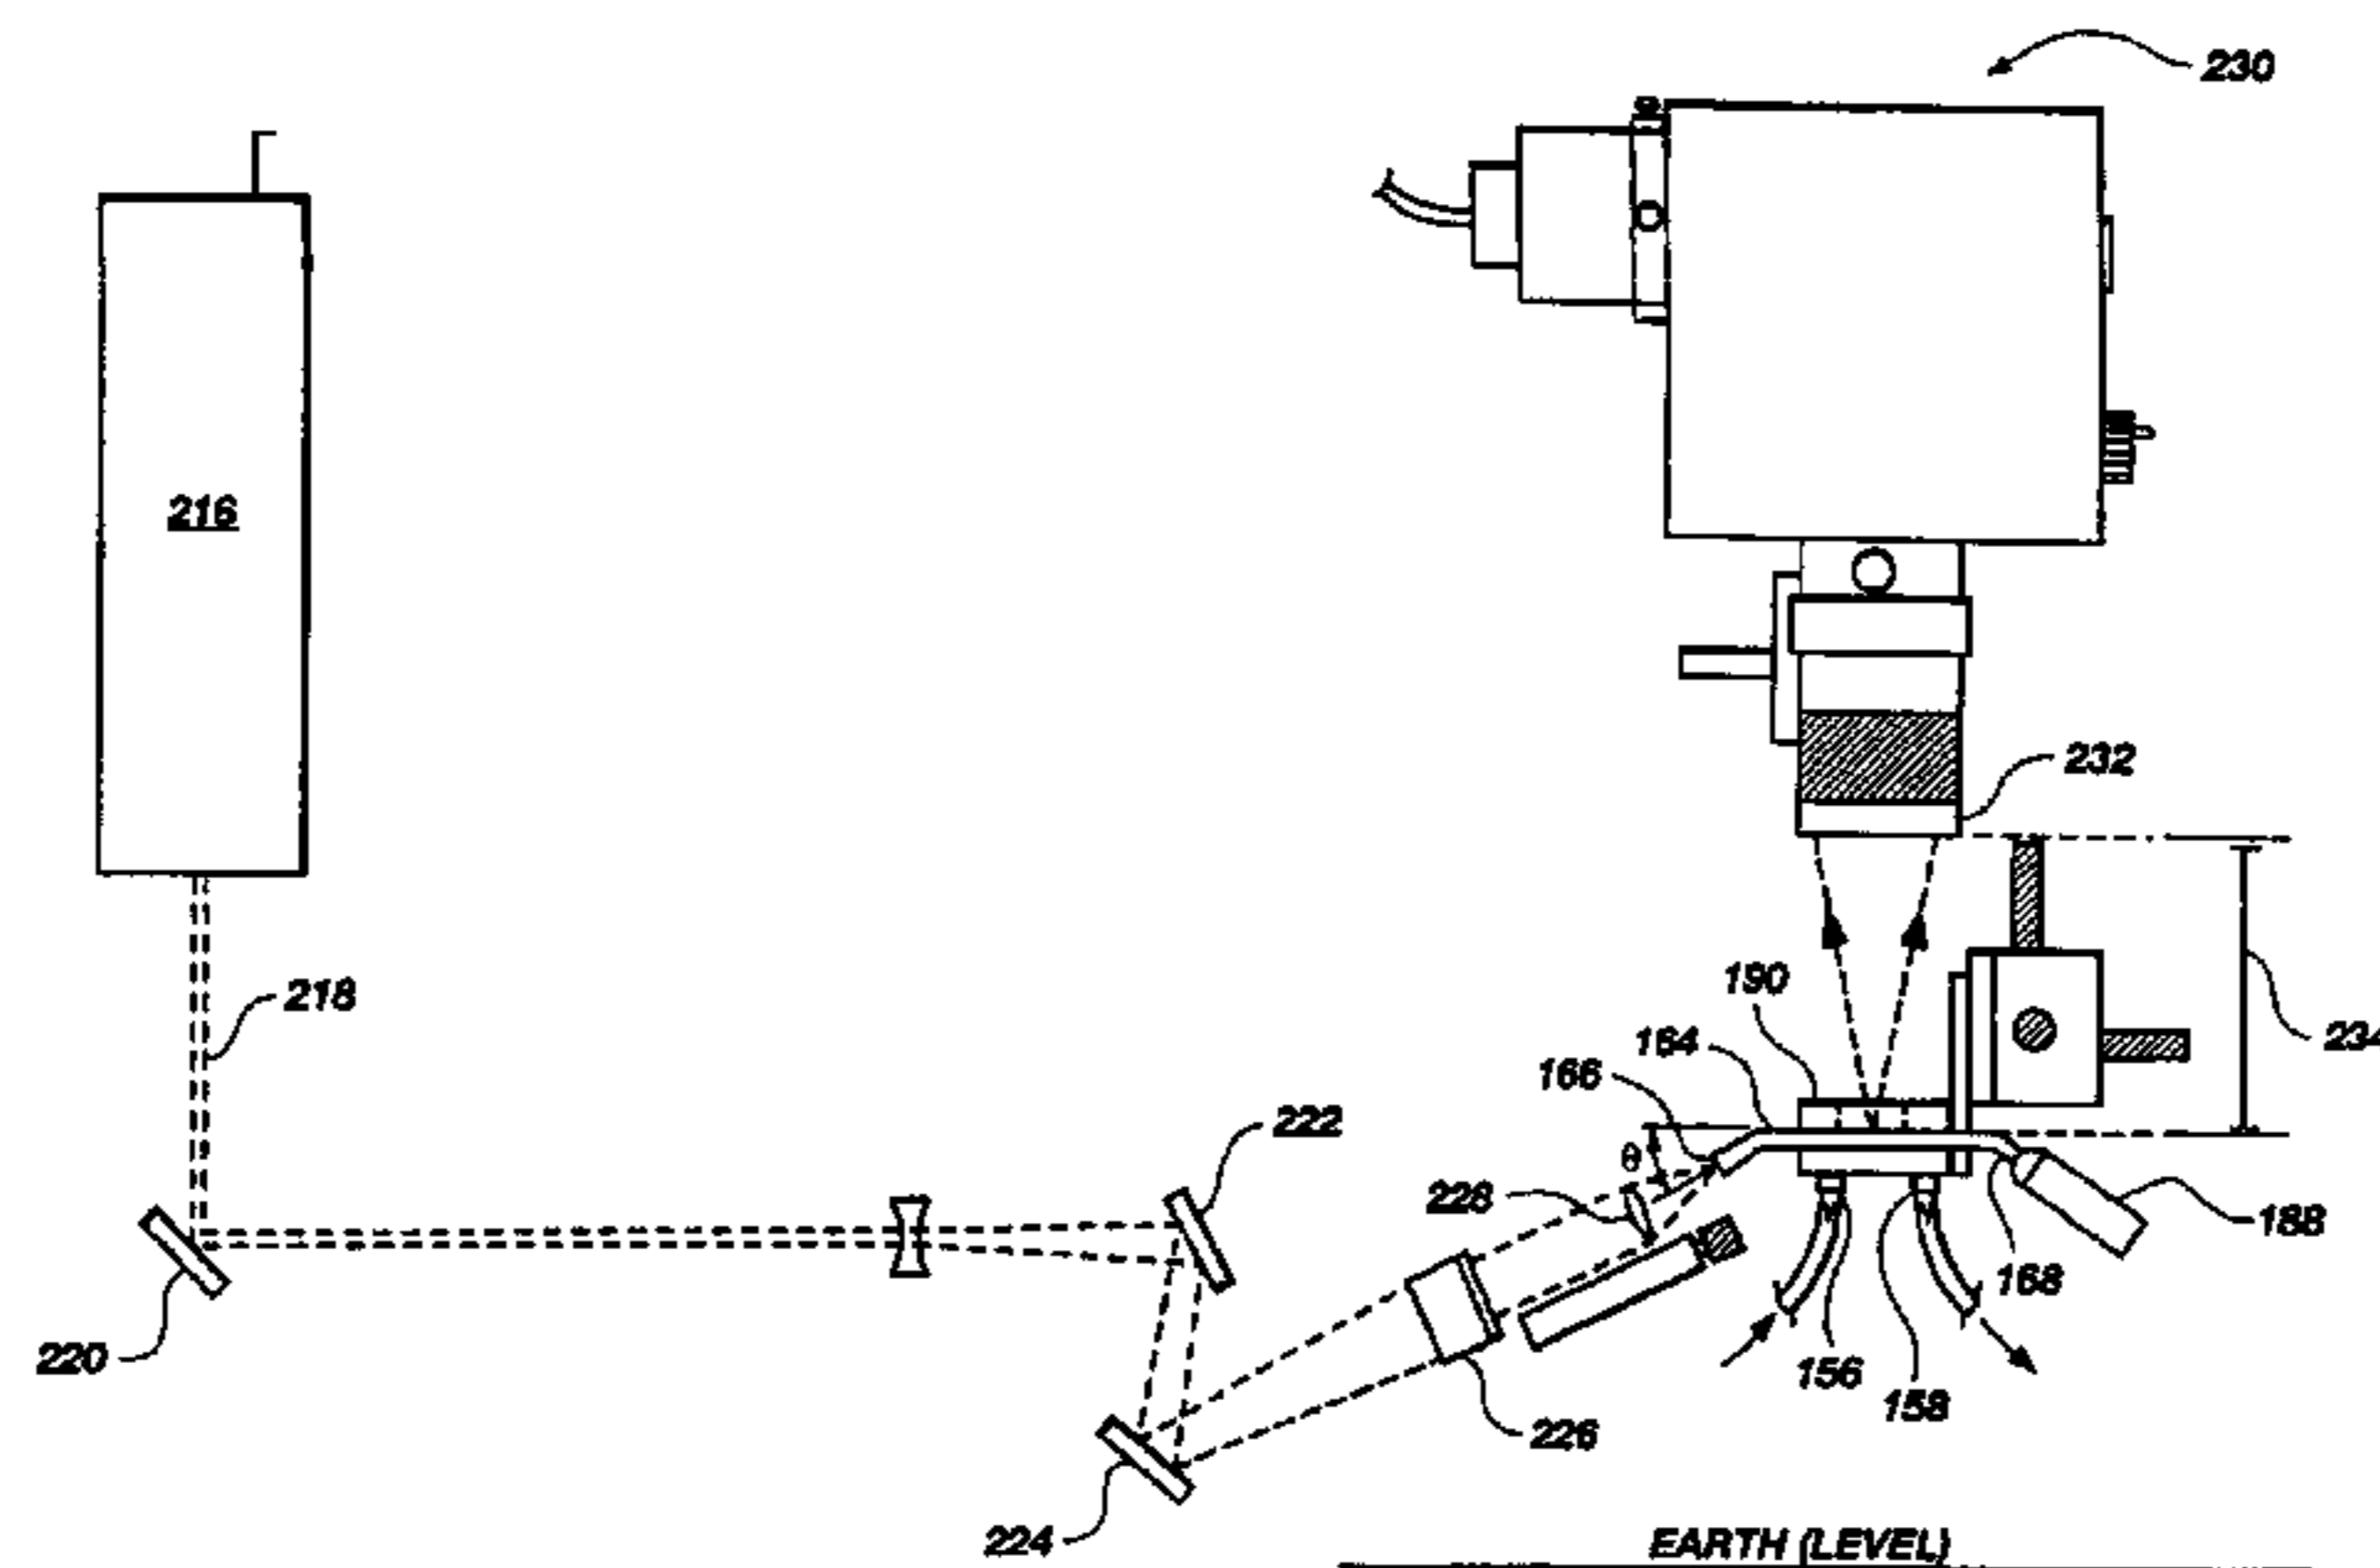

US RE39,772 E

Page 2

U.S. PATENT DOCUMENTS

4,746,179 A * 5/1988 Dahne et al. 385/12
4,818,710 A * 4/1989 Sutherland et al. 436/527
4,857,273 A * 8/1989 Stewart 422/82.11
4,980,278 A * 12/1990 Yamada et al. 435/7.92
5,064,619 A * 11/1991 Finlan 422/82.05
5,202,950 A * 4/1993 Arego et al. 385/146
5,485,277 A 1/1996 Foster 356/445
5,512,492 A * 4/1996 Herron et al. 436/518

FOREIGN PATENT DOCUMENTS

EP 0185126 6/1986 385/12 X
EP 94/27137 11/1994 385/12 X
EP 95/03538 2/1995 385/12 X

OTHER PUBLICATIONS

Supplementary European Search Report, EP 97 91 6086,
dated Jan. 31, 2000.

* cited by examiner

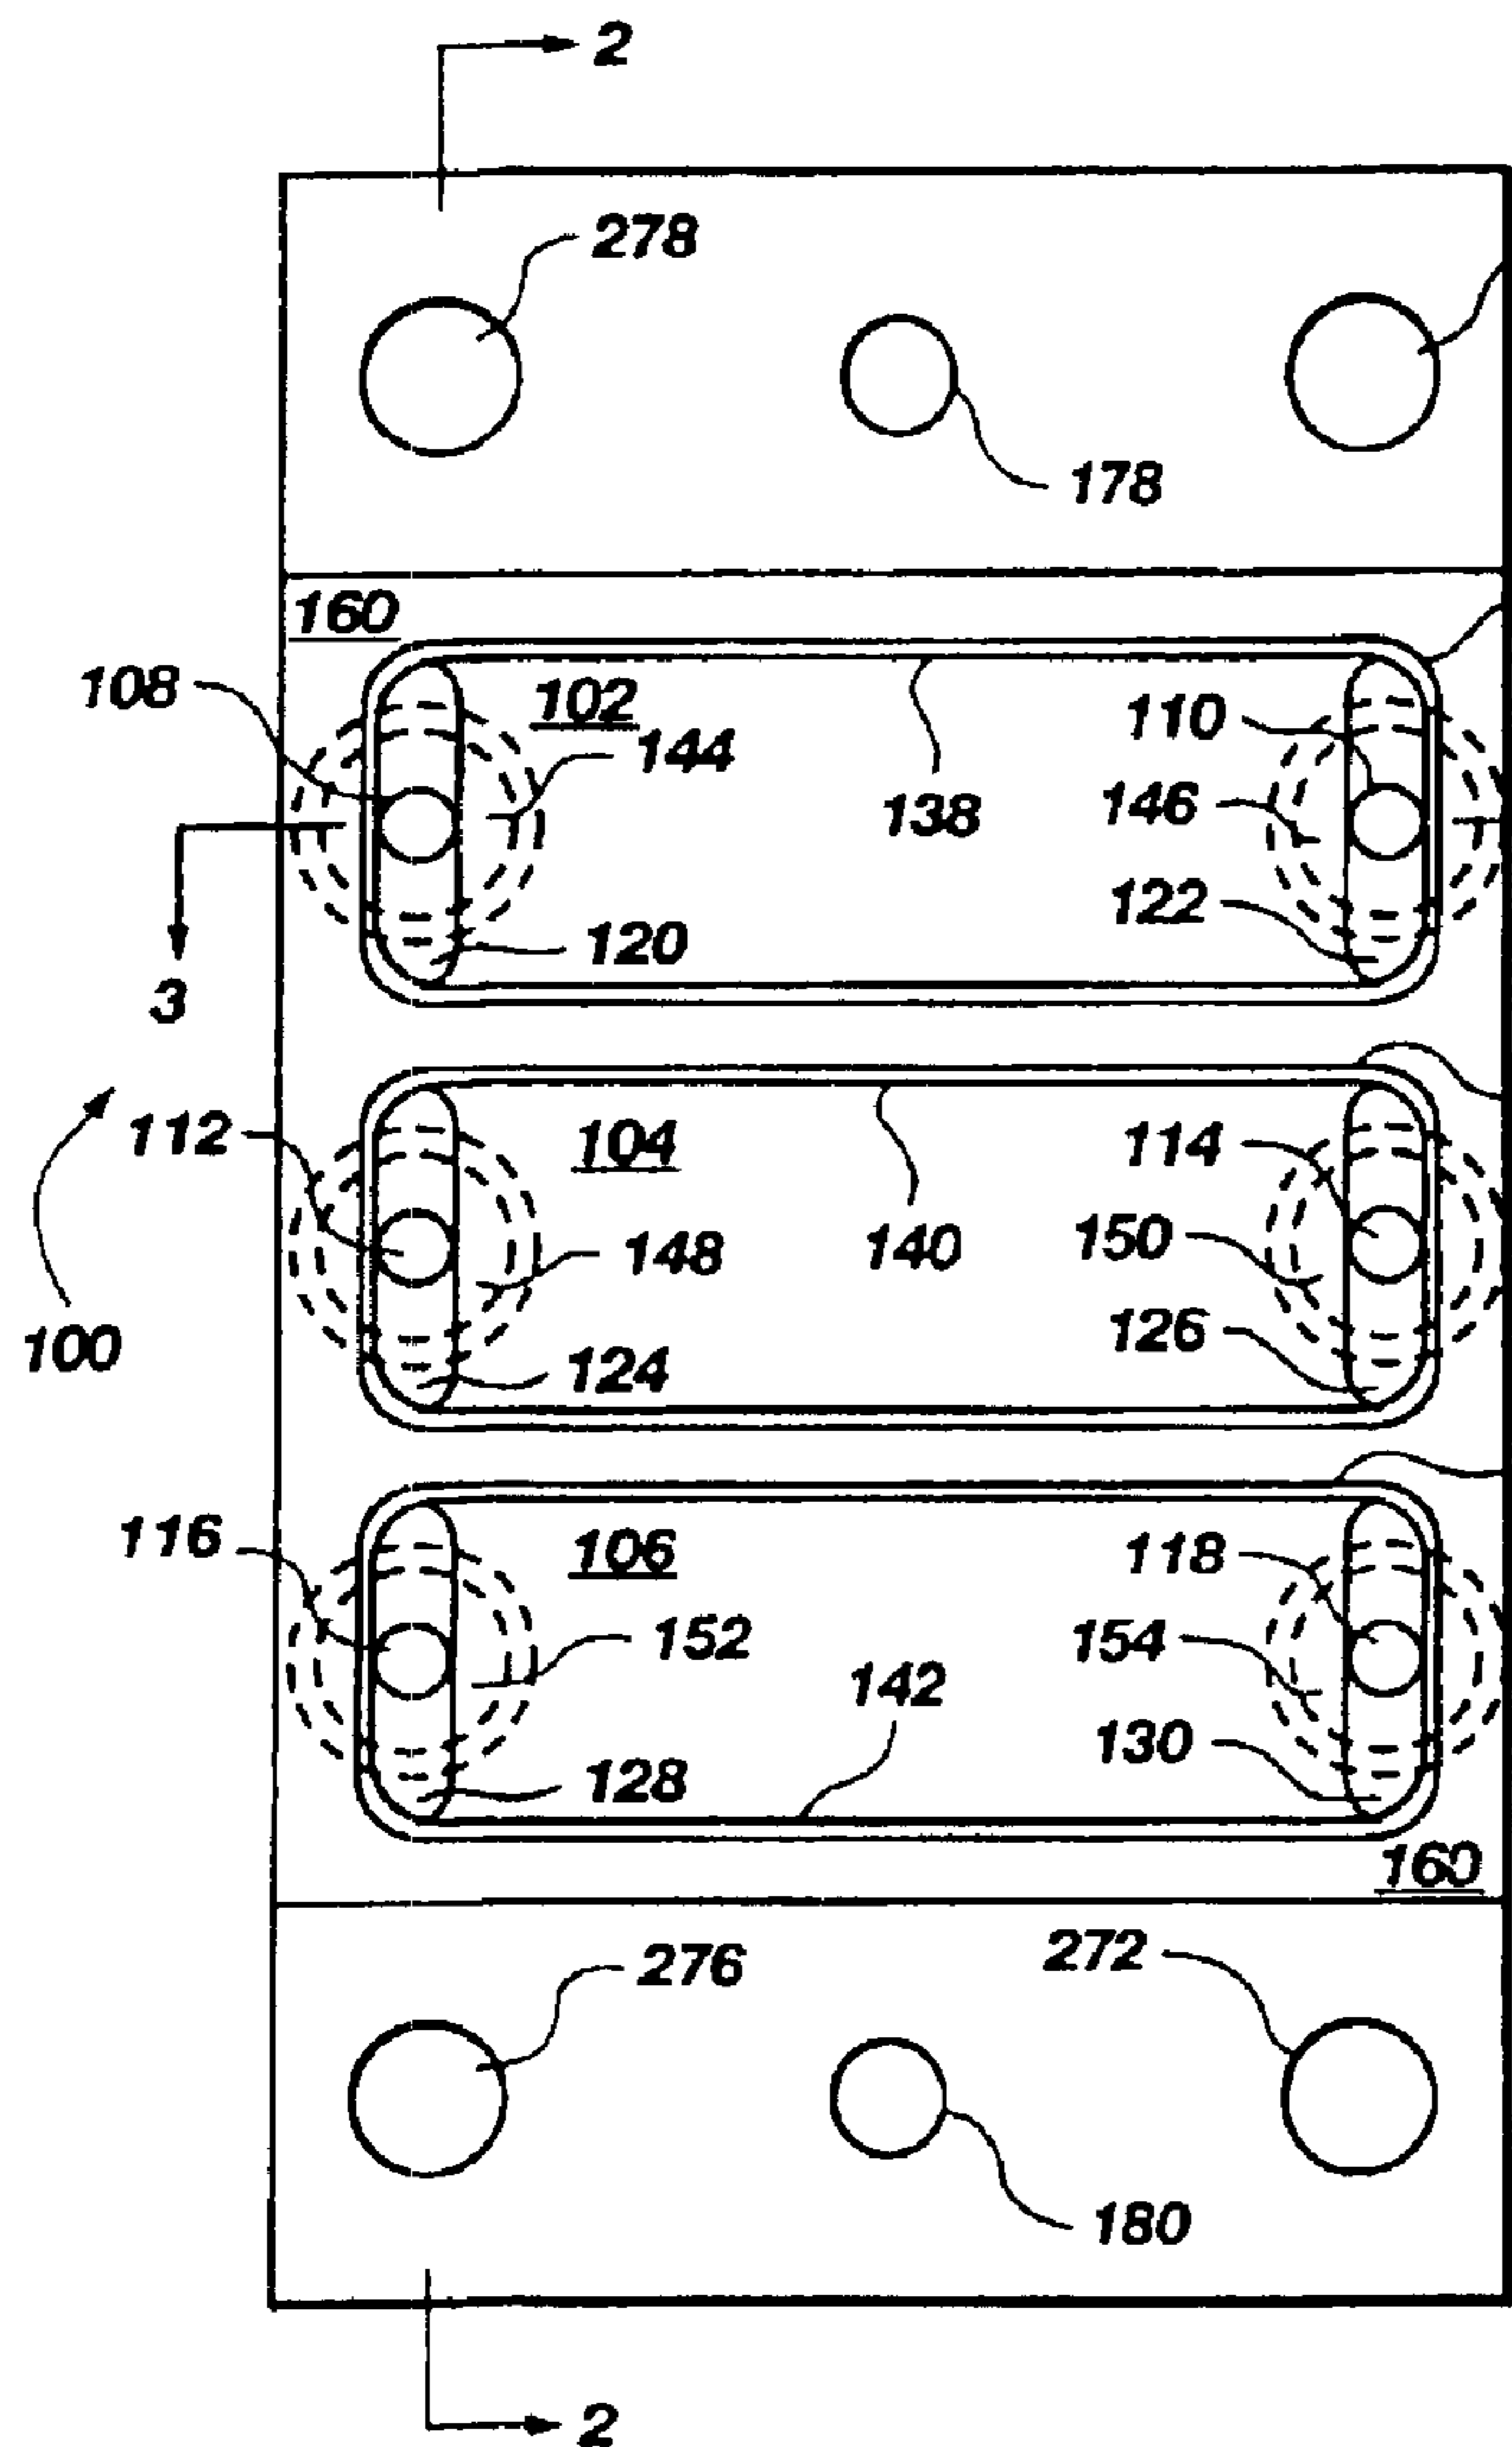


Fig. 1

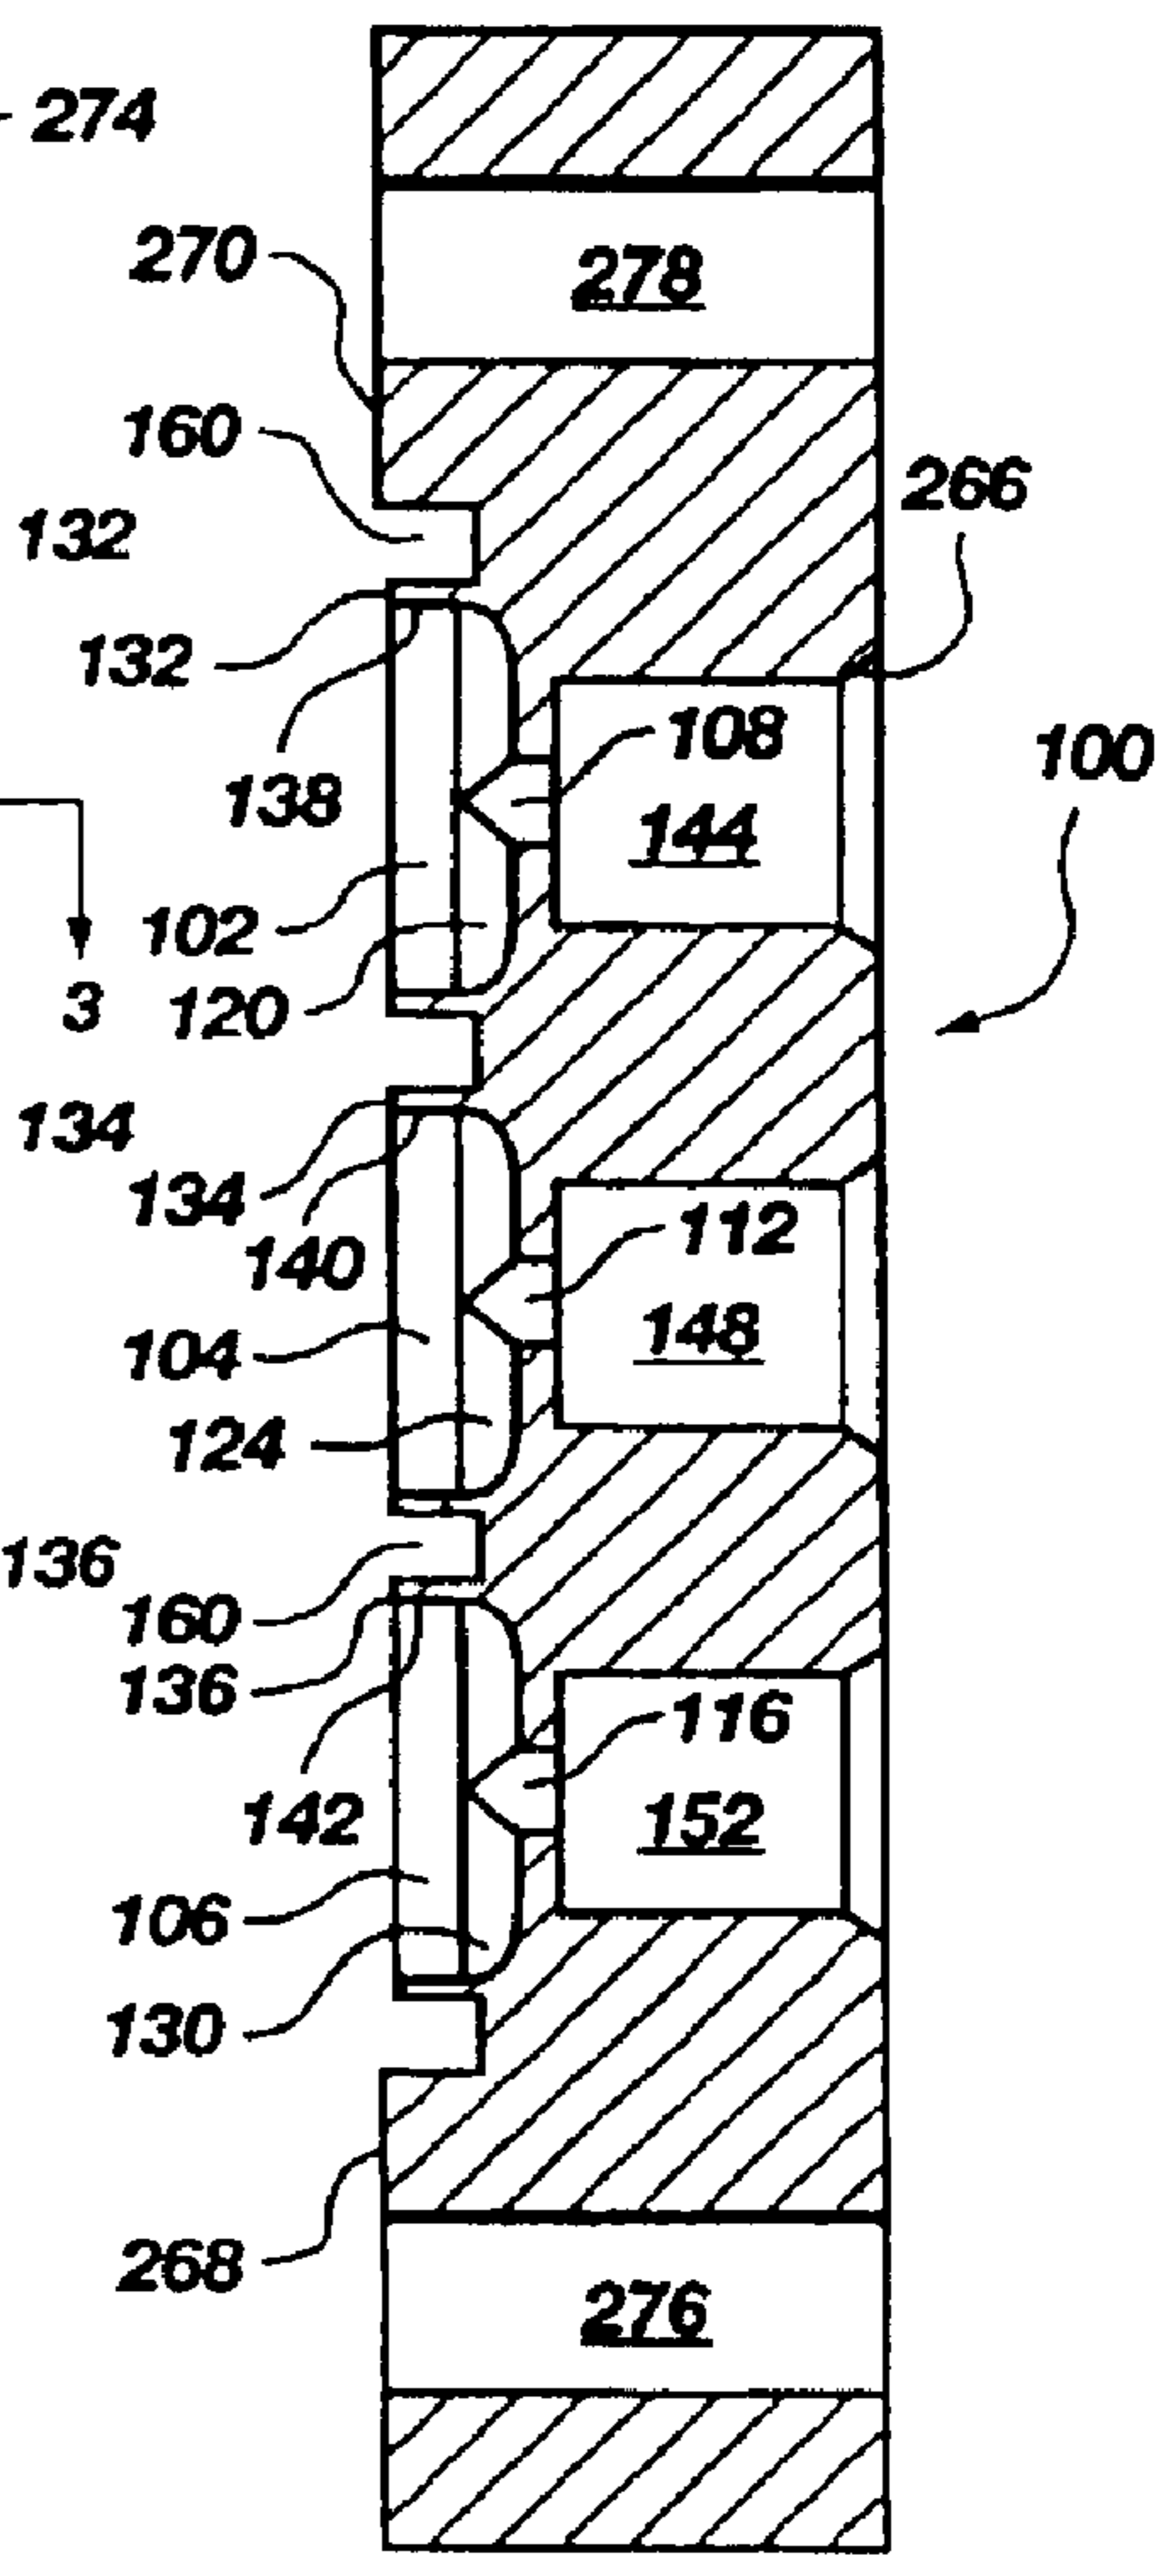


Fig. 2

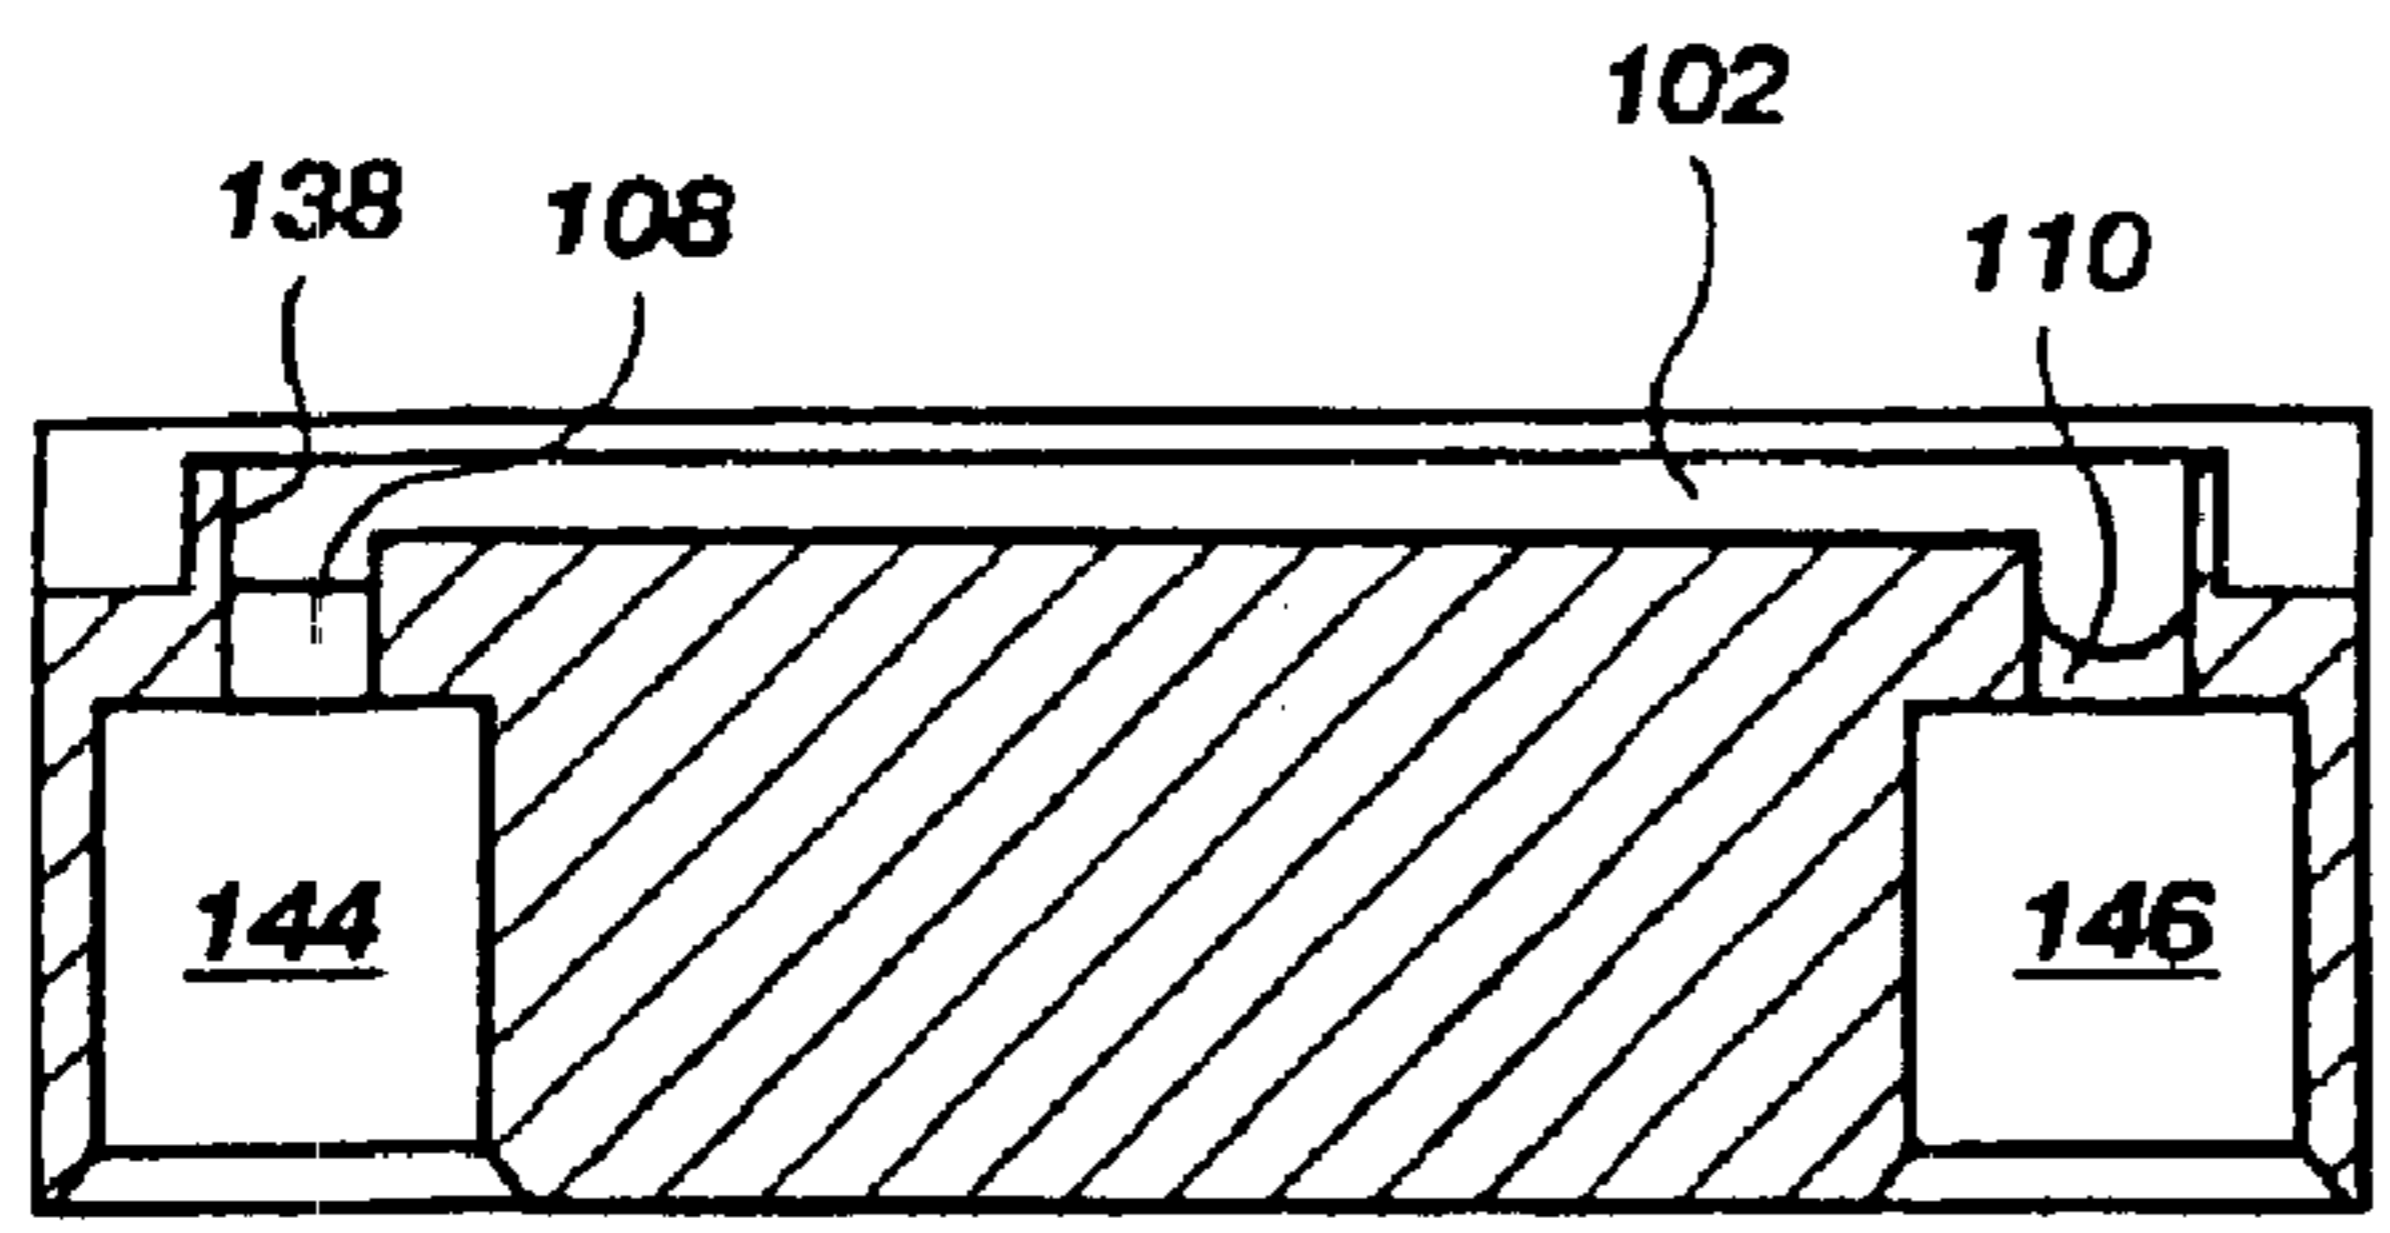


Fig. 3

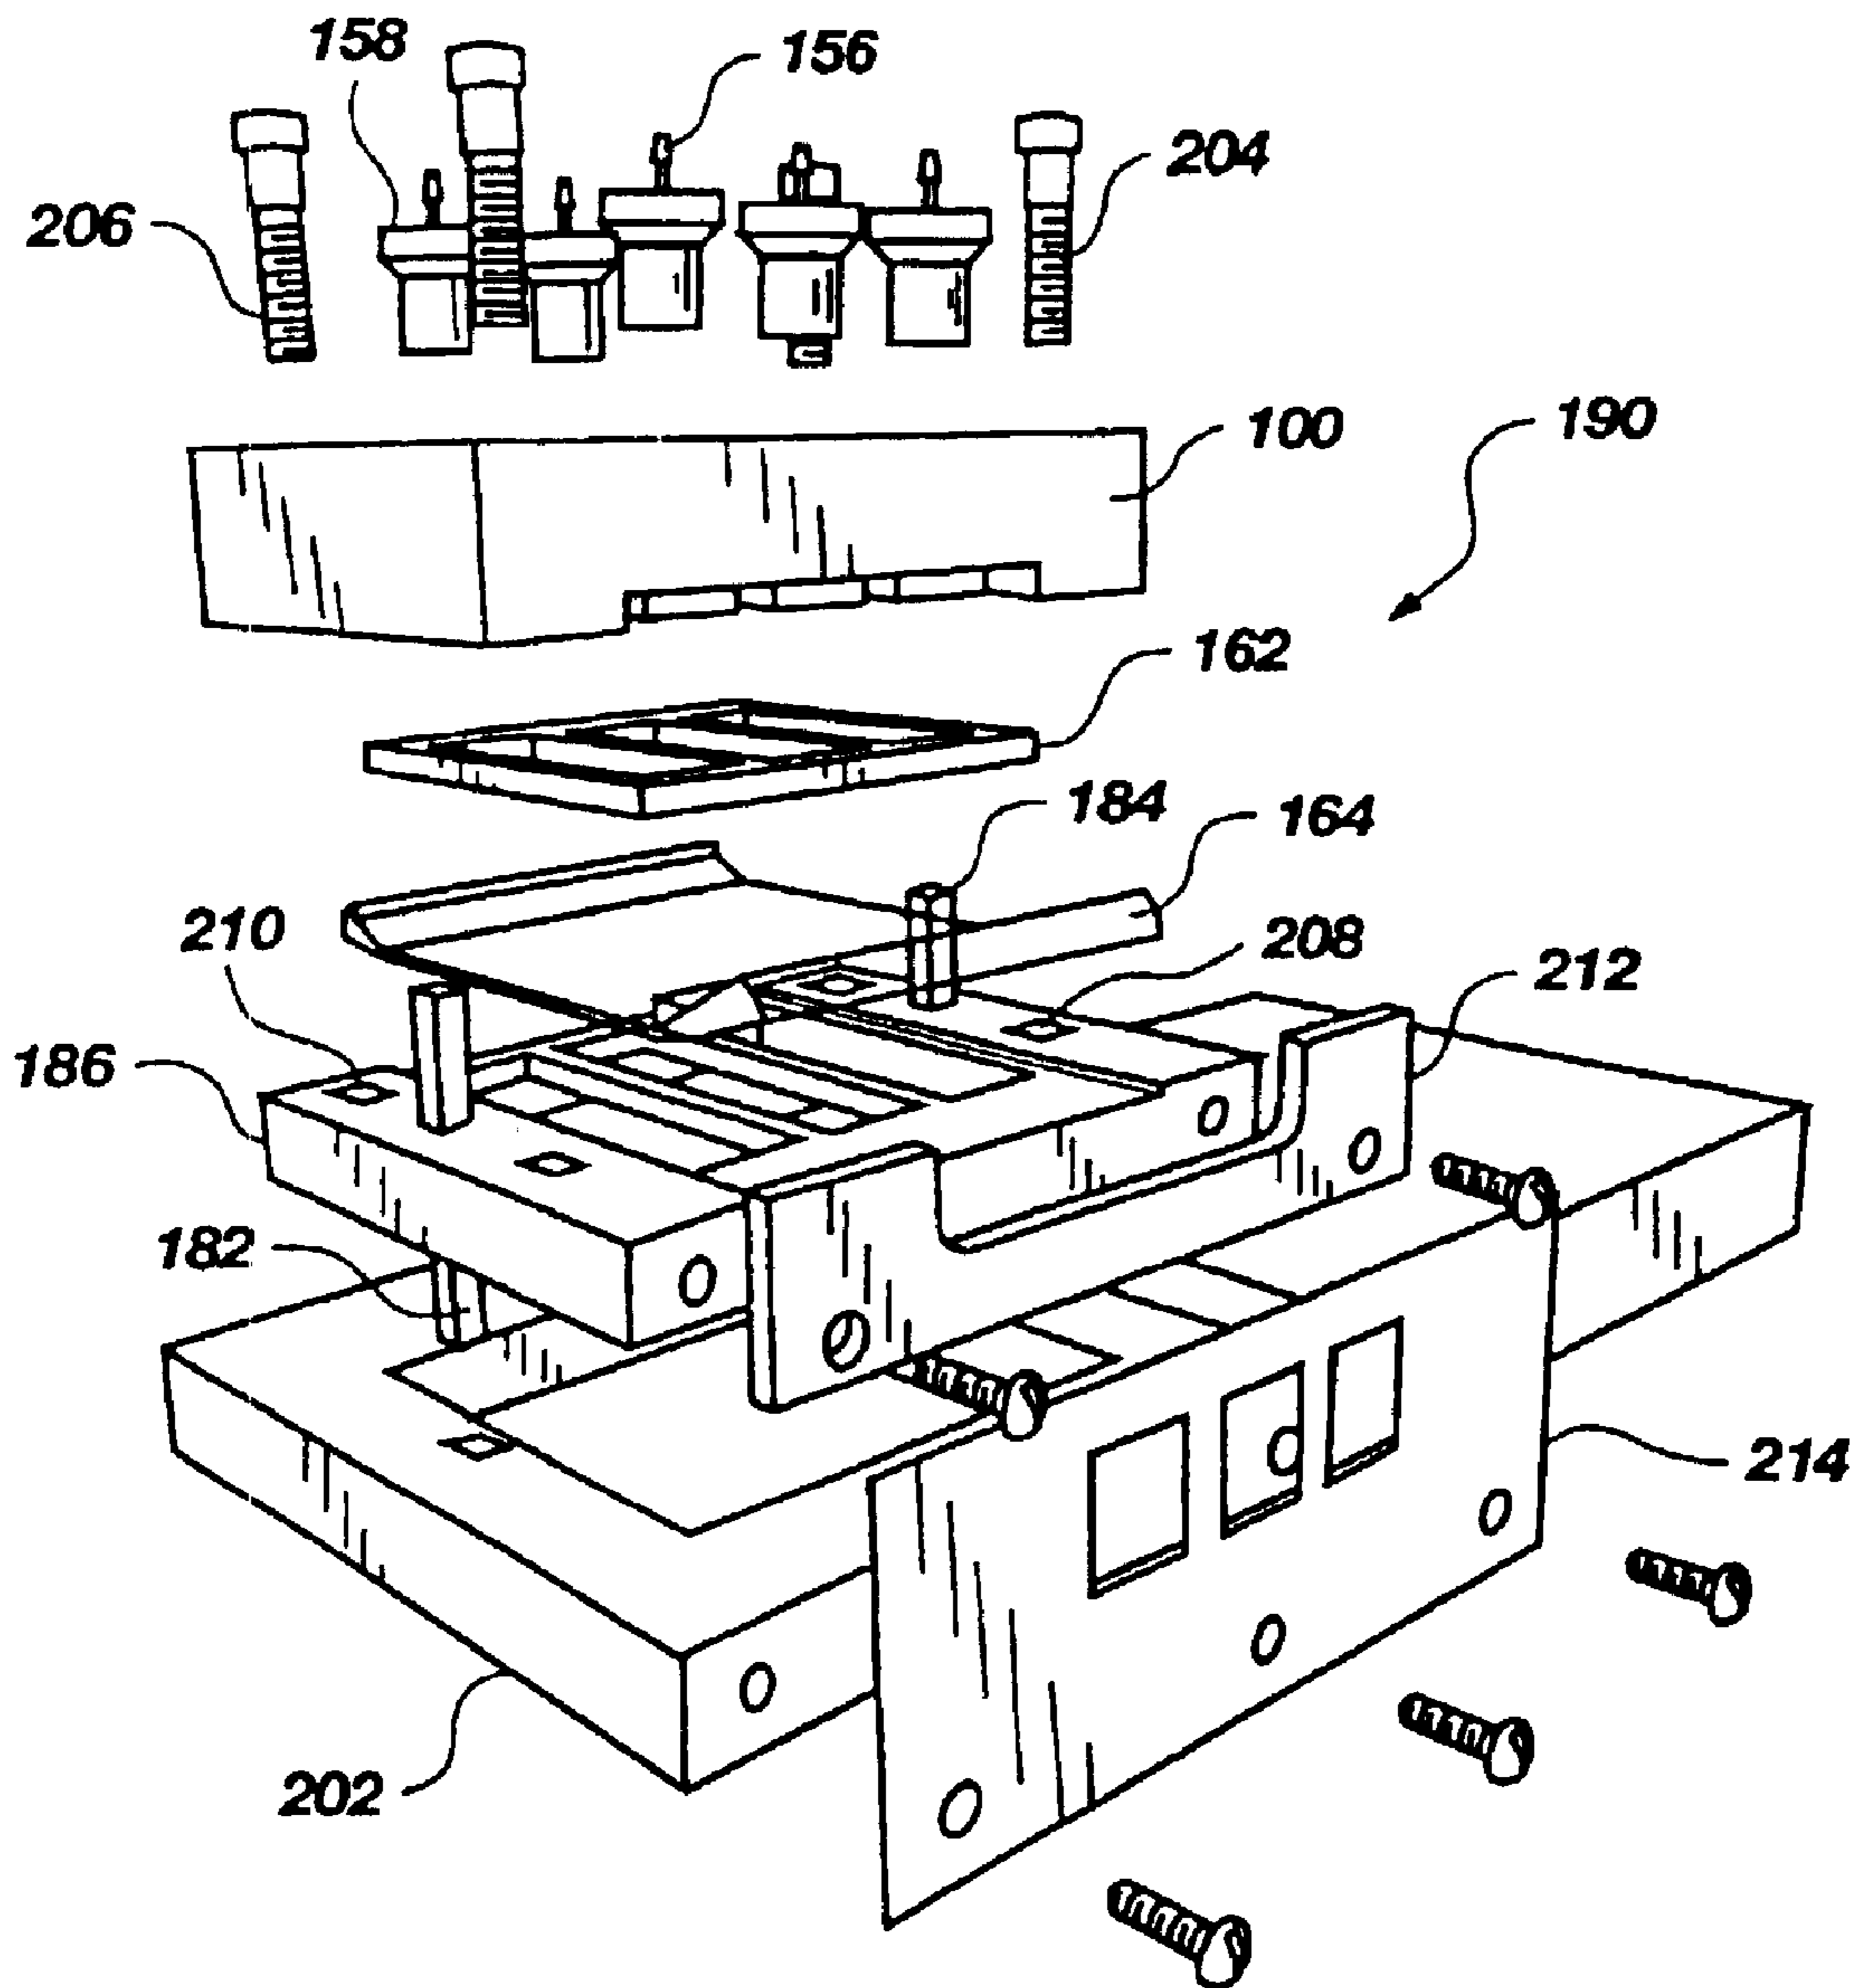


Fig. 4



Fig. 5

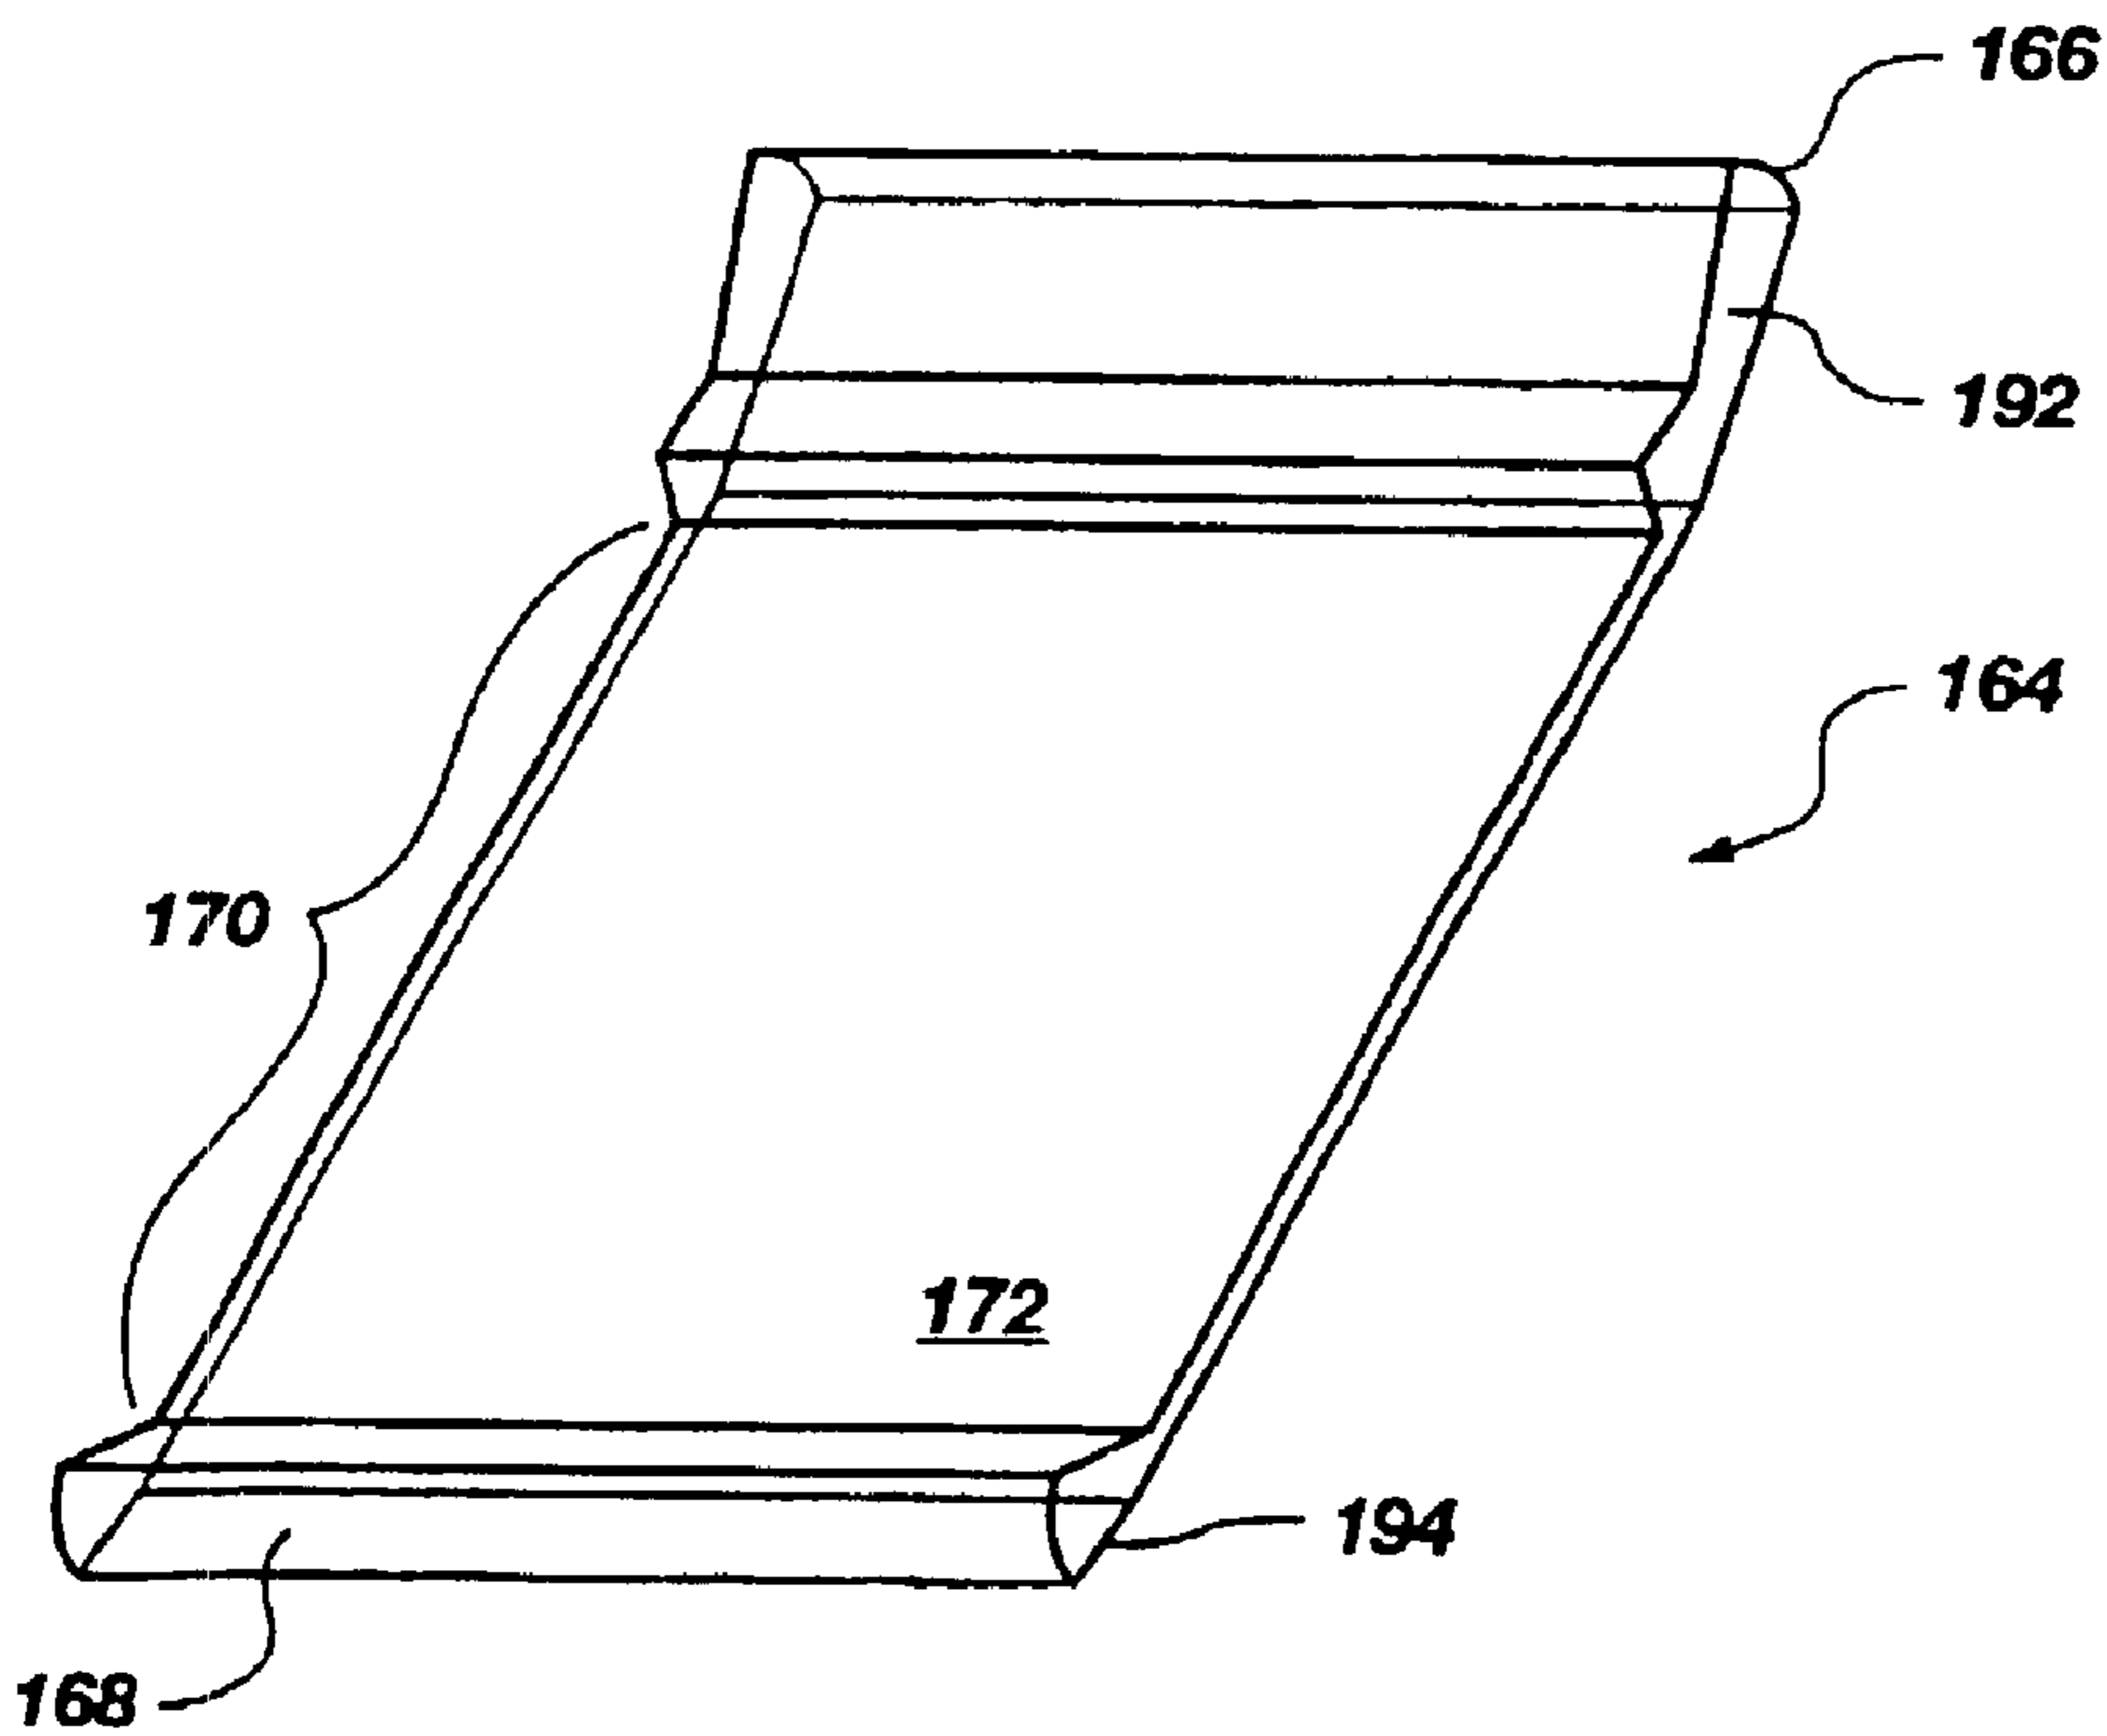


Fig. 6

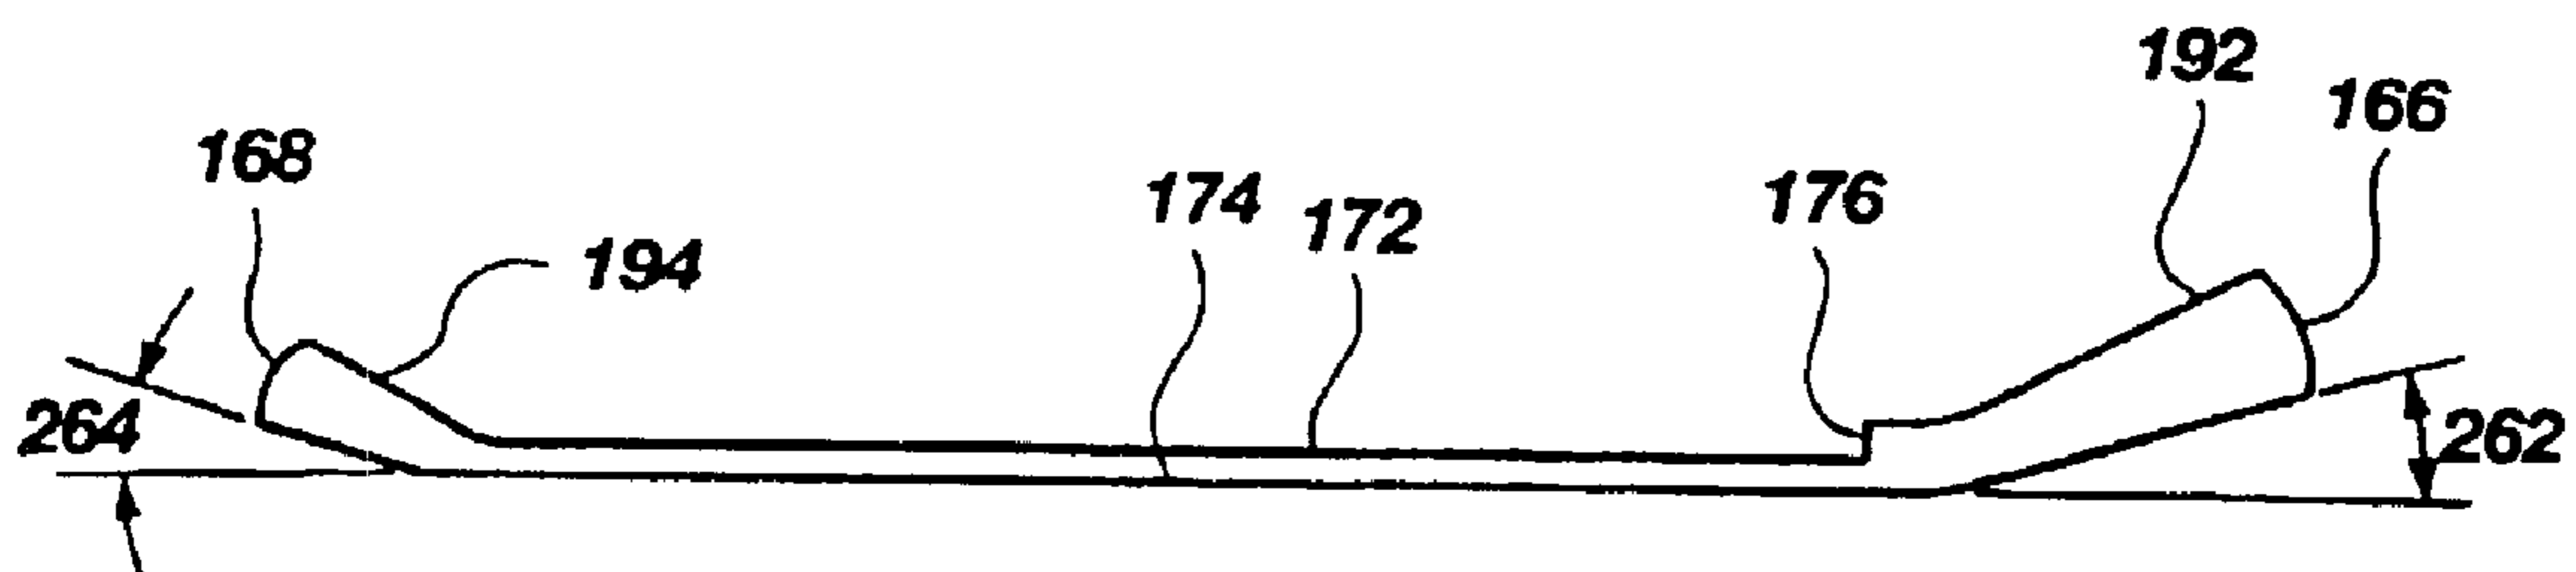


Fig. 7

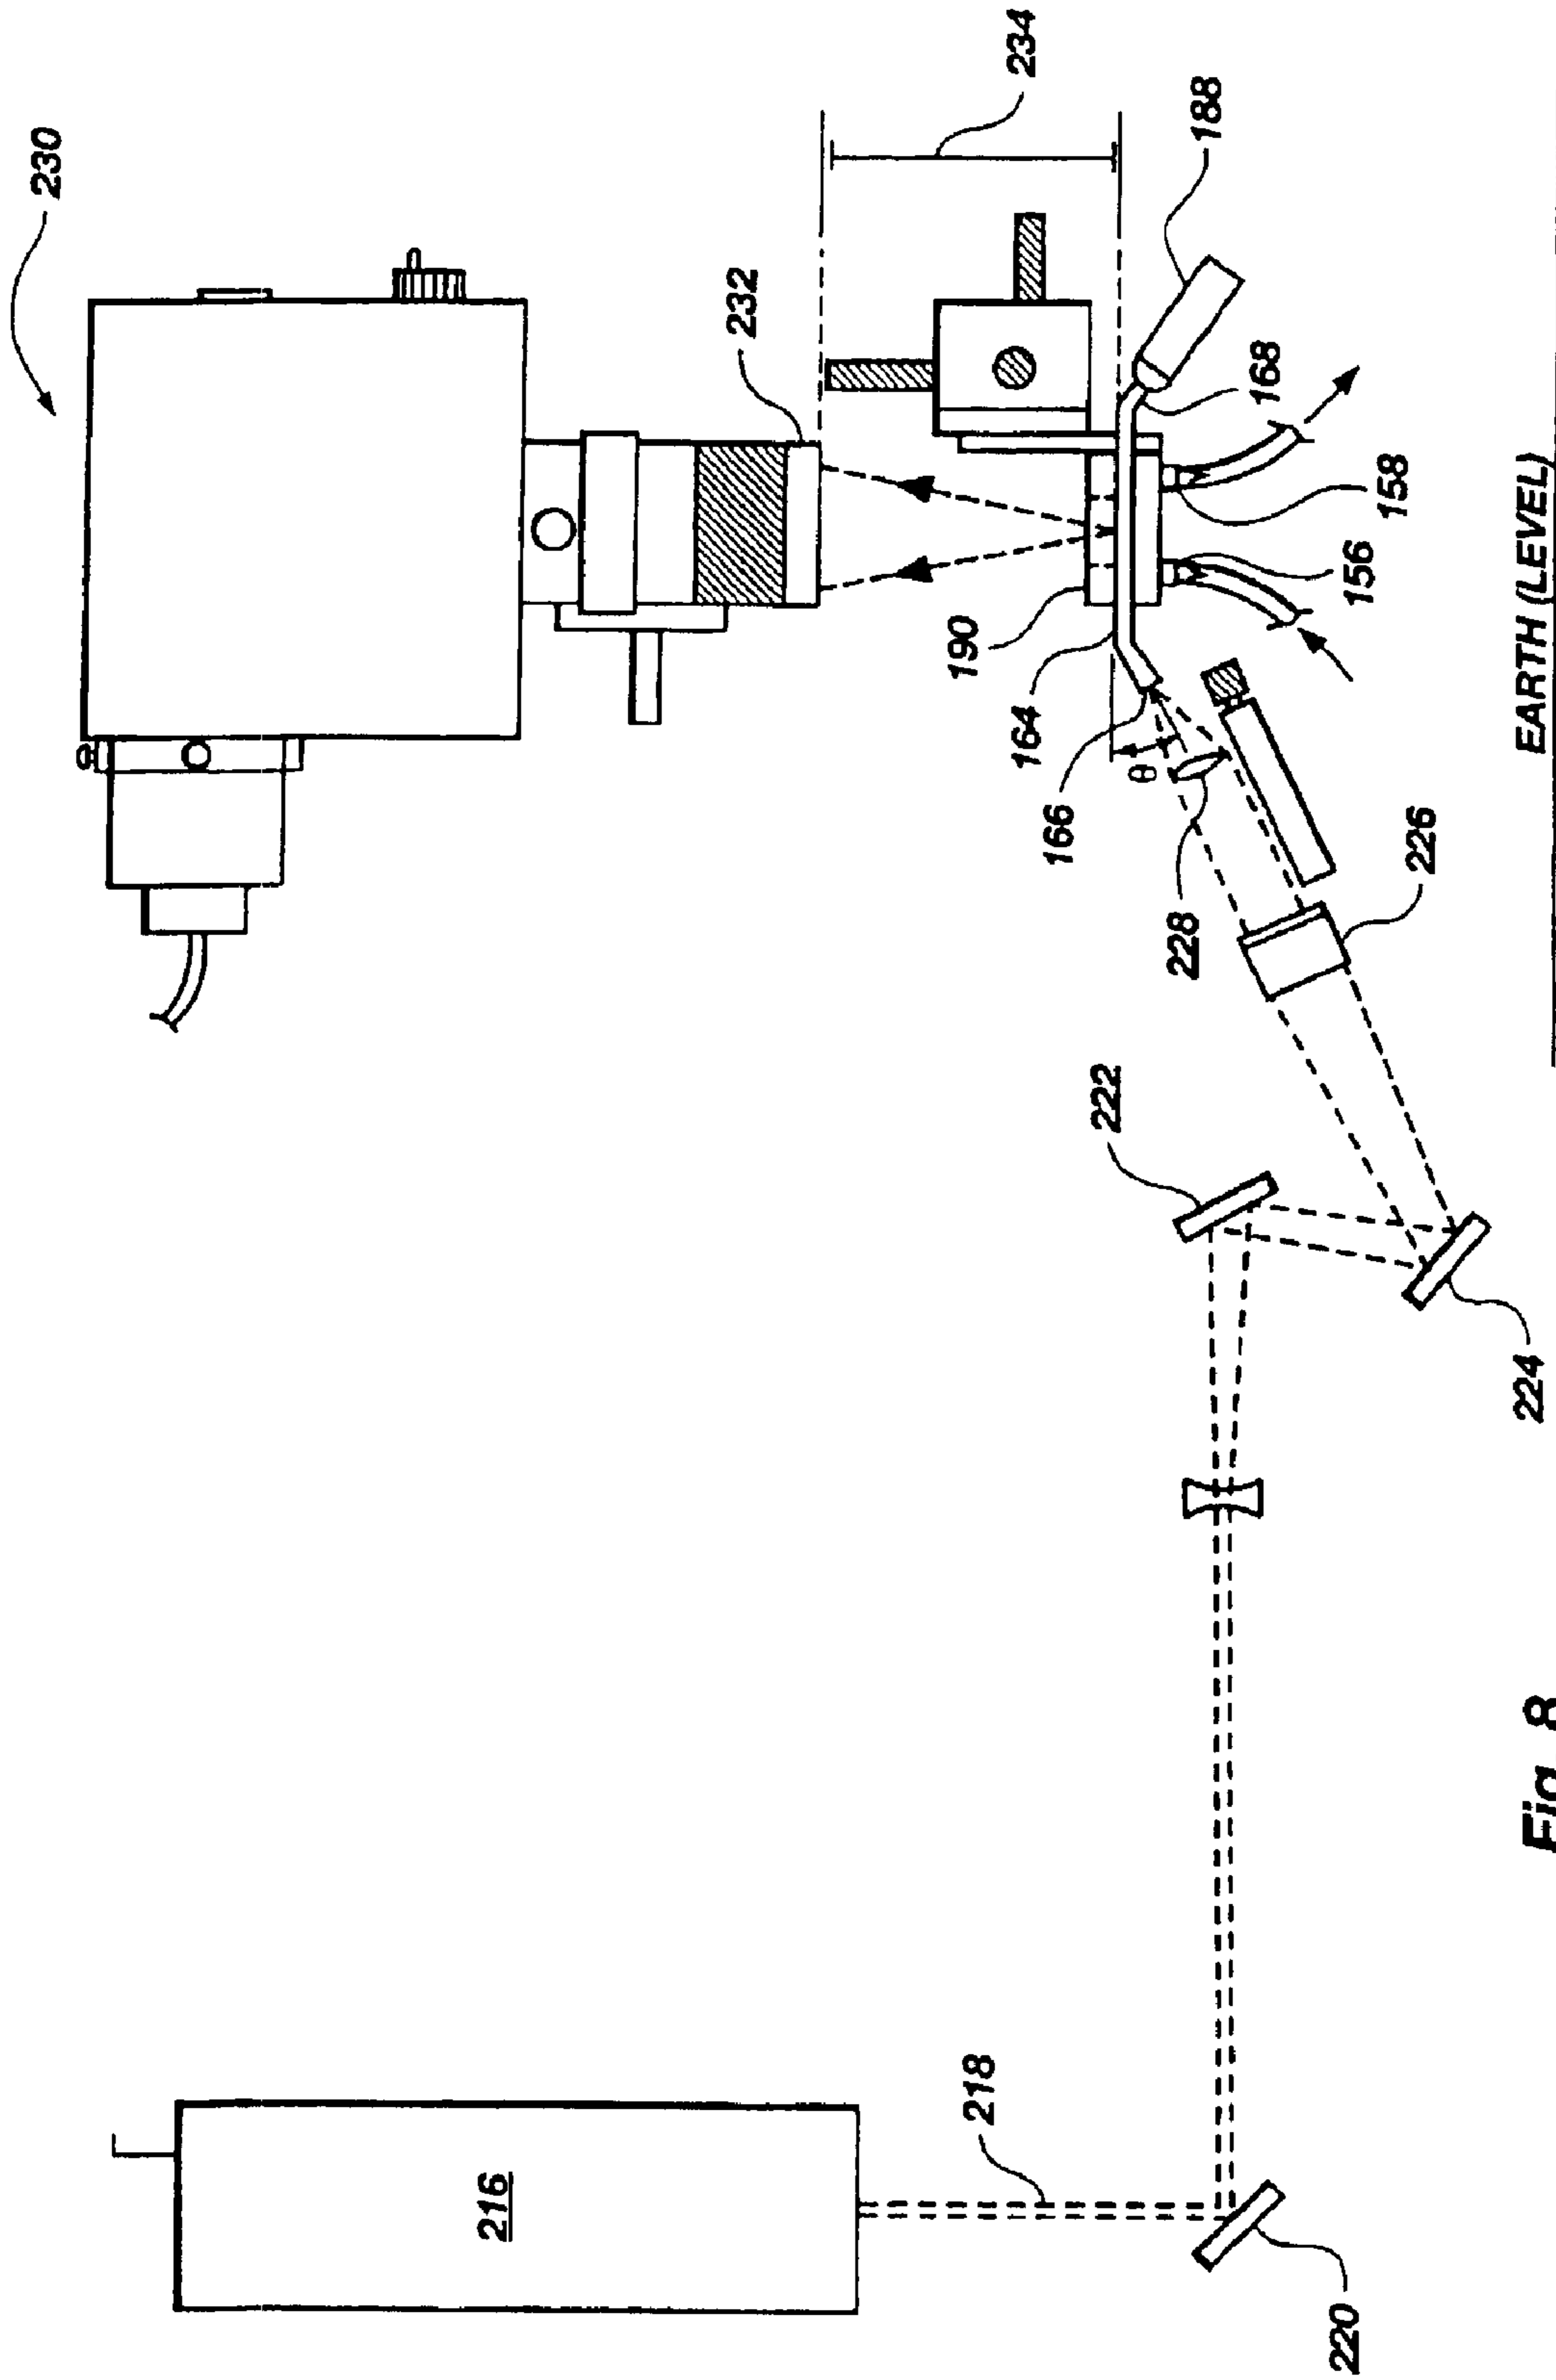


Fig. 8

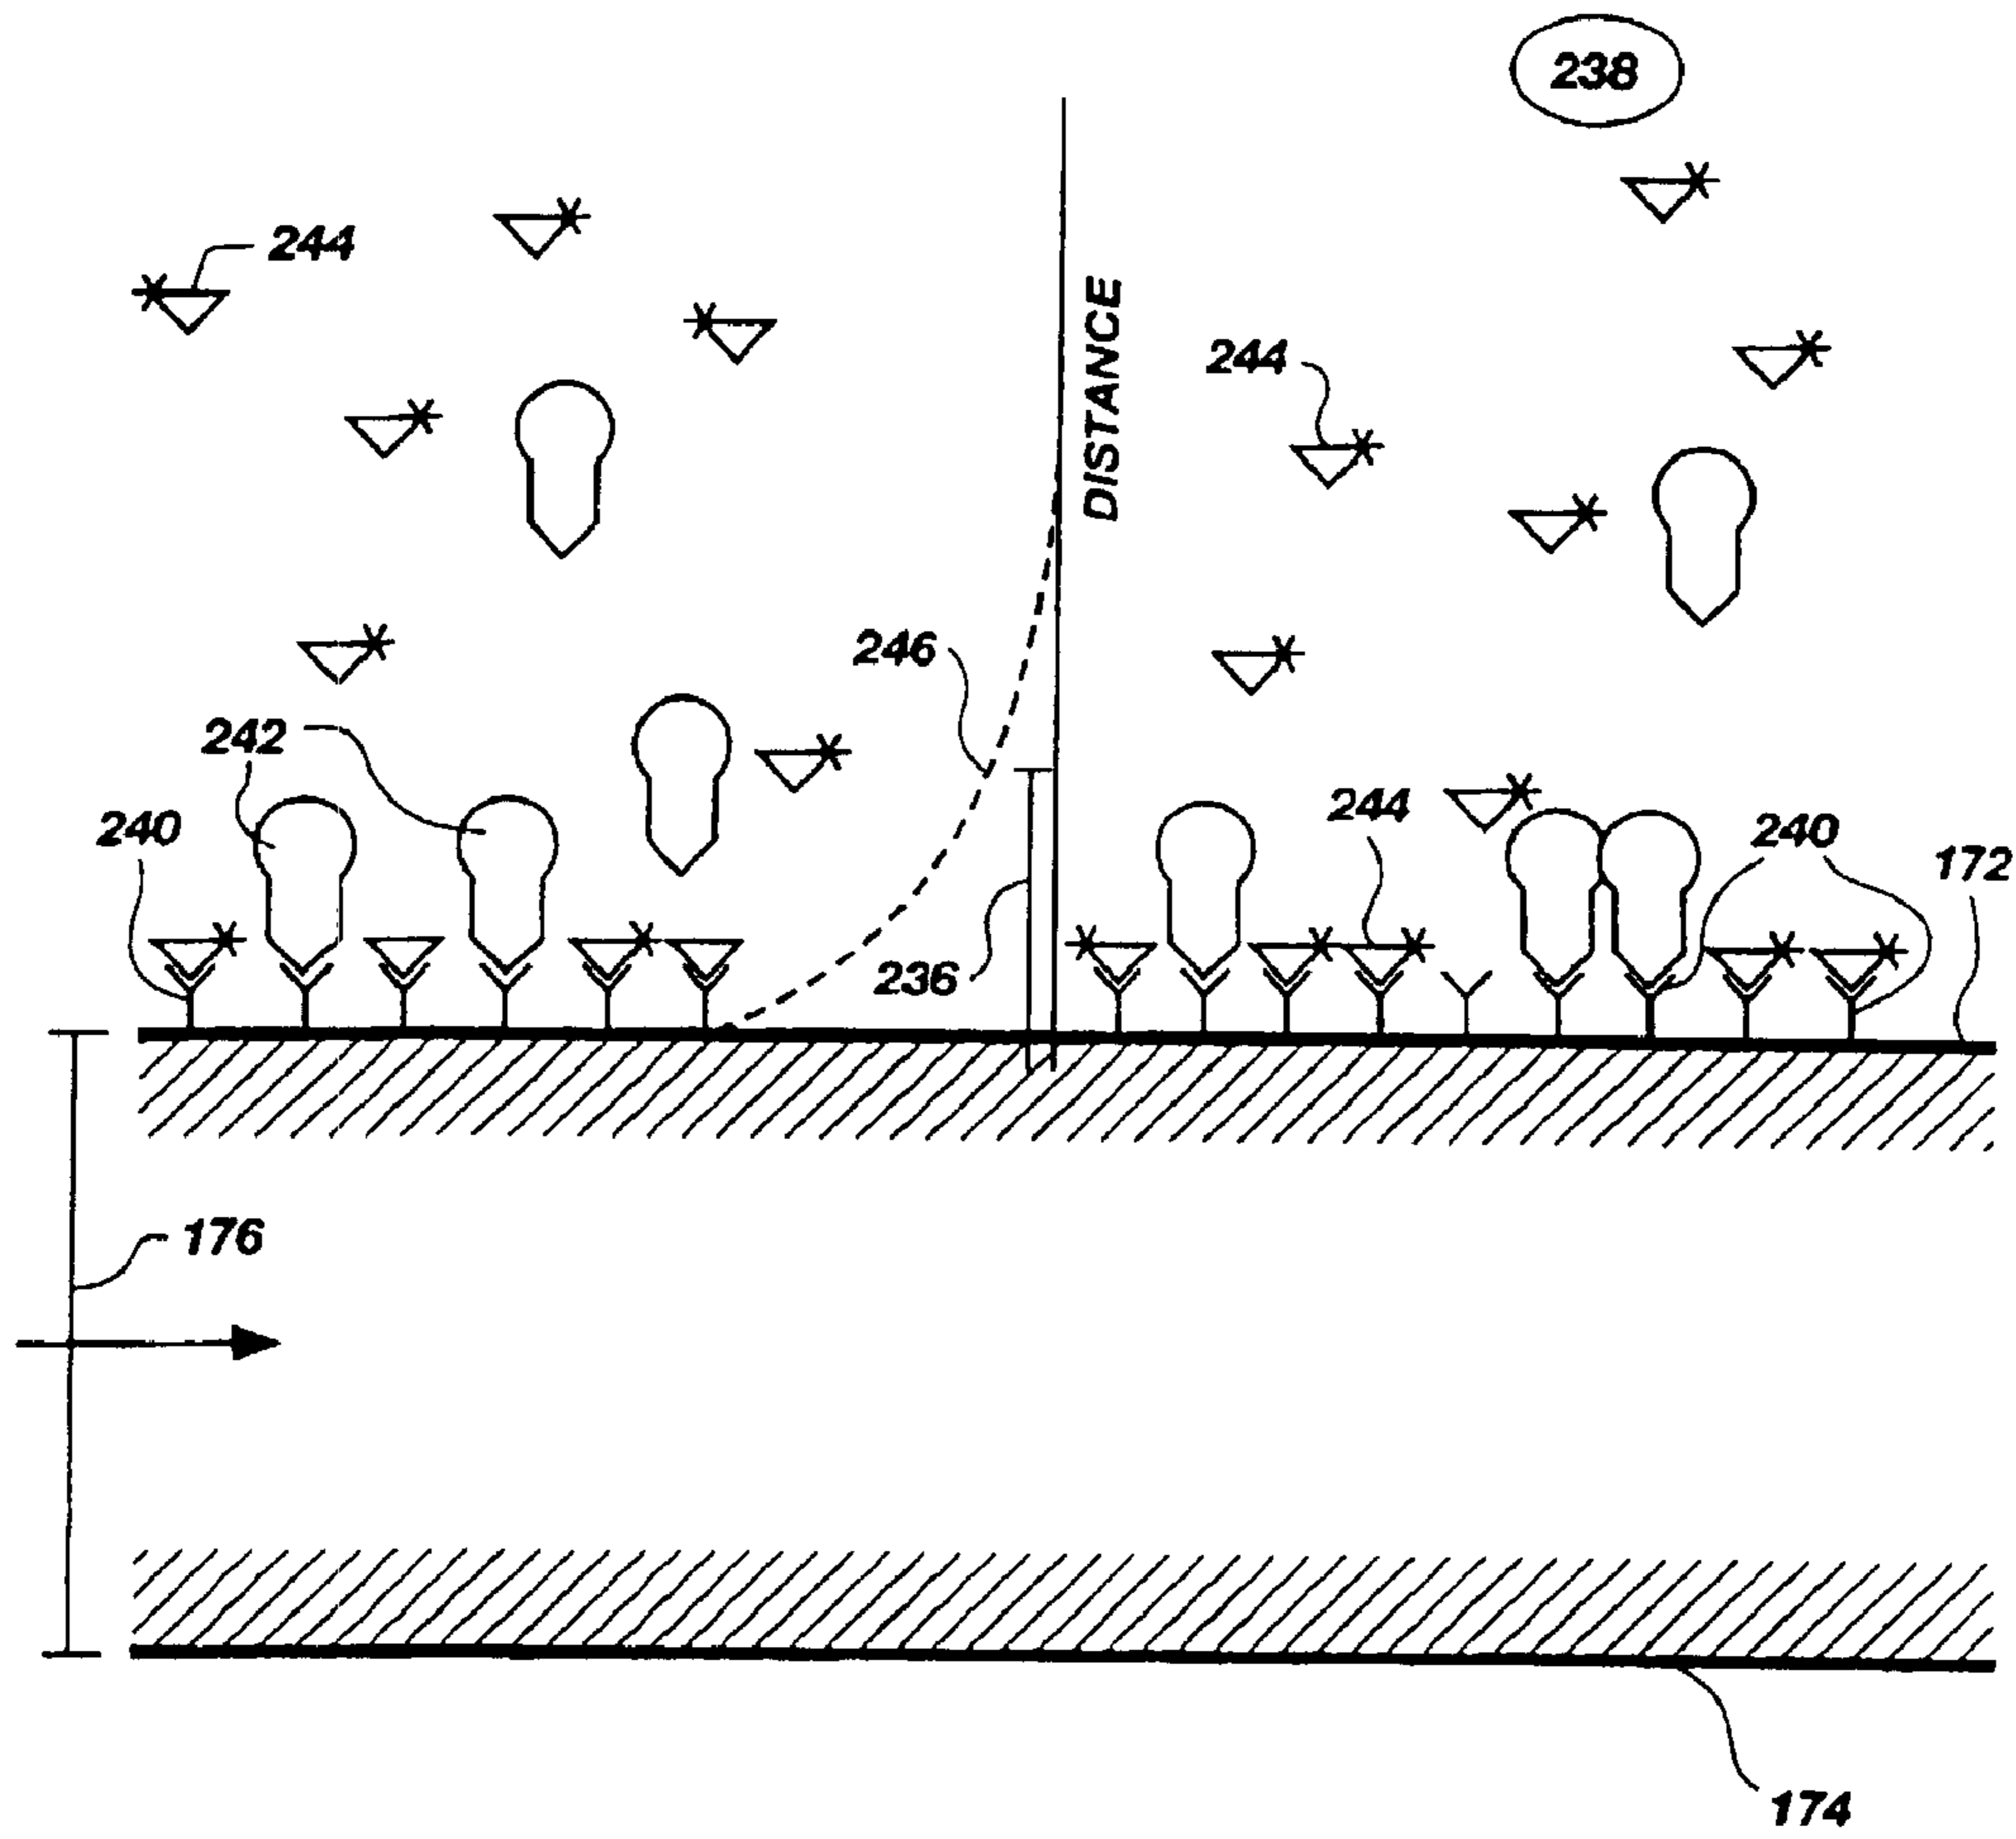


Fig. 9

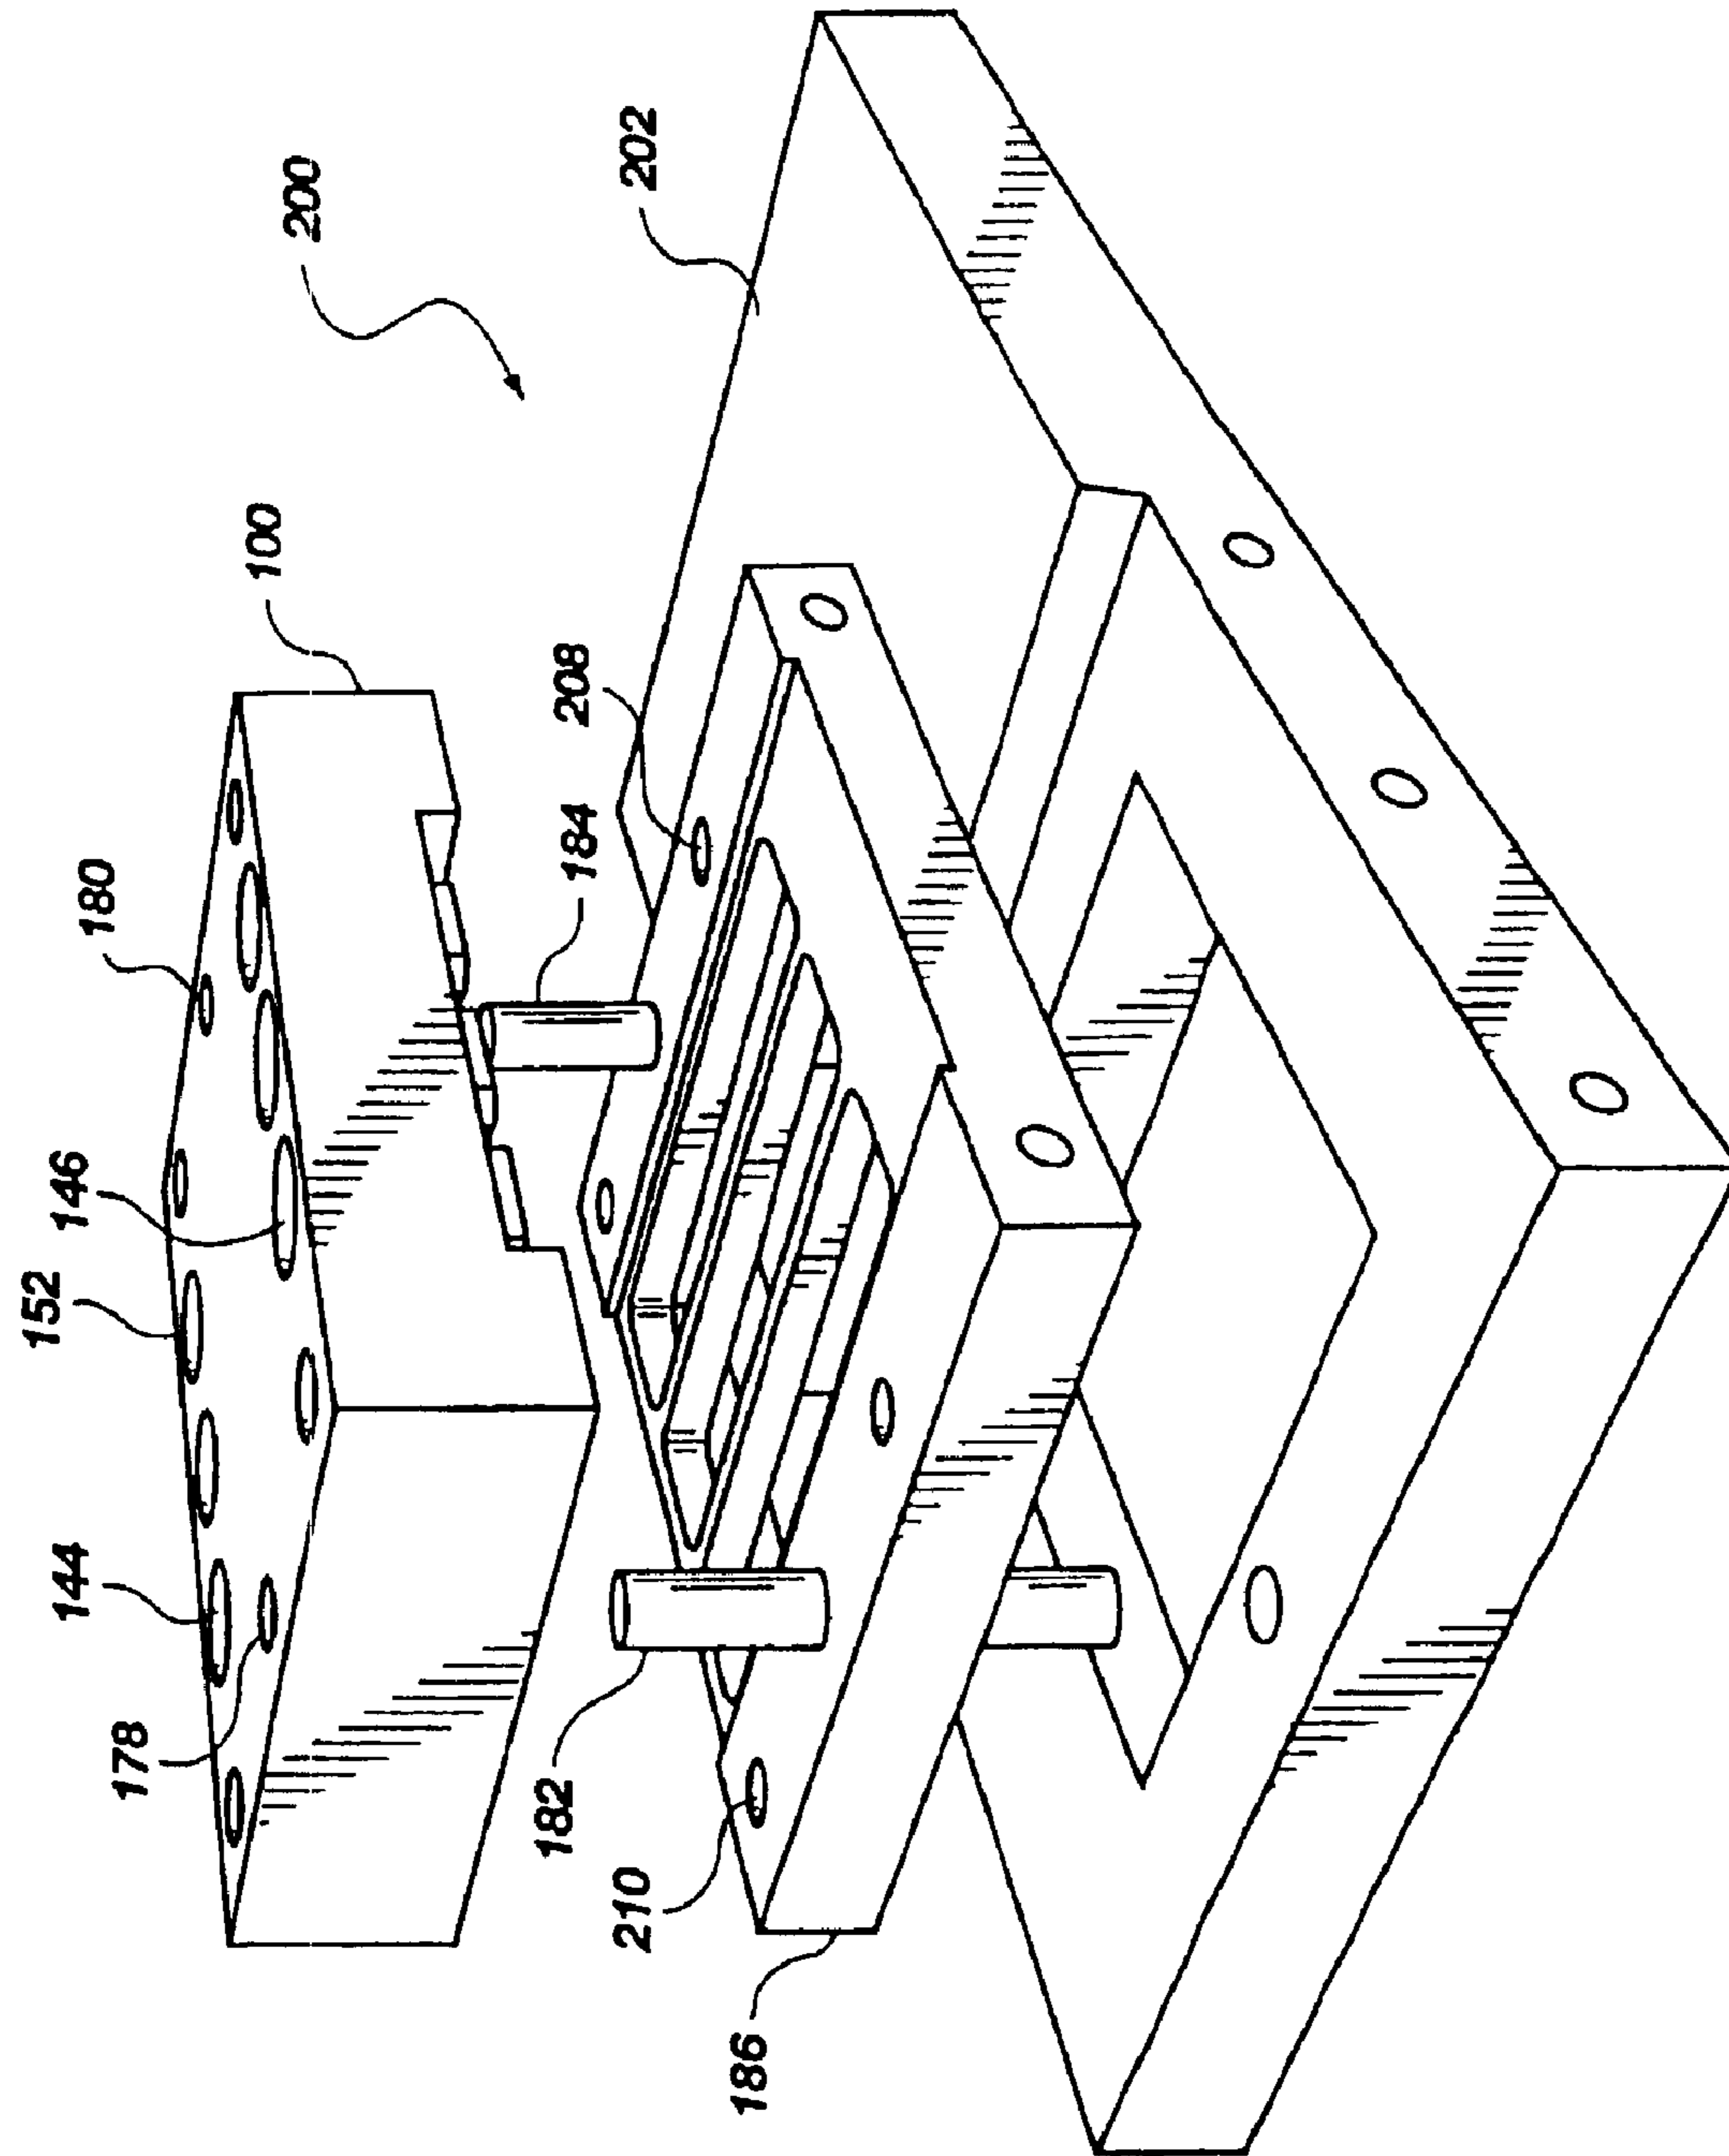


Fig. 10

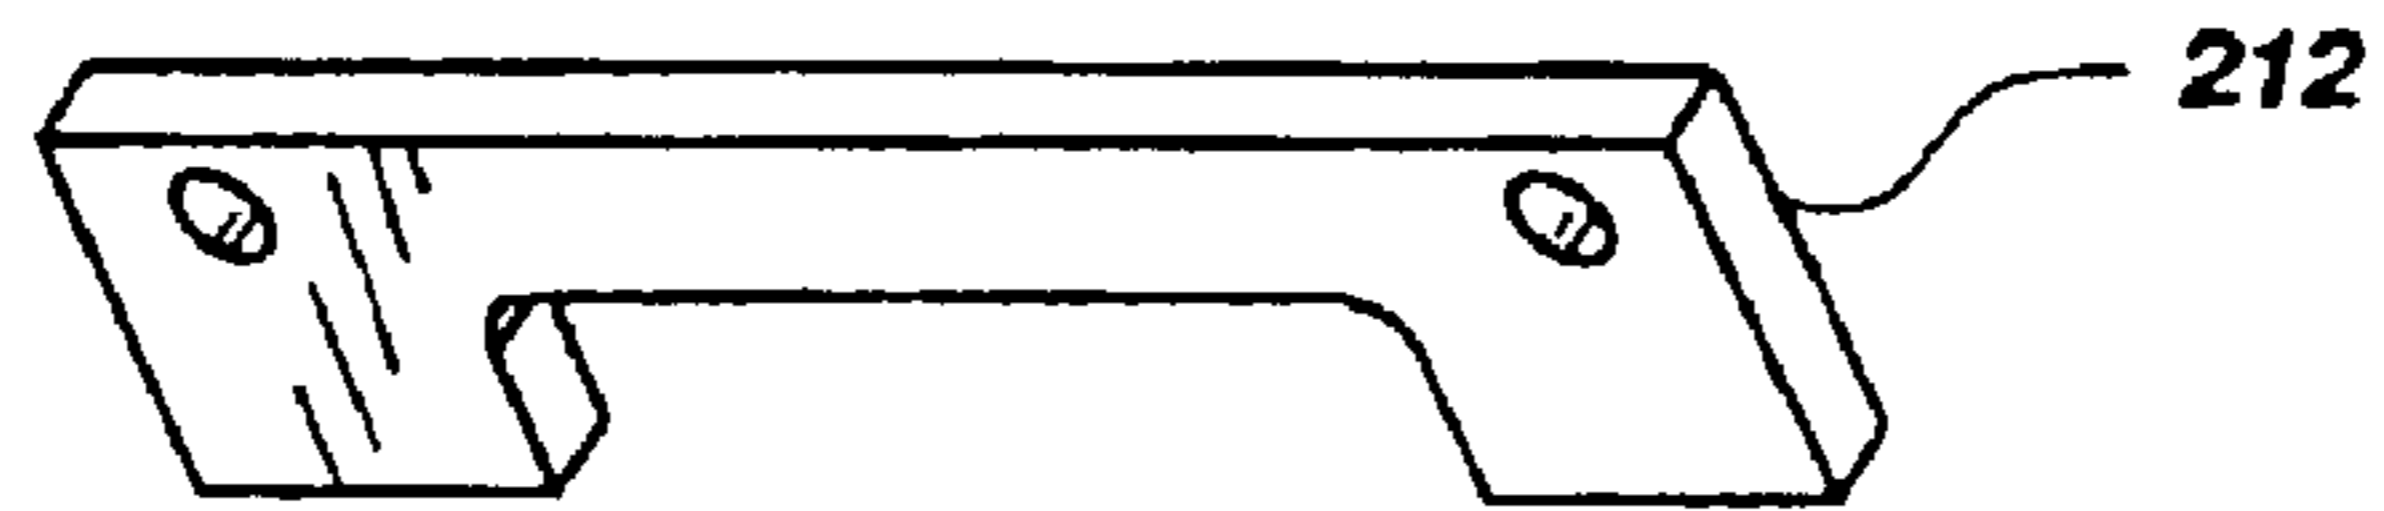


Fig. 14

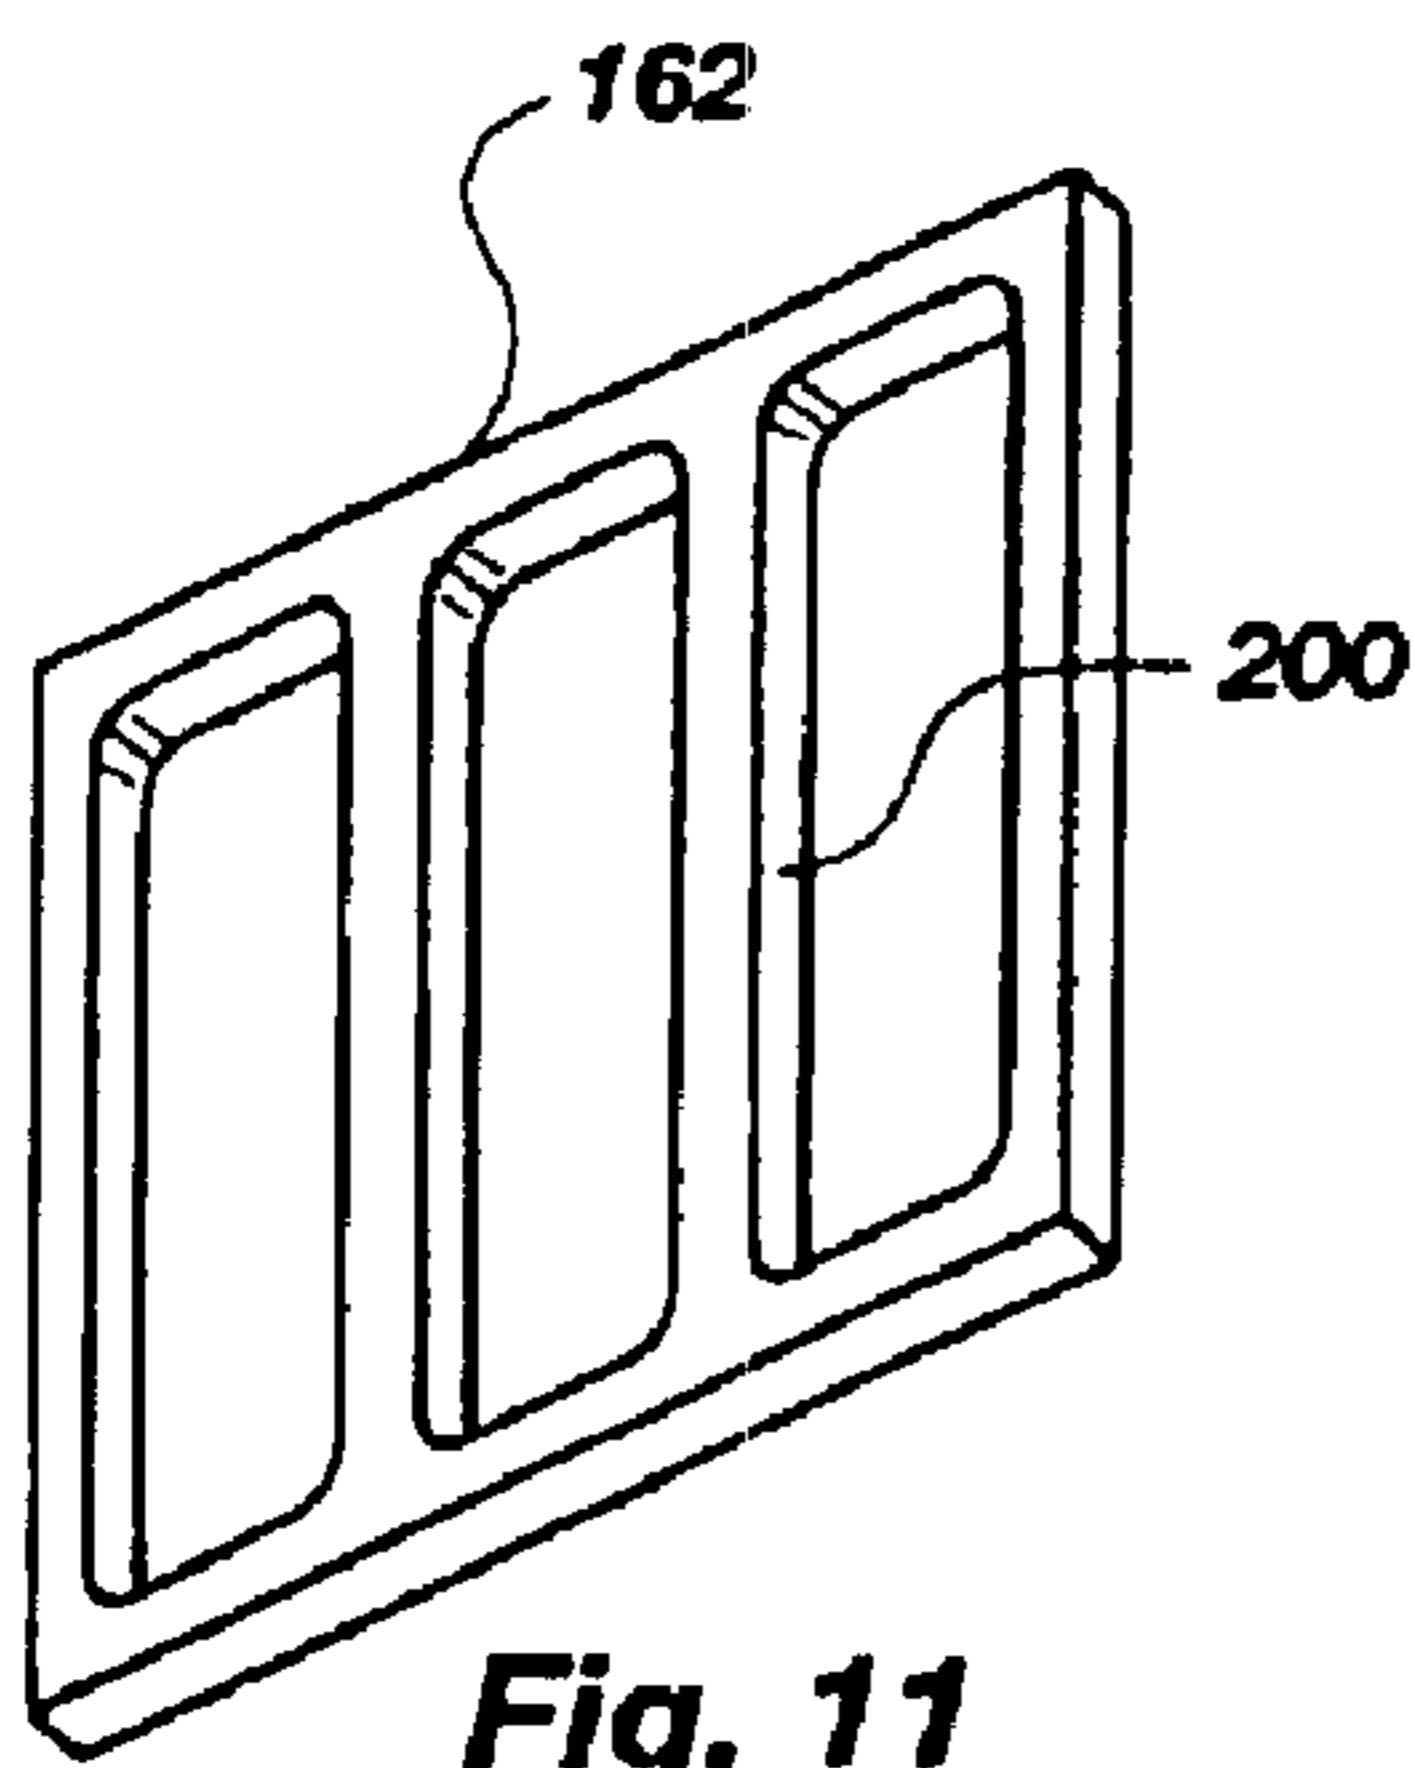


Fig. 11

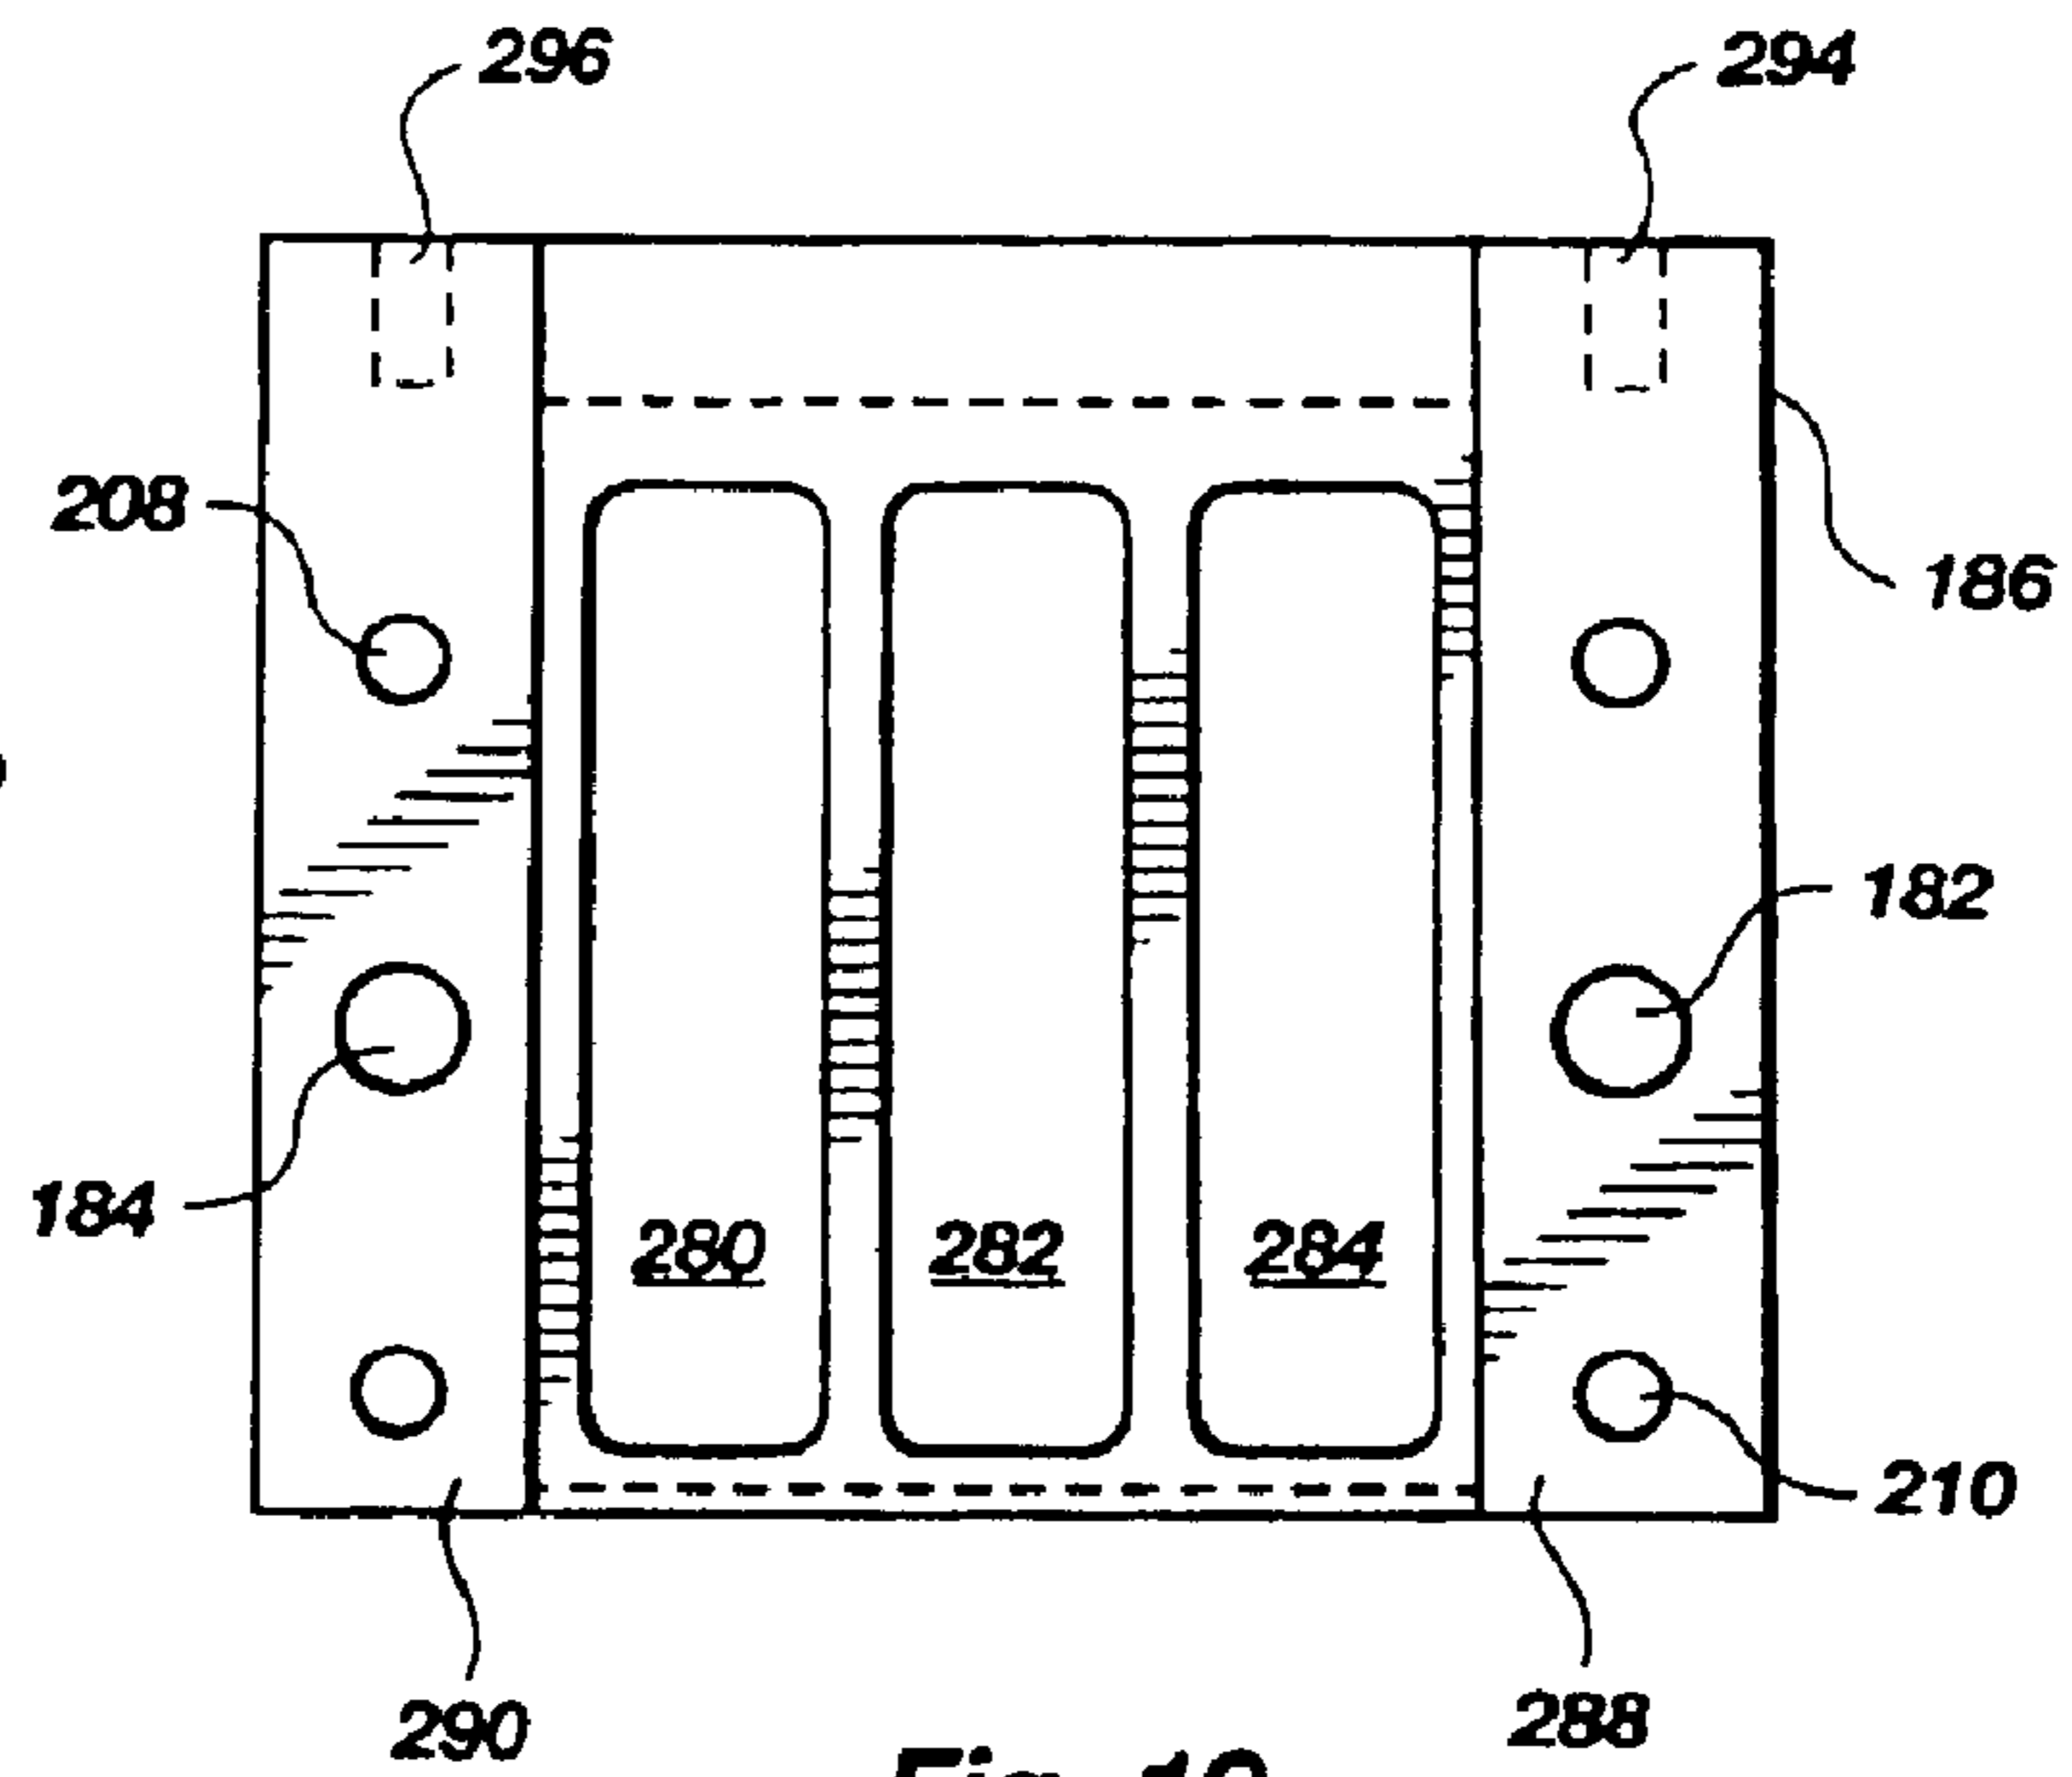


Fig. 12

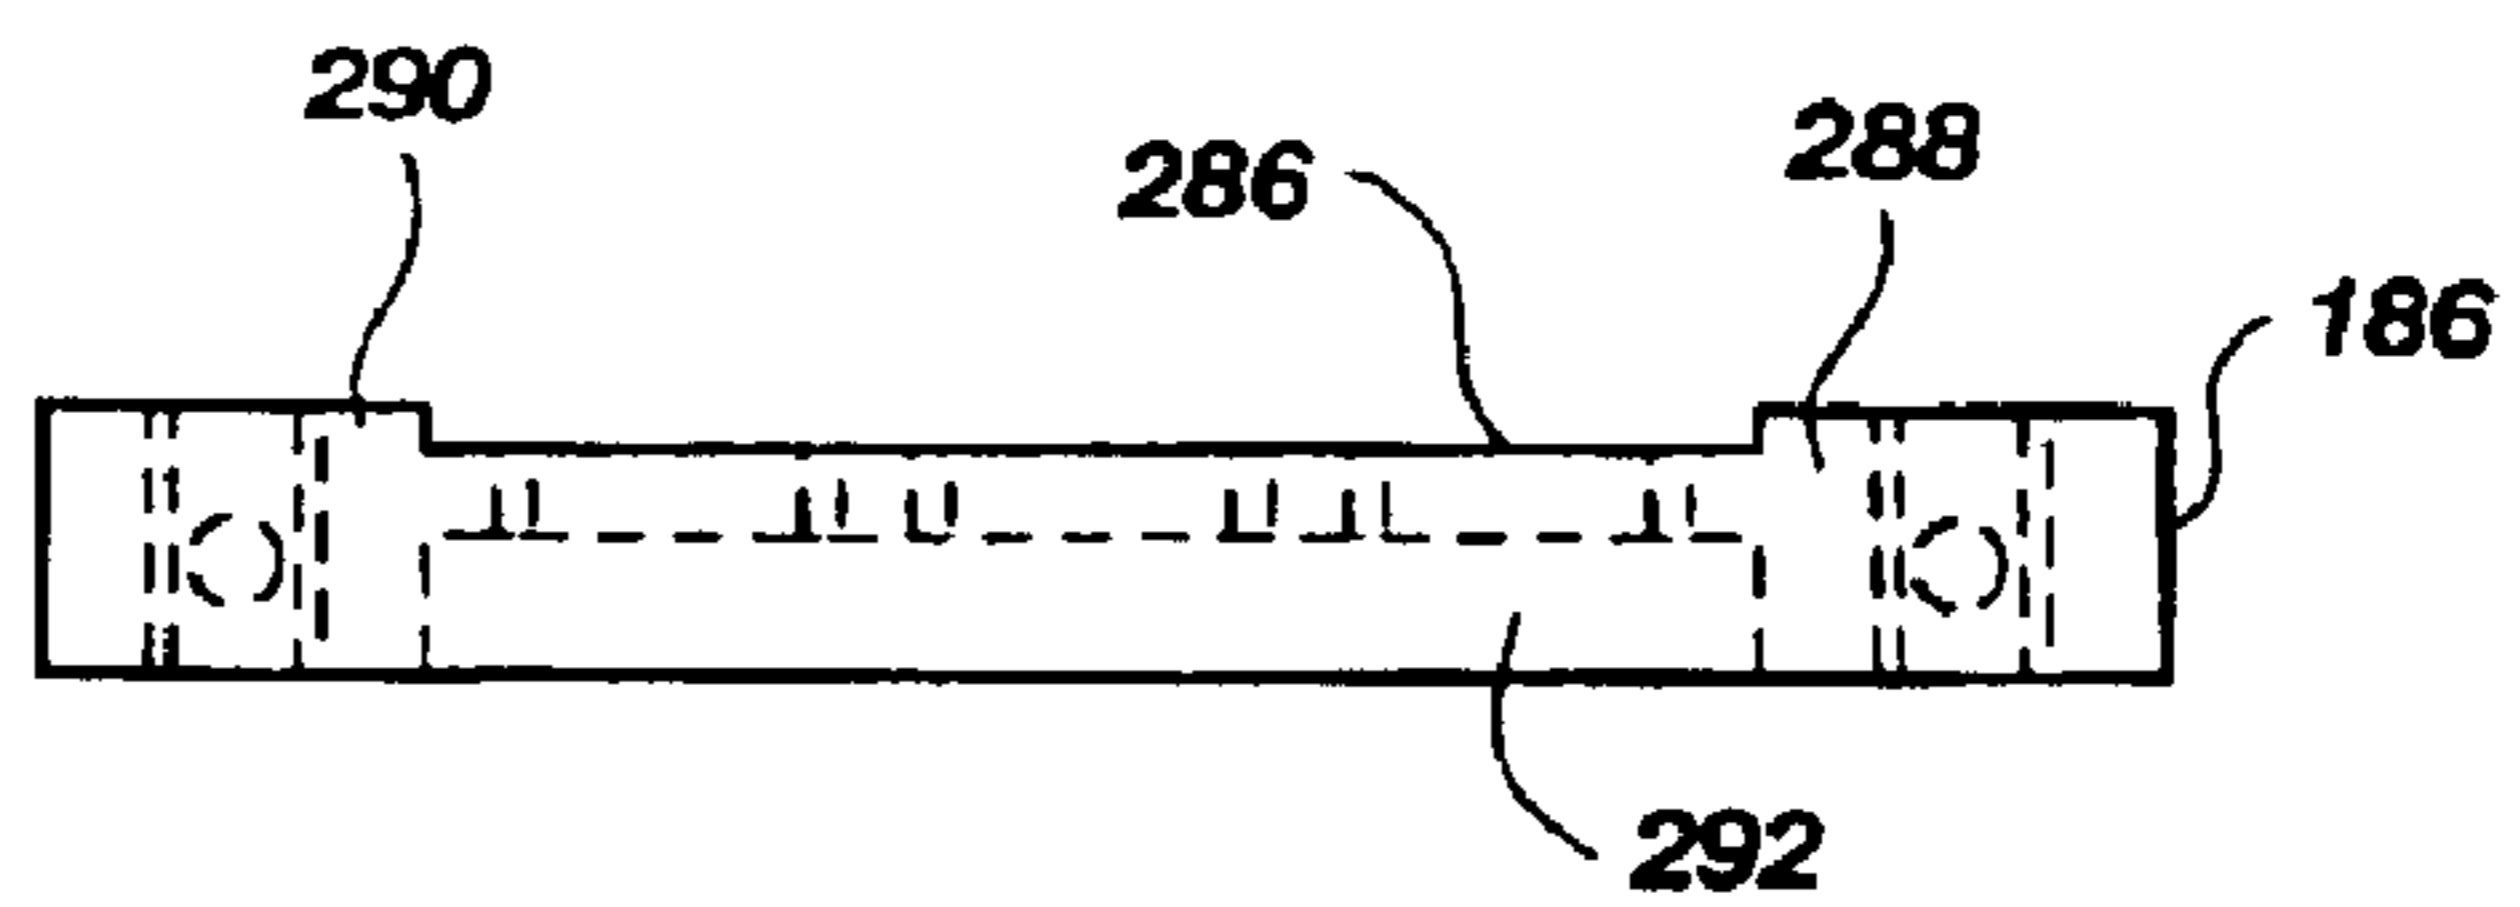


Fig. 13

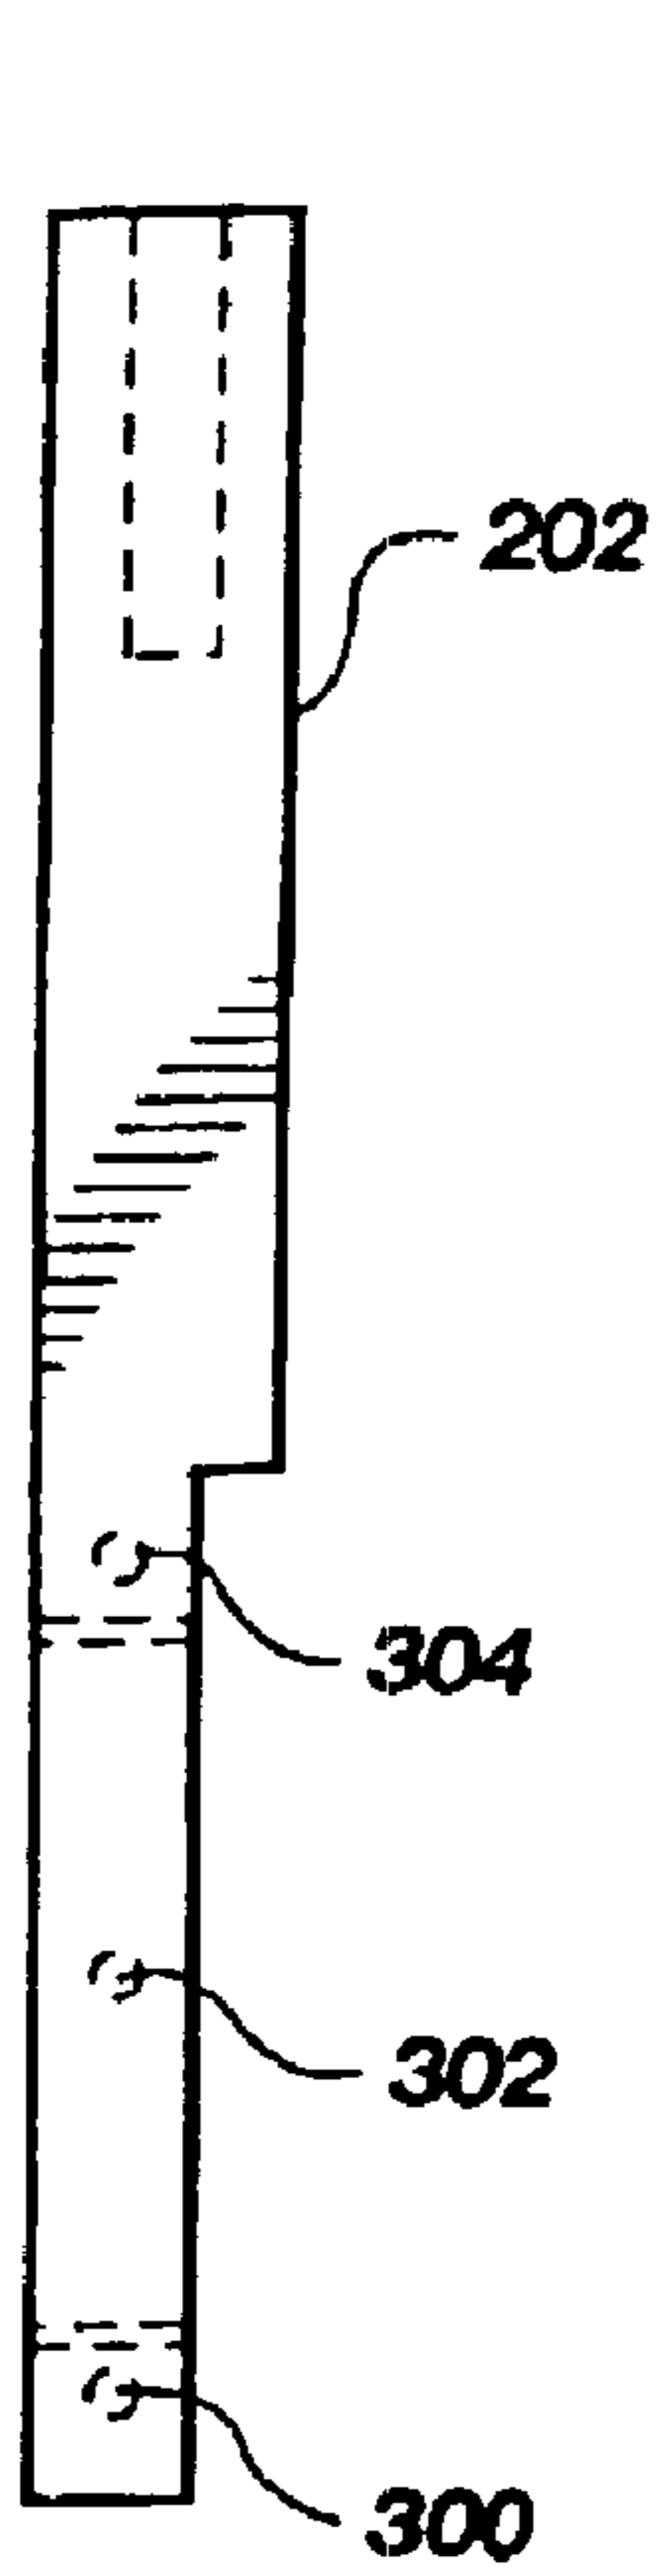


Fig. 16

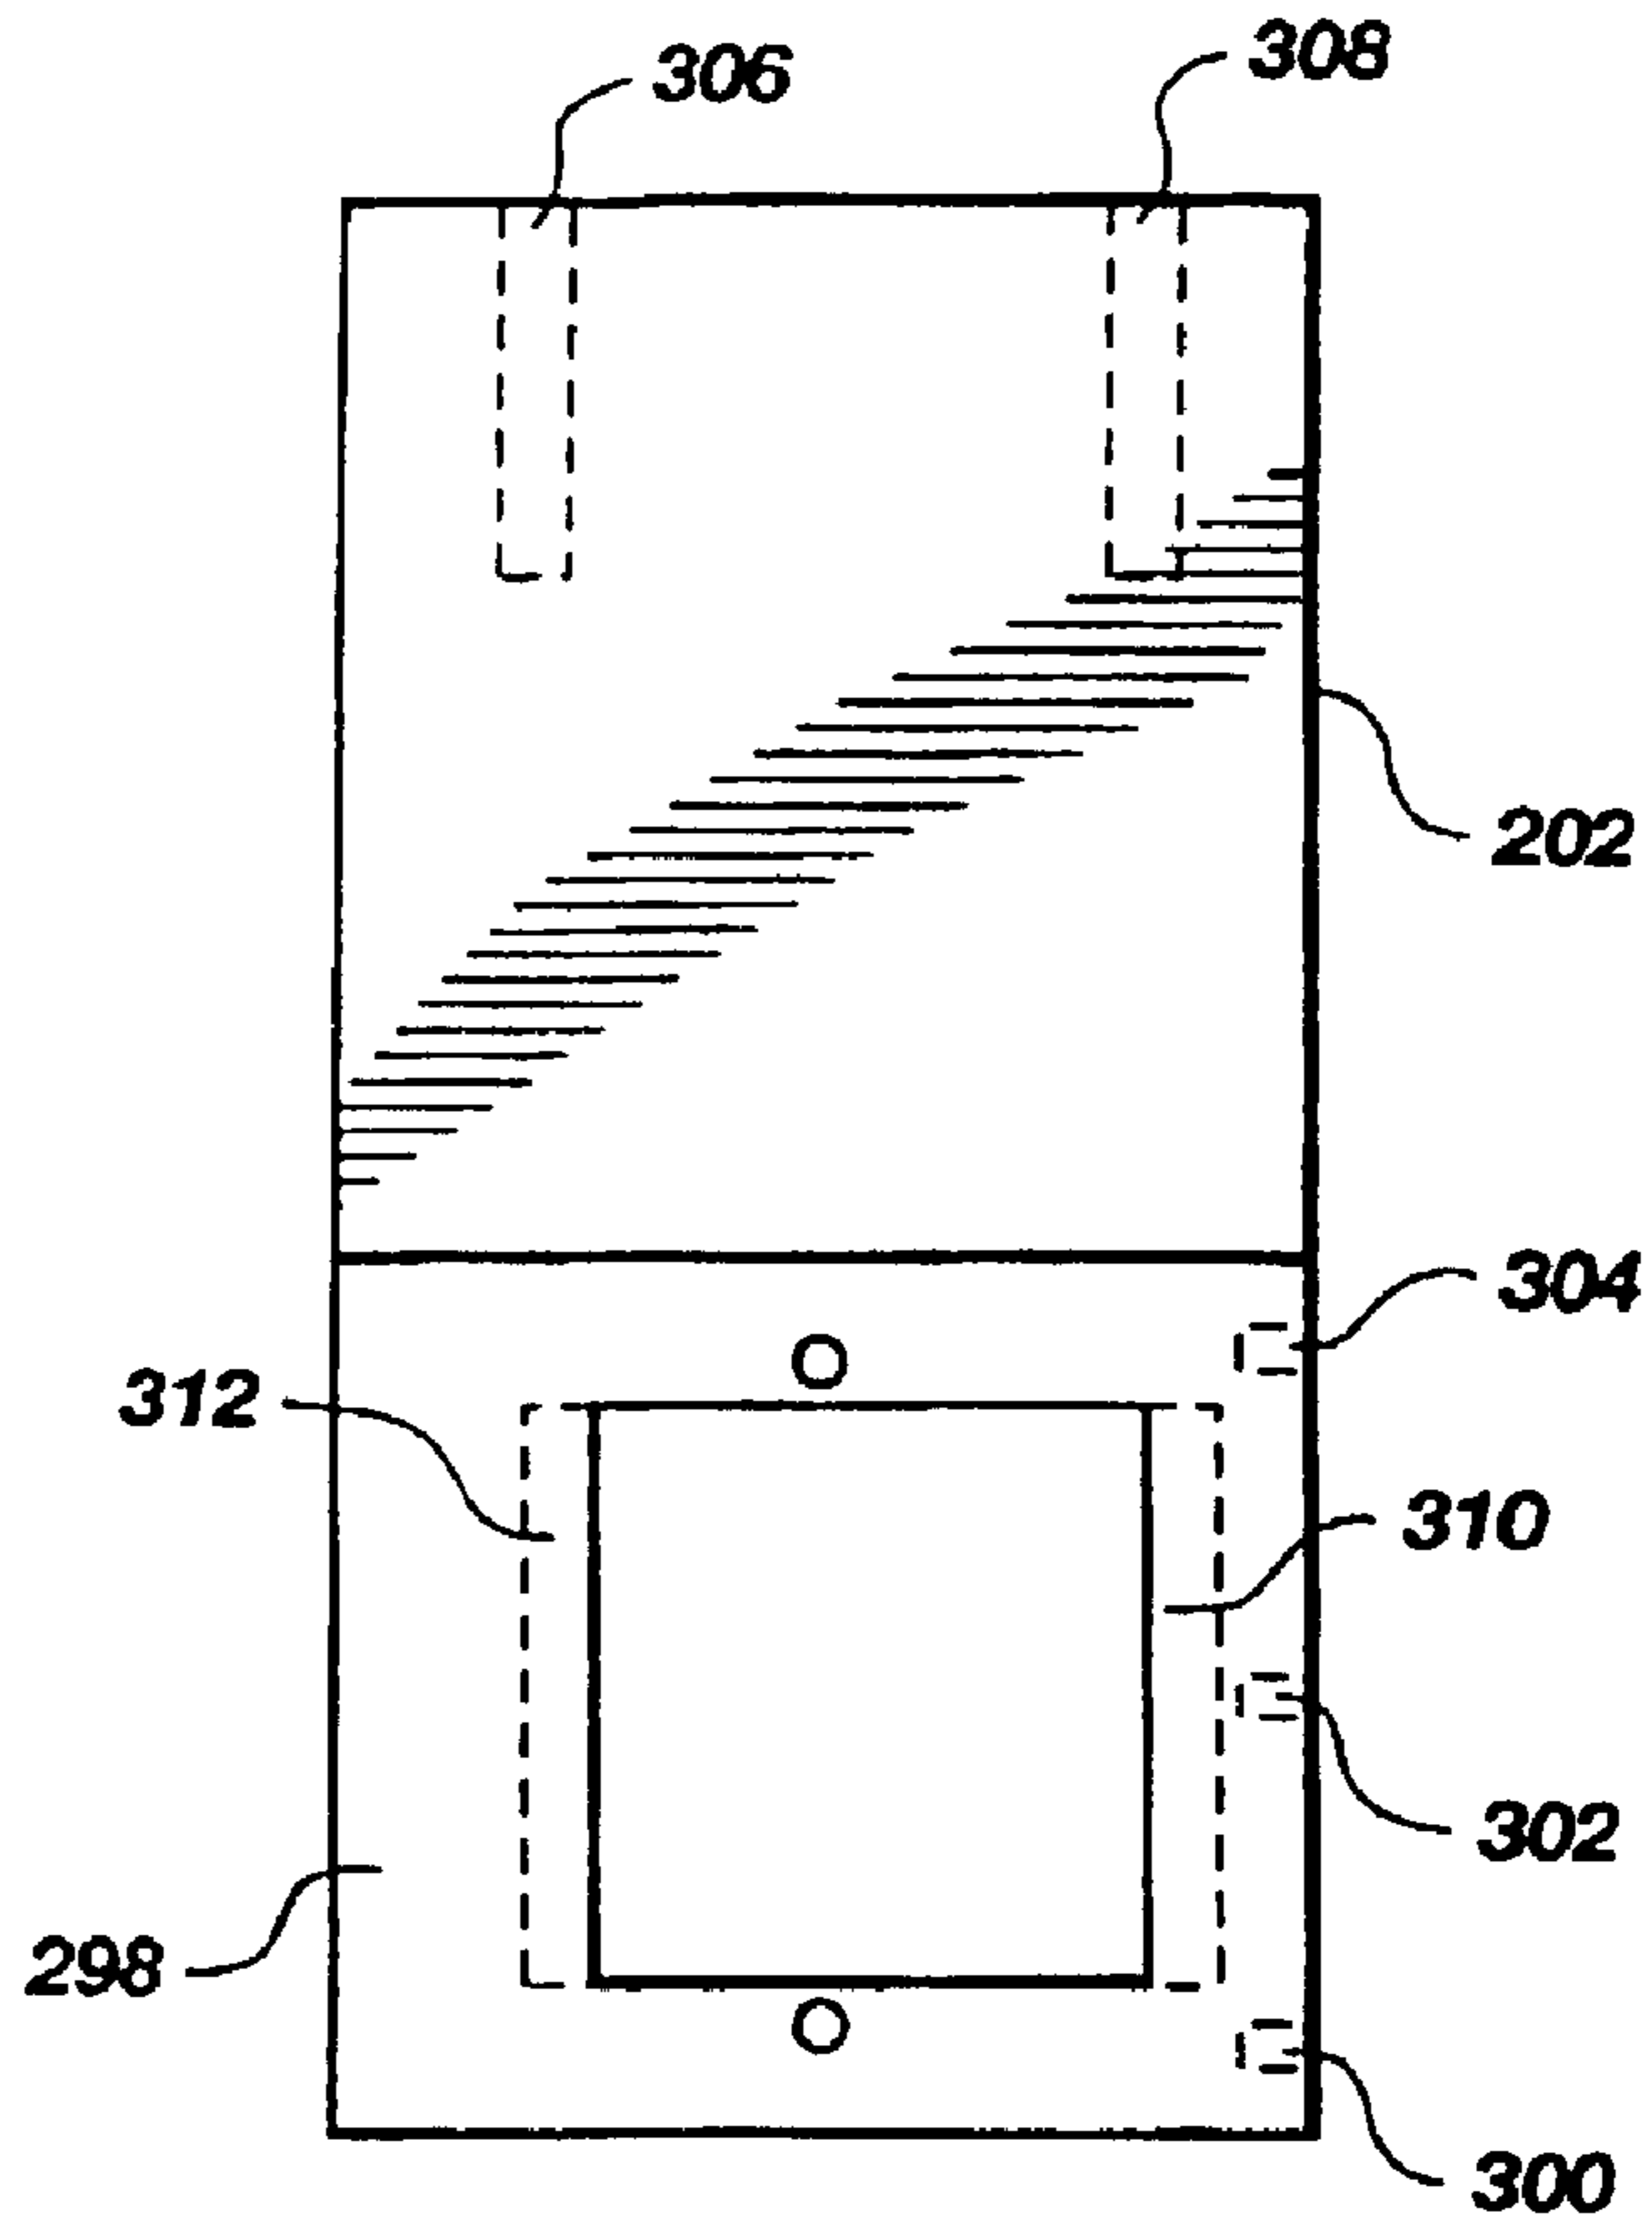


Fig. 15

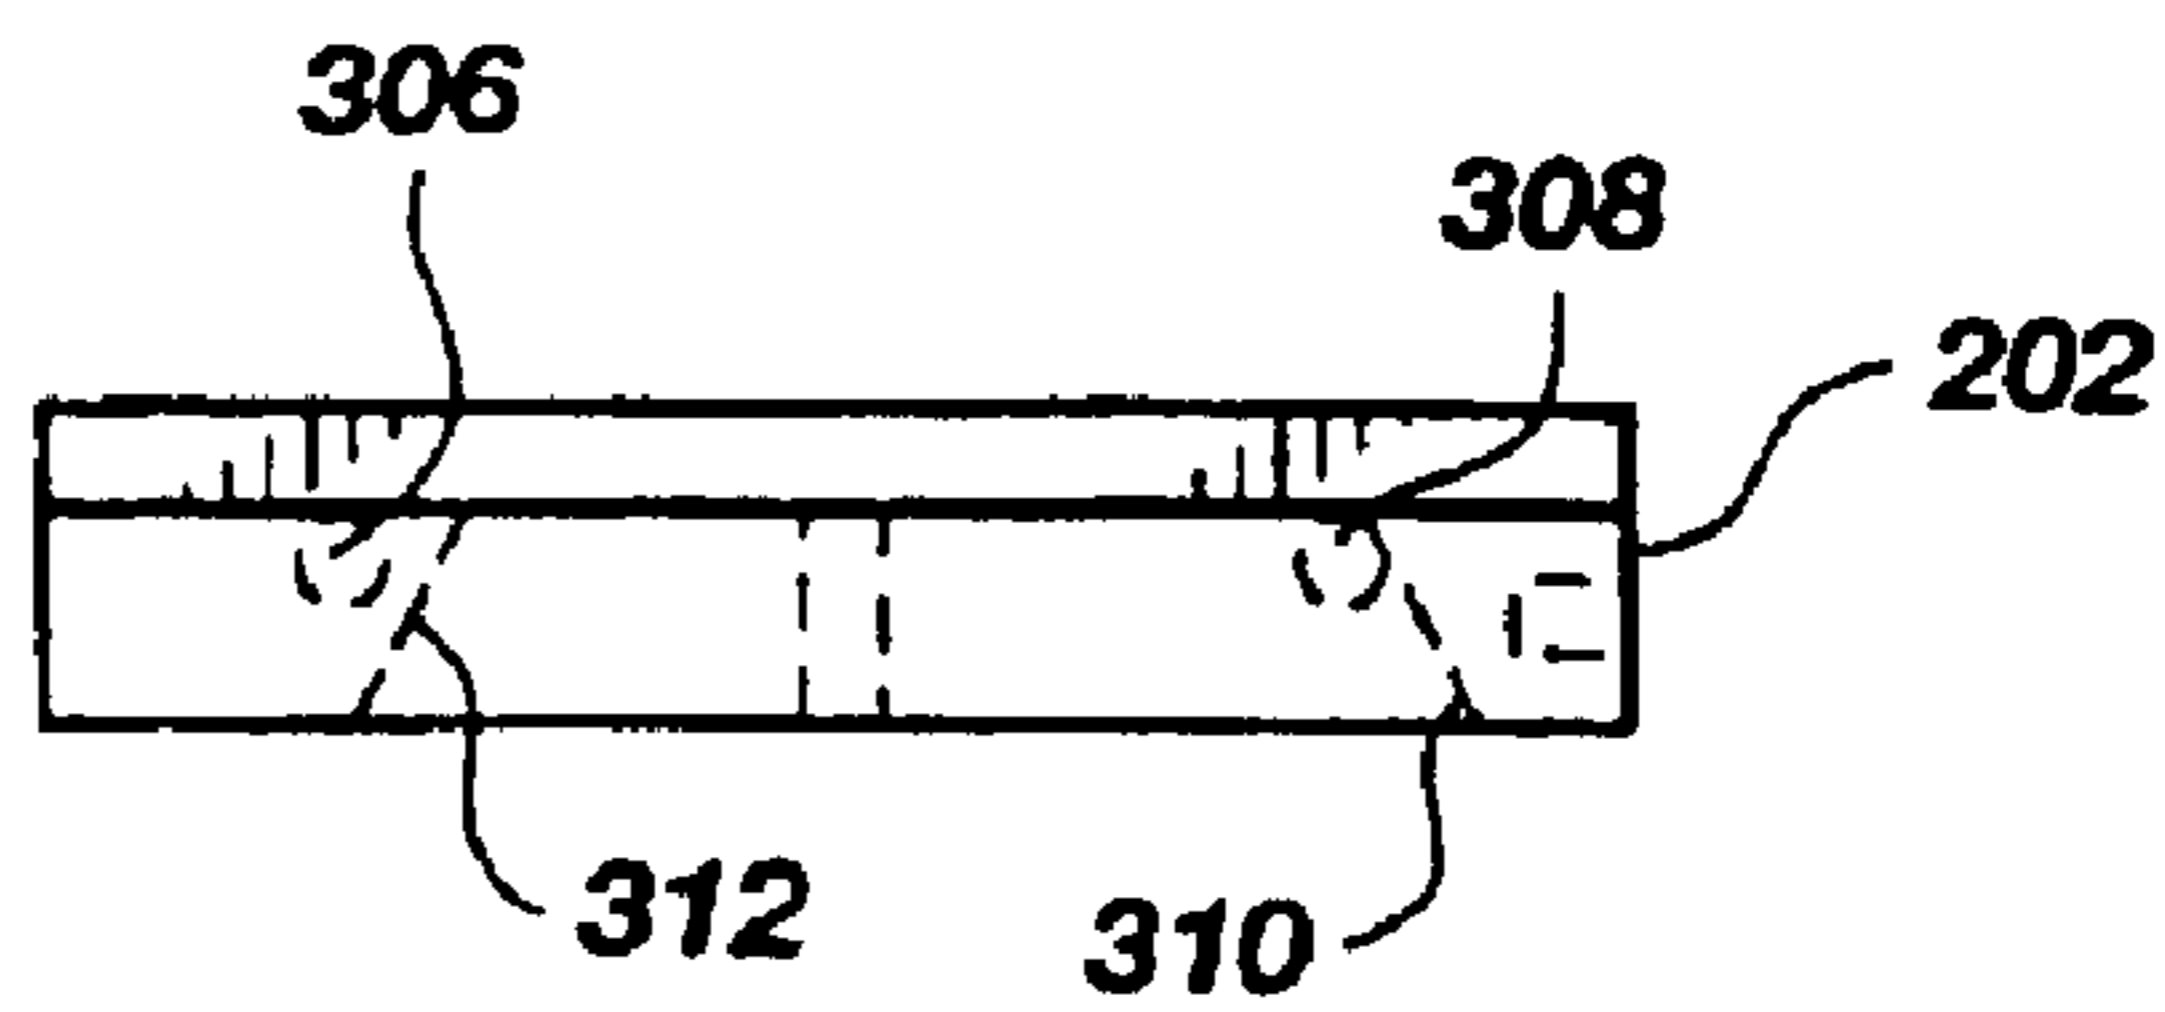


Fig. 17

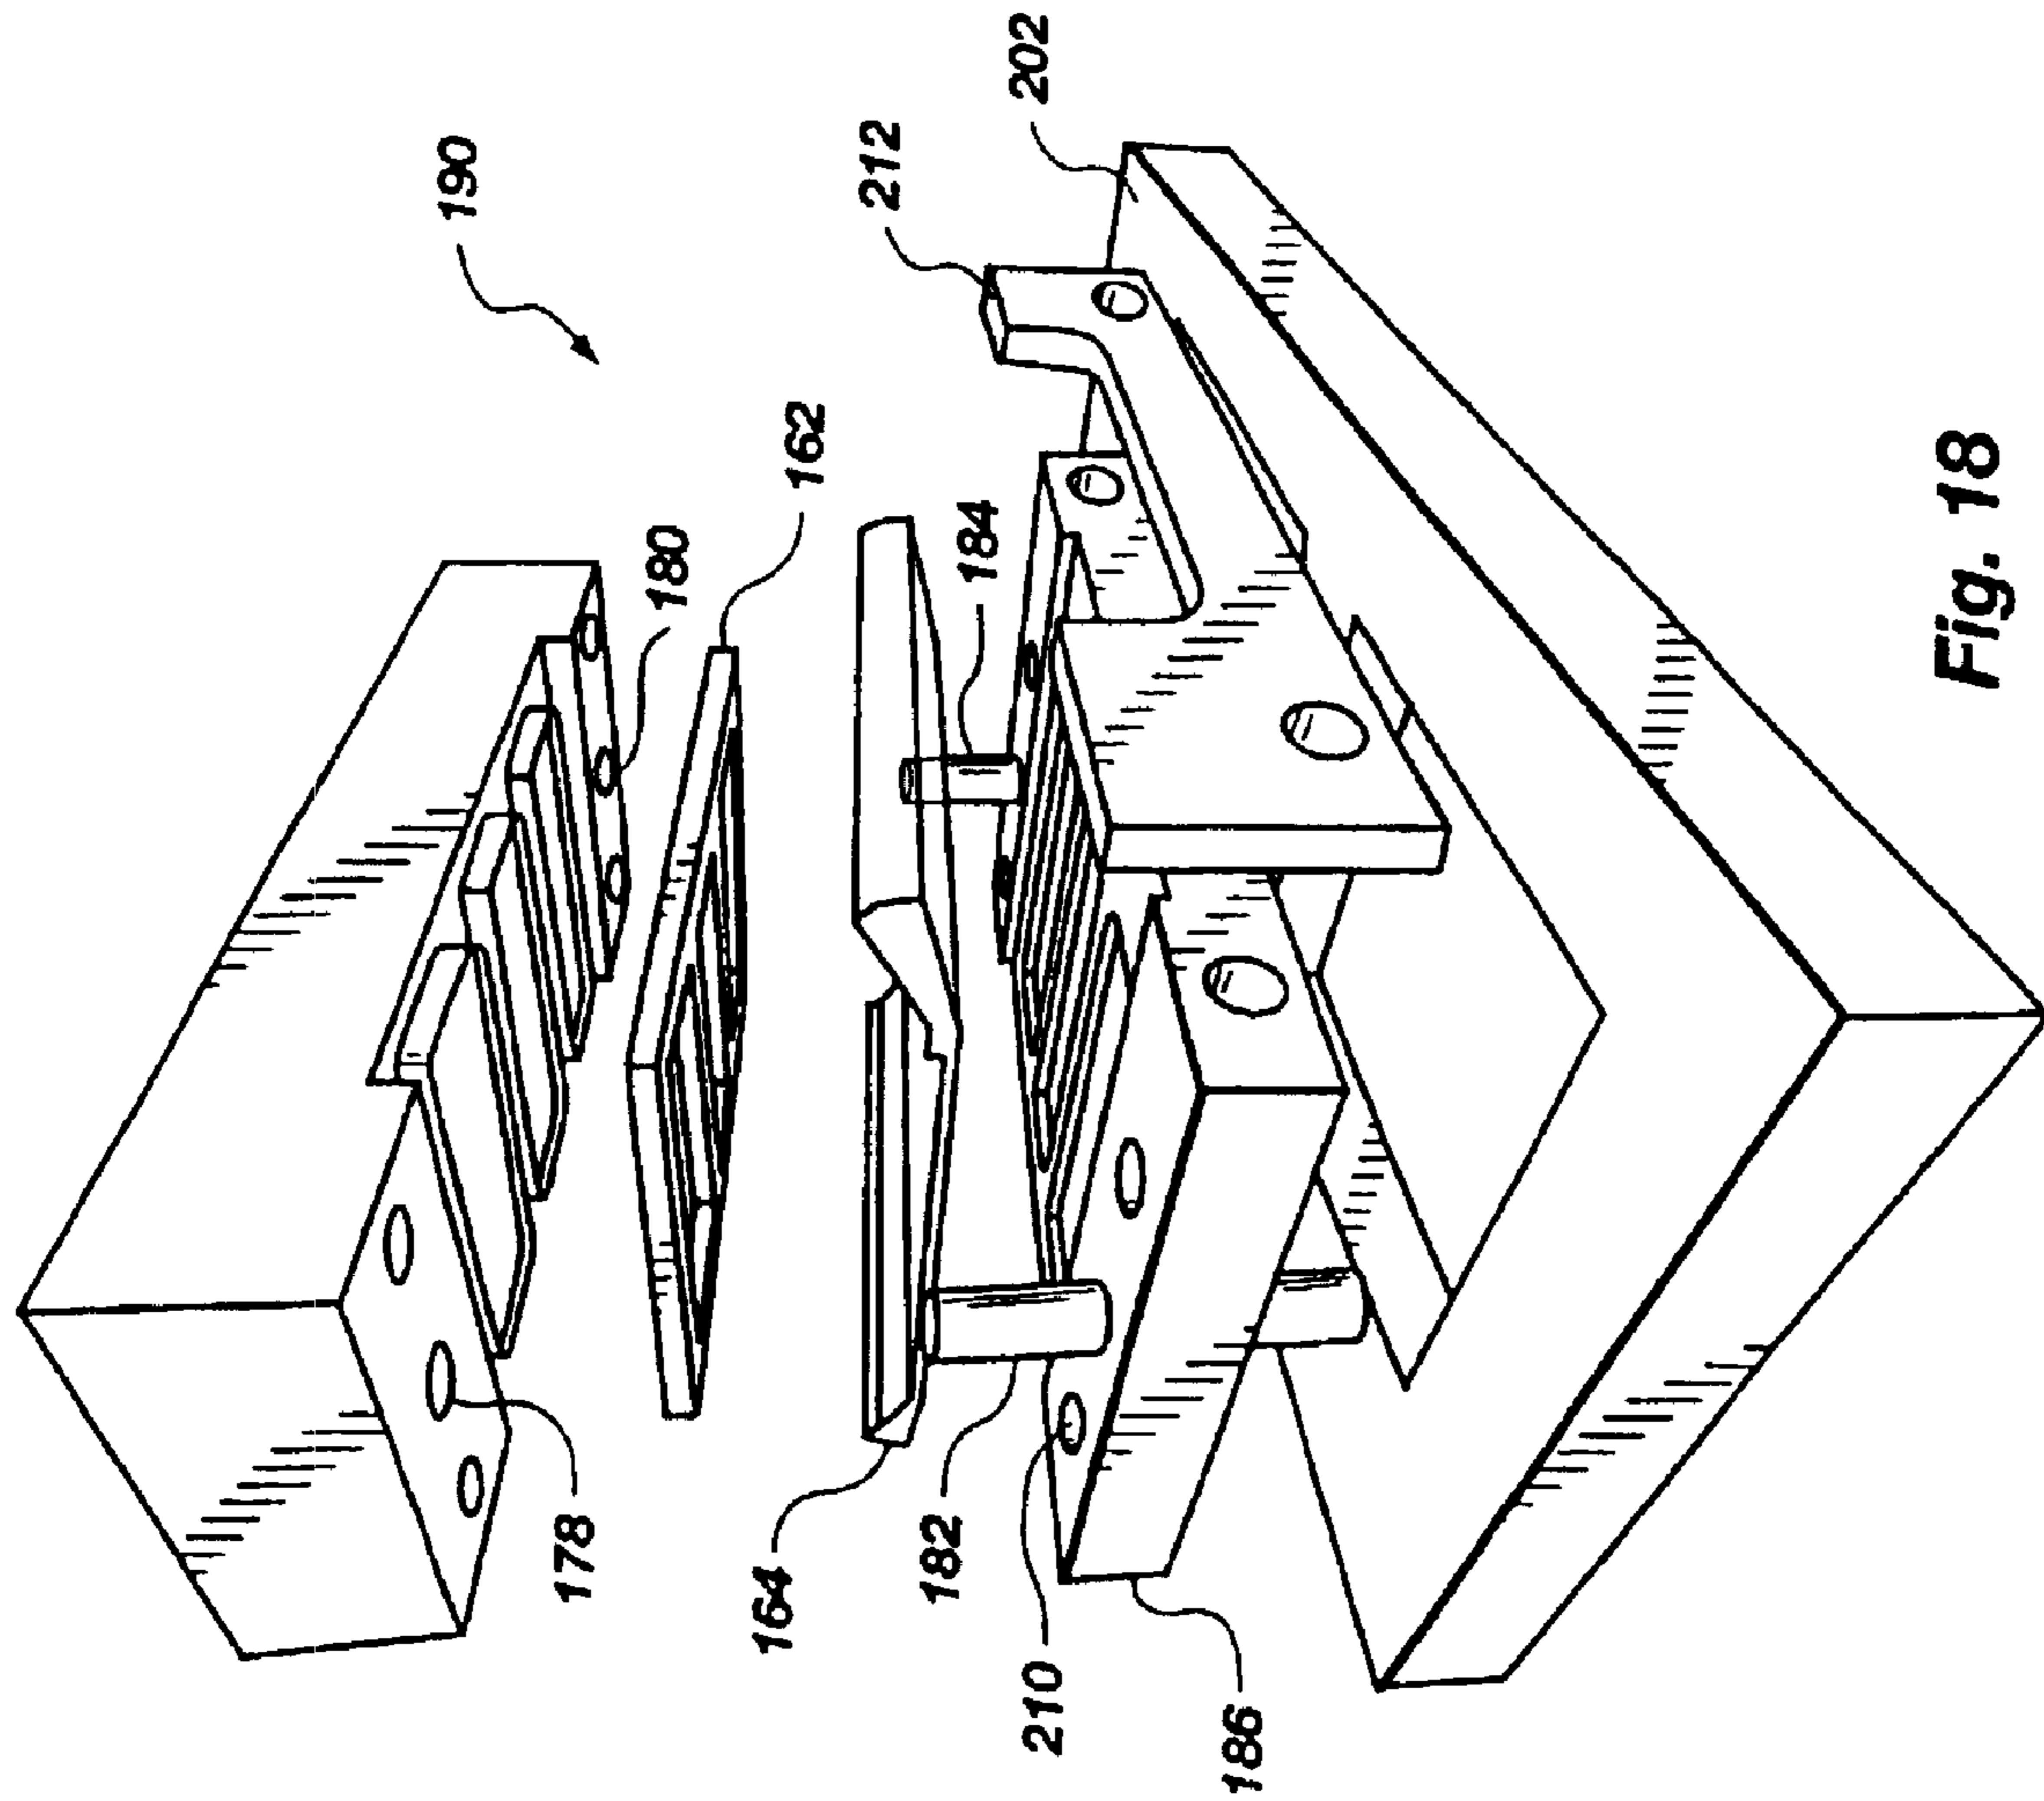


Fig. 18

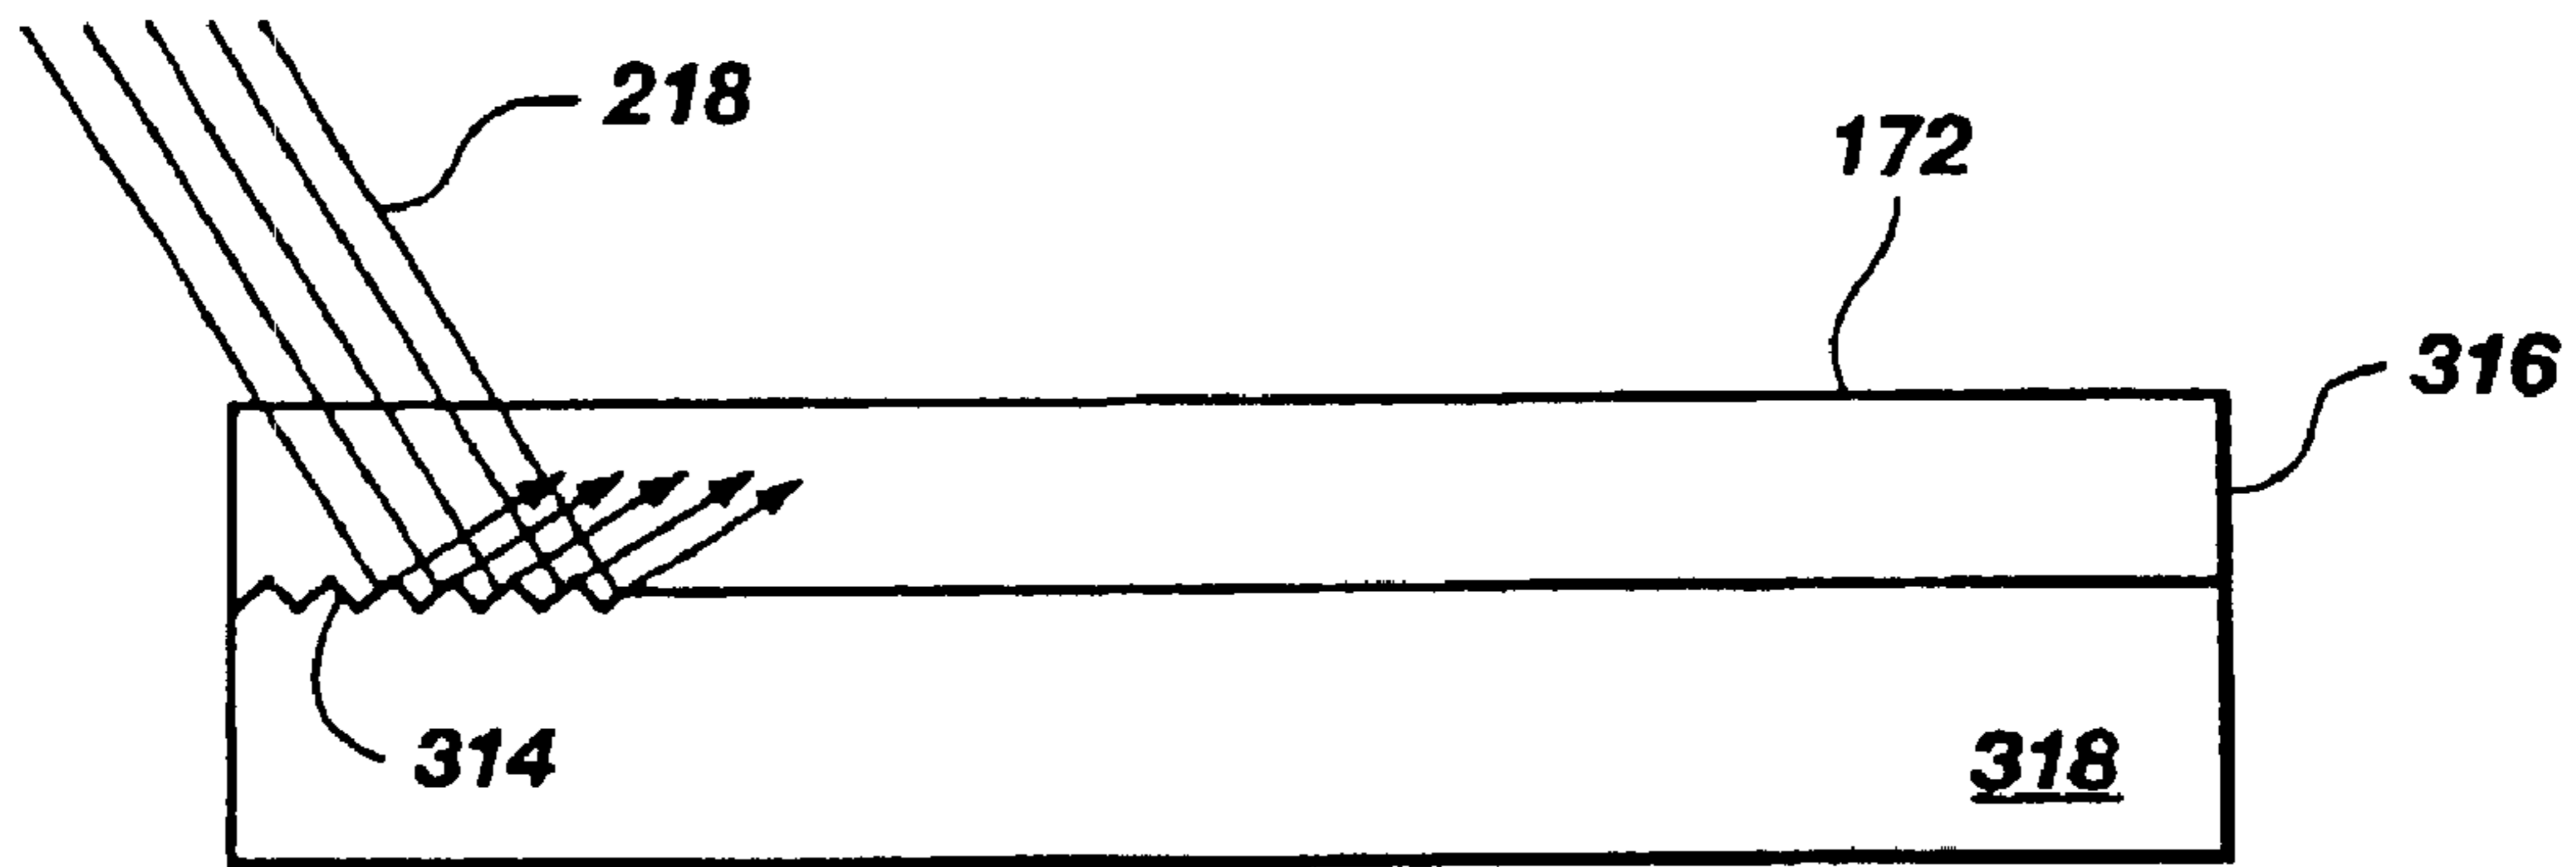


Fig. 19

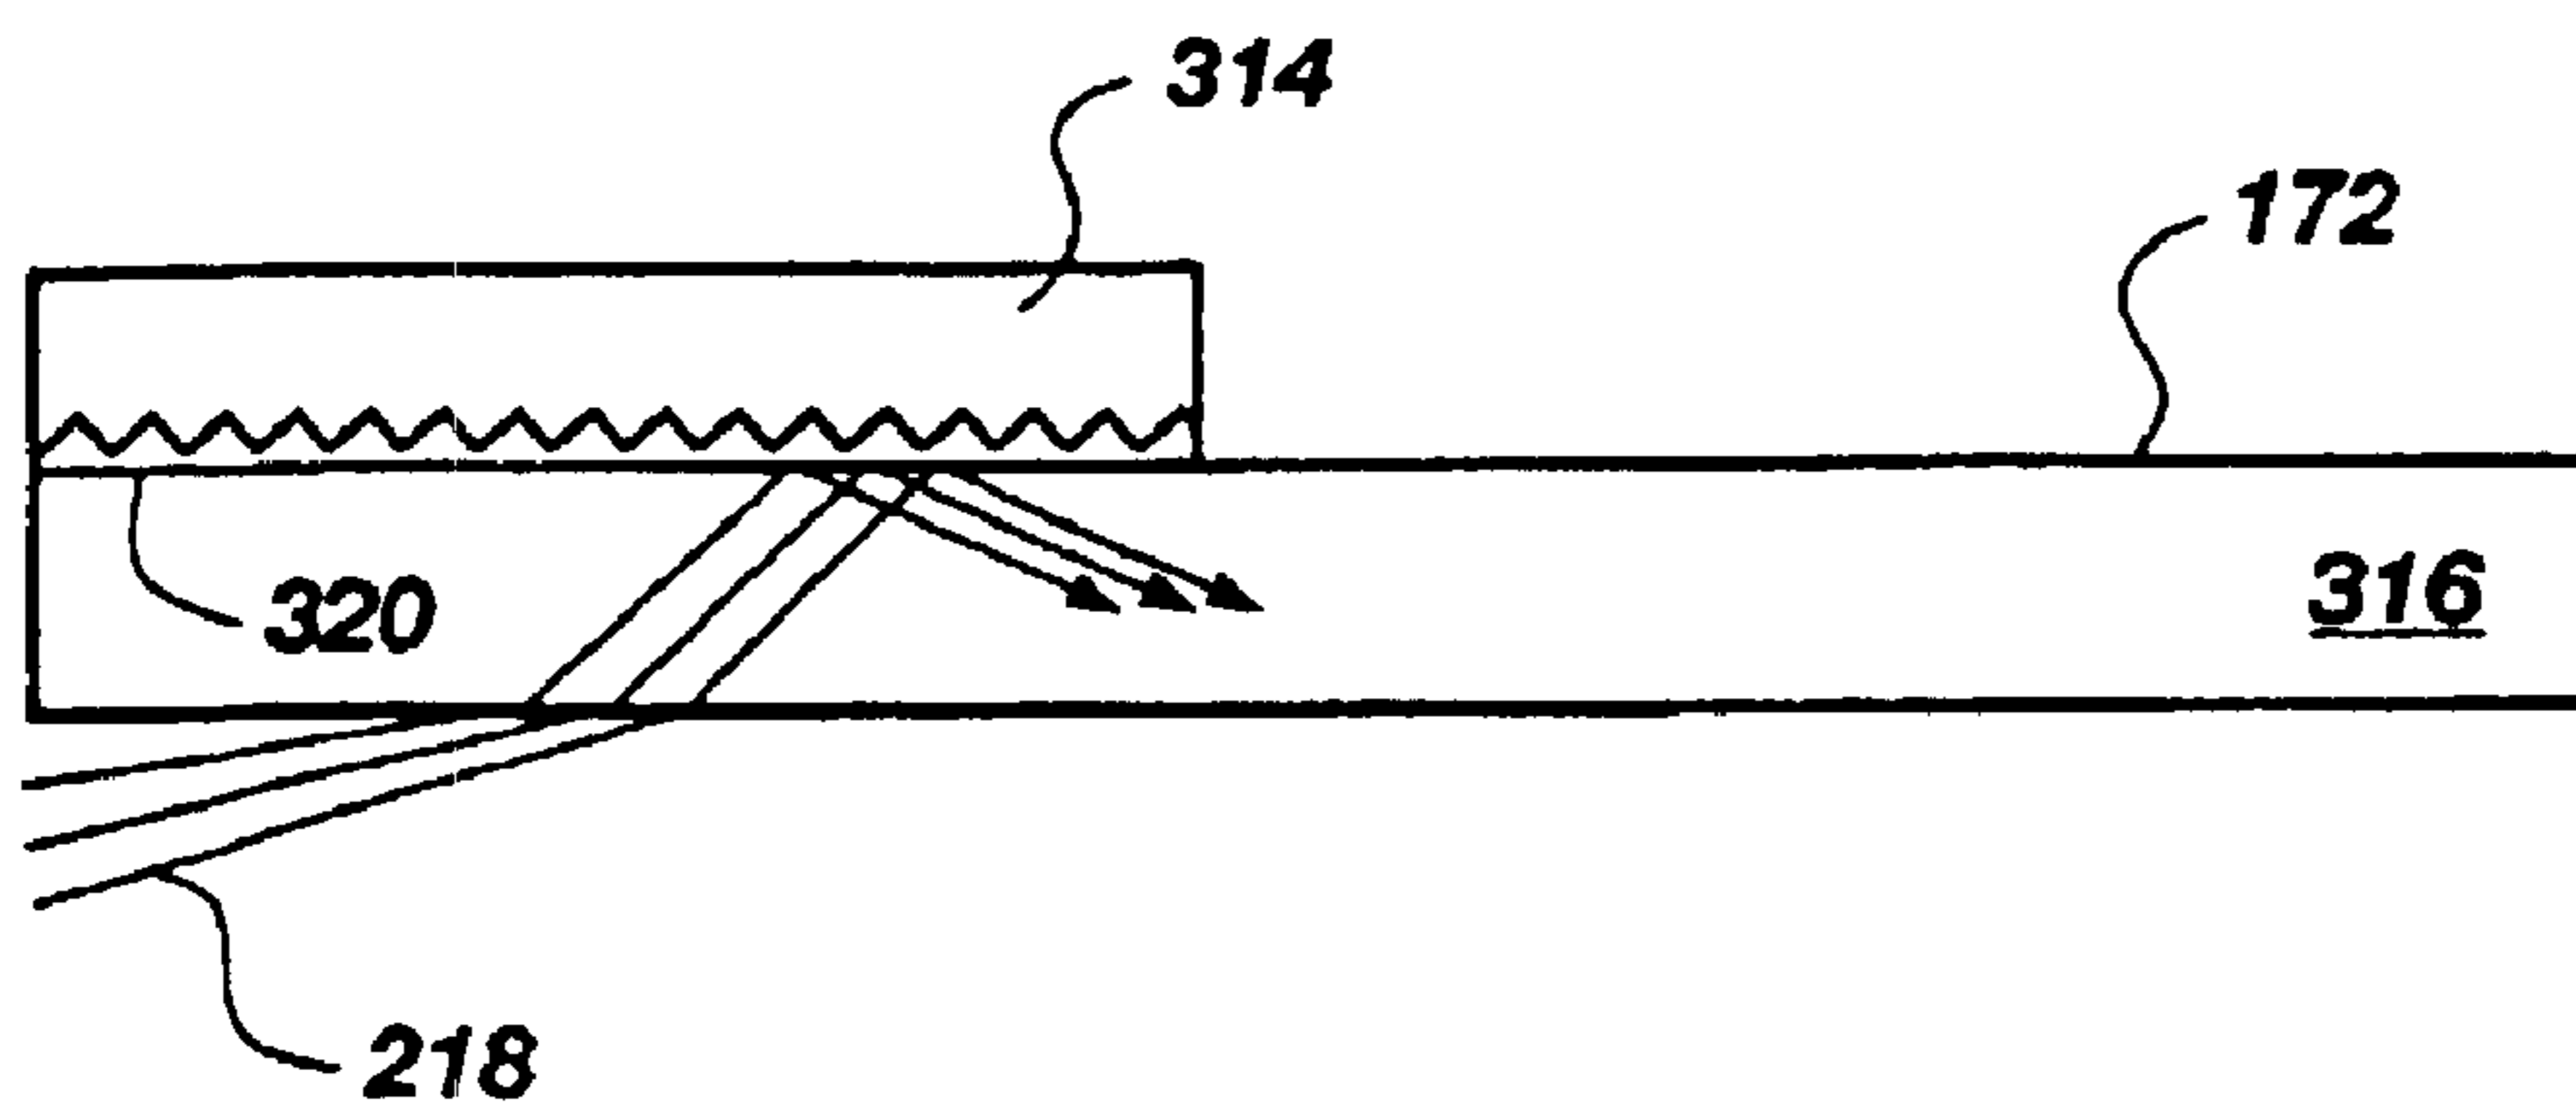


Fig. 20

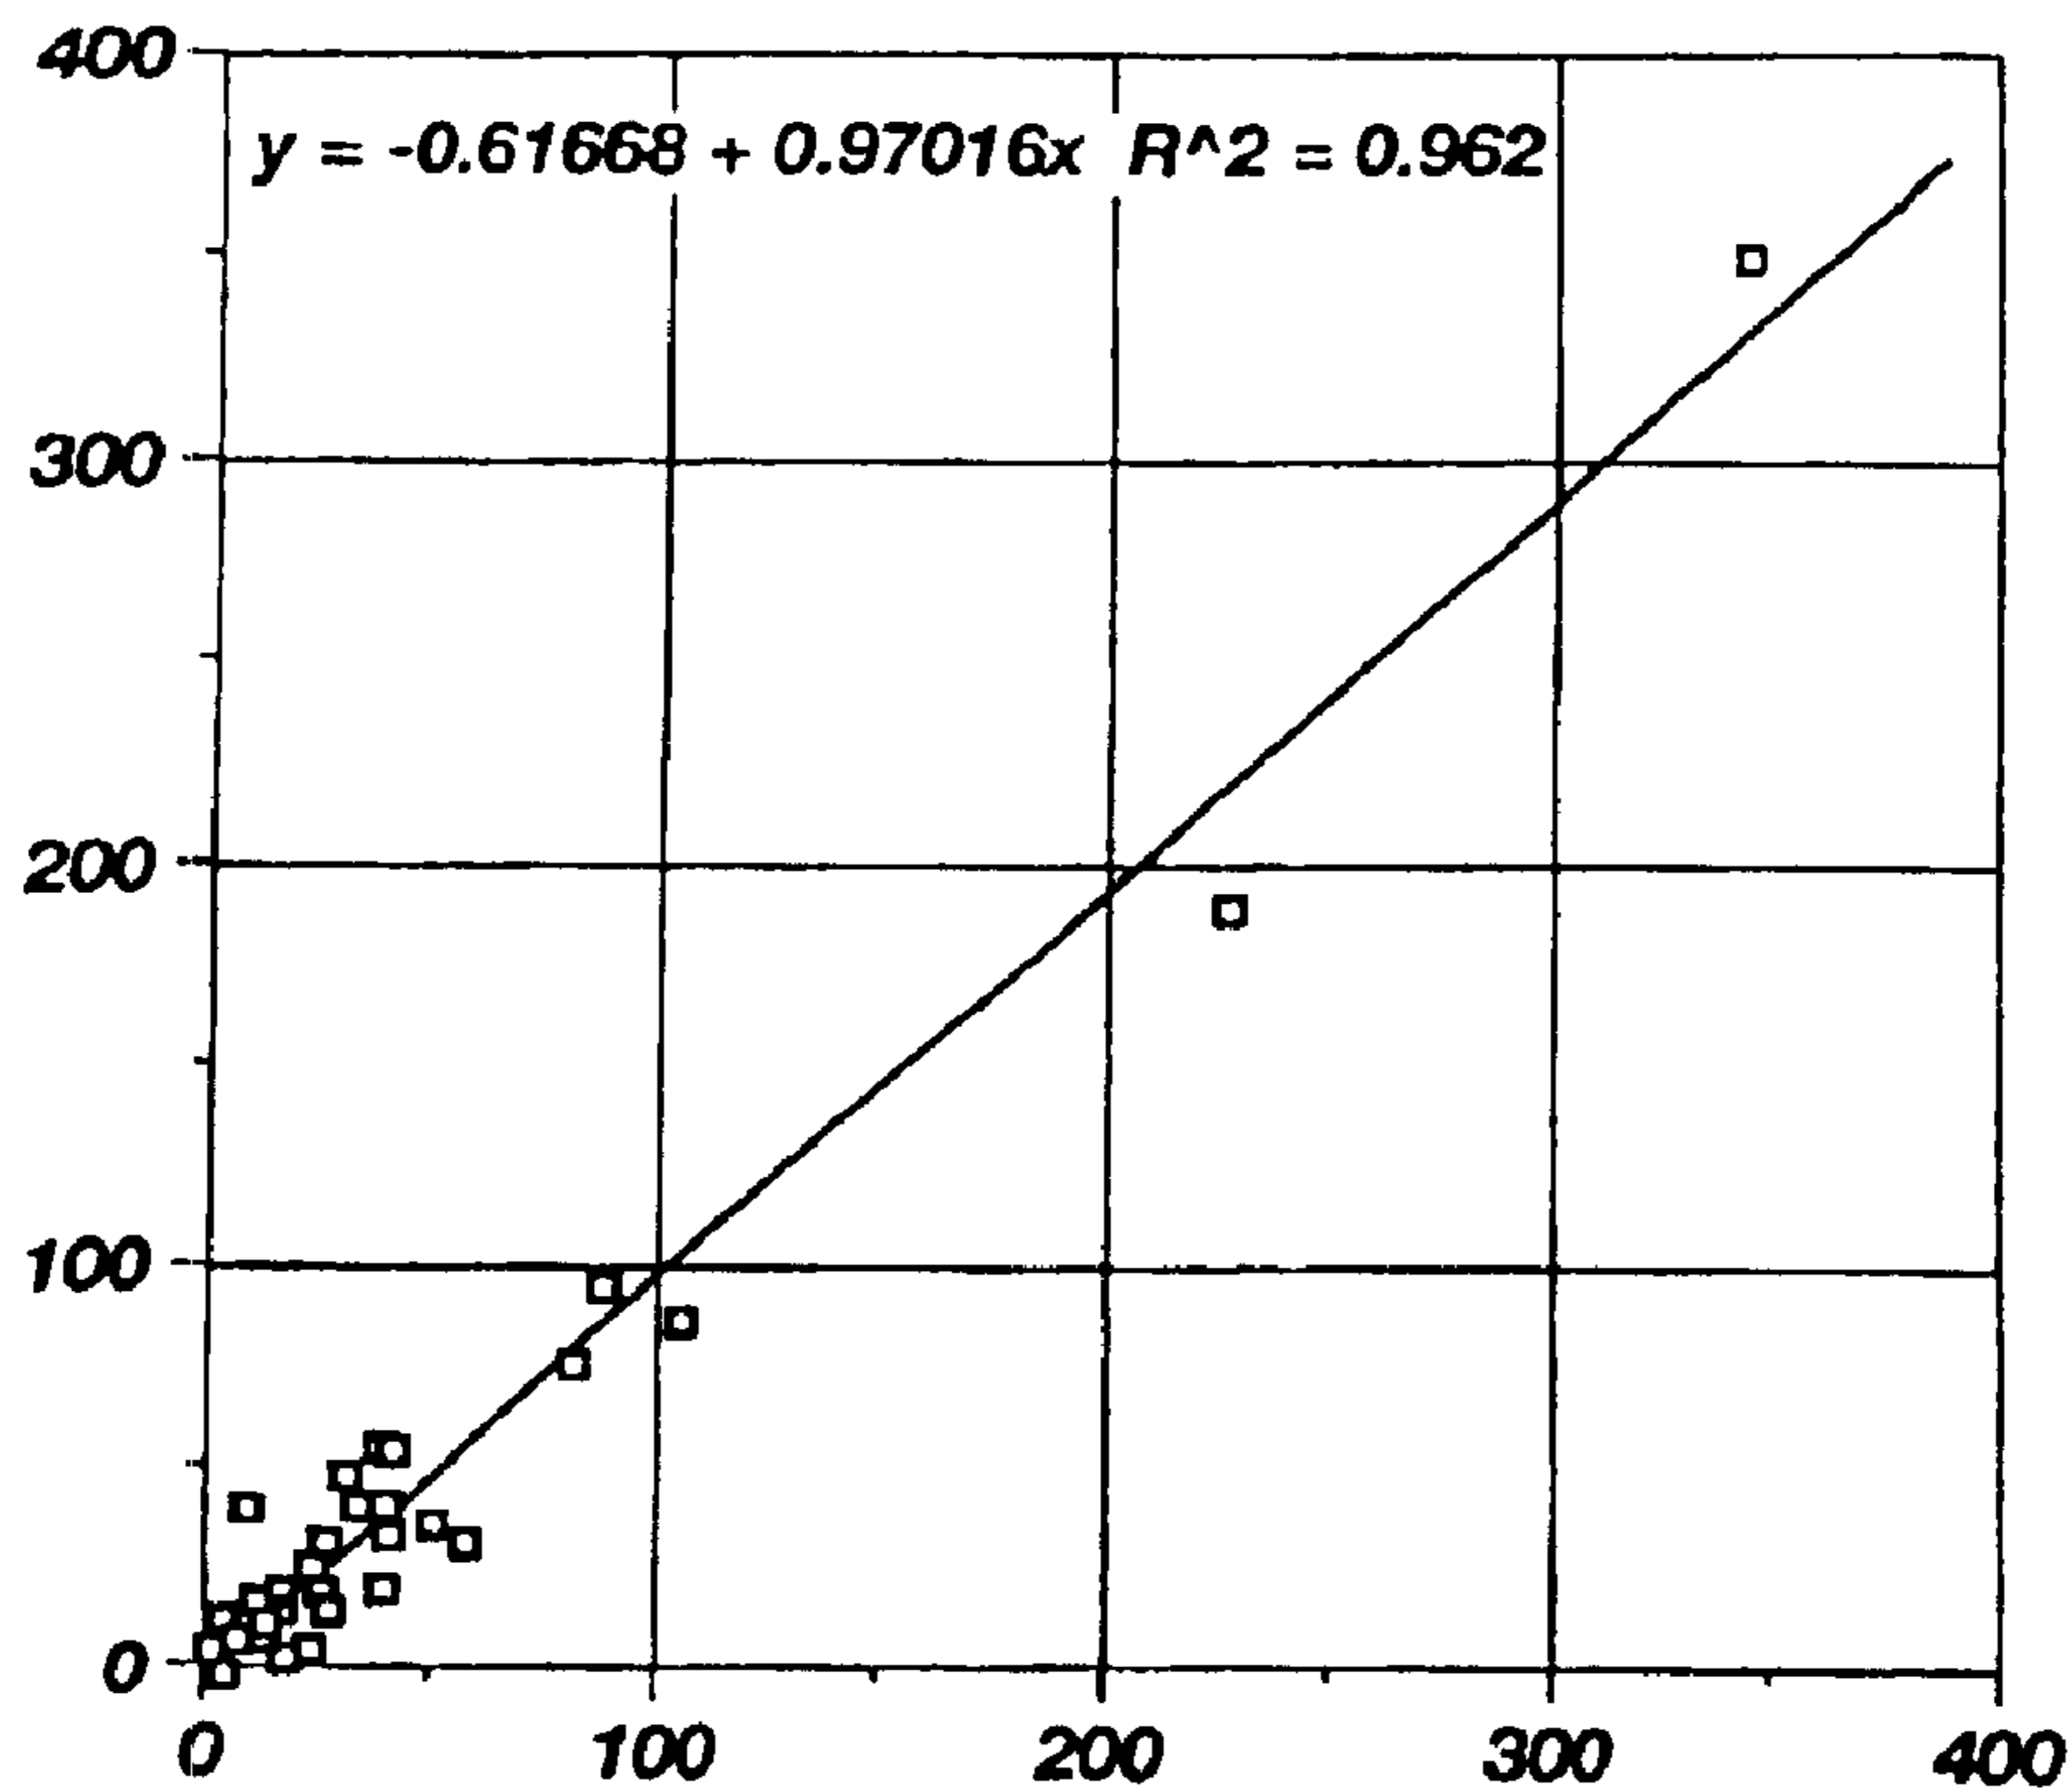


Fig. 21

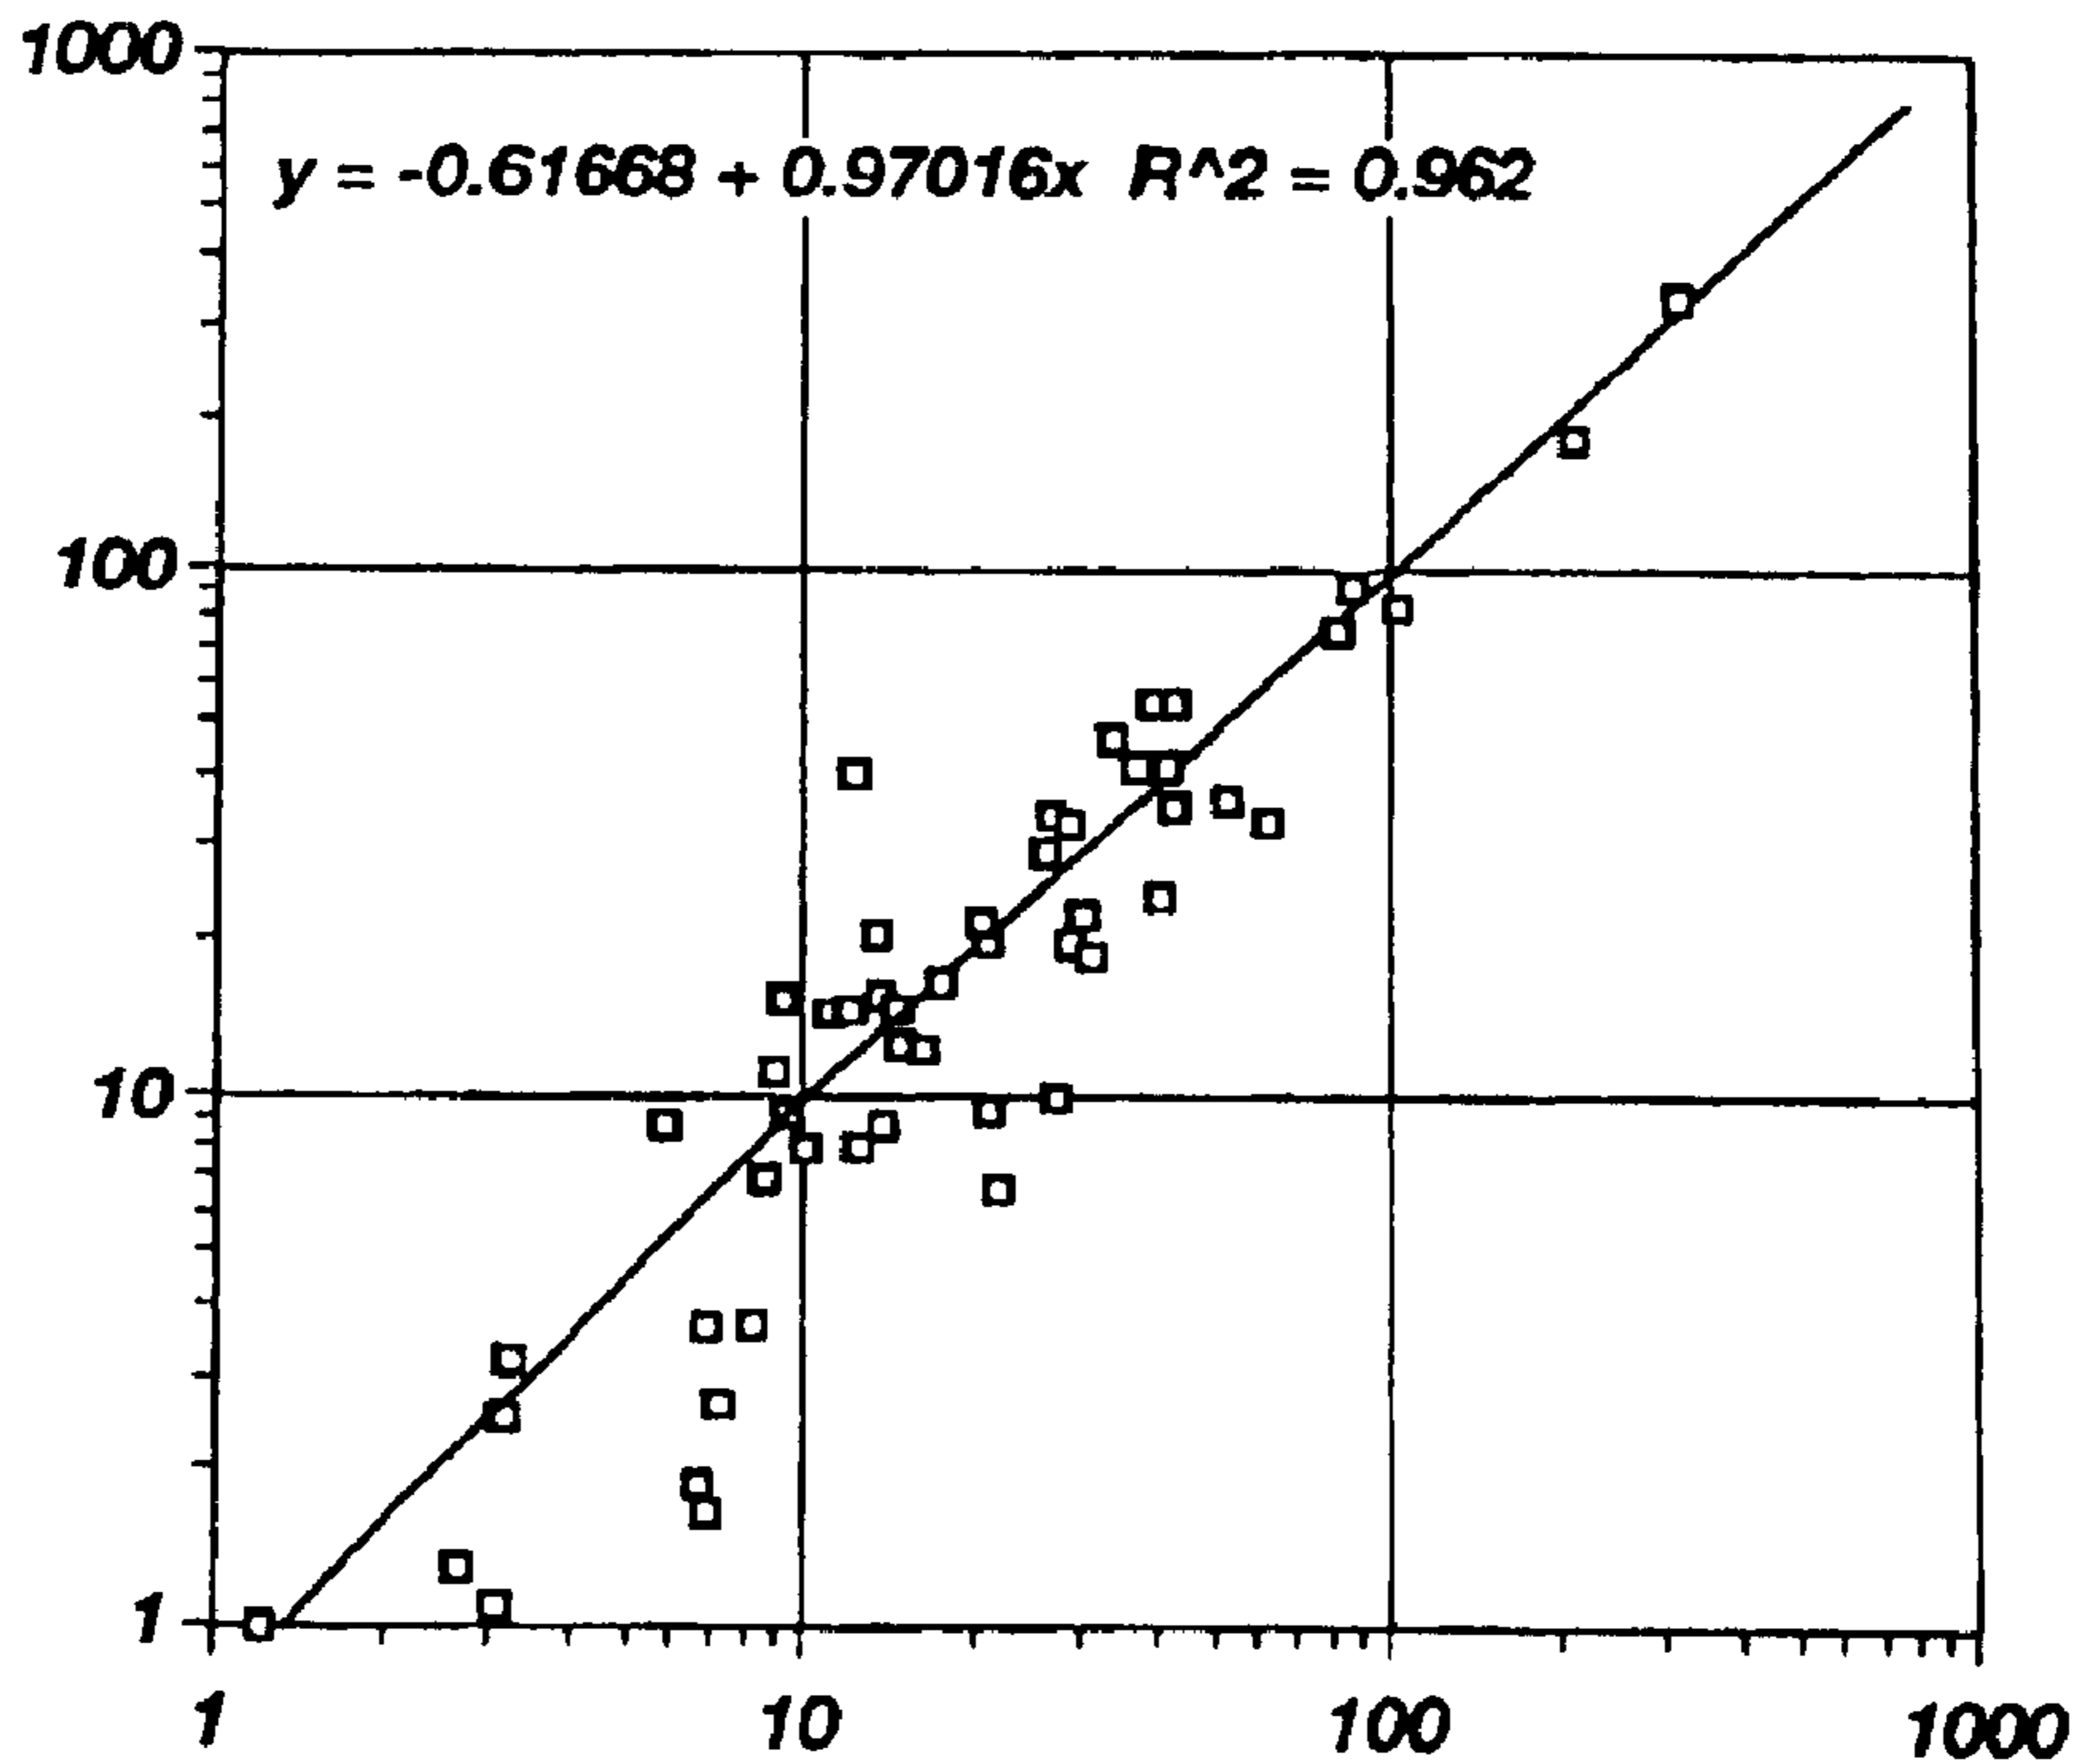


Fig. 22

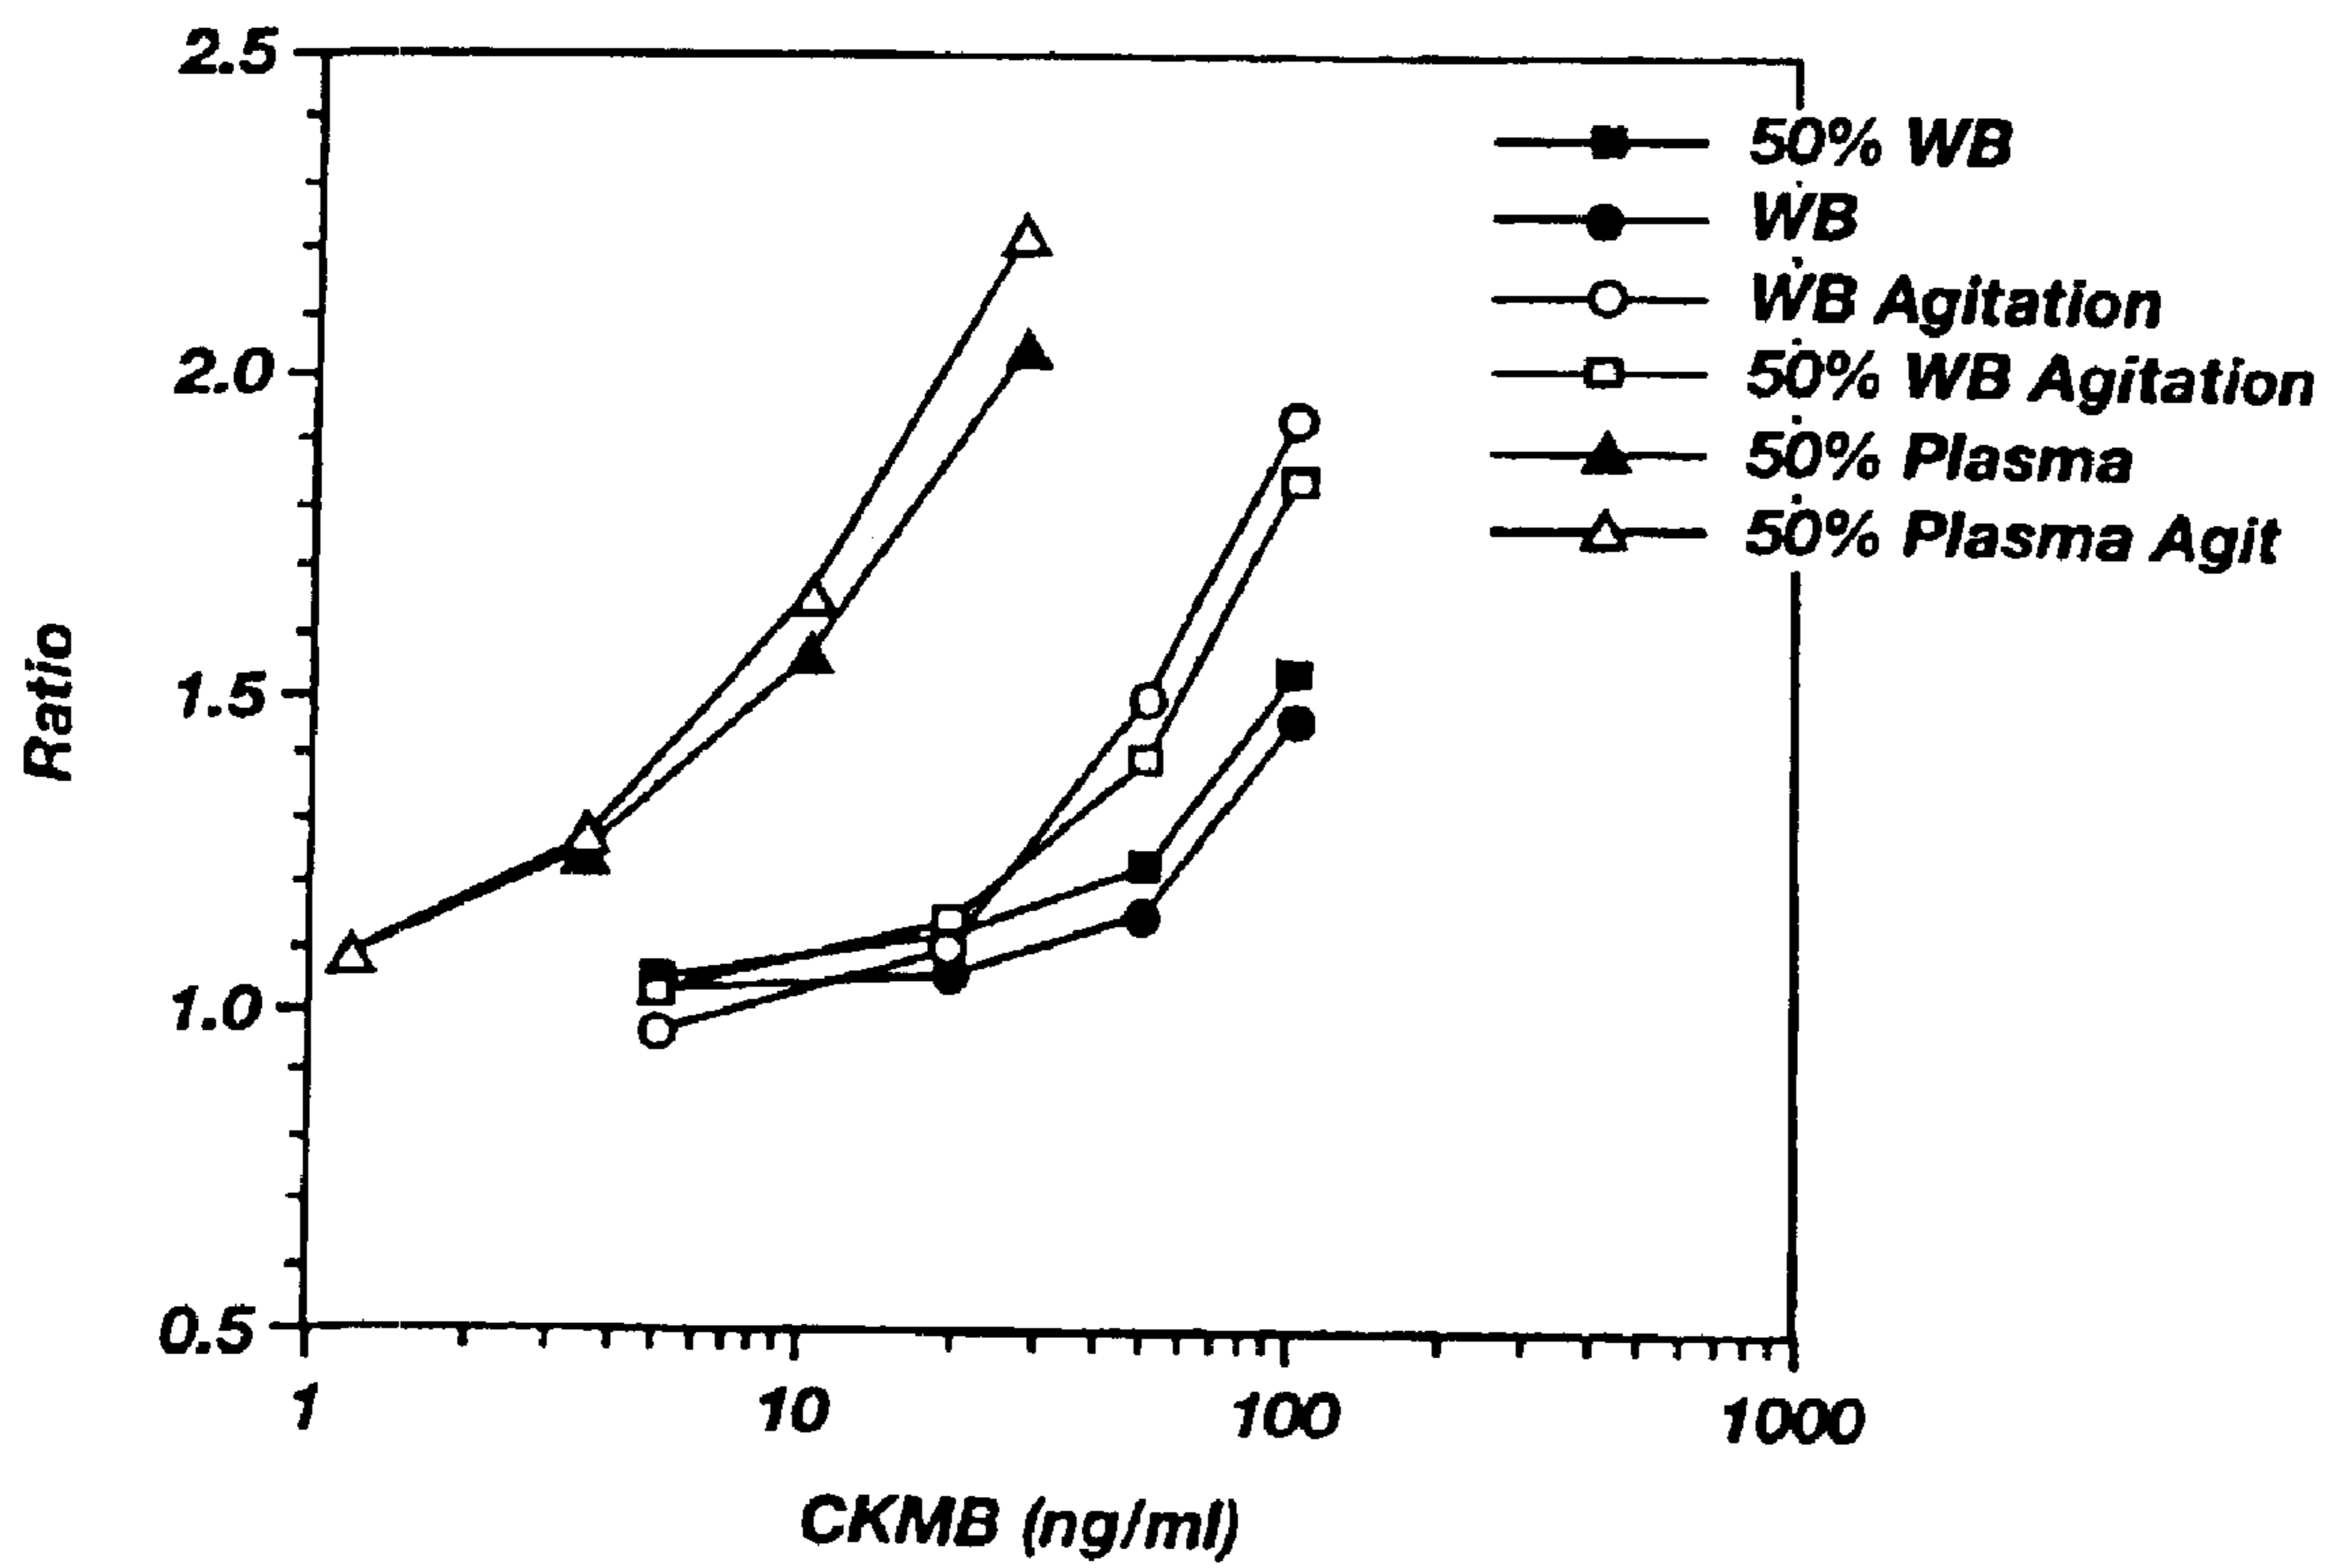


Fig. 23

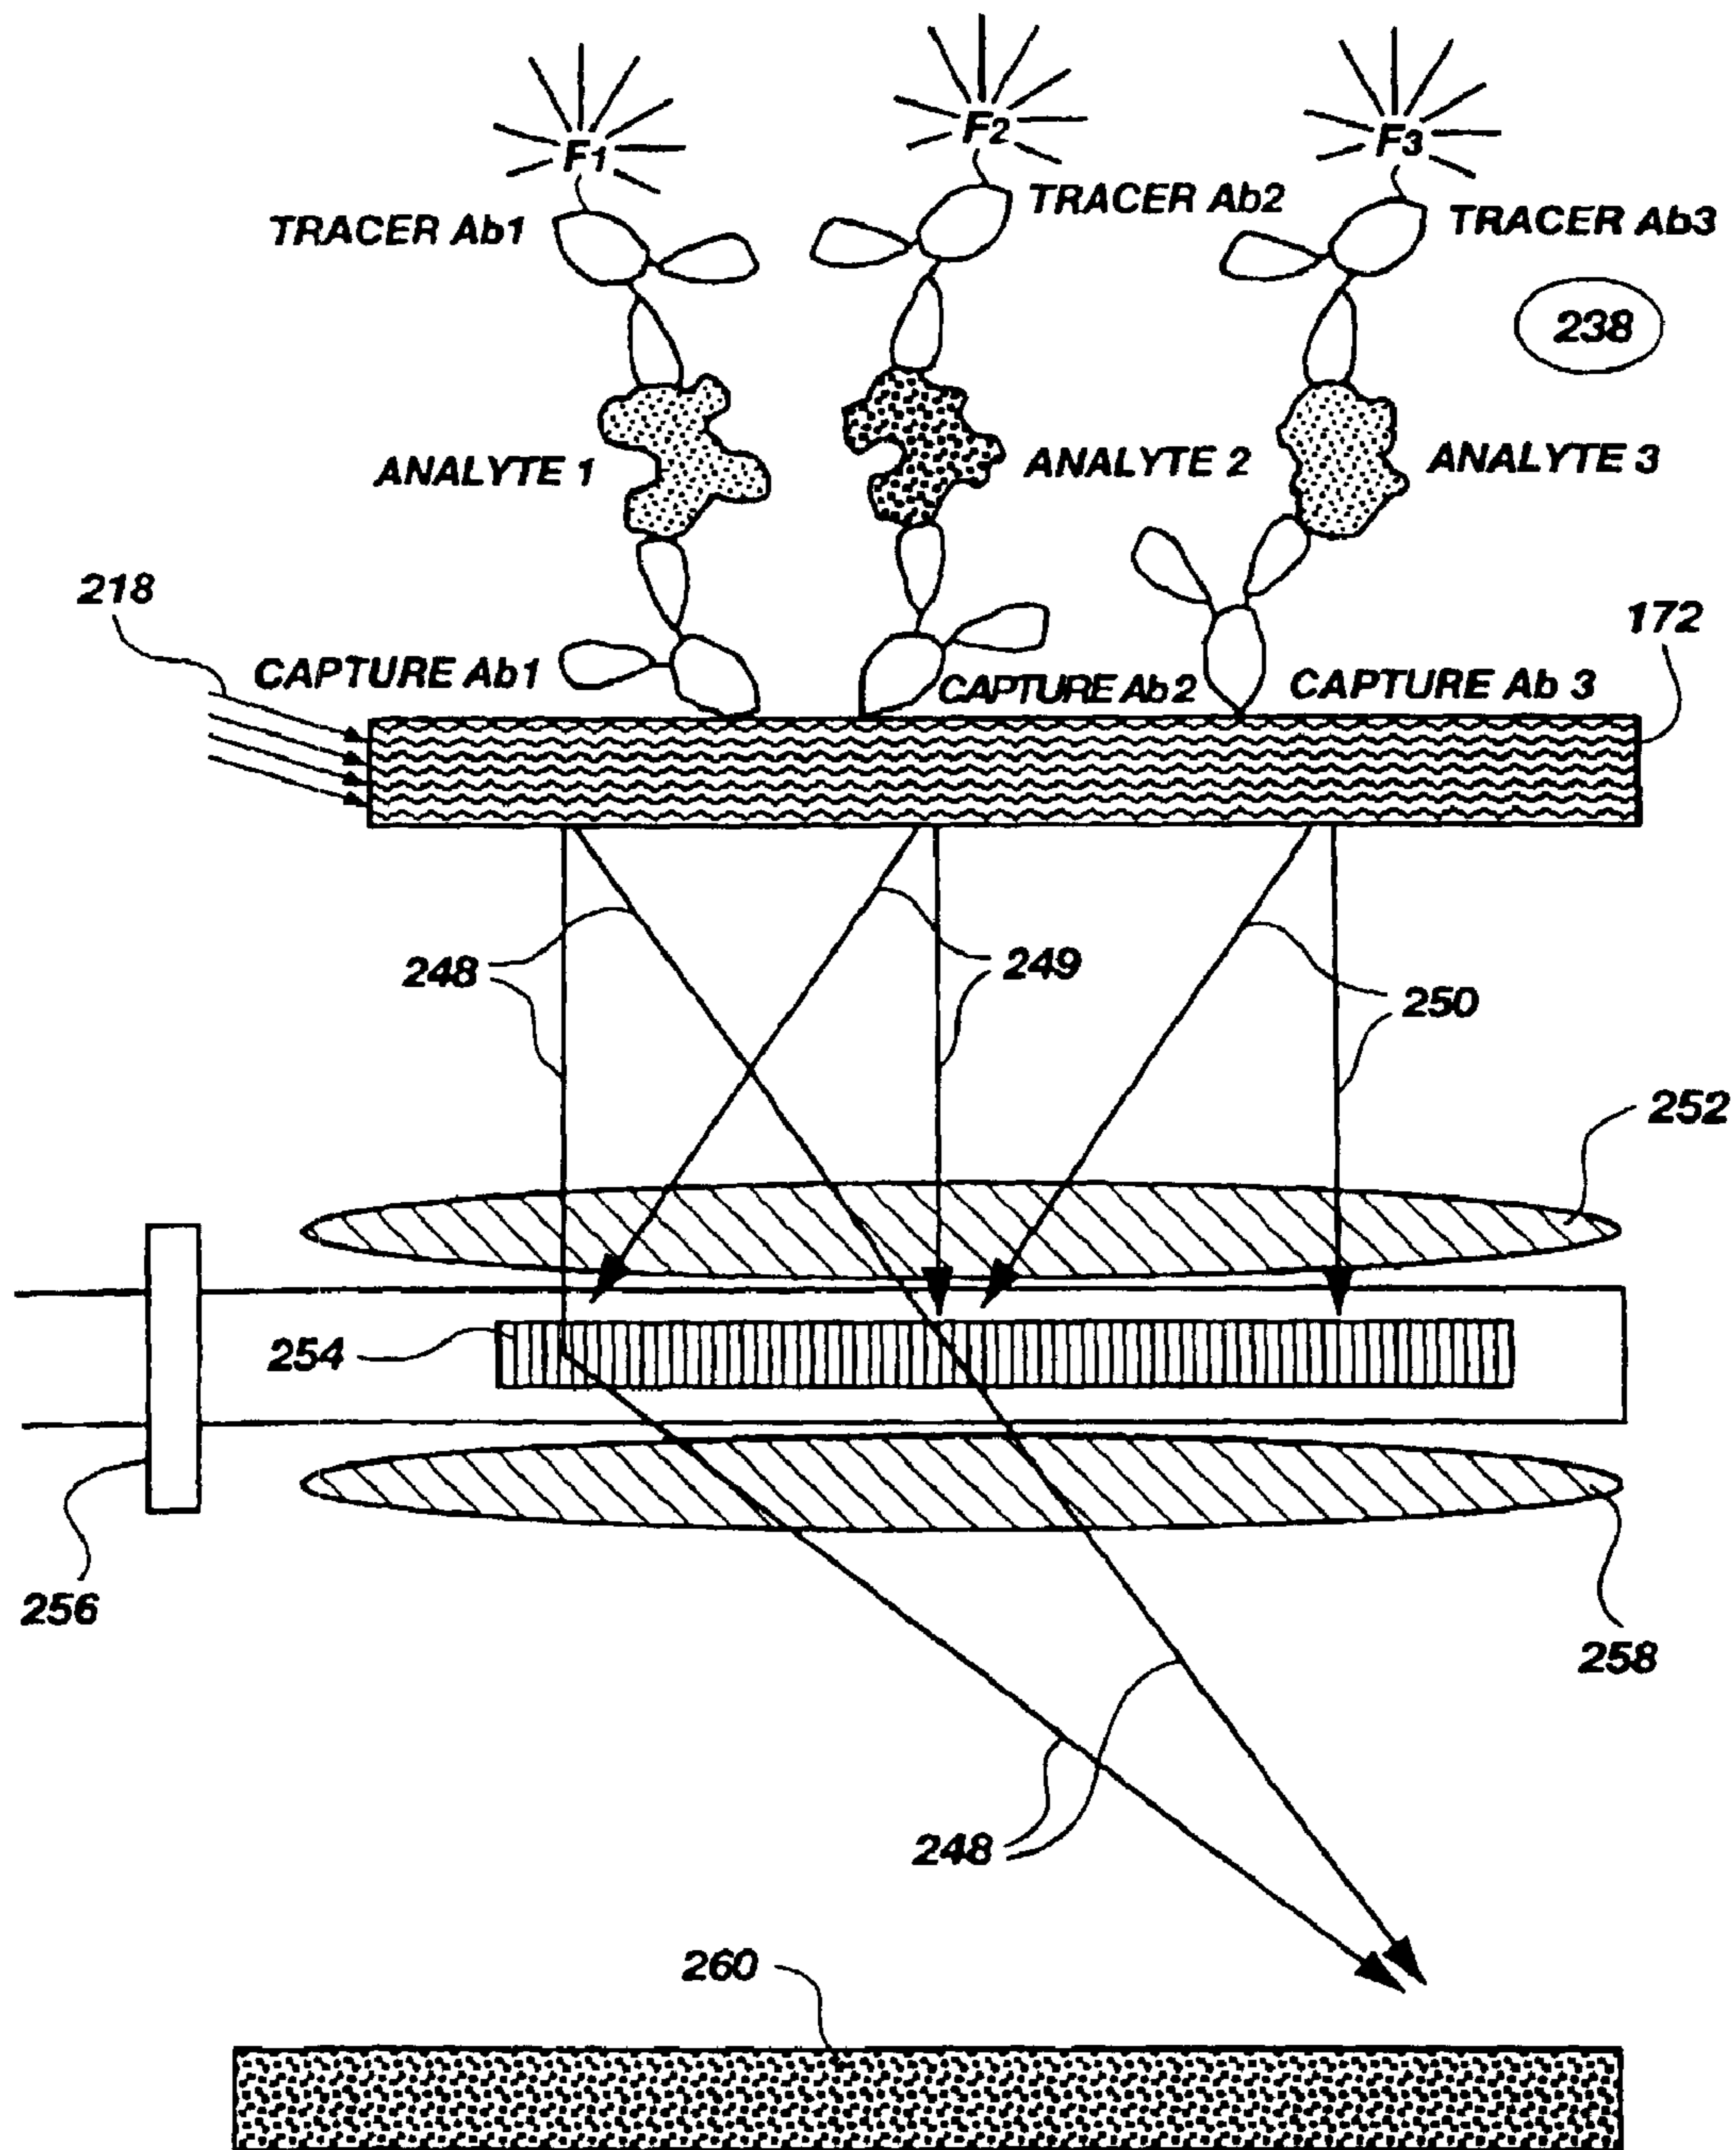


Fig. 24

LENS AND ASSOCIABLE FLOW CELL

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue.

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is an application under 35 U.S.C. § 371 of PCT/US97/04398 filed on Mar. 19, 1997, claiming priority from U.S. Provisional patent application No. 60/022,434 filed on Aug. 8, 1996 and U.S. Provisional patent application No. 60/013,695 filed on Mar. 19, 1996.

TECHNICAL FIELD

This invention relates generally to components of a diagnostic apparatus, and more particularly to an improved biosensor having a lens ("waveguide") and associated flow cell.

BACKGROUND ART

International Application No. PCT/US94/05567 (International Publication No. 94/27137, published Nov. 24, 1994) to the University of Utah Research Foundation discloses an apparatus for multi-analyte homogeneous, fluorimmunoassays. In one embodiment, the application discloses an apparatus which uses a biosensor having a planar waveguide sandwiched, with an associated gasket, between two plates (FIGS. 3A-3C of Internat'l Publ. No. 94/27137). The inner edges of the gaskets serve as walls for a reaction reservoir or well. Fluorescence-emitting tracer molecules are bound to the waveguide surface and are excited by an evanescent field penetrating into the adjacent solution from a light beam propagated within the waveguide, the beam being introduced at, for example, a front end of the waveguide. In the reaction reservoir, a liquid (e.g. serum or blood) is introduced and is allowed to admix with capture molecules associated with the waveguide surface (e.g. by "coating chemistry" as disclosed on pages 32 to 33 of the international application). The emitted fluorescence is then directly collected from the zone of evanescent penetration. In one particular embodiment, the biosensor has transparent walls which define the reservoirs. (E.g., FIGS. 11A-C of Internat'l. Publn. No. 94/27137). The application also discloses integrally formed or molded biosensors. E.g., FIGS. 12A, 12B & 13 of Internat'l. Publn. No. 94/27137).

Unfortunately, the waveguide portion of integrally formed or molded biosensors may exhibit deformation upon fabrication, or warping during storage or temperature changes. Also, gaskets may not reliably seal or are not always sufficiently inert to reactants, and thus may interfere with the desired analysis.

It would be desirable to have a biosensor having reservoirs with inert walls, the walls being readily detachable from the waveguide so that one waveguide could be readily exchanged for another.

DISCLOSURE OF THE INVENTION

The invention includes a biosensor with a reservoir or reservoirs, the biosensors including a waveguide placed (e.g. "sandwiched") between a plurality of members such as plates, at least one of the members being formed to define the walls of the reservoir or reservoirs where the reaction to be analyzed takes place. The reservoir walls are preferably

an inert, opaque material such as a passivated metal (e.g., black anodized aluminum). Although the biosensor may include a gasket, the gasket is associated with the plurality of members and waveguide in such a way (e.g. by recessing the gasket into a channel formed into a metal plate) so that the gasket does not form any significant portion of the reservoir wall. Waveguides of varying composition (e.g. plastic, quartz, glass or siliconoxynitride) may be associated with the members to form the biosensor. A lens or lenses may be integrated with the waveguide. The metal plate of the biosensor has input and output ports for infusing, draining, or oscillating the liquid to be analyzed in the reaction reservoir.

Due to the sandwiching of the waveguide in between the members, the planar waveguide is generally less distorted than that of an integrally formed biosensor. A reaction to be analyzed is not interfered with due to the use of opaque, inert metal to structurally define the reservoir.

The biosensor design is advantageously configured to interact with a flat waveguide having a rear integrated lens design for reading light passing through the waveguide (not fluorescent/evanescent light, but reading the core laser beam light) to monitor coupling efficiency and beam quality. The invention thus also includes a flat waveguide associated with a rear lens to couple light out of the waveguide (and a biosensor using such a lens) to serve as a quality control measure, thus insuring that the biosensor is properly placed and that the light source is working.

The invention also includes orienting the biosensor in a particular position relative to an optical reading device and laser which increases the performance of the biosensor to the point where, surprisingly, whole blood can be quickly analyzed.

BRIEF DESCRIPTION OF DRAWINGS

In the drawings, which depict presently preferred embodiments of the invention and in which like reference numerals refer to like parts in different views:

FIG. 1 depicts an enlarged bottom view of the flow cell top which may be used with the invention.

FIG. 2 depicts an enlarged section view of the flow cell top of the preceding figure along section line 2-2.

FIG. 3 depicts an enlarged section view of the flow cell top of FIG. 1 along section line 3-3.

FIG. 4 depicts an enlarged, exploded, perspective view of a biosensor according to the invention.

FIG. 5 depicts an enlarged, side view of a laminated gasket which interacts with the flow cell top of FIG. 1.

FIG. 6 depicts an enlarged view of a plastic, molded flat waveguide with integrated input and output coupling lenses.

FIG. 7 is an enlarged side view of the waveguide of the preceding figure.

FIG. 8 is a schematic diagram of a fluorescent assay apparatus useful for practicing the invention, showing the flow cell assembly of FIG. 4 in a particularly useful orientation with respect to the earth.

FIG. 9 is a stylized, enlarged side view of a portion of a waveguide and biochemical components of a competition immunofluorescent assay according to the invention.

FIG. 10 depicts an enlarged, exploded, perspective view of the flow cell portion of a biosensor according to the invention.

FIG. 11 depicts an enlarged perspective view of a gasket for use with the invention.

3

FIG. 12 depicts an enlarged top view of a second frame member ("flow cell bottom") for association with the flow cell top of FIGS. 1 through 3.

FIG. 13 depicts an enlarged side view of the second frame member of the preceding figure.

FIG. 14 depicts an enlarged perspective view of the registration plate forming part of the flow cell assembly of FIG. 4.

FIG. 15 depicts an enlarged top view of the stage member of the flow cell assembly of FIG. 4.

FIG. 16 depicts an enlarged side view of the stage member of the preceding figure.

FIG. 17 depicts an enlarged view of the preceding two figures.

FIG. 18 depicts an enlarged, exploded, perspective view of a biosensor according to the invention.

FIG. 19 depicts an enlarged, stylized, side view of a portion of a plastic film waveguide having an optical diffraction grating coupler.

FIG. 20 depicts an enlarged, stylized, side view of a portion of a plastic film waveguide to which a separate optical diffraction grating has been associated.

FIG. 21 is a graph depicting the results of a correlational analysis comparing an evanescent assay (CK-MB) of the instant invention with a prior art device.

FIG. 22 is a graph depicting the double logarithm plot of the data of the preceding figure showing the correlation.

FIG. 23 is a graph depicting the effect of agitation (oscillation) on a CK-MB assay on whole blood ("WB"), 50% WB, and 50% plasma using a device according to the invention (dilution with outdated CPDA anticoagulant solution).

FIG. 24 is an enlarged, stylized illustration of wavelength- and spatially-resolved detection of fluorescence emitted from a planar waveguide sensor using different capture molecules and tracer molecules for detecting different analytes of interest in a sample solution.

BEST MODE FOR CARRYING OUT THE INVENTION

A. Flow Cell

The flow cell top, generally 100, depicted in FIGS. 1 through 3 is preferably made of a light absorbing material (e.g. a metal such as aluminum having a passivated surface such as black anodized surface). The depicted flow cell top 100 is generally plate-like, and is formed to contain a plurality of wells or reservoirs 102, 104, 106 (for example, two to ten reservoirs).

A design with at least two individual reservoirs has significant advantages over a single reservoir embodiment for instances when it is desirable to measure the test sample fluorescent simultaneously with fluorescence from a "control" region on the same waveguide. For example, the level of non-specific binding to the waveguide (or non-specific fluorescence) can be subtracted from test sample fluorescence. Also, measurement changes due to fluctuations in intensity of the exciting light can be corrected. In a displacement assay, the "control" region could be a pre-loaded waveguide with no analyte present in the sample, or with a known amount of analyte. With the depicted embodiment of three or more wells, fluorescence can be measured for both a no-analyte control and at least one known calibration analyte sample in addition to the "unknown" or test sample. Although, even with a single reservoir, the invention is able to analyze multiple analytes in a single sample (e.g. by use of a single waveguide in multiple experiments).

4

In the depicted embodiment, the reservoirs 102–106 have respective inlet/outlet apertures 108, 110, 112, 114, 116, 118 extending through the flow cell top 100 for injecting and withdrawing the liquid to be analyzed into the reservoirs 102–106. In some cases, this liquid may be oscillated into and out of the reservoir with a pump, which enhances the mixing of the analyte and reactant (see, e.g., FIG. 23). With oscillation, the performance (e.g. speed) of the assay is increased. In the depicted embodiment, each port 108–118 is associated with its own depressed recess formed 120, 122, 124, 126, 128, 130 in the flow cell top 100.

Between the recesses associated with a particular reservoir, lateral or longitudinal channels may be formed in the flow cell top to aid in mixing the liquid contained within the reservoir (not shown).

The outer periphery of the reservoirs 102–106 are each defined by respective walls 132, 134, 136 which are preferably integrally formed with the rest of the flow cell top 100, although they may be a separate component of the flow cell top. The inner circumferences 138, 140, 142 of the walls 132–136 are made of an inert, opaque material such as an inert, opaque plastic, or a metal such as passivated, black anodized aluminum, copper, stainless steel, or similar alloy. In the depicted embodiment, the entire flow cell top 100 is made of a metal, while in other embodiments (not shown), the flow cell may be made of a non-metallic material, and an opaque, dark material or metal sleeve placed within the reservoirs (not shown). Material in contact with the liquid should exhibit low protein absorption properties. Accordingly, a metal, a hydrophilic non-metallic material or a hydrophobic non-metallic material coated with a thin film of hydrophilic material (e.g. PEG, PLURONICS or other hydrogels) may be used.

In the depicted embodiment, the apertures 108–118 associated with the respective reservoirs 102–106 fluidically communicate the recessed portions 120–130 of the reservoirs with a pair of respective receptacles 144, 146, 148, 150, 152, 154 (shown by construction lines in FIG. 1) for receiving fluid inlet/outlet ports 156, 158 which are associated with the flow cell top 100 (FIG. 4). Although the fluid inlet/outlet ports 156, 158 will be described with regard only to one reservoir, it is to be understood that the description applies likewise for the other reservoirs of the flow cell (if any).

As depicted in FIG. 4, the fluid inlet/outlet ports 156, 158 may be male threaded nipples which interact with corresponding threaded members (threads not shown) bored into the flow cell top 100. The open ends of the nipples are in fluid communication (e.g. by tubing or other conduit—FIG. 8) with a, for example, syringe pump (not shown). Other fluid tight arrangements between the ports and the flow cell top can be used, so long as the sample fluid communicates to the apertures 108–118. The liquid to be analyzed (e.g. whole blood, plasma, diluents, or mixtures thereof) can thus be injected and withdrawn from the reservoirs 102–106 by use of an, for example, oscillating pump (not shown).

As further depicted in FIGS. 1 and 4, the outer peripheries of the walls 132–136 also partially define a recess 160 formed in the flow cell top. This recess 160 is formed to accept a gasket 162 (FIGS. 4, 5 & 11) which is more thoroughly described hereinafter. This gasket 162 cushions placement of a waveguide onto the flow cell top 100 and impedes slippage of the waveguide when associated with the flow cell top. As is also more thoroughly described herein, the gasket, preferably, does not serve as any part of the walls 132–136 to contain the liquid within a reservoir 102–106. The flow cell may be used with a quartz waveguide or, more

preferably, with the hereinafter described plastic molded waveguide **164**.

B. The Waveguide

As depicted in FIGS. **4, 6 & 7**, a preferred waveguide **164** is a plastic molded waveguide (e.g. molded of an optical plastic) having integrated input **166** and output **168** coupling lenses. Such a waveguide **164** is preferably sled-shaped, having a planar (optical substrate) portion **170** with first **172** and second **174** parallel plane surfaces and an edge having a thickness **176** extending therebetween (FIG. **9**). At least one of the waveguide surfaces **172** has a plurality of capture molecules **240** associated therewith (e.g. immobilized thereon as depicted in FIG. **9**, although other methods of bringing the capture molecules into sufficiently close association with the surface may be used (e.g. by placing a strip immunoassay onto the waveguide surface, or using a fibrous "mat" with capture molecules attached to the fibers)). These surfaces **172, 174** should have the best optical smoothness possible. For example, surface waviness and roughness spacing should lie outside a range of about 65 nm to 195 micrometers ("µm"), while spacings close to 650 nm should be avoided (when 632.8 nm laser light is used). Surface roughness amplitude or "Ra" (theoretical surface plane to average peak or valley) should be less than 0.0065 µm (0.26 µin); however twice this amount is still functional. The thickness will typically be between 0.20 and one millimeter ("mm"), more preferably about 0.5 mm.

The edge of the planar portion has a receiving region (e.g. lens **166**) for receiving light to be integrally propagated. In the embodiment depicted in FIGS. **6 & 7**, an input or receiving lens **166** is integrally adapted to the waveguide adjacent the receiving region at the "front" of the waveguide. Other methods of optically associating the lens to the planar portion could also be used. Surface specifications for such a lens or lenses are similar to the planar or "plate" portion of the waveguide. A maximum roughness amplitude of 0.013 to 0.025 µm (0.5 to 1 µin) is preferred. Preferably, machine lines should be parallel (vertical when looking at lens) to the long axis of the waveguide. Surface specifications for the side of the part and lens ramp areas are less stringent than the top and bottom surfaces of the plate structure.

In another embodiment (not shown), the lens (or lenses) is not integrally associated with the waveguide, but is adapted to interact optically with the waveguide, or multiple waveguides.

Alternatively, rather than using a lens to coupling light into the waveguide, a grating could be used. Various gratings as well as methods for incorporating them into a waveguide are known. See, e.g., U.S. Pat. No. 5,480,687 (Jan. 2, 1996) to Heming et al. at column 4, lines 1-10, and column 6, line 20 to column 7, line 55, U.S. Pat. No. 5,081,012 (Jan. 14, 1992) to Flanagan et al., U.S. Pat. No. 5,455,178 (Oct. 3, 1995) to Fattinger, U.S. Pat. No. 5,442,169 (Aug. 15, 1995) to Kunz, and U.S. Pat. No. 5,082,629 (Jan. 21, 1992) to Burgess, Jr. et al. Gratings may be fabricated by a number of means including but not limited to: embossing, molding, photolithography, direct etch electron beam lithography, interference lithography, and phase shift lithography. Embossed gratings are mechanically stamped or thermally imbued onto a surface and thereupon affixed to a substrate. Photolithographic gratings are formed from the chemical development and etching of photoresist and substrate after masked illumination by an appropriate source. Interference and phase shift lithography are similar techniques which allow finer resolution of etched structures than does conventional photolithography. Ion or particle beam methods

fabricate precise gratings by directly etching or "writing" a grating substrate with a stream of ions or molecular particles.

The grating itself can consist of an etched pattern of regular features in a metal film coated onto the planar portion of the waveguide or the front ramp. Standard diffraction gratings such as those used in spectrometers like "replica" gratings (gratings comprised of a dried epoxy coated with metal) can be used. The use of such grating couplers helps to avoid fabrication complexities associated with the use of a receiving lens or plasma-etched gratings. The procedure for applying such couplers is presently used to emboss holograms onto plastic credit cards, and, using such a process, the coupler could be mass produced at a relatively low cost.

In an alternative embodiment shown in FIG. **19**, a corrugated waveguide with gratings **314** (>5 nanometers ("nm") deep or thick) is associated with (e.g. molded on, adhered to, or hot stamped onto or embossed onto) the receiving region of a plastic thin film waveguide **316** (or a cast thin plastic planar waveguide), associated with (e.g. adhered to) a lower index substrate **318**. Although in the depicted embodiment, the grating **314** is positioned between the thin film and the lower index substrate, other orientations such as applying the grating to the surface **172** of the thin film waveguide could also be used. Also, alternatively, the light could be directed into the waveguide from a different direction. In any event, the grating receives light **218** to be internally propagated. In such a case, the waveguide portion will typically be made of a transparent optical plastic and have a thickness of from about 10 micrometers to about 200 micrometers, preferably about 125 micrometers. In the case of extremely thin waveguide films (e.g. about 10 to 25 µm), the resulting film may be attached to a preferably rigid, open support structure [**317** (FIG. **20**)] (not shown). Alternately, the resulting thin film may be affixed to a supporting substrate having a lower index of refraction than the film (FIG. **19**).

From efficiency measurements, it can be determined that for an integrated optical waveguide-fluoroimmunoassay, the most efficient etch depths are about 1.5 times that of the grating period. For diffraction to occur in a grating, the period d should be on the order of the wavelength of light (λ). Given the pathlength difference, δ , between the light rays from two neighboring grating features (slits, rigids, and the like), a constructive interference pattern is established by the light leaving the grating when δ is an integer multiple, m , of the wavelength.

$$\delta = d(n_t \sin \theta_t - n_i \sin \theta_i) = \lambda(m)$$

wherein d is the grating period, θ_t and θ_i are the transmitted and incident angles at the grating interface (measured relative to the surface normal), and n_t and n_i are the refractive indices of the transmitting and incident mediums (i.e. the waveguide and the substrate). Using this formula, one determines that the incident angle for coupling 632.8 nm light is 38.03° when the grating period is 0.7 µm.

The angle of incidence of light from air into the lowest order mode of the waveguide and the groove density into waveguide films can be calculated by the use of the equation above, and was determined to be 4.6°, 27.4° and 57.2° for polystyrenes having densities of 2400 g/mm, 1800 g/mm, and 1200 g/mm, respectively, for incident light of 632.8 µm wavelength.

In still other embodiments, laser light may be prism-coupled onto an integrated optic waveguide ("IOW") (not shown), end-fire coupled (i.e. direct focusing of light into the

waveguide), or taper-coupled (e.g. by use of an adlayer film tapered in thickness or refractive index, preferably in conjunction with a grating coupler) into the waveguide (also not shown).

In order to taper-couple light into the flow cell, a gentle tapered section (e.g. either curved or linear) can be used to “funnel” light into the end of a thin planar waveguide. A well-collimated input beam (e.g. about 50 μm in thickness) due to the “Law of Brightness” constraint (i.e. the product of the beam extent and numerical aperture is a constant through the taper). The taper may be also coupled with a lens.

The waveguide depicted in FIGS. 6 & 7 has a shelf or ridge 176. The ridge 176 abuts against an edge of the flow cell top when the waveguide 164 is functionally associated with the flow cell (FIG. 4). As shown (FIG. 1), the flow cell top 100 has two apertures 178, 180 which interact with registration members (“registration pins”) 182, 184 of a second frame cell members (“flow cell bottom”) 186 structured to interact with the flow cell top 100 and waveguide 164 in order to hold (“sandwich”) the waveguide in place (FIG. 4).

Laser light preferably enters the receiving lens 166 at mean angle θ (FIG. 8). The mean angle θ will typically vary dependent upon the type of material used 5 to form the waveguide and the optical properties of the media opposite both faces of the waveguide. When the waveguide or waveguide layer is made of polystyrene (e.g. NOVOCOR), then the mean angle will generally be less than 32° , e.g. 15° to 25° . Typical beam widths vary from 0.5 to 2.0 mm.

On the other side of the waveguide, an outcoupling 188 interacts with the rear or output lens 168 to ensure that light is detected (FIG. 8). The outcoupling 188 may be a single photodetector, multiple photodetectors, standard CCD (charge-coupled device) or like device. The light passing through the waveguide 164 and received by the outcoupling 188 is analyzed for quality and/or intensity. Unlike the end collection of light described in U.S. Pat. No. 4,582,809 to Block et al. (Apr. 15, 1986), in the present invention, the light may be detected at the end of the waveguide for two reasons. The first reason is as a quality control measure. The light passing through the waveguide may be measured so that the operator of the device knows that the biosensor has been properly placed in the apparatus and that the light source is still working. Alternatively, the device may be configured so that a predetermined strength of light must first be detected at the rear lens 168 before the apparatus will operate, again to ensure that the flow cell assembly (“biosensor”), generally 190, has been properly placed. The second reason for end detection involves calibration of the device to ensure that the amount of light travelling through the waveguide is uniform and, if it is not uniform to accommodate any differences. The light outcoupled from the lens 168 associated with the rear of the waveguide is preferably measured over the width of the lens to ensure that sufficient light is passing through the lens to create detectable fluorescence.

Preferably, a plastic waveguide such as that depicted in FIGS. 6 & 7 will be made (e.g. injection-molded) of an optical plastic such as polystyrene, polymethylmethacrylate (“PMMA”), polycarbonate or equivalent material, and will have a refractive index greater than 1.33 (the index of water being 1.33). The size of the waveguide will depend on its desired use.

Although the front lens ramp 192 and rear lens ramp 194 are shown in a “concave” or arced position relative to one another and the planar portion 170 (FIG. 7), the ramps need not angle towards a common center, and one of the lens

ramps could be angled in the opposite direction from the plane of the planar portion, and the ramps would fall in roughly parallel planes (not shown).

In another embodiment (not shown), the waveguide includes a laminate of layers, one layer serving as a structural substrate, and the other (e.g. thin film SiON) serving to transmit the light, such as those disclosed in International Application No. PCT/US96/02662 (International Publication No. WO 96/26432, published Aug. 29, 1996) to the University of Utah Research Foundation. In such an embodiment, the structural substrate can be made of a plastic such as polystyrene, PMMA, polyvinyl chloride (“PVC”), polyimide, polyester, polyurethane, organically modified ceramics, polymers of diethylene glycol bisallyl carbonate, allyldiglycolcarbonate, polycarbonate, or equivalent material. The waveguide layer is preferably an optical plastic such as polystyrene, although it can be made of other suitable materials such as TiO_2 , a mixture of TiO_2 - SiO_2 , SiO_2 , ZnO , Nb_2O_5 , Si_3N_4 , Ta_2O_5 , HfO_2 , or ZrO_2 . Waveguide layers such as TiO_2 , SiO_2 , or Si_3N_4 can be deposited by plasma chemical vapor deposition (“PVCVD”), plasma impulse chemical vapor deposition (“PICVD”) process, or the like.

C. Gasket

A gasket 162 is preferably seated between waveguide 164 and flow cell top 100 (FIGS. 4, 5 & 11). A preferred gasket 162 for use with the waveguide 164 with integrated lenses includes a clear TEFLON layer 196 adhered (e.g. with the use of a suitable glue or double-sided tape, e.g. MACTAC No. SB 1154 available from Morgan Adhesives Co. of Stow, Ohio, USA) to a silicon rubber gasket 198 shaped to fit the recess of the flow cell top. Alternatively, synthetic resin polymers (i.e. TEFLON-like materials) may be used. The depicted gasket 162 is configured with three internal openings (FIG. 11 and construction lines 200 of FIG. 5) which surround, but do not interact with, the reservoirs 102–106.

Upon assembly of the biosensor, in the reservoirs 102–106, the first planar surface 182 of the waveguide 164 constitutes a floor or ceiling (FIG. 8) of the particular reservoir, while the flow cell top 100 is formed to constitute the ceiling or floor and the walls. The orientation depicted in FIG. 8, wherein the planar surface 172 serves as a ceiling and lays level with the earth has been found to be especially useful, enhancing the ability of the device to detect the presence of target molecules in even whole blood over a shorter period of time (e.g. five to ten minutes), especially with oscillation. However, it is, of course, understood that the flow cell assembly 190 may be oriented in any position (e.g., vertical or any angle). Angling the flow cell assembly 190 assists in removing bubbles or heavy materials away from the waveguide 164, if desired. Alternatively, a dye can be incorporated into the sample solution for absorbing interfering signals. Although the reservoirs 102–106 are here shown to be generally rectangular in shape, other shapes could be used.

The gasket 162 is preferably made of a semi-rigid material having an index of refraction less than that of the waveguide material in the wavelength range of the ceiling light. For best results, it is believed that the index of refraction of the gasket material should be as low as possible compared to that of the waveguide. For a waveguide made of quartz or glass, the index of refraction would typically be from about 1.46 to 1.52, higher for high-lead glass. A transparent (non-pigmented) silicon rubber (siloxane polymer) with an index of refraction of 1.35–1.43 is a presently preferred material for gasket 162. TEFLON or TEFLON-type materials such as PTFE

(polytetrafluoroethylene) or FEP (fluorinated ethylene propylene) have indices of refraction of around 1.34–1.35, and may also be suitable for use as layer **196**.

The other portion **198** of the gasket may be formed of an opaque (e.g. red or black) neoprene or silicon rubber material which is preferably biologically inert although due to the metal walls, it need not be.

D. The Flow Cell Assembly

As depicted in FIG. **18**, a preferred flow cell assembly **190** according to the invention generally includes a flow cell portion (generally **200**, FIG. **10**), gasket **162**, and waveguide **164**. As shown in FIG. **10**, the flow cell portion includes the flow cell top **100**, flow cell bottom **186**, and a flow cell stage (or “flow cell platform”) **202**. As shown in FIG. **8**, and as more thoroughly described herein, these three components of the biosensor **190** are integrated with one another in such a manner that excitation light enters the front lens **166** of the waveguide **164**, travels through the front lens ramp **192** and planar portion **170**, and passes out of the rear lens ramp **194** and rear lens **168** to the outcoupling **188**.

The flow cell assembly can also include means for associating the flow cell top **100** with the flow cell bottom **186** thus sandwiching the gasket **162** and waveguide **162** therebetween. The depicted means for doing so are threaded clamping bolts **204**, **206** which interact with correspondingly threaded holes **208**, **210** in the flow cell bottom **186**. Of course however, equivalent means such as screws, nuts and bolts, clamps, snap fits, and the like could alternatively be used.

A waveguide registration plate **212** is shown associated with the flow cell bottom **186** (FIG. **4**). The waveguide is reproducibly positioned between the flow cell top and bottom when aligned with the registration plate. Also depicted is a 3-channel beam mask **214** having three apertures for receiving a light beam.

E. The Apparatus

Once the flow cell **200**, gasket **162** and particular waveguide **164** have been associated with one another, the thus formed biosensor **190** may be used in an apparatus for performing immunoassays such as fluoroimmunoassays. As depicted in FIG. **8**, such an apparatus includes a light source **216** which provides a light beam **218** which is directed by means of mirrors **220**, **222**, **224** to an optical biosensor **190**. The light source **216** may be an argon laser or laser diode capable of emitting at center wavelengths of between 488 and 514.5 nm and 600 to about 900 nm (e.g. 633 nm), respectively.

The embodiment of FIG. **8** further includes a 45° angle mirror **226** which is positioned for assisting in focussing the beam **218** onto the input lens **166** of a particular biosensor **190** if desired. The biosensor **190** has an optical substrate with one end **166** positioned to receive light from beams **218**. In the case of a nonintegrated quartz waveguide, a focussing lens **228** is preferably positioned between angle mirror **226** and the biosensor **190** for focussing light from beam **218** onto the end of the biosensor. Focussing lens **228** is removable, and is depicted mounted on an X-Y translation unit so that its position may be adjusted for best focussing. Furthermore, the translation unit can be moved to adjust the angle θ for waveguides of differing composition. A significant portion (in the case of the quartz waveguide, the entire portion) of the optical substrate **164** is of a generally planar shape having two planar surfaces spaced by a width **176** as shown in FIG. **9**, which is more thoroughly described herein.

Light detection means, generally **230**, are positioned to detect fluorescent light emitted from the biosensor **190**. As more thoroughly described herein with regard to FIG. **9**, the

emitted light is reflective of the concentration of a selected analyte in a sample. The light detection means **230** depicted in FIG. **8** includes a collection lens **232** positioned to collect the emitted fluorescence from a direction substantially orthogonal to the direction of propagation of light **218** through optical substrate **164**.

The distance **234** between collection lens **232** and optical substrate **164** is selected as known to those skilled to maximize the collection of light emitted from the region of evanescent light penetration while at the same time imaging this light onto the face of the photodetector. The light collected by collection lens **232** is then sent to detection means **230**, which responds by outputting signals reflective of the level of collected fluorescent light.

Detection means **230** may be any type of photodetector useful to detect light in the waveguide region spanning the wavelength range of the emitted fluorescence, as known in the art. However, in a preferred embodiment for simultaneous multianalyte assays, detection means **230** is an imaging-type detector providing direct imaging of each of the fluorescence signal(s) originating in the evanescent zone **236** (FIG. **9**). In the apparatus of FIG. **8**, detection means **230** is a CCD detector which produces a signal. Such imaging signal collection provides simultaneous measurement of multiple samples in a much simpler way than a system in which a separate optical element is needed to read each well or patch. The present imaging detection system also provides for collection of emitted fluorescence directly from the evanescent zone **236**, rather than via evanescent penetration of the fluorescence into the waveguide (FIG. **9**).

Alternatively, detection means **230** may be a photomultiplier, a semiconductor photodiode, or an array of such detectors. In embodiments other than a CCD, an array is generally preferable to a single detector for some purposes. With an array of small detectors, the user can determine that the maximum fluorescence is being detected and is not inadvertently missed due to misalignment of the collection and detection optics. Optionally, a grating spectrograph is coupled to the CCD or other detection means to provide spectral analysis of the detected light. In that case, means are also provided to integrate the signal function around each peak to determine the total collected fluorescence from a sample. Alternatively, in an embodiment for use in a setting such as in a testing laboratory, and for which all the parameters of the assay have been standardized, the spectrograph may be replaced by a filter which passes only wavelengths in the region of tract fluorescence.

As is better seen in FIG. **9**, optical substrate **164** is embodied as a planar portion of a waveguide having at least one planar surface **172** spaced from a second surface **174** by a width **176**. At least one surface **174** is disposed in contact with a sample solution **238**. Capture molecules **240** are immobilized on the exposed surface **172** of the waveguide. In one embodiment, the sample solution **238** contains a plurality of analyte molecules **242** of a selected analyte which also includes tracer molecules **244**. The tracer molecules can be incorporated into the sample solution by, for example, admixing them with the sample solution before incorporation into the assay or by “drying” the molecules onto the waveguide surface without actually chemically binding them to the surface **172** (or at least not binding them permanently as would be the case when the tracer molecules are associated with the surface by use of a water soluble component (e.g. a soluble sugar that does not interfere with the particular interaction between capture and tracer molecules)). The capture molecules are chosen or con-

structed to bind to a binding moiety present on each of the analyte molecules **242**. The tracer molecules **244** is a molecule chosen to be complementary (in a binding sense) with the capture molecules and is constructed to emit fluorescent light in response to stimulation by light of the appropriate wavelength (e.g. by tagging the capture molecule with a fluorescent label). The level of fluorescence emitted by the tracer molecules **244** is a measure of the amount of analyte bound to the capture molecule and is thereby reflective of the concentration of analyte molecules **242** in the solution.

When light is being propagated in the waveguide **164** and internally reflected at the surfaces **172**, **174** an evanescent light field is produced having an intensity curve **230** which drops off with distance from the surface **172**, as diagrammed relative to a distance axis **232** and a horizontal axis **234** (not to scale). Evanescent light intensity varies along axis **232**, co-linear with distance. An excitation zone **236** is the only region of the solution in which the evanescent light intensity is sufficient to excite a significant or detectable fraction of tracer molecules **244** (not to scale). Tracer molecules **244** outside zone **236** will contribute little or no induced fluorescence. Excitation zone **236** is typically between about 1000 and 2000 Å in depth.

Capture molecules **240** are reactive with the analyte molecules **242**, and may be whole antibodies, antibody fragments such as Fab' fragments, peptides, epitopes, membrane receptors, whole antigenic molecules (haptens) or antigenic fragments, oligopeptides, oligonucleotides, mimitopes, nucleic acids and/or mixtures thereof. Capture molecules **240** may also be a receptor molecule of the kind usually found on a cell or organelle membrane and which has specificity for a desired analyte, or a portion thereof carrying the analyte-specific-binding property of the receptor.

The capture molecules **240** may be immobilized on the surface **172** by any method known in the art. However, in the preferred embodiment, the capture molecules are immobilized in a site-specific manner. As used in this application, the term "site-specific" means that specific sites on the capture molecules are involved in the coupling to the waveguide, rather than random sites as with typical prior art methods. Int'l Publ. No. 94/27137, which has been previously referenced, details methods for site-specific immobilization of capture molecules to the surface of the optical substrate by means of a protein-resistant coating on the substrate.

The waveguide can be designed so that multiple (e.g. four) different assays can be performed on the same sample. This is accomplished by immobilizing different types of capture antibodies on different regions of the waveguide, a process referred to as patterning. Three different patterning methods appear suitable for immobilizing antibodies to the polystyrene sensors—gasketed multiwell coating tray, liquid jet printing and photolithography. In the former, a machine similar to an ink jet printer is used to spray reagents onto a specific region of the waveguide; in this latter, ultraviolet light is used to photochemically cross-link antibodies to selected regions.

One immobilization chemistry is based on physical adsorption of antibodies to the waveguide. In one method, an antibody is briefly exposed to acidic conditions just prior to immobilization. It has been shown that this acid pretreatment step improves the antigen-binding capacity (AgBC) of immobilized antibodies by up to 3-fold in some cases. This immobilization chemistry is relatively simple and compatible with gasketed multi-well coating tray or liquid jet printing technology, but in some cases it exhibits a higher degree of non-specific binding than other methods.

The other two immobilization chemistries are based on a family of tri-block polymers of the form PEO-PPO-PEO, where PEO stands for poly(ethylene oxide) and PPO stands for poly(propylene oxide). These surfactants are sold under the trade name PLURONICS and come in a variety of chain lengths for both the PEO and PPO blocks. The PPO block is significantly more hydrophobic than the PEO blocks and adsorbs readily to non-polar surfaces such as polystyrene, leaving the PEO blocks exposed to bulk solution. The free ends of the PEO chains exhibit high mobility, literally sweeping proteins away from the surface.

In both the second and third immobilization chemistries, the surface of the waveguide is coated with pluronics before attachment of antibodies, but the two chemistries differ in how the antibodies are attached. In the second chemistry a photochemical cross-linking agent is used to conjugate antigen-binding fragments (Fab') to the PEO blocks, making this method suitable for patterning by photolithography. In the third chemistry, Fab' fragments are attached to pluronics using a chemical cross-linking agent, making this method compatible with gasketed multi-well coating tray or liquid jet patterning. The photochemical cross-linking method was evaluated with two different PLURONICS (F108 & F105) and two different photochemical crosslinkers (BPM and BPIA). While acceptable levels of total antigen binding can be obtained with all four pairwise combinations, an unacceptable level of NSB may be obtained when antibodies are immobilized to F108 using the BPIA crosslinker. The other three pairwise combinations give very low levels of NSB (about 1.5% of total binding). Furthermore, the P105/BPM pair is especially good, giving an undetectable level of NSB.

In FIG. 9, a competition assay scheme is depicted (also termed a displacement assay). However, as will be apparent to the skilled person, alternate assay schemes such as sandwich assays may be performed with the present apparatus. See, e.g. U.S. Pat. Nos. 4,376,110 and 4,486,530 to Hybritech, Inc.

In the embodiment of FIG. 9, the competition immunoassay has tracer molecules **244** constructed such that the capture molecules **240** will bind tracer molecules **244** in place of analyte molecules **242**. Higher concentrations of analyte molecules **242** will cause most of the tracer molecules **244** to be displaced into the surrounding solution from capture molecules **240**, thus reducing the number of tracer molecules within excitation range **236** of the substrate **164**. This reduced binding of tracer molecules in turn reduces the amount of fluorescence. In contrast, lower concentrations of analyte molecules **242** will allow tracer molecules **244** to bind to capture molecules **240**, and thus to be held within the excitation range **236**.

In tests conducted with the point-of-care cardiovascular marker CK-MB (associated with acute myocardial infarction) on both plasma and whole blood, the results were comparable (taking into consideration diffusion and viscosity differences).

In the embodiment of the apparatus of FIG. 8, measurements of fluorescence are made by spectroscopy. Fluorescence detection was done with a monochromator (SPEX Industries, Inc., Model 1680C) and a CCD (Photometrics Ltd. Series 200, or CH-250). Alternatively, light source **216** can be any light source emitting at the wavelength desired for excitation of selected fluorescent dyes. Also, once an assay procedure has been validated and standardized, it may not be necessary to measure the fluorescence spectrum or spatial distribution of fluorescence. The detection means may be simplified in accordance with the minimum requirements of the assay.

In another alternate embodiment, light source **216** is a laser diode emitting in the red wavelength region of 600–700 nm which is commercially available. The laser diode may provide about 12 milliwatts of power with a peak emission wavelength of about 635 nm. Laser diodes emitting at 633 nm are also available and can be used. For an embodiment using a wavelength in this region, it is necessary to use dyes such as cyanine dyes, which fluorescence can be stimulated by excitation with wavelengths in the red spectral region. An example of such a dye is the fluorescent dye **CY5**, available from Biological Detection Systems, Inc., Pittsburgh, Pa. (catalog no. A25000). The **CY5** dye can be conjugated to the desired tracer molecule by the manufacturer's instructions and/or with a kit available from BDS. A second dye, **CY7**, may also be suitable. The dyes and methods for conjugating are also characterized in the paper by Southwick, P.L., et al., titled "Cyanine Dye Labelling Reagents—Carboxymethylindocyanine Succinimidyl Esters", *Cytometry* 11:418–430 (1990). The use of laser diodes as a light source permits the biosensor and waveguide to be formed of plastic, which considerably reduces the expense of manufacture and facilitates the integral molding of the semi-cylindrical lens with the waveguide and reservoirs.

Different labels can be used which emit light at different wavelengths if desired. In such a circumstance, different types of capture molecules (e.g. antibodies reactive with different antigens) can be immobilized to the surface so that the waveguide can be used to detect more than one molecule to be detected. In such a case, multiple wavelengths can be detected by multiplexing the signal from the waveguide.

FIG. **24** stylistically illustrates simultaneous wavelength- and spatially-resolved detection of fluorescence emitted from a waveguide sensor using different capture molecules (Capture Ab_1 , Capture Ab_2 , Capture Ab_3 , . . . Capture Ab_x), tracer molecules (Tracer Ab_1 , Tracer Ab_2 , Tracer Ab_3 , . . . Tracer Ab_x), and labels (F_1 , F_2 , F_3 , . . . F_x) with the purpose of detecting different analytes of interest (Analyte₁, Analyte₂, Analyte₃, . . . Analyte_x) in a sample solution **238**.

In the depicted embodiment, the device works as otherwise herein described, but each tracer molecule (e.g. Tracer Ab_1 , Tracer Ab_2 , Tracer Ab_3 , . . . Tracer Ab_x) is labeled with a different colored fluorophore (F_1 , F_2 , F_3 , . . . F_x).

The waveguide is illuminated by one or more different wavelengths of light **218** appropriate to excite all the fluorophores located within the evanescent region of the waveguide. In one configuration, the emissions from the different fluorophores are distinguished using [bandpass] *band pass* filters. Light rays **248**, **249** and **250** are emitted from the respective labels on the tracer molecules. This light then passes through a lens **252** which collimates the emitted light onto a band pass filter **254** selective for the wavelength emitted by the particular tracer molecule label, in the depicted case, Tracer Ab_1 . A filter switching member, such as a wheel **256**, houses, for example, three different band pass filters—each selective for a different fluorophore label. Thus, only the light rays **248** emitted by Tracer Ab_1 pass through the filter **254**. If spatial resolution is desired in addition to wavelength selection, the light **248** passing through the filter **254** passes through a second lens **258** which images the light **248** onto a spatially-resolved photodetector **260** such as a CCD or diode array. If only wavelength resolution is desired, the photodetector **260** may be a single spatially-integrating device, and lens **258** may be optionally omitted.

Alternatively, the wavelength selectivity may be accomplished by one of several means instead of a filter wheel,

such as employing a diffraction grating, a prism, or an acousto-optical modulator to angularly separate the different emitted wavelengths and thus direct them to separate individual photodetector elements whose outputs are representative of the signal strengths in each wavelength band. In another arrangement which avoids the use of the rotating filter wheel, stationary beam splitters are employed to direct portions of the emitted light through stationary filters placed in front of individual photodetector elements.

Alternatively, if the excitation wavelengths of the different fluorophores are sufficiently separated without appreciable overlap, the light source may sequence in time through each excitation wavelength. The emitted light at any given time is released to the signal strength of the fluorophore set whose excitation wavelength is chosen at that particular time, and no further wavelength selective devices, such as filters, are needed.

The invention is further explained by the following illustrative example.

EXAMPLES

Example I

A waveguide with integrated lenses, such as that depicted in FIGS. **6** & **7**, was injection molded in a clean environment from a transparent, general purpose polystyrene. The waveguide had a length of 38 mm, and a width of 25 mm. The thickness **176** of the planar surface **170** was a consistent 0.5 mm. The ridge or "shelf" had a height of 1.3 mm. The front lens and rear lens had bottom edges co-planar with their respective centers of curvature. The front lens horizontal angle **262** was about 15°. The rear lens horizontal angle **264** was about 19°. The radii of curvature of the front and rear lenses were about 3.2 mm and 1.6 mm respectively. The mean angle θ of the front lens was 21°. The mean angle of the rear lens was about 24°.

Example II

A flow cell top, such as that depicted in FIGS. **1–3**, and **8**, was made of hard black anodized 6061-T6 aluminum. It contained three reservoirs each of which had a 0.25 mm (0.010 in.) thick wall surrounding it, a flat floor in middle, two half-capsule shaped recesses at either end 1.6 mm ($1/16$ in.) in width, and ports 1.6 mm ($1/16$ in.) in diameter running into the center of each recess. The ports opened into a #10-32 (standard thread, not NPT) connector which ran out to the opposite face of the flow cell and was 5.1 mm (0.200 in.) deep. A 90° countersink **266** (FIG. **2**) was given at the surface of the port connector (a plastic barbed tubing connector screwed into the port connector and sealed on the countersink). On both sides of the array of reservoirs were two raised platforms which were referred to as lands **268**, **270**. Each land had three holes running through the thickness of the part. The four #31 clamping holes **272**, **274**, **276**, **278** were formed (i.e. drilled through). The two apertures **178**, **180** were drilled and reamed to achieve a close sliding fit with 2.4 mm ($3/32$ in.) nominal four-sided pins **182**, **184** press fit into the second frame member **186**.

Example III

A gasket **162**, such as that depicted in FIGS. **4**, **5**, and **11**, was made as a composite structure laminated from 1.6 mm ($1/16$ in.) silicone rubber sheeting and 0.076 mm (0.003 in.) self-adhesive FEP film (total thickness: 1.676 mm (0.066 in.) nominal). Its outer dimensions were about 25 mm (1 in.) by 25.40 mm (1.000 in.) and it had three internal openings

which corresponded to the flow cell reservoirs. The gasket was produced using a waterjet cutter and was seated on the flow cell such that the FEP layer faced away from the flow cell surface.

Example IV

A second member **186**, such as that depicted in FIGS. **4**, **10**, **12**, **13** and **18** was made from hard black anodized 6061-T6 aluminum. It contained three internal openings **280**, **282**, **284** which corresponded to the three reservoirs **102**, **104**, **106** of the flow cell **100** (but were slightly longer). The internal openings were positioned in a shallow depression (0.46 mm (0.018 in.) deep) **286** which seated the waveguide, and allow evanescent light emitted from any reacting tracer molecules on the waveguide surface to be detected by the detection means **230**. As with the flow cell **102**, two lands **288**, **290** resided on either side of the internal openings, each land having three holes. Four clamping holes (e.g. **208**, **210**) were drilled through and tapped to #4-40 to receive thumb screws. Two apertures were drilled through to receive a 3.2 mm ($\frac{1}{8}$ in.) nominal dowel which was press fit into the hole. The dowel was stainless steel and projected approximately 7 mm (0.280 in.) above the top surface and 6.6 mm (0.260 in.) below the bottom surface of the second member. The exposed dowel was machined down to 2.4 mm ($\frac{3}{32}$ in.) nominal diameter was squared off to produce a low-friction locating pin **182**, **184**. The bottom aspect of the secondary member was milled out to provide a single large window **292** for emitted fluorescence from the waveguide. The front surface of the secondary member contains two mounting holes **294**, **296** #2-56 drilled and tapped to a depth of about 4 mm (0.15 in.) to fasten the flow cell registration plate **212**. The registration plate, depicted in FIGS. **14**, is a simple U-shaped bracket which was produced from 1.6 mm ($\frac{1}{16}$ in.) nominal 6061-T6 aluminum plate. It contained two #42 holes which corresponds to the holes on the front of the second member. The purpose of the registration plate was to provide a lateral hard-stop for the waveguide during clamping into the flow cell. The upright arms of the part contact the waveguide at the outer edges of the input coupling lens while allowing unimpeded coupling with the incoming laser beam.

Example V

A stage **202**, best depicted in FIGS. **15-17**, is a plate-like structure which was made from hard black anodized 6061-T6 aluminum. The receiving site **298** of the part was down-stepped and contains a single rectangular internal opening. Three #2-56 drilled and tapped holes **300**, **302**, **304** were positioned on the front of the part which were used to fasten a laser beam mask (not shown). Two #10-32 holes **306**, **308** were drilled to a depth of 19 mm (0.750 in.) on the right side of the part to mount the stage to the test apparatus. The internal opening had beveled front **310** and rear **312** sides. Located on either side of the window were two 2.4 mm ($\frac{3}{32}$ in.) apertures (analogous to those in the flow cell) which allowed the clamped flow cell and second member to be mounted to the stage **202**.

Example VI

The waveguide and integrated lenses of EXAMPLE I, the flow cell top of EXAMPLE II, the gasket of EXAMPLE III, the second member and registration plate of EXAMPLE IV, and the stage of EXAMPLE V were associated as in FIG. **4**. A hard, black anodized coating was added to the parts with a nominal build-up of 0.0025 mm (0.001 in.), however, the

assembly **190** was checked as much as possible prior to anodization to maximize the probability of proper fit.

The gasket was cut to correspond to the outside dimensions of the three reservoirs **102-106** of the flow cell top **100**. The silicone rubber surface contacted the flow cell and the FEP surface contacted the waveguide when the assembly was clamped. Any flash present on the gasket which interfered with seating or which came over the top of the walls was carefully trimmed back with a razor knife (the top of the dam was exposed to the surface of the waveguide, but did not touch it; flash from the gasket can interfere with proper clamping).

The waveguide **164** was seated in the shallow depression in the second member **186**. The waveguide fit into the depression with minimal lateral movement, but without compression or pinching. A small amount (e.g. less than about 0.1 mm (0.003 in.)) of lateral movement was acceptable. If pinching occurred, additional milling to the walls of the depression was necessary to allow proper seating.

To insure that the waveguide **164** was reproducibly positioned directly beneath the flow cell, it was butted up against the registration plate **214** after being seated in the secondary member **186**. Contact with the registration plate **214** was only at the outermost corners of the front lens; no contact with the injection mold stub on the underside of the front lens occurred (injection mold may be designed to place resultant stub at an alternate location). The front of the second member may need to be milled to ensure the waveguide sits directly beneath the flow cell when in contact with the registration plate.

After seating the gasket into the flow cell and positioning the waveguide on the second member, the flow cell was mated with the second member by engaging the locating pins into the apertures in the flow cell. When fully engaged, but without adding additional clamping force (i.e., the gasket was not compressed), there was a 0.15 mm (0.006 in.) gap between the lands of the flow cell and the lands of the second member. When fully clamped with four thumb screws such that the lands are in contact, the gasket is compressed 0.15 mm (0.006 in.). The flow cell and second member readily separated using manual force; no sticking occurred, but a thin coat of lubricant may be used on the pins if necessary. It may be desirable to slightly countersink the press fit hole on the second member and/or the aperture on the flow cell to avoid burrs or bulges which might impair mating of the two parts.

The locating pins from the bottom of the second member readily aligned and fit into the apertures on the stage. No perceptible play existed between the parts when mated. As with the flow cell and second member fit, the second member and stage readily separated using moderate manual force.

Example VI

As shown in FIG. **20**, onto a polystyrene sheet waveguide **316** (Scenic Materials, 125 μm thick, $n=1.60$) was adhered a piece of holographic diffraction grating **314** (Edmund Scientific #43226, 2400 g/mm, $\text{Al/N}_2\text{F}_2$ coated) with an index-matching cement **320** consisting of 10% polystyrene chips discussed in toluene. Incoupling into the resulting waveguide was achieved with a helium-neon laser at an approximately 5° angle. The resulting coupling structure was thinner than a molded lens input coupler.

Example VIII

A. Waveguide Fabrication

Thin film channel waveguide layers of SiON were formed on grating etched quartz wafers in a manner such as that described in Walker et al. "Corning 7059, silicon oxynitride, and silicon dioxide thin-film integrated optical waveguides: In search of low-loss, non-fluorescent reusable glass waveguides", *Appl.Spectrosc.*, 46: 1437-1441 (1992). Briefly, the wafers were introduced into a plasma impulse chemical vapor deposition ("PECVD") chamber (Texas Instruments) operating at 300° C., 50 W, and 1.25 Torr. The gases used were SiH₄, silane, nitrogen, ammonia, and nitrous oxide. SiON films were produced at a deposition rate of approximately 590 Å/minute for 25.42 min., yielding a film thickness of 1.5 μ. As described in Plowman et al., "Femtomolar sensitivity using a channel-etched thin film waveguide fluorosensor", *Biosensors & Bioelectronics*, 11:149-160 (1996), nine parallel 1 mm×65 mm channels are formed when etched into the SiON from an additional layer of photoresist. The resulting waveguide wafers were diced (Disco DAD-2H/6) into three rectangular pieces measuring about 2.5 cm×7.8 cm each with three waveguiding channels (although in this EXAMPLE, grating waveguides without channels were employed).

B. Grating Fabrication

Quartz wafer substrates (Hoya, Woodcliff Lake, N.J., QZ 4W55-325-UP) measuring 100 mm in flat length and 0.5 mm in thickness were cleaned at room temp. in a 6% solution of H₂O₂ in H₂SO₄. The wafers then received a HMDS vacuum vapor prime, were spin-coated with photoresist (Shipley SNR 200, MA, USA) at a rate of 4200 rpm for 1 min. to produce a film approximately 0.7 μ thick and then soft-baked at 100° C. for 1 min. The negative resist was exposed to define 0.7 μ periodic groove patterns using ultraviolet light (248 nm KrF excimer laser, Laser Stepper GCA-ALS, Tukesbury, Mass., USA) with a chrome-quartz mask (DuPont, Kokomo, Ind., USA) at a dose of 20 mJ/cm². The wafers received a post-exposure bake at 130° C. for 90 sec. Photoresist was developed in a solution of Shipley MF 312 (MA, USA) at a normalization of 0.17, then spun dry. A 60 sec. 100° C. post-development bake was then performed. The resulting photoresist pattern was reactive ion-etched (8110 Reactive Ion Etcher, AME, Santa Clara, Calif., USA) with O₂ and CHF₃ gases at an etch rate of 450 Å/min. Etch times of 13.33, 17.77 and 22.22 min. were employed to produce grating etch depths of 0.6, 0.8, and 1.0 μ giving aspect ratios of 0.8, 1.0, and 1.4, respectively. Residual photoresist was removed by O₂ plasma.

C. Testing

When used as light couplers for thin film IOWs, the gratings were roughly half as efficient as prisms in coupling laser light (the light source being a 2 mW He-Ne laser (632.8 nm, 10 nW maximum, Melles-Groit, Uniphase, Manteca, Calif., USA). Both approaches (i.e. prism and grating) detected samples with femtomolar concentration above background.

Example IX

An evanescent wave assay apparatus of the instant invention was compared with a standard ABBOTTS STAT CK-MB IMx system.

A. Clinical Samples

63 clinical samples (submitted by physicians for hospital CK-MB testing) were obtained, and were assayed for CK-MB using the ABBOTT IMx system. The values thus obtained for each clinical sample was noted. Each sample was aliquoted into 0.550 ml sample size, assigned a lot number, and stored at -20° C.

B. Instrumentation/Assay standardization

The samples were then assayed on a CK-MB system utilizing the biosensor **190** of the instant invention. CK-MB specificity was determined by spiking CK-MB stripped plasma (solid-phase absorption) with 1000 ng/ml CK-MM and CK-BB. Cross-reactivity with CK-MM was less than 0.1%. Standards were prepared by addition of a known mass quantity of recombinant CK-MB (Genzyme).

C. Monoclonal antibodies

Monoclonal antibodies were as described by J. Landenson, *Clinical Chemistry*, vol. 32, pp. 657-63 (1986). The capture antibody was coated onto the waveguide's surface with 2 hour incubation at room temp., at a concentration of 0.1 micromolar (diluted in PBSA buffer). After the incubation, each waveguide was washed once with PBSA, and then incubated with 1 ml of post-coating solution (0.5% bovine serum albumin ("BSA")/0.1% trehalose/PBSA) at room temp. for 1 hour. The post-coating solution was discarded and the waveguides dried in a vacuumed desiccator for an hour.

E. Specific Performance

The correlation of an apparatus according to the instant invention with the ABBOTTIMx assay for an CK-MB assay is graphically depicted in FIGS. **21** & **22**. The results showed the two sets of values to be comparable at a correlation coefficient of 0.98, and the sample population contained a higher proportion of samples below 50 ng/ml, the range in which the critical decision point for clinical evaluation has been established in the clinical laboratory environment. FIG. **21** plots the value obtained with the instant invention (y axis, in ng CK-MB/ml) against the ABBOTT IMx value on the x-axis (also ng CK-MB/ml). FIG. **22** depicts the double logarithm plot of the data from FIG. **21** (again, instant invention y-axis, ABBOTT IMx x-axis).

Example X

The preceding example was continued to further establish the utility of the system, and to incorporate more extensive studies of known interfering substances (e.g. hemoglobin and bilirubin), known CK-MB concentrations were analyzed (20 ng/ml CK-MB into human plasma), with concentrations of hemoglobin (15 mg/ml) and bilirubin (1 mg/ml) known to interfere with immunofluorescence assays. The system was still able to detect 100% of the CK-MB.

Characteristics of the described and illustrated embodiments are intended for illustrative purposes, and are not to be considered limiting or restrictive. It is to be understood that various adaptations and modifications may be made by those skilled in the art to the embodiments illustrated herein, without departing from the spirit and scope of the invention, as defined by the following claims thereof.

What is claimed is:

1. An improvement in a biosensor of the type for use in an apparatus for analyzing a biological liquid, the biosensor comprising:

a waveguide having at least one planar surface, said waveguide associated, in liquid tight attachment, with a first member, said first member, in conjunction with the waveguide, defining walls of reservoirs for containing the biological liquid while, a planar surface of the waveguide defines a floor of said reservoirs, the floor being associated in part with capture molecules, the improvement comprising reservoir walls formed of an inert, opaque material.

2. The improvement of claim **1** wherein said inert, opaque material is metal.

19

3. The improvement of claim 1 wherein the entire first member is made of metal.

4. The improvement of claim 1 wherein said first member has ports for oscillating liquid into and out of a reservoir.

5. The improvement of claim 1, wherein the biosensor further comprises a gasket positioned to cushion the attachment of the first member to the waveguide.

6. The improvement of claim 5, wherein the gasket is a laminate of elastic material and a synthetic resin polymer material.

7. The improvement of claim 1 wherein the waveguide is made of an optical material selected from the group of optical materials consisting of plastic, quartz, and glass.

8. The improvement of claim 7 wherein the waveguide is flat and is associated with a rear lens for reading light passing through the waveguide to monitor coupling efficiency and beam quality.

9. The improvement of claim 1 wherein the biosensor further includes a second member, the waveguide being sandwiched between said first member and said second member.

10. The improvement of claim 9 wherein the biosensor further includes a registration plate.

11. The improvement of claim 10 placed in an assay apparatus wherein the biosensor further includes a third member, the third member having a means for connecting the biosensor to the assay apparatus.

12. The improvement of claim 7 wherein the waveguide is flat, and is associated with a grating for coupling light into the waveguide.

13. A waveguide comprising:

a front ramp with associated lens end for receiving light, a rear ramp with associated lens for transmitting light out of said waveguide,

a planar portion having first and second parallel planar surfaces for transmitting light from the front ramp to the rear ramp so as to transmit light received at the lens associated with the front ramp through the lens associated with the rear ramp, and

wherein the waveguide is made from an optical plastic, and the front ramp is angled away from the planar portion's plane at a mean angle of from about 15° to 32°.

14. A biosensor of the type for use in an apparatus for analyzing a biological liquid, the biosensor comprising:

a waveguide having at least one planar surface and being optically associated with a rear lens oriented for reading light passing through the waveguide, to monitor coupling efficiency and beam quality, said waveguide further associated in liquid tight attachment with

a first member, said first member, in conjunction with the waveguide, defining metal walls of a plurality of reservoirs for containing the biological liquid while a planar surface of the waveguide defines a nonmetal floor of said plurality of reservoirs, the floor being associated in part with capture molecules,

a gasket positioned to cushion the attachment of the first member to the waveguide, and

20

a second member, the waveguide being sandwiched between the first and second members.

15. The biosensor of claim 14 wherein said first member has ports for infusing and draining liquid into and out of a reservoir.

16. An improvement in an apparatus for analyzing a biological liquid, said apparatus being of the type having:

a light source;

a biosensor comprising:

a waveguide having at least one planar surface, and being further associated in liquid tight attachment with

a first member, said first member, in conjunction with the waveguide, defining at least one reservoir for containing the biological liquid, the planar surface being associated in part with capture molecules, and an inlet and outlet in fluid communication with said reservoir for infusing and draining said biological liquid into and out of said reservoir so as to allow the biological liquid to contact said capture molecules; and

a light detector for detecting the light emitted through said planar surface;

the improvement comprising orienting said biosensor in such a way that the planar surface is generally horizontal and level with a surface upon which the apparatus sits and so that the planar surface forms a ceiling to said reservoir.

17. An improvement in a biosensor of the type for use in an apparatus for analyzing a biological liquid, the biosensor comprising:

a waveguide having at least one planar surface, said waveguide associated, in liquid tight attachment with a first member, said first member, in conjunction with the waveguide, defining walls of at least one reservoir for containing the biological liquid while, a planar surface of the waveguide defines a surface of said reservoirs, the surface being associated in part with capture molecules, the improvement comprising reservoir walls formed of an inert, opaque material.

18. A biosensor of the type for use in an apparatus for analyzing a biological liquid, the biosensor comprising:

a waveguide having at least one planar surface and being optically associated with a rear lens oriented for reading light passing through the waveguide, to monitor coupling efficiency and beam quality, said waveguide further associated in liquid tight attachment with

a first member, said first member, in conjunction with the waveguide, defining metal walls of at least one reservoir for containing the biological liquid while a planar surface of the waveguide defines a nonmetal surface of said at least one reservoir, the surface being associated in part with capture molecules,

a gasket positioned to cushion the attachment of the first member to the waveguide, and

a second member, the waveguide being sandwiched between the first and second members.

* * * * *