

US00RE43882E

(19) **United States**
(12) **Reissued Patent**
Hopkins et al.

(10) **Patent Number:** **US RE43,882 E**
(45) **Date of Reissued Patent:** ***Dec. 25, 2012**

(54) **VASCULAR DEVICE FOR EMBOLI, THROMBUS AND FOREIGN BODY REMOVAL AND METHODS OF USE**

is a continuation-in-part of application No. 09/364,064, filed on Jul. 30, 1999, now Pat. No. 6,530,939.

(75) Inventors: **Leo N. Hopkins**, Buffalo, NY (US);
Farhad Khosravi, San Mateo, CA (US);
Amr Salahieh, Campbell, CA (US);
Jackson F. Demond, Santa Cruz, CA (US);
Jonah Lepak, Santa Cruz, CA (US);
Stephen Ramee, New Orleans, LA (US);
Jeff A. Krolik, Campbell, CA (US);
Richard Renati, San Jose, CA (US)

(51) **Int. Cl.**
A61M 29/00 (2006.01)
(52) **U.S. Cl.** **606/200**; 606/194
(58) **Field of Classification Search** 606/108,
606/110, 113, 159, 200, 194
See application file for complete search history.

(73) Assignee: **Incept, LLC**, San Mateo, CA (US)

(56) **References Cited**

(*) Notice: This patent is subject to a terminal disclaimer.

U.S. PATENT DOCUMENTS
3,592,186 A 7/1971 Oster
(Continued)

(21) Appl. No.: **13/162,769**

FOREIGN PATENT DOCUMENTS
DE 2821048 A 11/1979
(Continued)

(22) Filed: **Jun. 17, 2011**

OTHER PUBLICATIONS

Related U.S. Patent Documents

“Atherosclerotic Disease of the Aortic Arch as a Risk Factor of Recurrent Ischemic Stroke,” *The New England Journal of Medicine*, pp. 1216-1221 (May 1996).

Reissue of:

(64) Patent No.: **6,544,279**
Issued: **Apr. 8, 2003**
Appl. No.: **09/636,040**
Filed: **Aug. 9, 2000**

(Continued)

U.S. Applications:


(63) Continuation-in-part of application No. 09/611,428, filed on Jul. 7, 2000, now Pat. No. 6,616,679, and a continuation-in-part of application No. 09/470,857, filed on Dec. 23, 1999, now Pat. No. 6,129,739, and a continuation-in-part of application No. 09/470,703, filed on Dec. 23, 1999, now Pat. No. 6,179,861, and a continuation-in-part of application No. 09/470,682, filed on Dec. 23, 1999, now Pat. No. 6,214,026, and a continuation-in-part of application No. 09/470,681, filed on Dec. 23, 1999, now Pat. No. 6,203,561, and a continuation-in-part of application No. 09/430,211, filed on Oct. 29, 1999, now Pat. No. 6,589,263, which

Primary Examiner — Elizabeth Houston
(74) *Attorney, Agent, or Firm* — Seager, Tufte & Wickhem LLC

(57) **ABSTRACT**

Apparatus and methods are provided for use in filtering emboli from a vessel and/or performing thrombectomy and embolectomy, wherein a vascular device comprises one or more support hoops connected near a distal end of a guide wire, each support hoop having an articulation region, and a blood permeable sac affixed to the support hoop or hoops to form a mouth of the blood permeable sac. The mouth of the sac closes when the apparatus is collapsed for removal to prevent material from escaping from the sac.

26 Claims, 15 Drawing Sheets

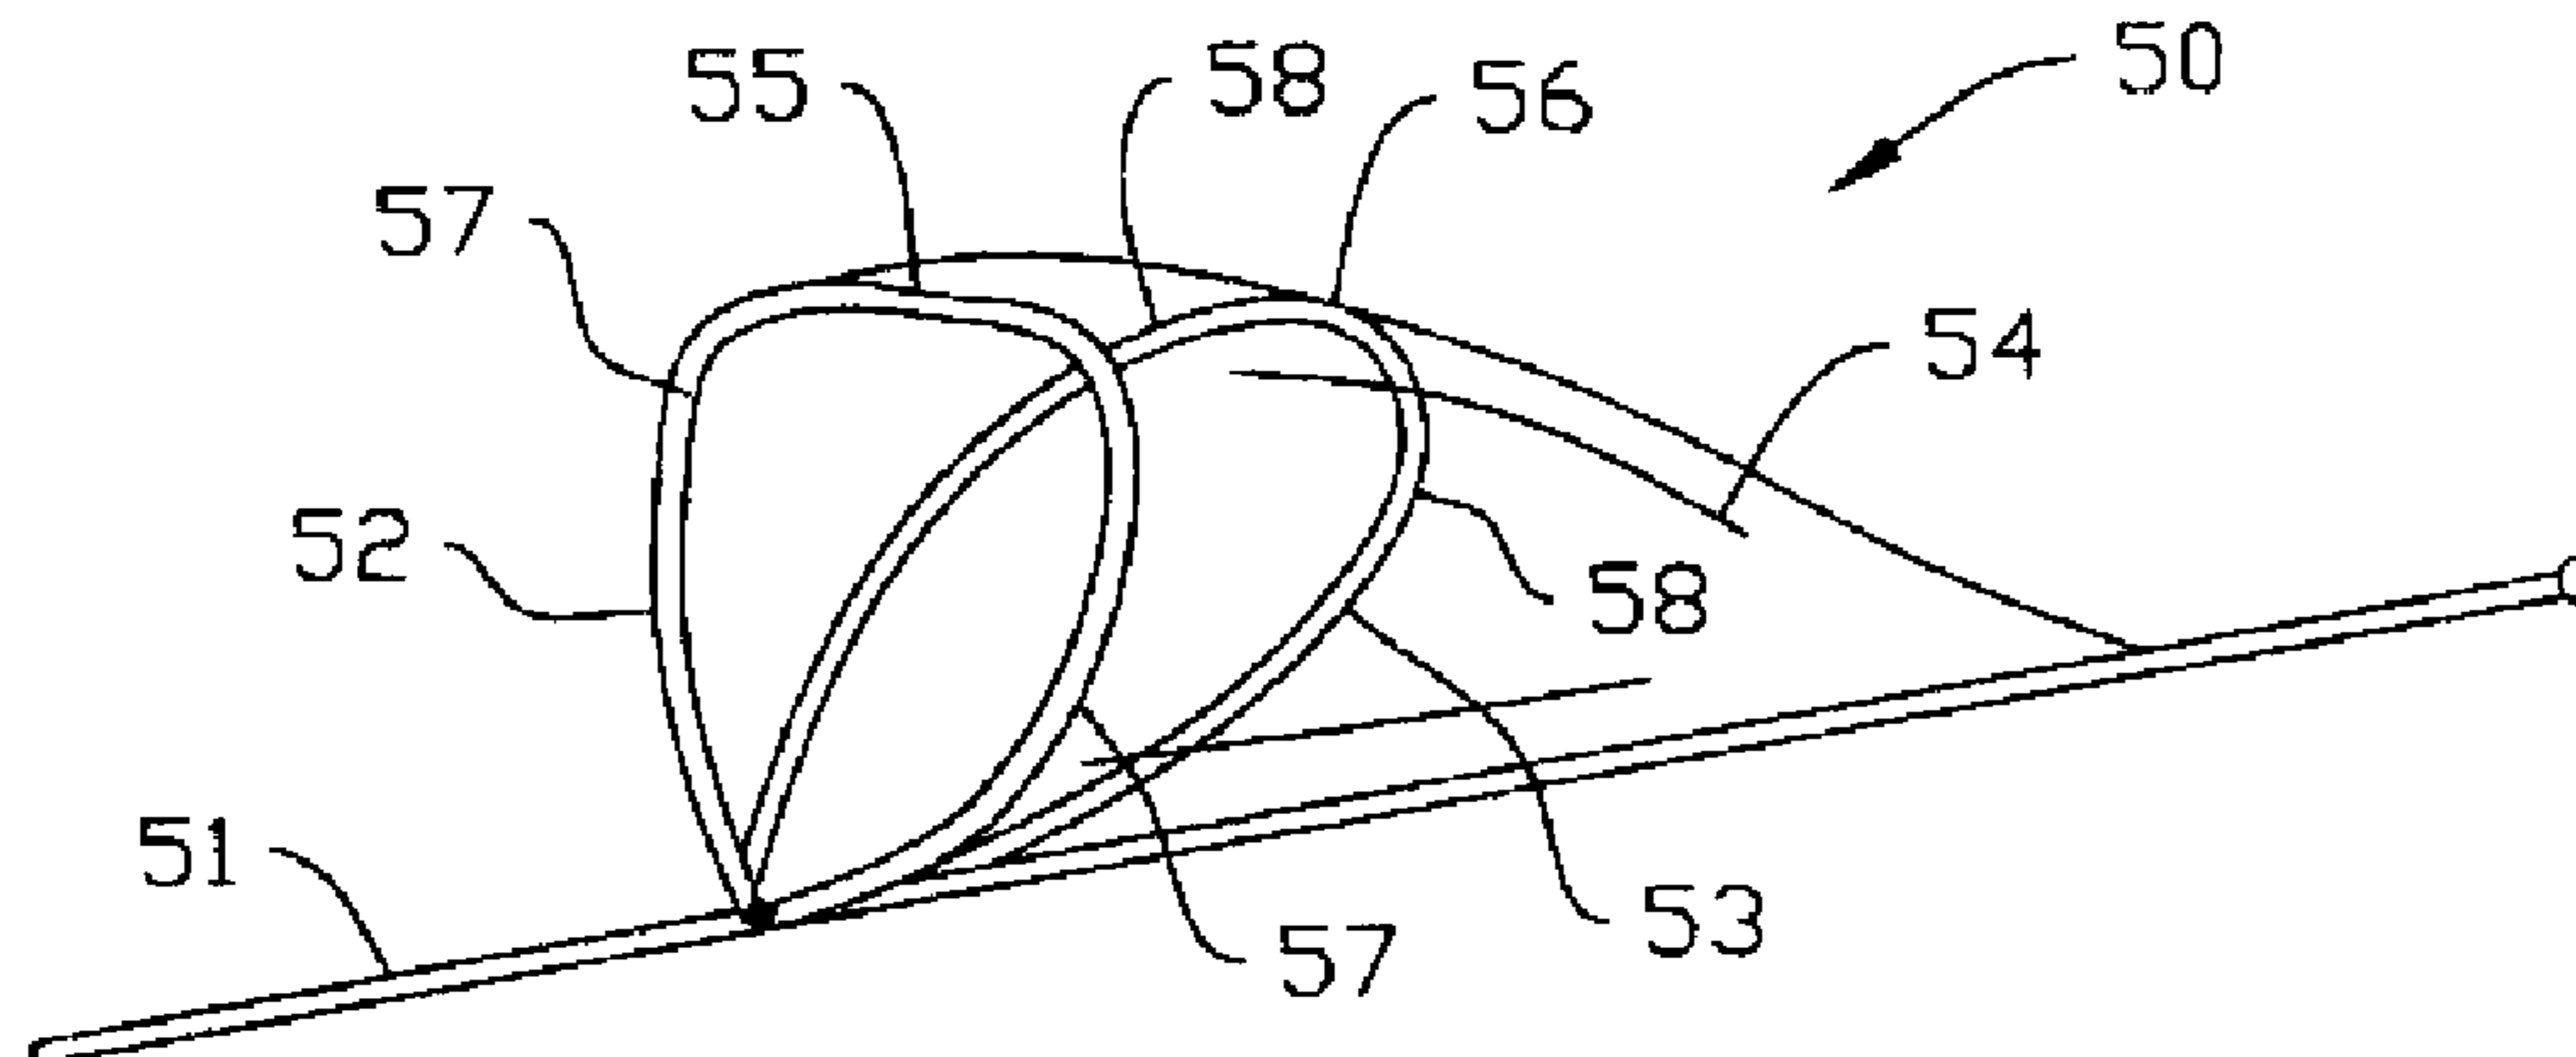

US RE43,882 E

Page 2

U.S. PATENT DOCUMENTS					
3,683,904 A	8/1972	Forster	5,354,310 A	10/1994	Garnic et al.
3,952,747 A	4/1976	Kimmell, Jr.	5,356,423 A	10/1994	Tihon et al.
3,996,938 A	12/1976	Clark, III	5,366,464 A	11/1994	Belknap
4,046,150 A	9/1977	Schwartz et al.	5,366,473 A	11/1994	Winston et al.
4,425,908 A	1/1984	Simon	5,370,657 A	12/1994	Irie
4,447,227 A	5/1984	Kotsanis	5,370,683 A	12/1994	Fontaine
4,580,568 A	4/1986	Gianturco	5,376,100 A	12/1994	Lefebvre
4,590,938 A	5/1986	Segura et al.	5,383,887 A	1/1995	Nadal
4,619,246 A	10/1986	Molgaard-Nielsen et al.	5,383,892 A	1/1995	Cardon et al.
4,631,052 A	12/1986	Kensey	5,383,926 A	1/1995	Lock et al.
4,643,184 A	2/1987	Mobin-Uddin	5,387,235 A	2/1995	Chuter
4,650,466 A	3/1987	Luther	5,395,349 A	3/1995	Quiachon et al.
4,662,885 A	5/1987	DiPisa, Jr.	5,397,345 A	3/1995	Lazarus
4,705,517 A	11/1987	DiPisa, Jr.	5,405,377 A	4/1995	Cragg
4,706,671 A	11/1987	Weinrib	5,409,454 A	4/1995	Fischell et al.
4,723,549 A	2/1988	Wholey et al.	5,415,630 A	5/1995	Gory et al.
4,728,319 A	3/1988	Masch	5,419,774 A	5/1995	Willard et al.
4,733,665 A	3/1988	Palmaz	5,421,832 A	6/1995	Lefebvre
4,790,812 A	12/1988	Hawkins, Jr. et al.	5,423,742 A	6/1995	Theron
4,790,813 A	12/1988	Kensey	5,423,885 A	6/1995	Williams
4,794,928 A	1/1989	Kletschka	5,425,765 A	6/1995	Tiefenbrun et al.
4,794,931 A	1/1989	Yock	5,443,498 A	8/1995	Fontaine
4,800,882 A	1/1989	Gianturco	5,449,372 A	9/1995	Schmaltz et al.
4,807,626 A	2/1989	McGirr	5,456,667 A	10/1995	Ham et al.
4,842,579 A	6/1989	Shiber	5,462,529 A	10/1995	Simpson et al.
4,857,045 A	8/1989	Rydell	5,476,104 A	12/1995	Sheahon
4,857,046 A	8/1989	Stevens et al.	5,484,418 A	1/1996	Quiachon et al.
4,867,157 A	9/1989	McGurk-Burleson et al.	5,507,767 A	4/1996	Maeda et al.
4,873,978 A	10/1989	Ginsburg	5,512,044 A	4/1996	Duer
4,898,575 A	2/1990	Fischell et al.	5,527,354 A	6/1996	Fontaine et al.
4,907,336 A	3/1990	Gianturco	5,536,242 A	7/1996	Willard et al.
4,921,478 A	5/1990	Solano et al.	5,540,707 A	7/1996	Ressemann et al.
4,921,484 A	5/1990	Hillstead	5,549,626 A	8/1996	Miller et al.
4,926,858 A	5/1990	Gifford et al.	5,562,724 A	10/1996	Vorwerk et al.
4,950,277 A	8/1990	Farr	5,569,274 A	10/1996	Rapacki et al.
4,955,895 A	9/1990	Sugiyama et al.	5,569,275 A	10/1996	Kotula et al.
4,957,482 A	9/1990	Shiber	5,634,897 A	6/1997	Dance et al.
4,969,891 A	11/1990	Gewertz	5,658,296 A	8/1997	Bates et al.
4,979,951 A	12/1990	Simpson	5,662,671 A	9/1997	Barbut et al.
4,986,807 A	1/1991	Farr	5,669,933 A	9/1997	Simon et al.
4,998,539 A	3/1991	Delsanti	5,695,519 A	12/1997	Summers et al.
5,002,560 A	3/1991	Machold et al.	5,709,704 A	1/1998	Nott et al.
RE33,569 E	4/1991	Gifford, III et al.	5,720,764 A	2/1998	Naderlinger
5,007,896 A	4/1991	Shiber	5,728,066 A	3/1998	Daneshvar
5,007,917 A	4/1991	Evans	5,746,758 A	5/1998	Nordgren et al.
5,011,488 A	4/1991	Ginsburg	5,749,848 A	5/1998	Jang et al.
5,019,088 A	5/1991	Farr	5,769,816 A	6/1998	Barbut et al.
5,041,126 A	8/1991	Gianturco	5,776,183 A *	7/1998	Kanesaka et al. 623/1.15
5,053,008 A	10/1991	Bajaj	5,779,716 A	7/1998	Cano et al.
5,053,044 A	10/1991	Mueller et al.	5,792,157 A	7/1998	Mische et al.
5,071,407 A	12/1991	Termin et al.	5,792,300 A	8/1998	Inderbitzen et al.
5,071,425 A	12/1991	Gifford, III et al.	5,795,322 A	8/1998	Boudewijn
5,085,662 A	2/1992	Willard	5,797,952 A	8/1998	Klein
5,087,265 A	2/1992	Summers	5,800,457 A	9/1998	Gelbfish
5,100,423 A	3/1992	Fearnot	5,800,525 A	9/1998	Bachinski et al.
5,100,424 A	3/1992	Jang et al.	5,810,874 A	9/1998	Lefebvre
5,100,425 A	3/1992	Fischell et al.	5,814,064 A	9/1998	Daniel et al.
5,102,415 A	4/1992	Guenther et al.	5,817,102 A	10/1998	Johnson et al.
5,104,399 A	4/1992	Lazarus	5,827,324 A	10/1998	Cassell et al.
5,108,419 A	4/1992	Reger et al.	5,833,644 A	11/1998	Zadno-Azizi et al.
5,133,733 A	7/1992	Rasmussen et al.	5,833,650 A	11/1998	Imran
5,135,531 A	8/1992	Shiber	5,846,260 A	12/1998	Maahs
5,152,771 A	10/1992	Sabbaghian et al.	5,848,964 A	12/1998	Samuels
5,152,777 A	10/1992	Goldberg et al.	5,876,367 A	3/1999	Kaganov
5,160,342 A	11/1992	Reger et al.	5,893,867 A	4/1999	Bagaoisan et al.
5,171,233 A	12/1992	Amplatz et al.	5,895,399 A	4/1999	Barbut et al.
5,190,546 A	3/1993	Jervis	5,902,263 A	5/1999	Patterson et al.
5,192,286 A	3/1993	Phan et al.	5,906,618 A	5/1999	Larson, III
5,195,955 A	3/1993	Don Michael	5,908,435 A	6/1999	Samuels
5,224,953 A	7/1993	Morgentaler	5,910,154 A	6/1999	Tsugita et al.
5,306,286 A	4/1994	Stack et al.	5,911,734 A	6/1999	Tsugita et al.
5,314,444 A	5/1994	Gianturco	5,916,193 A	6/1999	Stevens et al.
5,314,472 A	5/1994	Fontaine	5,922,020 A *	7/1999	Klein et al. 623/1.15
5,318,576 A	6/1994	Plassche, Jr. et al.	5,925,016 A	7/1999	Chornenky et al.
5,329,942 A	7/1994	Gunther et al.	5,925,060 A	7/1999	Forber
5,330,484 A	7/1994	Gunther	5,925,062 A	7/1999	Purdy
5,330,500 A	7/1994	Song	5,925,063 A	7/1999	Khosravi
5,350,398 A	9/1994	Pavcnik et al.	5,928,203 A	7/1999	Davey et al.
			5,928,218 A	7/1999	Gelbfish

US RE43,882 E

5,934,284	A	8/1999	Plaia et al.	EP	0200688	A1	11/1986
5,935,139	A	8/1999	Bates	EP	0 293 605	A1	12/1988
5,938,645	A	8/1999	Gordon	EP	0293605	A1	12/1988
5,941,869	A	8/1999	Patterson et al.	EP	0 411 118	A1	2/1991
5,941,896	A	8/1999	Kerr	EP	0411118	A1	2/1991
5,947,995	A	9/1999	Samuels	EP	0 427 429	A1	5/1991
5,951,585	A	9/1999	Cathcart et al.	EP	0427429	A1	5/1991
5,954,745	A	9/1999	Gertler et al.	EP	0 437 121	B1	7/1991
5,976,172	A	11/1999	Homsma et al.	EP	0437121	B1	7/1991
5,980,555	A	11/1999	Barbut et al.	EP	0 472 334	A1	2/1992
5,989,210	A	11/1999	Morris et al.	EP	0 472 368	A2	2/1992
5,989,271	A	11/1999	Bonnette et al.	EP	0472334	A1	2/1992
5,989,281	A	11/1999	Barbut et al.	EP	0472368	A2	2/1992
5,993,469	A	11/1999	McKenzie et al.	EP	0 533 511	A1	3/1993
5,997,557	A	12/1999	Barbut et al.	EP	0533511	A1	3/1993
6,001,118	A	12/1999	Daniel et al.	EP	0 655 228	A1	11/1994
6,007,557	A	12/1999	Ambrisco et al.	EP	0655228	A1	5/1995
6,010,522	A	1/2000	Barbut et al.	EP	0 686 379	A2	6/1995
6,013,085	A	1/2000	Howard	EP	0686379	A2	12/1995
6,027,520	A	2/2000	Tsugita et al.	EP	0 696 447	A2	2/1996
6,042,598	A	3/2000	Tsugita et al.	EP	0696447	A2	2/1996
6,051,014	A	4/2000	Jang	EP	0 737 450	A1	10/1996
6,051,015	A	4/2000	Maahs	EP	0737450	A1	10/1996
6,053,932	A	4/2000	Daniel et al.	EP	0 743 046	A1	11/1996
6,059,814	A	5/2000	Ladd	EP	0 759 287	A1	2/1997
6,066,149	A	5/2000	Samson et al.	EP	0759287	A1	2/1997
6,066,158	A	5/2000	Engelson et al.	EP	0 771 549	A2	5/1997
6,068,645	A	5/2000	Tu	EP	0771549	A2	5/1997
6,086,605	A	7/2000	Barbut et al.	EP	0 784 988	A1	7/1997
6,117,154	A	9/2000	Barbut et al.	EP	0784988	A1	7/1997
6,129,739	A	10/2000	Khosravi	EP	0 852 132	A1	7/1998
6,136,016	A	10/2000	Barbut et al.	EP	0852132	A1	7/1998
6,142,987	A	11/2000	Tsugita	EP	0 934 729		8/1999
6,152,946	A	11/2000	Broome et al.	EP	0934729	A	8/1999
6,165,200	A	12/2000	Tsugita et al.	EP	1 127 556	A2	8/2001
6,168,579	B1	1/2001	Tsugita	EP	1127556	A2	8/2001
6,168,604	B1 *	1/2001	Cano 606/114	EP	0743046	A1	6/2011
6,171,327	B1	1/2001	Daniel et al.	FR	2 580 504		10/1986
6,171,328	B1	1/2001	Addis	FR	2580504	A	10/1986
6,179,851	B1	1/2001	Barbut et al.	FR	2 643 250	A1	8/1990
6,179,859	B1	1/2001	Bates et al.	FR	2643250	A	8/1990
6,179,861	B1	1/2001	Khosravi et al.	FR	2 666 980		3/1992
6,187,025	B1 *	2/2001	Machek 606/200	FR	2666980	A	3/1992
6,203,561	B1	3/2001	Ramee et al.	FR	2 694 687		8/1992
6,206,868	B1	3/2001	Parodi	FR	2694687	A	2/1994
6,214,026	B1	4/2001	Lepak et al.	FR	2 768 326	A1	3/1999
6,221,006	B1	4/2001	Dubrul et al.	FR	2768326	A1	3/1999
6,224,620	B1	5/2001	Maahs	GB	2 020 557	B	11/1979
6,231,544	B1	5/2001	Tsugita et al.	GB	2020557	B	11/1979
6,235,044	B1	5/2001	Root et al.	JP	8-187294	A	7/1996
6,235,045	B1	5/2001	Barbut et al.	JP	8187294	A	7/1996
6,238,412	B1	5/2001	Dubrul et al.	SU	764684		9/1980
6,245,087	B1	6/2001	Addis	SU	764684	A	9/1980
6,245,088	B1	6/2001	Lowery	WF	WO 97/27808		8/1997
6,245,089	B1	6/2001	Daniel et al.	WO	9203097	A1	3/1992
6,258,115	B1	7/2001	Dubrul	WO	WO 92/03097		3/1992
6,264,663	B1	7/2001	Cano	WO	9414389	A1	7/1994
6,264,672	B1	7/2001	Fisher	WO	WO 94/14389		7/1994
6,270,513	B1	8/2001	Tsugita et al.	WO	9424946	A1	11/1994
6,277,138	B1	8/2001	Levinson et al.	WO	WO 94/24946		11/1994
6,277,139	B1	8/2001	Levinson et al.	WO	9601591	A1	1/1996
6,280,413	B1	8/2001	Clark et al.	WO	WO 96/01591		1/1996
6,287,321	B1	9/2001	Jang	WO	9610375	A1	4/1996
6,290,710	B1	9/2001	Cryer et al.	WO	WO 96/10375		4/1996
6,309,399	B1	10/2001	Barbut et al.	WO	9619941	A1	7/1996
6,319,268	B1	11/2001	Ambrisco et al.	WO	WO 96/19941		7/1996
6,336,934	B1 *	1/2002	Gilson et al. 606/200	WO	9623441	A1	8/1996
6,344,049	B1	2/2002	Levinson et al.	WO	WO 96/23441		8/1996
6,511,492	B1 *	1/2003	Rosenbluth et al. 606/159	WO	9633677	A1	10/1996
				WO	WO 96/33677		10/1996
				WO	9717100	A1	5/1997
				WO	WO 97/17100		5/1997
DE	28 21 048	7/1980		WO	9727808	A1	8/1997
DE	34 17 738	11/1985		WO	9742879	A1	11/1997
DE	3417738	A	11/1985	WO	WO 97/42879		11/1997
DE	40 30 998	A1	10/1990	WO	9802084	A3	1/1998
DE	4030998	A	4/1991	WO	9802112	A1	1/1998
DE	199 16 162		10/2000	WO	WO 98/02084		1/1998
DE	19916162	A	10/2000	WO	WO 98/02112		1/1998
EP	0 200 688		11/1986	WO			

FOREIGN PATENT DOCUMENTS

WO	9823322	A1	6/1998
WO	WO 98/23322		6/1998
WO	9833443	A1	8/1998
WO	9834673	A1	8/1998
WO	9836786	A1	8/1998
WO	WO 98/33443		8/1998
WO	WO 98/34673		8/1998
WO	WO 98/36786		8/1998
WO	9838920	A1	9/1998
WO	9838929	A1	9/1998
WO	9839046	A1	9/1998
WO	9839053	A1	9/1998
WO	WO 98/38920		9/1998
WO	WO 98/38929		9/1998
WO	WO 98/39046		9/1998
WO	WO 98/39053		9/1998
WO	9846297	A1	10/1998
WO	9847447	A1	10/1998
WO	WO 98/46297		10/1998
WO	WO 98/47447		10/1998
WO	9849952	A1	11/1998
WO	9850103	A1	11/1998
WO	9851237	A1	11/1998
WO	WO 98/49952		11/1998
WO	WO 98/50103		11/1998
WO	WO 98/51237		11/1998
WO	9855175	A1	12/1998
WO	WO 98/55175		12/1998
WO	9909895	A1	3/1999
WO	WO 99/09895		3/1999
WO	9922673	A1	5/1999
WO	9923976	A1	5/1999
WO	9925252	A1	5/1999
WO	WO 99/22673		5/1999
WO	WO 99/23976		5/1999
WO	WO 99/25252		5/1999
WO	9930766	A1	6/1999
WO	WO 99/30766		6/1999
WO	9940964	A1	8/1999
WO	9942059	A1	8/1999
WO	WO 99/40964		8/1999
WO	WO 99/42059		8/1999
WO	9944510	A1	9/1999
WO	9944542	A1	9/1999
WO	WO 99/44510		9/1999
WO	WO 99/44542		9/1999
WO	WO9944535	*	9/1999
WO	9955236	A1	11/1999
WO	9958068	A1	11/1999
WO	WO 99/55236		11/1999
WO	WO 99/58068		11/1999
WO	0007521	A1	2/2000
WO	0007655	A1	2/2000
WO	0009054	A1	2/2000
WO	WO 00/07521		2/2000
WO	WO 00/07655		2/2000
WO	WO 00/09054		2/2000
WO	0016705	A1	3/2000
WO	WO 00/16705		3/2000
WO	0049970	A1	8/2000
WO	WO 00/49970		8/2000
WO	0053120	A1	9/2000
WO	WO 00/53120		9/2000
WO	0067664	A1	11/2000
WO	0067665	A1	11/2000
WO	0067666	A1	11/2000
WO	0067668	A1	11/2000
WO	0067669	A1	11/2000
WO	WO 00/67664		11/2000
WO	WO 00/67665		11/2000
WO	WO 00/67666		11/2000
WO	WO 00/67668		11/2000
WO	WO 00/67669		11/2000
WO	0105462	A1	1/2001
WO	WO 01/05462		1/2001
WO	0108595	A1	2/2001
WO	0108596	A1	2/2001
WO	0108742	A1	2/2001
WO	0108743	A1	2/2001

WO	0110320	A1	2/2001
WO	WO 01/08595		2/2001
WO	WO 01/08596		2/2001
WO	WO 01/08742		2/2001
WO	WO 01/08743		2/2001
WO	WO 01/10320		2/2001
WO	0115629	A1	3/2001
WO	0121077	A1	3/2001
WO	0121100	A1	3/2001
WO	WO 01/15629		3/2001
WO	WO 01/21077		3/2001
WO	WO 01/21100		3/2001
WO	0126726	A1	4/2001
WO	WO 01/26726		4/2001
WO	0135857	A1	5/2001
WO	WO 01/35857		5/2001
WO	0143662	A1	6/2001
WO	WO 01/43662		6/2001
WO	0147579	A1	7/2001
WO	0149208	A1	7/2001
WO	0149209	A1	7/2001
WO	0149215	A1	7/2001
WO	0149355	A1	7/2001
WO	0152768	A1	7/2001
WO	WO 01/47579		7/2001
WO	WO 01/49208		7/2001
WO	WO 01/49209		7/2001
WO	WO 01/49215		7/2001
WO	WO 01/49355		7/2001
WO	WO 01/52768		7/2001
WO	0158382	A1	8/2001
WO	0160442	A1	8/2001
WO	WO 01/58382		8/2001
WO	WO 01/60442		8/2001
WO	0167989	A1	9/2001
WO	0170326	A1	9/2001
WO	WO 01/67989		9/2001
WO	WO 01/70326		9/2001
WO	0172205	A2	10/2001
WO	WO 01/72205		10/2001
WO	0187183	A3	11/2001
WO	0189413	A3	11/2001
WO	WO 01/87183		11/2001
WO	WO 01/89413		11/2001
WO	0191824	A2	12/2001
WO	WO 01/91824		12/2001

OTHER PUBLICATIONS

"Endovascular Grafts, Stents Drive Interventional Radiology Growth," *Cardiovascular Device Update*, 2(3):1-12 (Mar. 1996).

"Protruding Atheromas in the Thoracic Aortic and Systemic Embolization," *American College of Physicians*, pp. 423-427(1991).

"Recognition and Embolic Potential of Intraaortic Atherosclerotic Debris," *American College of Cardiology* (Jan. 1991).

Cragg, Andrew et al., "A New Percutaneous Vena Cava Filter," *AJR*, 141:601-604 (Sep. 1983).

Cragg, Andrew et al., "Nonsurgical Placement of Arterial Endoprosthesis: A New Technique Using Nitinol Wire," *AJR*, pp. 261-263 (Apr. 1983).

Diethrich et al., "Percutaneous Techniques for Endoluminal Carotid Interventions," *Journal of Endovascular Surgery*, 3:182-202 (1996).

Fadali, A. Moneim, "A filtering device for the prevention of particulate embolization during the course of cardiac surgery", *Surgery*, 64(3), pp. 634-639 (Sep. 1968).

Haissaguerre et al., "Spontaneous Initiation of Atrial Fibrillation by Ectopic Beats Originating in the Pulmonary Veins," *The New England Journal of Medicine*, 339(10):659-666 (Sep. 1988).

Jordan, Jr. et al., "Microemboli Detected by Transcranial Doppler Monitoring . . .," *Cardiovascular Surgery*, 7(1):33-38 (Jan. 1999).

Lesh, "Can Catheter Ablation Cure Atrial Fibrillation?" *ACC Current Journal Review*, pp. 38-40 (Sep./Oct. 1997).

Lund et al., "Long-Term Patency of Ductus Arteriosus After Balloon Dilatation: an Experimental Study," *Laboratory Investigation*, 69(4):772-774 (Apr. 1984).

Marache et al., "Percutaneous Transluminal Venous Angioplasty . . .," *American Heart Journal*, 125(2 Pt 1):362-366 (Feb. 1993).

- Mazur et al., "Directional Atherectomy with the Omnicath.TM.: A Unique New Catheter System," *Catheterization and Cardiovascular Diagnosis*, 31:17-84 (1994).
- Moussa, MD, Issaam "Stents Don't Require Systemic Anticoagulation . . . But the Technique (and Results) Must be Optimal," *Journal of Invasive Cardiol.*, 8(E):3E-7E, (1996).
- Nakanishi et al., "Catheter Intervention to Venous System Using Expandable Metallic Stents," *Rinsho Kyobu Geka*, 14 (2): English Abstract Only (Apr. 1994).
- Onal et al., "Primary Stenting for Complex Atherosclerotic Plaques in Aortic and Iliac Stenoses," *Cardiovascular & Interventional Radiology*, 21(5):386-392 (1998).
- Theron et al., "New Triple Coaxial Catheter System for Carotid Angioplasty with Cerebral Protection," *American Journal of Neuroradiology*, 11:869-874 (1990).
- Tunick et al., "Protruding atherosclerotic plaque in the aortic arch of patients with systemic embolization: A new finding seen by transesophageal echocardiography," *American Heart Journal*, 120(3):658-660 (Sep. 1990).
- Waksman et al., "Distal Embolization is Common After Directional Atherectomy . . .," *American Heart Journal*, 129 (3):430-435 (1995).
- Wholey, Mark H. et al., "PTA and Stents in the Treatment of Extracranial Circulation," *The Journal of Invasive Cardiology*, Health Management Publications, Inc., vol. 8 Supplement E, pp. 25E-30E (1996).
- Wholey, Mark H. et al., "PTA and Stents in the Treatment of Extracranial Circulation," *The Journal of Invasive Cardiology*: vol. 8/Supplement E, Health Management Publications, Inc., 1996, pp. 25E-30E.
- Fadali, A. Moneim, "A filtering device for the prevention of particulate embolization during the course of cardiac surgery", *Surgery*, vol. 64(3), pp. 634-639 (Sep. 1968).
- "Protruding Atheromas in the Thoracic Aortic and Systemic Embolization," pp. 423-427 American College of Physicians (1991).
- "Recognition and Embolic Potential of Intraaortic Atherosclerotic Debris," *American College of Cardiology* (Jan. 1991).
- Diethrich et al., "Percutaneous Techniques for Endoluminal Carotid Interventions," *J. Endovasc. Surg.*, 3:182-202 (1996).
- Lund et al., "Long-Term Patency of Ductus Arteriosus After Balloon Dilation: an Experimental Study," *Laboratory Investigation*, 69 (4):772-774 (Apr. 1984).
- Mazur et al., "Directional Atherectomy with the Omnicath™: A Unique New Catheter System," *Catheterization and Cardiovascular Diagnosis*, 31:17-84 (1994).
- Nakanishi et al., "Catheter Intervention to Venous System Using Expandable Metallic Stents," *Rinsho Kyobu Geka*, 14(2): English Abstract Only (Apr. 1994).
- Onal et al., "Primary Stenting for Complex Atherosclerotic Plaques in Aortic and Iliac Stenoses," *Cardiovascular & Interventional Radiology*, 21(5):386-392(1998).
- Theron et al., "New Triple Coaxial Catheter System for Carotid Angioplasty with Cerebral Protection," *American Journal of Neuroradiology*, 11:869-874 (1990).
- Tunick et al., "Protruding atherosclerotic plaque in the aortic arch of patients with systemic embolization: A new finding seen by transesophageal echocardiography," *American Heart Journal* 120(3):658-660 (Sep. 1990).
- Waksman et al., "Distal Embolization is Common After Directional Atherectomy . . .," *American Heart Journal*, 129(3):430-435 (1995).

* cited by examiner

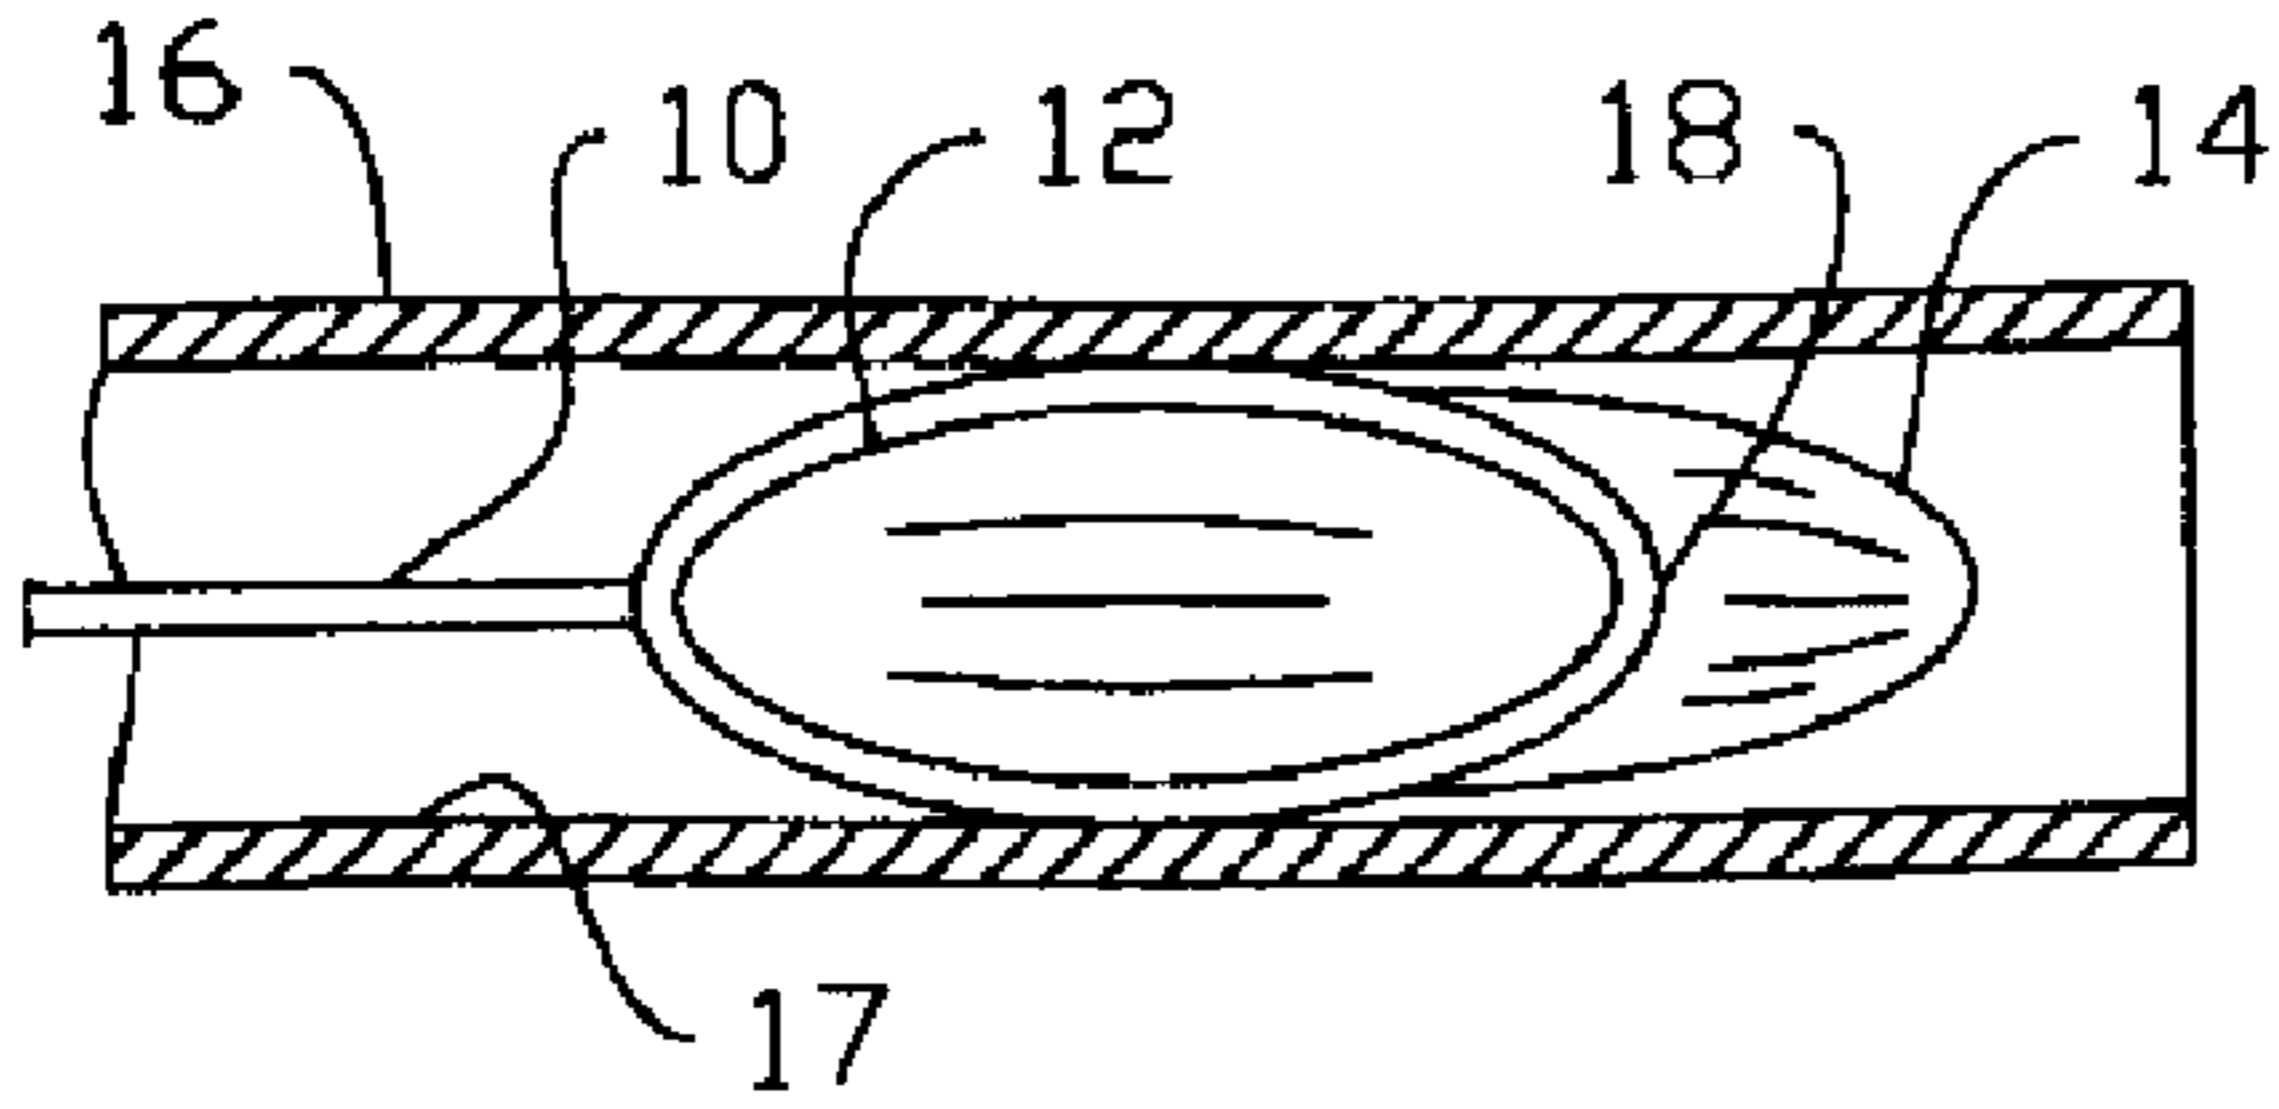


FIG. 1A (PRIOR ART)

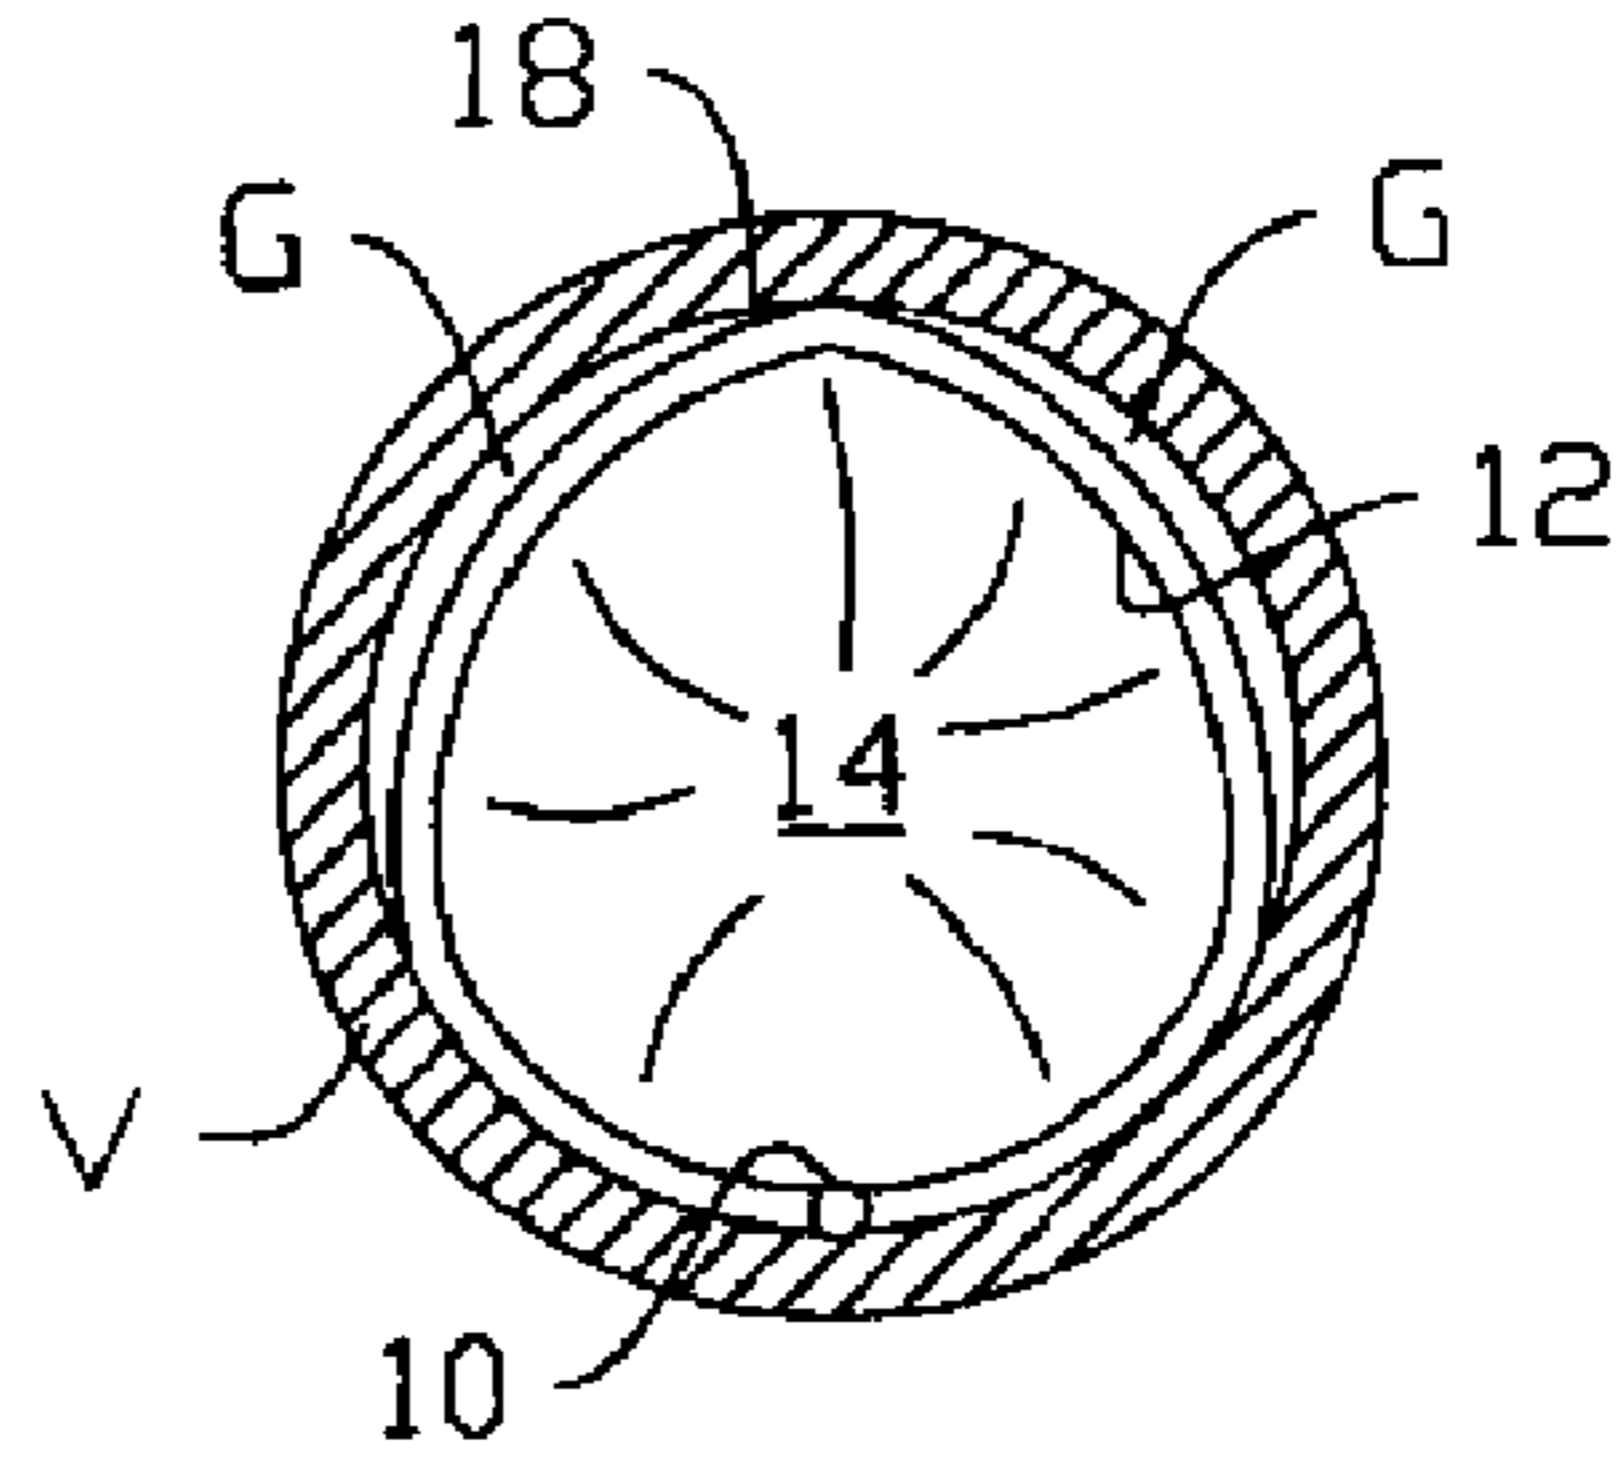


FIG. 1B (PRIOR ART)

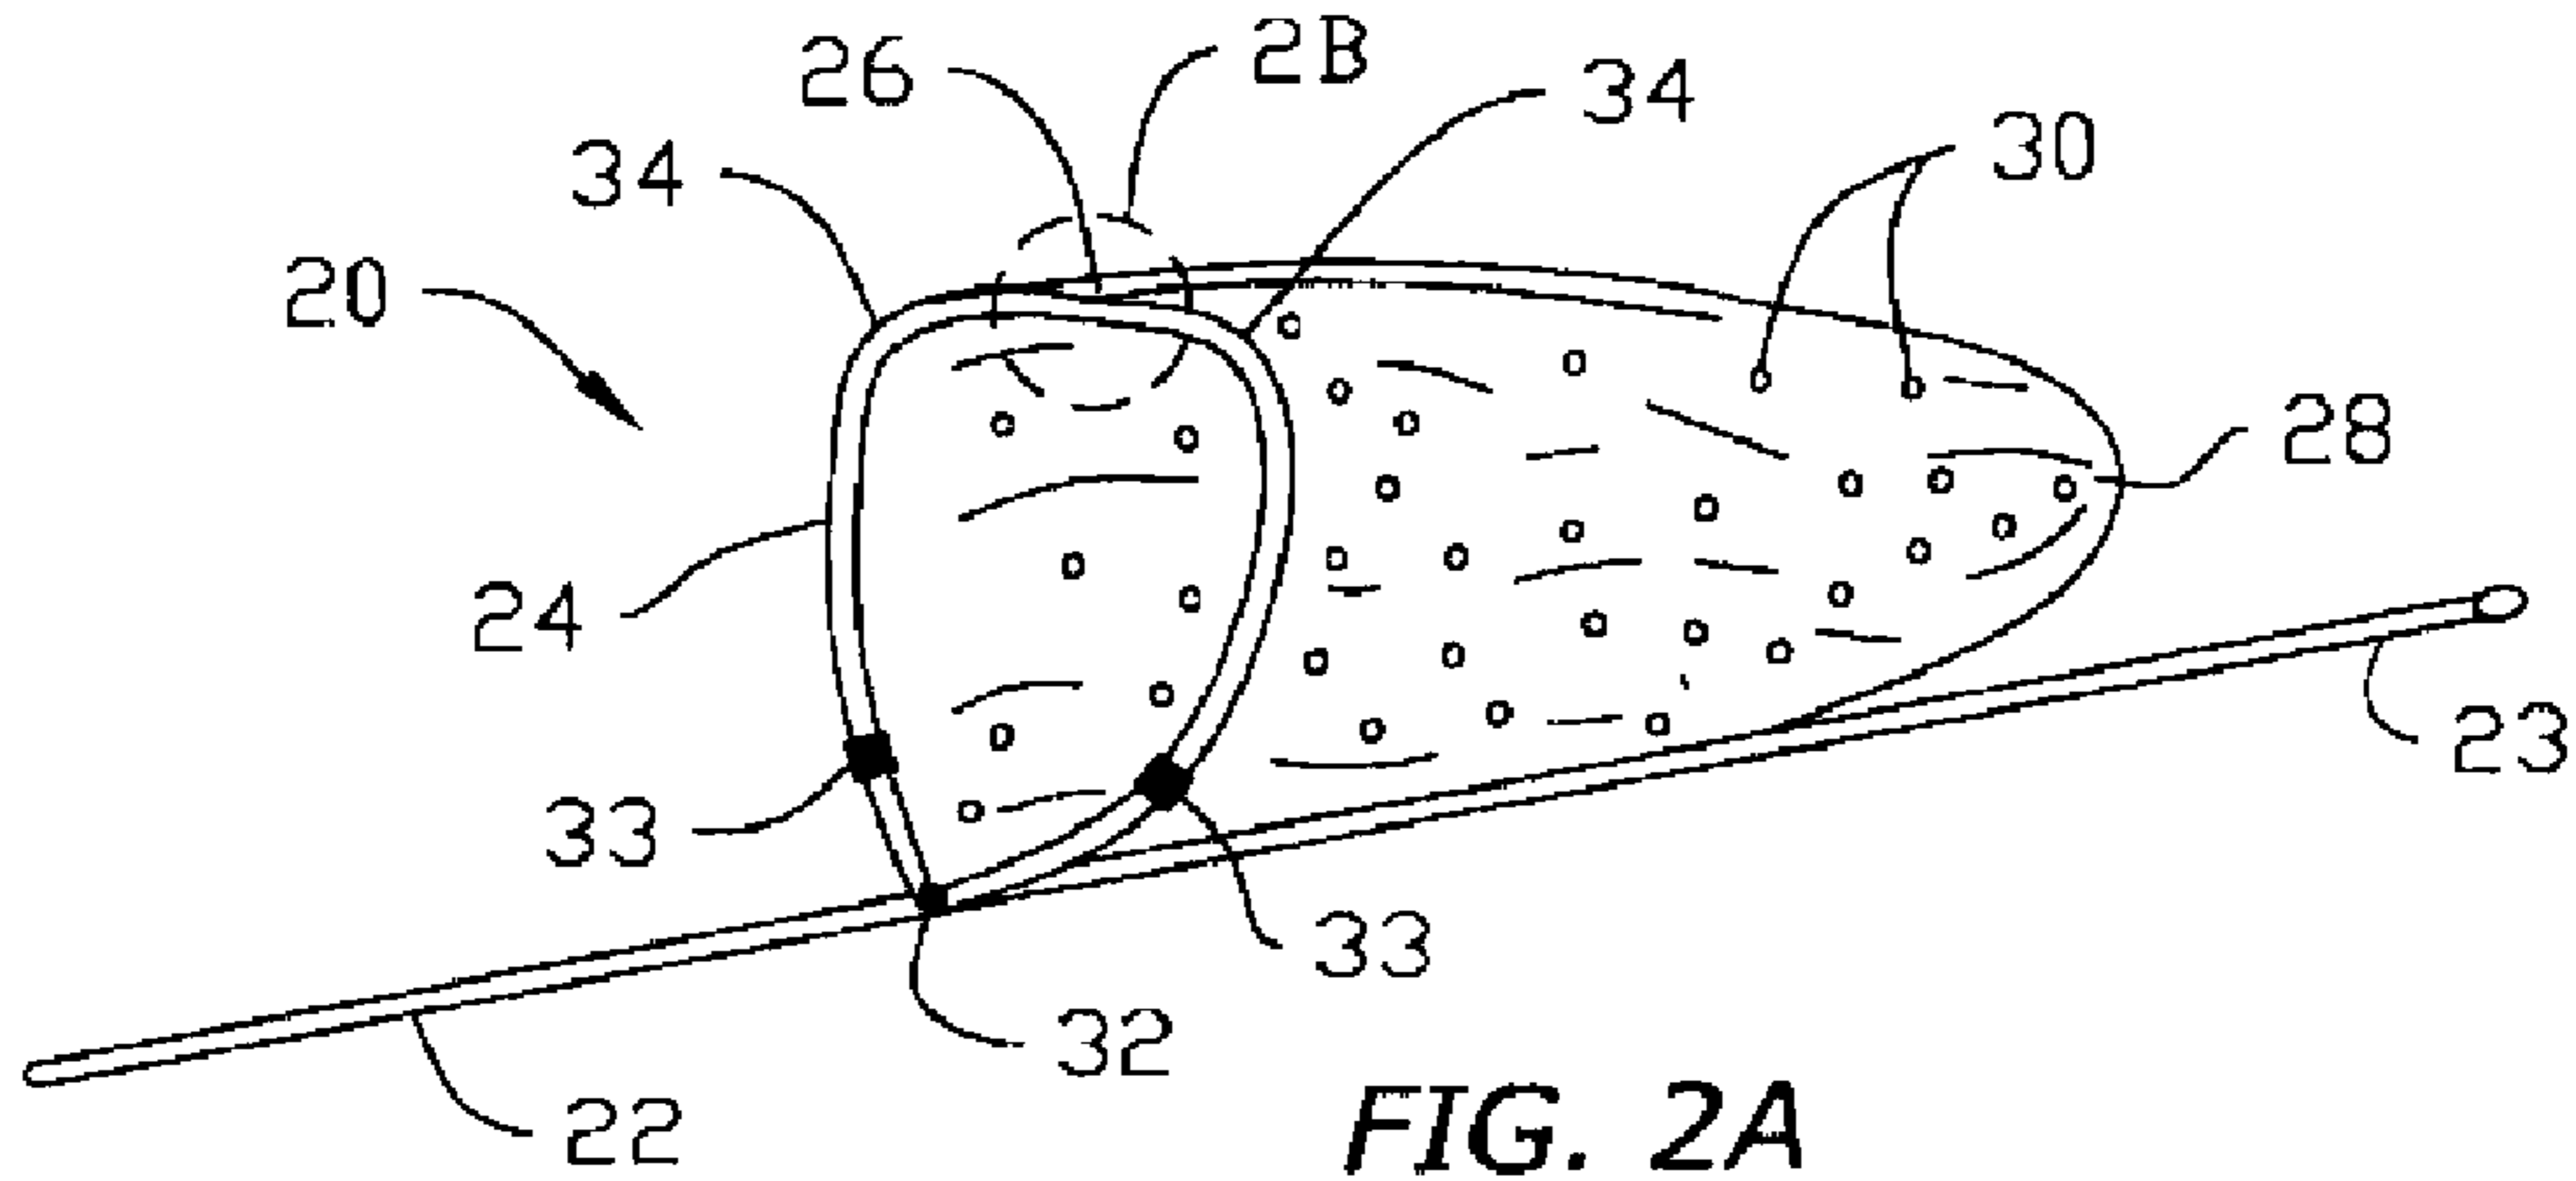


FIG. 2A

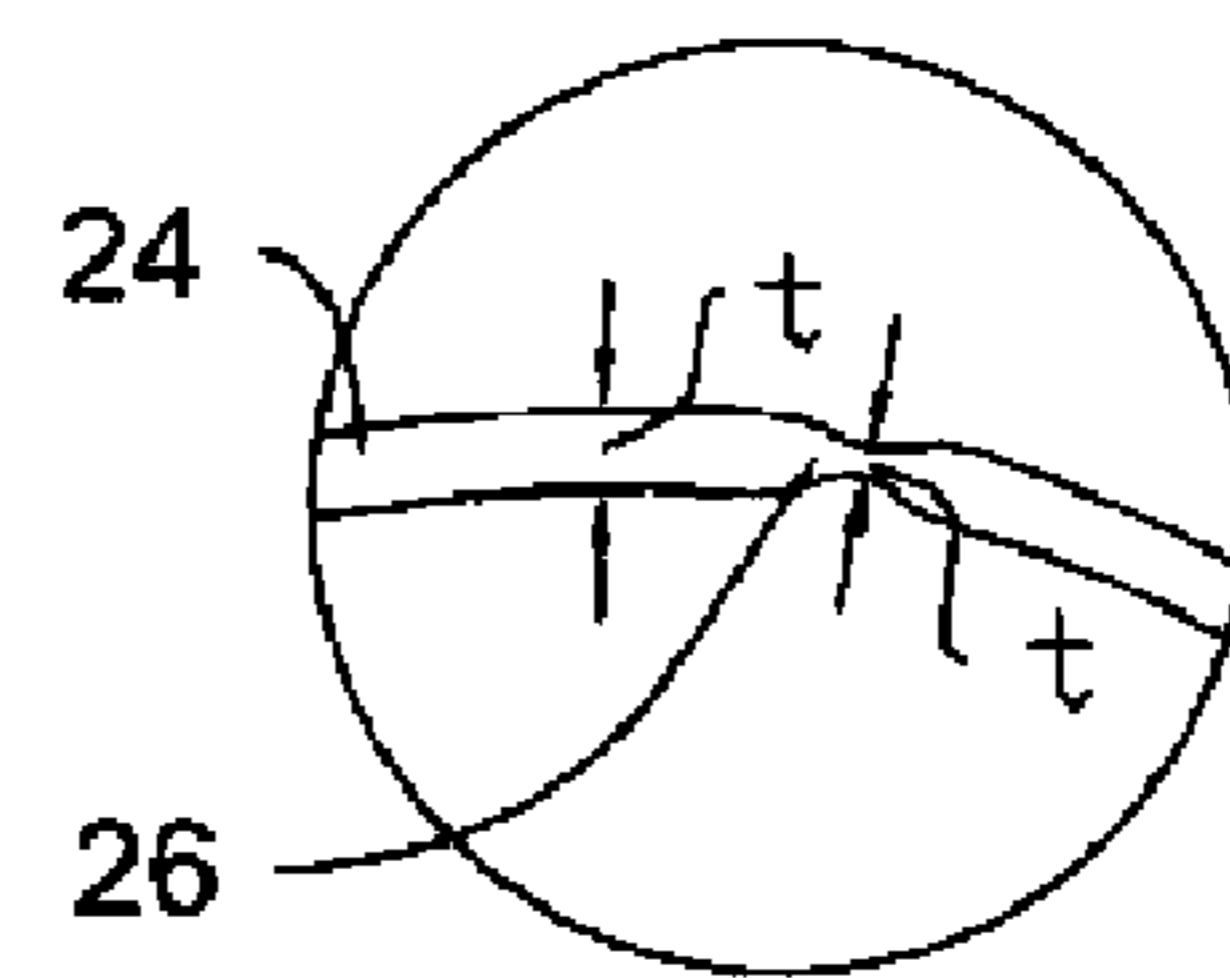


FIG. 2B

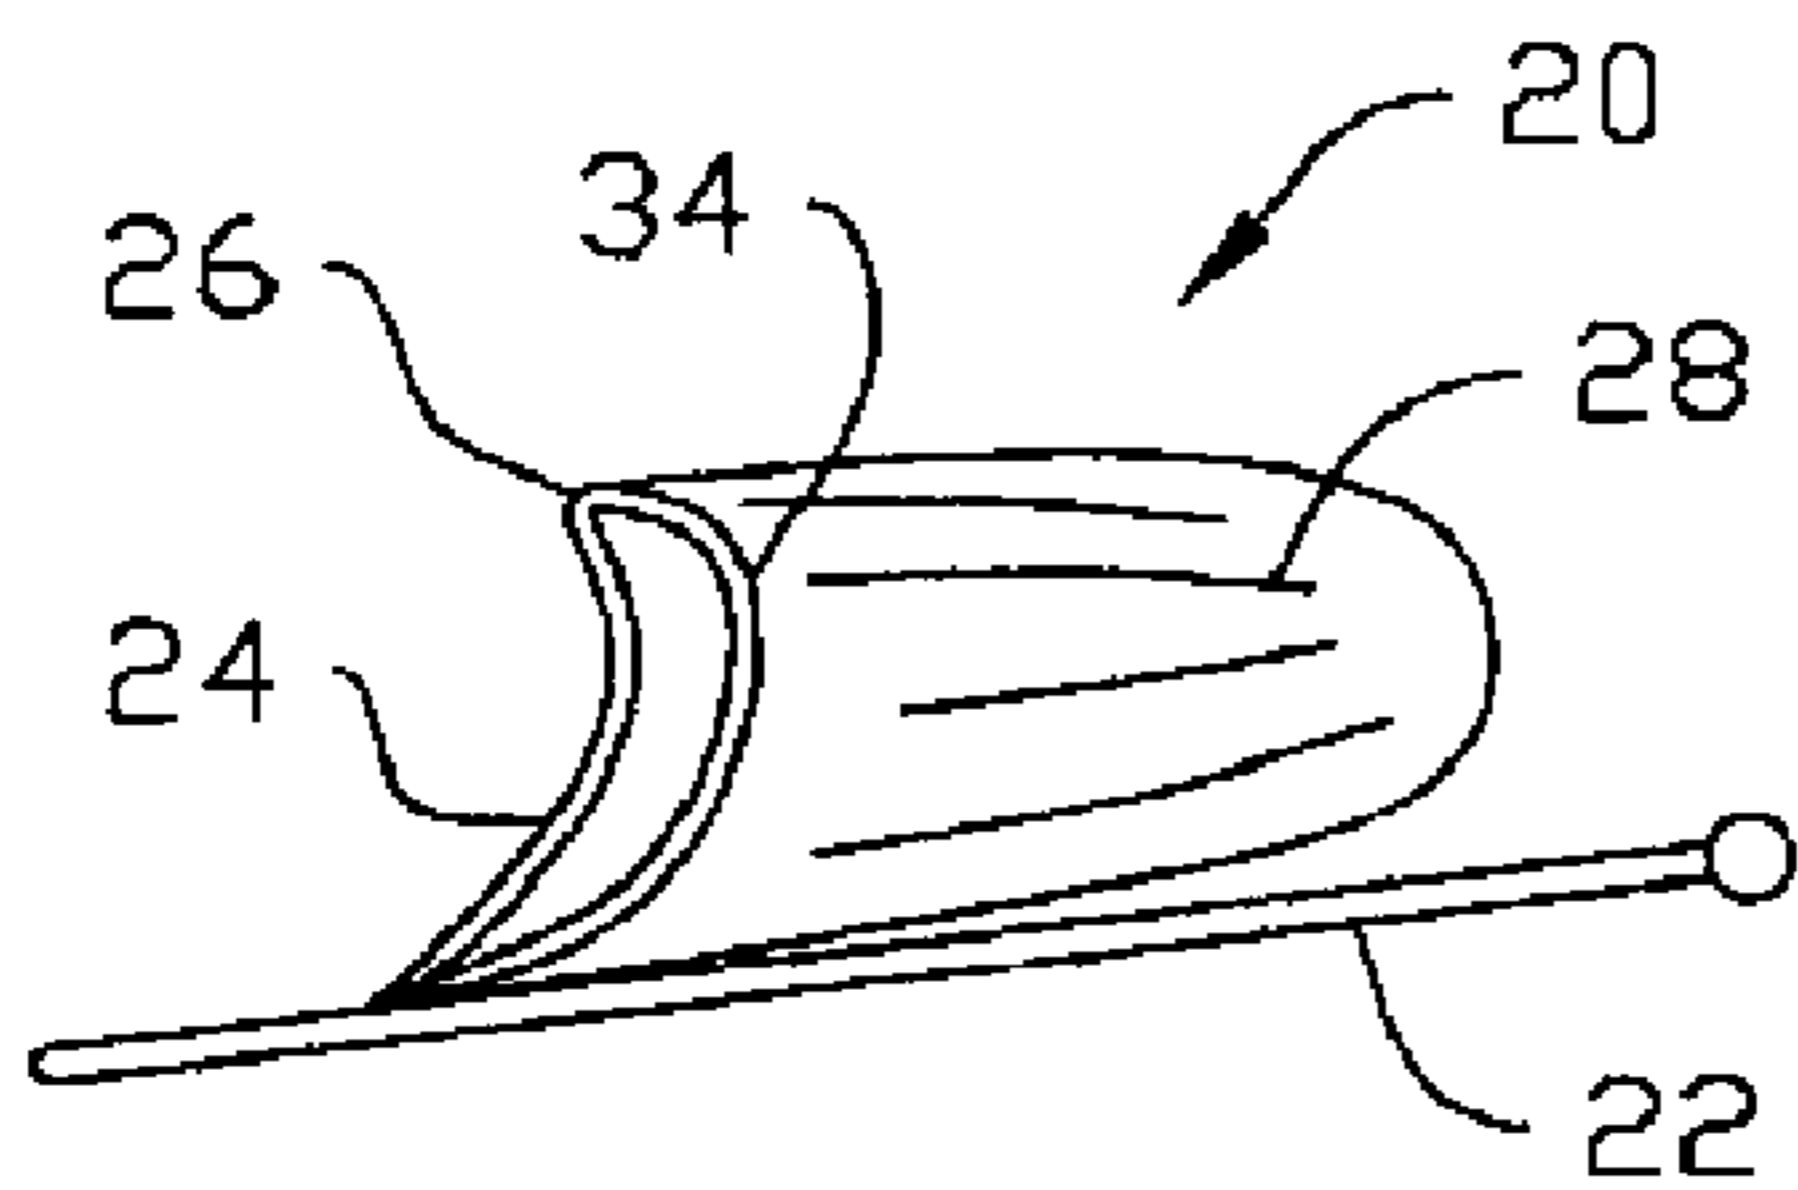


FIG. 3

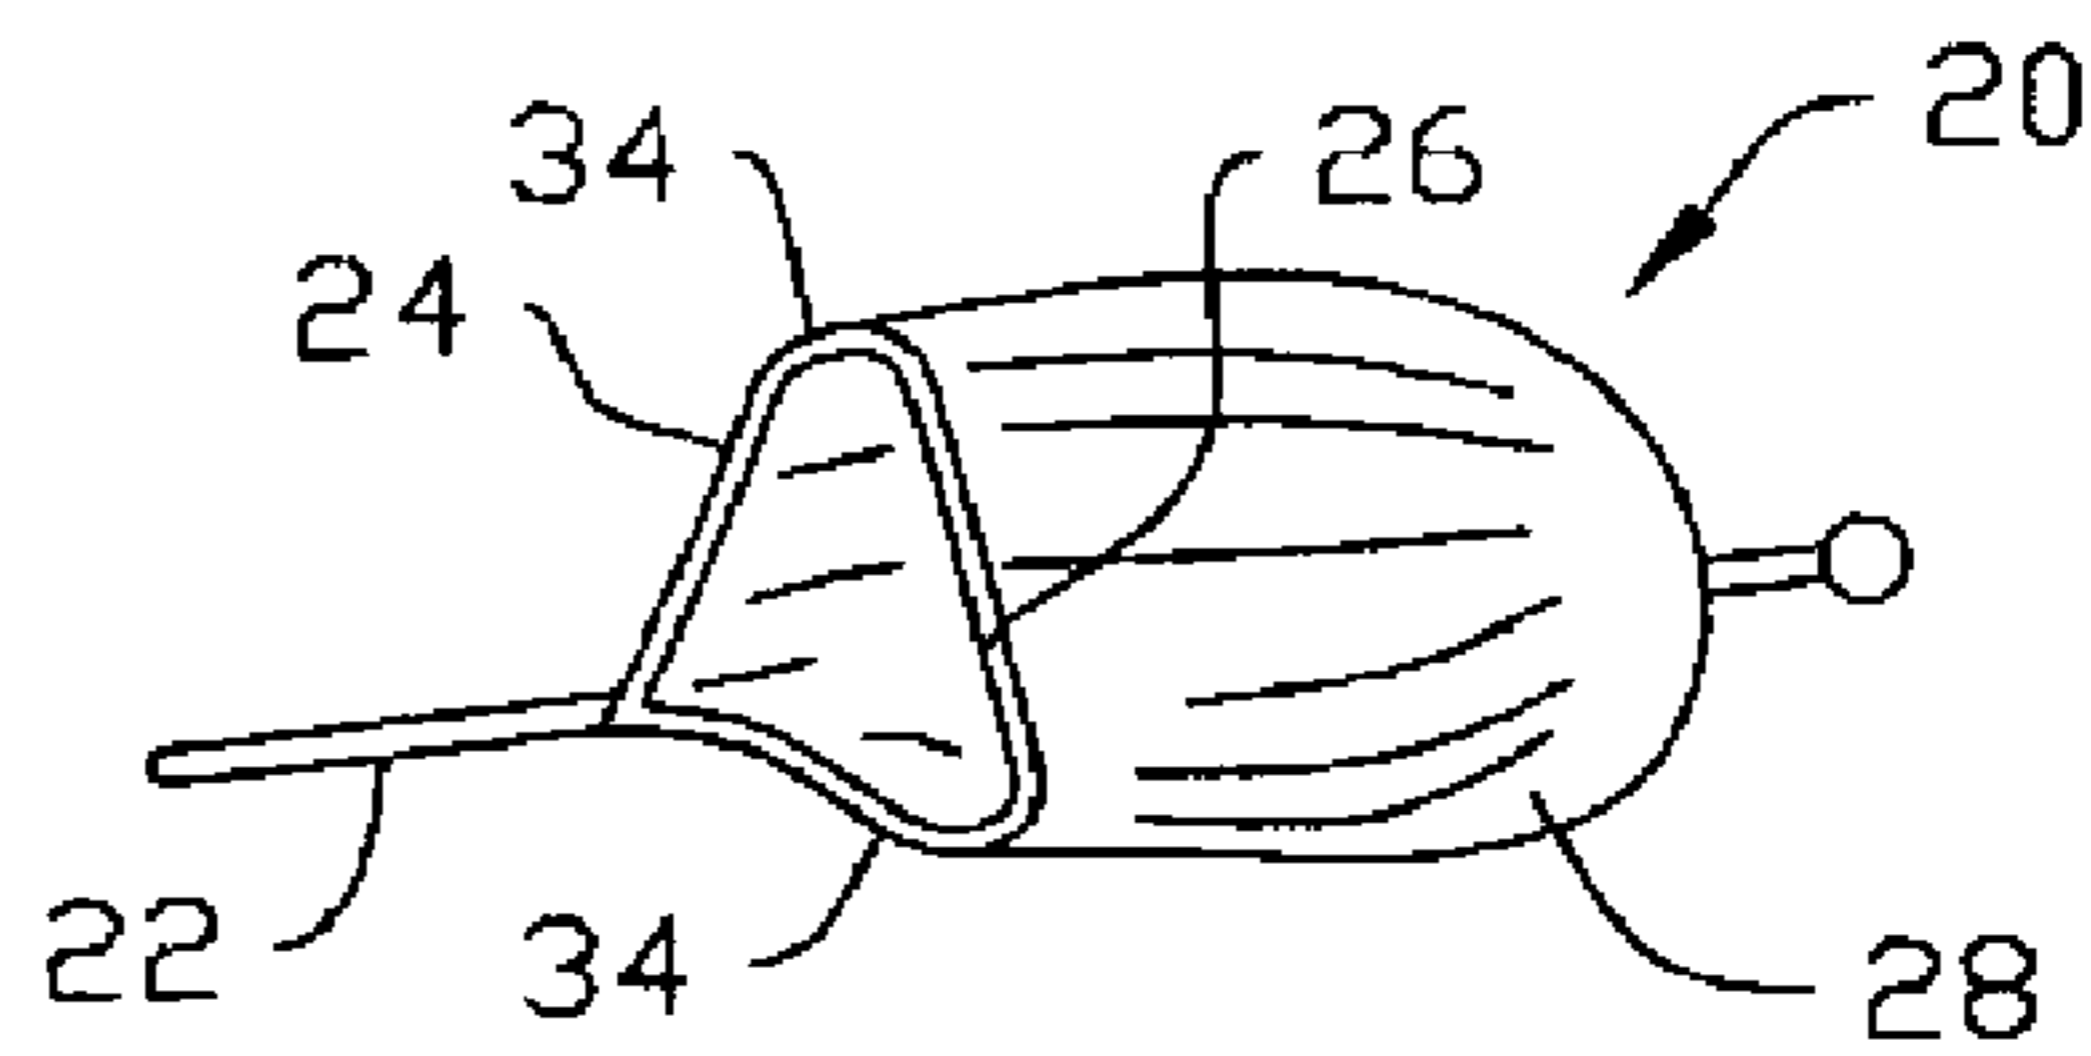
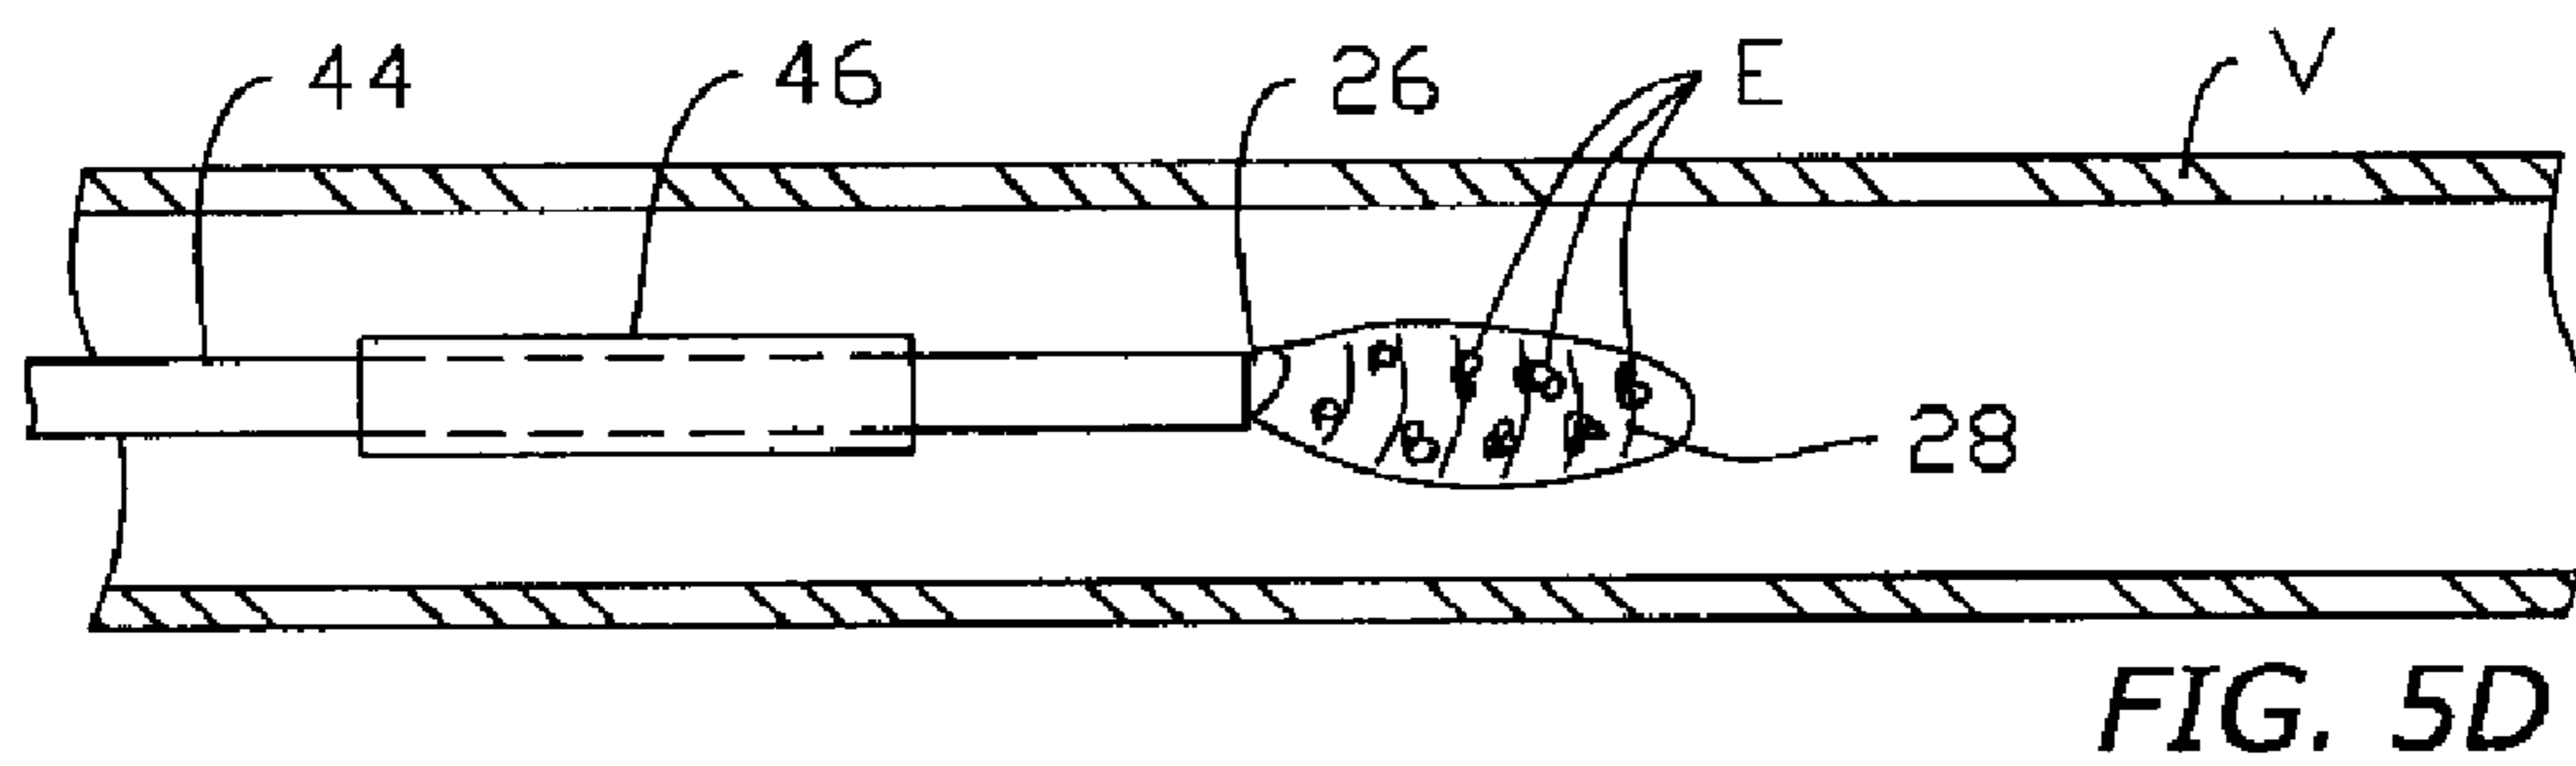
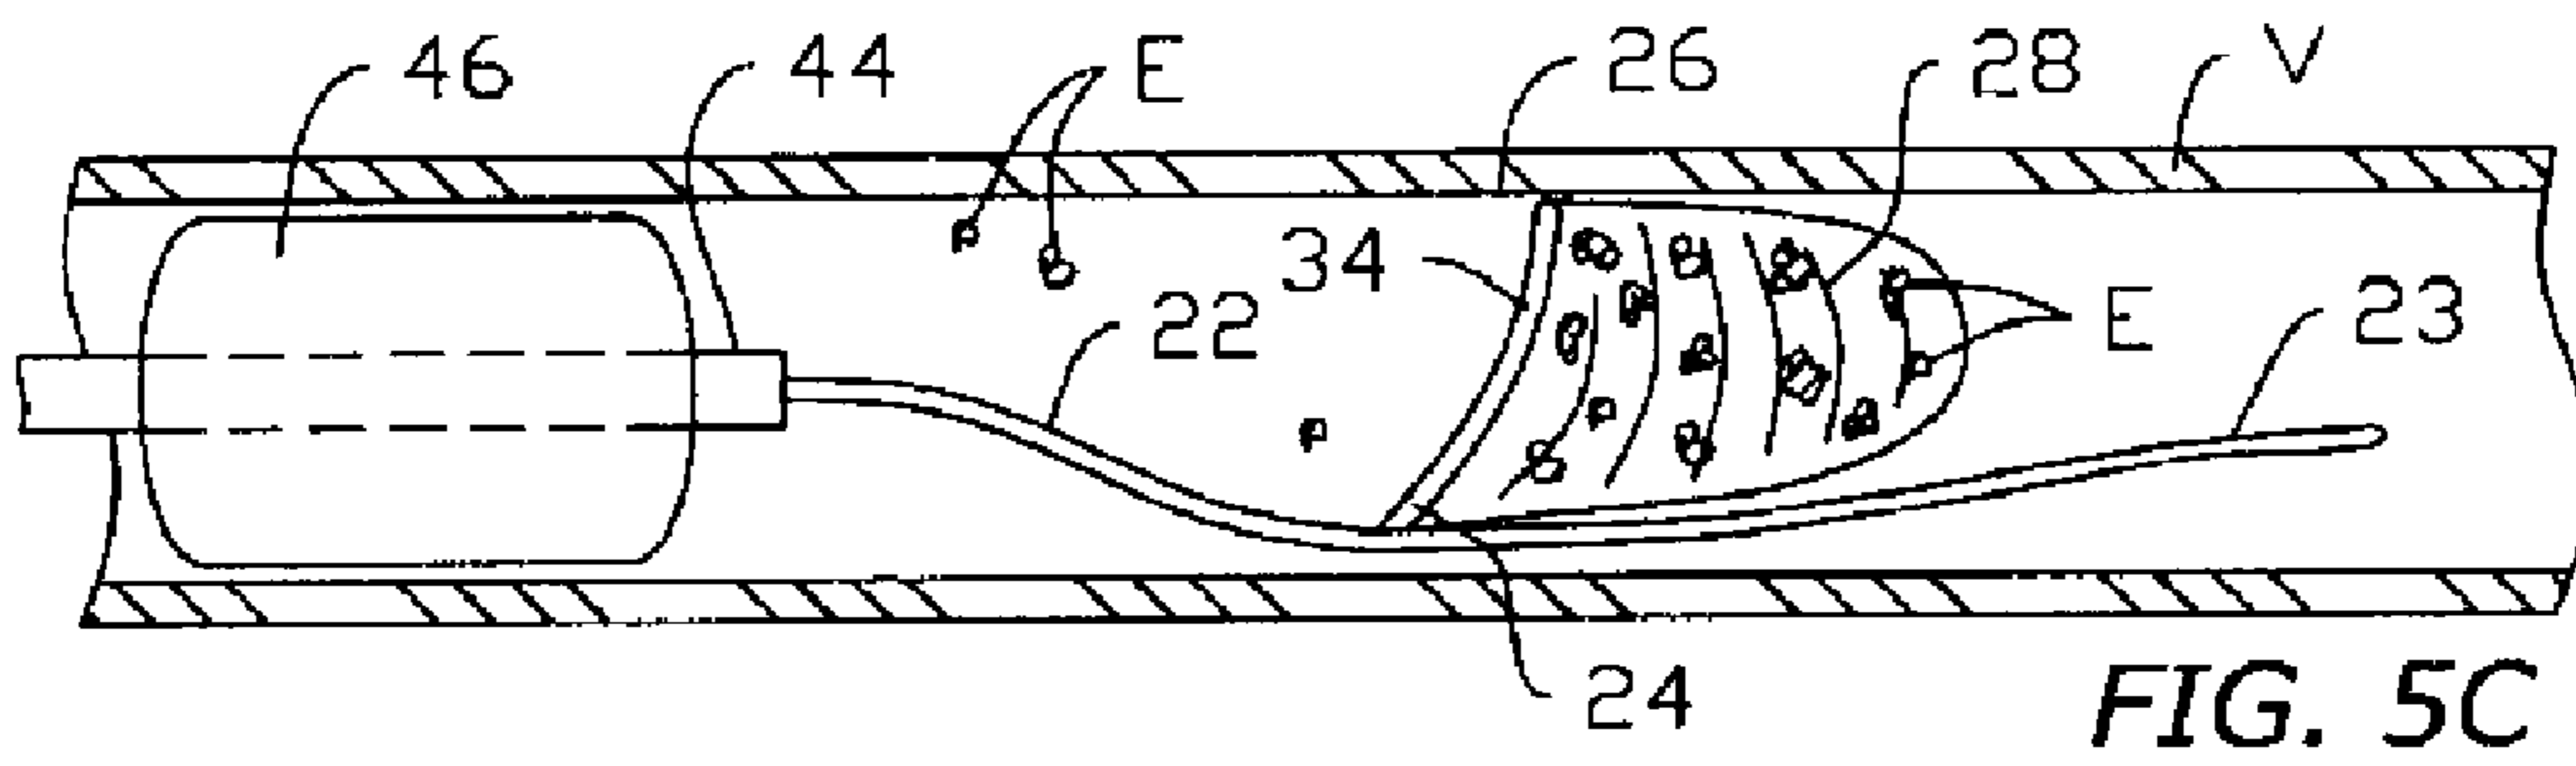
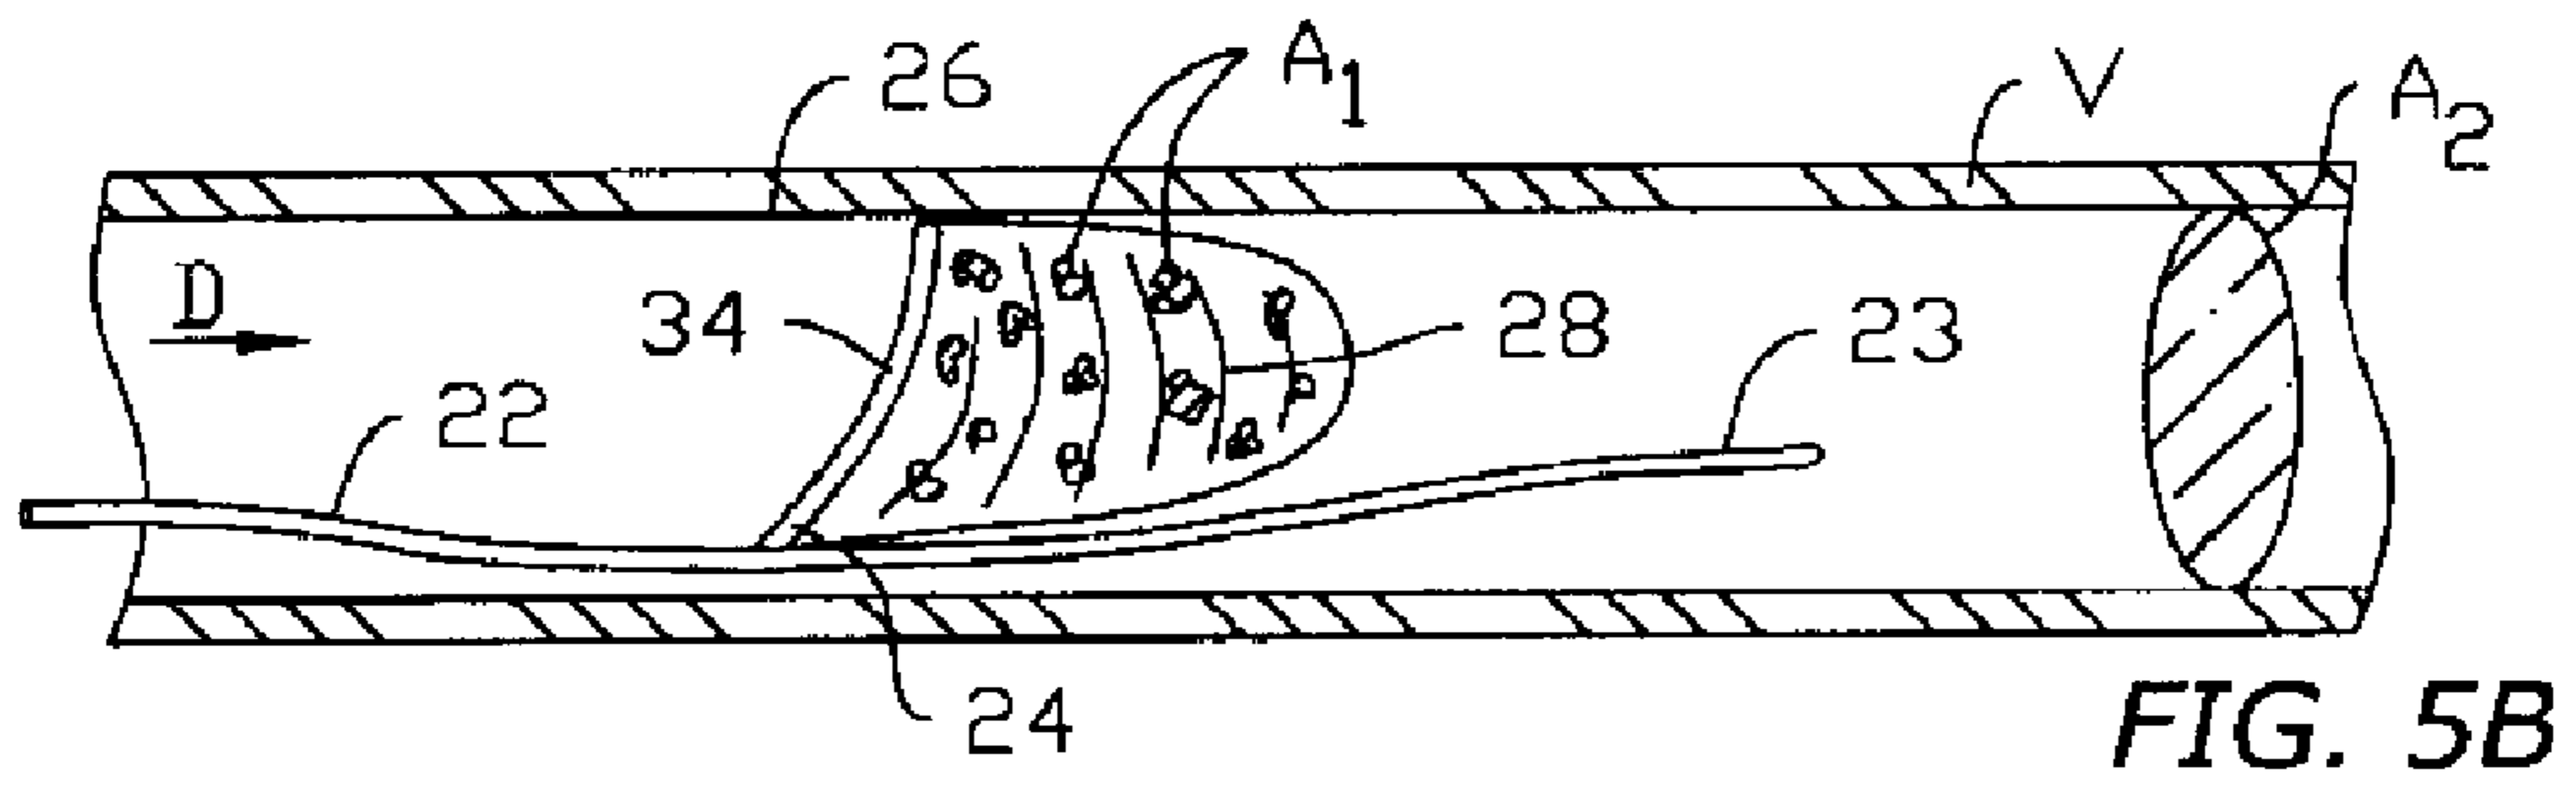
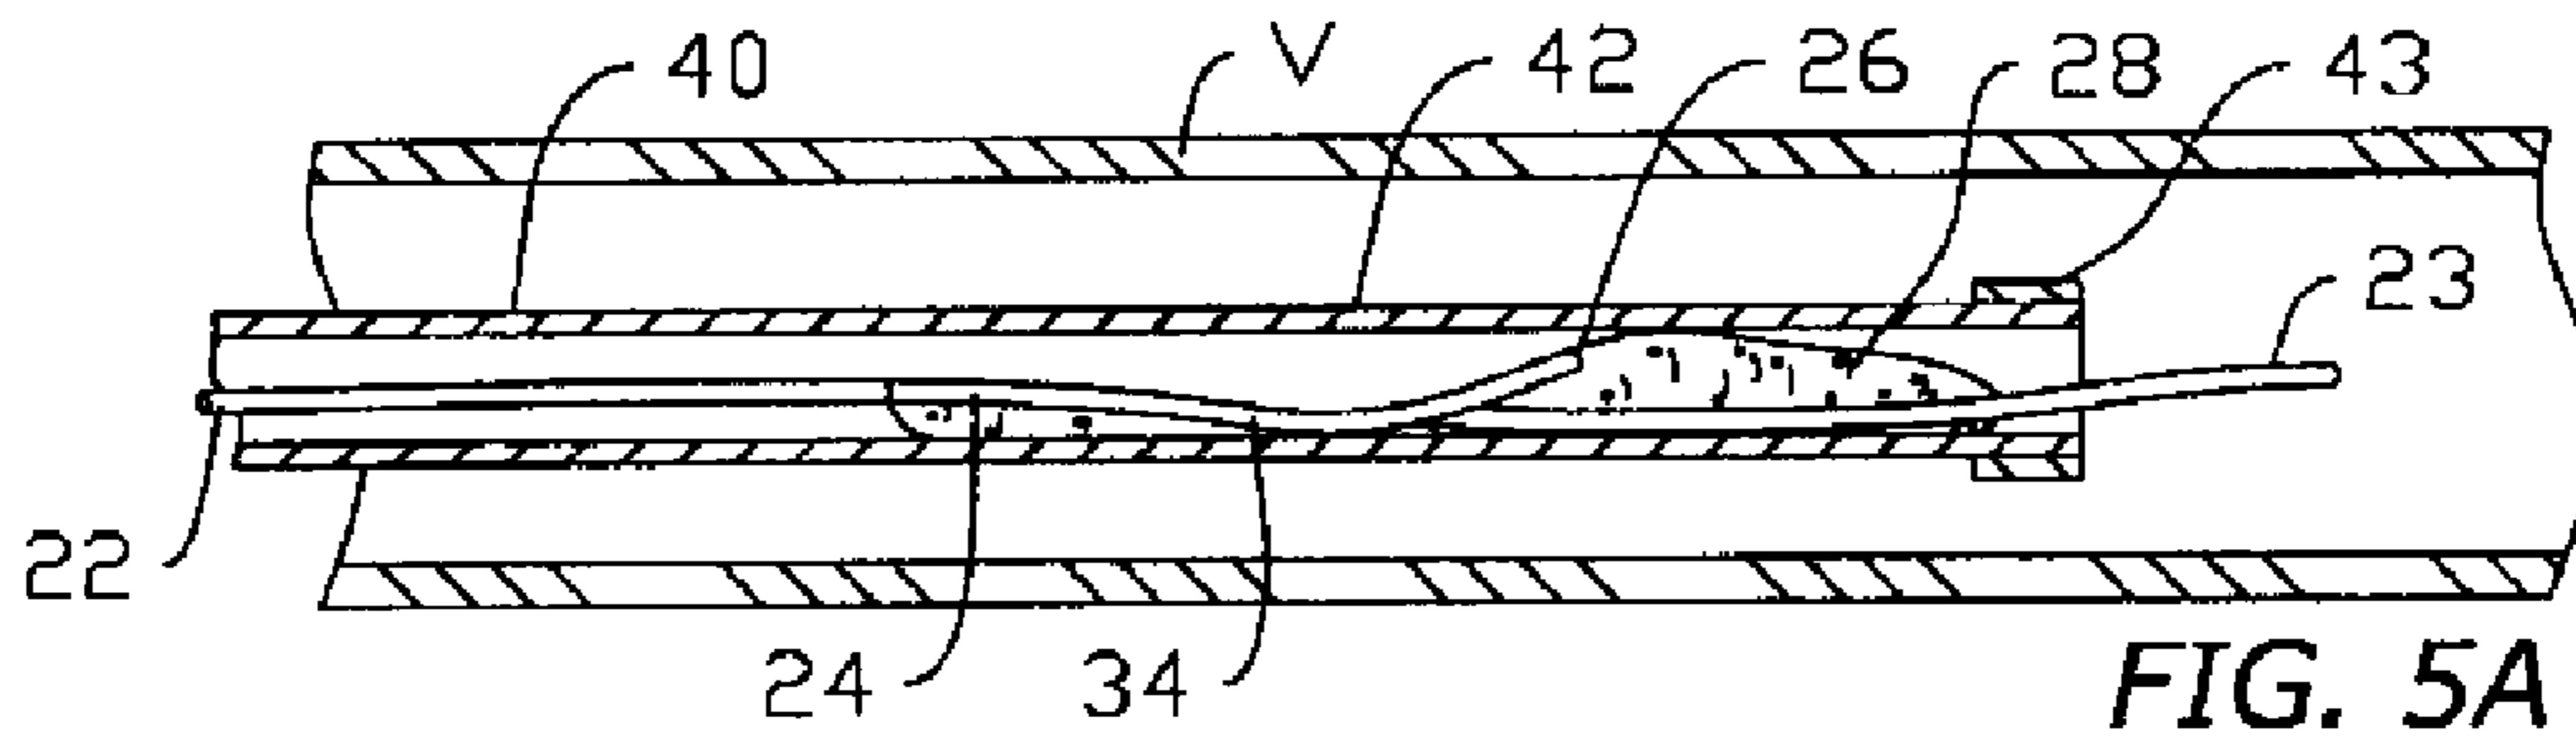


FIG. 4



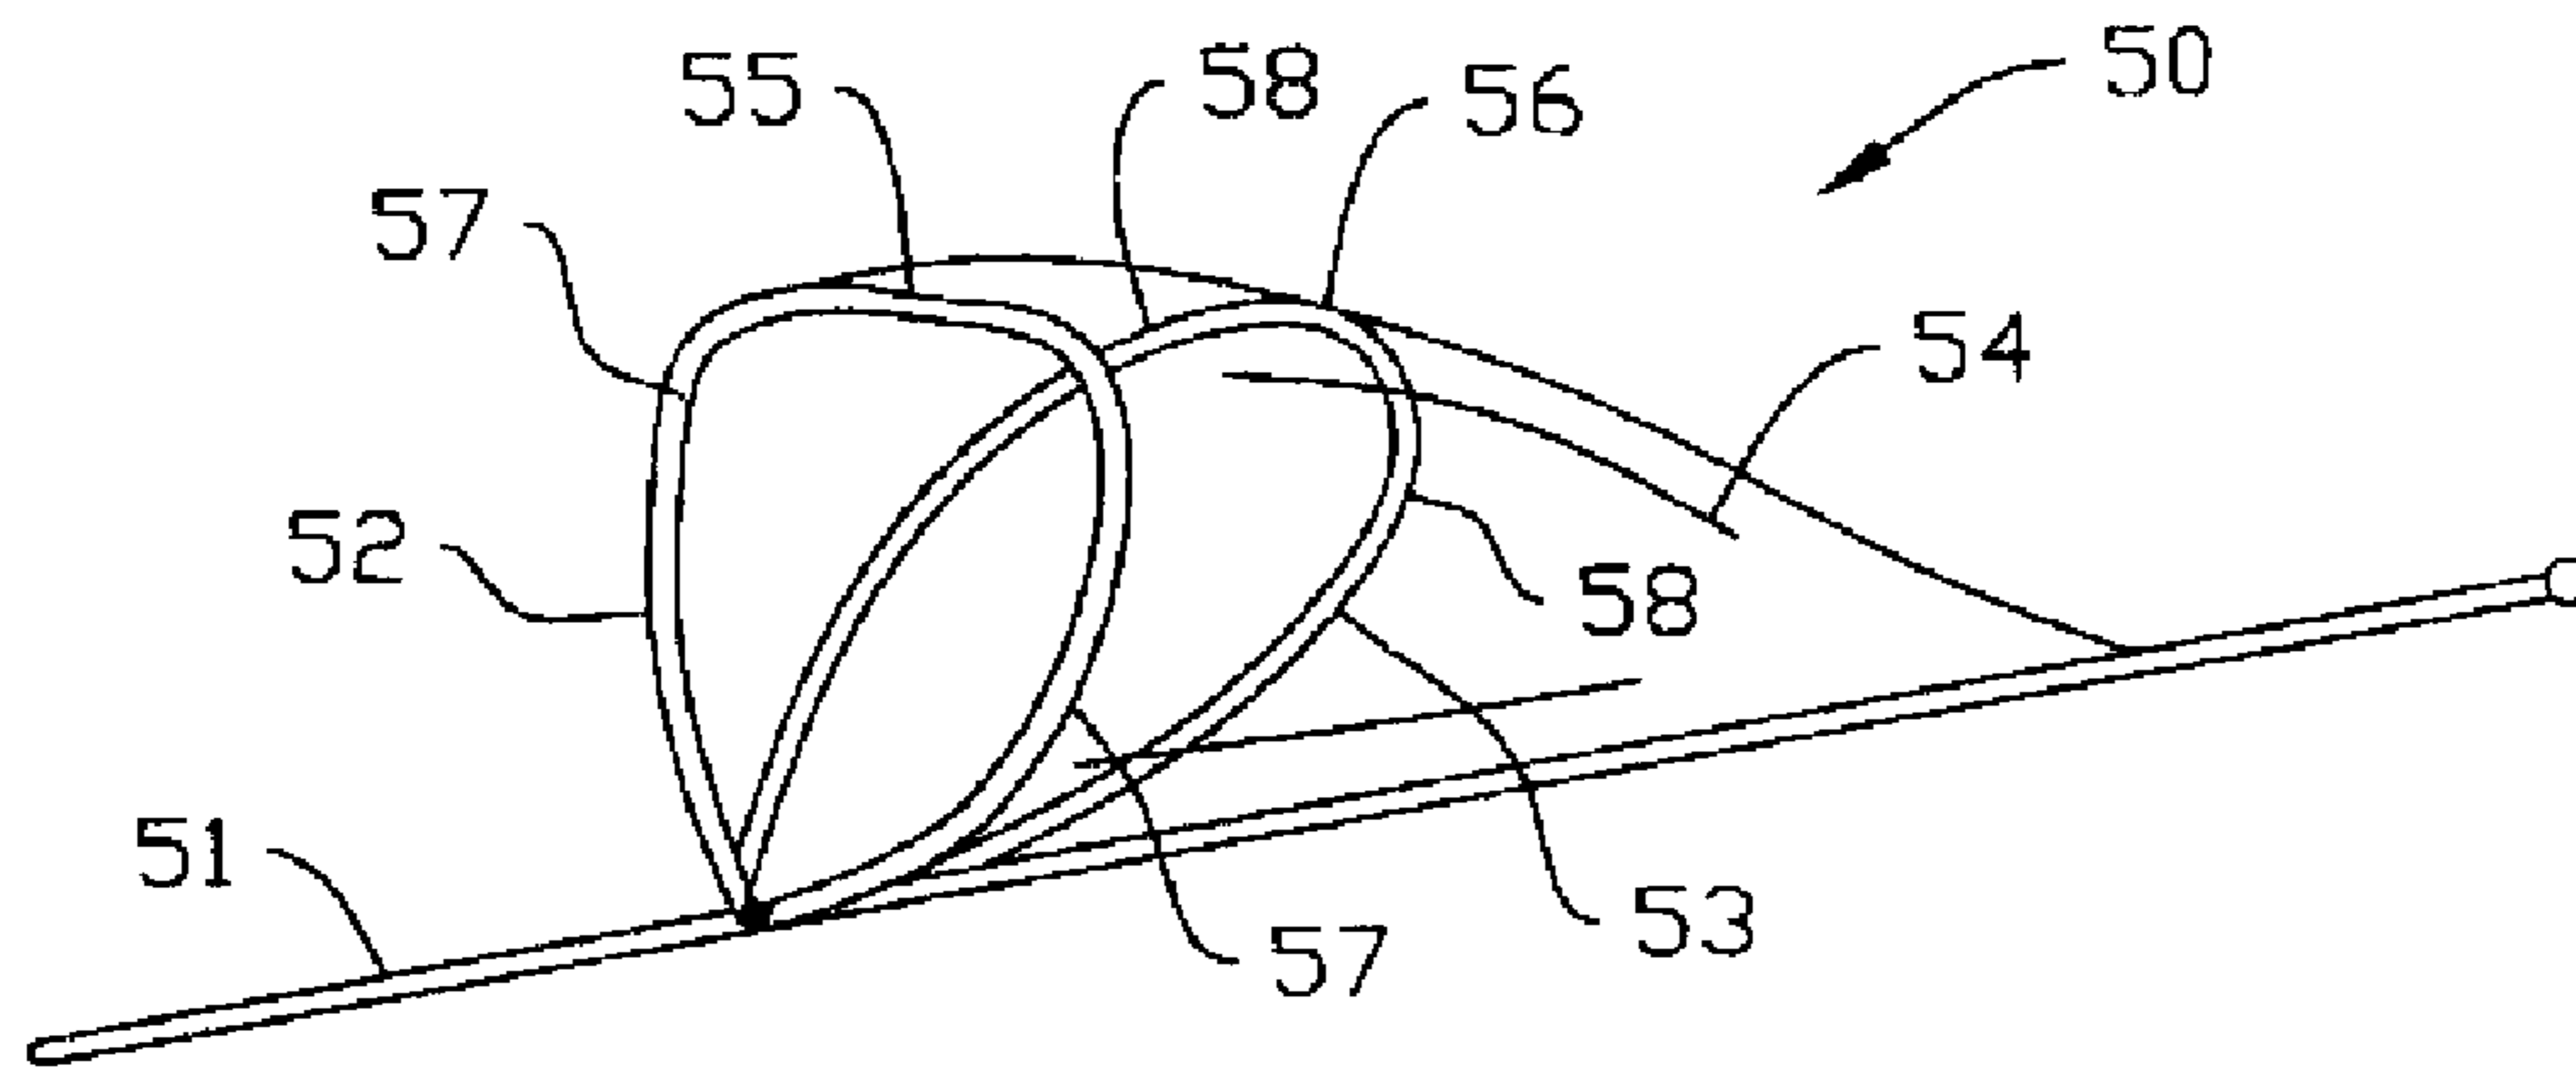


FIG. 6

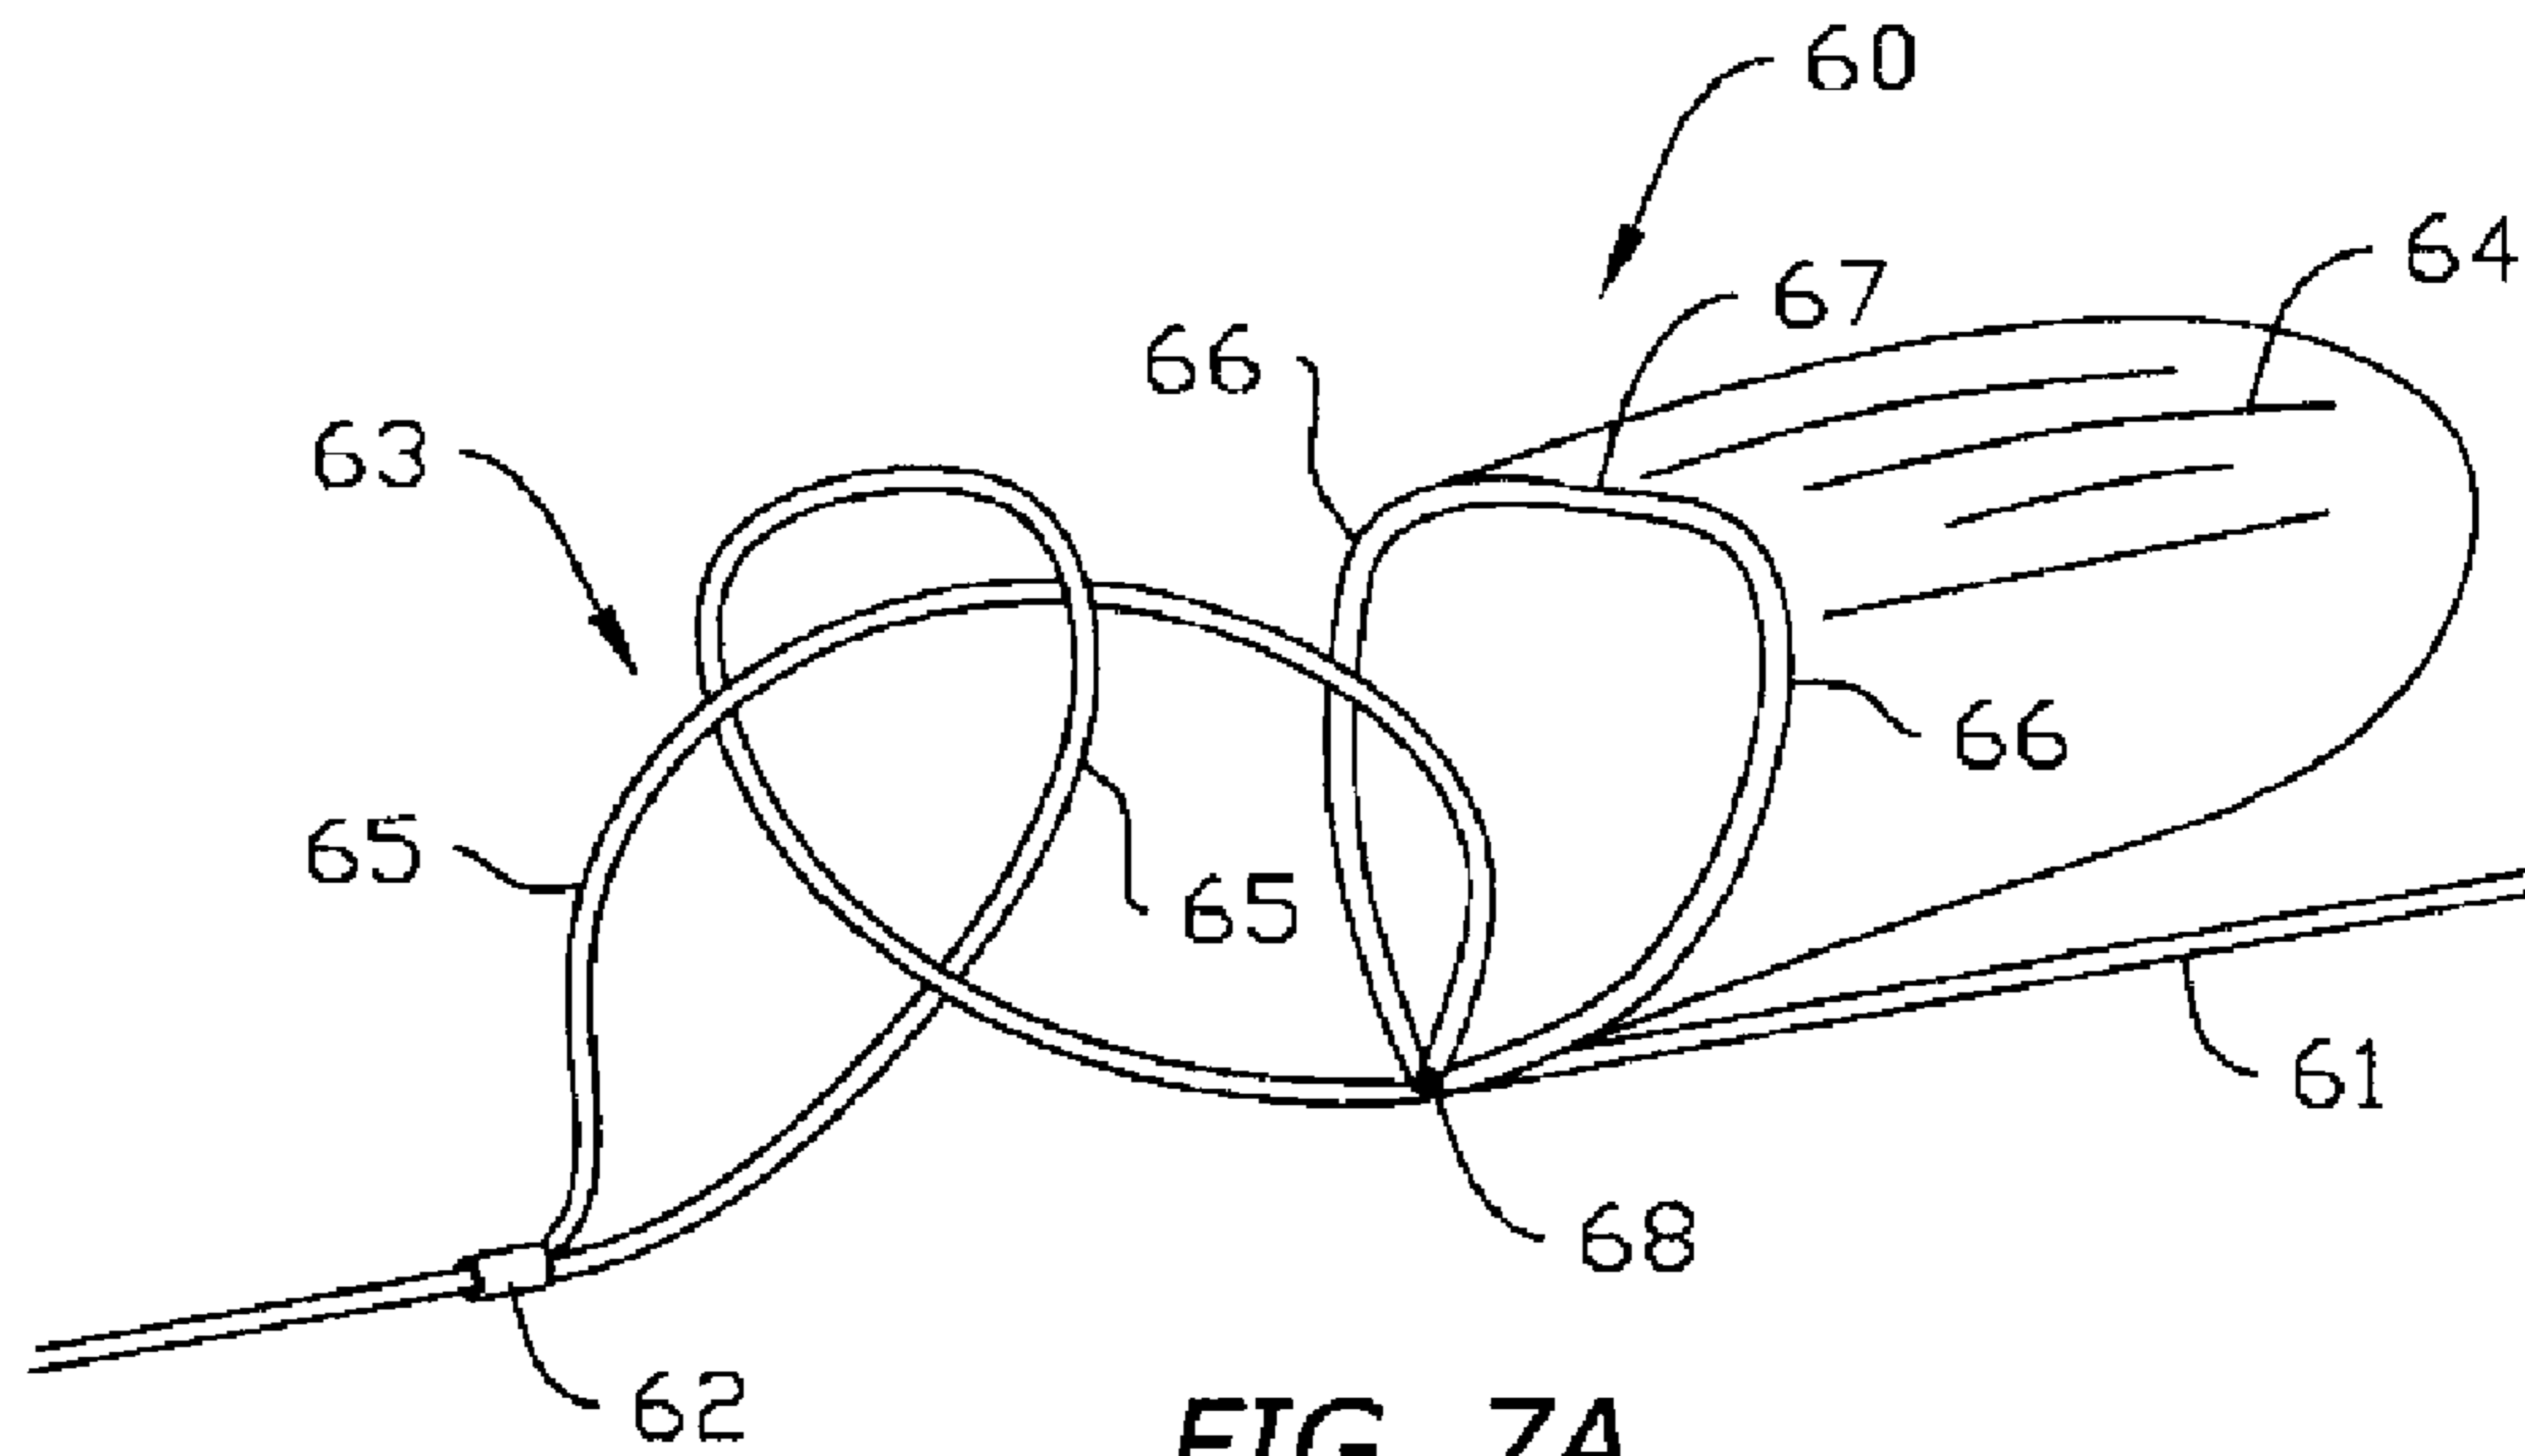


FIG. 7A

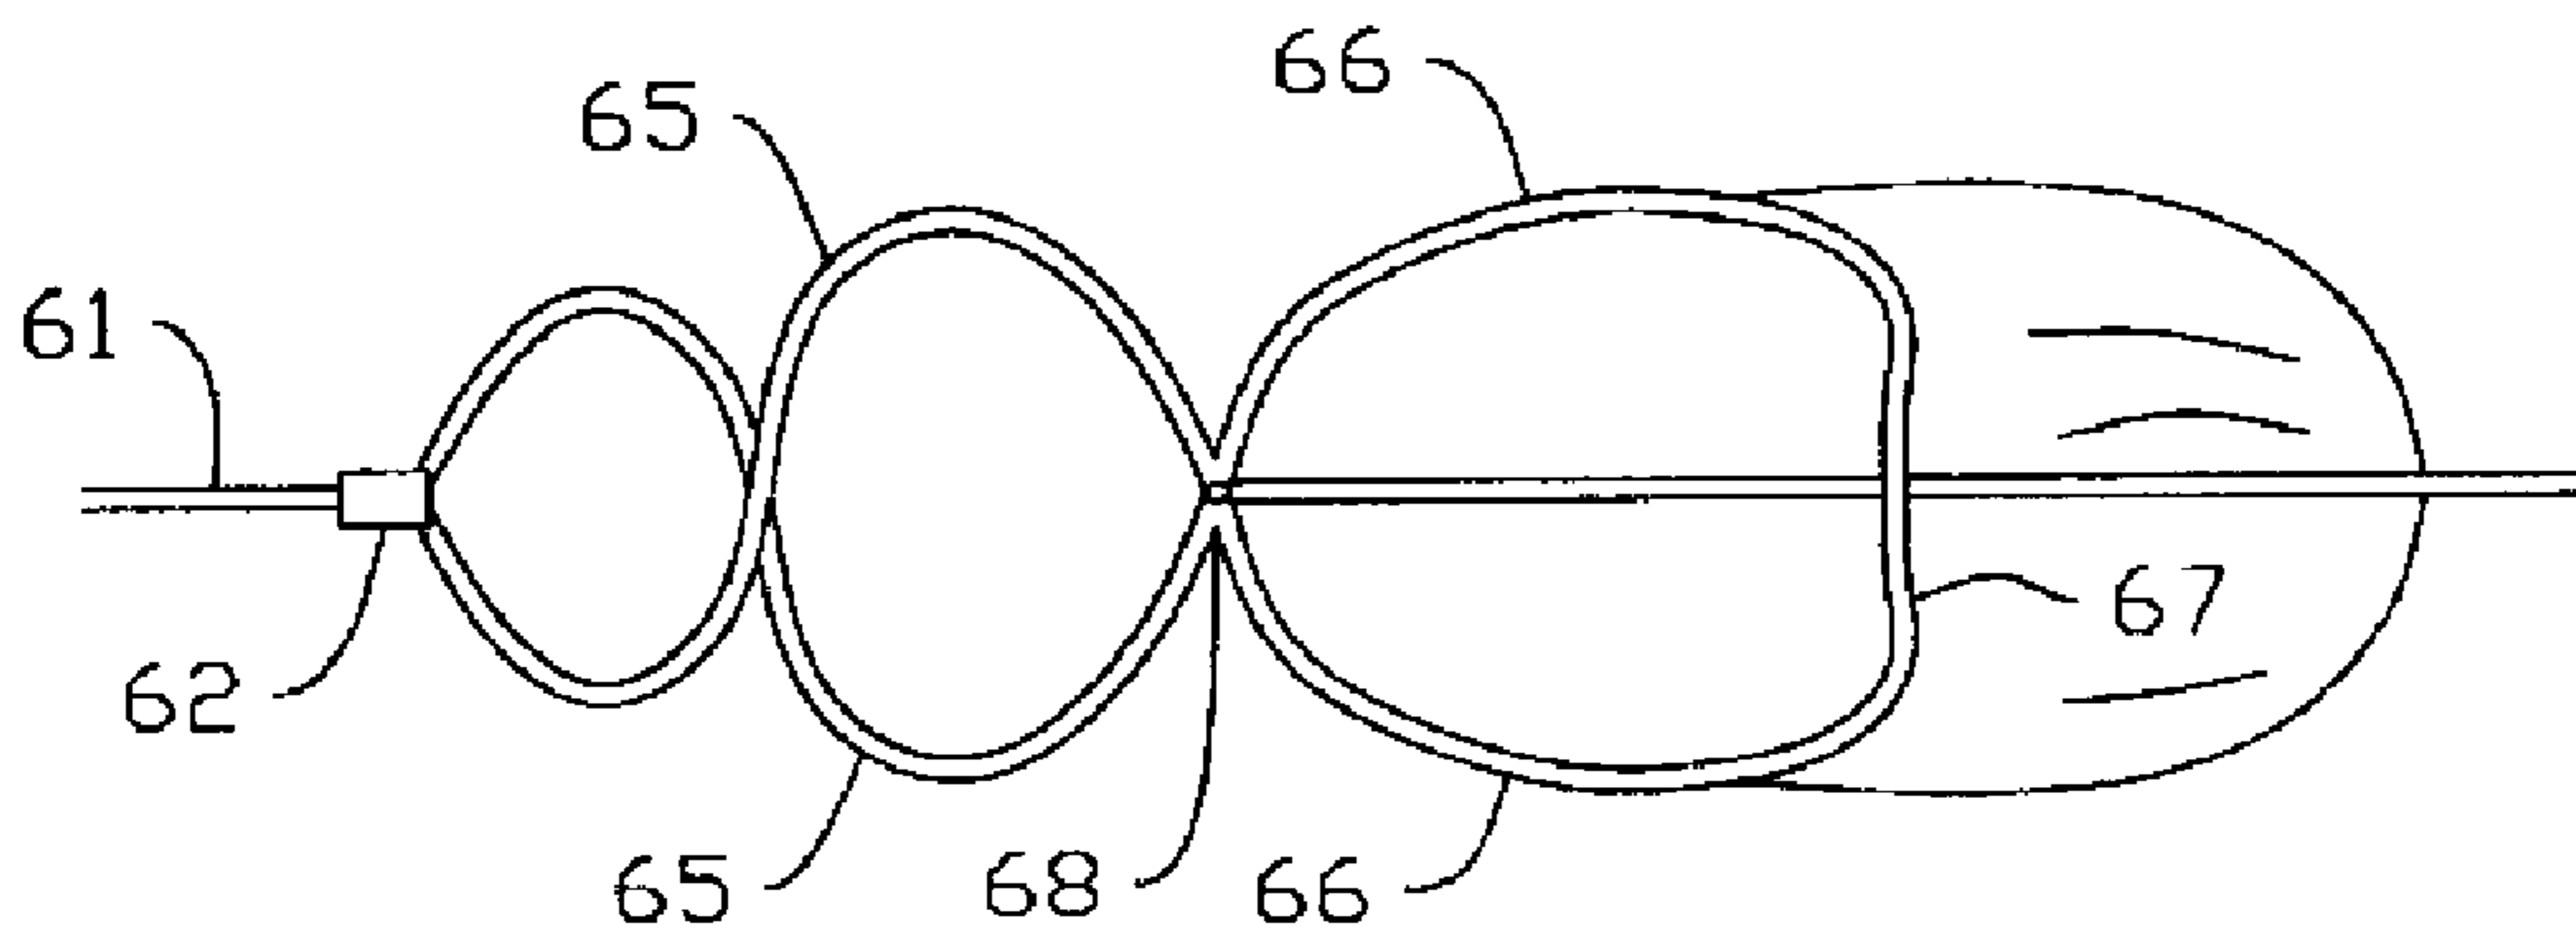
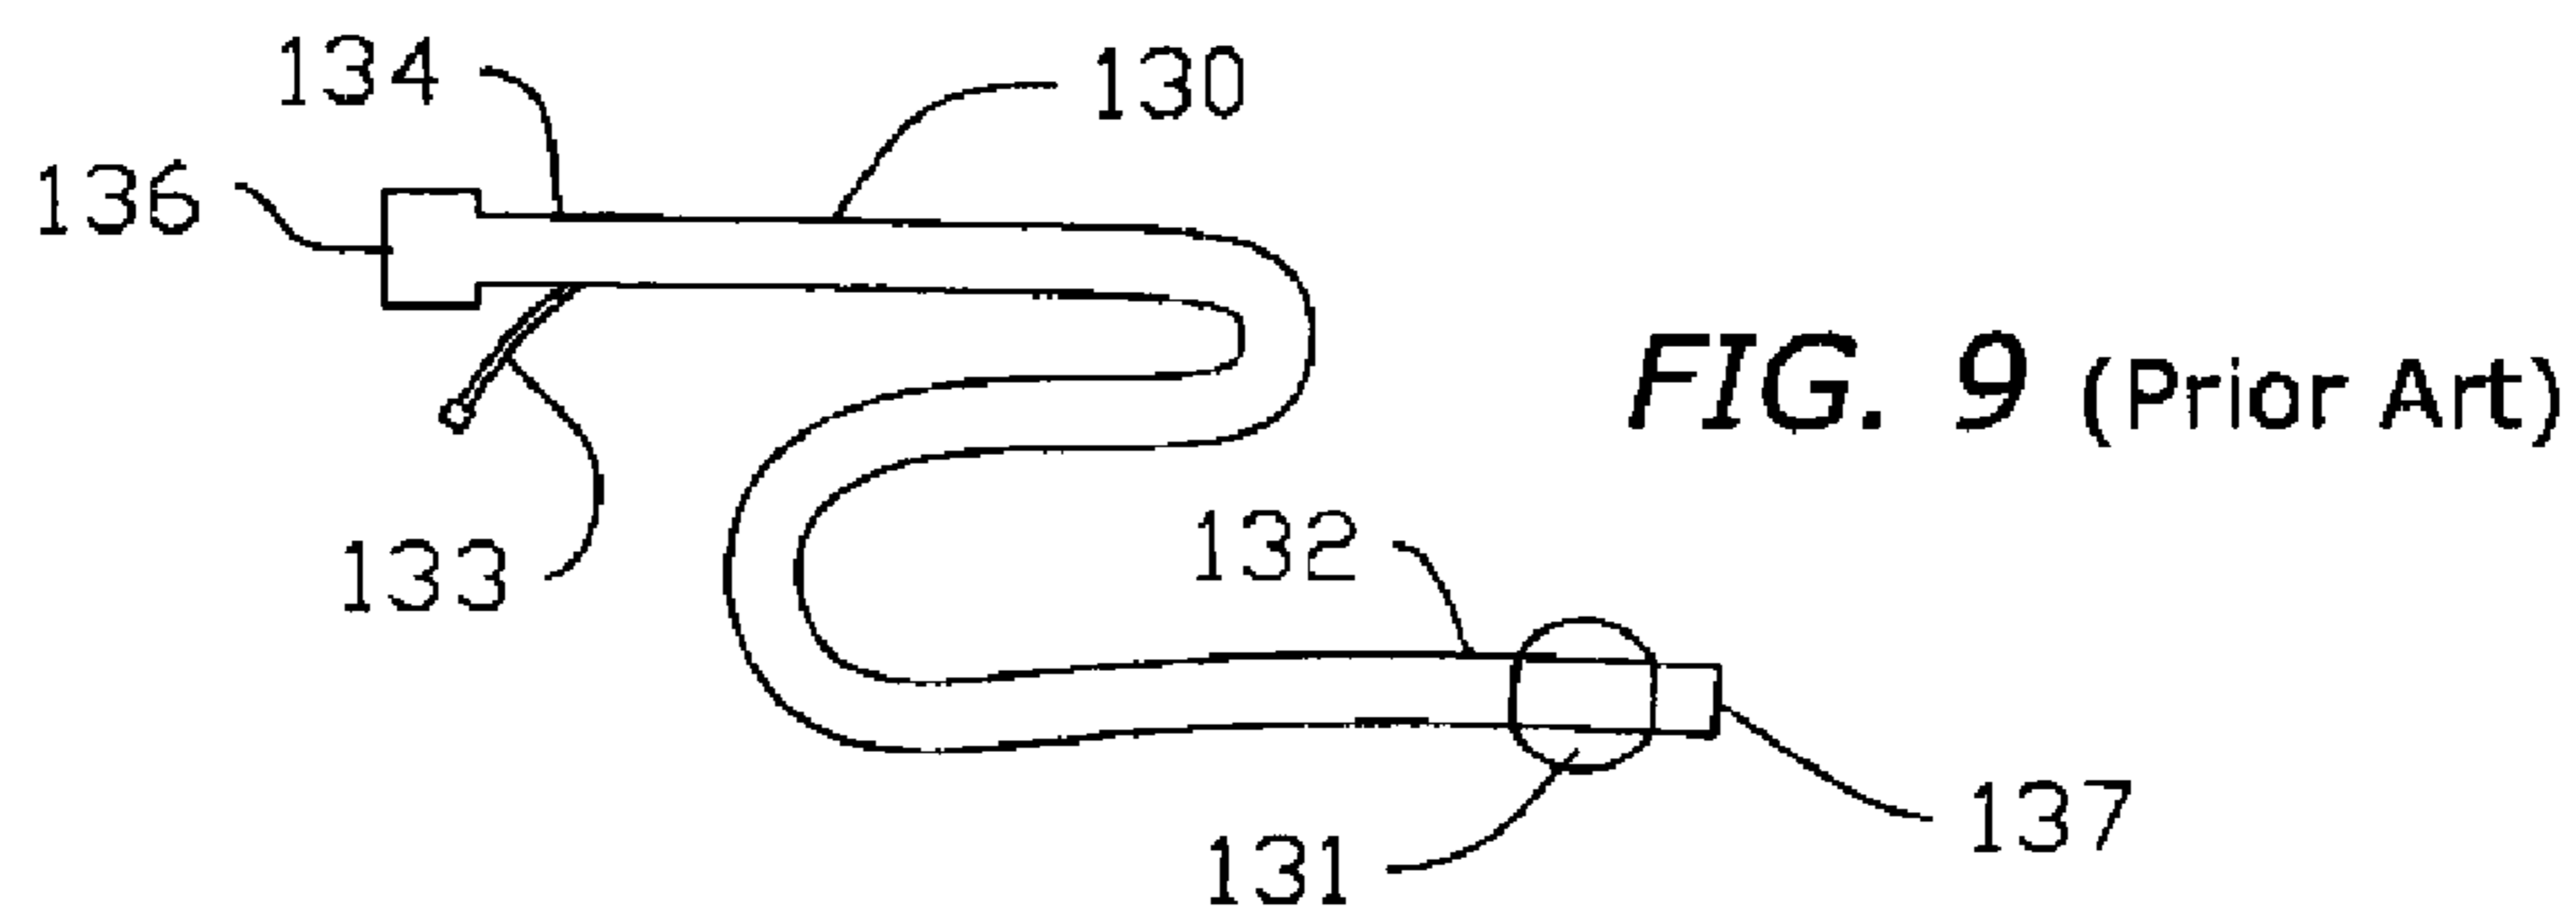
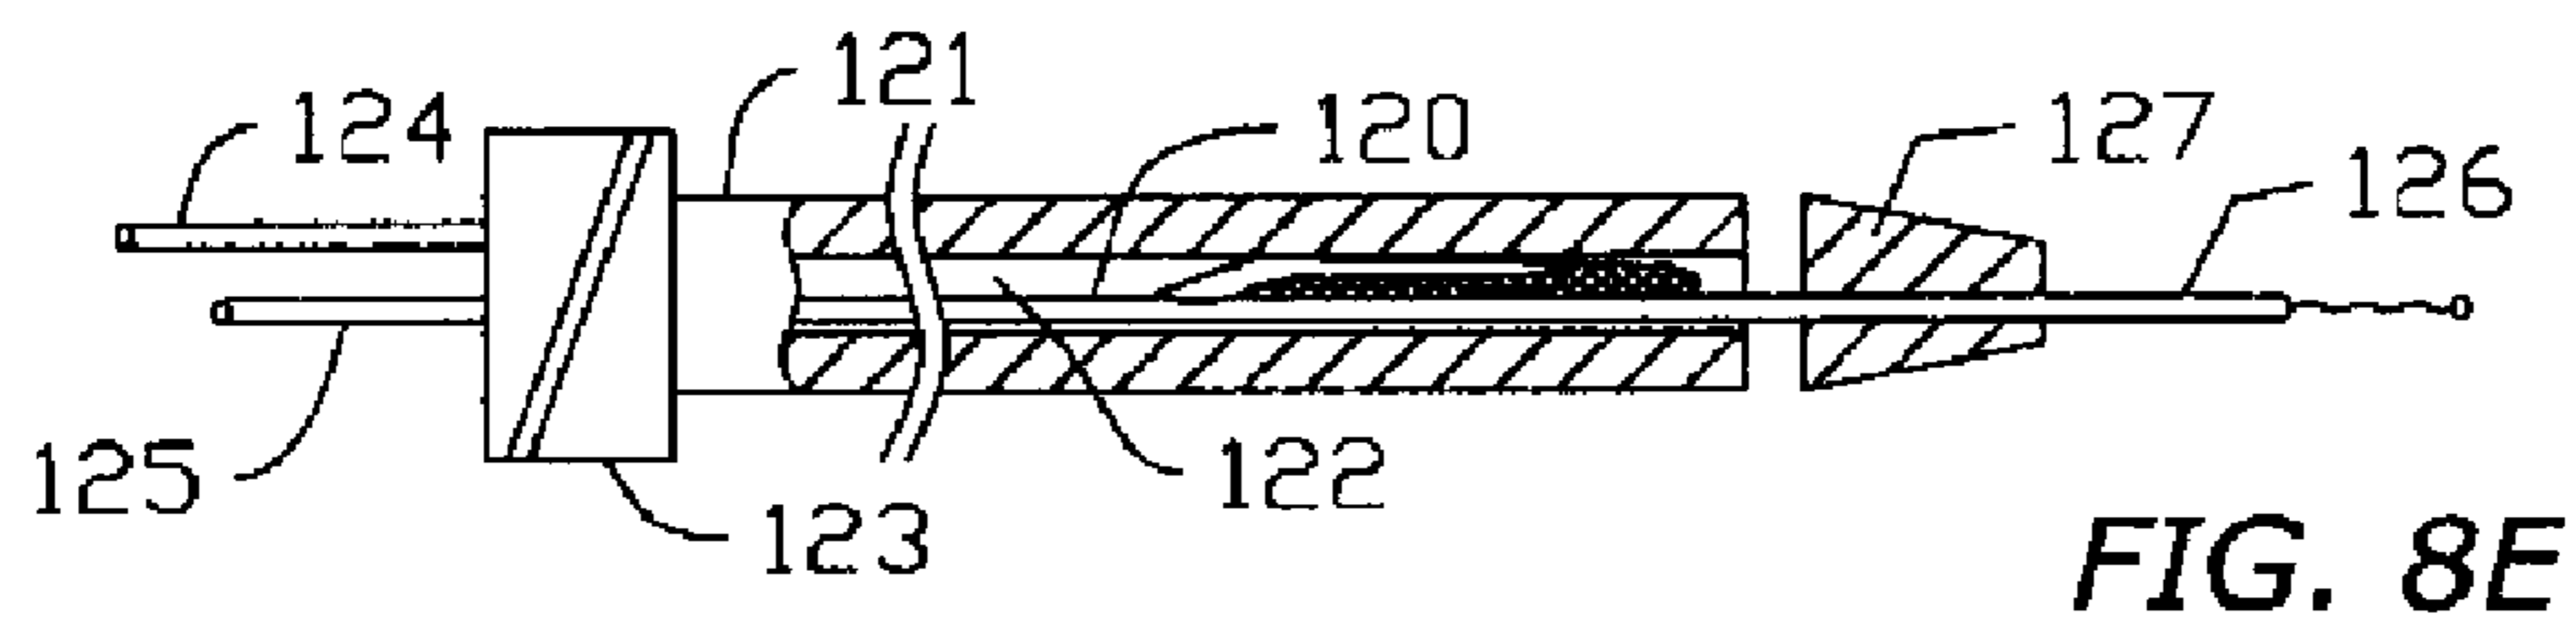
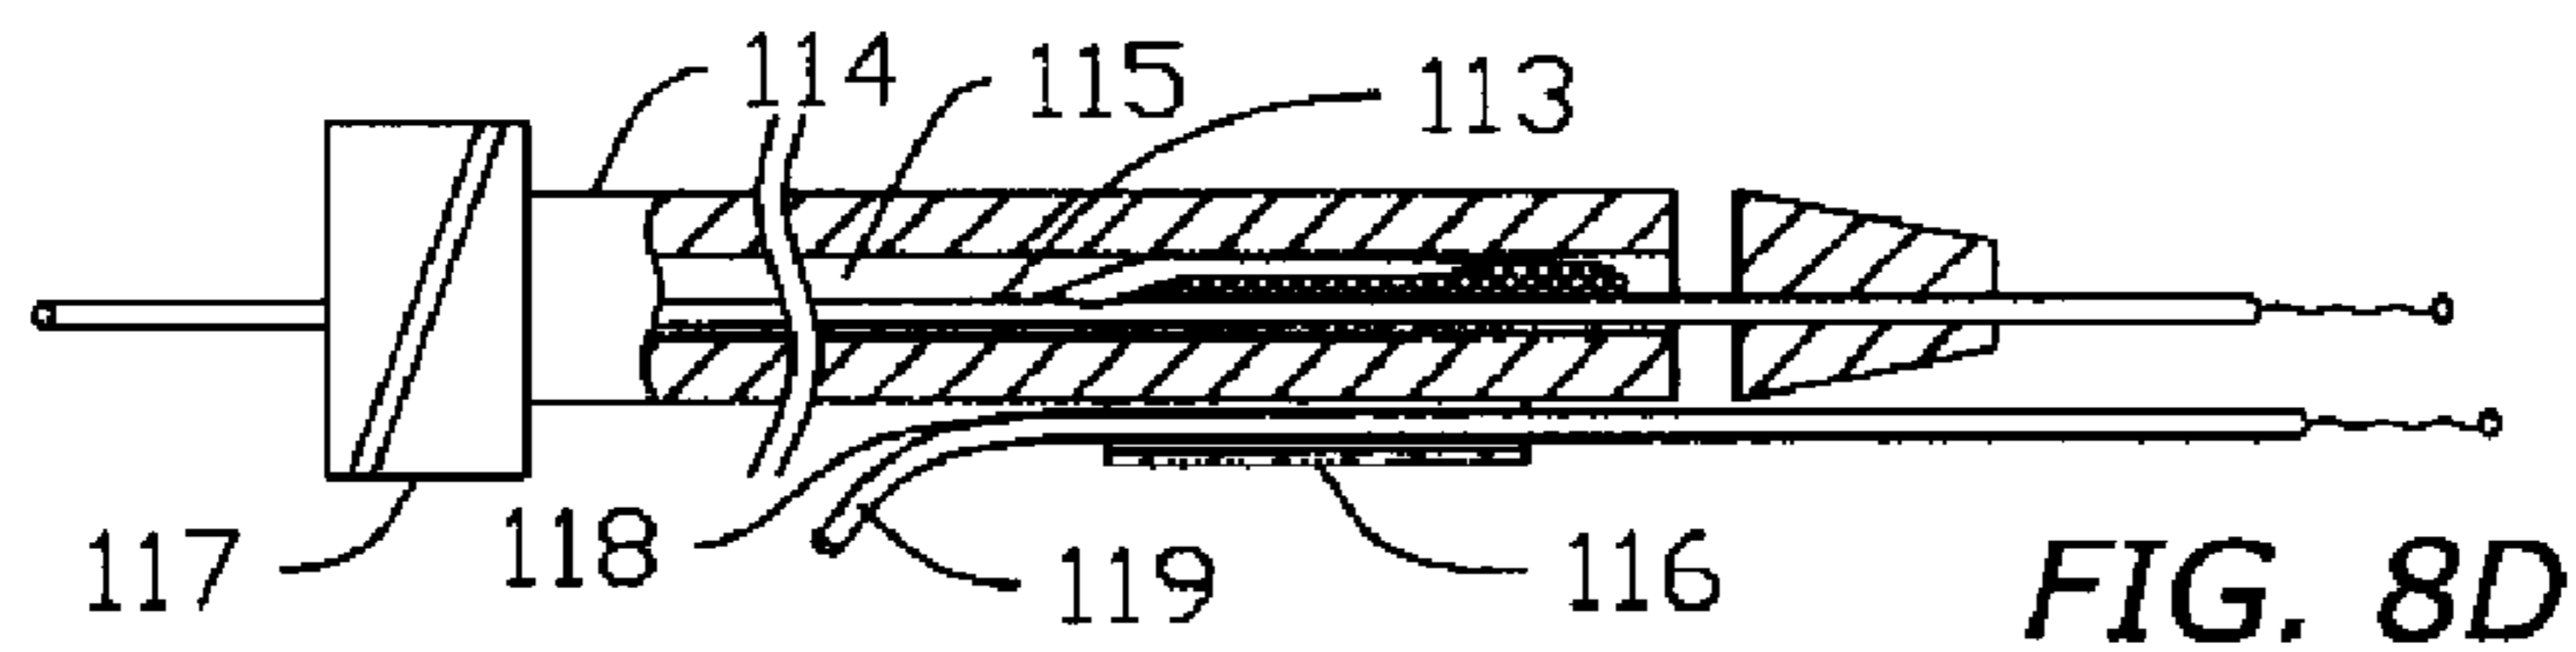
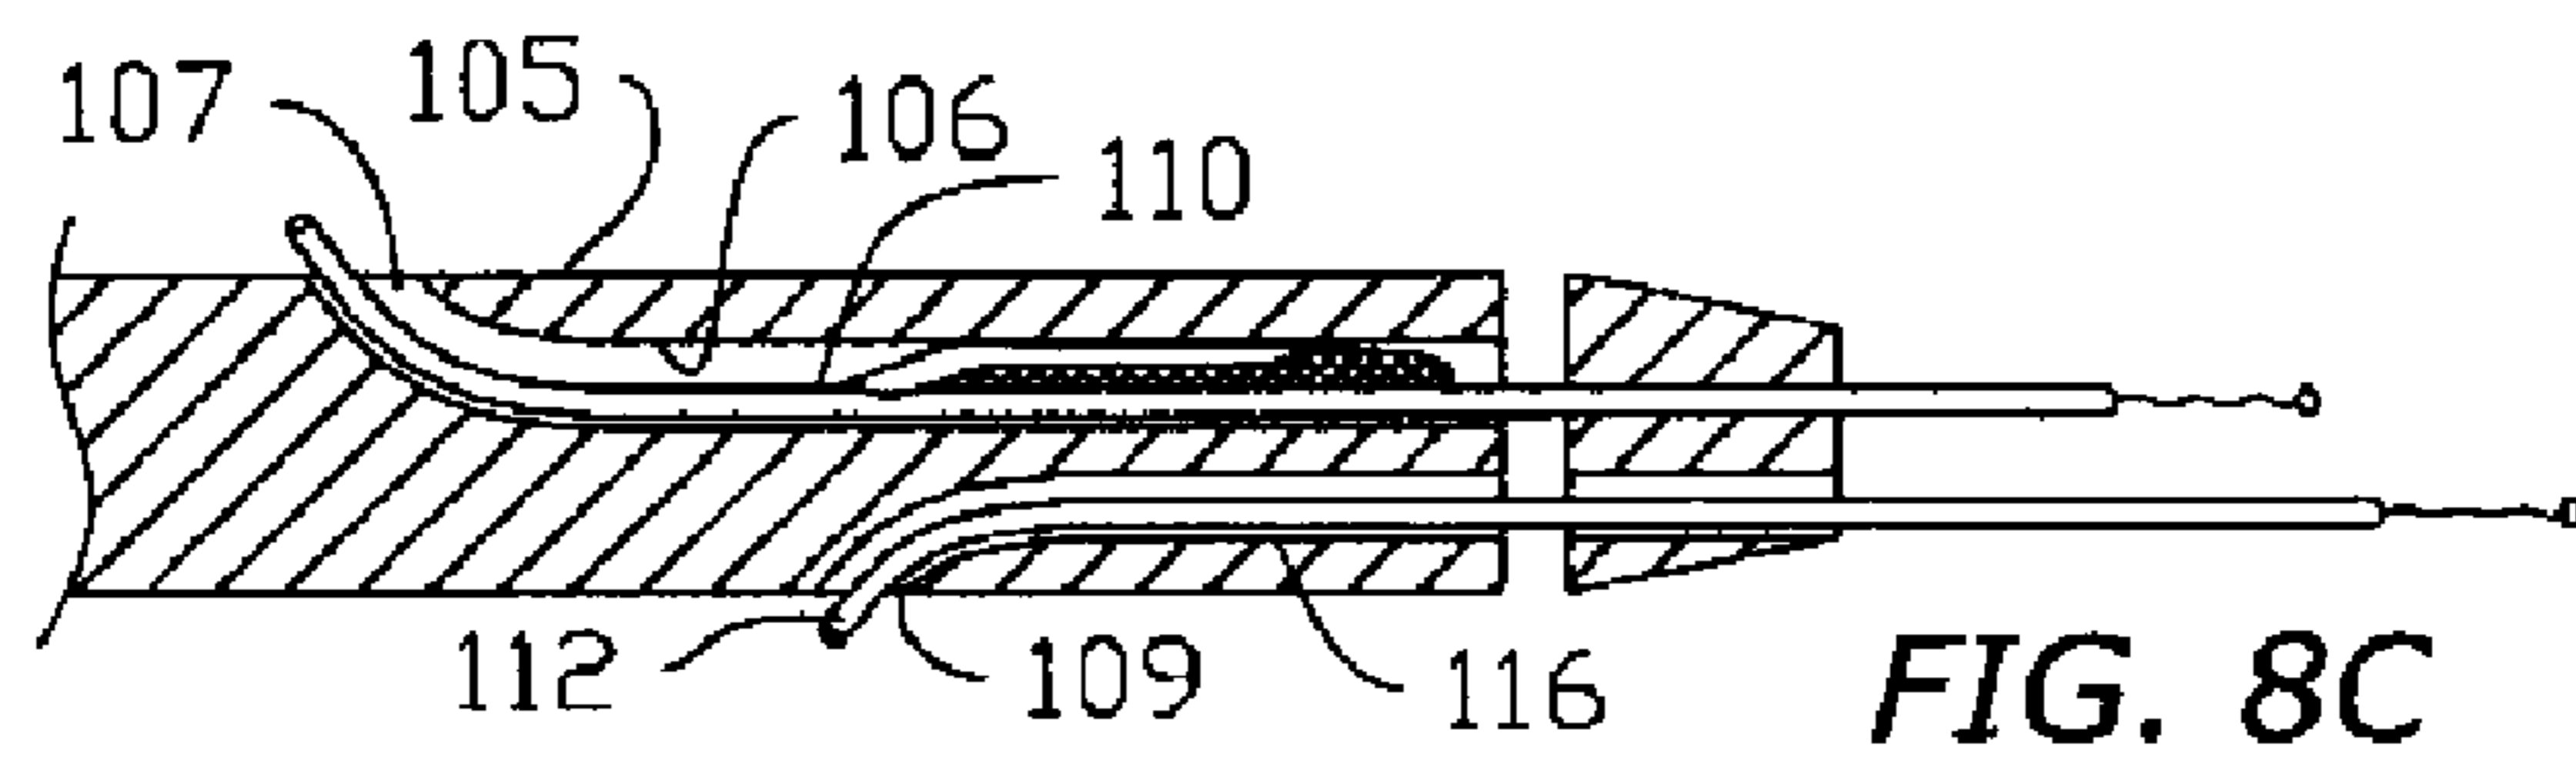
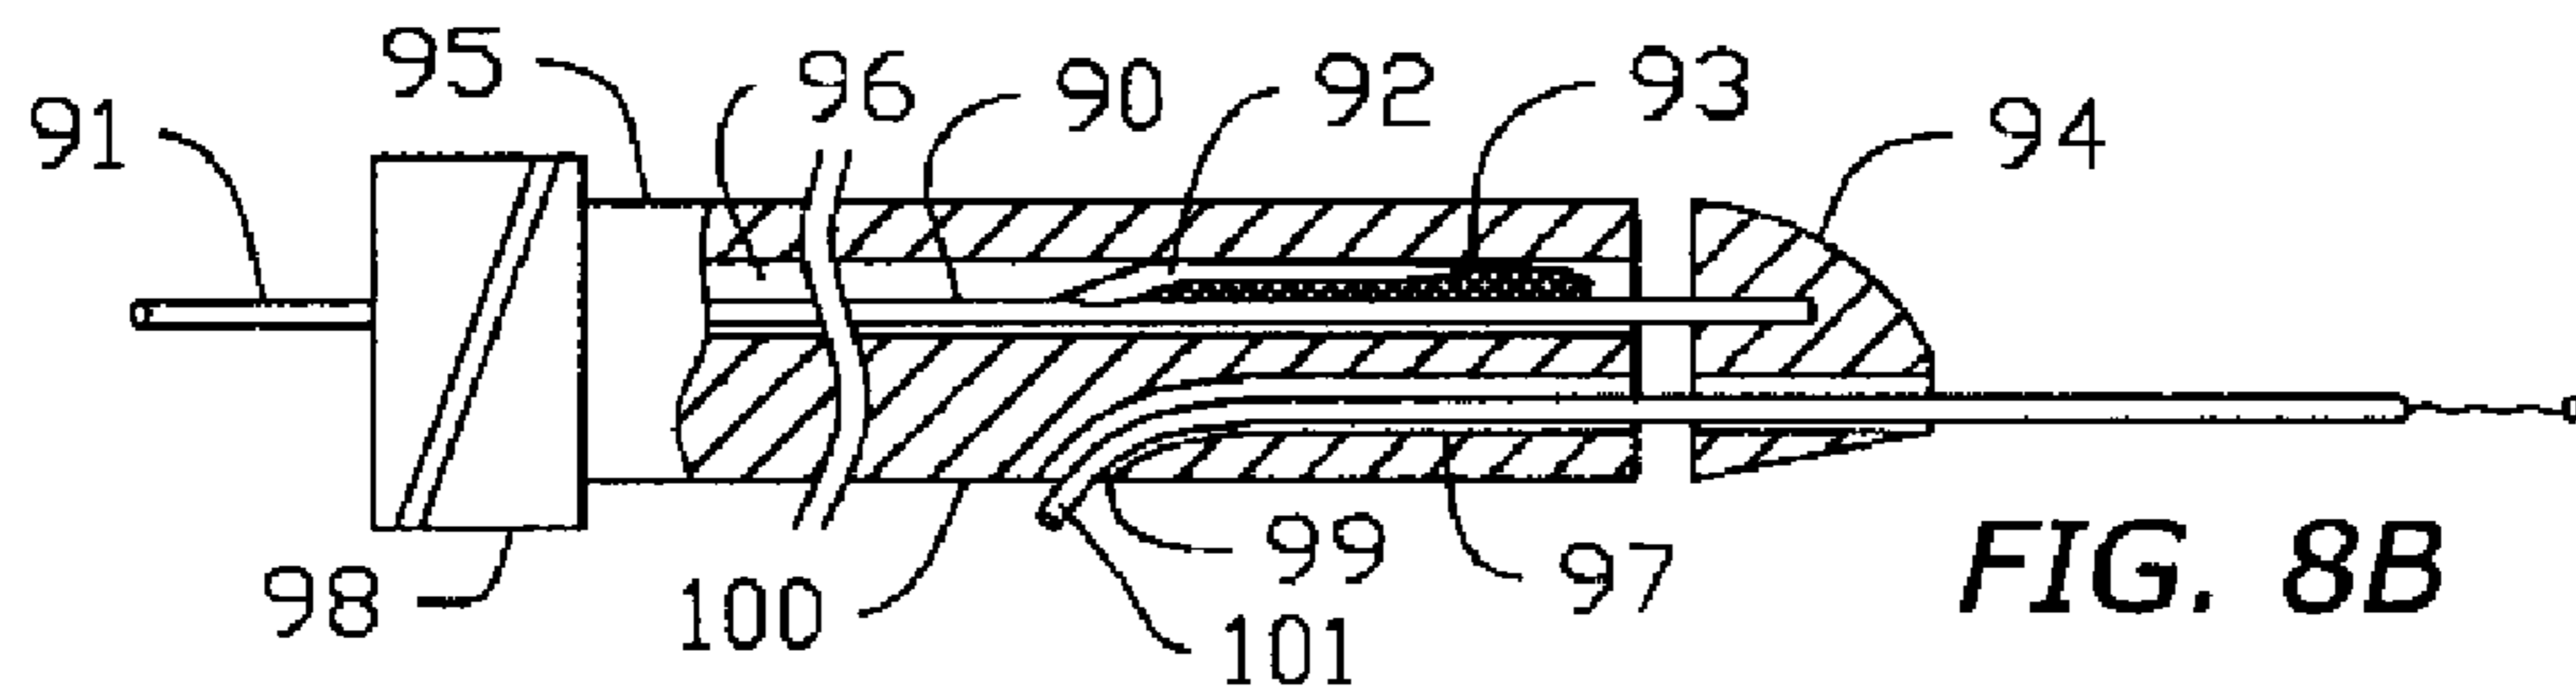
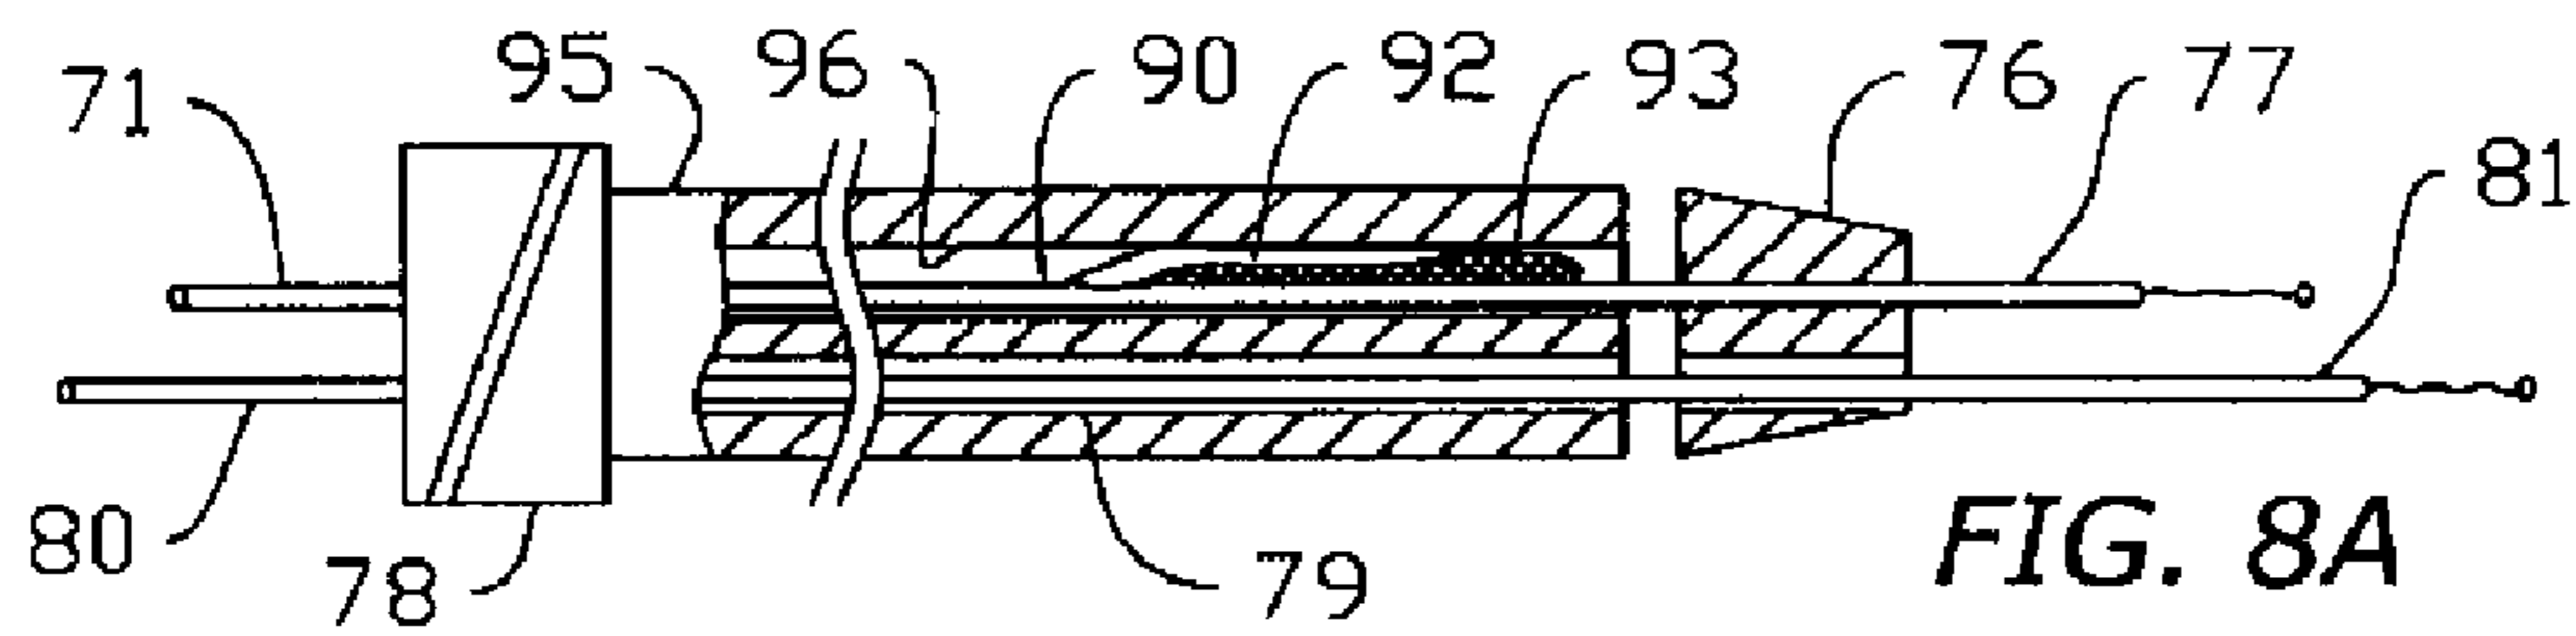


FIG. 7B



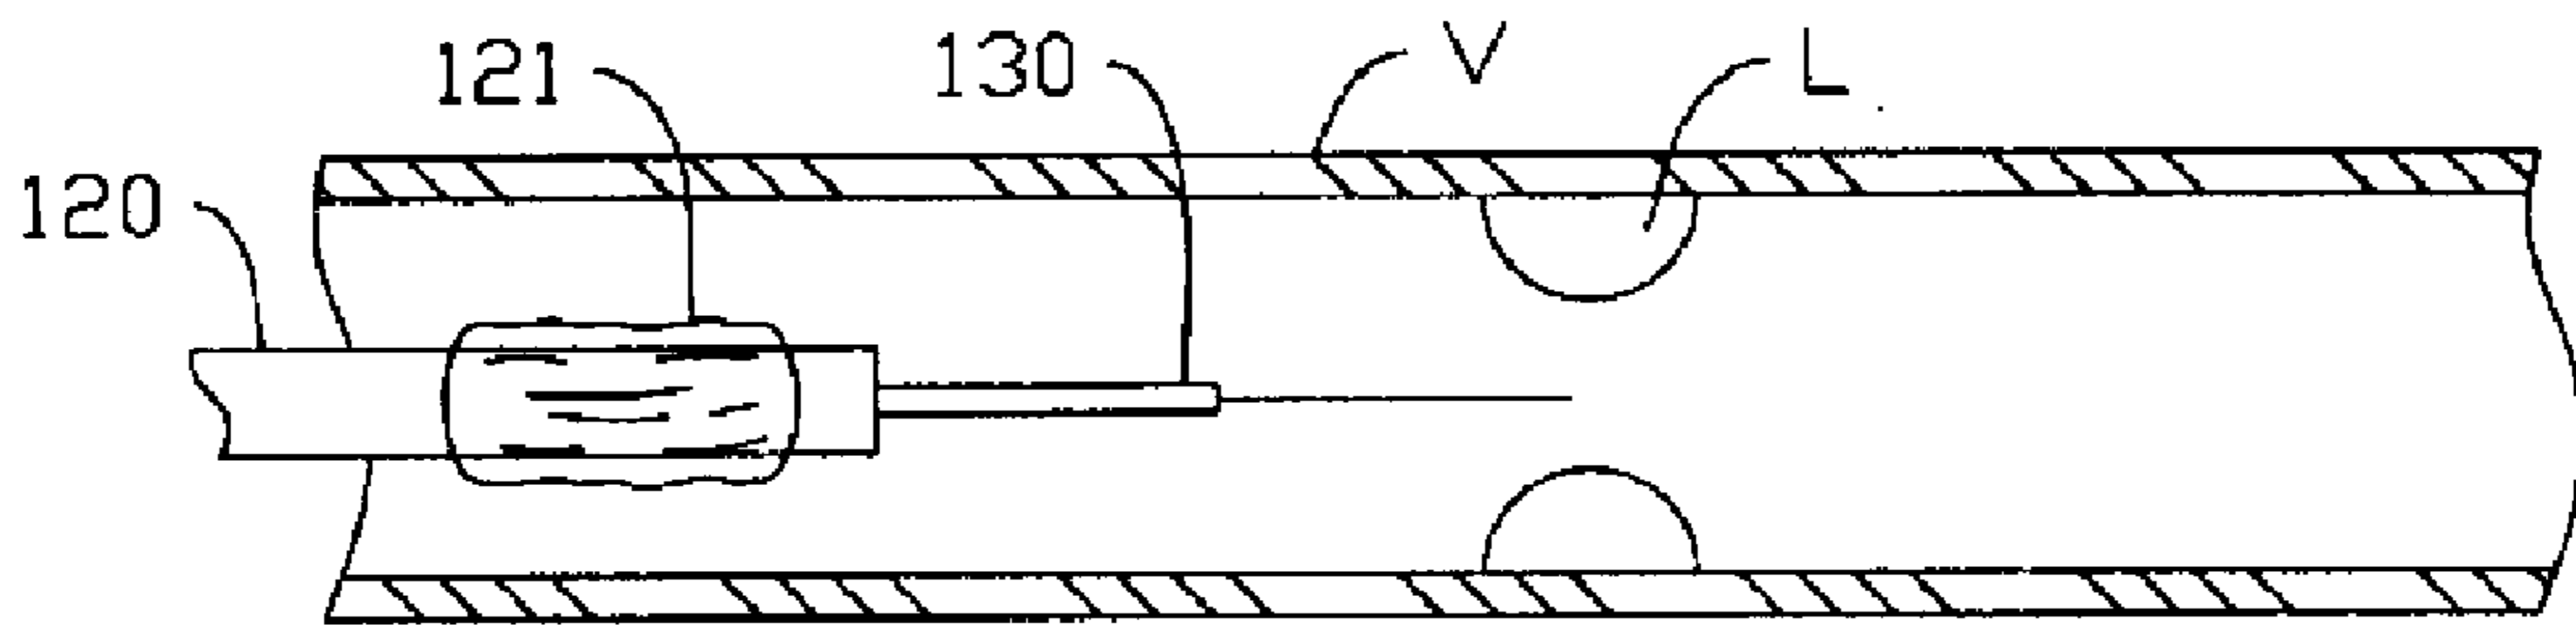


FIG. 10A

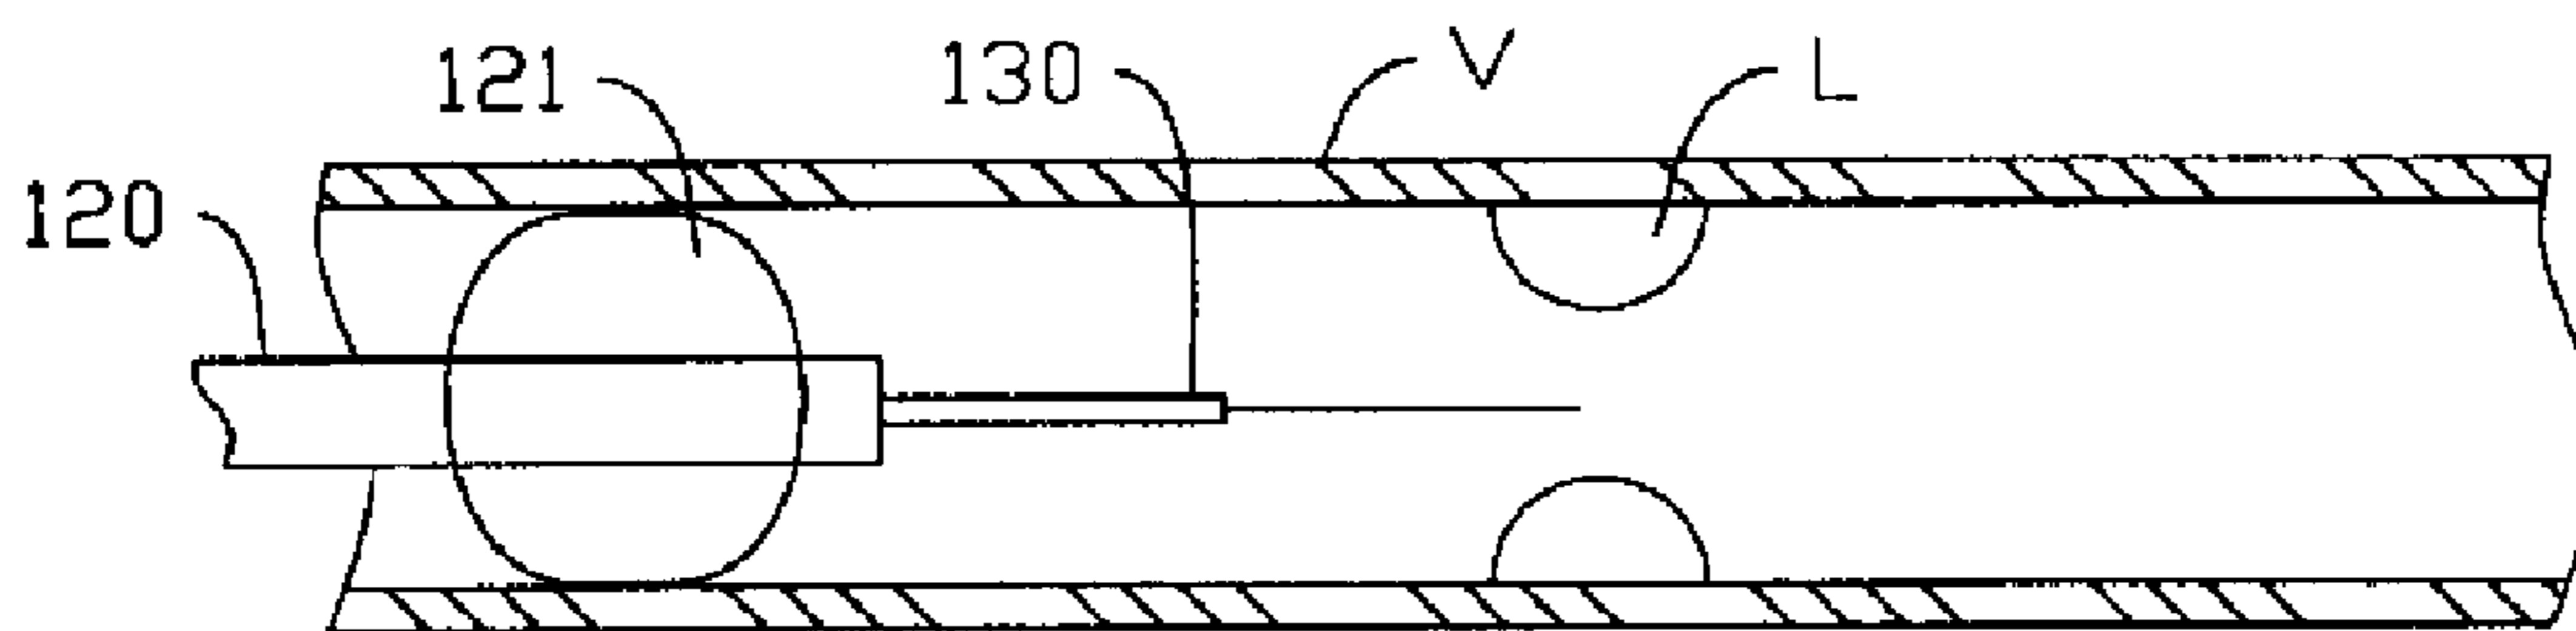


FIG. 10B

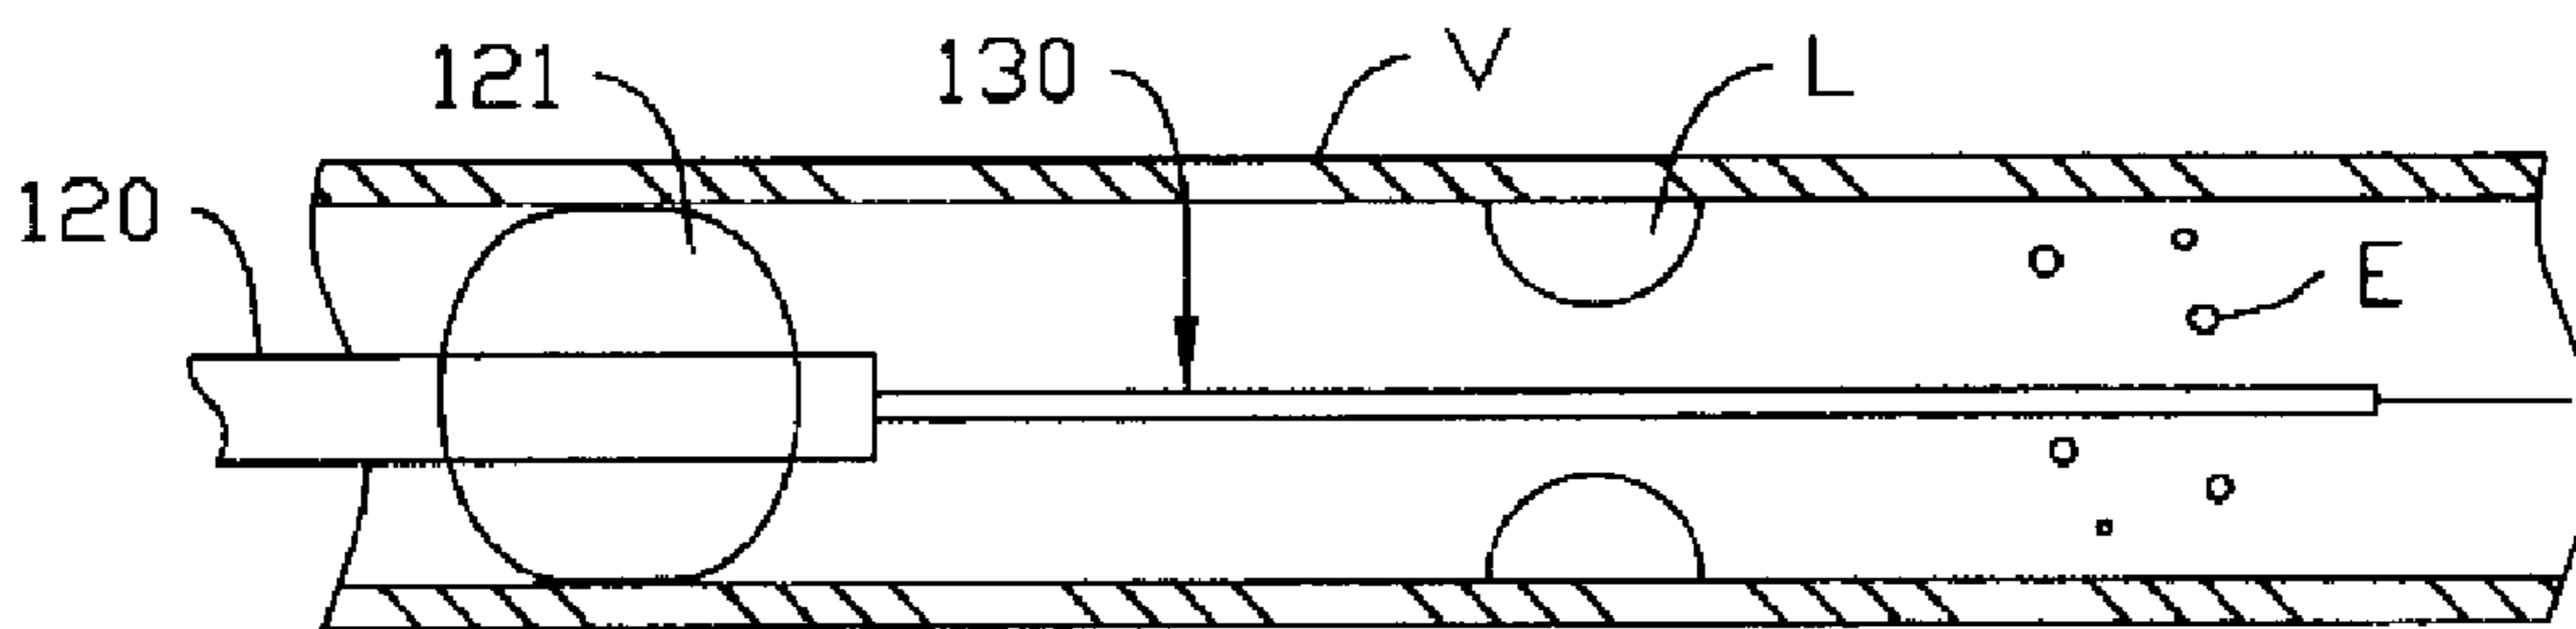


FIG. 10C

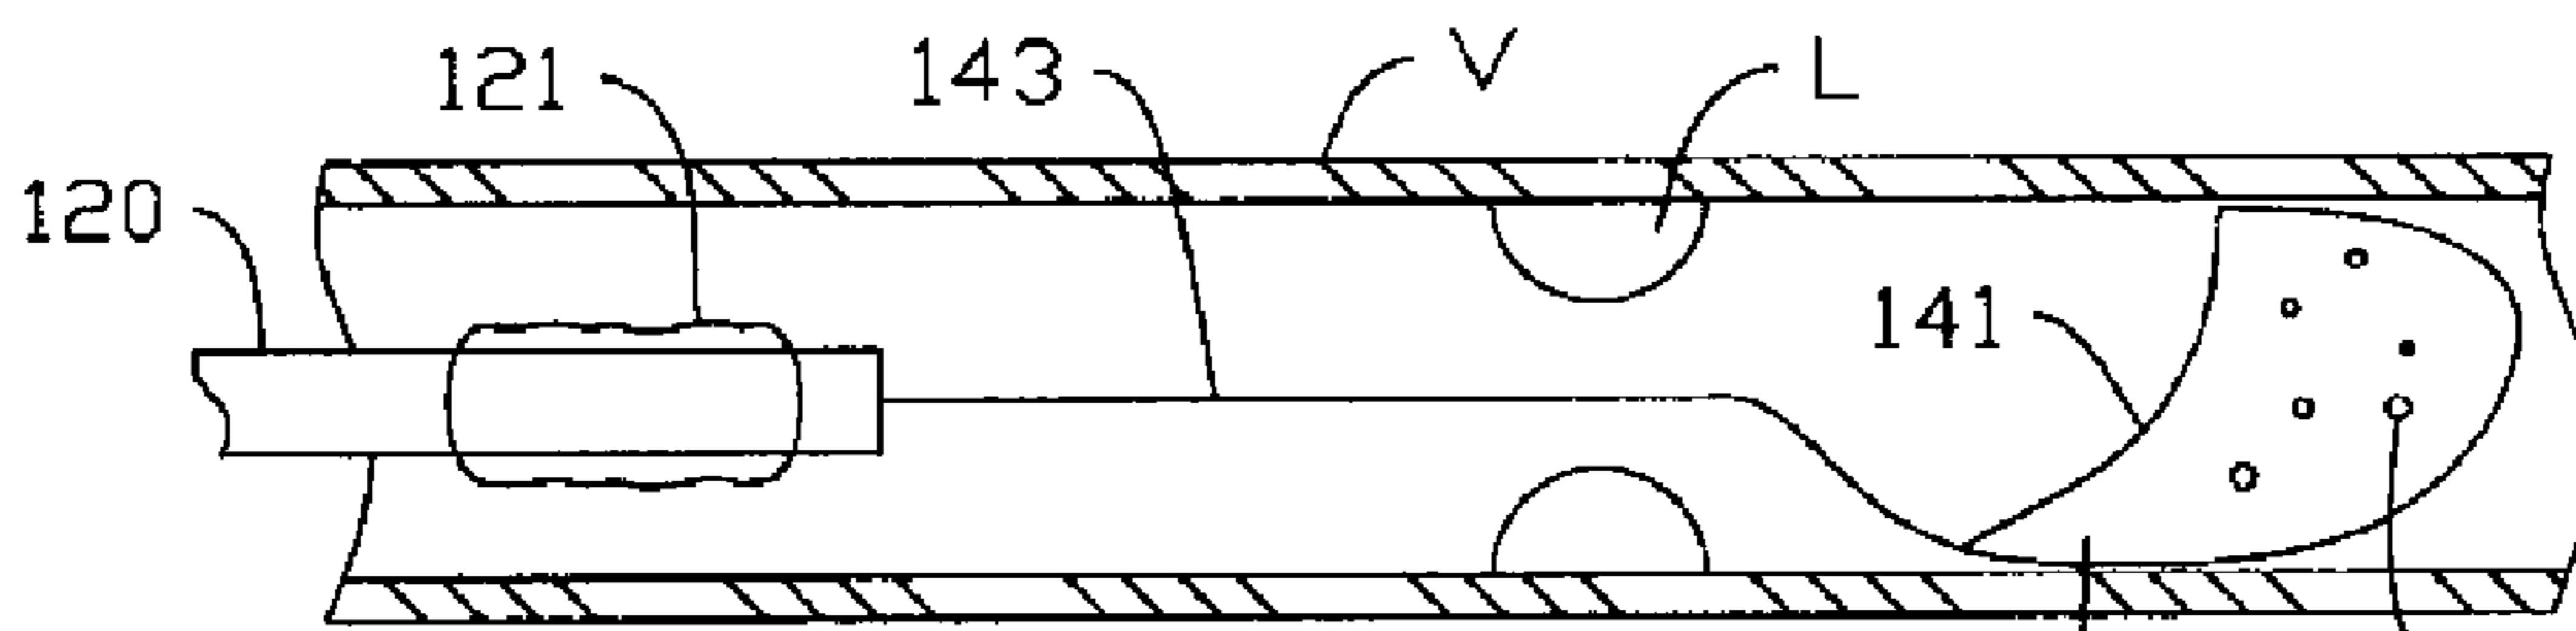


FIG. 10D

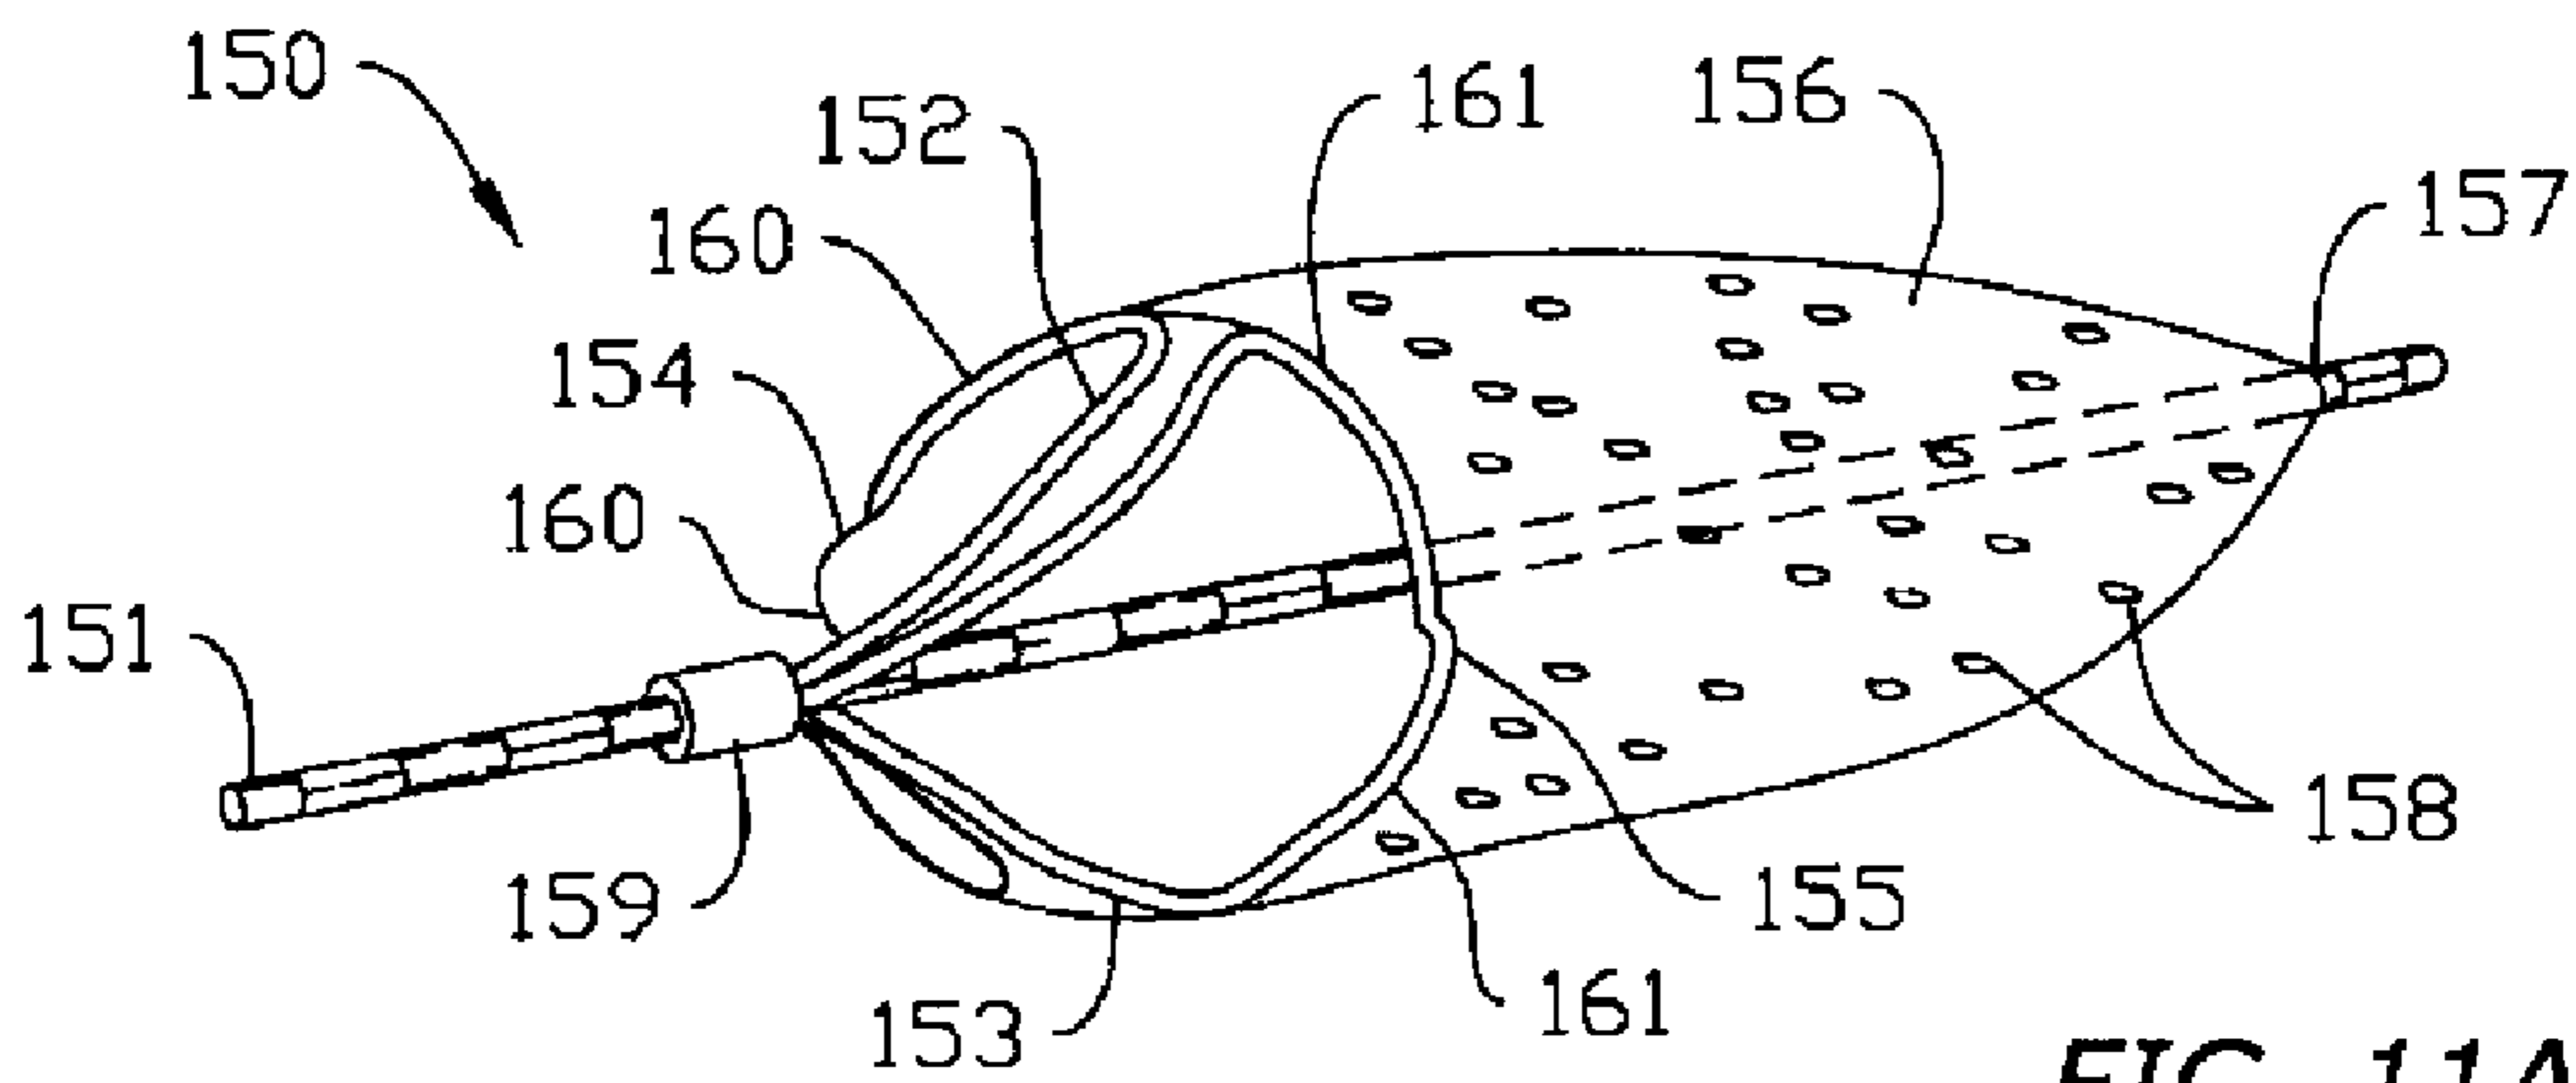


FIG. 11A

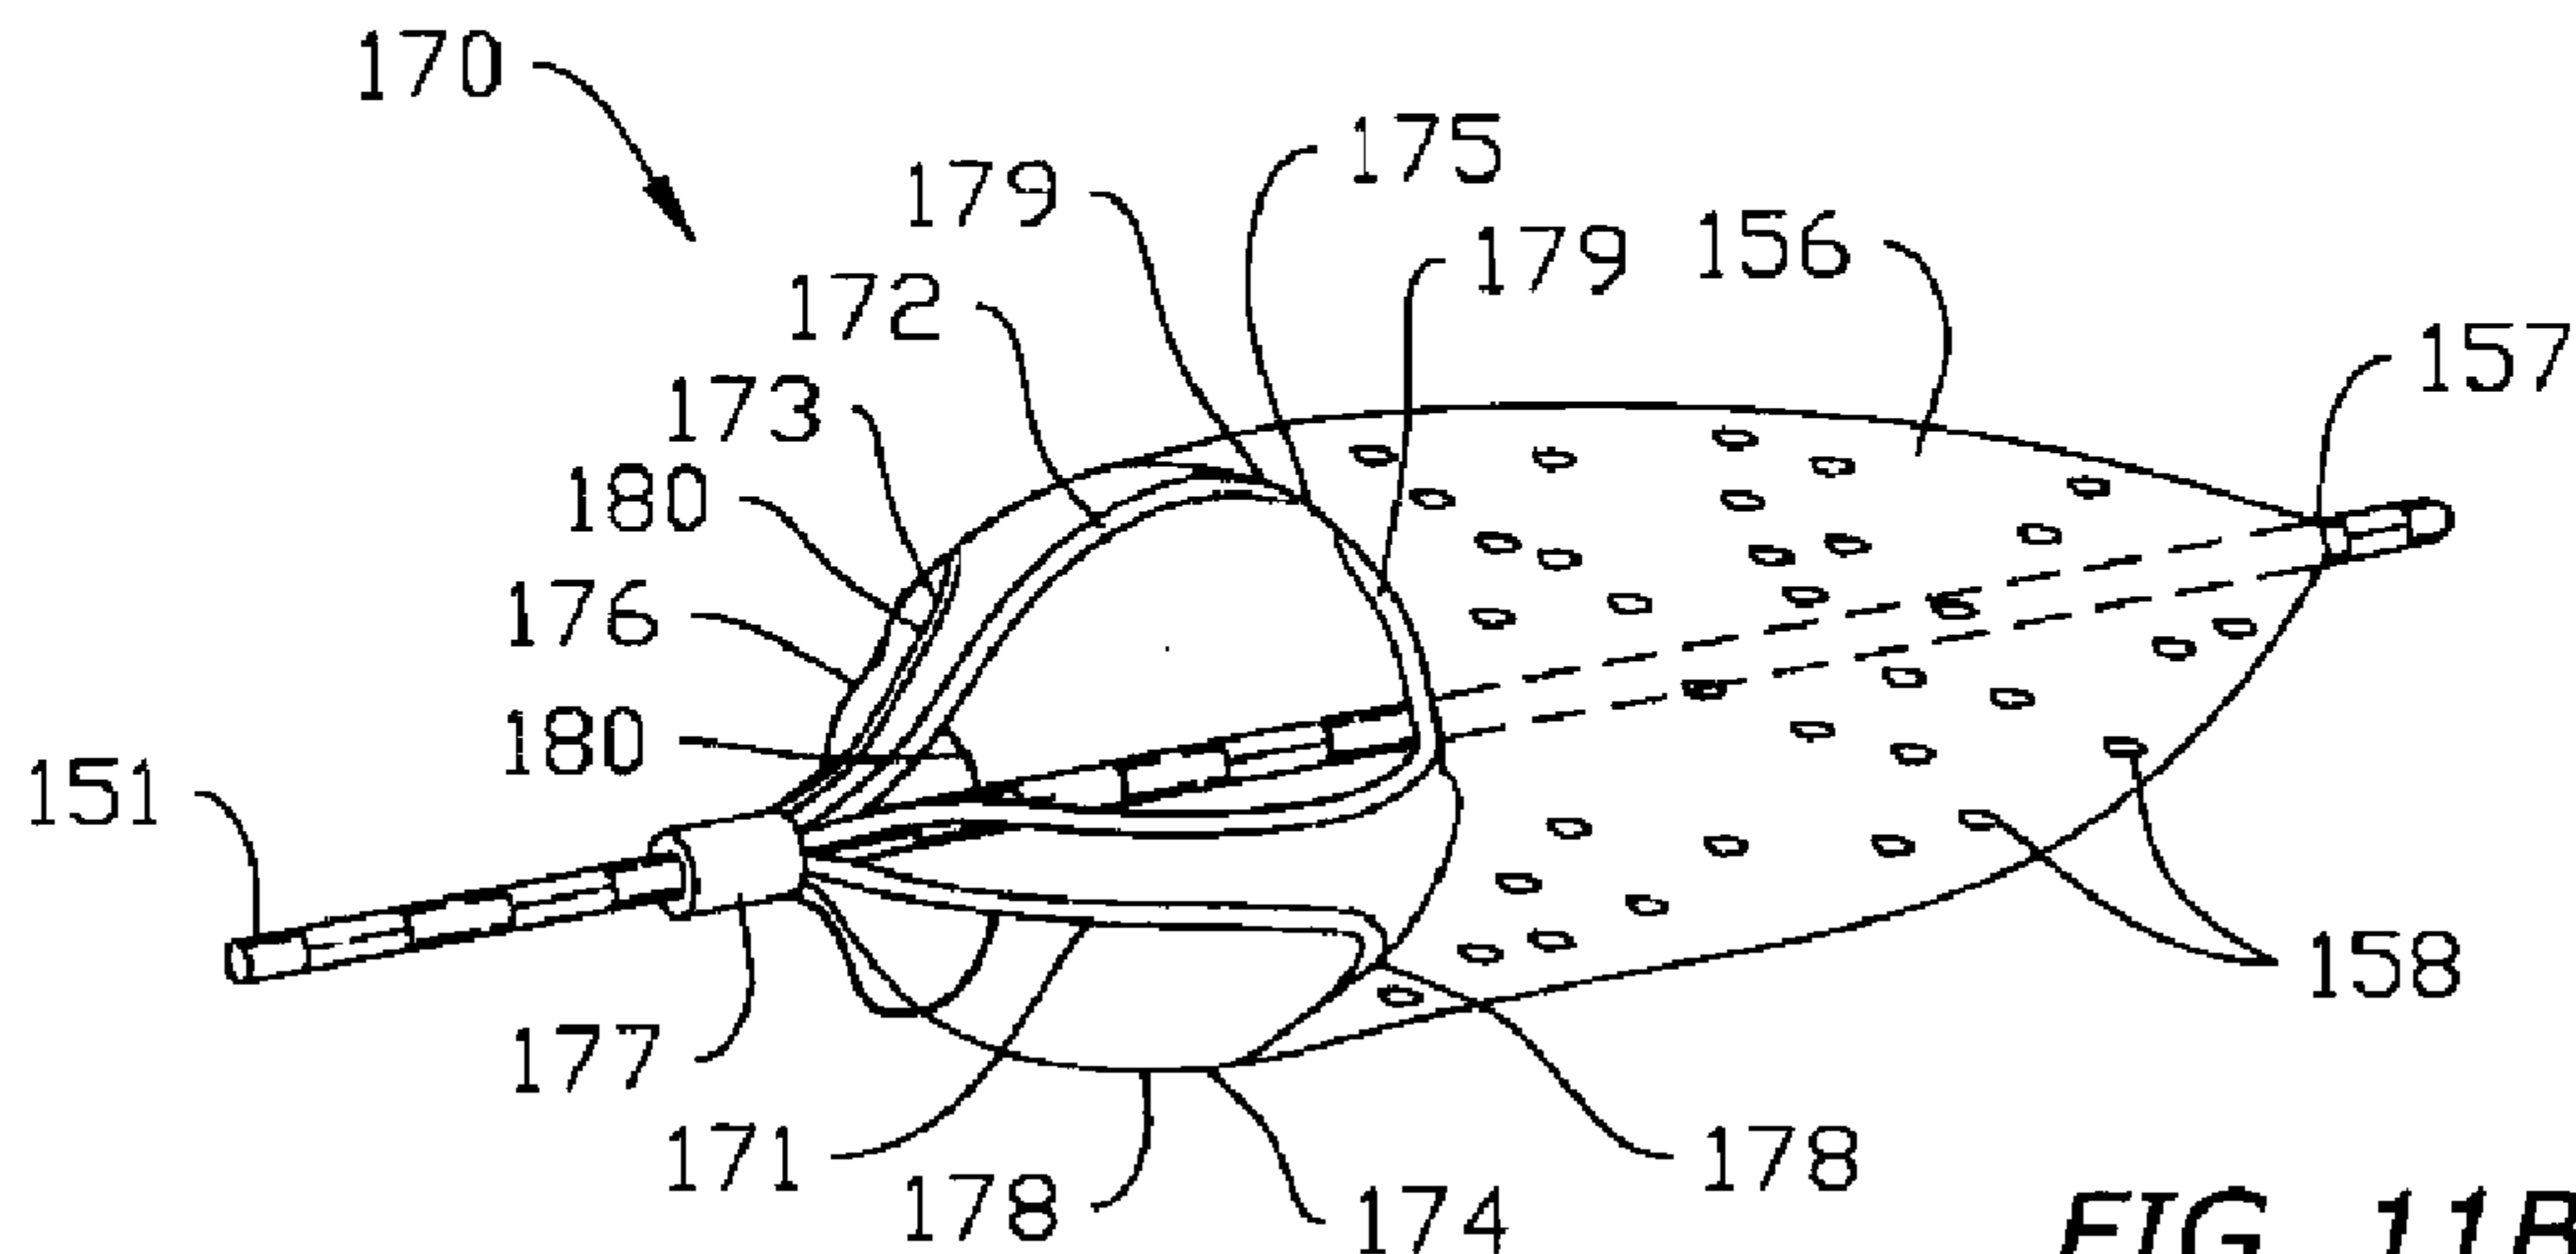


FIG. 11B

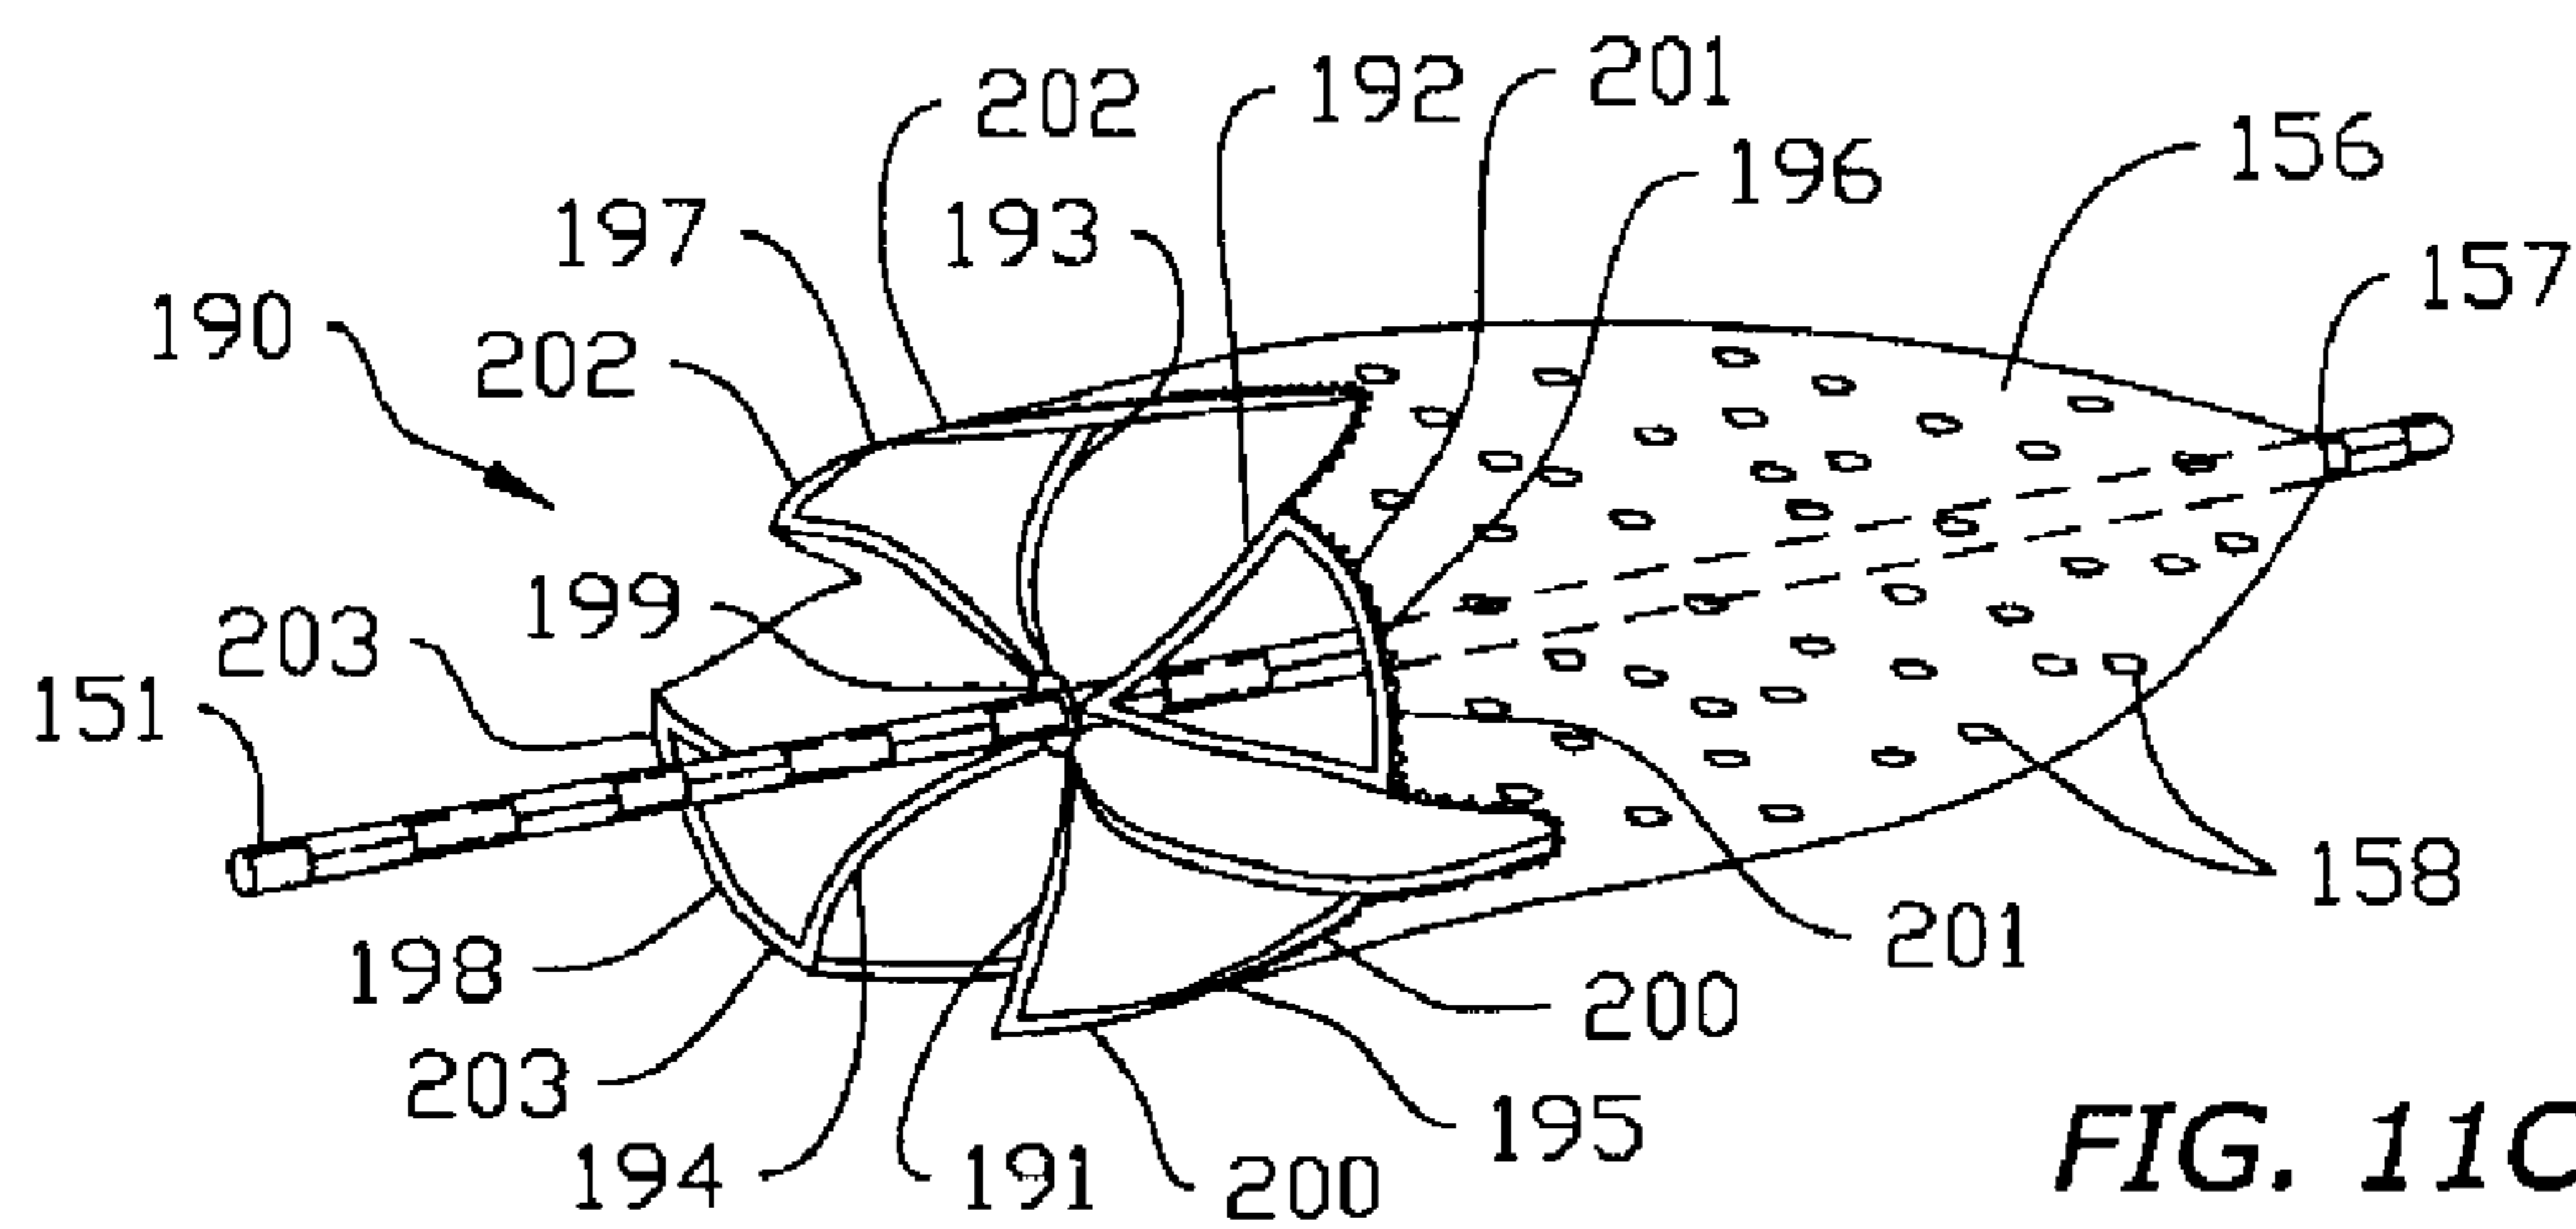


FIG. 11C

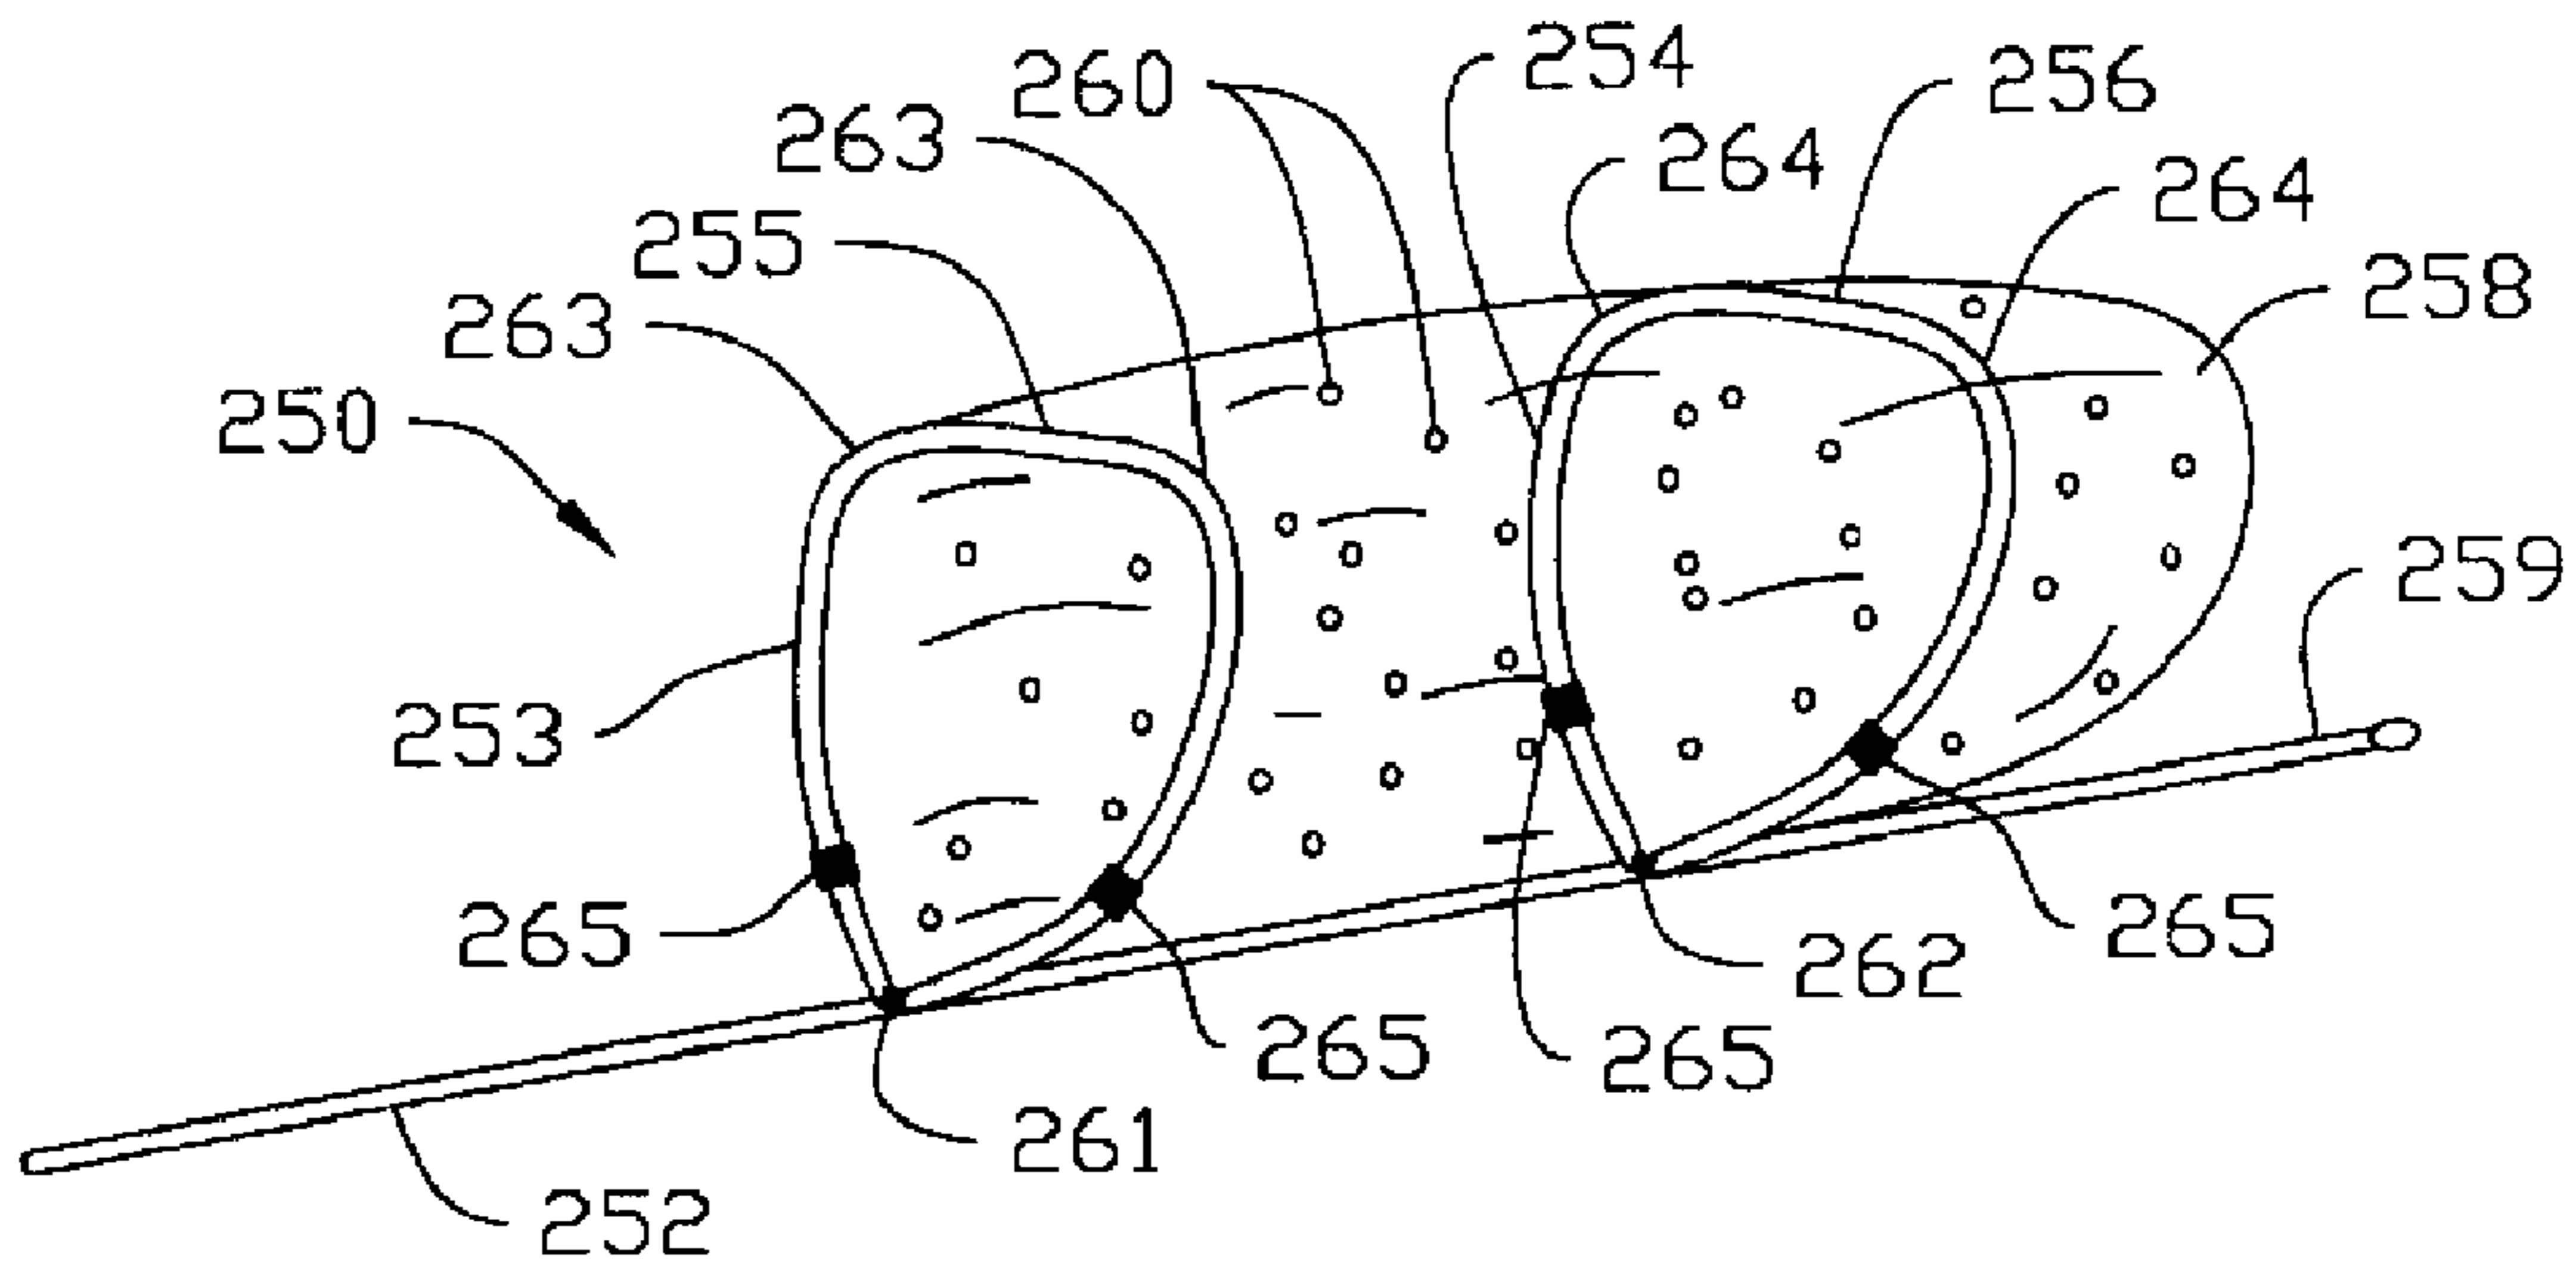


FIG. 12

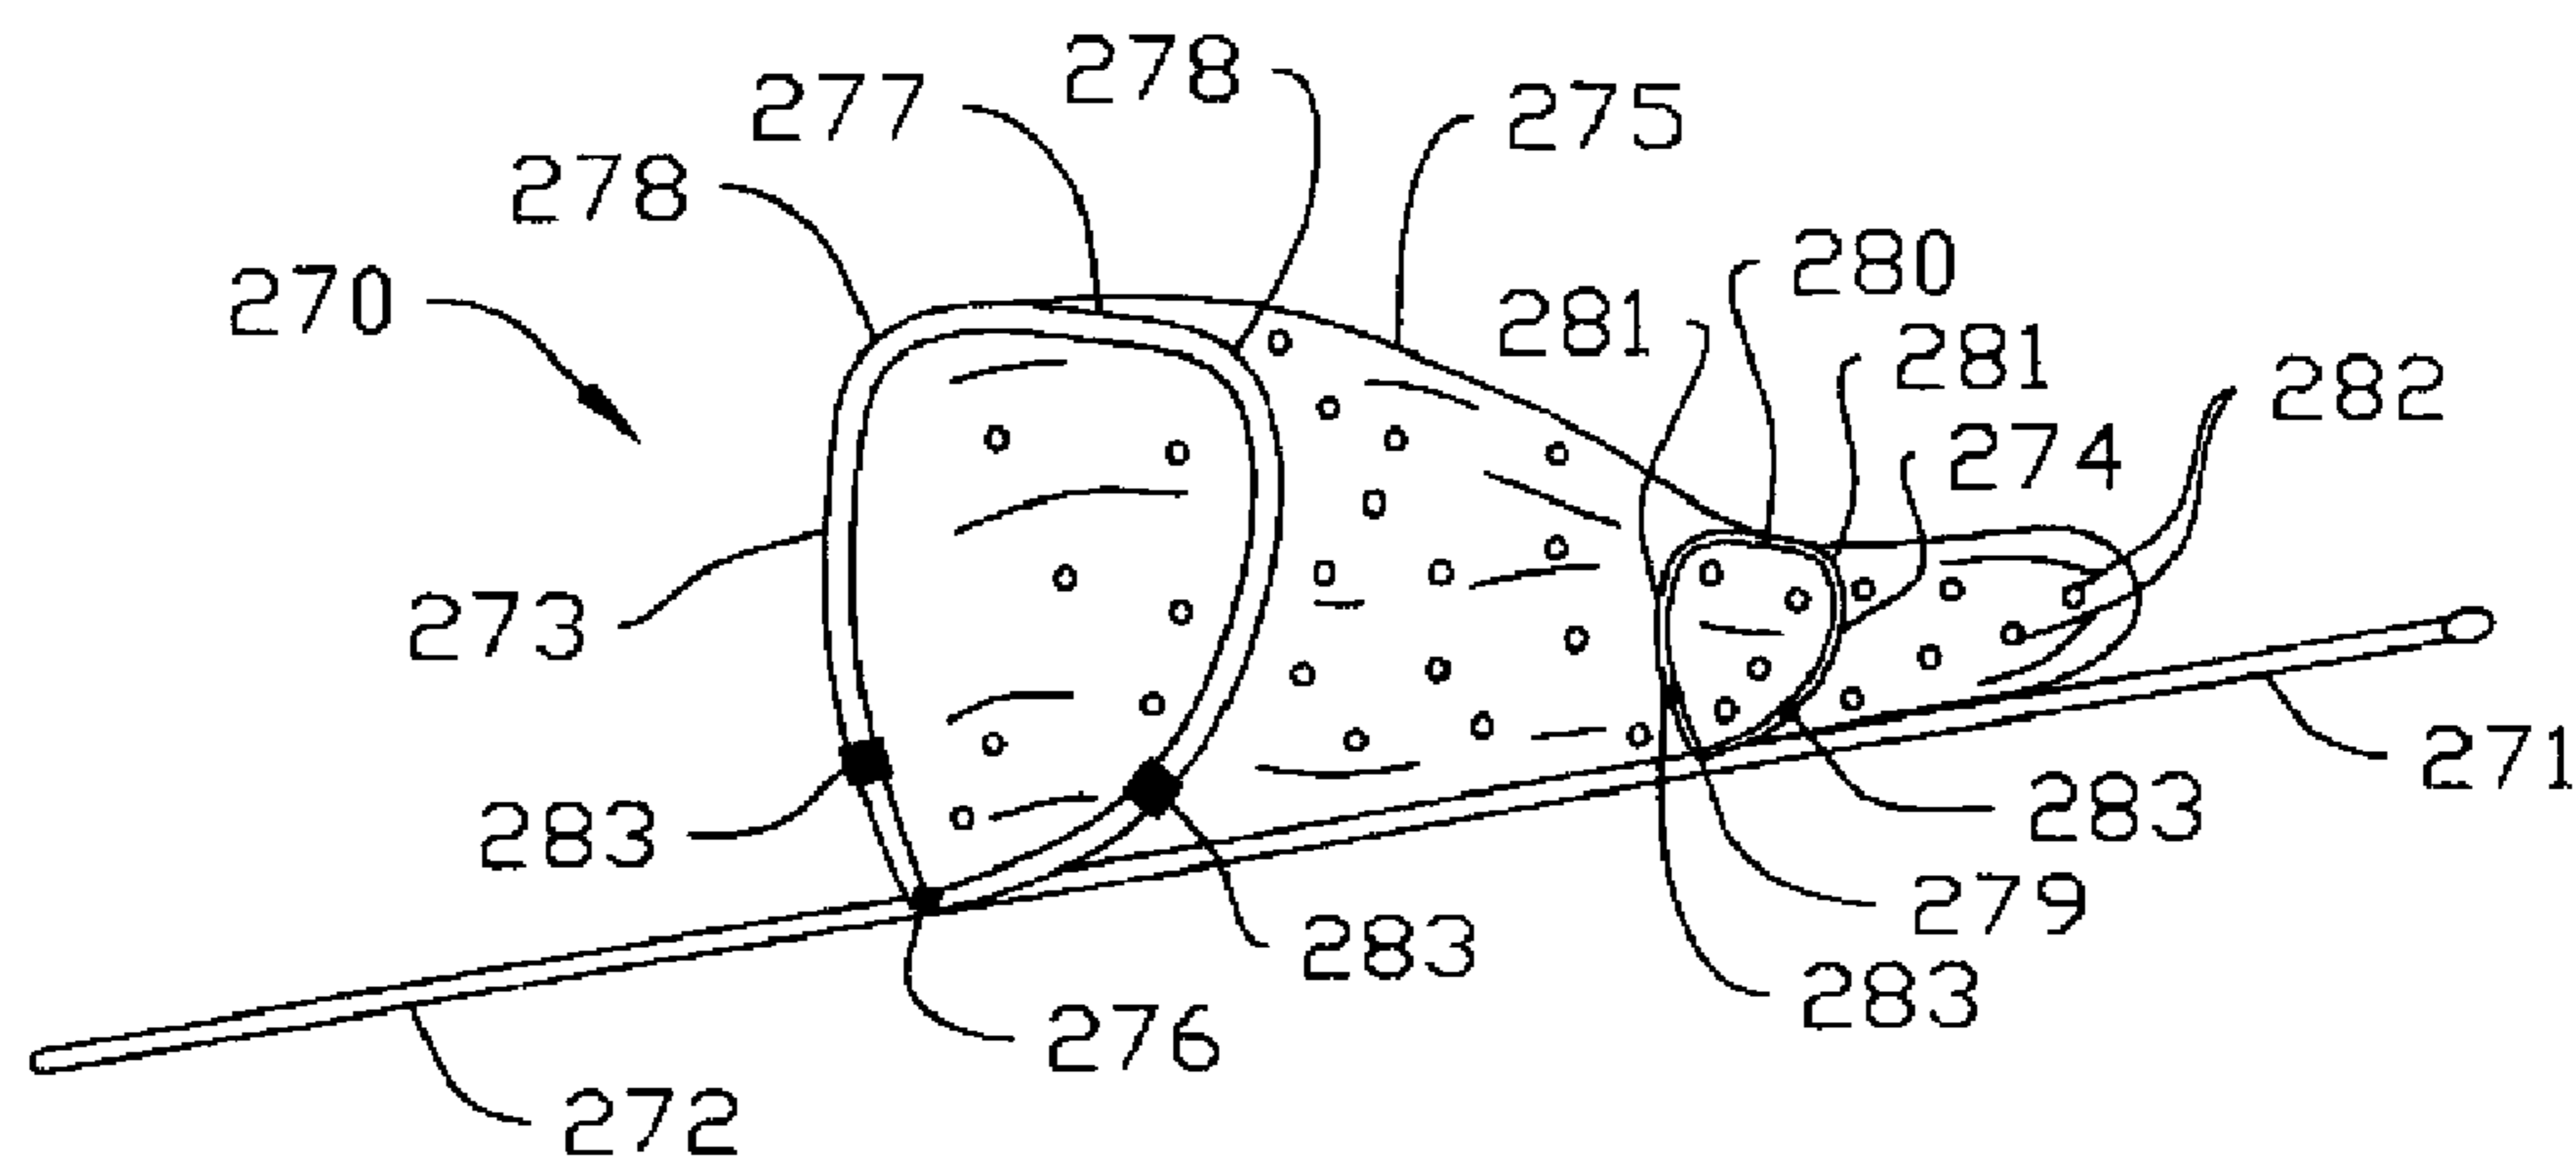
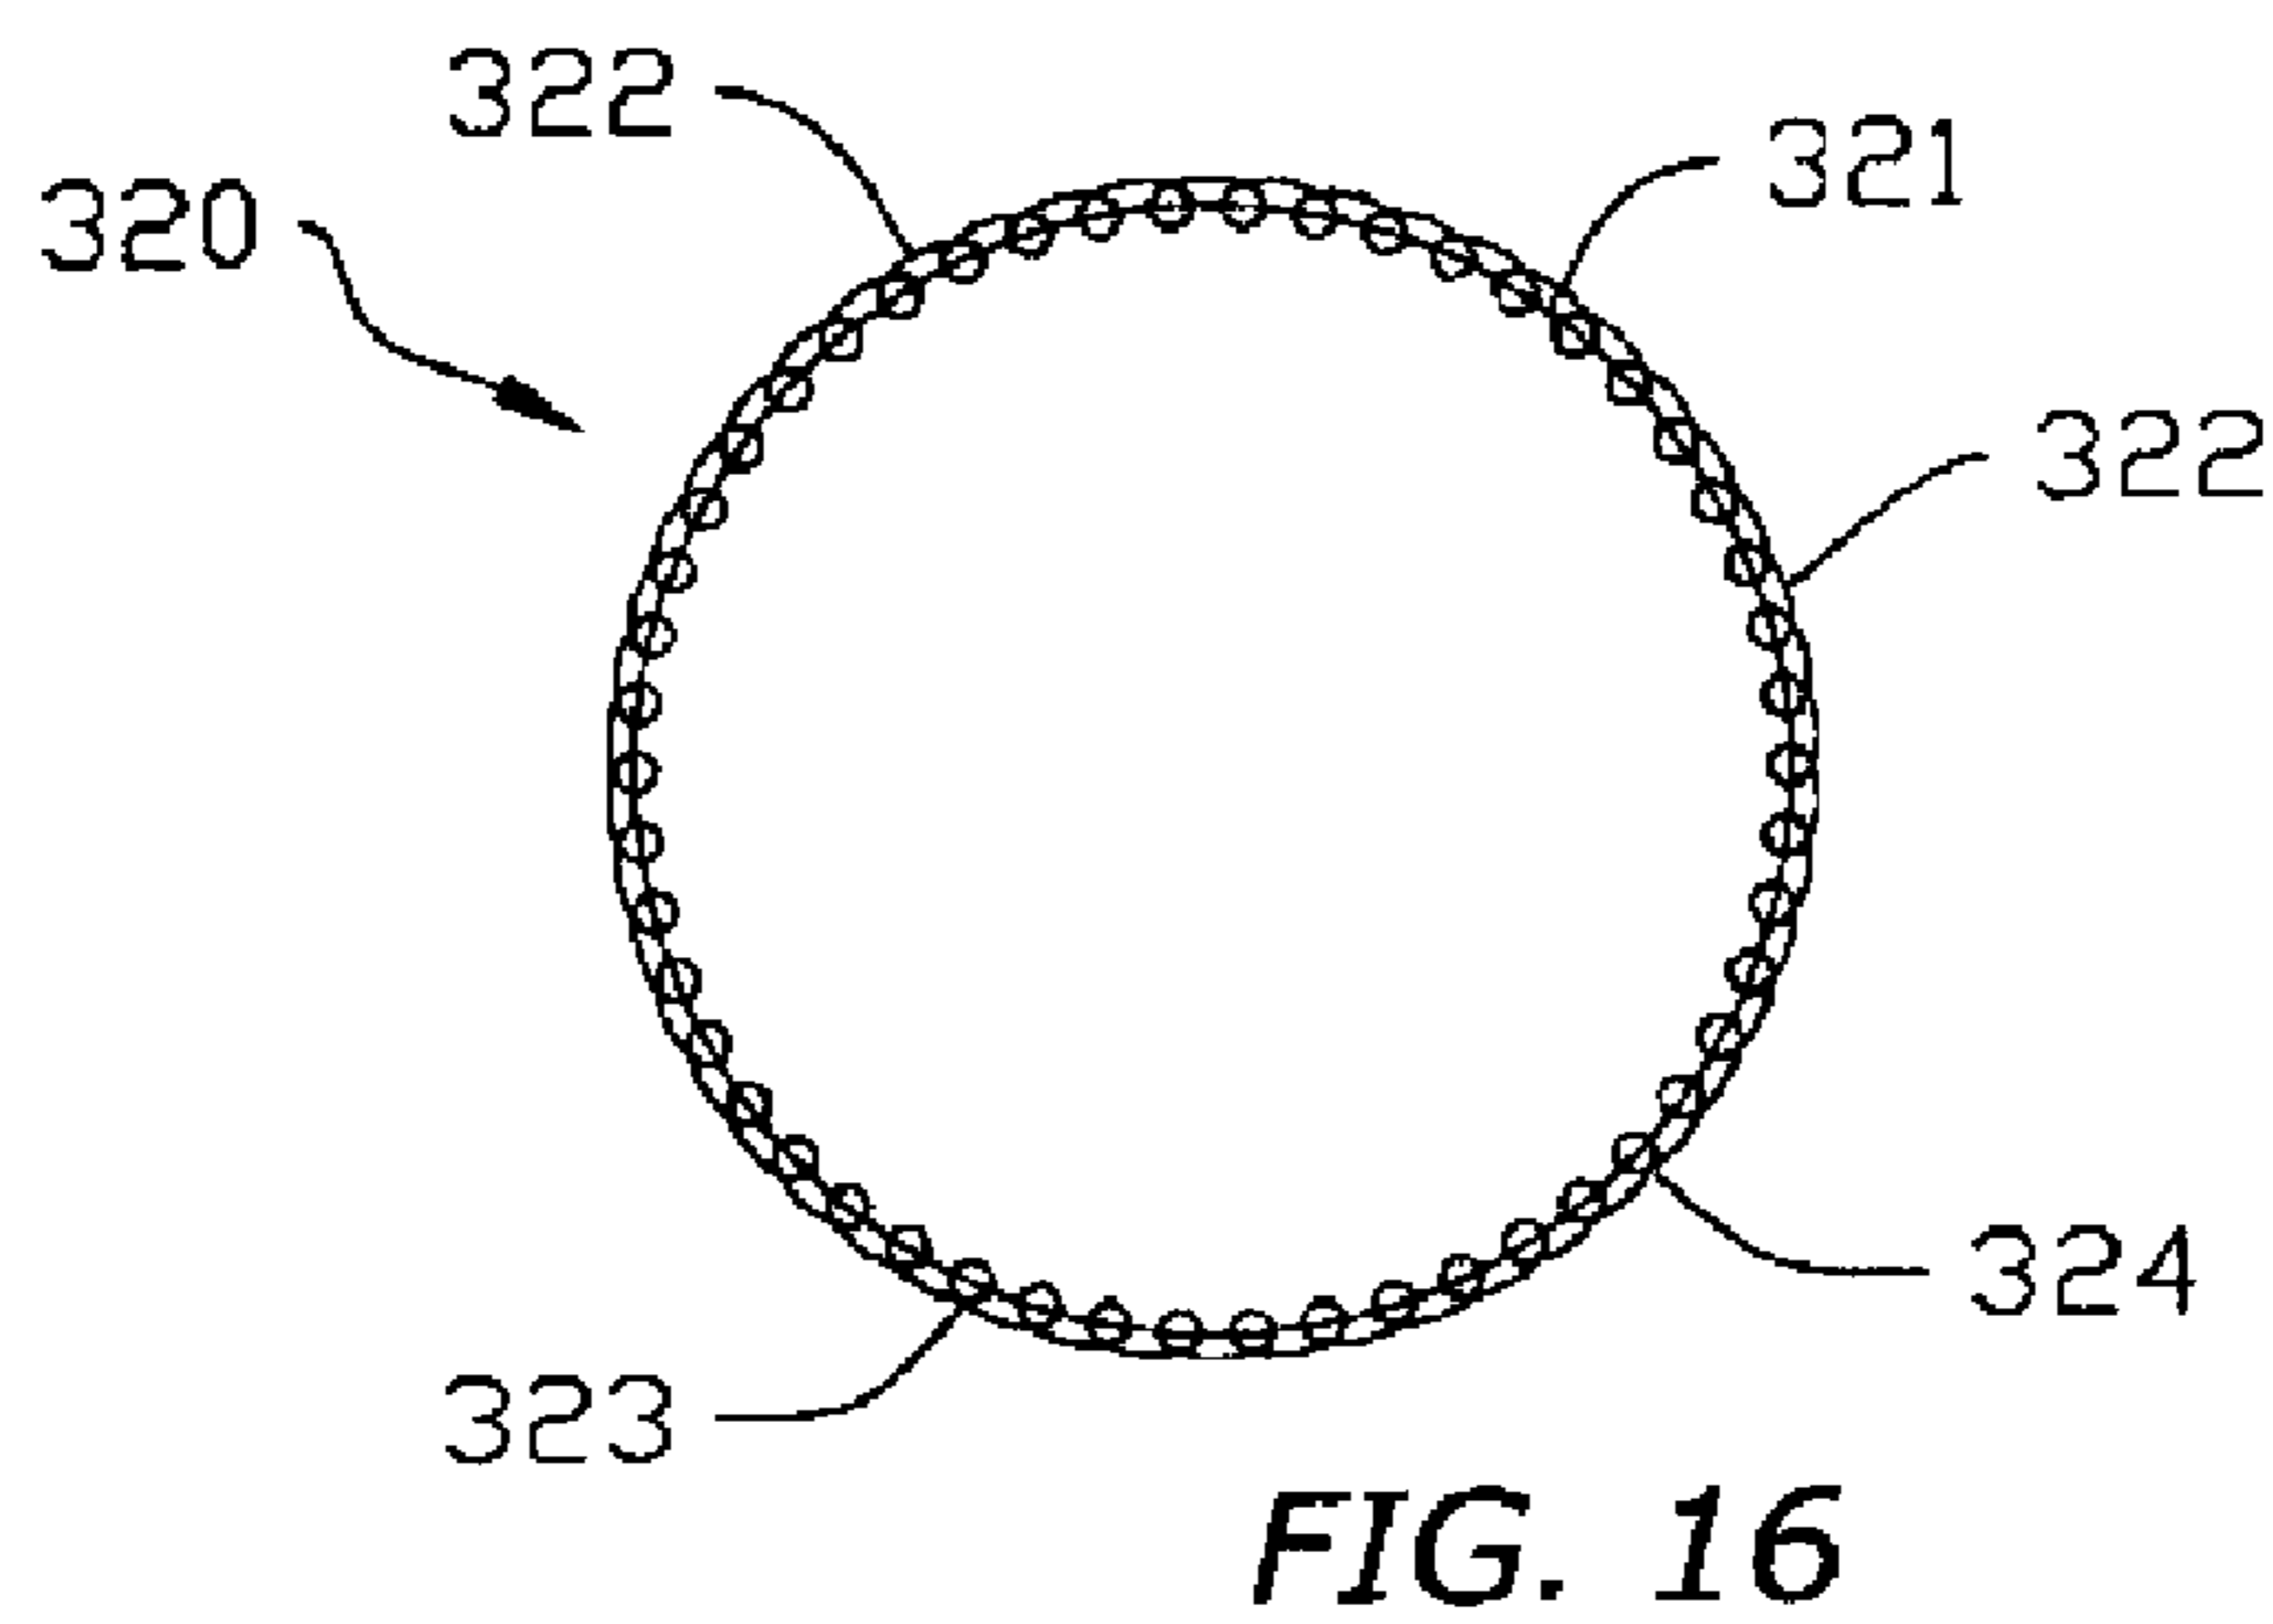
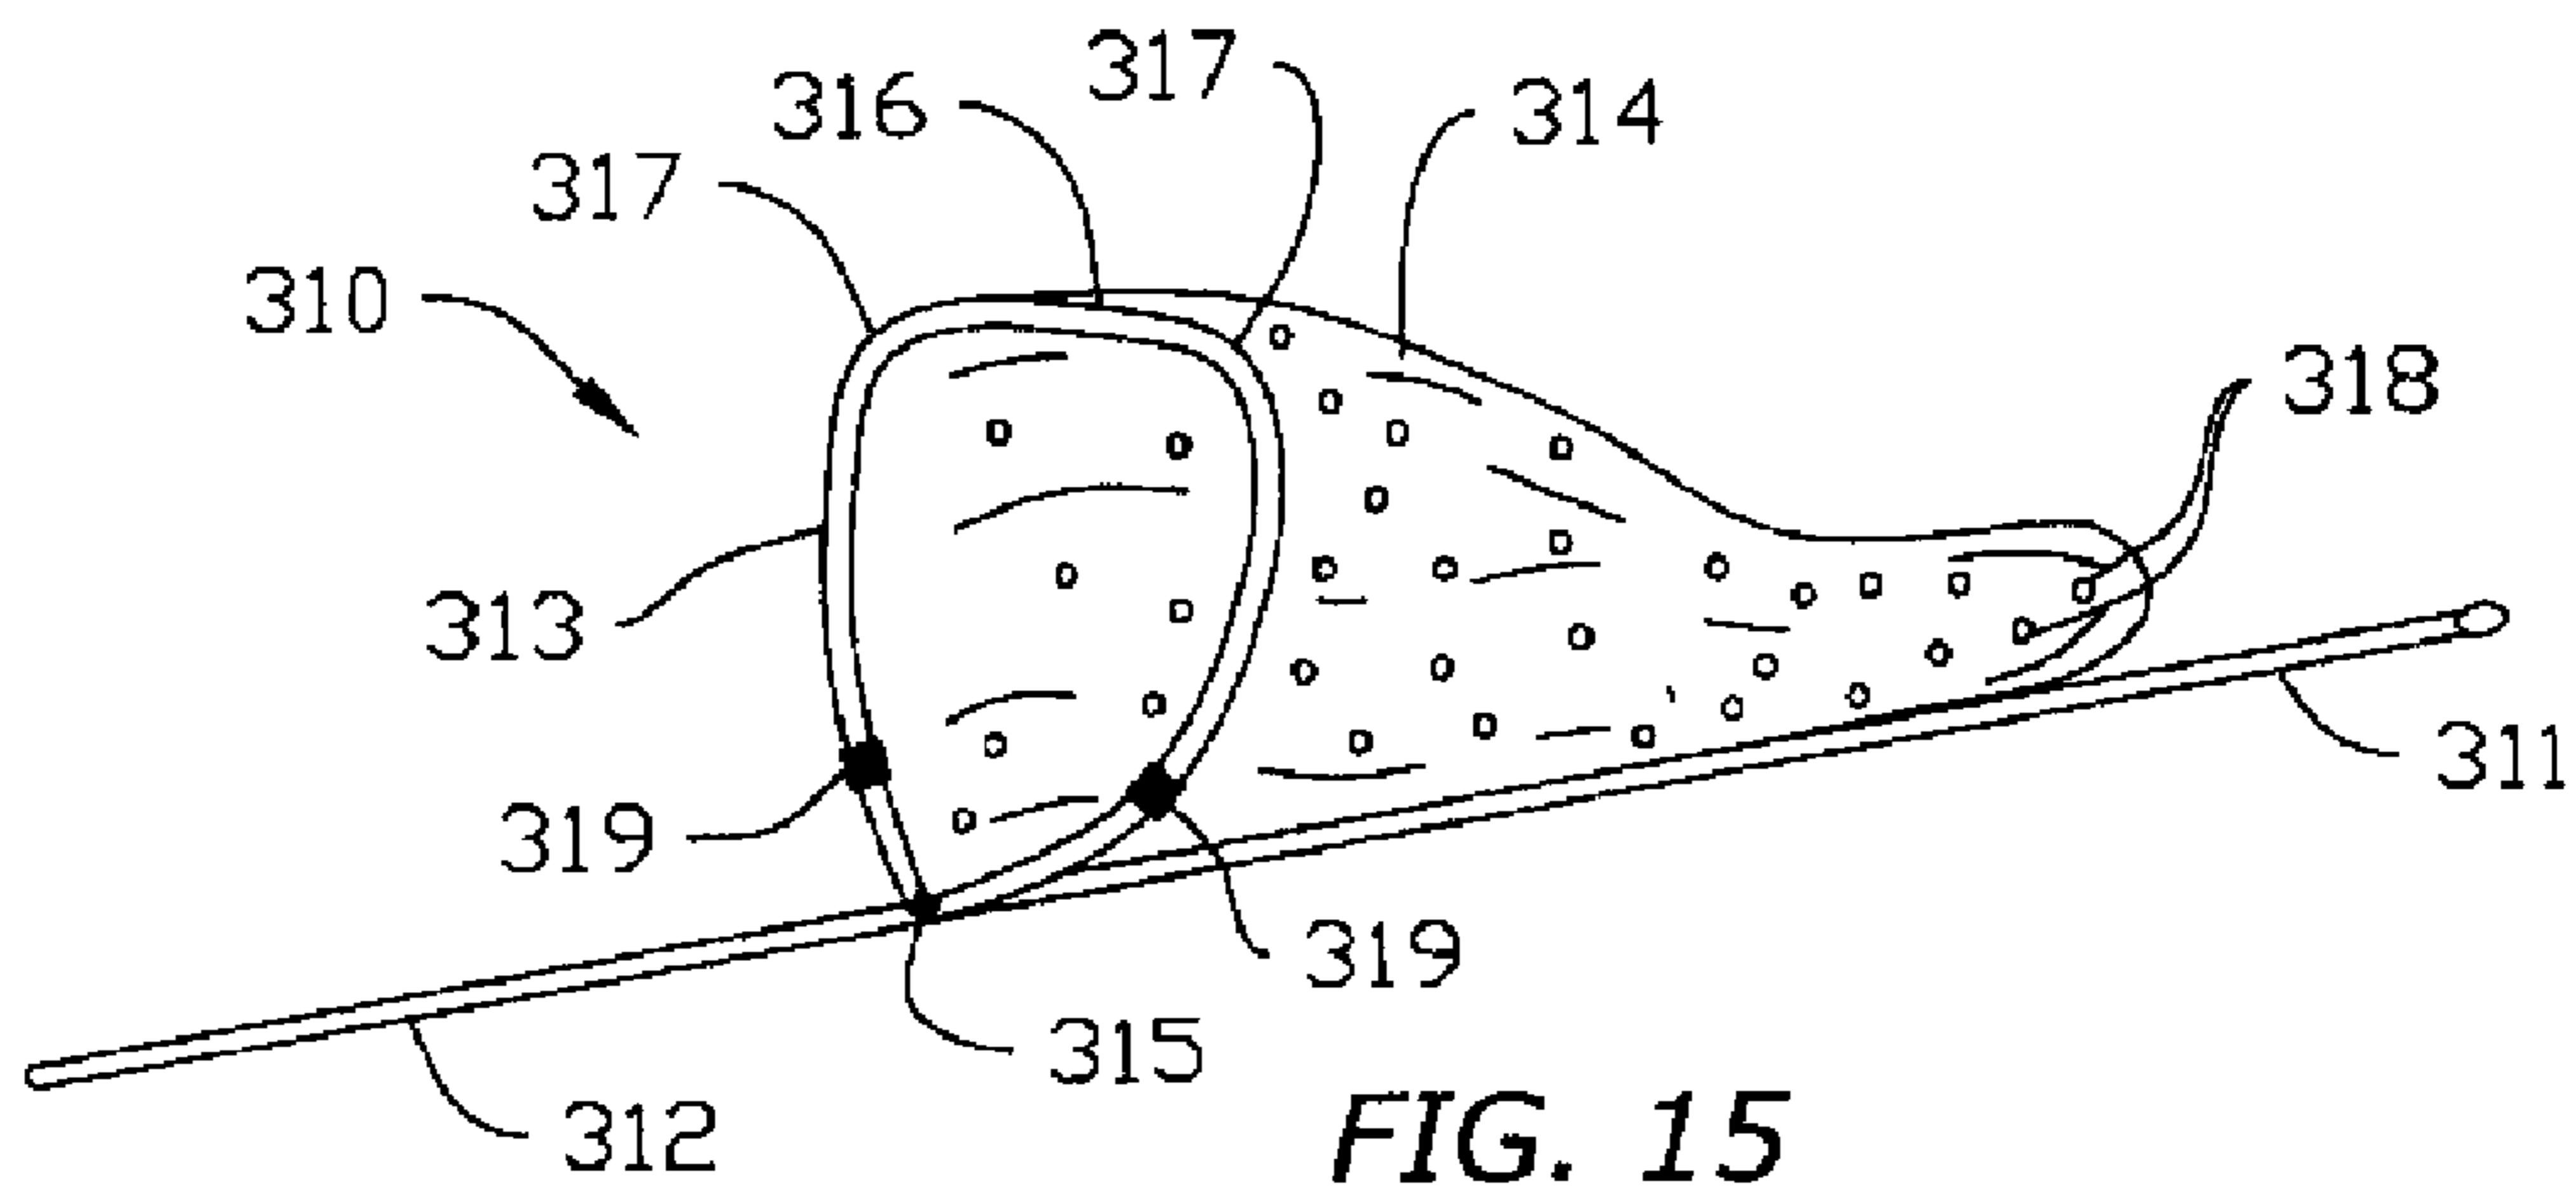
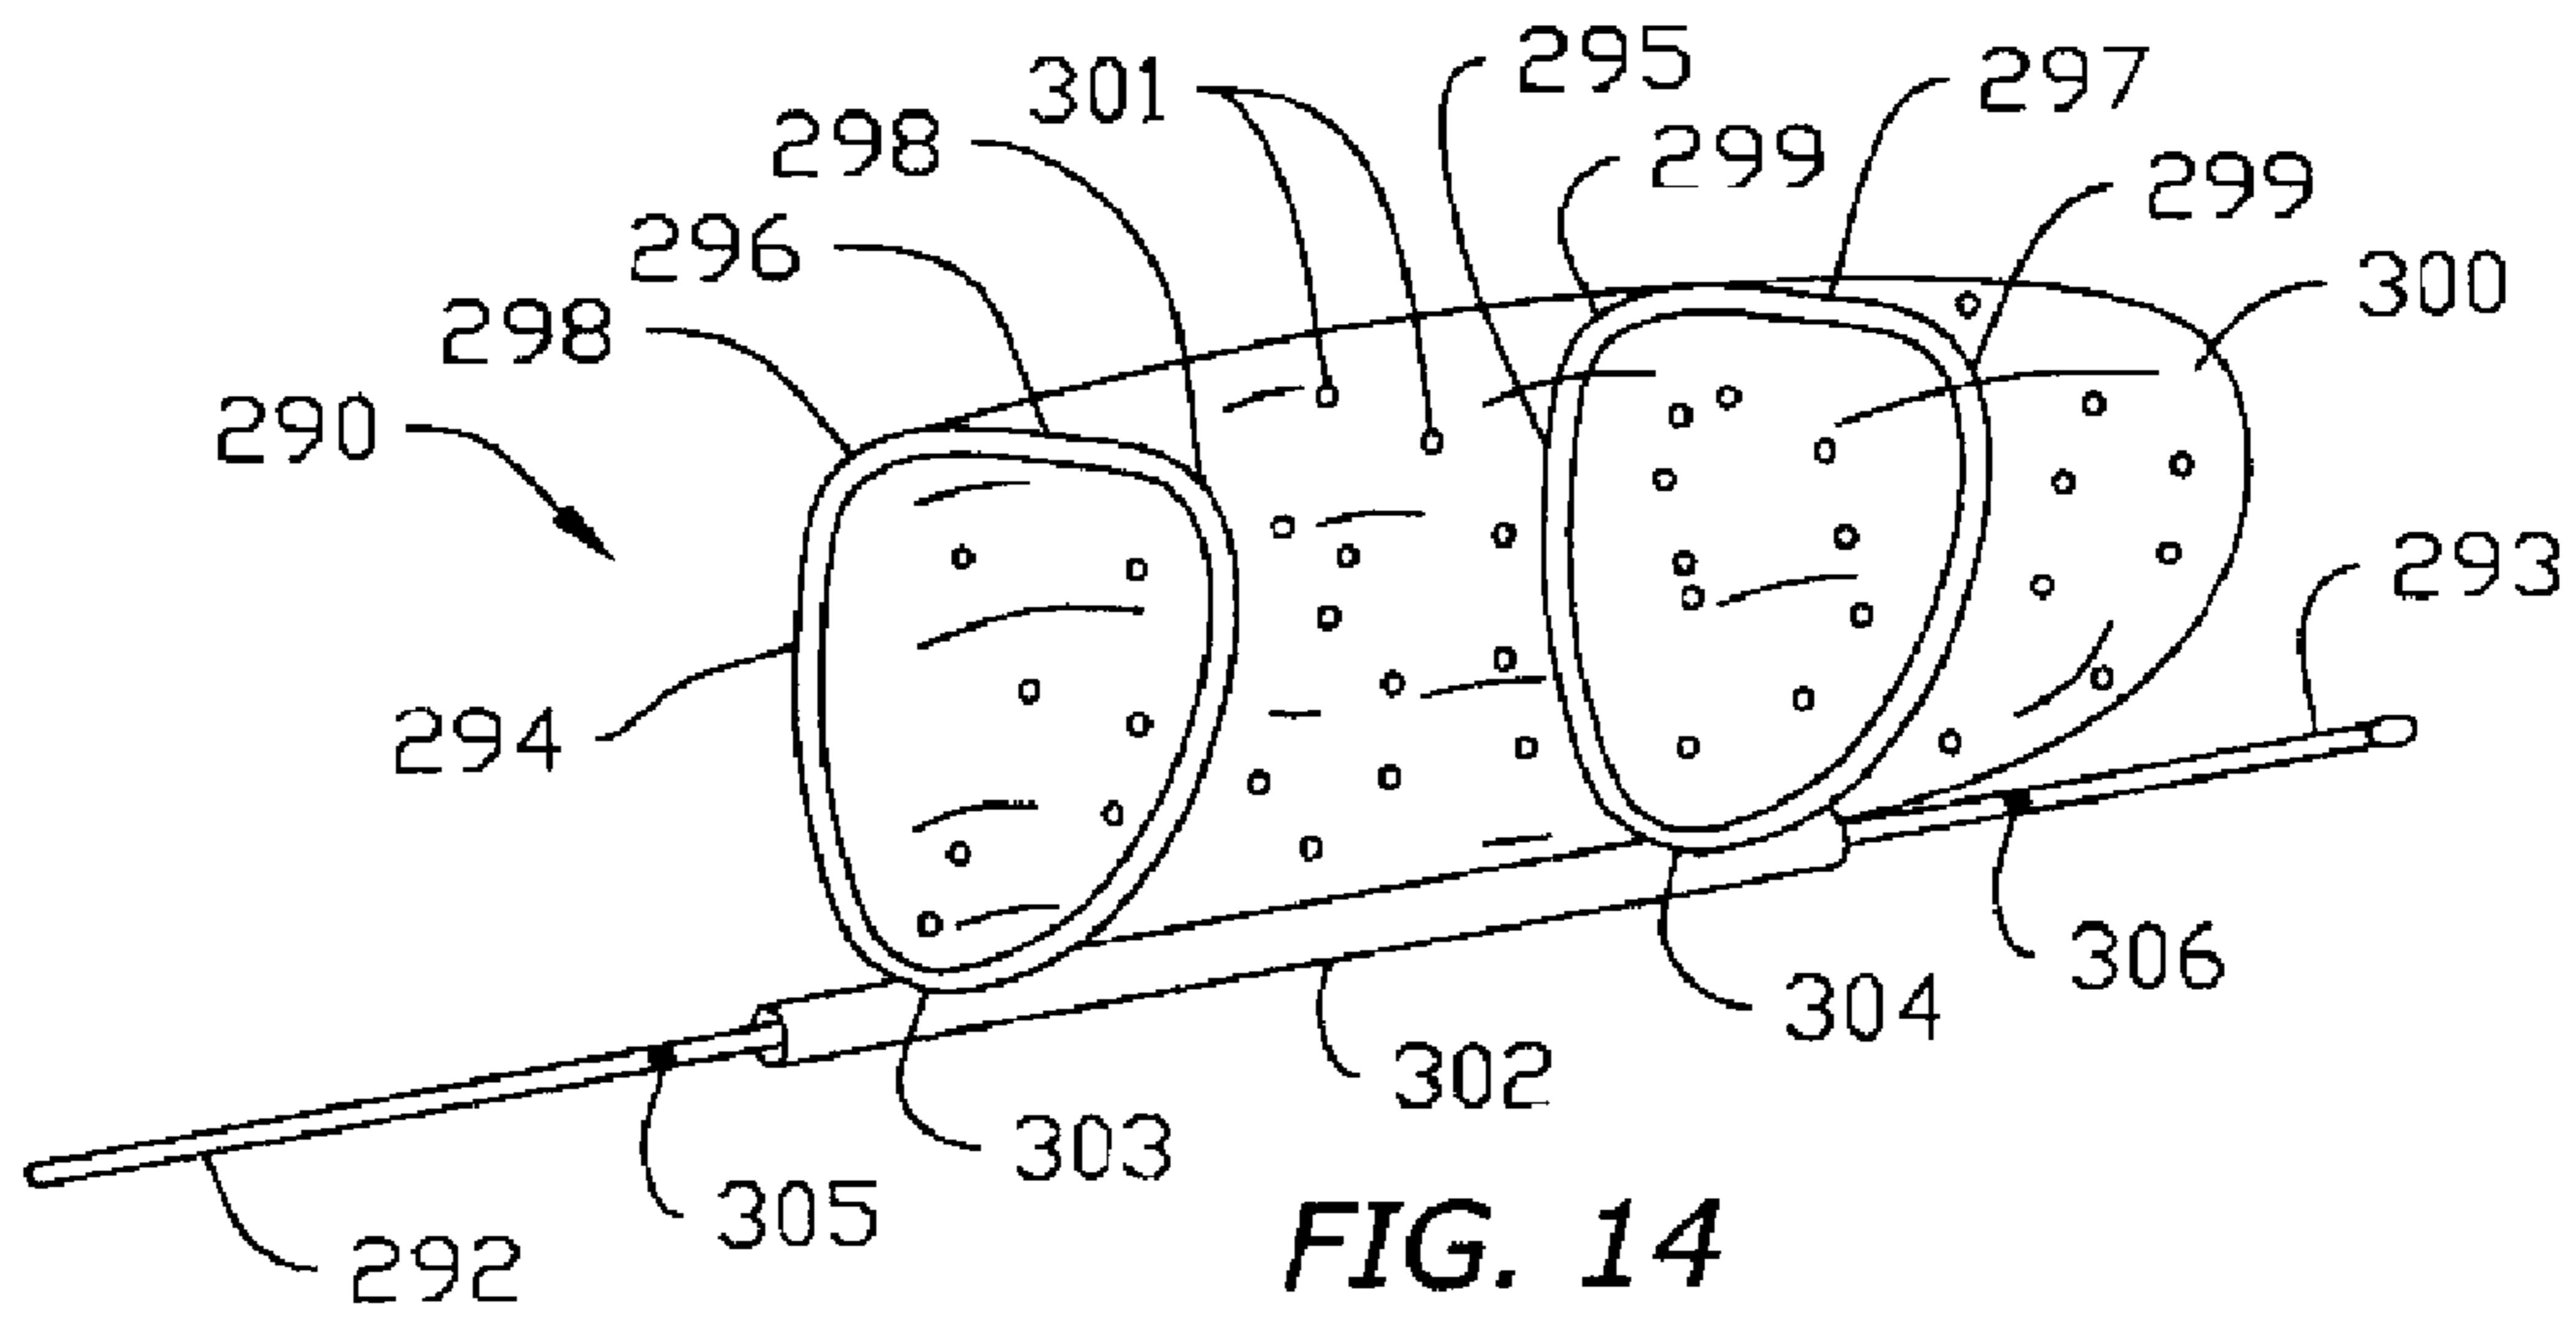
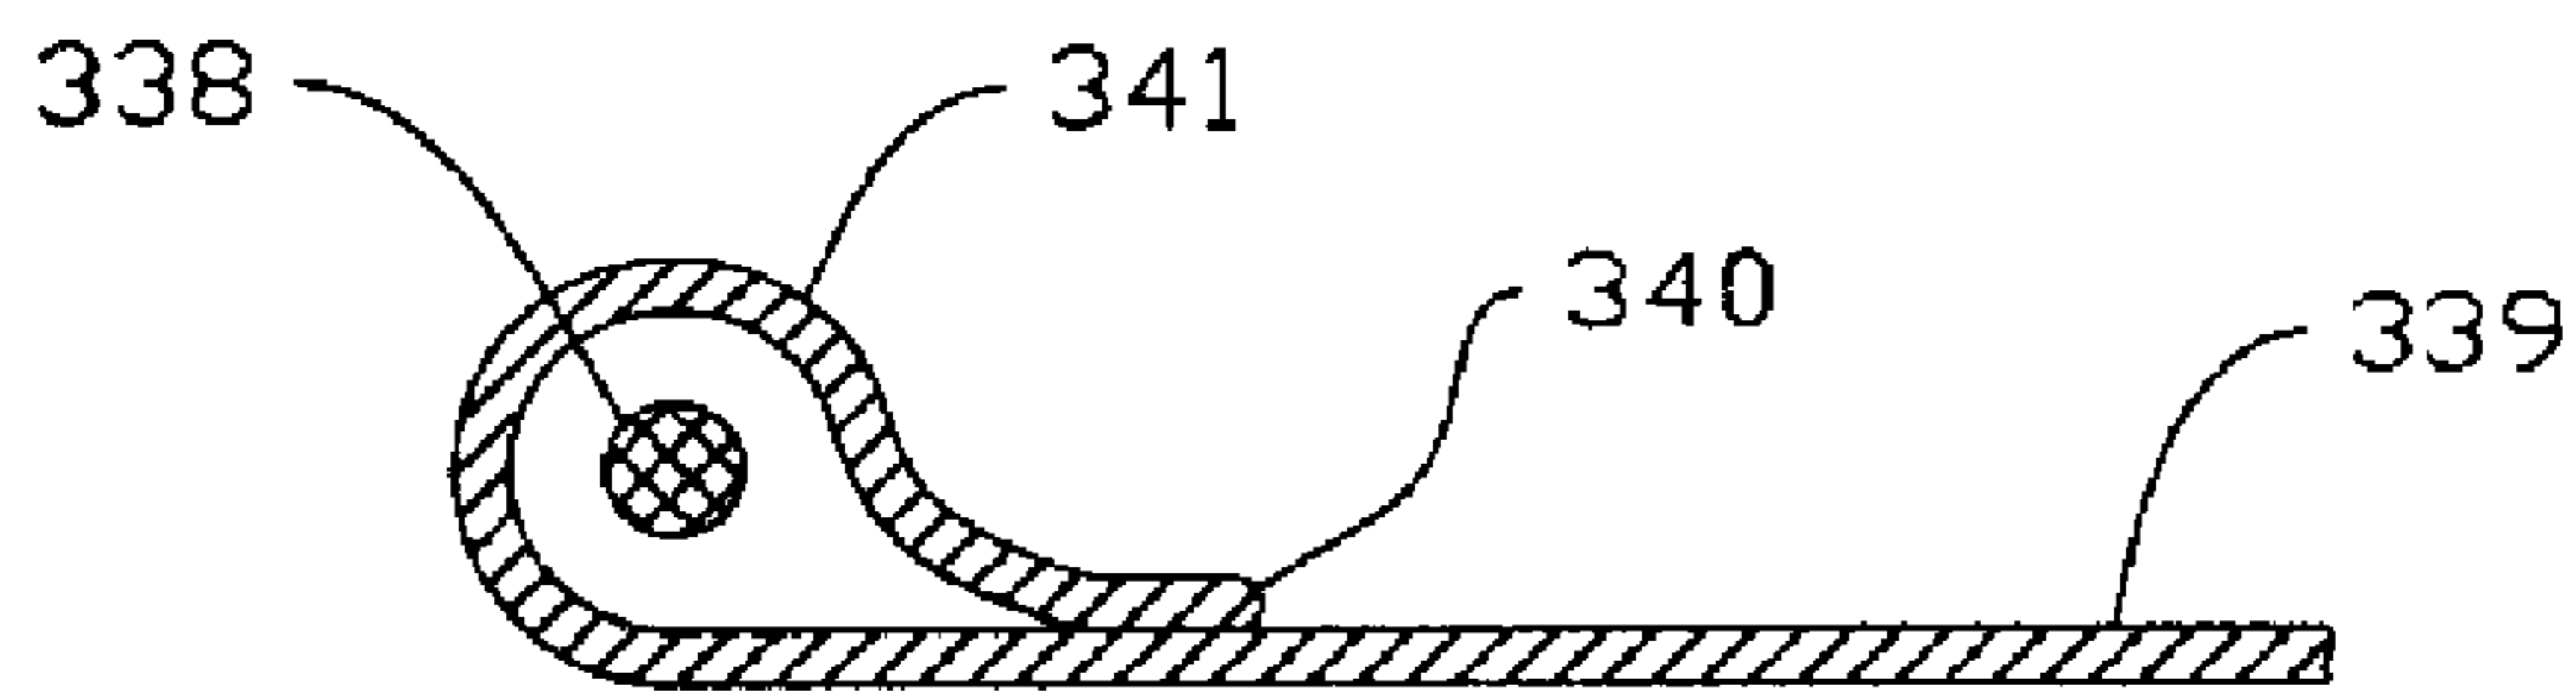
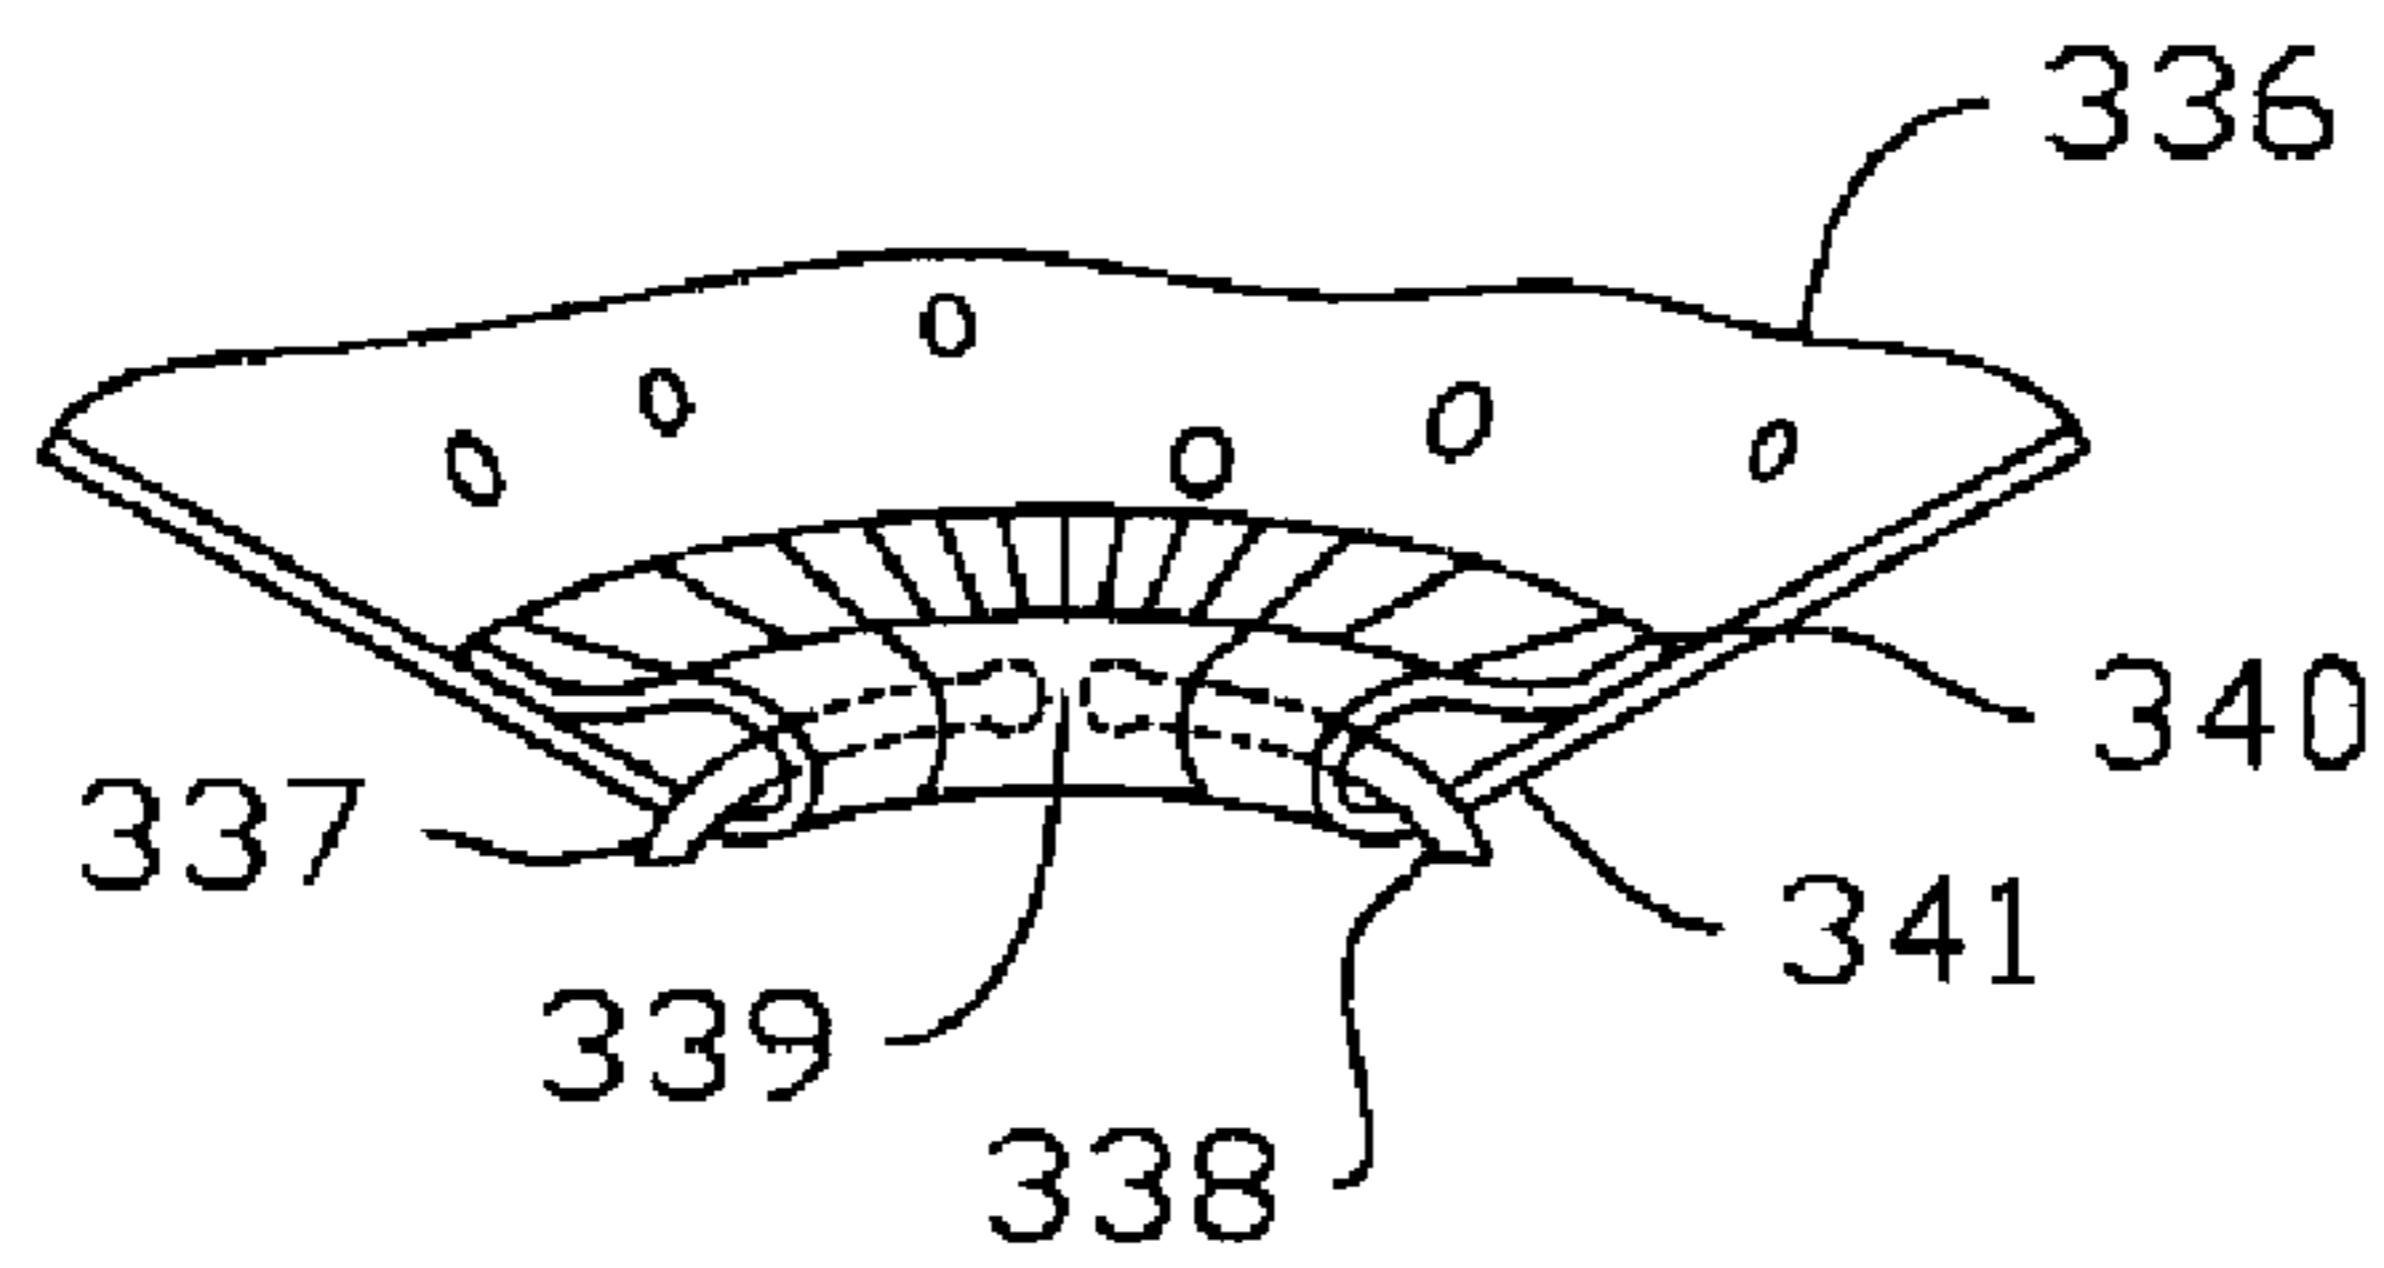
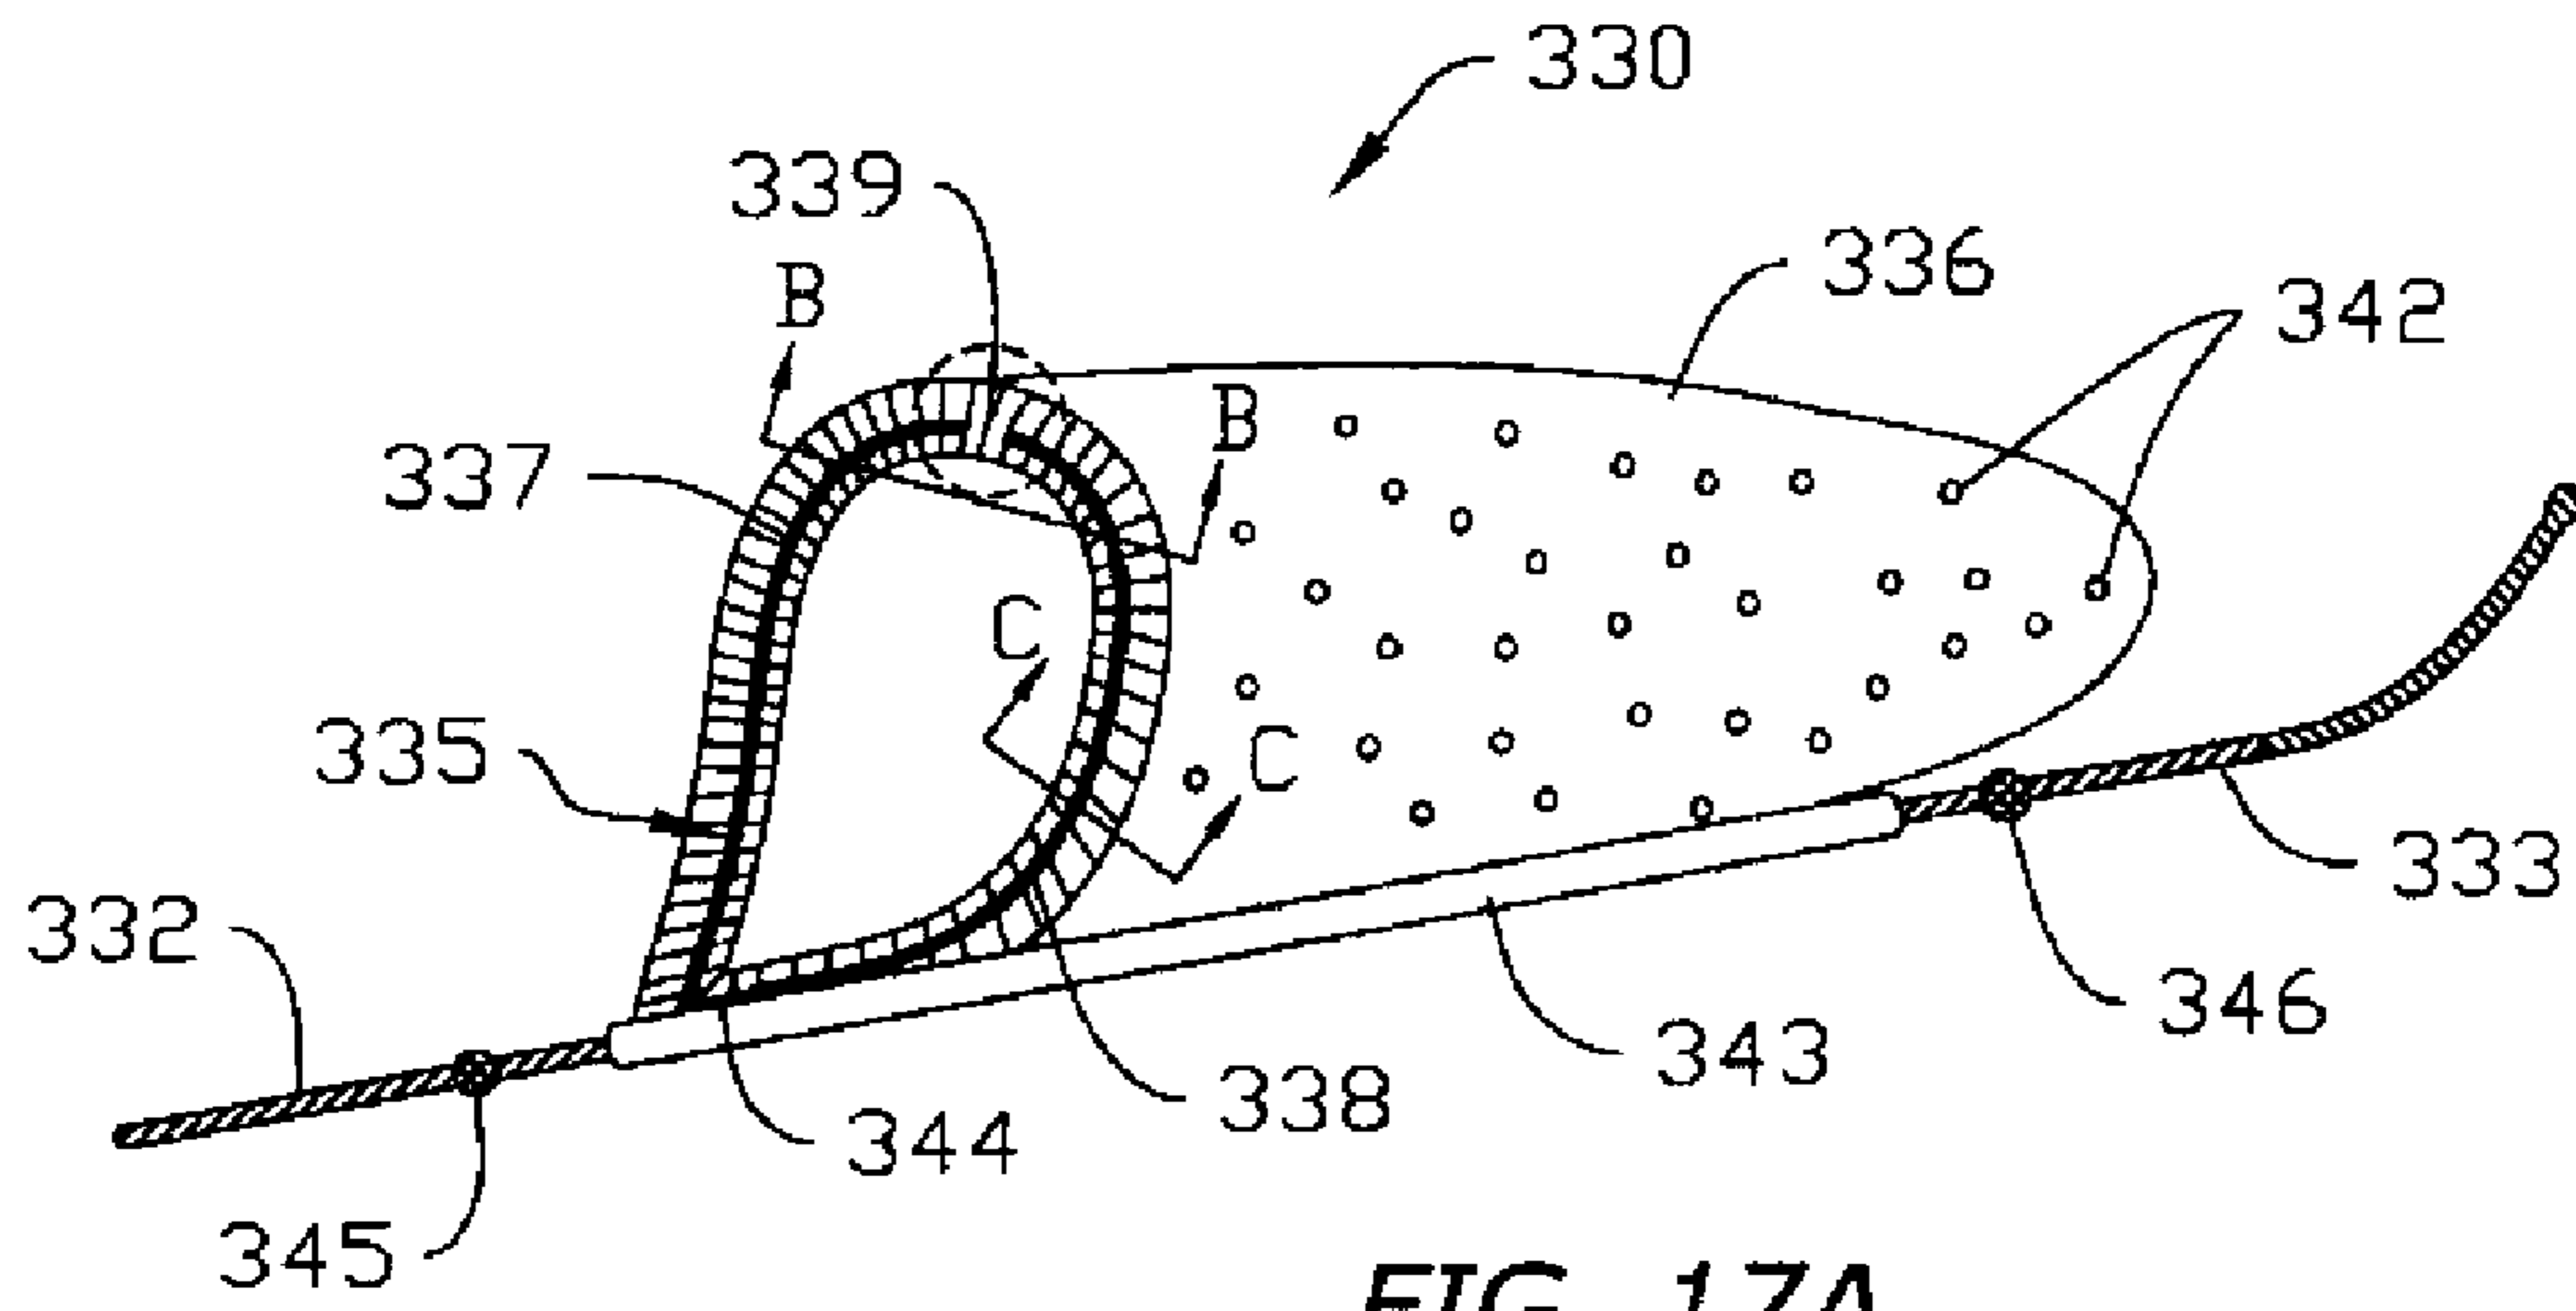
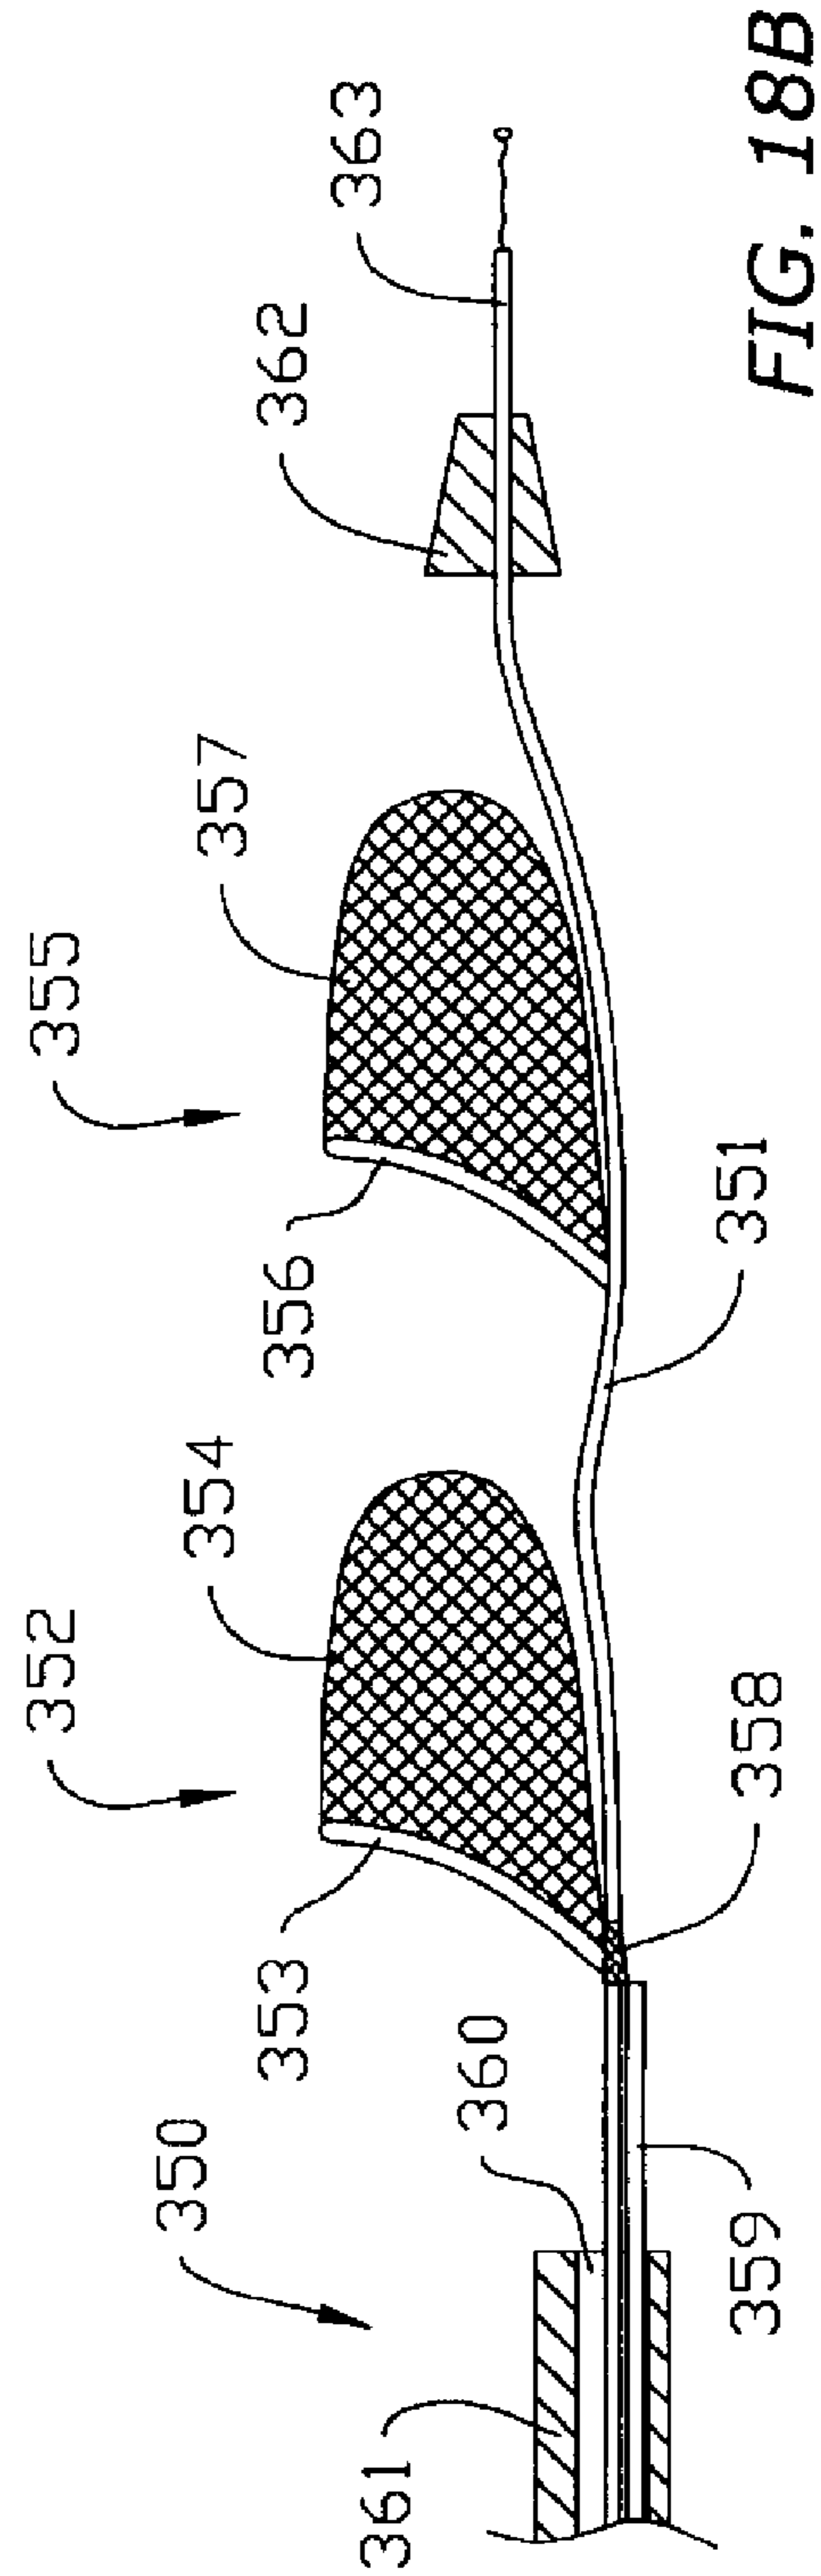
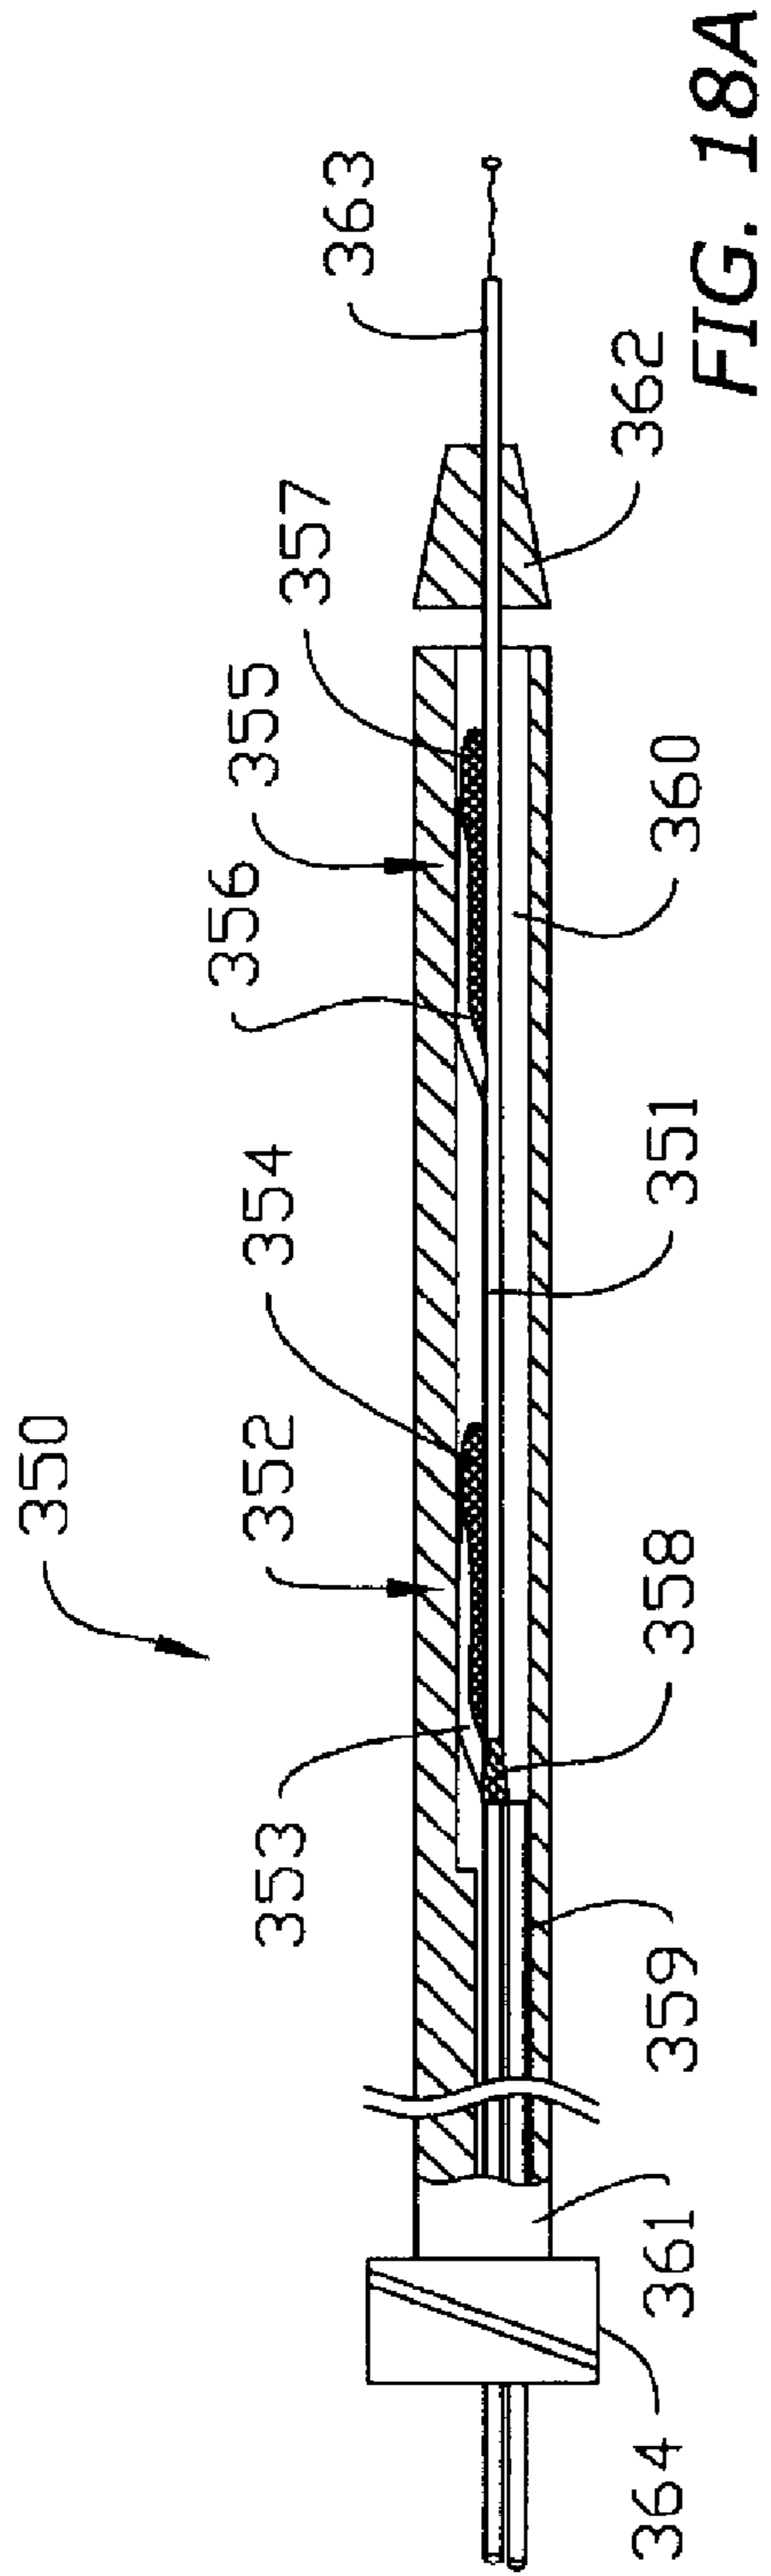
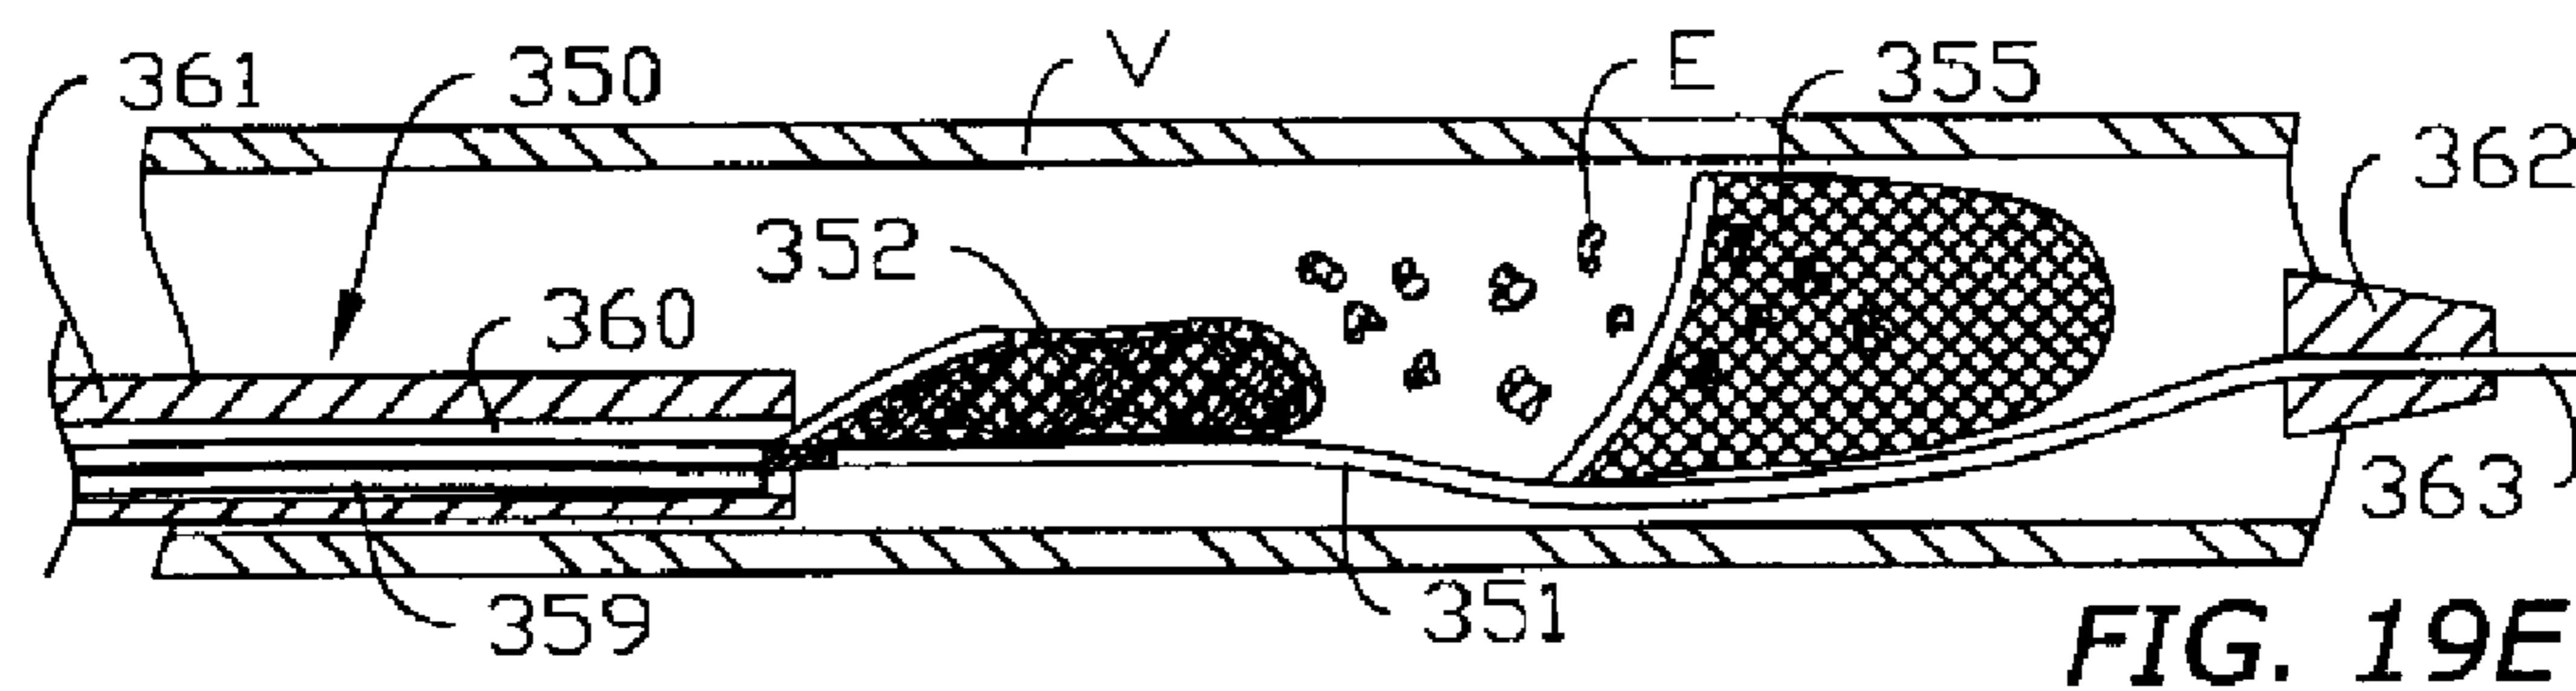
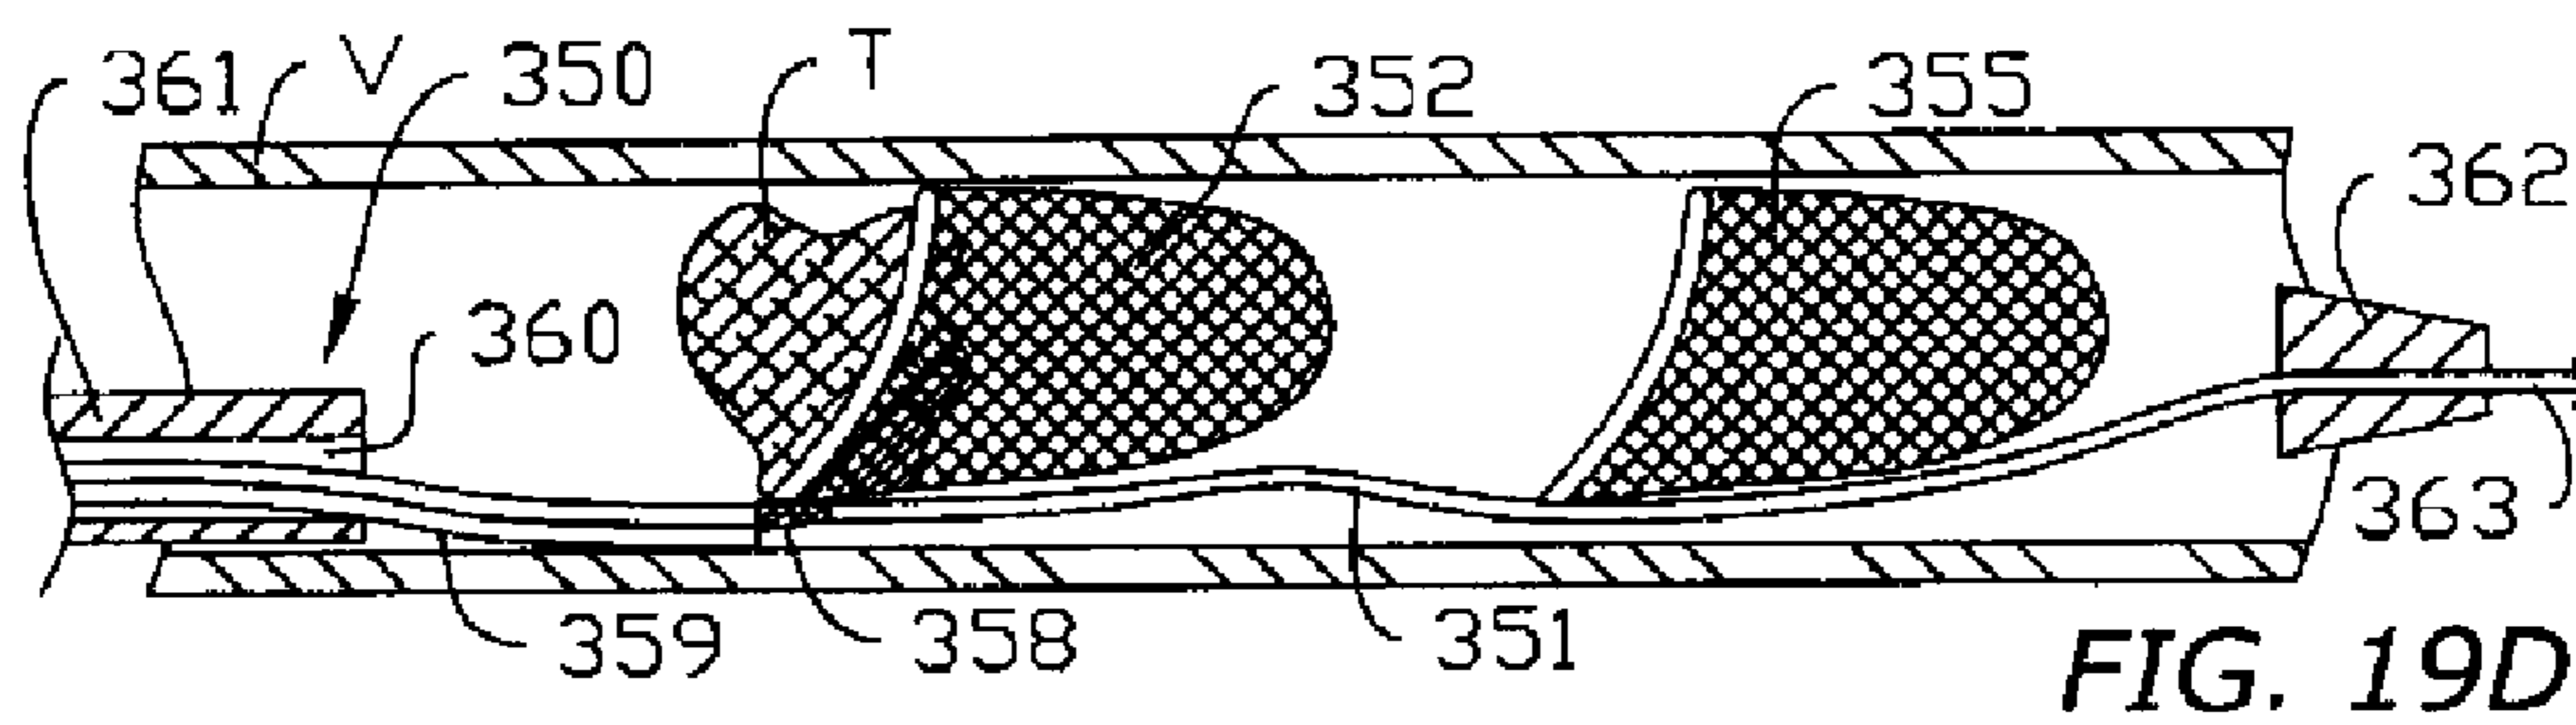
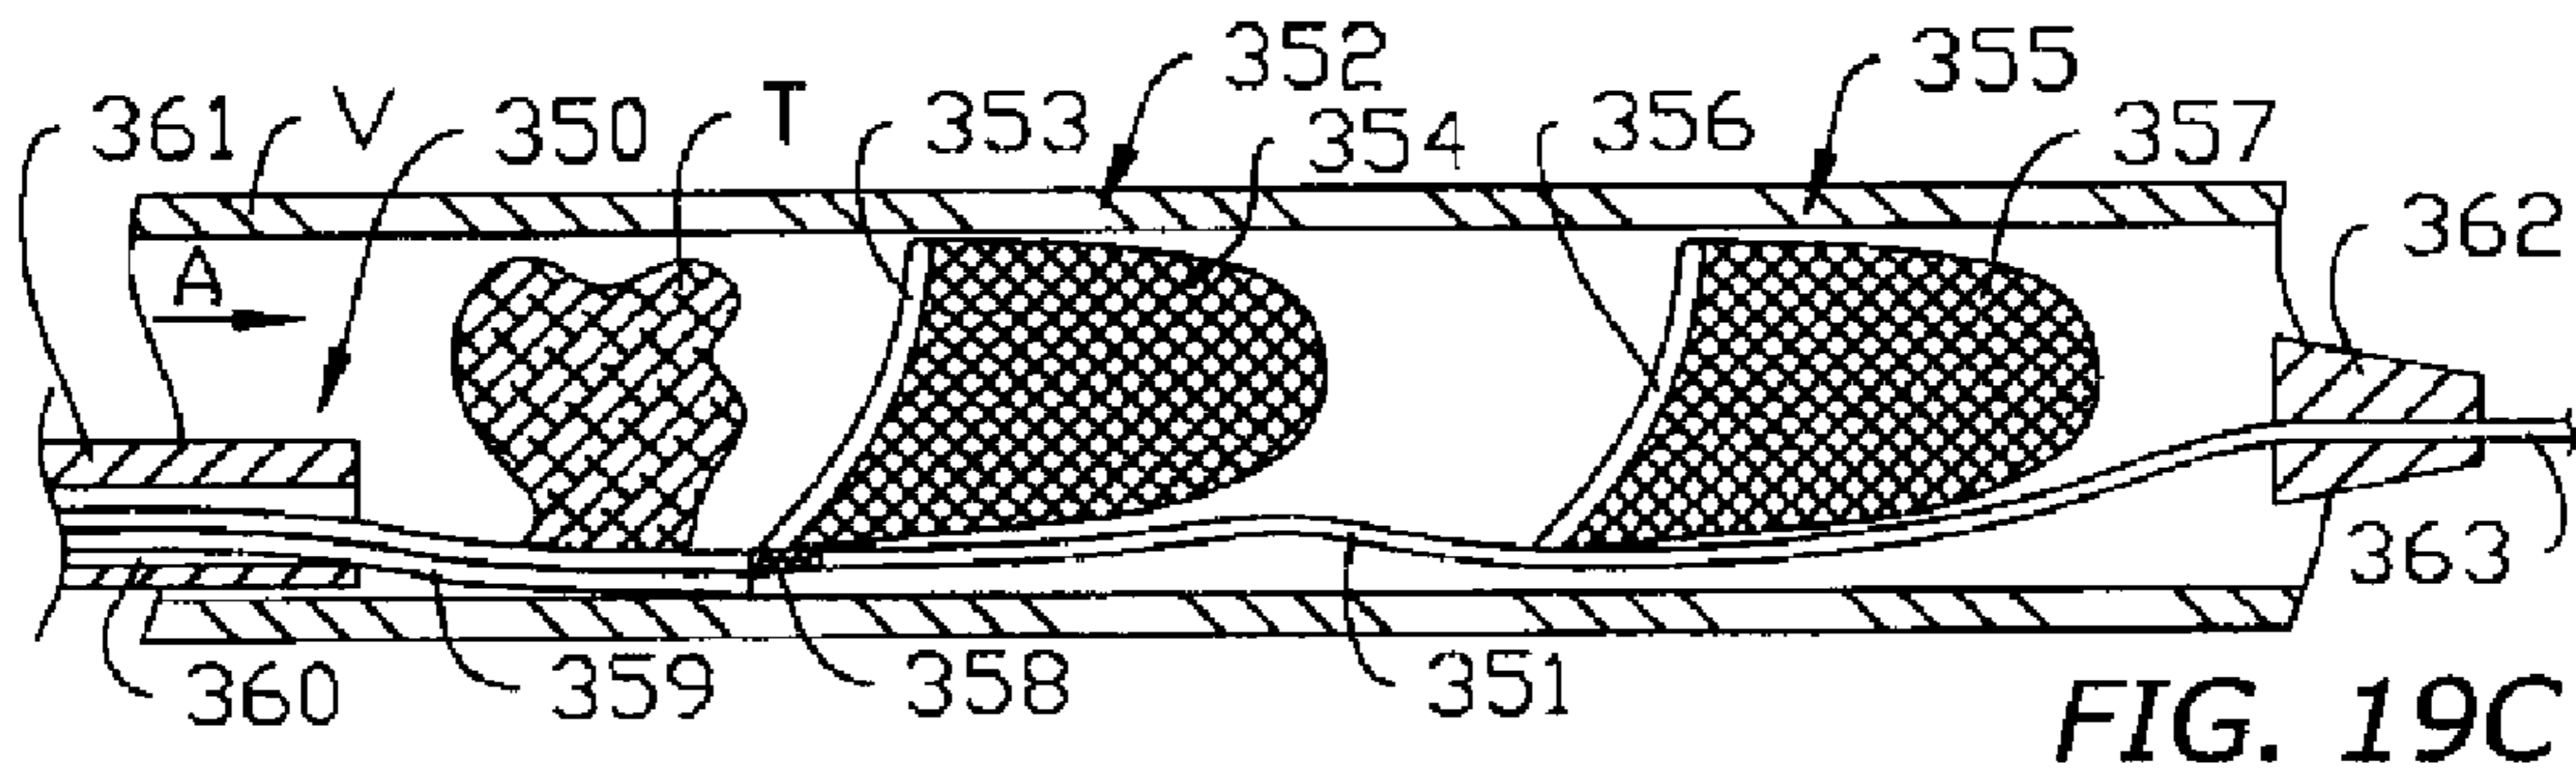
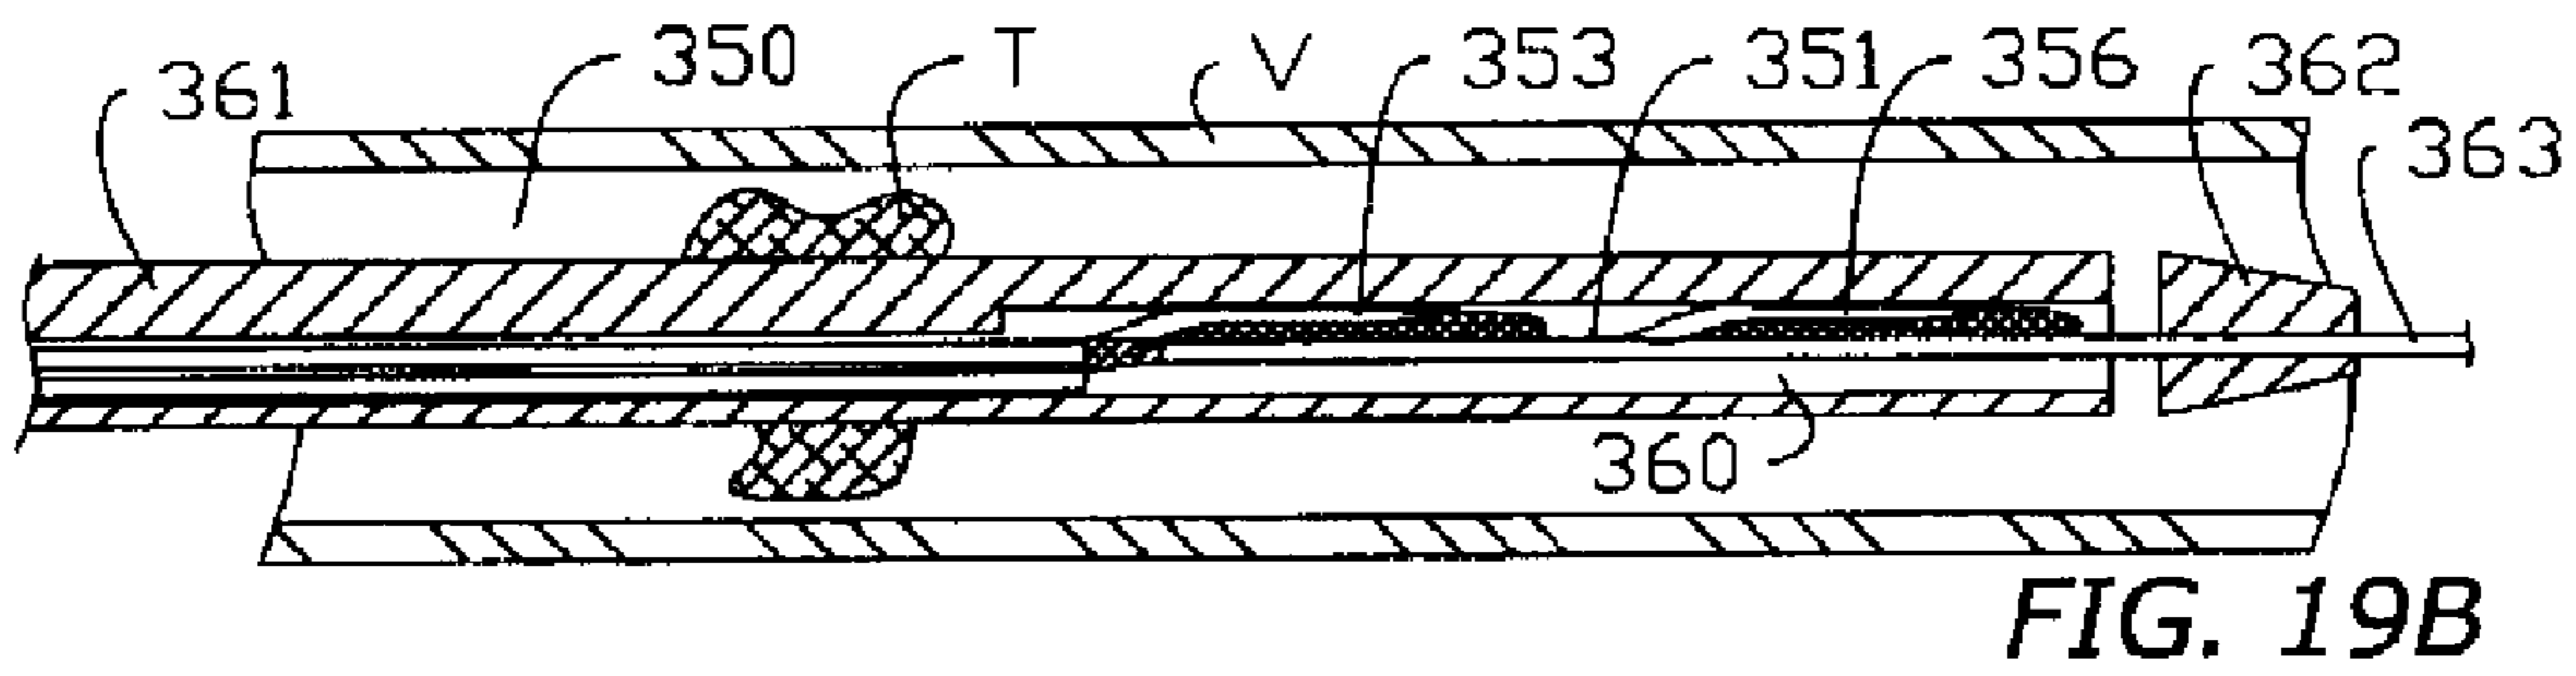
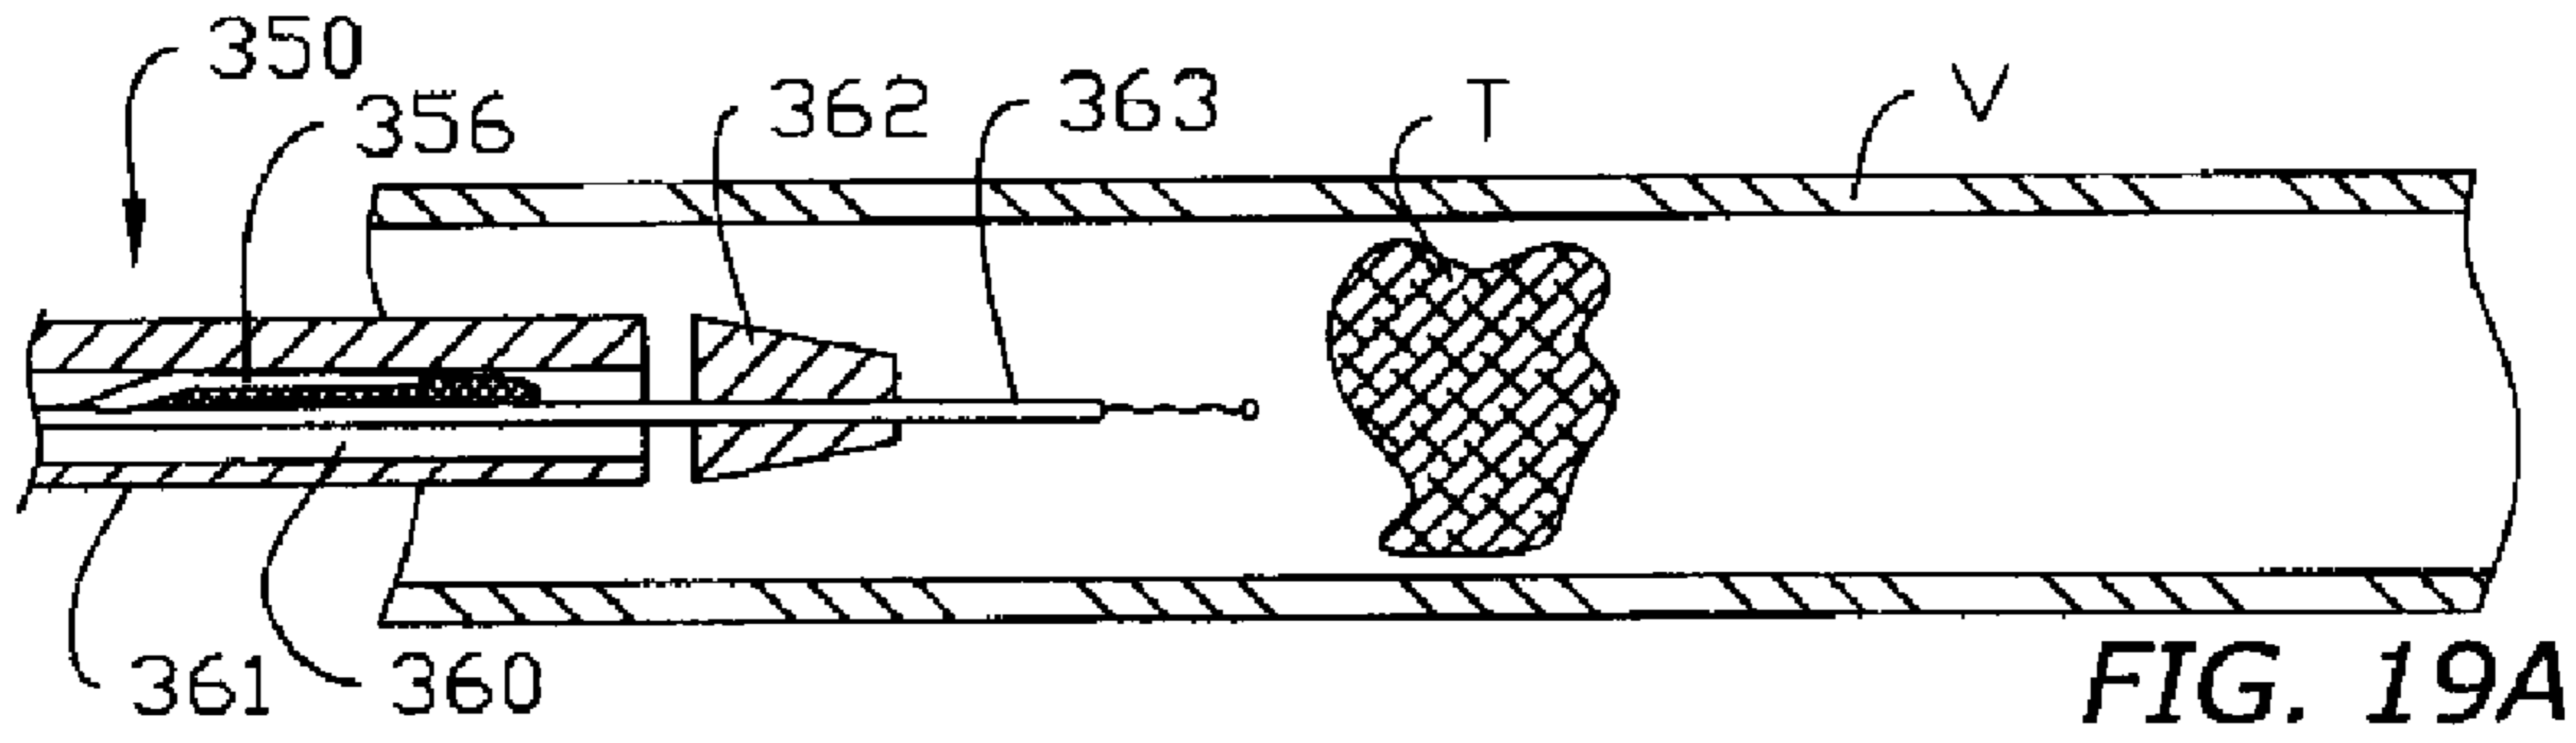


FIG. 13









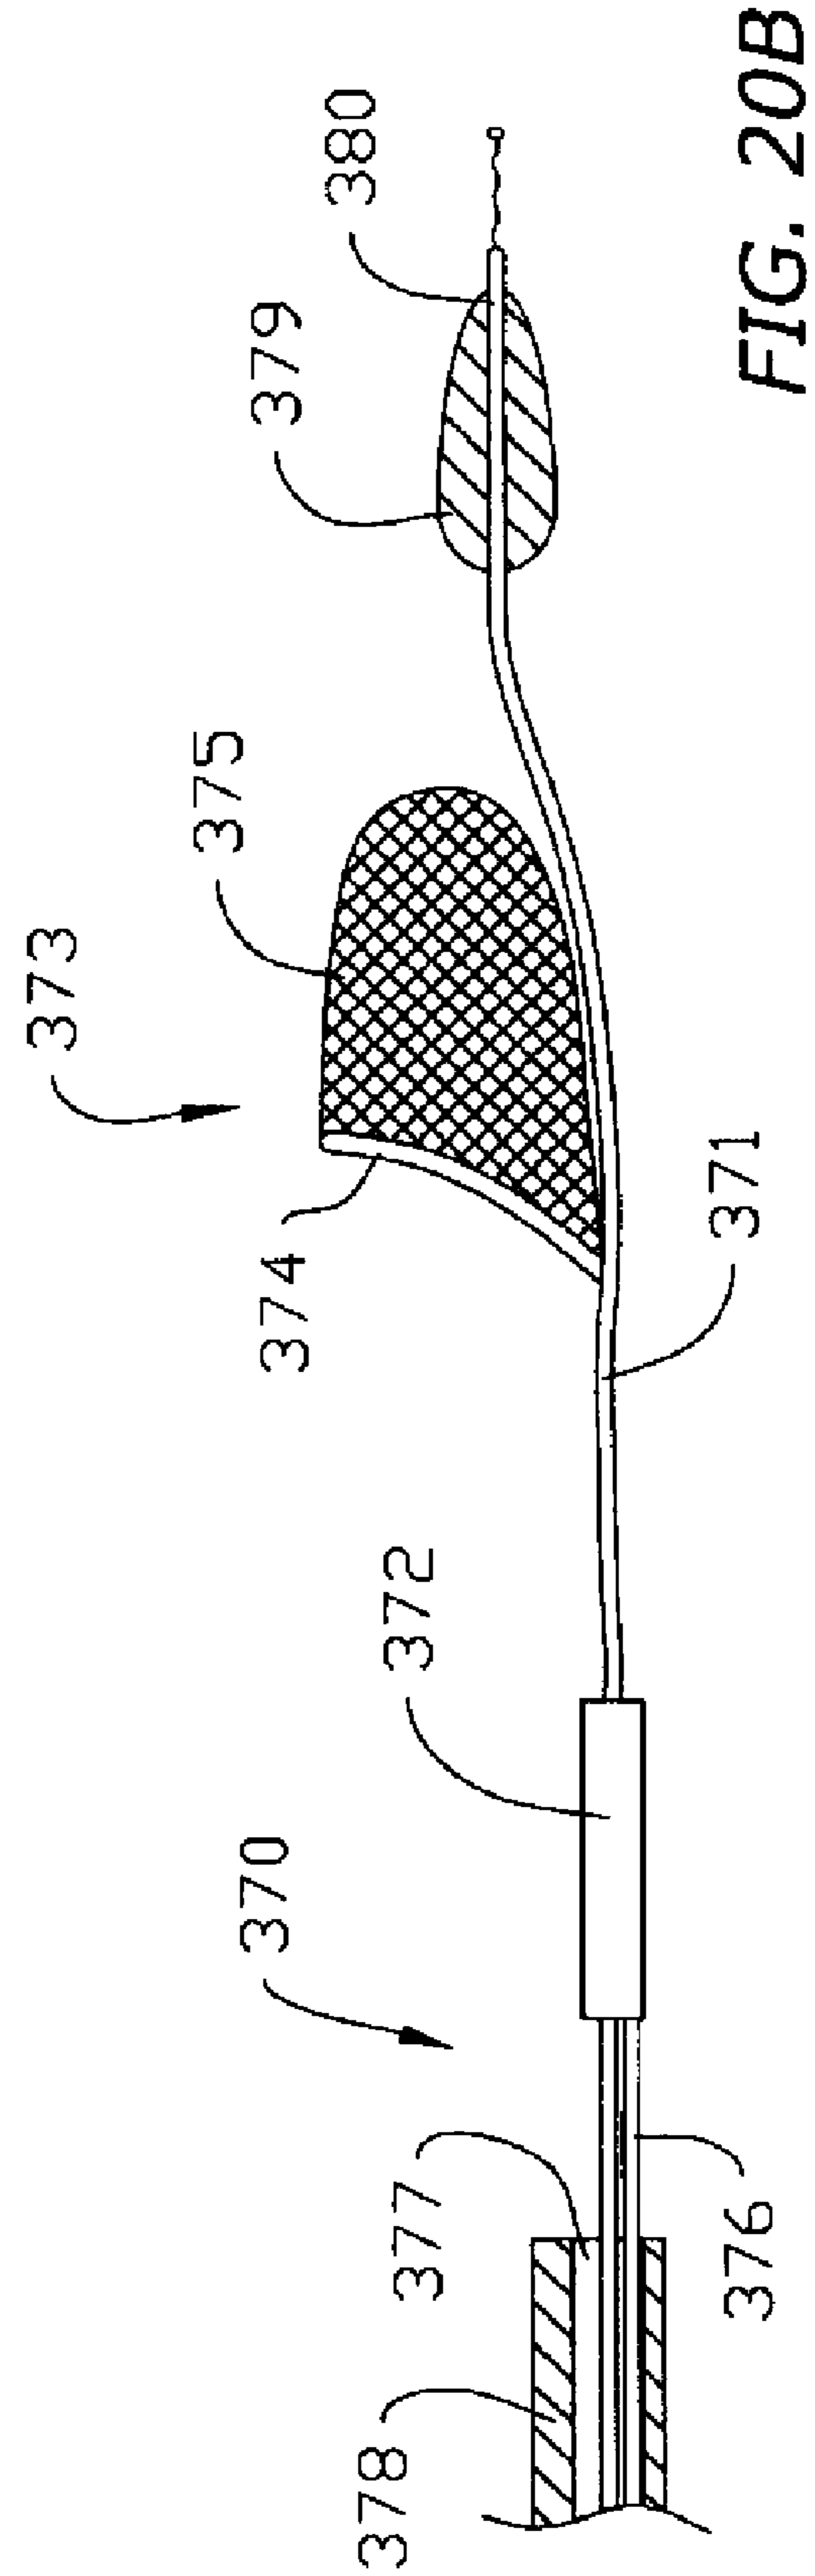
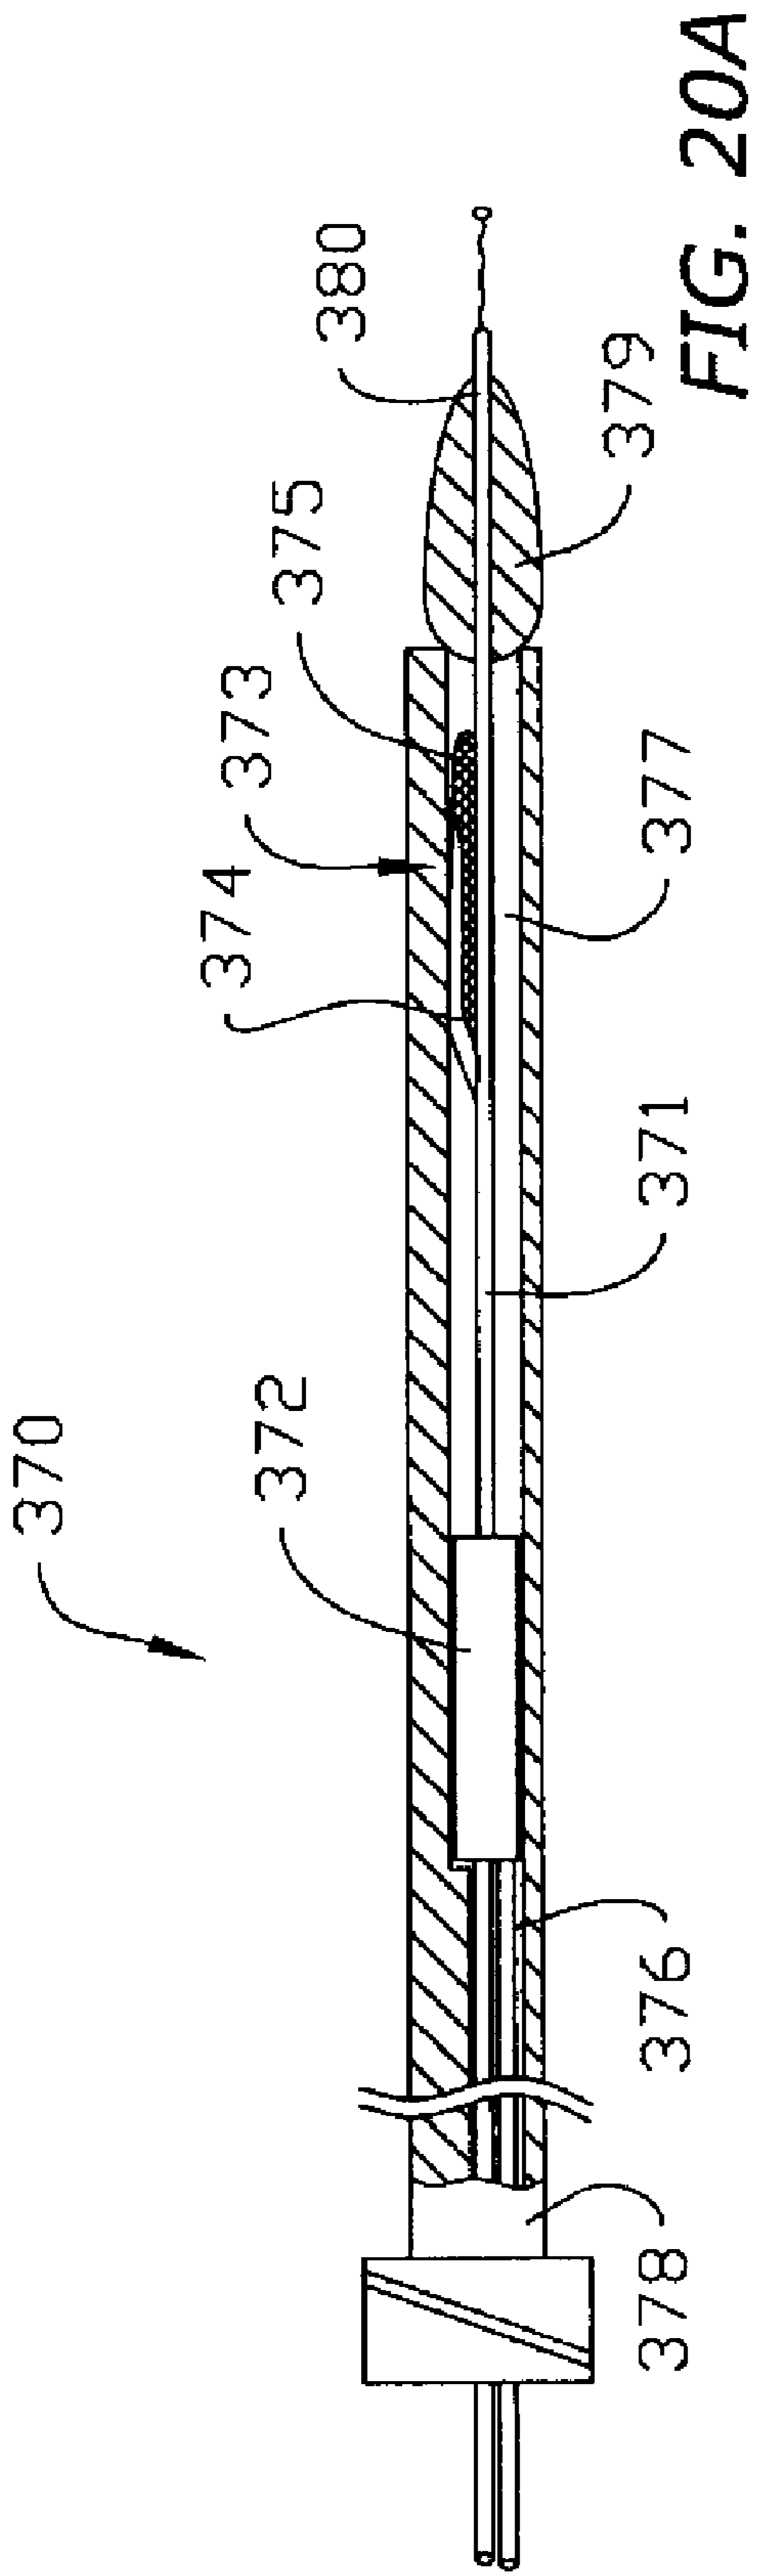


FIG. 20A

FIG. 20B

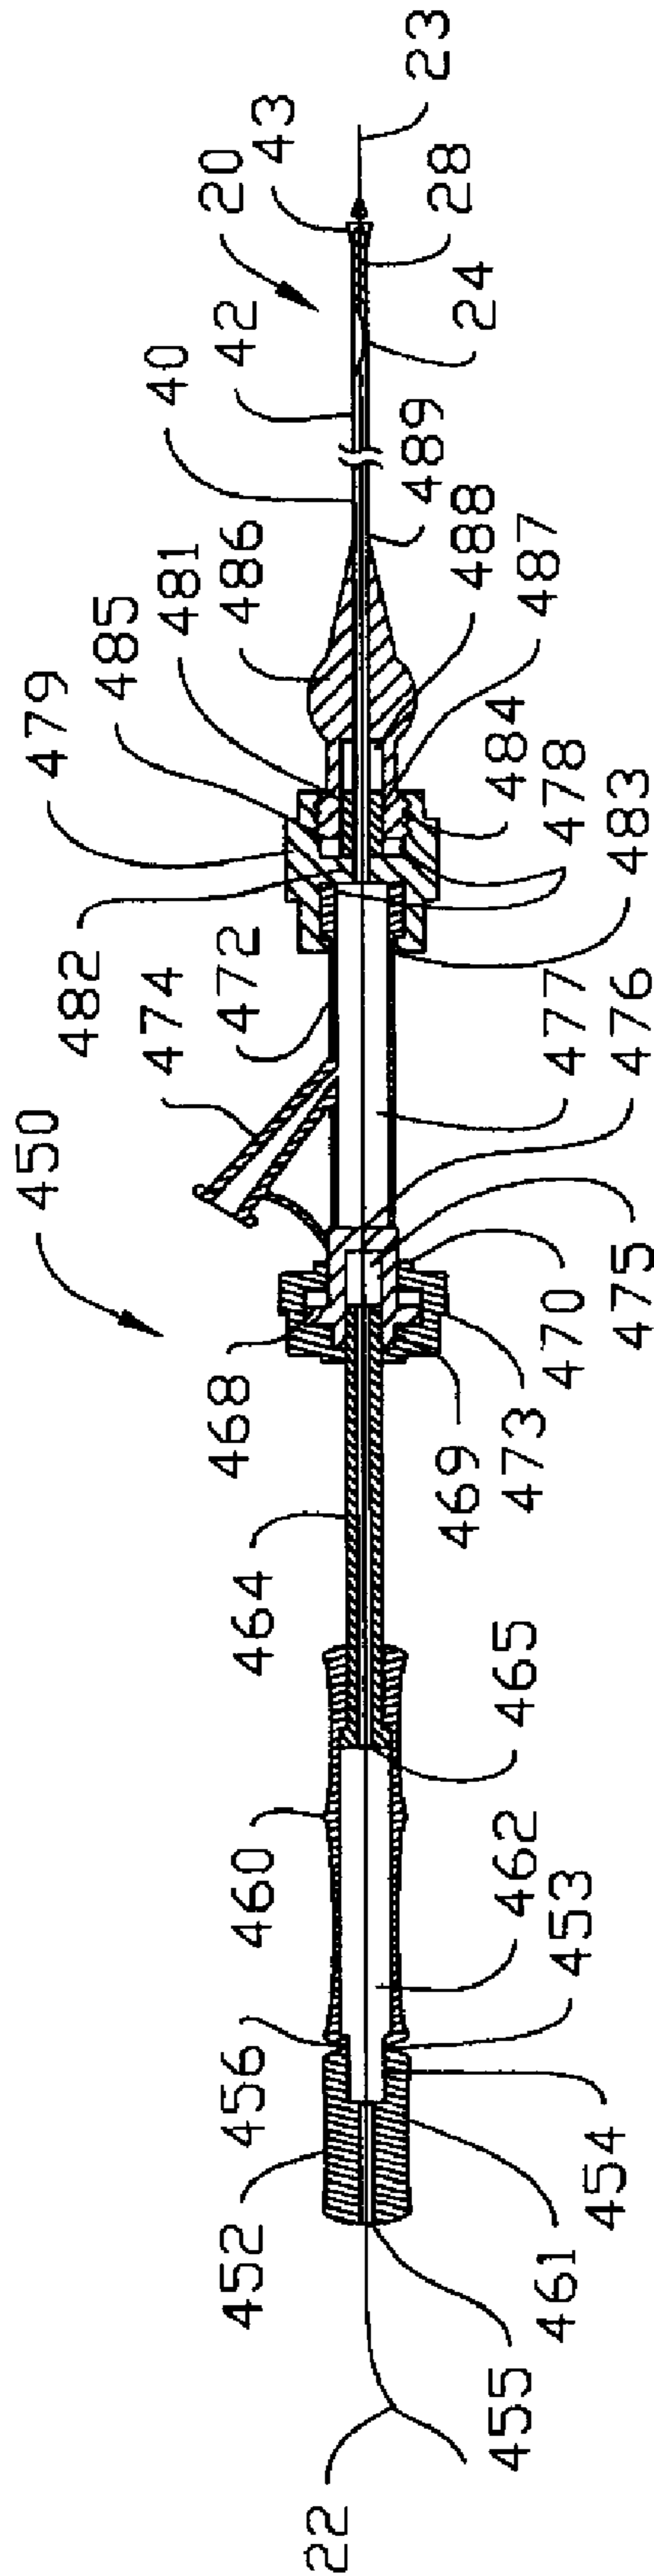


FIG. 21A

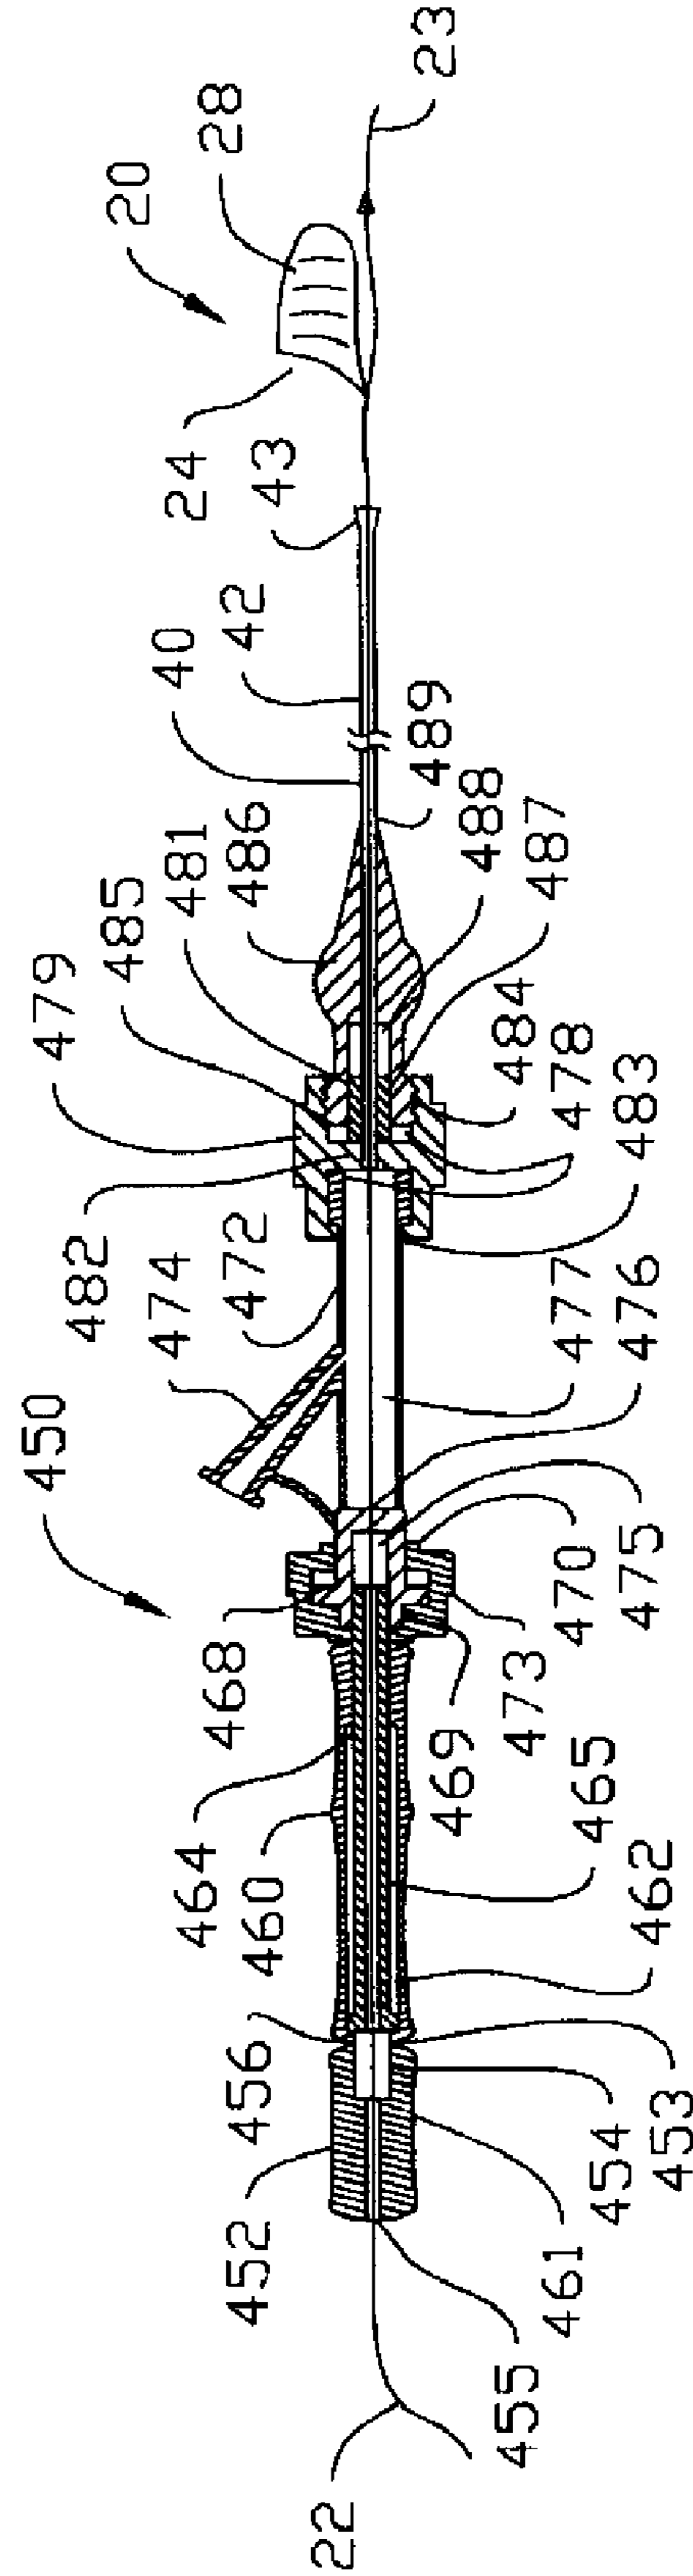
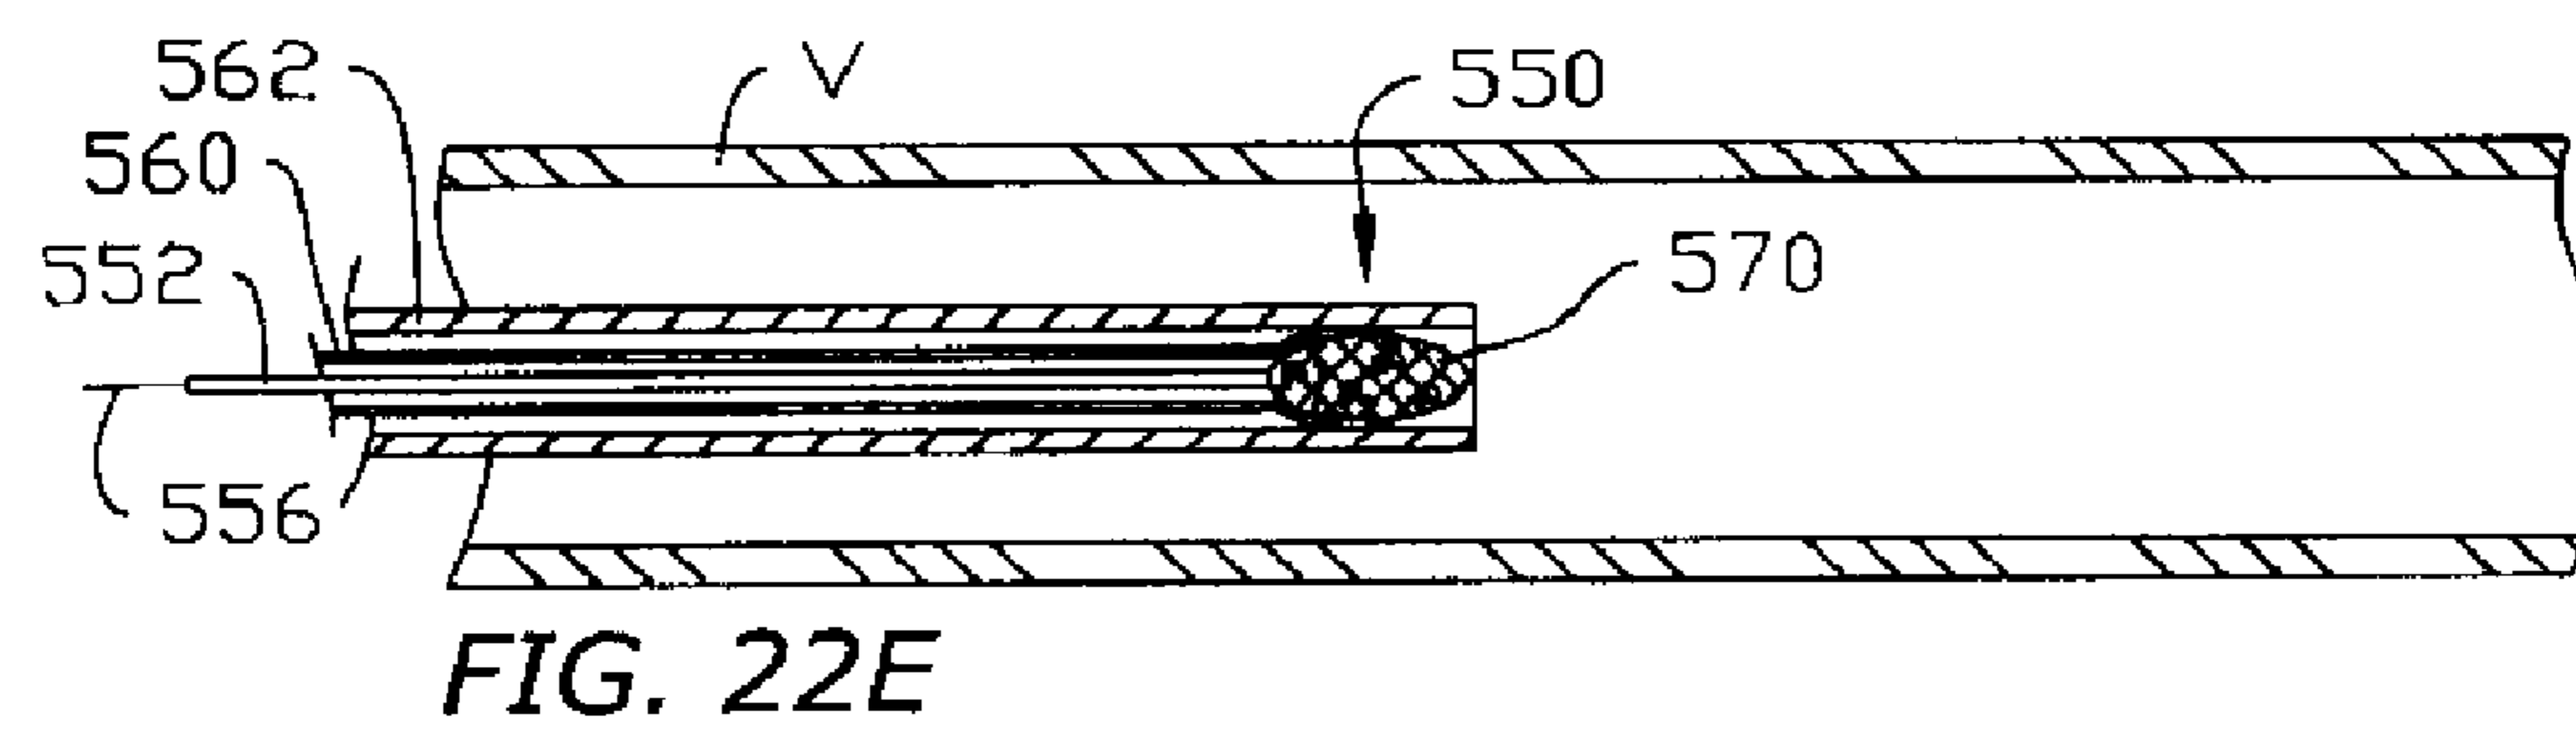
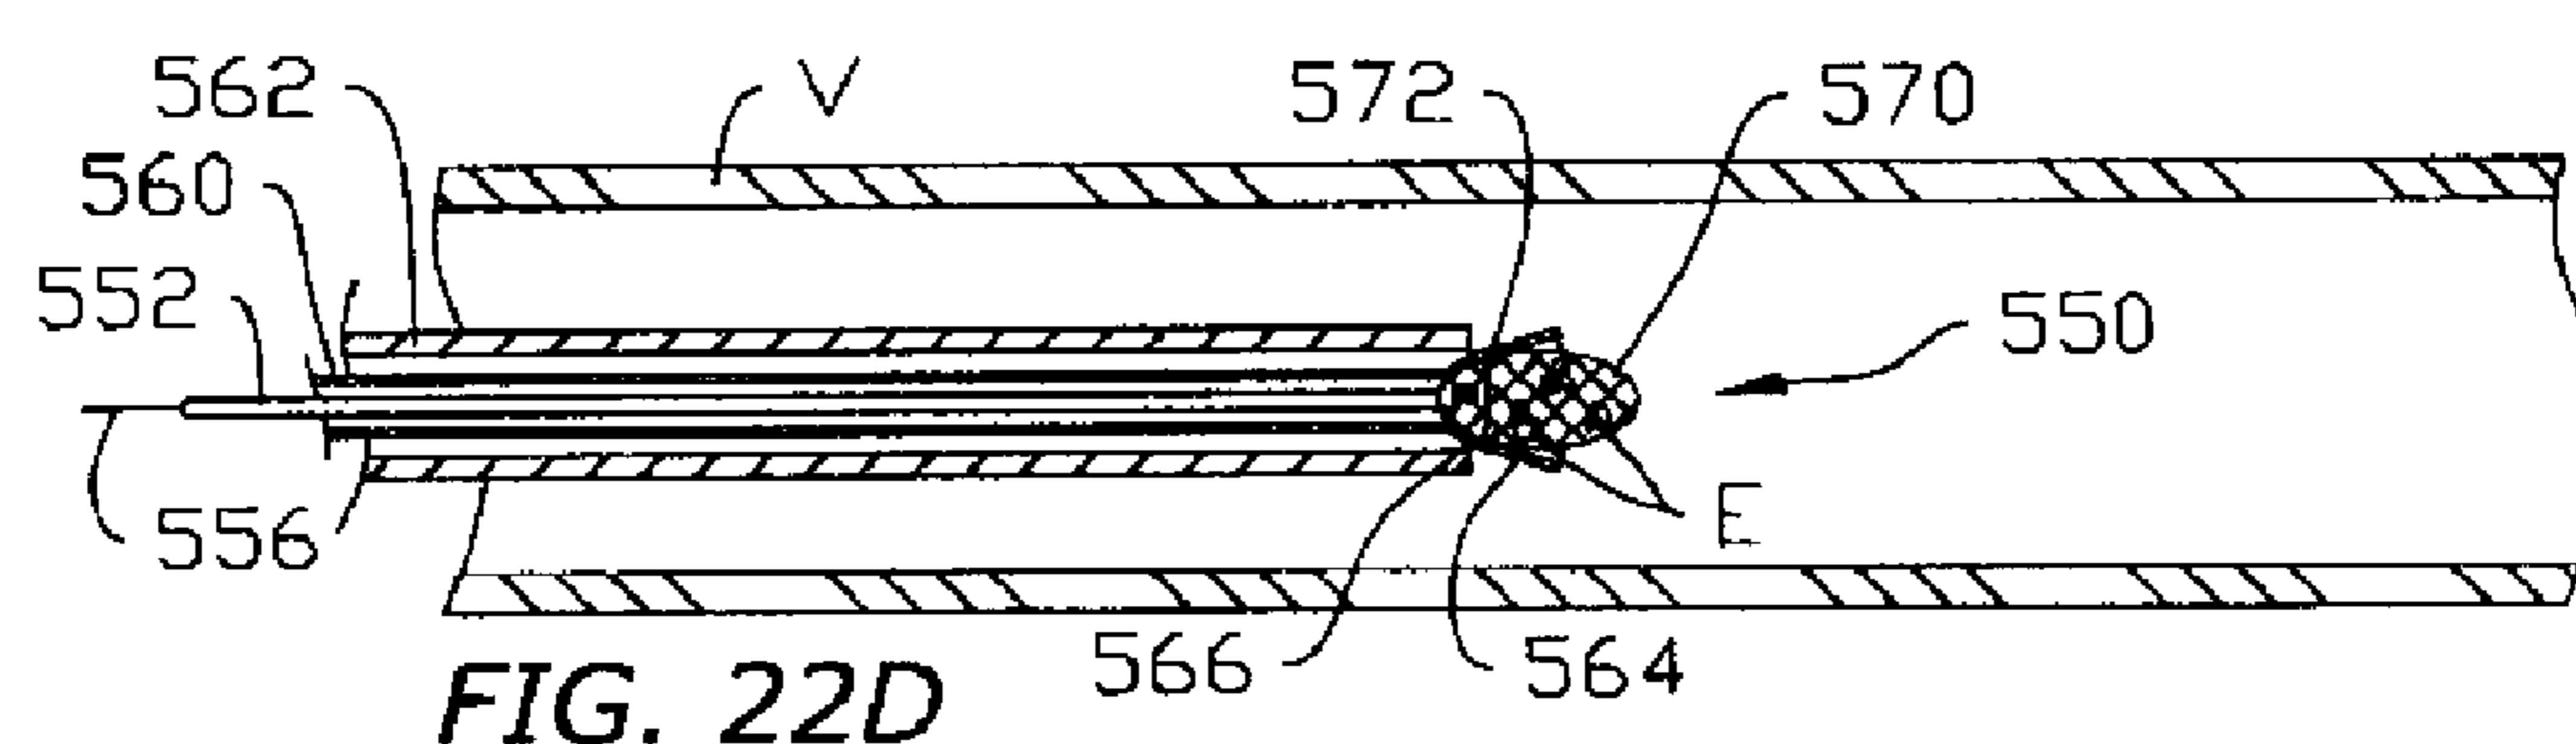
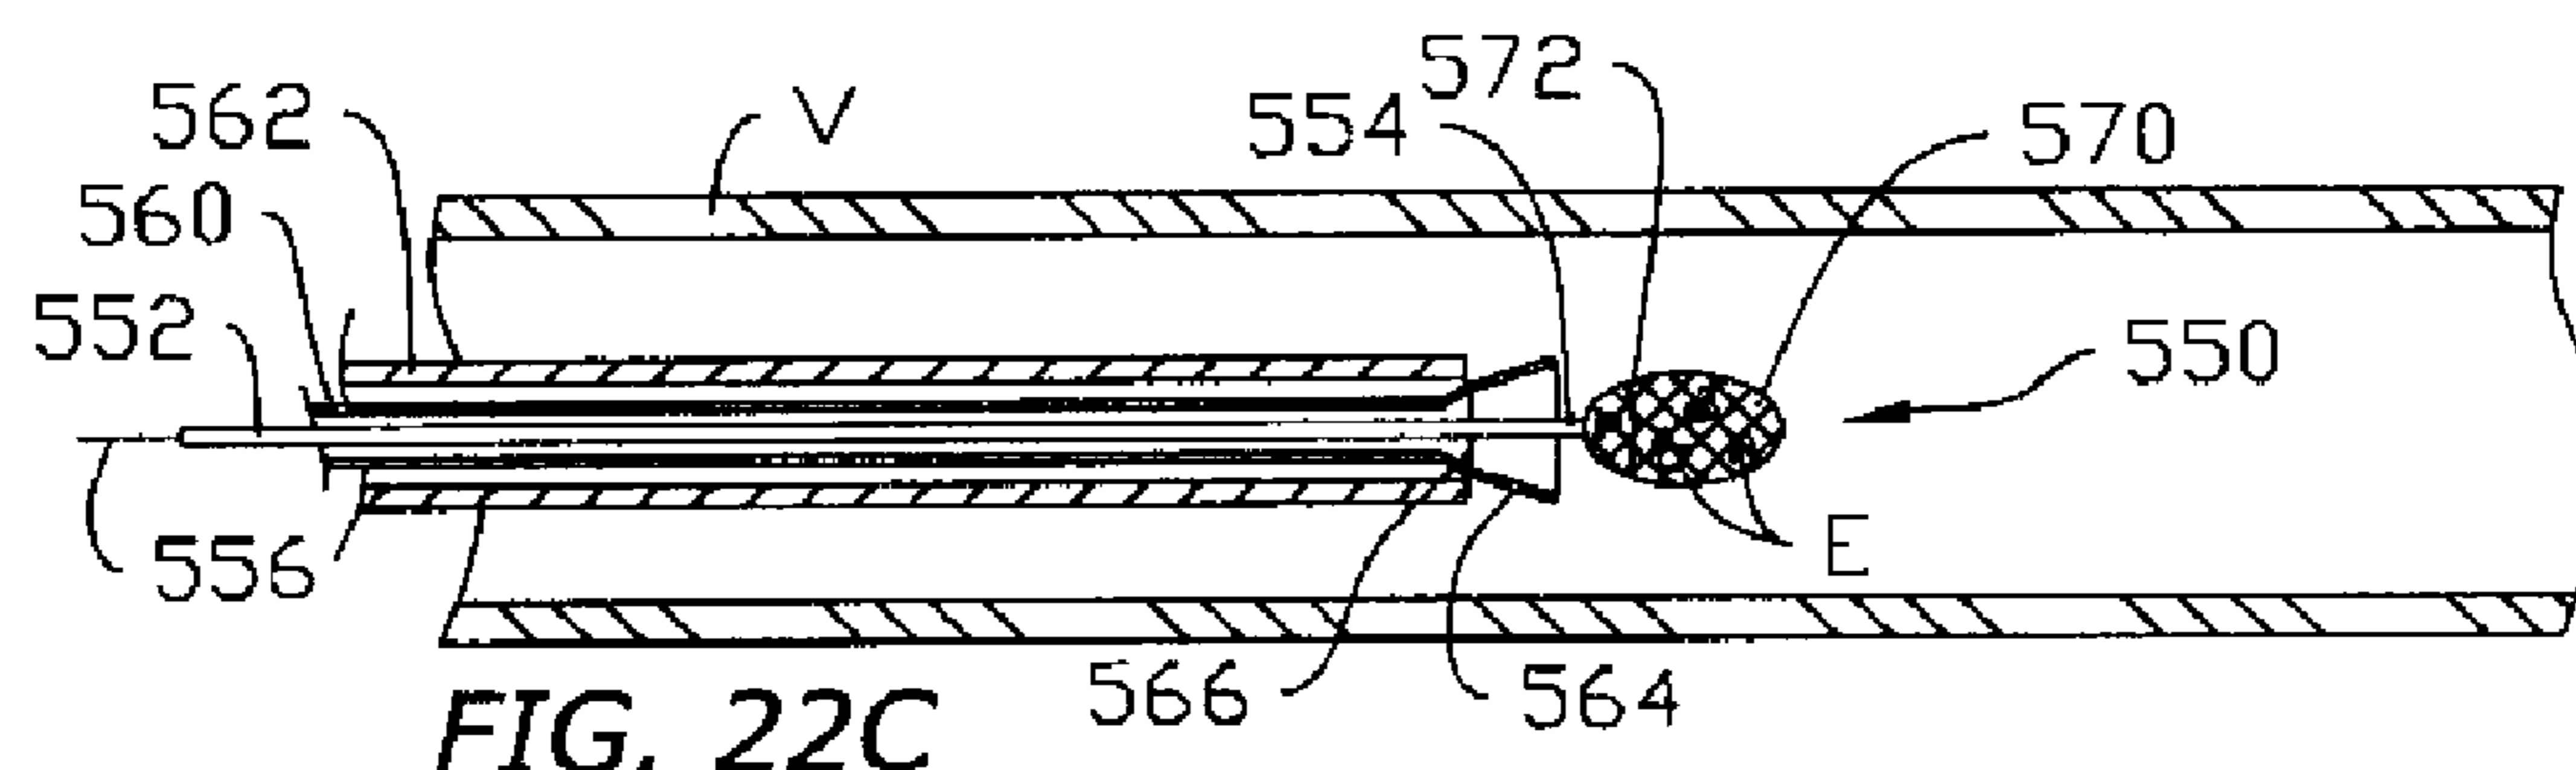
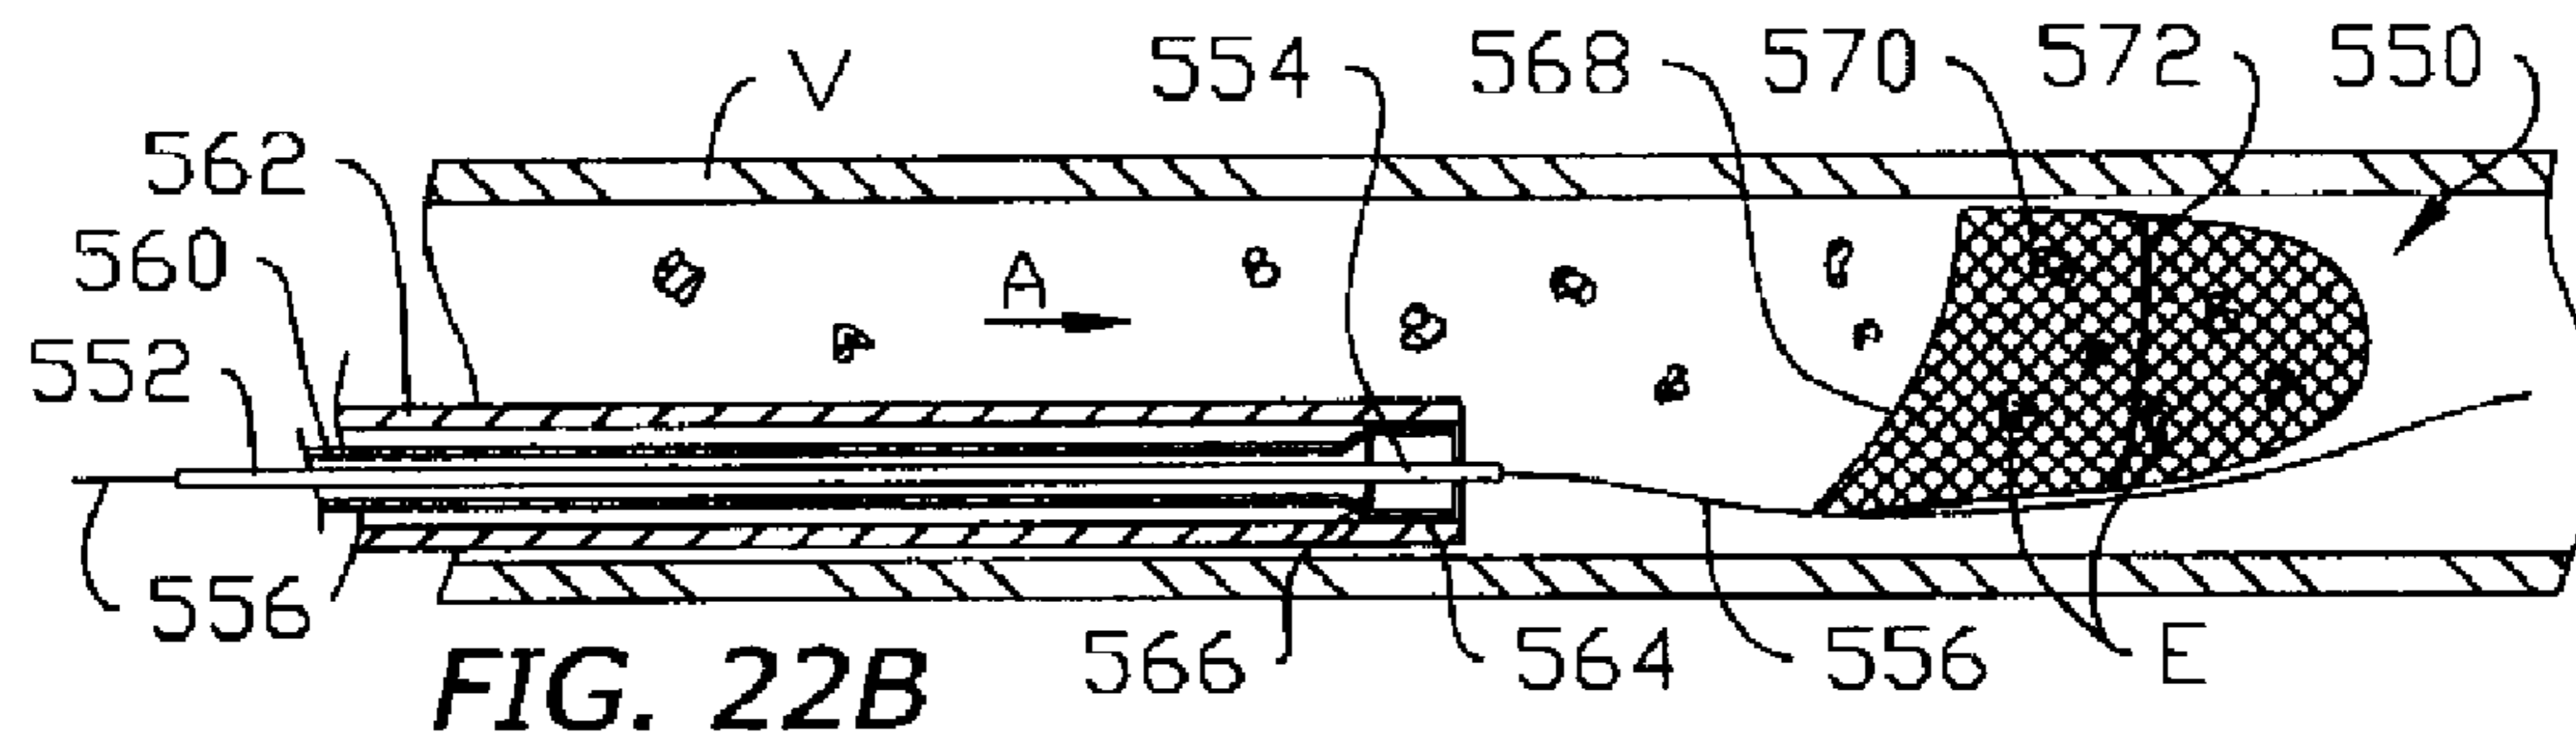
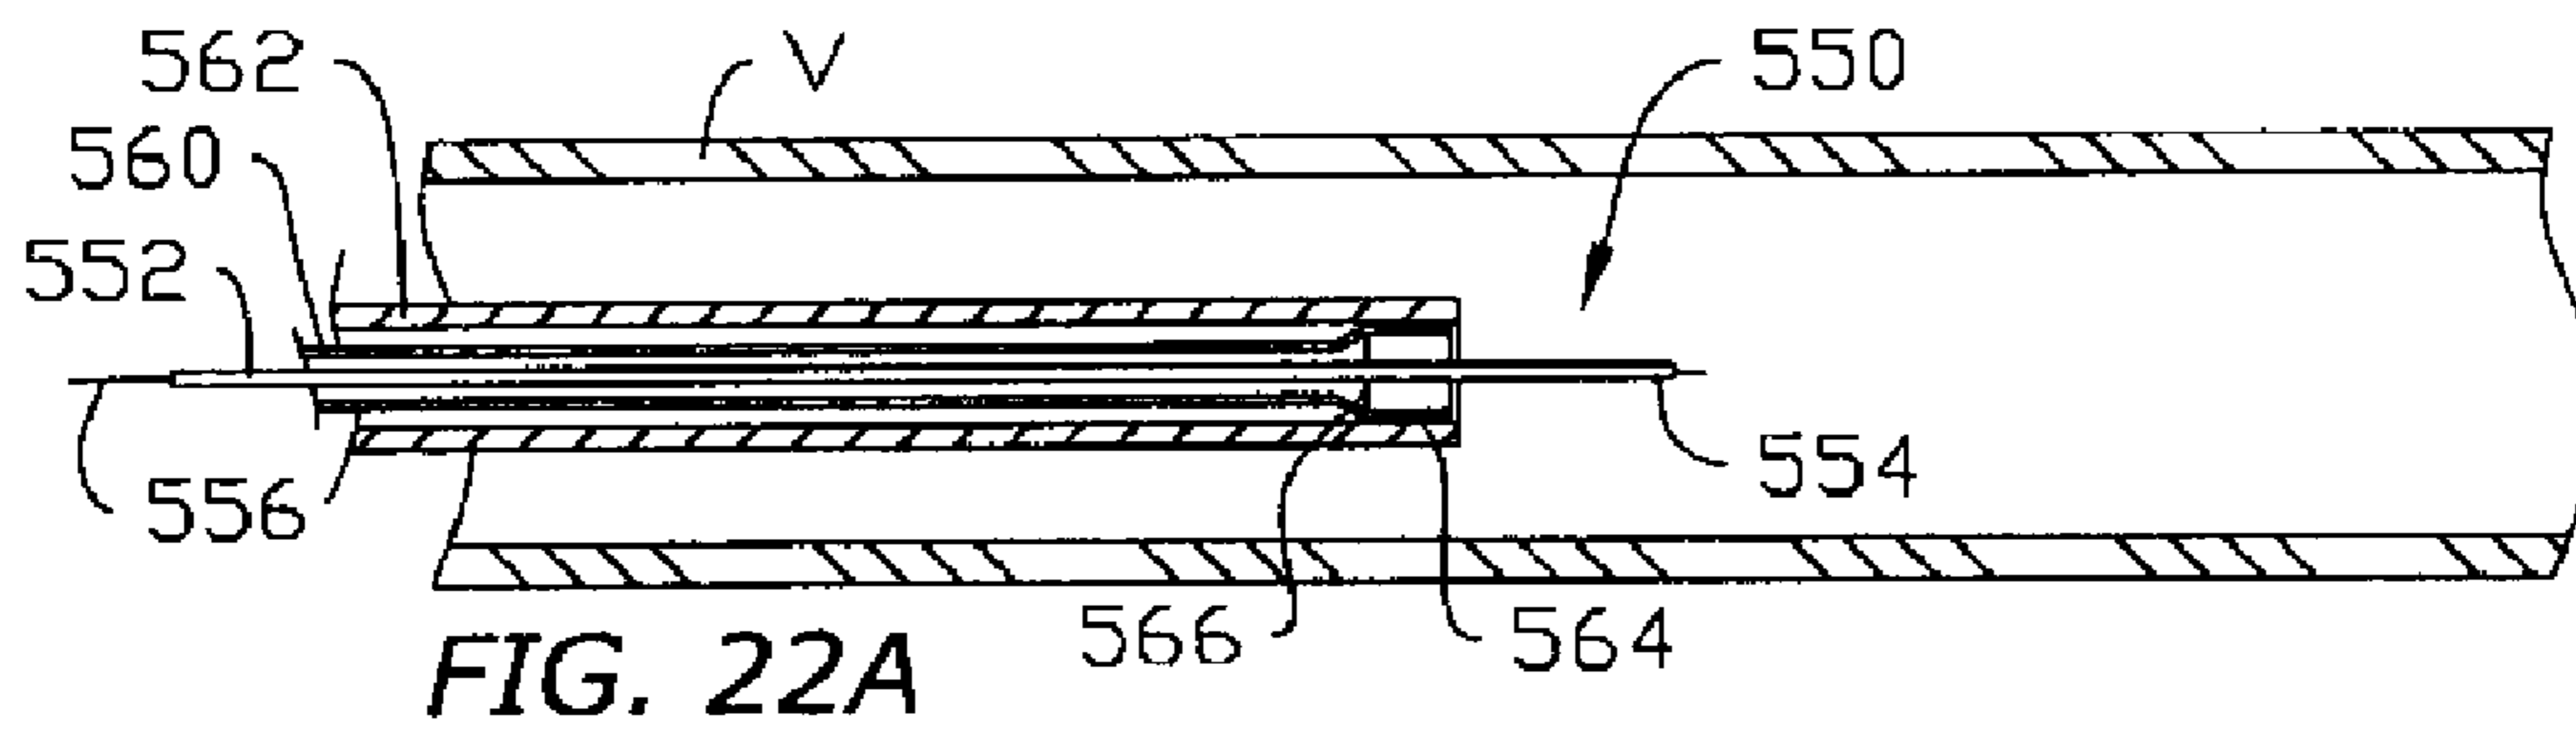


FIG. 21B



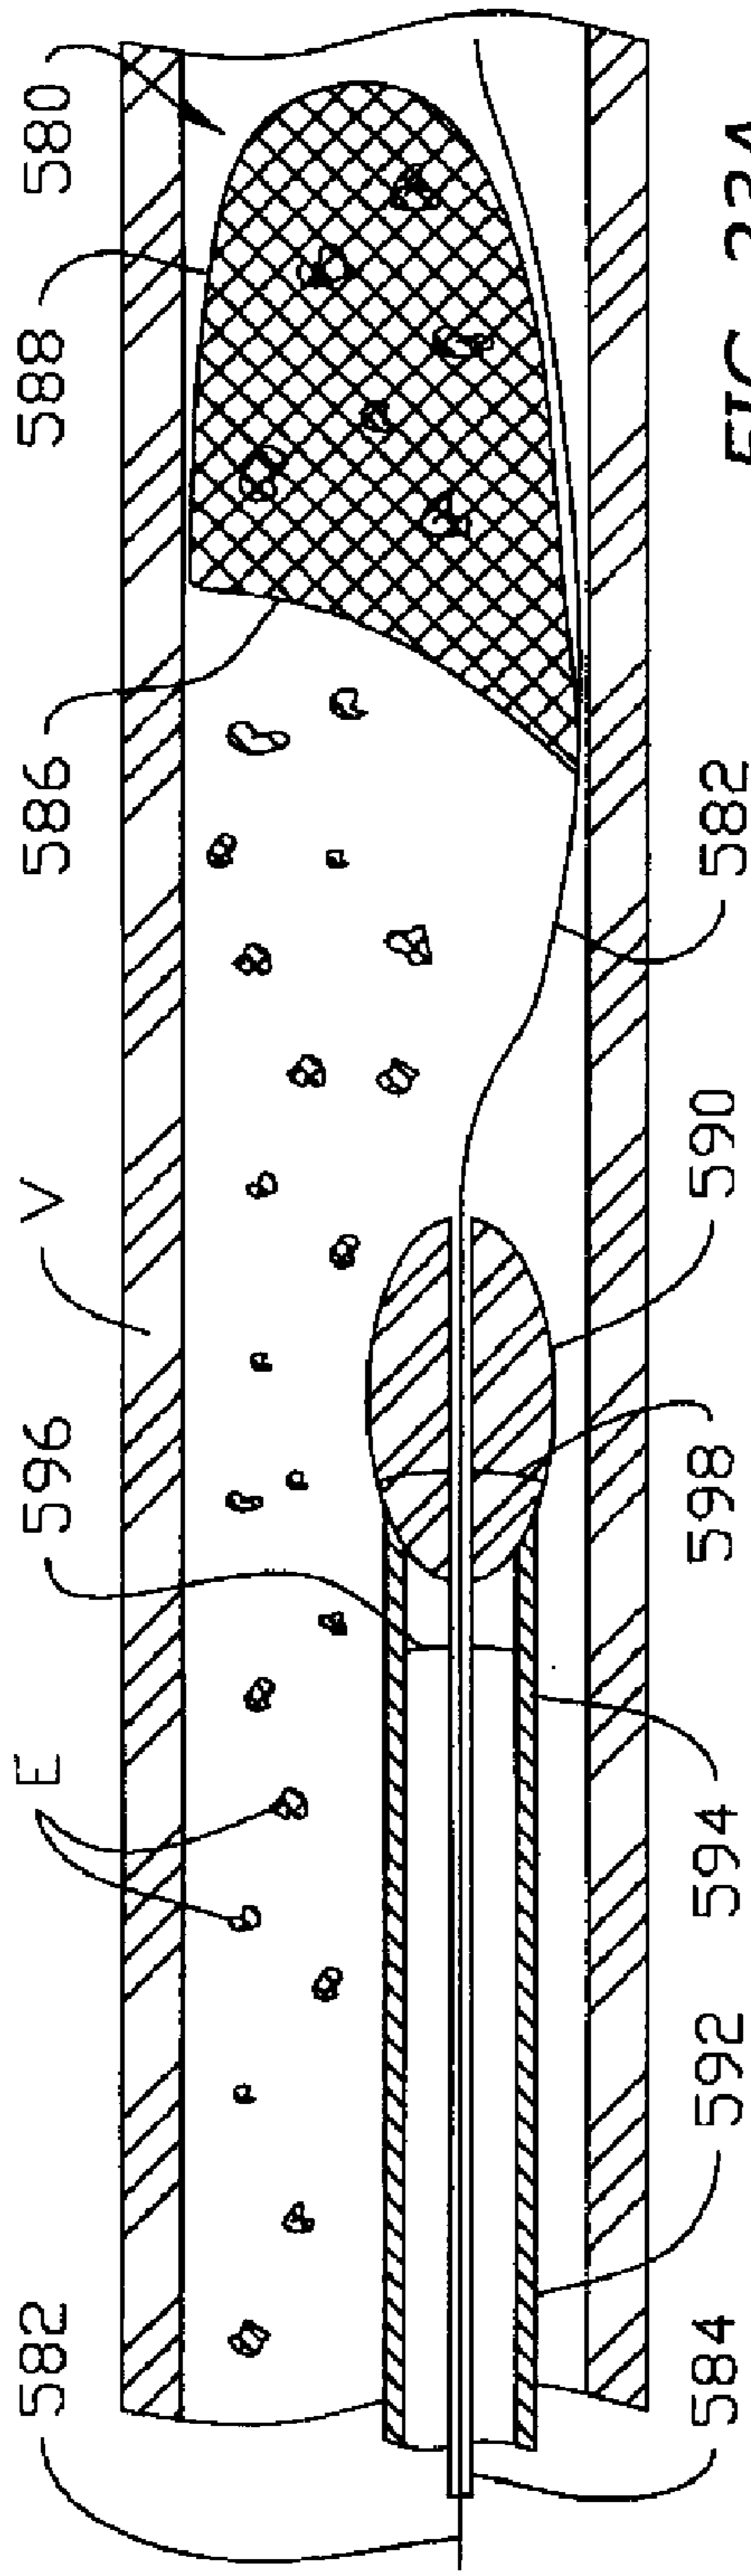


FIG. 23A

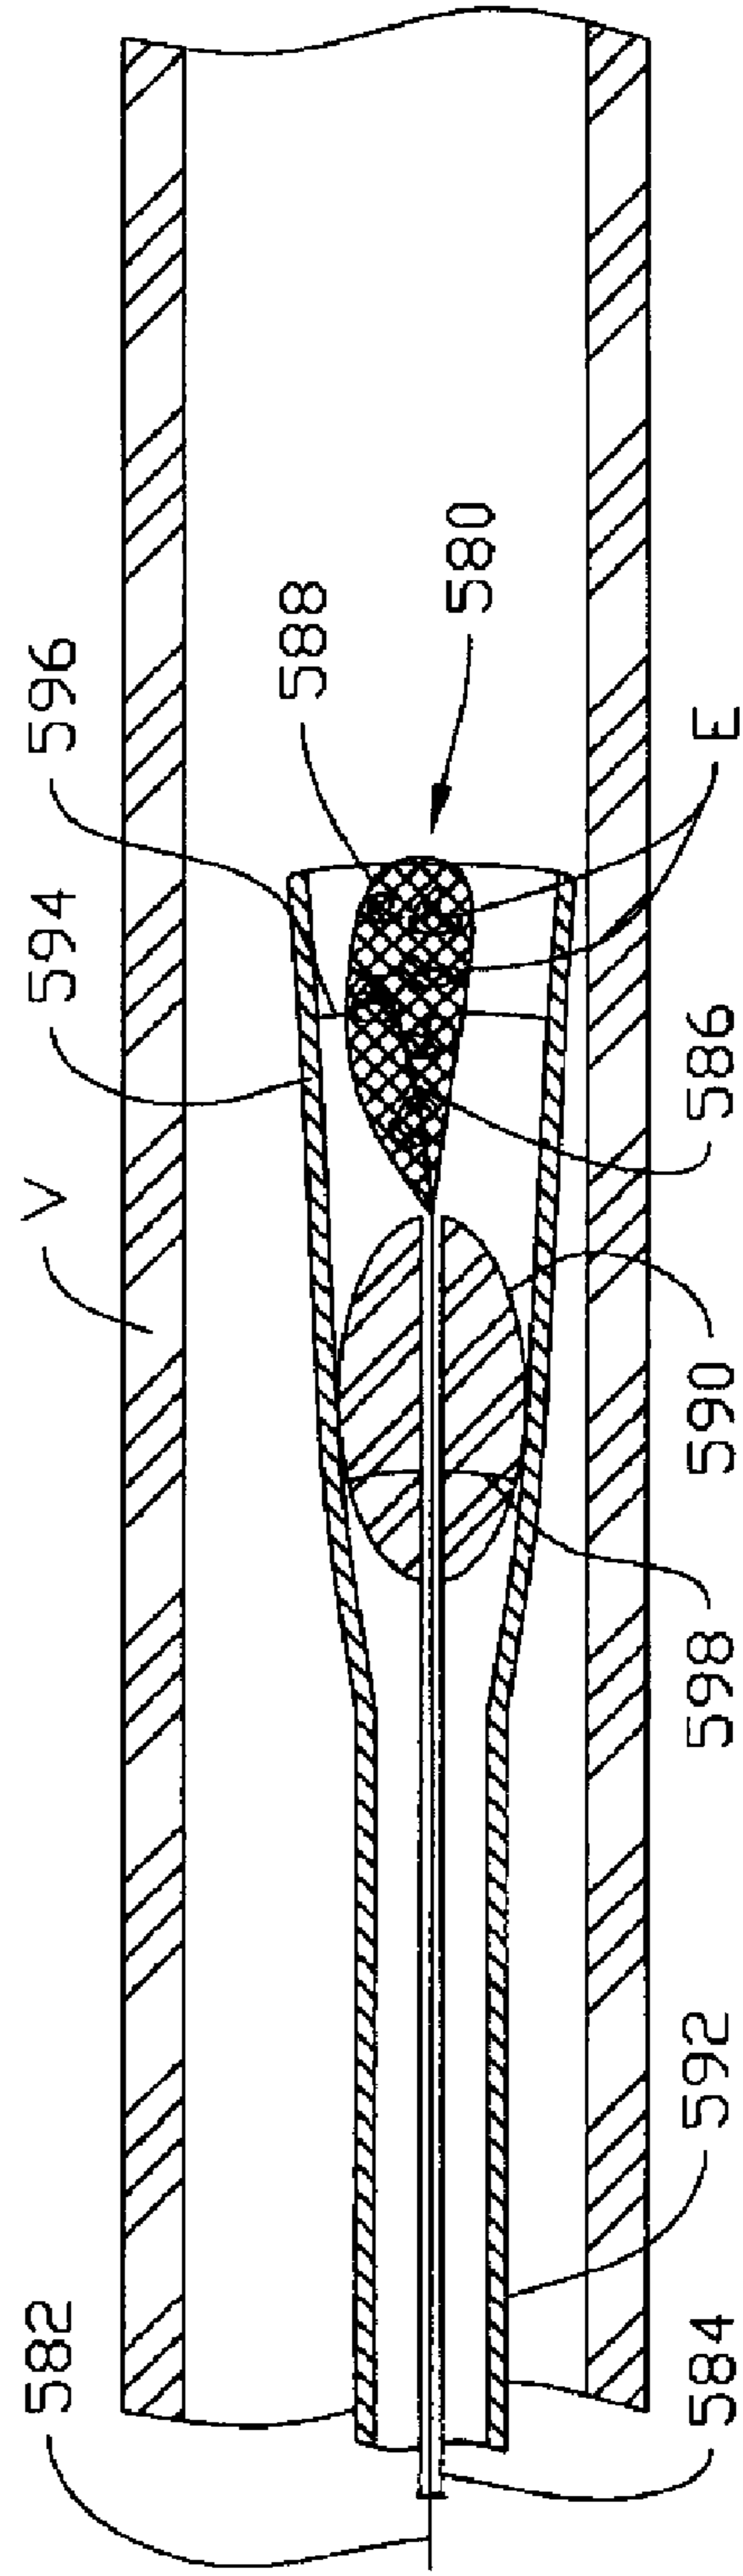


FIG. 23B

**VASCULAR DEVICE FOR EMBOLI,
THROMBUS AND FOREIGN BODY
REMOVAL AND METHODS OF USE**

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue.

REFERENCE TO RELATED APPLICATIONS

This application [claims the benefit of] *is a continuation-in-part of* U.S. patent application Ser. No. 09/364,064, filed Jul. 30, 1999, *now U.S. Pat. No. 6,530,939.*

This application is also a continuation-in-part of U.S. patent application Ser. No. 09/430,211, filed Oct. 29, 1999, *now U.S. Pat. No. 6,589,263.*

This application is also a continuation-in-part of U.S. patent application Ser. No. 09/470,681, filed Dec. 23, 1999, *now U.S. Pat. No. 6,203,561.*

This application is also a continuation-in-part of U.S. [Pat.] patent application Ser. No. 09/470,682, filed Dec. 23, 1999, *now U.S. Pat. No. 6,214,026.*

This application is also a continuation-in-part of U.S. [Pat.] patent application Ser. No. 09/470,703, filed Dec. 23, 1999, *now U.S. Pat. No. 6,179,861.*

This application is also a continuation-in-part of U.S. [Pat.] patent application Ser. No. 09/470,857, filed Dec. 23, 1999, *now U.S. Pat. No. 6,129,739 [and].*

This application is also a continuation-in-part of U.S. [Pat.] patent application Ser. No. 09/611,428, filed Jul. 7, 2000, [all of which] *now U.S. Pat. No. 6,616,678.*

Each of the above-cited documents are incorporated herein by reference.

FIELD OF THE INVENTION

The present invention relates to apparatus and methods for filtering or removing matter from within a vascular system. More particularly, the present invention provides a low profile self-expanding vascular device useful for capturing emboli or foreign bodies generated during interventional procedures, and for thrombectomy and embolectomy.

BACKGROUND OF THE INVENTION

Percutaneous interventional procedures to treat occlusive vascular disease, such as angioplasty, atherectomy and stenting, often dislodge material from the vessel walls. This dislodged material, known as emboli, enters the bloodstream, and may be large enough to occlude smaller downstream vessels, potentially blocking blood flow to tissue. The resulting ischemia poses a serious threat to the health or life of a patient if the blockage occurs in critical tissue, such as the heart, lungs, or brain.

The deployment of stents and stent-grafts to treat vascular disease, such as aneurysms, also involves the introduction of foreign objects into the bloodstream, and also may result in the formation of clots or release of emboli. Such particulate matter, if released into the bloodstream, also may cause infarction or stroke.

Furthermore, interventional procedures may generate foreign bodies that are left within a patient's bloodstream, thereby endangering the life of the patient. Foreign bodies may include, for example, a broken guide wire, pieces of a stent, or pieces of a catheter.

Numerous previously known methods and apparatus have been proposed to reduce complications associated with embolism, release of thrombus, or foreign body material generation. U.S. Pat. No. 5,833,644 to Zadno-Azizi et al., for example, describes the use of a balloon-tipped catheter to temporarily occlude flow through a vessel from which a stenosis is to be removed. Stenotic material removed during a treatment procedure is evacuated from the vessel before the flow of blood is restored. A drawback of such previously known systems, however, is that occlusion of antegrade flow through the vessel may result in damage to the tissue normally fed by the blocked vessel.

U.S. Pat. No. 5,814,064 to Daniel et al. describes an emboli filter system having a radially expandable mesh filter disposed on the distal end of a guide wire. The filter is deployed distal to a region of stenosis, and any interventional devices, such as angioplasty balloons or stent delivery systems, are advanced along the guide wire. The filter is designed to capture emboli generated during treatment of the stenosis while permitting blood to flow through the filter. Similar filter systems are described in U.S. Pat. No. 4,723,549 to Wholey et al. and U.S. Pat. No. 5,827,324 to Cassell et al.

One disadvantage of radially expandable filter systems such as described in the foregoing patents is the relative complexity of the devices, which typically comprise numerous parts. Connecting more than a minimal number of such parts to a guide wire generally increases delivery complications. The ability of the guide wire to negotiate tortuous anatomy is reduced, and the profile of the device in its delivery configuration increases. Consequently, it may be difficult or impossible to use such devices in small diameter vessels, such as are commonly found in the carotid artery and cerebral vasculature. Moreover, such filter devices are generally incapable of preventing material from escaping from the filter during the process of collapsing the filter for removal.

International Publication No. WO 98/39053 describes a filter system comprising an elongated member, a radially expandable hoop and a cone-shaped basket. The hoop is affixed to the elongated member, and the cone-shaped basket is attached to the hoop and the elongated member, so that the hoop forms the mouth of the basket. The filter system includes a specially configured delivery catheter that retains the mouth of the basket in a radially retracted position during delivery.

While the filter system described in the foregoing International Publication reduces the number of components used to deploy the cone-shaped basket, as compared to the radial strut-type filter elements described hereinabove, it too has drawbacks. Chief among these, it is expected that it will be difficult to reduce the diameter of the radially expandable hoop to its retracted position. In particular, as the hoop is contracted through smaller radii of curvature, the stiffness of the hoop is expected to increase dramatically. This increased stiffness prevents the hoop from being contracted more tightly, and is expected to result in a delivery profile too large to permit use of the device in critical regions of the body, such as the smaller coronary arteries, carotid arteries, and cerebral vasculature.

In view of the foregoing disadvantages of previously known apparatus and methods, it would be desirable to provide a vascular device, e.g., for use as a vascular filter, that overcomes such disadvantages and employs few components.

It would be desirable to provide a reliable and multi-functional delivery system for use with the vascular device.

It would be desirable to provide an integrated vascular device with a thrombectomy element and a vascular filter.

It also would be desirable to provide a vascular device that is capable of being contracted to a small delivery profile, thus permitting use of the device in small vessels.

It further would be desirable to provide a vascular device that is capable of being contracted to a sufficiently small profile that it may be retrieved using the guide wire lumen of previously known treatment devices, and without the need for specialized delivery catheters.

It still further would be desirable to provide a vascular device that reduces the risk of emboli or thrombus removed from the vessel wall escaping from the device when the device is collapsed and removed.

It also would be desirable to provide a vascular device that permits a rapid exchange deployment modality.

SUMMARY OF THE INVENTION

In view of the foregoing, it is an object of the present invention to provide a vascular device that overcomes disadvantages of previously known vascular filters, thrombectomy/embolectomy and foreign body removal devices, and employs few components.

It is an object of the present invention to provide a reliable and multi-functional delivery system for use with the vascular device.

It is an object to provide an integrated vascular device with a thrombectomy element and a vascular filter.

It also is an object of this invention to provide a vascular device that is capable of being contracted to a small delivery profile, thus permitting use of the device in small vessels.

It is a further object to provide a vascular device that is capable of being contracted to a sufficiently small profile that it may be retrieved using the guide wire lumen of previously known treatment devices, and without the need for specialized delivery catheters.

It is another object to provide a vascular device that reduces the risk of emboli or thrombus removed from the vessel wall escaping from the device when the device is collapsed and removed.

It also is an object to provide a vascular device that permits a rapid exchange deployment modality.

These and other objects of the present invention are accomplished by providing a vascular device, suitable for use as a vascular filter or thrombectomy/embolectomy device that comprises a blood permeable sac affixed at its perimeter to a support hoop having an articulation region. The support hoop is attached to a distal region of an elongated member, such as a guide wire, and supports a proximally-oriented mouth of the sac when the device is deployed in a vessel. The device may also comprise a nose cone to facilitate percutaneous introduction, and a delivery sheath having one or more lumens. The lumens may further be configured for a rapid exchange mode of introduction along the guide wire.

In a first embodiment, the support hoop includes one or more reduced-thickness articulation regions that enable the support hoop to be contracted to very small radii of curvature without the problems of increased stiffness and kinking of previously known devices. In an alternative embodiment, the articulation region may comprise a gap in the support hoop bridged by the perimeter of the blood permeable sac.

The support hoop preferably also has a curved profile that prevents the articulation region, when folded, from damaging the wall of the vessel. The curved profile permits the device to effectively contact the walls of the vessel and reduce emboli or thrombus removed from the vessel wall from bypassing the sac. Moreover, the articulation region, when combined with a support hoop having a curved profile, causes the sides of the

support hoop to fold inwards towards one-another when the vascular device is collapsed into a sheath for removal. This, in turn, closes the mouth of the sac and reduces the potential for emboli or thrombus to be released from the vascular device during removal.

Advantageously, use of an articulation region permits vascular devices of the present invention to be contracted to very small diameters, thereby enabling the use of delivery catheters having diameters as small as 3 Fr. Moreover, the vascular devices may be retracted within the guide wire lumens of conventional treatment devices, such as angioplasty catheters and stent delivery systems, thereby obviating the need to re-insert a specialized delivery catheter to remove the vascular device. However, a retrieval sheath having a distal region that flares or expands outwardly to receive the emboli-filled sac upon completion of an interventional procedure, and which reduces risk of rupture to the sac, optionally may be provided in accordance with the present invention.

In embodiments suitable for use as embolic filters, the vascular device may include a separate guide wire for introducing treatment devices proximal of the deployed vascular device. Additionally, the vascular device may have a second support hoop attached to the distal end of the sac. During retrieval, multiple hoops ensure that emboli are retained within the sac and prevent the sac from bunching. Where multiple hoops are rotated, they may be arranged such that they rotate independently of the guide wire, thereby reducing risk that the sac wall will become twisted during advancement.

In alternative embodiments, sac bunching is mitigated by tapering the sac and attaching it to one or more support hoops, or to the guide wire. Sac porosity may also be specified to ensure passage of blood cells and capture of emboli, as well as to control a pressure drop across the vascular device. In other embodiments, a delivery sheath is provided that permits a lesion to first be crossed with an unencumbered guide wire prior to passing the vascular device across the lesion. In still further embodiments, several support hoops may be provided at the mouth of a single sac to facilitate opening and closing of the sac.

In thrombectomy applications, a separate thrombectomy element may be provided in addition to the vascular filter. The thrombectomy element may be attached to the elongated member proximal of the vascular filter or may comprise a separate catheter. In a preferred embodiment, the thrombectomy element is similar in construction to the vascular filter and may be retracted independently. Alternatively, the thrombectomy element may be any conventional atherectomy device used in conjunction with the vascular filter and may be advanced and retracted either in conjunction or independently of the vascular filter.

A delivery system in accordance with the present invention, configured for use with the vascular devices described herein, is also provided. The delivery system integrates the functions of a Touhy Borst, a torquer, and a pusher into a single device, thereby facilitating introduction and retrieval of embodiments of the present invention. The torqueing function allows a vascular device to navigate tortuous anatomy. For example, the distal end of a guide wire may be rotated to selectively orient the vascular device in a selected branch of a bifurcated vessel.

The Touhy-Borst adapter permits liquid to be introduced or withdrawn through the lumen of the vascular device delivery catheter. The pusher feature of the delivery system allows deployment and retraction of the vascular device from within the delivery catheter.

5

Methods of using embodiments of the present invention are also provided, including use of novel radiopaque features, and use of a previously known balloon catheter to arrest antegrade flow through a vessel until the vascular device of the present invention is deployed.

BRIEF DESCRIPTION OF THE DRAWINGS

The above and other objects and advantages of the present invention will be apparent upon consideration of the following detailed description, taken in conjunction with the accompanying drawings, in which like reference characters refer to like parts throughout, and in which:

FIGS. 1A and 1B are, respectively, a side-sectional view of a previously known vascular device contracted within a delivery sheath, and an end view of that vascular device deployed in a vessel;

FIGS. 2A and 2B are, respectively, a perspective view of a vascular device constructed in accordance with the principles of the present invention in a deployed state, and a detailed view of the articulation region of the device of FIG. 2A;

FIG. 3 is a perspective view of the vascular device of FIGS. 2 in a folded configuration, prior to removal;

FIG. 4 is a plan view of the vascular device of FIGS. 2;

FIGS. 5A-5D are side sectional views depicting a method of deploying, using, and retrieving the vascular device of FIGS. 2-4;

FIG. 6 is a perspective view of an alternative embodiment of a vascular device of the present invention in a deployed state;

FIGS. 7A and 7B are, respectively, a perspective view and a plan view of a further alternative embodiment of the present invention in a deployed state;

FIGS. 8A-8E are sectional views of a vascular device disposed within alternative embodiments of delivery sheaths of the present invention;

FIG. 9 is a side view of a previously known balloon catheter;

FIGS. 10A-10D are views illustrating the steps of using the balloon catheter of FIG. 9 with the vascular device of FIGS. 2;

FIGS. 11A-11C are perspective views of further alternative embodiments of vascular devices constructed in accordance with the principles of the present invention;

FIG. 12 is a perspective view of an alternative embodiment of the vascular device of the present invention with two support hoops, shown in a deployed state;

FIG. 13 is a perspective view of an alternative embodiment of the vascular device of FIG. 12 with a smaller distal support hoop;

FIG. 14 is a perspective view of a still further alternative embodiment of the vascular device of FIG. 12 that allows the vascular device to independently rotate with respect to the guide wire;

FIG. 15 is a perspective view of an alternative embodiment of the present invention with a tapered blood permeable sac, shown in a deployed state;

FIG. 16 is a perspective view of a radiopaque support hoop constructed in accordance with one aspect of the present invention;

FIGS. 17A-17C illustrate another alternative embodiment of the vascular device of the present invention in which the articulation region comprises a gap in the support hoop bridged by the perimeter of the blood permeable sac;

FIGS. 18A and 18B are side-sectional views depicting an integrated vascular device of the present invention suitable for thrombectomy, disposed, respectively, within a delivery sheath and in a deployed state;

6

FIGS. 19A-19E are side-sectional views depicting a method of deploying, using, and retrieving the integrated vascular device of FIGS. 18;

FIGS. 20A and 20B are side-sectional views depicting an alternative embodiment of the integrated vascular device of FIGS. 18, disposed, respectively, within a delivery sheath and in a deployed state;

FIGS. 21A and 21B are side sectional views of delivery system constructed in accordance with the present invention coupled to the vascular device of FIG. 5A, shown, respectively, in a delivery configuration and in a deployed configuration;

FIGS. 22A-22E are side sectional views depicting a method of deploying, using, and retrieving a vascular device of the present invention in conjunction with a specially configured retrieval sheath; and

FIGS. 23A and 23B are side sectional views depicting a method of using and retrieving the vascular device in conjunction with an alternative embodiment of the specially configured retrieval sheath.

DETAILED DESCRIPTION OF THE INVENTION

Referring to FIGS. 1A and 1B, some of the disadvantages associated with previously known vascular devices, such as the emboli filters described in the above-mentioned International Publication WO 98/39053, are described. In FIGS. 1, the vascular filter comprises guide wire 10 having hoop 12 coupled to its end. Filter sac 14 is affixed to hoop 12, so that when delivery catheter 16 is retracted proximally and guide wire 10 is held stationary, hoop 12 radially expands to contact the walls of vessel V.

As described hereinabove, one difficulty with such vascular filters is that the hoop used to support the filter sac experiences increased stiffness when contracted to small diameters, i.e., due to the sharp directional change at the tip of the hoop, thereby limiting the minimum delivery profile achievable for such instruments. Although this effect may be reduced by decreasing the thickness of the wire employed in hoop 12, at the point at which the wire becomes sufficiently thin to accommodate the bending stresses, the wire is too thin to effectively radially expand and urge the filter sac into engagement with the vessel wall.

On the other hand, as shown in FIGS. 1A and 1B, the bending stresses imposed upon the hoop of such previously known devices, if drawn within a delivery catheter, may be sufficiently high to result in the formation of kink 18 at the tip of the hoop. This "kinking" effect becomes more severe in sheaths having a small inner diameter. Thus, for example, applicant has observed that when sheaths having inner diameters of 0.035" or smaller are used, a hoop of nitinol or multi-strand nitinol cable having a diameter of 0.0055" will form kink 18. Kink 18 in turn may apply relatively high localized pressure and friction against wall 17 of sheath 16, thereby making the vascular filter difficult to deploy. In particular, the kink may impale wall 17 of delivery sheath 16 and may make it difficult or impossible to deploy the vascular filter, especially in tortuous anatomy.

In addition, when the filter is subsequently deployed in vessel V, as shown in FIG. 1B, kink 18 may deform the pre-formed shape of hoop 12, impairing the ability of the filter to seal against the walls of vessel V. This may in turn lead to the presence of gaps G between the perimeter of the hoop and the vessel wall, depending upon the severity of the kink. Consequently, emboli may pass through the gaps with antegrade flow and significantly reduce the efficacy of the filter.

Additionally, kink **18** may be sufficiently sharp to damage or dissect the wall of vessel **V** when the filter is deployed.

The vascular device of the present invention solves the above-described disadvantages, providing a vascular device, suitable for use as a vascular filter or thrombectomy/embol-
5 lectomy device, with a self-expanding support hoop that is sufficiently thick to radially expand and urge a blood permeable sac into engagement with the vessel wall, but which includes an articulation region that overcomes the problems associated with kinking. In particular, the vascular device of
10 the present invention includes a reduced thickness articulation region and a pre-formed curved profile that avoids the difficulties of previously known systems while providing a high degree of efficacy in capturing emboli or thrombus, and ease of deployment and retrieval.

Referring now to FIGS. **2A** and **2B**, vascular device **20** constructed in accordance with the principles of the present invention, illustratively an embolic filler, comprises guide
15 wire **22**, support hoop **24** having articulation region **26**, and blood permeable sac **28** affixed to support hoop **24**. Sac **28** is coupled to support hoop **24** so that the support hoop **24** forms an opening for the sac. Support hoop **24** preferably is connected to guide wire **22** near distal end **23** of the guide wire.

Sac **28** preferably is constructed of a thin, flexible biocompatible material, such as polyethylene, polypropylene, poly-
20 urethane, polyester, polyethylene tetraphthalate, nylon or polytetrafluoroethylene, or combinations thereof. The material should be sufficiently thin, such that the sac is non-thrombogenic. Sac **28** includes openings or pores **30** that permit blood cells to pass through the sac substantially unhindered, while capturing any larger emboli, thrombus, or for-
25 eign bodies that may be released during a procedure, such as angioplasty or stent placement. In a preferred embodiment, sac **28** has openings or pores **30** in a range of about 20 to 400 microns in diameter, and more preferably, about approxi-
30 mately 80 microns. These pore sizes permit red blood cells (which have a diameter of approximately 5 microns) to easily pass through the sac, while capturing thrombus or emboli.

Pores **30** are preferably formed by a laser drilling process.
35 For example, a thin sheet of the flexible biocompatible material may be thermoformed to create sac **28**, for example, by stretching the sheet over a mandrel, by dip forming, or by blow molding. Sac **28** may alternatively be fabricated from an extruded tube of the biocompatible material. A flat metal
40 mask, with tiny holes approximately the size of pores **30**, may then be placed in front of the sac. A laser having a beam diameter equal to or greater than the diameter of the material illuminates the mask. The laser beam passes through the holes
45 in the mask and strikes the material, thereby forming pores **30** in sac **28**.

Laser drilling may also be accomplished with a laser hav-
ing a beam diameter approximately the size of pores **30**, in which case pores **30** may drilled individually. Sac **28** may
50 alternatively comprise a woven material, for example, formed from the above-mentioned polymers, having a pore diameter determined as a function of the pattern and tightness of the weave.

Support hoop **24** comprises a hoop having a circular or rectangular cross-section that is formed of a super-elastic
55 material, such as a nickel-titanium alloy ("nitinol"). During deployment and retrieval of vascular device **20**, described hereinafter, support hoop **24** folds in half and collapses to fit within a small diameter delivery sheath. When vascular device **20** is in a deployed state, as depicted in FIG. **2A**,
60 support hoop **24** resumes its pre-formed shape. Support hoop **24** preferably comprises nitinol wire, although it may also be

formed from a multi-strand nitinol cable, a spring tempered stainless steel, or other super-elastic material.

In accordance with the principles of the present invention, support hoop **24** includes one or more reduced-thickness
5 articulation regions **26**, and pre-formed curved regions **34**. As depicted in FIG. **2B**, articulation region **26** includes a region having reduced thickness t_1 compared to thickness t of the remainder of support hoop **24**. Articulation region **26** and
10 curved regions **34** enable support hoop **24** to fold with a predetermined shape when vascular device **20** is collapsed to a contracted state for delivery or retrieval.

In FIG. **2B**, articulation region **26** is depicted as a localized reduction in the thickness of support hoop **24**, as may be
15 achieved, for example, using conventional grinding, chemical etching, or electroless polishing processes. Alternatively, support hoop **24** may be continuously tapered along its circumference, so that articulation region **26** results from a more gradual reduction in the wall thickness of the support hoop.
20 Tapering support hoop **24** may permit greater flexibility in the vicinity of articulation region **26**, thus enabling support hoop **24** to fold more easily at the articulation region. Such tapering of the thickness of the support hoop along a portion of its circumference also may reduce the potential for stress-in-
25 duced fracture typically associated with abrupt changes in diameter.

In a preferred embodiment of vascular device **20** of the present invention, vascular device **20** easily fits within a deliv-
ery sheath having an inner diameter of 0.033", and, more preferably, may be used with a delivery sheath having an
30 inner diameter as small as 0.026". The deployed diameter of support hoop **24** preferably is approximately 7 mm, while guide wire **22** preferably has a diameter of 0.014". The distal end of guide wire **22** also may be tipped with a spring section or coil tip, as is per se known.

Support hoop **24** preferably is constructed of 0.0055" niti-
35 nol wire tapered (by a grinding, chemical etching, or electroless polishing process) to 0.0025" at articulation region **26**. Specifically, articulation region **26** preferably consists of a length about 0.05" long and having a diameter of 0.0025",
40 coupled on either side to curved regions **34**. Each of curved regions **34** includes a length of wire that is tapered from a diameter of 0.055" to a diameter of 0.0025" over a length of about 0.025". Support hoop **24** also may include radiopaque
45 features, such as gold or platinum bands **33**, spaced at intervals around the circumference of support hoop **24**, or a coil of radiopaque material wrapped around the support hoop, as described hereinafter with respect to FIG. **16**, or a gold plated coating.

Referring to FIGS. **3** and **4**, additional features of vascular
50 device **20** are described. FIG. **3** depicts vascular device **20** of FIG. **2A** in a contracted state, while FIG. **4** illustrates a directional change in support hoop **24** preferably caused by the presence of curved regions **34**. Advantageously, use of articu-
55 lation region **26** and the curved profile of support hoop **24** introduced by curved regions **34** also cause support hoop **24** to fold in half during retrieval. As shown in FIG. **3**, support hoop **24** folds in half, effectively closing the mouth of blood permeable sac **28** and preventing the escape of collected emboli or thrombus. This feature also may permit the use of a
60 smaller or shallower sac than would otherwise be possible, without increasing the risk of material escaping from the device when the sac is collapsed for retrieval. Use of a smaller or shallower sac also enables vascular device **20** to be delivered in a smaller delivery sheath, having an inner diameter as
65 small as 0.026" for the preferred embodiment.

Referring now to FIGS. **5A-5D**, methods of using the vas-
cular device of the present invention as a vascular filter are

described. In FIG. 5A, guide wire 22 and delivery sheath 40 are manipulated into position within vessel V using well-known percutaneous techniques. Vascular device 20 of FIG. 2A is disposed in its contracted delivery state within distal end 42 of delivery sheath 40, and delivery sheath 40 is advanced through the vessel using distal end 23 of guide wire 22. Articulation region 26 and curved regions 34 of support hoop 24 enable the sides of the support hoop to fold together and become elongated when drawn within delivery sheath 40. The size of delivery sheath 40 and guide wire 22 have been exaggerated to illustrate structure. In reality, the diameter of delivery sheath 40 is approximately an order of magnitude smaller than the internal diameter of vessel V.

With respect to FIG. 5B, once delivery sheath 40 is disposed at a desired location within a patient's vessel V, such as a coronary artery or carotid artery, as determined, for example, by the position of radiopaque band 43 under a fluoroscope, guide wire 22 is held stationary while delivery sheath 40 is retracted proximally. Alternatively, delivery sheath 40 may be held stationary while guide wire 22 is advanced. In either case, when vascular device 20 is no longer confined within delivery sheath 40, support hoop 24 expands to seal against the walls of vessel V. When in its deployed state, curved regions 34 of support hoop 24 orient articulation region 26 concentrically against the inside wall of the vessel, thus reducing the risk of impaling the vessel wall, as might be expected of the kinked support hoop of FIG. 1B. Blood continues to flow unimpeded through vessel V in direction D.

In FIG. 5C, once vascular device 20 is deployed in vessel V, other interventional instruments, such as angioplasty catheters, atherectomy devices, or stent delivery systems may be advanced along guide wire 22 to position such devices at treatment zones located proximally of vascular device 20. For example, in FIG. 5C, angioplasty balloon catheter 44 has been advanced along guide wire 22 to a position proximal of vascular device 20 to trap emboli E, i.e., pieces of plaque dislodged from the walls of vessel V by balloon 46.

With respect to FIG. 5D, upon completion of the angioplasty procedure using angioplasty balloon catheter 44, guide wire 22 is pulled proximally to cause the sides of support hoop 24 to collapse together to close the mouth of sac 28 (see FIG. 3). Additional proximal retraction of guide wire 22 causes support hoop 24 and sac 28 to enter at least partially within the guide wire lumen of angioplasty catheter 44. As depicted in FIG. 5D, only a portion of support hoop 24, near articulation region 26, and a distal portion of sac 28 extend out of the guide wire lumen of angioplasty catheter 44. Alternatively, vascular device 20 may be fully retracted within the guide wire lumen. Angioplasty catheter 44 then is withdrawn with vascular device 20 and any trapped emboli E.

Advantageously, the compliant design of vascular device 20 permits the device to be contracted to its delivery state within the guide wire lumen of conventional previously known interventional devices. Accordingly, unlike previously known vascular devices, which require removal of the interventional device followed by re-insertion of a specially designed catheter to retrieve the vascular device, the system of the present invention reduces the time, effort and trauma of this additional step. Instead, the vascular device may be readily closed and retrieved upon completion of the interventional procedure.

Vascular device 20 alternatively may be used in performing thrombectomy/embolectomy. In this case, the vascular device is deployed in a vessel at a location distal to a lesion, in the manner depicted in FIGS. 5A and 5B. Once support hoop 24 is deployed into contact with the vessel wall, vascular device 20 may be retracted proximally to scrape along the wall of the

vessel, and excise thrombus so that it is captured in sac 28. Delivery sheath 44 may then be re-inserted into the vessel along guide wire 22, and vascular device 20 is retracted and removed from the vessel. Additional thrombectomy embodiments are described hereinbelow with respect to FIGS. 18-20.

As discussed hereinabove, sac 28 is porous so that blood cells may pass through while emboli E are captured. As seen in FIG. 5B, if the sum of the area of all these pores A_1 is less than the internal cross-sectional area A_2 of vessel V, a pressure drop is expected across the vascular device. This may lead to hemolysis and insufficient downstream flow. If A_1 is greater than or equal to A_2 , the pressure drop is expected to decrease. Proper selection of pore diameter (in the range of 20-400 microns) and pore density ensures that A_1 is greater than or equal to A_2 .

Selection of a larger pore diameter within the provided range may also reduce the pressure drop by decreasing drag as blood passes through sac 28. Drag may further be decreased by providing elliptical pores through the sac that project round relative to blood flow when sac 28 is deployed. Furthermore, the porosity of sac 28 may be specified such that, if distal pores become occluded with thrombus, emboli, etc., proximal pores remain open to ensure continuous blood flow. It should also be noted that flow through vessel V is substantially unaffected by placement of sac 28 and hoop 24 in the flow path.

Referring now to FIG. 6, an alternative embodiment of the vascular device of the present invention, again illustratively a vascular filter, is described. Vascular device 50 comprises guide wire 51 and support hoops 52 and 53 connected to blood permeable sac 54. As discussed hereinabove, vascular device 50 includes articulation regions 55 and 56 formed at the intersection of opposing curved regions 57 and 58 of support hoops 52 and 53. Sac 54 preferably also is connected to guide wire 51 along its entire length, thereby providing more controlled deployment and removal of vascular device 50. Support hoop 53 serves to stabilize and deploy the distal portion of sac 54. In addition, affixing sac 54 to guide wire 51 may provide a more compact arrangement within a delivery sheath, and prevent bunching of the sac material.

In FIGS. 7A and 7B, a further alternative embodiment of the vascular device of the present invention is described. Vascular device 60, shown in the deployed state, comprises guide wire 61 having multi-turn helical support hoop 63 connected at weld point 62. Blood permeable sac 64 is affixed to the distal-most portion of support hoop 63. Support hoop 63 includes one or more side turns 65 that terminate in curved regions 66, as described hereinabove. Curved regions 66 in turn are joined together by articulation region 67. Preferably, side turns 65 are coupled to one another and to the distal region of guide wire 61, e.g., by a weld bead, at point 68.

In accordance with this aspect of the present invention, vascular device 60 may be contracted to small profile delivery state. When deployed from a delivery catheter, such as delivery sheath 40 of FIG. 5A, side turns 65 expand into contact with the walls of the vessel proximal to the location at which curved regions 66 contact the vessel wall. Side turns 65 serve to stabilize the support hoop 63 and sac 64 when vascular device 60 is deployed within a blood vessel. In addition, side turns 64 are expected to assist in orienting the axis of support hoop 63 and sac 64 in alignment with the longitudinal axis of vessel V. Accordingly, support hoop 63 is expected to reduce the risk of tilting of the vascular device within the vessel, and thus enhance the safety and reliability of the device.

Referring now to FIGS. 8A-8E, several embodiments of a delivery sheath suitable for use with the vascular device of the present invention are described. Each of these embodiments

are designed to permit the physician to first pass a guide wire across a lesion before passing the vascular device of the present invention across the lesion. Thus, the risk of generating emboli, during the step of positioning the vascular device of the present invention distal to a lesion, is expected to be reduced.

In particular, in FIG. 8A, vascular device [70] of the present invention comprises guide wire 71, support hoop [72] 92 and blood permeable sac [73] 93 folded in a contracted delivery state within lumen [74] 96 of delivery sheath [75] 95. Vascular device [70] in FIG. 8A is similar in design to vascular device 20 of FIG. 2A, except that the device [70] in FIG. 8A includes nose cone 76 affixed to distal region 77 of guide wire 71. Delivery sheath [75] 95 includes hemostatic fitting 78 at its proximal end and guide wire lumen 79.

In accordance with the methods of the present invention, the vascular device [70] and guide wire 80 are used as follows. First, unencumbered guide wire 80 is advanced through a vessel until distal region 81 of the guide wire crosses a lesion. The proximal end of guide wire 80 then is inserted into the distal end of guide wire lumen 79 of delivery sheath [75] 95 using previously known "over the wire" techniques.

Delivery sheath [75] 95 then is advanced over guide wire 80, which is held stationary, until nose cone 76 and a distal portion of the delivery sheath cross the lesion. Once support hoop [72] 92 and sac [73] 93 of the vascular device [70] are positioned distal to the lesion, guide wire 80 is withdrawn from the vessel and delivery sheath [75] 95 is retracted proximally, thereby deploying the vascular device [70] to its deployed state. As will of course be understood, nose cone 76 remains in the vessel, distal to sac [73] 93, during deployment of the vascular device. Upon completion of use of the vascular device [70], delivery sheath [75] 95 may once again be advanced along guide wire 71 and the support hoop and sac retracted within lumen [74] 96 of delivery sheath [75] 95. Alternatively, an interventional device may be advanced over guide wire 71 to perform a medical procedure, and the vascular device may be retrieved within a guide wire lumen of the interventional device, as discussed hereinabove with respect to FIGS. 5.

Vascular device 90 of FIG. 8B is similar in construction to that of FIG. 8A, and includes guide wire 91, support hoop 92, blood permeable sac 93 and nose cone 94. Delivery sheath 95 includes lumen 96 housing device 90, guide wire lumen 97, and hemostatic fitting 98. Guide wire lumen 97 opens through skive 99 in lateral wall 100 of delivery sheath 95. Guide wire 101 therefore may be used in accordance with well-known "rapid exchange" techniques, wherein the length of unencumbered guide wire 101 may be significantly shorter than in the case of the "over the wire" arrangement depicted in FIG. 8B. Operation of delivery sheath 95 and vascular device 90 is similar to that described hereinabove with respect to FIG. 8A, except that the proximal end of unencumbered guide wire 101 is passed through the distal end of lumen 97 and passes out through skive 99.

In FIG. 8C, delivery sheath 105 includes lumen 106 that opens through the lateral wall via skive 107, and guide wire lumen 108 that opens through the lateral wall via skive 109. Accordingly, as will be apparent to one of ordinary skill, both vascular device 110 and guide wire 112 may be used as described hereinabove with respect to FIG. 8A and further in accordance with "rapid exchange" techniques.

Vascular device 113 of FIG. 8D is similar in construction to those described hereinabove. Delivery sheath 114 includes lumen 115, guide tube 116, and hemostatic fitting 117. Lumen 115 houses device 113 during delivery and retrieval. Guide tube 116 comprises guide wire lumen 118, which is

configured to receive unencumbered guide wire 119. In operation, the proximal end of guide wire 119 is passed through guide wire lumen 118 of guide tube 116. Thus, guide wire 119 may be used in accordance with "rapid exchange" techniques described with respect to FIG. 8B and with "over the wire" techniques described with respect to FIG. 8A.

Vascular device 120 of FIG. 8E is also similar to those described hereinabove. Delivery sheath 121 includes lumen 122 and hemostatic fitting 123. Lumen 122 houses device 120. Guide wire 124 is coupled to and terminates at the proximal end of delivery sheath 121. Thus, distal end 126 of guide wire 125 of vascular device 120 is first to cross the lesion. Then, nose cone 127, attached to guide wire 125, and a distal portion of delivery sheath 121 cross the lesion. Guide wire 124 and attached delivery sheath 121 are retracted proximally, thereby deploying vascular device 120 to its deployed state. Device 120 may then be retrieved within sheath 121 or within an interventional device, as discussed hereinabove.

Referring now to FIG. 9, a previously known balloon catheter is described. Catheter 130 is constructed of materials typically used in catheters, such as polyethylene or polyurethane, and includes compliant balloon 131 disposed in distal region 132. Compliant balloon, which may be formed of nylon or latex, is inflated using inflation port 133 at proximal end 134 of the catheter. Catheter 135 also includes hemostatic port 136 and an interior lumen through which a delivery sheath may be advanced to pass out of an opening in distal end 137.

With respect to FIGS. 10A-10C, a method of using catheter 130 of FIG. 9 in conjunction with the vascular device of the present invention is described. In accordance with this aspect of the present invention, antegrade blood flow through a vessel is occluded while a vascular device constructed in accordance with the present invention is advanced across a lesion. Once the vascular device, illustratively a vascular filter, is deployed, the balloon is deflated, thereby permitting antegrade flow to be established. Importantly, because flow through the vessel is stopped prior to deployment of the vascular device, few or no emboli are expected to bypass the filter.

More particularly, with respect to FIG. 10A, catheter 130 is disposed in vessel V at a location proximal to lesion L, with the vascular device of the present invention disposed in its contracted delivery state in delivery sheath 138. In FIG. 10B, balloon 131 is inflated via inflation port 133 to engage the interior wall of vessel V, thereby arresting antegrade flow in the vessel.

As shown in FIG. 10C, delivery sheath 130 then is advanced across lesion L so that the support hoop and sac of the vascular device will be disposed distal to lesion L when deployed. During this step, delivery sheath 138 may generate emboli E as it passes across the lesion. However, because antegrade flow in the vessel is stopped, the emboli will not travel distally in the vessel.

With respect to FIG. 10D, once vascular device 140 is deployed, so that support hoop 141 and sac 142 span vessel V, balloon 131 is deflated. This, in turn, causes antegrade flow to become re-established in vessel V, urging emboli E into sac 142. Catheter 130 then may be withdrawn, and additional treatment devices advanced along guide wire 143 of vascular device 140. Removal of vascular device 140 may be by any of the methods described hereinabove with respect to FIG. 5D.

Referring now to FIGS. 11A-11C, still further alternative embodiments of vascular devices constructed in accordance with the present invention are described. Each of the devices of FIGS. 11A-11C, which are shown in the deployed state, includes two or more support hoops to support the blood

permeable sac. Each of those support hoops in turn includes an articulation region that permits the sides of the support hoops to collapse inwards to each other as described hereinabove with-respect to FIGS. 3 and 4.

Specifically, in FIG. 11A vascular device 150, illustratively an embolic filter, comprises guide wire 151, support hoops 152 and 153 having articulation regions 154 and 155, respectively, and blood permeable sac 156 affixed to support hoops 152 and 153. Sac 156 is coupled to support hoops 152 and 153 so that the support hoops form an opening for the sac. Support hoops 152 and 153 preferably are connected to guide wire 151 near its distal end.

Sac 156 is also attached to the distal end of guide wire 151 at point 157. Sac 156 preferably is constructed of a thin, flexible biocompatible material, as for the embodiments described hereinabove, and includes openings or pores 158 that permit blood cells to pass through the sac substantially unhindered, while capturing any larger material that may be released during a procedure such as angioplasty or stent placement. Pore sizes are selected as described hereinabove with respect to FIG. 2A.

Support hoops 152 and 153 comprise hoops having circular or rectangular cross-sections that are formed of a superelastic material, such as a nickel-titanium alloy ("nitinol"). During deployment and retrieval of vascular device 150, support hoops 152 and 153 fold in half and collapse to fit within a small diameter delivery sheath. When the delivery sheath is retracted, support hoops 152 and 153 resume their pre-formed shape and deploy the perimeter of sac 156 into contact with the vessel walls. Support hoops 152 and 153 preferably comprise a nitinol wire, but also may be formed from a multi-strand nitinol cable, or other superelastic material.

In accordance with the principles of the present invention, support hoops 152 and 153 are affixed to guide wire 151 at ring 159 and include reduced-thickness articulation regions 154 and 155, constructed as described hereinabove. More particularly, support hoops 152 and 153 are pre-formed to form structures having curved regions 160 and 161, respectively, so that articulation regions 154 and 155 are disposed in a portion of the support hoop that is approximately concentric with a vessel wall when vascular device 150 is deployed. Articulation regions 154 and 155 and curved regions 160 and 161 thus enable support hoops 152 and 153 to fold with a pre-determined shape when vascular device 150 is collapsed to a contracted state for delivery or retrieval.

In a preferred embodiment of vascular device 150 of the present invention, vascular device 150 easily fits within a delivery sheath having an inner diameter of 0.033", and more preferably, may be used with a delivery sheath having an inner diameter as small as 0.026". The deployed diameter of vascular device 150 preferably is approximately 7 mm.

Compared to vascular device 20 of FIGS. 2-4, vascular device 150 of FIG. 11A employs two support hoops instead of one and provides central location of guide wire 151 and attachment of blood permeable sac 156 to the distal end of the guide wire. These differences may provide more controlled deployment and removal of vascular device 150. In addition, affixing sac 156 to guide wire 151 may provide a more compact arrangement within a delivery sheath, and prevent bunching of the sac material.

Referring now to FIG. 11B, another alternative embodiment of the vascular device of the present invention, again illustratively a vascular filter, is described. Vascular device 170 is similar in construction to vascular device 150, except that vascular device 170 employs three support hoops instead

of two. Device 170 comprises guide wire 151 and support hoops 171, 172 and 173 connected to blood permeable sac 156.

As discussed hereinabove, vascular device 170 includes articulation regions 174, 175 and 176 formed at the intersection of opposing curved regions 178, 179 and 180 of support hoops 171, 172 and 173. Support hoops 171, 172 and 173 preferably are connected to the distal end of guide wire 151 at ring 177. Sac 156 preferably also is connected to guide wire 151 at point 157. Vascular device 170 is expected to provide similar advantages to those contemplated for vascular device 150.

With reference to FIG. 11C, yet another alternative embodiment of the vascular device of the present invention, again illustratively a vascular filter, is described. Vascular device 190 is similar in construction to vascular devices 150 and 170, except that vascular device 190 employs four articulated support hoops. Device 190 comprises guide wire 151 and support hoops 191, 192, 193 and 194 connected to blood permeable sac 156, with articulation regions 195, 196, 197 and 198 formed at the intersection of opposing curved regions 200, 201, 202 and 203 of the respective support hoops 191-194. Support hoops 191-194 are preferably connected to the distal end of guide wire 151 at ring 199.

Alternative embodiments of vascular devices of the present invention have been described with one to four support hoops. As will be apparent to one of ordinary skill in the art of interventional device design, any number of support hoops may be used with minor modifications to the designs described hereinabove.

Referring now to FIGS. 12-15, further alternative embodiments of the vascular device of the present invention are described. In FIG. 12, vascular device 250, illustratively an embolic filter, comprises guide wire 252, support hoops 253 and 254 having articulation regions 255 and 256, respectively, and blood permeable sac 258 affixed to support hoops 253 and 254. Sac 258 is coupled to support hoop 253 at its proximal end so that the support hoop forms an opening for the sac. Sac 258 is coupled to support hoop 254 at its distal end to prevent emboli from spilling from sac 258 during retrieval. Support hoops 253 and 254 preferably are connected to guide wire 252 near distal end 259 of the guide wire. Sac 258 has openings or pores 260 that permit red blood cells to easily pass through the sac.

During deployment and retrieval of vascular device 250, support hoops 253 and 254 expand and collapse as discussed hereinabove with respect to support hoop 24 of FIGS. 2. Support hoops 253 and 254 are attached to guide wire 252 at attachment points 261 and 262, respectively, and further comprise curved regions 263 and 264, respectively. Support hoops 253 and 254 may include radiopaque features, such as gold or platinum bands 265, spaced at intervals around the circumference of the hoops.

Applicant expects that vascular device 250 may further reduce the risk that captured emboli could spill during retrieval, and also may provide a better seal against the artery.

With reference to FIG. 13, an alternative embodiment of vascular device 250 that prevents bunching is disclosed that may provide even further benefits. Vascular device 270 comprises guide wire 272 on which proximal support hoop 273 and distal support hoop 274 are disposed. The proximal and distal portions of blood permeable sac 275 are affixed to support hoops 273 and 274, respectively. Proximal support hoop 273 is attached to distal end 271 of guide wire 272 at attachment point 276 and includes articulation region 277 and curved regions 278. Likewise, distal support hoop 274 is attached to guide wire 272 at attachment point 279 and

15

includes articulation region **280** and curved regions **281**. Sac **275** includes blood permeable pores **282**. Hoops **273** and **274** may include radiopaque features, such as gold or platinum bands **283**, spaced at intervals around the circumference of the hoops.

Proximal support hoop **273** is significantly larger in circumference than distal hoop **274**. Proximal hoop **273** seals against the artery walls and defines the diameter of the mouth of sac **275**. Smaller distal hoop **274** prevents emboli from spilling from sac **275** when retrieving device **270**. It also allows the diameter of sac **275** to decrease along its length. This taper in sac **275** is expected to reduce the risk that sac **275** will bunch when the sac is retrieved. Sac **275** may further be attached to guide wire **272**.

Applicant has determined that where multiple support hoops are employed, as in the embodiments of FIGS. **12** and **13**, twisting of the guide wire during deployment may prevent the sac of the vascular device from properly sealing against the vessel wall. For example, if guide wire **252** in the embodiment of FIG. **12** is rotated after distal hoop **254** has been deployed, but before proximal hoop **253** has been deployed, proximal hoop **253** may deploy at an angle with respect to distal hoop **254**. This, in turn, may constrict, or all together close, the opening of sac **258**, thereby rendering the vascular device ineffective.

FIG. **14** discloses a vascular device in accordance with the present invention that overcomes problems associated with twisting of the guide wire during deployment. Vascular device **290** comprises guide wire **292** with distal end **293**, and support hoops **294** and **295**. Support hoops **294** and **295** further comprise articulation regions **296** and **297**, respectively, and curved regions **298** and **299**, respectively. The proximal and distal portions of blood permeable sac **300** are attached to support hoops **294** and **295**, respectively. Sac **300** includes pores **301**. Support hoops **294** and **295** are attached to sheath **302** at attachment points **303** and **304**, respectively. Sheath **302** preferably comprises a flexible, 0.001" thick tube made of a biocompatible material, such as polyamide or polytetraethylene. Guide wire **292** passes through the lumen of sheath **302**. Sheath **302** is able to rotate with respect to guide wire **292** but is translationally restrained by stops **305** and **306**, for example, solder beads.

By attaching support hoops **294** and **295** to sheath **302**, rotational problems are mitigated. Sheath **302** only transmits translational motion of guide wire **292** to support hoops **294** and **295**. Thus, twisting moments applied to wire **292** will not affect the performance of vascular device **290**. Sac **300** may also be attached to sheath **302**.

With reference to FIG. **15**, a further alternative embodiment of the vascular device of the present invention is disclosed that also prevents bunching. Vascular device **310** comprises guide wire **312** on which support hoop **313** is disposed. Tapered blood permeable sac **314** is affixed to support hoop **313**. Hoop **313** is attached to distal end **311** of guide wire **312** at attachment point **315** and includes articulation region **316** and curved regions **317**. Tapered sac **314** includes blood permeable pores **318**. Hoop **313** may include radiopaque features, such as gold or platinum bands **319**, spaced at intervals around the circumference of the hoop.

As with vascular device **270** of FIG. **13**, the diameter of tapered sac **314** decreases along its length to reduce the risk of bunching when the sac is retrieved. Tapering also reduces the amount of material that must fit within the lumen of a delivery sheath, and thereby allows a delivery sheath of smaller profile to be used. Furthermore, tapering the blood permeable sac reduces the risk that the sac will snag on a stent during retrieval.

16

Because vascular device **310** lacks the distal support hoop of the embodiments of FIGS. **12** and **13**, there is a reduced risk of problems associated with twisting. In a preferred embodiment, the diameter at the distal end of tapered sac **314** is less than the internal diameter of the retrieval sheath with which the apparatus is used. Tapered sac **314** may optionally be attached to guide wire **312**, for example, to further mitigate bunching.

Referring now to FIG. **16**, a support hoop including a radiopaque feature is disclosed. Support hoop **320**, illustratively shown in the deployed state, comprises articulation region **321**, curved regions **322**, attachment point **323**, and wound radiopaque wire **324**. In the preferred embodiment, wire **324** is platinum and is either round or a strip approximately 0.001" in diameter. Wire **324** is wrapped around hoop **320** all along its circumference.

One method of making a vascular device radiopaque is to electroplate platinum or gold onto the device. However, electroplating can be complex and expensive, and may cause manufacturing difficulties. Because the hoop must change shape during deployment and retrieval, increased thickness or flaking of plated gold are undesirable characteristics and may promote failure of the support hoop. By wrapping wire **324**, hoop **320** maintains its strength and flexibility. Radiopaque wire **324** may be used in conjunction with any of the vascular devices discussed herein. Radiopaque wire **324** may further be used with a wide variety of other vascular filter devices, as are known in the art.

Referring now to FIGS. **17A-17C**, another alternative embodiment of the vascular device of the present invention is described. As illustrated in FIG. **17A**, vascular device **330** comprises guide wire **332** with distal region **333**, wishbone support hoop **335**, and blood permeable sac **336**. Wishbone hoop **335** comprises spines **337** and **338** separated by a gap that serves as articulation region **339**. Articulation region **339** is shown in greater detail in FIG. **17B**, which corresponds to the area circled in FIG. **17A** taken along section B-B. Blood permeable sac **336** is wrapped around and attached to itself all along its perimeter, creating hem bond **340** and lumen **341**. Sac **336** includes pores **347**. Lumen **341** is configured to receive spines **337** and **338** and bridge the gap between them. FIG. **17C** is a sectional view taken along line C-C of FIG. **17A**, showing hem bond **340** and lumen **341** with spine **338** passing there through.

Referring again to FIG. **17A**, wishbone support hoop **335** is attached to sheath **343** at attachment point **344**. Sheath **343** is similar to sheath **302** of the embodiment of FIGS. **14**, and preferably comprises a flexible, 0.001" thick tube made of a biocompatible material, such as polyamide or polytetraethylene. Distal end **333** of guide wire **332** passes through the lumen of sheath **343**. Sheath **343** may rotate with respect to guide wire **332** but is translationally restrained by stops **345** and **346**, for example, solder beads. Sheath **343** mitigates rotational problems by only transmitting translational motion of guide wire **332** to wishbone hoop **335**. Twisting moments applied to wire **332** do not affect the performance of vascular device **330**.

The wishbone design of support hoop **335** advantageously enables a wider variety of materials to be used to fabricate the support hoop. Articulation region **339** allows vascular device **330** to deploy and contract in a manner similar to that described above for alternative embodiments. Deployment and retraction of wishbone hoop **335** induces minimal deformation of spines **337** and **338**, thereby permitting use of materials such as spring steel. As will of course be apparent,

the support hoop of the embodiment of FIGS. 17A-17C may advantageously be incorporated in any of the foregoing embodiments.

Referring now to FIGS. 18A and 18B, an integrated vascular device suitable for thrombectomy is described. The integrated device comprises a thrombectomy element and a vascular filter. In a preferred embodiment, the thrombectomy element is similar in construction to vascular filter 20 described above and is connected to the guide wire proximal of the vascular filter. Alternatively, the thrombectomy element may be disposed on a separate catheter. The thrombectomy element may be retracted independently of the vascular filter.

In FIGS. 18, integrated vascular device 350 comprises guide wire 351, thrombectomy element 352 including support hoop 353 and blood permeable sac 354, and vascular filter element 355 including support hoop 356 and blood permeable sac 357. Filter hoop 356 is attached to guide wire 351 while thrombectomy hoop 353 is attached to ring 358. Ring 358 is attached to pull wire 359 and has a bore through which guide wire 351 passes. Ring 358 therefore acts as a linear bearing and allows thrombectomy hoop 353 to be moved by pull wire 359 independently of guide wire 351. Alternatively, thrombectomy element 352 may omit sac 354 and simply comprise a wire hoop; in this case severed thrombus is captured by vascular filter 355.

In FIG. 18A, support hoops 353 and 356 and blood permeable sacs 354 and 356 are contracted to a delivery state within lumen 360 of delivery sheath 361. Delivery sheath 361 includes nose cone 362 affixed to distal region 363 of guide wire 351. In FIG. 18B, integrated vascular device 350 is shown deployed in a vessel. As illustrated in FIG. 18B, vascular filter 355 expands to engage the perimeter of the vessel and prevent thrombus from bypassing the blood permeable sac, while thrombectomy element 352 engages the vessel wall proximal of vascular filter 355. As described hereinbelow, proximal movement of thrombectomy device 352 scrapes thrombus from the wall of the vessel when pull wire 359 pulls ring 358 and support hoop 353 proximally.

Referring now to FIGS. 19A-19E, an illustrative method of using the integrated vascular device of the present invention for thrombectomy is described. In FIG. 19A, guide wire 351 is manipulated into position proximal to thrombus T within vessel V using well-known percutaneous techniques. Vascular device 350 of FIGS. 18A and 18B is disposed in its contracted delivery state within the distal end of delivery sheath 361 and the delivery sheath is advanced through the vessel using distal end 363 of guide wire 351. The sides of support hoops 353 and 356 are folded together and become elongated when drawn within delivery sheath 361, as described with respect to vascular device 20 of FIGS. 2-4.

With respect to FIG. 19B, once delivery sheath 361 is disposed at the desired location proximal to thrombus T within a patient's vessel V, such as a coronary artery or carotid artery, based on the position of, for example, radiopaque bands under a fluoroscope, integrated vascular device 350 is advanced through thrombus T. Distal end 363 of guide wire 351 is advanced through the lesion, then nose cone 362 gradually increases the diameter of the void within thrombus T so that the remainder of delivery sheath 361 can be advanced far enough that thrombectomy element 352 (still within delivery sheath 361) is located distal to thrombus T.

With integrated vascular device 350 in position, guide wire 351 is held stationary while delivery sheath 361 is retracted proximally, as seen in FIG. 19C. Alternatively, delivery sheath 361 may be held stationary while guide wire 351 is advanced. In either case, when vascular device 350 is no

longer confined within delivery sheath 361, support hoops 353 and 356 expand to seal against the walls of the vessel V and deploy blood permeable sacs 354 and 357, respectively. Blood continues to flow through vessel V in direction A, impeded only by thrombus T.

In FIG. 19D, once vascular device 350 is deployed in vessel V, thrombus T is removed in the following manner. Vascular filter support hoop 353 is rigidly attached to guide wire 351, while thrombectomy support hoop 353 is attached to pull wire 359 via ring 358. Thrombectomy element 352 then is retracted proximally to scrape along the wall of the vessel V by motion at the proximal end of pull wire 359. Thrombus T, located proximal to thrombectomy element 352, is excised so that it is captured in blood permeable sac 354 during the retraction.

With respect to FIG. 19E, once thrombus T has been captured within sac 354, pull wire 359 is pulled proximally to cause the sides of thrombectomy support hoop 353 to collapse together to close the mouth of sac 354 (see FIG. 3). Additional proximal retraction of pull wire 359 causes support hoop 353 and sac 354 to enter within lumen 360 of delivery sheath 361, restoring normal blood flow to vessel V. Meanwhile, vascular filter 355 is in a position distal to thrombectomy element 352 to trap emboli E, i.e., pieces of plaque dislodged from either thrombus T or the walls of vessel V by thrombectomy element 352. Once any emboli E have been collected, filter hoop 356 and sac 357 are retracted into delivery sheath 361 by motion at the proximal end of guide wire 351, in a manner similar to the retraction of hoop 353 and sac 354. Once guide wire 351 has been fully retracted, and nose cone 362 at the distal end 363 of guide wire 351 is again in contact with delivery sheath 361, the delivery sheath is withdrawn with integrated vascular device 350, the trapped thrombus T, and any trapped emboli E.

As with previous embodiments, the compliant design of integrated vascular device 350 permits the device to be contracted to its delivery state within the guide wire lumen of conventional previously known interventional devices, thereby reducing time, effort, and trauma. The vascular device may be readily closed and retrieved upon completion of the interventional procedure.

Referring now to FIGS. 20A and 20B, an alternative embodiment of the integrated vascular device is described. Integrated vascular device 370 comprises guide wire 371, thrombectomy element 372, and vascular filter 373 having support hoop 374 and blood permeable sac 375. Filter hoop 374 is attached to guide wire 371, while thrombectomy element 372 is disposed to slide along guide wire 371. Alternatively, thrombectomy element 372 may be disposed on a separate catheter element that extends either through lumen 377 of delivery sheath 378 or is separately disposed proximal to vascular filter 373. FIG. 20A shows thrombectomy element 372 and vascular filter 373 contracted in a delivery state within lumen 377 of delivery sheath 378. Delivery sheath 378 includes nose cone 379 affixed to distal region 380 of guide wire 371. In FIG. 20B, integrated vascular device 370 is shown in the deployed state.

Thrombectomy element 372 may comprise any of a family of known thrombectomy, atherectomy, or, alternatively, drug delivery devices suitable for use in conjunction with vascular filter 373. Thrombectomy element 372 may, for example, comprise any of: a rotary ablation device, such as described in U.S. Pat. No. 4,867,156 to Stack et al., U.S. Pat. No. 4,990,134 to Auth, and U.S. Pat. No. 5,314,407 to Auth et al.; an atherectomy technology, such as described in U.S. Pat. No. 5,181,920 to Mueller et al., and U.S. Pat. No. 5,074,841 to Ademovic et al.; or a balloon embolectomy technology, such as

described in U.S. Pat. No. 3,923,065 to Nozick et al., U.S. Pat. No. 5,769,871 to Mers Kelly et al., U.S. Pat. No. 5,192,290 to Hilal, U.S. Pat. No. 5,112,347 to Taheri, and U.S. Pat. No. 4,030,503 to Clark III. All of the foregoing patents are incorporated herein by reference. Thrombectomy element **372** may alternatively comprise a wire loop or ring, such as described for the embodiment of FIGS. **18A** and **18B**, a laser ablation device, a chemical flushing system, etc.

Referring now to FIGS. **21A** and **21B**, a delivery system configured for use with embodiments of the present invention is described. The delivery system facilitates deployment and retrieval of the embodiments by integrating the functions of a torquer, a Touhy Borst adapter, and a pusher into a single device. In FIGS. **21**, the delivery system is illustratively used in conjunction with vascular device **20** of FIGS. **2-5**. In FIG. **21A**, vascular device **20** is in the retracted delivery configuration, while in FIG. **21B** vascular device **20** is in the expanded deployed configuration. Delivery system **450** comprises proximal screw cap **452**, collet **456**, handle **460**, rod **464**, central screw cap **468**, lumen flushing section **472**, distal hub **479**, and nose piece **486**.

Proximal screw cap **452** includes bore **453** with female screw thread **454** and guide wire lumen **455**. Bore **453** extends proximally from the distal face of cap **452**. Guide wire lumen **455** extends from the proximal end of bore **453** to the proximal end of cap **452**.

Handle **460** comprises proximal male screw thread **461** configured to engage female screw thread **454** of cap **452**, and lumen **462** configured to receive collet **456** in its proximal end and rod **464** in its distal end. Lumen **462** has a reduced diameter at the distal end of handle **460** that captures a step on the proximal end of rod **464**. Thus, while collet **456** is removable received within lumen **462**, rod **464** may translate and rotate within, but may not be removed from, lumen **462**. Guide wire **422** freely passes through collet **456** when screw cap **452** is not securely fastened to handle **460**. When cap **452** is securely fastened to handle **460**, it causes collet **456** to elastically deform, decreasing the diameter of the lumen extending through the collet, and frictionally locking guide wire **422** into rigid attachment with collet **456**. Guide wire **422** is thereby rigidly connected to handle **460**.

Rod **464** further comprises guide wire lumen **465** extending therethrough. Rod **464** has its distal end rigidly and permanently affixed to central screw cap **468**. Cap **468** comprises female screw thread **469** and lumen **470**. Lumen **470** includes a proximal reduced-diameter step that captures rod **464** within the proximal end of cap **468**, and a distal portion that receives lumen flushing or fluid port section **472**.

Section **472** comprises male screw thread **473**, side port **474**, bore **475**, guide wire lumen **476**, and fluid lumen **477**. Male screw thread **473** is configured to engage female thread **469** of cap **468**. Section **472** includes a flange disposed just distal of thread **473** that is captured within lumen **470** of cap **468**. Thus, cap **468** may be tightened onto and loosened from, but not removed from, section **472**.

Rod **464** is received within bore **475** of section **472**. Guide wire **22** passes between bore **475** and fluid lumen **477** within guide wire lumen **476**. Fluid lumen **477** connects side port **474** to the guide wire lumen of delivery sheath **40**. O-rings **478** provide a fluid seal at the distal end of lumen **477**.

Distal hub **479** connects section **472** to nose piece **486**. Hub **479** comprises bore **483**, female screw thread **484**, and annulus **485** containing tapered projection **481**. Bore **483** includes flange **482** that rotatably receives section **472** in its proximal end. Nose piece **486** comprises male screw thread **487**, tapered bore **488**, and delivery sheath lumen **489**. Male screw thread **487** is configured to engage female thread **484** in

annulus **485** of hub **479**. Tapered bore **488** allows tapered projection **481** of hub **479** to extend within nose piece **486** and permit delivery sheath **40** from delivery sheath lumen **489** to extend therethrough. O-rings **478** are disposed between the hub **479** and nose piece **486** and between hub **479** and section **472**.

Delivery system **450** advantageously may be implemented in a variety of ways. For example, the delivery system may be offered with a delivery catheter or sheath pre-attached. In this embodiment, proximal screw cap **452** is loosened, and the proximal end of guide wire **22** may be passed through the delivery catheter or sheath, and delivery system **450**, until vascular device **20** is in its retracted state within the delivery catheter or sheath. Insertion of the vascular device into the patient may then proceed. Alternatively, delivery system **450** may be commercially supplied in the configuration shown in FIG. **5A**, i.e., pre-loaded with a delivery catheter or sheath, such as sheath **40**, already attached and a vascular device, such as vascular device **20**, retracted therein. As another alternative, delivery system **450** may be offered without either a delivery sheath or vascular device attached, or the delivery catheter or sheath may be an interventional instrument, such as an angioplasty, atherectomy, or stent delivery catheter.

Referring again to FIGS. **5A-5D** in conjunction with FIGS. **21A** and **21B**, a method of using the delivery system of the present invention in conjunction with a vascular filter is described. With vascular device **20** contracted within distal end **42** of delivery sheath **40** (FIGS. **5A** and **21A**), delivery sheath **40** is attached to delivery system **450** by loosening proximal screw cap **452** and extending the proximal end of guide wire **22** through delivery system **450**, with handle **460** in its proximal-most position (FIG. **21A**). Screw cap **452** is then tightened to cause collet **456** to engage guide wire **22** to handle **460**.

Delivery sheath **40** then is advanced through a patient's vasculature using well-known percutaneous techniques using distal end **23** of guide wire **22**. If a vessel bifurcation is to be crossed during advancement, handle **460** may be rotated to divert the distal end of sheath **40** into the desired branch of the bifurcation. The rotational moment or torque applied to handle **460** is transmitted to guide wire **22** (when screw cap **452** is tightened), which causes distal end **23** to rotate and facilitates positioning of vascular device **20** in the proper side of the bifurcation. As shown in FIG. **5A**, advancement continues until delivery sheath **40** is disposed at a desired location within a patient's vessel **V**, such as a coronary or carotid artery, as determined, for example, by the position of radiopaque band **43** under a fluoroscope.

With the vascular device in position, handle **460**, and thus guide wire **22**, is held stationary while section **472** and attached delivery sheath **40** are retracted proximally. Alternatively, handle **460** may be advanced while section **472** and sheath **40** are held stationary. In either case, when vascular device **20** is no longer confined within delivery sheath **40**, support hoop **24** expands to seal against the walls of the vessel **V**, as depicted in FIGS. **5B** and **21B**. Blood continues to flow unimpeded through vessel **V** in direction **A**.

Depending on the medical procedure prescribed in conjunction with the use of vascular device **20**, delivery sheath **40** may retrieve vascular device **20** at the conclusion of the procedure, or sheath **40** may be detached from delivery system **450** and removed from the patient. If sheath **40** is detached, guide wire **22** may be removed from delivery system **450** so that other interventional instruments, such as angioplasty catheters, atherectomy devices, or stent delivery systems may be advanced along guide wire **22** to position such devices at treatment zones located proximally of vascu-

lar device **20**. Guide wire **22** and the interventional catheter then may be passed through and fastened to delivery system **450**. For example, as shown in FIG. **5C**, angioplasty balloon catheter **44** may be advanced along guide wire **22** to a position proximal of vascular device **20** so that device **20** may trap emboli E, i.e., pieces of plaque dislodged from the walls of vessel V by balloon **46**.

Upon completion of the angioplasty procedure using angioplasty balloon catheter **44**, handle **460** with attached guide wire **22** is pulled proximally to cause the sides of support hoop **24** to collapse together to close the mouth of sac **28** (FIG. **3**). Additional proximal retraction of guide wire **22** causes support hoop **24** and sac **28** to enter at least partially within the guide wire lumen of angioplasty catheter **44**. As depicted in FIG. **4D**, only a portion of support hoop **24**, near articulation region **26**, and a distal portion of sac **28** extend out of the guide wire lumen of angioplasty catheter **44**. Angioplasty catheter **44** then is withdrawn with vascular device **20** and any trapped emboli E.

It also may be beneficial during a medical procedure to introduce or withdraw fluids from the operative site. For example, it may be beneficial to deliver medicaments, or draw suction to remove blood. The delivery sheath lumen also may require flushing with saline to prevent clotting within the lumen. These and other procedures are made possible by side port **474** of section **472**, which, as described hereinabove, is in fluid communication with the lumen of delivery sheath **40**.

In addition to applications with vascular filters, delivery system **450** may be used as part of the thrombectomy/embolectomy procedure described herein above, as well as in a variety of other procedures.

Embodiments of the present invention may optionally be used in conjunction with a specially configured retrieval sheath. Applicant has determined that bunching of sac **28** in FIG. **5D** may occur during retraction into catheter **44**, resulting in a retrieval profile that may be difficult to navigate through a patient's vasculature. However, additional proximal retraction of guide wire **22** in an attempt to decrease the profile of sac **28** may generate stress loads sufficient to tear sac **28** and release captured emboli.

With reference to FIGS. **22A-22E**, a specially configured retrieval sheath and methods of use with the vascular device of the present invention are described. As with FIGS. **5**, sizes have been exaggerated to illustrate structure. In FIG. **22A**, guide wire **556** is positioned within vessel V using well-known percutaneous techniques. Vascular device **550** is disposed in its contracted delivery state within distal end **554** of delivery sheath **552**. Retrieval sheath **560** and guide catheter **562** are advanced over delivery sheath **552** to a position located just proximal of distal end **554**.

Retrieval sheath **560** includes collapsible flared end region **564**, which is shown in a contracted delivery state within catheter **562** in FIG. **22A**. Flared end region **564** has a deployed state, wherein the wall flares outward to form a frustrum of a cone, and a contracted state, wherein the wall is substantially cylindrical. Flared end region **564** preferably includes radiopaque band **566**.

With respect to FIG. **22B**, once delivery sheath **552** is disposed at a desired location within a patient's vessel V, guide wire **556** is held stationary while delivery sheath **552** is retracted proximally. Alternatively, delivery sheath **552** may be held stationary while guide wire **556** is advanced. In either case, when vascular device **550** is no longer confined within delivery sheath **552**, support hoop **568** and attached blood permeable sac **570**, expands to seal against the walls of the vessel V. Sac **570** further comprises radiopaque band **572**. When in the deployed state, the curved regions of support

hoop orient its articulation region concentrically against the inside wall of the vessel. Blood continues to flow unimpeded through vessel V in direction A.

With vascular device **550** deployed, an interventional procedure is performed proximal of the device. For example, guide catheter **562** may be an angioplasty balloon catheter similar to catheter **44** of FIGS. **5C** and **5D**. The interventional procedure generates emboli E proximal of device **550**, which travel downstream and are captured in sac **570**.

With respect to FIG. **22C**, upon completion of the interventional procedure, guide wire **556** is pulled proximally to cause the sides of support hoop **568** to collapse together to close the mouth of sac **570** (see FIG. **3**). Additional proximal retraction of guide wire **556** causes support hoop **568** and sac **570** to partially enter within distal end **554** of delivery sheath **552**. If bunching of the sac is anticipated or suspected, flared sheath **560** may be advanced distally to expand end region **564**, which comprises a suitable elastomeric material, such as latex, rubber, or a synthetic variant thereof.

As depicted in FIG. **22D**, delivery sheath **552** is retracted proximally while retrieval sheath **560** is held stationary, until radiopaque bands **572** and **566** are concentrically aligned, as determined, for example, with a fluoroscope. Then, as illustrated in FIG. **22E**, sheaths **552** and **560** are simultaneously withdrawn proximally while guide catheter **562** is held stationary. This motion causes flared end region **564** to collapse sac **570** to its contracted state. In so doing, flared end region **564** applies a distributed load over the surface of sac **570**, thereby decreasing the retrieval profile of sac **570** with reduced risk of rupture of sac **570**.

Vascular device **550** also may be used in performing thrombectomy/embolectomy. In this case, vascular device **550** is advanced in its retracted state within delivery sheath **552** to a location distal of a lesion. Delivery sheath **552** is withdrawn proximally, and vascular device **550** is deployed. With support hoop **568** in contact with the vessel wall, vascular device **550** may be retracted proximally to scrape along the wall of the vessel and excise thrombus so that it is captured in sac **570**. Delivery sheath **552**, as well as flared sheath **560** and guide catheter **562**, then may be reinserted into the vessel along guide wire **556**, and vascular device **550** may be retracted and removed from the vessel in the manner described hereinabove.

With reference to FIGS. **23A** and **23B**, an alternative embodiment of the specially configured retrieval sheath, and methods of use with the vascular device of the present invention, are described. Again, sizes have been exaggerated to illustrate structure. In FIG. **23A**, guide wire **582** has been positioned within vessel V using well-known percutaneous techniques. Vascular device **580** has been expanded to its deployed state after delivery within delivery sheath **584**, in the manner discussed hereinabove. Support hoop **586** seals against the walls of vessel V, and blood permeable sac **588** is positioned to capture emboli E generated by, for example, an upstream interventional procedure. Blood continues to flow unimpeded through vessel V in direction A.

Delivery sheath **584** further comprises atraumatic expander **590** disposed on a distal end. Retrieval sheath **592** is advanced over delivery sheath **584** to a position located just proximal of expander **590**. Retrieval sheath **592** includes expandable end region **594**, which is shown in a contracted delivery state in FIG. **23A**. Expandable end region **594** has a deployed state, wherein the wall flares outward to form a frustrum of a cone, and a contracted state, wherein the wall is substantially cylindrical. Expander **590** has a larger maximum diameter than end region **594**. Expandable end region **594** preferably includes radiopaque band **596**, while expander

590 preferably includes radiopaque band **598** so that their positions relative to one another may be accurately determined.

With respect to FIG. **23B**, upon completion of the interventional procedure, guide wire **582** is pulled proximally to cause the sides of support hoop **586** to collapse together to close the mouth of sac **588** (see FIG. **3**). Additional proximal retraction of guide wire **582** causes support hoop **586** and sac **588** to partially enter within the distal end of delivery sheath **584**.

If bunching of the sac is anticipated or suspected, delivery sheath **584** may be retracted proximally while retrieval sheath **592** is held stationery to expand end region **594** of retrieval sheath **592** with expander **590**. Delivery sheath **584** is retracted a sufficient distance to protect sac **588** and its embolic contents within end region **594**. The distance may be determined by means of radiopaque bands **596** and **598**. End region **594** comprises a suitable elastomeric material, such as latex, rubber or a synthetic variant thereof.

The profile of end region **594** in the expanded state allows for retraction of retrieval sheath **592**, as well as delivery sheath **584** and vascular device **580** disposed therein, in a manner that mitigates dangerous interaction with the vascular wall. It also allows vascular device **580** to be retrieved in a partially collapsed state that reduces the risk of sac **588** tearing. As with vascular device **550**, vascular device **580** may be used in performing thrombectomy/embolectomy.

The support hoops depicted herein illustratively are shown as oval or heart-shaped in the deployed state, where the shape is exaggerated for the sake of clarity. In preferred embodiments, the support hoops are substantially round when deployed, to ensure contact around the circumference of the support hoop and provide a positive seal against the arterial wall.

Although preferred illustrative embodiments of the present invention are described above, it will be evident to one skilled in the art that various changes and modifications may be made without departing from the invention. It is intended in the appended claims to cover all such changes and modifications that fall within the true spirit and scope of the invention.

What is claimed is:

[1. Apparatus suitable for filtering emboli or performing thrombectomy, embolectomy or foreign body removal, comprising:

an elongated member having a distal region;

a first support hoop attached to the distal region, the first support hoop having an articulation region interposed between curved regions;

a blood permeable sac affixed to the first support hoop so that the first support hoop forms a mouth of the blood permeable sac;

wherein the apparatus has a deployed state, wherein the first support hoop engages an interior wall of a patient's vessel, and a delivery state, wherein the apparatus has a contracted configuration to permit insertion within a delivery sheath; and

wherein the first support hoop is folded at the articulation region when the apparatus is in the delivery state.]

[2. The apparatus of claim **1**, wherein the blood permeable sac comprises a biocompatible material.]

[3. The apparatus of claim **2**, wherein the biocompatible material comprises a material chosen from a group consisting of polyethylene, polypropylene, polyurethane, polyester, polyethylene tetrphthalate, nylon and polytetrafluoroethylene.]

[4. The apparatus of claim **2**, wherein the biocompatible material is substantially non-thrombogenic.]

[5. The apparatus of claim **2**, wherein the biocompatible material is formed into the blood permeable sac by a thermoforming process.]

[6. The apparatus of claim **1**, wherein the blood permeable sac comprises a woven material having a plurality of pores, the pores having a size determined by a weave pattern of the woven material.]

[7. The apparatus of claim **4**, wherein each one of the plurality of pores has a diameter in a range of 20 to 400 microns.]

[8. The apparatus of claim **4**, wherein each one of the plurality of pores has a cross-sectional area, and a sum area of the cross-sectional areas is greater than or equal to a cross-sectional area of a patient's vessel.]

[9. The apparatus of claim **1**, wherein the first support hoop comprises a super-elastic material.]

[10. The apparatus of claim **6**, wherein the super-elastic material comprises a nickel-titanium alloy.]

[11. The apparatus of claim **6**, wherein the super-elastic material comprises a spring tempered stainless steel.]

[12. The apparatus of claim **1**, wherein the first support hoop comprises a wire having a thickness that tapers to a minimum thickness at the articulation region.]

[13. The apparatus of claim **1**, wherein the mouth of the blood permeable sac is closed when the apparatus is in the contracted configuration, thereby preventing emboli from escaping from the blood permeable sac.]

[14. The apparatus of claim **11** wherein opposite sides of the first support hoop close towards one another when the apparatus is contracted to its contracted configuration.]

[15. The apparatus of claim **1**, wherein the first support hoop comprises a radiopaque feature. member.]

[16. The apparatus of claim **13**, wherein the radiopaque feature comprises a radiopaque wire wrapped around the first support hoop.]

[17. The apparatus of claim **1**, wherein the blood permeable sac is affixed to the elongated member along a length of the blood permeable sac.]

[18. The apparatus of claim **1** wherein the first support hoop includes one or more side turns that stabilize and orient the apparatus in the deployed state.]

[19. The apparatus of claim **1** wherein the elongated member serves as a guide wire.]

[20. The apparatus of claim **1** further comprising:
a nose cone disposed on the distal region of the elongated member distal to the first support hoop; and
a delivery sheath having a first lumen for accepting the elongated member, first support hoop and blood permeable sac.]

[21. The apparatus of claim **17**, wherein the delivery sheath further comprises a second lumen for accepting a guide wire.]

[22. The apparatus of claim **18** wherein the first lumen of the delivery sheath opens to a skive in a lateral wall of the delivery sheath in a distal region of the delivery sheath.]

[23. The apparatus of claim **18** wherein the second lumen of the delivery sheath opens to a skive in a lateral wall of the delivery sheath in a distal region of the delivery sheath.]

[24. The apparatus of claim **18**, wherein the delivery sheath further comprises a guide tube attached to an exterior surface of the delivery sheath, the guide tube having a portion defining the second lumen.]

[25. The apparatus of claim **17** further comprising a guide wire in communication with the delivery sheath.]

[26. The apparatus of claim **23**, wherein a distal end of the guide wire is attached to a proximal end of the delivery sheath.]

25

[27. The apparatus of claim 1 further comprising a balloon catheter.]

[28. The apparatus of claim 1, wherein the articulation region comprises a gap, the gap bridged by a portion of the blood permeable sac.]

[29. The apparatus of claim 25, wherein the proximal end of the blood permeable sac comprises a lumen.]

[30. The apparatus of claim 29, wherein the lumen is configured to receive the curved regions and bridge the gap.]

[31. The apparatus of claim 25, wherein the curved regions of the first support hoop comprise an elastic material.]

[32. The apparatus of claim 1, wherein the blood permeable sac is further affixed to the elongated member.]

[33. The apparatus of claim 1, wherein the blood permeable sac has a length and a diameter that tapers along the length.]

[34. The apparatus of claim 29, wherein tapering the blood permeable sac reduces bunching of the sac during retrieval within a delivery sheath.]

[35. The apparatus of claim 29, wherein tapering the blood permeable sac reduces a delivery profile of the apparatus.]

[36. The apparatus of claim 29, wherein tapering the blood permeable sac reduces a risk of snagging the sac on a stent during retrieval.]

[37. The apparatus of claim 1, wherein the first support hoop is attached to a sheath slidably disposed on the elongated member.]

[38. The apparatus of claim 33 further comprising means for constraining longitudinal motion of the sheath with respect to the elongated member.]

[39. The apparatus of claim 1 further comprising a second support hoop disposed circumferentially adjacent to the first support hoop, the blood permeable sac further affixed to the second support hoop.]

40. [The apparatus of claim 1 further comprising:] *Apparatus suitable for filtering emboli or performing thrombectomy, embolectomy or foreign body removal, comprising:*

an elongated member having a distal region;

a first support hoop attached to the distal region, the first support hoop having an articulation region interposed between curved regions;

a blood permeable sac affixed to the first support hoop so that the first support hoop forms a mouth of the blood permeable sac;

wherein the apparatus has a deployed state, wherein the first support hoop engages an interior wall of a patient's vessel, and a delivery state, wherein the apparatus has a contracted configuration to permit insertion within a delivery sheath;

wherein the first support hoop is folded at the articulation region when the apparatus is in the delivery state; and a second support hoop coupled to the distal region and spaced apart longitudinally from the first support hoop, the blood permeable sac further affixed to the second support hoop.

41. The apparatus of claim [36] 40, wherein the second support hoop comprises a wire having a thickness that tapers to a minimum thickness at an articulation region.

42. The apparatus of claim [36] 40, wherein the blood permeable sac has a length and a diameter that tapers along the length.

43. The apparatus of claim [36] 40, wherein the second support hoop is smaller than the first support hoop.

44. The apparatus of claim [36] 40, wherein the second support hoop comprises an articulation region having a gap, the gap bridged by a portion of the blood permeable sac.

26

45. The apparatus of claim [36] 40, wherein the first and second support hoops are attached to a sheath slidably disposed on the elongated member.

46. The apparatus of claim [41] 45, further comprising means for constraining longitudinal motion of the sheath with respect to the elongated member.

47. The apparatus of claim [1] 40, further comprising: a delivery sheath having a lumen for accepting the elongated member, support hoop and blood permeable sac; a retrieval sheath having a flared end region and a lumen for accepting the delivery sheath; and a guide catheter having a lumen for accepting the retrieval sheath.

48. The apparatus of claim [43] 47, wherein the apparatus has a deployed state, wherein the support hoop engages an interior wall of a patient's vessel, and a delivery state, wherein the apparatus has a contracted configuration to permit insertion within the delivery sheath.

49. The apparatus of claim [44] 48, wherein the first support hoop folds at the articulation region when the apparatus is contracted to the delivery state.

50. The apparatus of claim [44] 48, wherein the mouth of the blood permeable sac closes when the apparatus is contracted to the delivery state.

51. The apparatus of claim [43] 47, wherein the flared end region comprises a radiopaque feature.

52. The apparatus of claim [43] 47, wherein the retrieval sheath has a deployed state, wherein the flared end region extends distal of the guide catheter and is expanded, and a contracted state, wherein the flared end region is collapsed to fit within the guide catheter lumen.

53. The apparatus of claim [48] 52, wherein the retrieval sheath is retracted from the deployed state to the contracted state when a radiopaque feature on the flared end region is aligned with a radiopaque feature on the blood permeable sac.

54. The apparatus of claim [48] 52, wherein the flared end region contracts the portion of the vascular device remaining in the deployed state within the guide catheter lumen when the retrieval sheath is retracted from the deployed state to the contracted state.

55. The apparatus of claim [43] 47, wherein the flared end region comprises an elastomeric material.

56. [The apparatus of claim 1 further comprising:] *Apparatus suitable for filtering emboli or performing thrombectomy, embolectomy or foreign body removal, comprising:*

an elongated member having a distal region;

a first support hoop attached to the distal region, the first support hoop having an articulation region interposed between curved regions;

a blood permeable sac affixed to the first support hoop so that the first support hoop forms a mouth of the blood permeable sac;

wherein the apparatus has a deployed state, wherein the first support hoop engages an interior wall of a patient's vessel, and a delivery state, wherein the apparatus has a contracted configuration to permit insertion within a delivery sheath;

wherein the first support hoop is folded at the articulation region when the apparatus is in the delivery state;

a delivery sheath having a lumen for accepting the elongated member, support hoop and blood permeable sac, and having an atraumatic expander; and a retrieval sheath having an expandable end region and a lumen for accepting the delivery sheath.

27

[57. The apparatus of claim 1 further comprising:
 a handle having a collet for selectively grasping and releasing the elongated member;
 and a lumen flushing section coupled to the handle to allow translation and rotation therebetween, the lumen flushing section having a side port in fluid communication with the lumen of the delivery sheath and configured to allow the elongated member to pass therethrough to the handle.]

[58. The apparatus of claim 53, wherein the apparatus has a delivery state, wherein the handle is translated longitudinally to a proximal-most position relative to the lumen flushing section, and the first support hoop is retracted within the delivery sheath, and a deployed state wherein the handle is translated longitudinally to a distal-most position adjacent the lumen flushing section, wherein the first support hoop extends beyond a distal end of the delivery sheath and engages an interior wall of a patient's vessel.]

[59. The apparatus of claim 1 further comprising:
 a handle configured to selectively grasp and release the elongated member; and
 a fluid port section coupled to the handle to allow translation and rotation therebetween, the fluid port section having a side port in fluid communication with the lumen of the delivery sheath and configured to allow the elongated member to pass therethrough to the handle.]

[60. The apparatus of claim 55, wherein the apparatus has a delivery state, wherein the handle is translated longitudinally to a proximal-most position relative to the fluid port section, and the first support hoop is retracted within the delivery sheath, and a deployed state wherein the handle is translated longitudinally to a distal-most position adjacent the fluid port section, wherein the first support hoop extends

28

beyond a distal end of the delivery sheath and engages an interior wall of a patient's vessel.]

61. The apparatus of claim [1] 56, further comprising:
 a thrombus removal element disposed proximal of the first support hoop, the thrombus removal element movable in a proximal direction independent of the elongated member.

62. The apparatus of claim [57] 61, wherein the thrombus removal element comprises a third support hoop with blood permeable sac.

63. The apparatus of claim [58] 62, wherein the third support hoop is slidably disposed on the elongated member.

64. The apparatus of claim [57] 61, wherein the removal element is configured to excise or ablate thrombus from within a patient's vessel.

65. The apparatus of claim [57] 61, further comprising:
 a nose cone disposed on the distal region of the elongated member distal to the support hoop;
 and a delivery sheath having a lumen for accepting the elongated member, thrombus removal element, first support hoop, and blood permeable sac.

66. The apparatus of claim [1] 40, wherein the blood permeable sac comprises a plurality of pores formed by laser drilling.

67. The apparatus of claim [62] 66, wherein each one of the plurality of pores has a diameter in a range of 20 to 400 microns.

68. The apparatus of claim [1] 40, wherein the blood permeable sac comprises a plurality of elliptical pores.

69. The apparatus of claim [1] 40, wherein the blood permeable sac comprises a plurality of pores provided in sufficient density, such that proximal pores remain open when distal pores become occluded, thereby ensuring continuous blood flow through a patient's vessel.

* * * * *