

US00RE43952E

(19) **United States**
(12) **Reissued Patent**
Uhl et al.

(10) **Patent Number:** **US RE43,952 E**
(45) **Date of Reissued Patent:** **Jan. 29, 2013**

(54) **INTERACTIVE SYSTEM FOR LOCAL INTERVENTION INSIDE A NON-HOMOGENEOUS STRUCTURE**

(75) Inventors: **Jean Francois Uhl**, Paris (FR); **Joel Henrion**, Suippes (FR); **Michel Scriban**, Ternay (FR); **Jean-Baptiste Thiebaut**, Paris (FR)

(73) Assignee: **Medtronic Navigation, Inc.**, Louisville, CO (US)

(21) Appl. No.: **09/784,829**

(22) Filed: **Feb. 8, 2001**

Related U.S. Patent Documents

Reissue of:

(64) Patent No.: **5,868,675**
Issued: **Feb. 9, 1999**
Appl. No.: **07/847,059**
PCT Filed: **Oct. 5, 1990**
PCT No.: **PCT/FR90/00714**
§ 371 (c)(1),
(2), (4) Date: **Jun. 22, 1992**
PCT Pub. No.: **WO91/04710**
PCT Pub. Date: **Apr. 18, 1991**

(30) **Foreign Application Priority Data**

Oct. 5, 1989 (FR) 89 13028

(51) **Int. Cl.**
A61B 19/00 (2006.01)

(52) **U.S. Cl.** **600/424; 600/425; 600/426; 600/427; 606/130**

(58) **Field of Classification Search** **600/407, 600/411, 415, 417, 424, 425, 426, 427; 606/130; 378/4, 20, 41, 58, 205; 901/6, 16, 41**

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,576,781 A 3/1926 Phillips
1,735,726 A 11/1929 Bornhardt
2,407,845 A 9/1946 Nemeyer
(Continued)

FOREIGN PATENT DOCUMENTS

CA 964149 3/1975
(Continued)

OTHER PUBLICATIONS

Adams et al., "Orientation Aid for Head and Neck Surgeons," Innov. Tech. Biol. Med., vol. 13, No. 4, 1992, pp. 409-424.

(Continued)

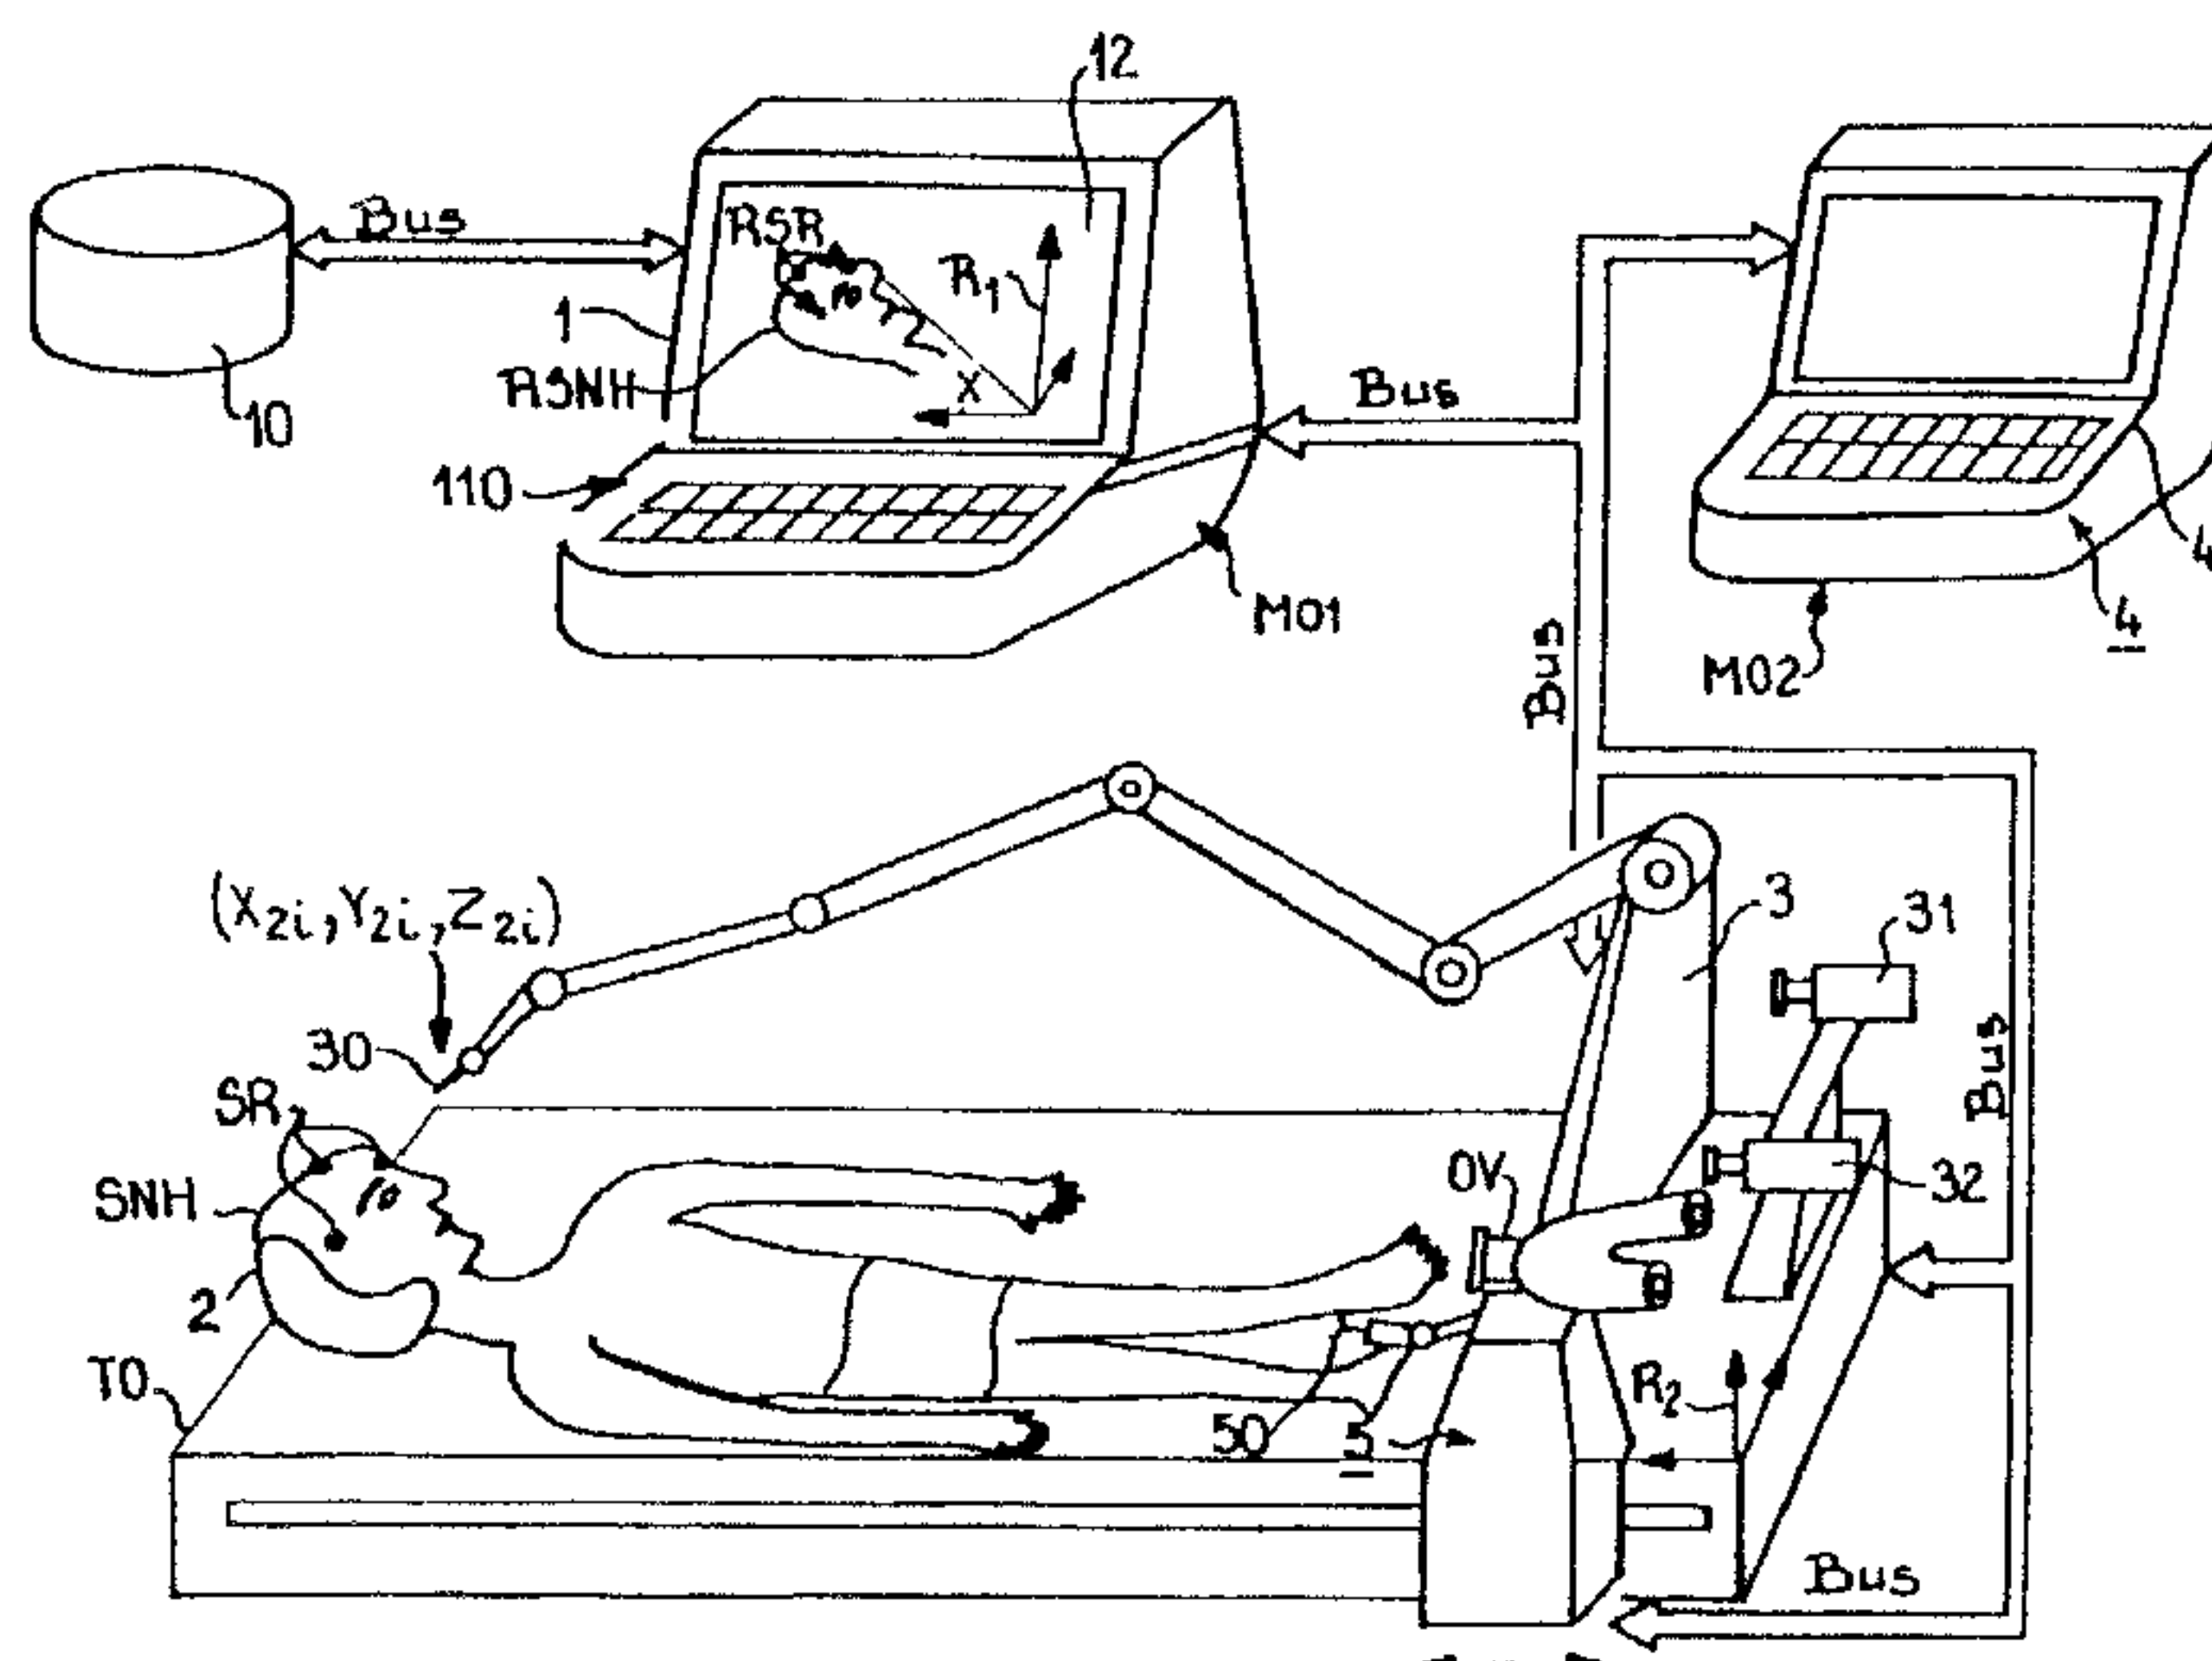
Primary Examiner — Ruth S Smith

(74) *Attorney, Agent, or Firm* — Harness, Dickey

(57) **ABSTRACT**

An interactive system for a local intervention inside a region of a non-homogeneous structure, such as the skull of a patient, which is related to the frame of reference (R_2) of an operation table, and which is connected to a reference structure comprising a plurality of base points. The system creates on a screen a representation of the non-homogeneous structure and of the reference structure connected thereto, provides the coordinates of the images of the base points in the first frame of reference (R_1), allows the marking of the coordinates of the base points in R_2 , and allows the carrying out of the local intervention with an active member such as a trephining tool, a needle, or a radioactive or chemical implant. The systems also optimizes the transfer of reference frames between R_1 and R_2 , from the coordinates of the base points in R_2 and the images in R_1 by reducing down to a minimum the deviations between the coordinates of images in R_1 and the base points in R_1 after transfer. The system also establishes real time bi-directional coupling between: (1) an origin and a direction of intervention simulated on the screen, (2) the position of the active member.

101 Claims, 13 Drawing Sheets



US RE43,952 E

Page 2

U.S. PATENT DOCUMENTS					
2,650,588 A	9/1953	Drew	4,706,665 A	11/1987	Gouda
2,697,433 A	12/1954	Sehnder	4,709,156 A	11/1987	Murphy et al.
3,016,899 A	1/1962	Stenvall	4,710,708 A	12/1987	Rorden et al.
3,017,887 A	1/1962	Heyer	4,719,419 A	1/1988	Dawley
3,061,936 A	11/1962	Dobbeleer	4,722,056 A	1/1988	Roberts et al.
3,073,310 A	1/1963	Mocarski	4,722,336 A	2/1988	Kim et al.
3,109,588 A	11/1963	Polhemus et al.	4,723,544 A	2/1988	Moore et al.
3,294,083 A	12/1966	Alderson	4,727,565 A	2/1988	Ericson
3,367,326 A	2/1968	Frazier	RE32,619 E	3/1988	Damadian
3,439,256 A	4/1969	Kähne et al.	4,733,969 A	3/1988	Case et al.
3,577,160 A	5/1971	White	4,737,032 A	4/1988	Addleman et al.
3,614,950 A	10/1971	Rabey	4,737,794 A	4/1988	Jones
3,644,825 A	2/1972	Davis, Jr. et al.	4,737,921 A	4/1988	Goldwasser et al.
3,674,014 A	7/1972	Tillander	4,742,356 A	5/1988	Kuipers
3,702,935 A	11/1972	Carey et al.	4,742,815 A	5/1988	Ninan et al.
3,704,707 A	12/1972	Halloran	4,743,770 A	5/1988	Lee
3,821,469 A	6/1974	Whetstone et al.	4,743,771 A	5/1988	Sacks et al.
3,868,565 A	2/1975	Kuipers	4,745,290 A	5/1988	Frankel et al.
3,941,127 A	3/1976	Froning	4,750,487 A	6/1988	Zanetti
3,983,474 A	9/1976	Kuipers	4,753,528 A	6/1988	Hines et al.
4,017,858 A	4/1977	Kuipers	4,761,072 A	8/1988	Pryor
4,037,592 A	7/1977	Kronner	4,764,016 A	8/1988	Johansson
4,052,620 A	10/1977	Brunnett	4,771,787 A	9/1988	Wurster et al.
4,054,881 A	10/1977	Raab	4,779,212 A	10/1988	Levy
4,117,337 A	9/1978	Staats	4,782,239 A	11/1988	Hirose et al.
4,173,228 A	11/1979	Van Steenwyk et al.	4,788,481 A	11/1988	Niwa
4,182,312 A	1/1980	Mushabac	4,791,934 A	12/1988	Brunett
4,197,855 A *	4/1980	Lewin 600/409	4,793,355 A	12/1988	Crum et al.
4,202,349 A	5/1980	Jones	4,794,262 A	12/1988	Sato et al.
4,228,799 A	10/1980	Anichkov et al.	4,797,907 A	1/1989	Anderton
4,256,112 A	3/1981	Kopf et al.	4,803,976 A	2/1989	Frigg et al.
4,262,306 A	4/1981	Renner	4,804,261 A	2/1989	Kirschen
4,287,809 A	9/1981	Egli et al.	4,805,615 A	2/1989	Carol
4,298,874 A	11/1981	Kuipers	4,809,694 A	3/1989	Ferrara
4,314,251 A	2/1982	Raab	4,821,200 A	4/1989	Öberg
4,317,078 A	2/1982	Weed et al.	4,821,206 A	4/1989	Arora
4,319,136 A	3/1982	Jenkins	4,821,731 A	4/1989	Martinelli et al.
4,328,548 A	5/1982	Crow et al.	4,822,163 A	4/1989	Schmidt
4,328,813 A	5/1982	Ray	4,825,091 A	4/1989	Breyer et al.
4,339,953 A	7/1982	Iwasaki	4,829,373 A	5/1989	Leberl et al.
4,341,220 A	7/1982	Perry	4,836,778 A	6/1989	Baumrind et al.
4,346,384 A	8/1982	Raab	4,838,265 A	6/1989	Cosman et al.
4,358,856 A	11/1982	Stivender et al.	4,841,967 A	6/1989	Chang et al.
4,368,536 A	1/1983	Pfeiler	4,845,771 A	7/1989	Wislocki et al.
4,396,885 A	8/1983	Constant	4,849,692 A	7/1989	Blood
4,396,945 A	8/1983	DiMatteo et al.	4,860,331 A	8/1989	Williams et al.
4,403,321 A	9/1983	DiMarco	4,862,893 A	9/1989	Martinelli
4,418,422 A	11/1983	Richter et al.	4,869,247 A	9/1989	Howard, III et al.
4,419,012 A	12/1983	Stephenson et al.	4,875,165 A	10/1989	Fencil et al.
4,422,041 A	12/1983	Lienau	4,875,478 A	10/1989	Chen
4,431,005 A	2/1984	McCormick	4,884,566 A	12/1989	Mountz et al.
4,485,815 A	12/1984	Amplatz	4,889,526 A	12/1989	Rauscher et al.
4,506,676 A	3/1985	Duska	4,896,673 A	1/1990	Rose et al.
4,543,959 A	10/1985	Sepponen	4,905,698 A	3/1990	Strohl, Jr. et al.
4,548,208 A	10/1985	Niemi	4,923,459 A	5/1990	Nambu
4,571,834 A	2/1986	Fraser et al.	4,931,056 A	6/1990	Ghajar et al.
4,572,198 A	2/1986	Codrington	4,945,305 A	7/1990	Blood
4,583,538 A	4/1986	Onik et al.	4,945,914 A	8/1990	Allen
4,584,577 A	4/1986	Temple	4,951,653 A	8/1990	Fry et al.
4,608,977 A	9/1986	Brown	4,955,891 A	9/1990	Carol
4,613,866 A	9/1986	Blood	4,961,422 A	10/1990	Marchosky et al.
4,617,925 A	10/1986	Laitinen	4,977,655 A	12/1990	Martinelli
4,618,978 A	10/1986	Cosman	4,989,608 A	2/1991	Ratner
4,621,628 A	11/1986	Brudermann	4,991,579 A	2/1991	Allen
4,625,718 A	12/1986	Olerud et al.	5,002,058 A	3/1991	Martinelli
4,638,798 A	1/1987	Shelden et al.	5,005,592 A	4/1991	Cartmell
4,642,786 A	2/1987	Hansen	5,013,317 A	5/1991	Cole et al.
4,645,343 A	2/1987	Stockdale et al.	5,016,639 A	5/1991	Allen
4,649,504 A	3/1987	Krouglicof et al.	5,017,139 A	5/1991	Mushabac
4,651,732 A	3/1987	Frederick	5,027,818 A	7/1991	Bova et al.
4,653,509 A	3/1987	Oloff et al.	5,030,196 A	7/1991	Inoue
4,659,971 A	4/1987	Suzuki et al.	5,030,222 A	7/1991	Calandruccio et al.
4,660,970 A	4/1987	Ferrano	5,031,203 A	7/1991	Trecha
4,673,352 A	6/1987	Hansen	5,042,486 A	8/1991	Pfeiler et al.
4,688,037 A	8/1987	Krieg	5,047,036 A	9/1991	Koutrouvelis
4,701,049 A	10/1987	Beckmann et al.	5,050,608 A	9/1991	Watanabe et al.
4,705,395 A	11/1987	Hageniers	5,054,492 A	10/1991	Scribner et al.
4,705,401 A	11/1987	Addleman et al.	5,057,095 A	10/1991	Fabian
			5,059,789 A	10/1991	Salcudean

US RE43,952 E

Page 3

5,078,140 A	1/1992	Kwoh	5,325,728 A	7/1994	Zimmerman et al.
5,079,699 A	1/1992	Tuy et al.	5,325,873 A	7/1994	Hirschi et al.
5,086,401 A	2/1992	Glassman et al.	5,329,944 A	7/1994	Fabian et al.
5,094,241 A	3/1992	Allen	5,330,485 A	7/1994	Clayman et al.
5,097,839 A	3/1992	Allen	5,333,168 A	7/1994	Fernandes et al.
5,098,426 A	3/1992	Sklar et al.	5,353,795 A	10/1994	Souza et al.
5,099,845 A	3/1992	Besz et al.	5,353,800 A	10/1994	Pohndorf et al.
5,099,846 A	3/1992	Hardy	5,353,807 A	10/1994	DeMarco
5,105,829 A	4/1992	Fabian et al.	5,359,417 A	10/1994	Müller et al.
5,107,839 A	4/1992	Houdek et al.	5,368,030 A	11/1994	Zinreich et al.
5,107,843 A	4/1992	Aarnio et al.	5,371,778 A	12/1994	Yanof et al.
5,107,862 A	4/1992	Fabian et al.	5,375,596 A	12/1994	Twiss et al.
5,109,194 A	4/1992	Cantaloube	5,377,678 A	1/1995	Dumoulin et al.
5,119,817 A	6/1992	Allen	5,383,454 A	1/1995	Bucholz
5,142,930 A	9/1992	Allen et al.	5,385,146 A	1/1995	Goldreyer
5,143,076 A	9/1992	Hardy et al.	5,385,148 A	1/1995	Lesh et al.
5,152,288 A	10/1992	Hoenig et al.	5,386,828 A	2/1995	Owens et al.
5,160,337 A	11/1992	Cosman	5,389,101 A	2/1995	Heilbrun et al.
5,161,536 A	11/1992	Vikomerson et al.	5,391,199 A	2/1995	Ben-Haim
5,178,164 A	1/1993	Allen	5,394,457 A	2/1995	Leibinger et al.
5,178,621 A	1/1993	Cook et al.	5,394,875 A	3/1995	Lewis et al.
5,186,174 A	2/1993	Schlondorff et al.	5,397,329 A	3/1995	Allen
5,187,475 A	2/1993	Wagener et al.	5,398,684 A	3/1995	Hardy
5,188,126 A	2/1993	Fabian et al.	5,399,146 A	3/1995	Nowacki et al.
5,190,059 A	3/1993	Fabian et al.	5,400,384 A	3/1995	Fernandes et al.
5,193,106 A	3/1993	DeSena	5,402,801 A	4/1995	Taylor
5,197,476 A	3/1993	Nowacki et al.	5,408,409 A	4/1995	Glassman et al.
5,197,965 A	3/1993	Cherry et al.	5,409,497 A	4/1995	Siczek et al.
5,198,768 A	3/1993	Keren	5,413,573 A	5/1995	Koivukangas
5,198,877 A	3/1993	Schulz	5,417,210 A	5/1995	Funda et al.
5,207,688 A	5/1993	Carol	5,419,325 A	5/1995	Dumoulin et al.
5,211,164 A	5/1993	Allen	5,423,334 A	6/1995	Jordan
5,211,165 A	5/1993	Dumoulin et al.	5,425,367 A	6/1995	Shapiro et al.
5,211,176 A	5/1993	Ishiguro et al.	5,425,382 A	6/1995	Golden et al.
5,212,720 A	5/1993	Landi et al.	5,426,683 A	6/1995	O'Farrell, Jr. et al.
5,214,615 A	5/1993	Bauer	5,426,687 A	6/1995	Goodall et al.
5,219,351 A	6/1993	Teubner et al.	5,427,097 A	6/1995	Depp
5,222,499 A	6/1993	Allen et al.	5,429,132 A	7/1995	Guy et al.
5,224,049 A	6/1993	Mushabac	5,433,198 A	7/1995	Desai
5,228,442 A	7/1993	Imran	RE35,025 E	8/1995	Anderton
5,230,338 A	7/1993	Allen et al.	5,437,277 A	8/1995	Dumoulin et al.
5,230,623 A	7/1993	Guthrie et al.	5,443,066 A	8/1995	Dumoulin et al.
5,233,990 A	8/1993	Barnea	5,443,489 A	8/1995	Ben-Haim
5,237,996 A	8/1993	Waldman et al.	5,444,756 A	8/1995	Pai et al.
5,249,581 A	10/1993	Horbai et al.	5,445,144 A	8/1995	Wodicka et al.
5,251,127 A	10/1993	Raab	5,445,150 A	8/1995	Dumoulin et al.
5,251,635 A	10/1993	Dumoulin et al.	5,445,166 A	8/1995	Taylor
5,253,647 A	10/1993	Takahashi et al.	5,446,548 A	8/1995	Gerig et al.
5,255,680 A	10/1993	Darrow et al.	5,447,154 A	9/1995	Cinquin et al.
5,257,636 A	11/1993	White	5,448,610 A	9/1995	Yamamoto et al.
5,257,998 A	11/1993	Ota et al.	5,453,686 A	9/1995	Anderson
5,261,404 A	11/1993	Mick et al.	5,456,718 A	10/1995	Szymaitis
5,265,610 A	11/1993	Darrow et al.	5,457,641 A	10/1995	Zimmer et al.
5,265,611 A	11/1993	Hoenig et al.	5,458,718 A	10/1995	Venkitachalam
5,269,759 A	12/1993	Hernandez et al.	5,464,446 A	11/1995	Dreessen et al.
5,271,400 A	12/1993	Dumoulin et al.	5,469,847 A	11/1995	Zinreich et al.
5,273,025 A	12/1993	Sakiyama et al.	5,478,341 A	12/1995	Cook et al.
5,273,039 A	12/1993	Fujiwara et al.	5,478,343 A	12/1995	Ritter
5,274,551 A	12/1993	Corby, Jr.	5,480,422 A	1/1996	Ben-Haim
5,279,309 A	1/1994	Taylor et al.	5,480,439 A	1/1996	Bisek et al.
5,280,427 A	1/1994	Magnusson et al.	5,483,961 A	1/1996	Kelly et al.
5,285,787 A	2/1994	Machida	5,485,849 A	1/1996	Panescu et al.
5,291,199 A	3/1994	Overman et al.	5,487,391 A	1/1996	Panescu
5,291,889 A	3/1994	Kenet et al.	5,487,729 A	1/1996	Avellanet et al.
5,295,483 A	3/1994	Nowacki et al.	5,487,757 A	1/1996	Truckai et al.
5,297,549 A	3/1994	Beatty et al.	5,490,196 A	2/1996	Rudich et al.
5,299,253 A	3/1994	Wessels	5,494,034 A	2/1996	Schlondorff et al.
5,299,254 A	3/1994	Dancer et al.	5,503,416 A	4/1996	Aoki et al.
5,299,288 A	3/1994	Glassman et al.	5,513,637 A	5/1996	Twiss et al.
5,300,080 A	4/1994	Clayman et al.	5,514,146 A	5/1996	Lam et al.
5,305,091 A	4/1994	Gelbart et al.	5,515,160 A	5/1996	Schulz et al.
5,305,203 A	4/1994	Raab	5,517,990 A	5/1996	Kalfas et al.
5,306,271 A	4/1994	Zinreich et al.	5,531,227 A	7/1996	Schneider
5,307,072 A	4/1994	Jones, Jr.	5,531,520 A	7/1996	Grimson et al.
5,309,913 A	5/1994	Kormos et al.	5,542,938 A	8/1996	Avellanet et al.
5,315,630 A	5/1994	Sturm et al.	5,543,951 A	8/1996	Moehrmann
5,316,024 A	5/1994	Hirschi et al.	5,546,940 A	8/1996	Panescu et al.
5,318,025 A	6/1994	Dumoulin et al.	5,546,949 A	8/1996	Frazin et al.
5,320,111 A	6/1994	Livingston	5,546,951 A	8/1996	Ben-Haim

US RE43,952 E

Page 4

5,551,429 A	9/1996	Fitzpatrick et al.	5,776,064 A	7/1998	Kalfas et al.
5,558,091 A	9/1996	Acker et al.	5,782,765 A	7/1998	Jonkman
5,566,681 A	10/1996	Manwaring et al.	5,787,886 A	8/1998	Kelly et al.
5,568,384 A	10/1996	Robb et al.	5,792,055 A	8/1998	McKinnon
5,568,809 A	10/1996	Ben-haim	5,795,294 A	8/1998	Luber et al.
5,572,999 A	11/1996	Fubda et al.	5,797,849 A	8/1998	Vesely et al.
5,573,533 A	11/1996	Strul	5,799,055 A	8/1998	Peshkin et al.
5,575,794 A	11/1996	Walus et al.	5,799,099 A	8/1998	Wang et al.
5,575,798 A	11/1996	Koutrouvelis	5,800,352 A	9/1998	Ferre et al.
5,583,909 A	12/1996	Hanover	5,800,535 A	9/1998	Howard, III
5,588,430 A	12/1996	Bova et al.	5,802,719 A	9/1998	O'Farrell, Jr. et al.
5,590,215 A	12/1996	Allen	5,803,089 A	9/1998	Ferre et al.
5,592,939 A	1/1997	Martinelli	5,807,252 A	9/1998	Hassfeld et al.
5,595,193 A	1/1997	Walus et al.	5,810,008 A	9/1998	Dekel et al.
5,596,228 A	1/1997	Anderton et al.	5,810,728 A	9/1998	Kuhn
5,600,330 A	2/1997	Blood	5,810,735 A	9/1998	Halperin et al.
5,603,318 A	2/1997	Heilbrun et al.	5,820,553 A	10/1998	Hughes
5,611,025 A	3/1997	Lorensen et al.	5,823,192 A	10/1998	Kalend et al.
5,617,462 A	4/1997	Spratt	5,823,958 A	10/1998	Truppe
5,617,857 A	4/1997	Chader et al.	5,828,725 A	10/1998	Levinson
5,619,261 A	4/1997	Anderton	5,828,770 A	10/1998	Leis et al.
5,622,169 A	4/1997	Golden et al.	5,829,444 A	11/1998	Ferre et al.
5,622,170 A	4/1997	Schulz	5,831,260 A	11/1998	Hansen
5,627,873 A	5/1997	Hanover et al.	5,833,608 A	11/1998	Acker
5,628,315 A	5/1997	Vilsmeier et al.	5,834,759 A	11/1998	Glossop
5,630,431 A	5/1997	Taylor	5,836,954 A	11/1998	Heilbrun et al.
5,636,644 A	6/1997	Hart et al.	5,840,024 A	11/1998	Taniguchi et al.
5,638,819 A	6/1997	Manwaring et al.	5,840,025 A	11/1998	Ben-Haim
5,640,170 A	6/1997	Anderson	5,843,076 A	12/1998	Webster, Jr. et al.
5,642,395 A	6/1997	Anderton et al.	5,848,967 A	12/1998	Cosman
5,643,268 A	7/1997	Vilsmeier et al.	5,851,183 A	12/1998	Bucholz
5,645,065 A	7/1997	Shapiro et al.	5,865,846 A	2/1999	Bryan et al.
5,646,524 A	7/1997	Gilboa	5,868,674 A	2/1999	Glowinski et al.
5,647,361 A	7/1997	Damadian	5,868,675 A	2/1999	Henrion et al.
5,662,111 A	9/1997	Cosman	5,871,445 A	2/1999	Bucholz
5,664,001 A	9/1997	Tachibana et al.	5,871,455 A	2/1999	Ueno
5,674,296 A	10/1997	Bryan et al.	5,871,487 A	2/1999	Warner et al.
5,676,673 A	10/1997	Ferre et al.	5,873,822 A	2/1999	Ferre et al.
5,681,260 A	10/1997	Ueda et al.	5,882,304 A	3/1999	Ehnholm et al.
5,682,886 A	11/1997	Delp et al.	5,884,410 A	3/1999	Prinz
5,682,890 A	11/1997	Kormos et al.	5,889,834 A	3/1999	Vilsmeier et al.
5,690,108 A	11/1997	Chakeres	5,891,034 A	4/1999	Bucholz
5,694,945 A	12/1997	Ben-Haim	5,891,157 A	4/1999	Day et al.
5,695,500 A	12/1997	Taylor et al.	5,904,691 A	5/1999	Barnett et al.
5,695,501 A	12/1997	Carol et al.	5,907,395 A	5/1999	Schultz et al.
5,697,377 A	12/1997	Wittkampf	5,913,820 A	6/1999	Bladen et al.
5,702,406 A	12/1997	Vilsmeier et al.	5,920,395 A	7/1999	Schulz
5,711,299 A	1/1998	Manwaring et al.	5,921,992 A	7/1999	Costales et al.
5,713,946 A	2/1998	Ben-Haim	5,923,727 A	7/1999	Navab
5,715,822 A	2/1998	Watkins	5,928,248 A	7/1999	Acker
5,715,836 A	2/1998	Kliegis et al.	5,938,603 A	8/1999	Ponzi
5,718,241 A	2/1998	Ben-Haim et al.	5,938,694 A	8/1999	Jaraczewski et al.
5,727,552 A	3/1998	Ryan	5,947,980 A	9/1999	Jensen et al.
5,727,553 A	3/1998	Saad	5,947,981 A	9/1999	Cosman
5,729,129 A	3/1998	Acker	5,950,629 A	9/1999	Taylor et al.
5,730,129 A	3/1998	Darrow et al.	5,951,475 A	9/1999	Gueziec et al.
5,730,130 A	3/1998	Fitzpatrick et al.	5,951,571 A	9/1999	Audette
5,732,703 A	3/1998	Kalfas et al.	5,954,647 A	9/1999	Bova et al.
5,735,278 A	4/1998	Hoult et al.	5,957,844 A	9/1999	Dekel et al.
5,738,096 A	4/1998	Ben-Haim	5,964,796 A	10/1999	Imran
5,740,802 A	4/1998	Nafis et al.	5,967,980 A	10/1999	Ferre et al.
5,741,214 A	4/1998	Ouchi et al.	5,967,982 A	10/1999	Barnett
5,742,394 A	4/1998	Hansen	5,968,047 A	10/1999	Reed
5,744,953 A	4/1998	Hansen	5,971,997 A	10/1999	Guthrie et al.
5,748,767 A	5/1998	Raab	5,976,156 A	11/1999	Taylor et al.
5,749,362 A	5/1998	Funda et al.	5,980,535 A	11/1999	Barnett et al.
5,749,835 A	5/1998	Glantz	5,983,126 A	11/1999	Wittkampf
5,752,513 A	5/1998	Acker et al.	5,987,349 A	11/1999	Schulz
5,755,725 A	5/1998	Druais	5,987,960 A	11/1999	Messner et al.
RE35,816 E	6/1998	Schulz	5,999,837 A	12/1999	Messner et al.
5,758,667 A	6/1998	Slettenmark	5,999,840 A	12/1999	Grimson et al.
5,762,064 A	6/1998	Polyani	6,001,130 A	12/1999	Bryan et al.
5,767,669 A	6/1998	Hansen et al.	6,006,126 A	12/1999	Cosman
5,767,960 A	6/1998	Orman	6,006,127 A	12/1999	Van Der Brug et al.
5,769,789 A	6/1998	Wang et al.	6,013,087 A	1/2000	Adams et al.
5,769,843 A	6/1998	Abela et al.	6,014,580 A	1/2000	Blume et al.
5,769,861 A	6/1998	Vilsmeier	6,016,439 A	1/2000	Acker
5,772,594 A	6/1998	Barrick	6,019,725 A	2/2000	Vesely et al.
5,775,322 A	7/1998	Silverstein et al.	6,024,695 A	2/2000	Taylor et al.

6,050,724	A	4/2000	Schmitz et al.	EP	0419729	A1	9/1989
6,059,718	A	5/2000	Taniguchi et al.	EP	0350996	A1	1/1990
6,063,022	A	5/2000	Ben-Haim	EP	0 651 968	A1	8/1990
6,071,288	A	6/2000	Carol et al.	EP	0 427 358		10/1990
6,073,043	A	6/2000	Schneider	EP	0 456 103		5/1991
6,076,008	A	6/2000	Bucholz	EP	0 581 704	B1	7/1993
6,096,050	A	8/2000	Audette	EP	0655138	B1	8/1993
6,104,944	A	8/2000	Martinelli	EP	0894473	A2	1/1995
6,118,845	A	9/2000	Simon et al.	EP	0 908 146		10/1998
6,122,538	A	9/2000	Sliwa, Jr. et al.	EP	0 930 046		10/1998
6,122,541	A	9/2000	Cosman et al.	FR	2417970		2/1979
6,131,396	A	10/2000	Duerr et al.	GB	2 094 590		2/1982
6,139,183	A	10/2000	Graumann	GB	2 164 856		10/1984
6,147,480	A	11/2000	Osadchy et al.	JP	61-94639		10/1984
6,149,592	A	11/2000	Yanof et al.	JP	62-327		6/1985
6,156,067	A	12/2000	Bryan et al.	JP	63-240851		3/1987
6,161,032	A	12/2000	Acker	JP	3-267054		3/1990
6,165,181	A	12/2000	Heilbrun et al.	WO	FR 2 618 211		7/1987
6,167,296	A	12/2000	Shahidi	WO	0009151		12/1988
6,172,499	B1	1/2001	Ashe	WO	WO 88/09151		12/1988
6,175,756	B1	1/2001	Ferre et al.	WO	WO 89/05123		6/1989
6,178,345	B1	1/2001	Vilsmeier et al.	WO	WO 90/05494		11/1989
6,194,639	B1	2/2001	Botella et al.	WO	WO 91/03982		4/1991
6,201,387	B1	3/2001	Govari	WO	WO 91/04711		4/1991
6,203,497	B1	3/2001	Dekel et al.	WO	WO 91/07726		5/1991
6,211,666	B1	4/2001	Acker	WO	WO 92/03090		3/1992
6,223,067	B1	4/2001	Vilsmeier	WO	WO 92/06645		4/1992
6,233,476	B1	5/2001	Strommer et al.	WO	WO 94/04938		3/1994
6,246,231	B1	6/2001	Ashe	WO	WO 95/07055		9/1994
6,259,942	B1	7/2001	Westermann et al.	WO	WO 94/23647		10/1994
6,273,896	B1	8/2001	Franck et al.	WO	WO 94/24933		11/1994
6,285,902	B1	9/2001	Kienzle, III et al.	WO	WO 96/32059		11/1995
6,298,262	B1	10/2001	Franck et al.	WO	WO 96/11624		4/1996
6,314,310	B1	11/2001	Ben-Haim et al.	WO	WO 97/49453		6/1997
6,332,089	B1	12/2001	Acker et al.	WO	WO 97/36192		10/1997
6,341,231	B1	1/2002	Ferre et al.	WO	WO 99/23956		11/1997
6,351,659	B1	2/2002	Vilsmeier	WO	WO 98/08554		3/1998
6,381,485	B1	4/2002	Hunter et al.	WO	WO 98/38908		9/1998
6,424,856	B1	7/2002	Vilsmeier et al.	WO	WO 99/15097		9/1998
6,427,314	B1	8/2002	Acker	WO	WO 99/21498		10/1998
6,428,547	B1	8/2002	Vilsmeier et al.	WO	WO 99/27839		12/1998
6,434,415	B1	8/2002	Foley et al.	WO	WO 99/33406		12/1998
6,437,567	B1	8/2002	Schenck et al.	WO	WO 99/38449		1/1999
6,445,943	B1	9/2002	Ferre et al.	WO	WO 99/52094		4/1999
6,470,207	B1	10/2002	Simon et al.	WO	WO 99/26549		6/1999
6,474,341	B1	11/2002	Hunter et al.	WO	WO 99/29253		6/1999
6,478,802	B2	11/2002	Kienzle, III et al.	WO	WO 99/37208		7/1999
6,484,049	B1	11/2002	Seeley et al.	WO	WO 99/60939		12/1999
6,490,475	B1	12/2002	Seeley et al.	WO	WO 01/30437	A1	5/2001
6,493,573	B1	12/2002	Martinelli et al.				
6,498,944	B1	12/2002	Ben-Haim et al.				
6,499,488	B1	12/2002	Hunter et al.				
6,516,046	B1	2/2003	Fröhlich et al.				
6,527,443	B1	3/2003	Vilsmeier et al.				
6,609,022	B2	8/2003	Vilsmeier et al.				
6,611,700	B1	8/2003	Vilsmeier et al.				
6,701,179	B1	3/2004	Martinelli et al.				
2001/0007918	A1	7/2001	Vilsmeier et al.				
2002/0095081	A1	7/2002	Vilsmeier				
2004/0024309	A1	2/2004	Ferre et al.				

FOREIGN PATENT DOCUMENTS

DE	3042343	A1	6/1982
DE	35 08730		3/1985
DE	37 17 871		5/1987
DE	38 38011		11/1988
DE	3831278	A1	3/1989
DE	42 13 426		4/1992
DE	42 25 112		7/1992
DE	4233978	C1	4/1994
DE	197 15 202		4/1997
DE	197 47 427		10/1997
DE	197 51 761		11/1997
DE	198 32 296		7/1998
EP	0 062 941		3/1982
EP	0 119 660		9/1984
EP	0 155 857		1/1985
EP	0 319 844	A1	1/1988
EP	0 326 768		12/1988

OTHER PUBLICATIONS

Barrick et al., "Prophylactic Intramedullary Fixation of the Tibia for Stress Fracture in a Professional Athlete," *Journal of Orthopaedic Trauma*, vol. 6, No. 2, pp. 241-244 (1992).

Barrick et al., "Technical Difficulties with the Brooker-Wills Nail in Acute Fractures of the Femur," *Journal of Orthopaedic Trauma*, vol. 6, No. 2, pp. 144-150 (1990).

Barrick, "Distal Locking Screw Insertion Using a Cannulated Drill Bit: Technical Note," *Journal of Orthopaedic Trauma*, vol. 7, No. 3, 1993, pp. 248-251.

Benzel et al., "Magnetic Source Imaging: a Review of the Magnes System of Biomagnetic Technologies Incorporated," *Neurosurgery*, vol. 33, No. 2 (Aug. 1993), pp. 252-259.

Bouazza-Marouf et al., "Robotic-Assisted Internal Fixation of Femoral Fractures", *IMECHE.*, pp. 51-58 (1995).

Brack et al., "Accurate X-ray Based Navigation in Computer-Assisted Orthopedic Surgery," *CAR '98*, pp. 716-722.

Bryan, "Bryan Cervical Disc System Single Level Surgical Technique", *Spinal Dynamics*, 2002, pp. 1-33.

Bucholz et al., "Variables affecting the accuracy of stereotactic localization using computerized tomography," *Journal of Neurosurgery*, vol. 79, Nov. 1993, pp. 667-673.

Champleboux et al., "Accurate Calibration of Cameras and Range Imaging Sensors: the NPBS Method," *IEEE International Conference on Robotics and Automation*, Nice, France, May 1992.

- Champleboux, "Utilisation de Fonctions Splines pour la Mise au Point D'un Capteur Tridimensionnel sans Contact," *Quelques Applications Medicales*, Jul. 1991.
- Cinquin et al., "Computer Assisted Medical Interventions," *IEEE Engineering in Medicine and Biology*, May/Jun. 1995, pp. 254-263.
- Cinquin et al., "Computer Assisted Medical Interventions," *International Advanced Robotics Programme*, Sep. 1989, pp. 63-65.
- Clarysse et al., "A Computer-Assisted System for 3-D Frameless Localization in Stereotaxic MRI," *IEEE Transactions on Medical Imaging*, vol. 10, No. 4, Dec. 1991, pp. 523-529.
- Feldmar et al., "3D-2D Projective Registration of Free-Form Curves and Surfaces," *Rapport de recherche (Inria Sophia Antipolis)*, 1994, pp. 1-44.
- Foley et al., "Fundamentals of Interactive Computer Graphics," *The Systems Programming Series*, Chapter 7, Jul. 1984, pp. 245-266.
- Foley et al., "Image-guided Intraoperative Spinal Localization," *Intraoperative Neuroprotection*, Chapter 19, 1996, pp. 325-340.
- Foley, "The StealthStation: Three-Dimensional Image-Interactive Guidance for the Spine Surgeon," *Spinal Frontiers*, Apr. 1996, pp. 7-9.
- Gildenberg et al., "Calculation of Stereotactic Coordinates from the Computed Tomographic Scan," *Neurosurgery*, vol. 10, No. 5, May 1982, pp. 580-586.
- Gonzalez, "Digital Image Fundamentals," *Digital Image Processing*, Second Edition, 1987, pp. 52-54.
- Gottesfeld Brown et al., "Registration of Planar Film Radiographs with Computer Tomography," *Proceedings of MMBIA*, Jun. 1996, pp. 42-51.
- Guezic et al., "Registration of Computed Tomography Data to a Surgical Robot Using Fluoroscopy: A Feasibility Study," *Computer Science/Mathematics*, Sep. 27, 1996, 6 pages.
- Hamadeh et al., "Automated 3-Dimensional Computed Tomographic and Fluoroscopic Image Registration," *Computer Aided Surgery* (1998), 3:11-19.
- Hamadeh et al., "Towards Automatic Registration Between CT and X-ray Images: Cooperation Between 3D/2D Registration and 2D Edge Detection," *MRCAS '95*, pp. 39-46.
- Hatch, "Reference-Display System for the Integration of CT Scanning and the Operating Microscope," *Thesis, Thayer School of Engineering*, Oct. 1984, pp. 1-189.
- Heilbrun et al., "Preliminary experience with Brown-Roberts-Wells (BRW) computerized tomography stereotaxic guidance system," *Journal of Neurosurgery*, vol. 59, Aug. 1983, pp. 217-222.
- Henderson et al., "An Accurate and Ergonomic Method of Registration for Image-guided Neurosurgery," *Computerized Medical Imaging and Graphics*, vol. 18, No. 4, Jul.-Aug. 1994, pp. 273-277.
- Hoerenz, "The Operating Microscope I. Optical Principles, Illumination Systems, and Support Systems," *Journal of Microsurgery*, vol. 1, 1980, pp. 364-369.
- Hofstetter et al., "Fluoroscopy Based Surgical Navigation—Concept and Clinical Applications," *Computer Assisted Radiology and Surgery*, 1997, pp. 956-960.
- Horner et al., "A Comparison of CT-Stereotaxic Brain Biopsy Techniques," *Investigative Radiology*, Sep.-Oct. 1984, pp. 367-373.
- Hounsfield, "Computerized transverse axial scanning (tomography): Part 1. Description of system," *British Journal of Radiology*, vol. 46, No. 552, Dec. 1973, pp. 1016-1022.
- Jacques et al., "A Computerized Microstereotactic Method to Approach, 3-Dimensionally Reconstruct, Remove and Adjuvantly Treat Small CNS Lesions," *Applied Neurophysiology*, vol. 43, 1980, pp. 176-182.
- Jacques et al., "Computerized three-dimensional stereotaxic removal of small central nervous system lesion in patients," *J. Neurosurg.*, vol. 53, Dec. 1980, pp. 816-820.
- Joskowicz et al., "Computer-Aided Image-Guided Bone Fracture Surgery: Concept and Implementation," *CAR '98*, pp. 710-715.
- Kelly et al., "Precision Resection of Intra-Axial CNS Lesions by CT-Based Stereotactic Craniotomy and Computer Monitored CO₂ Laser," *Acta Neurochirurgica*, vol. 68, 1983, pp. 1-9.
- Laitinen et al., "An Adapter for Computed Tomography-Guided, Stereotaxis," *Surg. Neurol.*, 1985, pp. 559-566.
- Laitinen, "Noninvasive multipurpose stereoadapter," *Neurological Research*, Jun. 1987, pp. 137-141.
- Lavallee et al., "Matching 3-D Smooth Surfaces with their 2-D Projections using 3-D Distance Maps," *SPIE*, vol. 1570, *Geometric Methods in Computer Vision*, 1991, pp. 322-336.
- Lavallee et al., "Computer Assisted Driving of a Needle into the Brain," *Proceedings of the International Symposium CAR '89, Computer Assisted Radiology*, 1989, pp. 416-420.
- Lavallee et al., "Computer Assisted Interventionist Imaging: The Instance of Stereotactic Brain Surgery," *North-Holland MEDINFO 89, Part 1*, 1989, pp. 613-617.
- Lavallee et al., "Image guided operating robot: a clinical application in stereotactic neurosurgery," *Proceedings of the 1992 IEEE International Conference on Robotics and Automation*, May 1992, pp. 618-624.
- Lavallee et al., "Matching of Medical Images for Computed and Robot Assisted Surgery," *IEEE EMBS*, Orlando, 1991.
- Leksell et al., "Stereotaxis and Tomography—A Technical Note," *ACTA Neurochirurgica*, vol. 52, 1980, pp. 1-7.
- Lemieux et al., "A Patient-to-Computed-Tomography Image Registration Method Based on Digitally Reconstructed Radiographs," *Med. Phys.* 21 (11), Nov. 1994, pp. 1749-1760.
- Levin et al., "The Brain: Integrated Three-dimensional Display of MR and PET Images," *Radiology*, vol. 172, No. 3, Sep. 1989, pp. 783-789.
- Mazier et al., "Computer-Assisted Interventionist Imaging: Application to the Vertebral Column Surgery," *Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 12, No. 1, 1990, pp. 0430-0431.
- Mazier et al., *Chirurgie de la Colonne Vertebrale Assistee par Ordinateur: Application au Vissage Pediculaire*, *Innov. Tech. Biol. Med.*, vol. 11, No. 5, 1990, pp. 559-566.
- Pelizzari et al., "Accurate Three-Dimensional Registration of CT, PET, and/or MR Images of the Brain," *Journal of Computer Assisted Tomography*, Jan./Feb. 1989, pp. 20-26.
- Pelizzari et al., "Interactive 3D Patient-Image Registration," *Information Processing in Medical Imaging*, 12th International Conference, IPMI '91, Jul. 7-12, 136-141 (A.C.F. Colchester et al. eds. 1991).
- Pelizzari et al., No. 528—"Three Dimensional Correlation of PET, CT and MRI Images," *The Journal of Nuclear Medicine*, vol. 28, No. 4, Apr. 1987, p. 682.
- Phillips et al., "Image Guided Orthopaedic Surgery Design and Analysis," *Trans Inst. MC*, vol. 17, No. 5, 1995, pp. 251-264.
- Potamianos et al., "Intra-Operative Imaging Guidance for Keyhole Surgery Methodology and Calibration," *First International Symposium on Medical Robotics and Computer Assisted Surgery*, Sep. 22-24, 1994, pp. 98-104.
- Reinhardt et al., "CT-Guided 'Real Time' Stereotaxy," *ACTA Neurochirurgica*, 1989.
- Rosenbaum et al., "Computerized Tomography Guided Stereotaxis: A New Approach," *Applied Neurophysiology*, vol. 43, No. 3-5, 1980, pp. 172-173.
- Sautot, "Vissage Pediculaire Assiste Par Ordinateur," Sep. 20, 1994.
- Schueler et al., "Correction of Image Intensifier Distortion for Three-Dimensional X-Ray Angiography," *SPIE Medical Imaging 1995*, vol. 2432, pp. 272-279.
- Selvik et al., "A Roentgen Stereophotogrammetric System," *Acta Radiologica Diagnosis*, 1983, pp. 343-352.
- Shelden et al., "Development of a computerized microstereotaxic method for localization and removal of minute CNS lesions under direct 3-D vision," *J. Neurosurg.*, vol. 52, 1980, pp. 21-27.
- Smith et al., "Computer Methods for Improved Diagnostic Image Display Applied to Stereotactic Neurosurgery," *Automedical*, vol. 14, 1992, pp. 371-382 (4 unnumbered pages).
- Smith et al., "The Neurostation™—A Highly Accurate, Minimally Invasive Solution to Frameless Stereotactic Neurosurgery," *Computerized Medical Imaging and Graphics*, vol. 18, Jul.-Aug. 1994, pp. 247-256.
- Viant et al., "A Computer Assisted Orthopaedic System for Distal Locking of Intramedullary Nails," *Proc. of MediMEC '95*, Bristol, 1995, pp. 86-91.
- Watanabe, "Neuronavigator," *Igaku-no-Ayumi*, vol. 137, No. 6, May 10, 1986, pp. 1-4.

- Germano, "Instrumentation, Technique and Technology", *Neurosurgery*, vol. 37, No. 2, Aug. 1995, pp. 348-350.
- Hatch, et al., "Reference-Display System for the Integration of CT Scanning and the Operating Microscope", *Proceedings of the Eleventh Annual Northeast Bioengineering Conference*, Mar. 14-15, 1985, pp. 252-254.
- International Search Report, Jan. 1991, France.
- Adams et al., *Computer-Assisted Surgery*, IEEE Computer Graphics & Applications, pp. 43-51, (May 1990).
- Batnitzky, S. et al.; *Three-Dimensional Computer Reconstruction from Surface Contours for Head CT Examinations*. J. Comp. Asst. Tomogr., vol. 5, No. 1, pp. 60-67, Feb. 1981.
- Bergstrom et al. *Stereotaxic Computed Tomography*, Am. J. Roentgenol, vol. 127 pp. 167-170 (1976).
- Brown, R., M.D., *A Stereotactic Head Frame for Use with CT Body Scanners*, Investigative Radiology © J.B. Lippincott Company, pp. 300-304 (Jul.-Aug. 1979).
- Bucholz, R.D., et al. *Image-guided surgical techniques for infections and trauma of the central nervous system*, *Neurosurg. Clinics of N.A.*, vol. 7, No. 2, pp. 187-200 (1996).
- Bucholz, R.D., et al., *A Comparison of Sonic Digitizers Versus Light Emitting Diode-Based Localization*, *Interactive Image-Guided Neurosurgery*, Chapter 16, pp. 179-200 (1993).
- Bucholz, R.D., et al., *Intraoperative localization using a three dimensional optical digitizer*, SPIE—The Intl. Soc. for Opt. Eng., vol. 1894, pp. 312-322 (Jan. 17-19, 1993).
- Bucholz, R.D., et al., *Intraoperative Ultrasonic Brain Shift Monitor and Analysis*, *Stealth Station Marketing Brochure* (2 pages) (undated).
- Bucholz, R.D., et al., *The Correction of Stereotactic Inaccuracy Caused by Brain Shift Using an Intraoperative Ultrasound Device*, *First Joint Conference, Computer Vision, Virtual Reality and Robotics in Medicine and Medical Robotics and Computer-Assisted Surgery*, Grenoble, France, pp. 459-466 (Mar. 19-22, 1997).
- Cutting M.D. et al., *Optical Tracking of Bone Fragments During Craniofacial Surgery*, *Second Annual International Symposium on Medical Robotics and Computer Assisted Surgery*, pp. 221-225, (Nov. 1995).
- Friets, E.M., et al. *A Frameless Stereotaxic Operating Microscope for Neurosurgery*, *IEEE Trans. on Biomed. Eng.*, vol. 36, No. 6, pp. 608-617 (Jul. 1989).
- Gallen, C.C., et al., *Intracranial Neurosurgery Guided by Functional Imaging*, *Surg. Neurol.*, vol. 42, pp. 523-530 (1994).
- Galloway, R.L., et al., *Interactive Image-Guided Neurosurgery*, *IEEE Trans. on Biomed. Eng.*, vol. 89, No. 12, pp. 1226-1231 (1992).
- Galloway, R.L., Jr. et al, *Optical localization for interactive, image-guided neurosurgery*, SPIE, vol. 2164, pp. 137-145 (undated).
- Gomez, C.R., et al., *Transcranial Doppler Ultrasound Following Closed Head Injury: Vasospasm or Vasoparalysis?*, *Surg. Neurol.*, vol. 35, pp. 30-35 (1991).
- Grimson, W.E.L., *An Automatic Registration Method for Frameless Stereotaxy, Image Guided Surgery, and enhanced Reality Visualization*, *IEEE*, pp. 430-436 (1994).
- Grimson, W.E.L., et al., *Virtual-reality technology is giving surgeons the equivalent of x-ray vision helping them to remove tumors more effectively, to minimize surgical wounds and to avoid damaging critical tissues*, *Sci. Amer.*, vol. 280, No. 6, pp. 62-69 (Jun. 1999).
- Guthrie, B.L., *Graphic-Interactive Cranial Surgery: The Operating Arm System*, *Handbook of Stereotaxy Using the CRW Apparatus*, Chapter 13, pp. 193-211 (undated).
- Hardy, T., M.D., et al., *CASS: A Program for Computer Assisted Stereotaxic Surgery*, *The Fifth Annual Symposium on Computer Applications in Medical Care*, *Proceedings*, Nov. 1-4, 1981, *IEEE*, pp. 1116-1126, (1981).
- Heilbrun, M.D., *Progressive Technology Applications, Neurosurgery for the Third Millennium*, Chapter 15, J. Whitaker & Sons, Ltd., Amer. Assoc. of Neurol. Surgeons, pp. 191-198 (1992).
- Heilbrun, M.P., *Computed Tomography—Guided Stereotactic Systems*, *Clinical Neurosurgery*, Chapter 31, pp. 564-581 (1983).
- Heilbrun, M.P., et al., *Stereotactic Localization and Guidance Using a Machine Vision Technique*, *Stereotact & Funct. Neurosurg.*, *Proceed. of the Mtg. of the Amer. Soc. for Sterot. and Funct. Neurosurg.* (Pittsburgh, PA) vol. 58, pp. 94-98 (1992).
- Kall, B., *The Impact of Computer and Imaging Technology on Stereotactic Surgery*, *Proceedings of the Meeting of the American Society for Stereotactic and Functional Neurosurgery*, pp. 10-22 (1987).
- Kato, A., et al., *A frameless, armless navigational system for computer-assisted neurosurgery*, *J. Neurosurg.*, vol. 74, pp. 845-849 (May 1991).
- Kelly, P.J. et al.; *Computer assisted Stereotactic Laser Microsurgery for the Treatment of Intracranial Neoplasms*, *Neurosurgery*. vol. 10, No. 3, pp. 324-330, 1982.
- Kelly, P.J., *Computer Assisted Stereotactic Biopsy and Volumetric Resection of Pediatric Brain Tumors*, *Brain Tumors in Children*, *Neurologic Clinics*, vol. 9, No. 2, pp. 317-336 (May 1991).
- Kelly, P.J., *Computer-Directed Stereotactic Resection of Brain Tumors*, *Neurologica Operative Atlas*, vol. 1, No. 4, pp. 299-313 (1991).
- Kelly, P.J., et al., *Results of Computed Tomography-based Computer-assisted Stereotactic Resection of Metastatic Intracranial Tumors*, *Neurosurgery*, vol. 22, No. 1, Part 1, 1988, pp. 7-17 (Jan. 1988).
- Kelly, P.J., *Stereotactic Imaging, Surgical Planning and Computer-Assisted Resection of Intracranial Lesions: Methods and Results*, *Advances and Technical Standards in Neurosurgery*, vol. 17, pp. 78-118, (1990).
- Kim, W.S. et al., *A Helmet Mounted Display for Telerobotics*, *IEEE*, pp. 543-547 (1988).
- Klimek, L., et al., *Long-Term Experience with Different Types of Localization Systems in Skull-Base Surgery*, *Ear, Nose & Throat Surgery*, Chapter 51, pp. 635-638 (undated).
- Kosugi, Y., et al., *An Articulated Neurosurgical Navigation System Using MRI and CT Images*, *IEEE Trans. on Biomed. Eng.* vol. 35, No. 2, pp. 147-152 (Feb. 1988).
- Krybus, W., et al., *Navigation Support for Surgery by Means of Optical Position Detection*, *Computer Assisted Radiology Proceed. of the Intl. Symp. CAR '91 Computed Assisted Radiology*, pp. 362-366 (Jul. 3-6, 1991).
- Kwoh, Y.S., Ph.D., et al., *A New Computerized Tomographic-Aided Robotic Stereotaxis System*, *Robotics Age*, vol. 7, No. 6, pp. 17-22 (Jun. 1985).
- Lavallee, S. *A New System for Computer Assisted Neuro-surgery*. *IEEE Engineering in Medicine & Biology Society 11th Annual International Conference*, vol. 11, pp. 926-927, Nov. 1989.
- Lavallee, S., et al., *Computer Assisted Knee Anterior Cruciate Ligament Reconstruction First Clinical Tests*, *Proceedings of the First International Symposium on Medical Robotics and Computer Assisted Surgery*, pp. 11-16 (Sep. 1994).
- Lavallee, S., et al., *Computer Assisted Medical Interventions*, *NATO ASI Series*, vol. F 60, 3d Imaging in Medic., pp. 301-312 (1990).
- Lavallee, S.A., *New System for Computer Assisted Neurosurgery*. *IEEE Engineering in Medicine & Biology Society 11th Annual International Conference*, vol. 11, pp. 926-927, Nov. 1989.
- Leavitt, D.D., et al., *Dynamic Field Shaping to Optimize Stereotactic Radiosurgery*, *I.J. Rad. Onc. Biol. Physc.*, vol. 21, pp. 1247-1255 (1991).
- Maurer, Jr., et al., *Registration of Head CT Images to Physical Space Using a Weighted Combination of Points and Surfaces*, *IEEE Trans. on Med. Imaging*, vol. 17, No. 5, pp. 753-761 (Oct. 1998).
- McGirr, S., M.D., et al., *Stereotactic Resection of Juvenile Pilocytic Astrocytomas of the Thalamus and Basal Ganglia*, *Neurosurgery*, vol. 20, No. 3, pp. 447-452, (1987).
- Ng, W.S. et al., *Robotic Surgery—A First-Hand Experience in Transurethral Resection of the Prostate Surgery*, *IEEE Eng. in Med. and Biology*, pp. 120-125 (Mar. 1993).
- Penn, R.D., et al., *Stereotactic Surgery with Image Processing of Computerized Tomographic Scans*, *Neurosurgery*, vol. 3, No. 2, pp. 157-163 (Sep.-Oct. 1978).
- Pixsys, *3-D Digitizing Accessories*, by Pixsys (marketing brochure)(undated) (2 pages).
- Reinhardt, H., et al., *A Computer-Assisted Device for Intraoperative CT-Correlated Localization of Brain Tumors*, pp. 51-58 (1988).
- Reinhardt, H.F. et al., *Sonic Stereometry in Microsurgical Procedures for Deep-Seated Brain Tumors and Vascular Malformations*, *Neurosurgery*, vol. 32, No. 1, pp. 51-57 (Jan. 1993).

Reinhardt, H.F., et al., Mikrochirurgische Entfernung tiefliegender Gefäßmißbildungen mit Hilfe der Sonar-Stereometrie (Microsurgical Removal of Deep-Seated Vascular Malformations Using Sonar Stereometry). *Ultraschall in Med.* 12, pp. 80-83 (1991).

Reinhardt, Hans. F., Neuronavigation: A Ten-Year Review, *Neurosurgery*, pp. 329-341 (undated).

Roberts, D.W., et al.; A Frameless Stereotaxic Integration of Computerized Tomographic Imaging and the Operating Microscope. *J. Neurosurg.*, vol. 65, pp. 545-549, 1986.

Simon, D.A., Accuracy Validation in Image-Guided Orthopaedic Surgery, Second Annual Intl. Symp. on Med. Rob. and Comp-Assisted surgery, MRCAS '95, pp. 185-192 (undated).

Smith, K.R., et al. Multimodality Image Analysis and Display Methods for Improved Tumor Localization in Stereotactic Neurosurgery, *Annul Intl. Conf. of the IEEE Eng. in Med. and Biol. Soc.*, vol. 13, No. 1, p. 210 (1991).

Tan, K., Ph.D., et al., A frameless stereotactic approach to neurosurgical planning based on retrospective patient-image registration, *J Neurosurg*, vol. 79, pp. 296-303 (Aug. 1993).

Thompson, et al., A System for Anatomical and Functional Mapping of the Human Thalamus, *Computers and Biomedical Research*, vol. 10, pp. 9-24 (1977).

Trobraugh, J.W., et al., Frameless Stereotactic Ultrasonography: Method and Applications, *Computerized Medical Imaging and Graphics*, vol. 18, No. 4, pp. 235-246 (1994).

Von Hanwehr et al., Foreword, *Computerized Medical Imaging and Graphics*, vol. 18, No. 4, pp. 225-228, (Jul.-Aug. 1994).

Wang, M.Y., et al., An Automatic Technique for Finding and Localizing Externally Attached Markers in CT and MR Volume Images of the Head, *IEEE Trans. on Biomed. Eng.*, vol. 43, No. 6, pp. 627-637 (Jun. 1996).

Watanabe, E et al., Three-Dimensional Digitizer (Neuronavigator): New Equipment for Computed Tomography-Guided Stereotaxic Surgery. *Surg. Neurol.*, vol. 27, pp. 543-547, 1987.

Watanabe, E., M.D., et al., Open Surgery Assisted by the Neuronavigator, a Stereotactic, Articulated, Sensitive Arm, *Neurosurgery*, vol. 28, No. 6, pp. 792-800 (1991).

Lavallee, S. A New System for Computer Assisted Neurosurgery. *IEEE Engineering in Medicine & Biology Society 11th Annual International Conference*, vol. 11, pp. 926-927, Nov. 1989.

Watanabe, E et al. Three-Dimensional Digitizer (Neuronavigator): New Equipment for Computed Tomography—Guided Stereotaxic Surgery. *Surg. Neurol.*, vol. 27, pp. 543-547, 1987.

Batnitzky, S. et al. Three-Dimensional Computer Reconstruction from Surface Contours for Head CT Examinations.

J. Comp. Asst. Tomogr., vol. 5, No. 1, pp. 60-67, Feb. 1981.

Roberts, D.W., et al. A Frameless Stereotaxic Integration of Computerized Tomographic Imaging and the Operating Microscope, *J. Neurosurg.*, vol. 65, pp. 545-549, 1986.

Kelly, P.J. et al. Computer-assisted Stereotactic Laser Microsurgery for the Treatment of Intracranial Neoplasms, *Neurosurgery*, vol. 10, No. 3, pp. 324-330, 1982.

S. Lavallee, "A New System for Computer Neurosurgery", *IEEE Eng. in Medicine & Bio. Soc. 11th Annual Int. Conf.*, Nov. 9-12, 1989, pp. 926-927.


Watanabe et al., Three Dimensional Digitizer (Neuronavigator): New Equipment for Computed Tomography—Guided Stereotaxic Surgery, *Surg. Neurol.*, 1987, No. 27, pp. 543-547.

P.J. Kelly et al., "Computer-Assisted Stereotactic Laser Micro-Surgery for the Treatment of Intracranial Neoplasms", *Neuro.*, vol. 10, No. 3, 1982, pp. 324-330.

Batnitzky et al., "Three-dimensional Computer Reconstruction From Surface Contours for Head CT Examinations", *Journal of Comp. Assisted Tomography*, No. 5, Feb. 1981, pp. 60-67.

Roberts et al., "A Frameless Stereotaxic Integration of Computerized Tomographic Imaging and the Operating Microscope", *J. of Neuro. Surg.* No. 65, 1986, pp. 545-549.

* cited by examiner

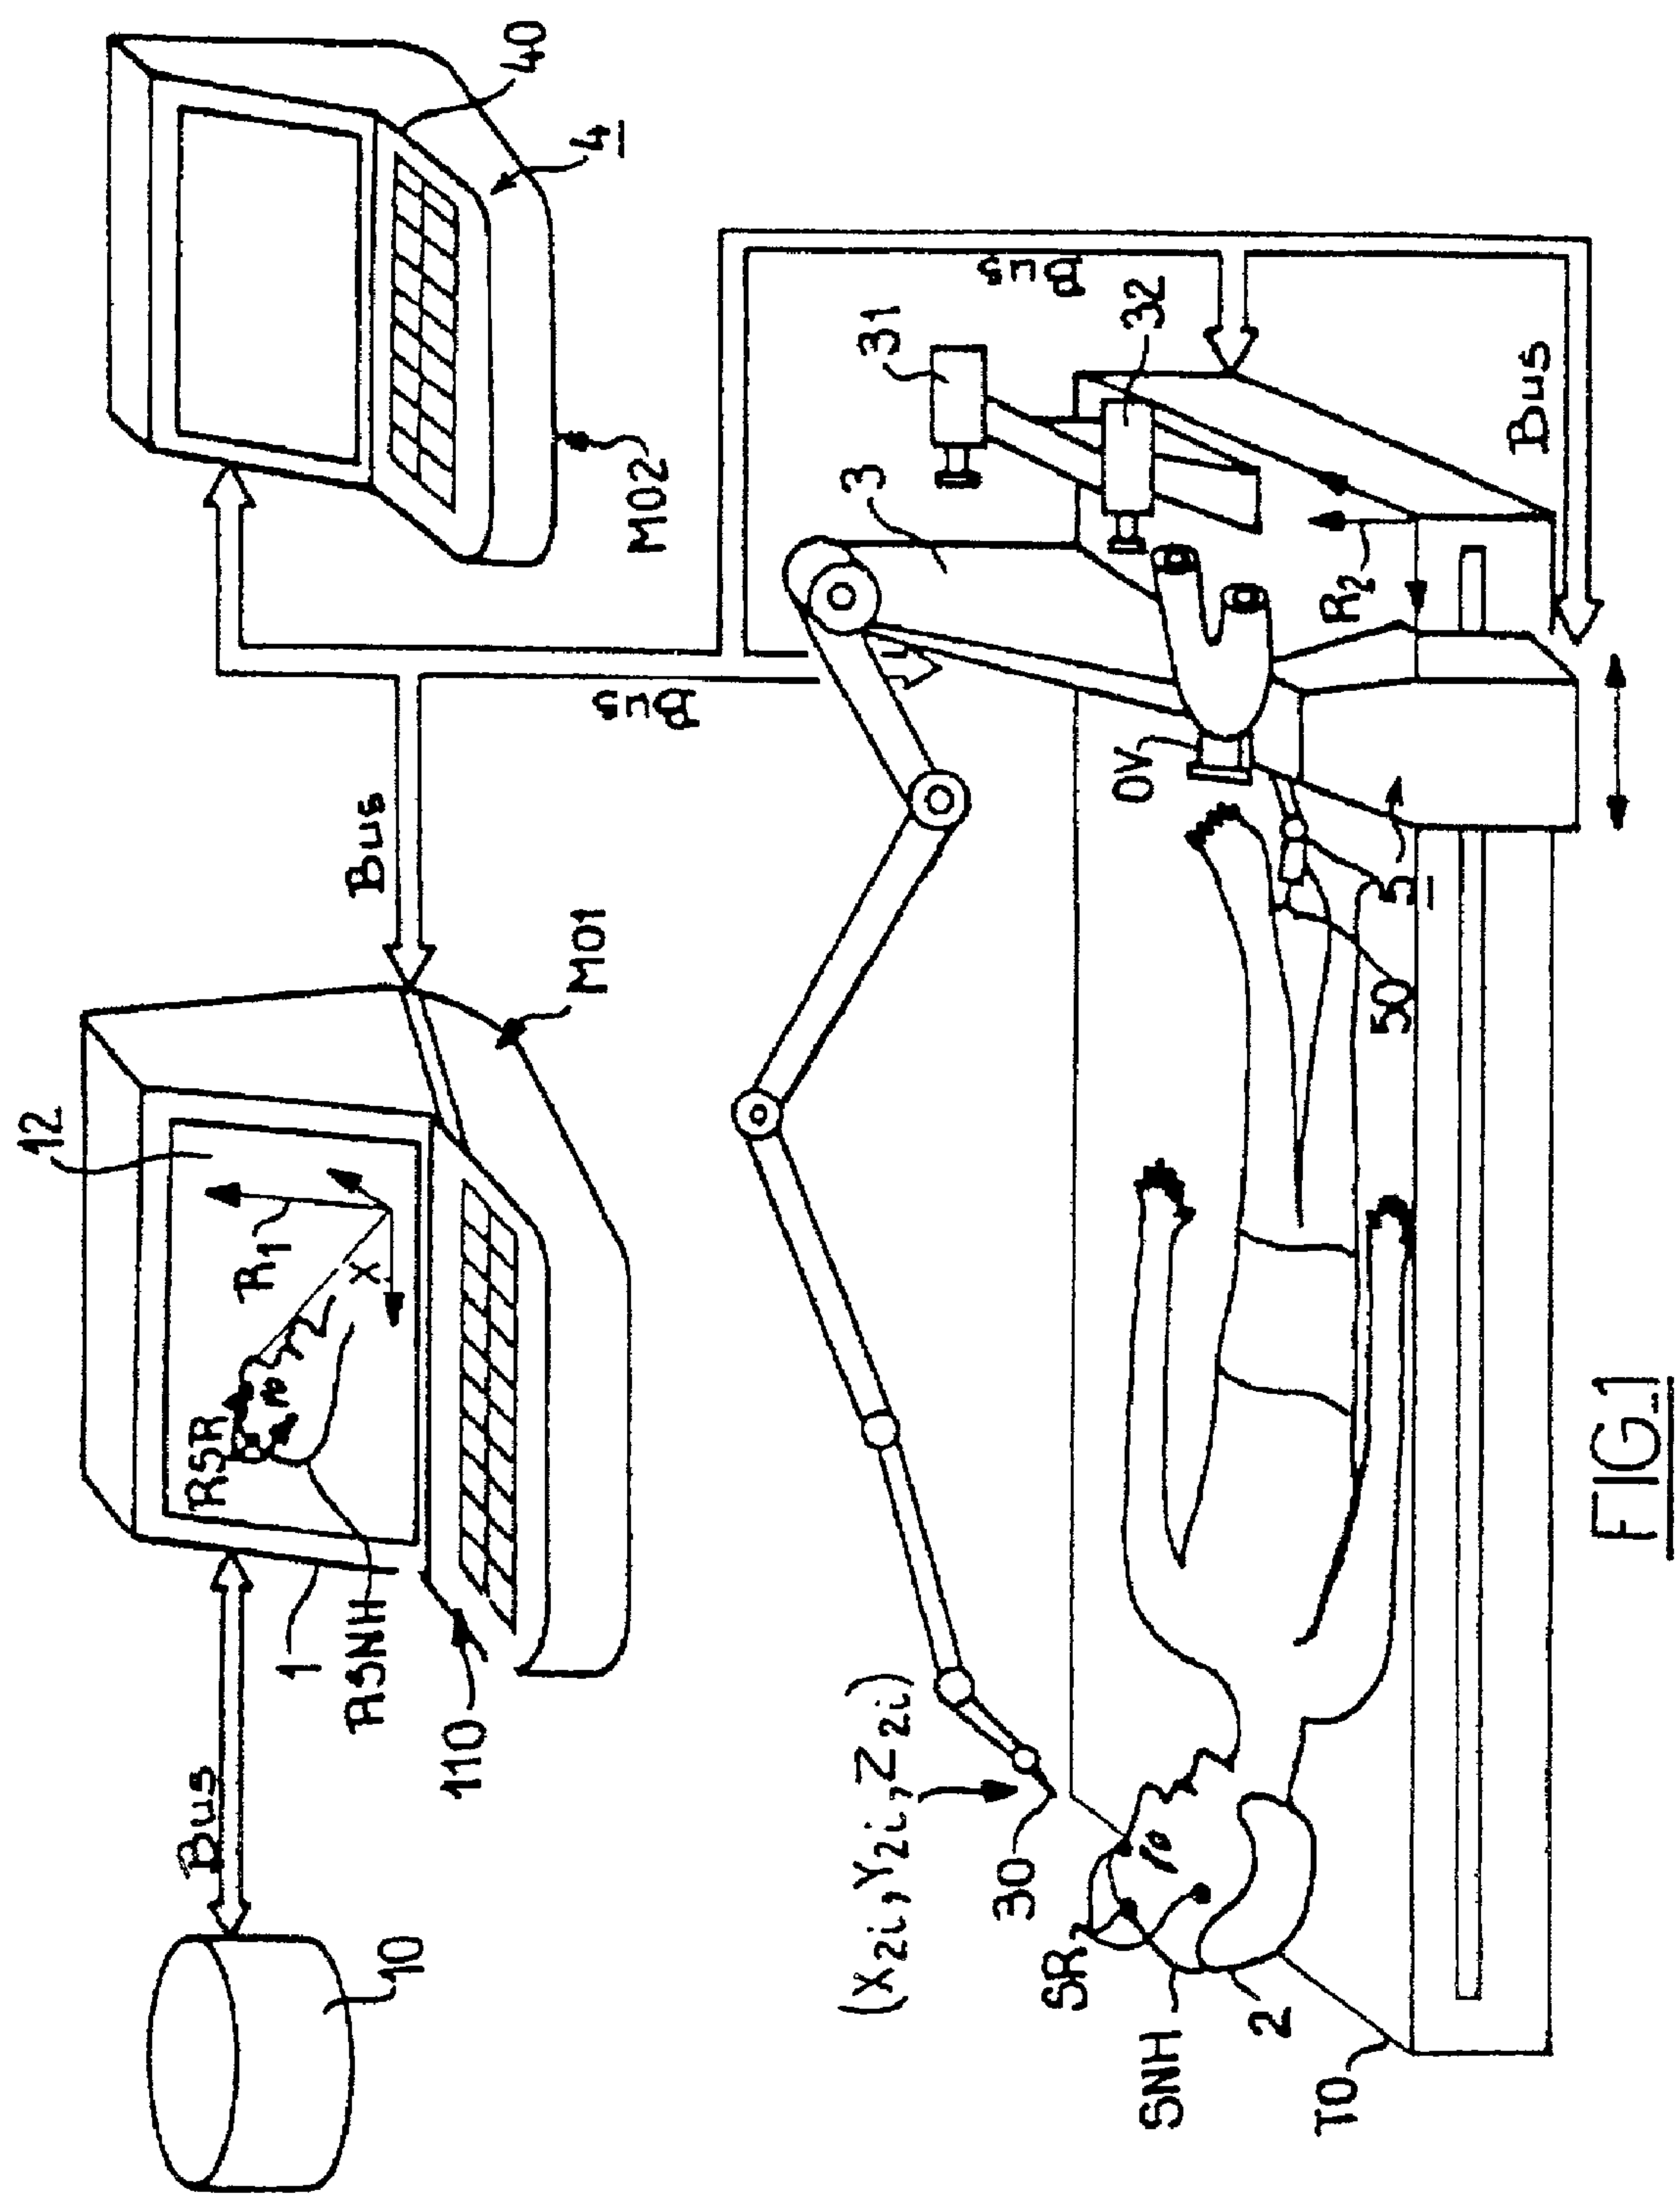

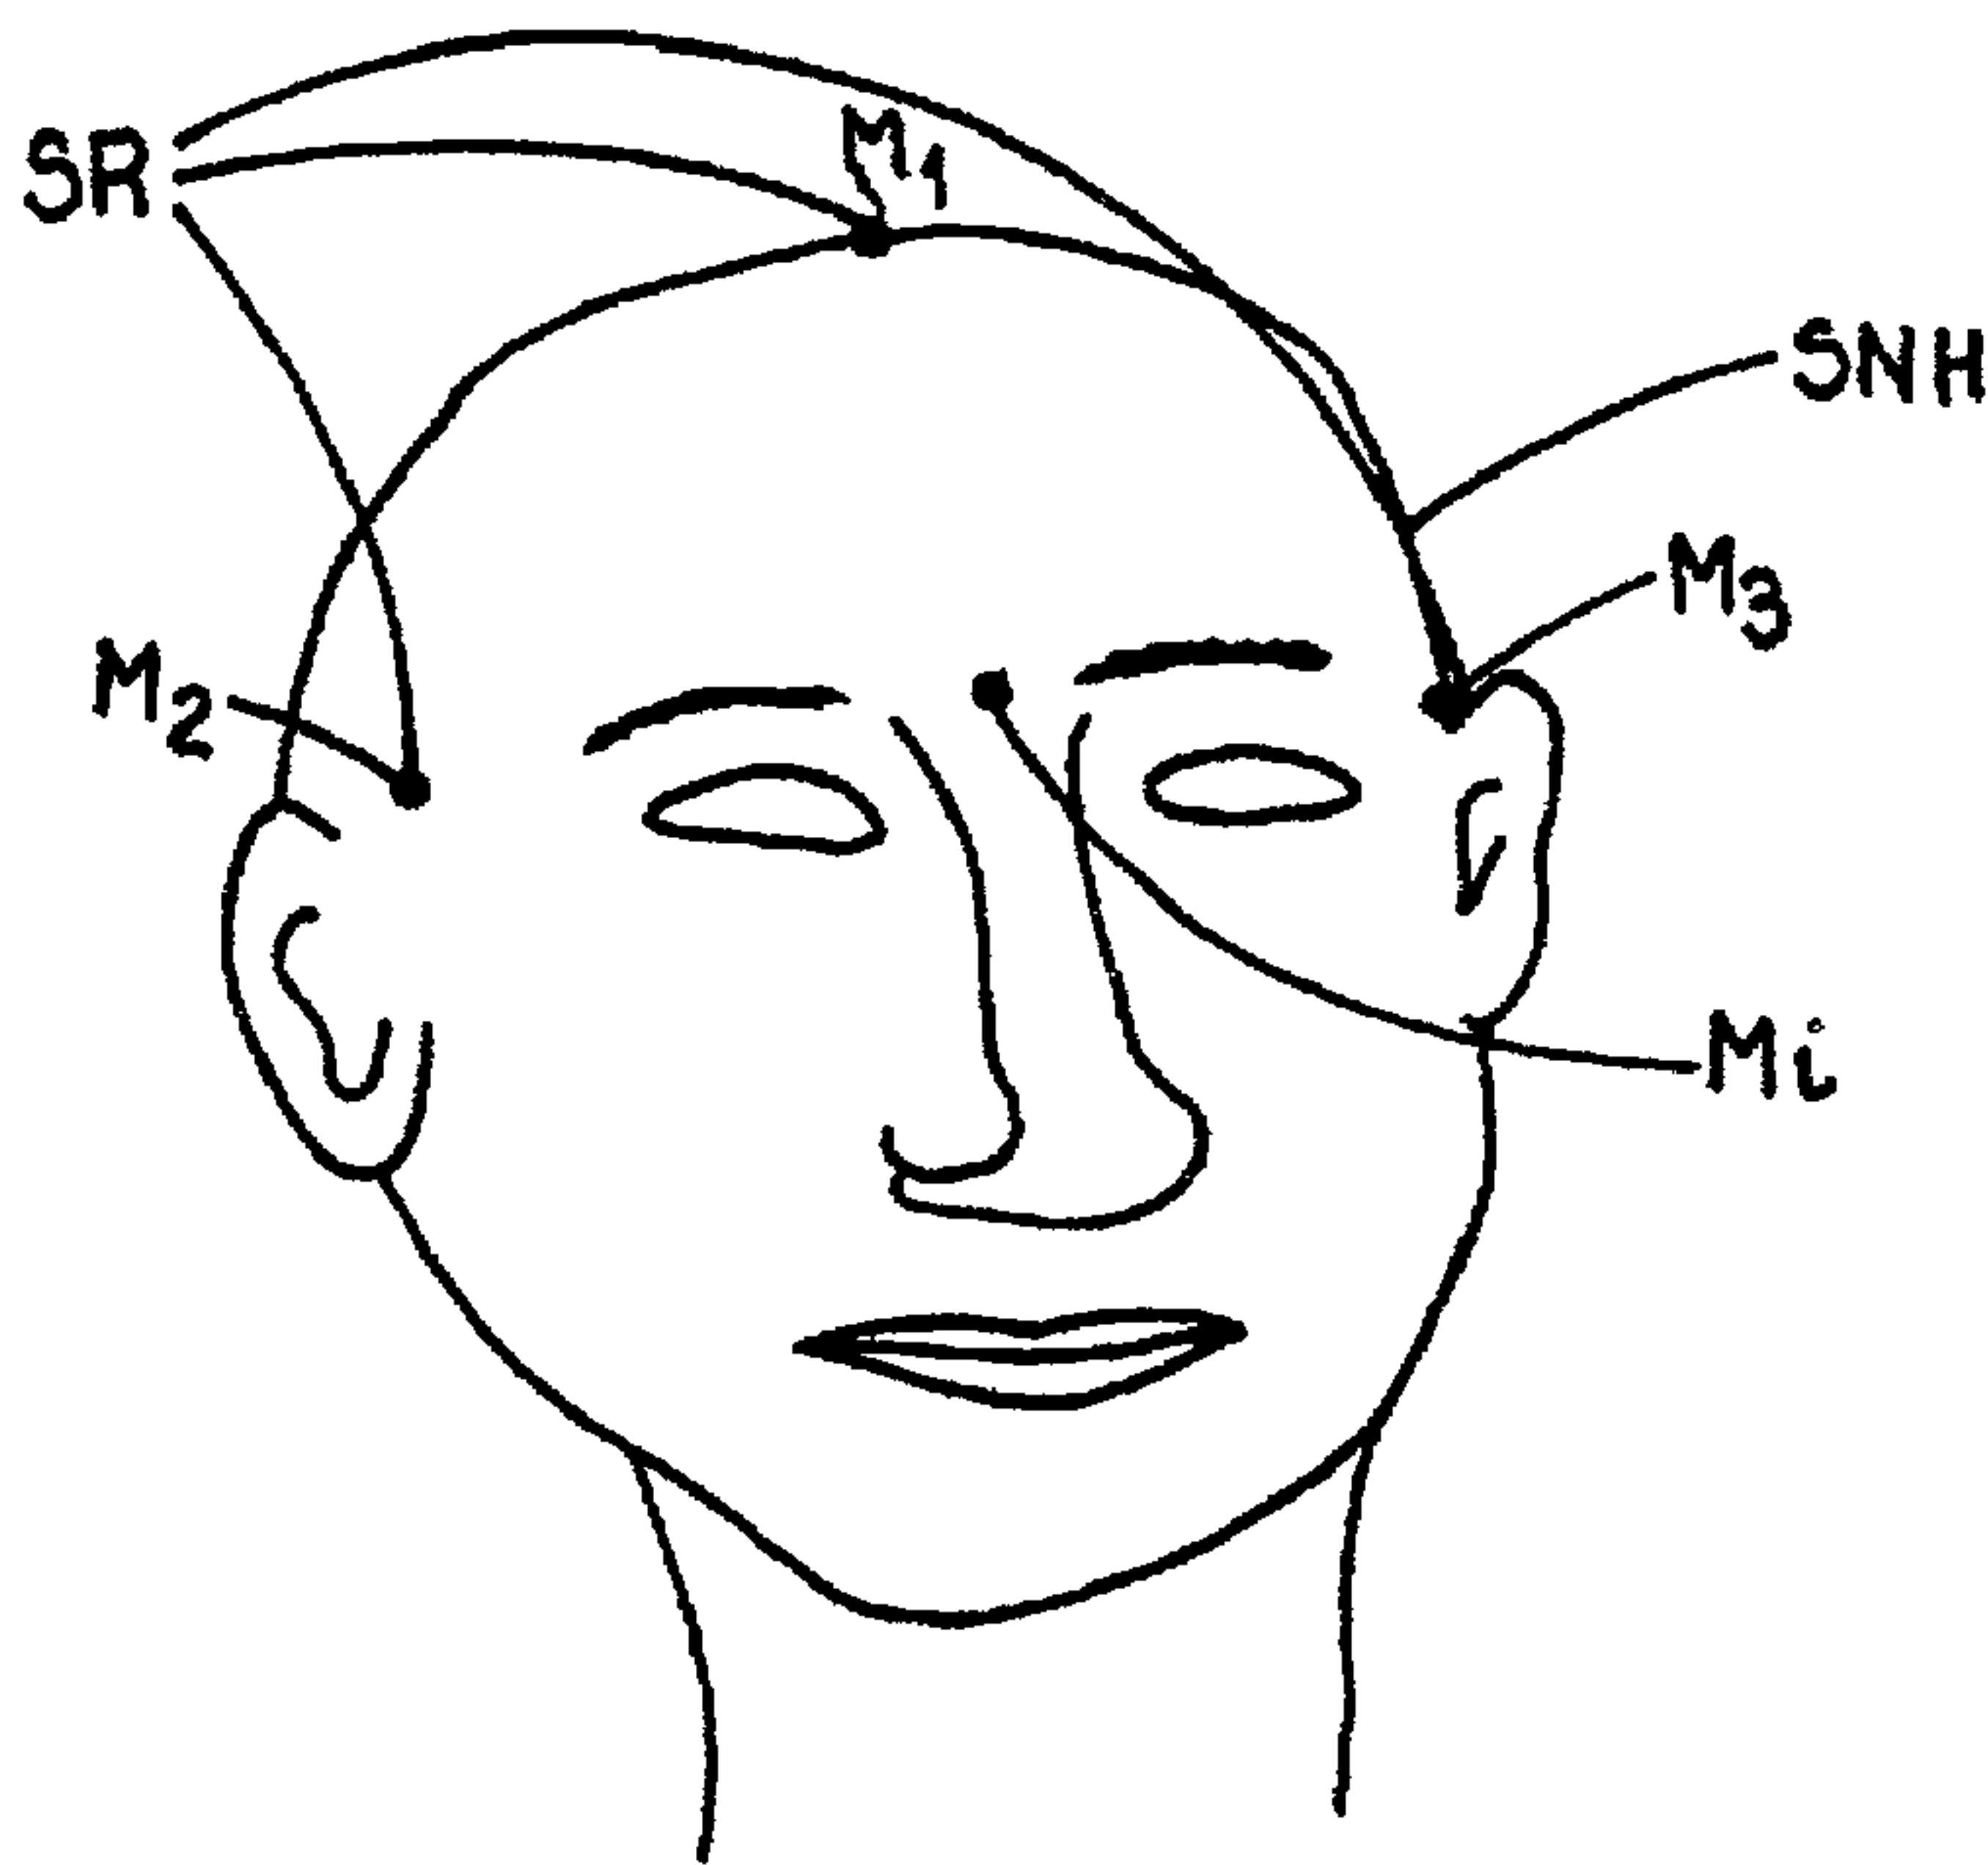


FIG. 2


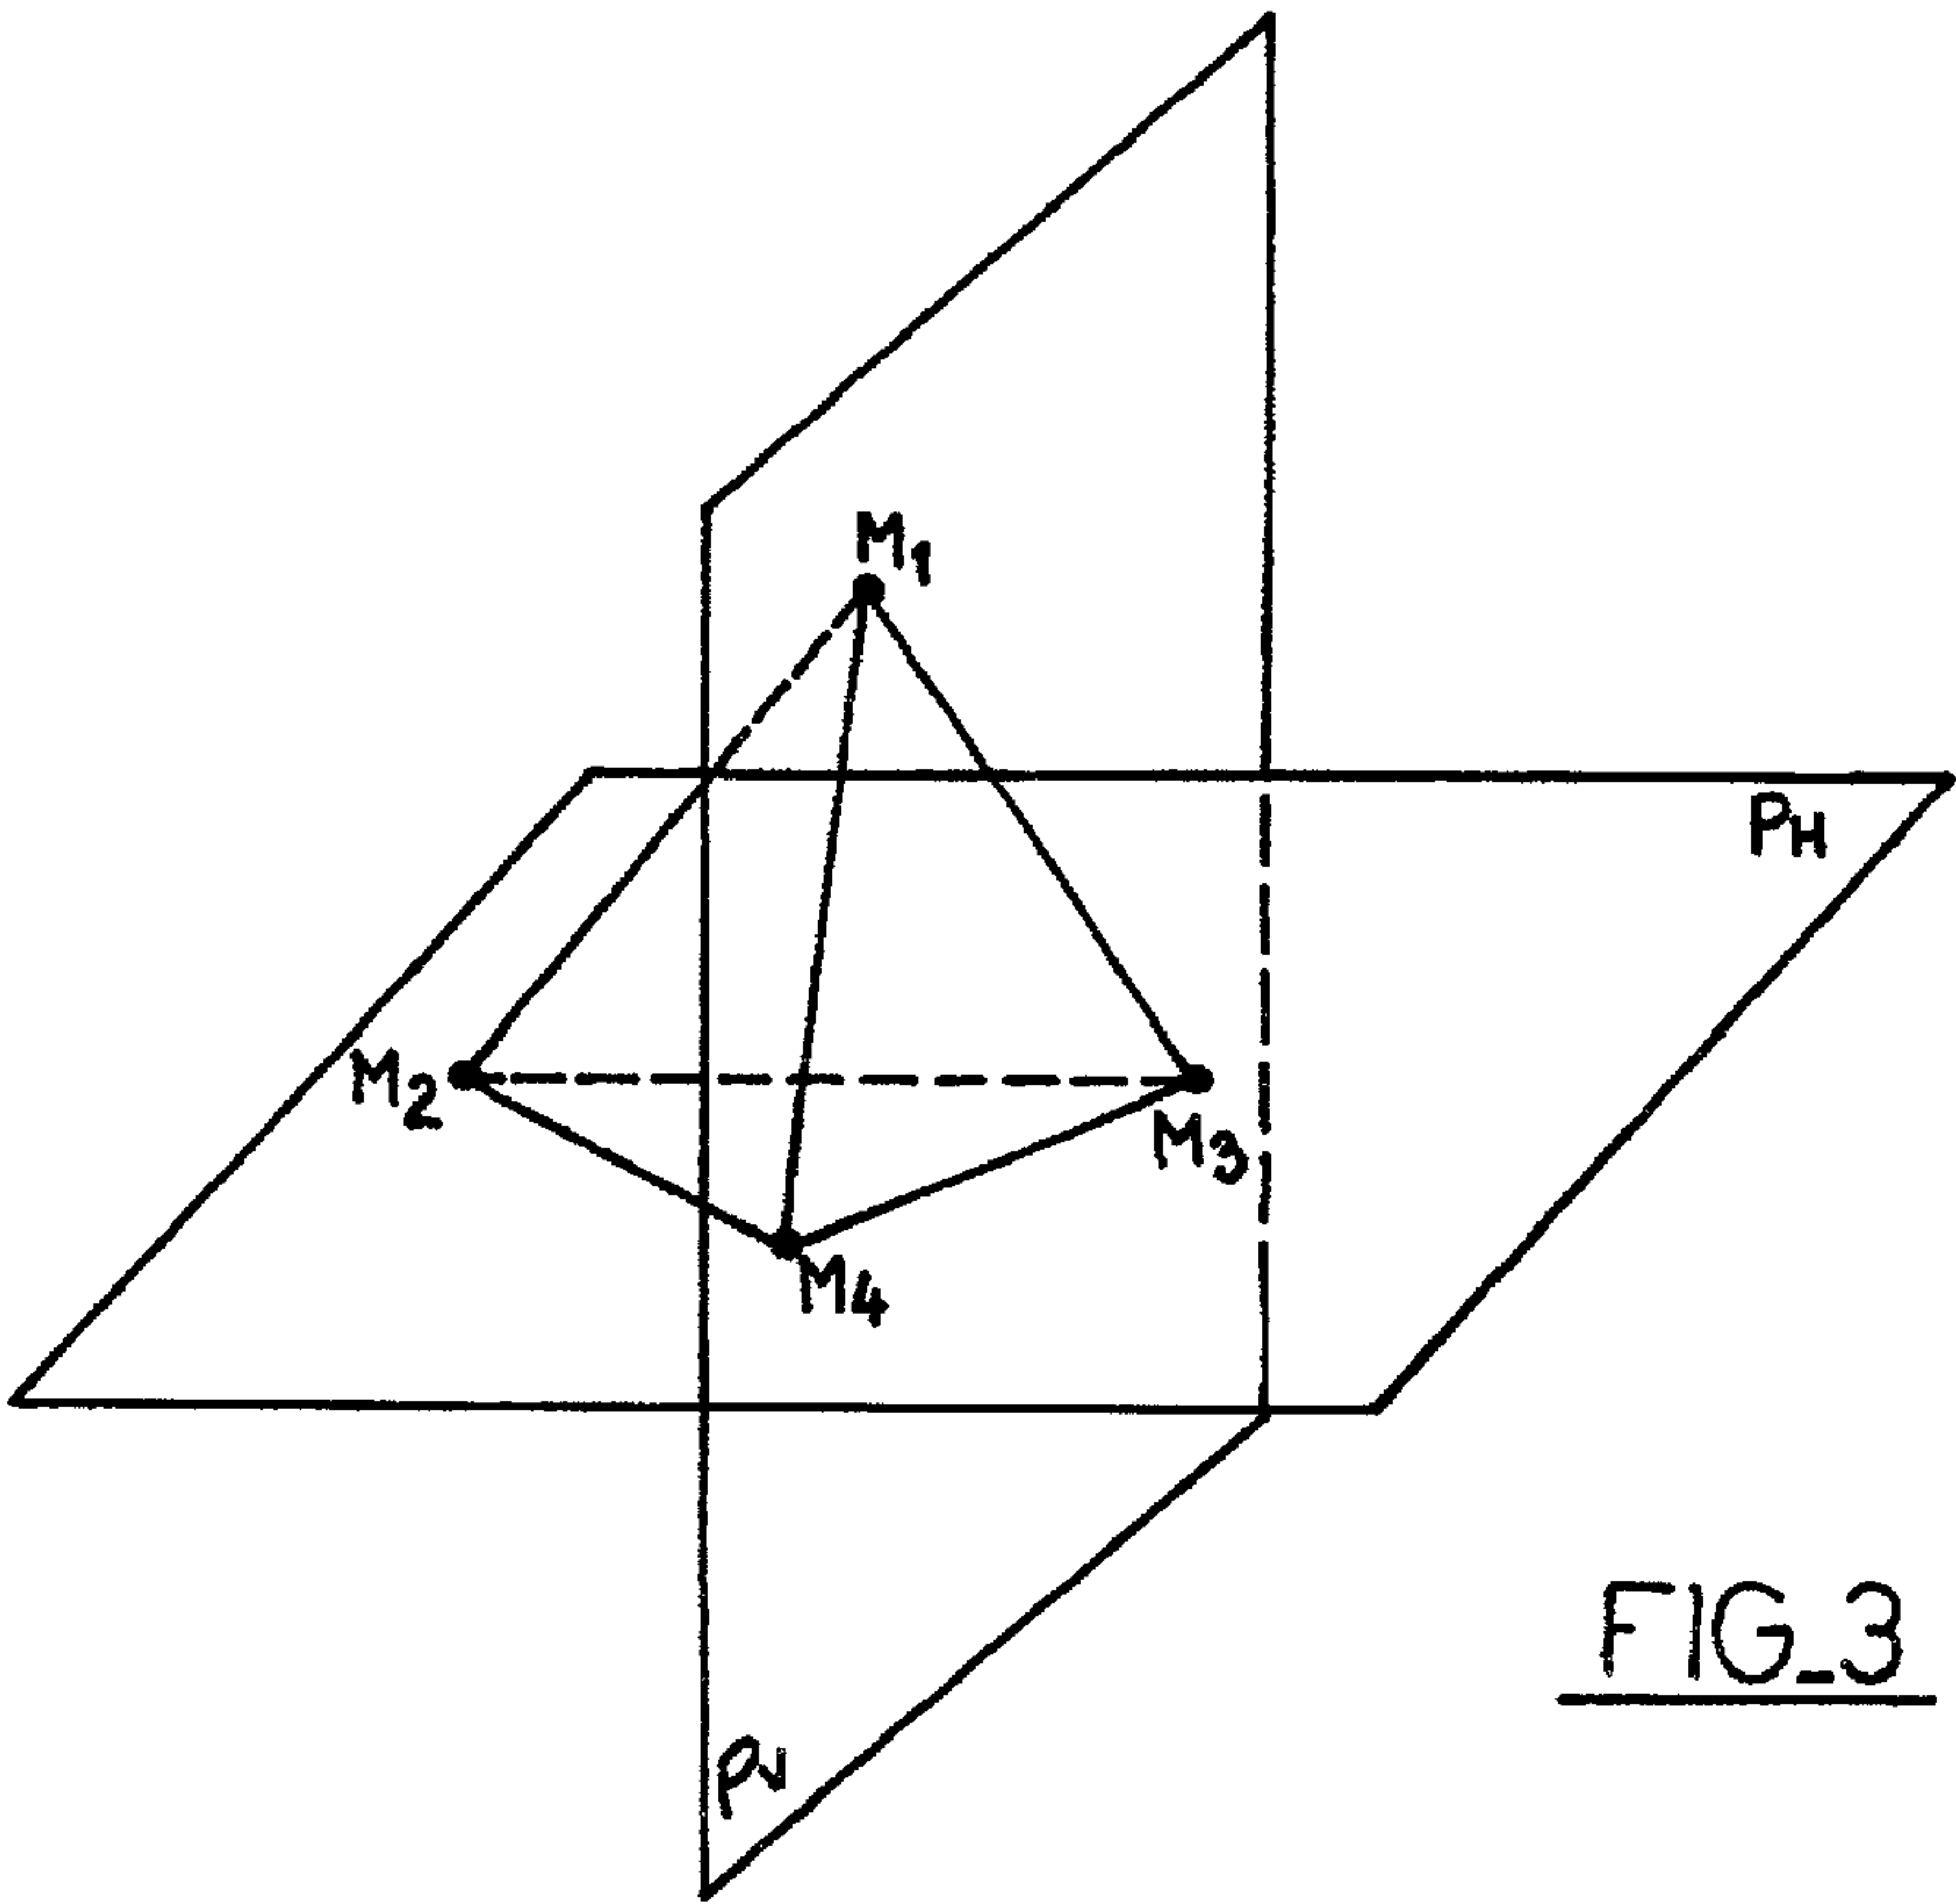
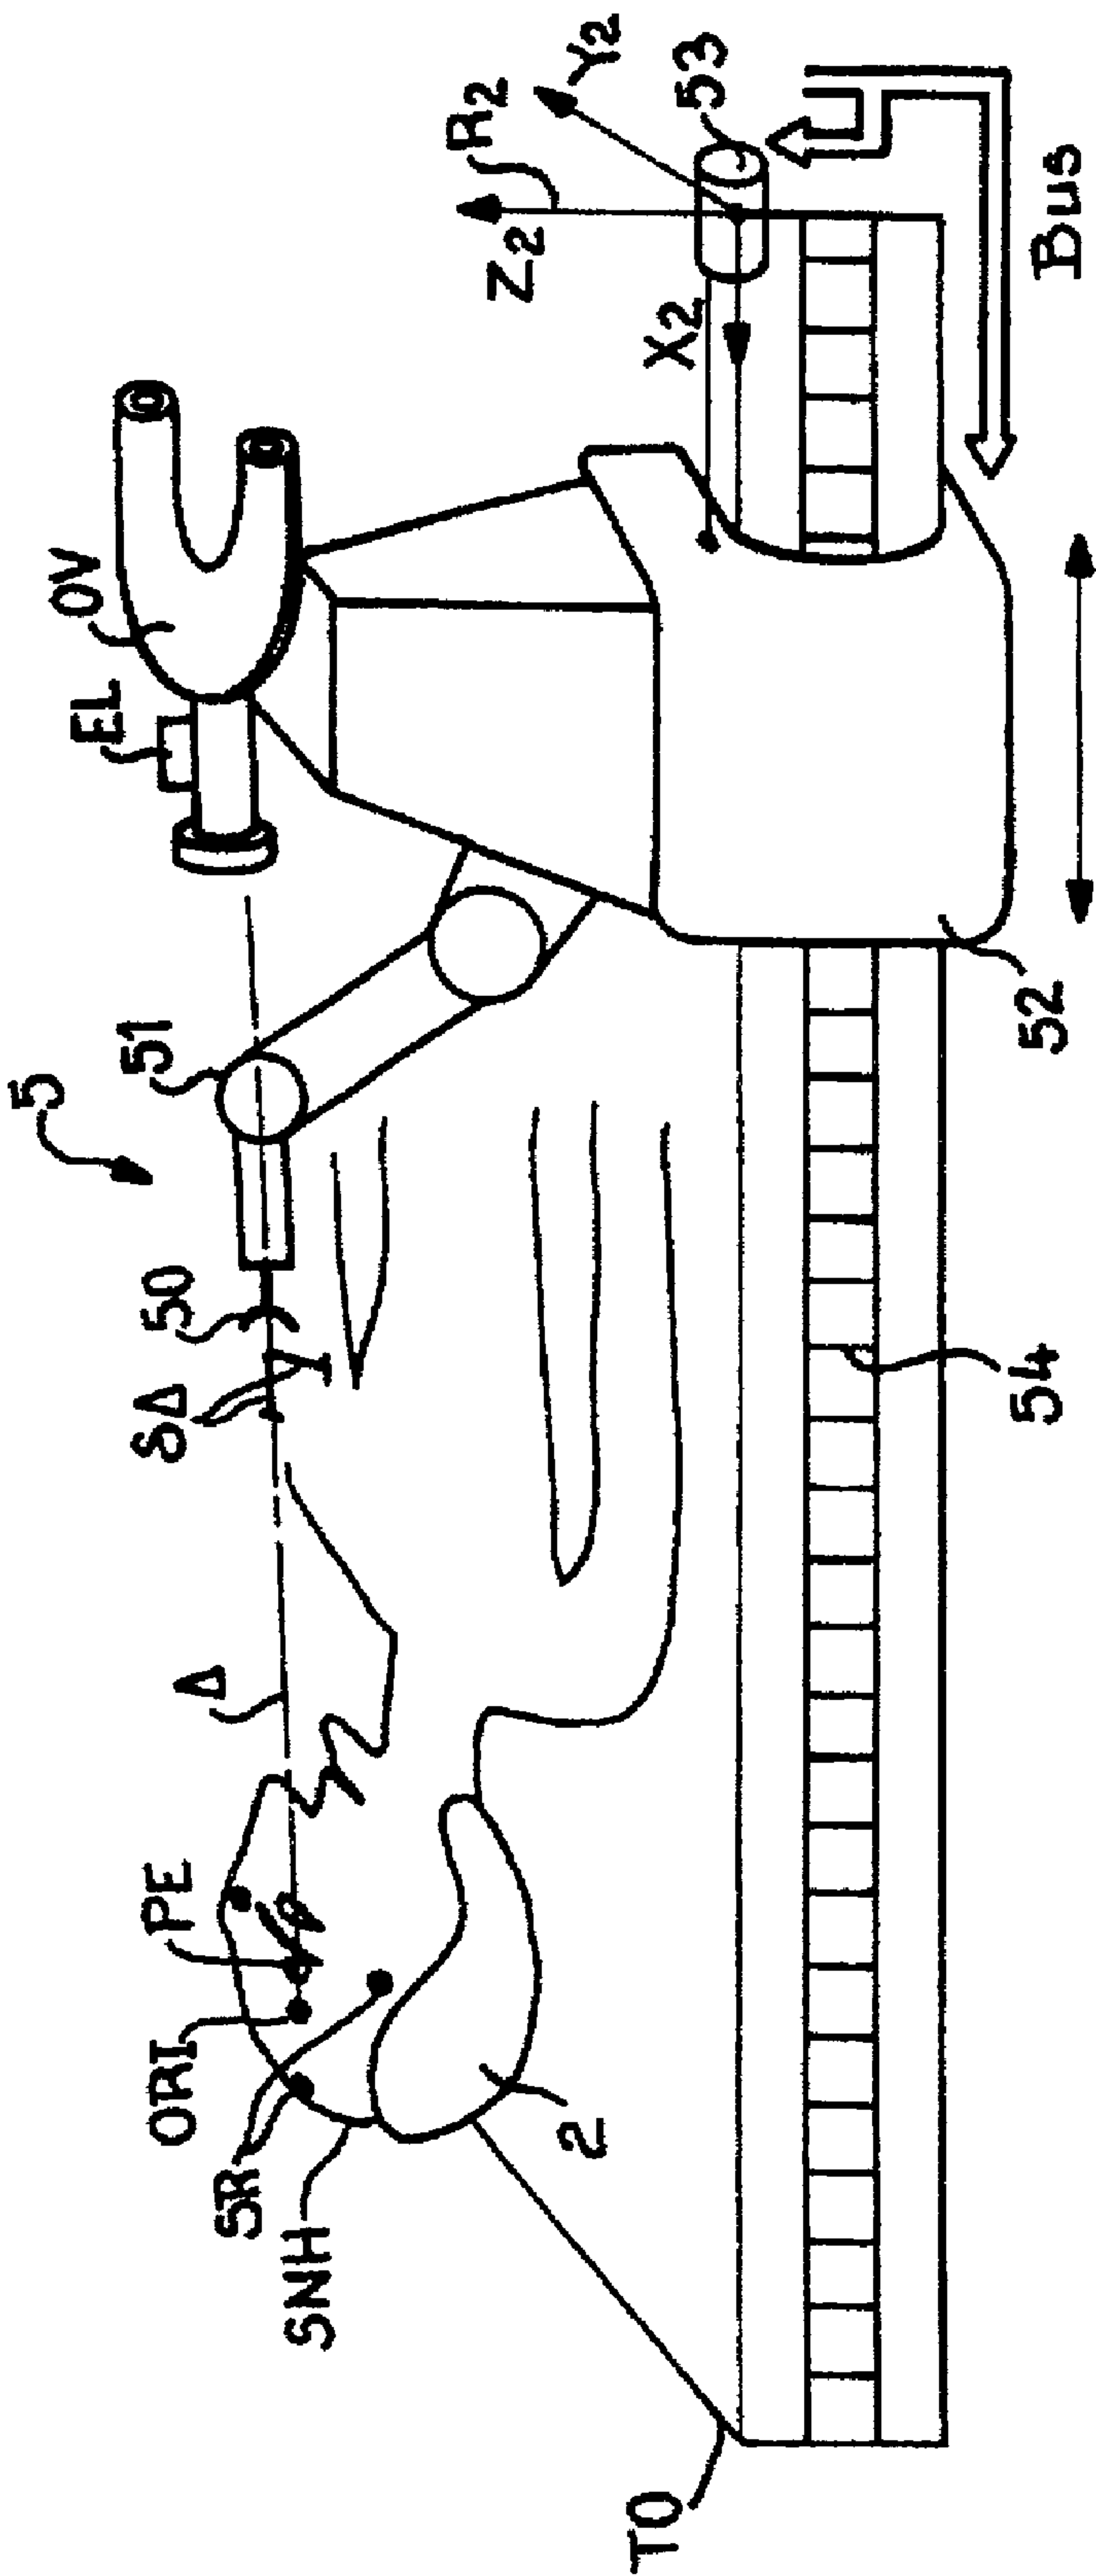
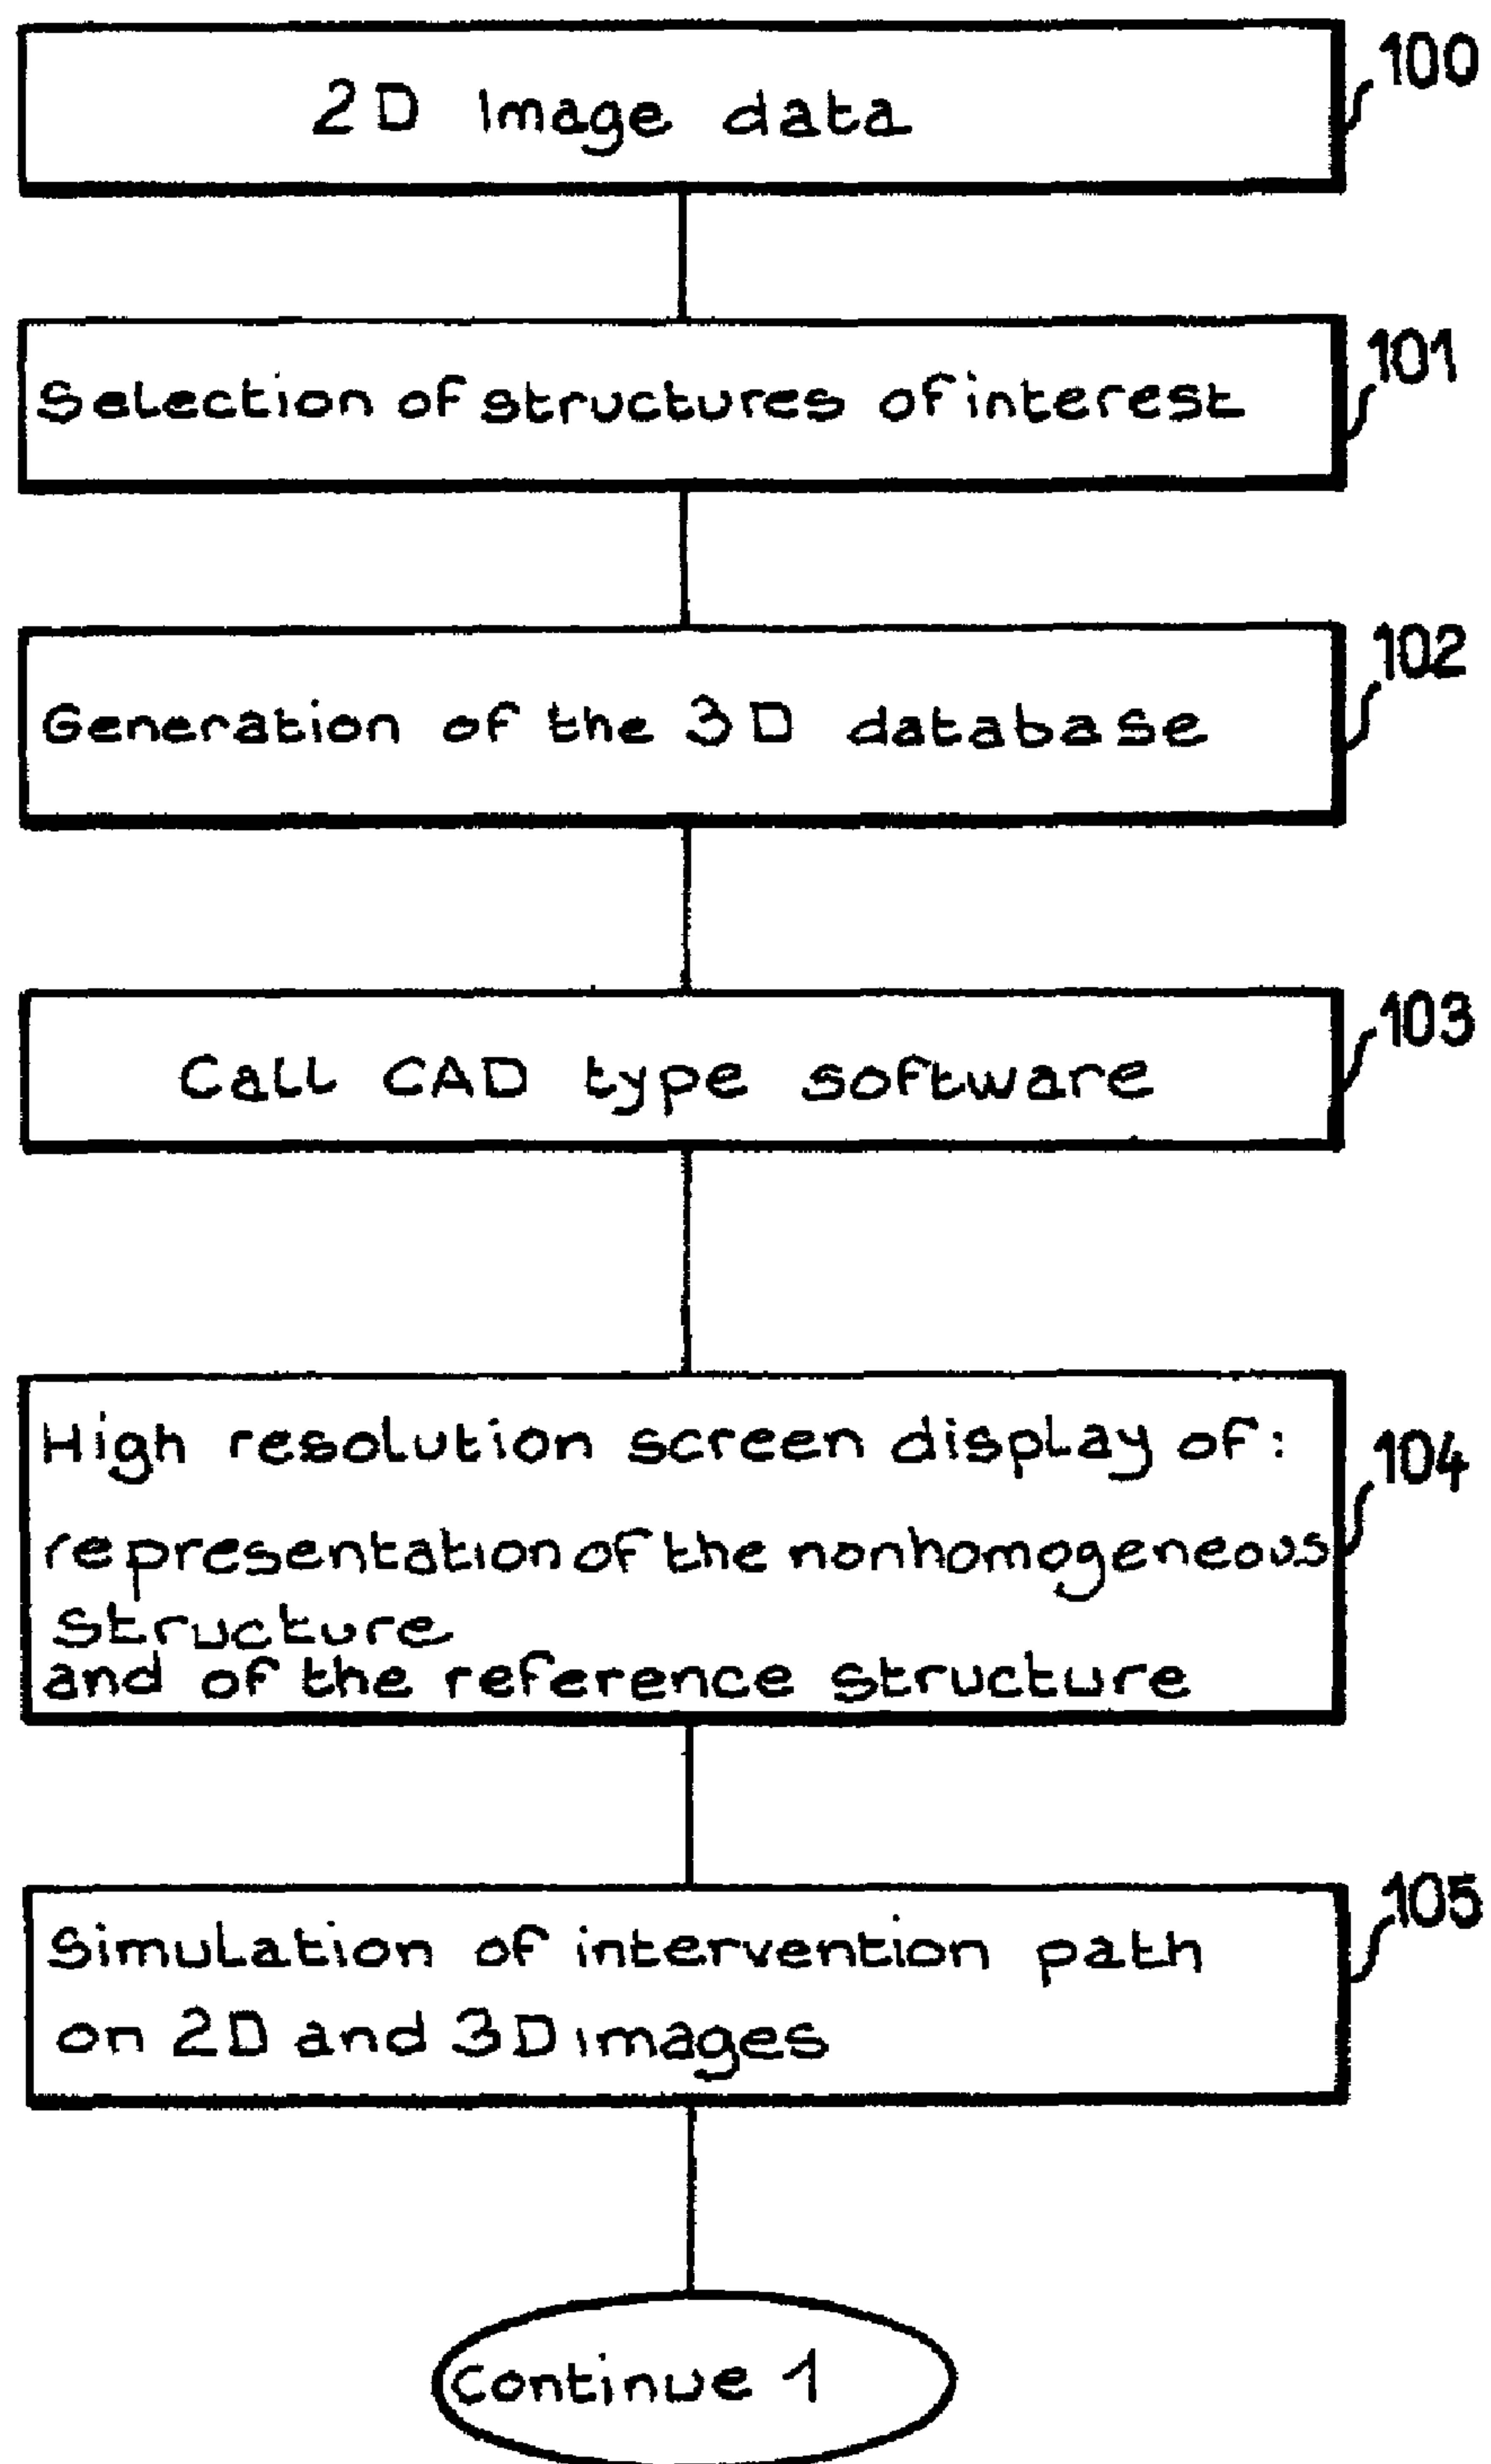


FIG. 3

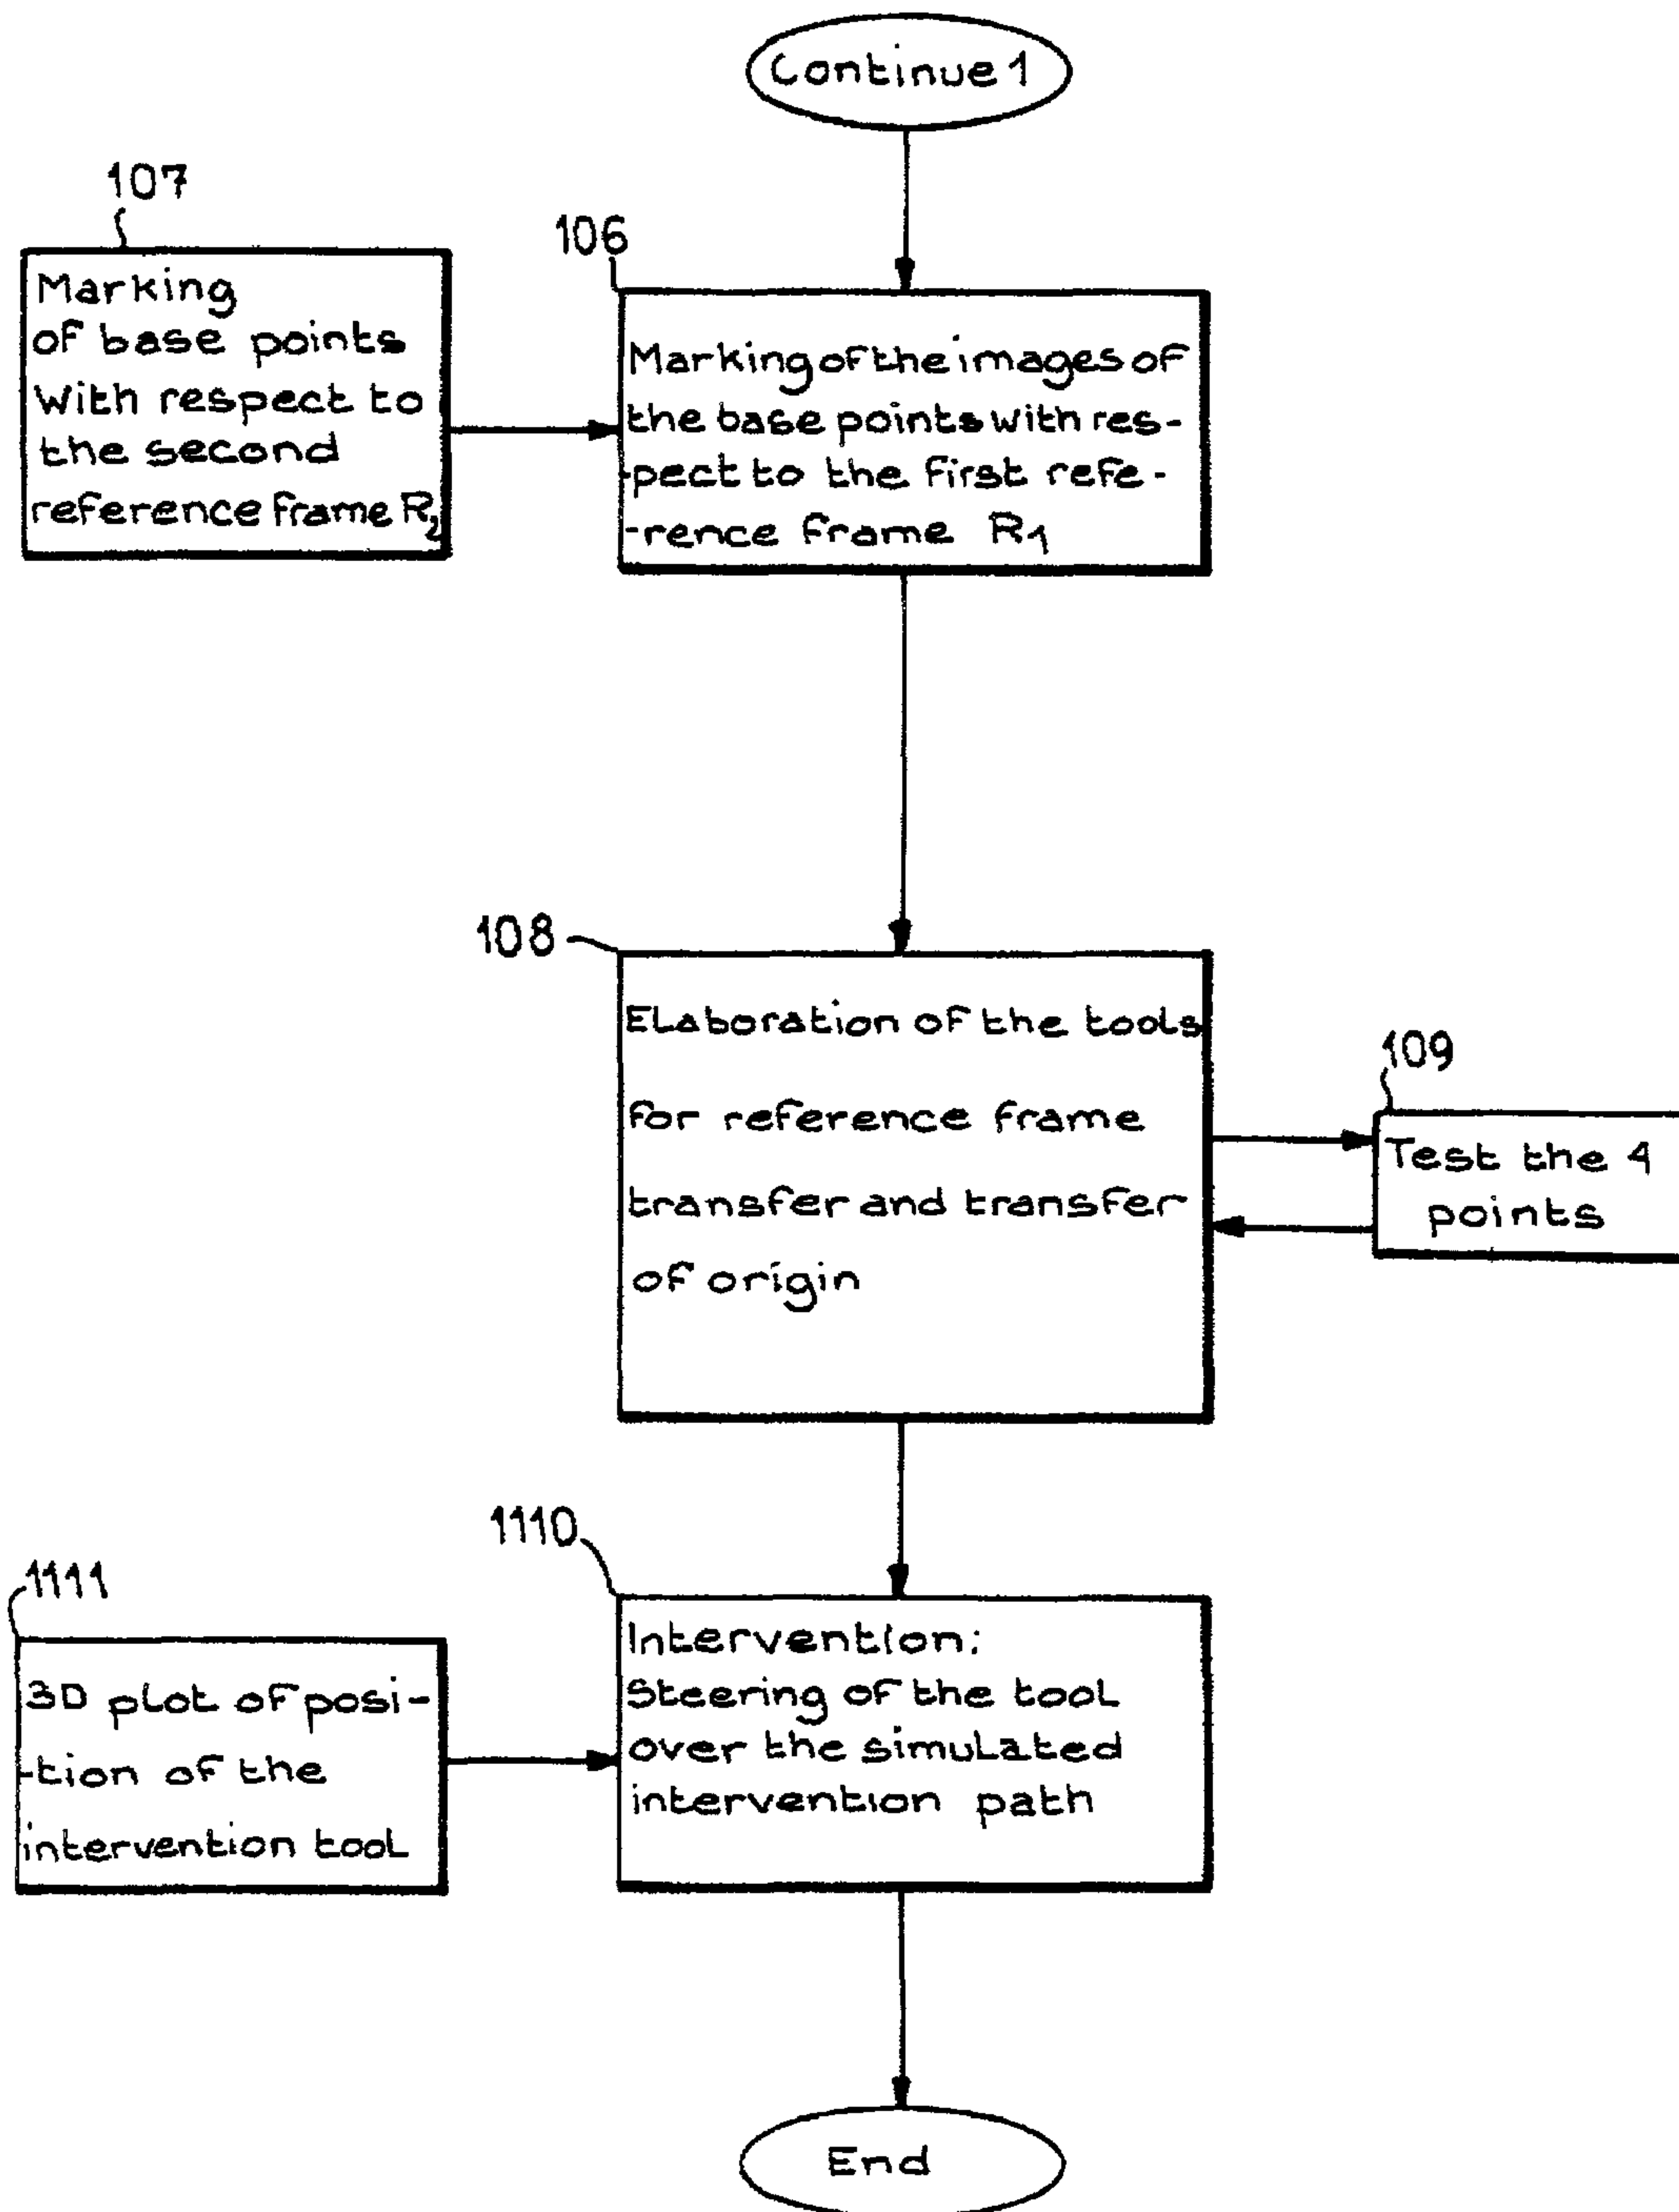

FIG. 5a

FIG. 5b

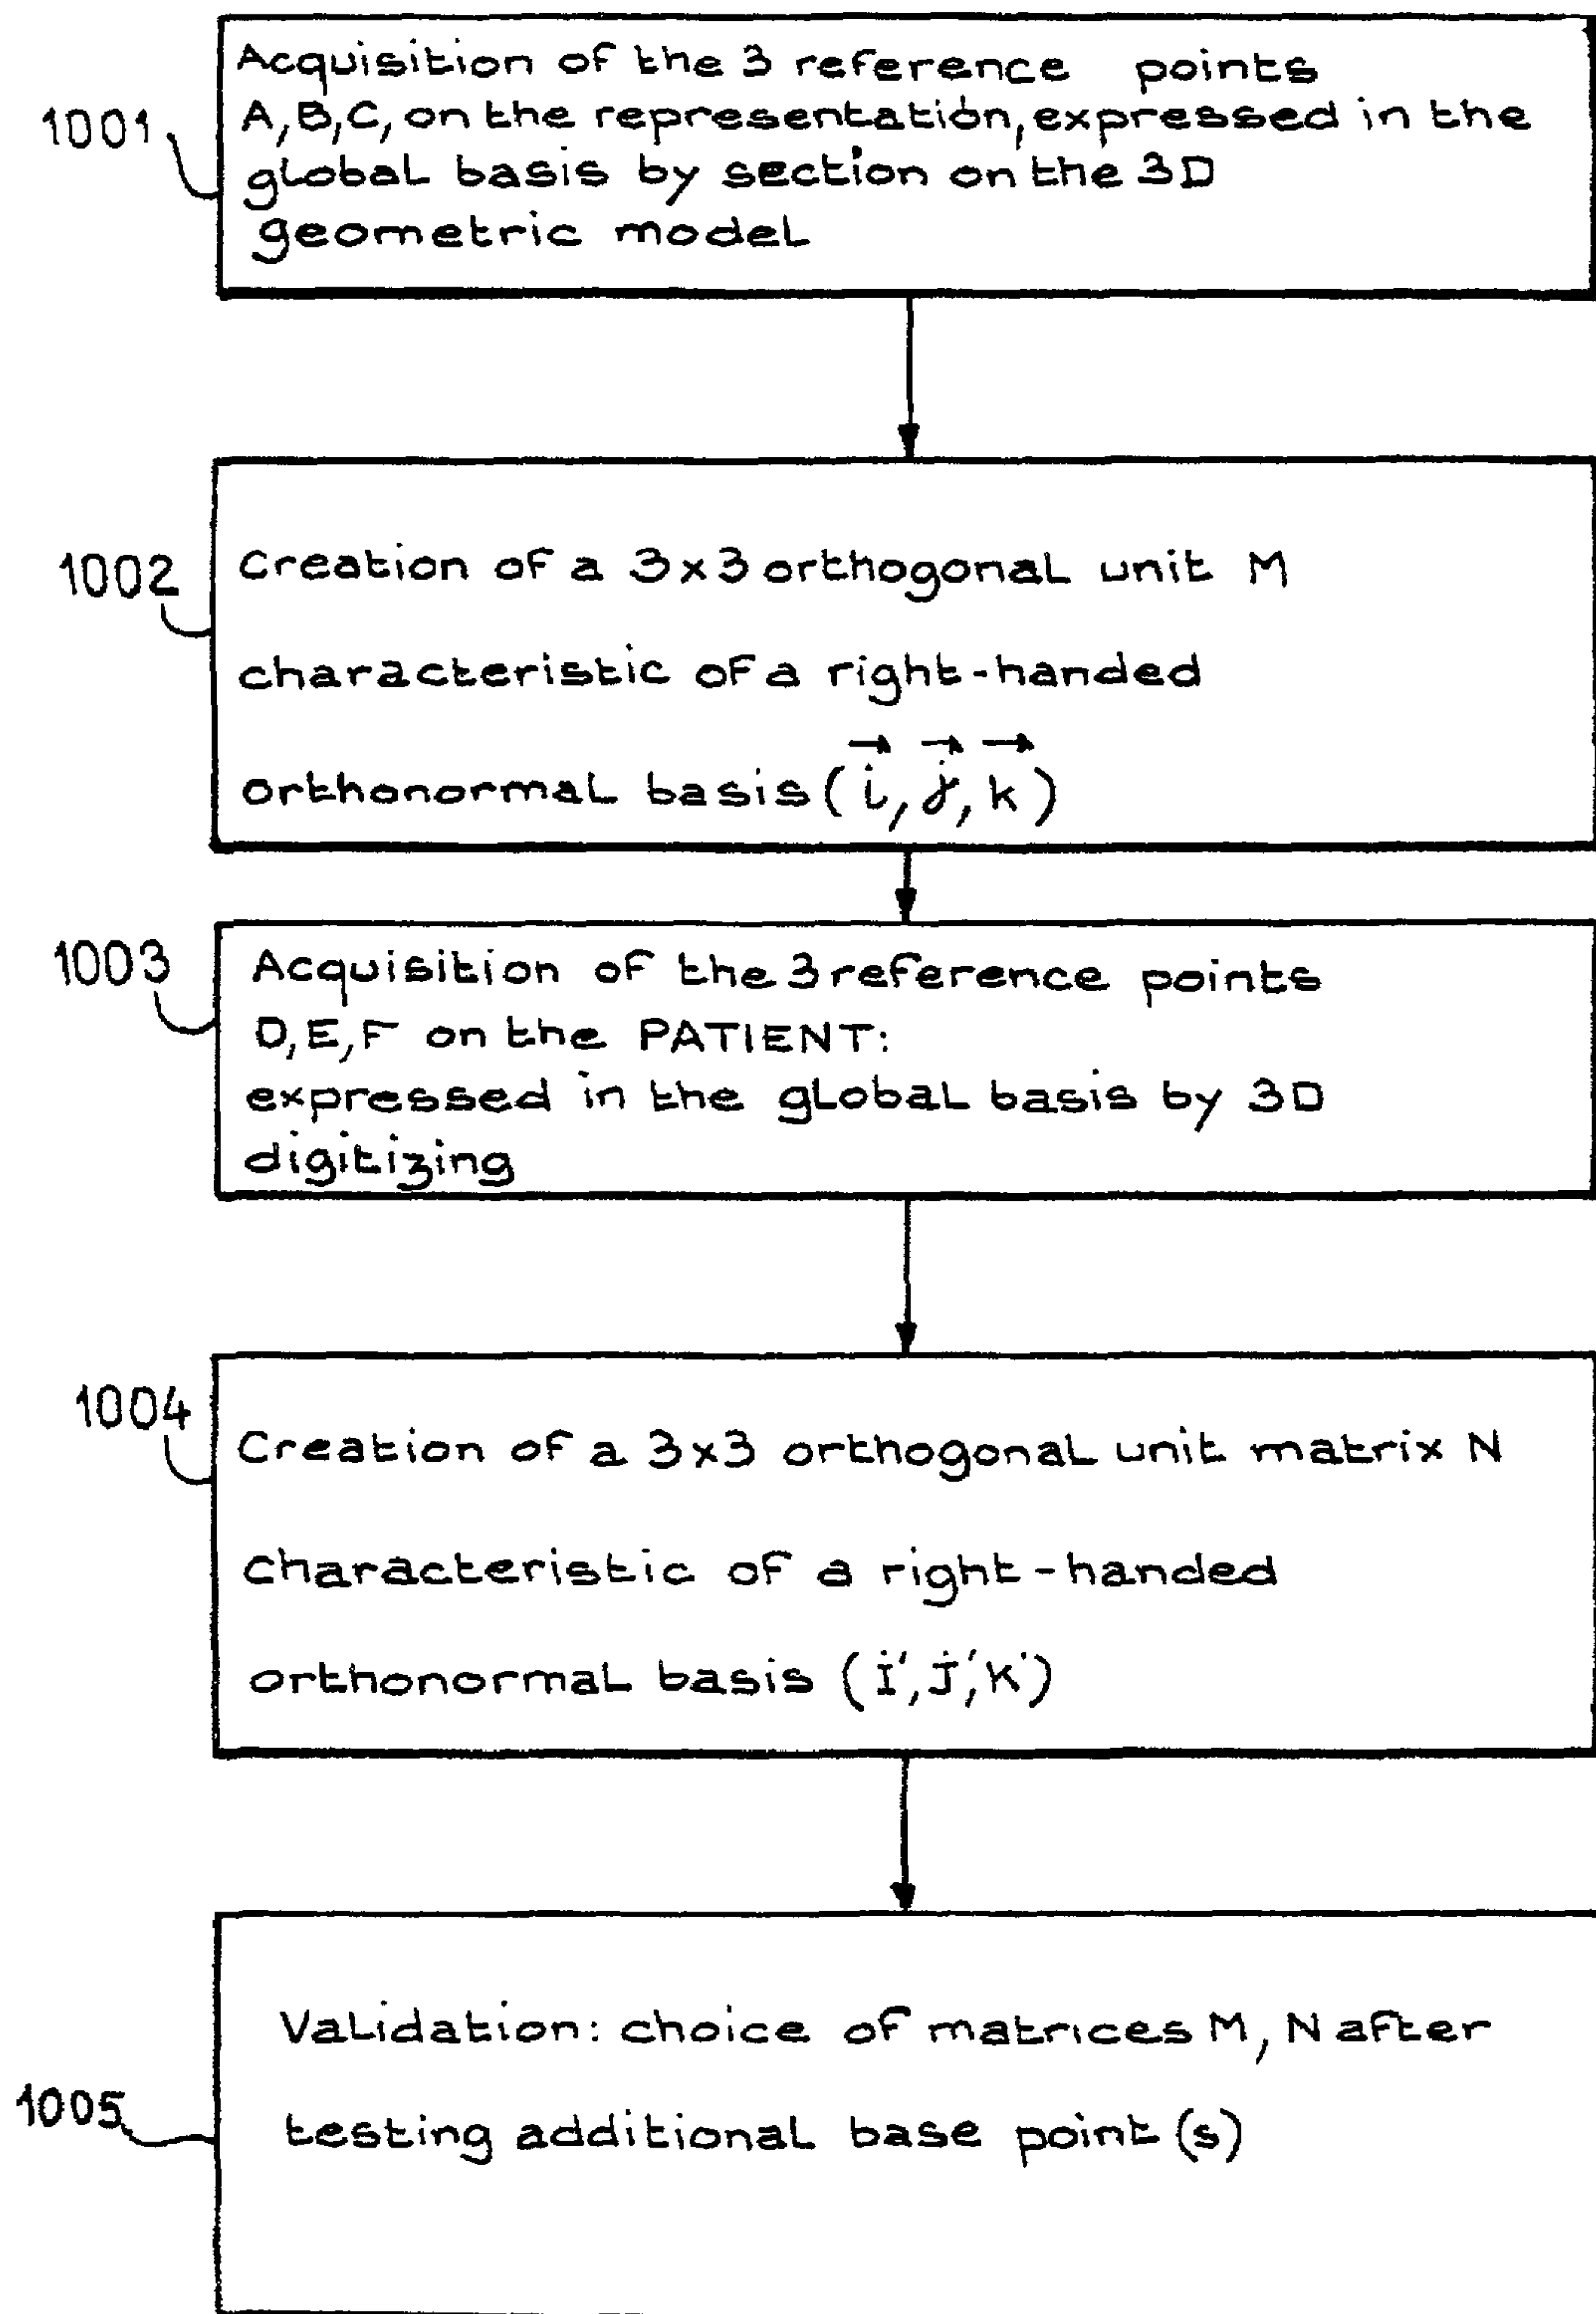
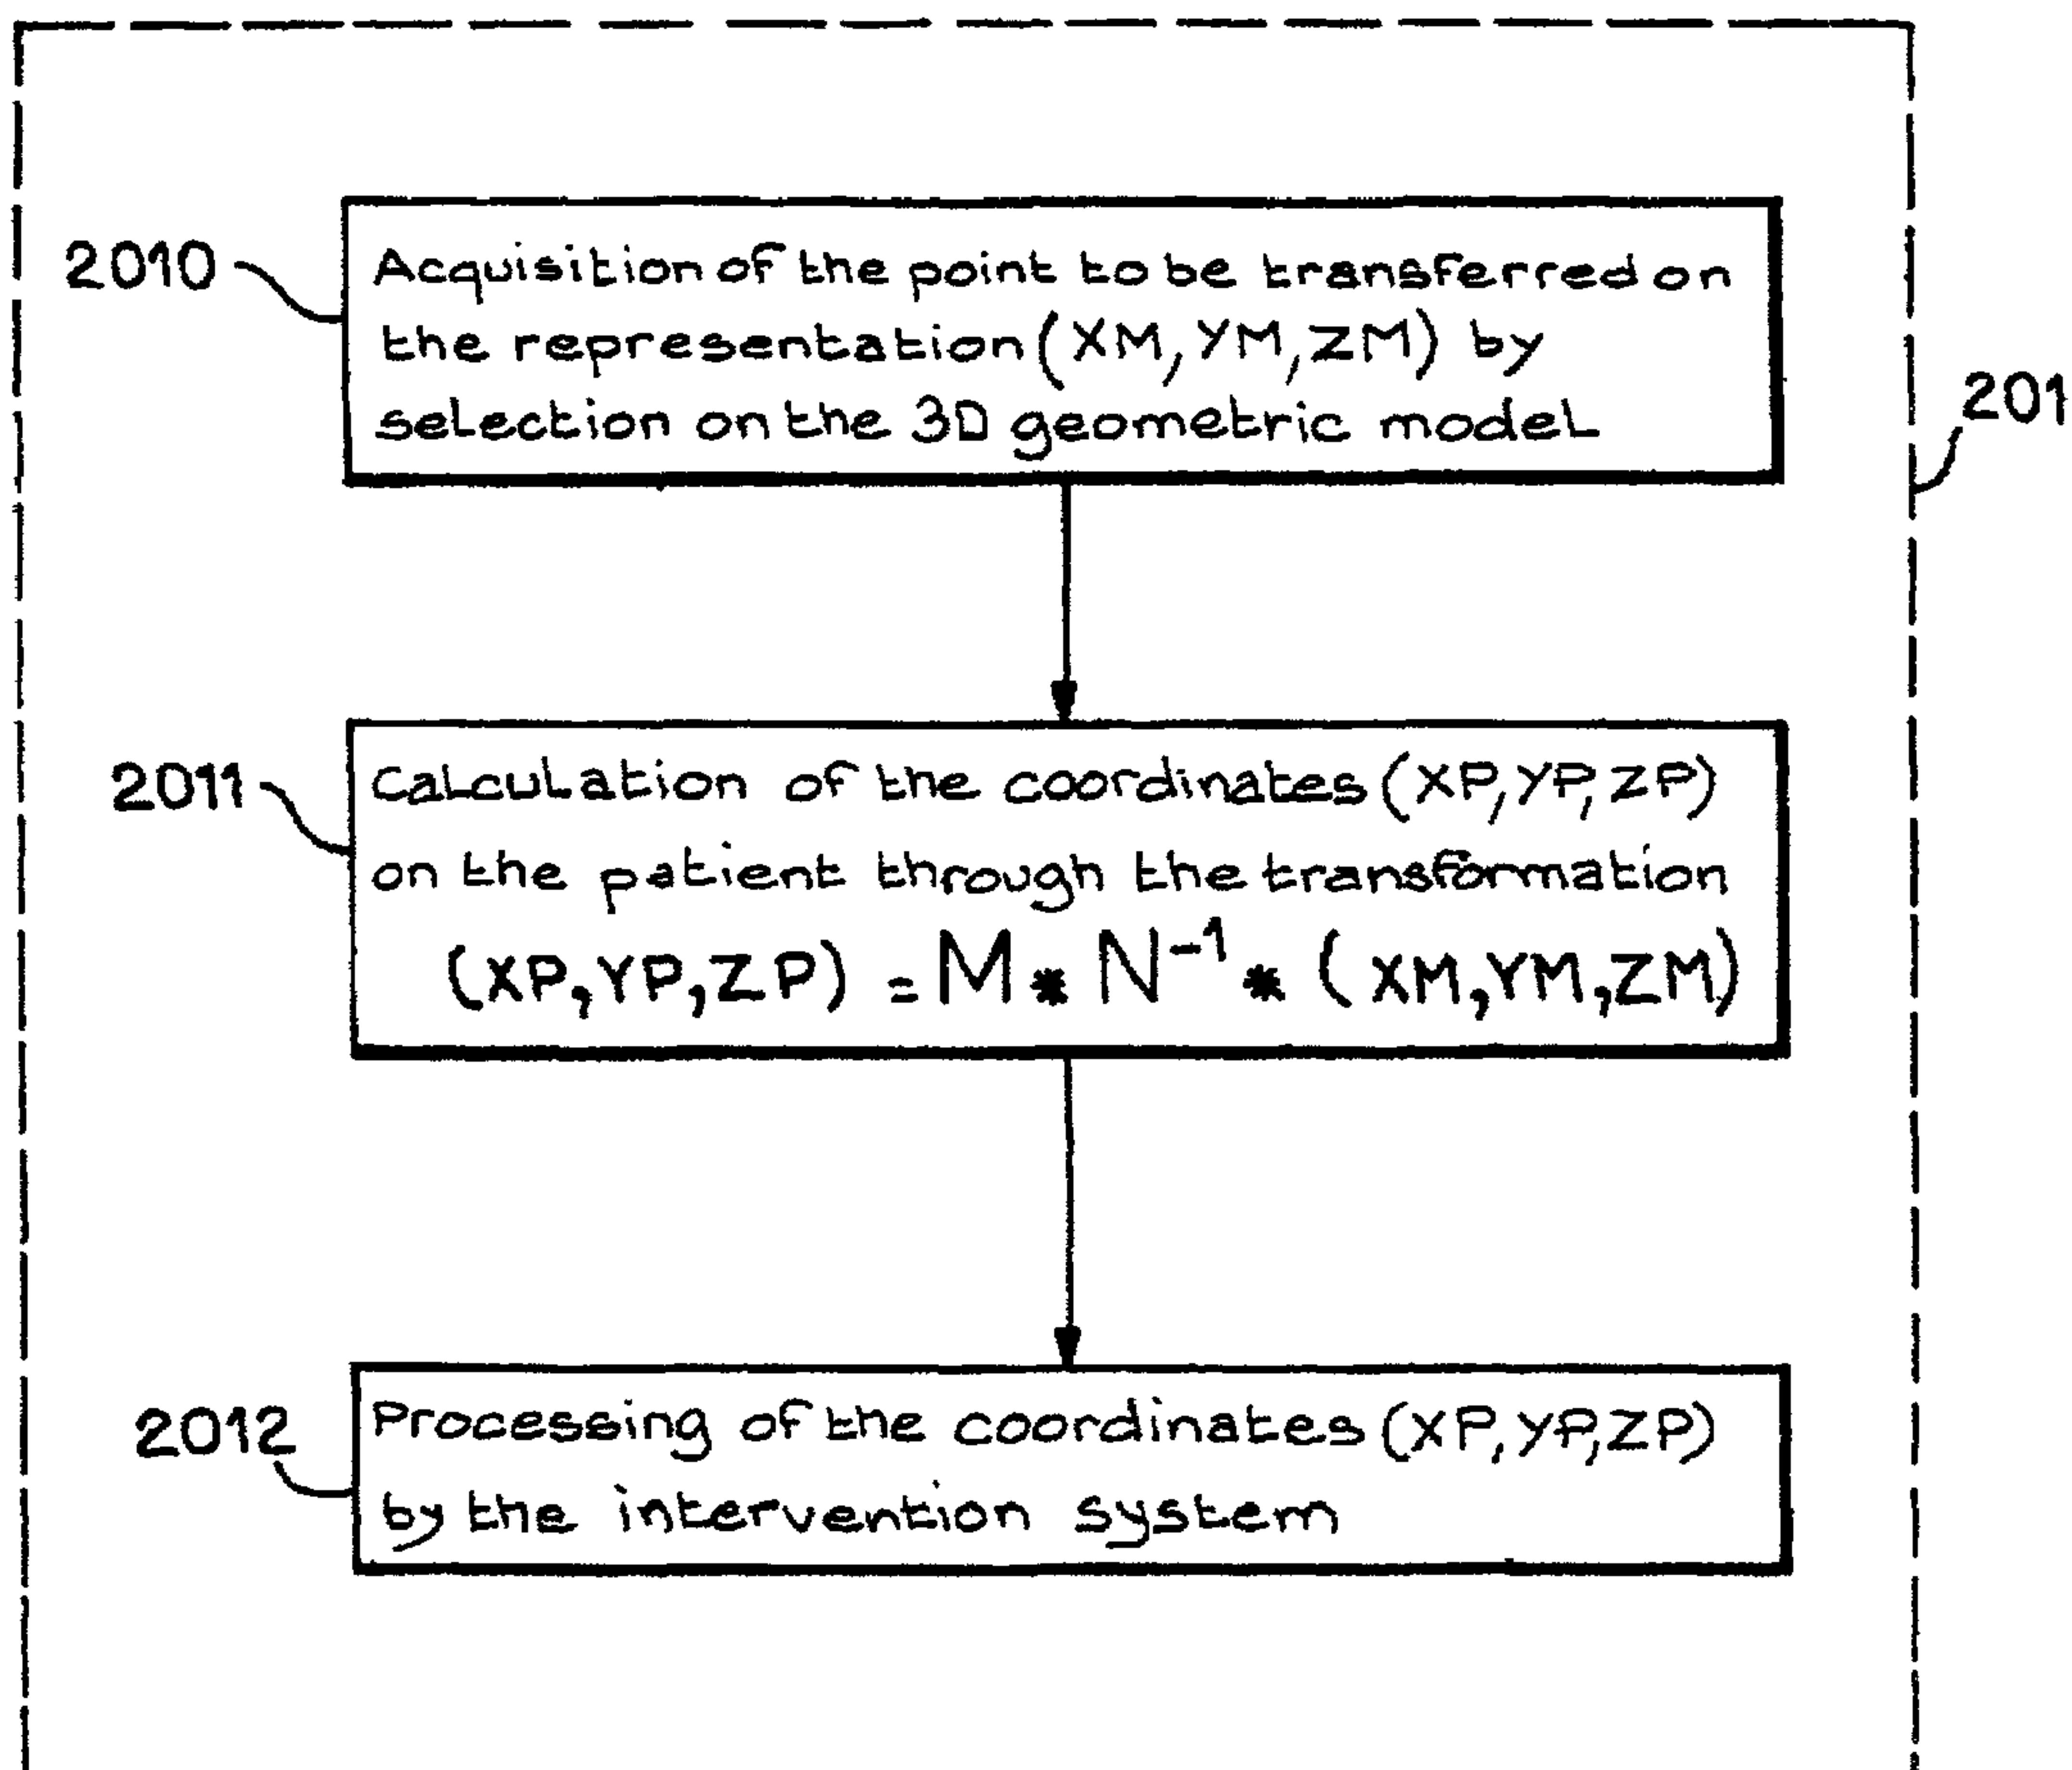
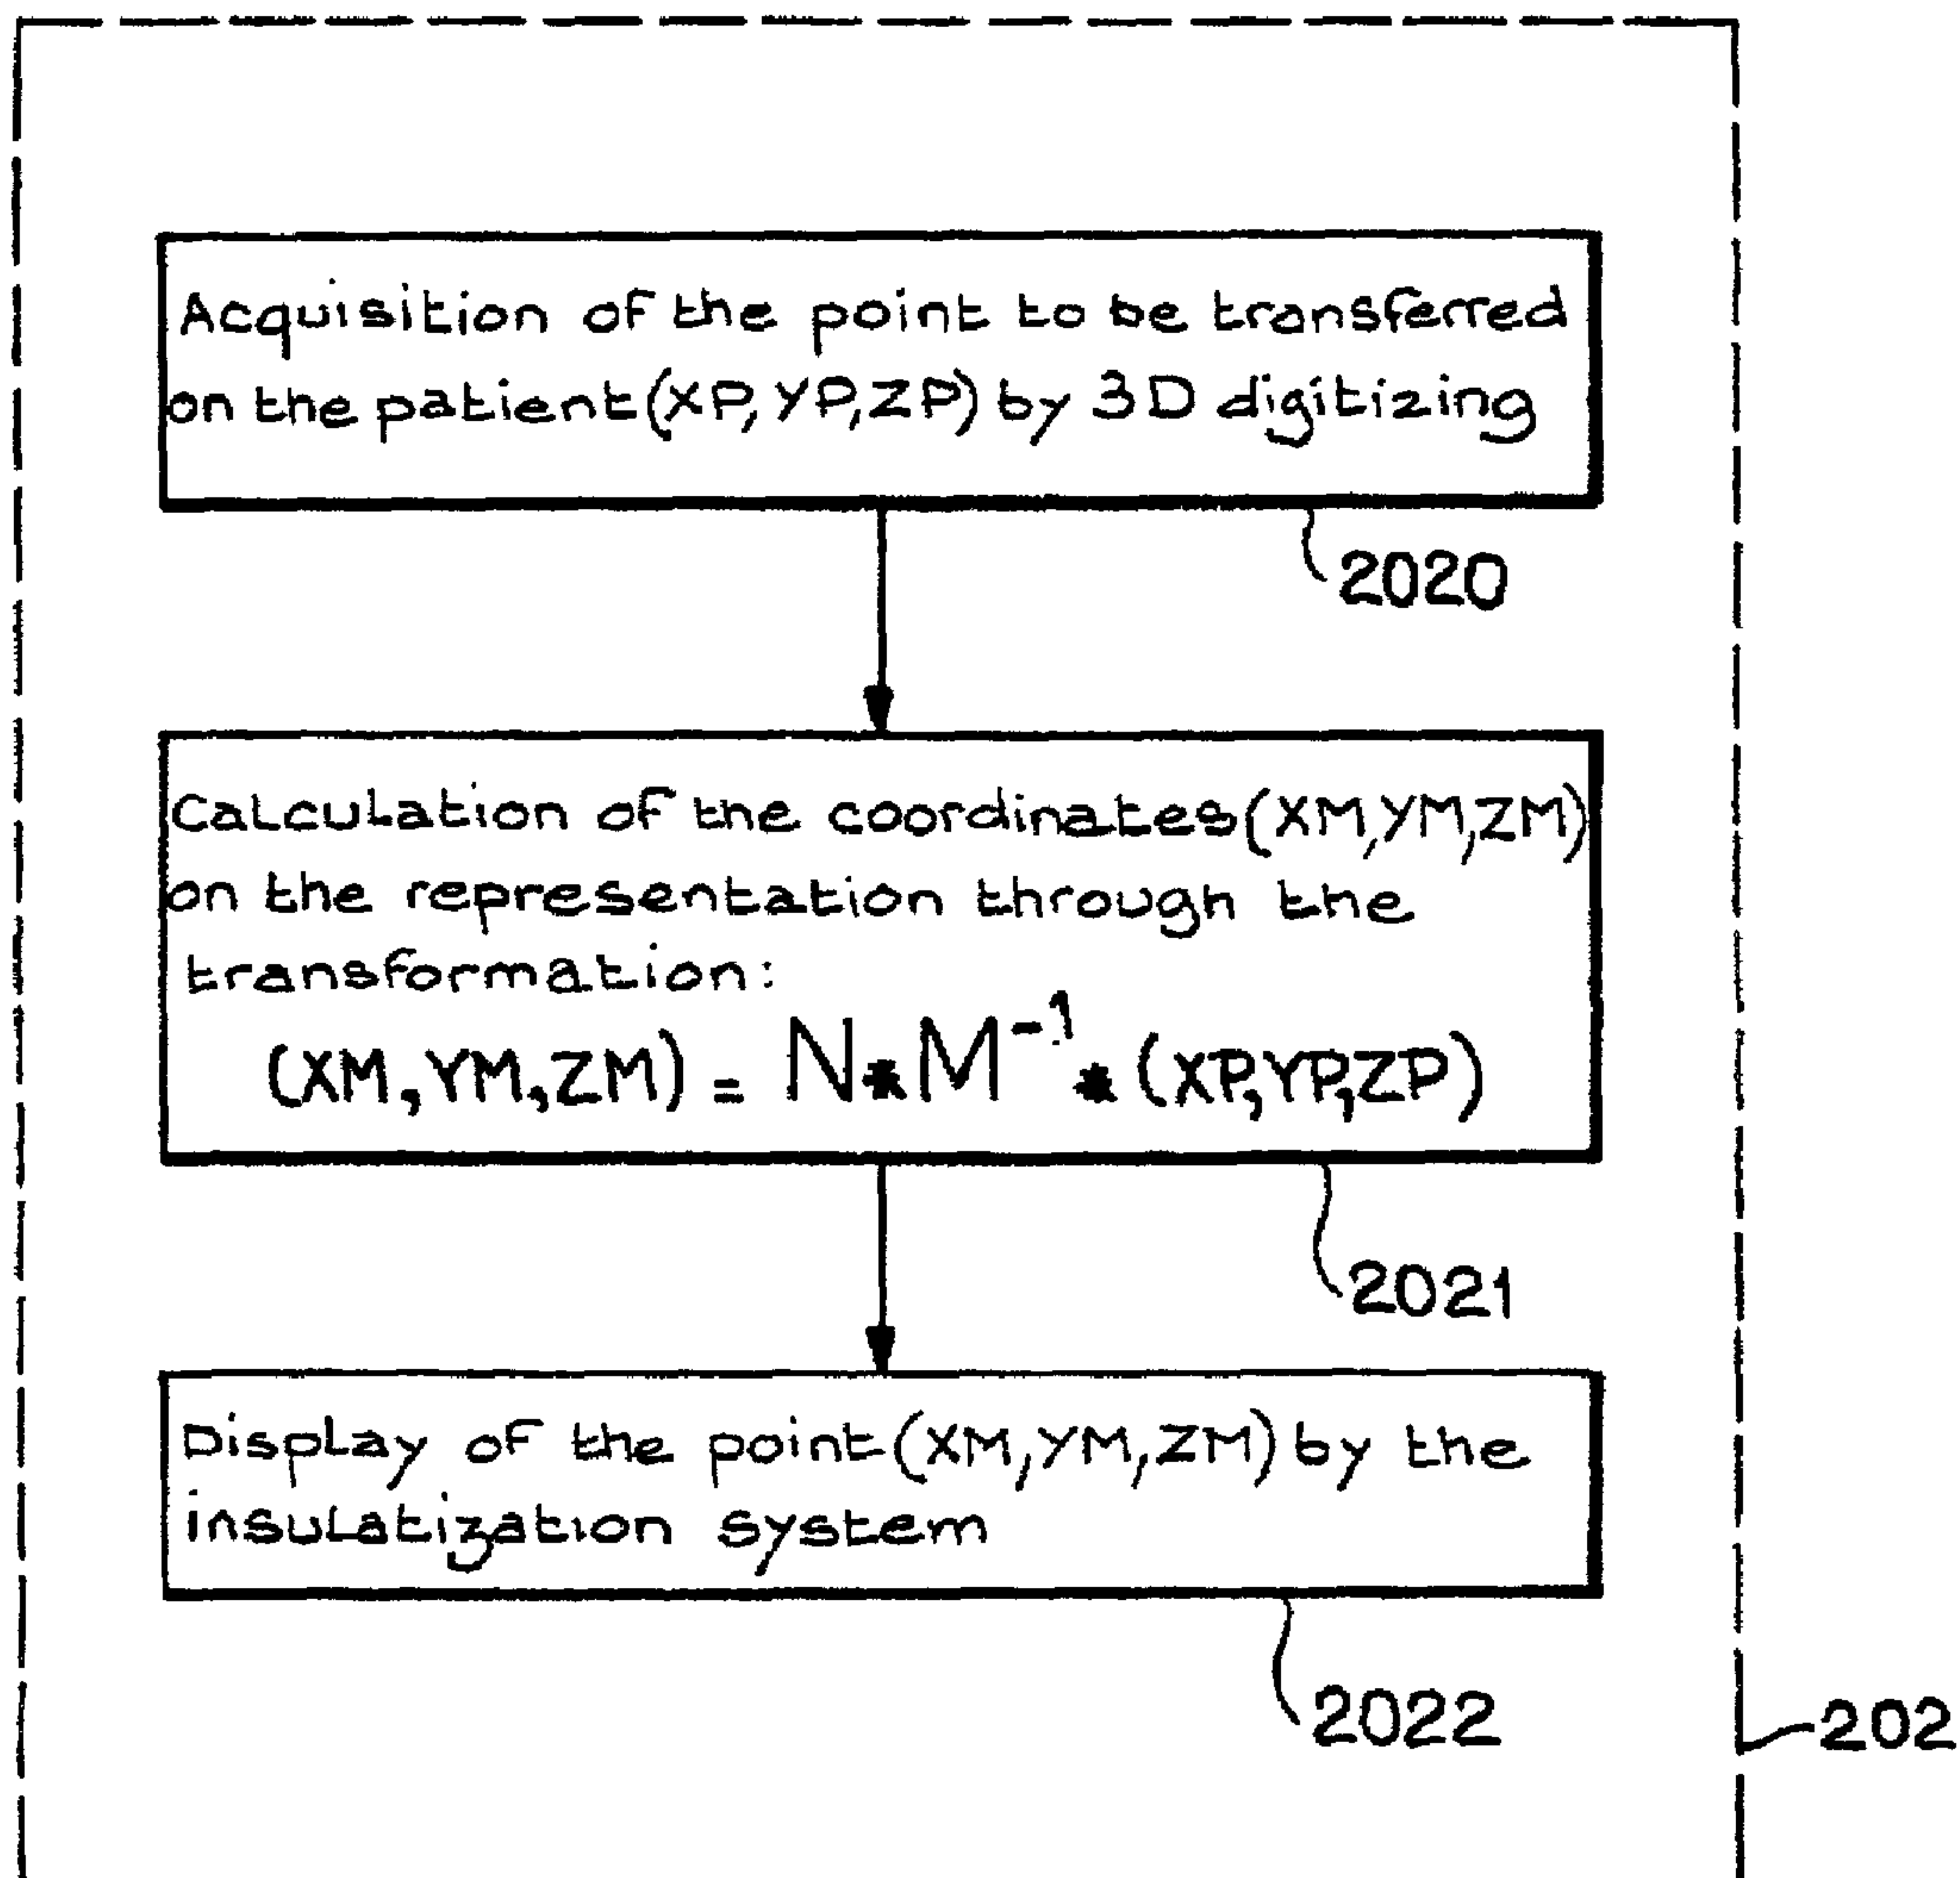


FIG 6

FIG. 7

FIG. 8

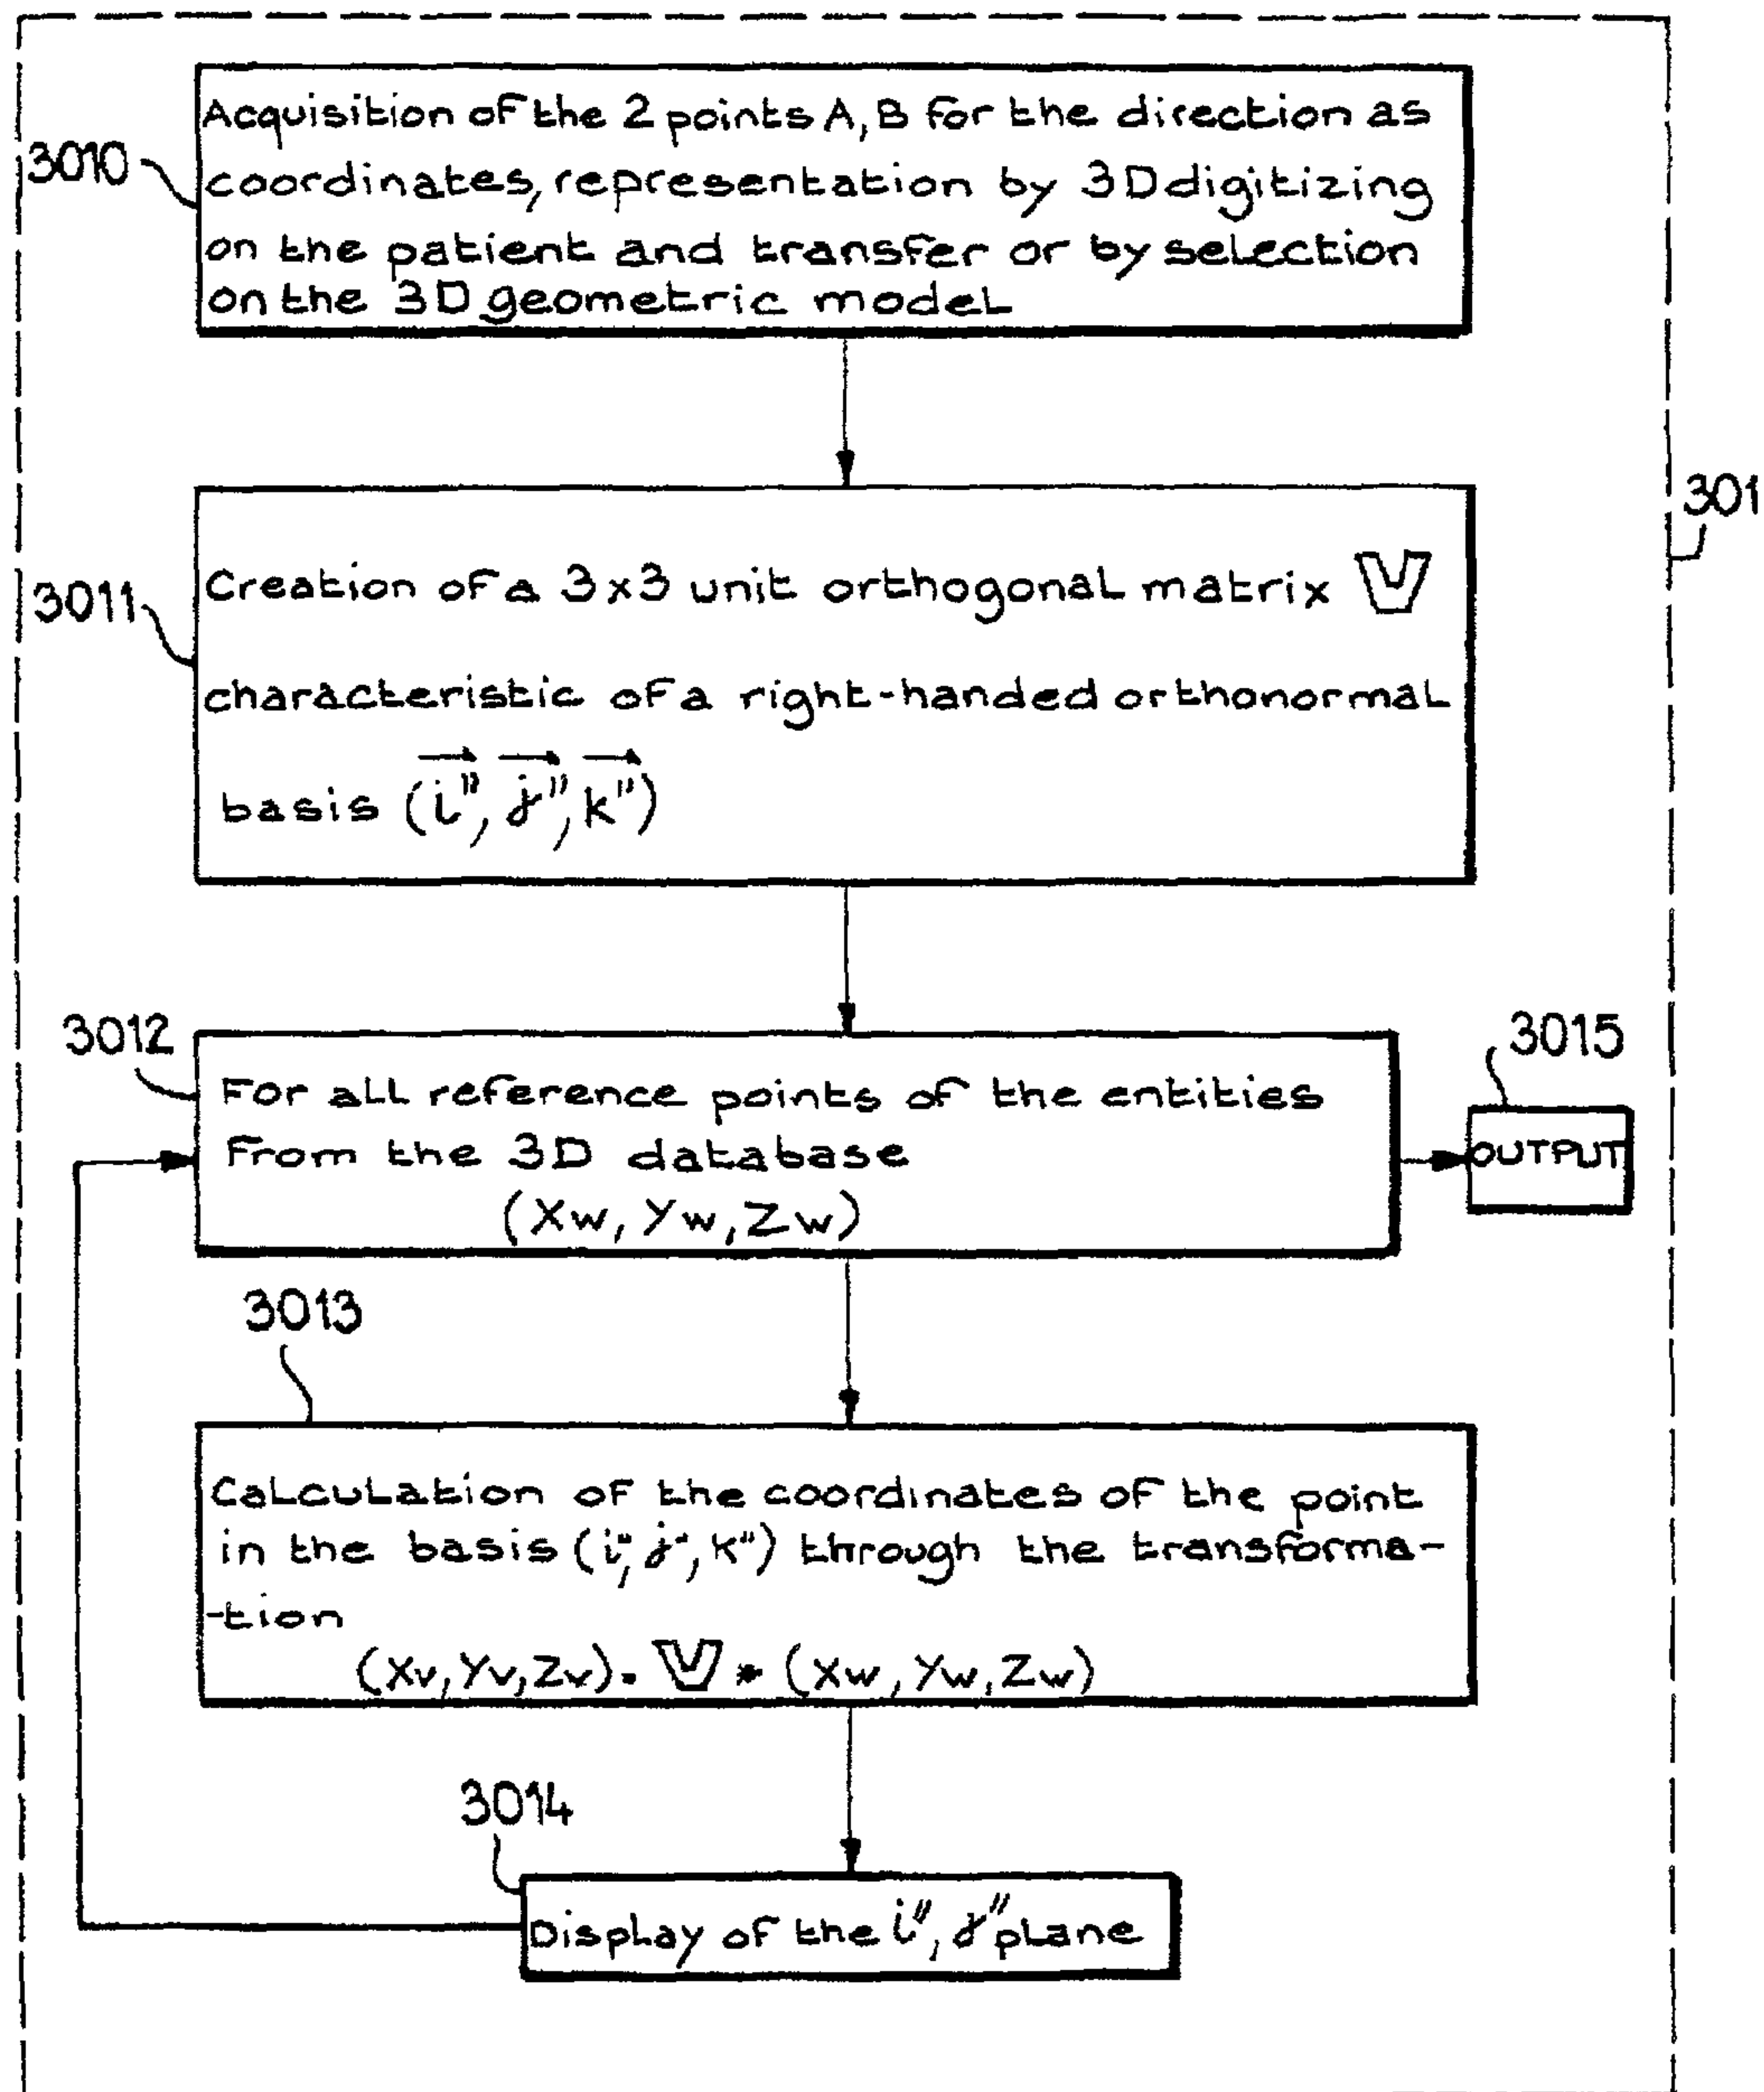
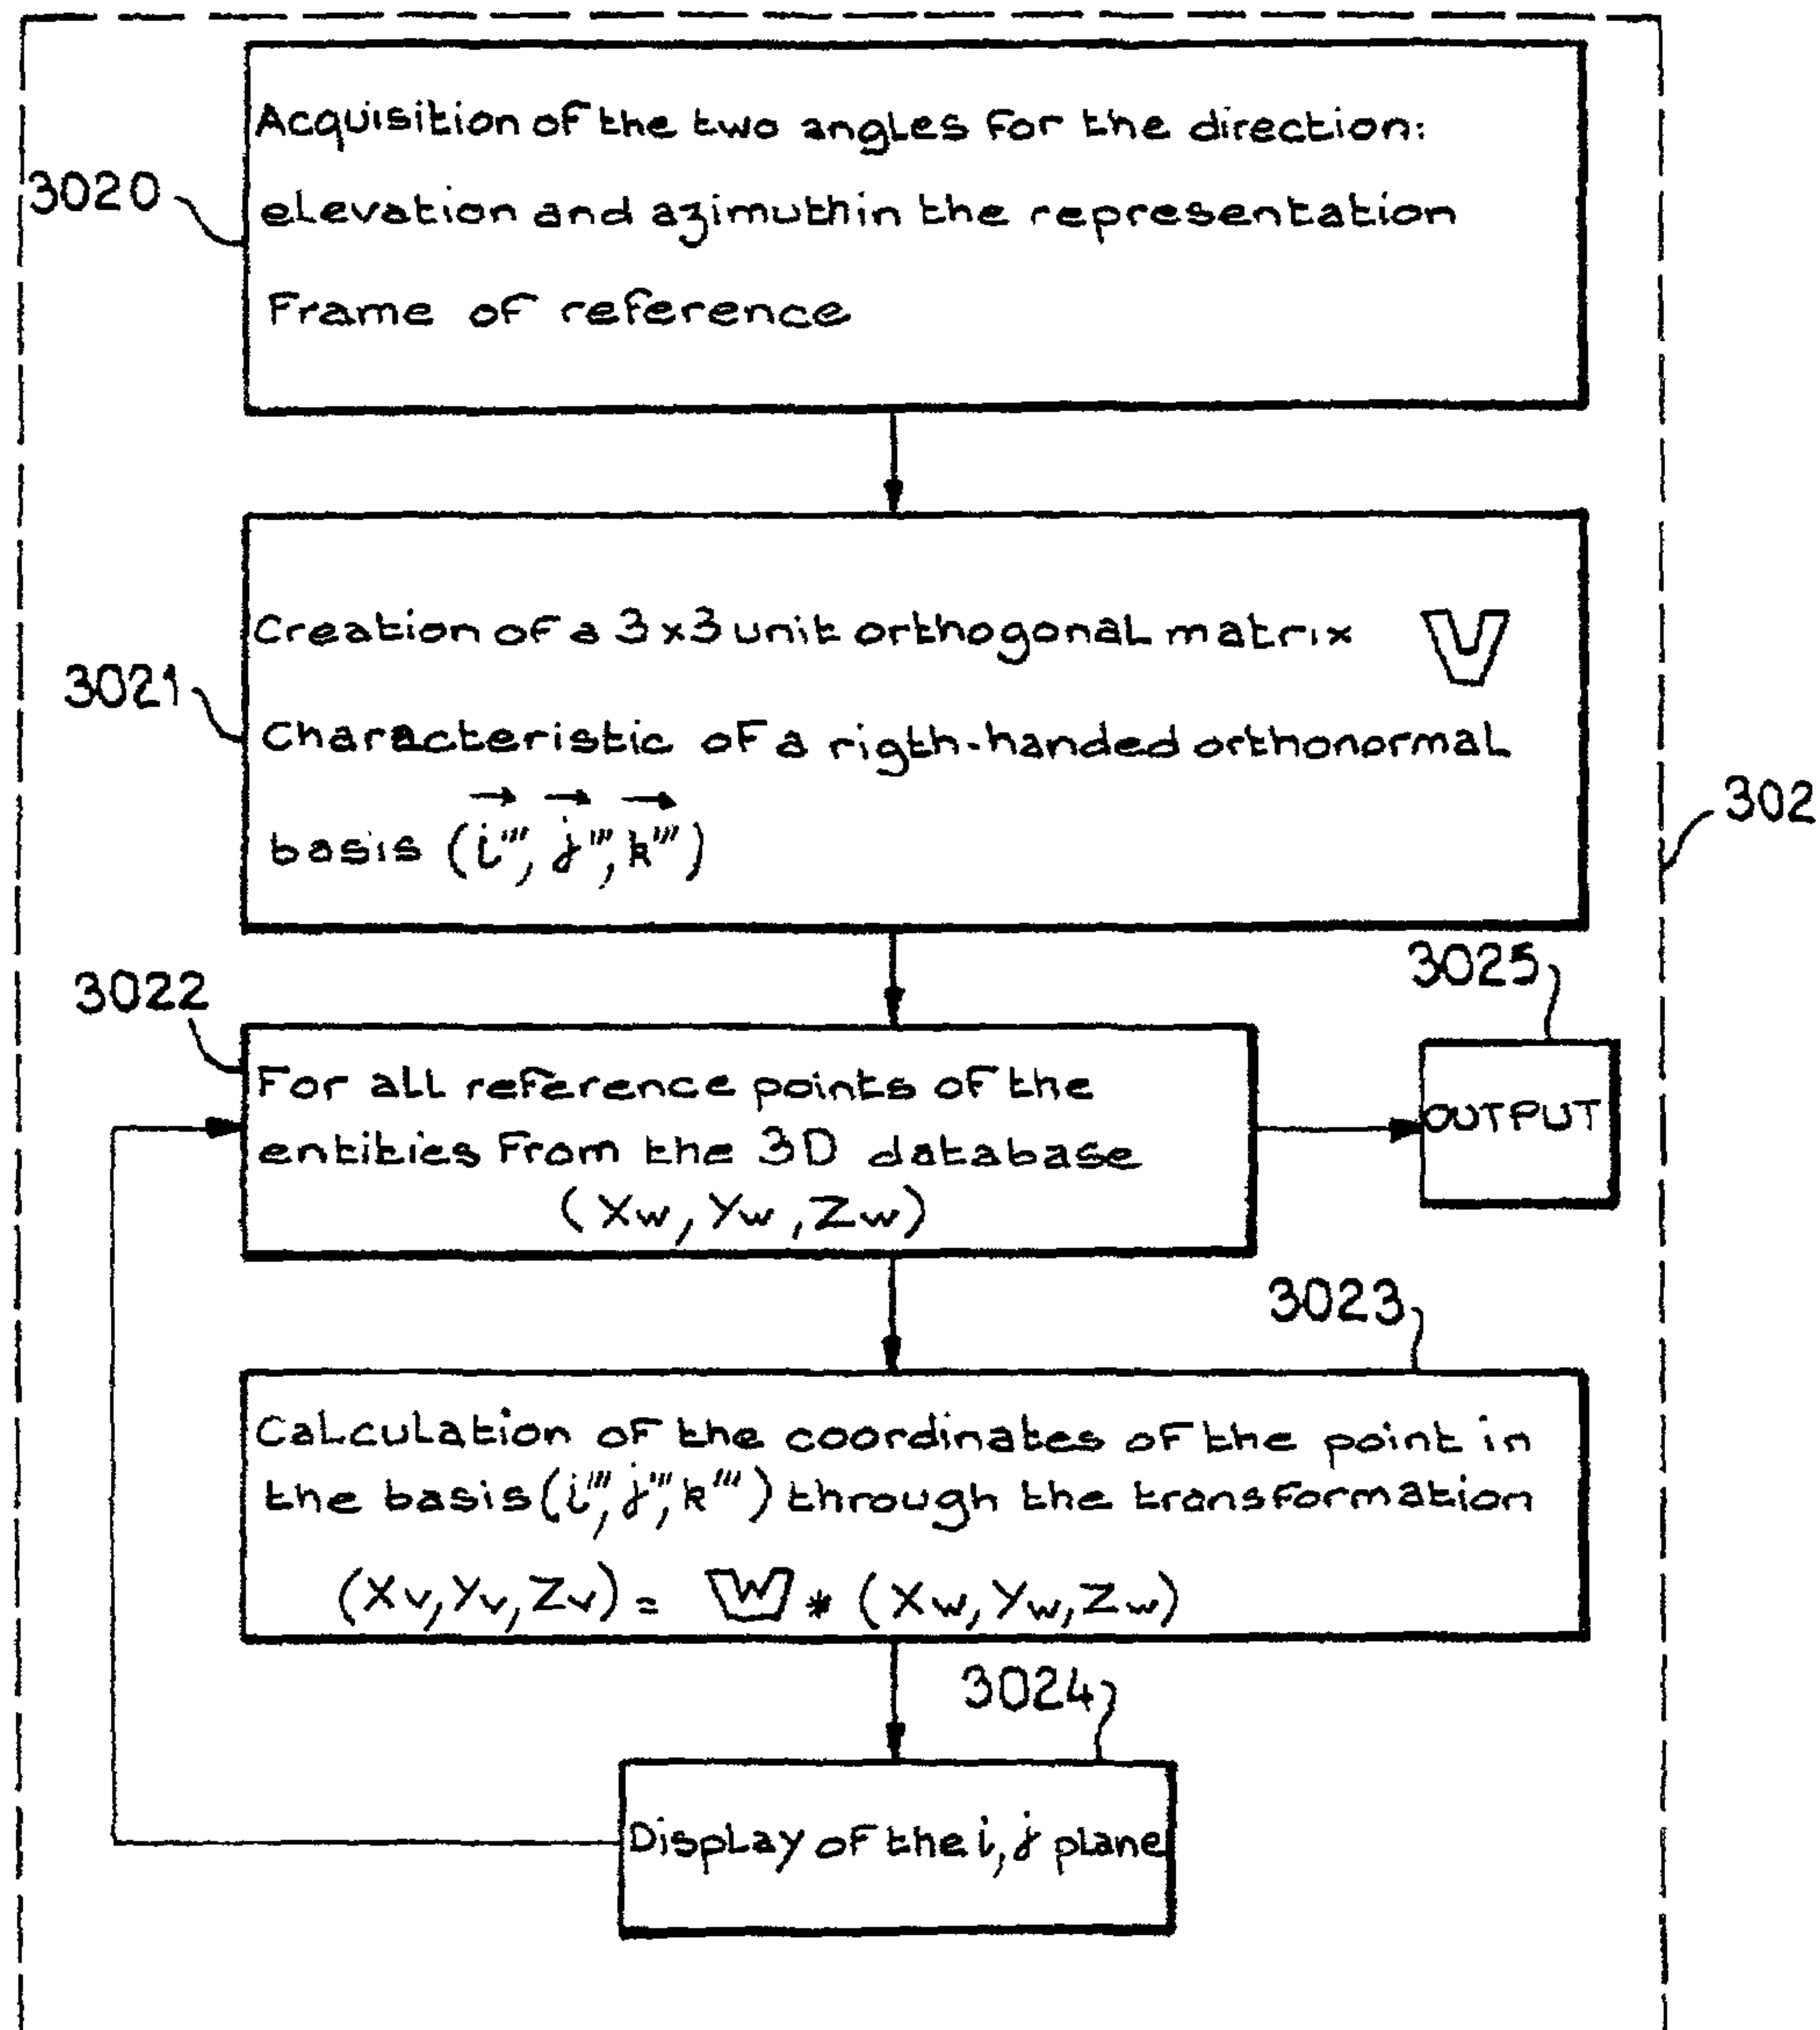


FIG. 9a

FIG_9b

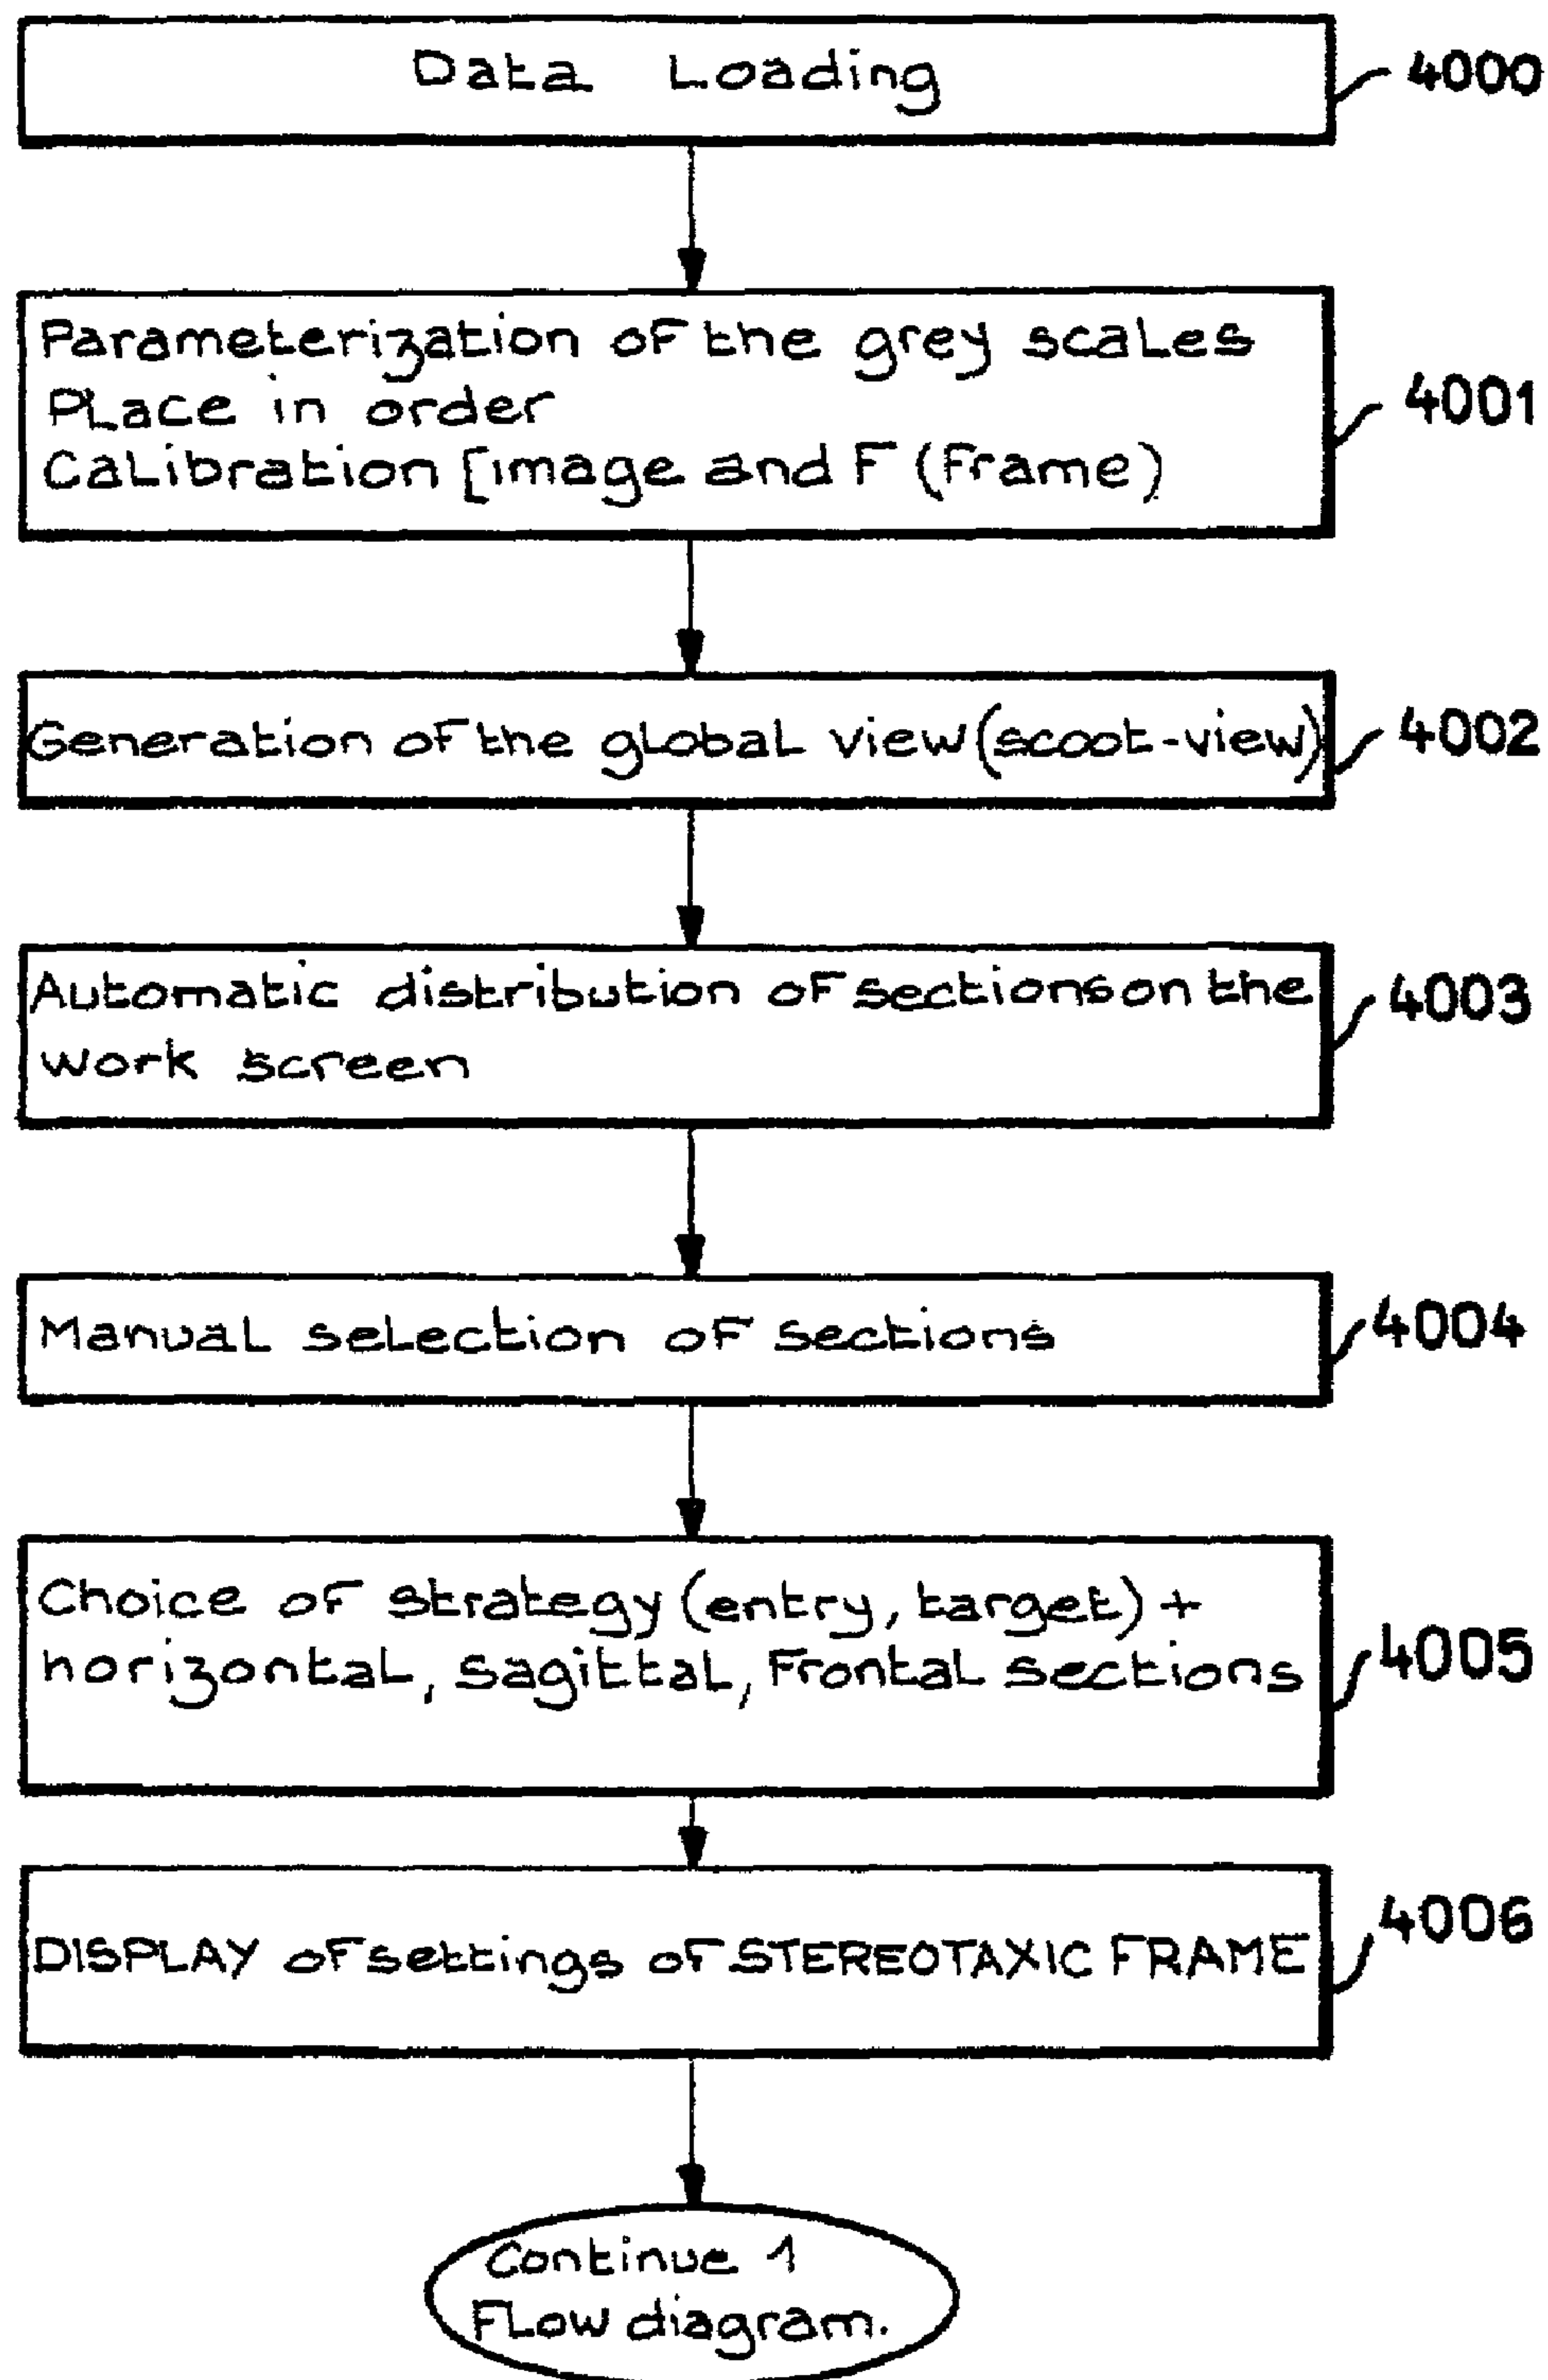
FIG. 10a


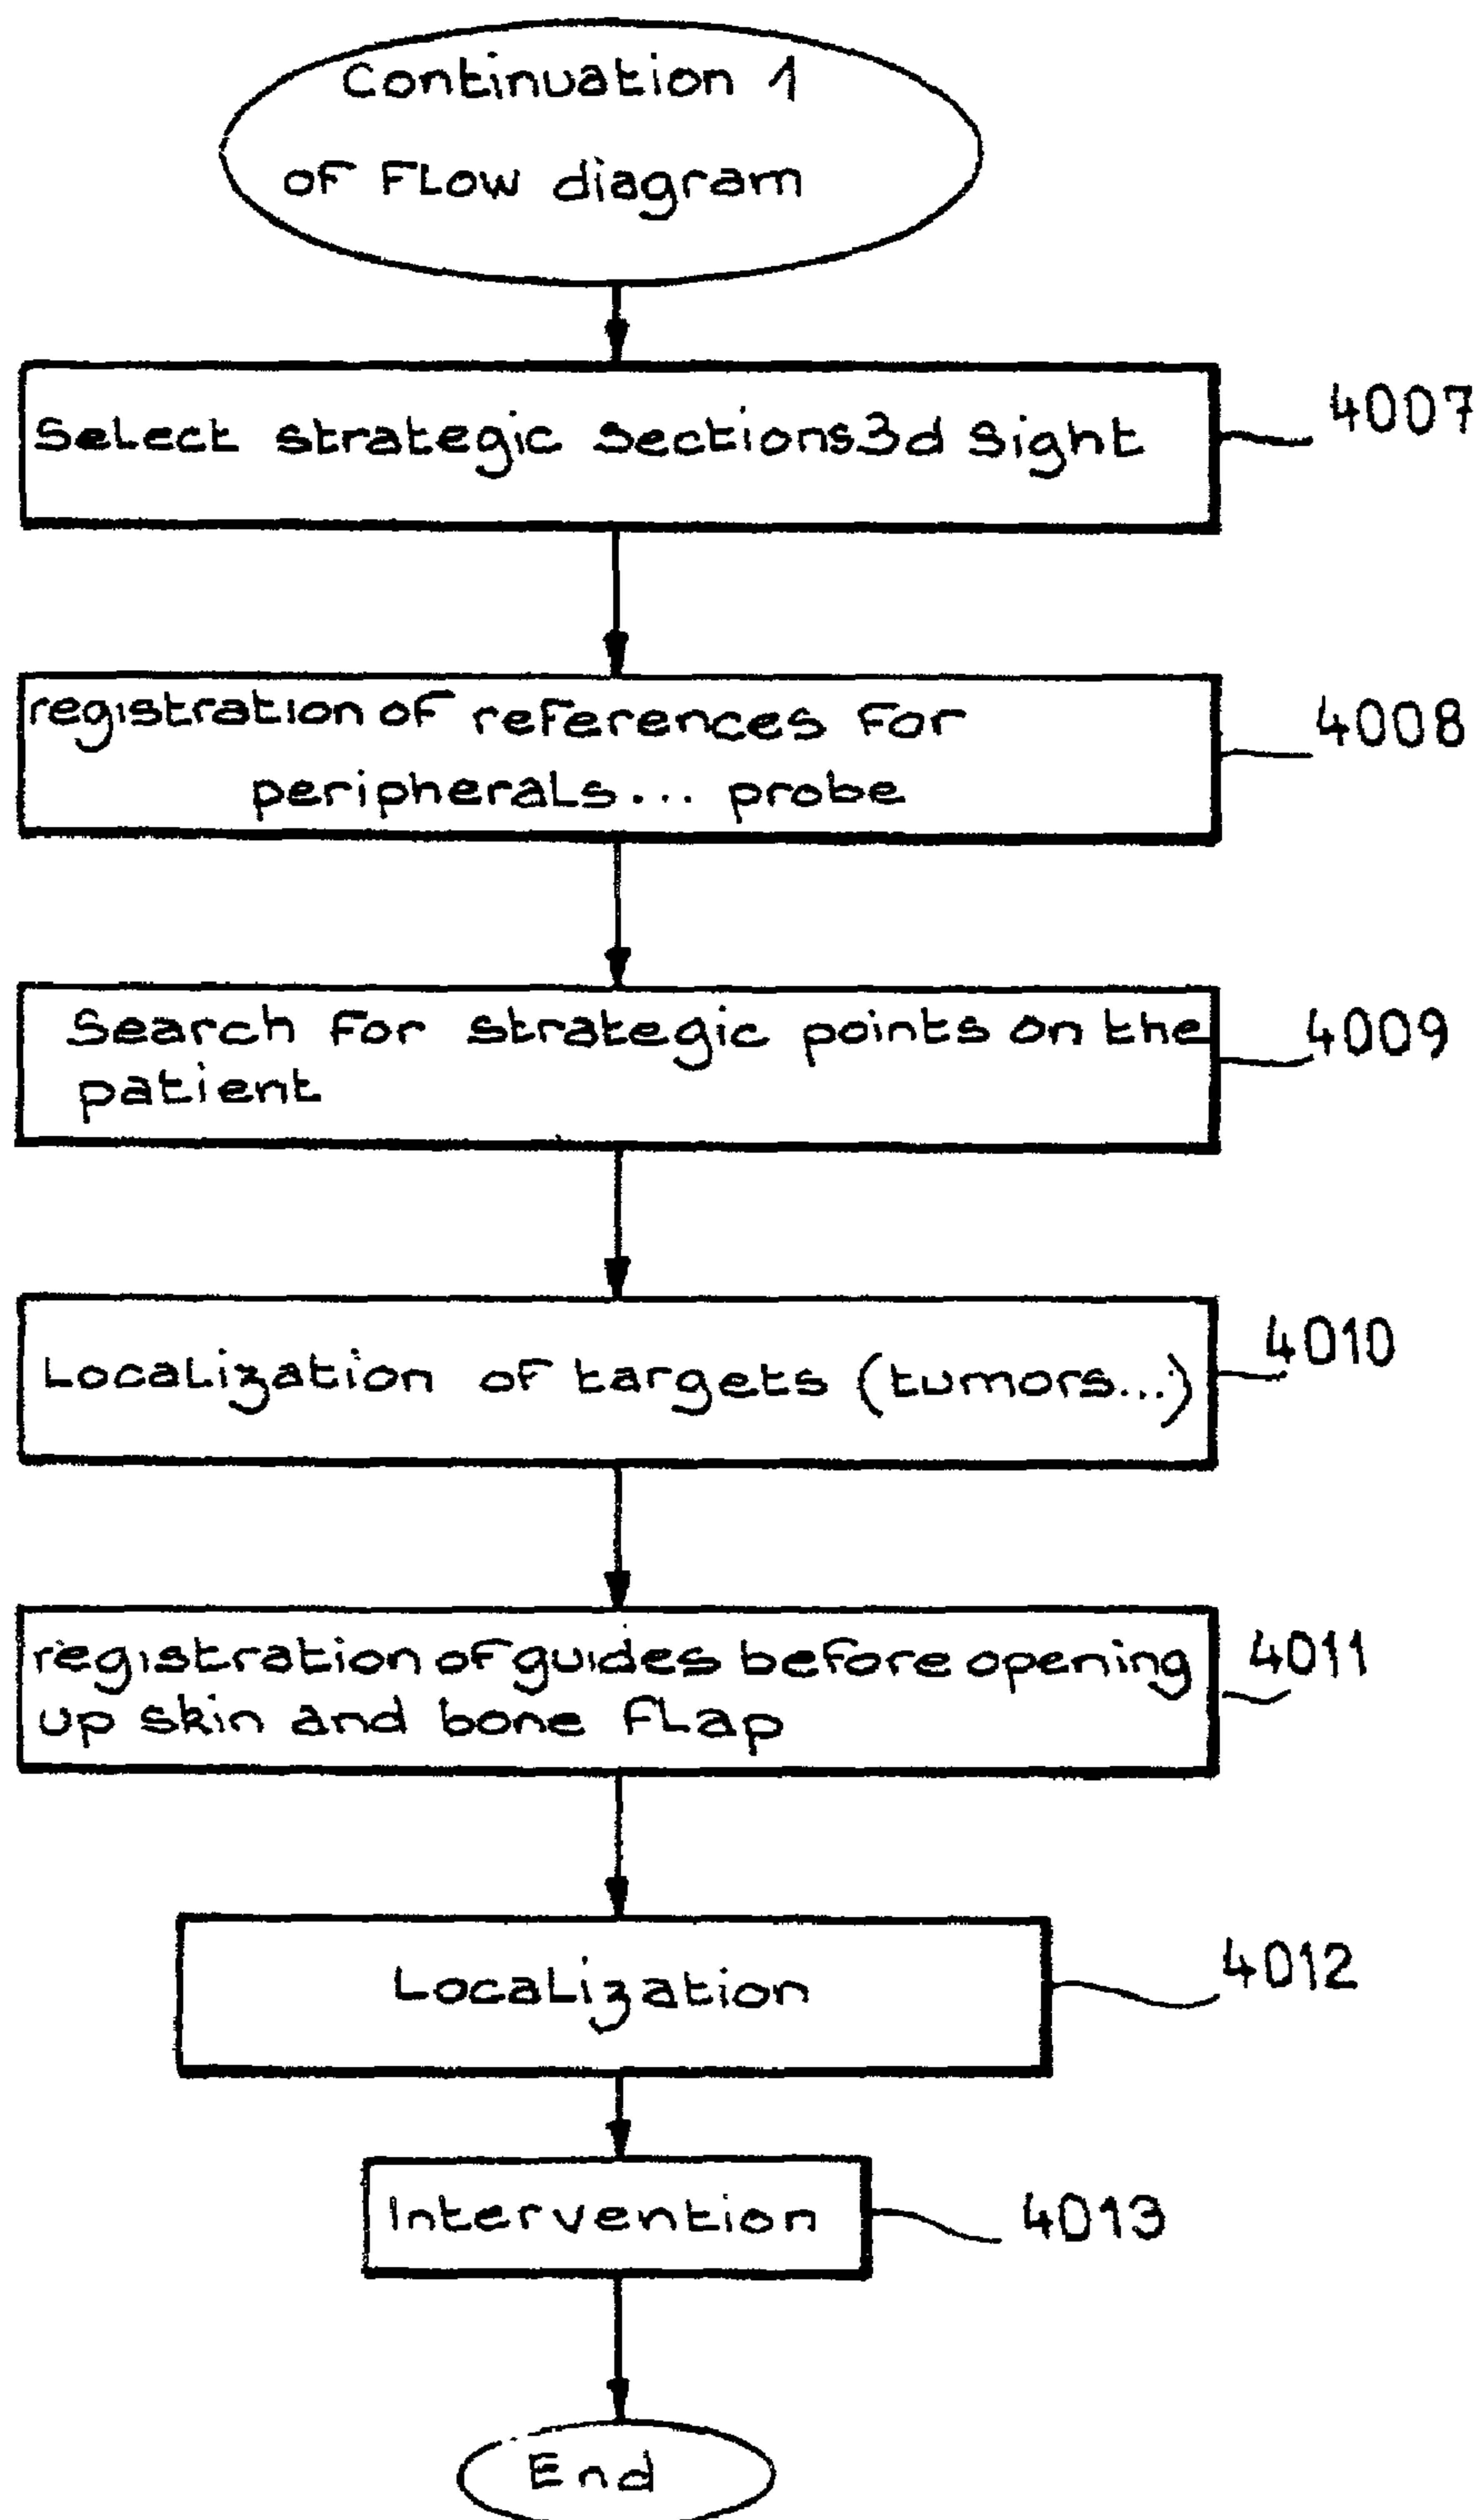
FIG. 10b

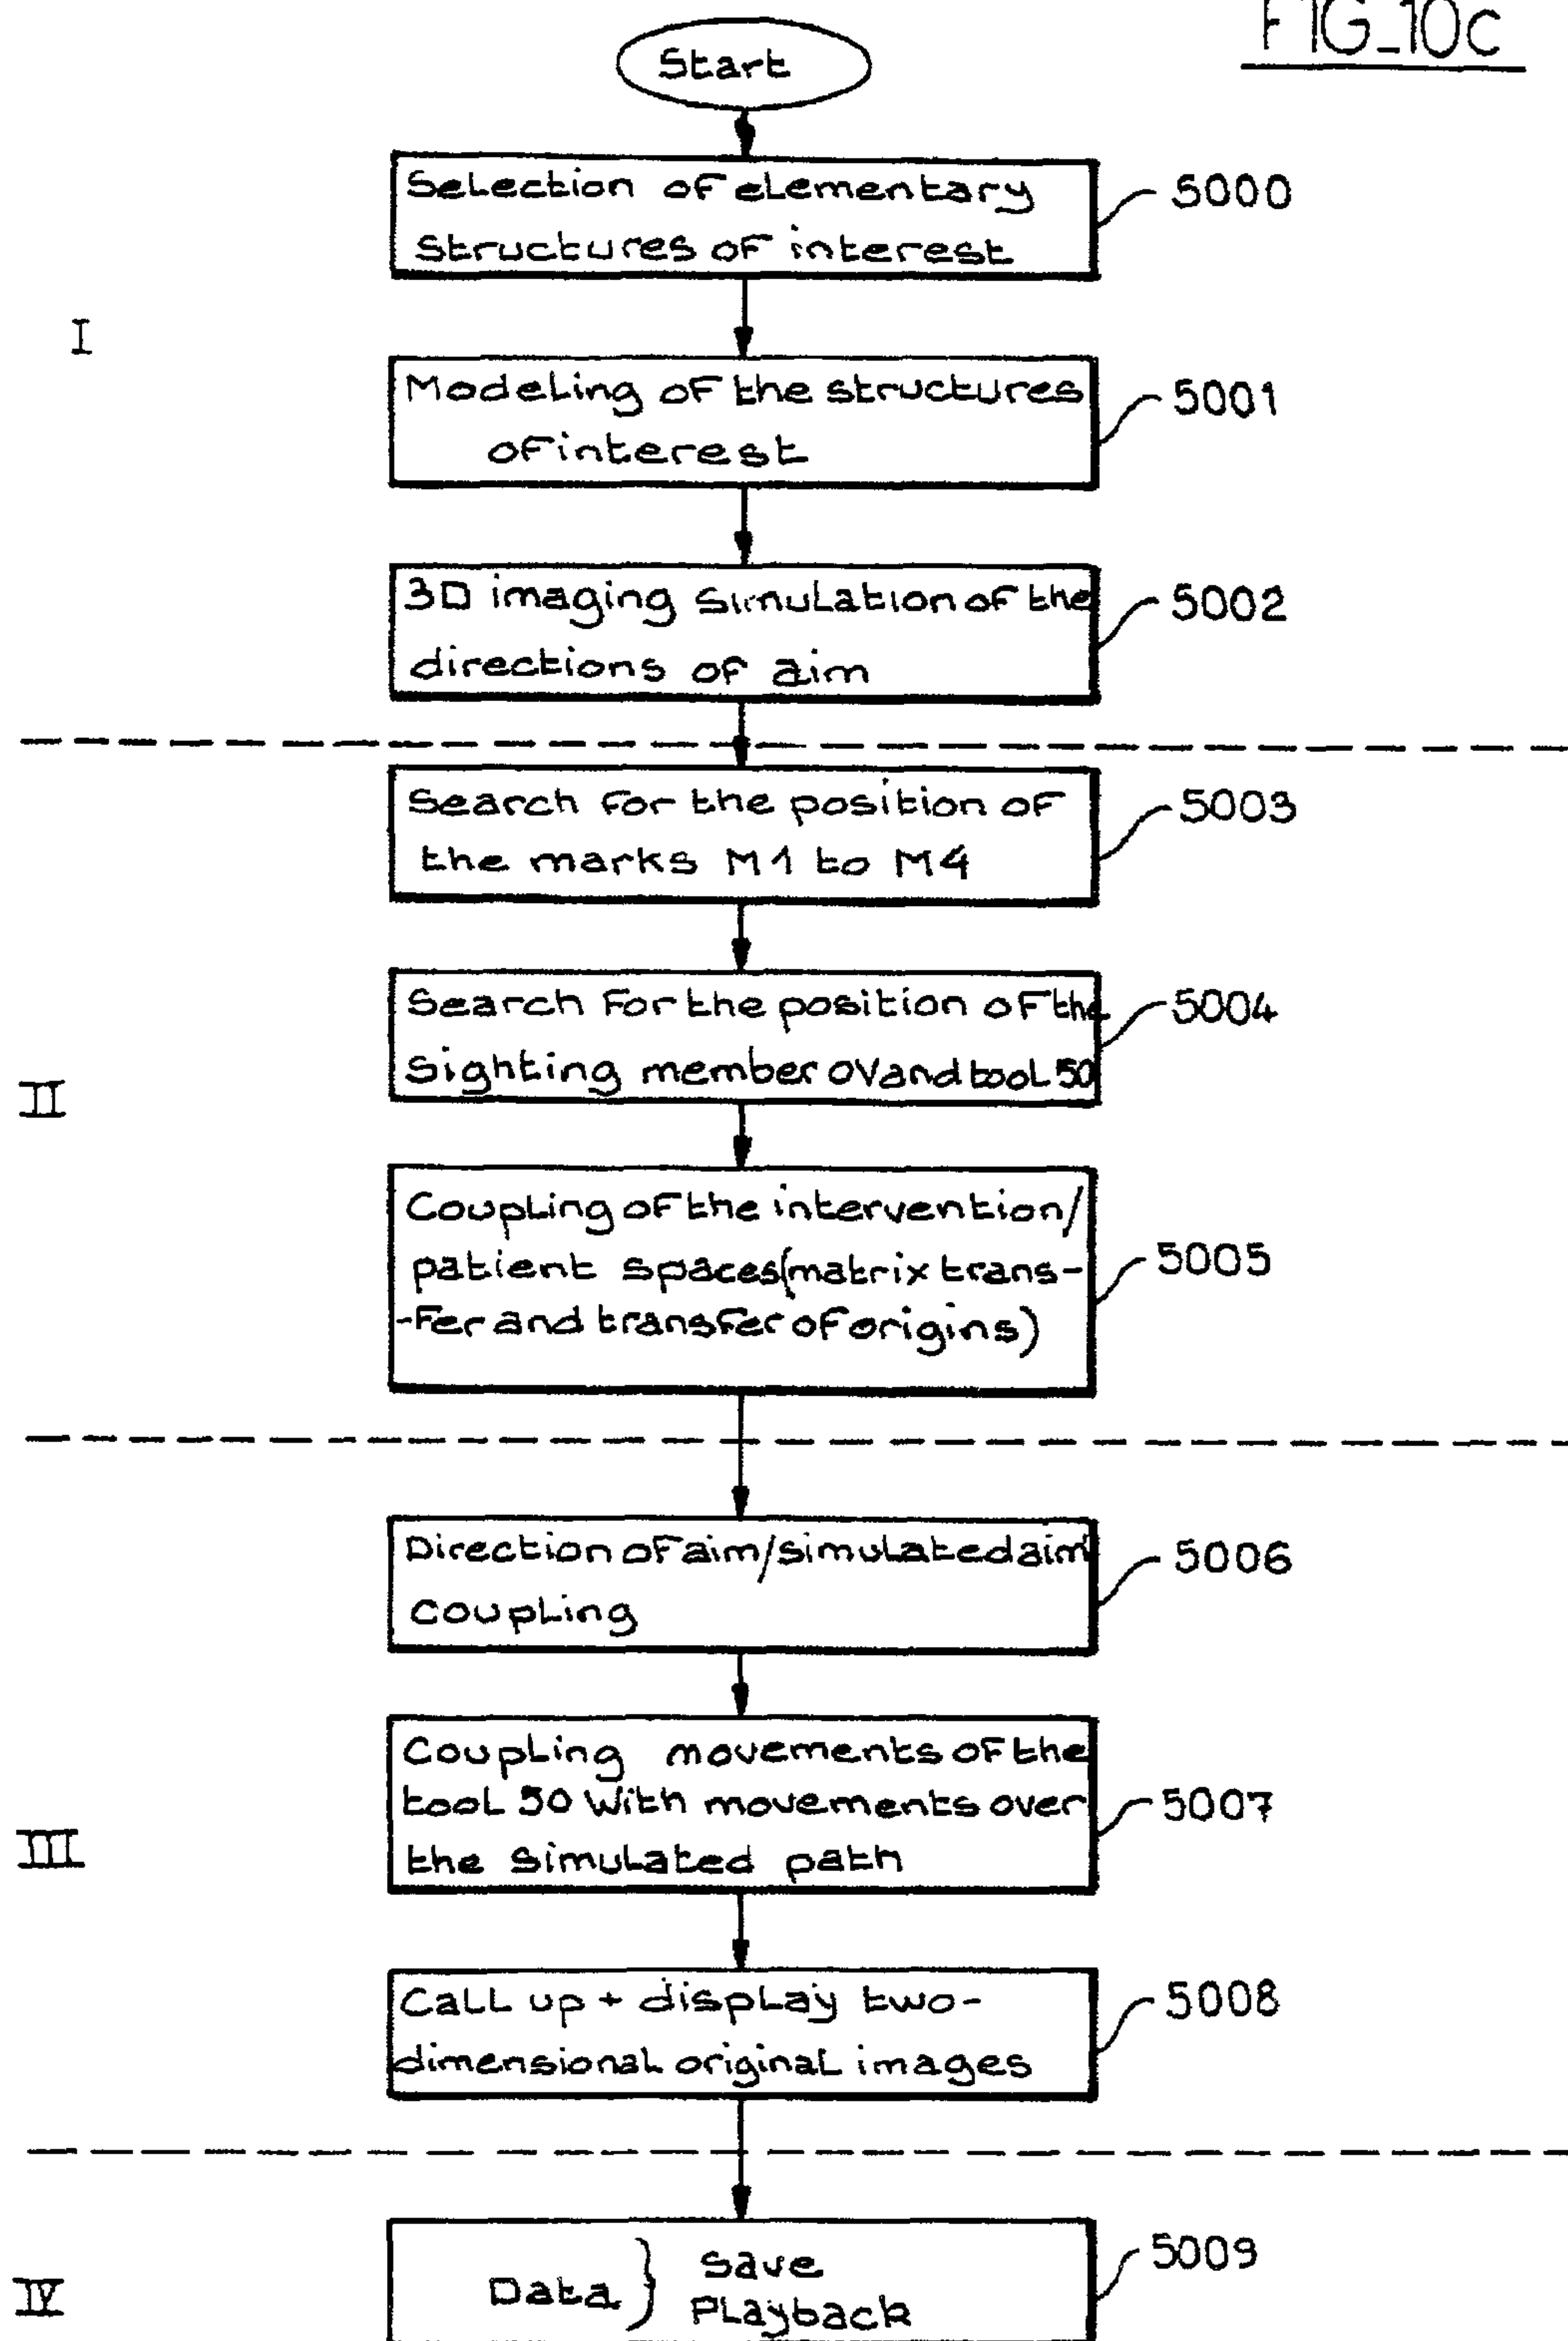FIG. 10c



1

**INTERACTIVE SYSTEM FOR LOCAL
INTERVENTION INSIDE A
NON-HOMOGENEOUS STRUCTURE**

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue.

The invention relates to an interactive system for local intervention inside a region of a nonhomogeneous structure.

The performing of local interventions inside a nonhomogeneous structure, such as intracranial surgical operations or orthopedic surgery currently poses the problem of optimizing the intervention path or paths so as to secure, on the one hand, total intervention over the region or structure of interest, such as a tumor to be treated or explored and, on the other hand, minimal lesion to the regions neighboring or adjoining the region of interest, this entailing the localizing and then the selecting of the regions of the nonhomogeneous structure which are least sensitive to being traversed or the least susceptible to damage as regards the integrity of the structure.

Numerous works aimed at providing a solution to the abovementioned problem have hitherto been the subject of publications. Among the latter may be cited the article entitled "Three Dimensional Digitizer (Neuronavigator): New Equipment for computed Tomography Guided Stereotaxic Surgery", published by Eiju Watanabe, M.D., Takashi Watanabe, M.D., Shinya Manaka, M.D., Yoshiaki Mayanagi, M.D., and Kintomo Takakura, M.D. Department of Neurosurgery, Faculty of Medicine, University of Tokyo, Japan, in the journal Surgery Neurol. 1987: 27 pp. 543-547, by Elsevier Science Publishing Co., Inc. The Patent WO-A-88 09151 teaches a similar item of equipment.

In the abovementioned publications are described in particular a system and an operational mode on the basis of which a three-dimensional position marking system, of the probe type, makes it possible to mark the three-dimensional position coordinates of a nonhomogeneous structure, such as the head of a patient having to undergo a neurosurgical intervention, and then to put into correspondence as a function of the relative position of the nonhomogeneous structure a series of corresponding images consisting of two-dimensional images sectioned along an arbitrary direction, and obtained previously with the aid of a medical imaging method of the "scanner" type.

The system and the operational mode mentioned above offer a sure advantage for the intervening surgeon since the latter has available, during the intervention, apart from a direct view of the intervention, at least one two-dimensional sectional view enabling him to be aware, in the sectional plane, of the state of performance of the intervention.

However, and by virtue of the very design of the system and of the operational mode mentioned above, the latter allow neither a precise representation of the state of performance of the intervention, nor partially or totally automated conduct of the intervention in accordance with a program for advance of the instrument determined prior to the intervention.

Such a system and such an operational mode cannot therefore claim to eradicate all man-made risk, since the intervention is still conducted by the surgeon alone.

The objective of the present invention is to remedy the whole of the problem cited earlier, and in particular to propose a system permitting as exact as possible a correlation, at any instant, between an intervention modeling on the screen

2

and the actual intervention, and furthermore the representation from one or more viewing angles, and if appropriate in one or more sectional planes, of the nonhomogeneous structure, the sectional plane or planes possibly being for example perpendicular to the direction of the path of advance of the instrument or of the intervention tool.

Another objective of the present invention is also the implementation of a system permitting simulation of an optimal trajectory of advance of the tool, so as to constitute an assisted or fully programed intervention.

Finally, an objective of the present invention is to propose a system making it possible, on the basis of the simulated trajectory and of the programed intervention, to steer the movement of the instrument or tool to the said trajectory so as to carry out the programed intervention.

The invention proposes to this effect an interactive system for local intervention inside a region of a nonhomogeneous structure to which is tied a reference structure containing a plurality of base points, characterized in that it comprises:

means of dynamic display by three-dimensional imaging of a representation of the nonhomogeneous structure and of a reference structure tied to the nonhomogeneous structure, including images of the base points,

means of delivering the coordinates of the images of the base points in the first reference frame,

means of securing the position of the non-homogeneous structure and the reference structure with respect to a second reference frame.

marker means for delivering the coordinates of the base points in the second reference frame,

means of intervention comprising an active member whose position is determined with respect to the second reference frame,

means of optimizing the transfer of reference frames from the first reference frame to the second reference frame and vice versa, on the basis of the coordinates of the images of the base points in the first reference frame and of the coordinates of the base points in the second reference frame, in such a way as to reduce to a minimum the deviations between the coordinates of the images of the base points in the first reference frame and the coordinates of the base points, expressed in the said first reference frame with the aid of the said reference frame transfer tools,

means for defining with respect to the first reference frame a simulated origin of intervention and a simulated direction of intervention, and

reference frame transfer means using the said reference frame transfer tools to establish a bidirectional coupling between the simulated origin of intervention and the simulated direction of intervention and the position of the active member.

A more detailed description of the system of the invention will be given below with reference to the drawings in which:

FIG. 1 represents a general view of an interactive system for local intervention inside a region of a nonhomogeneous structure according to the present invention,

FIG. 2 represents, in the case where the nonhomogeneous structure consists of the head of a patient, and with a view to a neurosurgical intervention, a reference structure tied to the nonhomogeneous structure and enabling a correlation to be established between a "patient" reference frame and a reference frame of images of the patient which were made and stored previously,

FIG. 3 represents an advantageous embodiment of the spatial distribution of the reference structure of FIG. 2,

3

FIG. 4 presents an advantageous embodiment of the intervention means set up on an operating table in the case of a neurosurgical intervention,

FIGS. 5a and 5b represent a general flow diagram of functional steps implemented by the system,

FIGS. 6 thru 8 represent flow diagrams of programs permitting implementation of certain functional steps of FIG. 5b,

FIG. 9a represents a flow diagram of a program permitting implementation of a functional step of FIG. 5a,

FIG. 9b represents a flow diagram of a program permitting implementation of another functional step of FIG. 5a,

FIGS. 10a and 10b represent a general flow diagram of the successive steps of an interactive dialogue between the system of the present invention and the intervening surgeon and

FIG. 10c represents a general flow diagram of the successive functional steps carried out by the system of the invention, having (sic) the intervention, prior to the intervention, during the intervention and after the intervention.

The interactive system for local intervention according to the invention will firstly be described in connection with FIG. 1.

A nonhomogeneous structure, denoted SNH, on which an intervention is to be performed, consists for example of the head of a patient in which a neurosurgical intervention is to be performed. It is however understood that the system of the invention can be used to carry out any type of intervention in any type of nonhomogeneous structure inside which structural and/or functional elements or units may be in evidence and whose integrity, during the intervention, is to be respected as far as possible.

The system comprises means, denoted 1, of dynamic display by three-dimensional imaging, with respect to a first reference frame R_1 , of a representation (denoted RSR) of a reference structure SR (described later) tied to the structure SNH, and a representation or modeling of the nonhomogeneous structure, denoted RSNH.

More precisely, the means 1 make it possible to display a plurality of successive three-dimensional images, from different angles, of the representations RSNH and RSR.

The system of the invention also comprises means, denoted 2, of tied positioning, with respect to a second reference frame R_2 , of the structures SNH and SR.

In the present non-limiting example, the head of the patient, bearing the reference structure SR, is fixed on an operating table TO to which are fixed the means 2 of tied positioning.

Of course, the patient whose head has been placed in the means 2 for tied positioning has previously been subjected to the customary preparations, in order to enable him to undergo the intervention.

The means 2 of the tied positioning with respect to R_2 will not be described in detail since they can consist of any means (such as a retaining headset) normally used in the field of surgery or neurosurgery. The reference frame R_2 can arbitrarily be defined as a tri-rectangular reference trihedron tied to the operating table TO, as represented in FIG. 1.

Means 3 of marking, with respect to the second reference frame R_2 , the coordinates, denoted X2, Y2, Z2, of arbitrary points, and in particular of a certain number of base points of the reference structure SR are furthermore provided.

These base points constituting the reference structure SR can consist of certain notable points and/or of marks fixed to the patient, at positions selected by the surgeon and in particular at these notable points.

The system of the invention further comprises computing means 4 receiving means 3 of marking the coordinates X2, X2, Z2.

4

The computing means 4, as will be seen in detail later, are designed to elaborate optimal tools for reference frame transfer using on the one hand the coordinates in R_2 , measured by the probe 3, of a plurality of base points of the structure SR, and on the other hand the coordinates in R_1 , determined by graphical tools of the computer M01 (pointing by mouse, etc.), of the images of the corresponding base points in the representation RSR, so as to secure the best possible correlation between the information modeled in the computer equipment and the corresponding real-world information.

There is furthermore provision for reference frame transfer means 11 designed to use the tools thus elaborated and to secure this correlation in real time.

Moreover, means 40 are provided, as will be seen in detail later, for determining or modeling a reference origin of intervention ORI and a direction of intervention Δ .

With the aid of the means 11, the modeled direction of intervention Δ can, at least prior to the intervention and at the start of the intervention, be materialized through an optical sighting system available to the surgeon, it being possible to steer this sighting system positionally with respect to the second reference frame R_2 .

The sighting system will be described later.

The system of the present invention finally comprises means 5 of intervention comprising an active member, denoted 50, whose position is specified with respect to the second reference frame R_2 . The active member can consist of the various tools used in surgical intervention. For example, in the case of an intercranial neurosurgical intervention, the active member could be a trephining tool, a needle, a laser or radioscope emission head, or an endoscopic viewing system.

According to an advantageous characteristic of the invention, by virtue of the reference frame transfer means 11, the position of the active member can be controlled dynamically on the basis of the prior modeling of the origin of intervention ORI and of the direction of intervention Δ .

The means 1 of dynamic display by three-dimensional imaging of the representations RSNH and RSR comprise a file 10 of two-dimensional image data. The file 10 consists for example of digitized data from tomographic sections, from radiographs, from maps of the patient's head, and contained in an appropriate mass memory.

The successive tomographic sections can be produced prior to the intervention in a conventional manner, after the reference structure SR has been put in place on the nonhomogeneous structure SNH.

According to an advantageous feature, the reference structure SR can consist of a plurality of marks or notable points which can be both sensed by the marker means 3 and detected on the two-dimensional images obtained.

Of course, the abovementioned two-dimensional tomographic sections can likewise be produced by any medical imaging means such as a nuclear magnetic resonance system.

In a characteristic and well-known manner, each two-dimensional image corresponding to a tomographic scanner section corresponds to a structural slice thickness of about 2 to 3 mm, the pixels or image elements in the plane of the tomographic section being obtained with a precision of the order of ± 1 mm. It is therefore understood that the marks or points constituting the reference structure SR appear on the images with a positional uncertainty, and an important feature of the invention will consist in minimizing these uncertainties as will be described later.

The system also comprises first means 110 for calculating and reconstructing three-dimensional images from the data from the file 10.

5

It also comprises a high-resolution screen **12** permitting the displaying of one or more three-dimensional or two-dimensional images constituting so many representations of the reference structure RSR and of the nonhomogeneous structure SNH.

Advantageously, the calculating means **110**, the high-resolution screen and the mass memory containing the file **10** form part of a computer of the workstation type with conventional design and denoted MO1.

Preferably, the first calculating means **110** can consist of a CAD type program installed in the workstation MO1.

By way of non-limiting example, this program can be derived from the software marketed under the tradename "AUTOCAD" by the "AUTODESK" company in the United States of America.

Such software makes it possible, from the various digitized two-dimensional images, to reconstruct three-dimensional images constituting the representations of the structures RSR and RSNH in arbitrary orientations.

Thus, as has furthermore been represented in FIG. 1, the calculating means **4** and **11** can consist of a third computer, denoted MO2 in FIG. 1.

The first and second computers MO1 and MO2 are interconnected by a conventional digital link (bus or network).

As a variant, the computers MO1 and MO2 can be replaced by a single workstation.

The marker means **3** consist of a three-dimensional probe equipped with a tactile tip **30**.

This type of three-dimensional probe, known per se and not described in detail, consists of a plurality of hinged arms, marked in terms of position with respect to a base integral with the operating table TO. It makes it possible to ascertain the coordinates of the tactile tip **30** with respect to the origin O_2 of the reference frame R_2 with a precision better than 1 mm.

The probe is for example equipped with resolvers delivering signals representing the instantaneous position of the abovementioned tactile tip **30**. The resolvers are themselves connected to the circuits for digital/analog conversion and sampling of the values representing these signals, these sampling circuits being interconnected in conventional manner to the second computer MO2 in order to supply it with the coordinates X2, X2, Z2 of the tactile tip **30**.

As a variant or additionally, and as represented diagrammatically, the marker means **3** can comprise a set of video cameras **31** and **32** (or else infrared cameras) enabling pictures to be taken of the structures SNH and SR.

The set of cameras can act as a stereoscopic system permitting the positional plotting of the base points of the reference structure SR, or of other points of the nonhomogeneous structure SNH, with respect to the second reference frame R_2 . The positional plotting can be done for example by appending a laser beam emission system making it possible to illuminate successively the points whose coordinates are sought, appropriate software making it possible to then determine the position of these points one by one with respect to R_2 . This software will not be described since it can consist of position and shape recognition software normally available on the market.

According to another variant, the marker means **3** can comprise a telemetry system.

In this case, the marks of the structure SR can consist of small radiotransmitters implanted for example on the relevant points of the patient's head and designed to be visible on the two-dimensional images, appropriate electromagnetic or optical sensors (not shown) being provided in order to deter-

6

mine the coordinates of the said marks in the reference frame R_2 or in a reference frame tied to the latter.

It is important to note here that the general function of the base points of the reference structure is, on the one hand, to be individually localizable on the reference structure, in order to deduce from this the coordinates in R_2 , and on the other hand, to be visualizable on the two-dimensional images so as to be identified (by their coordinates in R_1) and included in the representation RSR on the screen.

It can therefore involve special marks affixed at arbitrary points of the lateral surface of the structure SNH, or else at notable points of the latter, or else, when the notable points can in themselves be localized with high precision both on the structure SNH and on the 2D sections, notable points totally devoid of marks.

In FIG. 2 a plurality of marks, denoted M1 to Mi, these marks, in the case where the nonhomogeneous structure consists of the head of a patient, being localized for example between the eyebrows of the patient, on the latter's temples, and at the apex of the skull at a notable point such as the frontal median point.

More generally, for a substantially ovoid volume constituting the nonhomogeneous structure, there is advantageously provision for four base points at least on the outer surface of the volume.

Thus, as has been represented in FIG. 3, the four marks M1 to M4 of the reference structure are distributed so as preferably to define a more or less symmetric tetrahedron. The symmetry of the tetrahedron, represented in FIG. 3, is materialized by the vertical symmetry plane PV and the horizontal symmetry plane PH.

According to an advantageous characteristic, as will be seen later, the means of elaborating the reference frame transfer tools are designed to select three points of the tetrahedron which will define the "best plane" for the reference frame transfer.

Also, the presence of four or more points enables the additional point(s) to validate a specified selection.

More precisely, the presence of a minimum of four base points on the reference structure makes it possible to search for the minimum distortion between the points captured on the patient by the marker means consisting for example of the three-dimensional probe and the images of these points on the representation by three-dimensional imaging, the coordinates of which are calculated during processing. The best plane of the tetrahedron described earlier, that is to say the plane for which the uncertainty in the coordinates of the points between the points actually captured by the three-dimensional probe and the points of the representation of the reference structure RSR, is minimal, then becomes the reference plane for the reference frame transfer. Thus, the best correlation will be established between a modeled direction of intervention and a modeled origin of intervention, on the one hand, and the action of the member **50**. Preferably, the origin of intervention will be placed at the center of the region in which the intervention is to be carried out, that is to say a tumor observed or treated for example.

Furthermore, it will be possible to take the noted residual uncertainty into account in order to effect the representation of the model and of the tools on the dynamic display means.

A more detailed description of the means of intervention **5** will now be given in connection with FIG. 4.

Preferably, the means of intervention **5** comprise a carriage **52** which is translationally mobile along the operating table TO, for example on a rack, denoted **54**, whilst being driven by a motor, not shown, itself controlled by the computer MO2 for example, via an appropriate link. This movement system will

not be described in detail since it corresponds to a conventional movement system available on the market. As a variant, the carriage **52** can be mobile over a distinct path separated from the operating table TO, or immobile with respect to the operating table and then constitute a support.

The support carriage **52** comprises in the first place a sighting member OV, constituting the above-mentioned sighting system, which can consist of a binocular telescope.

The sighting member OV enables the surgeon, prior to the actual intervention, or during the latter, to sight the presumed position of the region in which the intervention is to be carried out.

Furthermore, and in a non-limiting manner, with the sighting member OV can be associated a helium-neon laser emission system, denoted EL, making it possible to secure the aiming of a fine positioning or sighting laser beam on the structure SNH and in particular, as will be seen in detail later, to indicate to the surgeon the position of an entry point PE prior to the intervention, to enable the latter to open the skull at the appropriate location, and likewise to indicate to him what the direction of intervention will be. Additionally, the illuminating of the relevant point of the nonhomogeneous structure or at the very least the lateral surface of the latter enables the video cameras **31** and **32** to carry out, if necessary, a positional plotting.

Preferably, a system for measuring position by telemetry **53** is provided to secure the precise measurement of the position of the support carriage **52** of the sighting member OV and of the laser emission system EL. During the operation, and in order to secure the intervention, the carriage **52** can be moved along the rack **54**, the position of the carriage **52** being measured very precisely by means of the system **53**. The telemetry system **53** is interconnected with the microcomputer MO2 by an appropriate link.

The means of intervention **5** can advantageously consist of a guide arm **51** for the active member **50**.

The guide arm **51** can advantageously consist of several hinged segments, each hinge being equipped with motors and resolvers making it possible to secure control of movement of the end of the support arm and the positional plotting of this same end and therefore of the active member **50** according to six degrees of freedom with respect to the carriage **52**. The six degrees of freedom comprise, of course, three translational degrees of freedom with respect to a reference frame tied to the carriage **52** and three rotational degrees of freedom along these same axes.

Thus, the support arm **51** and the member **50** are marked in terms of instantaneous position with respect to the second reference frame R_2 , on the one hand by way of the positional plot of the mobile carriage **52** and, on the other hand, by way of the resolvers associated with each hinge of the support arm **51**.

In the case of an intracranial neurosurgical surgical intervention, the active member **50** can be removed and can consist of a trephining tool, a needle or radioactive or chemical implant, a laser or radioisotope emission head or an endoscopic viewing system. These various members will not be described since they correspond to instruments normally used in neurosurgery.

The materializing of the modeled direction of intervention can be effective by means of the laser emitter EL. This sighting being performed, the guide arm **51** can then be brought manually or in steered manner into superposition with the direction of intervention Δ .

In the case of manual positioning, the resolvers associated with the sighting member OV and the laser emitter EL, if appropriate, make it possible to record the path of the sighting

direction, constituting in particular the actual direction of intervention, on the representation of the nonhomogeneous structure in the dynamic display means **1**.

Furthermore, as will be described later and in preferential manner, the intervening surgeon will be able firstly to define a simulated intervention path and steer thereto the movements of the active member **50** in the nonhomogeneous structure in order effectively to secure all or part of the intervention.

In this case, the progress of the intervention tool **50** is then steered directly to the simulated path (data ORI, Δ) by involving the reference frame transfer means **11** in order to express the path in the reference frame R_2 .

A more detailed description of the implementation of the operational mode of the system of the invention will now be described in connection with FIGS. **5a** and **5b**.

According to FIG. **5a**, the first step consists in obtaining and organizing in memory the two-dimensional image data (step **100**). Firstly, the nonhomogeneous structure SNH is prepared. In the case of a neurosurgical intervention for example, this means that the patient's head can be equipped with marks constituting the base points of the reference structure SR. These marks can be produced by means of points consisting of a dye partially absorbing the X-rays, such as a radiopaque dye.

The abovementioned marks are implanted by the surgeon on the patient's head at notable points of the latter [sic], and images can then be taken of the nonhomogeneous structure SNH by tomography for example, by means of an apparatus of the X-ray scanner type.

This operation will not be described in detail since it corresponds to conventional operations in the field of medical imaging.

The two-dimensional image data obtained are then constituted as digitized data in the file **10**, these data being themselves marked with respect to the reference frame R_1 and making it possible, on demand, to restore the two-dimensional images onto the dynamic display means **1**, these images representing superimposed sections of the nonhomogeneous structure SNH.

From the digitized image data available to the surgeon, the latter then proceeds, as indicated at **101** in FIG. **5a**, to select the structures of interest of the abovementioned images.

The purpose of this step is to facilitate the work of the surgeon by forming three-dimensional images which contain only the contours of the elements of the structure which are essential for geometrical definition and real-time monitoring of the progress of the intervention.

In the case where the nonhomogeneous structure SNH consists of the head of a patient, an analysis of the two-dimensional image data makes it possible, from values of optical density of the corresponding image-points, straightaway to extract the contours of the skull, to check the distance scales, etc.

Preferably, the abovementioned operations are performed on a rectangle of interest for a given two-dimensional image, this making it possible, by moving the rectangle of interest, to cover the whole of the image.

The above analysis is performed by means of suitable software which thus makes it possible to extract and vectorize the contours of the structures which will be modeled in the representations RSNH and RSR.

The structures modeled in the case of a neurosurgical intervention are for example the skull, the cerebral ventricles, the tumor to be observed or treated, the falx cerebri, and the various functional regions.

According to a feature of the interactive system of the invention, the surgeon may have available a digitizing table or

other graphics peripheral making it possible, for each displayed two-dimensional image, to rectify or complete the definition of the contour of a particular region of interest.

It will be noted finally that by superimposing the extracted contours on the displayed two-dimensional image, the surgeon will be able to validate the extractions carried out.

The extracted contours are next processed by sampling points to obtain their coordinates in the reference frame R_1 , it being possible to constitute these coordinates as an ASCII type file. This involves step **102** for generating the three-dimensional data base.

This step is followed by a step **103** of reconstructing the three-dimensional model. This step consists firstly, with the aid of the CAD type software, in carrying out on the basis of the contours of the structures of interest constituted as vectorized two-dimensional images an extrapolation between the various sectional planes.

The abovementioned extrapolation is carried out preferably by means of a "B-spline" type algorithm which seems best suited. This extrapolation transforms a discrete item of information, namely the successive sections obtained by means of the scanner analysis, into a continuous model permitting three-dimensional representation of the volume envelopes of the structures.

It should be noted that the reconstruction of the volumes constituting the structures of interest introduces an approximation related in particular to the spacing and non-zero thickness of the acquisition sections. An important characteristic of the invention, as explained in detail elsewhere, is on the one hand to minimize the resulting uncertainties in the patient-model correlation, and on the other hand to take into account the residual uncertainties.

The CAD type software used possesses standard functions which enable the model to be manipulated in space by displaying it from different viewpoints through just a criterion defined by the surgeon (step **104**).

The software can also reconstruct sectional representation planes of the nonhomogeneous structure which differ from the planes of the images from the file **10**, this making it possible in particular to develop knowledge enhancing the data for the representation by building up a neuro-anatomical map.

The surgeon can next (step **105**) determine a model of intervention strategy taking into account the modeled structures of interest, by evaluating the distance and angle ratios on the two-and three-dimensional representations displayed.

This intervention strategy will consist, in actual fact, on the one hand in localizing the tumor and in associating therewith a "target point", which will subsequently be able to substitute for the origin common to all the objects (real and images) treated by the system, and on the other hand in determining a simulated intervention path respecting to the maximum the integrity of the structures of interest. This step can be carried out "in the office", involving only the workstation.

Once this operation is performed and prior to the intervention, the following phase consists in implementing the steps required to establish as exact as possible a correlation between the structure SNH (real world) and the representation RSNH (computer world). This involves steps **106** to **109** of FIG. **5b**.

Firstly, as represented in FIG. **5b** at step **107**, marking of the base points of the reference structure SR with respect to the second reference frame is carried out with the aid of the marker means **3**, by delivering to the system the coordinates X_2, Y_2, Z_2 of the said base points.

The following step **106** consists in identifying on the representations RSNH and RSR displayed on the screen the

images of the base points which have just been marked. More precisely, with the aid of appropriate graphics peripherals, these representations (images) of the base points are selected one by one, the workstation supplying on each occasion (in this instance to the computer MO2) the coordinates of these points represented in the reference frame R_1 .

Thus the computer MO2 has available a first set of three-dimensional coordinates representing the position of the base points in R_2 , and a second set of three-dimensional coordinates representing the position of the representations of the base points in R_1 .

According to an essential feature of the invention, these data will be used to elaborate at **108, 109**, tools for reference frame transfer (from R_1 to R_2 and vice versa) by calling upon an intermediate reference frame determined from the base points and constituting an intermediate reference frame specific to the reconstructed model.

More precisely, the intermediate reference frame is constructed from three base points selected so that, in this reference frame, the coordinates of the other base points after transfer from R_2 and the coordinates of the representations of these other base points after transfer from R_1 are expressed with the greatest consistency and minimum distortion.

When the step of elaborating the reference frame transfer tools is concluded, these tools can be used by the system to secure optimal coupling between the real world and the computer world (step **110**).

Furthermore, according to a subsidiary feature of the present invention, the system can create on the display means a representation of the nonhomogeneous structure and of the intervention member which takes account of the deviations and distortions remaining after the "best" reference frame transfer tools have been selected (residual uncertainties). More precisely, from these deviations can be deduced by the calculating means a standard error likely to appear in the mutual positioning between the representation of the nonhomogeneous structure and the representation of elements (tools, sighting axes, etc.) referenced on R_2 when using the reference frame transfer tools. This residual uncertainty, which may in practice be given substance through an error matrix, can be used for example to represent certain contours (tool, structures of interest to be avoided during the intervention, etc.) with dimensions larger than those which would normally be represented starting from the three-dimensional data base or with the aid of coordinates marked in R_2 , the said larger dimensions being deduced from the "normal" dimensions by involving the error matrix. For example, if the member were represented normally, in transverse section, by a circle of diameter D_1 , a circle of diameter $D_2 > D_1$ can be represented in substance, with the difference $D_2 - D_1$ deduced from the standard error value. In this way, when a direction of intervention will be selected making it possible to avoid traversing certain structures of interest, the taking into account of an "enlarged" size of the intervention tool will eradicate any risk of the member, because of the abovementioned errors, accidentally traversing these structures.

Back at step **105**, and as will be seen in more detail with reference to FIGS. **9a** and **9b**, the reference origin of intervention ORI and the direction of intervention Δ , that is to say the simulated intervention path, can be determined according to various procedures.

According to a first procedure, the trajectory can be defined from two points, namely an entry point PE (FIG. **3**) and a target point, that is to say substantially the center of the structure of interest consisting of the tumor to be observed or treated. Initially, these two points are localized on the model represented on the screen.

11

According to a second methodology, the trajectory can be determined from the abovementioned target point and from a direction which takes account of the types of structures of interest and of their positions with a view to optimally respecting their integrity.

After the abovementioned step **108**, the surgeon can at step **1110** perform the actual intervention.

The intervention can advantageously be performed by steering the tool or active member over the simulated intervention path, determined in step **1110**.

As a variant, given that the support arm **51** for the active member, equipped with its resolvers, continuously delivers the coordinates in R_2 of the said active member to the system, it is also possible to perform the operation manually or semi-manually, by monitoring on the screen the position and motions of a representation of the tool and by comparing them with the simulated, displayed intervention path.

It will furthermore be noted that the modeled direction of intervention can be materialized with the aid of the laser beam described earlier, the positioning of the latter (with respect to R_2) being likewise carried out by virtue of the reference frame transfer tools.

Certain functional features of the system of the invention will now be described in further detail with reference to FIGS. **6**, **7**, **8**, **9a** and **9b**.

The module for elaborating the reference frame transfer tools (steps **108**, **109** of FIG. **5b**) will firstly be described with reference to FIG. **6**.

This module comprises a first sub-module **1001** for acquiring three points A, B, C, the images of the base points of SR on the representation RSNH (the coordinates of these points being expressed in the computer reference frame R_1), by successive selections of these points on the representation. To this effect, the surgeon is led, by means of a graphics interface such as a "mouse" to point successively at the three selected points A, B, C.

The module for preparing the transfer tools also comprises a second sub-module, denoted **1002**, for creating a unit three-dimensional orthogonal matrix M, this matrix being characteristic of a right-handed orthonormal basis represented by three unit vectors \vec{i} , \vec{j} , \vec{k} , which define an intermediate reference frame tied to R_1 .

The unit vectors \vec{i} , \vec{j} and \vec{k} are given by the relations:

$$\begin{aligned}\vec{j} &= \overrightarrow{AB} / \|\overrightarrow{AB}\| \\ \vec{k} &= (\overrightarrow{BA} \wedge \overrightarrow{BC}) / \|\overrightarrow{BA} \wedge \overrightarrow{BC}\| \\ \vec{i} &= \vec{j} \wedge \vec{k}\end{aligned}$$

where $\|\cdot\|$ designates the norm of the relevant vector.

In the above relations, the sign "A" designates the vector product of the relevant vectors.

Similarly, the module for preparing the transfer tools comprises a third sub-module, denoted **1003**, for acquiring three base points D, E, F, of the structure SR, these three points being those whose images on the model are the points A, B, C respectively. For this purpose, the surgeon, for example by means of the tactile tip **30**, successively senses these three points to obtain their coordinates in R_2 .

The sub-module **1003** is itself followed, as represented in FIG. **6**, by a fourth sub-module **1004** for creating a unit three-dimensional orthogonal matrix N, characteristic of a

12

right-handed orthonormal basis comprising three unit vectors \vec{i}' , \vec{j}' , \vec{k}' and which is tied to the second reference frame R_2 owing to the fact that the nonhomogeneous structure SNH is positionally tied with respect to this reference frame.

The three unit vectors \vec{i}' , \vec{j}' , \vec{k}' are defined by the relations:

$$\begin{aligned}\vec{j}' &= \overrightarrow{DE} / \|\overrightarrow{DE}\| \\ \vec{k}' &= (\overrightarrow{ED} \wedge \overrightarrow{EF}) / \|\overrightarrow{ED} \wedge \overrightarrow{EF}\| \\ \vec{i}' &= \vec{j}' \wedge \vec{k}'\end{aligned}$$

As indicated above, to the extent that the base points of the reference structure can be marked in R_2 with high precision, so their representation in the computer base R_1 is marked with a certain margin of error given on the one hand the non-zero thickness (typically from 2 to 3 mm) of the slices represented by the two-dimensional images from the file **10**, and on the other hand (in general to a lesser extent) the definition of each image element or pixel of a section.

According to the invention, once a pair of transfer matrices M, N has been elaborated with selected points A, B, C, D, E, F, it is sought to validate this selection by using one or more additional base points; more precisely, for the or each additional base point, this point is marked in R_2 with the aid of the probe **30**, the representation of this point is marked in R_1 after selection on the screen, and then the matrices N and M are applied respectively to the coordinates obtained, in order to obtain their expressions in the bases $(\vec{i}', \vec{j}', \vec{k}')$ and $(\vec{i}, \vec{j}, \vec{k})$ respectively. If these expressions are in good agreement, these two bases can be regarded as a single intermediate reference frame, this securing the exact as possible mathematical coupling between the computer reference frame R_1 tied to the model and the "real" reference frame R_2 tied to the patient.

In practice, the module for elaborating the reference frame transfer tools can be designed to perform steps **1001** to **1004** in succession on basic triples which differ on each occasion (for example, if four base points have been defined associated with four representations in RSR, there are four possible triples), in order to perform the validation step **1005** for each of these selections and finally in order to choose the triple for which the best validation is obtained, that is to say for which the deviation between the abovementioned expressions is smallest. This triple defines the "best plane" mentioned elsewhere in the description, and results in the "best" transfer matrices M and N.

As a variant, it will be possible for the selection of the best plane to be made at least in part by the surgeon by virtue of his experience.

It should be noted that the reference frame transfer will only be concluded by supplementing the matrix calculation with the matrices M, N with a transfer of origin, so as to create a new common origin for example at the center of the tumor to be observed or treated (point ORI). This transfer of origin is effected simply by appropriate subtraction of vectors on the one hand on the coordinates in R_1 , and on the other hand on the coordinates in R_2 . These vectors to be subtracted are determined after localization of the center of the tumor on the representation.

Furthermore, the means described above for establishing the coupling between the patient's world and the model's world can also be used to couple to the model's world that of map data, also stored in the workstation and expressed in a different reference frame denoted R_3 . In this case, since these data contain no specific visible mark, the earlier described

elaboration of matrices is performed by substituting for these marks the positions of notable points of the patient's head. These may be temporal points, the frontal median point, the apex of the skull, the center of gravity of the orbits of the eyes, etc.

The corresponding points of the model can be obtained either by selection by mouse or graphics tablet on the model, or by sensing on the patient himself and then using the transfer matrices.

The above step of elaborating the reference frame transfer tools, conducted in practice by the calculating means 4, makes it possible subsequently to implement the reference frame transfer means (FIGS. 7 and 8).

With reference to FIG. 7, the first transfer sub-module 201 comprises a procedure denoted 2010 for acquiring the coordinates XM, YM, ZM, expressed in R_1 , of the point to be transferred, by selecting on the representation.

The procedure 2010 followed by a procedure 2011 for calculating the coordinates XP, YP, ZP (expressed in R_2) of the corresponding real point on the patient through the transformation:

$\{XP, YP, ZP\} = M \cdot N^{-1} \cdot \{XM, YM, ZM\}$ where $M \cdot N^{-1}$ represents the product of the matrix M and the inverse matrix N.

The procedure 2011 is followed by a processing procedure 2012 utilizing the calculated coordinates XP, YP, ZP, for example to indicate the corresponding point on the surface of the structure SNH by means of the laser emission system EL, or again to secure the intervention at the relevant point with coordinates XP, YP, ZP (by steering the active member).

Conversely, in order to secure a transfer from SNH to RSNH, the second sub-module 202 comprises (FIG. 8) a procedure denoted 2020 for acquiring on the structure SNH the coordinates XP, YP, ZP (expressed in R_2) of a point to be transferred.

These coordinates can be obtained by means of the tactile tip 30 for example. The procedure 2020 is followed by a procedure 2021 for calculating the corresponding coordinates XM, YM, ZM in R_1 through the transformation:

$\{XM, YM, ZM\} = N \cdot M^{-1} \cdot \{XP, YP, ZP\}$

A procedure 2022 next makes it possible to effect the displaying of the point with coordinates XM, YM, ZM on the model or again of a straight line or of a plane passing through this point and furthermore meeting other criteria.

It will be noted here that the two sub-modules 201, 202 can be used [sic] by the surgeon at any moment for the purpose of checking the valid nature of the transfer tools; in particular, it is possible to check at any time that a real base point, with coordinates known both in R_2 and R_1 (for example a base point of SR or an arbitrary notable point of the structure SNH visible on the images), correctly relocates with respect to its image after transferring the coordinates in step 2011.

In the event of an excessive difference, a new step of elaboration of the transfer tools is performed.

Furthermore, the sub-modules 201, 202 can be designed to also integrate the taking into account of the residual uncertainty, as spoken of above, so as for example to represent on the screen a point sensed not in a pointwise manner, but in the form for example of a circle or a sphere representing the said uncertainty.

From a simulated intervention path, for example on the representation RSNH, or from any other straight line selected by the surgeon, the invention furthermore enables the model to be represented on the screen from a viewpoint corresponding to this straight line. Thus the third transfer subroutine comprises, as represented in FIGS. 9a and 9b, a first module 301 for visualizing the representation in a direction given by two points and a second module 302 for visualizing the representation in a direction given by an angle of elevation and an angle of azimuth.

The first module 301 for visualizing the representation in a direction given by two points comprises a first sub-module denoted 3010 permitting acquisition of the two relevant points which will define the selected direction. The coordinates of these points are expressed in the reference frame R_1 , these points having either been acquired previously on the nonhomogeneous structure SNH for example by means of the tactile tip 30 and then subjected to the reference frame transfer, or chosen directly on the representation by means of the graphics interface of the "mouse" type.

The first sub-module 3010 is followed by a second sub-module denoted 3011 permitting the creation of a unit, orthogonal three-dimensional matrix V characteristic of a right-handed orthonormal basis \vec{i}'' , \vec{j}'' , \vec{k}'' the unit vectors \vec{i}'' , \vec{j}'' , \vec{k}'' , being determined through the relations:

$$\vec{k}'' = \overline{AB} / \|\overline{AB}\|;$$

$$\vec{i}'' \cdot \vec{k}'' = 0; \vec{i}'' \cdot \vec{j}'' = 0; \|\vec{i}''\| = 1;$$

$$\vec{j}'' = \vec{k}'' \wedge \vec{i}''$$

where " \wedge " represents the vector product and " \cdot " symbolizes the scalar product.

The sub-module 3011 is followed by a routine 3012 making it possible to secure for all the points of the entities (structures of interest) of the three-dimensional data base of coordinates XW, YW, ZW in R_1 a conversion into the

orthonormal basis (\vec{i}'' , \vec{j}'' , \vec{k}'') by the relation:

$$\{XV, YV, ZV\} = V \cdot \{XW, YW, ZW\}$$

The subroutine 3013 is then followed by a subroutine 3014 for displaying the plane i'' , j'' , the subroutines 3013 and 3014 being called up for all the points, as symbolized by the arrow returning to block 3012 in FIG. 9a.

When all the points have been processed, an output module 3015 permits return to a general module, which will be described later in the description. It is understood that this module enables two-dimensional images to be reconstructed in planes perpendicular to the direction defined by A and B.

In the same way, the second module 302 (FIG. 9b) for visualizing the representation from a viewpoint given by an angle of elevation and an angle of azimuth comprises a first sub-module 3020 for acquiring the two angles in the representation frame of reference.

The selection of the angles of elevation and of azimuth can be made by selecting from a predefined data base or by moving software cursors associated with each view or else by modification relative to a current direction, such as the modeled direction of intervention. The sub-module 3020 is itself followed by a second sub-module 3021 for creating a unit orthogonal three-dimensional matrix W characteristic of a right-handed orthonormal basis of unit vectors \vec{i}''' , \vec{j}''' , \vec{k}''' . They are defined by the relations:

$$\vec{i}''' \cdot \vec{k}''' = 0;$$

$$\vec{k}''' \cdot \vec{z}''' = \sin(\text{azimuth})$$

$$\vec{j}''' \cdot \vec{z}''' = 0;$$

$$\vec{i}''' \cdot \vec{y}''' = \cos(\text{elevation});$$

$$\vec{i}''' \cdot \vec{x}''' = \sin(\text{elevation})$$

$$\vec{j}''' = \vec{k}''' \wedge \vec{i}'''$$

15

A routine **3022** is then called for all the points of the entities of the three-dimensional data base of coordinates XW, YW, ZW and enables a first sub-routine **3023** to be called permitting calculation of the coordinates of the relevant point in the right-handed orthonormal bases \vec{i}''' , \vec{j}''' , \vec{k}''' through the transformation:

$$\{XV, YV, ZV\} = V * \{XW, YW, ZW\}$$

The sub-routine **3023** is itself followed by a sub-routine **3024** for displaying the plane i''' , j''' , the two sub-routines **3023** and **3024** then being called up for each point as symbolized by the return via the arrow to the block **3022** for calling the abovementioned routine. When all the points have been processed, an output sub-module **3025** permits a return to the general menu.

Of course, all of the programs, sub-routines, modules, sub-modules and routines destroyed earlier are managed by a general "menu" type program so as to permit interactive driving of the system by screen dialogue with the intervening surgeon by specific screen pages.

A more specific description of a general flow diagram illustrating this general program will now be given in connection with FIGS. **10a** and **10b**.

Thus, in FIG. **10a** has been represented in succession a screen page **4000** relating to the loading of data from the digitized file **10**, followed by a screen page **4001** making it possible to secure the parameterizing of the grey scales of the display on the dynamic display means **1** and to calibrate the image, for example.

The screen page **4001** is followed by a screen page **4002** making it possible to effect the generation of a global view and then a step or screen page **4003** makes it possible to effect an automatic distribution of the sections on the screen of the workstation.

A screen page **4004** makes it possible to effect a manual selection of sections and then a screen page **4005** makes it possible to effect the selection of the strategy (search for the entry points and for the possible directions of intervention, first localizing of the target (tumor . . .) to be treated . . .), as defined earlier, and to select the position and horizontal, sagittal and frontal distribution of the sections.

A screen page **4006** also makes it possible to effect a display of the settings of a possible stereotaxic frame.

It will be recalled that the reference structure SR advantageously replaces the stereotaxic frame formerly used to effect the marking of position inside the patient's skull.

There may furthermore be provided a screen-page **4007** for choosing strategic sections by three-dimensional viewing, on selection by the surgeon, and then at **4008** the aligning of the references of the peripherals (tool, sighting members, etc., with the aid of the probe **30**.

A screen page **4009** is also provided to effect the search for the base points on the patient with the aid of the said probe, following which the steps of construction of the reference frame transfer tools and of actual reference frame transfer are performed, preferably in a user-transparent manner.

Another screen page **4010** is then provided, so as to effect the localizing of the target on the representation (for example a tumor to be observed or treated in the case of a neurosurgical intervention) in order subsequently to determine a simulated intervention path.

Then a new screen page **4011** makes it possible to effect the setting of the guides for the tool on the basis of this simulated path before opening up the skin and bone flaps on the patient's skull.

16

Then a new localizing step **4012** makes it possible to check whether the position of the guides corresponds correctly to the simulated intervention path.

The screen page **4012** is followed by a so-called intervention screen page, the intervention being performed in accordance with step **1110** of FIG. **5b**.

A more detailed description of the interactive dialogue between the surgeon and the system during a surgical, and in particular a neurosurgical, intervention will follow with reference to FIG. **10c** and to all of the preceding description.

The steps of FIG. **10c** are also integrated in the general program mentioned earlier; there are undertaken in succession a first phase I (preparation of the intervention), then a second phase II, (prior to the actual intervention, the patient is placed in a condition for intervention, the reference structure SR being tied to the second reference frame R_2), then a third phase III (intervention) and finally a post-intervention phase IV.

With a view to preparing the intervention, the system requests the surgeon (step **5000**) to choose the elementary structures of interest (for example bones of the skull, ventricles, vascular regions, the tumor to be explored or treated, and the images of the marks constituting in the first reference frame the representation RSR).

The choice of the elementary structures of interest is made on the display of the tomographic images, for example, called up from the digitized file **10**.

The system next performs, at step **5001**, a modeling of the structures of interest, as described earlier. Then, the nonhomogeneous structure having been thus constituted as a three-dimensional model RSNH displayed on the screen, the intervening surgeon is then led to perform a simulation by three-dimensional imaging, at step **5002**, with a view to defining the intervention path of the tool **50**.

During phase II the patient being placed in a condition for intervention and his head and the reference structure SR being tied to the second reference frame R_2 , the surgeon performs at step **5003** a search for the position of the marks M1 to M4 constituting base points of the reference structure in the second reference frame R_2 , and then during a step **5004**, performs a search for the position of the sighting systems, visualizing member OV, or of the tools and intervention instruments **50**, still in the second reference frame R_2 , so as, if appropriate, to align these implements with respect to R_2 .

The system then performs the validation of the intervention/patient spaces and representation by three-dimensional imaging in order to determine next the common origin of intervention ORI. In other words, the matrix reference frame transfer described above is supplemented with the necessary origin translations (origins **01** and **02** aligned on ORI).

This operation is performed as described earlier.

Phase III corresponds to the intervention, during which the system effects at step **5006** a permanent coupling in real time between the direction of aim of the active member **50**, and/or of the direction of aim of the sighting member OV (and if appropriate of the laser beam), with the direction of aim (of observation) simulated by three-dimensional imaging on the display means **1**, and vice versa.

In the following step **5007**, the coupling is effected of the movements and motions of the intervention instrument with their movements simulated by three-dimensional imaging, with automatic or manual conduct of the intervention.

As noted at **5008**, the surgeon can be supplied with a permanent display of the original two-dimensional sectional images in planes specified with respect to the origin ORI and to the direction of intervention. Such a display enables the surgeon at any time to follow the progress of the intervention

in real time and to be assured that the intervention is proceeding in accordance with the simulated intervention. In phase IV which is executed after the intervention, the system effects a saving of the data acquired during the intervention, this saving making it possible subsequently to effect a comparison in real time or deferred in the event of successive interventions on the same patient.

Furthermore, the saved data make it possible to effect a playback of the operations carried out with the option of detailing and supplementing the regions traversed by the active member 50.

Thus, a particularly powerful interactive system for local intervention has been described.

Thus, the system which is the subject of the present invention makes it possible to represent a model containing only the essential structures of the nonhomogeneous structure, this facilitating the work of preparation and of monitoring of the intervention by the surgeon.

Moreover, the system, by virtue of the algorithms used and in particular by minimizing the distortion between the real base points and their images in the 2D sections or the maps, makes it possible to establish a two-way coupling between the real world and the computer world through which the transfer errors are minimized, making possible concrete exploitation of the imaging data in order to steer the intervention tool.

To summarize, the system makes possible an interactive [sic] medical usage not only to create a three-dimensional model of the nonhomogeneous structure but also to permit a marking in real time with respect to the internal structures and to guide the surgeon in the intervention phase.

More generally, the invention makes it possible to end up with a coherent system in respect of:

the two-dimensional imaging data (scanner sections, maps, etc.)

the three-dimensional data base;

the data supplied by the marker means 3 in the reference frame R_2 ;

the coordinate data for the sighting systems and intervention tools;

the real world of the patient on the operating table.

Accordingly, the options offered by the system are, in a non-limiting manner, the following:

the tools and of [sic] their position can be represented on the screen;

the position of a point on the screen can be materialized on the patient for example with the aid of the laser emission device EL;

the orientation and the path of a tool such as a needle can be represented on the screen and materialized on the patient optically (laser emission) or mechanically (positioning of the guide-arm in which the tool is guided in translation);

an image of the patient, yielded for example by a system for taking pictures if appropriate in relief, can be superimposed on the three-dimensional representation modeled on the screen; thus, any change in the soft external parts of the patient can be visualized as compared with the capture by the scanner;

it being possible for the surgeon's field of view given by a sighting member (such as a surgical microscope) to be referenced with respect to R_2 , the direction of visualization of the model on the screen can be made identical to the real sight by the sighting member;

finally, the three-dimensional images, normally displayed on the screen in the preceding description, may as a variant be introduced into the surgeon's microscope so as to obtain the superposition of the real image and the representation of the model.

We claim:

1. An interactive system for local intervention inside a region of a non-homogeneous structure to which is connected a reference structure containing a plurality of base points, the interactive system comprising:

means for dynamically displaying a three-dimensional image of a representation of the non-homogeneous structure and of the reference structure connected to the non-homogeneous structure, wherein the three-dimensional image also includes a plurality of images of the plurality of base points;

means for determining a set of coordinates of the plurality of images of the plurality of base points in a first reference frame;

means for fixing a position of the non-homogeneous structure and of the reference structure with respect to a second reference frame;

means for determining a set of coordinates of the plurality of base points in the second reference frame;

means of intervention comprising an active member whose position is determined with respect to the second reference frame;

means for generating a plurality of reference frame translation tools for translating a plurality of reference frames from the first reference frame to the second reference frame and vice versa, based on the set of coordinates of the plurality of images of the plurality of base points in the first reference frame and of the set of coordinates of the plurality of base points in the second reference frame, in such a way as to reduce to a minimum at least one of a set of deviations between the set of coordinates of the plurality of images of the plurality of base points in the first reference frame and the set of coordinates of the base points, expressed in the first reference frame using the plurality of reference frame translation tools;

means for defining, with respect to the first reference frame, a simulated origin of intervention and a simulated direction of intervention; and,

means for transferring the plurality of reference frames using the plurality of reference frame translation tools to establish a bidirectional coupling between the simulated origin of intervention and the simulated direction of intervention and the position of the active member.

2. The interactive system according to claim 1, wherein the plurality of reference frame translation tools comprise:

means for creating a matrix (M) for transferring between the first reference frame and a first intermediate reference frame based on a set of coordinates of a set of three images of a set of three base points of the reference structure;

means for creating a matrix (N) for transferring between the second reference frame and a second intermediate reference frame based on the set of coordinates of the set of three images of the set of three base points of the reference structure; and,

means for validating matrix (M) and matrix (N) based on the set of three base points and the set of three images, such that at least one deviation between an expression for at least one additional base point in the second intermediate reference frame and an expression for at least one image point of the additional base point in the first intermediate reference frame is reduced to a minimum.

3. The interactive system according to plurality of claim 2, wherein the means for transferring the reference frames using the plurality of reference frame translation tools further comprises:

19

a first transfer sub-module for transferring a set of representation/non-homogeneous structure coordinates, and a second transfer sub-module for transferring a set of non-homogeneous structure/representation coordinates.

4. The interactive system according to claim 3, wherein the first transfer sub-module comprises:

means for acquiring a set of coordinates (XM, YM, ZM), expressed in the first reference frame, of a point of the representation of the non-homogeneous structure to be transferred, by selection on the representation;

means for calculating a set of corresponding coordinates (XP, YP, ZP), expressed in the second reference frame, on the non-homogeneous structure through a transformation:

$\{Y_P, Y_P, Z_P\} = M * N^{-1} * \{X_M, Y_M, Z_M\}$ where $M * N^{-1}$ represents a product of the matrix (M) and an inverse of the matrix (N), and

means for processing, with the aid of the corresponding coordinates (YP, YP, ZP), to display a corresponding point on a surface of the non-homogeneous structure and to secure the intervention.

5. The interactive system according to claim 3, wherein the second transfer sub-module comprises:

means for acquiring a set of coordinates (XP, YP, ZP), expressed in the second reference frame, of a point of the non-homogeneous structure to be transferred;

means for calculating a set of corresponding coordinates (XM, YM, ZM), expressed in the first reference frame, of the representation through a transformation:

$\{Y_M, Y_M, Z_M\} = N * M^{-1} * \{X_P, Z_P, Z_P\}$ where $N * M^{-1}$ represents the product of the matrix (N) and an inverse of the matrix (M); and,

means for displaying the representation using the set of corresponding coordinates (YM, YM, ZM).

6. The interactive system according to claim 1, wherein the means for generating the plurality of reference frame translation tools also generate, in association with the reference frame translation tools, tools for taking into account a residual uncertainty which is based on the set of deviations between the set of coordinates of the plurality of images of the plurality of base points in the first reference frame and the set of coordinates of the base points, the tools for taking into account the residual uncertainty usable for displaying a set of contours in the representation whilst taking into account the residual uncertainties.

7. The interactive system according to claim 1, wherein the means of dynamic displaying the three-dimensional image comprises:

a file containing digitized data from a set of two-dimensional images constituted by successive non-invasive tomographic sections of the non-homogeneous structure;

means for calculating and reconstructing the three-dimensional image from the set of two-dimensional images; and

a high-resolution display screen.

8. The interactive system according to claim 7, wherein the means for calculating and reconstructing the three-dimensional image from the set of two-dimensional images comprises a program consisting of computer-aided design type software.

9. The interactive system according to claim 1, wherein the means for determining the set of coordinates of the plurality of base points in the second reference frame comprises a three-dimensional probe equipped with a tactile tip for delivering a set of coordinates of the tactile tip in the said second reference frame.

20

10. The interactive system according to claim 1, wherein the means for determining the set of coordinates of the plurality of base points is the second reference frame comprises at least one of a set of optical sensors and a set of electromagnetic sensors.

11. The interactive system according to claim 1, wherein a portion of the set of the plurality of base points of the reference structure comprises a plurality of marks positioned on a lateral surface of the non-homogeneous structure.

12. The interactive system according to claim 11, wherein the plurality of marks are four in number and are distributed over the lateral surface so as to define a substantially symmetrical tetrahedron.

13. The interactive system according to claim 1, wherein the means of intervention comprises:

a guide arm to secure intervention in the region of the non-homogeneous structure, the guide arm having a position marked with respect to the second reference frame; and,

an active intervention member whose position is marked with respect to the second reference frame.

14. The interactive system according to claim 13, wherein the active intervention member is removable and selected from the group consisting of:

tools for trephining;

needles and implants;

laser and radioisotope emission heads; and, sighting and viewing systems.

15. The interactive system according to claim 1, wherein the means for transferring the plurality of reference frames establishes a coupling between a direction of visualization of the representation of the non-homogeneous structure on the display means and a direction of observation of the non-homogeneous structure and of the reference structure by the active intervention member.

16. The interactive system according to claim 15, further comprising:

a first module for visualizing a representation in a direction given by two points;

a second module for visualizing a representation in a direction given by an angle of elevation and an angle of azimuth.

17. *An interactive system for intervention inside a region of a patient, said interactive system comprising:*

a device operable to receive image data of the region of the patient, wherein the image data includes image data of a first reference structure to establish an image reference frame for the region of the patient;

a second reference structure positioned relative to the patient to establish a patient reference frame for the region of the patient;

a controller operable to correlate the position of the first reference structure in the image reference frame with the position of the second reference structure in the patient reference frame;

an active member operable to perform the intervention; and

a tracking system operable to determine a position of at least the second reference structure and a position of the active member and configured to transmit the determined positions of the second reference structure and the active member to the controller;

wherein the controller is configured to determine the position of the active member based on the determined position of at least the active member and the correlation of the first reference structure and the second reference structure.

21

18. The interactive system as defined in claim 17 wherein the first reference structure includes a plurality of base points.

19. The interactive system as defined in claim 18 wherein the second reference structure includes a plurality of tracking markers.

20. The interactive system as defined in claim 19 wherein the plurality of base points are generated from the plurality of tracking markers.

21. The interactive system as defined in claim 18 wherein the plurality of base points are at least one of a plurality of notable points on the patient and marks fixed to the patient.

22. The interactive system as defined in claim 21 wherein the notable points are selected from a group comprising a head, eyebrows, temples, frontal medial point, an apex of a skull, a center of gravity of an orbits of the eyes and a combination thereof.

23. The interactive system as defined in claim 18 wherein the controller further includes a graphical tool operable to identify the plurality of base points of the first reference structure in the image data of the image data reference frame.

24. The interactive system as defined in claim 23 wherein the graphical tool is a mouse in communication with the controller.

25. The interactive system as defined in claim 17 wherein the second reference structure includes a plurality of tracking markers.

26. The interactive system as defined in claim 25 wherein the plurality of tracking markers are attached to the patient.

27. The interactive system as defined in claim 17 wherein the second reference structure is attached to the patient.

28. The interactive system as defined in claim 17 wherein the first reference structure is attached to the patient.

29. The interactive system as defined in claim 17 wherein the tracking system includes a marker device operable to determine a position of the second reference structure in relation to the patient reference frame.

30. The interactive system as defined in claim 29 wherein the marker device includes a telemetry system operable to determine the position of the second reference structure in the patient reference frame and transmit the determined position to the controller, wherein the controller is operable to perform the correlation at least with the transmitted determined position.

31. The interactive system as defined in claim 30 wherein the telemetry system is an electromagnetic telemetry system.

32. The interactive system as defined in claim 31 wherein the second reference structure includes electromagnetic tracking markers, wherein the electromagnetic telemetry system is operable to determine the position of the electromagnetic tracking markers of the second reference structure in relation to the patient reference frame.

33. The interactive system as defined in claim 32, wherein the electromagnetic tracking markers are transmitters and the electromagnetic telemetry system is an electromagnetic sensor.

34. The interactive system as defined in claim 30 wherein the telemetry system is an optical telemetry system.

35. The interactive system as defined in claim 34 wherein the optical telemetry system includes at least one of a video camera or an infrared camera to image at least the second reference structure and configured to plot points of the second reference structure.

36. The interactive system as defined in claim 34 wherein the second reference structure includes optical tracking markers, wherein the optical telemetry system is operable to

22

determine the position of the optical tracking markers of the second reference structure in relation to the patient reference frame.

37. The interactive system as defined in claim 34 wherein the optical telemetry system utilizes position and shape recognition to identify the second reference structure.

38. The interactive system as defined in claim 29 wherein the marker device includes a three-dimensional probe.

39. The interactive system as defined in claim 38 wherein the three-dimensional probe includes a tactile tip operable to engage the second reference structure.

40. The interactive system as defined in claim 38 wherein the three-dimensional probe is robotically manipulated, such that the instantaneous position of the three-dimensional probe is known.

41. The interactive system as defined in claim 29 wherein the marker device includes a set of cameras operable to determine the position of the second reference structure in relation to the patient reference frame.

42. The interactive system as defined in claim 41 wherein the set of cameras are selected from video and infrared cameras.

43. The interactive system as defined in claim 29 wherein the marker device is a laser beam emission system operable to illuminate the second reference structure to determine a position of the second reference structure in relation to the patient reference frame.

44. The interactive system as defined in claim 17 wherein the first reference structure is generated from the second reference structure.

45. The interactive system as defined in claim 17 wherein the active member is selected from a group comprising a trephining tool, a needle, a laser, a radioscope emission head, an endoscopic viewing system, a tool used in the intervention, an implant, a sighting system, a microscope, and combinations thereof.

46. The interactive system as defined in claim 17 further comprising a telemetry system operable to determine the position of the active member in the patient reference frame, said telemetry system in communication with the controller.

47. The interactive system as defined in claim 46 wherein the position information of the active member is six degree of freedom information in relation to the patient reference frame.

48. The interactive system as defined in claim 17 wherein the device includes a display operable to display the image data of the region of the patient in relation to the image reference frame.

49. The interactive system as defined in claim 48 wherein the controller is further operable to determine a reference origin of intervention and a direction of intervention and said display is further operable to display the reference origin of intervention and direction of intervention.

50. The interactive system as defined in claim 48 wherein the controller is further operable to model a reference origin of intervention and a direction of intervention and said display is further operable to display the modeled reference origin of intervention and direction of intervention.

51. The interactive system as defined in claim 48 wherein the display is further operable to display the real-time position of the active member in the image reference frame based on the determined position of the active member with the tracking system.

52. The interactive system as defined in claim 48 wherein the display is further operable to display image data relative to a direction of intervention of the active member.

23

53. The interactive system as defined in claim 52 wherein the image data is displayed perpendicular to a direction of intervention of the active member.

54. The interactive system as defined in claim 48 wherein the controller is further operable to simulate an optimal trajectory of advance of the active member and said display is operable to display the optimal trajectory in the image data relative to the image reference frame.

55. The interactive system as defined in claim 54 wherein movement of the active member is steered to the optimal trajectory to carry out a programmed intervention.

56. The interactive system as defined in claim 17 wherein the active member is robotically controlled.

57. The interactive system as defined in claim 17 wherein the image data is at least one of a magnetic resonance image data, a tomographic image data, a radiographic image data, x-ray image data, and combinations thereof.

58. The interactive system as defined in claim 57 wherein the head set is further fixed to an operating table.

59. The interactive system as defined in claim 17 wherein the device is operable to construct three-dimensional images from captured two-dimensional images.

60. The interactive system as defined in claim 17 wherein the controller is further operable to correlate map data in a map reference frame with the patient reference frame.

61. The interactive system as defined in claim 17 wherein the intervention is at least one of a neurosurgery, orthopedic surgery, cranial surgery, and combinations thereof.

62. The interactive system as defined in claim 17 wherein the second reference structure is fixed to a head set.

63. The interactive system as defined in claim 17 wherein the device further includes memory operable to store the image data.

64. The interactive system as defined in claim 17 wherein the device is a first computer.

65. The interactive system as defined in claim 64 wherein the controller is a second computer.

66. The interactive system as defined in claim 65 wherein the first computer and the second computer is a single work station.

67. An interactive system for intervention inside a region of a patient, said interactive system comprising:

a device operable to receive image data of the region of the patient, wherein the image data includes image data of a first reference structure to establish an image reference frame for the region of the patient;

a second reference structure positioned relative to the patient to establish a patient reference frame for the region of the patient; and

a controller operable to correlate the position of the first reference structure in the image reference frame with the position of the second reference structure in the patient reference frame;

wherein the device is operable to construct three-dimensional images from captured two-dimensional images; wherein the controller is operable to superimpose two-dimensional image data on the three-dimensional images wherein any change in soft external parts of the patient can be visualized as compared with the image captured by the imaging device.

68. An interactive system for intervention inside a region of a patient, said interactive system comprising:

a device operable to receive image data of the region of the patient, wherein the image data includes image data of a first reference structure to establish an image reference frame for the region of the patient;

24

a second reference structure positioned relative to the patient to establish a patient reference frame for the region of the patient;

a controller operable to correlate the position of the first reference structure in the image reference frame with the position of the second reference structure in the patient reference frame; and

an active member operable to perform the intervention; wherein the device includes a display operable to display the image data of the region of the patient in relation to the image reference frame;

wherein the controller is further operable to determine residual uncertainty which is used to represent a contour with dimensions larger than those which would normally be represented and the display is operable to display the residual uncertainty of the contour.

69. The interactive system as defined in claim 68 wherein the contour is a display of an active member and a representation of residual uncertainty in order to reduce the chance of traversing undesired structures.

70. An interactive system for intervention inside a region of a patient, said interactive system comprising:

a device operable to receive image data of the region of the patient, wherein the image data includes image data of a first reference structure to establish an image reference frame for the region of the patient;

a second reference structure positioned relative to the patient to establish a patient reference frame for the region of the patient;

a controller operable to correlate the position of the first reference structure in the image reference frame with the position of the second reference structure in the patient reference frame;

an active member operable to perform the intervention inside the region of the patient;

a tracking system operable to track the position of the active member in relation to the patient reference frame, the tracking system being in communication with the controller to transmit the tracked position of the active member as position information to the controller, wherein the controller is operable to determine the position of the active member relative to the image reference frame; and

a display operable to display the real-time position of the active member in the image reference frame based on the controller determined position of the active member based on the tracked position of the active member from the tracking system, wherein the controller is configured to generate a representation of the active member that is displayed on the display relative to a display of the received image data.

71. The interactive system as defined in claim 70 wherein the active member is selected from a group comprising a trephining tool, a needle, a laser, a radioscope emission head, an endoscopic viewing system, a tool used in the intervention, an implant, a sighting system, a microscope, and combinations thereof.

72. The interactive system as defined in claim 70 wherein the position information of the active member is six degree of freedom information in relation to the patient reference frame.

73. The interactive system as defined in claim 70 wherein the tracking system that tracks the position of the active member is a telemetry system in communication with the controller.

74. The interactive system as defined in claim 70 wherein the active member is robotically controlled.

25

75. The interactive system as defined in claim 70 wherein the image data is at least one of a magnetic resonance image data, a tomographic image data, a radiographic image data, x-ray image data, and combinations thereof.

76. The interactive system as defined in claim 70 wherein the controller is further operable to determine a reference origin of intervention and a direction of intervention and said display is further operable to display the reference origin of intervention and direction of intervention.

77. The interactive system as defined in claim 70 wherein the first reference structure includes a plurality of base points.

78. The interactive system as defined in claim 77 wherein the second reference structure includes a plurality of tracking markers.

79. The interactive system as defined in claim 78 wherein the plurality of base points are generated by the plurality of tracking markers.

80. The interactive system as defined in claim 70 wherein the second reference structure is attached to the patient.

81. The interactive system as defined in claim 70 wherein intervention is at least one of a neurosurgery, orthopedic surgery, cranial surgery intervention, and combinations thereof.

82. The interactive system as defined in claim 70 wherein the second reference structure is fixed to a head set.

83. The interactive system as defined in claim 70 wherein the display forms part of the device and wherein the image data received is acquired image data of the region of the patient and is displayed on the display, further wherein the representation of the active member is displayed on the acquired image data of the region of the patient.

84. A method for performing an image guided intervention inside a region of a patient, said method comprising:

accessing a first image data of the region of the patient captured with an imaging system where the first image data includes image data of a first reference structure; identifying the first reference structure in the first image data to establish an image reference frame; identifying a second reference structure relative to the patient to establish a patient reference frame; correlating the position of the first reference structure in the image reference frame in the first image data with the position of the second reference structure in the patient reference frame; and

tracking an active member at least to determine a position of the active member in the patient reference frame to determine a location of the active member based on the tracking of the active member and transmitting the determined position in the patient reference frame for display on a display device relative to the image reference frame of the first image data based at least on the correlation of the first reference structure and the second reference structure.

85. The method as defined in claim 84 further comprising attaching a plurality of tracking markers to the patient where the tracking markers form the second reference structure.

86. The method as defined in claim 85 further comprising identifying the position of the tracking markers in the patient reference frame using a telemetry system.

26

87. The method as defined in claim 86 further comprising transmitting from the tracking markers a signal and receiving the transmitted signal with an electromagnetic sensor to identify the position of the second reference structure in the patient reference frame.

88. The method as defined in claim 84 wherein identifying the first reference structure includes identifying a plurality of base points visible in the image data.

89. The method as defined in claim 88 wherein identifying the plurality of base points includes identifying at least one of notable points on the patient as marks fixed to the patient representing the plurality of base points.

90. The method as defined in claim 89 wherein the notable points are selected from a group comprising a head, eyebrows, temporal point, frontal medial point, an apex of a skull, a center of gravity of an orbits of the eyes and a combination thereof.

91. The method as defined in claim 88 wherein the plurality of base points visible in the image data are generated from the plurality of tracking markers attached to the patient.

92. The method as defined in claim 84 further comprising attaching the second reference structure to the patient.

93. The method as defined in claim 92 further comprising attaching the second reference structure to a head set.

94. The method as defined in claim 84 further comprising displaying the image data of the region of the patient, including displaying the first reference structure.

95. The method as defined in claim 94 further comprising: displaying the position of the active member as a representation of the active member in the accessed first image data that is captured image data that is correlated to the patient based on the correlation and displayed on a display device with the position of the active member being correlated between the patient reference frame defined by the first reference structure fixed to the patient and the image reference frame based on the tracking of the active member.

96. The method as defined in claim 95 further comprising identifying the position of the active member with a telemetry system by transmitting the tracked location of the active member for displaying the representation of the active member.

97. The method as defined in claim 95 further comprising displaying a reference origin of intervention and a direction of intervention in the image data.

98. The method as defined in claim 97 further comprising tracking the position of the active member relative to the reference origin of intervention and the direction of intervention.

99. The method as defined in claim 84 further comprising performing an intervention on the patient with an active member.

100. The method as defined in claim 99 wherein the intervention is selected from at least one of a neurosurgery, orthopedic surgery, cranial surgery, and combinations thereof.

101. The method as defined in claim 84 further comprising converting two-dimensional image data to three-dimensional image data.

* * * * *