



US00RE44305E

(19) **United States**
(12) **Reissued Patent**
Foley et al.

(10) **Patent Number:** **US RE44,305 E**
(45) **Date of Reissued Patent:** ***Jun. 18, 2013**

(54) **PERCUTANEOUS REGISTRATION APPARATUS AND METHOD FOR USE IN COMPUTER-ASSISTED SURGICAL NAVIGATION**

(75) Inventors: **Kevin T. Foley**, Germantown, TN (US); **John B. Clayton**, Superior, CO (US); **Anthony Melkent**, Germantown, TN (US); **Michael C. Sherman**, Memphis, TN (US)

(73) Assignee: **Medtronic Navigation, Inc.**, Louisville, CO (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(21) Appl. No.: **13/036,939**

(22) Filed: **Feb. 28, 2011**

Related U.S. Patent Documents

Reissue of:

(64) Patent No.: **6,226,548**
Issued: **May 1, 2001**
Appl. No.: **09/148,498**
Filed: **Sep. 4, 1998**

U.S. Applications:

(63) Continuation of application No. 11/451,595, filed on Jun. 12, 2006, now Pat. No. Re. 42,226, and a continuation of application No. 11/451,594, filed on Jun. 12, 2006, now Pat. No. Re. 42,194, which is a continuation of application No. 10/423,332, filed on Apr. 24, 2003, now Pat. No. Re. 39,133.

(60) Provisional application No. 60/059,915, filed on Sep. 24, 1997.

(51) **Int. Cl.**
A61B 5/05 (2006.01)

(52) **U.S. Cl.**
USPC **600/426**

(58) **Field of Classification Search**
USPC 600/426, 407, 414, 417, 427, 429; 606/60, 606/61, 65, 104, 130
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,576,781 A 3/1926 Phillips
1,735,726 A 11/1929 Bornhardt

(Continued)

FOREIGN PATENT DOCUMENTS

CA 964149 3/1975
DE 3042343 A1 6/1982

(Continued)

OTHER PUBLICATIONS

“Prestige Cervical Disc System Surgical Technique”, 12 pgs.

(Continued)


Primary Examiner — George Manuel

(74) *Attorney, Agent, or Firm* — Harness, Dickey

(57) **ABSTRACT**

An apparatus and procedures for percutaneous placement of surgical implants and instruments such as, for example, screws, rods, wires and plates into various body parts using image guided surgery. The invention includes an apparatus for use with a surgical navigation system, an attaching device rigidly connected to a body part, such as the spinous process of a vertebrae, with an identification superstructure rigidly but removably connected to the attaching device. This identification superstructure, for example, is a reference arc and fiducial array which accomplishes the function of identifying the location of the superstructure, and, therefore, the body part to which it is fixed, during imaging by CAT scan or MRI, and later during medical procedures.

23 Claims, 19 Drawing Sheets

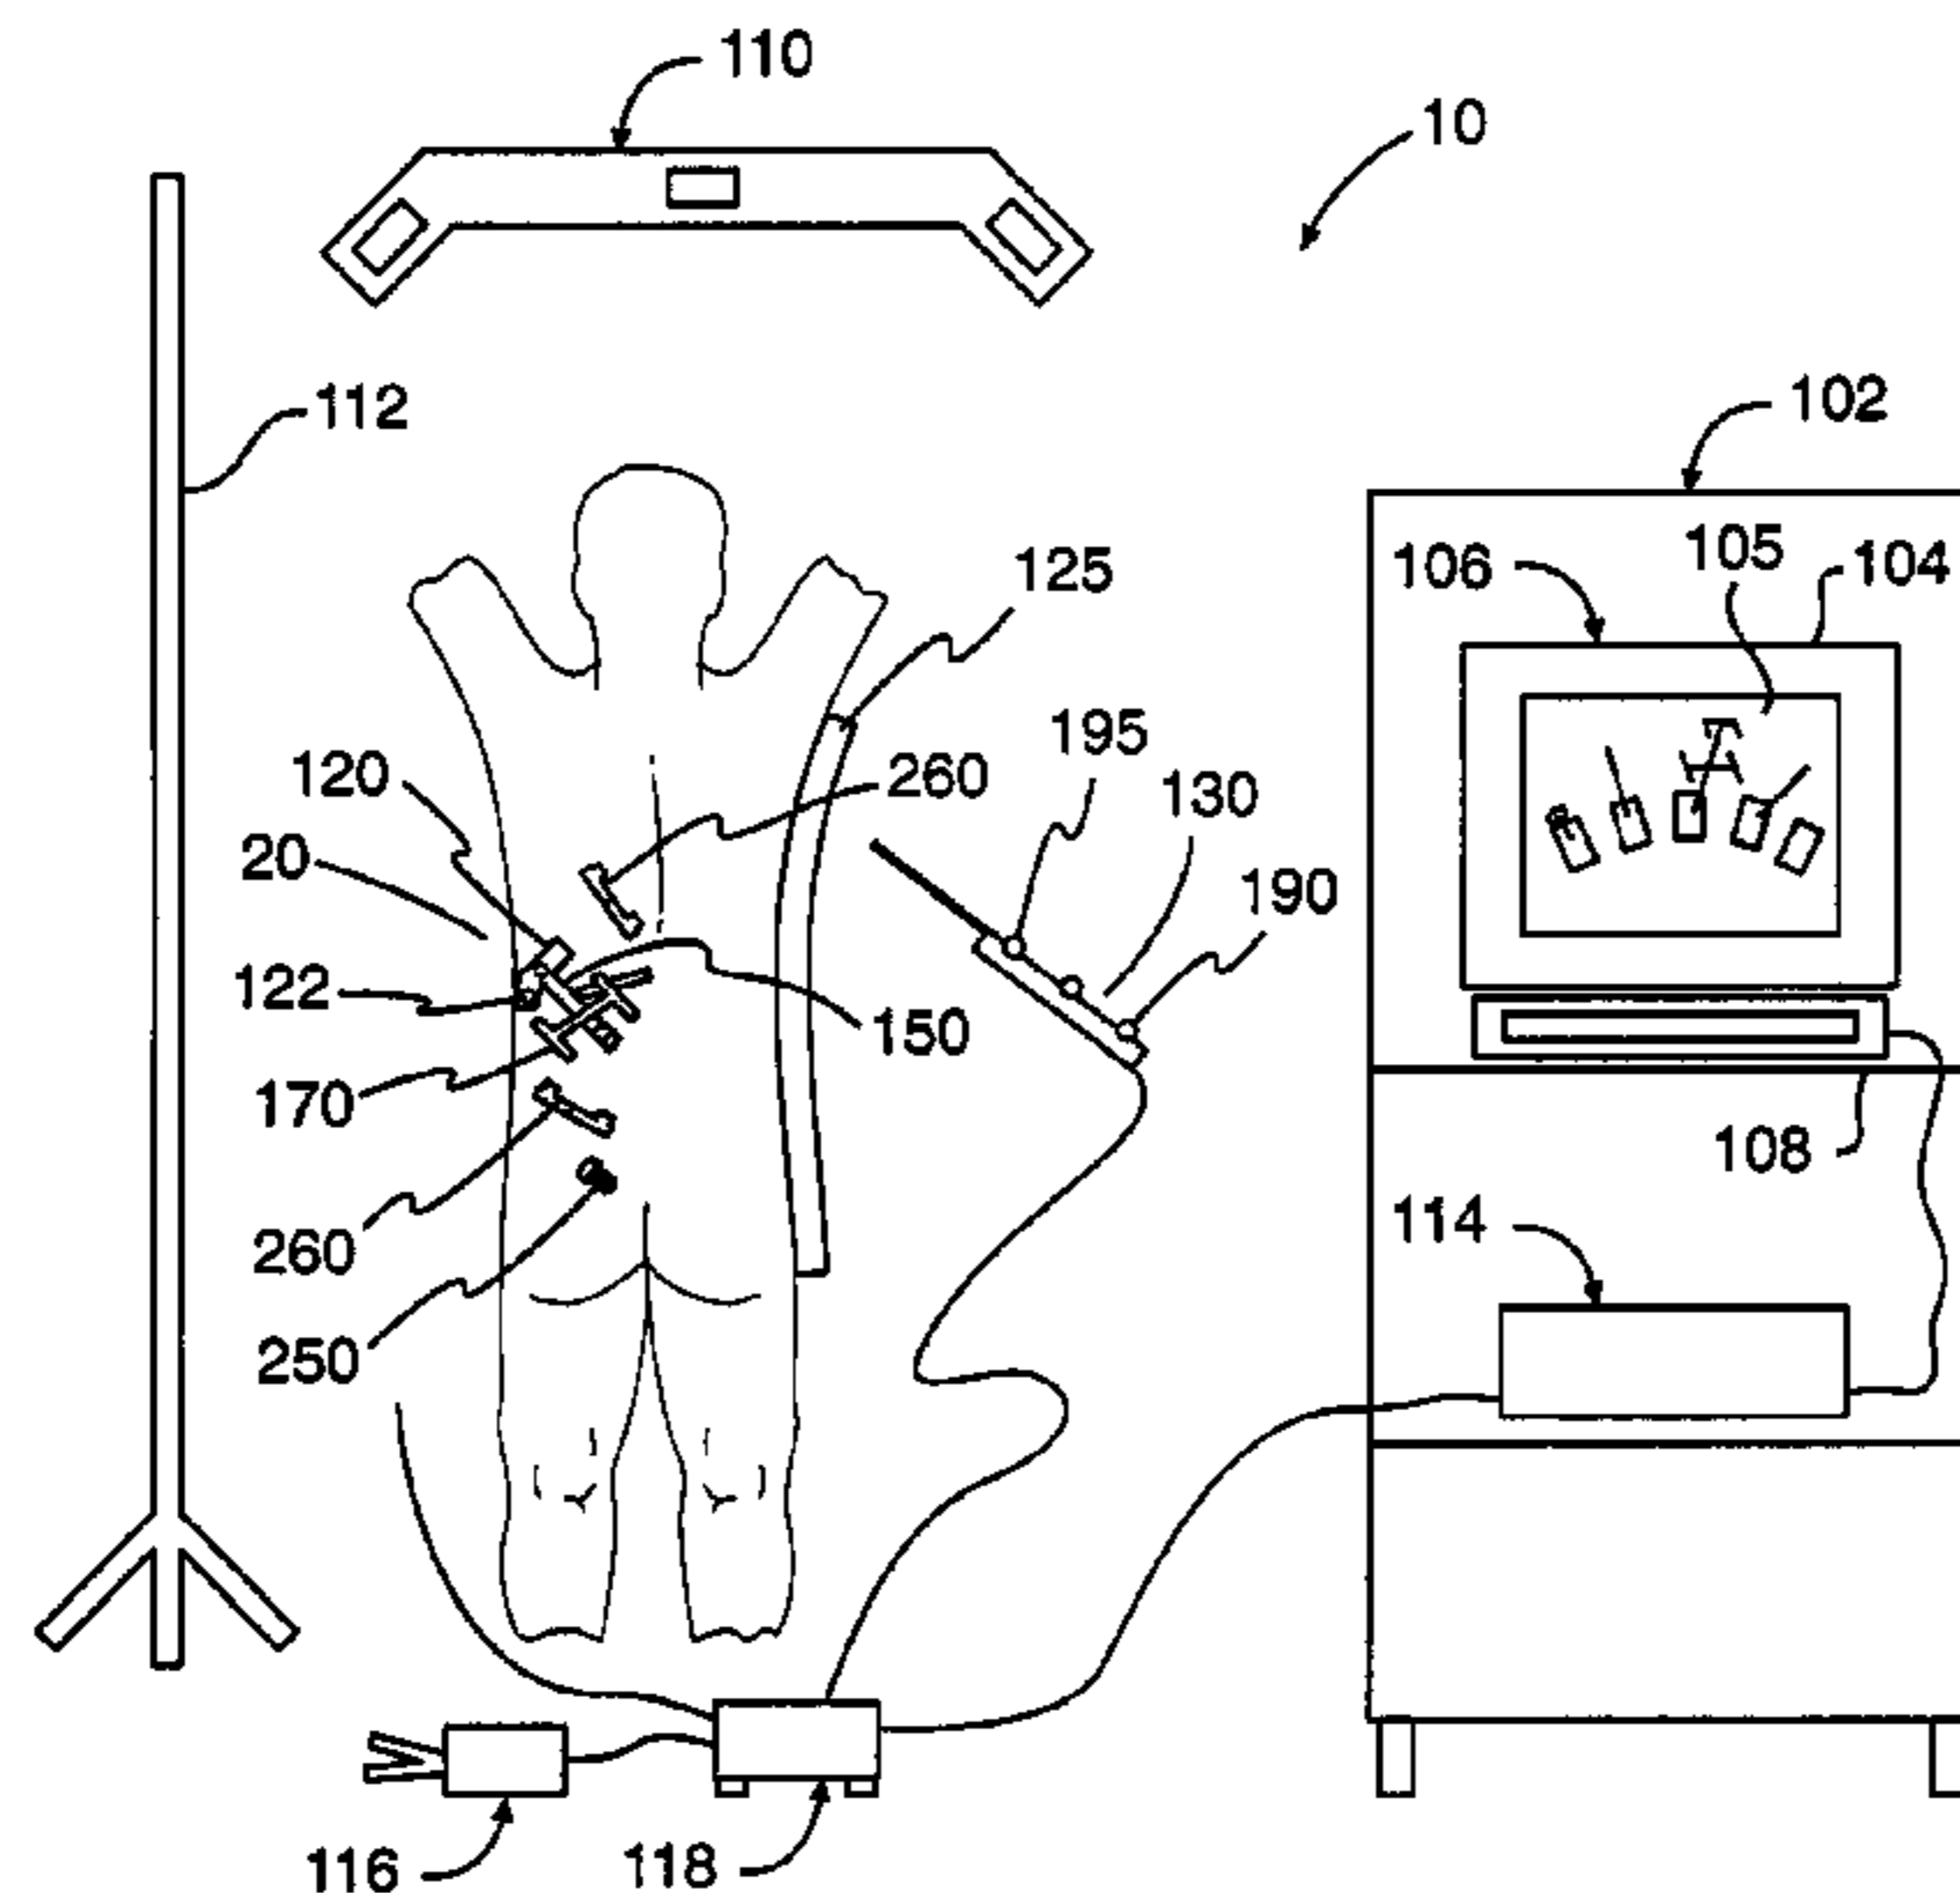

US RE44,305 E

Page 2

U.S. PATENT DOCUMENTS							
2,407,845	A	9/1946	Nemeyer	4,659,971	A	4/1987	Suzuki et al.
2,650,588	A	9/1953	Drew	4,660,970	A	4/1987	Ferrano
2,697,433	A	12/1954	Sehnder	4,673,352	A	6/1987	Hansen
3,016,899	A	1/1962	Stenvall	4,686,997	A	8/1987	Oloff et al.
3,017,887	A	1/1962	Heyer	4,688,037	A	8/1987	Krieg
3,061,936	A	11/1962	Dobbeleer	4,701,049	A	10/1987	Beckman et al.
3,073,310	A	1/1963	Mocarski	4,705,395	A	11/1987	Hageniers
3,109,588	A	11/1963	Polhemus et al.	4,705,401	A	11/1987	Addleman et al.
3,294,083	A	12/1966	Alderson	4,706,665	A	11/1987	Gouda
3,367,326	A	2/1968	Frazier	4,709,156	A	11/1987	Murphy et al.
3,439,256	A	4/1969	Kahne	4,710,708	A	12/1987	Rorden et al.
3,577,160	A	5/1971	White	4,719,419	A	1/1988	Dawley
3,614,950	A	10/1971	Rabey	4,722,056	A	1/1988	Roberts et al. 606/130
3,644,825	A	2/1972	Davis, Jr. et al.	4,722,336	A	2/1988	Kim et al.
3,674,014	A	7/1972	Tillander	4,723,544	A	2/1988	Moore et al.
3,702,935	A	11/1972	Carey et al.	4,727,565	A	2/1988	Ericson
3,704,707	A	12/1972	Halloran	RE32,619	E	3/1988	Damadian
3,821,469	A	6/1974	Whetstone et al.	4,733,661	A	3/1988	Palestrant
3,868,565	A	2/1975	Kuipers	4,733,969	A	3/1988	Case et al.
3,941,127	A	3/1976	Froning	4,737,032	A	4/1988	Addleman et al.
3,983,474	A	9/1976	Kuipers	4,737,794	A	4/1988	Jones
4,017,858	A	4/1977	Kuipers	4,737,921	A	4/1988	Goldwasser et al.
4,037,592	A	7/1977	Kronner	4,742,356	A	5/1988	Kuipers
4,052,620	A	10/1977	Brunnett	4,742,815	A	5/1988	Ninan et al.
4,054,881	A	10/1977	Raab	4,743,770	A	5/1988	Lee
4,058,114	A	11/1977	Soldner	4,743,771	A	5/1988	Sacks et al.
4,117,337	A	9/1978	Staats	4,745,290	A	5/1988	Frankel et al.
4,173,228	A	11/1979	Van Steenwyk et al.	4,750,487	A	6/1988	Zanetti
4,182,312	A	1/1980	Mushabac	4,753,528	A	6/1988	Hines et al.
4,202,349	A	5/1980	Jones	4,760,851	A	8/1988	Fraser et al.
4,209,254	A	6/1980	Reymond et al.	4,761,072	A	8/1988	Pryor
4,228,799	A	10/1980	Anichkov et al.	4,764,016	A	8/1988	Johansson
4,256,112	A	3/1981	Kopf et al.	4,771,787	A	9/1988	Wurster et al.
4,259,725	A	3/1981	Andrews et al.	4,779,212	A	10/1988	Levy
4,262,306	A	4/1981	Renner	4,782,239	A	11/1988	Hirose et al.
4,287,809	A	9/1981	Egli et al.	4,788,481	A	11/1988	Niwa
4,298,874	A	11/1981	Kuipers	4,791,934	A	12/1988	Brunnett
4,314,251	A	2/1982	Raab	4,793,355	A	12/1988	Crum et al.
4,317,078	A	2/1982	Weed et al.	4,794,262	A	12/1988	Sato et al.
4,319,136	A	3/1982	Jinkins	4,797,907	A	1/1989	Anderton
4,328,548	A	5/1982	Crow et al.	4,803,976	A	2/1989	Frigg et al.
4,328,813	A	5/1982	Ray	4,804,261	A	2/1989	Kirschen
4,339,953	A	7/1982	Iwasaki	4,805,615	A	2/1989	Carol
4,341,220	A	7/1982	Perry	4,809,694	A	3/1989	Ferrara
4,346,384	A	8/1982	Raab	4,821,200	A	4/1989	Oberg
4,358,856	A	11/1982	Stivender et al.	4,821,206	A	4/1989	Arora
4,368,536	A	1/1983	Pfeiler	4,821,731	A	4/1989	Martinelli et al.
4,396,885	A	8/1983	Constant	4,822,163	A	4/1989	Schmidt
4,396,945	A	8/1983	DiMatteo et al.	4,825,091	A	4/1989	Breyer et al.
4,398,540	A	8/1983	Takemura et al.	4,829,373	A	5/1989	Leberl et al.
4,403,321	A	9/1983	Kruger	4,836,778	A	6/1989	Baumrind et al.
4,418,422	A	11/1983	Richter et al.	4,838,265	A	6/1989	Cosman et al.
4,419,012	A	12/1983	Stephenson et al.	4,841,967	A	6/1989	Chang et al.
4,422,041	A	12/1983	Lienau	4,845,771	A	7/1989	Wislocki et al.
4,431,005	A	2/1984	McCormick	4,849,692	A	7/1989	Blood
4,457,311	A	7/1984	Sorenson et al.	4,860,331	A	8/1989	Williams et al.
4,485,815	A	12/1984	Amplatz et al.	4,862,893	A	9/1989	Martinelli
4,506,676	A	3/1985	Duska	4,869,247	A	9/1989	Howard, III et al.
4,543,959	A	10/1985	Sepponen	4,875,165	A	10/1989	Fencil et al.
4,548,208	A	10/1985	Niemi	4,875,478	A	10/1989	Chen
4,571,834	A	2/1986	Fraser et al.	4,884,566	A	12/1989	Mountz et al.
4,572,198	A	2/1986	Codrington	4,889,526	A	12/1989	Rauscher et al.
4,583,538	A	4/1986	Onik et al.	4,896,673	A	1/1990	Rose et al.
4,584,577	A	4/1986	Temple	4,905,698	A	3/1990	Strohl, Jr. et al.
4,592,352	A	6/1986	Patil	4,923,459	A	5/1990	Nambu
4,602,622	A	7/1986	Bar et al.	4,931,056	A	6/1990	Ghajar et al.
4,608,977	A	9/1986	Brown	4,943,296	A	7/1990	Funakubo et al.
4,613,866	A	9/1986	Blood	4,945,305	A	7/1990	Blood
4,617,925	A	10/1986	Laitinen	4,945,914	A	8/1990	Allen
4,618,978	A	10/1986	Cosman	4,951,653	A	8/1990	Fry et al.
4,621,628	A	11/1986	Brudermann	4,955,891	A	9/1990	Carol
4,625,718	A	12/1986	Olerud et al.	4,961,422	A	10/1990	Marchosky et al.
4,638,798	A	1/1987	Shelden et al.	4,971,069	A	11/1990	Gracovetsky
4,642,786	A	2/1987	Hansen	4,977,655	A	12/1990	Martinelli
4,645,343	A	2/1987	Stockdale et al.	4,989,608	A	2/1991	Ratner
4,649,504	A	3/1987	Krouglicof et al.	4,991,579	A	2/1991	Allen
4,651,732	A	3/1987	Frederick	5,002,058	A	3/1991	Martinelli
4,653,509	A	3/1987	Oloff et al.	5,005,592	A	4/1991	Cartmell
				5,013,317	A	5/1991	Cole et al.

US RE44,305 E

Page 3

5,016,639 A	5/1991	Allen	5,299,254 A	3/1994	Dancer et al.
5,017,139 A	5/1991	Mushabac	5,299,288 A	3/1994	Glassman et al.
5,027,818 A	7/1991	Bova et al.	5,300,080 A	4/1994	Clayman et al.
5,030,196 A	7/1991	Inoue	5,305,091 A	4/1994	Gelbart et al.
5,030,222 A	7/1991	Calandruccio et al.	5,305,203 A	4/1994	Raab
5,031,203 A	7/1991	Trecha	5,306,271 A	4/1994	Zinreich et al.
5,042,486 A	8/1991	Pfeiler et al.	5,307,072 A	4/1994	Jones, Jr.
5,047,036 A	9/1991	Koutrouvelis	5,309,913 A	5/1994	Kormos et al.
5,050,608 A	9/1991	Watanabe et al.	5,315,630 A	5/1994	Sturm et al.
5,054,492 A	10/1991	Scribner et al.	5,316,024 A	5/1994	Hirschi et al.
5,057,095 A	10/1991	Fabian	5,318,025 A	6/1994	Dumoulin et al.
5,059,789 A	10/1991	Salcudean	5,320,111 A	6/1994	Livingston
5,078,140 A	1/1992	Kwoh	5,325,728 A	7/1994	Zimmerman et al.
5,079,699 A	1/1992	Tuy et al.	5,325,873 A	7/1994	Hirschi et al.
5,080,662 A	1/1992	Paul	5,329,944 A	7/1994	Fabian et al.
5,086,401 A	2/1992	Glassman et al.	5,330,485 A	7/1994	Clayman et al.
5,094,241 A	3/1992	Allen	5,333,168 A	7/1994	Fernandes et al.
5,097,839 A	3/1992	Allen	5,353,795 A	10/1994	Souza et al.
5,098,426 A	3/1992	Sklar et al.	5,353,800 A	10/1994	Pohndorf et al.
5,099,845 A	3/1992	Besz et al.	5,353,807 A	10/1994	DeMarco
5,099,846 A	3/1992	Hardy	5,359,417 A	10/1994	Muller et al.
5,105,829 A	4/1992	Fabian et al.	5,368,030 A	11/1994	Zinreich et al.
5,107,839 A	4/1992	Houdek et al.	5,371,778 A	12/1994	Yanof et al.
5,107,843 A	4/1992	Aarnio et al.	5,375,596 A	12/1994	Twiss et al.
5,107,862 A	4/1992	Fabian et al.	5,377,678 A	1/1995	Dumoulin et al.
5,109,194 A	4/1992	Cantaloube	5,383,454 A	1/1995	Bucholz
5,119,817 A	6/1992	Allen	5,385,146 A	1/1995	Goldreyer
5,142,930 A	9/1992	Allen et al.	5,385,148 A	1/1995	Lesh et al.
5,143,076 A	9/1992	Hardy et al.	5,386,828 A	2/1995	Owens et al.
5,152,288 A	10/1992	Hoening et al.	5,389,101 A	2/1995	Heilbrun et al.
5,160,337 A	11/1992	Cosman	5,391,199 A	2/1995	Ben-Haim
5,161,536 A	11/1992	Vilkomerson et al.	5,394,457 A	2/1995	Leibinger et al.
5,178,164 A	1/1993	Allen	5,394,875 A	3/1995	Lewis et al.
5,178,621 A	1/1993	Cook et al.	5,397,329 A	3/1995	Allen
5,186,174 A	2/1993	Schlondorff et al.	5,398,684 A	3/1995	Hardy
5,187,475 A	2/1993	Wagener et al.	5,399,146 A	3/1995	Nowacki et al.
5,188,126 A	2/1993	Fabian et al.	5,400,384 A	3/1995	Fernandes et al.
5,190,059 A	3/1993	Fabian et al.	5,402,801 A	4/1995	Taylor
5,193,106 A	3/1993	DeSena	5,408,409 A	4/1995	Glassman et al.
5,197,476 A	3/1993	Nowacki et al.	5,413,573 A	5/1995	Koivukangas
5,197,965 A	3/1993	Cherry et al.	5,417,210 A	5/1995	Funda et al.
5,198,768 A	3/1993	Keren	5,419,325 A	5/1995	Dumoulin et al.
5,198,877 A	3/1993	Schulz	5,423,334 A	6/1995	Jordan
5,207,688 A	5/1993	Carol	5,425,367 A	6/1995	Shapiro et al.
5,211,164 A	5/1993	Allen	5,425,382 A	6/1995	Golden et al.
5,211,165 A	5/1993	Dumoulin et al.	5,426,683 A	6/1995	O'Farrell, Jr. et al.
5,211,176 A	5/1993	Ishiguro et al.	5,426,687 A	6/1995	Goodall et al.
5,212,720 A	5/1993	Landi et al.	5,427,097 A	6/1995	Depp
5,214,615 A	5/1993	Bauer	5,429,132 A	7/1995	Guy et al.
5,219,351 A	6/1993	Teubner et al.	5,433,198 A	7/1995	Desai
5,222,499 A	6/1993	Allen et al.	RE35,025 E	8/1995	Anderton
5,224,049 A	6/1993	Mushabac	5,437,277 A	8/1995	Dumoulin et al.
5,228,442 A	7/1993	Imran	5,443,066 A	8/1995	Dumoulin et al.
5,230,338 A	7/1993	Allen et al.	5,443,489 A	8/1995	Ben-Haim
5,230,623 A	7/1993	Guthrie et al.	5,444,756 A	8/1995	Pai et al.
5,233,990 A	8/1993	Barnea	5,445,144 A	8/1995	Wodicka et al.
5,237,996 A	8/1993	Waldman et al.	5,445,150 A	8/1995	Dumoulin et al.
5,249,581 A	10/1993	Horbal et al.	5,445,166 A	8/1995	Taylor
5,251,127 A	10/1993	Raab	5,446,548 A	8/1995	Gerig et al.
5,251,635 A	10/1993	Dumoulin et al.	5,447,154 A	9/1995	Cinquin et al.
5,253,647 A	10/1993	Takahashi et al.	5,448,610 A	9/1995	Yamamoto et al.
5,255,680 A	10/1993	Darrow et al.	5,453,686 A	9/1995	Anderson
5,257,636 A	11/1993	White	5,456,718 A	10/1995	Szymaitis
5,257,998 A	11/1993	Ota et al.	5,457,641 A	10/1995	Zimmer et al.
5,261,404 A	11/1993	Mick et al.	5,458,718 A	10/1995	Venkitachalam
5,265,610 A	11/1993	Darrow et al.	5,464,446 A	11/1995	Dreessen et al.
5,265,611 A	11/1993	Hoening et al.	5,469,847 A	11/1995	Zinreich et al.
5,269,759 A	12/1993	Hernandez et al.	5,478,341 A	12/1995	Cook et al.
5,271,400 A	12/1993	Dumoulin et al.	5,478,343 A	12/1995	Ritter
5,273,025 A	12/1993	Sakiyama et al.	5,480,422 A	1/1996	Ben-Haim
5,274,551 A	12/1993	Corby, Jr.	5,480,439 A	1/1996	Bisek et al.
5,279,309 A	1/1994	Taylor et al.	5,483,961 A	1/1996	Kelly et al.
5,285,787 A	2/1994	Machida	5,484,437 A	1/1996	Michelson
5,291,199 A	3/1994	Overman et al.	5,485,849 A	1/1996	Panescu et al.
5,291,889 A	3/1994	Kenet et al.	5,487,391 A	1/1996	Panescu
5,295,200 A	3/1994	Boyer	5,487,729 A	1/1996	Avellanet et al.
5,295,483 A	3/1994	Nowacki et al.	5,487,757 A	1/1996	Truckai et al.
5,297,549 A	3/1994	Beatty et al.	5,490,196 A	2/1996	Rudich et al.
5,299,253 A	3/1994	Wessels	5,494,034 A	2/1996	Schlondorff et al.

US RE44,305 E

5,503,416 A	4/1996	Aoki et al.	5,744,953 A	4/1998	Hansen
5,513,637 A	5/1996	Twiss et al.	5,748,767 A	5/1998	Raab
5,514,146 A	5/1996	Lam et al.	5,749,362 A	5/1998	Funda et al.
5,515,160 A	5/1996	Schulz et al.	5,749,835 A	5/1998	Glantz
5,517,990 A	5/1996	Kalfas et al.	5,752,513 A	5/1998	Acker et al.
5,520,660 A	5/1996	Loos et al.	5,755,725 A	5/1998	Druais
5,526,576 A	6/1996	Fuchs et al.	RE35,816 E	6/1998	Schulz
5,531,227 A	7/1996	Schneider	5,758,667 A	6/1998	Slettenmark
5,531,520 A	7/1996	Grimson et al.	5,762,064 A	6/1998	Polvani
5,542,938 A	8/1996	Avellanet et al.	5,767,669 A	6/1998	Hansen et al.
5,543,951 A	8/1996	Moehrmann	5,767,960 A	6/1998	Orman
5,546,940 A	8/1996	Panescu et al.	5,769,789 A *	6/1998	Wang et al. 600/414
5,546,949 A	8/1996	Frazin et al.	5,769,843 A	6/1998	Abela et al.
5,546,951 A	8/1996	Ben-Haim	5,769,861 A	6/1998	Vilsmeier
5,551,429 A	9/1996	Fitzpatrick et al.	5,772,594 A	6/1998	Barrick
5,558,091 A	9/1996	Acker et al.	5,772,661 A	6/1998	Michelson
5,566,681 A	10/1996	Manwaring et al.	5,775,322 A	7/1998	Silverstein et al.
5,568,384 A	10/1996	Robb et al.	5,776,064 A	7/1998	Kalfas et al.
5,568,809 A	10/1996	Ben-haim	5,782,765 A	7/1998	Jonkman
5,571,109 A	11/1996	Bertagnoli	5,787,886 A	8/1998	Kelly et al.
5,572,999 A	11/1996	Funda et al.	5,792,055 A	8/1998	McKinnon
5,573,533 A	11/1996	Strul	5,792,147 A	8/1998	Evans et al.
5,575,794 A	11/1996	Walus et al.	5,795,294 A	8/1998	Luber et al.
5,575,798 A	11/1996	Koutrouvelis	5,797,849 A	8/1998	Vesely et al.
5,583,909 A	12/1996	Hanover	5,799,055 A	8/1998	Peshkin et al.
5,588,430 A	12/1996	Bova et al.	5,799,099 A	8/1998	Wang et al.
5,590,215 A	12/1996	Allen	5,800,352 A	9/1998	Ferre et al.
5,592,939 A	1/1997	Martinelli	5,800,535 A	9/1998	Howard, III
5,595,193 A	1/1997	Walus et al.	5,802,719 A	9/1998	O'Farrell, Jr. et al.
5,596,228 A	1/1997	Anderton et al.	5,803,089 A	9/1998	Ferre et al.
5,600,330 A	2/1997	Blood	5,807,252 A	9/1998	Hassfeld et al.
5,603,318 A	2/1997	Heilbrun et al.	5,810,008 A	9/1998	Dekel et al.
5,603,328 A	2/1997	Zucker et al.	5,810,728 A	9/1998	Kuhn
5,611,025 A	3/1997	Lorensen et al.	5,810,735 A	9/1998	Halperin et al.
5,617,462 A	4/1997	Spratt	5,820,553 A	10/1998	Hughes
5,617,857 A	4/1997	Chader et al.	5,823,192 A	10/1998	Kalend et al.
5,619,261 A	4/1997	Anderton	5,823,958 A	10/1998	Truppe
5,622,169 A	4/1997	Golden et al.	5,828,725 A	10/1998	Levinson
5,622,170 A	4/1997	Schulz	5,828,770 A	10/1998	Leis et al.
5,627,873 A	5/1997	Hanover et al.	5,829,444 A	11/1998	Ferre et al.
5,628,315 A	5/1997	Vilsmeier et al.	5,831,260 A	11/1998	Hansen
5,630,431 A	5/1997	Taylor	5,833,608 A	11/1998	Acker
5,636,644 A	6/1997	Hart et al.	5,834,759 A	11/1998	Glossop
5,638,819 A	6/1997	Manwaring et al.	5,836,954 A	11/1998	Heilbrun et al.
5,640,170 A	6/1997	Anderson	5,840,024 A	11/1998	Taniguchi et al.
5,642,395 A	6/1997	Anderton et al.	5,840,025 A	11/1998	Ben-Haim
5,643,268 A	7/1997	Vilsmeier et al.	5,843,076 A	12/1998	Webster, Jr. et al.
5,645,065 A	7/1997	Shapiro et al.	5,848,967 A	12/1998	Cosman
5,646,524 A	7/1997	Gilboa	5,851,183 A	12/1998	Bucholz
5,647,361 A	7/1997	Damadian	5,865,846 A	2/1999	Bryan et al.
5,662,111 A	9/1997	Cosman	5,868,674 A	2/1999	Glowinski et al.
5,664,001 A	9/1997	Tachibana et al.	5,868,675 A	2/1999	Henrion et al.
5,674,296 A	10/1997	Bryan et al.	5,871,445 A	2/1999	Bucholz
5,676,673 A	10/1997	Ferre et al.	5,871,455 A	2/1999	Ueno
5,681,260 A	10/1997	Ueda et al.	5,871,487 A	2/1999	Warner et al.
5,682,886 A	11/1997	Delp et al.	5,873,822 A	2/1999	Ferre et al.
5,682,890 A	11/1997	Kormos et al.	5,882,304 A	3/1999	Ehnholm et al.
5,690,108 A	11/1997	Chakeres	5,884,410 A	3/1999	Prinz
5,694,945 A	12/1997	Ben-Haim	5,889,834 A	3/1999	Vilsmeier et al.
5,695,500 A	12/1997	Taylor et al.	5,891,034 A	4/1999	Bucholz
5,695,501 A	12/1997	Carol et al.	5,891,157 A	4/1999	Day et al.
5,697,377 A	12/1997	Wittkampf	5,904,691 A	5/1999	Barnett et al.
5,702,406 A	12/1997	Vilsmeier et al.	5,907,395 A	5/1999	Schulz et al.
5,711,299 A	1/1998	Manwaring et al.	5,913,820 A	6/1999	Bladen et al.
5,713,946 A	2/1998	Ben-Haim	5,920,395 A	7/1999	Schulz
5,715,822 A	2/1998	Watkins et al.	5,921,992 A	7/1999	Costales et al.
5,715,836 A	2/1998	Kliegis et al.	5,923,727 A	7/1999	Navab
5,718,241 A	2/1998	Ben-Haim et al.	5,928,248 A	7/1999	Acker
5,727,552 A	3/1998	Ryan	5,938,603 A	8/1999	Ponzi
5,727,553 A	3/1998	Saad	5,938,694 A	8/1999	Jaraczewski et al.
5,729,129 A	3/1998	Acker	5,947,980 A	9/1999	Jensen et al.
5,730,129 A	3/1998	Darrow et al.	5,947,981 A	9/1999	Cosman
5,730,130 A	3/1998	Fitzpatrick et al.	5,950,629 A	9/1999	Taylor et al.
5,732,703 A	3/1998	Kalfas et al.	5,951,475 A	9/1999	Gueziec et al.
5,735,278 A	4/1998	Hoult et al.	5,951,571 A	9/1999	Audette
5,738,096 A	4/1998	Ben-Haim	5,954,647 A	9/1999	Bova et al.
5,740,802 A	4/1998	Nafis et al.	5,957,844 A	9/1999	Dekel et al.
5,741,214 A	4/1998	Ouchi et al.	5,964,796 A	10/1999	Imran
5,742,394 A	4/1998	Hansen	5,967,980 A	10/1999	Ferre et al.

US RE44,305 E

5,967,982 A	10/1999	Barnett	6,584,174 B2	6/2003	Schubert et al.
5,968,047 A	10/1999	Reed	6,609,022 B2	8/2003	Vilsmeier et al.
5,971,997 A	10/1999	Guthrie et al.	6,611,700 B1	8/2003	Vilsmeier et al.
5,976,156 A	11/1999	Taylor et al.	6,640,128 B2	10/2003	Vilsmeier et al.
5,980,535 A	11/1999	Barnett et al.	6,694,162 B2	2/2004	Hartlep
5,983,126 A	11/1999	Wittkamp	6,701,179 B1	3/2004	Martinelli et al.
5,987,349 A	11/1999	Schulz	RE39,133 E	6/2006	Clayton et al.
5,987,960 A	11/1999	Messner et al.	RE42,194 E	3/2011	Foley et al.
5,999,837 A	12/1999	Messner et al.	RE42,226 E	3/2011	Foley et al.
5,999,840 A	12/1999	Grimson et al.	2001/0007918 A1	7/2001	Vilsmeier et al.
6,001,130 A	12/1999	Bryan et al.	2002/0095081 A1	7/2002	Vilsmeier et al.
6,006,126 A	12/1999	Cosman	2004/0024309 A1	2/2004	Ferre et al.
6,006,127 A	12/1999	Van Der Brug et al.			

FOREIGN PATENT DOCUMENTS

6,013,087 A	1/2000	Adams et al.	DE	3508730	9/1986
6,014,580 A	1/2000	Blume et al.	DE	3717871	12/1988
6,016,439 A	1/2000	Acker	DE	3831278 A1	3/1989
6,019,725 A	2/2000	Vesely et al.	DE	3838011	7/1989
6,024,695 A	2/2000	Taylor et al.	DE	4213426 A1	10/1992
6,050,724 A	4/2000	Schmitz et al.	DE	4225112	12/1993
6,059,718 A	5/2000	Taniguchi et al.	DE	4233978 C1	4/1994
6,063,022 A	5/2000	Ben-Haim	DE	197 15 202 A1	4/1997
6,071,288 A	6/2000	Carol et al.	DE	19715202	10/1998
6,073,043 A	6/2000	Schneider	DE	19751761	10/1998
6,076,008 A	6/2000	Bucholz	DE	19832296	2/1999
6,096,050 A	8/2000	Audette	DE	19747427	5/1999
6,104,944 A	8/2000	Martinelli	DE	10085137	11/2002
6,118,845 A	9/2000	Simon et al.	EP	0018166 A1	10/1980
6,122,538 A	9/2000	Sliwa, Jr. et al.	EP	0062941	10/1982
6,122,541 A	9/2000	Cosman et al.	EP	0119660	9/1984
6,131,396 A	10/2000	Duerr et al.	EP	0155857	9/1985
6,139,183 A	10/2000	Graumann	EP	0 359 773 B1	5/1988
6,143,003 A *	11/2000	Cosman 606/130	EP	0 326 768 A2	12/1988
6,147,480 A	11/2000	Osadchy et al.	EP	0319844	6/1989
6,149,592 A	11/2000	Yanof et al.	EP	0326768	8/1989
6,156,067 A	12/2000	Bryan et al.	EP	350996 A1	1/1990
6,161,032 A	12/2000	Acker	EP	0359773 A1	3/1990
6,165,181 A	12/2000	Heilbrun et al.	EP	0 427 358 A1	10/1990
6,167,296 A	12/2000	Shahidi	EP	0 501 993 B1	11/1990
6,172,499 B1	1/2001	Ashe	EP	0419729 A1	4/1991
6,174,330 B1	1/2001	Stinson	EP	0 456 103 A2	5/1991
6,175,756 B1	1/2001	Ferre et al.	EP	0427358	5/1991
6,178,345 B1	1/2001	Vilsmeier et al.	EP	0 469 966 A1	7/1991
6,194,639 B1	2/2001	Botella et al.	EP	0456103	11/1991
6,201,387 B1	3/2001	Govari	EP	0469966 A1	2/1992
6,203,497 B1	3/2001	Dekel et al.	EP	0501993 A1	9/1992
6,211,666 B1	4/2001	Acker	EP	0581704	2/1994
6,223,067 B1	4/2001	Vilsmeier et al.	EP	0651968	5/1995
6,226,548 B1	5/2001	Foley et al.	EP	0655138	5/1995
6,233,476 B1	5/2001	Strommer et al.	EP	0894473 A2	2/1999
6,236,875 B1	5/2001	Bucholz et al.	EP	0908146	4/1999
6,246,231 B1	6/2001	Ashe	EP	0930046	7/1999
6,259,942 B1	7/2001	Westermann et al.	FR	2417970	9/1979
6,259,943 B1 *	7/2001	Cosman et al. 600/429	FR	2618211 A1	1/1989
6,273,896 B1	8/2001	Franck et al.	GB	2094590 A	9/1982
6,285,902 B1	9/2001	Kienzle, III et al.	GB	2164856 A	4/1986
6,298,262 B1	10/2001	Franck et al.	JP	62327	1/1983
6,314,310 B1	11/2001	Ben-Haim et al.	JP	2765738	6/1988
6,332,089 B1	12/2001	Acker et al.	JP	63240851	10/1988
6,341,231 B1	1/2002	Ferre et al.	JP	3267054	11/1991
6,348,058 B1	2/2002	Melkent et al.	JP	6194639	7/1994
6,351,659 B1	2/2002	Vilsmeier	WO	WO 88/09151	12/1988
6,381,485 B1	4/2002	Hunter et al.	WO	WO-8809151	12/1988
6,424,856 B1	7/2002	Vilsmeier et al.	WO	WO-8905123	6/1989
6,427,314 B1	8/2002	Acker	WO	WO-9005494 A1	5/1990
6,428,547 B1	8/2002	Vilsmeier et al.	WO	WO-9103982 A1	4/1991
6,434,415 B1	8/2002	Foley et al.	WO	WO-9104711	4/1991
6,437,567 B1	8/2002	Schenck et al.	WO	WO 91/07726	5/1991
6,445,943 B1	9/2002	Ferre et al.	WO	WO-9203090	3/1992
6,470,207 B1	10/2002	Simon et al.	WO	WO 92/06645	4/1992
6,474,341 B1	11/2002	Hunter et al.	WO	WO-9404938 A1	3/1994
6,478,802 B2	11/2002	Kienzle, III et al.	WO	WO 94/23647	10/1994
6,484,049 B1	11/2002	Seeley et al.	WO	WO 94/24933	11/1994
6,490,475 B1	12/2002	Seeley et al.	WO	WO-94024933	11/1994
6,493,573 B1	12/2002	Martinelli et al.	WO	WO-9507055 A1	3/1995
6,498,944 B1	12/2002	Ben-Haim et al.	WO	WO 96/11624	4/1996
6,499,488 B1	12/2002	Hunter et al.	WO	WO-9611624 A2	4/1996
6,516,046 B1	2/2003	Frohlich et al.	WO	WO 96/32059	10/1996
6,527,443 B1	3/2003	Vilsmeier et al.	WO	WO-9632059 A1	10/1996
6,551,325 B2	4/2003	Neubauer et al.	WO		

WO	WO-9736192	A1	10/1997
WO	WO 97/40764		11/1997
WO	WO-9740764	A2	11/1997
WO	WO-9749453	A1	12/1997
WO	WO-9808554	A1	3/1998
WO	WO-9838908		9/1998
WO	WO-9915097	A2	4/1999
WO	WO-9921498	A1	5/1999
WO	WO-9923956	A1	5/1999
WO	WO-9926549	A1	6/1999
WO	WO-9927839	A2	6/1999
WO	WO-9929253	A1	6/1999
WO	WO-9933406	A1	7/1999
WO	WO-9937208	A1	7/1999
WO	WO-9938449	A1	8/1999
WO	WO-9952094	A1	10/1999
WO	WO-9960939	A1	12/1999
WO	WO-0130437	A1	5/2001

OTHER PUBLICATIONS

Adams et al., "Orientation Aid for Head and Neck Surgeons," *Innov. Tech. Biol. Med.*, vol. 13, No. 4, 1992, pp. 409-424.

Barrick et al., "Prophylactic Intramedullary Fixation of the Tibia for Stress Fracture in a Professional Athlete," *Journal of Orthopaedic Trauma*, vol. 6, No. 2, pp. 241-244 (May 27, 1992).

Barrick et al., "Technical Difficulties with the Brooker-Wills Nail in Acute Fractures of the Femur," *Journal of Orthopaedic Trauma*, vol. 4, No. 2, pp. 144-150 (1990).

Barrick, "Distal Locking Screw Insertion Using a Cannulated Drill Bit: Technical Note," *Journal of Orthopaedic Trauma*, vol. 7, No. 3, 1993, pp. 248-251.

Batnitzky et al., "Three-Dimensional Computer Reconstructions of Brain Lesions from Surface Contours Provided by Computed Tomography: A Prospectus," *Neurosurgery*, vol. 11, No. 1, Part 1 (Jul. 1982) pp. 73-84.

Benzel et al., "Magnetic Source Imaging: a Review of the Magnes System of Biomagnetic Technologies Incorporated," *Neurosurgery*, vol. 33, No. 2 (Aug. 1993), pp. 252-259.

Bergstrom et al. Stereotaxic Computed Tomography, *Am. J. Roentgenol.*, vol. 127 pp. 167-170 (Jul. 1976).

Bouazza-Marouf et al.; "Robotic-Assisted Internal Fixation of Femoral Fractures", *IMECHE.*, pp. 51-58 (1995).

Brack et al., "Accurate X-ray Based Navigation in Computer-Assisted Orthopedic Surgery," *CAR '98*, pp. 716-722.

Brown, R., M.D., A Stereotactic Head Frame for Use with CT Body Scanners, *Investigative Radiology* © J.B. Lippincott Company, pp. 300-304 (Jul.-Aug. 1979).

Bryan, "Bryan Cervical Disc System Single Level Surgical Technique", *Spinal Dynamics*, 2002, pp. 1-33.

Bucholz et al., "Variables affecting the accuracy of stereotactic localization using computerized tomography," *Journal of Neurosurgery*, vol. 79, Nov. 1993, pp. 667-673.

Bucholz, R.D., et al. Image-guided surgical techniques for infections and trauma of the central nervous system, *Neurosurg. Clinics of N.A.*, vol. 7, No. 2, pp. 187-200 (Apr. 1996).

Bucholz, R.D., et al., A Comparison of Sonic Digitizers Versus Light Emitting Diode-Based Localization, *Interactive Image-Guided Neurosurgery*, Chapter 16, pp. 179-200 (1993).

Bucholz, R.D., et al., Intraoperative localization using a three dimensional optical digitizer, *SPIE—The Intl. Soc. for Opt. Eng.*, vol. 1894, pp. 312-322 (Jan. 17-19, 1993).

Bucholz, R.D., et al., Intraoperative Ultrasonic Brain Shift Monitor and Analysis, *Stealth Station Marketing Brochure* (2 pages) (date unknown).

Bucholz, R.D., et al., The Correction of Stereotactic Inaccuracy Caused by Brain Shift Using an Intraoperative Ultrasound Device, *First Joint Conference, Computer Vision, Virtual Reality and Robotics in Medicine and Medical Robotics and Computer-Assisted Surgery*, Grenoble, France, pp. 459-466 (Mar. 19-22, 1997).

Champleboux et al., "Accurate Calibration of Cameras and Range Imaging Sensors: the NPBS Method," *IEEE International Conference on Robotics and Automation*, Nice, France, May 1992.

Champleboux, "Utilisation de Fonctions Splines pour la Mise au Point D'un Capteur Tridimensionnel sans Contact," *Quelques Applications Medicales*, Jul. 1991.

Cinquin et al., "Computer Assisted Medical Interventions," *IEEE Engineering in Medicine and Biology*, May/June. 1995, pp. 254-263.

Cinquin et al., "Computer Assisted Medical Interventions," *International Advanced Robotics Programme*, Sep. 1989, pp. 63-65.

Clarysse et al., "A Computer-Assisted System for 3-D Frameless Localization in Stereotaxic MRI," *IEEE Transactions on Medical Imaging*, vol. 10, No. 4, Dec. 1991, pp. 523-529.

Cutting M.D. et al., *Optical Tracking of Bone Fragments During Craniofacial Surgery*, Second Annual International Symposium on Medical Robotics and Computer Assisted Surgery, pp. 221-225, (Nov. 1995).

Feldmar et al., "3D-2D Projective Registration of Free-Form Curves and Surfaces," *Rapport de recherche (Inria Sophia Antipolis)* (Dec. 1994) pp. 1-44.

Foley et al., "Fundamentals of Interactive Computer Graphics," *The Systems Programming Series*, Chapter 7, Jul. 1984, pp. 245-266.

Foley et al., "Image-guided Intraoperative Spinal Localization," *Intraoperative Neuroprotection*, Chapter 19, 1996, pp. 325-340.

Foley, "The StealthStation: Three-Dimensional Image-Interactive Guidance for the Spine Surgeon," *Spinal Frontiers*, Apr. 1996, pp. 7-9.

Friets, E.M., et al. A Frameless Stereotaxic Operating Microscope for Neurosurgery, *IEEE Trans. on Biomed. Eng.*, vol. 36, No. 6, pp. 608-617 (Jul. 1989).

Gallen, C.C., et al., *Intracranial Neurosurgery Guided by Functional Imaging*, *Surg. Neurol.*, vol. 42, pp. 523-530 (1994).

Galloway, R.L., et al., *Interactive Image-Guided Neurosurgery*, *IEEE Trans. on Biomed. Eng.*, vol. 89, No. 12, pp. 1226-1231 (1992).

Galloway, R.L., Jr. et al, *Optical localization for interactive, image-guided neurosurgery*, *SPIE*, vol. 2164, (May 1, 1994) pp. 137-145.

Germano, "Instrumentation, Technique and Technology", *Neurosurgery*, vol. 37, No. 2, Aug. 1995, pp. 348-350.

Gildenberg et al., "Calculation of Stereotactic Coordinates from the Computed Tomographic Scan," *Neurosurgery*, vol. 10, No. 5, May 1982, pp. 580-586.

Gomez, C.R., et al., *Transcranial Doppler Ultrasound Following Closed Head Injury: Vasospasm or Vasoparalysis?*, *Surg. Neurol.*, vol. 35, pp. 30-35 (1991).

Gonzalez, "Digital Image Fundamentals," *Digital Image Processing*, Second Edition, 1987, pp. 52-54.

Gottesfeld Brown et al., "Registration of Planar Film Radiographs with Computer Tomography," *Proceedings of MMBIA*, Jun. '96, pp. 42-51.

Grimson, W.E.L., *An Automatic Registration Method for Frameless Stereotaxy, Image Guided Surgery, and enhanced Reality Visualization*, *IEEE*, pp. 430-436 (1994).

Grimson, W.E.L., et al., *Virtual-reality technology is giving surgeons the equivalent of x-ray vision helping them to remove tumors more effectively, to minimize surgical wounds and to avoid damaging critical tissues*, *Sci. Amer.*, vol. 280, No. 6, pp. 62-69 (Jun. 1999).

Guezic et al., "Registration of Computed Tomography Data to a Surgical Robot Using Fluoroscopy: A Feasibility Study," *Computer Science/Mathematics*, Sep. 27, 1996, 6 pages.

Guthrie, B.L., *Graphic-Interactive Cranial Surgery: The Operating Arm System*, *Handbook of Stereotaxy Using the CRW Apparatus*, Chapter 13, (1994) pp. 193-211.

Hamadeh et al., "Kinematic Study of Lumbar Spine Using Functional Radiographies and 3D/2D Registration," *TIMC UMR 5525—IMAG* (Mar. 19-22, 1997).

Hamadeh et al., "Automated 3-Dimensional Computed Tomographic and Fluoroscopic Image Registration," *Computer Aided Surgery* (1998), 3:11-19.

Hamadeh et al., "Towards Automatic Registration Between CT and X-ray Images: Cooperation Between 3D/2D Registration and 2D Edge Detection," *MRCAS '95*, pp. 39-46.

Hardy, T., M.D., et al., *CASS: A Program for Computer Assisted Stereotaxic Surgery*, *The Fifth Annual Symposium on Computer Applications in Medical Care*, Proceedings, Nov. 1-4, 1981, *IEEE*, pp. 1116-1126 (Nov. 1-4, 1981).

- Hatch, "Reference-Display System for the Integration of CT Scanning and the Operating Microscope," Thesis, Thayer School of Engineering, Oct. 1984, pp. 1-189.
- Hatch, et al., "Reference-Display System for the Integration of CT Scanning and the Operating Microscope", Proceedings of the Eleventh Annual Northeast Bioengineering Conference, Mar. 14-15, 1985, pp. 252-254.
- Heilbrun et al., "Preliminary experience with Brown-Roberts-Wells (BRW) computerized tomography stereotaxic guidance system," *Journal of Neurosurgery*, vol. 59, Aug. 1983, pp. 217-222.
- Heilbrun, M.D., *Progressive Technology Applications, Neurosurgery for the Third Millennium*, Chapter 15, J. Whitaker & Sons, Ltd., Amer. Assoc. of Neurol. Surgeons, pp. 191-198 (Oct. 1992).
- Heilbrun, M.P., *Computed Tomography—Guided Stereotactic Systems*, *Clinical Neurosurgery*, Chapter 31, pp. 564-581 (1983).
- Heilbrun, M.P., et al., *Stereotactic Localization and Guidance Using a Machine Vision Technique*, *Stereotact & Funct. Neurosurg.*, Proceed. of the Mtg. of the Amer. Soc. for Sterot. and Funct. Neurosurg. (Pittsburgh, PA) vol. 58, pp. 94-98 (Sep. 1992).
- Henderson et al., "An Accurate and Ergonomic Method of Registration for Image-guided Neurosurgery," *Computerized Medical Imaging and Graphics*, vol. 18, No. 4, Jul.-Aug. 1994, pp. 273-277.
- Hoerenz, "The Operating Microscope I. Optical Principles, Illumination Systems, and Support Systems," *Journal of Microsurgery*, vol. 1 (Mar./Apr. 1980) pp. 364-369.
- Hofstetter et al., "Fluoroscopy Based Surgical Navigation—Concept and Clinical Applications," *Computer Assisted Radiology and Surgery* (Jun. 1997) pp. 956-960.
- Horner et al., "A Comparison of CT-Stereotaxic Brain Biopsy Techniques," *Investigative Radiology*, Sep.-Oct. 1984, pp. 367-373.
- Hounsfield, "Computerized transverse axial scanning (tomography): Part 1. Description of system," *British Journal of Radiology*, vol. 46, No. 552, Dec. 1973, pp. 1016-1022.
- Jacques et al., "A Computerized Microstereotactic Method to Approach, 3-Dimensionally Reconstruct, Remove and Adjuvantly Treat Small CNS Lesions," *Applied Neurophysiology*, vol. 43, 1980, pp. 176-182.
- Jacques et al., "Computerized three-dimensional stereotaxic removal of small central nervous system lesion in patients," *J. Neurosurg.*, vol. 53, Dec. 1980, pp. 816-820.
- Joskowicz et al., "Computer-Aided Image-Guided Bone Fracture Surgery: Concept and Implementation," *CAR '98*, pp. 710-715.
- Kall, B., *The Impact of Computer and Imaging Technology on Stereotactic Surgery*, Proceedings of the Meeting of the American Society for Stereotactic and Functional Neurosurgery, pp. 10-22 (1987).
- Kato, A., et al., *A frameless, armless navigational system for computer-assisted neurosurgery*, *J. Neurosurg.*, vol. 74, pp. 845-849 (May 1991).
- Kelly et al., "Computer-assisted stereotaxic laser resection of intra-axial brain neoplasms," *Journal of Neurosurgery*, vol. 64, Mar. 1986, pp. 427-439.
- Kelly et al., "Precision Resection of Intra-Axial CNS Lesions by CT-Based Stereotactic Craniotomy and Computer Monitored CO₂ Laser," *Acta Neurochirurgica*, vol. 68, 1983, pp. 1-9.
- Kelly, P.J., *Computer Assisted Stereotactic Biopsy and Volumetric Resection of Pediatric Brain Tumors*, *Brain Tumors in Children*, *Neurologic Clinics*, vol. 9, No. 2, pp. 317-336 (May 1991).
- Kelly, P.J., *Computer-Directed Stereotactic Resection of Brain Tumors*, *Neurologica Operative Atlas*, vol. 1, No. 4, pp. 299-313 (1991).
- Kelly, P.J., et al., *Results of Computed Tomography-based Computer-assisted Stereotactic Resection of Metastatic Intracranial Tumors*, *Neurosurgery*, vol. 22, No. 1, Part 1, 1988, pp. 7-17 (Jan. 1988).
- Kelly, P.J., *Stereotactic Imaging, Surgical Planning and Computer-Assisted Resection of Intracranial Lesions: Methods and Results*, *Advances and Technical Standards in Neurosurgery*, vol. 17, pp. 78-118, (1990).
- Kim, W.S. et al., *A Helmet Mounted Display for Telerobotics*, *IEEE*, pp. 543-547 (1988).
- Klimek, L., et al., *Long-Term Experience with Different Types of Localization Systems in Skull-Base Surgery, Ear, Nose & Throat Surgery*, Chapter 51, (1996) pp. 635-638.
- Kosugi, Y., et al., *An Articulated Neurosurgical Navigation System Using MRI and CT Images*, *IEEE Trans. on Biomed. Eng.* vol. 35, No. 2, pp. 147-152 (Feb. 1988).
- Krybus, W., et al., *Navigation Support for Surgery by Means of Optical Position Detection*, *Computer Assisted Radiology Proceed. of the Intl. Symp. CAR '91 Computed Assisted Radiology*, pp. 362-366 (Jul. 3-6, 1991).
- Kwoh, Y.S., Ph.D., et al., *A New Computerized Tomographic-Aided Robotic Stereotaxis System*, *Robotics Age*, vol. 7, No. 6, pp. 17-22 (Jun. 1985).
- Laitinen et al., "An Adapter for Computed Tomography-Guided, Stereotaxis," *Surg. Neurol.*, 1985, pp. 559-566.
- Laitinen, "Noninvasive multipurpose stereoadapter," *Neurological Research*, Jun. 1987, pp. 137-141.
- Lavallee et al., "Matching 3-D Smooth Surfaces with their 2-D Projections using 3-D Distance Maps," *SPIE*, vol. 1570, *Geometric Methods in Computer Vision*, 1991, pp. 322-336.
- Lavallee et al., "Computer Assisted Driving of a Needle into the Brain," *Proceedings of the International Symposium CAR '89, Computer Assisted Radiology*, 1989, pp. 416-420.
- Lavallee et al., "Computer Assisted Interventionist Imaging: The Instance of Stereotactic Brain Surgery," *North-Holland MEDINFO 89, Part 1*, 1989, pp. 613-617.
- Lavallee et al., "Computer Assisted Spine Surgery: A Technique For Accurate Transpedicular Screw Fixation Using CT Data and a 3-D Optical Localizer," *TIMC, Faculte de Medecine de Grenoble*. (1995).
- Lavallee et al., "Image guided operating robot: a clinical application in stereotactic neurosurgery," *Proceedings of the 1992 IEEE International Conference on Robotics and Automation*, May 1992, pp. 618-624.
- Lavallee et al., "Matching of Medical Images for Computed and Robot Assisted Surgery," *IEEE EMBS, Orlando* (Oct. 31-Nov. 3, 1991).
- Lavallee, "A New System for Computer Assisted Neurosurgery," *IEEE Engineering in Medicine & Biology Society 11th Annual International Conference*, 1989, pp. 0926-0927.
- Lavallee, "VI Adaption de la Methodologie a Quelques Applications Cliniques," *Chapitre VI*, pp. 133-148.
- Lavallee, S., et al., *Computer Assisted Knee Anterior Cruciate Ligament Reconstruction First Clinical Tests*, *Proceedings of the First International Symposium on Medical Robotics and Computer Assisted Surgery*, pp. 11-16 (Sep. 1994).
- Lavallee, S., et al., *Computer Assisted Medical Interventions*, *NATO ASI Series*, vol. F 60, *3d Imaging in Medic.*, pp. 301-312 (1990).
- Leavitt, D.D., et al., *Dynamic Field Shaping to Optimize Stereotactic Radiosurgery*, *I.J. Rad. Onc. Biol. Physc.*, vol. 21, pp. 1247-1255 (Oct. 1991).
- Leksell et al., "Stereotaxis and Tomography—A Technical Note," *ACTA Neurochirurgica*, vol. 52, 1980, pp. 1-7.
- Lemieux et al., "A Patient-to-Computed-Tomography Image Registration Method Based on Digitally Reconstructed Radiographs," *Med. Phys.* 21 (11), Nov. 1994, pp. 1749-1760.
- Levin et al., "The Brain: Integrated Three-dimensional Display of MR and PET Images," *Radiology*, vol. 172, No. 3, Sep. 1989, pp. 783-789.
- Maurer, Jr., et al., *Registration of Head CT Images to Physical Space Using a Weighted Combination of Points and Surfaces*, *IEEE Trans. on Med. Imaging*, vol. 17, No. 5, pp. 753-761 (Oct. 1998).
- Mazier et al., "Computer-Assisted Interventionist Imaging: Application to the Vertebral Column Surgery," *Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 12, No. 1, 1990, pp. 0430-0431.
- Mazier et al., *Chirurgie de la Colonne Vertebrale Assiste par Ordinateur: Application au Vissage Pediculaire*, *Innov. Tech. Biol. Med.*, vol. 11, No. 5, 1990, pp. 559-566.
- McGirr, S., M.D., et al., *Stereotactic Resection of Juvenile Pilocytic Astrocytomas of the Thalamus and Basal Ganglia*, *Neurosurgery*, vol. 20, No. 3, pp. 447-452, (Mar. 1987).
- Merloz, et al., "Computer Assisted Spine Surgery", *Clinical Assisted Spine Surgery*, No. 337, (Apr. 1997) pp. 86-96.

- Ng, W.S. et al., Robotic Surgery—A First-Hand Experience in Transurethral Resection of the Prostate Surgery, *IEEE Eng. in Med. and Biology*, pp. 120-125 (Mar. 1993).
- Pelizzari et al., "Accurate Three-Dimensional Registration of CT, PET, and/or MR Images of the Brain," *Journal of Computer Assisted Tomography*, Jan./Feb. 1989, pp. 20-26.
- Pelizzari et al., "Interactive 3D Patient-Image Registration," *Information Processing in Medical Imaging*, 12th International Conference, IPMI '91, Jul. 7-12, 136-141 (A.C.F. Colchester et al. eds. 1991).
- Pelizzari et al., No. 528—"Three Dimensional Correlation of PET, CT and MRI Images," *The Journal of Nuclear Medicine*, vol. 28, No. 4, Apr. 1987, p. 682.
- Penn, R.D., et al., Stereotactic Surgery with Image Processing of Computerized Tomographic Scans, *Neurosurgery*, vol. 3, No. 2, pp. 157-163 (Sep.-Oct. 1978).
- Phillips et al., "Image Guided Orthopaedic Surgery Design and Analysis," *Trans Inst. MC*, vol. 17, No. 5, 1995, pp. 251-264.
- Pixsys, 3-D Digitizing Accessories, by Pixsys (marketing brochure) (date unknown) (2 pages).
- Potamianos et al., "Intra-Operative Imaging Guidance for Keyhole Surgery Methodology and Calibration," *First International Symposium on Medical Robotics and Computer Assisted Surgery*, Sep. 22-24, 1994, pp. 98-104.
- Reinhardt et al., "CT-Guided 'Real Time' Stereotaxy," *ACTA Neurochirurgica*, 1989.
- Reinhardt, H., et al., A Computer-Assisted Device for Intraoperative CT-Correlated Localization of Brain Tumors, pp. 51-58 (1988).
- Reinhardt, H.F. et al., Sonic Stereometry in Microsurgical Procedures for Deep-Seated Brain Tumors and Vascular Malformations, *Neurosurgery*, vol. 32, No. 1, pp. 51-57 (Jan. 1993).
- Reinhardt, H.F., et al., Mikrochirurgische Entfernung tiefliegender Gefäßmißbildungen mit Hilfe der Sonar-Stereometrie (Microsurgical Removal of Deep-Seated Vascular Malformations Using Sonar Stereometry). *Ultraschall in Med.* 12, pp. 80-83 (1991).
- Reinhardt, Hans. F., Neuronavigation: A Ten-Year Review, *Neurosurgery*, (1996) pp. 329-341.
- Roberts et al., "A frameless stereotaxic integration of computerized tomographic imaging and the operating microscope," *J. Neurosurg.*, vol. 65, Oct. 1986, pp. 545-549.
- Rosenbaum et al., "Computerized Tomography Guided Stereotaxis: A New Approach," *Applied Neurophysiology*, vol. 43, No. 3-5, 1980, pp. 172-173.
- Sautot, "Vissage Pediculaire Assiste Par Ordinateur," Sep. 20, 1994.
- Schueler et al., "Correction of Image Intensifier Distortion for Three-Dimensional X-Ray Angiography," *SPIE Medical Imaging* (Feb. 26-27, 1995) vol. 2432, pp. 272-279.
- Selvik et al., "A Roentgen Stereophotogrammetric System," *Acta Radiologica Diagnosis*, 1983, pp. 343-352.
- Shelden et al., "Development of a computerized microstereotaxic method for localization and removal of minute CNS lesions under direct 3-D vision," *J. Neurosurg.*, vol. 52 (Jan. 1980) pp. 21-27.
- Simon, D.A., Accuracy Validation in Image-Guided Orthopaedic Surgery, *Second Annual Intl. Symp. on Med. Rob. and Comp-Assisted surgery*, MRCAS (1995) pp. 185-192.
- Smith et al., "Computer Methods for Improved Diagnostic Image Display Applied to Stereotactic Neurosurgery," *Automedical*, vol. 14, 1992, pp. 371-382 (4 unnumbered pages).
- Smith et al., "The Neurostation™—A Highly Accurate, Minimally Invasive Solution to Frameless Stereotactic Neurosurgery," *Computerized Medical Imaging and Graphics*, vol. 18, Jul.-Aug. 1994, pp. 247-256.
- Smith, K.R., et al. Multimodality Image Analysis and Display Methods for Improved Tumor Localization in Stereotactic Neurosurgery, *Annul Intl. Conf. of the IEEE Eng. in Med. and Biol. Soc.*, vol. 13, No. 1, p. (Oct. 31-Nov. 3, 1991).
- Tan, K., Ph.D., et al., A frameless stereotactic approach to neurosurgical planning based on retrospective patient-image registration, *J Neurosurg*, vol. 79, pp. 296-303 (Aug. 1993).
- The Laitinen Stereotactic System, E2-E6.
- Thompson, et al., A System for Anatomical and Functional Mapping of the Human Thalamus, *Computers and Biomedical Research*, vol. 10, pp. 9-24 (1977).
- Trobraugh, J.W., et al., Frameless Stereotactic Ultrasonography: Method and Applications, *Computerized Medical Imaging and Graphics*, vol. 18, No. 4, pp. 235-246 (Jul.-Aug. 1994).
- Viant et al., "A Computer Assisted Orthopaedic System for Distal Locking of Intramedullary Nails," *Proc. of MediMEC '95*, Bristol, 1995, pp. 86-91.
- Von Hanwhr et al., Foreword, *Computerized Medical Imaging and Graphics*, vol. 18, No. 4, pp. 225-228, (Jul.-Aug. 1994).
- Wang, M.Y., et al., An Automatic Technique for Finding and Localizing Externally Attached Markers in CT and MR Volume Images of the Head, *IEEE Trans. on Biomed. Eng.*, vol. 43, No. 6, pp. 627-637 (Jun. 1996).
- Watanabe et al., "Three-Dimensional Digitizer (Neuronavigator): New Equipment for Computed Tomography-Guided Stereotaxic Surgery," *Surgical Neurology*, vol. 27, No. 6, Jun. 1987, pp. 543-547.
- Watanabe, "Neuronavigator," *Igaku-no-Ayumi*, vol. 137, No. 6, May 10, 1986, pp. 1-4.
- Watanabe, E., M.D., et al., Open Surgery Assisted by the Neuronavigator, a Stereotactic, Articulated Sensitive Arm, *Neurosurgery*, vol. 28, No. 6, pp. 792-800 (Jun. 1991).
- Weese et al., "An Approach to 2D/3D Registration of a Vertebra in 2D X-ray Fluoroscopies with 3D CT Images," (Mar. 19-22, 1997) pp. 119-128.
- Office Action mailed Dec. 12, 2008 for U.S. Appl. No. 11/451,594, filed Jun. 12, 2006, now RE42,194 issued Mar. 1, 2011.
- Final Office Action mailed Sep. 21, 2009 for U.S. Appl. No. 11/451,594, filed Jun. 12, 2006, now RE42,194 issued Mar. 1, 2011.
- OA mailed Dec. 12, 2008 for U.S. Appl. No. 11/451,595, filed Jun. 12, 2006, now RE42,226 issued Mar. 15, 2011.
- Final OA mailed Sep. 21, 2009 for U.S. Appl. No. 11/451,595, filed Jun. 12, 2006, now RE42,226 issued Mar. 15, 2011.
- Final OA mailed Apr. 13, 2010 for U.S. Appl. No. 11/451,595, filed Jun. 12, 2006, now RE42,226 issued Mar. 15, 2011.
- Weinstein, et al., Spinal Pedicle Fixation: Reliability and Validity of Roentgenogram-Based Assessment and Surgical Factors on Successful Screw Placement, *Spine*, vol. 13, No. 9, 1988, pp. 1012-1018.
- Kelly, The NeuroStation System for Image-Guided, Frameless Stereotaxy, *Neurosurgery*, vol. 37, No. 2, Aug. 1995, pp. 348-350.
- Vector Vision: The Power of Surgical Tracking, *BrainLab*, 1997.
- J.F. Mallet, et al., Post-Laminectomy Cervical-Thoracic Kyphosis in a Patient with Von Recklinghausen's Disease, *Spinal Frontiers*, vol. Three, Issue One, Apr. 1996, pp. 1-15.
- Bucholz, et al., Image-Guided Surgical Techniques for Infections and Trauma of the Central Nervous System, *Neurosurgery Clinics of North America*, vol. 7, No. 2, Apr. 1996, pp. 187-200.
- Foley, et al., Image-guided Intraoperative Spinal Localization, *Intraoperative Neuroprotection: Monitoring*, Part Three, 1996, pp. 325-340.
- Mazier, et al., Computer Assisted Interventionist Imaging: Application to the Vertebral Column Surgery, *Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 12, No. 1, 1990, pp. 0430-0431.
- Lavallée, et al., Computer Assisted Medical Interventions, *NATO ASI Series*, vol. F 60, 1990, pp. 301-312.
- Adams et al., Computer-Assisted Surgery, *IEEE Computer Graphics & Applications*, May 1990, pp. 43-51.
- 3-D Digitizer Captures the World, *BYTE*, Oct. 1990, p. 43.
- Reinhardt, et al., Interactive Sonar-Operated Device for Stereotactic and Open Surgery, *Proceedings of the Xth Meeting of the World Society for Stereotactic and Functional Neurosurgery*, Maebashi, Japan, Oct. 1989, pp. 393-397.
- Kato, et al., A frameless, armless navigational system for computer-assisted neurosurgery, *J. Neurosurg* 74, 1991, pp. 845-849.
- Smith et al., Multimodality Image Analysis and Display Methods for Improved Tumor Localization in Stereotactic Neurosurgery, *Proceedings of the Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 13, 1991, p. 0210.
- Sautot et al., Computer Assisted Spine Surgery: a first step toward clinical application in orthopaedics, *IEEE*, 1992, p. 1071-1072.

Cinquin, et al., GOR: Image Guided Operating Robot. Methodology, Applications, *IEEE EMBS*, Paris 1992, pp. 1-2.

Alignment Procedure for the PixSys Two-Emitter Offset Probe for the SAC GP-8-3d Sonic Digitizer, *PixSys*, Jul. 2, 1992, pp. 1-4.

Smith, et al., Computer Methods for Improved Diagnostic Image Display Applied to Stereotactic Neurosurgery, *Automedica*, 1992, vol. 14, pp. 371-382.

Reinhardt, Neuronavigation: A Ten-Year Review, *Neurosurgery*, 1993, pp. 329-341.

Bucholz, et al., Intraoperative localization using a three dimensional optical digitizer, *SPIE* vol. 1894, Jan. 17, 1993, pp. 312-322.

Smith, et al., The Neurostation™—A Highly Accurate, Minimally Invasive Solution to Frameless Stereotactic Neurosurgery, *Computerized Medical Imaging and Graphics*, vol. 18, 1994, pp. 247-256.

Bucholz, et al., Halo vest versus spinal fusion for cervical injury: evidence from an outcome study, *J. Neurosurg.*, vol. 70, pp. 884-892.

Awwad, et al., Post-traumatic Spinal Synovial Cyst with Spondylolysis: CT Features, *Journal of Computer Assisted Tomography*, vol. 13, No. 2, 1989, pp. 334-337.

* cited by examiner

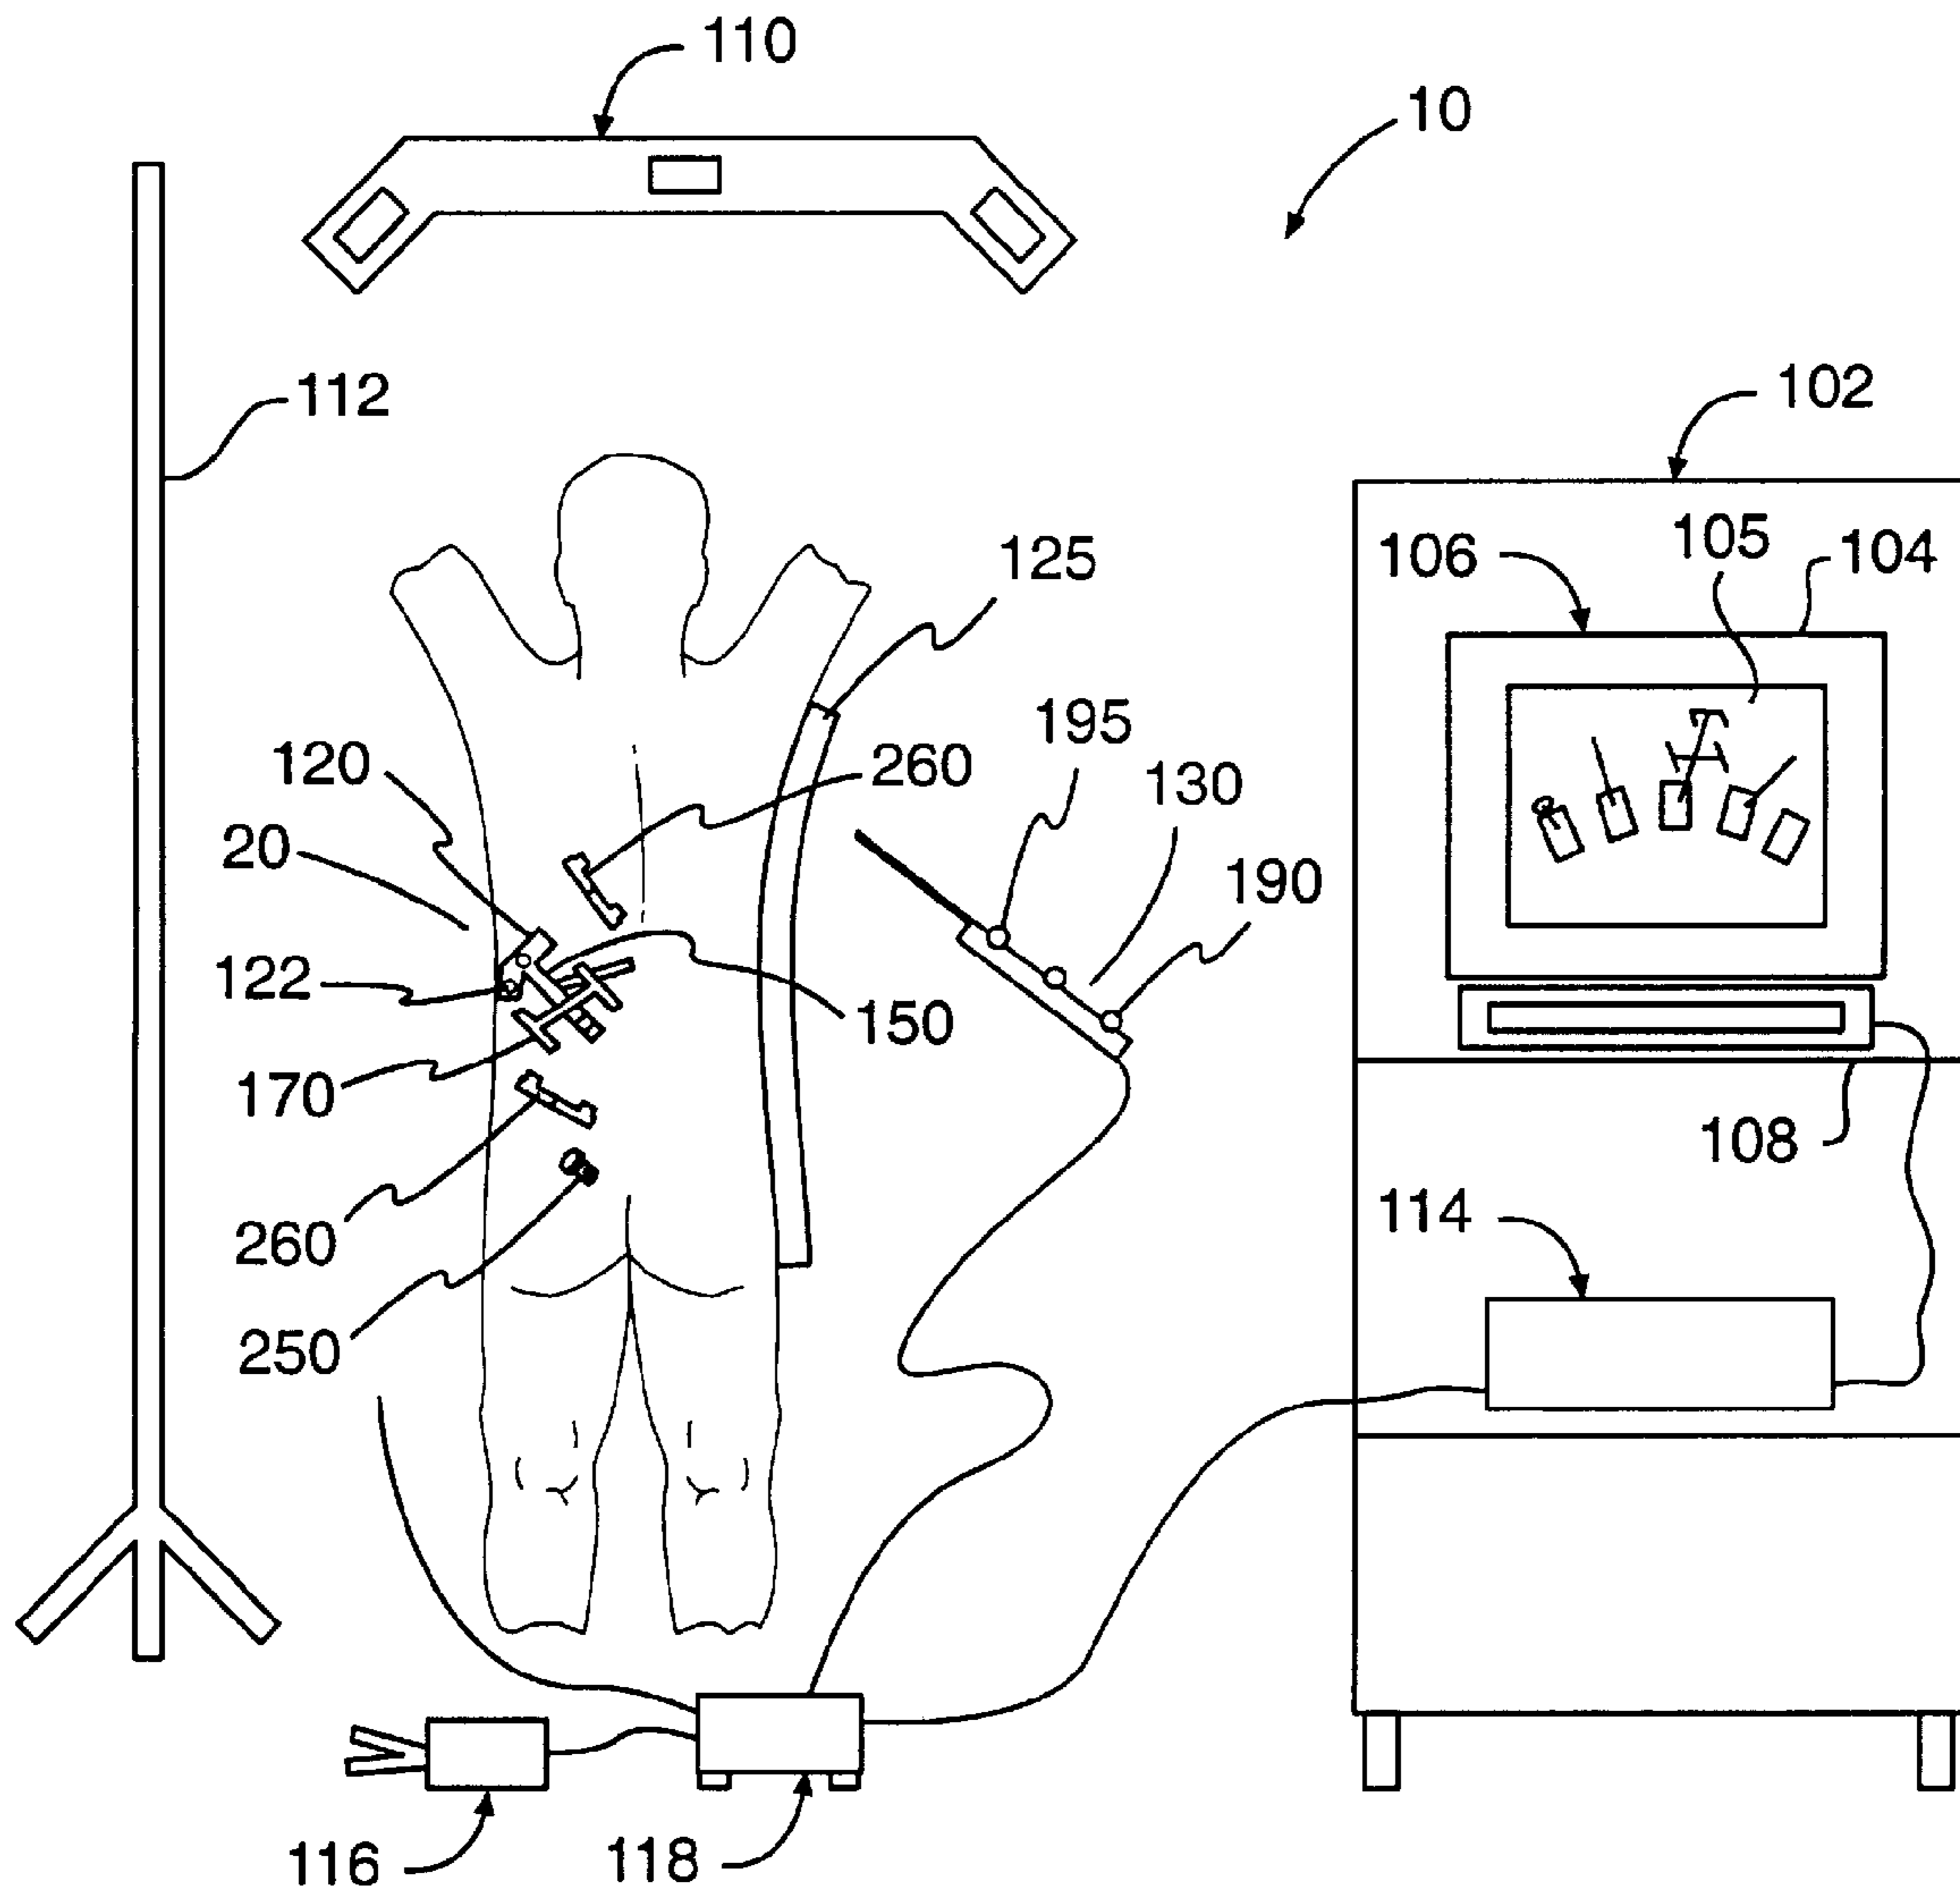


FIG. 1

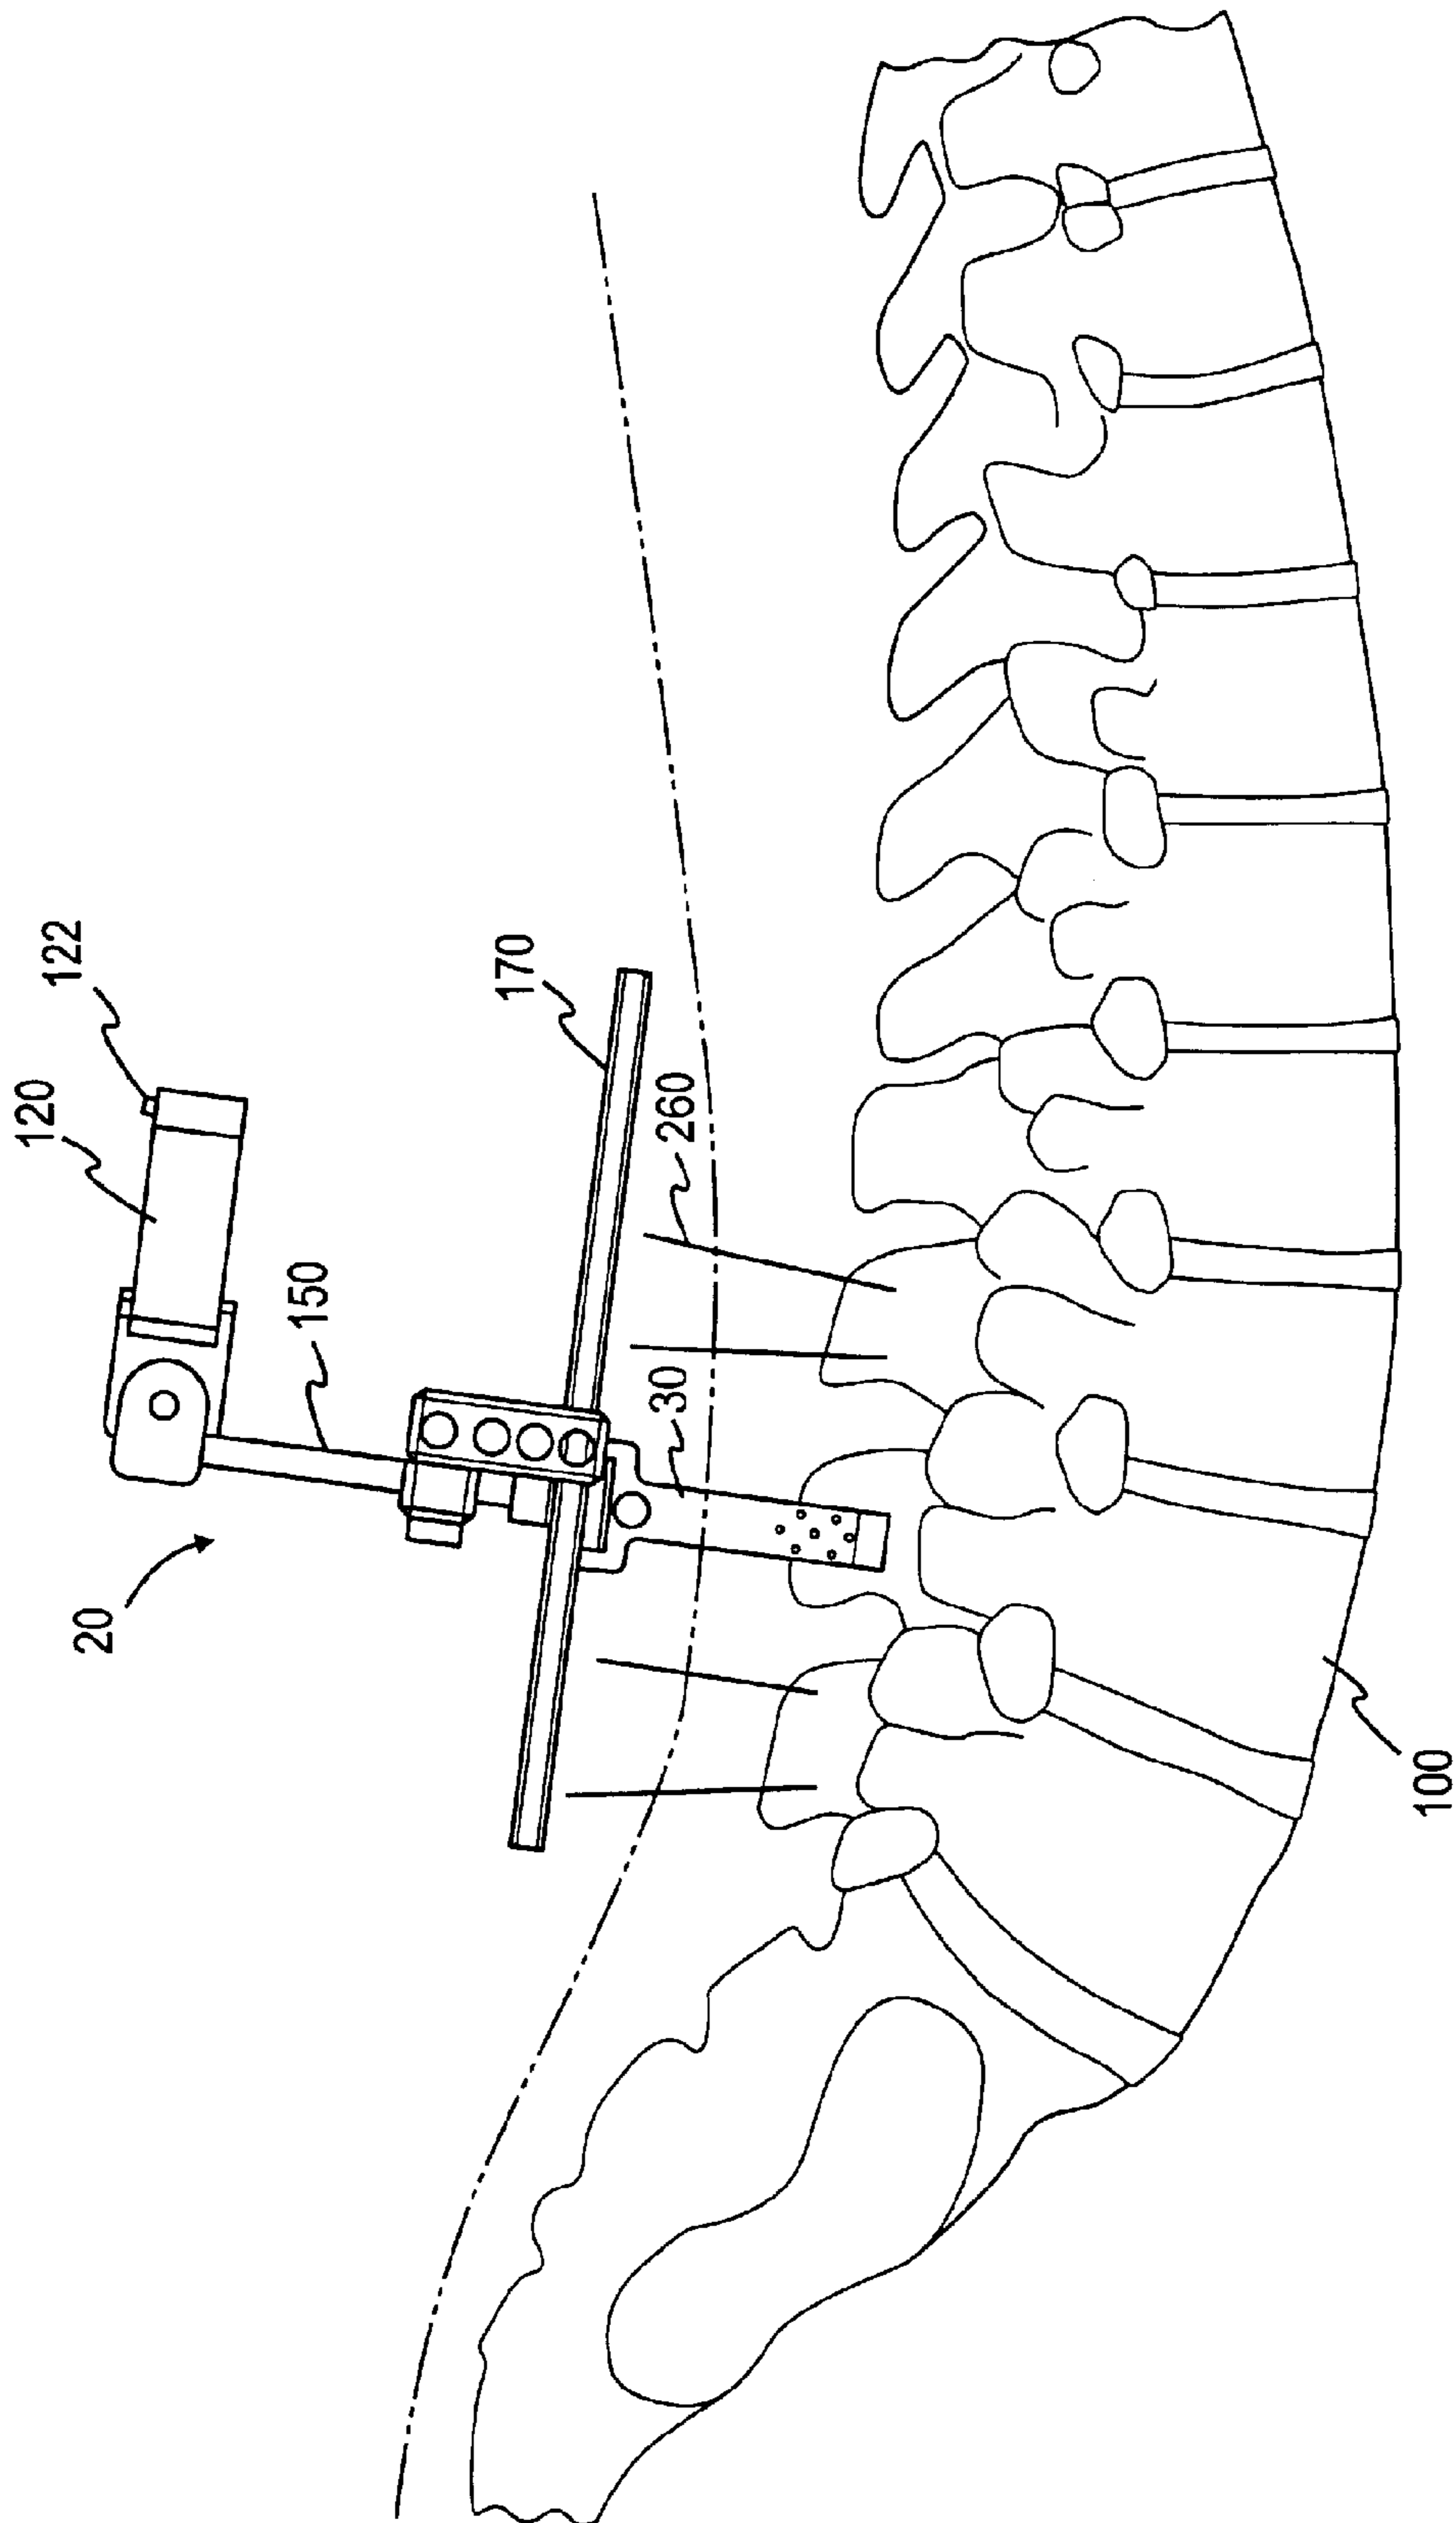


FIG. 1A

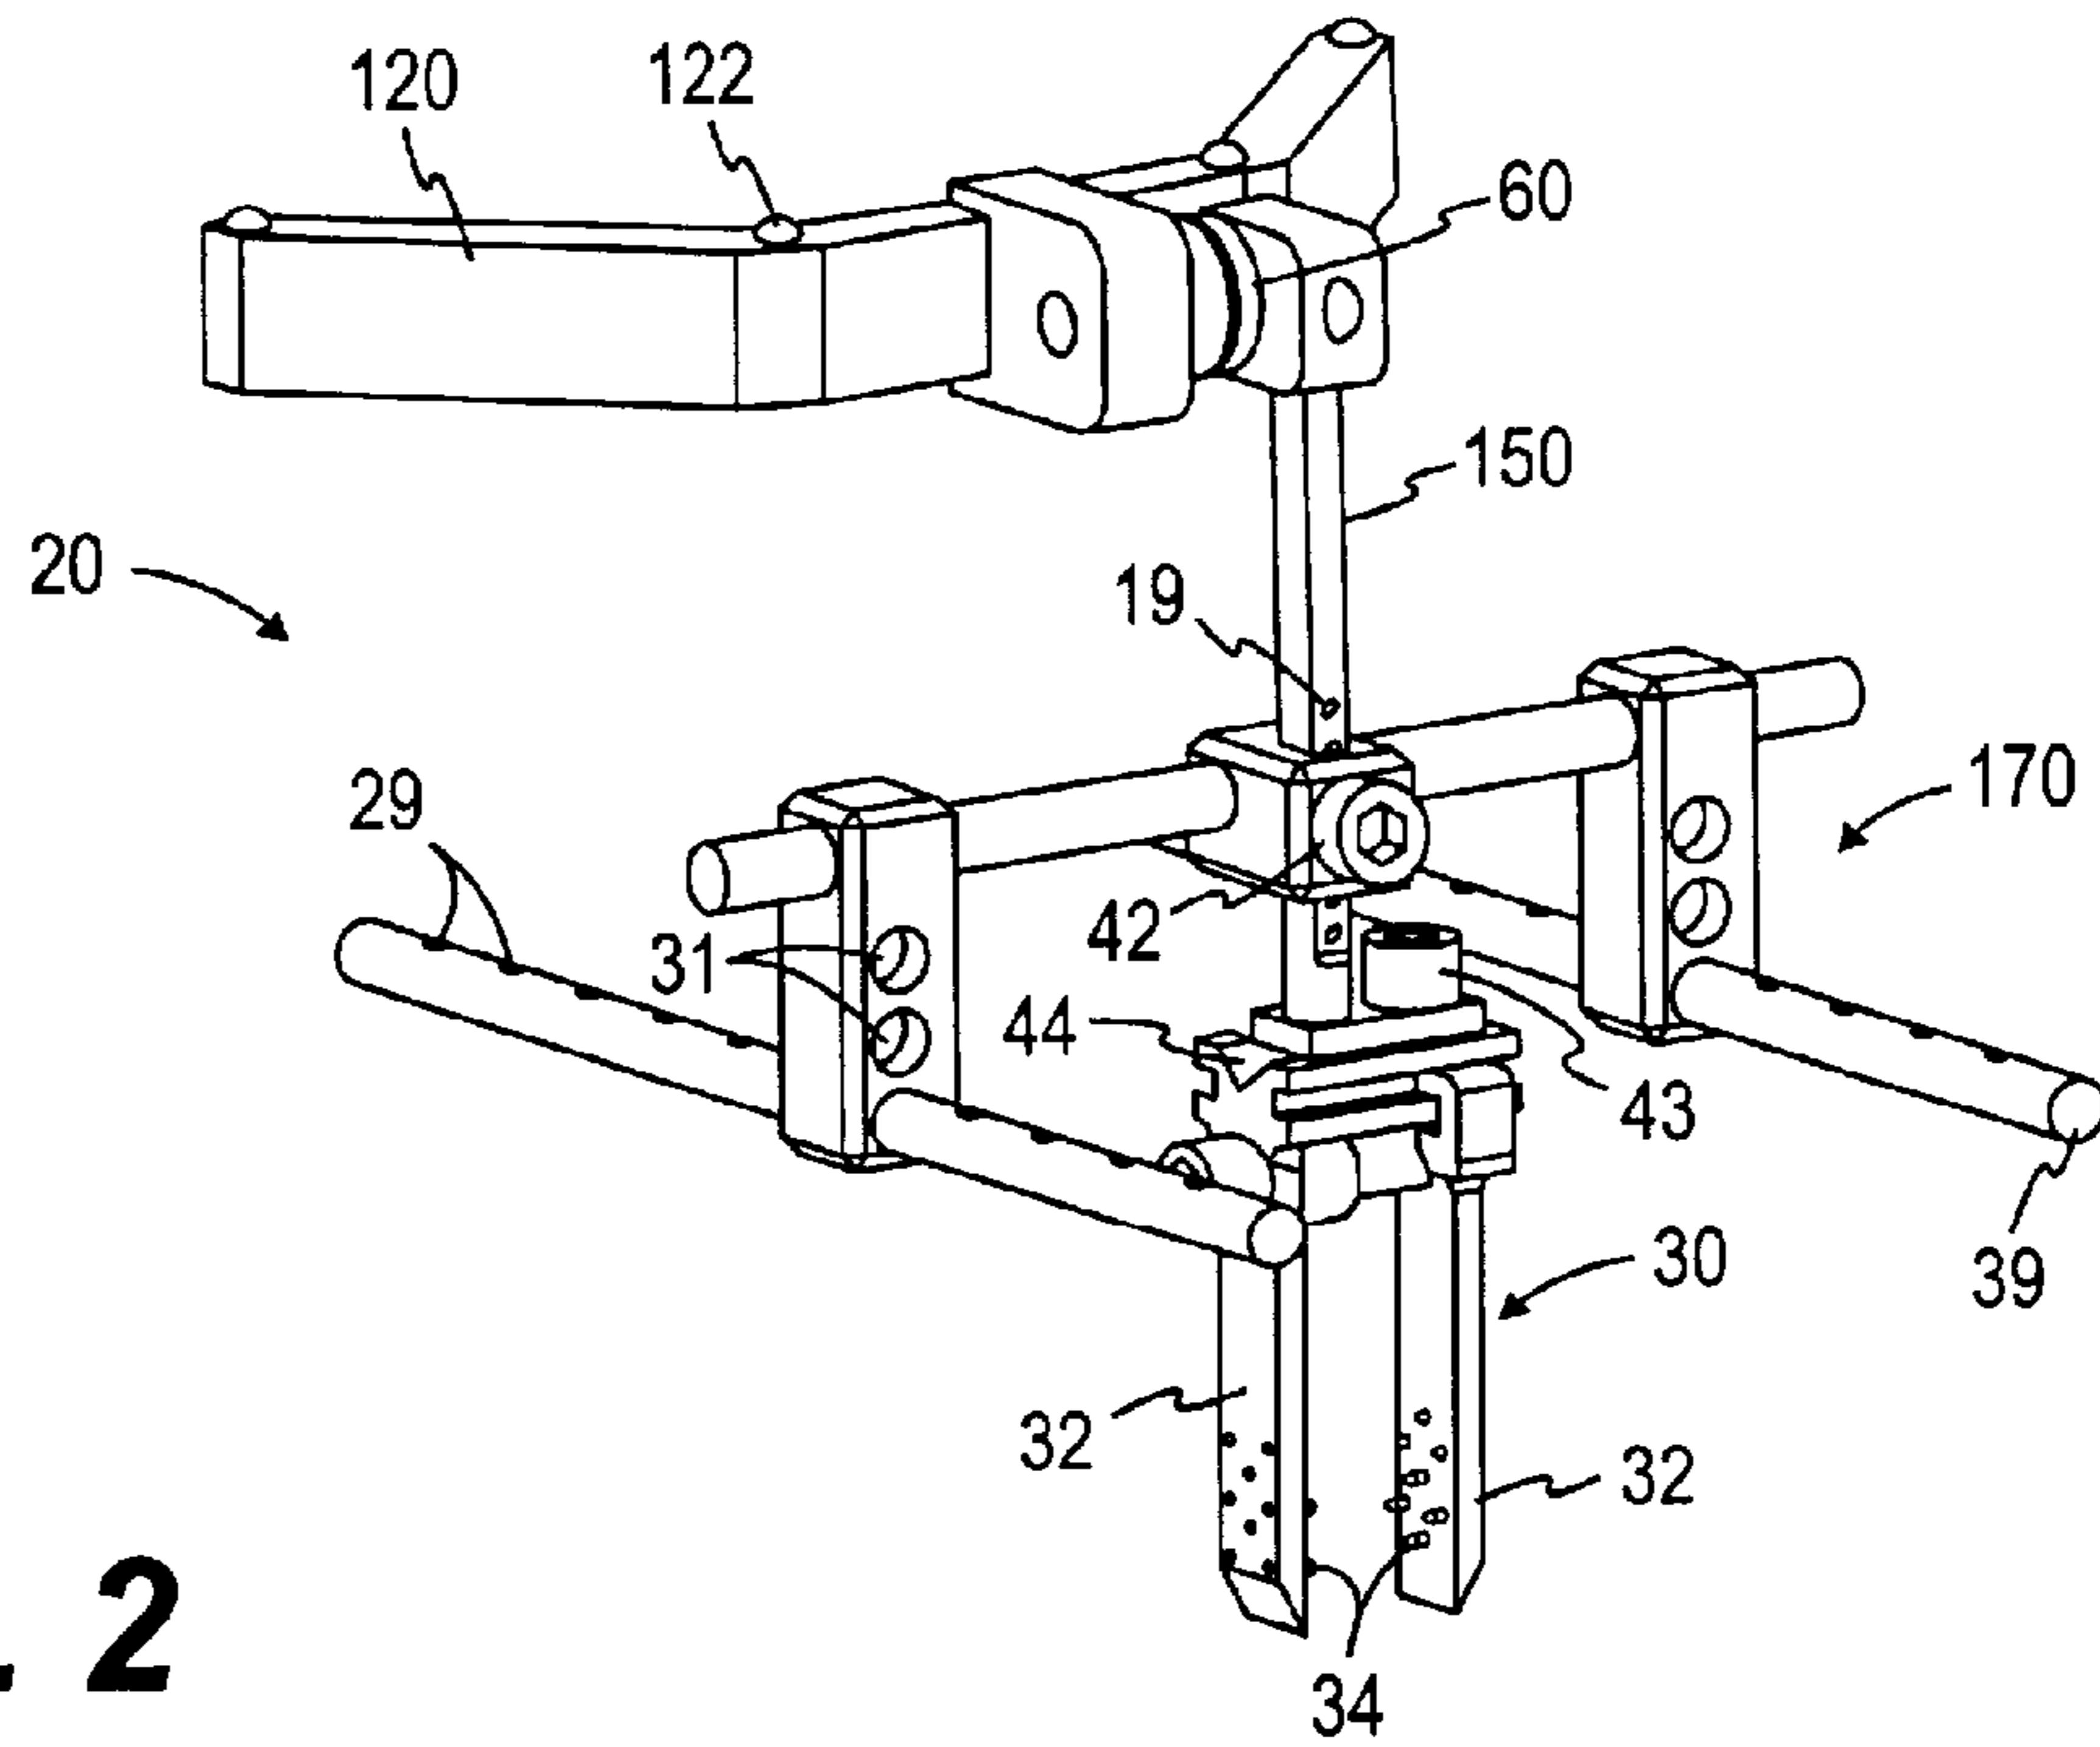


FIG. 2

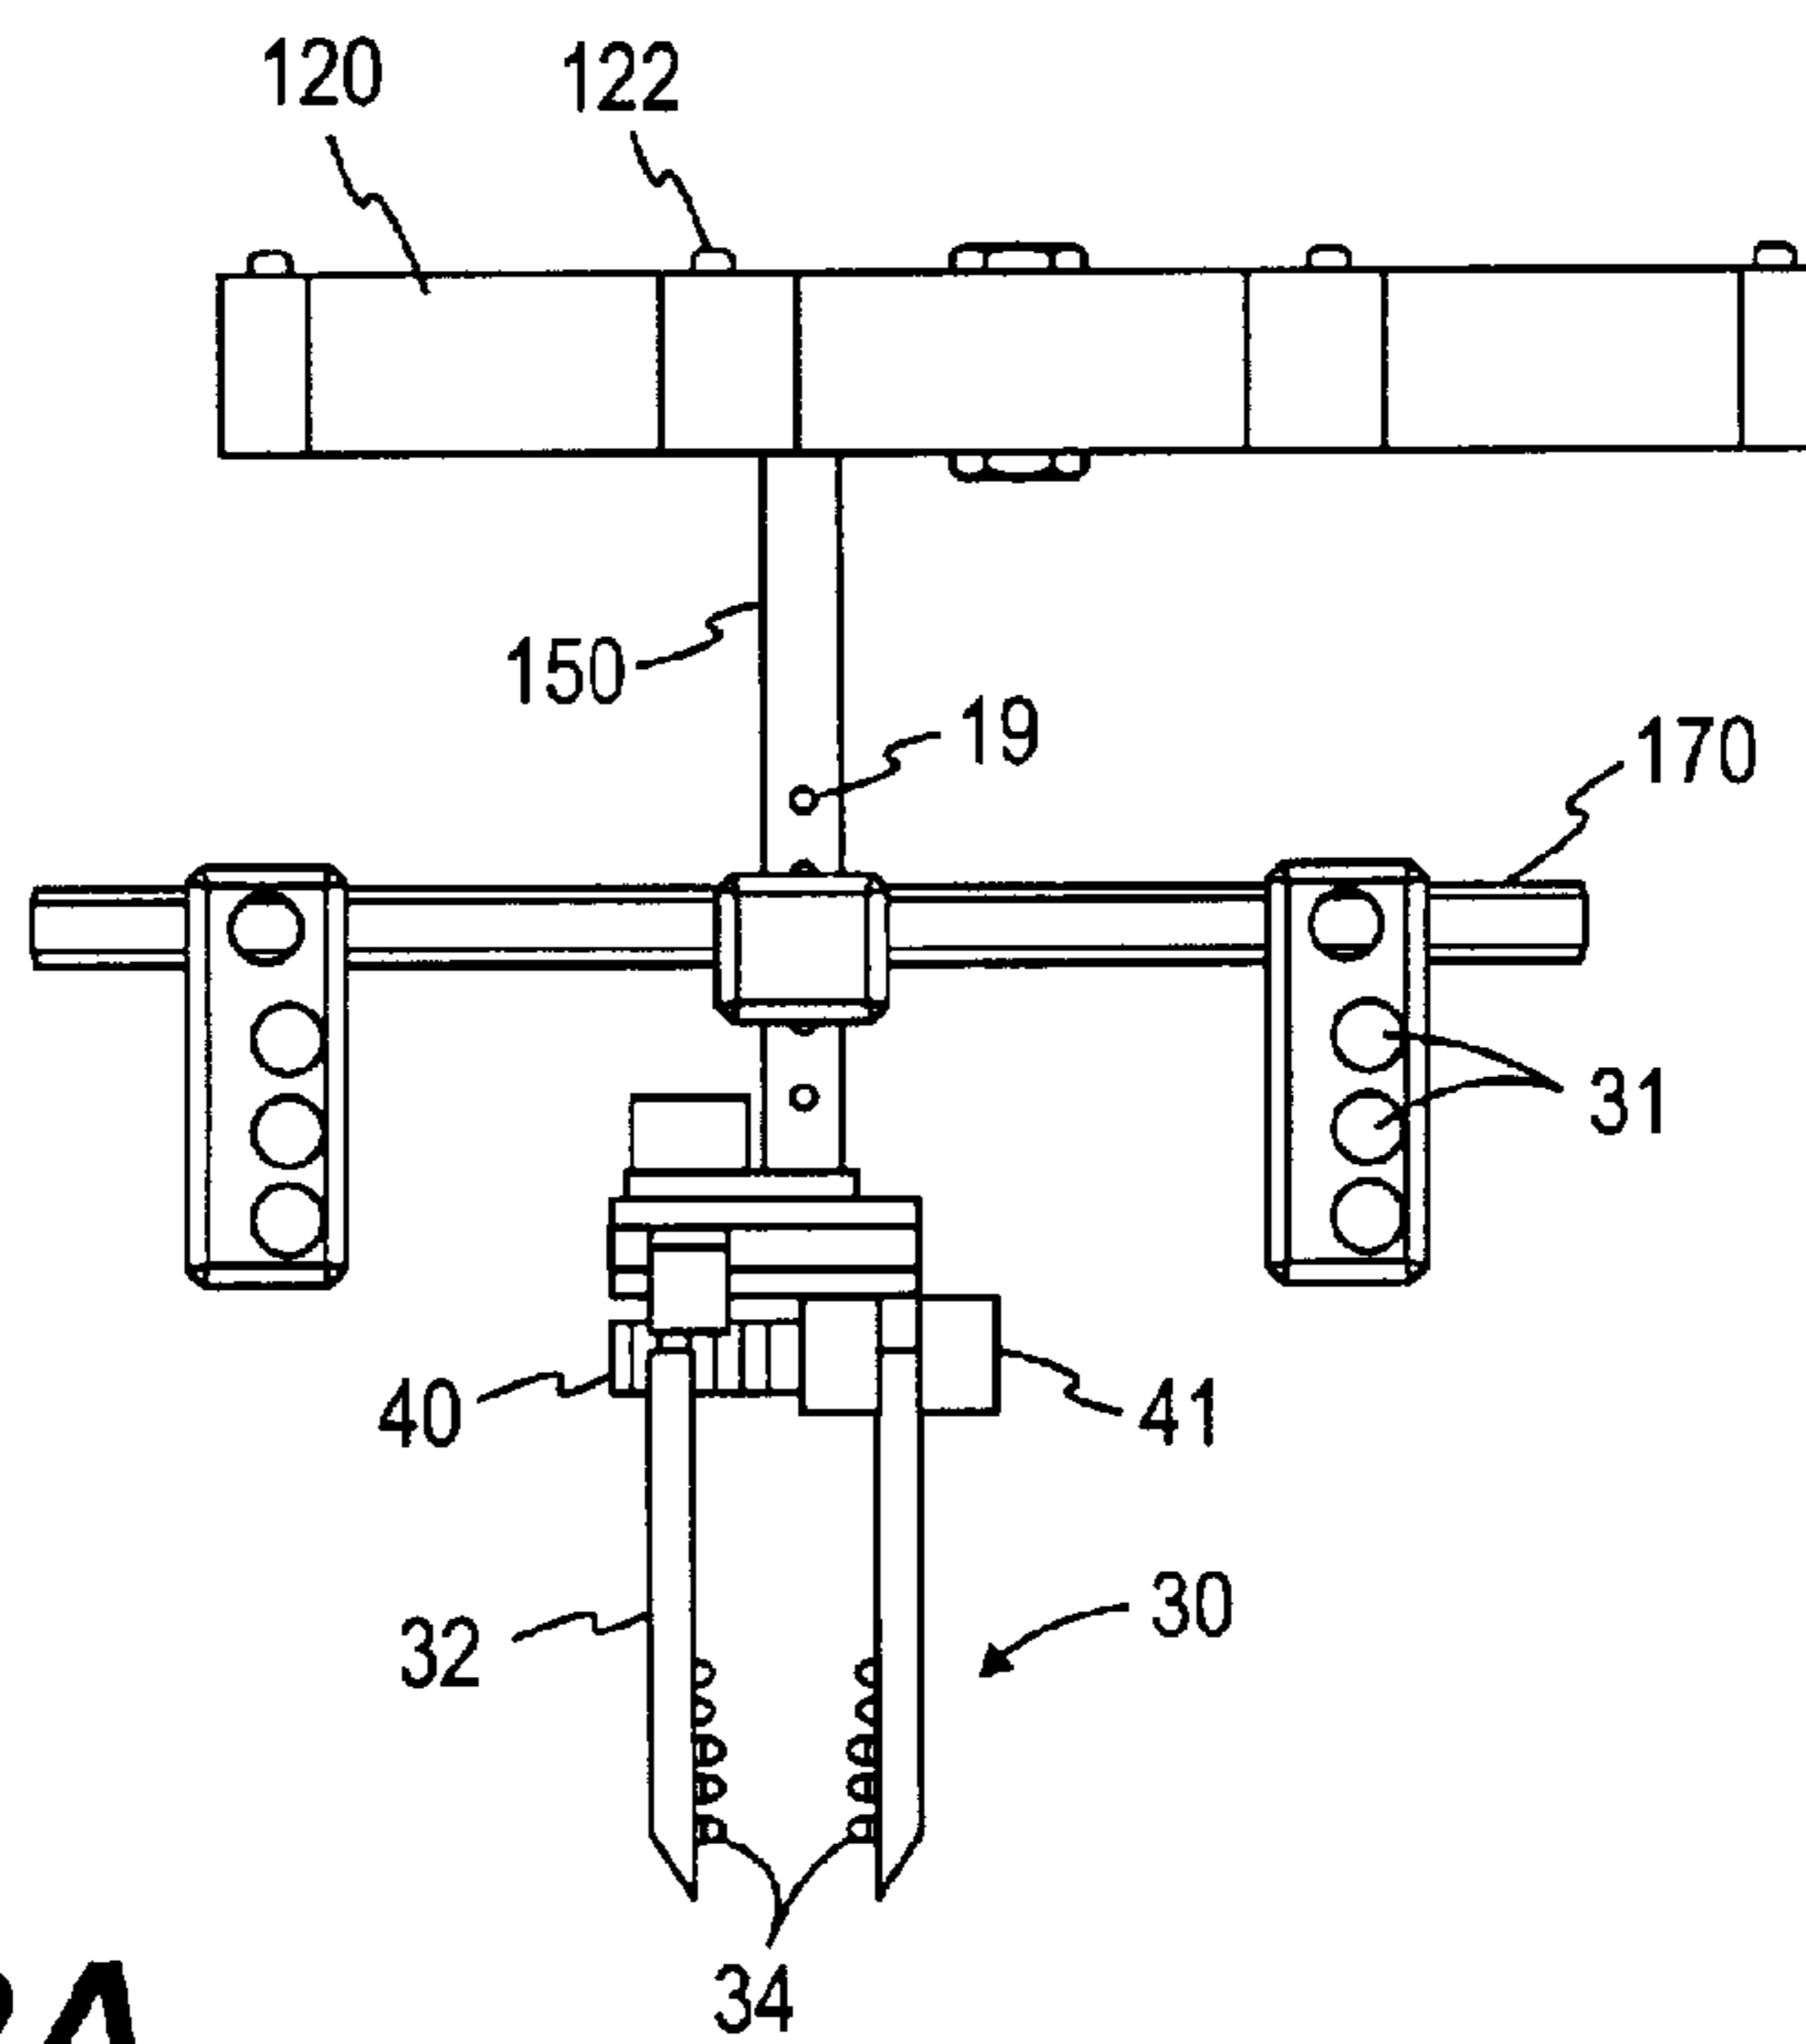


FIG. 2A

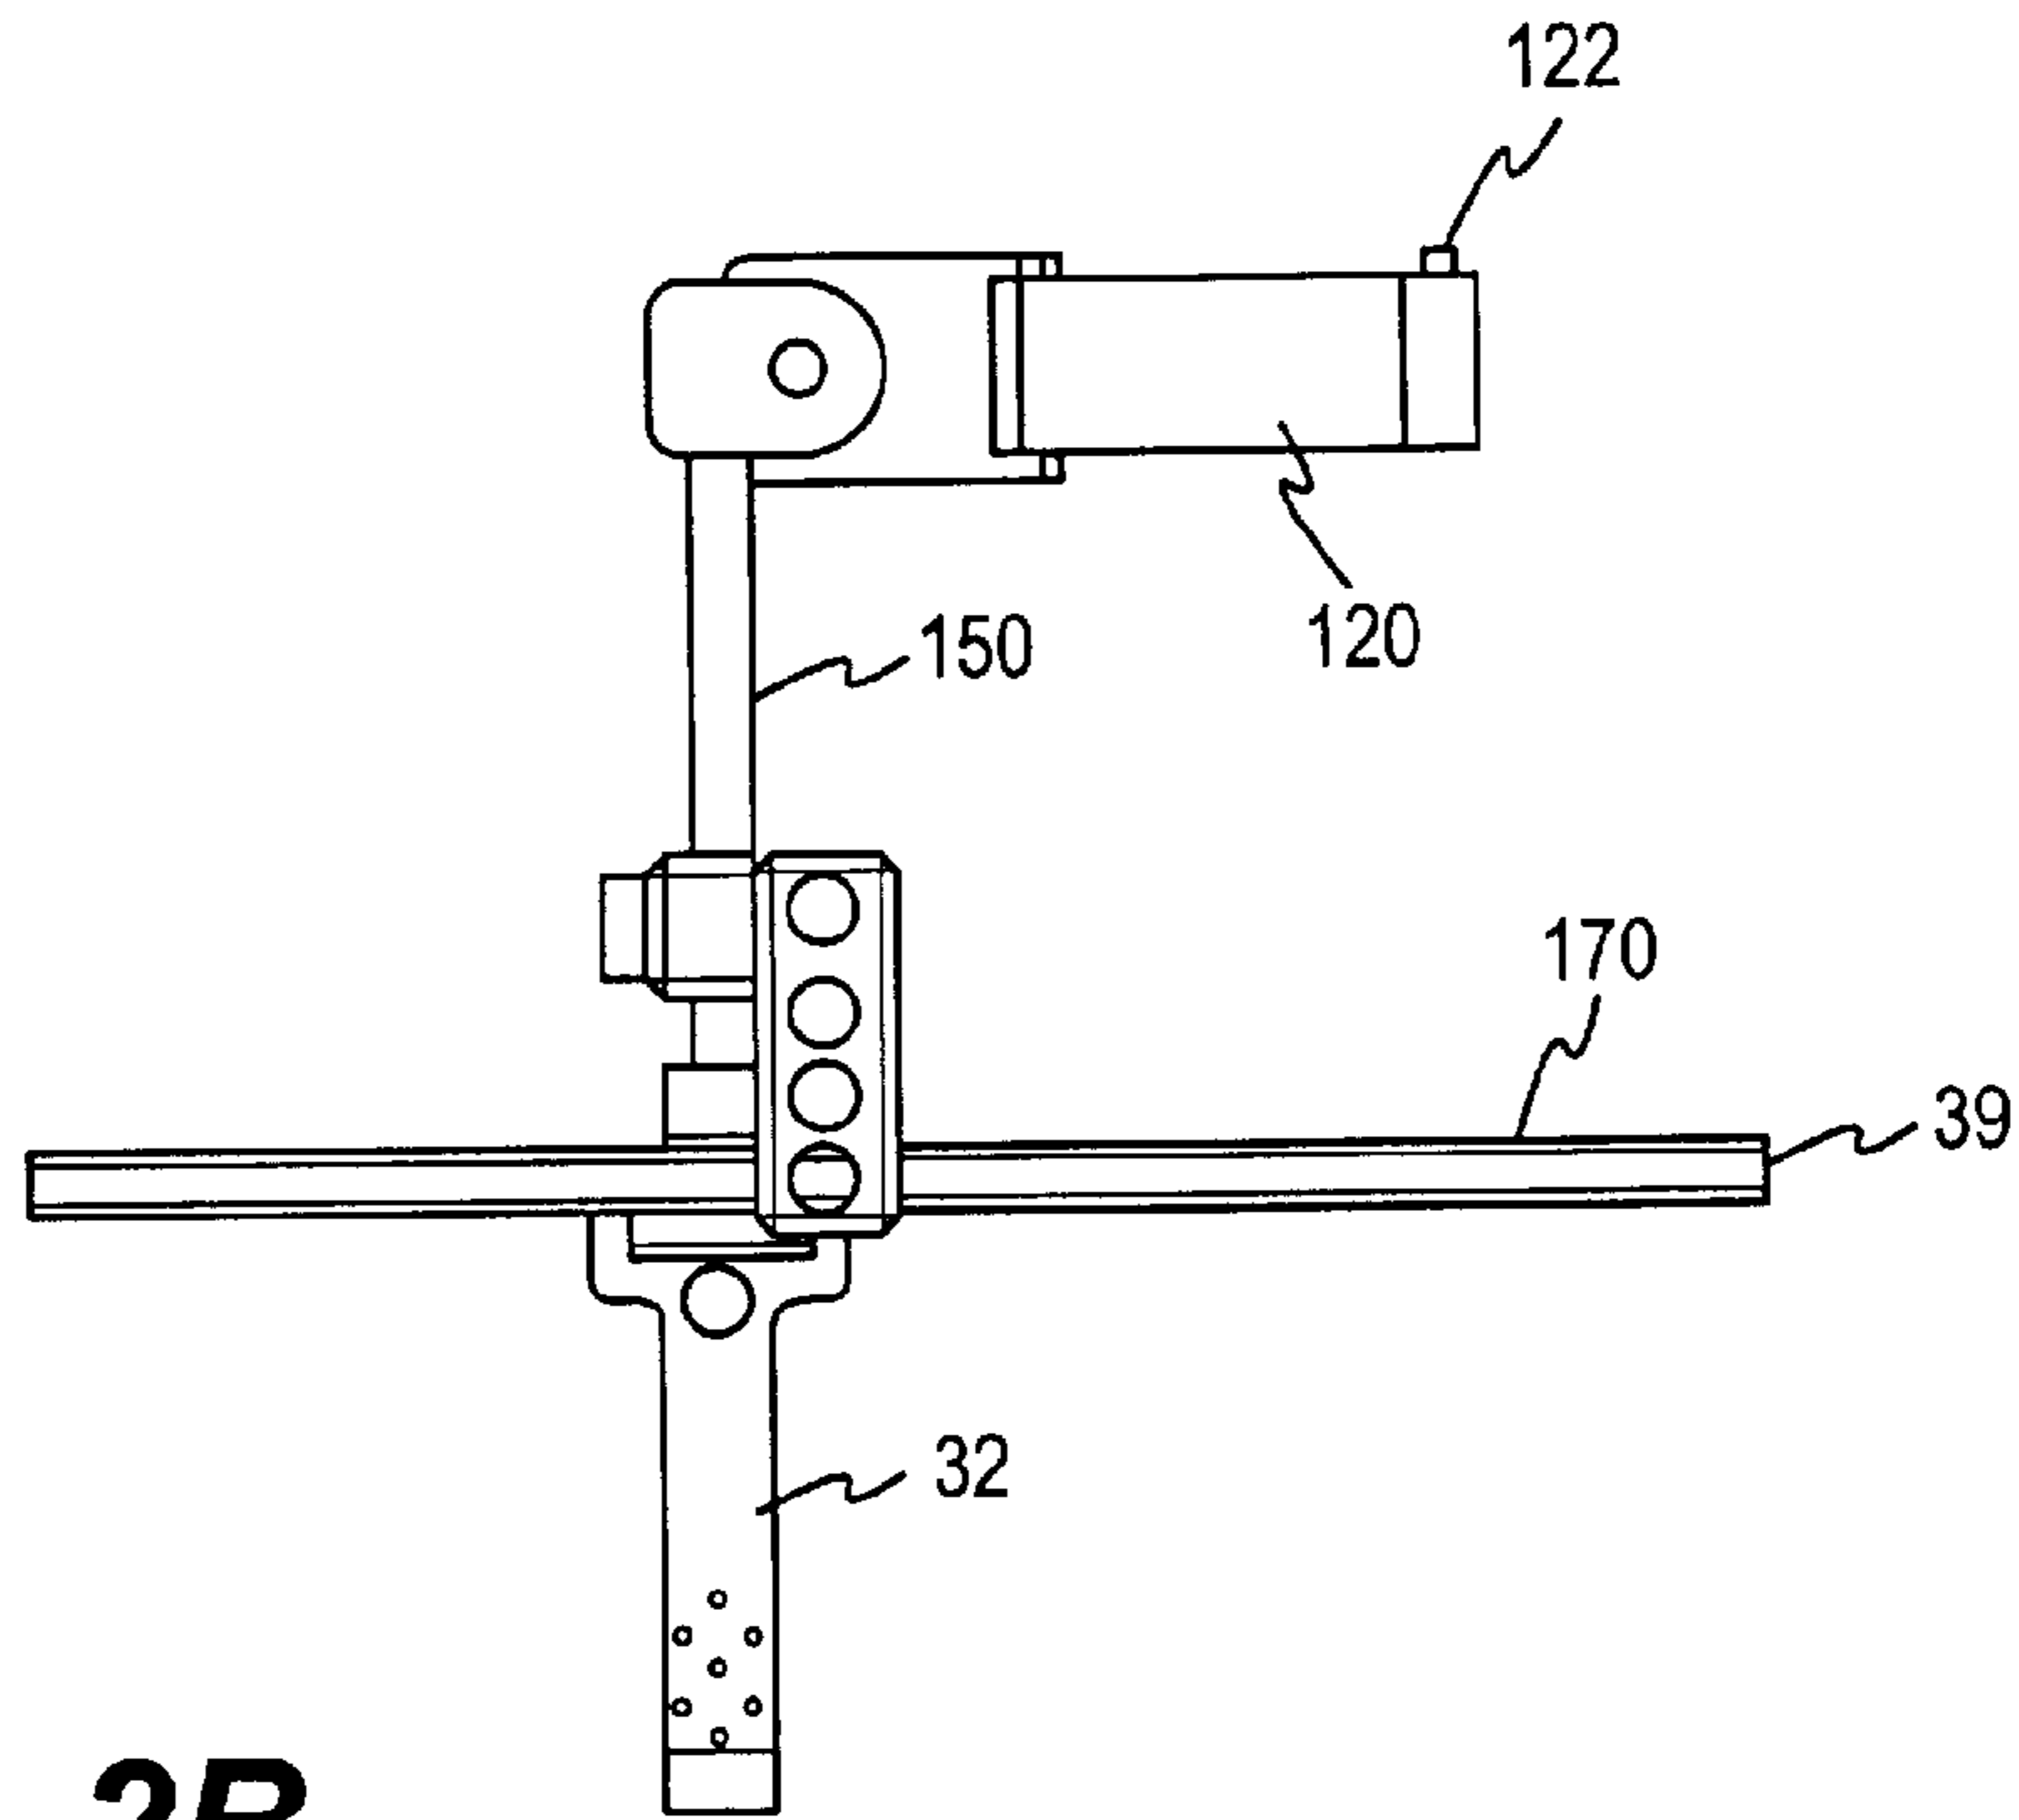


FIG. 2B

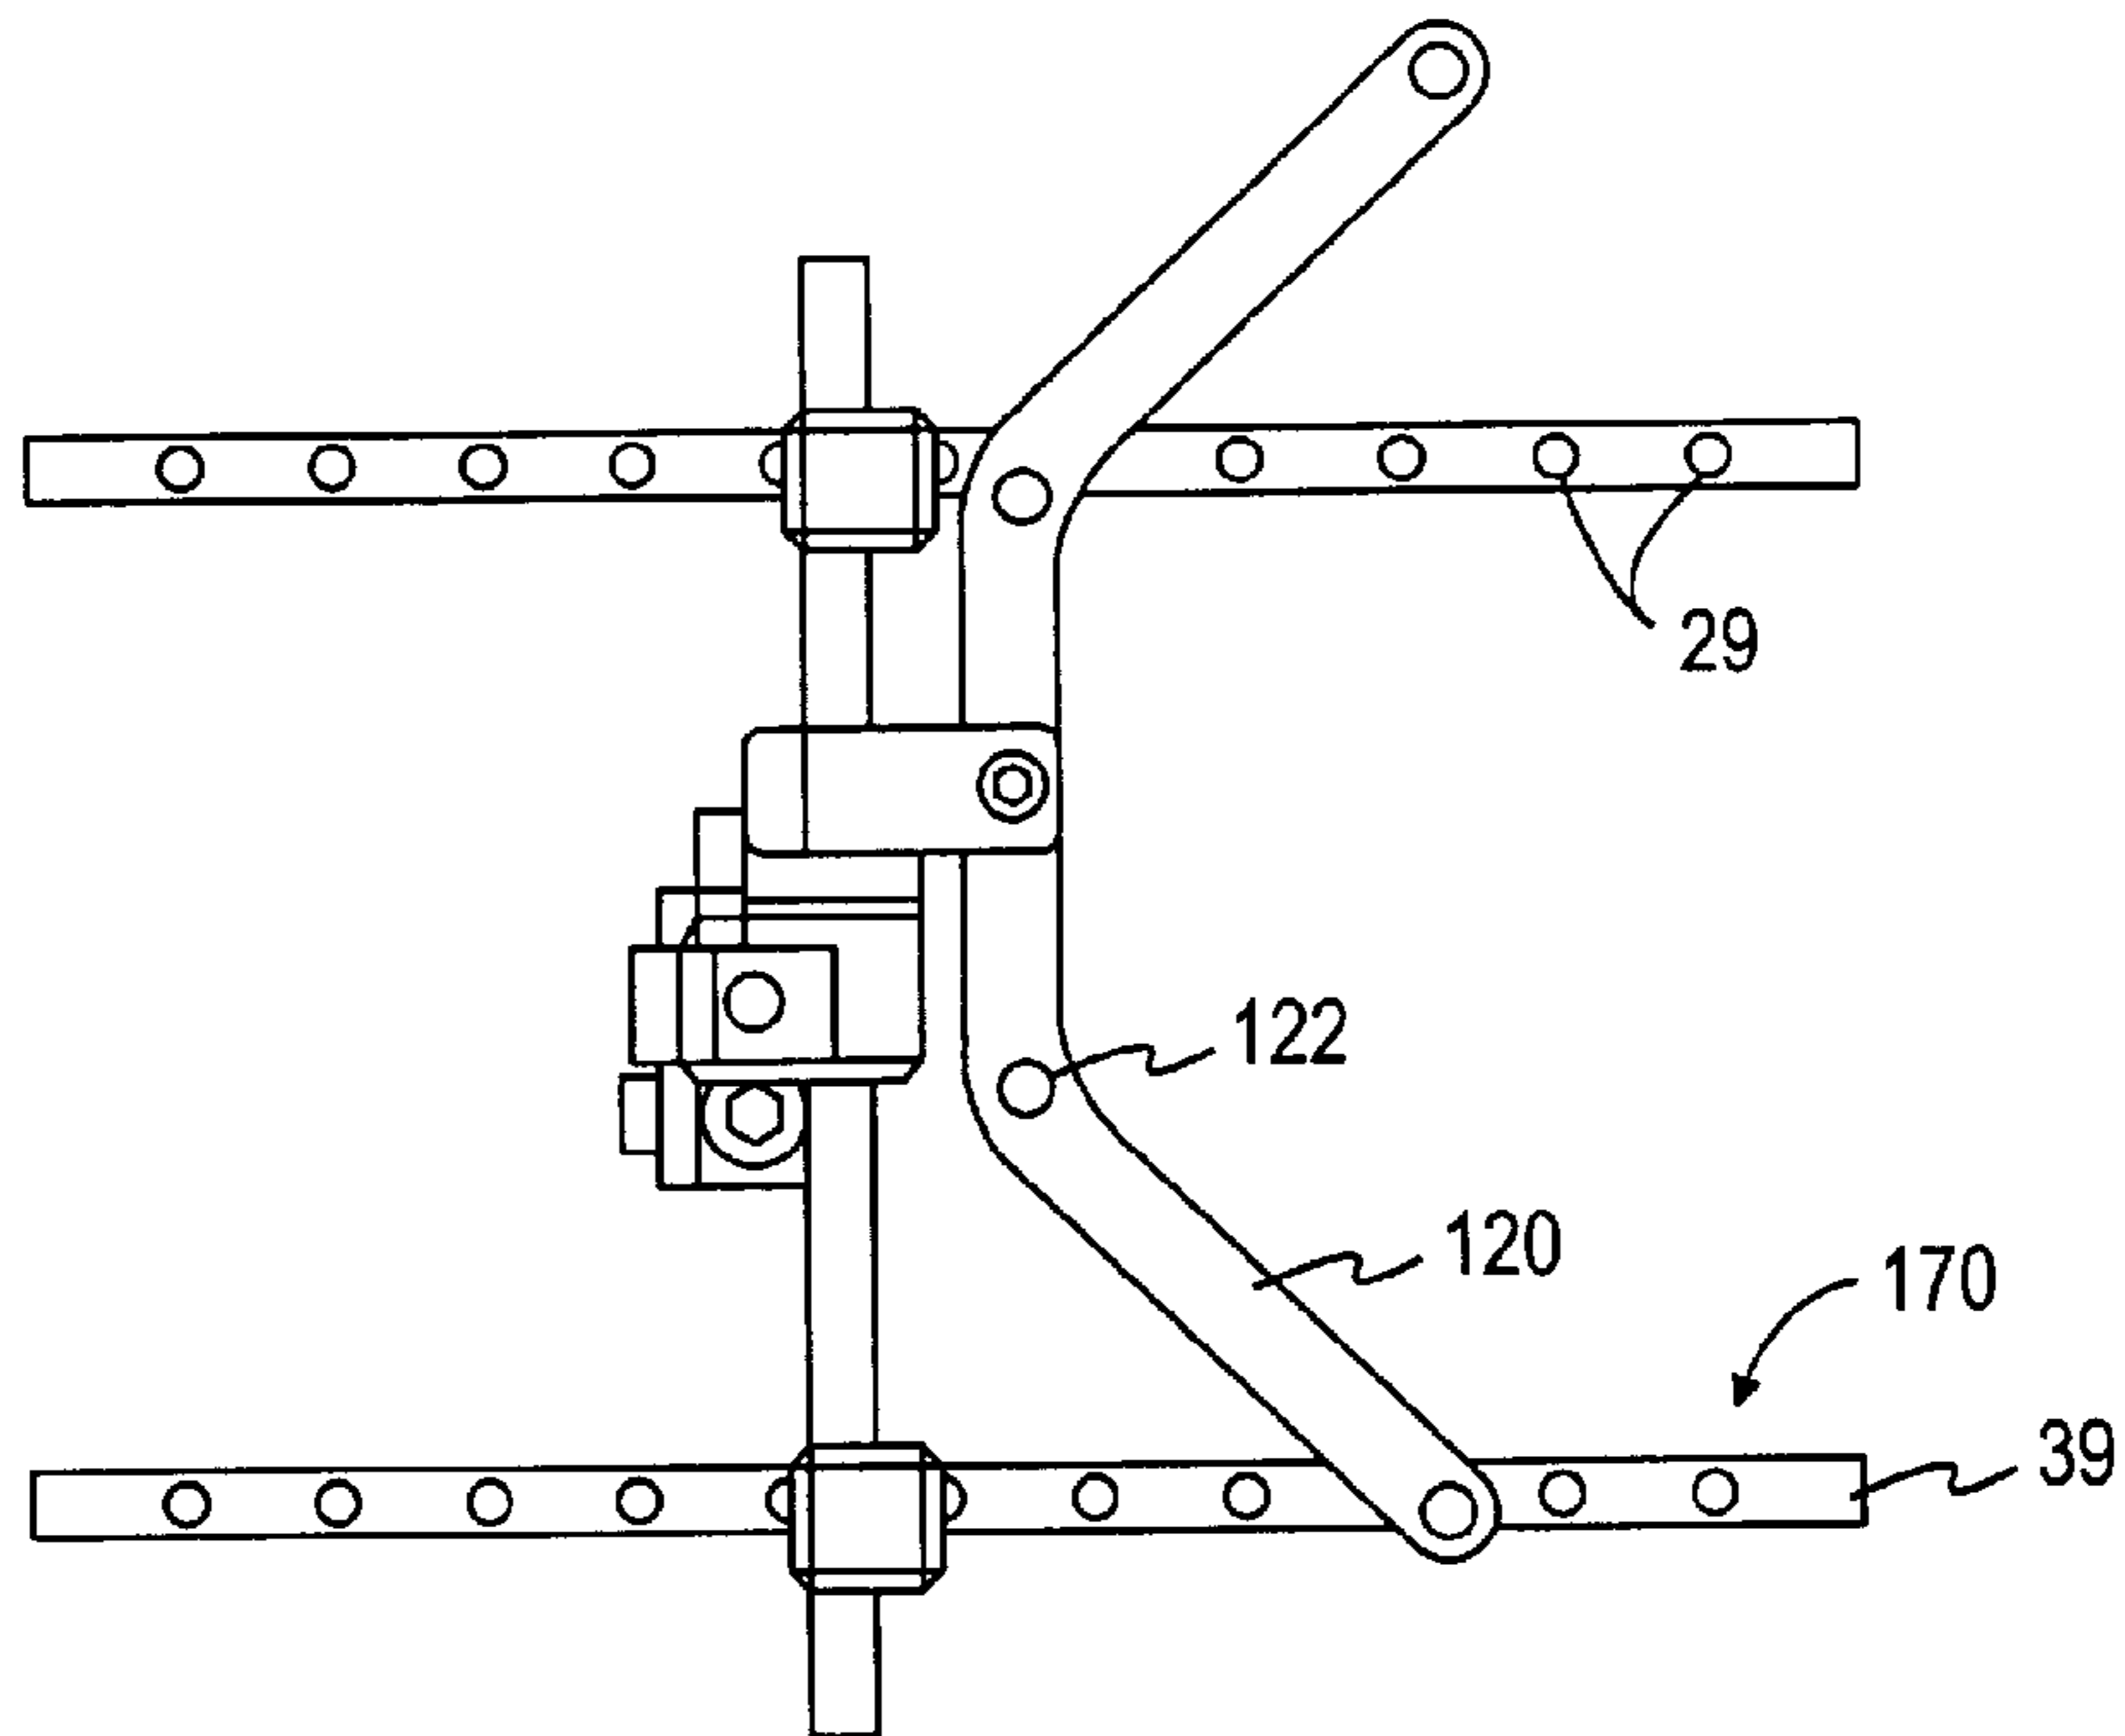


FIG. 2C

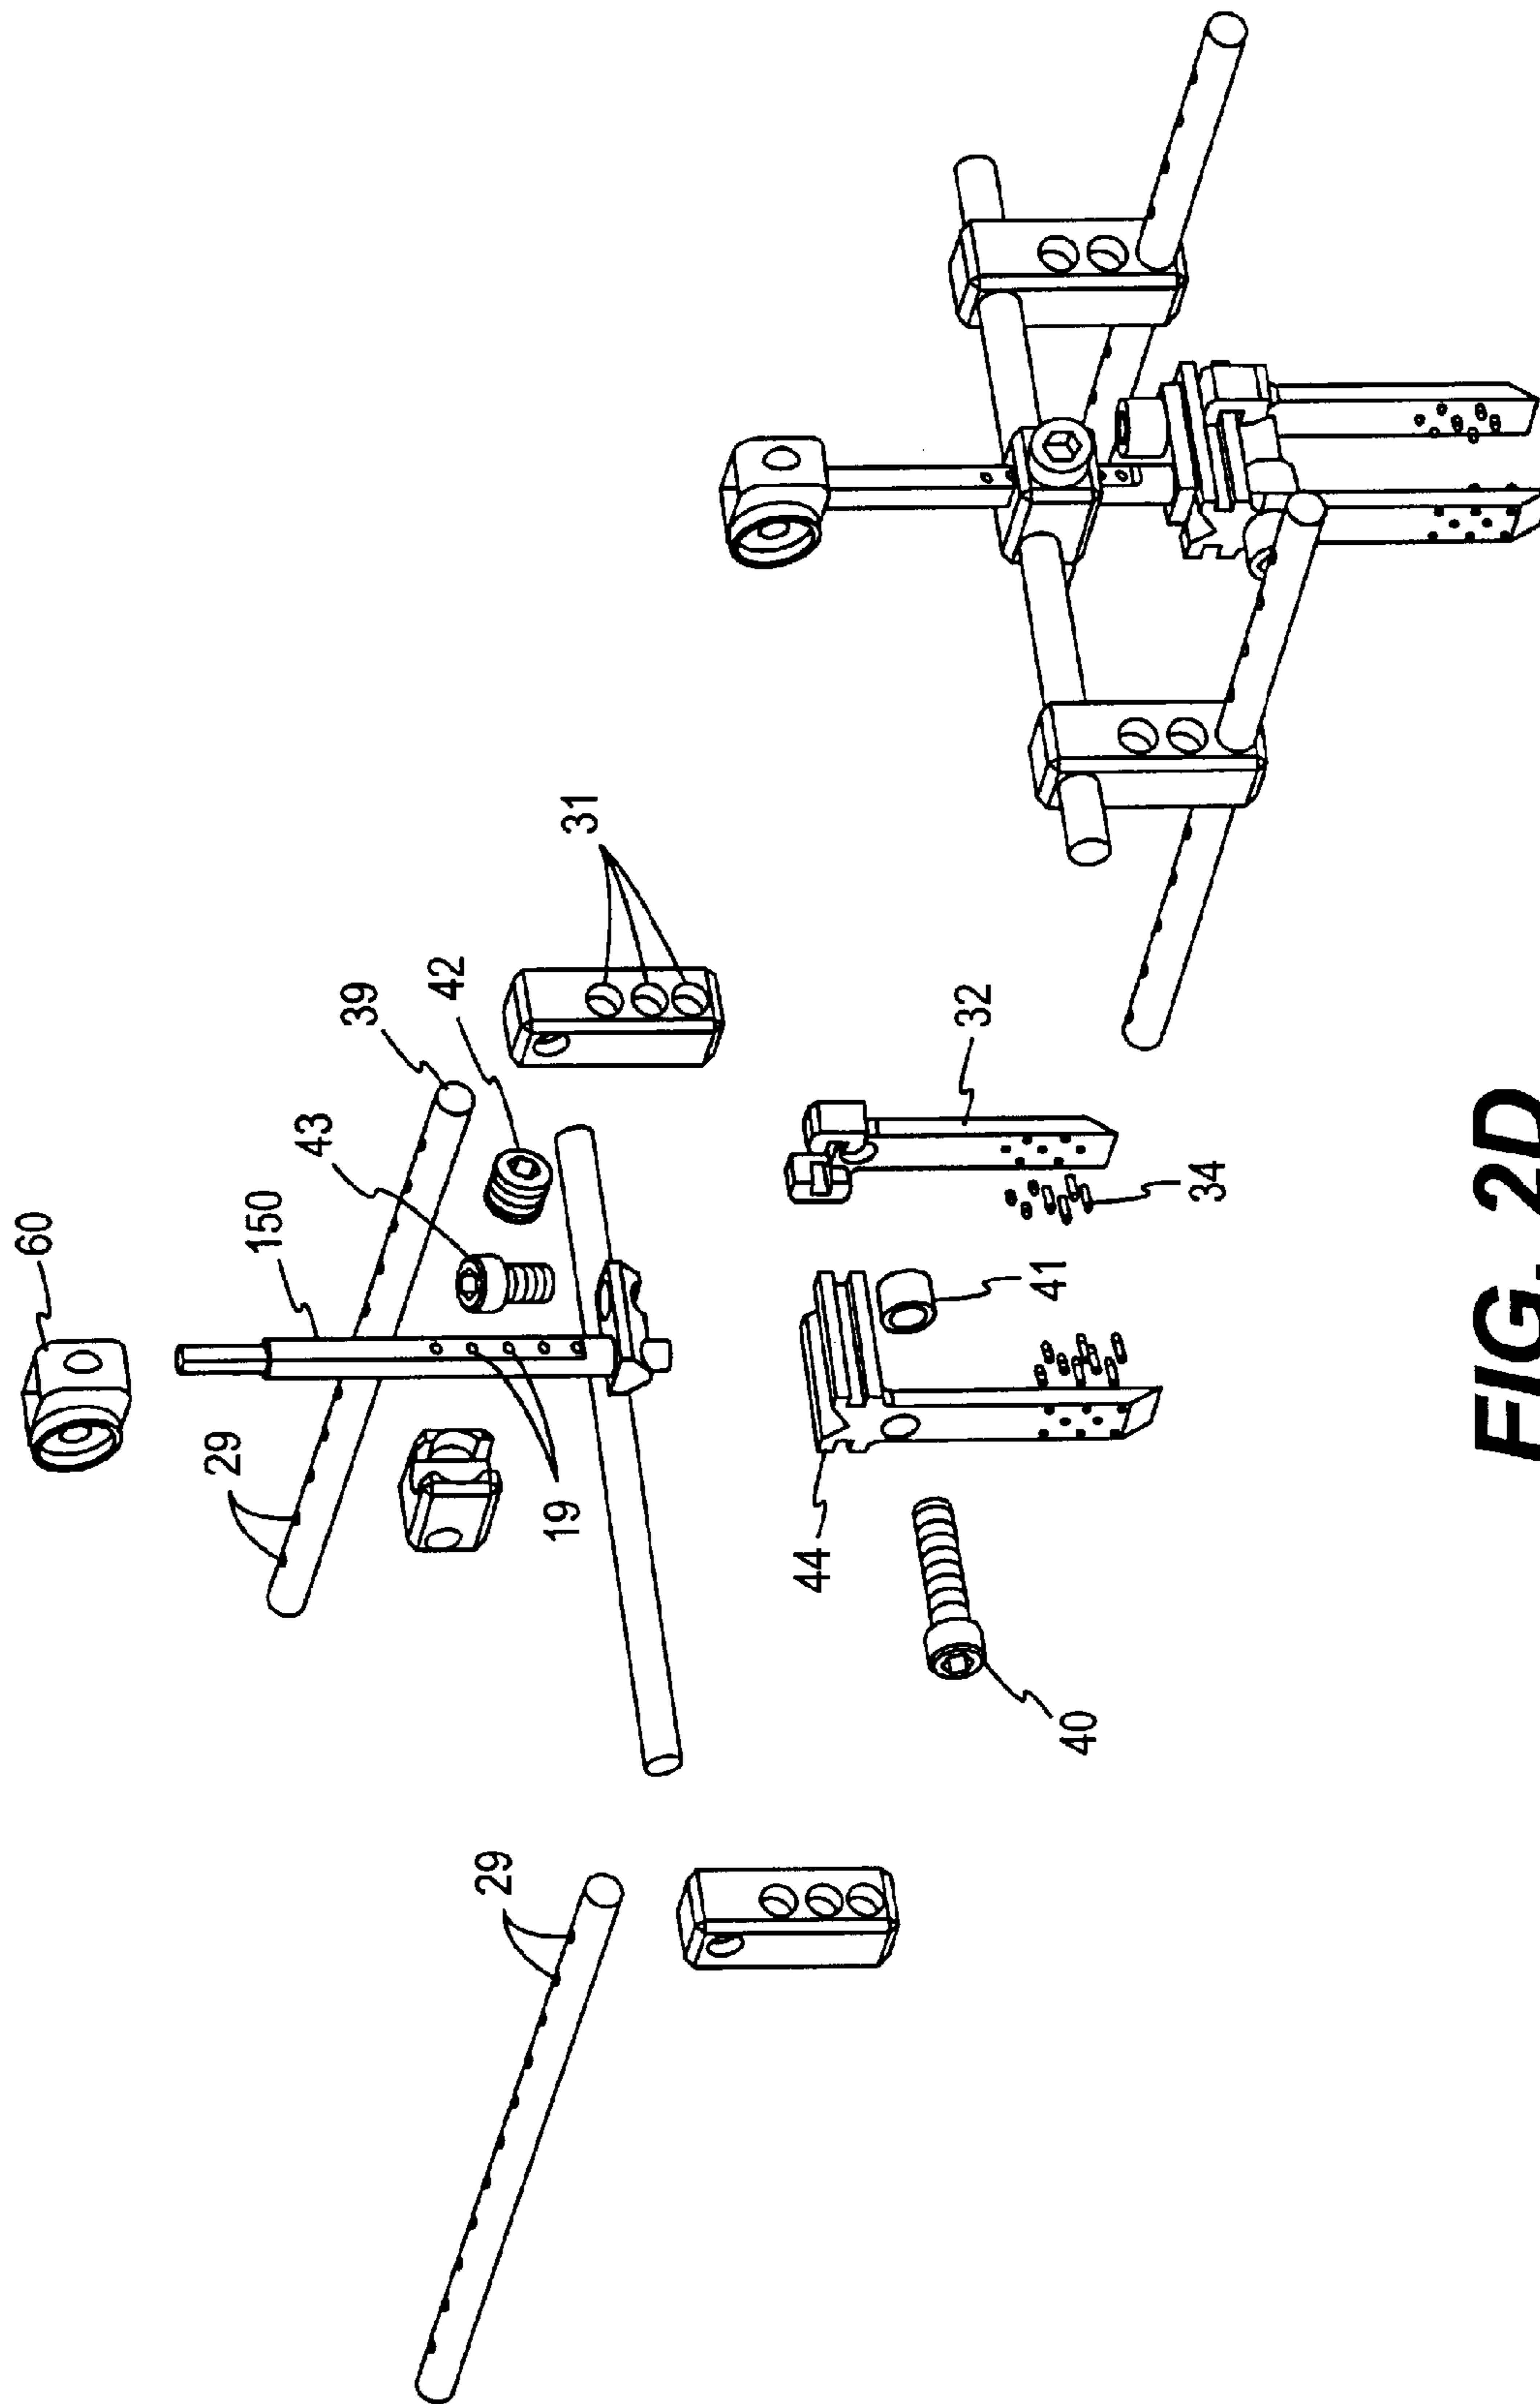


FIG. 2D

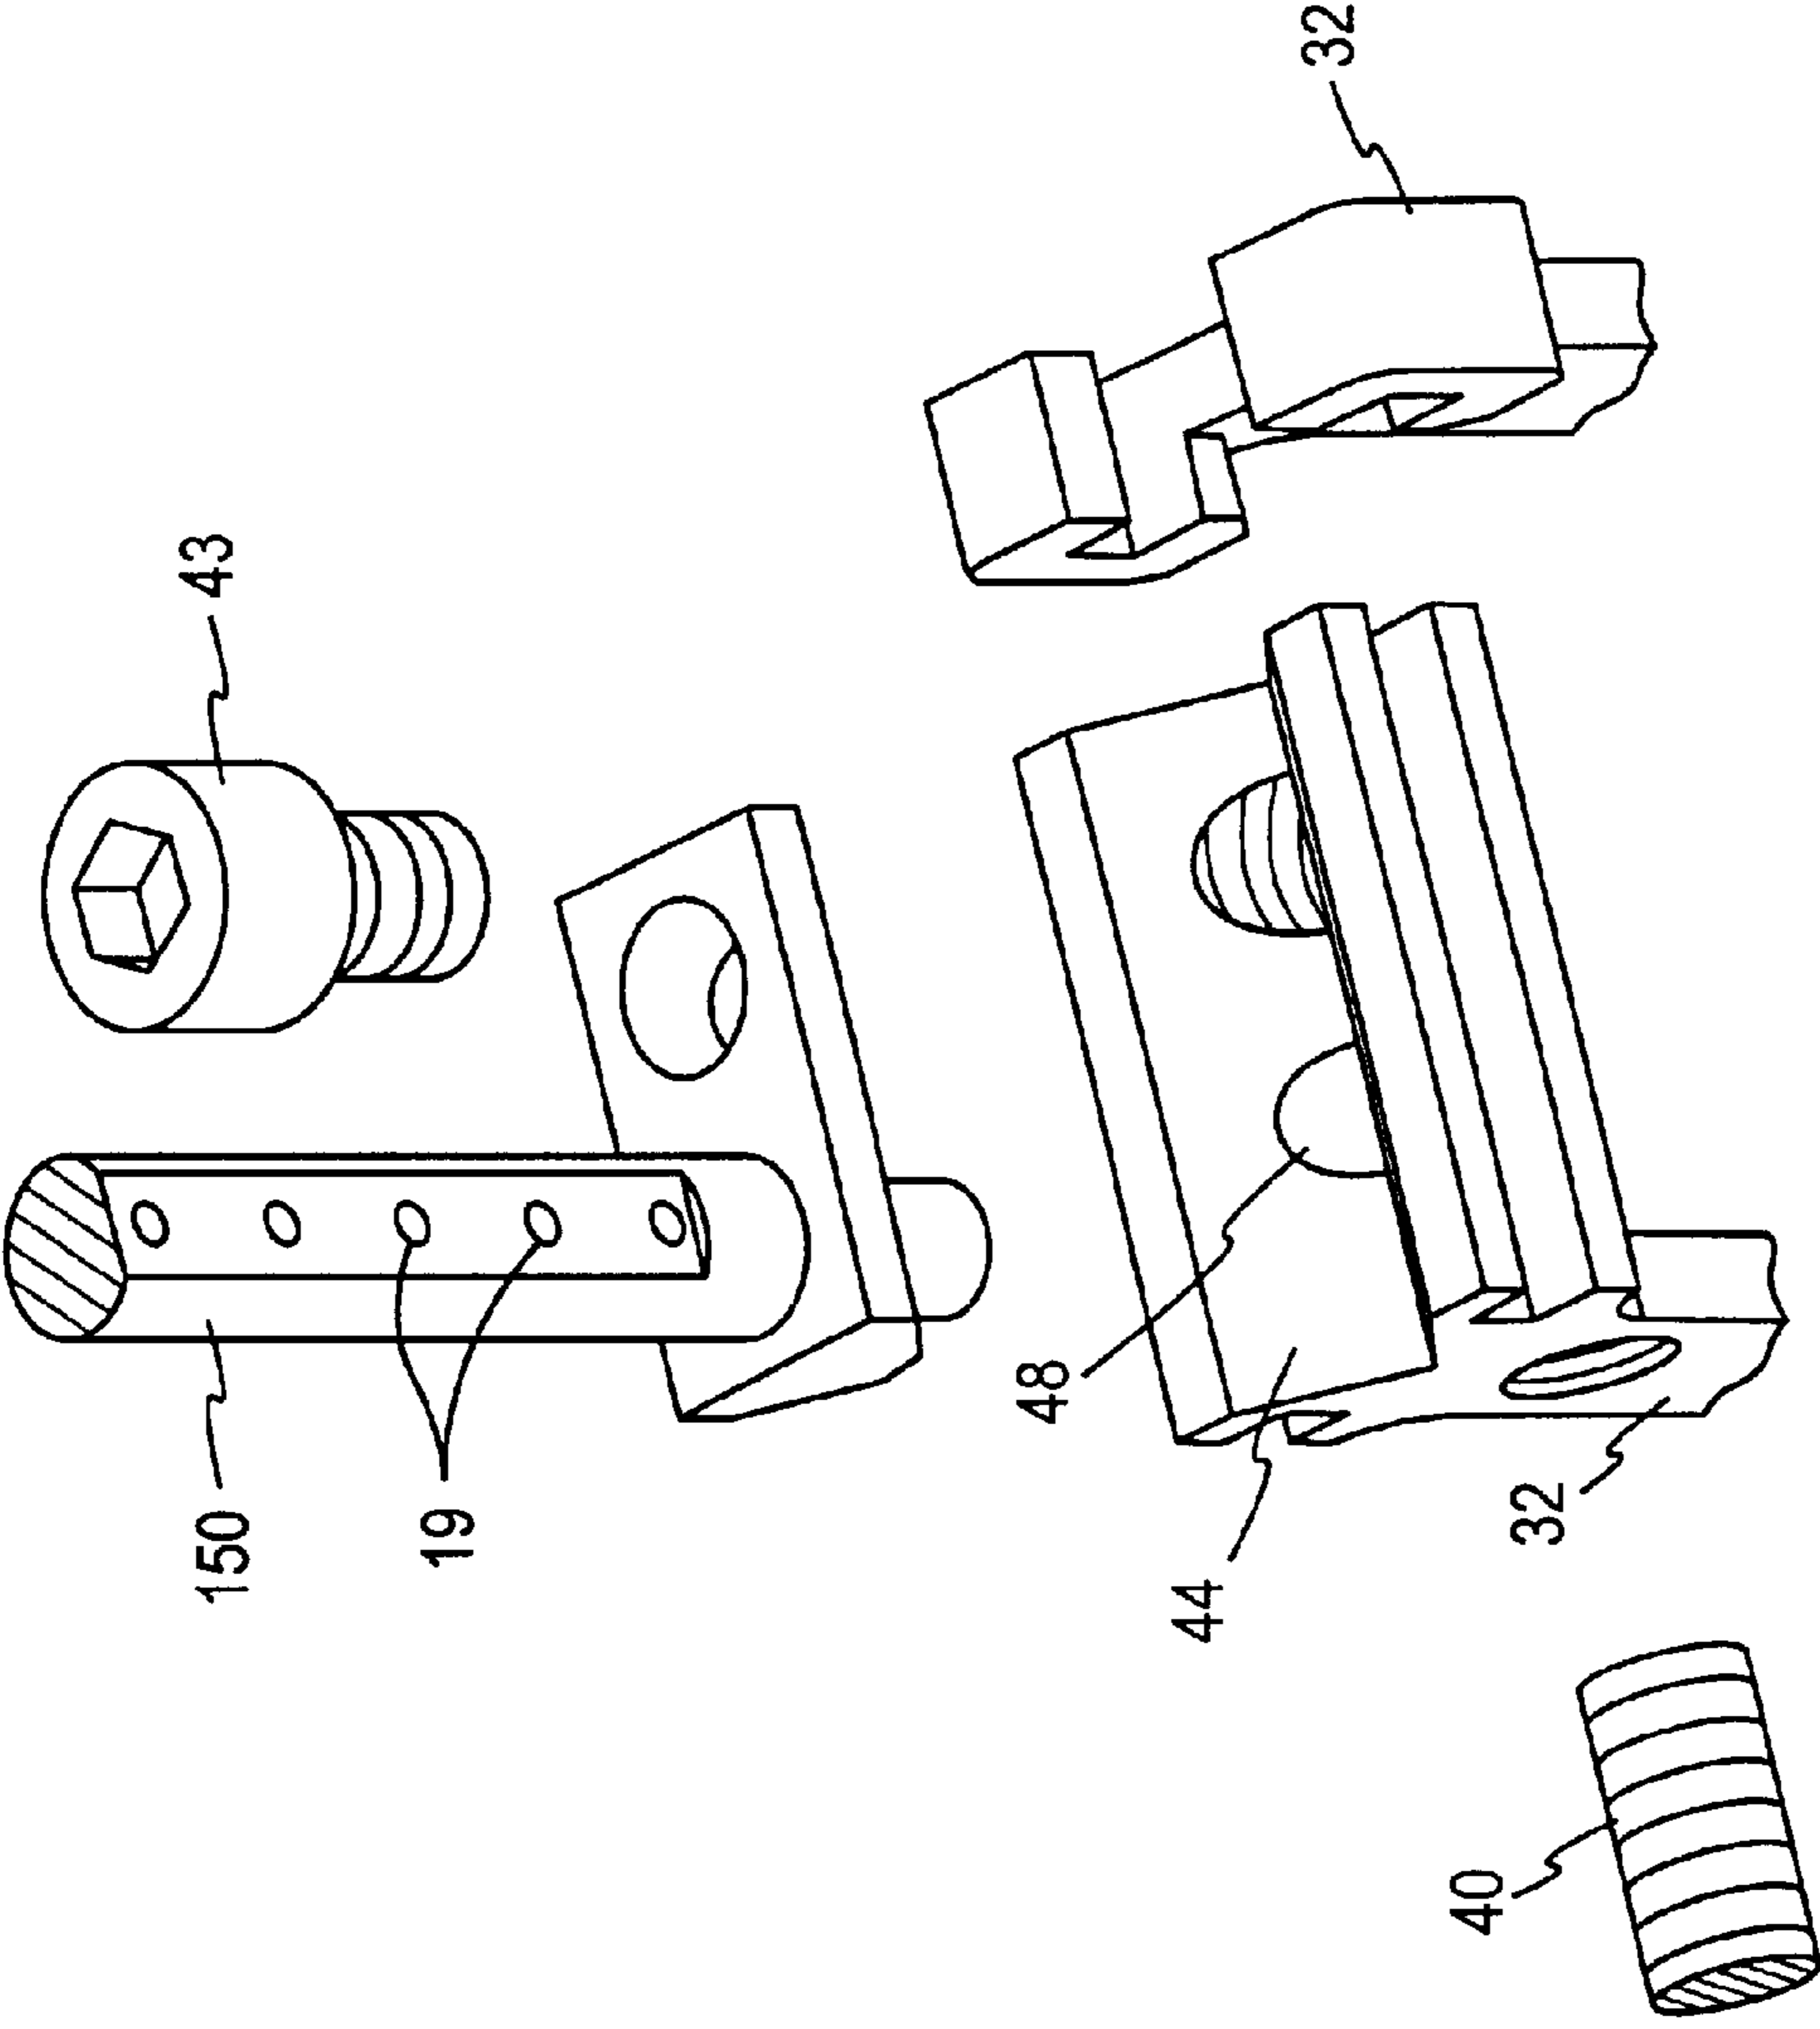


FIG. 2E

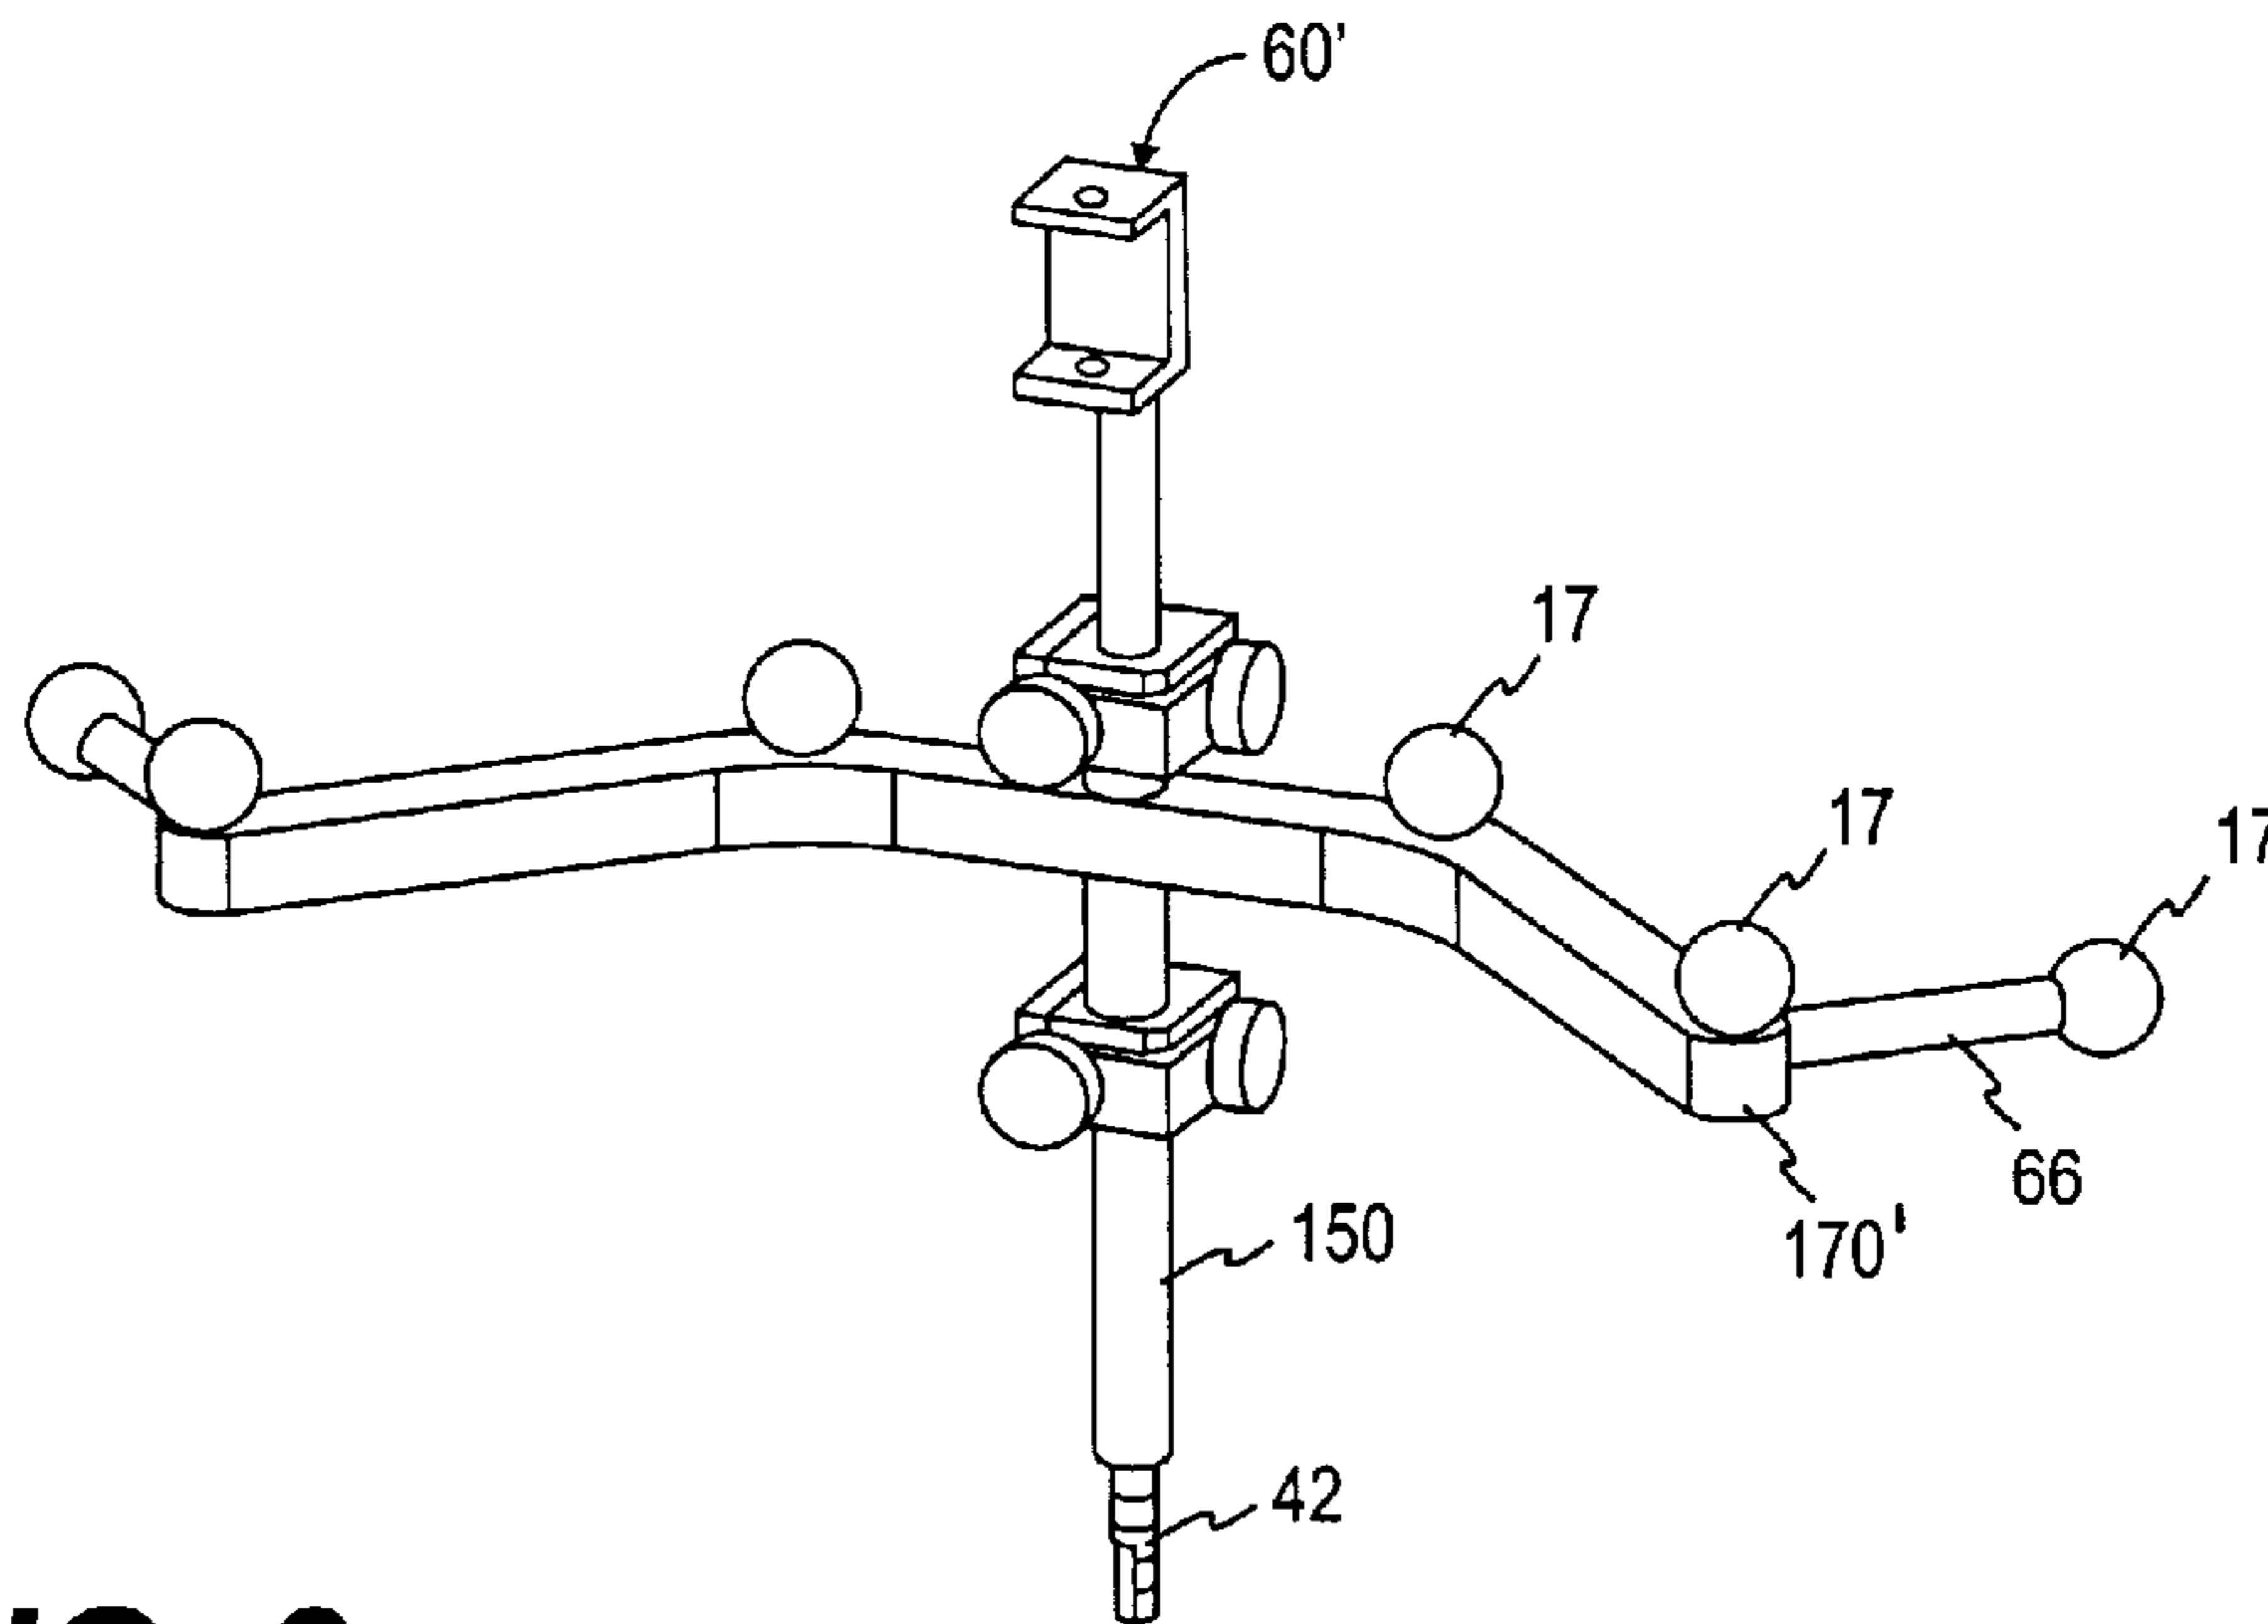


FIG. 3

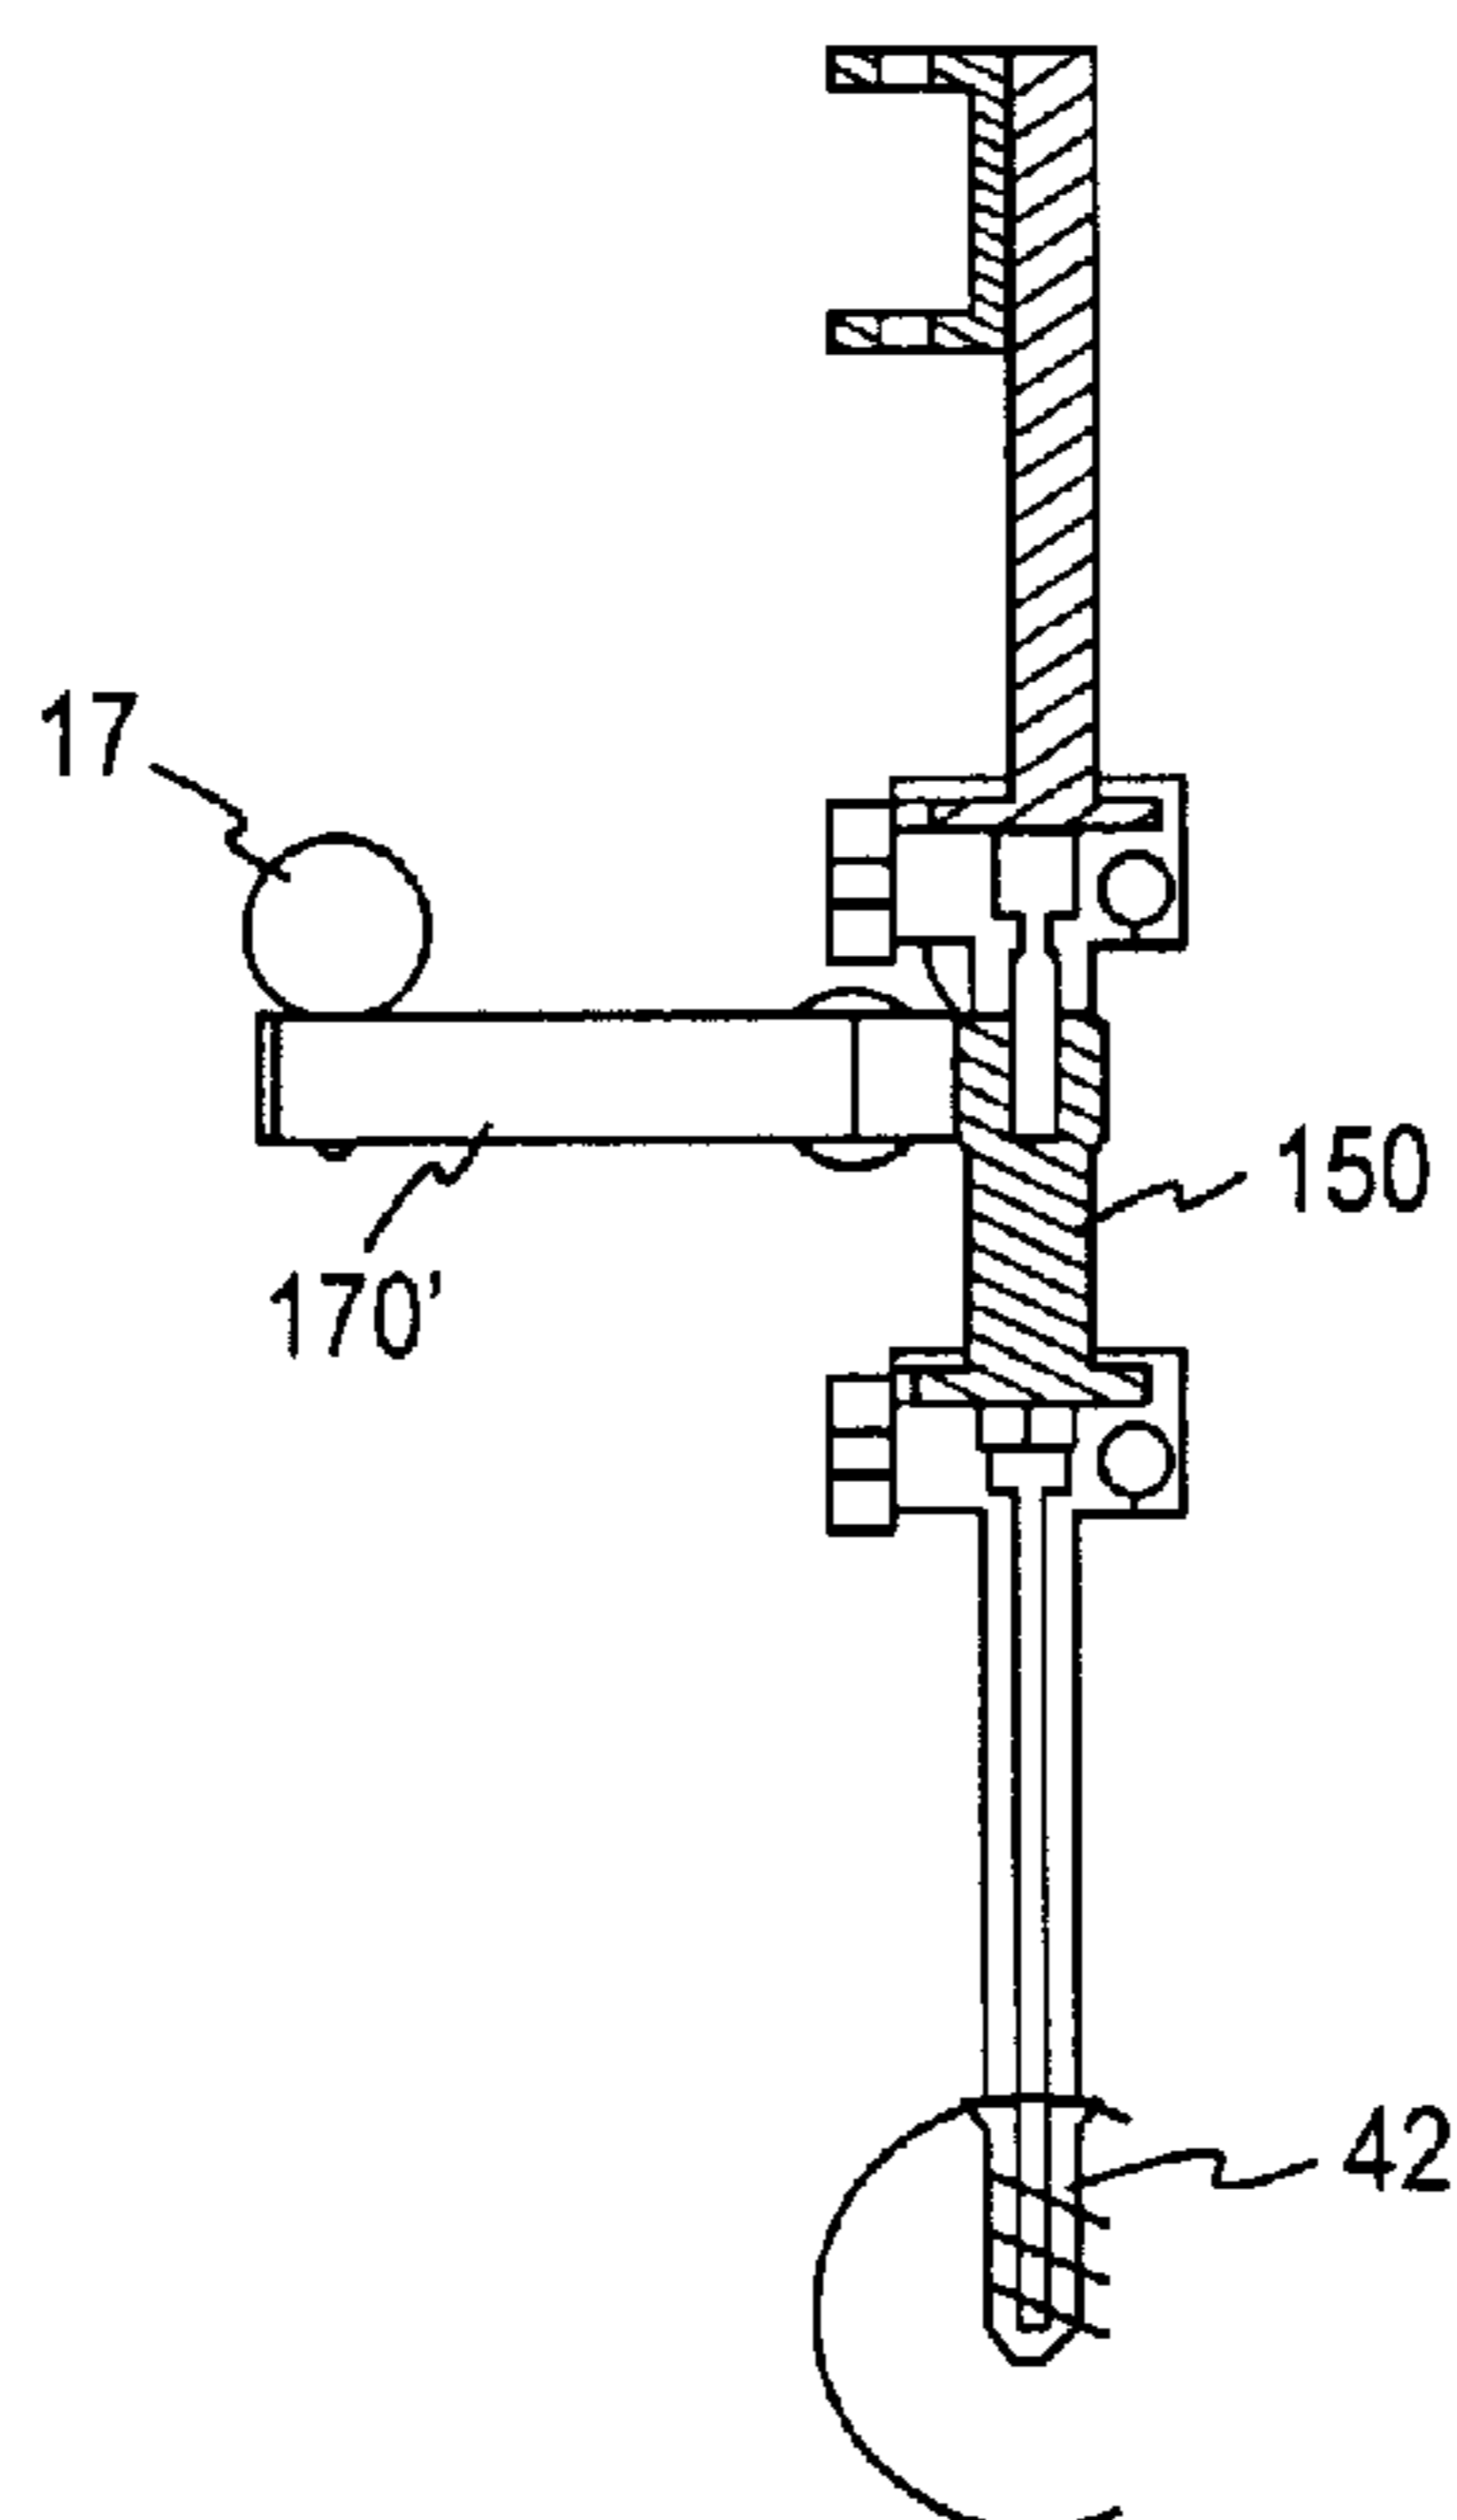


FIG. 3A

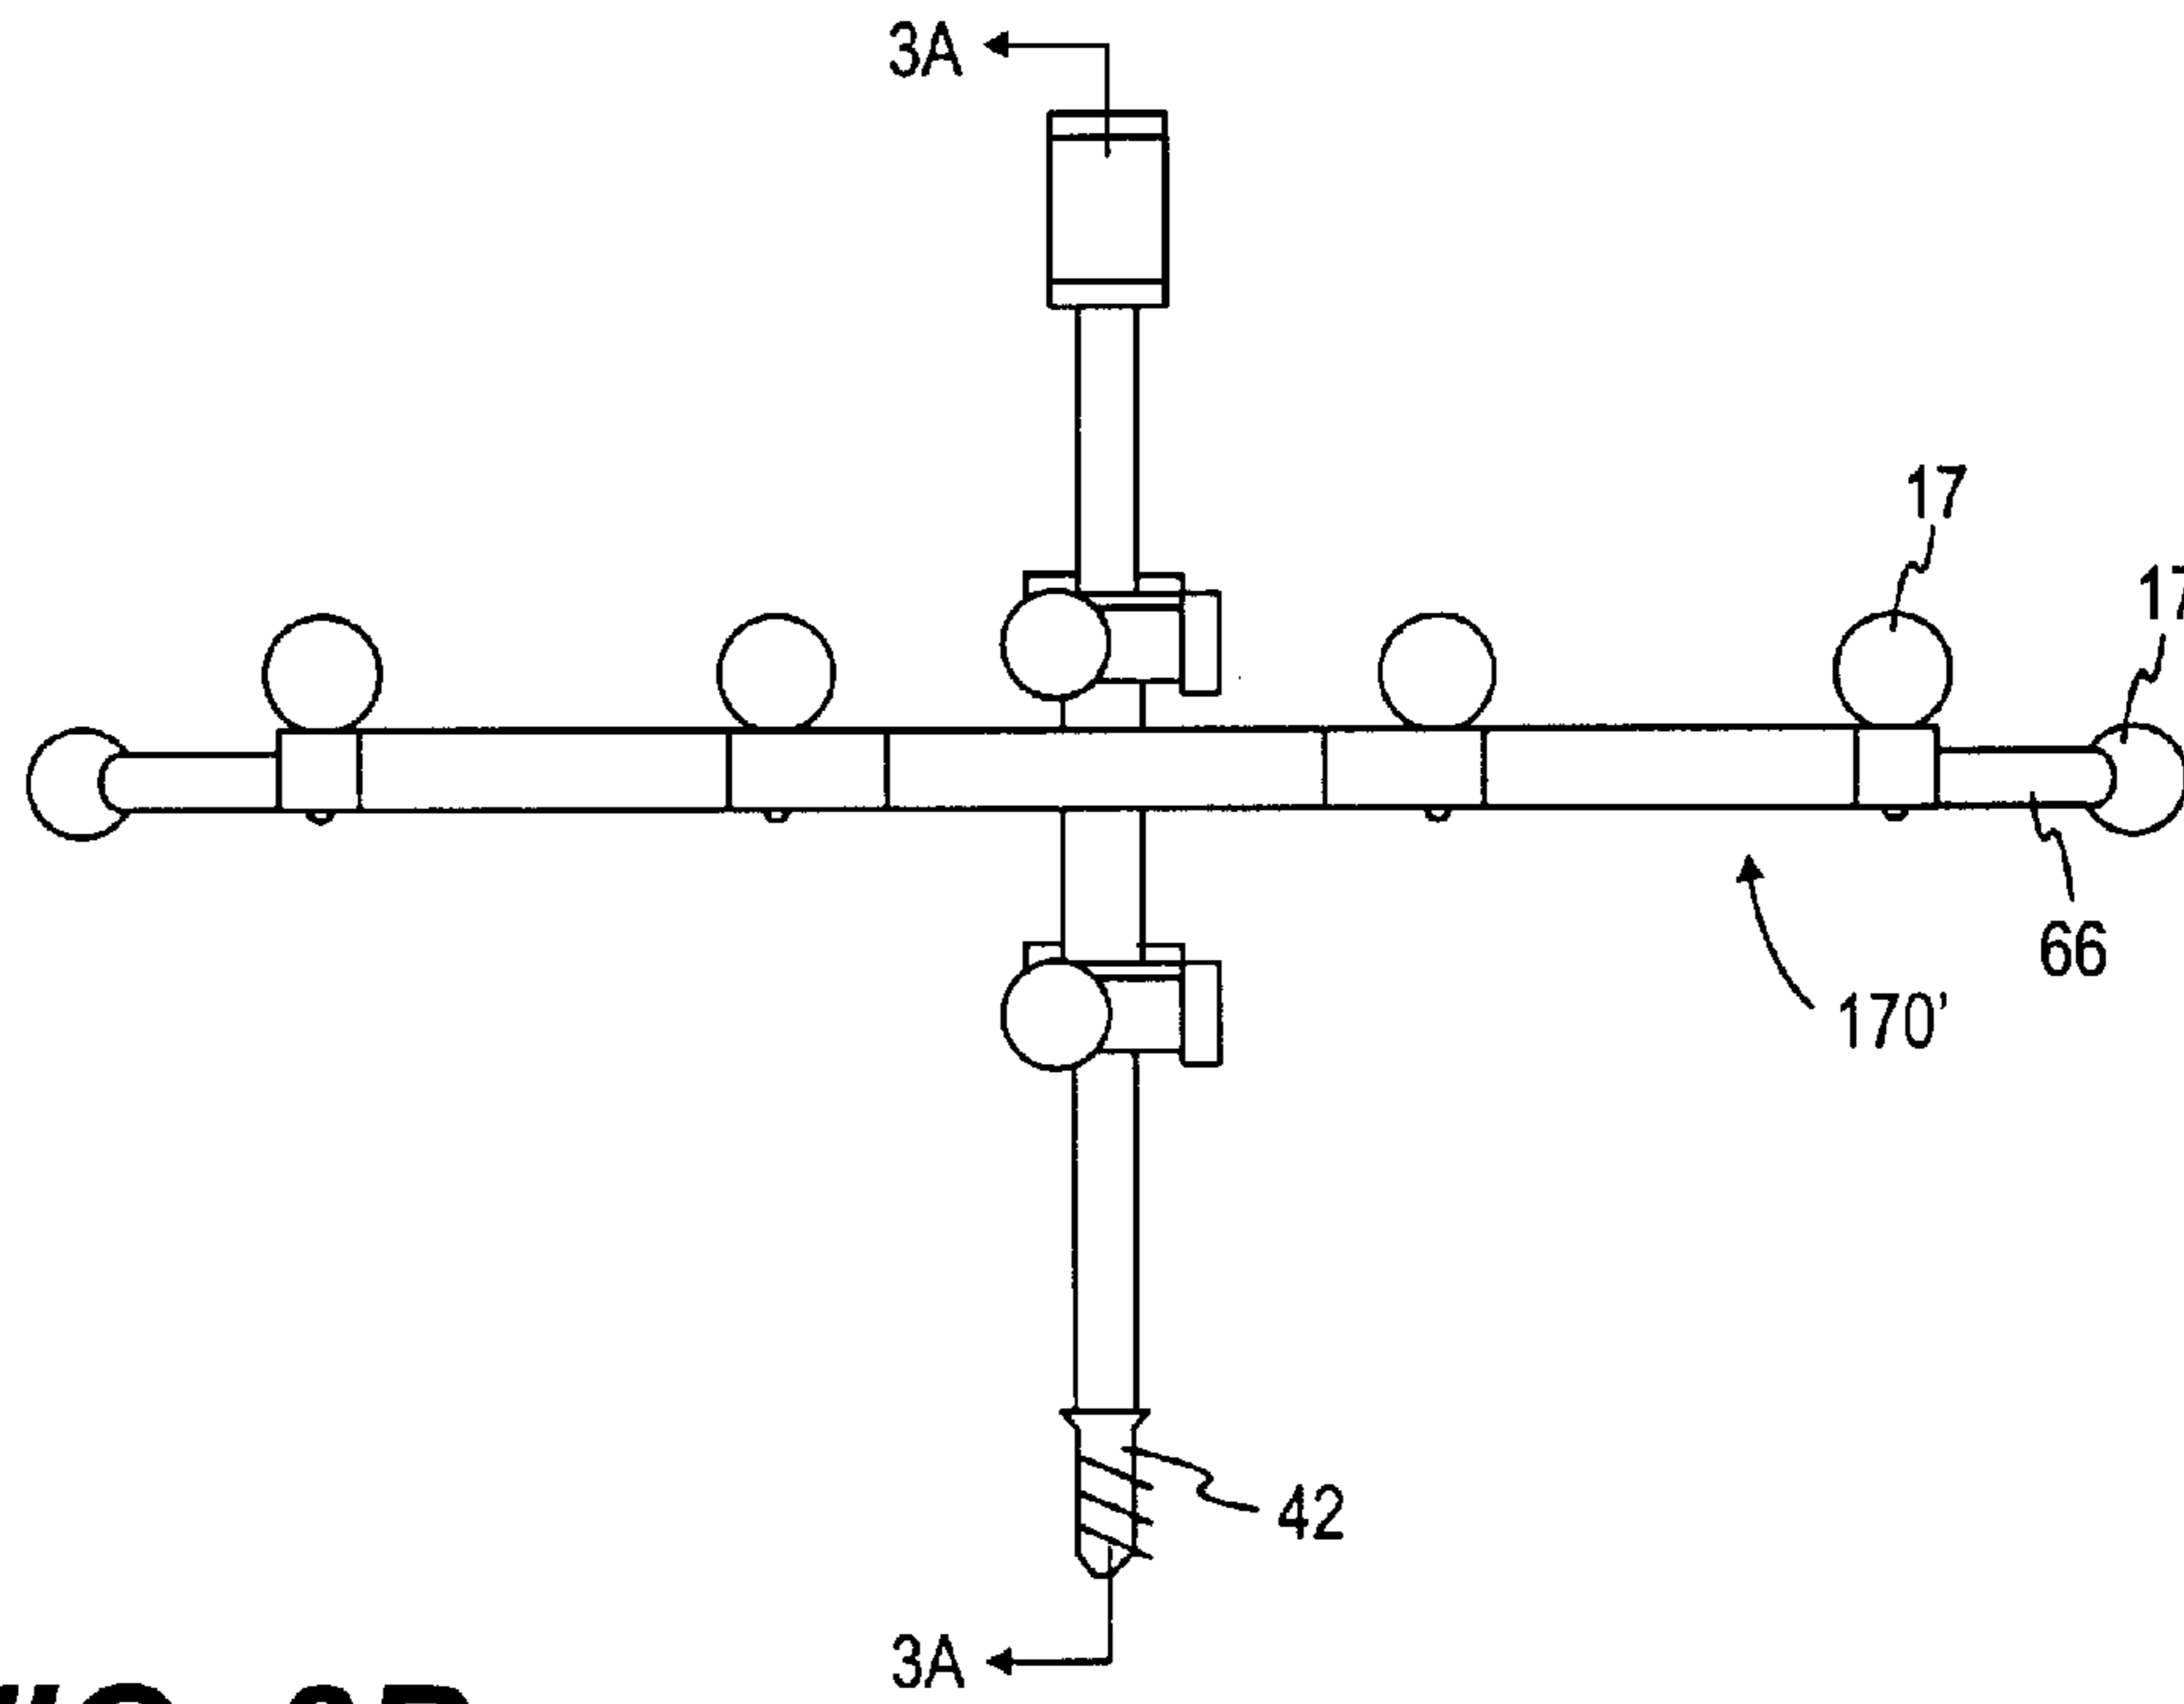


FIG. 3B

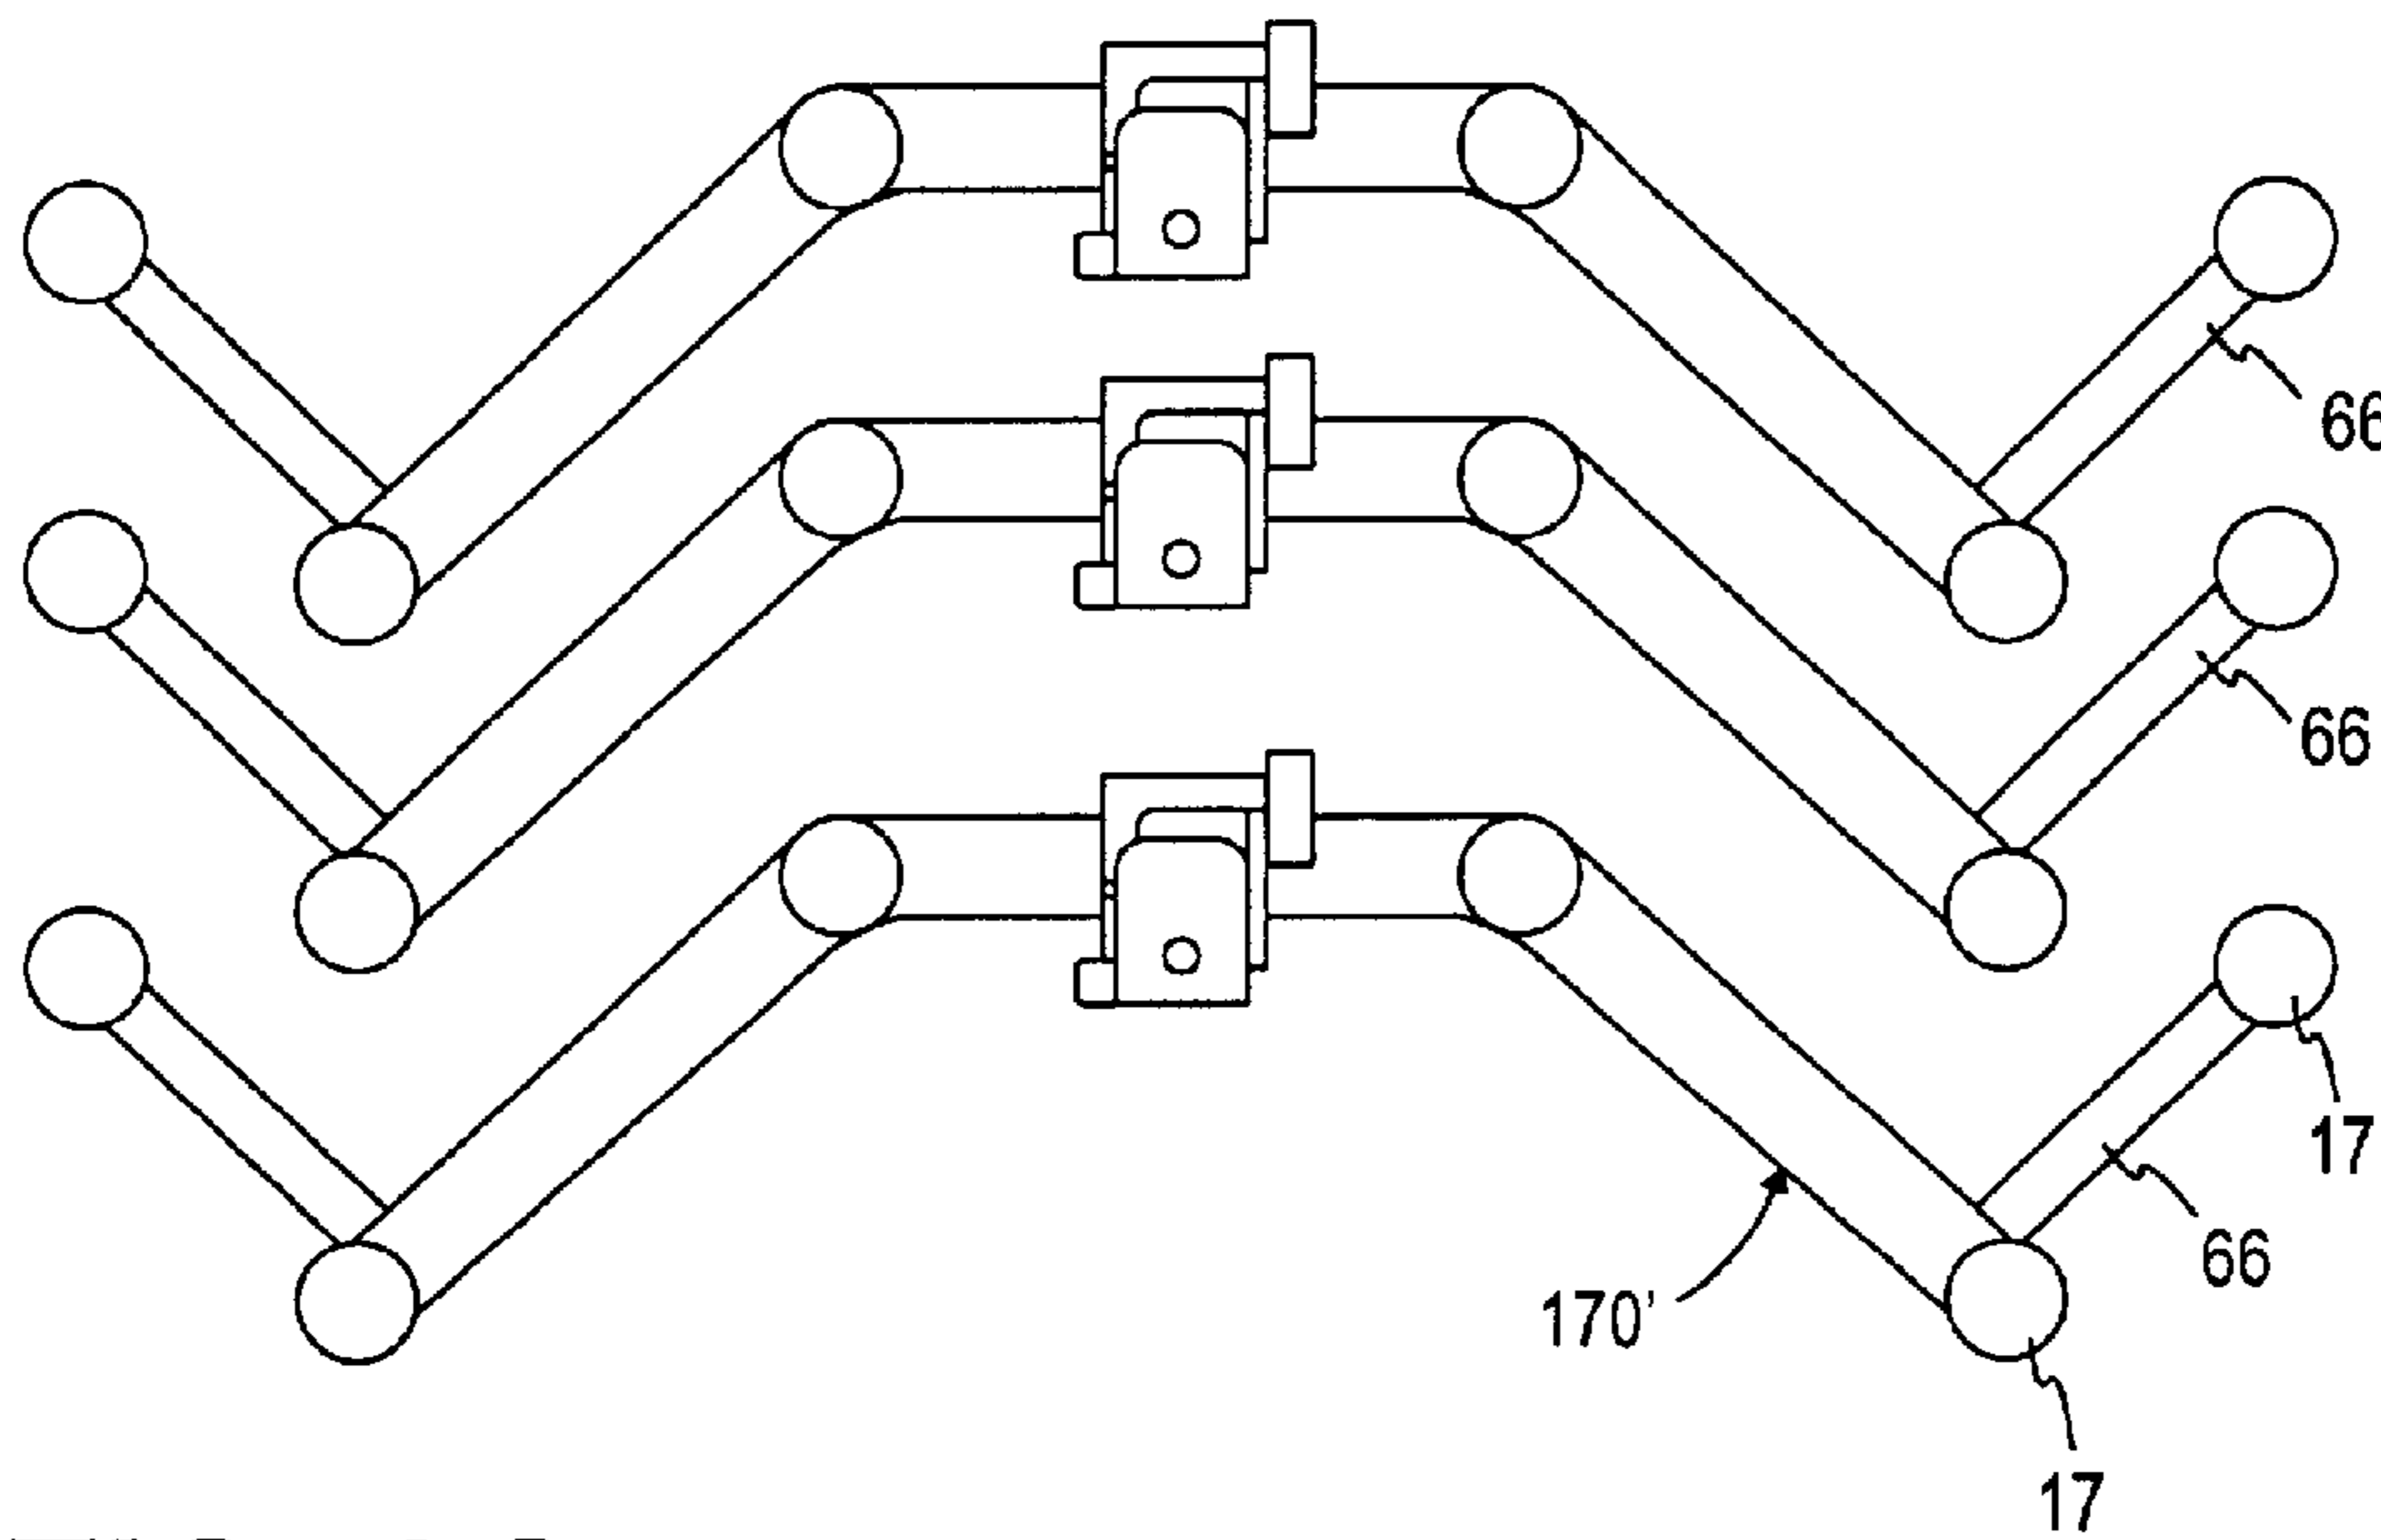


FIG. 3C

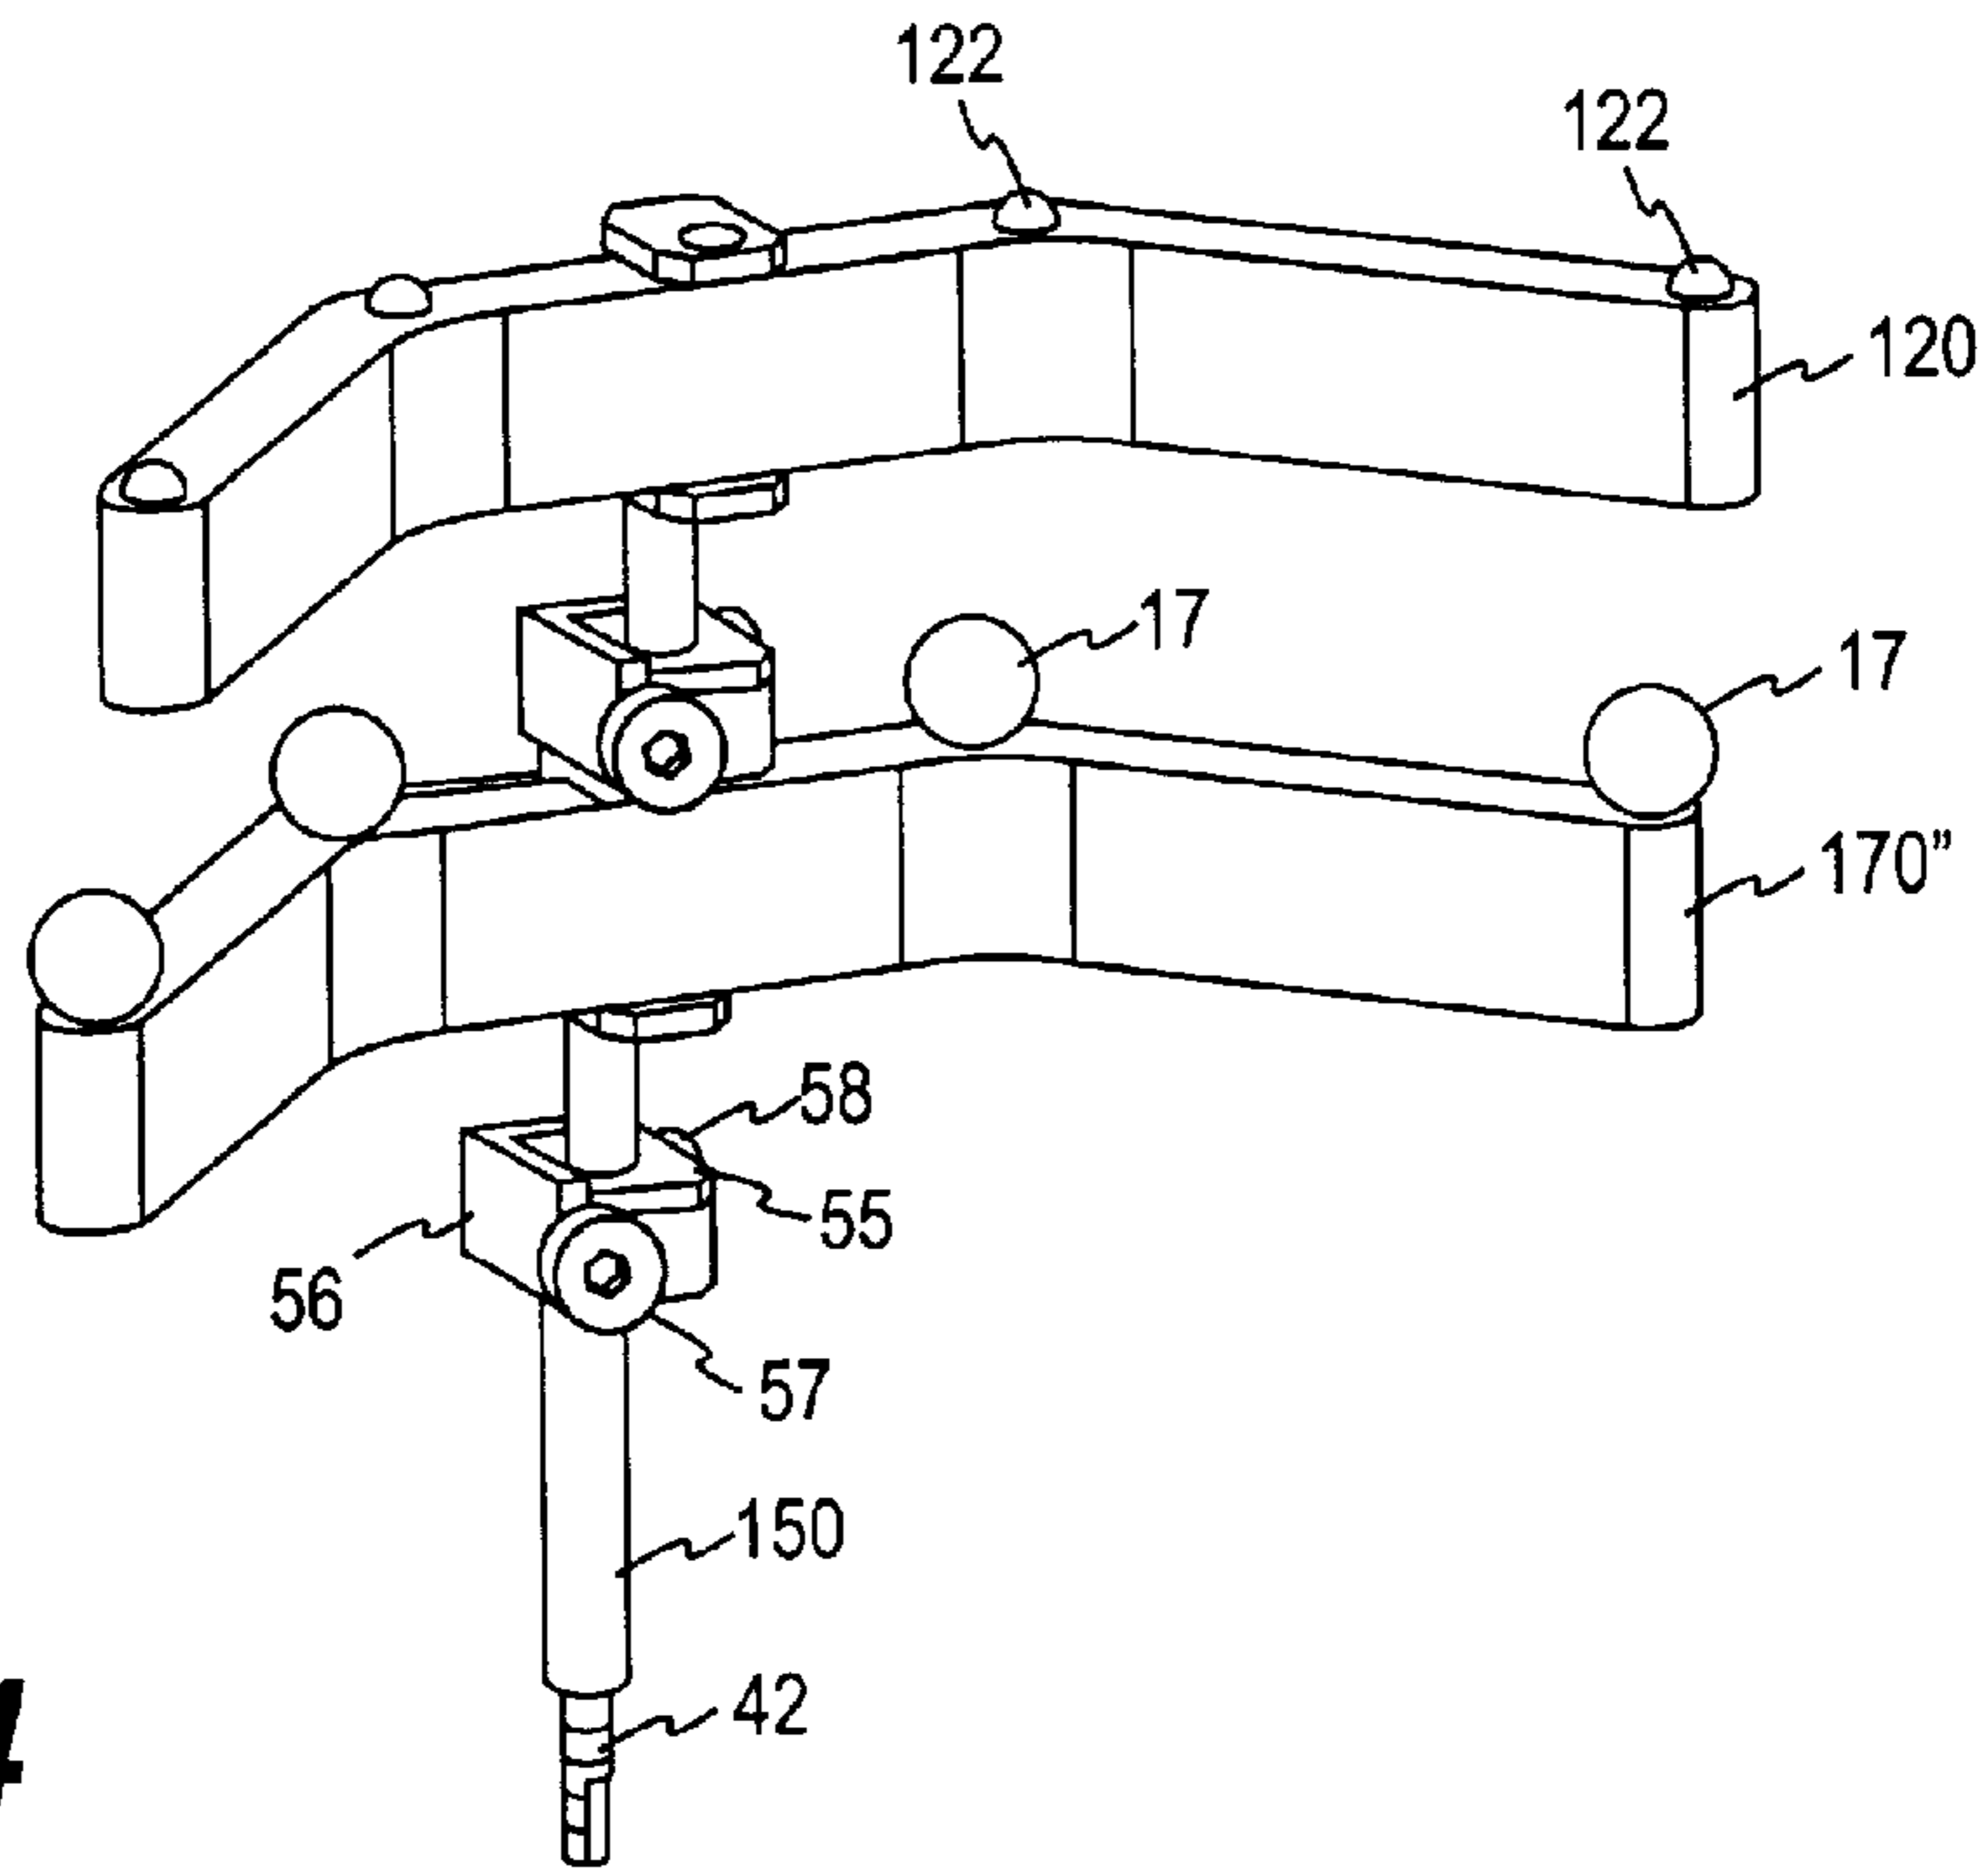


FIG. 4

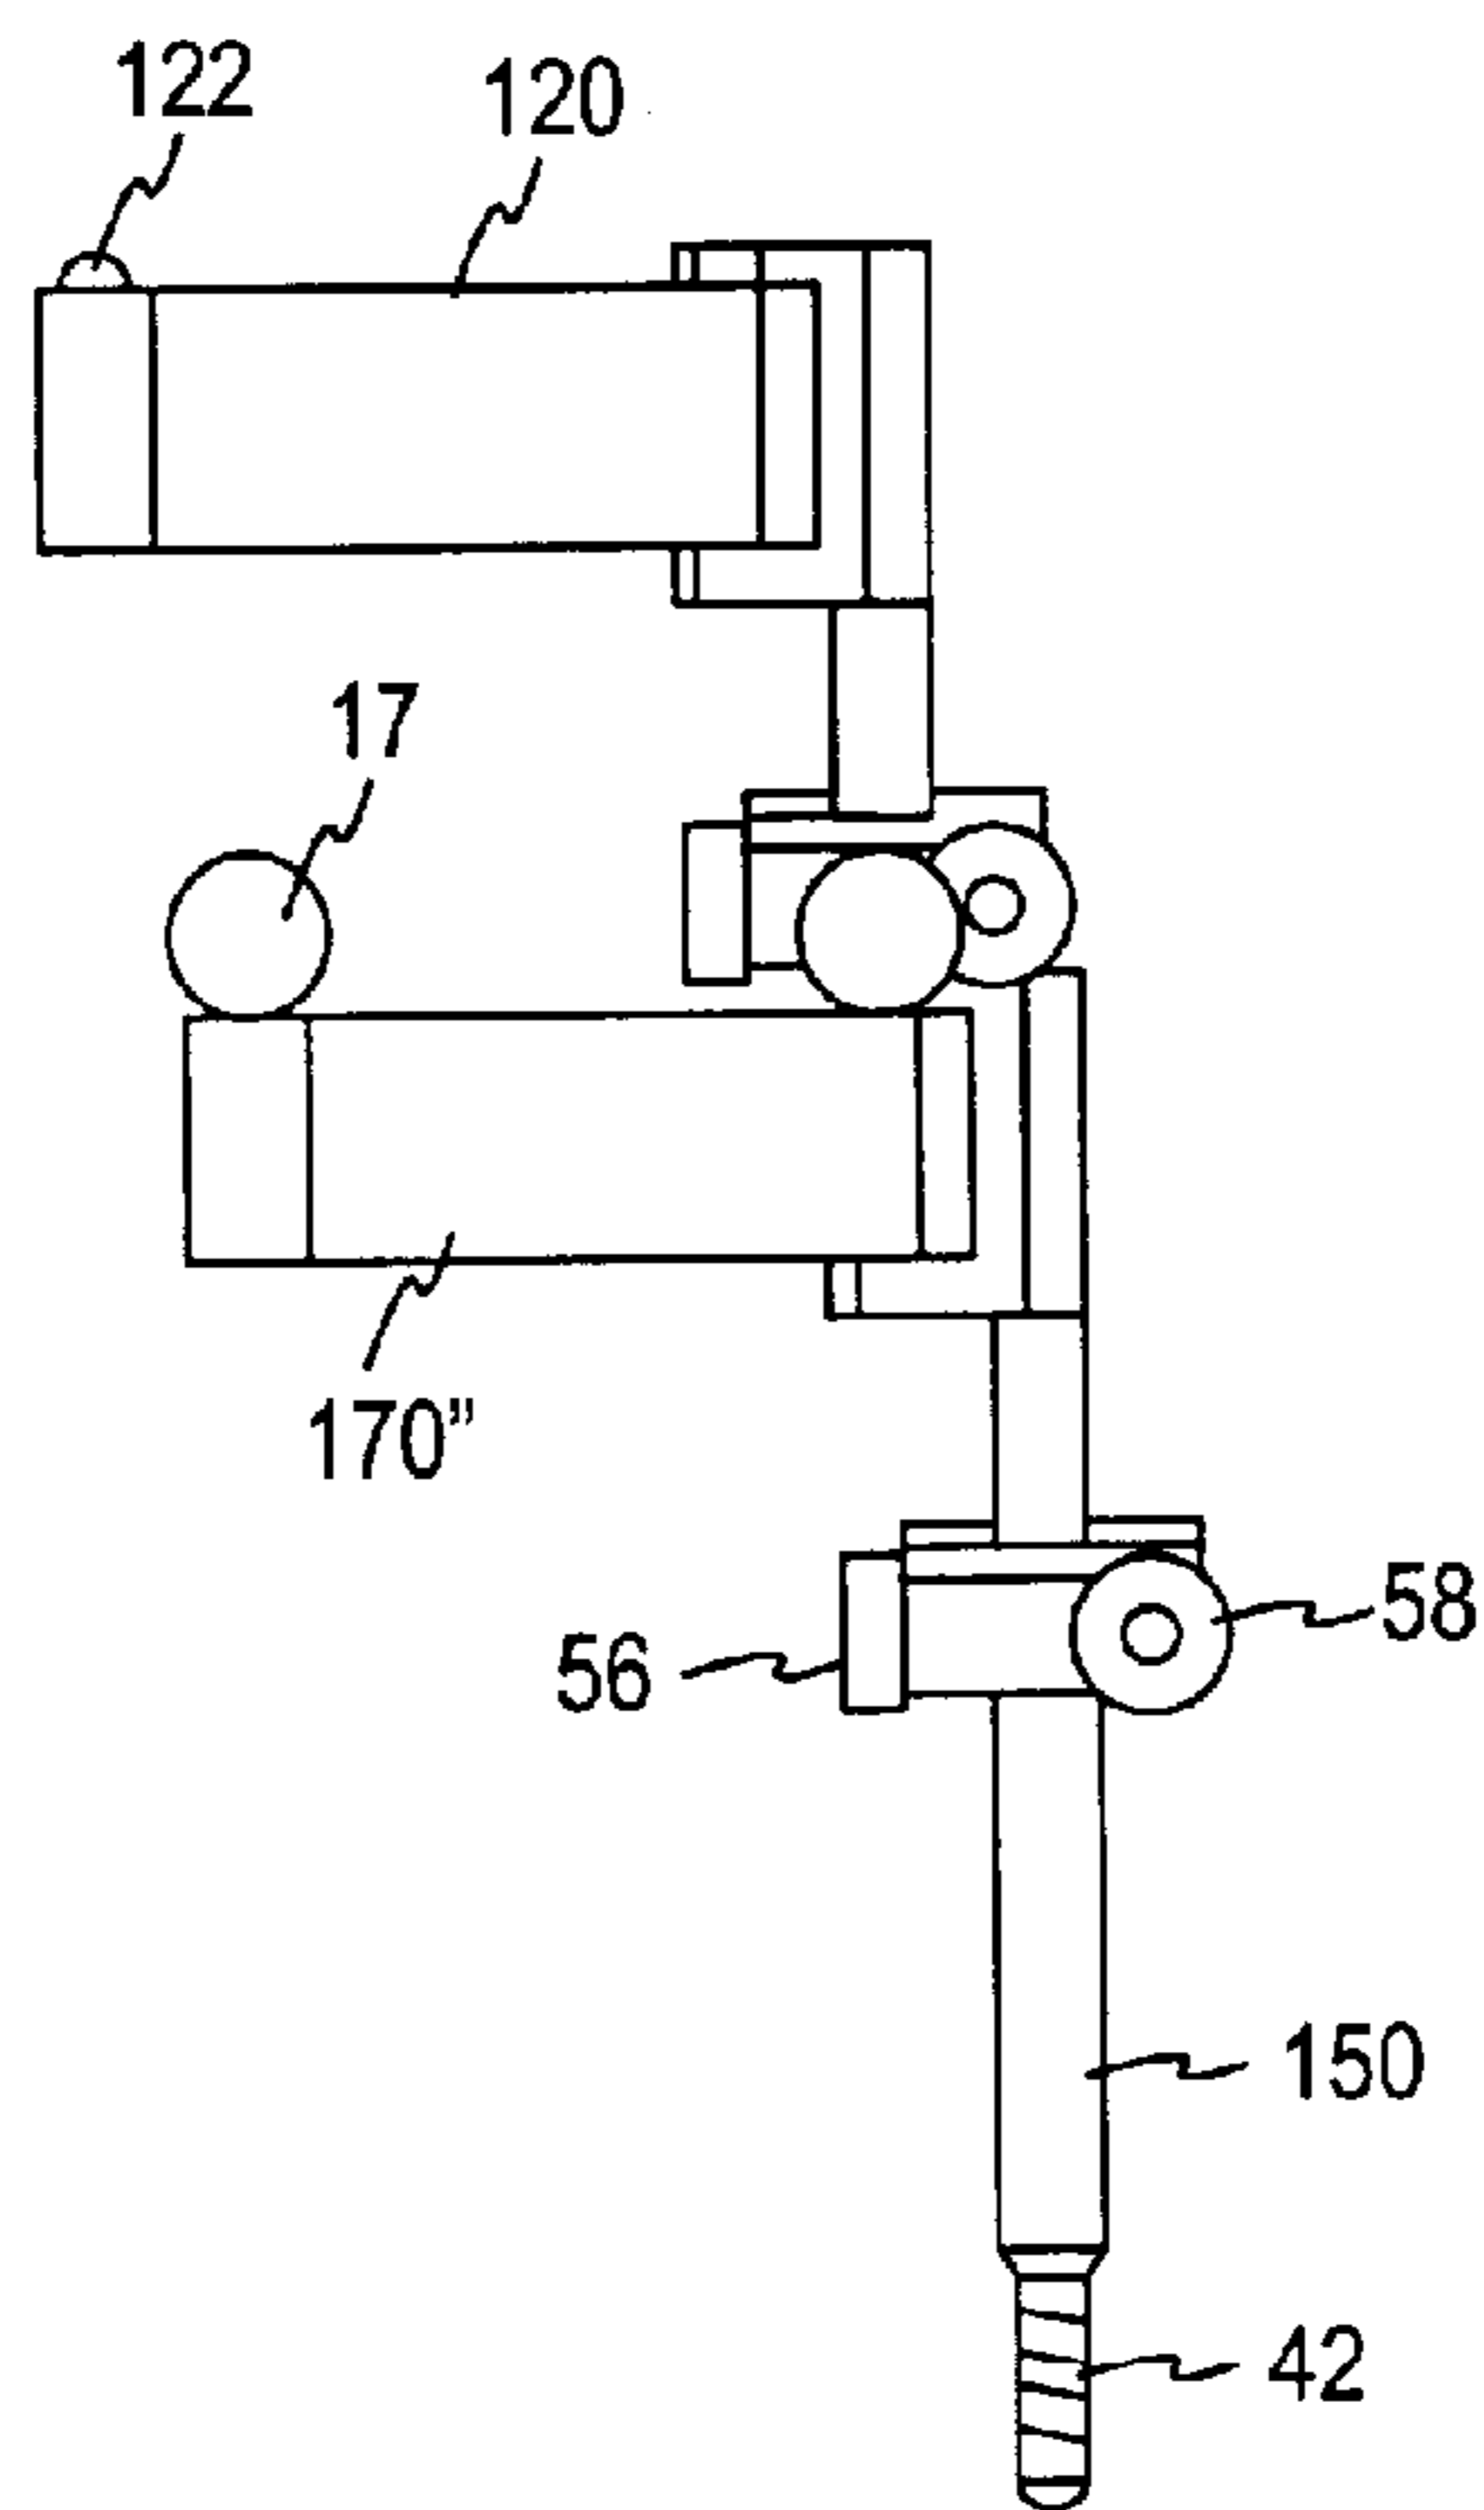
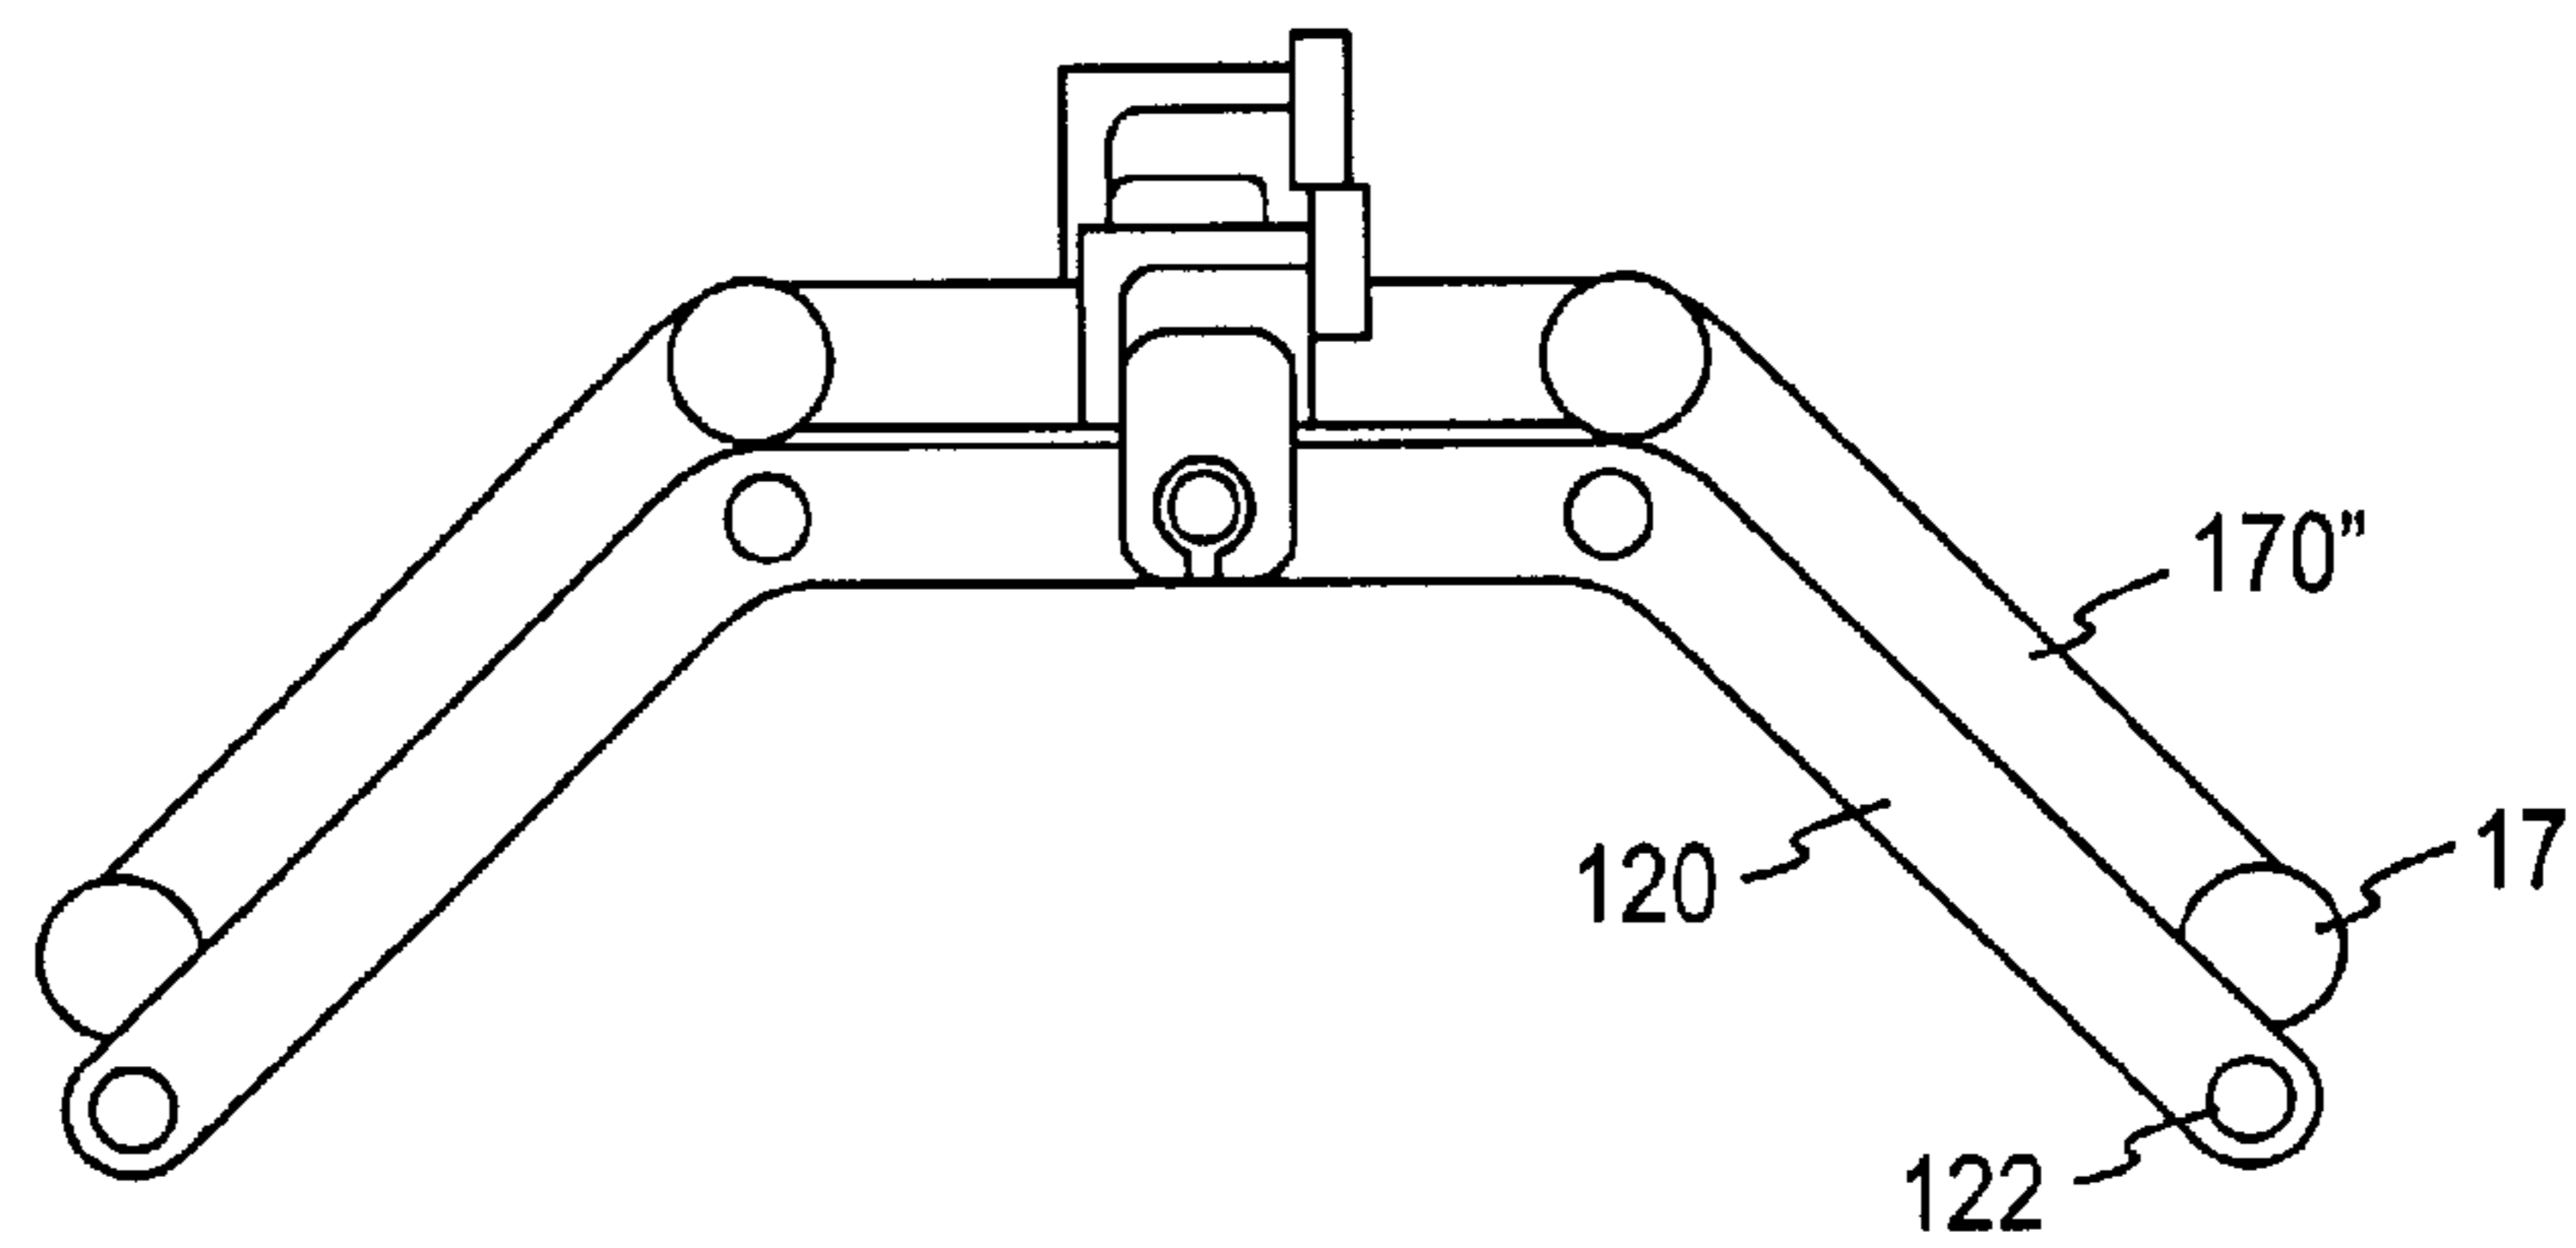
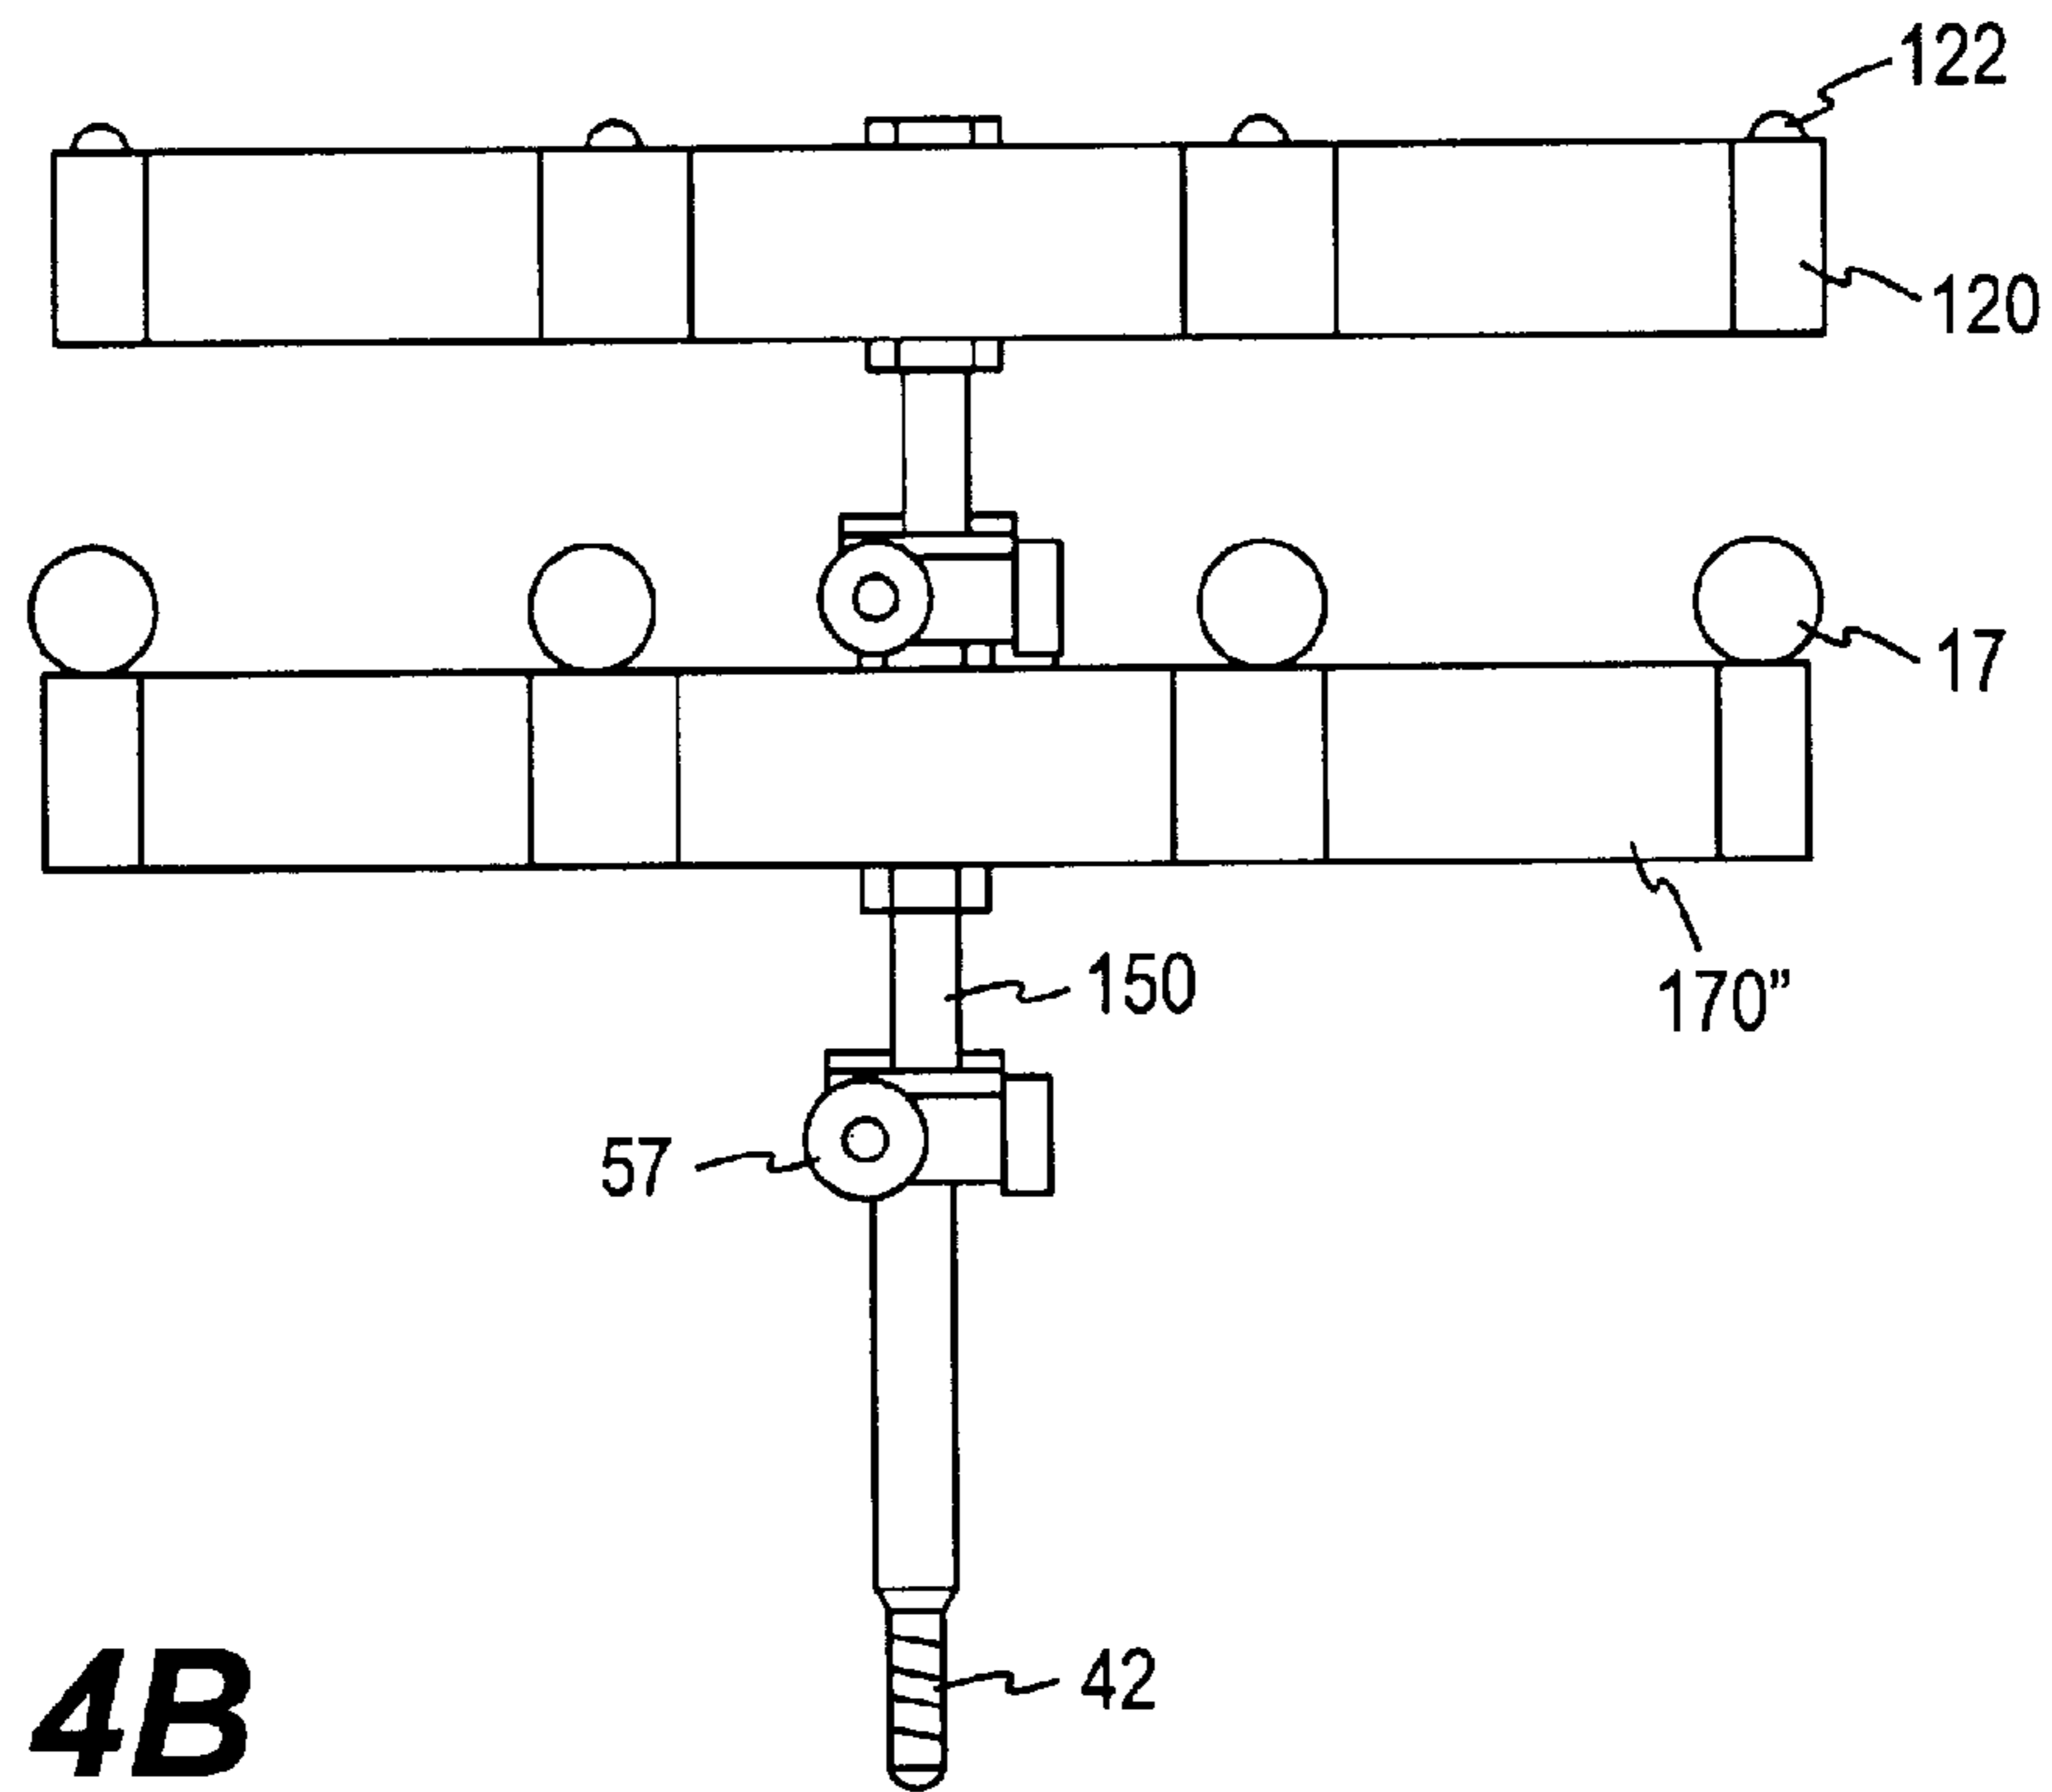


FIG. 4A



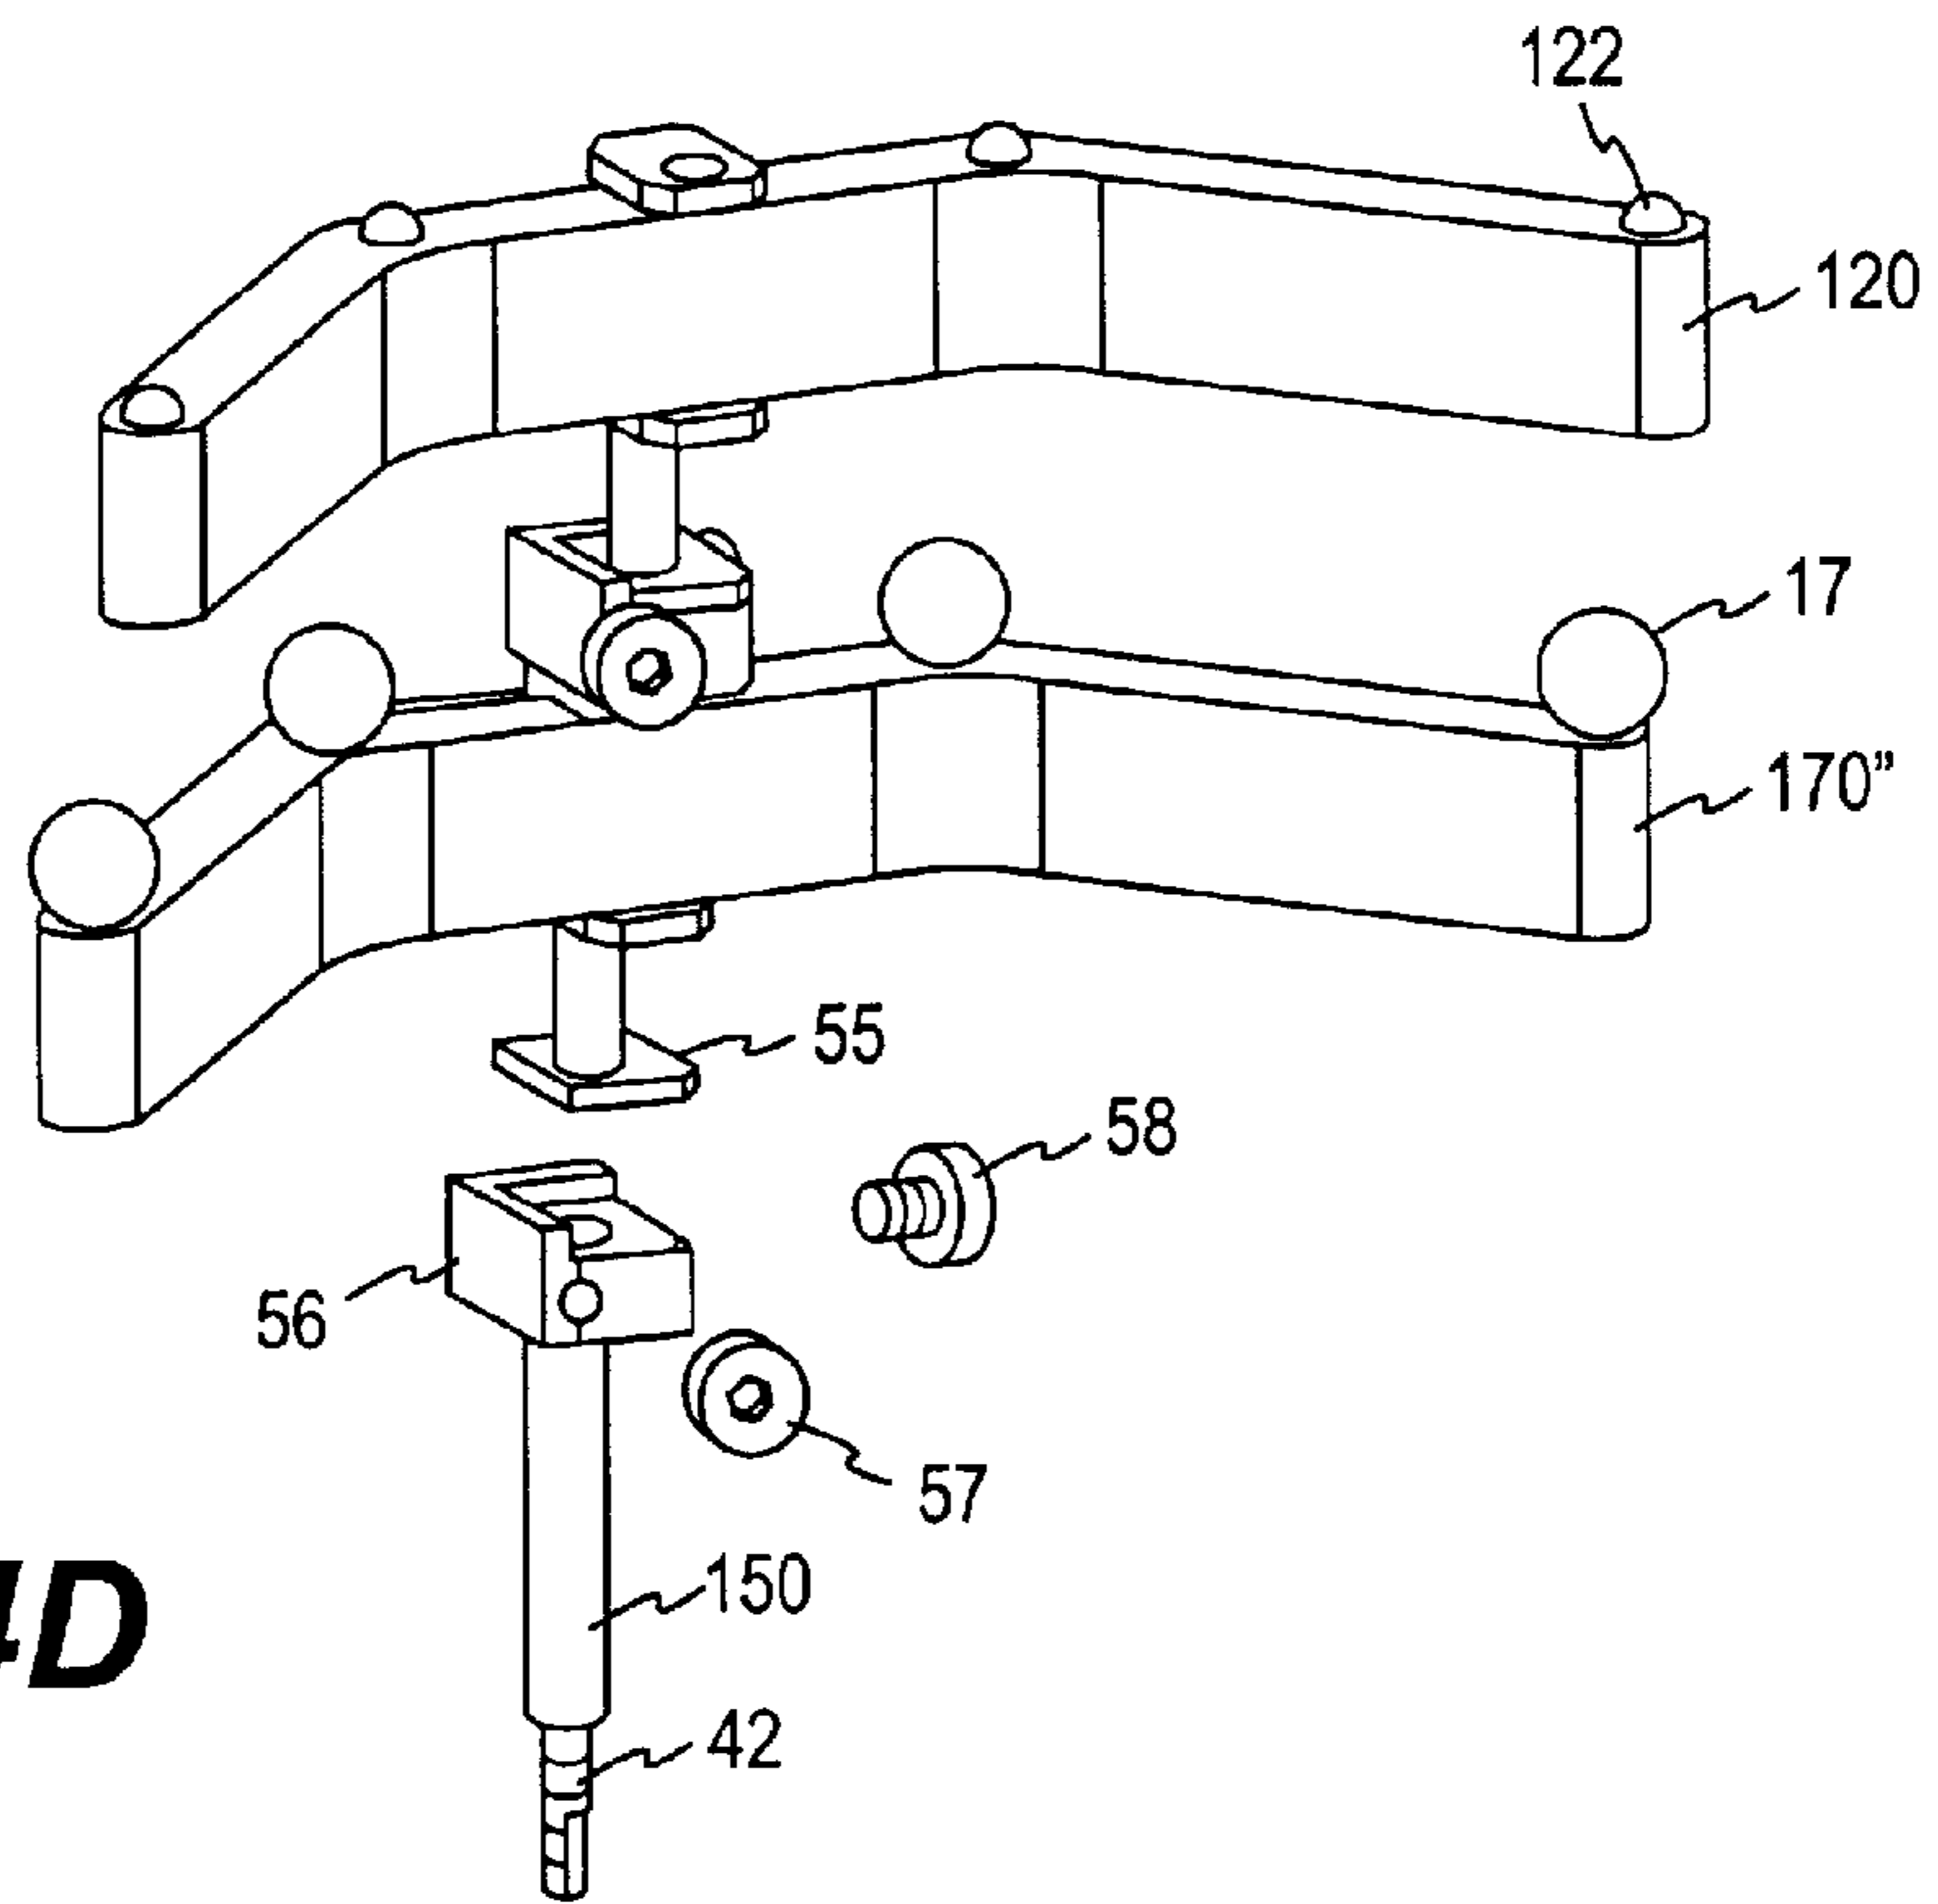


FIG. 4D

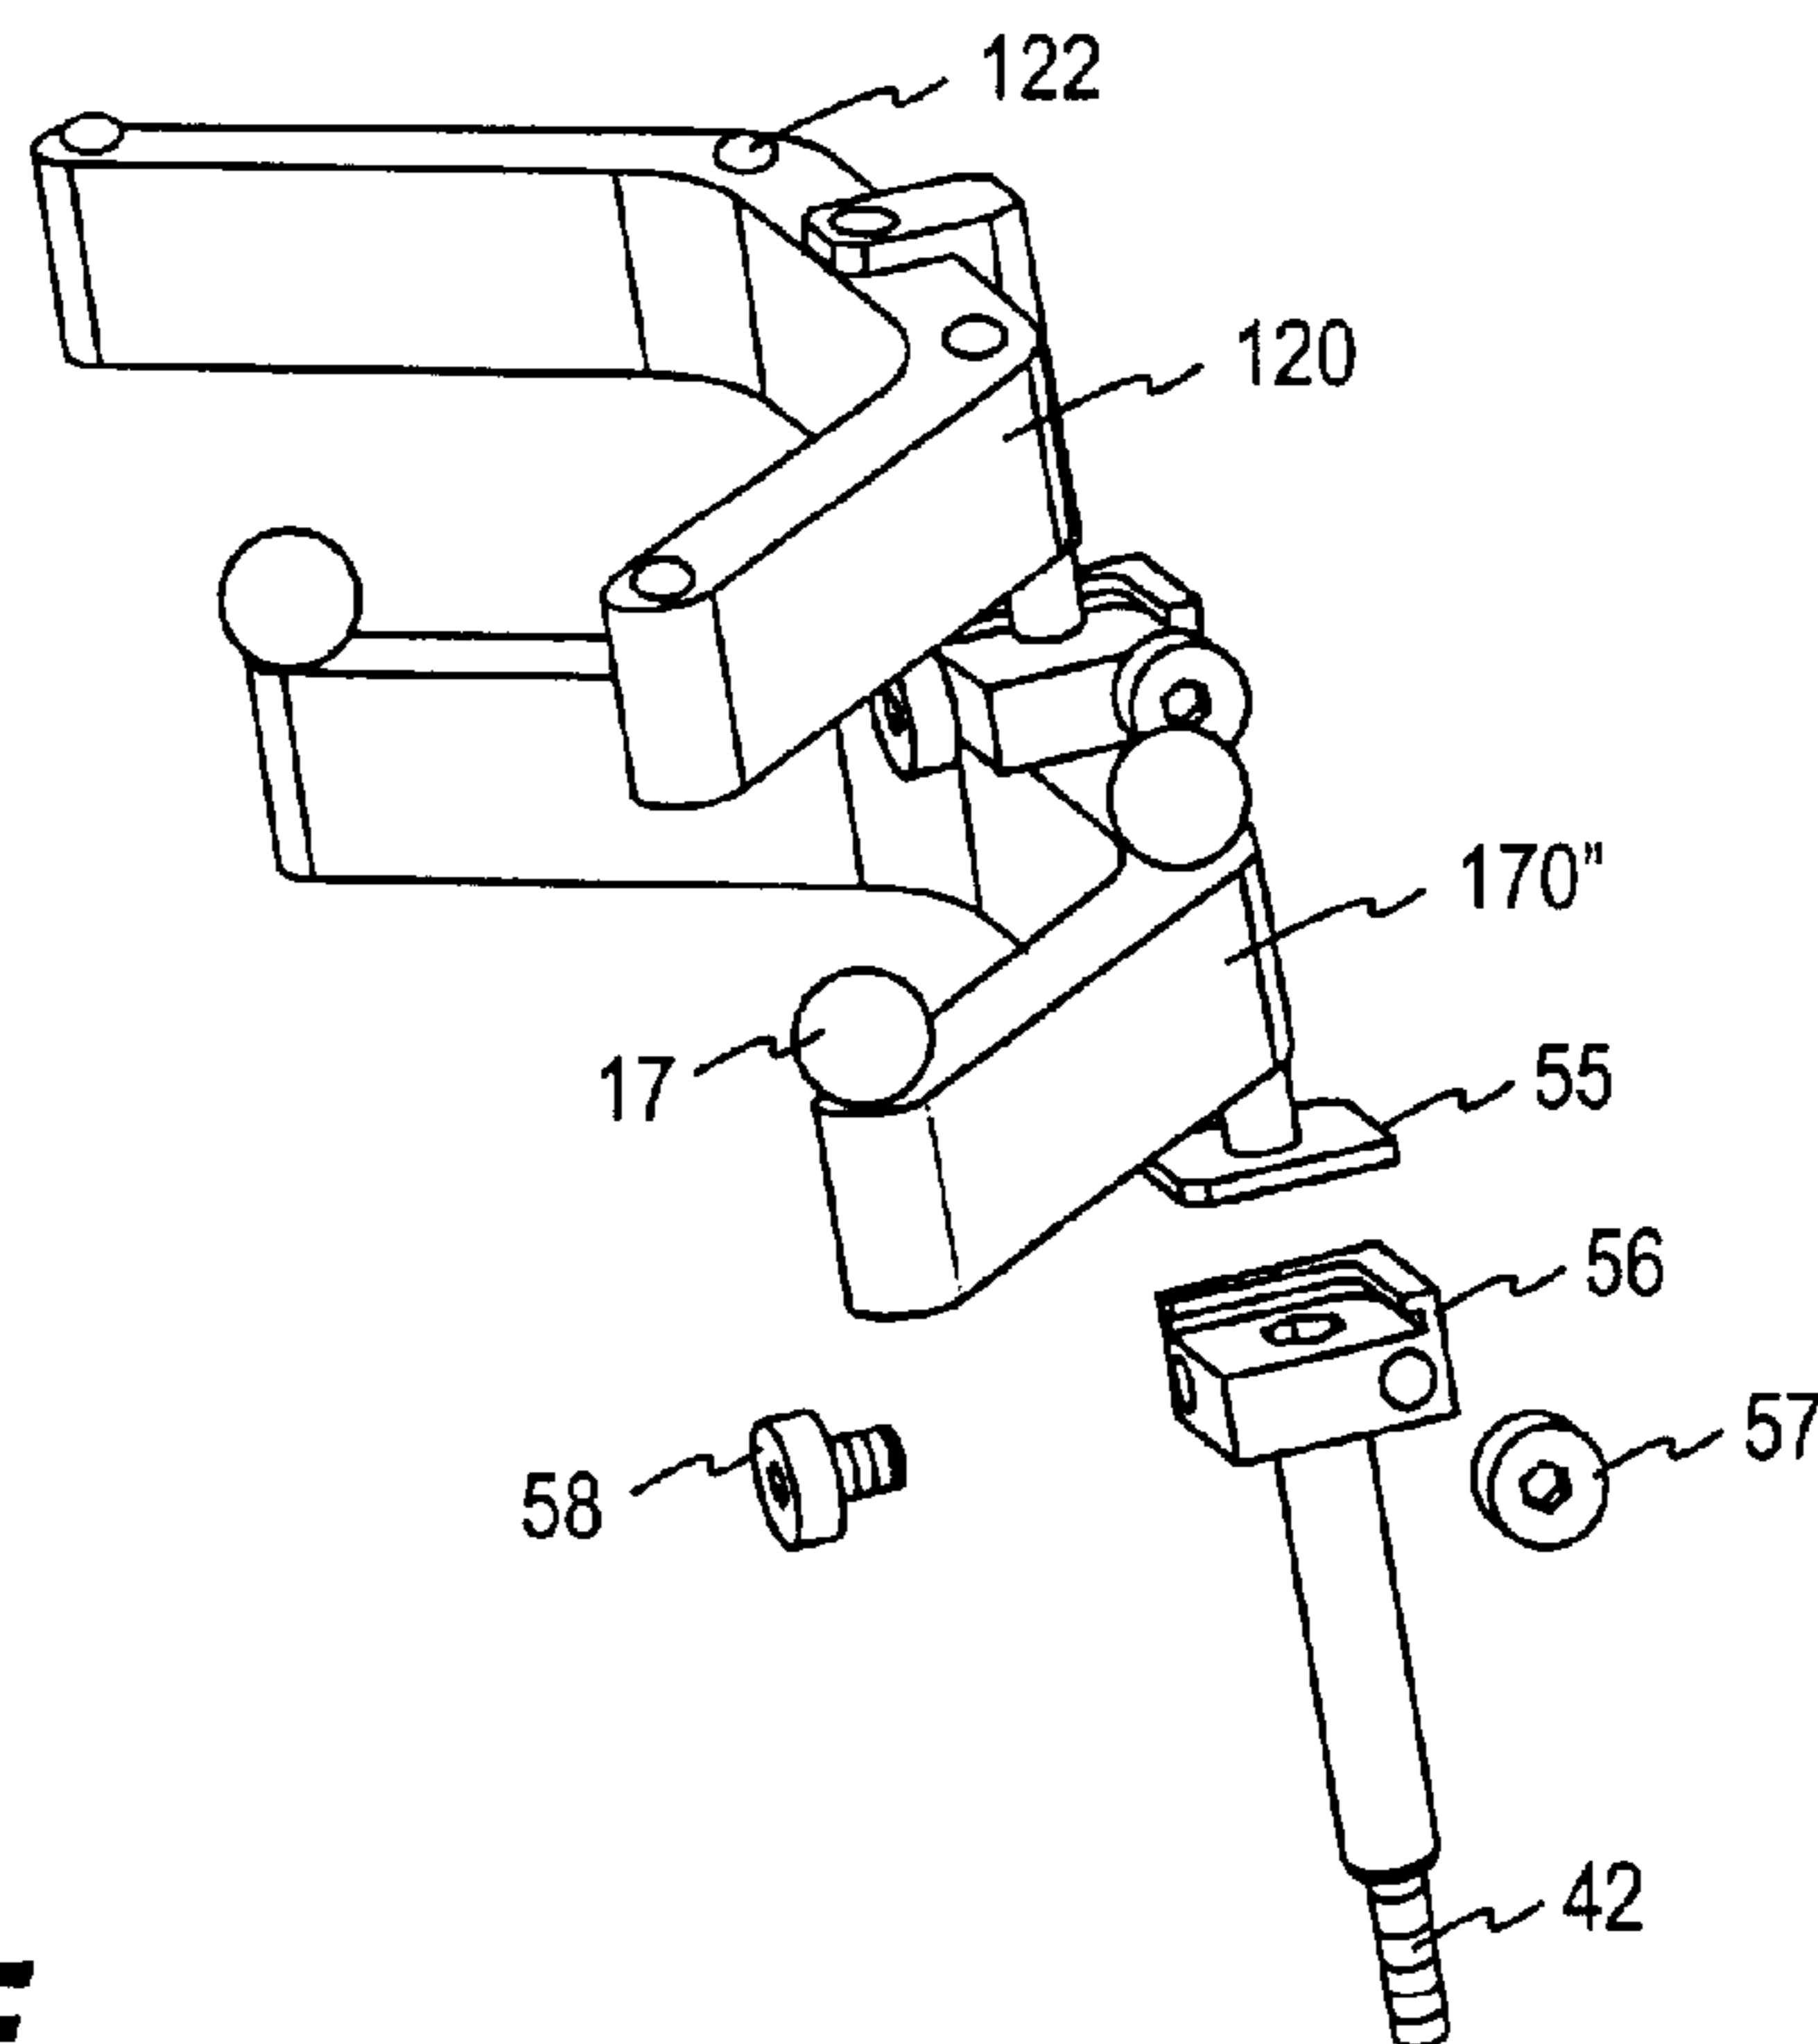


FIG. 4E

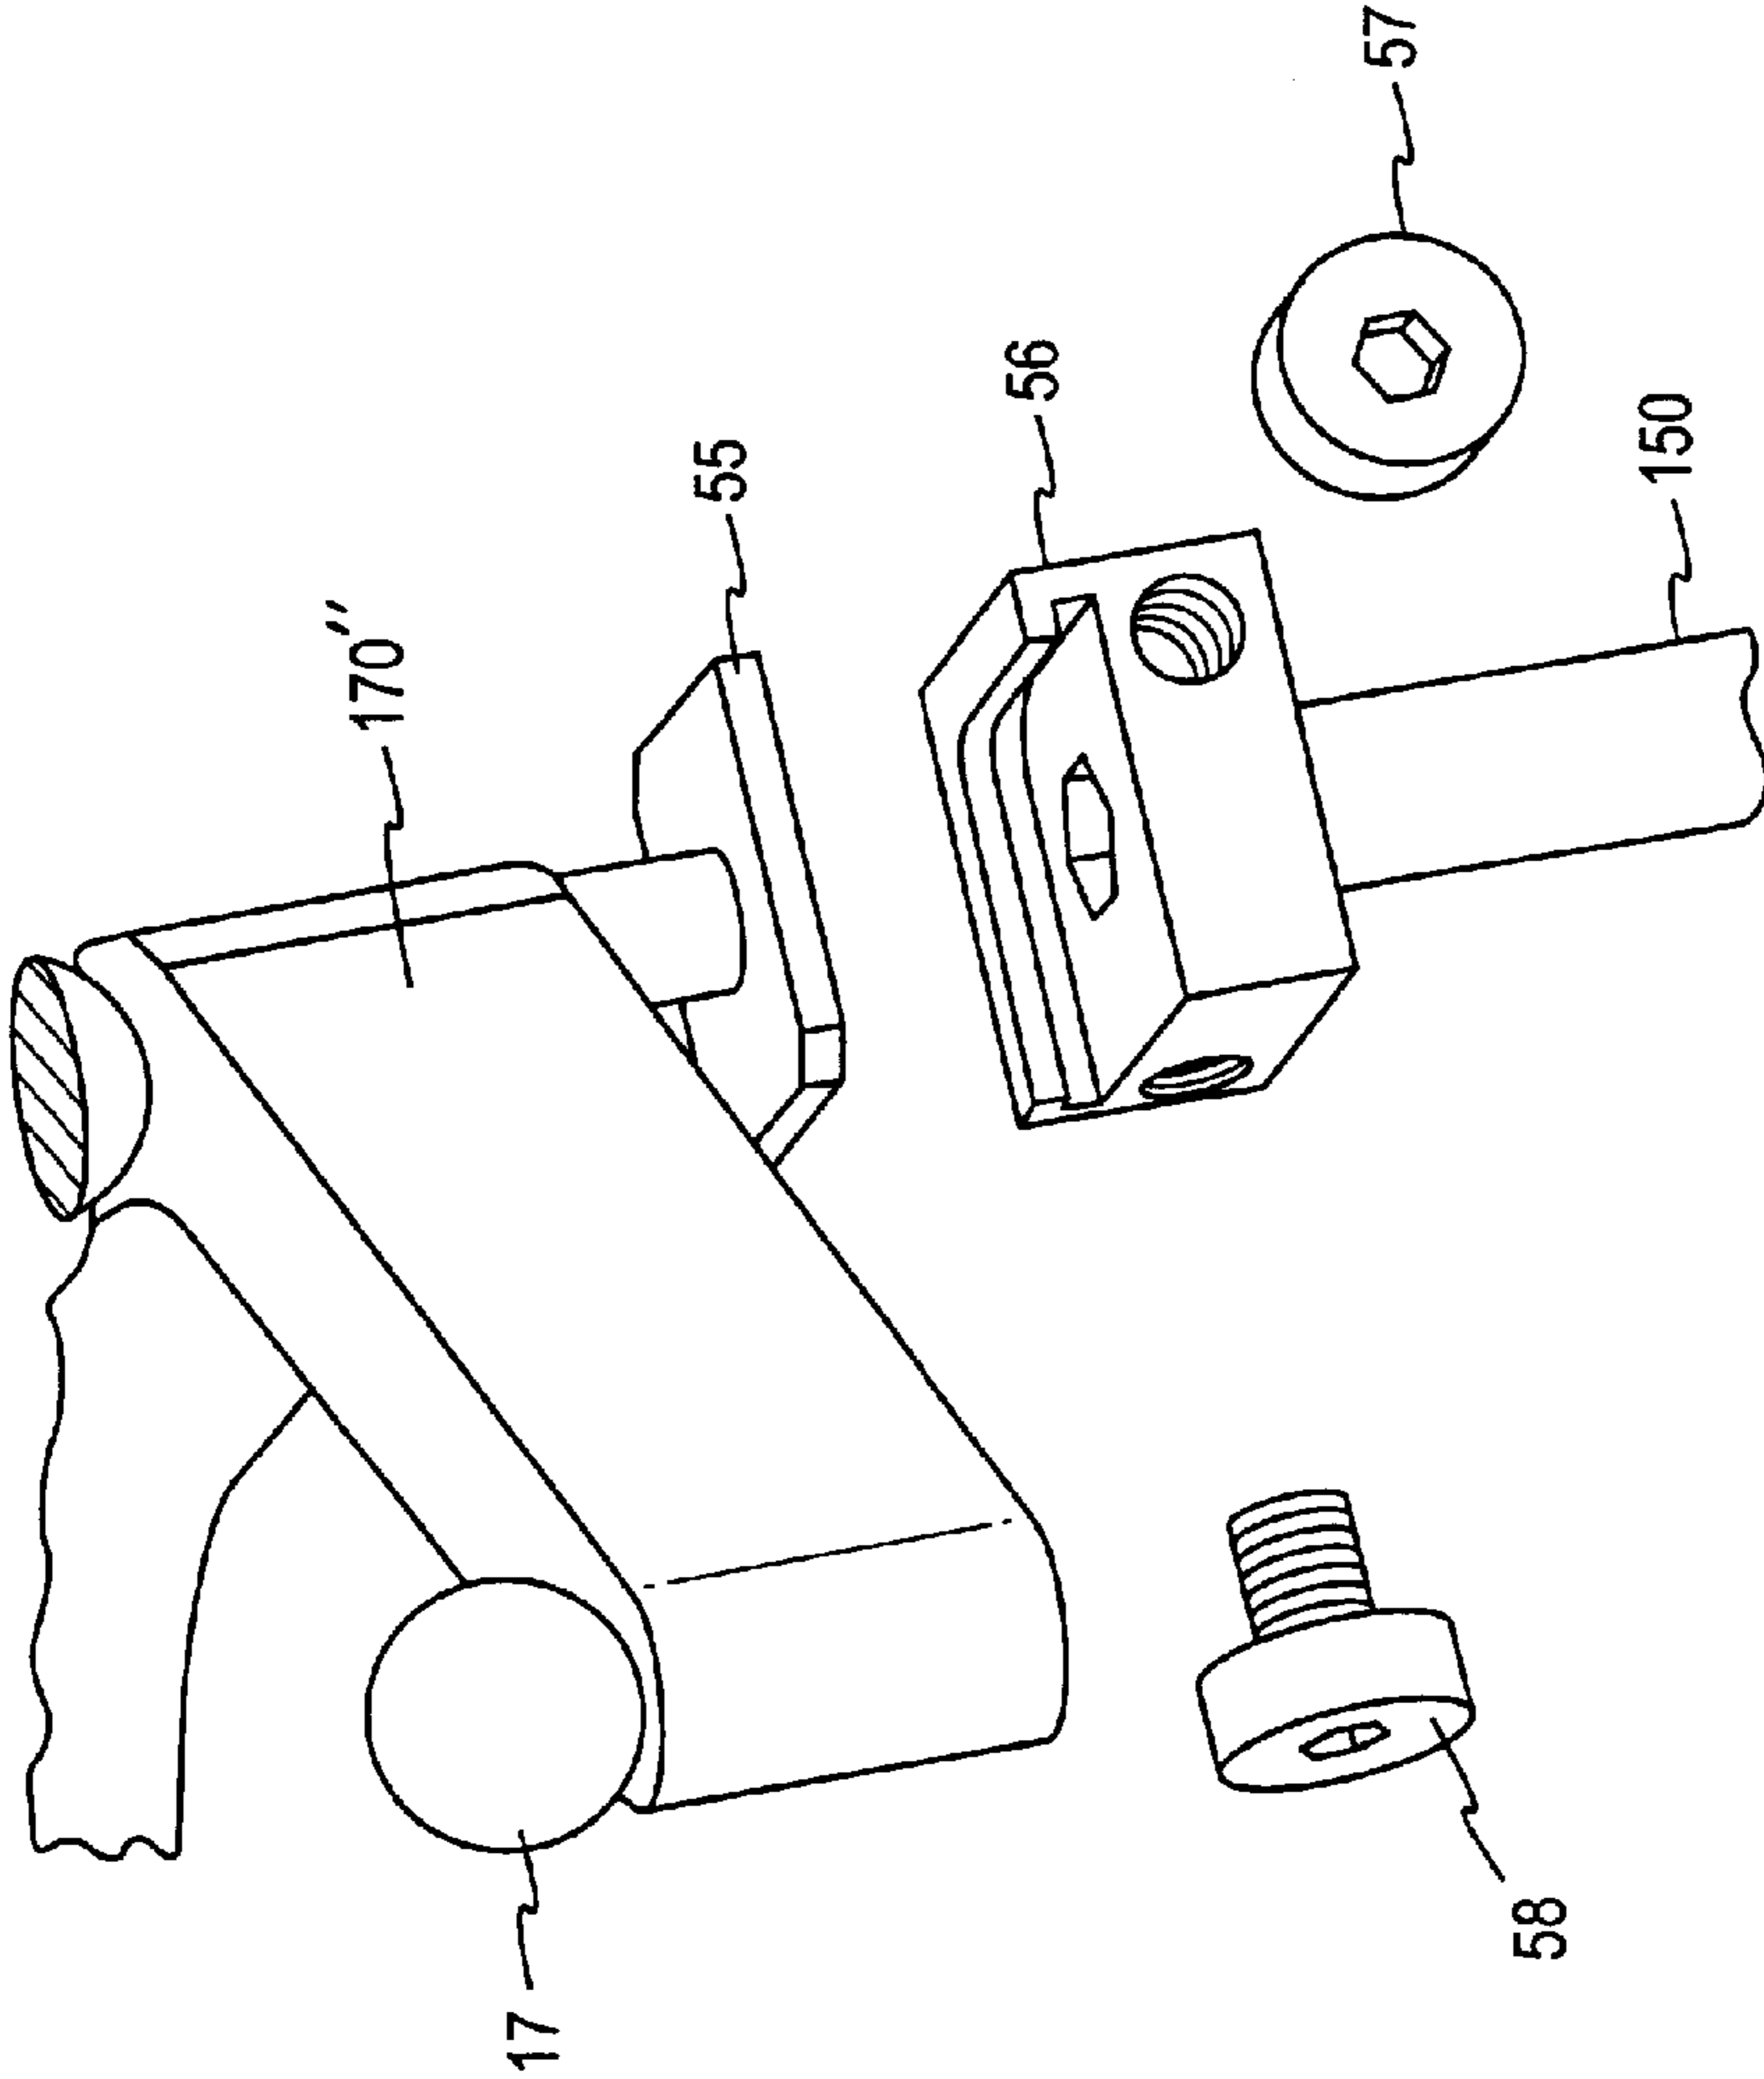


FIG. 4F

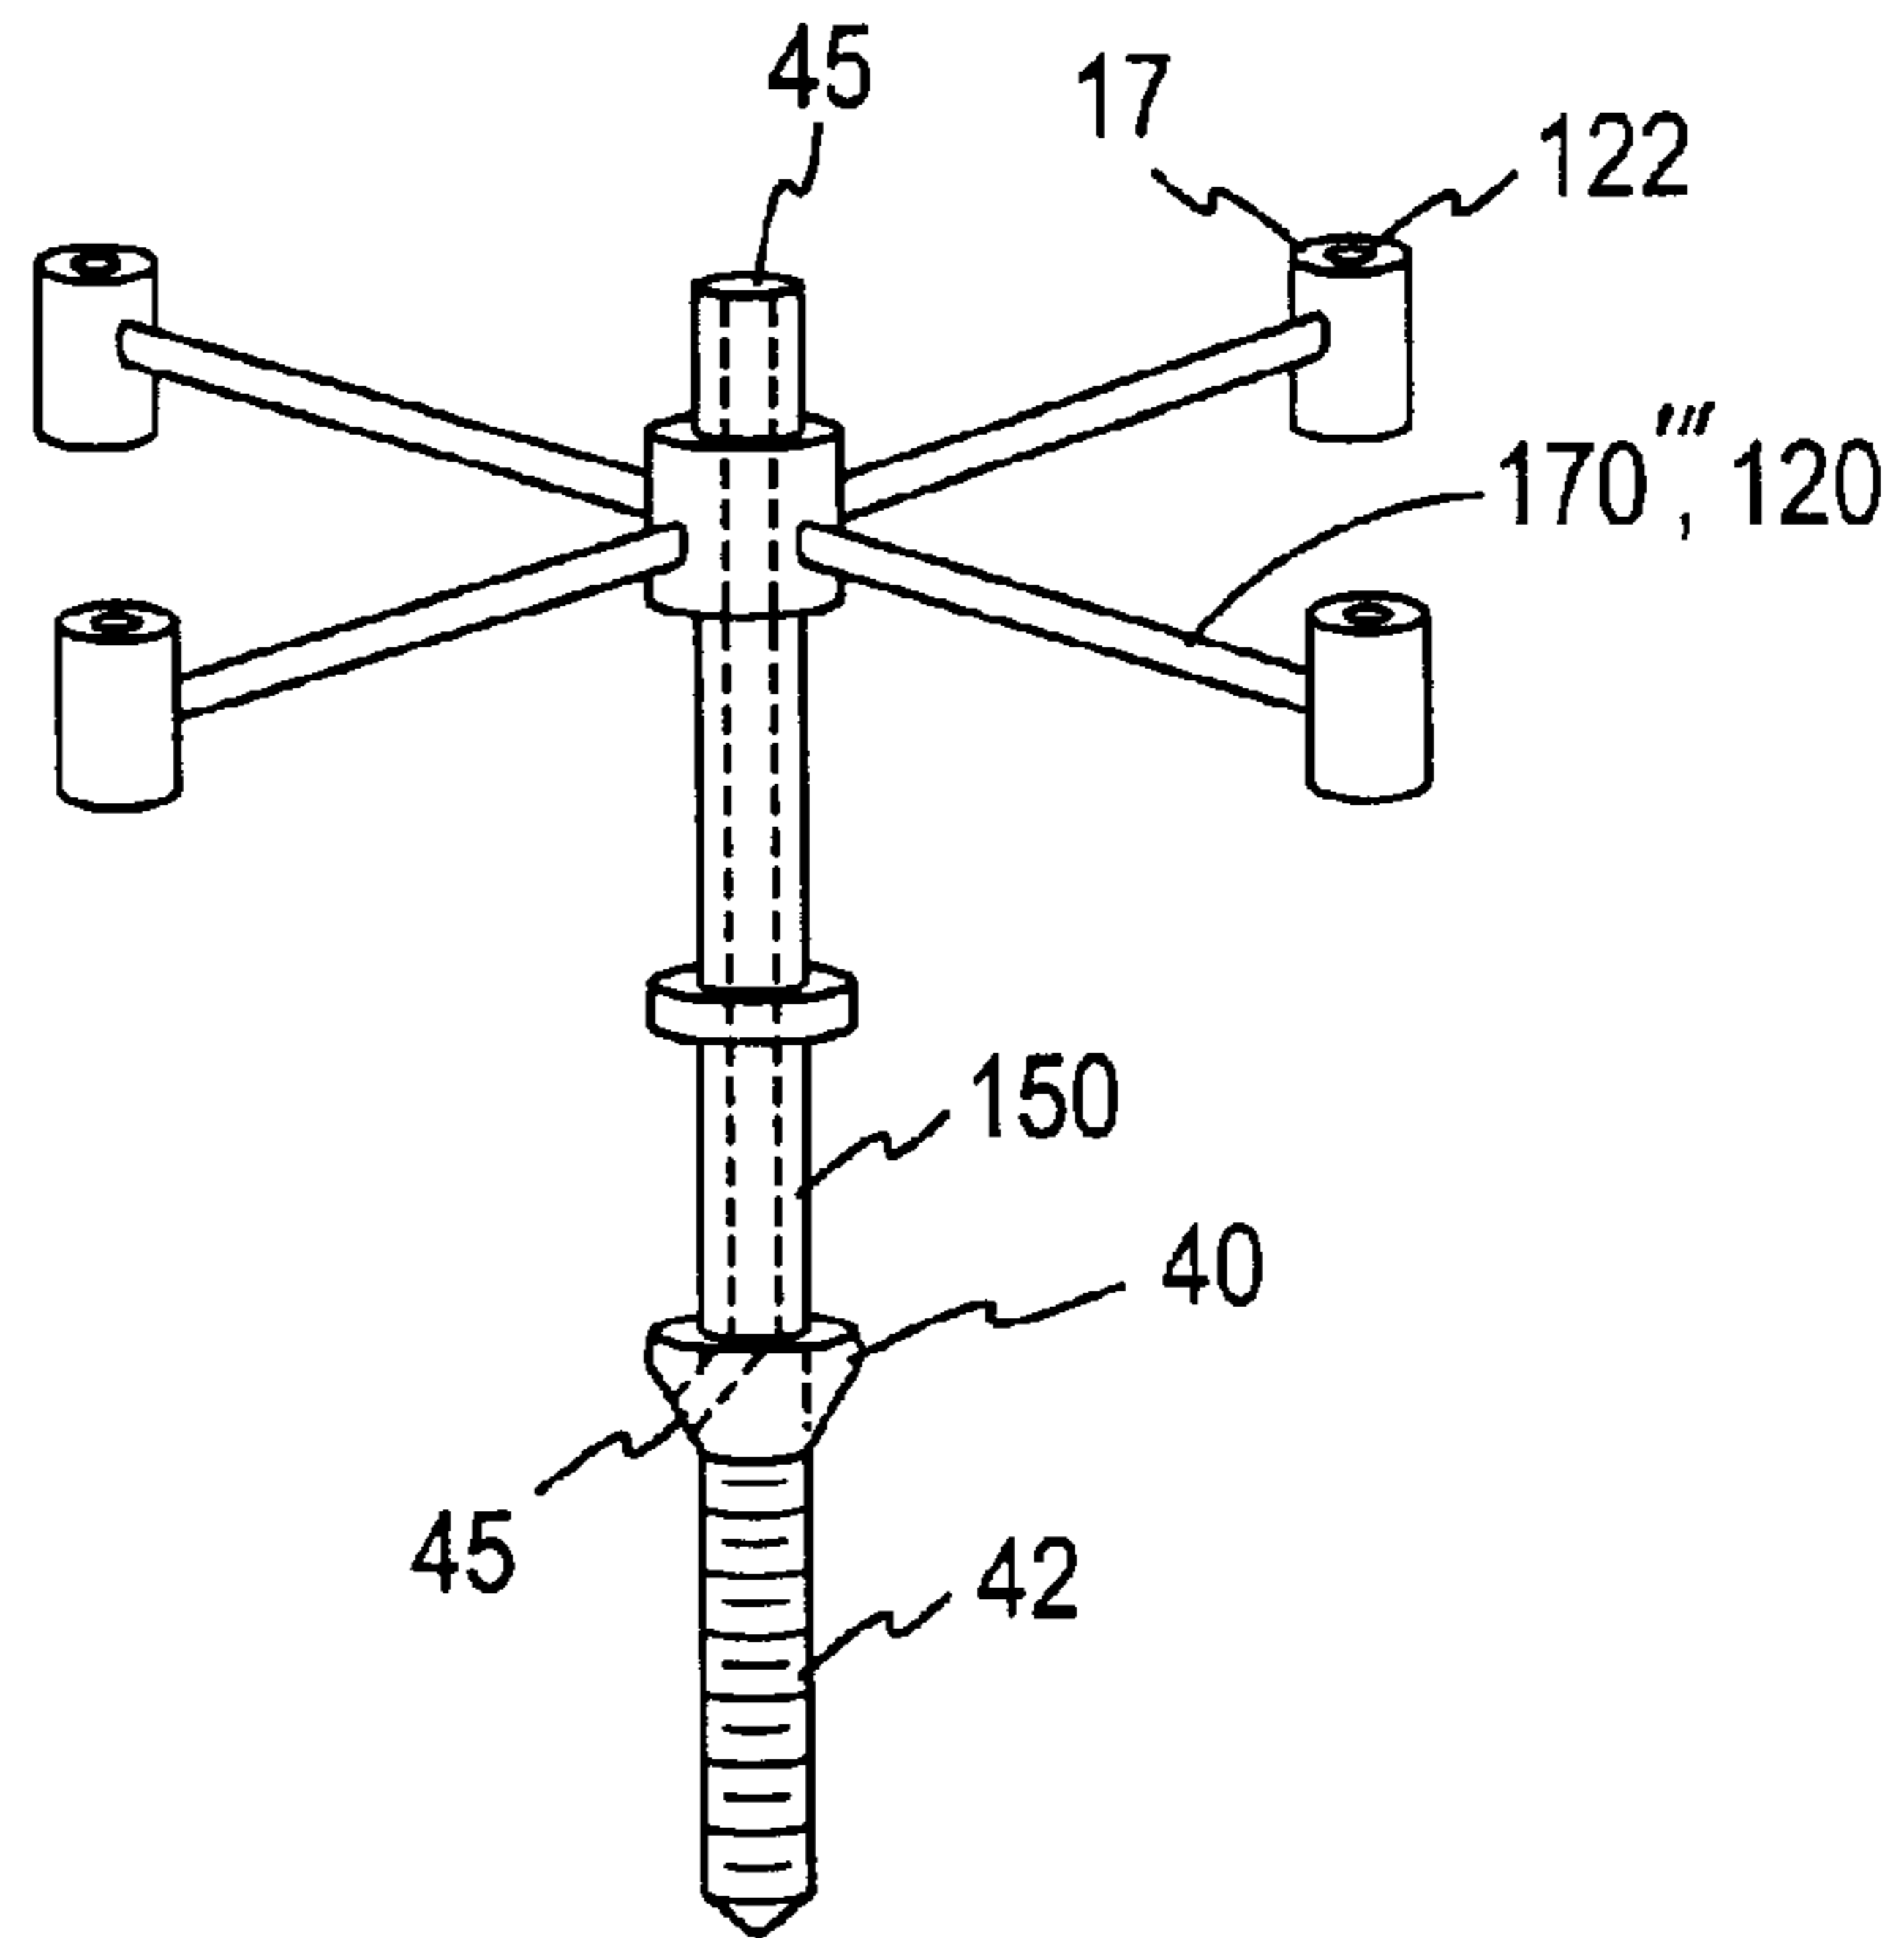


FIG. 5

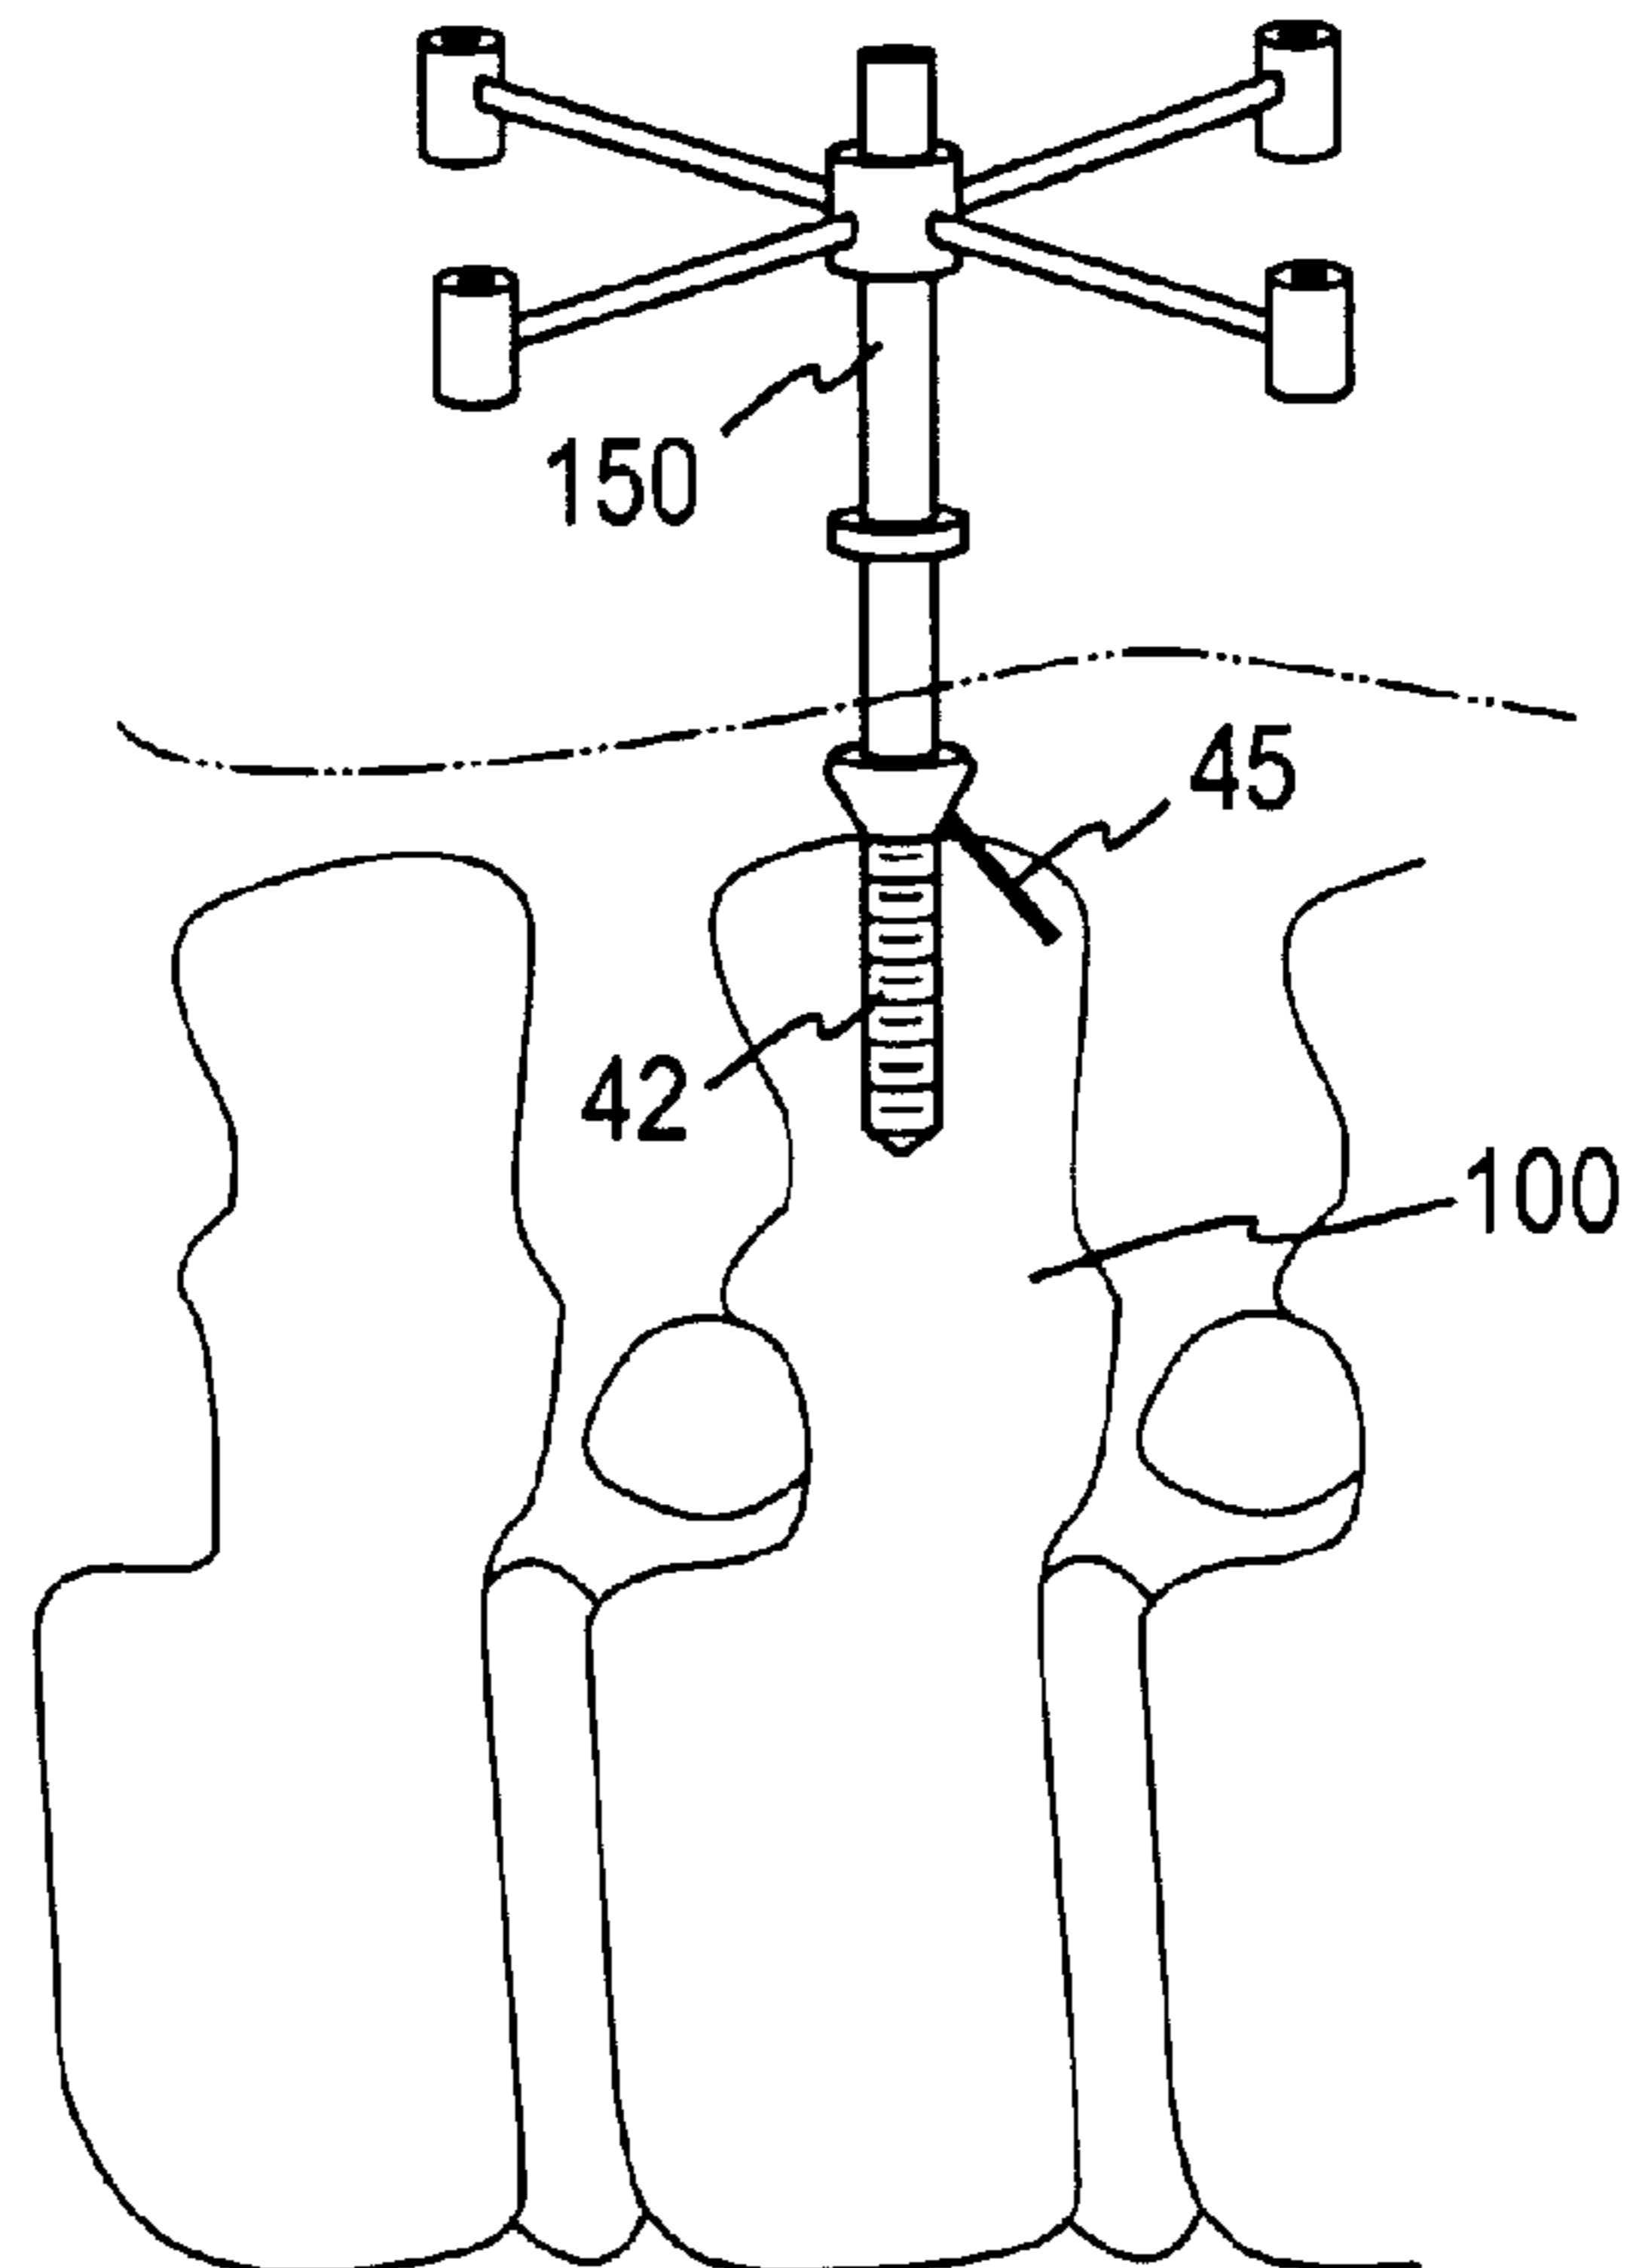


FIG. 6

FIG. 7

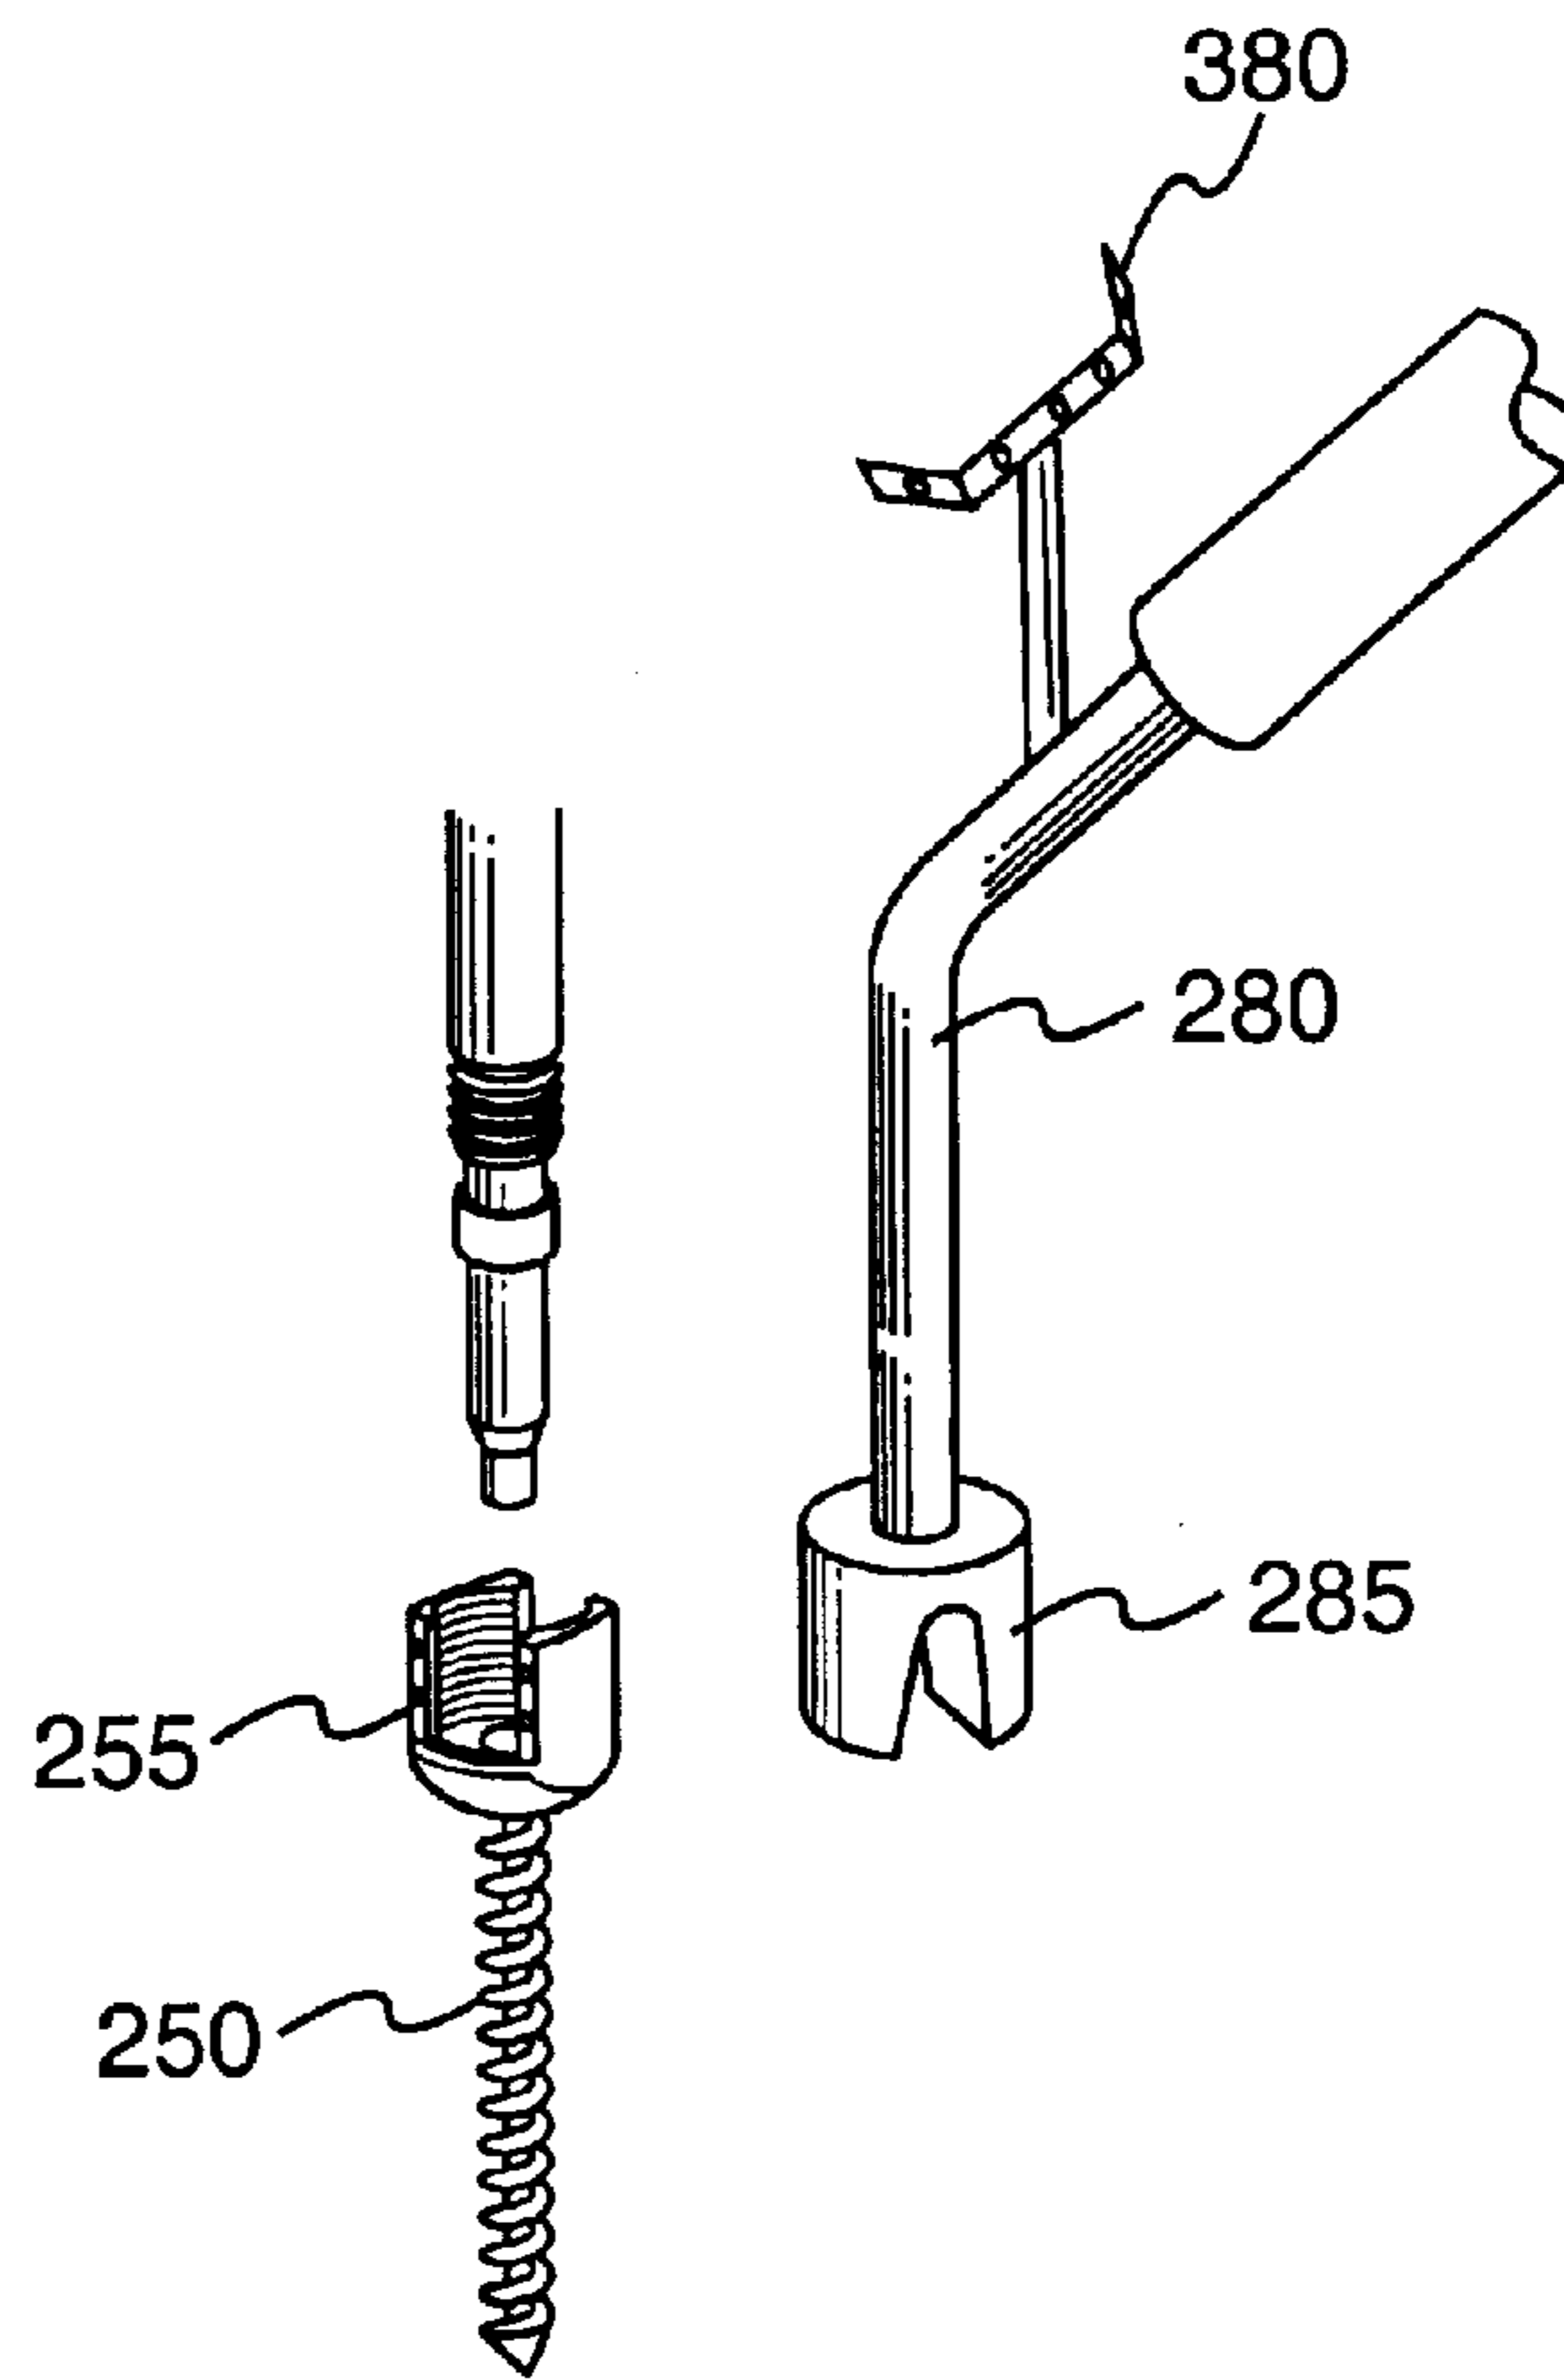
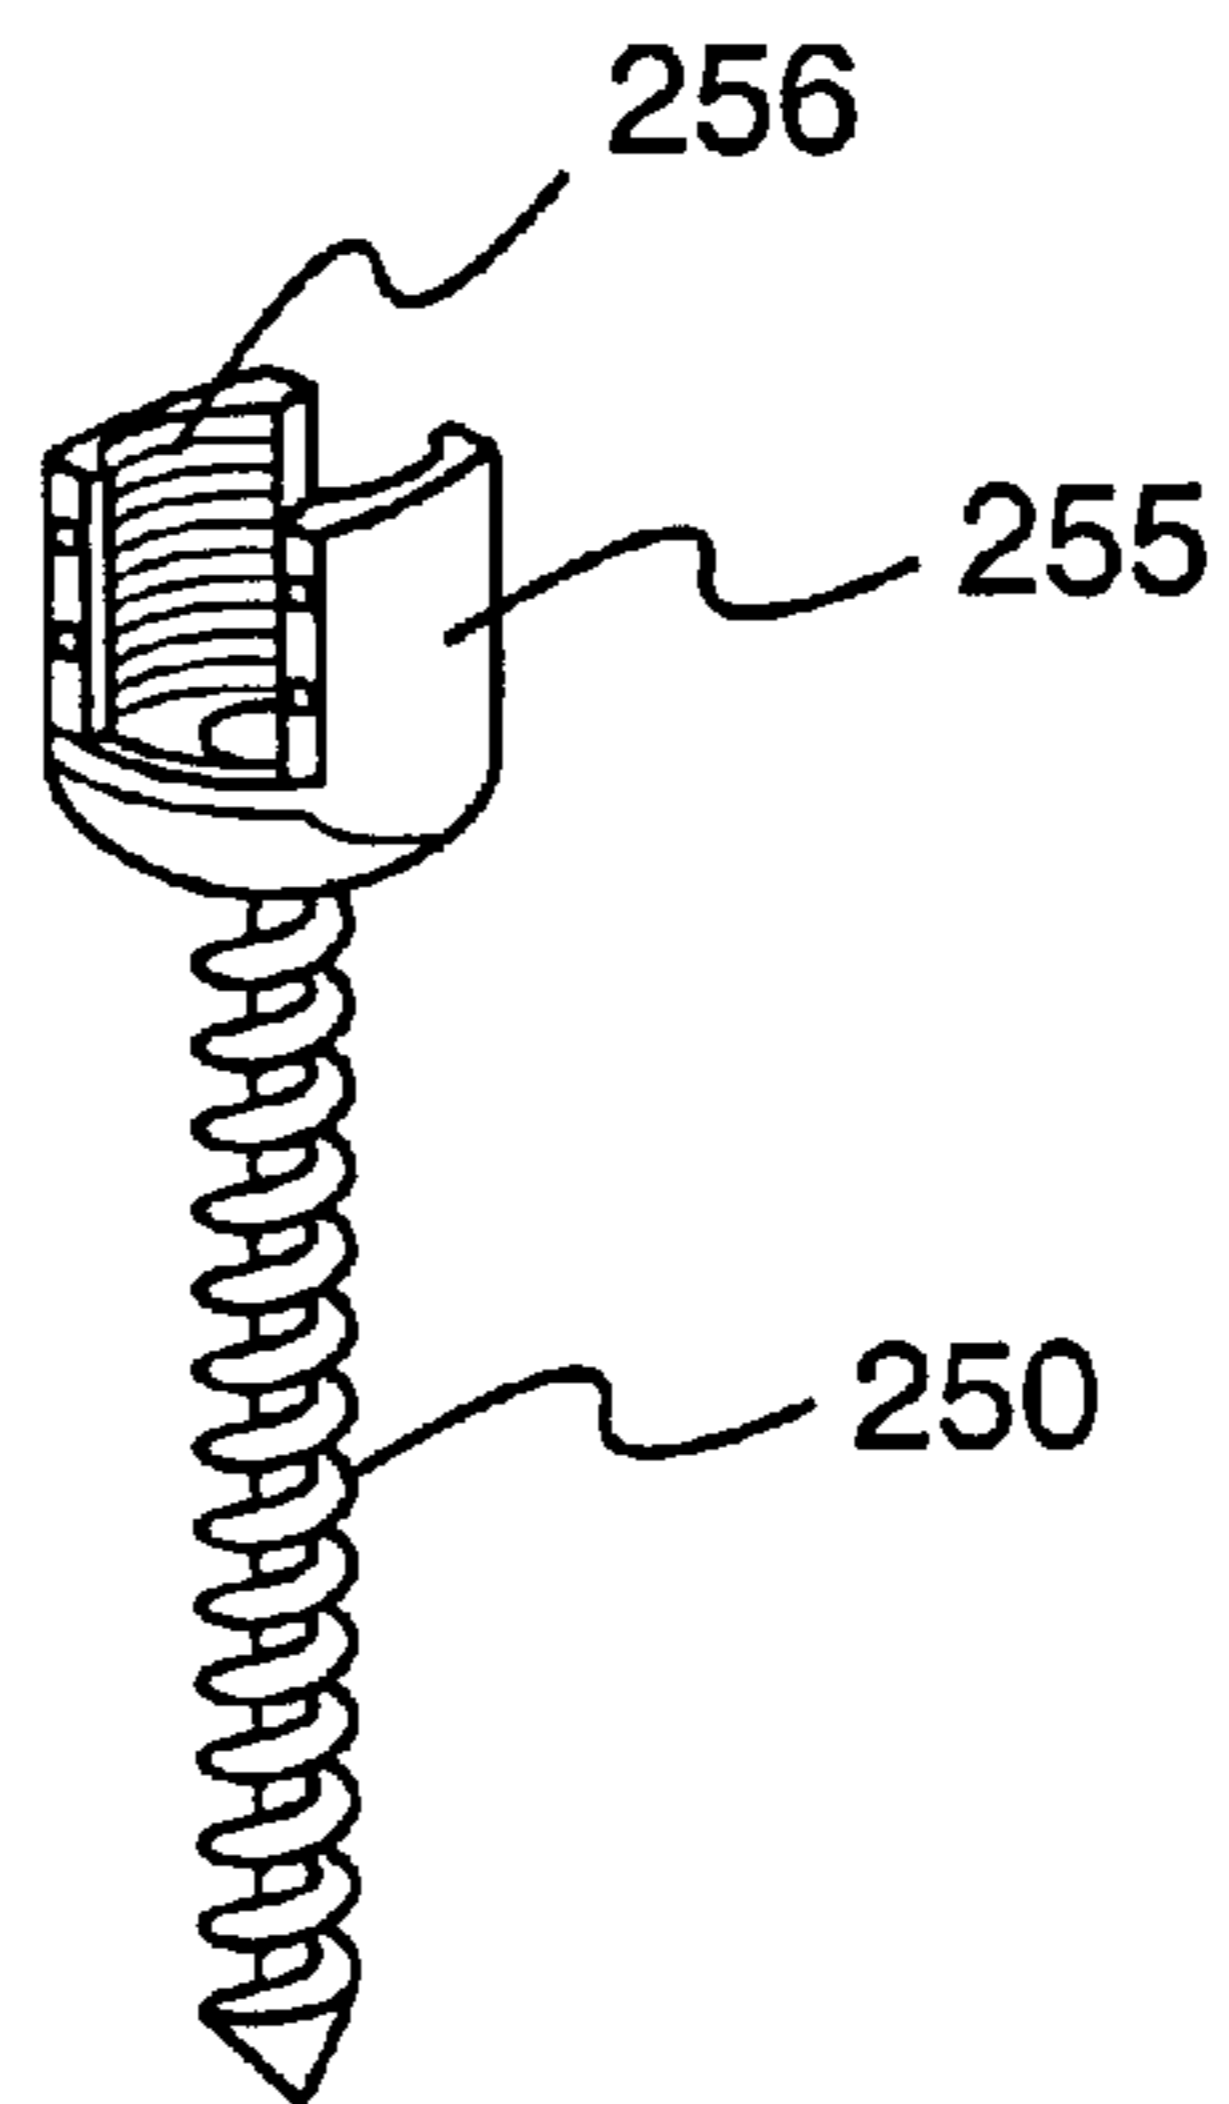


FIG. 7A



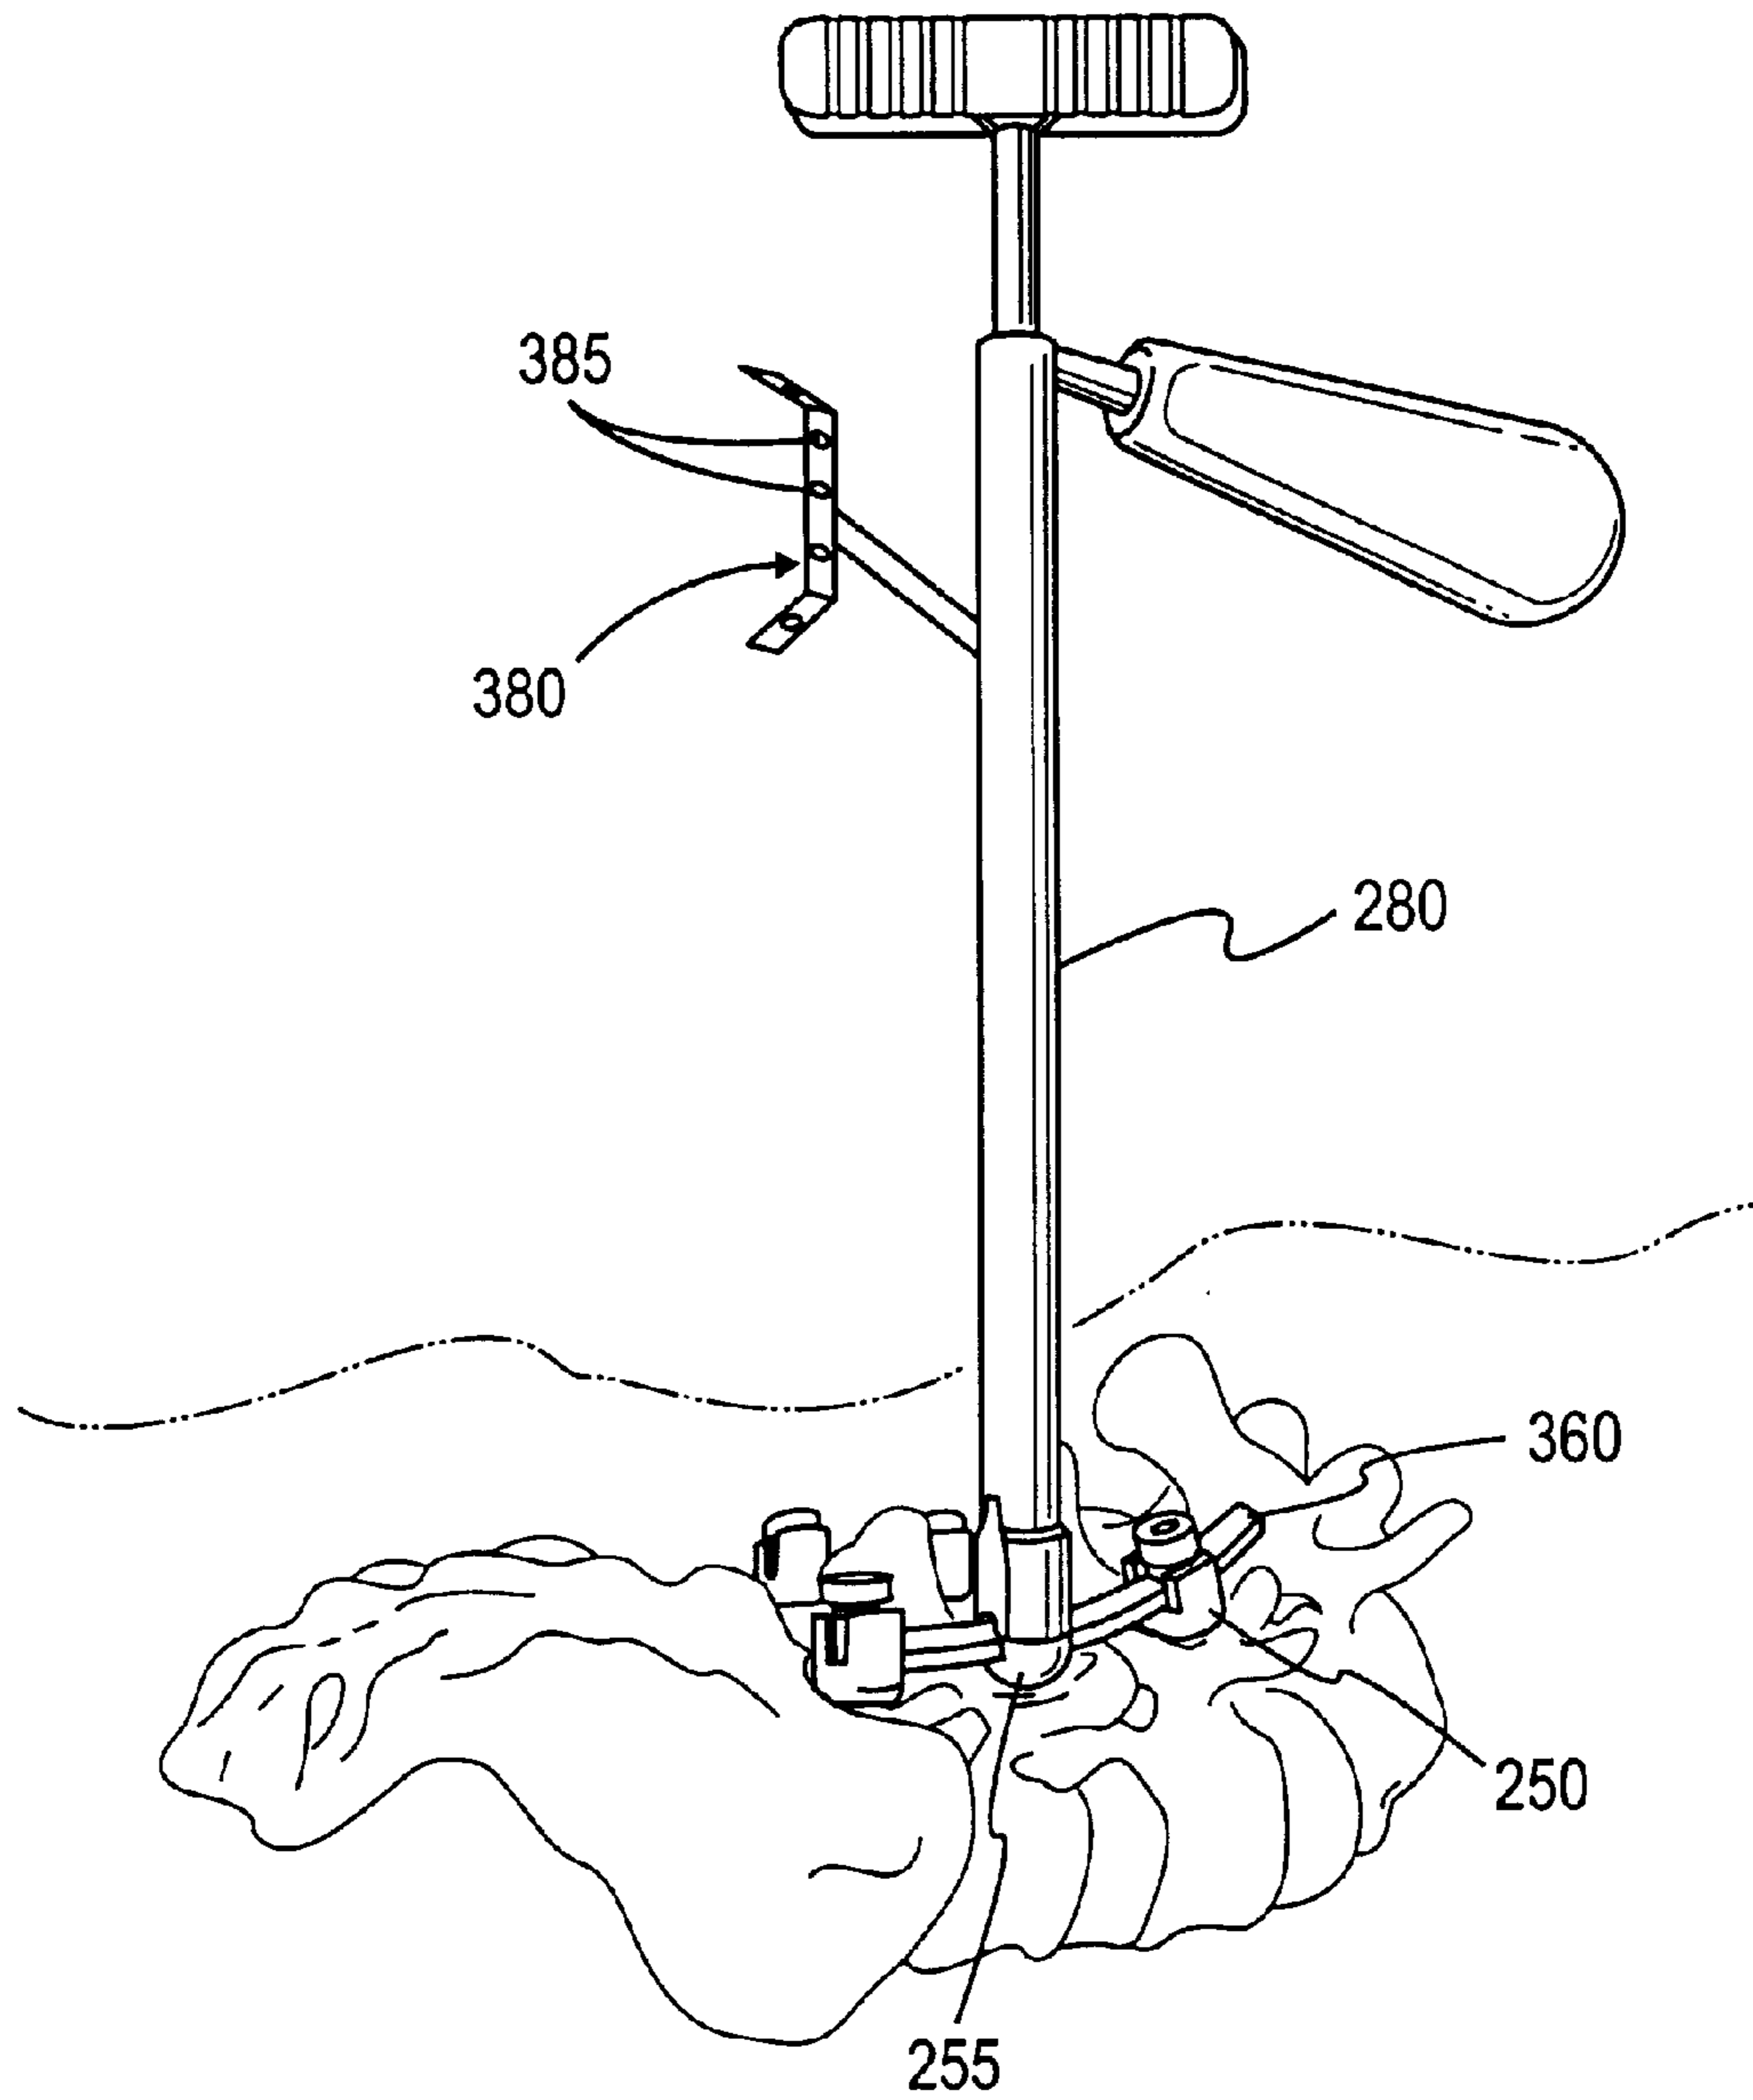


FIG. 8

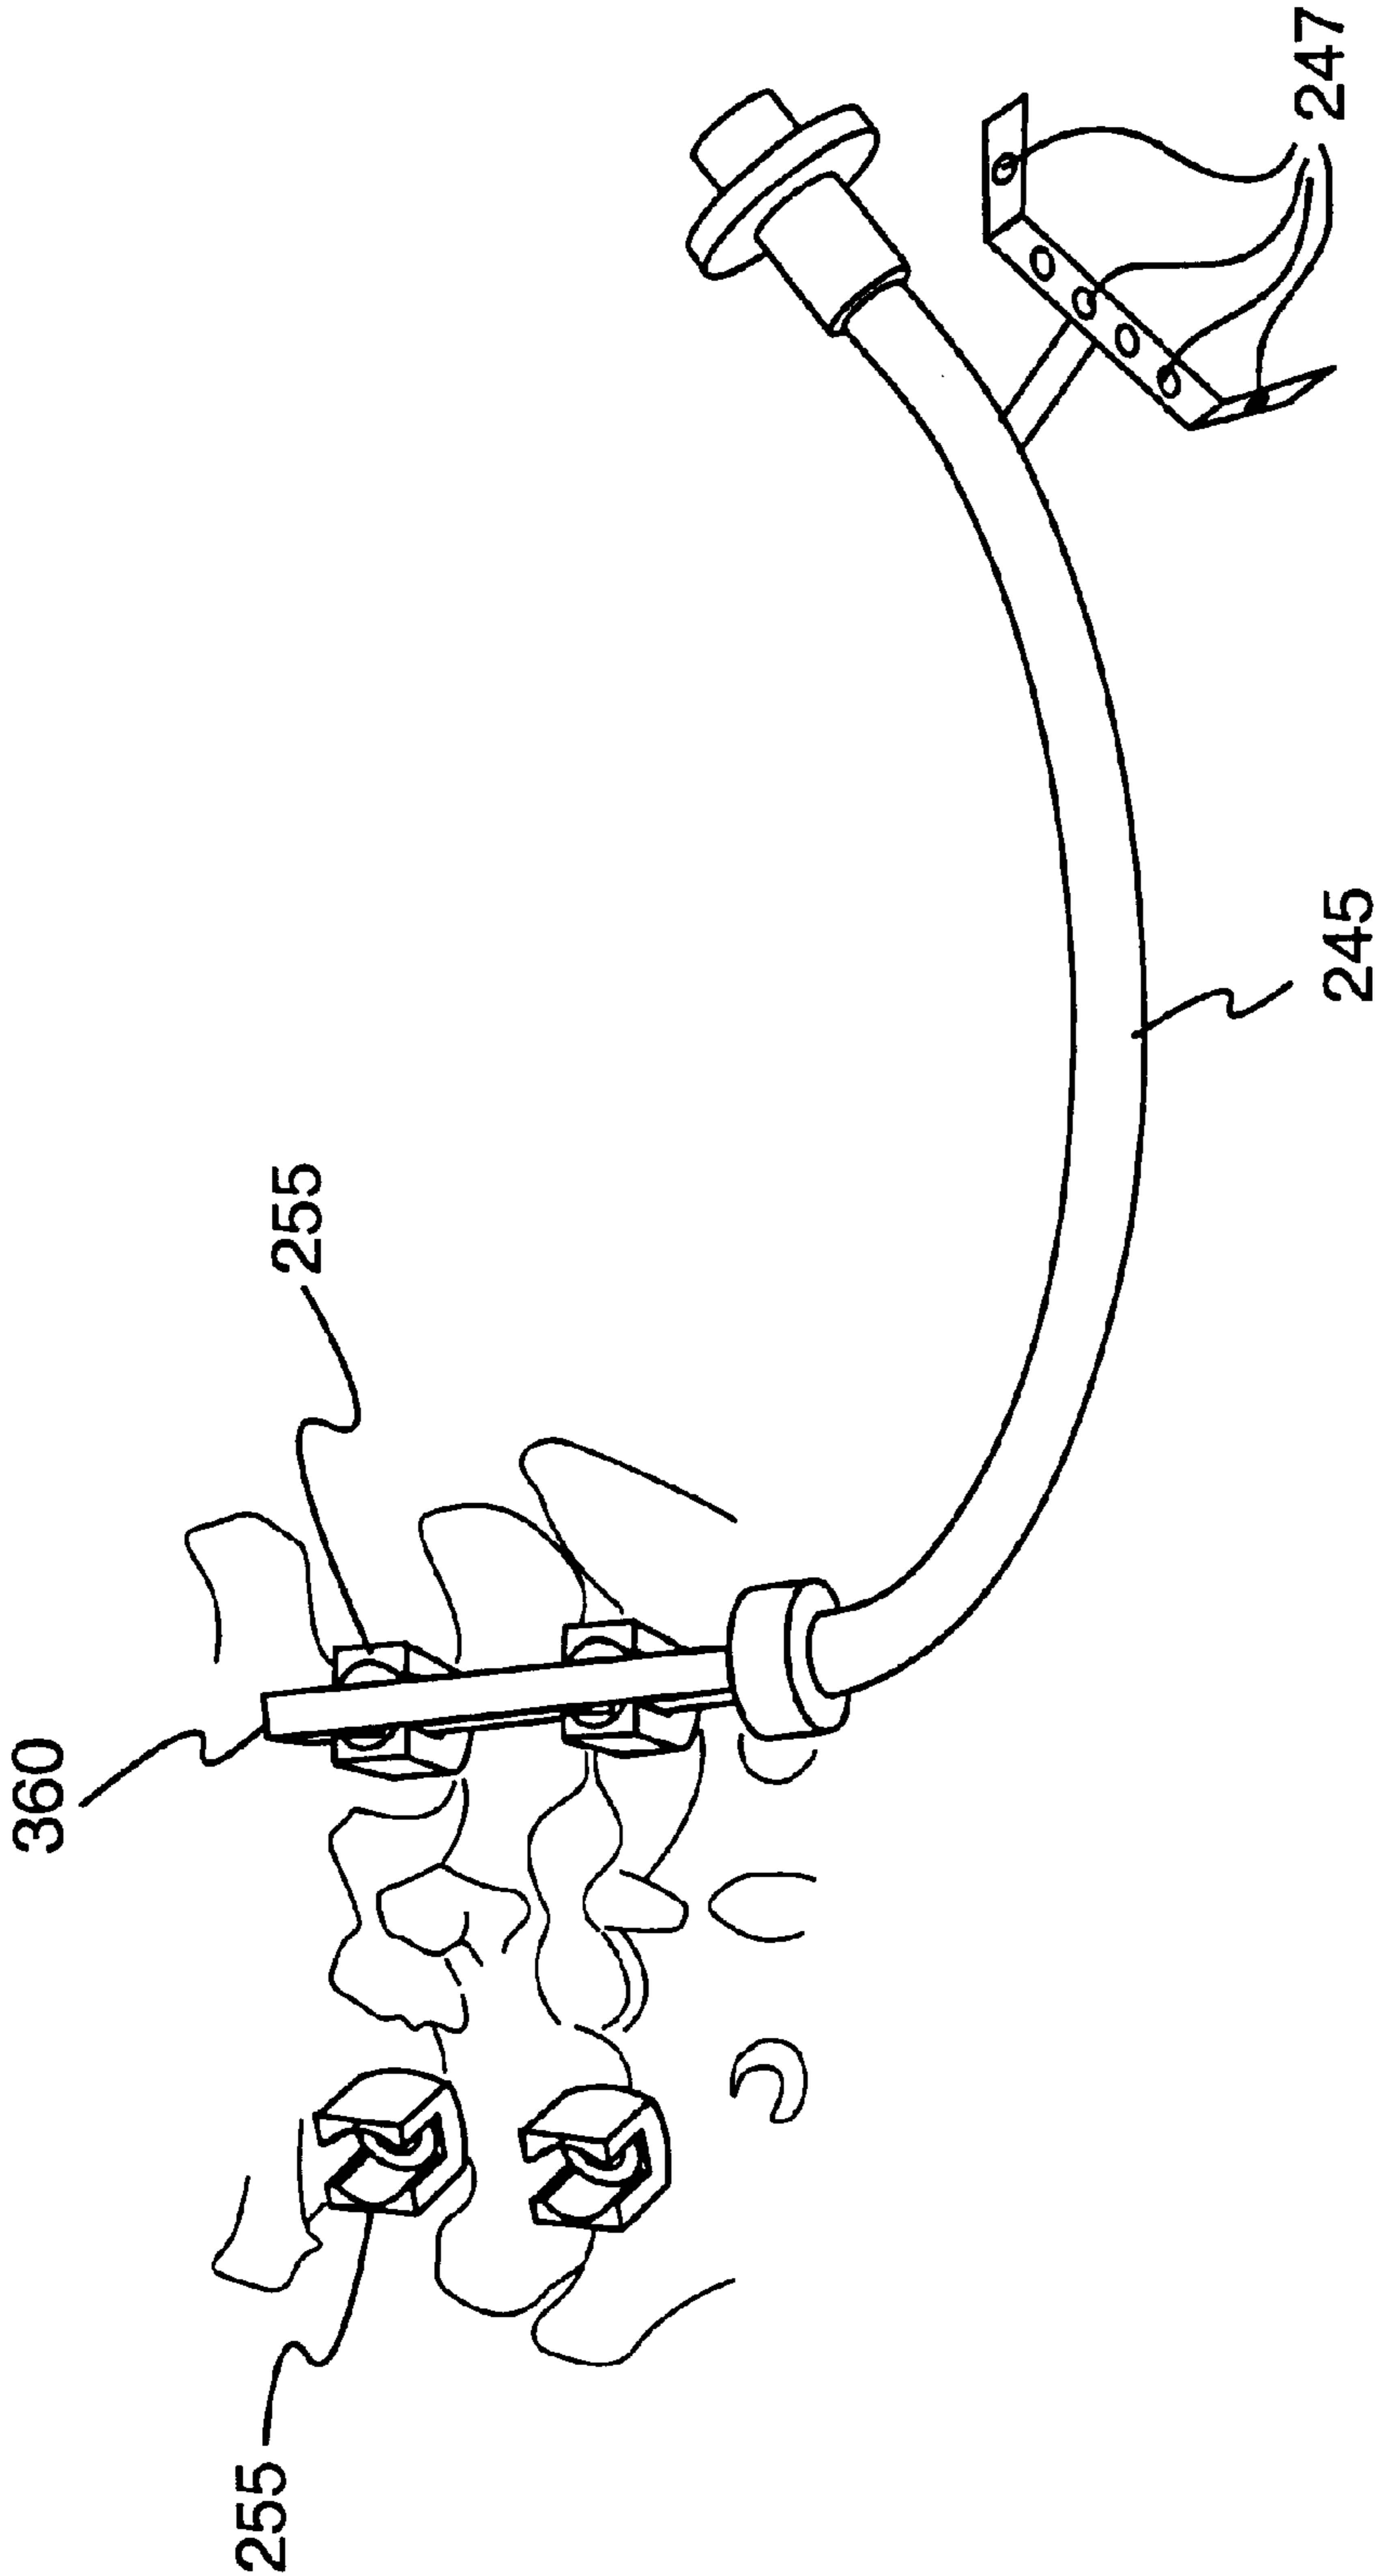


FIG. 9

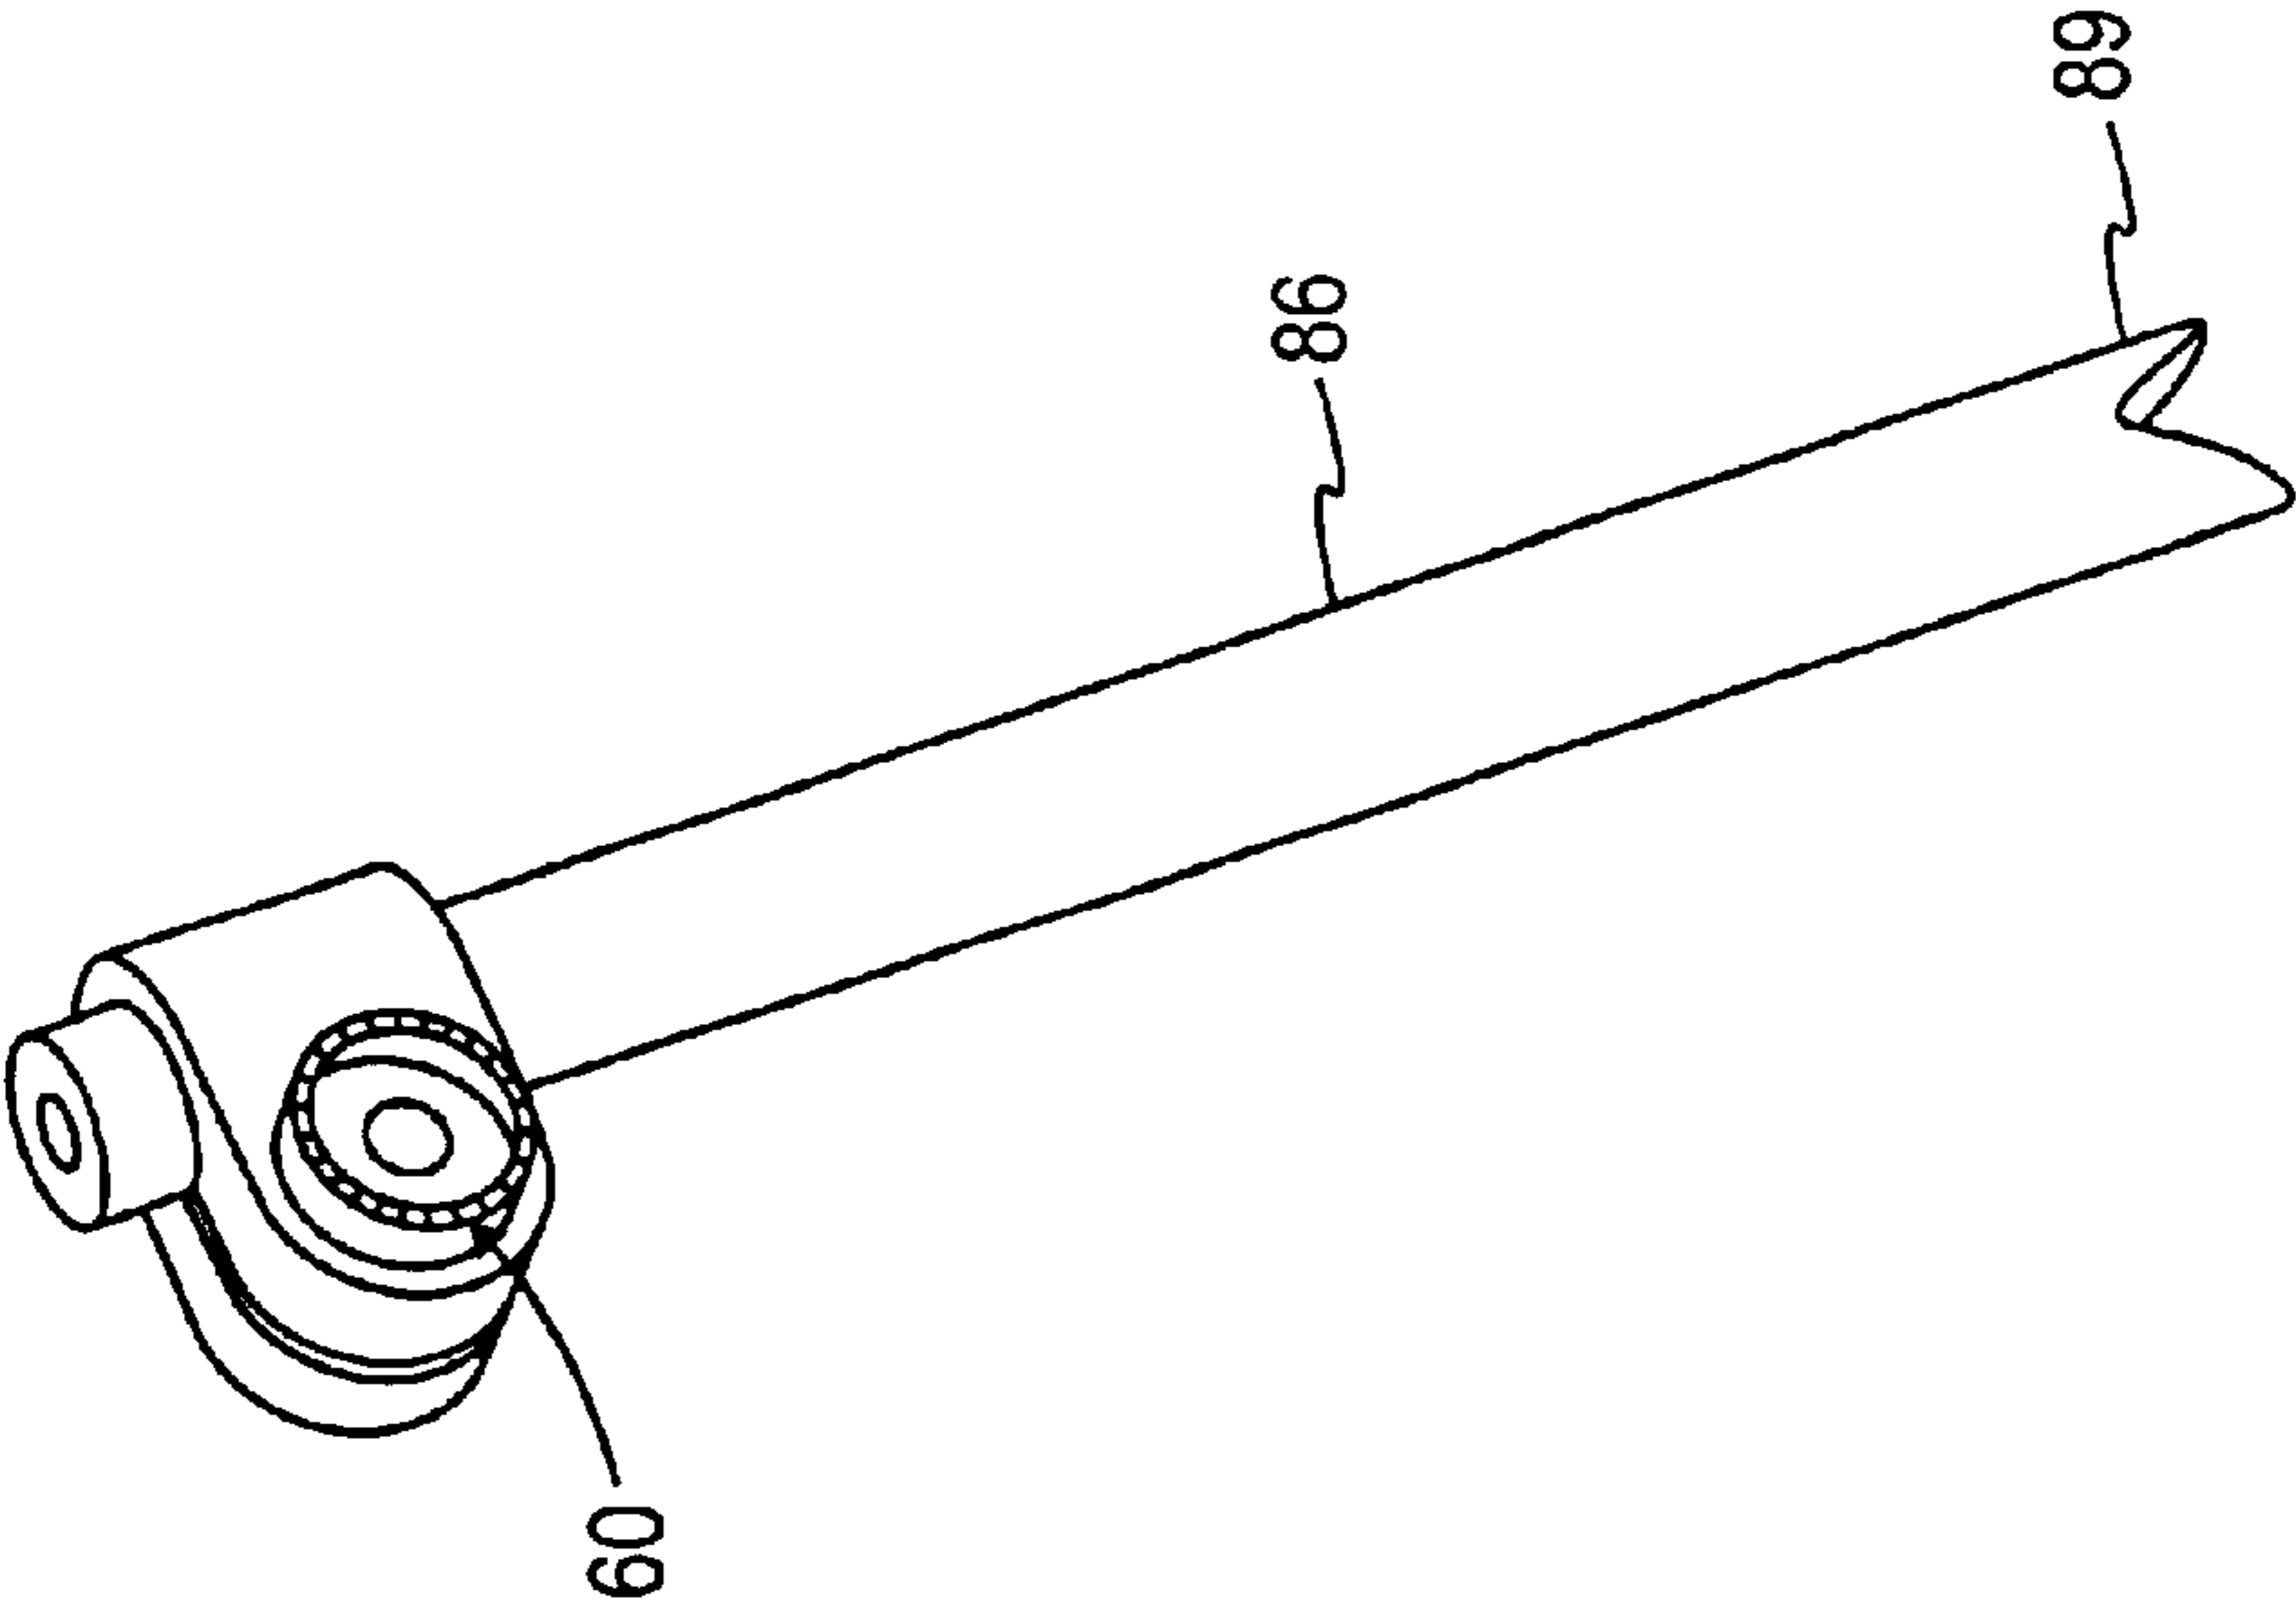


FIG. 10

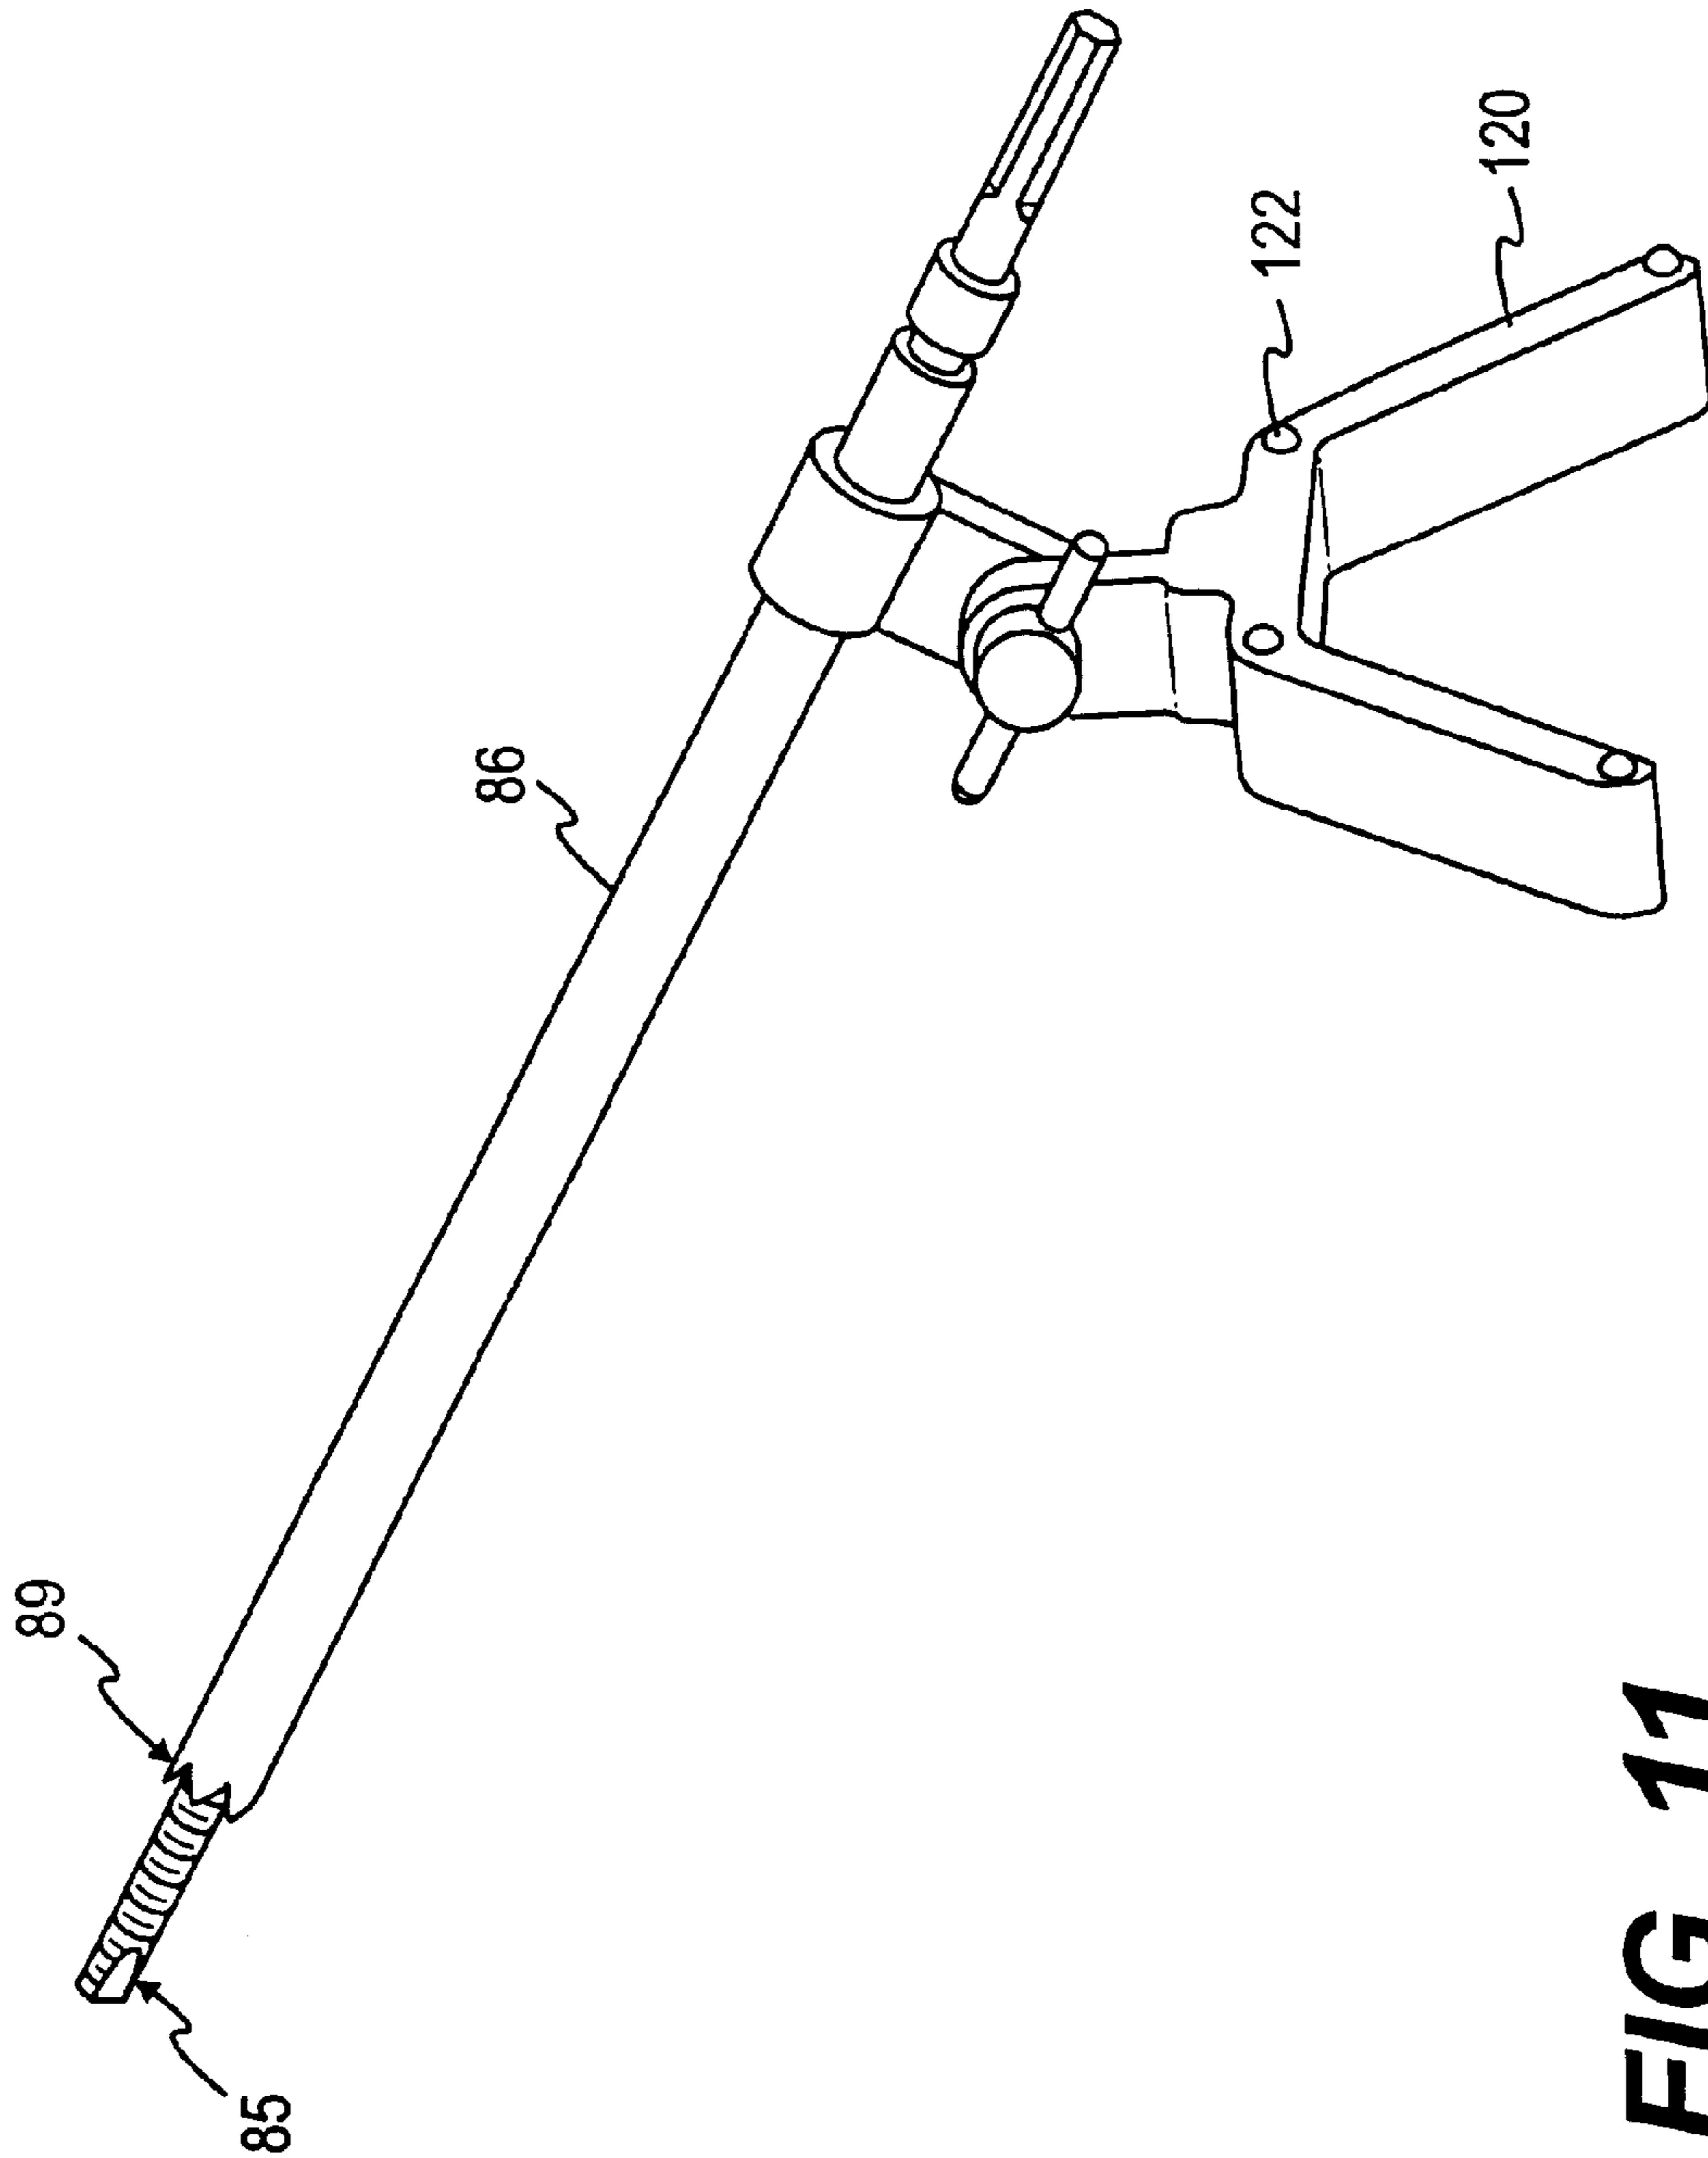


FIG. 11

FIG. 12


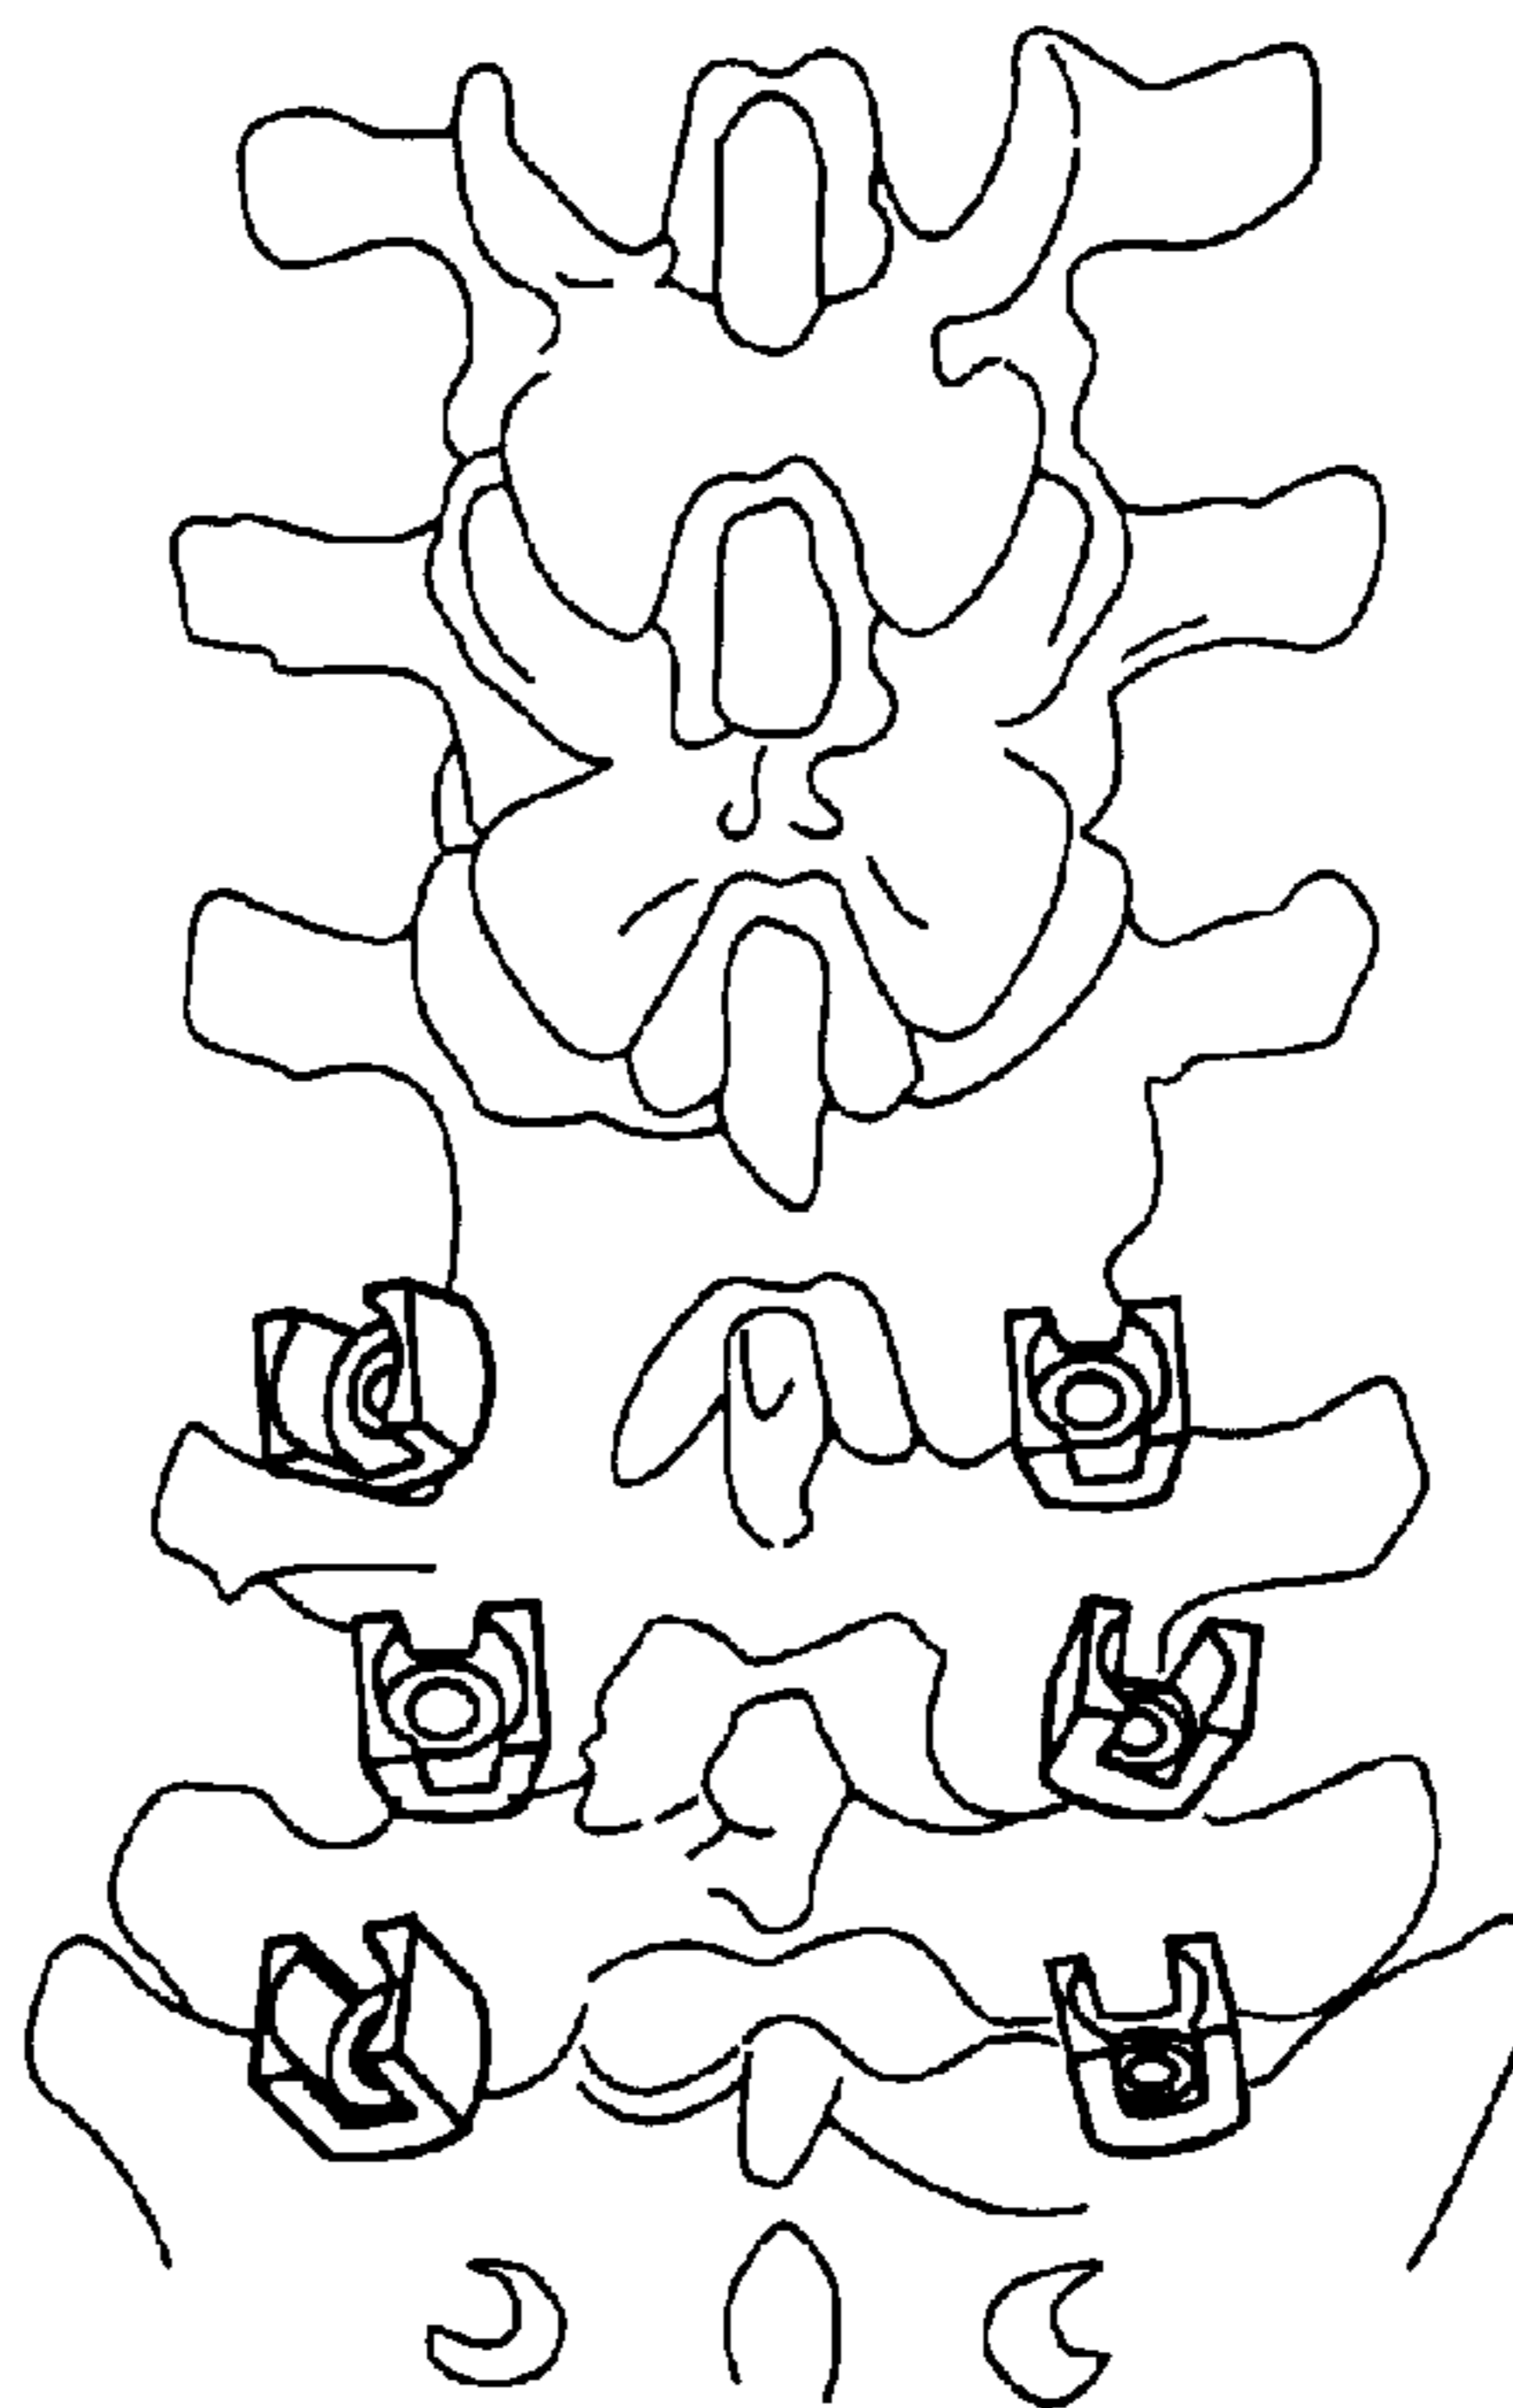


FIG. 13

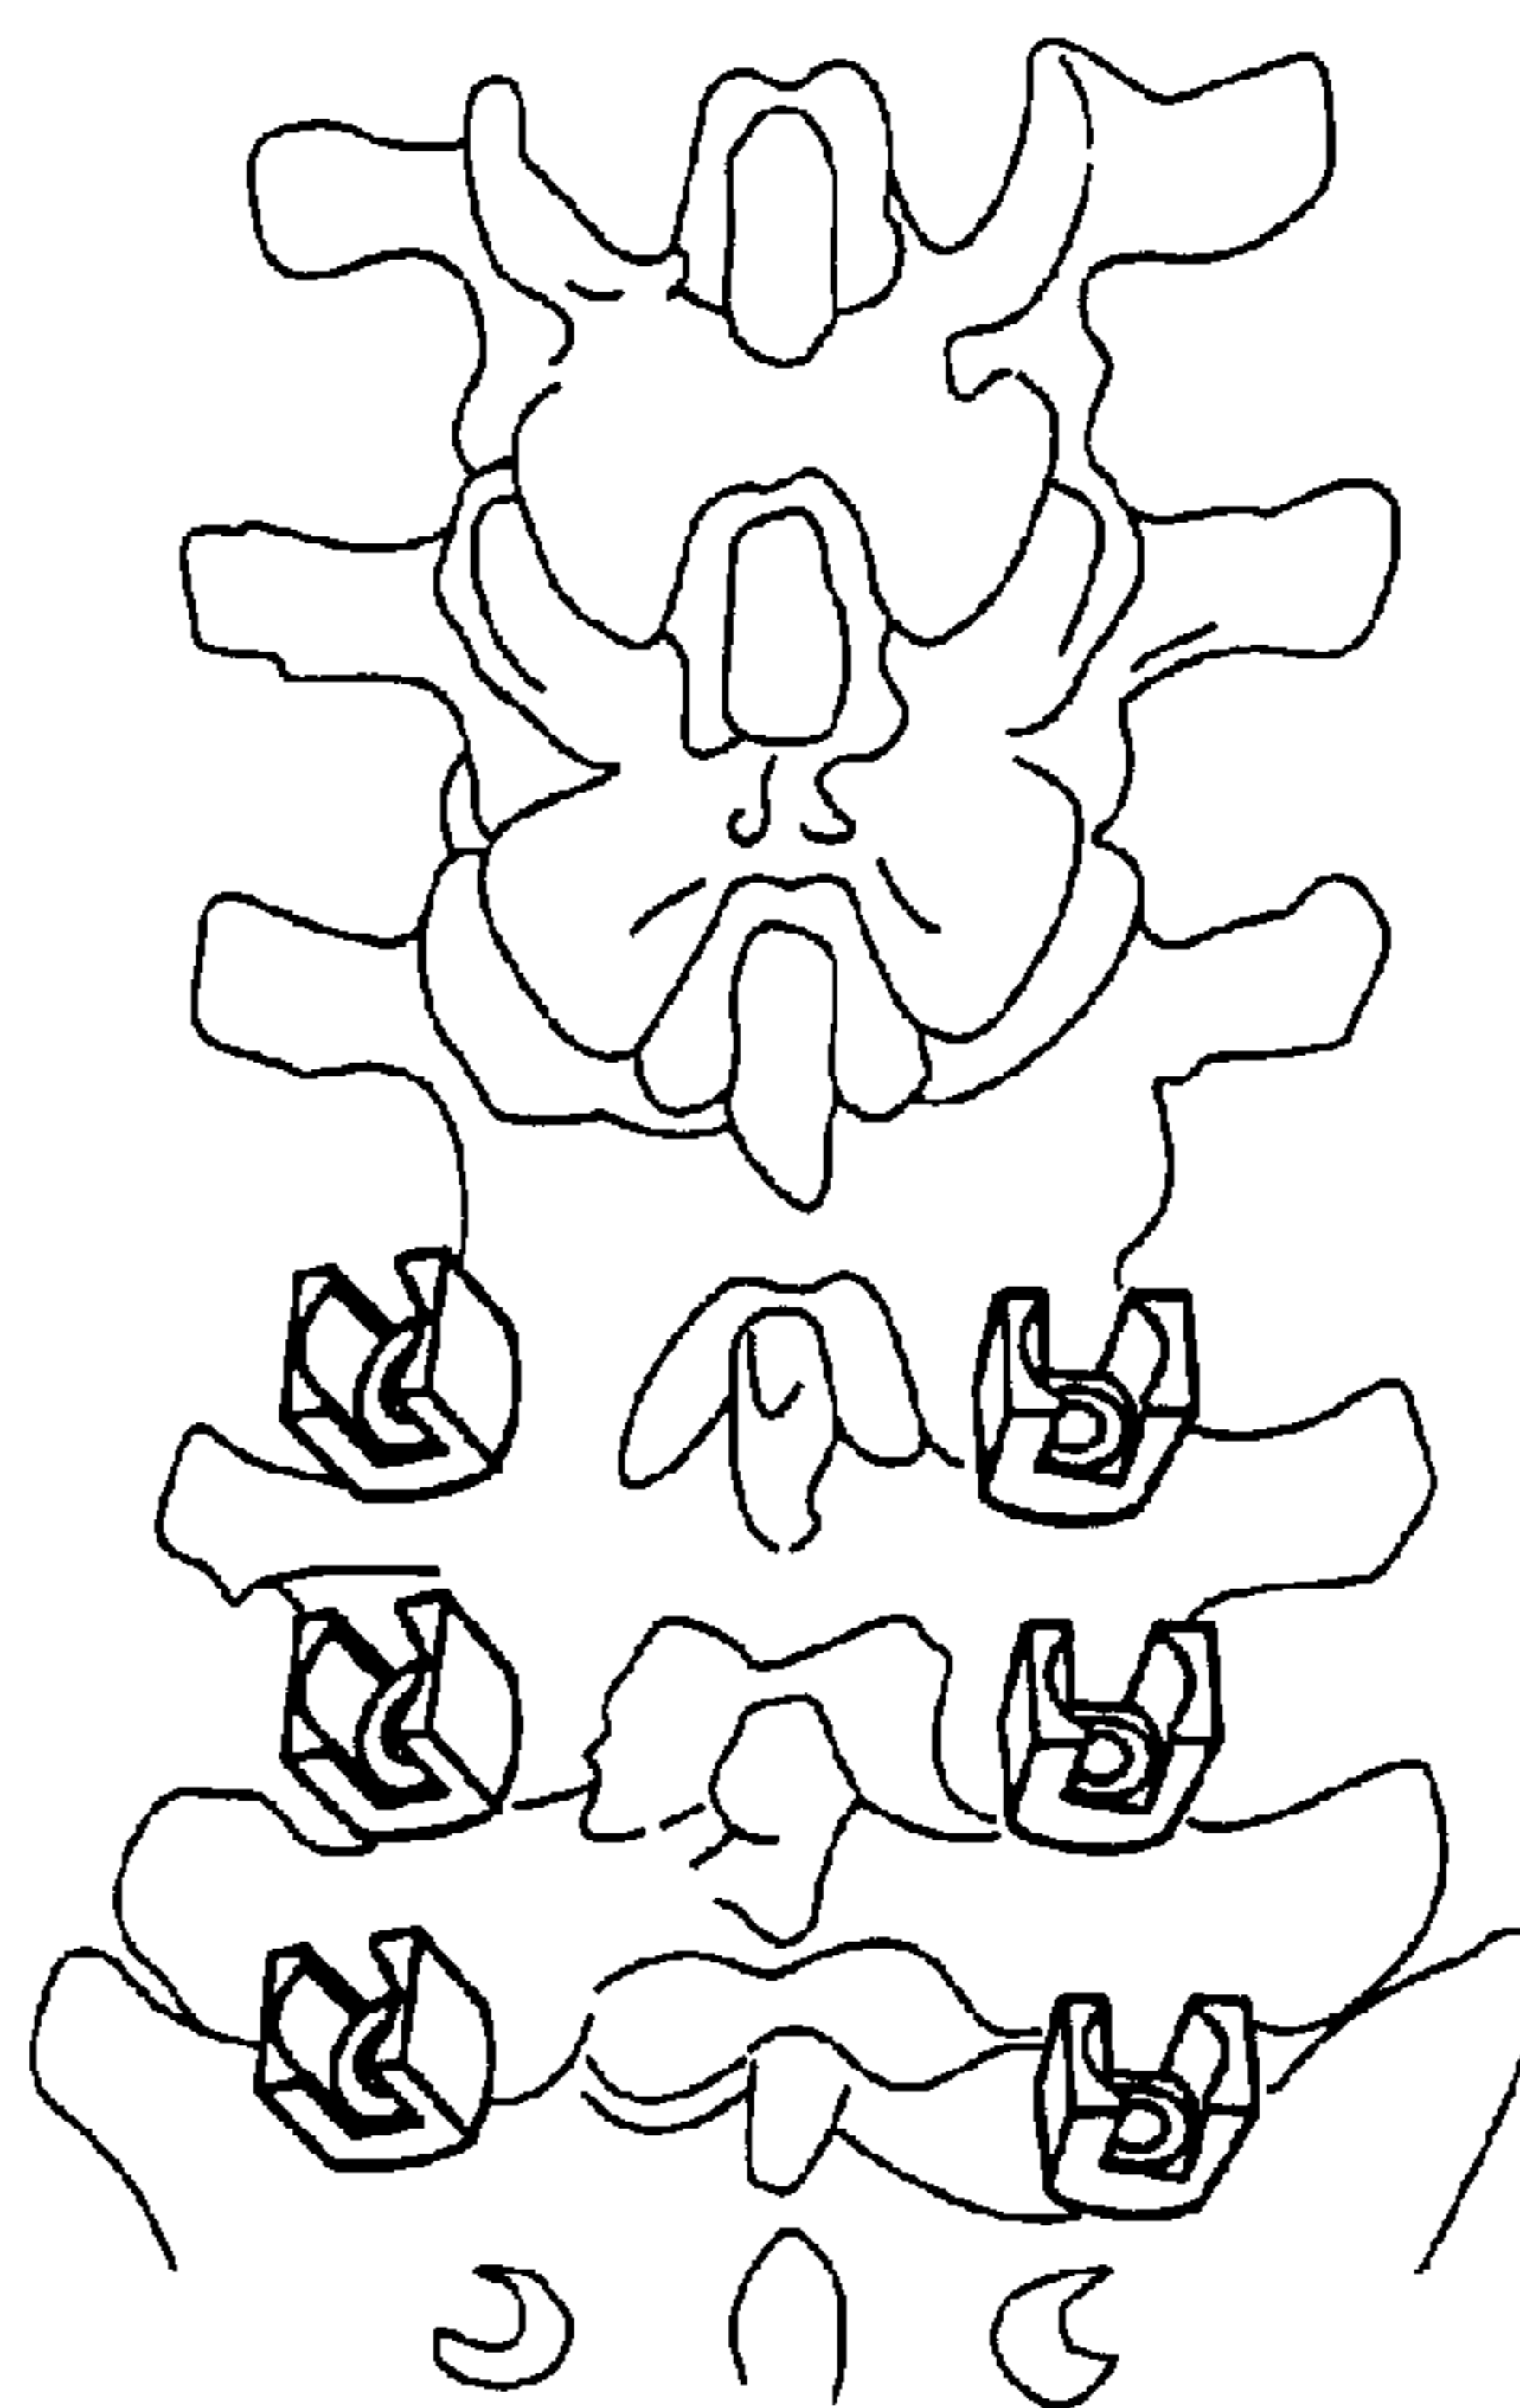

**PERCUTANEOUS REGISTRATION
APPARATUS AND METHOD FOR USE IN
COMPUTER-ASSISTED SURGICAL
NAVIGATION**

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue.

*CROSS-REFERENCE TO RELATED
APPLICATIONS*

[The present invention claims rights under 35 U.S.C. §119 on provisional application No. 60/059,915, filed on Sep. 24, 1997, and entitled "Percutaneous Registration Apparatus and Method for Use in Computer-Assisted Surgical Navigation."]
This application is a reissue of U.S. Pat. No. 6,226,548 issued on May 1, 2001 and also claims benefit under 35 U.S.C. §120 as a continuation of U.S. patent application Ser. No. 11/451,594 filed on Jun. 12, 2006, now U.S. Pat. No. Re. 42,194; which also claims benefit under 35 U.S.C. §120 as a continuation of U.S. patent application Ser. No. 10/423,332 filed on Apr. 24, 2003, now U.S. Pat. No. Re. 39,133; which is also a reissue of U.S. Pat. No. 6,226,548 issued on May 1, 2001; which claims rights under 35 U.S.C. §119 of provisional application No. 60/059,915, filed on Sep. 24, 1997.

This application also claims benefit under 35 U.S.C. §120 as a continuation of U.S. patent application Ser. No. 11/451,595 filed on Jun. 12, 2006, now U.S. Pat. No. Re. 42,226; which also claims benefit under 35 U.S.C. §120 as a continuation of U.S. patent application Ser. No. 10/423,332 filed on Apr. 24, 2003, now U.S. Pat. No. Re. 39,133; which is a reissue of U.S. Pat. No. 6,226,548 issued on May 1, 2001; which claims rights under 35 U.S.C. §119 of provisional application No. 60/059,915, filed on Sep. 24, 1997.

FIELD OF THE INVENTION

The present invention relates generally to guiding, directing, or navigating instruments or implants in a body percutaneously, in conjunction with systems that use and generate images during medical and surgical procedures, which images assist in executing the procedures and indicate the relative position of various body parts, surgical implants, and instruments. In particular the invention relates to apparatus and minimally invasive procedures for navigating instruments and providing surgical implants percutaneously in the spine, for example, to stabilize the spine, correct deformity, or enhance fusion in conjunction with a surgical navigation system for generating images during medical and surgical procedures.

BACKGROUND OF THE INVENTION

Typically, spinal surgical procedures used, for example, to provide stabilization, fusion, or to correct deformities, require large incisions and substantial exposure of the spinal areas to permit the placement of surgical implants such as, for example, various forms of screws or hooks linked by rods, wires, or plates into portions of the spine. This standard procedure is invasive and can result in trauma, blood loss, and post operative pain. Alternatively, fluoroscopes have been used to assist in placing screws beneath the skin. In this alternative procedure at least four incisions must be made in the patient's back for inserting rods or wires through previ-

ously inserted screws. However, this technique can be difficult in that fluoroscopes only provide two-dimensional images and require the surgeon to rotate the fluoroscope frequently in order to get a mental image of the anatomy in three dimensions. Fluoroscopes also generate radiation to which the patient and surgical staff may become over exposed over time. Additionally, the subcutaneous implants required for this procedure may irritate the patient. A lever arm effect can also occur with the screws that are not connected by the rods or wires at the spine. Fluoroscopic screw placement techniques have traditionally used rods or plates that are subcutaneous to connect screws from vertebra to vertebra. This is due in part to the fact that there is no fluoroscopic technique that has been designed which can always adequately place rods or plates at the submuscular region (or adjacent to the vertebrae). These subcutaneous rods or plates may not be well tolerated by the patient. They also may not provide the optimal mechanical support to the spine because the moment arm of the construct can be increased, thereby translating higher loads and stresses through the construct.

A number of different types of surgical navigation systems have been described that include indications of the positions of medical instruments and patient anatomy used in medical or surgical procedures. For example, U.S. Pat. No. 5,383,454 to Bucholz; PCT Application No. PCT/US94/04530 (Publication No. WO 94/24933) to Bucholz; and PCT Application No. PCT/US95/12894 (Publication No. WO 96/11624) to Bucholz et al., the entire disclosures of which are incorporated herein by reference, disclose systems for use during a medical or surgical procedure using scans generated by a scanner prior to the procedure. Surgical navigation systems typically include tracking means such as, for example, an LED array on the body part, LED emitters on the medical instruments, a digitizer to track the positions of the body part and the instruments, and a display for the position of an instrument used in a medical procedure relative to an image of a body part.

Bucholz et al. WO 96/11624 is of particular interest, in that it identifies special issues associated with surgical navigation in the spine, where there are multiple vertebral bodies that can move with respect to each other. Bucholz et al. describes a procedure for operating on the spine during an open process where, after imaging, the spinous process reference points may move with respect to each other. It also discloses a procedure for modifying and repositioning the image data set to match the actual position of the anatomical elements. When there is an opportunity for anatomical movement, such movement degrades the fidelity of the pre-procedural images in depicting the intra-procedural anatomy. Therefore, additional innovations are desirable to bring image guidance to the parts of the body experiencing anatomical movement.

Furthermore, spinal surgical procedures are typically highly invasive. There is, thus, a need for more minimally invasive techniques for performing these spinal procedures, such as biopsy, spinal fixation, endoscopy, spinal implant insertion, fusion, and insertion of drug delivery systems, by reducing incision size and amount. One such way is to use surgical navigation equipment to perform procedures percutaneously, that is beneath the skin. To do so by means of surgical navigation also requires apparatus that can indicate the position of the spinal elements, such as, for example the vertebrae, involved in the procedure relative to the instruments and implants being inserted beneath the patient's skin and into the patient's spine. Additionally, because the spinal elements naturally move relative to each other, the user requires the ability to reorient these spinal elements to align with earlier scanned images stored in the surgical navigation

system computer, to assure the correct location of those elements relative to the instruments and implants being applied or inserted percutaneously.

In light of the foregoing, there is a need in the art for apparatus and minimally invasive procedures for percutaneous placement of surgical implants and instruments in the spine, reducing the size and amount of incisions and utilizing surgical navigation techniques.

SUMMARY OF THE INVENTION

Accordingly, the present invention is directed to apparatus and procedures for percutaneous placement of surgical implants and instruments such as, for example, screws, rods, wires and plates into various body parts using image guided surgery. More specifically, one object of the present invention is directed to apparatus and procedures for the percutaneous placement of surgical implants and instruments into various elements of the spine using image guided surgery.

To achieve these objects and other advantages and in accordance with the purpose of the invention, as embodied and broadly described herein, the invention includes an apparatus for use with a surgical navigation system and comprises an attaching device rigidly connected to a body part, such as the spinous process of a vertebrae, with an identification superstructure rigidly but removably connected to the attaching device. This identification superstructure is a reference arc and fiducial array, which accomplishes the function of identifying the location of the superstructure, and, therefore, the body part to which it is fixed, during imaging by CAT scan or MRI, and later during medical procedures.

In one aspect, the attaching device is a clamp with jaws and sharp teeth for biting into the spinous process.

In another aspect, the fixture is a screw, having a head, wherein the screw is implanted into the spinous process and a relatively rigid wire is attached to the head of the screw and also implanted into the spinous process at an angle to the axis of the screw to prevent the screw from rotating in either direction.

In another aspect, the superstructure includes a central post, and a fiducial array and a reference arc rigidly but removably attached to the central post. The fiducial array is composed of image-compatible materials, and includes fiducials for providing a reference point, indicating the position of the array, which are rigidly attached to the fiducial array, composed of, for example titanium or aluminum spheres. The reference arc includes emitters, such as, for example Light Emitting Diodes ("LEDs"), passive reflective spheres, or other tracking means such as acoustic, magnetic, electromagnetic, radiologic, or micropulsed radar, for indicating the location of the reference arc and, thus, the body part it is attached to, during medical procedures.

In addition, the invention further comprises a method for monitoring the location of an instrument, surgical implants and the various portions of the body, for example, vertebrae, to be operated on in a surgical navigation system comprising the steps of: attaching a fixture to the spinous process; attaching a superstructure including a fiducial array with fiducials and a reference arc to the fixture; scanning the patient using CT, MRI or some other three-dimensional method, with fiducial array rigidly fixed to patient to identify it on the scanned image; and thereafter, in an operating room, using image-guided technology, touching an image-guided surgical pointer or other instrument to one or more of the fiducials on the fiducial array to register the location of the spinal element fixed to the array and emitting an audio, visual, radiologic, magnetic or other detectable signal from the reference arc to

an instrument such as, for example, a digitizer or other position-sensing unit, to indicate changes in position of the spinal element during a surgical procedure, and performing a surgical or medical procedure percutaneously on the patient using instruments and implants locatable relative to spinal elements in a known position in the surgical navigation system.

In another aspect, the method includes inserting screws or rigid wires in spinal elements in the area involved in the anticipated surgical procedure before scanning the patient, and after scanning the patient and bringing the patient to the operating area, touching an image-guided or tracked surgical pointer to these screws and wires attached to the vertebrae to positively register their location in the surgical navigation computer, and manipulating either the patient's spine or the image to align the actual position of the spinal elements with the scanned image.

In another aspect, the method includes percutaneously implanting screws into spinal elements, which screws are located using image guided surgical navigation techniques, and further manipulating the orientation of the screw heads percutaneously using a head-positioning probe containing an emitter, that can communicate to the surgical navigation computer the orientation of the screw heads and position them, by use of a specially designed head-positioning tool with an end portion that mates with the heads of the screws and can rotate those screw heads to receive a rod, wire, plate, or other connecting implant. If a rod is being inserted into the screw heads for example, the method further includes tracking the location and position of the rod, percutaneously using a rod inserter having one or more emitters communicating the location and orientation of the rod to the surgical navigation computer.

The objects of the invention are to provide a user, such as a surgeon, with the system and method to track an instrument and surgical implants used in conjunction with a surgical navigation system in such a manner to operate percutaneously on a patient's body parts, such as spinal vertebrae which can move relative to each other.

It is a further object of this invention to provide a system and method to simply and yet positively indicate to the user a change in position of body parts, such as spinal vertebrae segments, from that identified in a stored image scan, such as from an MRI or CAT scan, and provide a method to realign those body parts to correspond with a previously stored image or the image to correspond with the actual current position of the body parts.

It is a further object of this invention to provide a system or method for allowing a fiducial array or reference arc that is removable from a location rigidly fixed to a body part and replaceable back in that precise location.

It is another object of this invention to provide a system and method for positively generating a display of instruments and surgical implants, such as, for example screws and rods, placed percutaneously in a patient using image-guided surgical methods and techniques.

It is another object of this invention for a percutaneous reference array and fiducial array, as described in this application, to be used to register and track the position of the vertebrae for the purposes of targeting a radiation dose to a diseased portion of said vertebrae using a traditional radio-surgical technique.

Additional objects and advantages of the invention will be set forth in part in the description which follows, and in part will be obvious from the description, or may be learned by practice of the invention. The objects and advantages of the invention will be realized and attained by means of the elements and combinations particularly pointed out in this description.

5

It is to be understood that both the foregoing general description and the following detailed description are exemplary and explanatory only and are not restrictive of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate one embodiment of the invention and together with the description, serve to explain the principles of the invention.

FIG. 1 is a schematic diagram of one preferred embodiment of a superstructure for use in the current invention, including a reference arc, center post and fiducial array and rigid Kirschner wires ("K wires") and screws placed in the spine for use with a surgical navigation system for percutaneous spinal surgical procedures.

FIG. 1A is an enlarged view of the superstructure depicted in FIG. 1 engaging a vertebra by a clamp and also K wires implanted in adjacent vertebrae in the superior and inferior positions of the spinous process.

FIG. 2 is a diagram of the preferred embodiment of a clamp fixture for rigid connection to the spinous process of a single vertebrae with an H-shaped fiducial array attached to a center post rigidly attached to the clamp and a mating connector at the tip of the post for mating with a reference array, and a reference array for use in the current invention.

FIG. 2A is a side view of FIG. 2. FIG. 2B is another side view of FIG. 2.

FIG. 2C is a top view of FIG. 2.

FIG. 2D is an exploded view of FIG. 2 without the reference arc.

FIG. 2E is an exploded view of the interface of the center post and clamp of FIG. 2.

FIG. 3 is a diagram of a W-Shaped fiducial array mounted to a central post with generally spherical fiducials attached to the array, for mounting to a single vertebrae.

FIG. 3A is a side view of FIG. 3.

FIG. 3B is another side view of FIG. 3.

FIG. 3C is a top view of FIG. 3.

FIG. 4 is a diagram of a reference arc and fiducial attached to a center post for use in the current invention in mounting to a single vertebrae.

FIG. 4A is a side view of FIG. 4.

FIG. 4B is a back view of FIG. 4.

FIG. 4C is a top view of FIG. 4.

FIG. 4D is an expanded view of FIG. 4.

FIG. 4E is an expanded side view of FIG. 4.

FIG. 4F is an expanded view of the array foot and shoe of FIG. 4E.

FIG. 5 is a diagram of an alternative embodiment of a fixture for use in the current invention using a cannulated screw for insertion into a vertebrae, with Kirschner wire mounted on a central post and including an alternate embodiment of a fiducial array and reference arc combined on a single structure.

FIG. 6 is a side view of the screw and Kirschner wire fixture of FIG. 5 implanted in a spinous process of a vertebrae.

FIG. 7 is a diagram of a screw-head positioning probe and multi-axial screw for insertion into a single vertebrae.

FIG. 7A is a diagram of the screw of FIG. 7.

FIG. 8 is a diagram of a head positioning probe, multi-axial screw and spinal segment.

FIG. 9 is a diagram of a rod inserter with an LED.

FIG. 10 is a diagram of an alternative embodiment of the invention depicting a cannulated tube and attachment for holding a reference arc.

6

FIG. 11 is a diagram of the cannulated tube of FIG. 10 with a reference arc and screw for attachment to a spinal process.

FIG. 12 is a posterior view of spinal segment and implanted screws before alignment.

FIG. 13 is a posterior view of spinal segment and implanted screws after alignment.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Reference will now be made in detail to the present preferred embodiment of the invention, an example of which is illustrated in the accompanying drawings. Wherever possible, the same reference numbers will be used throughout the drawings to refer to the same or like parts. The following example is intended to be purely exemplary of the invention.

As generally described in PCT/US95/12894, the entire disclosure of which is incorporated herein by reference, a typical surgical navigation system is shown in FIG. 1 adopted to be used in the present invention. A computer assisted image-guided surgery system, indicated generally at 10, generates an image for display on a monitor 106 representing the position of one or more body elements, such as spinal elements fixedly held in a stabilizing frame or device such as a spinal surgery frame 125 commonly used for spinal surgery. A reference arc 120 bearing tracking means or emitters, such as for example LED emitters 122, is mounted to the spinous process by a central post 150. The structures 20 and K wires 260 of FIG. 1 are depicted in more detail in FIG. 1A. The image 105 is generated from an image data set, usually generated preoperatively by a CAT scanner or by MRI for example, which image 105 has reference points for at least one body element, such as a spinal element or vertebrae. The reference points of the particular body element have a fixed spatial relation to the particular body element.

The system includes an apparatus such as a digitizer or other Position Sensing Unit (PSU), such as for example sensor array 110 on support 112 for identifying, during the procedure, the relative position of each of the reference points to be displayed by tracking the position of emitters 122 on arc 120. The system also includes a processor 114 such as a PC or other suitable workstation processor associated with controller 108 for modifying the image data set according to the identified relative position of each of the reference points during the procedure, as identified by digitizer 110. The processor 114 can then, for example, generate an image data set representing the position of the body elements during the procedure for display on monitor 106. A surgical instrument 130, such as a probe or drill or other tool, may be included in the system, which is positioned relative to a body part and similarly tracked by sensor array 110.

In summary, the general operation of a surgical navigating system is well known in the art and need not further be described here.

In accordance with the preferred embodiment of the present invention, with further reference to FIGS. 1 through 6, a registration device 20 is rigidly fixed to a spinal element by, for example, a device such as a bone clamp 30 depicted in FIG. 2. Alternatively, a screw retention device 40, such as the cannulated screw 42 depicted in FIG. 5, and described in more detail below, can be used.

With reference now to FIG. 2, bone clamp 30 is fixedly attached to the spinous process. The clamp 30 includes at least two blades (or jaws) 32 with tips or teeth 34, which are preferably sharp, for driving together and penetrating soft tissue or more dense bone for rigid fixation to the spinous process. The teeth 34 are also preferably sized to accommo-

date the bulb shape of the spinous process. The driving mechanism **40** is, for example, a screw driven into a sleeve **41** and is also preferably located such that it will be accessible in a percutaneous manner. Attached to the clamp **30** is a superstructure **20**. The superstructure **20** includes a central post **150** which is relocatable, that is, it fixes to the clamp **30** in a rigid fashion, for example, as depicted in FIGS. **2D** and **2E**, by being inserted into a V-shaped wedge **44** orienting the post **150** front to back and providing a mating hole **48** along the wedge **44** for insertion of post **150** in a single orientation and also providing fasteners such as screw **43** for tightening to lock the post **150** in place. The post **150** can be removed and reapplied by loosening and tightening screw **43**, such that the original geometry and orientation is maintained. The central post **150** has at its apex a connector **60** with unique geometrical configuration, such as, for example, a starburst, onto which a spinal reference arc **120** of the superstructure **20** attaches. Any such standard reference arc **120** can be used, such as depicted in FIGS. **1A**, **4**, and **11**, preferably including emitters **122**, such as for example LEDs or reflective spheres for providing a positive indication of movement to the surgical navigation system during a procedure.

Also rigidly attached to the central post **150**, as part of the superstructure **20** preferably at a location closer to the skin, or possibly collocated with or also performing the function of the reference arc **120**, is a fiducial array **170**, which can be of various different shapes, such as, for example the H-shaped frame **170** depicted in FIG. **2**, the W-shaped frame **170'** as depicted in FIG. **3**, the U-shaped frame **170''** as depicted in FIG. **4** or the X-shaped frame **120'**, **170'''** depicted in FIG. **5** (depicting a structure that is both a fiducial array and a reference arc). As depicted in FIGS. **2** and **3**, this array can include fiducial points **29** or spheres **17**, rigidly attached to fiducial array **170**, **170'** and is, for example, as depicted in FIG. **3**, substantially in the shape of spheres **17** and of a material detectable by the CAT scan or MRI, preferably titanium or aluminum. This fiducial array such as **170** indicates to the surgical navigation system the location of the bone structure to which the clamp **30** and central post **150** are attached by touching a pointed surgical tracker to fiducial points **29** or a cup-shaped probe to fiducial spheres **17**, thereby indicating the center of the fiducial to the surgical navigation controller **114**. The array **170** and central post **150** are also attached to the clamp **30**, as described above, in such a way that they can be removed and replaced in the same geometric orientation and location, for example, by means of a uniquely shaped interface, for example, a triangle, or a single unique shape or a combination of unique angles or pins with the clamp **30** such that the post **150** can only be reinserted the same way it was removed.

Additionally, the fiducial array **170**, can be located at various heights on the post **150** to accommodate variations in patient tissue depth and size, preferably as close to the patient's body as possible, and then fixed at that specific height by the use of pins or indents matched to holes **19** (shown in FIG. **2**) in the central post **150** or by placing the rods **39** of H-shaped array **170** in different holes **31**. The fiducial array **170** also has, for example, divots **29** (shown in FIG. **2**) shaped to interface with an instrument such as a surgical pointer **130** which can touch that divot **29** to register the location of the divot **29** and, thus, the location of the fiducial array **170** and likewise the spinal element in the surgical navigation system. Multiple divots can be registered to further increase accuracy of the registration system. In one preferred embodiment of the array, the fiducials **17** or **29** can be mounted in a manner such that they can be adjusted, for example by mounting them on a rotatable or collapsible arm

66 (as depicted in FIG. **3**) that pivots and folds together, to get the maximum distance between fiducials while not dramatically increasing the field of view required at the time of scanning.

Alternatively, rather than using clamp **30**, a screw **42** and rigid wire **45** attachment, as depicted in FIGS. **5** and **6**, may be used to rigidly attach the central post of the superstructure **20** to a body element, such as, for example, a vertebrae. As depicted in FIG. **6**, screw **42** is screwed into the spinal process of spinal element **100**. A rigid wire **45**, post, or other sufficiently rigid fastener such as for example a Kirschner wire (K-wire), is inserted through the cannulation in the center of post **150** and the screw **42** or is otherwise fixed to the screw **42**, and exits the tip of the screw **42** at some angle, and is also implanted into the spinal element **100** to prevent the screw **42** from rotating in either direction.

Another embodiment for preventing the superstructure **20** from rotating as depicted in FIGS. **10** and **11** includes the insertion of a screw **85** through a cannulated tube **86** which has teeth **89** in the end (or V-shaped end) that would bite into the tip of the spinous process, preventing rotation.

Having described the preferred embodiment of this apparatus of the present system, the method of using this apparatus to practice the invention of registering a single vertebrae will now be discussed. The operation of a surgical navigating system is generally well known and is described in PCT/US95/12894. In the preferred method of operation, clamp **30** of FIG. **2** or screw **42** and K-Wire **45** of FIG. **5** are implanted percutaneously through a small incision in the skin and rigidly attached to the spinal process. This attachment occurs with the clamp **30**, by driving the blades **32** of the clamp **30** together to hold the spinous process rigidly. The central post **150** is then rigidly fixed to the clamp **30** or screw **42** and the fiducial array **170** is rigidly fixed to the central post **150**. The patient is then scanned and imaged with a CAT scan or MRI with a field of view sufficiently large to display the spinal anatomy and the clamp **30** or screw **42** and the fiducial array **170**. This scan is loaded into the surgical navigation system processor **104**.

After scanning the patient, the array **120** and post **150** can be removed from the patient, while leaving in place the rigidly connected clamp **30** or screw **42**. For example, as depicted in FIGS. **4D** and **4E**, a foot **55** located below array **170''** engages with shoe **56** and rigidly connected by screws **57** and **58**. Before the surgical procedure, the post **150**, array **120** and other remaining portions of the superstructure **20**, once removed, may be sterilized. The patient is then moved to the operating room or similar facility from, for example, the scanning room.

Once in the operating room, the patient may be positioned in an apparatus, such as, for example, a spinal surgery frame **125** to help keep the spinal elements in a particular position and relatively motionless. The superstructure **20** is then replaced on the clamp **30** or screw **42** in a precise manner to the same relative position to the spinal elements as it was in the earlier CAT scan or MRI imaging. The reference arc **120** is fixed to the starburst or other interface connector **60** on the central post **150** which is fixed to the clamp **30** or screw **42**. The operator, for example a surgeon, then touches an instrument with a tracking emitter such as a surgical pointer **130** with emitters **195** to the divots **29** on the fiducial array **170** to register the location of the array **170** and, thus, because the spinal process is fixed to the fiducial array **170**, the location of the spinal element is also registered in the surgical navigation system.

Once the superstructure **20** is placed back on the patient, any instrument **130** fitted with tracking emitters thereon such

as, for example, a drill or screw driver, can be tracked in space relative to the spine in the surgical navigation system without further surgical exposure of the spine. The position of the instrument **130** is determined by the user stepping on a foot pedal **116** to begin tracking the emitter array **190**. The emitters **195** generate infrared signals to be picked up by camera digitizer array **110** and triangulated to determine the position of the instrument **130**. Additionally, other methods may be employed to track reference arcs, pointer probes, and other tracked instruments, such as with reflective spheres, or sound or magnetic emitters, instead of LED's. For example, reflective spheres can reflect infrared light that is emitted from the camera array **110** back to the camera array **110**. The relative position of the body part, such as the spinal process is determined in a similar manner, through the use of similar emitters **122** mounted on the reference frame **120** in mechanical communication with the spinal segment. As is well known in this art and described generally in PCT/US95/12894, based upon the relative position of the spinal segment and the instrument **130** (such as by touching a known reference point) the computer would illustrate a preoperative scan—such as the proper CAT scan slice—on the screen of monitor **106** which would indicate the position of the tool **130** and the spinal segment for the area of the spine involved in the medical procedure.

For better access by the operator of various areas near the central post **150**, the fiducial array **170** can be removed from the central post **150**, by, for example, loosening screw **42** and sliding the array **170** off post **150**, leaving the reference arc **120** in place or replacing it after removal of array **170**. By leaving the reference arc **120** in place, the registration of the location of the spinal process is maintained. Additionally, the central post **150**, reference arc **120**, and fiducial array **170** can be removed after the spinal element has been registered leaving only the clamp **30** or screw **42** in place. The entire surgical field can then be sterilized and a sterile post **150** and reference arc **170** fixed to the clamp **30** or screw **42** with the registration maintained.

This surgical navigation system, with spinal element registration maintained, can then be used, for example, to place necessary and desired screws, rods, hooks, plates, wires, and other surgical instruments and implants percutaneously, using image-guided technology. Once the location of the spinal element **100** involved in the procedure is registered, by the process described above, in relation to the image data set and image **105** projected on monitor **106**, other instruments **130** and surgical implants can be placed under the patient's skin at locations indicated by the instrument **130** relative to the spinal element **100**.

Additionally, the location of other spinal elements, relative to the spinal element **100** containing the fiducial array **170**, can be registered in the surgical navigation system by, for example, inserting additional screws **250**, rigid wires **260**, or other rigid implants or imageable devices into the spinal segment.

For example, as depicted in FIG. 1, and in more detail FIG. 1A, additional screws **250** or rigid and pointed wires **260** are placed in the vertebrae adjacent to the vertebrae containing the clamp **30** and post **150** prior to scanning. On the image **105** provided by monitor **106**, the surgeon can see the clamp **30** or screw **42** and fiducial array **170** and also the additional screws **250**, wires **260** or other imageable devices. When screws **250** or other devices are used, these screws **250** (as depicted in FIG. 7) may contain a divot **256** or other specially shaped interface on the head **255** so that a pointer probe **130** can be used to point to the head **255** of the screw **250** (or wire) and indicate the orientation of the screw **250** or wire **260** to the surgical navigation system by communicating to the control-

ler **114** or by emission from LEDs **195** on probe **130** to digitizer **110**. The image of these additional screws **250** also appear in the scan. Once the patient is then moved to the operating facility, rather than the scanning area, the image of the screw **250** can be compared to the actual position of the screw **250** as indicated by the pointer probe **130** that is touched to the head **255** of the screw **250** or wire **260**. If necessary, the operator can manipulate the position of the patient to move the spinal element and thus the location of the screw **250** or wire **260** to realign the spinal elements with the earlier image of the spine. Alternatively, the operator can manipulate the image to correspond to the current position of the spinal segments.

For additional positioning information, the operator can place additional rigid wires **260** or screws **250** into the vertebrae, for example, located at the superior (toward the patient's head) and inferior (towards the patient's feet) ends of the spinal process to more accurately position those vertebrae relative to the other vertebrae and the image data. Additionally, the wires **260** and screws **250** implanted to provide positioning information can also be equipped with emitters, such as, for example, LEDs, to provide additional information to the surgical navigation system on the location of the wire **260** or screw **250**, and thus the vertebra to which they are affixed.

Alternatively, the patient can be placed in a position stabilizing device, such as a spinal surgery frame **125** or board, before a scan is taken, and then moved to the operating facility for the procedure, maintaining the spine segments in the same position from the time of scanning until the time of surgery. Alternatively, a fluoroscope can be used to reposition the spinal segments relative to the earlier image from the scan. An ultrasound probe can be used to take real-time images of the spinal segment which can be portrayed by monitor **106** overlaid or superimposed on image **105**. Then the operator can manually manipulate the spinal elements and take additional images of these elements with the fluoroscope to, in an iterative fashion, align the spinal elements with the previously scanned image **105**.

Alternatively, a clamp **30** or screw **42** and superstructure **20** can be rigidly fixed to each vertebra involved in the surgical or medical procedure to register the position of each vertebra as explained previously for a single vertebra:

After the spinal elements are registered in the spine, various medical and surgical procedures can be performed on that patient. For example, spinal implants, endoscopes, or biopsy probes can be passed into the spine and procedures such as, for example, spinal fusion, manipulation, or disc removal can be performed percutaneously and facilitated by the surgical navigation image-guiding system. Additionally, a radiation dose can be targeted to a specific region of the vertebrae.

One such procedure facilitated by the apparatus and methods described above is the percutaneous insertion of screws and rods, fixed to different vertebra in a spine to stabilize them. Once screws, for example multiaxial screws **250**, (as depicted in FIG. 12, before manipulation) are implanted through small incisions they can be manipulated by a head-positioning probe **280**. The final position of screws **250** and heads **255** are depicted in FIG. 13. This probe **280**, as depicted in FIG. 7, includes a head **285** that mates in a geometrically unique fashion with the head **255** of the screw **250**. An emitter, such as for example an LED array **380** on the probe **280**, indicates the location and orientation of the screw head **255** to the computer **114** of the surgical navigation system by providing an optical signal received by digitizer **110**. The screw head **255** can then be rotatably manipulated under the patient's skin by the head positioning probe **280** to be prop-

11

erly oriented for the receipt of a rod 360 inserted through the rotating head 255. The operator can then plan a path from the head 255 of each screw 250 to the other screws 250 to be connected. Then, with reference now to FIG. 9, an optically tracked rod inserter 245 also equipped with emitters, such as, for example LEDs 247, can be placed through another small incision to mate with and guide a rod 360 through the holes or slots in the screw heads 245, through and beneath various tissues of the patient, with the rod inserter 245, and, therefore, the rod 360, fixed to the inserter 245, being tracked in the surgical navigation system. The operator can also use the computer 114 to determine the required bending angles of the rod 360. For greater visualization, the geometry of the screws 250 could be loaded into the computer 114 and when the position and orientation of the head 255 is given to the computer 114 via the probe 280, the computer 114 could place this geometry onto the image data and three-dimensional model. The rod 360 geometry could also be loaded into the computer 114 and could be visible and shown in real time on monitor 106 as the operator is placing it in the screw heads 255.

In an alternative procedure, one or more plates and/or one or more wires may be inserted instead of one or more rods 360.

It will be apparent to those skilled in the art that various modifications and variations can be made in the present invention and in construction of this surgical navigation system without departing from the scope or spirit of the invention. Other embodiments of the invention will be apparent to those skilled in the art from consideration of the specification and practice of the invention disclosed herein. It is intended that the specification and examples be considered as exemplary only.

What is claimed is:

[1. An apparatus for facilitating percutaneous placement of surgical instruments into the spine, adapted for use with a surgical navigation system employing an energy-detecting array in communication with a surgical navigation computer to track positions of instruments in three dimensional space relative to a known reference point, said apparatus comprising:

a connector adapted to be rigidly attached to a portion of the spine;

at least one central post connected to said connector;

a position identification structure rigidly and removably connected to said central post at a predetermined position on said central post and adapted to be reconnected at the same said predetermined position, said identification structure being further adapted to allow a patient to be scanned with the structure connected to the central post, said structure including an assembly for communicating positioning information with respect to said assembly to the energy detecting array and surgical navigation computer; and

a connector assembly for said reconnecting of said structure substantially to said predetermined position on said central post.]

[2. The apparatus of claim 1, wherein the connector is a clamp having teeth adapted for biting into a spinous process.]

[3. The apparatus of claim 1, wherein the connector includes an elongated fixture with a central axis and a threaded end adapted to be inserted into the spinous process and a substantially rigid wire connected to the fixture with the central axis of the wire adapted to be implanted into the spinous process at an angle to elongated fixture to prevent the fixture from rotating.]

12

[4. The apparatus of claim 1, wherein said assembly for communication positioning information is a substantially H-shaped frame.]

[5. The apparatus of claim 1, wherein said assembly for communicating positioning information is a substantially W-shaped frame.]

[6. The apparatus of claim 1, wherein said assembly for communicating positioning information is a substantially U-shaped frame.]

[7. The apparatus of claim 1, wherein said assembly for communicating positioning information is a substantially X-shaped frame.]

[8. The apparatus of claim 1, wherein said assembly for communicating positioning information comprises:

a fiducial array for registering the location of a spinal element with rigidly connected fiducials; and

a reference arc for signaling the position of a spinal element, said arc further comprising rigidly connected emitters.]

[9. The apparatus of claim 1, wherein said reference point is on the spine.]

[10. A method for monitoring the location of an instrument, surgical implant and various portions of the body, to be operated on, using a surgical navigation system with a surgical navigation computer and a digitizer array for monitoring the location of instruments in three-dimensional space relative to a known reference point, said method comprising the steps of:

attaching a fixture having a central post to a portion of the spine;

removably attaching an identification structure including a fiducial array and a reference arc to said central post;

providing a scanned three-dimensional image of a patient including said fiducial array rigidly attached to said central post of said fixture, said fixture being rigidly attached to the patient to identify the position of said fixture and said fiducial array on the scanned image;

using an image-guided system, by touching an image guided surgical pointer to one or more fiducials on the fiducial array to register the location of a spinal element fixed to said array; and

emitting a signal from said reference arc to indicate changes in position of the spinal element during a surgical procedure.]

[11. The method of claim 10, further comprising:

performing a surgical procedure percutaneously on a patient using an instrument and implant locatable relative to the spinal element and said structure in known positions identified in the surgical navigation system.]

[12. The method of claim 10, further comprising:

inserting a threaded fixture having a substantially rigid wire into a spinal element; and

touching an image guided pointer to said threaded fixture and wire to positively register the location of said fixture and wire in a surgical navigation computer.]

[13. The method of claim 10, further comprising:

implanting imageable devices into spinal elements to identify the location of the spinal elements in the surgical navigation computer.]

[14. The method of claim 10, further comprising:

implanting imageable devices into a plurality of spinal elements; and

manipulating the patient's spine by viewing the location of the implanted devices, as communicated to the surgical navigation computer by touching an instrument with a tracking emitter to said implanted imageable devices to align the actual position of the spinal elements with the previously scanned image.]

13

[15. The method of claim 10 further comprising:
percutaneously implanting screws into spinal elements;
and

locating the position of said screws using image guided
surgical navigation techniques.]

[16. The method of claim 15 further comprising:
manipulating the orientation of the screw heads percutane-
ously using a head-positioning probe for communicat-
ing location containing an emitter, said probe commu-
nicating to the surgical navigation computer the

orientation of the screw heads; and
using a head positioning tool for manipulating implants
having an end portion that mates with the heads of the
screws and rotating the screws to receive a connecting
implant.]

[17. The method of claim 16 further comprising:
tracking the location and position of the connecting
implant by means of an instrument affixed to the implant
having emitters capable of communicating orientation
and location to the surgical navigation computer.]

[18. A system for use in performing the percutaneous
placement of surgical implants and instruments into the spine
using image guided surgery and a surgical navigation com-
puter and energy detecting array, said system comprising:

means for attaching a fixture to a portion of the spine;

means for communicating position information to the sur-
gical navigation computer and energy detecting array
said means rigidly and removably connected to said
means for attaching a fixture;

means for providing location information of said spinal
portion to the surgical navigation system adapted to be
connected to spinal elements;

means for indicating screw-head position said means elec-
trically connected to the surgical navigation system and
adapted to mate with the head of a screw implanted in
one or more of said spinal elements.]

[19. The system of claim 18 further comprising:
an elongated implant adapted to be inserted into said
implanted screws;

means for indicating the position of said elongated implant
electrically connected to the surgical navigation system
and adapted to mate with the elongated implant.]

[20. The system of claim 18, wherein said implanted
screws have heads and the elongated implant is a rod adapted
to be guided through holes in said implanted screw heads.]

21. An apparatus for use in computer assisted procedures,
comprising:

*a device operable to be connected to a structure and
including:*

*a clamp operable to engage the structure having a first
member and a second member to engage substan-
tially opposite sides of the structure;*

*a member extending from and detachably connected to
the clamp; and*

*at least one of a reference portion operable to be detach-
ably connected to the member or a fiducial member
operable to be connected to the member;*

*wherein the first member of the clamp includes a first arm
and the second member of the clamp includes a second
arm operable to compress the structure therebetween to
hold the device relative to the structure;*

*wherein the reference portion is operable to determine a
location of the structure and the fiducial member is
operable to be registered relative to an image of the
structure.*

22. An apparatus for use in computer assisted procedures,
comprising:

14

*a device operable to be connected to a structure and
including:*

*a clamp operable to engage the structure having a first
member and a second member to engage substan-
tially opposite sides of the structure;*

*a member extending from and connected to the clamp;
and*

*at least one of a reference portion operable to be detach-
ably connected to the member or a fiducial member
operable to be detachably connected to the member;*

a monitor;

a screw or wire positioned in a bone; and

*a pointer operable to touch at least one of the screw or the
wire;*

*wherein the monitor is operable to display an image of at
least one of the screw or the wire and an indication of a
position of at least one of the screw or the wire based on
the pointer touching at least one of the screw or the wire;*

*wherein the reference portion is operable to determine a
location of the structure and the fiducial member is
operable to be registered relative to an image of the
structure.*

23. The apparatus of claim 21, further comprising:
*a fiducial sphere associated with the fiducial member and
imageable with the structure.*

24. The apparatus of claim 21, further comprising:

a connector connected to the member;

*wherein the member extends from a first end to a second
end, where the first end is operable to be connected to the
clamp;*

*wherein the connector is connected near the second end;
wherein the connector is operable to interconnect the ref-
erence portion and the member.*

25. The apparatus of claim 21, wherein the clamp and the
member are configured such that the clamp and the member
can be separated and replaced in the same geometric orien-
tation and location.

26. An apparatus for use in computer assisted procedures,
comprising:

*a device operable to be connected to a structure and
including:*

*a clamp operable to engage the structure having a first
member and a second member to engage substan-
tially opposite sides of the structure;*

*a member extending from and detachably connected to
the clamp; and*

*at least one of a reference portion operable to be detach-
ably connected to the member or a fiducial member
operable to be detachably connected to the member;*

a tool;

*a tracking device fixed to the tool to track the tool relative
to the structure; and*

*a tracking system to track the tracking device and the
reference portion;*

*wherein the reference portion is operable to determine a
location of the structure and the fiducial member is
operable to be registered relative to an image of the
structure.*

27. The apparatus of claim 21, wherein the fiducial portion
includes a plurality of divots operable to be registered to
increase accuracy when compared to a single registered divot
and to be connected simultaneously with the reference por-
tion to the member.

28. The apparatus of claim 27, wherein the fiducial portion
includes an elongated arm member such that each of the
plurality of divots are spaced apart from one another.

15

29. The apparatus of claim 27, wherein the elongated member is collapsible and operable to fold together.

30. An apparatus for use in computer assisted procedures, comprising:

a device operable to be connected to a structure and including:

a clamp operable to engage the structure having a first member and a second member to engage substantially opposite sides of the structure;

a member extending from and connected to the clamp; and

at least one of a reference portion operable to be detachably connected to the member or a fiducial member operable to be detachably connected to the member;

wherein the reference portion is operable to determine a location of the structure and the fiducial member is operable to be registered relative to an image of the structure;

wherein the clamp and the member are configured in a geometric orientation and location;

wherein the at least one of a reference portion is operable to be detachably connected to the member or a fiducial member is operable to be detachably connected to the member with a starburst connector.

31. An apparatus for use in computer assisted procedures, comprising:

a device operable to be connected to a structure and including:

a screw operable to be driven into the structure;

a member extending and detachable from the screw; and

at least one of a reference portion operable to be detachably connected to the member or a fiducial member operable to be detachably connected to the member;

wherein the reference portion is operable to determine a location of the structure and the fiducial member is operable to be registered relative to an image of the structure.

32. The apparatus of claim 31, further comprising:

a fiducial sphere associated with the fiducial member.

33. The apparatus of claim 31, further comprising:

a connector connected to the member;

wherein the member extends from a first end to a second end, wherein one of the first end or the second end of the member is operable to be connected to the screw;

wherein the connector is connected near the second end;

wherein the connector is operable to interconnect the reference portion and the member.

34. The apparatus of claim 33, wherein the connector includes a uniquely shaped interface such that the screw and

16

the member can be separated and replaced in the same geometric orientation and location.

35. The apparatus of claim 34, wherein the uniquely shaped connector is a starburst connector.

36. The apparatus of claim 35, wherein the fiducial member includes a plurality of divots operable to be registered to increase accuracy when compared to a single registered divot and connected to the screw with the connector.

37. The apparatus of claim 36, wherein the fiducial portion includes an elongated arm member such that each of the plurality of divots are spaced apart from one another; wherein the elongated member is collapsible and operable to fold together.

38. A method of registering a physical space defined relative to a subject to an image space of the subject, comprising:

fixing a clamp to a structure of the subject;

fixing a fiducial portion to the clamp with a connector;

acquiring image data of the subject and the fiducial portion connected to the subject;

removing the fiducial portion from the clamp after acquiring the image data;

registering the subject space to the image space of the acquired image data, including:

reattaching the fiducial portion to the clamp in a same geometric orientation and location as during the acquiring the image data;

determining a location of a registration portion of the fiducial portion.

39. The method of claim 38, further comprising: attaching reference arc to the clamp.

40. The method of claim 38, wherein determining a location of a registration portion of the fiducial portion includes determining a location of a plurality of divots on the fiducial portion.

41. The method of claim 40, further comprising: folding the fiducial portion to reduce a volume encompassed by the fiducial portion.

42. The method of claim 40, further comprising:

removing the fiducial portion subsequent to the registering the subject space to the image space and maintaining registration of the subject space to the image space via the attached reference arc.

43. The method of claim 38, wherein the fixing a clamp to a structure of the subject includes moving a first arm and a second arm towards one another to compress the structure therebetween to hold the clamp relative to the structure.

* * * * *