

US00RE46356E

(19) **United States**
(12) **Reissued Patent**
Pellegrino et al.

(10) **Patent Number:** **US RE46,356 E**
(45) **Date of Reissued Patent:** **Apr. 4, 2017**

(54) **METHOD OF TREATING AN
INTRAOSSEOUS NERVE**

(56) **References Cited**

U.S. PATENT DOCUMENTS

- (75) Inventors: **Richard Pellegrino**, Half Moon Bay,
CA (US); **Paula Papineau**,
Bridgewater, MA (US); **John S.
Crombie**, East Hanover, NJ (US);
Samit Patel, San Francisco, CA (US);
Thomas Ryan, Austin, TX (US)
- (73) Assignee: **Relievant Medsystems, Inc.**, Redwood
City, CA (US)
- (21) Appl. No.: **13/541,591**
- (22) Filed: **Jul. 3, 2012**

3,845,771 A	11/1974	Vise
3,920,021 A	11/1975	Hiltebrandt
4,044,774 A	8/1977	Corgin et al.
4,116,198 A	9/1978	Roos
4,312,364 A	1/1982	Convert et al.
4,448,198 A	5/1984	Turner
4,573,448 A	3/1986	Kambin
4,657,017 A	4/1987	Sorochenko
4,679,561 A	7/1987	Doss
4,754,757 A	7/1988	Feucht
4,907,589 A	3/1990	Cosman
4,950,267 A	8/1990	Ishihara et al.
4,959,063 A	9/1990	Kojima

(Continued)

Related U.S. Patent Documents

Reissue of:

- (64) Patent No.: **7,749,218**
Issued: **Jul. 6, 2010**
Appl. No.: **11/123,766**
Filed: **May 6, 2005**

U.S. Applications:

- (62) Division of application No. 10/260,879, filed on Sep.
30, 2002, now Pat. No. 6,907,884.
- (51) **Int. Cl.**
A61B 19/00 (2006.01)
A61B 18/14 (2006.01)
A61B 18/00 (2006.01)
- (52) **U.S. Cl.**
CPC .. **A61B 18/1477** (2013.01); **A61B 2018/0044**
(2013.01); **A61B 2018/00083** (2013.01); **A61B**
2018/00434 (2013.01)
- (58) **Field of Classification Search**
CPC **A61B 18/1477**; **A61B 2018/0044**; **A61B**
2018/00434; **A61B 2018/00083**
USPC **606/41-49**; **607/96**, **98-101**; **128/898**
See application file for complete search history.

FOREIGN PATENT DOCUMENTS

DE	43 23 585 A1	1/1995
EP	0 040 658 A2	12/1981

(Continued)

OTHER PUBLICATIONS

Mary S. Sherman; The Nerves of Bone, The Journal of Bone and
Joint Surgery, Apr. 1963, pp. 522-528, vol. 45-A, No. 3.
(Continued)


Primary Examiner — Jeffrey R Jastrzab

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson
& Bear LLP

(57) **ABSTRACT**

This invention relates to a method of straddling an intraosseous nerve with an energy transmitting device to improve the therapeutic treatment of the nerve.

13 Claims, 32 Drawing Sheets

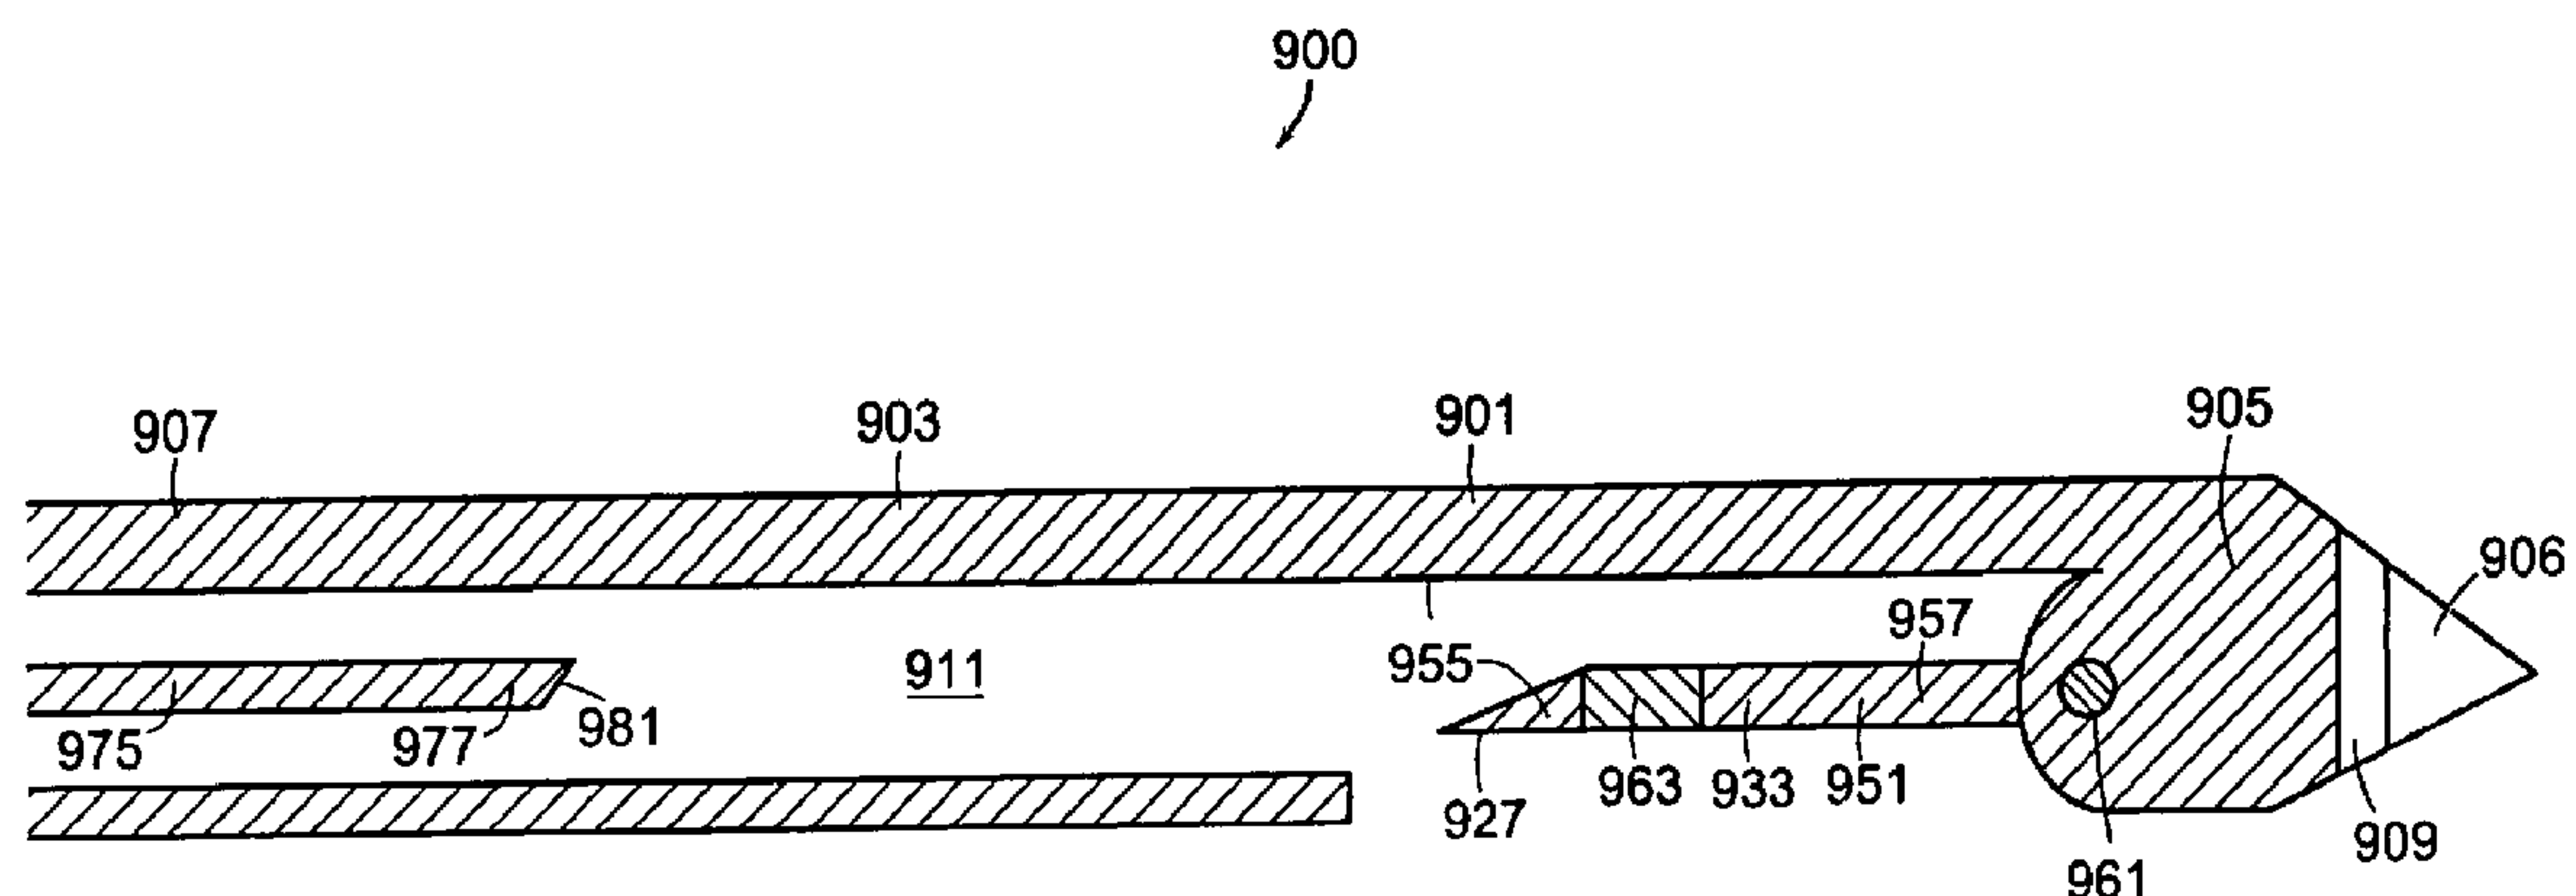

(56)

References Cited

U.S. PATENT DOCUMENTS

4,963,142	A	10/1990	Loertscher	5,843,021	A	12/1998	Edwards et al.
4,966,144	A	10/1990	Rochkind et al.	5,846,218	A	12/1998	Briskin et al.
5,061,266	A	10/1991	Hakky	5,849,011	A	12/1998	Jones et al.
5,080,660	A	1/1992	Buelna	5,855,576	A	1/1999	LeVeen et al.
5,084,043	A	1/1992	Hertzmann et al.	5,860,951	A	1/1999	Eggers et al.
5,098,431	A	3/1992	Rydell	5,865,788	A	2/1999	Edwards et al.
5,106,376	A	4/1992	Mononen et al.	5,868,740	A	2/1999	LeVeen et al.
5,108,404	A	4/1992	Scholten et al.	5,871,469	A	2/1999	Eggers et al.
5,161,533	A	11/1992	Press et al.	5,871,470	A	2/1999	McWha
5,190,546	A	3/1993	Jervis	5,871,481	A	2/1999	Kannenbergen et al.
5,201,729	A	4/1993	Hertzmann et al.	5,873,855	A	2/1999	Eggers et al.
5,209,748	A	5/1993	Daikuzono	5,873,877	A	2/1999	McGaffigan et al.
5,222,953	A	6/1993	Dowlatsahi	5,888,198	A	3/1999	Eggers et al.
5,242,439	A	9/1993	Larsen et al.	5,891,095	A	4/1999	Eggers et al.
5,273,026	A	12/1993	Wilk	5,895,370	A	4/1999	Edwards et al.
5,281,213	A	1/1994	Milder et al.	5,902,272	A	5/1999	Eggers et al.
5,295,484	A	3/1994	Marcus et al.	5,904,681	A	5/1999	West, Jr.
5,320,617	A	6/1994	Leach	5,931,805	A	8/1999	Briskin
5,350,377	A	9/1994	Winston et al.	5,935,123	A	8/1999	Edwards et al.
5,366,443	A	11/1994	Eggers et al.	5,941,722	A	8/1999	Chen
5,368,031	A	11/1994	Cline et al.	5,941,876	A	8/1999	Nardella et al.
5,374,265	A	12/1994	Sand	5,944,715	A	8/1999	Goble et al.
5,391,197	A	2/1995	Burdette et al.	5,948,007	A	9/1999	Starkebaum et al.
5,419,767	A	5/1995	Eggers et al.	5,948,008	A	9/1999	Daikuzono
5,433,739	A	7/1995	Cosman et al.	5,954,716	A	9/1999	Sharkey et al.
5,437,661	A	8/1995	Rieser	5,964,727	A	10/1999	Edwards et al.
5,441,499	A	8/1995	Fritzsche	5,983,141	A	11/1999	Sluijter et al.
5,443,463	A	8/1995	Stern	5,997,497	A	12/1999	Nita et al.
5,458,596	A	10/1995	Lax et al.	6,001,095	A	12/1999	de la Rama et al.
5,458,597	A	10/1995	Edwards et al.	6,007,533	A	12/1999	Casscells et al.
5,472,441	A	12/1995	Edwards et al.	6,007,570	A	12/1999	Sharkey et al.
5,484,432	A	1/1996	Sand	6,012,457	A	1/2000	Lesh
5,486,170	A	1/1996	Winston et al.	6,016,452	A	1/2000	Kasevich
5,514,130	A	5/1996	Baker	6,017,356	A	1/2000	Frederick et al.
5,540,684	A	7/1996	Hassler, Jr.	6,019,776	A	2/2000	Preissman et al.
5,569,242	A	10/1996	Lax et al.	6,022,334	A	2/2000	Edwards et al.
5,571,147	A	11/1996	Sluijter et al.	6,024,733	A	2/2000	Eggers et al.
5,596,988	A	1/1997	Markle et al.	6,024,740	A	2/2000	Lesh et al.
5,620,479	A	4/1997	Diederich	6,030,402	A	2/2000	Thompson et al.
5,630,426	A	5/1997	Shmulewitz et al.	6,032,674	A	3/2000	Eggers et al.
5,630,837	A	5/1997	Crowley	6,033,411	A	3/2000	Preissman et al.
5,643,319	A	7/1997	Green et al.	6,035,238	A	3/2000	Ingle et al.
5,647,871	A	7/1997	Levine et al.	6,045,532	A *	4/2000	Eggers et al. 604/114
5,672,173	A *	9/1997	Gough et al. 606/41	6,050,995	A	4/2000	Durgin
5,681,282	A	10/1997	Eggers et al.	6,053,172	A	4/2000	Hovda et al.
5,683,366	A	11/1997	Eggers et al.	6,053,909	A	4/2000	Shaddock
5,693,052	A	12/1997	Weaver	6,063,079	A	5/2000	Hovda et al.
5,697,281	A	12/1997	Eggers et al.	6,066,134	A	5/2000	Eggers et al.
5,697,536	A	12/1997	Eggers et al.	6,068,642	A	5/2000	Johnson et al.
5,697,882	A	12/1997	Eggers et al.	6,073,051	A	6/2000	Sharkey et al.
5,697,909	A	12/1997	Eggers et al.	6,086,585	A	7/2000	Hovda et al.
5,697,927	A	12/1997	Imran et al.	6,090,105	A	7/2000	Zepeda et al.
5,700,262	A	12/1997	Acosta et al.	6,095,149	A	8/2000	Sharkey et al.
5,720,287	A	2/1998	Chapelon et al.	6,099,514	A	8/2000	Sharkey et al.
5,725,494	A	3/1998	Briskin	6,102,046	A	8/2000	Weinstein et al.
5,728,062	A	3/1998	Briskin	6,104,957	A	8/2000	Alo et al.
5,733,280	A	3/1998	Sherman et al.	6,105,581	A	8/2000	Eggers et al.
5,733,315	A	3/1998	Burdette et al.	6,109,268	A	8/2000	Thaliyal et al.
5,735,811	A	4/1998	Briskin	6,113,597	A	9/2000	Eggers et al.
5,735,847	A	4/1998	Gough et al.	6,117,101	A	9/2000	Diederich et al.
5,738,680	A	4/1998	Mueller et al.	6,117,109	A	9/2000	Eggers et al.
5,743,904	A	4/1998	Edwards	6,117,128	A	9/2000	Gregory
5,746,737	A	5/1998	Saadat	6,120,467	A	9/2000	Schallhorn
5,752,969	A	5/1998	Cunci et al.	6,122,549	A	9/2000	Sharkey et al.
5,762,066	A	6/1998	Law et al.	6,139,545	A	10/2000	Utley et al.
5,762,616	A	6/1998	Talish	6,142,992	A	11/2000	Cheng et al.
5,766,153	A	6/1998	Eggers et al.	6,143,019	A	11/2000	Motamedi et al.
5,776,092	A	7/1998	Farin et al.	6,146,380	A	11/2000	Racz et al.
5,785,705	A	7/1998	Baker	6,149,620	A	11/2000	Baker et al.
5,800,378	A	9/1998	Edwards et al.	6,159,194	A	12/2000	Eggers et al.
5,807,237	A	9/1998	Tindel	6,159,208	A	12/2000	Hovda et al.
5,807,392	A	9/1998	Eggers	6,161,048	A	12/2000	Sluijter et al.
5,810,764	A	9/1998	Eggers et al.	6,164,283	A	12/2000	Lesh
5,817,021	A	10/1998	Reichenberger	6,165,172	A	12/2000	Farley et al.
5,843,019	A	12/1998	Eggers et al.	6,168,593	B1	1/2001	Sharkey et al.
				6,176,857	B1	1/2001	Ashley
				6,179,824	B1	1/2001	Eggers et al.
				6,179,836	B1	1/2001	Eggers et al.
				6,183,469	B1	2/2001	Thaliyal et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,190,381 B1	2/2001	Olsen et al.	6,558,385 B1	5/2003	McClurken et al.
6,190,383 B1	2/2001	Schmaltz et al.	6,560,486 B1	5/2003	Osorio et al.
6,193,715 B1	2/2001	Wrublewski et al.	6,575,968 B1	6/2003	Eggers et al.
6,203,542 B1	3/2001	Ellsberry et al.	6,582,423 B1	6/2003	Thaliyal et al.
6,206,842 B1	3/2001	Tu et al.	6,585,656 B2	7/2003	Masters
6,210,393 B1	4/2001	Briskin	6,589,237 B2	7/2003	Woloszko et al.
6,210,402 B1	4/2001	Olsen et al.	6,595,990 B1	7/2003	Weinstein et al.
6,210,415 B1	4/2001	Bester	6,602,248 B1	8/2003	Sharps et al.
6,221,038 B1	4/2001	Briskin	6,622,731 B2	9/2003	Daniel et al.
6,224,592 B1	5/2001	Eggers et al.	6,632,193 B1	10/2003	Davison et al.
6,228,046 B1	5/2001	Briskin	6,632,220 B1	10/2003	Eggers et al.
6,228,078 B1	5/2001	Eggers et al.	6,659,106 B1	12/2003	Hovda et al.
6,228,082 B1	5/2001	Baker et al.	6,699,242 B2 *	3/2004	Heggeness 606/41
6,231,571 B1	5/2001	Ellman et al.	6,726,684 B1	4/2004	Woloszko et al.
6,231,615 B1	5/2001	Preissman	6,736,835 B2	5/2004	Pellegrino et al.
6,235,020 B1	5/2001	Cheng et al.	6,746,447 B2	6/2004	Davison et al.
6,235,024 B1	5/2001	Tu	6,749,604 B1	6/2004	Eggers et al.
6,238,391 B1	5/2001	Olsen et al.	6,758,846 B2	7/2004	Goble et al.
6,241,665 B1	6/2001	Negus et al.	6,770,071 B2	8/2004	Woloszko et al.
6,241,725 B1	6/2001	Cosman	6,772,012 B2	8/2004	Ricart et al.
6,245,064 B1	6/2001	Lesh et al.	6,773,431 B2	8/2004	Eggers et al.
6,246,912 B1	6/2001	Sluijter et al.	6,827,716 B2	12/2004	Ryan et al.
6,254,553 B1	7/2001	Lidgren et al.	6,832,996 B2	12/2004	Woloszko et al.
6,254,599 B1	7/2001	Lesh et al.	6,837,887 B2	1/2005	Woloszko et al.
6,254,600 B1	7/2001	Willink et al.	6,837,888 B2	1/2005	Ciarrocca et al.
6,258,086 B1	7/2001	Ashley et al.	6,863,672 B2	3/2005	Reiley et al.
6,259,952 B1	7/2001	Sluijter	6,875,219 B2	4/2005	Arramon et al.
6,261,311 B1	7/2001	Sharkey et al.	6,881,214 B2	4/2005	Cosman et al.
6,264,650 B1	7/2001	Hovda et al.	6,896,674 B1	5/2005	Woloszko et al.
6,264,651 B1	7/2001	Underwood et al.	6,907,884 B2 *	6/2005	Pellegrino et al. 128/898
6,264,652 B1	7/2001	Eggers et al.	6,915,806 B2	7/2005	Pacek et al.
6,264,659 B1	7/2001	Ross et al.	6,922,579 B2	7/2005	Taimisto et al.
6,267,770 B1	7/2001	Truwit	6,923,813 B2	8/2005	Phillips et al.
6,277,112 B1	8/2001	Underwood et al.	6,960,204 B2	11/2005	Eggers et al.
6,277,122 B1	8/2001	McGahan et al.	6,974,453 B2	12/2005	Woloszko et al.
6,280,441 B1	8/2001	Ryan	7,048,743 B2	5/2006	Miller et al.
6,283,961 B1 *	9/2001	Underwood et al. 606/41	7,090,672 B2	8/2006	Underwood et al.
6,287,114 B1	9/2001	Meller et al.	7,131,969 B1	11/2006	Hovda et al.
6,287,272 B1	9/2001	Briskin et al.	7,177,678 B1	2/2007	Osorio et al.
6,287,304 B1	9/2001	Eggers et al.	7,179,255 B2	2/2007	Lettice et al.
6,290,715 B1	9/2001	Sharkey et al.	7,186,234 B2	3/2007	Dahla et al.
6,296,619 B1	10/2001	Briskin et al.	7,192,428 B2	3/2007	Eggers et al.
6,296,636 B1	10/2001	Cheng et al.	7,201,731 B1	4/2007	Lundquist et al.
6,296,638 B1	10/2001	Davison et al.	7,201,750 B1	4/2007	Eggers et al.
6,305,378 B1	10/2001	Lesh et al.	7,211,055 B2	5/2007	Diederich
6,309,387 B1	10/2001	Eggers et al.	7,217,268 B2	5/2007	Eggers et al.
6,309,420 B1	10/2001	Preissman	7,258,690 B2	8/2007	Sutton et al.
6,312,408 B1	11/2001	Eggers et al.	7,270,659 B2	9/2007	Ricart et al.
6,312,426 B1	11/2001	Goldberg et al.	7,270,661 B2	9/2007	Dahla et al.
6,322,549 B1	11/2001	Eggers et al.	7,276,063 B2	10/2007	Davison et al.
6,348,055 B1	2/2002	Preissman	7,294,127 B2	11/2007	Leung et al.
6,355,032 B1	3/2002	Hovda et al.	7,318,823 B2	1/2008	Sharps et al.
6,363,937 B1	4/2002	Hovda et al.	7,326,203 B2	2/2008	Papineau et al.
6,379,351 B1	4/2002	Thaliyal et al.	7,331,957 B2	2/2008	Woloszko et al.
6,383,190 B1	5/2002	Preissman	RE40,156 E	3/2008	Sharps et al.
6,391,025 B1	5/2002	Weinstein et al.	7,346,391 B1	3/2008	Osorio et al.
6,416,507 B1	7/2002	Eggers et al.	7,386,350 B2	6/2008	Vilims
6,416,508 B1	7/2002	Eggers et al.	7,387,625 B2	6/2008	Hovda et al.
6,423,059 B1	7/2002	Hanson et al.	7,393,351 B2	7/2008	Woloszko et al.
6,432,103 B1	8/2002	Ellsberry et al.	7,422,585 B1	9/2008	Eggers et al.
6,436,060 B1	8/2002	Talish	7,429,262 B2	9/2008	Woloszko et al.
6,451,013 B1	9/2002	Bays et al.	7,435,247 B2	10/2008	Woloszko et al.
6,454,727 B1	9/2002	Burbank et al.	7,442,191 B2	10/2008	Hovda et al.
6,461,350 B1	10/2002	Underwood et al.	7,468,059 B2	12/2008	Eggers et al.
6,461,354 B1	10/2002	Olsen et al.	7,480,533 B2	1/2009	Cosman et al.
6,464,695 B2	10/2002	Hovda et al.	7,502,652 B2	3/2009	Gaunt et al.
6,468,270 B1	10/2002	Hovda et al.	7,507,236 B2	3/2009	Eggers et al.
6,468,274 B1	10/2002	Alleyne et al.	7,553,307 B2	6/2009	Bleich et al.
6,478,793 B1	11/2002	Cosman et al.	7,555,343 B2	6/2009	Bleich
6,482,201 B1	11/2002	Olsen et al.	7,645,277 B2	1/2010	McClurken et al.
6,500,173 B2	12/2002	Underwood et al.	7,738,968 B2	6/2010	Bleich
6,527,759 B1	3/2003	Tachibana et al.	7,740,631 B2	6/2010	Bleich et al.
6,540,741 B1	4/2003	Underwood et al.	7,749,218 B2	7/2010	Pellegrino et al.
6,544,261 B2	4/2003	Ellsberry et al.	7,819,826 B2	10/2010	Diederich et al.
6,557,559 B1	5/2003	Eggers et al.	7,819,869 B2	10/2010	Godara et al.
			7,824,398 B2	11/2010	Woloszko et al.
			7,824,404 B2	11/2010	Godara et al.
			7,857,813 B2	12/2010	Schmitz et al.
			7,901,403 B2	3/2011	Woloszko et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,909,827 B2	3/2011	Reiley et al.	2003/0158545 A1	8/2003	Hovda et al.
7,917,222 B1	3/2011	Osorio et al.	2003/0181963 A1	9/2003	Pellegrino et al.
7,918,849 B2	4/2011	Bleich et al.	2003/0208194 A1	11/2003	Hovda et al.
7,945,331 B2	5/2011	Vilims	2003/0216725 A1	11/2003	Woloszko et al.
7,963,915 B2	6/2011	Bleich	2003/0216726 A1	11/2003	Eggers et al.
8,066,702 B2	11/2011	Rittman, III et al.	2003/0225364 A1	12/2003	Kraft
8,083,736 B2	12/2011	McClurken et al.	2004/0006339 A1	1/2004	Underwood et al.
8,100,896 B2	1/2012	Podhajsky	2004/0024399 A1	2/2004	Sharps et al.
8,192,424 B2	6/2012	Woloszko	2004/0054366 A1	3/2004	Davison et al.
8,192,435 B2	6/2012	Bleich et al.	2004/0064137 A1	4/2004	Pellegrino et al.
8,265,747 B2	9/2012	Rittman, III et al.	2004/0087937 A1	5/2004	Eggers et al.
8,282,628 B2	10/2012	Paul et al.	2004/0133124 A1	7/2004	Bates et al.
8,292,887 B2	10/2012	Woloszko et al.	2004/0162559 A1	8/2004	Arramon
8,323,279 B2	12/2012	Dahla et al.	2004/0193151 A1	9/2004	To et al.
8,355,799 B2	1/2013	Marion et al.	2004/0220577 A1	11/2004	Cragg et al.
8,361,067 B2	1/2013	Pellegrino et al.	2004/0225228 A1	11/2004	Ferree
8,414,509 B2	4/2013	Diederich et al.	2004/0230190 A1	11/2004	Dahla et al.
8,414,571 B2	4/2013	Pellegrino et al.	2005/0004634 A1	1/2005	Ricart et al.
8,419,730 B2	4/2013	Pellegrino et al.	2005/0010203 A1	1/2005	Edwards et al.
8,419,731 B2	4/2013	Pellegrino et al.	2005/0010205 A1	1/2005	Hovda et al.
8,425,507 B2	4/2013	Pellegrino et al.	2005/0182417 A1	8/2005	Pagano
8,535,309 B2	9/2013	Pellegrino et al.	2005/0192564 A1	9/2005	Cosman et al.
8,597,301 B2	12/2013	Mitchell	2005/0209659 A1	9/2005	Pellegrino et al.
8,613,744 B2	12/2013	Pellegrino et al.	2005/0283148 A1	12/2005	Janssen et al.
8,623,014 B2	1/2014	Pellegrino et al.	2006/0004369 A1	1/2006	Patel et al.
8,628,528 B2	1/2014	Pellegrino et al.	2006/0064101 A1	3/2006	Arramon
8,808,284 B2	8/2014	Pellegrino et al.	2006/0095026 A1	5/2006	Ricart et al.
8,882,764 B2	11/2014	Pellegrino et al.	2006/0095028 A1	5/2006	Bleich
8,992,522 B2	3/2015	Pellegrino et al.	2006/0122458 A1	6/2006	Bleich
8,992,523 B2	3/2015	Pellegrino et al.	2006/0129101 A1	6/2006	McGuckin
9,017,325 B2	4/2015	Pellegrino et al.	2006/0178670 A1	8/2006	Woloszko et al.
9,023,038 B2	5/2015	Pellegrino et al.	2006/0229625 A1	10/2006	Truckai et al.
9,039,701 B2	5/2015	Pellegrino et al.	2006/0253117 A1	11/2006	Hovda et al.
9,173,676 B2	11/2015	Pellegrino et al.	2006/0264957 A1	11/2006	Cragg et al.
9,259,241 B2	2/2016	Pellegrino et al.	2006/0265014 A1	11/2006	Demarais et al.
9,265,522 B2	2/2016	Pellegrino et al.	2006/0276749 A1	12/2006	Selmon et al.
9,421,064 B2	8/2016	Pellegrino et al.	2007/0118142 A1	5/2007	Krueger et al.
2001/0001314 A1	5/2001	Davison et al.	2007/0129715 A1	6/2007	Eggers et al.
2001/0001811 A1	5/2001	Burney et al.	2007/0149966 A1	6/2007	Dahla et al.
2001/0020167 A1	9/2001	Woloszko et al.	2007/0179497 A1	8/2007	Eggers et al.
2001/0023348 A1	9/2001	Ashley et al.	2007/0260237 A1	11/2007	Sutton et al.
2001/0025176 A1	9/2001	Ellsberry et al.	2008/0004621 A1	1/2008	Dahla et al.
2001/0025177 A1	9/2001	Woloszko et al.	2008/0004675 A1	1/2008	King et al.
2001/0029370 A1	10/2001	Hodva et al.	2008/0009847 A1	1/2008	Ricart et al.
2001/0029373 A1	10/2001	Baker et al.	2008/0021447 A1	1/2008	Davison et al.
2001/0032001 A1	10/2001	Ricart et al.	2008/0021463 A1	1/2008	Georgy
2001/0047167 A1	11/2001	Heggeness	2008/0058707 A1	3/2008	Ashley et al.
2001/0049522 A1	12/2001	Eggers et al.	2008/0114364 A1	5/2008	Goldin et al.
2001/0051802 A1	12/2001	Woloszko et al.	2008/0119844 A1	5/2008	Woloszko et al.
2001/0056280 A1	12/2001	Underwood et al.	2008/0119846 A1	5/2008	Rioux
2002/0016600 A1	2/2002	Cosman	2008/0132890 A1	6/2008	Woloszko et al.
2002/0019626 A1	2/2002	Sharkey et al.	2008/0161804 A1	7/2008	Rioux et al.
2002/0026186 A1	2/2002	Woloszko et al.	2008/0275458 A1	11/2008	Bleich et al.
2002/0052600 A1	5/2002	Davison et al.	2008/0294166 A1	11/2008	Goldin et al.
2002/0068930 A1	6/2002	Tasto et al.	2009/0030308 A1	1/2009	Bradford et al.
2002/0095144 A1	7/2002	Carl	2009/0069807 A1	3/2009	Eggers et al.
2002/0095151 A1	7/2002	Dahla et al.	2009/0105775 A1	4/2009	Mitchell et al.
2002/0095152 A1	7/2002	Ciarrocca et al.	2009/0118731 A1	5/2009	Young et al.
2002/0099366 A1	7/2002	Dahla et al.	2009/0131867 A1	5/2009	Liu et al.
2002/0120259 A1	8/2002	Lettice et al.	2009/0131886 A1	5/2009	Liu et al.
2002/0147444 A1	10/2002	Shah et al.	2009/0222053 A1	9/2009	Gaunt et al.
2002/0151885 A1	10/2002	Underwood et al.	2009/0312764 A1	12/2009	Marino
2002/0188284 A1	12/2002	To et al.	2010/0016929 A1	1/2010	Prochazka
2002/0188290 A1	12/2002	Sharkey et al.	2010/0023006 A1	1/2010	Ellman
2002/0193789 A1	12/2002	Underwood et al.	2010/0082033 A1	4/2010	Germain
2003/0009164 A1	1/2003	Woloszko et al.	2010/0094269 A1	4/2010	Pellegrino et al.
2003/0014047 A1	1/2003	Woloszko et al.	2010/0114098 A1	5/2010	Carl
2003/0028189 A1	2/2003	Woloszko et al.	2010/0145424 A1	6/2010	Podhajsky et al.
2003/0040742 A1	2/2003	Underwood et al.	2010/0185161 A1	7/2010	Pellegrino et al.
2003/0055418 A1	3/2003	Tasto et al.	2010/0211076 A1	8/2010	Germain et al.
2003/0083592 A1	5/2003	Faciszewski	2010/0222777 A1	9/2010	Sutton et al.
2003/0084907 A1	5/2003	Pacek et al.	2010/0298832 A1	11/2010	Lau et al.
2003/0097126 A1	5/2003	Woloszko et al.	2010/0324506 A1	12/2010	Pellegrino et al.
2003/0097129 A1	5/2003	Davison et al.	2011/0022133 A1	1/2011	Diederich et al.
2003/0130655 A1	7/2003	Woloszko et al.	2011/0034884 A9	2/2011	Pellegrino et al.
			2011/0040362 A1	2/2011	Godara et al.
			2011/0077628 A1	3/2011	Hoey et al.
			2011/0087314 A1	4/2011	Diederich et al.
			2011/0196361 A1	8/2011	Vilims

(56)

References Cited**U.S. PATENT DOCUMENTS**

2011/0264098	A1	10/2011	Cobbs
2011/0276001	A1	11/2011	Schultz et al.
2011/0319765	A1	12/2011	Gertner et al.
2012/0029420	A1	2/2012	Rittman, III et al.
2012/0123427	A1	5/2012	McGuckin, Jr.
2012/0196251	A1	8/2012	Taft et al.
2012/0197344	A1	8/2012	Taft et al.
2012/0203219	A1	8/2012	Evans et al.
2012/0226273	A1	9/2012	Nguyen et al.
2012/0239050	A1	9/2012	Linderman
2012/0330180	A1	12/2012	Pellegrino et al.
2012/0330300	A1	12/2012	Pellegrino et al.
2012/0330301	A1	12/2012	Pellegrino et al.
2013/0006232	A1	1/2013	Pellegrino et al.
2013/0006233	A1	1/2013	Pellegrino et al.
2013/0012933	A1	1/2013	Pellegrino et al.
2013/0012935	A1	1/2013	Pellegrino et al.
2013/0012936	A1	1/2013	Pellegrino et al.
2013/0103022	A1	4/2013	Sutton et al.
2013/0261507	A1	10/2013	Diederich et al.
2013/0324994	A1	12/2013	Pellegrino et al.
2013/0324996	A1	12/2013	Pellegrino et al.
2013/0324997	A1	12/2013	Pellegrino et al.
2014/0039500	A1	2/2014	Pellegrino et al.
2014/0288544	A1	9/2014	Diederich et al.
2014/0336630	A1	11/2014	Woloszko et al.
2015/0005614	A1	1/2015	Heggeness et al.
2015/0045783	A1	2/2015	Edidin
2015/0057658	A1	2/2015	Sutton et al.
2015/0164546	A1	6/2015	Pellegrino et al.
2015/0297246	A1	10/2015	Patel et al.
2015/0335349	A1	11/2015	Pellegrino et al.
2015/0335382	A1	11/2015	Pellegrino et al.
2015/0342670	A1	12/2015	Pellegrino et al.
2016/0278791	A1	9/2016	Pellegrino et al.

FOREIGN PATENT DOCUMENTS

EP	0040658	12/1981
EP	0584959	3/1994
EP	0597463	5/1994
EP	1 013 228 A1	6/2000
EP	1013228	6/2000
EP	1 059 067 A1	12/2000
EP	1059067	12/2000
EP	1059087	12/2000
JP	6-47058	2/1994
JP	6-47058 A	2/1994
JP	10-290806	11/1998
JP	2001-037760	2/2001
JP	2005-169012	6/2005
WO	9636289 A1	11/1996
WO	WO 96/36289	11/1996
WO	98-27876 A1	7/1998
WO	WO 98/27876	7/1998
WO	WO 98/34550	8/1998
WO	WO 99/19025	4/1999
WO	WO 99/44519	9/1999
WO	WO 99/48621	9/1999
WO	WO 00/21448	4/2000
WO	WO 00/33909	6/2000
WO	WO 00/49978	8/2000
WO	WO 00/56237	9/2000
WO	WO 00/67648	11/2000
WO	WO 00/67656	11/2000
WO	WO 01/01877	1/2001
WO	WO 01/26570	4/2001
WO	WO 01/45579	6/2001
WO	0157655 A2	8/2001
WO	WO 01/57655	8/2001
WO	WO 02/05699	1/2002
WO	WO02/05897	1/2002
WO	0228302 A1	4/2002
WO	WO 02/28302	4/2002
WO	02054941 A2	7/2002

WO	WO 02/054941	7/2002
WO	02-067797 A2	9/2002
WO	WO 02/067797	9/2002
WO	WO 02/096304	12/2002
WO	WO2007/031264	3/2007
WO	WO2008/001385	1/2008
WO	WO2008/008522	1/2008
WO	WO2008/121259	10/2008
WO	WO 2008/140519	11/2008
WO	WO2013/101772	7/2013

OTHER PUBLICATIONS

Michael H. Heggeness, et al., The Trabecular Anatomy of Thoracolumbar Vertebrae: Implications for Burst Fractures, *Journal of Anatomy*, 1997, pp. 309-312, vol. 191, Great Britain.

J.B. Martin, et al., Vertebroplasty: Clinical Experience and Follow-up Results, *Bone*, Aug. 1999, pp. 11S-15S, vol. 25, No. 2, Supplement.

H. Deramond, et al., Temperature Elevation Caused by Bone Cement Polymerization During Vertebroplasty, *Bone*, Aug. 1999, pp. 17S-21S, vol. 25, No. 2, Supplement.

Cosman, E.R. et al. Theoretical Aspects of Radiofrequency Lesions in the Dorsal Root Entry Zone. *Neurosurgery*, vol. 1, No. 6, 1984, pp. 945-950.

Massad, Malek M.D. et al.; Endoscopic Thoracic Sympathectomy: Evaluation of Pulsatile Laser, Non-Pulsatile Laser, and Radiofrequency-Generated Thermocoagulation; *Lasers in Surgery and Medicine*; 1991; pp. 18-25.

Kleinstueck, Frank S. et al.; Acute Biomechanical and Histological Effects of Intradiscal Electrothermal Therapy on Human Lumbar Discs; *Spine* vol. 26, No. 20, pp. 2198-2207; 2001, Lippincott Williams & Wilkins, Inc.

Heggeness, Michael H. et al. Discography Causes End Plate Deflection; *Spine* vol. 18, No. 8, pp. 1050-1053, 1993, J.B. Lippincott Company.

Letcher, Frank S. et al.; The Effect of Radiofrequency Current and Heat on Peripheral Nerve Action Potential in the Cat; U.S. Naval Hospital, Philadelphia, PA (1968).

Haupt, Jonathan C. et al.; Experimental Study of Temperature Distributions and Thermal Transport During Radiofrequency Current Therapy of the Intervertebral Disc; *Spine* vol. 21, No. 15, pp. 1808-1813, 1996, Lippincott-Raven Publishers.

Lundskog, Jan; Heat and Bone Tissue—An experimental investigation of the thermal properties of bone tissue and threshold levels for thermal injury; *Scandinavian Journal of Plastic and Reconstructive Surgery Supplement 9*, From the Laboratory of Experimental Biology, Department of anatomy, University of Gothenburg, Gothenburg, Sweden, Goteborg (1972).

Antonacci, M. Darryl et al.; Innervation of the Human Vertebral Body: A Histologic Study; *Journal of Spinal Disorder*, vol. 11, No. 6, pp. 526-531, 1998 Lippincott Williams & Wilkins, Philadelphia.

Arnoldi, Carl C.; Intraosseous Hypertension—A Possible Cause of Low Back Pain?; *Clinical Orthopedics and Related Research*, No. 115, Mar.-Apr. 1976.

Esses, Stephen I. et al.; Intraosseous Vertebral Body Pressures; *Spine* vol. 17 No. 6 Supplement (1992).

Troussier, B. et al.; Percutaneous Intradiscal Radio-Frequency Thermocoagulation A Cadaveric Study; *Spine* vol. 20, No. 15, pp. 1713-1718, 1995, Lippincott-Raven Publishers.

Choy, Daniel SS.J. et al.; Percutaneous Laser Disc Decompression, A New Therapeutic Modality; *Spine* vol. 17, No. 8 (1992).

Shealy, C. Norman; Percutaneous radiofrequency denervation of spinal facets: Treatment for chronic back pain and sciatica; *Journal of Neurosurgery*/vol. 43/Oct. 1975.

Depuy, Damian E.; Radiofrequency Ablation: An Outpatient Percutaneous Treatment; *Medicine and Health/Rhode Island* vol. 82, No. 6, Jun. 1999.

Rashbaum, Ralph F.; Radiofrequency Facet Denervation A Treatment alternative in Refractory Low Back Pain with or without Leg Pain; *Orthopedic Clinics of North America*—vol. 14, No. 3, Jul. 1983.

(56)

References Cited

OTHER PUBLICATIONS

Lehmann, Justus F. et al.; Selective Heating Effects of Ultrasound in Human Beings; *Archives of Physical Medicine & Rehabilitation* Jun. 1966.

Hanai, Kenji et al.; Simultaneous Measurement of Intraosseous and Cerebrospinal Fluid Pressures in the Lumbar Region; *Spine* vol. 10, No. 1 (1985).

Bogduk, Nikolai, et al.; Technical Limitations to the efficacy of Radiofrequency Neurotomy for Spinal Pain; *Neurosurgery* vol. 20, No. 4 (1987).

Mehta, Mark et al.; The treatment of chronic back pain; *Anaesthesia*, 1979, vol. 34, pp. 768-775.

Deardorff, Dana L. et al.; Ultrasound applicators with internal cooling for interstitial thermal therapy; *SPIE* vol. 3594 (1999).

Diederich, Chris J. et al.; Ultrasound Catheters for Circumferential Cardiac Ablation; *SPIE* vol. 3594 (1999).

Diederich C J, et al. "IDTT Therapy in Cadaveric Lumbar Spine: Temperature and thermal dose distributions, Thermal Treatment of Tissue: Energy Delivery and Assessment," Thomas P. Ryan, Editor, *Proceedings of SPIE* vol. 4247:104-108 (2001).

Nau, William H., Ultrasound interstitial thermal therapy (USITT) in the prostate; *SPIE* vol. 3594 (1999).

The AVAmax System—Cardinal Health Special Procedures, Lit. No. 25P0459-01—www.cardinal.com (allegedly dated 2007).

Kopecky, Kenyon K. et al. "Side-Exiting Coaxial Needle for Aspiration Biopsy"—*AJR*—1996; 167, pp. 661-662.

A Novel Approach for Treating Chronic Lower Back Pain, Abstract for Presentation at North American Spine Society 26th Annual Meeting in Chicago, IL on Nov. 4, 2011.

Stanton, Terry, "Can Nerve Ablation Reduce Chronic Back Pain ?" *AAOS Now* Jan. 2012.

Ryan et al., "Three-Dimensional Finite Element Simulations of Vertebral Body Thermal Treatment," *Thermal Treatment of Tissue: Energy Delivery and Assessment III*, edited by Thomas P. Ryan, *Proceedings of SPIE*, vol. 5698 (SPIE, Bellingham, WA, 2005) pp. 137-155.

Bergeron et al., "Fluoroscopic-guided radiofrequency ablation of the basivertebral nerve: application and analysis with multiple

imaging modalities in an ovine model," *Thermal Treatment of Tissue: Energy Delivery and Assessment III*, edited by Thomas P. Ryan, *Proceedings of SPIE*, vol. 5698 (SPIE, Bellingham, WA, 2005) pp. 156-167.

Hoopes et al., "Radiofrequency Ablation of The Basivertebral Nerve as a Potential Treatment of Back Pain: Pathologic Assessment in an Ovine Model," *Thermal Treatment of Tissue: Energy Delivery and Assessment III*, edited by Thomas P. Ryan, *Proceedings of SPIE*, vol. 5698 (SPIE, Bellingham, WA, 2005) pp. 168-180. FDA Response to 510(k) Submission by Relievant Medsystems, Inc. submitted on Sep. 27, 2007 (date stamped on Oct. 5, 2007) and associated documents.

Ullrich, Jr., Peter F., "Lumbar Spinal Fusion Surgery" Jan. 9, 2013, *Spine-Health* (available via wayback machine Internet archive at <http://web.archive.org/web/20130109095419/http://www.spine-health.com/treatment/spinal-fusion/lumbar-spinal-fusion-surgery>).

E.R. Cosman et al. Theoretical aspects of radiofrequency lesions in the dorsal root entry zone. *Neurosurgery*, vol. 15, No. 6, pp. 945-950 (1984).

D.E. Dupuy et al. Radiofrequency ablation of spinal tumors: Temperature distribution in the spinal canal *AJR*, vol. 175, pp. 1263-1266, Nov. 2000.

S.N. Goldberg et al. Tissue ablation with radiofrequency: Effect of probe size, gauge, duration, and temperature on lesion volume, *Acad. Radiol.*, vol. 2, pp. 399-404 (1995).

M. Massad et al.; Endoscopic Thoracic Sympathectomy: Evaluation of pulsatile laser, non-pulsatile laser, and radiofrequency-generated thermocoagulation; *lasers in surgery and medicine*; pp. 18-25 (1991).

D.I. Rosenthal. *Seminars in Musculoskeletal Radiology*, vol. 1, No. 2., pp. 265-272 (1997).

L. Solbiati et al. Hepatic metastases: Percutaneous radio-frequency ablation with cooled-tip electrodes. *Interventional Radiology*, vol. 205, No. 2, pp. 367-373 (1997).

C.L. Tillotson et al. Controlled thermal injury of bone: Report of a percutaneous technique using radiofrequency electrode and generator. *Investigative Radiology*, Nov. 1989, pp. 888-892.

EP Search Report dated Jan. 14, 2004, for EPO Application No. EP 03 25 6168.

* cited by examiner

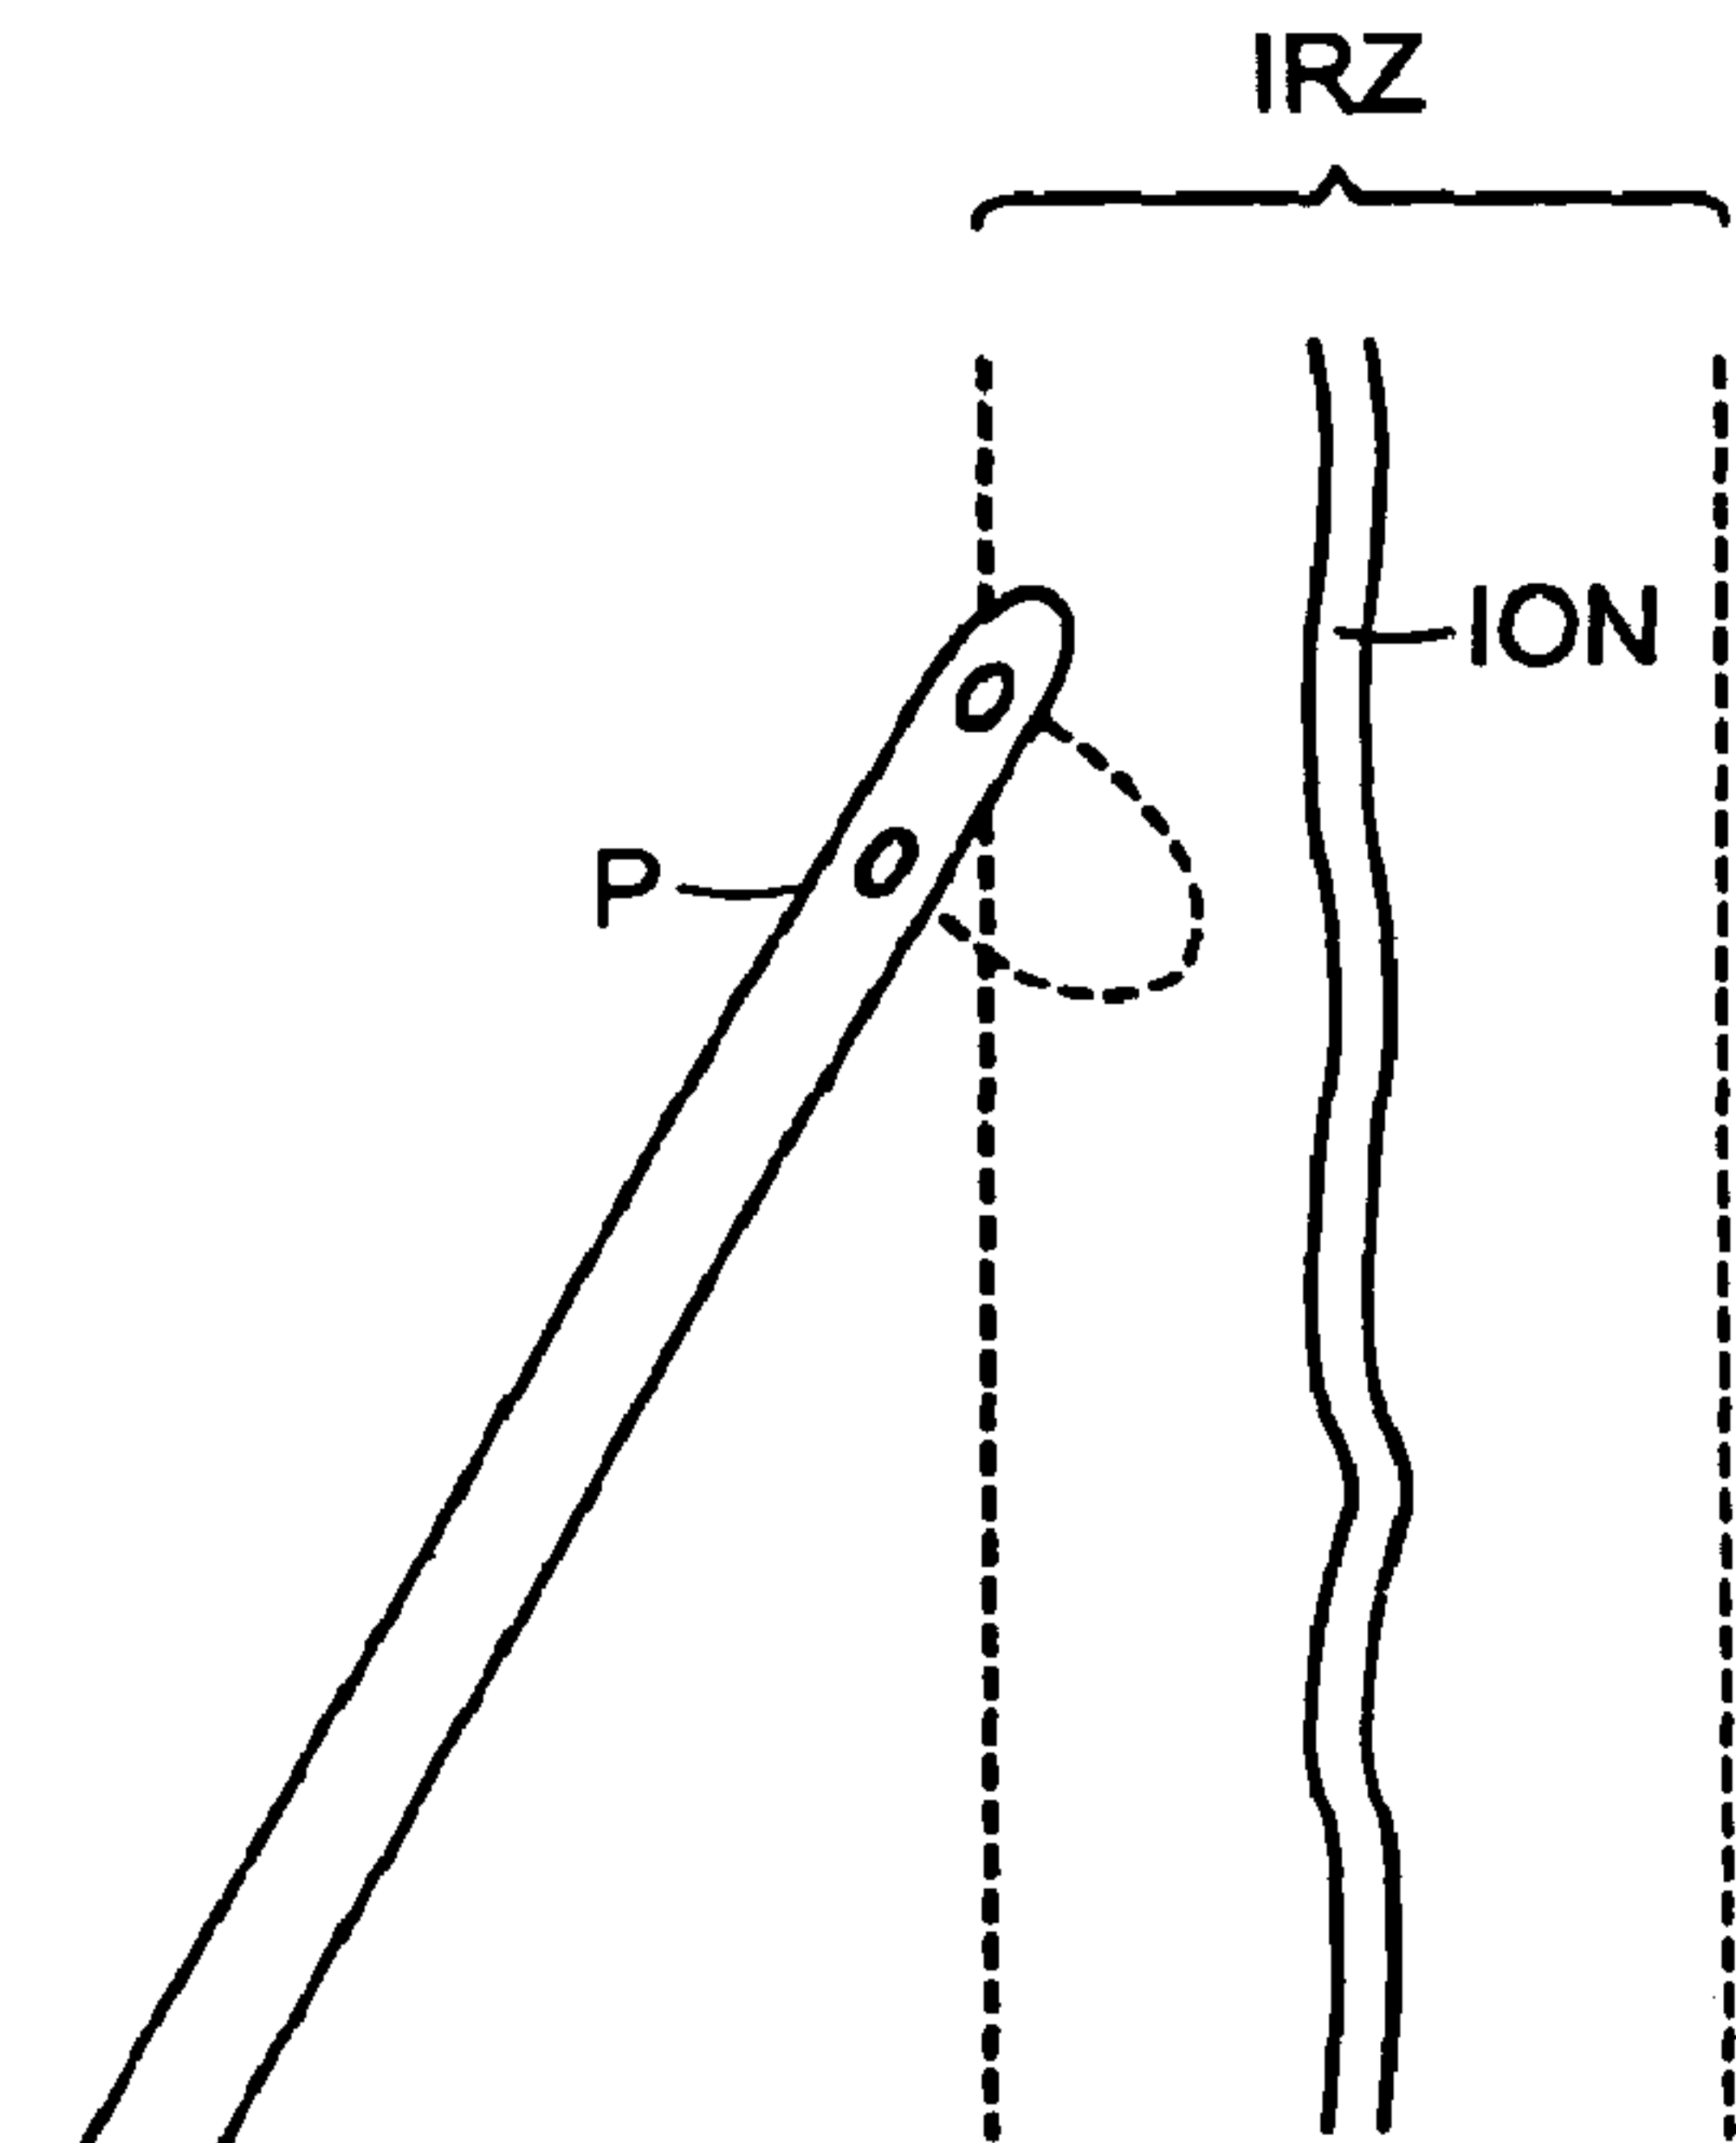


FIG. 1
PRIOR ART

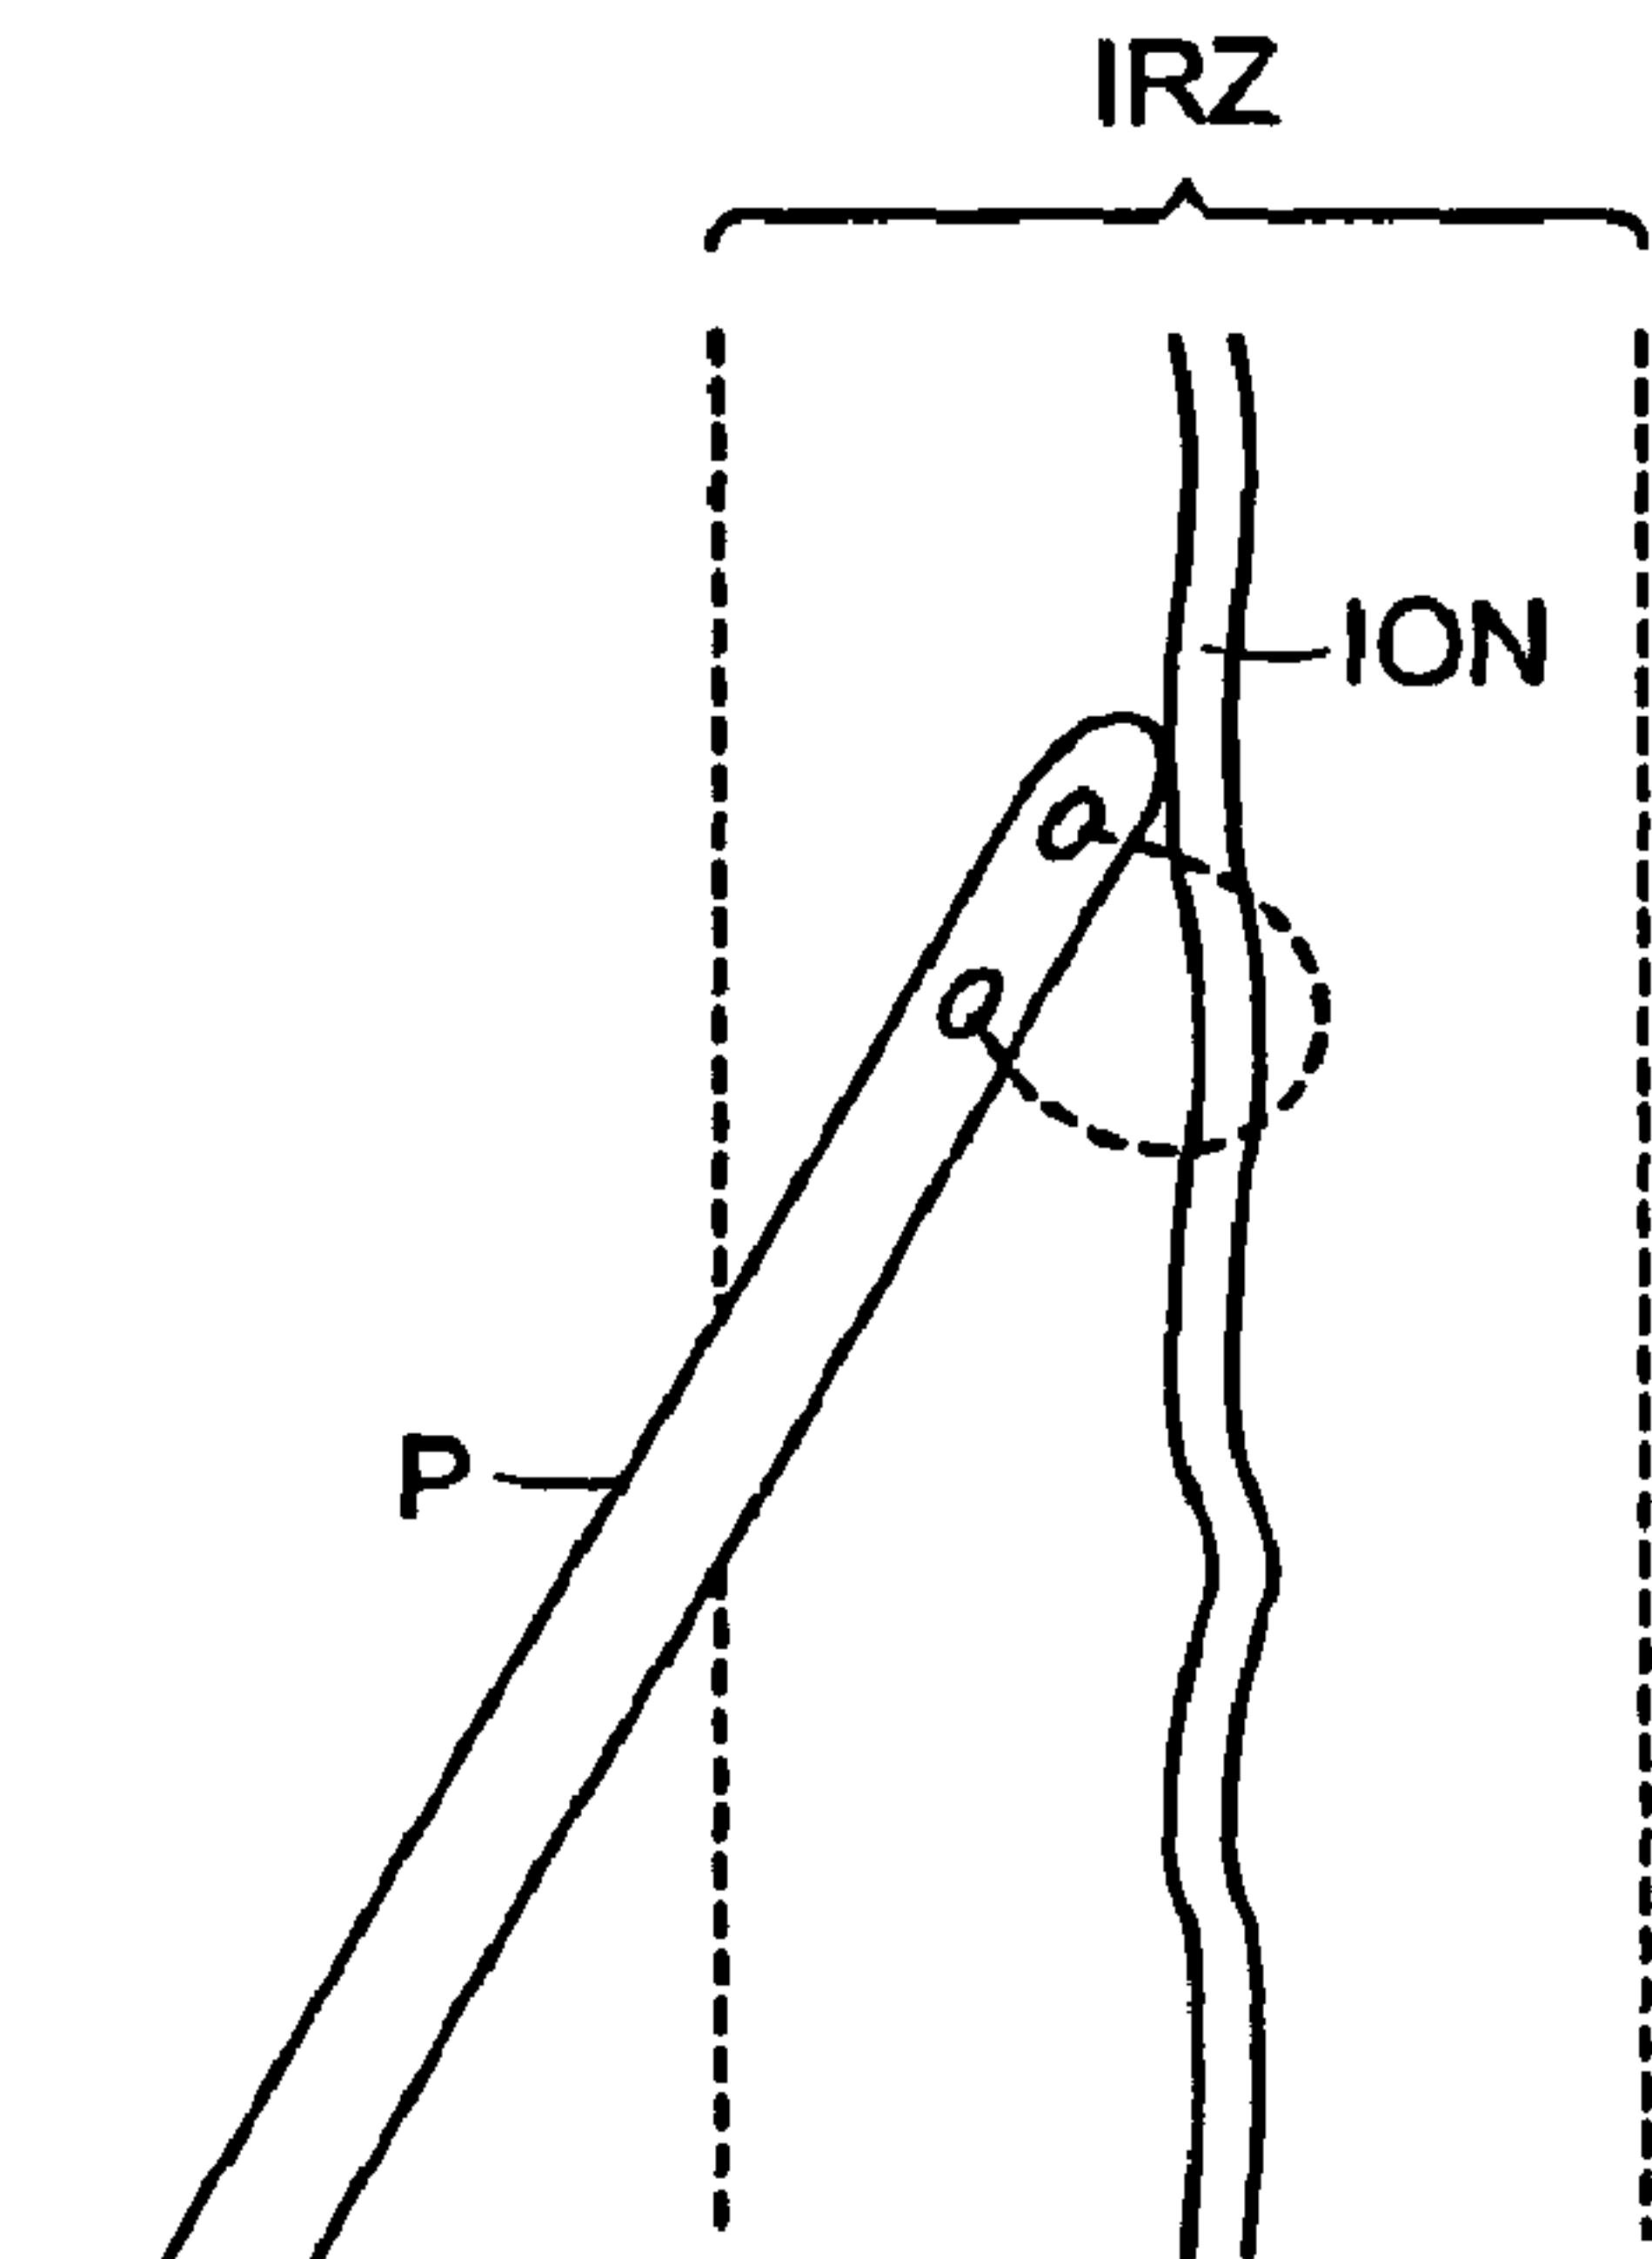


FIG. 2
PRIOR ART

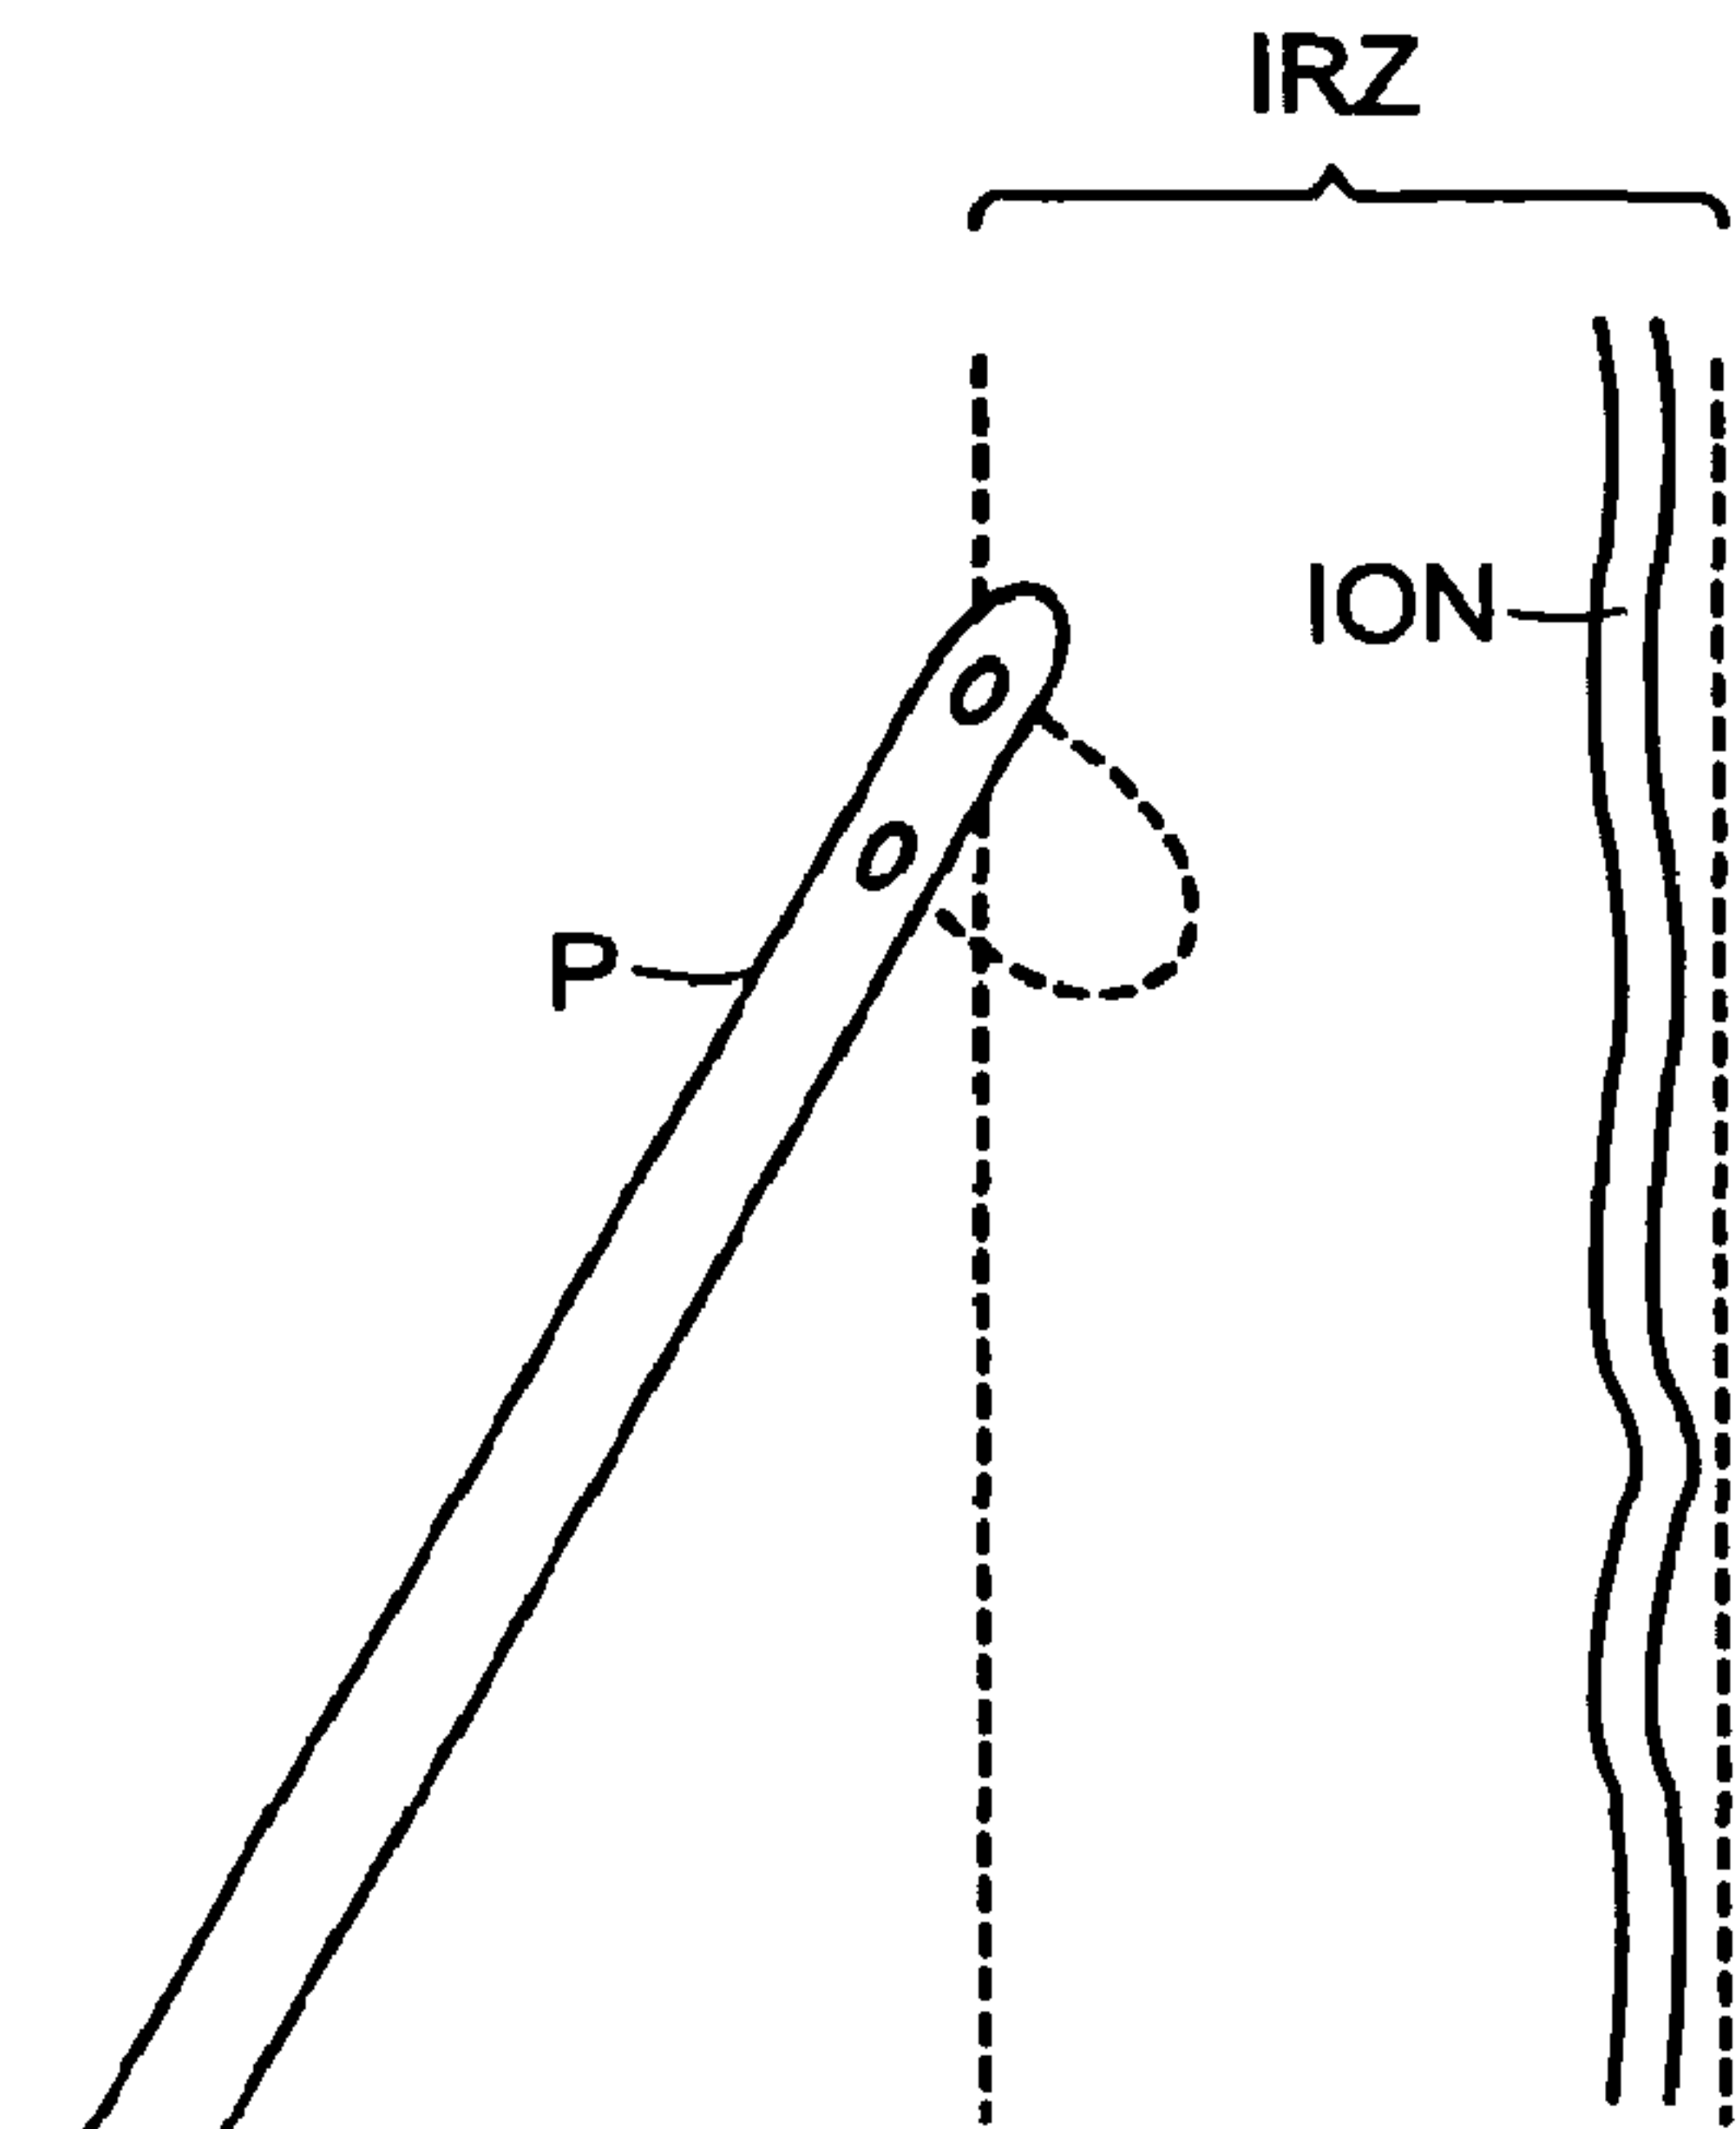


FIG. 3
PRIOR ART

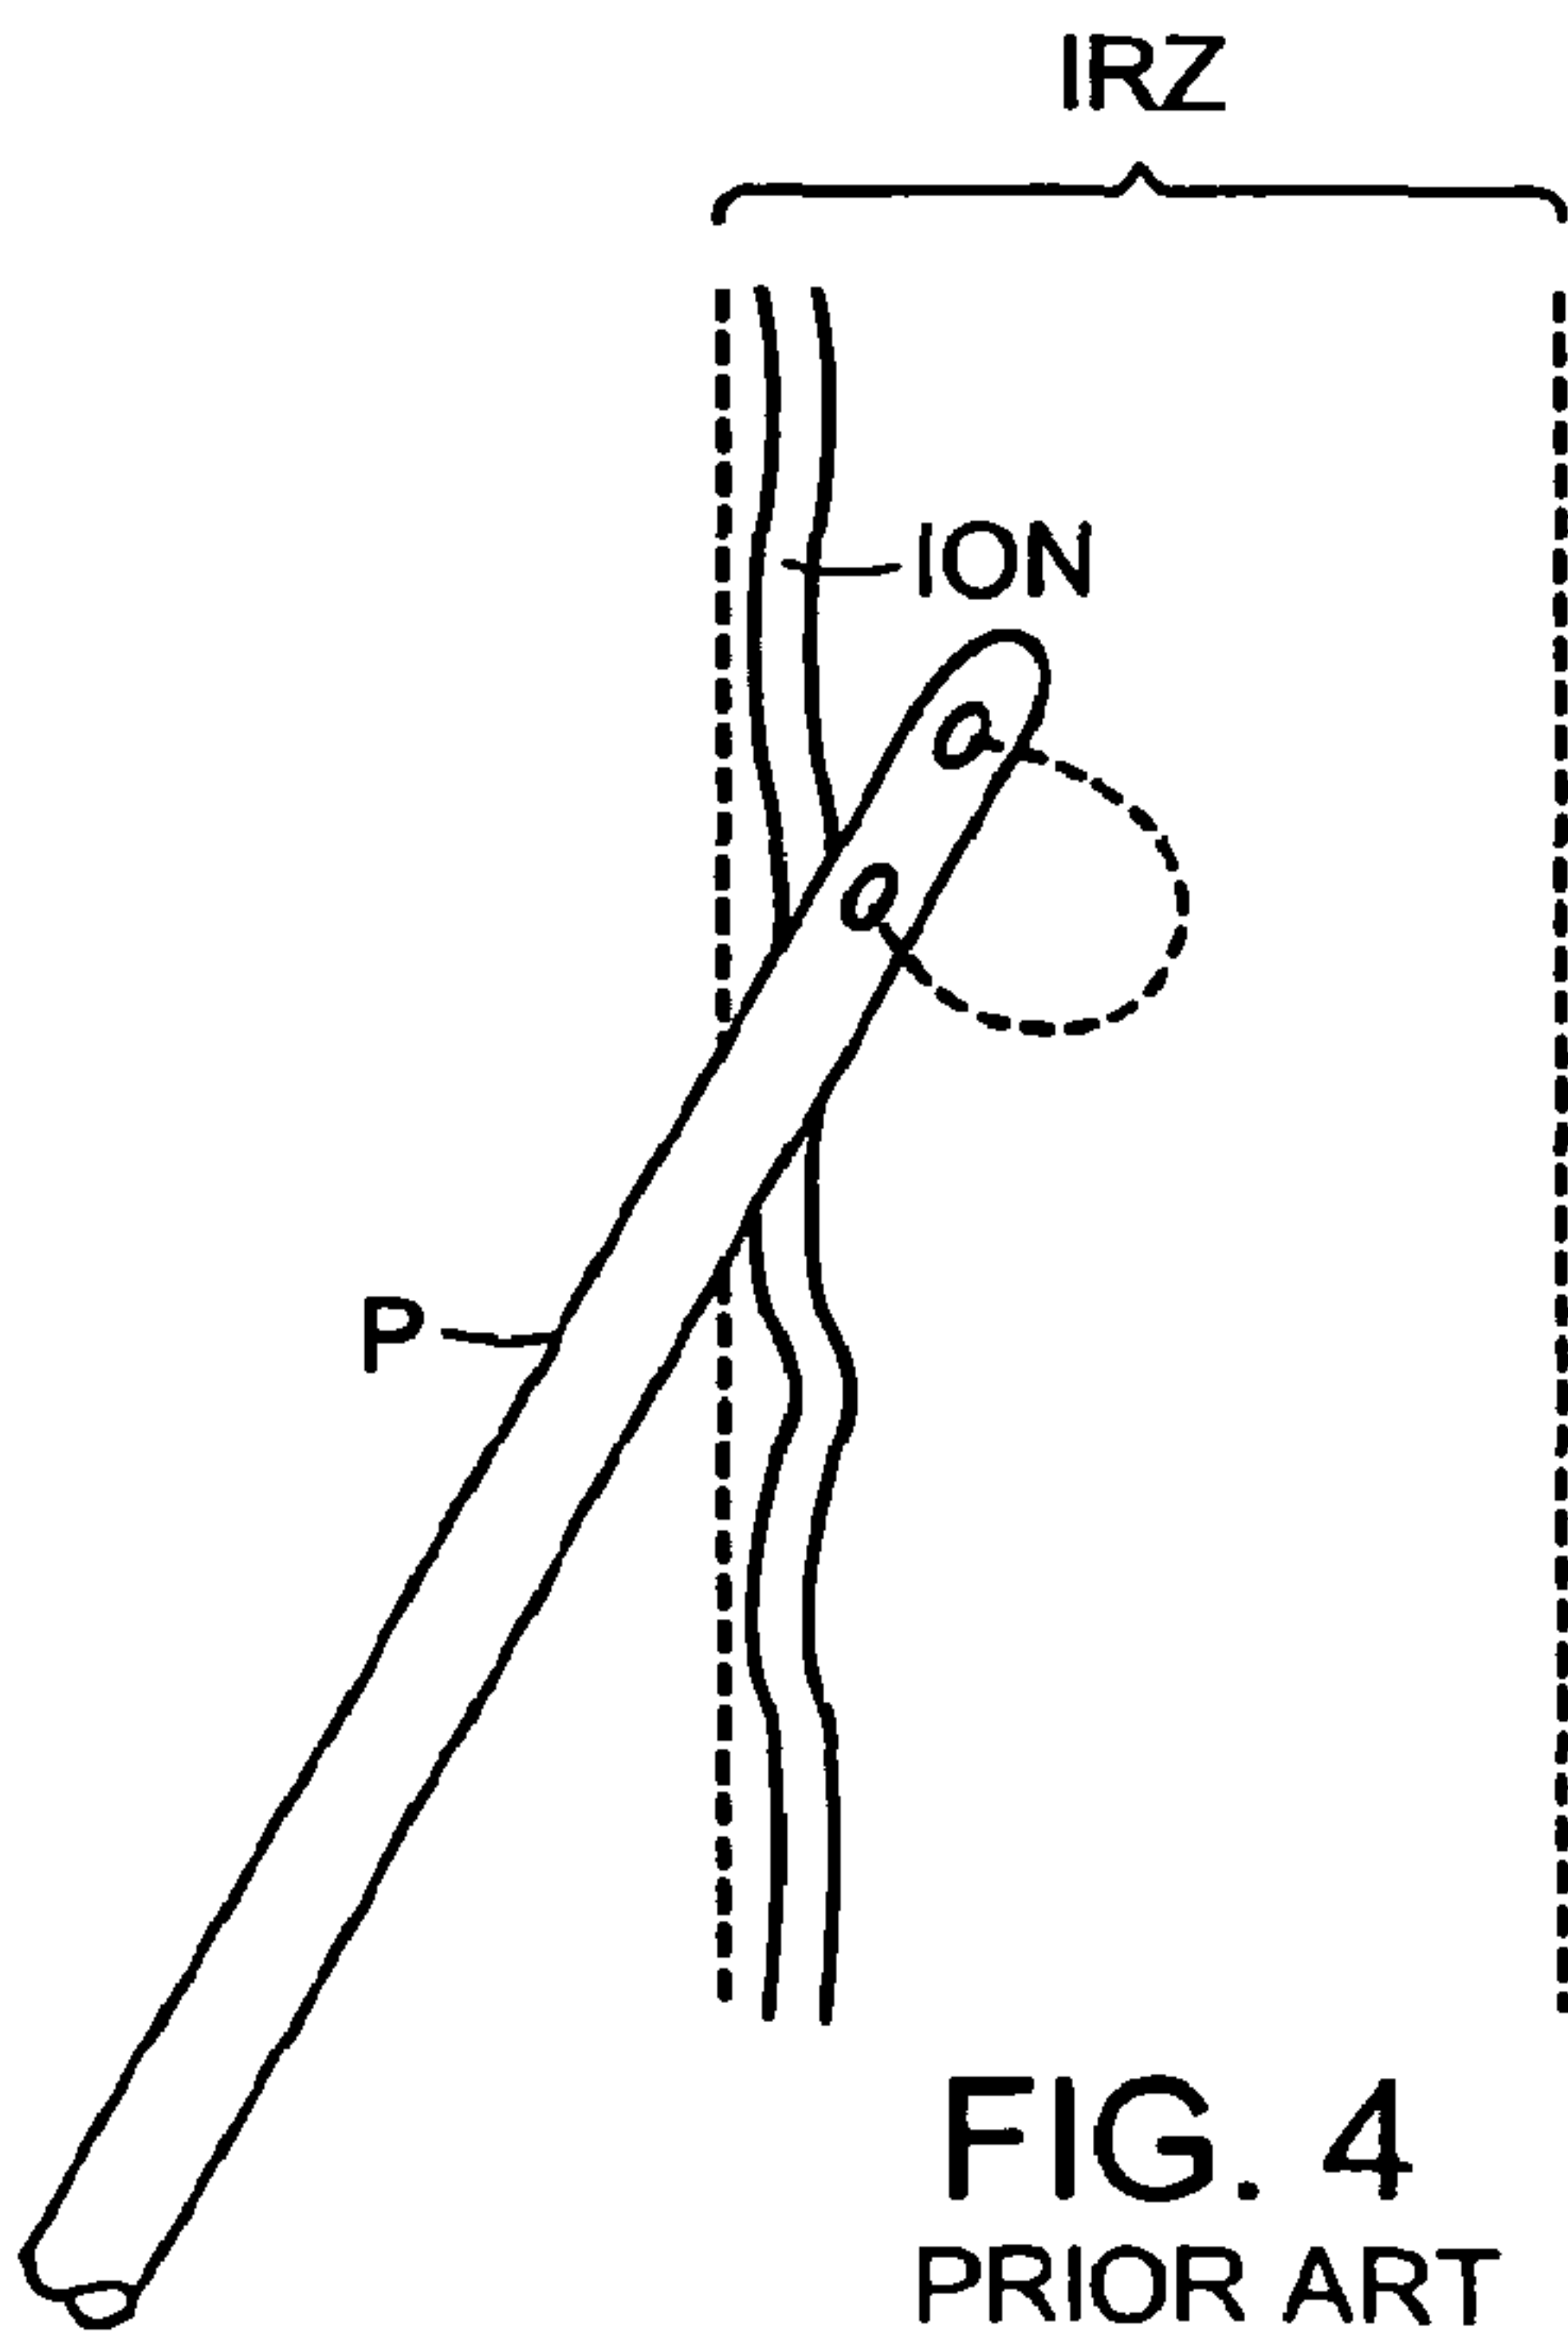


FIG. 4
PRIOR ART

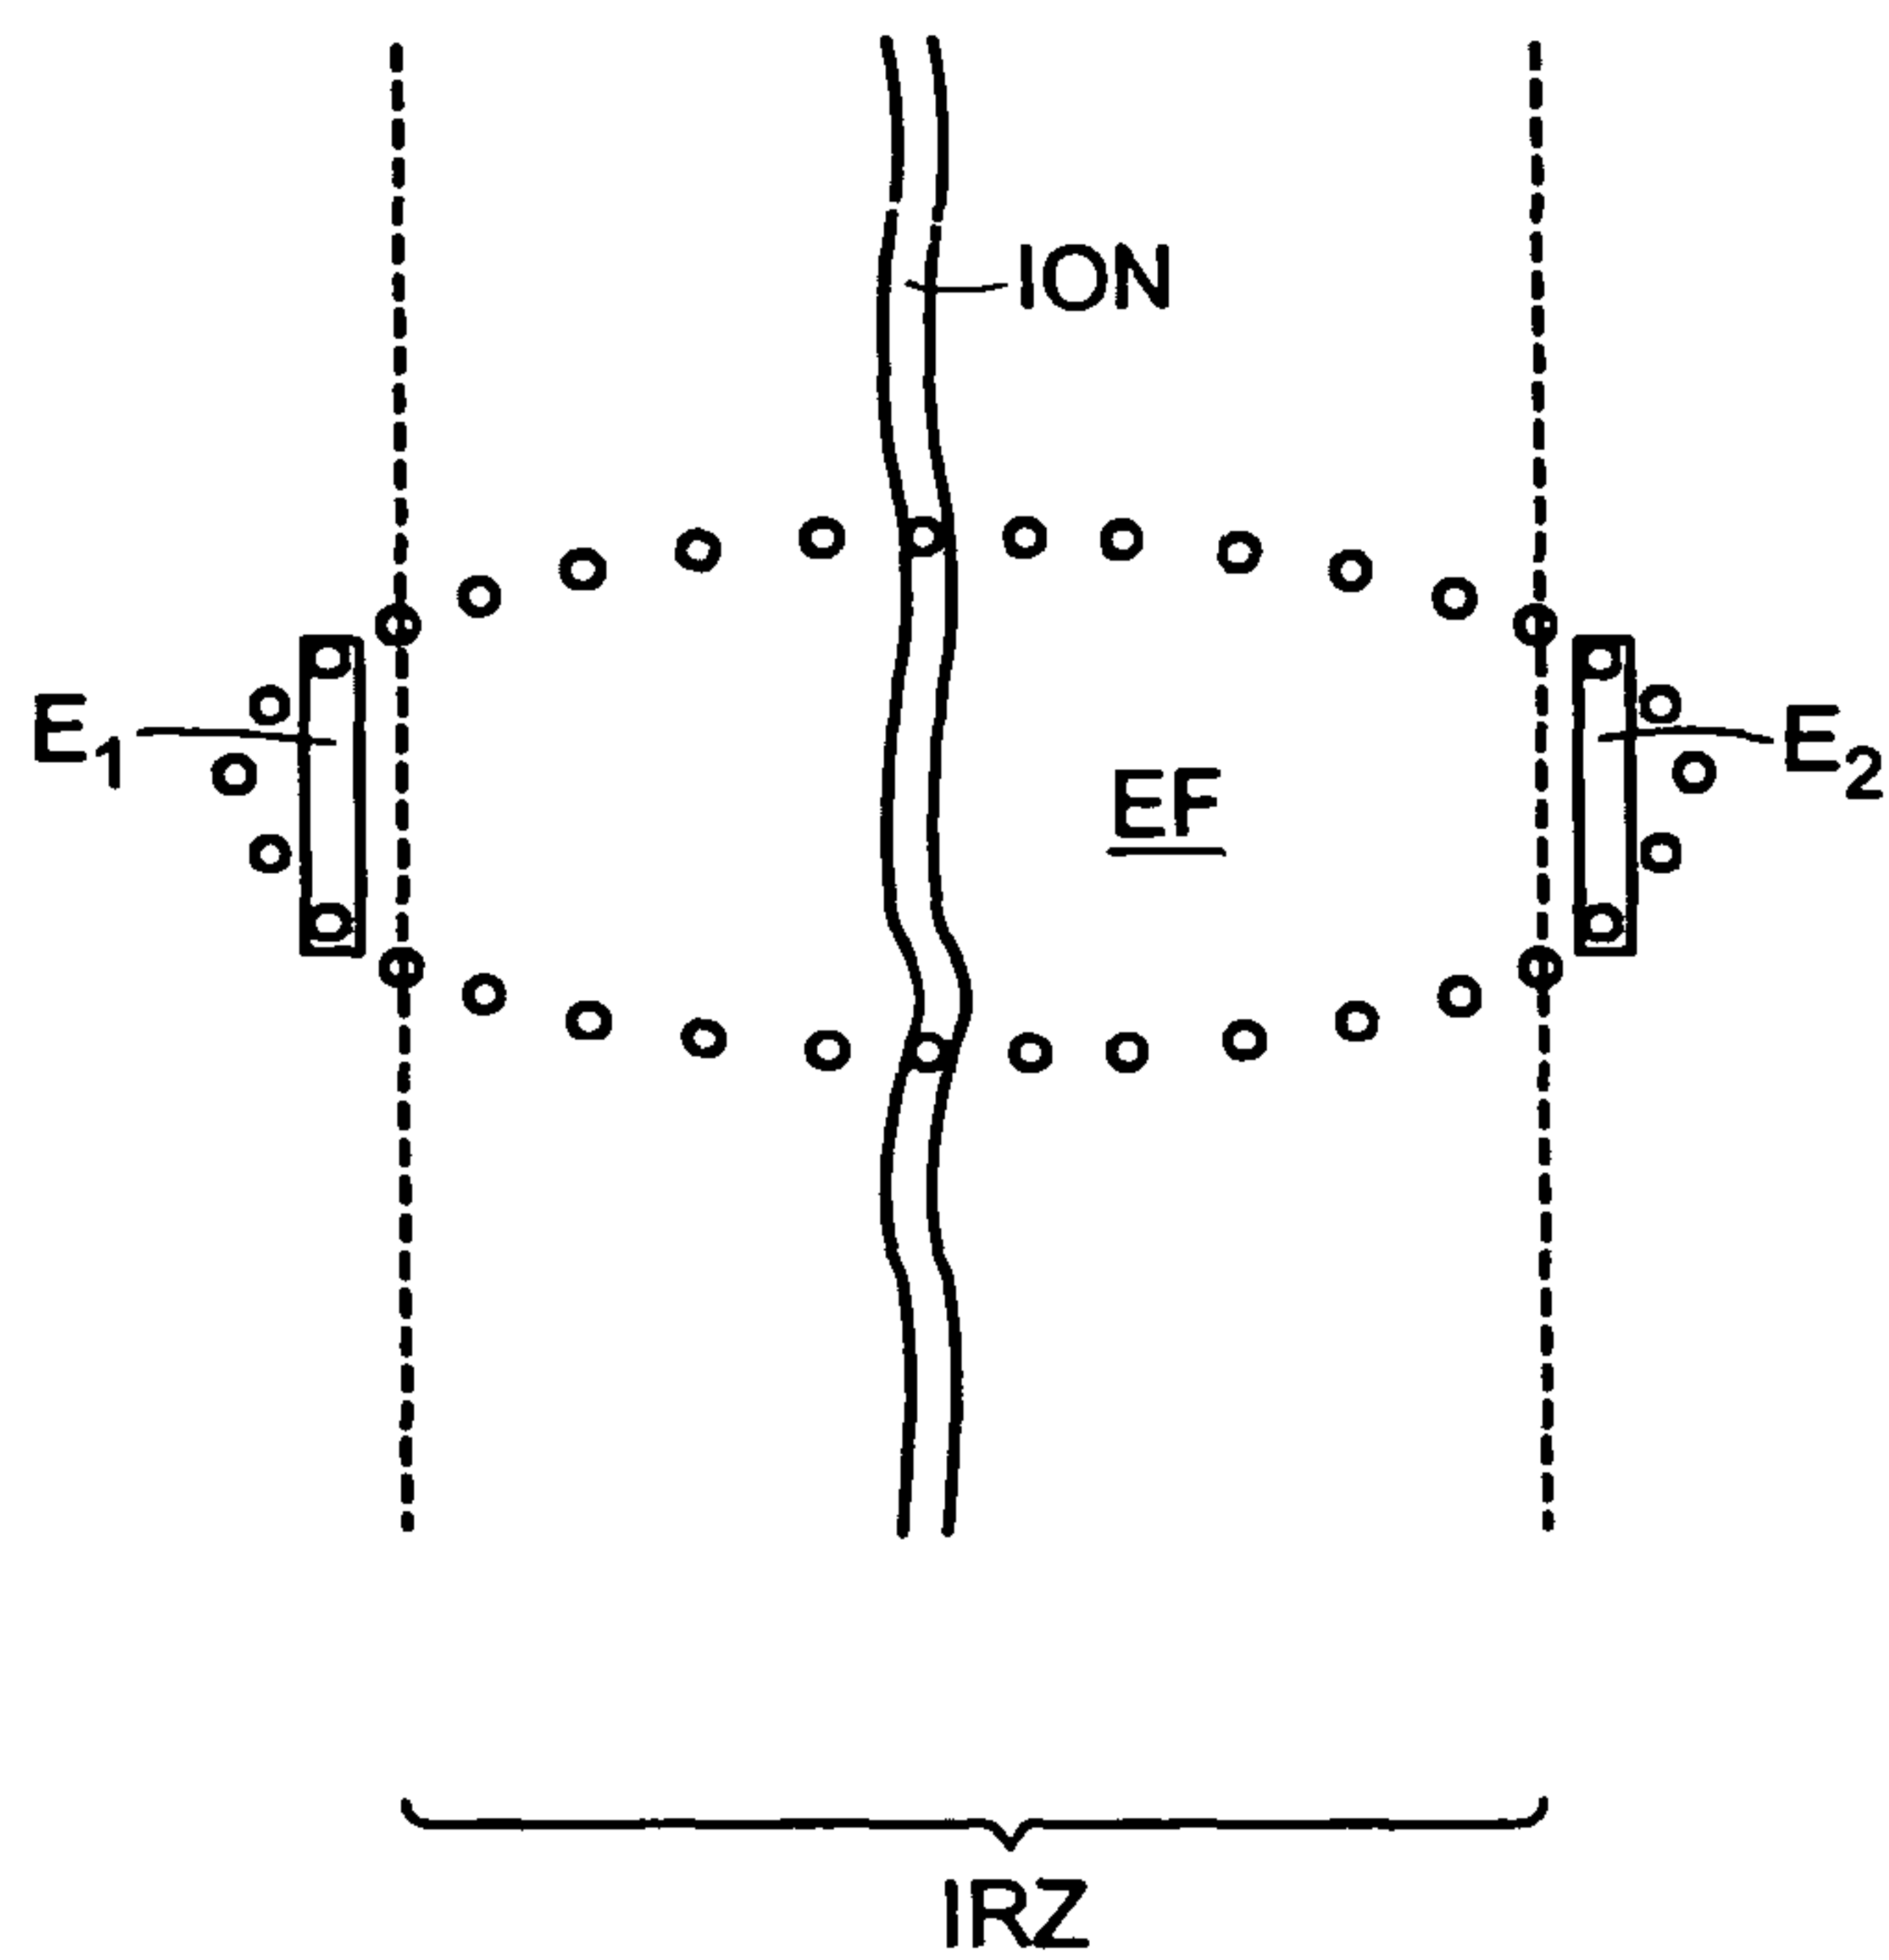


FIG. 5

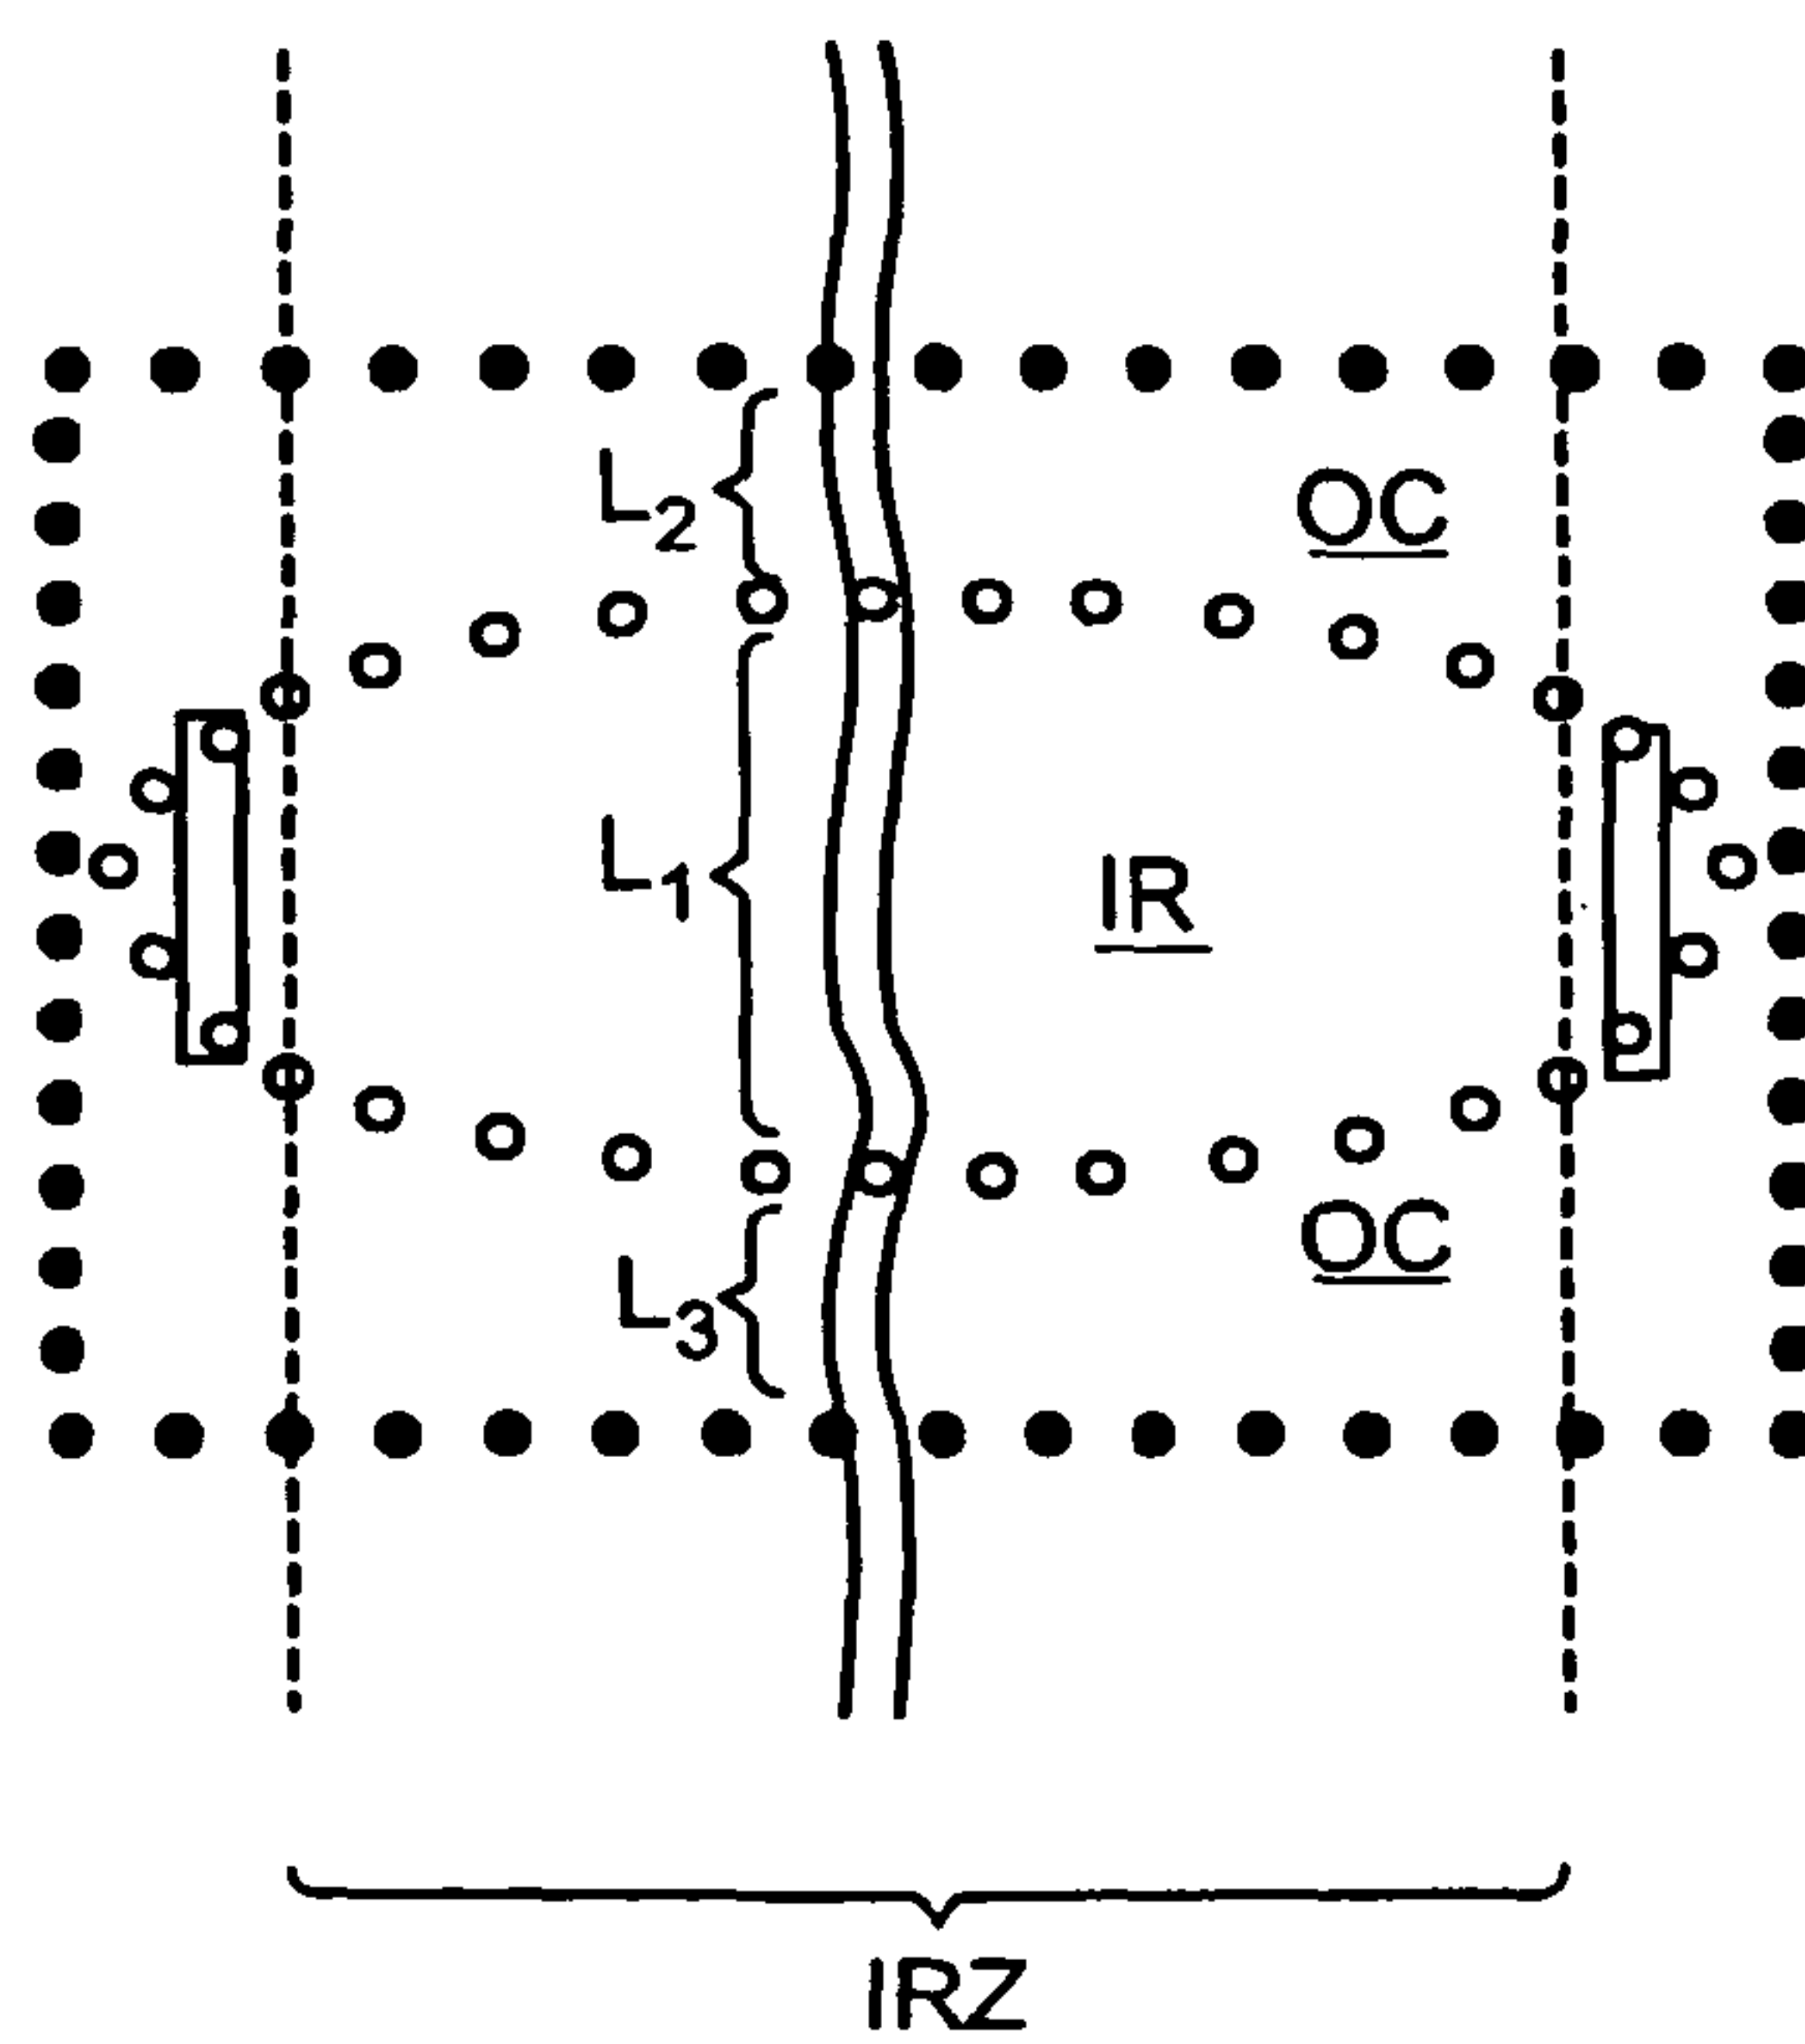


FIG. 6

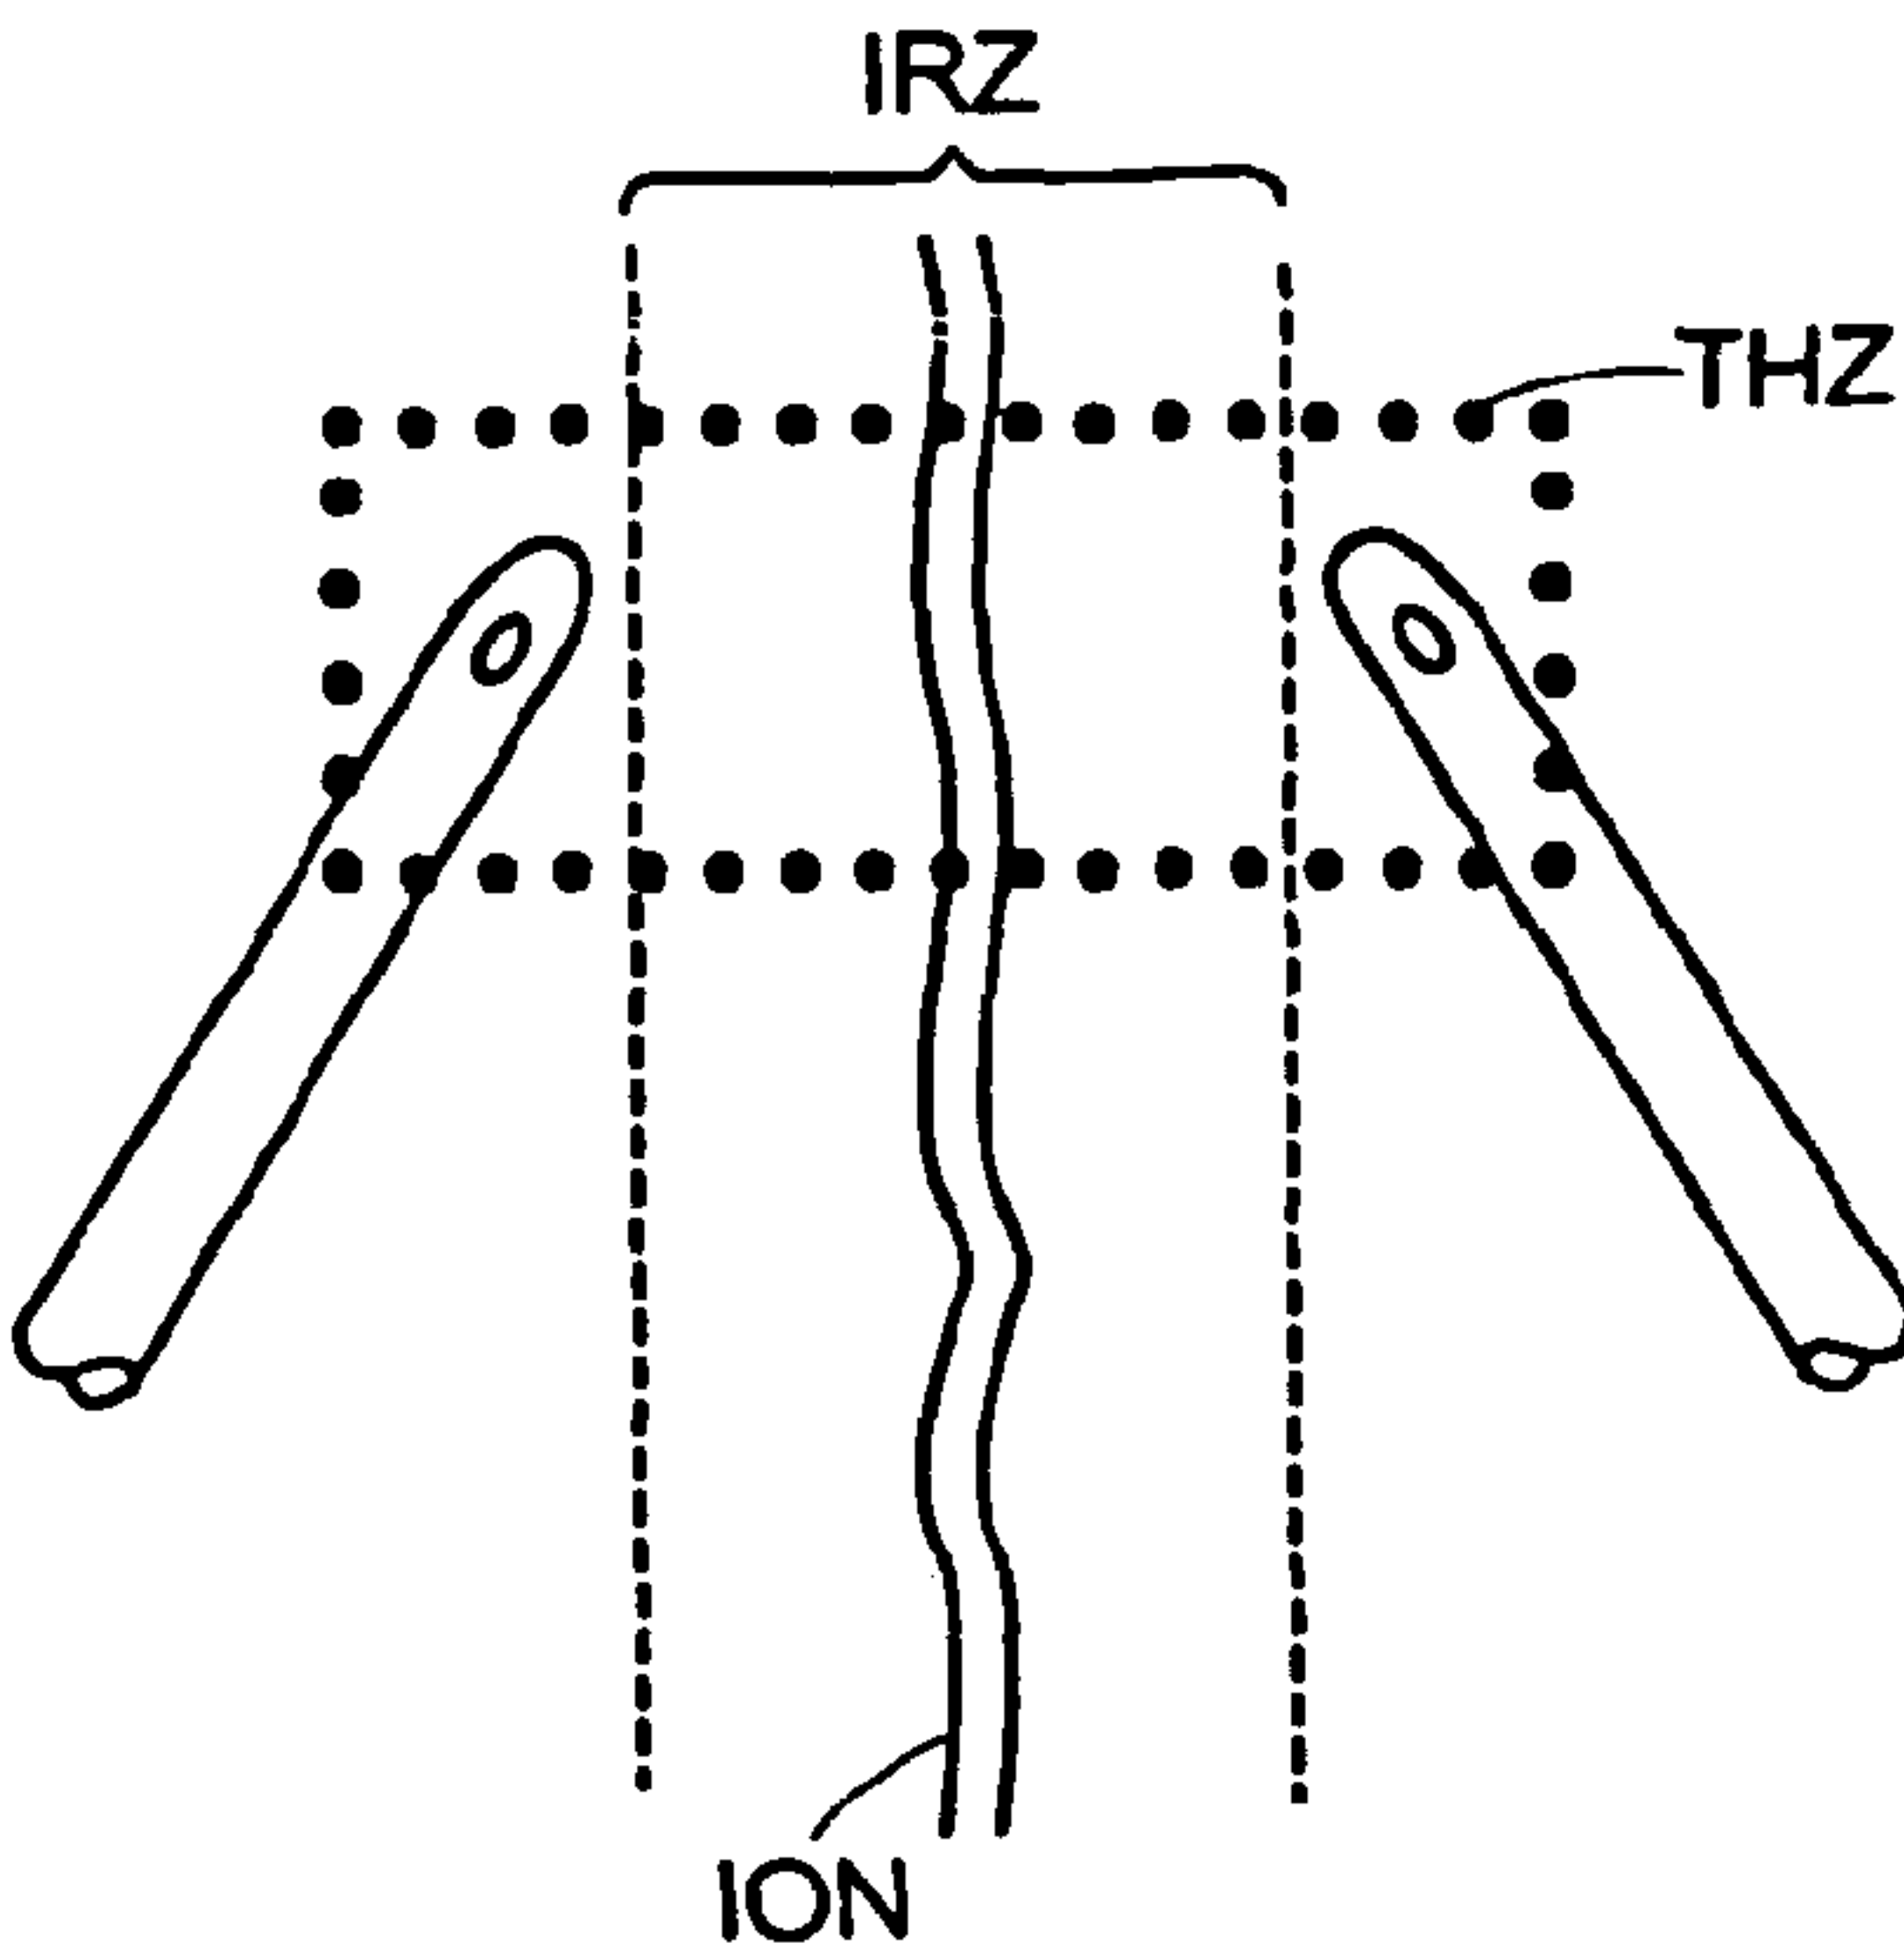


FIG. 7

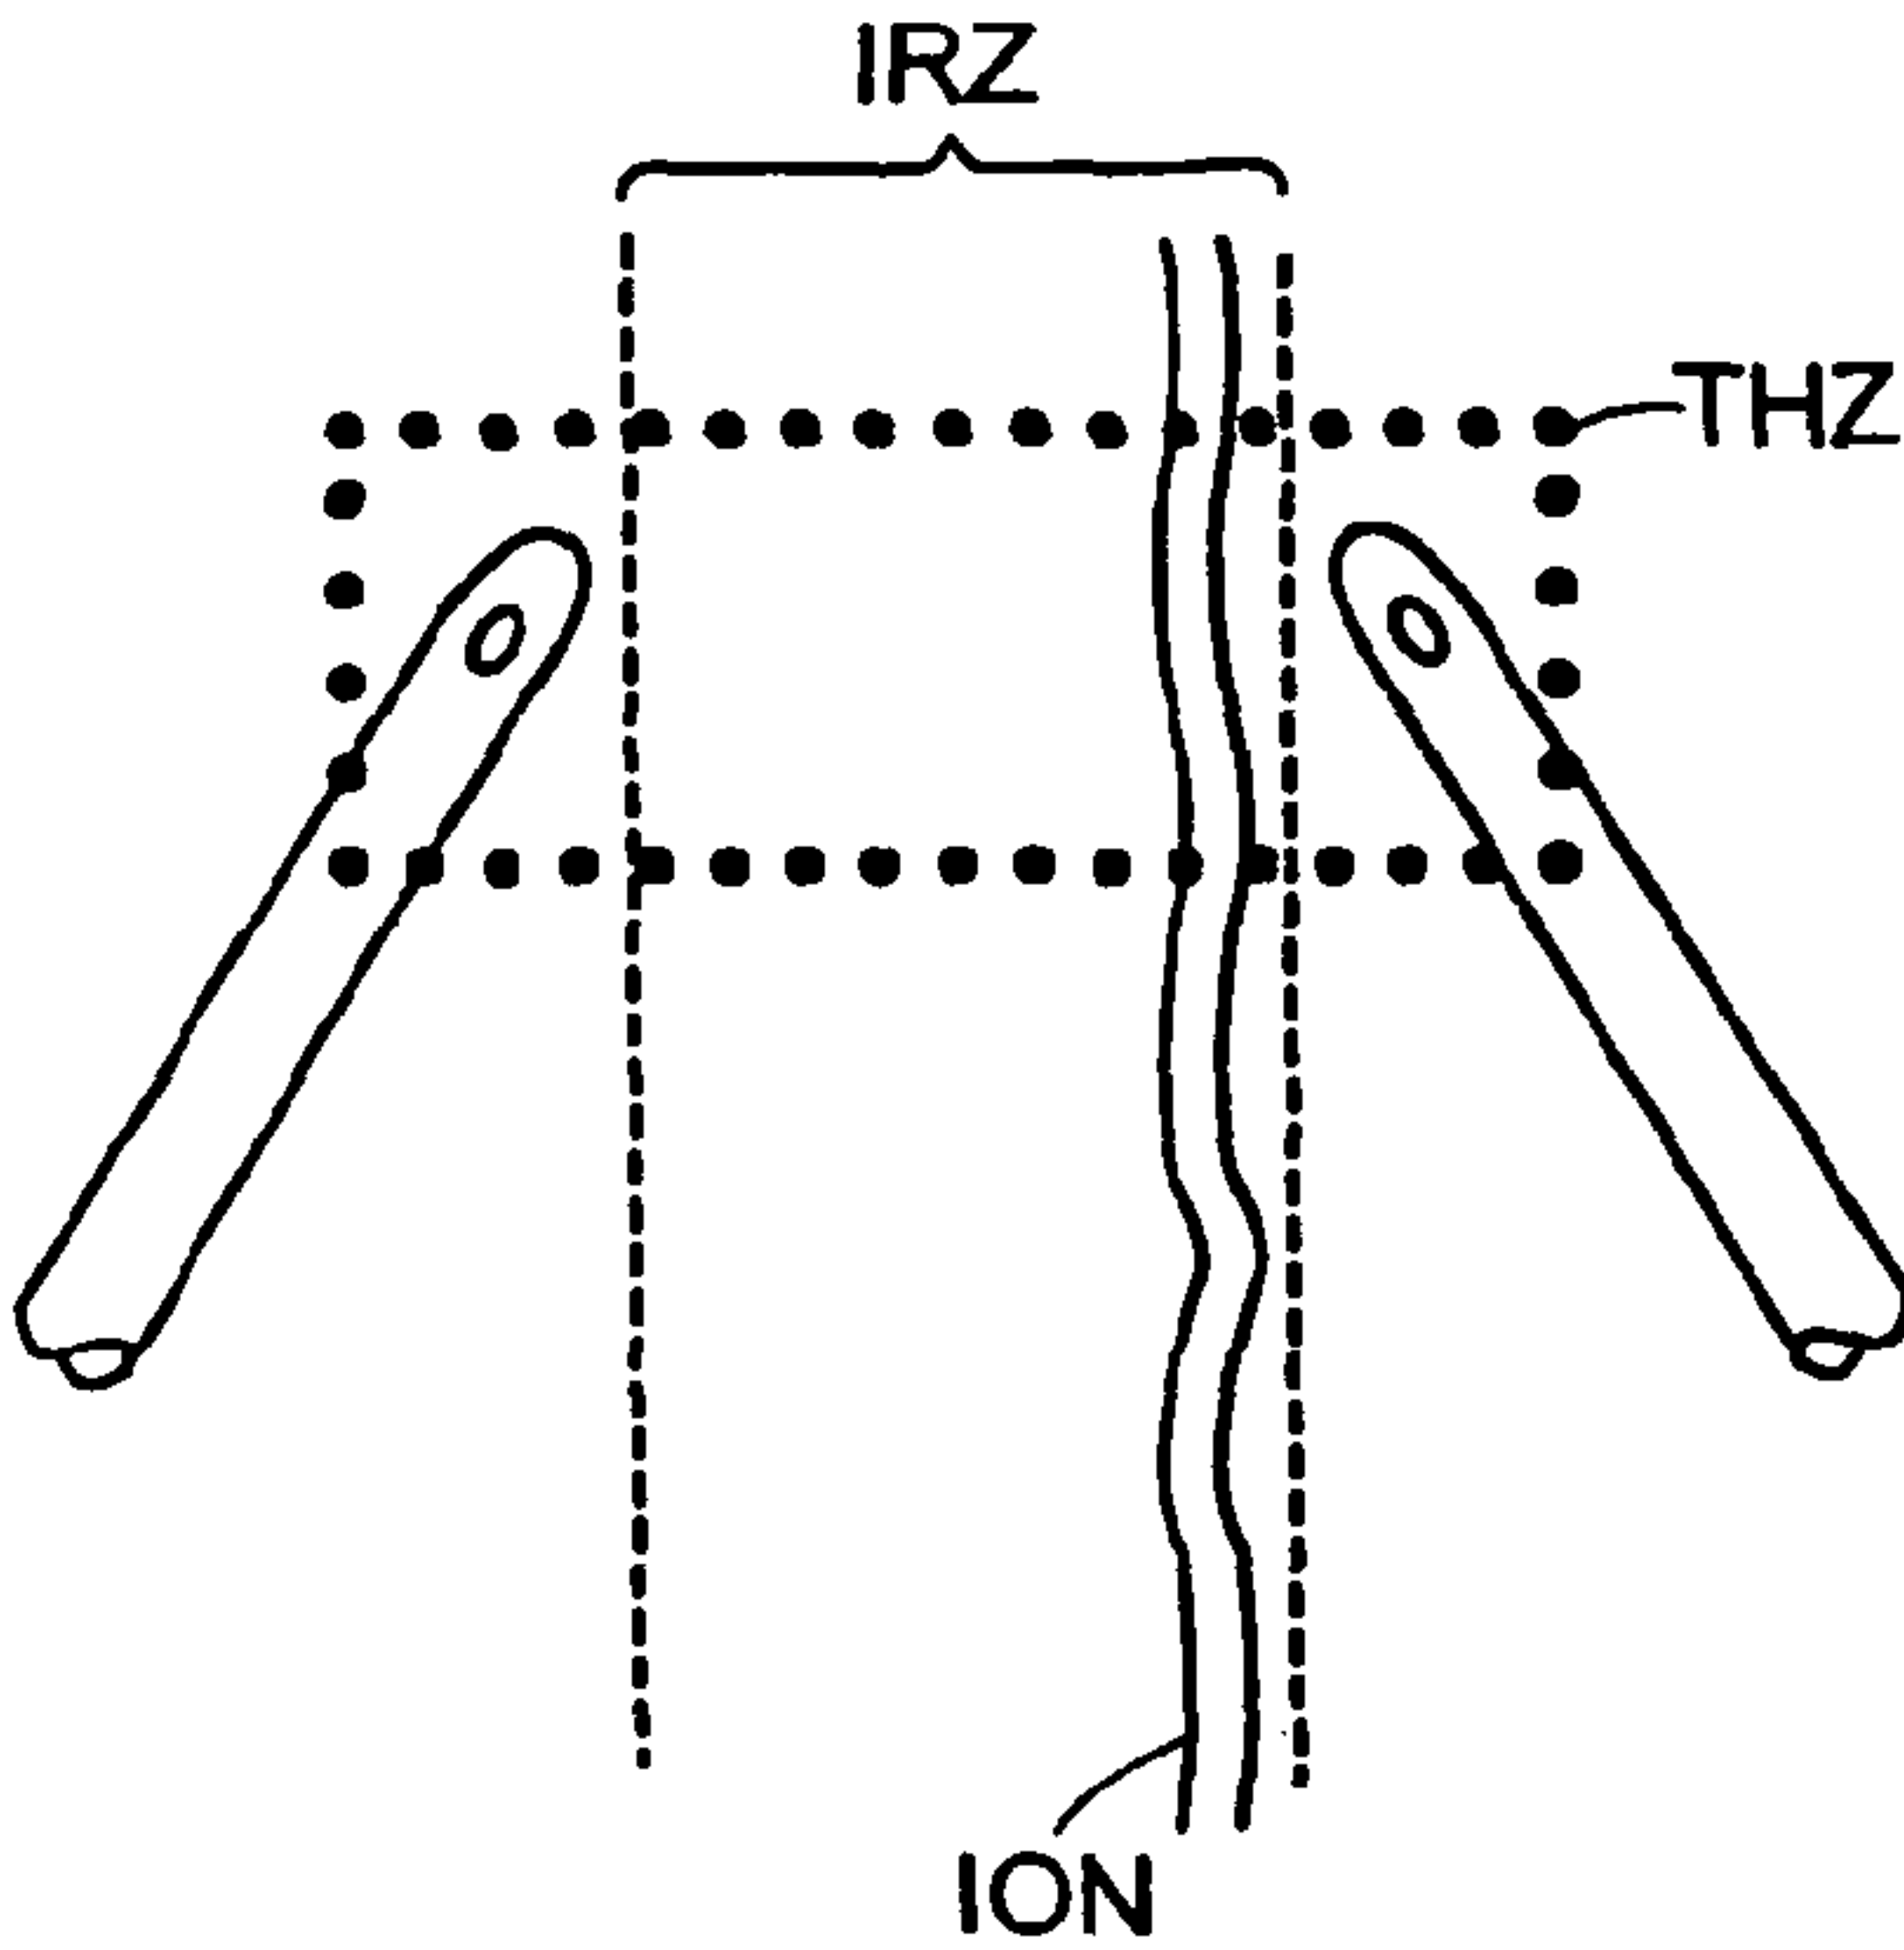


FIG. 8

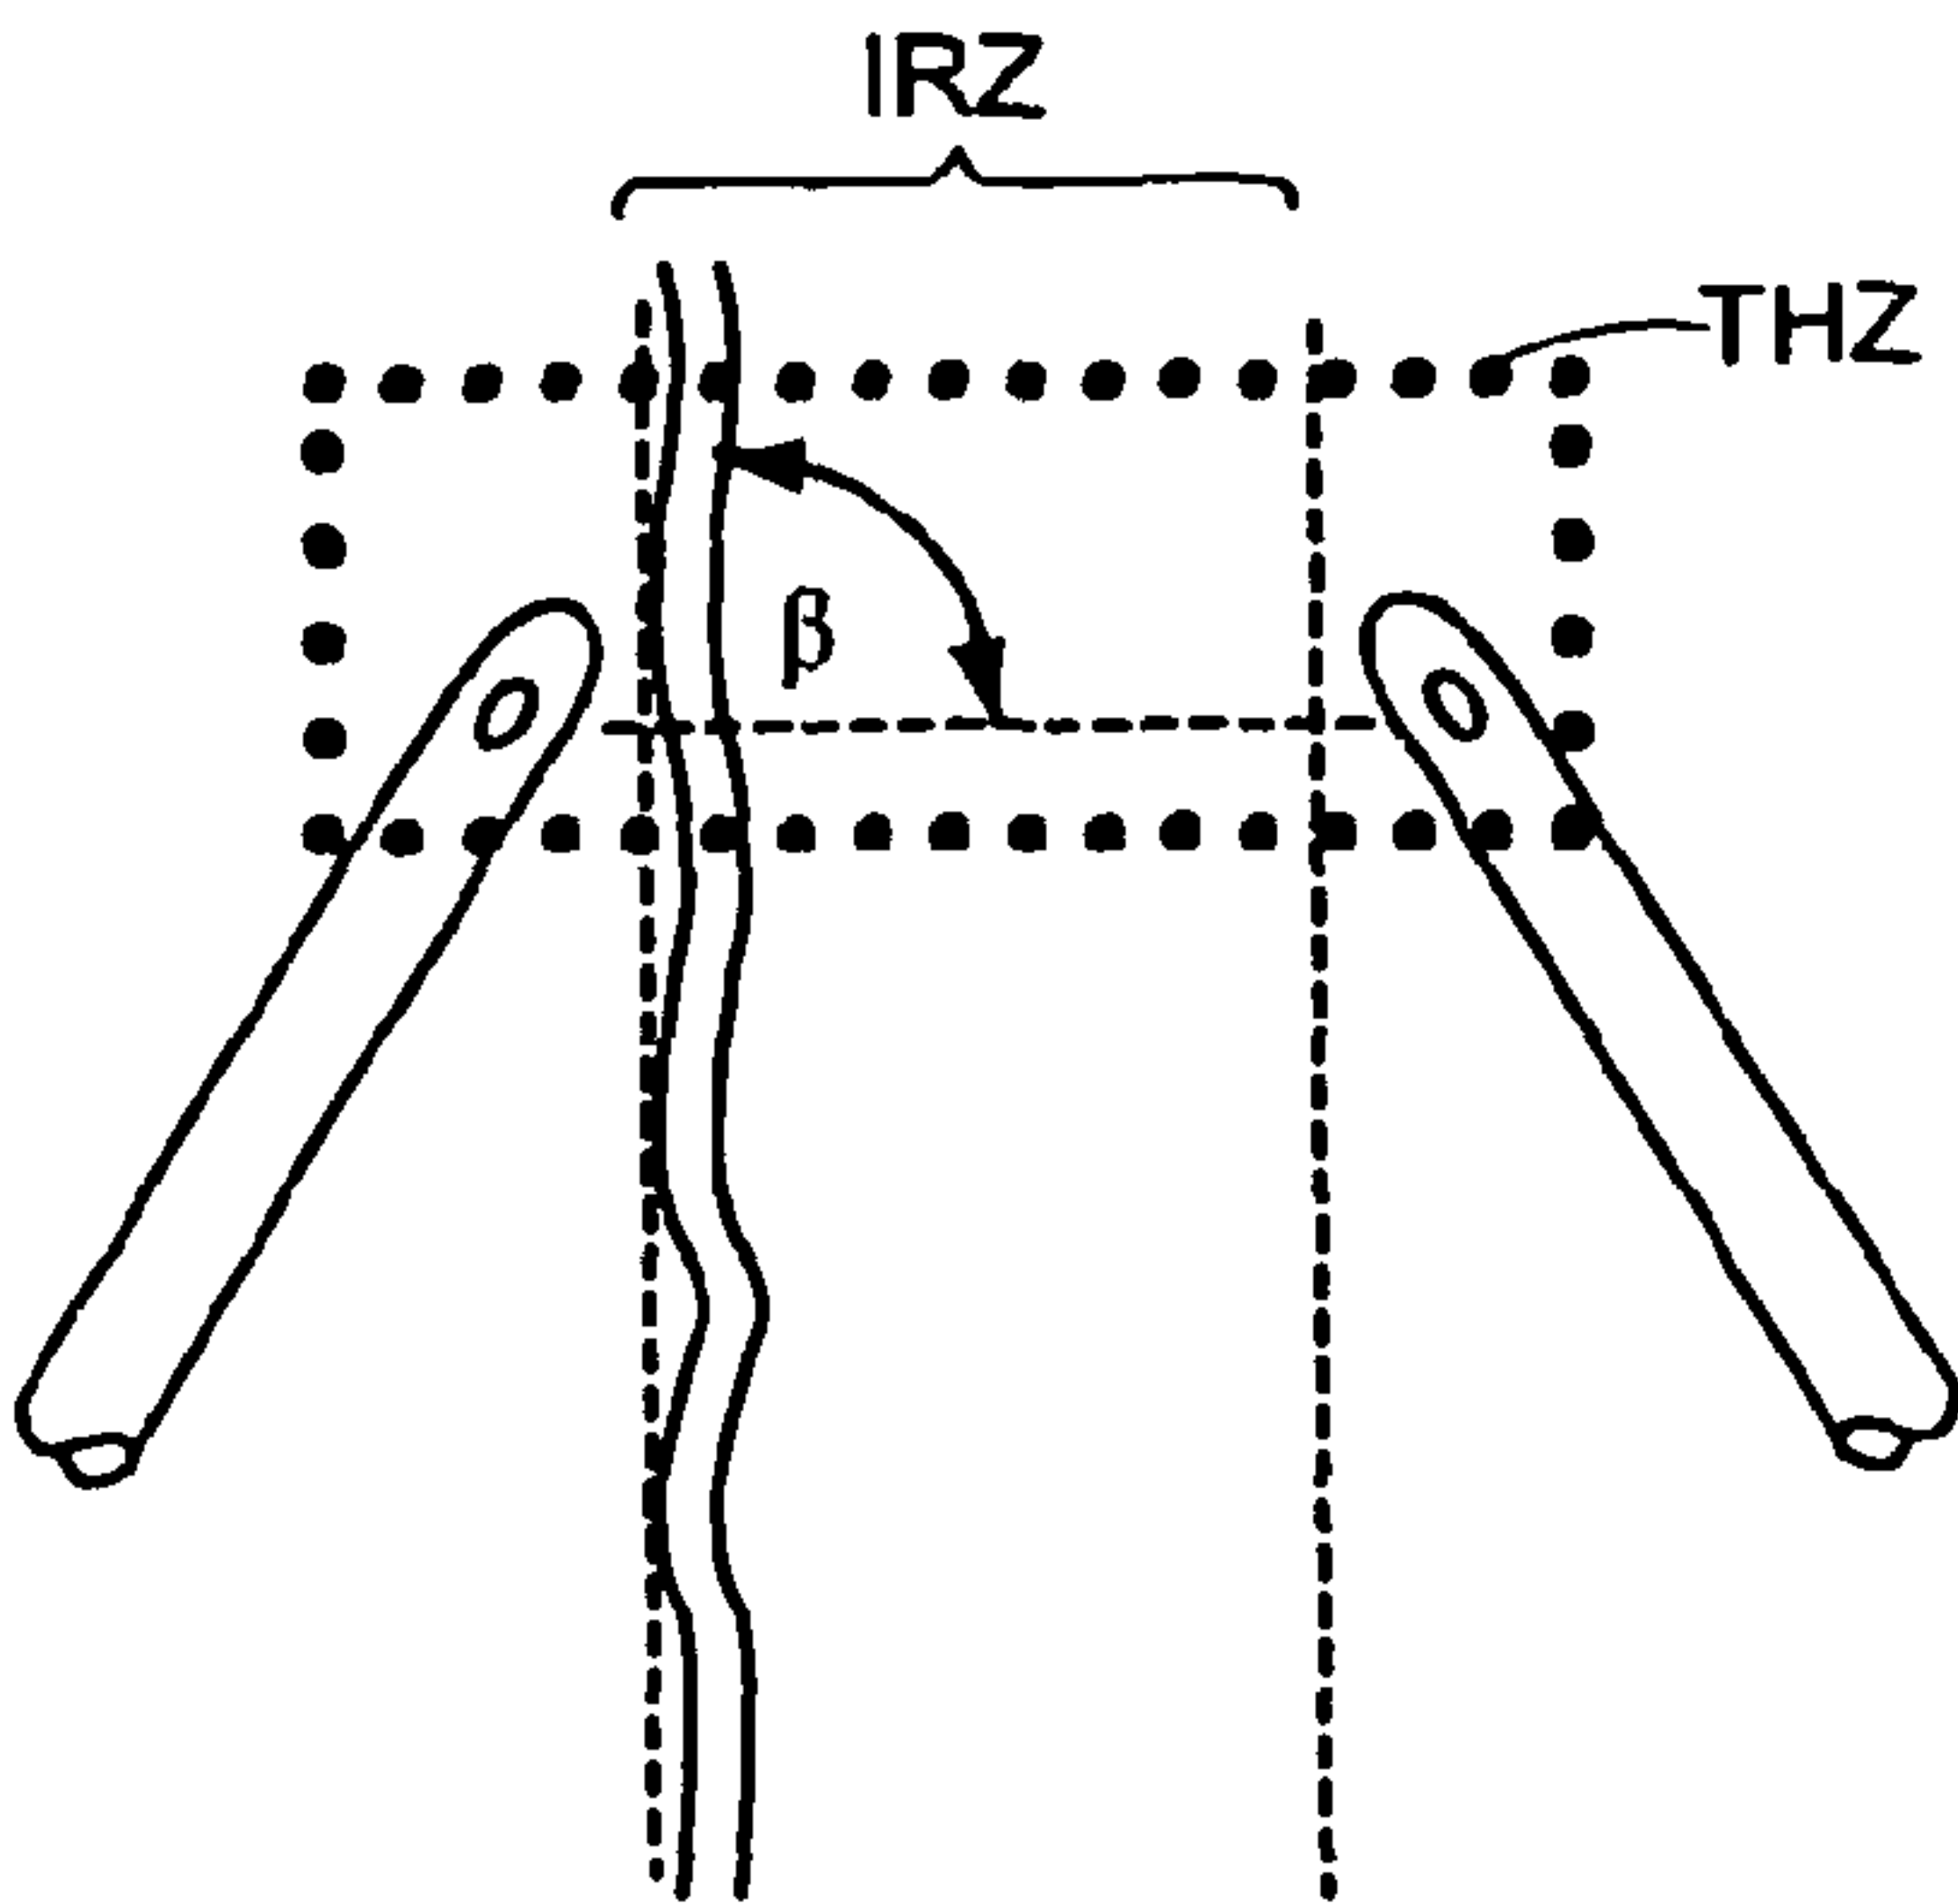


FIG. 9

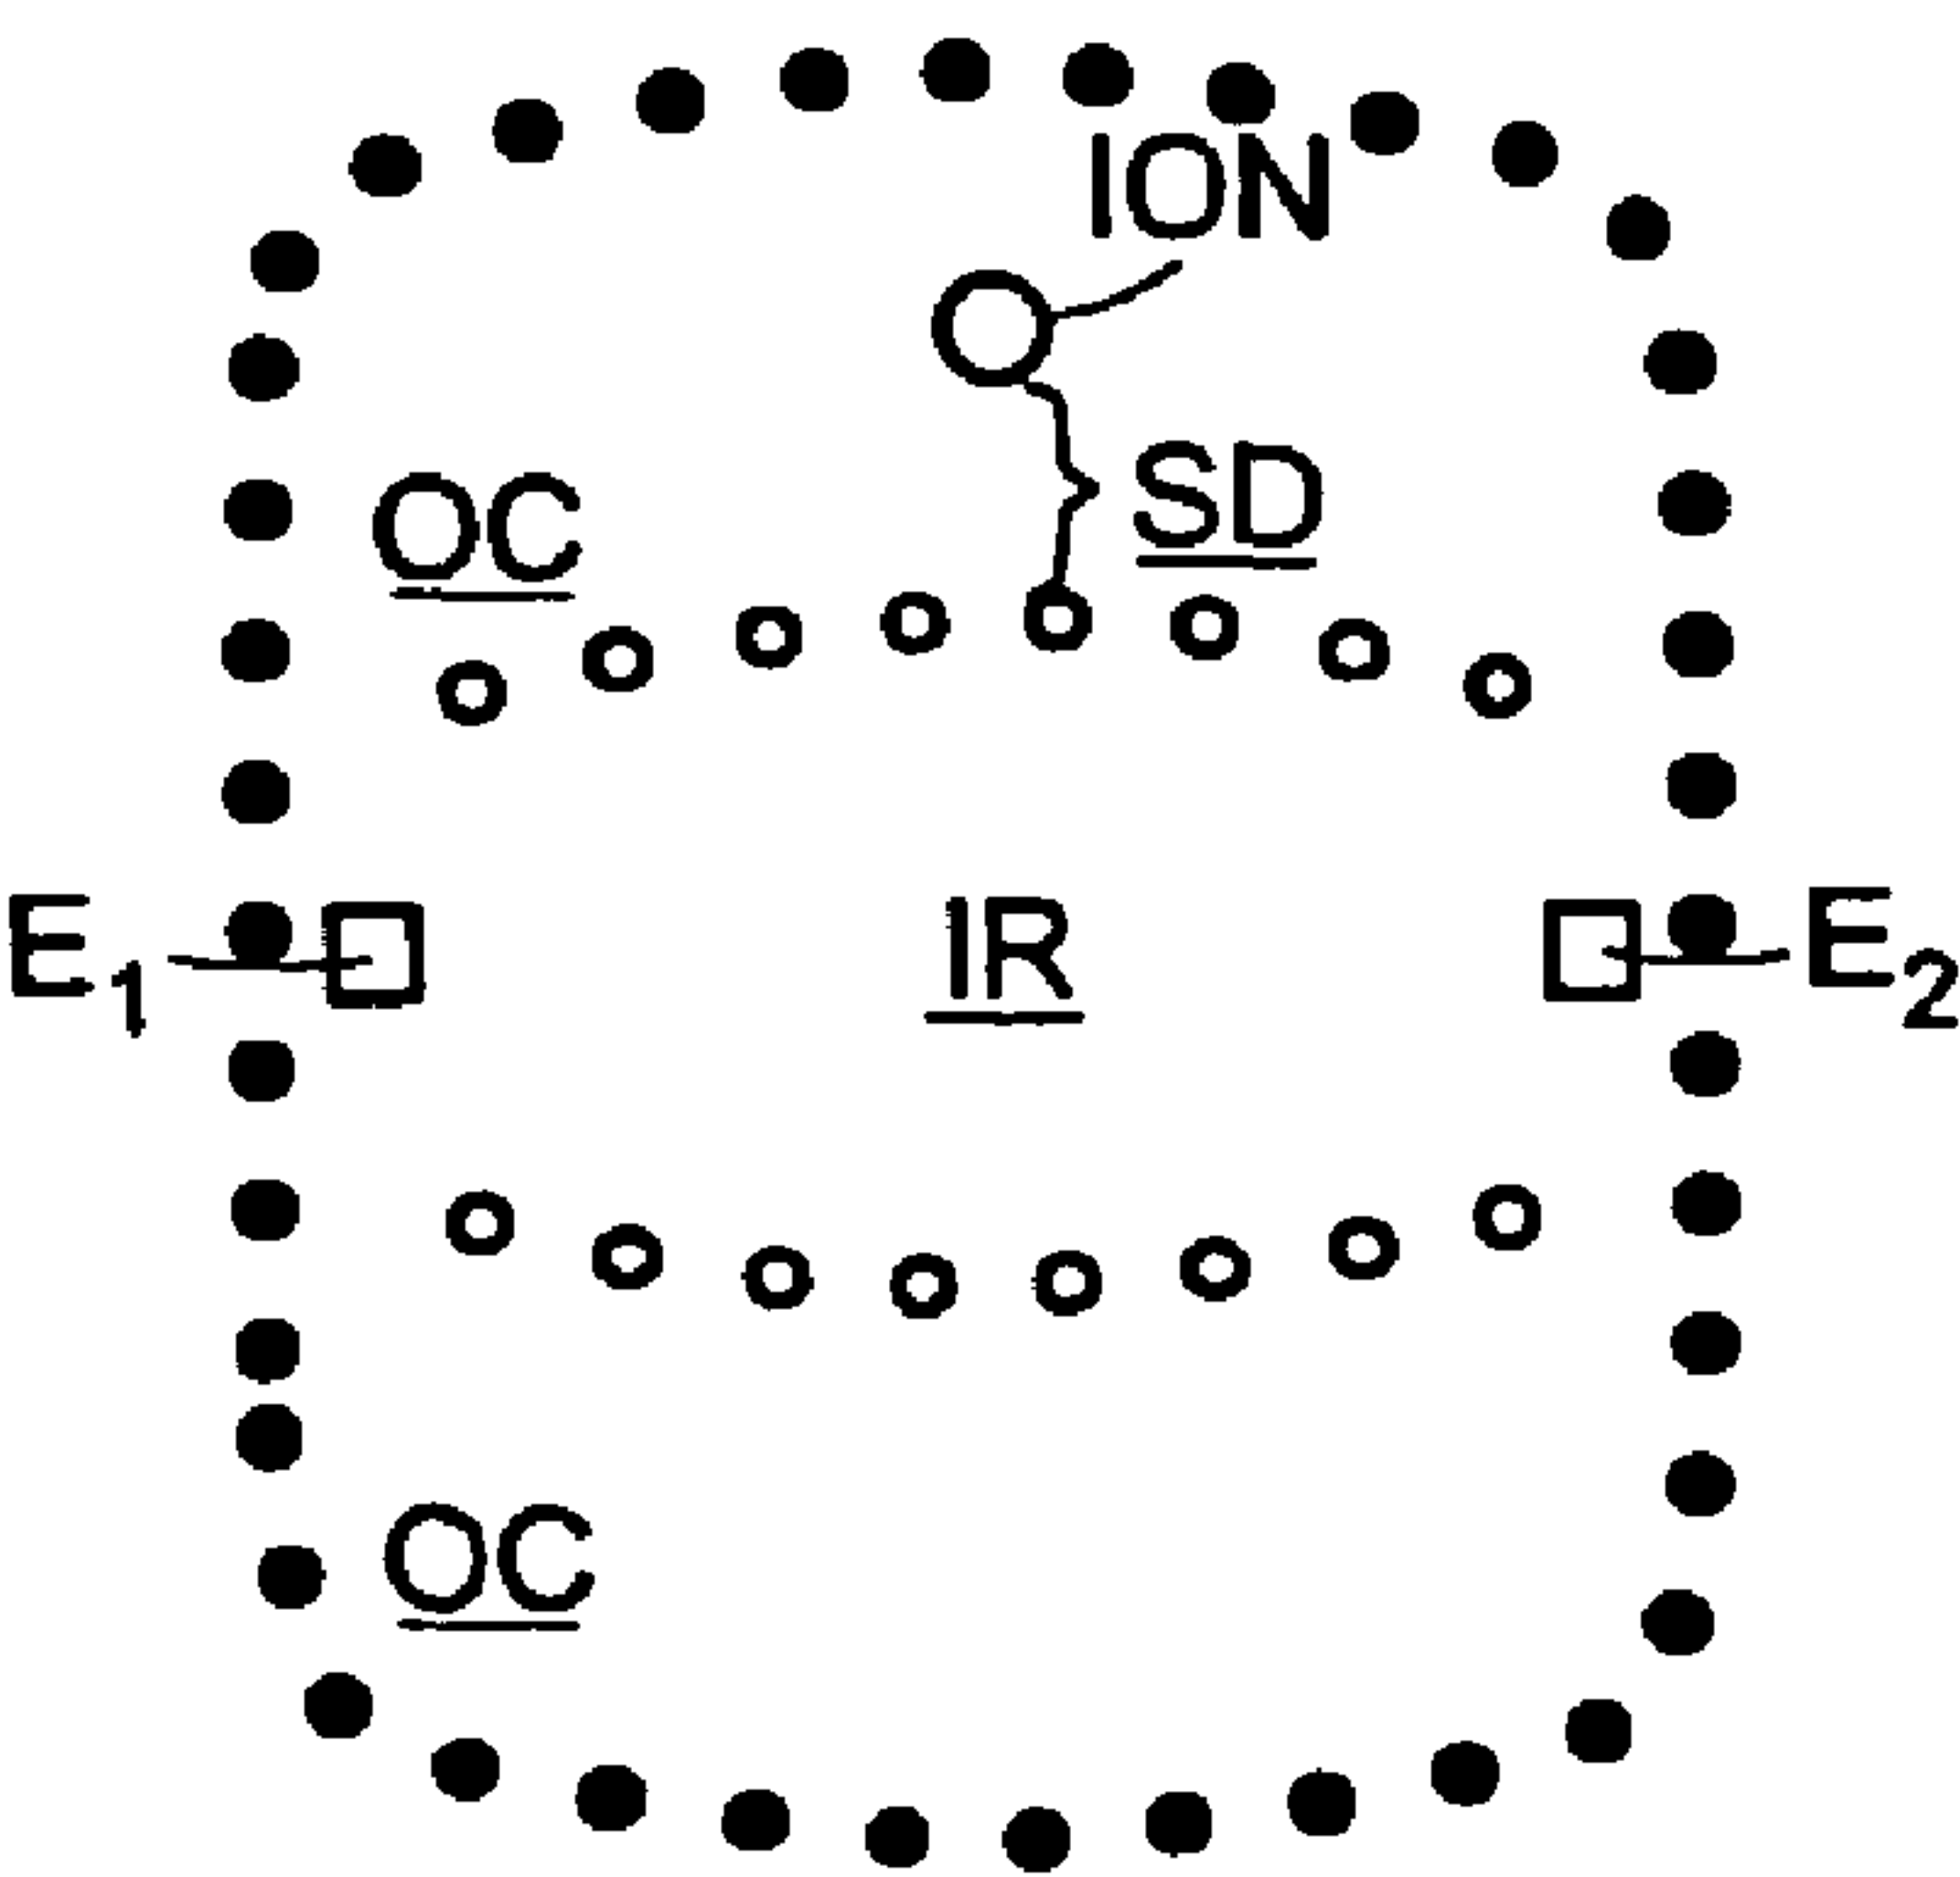


FIG. 10A

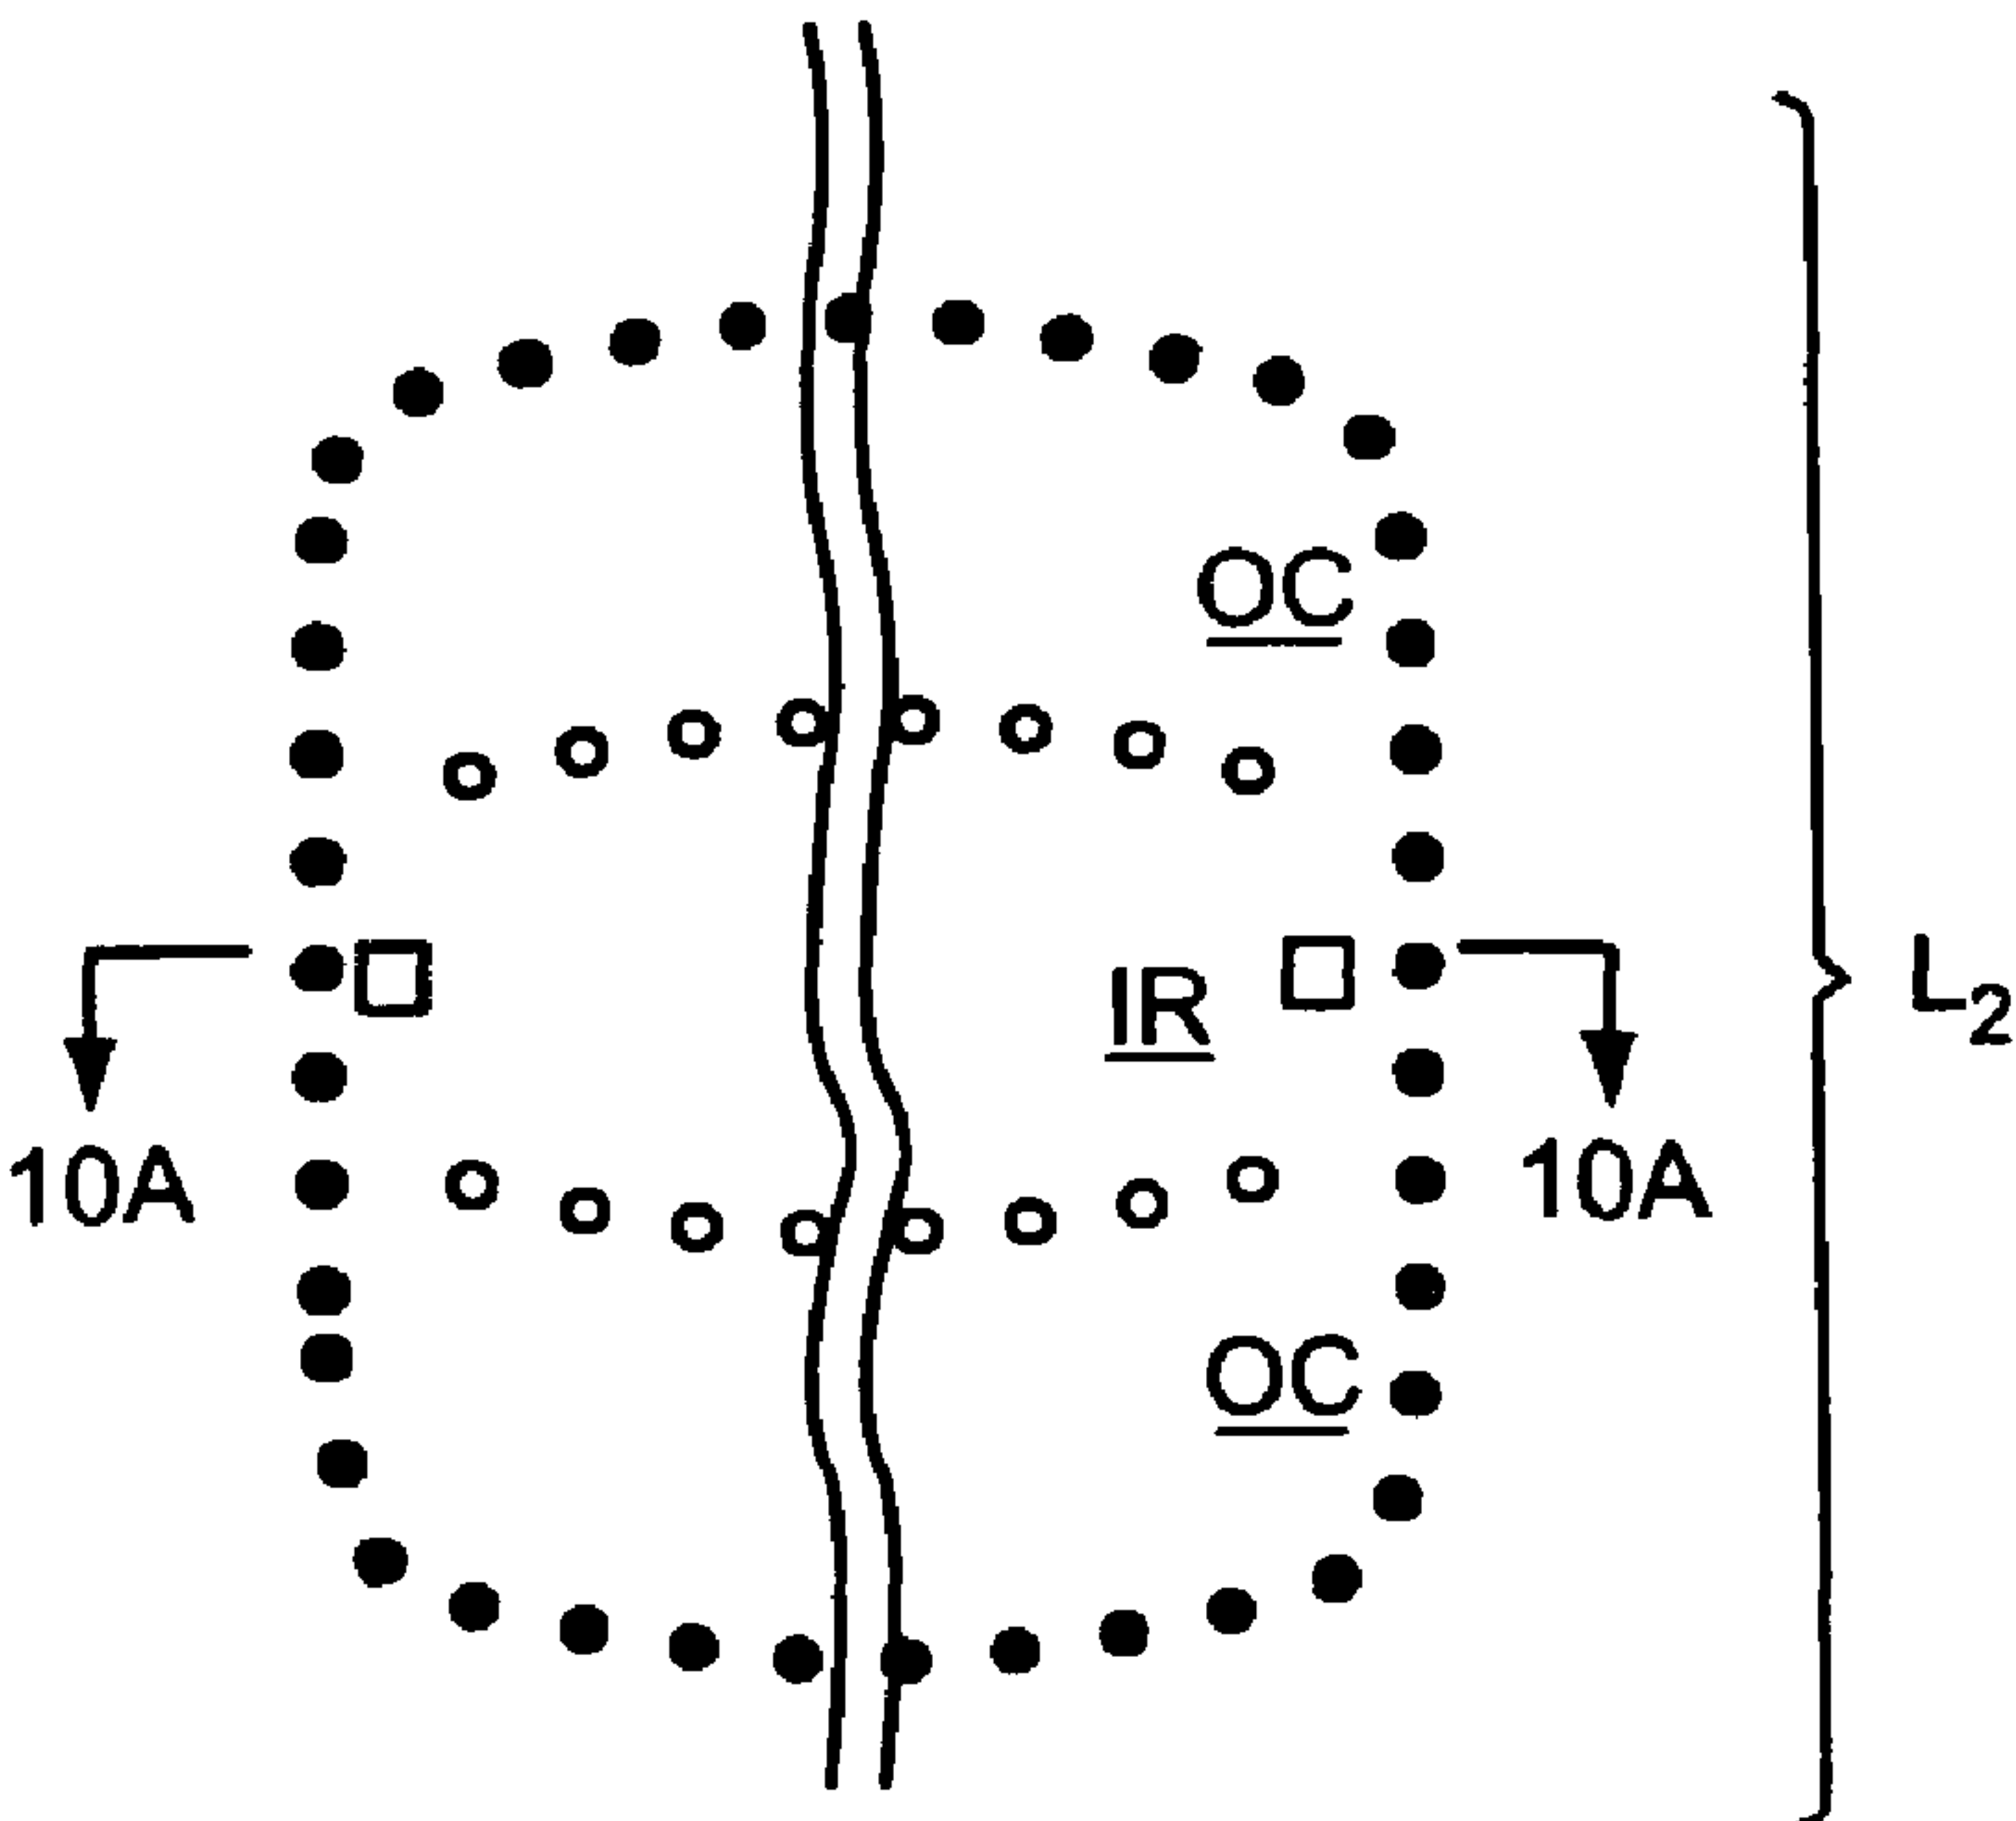


FIG. 10B

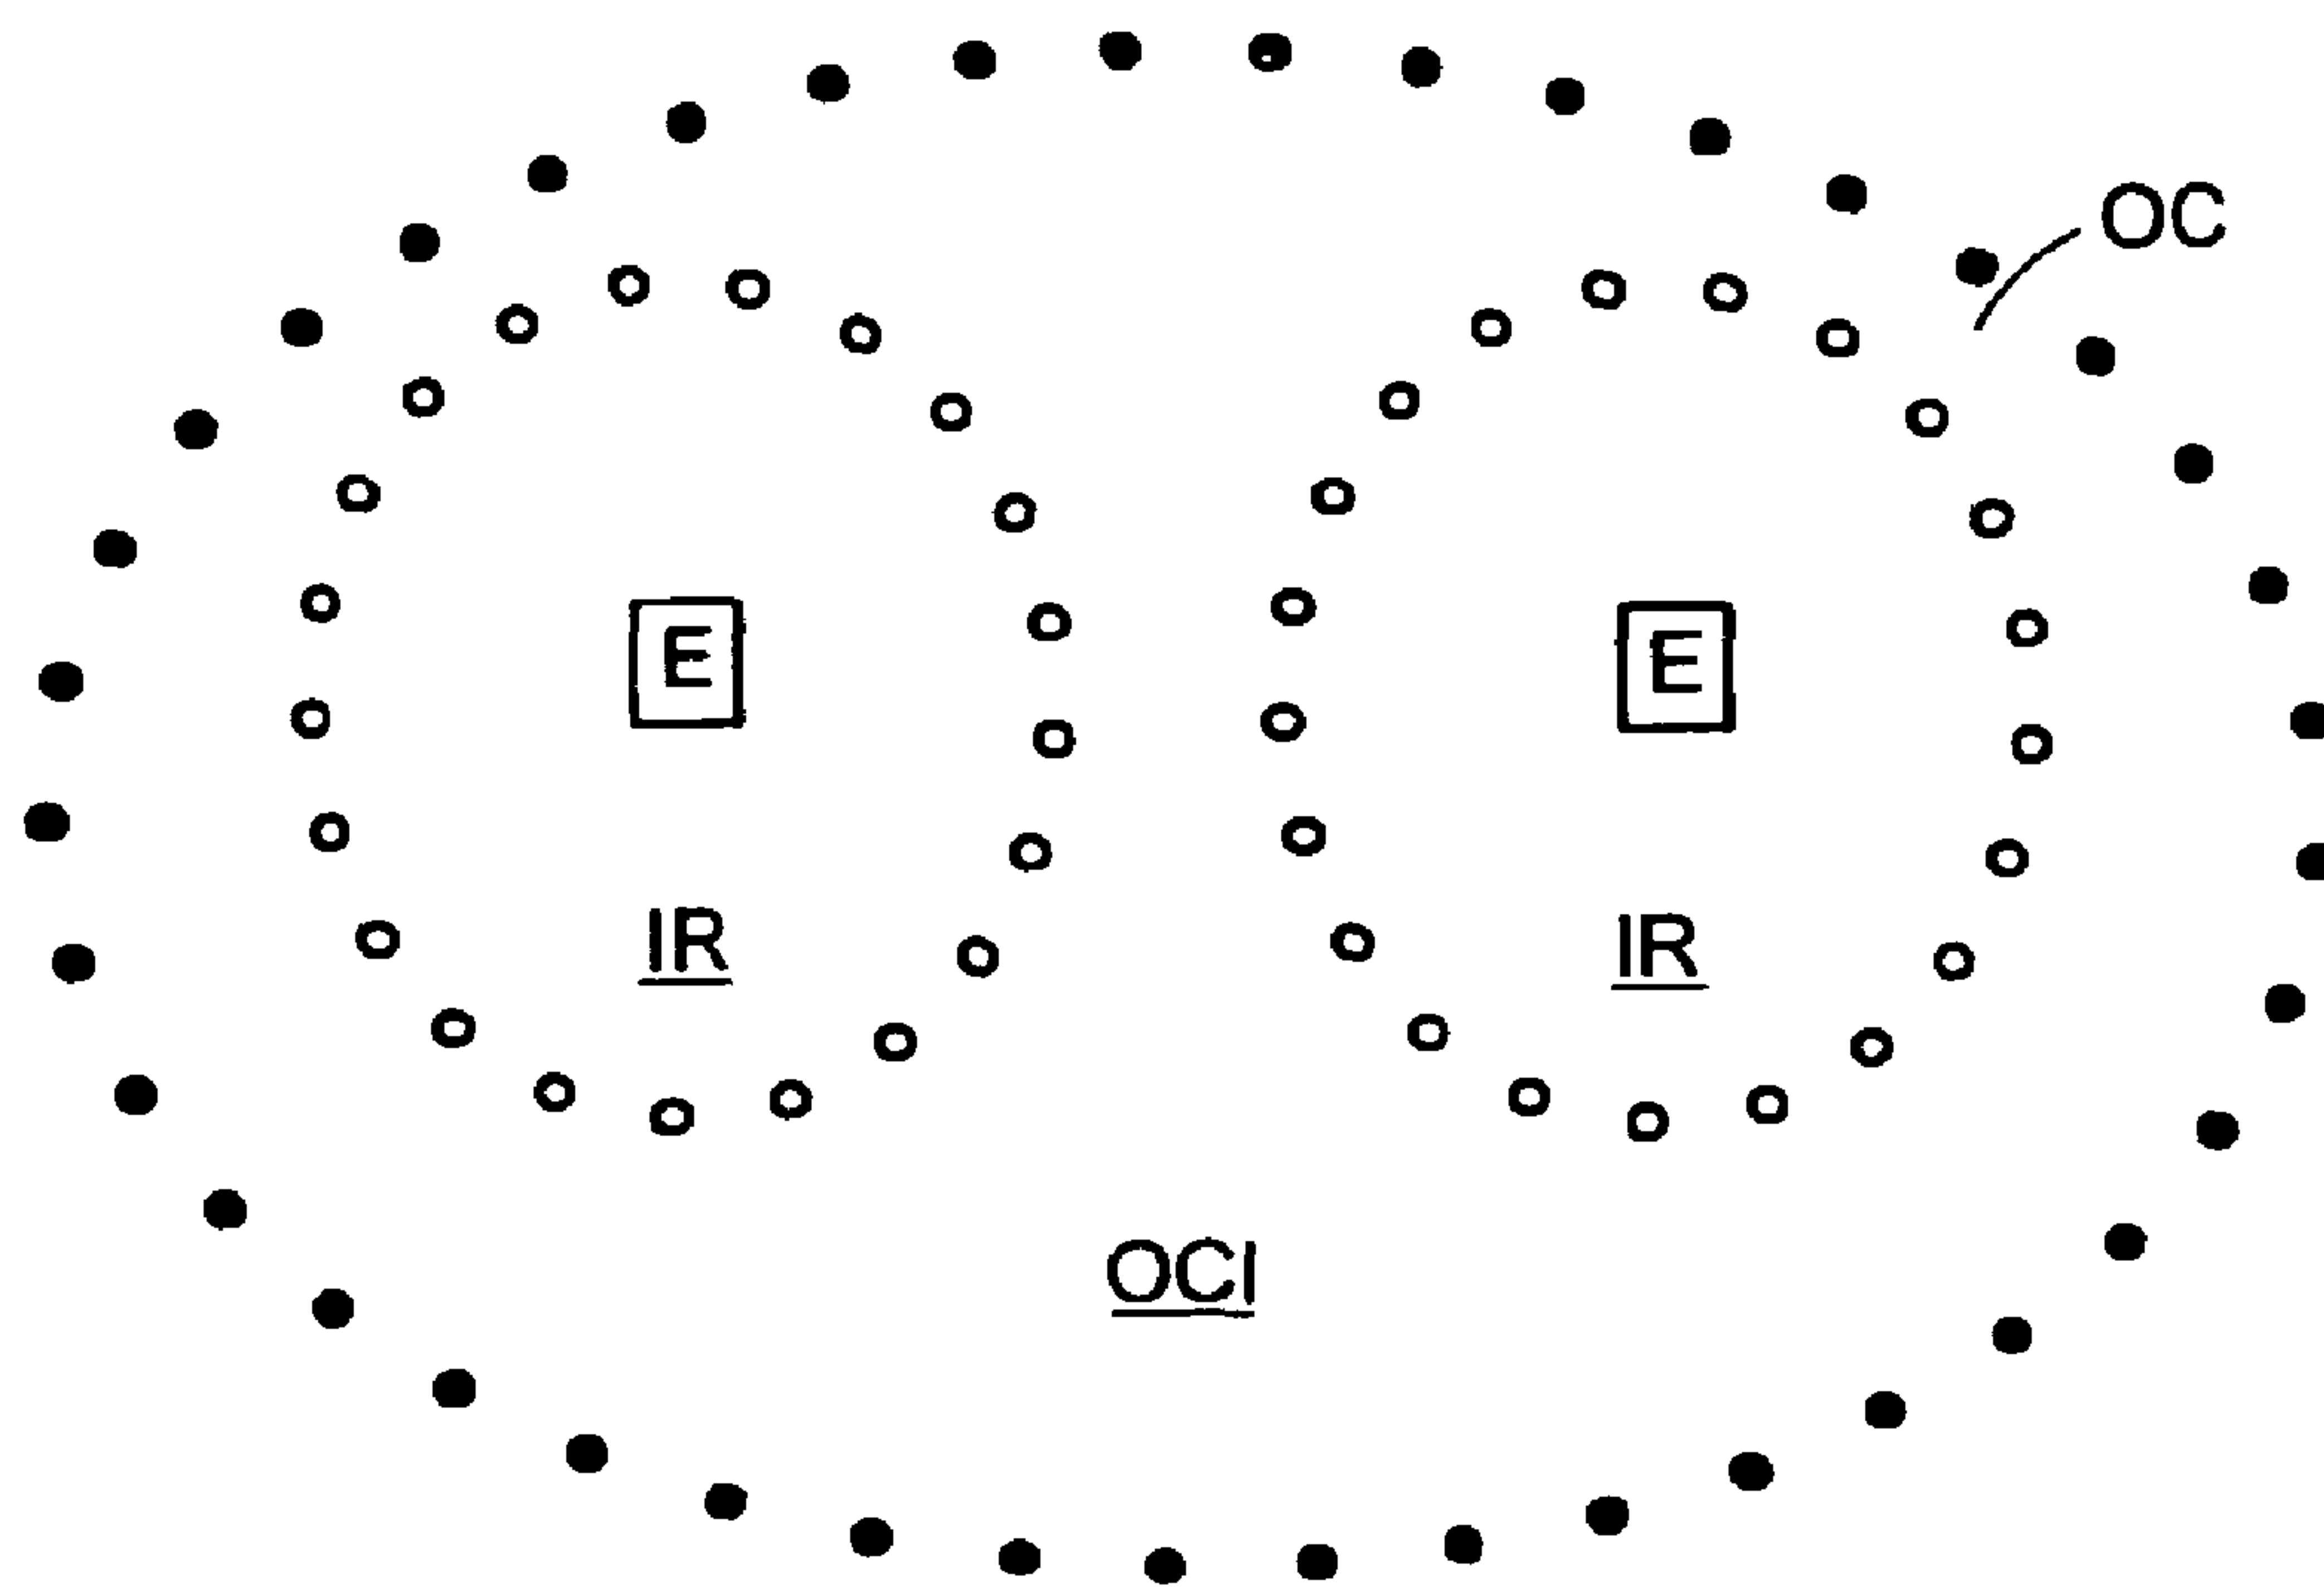


FIG. 11

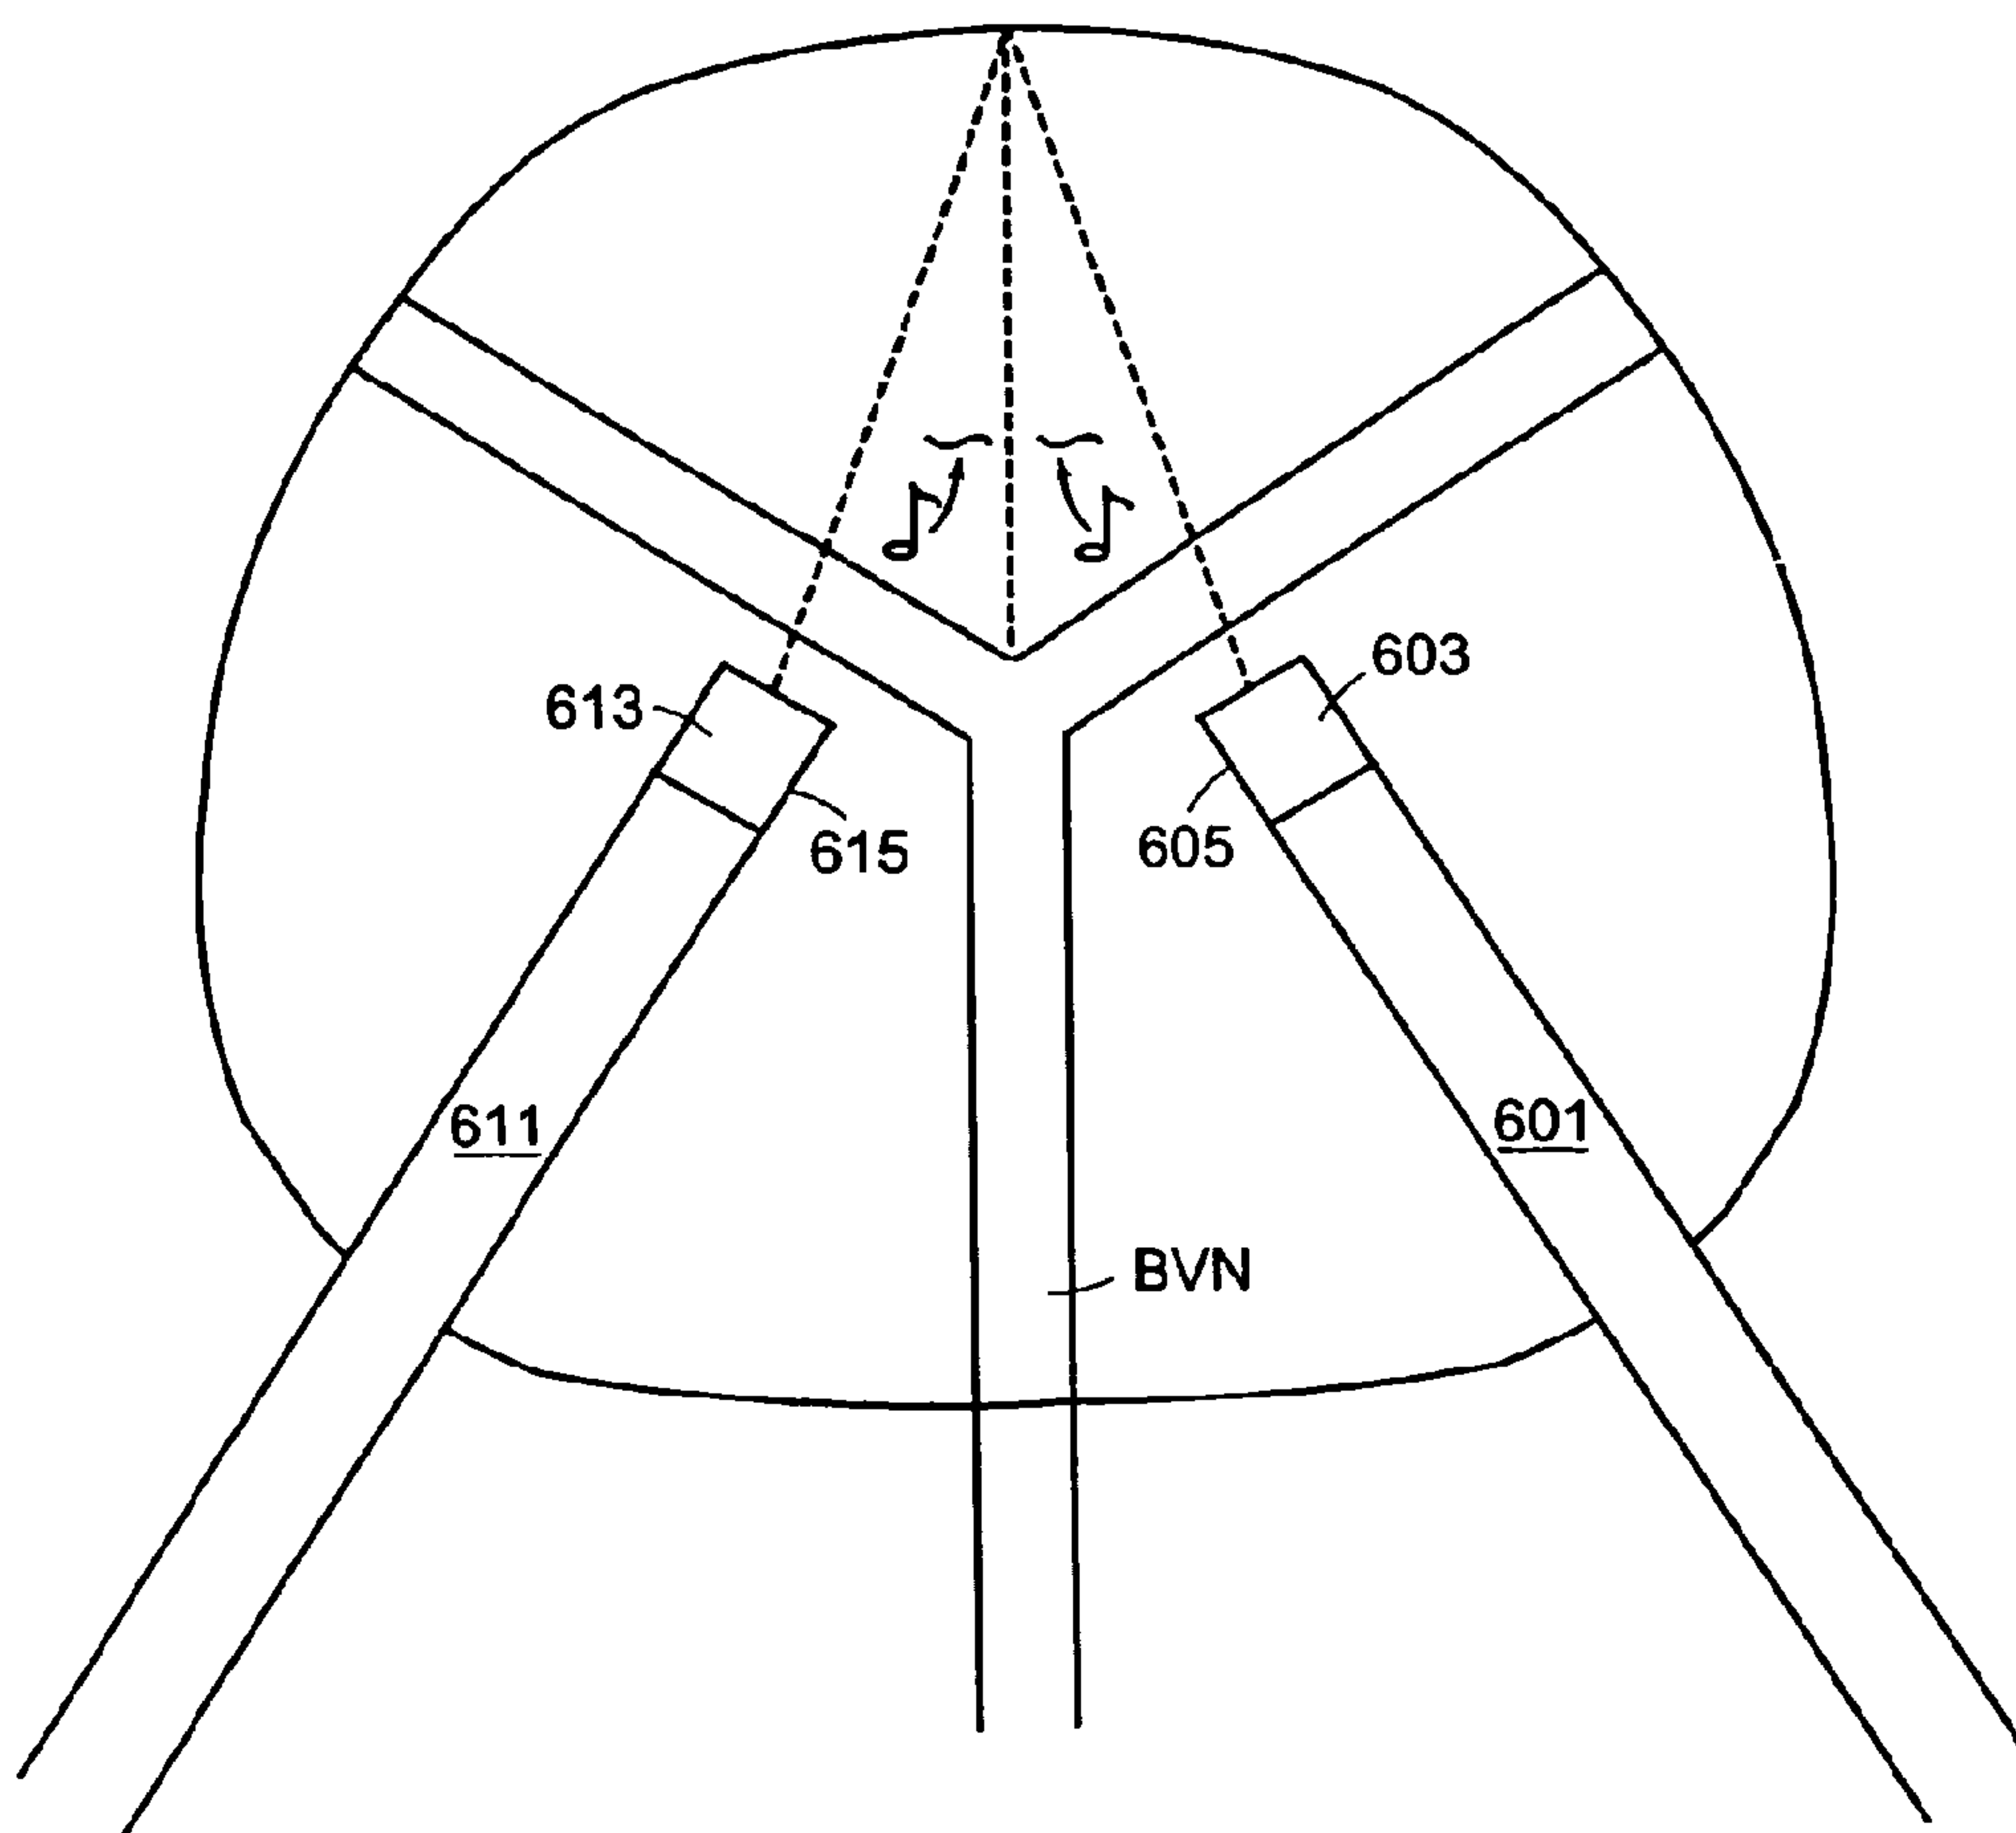


FIG. 12

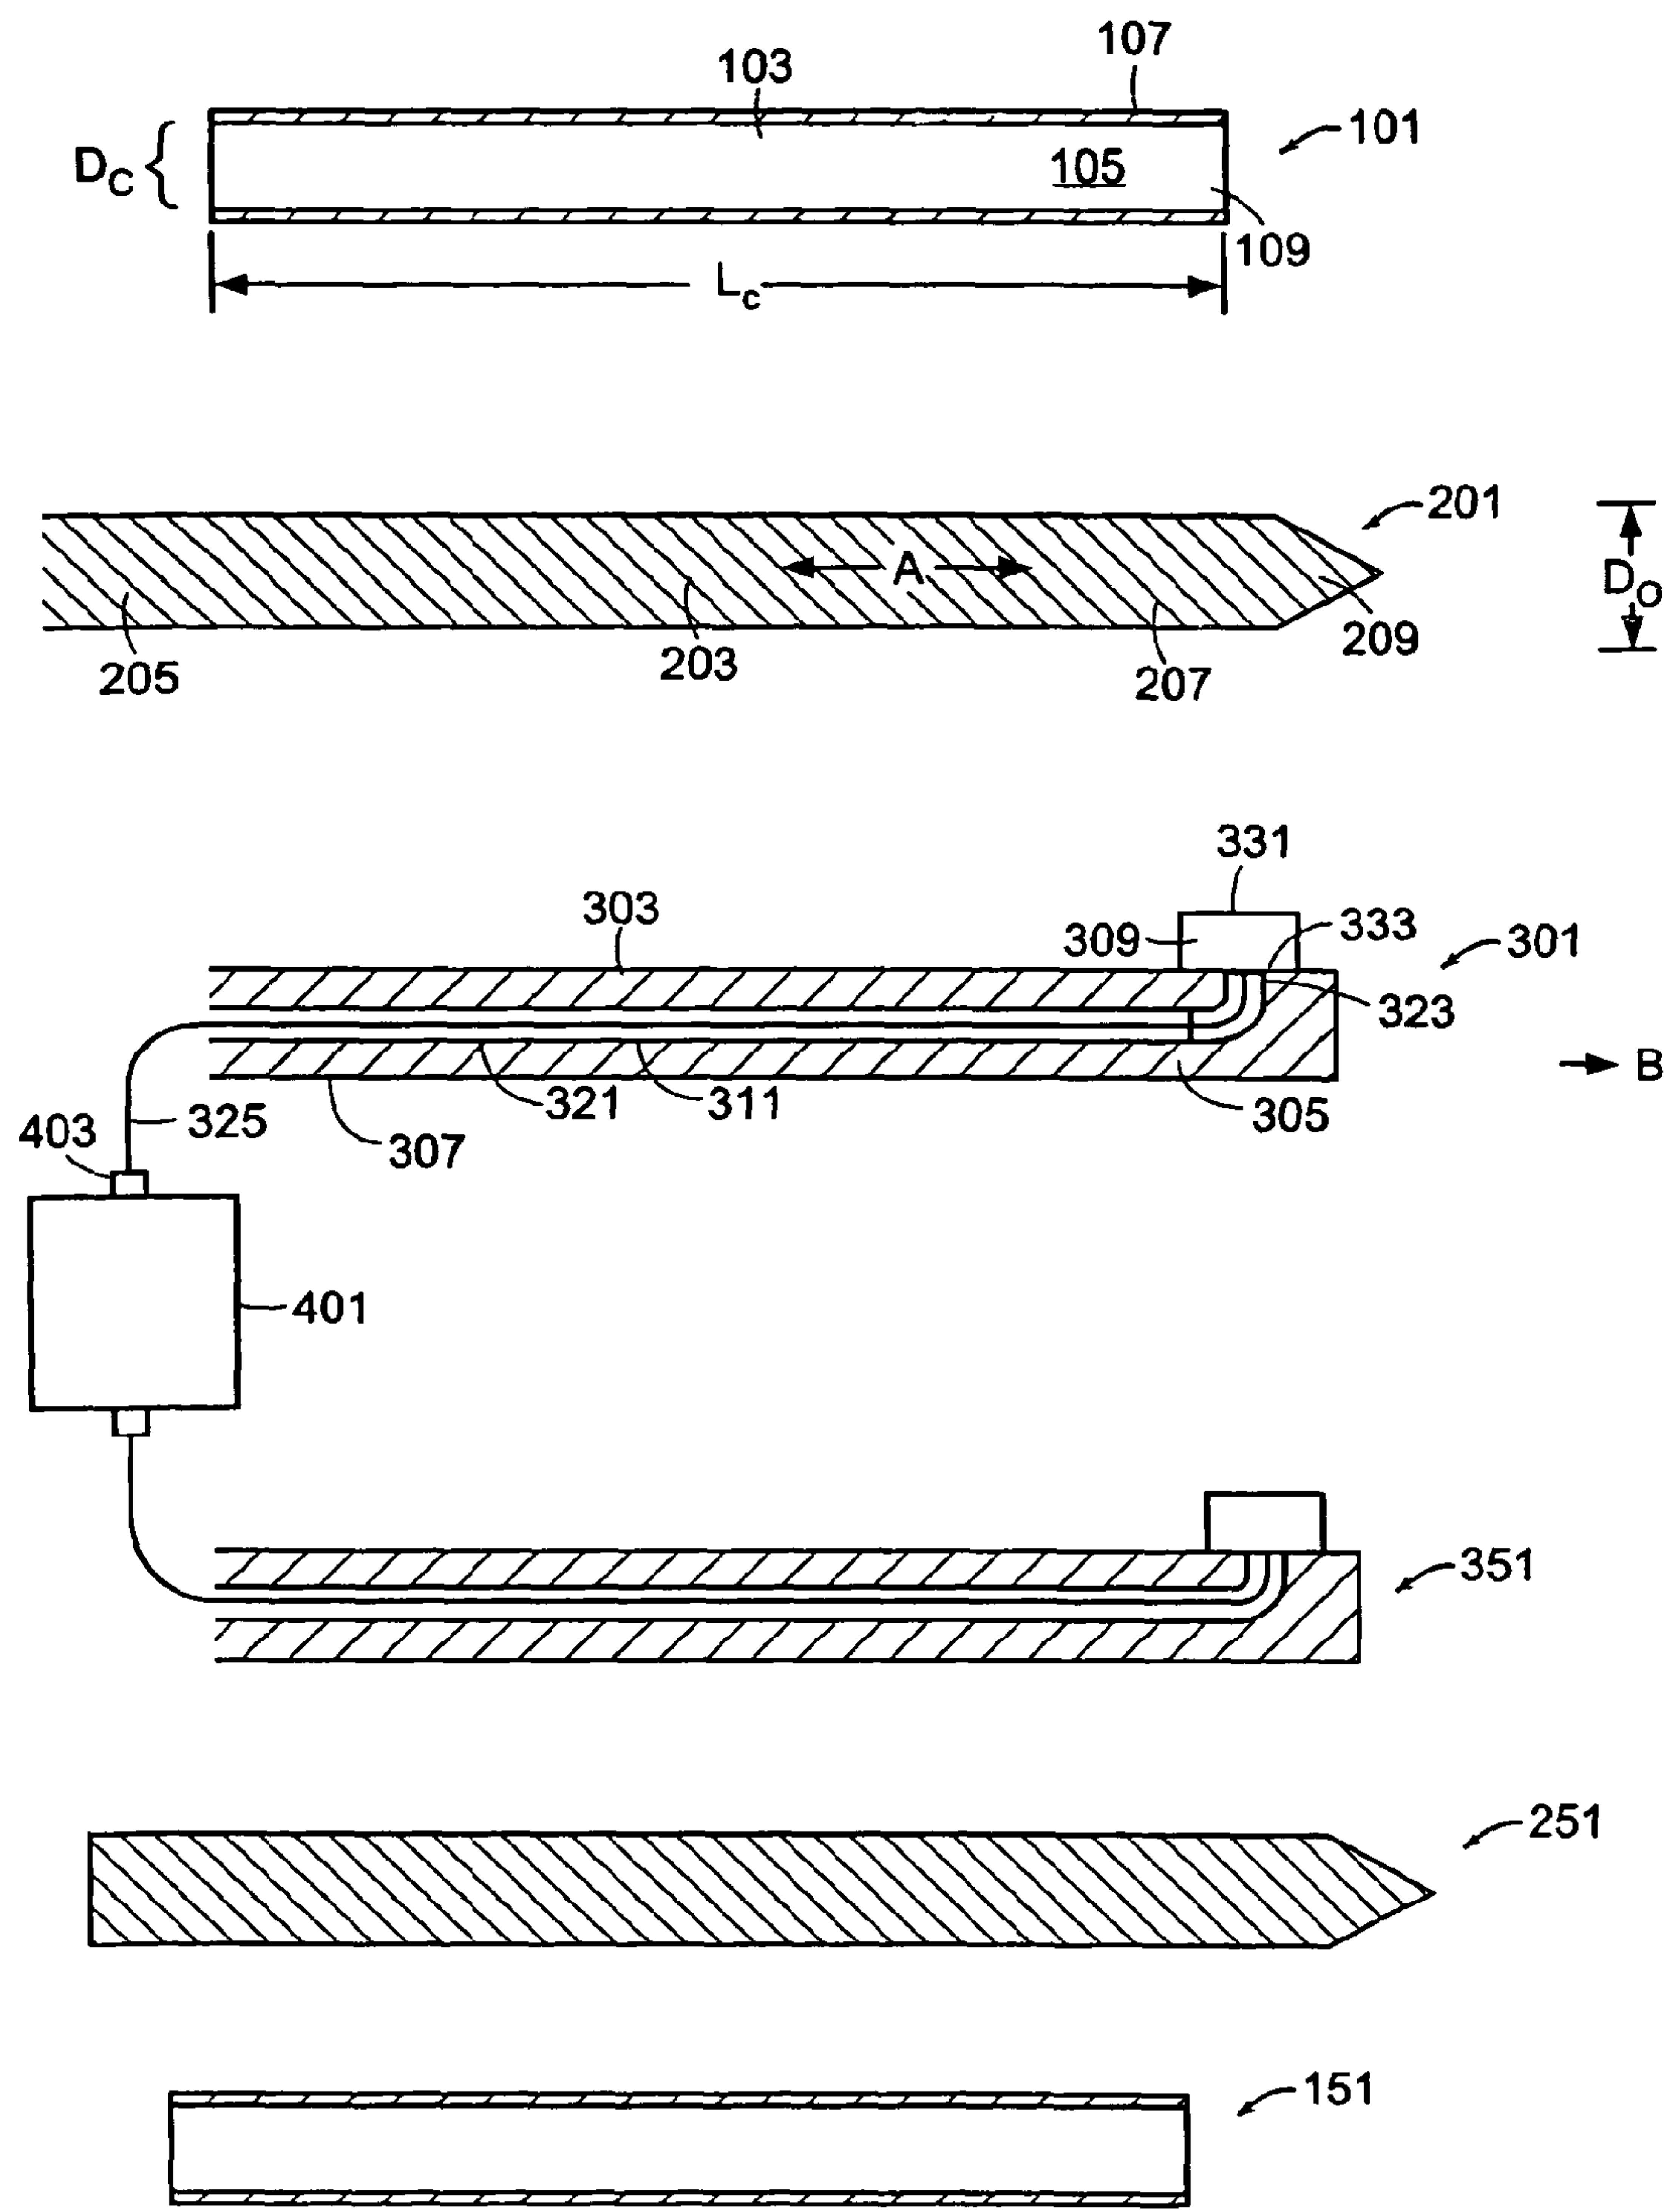


FIG. 13

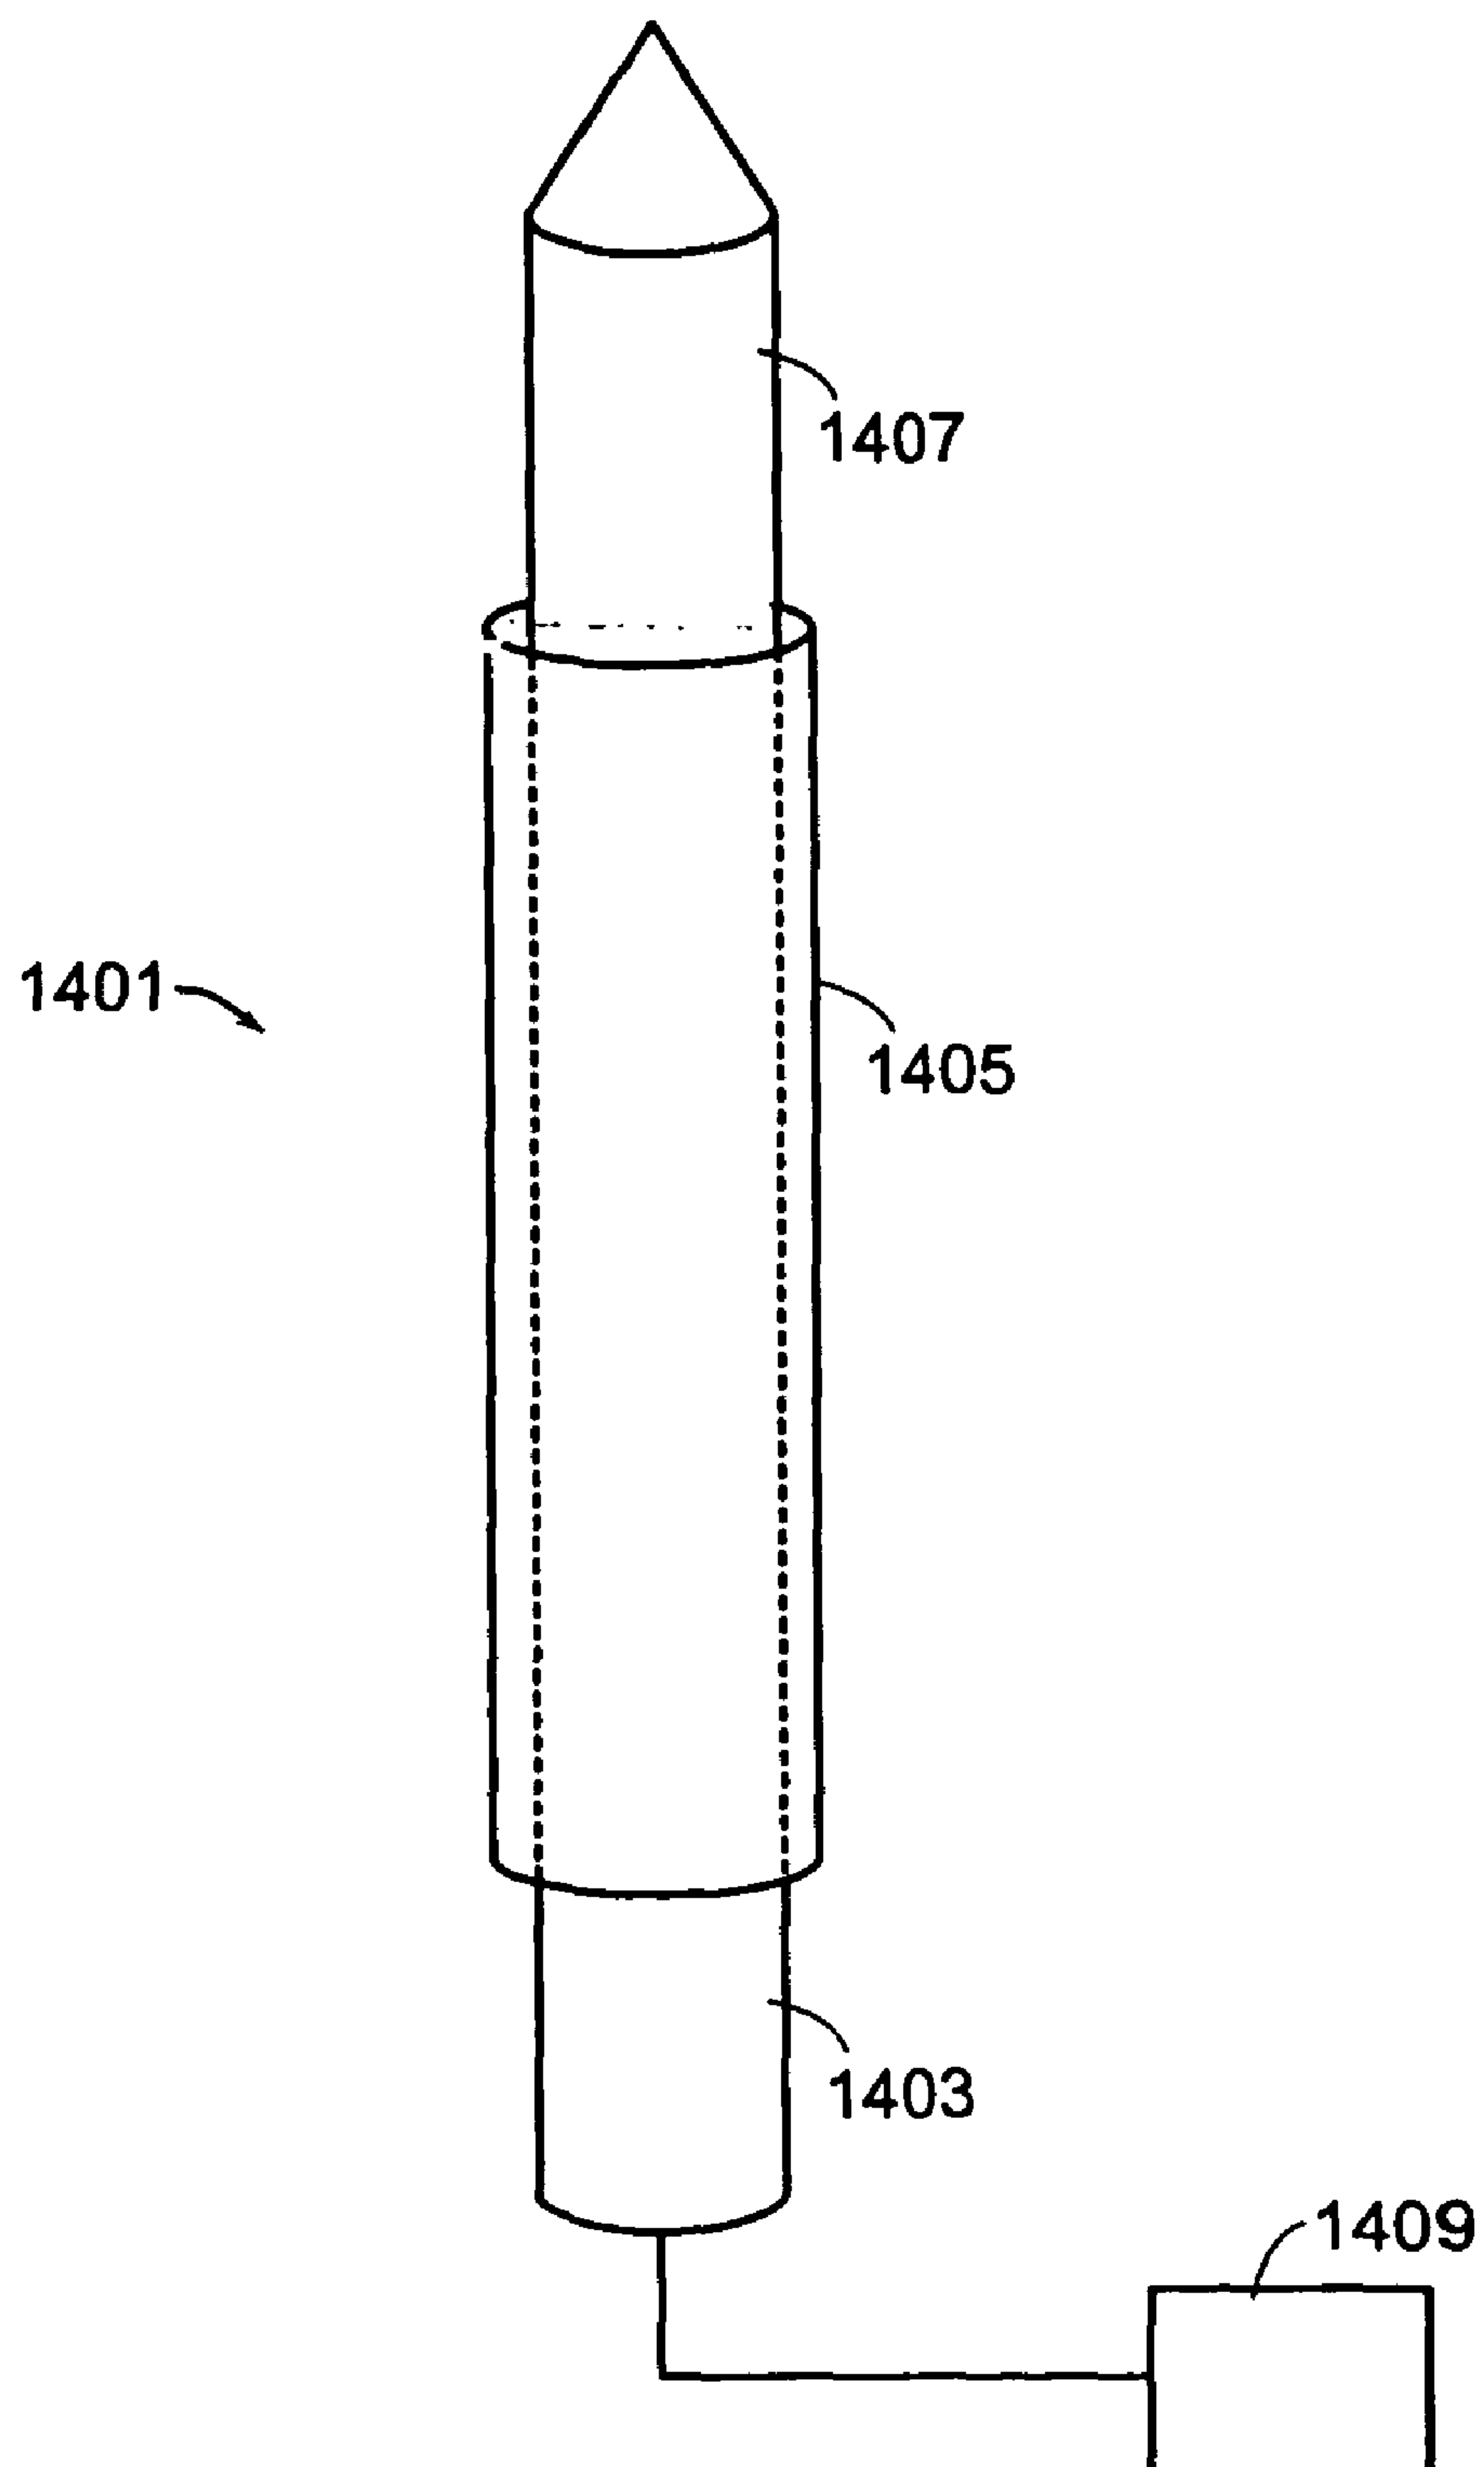


FIG. 14

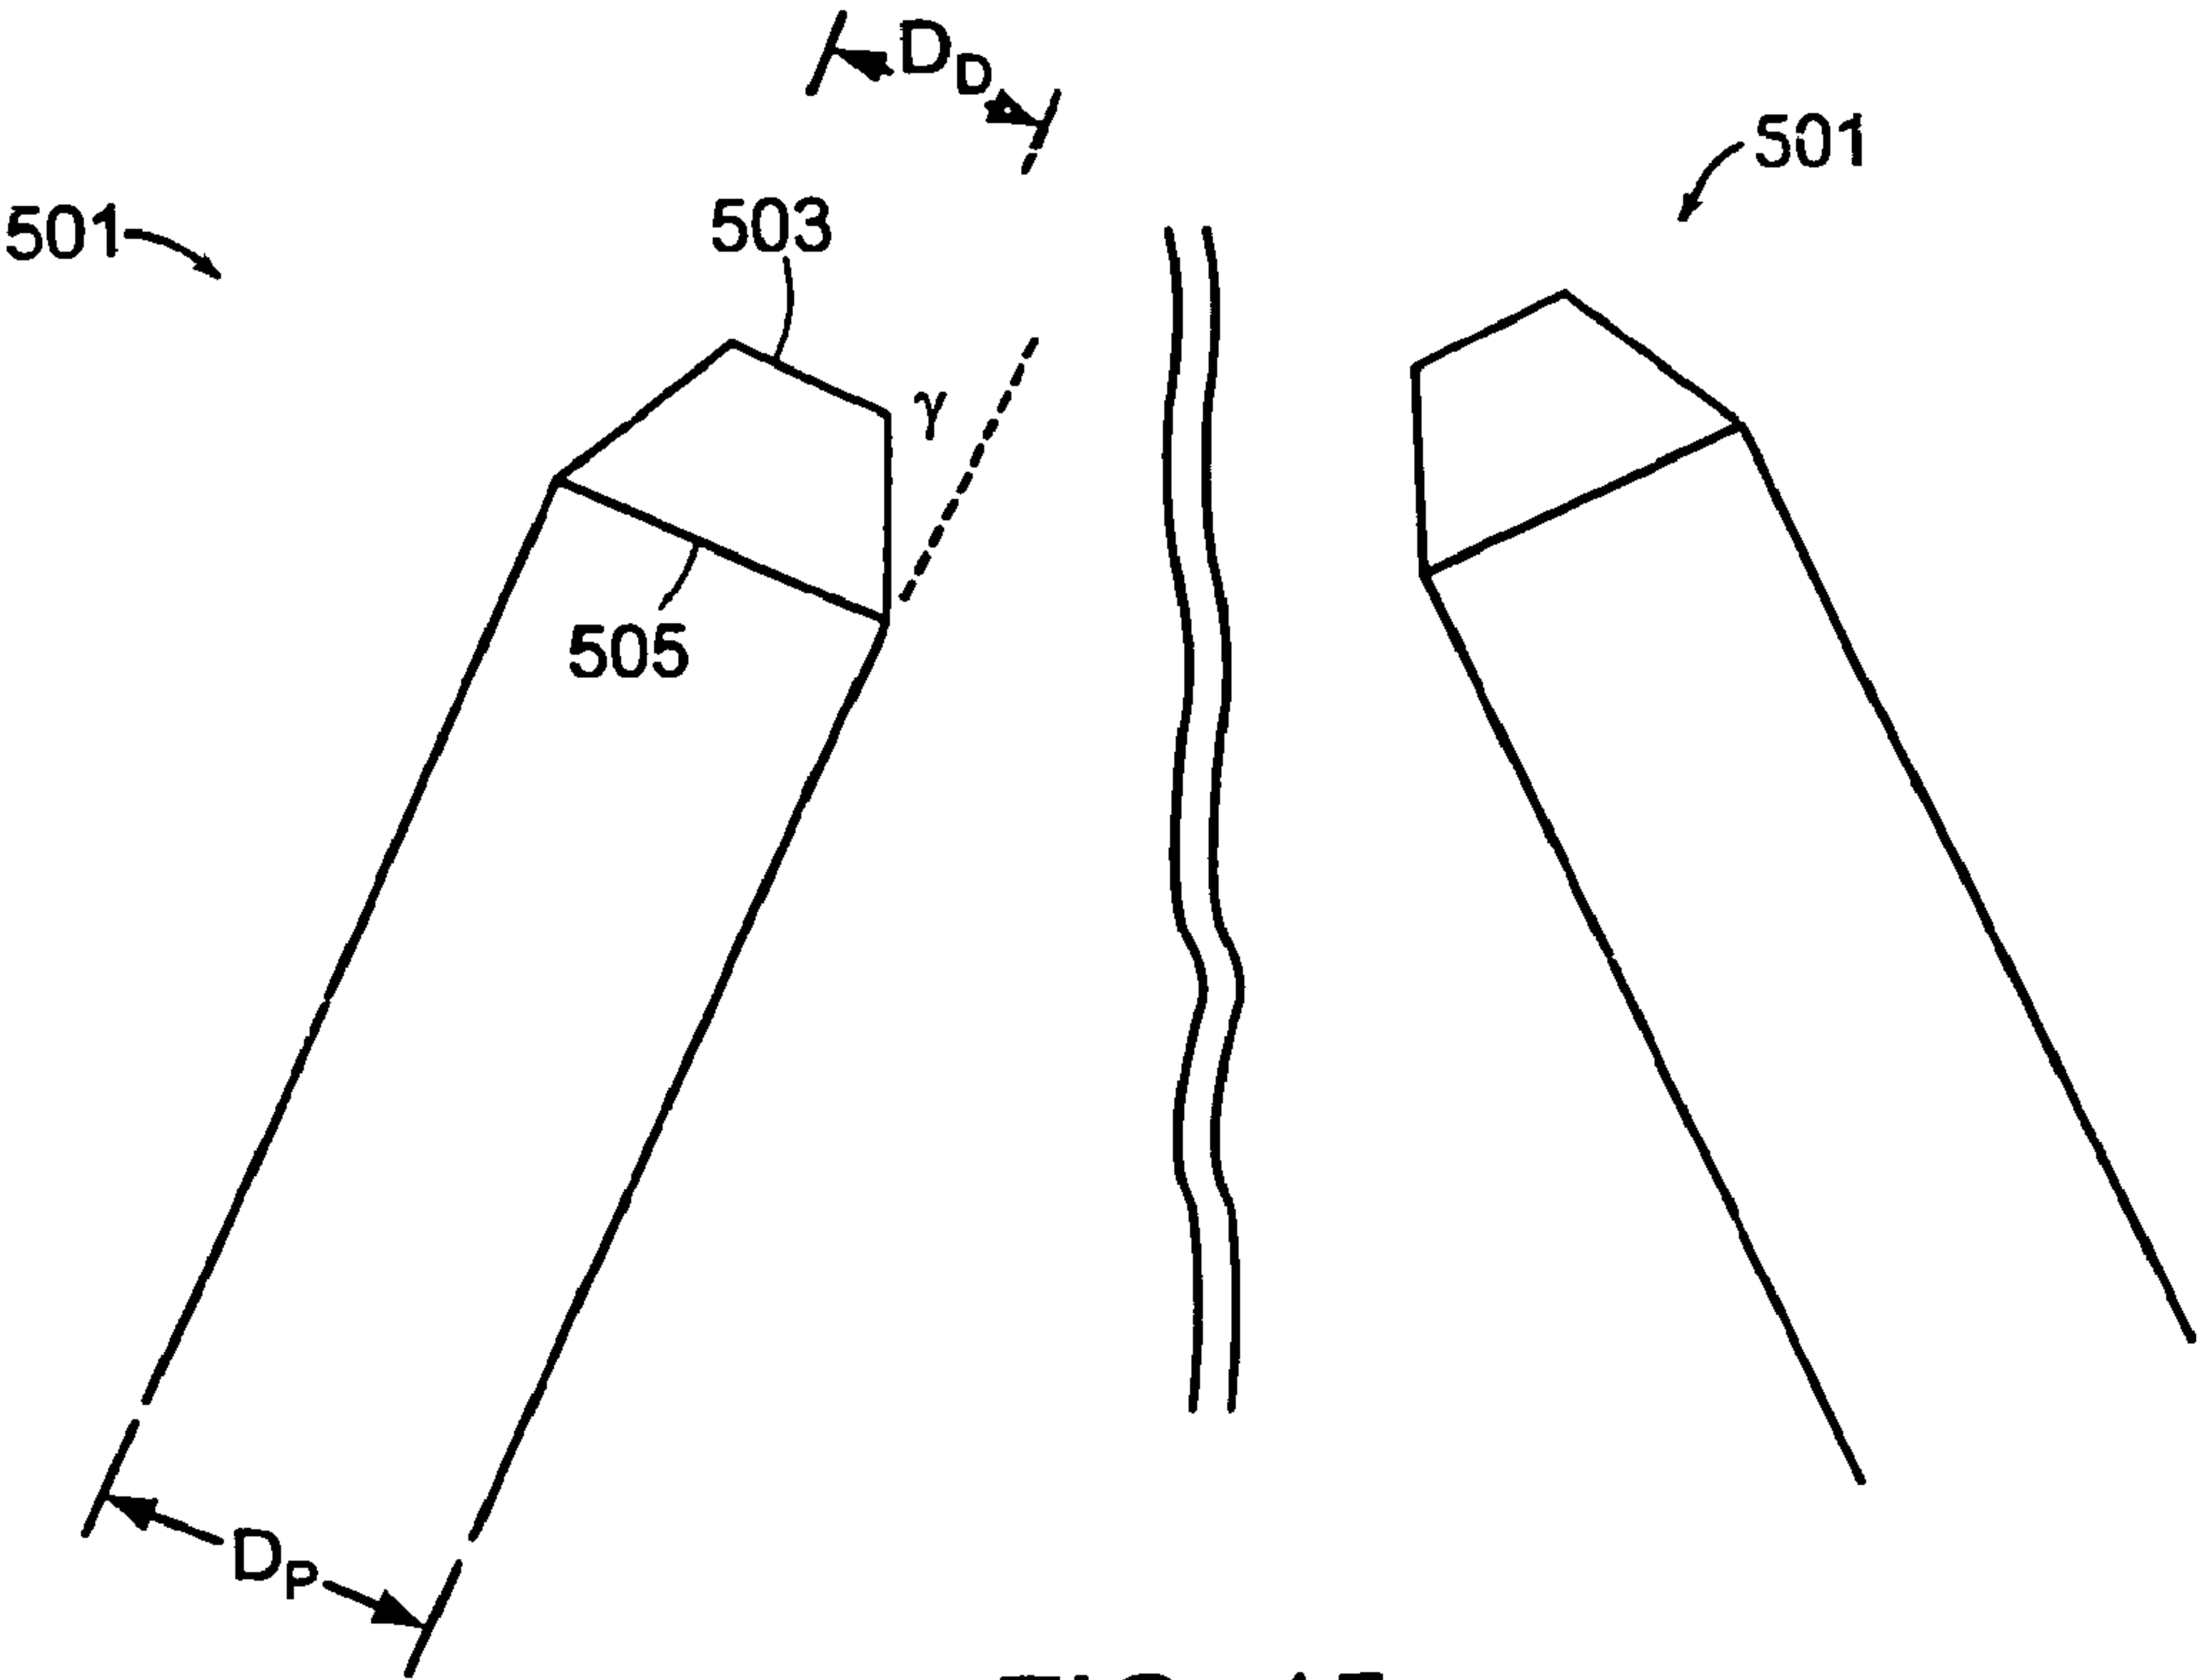


FIG. 15

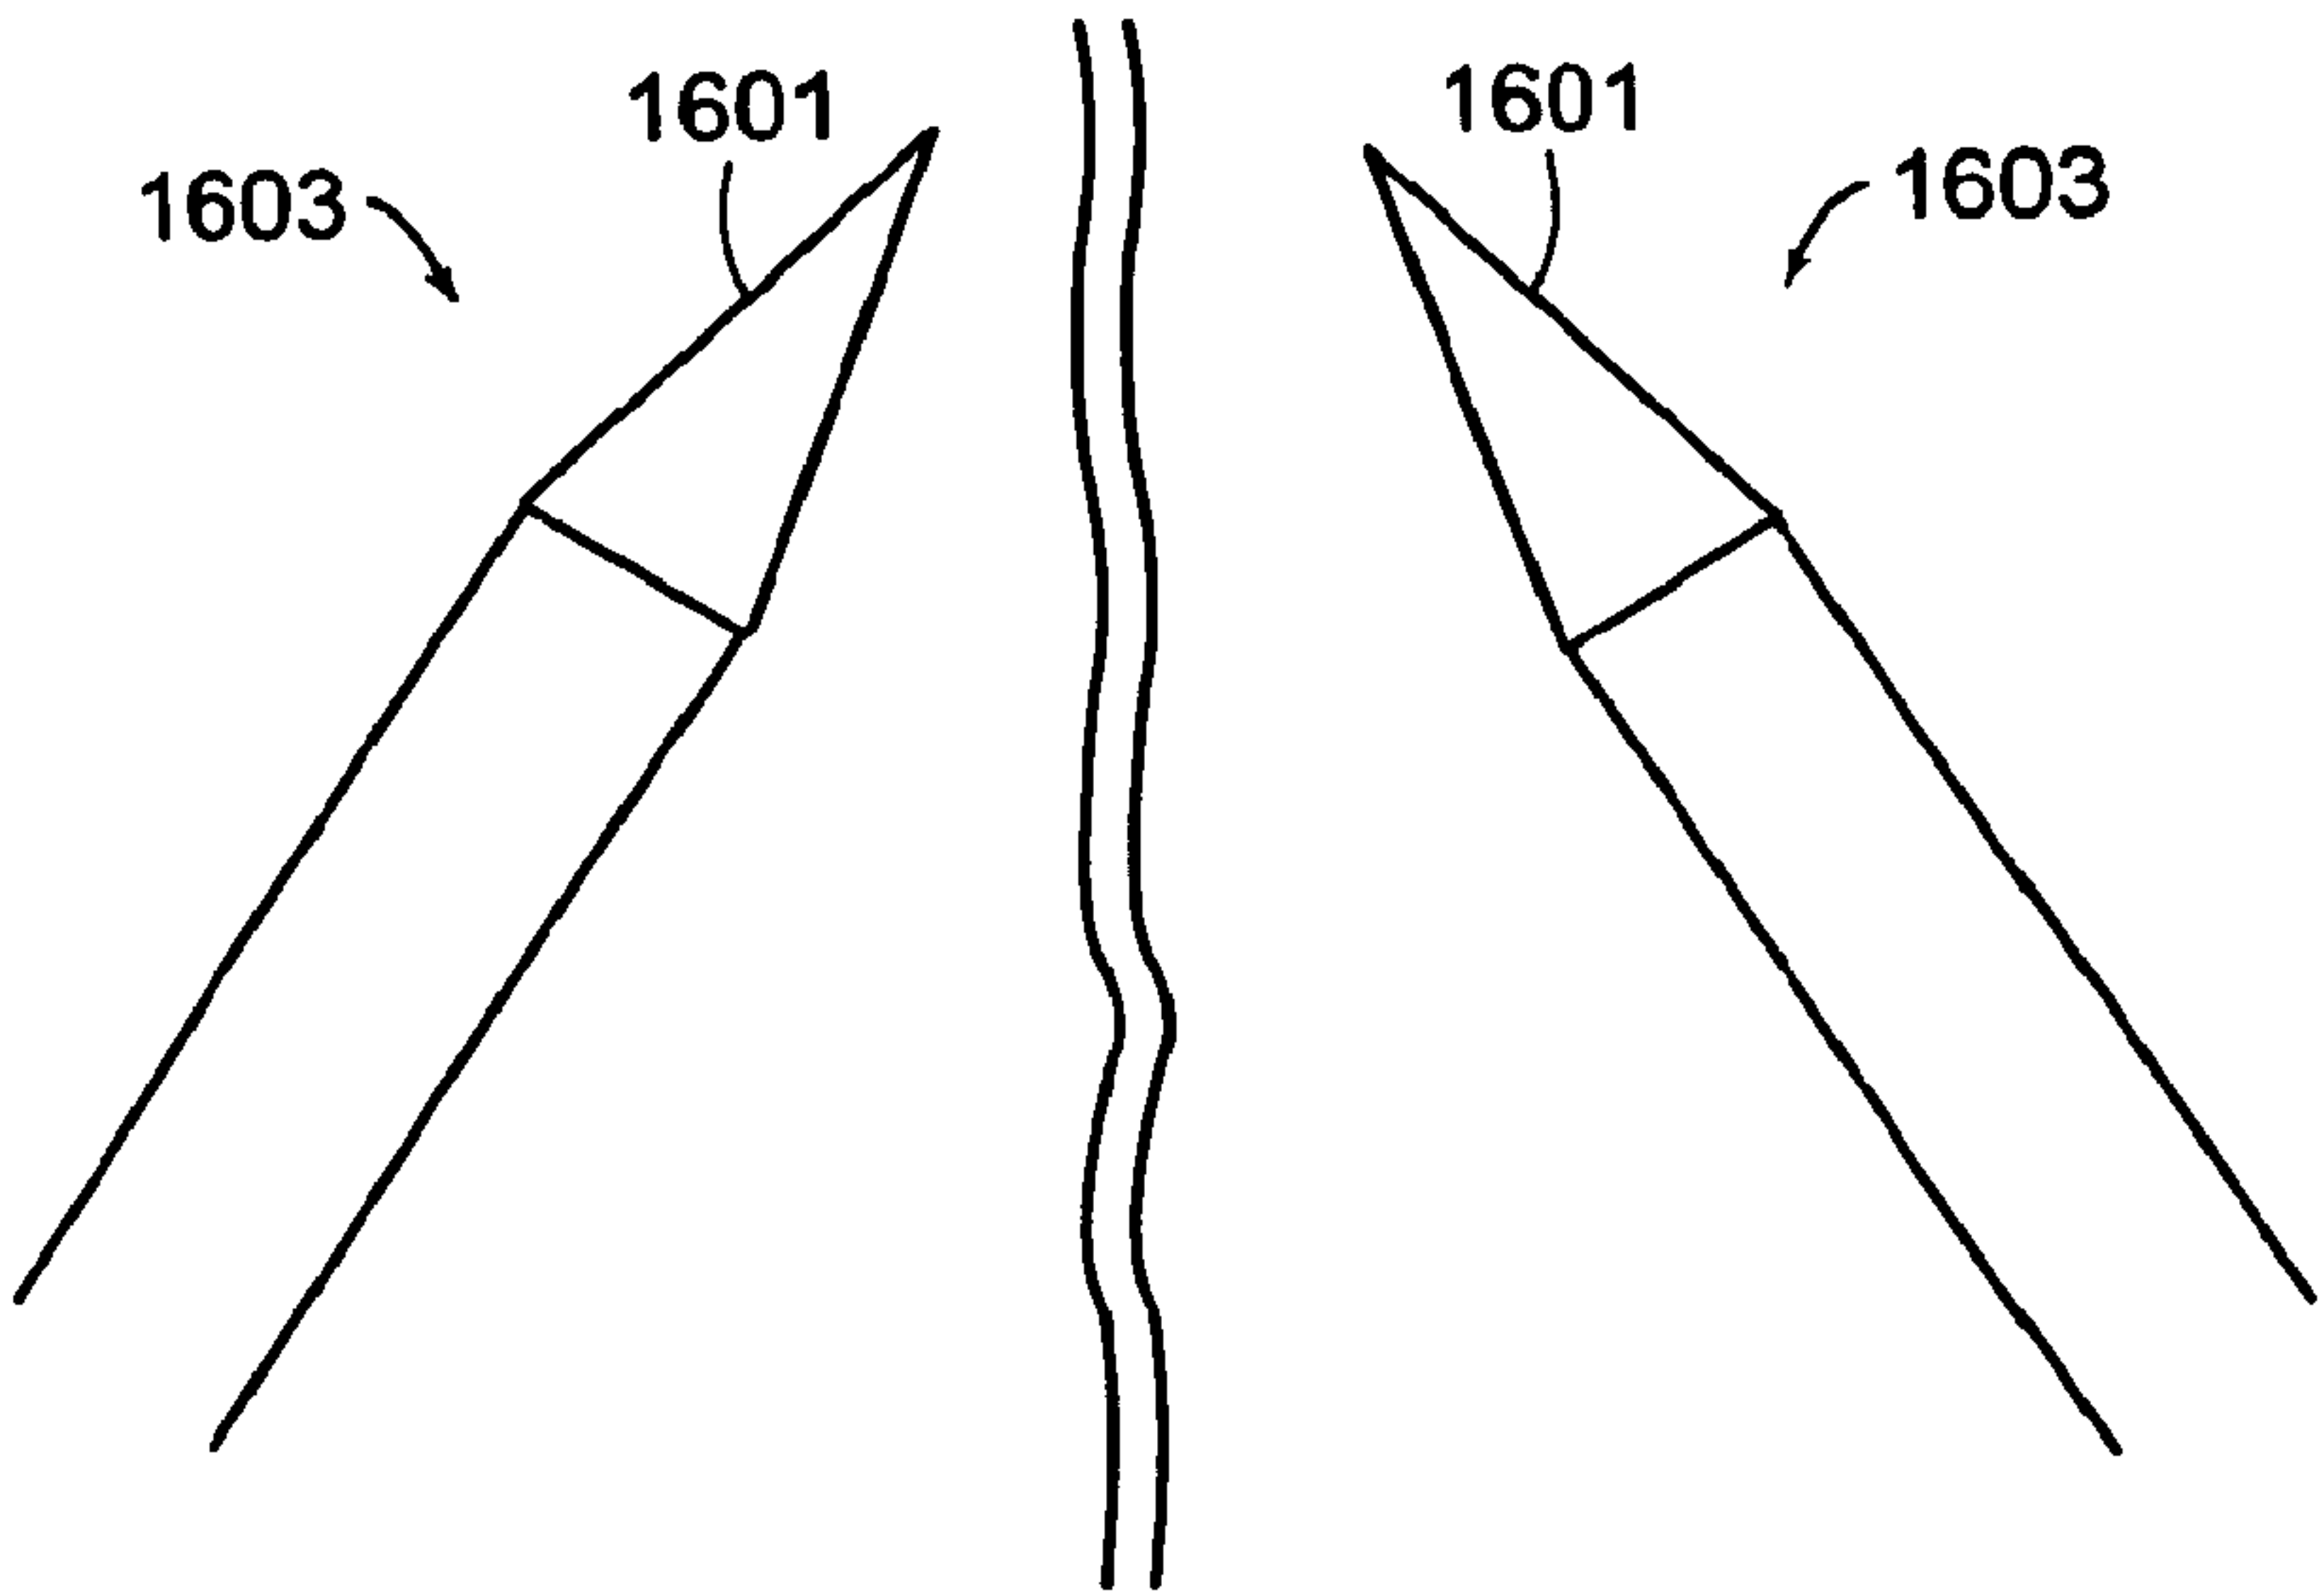


FIG. 16

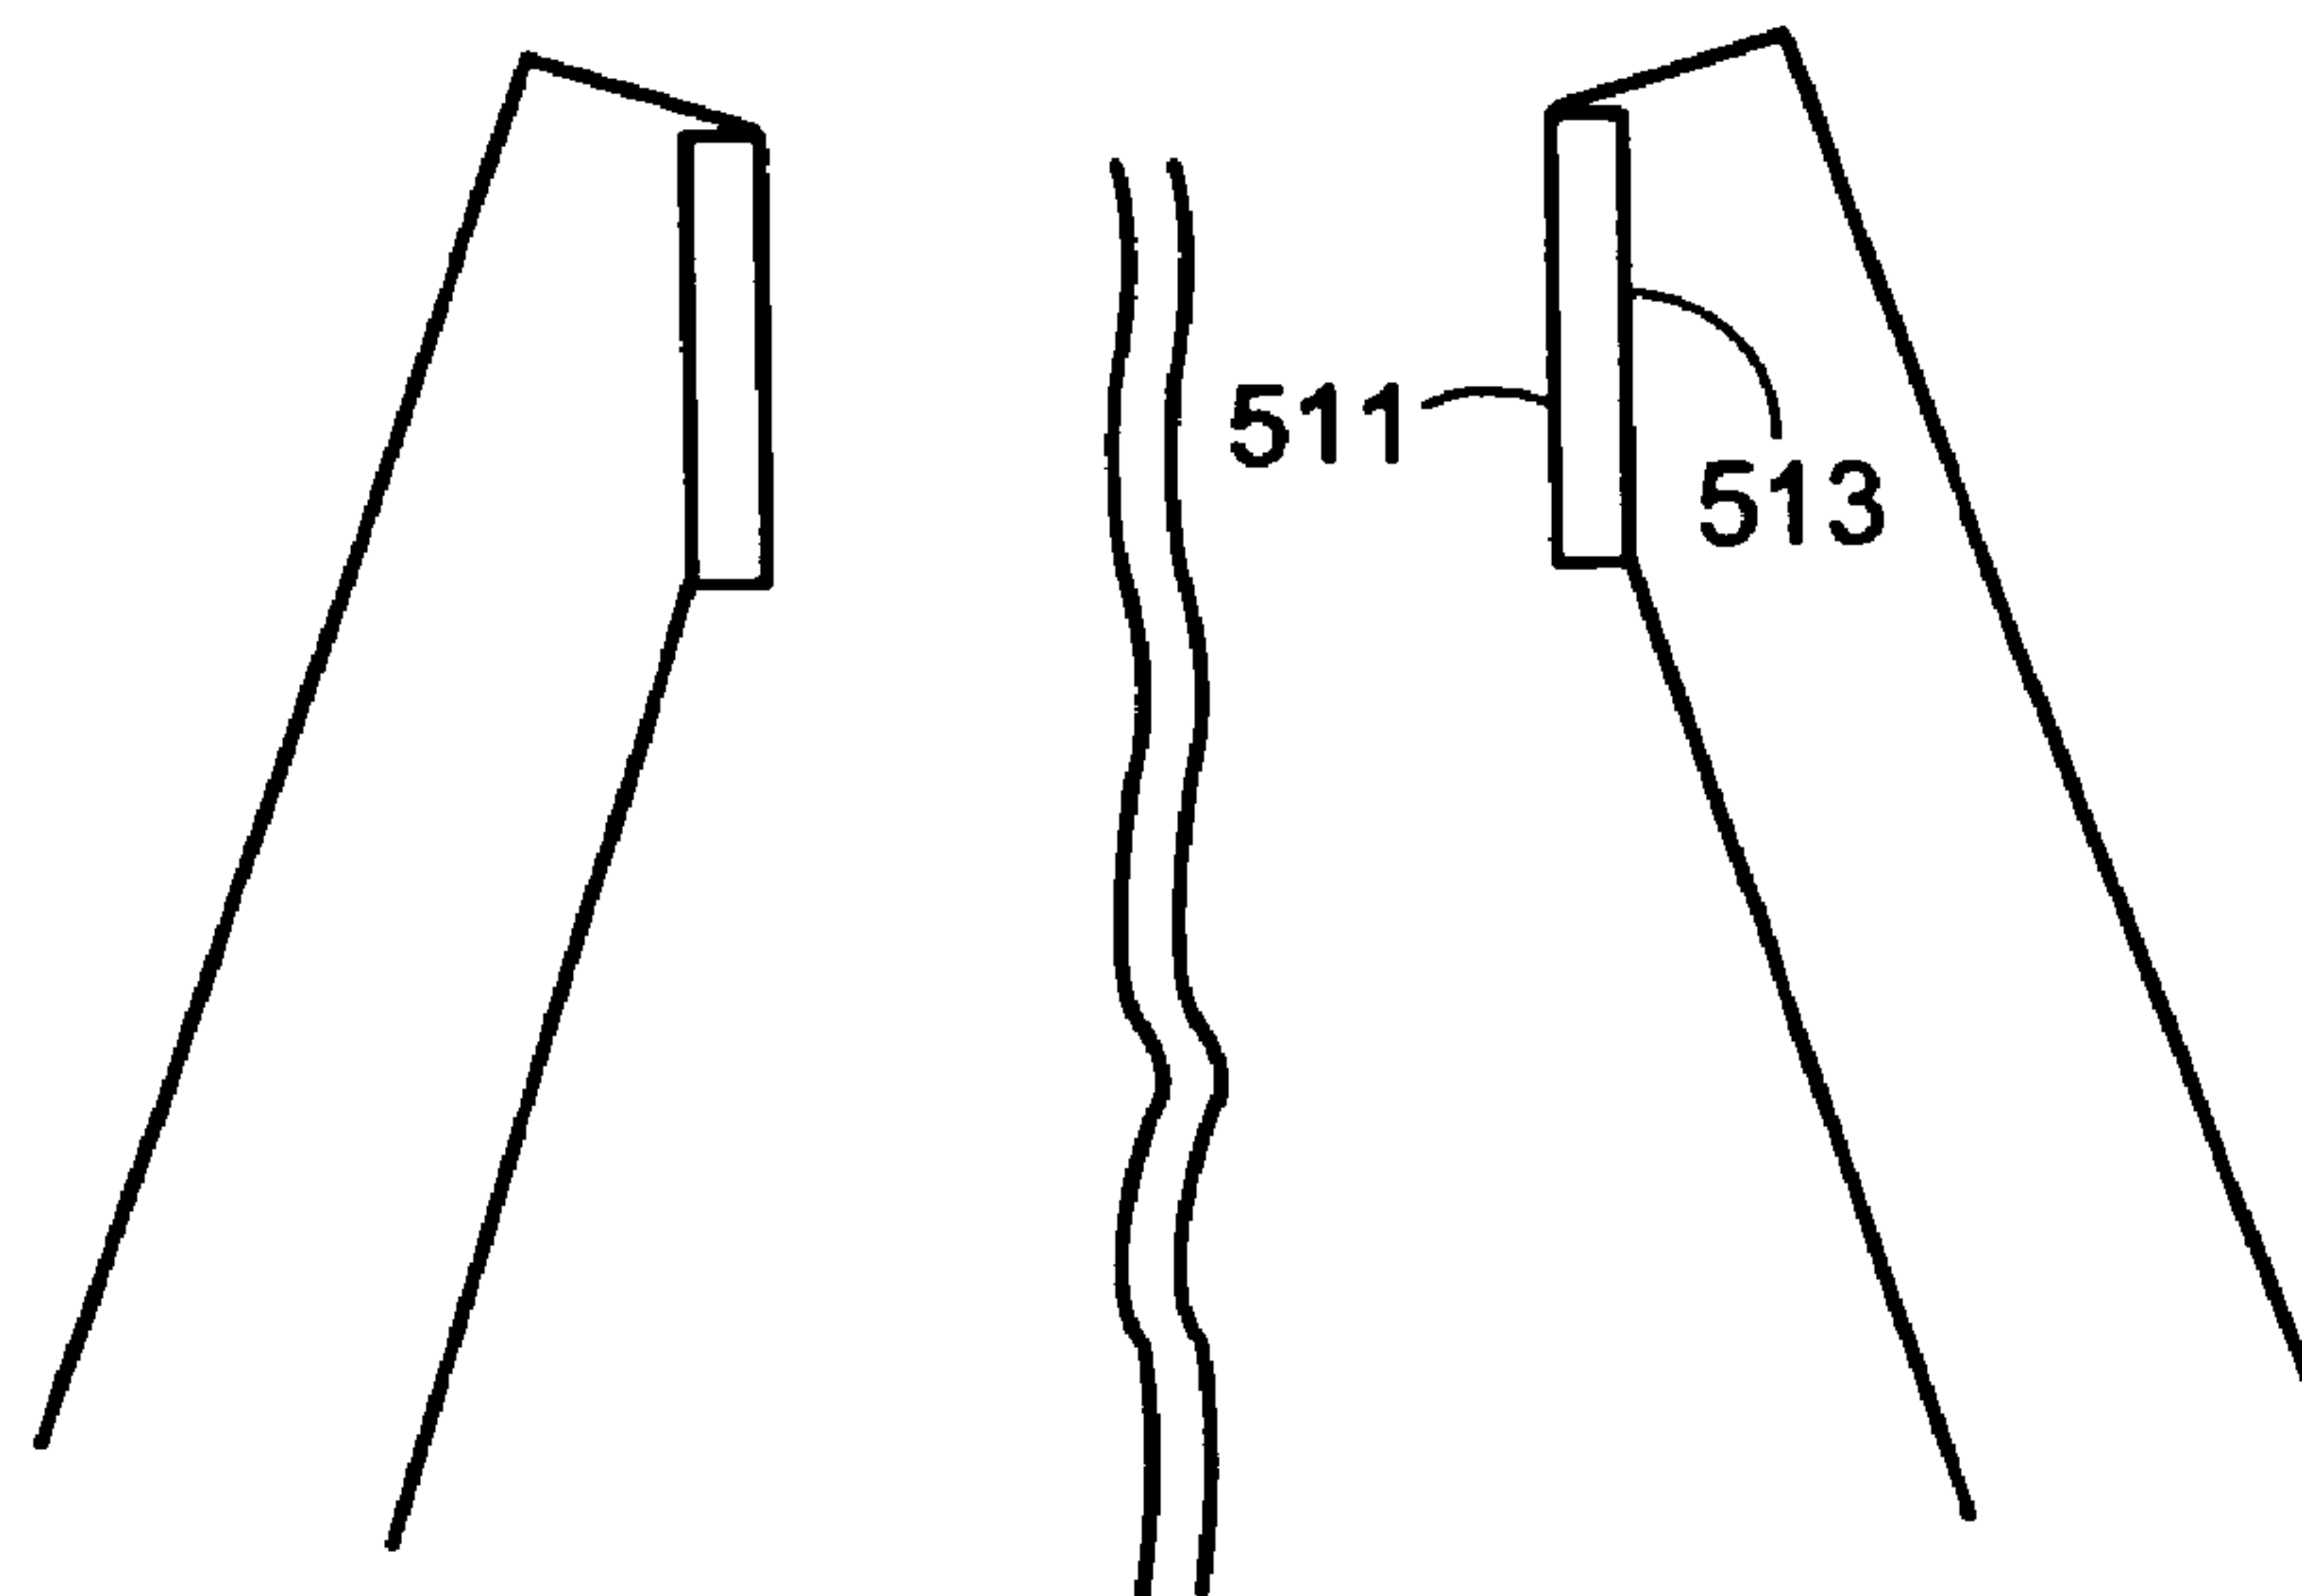


FIG. 17

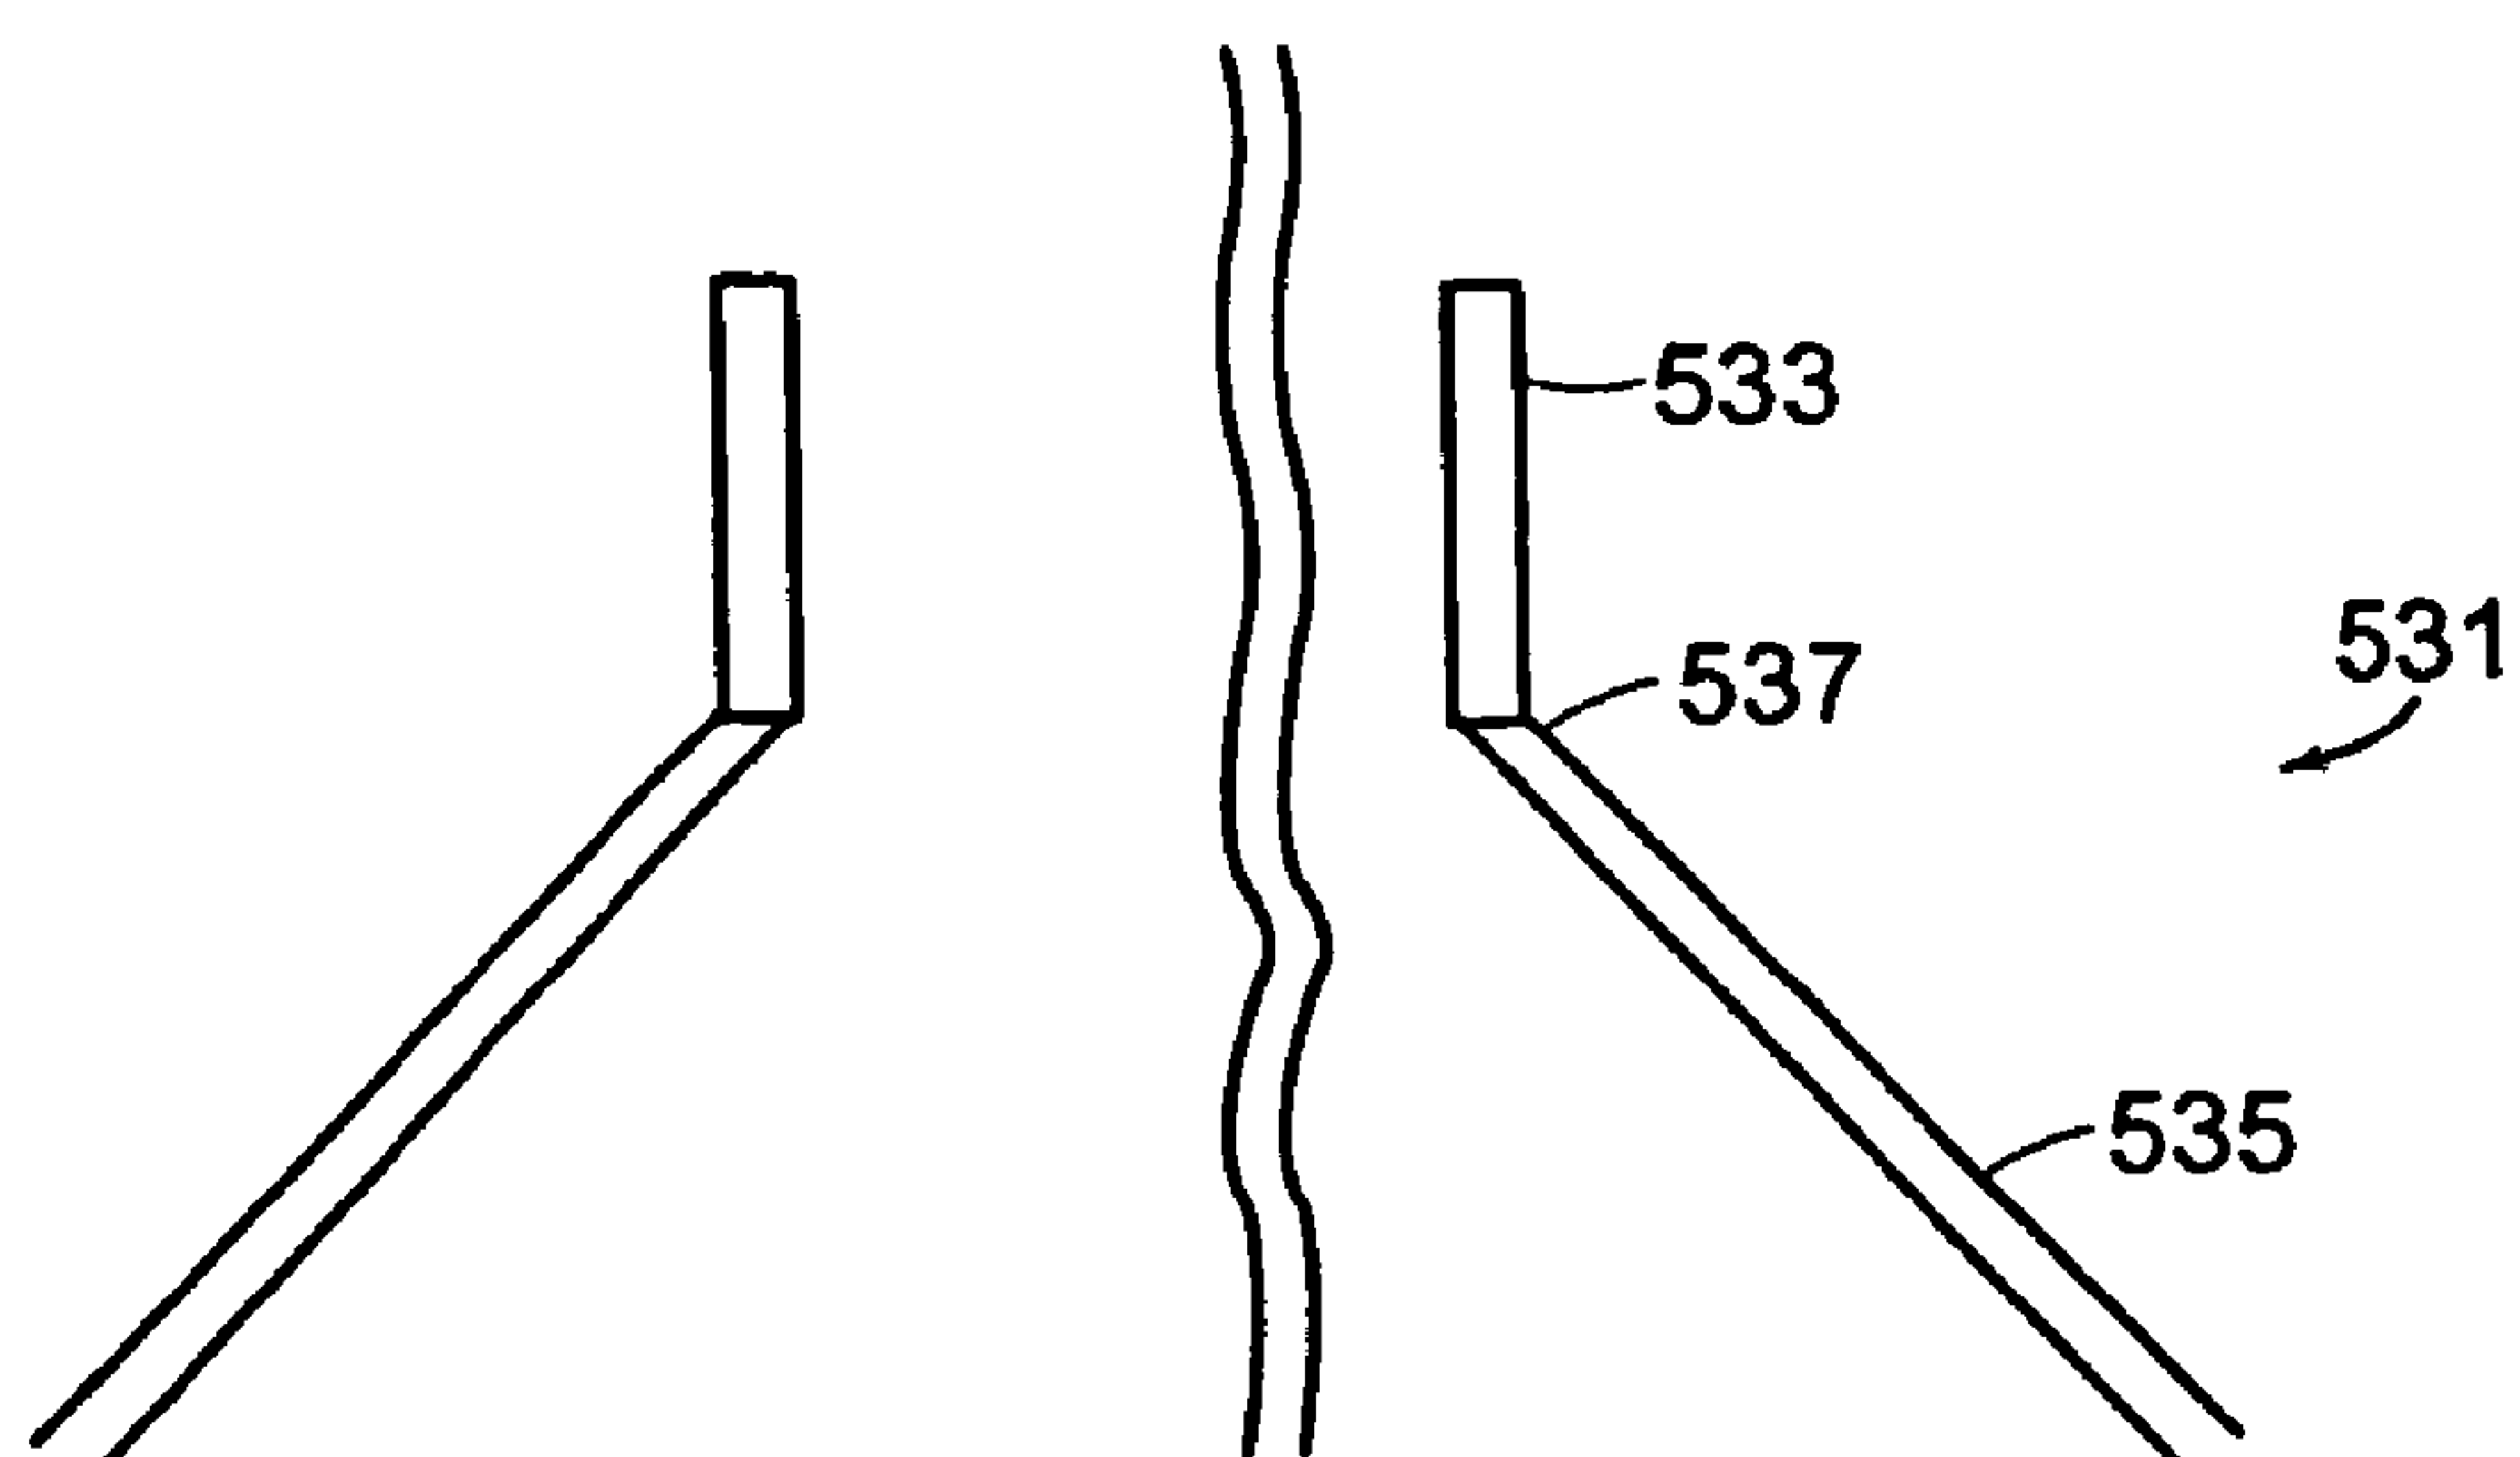
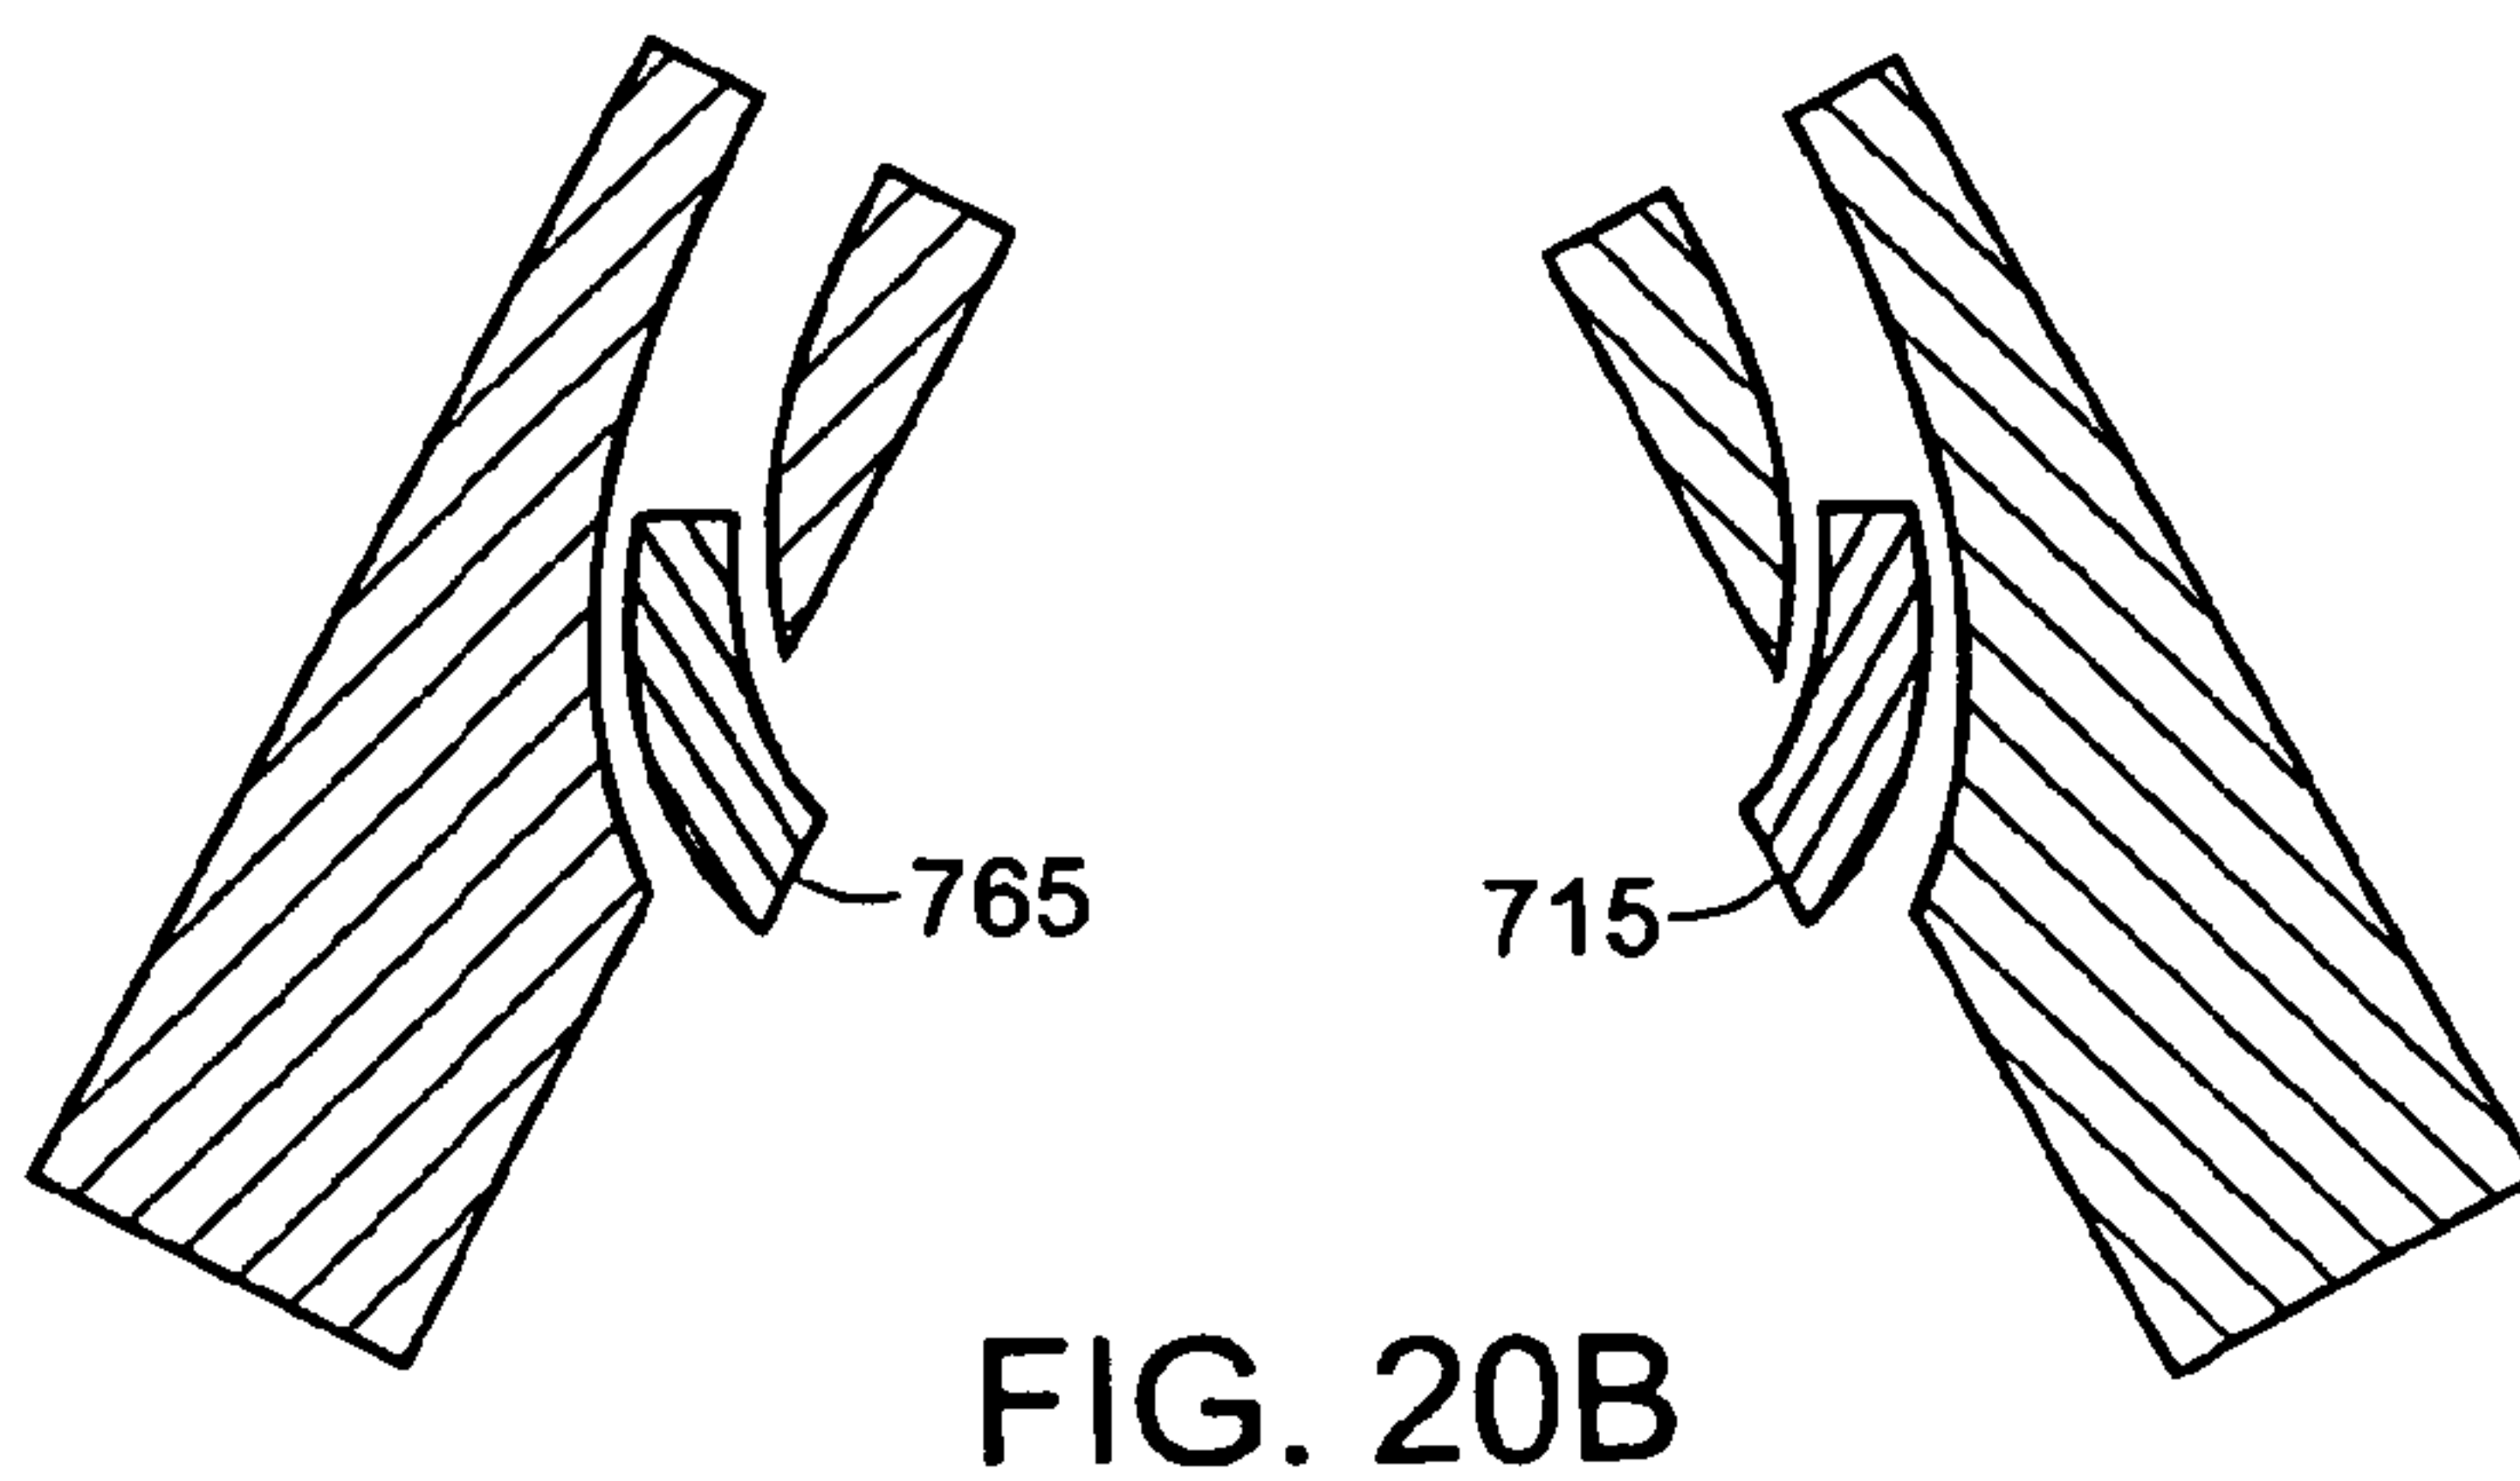
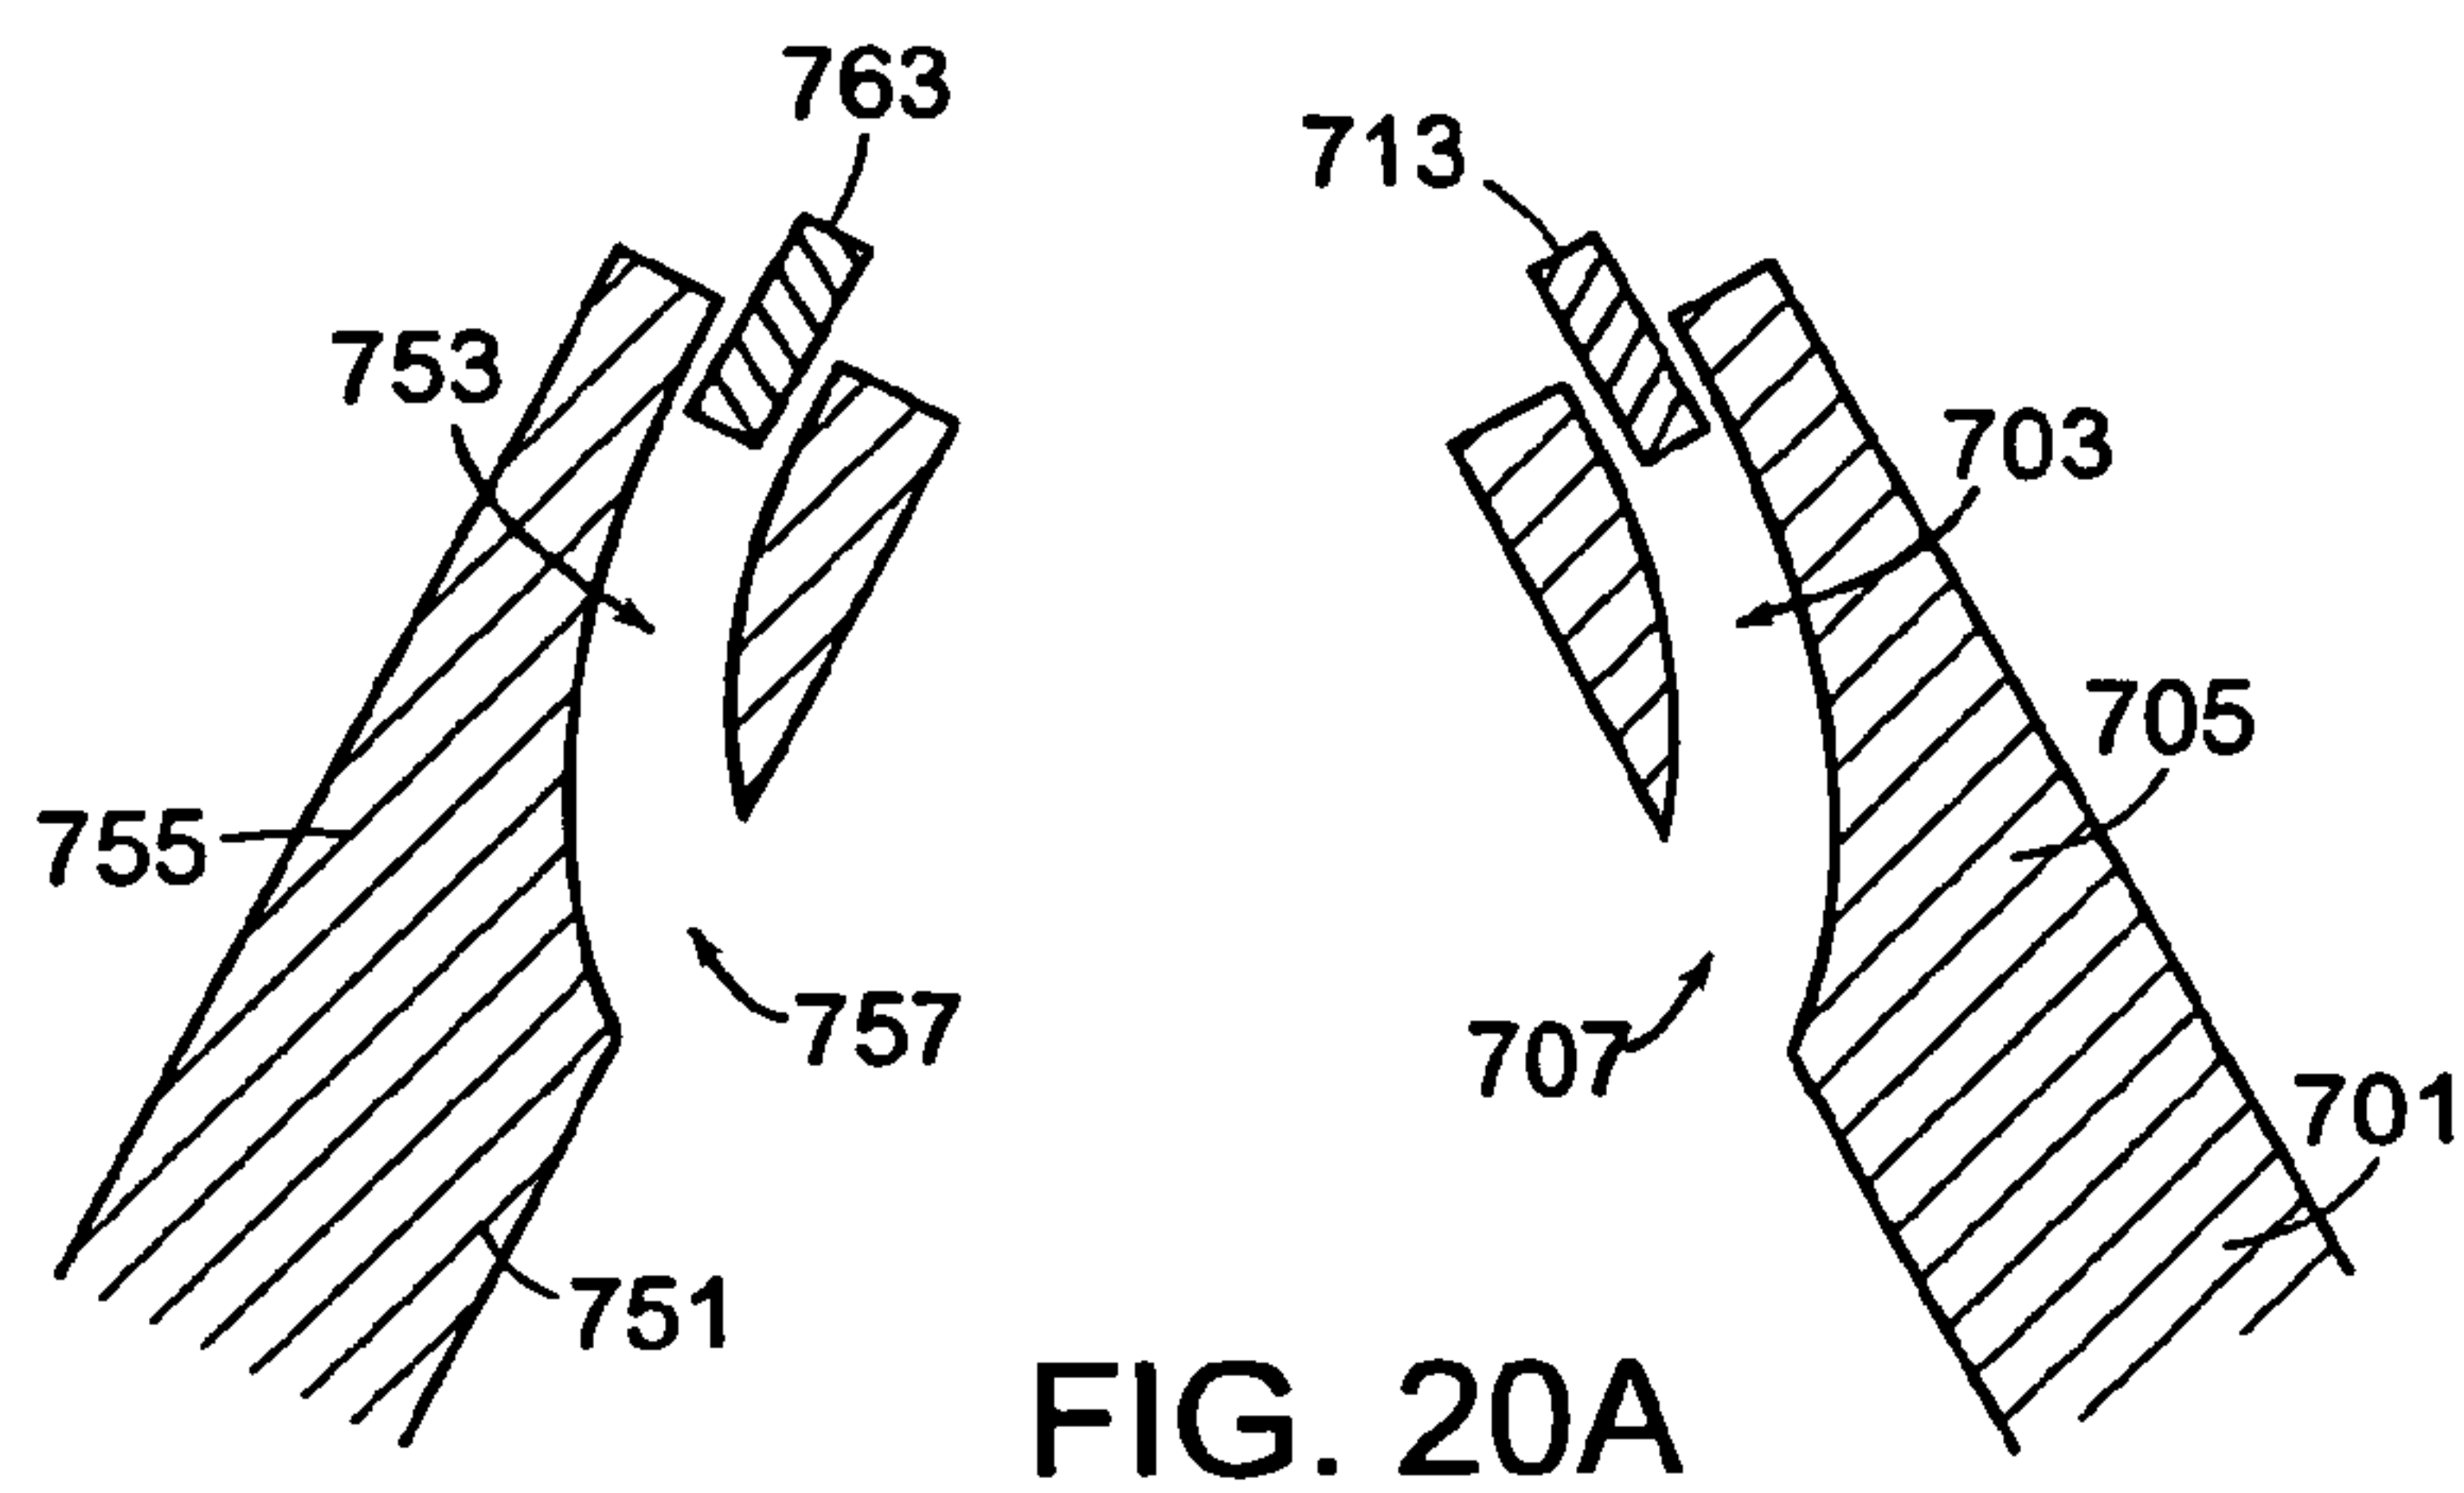
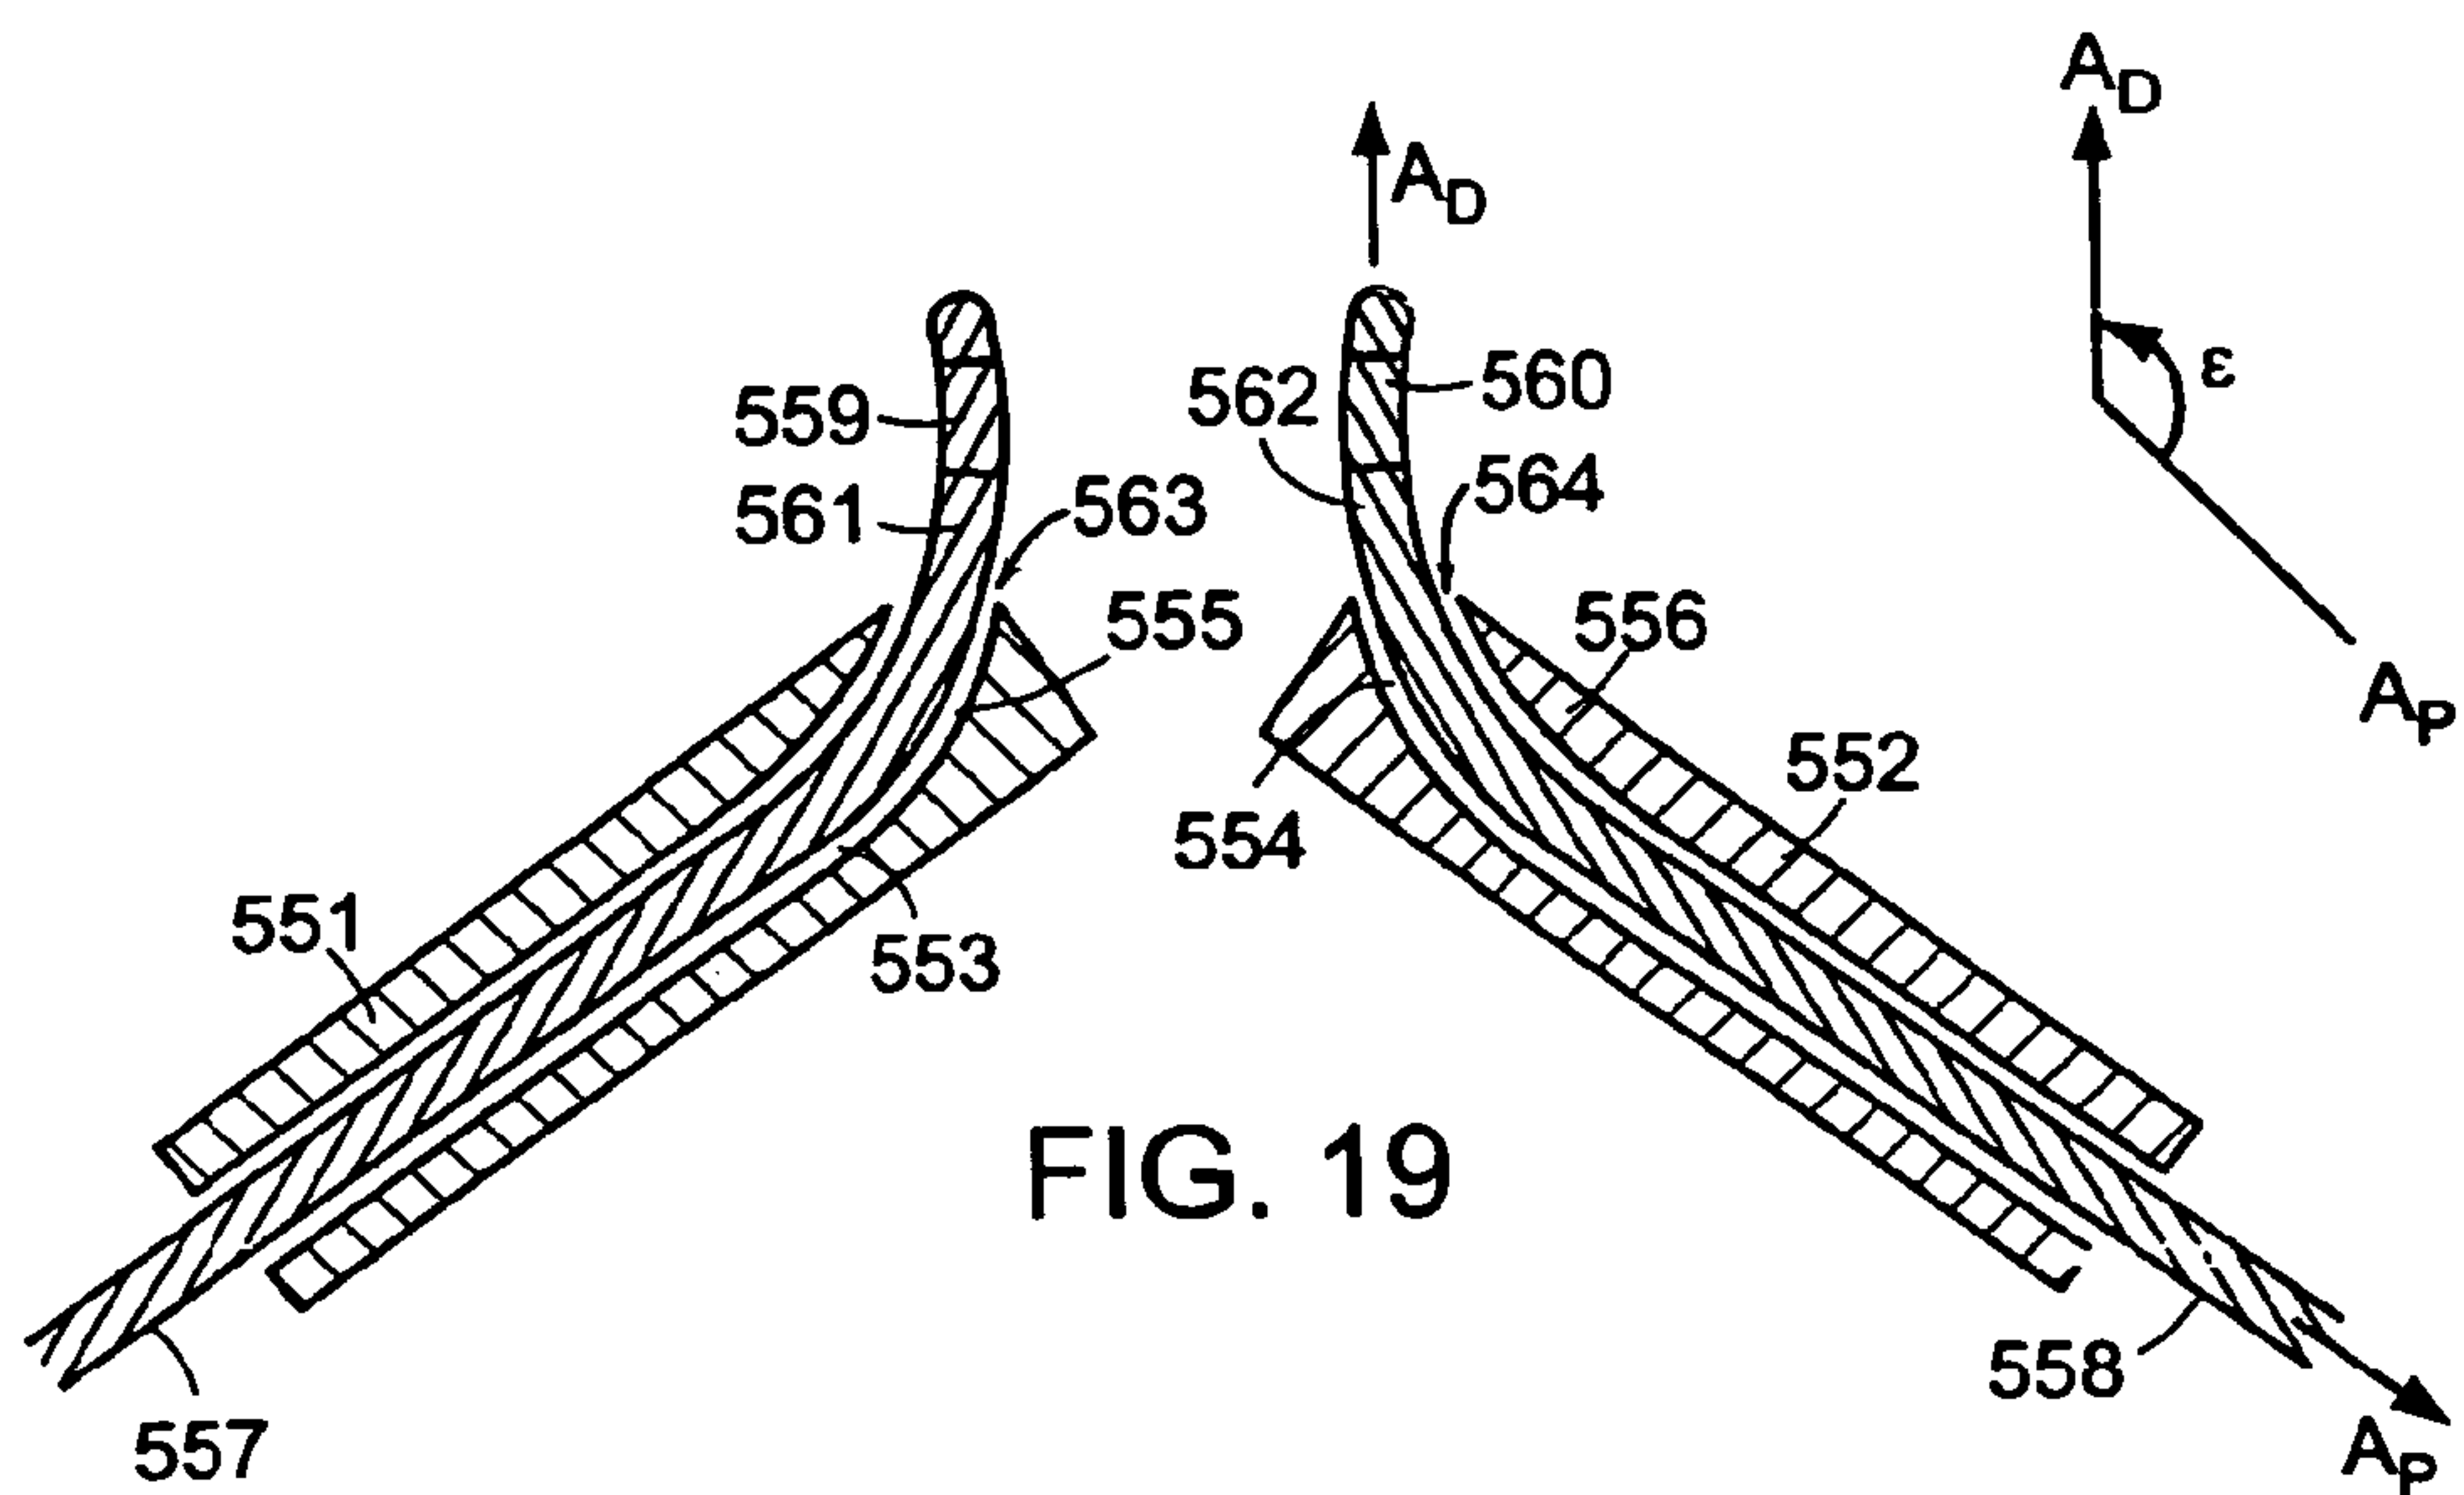


FIG. 18



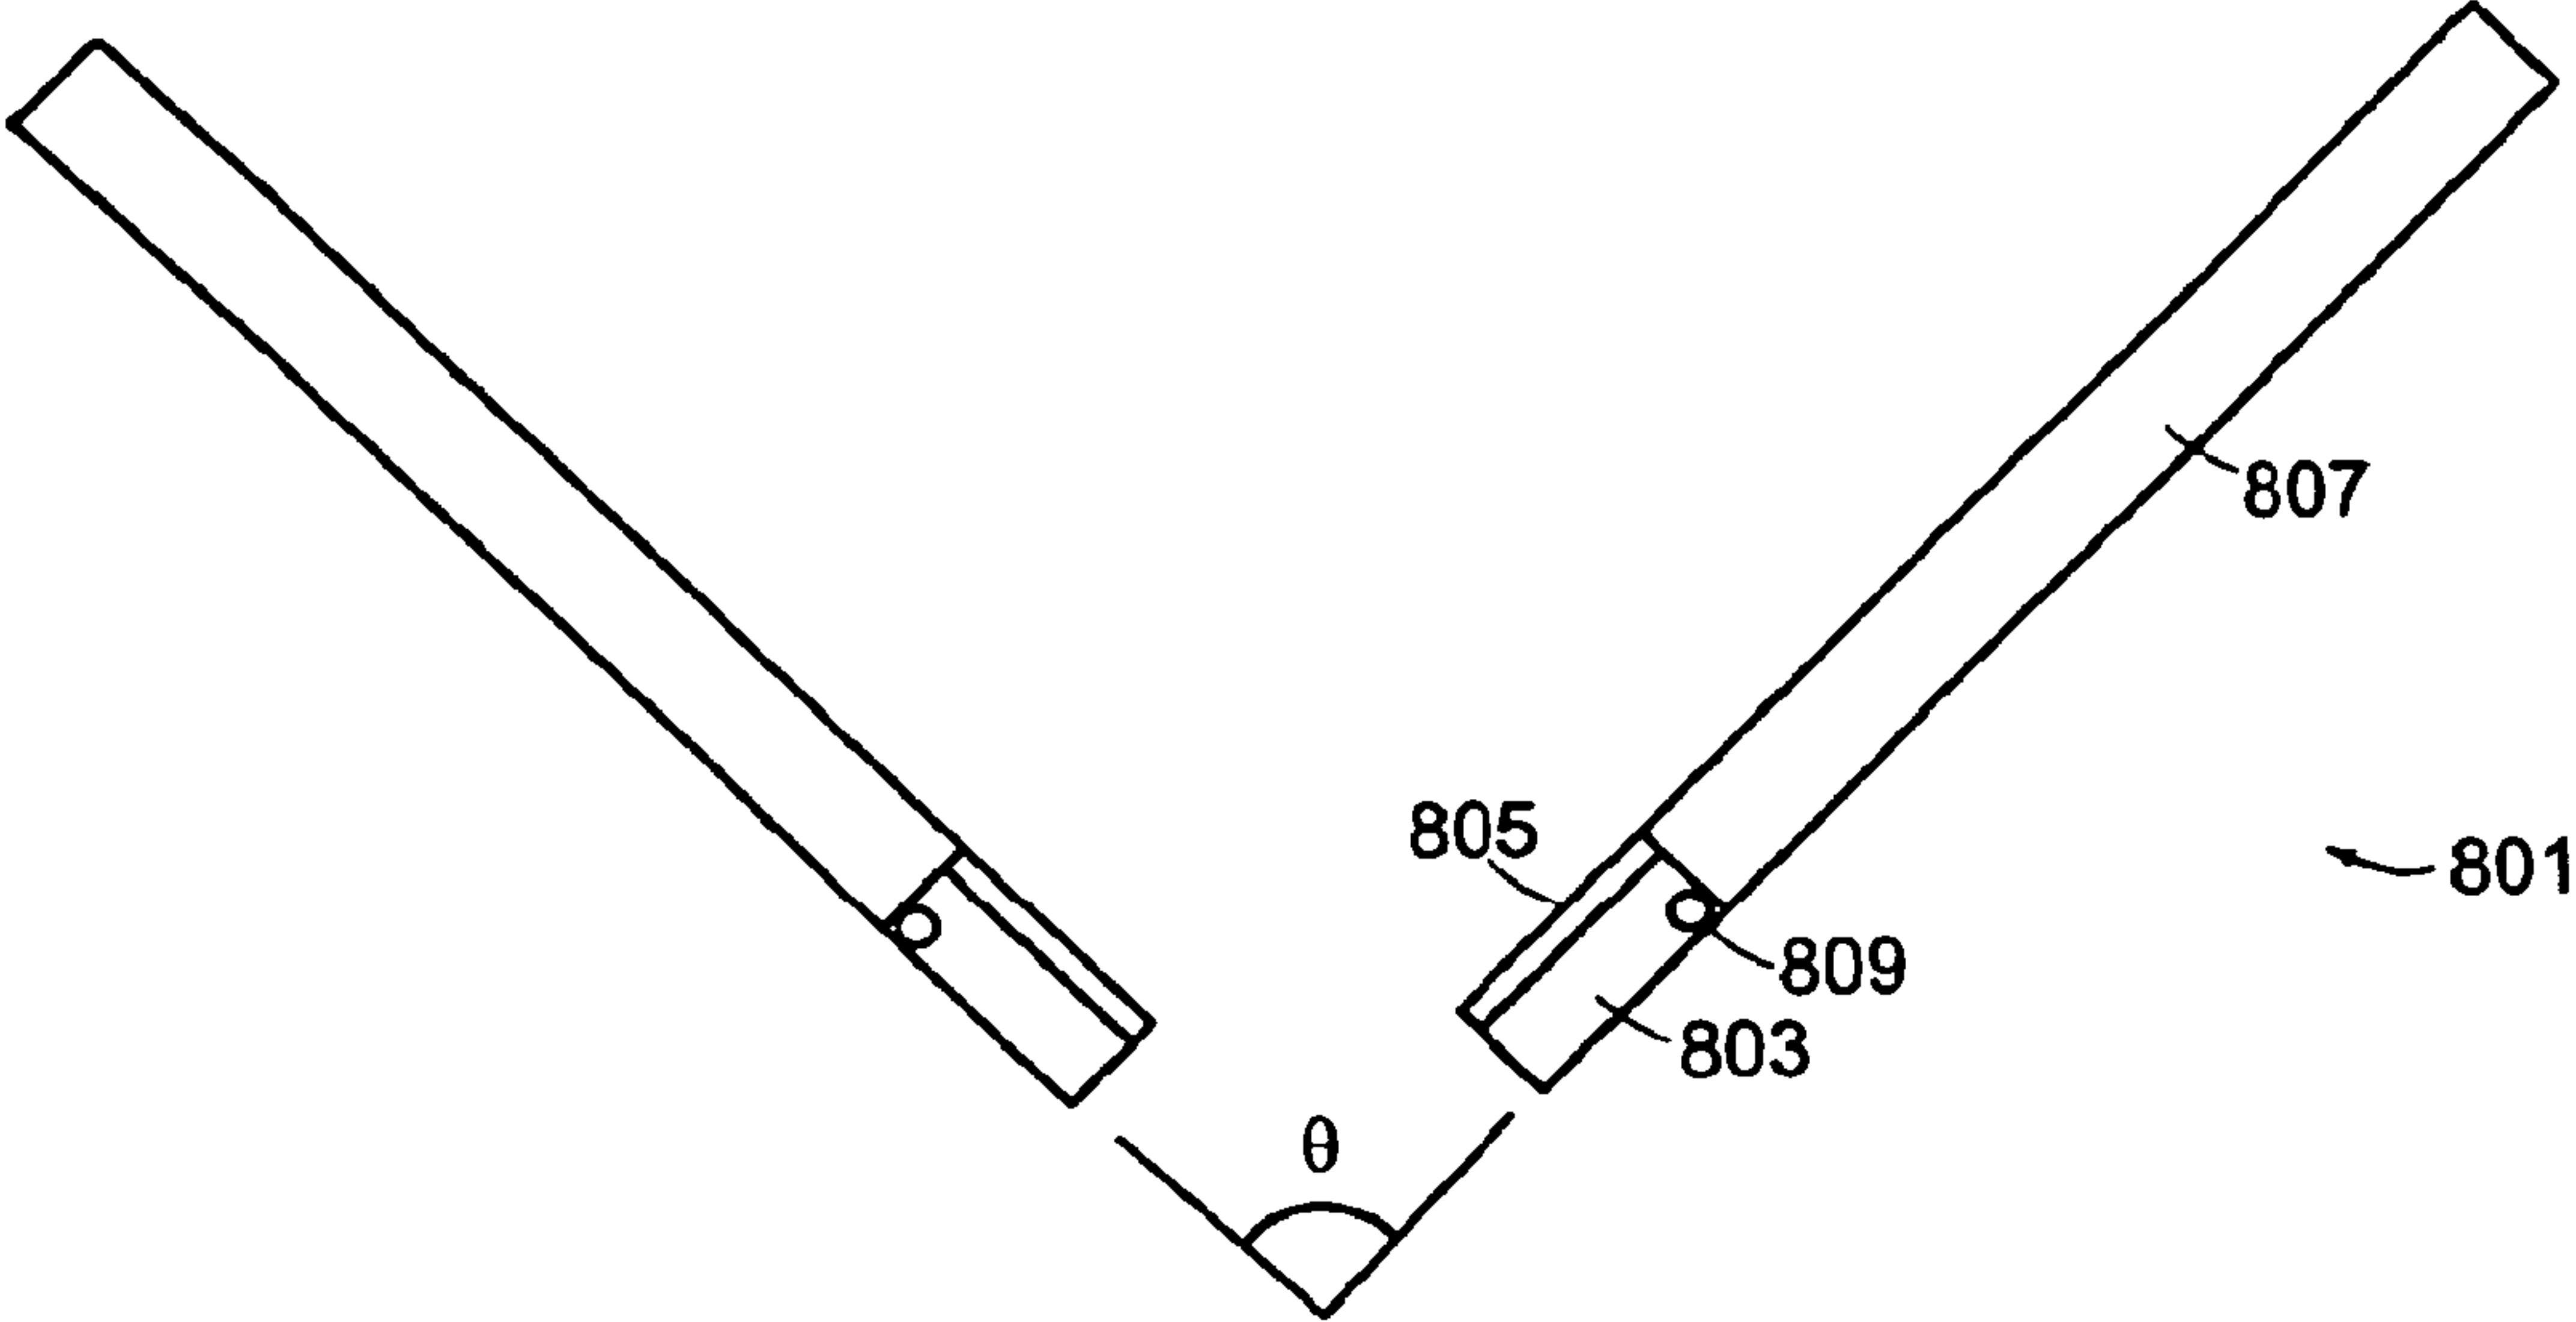


FIG. 21A

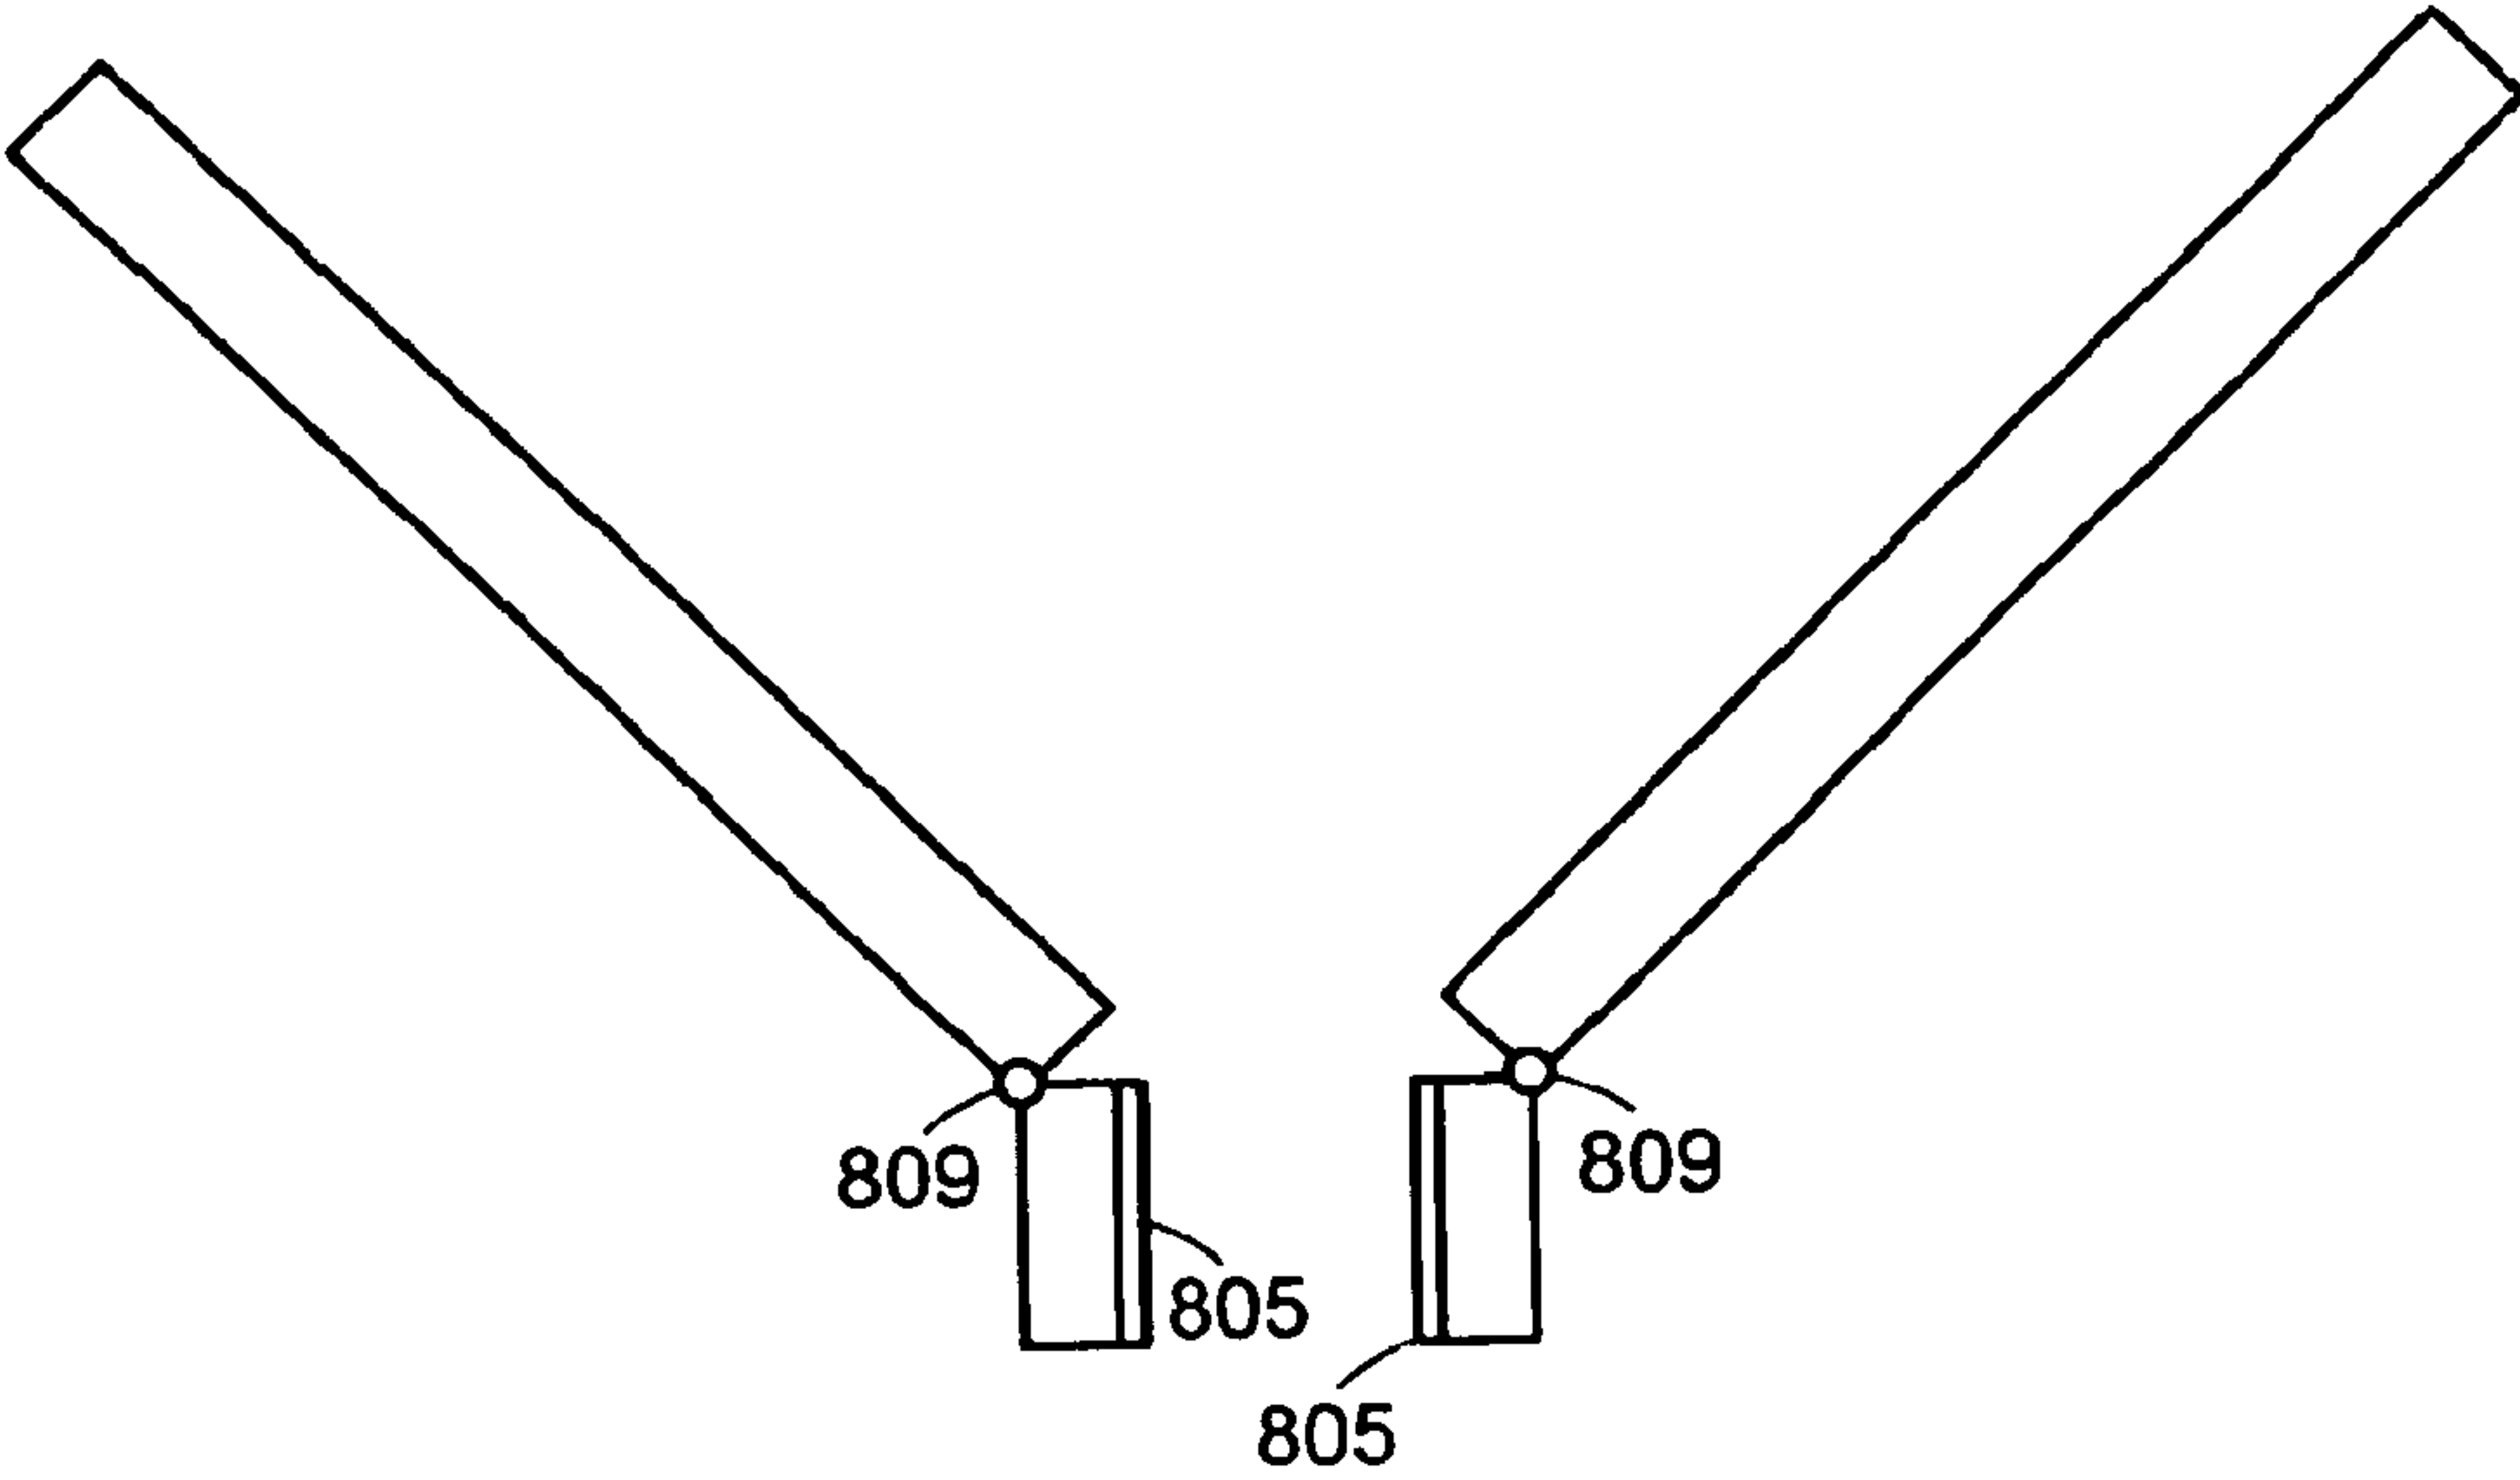


FIG. 21B

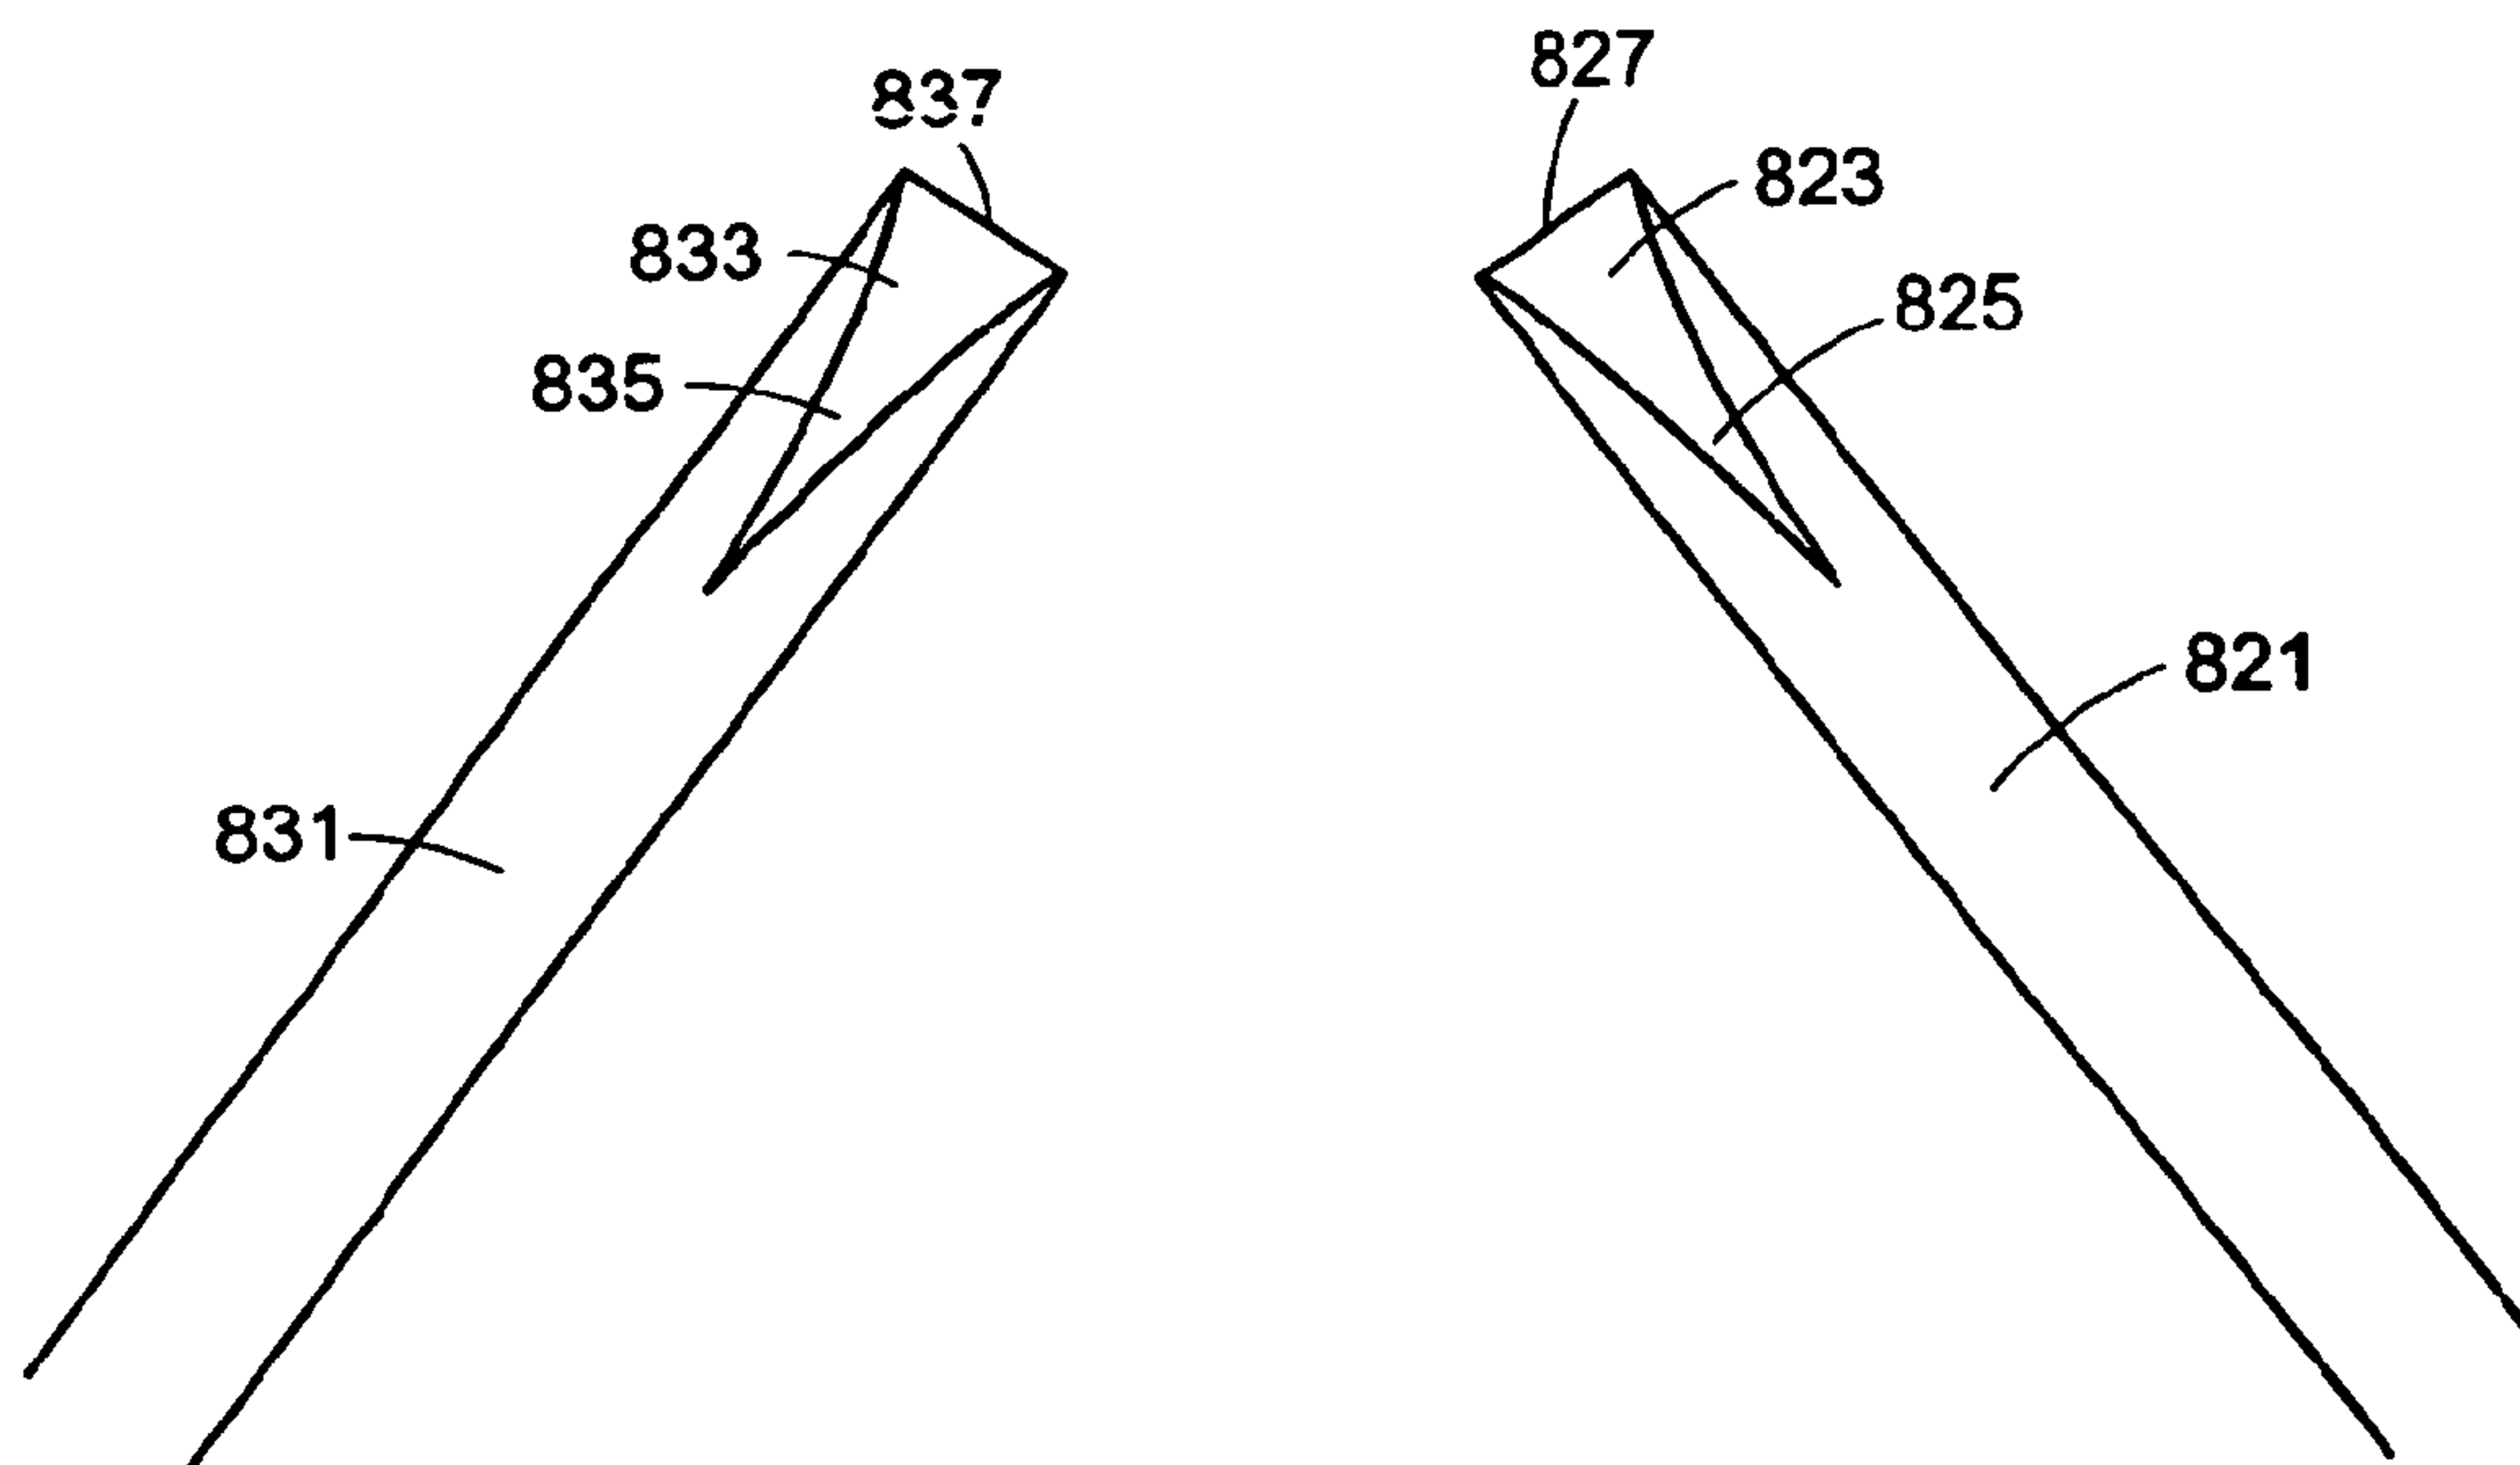


FIG. 22

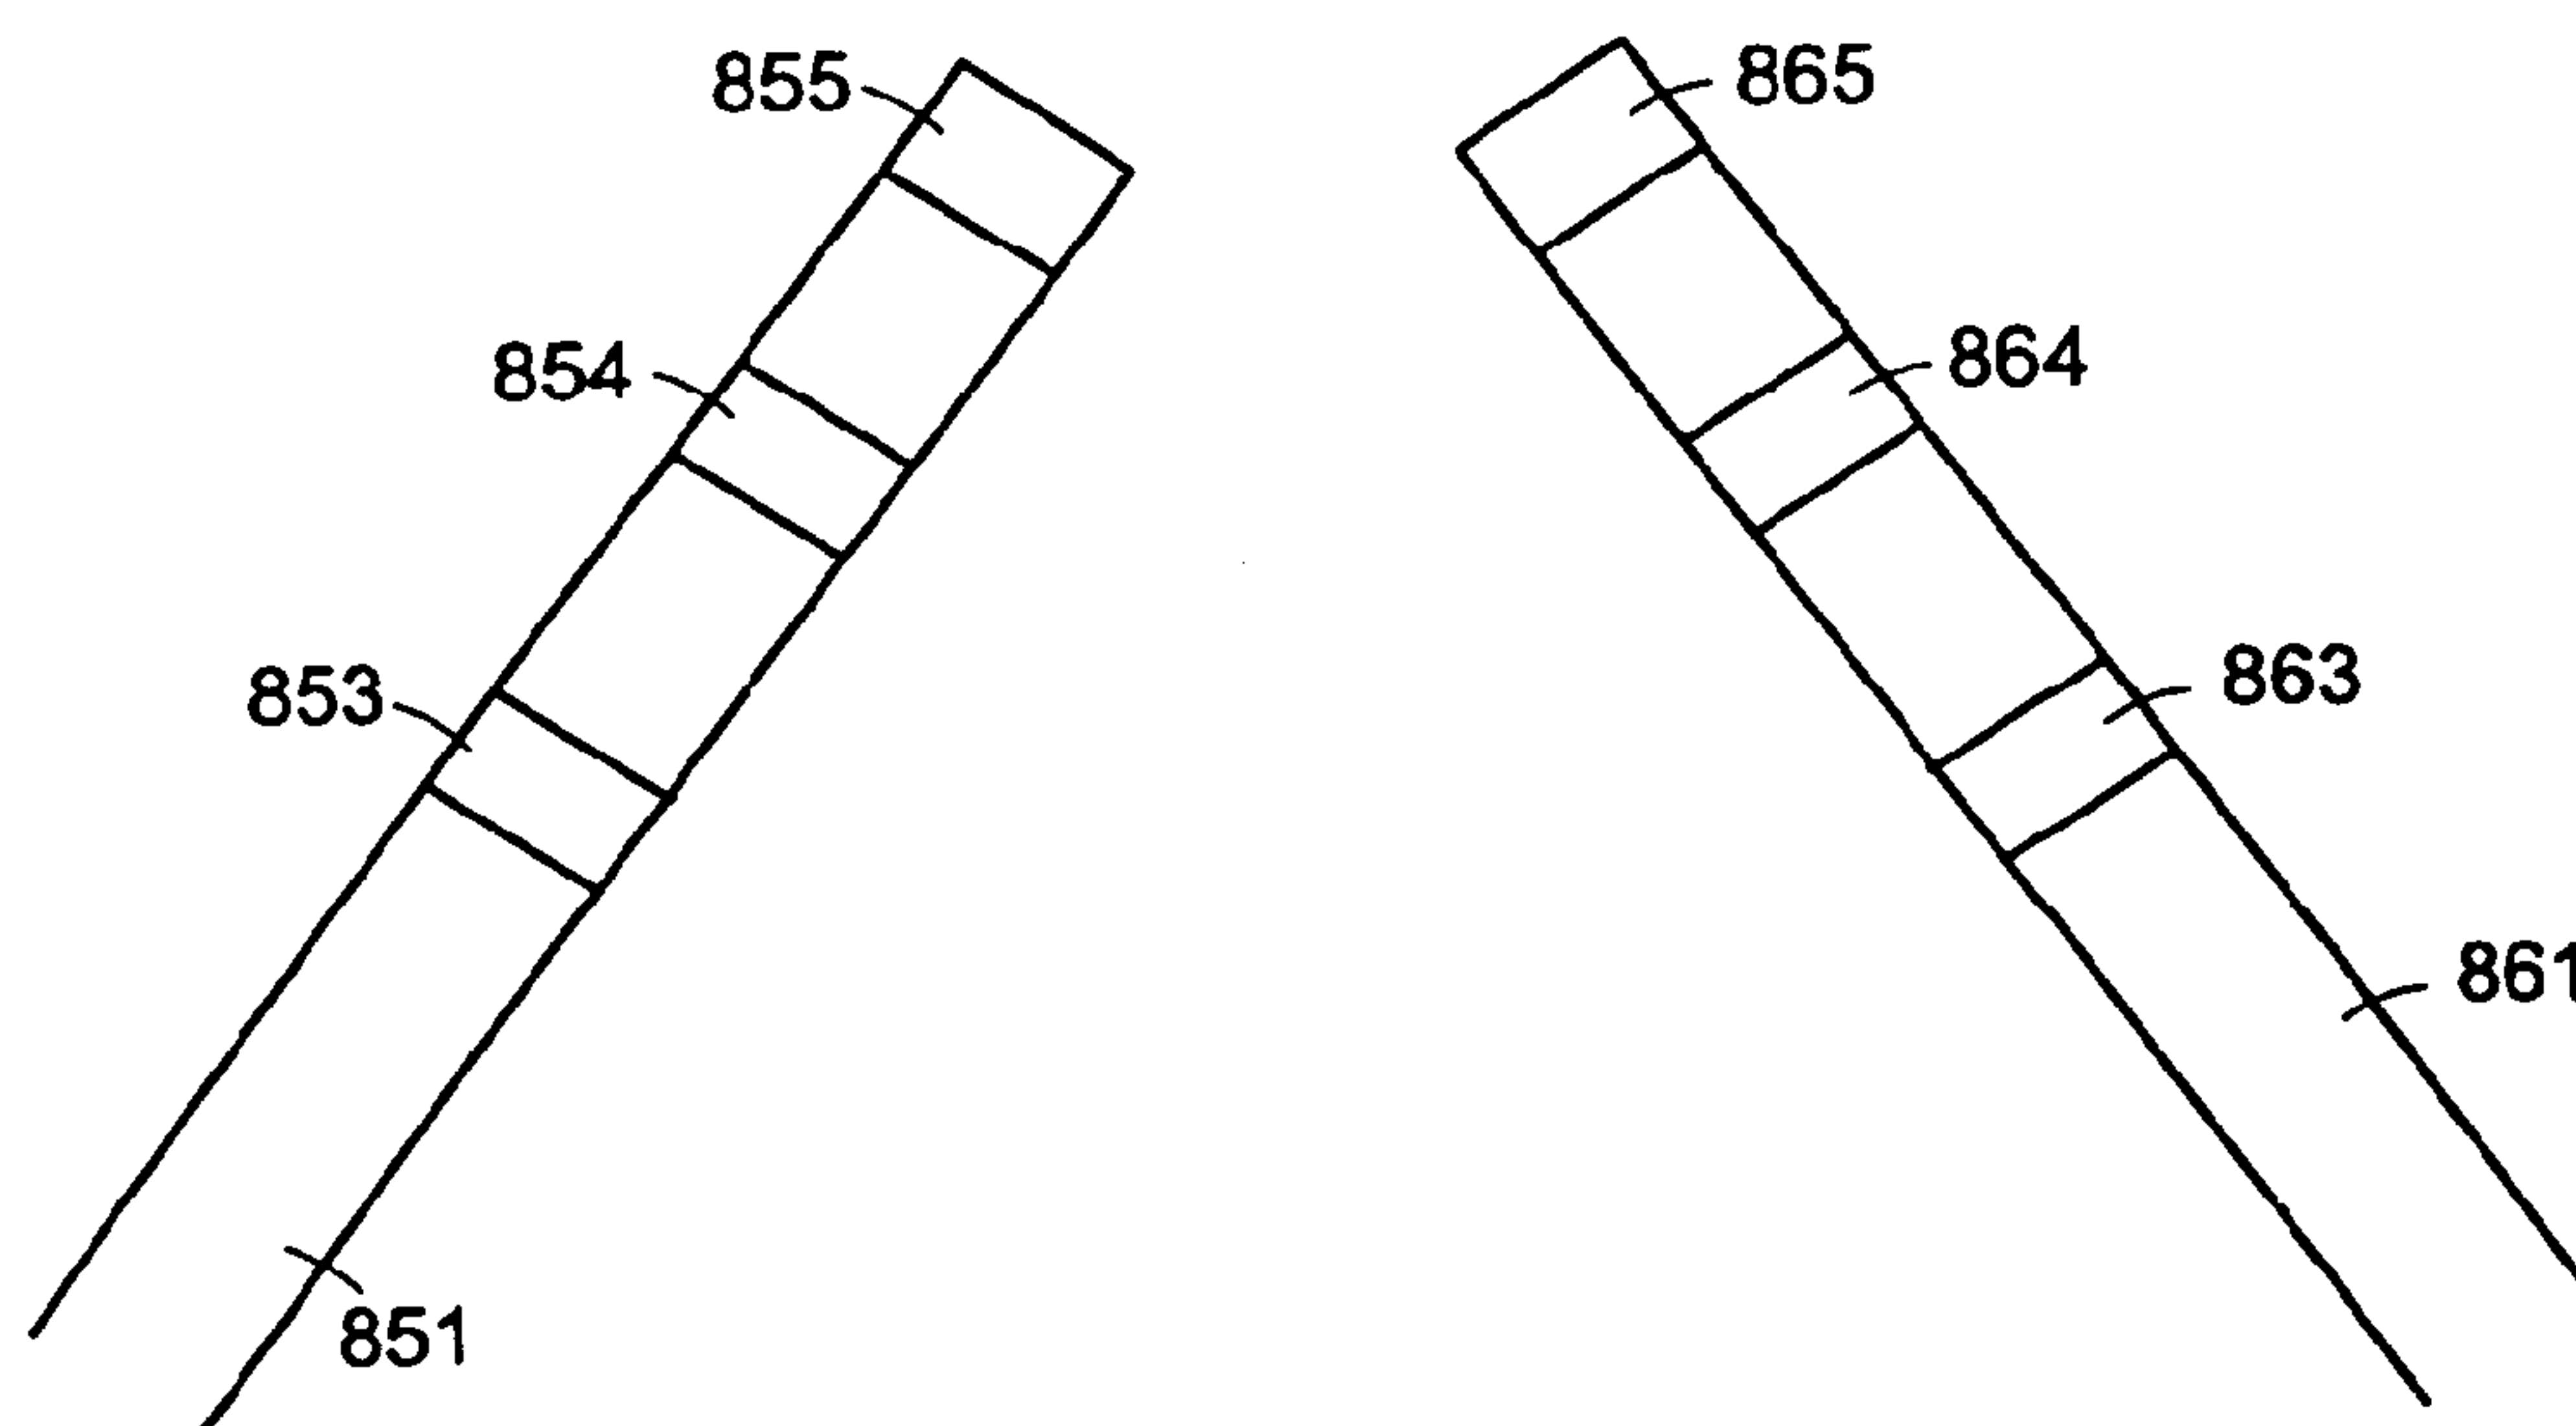


FIG. 23

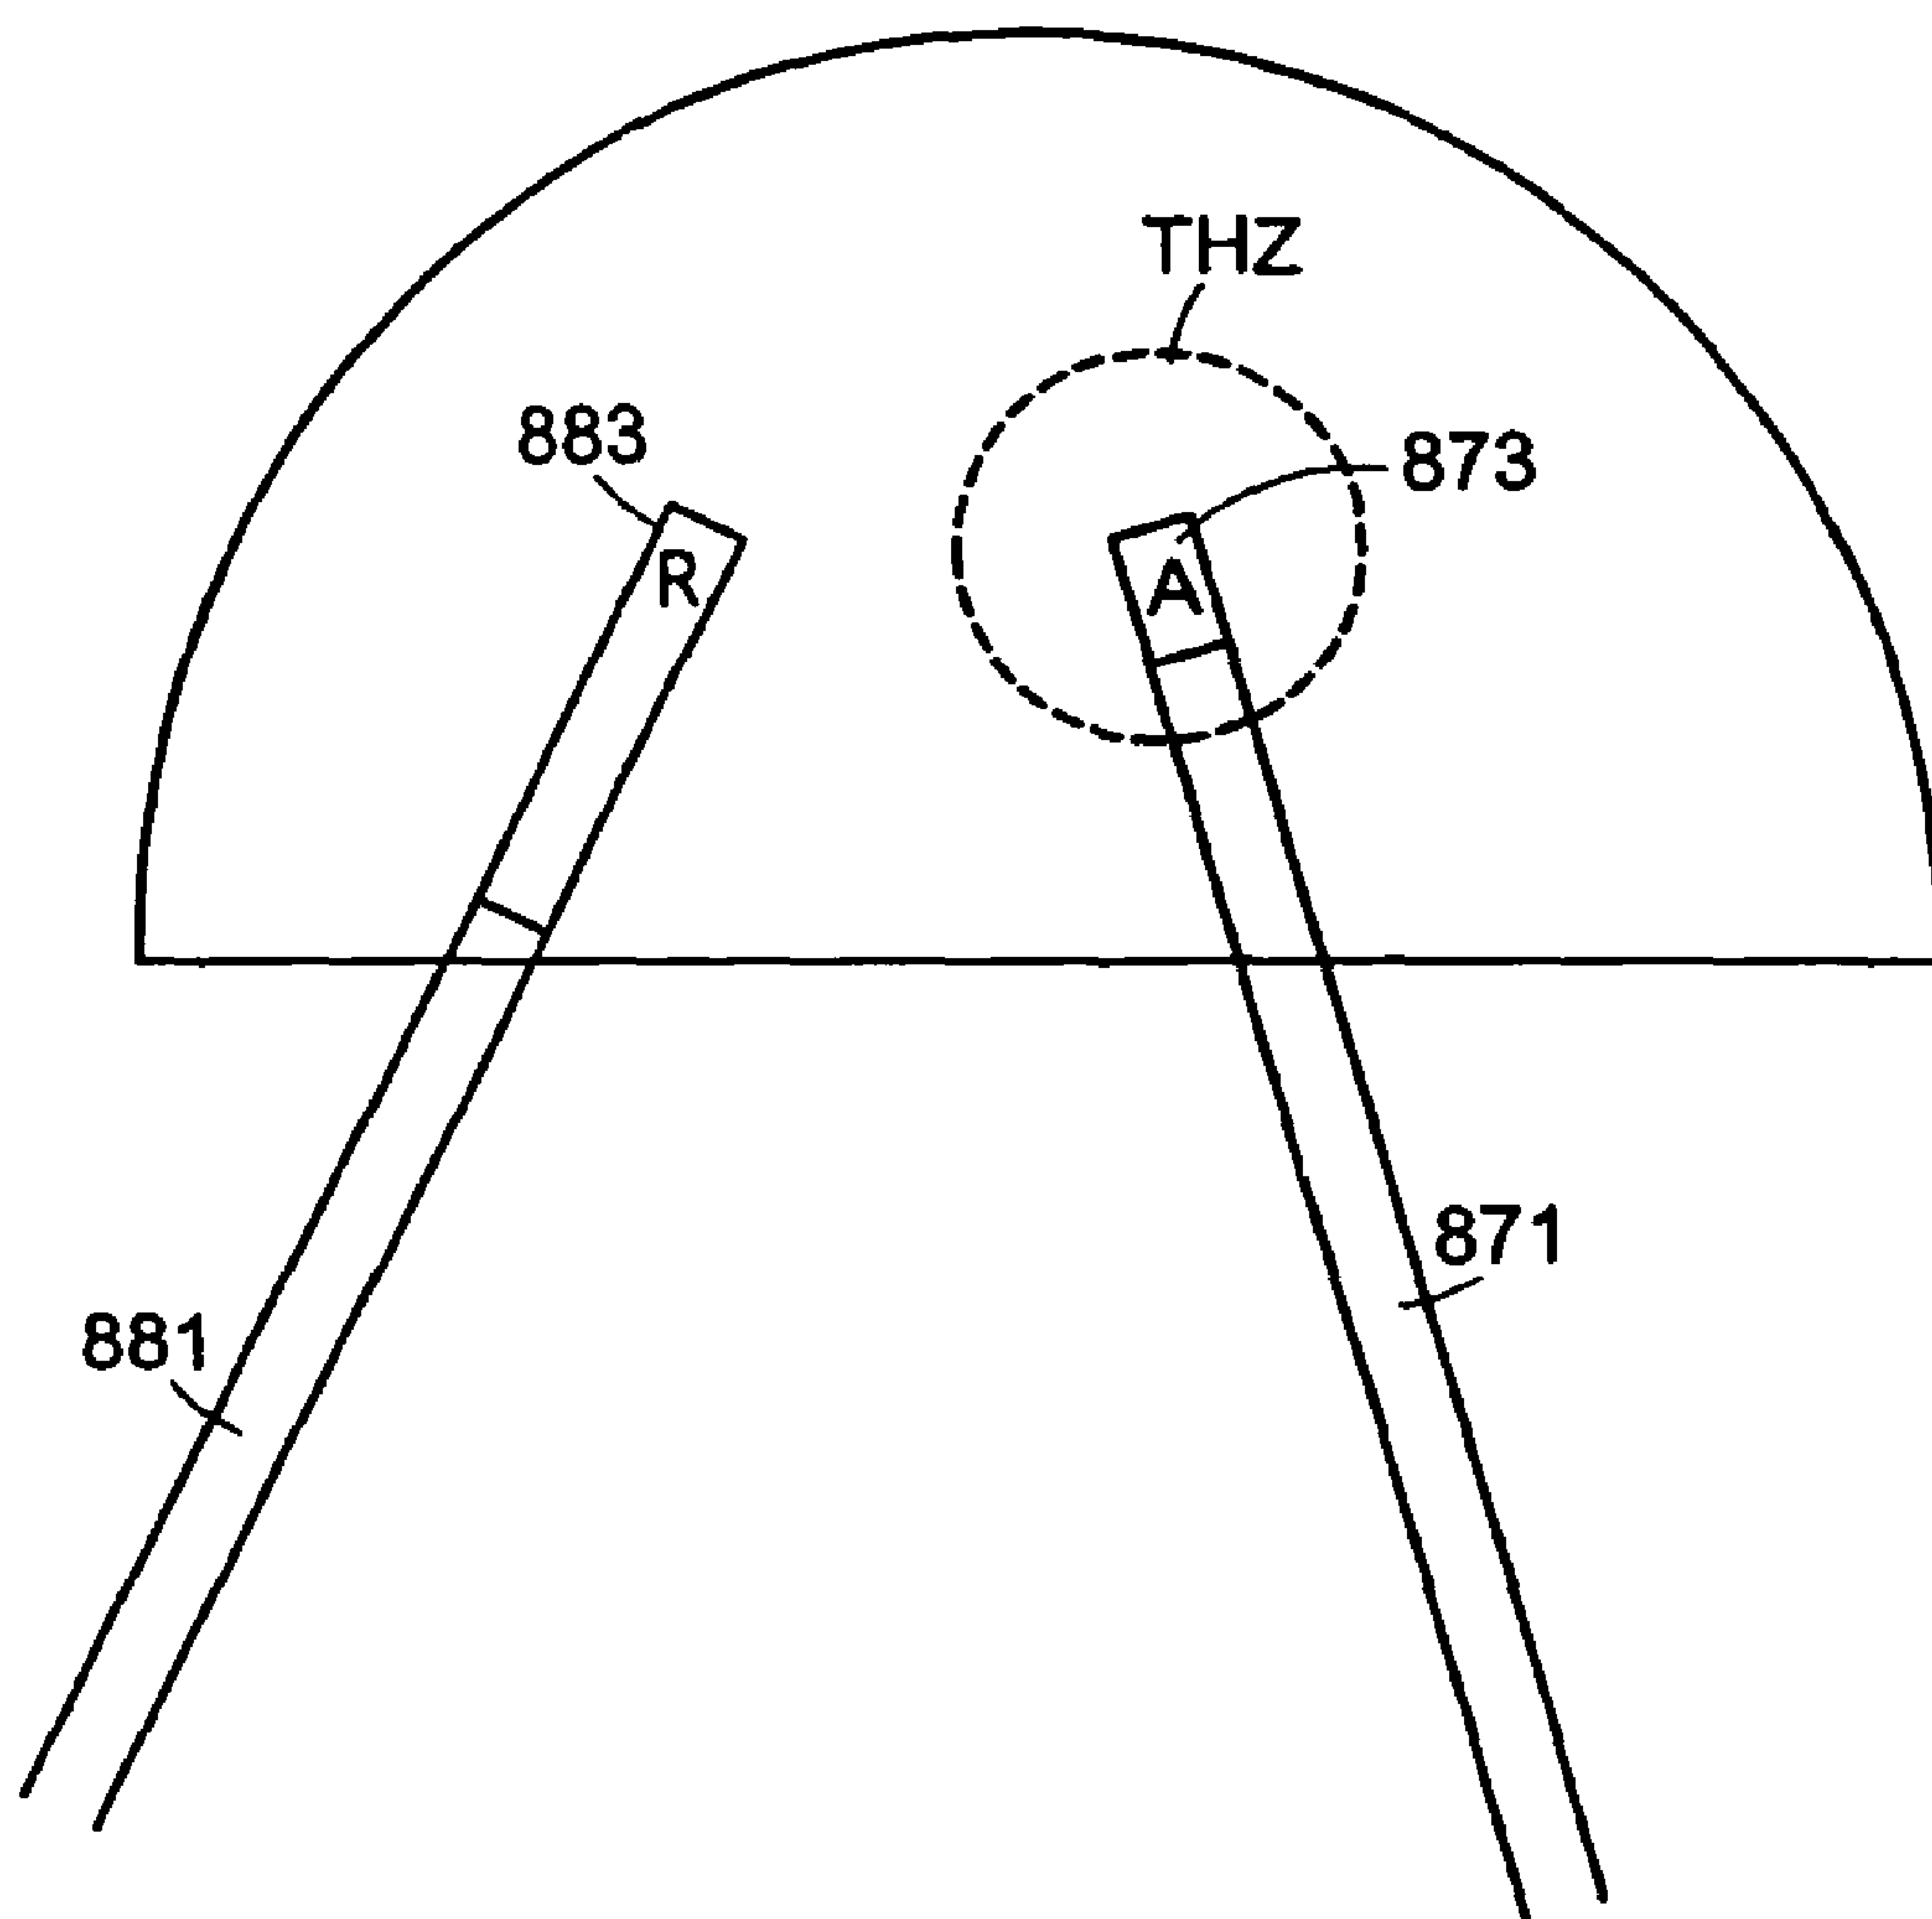


FIG. 24

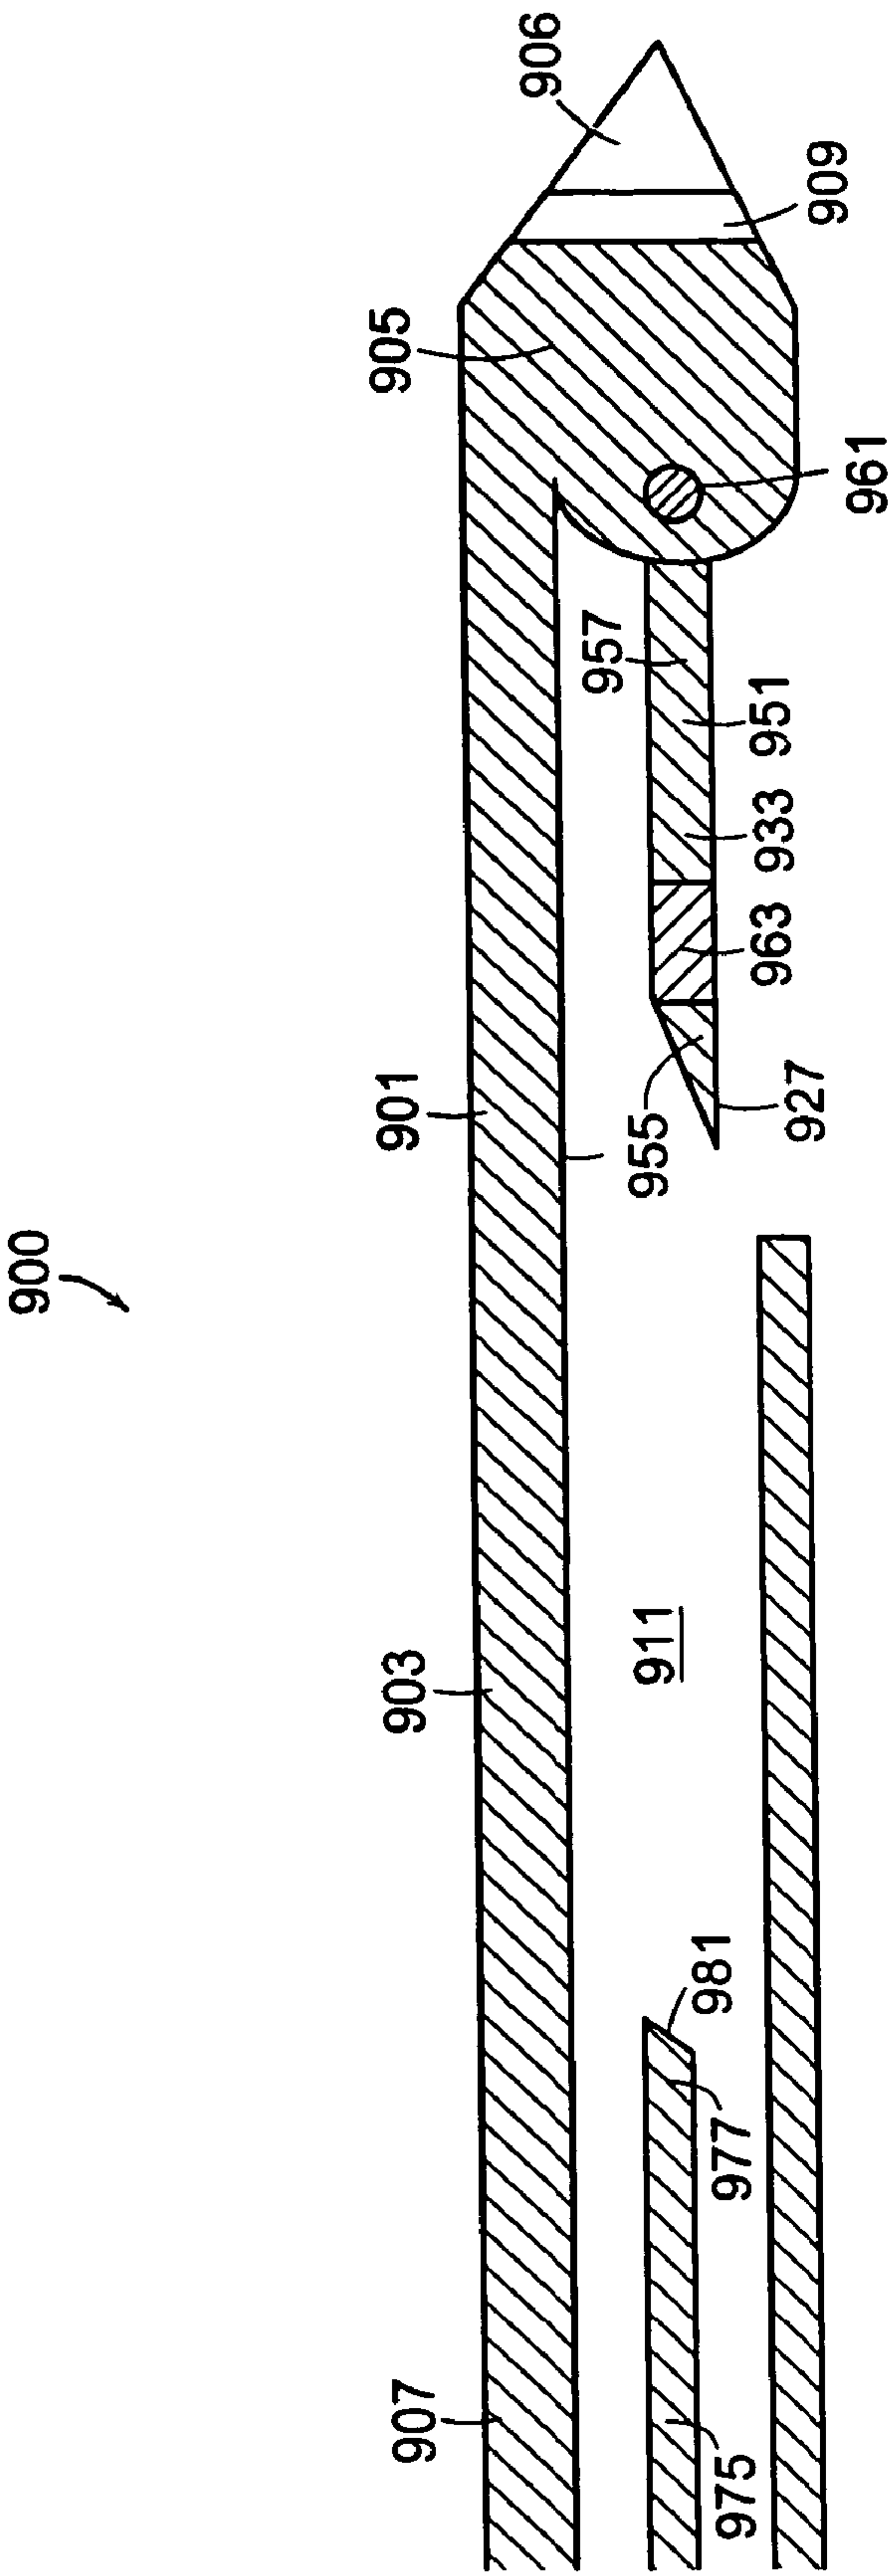


FIG. 25

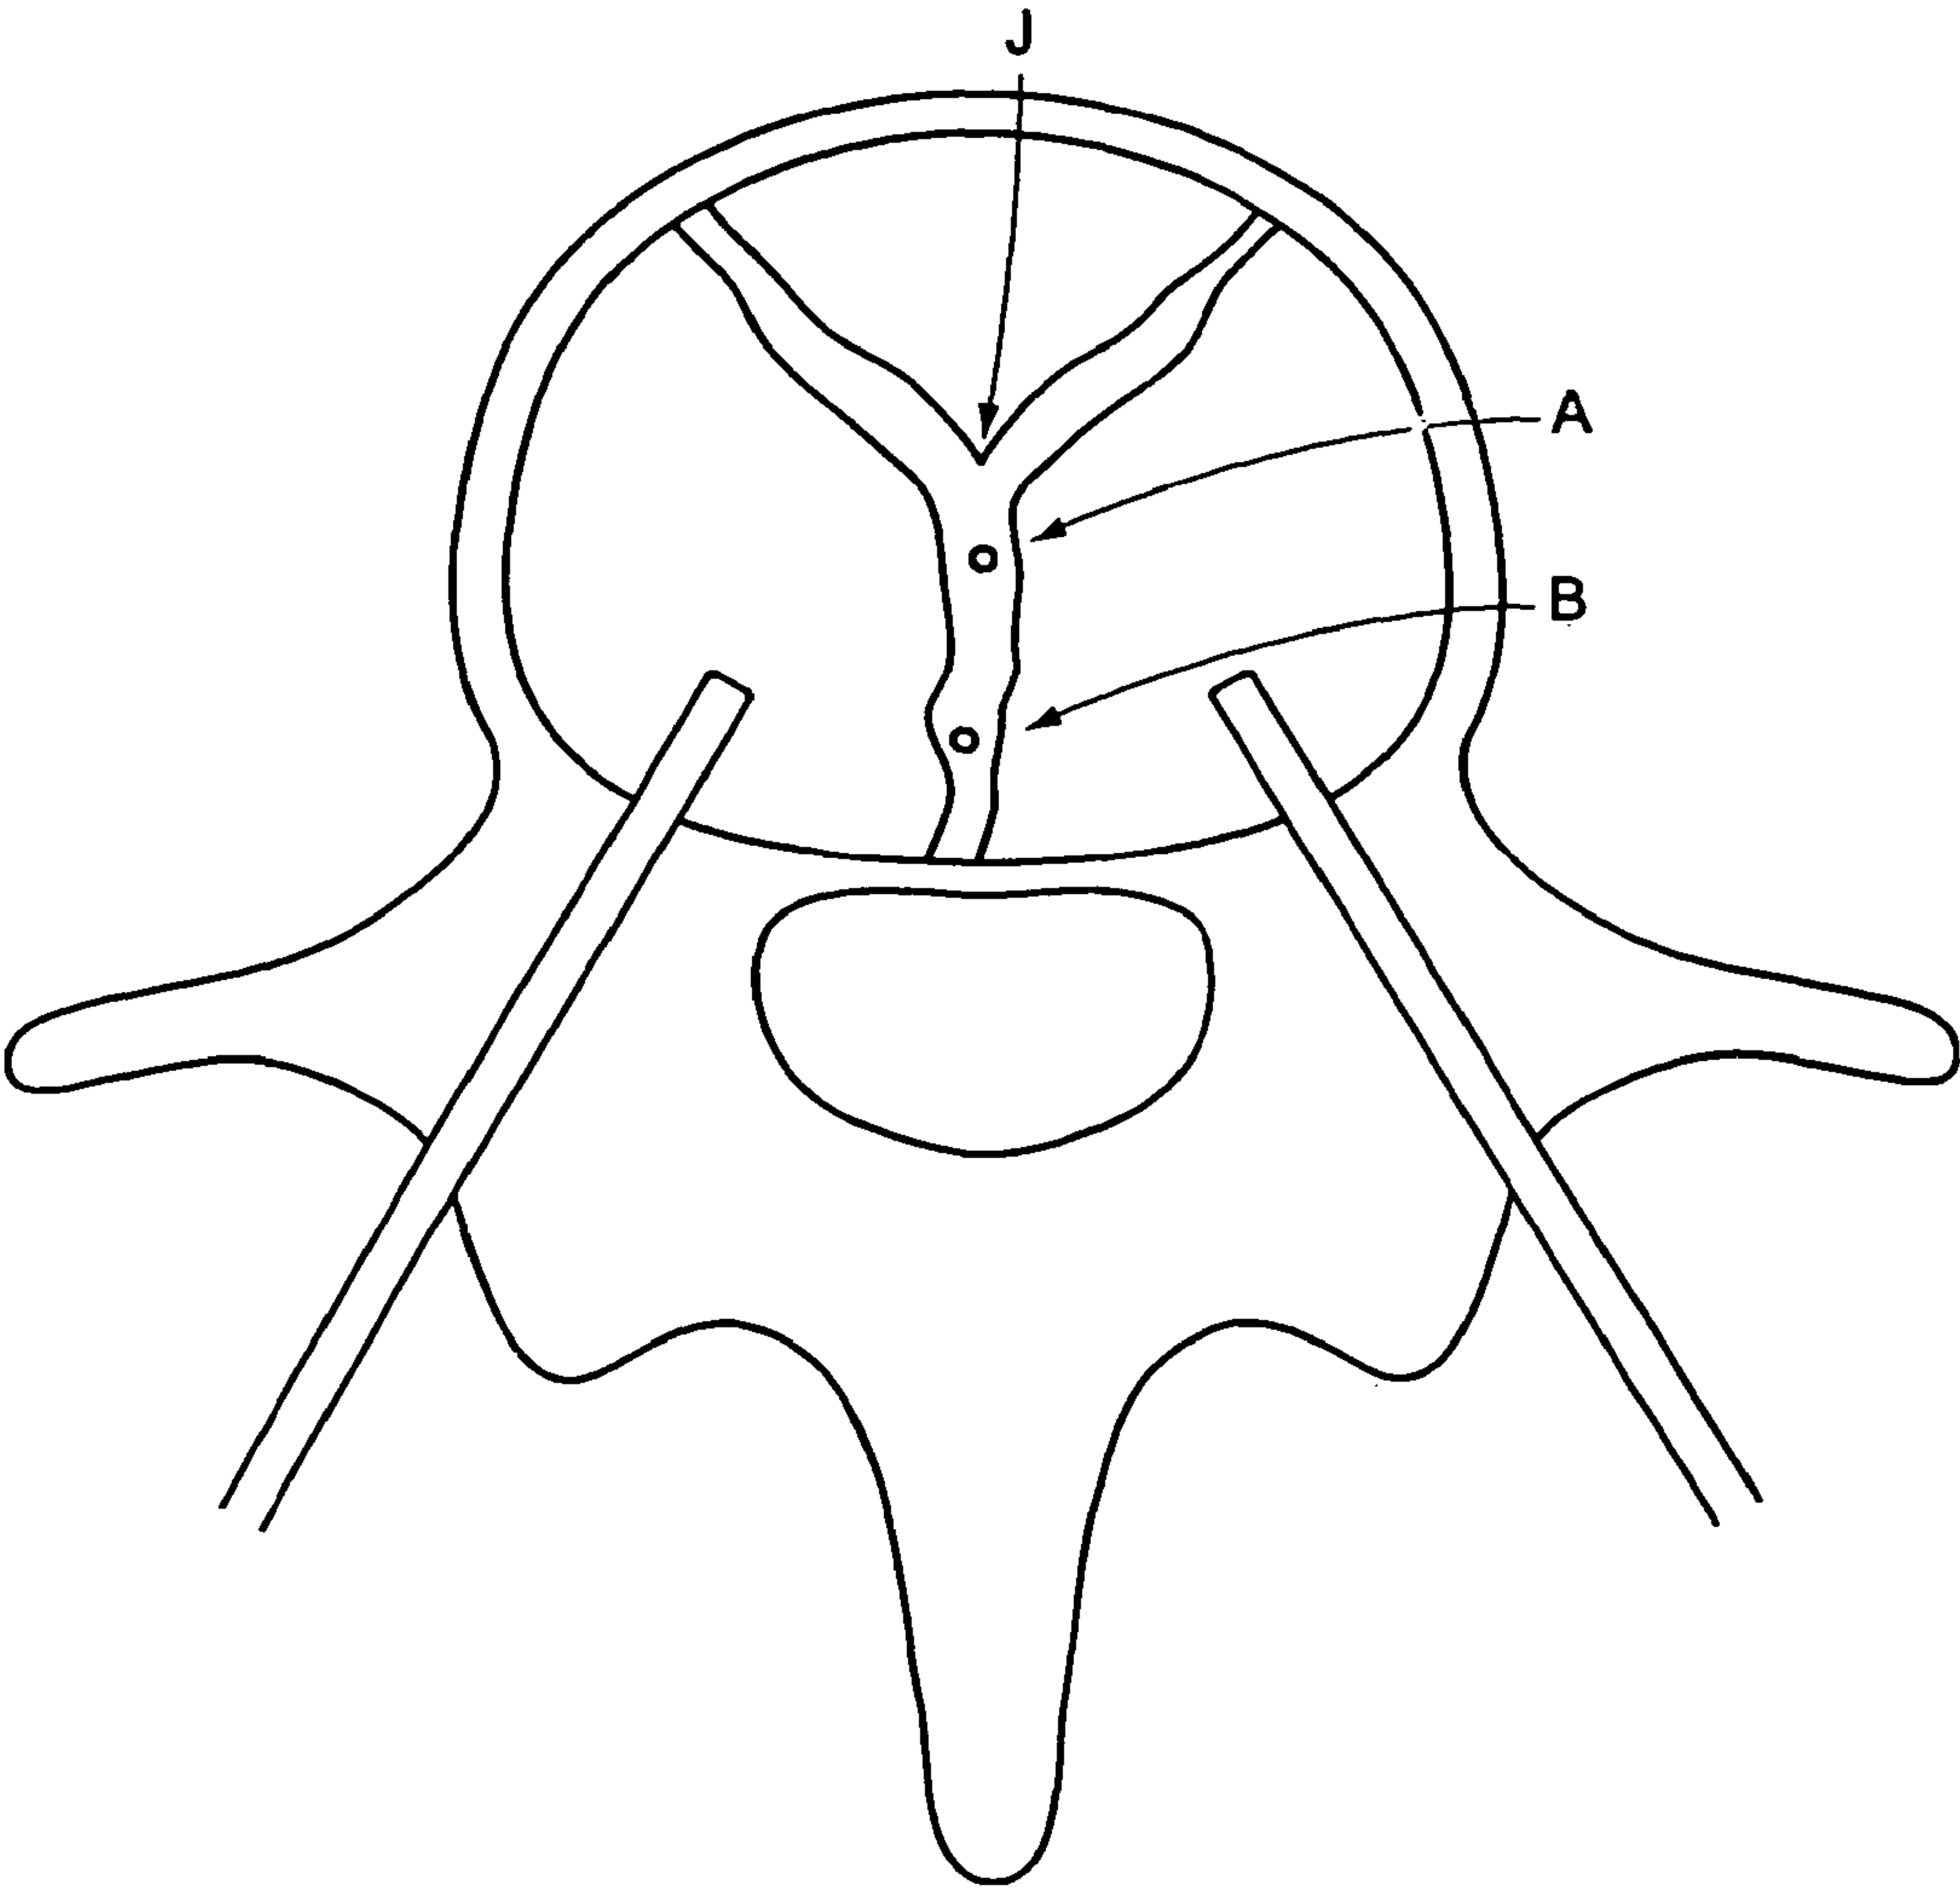


FIG. 26

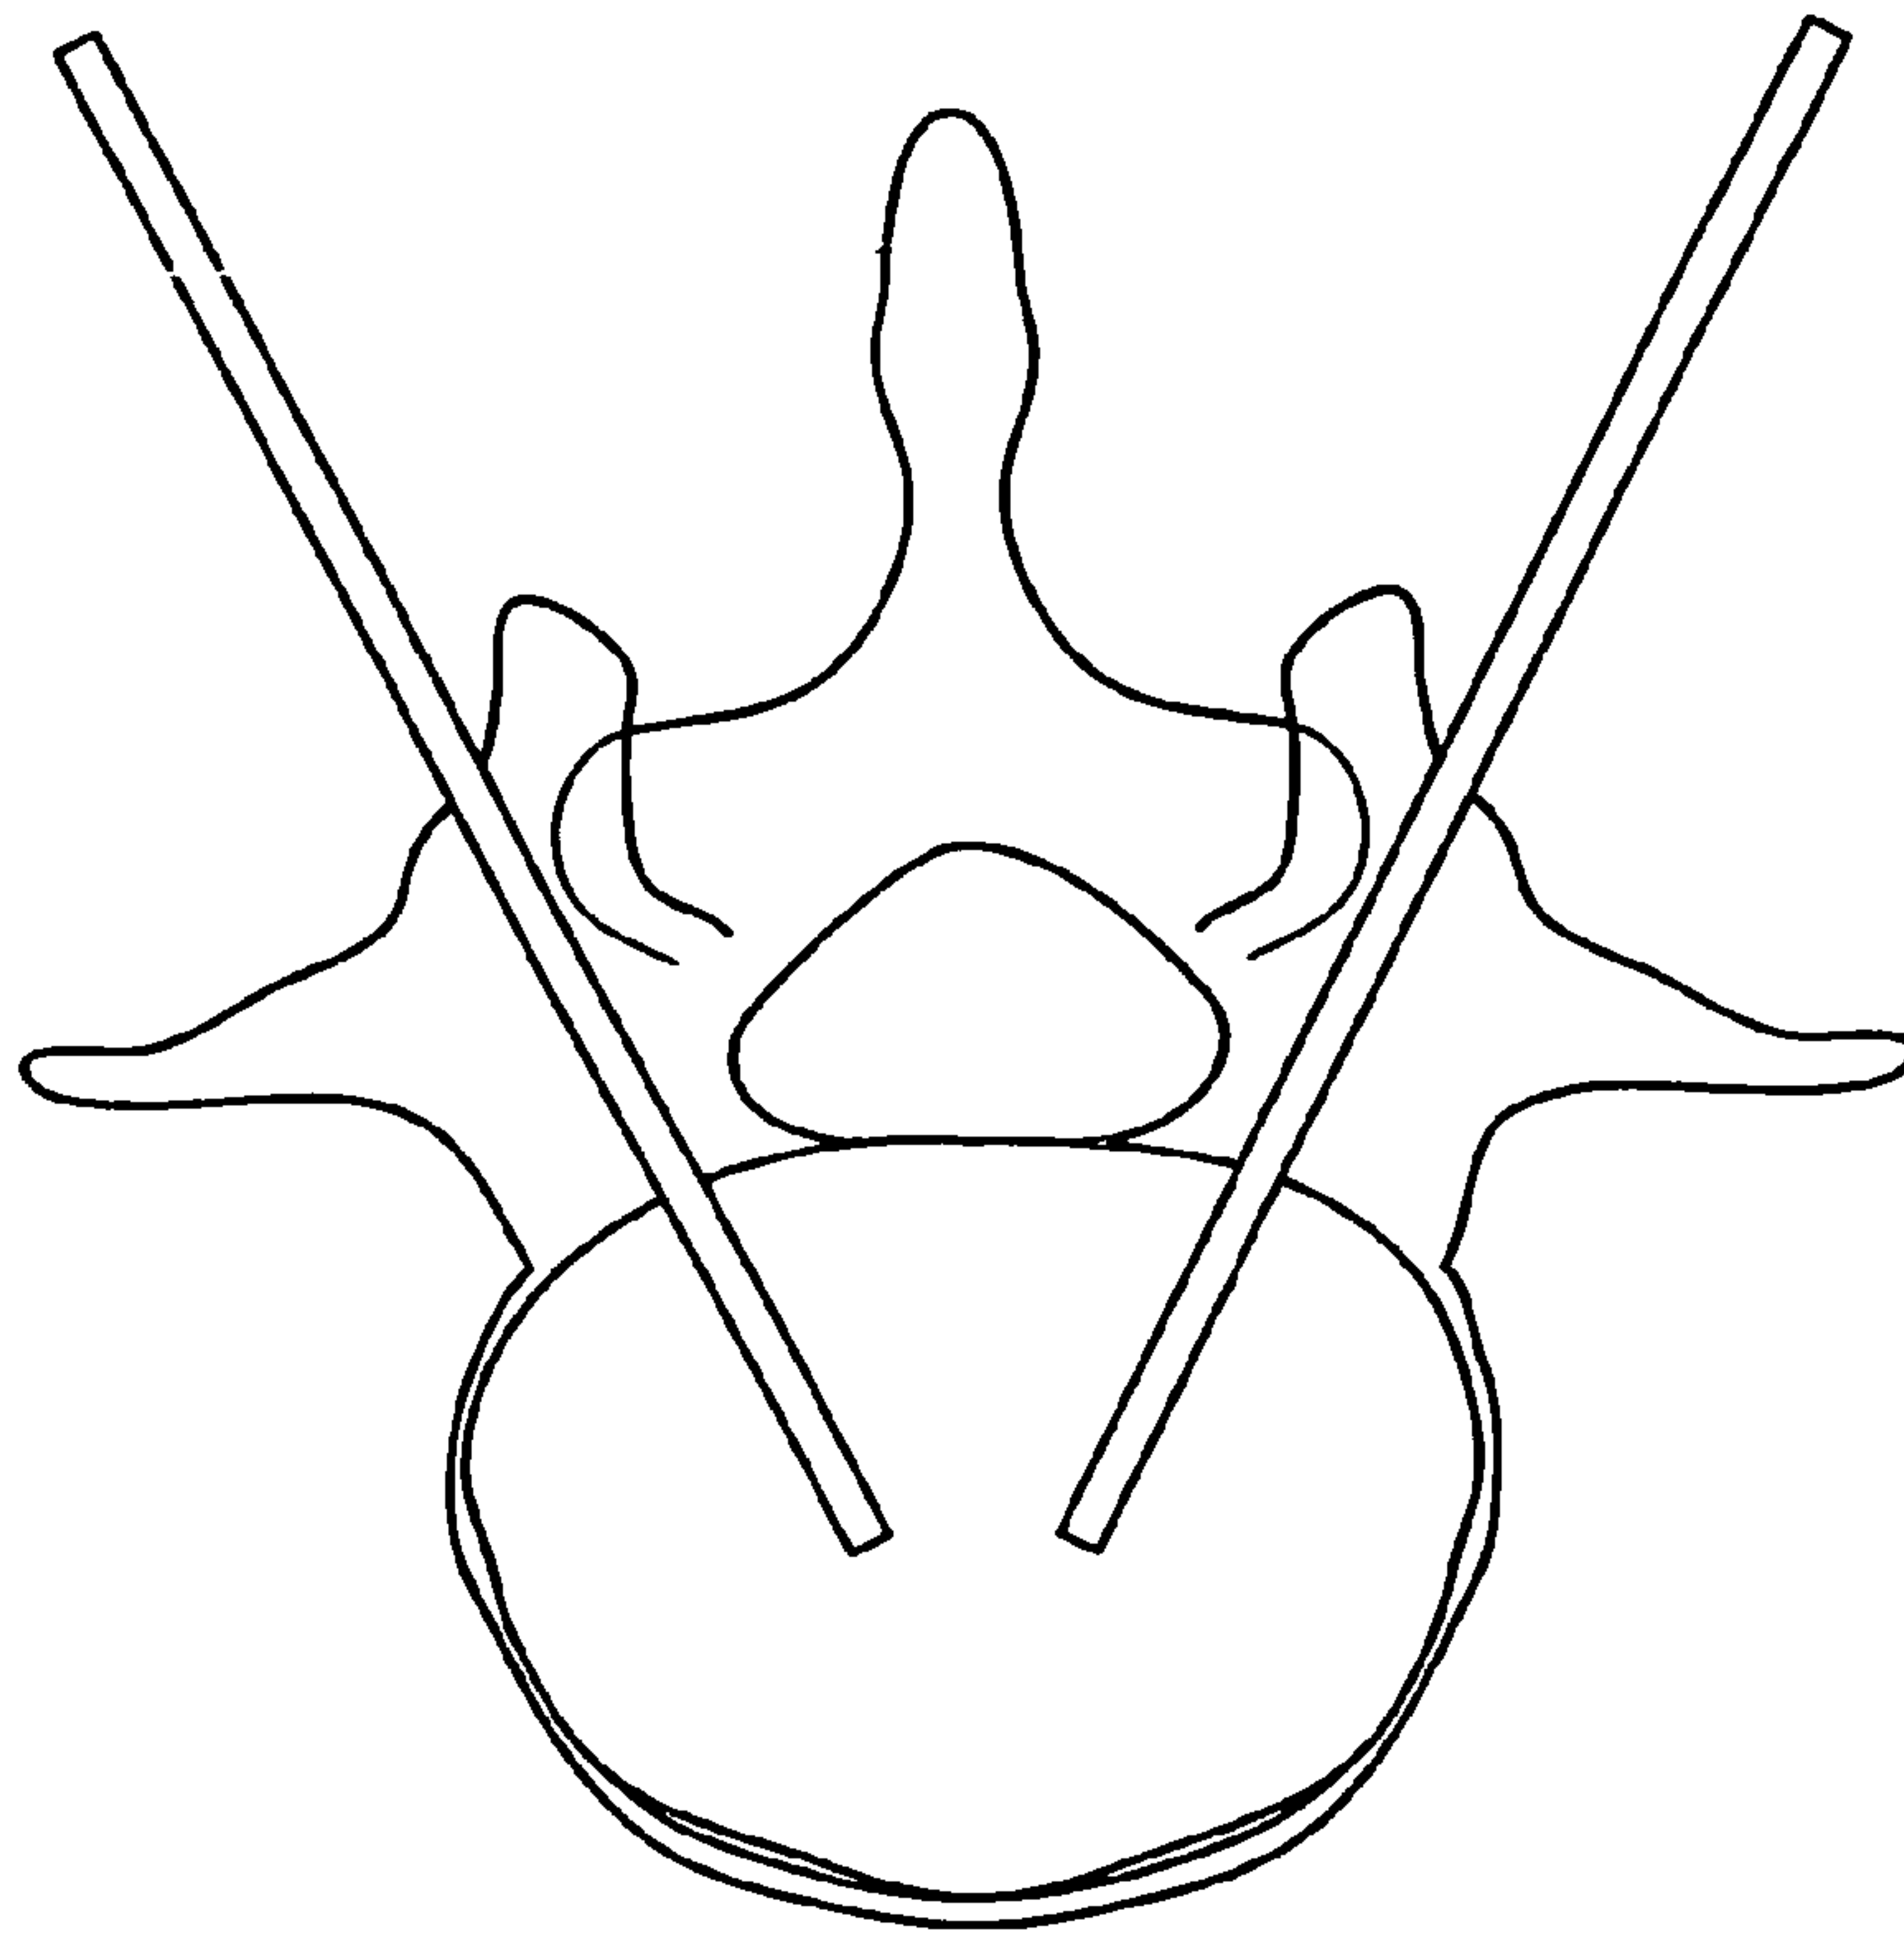


FIG. 27A

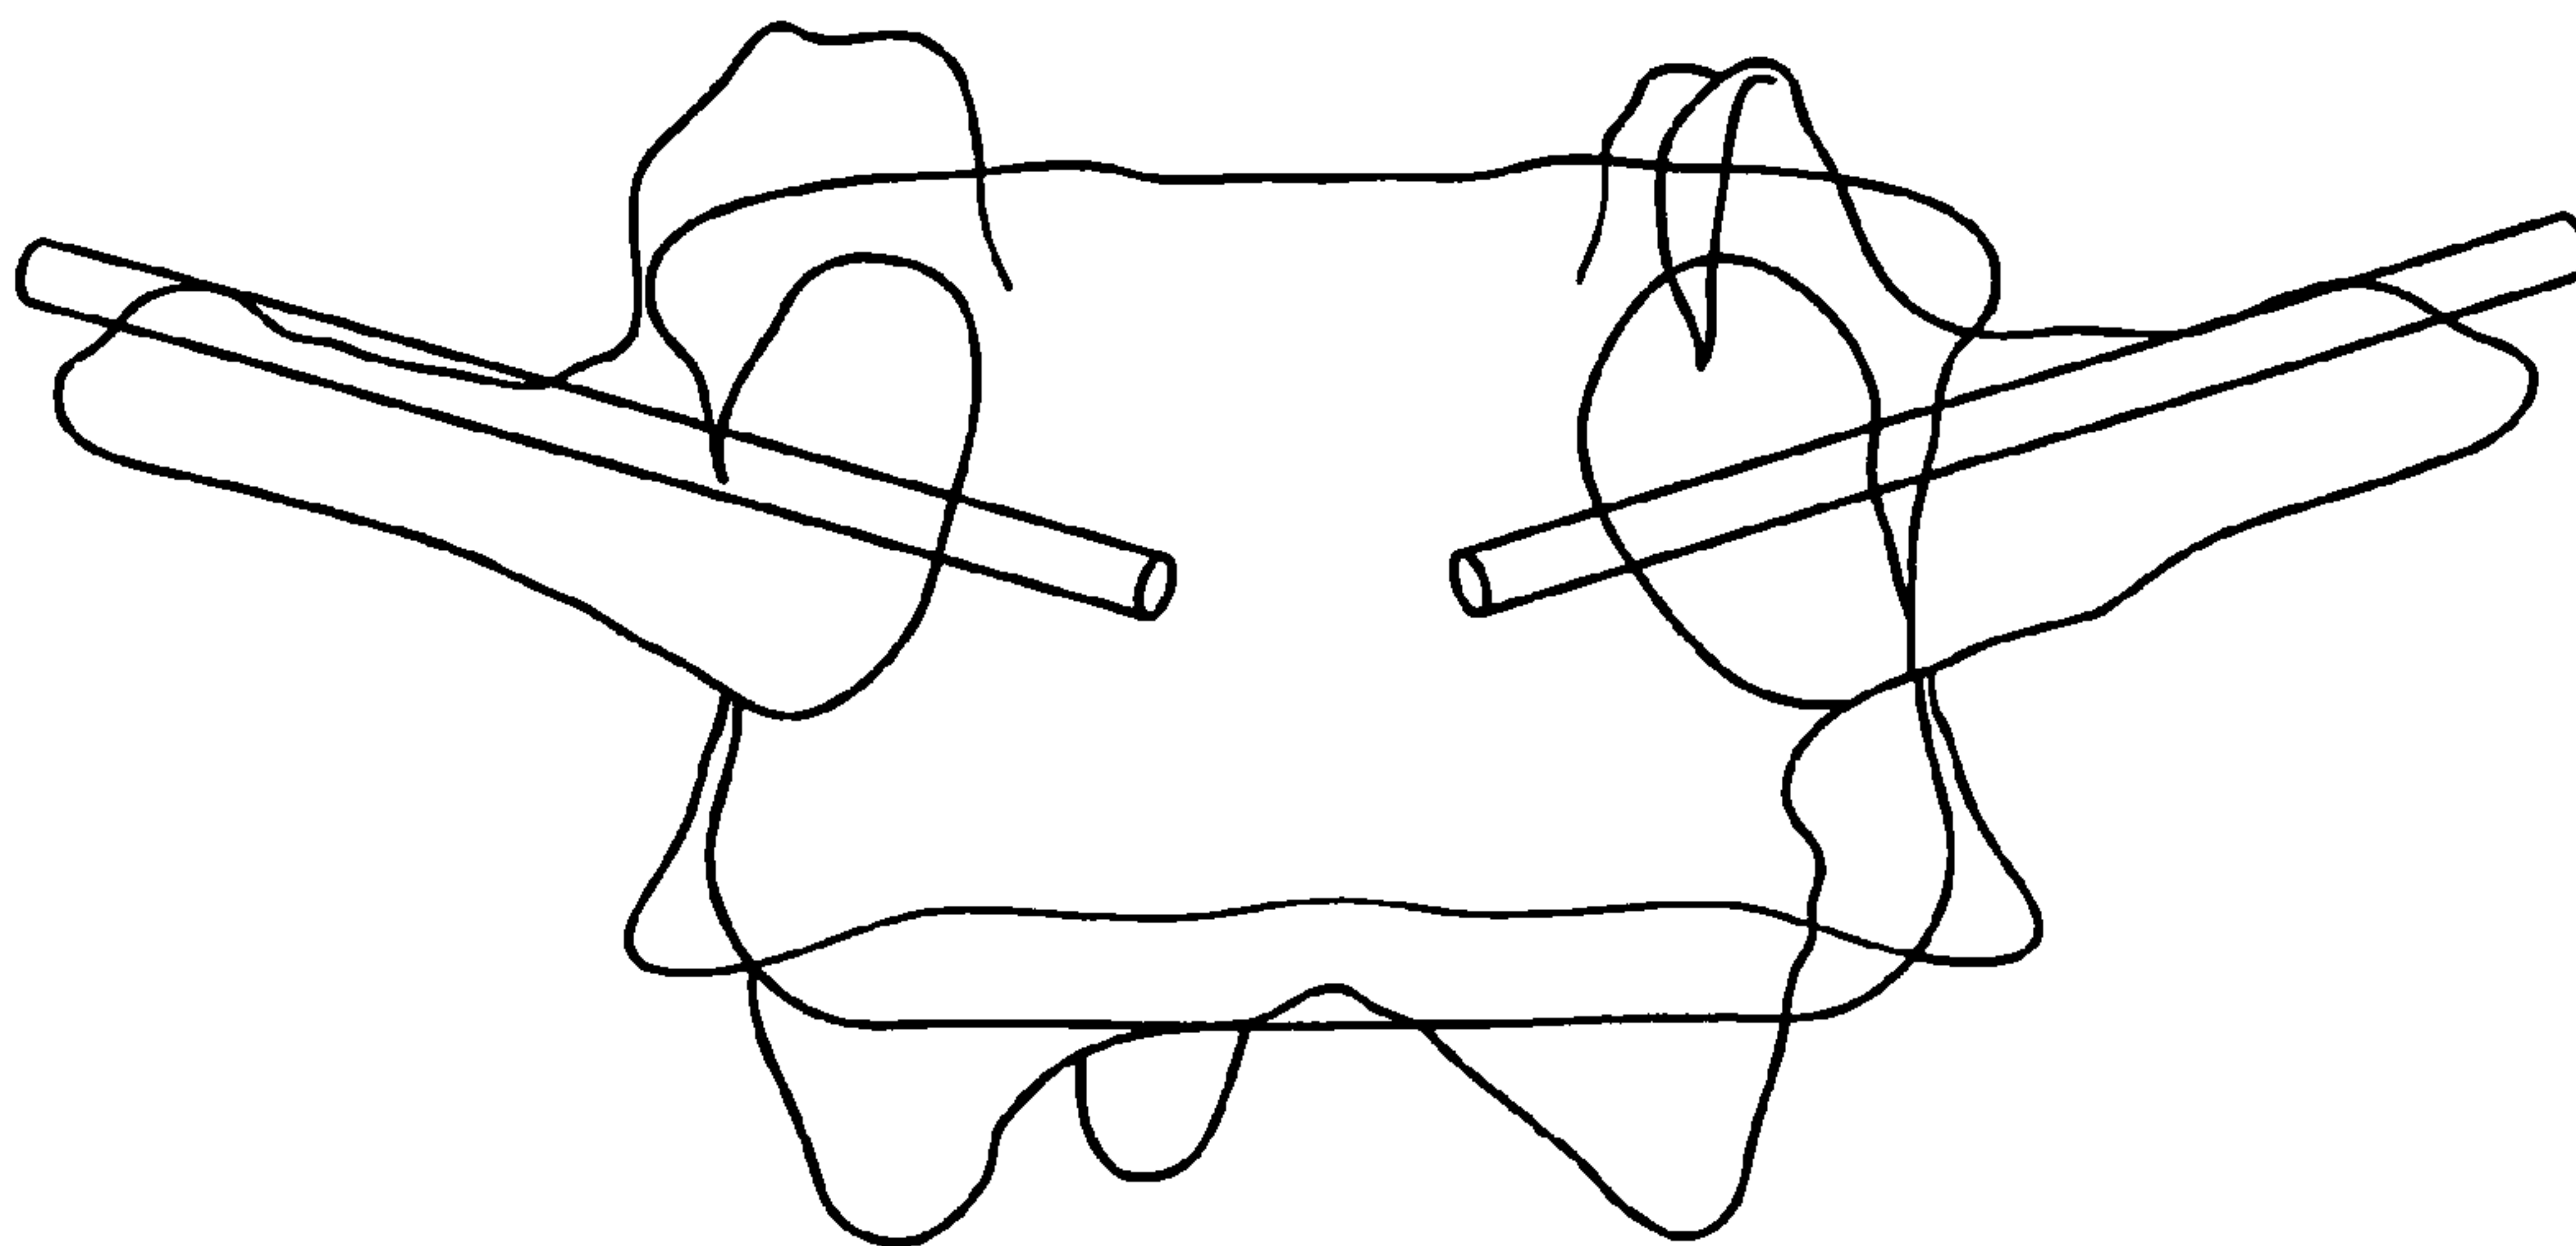


FIG. 27B

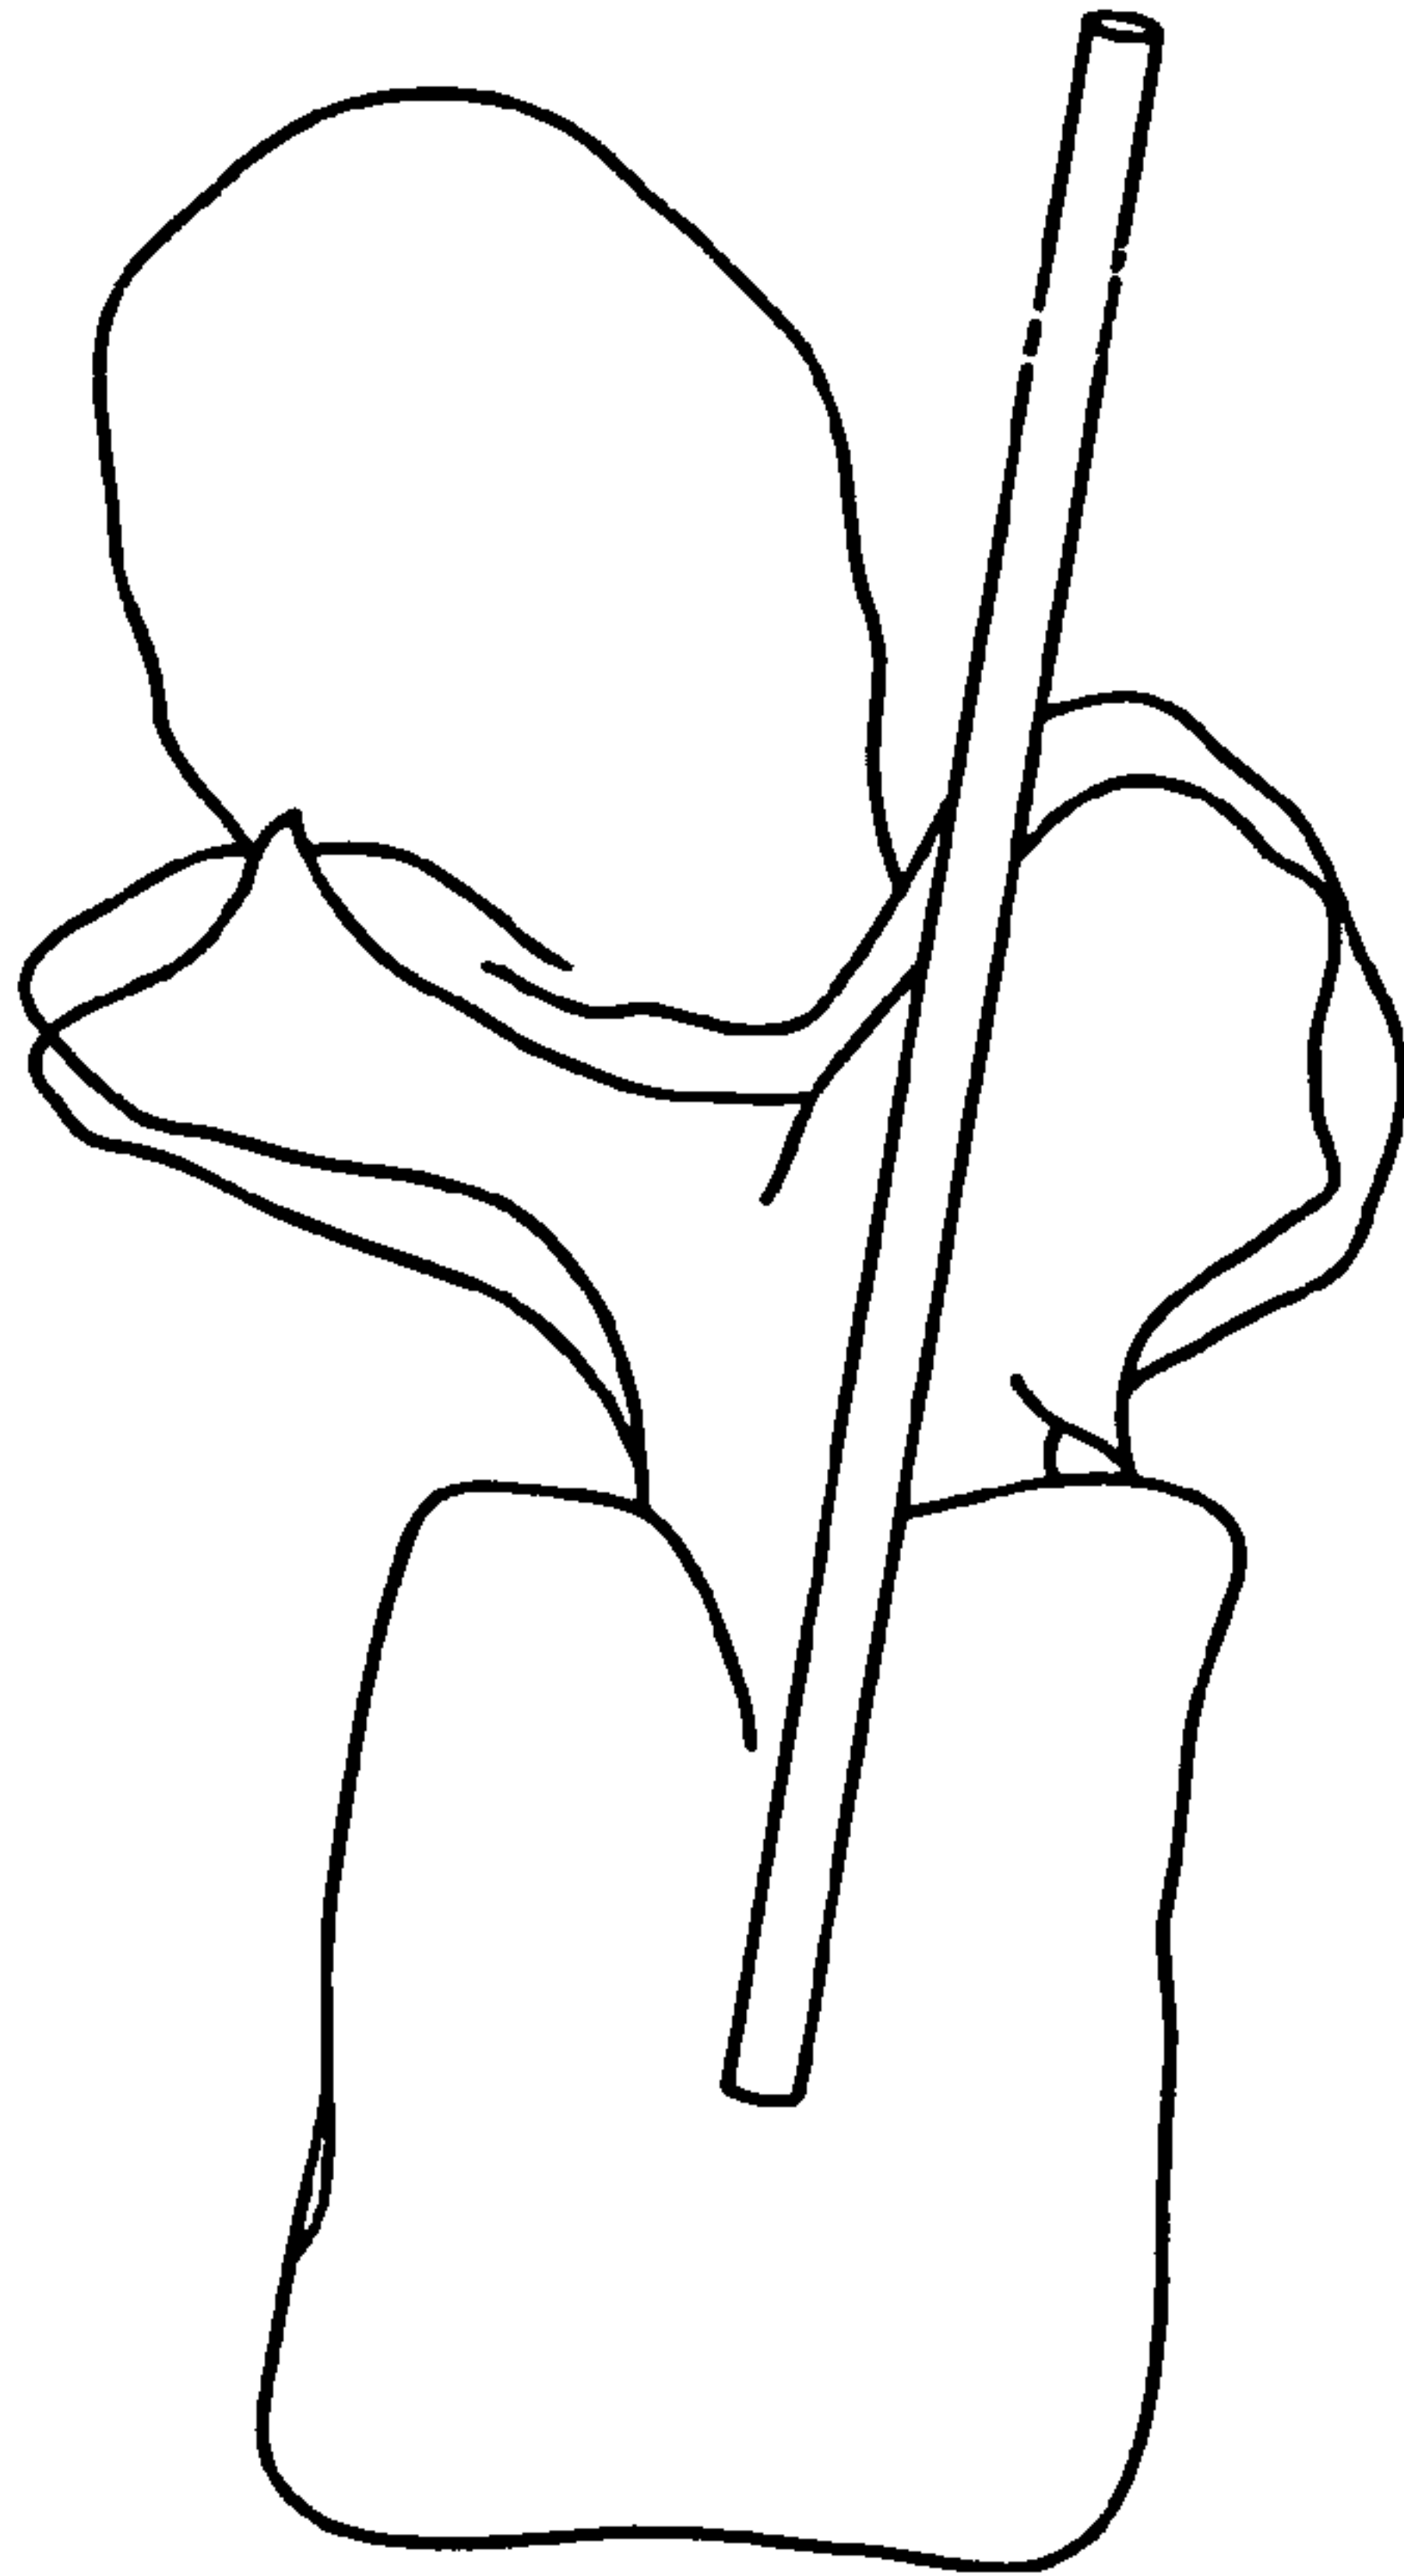


FIG. 27C

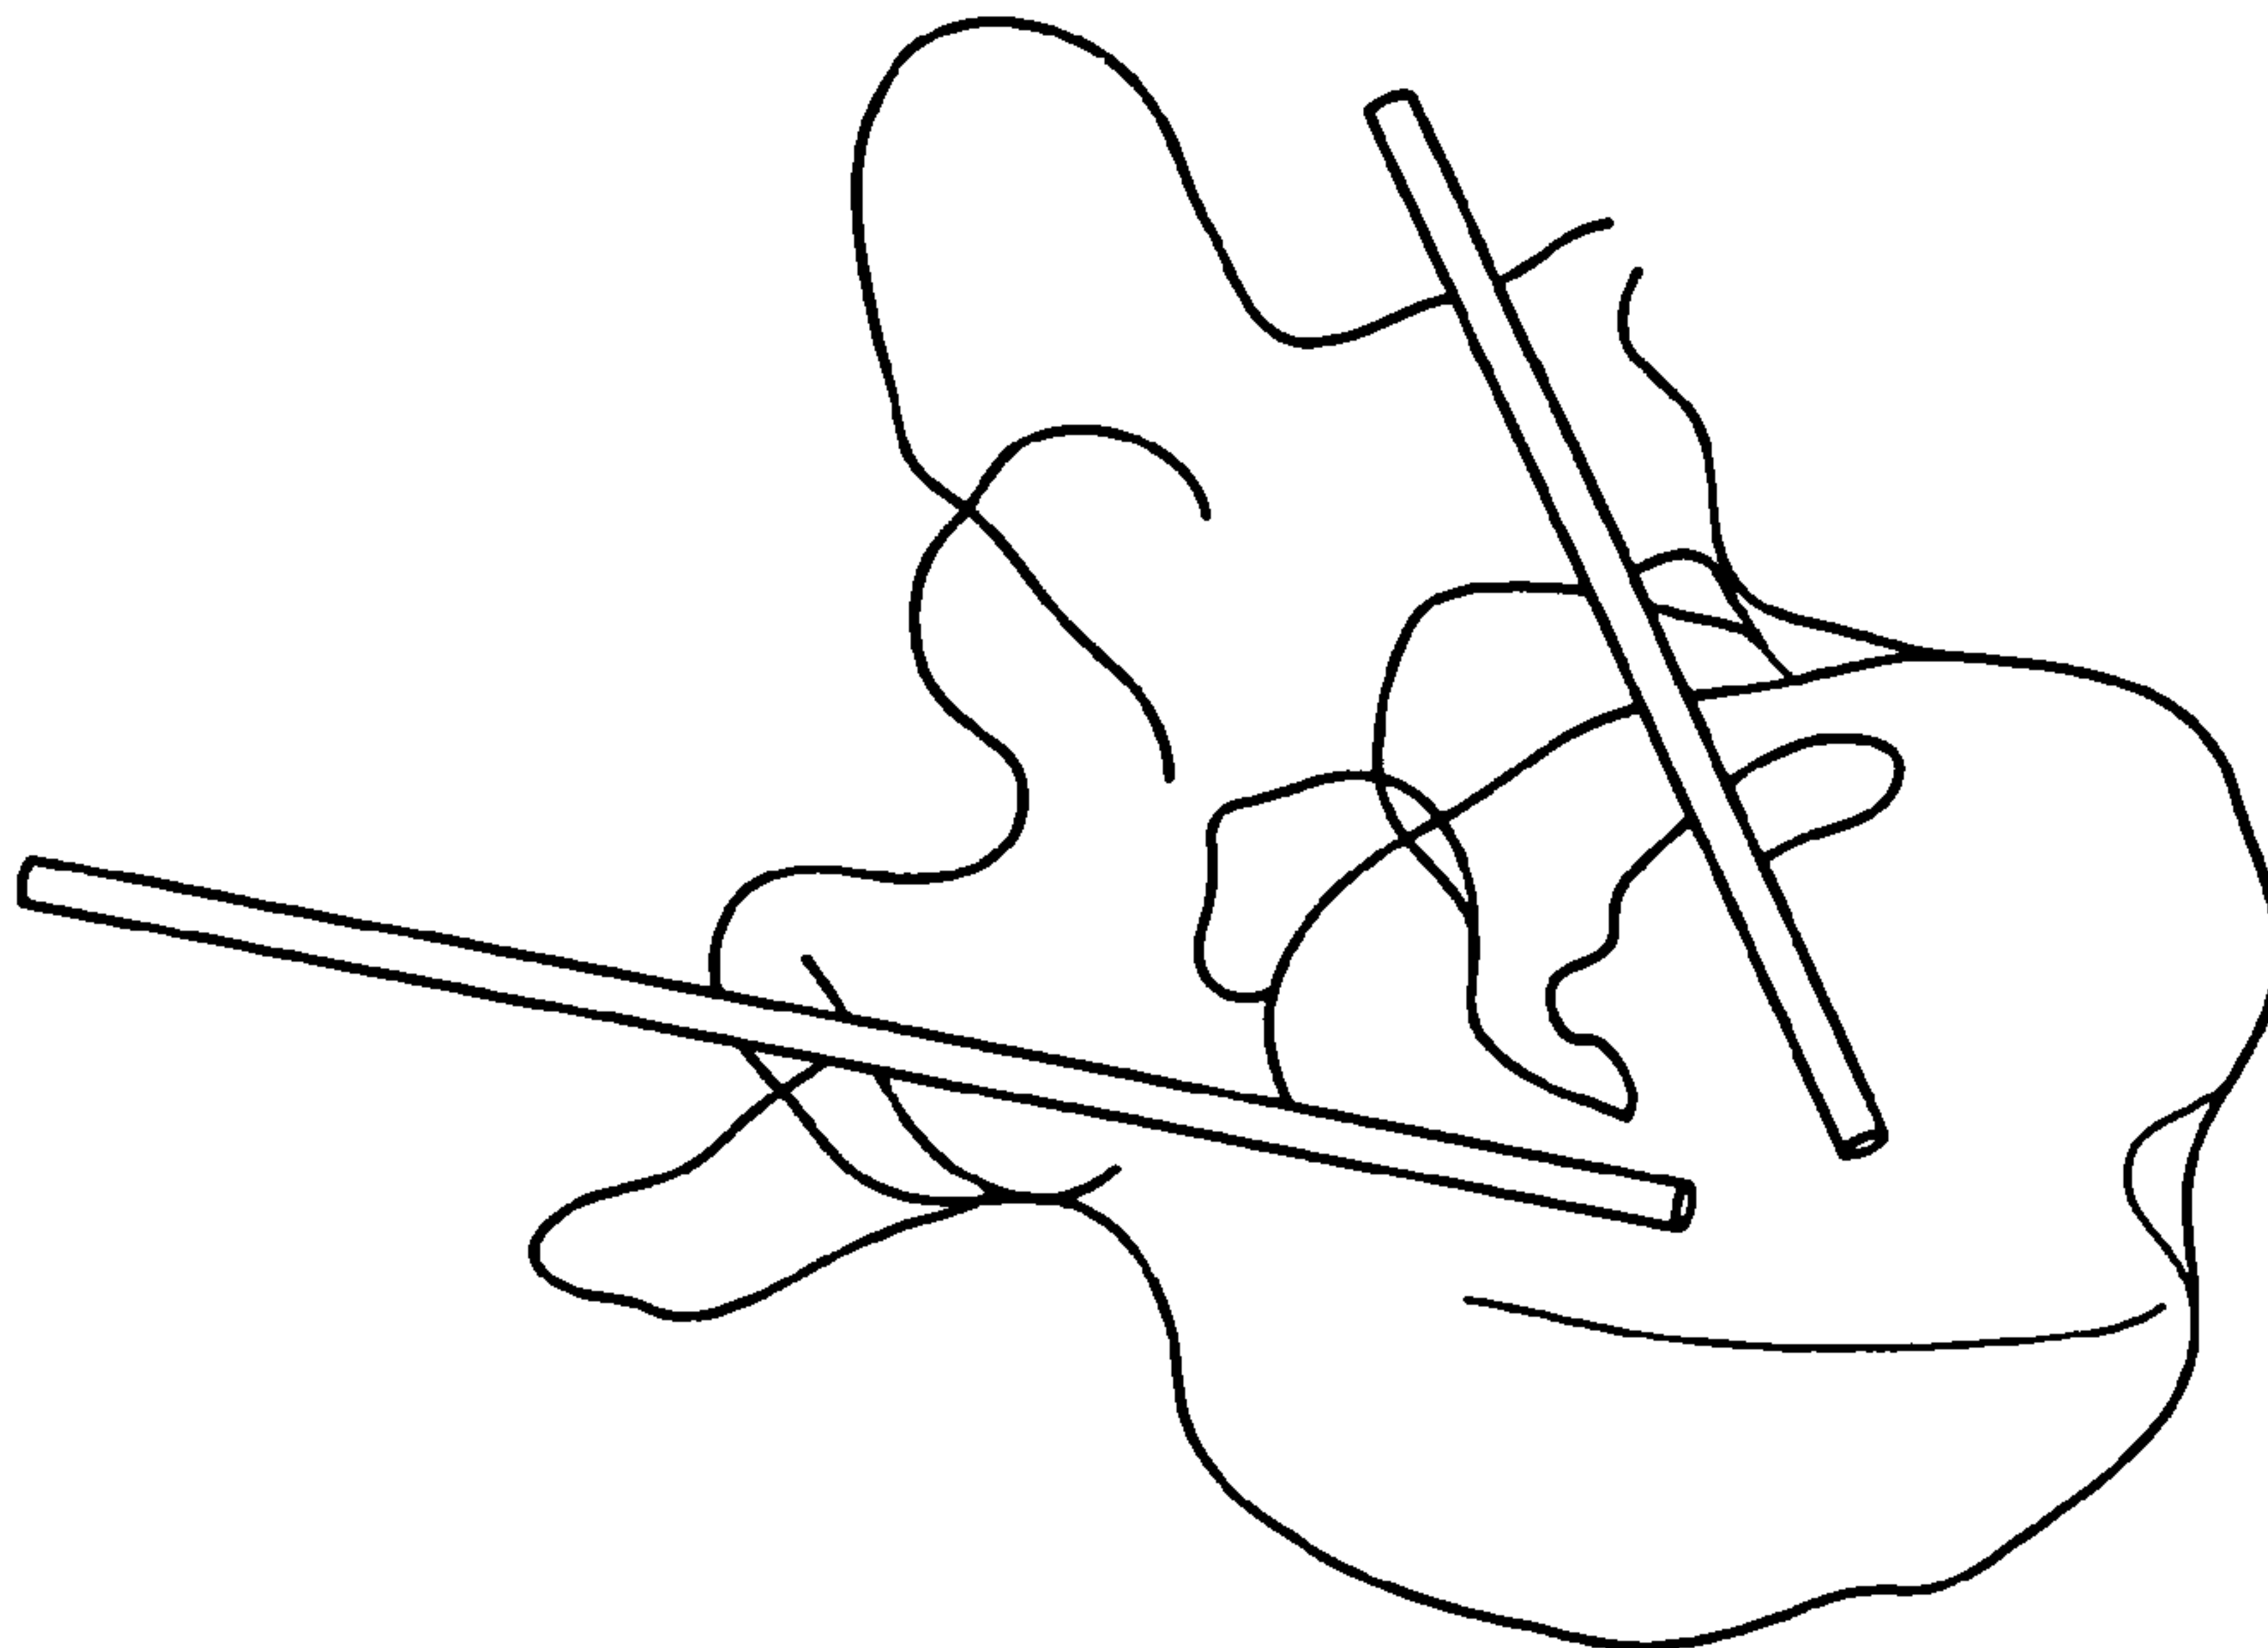


FIG. 27D

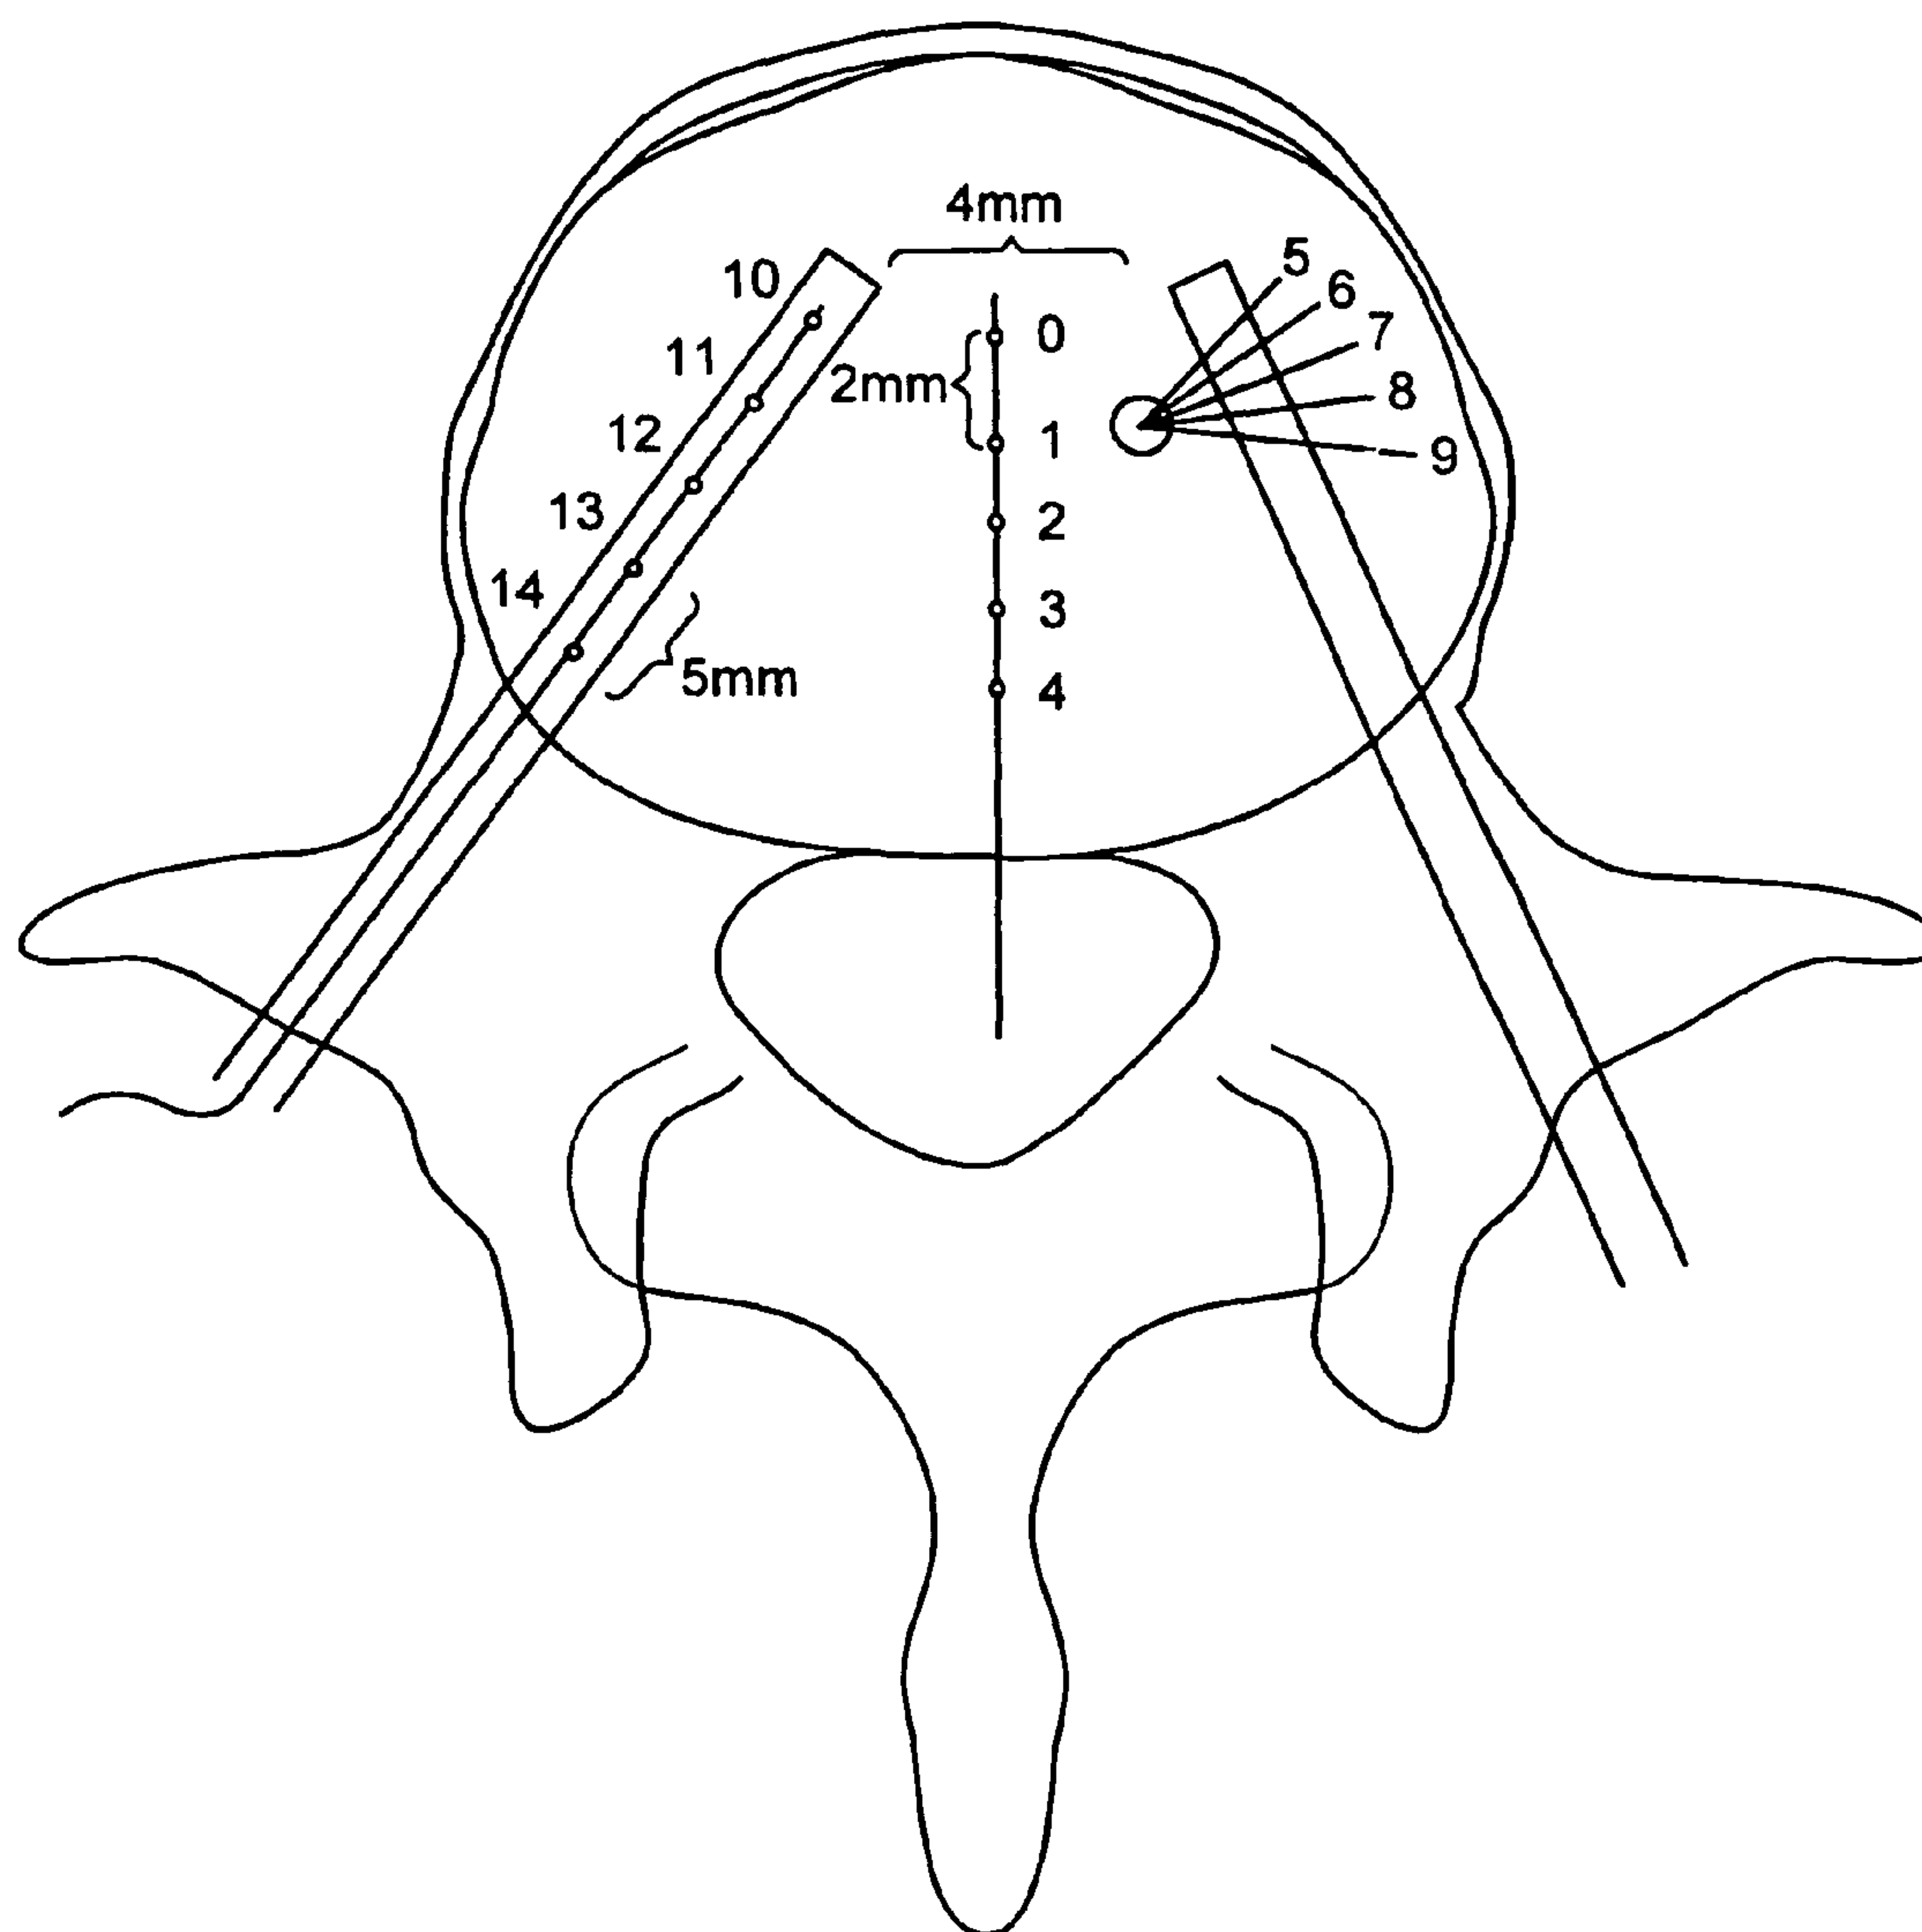


FIG. 28A

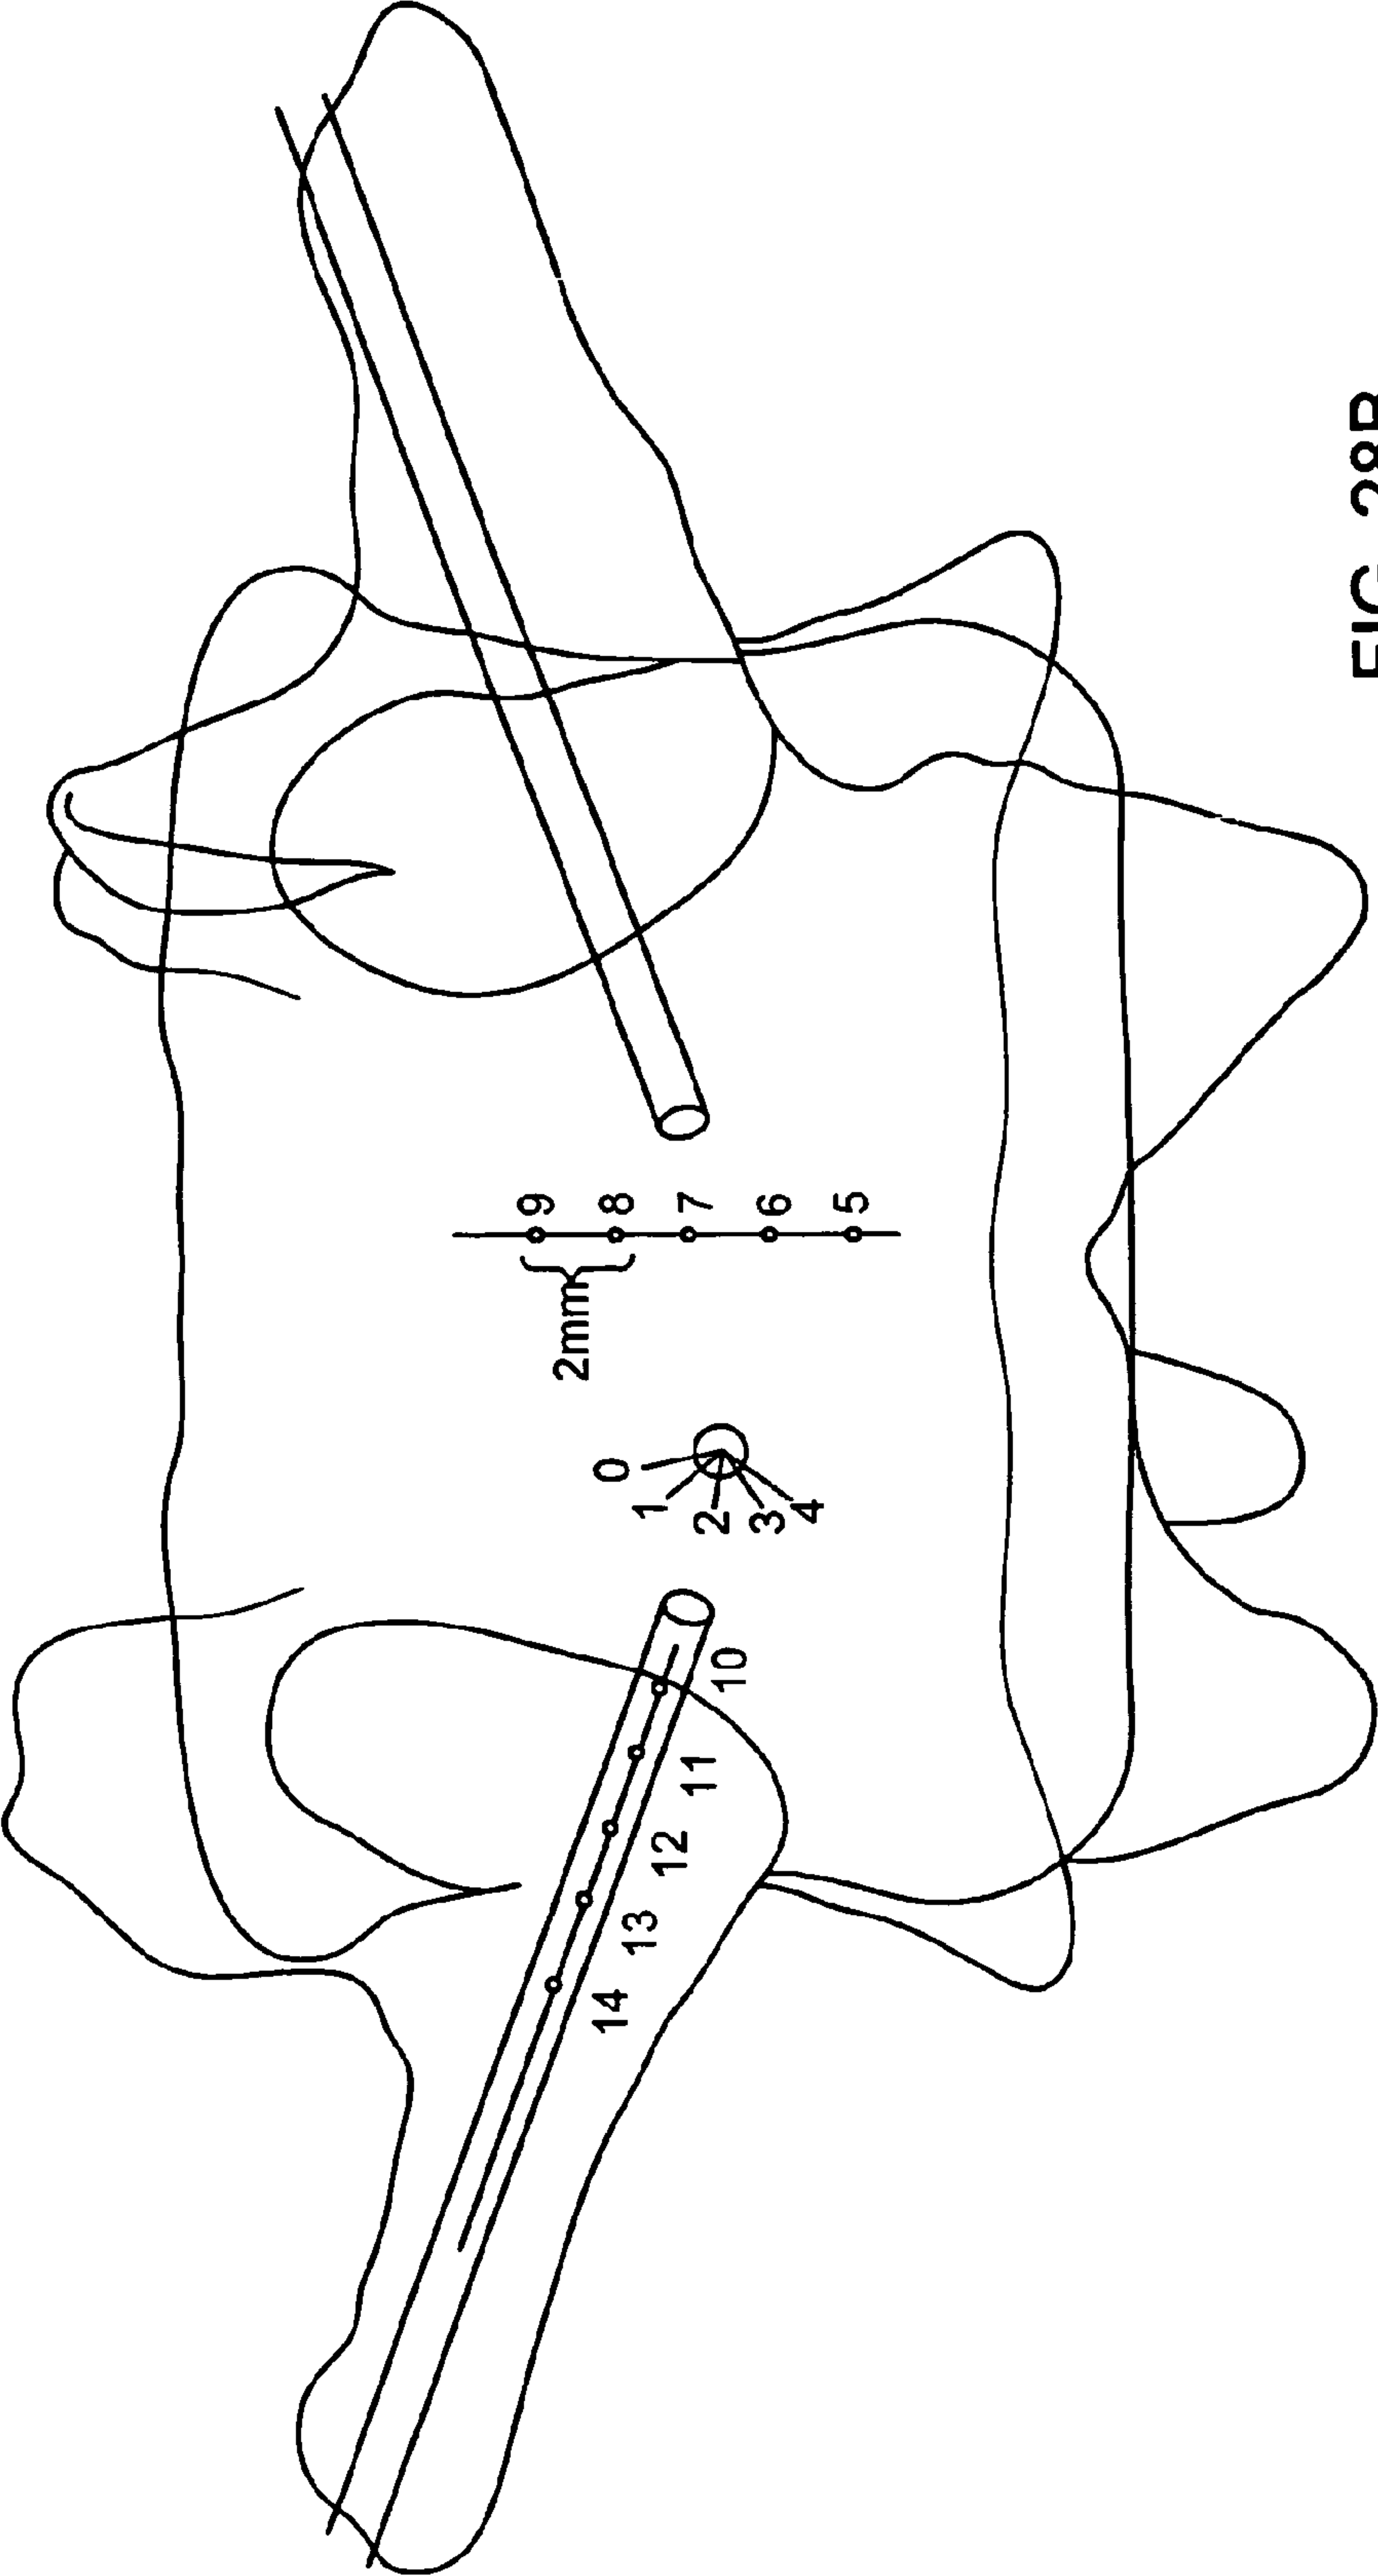


FIG. 28B

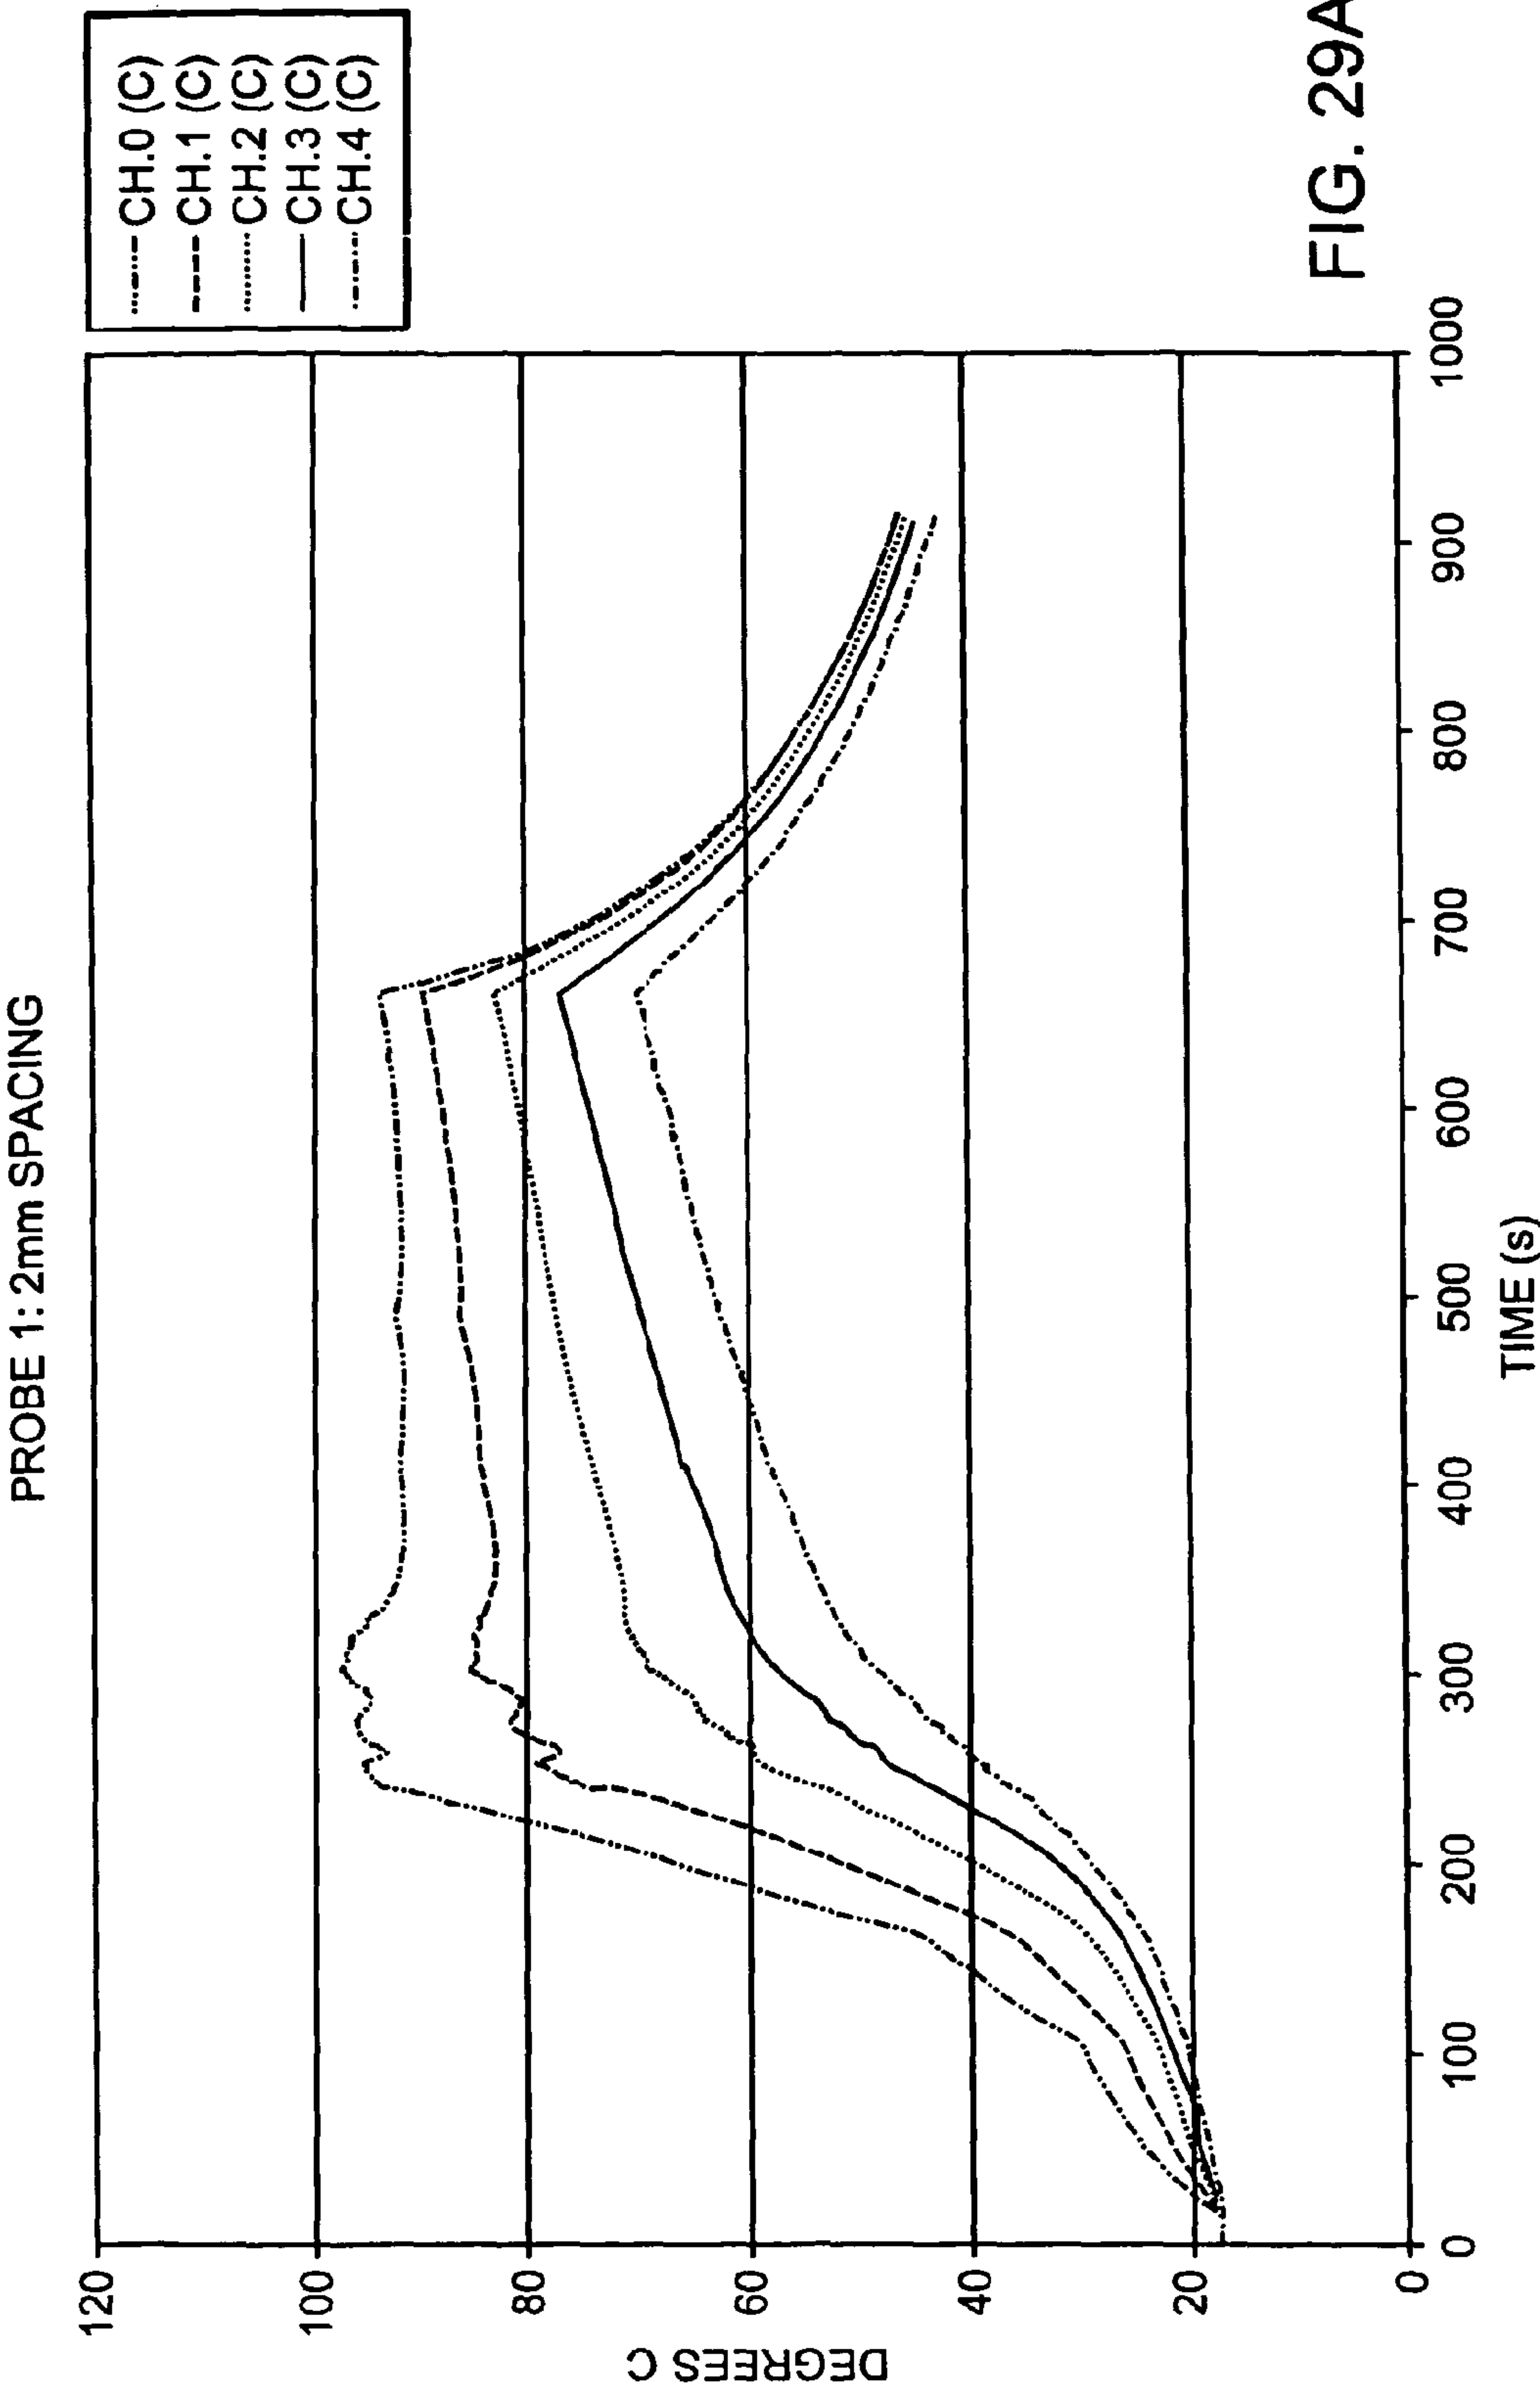


FIG. 29A

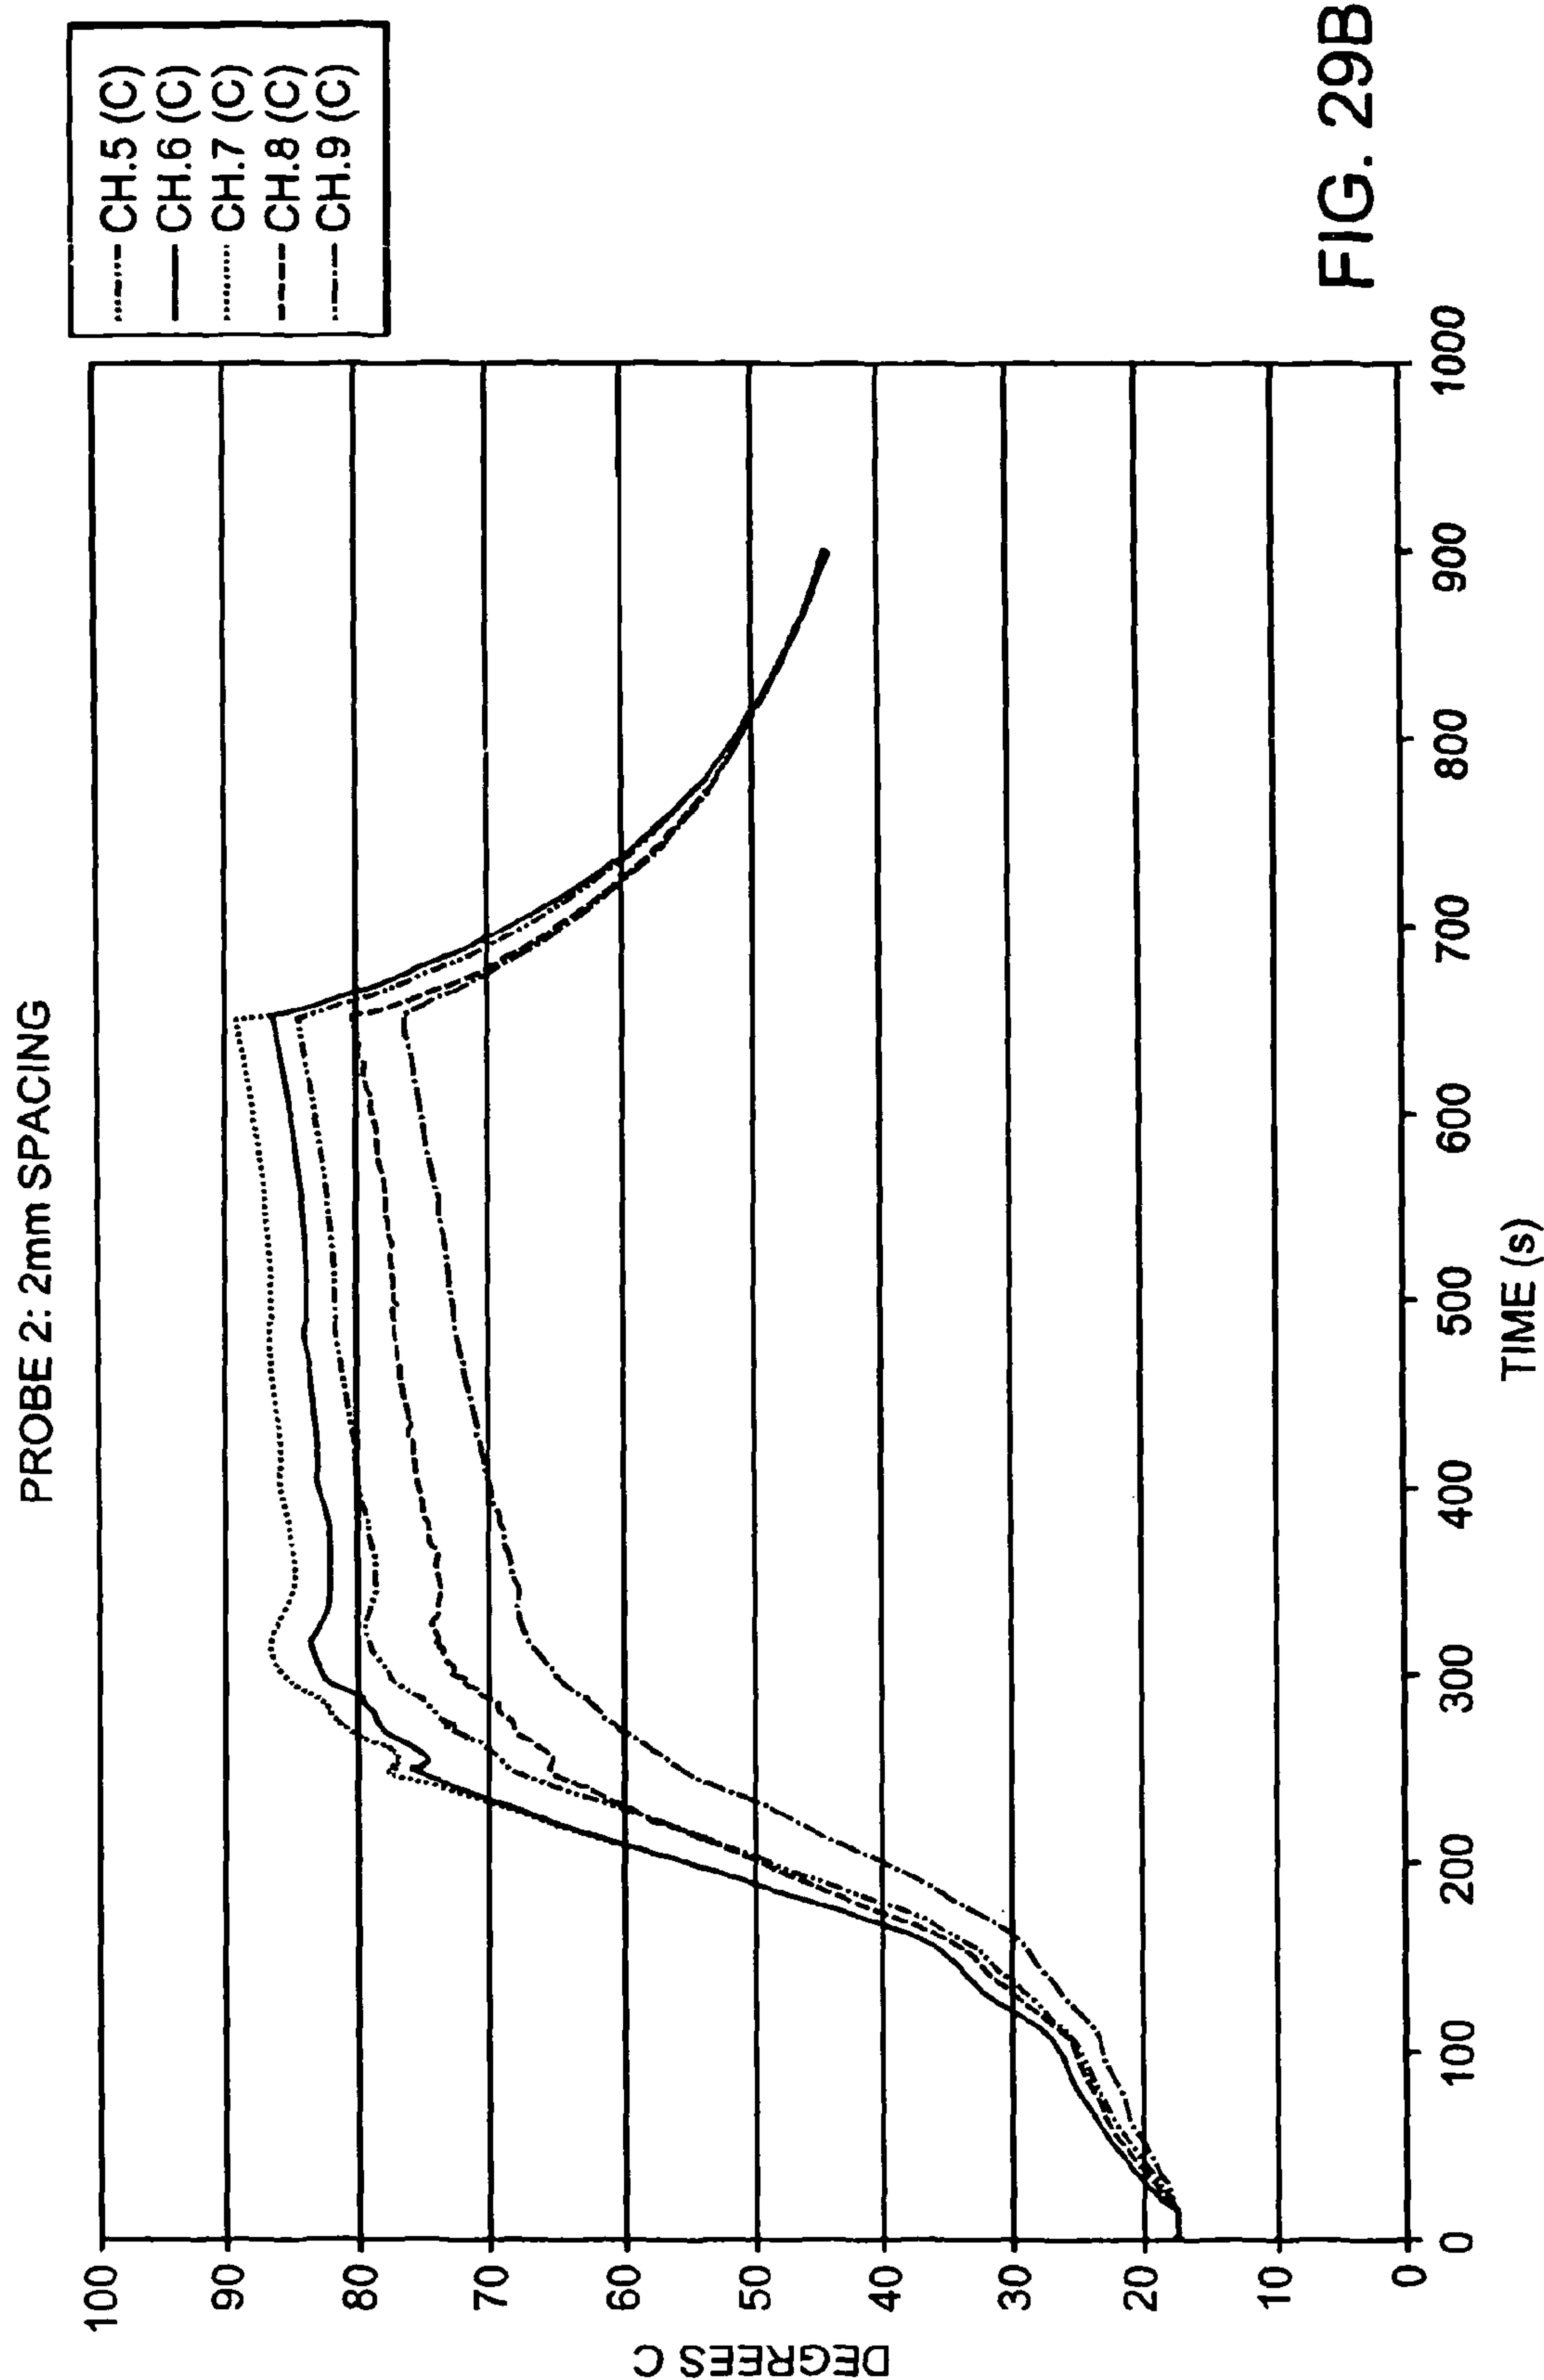


FIG. 29B

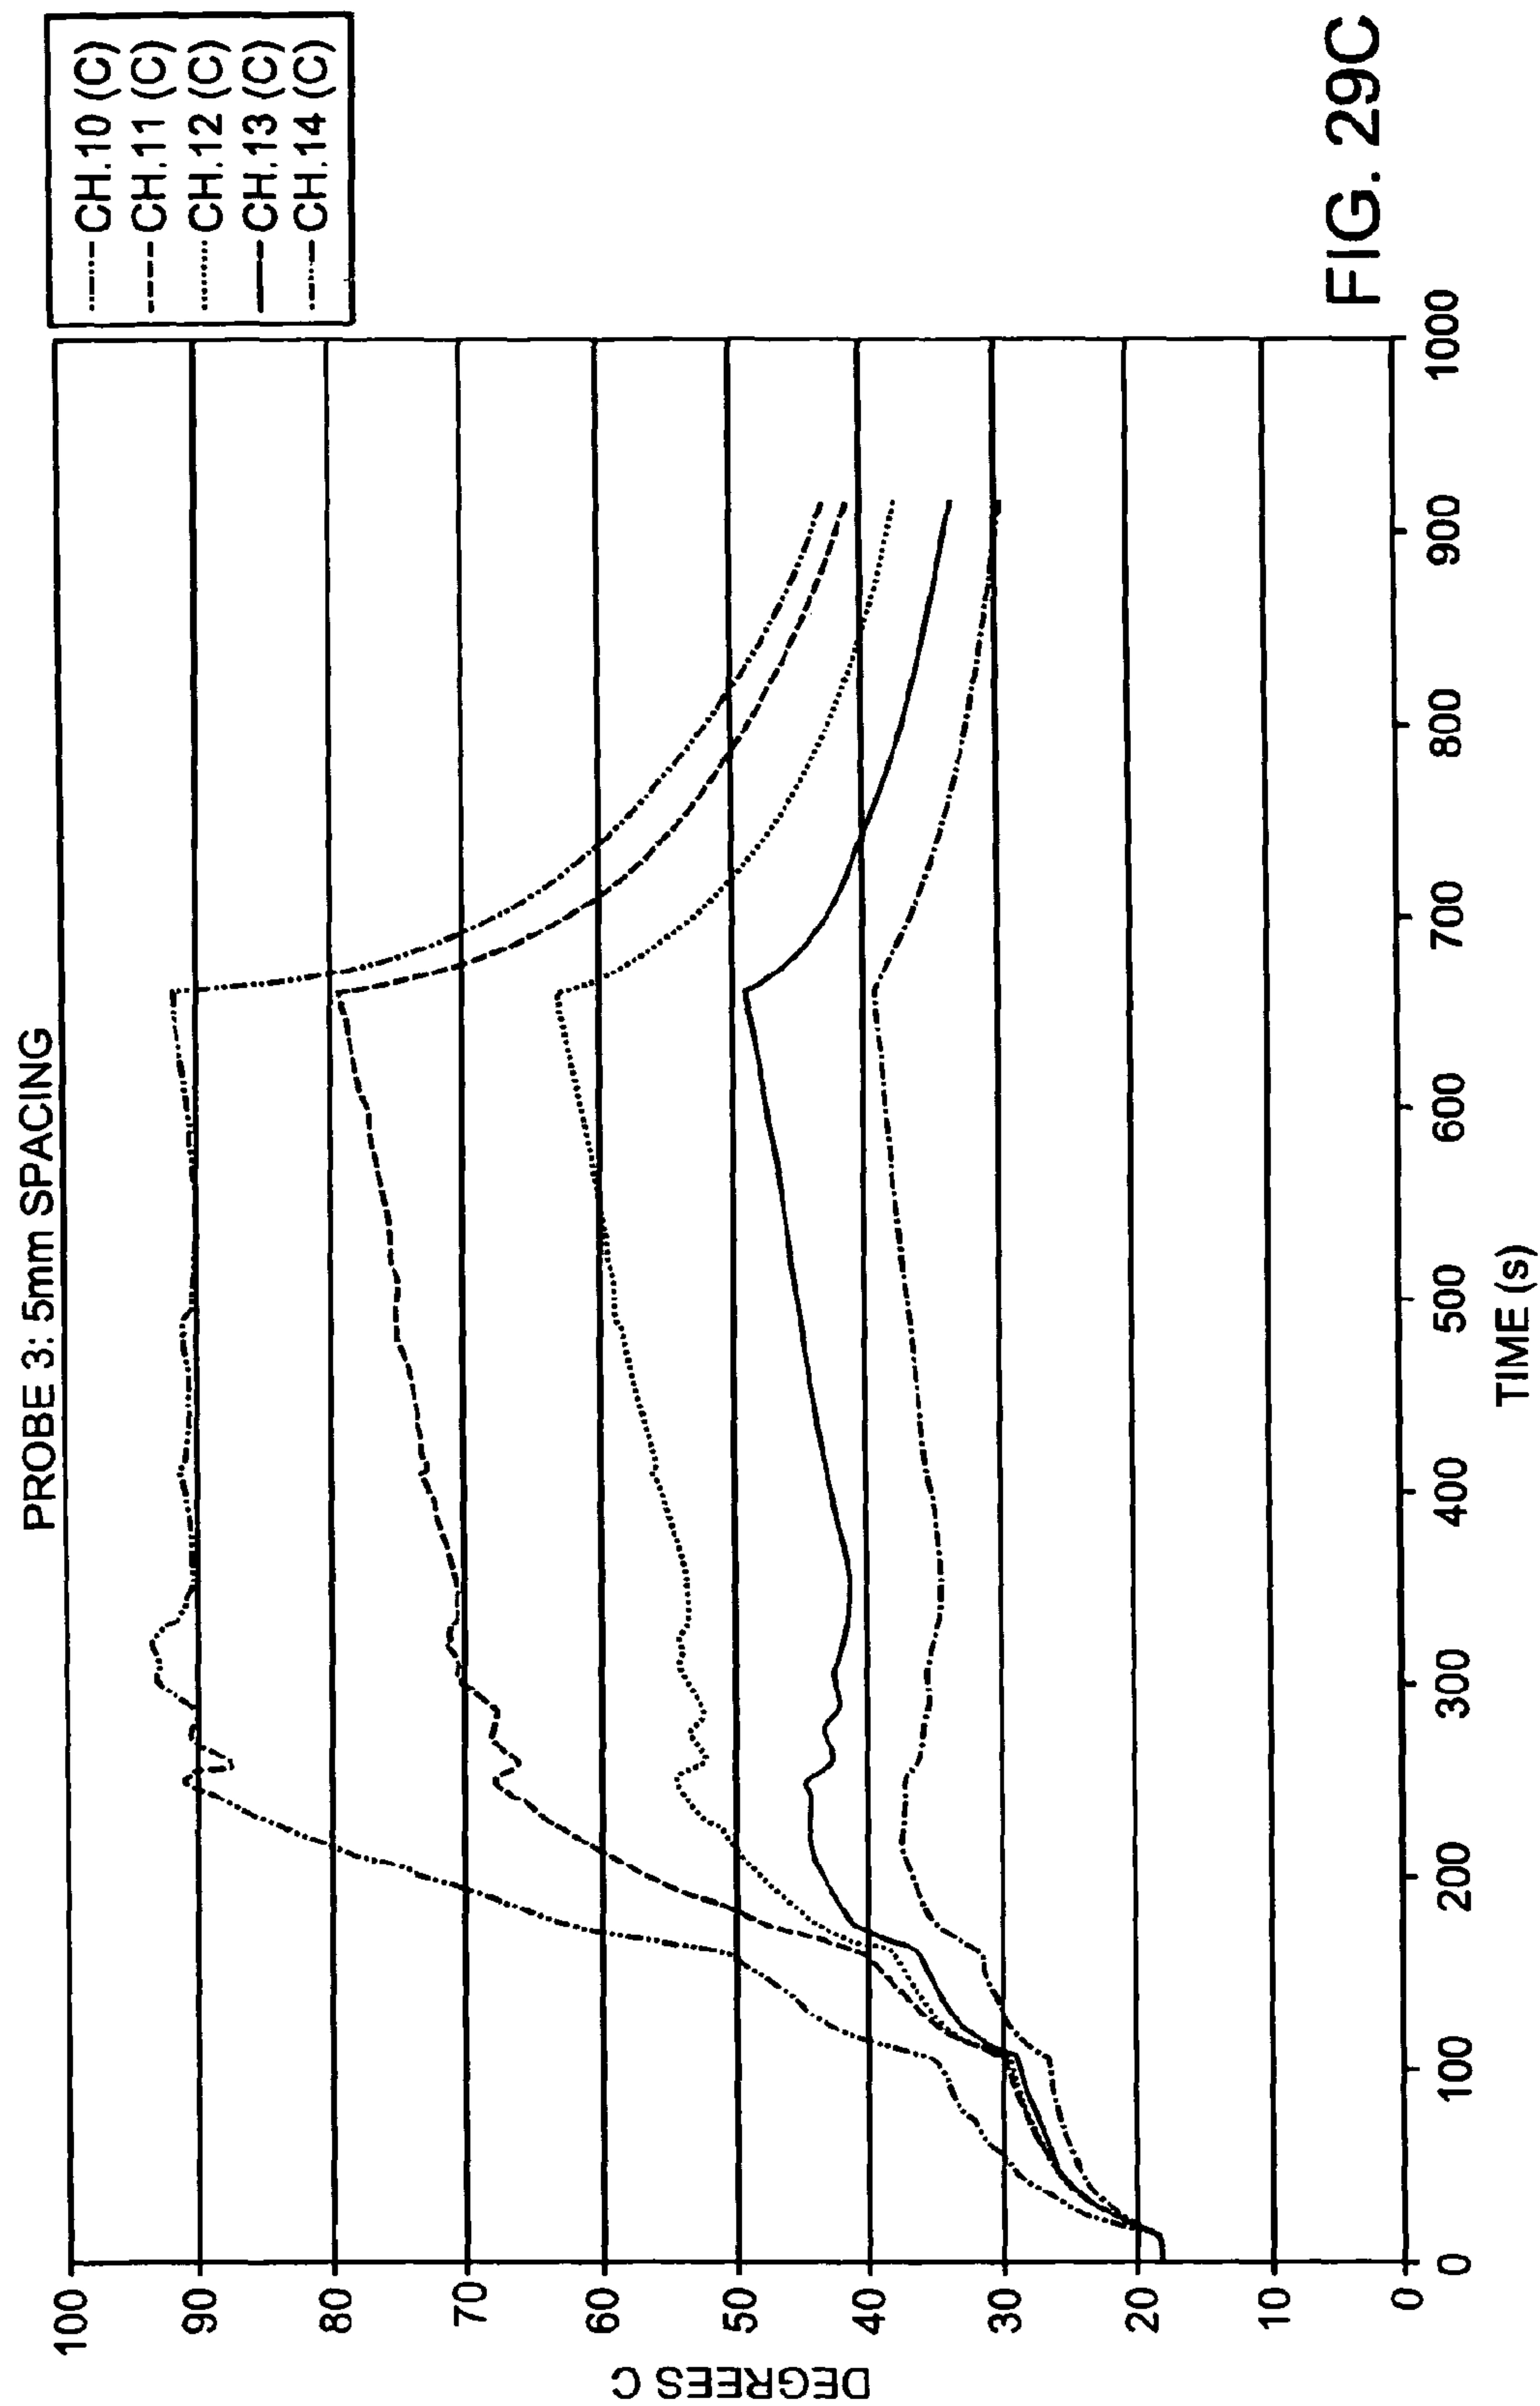


FIG. 29C

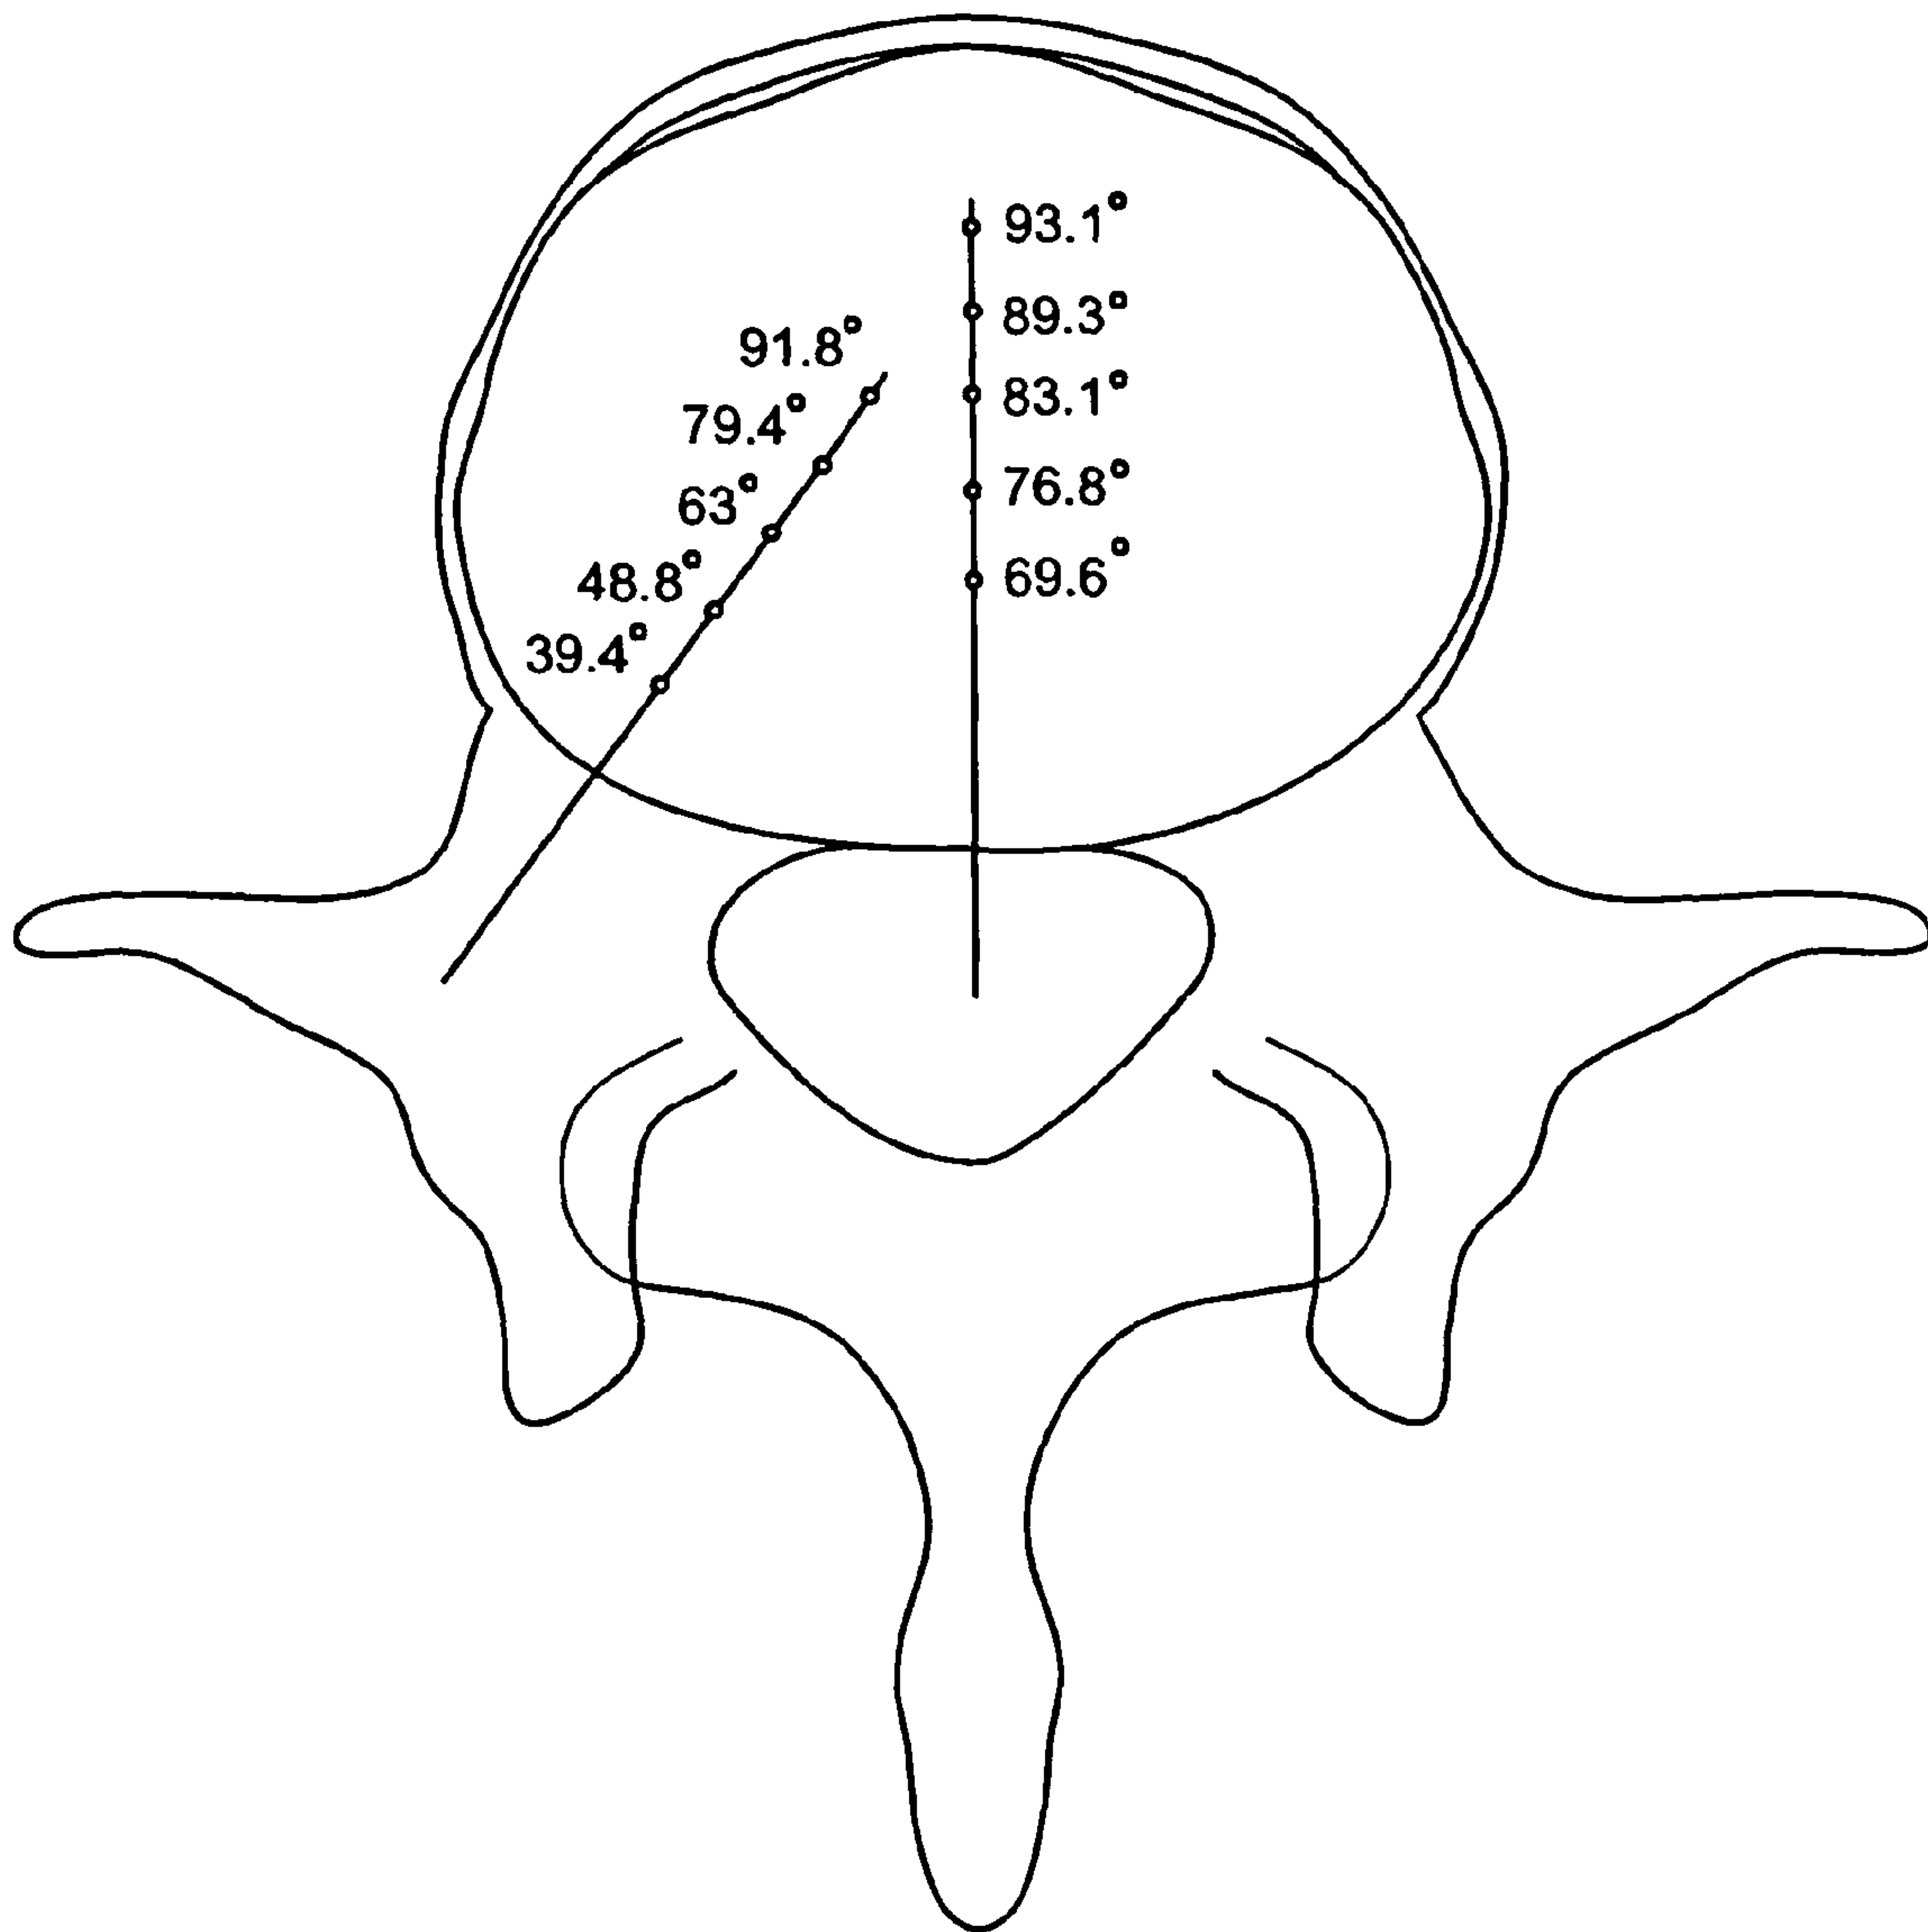


FIG. 30A

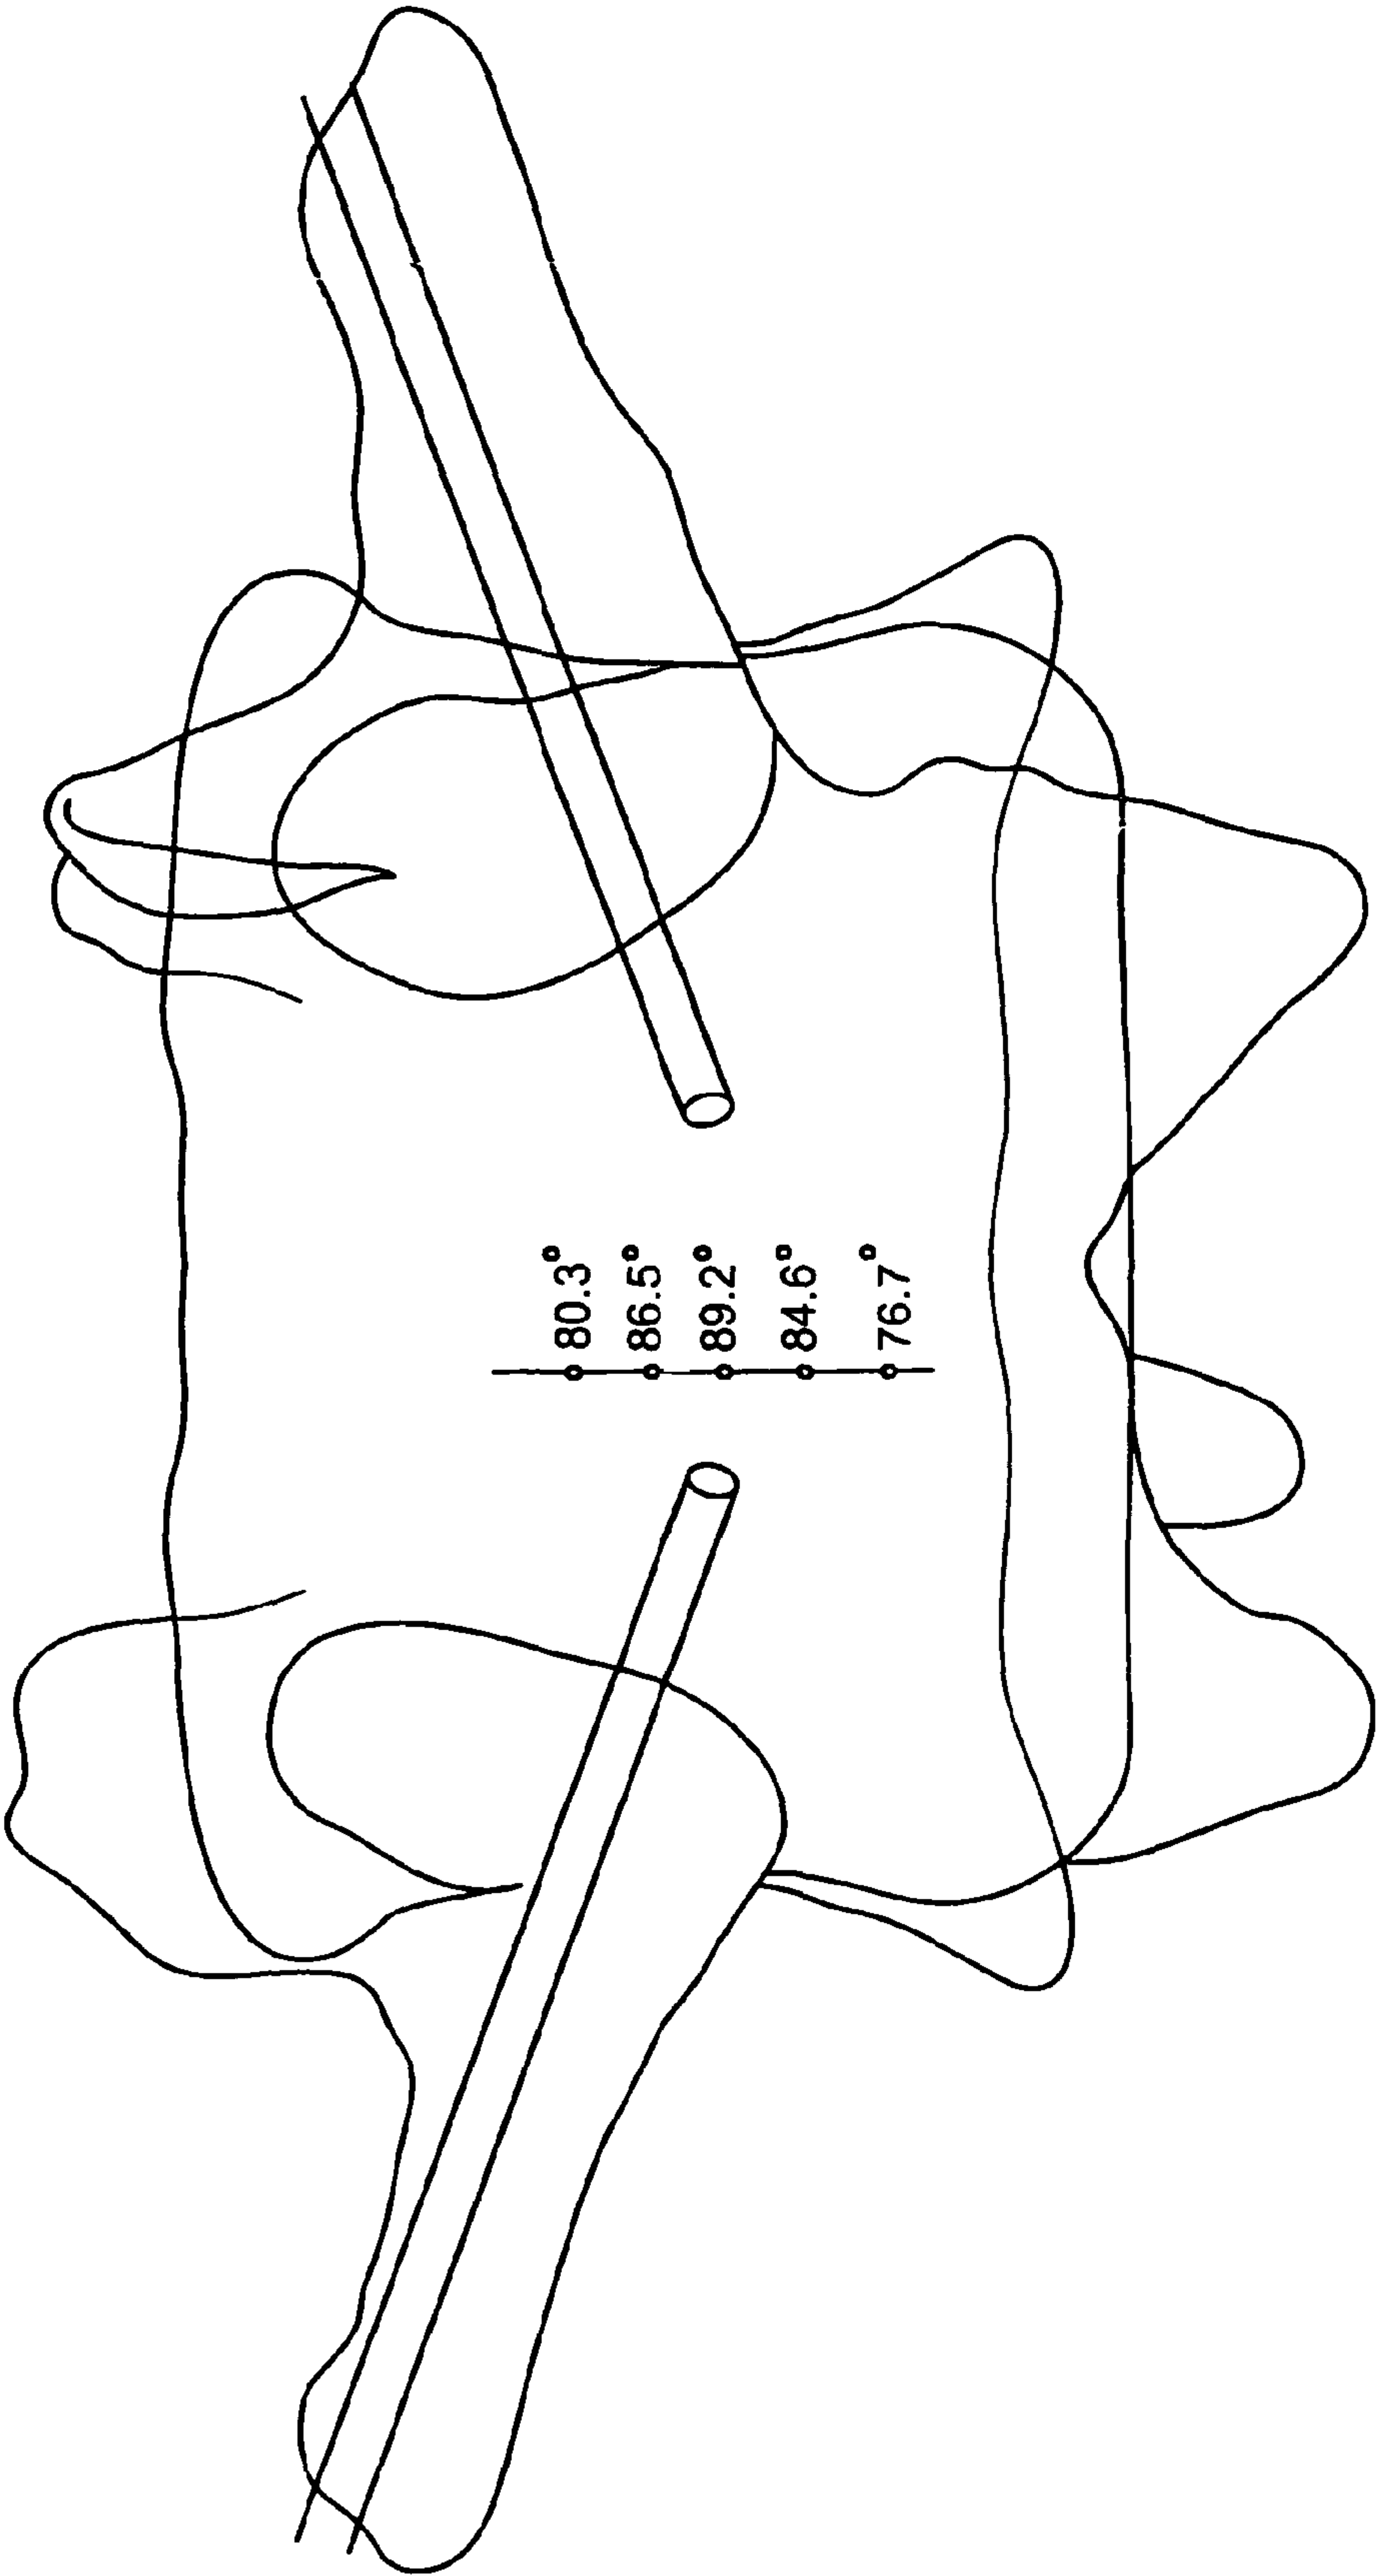


FIG. 30B

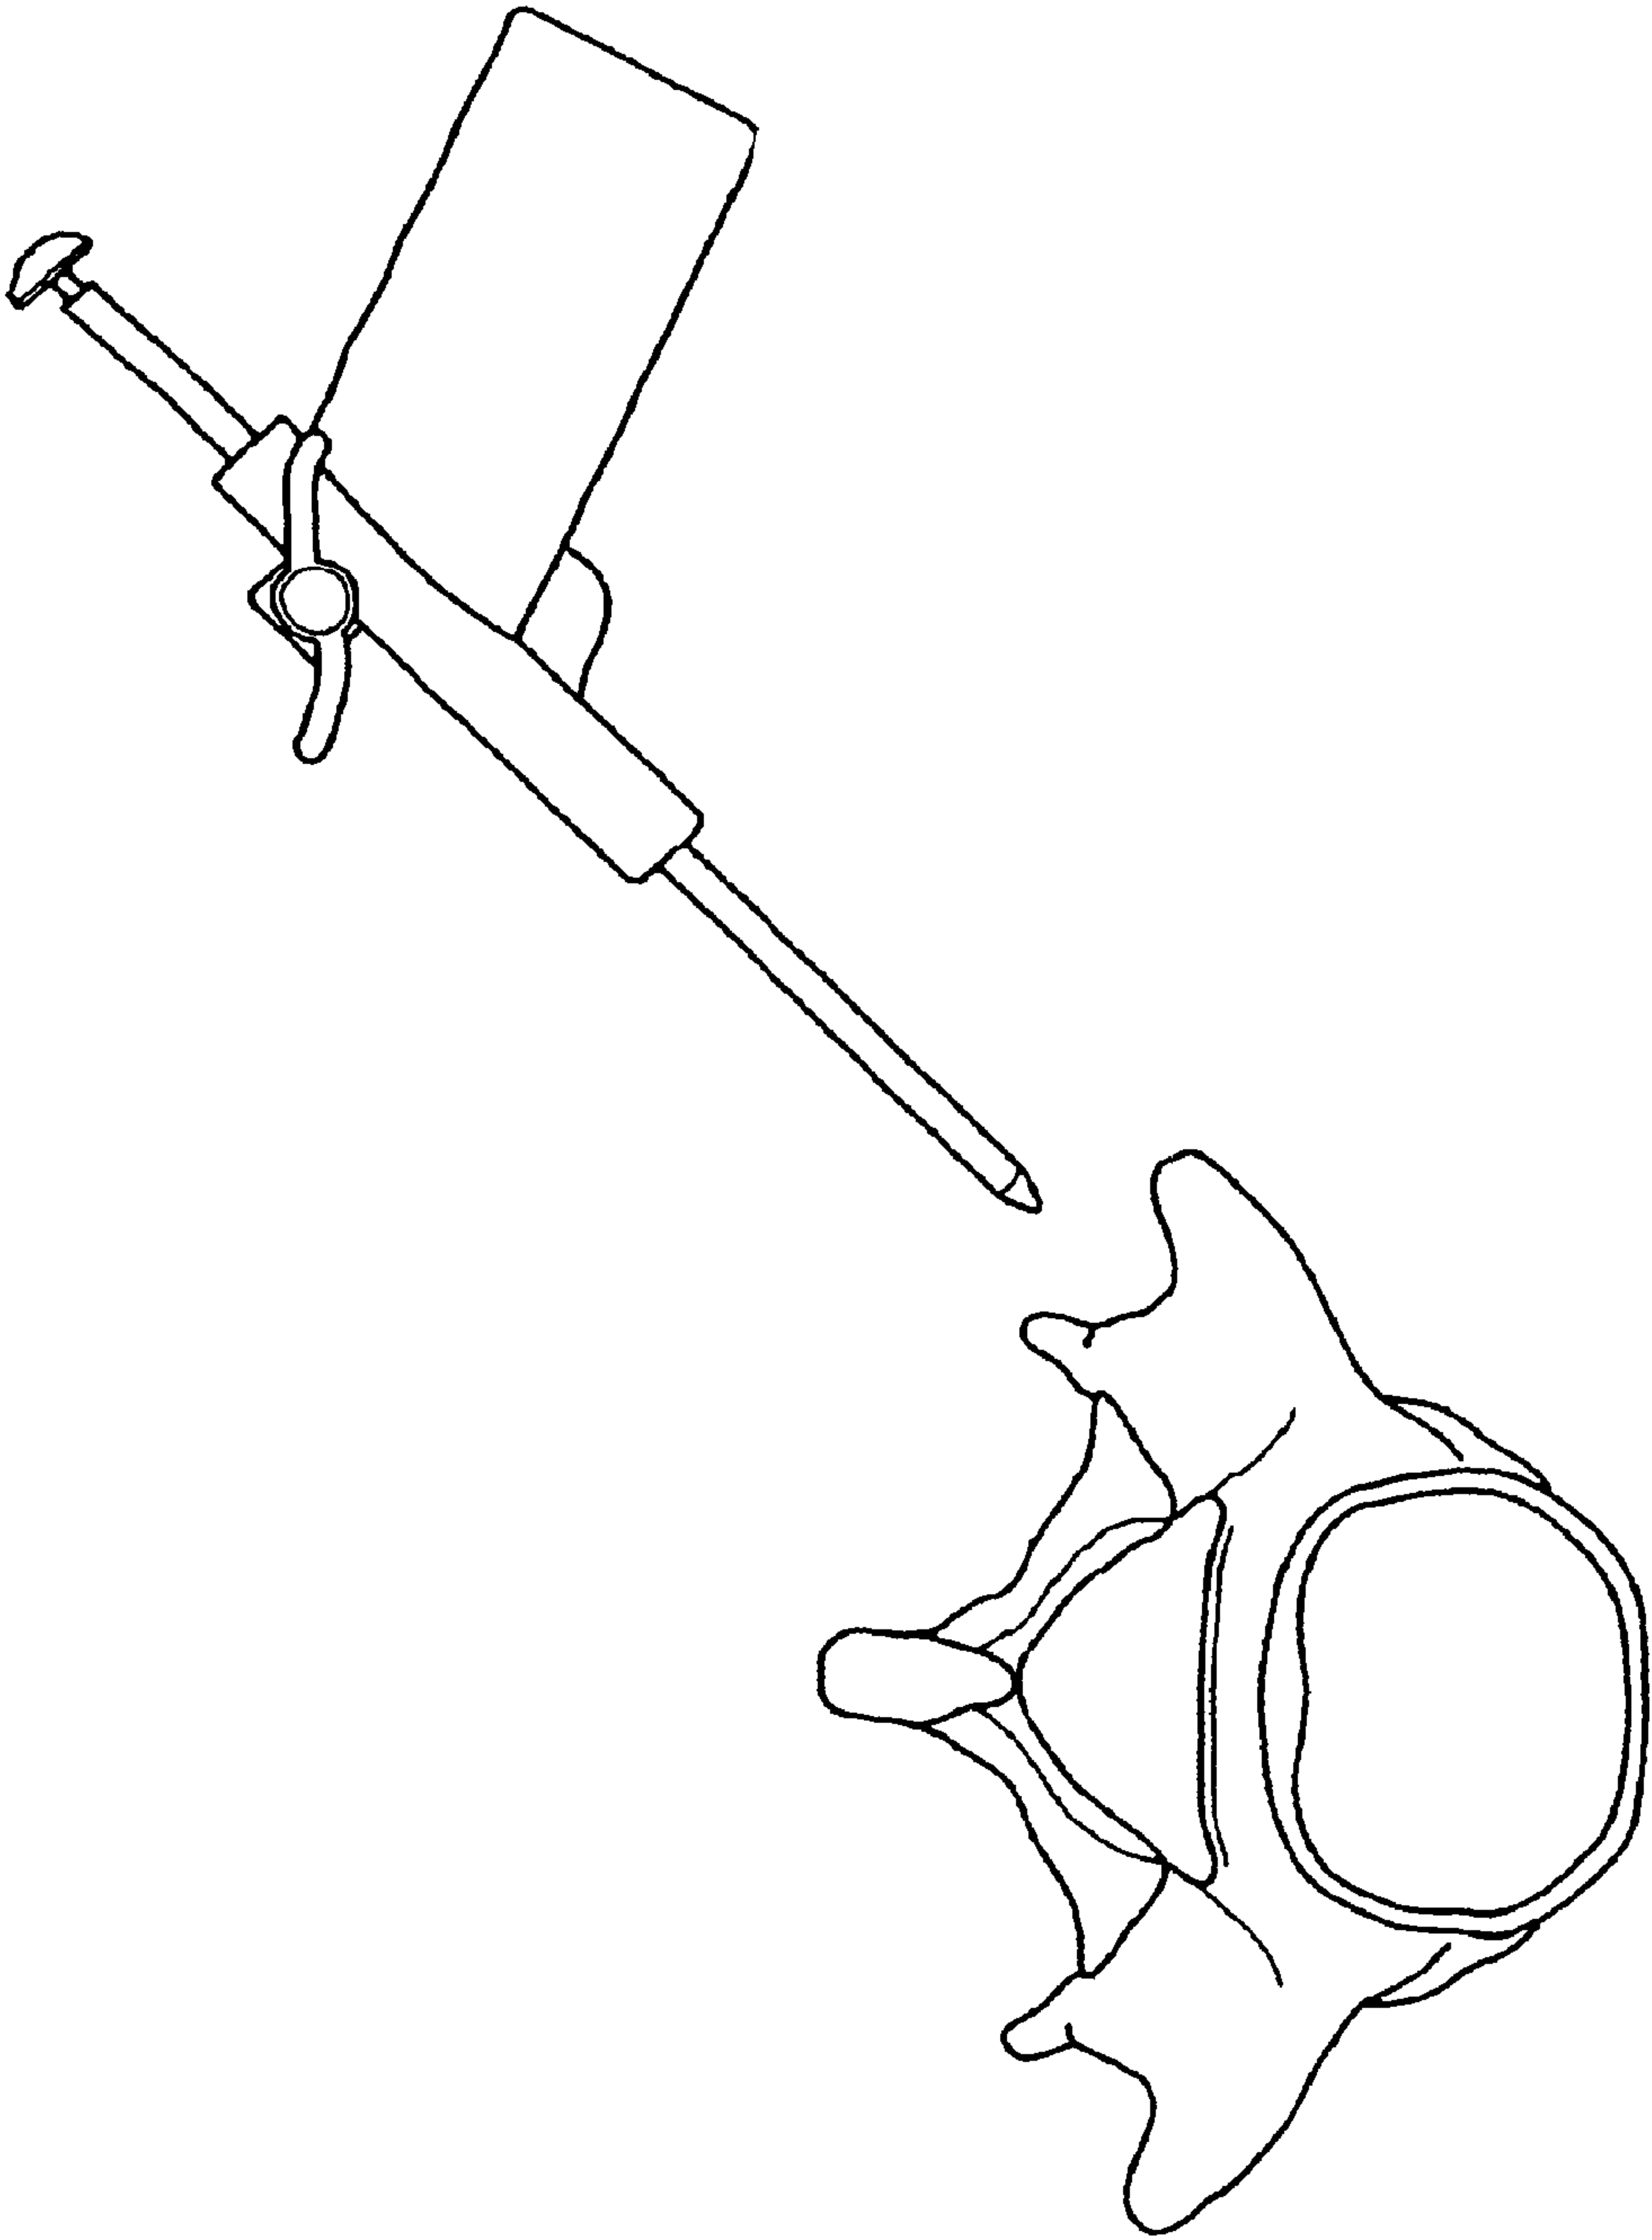


FIG. 31A

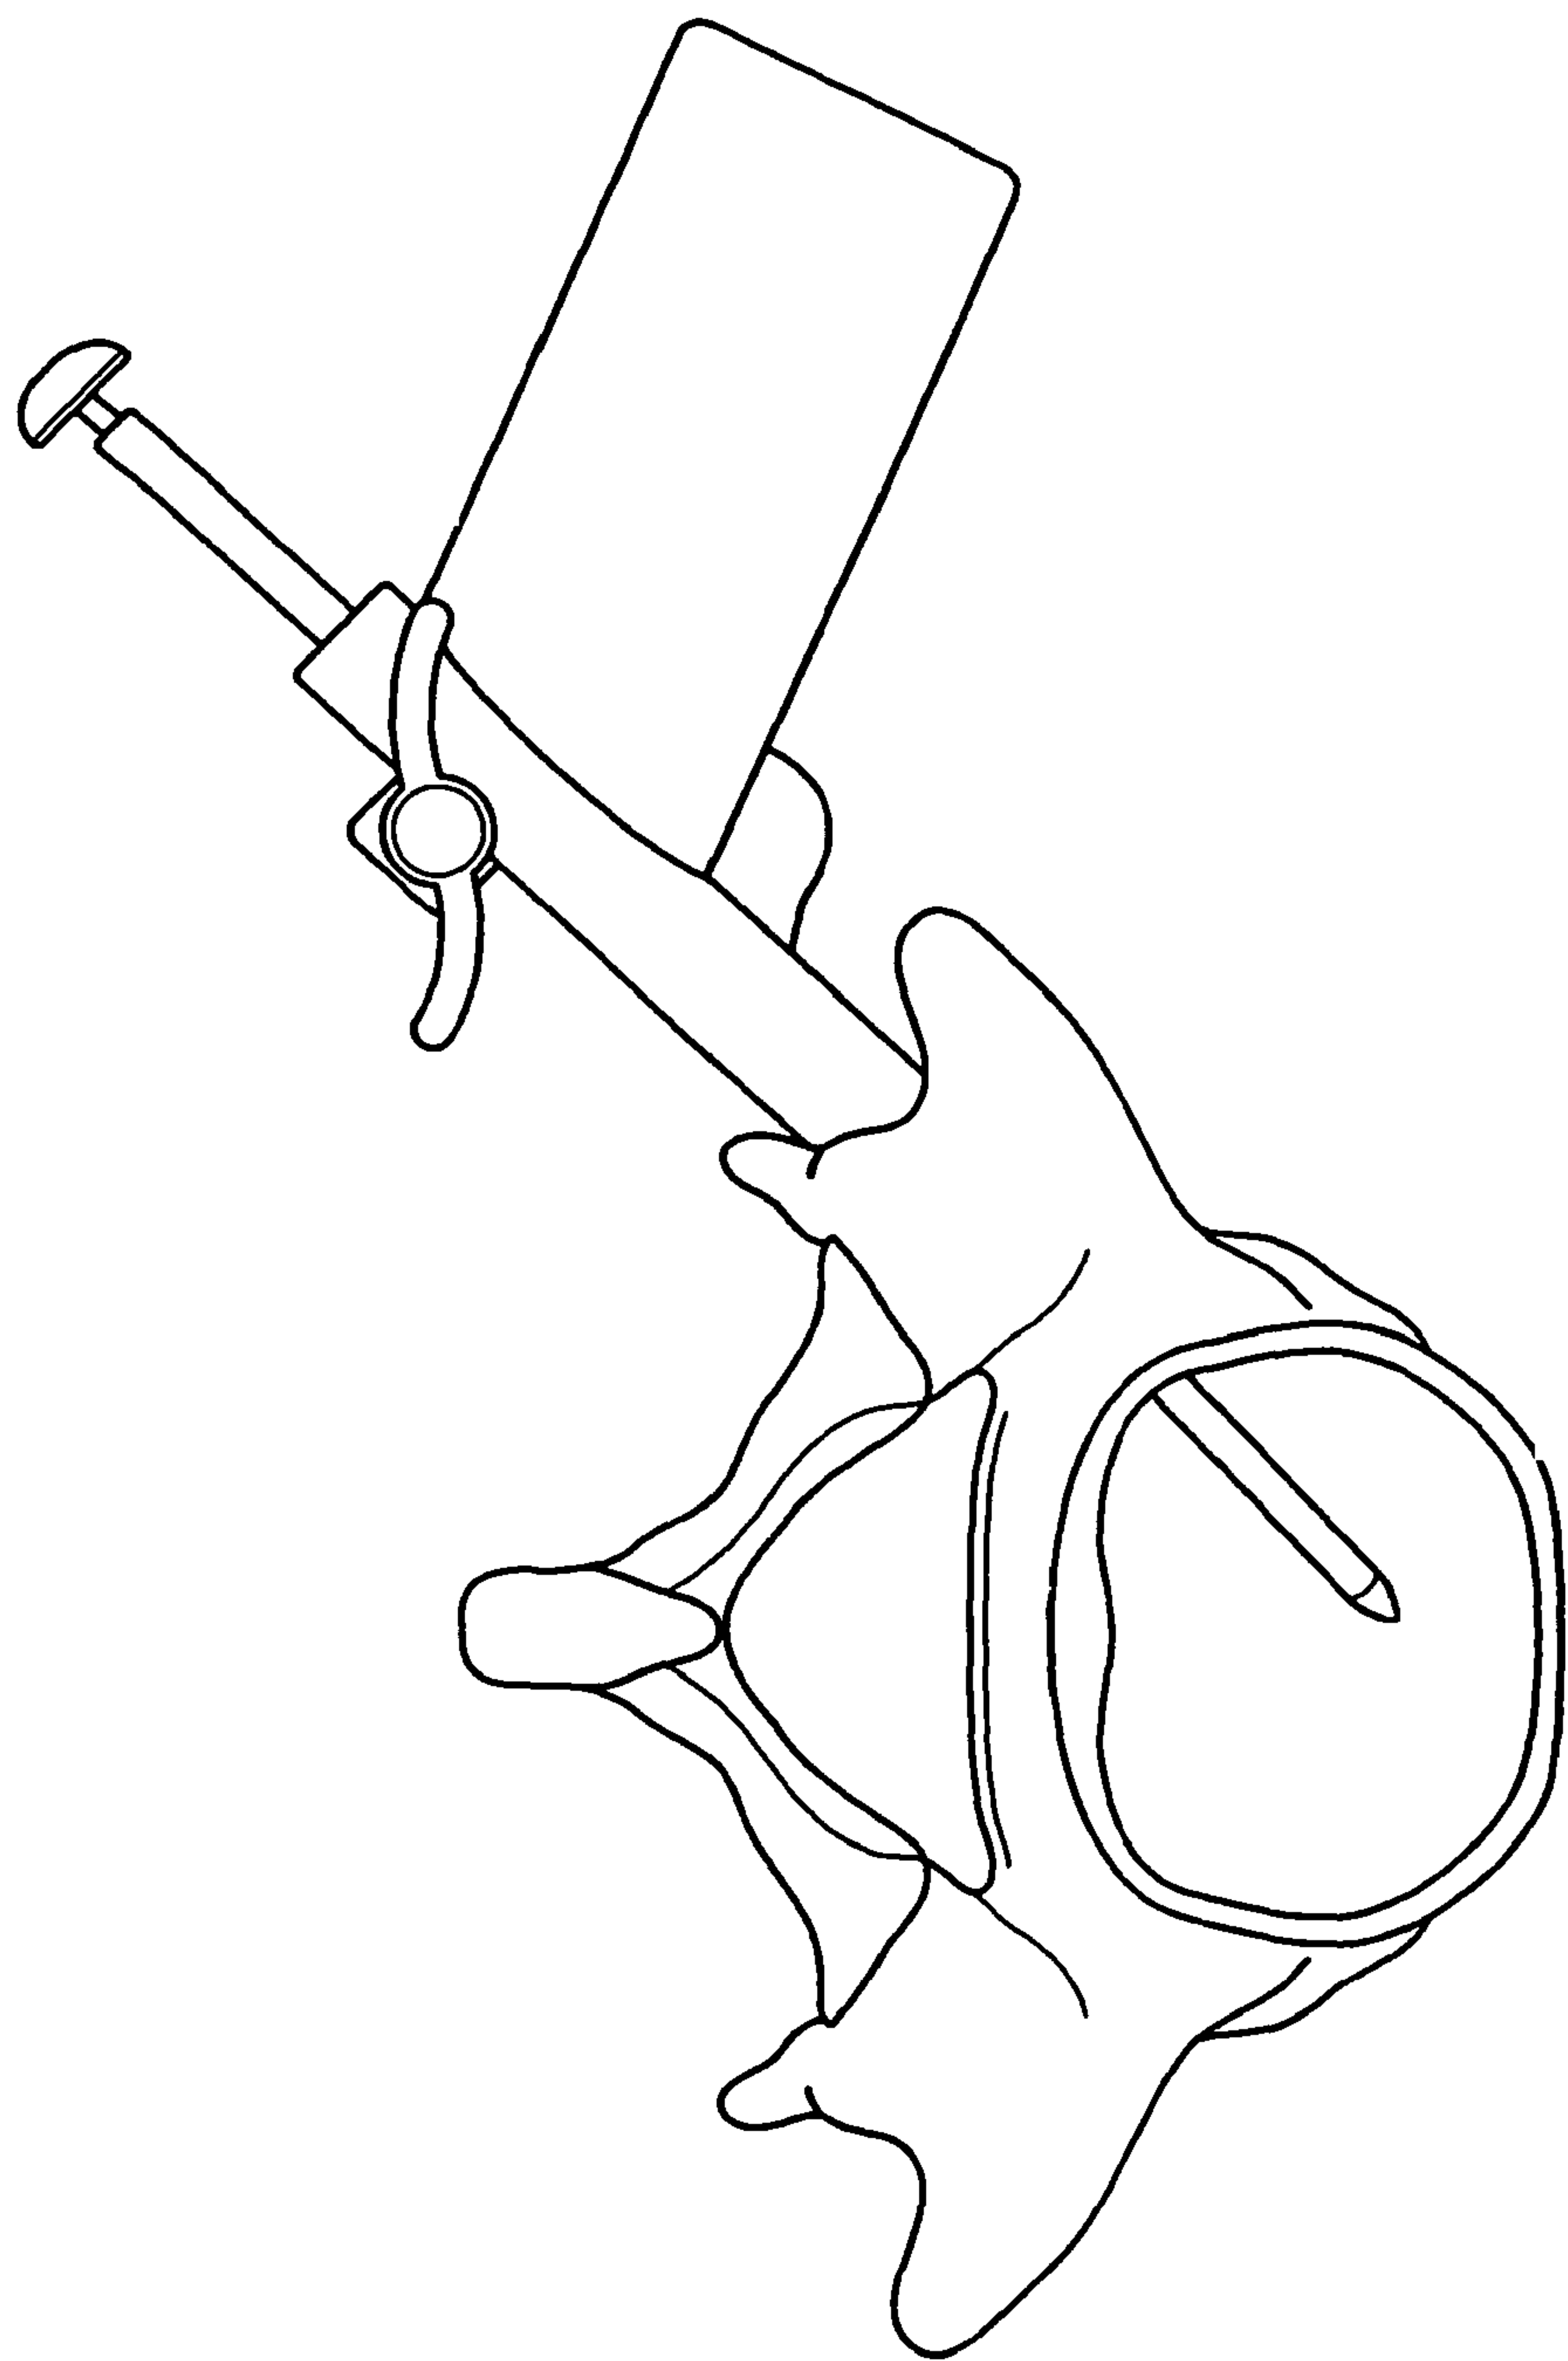


FIG. 31B

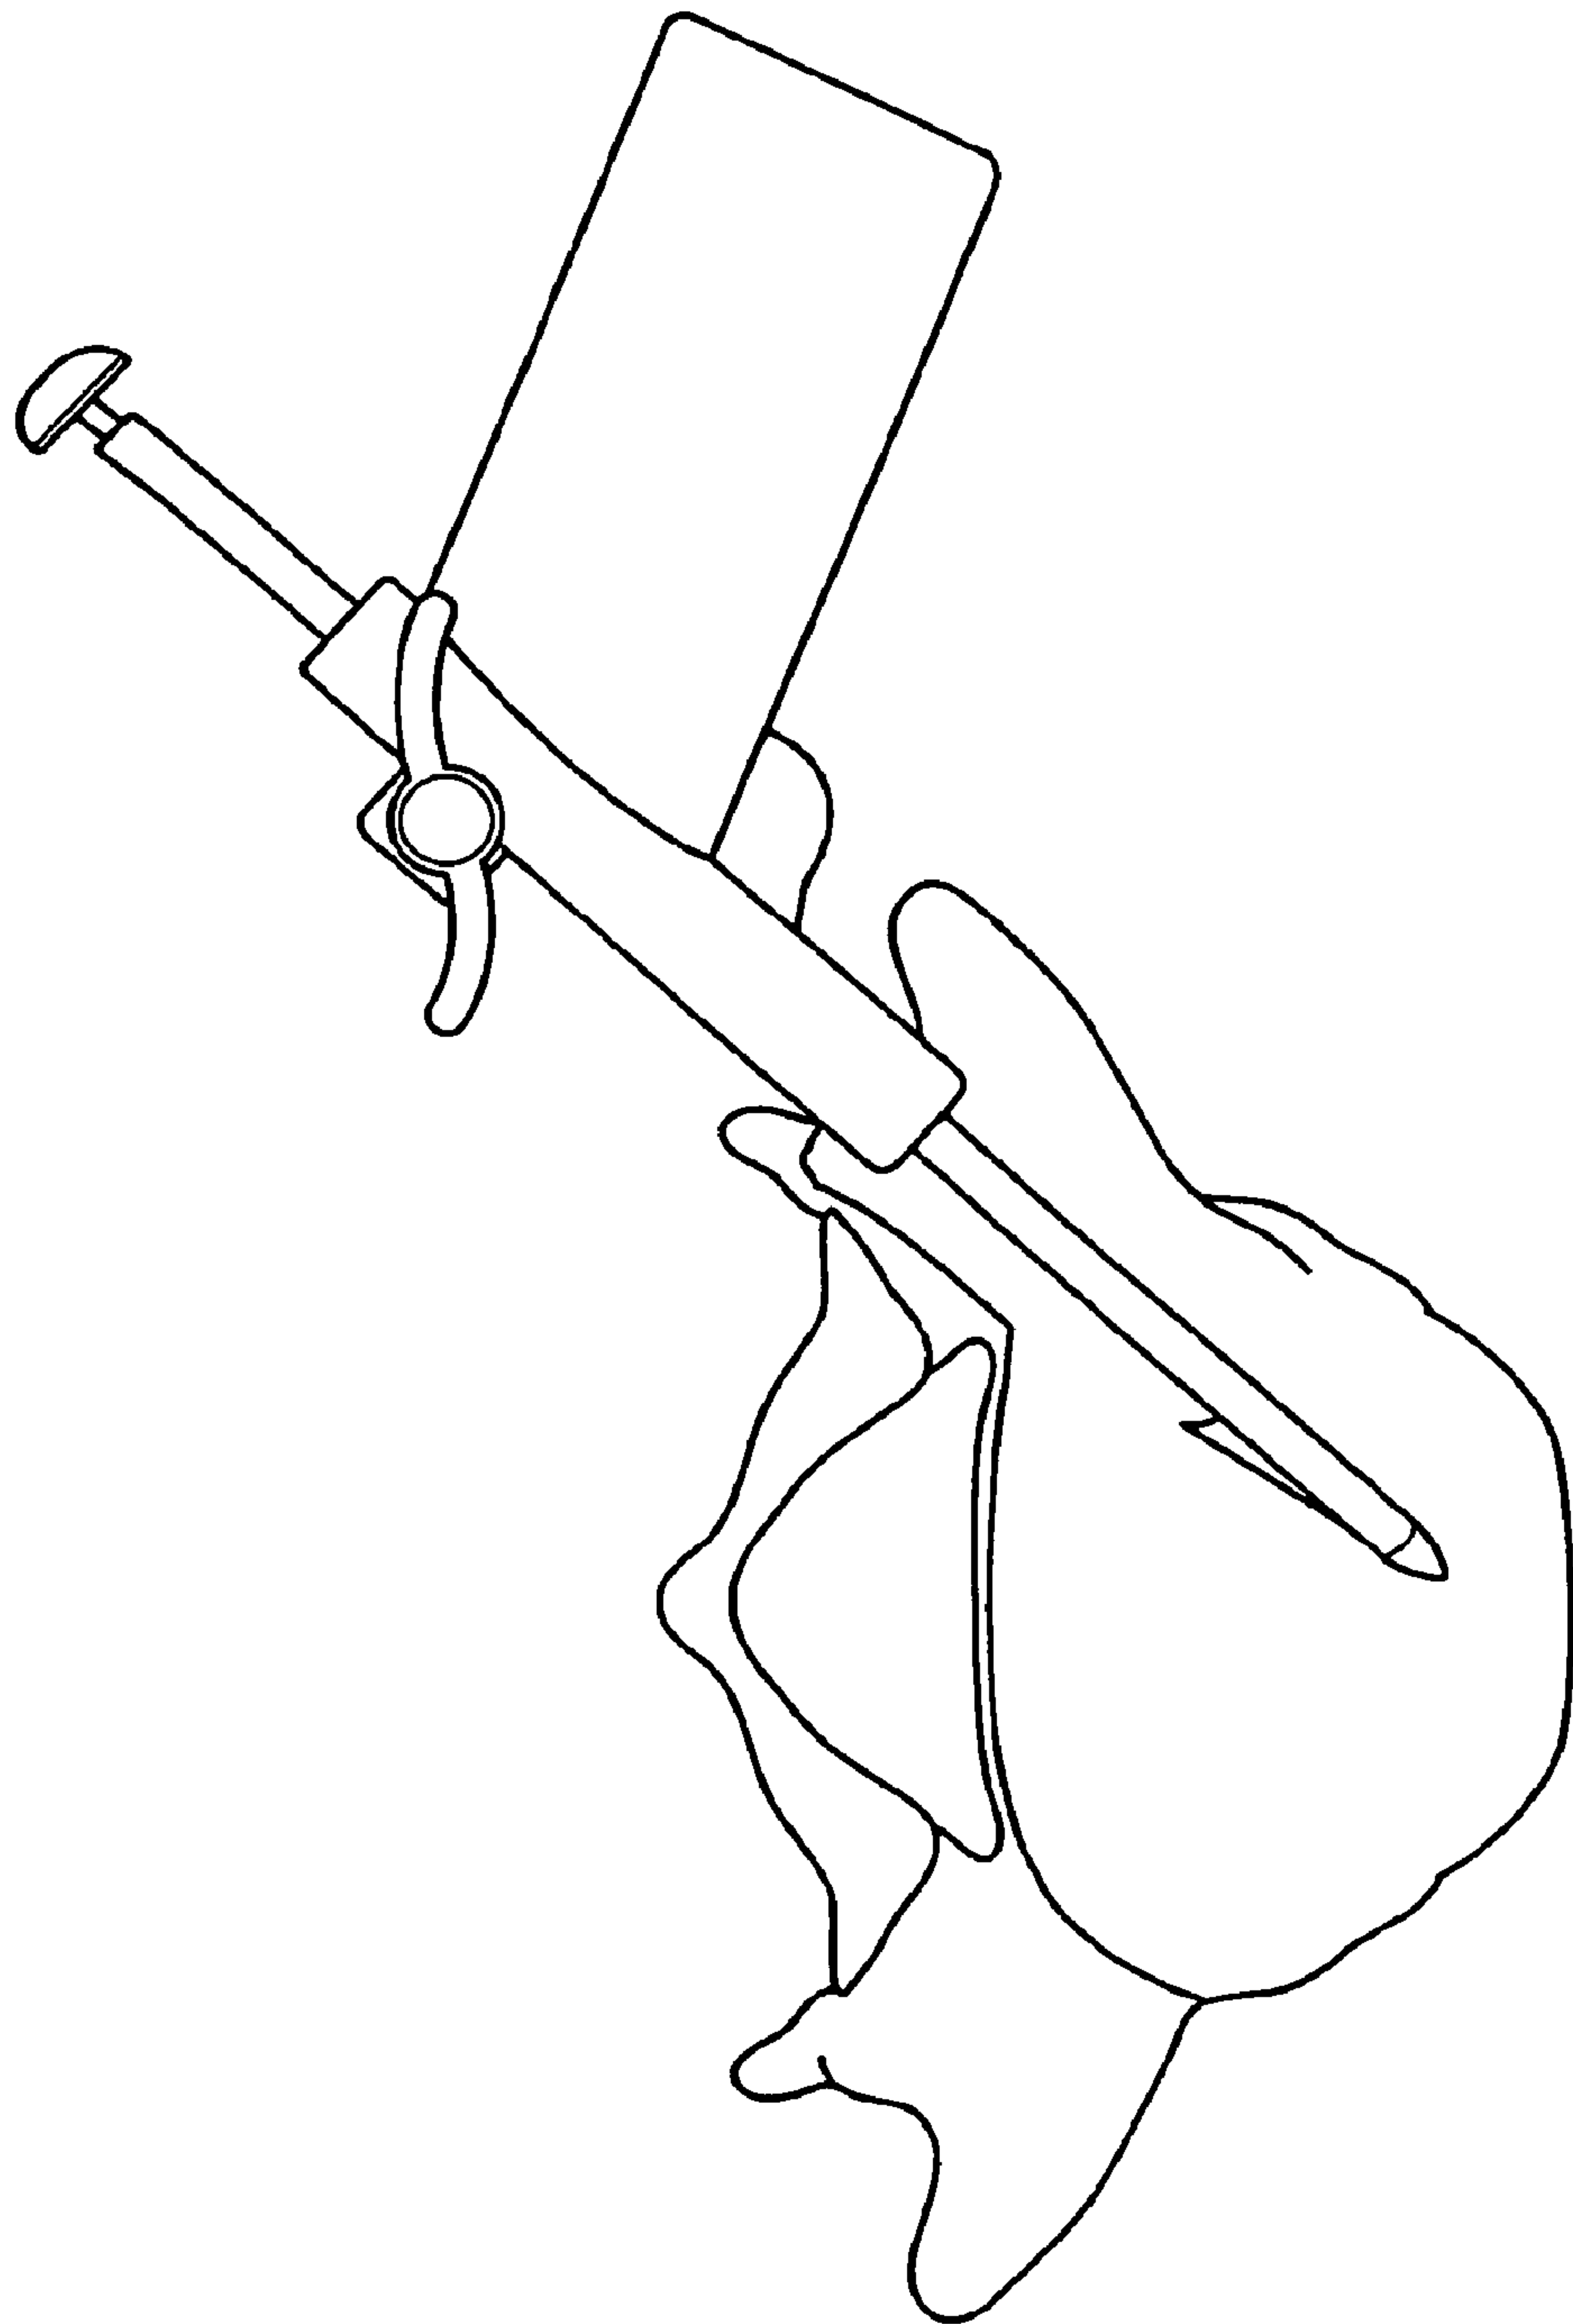


FIG. 31C

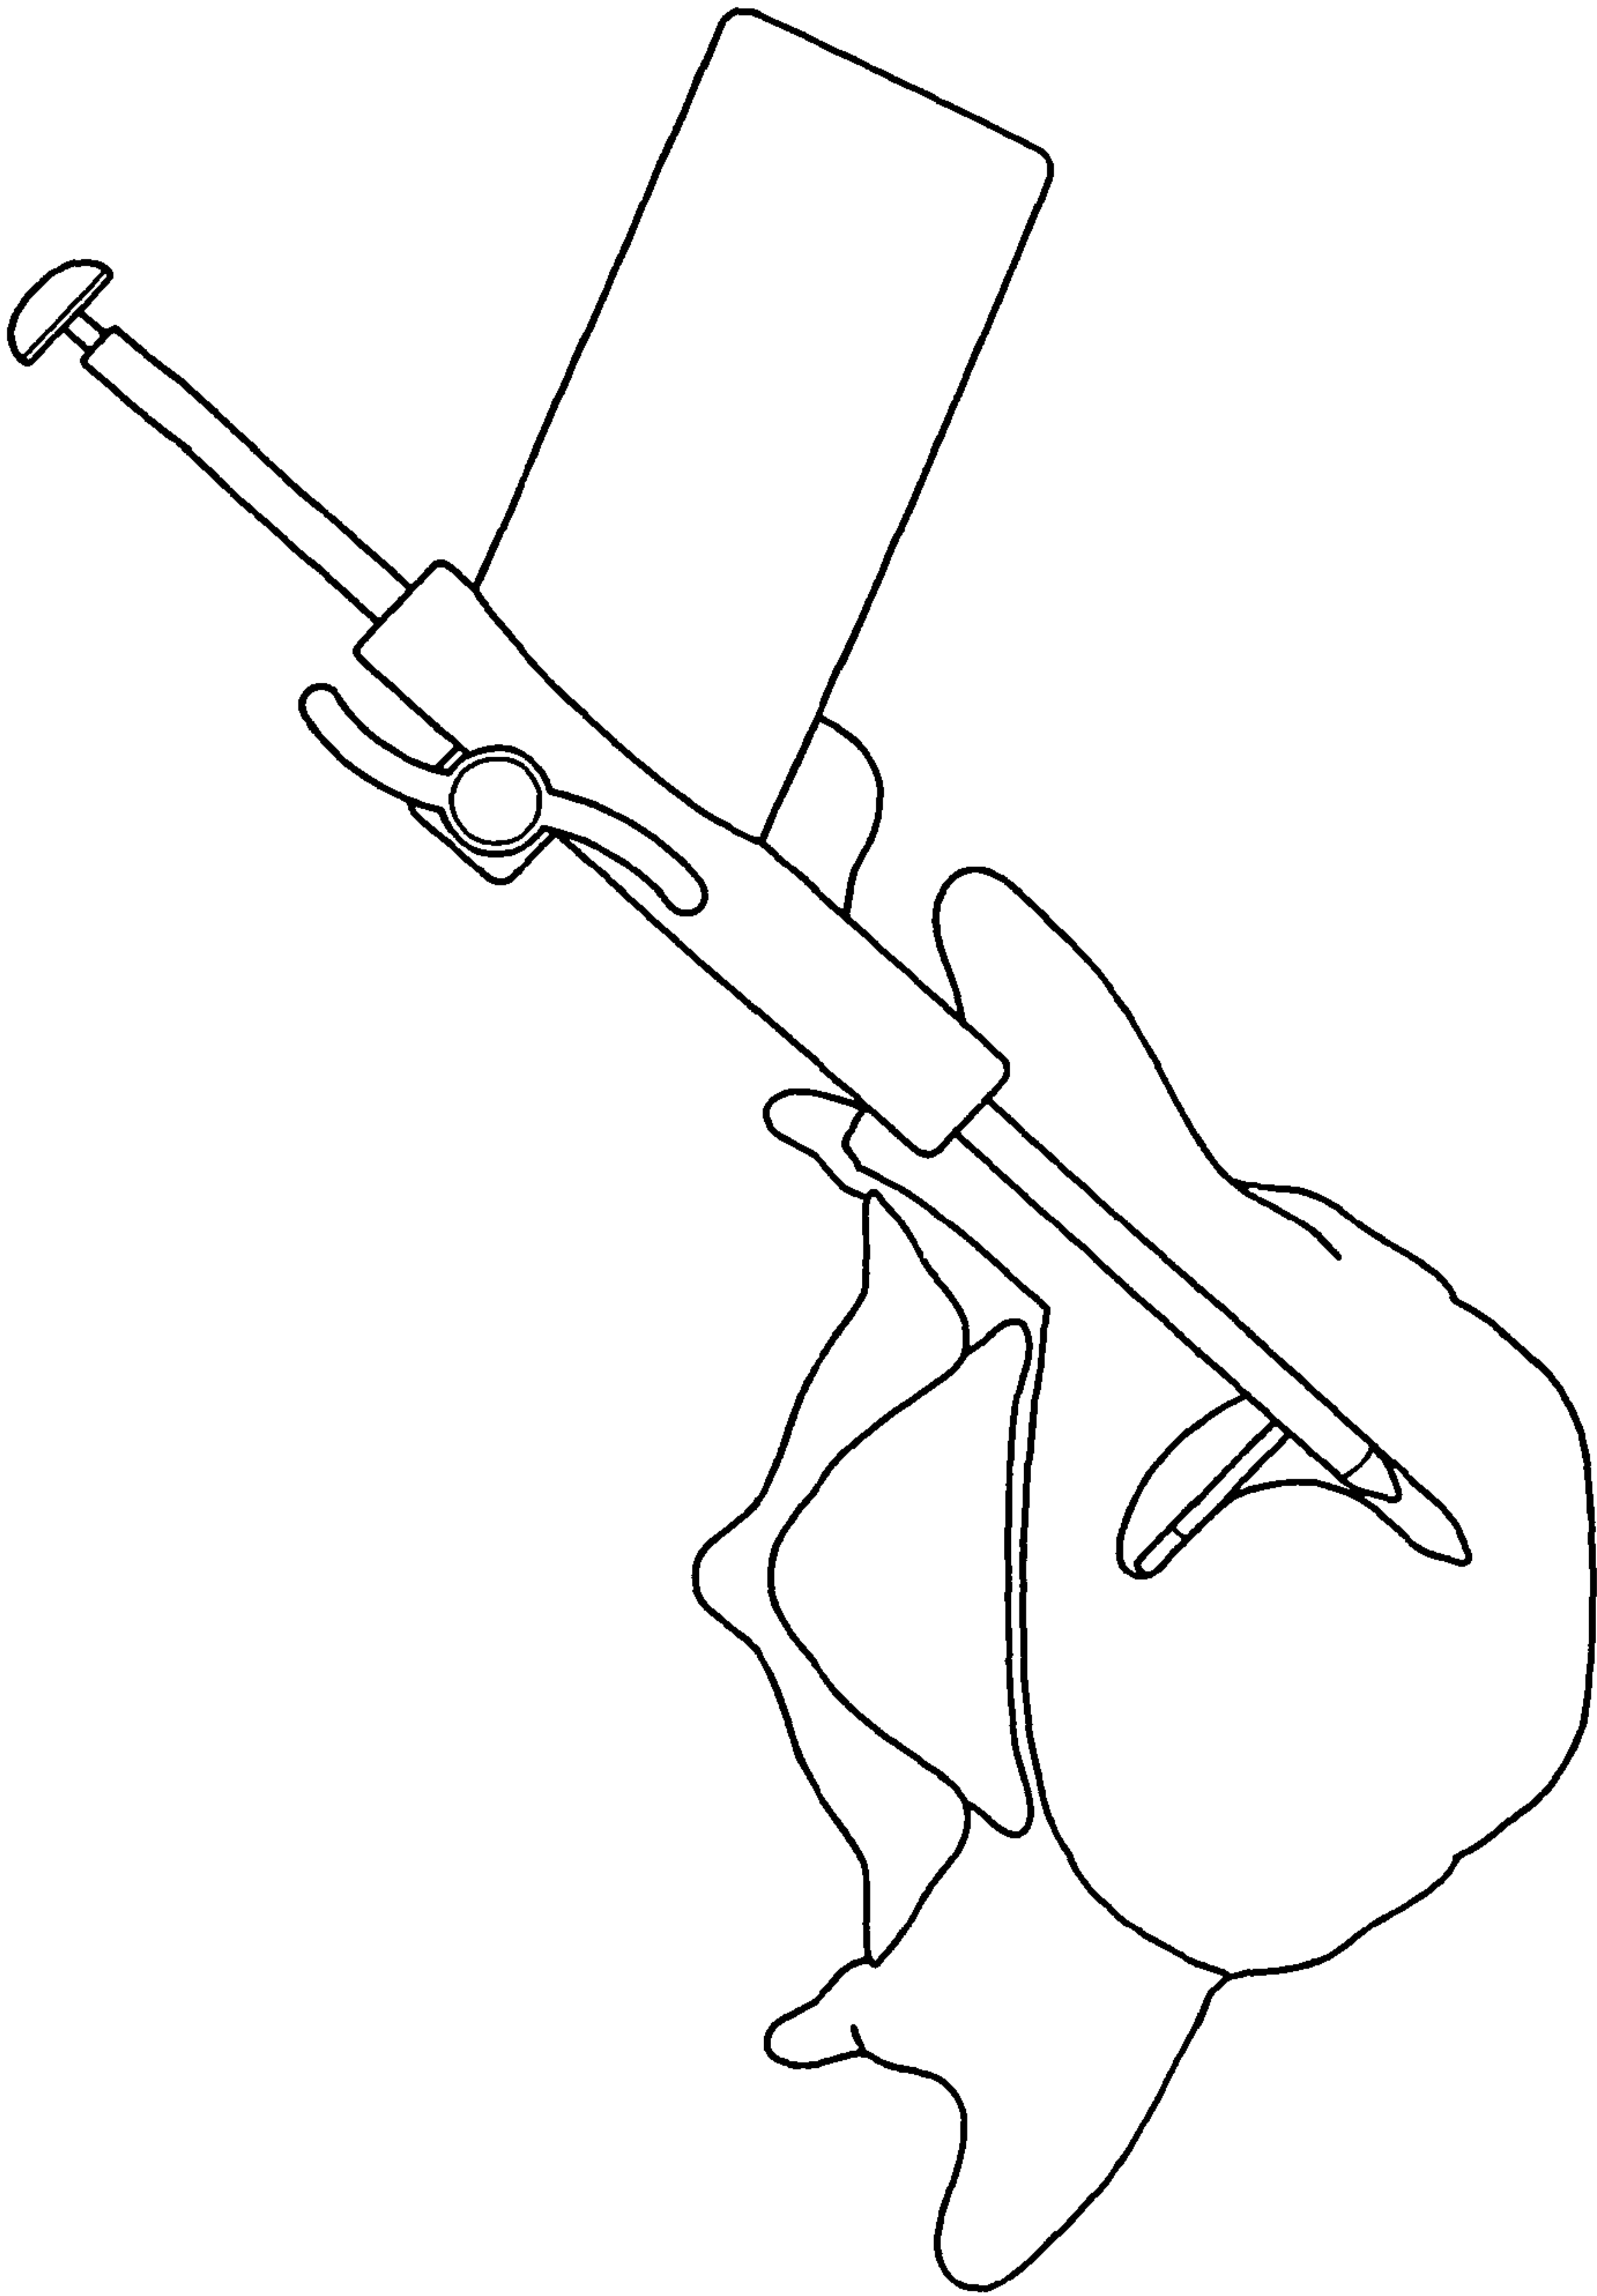


FIG. 31D

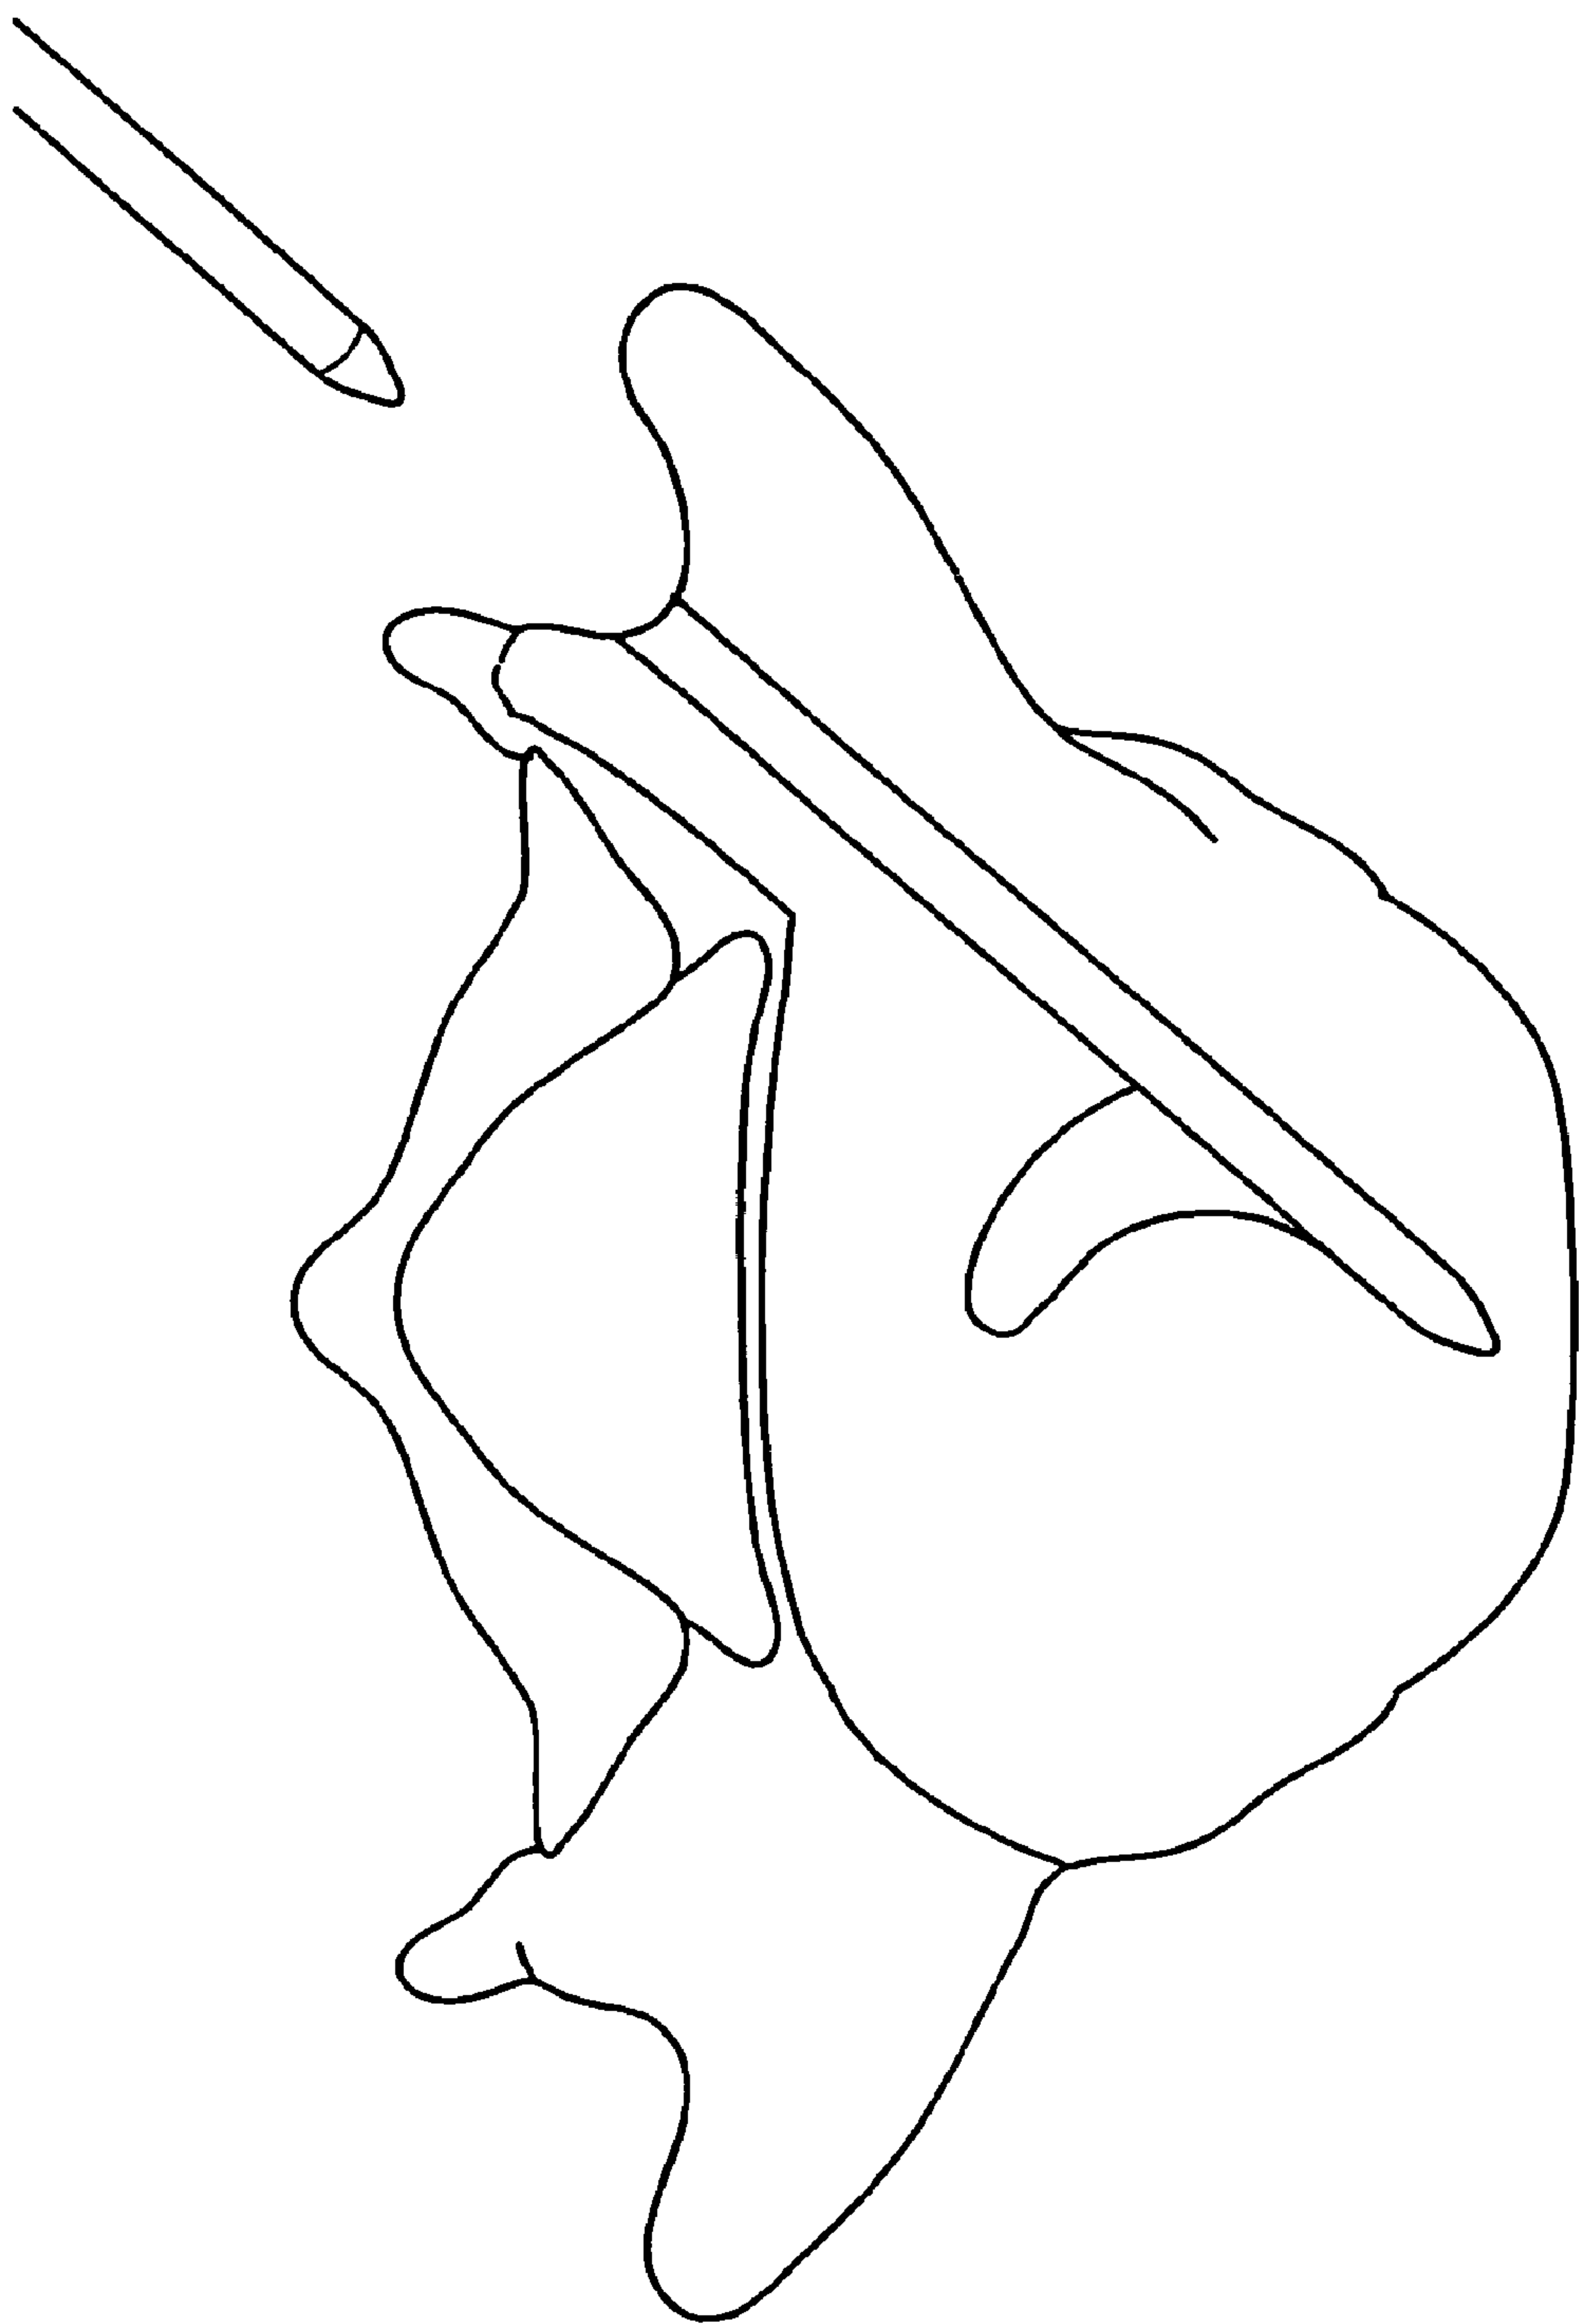


FIG. 31E

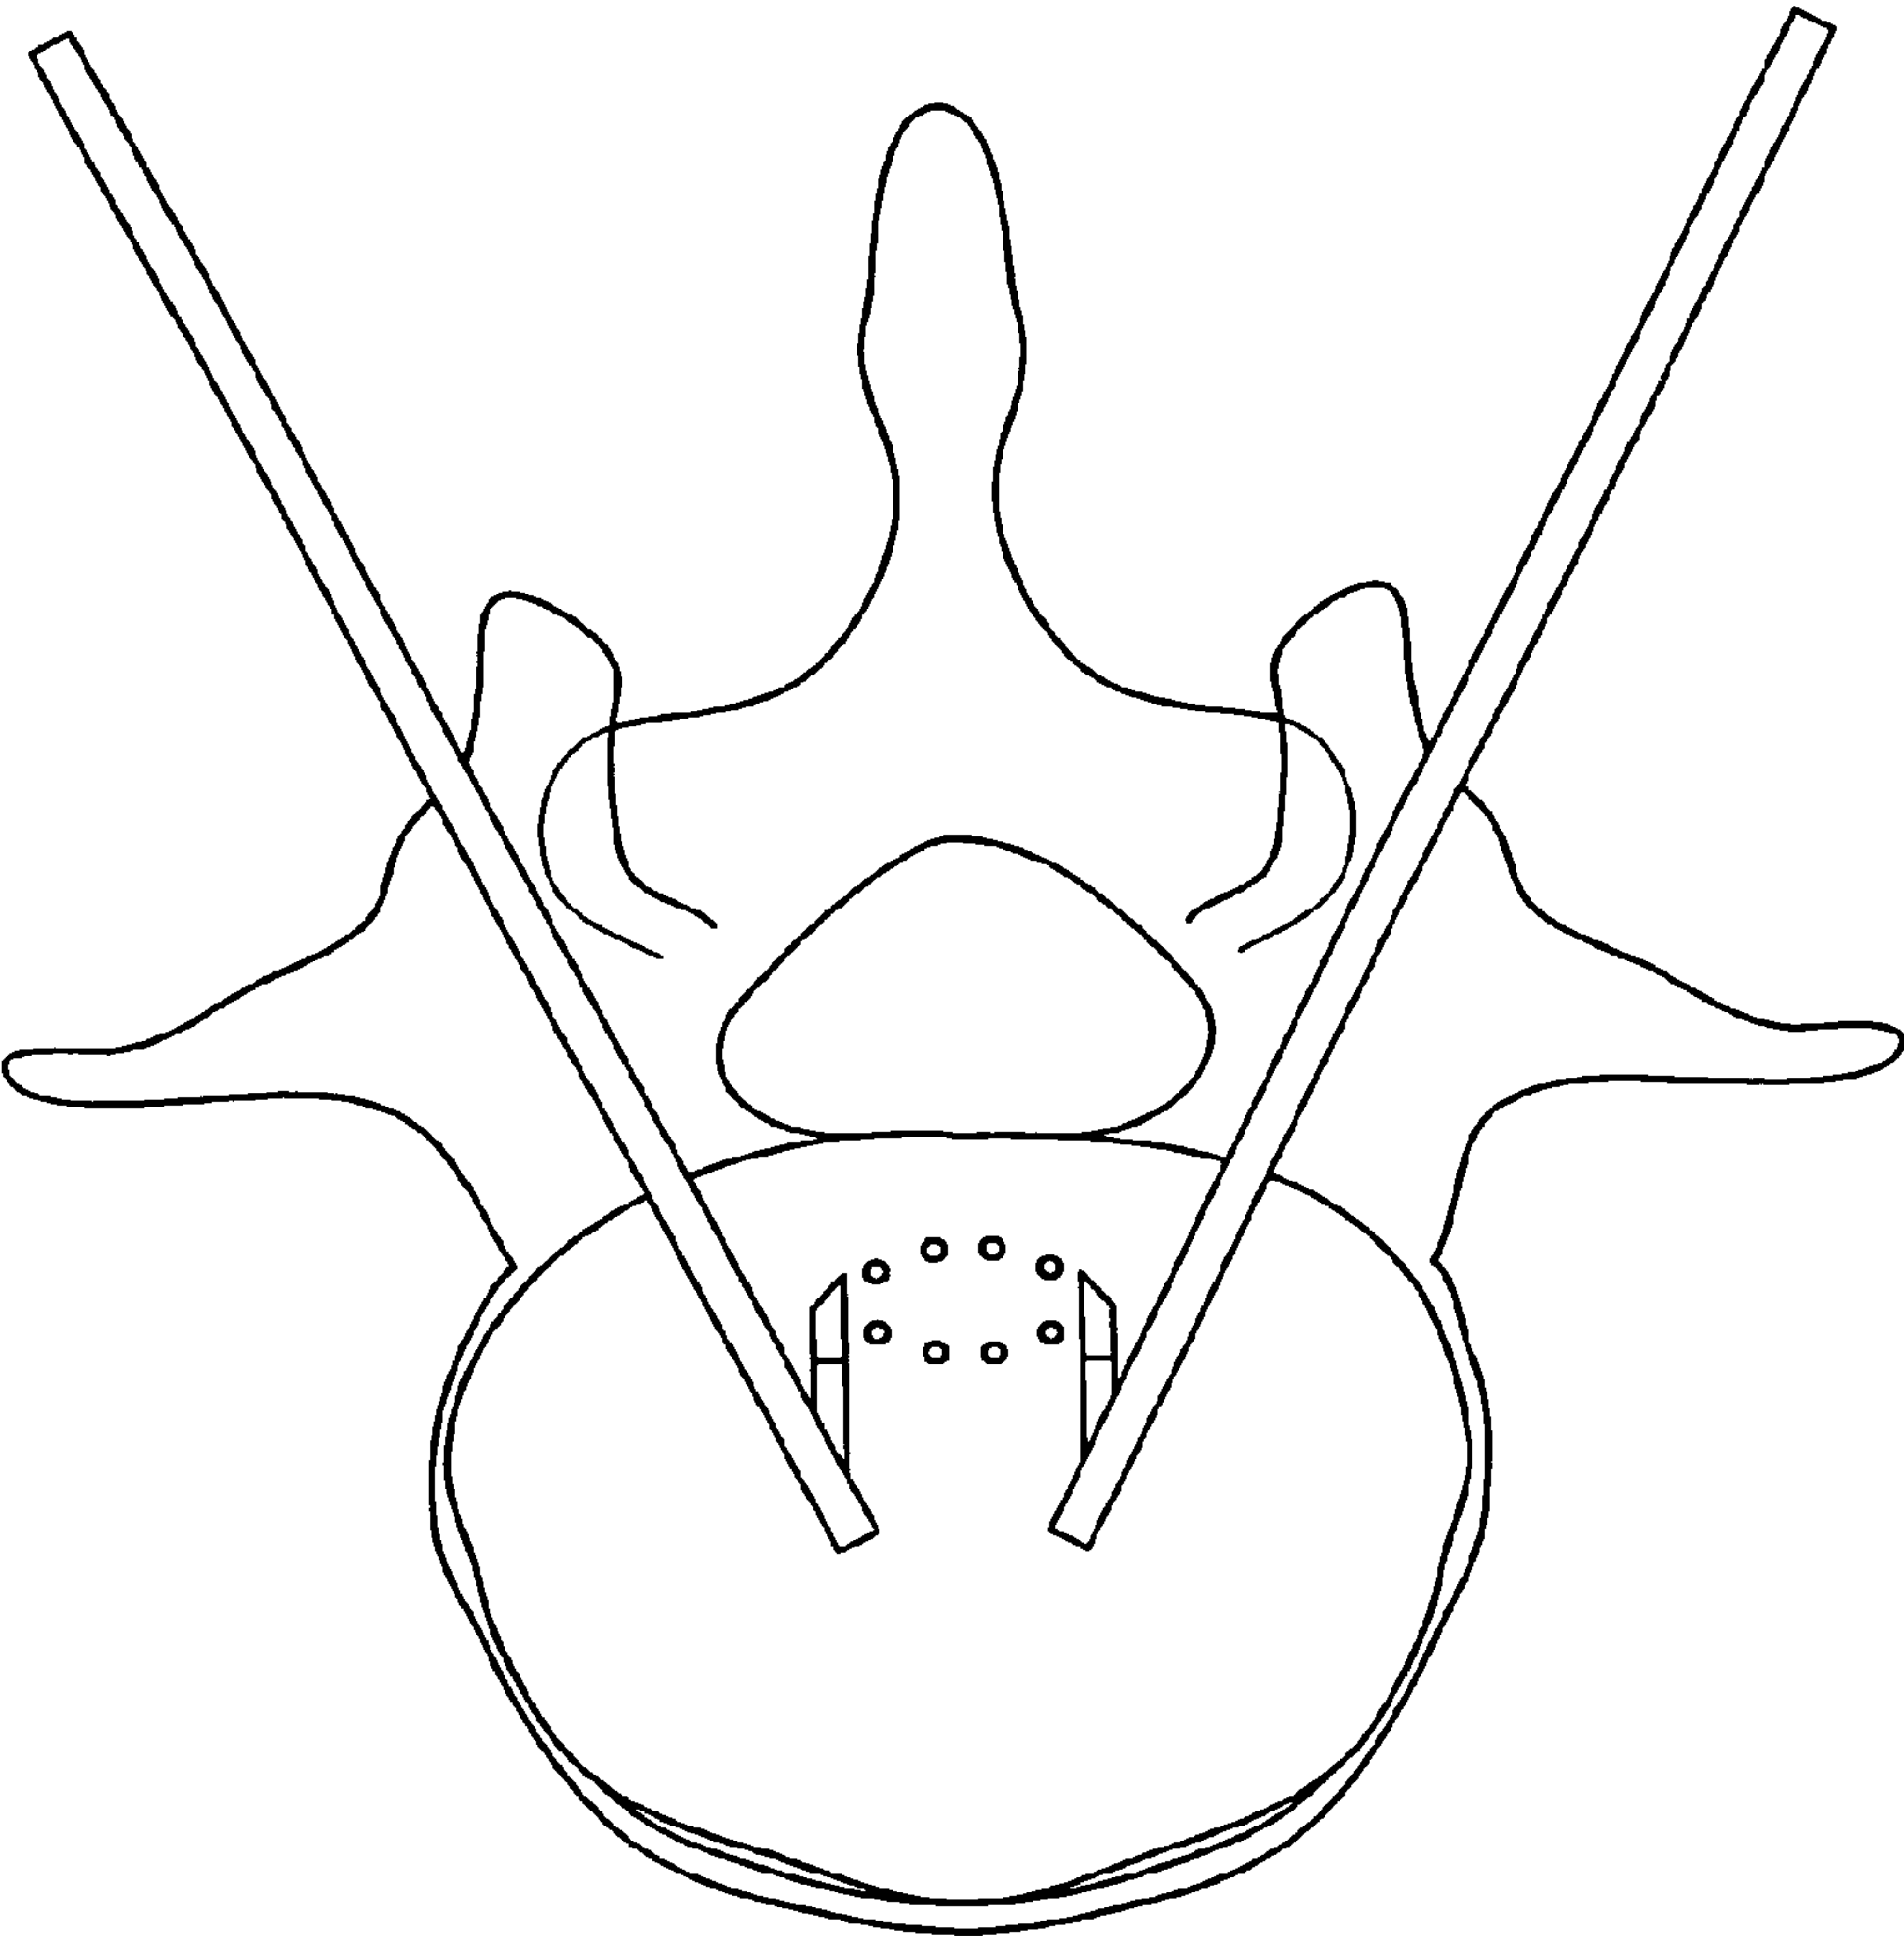


FIG. 32

METHOD OF TREATING AN INTRAOSSEOUS NERVE

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue; a claim printed with strikethrough indicates that the claim was canceled, disclaimed, or held invalid by a prior post-patent action or proceeding.

RELATED APPLICATIONS

This application is a *reissue of U.S. Pat. No. 7,749,218, which issued Jul. 6, 2010 from U.S. patent application Ser. No. 11/123,766, is which is a divisional of U.S. patent application Ser. No. 10/260,879, filed Sep. 30, 2002, entitled "Method of straddling an intraosseous nerve", now issued as U.S. Pat. No. 6,907,884, the specification of which is incorporated by reference.*

BACKGROUND OF THE INVENTION

In an effort to reduce back pain through early intervention techniques, some investigators have focused upon nerves contained within the vertebral bodies which are adjacent the problematic disc.

For example, PCT Patent Publication No. WO 01/0157655 ("Heggeness") discloses ablating nerves contained within the vertebral body by first boring into the vertebral body with a nerve ablation device, placing the tip of the device in close proximity to the nerve, and then ablating the nerves with the tip. Heggeness discloses using laser devices, electricity transmitting devices, fluid transmitting devices and thermal devices, and devices for carrying either chemotherapeutic or radioactive substances as candidate nerve ablation devices.

In describing techniques using electricity transmitting devices, Heggeness discloses "raising the temperature of tip 24 such that the intraosseous nerve is ablated by the heat generated by electrical current passing through tip." See Heggeness at 8,28.

Heggeness further discloses multiple methods of accessing the intraosseous nerve (ION). However, each of these methods essentially disclose either i) boring a straight channel into the vertebra such that placement of an electrode tip near the end of that channel will bring the electrode tip sufficiently close to the ION to effect its ablation, or ii) accessing the basivertebral nerve (BVN) via the vertebral foramen. None of these techniques recognize how to effectively carry out nerve ablation when the precise locations of the ION is unknown, or when the electrode tip can not be maneuvered relatively close to the ION.

EPO Patent Published Patent Application No. EP 1 059067 A1 ("Cosman") discloses ablative treatment of metastatic bone tumors, including those within the spine. Pain relief is reportedly achieved by penetrating the bone wall with a suitable probe, and applying heat through the probe to ablate either the bone tumor or the tissue near the bone tumor. Cosman teaches the use of both monopolar and bipolar probes in this application. Cosman also teaches that the treatment may also be used to ablate the nerves and nerve ramifications in and/or around the bone to desensitize them against further tumor encroachment. See Cosman at col. 11, lines 7-11.

However, monopolar approaches require the use of a grounding pad beneath the patient and allows energy to flow

from the probe and to dissipate in the surrounding tissue. Because the path by which the energy flows from a monopolar probe to its corresponding pad is uncontrolled, the energy may undesirably flow through sensitive tissue, such as the spinal cord. Since this method may cause undesired local muscle or nerve stimulation, it may be difficult or dangerous to operate in sensitive areas of the human body.

Cosman discloses devices whose electrodes can deviate from the axis of the access channel. In particular, Cosman discloses steerable tips, spring-like electrodes that take a straight shape within the catheter and then curve upon exiting the catheter. Cosman discloses that the curved portion of the electrode may be a rigid and rugged permanent curve, or it may be a flexible configuration so that it can be steered, pushed or guided by the clinician to be positioned at various location. See Cosman at col. 8, lines 40-50). Cosman discloses that electrodes may comprise tubing made of elastic or super-elastic metal such as a spring steel or nitinol tubing so that the electrode can be inserted into straight segments of the cannula and still describes a curved path when the curved portion emerges from the opening. See Cosman at col. 10, lines 11-16. Cosman also discloses an electrode having a flexible but steerable tip which can define an arc, as set by the physician. See Cosman at col. 14, line 3.

In sum, Heggeness and Cosman disclose methods of treating that assume the tip of the electrode can be directed substantially to the target tissue.

A few investigators have examined the effectiveness of heating bone with monopolar RF electrodes. DuPuy, AJR: 175, November 2000, 1263-1266 noted decreased heat transmission at a 10 mm distance from the electrode through cancellous bone in ex vivo studies. DuPuy notes that local heat sinks from the rich epidural venous plexus and cerebrospinal pulsations may account for the decreased heat transmission in cancellous bone. Tillotson, Investigative Radiology, 24:11, November 1989, 888-892, studied the percutaneous ablation of the trigeminal ganglion using RF energy, and found that bone marrow necrosis was limited to a sphere of about 1 cm in diameter, regardless of the probe size and duration of heating. Tillotson further reports that Lindskog showed that the transmission of heat within bone is sharply limited by blood flow, and that lethal temperatures cannot be sustained over great distances.

In sum, these investigators appear to report that the well-vascularized nature of bone appears to limit the heating effect of RF electrodes to a distance of less than about 0.5 cm from the tip.

U.S. Pat. No. 6,312,426 ("Goldberg") discloses a system of RF plate-like electrodes for effecting large, uniform, and extended ablation of the tissue proximate the plate-like electrodes. In some embodiments, the plate-like electrodes are placed on the surface of the body tissue, where the ablation is desired, and are configured to lie approximately parallel or opposing one another, such that they make a lesion by coagulating most of the body tissue volume between them. Goldberg appears to be primarily directed to the treatment of tumors. Goldberg states that one advantage of the system is that the surgeon need not determine the precise position of the tumor. See Goldberg at col. 3, line 59-60. Goldberg does not appear to specifically discuss the treatment of nerves.

U.S. Pat. No. 6,139,545 ("Utley") discloses a facial nerve ablation system including at least two spaced apart bi-polar probe electrodes spanning between them a percutaneous tissue region containing a facial nerve branch. Utley teaches that the size and spacing of the electrodes are purposely set

3

to penetrate the skin to a depth sufficient to span a targeted nerve or nerve within a defined region. See col. 5, lines 44-47. Utley further teaches that the system makes possible the non-invasive selection of discrete motor nerve branches, which are small and interspersed in muscle, making them difficult to see and detect, for the purpose of specifically targeting them for ablation. See col. 2, lines 20-24. Utley does not disclose the use of such a system for the treatment of IONS, nor rigid probes, or deployable electrodes. The probes of Utley

SUMMARY OF THE INVENTION

In attempting to place an electrode in close proximity to the BVN, the present inventors have found the approaches disclosed in the teachings of the art to be somewhat problematic. In particular, although the location of the BVN is somewhat well known, the BVN is radiolucent and so its precise location can not be easily identified by an X-ray. Since the BVN is also extremely thin, knowingly placing the electrode in close proximity to the BVN may be problematic. Moreover, since conventional RF electrodes appear to heat only a fairly limited volume of bone, misplacement of the electrode tip vis-à-vis the BVN may result in heating a volume of bone that does not contain the BVN.

For example, and now referring to FIGS. 1 and 2, there is provided a representation of a treatment scheme involving the placement of a conventional bipolar electrode device in close proximity to the ION. In these FIGS., the ION is represented by the solid line identified as ION, while the vertically-disposed dotted lines identify the edges of the zone within which the practitioner believes the ION likely resides (i.e., the ION residence zone, or "IRZ"). As shown in FIGS. 1 and 2, if the ION is substantially in the center of the ION residence zone, then placement of the bipolar electrode either on the left hand boundary of the ION residence zone (as in FIG. 1) or substantially in the middle of the ION residence zone (as in FIG. 2) satisfactorily locates the electrodes in a region that allows the current flowing from the electrodes to flow across the ION. Since the current flowing across the ION may resistively and conductive heat the local bone tissue and the ION will be heated to therapeutically beneficial temperatures, these scenarios may provide beneficial treatment of the ION.

However, and now referring to FIG. 3, if the ION is substantially at the right edge of the ION residence zone, then placement of the bipolar electrodes on the left hand side of the ION residence zone fails to locate the electrodes in a region that allows the current flowing from the electrodes to flow across the ION. Accordingly, current flowing across the electrodes can not resistively heat the ION. Moreover, since bone is a heat sink that effectively limits the heat transport to about 0.5 cm, the heat produced by the electrodes may be effectively dissipated before it can reach the ION by conduction.

Similarly, and now referring to FIG. 4, if the ION is substantially at the left edge of the ION residence zone, then placement of the bipolar electrodes in the middle of the ION residence zone fails to locate the electrodes in a region that allows the current flowing from the electrodes to flow across the ION. Again current flowing across the electrodes can not resistively heat the ION, and the heat sink quality of bone may effectively dissipate the heat produced by the electrodes before it can reach the ION by conduction.

Moreover, even if the precise location of the BVN were known, it has been found to be difficult to access the

4

posterior portion of the BVN from a transpedicular approach with a substantially straight probe.

Therefore, the present inventors set out to produce a system that allows the practitioner to heat the BVN without having to know the precise location of the BVN, and without having to precisely place the electrode tip next to the portion of the BVN to be treated.

The present invention relates to the production of a large but well-controlled heating zone within bone tissue to therapeutically treat an ION within the heating zone.

Now referring to FIGS. 5-6, there is provided a representation of an embodiment of the present invention in which electrodes E1 and E2 respectively disposed probes (not shown) therapeutically treat the ION. FIG. 5 provides a schematic representation of the electric field EF produced in the bone tissue by activation of the electrodes. In this case, the electric field is relatively thin. FIG. 6 provides a schematic representation of the total heating zone THZ produced by the electric field of FIG. 5 including both an inner resistive heating zone IR (represented by open circle) and an outer conductive heating zone OC (represented by closed circles). In this case, the inner resistive zone is produced by the joule heating of bone tissue disposed within the electric field EF, while the outer conductive zone is heated by conduction of heat from the resistive heating zone.

Still referring to FIG. 6, the present inventors have found that positioning the active and return electrodes of an energy-transmitting device in a manner that allows the electrodes to straddle the ION residence zone IRZ provides a large but well-controlled total heating zone (IR+OC) within bone tissue to therapeutically treat the ION within the heating zone. Since the total heating zone is large and the electrodes straddle the IRZ, there is a high level of confidence that a portion of the ION will be present within the total heating zone. Since the total heating zone is well controlled, there is no danger (as with monopolar systems) that current flowing from the active electrode will undesirably affect collateral tissue structures.

Now referring to FIG. 7, if the ION is in fact substantially in the center of the ION residence zone, then placement of the bipolar electrodes in a manner that straddles the ION residence zone allows the production a total heating zone between the electrodes that includes a portion of the ION therein.

Moreover, the present invention allows the practitioner to therapeutically treat the ION even when the ION is in fact located at the edges of the ION residence zone IRZ. Now referring to FIGS. 8 and 9, if the ION is located substantially at the right edge (as in FIG. 8) or the left edge (as in FIG. 9) of the ION residence zone IRZ, then placement of the bipolar electrodes in a manner that straddles the ION residence zone still allows the production a total heating zone between the electrodes that includes a portion of the actual ION therein.

Therefore, the straddling of the ION residence zone by the present invention satisfactorily locates the electrodes so that the total heating zone produced by the electrode activation includes the ION irrespective of the actual location of the ION within the ION residence zone IRZ, thereby guaranteeing that the electrodes will always heat the ION to therapeutically beneficial temperatures.

Therefore, in accordance with the present invention, there is provided a method of therapeutically treating a bone having an intraosseous nerve ION defining first and second sides of the bone, comprising the steps of:

a) inserting an energy device having an active and a return electrode into the bone,

5

b) placing the active electrode on the first side of the bone and the return electrode on the second side of the bone to define a total heating zone therebetween, and applying a sufficiently high frequency voltage between the active and return electrodes to generate a current therebetween to resistively heat the total heating zone sufficient to denervate the ION.

In addition, the present invention provides a very controlled total heating zone which exists substantially only between the paired electrodes. The ability of the present invention to both therapeutically heat the BVN with substantial certainty and to minimize the volume of bone tissue affected by the heating appears to be novel in light of the conventional bone-related technology.

Accordingly, the present invention is further advantageous because it allows the clinician to create a sufficiently large heating zone for therapeutically treating the ION without requiring direct access to the ION.

Thus, in preferred embodiments, the present invention is advantageous because:

- 1) it does not require knowing the precise location of the ION,
- 2) it does not require directly accessing the ION, and 3) its controlled heating profile allows the clinician to avoid heating adjacent structures such as the healthy adjacent cancellous bone tissue, the spinal cord or opposing vertebral endplates.

Accordingly, there is also provide a method of therapeutically treating a vertebral body having a BVN defining first and second sides of the vertebral body, comprising the steps of:

- a) determining a BVN residence zone within which the BVN likely resides, the BVN residence zone having a first side and a second side,
- b) inserting an energy device having an active and a return electrode into the vertebral body,
- c) placing the active electrode on the first side of the residence zone and the return electrode on the second side of the residence zone to define a total heating zone therebetween, and
- d) applying a sufficiently high frequency voltage between the active and return electrodes to generate a current therebetween to resistively heat the total heating zone to a temperature sufficient to denervate the BVN.

DESCRIPTION OF THE FIGURES

FIGS. 1 and 2 depict the treatment of the BVN with a conventional bipolar electrode.

FIGS. 3 and 4 depict the difficulty of treating a BVN with a conventional bipolar electrode.

FIGS. 5 respectively depict top views of an electric field and a total heating zone produced within bone tissue by an embodiment of the present invention.

FIGS. 7-9 depict the treatment of the BVN with a bipolar electrode apparatus of the present invention.

FIGS. 10a and 10b disclose anterior and upper cross-sectional views of a straddled ION that extends in a plane above the electrodes but within the total heating zone.

FIG. 11 is a cross-sectional anterior view of an embodiment of the present invention in which the total heating zone has dumb-bell type resistive heating zones.

FIG. 12 depicts a top view of the treatment of the BVN with a bipolar electrode apparatus of the present invention wherein the distal ends of the probes are located substantially at the midline of the vertebral body.

6

FIG. 13 discloses cross-sections of components of a preferred dual probe apparatus according to the present invention.

FIG. 14 discloses an embodiment of the present invention in which a portion of the probe shaft acts as an electrode.

FIGS. 15-18 discloses four embodiments of the present invention in which at least a portion of the electrode faces thereof are disposed in a substantially parallel relation.

FIG. 19 discloses a cross-sectional view of an apparatus of the present invention in which the cannula has a bore having a distal bend and a lateral opening.

FIGS. 20a and 20b disclose cross-sectional views of an apparatus of the present invention in which the cannula has a proximal bend.

FIGS. 21a and 21b disclose cross-sectional views of an apparatus of the present invention in which the probe has a pivoted portion containing an electrode.

FIG. 22 discloses a probe of the present invention having reverse conical electrodes.

FIG. 23 discloses a probe of the present invention having a plurality of active electrodes and a corresponding plurality of return electrodes.

FIG. 24 discloses a bipolar probe of the present invention in which the return electrode has a relatively large surface area.

FIG. 25 presents a cross-sectional view of an articulated probe of the present invention having both active and return electrodes.

FIG. 26 discloses the treatment of a posterior portion of the BVN with a bipolar electrode apparatus of the present invention. FIGS. 27a-d disclose respective top, anterior, lateral and perspective views of the placement of a bipolar electrode apparatus of the present invention within a vertebral body.

FIGS. 28a and 28b show the location of thermocouples T0-T14 within the vertebral body.

FIG. 29a-c present the temperatures recorded by thermocouples T0-T14.

FIG. 30a-b present the peak temperatures recorded by thermocouples T0-T14 within the vertebral body.

FIGS. 31a-e present top views of a preferred use of the articulated probe of FIG. 25.

FIG. 32 presents a dual articulated needle embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

For the purposes of the present invention, the “resistive heating zone” is the zone of bone tissue that is resistively heated due to an energy loss incurred by current travelling directly through the bone tissue. Resistive heating, “joule” heating and “near-field” heating may be used interchangeably herein. The “conductive heating zone” is the zone of bone tissue that is heated due to the conduction of heat from an adjacent resistive heating zone. The total heating zone THZ in a bone tissue includes both the resistive heating zone and the conductive heating zone. The border between the conductive and resistive heating zones is defined by the locations where the strength of the electric field is 10% of the maximum strength of the electric field between the electrodes. For the purposes of the present invention, the heating zones encompass the volume of bone tissue heated to at least 42° C. by the present invention. For the purposes of the present invention, the “first and second sides” of a vertebral body are the lateral-lateral sides intersected by the BVN.

The therapeutic treatment of the ION may be carried out in accordance with the present invention by resistive heating, conductive heating, or by hybrid heating.

In some embodiments, the therapeutic heating of the ION is provided by both resistive and conductive heating. In some embodiments thereof, as in FIG. 6, the electrodes are placed such that the ION passes through resistive heating zone IR, so that length L_1 of the ION is therapeutically heated by bone tissue in the resistive heating zone IR and lengths L_2 and L_3 of the ION are therapeutically heated by the bone tissue in the conductive heating zone OC.

In embodiments wherein the therapeutic heating of the ION is provided substantially by both resistive and conductive heating, it is preferred that the length L_1 of the ION treated by resistive heating comprise at least 25% of the total therapeutically treated length of ION, more preferably at least 50%. In many embodiments, the peak temperature in the resistive heating zone IR is between 40° C. and 60° C. greater than the peak temperature in the conductive heating zone OC. Preferably, the peak temperature in the resistive heating zone IR is no more than 15° C. greater than the peak temperature in the conductive heating zone OC, more preferably no more than 10° C., more preferably no more than 5 degrees.

Now referring to FIGS. 10a and 10b, in some embodiments, the therapeutic heating of the ION is provided essentially by the conductive heating zone OC. This may occur when the ION is in fact located substantially far from the middle of the ION residence zone IRZ. In such an instance, the electrodes are placed such that the ION passes only through the conductive heating zone, so that length L_2 of the ION is therapeutically heated by bone tissue in the conductive heating zone OC.

In preferred embodiments thereof, it is desired that the separation distance SD between the ION and the resistive heating zone IR be no more than 1 cm. This is desired because the closer the ION is to the resistive heating zone, the higher the temperature experienced by the ION length L_2 . More preferably, the separation distance is no more than 0.5 cm, more preferably no more than 0.2 cm.

In some embodiments, as in FIG. 10, the electric field is sufficiently strong to be located substantially continuously between the two electrodes. This typically occurs when the electrodes are very close together (i.e., no more than 5 mm apart). In others, however, as in FIG. 11, the electric field is relatively weak and so resides substantially only in the vicinity of the two electrodes. In such cases, and now referring to FIG. 11, inward energy flow from the resistive heating zones IR conductively heats the intermediate area of the conductive heating zone OC₁. Preferably, the peak temperature in the resistive heating zone IR is no more than 15° C. greater than the peak temperature in the intermediate conductive heating zone OC₁, more preferably no more than 10° C., more preferably no more than 5° C.

In preferred embodiments, the present invention is carried out via a dual probe system. In particular, the present invention preferably comprises an energy delivery device comprising a first probe having an active electrode and a second probe having a return electrode. Now referring to FIG. 12, this dual probe embodiment allows the surgeon to approach the BVN from separate sides of the vertebral body to easily straddle the IRZ with the electrodes. With such a device, the surgeon can place the first probe 601 having an active electrode 603 on a first side of the vertebral body and the second probe 611 having a return electrode 613 on a second side of the vertebral body, and then align the paired

electrodes so that their activation produces a total heating zone that straddles the IRZ and therefore the BVN therein.

Since aligning the electrodes of such an apparatus to straddle the ION merely requires advancing the probes into the vertebral body, no complicated navigation is required. The present inventors have appreciated that, even if the location of the BVN were precisely known, conventional methods of accessing the BVN require either i) the BVN to be naturally located within the vertebral body so as to intersect the axis of the pedicle (Heggeness), or require a complicated probe configuration or navigation (such as those described by Cosman). Because the dual probe approach simply requires substantially linear advance of a pair of substantially straight probes, it is much simpler and/or much more robust than the conventional methods of accessing nerves in bone. Indeed, with this embodiment of the present invention, the clinician may now desirably access the vertebral body through the pedicles with substantially straight probes and have a high confidence that their activation can therapeutically treat the BVN.

Therefore, in accordance with the present invention, there is provided a method of therapeutically treating a vertebral body having a BVN, comprising the steps of:

- a) providing an energy device having an active electrode having a first face and a return electrode having a second face into the vertebral body, and
 - b) placing the active electrode in the vertebral body to face a first direction,
 - c) placing the return electrode in the vertebral body to face a second direction, the first and second faces defining an angle 2δ of no more than 60 degrees, and
- applying a sufficiently high frequency voltage difference between the active and return electrodes to generate a current therebetween to produce a total heating zone to therapeutically heat the BVN.

Therefore, in accordance with the present invention, there is provided a method of therapeutically treating a vertebral body having a BVN, comprising the steps of:

- a) providing an energy device having an active electrode and a return electrode,
- b) placing the active and return electrodes in the vertebral body to define an electrode axis, the axis forming an angle β of between 50 and 90 degrees with the BVN, and
- c) applying a sufficiently high frequency voltage difference between the active and return electrodes to generate a current therebetween to produce a total heating zone to therapeutically heat the BVN.

Now referring to FIG. 13, there is provided a preferred dual probe apparatus according to the present invention comprising first 101 and second 151 cannulae, first 201 and second 251 stylets, first 301 and second 351 probes, and a power supply 401 in electrical connection with the probes. For simplicity, only a single cannula, stylet and probe will be further described. However, the skilled artisan will appreciate that preferred embodiments use two sets of such devices.

Now referring to FIG. 13, cannula 101 comprises a shaft 103 having a longitudinal bore 105 therethrough defining an inner diameter D_c . Distal opening 109 of the cannula provides a working portal for the probe. It is further sized to allow the distal end of the probe to advance past the distal end 107 of the cannula. The length L_c of the cannula is sized to reach from the patient's skin to a location within the cancellous bone region of the target bone. Preferably, the cannula is made of a material selected from the group consisting of metal and polymer, and is preferably polymer. In many embodiments, the cannula is made of an insulating

material in order to prevent stray current from the probe from contacting non-targeted tissue.

In some embodiments, the cannula is shaped so as to guide the probe towards the midline of the vertebral body. This inward guidance will help move the electrodes closer to the BVN. In some embodiments, at least a portion of the cannula bore is curved. In some embodiments, at least half of the length of the cannula bore is curved. In other embodiments, substantially only the distal end portion of the cannula bore is curved.

Stylet **201** comprises a shaft **203** having a longitudinal axis A and a proximal **205** and distal end **207**. Disposed at the distal end of the shaft is a tip **209** adapted for boring or drilling through cortical bone. The outer diameter D_O of the stylet shaft is preferably adapted to be received within the inner diameter D_C of the cannula.

For the purposes of the present invention, the combination of the cannula and the stylet is referred to as a "cannulated needle". In some embodiments, access to the vertebral body is gained by first placing the stylet in the cannula to produce a cannulated needle, piercing the skin with the cannulated needle, and advancing the cannulated needle so that the stylet tip reaches a target tissue region within the cancellous portion of the vertebral body, and then withdrawing the stylet. At this point, the cannula is conveniently located at the target tissue region to receive a probe of the present invention.

Probe **301** comprises a shaft **303** having a longitudinal axis B, a distal end portion **305** and a proximal end portion **307**. Disposed near the distal end portion of the probe is first electrode **309** having a first face **331** and a connection face **333**. The probe is designed so that the connection face of the first electrode is placed in electrical connection with a first lead **403** of the power supply. In this particular embodiment, the shaft has a longitudinal bore **311** extending from the proximal end portion up to at least the first electrode. Disposed within the bore is a wire **321** electrically connected at its first end **323** to the first electrode and having a second end **325** adapted to be electrically connected to a first lead of a power supply.

Therefore, in accordance with the present invention, there is provided an intraosseous nerve denervation system, comprising:

- a) a cannula having a longitudinal bore,
- b) a stylet having an outer diameter adapted to be received within the longitudinal bore and a distal tip adapted to penetrate cortical bone, and
- c) a first probe comprising:
 - i) an outer diameter adapted to be received within the longitudinal bore, and
 - ii) a first electrode, and
 - iii) a lead in electrical connection with the first electrode.

In some embodiments, the outer surface of the probe is provided with depth markings so that the clinician can understand the extent to which it has penetrated the vertebral body.

In some embodiments in which a cannulated stylet is first inserted, the stylet is removed and the cannula remains in place with its distal opening residing in the target tissue while the probe is inserted into the cannula. In this embodiment, the cannula provides a secure portal for the probe, thereby insuring that the probe can enter the bone safely. This embodiment is especially preferred when the probe is made of a flexible material, or is shaped with an irregular cross-section that could undesirably catch on the bone during probe advancement into the bone.

In the FIG. **13** probe disclosed above, probe **301** has a blunt tip. In other embodiments, however, the probe carrying an electrode can be configured to possess a sharp distal tip having sufficient sharpness to penetrate cortical bone. With such a tip, the clinician can eliminate steps in the procedure that are related to either the stylet or the cannulated stylet, and thereby save time.

Now referring to FIG. **14**, in some embodiments, the electrode may include a portion of the probe shaft. For example, in the case of probe **1401**, the probe comprises:

- a) an inner electrically conductive shaft **1403** in electrical connection with a power supply **1409**, and
- b) an outer insulating jacket **1405** wrapped around a portion of the shaft.

In this configuration, the placement of the jacket provides a distal uninsulated shaft portion **1407** that could be used as an electrode. Preferably, the distal uninsulated portion of the shaft has a length of between 3 mm and 8 mm, and is more preferably about 5 mm. In preferred embodiments thereof, the insulation is selected from the group consisting of polyimide tape, PTFE tape, and heat shrink tubing. Preferred thickness of the insulation range from about 0.00025 to 0.0005 inches.

In other embodiments using insulating jackets, the jacket has either a longitudinally extending slit or slot that exposes a longitudinal surface area of the underlying shaft, thereby producing either an essentially linear or an essentially planar electrode. In such embodiments, the distal end of the shaft may preferably be insulated. In other embodiments using insulating jackets, the insulated portion may comprise a proximal jacket and a distal jacket positioned to provide a space therebetween that exposes a surface area of the underlying shaft to produce the electrode. In some embodiments, the proximal and distal jacket substantially encircle the shaft to provide an annular electrode therebetween.

In some embodiments in which a cannulated stylet is used, both the stylet and the cannula are removed, and the probe is inserted into the hole created by the cannulated stylet. In this embodiment, the hole provides a large portal for the probe. This embodiment conserves the annulus of bone removed by the cannula, and so is preferred when the probe has a relatively large diameter (e.g., more than 8 mm in diameter).

In some embodiments in which a cannulated stylet is used, the cannula comprises at least one electrode. In this embodiment, the cannula acts as the probe as well. With this embodiment, the clinician can eliminate steps in the procedure that are related to introducing a body into the cannula. In some embodiments, the outer surface of the cannula is provided with depth markings so that the clinician can understand the extent to which the cannula has penetrated the vertebral body.

In some embodiments in which a cannulated stylet is first inserted, the stylet comprises at least one electrode. In this embodiment, the stylet acts as the probe as well. With this embodiment, the clinician can eliminate steps in the procedure that are related to removing the stylet and introducing a body into the cannula. In some embodiments, the outer surface of the stylet is provided with depth markings so that the clinician can understand the extent to which it has penetrated the vertebral body.

In conducting initial animal experiments with a dual probe embodiment, the present inventors used a bipedicle approach as shown in FIG. **12**, so that each probe approached the ION at angle δ of 45 to about 55 degrees. Since both the probes and the electrodes disposed thereon were essentially cylindrical, the inner faces **605**, **615** of the

11

electrodes produced an angle 2δ . Subsequent testing of the configuration of FIG. 12 revealed somewhat higher temperatures at the distal portion of the electrodes and somewhat lower temperatures near the proximal portions of the electrodes. Without wishing to be tied to a theory, it is believed that the shorter path between the distal regions produced a lower resistance region (as compared to more proximal inter-electrode regions) and so caused current to preferentially follow the path of the least resistance between the distal portions. Accordingly, the present inventors sought to improve upon the relatively uneven temperature profile produced by the electrode design of FIG. 12.

In accordance with the present invention the present inventors modified its electrode design to reduce the angle 2δ produces by the inner faces, so that the distance between the proximal end of the electrodes is more equal to the distance between the proximal end of the electrodes (i.e., the faces are more parallel). When the electrodes are provided in such a condition, their orientation reduces the significance of any path of least resistance, and so current flows more evenly across the face of each electrode, thereby providing even heating and greater control over the system.

Therefore, in accordance with the present invention, there is provided an intraosseous nerve denervation device, comprising:

- a) a first probe having an active electrode and a first lead,
- b) a second probe having a return electrode and a second lead,
- c) means for creating first and second bores within a bone for accommodating the first and second probes,
- d) a power supply capable of generating a voltage difference between the active and return electrodes, the supply having third and fourth leads,

wherein the first and third leads are in electrical connection, and the second and fourth leads are in electrical connection.

Preferably, the electrodes are disposed so that the angle 2δ produced by the inner faces is less than 60 degrees, more preferably no more than 30 degrees. Still more preferably, the angle is less than 1 degree. Most preferably, the inner faces are substantially parallel.

Now referring to FIG. 15, in some embodiments, substantially parallel electrodes are provided by using conical electrodes 501 that taper distally. In this FIG. 15, each cone electrode 501 has a distal end 503 having a diameter D_D and a proximal end 505 having a diameter D_P , wherein the distal end diameter D_D is larger than the proximal end diameter D_P . Preferably, the angle γ of the cone taper is substantially equal to the angle δ . In this condition, the inner faces of the conical electrodes will be essentially parallel to each other.

Therefore, in accordance with the present invention, there is provided intraosseous nerve denervation system comprising:

- a) a first probe having a first electrode and a first lead in electrical connection with the first electrode, wherein the first electrode has a proximal end having a proximal diameter and a distal end having a distal diameter, and the proximal end diameter is less than the distal end diameter, and
- b) a second probe having a first electrode and a first lead in electrical connection with the first electrode, wherein the first electrode has a proximal end having a proximal diameter and a distal end having a distal diameter, and the proximal end diameter is less than the distal end diameter, and

12

wherein the first and second electrode are disposed so that the electrodes are parallel.

In FIG. 10, the conical shapes are frustoconical (i.e., they are portions of a cone). Frustoconical electrodes are desirable in situations where tissue charring needs to be avoided, as the relatively large diameter of the distal end of the electrode can not provide an avenue for high current density (relative to the proximal end of the electrode). Frustoconical electrodes are also desirable in situations where the probes are disposed at a relatively high angle δ , wherein the use of sharp tipped electrodes would substantially shorten the distance between the distal tips of the electrodes and thereby create an undesirable path of significantly less resistance.

In some embodiments, the frustoconical electrode is shaped so that the diameter of its distal end D_D is between about 10% and 25% of the diameter of its proximal end D . In some embodiments, the frustoconical nature of the electrode is provided by physically severing the sharp distal end of the electrode. In others, the frustoconical nature of the electrode is provided by insulating the sharp distal end of an electrode.

As noted above, when the probes are placed such that their corresponding electrodes are parallel to each other, the electric field produced by electrode activation is substantially uniform between the distal and proximal portions of the electrodes. However, as the probes are oriented at an angle from parallel, the electric field becomes strongest where the electrodes are closer together. In order to compensate for this non-uniform electric field, in some embodiments of the present invention, the distal ends of the electrodes are tapered. In this tapered state, the regions of the electrodes that are closer together (e.g., the tip) also have a smaller surface area (thereby reducing the electric field in that region), while the regions of the electrodes that are farther apart (e.g., the trunk) have a larger surface area (thereby increasing the electric field in that region). Typically, the effect is largely determined by the cone size, electrode spacing and tissue type therebetween.

In some preferred embodiments of the tapered electrode, and now referring to FIG. 16, the distal end of the electrode terminates in a sharp tip, so that the electrode has a more completely conical shape. Preferably, the conical electrode is shaped so that the diameter of its distal end is no more than 20% of the diameter of its proximal end, more preferably no more than 10%, more preferably no more than 1%. In addition to compensating for non-uniformity in the electric field, the sharp tip may also be adapted to penetrate the cortical shell of the vertebral body.

Now referring to FIG. 17, in some embodiments, current flows through an electrode having only a portion of the conical or frusto-conical shape. When electrodes of this embodiment, termed "sectored cones" face each other, their use is advantageous because they insure that current will flow the least distance, and so provide efficiency. The sectored cones of this embodiment can be produced by first manufacturing planar electrodes 511 and placing the planar electrode upon a conveniently angled probe surface 513. Alternatively, this embodiment can be produced by first manufacturing the conical electrode configuration of FIG. 15, and then masking a portion of the conical electrode with an insulating material. Unlike the embodiment of FIG. 15, this sectored cone embodiment requires careful alignment of the electrode faces and may require in vivo rotation of the electrodes to achieve the desired alignment.

Now referring to FIG. 18, in other embodiments, substantially parallel electrodes can be provided by using elbowed probes 531. The elbowed probes have a distal end 533 and

a proximal end **535** meeting at an elbow **537**. In some embodiments, the elbow may be produced during the manufacturing process (thereby requiring a smaller diameter probe in order to fit through the cannula). In other embodiments, the elbow is produced in vivo, such as through use of a pull-wire, a pivot or a memory metal disposed within the probe.

Now referring to FIG. **19**, in some embodiments, first **551** and second **552** cannulae are each provided with a curved bore **553**, **554** forming distal lateral openings **563**, **564** in their respective distal end portions **555**, **556**. When flexible probes **557**, **558** containing an electrode **559**, **560** are passed through the curved bore, the distal end **561**, **562** of the probe likewise conforms to the curved bore, thereby forming an intra-probe angle ϵ determined by the proximal A_P and distal A_D axes of the probe. Preferably, this intra-probe angle is between 90 and 135 degrees. Preferably, the intra-probe angle is selected so that the distal axes A_D of the probes exiting the cannulae form an angle of no more than 30 degrees, preferably no more than 10 degrees, more preferably form a substantially parallel relation.

Therefore, in accordance with the present invention, there is provided an intraosseous nerve denervation system, comprising:

- a) a cannula having a longitudinal bore defining a first axis,
- b) a stylet having an outer diameter adapted to be received within the longitudinal bore and a distal tip adapted to penetrate cortical bone, and
- c) a first probe comprising:
 - d) an outer diameter adapted to be received within the longitudinal bore, and
 - i) a first electrode, and
 - ii) a lead in electrical connection with the first electrode.

Now referring to FIGS. **20a** and **20b**, in some embodiments, first **701** and second **751** cannulae are each provided with a curved bore **703**, **753** in their respective distal portions **705**, **755**, wherein each bore has a proximal lateral opening **707**, **757**. The apparatus further comprises first and second probes **711**, **761**, each containing an electrode **713**, **763**. In some embodiments, the probe may sit in a distal region of the bore (as in FIG. **20a**) during advance of the cannula. Once the target tissue region is reached, then probes are moved proximally (by, for example, a pull wire—not shown) and exit the proximal lateral openings so that the inner faces **715**, **765** of the electrodes face other.

Therefore, in accordance with the present invention, there is provided an intraosseous nerve denervation system, comprising:

- a) a cannula having a longitudinal bore defining a first axis,
- b) a stylet having an outer diameter adapted to be received within the longitudinal bore and a distal tip adapted to penetrate cortical bone, and
- c) a first probe comprising:
 - i) an outer diameter adapted to be received within the longitudinal bore, and
 - ii) a first electrode, and
 - iii) a lead in electrical connection with the first electrode.

Now referring to FIGS. **21a** and **21b**, in some embodiments, at least one probe **801** comprises i) a distal portion **803** having an electrode **805** and ii) a proximal portion **807**, the distal portion being pivotally attached to the proximal portion by pivot **809**. In some embodiments, two probes having such pivotally attached electrodes are introduced through the cannulae in a first linear mode (shown in FIG. **21a**) to produce an angle θ between the electrodes. Next, the respective pivots are actuated (by for example, a pull wire—not shown) to produce the angled configuration shown in

FIG. **21b** which reduces the angle θ between the electrodes. Preferably, the pivoting brings the electrodes into a substantially parallel relation.

Therefore, in accordance with the present invention, there is provided intraosseous nerve denervation system comprising:

- a) a first probe having:
 - i) a distal portion having a first electrode,
 - ii) a proximal portion comprising a first lead in electrical connection with the first electrode, and
 - iii) a pivot pivotally connecting the proximal and distal portions of the probe.

In some embodiments, relatively even heating is provided by providing current density gradients. Now referring to FIG. **22**, in some embodiments, first **821** and second **831** probes have first **823** and second **833** electrodes having a reverse conical shape. In particular, each electrode has a relatively thick distal portion **827**, **837** and a relatively thin proximal portion **825**, **835**. When this probe is activated, it is believed that the current density of this electrode will vary axially, with a relatively high current density present at the proximal portion of each electrode (due to the smaller surface area) and a relatively low current density present at the distal portion of the electrode (due to the larger surface area). This current density gradient should provide a more even heating zone when the electrodes themselves are oriented at a significant angle, as the preference for tip heating (caused by the angled orientation of the electrodes) is substantially balanced by the higher current density at the proximal portions of the electrodes.

Therefore, in accordance with the present invention, there is provided an intraosseous nerve denervation system comprising:

- a) a first probe having a first electrode and a first lead in electrical connection with the first electrode, wherein the first electrode has a proximal end having a proximal diameter and a distal end having a distal diameter, and wherein the proximal end diameter is less than the distal end diameter.

Current density gradients can also be produced by providing a plurality of electrodes on each probe. Now referring to FIG. **23**, in some embodiments, first and second electrodes each have a plurality of electrodes. In particular, first probe **851** has first **853**, second **854** and third **855** active electrodes, while second probe **861** has first **863**, second **864** and third **865** return electrodes. The voltage across the probes can be selected so that there is increasing voltage (and therefore current) across the more widely spaced electrodes (i.e., $V_{855-865} < V_{854-864} < V_{853-863}$). In some embodiments, the probes of FIG. **23** are driven by multiple voltage sources (i.e., a first voltage source for providing voltage between first active electrode **853** and first return electrode **863**, etc.).

Therefore, in accordance with the present invention, there is provided a method of therapeutically treating a vertebral body having a BVN, comprising the steps of:

- a) providing a first energy device having distal and proximal active electrodes,
- b) providing a second energy device having distal and proximal return electrodes,
- c) placing the first and second energy devices in the vertebral body to define a first distance between the distal active electrode and the distal return electrode, and a second distance between the proximal active electrode and the proximal return electrode, wherein the first distance is less than the second distance,

15

- d) applying a first high frequency voltage between the distal active and distal return electrodes, and
 applying a second high frequency voltage between the proximal active and proximal return electrodes, wherein the first high frequency voltage is less than the second high frequency voltage.

Because multiple voltage sources may add complexity to the device, in other embodiments, the differences in voltage may be provided by a single voltage source by using a poorly conductive electrode. In particular, in some embodiments thereof, the probe comprises an electrically conductive probe shaft and a plurality of spaced apart insulating jackets wherein the spacing produces the electrodes of FIG. 23. In this jacketed embodiment, the probe shaft can be made of a material that is a relatively poor electrical conductor (such as tantalum) so that, when a single driving force is applied between the jacketed probes, the voltage is highest at the proximal electrode 853, but loss due to the poor conductance produces a substantially lower voltage at distal electrode 855. This jacketed embodiment eliminates the need for multiple voltage sources.

In another dual probe approach, in some embodiments, and now referring to FIG. 24, there is provided an apparatus having first probe 871 having an active electrode 873, and a second 881 probe having a return electrode 883, wherein the ratio of the surface area of the active electrode to the surface area of the return electrode is very high, i.e., at least 2:1 (more preferably at least 5:1). In this condition, the current density will be very high at the active electrode and very low at the return electrode, so that the total heating zone THZ will occur essentially only around the active electrode. Since this device heats essentially only at the active electrode, this device substantially mimics the heating profile of a monopolar electrode, but provides the desirable safety feature of locally directing the current to the return electrode.

Therefore, in accordance with the present invention, there is provided an intraosseous nerve denervation system comprising:

- a) a first probe having:
 - i) an active electrode having a first surface area, and
 - ii) a first lead in electrical connection with the first electrode,
- b) a second probe having:
 - i) a return electrode having a first surface area, and
 - ii) a second lead in electrical connection with the second electrode,

wherein the first surface area is at least two times greater than the second surface area, and, means for creating first and second bores within a bone for accommodating the first and second probes.

Although the dual probe approach has many benefits, in other embodiments of the present invention, an articulated probe having both active and return electrodes may be used in accordance with the present invention.

Now referring to FIG. 25, there is provided a preferred articulated device according to the present invention. In preferred embodiments, this device 900 comprises a fixed probe 901 and a pivotable probe 951.

Fixed probe 901 comprises a shaft 903 having a longitudinal axis and a distal end portion 905 comprising sharpened distal tip 906 and a proximal end portion 907. Disposed near the distal end portion of the probe is first electrode 909. The fixed probe is designed so that the first electrode is placed in electrical connection with a first lead of a power supply. In this particular embodiment, the shaft has a longitudinal bore 911 running from the proximal end portion up to at least the first electrode. Disposed within the bore is a first wire (not

16

shown) electrically connected at its first end to the first electrode and having a second end adapted to be electrically connected to a first lead of a power supply (not shown). The fixed probe also comprises a recess 927 forming a lateral opening in the shaft and designed to house the pivotable probe when in its undeployed mode.

Pivotable probe 951 comprises a shaft 953 having a longitudinal axis, a distal end portion 955, and a proximal end portion 957 pivotally attached to the fixed probe by pivot 961. The pivot allows the pivoting probe to pivot about the fixed probe. Disposed near the distal end portion of the pivotable probe is second electrode 963. The probe is designed so that the second electrode is placed in electrical connection with a second lead of the power supply.

The pivotable probe has an undeployed mode and a deployed mode. In the un-deployed mode, the pivotable probe is seated within the recess of the fixed probe so that the axis of its shaft is essentially in line with the axis of the fixed probe shaft. In this state, the pivotable probe essentially hides within the fixed probe. In the deployed mode, the pivotable probe extends at a significant angle from the fixed probe so that the axis of its shaft forms an angle of at least 10 degrees with the axis of the fixed probe shaft.

In some embodiments, a pusher rod is used to deploy the pivotable probe. Pusher rod 975 comprises a proximal handle (not shown) for gripping and a distal end portion 977 having a shape for accessing the bore of the fixed probe. Distal end portion has a tip 981 having a shape which, when advanced distally, can push the distal end portion of the pivotable probe laterally out of the recess.

Therefore, in accordance with the present invention, there is provided a device for denervating an ION in a bone, comprising:

- a) a fixed probe having a first electrode thereon in electrical connection with the powder supply, and
- b) a pivotable probe comprising a second electrode having a proximal portion pivotally engaged to the fixed probe.

In some embodiments, the pivotable device has both an active and a return electrode, and the device is introduced through a single pedicle. The location of these electrodes may vary depending upon the use of the pivotable device. For example, when the active electrode is located on the pivotable probe, the return electrode may be positioned in a location selected from the group consisting of:

- a) a location on the fixed probe distal of the pivot (as in FIG. 25);
- b) a location on the fixed probe proximal of the pivot;
- c) a location on the pivotable probe located nearer the pivot; and
- d) a location on the pusher rod.

In other embodiments, the locations of the active and return electrodes are reversed from those described above.

In general, it is desirable to operate the present invention in a manner that produces a peak temperature in the target tissue of between about 80° C. and 95° C. When the peak temperature is below 80° C., the off-peak temperatures may quickly fall below about 45° C. When the peak temperature is above about 95° C., the bone tissue exposed to that peak temperature may experience necrosis and produce charring. This charring reduces the electrical conductivity of the charred tissue, thereby making it more difficult to pass RF current through the target tissue beyond the char and to resistively heat the target tissue beyond the char. In some embodiments, the peak temperature is preferably between 86° C. and 94° C.

It is desirable to heat the volume of target tissue to a minimum temperature of at least 42° C. When the tissue

experiences a temperature above 42° C., nerves within the target tissue may be desirably damaged. However, it is believed that denervation is a function of the total quantum of energy delivered to the target tissue, i.e., both exposure temperature and exposure time determine the total dose of energy delivered. Accordingly, if the temperature of the target tissue reaches only about 42° C., then it is believed that the exposure time of the volume of target tissue to that temperature should be at least about 30 minutes and preferably at least 60 minutes in order to deliver the dose of energy believed necessary to denervate the nerves within the target tissue.

Preferably, it is desirable to heat the volume of target tissue to a minimum temperature of at least 50° C. If the temperature of the target tissue reaches about 50° C., then it is believed that the exposure time of the volume of target tissue to that temperature need only be in the range of about 2 minutes to 10 minutes to achieve denervation.

More preferably, it is desirable to heat the volume of target tissue to a minimum temperature of at least 60° C. If the temperature of the target tissue reaches about 60° C., then it is believed that the exposure time of the volume of target tissue to that temperature need only be in the range of about 0.01 minutes to 1.5 minutes to achieve denervation, preferably 0.1 minutes to 0.25 minutes.

Typically, the period of time that an ION is exposed to therapeutic temperatures is in general related to the length of time in which the electrodes are activated. However, since it has been observed that the total heating zone remains relatively hot even after power has been turned off (and the electric field eliminated), the exposure time can include a period of time in which current is not running through the electrodes.

In general, the farther apart the electrodes, the greater the likelihood that the ION will be contained within the total heating zone. Therefore, in some embodiments, the electrodes are placed at least 5 mm apart, more preferably at least 10 mm apart. However, if the electrodes are spaced too far apart, the electric field takes on an undesirably extreme dumbbell shape. Therefore, in many preferred embodiments, the electrodes are placed apart a distance of between 5 mm and 25 mm, more preferably between 5 mm and 15 mm, more preferably between 10 mm and 15 mm.

In some embodiments, it is desirable to heat the target tissue so that at least about 1 cc of bone tissue experiences the minimum temperature. This volume corresponds to a sphere having a radius of about 0.6 cm. Alternatively stated, it is desirable to heat the target tissue so the minimum temperature is achieved by every portion of the bone within 0.6 cm of the point experiencing the peak temperature.

More preferably, it is desirable to heat the target tissue so that at least about 3 cc of bone experiences the minimum temperature. This volume corresponds to a sphere having a radius of about 1 cm.

In one preferred embodiment, the present invention provides a steady-state heated zone having a peak temperature of between 80° C. and 95° C. (and preferably between 86° C. and 94° C.), and heats at least 1 cc of bone (and preferably at least 3 cc of bone) to a temperature of at least 50° C. (and preferably 60° C.).

Therefore, in accordance with the present invention, there is provided a method of therapeutically treating a vertebral body having a BVN, comprising the steps of:

- a) providing an energy device having an active and a return electrode,
- a) inserting the active electrode into the vertebral body,
- b) inserting the return electrode into the vertebral body, and

- c) applying a sufficiently high frequency voltage difference between the active and return electrodes to generate a current therebetween to produce a total heating zone having a diameter of at least 0.5 cm and a steady state temperature of at least 50° C.

As noted above, a peak temperature below about 100° C. is desirable in order to prevent charring of the adjacent tissue, steam formation and tissue popping. In some embodiments, this is accomplished by providing the power supply with a feedback means that allows the peak temperature within the heating zone to be maintained at a desired target temperature, such as 90° C. In some embodiments, between about 24 watts and 30 watts of power is first supplied to the device in order to rapidly heat the relatively cool bone, with maximum amperage being obtained within about 10-15 seconds. As the bone is further heated to the target temperature, the feedback means gradually reduces the power input to the device to between about 6-10 watts.

If the active electrode has no active cooling means, it may become be subject to conductive heating by the heated tissue, and the resultant increased temperature in the electrode may adversely affect performance by charring the adjacent bone tissue. Accordingly, in some embodiments, a cool tip active electrode may be employed. The cooled electrode helps maintain the temperature of the electrode at a desired temperature. Cooled tip active electrodes are known in the art. Alternatively, the power supply may be designed to provided a pulsed energy input. It has been found that pulsing the current favorably allows heat to dissipate from the electrode tip, and so the active electrode stays relatively cooler.

The following section relates to the general structure of preferred energy devices in accordance with the present invention:

The apparatus according to the present invention comprises an electrosurgical probe having a shaft with a proximal end, a distal end, and at least one active electrode at or near the distal end. A connector is provided at or near the proximal end of the shaft for electrically coupling the active electrode to a high frequency voltage source. In some embodiments, a return electrode coupled to the voltage source is spaced a sufficient distance from the active electrode to substantially avoid or minimize current shorting therebetween. The return electrode may be provided integral with the shaft of the probe or it may be separate from the shaft.

In preferred embodiments, the electrosurgical probe or catheter will comprise a shaft or a handpiece having a proximal end and a distal end which supports one or more electrode terminal(s). The shaft or handpiece may assume a wide variety of configurations, with the primary purpose being to mechanically support the active electrode and permit the treating physician to manipulate the electrode from a proximal end of the shaft. The shaft may be rigid or flexible, with flexible shafts optionally being combined with a generally rigid external tube for mechanical support. Flexible shafts may be combined with pull wires, shape memory actuators, and other known mechanisms for effecting selective deflection of the distal end of the shaft to facilitate positioning of the electrode array. The shaft will usually include a plurality of wires or other conductive elements running axially therethrough to permit connection of the electrode array to a connector at the proximal end of the shaft.

Preferably, the shaft may be a rigid needle that is introduced through a percutaneous penetration in the patient. However, for endoscopic procedures within the spine, the

shaft will have a suitable diameter and length to allow the surgeon to reach the target site (e.g., a disc) by delivering the shaft through the thoracic cavity, the abdomen or the like. Thus, the shaft will usually have a length in the range of about 5.0 to 30.0 cm, and a diameter in the range of about 0.2 mm to about 10 mm. In any of these embodiments, the shaft may also be introduced through rigid or flexible endoscopes.

The probe will include one or more active electrode(s) for applying electrical energy to tissues within the spine. The probe may include one or more return electrode(s), or the return electrode may be positioned on the patient's back, as a dispersive pad. In either embodiment, sufficient electrical energy is applied through the probe to the active electrode(s) to either necrose the blood supply or nerves within the vertebral body.

The electrosurgical instrument may also be a catheter that is delivered percutaneously and/or endoluminally into the patient by insertion through a conventional or specialized guide catheter, or the invention may include a catheter having an active electrode or electrode array integral with its distal end. The catheter shaft may be rigid or flexible, with flexible shafts optionally being combined with a generally rigid external tube for mechanical support. Flexible shafts may be combined with pull wires, shape memory actuators, and other known mechanisms for effecting selective deflection of the distal end of the shaft to facilitate positioning of the electrode or electrode array. The catheter shaft will usually include a plurality of wires or other conductive elements running axially therethrough to permit connection of the electrode or electrode array and the return electrode to a connector at the proximal end of the catheter shaft. The catheter shaft may include a guide wire for guiding the catheter to the target site, or the catheter may comprise a steerable guide catheter. The catheter may also include a substantially rigid distal end portion to increase the torque control of the distal end portion as the catheter is advanced further into the patient's body. Specific deployment means will be described in detail in connection with the figures hereinafter.

In some embodiments, the electrically conductive wires may run freely inside the catheter bore in an unconstrained made, or within multiple lumens within the catheter bore.

The tip region of the instrument may comprise many independent electrode terminals designed to deliver electrical energy in the vicinity of the tip. The selective application of electrical energy is achieved by connecting each individual electrode terminal and the return electrode to a power source having independently controlled or current limited channels. The return electrode(s) may comprise a single tubular member of conductive material proximal to the electrode array. Alternatively, the instrument may comprise an array of return electrodes at the distal tip of the instrument (together with the active electrodes) to maintain the electric current at the tip. The application of high frequency voltage between the return electrode(s) and the electrode array results in the generation of high electric field intensities at the distal tips of the electrode terminals with conduction of high frequency current from each individual electrode terminal to the return electrode. The current flow from each individual electrode terminal to the return electrode(s) is controlled by either active or passive means, or a combination thereof, to deliver electrical energy to the surrounding conductive fluid while minimizing energy delivery to surrounding (non-target) tissue.

Temperature probes associated with the apparatus may preferably be disposed on or within the electrode carrier;

between the electrodes (preferred in bipolar embodiments); or within the electrodes (preferred for monopolar embodiments). In some embodiments wherein the electrodes are placed on either side of the ION, a temperature probe is disposed between the electrodes or in the electrodes. In alternate embodiments, the deployable portion of the temperature probe comprises a memory metal.

The electrode terminal(s) are preferably supported within or by an inorganic insulating support positioned near the distal end of the instrument shaft. The return electrode may be located on the instrument shaft, on another instrument or on the external surface of the patient (i.e., a dispersive pad). The close proximity of the dual needle design to the intra-osseous nerve makes a bipolar design more preferable because this minimizes the current flow through non-target tissue and surrounding nerves. Accordingly, the return electrode is preferably either integrated with the instrument body, or another instrument located in close proximity thereto. The proximal end of the instrument(s) will include the appropriate electrical connections for coupling the return electrode(s) and the electrode terminal(s) to a high frequency power supply, such as an electrosurgical generator.

In some embodiments, the active electrode(s) have an active portion or surface with surface geometries shaped to promote the electric field intensity and associated current density along the leading edges of the electrodes. Suitable surface geometries may be obtained by creating electrode shapes that include preferential sharp edges, or by creating asperities or other surface roughness on the active surface(s) of the electrodes. Electrode shapes according to the present invention can include the use of formed wire (e.g., by drawing round wire through a shaping die) to form electrodes with a variety of cross-sectional shapes, such as square, rectangular, L or V shaped, or the like. Electrode edges may also be created by removing a portion of the elongate metal electrode to reshape the cross-section. For example, material can be ground along the length of a round or hollow wire electrode to form D or C shaped wires, respectively, with edges facing in the cutting direction. Alternatively, material can be removed at closely spaced intervals along the electrode length to form transverse grooves, slots, threads or the like along the electrodes. In other embodiments, the probe can be sectored so that a given circumference comprises an electrode region and an inactive region. In some embodiments, the inactive region is masked.

The return electrode is typically spaced proximally from the active electrode(s) a suitable. In most of the embodiments described herein, the distal edge of the exposed surface of the return electrode is spaced about 5 to 25 mm from the proximal edge of the exposed surface of the active electrode(s), in dual needle insertions. Of course, this distance may vary with different voltage ranges, the electrode geometry and depend on the proximity of tissue structures to active and return electrodes. The return electrode will typically have an exposed length in the range of about 1 to 20 mm.

The application of a high frequency voltage between the return electrode(s) and the electrode terminal(s) for appropriate time intervals effects modifying the target tissue.

The present invention may use a single active electrode terminal or an array of electrode terminals spaced around the distal surface of a catheter or probe. In the latter embodiment, the electrode array usually includes a plurality of independently current-limited and/or power-controlled electrode terminals to apply electrical energy selectively to the target tissue while limiting the unwanted application of electrical energy to the surrounding tissue and environment

resulting from power dissipation into surrounding electrically conductive fluids, such as blood, normal saline, and the like. The electrode terminals may be independently current-limited by isolating the terminals from each other and connecting each terminal to a separate power source that is isolated from the other electrode terminals. Alternatively, the electrode terminals may be connected to each other at either the proximal or distal ends of the catheter to form a single wire that couples to a power source.

In one configuration, each individual electrode terminal in the electrode array is electrically insulated from all other electrode terminals in the array within said instrument and is connected to a power source which is isolated from each of the other electrode terminals in the array or to circuitry which limits or interrupts current flow to the electrode terminal when low resistivity material (e.g., blood) causes a lower impedance path between the return electrode and the individual electrode terminal. The isolated power sources for each individual electrode terminal may be separate power supply circuits having internal impedance characteristics which limit power to the associated electrode terminal when a low impedance return path is encountered. By way of example, the isolated power source may be a user selectable constant current source. In this embodiment, lower impedance paths will automatically result in lower resistive heating levels since the heating is proportional to the square of the operating current times the impedance. Alternatively, a single power source may be connected to each of the electrode terminals through independently actuable switches, or by independent current limiting elements, such as inductors, capacitors, resistors and/or combinations thereof. The current limiting elements may be provided in the instrument, connectors, cable, controller or along the conductive path from the controller to the distal tip of the instrument. Alternatively, the resistance and/or capacitance may occur on the surface of the active electrode terminal(s) due to oxide layers which form selected electrode terminals (e.g., titanium or a resistive coating on the surface of metal, such as platinum).

In a preferred aspect of the invention, the active electrode comprises an electrode array having a plurality of electrically isolated electrode terminals disposed over a contact surface, which may be a planar or non-planar surface and which may be located at the distal tip or over a lateral surface of the shaft, or over both the tip and lateral surface(s). The electrode array will include at least two and preferably more electrode terminals, and may further comprise a temperature sensor. In a preferred aspect, each electrode terminal will be connected to the proximal connector by an electrically isolated conductor disposed within the shaft. The conductors permit independent electrical coupling of the electrode terminals to a high frequency power supply and control system with optional temperature monitor for operation of the probe. The control system preferably incorporate active and/or passive current limiting structures, which are designed to limit current flow when the associated electrode terminal is in contact with a low resistance return path back to the return electrode.

The use of such electrode arrays in electrosurgical procedures is particularly advantageous as it has been found to limit the depth of tissue necrosis without substantially reducing power delivery. The voltage applied to each electrode terminal causes electrical energy to be imparted to any body structure which is contacted by, or comes into close proximity with, the electrode terminal, where a current flow through all low electrical impedance paths is preferably but not necessarily limited. Since some of the needles are

hollow, a conductive fluid could be added through the needle and into the bone structure for the purposes of lowering the electrical impedance and fill the spaces in the cancellous bone to make them better conductors to the needle.

It should be clearly understood that the invention is not limited to electrically isolated electrode terminals, or even to a plurality of electrode terminals. For example, the array of active electrode terminals may be connected to a single lead that extends through the catheter shaft to a power source of high frequency current. Alternatively, the instrument may incorporate a single electrode that extends directly through the catheter shaft or is connected to a single lead that extends to the power source. The active electrode(s) may have ball shapes, twizzle shapes, spring shapes, twisted metal shapes, cone shapes, annular or solid tube shapes or the like. Alternatively, the electrode(s) may comprise a plurality of filaments, rigid or flexible brush electrode(s), side-effect brush electrode(s) on a lateral surface of the shaft, coiled electrode(s) or the like.

The voltage difference applied between the return electrode(s) and the electrode terminal(s) will be at high or radio frequency, typically between about 50 kHz and 20 MHz, usually being between about 100 kHz and 2.5 MHz, preferably being between about 400 kHz and 1000 kHz, often less than 600 kHz, and often between about 500 kHz and 600 kHz. The RMS (root mean square) voltage applied will usually be in the range from about 5 volts to 1000 volts, preferably being in the range from about 10 volts to 200 volts, often between about 20 to 100 volts depending on the electrode terminal size, the operating frequency and the operation mode of the particular procedure. Lower peak-to-peak voltages will be used for tissue coagulation, thermal heating of tissue, or collagen contraction and will typically be in the range from 50 to 1500, preferably 100 to 1000 and more preferably 120 to 400 volts peak-to-peak. As discussed above, the voltage is usually delivered continuously with a sufficiently high frequency (e.g., on the order of 50 kHz to 20 MHz) (as compared with e.g., lasers claiming small depths of necrosis, which are generally pulsed about 10 to 20 Hz). In addition, the sine wave duty cycle (i.e., cumulative time in any one-second interval that energy is applied) is preferably on the order of about 100% for the present invention, as compared with pulsed lasers which typically have a duty cycle of about 0.0001%.

The preferred power source of the present invention delivers a high frequency current selectable to generate average power levels ranging from several milliwatts to tens of watts per electrode, depending on the volume of target tissue being heated, and/or the maximum allowed temperature selected for the instrument tip. The power source allows the user to select the power level according to the specific requirements of a particular procedure.

The power source may be current limited or otherwise controlled so that undesired heating of the target tissue or surrounding (non-target) tissue does not occur. In a presently preferred embodiment of the present invention, current limiting inductors are placed in series with each independent electrode terminal, where the inductance of the inductor is in the range of 10 uH to 50,000 uH, depending on the electrical properties of the target tissue, the desired tissue heating rate and the operating frequency. Alternatively, capacitor-inductor (LC) circuit structures may be employed, as described previously in U.S. Pat. No. 5,697,909. Additionally, current limiting resistors may be selected. Preferably, microprocessors are employed to monitor the measured current and control the output to limit the current.

The area of the tissue treatment surface can vary widely, and the tissue treatment surface can assume a variety of geometries, with particular areas and geometries being selected for specific applications. The geometries can be planar, concave, convex, hemispherical, conical, linear “in-line” array or virtually any other regular or irregular shape. Most commonly, the active electrode(s) or electrode terminal(s) will be formed at the distal tip of the electrosurgical instrument shaft, frequently being planar, disk-shaped, or hemispherical surfaces for use in reshaping procedures or being linear arrays for use in cutting. Alternatively or additionally, the active electrode(s) may be formed on lateral surfaces of the electrosurgical instrument shaft (e.g., in the manner of a spatula), facilitating access to certain body structures in endoscopic procedures.

The devices of the present invention may be suitably used for insertion into any hard tissue in the human body. In some embodiments, the hard tissue is bone. In other embodiments, the hard tissue is cartilage. In preferred embodiments when bone is selected as the tissue of choice, the bone is a vertebral body. Preferably, the present invention is adapted to puncture the hard cortical shell of the bone and penetrate at least a portion of the underlying cancellous bone. In some embodiments, the probe advances into the bone to a distance of at least $\frac{1}{3}$ of the cross-section of the bone defined by the advance of the probe. In some embodiments, the present invention is practiced in vertebral bodies substantially free of tumors. In others, the present invention is practiced in vertebral bodies having tumors.

Therefore, in accordance with the present invention, there is provided a method of therapeutically treating a healthy vertebral body having a BVN, comprising the steps of:

- a) providing an energy device having an active and a return electrode,
- b) inserting the active electrode into the healthy vertebral body,
- c) inserting the return electrode into the healthy vertebral body,
- d) placing the active electrode on a first side of the healthy vertebral body and the return electrode on a second side of the healthy vertebral body, and

applying a sufficiently high frequency voltage difference between the active and return electrodes to generate a current therebetween to produce a total heating zone to therapeutically heat the BVN.

In some embodiments using two separate probes, the device of the present invention enters the hard tissue (preferably bone, more preferably the vertebral body) through two access points. In preferred embodiments, the pair of separate probes is adapted to denervate the BVN and enter through separate pedicles transpedicularly. In other embodiments, the pair of separate probes each enters the vertebral body extrapedicularly. In other embodiments, a first of the pair of separate probes enters the vertebral body extrapedicularly and the second enters the vertebral body transpedicularly. In embodiments using a single articulated device, the device enters via a single pedicle.

Now referring to FIG. 26, in some embodiments, the target region of the BVN is located within the cancellous portion of the bone (i.e., to the interior of the outer cortical bone region), and proximal to the junction J of the BVN having a plurality of branches. Treatment in this region is advantageous because only a single portion of the BVN need be effectively treated to denervate the entire system. In contrast, treatment of the BVN in locations more downstream than the junction require the denervation of each branch.

Therefore, in accordance with the present invention, there is provided a method of therapeutically treating a vertebral body having an outer cortical bone region and an inner cancellous bone region, and a BVN having a trunk extending from the outer cortical bone region into the inner cancellous region and a branches extending from the trunk to define a BVN junction, comprising the steps of:

- a) inserting an energy device into the vertebral body, and
- b) exclusively depositing energy within the inner cancellous bone region of the vertebral body between, but exclusive of the BVN junction and the outer cortical bone region, to denervate the BVN.

Typically, treatment in accordance with this embodiment can be effectuated by placing the electrodes in the region of the vertebral body located between 60% (point A) and 90% (point B) of the distance between the anterior and posterior ends of the vertebral body, as shown in FIG. 26.

EXAMPLE I

This prophetic example describes a preferred dual probe embodiment of the present invention.

First, after induction of an appropriate amount of a local anesthesia, the human patient is placed in a prone position on the table. The C-arm of an X-ray apparatus is positioned so that the X-rays are perpendicular to the axis of the spine. This positioning provides a lateral view of the vertebral body, thereby allowing the surgeon to view the access of the apparatus into the vertebral body.

Next, a cannulated stylet comprising an inner stylet and an outer cannula are inserted into the skin above each of the respective pedicles so that the distal tip of each stylet is in close proximity to the respective pedicle.

Next, the probe is advanced interiorly into the body so that the stylet tips bores through the skin, into and through the pedicle, and then into the vertebral body. The stylet is advanced until the tips reach the anterior-posterior midline of the vertebral body.

Next, the stylet is withdrawn and probe is inserted into the cannula and advanced until the first and second electrodes thereof each reach the midline of the vertebral body. The location of the two probes is shown from various perspectives in FIG. 27a-d.

Next, the power supply is activated to provide a voltage between the first and second electrodes. The amount of voltage across the electrodes is sufficient to produce an electric current between the first and second electrodes. This current provides resistive heating of the tissue disposed between the electrodes in an amount sufficient to raise the temperature of the local portion of the BVN to at least 45° C., thereby denervating the BVN.

EXAMPLE II

This example describes the efficacy of heating a large zone of a vertebral body with a bipolar energy device.

A pair of probes were inserted into a vertebral body of a porcine cadaver so that the tips of the electrodes were located substantially at the midline and separated by about 4 mm. Each electrode had a cylindrical shape, a length of about 20 mm, and a diameter of about 1.65 mm² (16 gauge) to produce a surface area of about 100 mm².

Next, and now referring to FIGS. 28a and 28b, thermocouples 0-14 were placed within the vertebral body at the 15 locations. Thermocouples 0-4 were placed halfway between the electrode tips and were separated by a distance of 2 mm. Thermocouples 5-9 were placed about at the midpoint

25

between the probe tips, and were vertically separated by a distance of 2 mm. Thermocouples 10-14 were placed along the distal portion of the probe and were separated by a distance of 5 mm.

Next, about 57 volts of energy was applied across the electrodes, and the temperature rise in the tissue was recorded at the thermocouple sites. These temperatures are provided in FIGS. 29a-c. In general, the temperature at each site rose somewhat steadily from about 22° C. to its peak temperature in about 200-300 seconds, whereupon feedback controls maintained the peak temperatures.

FIGS. 30a and 30b provide the peak temperatures recorded by each thermocouple. Analysis of the results in FIGS. 17a and 17b reveals that peak temperatures of between about 80° C. and 95° C. were able to be sustained over substantial distances. In particular, a temperature of 79.4 degrees was reached about 10 mm along the electrode (T11); temperatures of between 76.7 and 80.3° C. were reached at a depth of about 4 mm within the tissue (T5 and T9); and a temperature of 76.8° C. was reached about 10 mm along the electrode (T3).

The positive results provided by this example has great significance to the problem of therapeutically heating IONs, and the BVN in particular. In particular, the results of thermocouples T5-9 indicates that if an ION were located along the z-axis within 2 mm of the presumed center of the IRZ, then the ION could be sufficiently treated to at least 80° C. Similarly, the results of thermocouples T0-4 indicates that as much as a 16 mm length of ION could be sufficiently treated to at least 80° C. Lastly, the results of thermocouples T 10-14 indicate that the ION could be off-center laterally in the IRZ by as much as 2 mm and at least about 10 mm of its length could be sufficiently treated to at least 80 C.

EXAMPLE III

This embodiment describes a preferred articulated probe embodiment of the present invention.

The initial steps described above in Example I are carried out so that the articulated probe is poised on the patient's skin and held in place by a ratchet type gun. See FIG. 31a.

Next, the distal end of the articulated probe is inserted into the skin above a pedicle so that the distal end of the fixed probe is in close proximity, to the pedicle.

Now referring to FIG. 31b, the probe is advanced interiorly into the body so that the distal tip bores through the skin, into and through the pedicle, and then into the vertebral body. The distal tip is advanced until it reaches about 30% beyond the anterior-posterior midline of the vertebral body.

Now referring to FIG. 31c, the distal end of the pusher rod is inserted into the bore of the fixed probe and advanced until the angled portion of the pusher rod contacts the angled portion of the pivotable probe, thereby nudging the pivotable probe out of the recess. The pivotable probe is now in a partially deployed mode.

Now referring to FIG. 31d, the apparatus is slightly withdrawn from the body. As this occurs, the bone disposed between the pivotable and fixed probes prevents the pivotable probe from withdrawing along with the fixed probe, but rather forces open the pivoting means, thereby bringing the axis of the pivotable probe to a position substantially normal to the axis of the fixed probe. The pivotable probe is now in extended mode.

Next, the power supply is activated to provide a voltage between the first and second electrodes. The amount of voltage across the electrodes is sufficient to produce an electric current between the first and second electrodes. This

26

current provides resistive heating of the tissue disposed between the electrodes in an amount sufficient to raise the temperature of the local portion of the BVN to at least 45° C., thereby denervating the BVN.

Next, the fixed probe is pushed forward to bring the pivotable probe back into the recess.

Now referring to FIGS. 31e, the probe is removed from the body.

EXAMPLE IV

Now referring to FIG. 32, there is provided a dual articulated needle embodiment of the present invention, wherein the articulated needles are each advanced down the pedicles of the vertebral body, and each of the pivotable probes are deployed at an angle of less than 90 degrees, so that the electrodes thereon align themselves in an essentially parallel relationship. Because the electric field produced by this embodiment is relatively even between the electrodes, the resulting total heating zone is also desirably homogeneous. Because the electrodes deploy in the central posterior portion of the vertebral body, the BVN is desirably denervated near its trunk.

We claim:

1. A method of therapeutically treating a vertebral body having an outer cortical bone region, an inner cancellous bone region, and a basivertebral nerve BVN, comprising the steps of:

providing a probe [configured to deploy an energy device] having [an] *a first* electrode;

the probe comprising a longitudinal bore extending from a proximal end of the probe toward a distal end of the probe;

the probe comprising a recess in communication with said bore, said recess forming a lateral opening at or near the distal end of the probe;

the probe further comprising a pivotable member; the pivotable member having a fixed end pivotably secured to the probe at a distal location within the recess of the probe, [and] a free end configured to be seated in said recess, *and a second electrode*;

wherein the pivotable member comprises an undeployed mode where the free end extends proximally from the fixed end within said recess, and a deployed mode where the free end is configured to pivot about said fixed end and extend outward from said probe;

articulating the pivotable member from the undeployed mode to the deployed mode to facilitate delivery of the [energy device] *second electrode* along a path associated with the free end of the pivotable member into the cancellous bone region of the vertebral body; and

applying a sufficiently high frequency voltage [to] *difference between the first electrode and the second electrode to generate a current therebetween to therapeutically heat the BVN.*

2. A method as recited in claim 1, the BVN having a trunk extending from the outer cortical bone region and into the inner cancellous bone region and branches extending from the trunk to define a BVN junction, wherein therapeutically heating the BVN comprises:

depositing therapeutic energy within the inner cancellous bone region of the vertebral body.

3. The method of claim 2, wherein the therapeutic energy is deposited in a region of the vertebral body located between 60% and 90% of the distance between the posterior and anterior ends of the vertebral body.

4. The method of claim 3, wherein said therapeutic energy is deposited in a region of the vertebral body located between 60% and 90% of the distance from the anterior wall to the posterior wall of the vertebral body.

5. The method of claim 2, wherein said therapeutic energy deposited includes a region that is proximal of the BVN junction.

6. The method of claim 2, wherein said therapeutic energy is deposited within a region that is at least 1 cm in diameter.

7. The method of claim 2, wherein said therapeutic energy deposited comprises a steady-state heated zone having a peak temperature of between 80 degrees C. and 95 degrees C.

8. The method of claim 7, wherein said steady-state heated zone heats at least 1 cc of bone to a temperature of at least 50 degrees C.

9. The method of claim 2, wherein the method is performed to treat pain in a patient diagnosed with pain.

10. The method of claim 1, wherein the method is performed to treat pain in a patient diagnosed with pain.

11. The method of claim 1, wherein the pivotable member in the undeployed mode is entirely contained within said recess.

12. The method of claim 1, wherein articulating the pivotable member from the undeployed mode to the deployed mode comprises advancing a member distally along said bore to push the free end of the of the pivotable member laterally out the recess.

13. The method of claim 1, wherein the free end of the pivotable member deploys pivotably outward from the recess into the cancellous bone region.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : RE46,356 E
APPLICATION NO. : 13/541591
DATED : April 4, 2017
INVENTOR(S) : Pellegrino et al.

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Specification

Please insert Line 11 (approx.) of Column 1 as follows:

--Notice: More than one reissue application has been filed for the reissue of U.S. Patent No. 7,749,218. The reissue applications are U.S. Reissue Patent Application Serial No. 15/469,315, filed on March 24, 2017, which is a divisional reissue application of U.S. Reissue Patent Application Serial No. 13/541,591 (the present application), filed on July 3, 2012, now U.S. Reissue Patent No. RE46,356 E, issued April 4, 2017.--

Signed and Sealed this
Twelfth Day of June, 2018

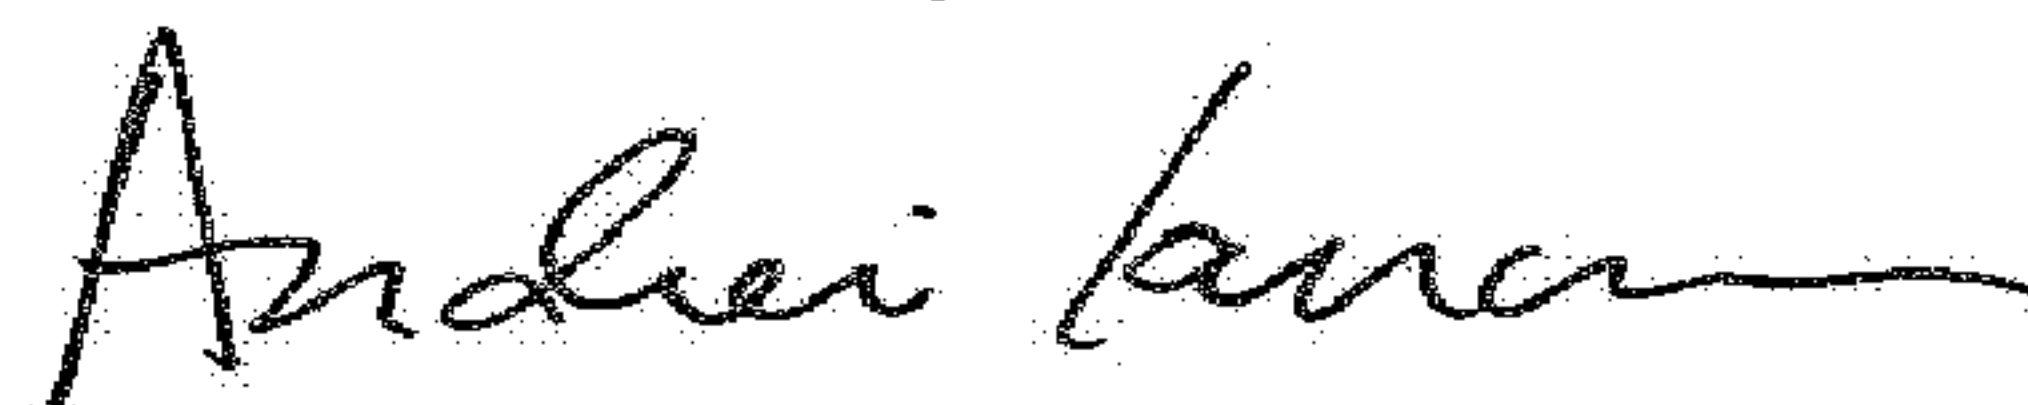

Andrei Iancu
Director of the United States Patent and Trademark Office