



US00RE46562E

(19) **United States**
(12) **Reissued Patent**
Huennekens et al.

(10) **Patent Number: US RE46,562 E**
(45) **Date of Reissued Patent: Oct. 3, 2017**

(54) **VASCULAR IMAGE CO-REGISTRATION**

(71) Applicant: **Volcano Corporation**, San Diego, CA (US)

(72) Inventors: **R. Scott Huennekens**, San Diego, CA (US); **Stephen M. Fry**, El Dorado Hills, CA (US); **Blair D. Walker**, Mission Viejo, CA (US); **Jon D. Klingensmith**, El Dorado Hills, CA (US); **Nancy Perry Pool**, El Dorado Hills, CA (US); **Vincent J. Burgess**, San Diego, CA (US); **William R. Kanz**, Sacramento, CA (US)

(73) Assignee: **Volcano Corporation**, San Diego, CA (US)

(21) Appl. No.: **14/727,617**

(22) Filed: **Jun. 1, 2015**

Related U.S. Patent Documents

Reissue of:

(64) Patent No.: **7,930,014**
Issued: **Apr. 19, 2011**
Appl. No.: **11/329,609**
Filed: **Jan. 11, 2006**

U.S. Applications:

(63) Continuation of application No. 13/865,803, filed on Apr. 18, 2013, now Pat. No. Re. 45,534, which is an application for the reissue of Pat. No. 7,930,014.

(Continued)

(51) **Int. Cl.**

A61B 5/05 (2006.01)
A61B 5/06 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 5/06** (2013.01); **A61B 6/4494** (2013.01); **A61B 6/463** (2013.01); **A61B 6/487** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC **A61B 6/504**; **A61B 6/5247**; **A61B 8/12**;
A61B 6/463; **A61B 8/463**; **A61B 8/543**;
A61B 6/4494

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,173,228 A 11/1979 Van Steenwyk
4,821,731 A 4/1989 Martinelli

(Continued)

FOREIGN PATENT DOCUMENTS

CA 2 449 080 5/2005
JP 01-204650 8/1989

(Continued)

OTHER PUBLICATIONS

Dorland's Medical Dictionary, www.mercksource.com/pp/us/cns/cns.sub.-h1.sub.-Split.jsp-?pg=/ppdocs/us/co44755mmon/dorlands/dorland/one/000005012.htm.


(Continued)

Primary Examiner — Jeffrey R Jastrzab

(57) **ABSTRACT**

A system and method for providing a vascular image are disclosed wherein a single composite display simultaneously provides a first view of a patient including an angiogram image and a second view including an intravascular image rendered from information provided by an imaging probe mounted on a distal end of a flexible elongate member. A cursor, having a position derived from image information provided by a radiopaque marker proximate the imaging probe, is displayed within the angiogram image to correlate the position of the imaging probe to a presently displayed intravascular image and thus provide an easily discernable identification of a position within a patient corresponding to a currently displayed intravascular image. The resulting composite display simultaneously provides: an intravascular image that includes information about a vessel that is not

(Continued)

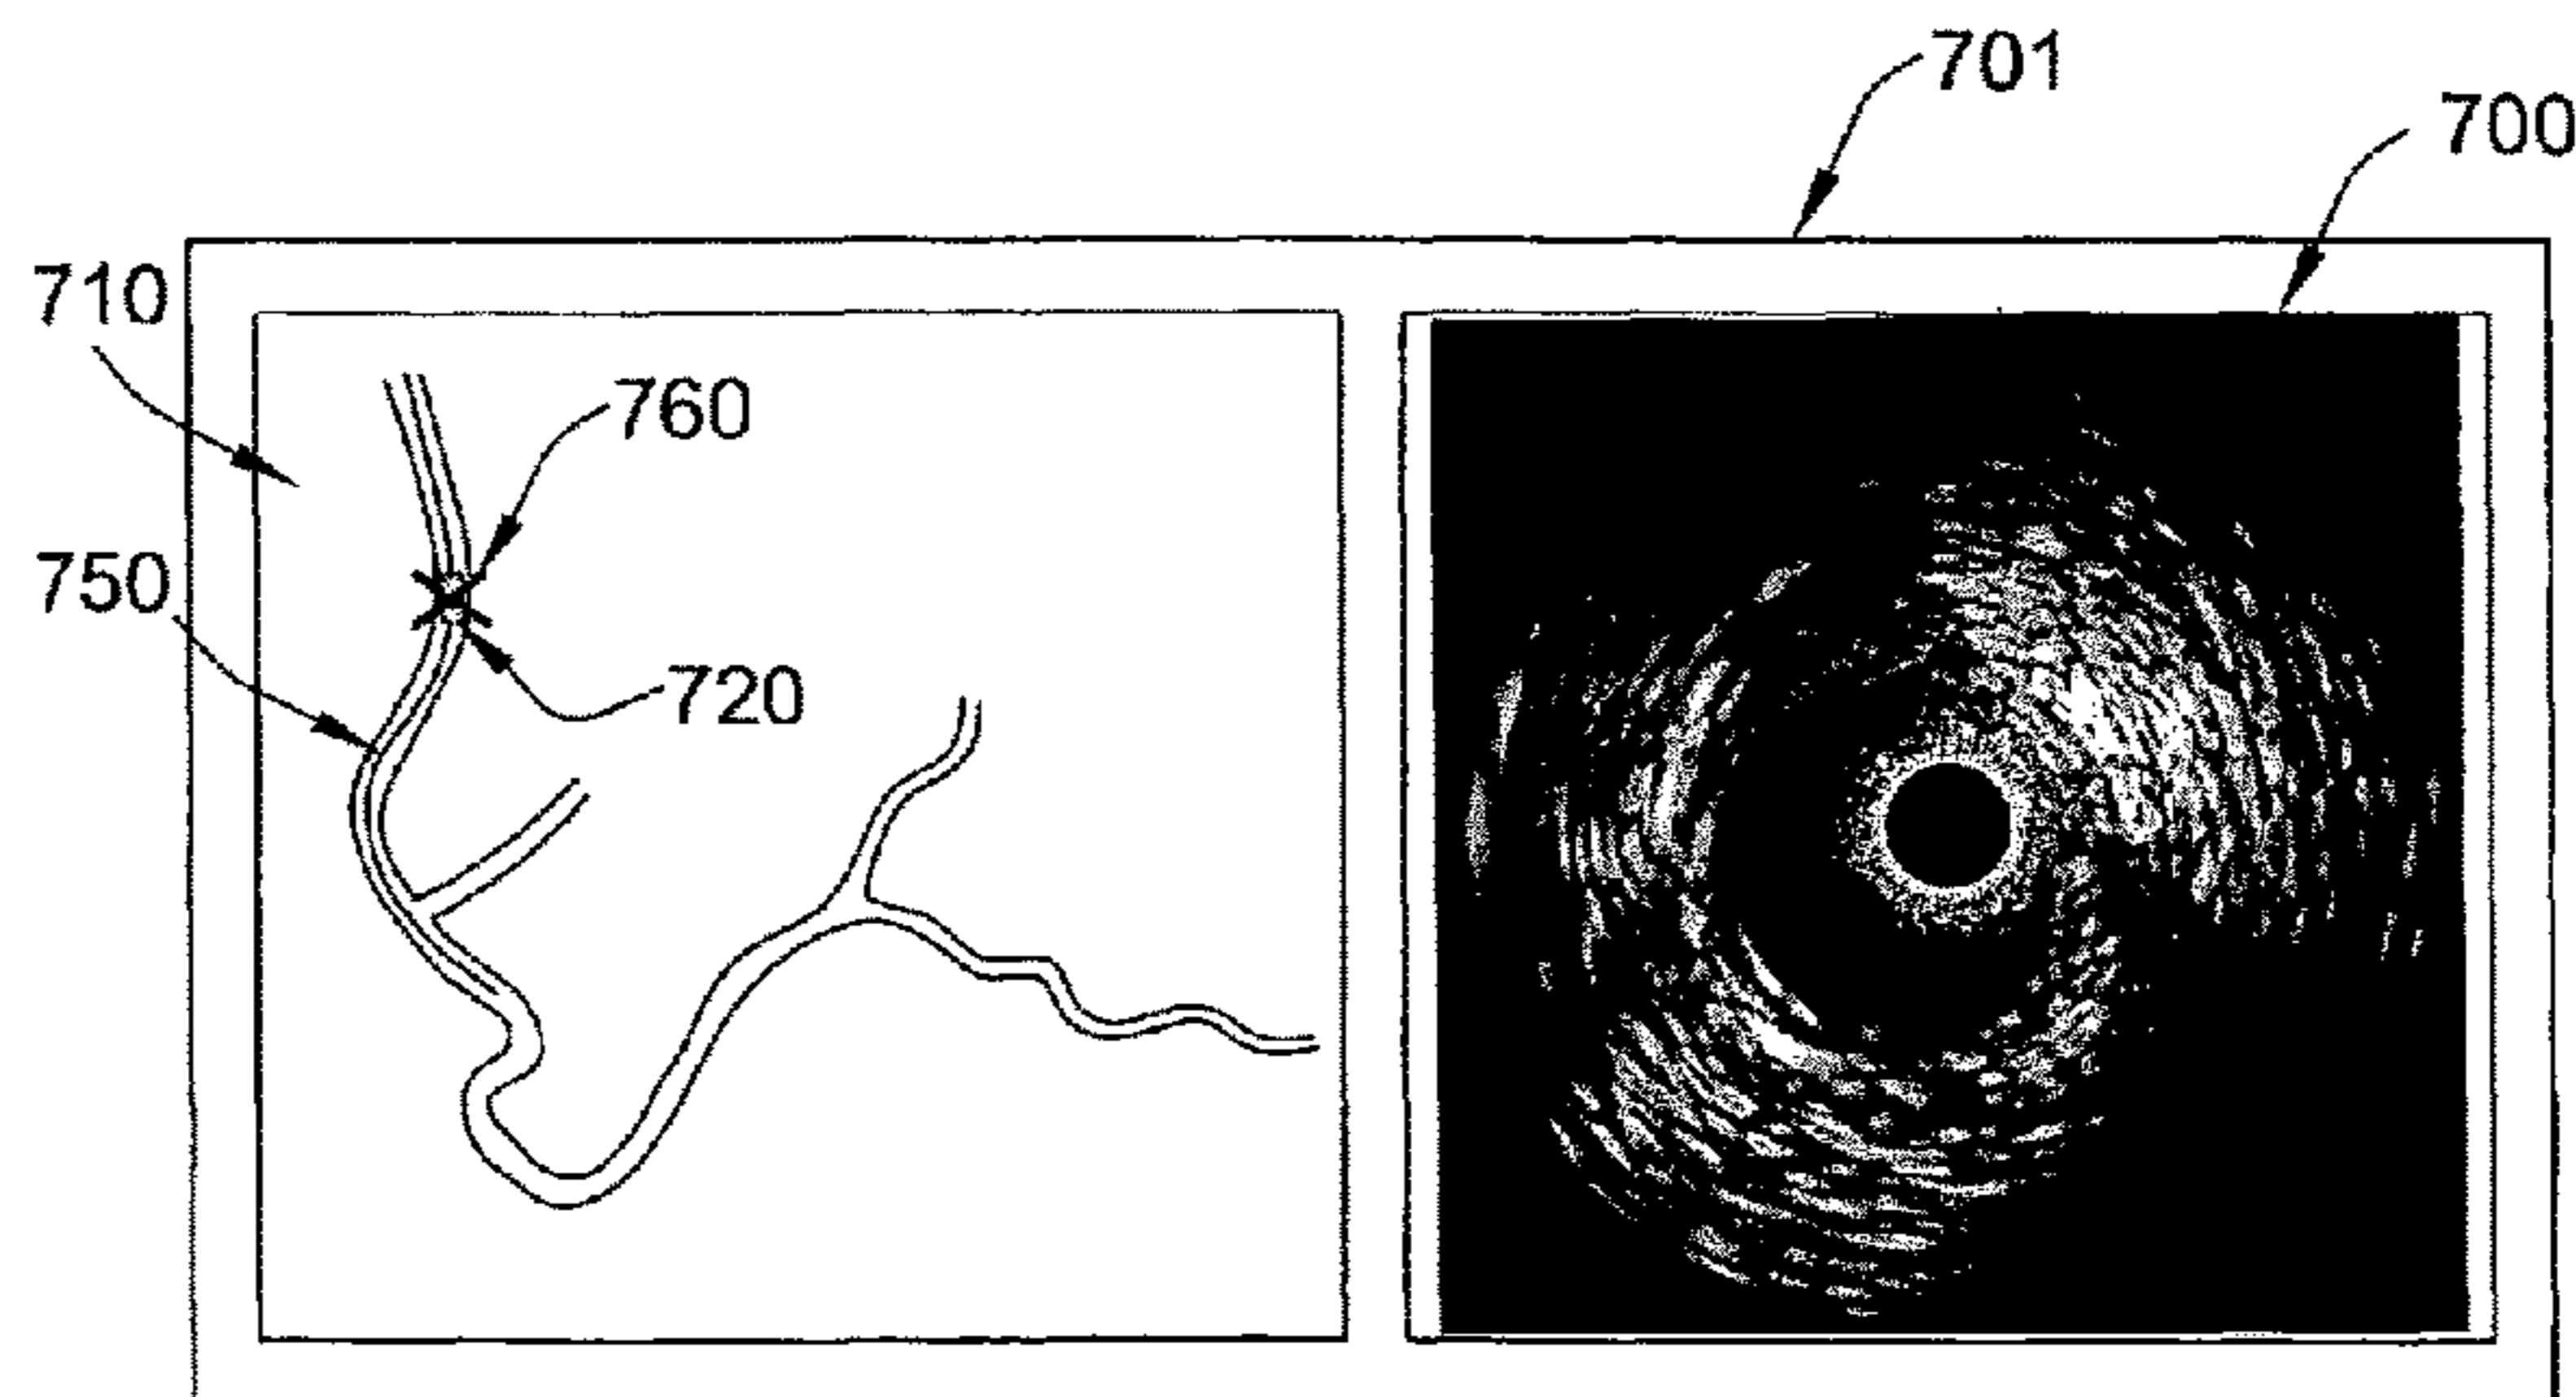

US RE46,562 E

available from an angiogram and a current location within a vessel of a source of intravascular image data from which the intravascular image is rendered.

18 Claims, 9 Drawing Sheets

Related U.S. Application Data

(60) Provisional application No. 60/642,893, filed on Jan. 11, 2005, provisional application No. 60/694,014, filed on Jun. 24, 2005.

(51) **Int. Cl.**

A61B 6/00 (2006.01)
A61B 8/12 (2006.01)
A61B 8/00 (2006.01)
A61B 34/20 (2016.01)
A61B 5/0215 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 6/504* (2013.01); *A61B 6/5247* (2013.01); *A61B 8/12* (2013.01); *A61B 8/463* (2013.01); *A61B 8/543* (2013.01); *A61B 34/20* (2016.02); *A61B 5/0215* (2013.01); *A61B 6/4441* (2013.01); *A61B 8/4494* (2013.01)

(58) **Field of Classification Search**

USPC 600/407, 424, 425, 426, 427, 437, 453, 600/454, 455, 462, 466, 467, 473, 476; 382/159, 165, 170, 181

See application file for complete search history.

(56)

References Cited

U.S. PATENT DOCUMENTS

4,838,879	A	6/1989	Tanabe
4,875,165	A	10/1989	Fencil
4,938,220	A	7/1990	Mueller, Jr.
5,042,486	A	8/1991	Pfeiler
5,109,859	A	5/1992	Jenkins
5,159,931	A	11/1992	Pini
5,203,777	A	4/1993	Lee
5,207,226	A *	5/1993	Bailin et al. 600/454
5,357,550	A *	10/1994	Asahina et al. A61B 6/481 378/98.2
5,386,828	A	2/1995	Owens
5,429,617	A	7/1995	Hammersmark
5,485,840	A	1/1996	Bauman
5,540,229	A	7/1996	Coliet-Billon
5,592,939	A	1/1997	Martinelli
5,619,995	A *	4/1997	Lobodzinski H04N 9/8042 348/77
5,690,113	A	11/1997	Sliwa, Jr.
5,699,446	A	12/1997	Rougee
5,699,805	A *	12/1997	Seward et al. 600/459
5,709,206	A	1/1998	Teboul
5,729,129	A	3/1998	Acker
5,744,953	A	4/1998	Hansen
5,752,513	A	5/1998	Acker
5,771,895	A	6/1998	Slager
5,824,042	A	10/1998	Lombardi
5,830,145	A	11/1998	Tenhoff
5,840,025	A	11/1998	Ben-Haim
5,872,861	A	2/1999	Makram-Ebeid
5,876,344	A	3/1999	Baker et al.
5,899,860	A	5/1999	Pfeiffer
5,921,978	A	7/1999	Thompson
5,954,647	A	9/1999	Bova
5,957,844	A	9/1999	Dekel
5,993,390	A	11/1999	Savord
6,014,473	A	1/2000	Hossack
6,016,439	A	1/2000	Acker

6,024,763	A	2/2000	Lenker
6,035,226	A	3/2000	Panescu
6,036,682	A	3/2000	Lange
6,083,167	A	7/2000	Fox
6,095,976	A	8/2000	Nachtomy
6,102,865	A	8/2000	Hossack
6,104,944	A	8/2000	Martinelli
6,132,376	A	10/2000	Hossack
6,148,095	A *	11/2000	Prause et al. 382/131
6,152,878	A	11/2000	Nachtomy
6,159,225	A	12/2000	Makower
6,166,740	A	12/2000	Malzbender
6,190,353	B1	2/2001	Makower
6,201,900	B1	3/2001	Hossack
6,216,029	B1	4/2001	Paltieli
6,233,476	B1	5/2001	Strommer
6,246,898	B1	6/2001	Vesely
6,248,075	B1	6/2001	McGee
6,273,858	B1 *	8/2001	Fox et al. 600/466
6,275,724	B1	8/2001	Dickinson
6,285,903	B1	9/2001	Rosenthal A61B 6/12 600/424
6,298,261	B1	10/2001	Rex
6,314,310	B1	11/2001	Ben-Haim
6,351,513	B1	2/2002	Bani-Hashemi
6,360,027	B1	3/2002	Hossack
6,374,134	B1	4/2002	Bladen
6,389,104	B1	5/2002	Bani-Hashemi
6,405,072	B1	6/2002	Cosman
6,464,645	B1 *	10/2002	Park et al. 600/462
6,471,656	B1 *	10/2002	Shalman A61B 5/0215 600/486
6,501,848	B1	12/2002	Carroll
6,515,657	B1	2/2003	Zanelli
6,546,271	B1	4/2003	Reisfeld
6,574,498	B1	6/2003	Gilboa
6,577,889	B2	6/2003	Ichihashi
6,612,992	B1	9/2003	Hossack
6,638,222	B2	10/2003	Chandrasekaran et al.
6,650,927	B1	11/2003	Keidar
6,673,018	B2	1/2004	Friedman
6,718,054	B1	4/2004	Lorigo
6,719,700	B1	4/2004	Willis
6,775,404	B1	8/2004	Pagoulatos
6,785,571	B2	8/2004	Glossap
6,805,132	B2	10/2004	Willis
6,831,644	B2	12/2004	Lienard
6,895,267	B2	5/2005	Panescu
6,896,657	B2	5/2005	Willis
6,923,768	B2	8/2005	Camus
6,970,733	B2	11/2005	Willis
6,970,734	B2	11/2005	Eidenschink
7,052,463	B2 *	5/2006	Peszynski et al. 600/459
2001/0041842	A1	11/2001	Eberle et al.
2002/0019644	A1	2/2002	Hastings
2002/0049375	A1	4/2002	Strommer
2002/0099428	A1	7/2002	Kaufman
2002/0115931	A1 *	8/2002	Strauss et al. A61B 5/06 600/420
2003/0163052	A1	8/2003	Mott et al.
2003/0220555	A1	11/2003	Heigl
2003/0231789	A1	12/2003	Willis
2004/0097805	A1	5/2004	Verard et al.
2004/0114146	A1	6/2004	Willis
2004/0138548	A1	7/2004	Strommer
2004/0236206	A1 *	11/2004	Sakas A61B 8/00 600/407
2004/0254463	A1 *	12/2004	Lehman 600/437
2005/0096647	A1	5/2005	Steinke
2005/0113685	A1	5/2005	Maschke
2005/0203369	A1	9/2005	Sathyanarayana
2006/0036167	A1 *	2/2006	Shina 600/433

FOREIGN PATENT DOCUMENTS

JP	04-246340	9/1992
JP	HEI 5-084248	4/1993

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP HEI 10-137238 5/1998
 WO WO 2004/075756 9/2004
 WO WO 2004075756 A1 * 9/2004 A61B 6/481

OTHER PUBLICATIONS

Written Opinion of the International Searching Authority for PCT/US06/00942 dated Sep. 20, 2007.

No author, "Radiation Safety Manual for the Fluoroscopist," Internet source, 2000, Saint Luke's Hospital of Kansas City, Kansas City, U.S.A.

Evans, J., Ng, K., Wiet, S., Vonesh, M., Burns, W., Radvany, M., Kane, B., Davidson, C., Roth, S., Kramer, B., Meyers, S., McPherson, D., "Accurate Three-Dimensional Reconstruction of Intravascular Ultrasound Data", *Circulation*, 1996, pp. 567-576, vol. 93, No. 3, American Heart Association, Dallas, U.S.A.

Fencil, L., Doi, K., Hoffman, K., "Accurate Analysis of Blood Vessel Sizes and Stenotic Lesions Using Stereoscopic DSA System", *Investigative Radiology*, 1988, pp. 33-41, vol. 23, No. 1, Lippincott, Philadelphia, U.S.A.

Fujita, H., Doi, K., Fencil, L., Chia, K., "Image Feature Analysis and Computer-Aided Diagnosis in Digital Radiography. 2. Computerized Determination of Vessel Sizes in Digital Subtraction Angiography", *Medical Physics*, 1987, pp. 549-556, vol. 14, No. 4, American Institute of Physics, New York, U.S.A.

Guggenheim, N., Doriot, P., Dorsaz, P., Descouts, P., Rutishauser, W., "Spatial Reconstruction of Coronary Arteries from Angiographic Images", *Physics in Medicine and Biology*, 1991, pp. 99-110, vol. 36, No. 1, Institute of Physics, London, England.

Hoffmann, K., Sen, A., Lan, L., Chua, K., Esthappan, J., Mazzucco, M., "A System for Determination of 3D Vessel Tree Centerlines from Biplane Images", *The International Journal of Cardiac Imaging*, 2000, pp. 315-330, vol. 16, No. 5, Nijhoff, Boston, U.S.A.

Jiang, H., Chen, W., Wang, G., Liu, H., "Localization Error Analysis for Stereo X-ray Image Guidance with Probability Method", *Medical Engineering & Physics*, 2001, pp. 573-581, vol. 23, No. 8, Butterworth-Heinemann, Oxford, England.

Prause, G., DeJong, S., McKay, C., Sonka, M., "Accurate 3-D Reconstruction of Tortuous Coronary Vessels Using Biplane Angiography and Intravascular Ultrasound" in *SPIE Medical imaging 1997. Physiology and function from multidimensional images* : Feb. 23-25, 1997, Newport Beach, California, 1997, pp. 225-234, vol. 3033, Ed. Hofman, E., SPIE, Bellingham, U.S.A.

Prause, G., DeJong, S., McKay, C., Sonka, M., "Semi-Automated Segmentation and 3-D Reconstruction of Coronary Trees: Biplane Angiography and Intravascular Ultrasound Data Fusion" in *SPIE Medical imaging 1996. Physiology and function from multidimensional images* : Feb. 11-13, 1996, Newport Beach, California, 1996, pp. 82-92, vol. 2709, Ed. Hofman, E., SPIE, Bellingham, U.S.A.

Sherknie, D., Meunier, J., Mongrain, R., Tardif, J., "Three-Dimensional Trajectory Assessment of an IVUS Transducer from Single-Plane Cineangiograms: A Phantom Study", *IEEE Transactions on Biomedical Engineering*, 2005, pp. 543-548, vol. 52, No. 3, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Wahle, A., Prause, G., Von Birgelen, C., Erbel, R., Sonka, M., "Automated Calculation of the Axial Orientation of Intravascular Ultrasound Images by Fusion with Biplane Angiography" in *SPIE Medical imaging 1999. Image processing* Feb. 22-25, 1999, San Diego, California, 1999, pp. 1094-1104, vol. 3661, Ed. Hanson, K., SPIE, Bellingham, U.S.A.

Wahle, A., Mitchell, S., Ramaswamy, S., Chandran, K., Sonka, M., "Four-Dimensional Coronary Morphology and Computational Hemodynamics" in *SPIE Medical imaging 2001 : Image processing* : Feb. 19-22, 2001, San Diego, USA, 2001, pp. 743-754, vol. 4322, Eds. Sonka, M. and Hanson, K., SPIE, Bellingham, U.S.A.

Weichert, F., Wawro, M., Muller, H., Wilke, C., "Registration of Biplane Angiography and Intravascular Ultrasound for 3D Vessel

Reconstruction", *Methods of Information in Medicine*, 2004, pp. 398-402, vol. 43, No. 4, F.K. Schattauer, Stuttgart, Germany.

Japanese Patent Office, Office Action dated May 2, 2014 for Japanese Application No. 2013-015279, 3 pages. (translated).

Japan Patent Office, "Office Action" for Application No. 2014-223907, mailed Sep. 17, 2015, 3 pages (with translation).

The On-line Medical Dictionary, <http://cancerweb.ncl.ac.uk/cgi-bin/omd?angiogram>.*

MedTerms.com, <http://www.medterms.com/script/main/art.asp?articlekey=2256>.*

Dictionary of Cancer Terms, <http://www.cancer.gov/Templates/db.sub--alpha.aspx?CdrID=46530>.*

Medical Dictionary, The Fite Dictionary; <http://medical-dictionary.thefreedictionary.com/angiogram>.*

International Search Report for PCT/US06/00942 dated Sep. 20, 2007.

Cavaye, D., Tabbara, M., Kopchok, G., Laas, T., White, R., "Three Dimensional Vascular Ultrasound Imaging", *The American Surgeon*, 1991, pp. 751-755, vol. 57, No. 12, Lippincott, Philadelphia, U.S.A.

Chen, S., Metz, C., "Improved Determination of Biplane Imaging Geometry from Two Projection Images and Its Application to Three-Dimensional Reconstruction of Coronary Trees", *Medical Physics*, 1997, pp. 633-654, vol. 24, No. 5, American Institute of Physics, New York, U.S.A.

Chen, S., Carroll, J., "3-D Reconstruction of Coronary Arterial Tree to Optimize Angiographic Visualization", *IEEE Transactions on Medical Imaging*, 2000, pp. 318-336, vol. 19, No. 4, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Chen, S., Carroll, J., Messenger, J., "Quantitative Analysis of Reconstructed 3-D Coronary Arterial Tree and Intracoronary Devices", *IEEE Transactions on Medical Imaging*, 2002, pp. 724-740, vol. 21, No. 7, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Cothren, R., Shekhar, R., Tuzcu, E., Nissen, S., Cornhill, J., Vince, D., "Three-Dimensional Reconstruction of the Coronary Artery Wall by Image Fusion of Intravascular ultrasound and Bi-Plane Angiography", *International Journal of Cardiac Imaging*, 2000, pp. 69-85, vol. 16, No. 2, Nijhoff, Boston, U.S.A.

Falk, V., Mourgues, F., Adhami, L., Jacobs, S., Thiele, H., Nitzsche, S., Mohr, F., Coste-Maniere, E., "Cardio Navigation: Planning, Simulation, and Augmented Reality in Robotic Assisted Endoscopic Bypass Grafting", *The Annals of Thoracic Surgery*, 2005, pp. 2040-2048, vol. 79, No. 6, Little, Brown & Co., Boston, U.S.A.

Godbout, B., De Guise, J., Soulez, G., Cloutier, G., "3D Elastic Registration of Vessel Structures from IVUS data on Biplane Angiography", *Academic Radiology*, 2005, pp. 10-16, vol. 12, No. 1, Association of University Radiologists, Reston, U.S.A.

Legget, M., Leotta, D., Bolson, E., McDonald, J., Martin, R., Li, X., Otto, C., Sheehan, F., "System for Quantitative Three-Dimensional Echocardiography of the Left Ventricle Based on a Magnetic-Field Position and Orientation Sensing System", *IEEE Transactions on Biomedical Engineering*, 1998, pp. 494-504, vol. 45, No. 4, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Leotta, D., "An Efficient Calibration Method for Freehand 3-D Ultrasound Imaging Systems", *Ultrasound in Medicine & Biology*, 2004, pp. 999-1008, vol. 30, No. 7, Elsevier, New York, U.S.A.

Liu, I., Sun, Y., "Fully Automatic Reconstruction of Three-Dimensional Vascular Tree Structures from Two Orthogonal Views Using Computational Algorithms and Production Rules", *Optical Engineering*, 1992, pp. 2197-2207, vol. 31, No. 10, The Society of Photo-optical Instrumentation Engineers, Redondo Beach, U.S.A.

Meyer, S., Wolf, P., "Registration of Three-Dimensional Cardiac Catheter Models to Single-Plane Fluoroscopic Images", *IEEE Transactions on Biomedical Engineering*, 1999, pp. 1471-1479, vol. 46, No. 12, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Movassaghi, B., Grass, V., Viergever, M., Niessen, W., "A Quantitative Analysis of 3-D Coronary Modeling from Two or More Projection Images", *IEEE Transactions on Medical Imaging*, 2004, pp. 1517-1531, vol. 23, No. 12, Institute of Electrical and Electronics Engineers, New York, U.S.A.

(56)

References Cited

OTHER PUBLICATIONS

Rotger, D., Radeva, P., Mauri, J., Fernandez-Nofrerias, E., "Internal and External Coronary Vessel Images Registration" in *Topics in Artificial Intelligence*, 2002, pp. 408-418, Eds. Escrig Monferrer M. and Toledo Lobo, F., Springer-Verlag, Berlin, Germany.

Sheehan, H., Hodgson, J., "Intravascular Ultrasound: Advantages and Indications," *International Journal of Cardiac Imaging*, 1995, pp. 9-14, vol. 11, No. Suppl 1, Kluwer Academic Publishers, Boston, U.S.A.

Takemura, A., Harauchi, H., Suzuki, M., Hoffmann, K., Inamura, K., Umeda, T., "An Algorithm for Mapping the Catheter Tip Position on a Fluorograph to the Three-Dimensional Position in Magnetic Resonance Angiography Volume Data", *Physics in Medicine and Biology*, 2003, pp. 2697-2711, vol. 48, No. 16, Institute of Physics, London, England.

Van Walsum, T., Baert, S., Niessen, W., "Guide Wire Reconstruction and Visualization in 3DRA Using Monoplane Fluoroscopic Imag-

ing", *IEEE Transactions on Medical Imaging*, 2005, pp. 612-623, vol. 24, No. 5, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Wahle, A., Lopez, J., Pennington, E., Meeks, S., Braddy, K., Fox, J., Brennan, T., Buatti, J., Rossen, J., Sonka, M., "Effects of Vessel Geometry and Catheter Position on Dose Delivery in Intracoronary Brachytherapy", *IEEE Transactions on Biomedical Engineering*, 2003, pp. 1286-1295, vol. 50, No. 11, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Wahle, A., Olszewski, M., Sonka, M., "Interactive Virtual Endoscopy in Coronary Arteries Based on Multimodality Fusion", *IEEE Transactions on Medical Imaging*, 2004, pp. 1391-1403, vol. 23, No. 11, Institute of Electrical and Electronics Engineers, New York, U.S.A.

Weichert, F., Wawro, M., Wilke, C., "A 3D Computer Graphics Approach To Brachytherapy Planning", *The International Journal of Cardiovascular Imaging*, 2004, pp. 173-182, vol. 20, No. 3, Kluwer Academic Publishers, Boston, U.S.A.

* cited by examiner

FIG. 1

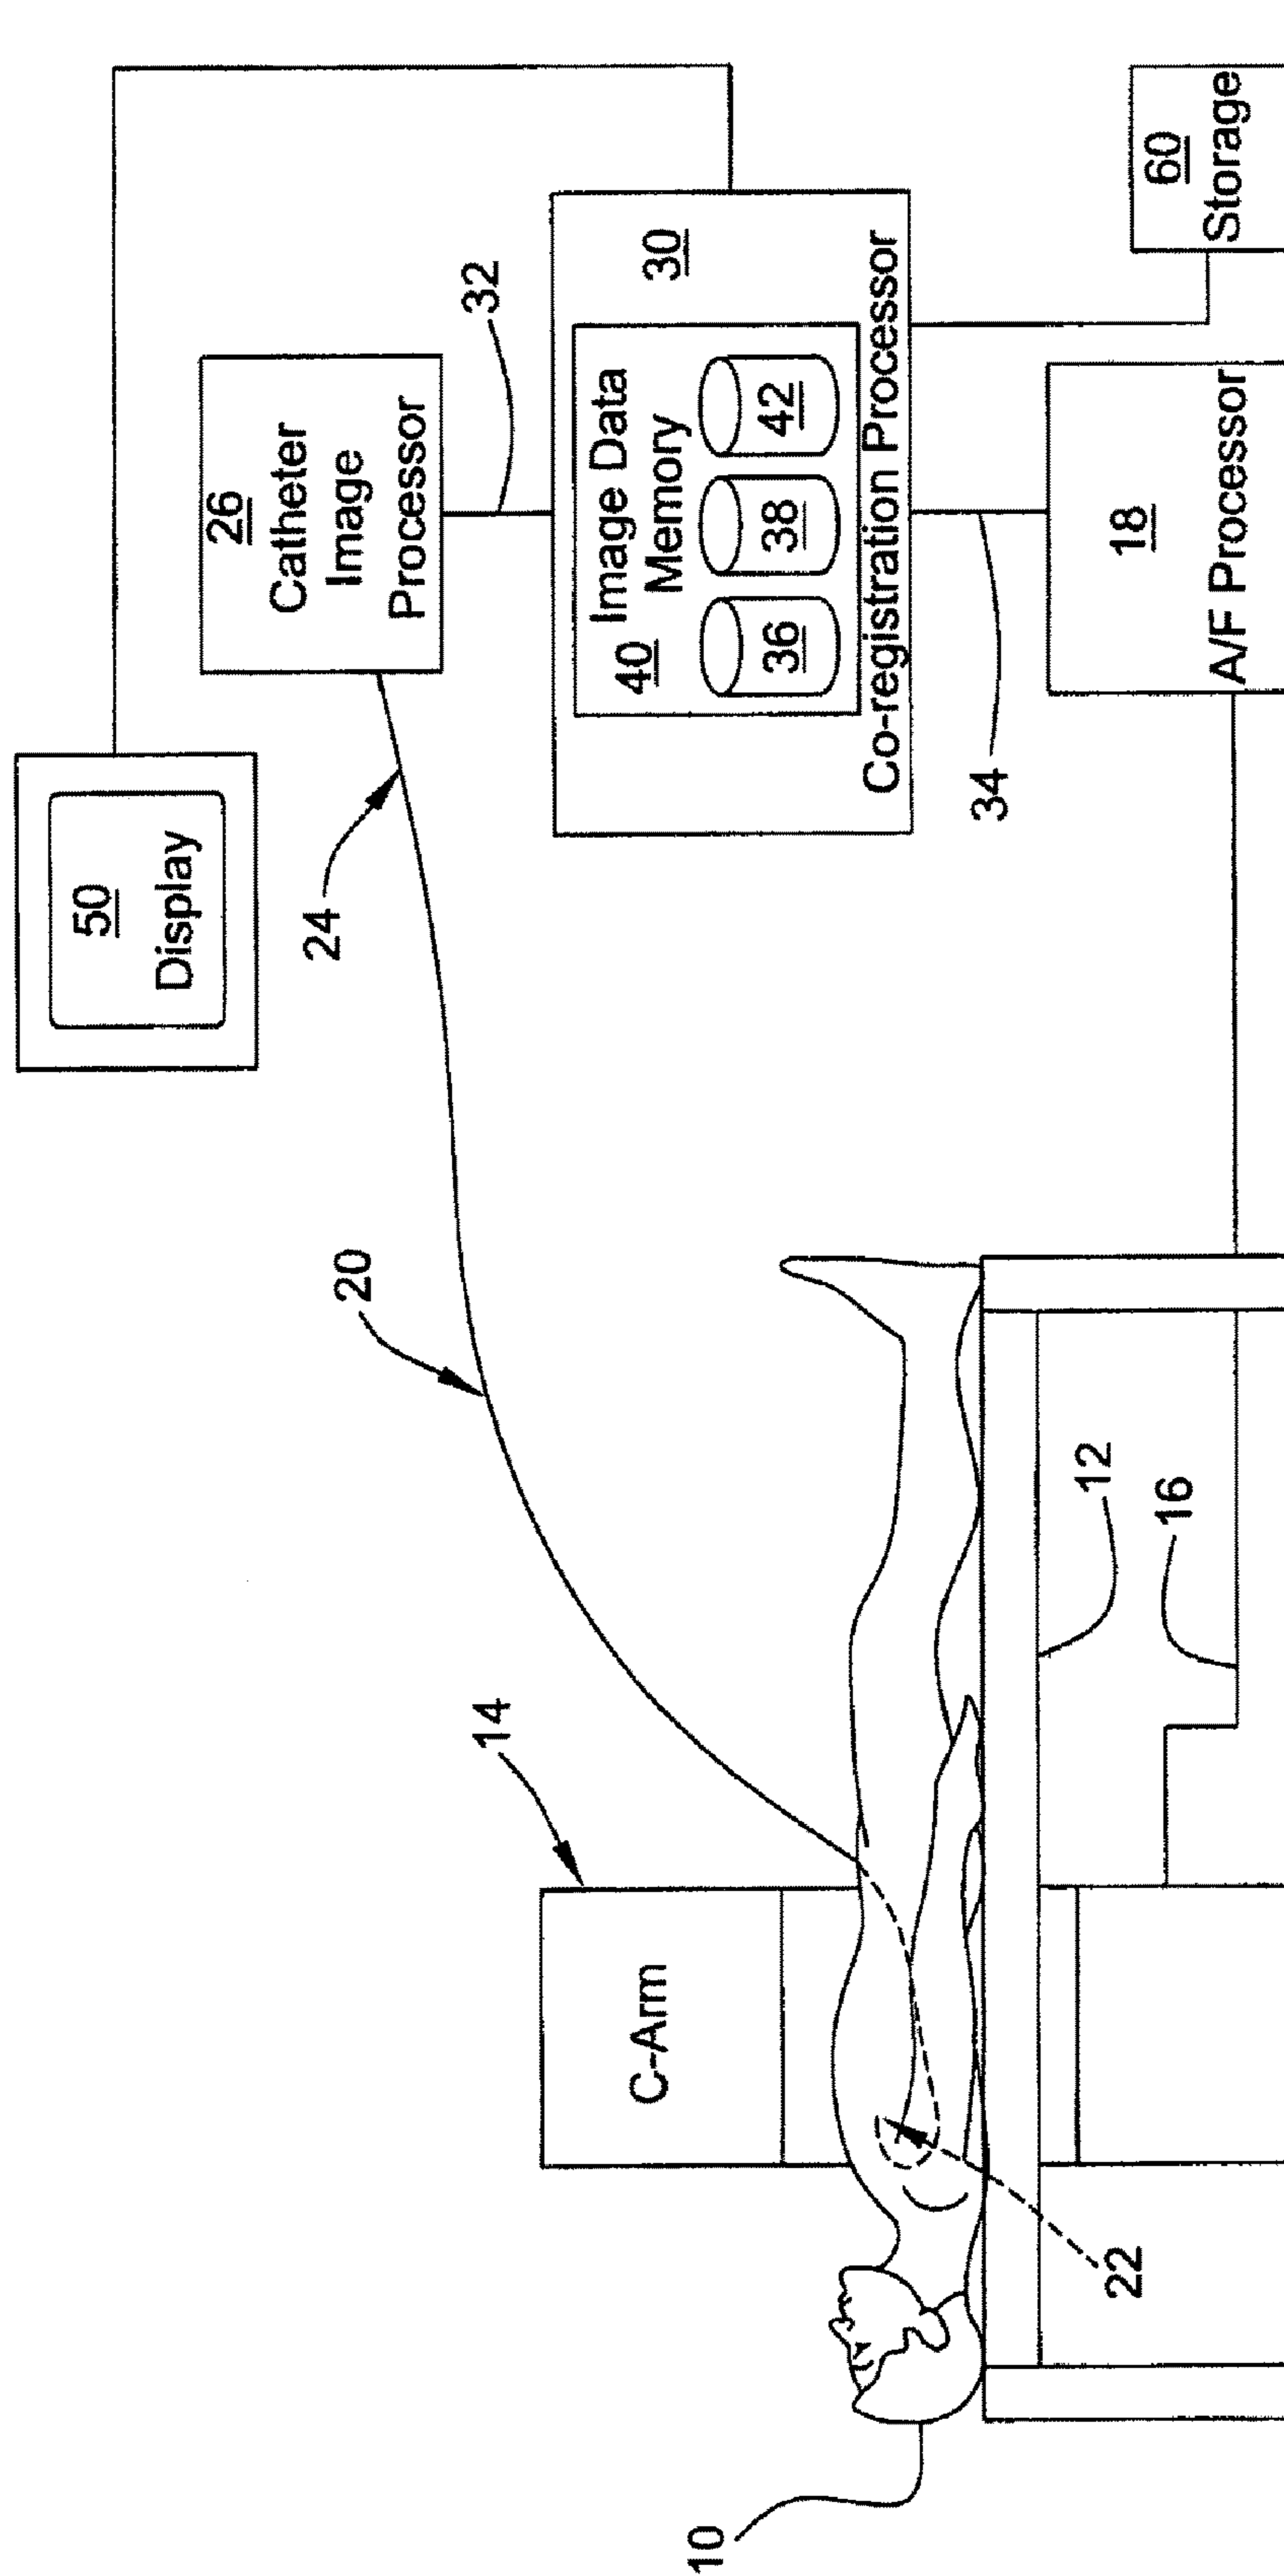


FIG. 2

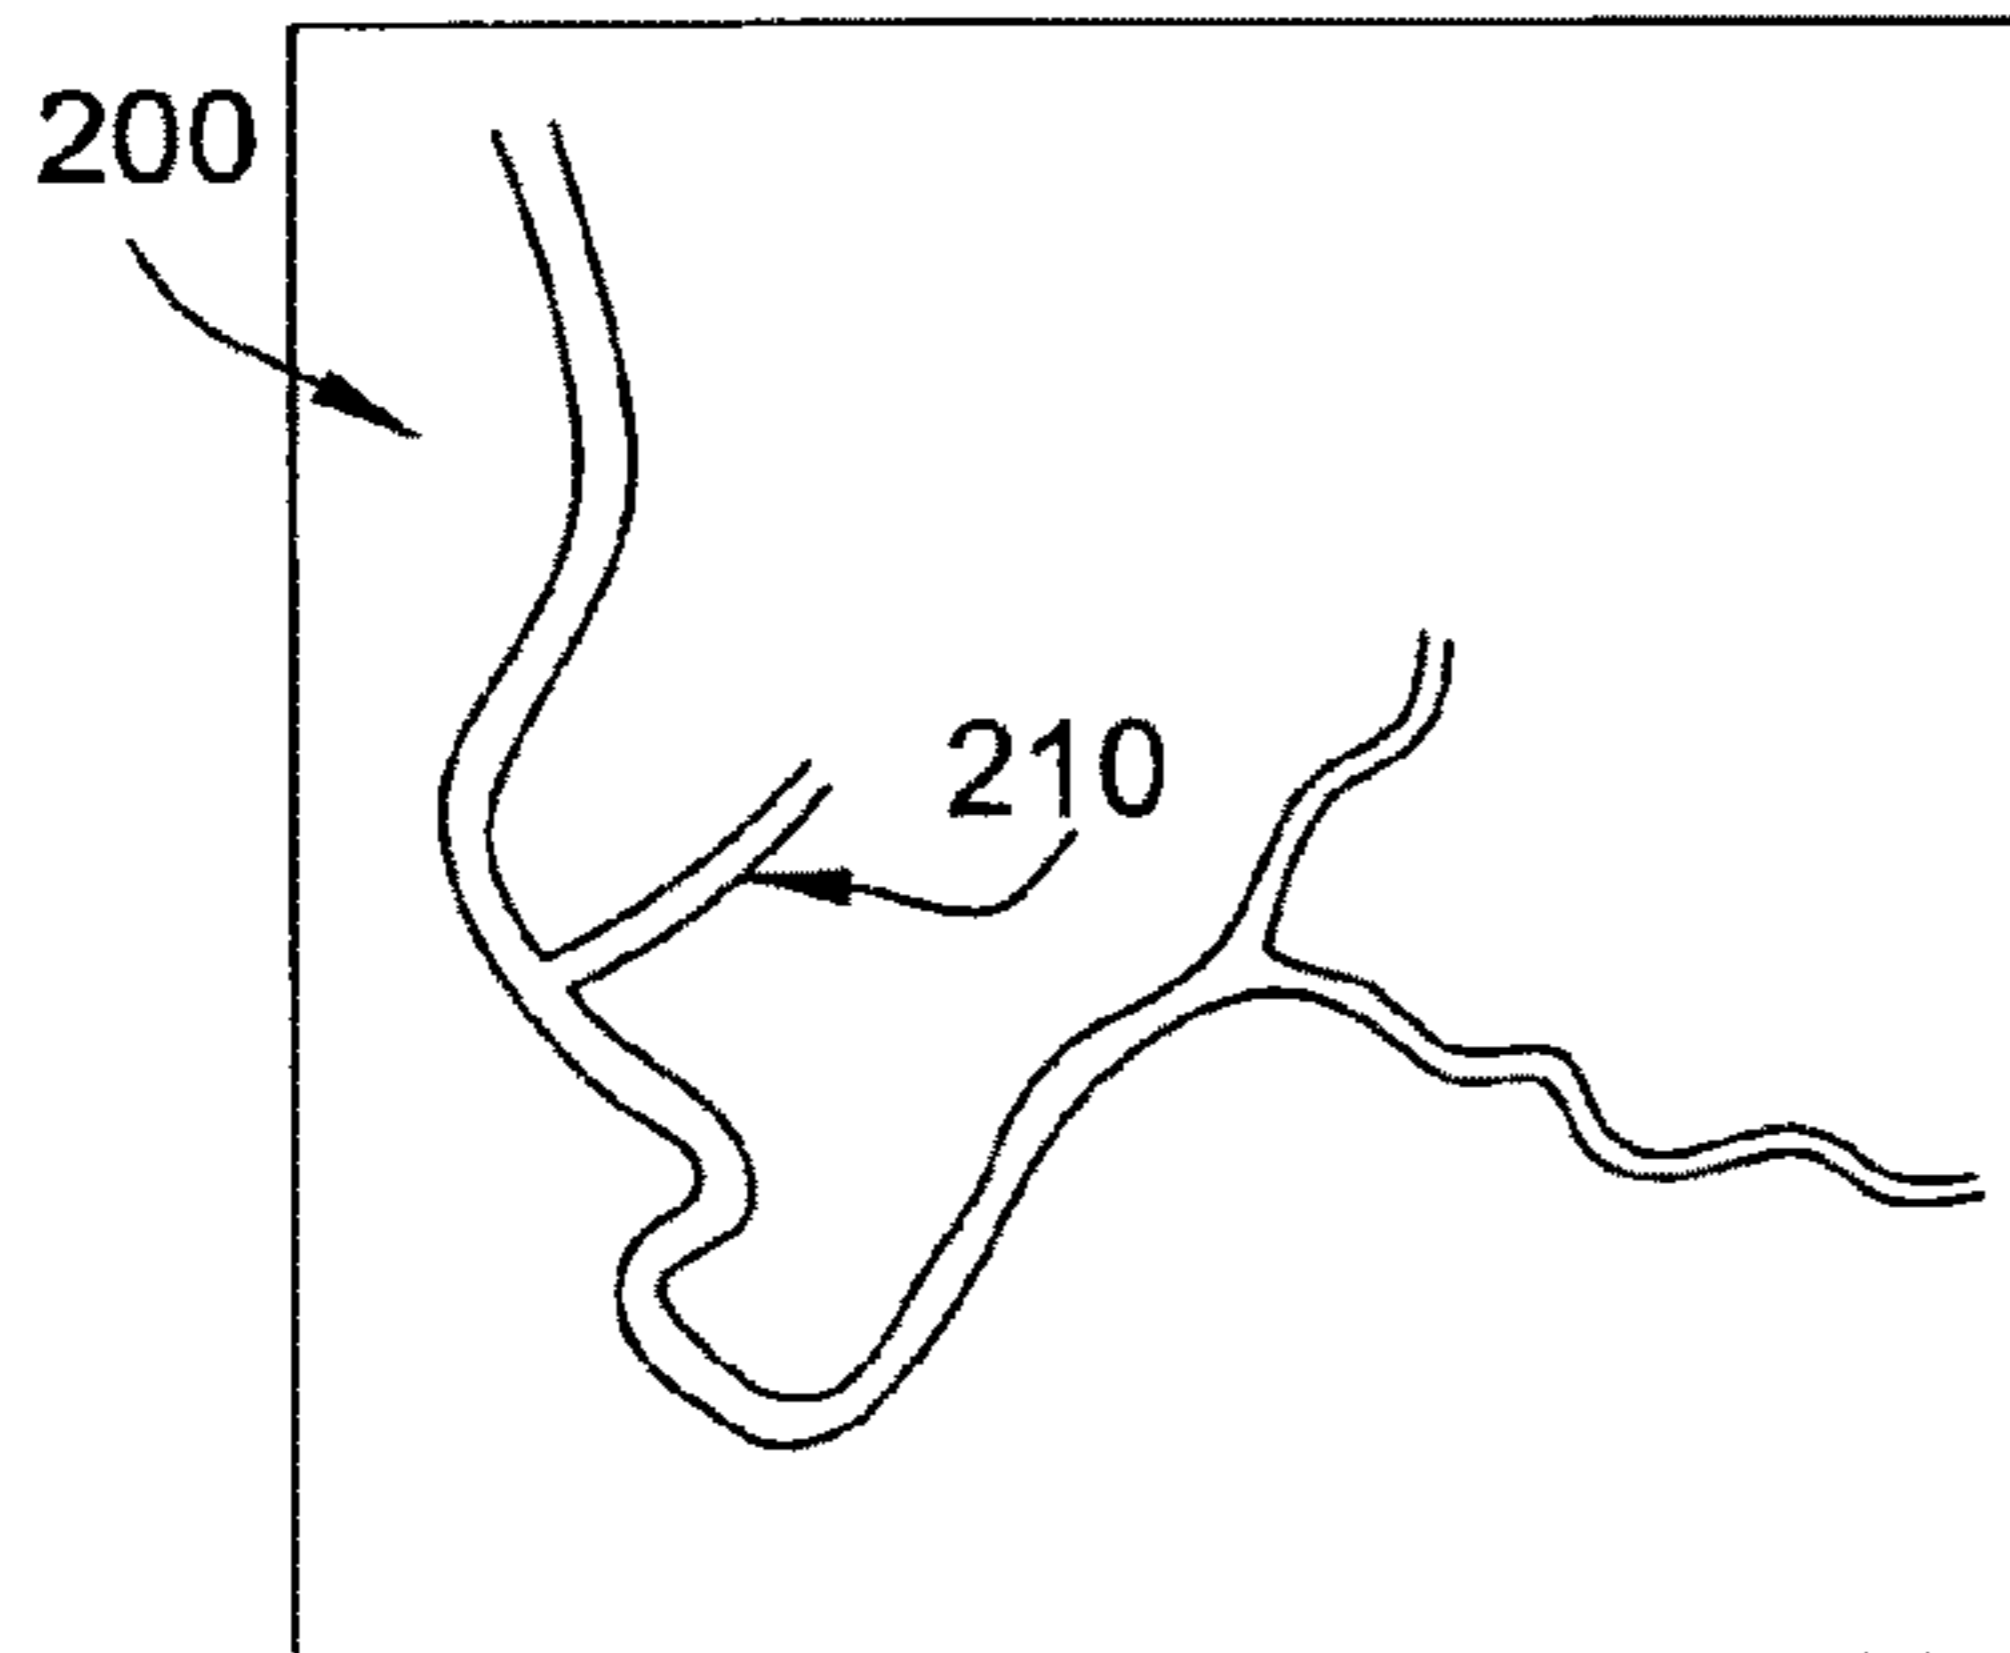


FIG. 3

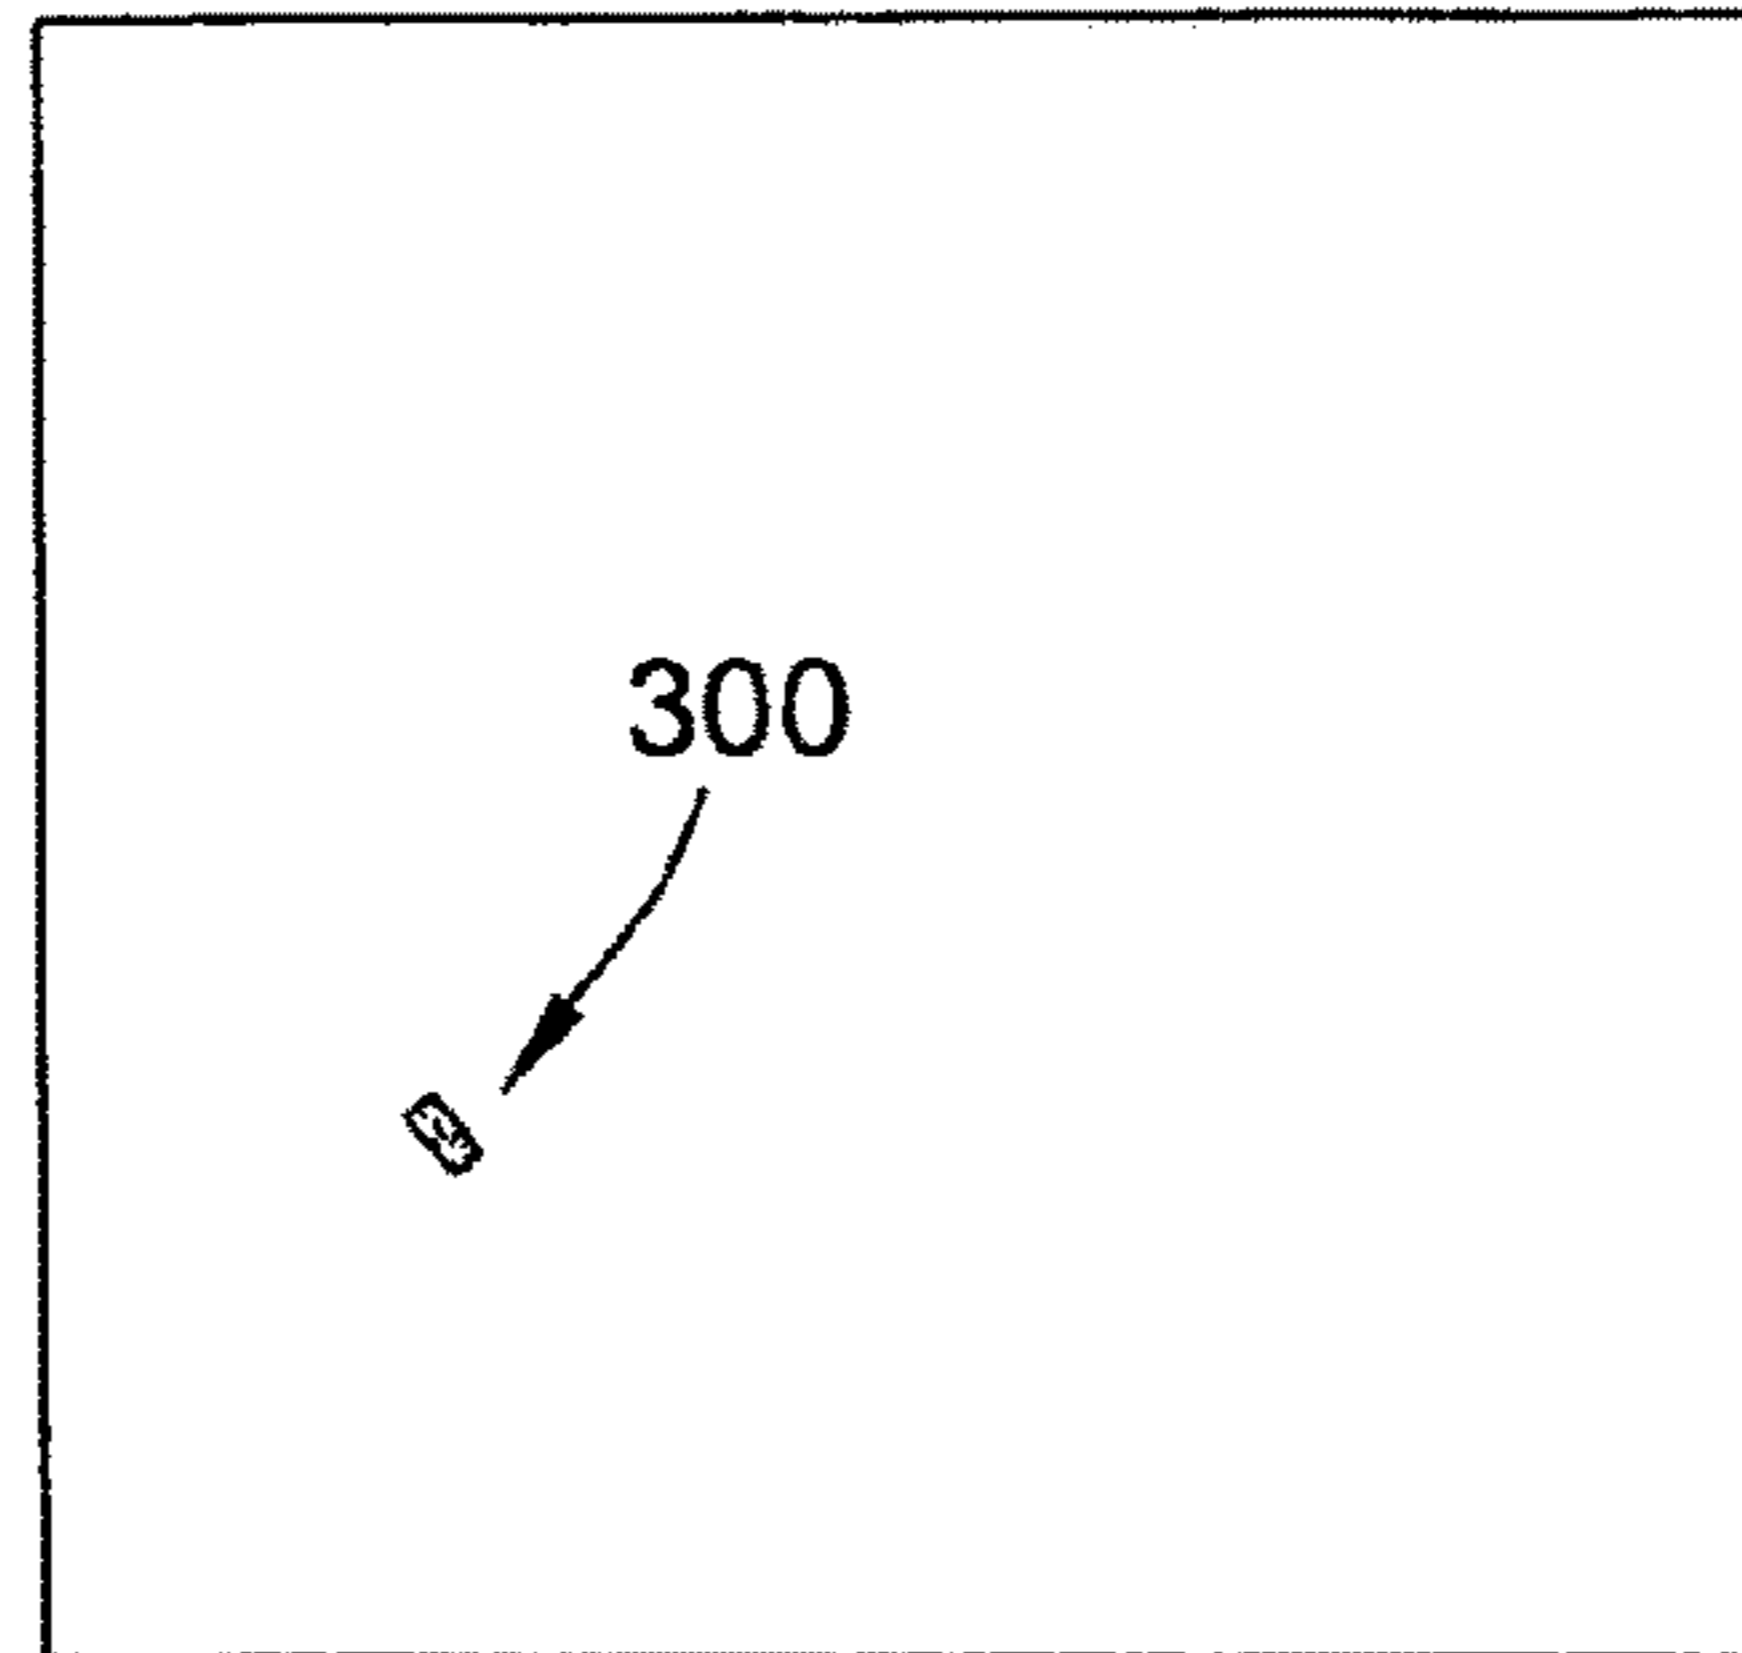


FIG. 4

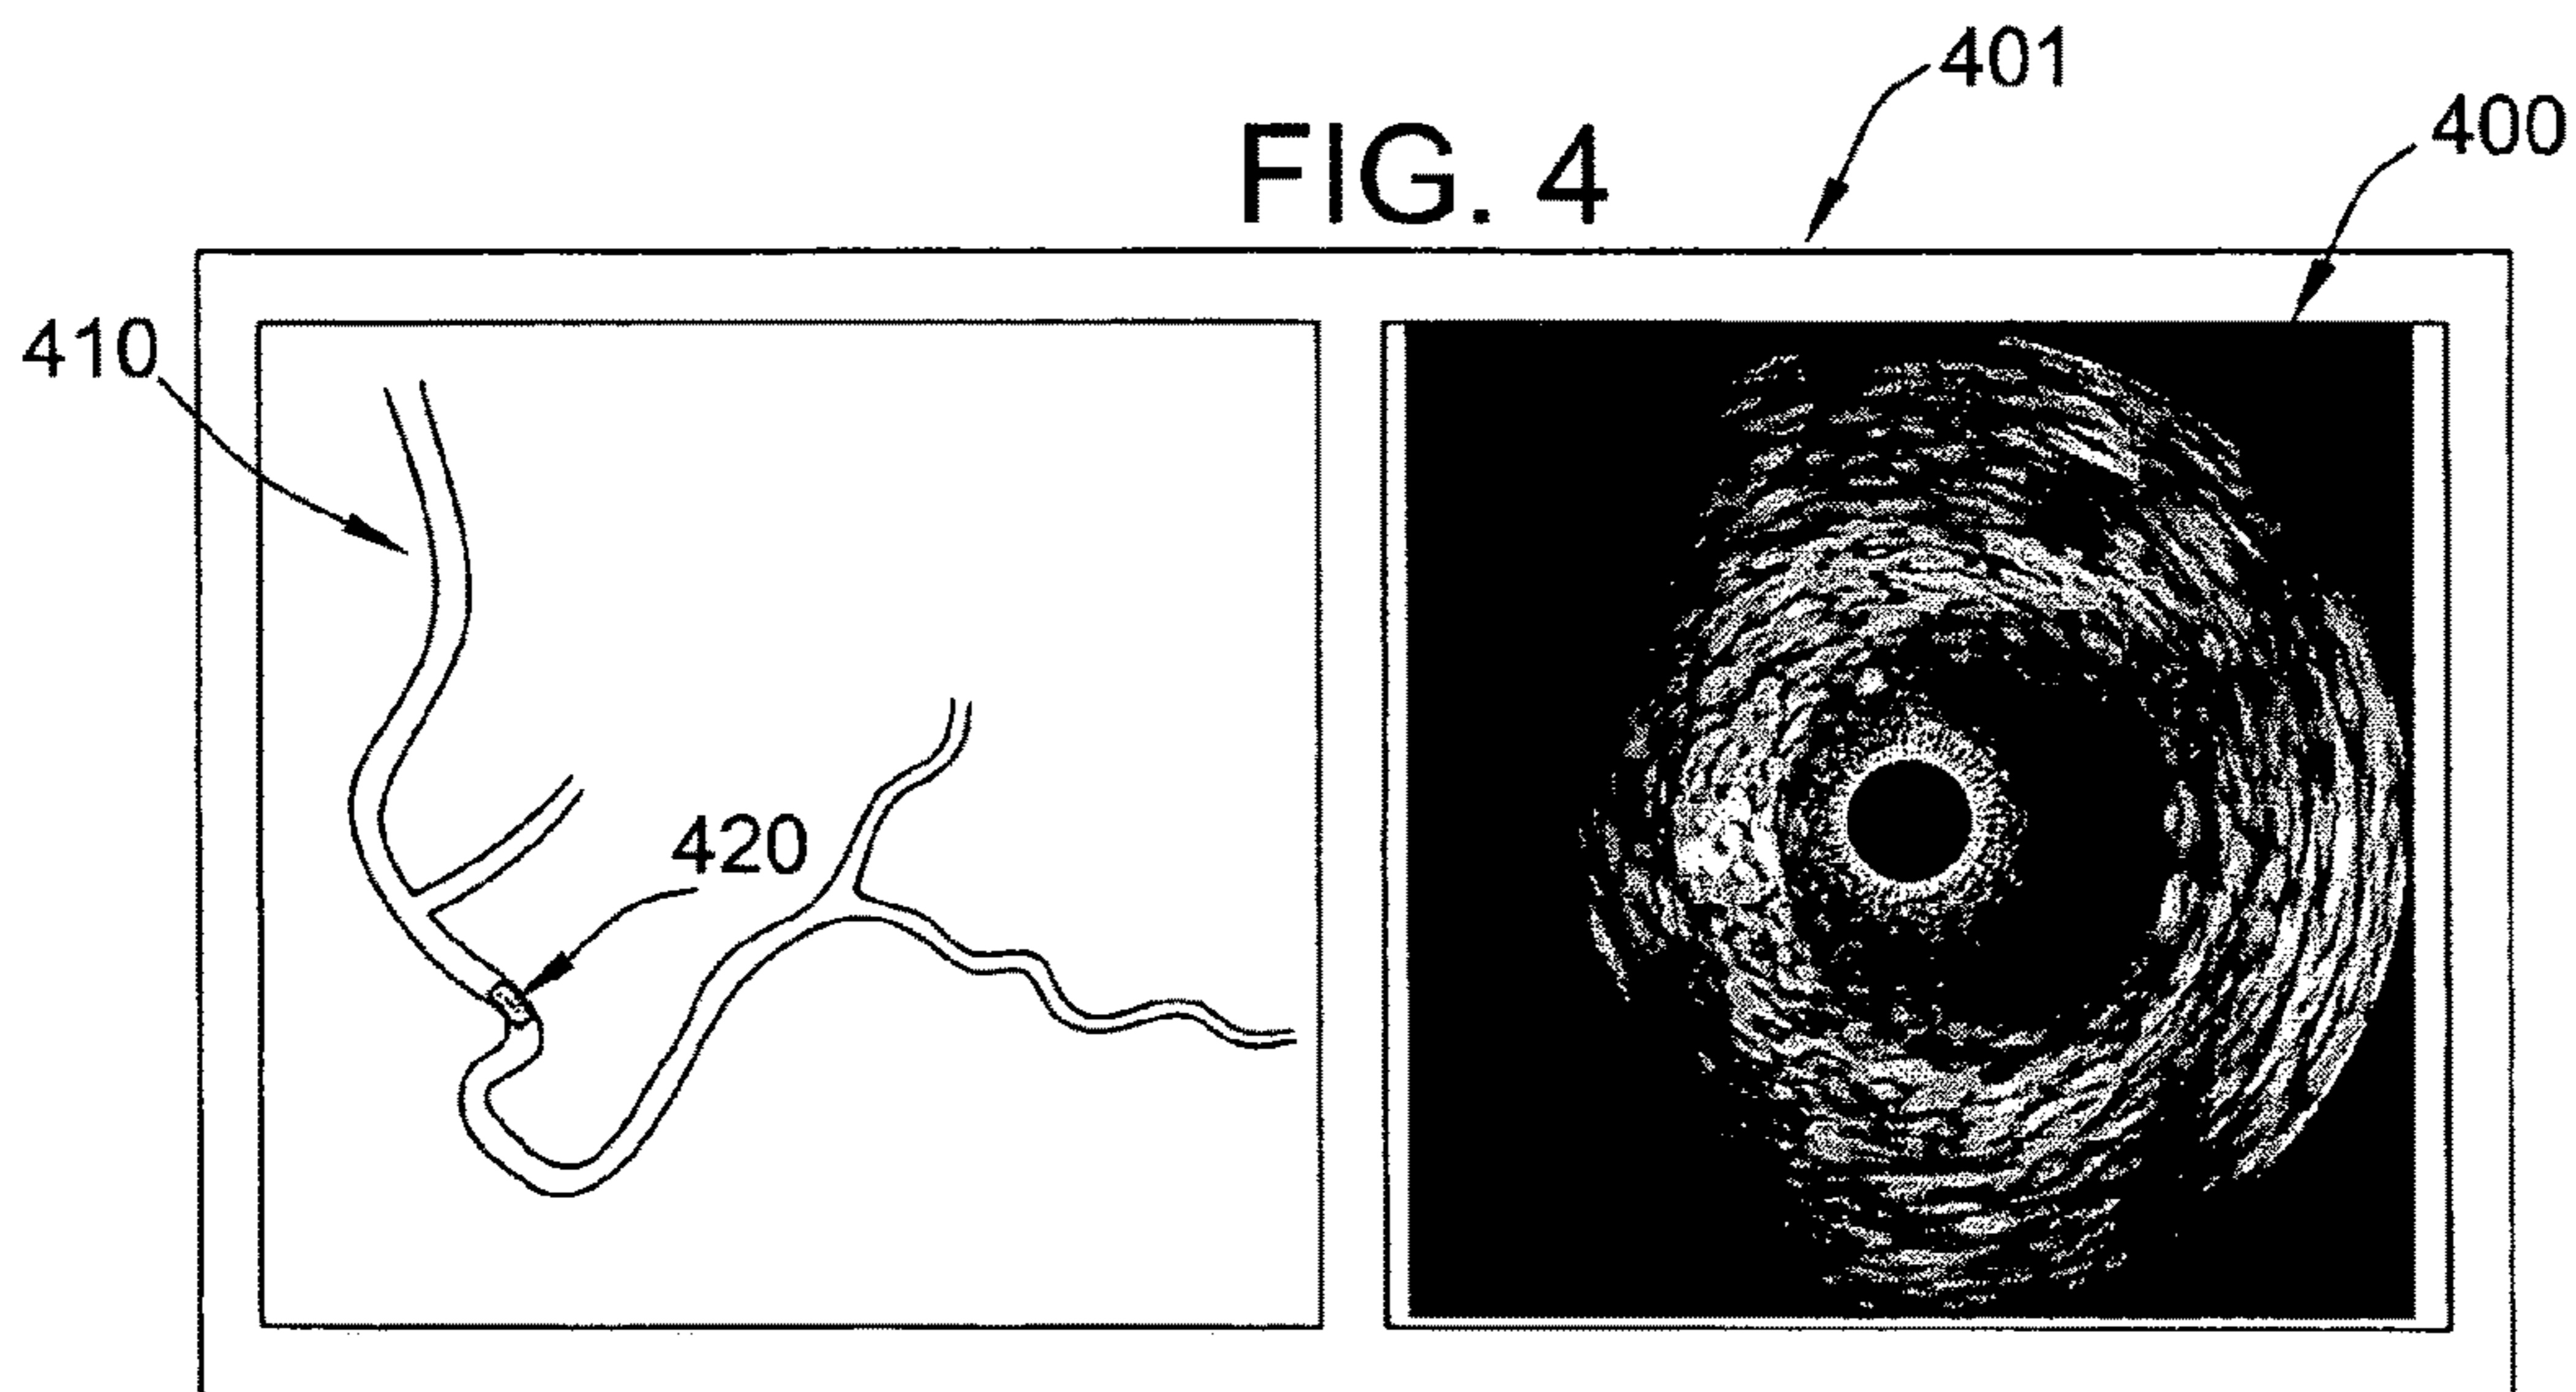


FIG. 5

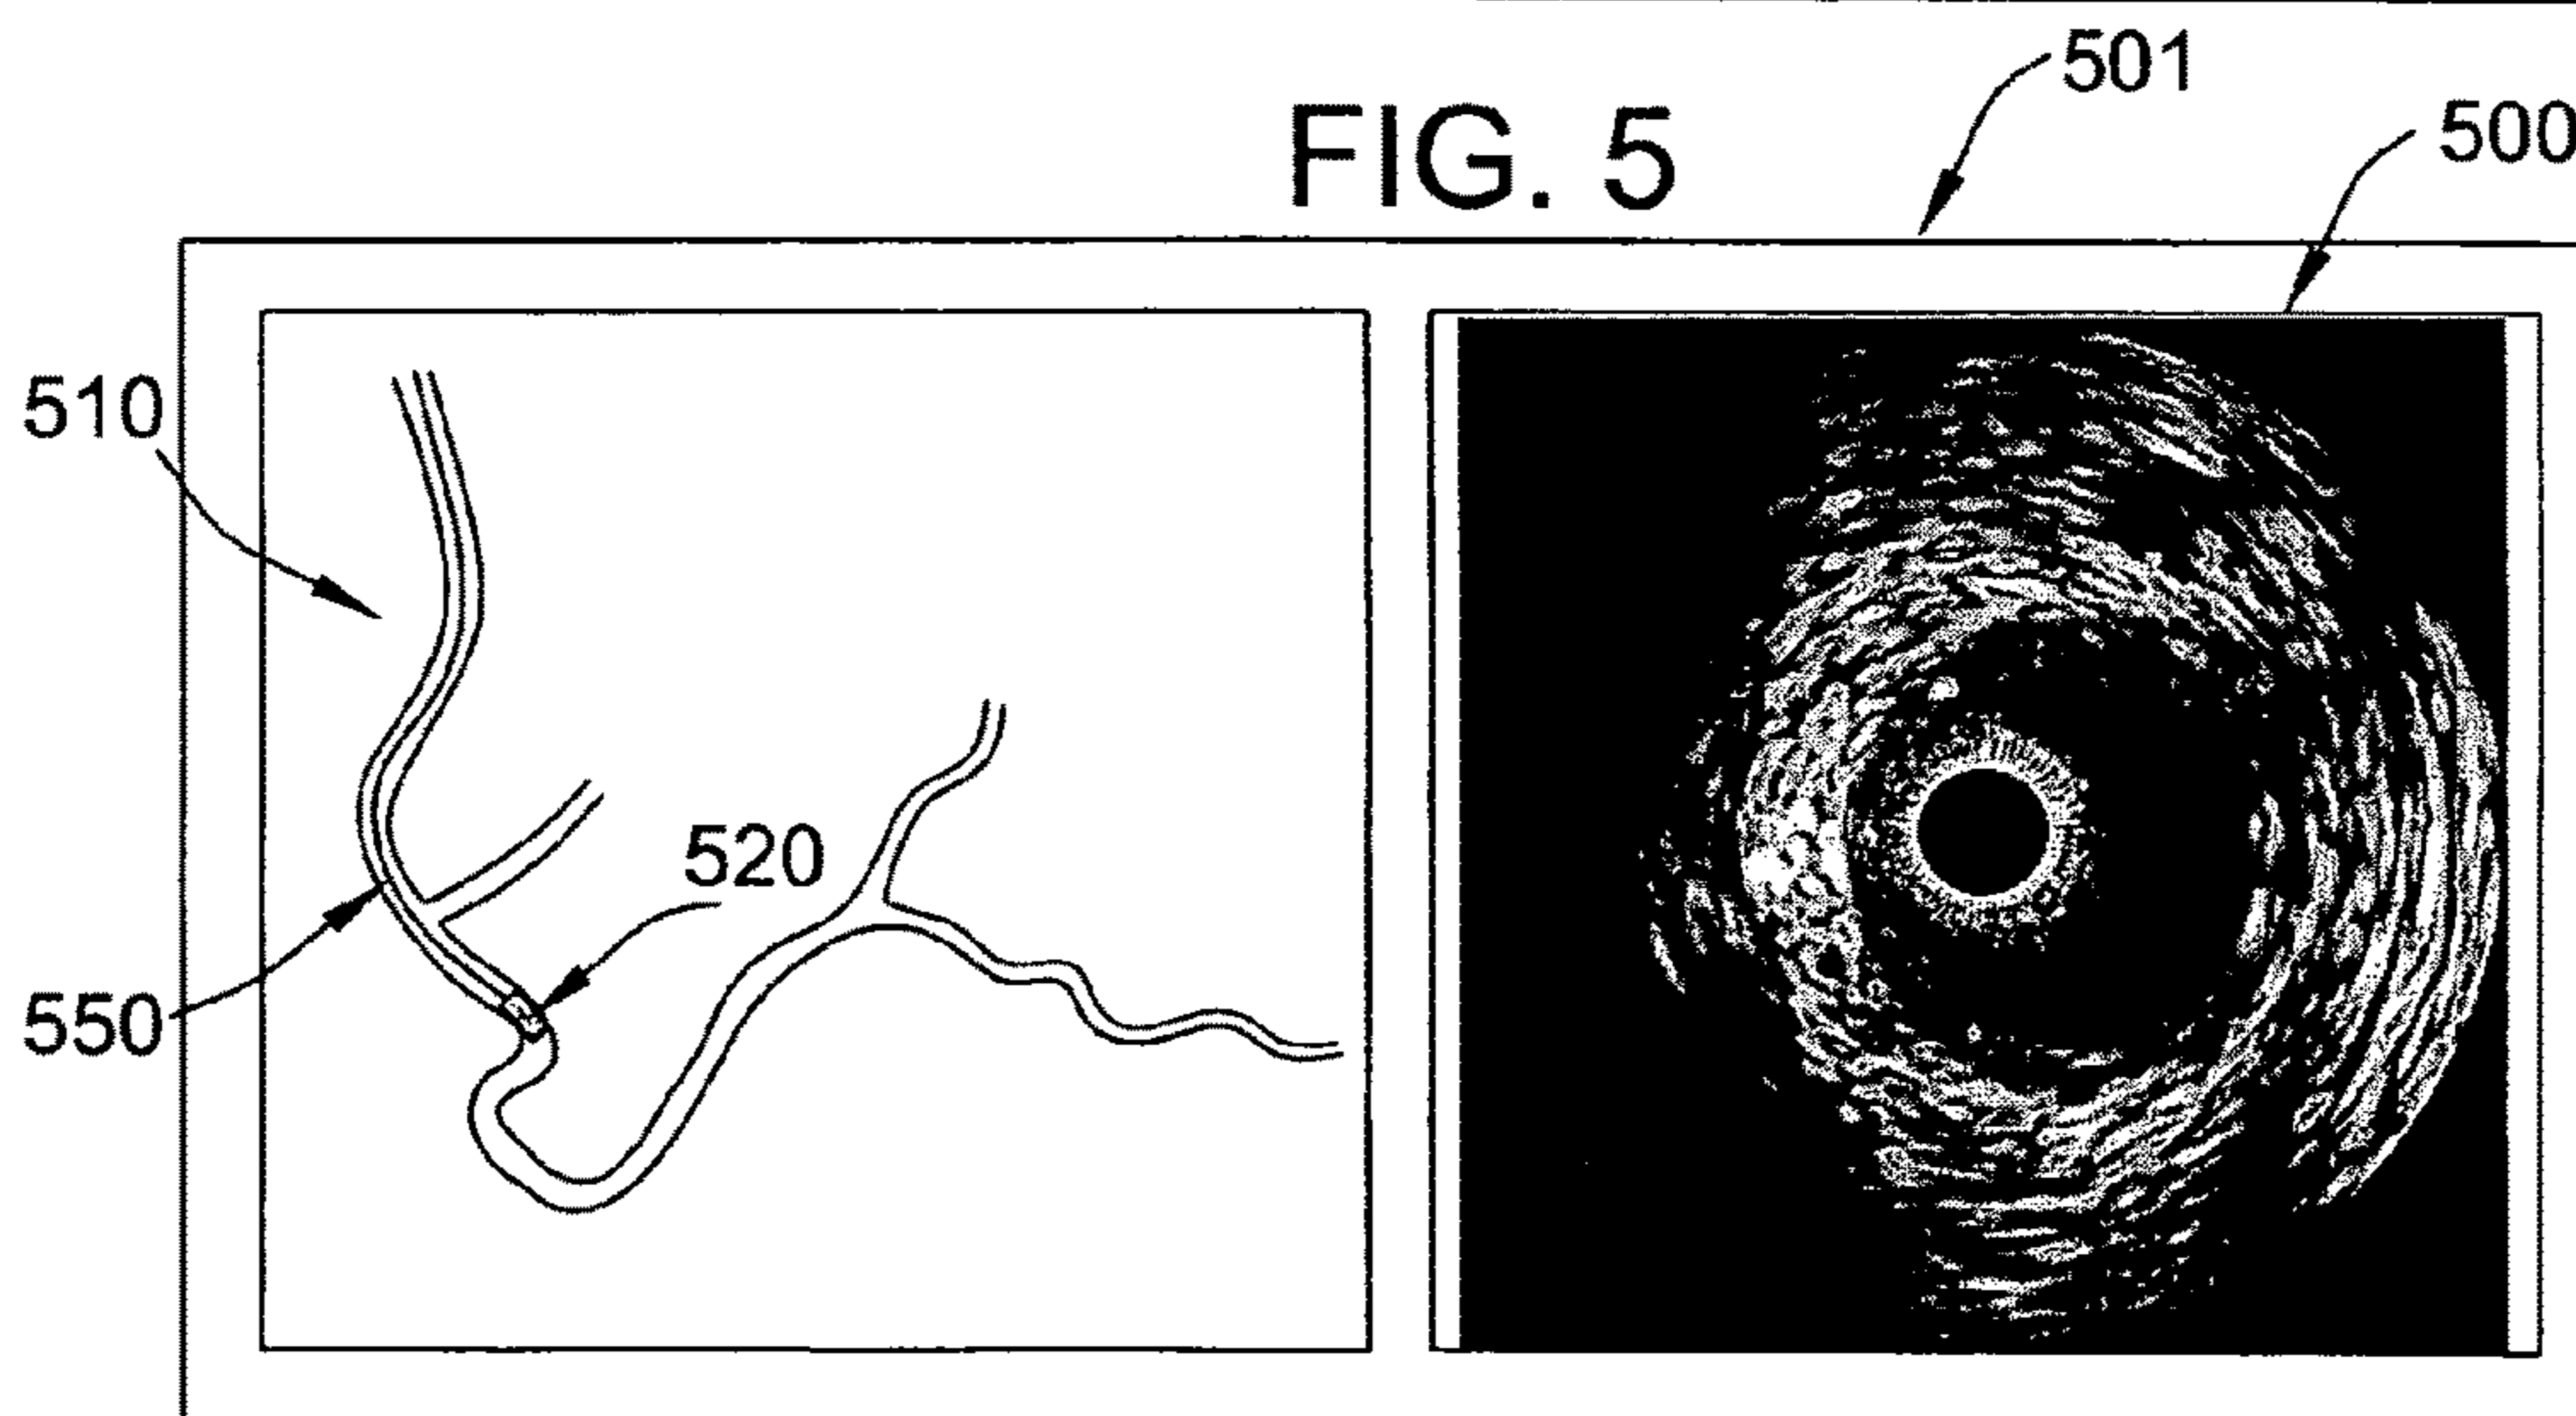


FIG. 6

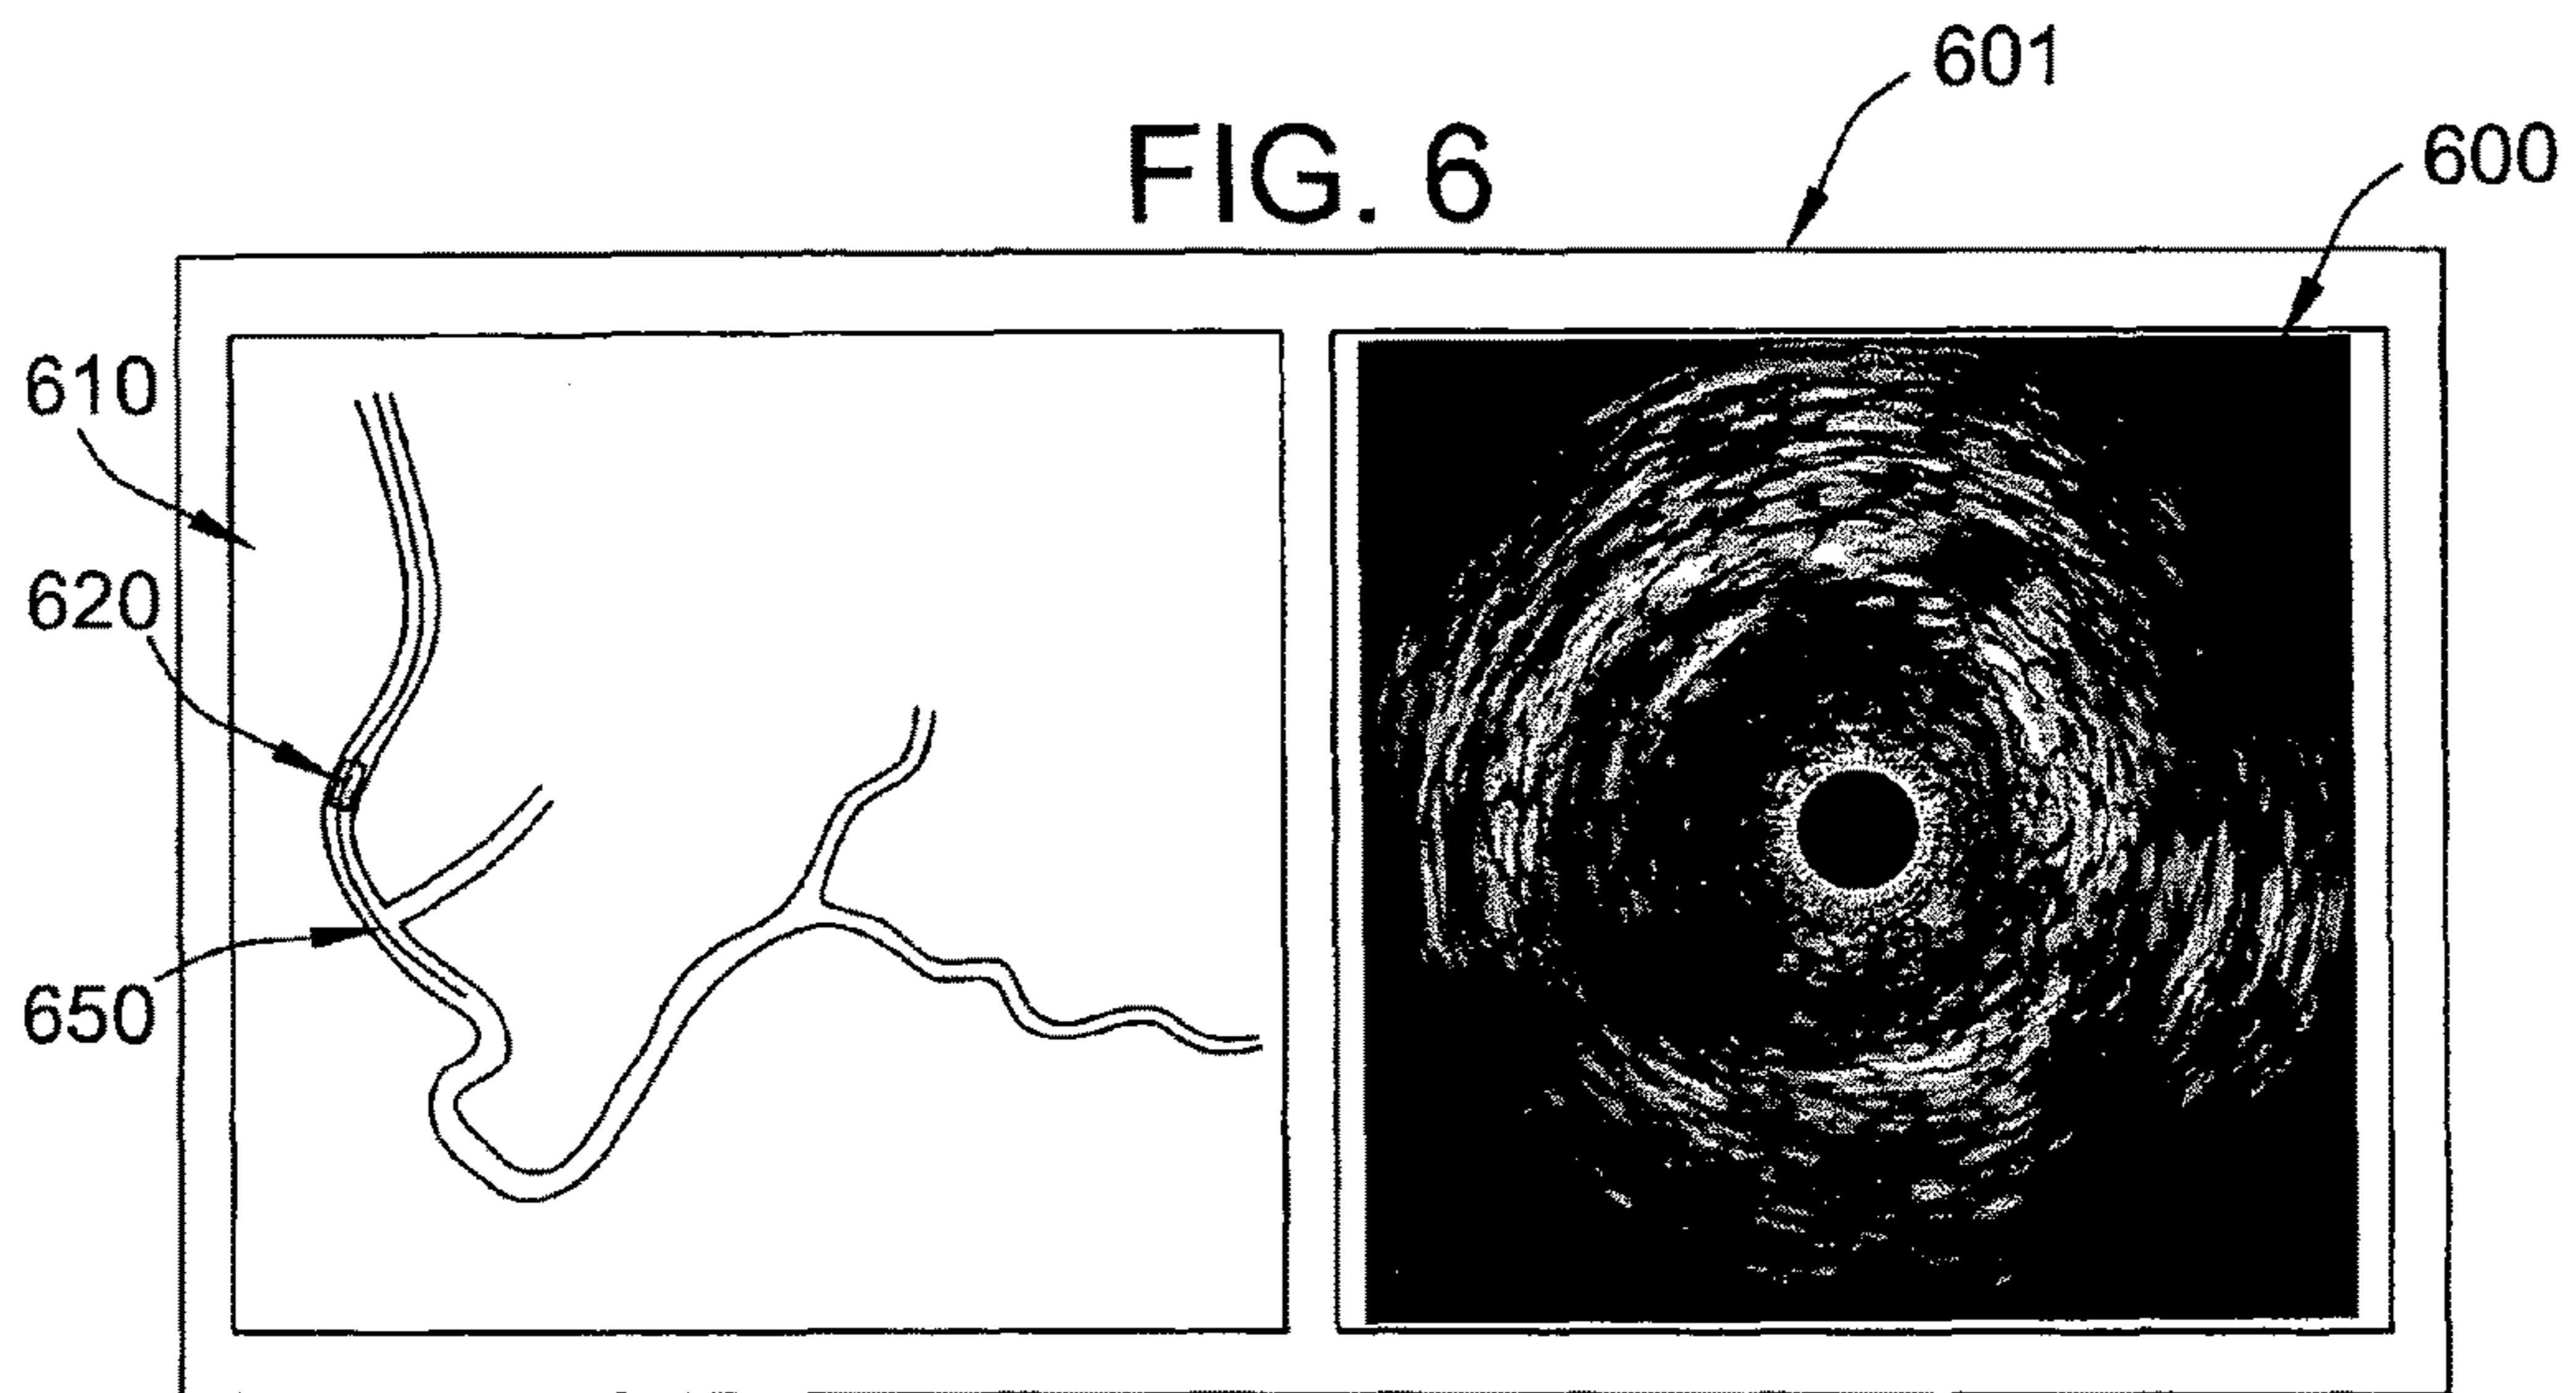


FIG. 7

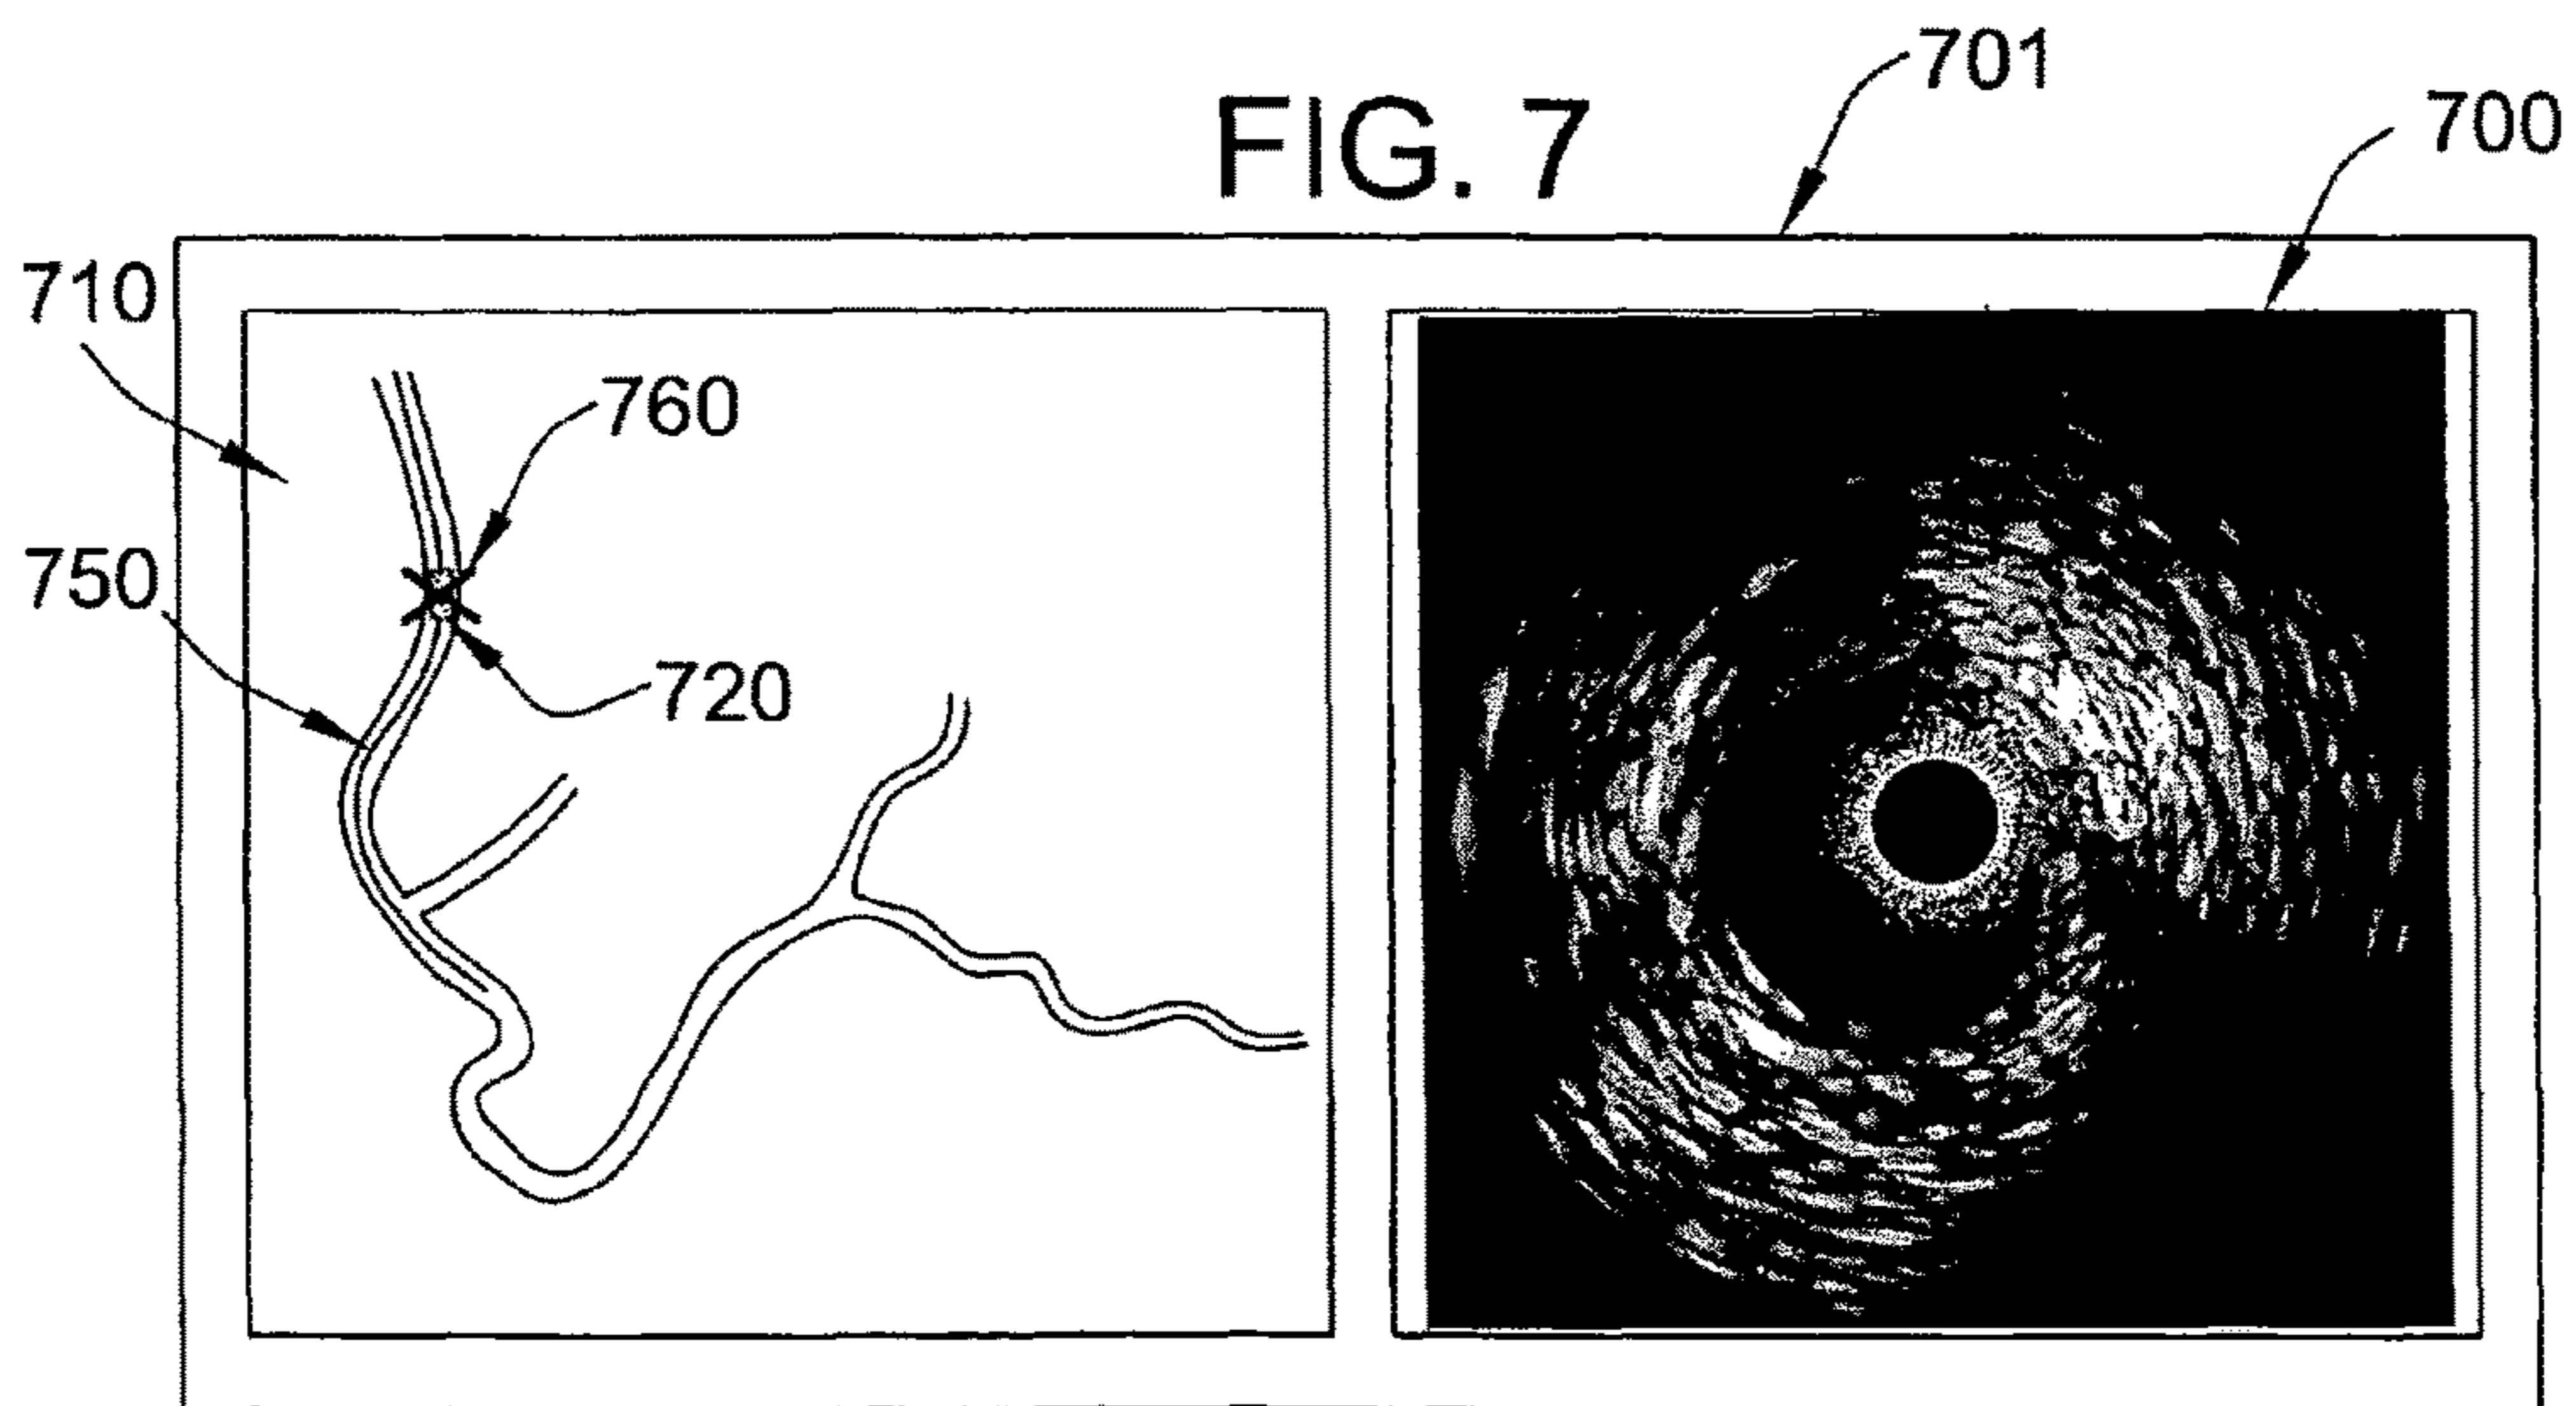


FIG. 8

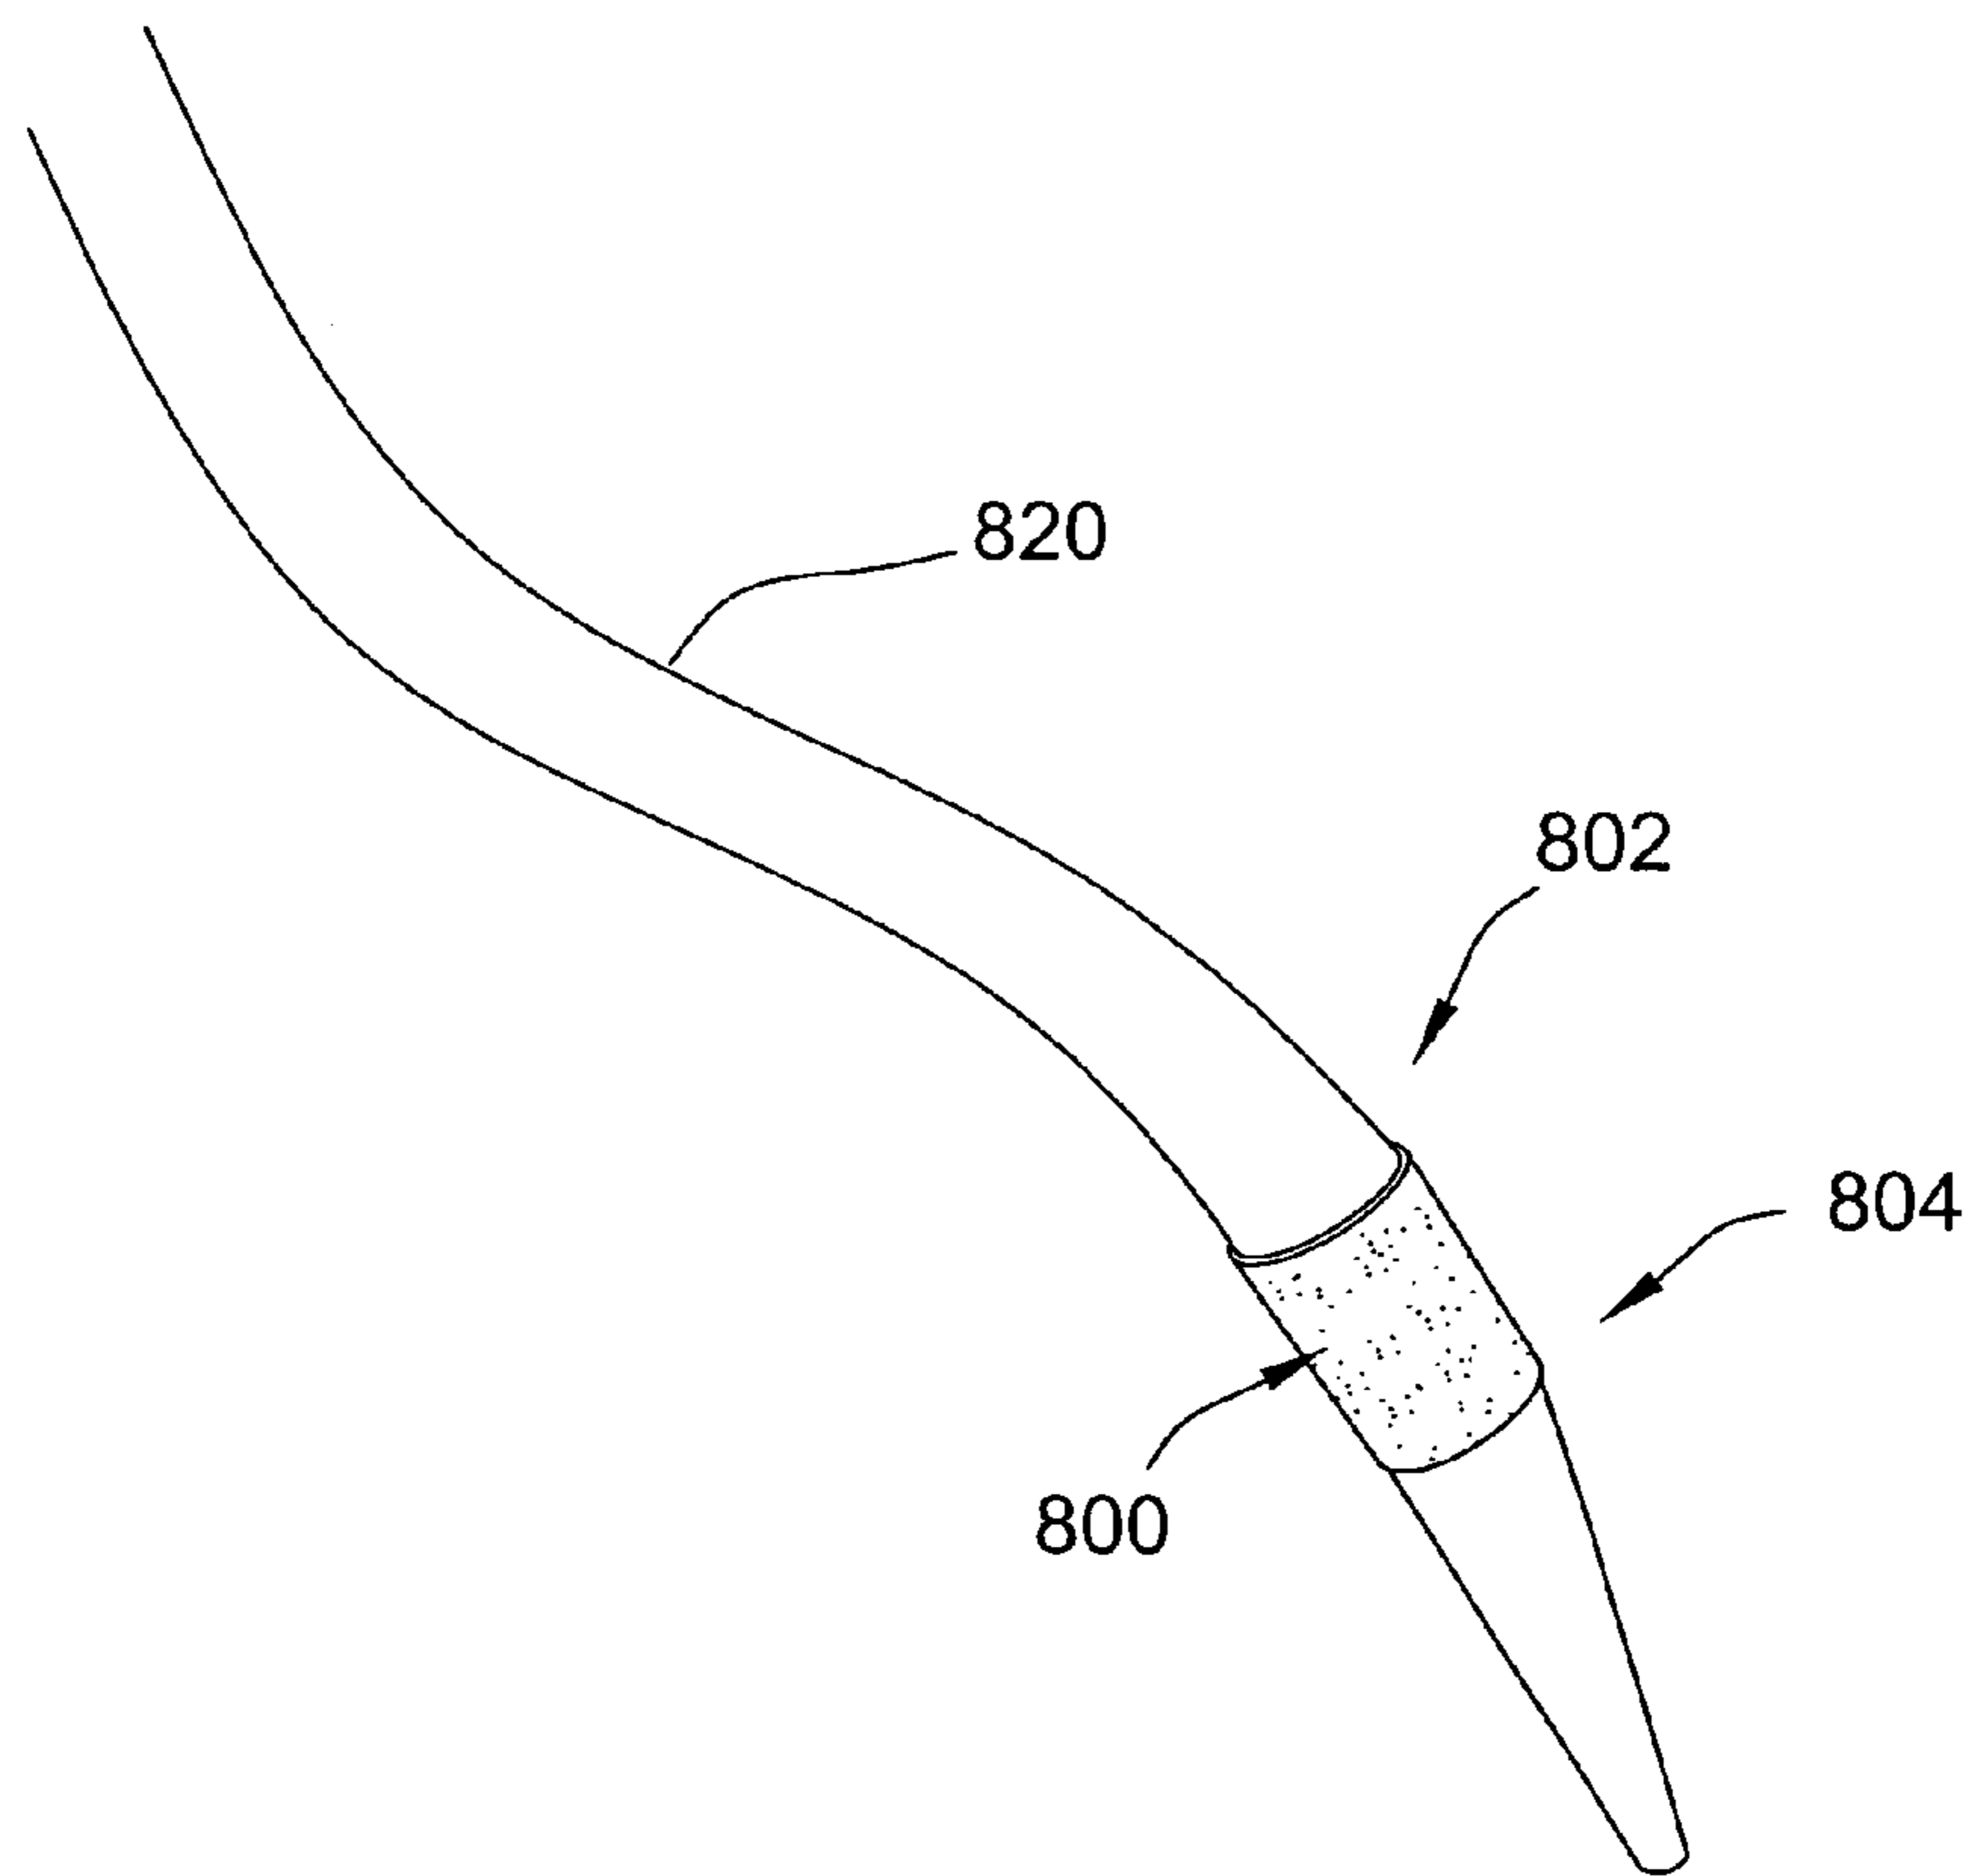


FIG. 9a

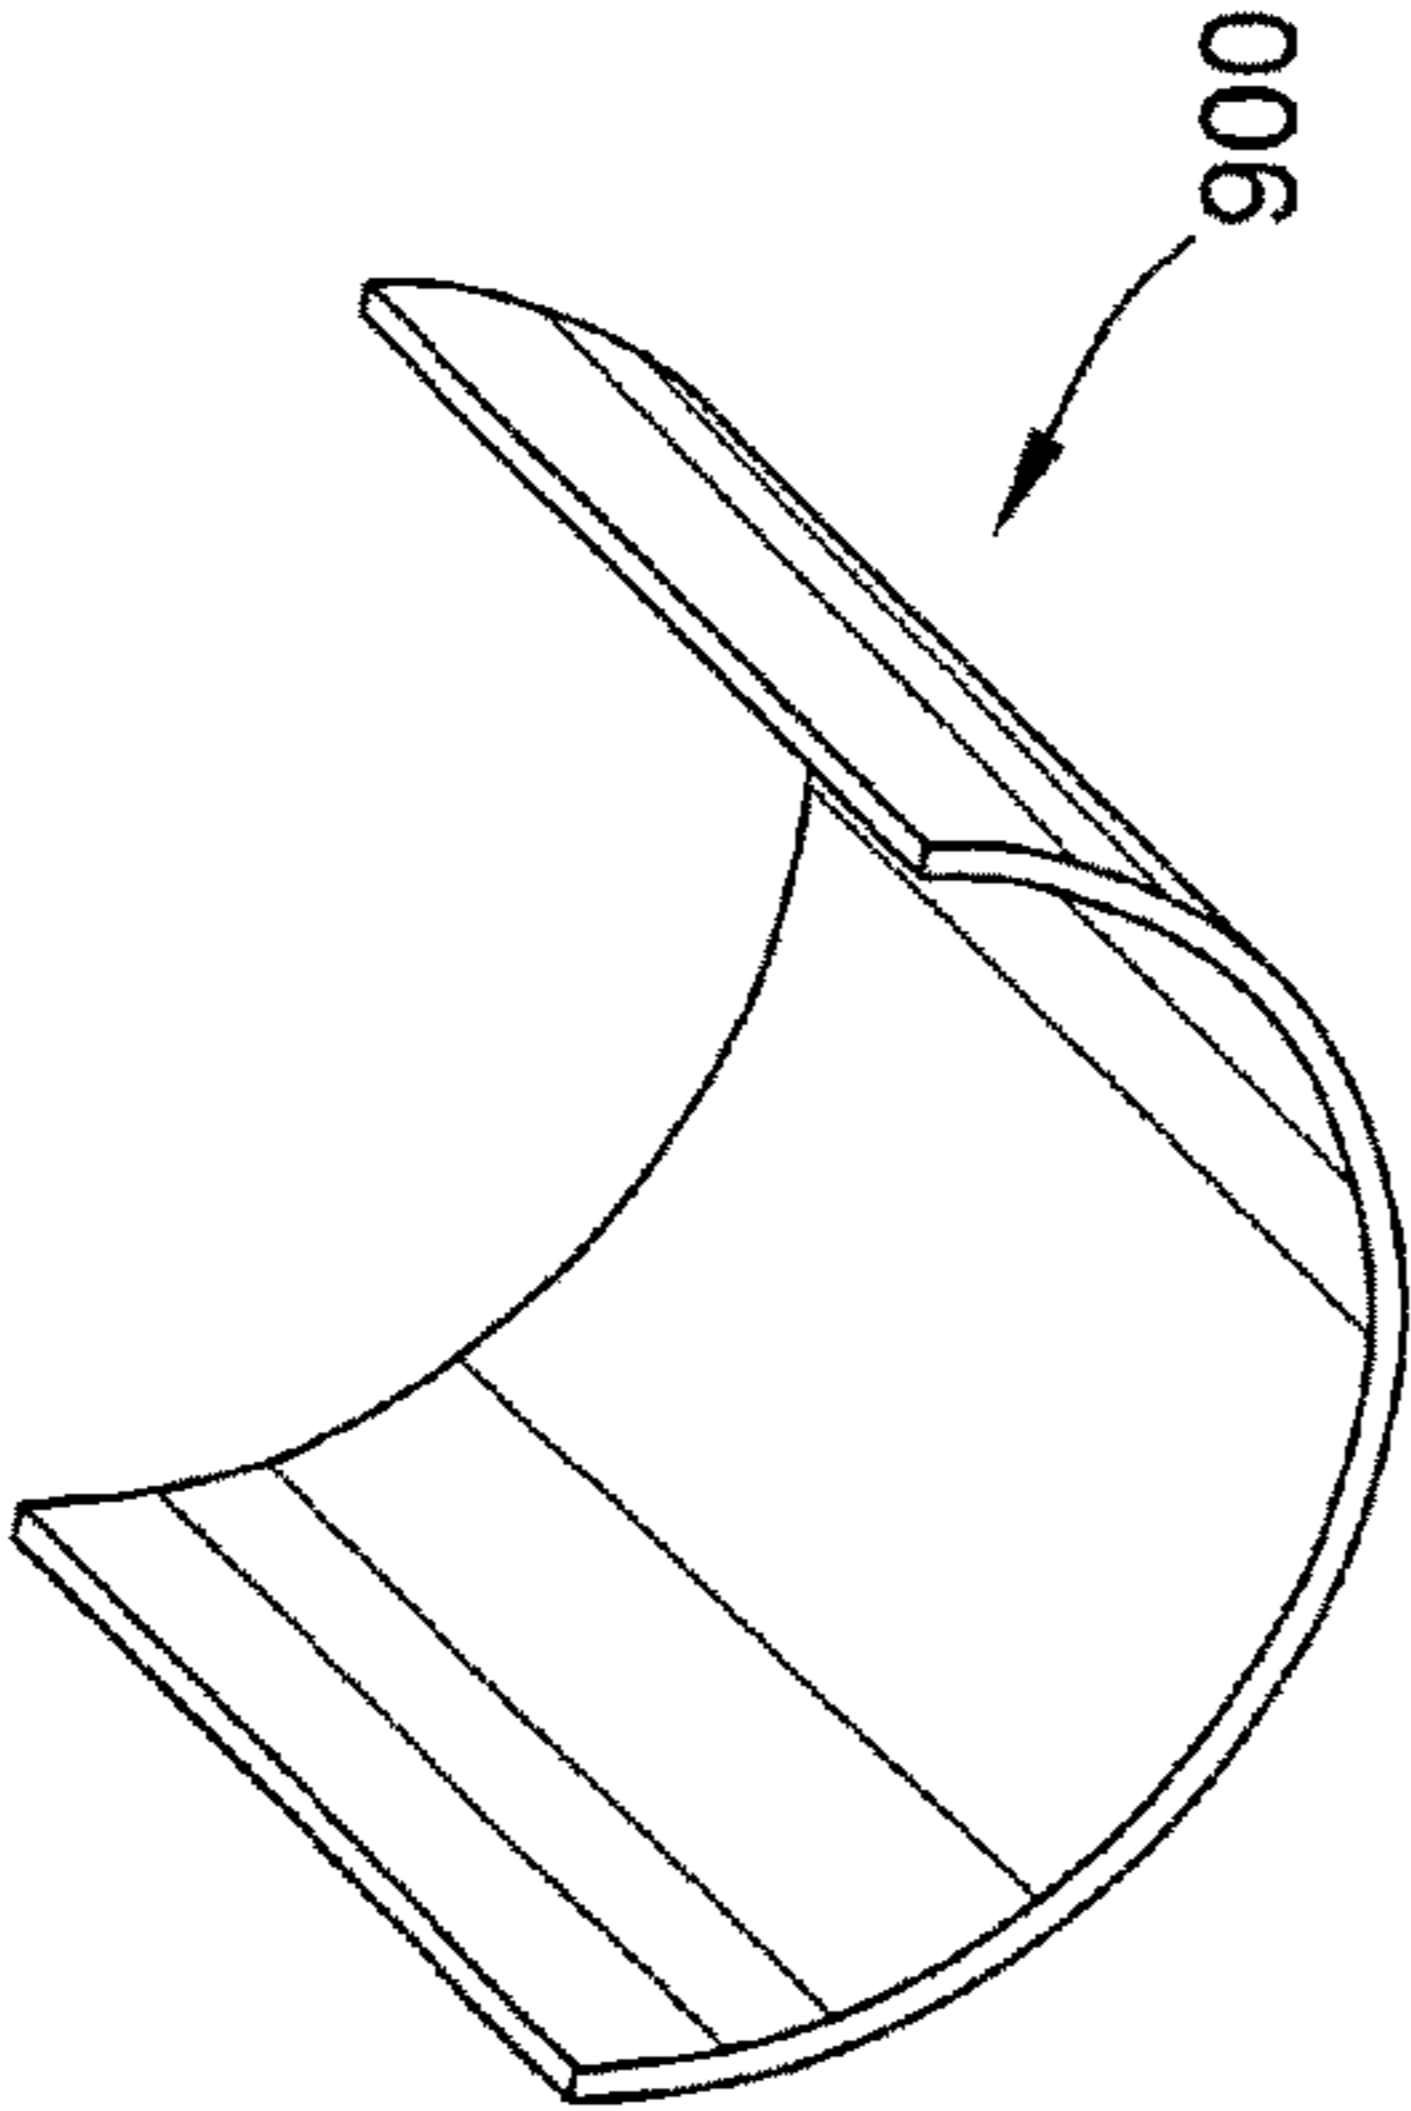
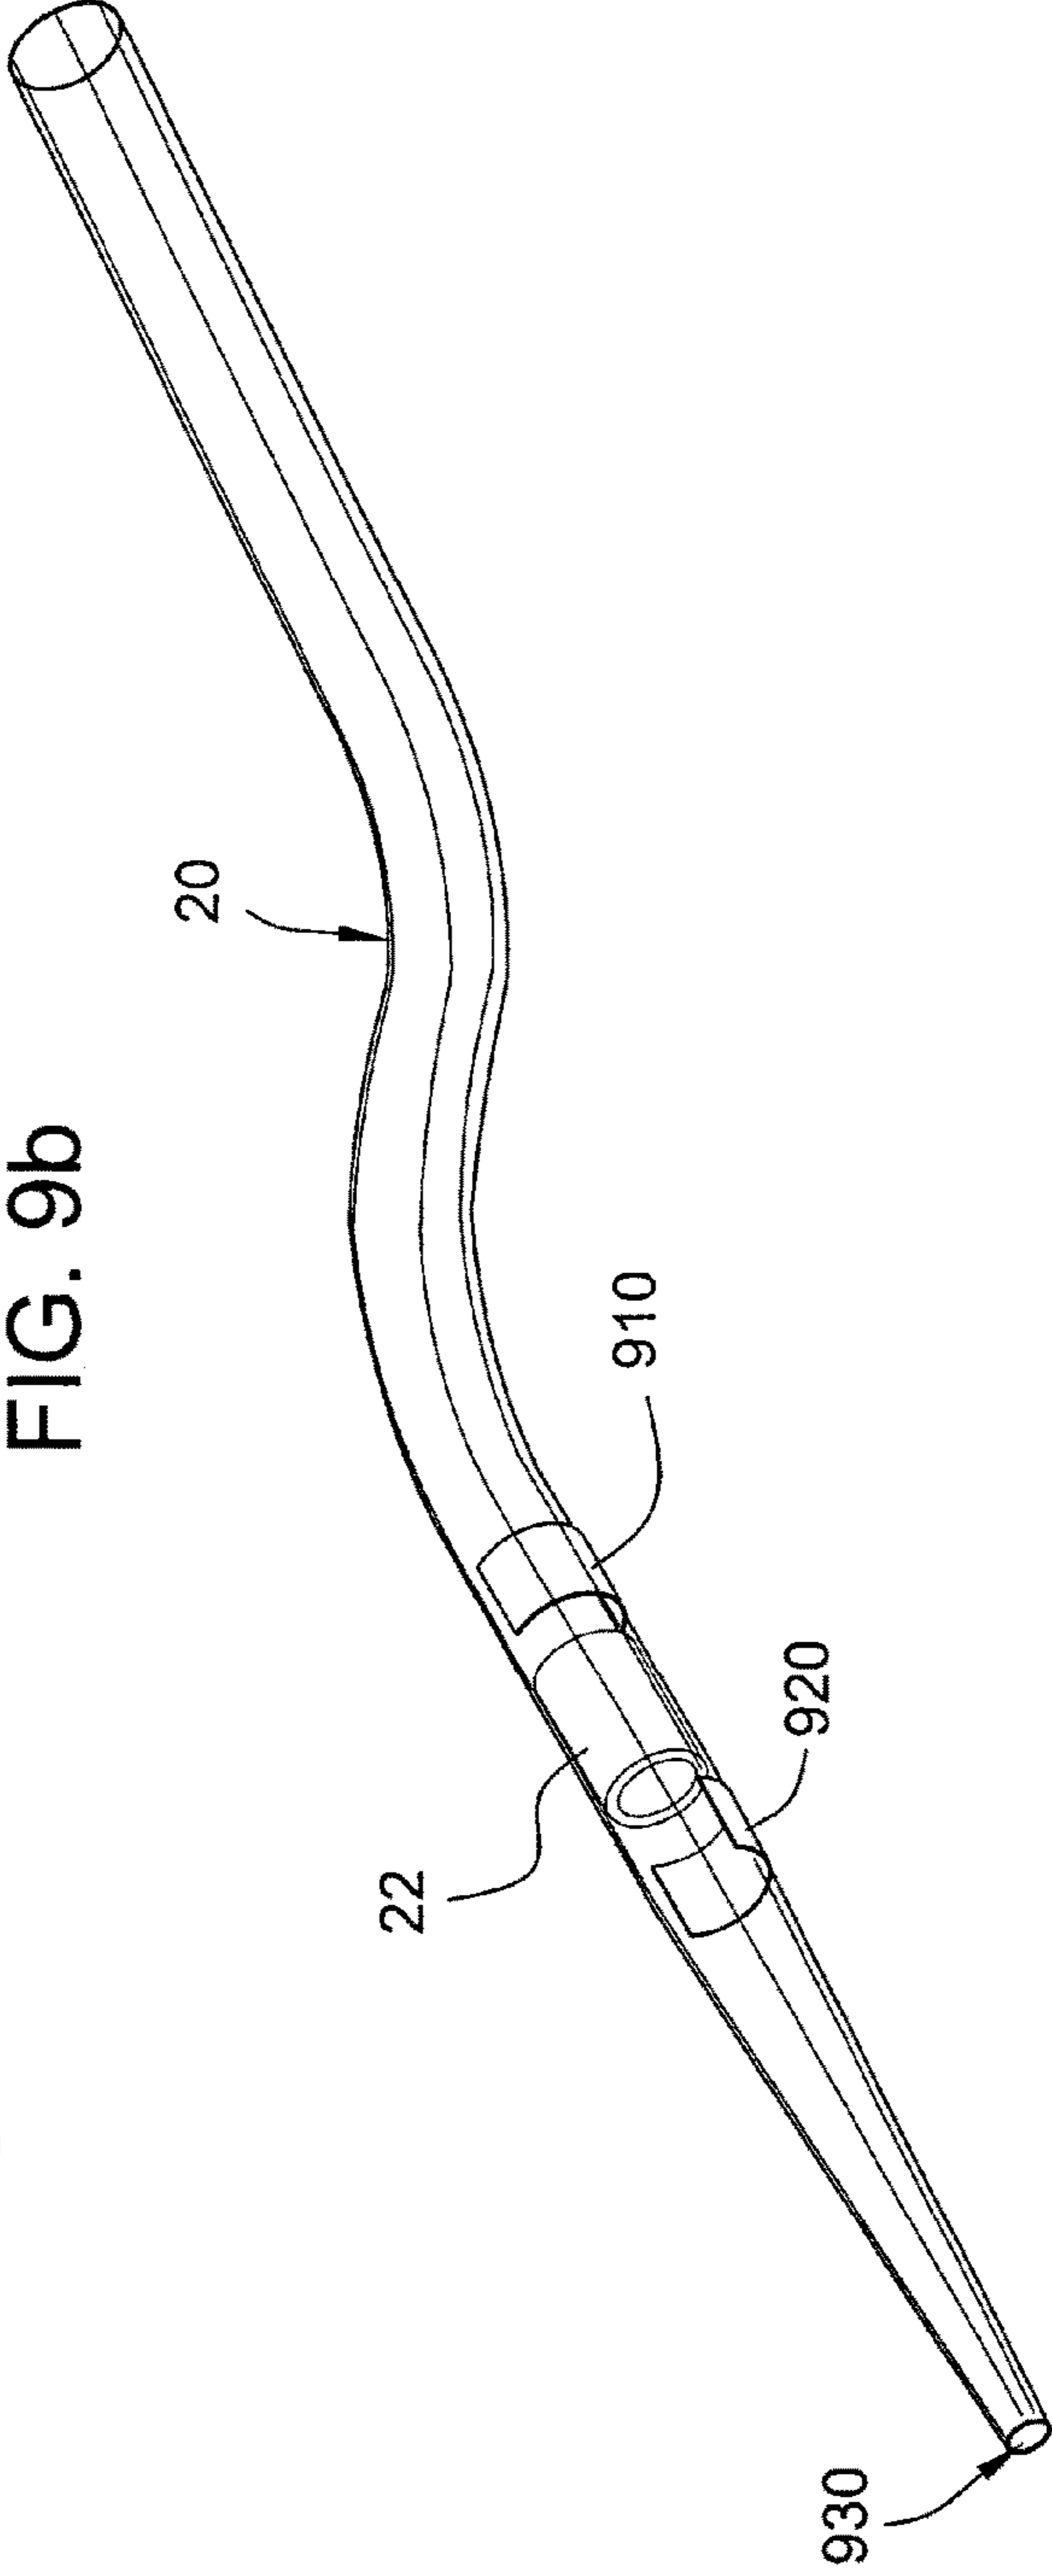


FIG. 9b



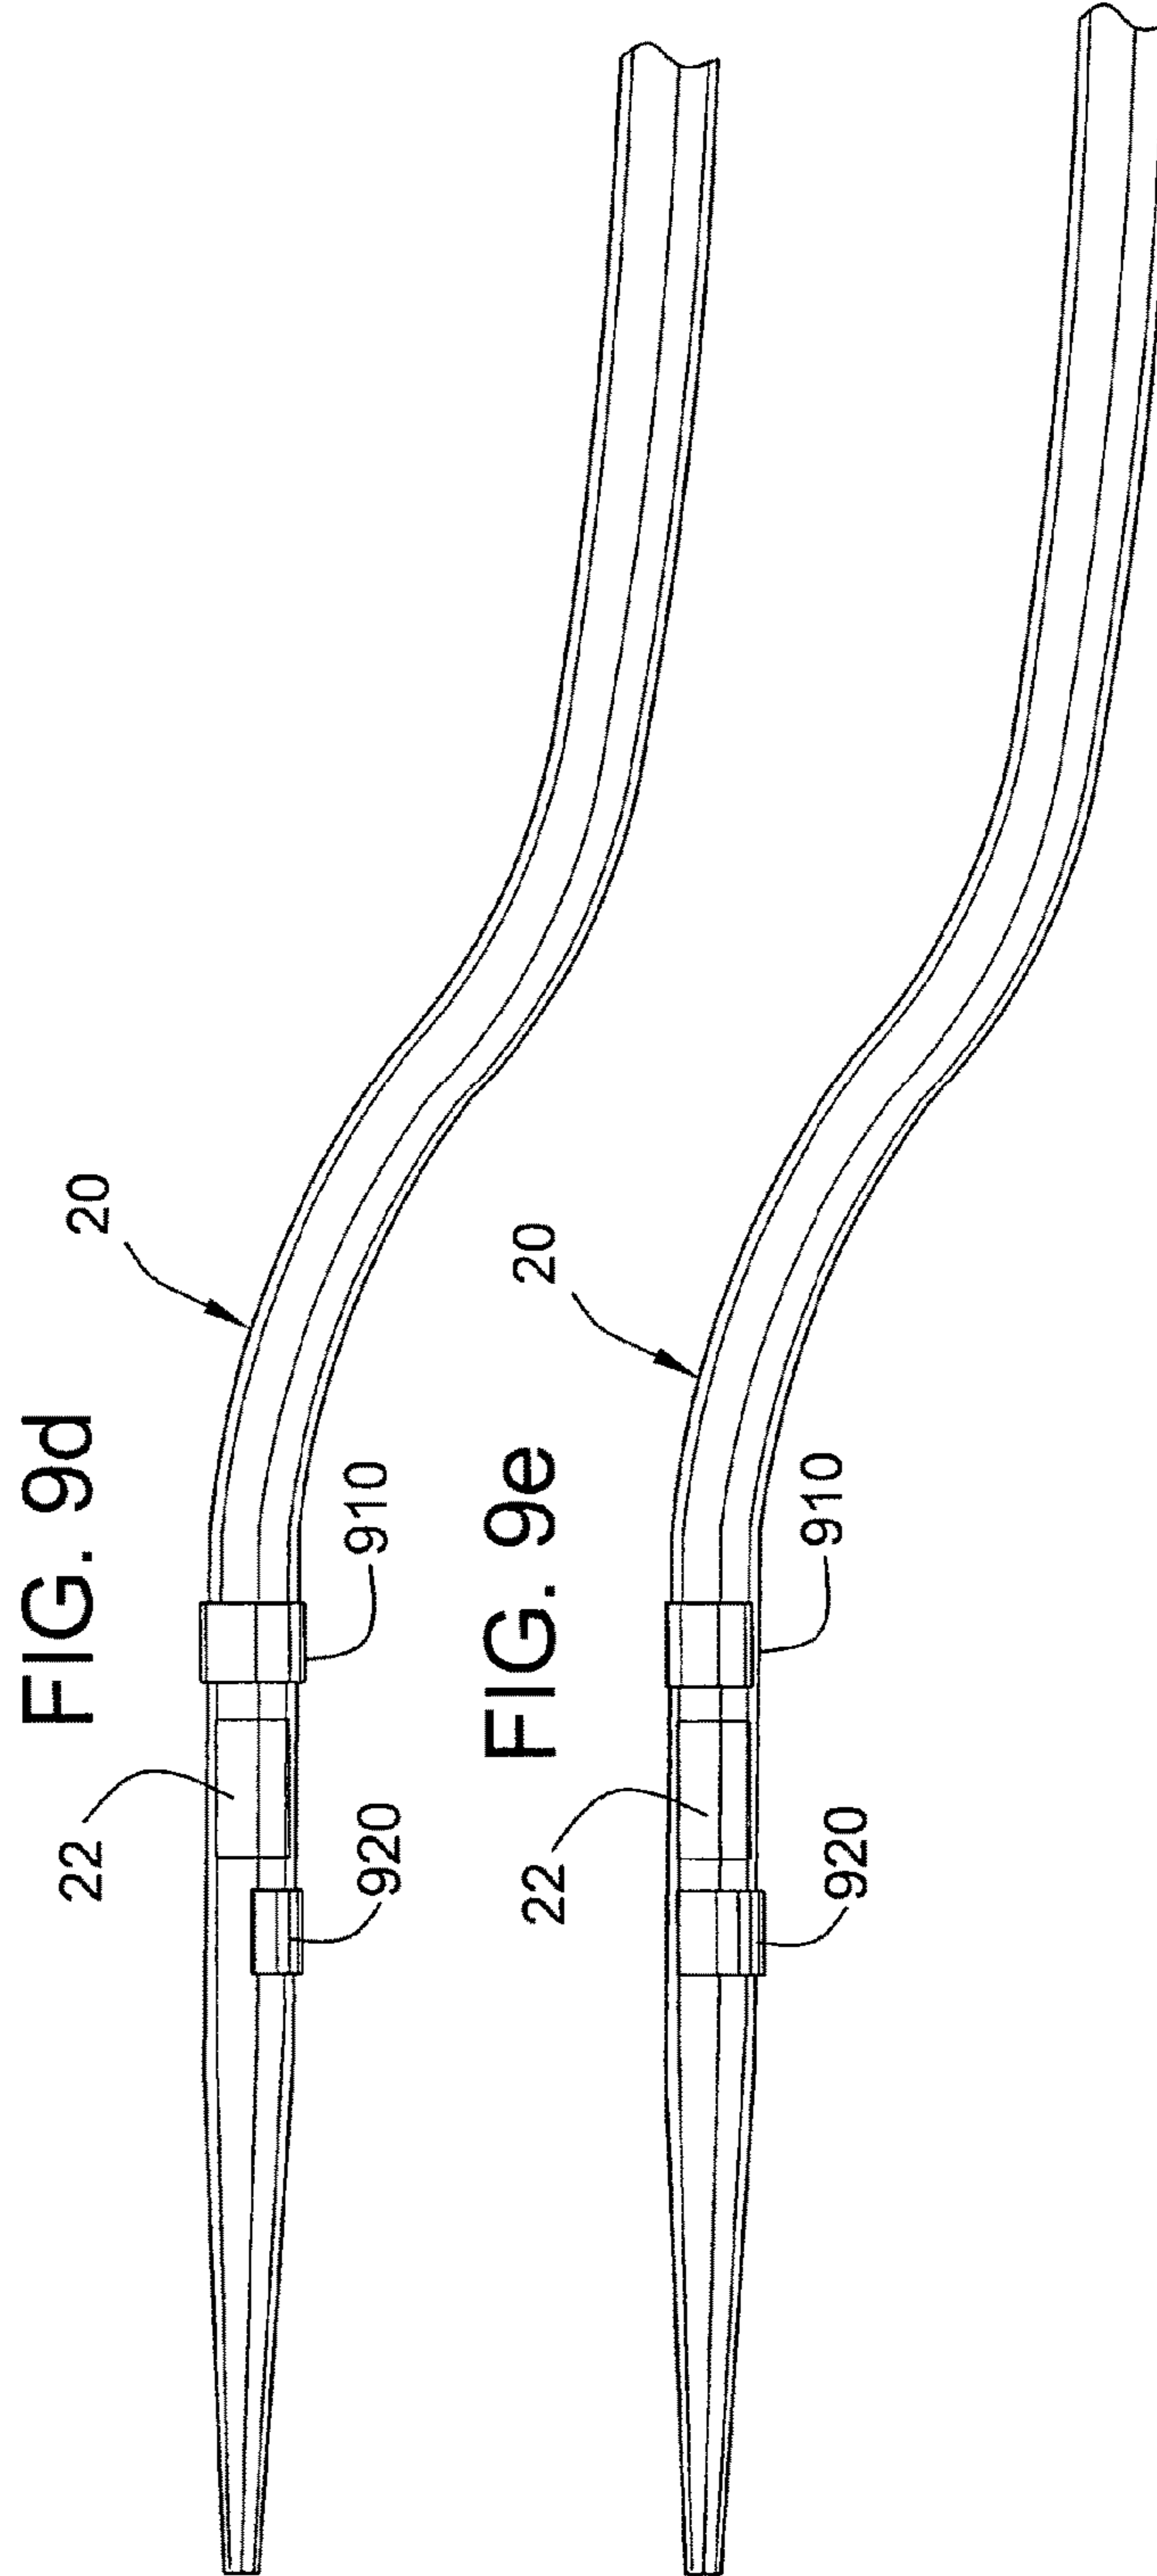
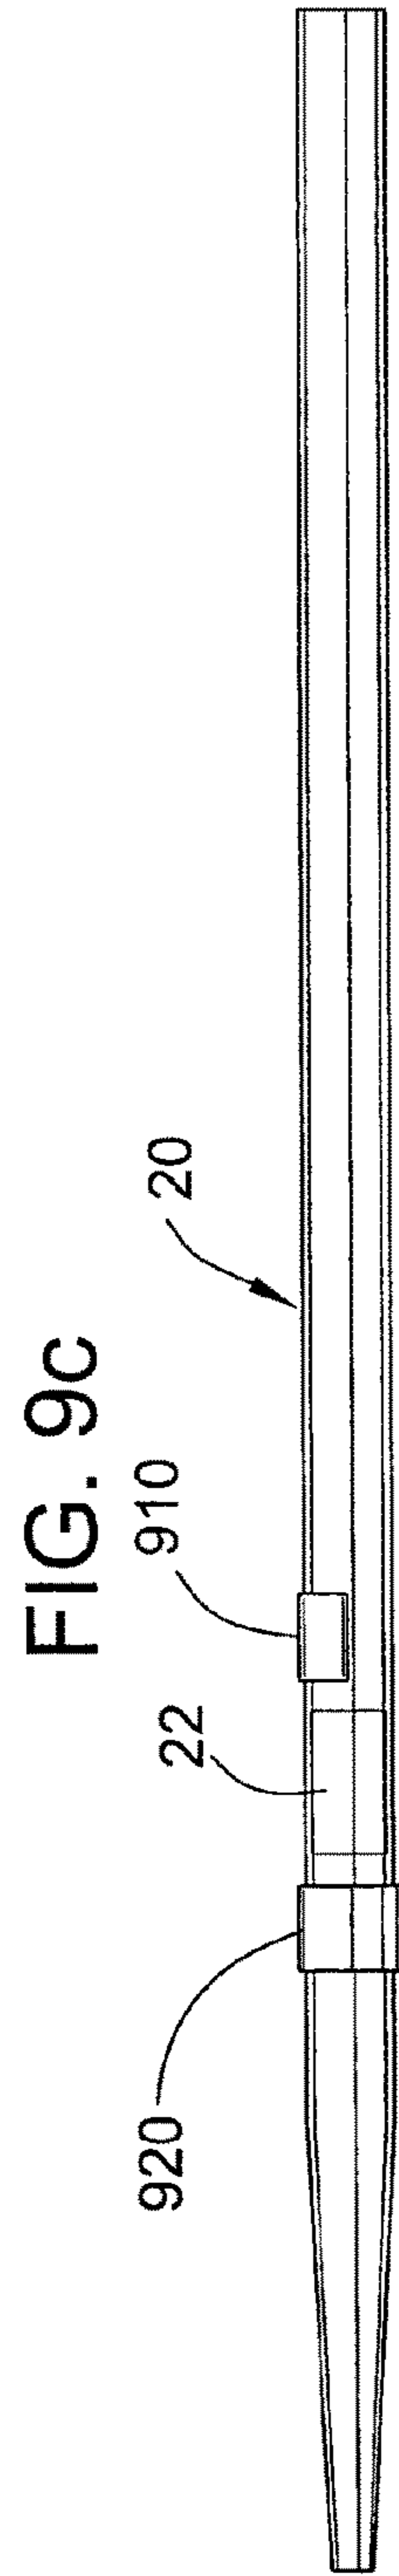
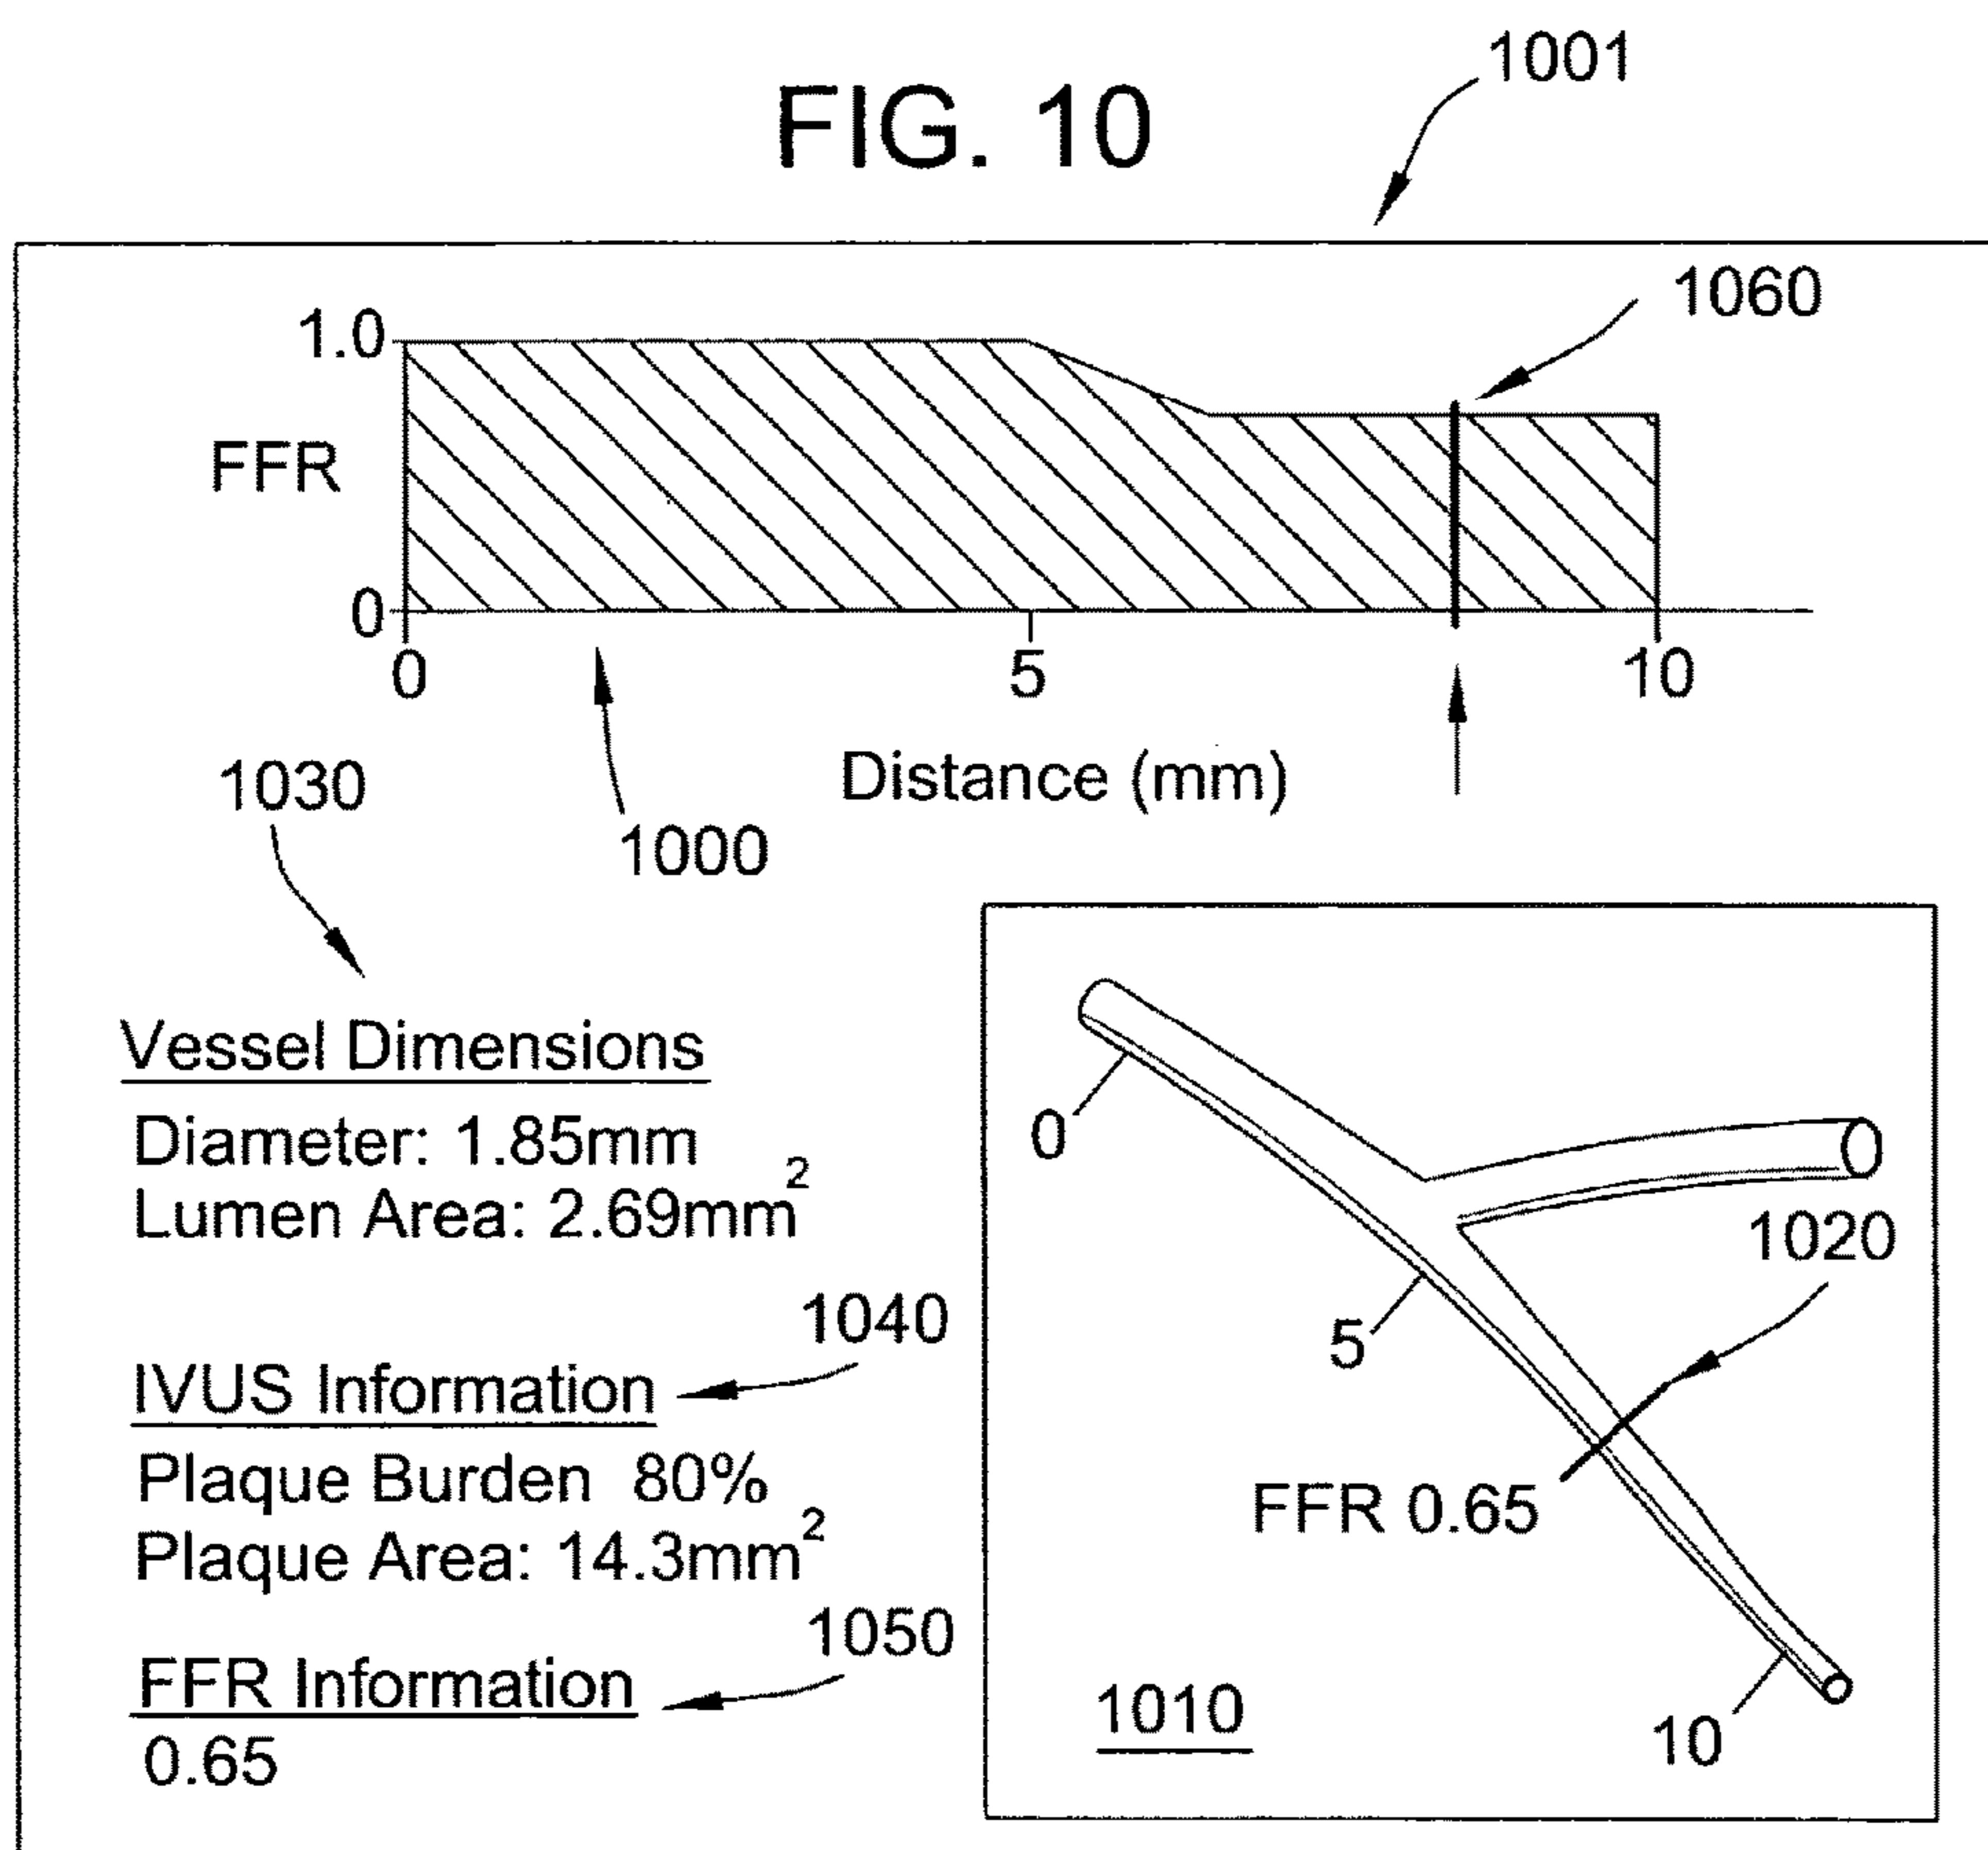


FIG. 10



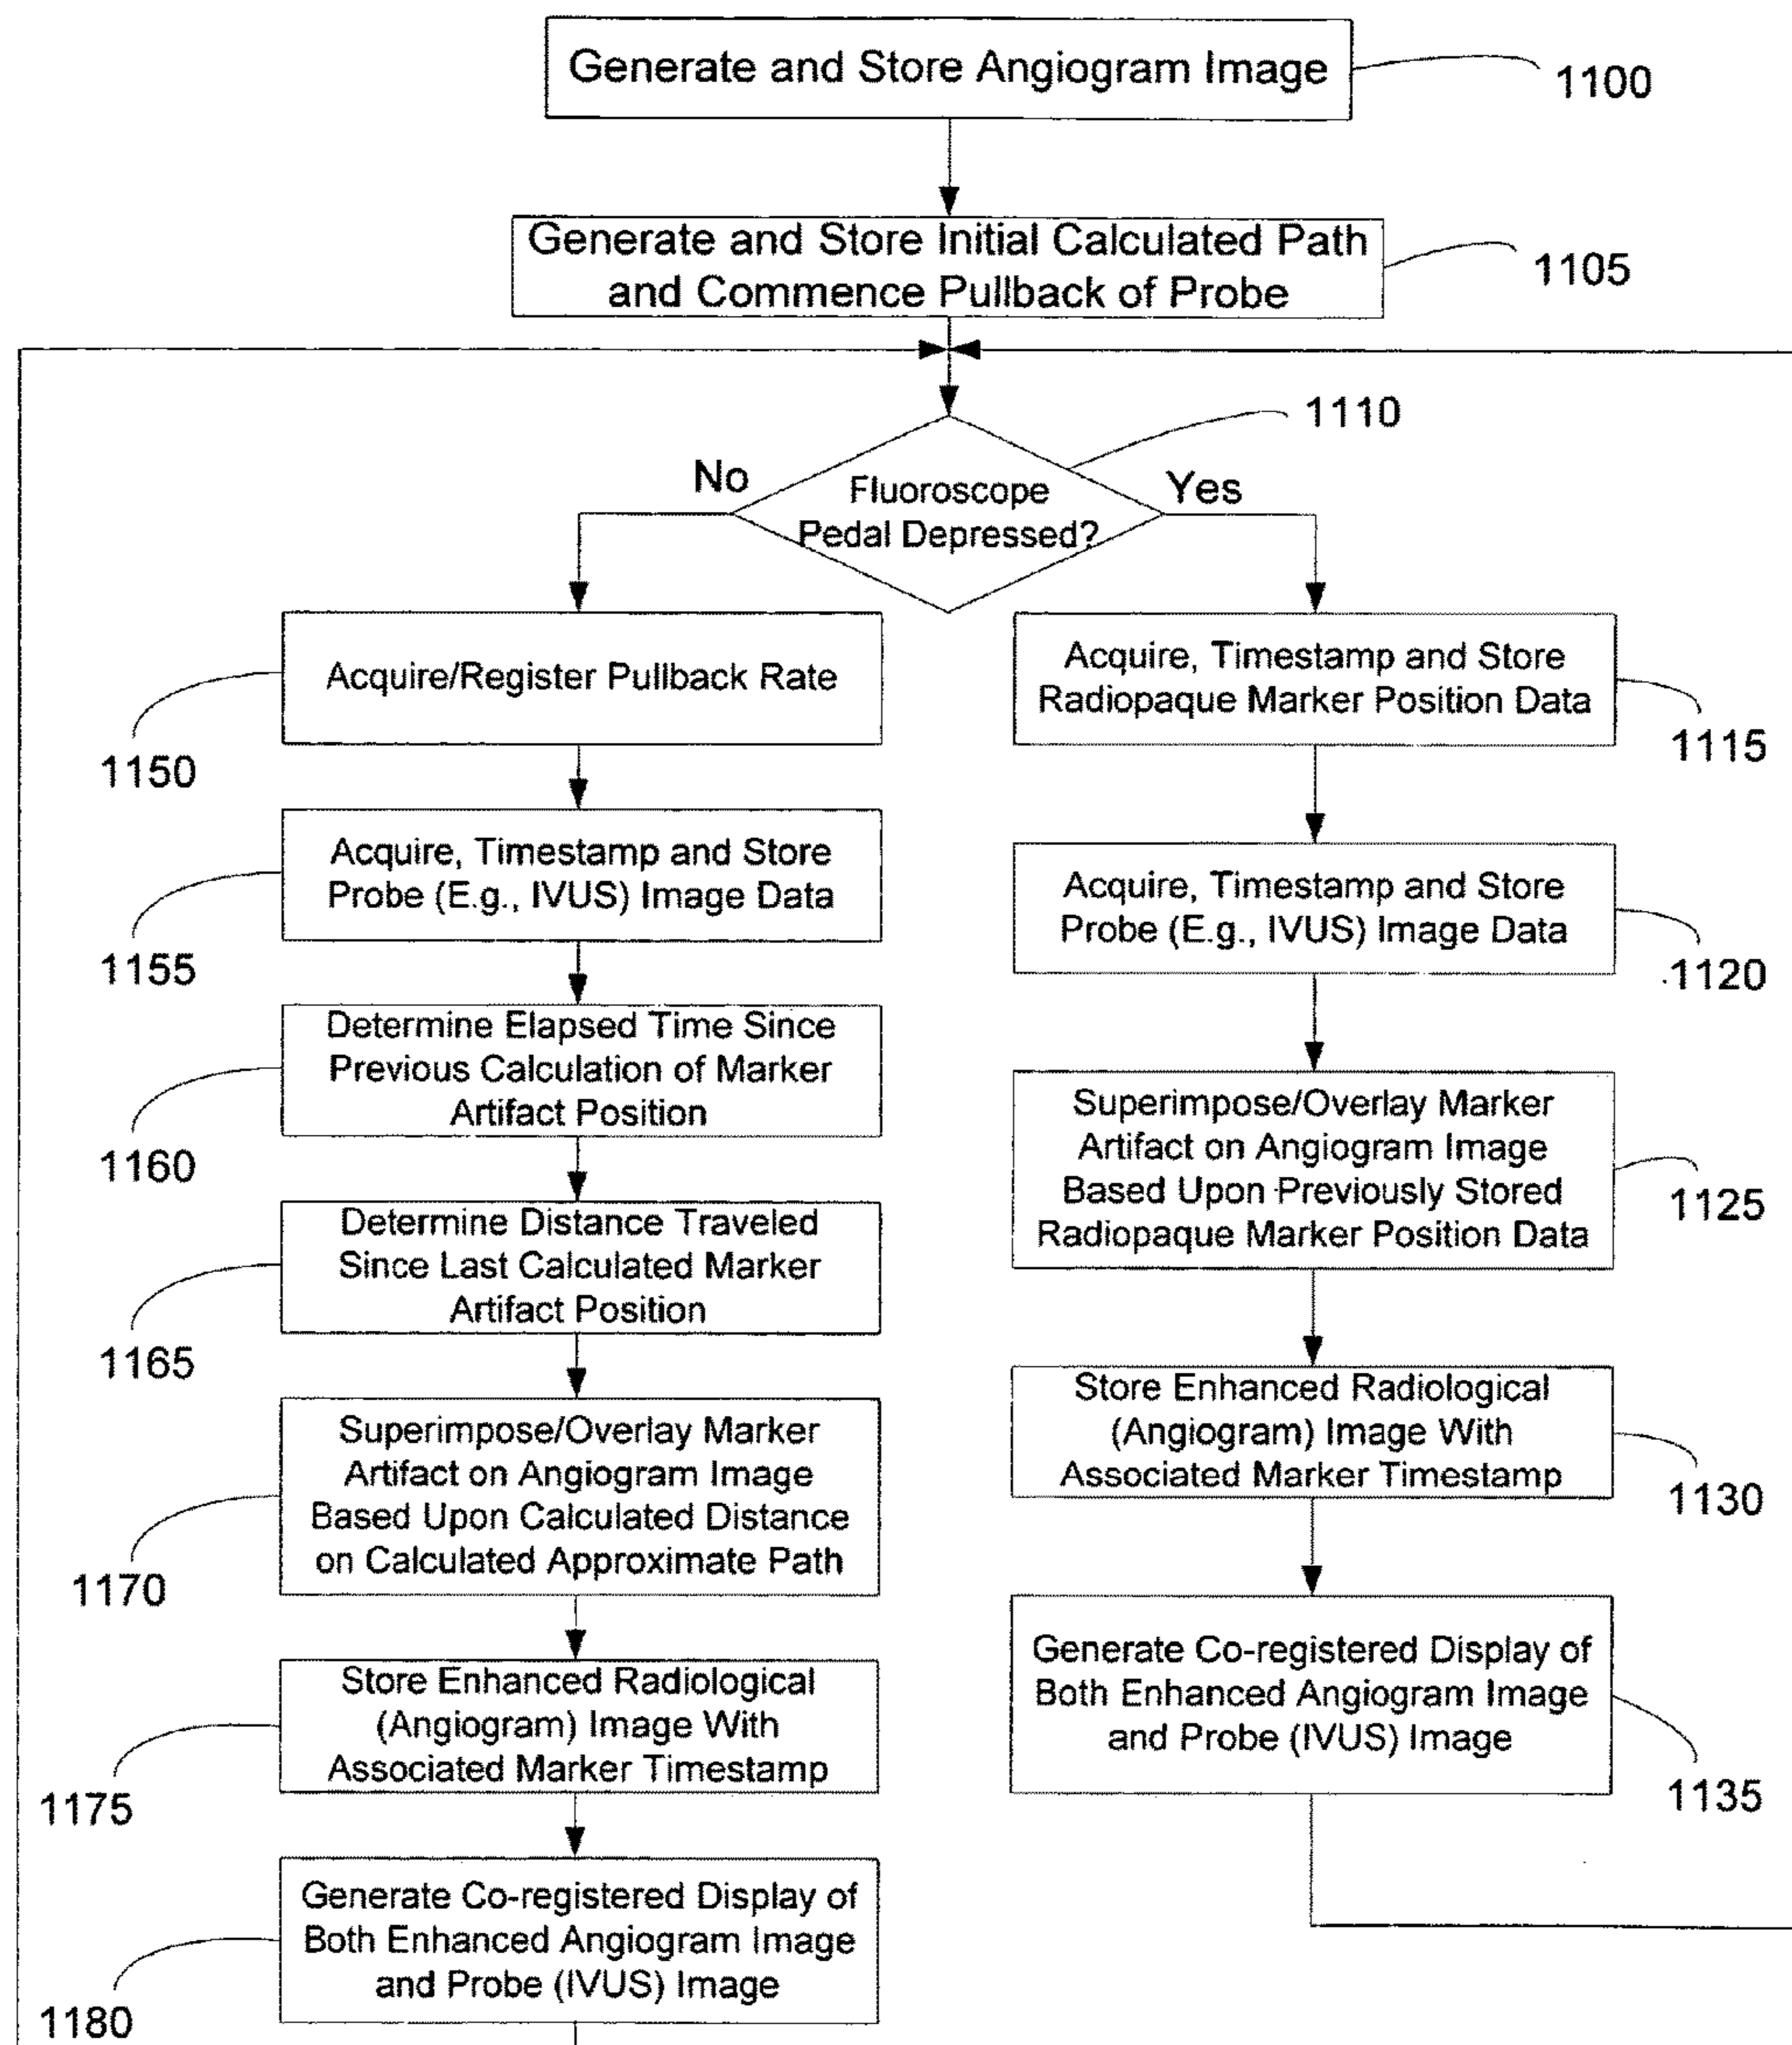


FIG. 11

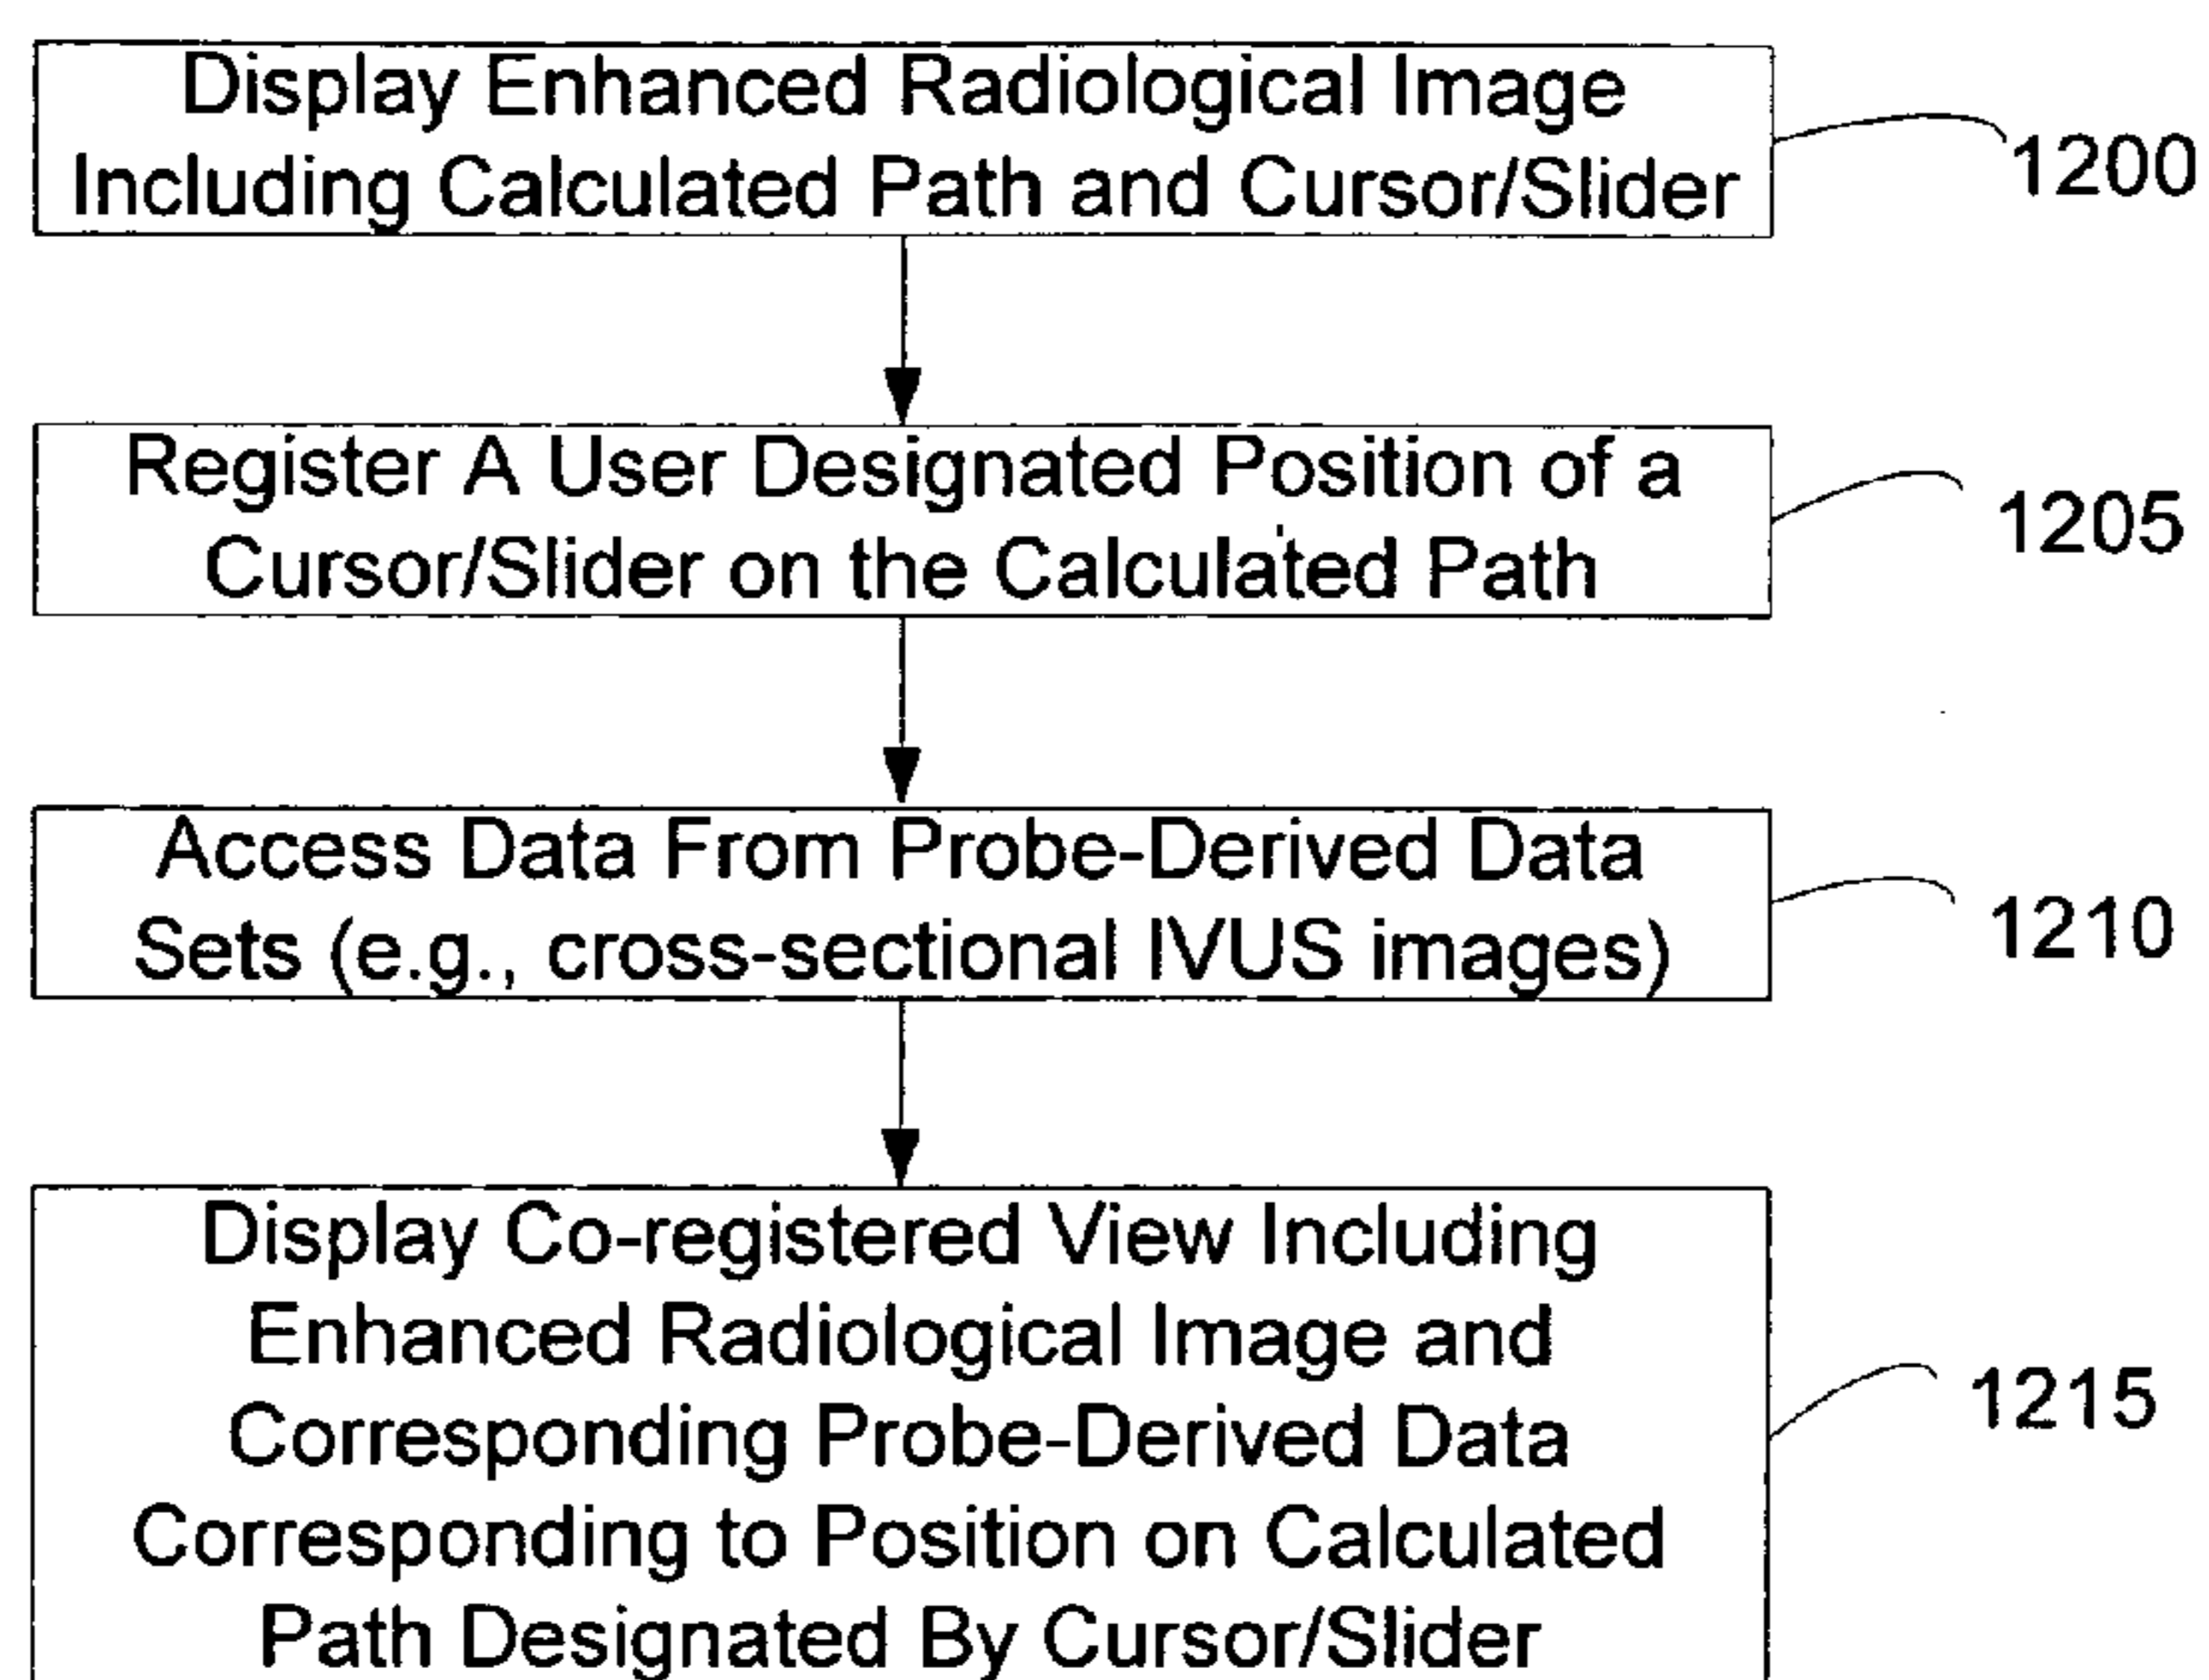


FIG. 12

VASCULAR IMAGE CO-REGISTRATION

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue; a claim printed with strikethrough indicates that the claim was canceled, disclaimed, or held invalid by a prior post-patent action or proceeding.

Notice: More than one reissue application has been filed for U.S. Pat. No. 7,930,014. The reissue applications are U.S. application Ser. No. 13/865,803, filed Apr. 18, 2013, and the present application, which is a continuation reissue of U.S. application Ser. No. 13/865,803.

CROSS-REFERENCE TO RELATED APPLICATION

This application is a continuation reissue of U.S. application Ser. No. 13/865,303, filed on Apr. 18, 2013, which in an application for reissue of U.S. Pat. No. 7,930,014, which claims priority of Huennekens et al. U.S. provisional application Ser. No. 60/642,893 filed on Jan. 11, 2005, entitled "Catheter Image Co-Registration," and Walker et al. U.S. provisional application Ser. No. 60/694,014 filed on Jun. 24, 2005, entitled "Three-Dimensional Co-Registration For Intravascular Diagnosis and Therapy", the contents of both of the above-identified provisional applications are expressly incorporated herein by reference in their entirety including the contents and teachings of any references contained therein.

AREA OF THE INVENTION

The present invention generally relates to imaging blood vessels. More particularly, the present invention is directed to methods and systems for generating composite displays relating a first image rendered from a first type of data and a second image rendered from a second type of data. A particular example of such composite display comprises an angiogram displayed along-side an IVUS image.

BACKGROUND OF THE INVENTION

In coronary arteries, vascular diseases including vessel lumen narrowing, usually due to atherosclerotic plaque, can lead to reduced blood flow to a heart muscle, angina (chest pain) and myocardial infarction—a heart attack. A variety of interventional treatments of cardiovascular disease are presently available to identify and treat such narrowing of a vessel lumen. Examples of such treatments include balloon angioplasty and/or deployment of stents. Diagnostic imaging is utilized to identify the extent and/or type of blockages within vessels prior to and/or during the treatment of such blockages. Diagnostic imaging enables doctors to ensure proper treatment of diseased vessels and verify the efficacy of such treatment.

In general, two distinct manners exist for generating diagnostic images for the identification and treatment of cardiovascular disease within a vasculature. A first manner of diagnostic imaging involves generating a radiological image of a stream flowing through a blood vessel's lumen from outside the vessel lumen. The purpose of generating an image of such flow is to identify blockages within diseased blood vessels that restrict blood flow. The extent of a

vessel's lumen is traditionally imaged using angiography, which involves rendering a two-dimensional view of one or more vessels within a portion of a patient's vasculature through which radiopaque contrast media has been injected.

The two-dimensional angiographic image can also be viewed real time by fluoroscopy. During such procedures, the images are potentially captured in various digital media, or in cine angiography (cine). Cine angiography, though rendering higher quality images of blood vessel lumens, exposes patients to high levels of ionizing radiation.

Fluoroscopy, generally using substantially less intense radiation than angiography, is used by physicians primarily to visually guide diagnostic and therapeutic catheters or guidewires, including one or more radiopaque markers, through vessels. The radiation intensity during fluoroscopy is typically one-tenth the intensity of radiation to which a patient is exposed during cine angiography. Many catheters have radiopaque markers that are viewable on a fluoroscope, thereby enabling a physician to track the location/path of such catheters as they are inserted within and/or withdrawn from patients. The platinum spring coil of guidewires also serves as a radiopaque marker. The lower radiation intensity of fluoroscopy allows a greater duration of use during a diagnostic/treatment procedure. However, due to its greater time of use, the total radiation exposure from fluoroscopy during an interventional treatment procedure can greatly exceed the radiation exposure during a typical cine angiography procedure. Thus, it is incumbent upon a physician to minimize the duration of time that a fluoroscope is used during a diagnostic and/or interventional treatment procedure.

The first manner of imaging, described above, has a number of drawbacks. For example, limited flow of contrast media near vessel walls and extreme variations in vessel cross-sections can result in incomplete filling of the vessel with a sufficient concentration of contrast media. As a consequence, the diameters of vessel segments can be misrepresented in an angiographic image. For example, a left main coronary artery cross-section is often underestimated by angiography. This can be problematic when attempting to judge the significance of a blockage within the vessel or when choosing the size of the treatment balloon or stent. An under-sized balloon or stent will not provide as effective treatment as a properly sized device. Furthermore, in angiography, a vessel's cross-section is determined by a two-dimensional view which may not accurately represent an actual extent of blood vessel narrowing.

Furthermore, to achieve an optimum treatment result, it is important to correctly determine a true target diameter of a native blood vessel—the diameter of a non-diseased blood vessel. However, angiography is ineffective in determining the target diameter of a vessel with disease along its entire length. For example, since vessels tend to taper in diameter along their length, a uniformly narrowed vessel may appear normal in an angiographic image.

Finally, angiography does not facilitate differentiating between different types of tissue found in atherosclerotic plaque. For example, in coronary arteries prone to producing a heart attack, necrotic tissue is thought to be more prevalent than purely fibrous tissue. Thus, while providing a good way to identify severe blockages, angiography is not always the best diagnostic imaging tool due to the incomplete nature of the angiographic image data.

The second manner of intravascular imaging comprises imaging the vessel itself using a catheter-mounted intravascular probe. Intravascular imaging of blood vessels provides a variety of information about the vessel including: the

cross-section of the lumen, the thickness of deposits on a vessel wall, the diameter of the non-diseased portion of a vessel, the length of diseased sections, and the makeup of the atherosclerotic plaque on the wall of the vessel.

Several types of catheter systems have been designed to track through a vasculature to image atherosclerotic plaque deposits on vessel walls. These advanced imaging modalities include, but are not limited to, intravascular ultrasound (IVUS) catheters, magnetic resonance imaging (MRI) catheters and optical coherence tomography (OCT) catheters. In addition, thermography catheters and palpography catheters have also been demonstrated to generate vessel image data via intravascular probes. Other catheter modalities that have been proposed include infrared or near-infrared imaging.

In operation, these intravascular catheter-mounted probes are moved along a vessel in the region where imaging is desired. As the probe passes through an area of interest, sets of image data are obtained that correspond to a series of "slices" or cross-sections of the vessel, the lumen, and surrounding tissue. As noted above, the catheters include radiopaque markers. Such markers are generally positioned near a distal catheter tip. Therefore, the approximate location of the imaging probe can be discerned by observing the catheterization procedure on either a fluoroscope or angiographic image. Typically imaging catheters are connected to a dedicated console, including specialized signal processing hardware and software, and display. The raw image data is received by the console, processed to render an image including features of concern, and rendered on the dedicated display device.

For example, IVUS images used to diagnose/treat vascular disease generally comprise sets of cross-sectional image "slices" of a vessel. A grayscale cross-sectional slice image is rendered, at each of a set of positions along the vessel based upon the intensity of ultrasound echoes received by an imaging probe. Calcium or stent struts, which produce relatively strong echoes, are seen as a lighter shade of gray. Blood or vessel laminae, which produce weaker echoes, are seen as a darker shade of gray.

Atherosclerotic tissue is identified as being the portion of a cross-sectional image between an internal elastic lamina (IEL) and an external elastic lamina (EEL). The ability to see the vessel lumen, and calculate its dimensions, allows the diameters and cross-sectional area of the vessel to be determined more reliably than the limited two-dimensional angiography. Because IVUS does not rely upon dispersing a contrast agent, IVUS is especially useful in generating images of the left main coronary artery as described above. Furthermore, the ability to view the EEL, and calculate its dimensions, allows an IVUS image to render a more reliable determination than angiography, of the correct diameter and length of the balloon or stent to use when restoring proper blood flow to a blocked/diseased vessel. Advanced IVUS images have also been described which perform tissue characterization and denote different types of tissue with a color code. One such modality is described in Vince, U.S. Pat. No. 6,200,268. Like IVUS, the other catheters mentioned above display a series of cross-sectional images from which additional information can be obtained.

Catheter-mounted probes, and in particular, IVUS probes can be configured to render a variety of two and three-dimensional images. In addition to the two-dimensional transverse cross-sectional images discussed above, a longitudinal planar image can be constructed from a plane which cuts through a "stack" of cross-section "slices". In addition, three-dimensional "fly-through" images can be constructed from information in a series of cross-sectional slices of a

vessel. Though these three-dimensional images can be visually impressive, the two dimensional angiography image remains the primary basis for determining the location of a catheter in a vessel, and the "schematic" reference through which the physician plans and carries out a treatment procedure.

In creating the "stack" or "flythrough" images, some assumptions are made by image data processing software in terms of the orientation of each slice to the next. In many cases the compound images, rendered from a series of transverse cross-sectional slices, are rendered in the form of a straight vessel segment. In reality, vessels can curve significantly. In segment visualizations that render straight segments, spatial orientation of each cross-sectional slice in relation to other slices is not measured. In addition, the rotational orientation of a catheter-mounted probe is generally not known due to twisting of the catheter as it passes through a vessel. Therefore, the angular relation between adjacent slices is not generally known. In many cases, these limitations do not significantly effect treatment of a diseased vessel because the typical treatment modalities (balloons, stents) are not circumferentially specific. A balloon, for example, dilates a vessel 360° around a lumen.

In view of the advantages provided by the two above described methods of imaging vessels, many catheter labs use both methods simultaneously to diagnose and treat a patient. However, an angiographic image provided on a different display monitor than a corresponding IVUS image (or the other image rendered by a catheter-mounted probe), presents challenges to a obtaining a comprehensive understanding of a state of a diseased vessel. For example, a physician identifies specific structures (e.g. feeder vessels) in cross-sectional images in order to determine a location on a vessel presented on an angiography display that needs to be treated. Coordinating images rendered by two distinct display devices can become cumbersome as the physician refers back and forth between two different screens on two distinct display devices. In addition, when a video loop of IVUS images is recorded, to be played back later on a machine, a corresponding angiographic image is not recorded in sync with it. Therefore, during playback, the specific cross-section being viewed needs to be compared to the vessel angiography, which is usually on a separate file.

A known visualization display simultaneously provides an angiogram, an IVUS transverse plane view, and an IVUS longitudinal plane view. A red dot is placed upon the angiogram corresponding to a currently displayed IVUS transverse plane view. A blue line is placed upon the angiogram corresponding to a currently displayed longitudinal plane view. The reference dot and line are only as valuable as the accuracy of the process that registers their positions on the angiogram.

SUMMARY OF THE INVENTION

In order to provide a better overall view of vascular systems, in accordance with the present invention, a system and method include a single display simultaneously providing a first view of a patient including an angiogram image and a second view including an intravascular image rendered from information provided by an imaging probe mounted on a distal end of a flexible elongate member. A cursor, having a position derived from image information provided by a radiopaque marker proximate the imaging probe, is displayed within the angiogram image to correlate the position of the imaging probe to a presently displayed intravascular image and thus provide an easily discernable

identification of a position within a patient corresponding to a currently displayed intravascular image. The resulting composite display simultaneously provides: an intravascular image that includes information about a vessel that is not available from an angiogram and a current location within a vessel of a source of intravascular image data from which the intravascular image is rendered.

BRIEF DESCRIPTION OF THE DRAWINGS

While the claims set forth the features of the present invention with particularity, the invention, together with its objects and advantages, may be best understood from the following detailed description taken in conjunction with the accompanying drawing of which:

FIG. 1 is a schematic illustration of a system for implementing catheter image co-registration;

FIG. 2 depicts an illustrative angiogram image;

FIG. 3 depicts an illustrative fluoroscopic image of a radiopaque marker mounted upon a catheter;

FIG. 4 depicts an illustrative enhanced radiological image along-side a cross-sectional IVUS image;

FIG. 5 depicts an illustrative enhanced radiological image along-side a cross-sectional IVUS image wherein the radiological image further includes a calculated path within a vessel of interest;

FIG. 6 depicts an illustrative enhanced radiological image along-side a cross-sectional IVUS image wherein the radiological image further includes a calculated path within a vessel of interest with a marker positioned at a different location than the view of FIG. 5;

FIG. 7 depicts an illustrative enhanced radiological image along-side a cross-sectional IVUS image wherein the radiological image further includes a calculated path within a vessel of interest and a reference mark providing a point of synchronization/calibration of a marker position;

FIG. 8 depicts an illustrative catheter distal end including a single cylindrical radiopaque marker band;

FIG. 9a depicts a radiopaque marker band 900, suitable for use in an exemplary embodiment, that partially encircles the catheter shaft;

FIG. 9b depicts an imaging catheter having two of the radiopaque marker bands of the type depicted in FIG. 9a wherein the two bands are skewed by a quarter rotation along the axis of the catheter;

FIG. 9c depicts the imaging catheter of 9b from a view that looks directly on the full surface of the distal marker band 920;

FIG. 9d depicts the imaging catheter of 9c at a view wherein the catheter is axially rotated 90 degrees from the position depicted in FIG. 9c;

FIG. 9e depicts the imaging catheter at a different rotational position from FIG. 9c and FIG. 9d;

FIG. 10 depicts an illustrative display for co-registration of radiological and hemodynamic image information;

FIG. 11 is a flowchart summarizing a set of steps for rendering and displaying a co-registered view during a data acquisition procedure; and

FIG. 12 is a flowchart summarizing a set of steps for rendering and displaying a co-registered view during playback of previously acquired image data.

DETAILED DESCRIPTION OF THE DRAWINGS

In accordance with embodiments of the present invention, a method and system are described by way of example herein below including image data acquisition equipment

and data/image processors that generate views on a single display that simultaneously provides positional information and intravascular images associated with a imaging probe (e.g., an IVUS transducer probe) mounted upon a flexible elongate member (e.g, a catheter, guidewire, etc.).

Turning initially to FIG. 1, an exemplary system is schematically depicted for carrying out the present invention in the form of co-registration of angiogram/fluoroscopy and intravascular ultrasound images. The radiological and ultrasound image data acquisition sub-systems are generally well known in the art. With regard to the radiological image data, a patient 10 is positioned upon an angiographic table 12. The angiographic table 12 is arranged to provide sufficient space for the positioning of an angiography/fluoroscopy unit c-arm 14 in an operative position in relation to the patient 10 on the table 12. Radiological image data acquired by the angiography/fluoroscopy c-arm 14 passes to an angiography/fluoroscopy processor 18 via transmission cable 16. The angiography/fluoroscopy processor 18 converts the received radiological image data received via the cable 16 into angiographic/fluoroscopic image data. The angiographic/fluoroscopic (“radiological”) image data is initially stored within the processor 18.

With regard to portions of the system associated with acquiring ultrasound image data, an imaging catheter 20, and in particular an IVUS catheter, is inserted within the patient 10 so that its distal end, including a diagnostic probe 22 (in particular an IVUS probe), is in the vicinity of a desired imaging location of a blood vessel. While not specifically identified in FIG. 1, a radiopaque material located near the probe 22 provides indicia of a current location of the probe 22 in a radiological image. By way of example, the diagnostic probe 22 generates ultrasound waves, receives ultrasound echoes representative of a region proximate the diagnostic probe 22, and converts the ultrasound echoes to corresponding electrical signals. The corresponding electrical signals are transmitted along the length of the imaging catheter 20 to a proximal connector 24. IVUS versions of the probe 22 come in a variety of configurations including single and multiple transducer element arrangements. In the case of multiple transducer element arrangements, an array of transducers is potentially arranged: linearly along a lengthwise axis of the imaging catheter 20, curvilinearly about the lengthwise axis of the catheter 20, circumferentially around the lengthwise axis, etc.

The proximal connector 24 of the catheter 20 is communicatively coupled to a catheter image processor 26. The catheter image processor 26 converts the signals received via the proximal connector 24 into, for example, cross-sectional images of vessel segments. Additionally, the catheter image processor 26 generates longitudinal cross-sectional images corresponding to slices of a blood vessel taken along the blood vessel’s length. The IVUS image data rendered by the catheter image processor 26 is initially stored within the processor 26.

The type of diagnostic imaging data acquired by the diagnostic probe 22 and processed by the catheter image processor 26 varies in accordance with alternative embodiments of the invention. In accordance with a particular alternative embodiment, the diagnostic probe 22 is equipped with one or more sensors (e.g., Doppler and/or pressure) for providing hemodynamic information (e.g., blood flow velocity and pressure)—also referred to as functional flow measurements. In such alternative embodiments functional flow measurements are processed by the catheter image processor 26. It is thus noted that the term “image” is intended to be broadly interpreted to encompass a variety of

ways of representing vascular information including blood pressure, blood flow velocity/volume, blood vessel cross-sectional composition, shear stress throughout the blood, shear stress at the blood/blood vessel wall interface, etc. In the case of acquiring hemodynamic data for particular portions of a blood vessel, effective diagnosis relies upon the ability to visualize a current location of the diagnostic probe **22** within a vasculature while simultaneously observing functional flow metrics indicative of cardiovascular disease. Co-registration of hemodynamic and radiological images facilitates precise treatment of diseased vessels. Alternatively, instead of catheter mounted sensors, the sensors can be mounted on a guidewire, for example a guidewire with a diameter of 0.018" or less. Thus, in accordance with embodiments of the present invention, not only are a variety of probe types used, but also a variety of flexible elongate members to which such probes are mounted at a distal end (e.g., catheter, guidewire, etc.).

A co-registration processor **30** receives IVUS image data from the catheter image processor **26** via line **32** and radiological image data from the radiological image processor **18** via line **34**. Alternatively, the communications between the sensors and the processors are carried out via wireless media. The co-registration processor **30** renders a co-registration image including both radiological and IVUS image frames derived from the received image data. In accordance with an embodiment of the present invention, indicia (e.g., a radiopaque marker artifact) are provided on the radiological images of a location corresponding to simultaneously displayed IVUS image data. The co-registration processor **30** initially buffers angiogram image data received via line **34** from the radiological image processor **18** in a first portion **36** of image data memory **40**. Thereafter, during the course of a catheterization procedure IVUS and radiopaque marker image data received via lines **32** and **34** is stored within a second portion **38** and a third portion **42**, respectively, of the image data memory **40**. The individually rendered frames of stored image data are appropriately tagged (e.g., time stamp, sequence number, etc.) to correlate IVUS image frames and corresponding radiological (radiopaque marker) image data frames. In an embodiment wherein hemodynamic data is acquired rather than IVUS data, the hemodynamic data is stored within the second portion **38**.

In addition, additional markers can be placed on the surface of the patient or within the vicinity of the patient within the field of view of the angiogram/fluoroscope imaging device. The locations of these markers are then used to position the radiopaque marker artifact upon the angiographic image in an accurate location.

The co-registration processor **30** renders a co-registration image from the data previously stored within the first portion **36**, second portion **38** and third portion **42** of the image data memory **40**. By way of example, a particular IVUS image frame/slice is selected from the second portion **38**. The co-registration processor **30** identifies fluoroscopic image data within the third portion **42** corresponding to the selected IVUS image data from the second portion **38**. Thereafter, the co-registration processor **30** superimposes the fluoroscopic image data from the third portion **42** upon the angiogram image frame retrieved from the first portion **36**. Thereafter, the co-registered radiological and IVUS image frames are simultaneously displayed, along-side one another, upon a graphical display device **50**. The co-registered image data frames driving the display device **50** are also stored upon a long-term storage device **60** for later review in a session

separate from a procedure that acquired the radiological and IVUS image data stored in the image data memory **40**.

While not shown in FIG. **1**, a pullback device is incorporated that draws the catheter **20** from the patient at a controlled/measured manner. Such devices are well known in the art. Incorporation of such devices facilitates calculating a current position of the probe **22** within a field of view at points in time when fluoroscopy is not active.

Turning to FIG. **2**, the angiography/fluoroscopy processor **18** captures an angiographic "roadmap" image **200** in a desired projection (patient/vessel orientation) and magnification. By way of example, the image **200** is initially captured by an angiography procedure performed prior to tracking the IVUS catheter to the region of interest within a patient's vasculature. Performing the angiography procedure without the catheter **20** in the vessel provides maximal contrast flow, better vessel filling and therefore a better overall angiogram image. Thus, side branches such as side branch **210** and other vasculature landmarks can be displayed and seen clearly on the radiological image portion of a co-registered image displayed upon the graphical display device **50**.

Turning to FIG. **3**, the catheter **20** is tracked to its starting position (e.g., a position where an IVUS pullback procedure begins). Typically the catheter **20** is tracked over a previously advanced guidewire (not shown). Thereafter, a fluoroscopic image is obtained. In the image, the catheter radiopaque marker **300** is visualized, but the vessel lumen is not, due to the absence of contrast flow. However, a set of locating markers present in both the angiogram and fluoroscopy images enable proper positioning (superimposing) of the marker image within the previously obtained angiogram image. Other ways of properly positioning the radiopaque marker image within the field of view of the angiogram image will be known to those skilled in the art in view of the teachings herein. Furthermore, the marker artifact can be automatically adjusted (both size and position) on the superimposed image frames to correspond to the approximate position of the transducers. The result of overlaying/superimposing the radiopaque marker artifact upon the angiogram image is depicted, by way of example in an exemplary co-registration image depicted in FIG. **4**.

Turning to FIG. **4** the exemplary co-registration display **401** (including the correlated radiological and IVUS images) depicts a selected cross-sectional IVUS image **400** of a vessel. A radiological image **410** is simultaneously displayed along-side the IVUS image **400** on the display **50**. The radiological image **410** includes a marker artifact **420**, generated from radiological image data rendered by a fluoroscope image frame, superimposed on an angiogram background rendered from the first portion **36** of the memory **40**. The fluoroscope image frame corresponds to the current location of the diagnostic probe **22** within a vessel under observation. Precise matching of the field of view represented in both the angiogram and fluoroscope images (i.e., precise projection and magnification of the two images) allows identification of the current position of the IVUS probe corresponding to the displayed IVUS image **400** in the right pane of the co-registered images displayed in FIG. **4**.

Alternatively, the composite radiological image **410** is obtained in one step. In such case, the original roadmap angiogram image is obtained with the catheter already in its starting position. However, once obtained, the angiogram image is reused as the IVUS probe is withdrawn from the vessel.

The system also takes heart motion into account when generating/acquiring the radiological and IVUS image data.

By way of example, by acquiring the image data for both the angiogram (background) and the radiopaque marker only during the peak R-wave of the EKG, heart motion is much less a factor and good overlay correlation exists between the angiogram and fluoroscope fields of view. The peak R-wave is selected because it represents end-diastole, during which the heart has the least amount of motion, and thus, a more consistent condition from which to obtain the radiological image data. The peak R-wave is also an easy point in the EKG for the system to detect.

With continued reference to FIG. 4, in an exemplary embodiment when the IVUS catheter **20** begins to image, the cross-sectional image **400** from the IVUS catheter is displayed in tandem with the enhanced radiological image **410** including both the angiogram background and the superimposed marker artifact **420**. The enhanced radiological image **410** and the cross-sectional IVUS image **400** are displayed close to (e.g., along side) each other on the display **50**, so that the operator can concentrate on the information in the cross-sectional image **400** while virtually simultaneously observing the status of the enhanced radiological image **410**.

The simultaneous display of both the composite/enhanced radiological image and the cross-sectional image allows instant awareness of both disease state of a vessel segment and the location of the vessel segment within a patient. Such comprehensive information is not readily discernable in a three dimensional flythrough image or a stacked longitudinal image. Neither flythrough nor stacked images alone allows for the simultaneous appreciation of 1) all of the information in a cross-section, 2) a feel for the shape of the vessel and 3) the location of the cross-section along the length of the vessel. The above-described "co-registration" of enhanced angiographic (including the marker artifact) and intravascular cross-sectional images/information delivers all three of these items in a presentation that is straight forward to an operator with even average visual and spatial abilities. The co-registration display is presented, by way of example, either on an IVUS console display, or the co-registration display is presented on one or more angiographic monitors, either in the room where the procedure is occurring or in a remote location. For example, one monitor over the table in the procedure room allows the attending physician to view the procedure, while at the same time a second consulting physician who has not scrubbed for the case is also able to view the case via a second monitor containing the co-registration display from a separate control room. Control room viewing is also possible without having to wear leaded covering.

With regard to the persistence of the background angiogram ("roadmap") image portion of the enhanced radiological image **410**, a single angiogram image is, by way of example, obtained/generated and stored in the first portion **36** of the memory **40** for a given procedure/patient position. If the field of view changes or the patient's position changes, then an updated background angiogram image is generated and stored in the first portion **36**. Alternatively, the background angiogram image is live or continuously updated, for example, at each additional step in which angiography is performed. The projection of the angiogram roadmap/background image portion of the enhanced radiological image **410** is preferably in an orientation and magnification that best displays the entire vessel to be viewed, taking into account the foreshortening that is present in a tortuous/winding vessel. Alternatively, two roadmap images (or even two enhanced radiological images **410**) can be used/displayed in place of the one image **410**. Such multiple views are provided in the context of biplane angiography.

Establishing a position for the marker artifact within the field of the enhanced radiological image, based at least in part upon a radiopaque marker on the imaging catheter **20** is achievable in a variety of ways. Examples, described further herein below include: user-specified points (by clicking at a position near the marker to establish a point); image pattern recognition (automatic identification of a marker's unique signature within a field of view); and combinations of manual and automated calculations of a path.

Enhancing the background/roadmap angiogram image to render the image **410** is achieved in a number of different ways. As mentioned above, in an illustrative embodiment, the marker artifact **420** (derived from a fluoroscope image of a radiopaque marker near the probe **22** mounted on the distal end of the catheter **20**) is superimposed upon/overlays the angiogram/roadmap background of the enhanced radiological image **410**. Because the live/marker artifact portion of the image **410** requires that fluoroscopy be performed the entire time of catheter movement (e.g. pullback), in an alternative embodiment, the marker artifact is displayed on the image **410** only during those periods when the fluoroscope is active. When the fluoroscope is inactive, only the background angiogram is presented on the enhanced image **410** of the display **50**.

Turning to FIGS. 5 and 6, in embodiments of the invention, when the fluoroscope is inactive, the co-registration processor **30** calculates an approximate location of the radiopaque marker based upon its last registered position and other indicators of catheter movement (e.g., pullback distance sensors/meters). The approximate location is utilized in place of the radiopaque marker image to render a marker artifact **520** on an enhanced radiological image **510** displayed along-side a corresponding IVUS cross-sectional image **500** within a display **501**. By way of a particular illustrative example, during periods in which a fluoroscope is inactive, the marker artifact **520**'s position is calculated by software/hardware within the co-registration processor **30** from sensor data indicative of a current/changed location of the radiopaque marker within the current image field provided by the current background angiogram image. In an embodiment of the invention, a visual characteristic (e.g., color, symbol, intensity, etc.) of the marker artifact **520** is used to distinguish when the fluoroscope is active/inactive and thus indicate whether the marker artifact position is actual/calculated. Furthermore, in more advanced systems, both the displacement and angular orientation of the marker (and thus the diagnostic probe **22**) are determined to render accurate approximations of the current position of the diagnostic probe **22** within a vessel as it acquires data for generating the image **500**.

With continued reference to FIGS. 5 and 6, a calculated path **550/650** is determined by the co-registration processor **30** within displays **501/601**. A marker artifact **520/620** is placed on top of the calculated path **550/650**. The marker artifact **520/620** is superimposed on the angiogram image at a location calculated from non-visual position data (e.g., pullback distance, spatial position sensors, angular orientation sensors, etc.). For example, if the initial location of a radiopaque marker within the enhanced radiological image **510/610** is known and the catheter is pulled by an automatic pullback system at a specific rate for a known amount of time, the cursor can be placed by the system at a distance from the initial location along the calculated path **550/650** that represents the product of the pullback rate and the time period. Furthermore, each subsequent time that a fluoroscope is activated and an image of the radiopaque marker is acquired and presented to the co-registration processor **30**,

an error between the actual radiopaque marker location and a current calculated marker artifact **520/620** location is eliminated by replacing the calculated position by a position calculated by the radiopaque marker image. The error between the corrected position and the calculated location of the marker artifact **520/620** is determined. In an exemplary embodiment, the error/total travel distance ratio is used as a scaling factor to recalculate and adjust all previously calculated/rendered/presented marker artifact overlay positions on the rendered/stored copies of the enhanced radiological image **510/610** for the entire preceding period in which the fluoroscope has been inactive.

Similarly, a re-calculation can also update a shape of the calculated path **550/560** curve. As seen in FIGS. **5** and **6**, the calculated path **550/650** is shown as a curve that matches the tortuosity of a vessel through which the probe **22** passes—represented by a center line through the displayed vessel. Alternatively, the catheter paths within vessels take a straighter and shorter path than the centerline of a blood vessel when pulled through such vessel. If, however, the catheter is being translated by pushing, instead of pulling, the calculated path **550/650** more closely matches the curvature of the vessel, or even exaggerates the tortuosity of the vessel by taking a longer path. A multiplication coefficient (e.g., 1.05 for pushing, 0.95 for pulling) can be introduced when calculating a path based upon this general observation of the path taken by a probe as it is pushed/pulled through a vessel. The path can alternatively be calculated from two different angiographic images taken at different projections (planes). This allows a three dimensional angiographic image, from which a true centerline can be calculated.

In accordance with yet another embodiment, represented by the co-registered IVUS image **700** and enhanced radiological image **710** in a display **701** presented in FIG. **7**, the operator creates a reference mark **760** at one or more points on a calculated path **750**. The reference mark **760** serves a variety of potential uses. By way of example, the reference mark **760** potentially serves as a benchmark (location synchronization point) for updating position of a marker artifact **720** within the enhanced radiological image **710**. In the embodiment represented by FIG. **7**, the co-registration processor **30** waits for manual input of the reference mark **760** location information prior to proceeding with calculations. The user creates the reference mark **760** which coincides with a marker artifact **720** rendered from image data provided by a fluoroscope of a field of view containing a radiopaque marker. The reference mark **760**, which potentially persists beyond its initial entry period, is distinguished from the marker artifact **720** which follows the current/estimated position of the probe **22**. Furthermore, in an exemplary embodiment the reference mark is used to highlight/mark actual positions of the probe **22** (rendered by a fluoroscope image of a radiopaque marker) as opposed to estimated points on a calculated point (e.g. points on a path e.g., **550/560**) from merely calculated position estimates upon the paths **550/560**. In yet other embodiments, the reference mark **760** is used to highlight a particular point of interest during a diagnostic/treatment procedure. A bookmark is placed within a series of cross-sectional images associated with the IVUS image **700** portion of the display **701**. The bookmark allows quick access to a particular archived image frame corresponding to the reference mark **760** in the display **701**.

In accordance with embodiments of the present invention, a user interface associated with the displayed images provided in FIGS. **4-7** includes a “slider” control that allows an operator to track through a series of stored frames repre-

sented sequentially acquired data along a traversed path within a vessel. The slider control can be a set of arrows on a keyboard, a bar/cursor displayed upon an enhanced radiological image that can be manipulated by an operator, during playback, using a mouse or other user interface device to traverse a vessel segment, etc. By way of example, a display similar to FIG. **7** is rendered by the co-registration processor **30** during playback of a previous data acquisition session. A cursor similar to the reference mark **760** is displayed during playback on the enhanced radiological image **710**. A user selects and drags the cursor along a path similar to the calculated path **750**. As the user drags and drops the cursor along the path, the co-registration processor **30** acquires and presents corresponding co-registered images. The user sequentially proceeds through the stored images using, by way of example, arrow keys, mouse buttons, etc.

It is noted that various catheter marking schemes are contemplated that improve/optimize the co-registration processor **30**'s calculations of a position of the marker artifact (representing a position within a vessel corresponding to a currently displayed IVUS cross-section image) when the fluoroscope is inactive. Turning to FIG. **8**, a single radiopaque marker band **800** is attached to the catheter **820** near an IVUS probe. The radiopaque band **800** includes a proximal edge **802** and a distal edge **804**. The band **800** is cylindrical, with the diameter at the proximal edge **802** equal to the diameter at the distal edge **804**. In addition, the band **800** has a known length.

Upon connection of the proximal connector **24** of the catheter **20** into an outlet on the catheter image processor **26** (or an interposed patient interface module which is communicatively connected to the processor **26**), the processor **26** receives identification information from the catheter **20** via EPROM, RFID, optical reader or any other appropriate method for identifying the catheter **20**. In an illustrative embodiment, the catheter length and diameter dimensions (or dimension ratio) are included in the received identification information. In addition, image field information such as magnification and/or projection angle) from the radiological image processor **18** is provided to the co-registration processor **30**. By identifying four points at the corners of an approximate four-sided polygon of the marker band image, the co-registration processor **30** automatically calculates foreshortening of a vessel in an enhanced radiological image view and the true length of a segment of a calculated path.

Turning briefly to FIGS. **9a-e**, a catheter **920** carries two marker bands having a known linear separation distance that facilitates making the calculations described herein above with reference to FIG. **8**. FIG. **9a** shows a radiopaque marker band **900**, suitable for use in an exemplary embodiment, that partially encircles the catheter shaft; In the exemplary embodiment, the marker band **900** extends about 180° (one half) of the perimeter of the catheter shaft. The band is potentially made, for example, of 100% Platinum, or 90% Platinum/10% Iridium, Tantalum, Gold or any other radiopaque materials or combinations/amalgams thereof.

FIG. **9b** shows an imaging catheter **20** having two of the radiopaque marker bands **910** and **920** of the type depicted in FIG. **9a**. The proximal band **910** is skewed 90° (a quarter of the circumference of the catheter **20**) in relation to the distal band **920**. In this embodiment, the bands **910/920** are shown equally spaced on opposite sides of the diagnostic probe **22**. This catheter **20** also has a guidewire lumen **930** for passing a guidewire, for example a 0.014" guidewire. The guidewire exits out the distal guidewire port. The proximal end of the guidewire can exit a proximal port either within the blood vessel (short lumen rapid exchange cath-

eter), within a guiding catheter (long lumen rapid exchange catheter) or outside of the patient (over-the-wire catheter).

FIG. 9c shows the imaging catheter **20** from a view that looks directly on the full surface of the distal marker band **920**. Exactly one half of the proximal marker band **910**, skewed by 90 degrees, is seen. An angiography image of the two marker bands, when viewed as shown in FIG. 9c reveals band **920** having a thickness that is twice the thickness of the image of the band **910**. Furthermore, an image length “L” of the marker bands **910/920** depends on angular position of the portion of the catheter **20** in the image containing the bands **910/920**. In a perfect side view, the length L is equal to the actual length of the marker band. Offset O is equal to the difference between the thickness of band **920** and the thickness of band **910**.

In FIG. 9d an image is taken at a view wherein the catheter **20** is axially rotated 90 degrees from the position depicted in FIG. 9c. The thickness of band **920** is half the thickness of band **910**. Also, the position of the relative positions of the bands **910/920** in relation to the axis of the catheter **20** is used to determine the actual angular orientation of the catheter **20** since the offset alone is not enough to establish a current rotational position of the catheter **20**.

FIG. 9e is an image of the catheter **20** and bands **910/910** at a different rotational position from FIG. 9c and FIG. 9d. The orientation of the catheter can be determined by comparing the relative thicknesses (e.g., the offset, a ratio) of the thickness of images of the bands **910** and **920**.

Other controls associated with the co-registration processor **30** facilitate performing a variety of additional tasks. For example, during a catheter pullback, a commenting functionality incorporated into the processor **30** enables a user to select a “bookmark” button. In response, the co-registration processor **30** attaches a note/comment to a specific cross-section and/or location along a calculated path on an enhanced radiological image.

As mentioned above, an alternative version of co-registration image scheme incorporates biplane angiography instead of standard, single view angiography images. In biplane angiography, two radiological projections are simultaneously presented to a user—e.g., two views skewed by 90 degrees on a common axis of rotation. In such systems, two enhanced radiological images are presented along-side a cross-sectional image. During an inactive fluoroscopy period, when marker artifact (cursor) position is determined by calculations in relation to a known pullback rate, two cursor positions are determined—one on each of the two enhanced radiological images. It is expected that at certain periods during which fluoroscopy is inactive, the foreshortening of the vessel seen on one biplane image is less than the other. Depending on the 3-dimensional vessel tortuosity, it is expected that the opposite biplane image would have less foreshortening at other periods where a marker artifact is based upon calculations rather than actual fluoroscope images. The errors are calculated independently in the two different biplane images, and corresponding scaling factors are generated for the correction. As previously mentioned, a derived 3-dimensional road-map is created based on information of the two images from different planes. In this case, the two different planes are the 90° biplane images. Locating a marker artifact on a derived 3-D image is calculated from locations of marker artifacts one each of two orthogonal biplane images.

All of the descriptions hereinabove associated with illustrative embodiments using an IVUS catheter are applicable to a variety of alternative types of imaging catheters. Similarly, an enhanced radiological image can be combined with

a longitudinal stack instead of a cross sectional slice—in fact, the enhanced radiological, transverse cross-sectional, and longitudinal cross-sectional images can be displayed together. In yet other embodiments, the enhanced radiological image is presented along-side an IVUS image including both grayscale and color image artifacts that characterizing tissue and deposits within a vessel. Additionally, the longitudinal IVUS grayscale image and/or the color (Virtual Histology) image are overlaid on the 2-D angiographic image or derived 3-D image.

The above-described examples of co-registration have primarily addressed IVUS examples. However, as mentioned above, co-registration is alternatively incorporated into functional flow measurement systems that provide hemodynamic image information such as blood flow velocity and pressure. Turning briefly to FIG. 10, an exemplary co-registration display **1001** rendered by the co-registration processor **30** includes an enhanced radiological image **1010** displayed along-side functional flow measurement values presented in a graph **1000**. In FIG. 10 functional flow reserve (FFR) is depicted in the graph **1000** as a function of displacement along a length of a blood vessel. The enhanced radiological image **1010** comprises a marker artifact **1020** superimposed upon an angiogram image. The marker artifact **1020** indicates the point at which the presently displayed functional flow measurements are being presented based upon measurements previously acquired by sensors/transducers on the probe **22** mounted at the distal end of a flexible elongate member such as a guidewire or the catheter **20**. In yet another illustrative embodiment, the co-registration image further includes an IVUS cross-sectional image (not depicted) corresponding to the vessel segment indicated by the marker artifact **1020** on the enhanced radiological image **1010**.

The display also includes a variety of additional text information associated with the section of the vessel identified by the marker artifact **1020**. Vessel dimensions **1030** specify an approximate diameter and lumen area of a particular cross section indicated by the marker artifact **1020**'s current position on the enhanced radiological image **1010**. Additionally, IVUS information **1040** specify a plaque burden percentage and a total plaque area for a current cross-sectional slice indicated by the marker artifact **1020**. An FFR information **1050** specifies a current FFR value associated with the current location of the marker artifact **1020**. It is noted that the marker artifact **1020** approximates the location of a probe (e.g., probe **22**) at the time data was acquired to render the presently displayed data values. In accordance with an exemplary embodiment of the present invention, the location of the marker artifact **1020** is derived from image data provided by a radiopaque element/marker located near a probe mounted upon a flexible elongate member such as probe **22** mounted on a guidewire or catheter **20**.

By way of example, the marker artifact **1020** operates as a slider control that enables a user to sequentially traverse a set of stored data records containing information of the type displayed in FIG. 10. Furthermore, in the particular example, an FFR value associated with a particular location designated by the marker artifact **1020** is displayed near the marker artifact **1020**. Also, a second slider **1060** is also provided that is linked to the position of marker artifact **1020** and thus moves in synchronism with the marker artifact **1020**. Moving either the slider **1060** or the marker artifact **1020** causes movement of the other.

Other types of interventional ultrasound imaging, such as Intracardiac Echocardiography are also envisioned that uti-

lize this co-registration system. For example a steerable catheter with a linear, curvilinear, circumferential or other ultrasonic array at the distal end is placed into or in proximity to the chambers of the heart, and its location is incorporated into an enhanced ultrasound image.

Having described exemplary systems embodying the present invention, attention is directed to FIG. 11 that summarizes a set of exemplary steps associated with the operation of the above-described systems. Initially, during step 1100 an angiogram image is generated and stored within the first portion 36 of image data memory 40. A single angiogram image can be used to support co-registered display of multiple acquired data sets from the probe 22 as the probe 22 passes within a length of a blood vessel. A visual artifact (e.g., marker artifact 420) having a position determined at least in part upon a radiopaque marker positioned near the probe 22 on the imaging catheter 20, is superimposed on the angiogram image. As the probe 22 passes within the blood vessel the visual artifact progresses along the angiogram image of the blood vessel thereby providing an approximate location of the probe 22 associated with currently displayed data rendered according to information provided by the probe 22.

Thereafter, during step 1105 an initial calculated path (e.g., path 550) is generated by the co-registration processor 30. This estimation of the path can be generated according to any of a variety of methods including: automated two-dimensional and three-dimensional path calculations; manual path specification; and user assisted automated path calculations (a combination of automated path calculation with user-specified over-rides). The calculated path is superimposed upon the angiogram image generated during step 1100 and represents the projected path of the probe 22 when pullback is commenced of the probe 22.

In an exemplary embodiment, the operation of the co-registration system is determined by whether the fluoroscope has been activated (providing a live image of a radiopaque marker mounted proximate the probe 22). If the fluoroscope is active, then control passes to step 1115 wherein a fluoroscope image (see, e.g., FIG. 3) of the radiopaque marker is acquired, timestamped and stored. Thereafter, at step 1120 image data associated with the probe 22 is acquired, timestamped and stored. In the illustrative example, the image data comprises an IVUS image generated by an ultrasound transducer probe mounted upon the imaging catheter 20.

At step 1125 the co-registration processor 30 superimposes/overlays a marker artifact on the previously stored angiogram image to render the aforementioned enhanced radiological image. The marker artifact derives its position, at least in part, from the previously acquired and stored radiopaque marker position data. The enhanced radiological (e.g., angiogram) image is thereafter stored with the timestamp associated with the radiopaque marker position data during step 1130.

Thereafter, at step 1135 the co-registration processor 30 renders and simultaneously presents on a display/monitor the previously generated enhanced angiogram image and a corresponding probe (IVUS) image. The enhanced angiogram image and the corresponding probe image are displayed along-side one another on the display/monitor. Selection of a corresponding image is based upon a timestamp associated with the selected IVUS probe image. The respective timestamps of the radiological and probe components of the co-registered display need not be identical. In an embodiment of the invention a closest match criterion is

applied to the selection process. Control then returns to step 1110 for another iteration of the co-registration imaging process.

Alternatively, if the fluoroscope is inactive during a period wherein a pullback mechanism is drawing the probe 22 through a segment of a vessel of interest, then control passes from step 1110 to step 1150. At 1150 the co-registration processor 30 acquires/registers a pullback rate for the pullback mechanism. At step 1155 image data associated with the probe 22 is acquired, timestamped and stored. In the illustrative example, the image data comprises an IVUS image generated by an ultrasound transducer probe mounted upon the imaging catheter 20. During step 1160 the processor 30 determines a time that has elapsed since the previous calculation of the artifact marker position. In cases where the elapsed time is a constant, this step need not be repeated once the elapsed time constant has been determined. During step 1165 the co-registration processor 30 generates an estimate of a present position of the probe 22 and a corresponding marker artifact position on the enhanced radiological image. By way of example, the pullback rate and the elapsed time between a previous marker artifact position determination and the present position determination are used to generate a present position estimate for the marker artifact.

Thereafter, during step 1170 the co-registration processor 30 superimposes/overlays a marker artifact on the angiogram at the new calculated position based upon the calculated path and the distance calculation rendered during step 1165. During step 1175 the enhanced radiological (e.g., angiogram) image is stored with the timestamp associated with the calculated marker artifact position data. Thereafter, at step 1180 the resulting enhanced radiological image is utilized to render and present a co-registered display including both the enhanced angiogram image and a corresponding (based upon timestamp) previously stored probe image. Control thereafter returns to step 1110.

The above-described steps are associated with providing a co-registered display as an intravascular probe mounted upon a flexible elongate member (e.g., a catheter, guidewire, etc.) progresses along a length of blood vessel. Co-registered displays are also rendered in a playback mode. Turning to FIG. 12, during step 1200 the co-registration processor 30 initially displays an enhanced radiological image including, for example, an angiogram image, a calculated path, and a cursor/slider mark positioned on the calculated path indicating a location associated with a presently provided image derived from data acquired by the probe 22 at the indicated location on the enhanced radiological image.

During step 1205 a user positions the cursor/slider mark on the calculated path. Such repositioning can occur in any of a number of ways. By way of example, the user drags and drops the cursor/slider using a mouse. Alternatively, a keyboard input can advance/backup the cursor/slider through a series of previously designated/bookmarked points along the calculated path displayed within the enhanced angiogram image provided during step 1200. Yet other keys can be used to advance the cursor/slider on a record-by-record basis through a set of stored records associated with the progression of the probe 22 along the calculated path. Still other modes of selecting a position of interest on the calculated path and its associated probe 22 (e.g., IVUS) image will be contemplated by those skilled in the art in view of the description provided herein.

During step 1210 in response to a particular position/timestamp associated with a current position of the cursor/slider on the enhanced radiological image, the co-registra-

tion processor 30 accesses a corresponding record within the set of records derived from the data provided by the probe 22. By way of example, such data sets include cross-sectional IVUS images or alternatively FFR values at specified positions along a blood vessel. Thereafter, during step 1215 a co-registered view is presented wherein the enhanced radiological image, including the calculated path and cursor/slider (derived at least partially from positional information provided by a radiopaque marker during data acquisition), is displayed along-side an image (e.g., an IVUS cross-section) derived from data provided by the probe 22 at a position indicated by the current cursor/slider position within the enhanced radiological image. The steps depicted in FIG. 12 are repeated in response to a detected change in the position of the cursor/slider to update the display to show the new position of the cursor/slider and the corresponding image (e.g. cross-sectional IVUS image) derived from data provided by the probe 22 at the designated cursor/slider position.

The structures, techniques, and benefits discussed above are merely exemplary embodiments of the invention. In view of the many possible embodiments to which the principles of this invention may be applied, it should be recognized that the embodiments described herein with respect to the drawing figures are meant to be illustrative only and should not be taken as limiting the scope of invention. For example, while separate processors are shown to carry out particular aspects of the invention, in alternative embodiments the functionality of the multiple processors can be incorporated into a single processor or even distributed among even more processors. Therefore, the invention as described herein contemplates all such embodiments as may come within the scope of the following claims and equivalents thereof.

What is claimed is:

[1. A system for acquisition and co-registered display of intravascular information, comprising:

an imaging flexible elongate member having a proximal end and a distal end;

an imaging probe located near the distal end of the flexible elongate member, and configured to obtain information for generating an image of a vessel;

a radiopaque marker located near the imaging probe;

a first memory for storing angiogram image data;

a second memory for storing intravascular image data derived from information obtained by the imaging probe;

a third memory for storing radiopaque marker image data, distinct from the angiogram image data, the radiopaque marker image data being derived from information obtained from a fluoroscopic imaging device;

a display processor configured to retrieve and combine data from the first memory, the second memory and the third memory, and further configured to render a composite image including:

an enhanced radiological image derived from the angiogram image data comprising a superimposition of at least a portion of the angiogram data and the radiopaque marker image data and providing a location of the radiopaque marker based upon an actual location during active fluoroscopy and an estimated location during inactive fluoroscopy,

an intravascular image element corresponding to the intravascular image data, wherein the enhanced radiological image and the intravascular image element are displayed proximate each other; and

a cursor, displayed upon the enhanced radiological image, indicative of a location of the imaging probe while acquiring data for the intravascular image element presently displayed on the composite image, said cursor having a position that is based at least in part on third data derived from the radiopaque marker image data stored in the third memory;

wherein the display processor is further configured to calculate an error function based on a difference between the estimated location of the radiopaque marker and the actual location of the radiopaque marker and wherein the display processor further configured to utilize the error function to correct the estimated location of the radiopaque marker for the preceding period of inactive fluoroscopy.]

[2. The system of claim 1 wherein the flexible elongate member is a catheter.]

[3. The system of claim 1 wherein the imaging probe comprises an ultrasound device.]

[4. The system of claim 3 wherein the ultrasound device is a side-firing intravascular ultrasound transducer assembly.]

[5. The system of claim 4 wherein the side-firing intravascular ultrasound transducer assembly comprises an array of transducer elements.]

[6. The system of claim 5 wherein the array of transducer elements are linearly arranged along a lengthwise axis of the flexible elongate member.]

[7. The system of claim 5 wherein the array of transducer elements are curvilinearly arranged about a lengthwise axis of the flexible elongate member.]

[8. The system of claim 5 wherein the array of transducer elements are circumferentially arranged about a lengthwise axis of the flexible elongate member.]

[9. The system of claim 3 wherein the ultrasound device comprises a Doppler transducer.]

[10. The system of claim 9 wherein the flexible elongate member comprises a guidewire.]

[11. The system of claim 1 wherein the flexible elongate member is a guidewire and the imaging probe comprises a pressure sensor.]

[12. The system of claim 1 wherein the radiopaque marker comprises a cylindrical marker band.]

[13. The system of claim 1 wherein the radiopaque marker comprises at least one partially complete cylindrical marker band.]

[14. The system of claim 13 wherein the radiopaque marker comprises two semi-cylindrical marker bands.]

[15. The system of claim 14 wherein the two semi-cylindrical marker bands are skewed in relation to one another along a lengthwise axis of the flexible elongate member.]

[16. The system of claim 15 wherein the display processor further comprises an orientation determination function for determining a relative orientation of the imaging probe within the vessel based upon at least a relative size and position of the two semi-cylindrical marker bands in relation to one another.]

[17. The system of claim 1 wherein the third data is derived from user-specified points.]

[18. The system of claim 1 wherein the third data is derived by automated processes that determine a position of the radiopaque marker within a field of view.]

[19. The system of claim 18 wherein the automated processes utilize image pattern recognition to determine the position.]

19

[20. The system of claim 1 wherein the third data is derived from a combination of manual user input and automated calculations.]

[21. The system of claim 20 wherein the automated calculations include determination of a predicted path of the imaging probe.]

[22. The system of claim 1 wherein the display processor further comprises a bookmark function enabling a user to designate particular images of interest in a stored set of images containing at least the intravascular image element.]

[23. The system of claim 1 wherein the enhanced radiological image includes a calculated path of the imaging probe.]

[24. The system of claim 1 wherein the display processor further comprises a slider function associated with the cursor that enables a user to reposition the cursor to a point of interest on the enhanced radiological image through a user interface control, and in response displays a particular instance of the intravascular image element associated with the point of interest.]

[25. The system of claim 1, wherein the estimated location is based at least in part on a calculated path of the imaging probe and wherein the calculated path is updated based on the error function that is calculated based on a difference between the estimated location of the radiopaque marker and the actual location of the radiopaque marker.]

[26. A method for acquiring and displaying intravascular information in a system including an imaging flexible elongate member having a proximal end and a distal end, an imaging probe located near the distal end of the flexible elongate member, and configured to obtain information for generating an image of a vessel, and a radiopaque marker located near the imaging probe, the method comprising the steps of:

- storing angiogram image data in a first memory;
- storing intravascular image data derived from information obtained by the imaging probe in a second memory;
- storing radiopaque marker image data, distinct from the angiogram image data, in a third memory, the radiopaque marker image data being derived from information obtained from a fluoroscopic imaging device;

combining, by a display processor, data retrieved from the first memory, the second memory and the third memory to render a composite image including:

- an enhanced radiological image derived from the angiogram image data comprising a superimposition of at least a portion of the angiogram data and the radiopaque marker data and providing a location of the radiopaque marker based upon an actual location during active fluoroscopy and an estimated location during inactive fluoroscopy, and

- an intravascular image element corresponding to the intravascular image data, wherein the enhanced radiological image and the intravascular image element are displayed proximate each other; and

displaying a cursor upon the enhanced radiological image, indicative of a location of the imaging probe while acquiring data for the intravascular image element presently displayed on the composite image, said cursor having a position that is based at least in part on third data derived from the radiopaque marker image data previously stored in the third memory;

wherein the estimated location is based on a calculated path of the imaging probe, and wherein an error function is calculated based on a difference between the estimated location of the radiopaque marker and the

20

actual location of the radiopaque marker when active fluoroscopy is resumed after inactive fluoroscopy and wherein the error function is utilized to correct the calculated path.]

[27. The method of claim 26 wherein the flexible elongate member is a catheter.]

[28. The method of claim 26 wherein the imaging probe comprises an ultrasound device.]

[29. The method of claim 28 wherein the ultrasound device comprises a Doppler transducer.]

[30. The method of claim 26 wherein the flexible elongate member is a guidewire and the imaging probe comprises a pressure sensor.]

[31. The method of claim 26 wherein the radiopaque marker comprises two semi-cylindrical marker bands that are skewed in relation to one another along a lengthwise axis of the flexible elongate member and wherein the method comprises determining an orientation of the imaging probe based upon at least a relative size and position of the two semi-cylindrical marker bands in relation to one another.]

[32. The method of claim 26 wherein the third data is derived from user-specified points.]

[33. The method of claim 26 wherein the third data is derived by automated processes that determine a position of the radiopaque marker within a field of view.]

[34. The method of claim 26 wherein the third data is derived from a combination of manual user input and automated calculations.]

[35. The method of claim 34 wherein the automated calculations determine a predicted path of the imaging probe.]

[36. The method of claim 26 further comprising storing a user-designated set of particular images of interest in a stored set of images containing at least the intravascular image element.]

[37. The method of claim 26 further comprising incorporating a calculated path of the imaging probe within the enhanced radiological image.]

[38. The method of claim 26 further comprising providing a slider function associated with the cursor that enables a user to reposition the cursor to a point of interest on the enhanced radiological image through a user interface control, and in response display a particular instance of the intravascular image element associated with the point of interest.]

[39. The method of claim 26, wherein the calculated path is calculated using a first multiplication coefficient if the imaging probe is being pulled through the vessel and a second multiplication coefficient if the imaging probe is being pushed through the vessel.]

[40. A system for acquisition and co-registered display of intravascular information, comprising:

- an imaging flexible elongate member having a proximal end and a distal end;

- an imaging probe located near the distal end of the flexible elongate member, and configured to obtain information for generating an image of a vessel;

- a radiopaque marker located near the imaging probe;

- a first memory portion for storing angiogram image data;
- a second memory portion for storing intravascular image data derived from information obtained by the imaging probe;

- a third memory portion for storing radiopaque marker image data, the radiopaque marker image data being derived from information obtained from a fluoroscopic imaging device;

a display processor configured to retrieve and combine data from the first memory portion, the second memory portion and the third memory portion, and further configured to render a composite image including:

an enhanced radiological image derived from the angiogram image data comprising a superimposition of at least a portion of the angiogram data and the radiopaque marker image data and providing a location of the radiopaque marker based upon an actual location during active fluoroscopy and an estimated location during inactive fluoroscopy, wherein an error function is calculated based on a difference between the estimated location of the radiopaque marker and the actual location of the radiopaque marker when active fluoroscopy is resumed after inactive fluoroscopy and wherein the error function is utilized to correct the estimated location of the radiopaque marker for the preceding period of inactive fluoroscopy,

an intravascular image element corresponding to the intravascular image data, wherein the enhanced radiological image and the intravascular image element are displayed proximate each other; and

a cursor, displayed upon the enhanced radiological image, indicative of a location of the imaging probe while acquiring data for the intravascular image element presently displayed on the composite image, said cursor having a position that is based at least in part on third data derived from the radiopaque marker image data stored in the third memory portion.]

[41. The method of claim 40, wherein the calculated path is calculated using a first multiplication coefficient if the imaging probe is being pulled through the vessel and a second multiplication coefficient if the imaging probe is being pushed through the vessel.]

[42. The system of claim 40, wherein the imaging flexible elongate member is a catheter.]

[43. The system of claim 40, wherein the imaging flexible elongate member is a guidewire.]

[44. The system of claim 40, wherein the imaging probe includes an ultrasound transducer.]

[45. The system of claim 40, wherein the imaging probe includes a pressure sensor.]

46. A system for providing an enhanced image of a vessel, the system comprising:

a processing system in communication with a diagnostic probe and a display, the processing system configured to:

receive angiogram image data of the vessel, wherein the angiogram image data is obtained with contrast flow;

receive fluoroscopic image data of the vessel and the diagnostic probe obtained while the diagnostic probe is positioned within and moved along a length of the vessel, the diagnostic probe including a radiopaque marker;

receive intravascular diagnostic data obtained by the diagnostic probe from within the vessel;

output an enhanced angiographic image of the vessel to the display, the enhanced angiographic image including:

an angiogram of the vessel based on the received angiogram image data; and

a marker indicative of a position of an element of the diagnostic probe along the length of the vessel based on a location of the radiopaque marker in the received fluoroscopic image data,

wherein the marker is superimposed on the angiogram of the vessel based on the location of the radiopaque marker in the received fluoroscopic image data; and

output a visual representation of the intravascular diagnostic data to the display, the visual representation of the intravascular diagnostic data including the intravascular diagnostic data associated with the position of the element of the diagnostic probe along the length of the vessel.

47. The system of claim 46, wherein the fluoroscopic image data is obtained without contrast flow.

48. The system of claim 46, wherein the diagnostic probe is an intravascular imaging probe.

49. The system of claim 48, wherein the intravascular imaging probe is at least one of an intravascular ultrasound (IVUS) probe and an optical coherence tomography (OCT) probe.

50. The system of claim 48, wherein the visual representation of the intravascular diagnostic data is a cross-sectional image of the vessel.

51. The system of claim 46, wherein the diagnostic probe is a hemodynamic intravascular probe.

52. The system of claim 47, wherein the hemodynamic intravascular probe includes at least one of a pressure sensor and a flow sensor.

53. The system of claim 52, wherein the visual representation of the intravascular diagnostic data is a graph of a hemodynamic variable along the length of the vessel.

54. The system of claim 53, wherein the hemodynamic variable is a fractional flow reserve (FFR) value.

55. The system of claim 46, wherein the marker of the enhanced angiographic image is generated by superimposing the fluoroscopic image data onto the angiogram image data.

56. The system of claim 55, wherein superimposing the fluoroscopic image data onto the angiogram image data accounts for an angular orientation of the radiopaque marker.

57. The system of claim 56, wherein the angular orientation of the radiopaque marker is determined by identifying corners of a four-sided polygon of an image of the radiopaque marker in the fluoroscopic image data.

58. The system of claim 56, wherein the diagnostic probe includes at least two radiopaque markers.

59. The system of claim 58, wherein the radiopaque markers have different profiles such that an angular orientation of the diagnostic probe can be determined from an image of the radiopaque markers in the fluoroscopic image data.

60. The system of claim 56, wherein superimposing the fluoroscopic image data onto the angiogram image data further utilizes at least one of: one or more dimensions of the diagnostic probe, image field information for the angiogram image data, and image field information for the fluoroscopic image data.

61. The system of claim 46, wherein the marker operates as a slider control such that as the marker is moved the output visual representation of the intravascular diagnostic data is updated based on the location of the marker and the associated position of the element of the diagnostic probe along the length of the vessel.

62. *The system of claim 46, further comprising the diagnostic probe.*

63. *The system of claim 62, wherein the diagnostic probe is at least one of a catheter or a guidewire.*

* * * * *