



US00RE47065E

(19) **United States**
(12) **Reissued Patent**
Stobie et al.

(10) **Patent Number:** **US RE47,065 E**
(45) **Date of Reissued Patent:** **Oct. 2, 2018**

(54) **HEART VALVE HOLDER AND METHOD FOR RESISTING SUTURE LOOPING**

(58) **Field of Classification Search**
CPC A61F 2/2427; A61F 2/2412
See application file for complete search history.

(71) Applicant: **Edwards Lifesciences Corporation**, Irvine, CA (US)

(56) **References Cited**

(72) Inventors: **Robert Stobie**, Laguna Woods, CA (US); **Ralph Kafesjian**, Newport Beach, CA (US); **Diana Nguyen-Thien-Nhon**, Irvine, CA (US); **Robert Ian Lister**, Sunnyvale, CA (US); **Andrzej Skoskiewicz**, Menlo Park, CA (US); **Adrian Benton James**, Oakland, CA (US); **Aaron Ernesto Sklar**, Castro Valley, CA (US); **Banny Banerjee**, Belmont, CA (US)

U.S. PATENT DOCUMENTS

3,409,013 A 11/1968 Barry
3,628,535 A 12/1971 Ostrowsky et al.
(Continued)

FOREIGN PATENT DOCUMENTS

WO 199725004 A1 7/1997

Primary Examiner — Catherine S Williams
(74) *Attorney, Agent, or Firm* — Pui Tong Ho

(73) Assignee: **Edwards Lifesciences Corporation**, Irvine, CA (US)

(57) **ABSTRACT**

(21) Appl. No.: **15/234,976**

An improved holder and method for implanting a tissue-type prosthetic mitral heart valve that prevents suture looping and may also constrict the commissure posts of the valve. An upstanding or shaft member axially positioned on the holder causes the lengths of attachment sutures to extend axially beyond the commissure post tips to create a tent and prevent looping of any of an array of pre-implanted sutures around the tips during deployment of the valve. The shaft member may be axially movable such that it can be initially retracted and then actuated just prior to valve deployment. The shaft member may have notches on its distal tip for capturing the attachment sutures, which are crossed over along the valve axis to ensure engagement by the notches. The attachment sutures may be strands or filaments, or may be wider bands of flexible biocompatible material. If bands are used, they desirably cover the commissure post tips to further help prevent suture looping thereover. The flexible lengths of material extend directly between commissures of the valve, or may extending radially inward from each commissure to a central upstanding member.

(22) Filed: **Aug. 11, 2016**

Related U.S. Patent Documents

Reissue of:

(64) Patent No.: **7,658,763**
Issued: **Feb. 9, 2010**
Appl. No.: **11/181,491**
Filed: **Jul. 13, 2005**


U.S. Applications:

(63) Continuation of application No. 10/705,587, filed on Nov. 10, 2003, now Pat. No. 6,966,925, which is a (Continued)

(51) **Int. Cl.**
A61F 2/24 (2006.01)

(52) **U.S. Cl.**
CPC **A61F 2/2427** (2013.01); **A61F 2/2412** (2013.01)

22 Claims, 14 Drawing Sheets

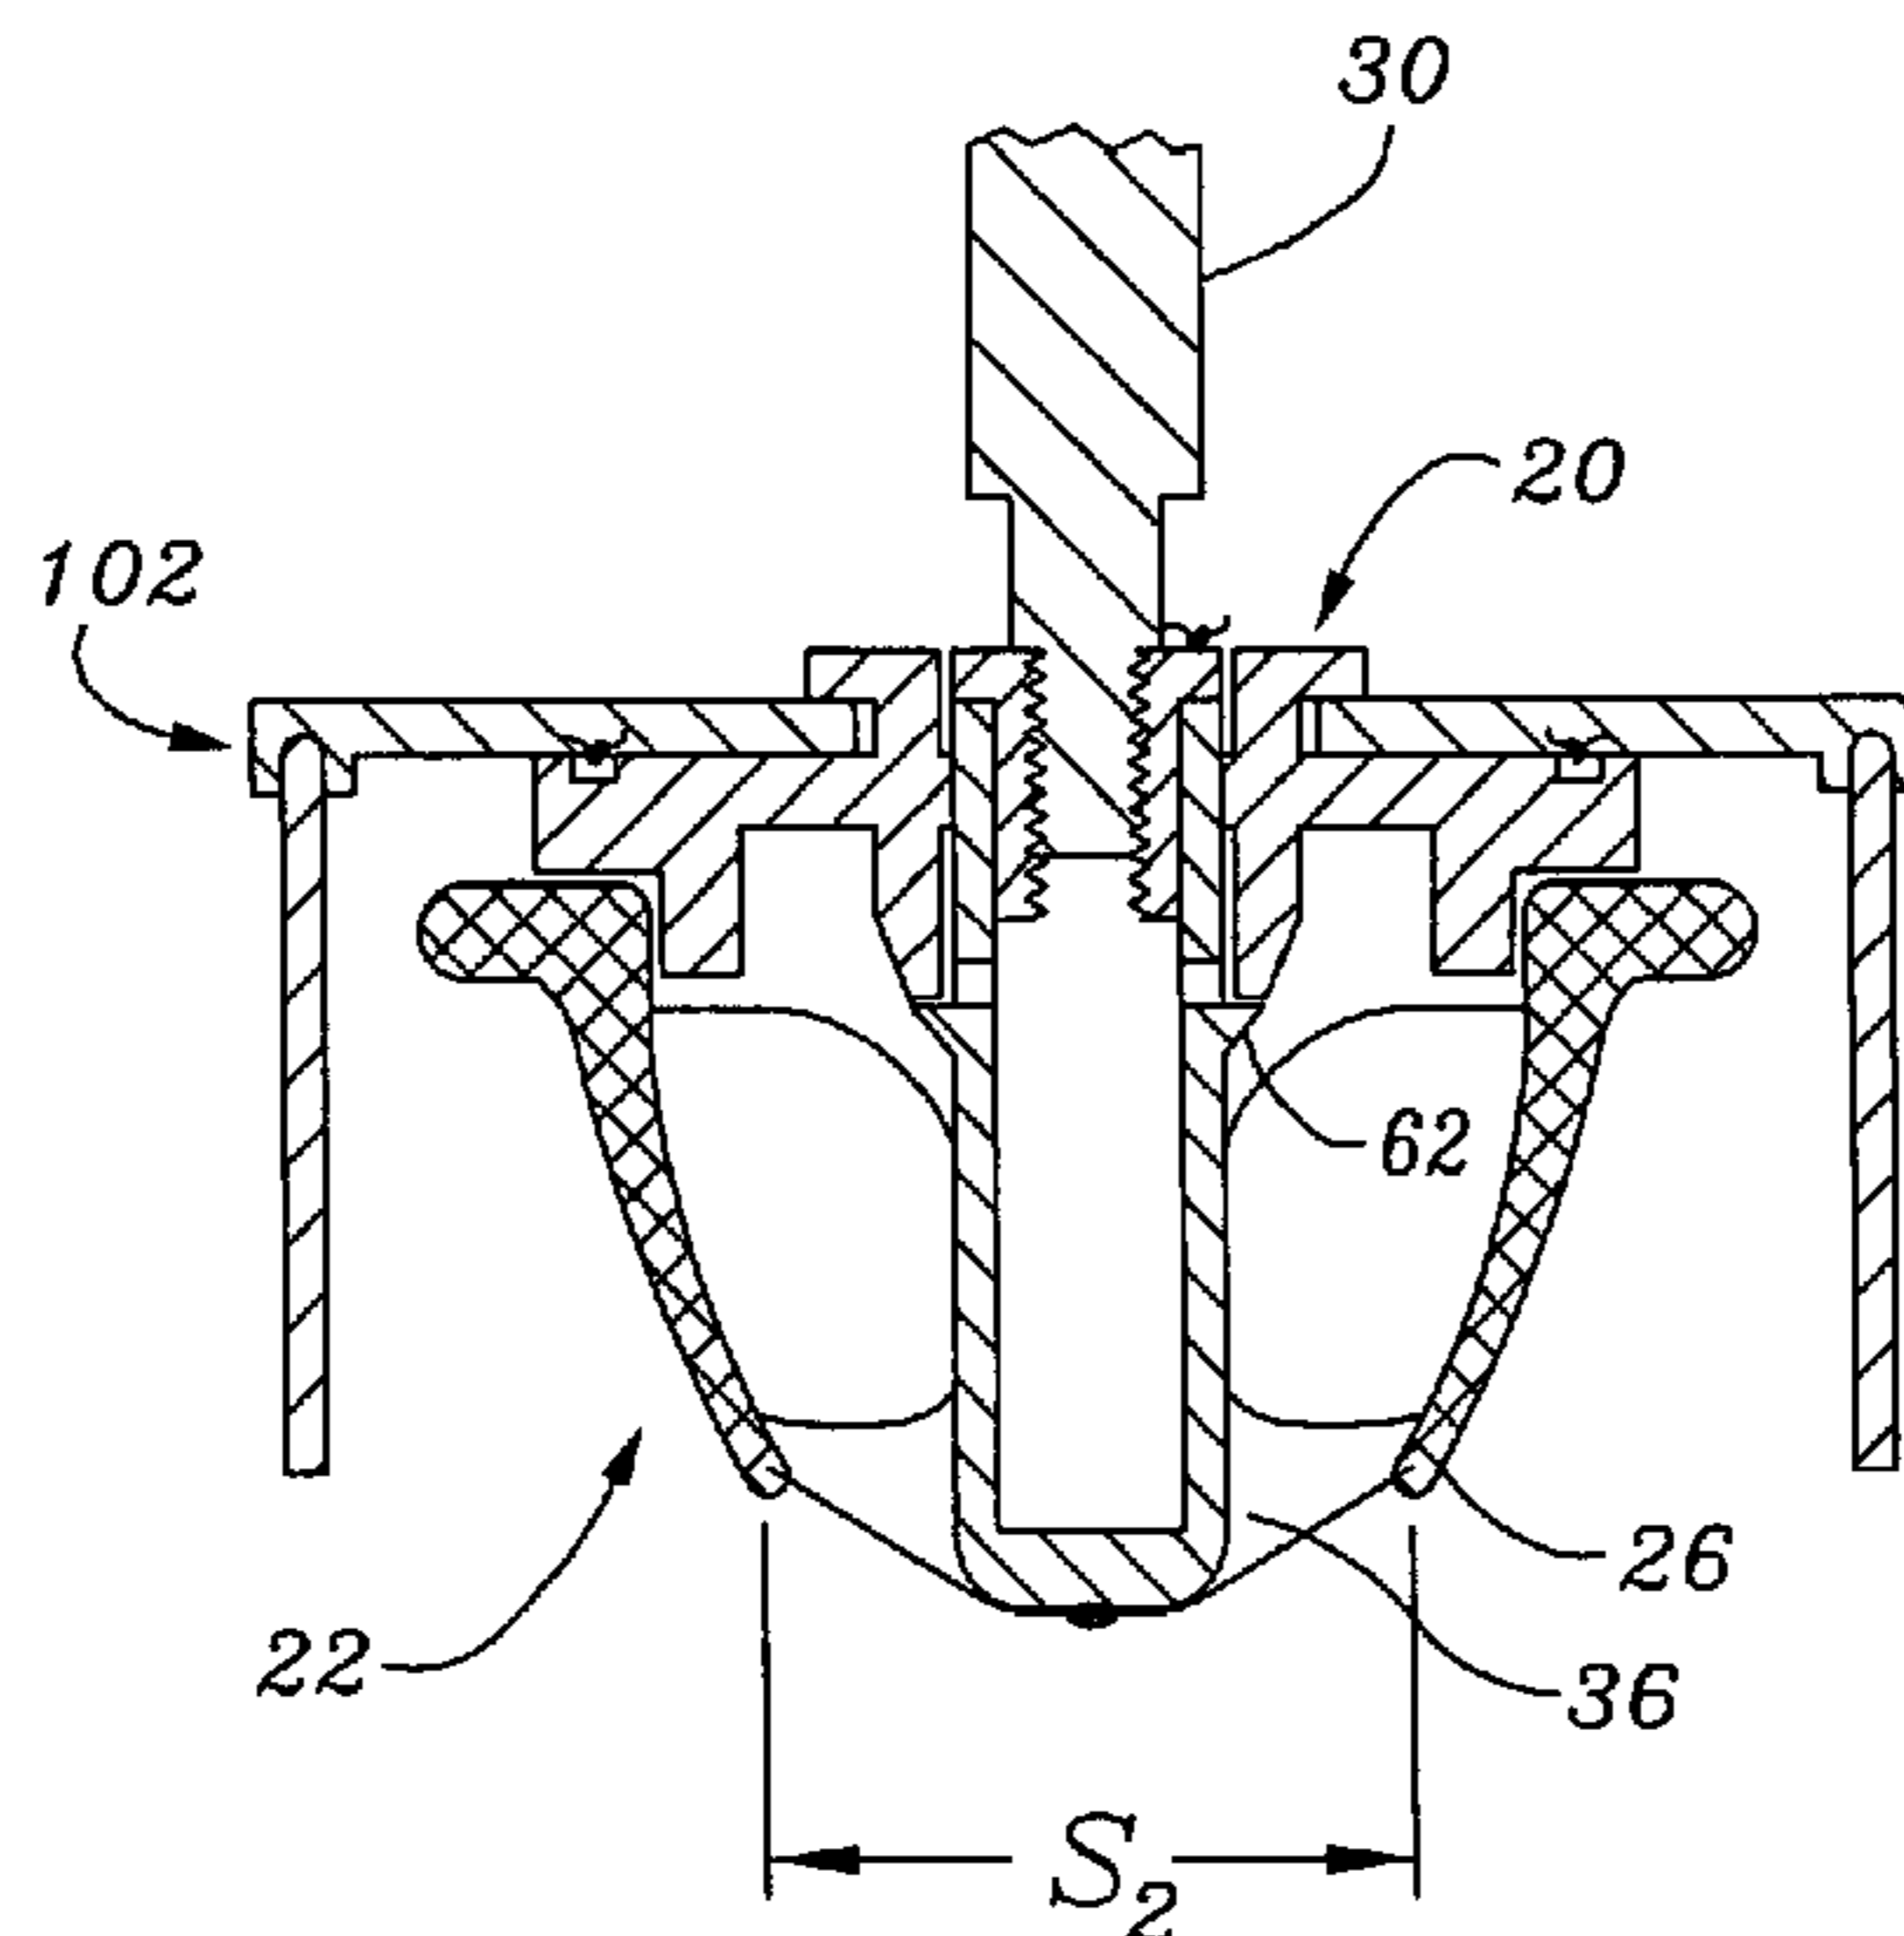

Related U.S. Application Data

continuation-in-part of application No. 09/745,386,
filed on Dec. 21, 2000, now Pat. No. 6,964,682.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,702,250	A	10/1987	Ovil et al.	
4,865,600	A *	9/1989	Carpentier et al.	623/2.11
5,443,502	A *	8/1995	Caudillo et al.	623/2.11
5,476,510	A *	12/1995	Eberhardt et al.	623/2.11
5,531,785	A *	7/1996	Love et al.	623/2.11
5,728,153	A *	3/1998	Menkis et al.	606/139
5,776,187	A *	7/1998	Krueger et al.	623/2.11
5,824,068	A	10/1998	Bugge	
5,861,028	A *	1/1999	Angell	623/2.11
6,126,007	A	10/2000	Kari et al.	
6,197,053	B1	3/2001	Cosgrove et al.	
6,214,043	B1	4/2001	Krueger et al.	
6,409,758	B2 *	6/2002	Stobie et al.	623/2.11
6,702,852	B2 *	3/2004	Stobie et al.	623/2.11
6,802,860	B2	10/2004	Cosgrove et al.	
6,964,682	B2 *	11/2005	Nguyen-Thien-Nhon et al.	623/2.11
				623/2.11
6,966,925	B2 *	11/2005	Stobie	623/2.11
7,189,258	B2 *	3/2007	Johnson et al.	623/2.11
7,468,073	B2 *	12/2008	Johnson et al.	623/2.11
7,503,929	B2 *	3/2009	Johnson et al.	623/2.11
2001/0010018	A1	7/2001	Cosgrove et al.	
2002/0082686	A1	6/2002	Nguyen-Thien-Nhon et al.	
2003/0023303	A1 *	1/2003	Palmaz et al.	623/2.18
2003/0125805	A1 *	7/2003	Johnson et al.	623/2.11
2004/0024451	A1 *	2/2004	Johnson et al.	623/2.11
2004/0138741	A1 *	7/2004	Stobie et al.	623/2.11

* cited by examiner

Fig. 1A

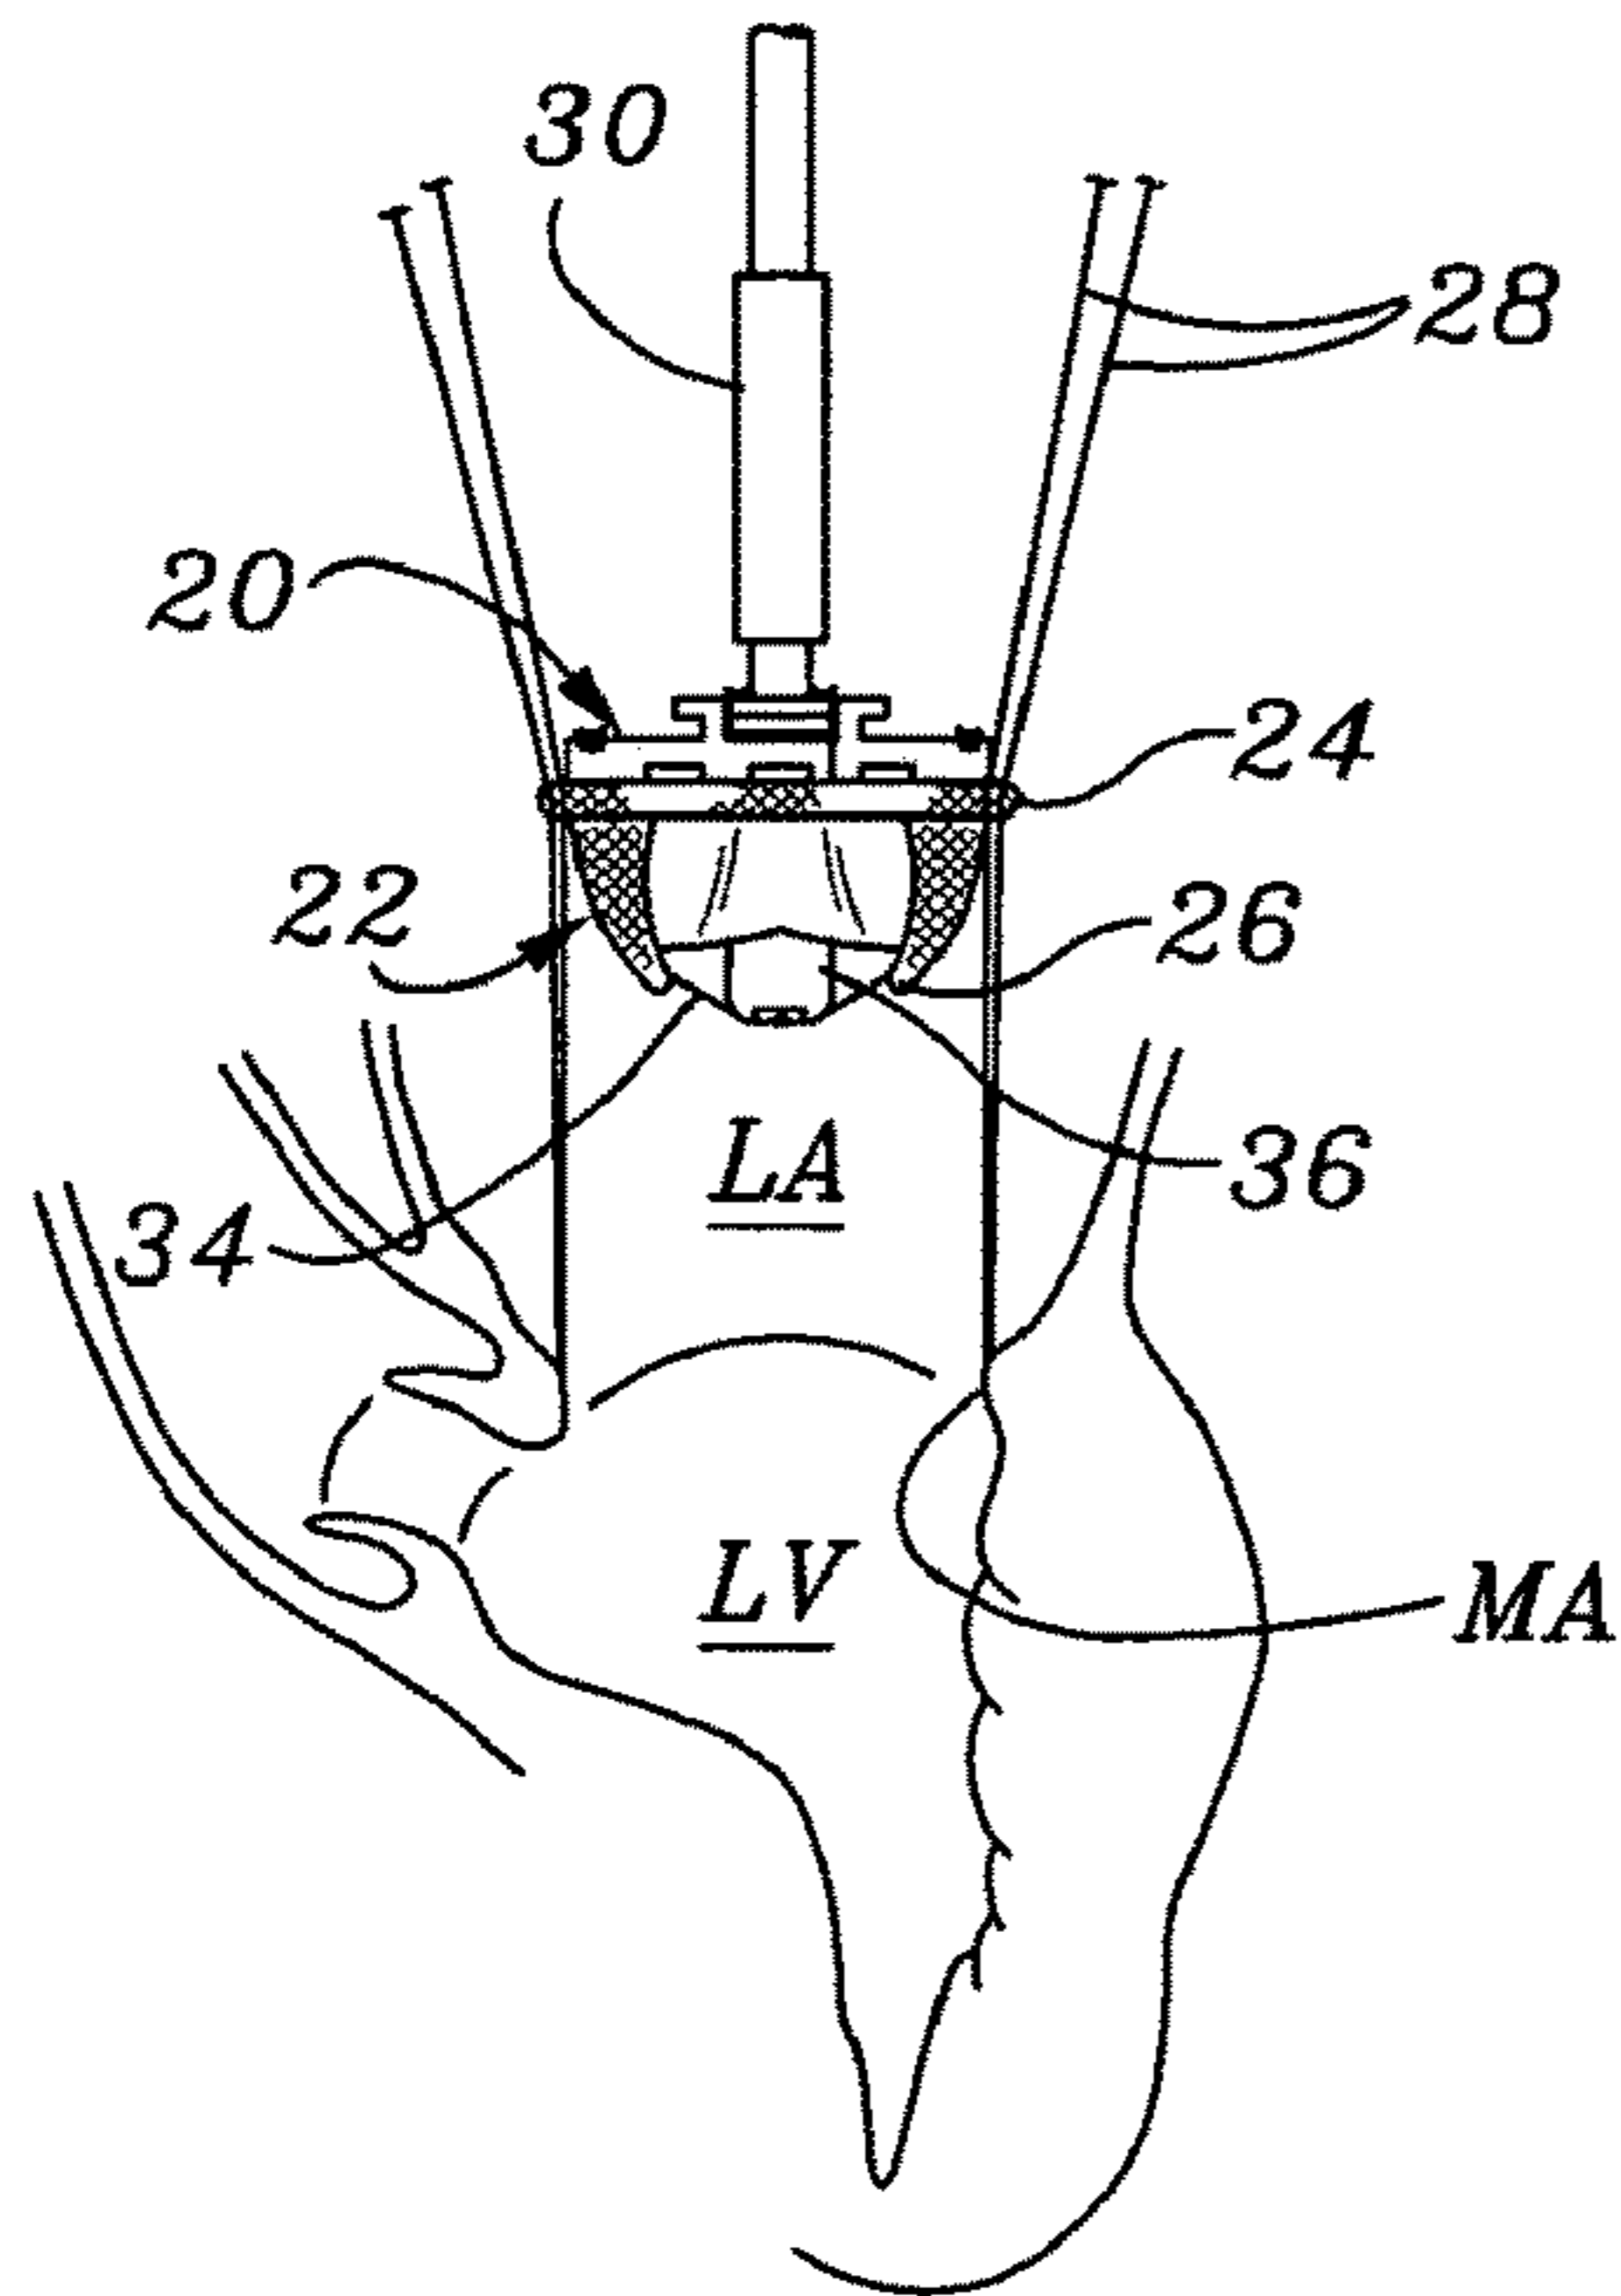


Fig. 1B

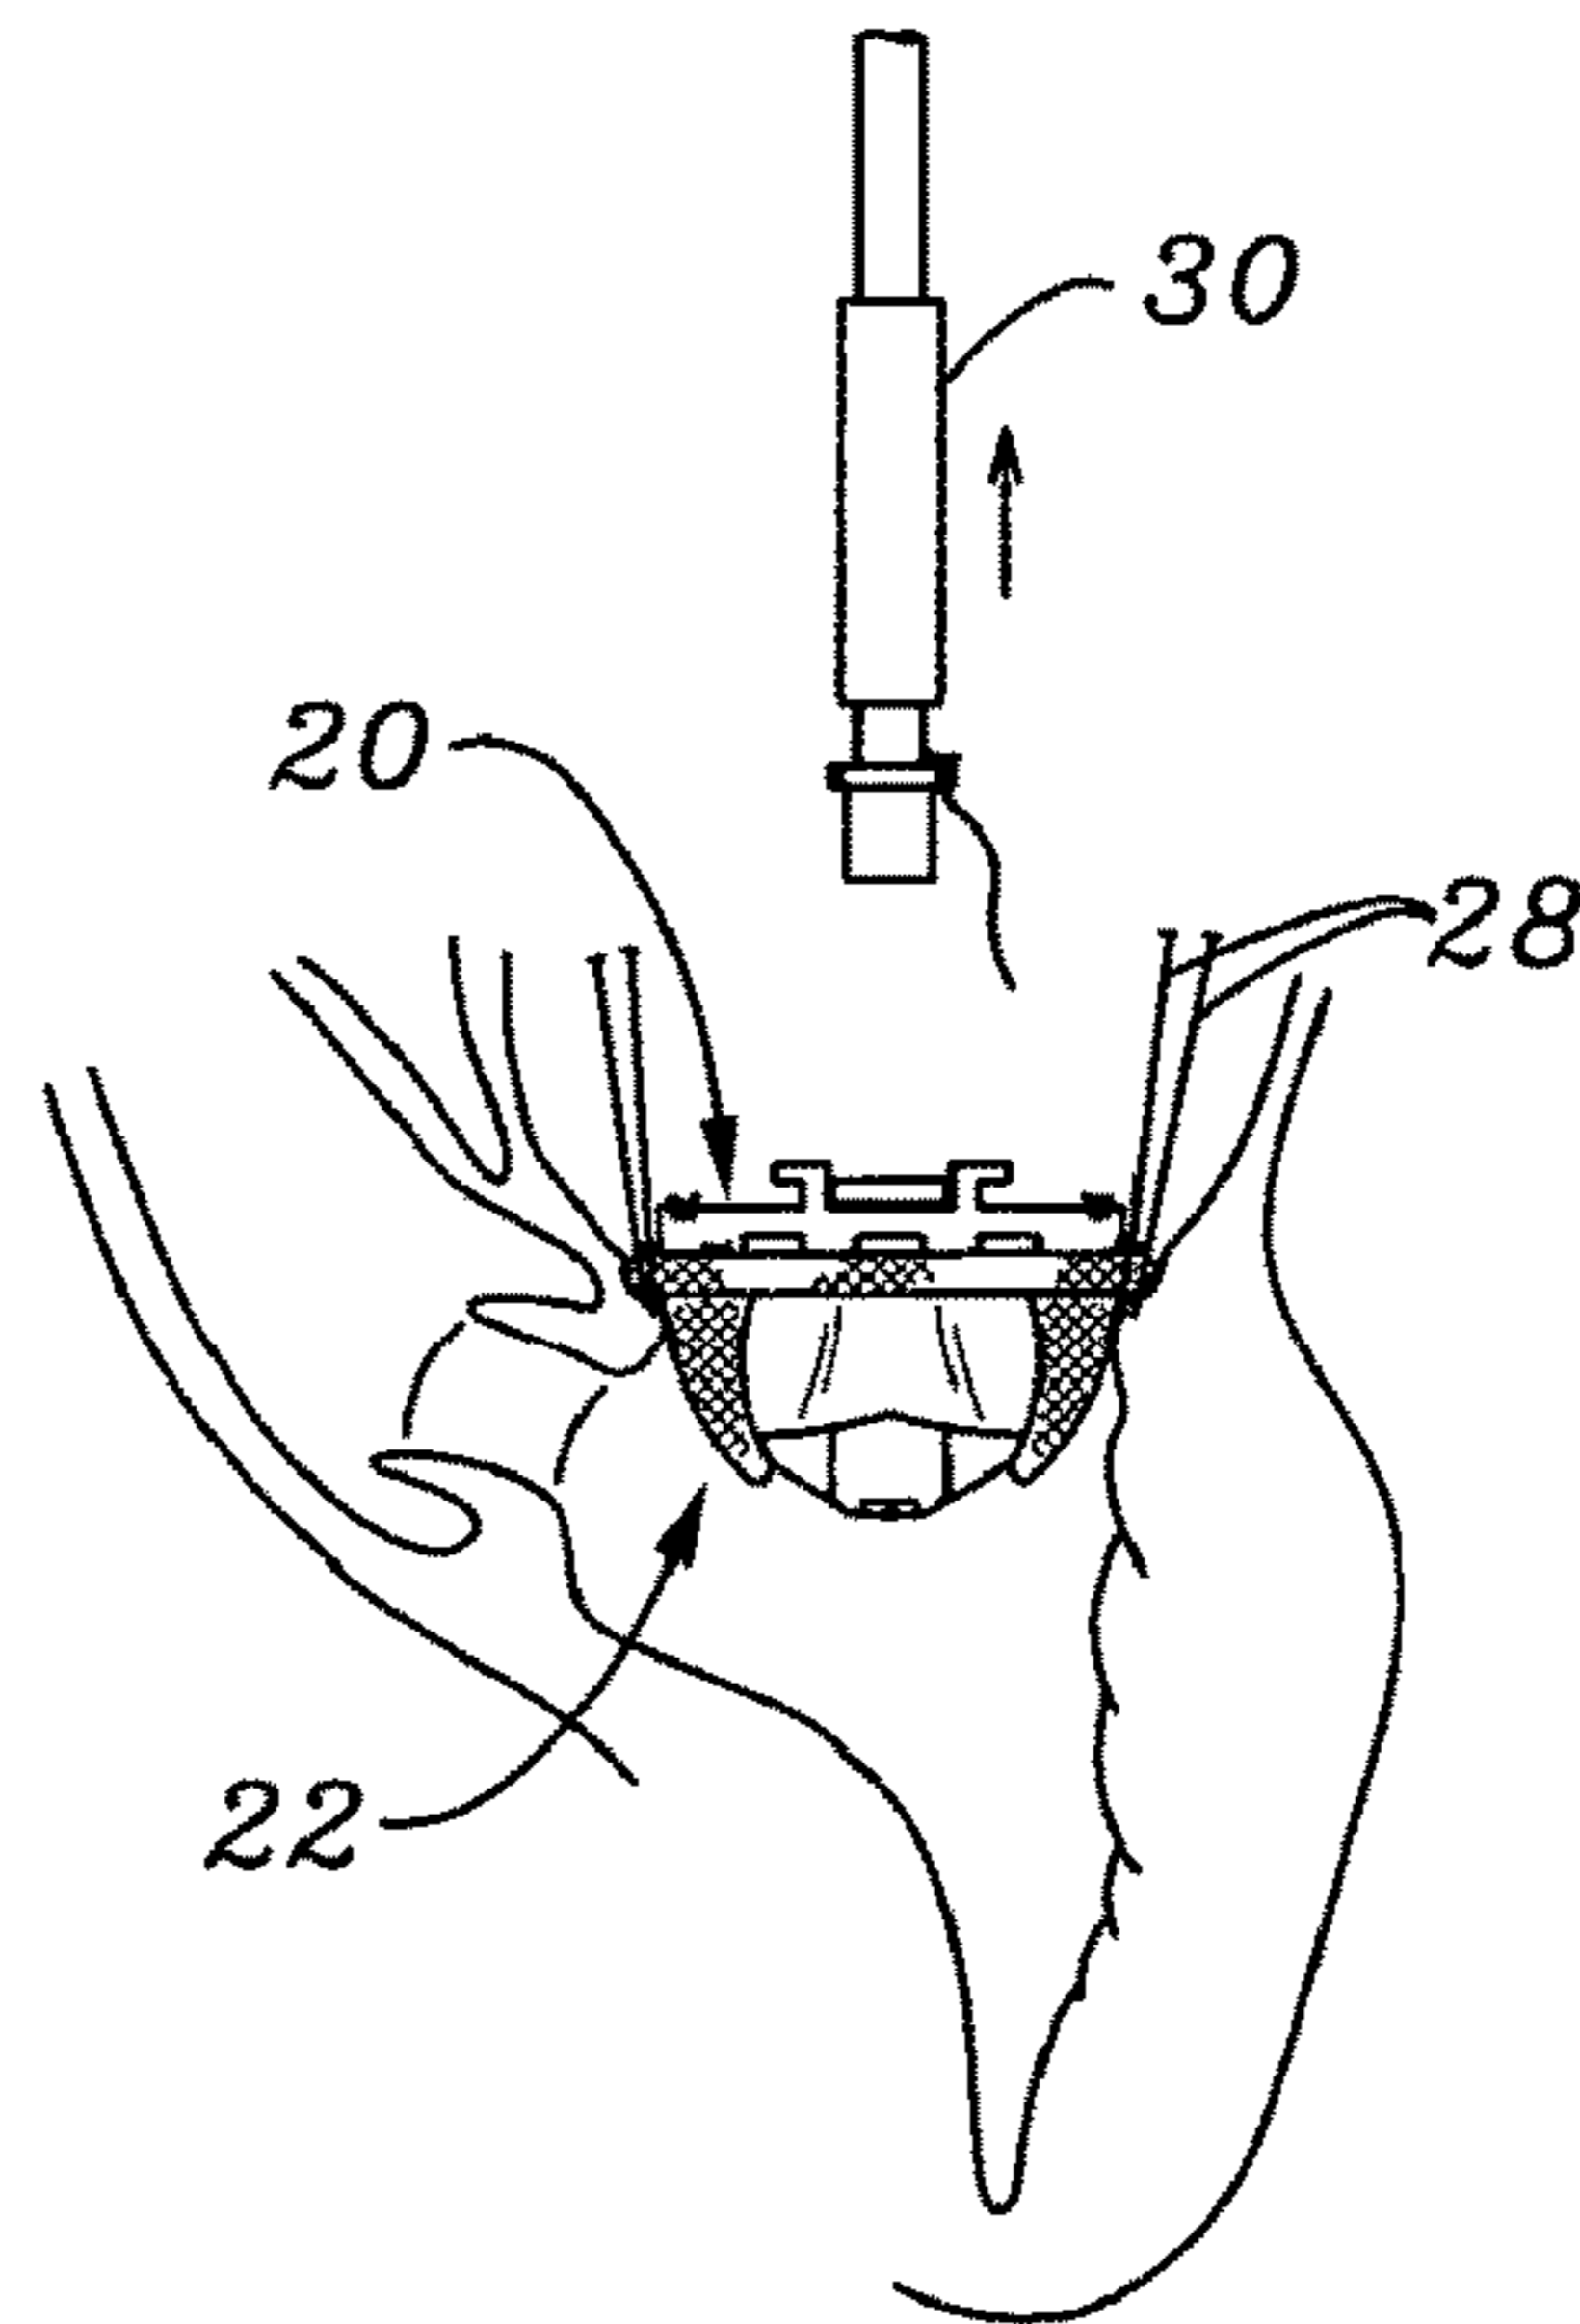
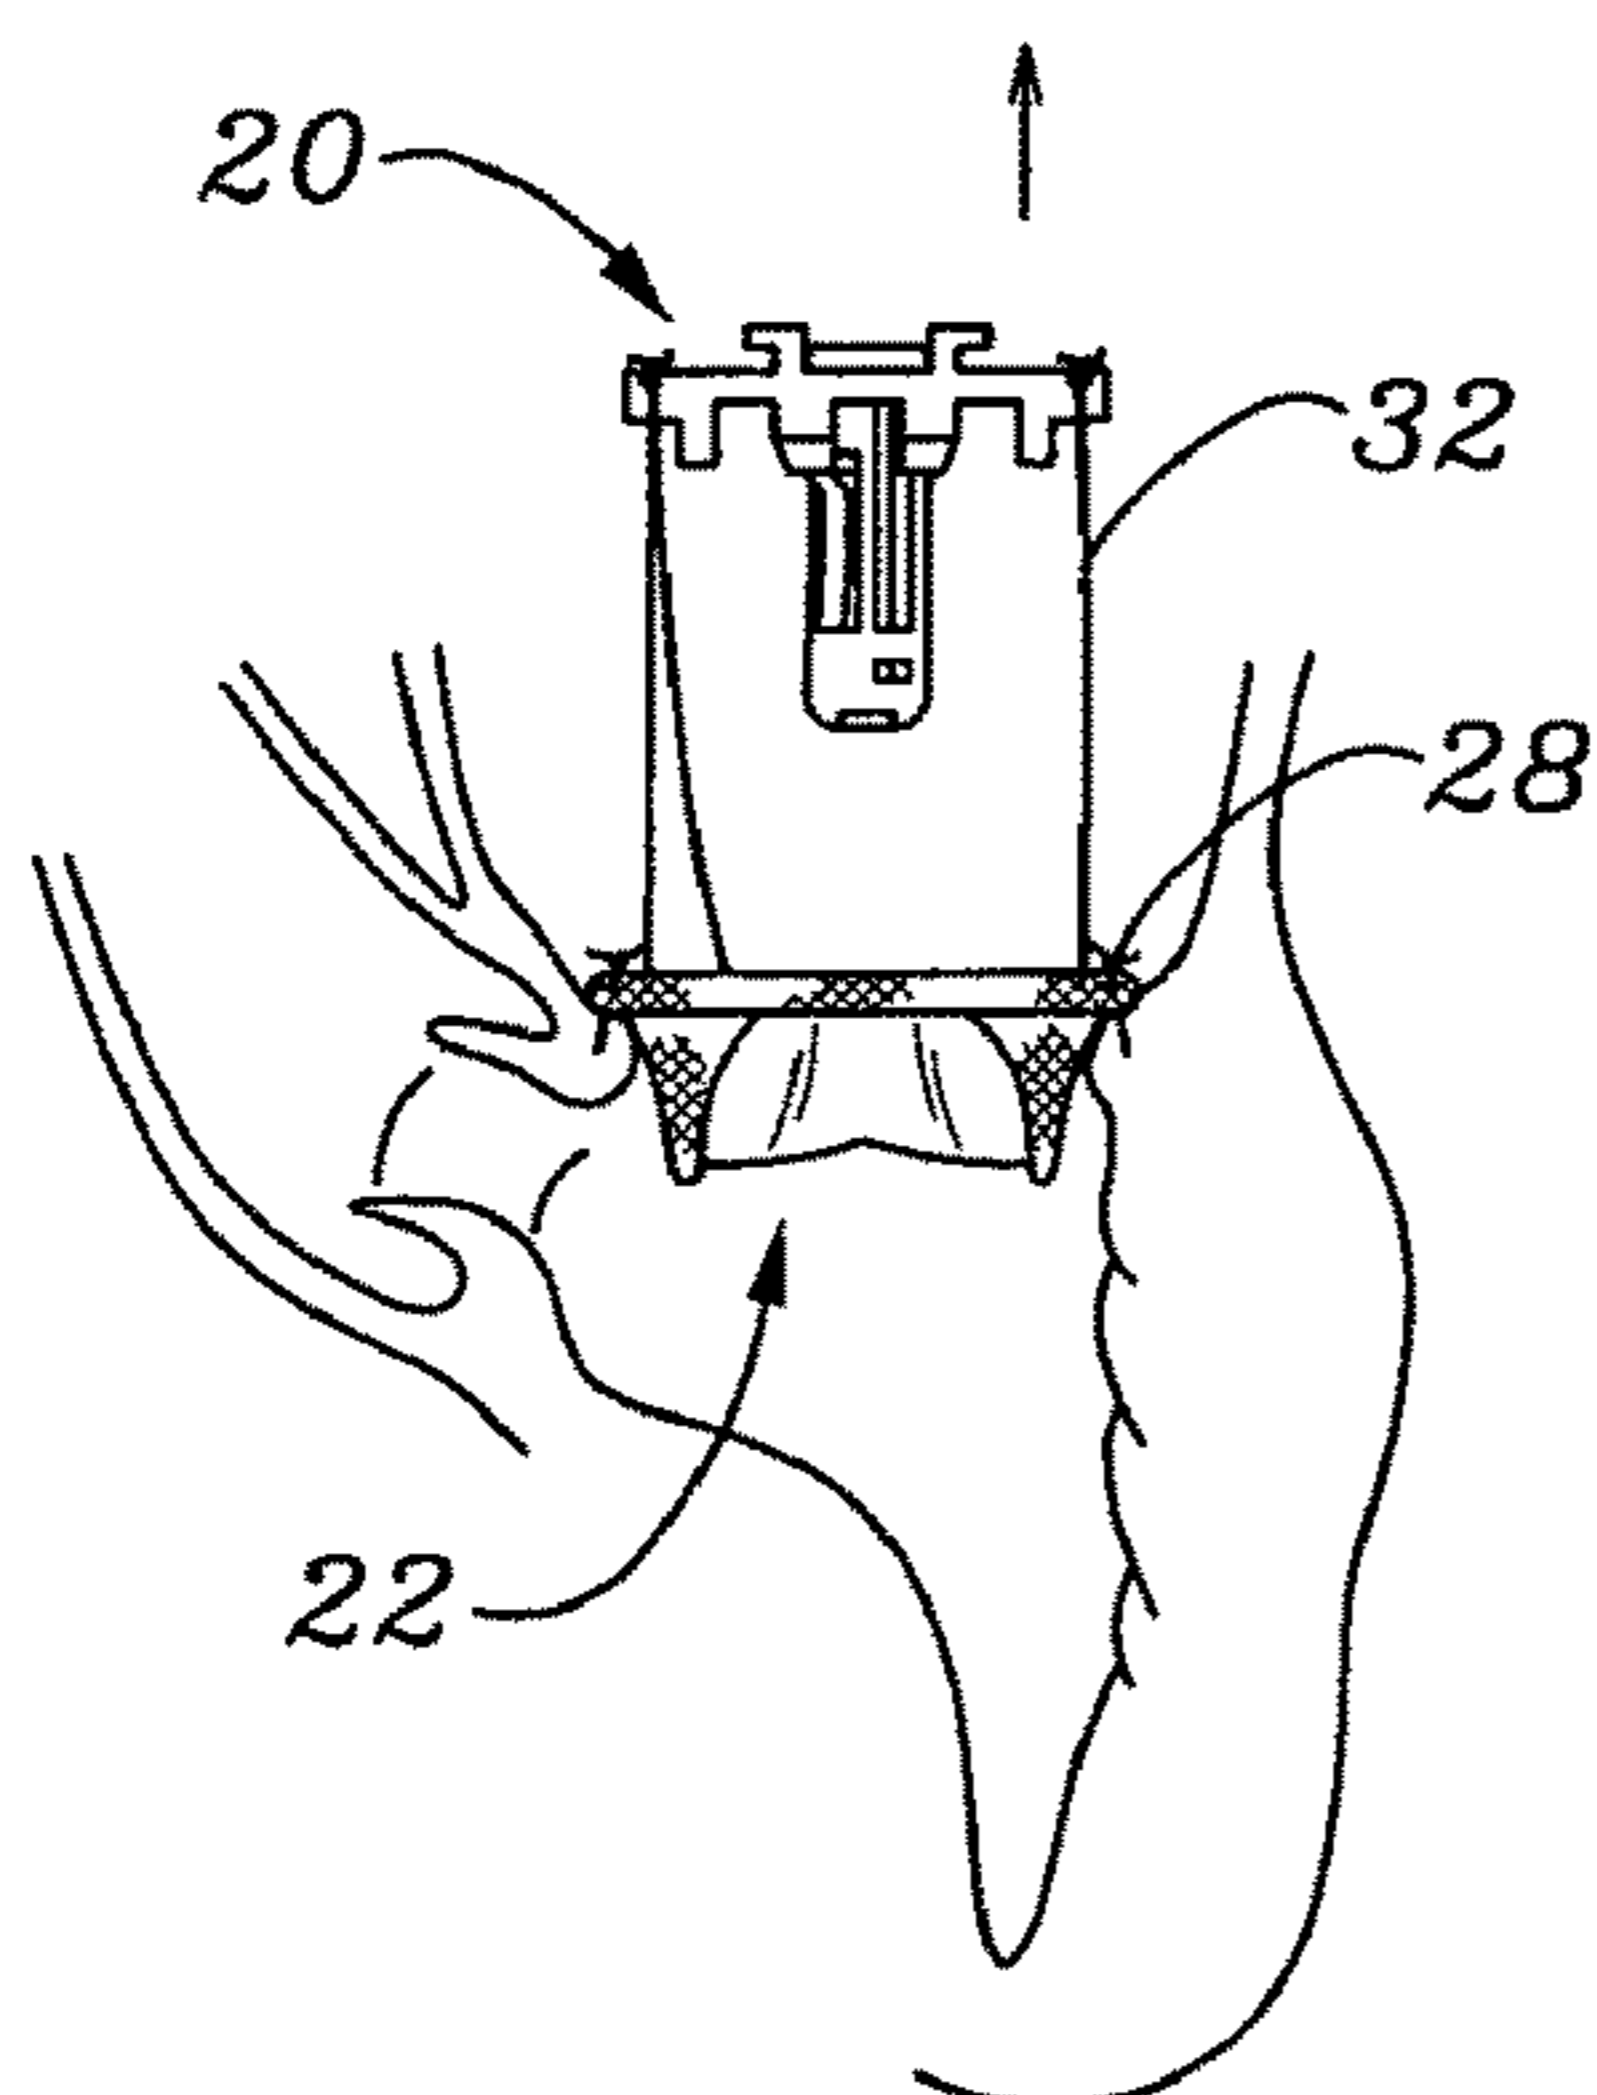


Fig. 1C



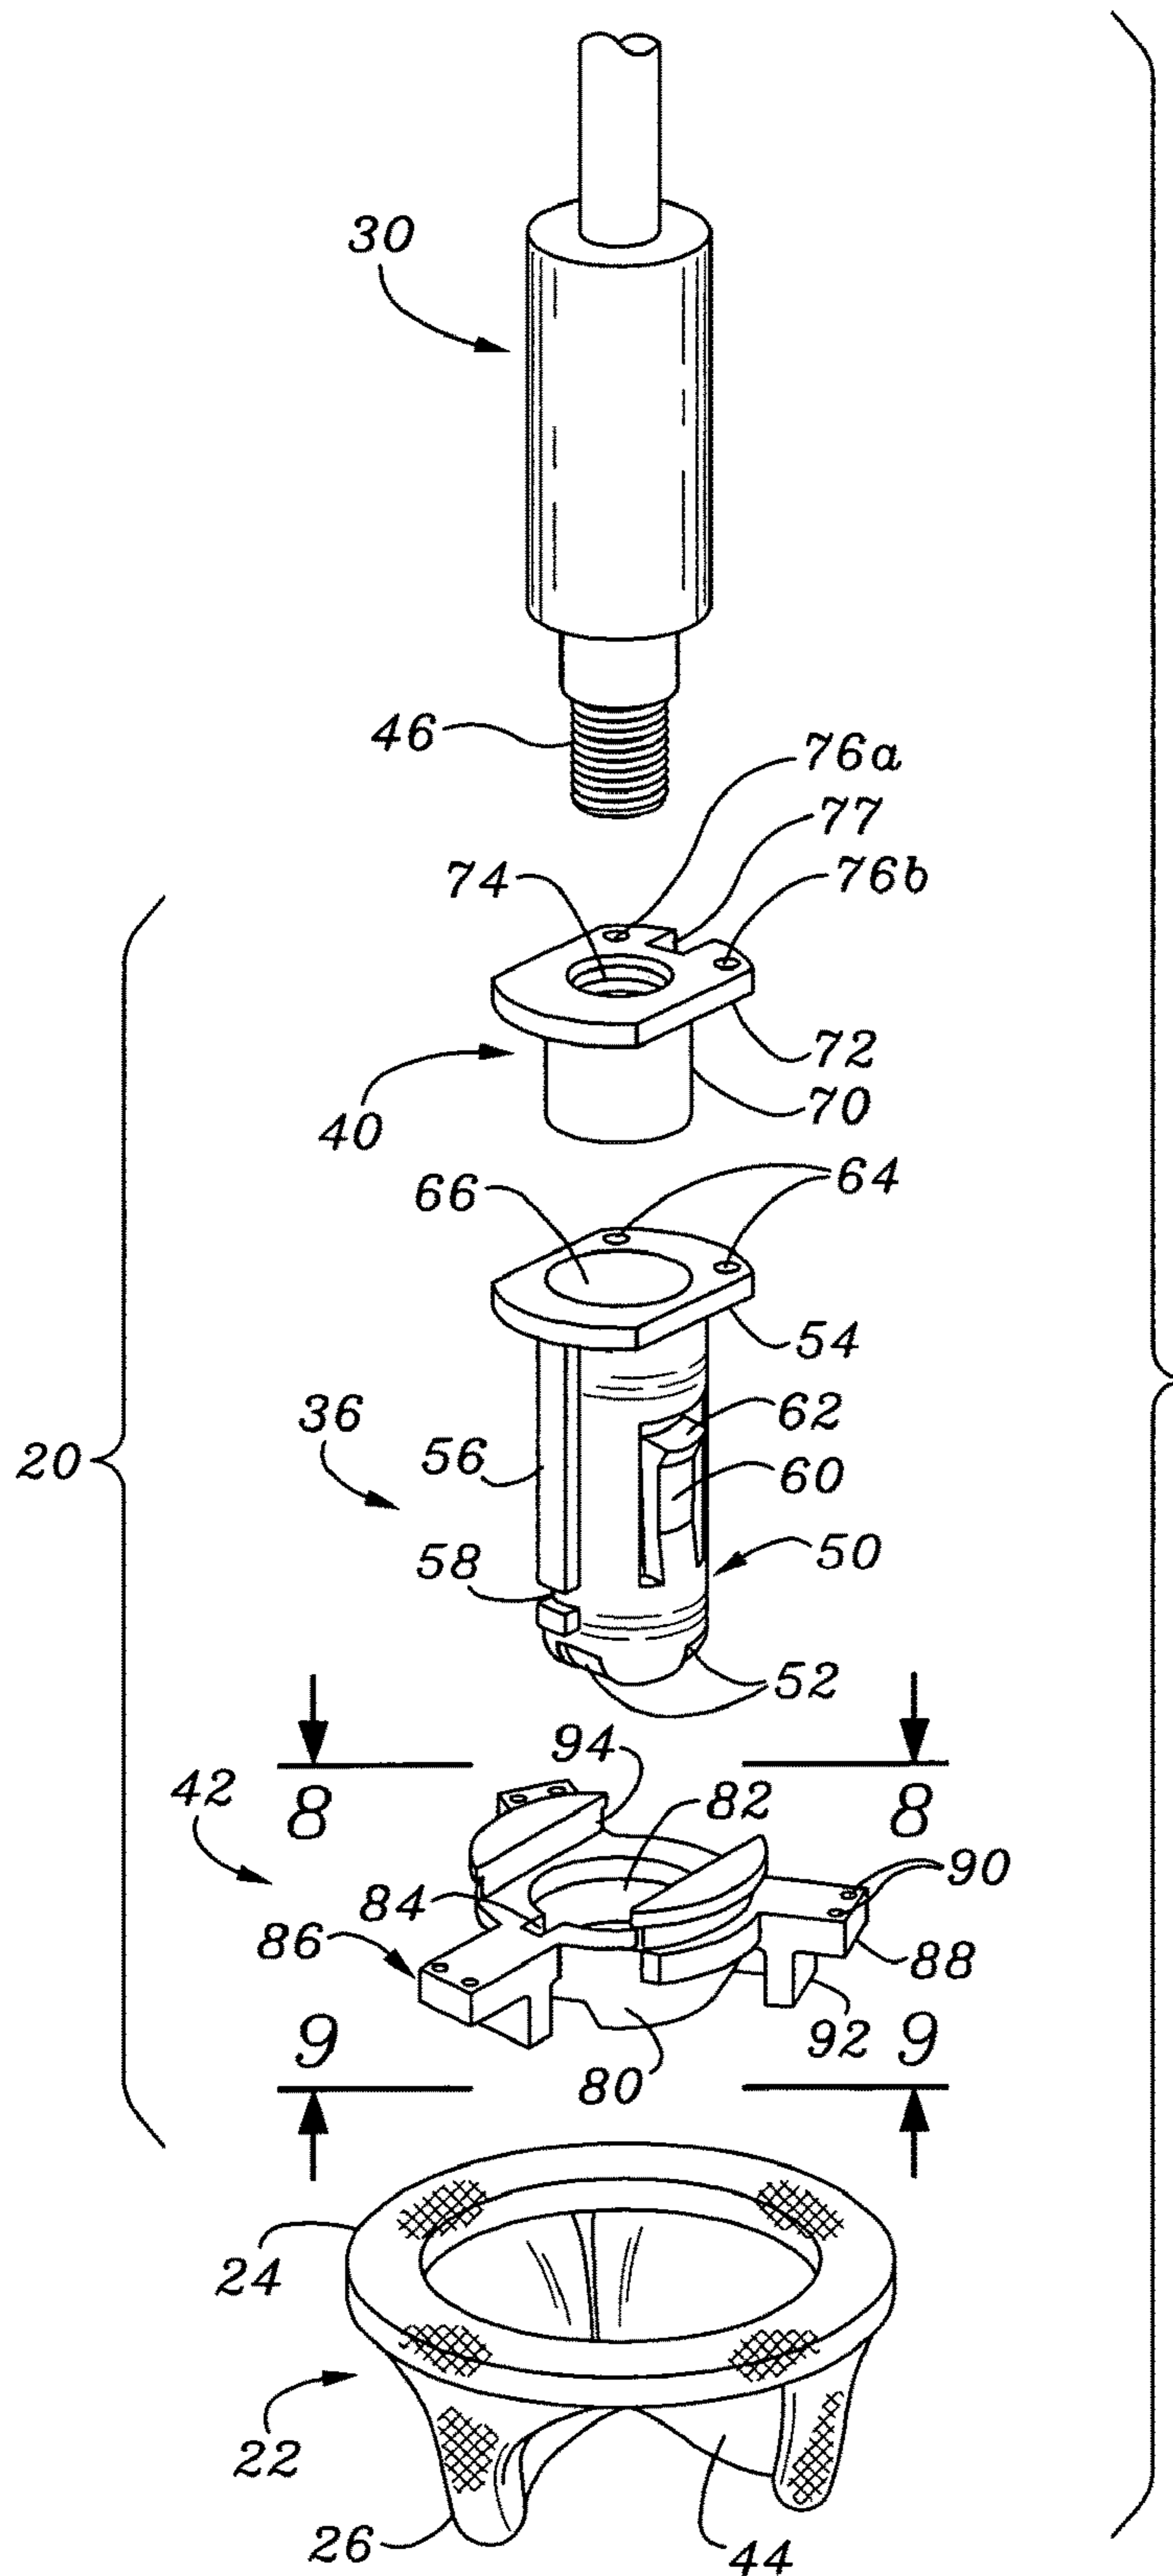


Fig. 2

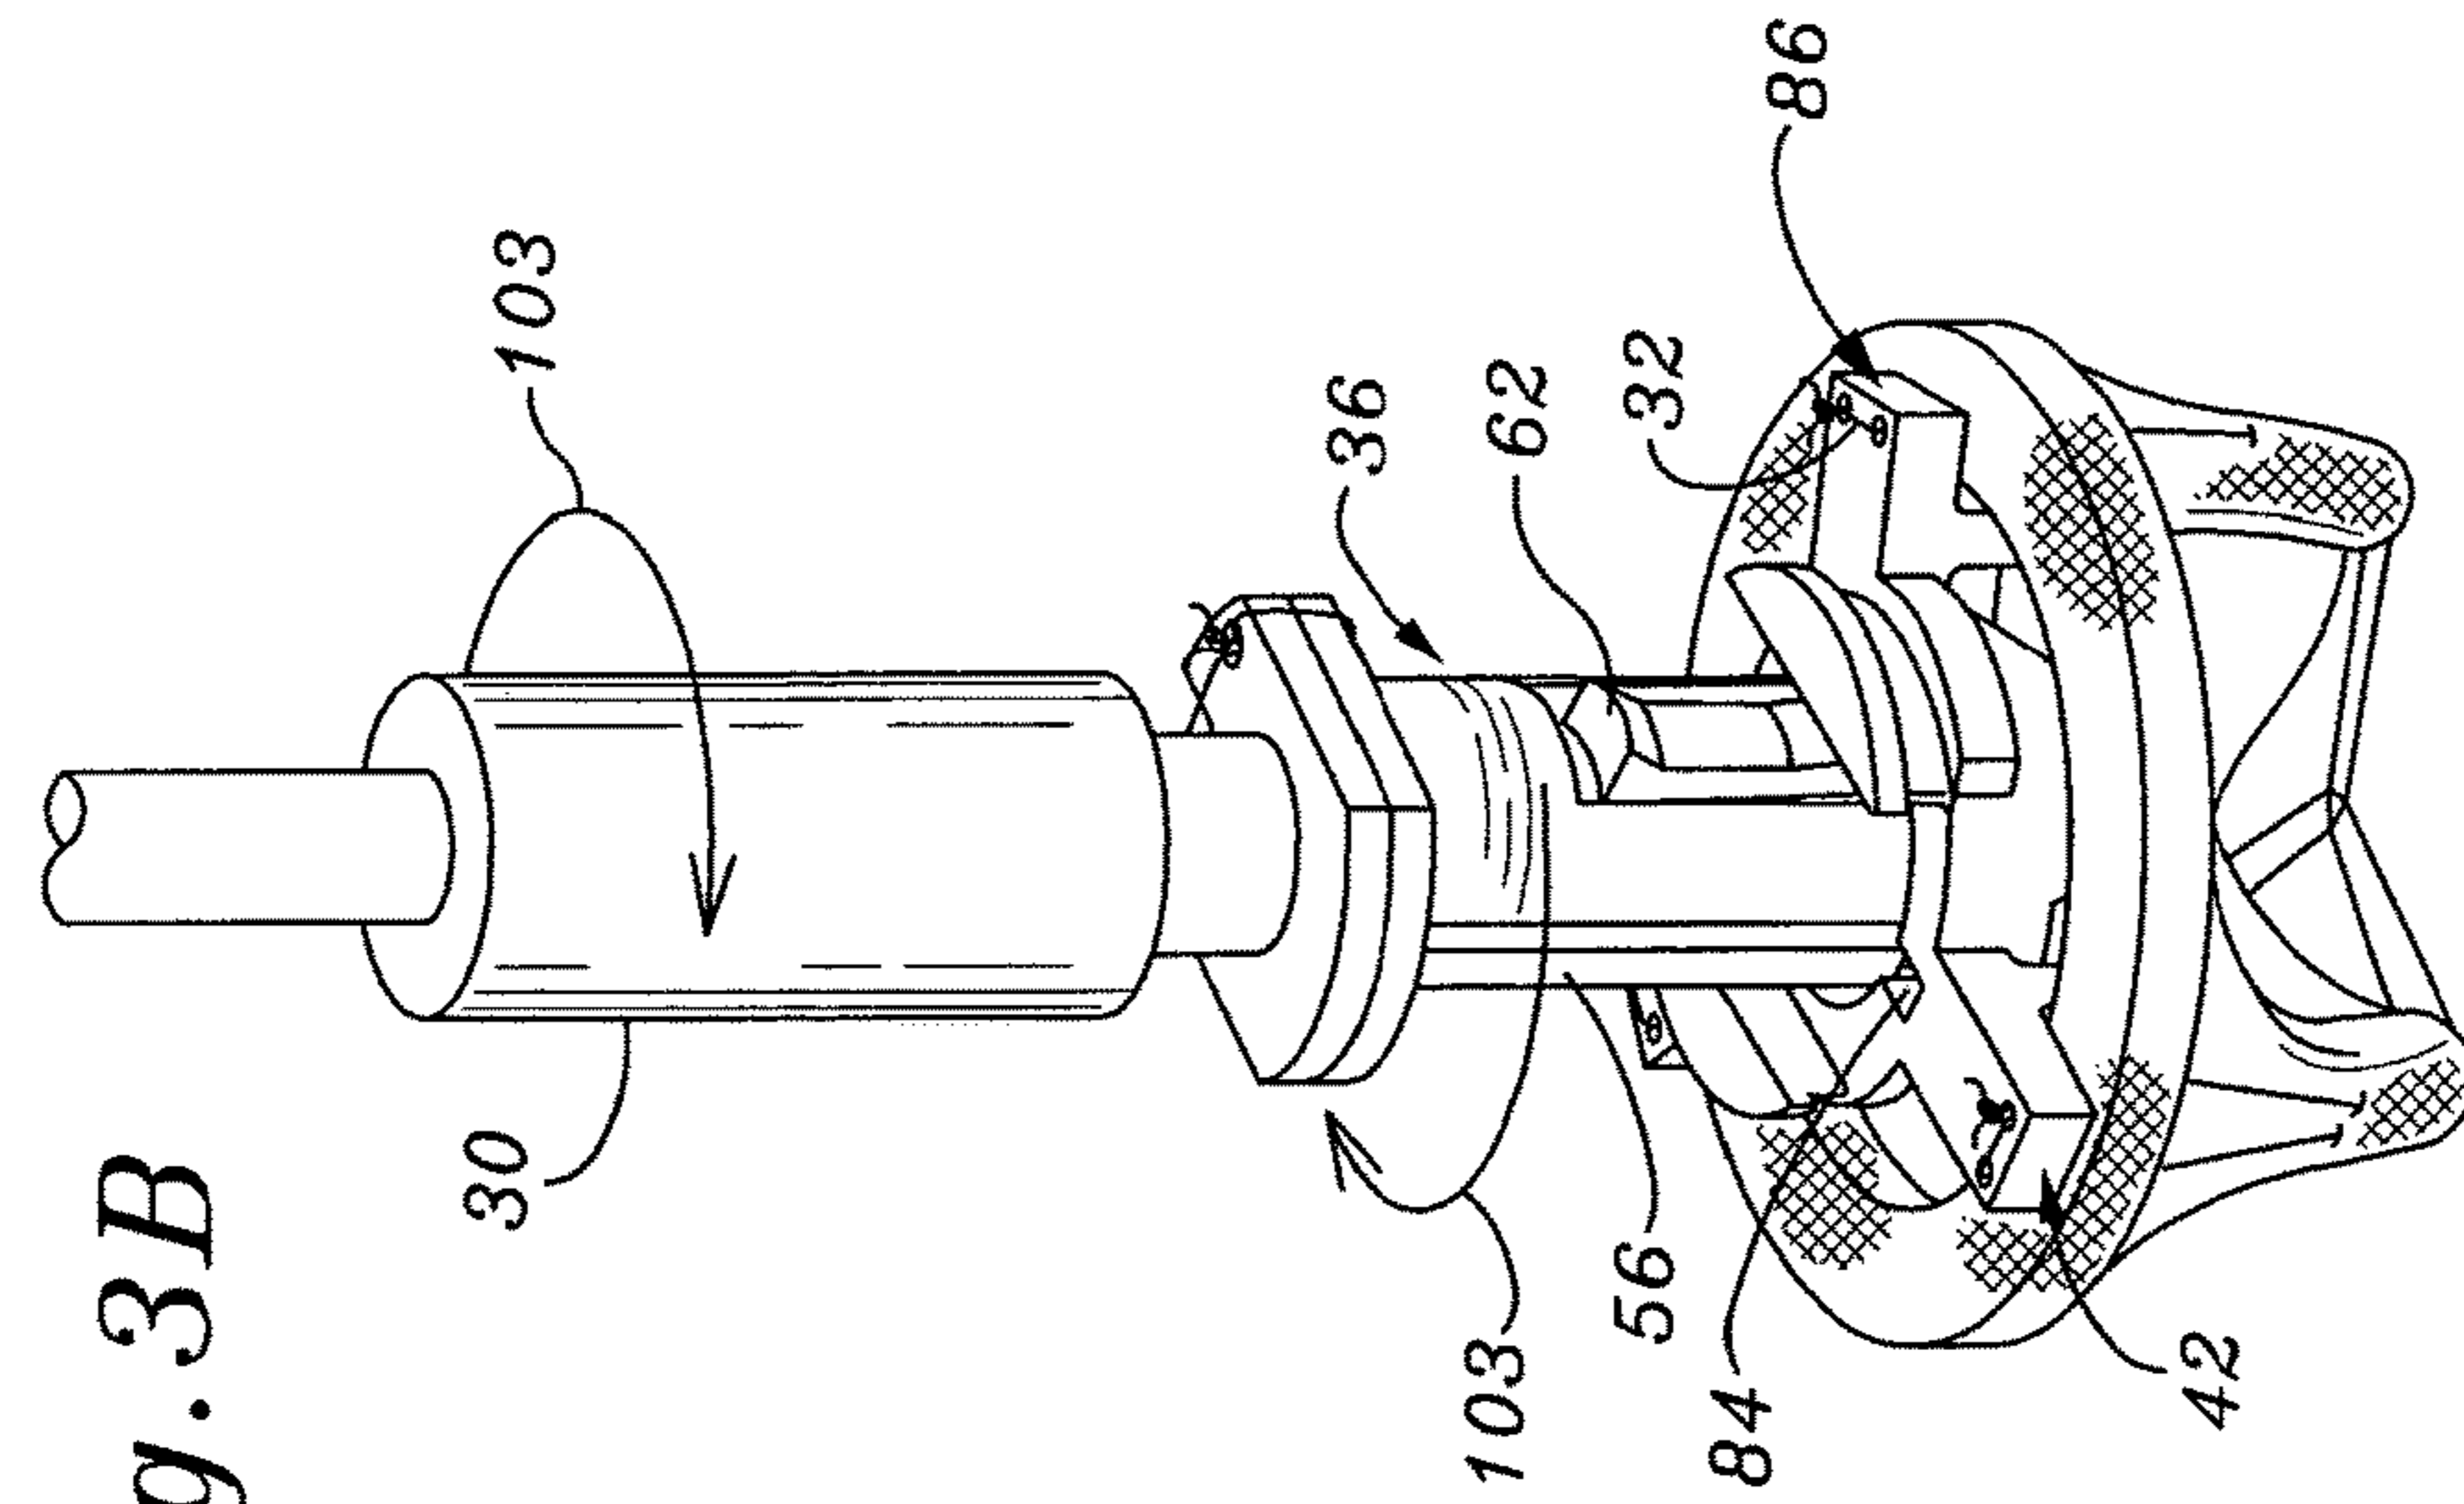


Fig. 3B

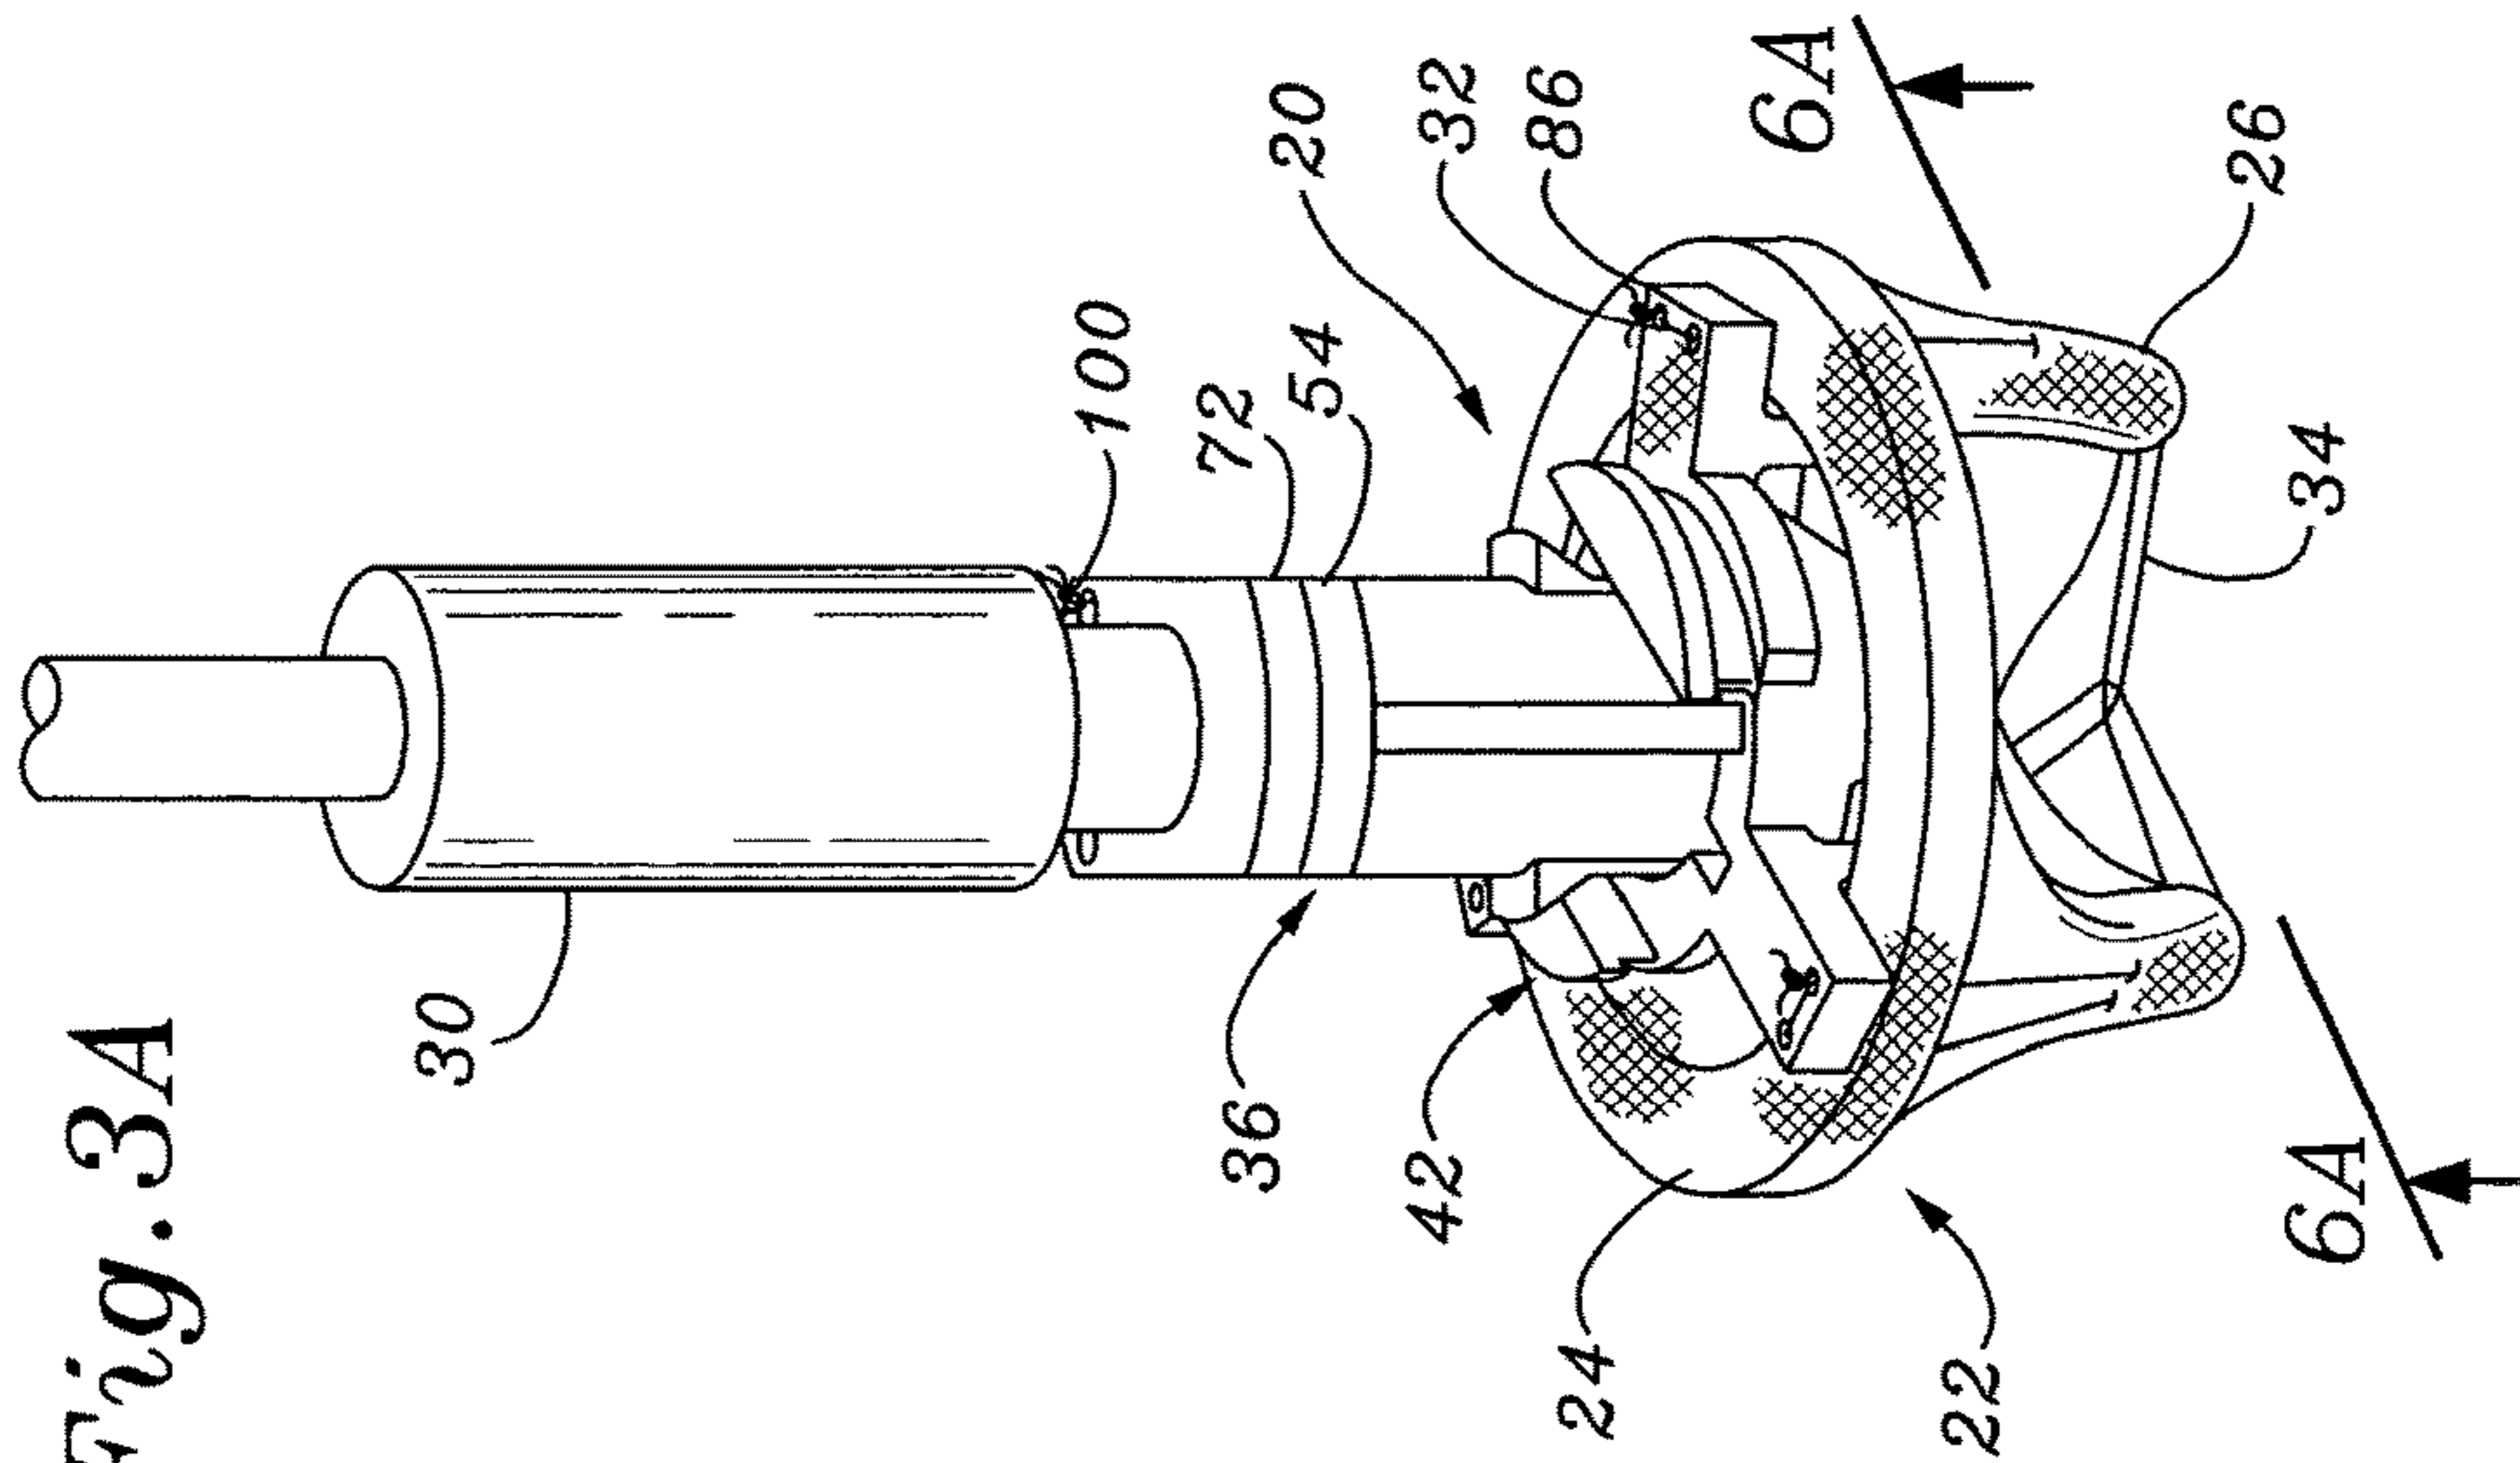


Fig. 3A

Fig. 3C

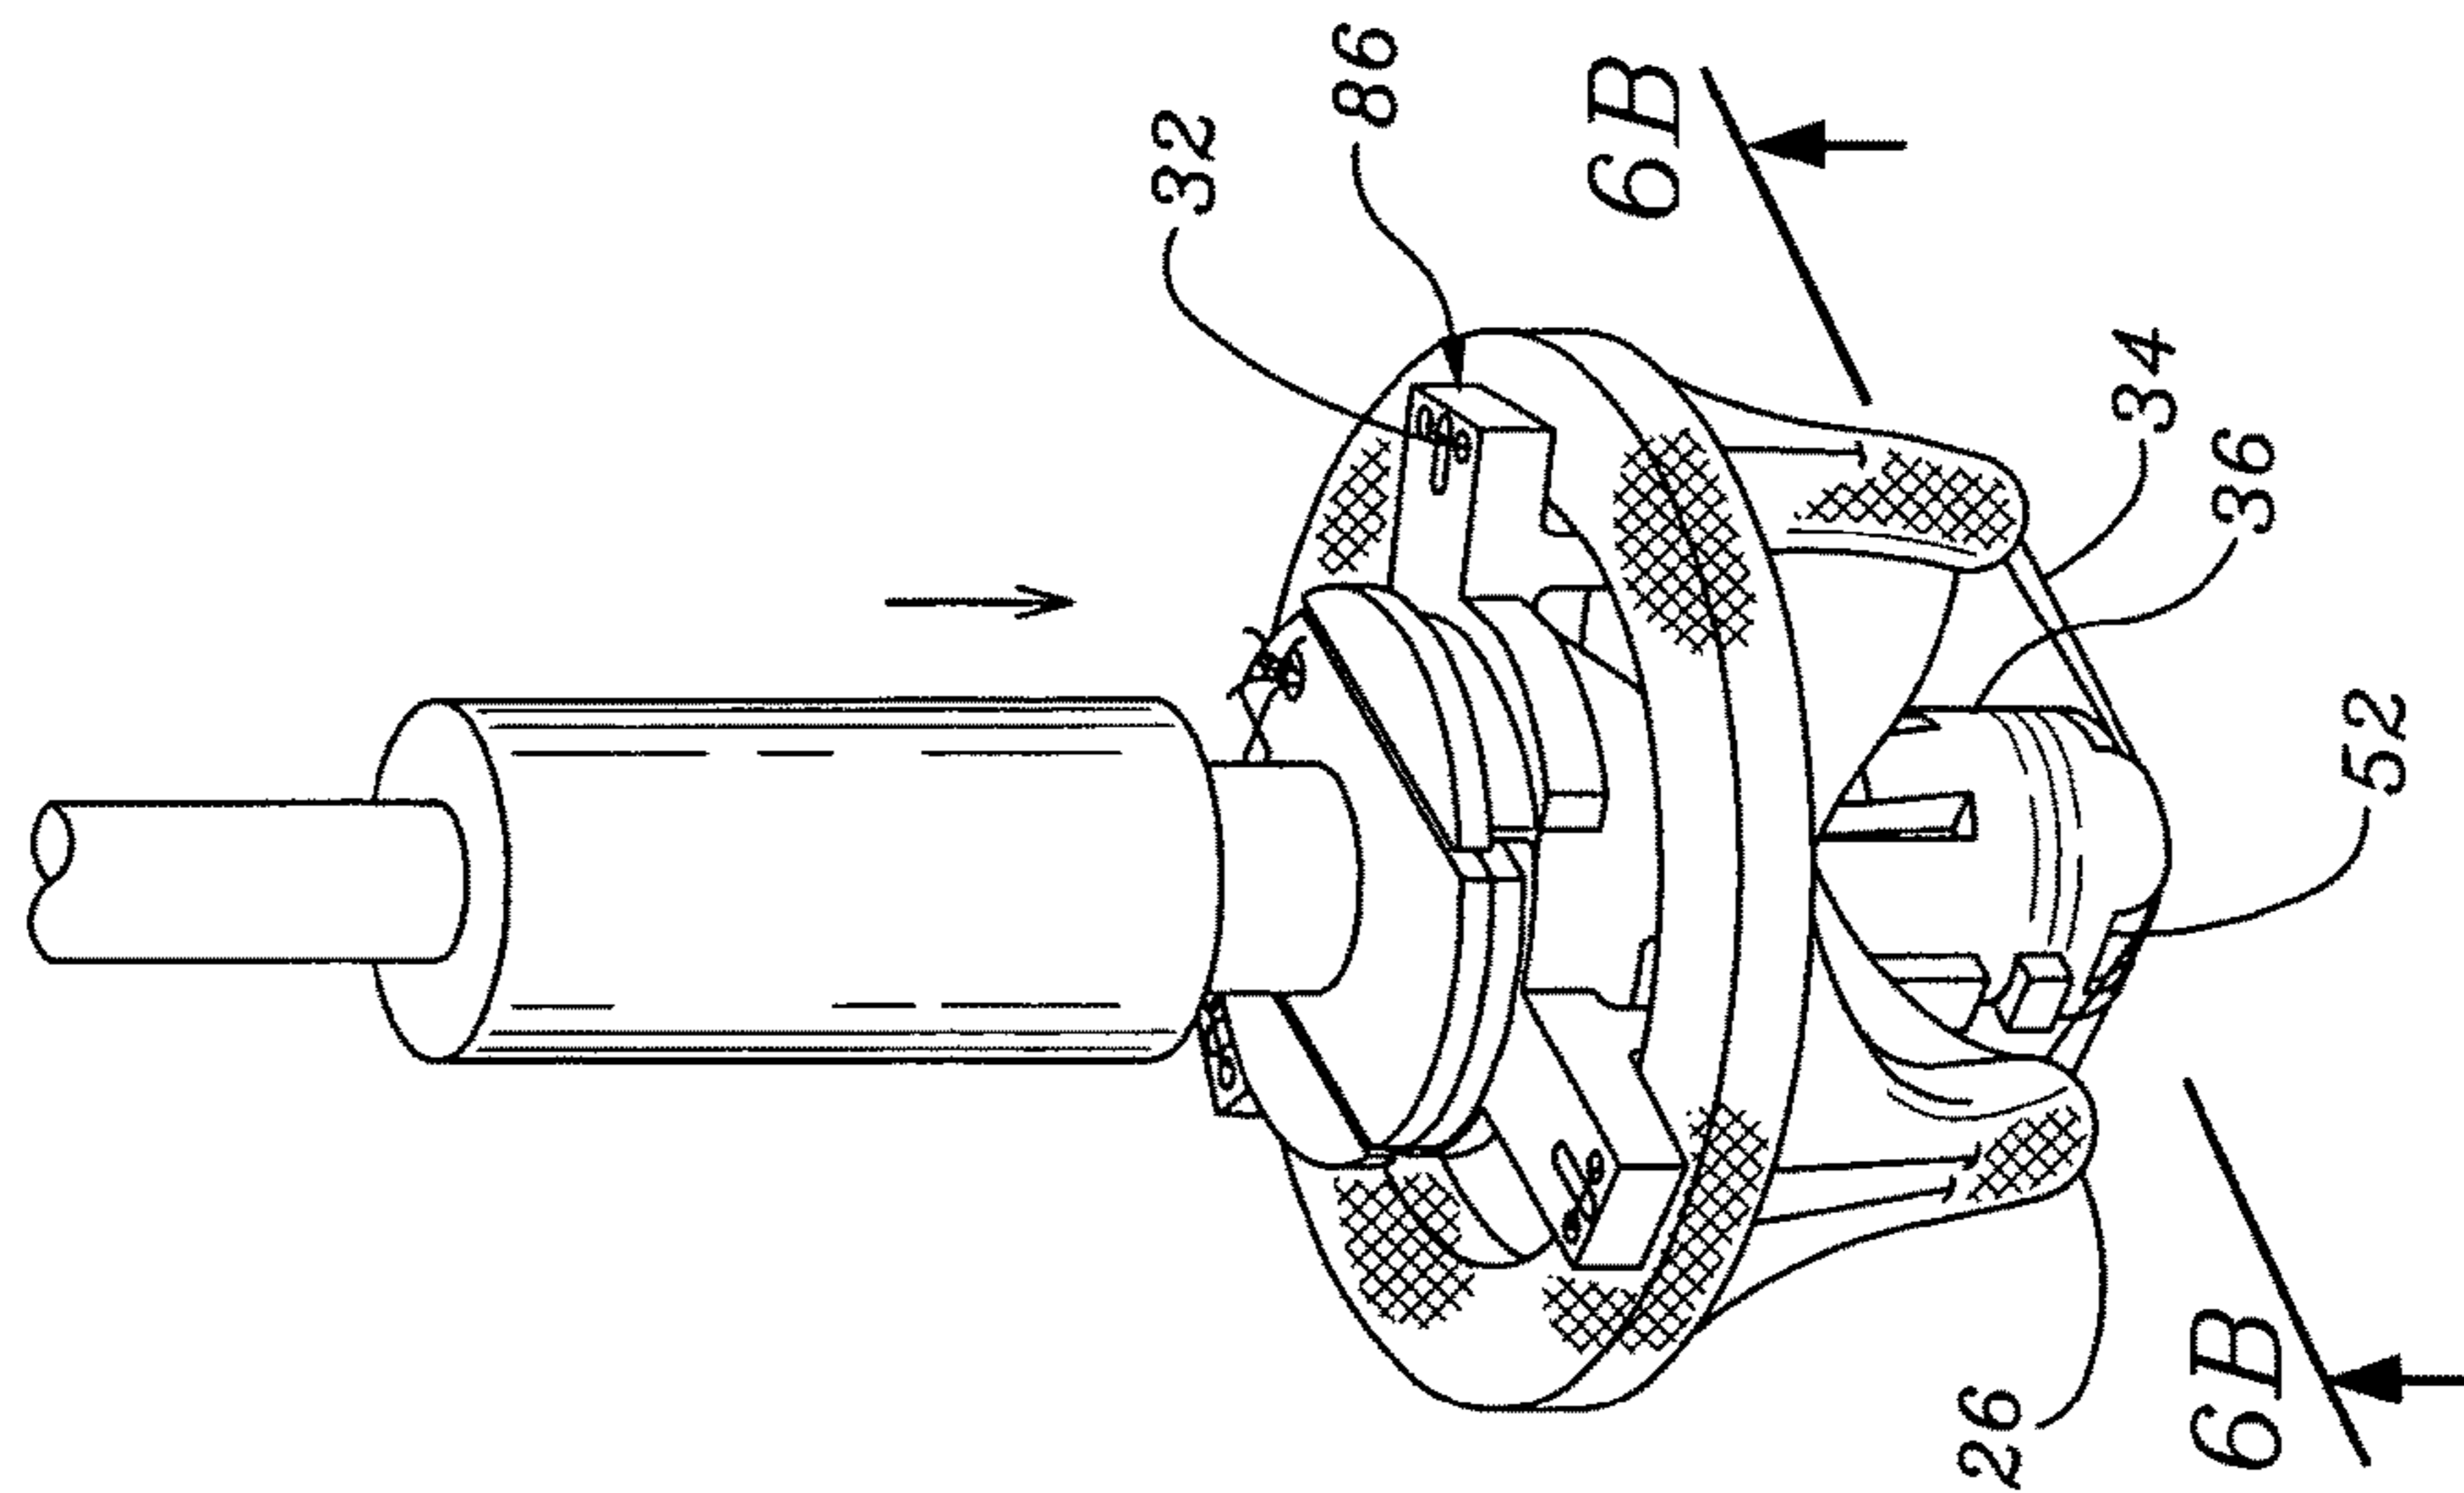


Fig. 3D

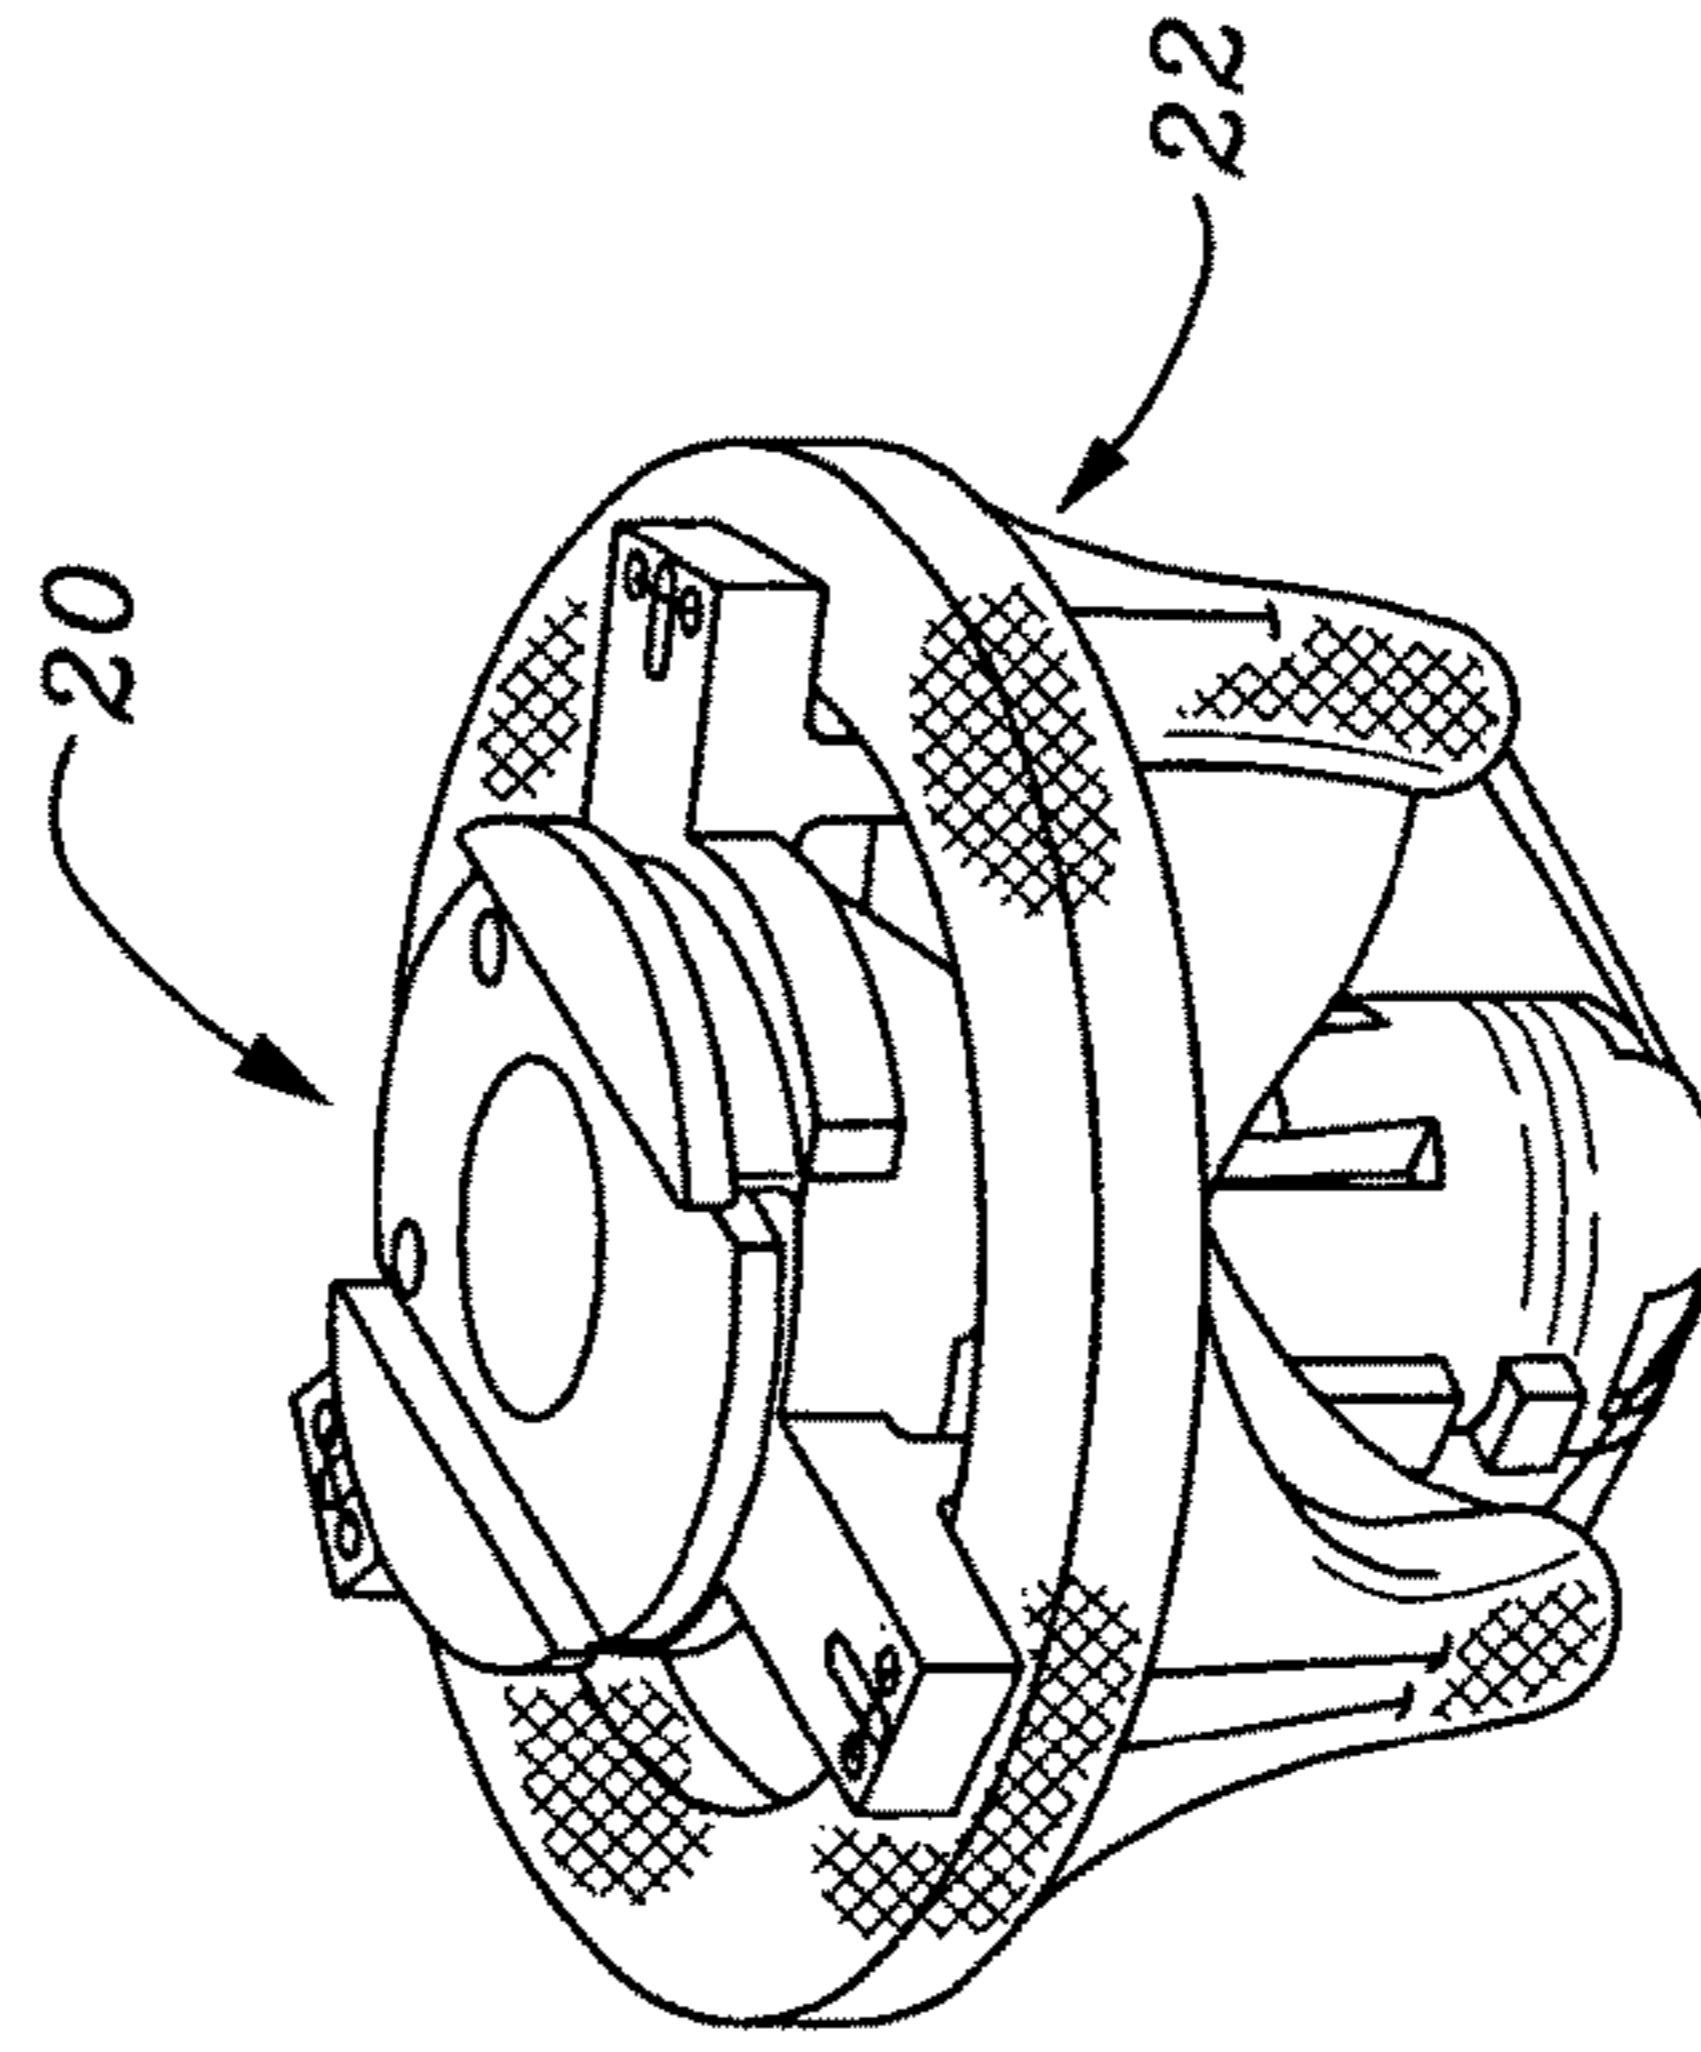


Fig. 4A

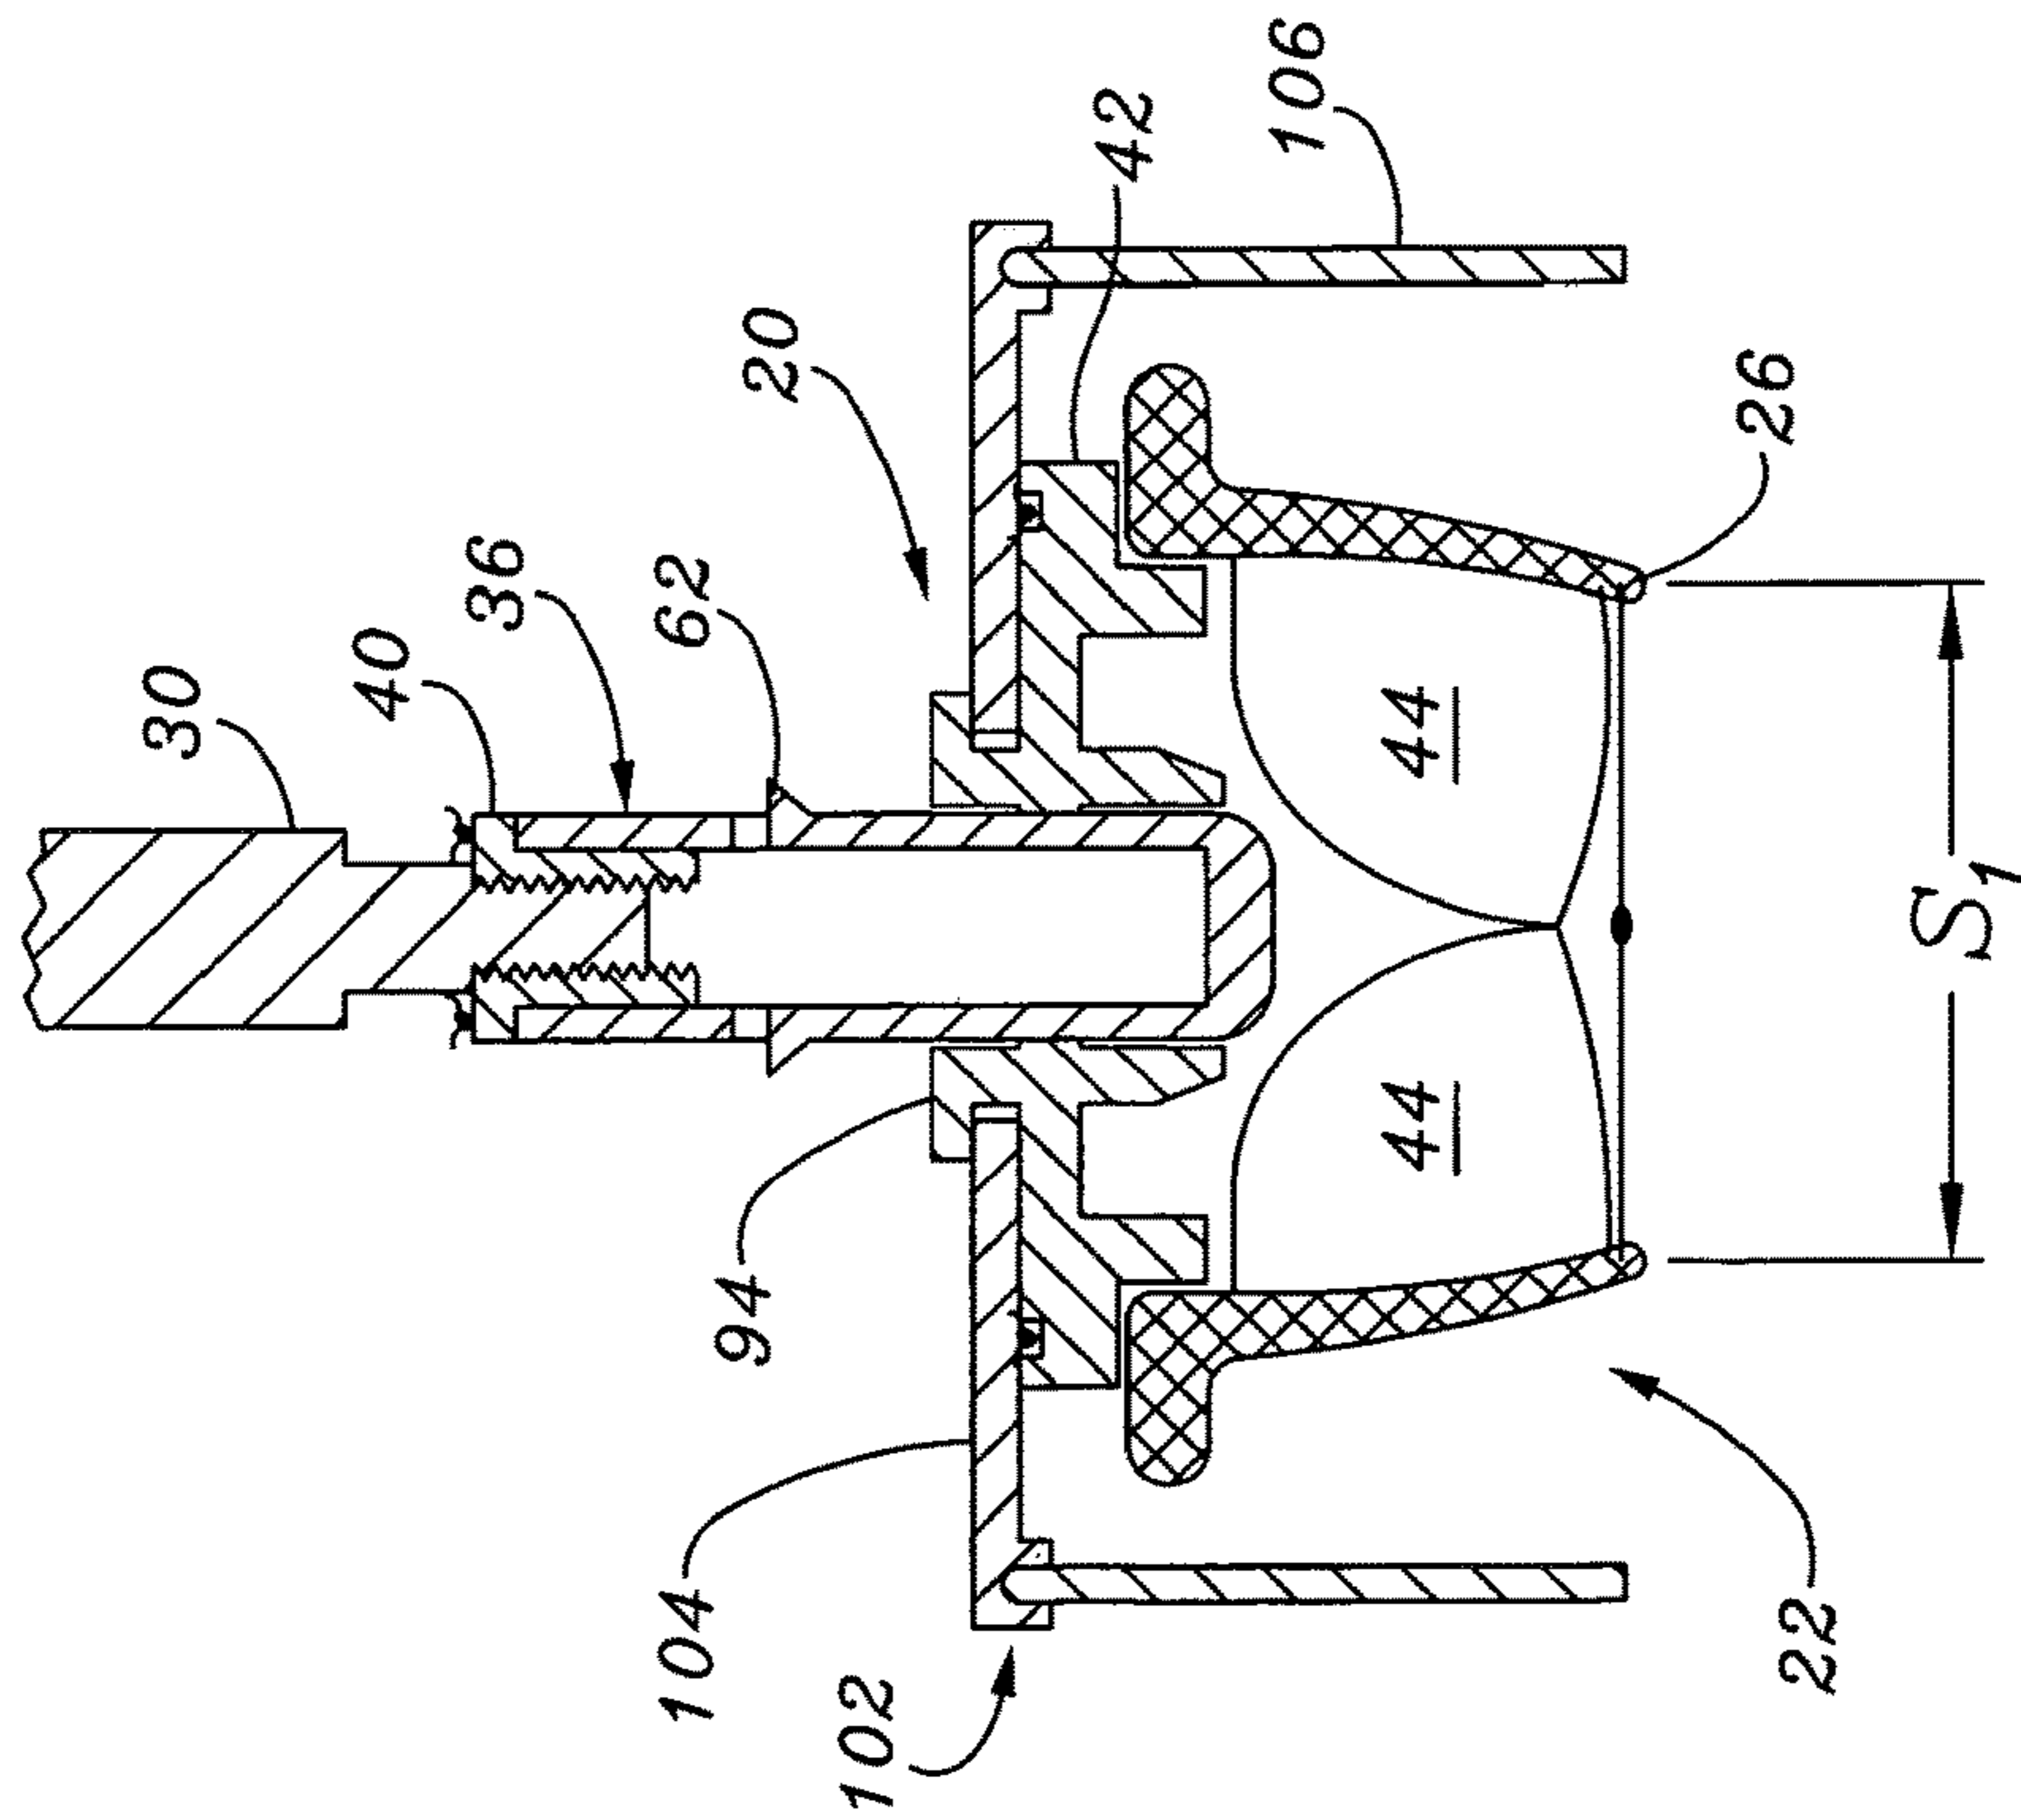
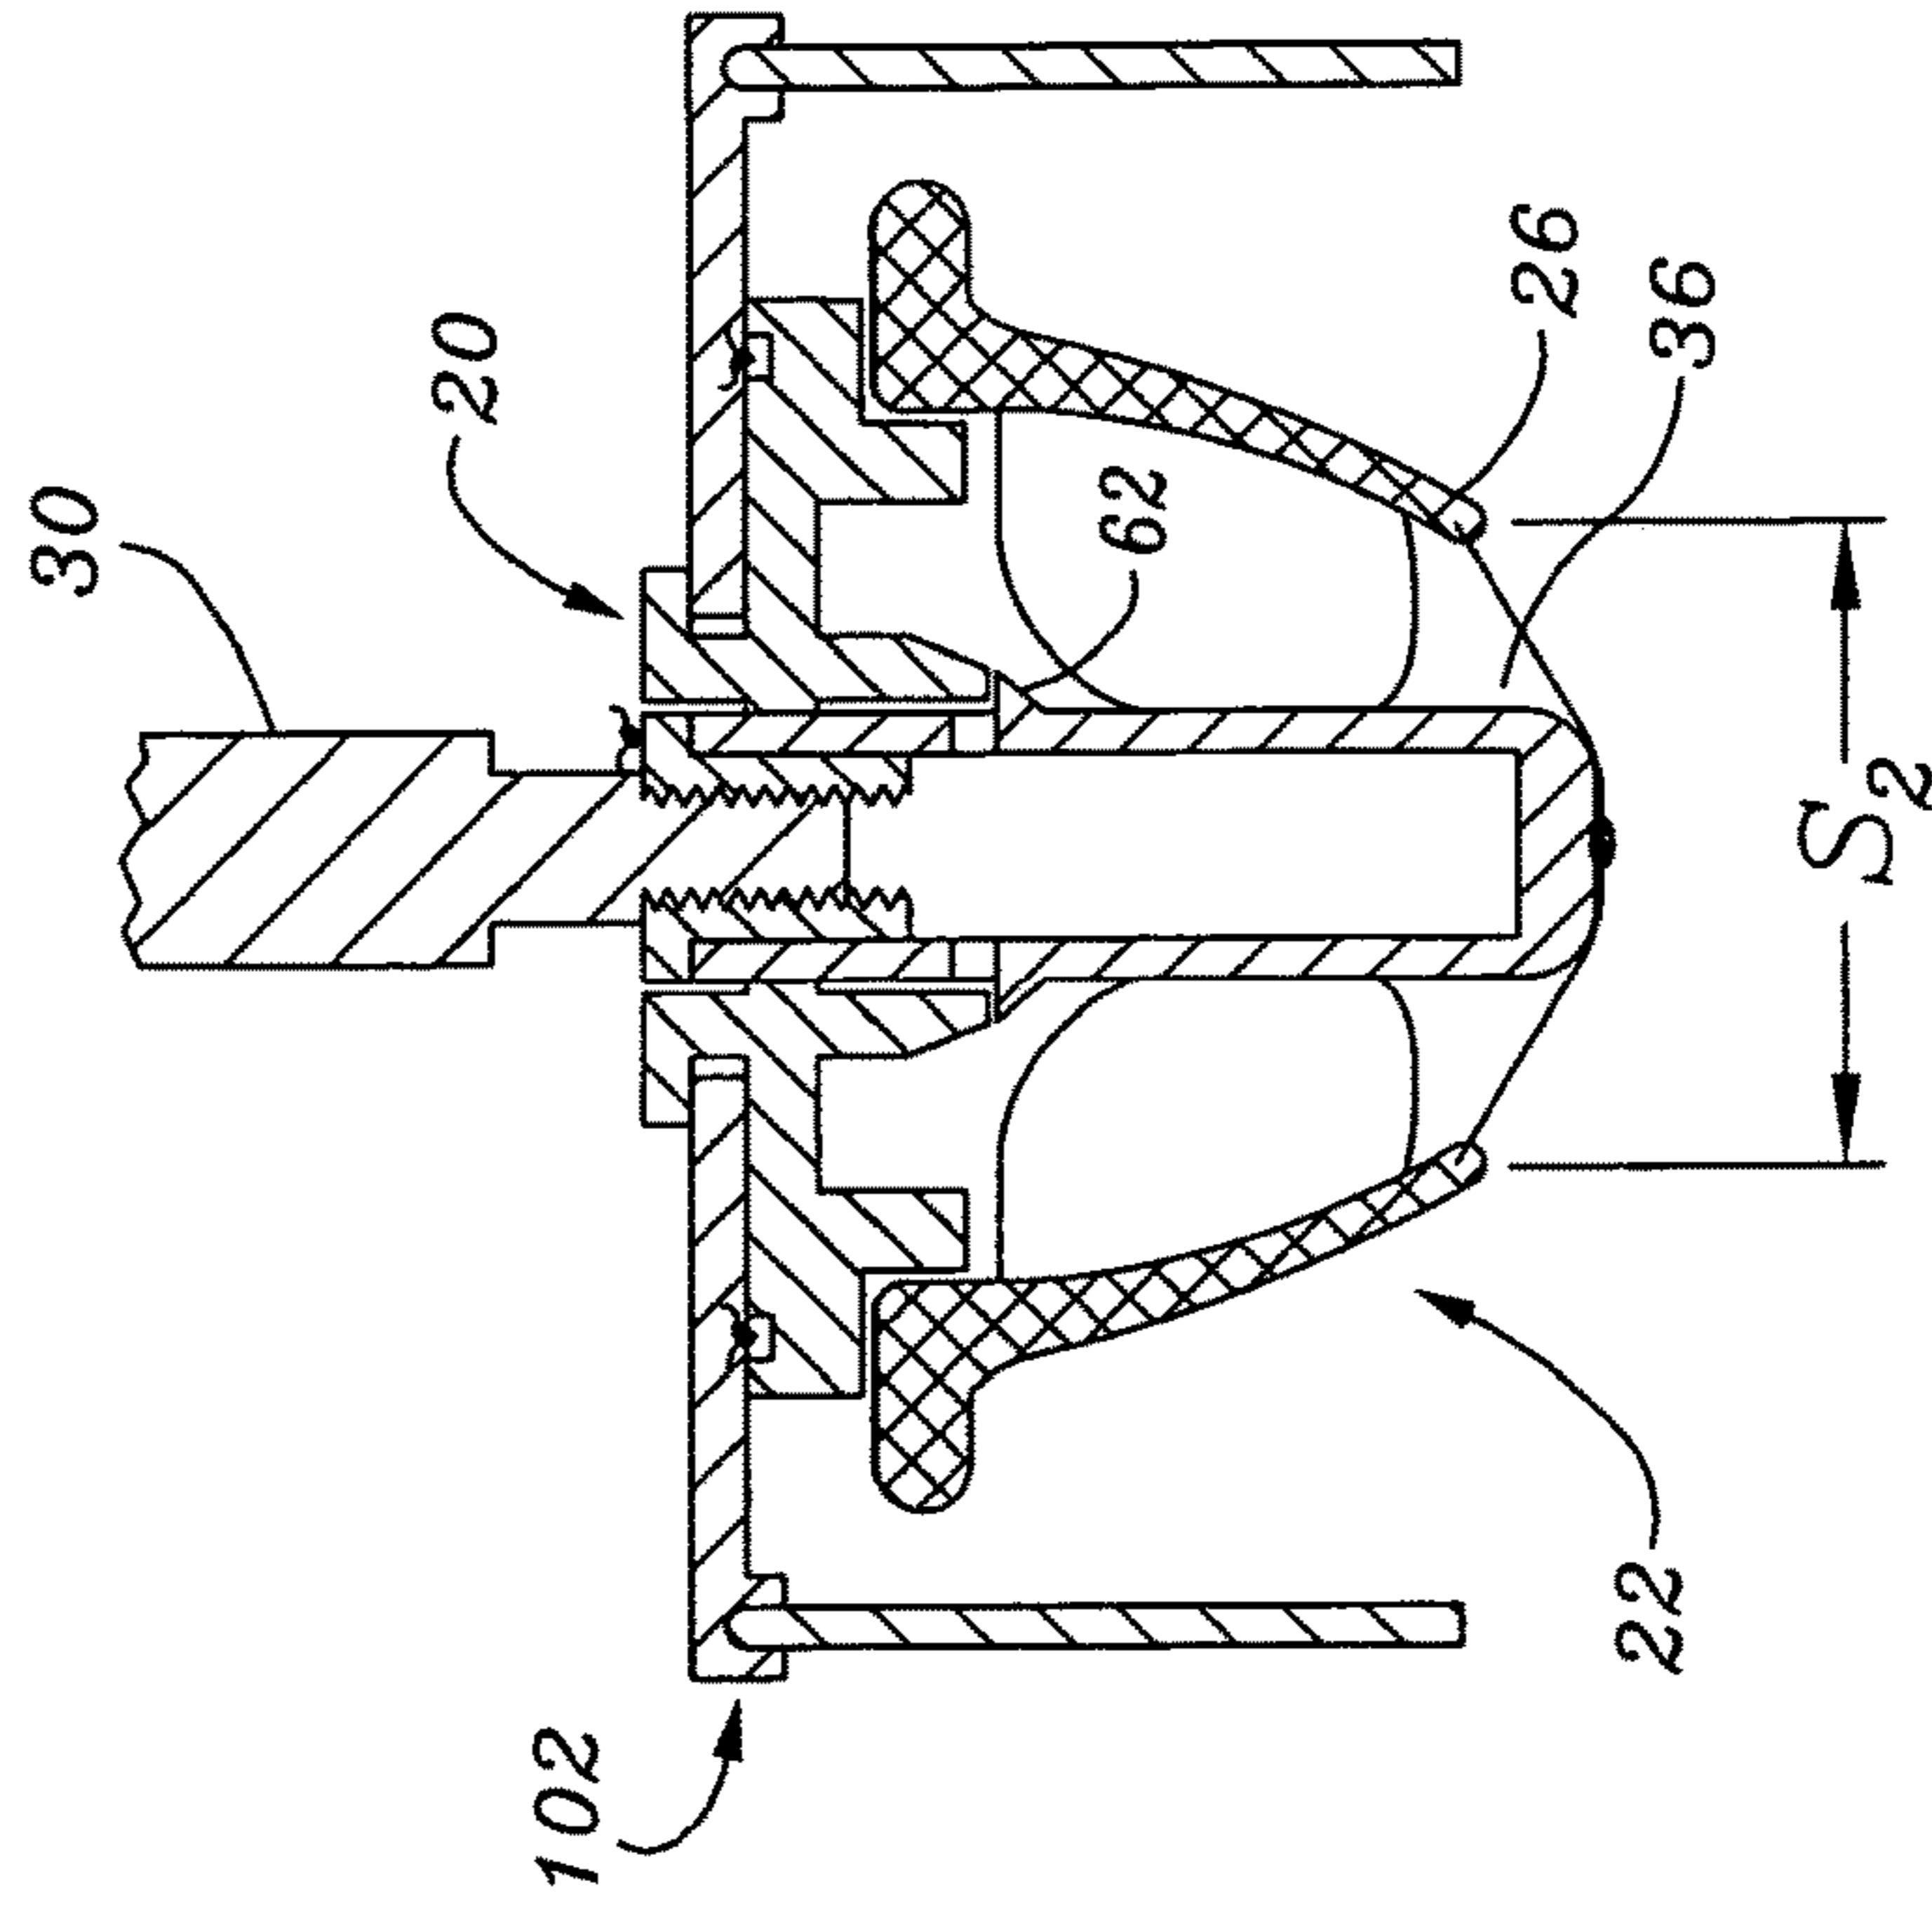


Fig. 4B



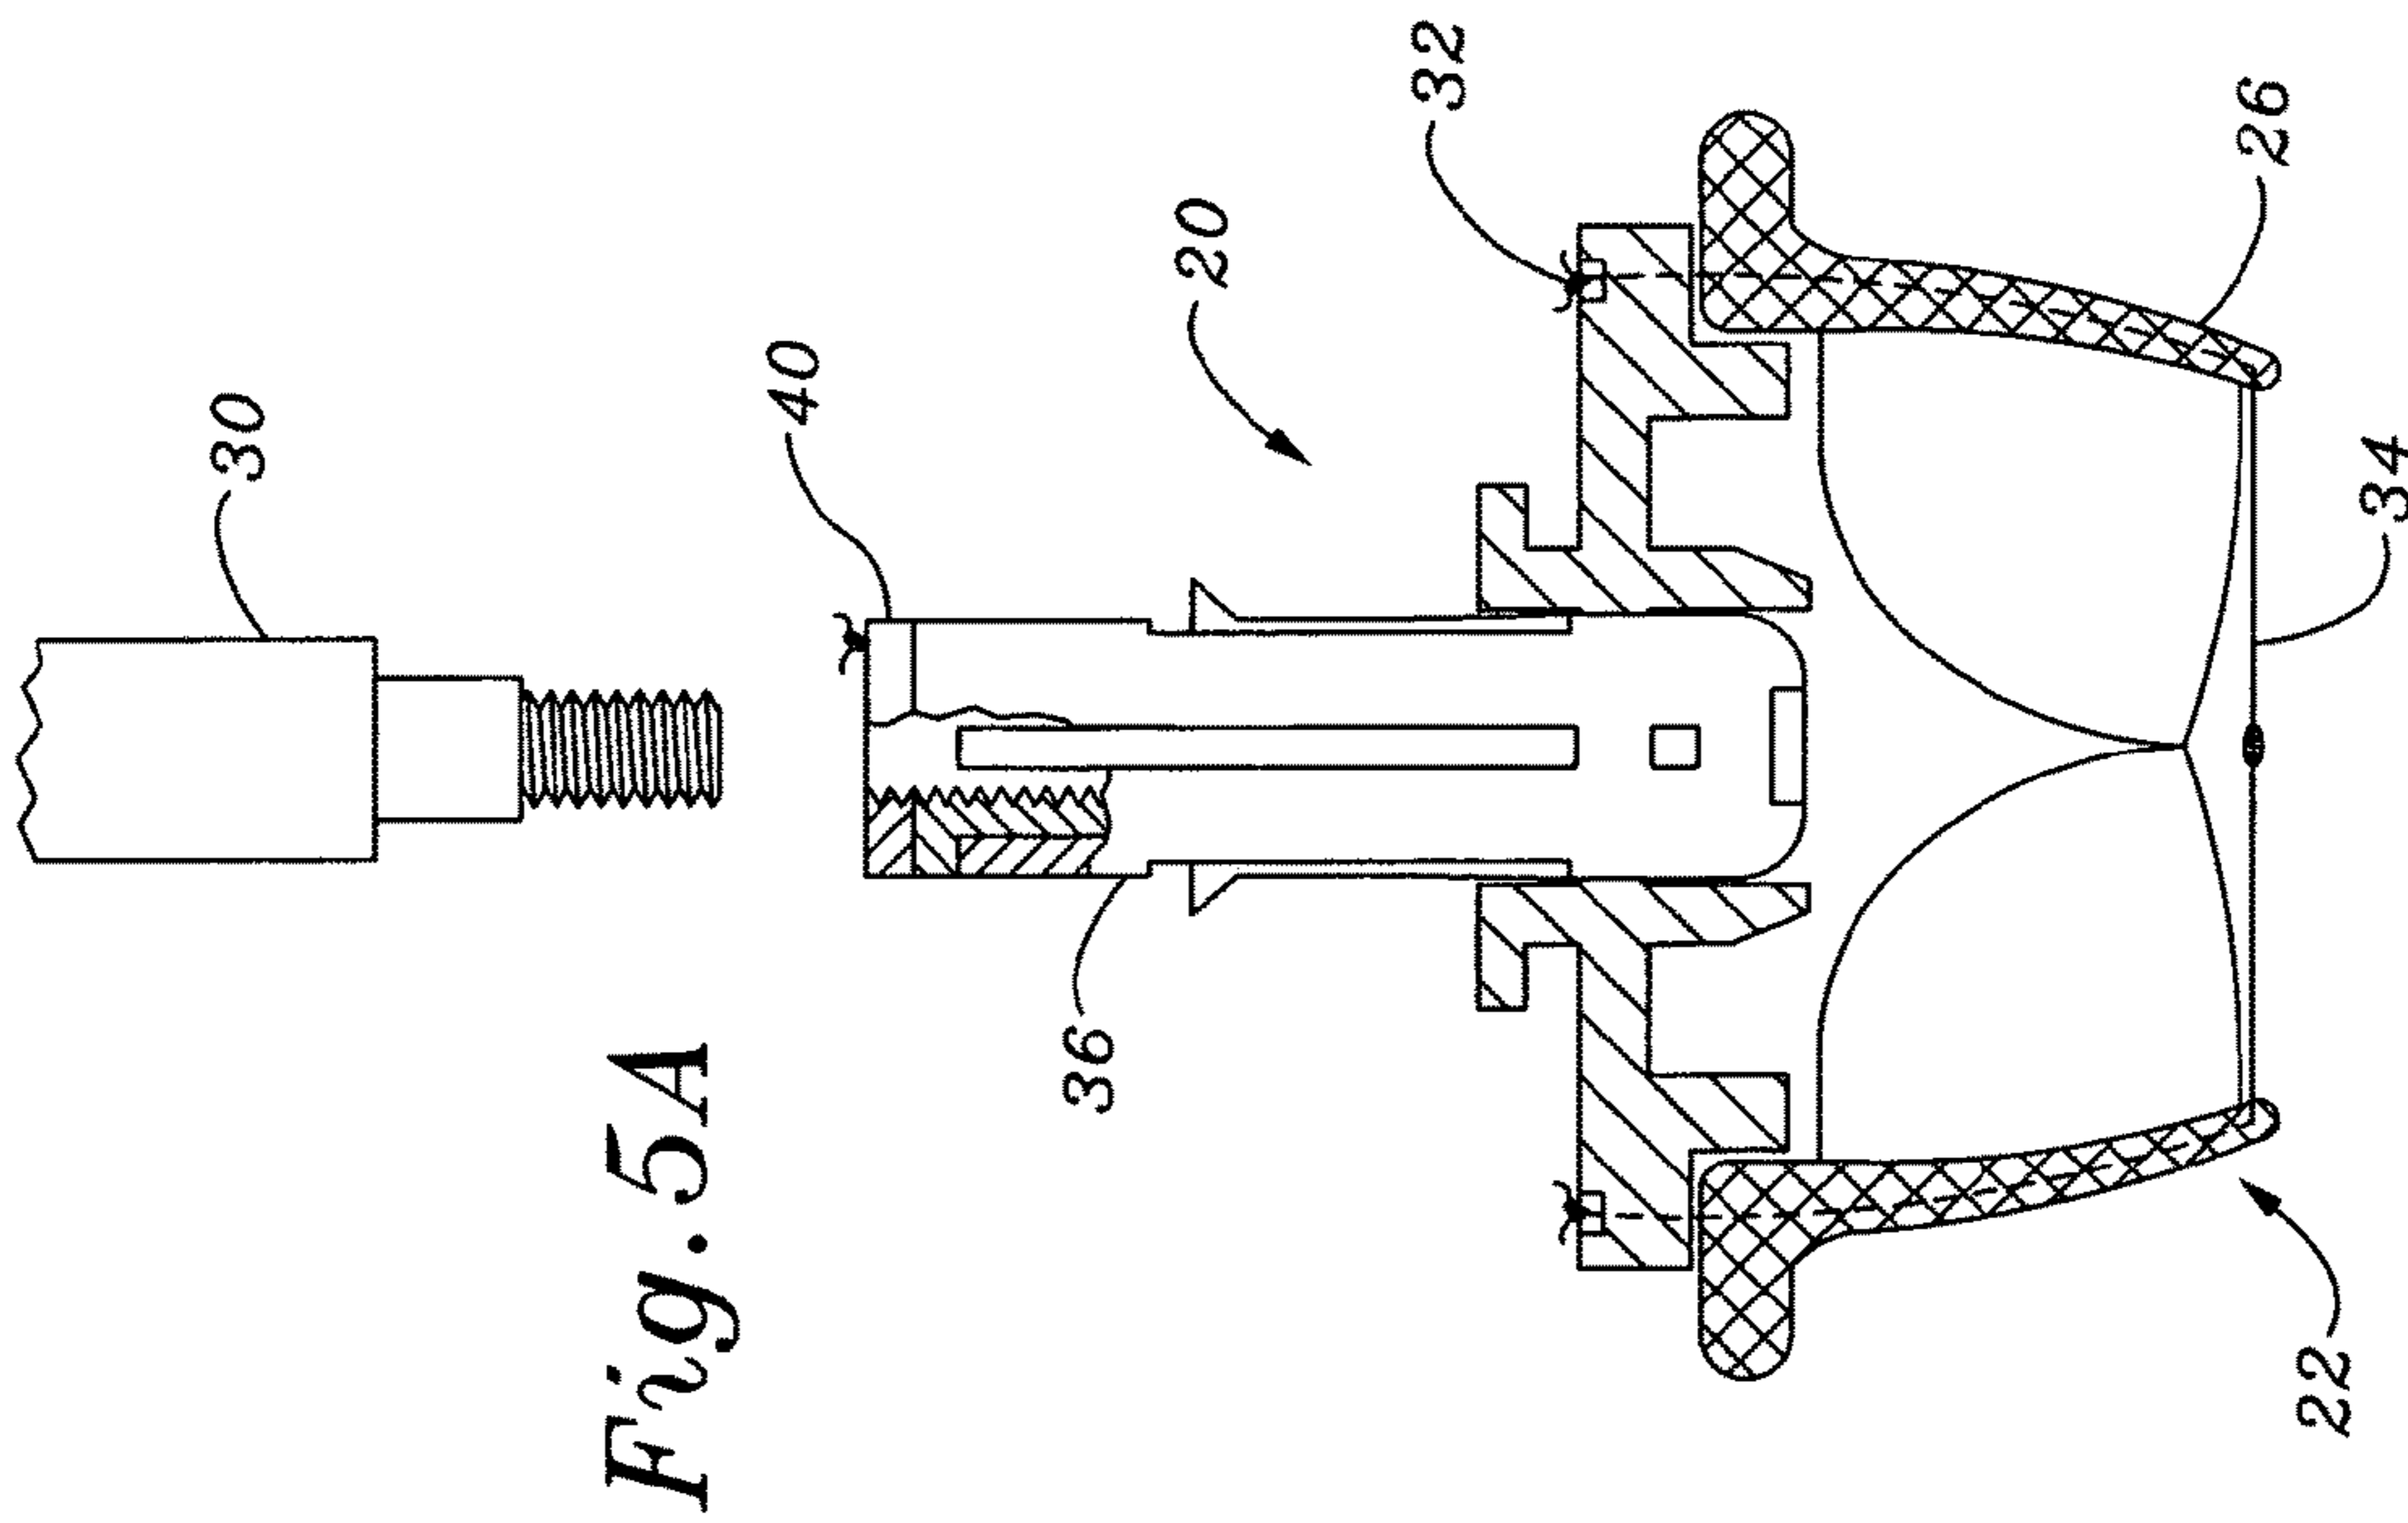
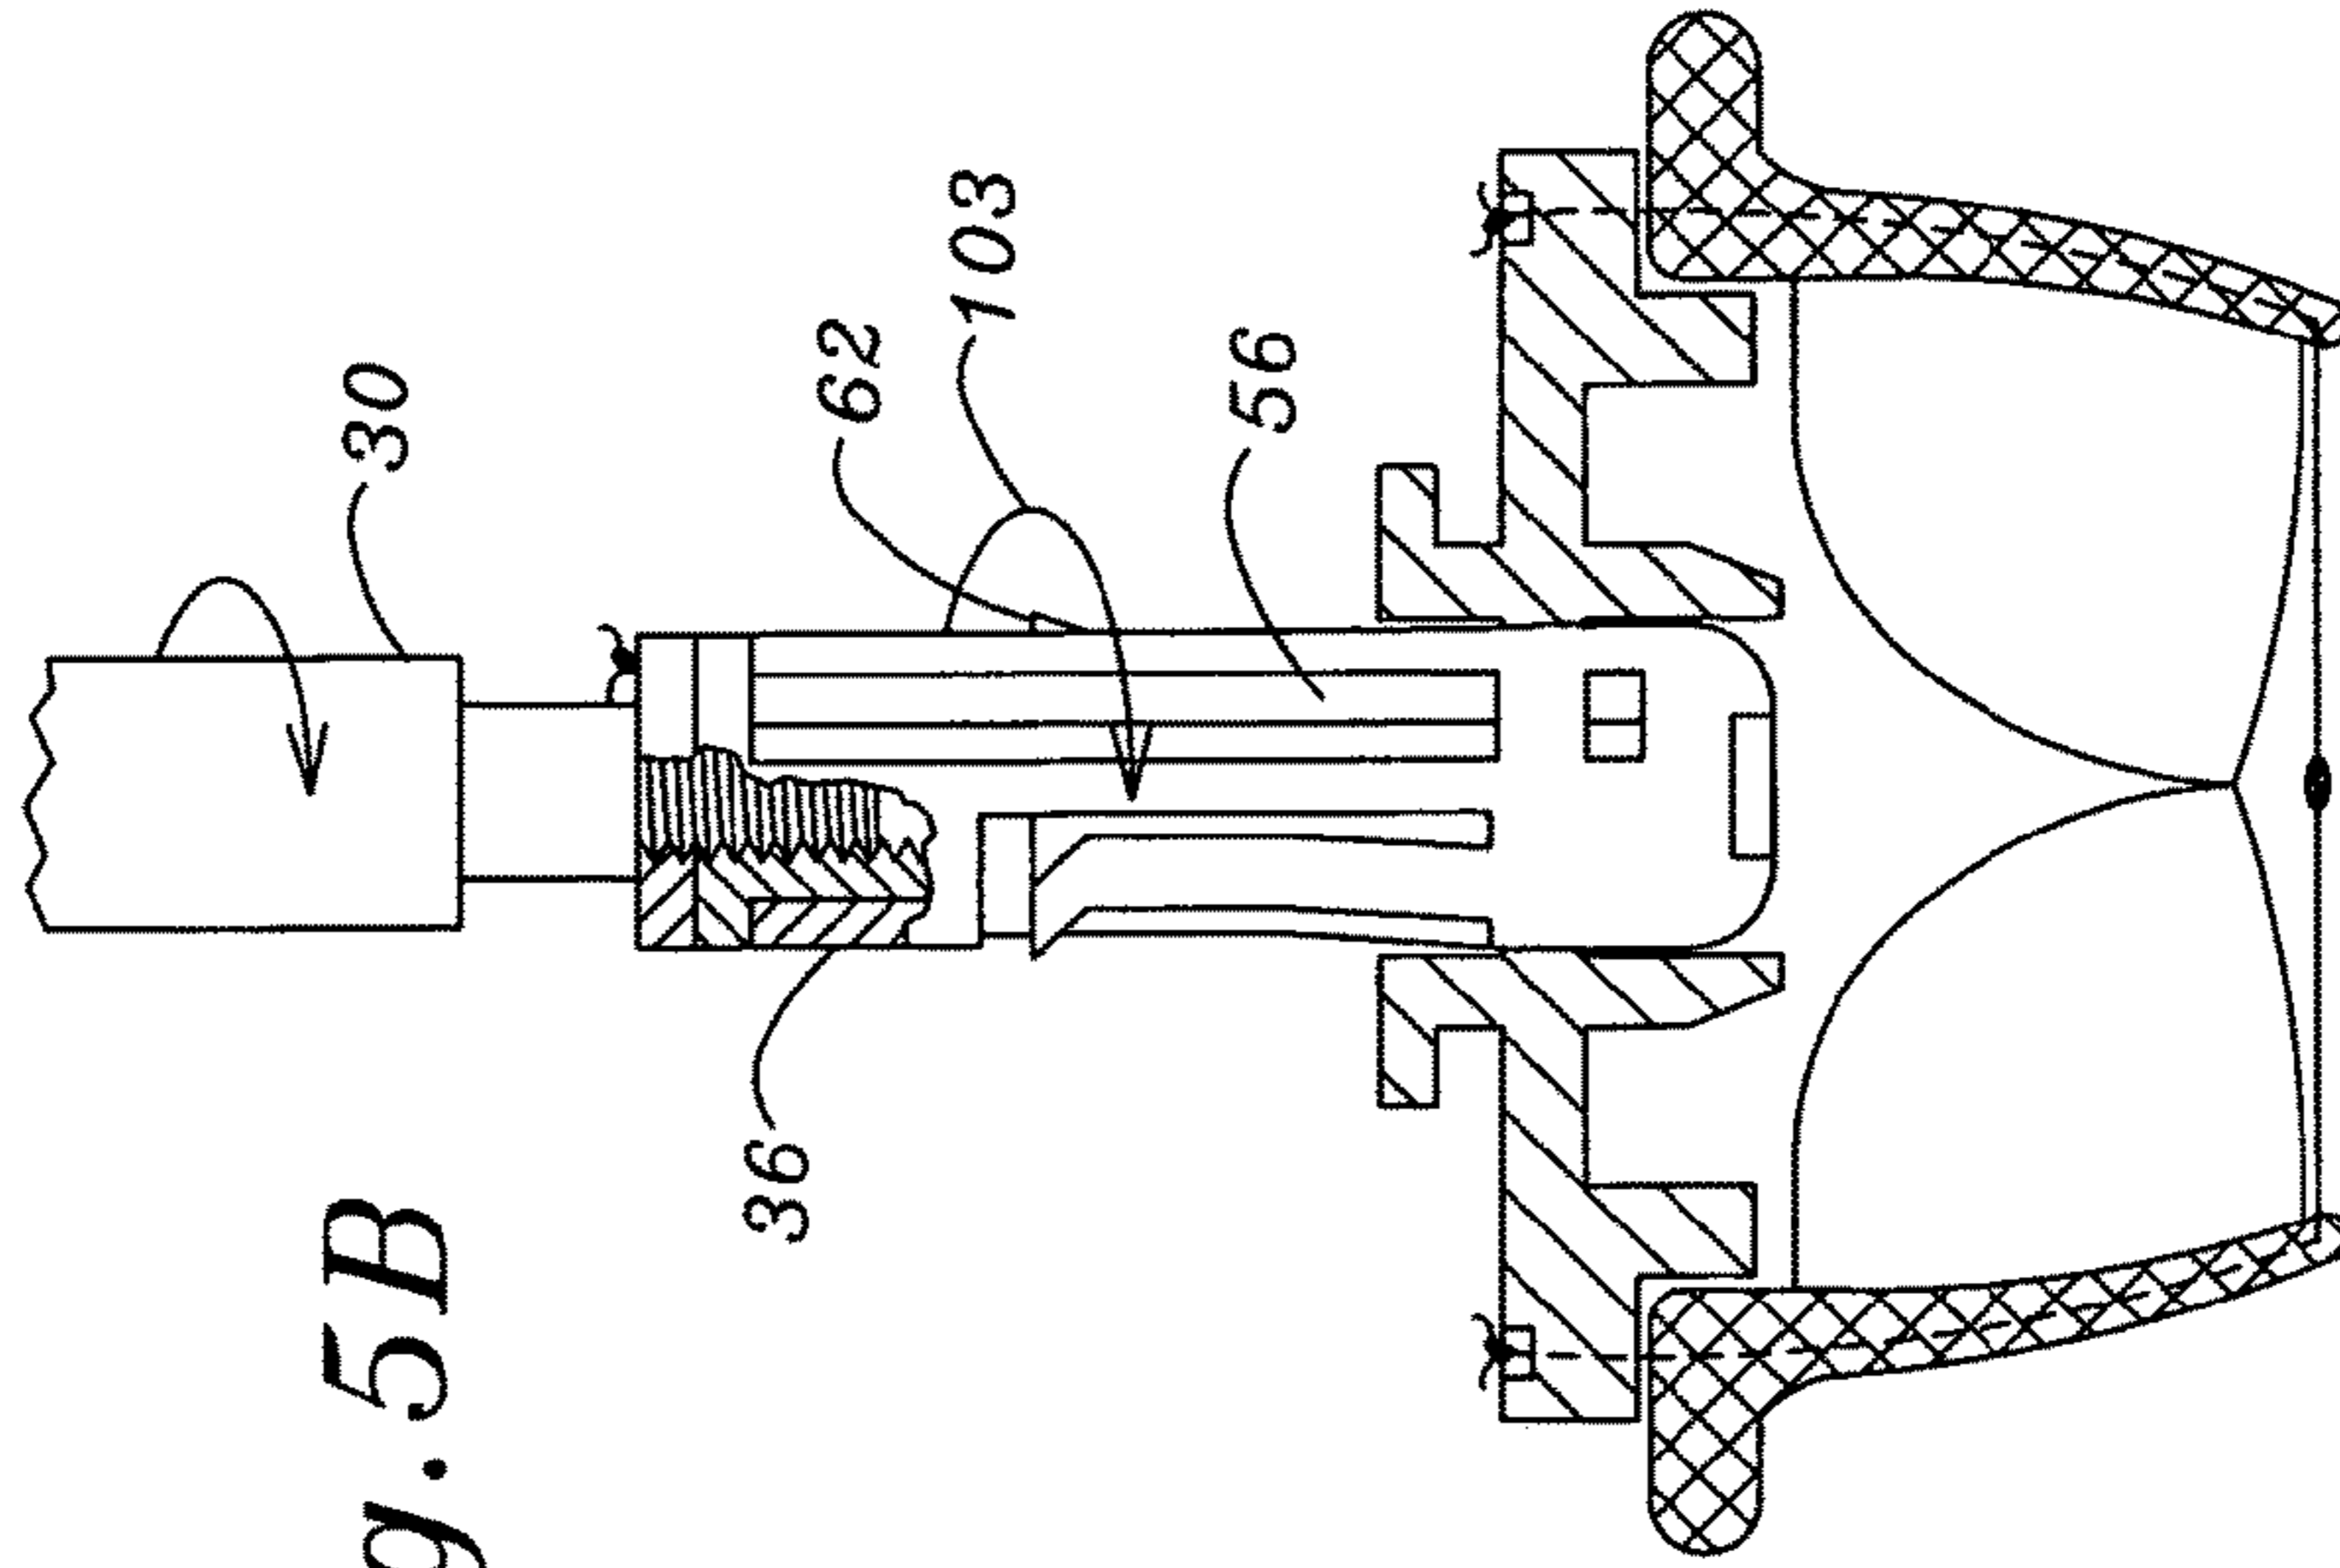


Fig. 5B



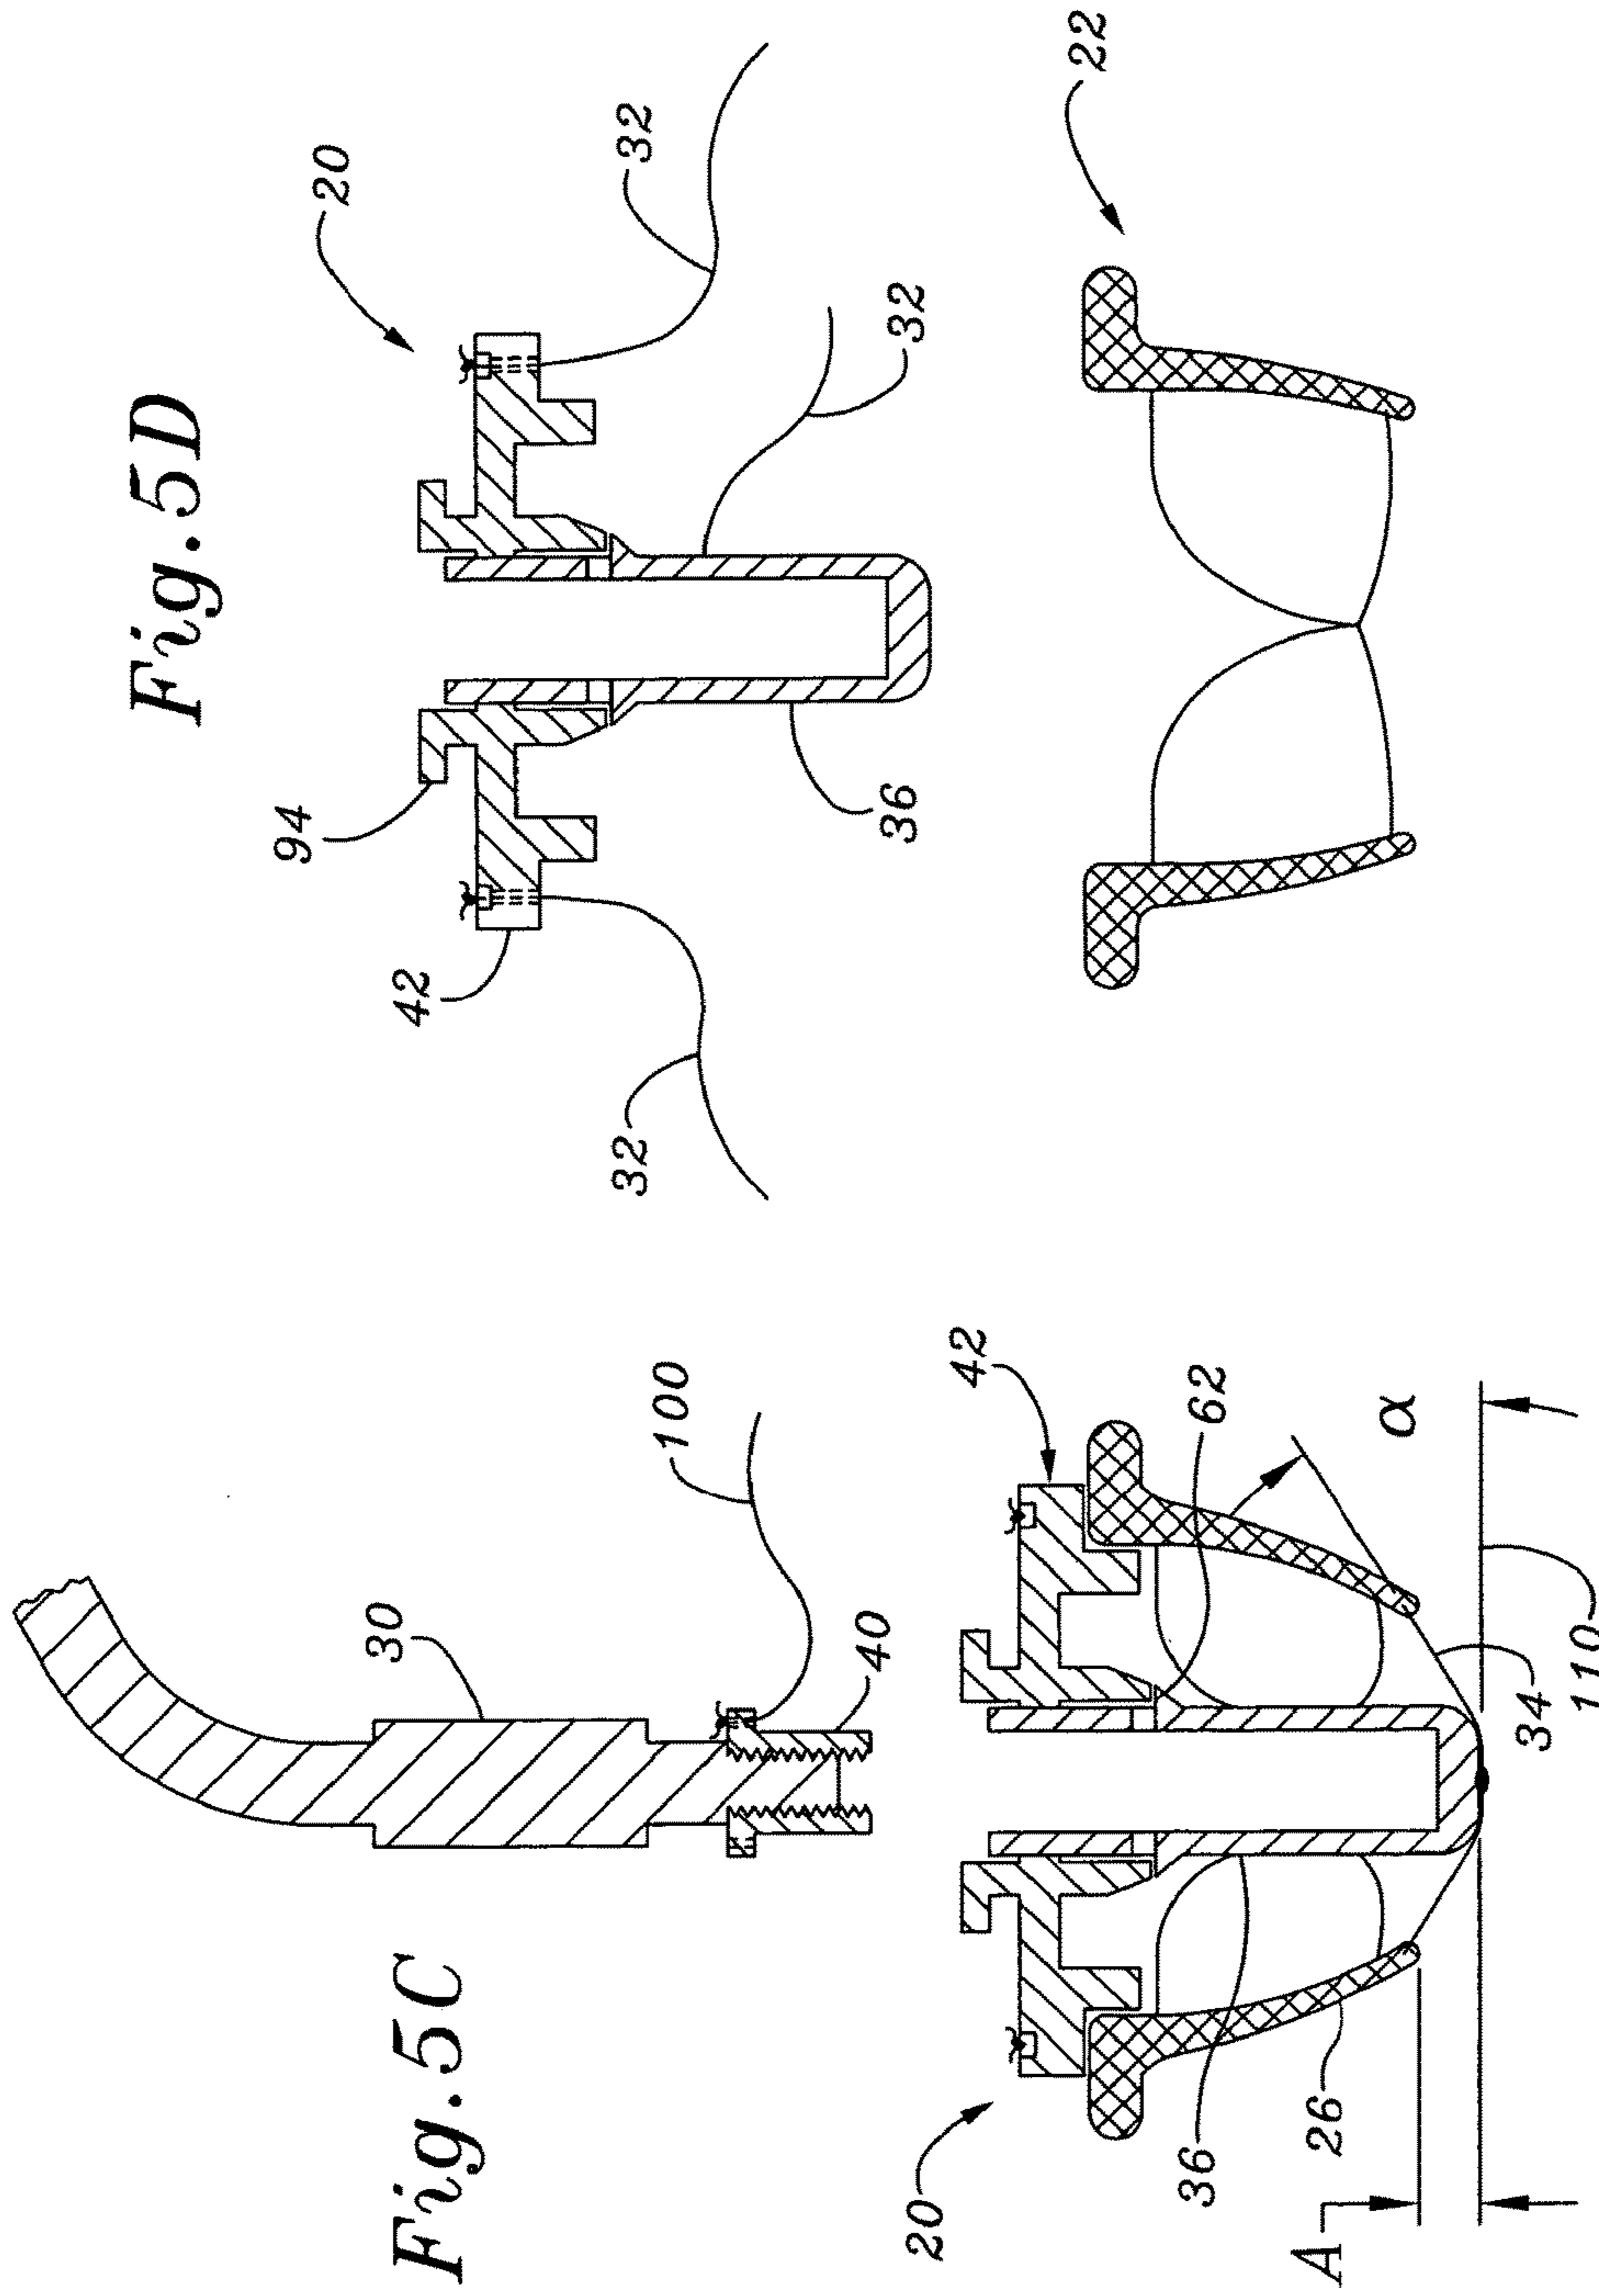


Fig. 6B

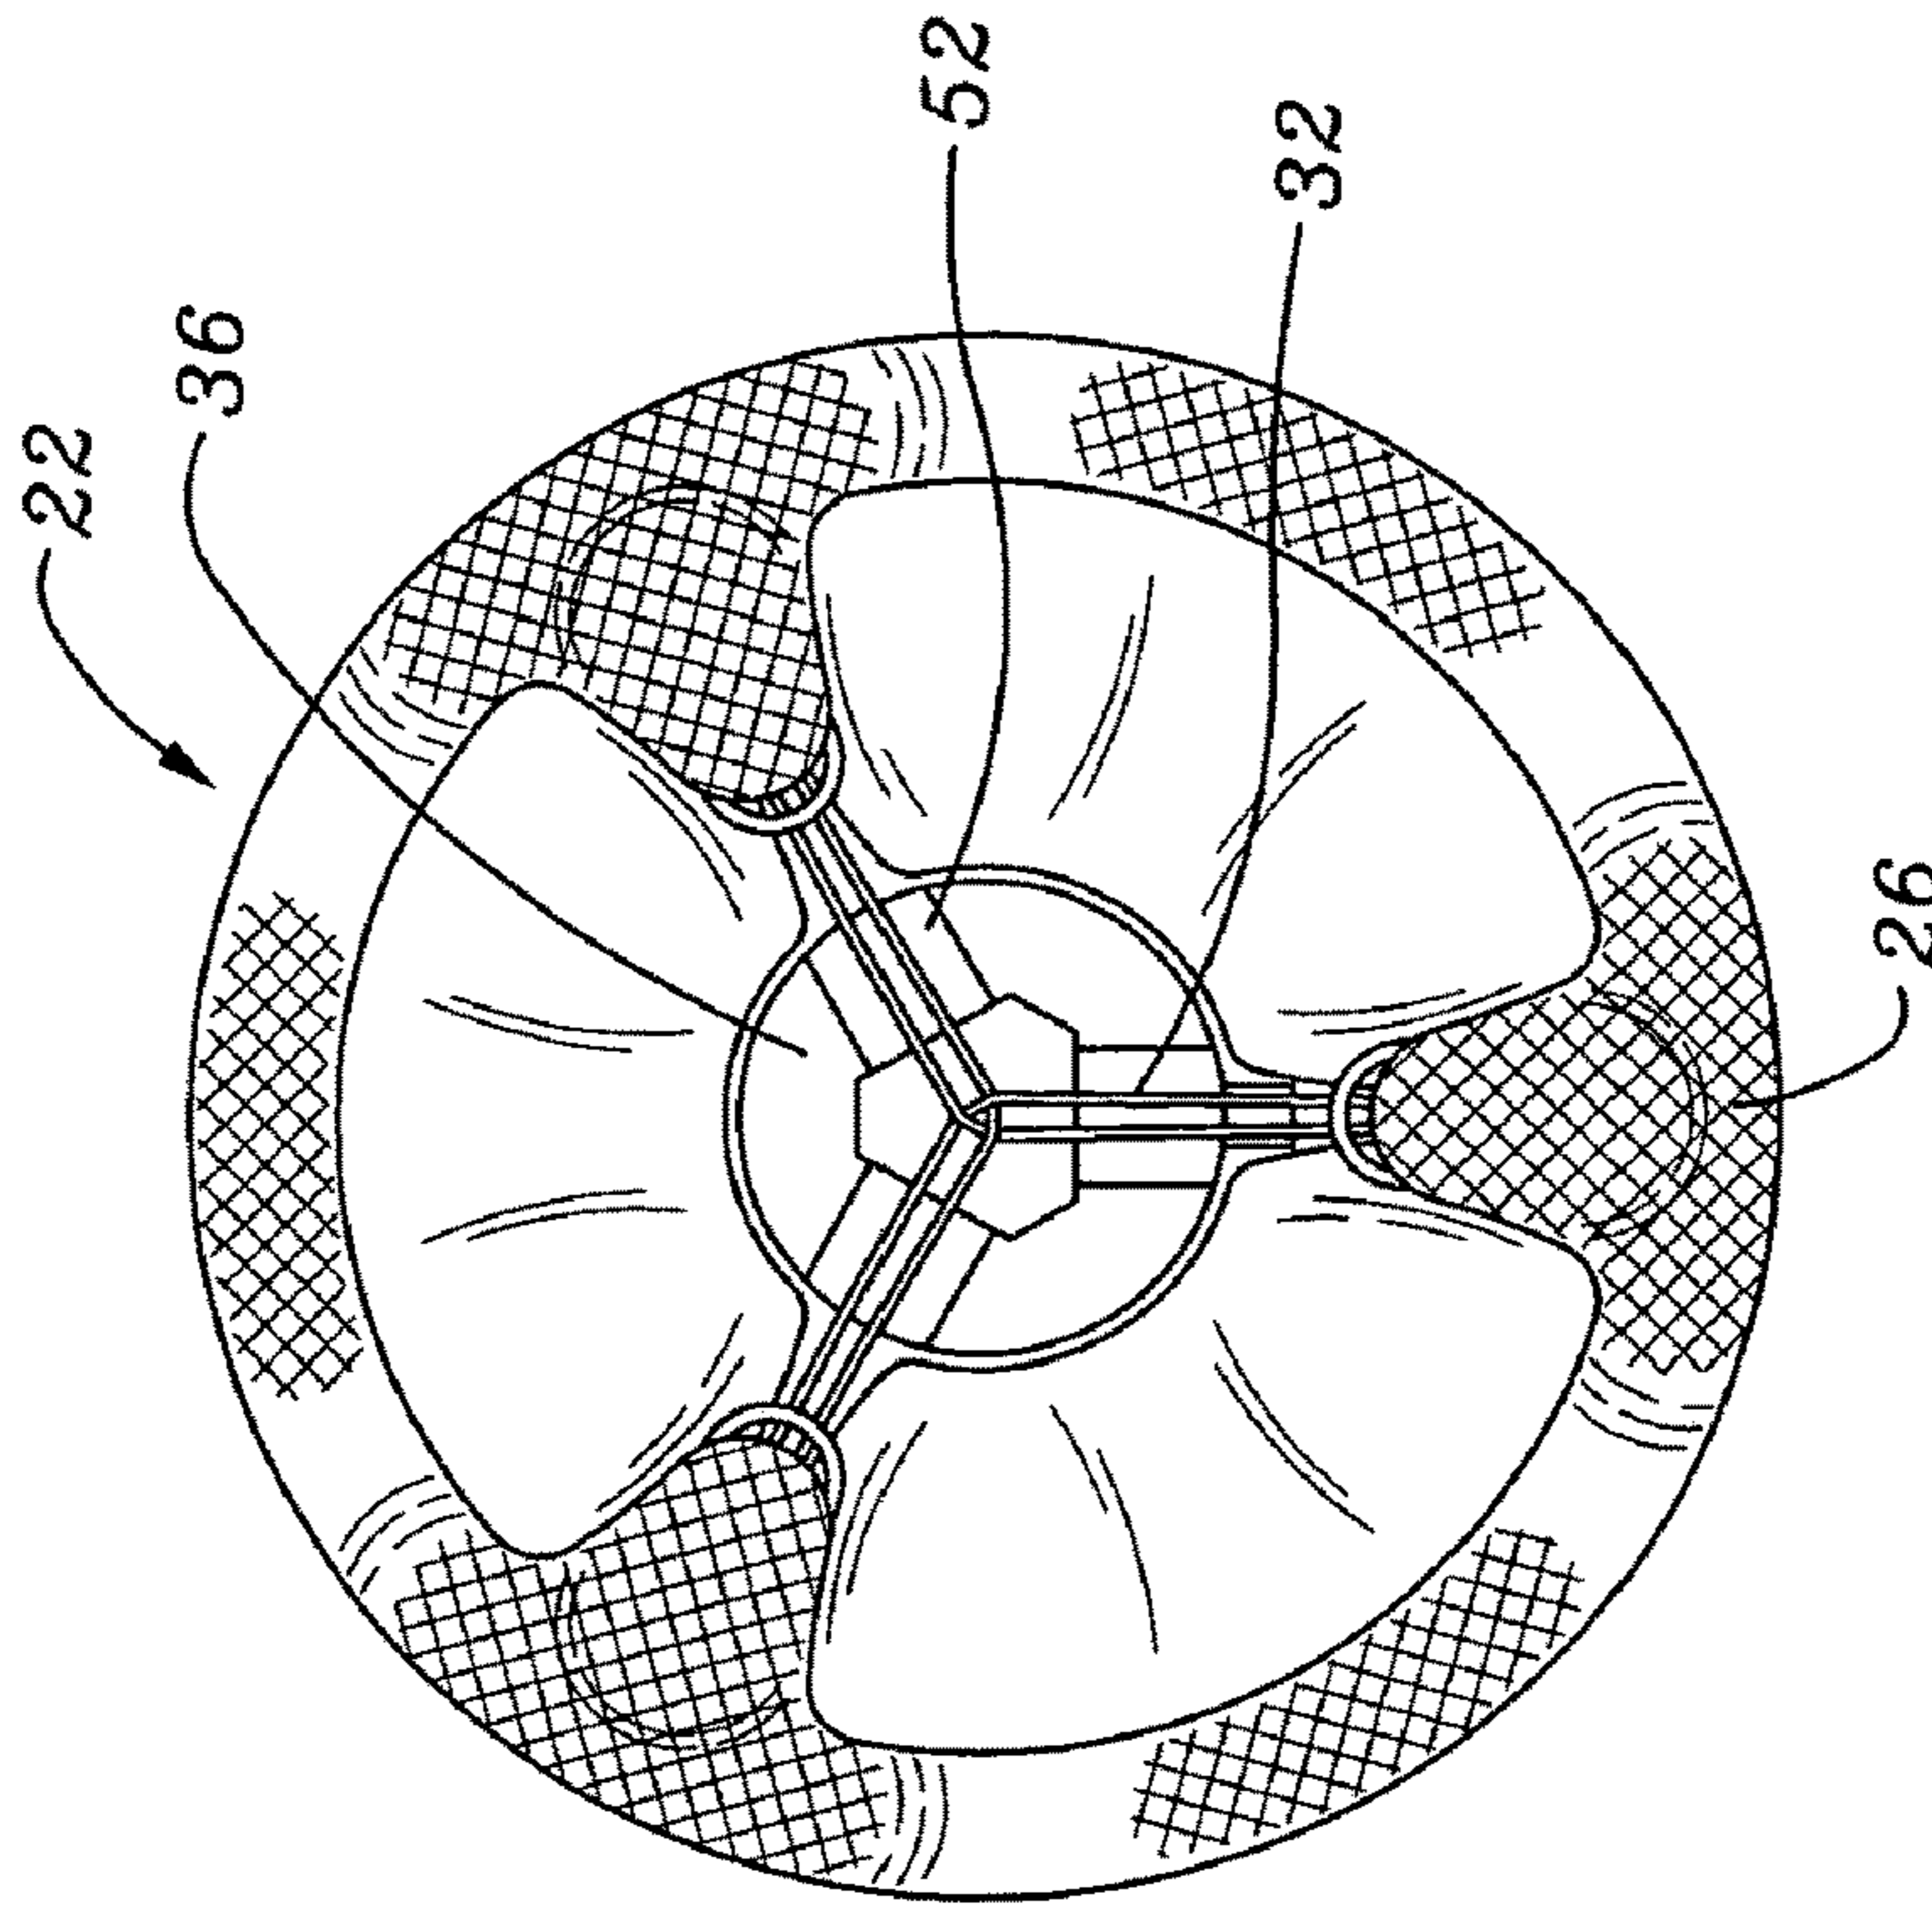
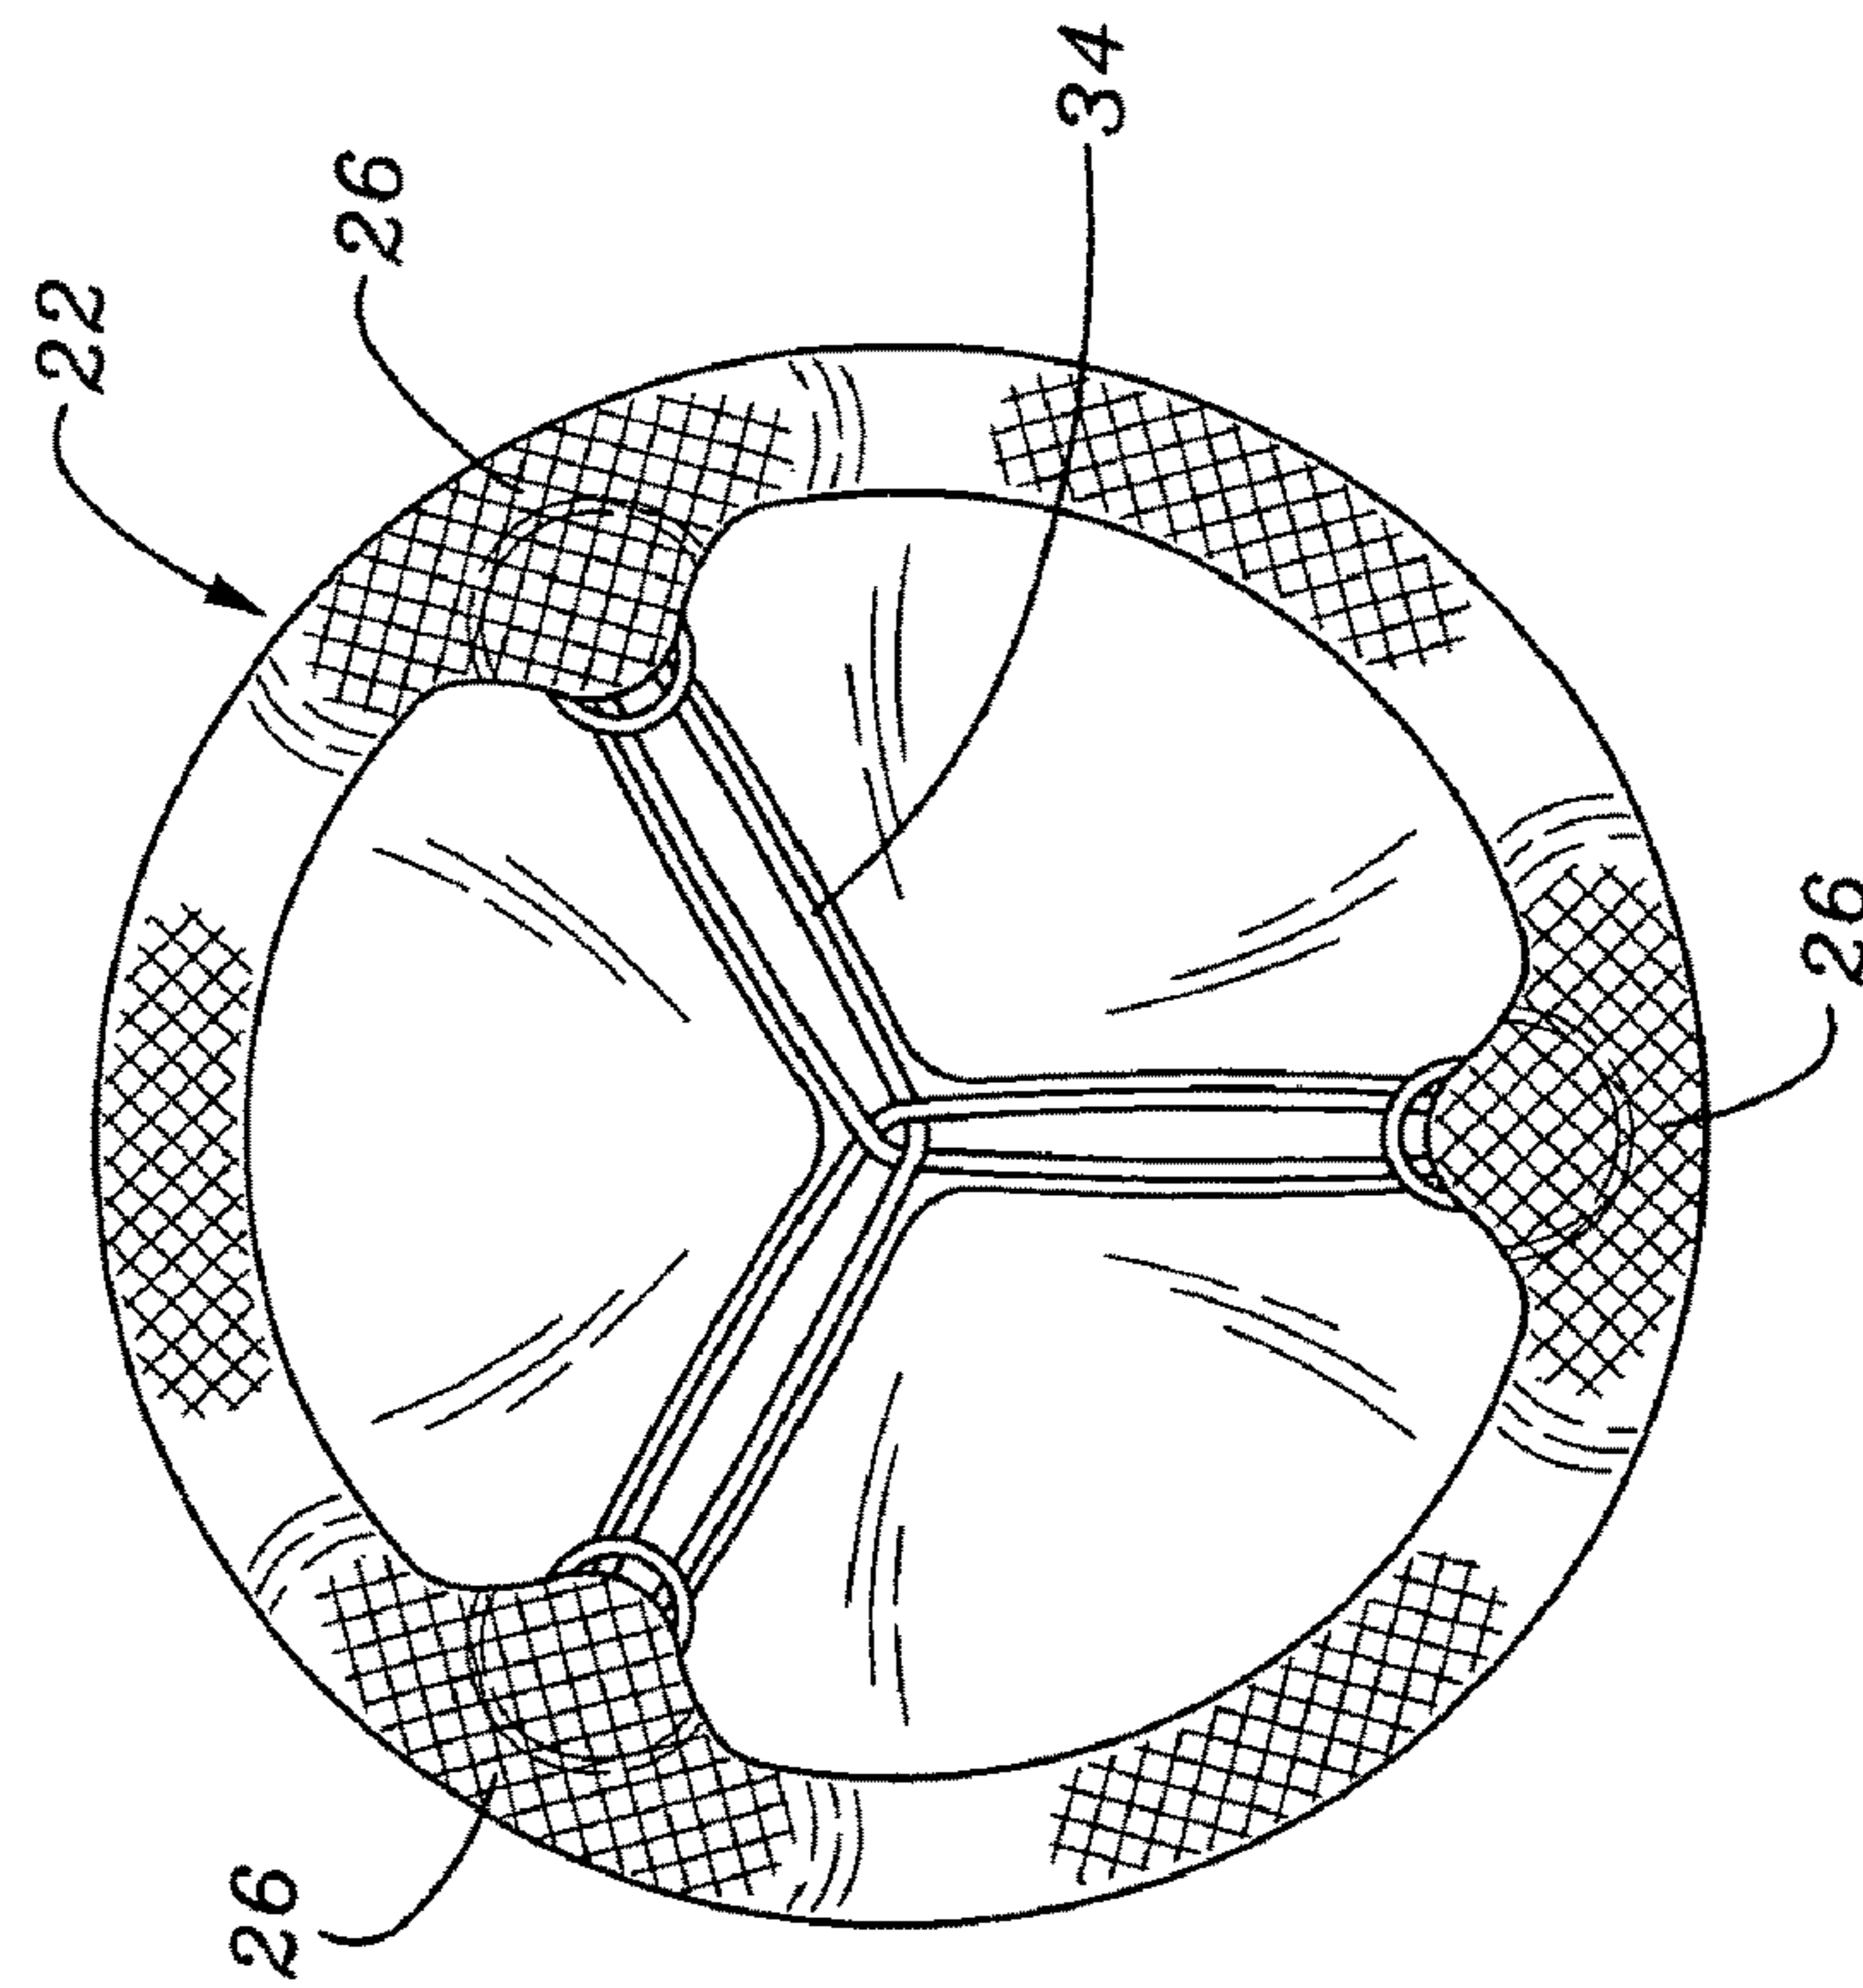
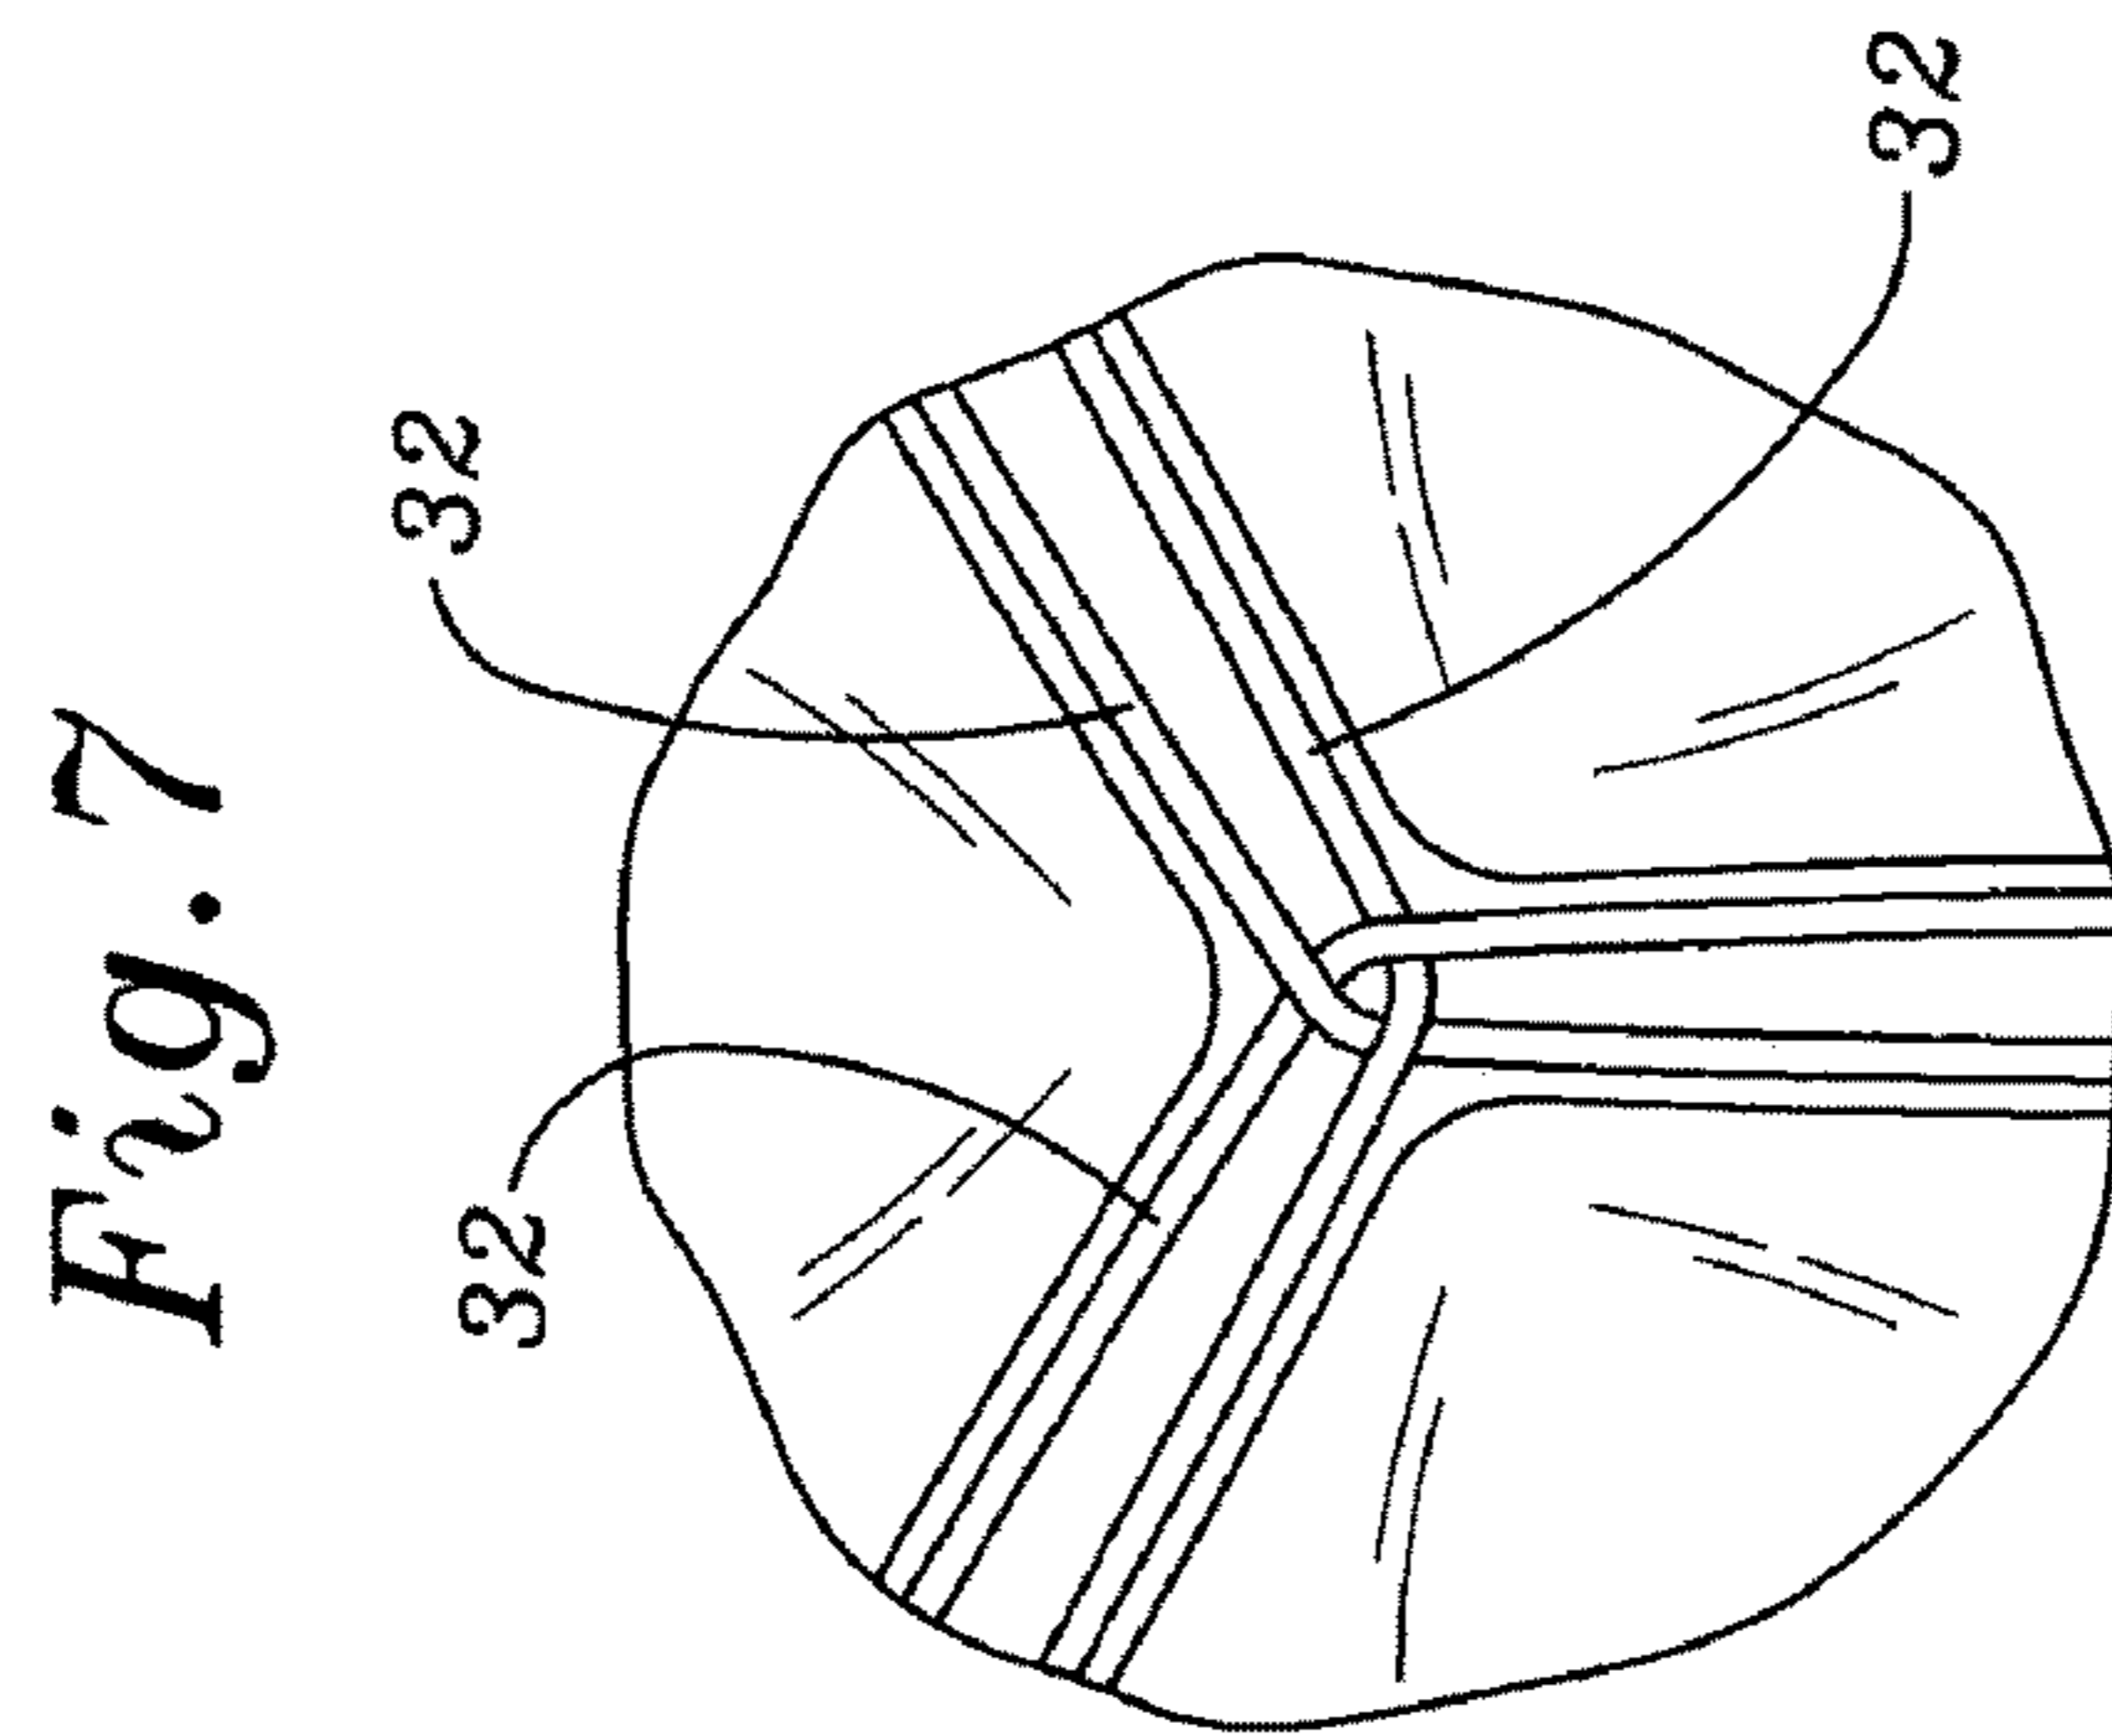
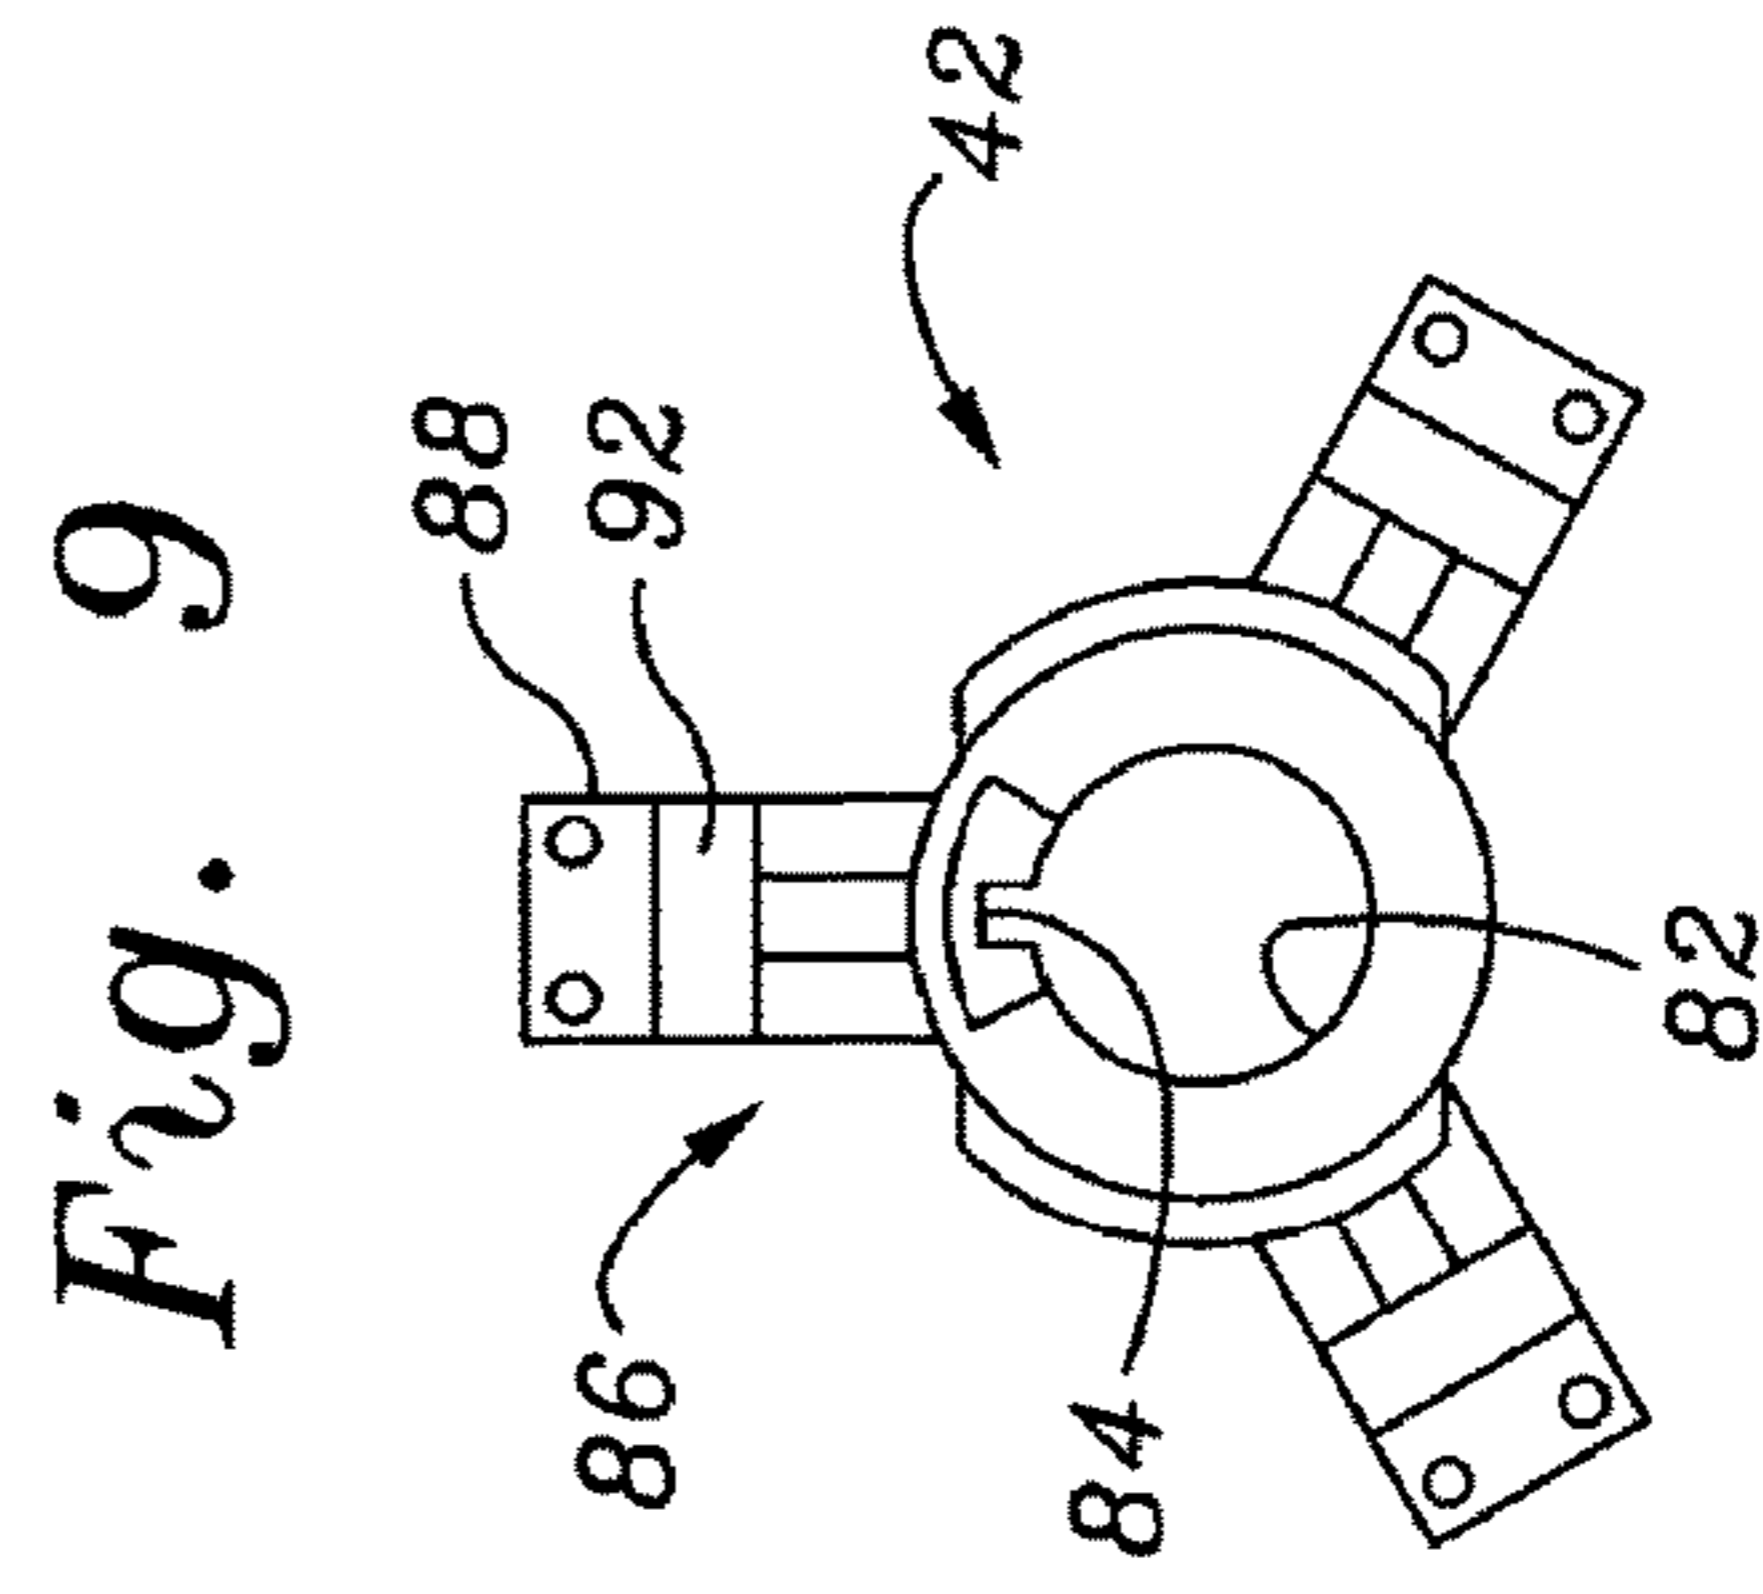
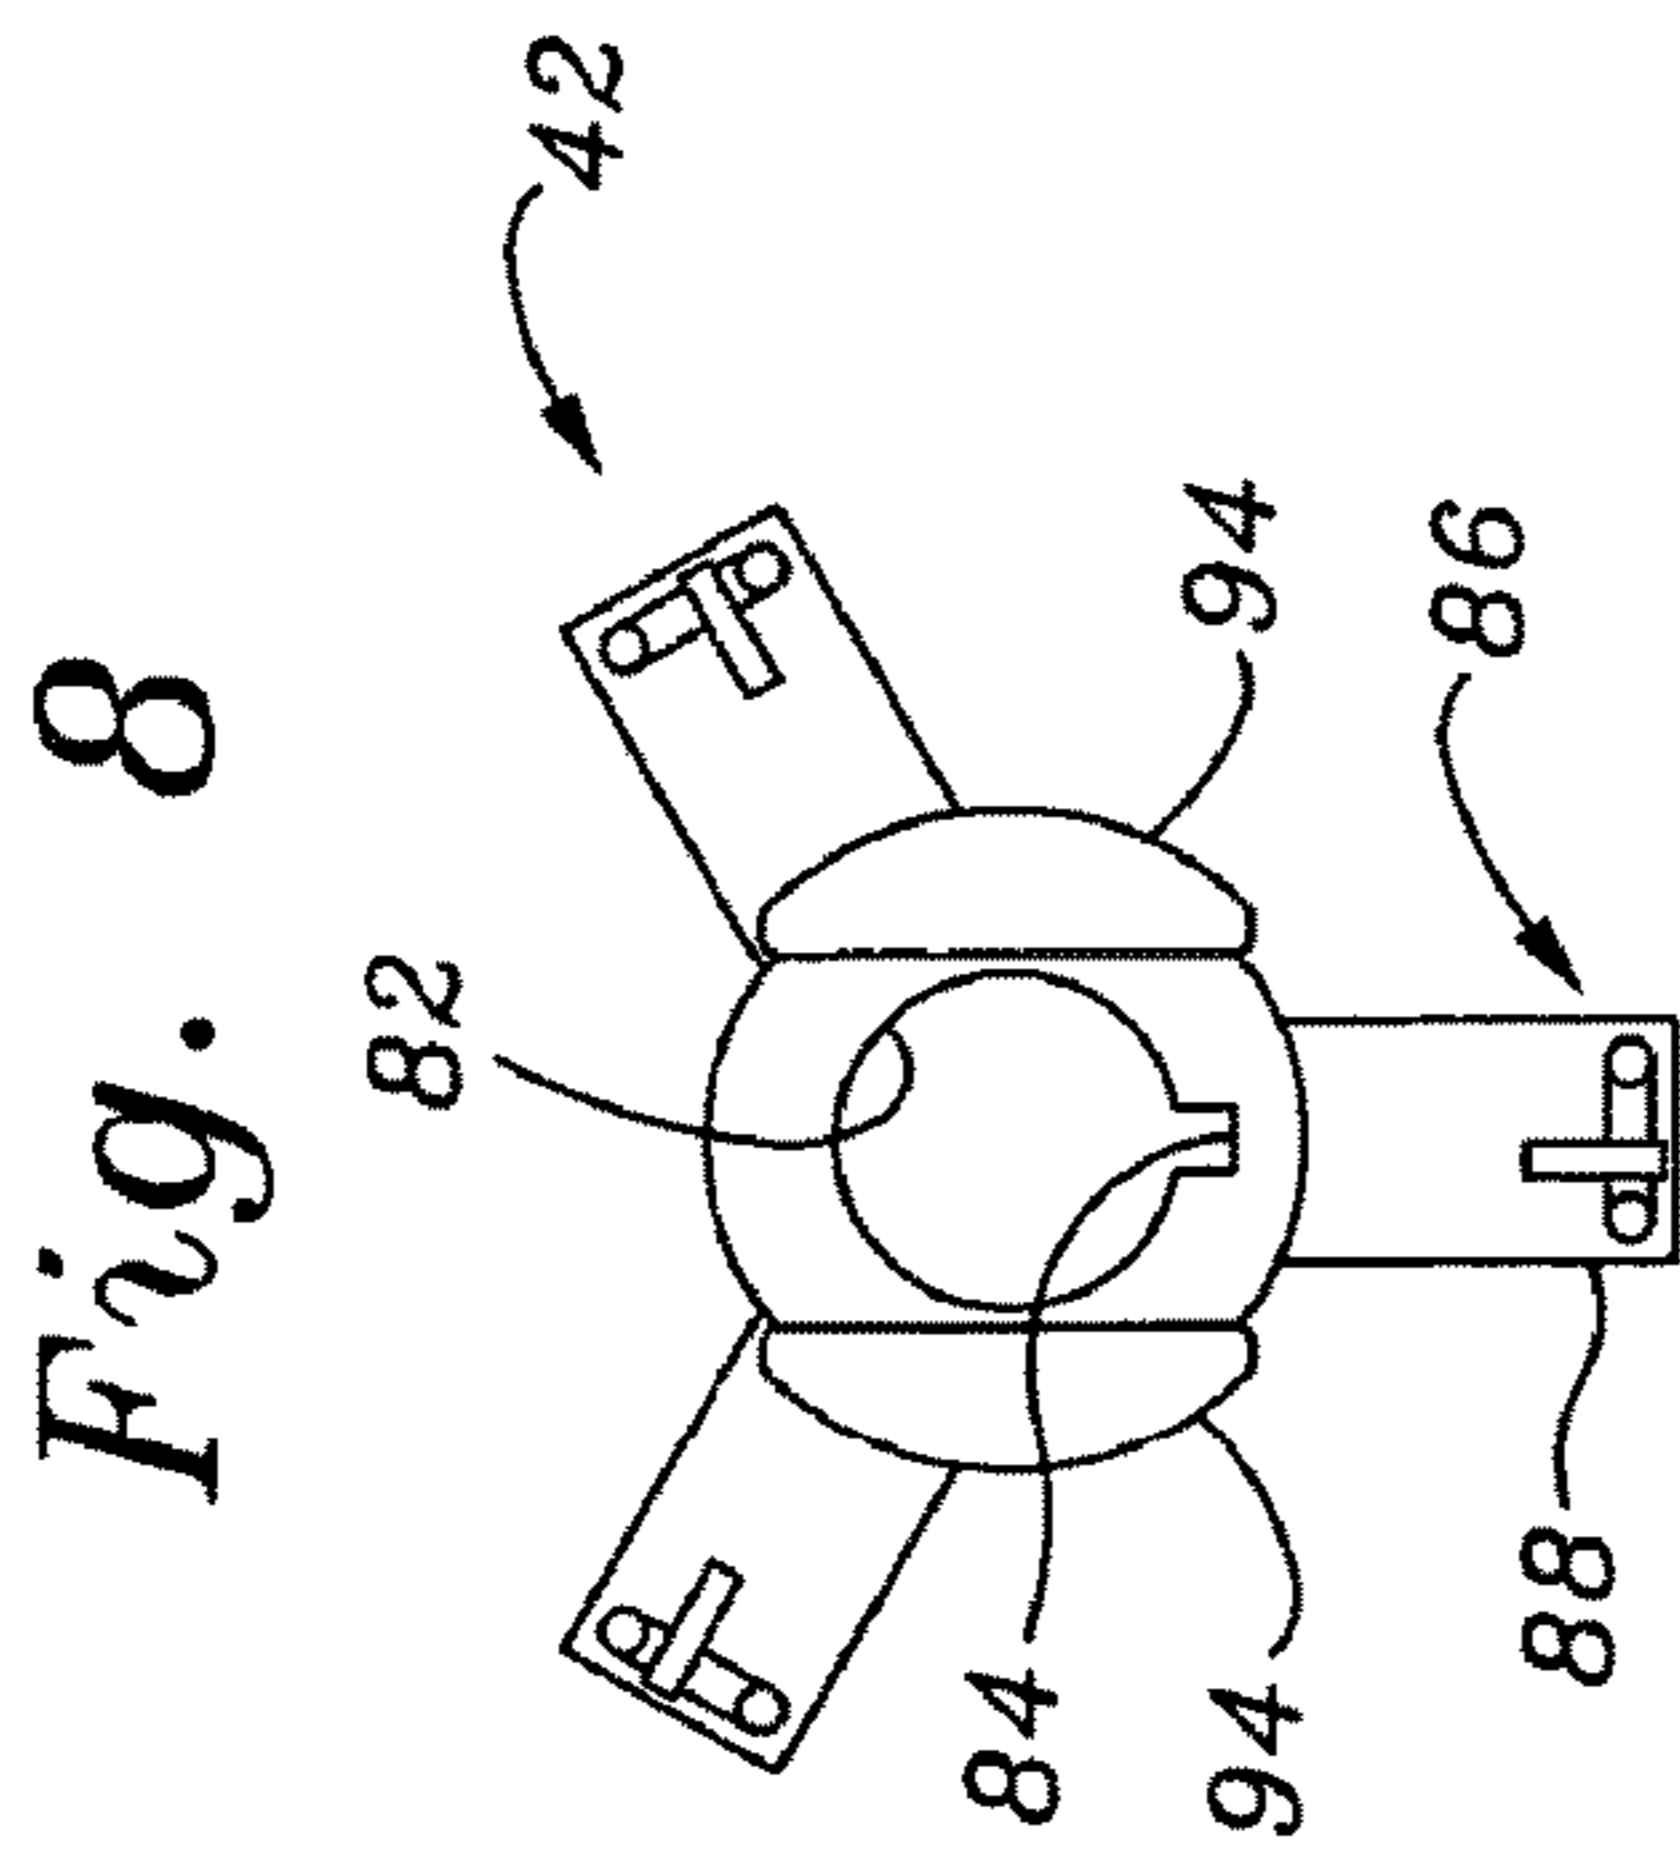


Fig. 6A






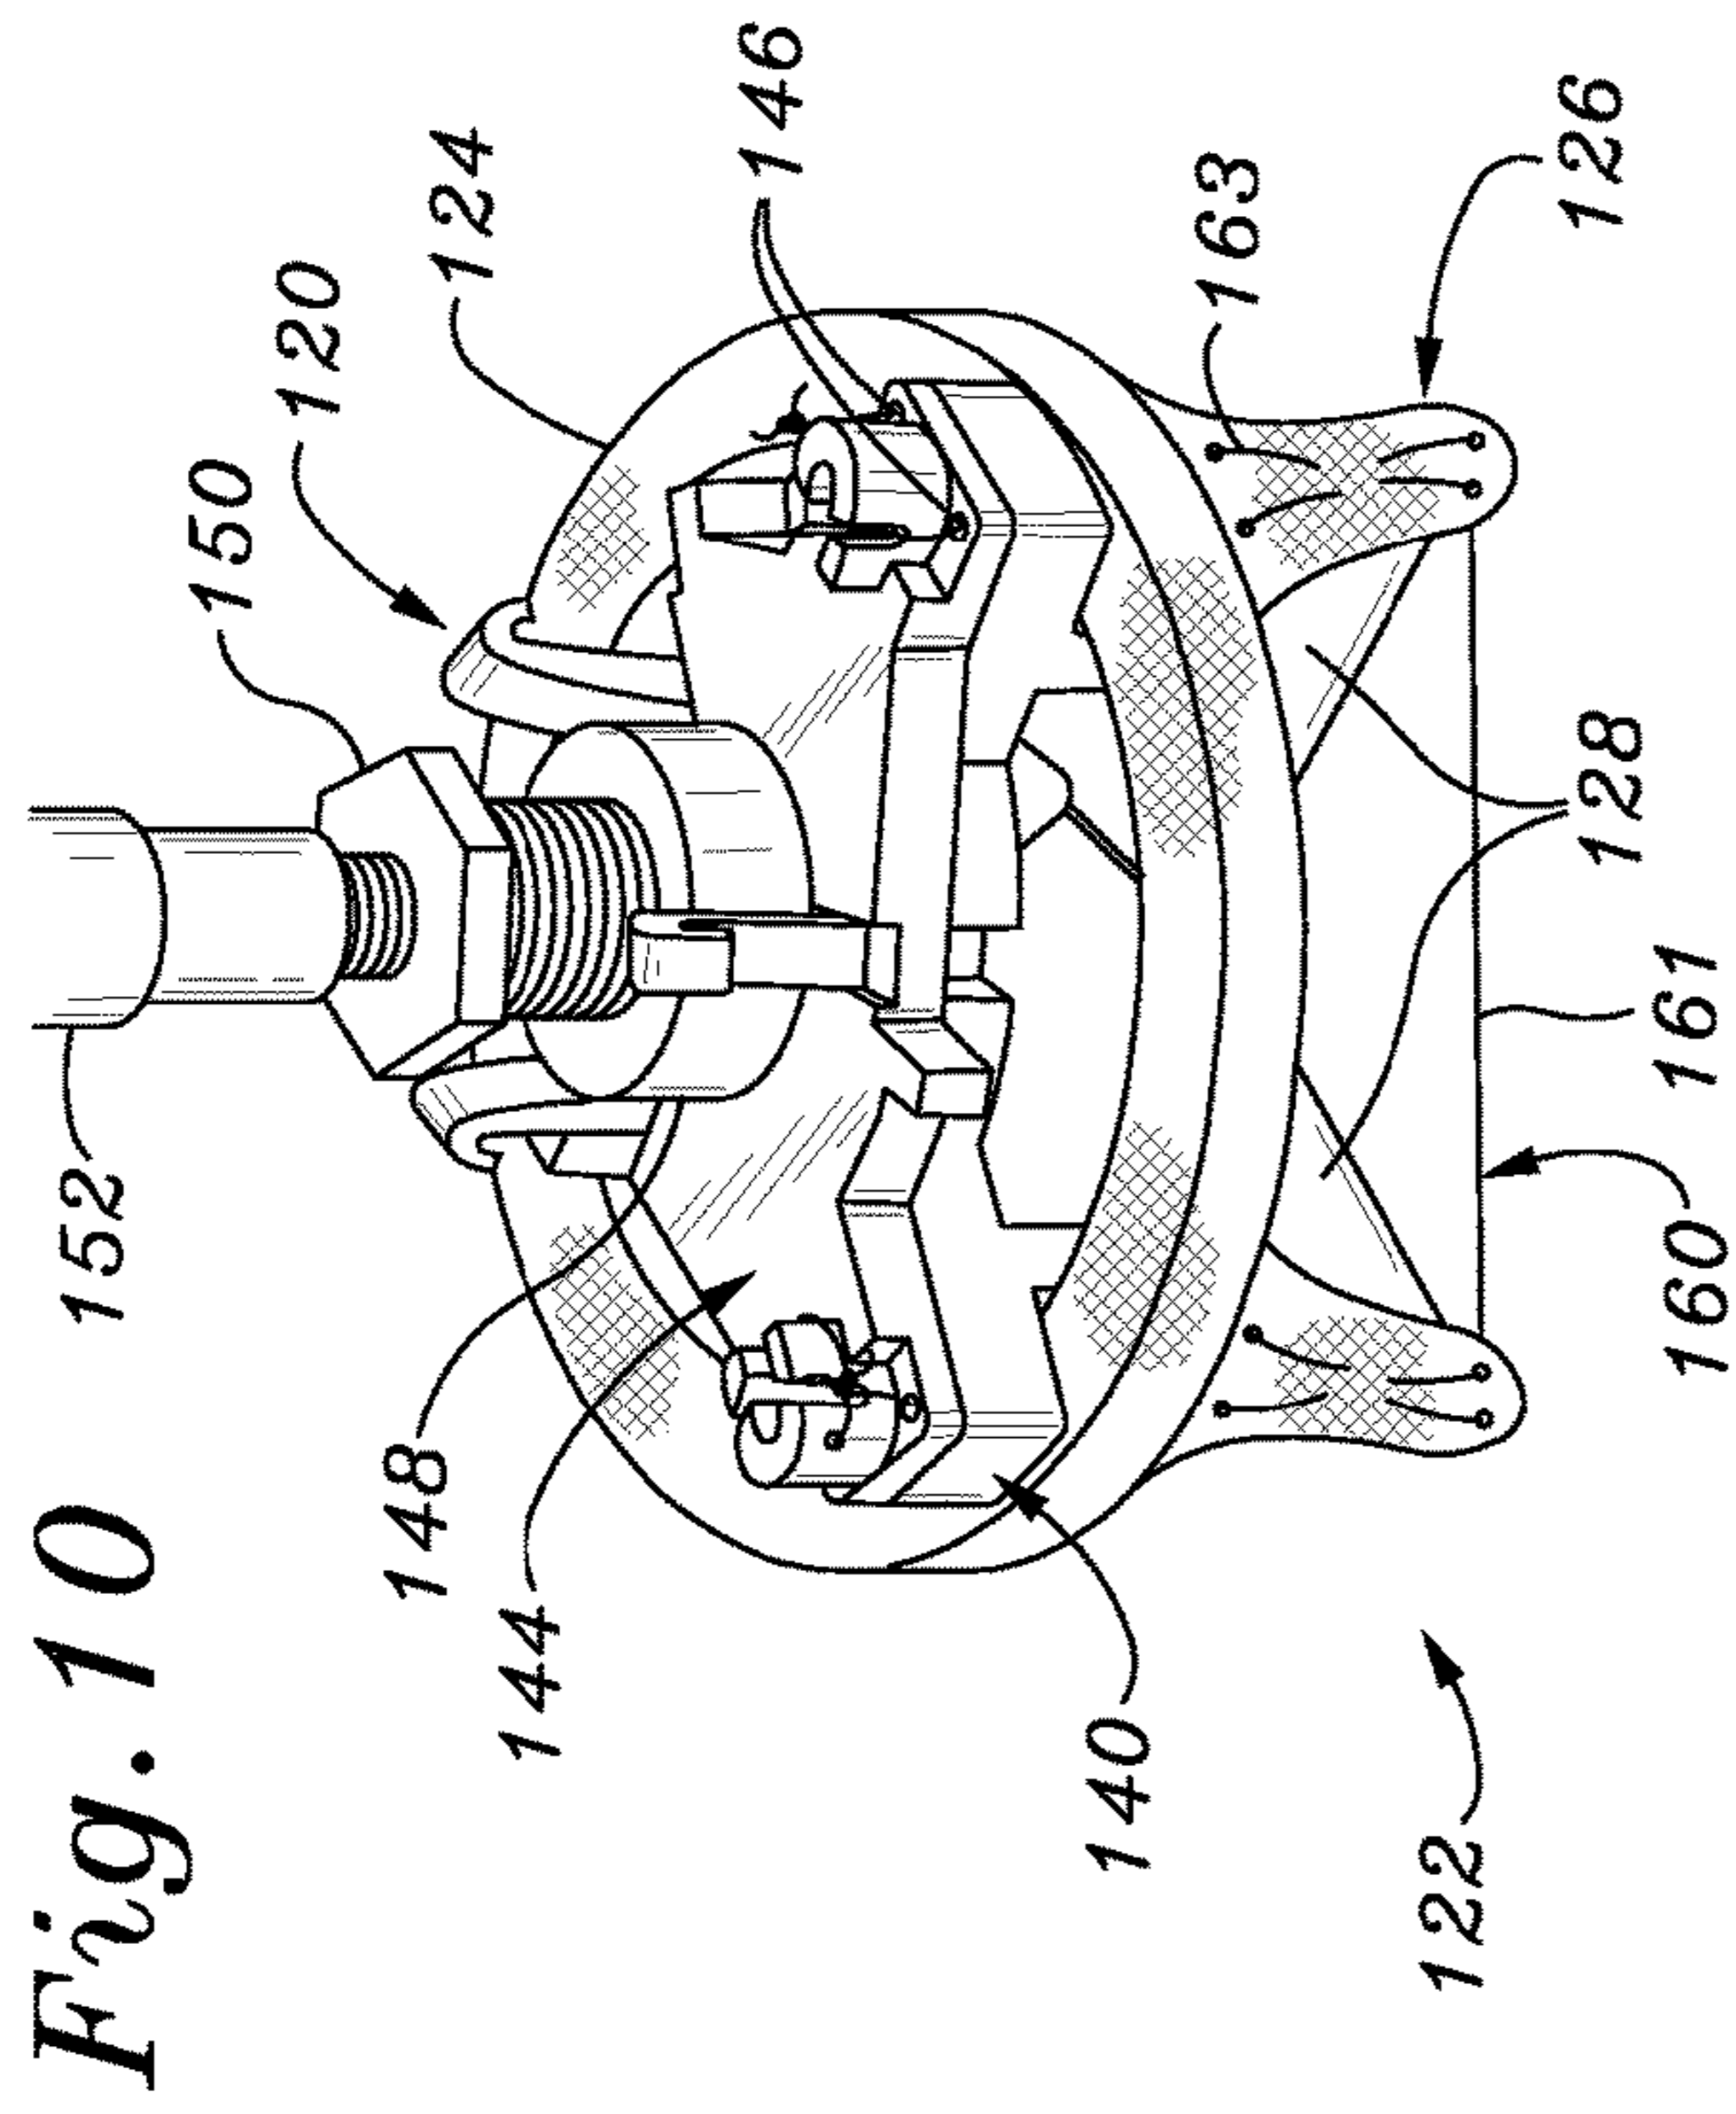


Fig. 10

Fig. 11



Amended

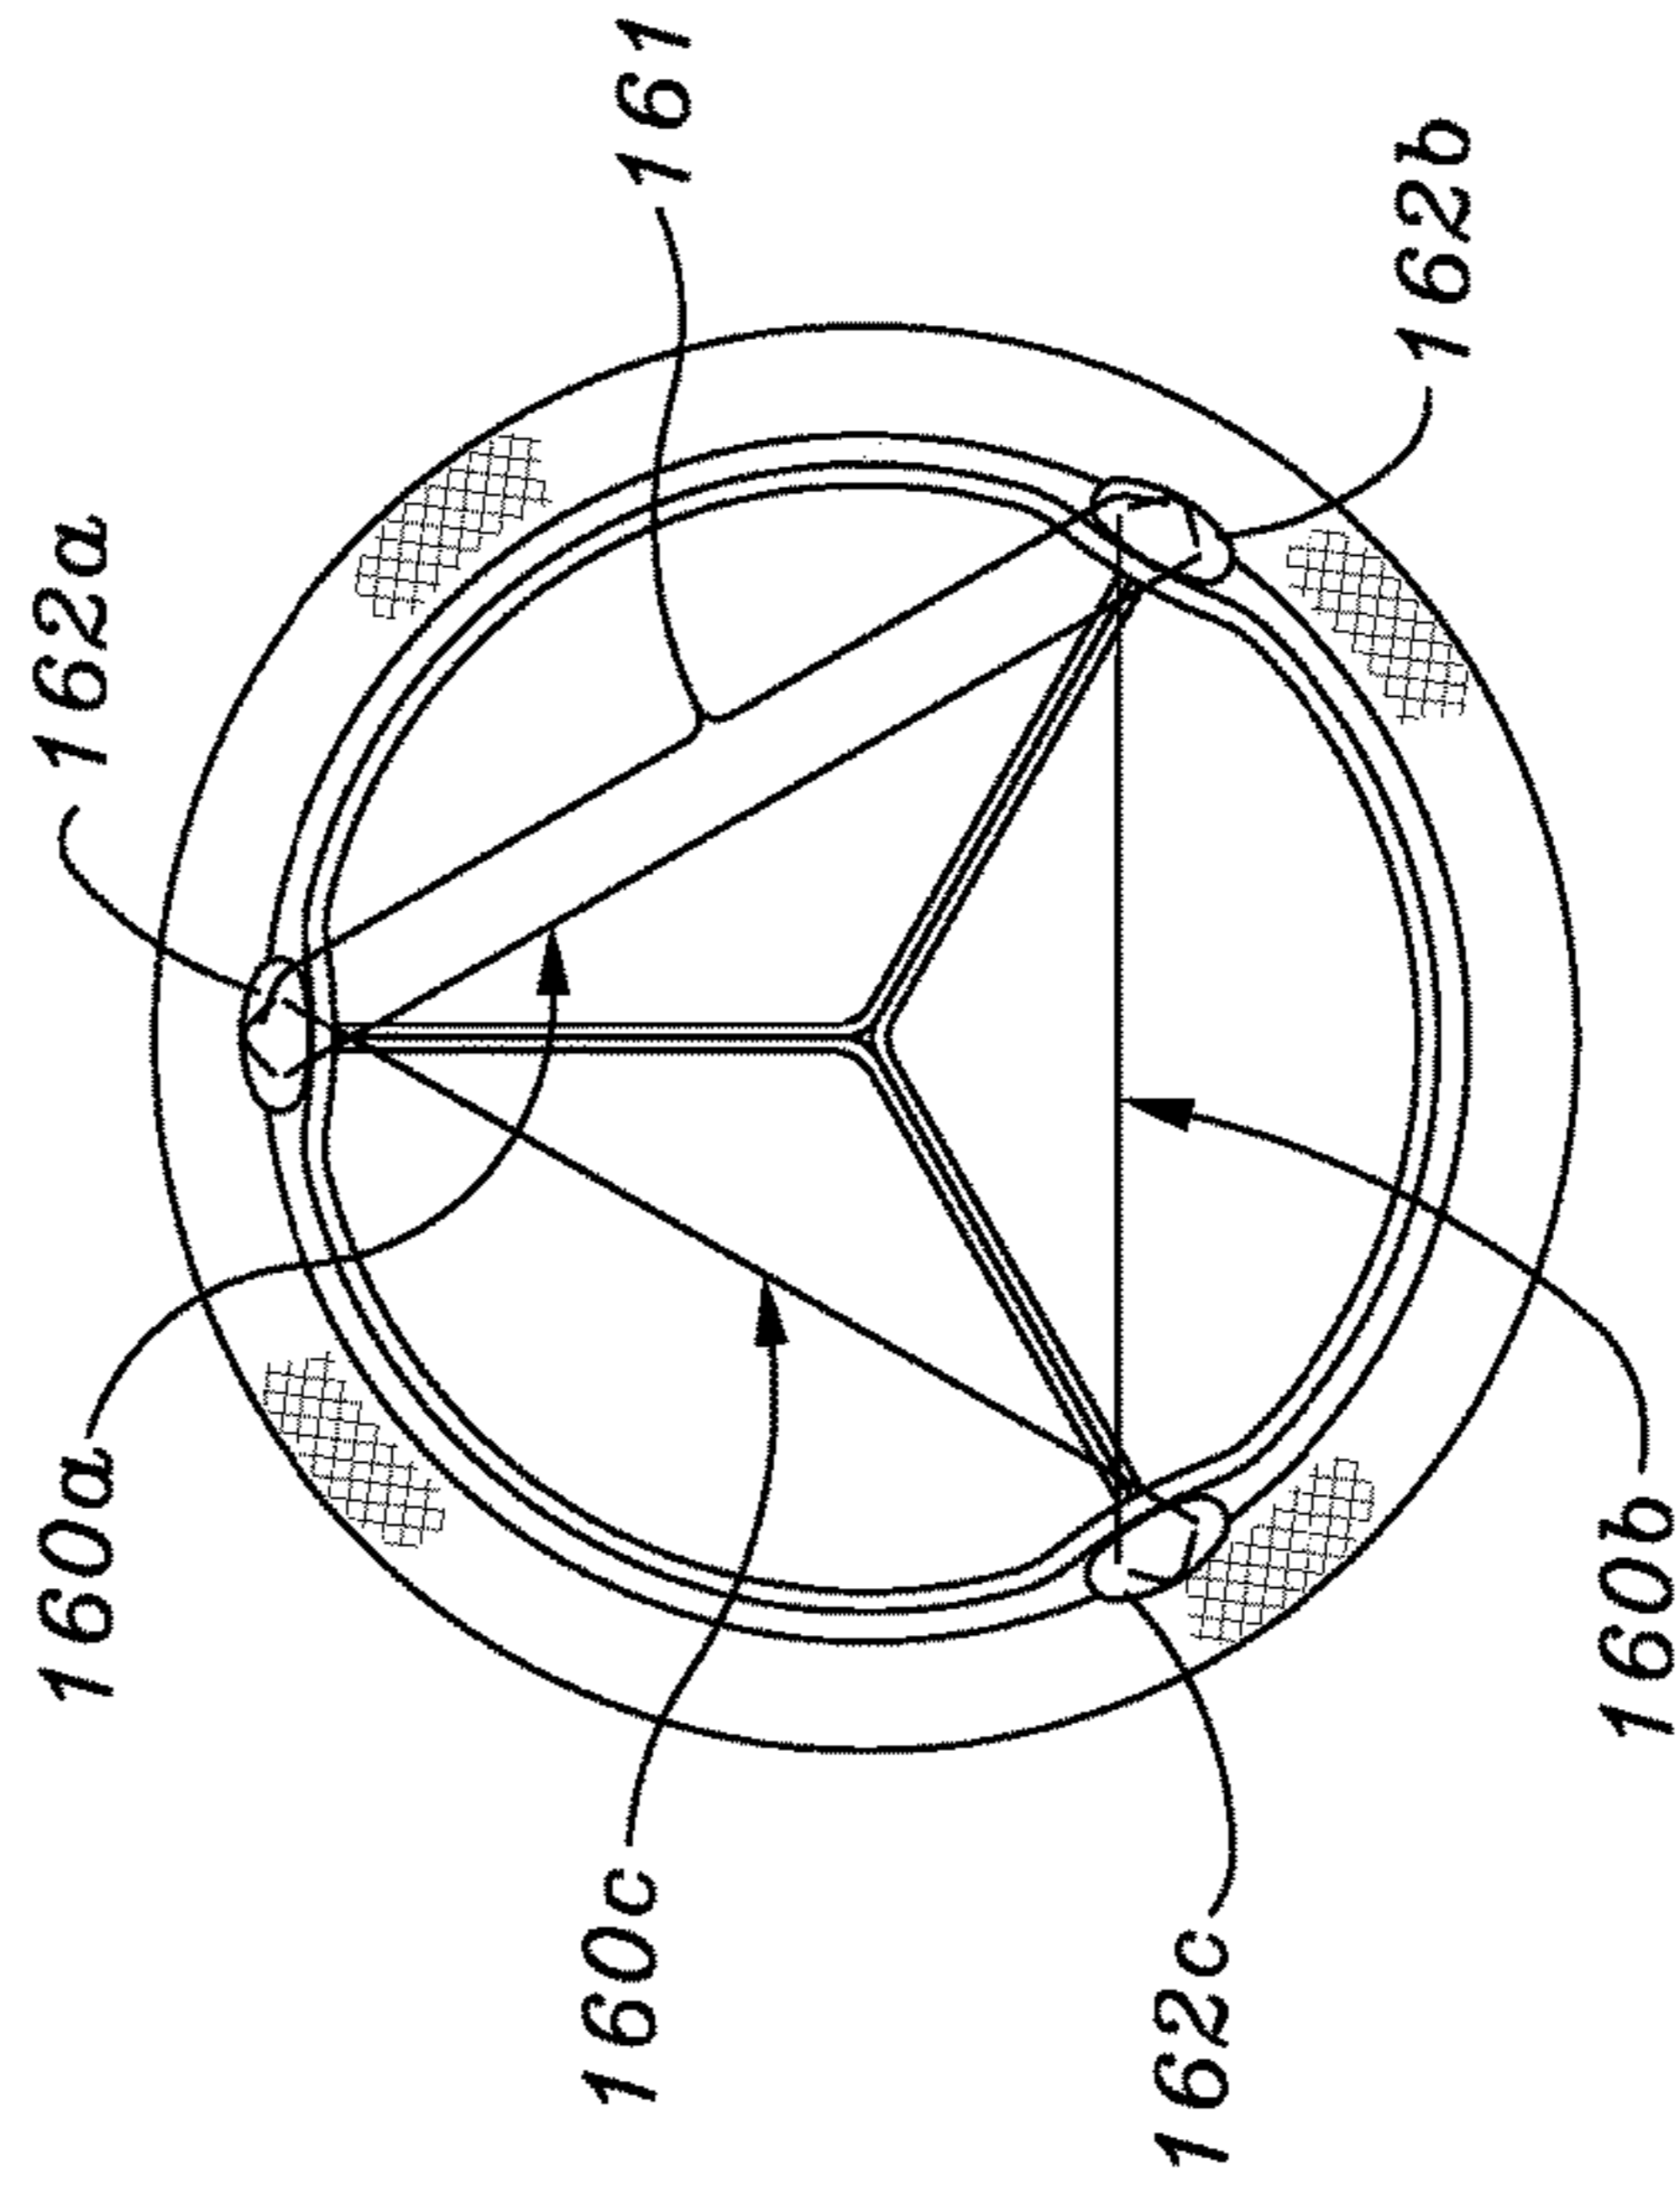

Amended

Fig. 13

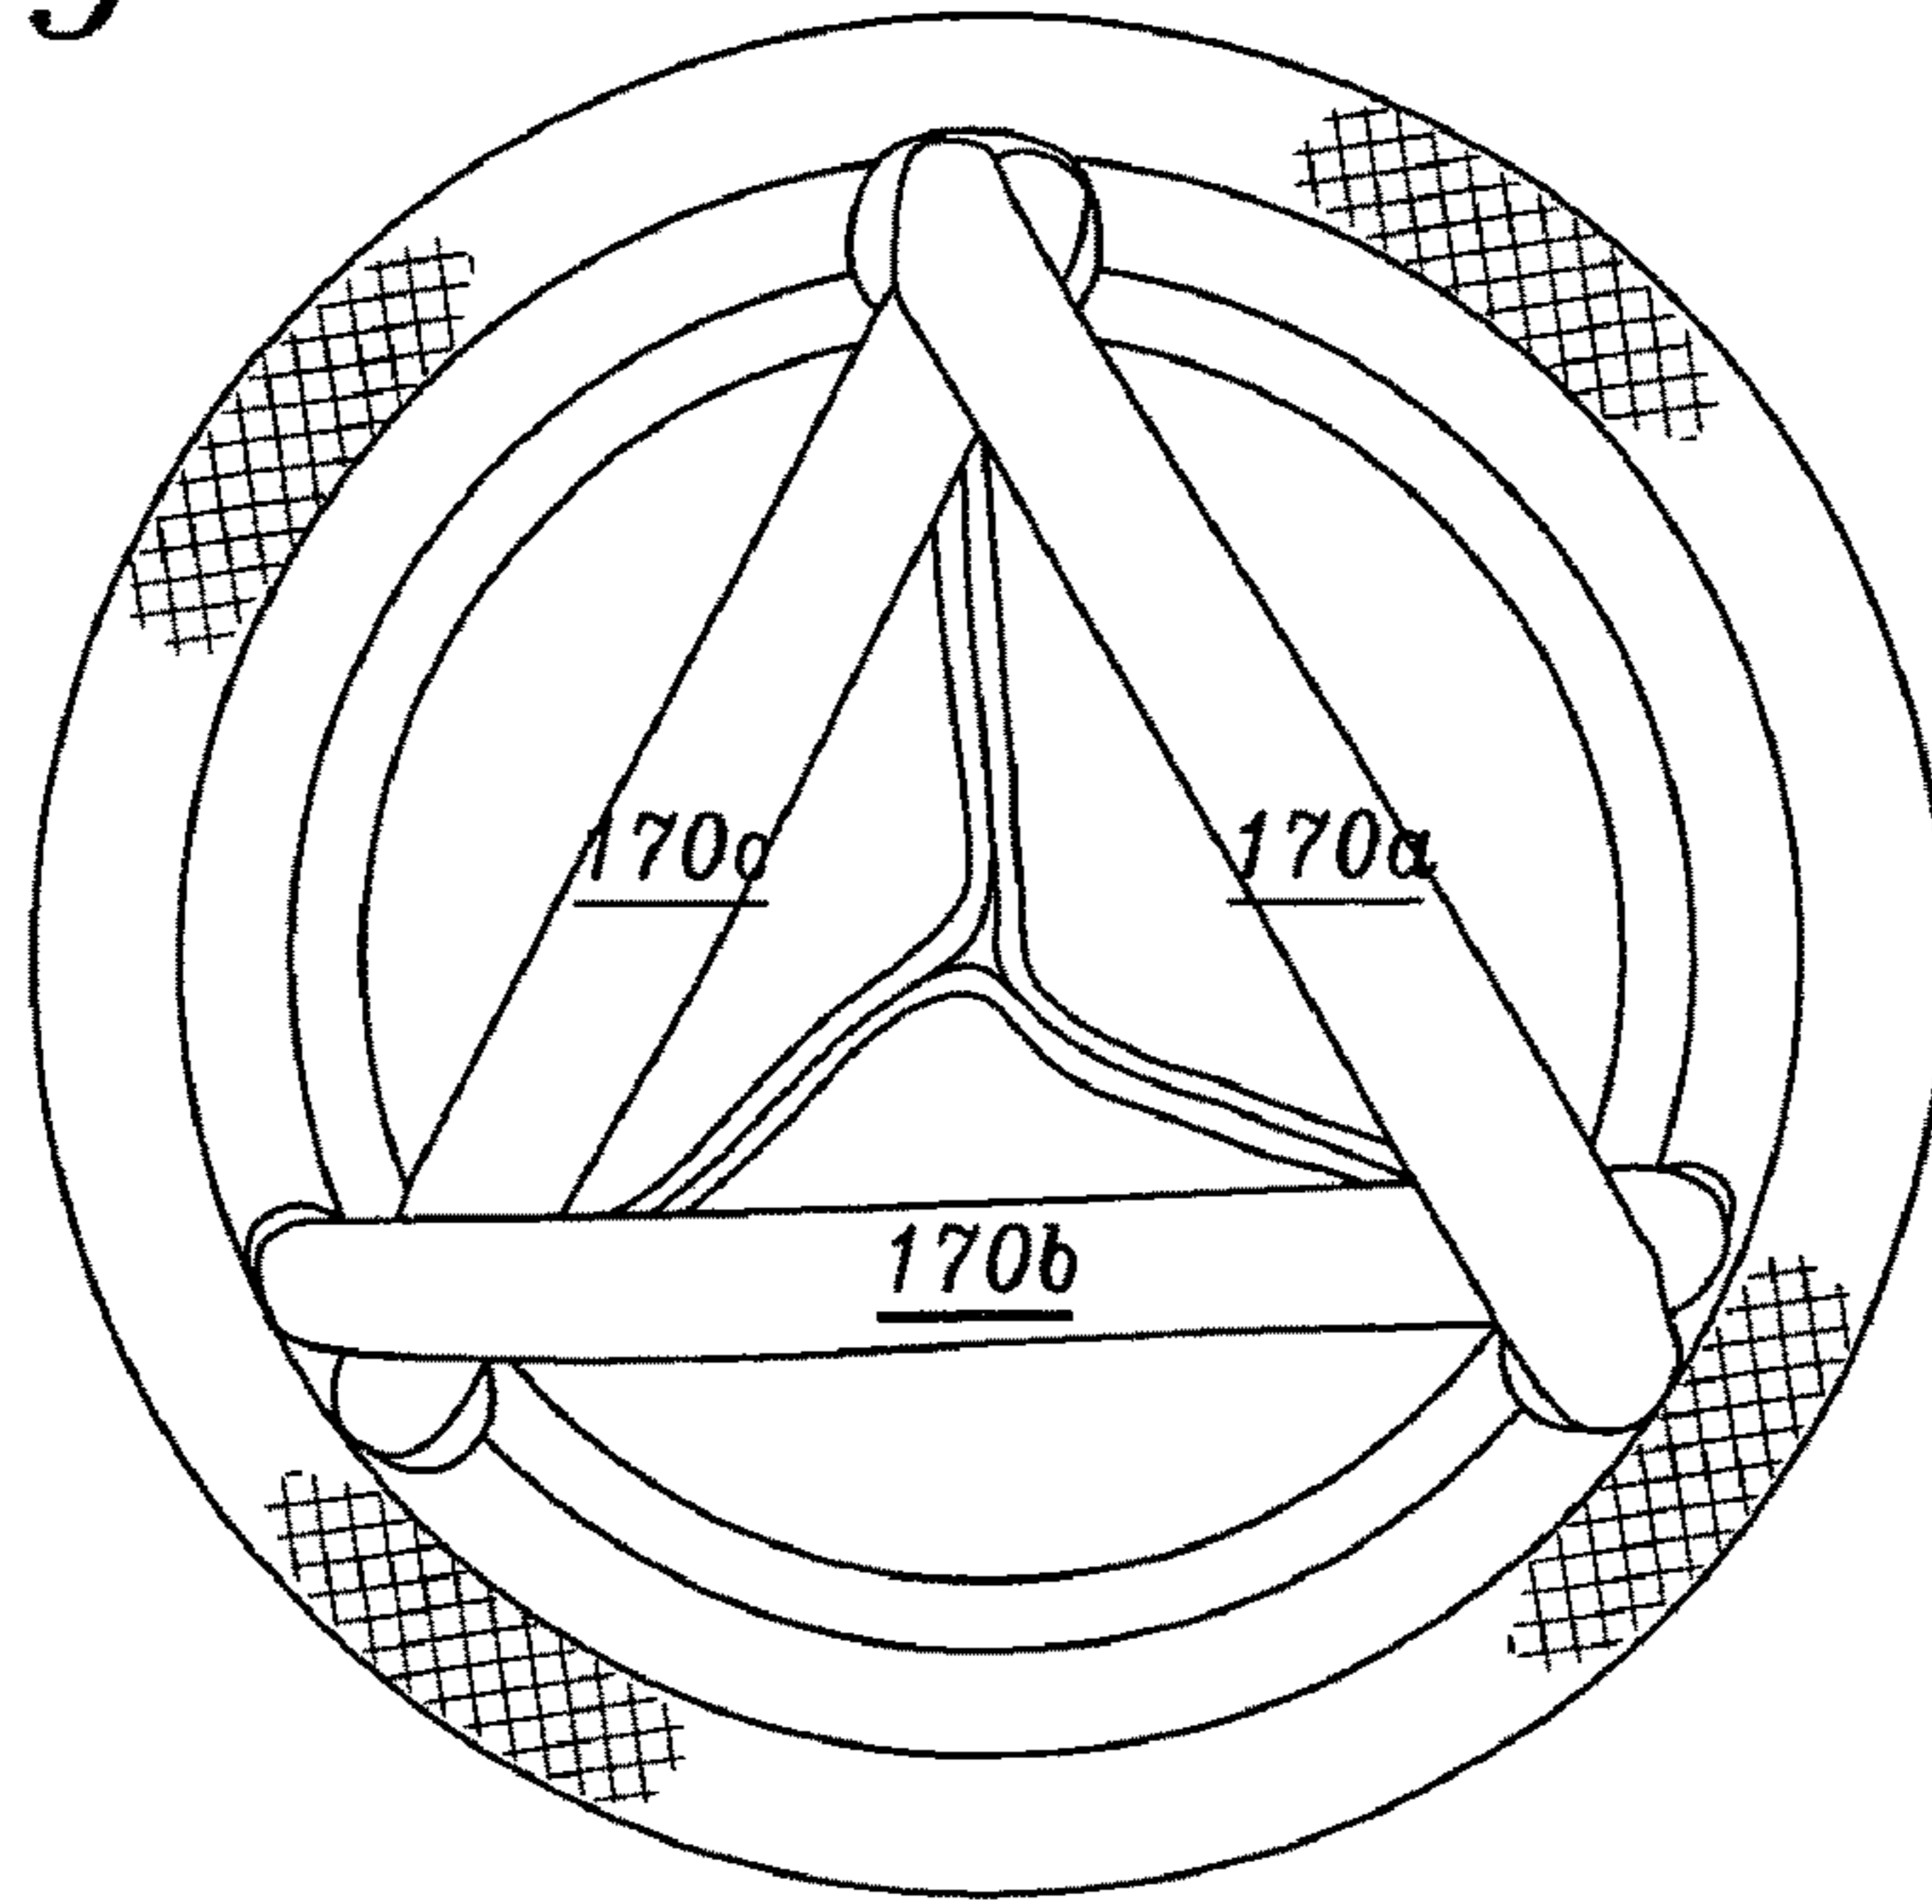


Fig. 14

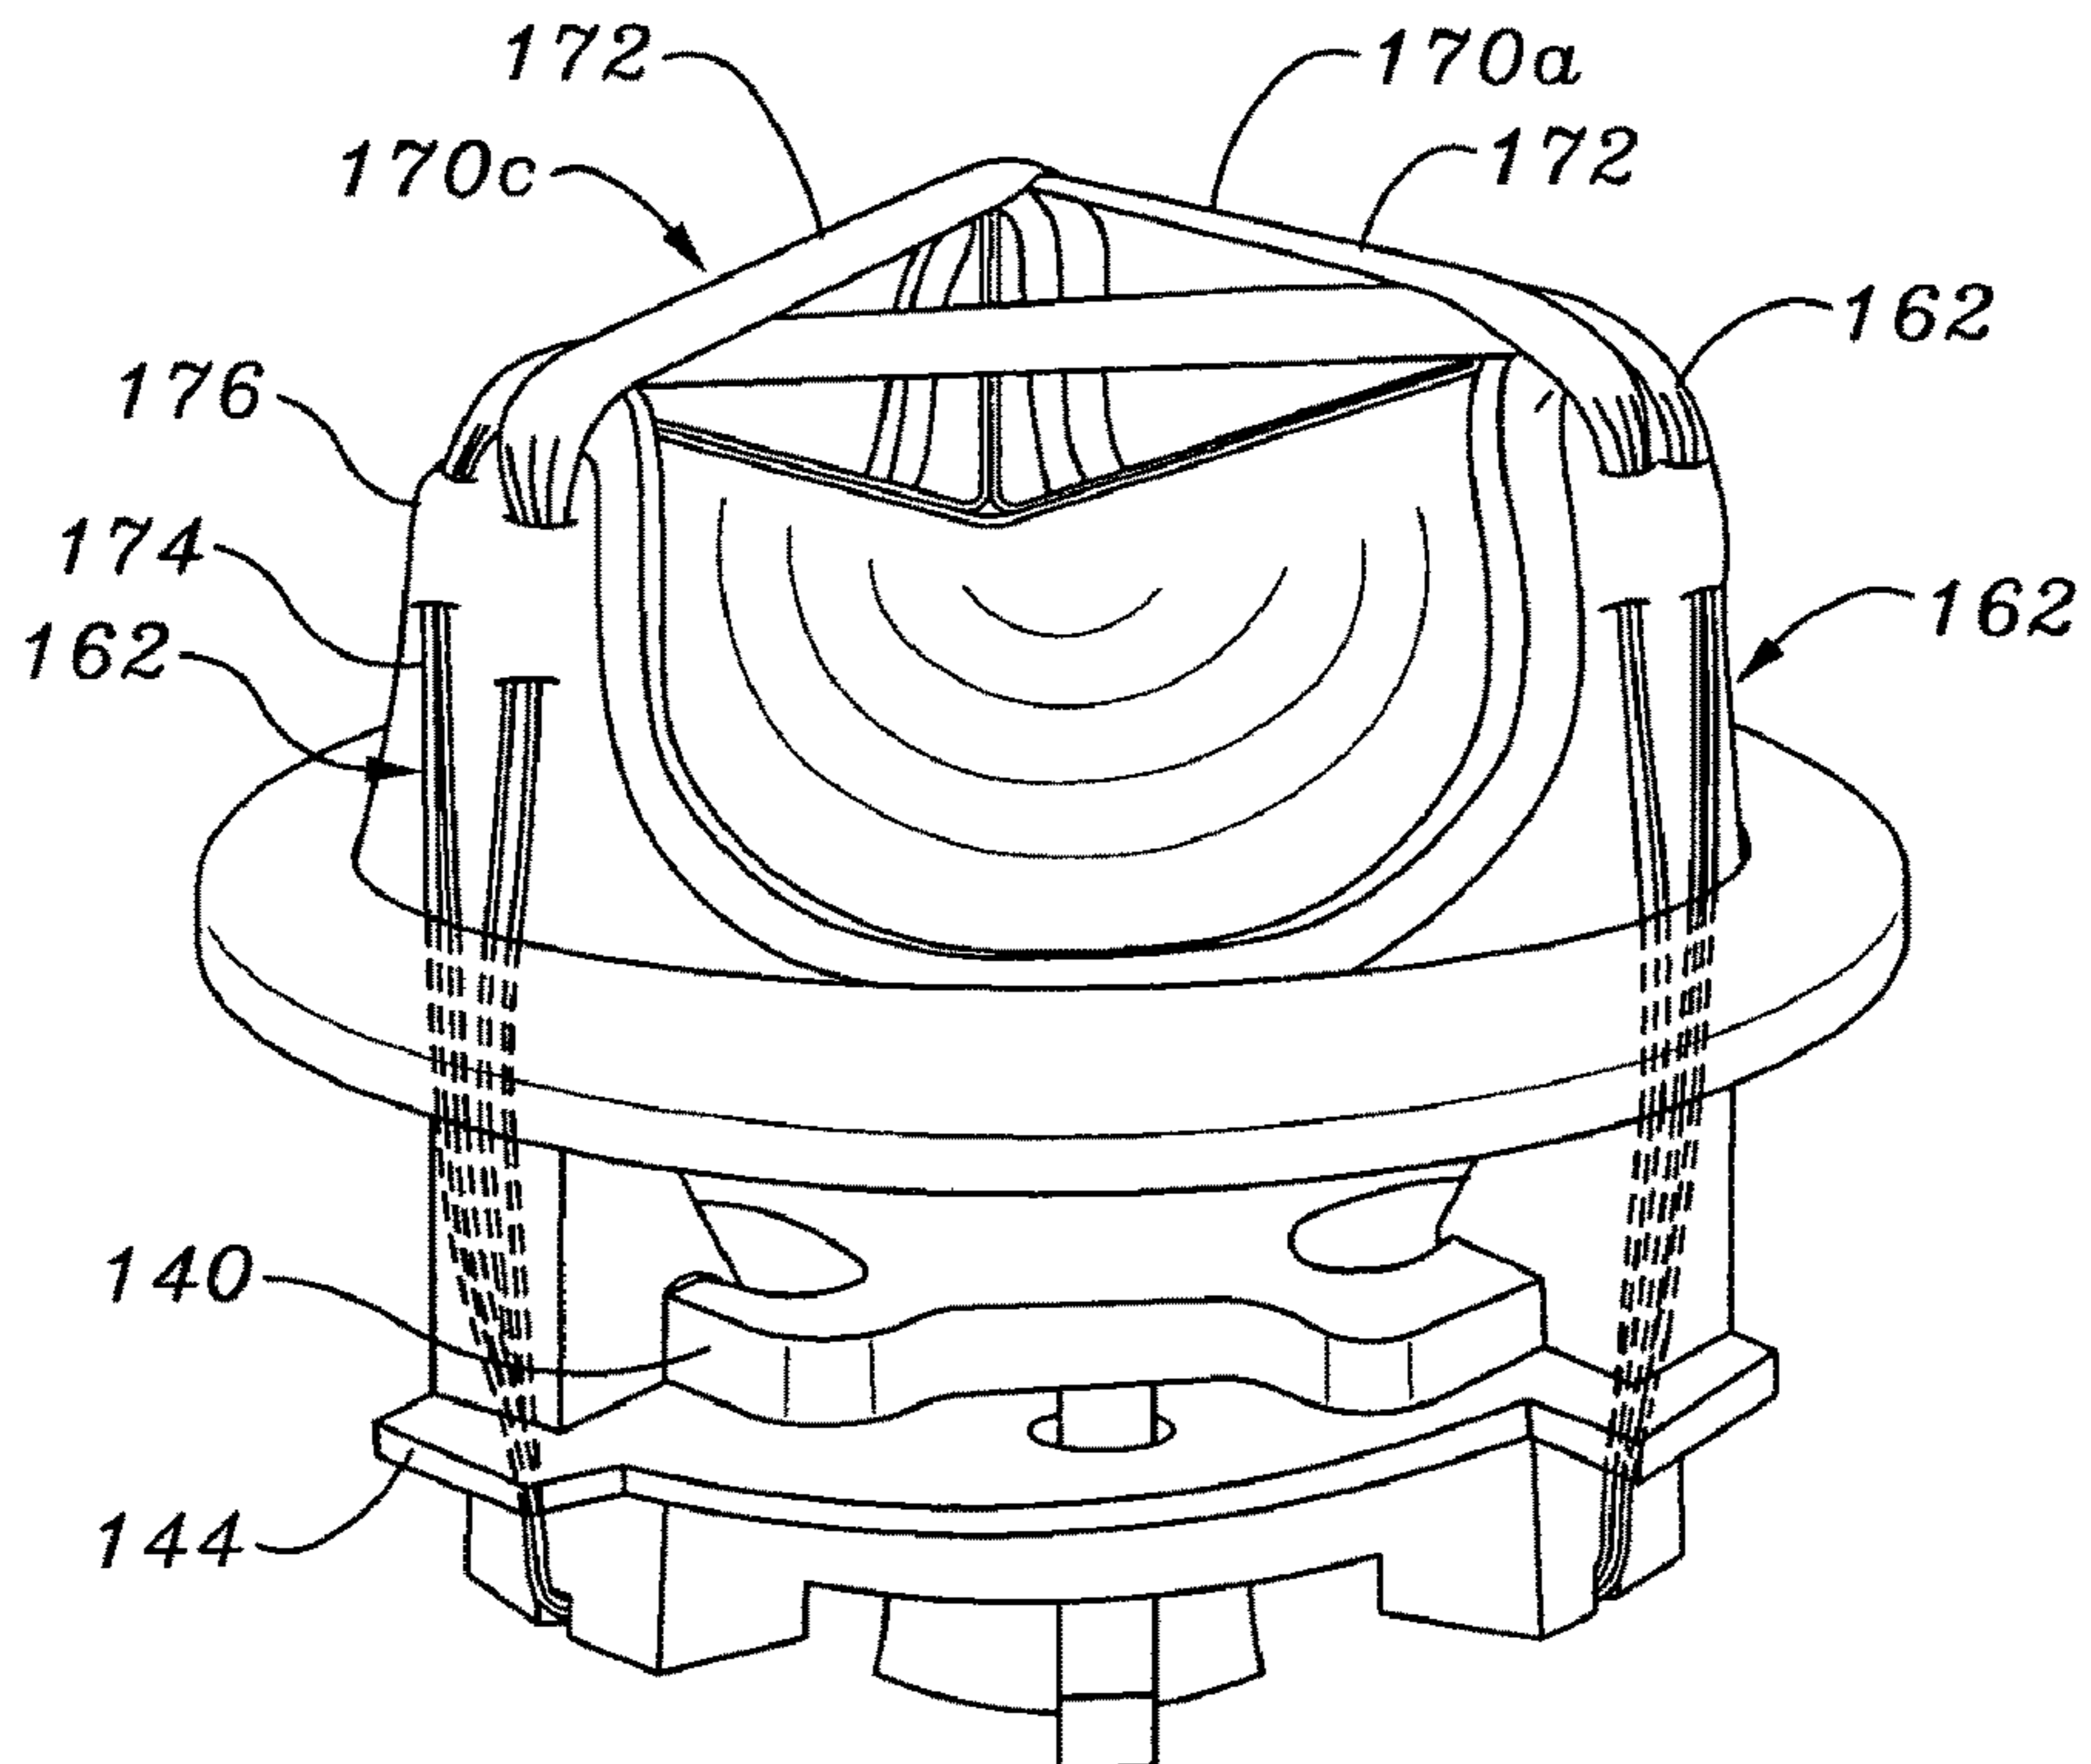


Fig. 15

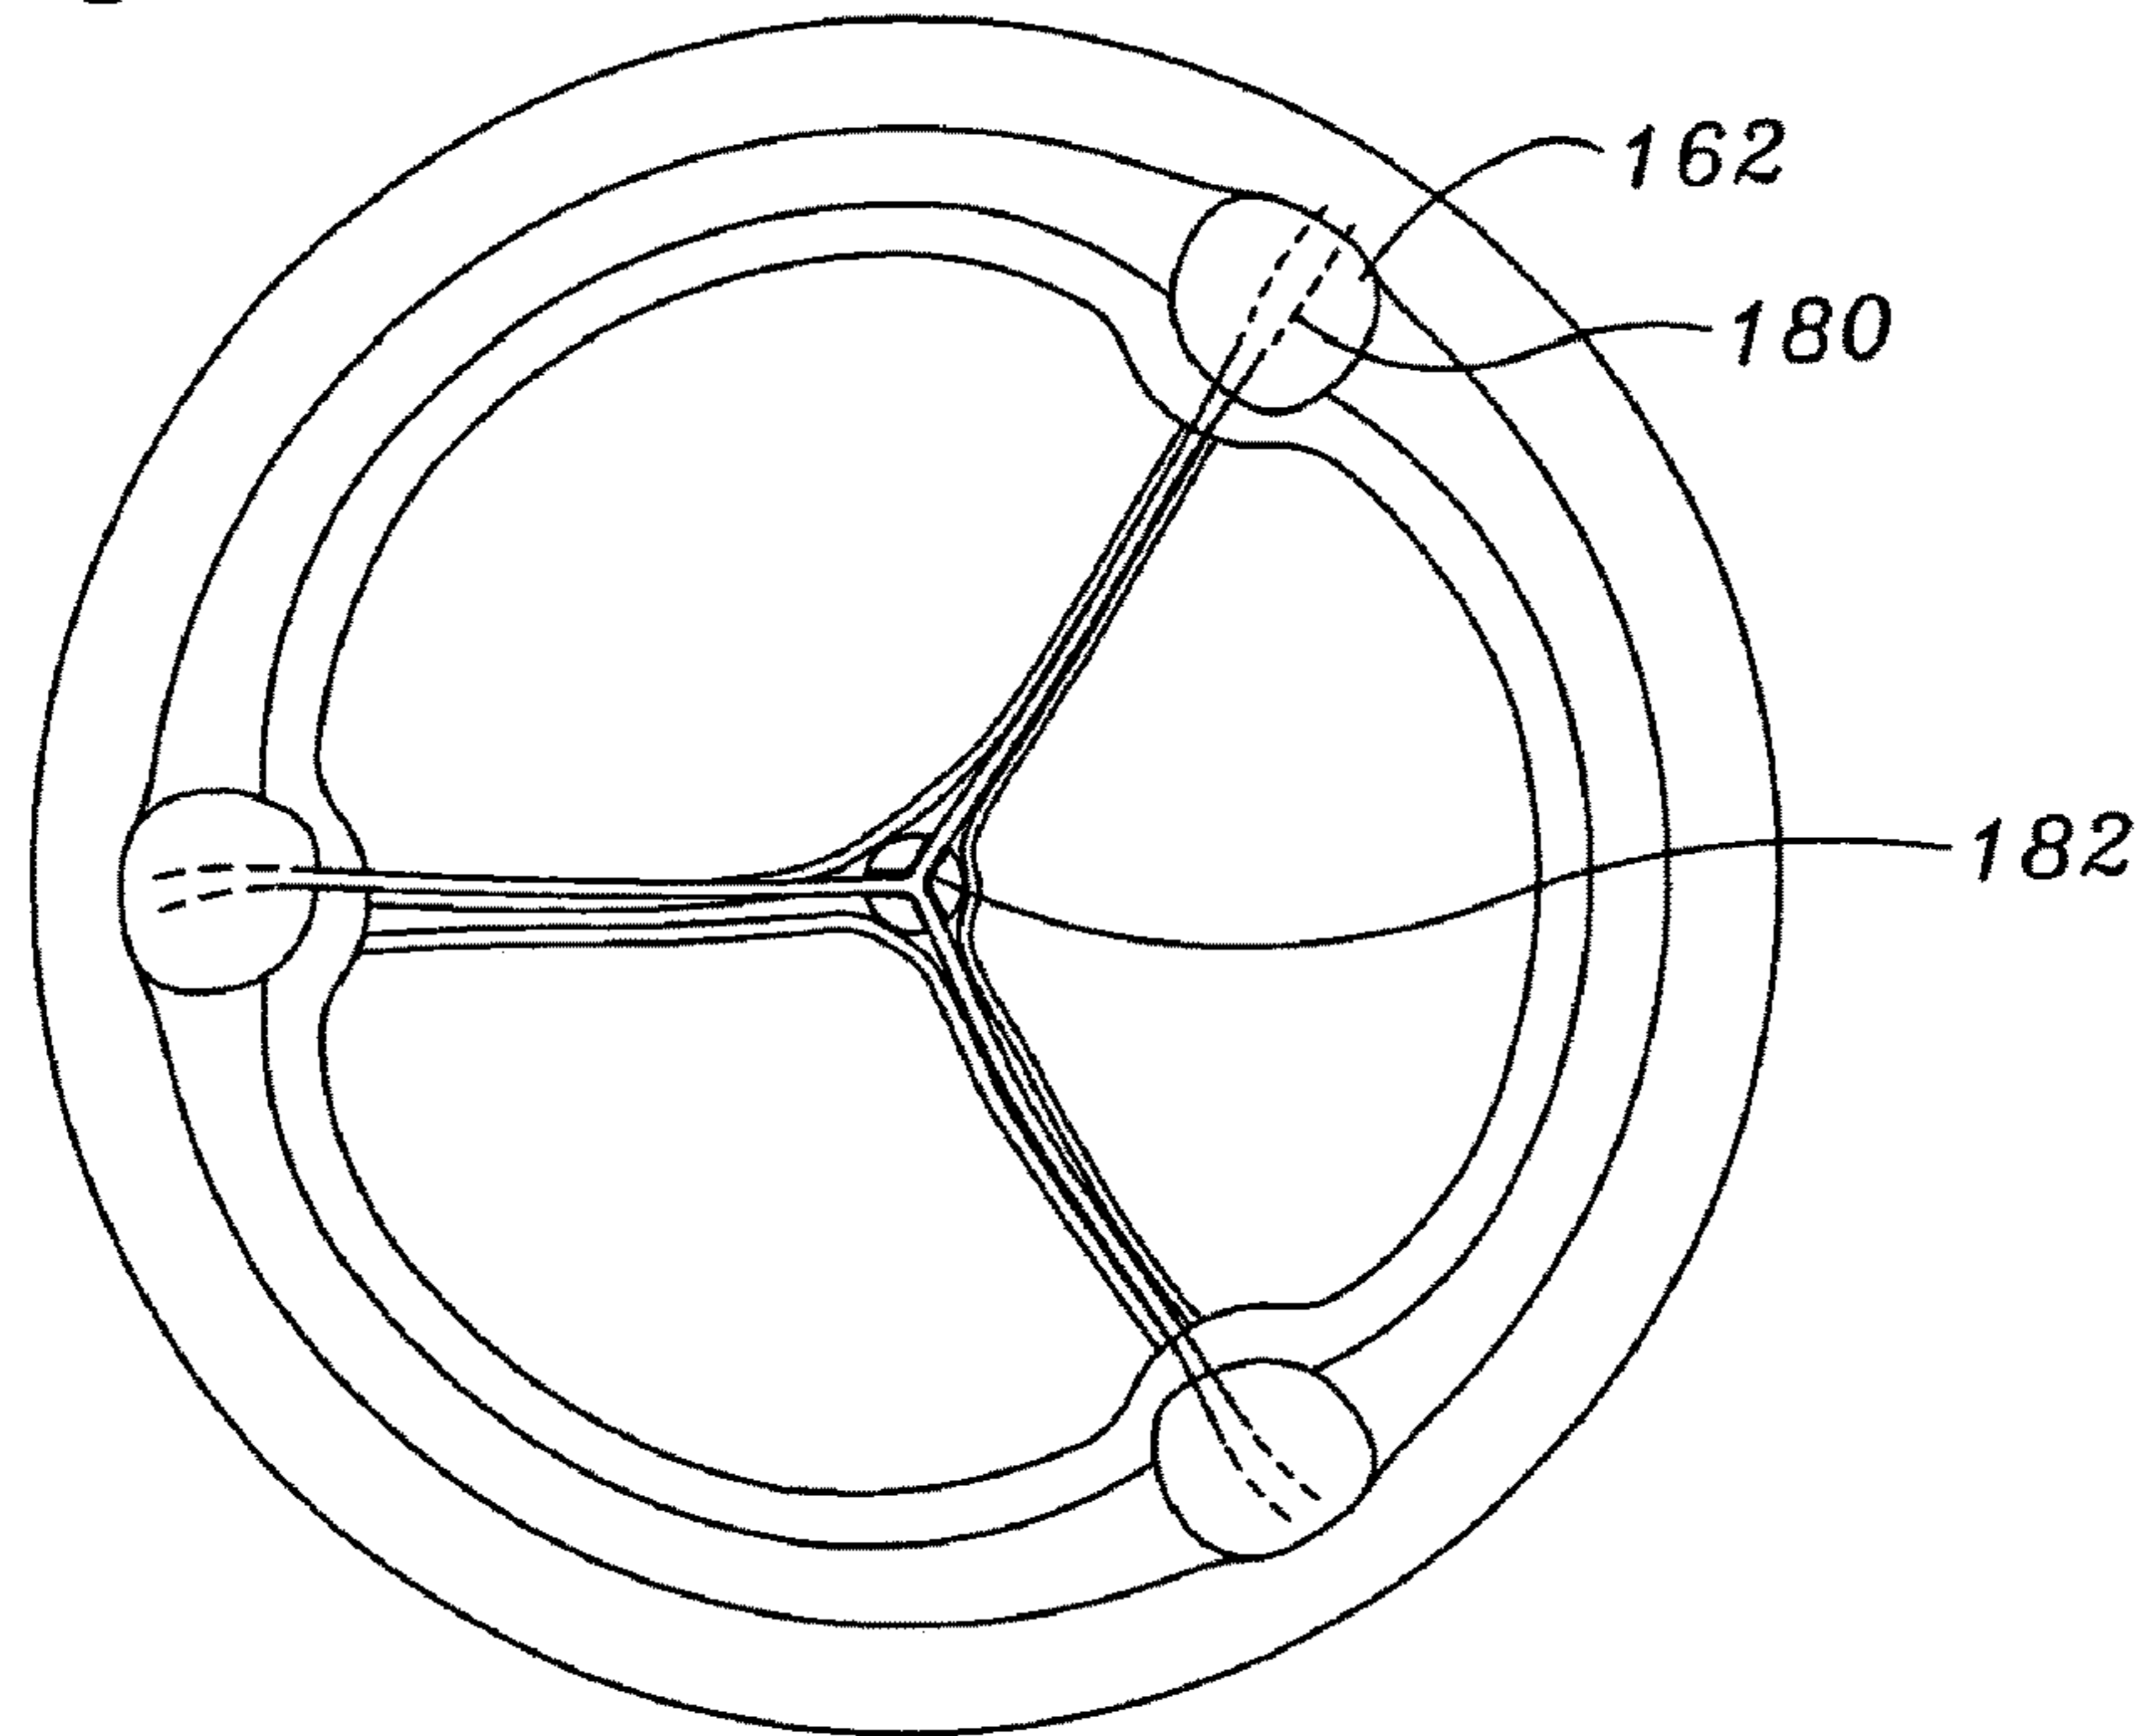
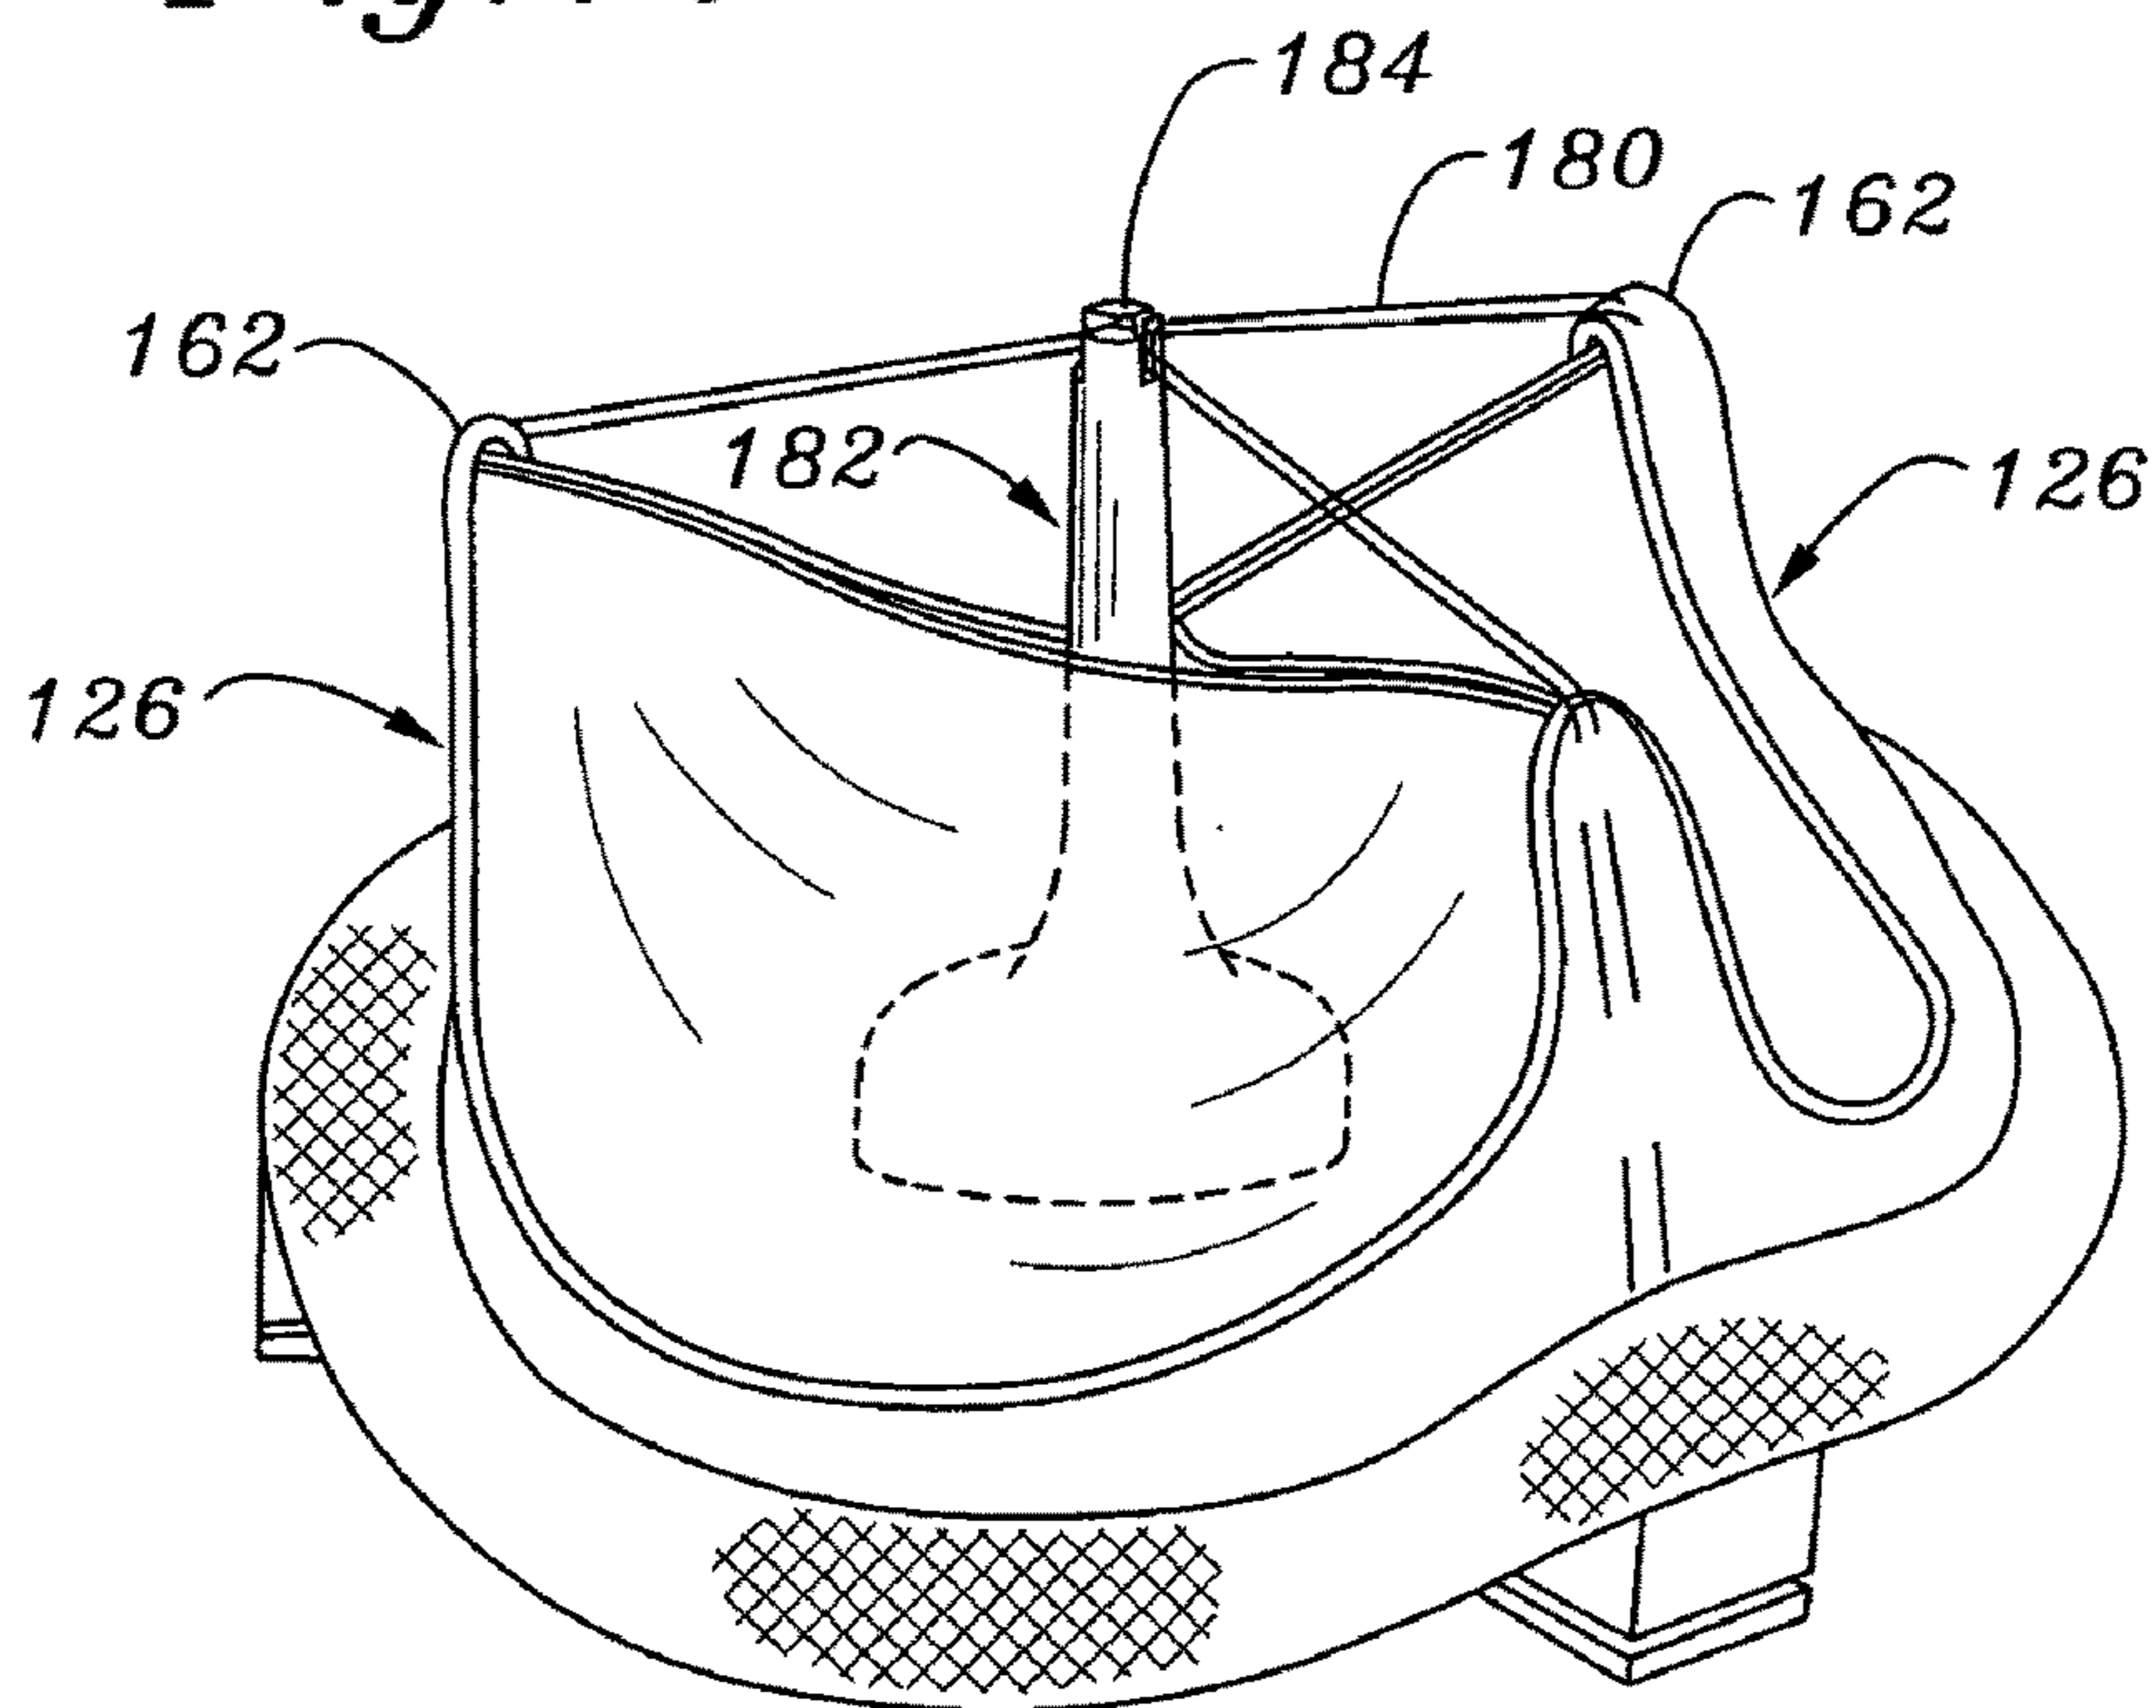


Fig. 16



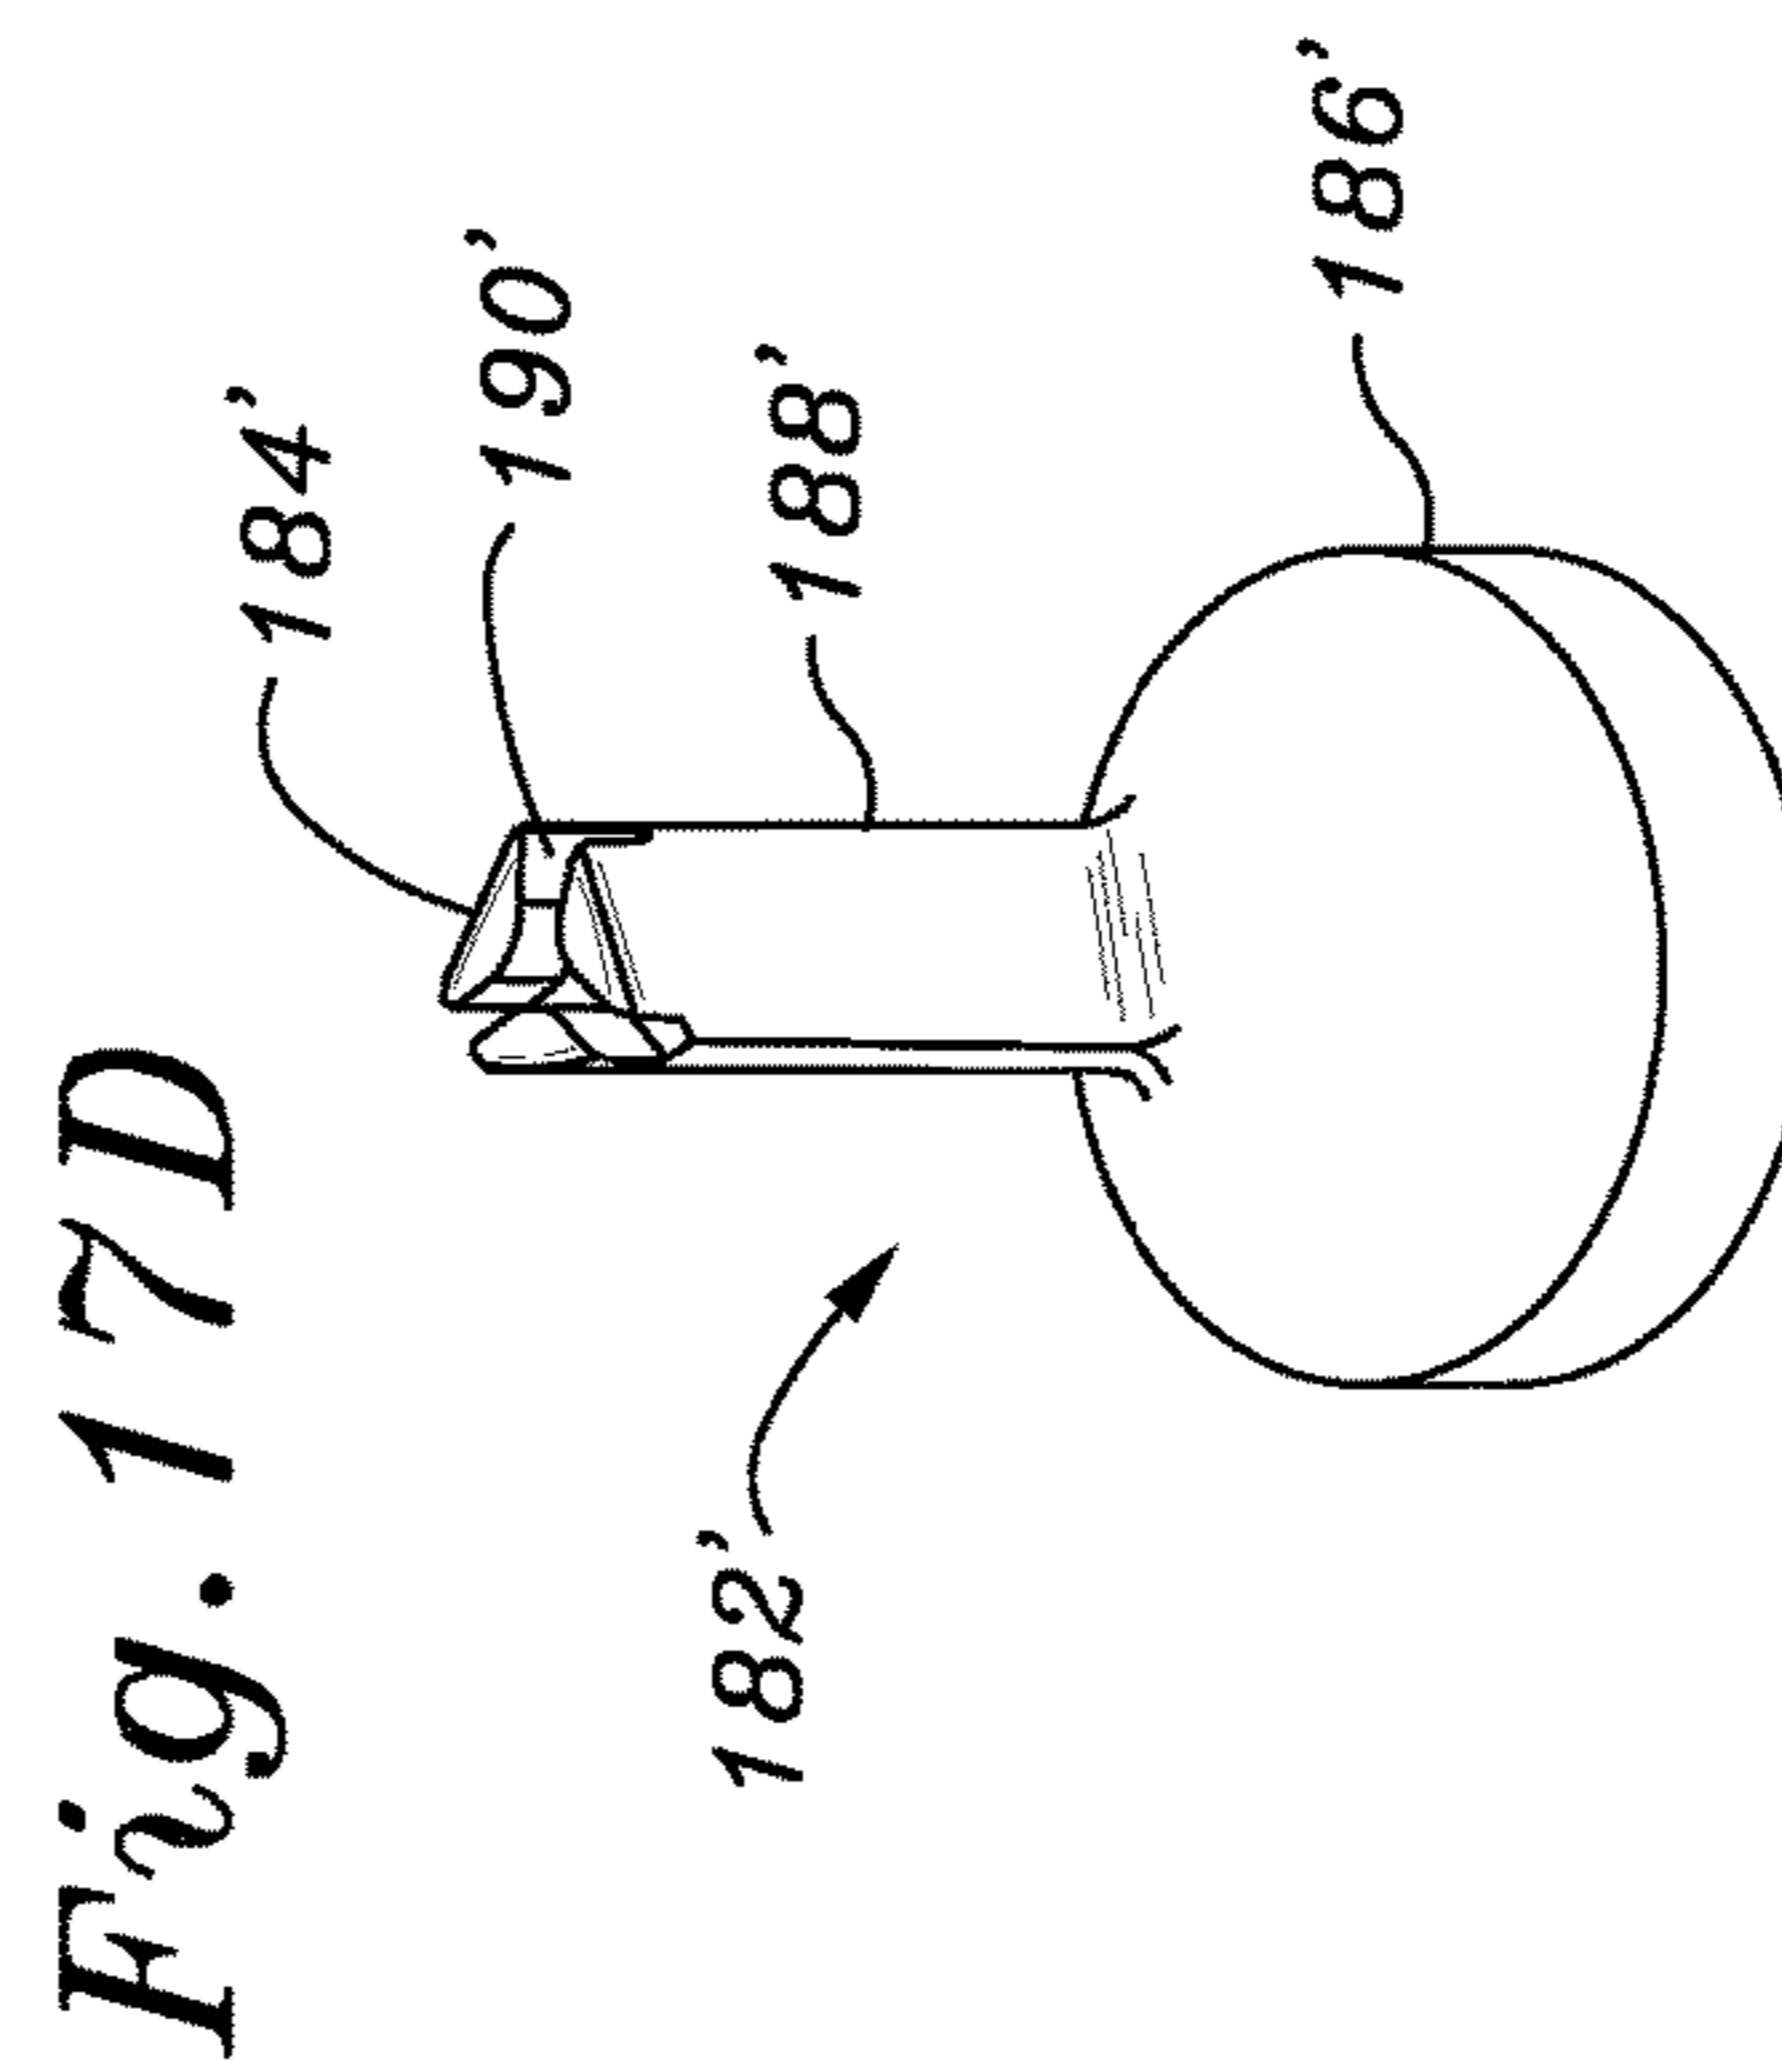
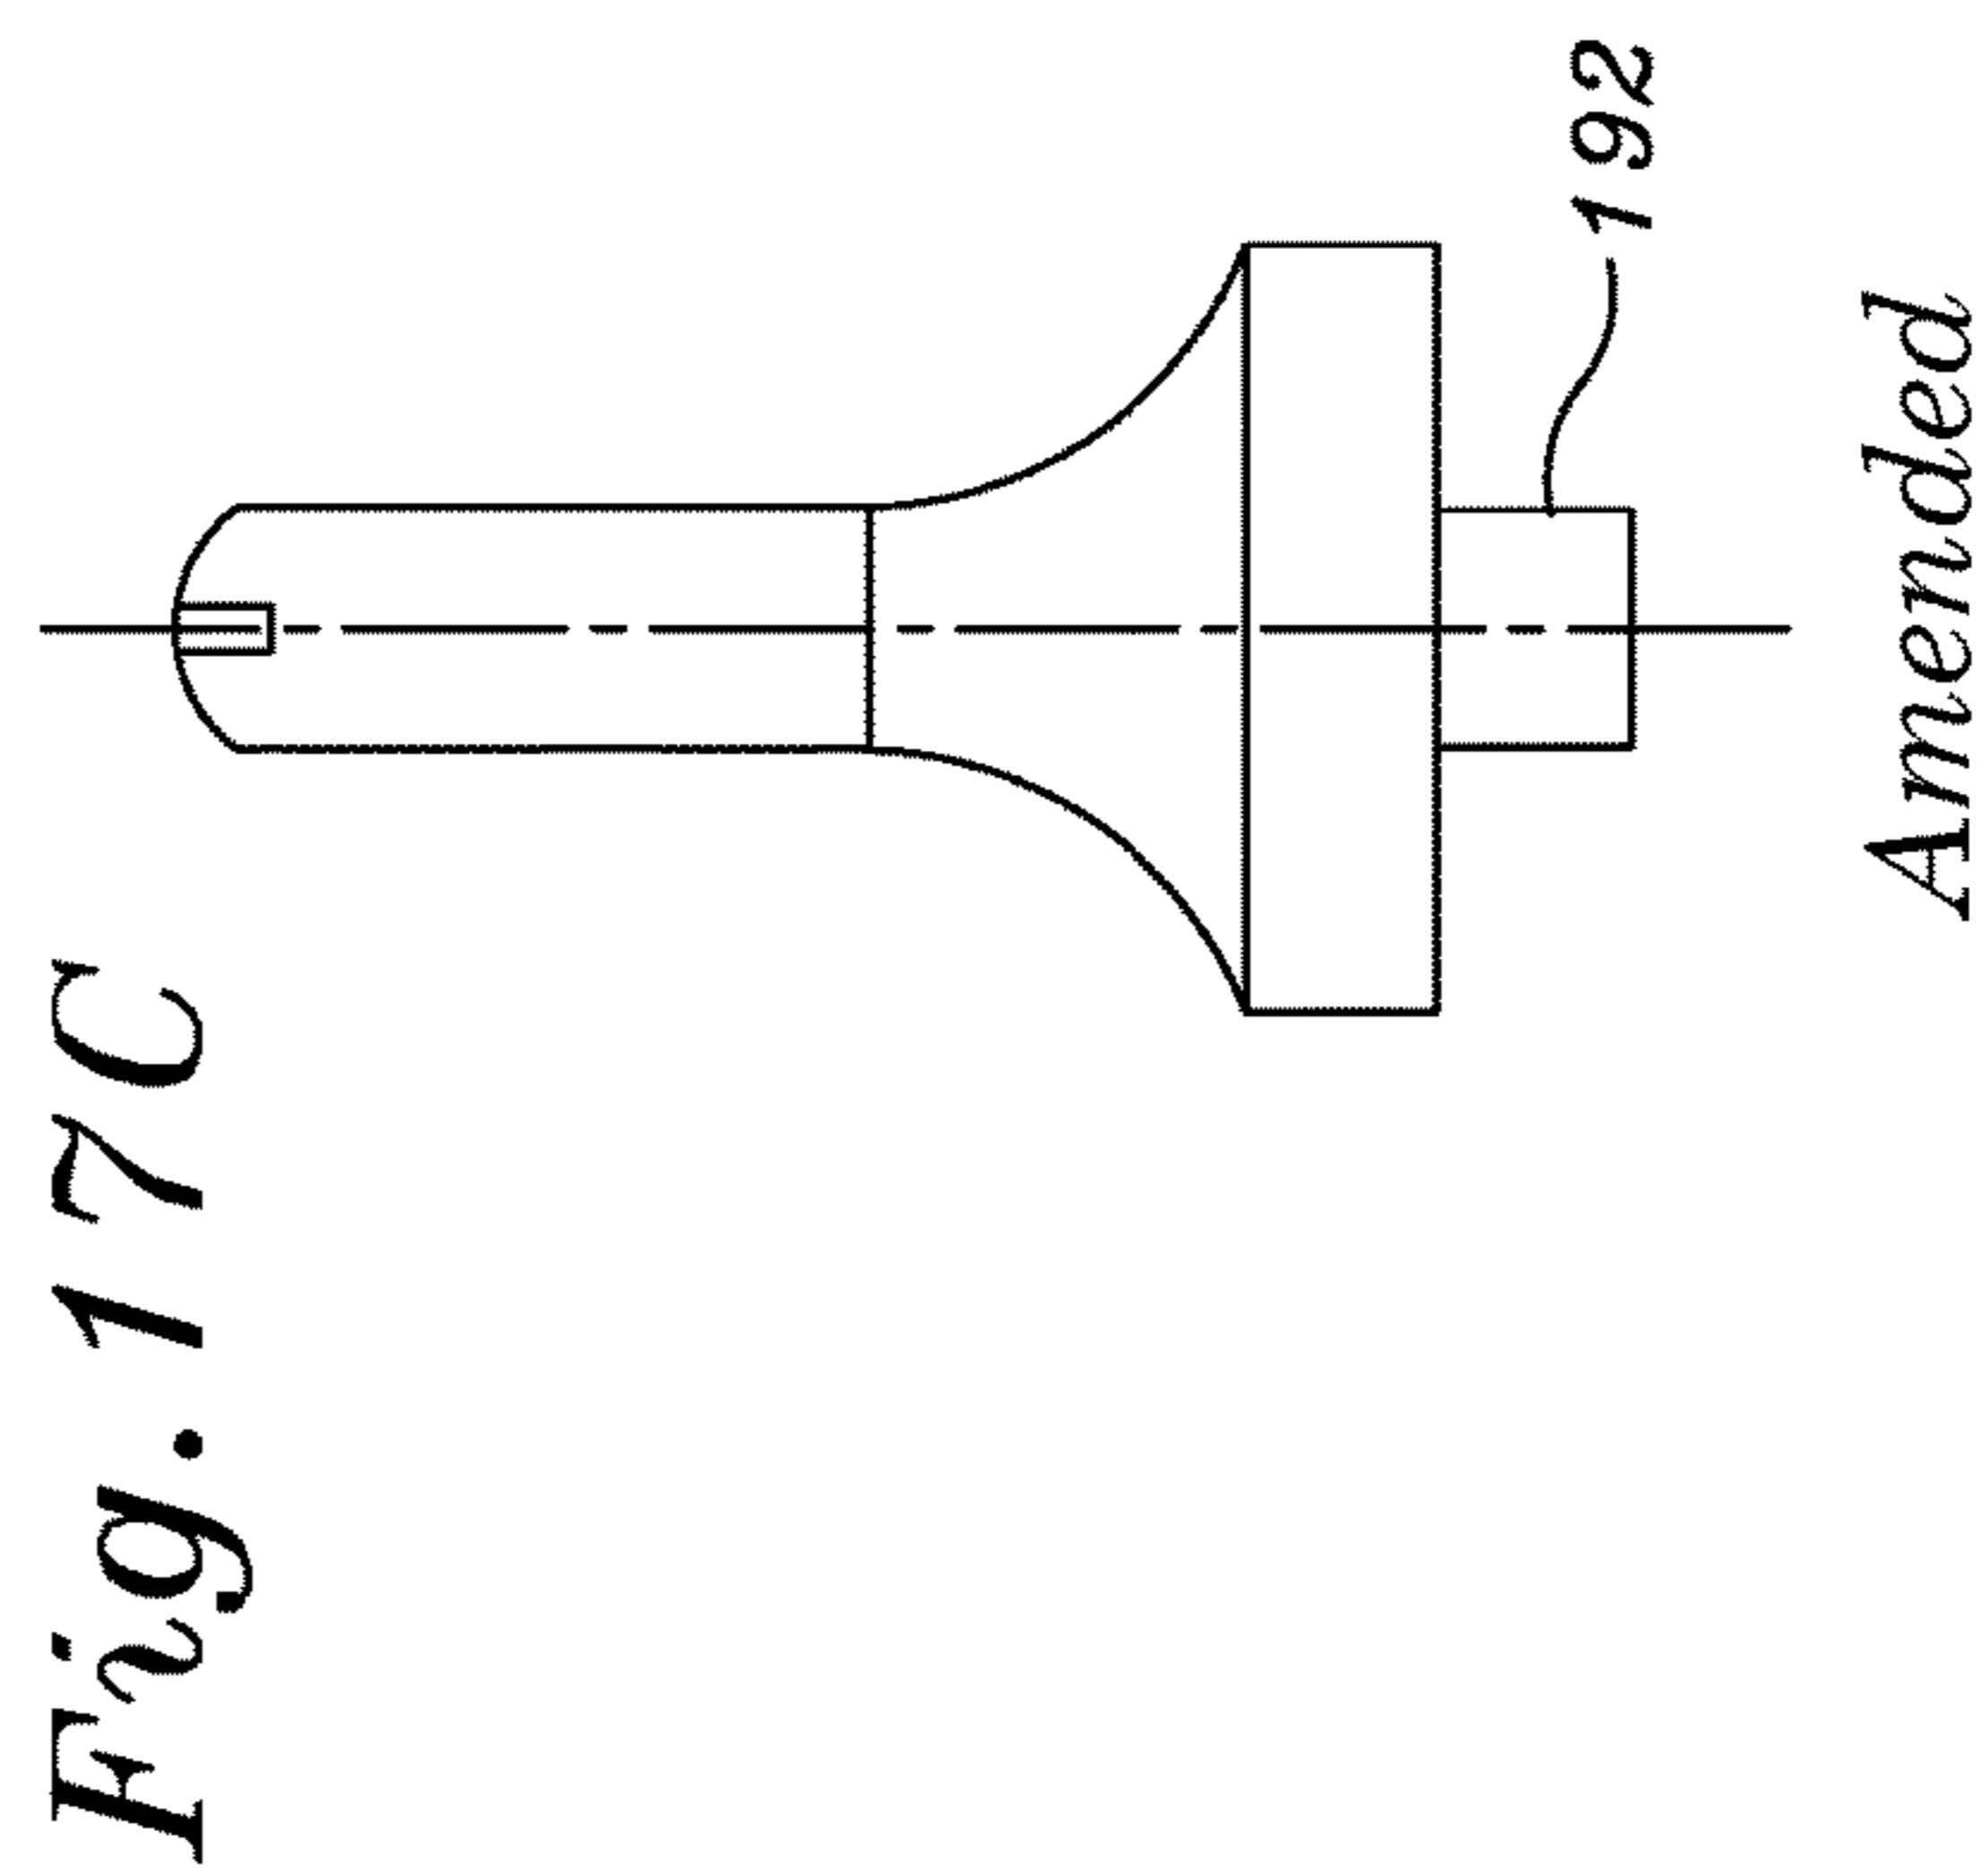
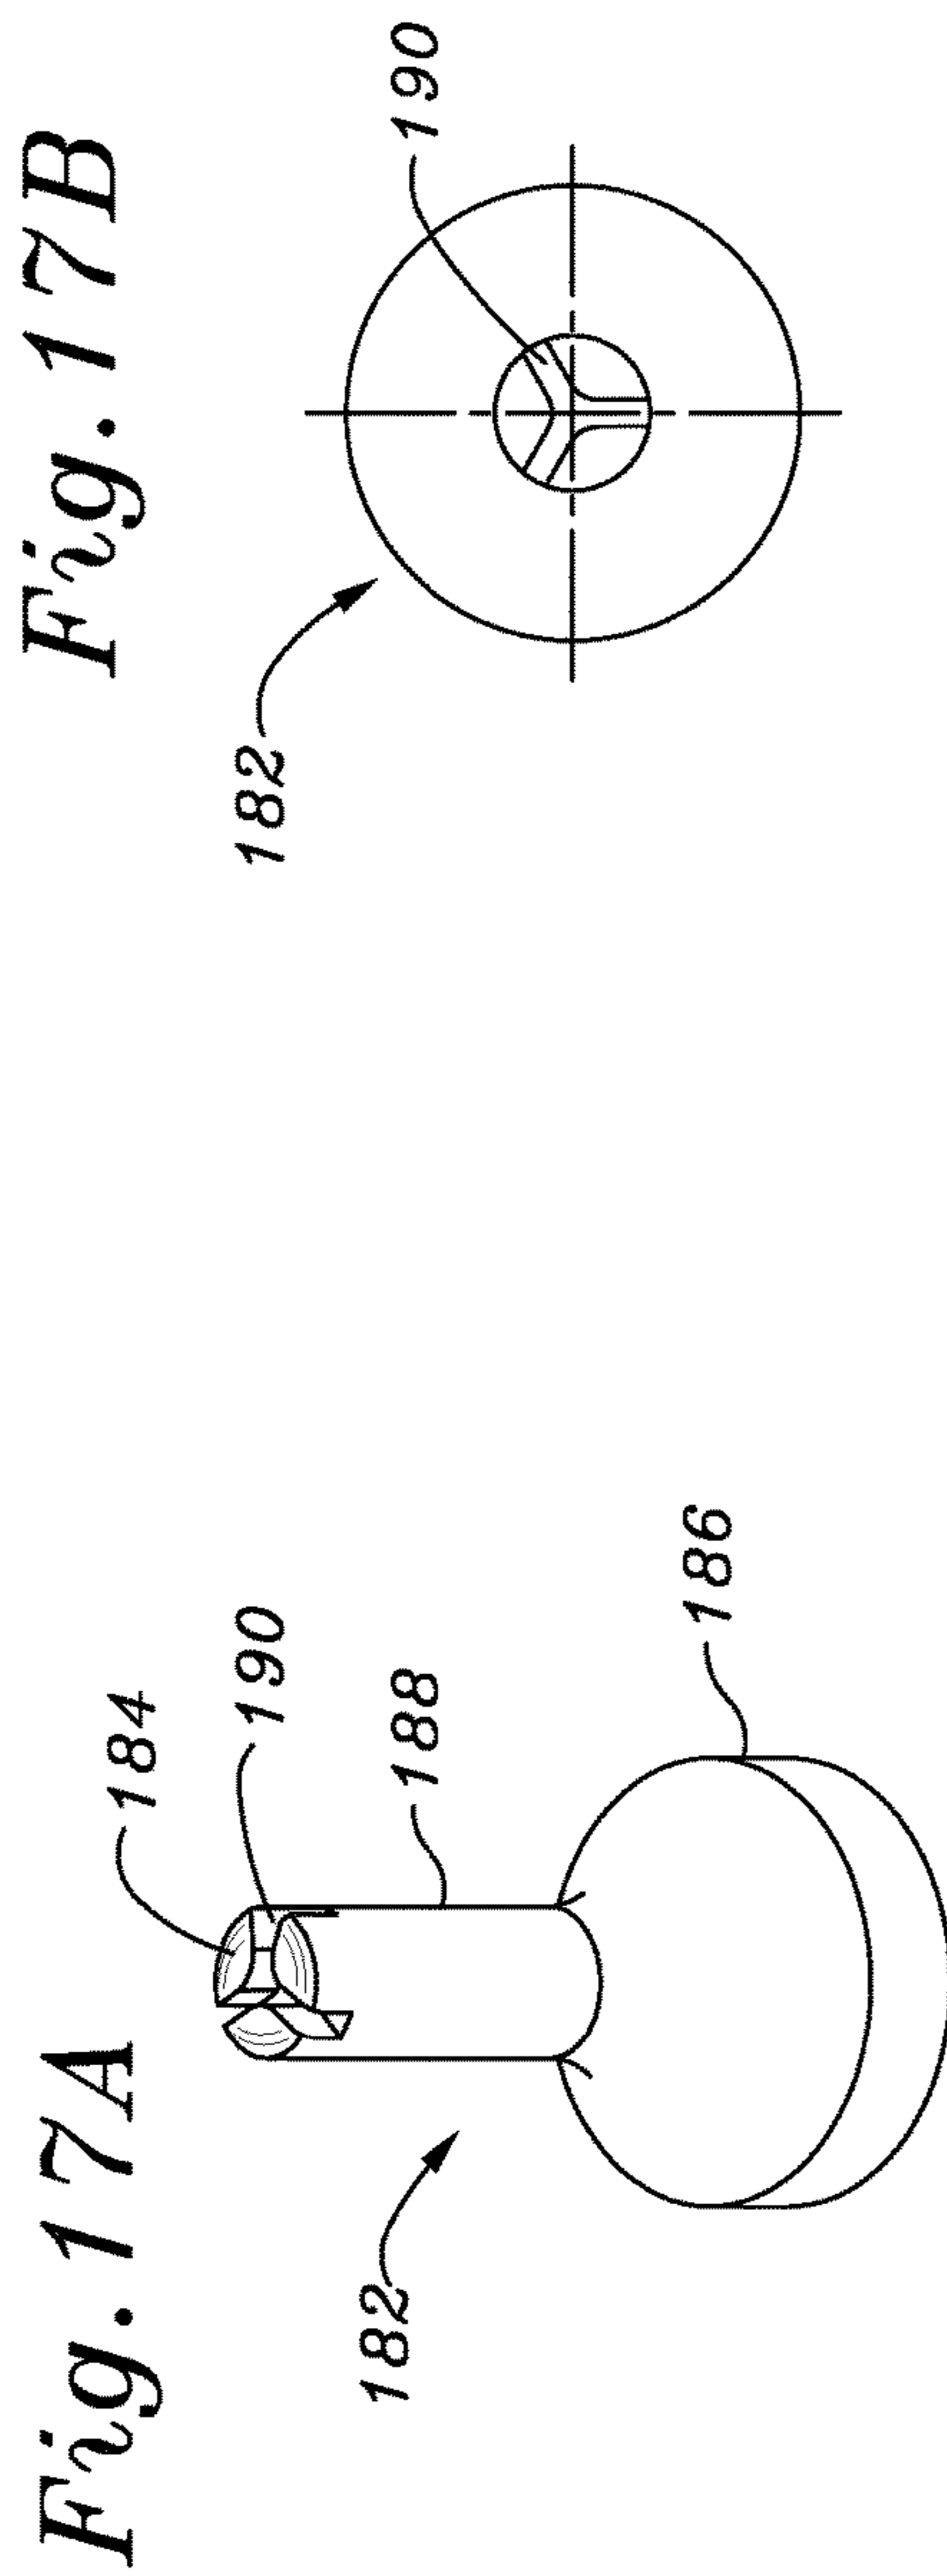


Fig. 18


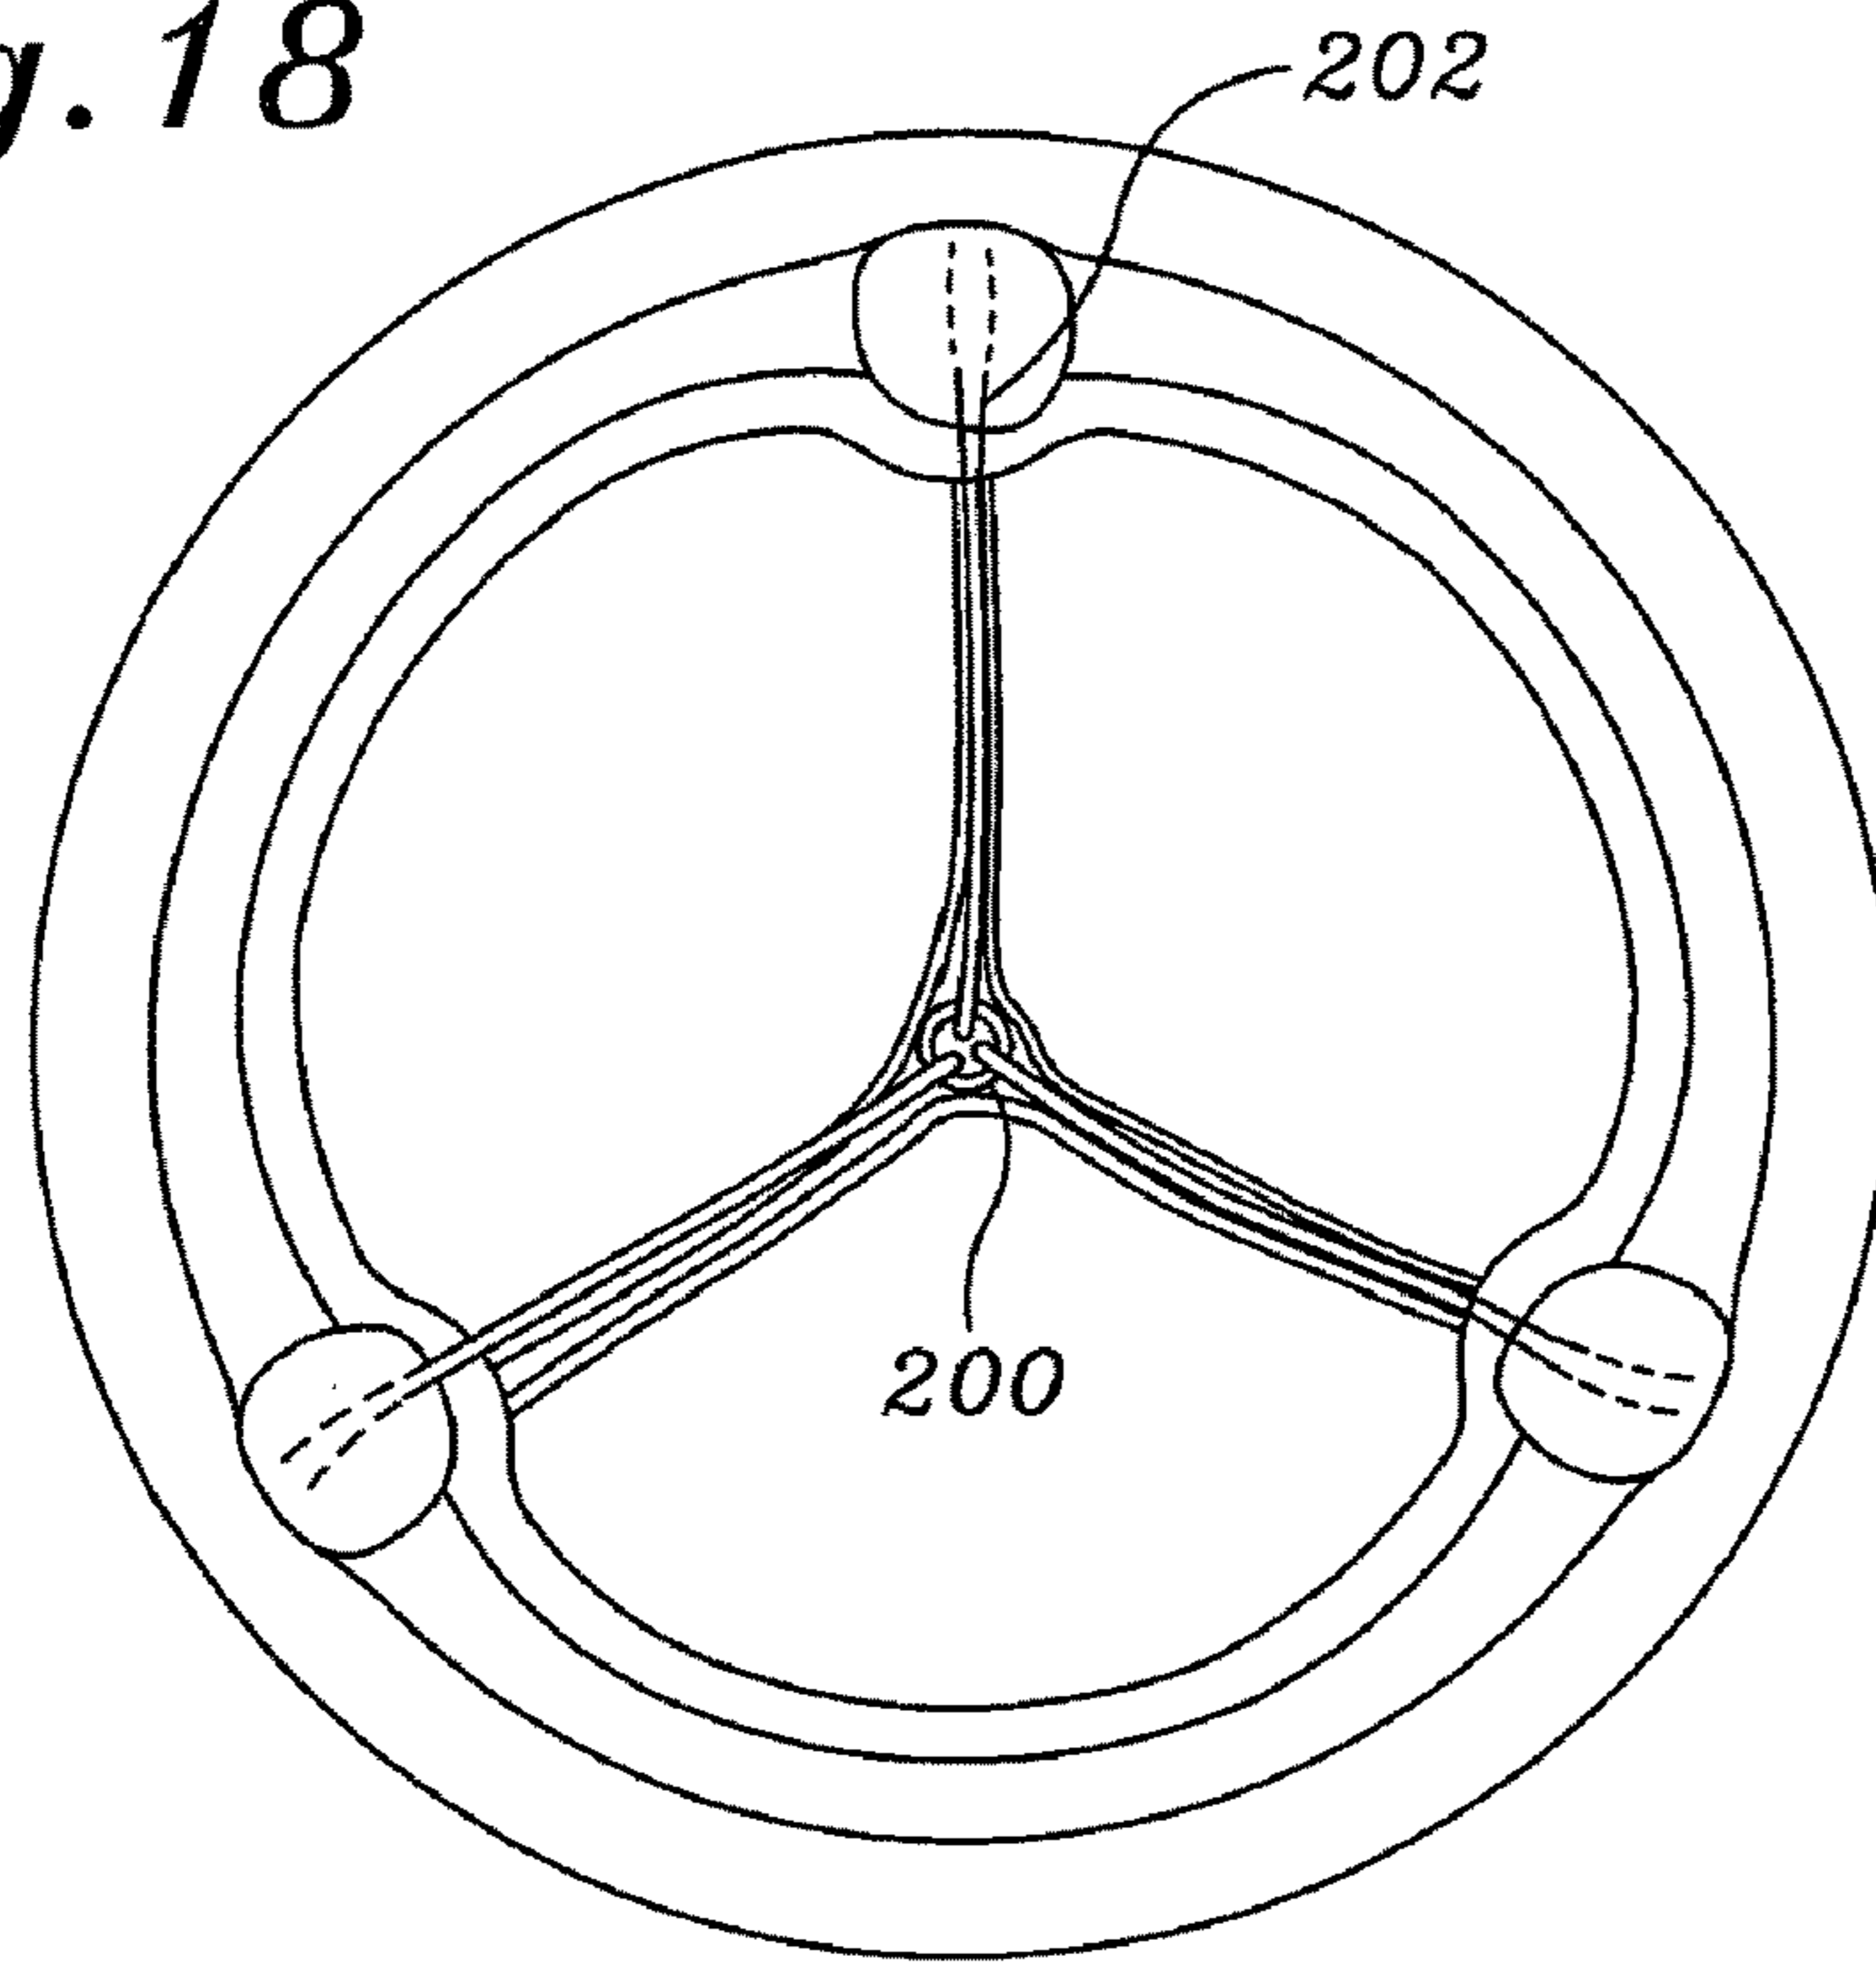


Fig. 19

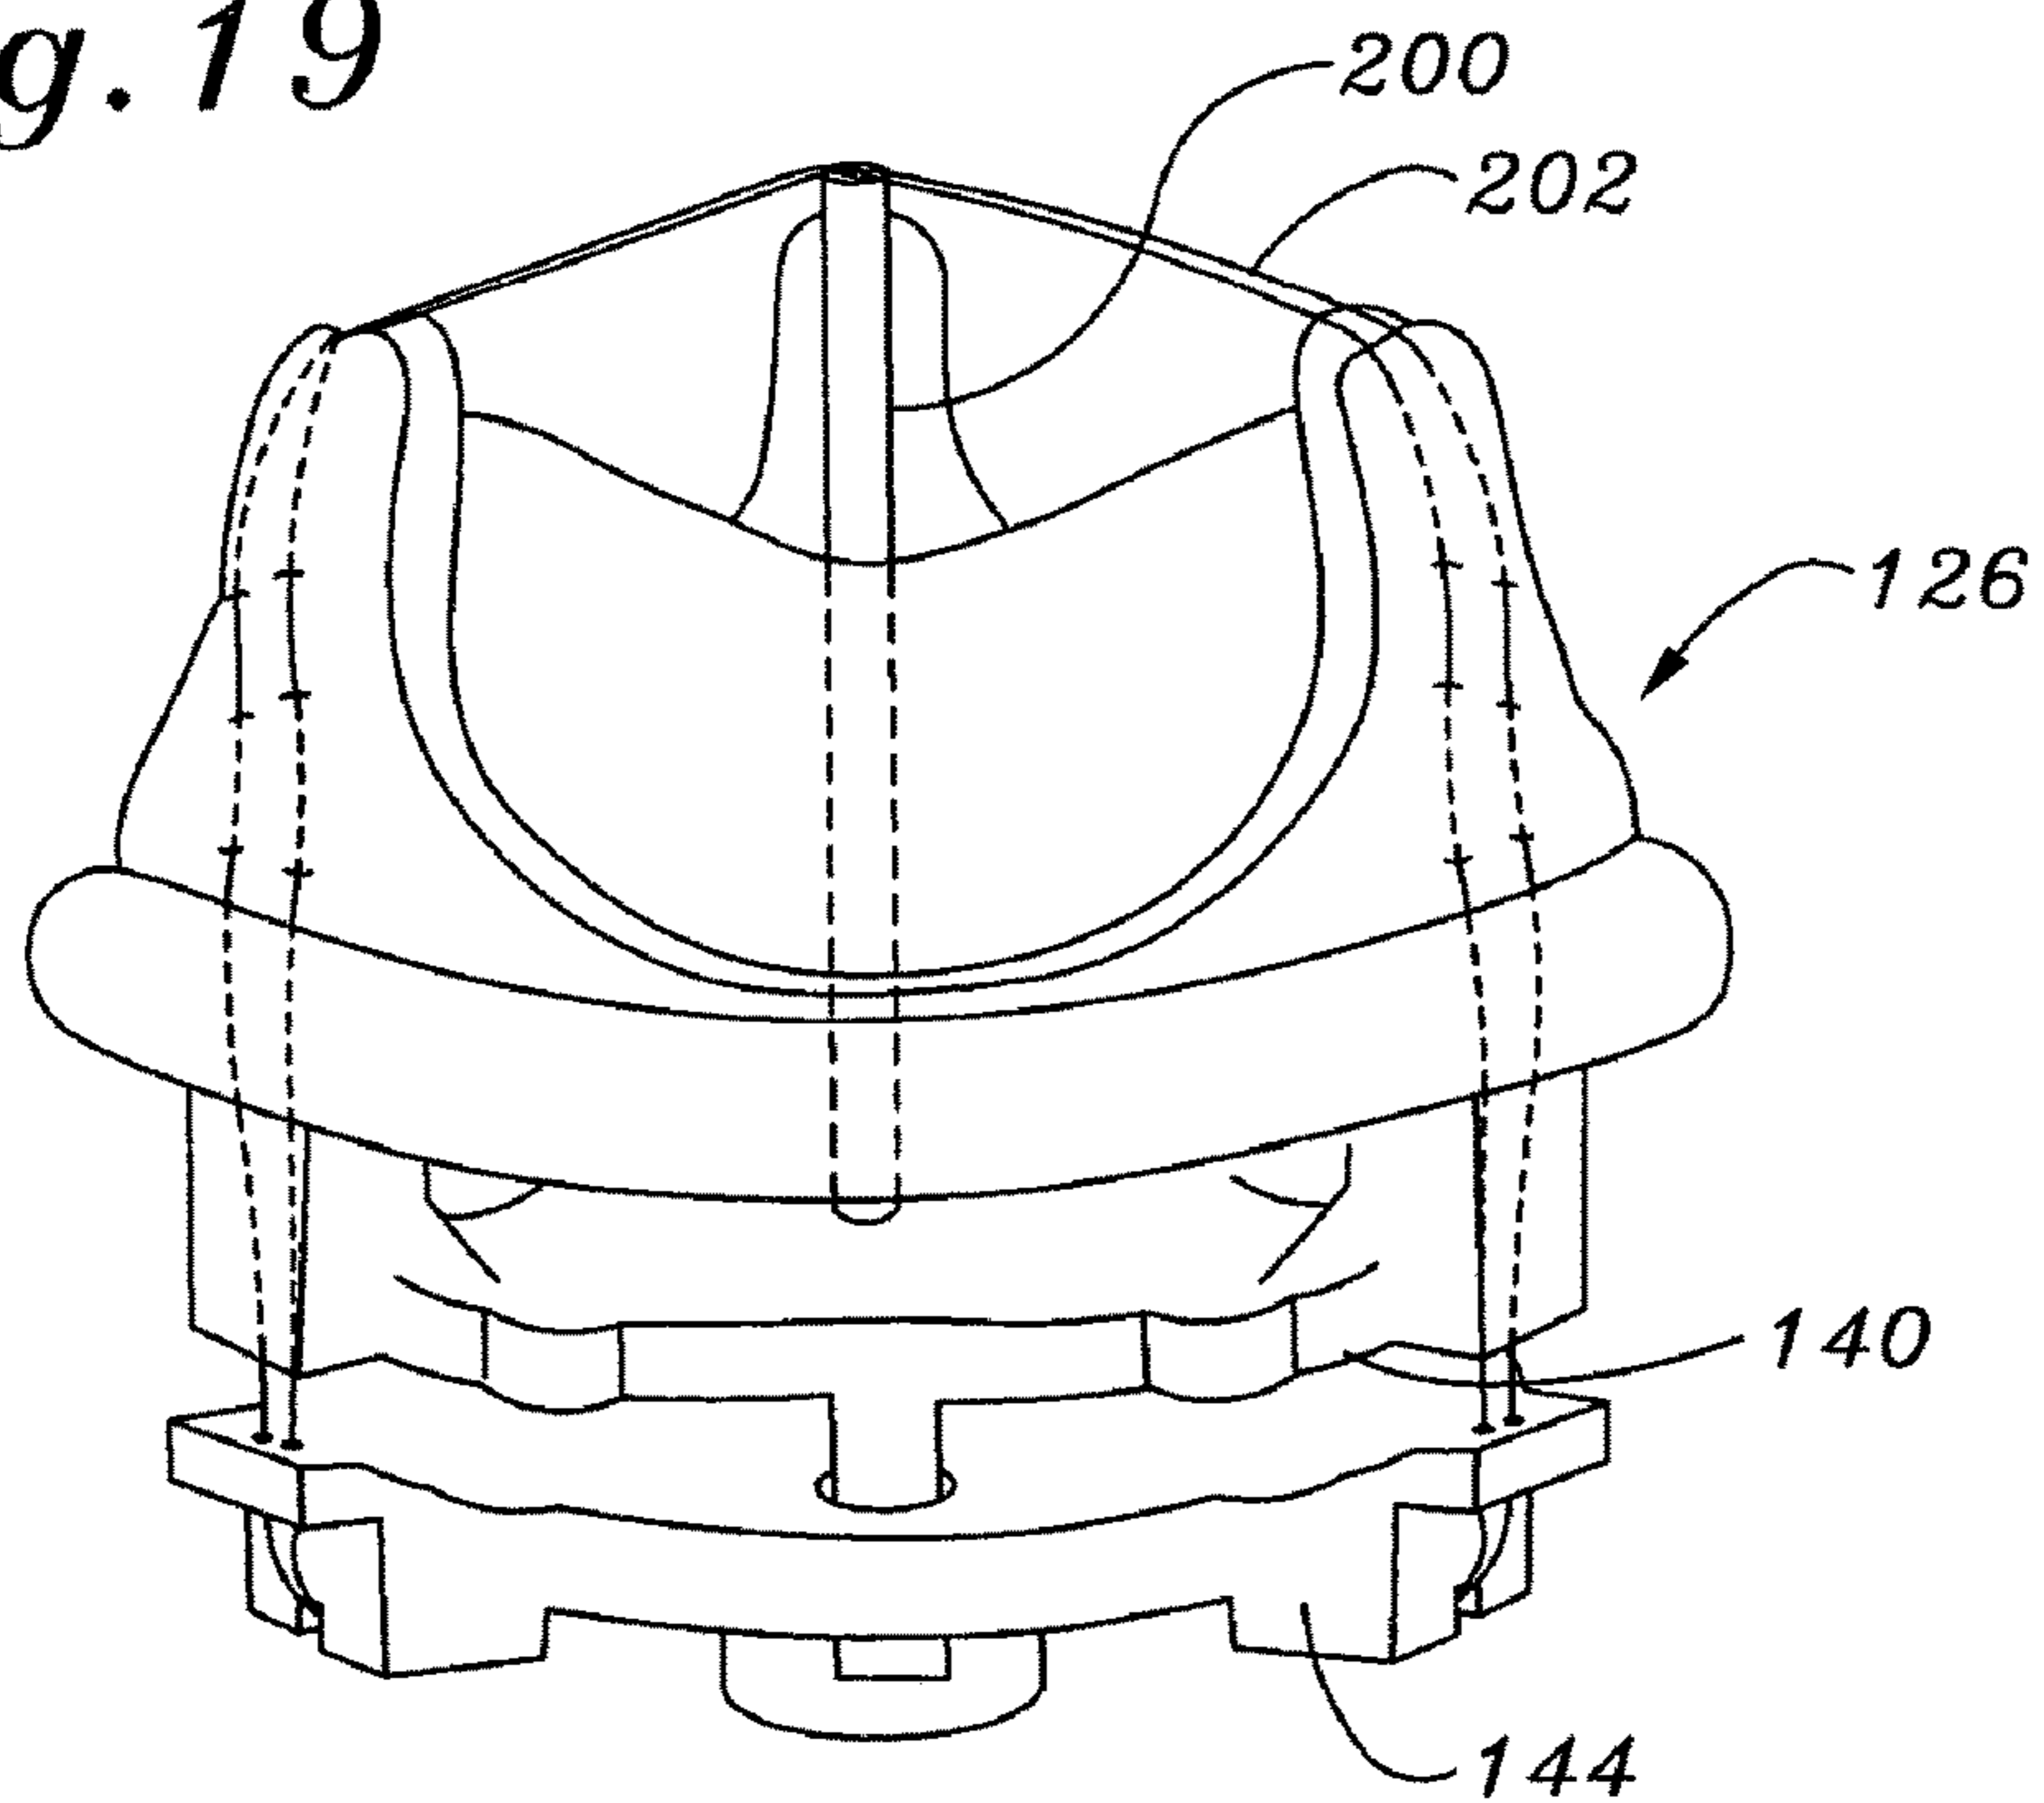

HEART VALVE HOLDER AND METHOD FOR RESISTING SUTURE LOOPING

Matter enclosed in heavy brackets [] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue; a claim printed with strikethrough indicates that the claim was canceled, disclaimed, or held invalid by a prior post-patent action or proceeding.

RELATED APPLICATIONS

The present application is a continuation of U.S. application Ser. No. 10/705,587, filed Nov. 10, 2003, now U.S. Pat. No. 6,966,925, entitled "HEART VALVE HOLDER AND METHOD FOR RESISTING SUTURE LOOPING," *reissued as RE46,668*, which is a continuation *in part* of U.S. application Ser. No. 09/745,386, filed Dec. 21, 2000, now U.S. Pat. No. 6,964,682, entitled "HEART VALVE HOLDER THAT RESISTS SUTURE LOOPING," the disclosures of which are expressly incorporated by reference herein.

FIELD OF THE INVENTION

The present invention relates generally to medical devices, and more particularly to a holder that facilitates the implantation of a bioprosthetic replacement heart valve, particularly a mitral valve, and associated methodology.

BACKGROUND OF THE INVENTION

In mammalian animals, the heart is a hollow muscular organ having four pumping chambers: the left and right atria and the left and right ventricles, each provided with its own one-way valve. The natural heart valves are identified as the aortic, mitral (or bicuspid), tricuspid and pulmonary valves, and each has leaflets to control the directional flow of blood through the heart. The valves are each supported by an annulus that comprises a dense fibrous ring attached either directly or indirectly to the atrial or ventricular muscle fibers. Various surgical techniques may be used to repair a diseased or damaged valve. In a valve replacement operation, the damaged leaflets are excised and the annulus sculpted to receive a replacement valve.

Two primary types of heart valve replacements or prostheses are known. One is a mechanical-type heart valve that uses a ball and cage arrangement or a pivoting mechanical closure to provide unidirectional blood flow. The other is a tissue-type or "bioprosthetic" valve which is typically constructed with natural-tissue valve leaflets that function much like a natural human heart valve's, imitating the natural action of the leaflets to coapt against each other and ensure the one-way blood flow. In tissue valves, a whole xenograft valve (e.g., porcine) or a plurality of xenograft leaflets (e.g., bovine pericardium) provide occluding surfaces that are mounted within a surrounding stent structure. Research is ongoing on synthesizing the tissue leaflets, and therefore the term "flexible leaflet valve" refers to both natural and artificial "tissue-type" valves. In both types of prosthetic valves, a biocompatible cloth-covered suture or sewing ring is provided, on the valve body for the mechanical type of prosthetic valve, or on the inflow end of the stent for the tissue-type of prosthetic valve.

When placing a tissue type prosthetic valve in the mitral position, the commissure posts are on the blind side of the

valve and may become entangled with pre-installed sutures, potentially damaging the annulus or tissue during delivery. The difficulty of the delivery task is compounded if the surgery is through a minimally-invasive access channel, a technique that is becoming more common. The problem of entanglement is termed "suture looping," and means that the suture that is used to attach or mount the valve to the heart tissue is inadvertently wrapped around the inside of one or more of the commissure post tips. If this occurs, the looped suture may damage one of the tissue leaflets when tightly tied down, or at least may interfere with the implant procedure or valve operation and prevent maximum coaptation of the valve leaflets, resulting in a deficiency in the prosthetic mitral valve.

Some attempts have been made to overcome these problems in current holders for prosthetic mitral valves. An example of such a holder is U.S. Pat. No. 4,865,600, Carpentier, et al., incorporated herein by reference. Carpentier provides a holder having a mechanism that constricts the commissure posts inwardly prior to implantation. The Carpentier device provides an elongate handle to both hold the valve/valve holder combination during implantation, as well as to cause the commissure posts to constrict inwardly. The valve is connected to the valve holder by the manufacturer using one or more sutures, and the combination shipped and stored as a unit. During the valve replacement procedure, the surgeon connects the handle to the holder and locks a locking nut to hold the commissure posts at a given constricted position. The surgeon then attaches the sewing ring of the valve to the native valve annulus with an array of sutures that has been pre-embedded in the annulus and extended outside the body. The valve is then advanced along the array of sutures to its desired implantation position and the sutures tied off. When the holder is cut free, the commissure posts are released to expand and the holder may be removed using the handle. However, even when the commissure posts are constricted, slack in the array of sutures, for example, may lead to looping of sutures around one of the cloth-covered commissure posts, which interferes with the implantation procedure.

What is needed then is an improved tissue-type prosthetic valve holder attachable to the inflow end of the valve that insures against suture looping.

SUMMARY OF THE INVENTION

The present invention provides a holder for a tissue-type prosthetic heart valve having an inflow end and an outflow end and a flow axis therebetween. The valve includes an annular sewing ring at the inflow end attached to a stent having posts circumferentially-spaced about the flow axis that support occluding tissue surfaces of the valve. In this type of valve the posts are cantilevered generally in the outflow direction.

The present invention provides an improved holder system for preventing suture looping around the commissure posts of tissue-type heart valves that are implanted in the direction where the commissure posts form the leading end of the valve. For instance, the present invention provides an improved holder for a mitral valve where lengths of flexible material connect the holder and valve and extend between the commissure posts of the valve. Each length of flexible material extends axially, desirably through the valve, to be connected at two points to a rigid holder structure that abuts the inflow end of the valve. Severing the lengths of flexible material near one of the attachment points permits removal of the entire length of material from the valve along with the

3

rigid structure, by virtue of the second attachment point. In a preferred embodiment, the rigid structure incorporates a mechanism for tensioning the lengths of flexible material to cause the commissure posts of the valve to flex inward.

In accordance with one aspect the present invention, a holder for a flexible leaflet prosthetic heart valve is provided. The heart valve is attachable to a surgical delivery handle and has an inflow end, an outflow end, and a flow axis therebetween. The heart valve is of the type that includes an annular sewing ring at its inflow end and a plurality of generally axially-extending commissure posts circumferentially-spaced around the outflow end that support occluding flexible leaflets of the valve. The holder includes a rigid valve abutment portion, a shaft member, and a plurality of lengths of flexible material. The valve abutment portion contacts the annular sewing ring at the inflow end of the valve. The shaft member is axially movable relative to the valve abutment portion between a first position wherein a distal tip of the shaft member is located to the inflow side of the leaflets, and a second position wherein the distal tip is located to the outflow side of the leaflets. The lengths of flexible material extend in a taut fashion across the outflow end of the valve to prevent suture looping, and each length of flexible material has first segments extending radially inward from the commissure posts to the shaft member in its second position. Desirably, the commissure tips of the valve are flexible and extend generally axially in the first position of the shaft member but are cantilevered radially inward by engagement of the shaft member with the lengths of flexible material in the second position of the shaft member. Furthermore, the lengths of flexible material may be secured to the valve abutment portion at both ends.

In accordance with one embodiment, the distal tip of the shaft member in its second position extends axially beyond the commissure posts such that each first segment of the lengths of flexible material extends at an angle both radially inward and axially in the outflow direction to the distal tip of the shaft member. Preferably, the shaft member includes notches on its distal tip for receiving midpoints of the first segments of the lengths of flexible material. Each first segment therefore extends from one of the commissure posts radially inward to the shaft member and then radially outward to an adjacent commissure post via a notch in the shaft member.

Desirably, the valve abutment portion comprises a tubular body having a bore for receiving the shaft member, shaft member being axially movable within the bore between the first and second positions. The holder may further include structure for axially restraining the shaft member in the second position with respect to the valve abutment portion. For example, a cantilevered pawl on the shaft member may be provided that engages the bore of the valve abutment portion and axially restrains the shaft member in the second position. Also, structure may be provided for rotationally restraining the shaft member with respect to the valve abutment portion as the shaft member moves between the first and second positions.

The present invention also provides a holder for a tri-leaflet flexible leaflet prosthetic heart valve as described above. The holder includes a shaft member that is axially movable relative to the valve along its flow axis between a first position and a second position, the shaft member having a distal tip. Three lengths of flexible material extend in a taut fashion across the outflow end of the valve to prevent suture looping, and each length of flexible material has a first segment that extends radially inward and mutually crosses over the other two first segments so that each remains along

4

the flow axis of the valve. With this arrangement, the distal tip of the shaft member contacts the crossed-over first segments in its second position and displaces them to be angled in the outflow direction.

The tri-leaflet valve holder may also include a valve abutment portion in contact with the valve sewing ring to which each length of flexible material is secured at both ends. The valve abutment portion may have outwardly extending brackets for engaging the valve sewing ring, the brackets having through holes for receiving and securing the lengths of flexible material. Preferably, the valve abutment portion comprises a tubular body having a bore for receiving the shaft member, which is axially movable therein between the first and second positions. The holder may include structure for axially restraining the shaft member in the second position with respect to the valve abutment portion, such as a cantilevered pawl on the shaft member that engages the bore of the valve abutment portion. Further, the holder may have structure for rotationally restraining the shaft member with respect to the valve abutment portion as the shaft member moves between the first and second positions. The holder may also include a handle interface releasably secured with sutures to the shaft member and having a threaded bore for receiving an externally threaded boss on a distal end of a surgical delivery handle. The handle interface and delivery handle can be disengaged from the shaft member upon severing the sutures. Desirably, the shaft member includes notches on its distal tip for capturing and retaining the first segments of the lengths of flexible material.

In one particular embodiment, a holder is provided that includes a plurality of lengths of flexible material extending in a taut fashion across the outflow end of the valve to prevent suture looping, each length of material having a first segment extending directly between adjacent commissure posts and crossing over each adjacent length of material adjacent to the commissure post. The lengths of flexible material may be sutures, or may comprise a band of bio-compatible material, such as polyester. In the latter instance, the band of material may completely cover each commissure post, and may cross over adjacent bands of material. Desirably, a slide is created by the lengths of flexible material adjacent each commissure post, for example by crossing over suture filaments at or radially inward from the commissure posts.

In another embodiment of the invention, the holder includes a plurality of lengths of flexible material extending in a taut fashion across the outflow end of the valve to prevent suture looping, each length of material having a first segment extending in a band that is substantially wider than it is thick directly between adjacent commissure posts. Each length of flexible material may extend in second segments along two adjacent commissure posts to be attached to the rigid structure at two points. Desirably, the commissure posts are cloth covered and the second segments pass beneath the cloth covering in a configuration that is not as wide as the first segments.

In a further aspect of the present invention, the holder includes a central upstanding member passing along the axis of the valve from the inflow side to the outflow side of the leaflets. A plurality of lengths of flexible material extend in a taut fashion across the outflow end of the valve to prevent suture looping, each length of flexible material having first segments extending radially inward from one of the commissure posts, preferably at a steep angle, to the central

5

upstanding member. The central upstanding member may be hollow, with each length of flexible material passing into and through the member.

Alternatively, the upstanding member may be solid and include notches for capturing and retaining the midpoints of the first segments of lengths of flexible material. In this case, each first segment extends, preferably at a steep angle, from one of the commissure posts radially inward to the upstanding member and then radially outward to an adjacent commissure post via a notch. The upstanding member may include a wide base on an end that is attached to a rigid structure of the holder that abuts the sewing ring. A narrow shaft extends from the wide base and passes between and to the outflow side of the leaflets. The narrow shaft may have a non-circular cross-section, such as triangular, to reduce deformation of the leaflets from long-term storage.

The holder may include a valve abutment portion sized and shaped to abut the sewing ring at the inflow end of the valve. The holder may further include a commissure post constriction mechanism adapted to constrict the commissure posts radially inward from a relaxed position to a constricted position when actuated by a handle. A retaining mechanism may also be provided that retains the commissure post constriction mechanism in the constricted position after the handle is removed.

In one embodiment the commissure post constriction mechanism comprises an adjusting portion and an adjusting member adapted to adjust the distance between the adjusting portion and the valve abutment portion, and one or more filaments attached to the adjusting portion and sutured through the end of the commissure posts distal to the adjusting portion. When the adjusting member is operated to separate the adjusting portion from the valve abutment portion the adjusting portion pulls the filaments, which in turn urge the end of the commissure posts distal to the adjusting portion radially inwardly, to the constricted position.

The valve abutment portion may have a planar shape, with the adjusting portion having a substantially complementary planar shape. It is preferred that the planar shape of the valve abutment portion be comprised of a plurality of tangs radiating from a central body to each cover a portion of the sewing ring. In this manner a sufficient amount of the sewing ring is left exposed to allow for suturing the sewing ring to the native annulus. Stated another way, the holder may include two relatively movable plates, one of which attaches to the valve sewing ring on the inflow end of the valve and the other which attaches via sutures or similar expedient to the valve commissures on the outflow end. Separation of the plates places the sutures in tension and constricts the commissures.

Adjustment of the distance between the valve abutment portion and the adjusting portion (e.g., relatively movable plates) may be achieved by providing a central threaded aperture in the adjusting portion and an adjusting member that cooperates with this threaded aperture. In this construction the end of the adjusting member proximal the valve abutment portion abuts the valve abutment portion during operation. When the adjusting member is advanced through the central aperture of the adjusting portion it pushes the valve abutment portion and the two portions separate.

A handle may be operatively connected to the adjusting member to turn it by providing a handle that has an externally threaded end portion and an adjusting member having a central longitudinal threaded bore sized to receive the threaded end portion. When the handle is introduced into the bore it is rotated in a first direction and will seat in the

6

threaded bore of the adjusting member. Further rotation of the adjusting member separates the adjusting portion from the valve abutment portion, as recited above, and causes the commissure posts to constrict inwardly.

A further understanding of the nature and advantages of the present invention are set forth in the following description and claims, particularly when considered in conjunction with the accompanying drawings in which like parts bear like reference numerals.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A-1C are schematic elevational views of the deployment of a prosthetic heart valve using an exemplary holder of the present invention;

FIG. 2 is an exploded perspective view of an exemplary heart valve holder of the present invention along with a representative heart valve and surgical handle;

FIG. 3A is a perspective view of an assembled heart valve holder of FIG. 2 attached to a heart valve and a surgical handle;

FIG. 3B is a perspective view as in FIG. 3A after rotation of the surgical handle and a shaft member of the holder relative to a valve abutment portion and prior to actuation of the shaft member;

FIG. 3C is a perspective view as in FIG. 3B after axial displacement of the shaft member from a first position to a second position where a distal tip of the shaft member contacts lengths of flexible material that secure the holder to the heart valve;

FIG. 3D is a perspective view as in FIG. 3C after removal of the surgical handle and a handle interface to permit greater visibility during the implant procedure;

FIG. 4A is an axial sectional view of the assembled holder of FIG. 2 and heart valve with the shaft member in its first position, and also showing a protective transport cage;

FIG. 4B is a sectional view like FIG. 4A and corresponding to the second position of the shaft member shown in FIG. 3C;

FIGS. 5A and 5B are partial axial sectional views of the holder, handle and valve combination corresponding to the positions of the shaft member shown in FIGS. 3A and 3B;

FIG. 5C is an axial sectional view of the holder, handle and valve combination and showing the rapid detachment of the handle along with the handle interface;

FIG. 5D is an axial sectional view of the holder after having been detached from the valve;

FIG. 6A is an outflow plan view of the assembled holder and valve as seen along line 6A-6A in FIG. 3A prior to actuation of the shaft member and simultaneous constriction of valve commissure tips;

FIG. 6B is an outflow plan view of the assembled holder and valve as seen along line 6B-6B in FIG. 3C after actuation of the shaft member and constriction of the valve commissure tips;

FIG. 7 is an enlarged plan view taken within the circle indicated in FIG. 6A along the valve flow axis illustrating the cross over of a plurality of lengths of flexible material securing the holder to the valve;

FIGS. 8 and 9 are opposite plan views of a valve abutment portion of the exemplary holder of FIG. 2.

FIG. 10 is a perspective view of a heart valve holder of the present invention assembled to the inflow side of a tissue-type heart valve;

FIG. 11 is a plan view of the outflow end of the valve and holder of FIG. 10;

FIG. 12 is a cutaway perspective view of one of the commissures of the valve shown in FIG. 10;

FIGS. 13 and 14 are outflow plan and perspective views, respectively, of an alternative heart valve and holder of present invention;

FIGS. 15 and 16 are outflow plan and perspective views, respectively, of a further alternative heart valve and holder of present invention having a central upstanding member;

FIGS. 17A-17C are several views of the upstanding member of the holder of FIGS. 15 and 16;

FIG. 17D is a perspective view of an alternative upstanding member of the holder of FIGS. 15 and 16 having a triangular cross-section; and

FIGS. 18 and 19 are outflow plan and perspective views, respectively, of a still further alternative heart valve and holder of present invention having a hollow central upstanding member.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

The present invention provides an improved heart valve holder for tissue-type prosthetic heart valves that facilitates implantation and reduces the chance of suture entanglement. The holder of the present invention is particularly useful for prosthetic mitral heart valves having commissure posts on the outflow side supporting flexible leaflets therebetween. The mitral position is such that the outflow side (and commissure posts) projects distally toward the left ventricle during implantation, and thus the holder must be attached to the inflow (i.e., accessible) side of the valve. Delivery of the valve to the mitral position involves sliding the valve down a plurality or array of sutures that have been pre-installed around the annulus and then passed through the valve sewing ring. The holder of the present invention constricts the commissure posts radially inward and at the same time moves the flexible material upwards to form a steep angle thus helping to prevent the leading posts from becoming entangled in the array of pre-installed sutures. This benefit is thus especially advantageous where the outflow side and commissure posts of the heart valve extend distally during delivery, forming the leading end of the valve, which is the case in a prosthetic mitral valve implantation. Nonetheless, the holder of the present invention may prove useful for the implantation of heart valves in other than the mitral position, and thus the invention may be applicable thereto.

FIGS. 1A-LC illustrates several steps in an exemplary heart valve deployment process using a holder 20 of the present invention. The holder 20 is shown assembled to a flexible leaflet heart valve 22 having a sewing ring 24 and a plurality of commissure posts 26 that support leaflets of a tissue valve or a plurality of separate flexible leaflets. This particular valve 22 is intended for implant in the mitral annulus MA, between the left atrium LA and left ventricle LV. Blood flows from the left atrium LA along a flow axis through the valve 22 and into the left ventricle LV during the heart's diastolic phase, and therefore the commissure posts 26 project in an outflow direction.

FIG. 1A illustrates a plurality of implant sutures 28 that have been pre-threaded through the periphery of the mitral annulus MA and then through the sewing ring 24 of the valve 22. In the typical procedure, an array of implant sutures 28 is pre-threaded around the periphery of the mitral annulus MA and loose ends are removed from the surgical site to be threaded through the sewing ring 24 outside of the body. The valve 22 is then "parachuted" down the array of sutures until it rests on the annulus. A surgical handle 30

removably attaches to the holder 20 and facilitates manipulation and advancement of the holder/valve combination down the array of implant sutures 28.

As will be more clear from the later drawings and description, the holder 20 removably attaches to the valve 22 using a plurality of lengths of flexible material 32, first segments 34 of which are visible in FIG. 1A at the outflow end of the valve 22. The holder 20 further includes an upstanding or shaft member 36 that extends along the flow axis of the valve and displaces the first segments 34 into the tent configuration shown. The first segments 34 extend radially inward from the outflow end of commissure posts 26 to the flow axis. Tension in the first segments 34 pulls the commissure posts 26 inward and also moves the first segments 34 upwards to form a steep angle, thus helping to prevent entanglement of any of the commissure posts with the array of implant sutures 28.

FIG. 1B shows the holder 20 and valve 22 combination assembled with the sewing ring 24 seated on the mitral annulus MA. The surgical handle 30 detaches from the holder 20 by unscrewing or, preferably, along with a handle interface of the holder by severing a flexible thread, as will be described below.

Once the handle 30, preferably along with the handle interface 40, is removed to provide greater visibility, the surgeon ties off the implant sutures 28 and severs them close to the sewing ring 24 to secure the valve 22 in the annulus, as seen in FIG. 1C. The surgeon then detaches the holder 20 from the valve 22 by severing each of the lengths of flexible material 32. Each length of flexible material 32 is tied to the holder at both ends, and severing it in the middle, at a cutting groove in the holder, permits the holder with the lengths of flexible material attached, to be pulled free of the valve 22.

With reference to FIG. 2, the components of an exemplary holder 20 are shown exploded along with the prosthetic heart valve 22 and handle 30. The holder 20 comprises the aforementioned shaft member 36, a handle interface 40, and a valve abutment portion 42. Prior to a detailed discussion of these components, it will be seen that the heart valve 22 includes a generally annular sewing ring 24 on an inflow end and a plurality of commissure posts 26 on an outflow end. Flexible leaflets 44 provide occluding surfaces for the valve 22 and are supported by the commissure posts 26. Various flexible leaflet prosthetic heart valves are known and would benefit from deployment using the holder 20 of the present invention. Exemplary heart valves are the CARPENTIER-EDWARDS porcine and pericardial bioprostheses, sold by Edwards Lifesciences Corp. of Irvine, Calif. The surgical handle 30 is of a conventional type and includes a threaded boss 46 on its distal end.

The lengths of flexible material 32, typically suture material, which couple the holder 20 to the valve 22 are not illustrated in FIG. 2. More detailed discussions of the attachment of a holder to a heart valve using such suture material, and structure on the holder permitting rapid detachment, can be found in U.S. Pat. Nos. 4,865,600 and 6,409,758, both of which are expressly incorporated herein by reference.

With reference still to FIG. 2, the shaft member 36 possesses a generally tubular body 50 having notches 52 on a distal end and an outwardly extending flange 54 on a proximal end (in this sense, proximal corresponds to the inflow side of the valve 22 and distal to the outflow side). On one lateral side of the tubular body 50, a rail 56 extends axially from the flange 54 into proximity with the distal end, and is interrupted by a small gap 58. One or more cantilevered fingers 60 having outwardly projecting pawls 62 are

formed in the tubular body **50**. Each of the pawls **62** is on the proximal end of the respective finger **60**. In a preferred embodiment, there are at least two such fingers **60** and pawls **62**. The flange **54** includes at least one, and preferably at least two coupling holes **64** whose purpose will be explained below. The shaft member **36** further defines a bore or cavity **66** opening to its proximal end, the distal end being closed in the illustrated embodiment.

The handle interface **40** comprises a short tube **70** having an outer diameter that fits closely within the cavity **66** of the shaft member **36**. A proximal flange **72** extends outward from the tube **70** and preferably mirrors the shape of the flange **54** on the shaft member **36**. More particularly, both flanges **54**, **72** have two opposed arcuate edges and two straight edges therebetween so as to have a circular shape with opposed chordal cutouts. An internally threaded bore **74** extends through the tube **70** and opens at its proximal end to receive the threaded boss **46** of the surgical handle **30**. Coupling holes **76** are also provided in the flange **72** in the same number and pattern as the coupling holes **64** on the flange **54**. In addition an open slot **77** is provided between the coupling holes to facilitate severing a flexible attachment thread (described below).

The valve abutment portion **42**, also seen in the plan views of FIGS. **8** and **9**, includes a tubular body **80** defining therethrough a central bore **82**. An axial slot **84** opens in one side of the bore and is sized to receive the rail **56** of the shaft member **36**. A plurality, in this case three, sewing ring brackets **86** extend outward from the tubular body **80**. Each bracket **86** has a radially-extending portion **88** with a pair of through holes **90** formed therein and an axially-extending portion **92**. The generally right angle combinations of the three radially-extending portions **88** and axially-extending portions **92** contact the sewing ring **24** of the valve **22**, with the portions **92** projecting within the annular sewing ring to accurately center the valve **22** in the holder **42**. A pair of ears **94** project in a proximal direction from the tubular body **80** on opposite lateral sides of the central bore **82**. These ears **94** each include an upper flange (not numbered) that provides structure for retaining a protective assembly **102** including a disk-shaped clip **104** and cage **106** (shown in FIGS. **4A-4B**) on the holder **20**. The cage **106** snaps on to the clip **104** and provides protection for the valve **22** during storage, transport, and handling in the operating room prior to implantation. The assembly **102** of the clip **104** and cage **106** also provides a means of grasping the complete unit in one hand while deploying the holder with the other hand. In addition the perforated cage **106** can potentially act as a rinsing cage protecting the valve during the operating room rinsing procedure.

Detailed operation of the valve holder **20** of the present invention will now be described with respect to FIGS. **3A-3D**, **4A-4B**, and **5A-5D**.

FIGS. **3A**, **4A**, and **5A** illustrate the holder **20** assembled and prior to actuation of the shaft member **36** to constrict the valve commissure posts **26** and move the attachment flexible material to a steep angle. Referring to FIG. **2**, in the assembled state of the holder **20**, the tubular body **50** of the shaft member **36** fits concentrically within the bore **82** of the valve abutment portion **42**, and the tube **70** of the handle interface **40** extends into the bore **66** of the shaft member. The flange **72** of the handle interface **40** matches up with the flange **54** of the shaft member **36**, such that the coupling holes **64**, **76** line up. FIGS. **3A** and **3B** show a coupling suture thread **100** initially tied to interface **40** via hole **76a** and crossed over slot **77** to hole **76b**. The thread **100** extends through aligned holes **76b** and **64**, and ties off again at hole

76a. The thread **100** can be severed with a scalpel in slot **77**. This configuration removably attaches the handle interface **40** to the shaft member **36**, and because the handle **30** threads into the bore **74**, the handle is removably attached to the shaft member (indeed, the handle is removably attached in two ways to the shaft member, by threading and by the quick release thread). In the position shown in FIG. **3A**, the shaft member **36** is constrained axially with respect to the valve abutment portion **42** by interaction of the gap **58** in the rail **56** (see FIG. **2**) with an internal shoulder (not numbered) in the valve abutment portion bore **82**. The internal shoulder projects into the gap **58** and because the rail **56** extends on either side of the shoulder the shaft member **36** is constrained from moving axially in either direction (but is not entirely constrained from rotational movement).

FIG. **3A** best illustrates the attachment of the holder **20** to the heart valve **22** using the lengths of flexible material **32**. As mentioned, the lengths of flexible material **32** may be sutures, and they pass through suture-permeable portions of the valve **22**, such as through an outer fabric covering. Each length of flexible material **32** extends through the valve **22** and the two holes **90** of the sewing ring bracket **86**. More specifically, each length of flexible material **32** is tied at one end to a first sewing ring bracket hole **90** and extends axially through the corresponding commissure posts **26** of the valve **22**, preferably crossing over as it does. The first segments **34** of the lengths of flexible material **32** extend radially inward from a distal tip of one of the commissure posts **26** to a central location generally along the flow axis of the valve **22**, and from there radially outward to a second commissure post. The flexible material **32** then extends axially through the second commissure post **26** and through a hole **90** in a second sewing ring bracket **86**, where it is tied off. In the tri-leaflet valve **22** shown, there are three lengths of flexible material **32** that each extend between two of the commissure posts **26**, and therefore the first segments **34** are arranged between the distal tips of the commissure posts as shown in FIG. **3A**. These three segments **34** are arranged generally in a plane between the commissure posts **26**, and though tautly threaded through the valve **22** they do not pull the commissure posts **26** inward to any great degree so that the valve can be in a relaxed state during a potentially long storage period.

FIGS. **4A-4B** show a protective transport cage **102** in cross-section coupled to the disk **104**. The transport cage **102** comprises a generally circular disk portion **104** and a tubular cage portion **106**. The disk portion **104** includes a central opening and a lateral cutout (not shown) enabling it to be coupled to the valve abutment portion **42**, and specifically to the ears **94** thereof. The cage portion **106** couples to and extends axially from a periphery of the disk portion **104**, and generally surrounds and protects the valve **22** when assembled with the holder **20**. Although not shown, the cage portion **106** includes a number of perforations or cutouts so that the valve **22** may be effectively rinsed while the transport cage **102** remains in place. That is, the assembly shown in FIG. **4A** minus the attached surgical handle **30** is that which is packaged for storage by the manufacture. The transport cage **102** remains in place during storage, transport, and subsequent deployment. It may also remain in place during rinsing by the surgical staff. The transport cage **102** functions much like the "rinse cage" disclosed in U.S. Pat. No. 6,416,547, the disclosure of which is expressly incorporated herein by reference.

FIGS. **3B** and **5B** show the assembled holder **20** after rotation of the shaft member **36** in the clockwise direction of the arrow **103** in FIG. **3B**. The handle **30** rotates in the same direction as shown, and is used to turn the shaft member **36**

after it has been fully threaded into the handle interface 40. The total extent of rotation is less than 45°. Once rotated, the axial rail 56 on the shaft member 36 lines up with the axial slot 84 in the valve abutment portion 42. The shaft member 36 is thus in a “first position” with respect to the valve abutment portion 42, which is to say that it is retracted in a proximal direction. In the first position the distal tip of the shaft member 36 is located to the inflow side of the valve leaflets 44. The “first position” as used in the appended claims could also refer to the slightly rotated position shown in FIG. 3A, the position being in reference to the relative axial position of the shaft member 36 with respect to the valve abutment portion 42 (or valve 22, for that matter). The reader will note in FIG. 3B that the cantilevered pawl 62 is located proximally with respect to the valve abutment portion 42.

FIGS. 1A-1C show commissure posts 26 pulled inward or constricted radially and the first segments 34 move to a steep angle position by deploying the holder 20. This step should be accomplished prior to threading the loose implant sutures 28 through the sewing ring 24. In the illustrated embodiment, the commissure posts 26 are pulled inward upon distal displacement of the shaft member 36 from a first position to a second position with respect to the valve abutment portion 42. In addition first segments 34 move to a steep angle position.

FIGS. 3C, 4B, and 5C show the shaft member 36 displaced to its second position with the first segments 34 moved to a steep angle position and the commissure posts 26 pulled inward. The shaft member 36 includes the aforementioned notches 52 at its outflow or distal end that engage and capture the first segments 34 of the lengths of flexible material 32. The notches 52 are preferably radially spaced 120° apart so as to accept and capture the similarly arrayed first segments 34. As the shaft member 36 moves from its proximal, first position to its distal, second position it pushes through the valve leaflets and displaces the first segments 34 in a distal direction creating greater tension in the lengths of flexible material 32, pulling the commissure posts 26 radially inward and moving first segments 34 to a steep angle. After a certain amount of axial travel of the shaft member 36, the pawls 62 spring outward from within the bore 82 of the valve abutment portion 42, as seen in FIG. 5C. The pawls 62 therefore restrain the shaft member 36 in its second position with respect to the valve abutment portion 42. In the second position the distal tip of the shaft member 36 is located to the outflow side of the valve leaflets.

The commissure posts 26 start from a relatively straight orientation seen in FIG. 4A, having a spacing S_1 (it will be understood that a true radial cross-section through the center of the valve 22 will not cross two commissure posts 26, and thus the cross-sectional view is in two planes). After movement of the shaft member 36 to its second position, the commissure posts 26 have a spacing S_2 seen in FIG. 4B. In a preferred embodiment, the range ratio of the spacing S_2 to S_1 is about 50 to 60%.

In its second position, the shaft member 36 creates a tent of sorts with the first segments 34, as seen in FIG. 5C. Desirably, the distal tip of the shaft member 36 extends a distance A past the tips of the commissure posts 26, such that the first segments 34 assume an angle α with respect to a radial plane 110. Preferably, the distance A range is about 9 mm, and the angle α is about 40°. This final configuration of the holder 20 just prior to implantation of the valve 22 helps prevent implant suture looping around the commissure posts 26 in three ways. First of all, the commissure posts 26 are pulled inward which reduces their radial profile and thus

reduces the likelihood of looping one of the implant sutures around one of the posts. Secondly, the tautly strung first segments 34 extending at an angle α as shown in FIG. 5C together form a conical deflection barrier of sorts guiding the implant sutures around commissure posts 26. Thirdly, the distal tip of the shaft member 36 is relatively broad which fills some of the space between the commissure posts 26 and further helps prevent looping.

FIG. 5C shows detachment of the surgical handle 30 along with the handle interface 40 from the holder 20, while FIG. 3D shows the remaining holder 20 coupled to the valve 22. The ability to quickly release the handle 30 from holder 20 by severing the coupling suture thread 100 is a great advantage to the surgeon after seating the valve 22 in the mitral annulus MA, such as seen in FIG. 1B. After removing the handle 30 with handle interface 40 and thread 100, the surgeon has much greater visibility to tie off the loose implant sutures 28. The shaft member 36 remains in its second position due to engagement of the pawls 62 with the valve abutment portion 42.

Finally, FIG. 5D illustrates removal of the holder 20 from the valve 22 by severance of a mid-portion of each of the lengths of flexible material 32. Because at least one free end of the lengths of flexible material 32 is tied to the valve abutment portion 42, the surgeon can easily pull the holder 20 from engagement with the valve 22. That is, the lengths of flexible material 32, which may be sutures, easily slide through the suture-permeable material of the valve 22. It should be noted that the ears 94 on the valve abutment portion 42 are convenient for use in gripping the holder 20 with forceps or the like.

FIGS. 6A and 6B are plan views of the outflow end of the valve 22 both before and after actuation of the shaft member 36. The first segments 34 of the lengths of flexible material 32 are shown thicker in FIGS. 6A and in the enlarged view of FIG. 7, and illustrate the interaction between them along the flow axis. That is, the three first segments 32 mutually cross over one another so that they meet along the flow axis. Because of this mutual interaction, all three first lengths 32 are located at the proper position for engagement with the shaft member 36. FIG. 6B shows the radially directed notches 52 receiving the three pairs of the first segments 32.

With reference to FIG. 10 an alternative exemplary holder 120 of the present invention is shown attached to a tissue-type heart valve 122. The heart valve 122 includes an annular sewing ring 124 on an inflow side, and a plurality of commissure posts 126 projecting generally axially in the outflow direction. The holder 120 attaches to the sewing ring 124 on the inflow side of the valve 122, which also is the proximal (i.e., accessible) side during implantation. That is, the commissure posts 126 project distally toward the outflow side of the valve 122, defining the leading end of the valve during implantation.

The heart valve 122 further includes a plurality of flexible leaflets 128 that are supported by and extend between the commissure posts 126. The leaflets 128 provide the occluding surfaces of the valve 122, and may be made of individual pieces of bovine pericardium, for example. Alternatively, the leaflets 128 may be part of an entire xenograft, or homograft. In the former instance, natural porcine (pig) valves are particularly useful. Therefore it should be understood that the leaflets 128 may be formed of a variety of materials, none of which is limiting with respect to the present invention. In addition, there are preferably three such leaflets 128 corresponding to three commissure posts 126.

Various constructions for the heart valve 122 are known, which may include metallic or plastic stent elements, a

silicone or urethane insert for the sewing ring **124**, biocompatible fabric (i.e., polyester) covering around one or more of the elements, etc. In a preferred embodiment, the heart valve **122** includes an internal metallic wireform (not shown) having an undulating shape with a plurality of arcuate cusps connected by upstanding commissures. The wireform commissures provide internal structure for the commissure posts **126** of the valve, and are somewhat flexible so as to be able to flex or cantilever inward. The holder **120** of the present invention facilitates this flexing, though the invention may be practiced in its broadest sense without causing inward movement of the commissure posts. It should be noted that other internal constructions of heart valve **122** having movable commissure posts are available with which the holder **120** of the present invention may function equally as well.

An exemplary holder **120** of the present invention includes a rigid structure of three relatively movable elements. A plate-like valve abutment portion **140** lies against the inflow side of the sewing ring **124** and includes a plurality of through holes around its periphery. A plate-like commissure adjusting portion **144** generally mirrors the shape of the valve abutment portion **140**, and also includes a plurality of peripheral through holes **146**. The adjusting portion **144** further includes a centrally located and internally threaded boss **148** that projects in a proximal direction from the otherwise generally planar adjusting portion. Finally, an adjusting member **150** having external threads thereon is sized to mate with the internal threads of the boss **148**. It should be understood that the function of the holder **120** in constricting the valve commissures may be accomplished with different structures than the one shown.

A plurality of lengths of flexible material **160** is shown in FIGS. **10-12** partly extending between the tips **162** of the commissure posts **126**. In the preferred embodiment, the lengths of flexible material **160** comprise mono- or poly-filament sutures, and that exemplary nomenclature will be used herein. Because there are three commissure posts **126**, there are at least three lengths of sutures **160** extending therebetween in an equilateral triangular configuration. Each length of suture **160** includes a first segment **161** spanning between two of the commissure posts **126**. Second segments **163** of each length of suture **160** extend axially in a proximal direction from the tips **162** and along the post **126**, the segments passing through the sewing ring **124** and attaching to the holder **120**. This is seen best in the perspective view of FIG. **10**. Specifically, both second segments **163** pass through the holes in the valve abutment portion **140** and attach to the adjusting portion **144** at discrete attachment points, for example by tying the free ends of each suture. In this manner, each length of suture **160** may be severed close to one of its points of attachment to the adjusting portion **144** and pulled free of the valve **122** along with the holder **120** by virtue of its remaining attachment point. Further specifics of this arrangement can be seen in U.S. Pat. No. 6,409,758, the disclosure of which is expressly incorporated herein by reference.

As mentioned, the abutment portion **140**, adjusting portion **144**, and adjusting member **150** are relatively movable. That is, the adjusting member **150** is adapted to cause relative axial displacement between the abutment portion **140** and the adjusting portion **144** (preferably by connecting a handle **152** thereto). Because the abutment portion **140** remains against the sewing ring **124**, the adjusting portion **144** translates proximally away from the abutment portion, and attached valve **122**. Because the lengths of suture **160** attach to the adjusting portion **144**, they are also pulled in the

proximal direction. Moreover, because the first segment **161** of each length of suture **160** spans between two of the commissure posts **126**, proximal movement of the adjusting portion **144** and attached second segments **163** causes radially inward movement of the tips **162**, with the commissure posts **126** generally flexing inward from their structural point of attachment within the valve **122** adjacent the sewing ring **124**.

It should be clearly understood that the inward flexing of the commissure post tips **162** reduces the chance of suture looping around the tips, but that certain aspects of the present invention reduce suture looping even without tip flexing. That is, the lengths of suture **160** may attach to the rigid structure of a holder that simply abuts the valve, without the relatively moving elements that cause commissure deflection.

With reference to FIGS. **10-12**, the arrangement of the discrete lengths of sutures **160** will now be described. There are desirably three equal lengths of suture **160**, each secured at its two free ends to the adjusting portion **144**. As mentioned, the second segments **163** pass through the aligned holes **146** in the adjusting portion **144** and abutment portion **140**, and then through the sewing ring **124** to a first commissure post **126**. From there, the second segments **163** continue generally axially to the tips **162** of adjacent commissure posts **126**, and the first segment **161** spans obliquely across the outflow side of the valve **122** structurally coupling the two tips. It should be noted that each of the commissure posts **126** desirably has a fabric covering, and the lengths of suture **160** pass at least once through the fabric covering at the tip **162** or along each post **126**. For example, FIG. **12** shows the first segments **161** passing below the fabric covering at the tip **162**, and FIG. **10** shows the second segments **163** threading at least once through the fabric. This threaded path guides the lengths of suture **160** along their predetermined paths. It is a simple matter to remove the lengths of suture **160** from the valve **122** along with the holder by pulling them free from the fabric cover.

As seen best in FIGS. **11** and **12**, the first segment **161** of each length of suture **160** extends from a circumferential side of the respective commissure post tip **162** that is farthest away from the destination tip. That is, three lengths of sutures **160a**, **160b**, **160c** are seen in FIG. **11** extending between three commissure post tips **162a**, **162b**, **162c**, using a clockwise nomenclature. The first segment **161** of the first length of suture **160a** extends from a counter-clockwise side of the first commissure post tip **162a** to a clockwise side of the second suture post tip **162b**. The other two lengths of sutures are arranged accordingly such that each two adjacent lengths of suture cross over (i.e., intersect) just prior to being threaded into (i.e., just radially inward from) the respective commissure post tips **162**. This intersection of the sutures **160** defines a plane or slide closely adjacent to each commissure post tip **162**. The plane or slide formed by the crossed sutures **160** helps prevent suture looping because a barrier of sorts is provided that guides loose sutures over each post tip **162**.

As seen in FIG. **10**, the second segment **163** of each length of suture **160** continues axially along the respective commissure posts **126** and may be threaded into and out of the cloth covering thereover. Desirably, a second crossover of the second segments **163** is provided in the commissure posts **126** to insure that each end is secured to the adjusting portion **144** in the proper orientation. As seen in FIG. **10**, therefore, the length of suture **160** that is seen extending between the two visible commissure posts **126** extends upward through the valve **122** and holder **120** to emerge

15

from the closest aligned holes **146** (as shown) and be secured in the cutting guide. This dual crossover thus helps a surgeon identify which lengths of sutures **160** extend between which commissure posts **126**.

FIGS. **13** and **14** illustrate a second embodiment of heart valve holder of the present invention for preventing suture looping which also provides a planar guard over the commissure tips, similar to the crossed-over lengths of filament-like material of FIGS. **10-12**. In general, the holder of FIGS. **13-14** is identical to the holder described above, with the substitution of flexible bands **170a**, **170b**, **170c** instead of lengths of suture **160**. The bands **170** may be made of polyester tape, or other suitable biocompatible material similar to sutures. In one embodiment, the bands **170** are substantially wider than they are thick (e.g., formed in a tape or flat strip), and desirably have a width that is approximately equal to the circumferential width of the each of the commissure post tips **162**.

As seen best in FIG. **14**, first segments **172** of the bands **170** extend between the commissure post tips **162** in a flattened configuration and cross over each adjacent band at or slightly inward from the tip. After extending to the outside of the commissure post tip **162**, each band **170** is folded, twisted, or otherwise narrowed into second segments **174** to pass through one or more fabric tunnels **176** along the commissure posts **126**. Ultimately, each narrowed second segment **174** passes through aligned holes in the abutment portion **140** and adjusting portion **144** and is secured to the adjusting portion, as described above. The mechanism for the holder **120** of FIGS. **13-14** is similar to that described above in that separation of the abutment portion **140** and adjusting portion **144** pulls the narrowed second segments **174** of the bands **170** to shorten the flattened first segments **172** between the commissure post tips **162**. As each second segment **174** is pulled, the first segment **172** follows and is folded or otherwise narrowed as it passes through the fabric cover of the commissure post **126**. Moreover, when the holder is removed, one of the second segments **174** of each band **170** is severed close to its point of attachment to the holder and the band **170** may then be pulled free from the valve by virtue of its remaining attachment to the holder. In this regard, the bands **170** may be TEFLON (PTFE) to facilitate sliding through the fabric tunnels in the valve.

Because of the flattened or otherwise planar configuration of the bands **170**, suture looping around the commissure post tips **162** is greatly reduced. That is, sutures that contact the bands **170** will be guided over and to the outside of each commissure post tip **162**. The bands **170** provide slides of sorts that guide the loose sutures over the commissure post tips **162**, and in the preferred embodiment, the bands completely cover the tips to present a smooth, even surface.

FIGS. **15-17** illustrate a further embodiment of a heart valve holder for preventing suture looping. As seen best in FIG. **16**, a plurality of lengths of sutures **180** extends between the commissure post tips **162** across the outflow side of the valve as before, although first to a central upstanding member **182** elevating the lengths of sutures above the commissure post tips. The upstanding member **182** has an upper end **184** with a plurality of grooves or notches therein through which the lengths of suture **180** are threaded. Although the upstanding member **182** is shown as being elevated axially beyond the commissure post tips **162**, some of the benefits of reduced suture looping may be realized if the member has the same axial height as the post tips.

An exemplary embodiment of the upstanding member **182** is illustrated in FIGS. **17A-17C**. The member **182**

16

includes a wide base **186** and a narrow shaft **188** terminating in the upper end **184**. Three generally radial grooves **190** are formed in the upper end **184** distributed about 120° with respect to each other. These grooves **190** are each aligned with one of the commissure post tips **162** to receive a length of suture **180** extending therefrom. A lower pin **192** in the upstanding member **182** fits within a central bore provided in the center of the abutment portion **140**. Alternatively, the upstanding member **182** may be integrally molded with the abutment portion **140**. The wide base **186** strengthens the upstanding member **182**, and the shaft **188** has a length that projects axially above the commissure posts **126**.

As seen in FIG. **16**, threading the lengths of suture **180** through the grooves **190** in the upper end **184** of the upstanding member **182** provides a tent of sorts. This suture tent helps to prevent suture looping around the commissure post tip **162**. That is, errant sutures that contact any of the angled lengths of suture **180** are guided up and over the nearest commissure post tip **162**.

An alternative embodiment of an upstanding member **182'** is illustrated in FIG. **17D**. As in the earlier embodiment, the member **182'** includes a wide base **186'** and a narrow shaft **188'** terminating in an upper end **184'** having three generally radial grooves **190'** distributed about 120° with respect to each other. The shaft **188'** has a triangular as opposed to circular cross-section so as to better mate with the surrounding leaflets in the assembly of the valve and holder. That is, the three leaflets come together in an equilateral triangle, desirably at the axis of the valve, and the upstanding member **182'** will be oriented such that the corners of the triangular shaft **188'** project toward each valve commissure, thus bifurcating two leaflets. In this way the midpoint of each leaflet free edge abuts the flat sides of the shaft **188'**, minimizing any deformation of the leaflet at that midpoint from the extended contact with the shaft **188'** during long term storage in a preservative solution.

FIGS. **18** and **19** illustrate a further heart valve holder of the present invention that also makes use of a central upstanding member **200**, although the member is hollow and the lengths of suture **202** extend axially through the member to be connected to either the abutment portion **140** or adjustment portion **144**. The lengths of suture **202** may be filaments or strands, or may be wider bands as described above with respect to FIGS. **13-14**. The upstanding member **200** maybe a hollow tubular structure fastened within or molded with the abutment portion **140**. Again, the axial height of the upstanding member **200** is greater than the axial height of the commissure posts **126** such that the lengths of suture **202** are tented across the outflow end of the valve.

It will also be appreciated by those of skill in the relevant art that various modifications or changes may be made to the examples and embodiments of the invention described in this provisional application, without departing from the intended spirit and scope of the invention. In this regard, the particular embodiments of the invention described herein are to be understood as examples of the broader inventive concept disclosed in this application.

What is claimed is:

1. A holder for a flexible leaflet prosthetic heart valve that helps prevent suture looping, the heart valve having an inflow end and an outflow end and a flow axis therebetween, the valve including a plurality of generally axially-extending commissure posts circumferentially-spaced around the outflow end that support occluding flexible leaflets of the valve, the holder comprising:

17

a valve abutment portion that contacts the inflow end of the valve;

a member coupled to the valve abutment portion and extending therefrom along the flow axis to a distal tip of the member on the outflow side of the leaflets; and

a plurality of lengths of flexible material each having first segments angled in the outflow direction from the commissure posts to the distal tip of the member in a tent configuration to help prevent suture looping during implant.

2. The holder of claim 1, wherein each first segment of the lengths of flexible material is angled in the outflow direction about 40° with respect to a radial plane.

3. The holder of claim 1, wherein the member is axially movable relative to the valve abutment portion between a first position wherein the distal tip of the member is located to the inflow side of the leaflets, and a second position wherein the distal tip is located to the outflow side of the leaflets.

4. The holder of claim 1, wherein the valve is of the type that has three leaflets and three commissure posts, and in the first position of the member each first segment extends radially inward and mutually crosses over the other two first segments to retain the point at which they cross over along the flow axis of the valve.

5. The holder of claim 1, wherein the member is solid and includes notches on its distal tip for capturing and retaining midpoints of the first segments of the lengths of flexible material, each first segment angling from one of the commissure posts radially inward to the distal tip of the member and then radially outward to an adjacent commissure post via a notch in the distal tip.

6. The holder of claim 5, wherein each length of flexible material axially extends in second segments along two adjacent commissure posts and attaches to the valve abutment portion at two points such that each length may be severed close to one of its points of attachment to the valve abutment portion and pulled free of the valve along with the valve abutment portion by virtue of its remaining attachment point.

7. The holder of claim 1, further including a generally radially extending clip adapted to removably attach to the valve abutment portion and a generally tubular cage that snaps on to the clip and surrounds the valve to provide protection for the valve during storage, transport, and handling prior to implantation.

8. The holder of claim 7, wherein the cage is perforated to permit rinsing of the valve prior to removal of the cage from the clip.

9. A method for delivering a flexible leaflet prosthetic heart valve and preventing suture looping, comprising:

providing a flexible leaflet prosthetic heart valve and holder combination, the heart valve having an inflow end and an outflow end and a flow axis therebetween, the valve including a plurality of generally axially-extending commissure posts circumferentially-spaced around the outflow end that support occluding flexible leaflets of the valve, the holder being releasably attached at the inflow end of the valve with a plurality of lengths of flexible material each passing through the valve and having two first segments that each extend radially inward from a commissure post to the flow axis, the holder having a member that is axially movable relative to the valve along the flow axis between a first position and a second position displaced from the first position in the outflow direction, the member having a distal tip; and

18

axially displacing the member from the first position to the second position so that the member distal tip passes from the inflow to the outflow side of the flexible leaflets of the valve and engages the first segments of the plurality of lengths of flexible material so that they are angled in the outflow direction from the commissure posts to the distal tip of the member and help prevent suture looping during implant.

10. The method of claim 9, wherein the valve is of the type that has three leaflets and three commissure posts, and in the first position of the member the first segments of each length of flexible material extends radially inward and mutually crosses over the other two first segments to retain the point at which they cross over along the flow axis of the valve, the member including at least one notch on its distal tip and the method including capturing the first segments in the notch when axially displacing the member from the first position to the second position.

11. The method of claim 9, wherein the commissure posts are flexible, the method further including pulling the commissure posts radially inward when axially displacing the member from the first position to the second position.

12. The method of claim 11, wherein the method includes pulling the commissure posts radially inward such that the diameter of a circle defined by tips of the pulled in commissure posts reduces to about 50-60% of a circle defined by the commissure post tips before being pulled inward.

13. The method of claim 9, wherein the holder includes a valve abutment portion that contacts the inflow end of the valve, and the holder includes structure that prevents axial displacement of the member from its first position with respect to the valve abutment portion.

14. The method of claim 13, further including preventing rotation of the member with respect to the valve abutment portion when axially displacing the member from the first position to the second position.

15. The method of claim 9, further including locking the member in its second position.

16. The method of claim 9, wherein the holder includes a valve abutment portion that contacts the inflow end of the valve and a handle interface attached to the valve abutment portion with at least one thread, the handle interface having structure for coupling to a surgical delivery handle, the method including quickly releasing the handle interface and coupled surgical delivery handle from the valve abutment portion by severing the thread.

17. A system for holding a flexible leaflet prosthetic heart valve, the heart valve having an inflow/proximal end and an outflow/distal end and a flow axis therebetween, the valve including a plurality of generally axially-extending commissure posts circumferentially-spaced around the outflow end that support occluding flexible leaflets of the valve, the system comprising:

a surgical delivery handle having a distal threaded end; and

a holder comprising a valve abutment portion that contacts the inflow end of the valve, and a handle interface having threading for coupling to the distal threaded end of the surgical delivery handle, the handle interface being coupled to the valve abutment portion with quick release structure to permit quick release of the handle interface and coupled surgical delivery handle from the valve abutment portion without having to unscrew the surgical delivery handle,

wherein the quick release structure comprises at least one thread coupling the handle interface and the valve abutment portion, wherein the handle interface and

19

coupled surgical delivery handle are released from the valve abutment portion upon severing the thread.

18. A system for holding a flexible leaflet prosthetic heart valve, the heart valve having an inflow/proximal end and an outflow/distal end and a flow axis therebetween, the valve including a plurality of generally axially-extending commissure posts circumferentially-spaced around the outflow end that support occluding flexible leaflets of the valve, the system comprising:

a surgical delivery handle having a distal threaded end;

a holder comprising a valve abutment portion that contacts the inflow end of the valve, and a handle interface having threading for coupling to the distal threaded end of the surgical delivery handle, the handle interface being coupled to the valve abutment portion with quick release structure to permit quick release of the handle interface and coupled surgical delivery handle from the valve abutment portion without having to unscrew the surgical delivery handle;

a plurality of lengths of flexible material secured to the valve abutment portion and passing through the valve to cross over the outflow end of the valve from the commissure posts to a location along the flow axis and help prevent suture looping during implant; and

a member coupled to the valve abutment portion and extending therefrom along the flow axis to a distal tip on the outflow side of the leaflets, the distal tip engaging the plurality of lengths of flexible material to angle

20

them in the outflow direction from the commissure posts to the distal tip of the member in a tent configuration to help prevent suture looping during implant, wherein the member couples between the valve abutment portion and the handle interface.

19. The system of claim **18**, wherein the valve abutment portion comprises a tubular body defining a bore for receiving the member and the member defines a bore for receiving the handle interface.

20. The system of claim **19**, wherein the member comprises a generally tubular body and an outwardly extending flange on a proximal end of the body, and the handle interface comprises a generally tubular body and an outwardly extending flange on a proximal end, wherein the handle interface tubular body fits concentrically within the member tubular body and both flanges include coupling holes that align for passage of at least one coupling thread.

21. The system of claim **19**, wherein the member is axially movable relative to the valve abutment portion between a first position wherein the distal tip of the member is located to the inflow side of the leaflets, and a second position wherein the distal tip is located to the outflow side of the leaflets.

22. The system of claim **21**, wherein the member comprises a generally tubular body having structure for axially restraining the member in the second position with respect to the valve abutment portion.

* * * * *