



US00RE47124E

(19) **United States**  
(12) **Reissued Patent**  
**Blomberg et al.**

(10) **Patent Number:** **US RE47,124 E**  
(45) **Date of Reissued Patent:** **Nov. 13, 2018**

(54) **AUTOMATED FLUID HANDLING SYSTEM**

(71) Applicant: **GE Healthcare Bio-Sciences AB**,  
Uppsala (SE)

(72) Inventors: **Johan Blomberg**, Uppsala (SE); **Mats Lundkvist**, Uppsala (SE)

(73) Assignee: **GE Healthcare Bio-Science AB**,  
Uppsala (SE)

(21) Appl. No.: **15/008,155**

(22) Filed: **Jan. 27, 2016**

**Related U.S. Patent Documents**

Reissue of:

(64) Patent No.: **8,821,718**  
Issued: **Sep. 2, 2014**  
Appl. No.: **13/376,929**  
PCT Filed: **Jun. 4, 2010**  
PCT No.: **PCT/SE2010/050624**  
§ 371 (c)(1),  
(2) Date: **Dec. 8, 2011**  
PCT Pub. No.: **WO2010/144037**  
PCT Pub. Date: **Dec. 16, 2010**

(30) **Foreign Application Priority Data**

Jun. 9, 2009 (SE) ..... 0950431

(51) **Int. Cl.**  
**B01D 35/00** (2006.01)  
**G01N 35/10** (2006.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... **G01N 35/1097** (2013.01); **B01D 15/10**  
(2013.01); **B01D 29/60** (2013.01);  
(Continued)

(58) **Field of Classification Search**  
CPC .... G01N 35/1097; G01N 30/38; G01N 30/24;  
G01N 30/88; G01N 2030/8804;  
(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,044,593 A 8/1977 Haruki et al.  
4,125,464 A \* 11/1978 Burger et al. .... 210/658  
(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 2567575 Y 8/2003  
CN 101358952 A 2/2009  
(Continued)

**OTHER PUBLICATIONS**

“Manual ADI 2040 Process Analyzer” 1999-2007, Applikon Analytical B.V., pp. 1-134 (part 1).  
(Continued)


*Primary Examiner* — Ling X Xu

(74) *Attorney, Agent, or Firm* — Arent Fox LLP

(57) **ABSTRACT**

Automated fluid handling system comprising a housing (20) and two or more fluid handling units (26) arranged as interchangeable modular components with an external fluidics section (30) and an internal non fluidics section (32), and wherein the housing (20) comprises a liquid handling panel (22) with two or more of component positions for receiving said interchangeable modular components (26) such that the external fluidics section (30) is separated from the non fluidics section (32) by the liquid handling panel (22).

**29 Claims, 10 Drawing Sheets**

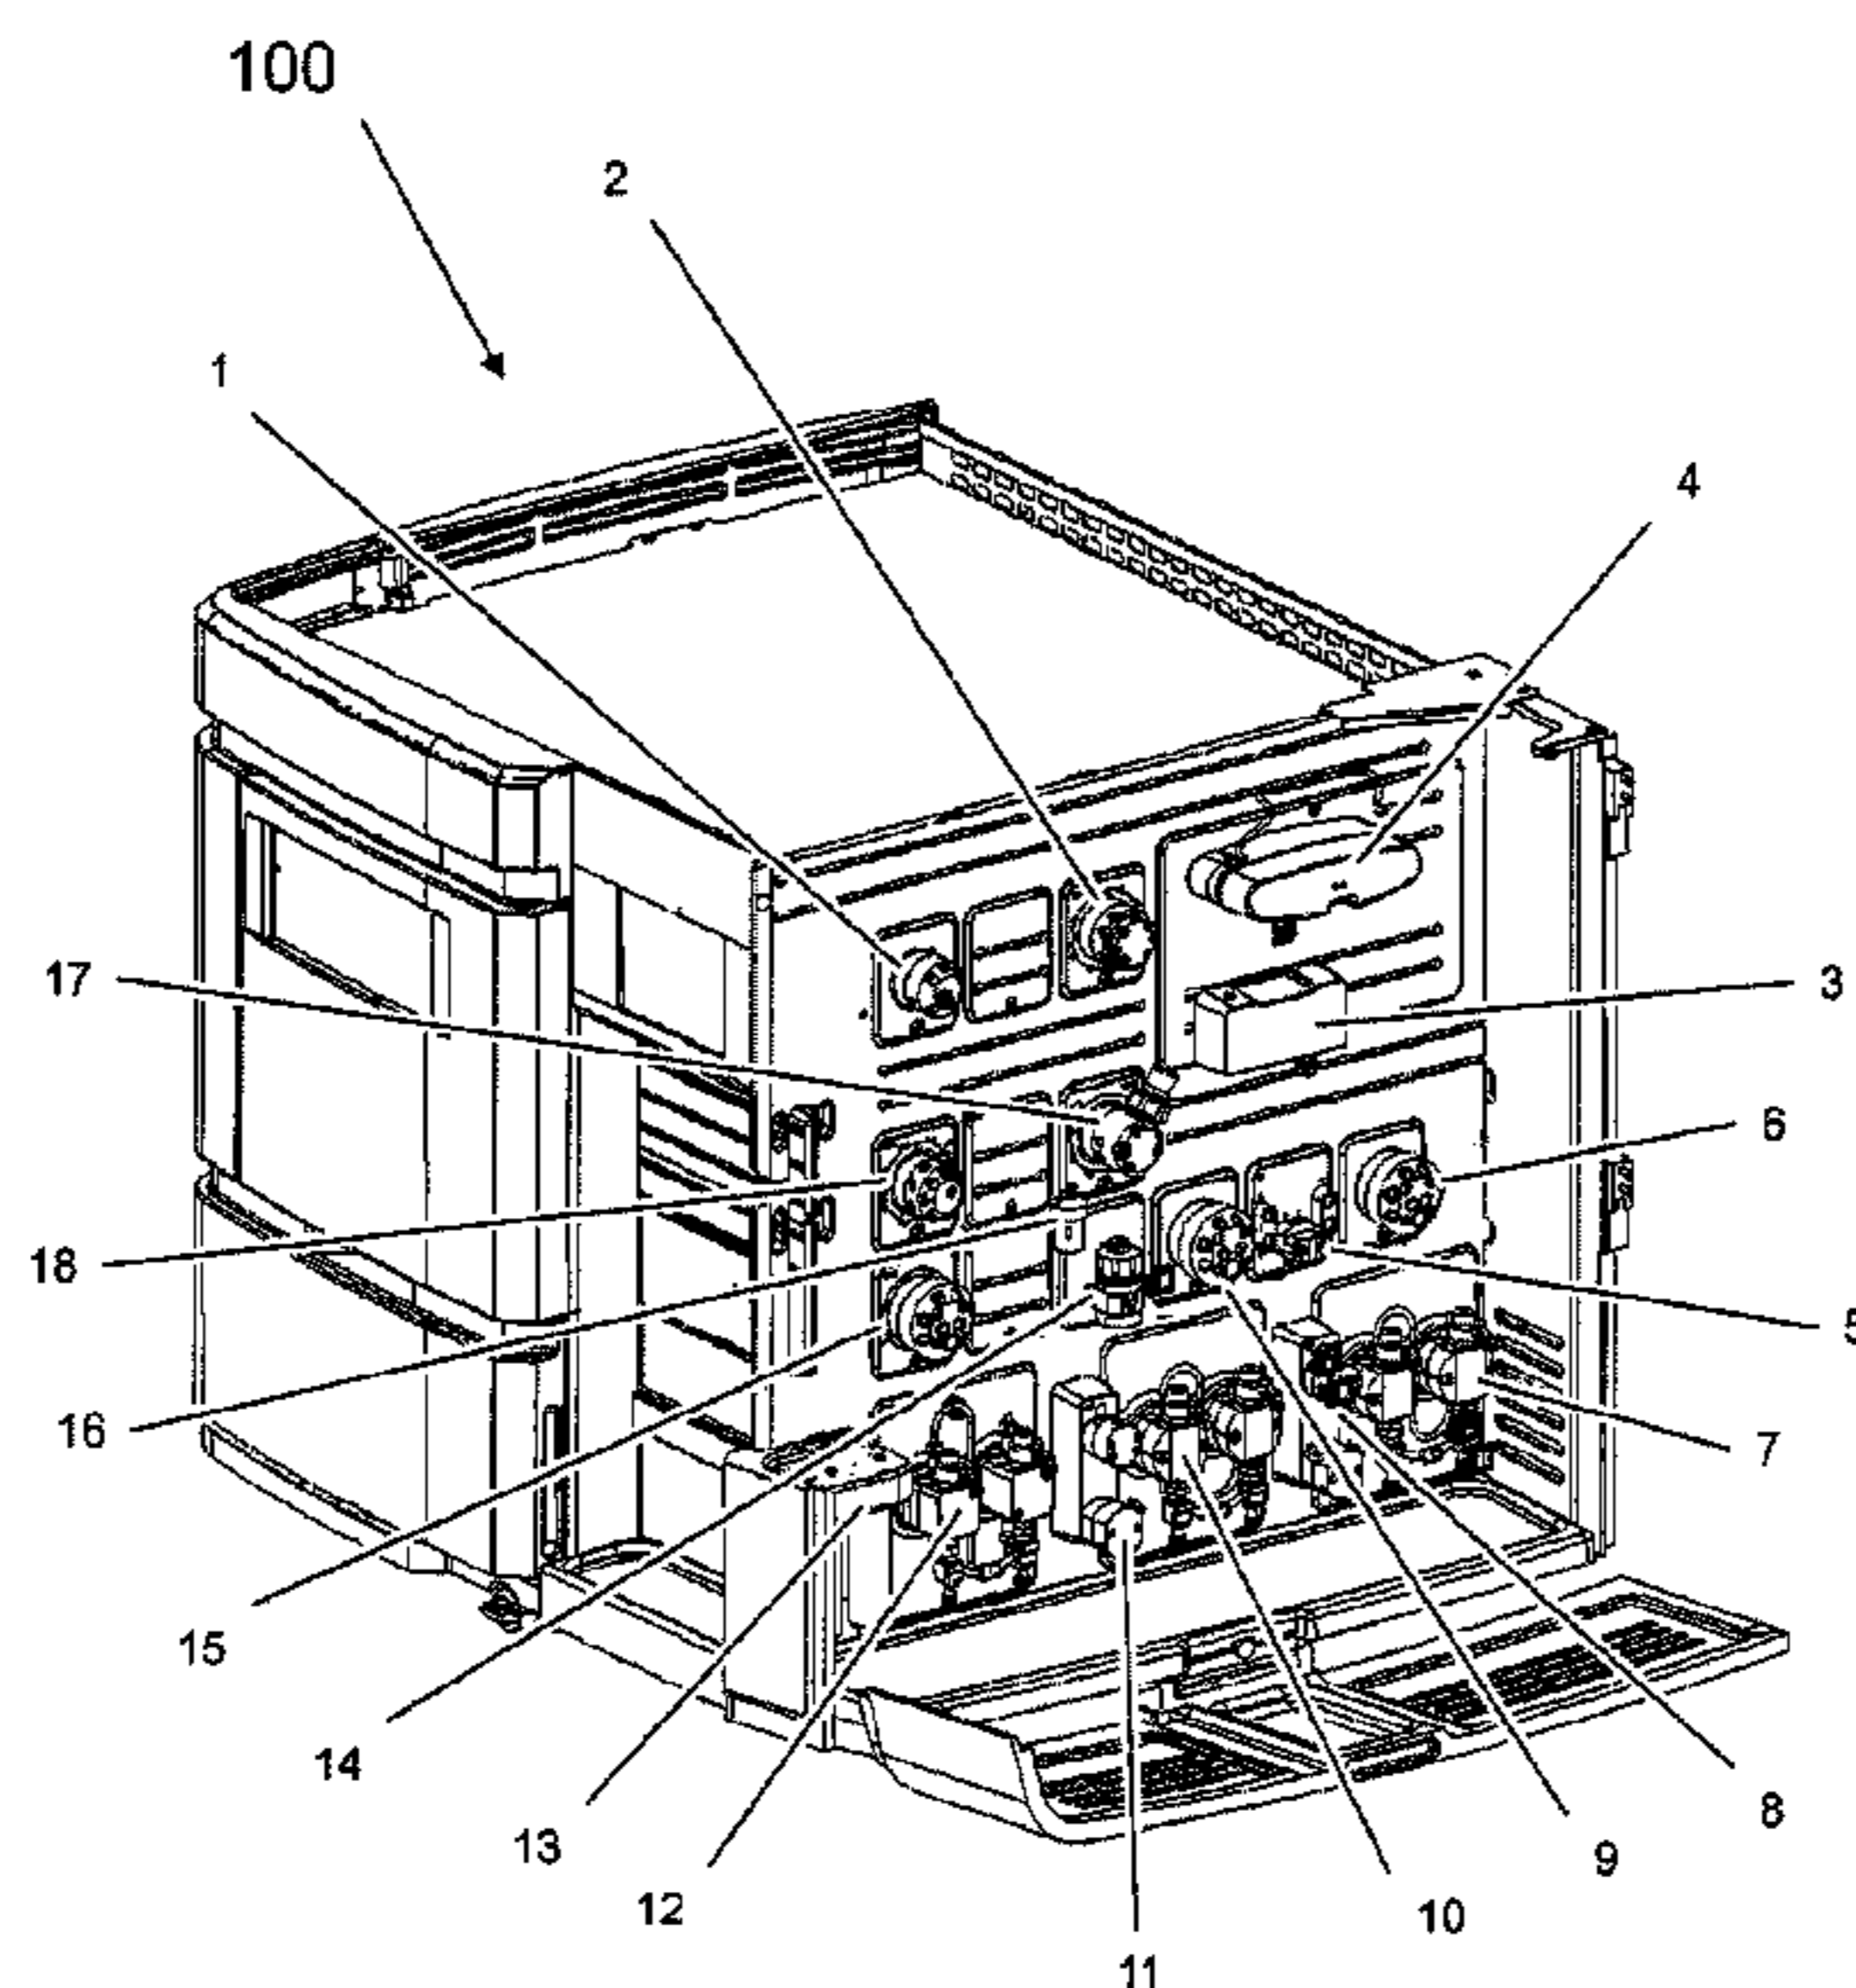

(51) **Int. Cl.**

**B01D 29/60** (2006.01)  
**B01D 15/10** (2006.01)  
**G01N 30/24** (2006.01)  
**G01N 30/38** (2006.01)  
**G01N 30/88** (2006.01)  
**G01N 30/02** (2006.01)  
**G01N 35/00** (2006.01)  
**B01D 15/08** (2006.01)  
**B01D 17/12** (2006.01)

(52) **U.S. Cl.**

CPC ..... **G01N 30/24** (2013.01); **G01N 30/38** (2013.01); **G01N 30/88** (2013.01); **B01D 15/08** (2013.01); **B01D 17/12** (2013.01); **B01D 2201/54** (2013.01); **G01N 2030/027** (2013.01); **G01N 2030/8804** (2013.01); **G01N 2030/8881** (2013.01); **G01N 2035/00326** (2013.01); **Y10T 137/6416** (2015.04); **Y10T 137/6525** (2015.04); **Y10T 137/6851** (2015.04); **Y10T 137/85986** (2015.04); **Y10T 137/87885** (2015.04)

(58) **Field of Classification Search**

CPC ... **G01N 2035/00326**; **G01N 2030/027**; **G01N 2030/8881**; **B01D 29/60**; **B01D 15/10**; **B01D 2201/54**; **B01D 17/12**; **B01D 15/08**; **Y10T 1375/6851**; **Y10T 137/6525**; **Y10T 137/6416**; **Y10T 137/85986**; **Y10T 137/87885**

See application file for complete search history.

(56)

**References Cited**

U.S. PATENT DOCUMENTS

4,224,033 A \* 9/1980 Hansen et al. .... 436/53  
 5,730,867 A 3/1998 Drew et al.  
 5,766,460 A 6/1998 Bergstrom et al.  
 5,792,742 A \* 8/1998 Gold et al. .... 514/9.3  
 5,896,273 A 4/1999 Varghese et al.  
 5,959,841 A 9/1999 Allen et al.  
 6,190,617 B1 \* 2/2001 Clark et al. .... 422/562  
 6,355,164 B1 3/2002 Wendell et al.  
 6,434,018 B1 8/2002 Waltz  
 6,599,484 B1 \* 7/2003 Zigler et al. .... 422/130  
 6,741,463 B1 5/2004 Akhtar et al.  
 6,832,622 B2 12/2004 Hassel et al.  
 6,968,958 B2 11/2005 Lauchner et al.  
 7,374,674 B2 5/2008 Miyauchi et al.  
 7,641,242 B2 1/2010 Van Pelt  
 7,910,067 B2 3/2011 Knight et al.  
 7,932,090 B2 4/2011 Carter et al.  
 8,821,718 B2 9/2014 Blomberg et al.  
 9,404,902 B2 8/2016 Blomberg et al.  
 9,671,420 B2 6/2017 Blomberg et al.  
 9,709,589 B2 7/2017 Blomberg et al.  
 9,709,590 B2 7/2017 Blomberg et al.  
 9,709,591 B2 7/2017 Blomberg et al.  
 2002/0185442 A1 12/2002 Maiefski et al.  
 2004/0089057 A1 5/2004 Hobbs et al.  
 2004/0264145 A1 12/2004 Miller et al.  
 2005/0051468 A1 3/2005 Miyauchi et al.  
 2006/0047466 A1 3/2006 White  
 2006/0274082 A1 12/2006 Cochran et al.  
 2007/0081308 A1 4/2007 Ishida  
 2007/0095126 A1 5/2007 Bailey et al.  
 2007/0097636 A1 5/2007 Johnson et al.  
 2007/0247826 A1 10/2007 Grady et al.  
 2008/0023653 A1 1/2008 Lee et al.  
 2008/0035542 A1 2/2008 Mourtada et al.  
 2008/0233653 A1 \* 9/2008 Hess et al. .... 436/43  
 2014/0353224 A1 12/2014 Blomberg et al.  
 2017/0284985 A1 10/2017 Blomberg et al.

FOREIGN PATENT DOCUMENTS

DE 19847439 A1 4/2000  
 EP 0309596 A1 4/1989  
 GB 1418503 A 12/1975  
 GB 1418503 A1 12/1975  
 JP 2002-333438 A 11/2002  
 JP 2005-106813 A 4/2005  
 WO 0022429 A1 4/2000  
 WO WO 00/22429 4/2000  
 WO WO-2001/089681 11/2001  
 WO WO-2005/042146 A2 5/2005  
 WO WO 2006/134035 12/2006  
 WO WO 2006/134035 A1 12/2006  
 WO WO-2007/036712 A1 4/2007

OTHER PUBLICATIONS

Final Written Decision, Inter Partes Review 2015-01826, Feb. 6, 2017.\*  
 Decision to Institute, Inter Partes Review 2015-01826, Feb. 29, 2016.\*  
 "Manual ADI 2040 Process Analyzer" 1999-2007, Applikon Analytical B.V., pp. 346-619 (part 2).\*  
 General Electric, "User Manual," ÄKTA pure, Dec. 2014, pp. 3929-4445.  
 Dionex, "ICS-3000 Ion Chromatography System Operator's Manual," Thermo Scientific, Jan. 2008, pp. 4779-5170.  
 Bio-Rad Laboratories, Inc., "Biologic Duoflow Chromatography System," Instruction Manual, 2003, pp. 5810-6048.  
 Larry Tucker et al., "Videotaped Deposition of Metrohm 30 (B) (6)," *GE Healthcare vs. Bio-Rad*, Aug. 10, 2015, pp. 1-292.  
 Tecan Systems, "Cavro XLP 6000 Modular Syringe Pump," Operating Manual, Part I, Oct. 2005, pp. 5542-5698.  
 Office Action issued in Chinese Patent Application No. 201510602257.9 dated Jul. 13, 2016.  
 European Search Report issued in European Patent Application No. 16205536 dated Mar. 17, 2017 (8 pages).  
 Metrohm-Peak, Inc., "Determination of Anions + Oxyhalides in Various Waters by Suppressed Conductivity (USEPA method 300 A&B)," IC Application Work AW US6-0125-052007, 2007, pp. 001327-001336.  
 Metrohm Ion analysis, "IC Pump-2.872.0010," 872 Extension Module, pp. 1-67.  
 Applikon Analytical, "Multi-purpose wet chemical analysis," Process Analyzer ADI 2040, Sep. 2008, pp. 1547-1554.  
 Applikon Analytical, "Trace Metal and Plating Bath Analysis," ADI2045VA Process Analyzer, Sep. 2007, pp. 1555-1562.  
 General Electric, "Operating Instructions Original Instructions," ÄKTA pure, Apr. 2014, pp. 3785-3928.  
 John Loffink, "Dell PowerEdge M1000e Modular Enclosure Architecture," Dell Enterprise White Paper, Jan. 2008, pp. 4577-4618.  
 APC, "Rack Enclosures and Open Frame Racks for Server and Networking Applications in IT Environments," Rack Systems, 2006, pp. 4619-4638.  
 Gilson, Inc., "Product Guide," The Element of Purification, Jul. 2008, pp. 5171-5207.  
 Gilson, Inc., "402 Syringe Pump User's Guide," Jul. 2003, pp. 5208-5293.  
 Gilson, Inc., "Gilson Product Guide," 2004, pp. 5294-5343.  
 Gilson, Inc., "Spec Sheet," 2003, 1 Page.  
 Gilson, Inc., "Brochure," 2003, 1 Page.  
 Gilson, Inc., "User's Guide," 2003, 1 Page.  
 Labomatic, "Labomatic HPLC valve and column system panel," pp. 5347-5348.  
 Andreas Schmid, "The Energy Issue in Whole Cell Oxyfunctionalization," GreenChem Symposium, Nov. 9, 2006, pp. 5349-5386.  
 Labomatic Instruments AG, "Customer-specific preparative HPLC Systems," 5387-5389.  
 Waters Corporation, "Waters 2767 Sample Manager, Injector, and Collector," Installation and Maintenance Guide, 2006, pp. 5390-5541.  
 Tecan Group Ltd, "Cavro OEM Pumps and Valves," 2008, 1 page.

(56)

**References Cited**

## OTHER PUBLICATIONS

Tecan Group Ltd, "Cavro XLP 6000," 2008, 1 page.

Eda Tezcanli, "An Analytical Survey on Customization at Modular Systems in the Context of Industrial Design," A Thesis Submitted to the Graduate School of Engineering and Sciences of Izmir Institute of Technology in Partial Fulfillment of the Requirements for the Degree of Master of Science in Industrial Design, Jan. 2006, pp. 5701-5809.

Applikon Analytical, "Box Wet Part Module 3X," Bio-Rad Ex. 1003, 1 page.

Gilson, Inc., "2007-2008 Product Guide," Bio-Rad Ex. 1010 pp. 1-37.

Gilson, Inc., "402 Syringe Pump User's Guide," Bio-Rad Ex. 1011, Jun. 2001, pp. 1-86.

David Bilsker, "*Bio-Rad Laboratories, Inc v. GE Healthcare Bio-Sciences AB*," United States Patent and Trademark Office, pp. 1-71.

Applikon Analytical Confidential, "Analyzers 1999-2008," Bio-Rad Ex. 1004, Jul. 8, 2015, pp. 1323-1326.

Thomas Koshy, "Declaration of Thomas Koshy," in the United States District Court for the Southern District of New York, Civil Action No. 1:14-cv-07080-LTS, pp. 1-3.

United States Patent and Trademark Office, "*Bio-Rad Laboratories, Inc. v. GE Healthcare Bio-Sciences AB*," Declaration of Dr. Bruce Gale in Support of Bio-Rad Laboratories' Petition for Institution of an IPR on U.S. Pat. No. 8,821,718, pp. 1-84.

Metrohm Ion Analysis, "Intelligent Ion Chromatography," Professional IC 850, pp. 1-24.

Brinkmann, "875 ProcessLab Hardware," ProcessLab, pp. 1-15.

Brinkmann, "875 ProcessLab Components," ProcessLab, pp. 1-26.

H. Schäfer, "Compact View of a Modular Design or a new Philosophy in Metrohm IC," Professional IC, pp. 1-90.

Brinkmann, "Is ProcessLab Explosion-Proof?" ProcessLab, pp. 1-12.

Metrohm—Intelligent Ion Chromatography, [www.professional-ic.com](http://www.professional-ic.com), 2012, pp. 1-28.

Metrohm—850 Professional IC Manual, <http://products.metrohm.com>, pp. 1-146.

ADI 2045 VA Instrument Manual, Applikon Analytical, 2007, pp. 1-80, Version 1.2.

ADI 2040 Process Analyzer Manual—Basic Maintenance & Spare parts, Applikon Analytical, Mar. 2008, Version 1.53, pp. 1-48.

ADI 2040 Process Analyzer Manual—Analysis Methods, Applikon Analytical, Sep. 2002, pp. 1-44, Version 1.4.

ADI 2040 Process Analyzer Manual—Serial Communication, Applikon Analytical, Version 1.4, Apr. 2006, pp. 1-134.

ADE 2040 Process Analyzer Manual—Basic Operation, Applikon Analytical, Version 1.4, pp. 1-30, Jul. 2006.

ADI Process Analyzer Manual—Advanced Operation, Applikon Analytical, Version 1.53, pp. 1-78, Oct. 2007.

ADI 2040 Process Analyzer Manual—Configuration, Applikon Analytical, Version 1.4, pp. 1-44, Jul. 2006.

ADI 2040 Process Analyzer Manual—Hardware & Installation, Applikon Analytical, Version 1.53, pp. 1-144, May 2008.

ADI 2040 Process Analyzer Manual, Applikon Analytical, 1-10 pp., Apr. 1999.

Bilsker, Petition for Inter Parties Review, *Bio-Rad Laboratories, Inc. v. GE Healthcare Bio-Science AB*, Sep. 2015, pp. 1-71.

Metrohm 850 Professional IC teardown summary (2.850.2220 ProfIC Anion MCS HP Gradient) Jul. 2016, pp. 1-9.

ADI 2040 Process Analyzer, Manual, Applikon Analytical, 1999-2007, *Bio-Rad Labs, Inc. v. GE Healthcare Biosciences AB*, IPR2015-01826, Bio-Rad Ex. 1002, pp. 1-619.

EP Office Action dated Feb. 26, 2014 Issued on Corresponding EP Application No. 10786454.8 (5 pages).

850 Professional IC Manual, Metrohm, AnCat-MCS-2.850.3030, May 2009, *Bio-Rad Labs, Inc. v. GE Healthcare Biosciences AB*, IPR2015-01826, Bio-Rad Ex. 1017, pp. 1-143, BIO-RAD001337-BIO-RAD001479.

Decision on Institution, *Bio-Rad Labs, Inc. v. GE Healthcare Biosciences AB*, IPR2015-01826, Paper No. 11, Feb. 29, 2016, pp. 1-47.

Metrohm 850 Professional IC Teardown Summary, 2.850.2220 ProfIC Anion MCS HP Gradient, Aug. 2016, pp. 1-9.

Biologic Duoflow Chromatography System, Instruction Manual, Bio-Rad Laboratories, Inc., 2003, BRGE00005810-BRGE00006048.

ICS-3000 Ion Chromatography System Operator's Manual, Dionex (Thermo Scientific), Doc. No. 065031, Rev. 04, Jan. 2008, BRGE00004779-BRGE00005170.

AKTA pure, User Manual, General Electric, Dec. 2014, BRGE00003929-BRGE00004445.

ADI 2045VA Manual, Applikon Analytical, 2007, BIO-RAD000620-BIO-RAD001322.

JP Office Action dated Dec. 17, 2013 issued on Corresponding JP Application No. 2012-514920, 6 pages (with English translation).

Deposition Transcript of Metrohm 30 (B) (6) Larry Tucker and Thomas Koshy, Aug. 10, 2015, *Bio-Rad Labs, Inc. v. GE Healthcare Biosciences AB*, IPR2015-01826, Bio-Rad Ex. 1005, p. 1-292.

Cavro XLP 6000 Modular Syringe Pump, Operating Manual, Tecan Systems, BRGE00005542-BRGE005698.

Waters 2767 Sample Manager, Injector, and Collector, Installation and Maintenance Guide, 71500276704 Rev B, Waters Corp., 2006, BRGE00005390-BRGE00005541.

European Search Report and Form 1507 issued in European Patent Application No. 16205536 dated Mar. 17, 2017 (8 pages).

Carvo OEM Pumps and Valves, Tecan Group, Ltd., Internet Archive, 1 page, BRGE00005699.

Carvo XLP 6000 60mm Stroke OEM Syringe Pump, Tecan Group, Ltd., Internet Archive, 1 page, BRGE00005700.

Gilson, Inc., Spec Sheet, Internet Archive, 1 page, BRGE00005344.

Gilson, Inc., Brochure, Internet Archive, 1 page, BRGE00005345.

Gilson, Inc., User Guide, Internet Archive, 1 page, BRGE00005346.

Andreas Schmid, "The Energy Issue in Whole Cell Oxyfunctionalization," GreenChem Symposium, Nov. 9, 2006, BRGE00005350-BRGE00005386.

Metrohm 811 Online IC / 821 Compact Online IC Brochure, pp. 1-11.

Brinkmann, "Is ProcessLab Explosion-Proof?" ProcessLab, 1 page.

\* cited by examiner

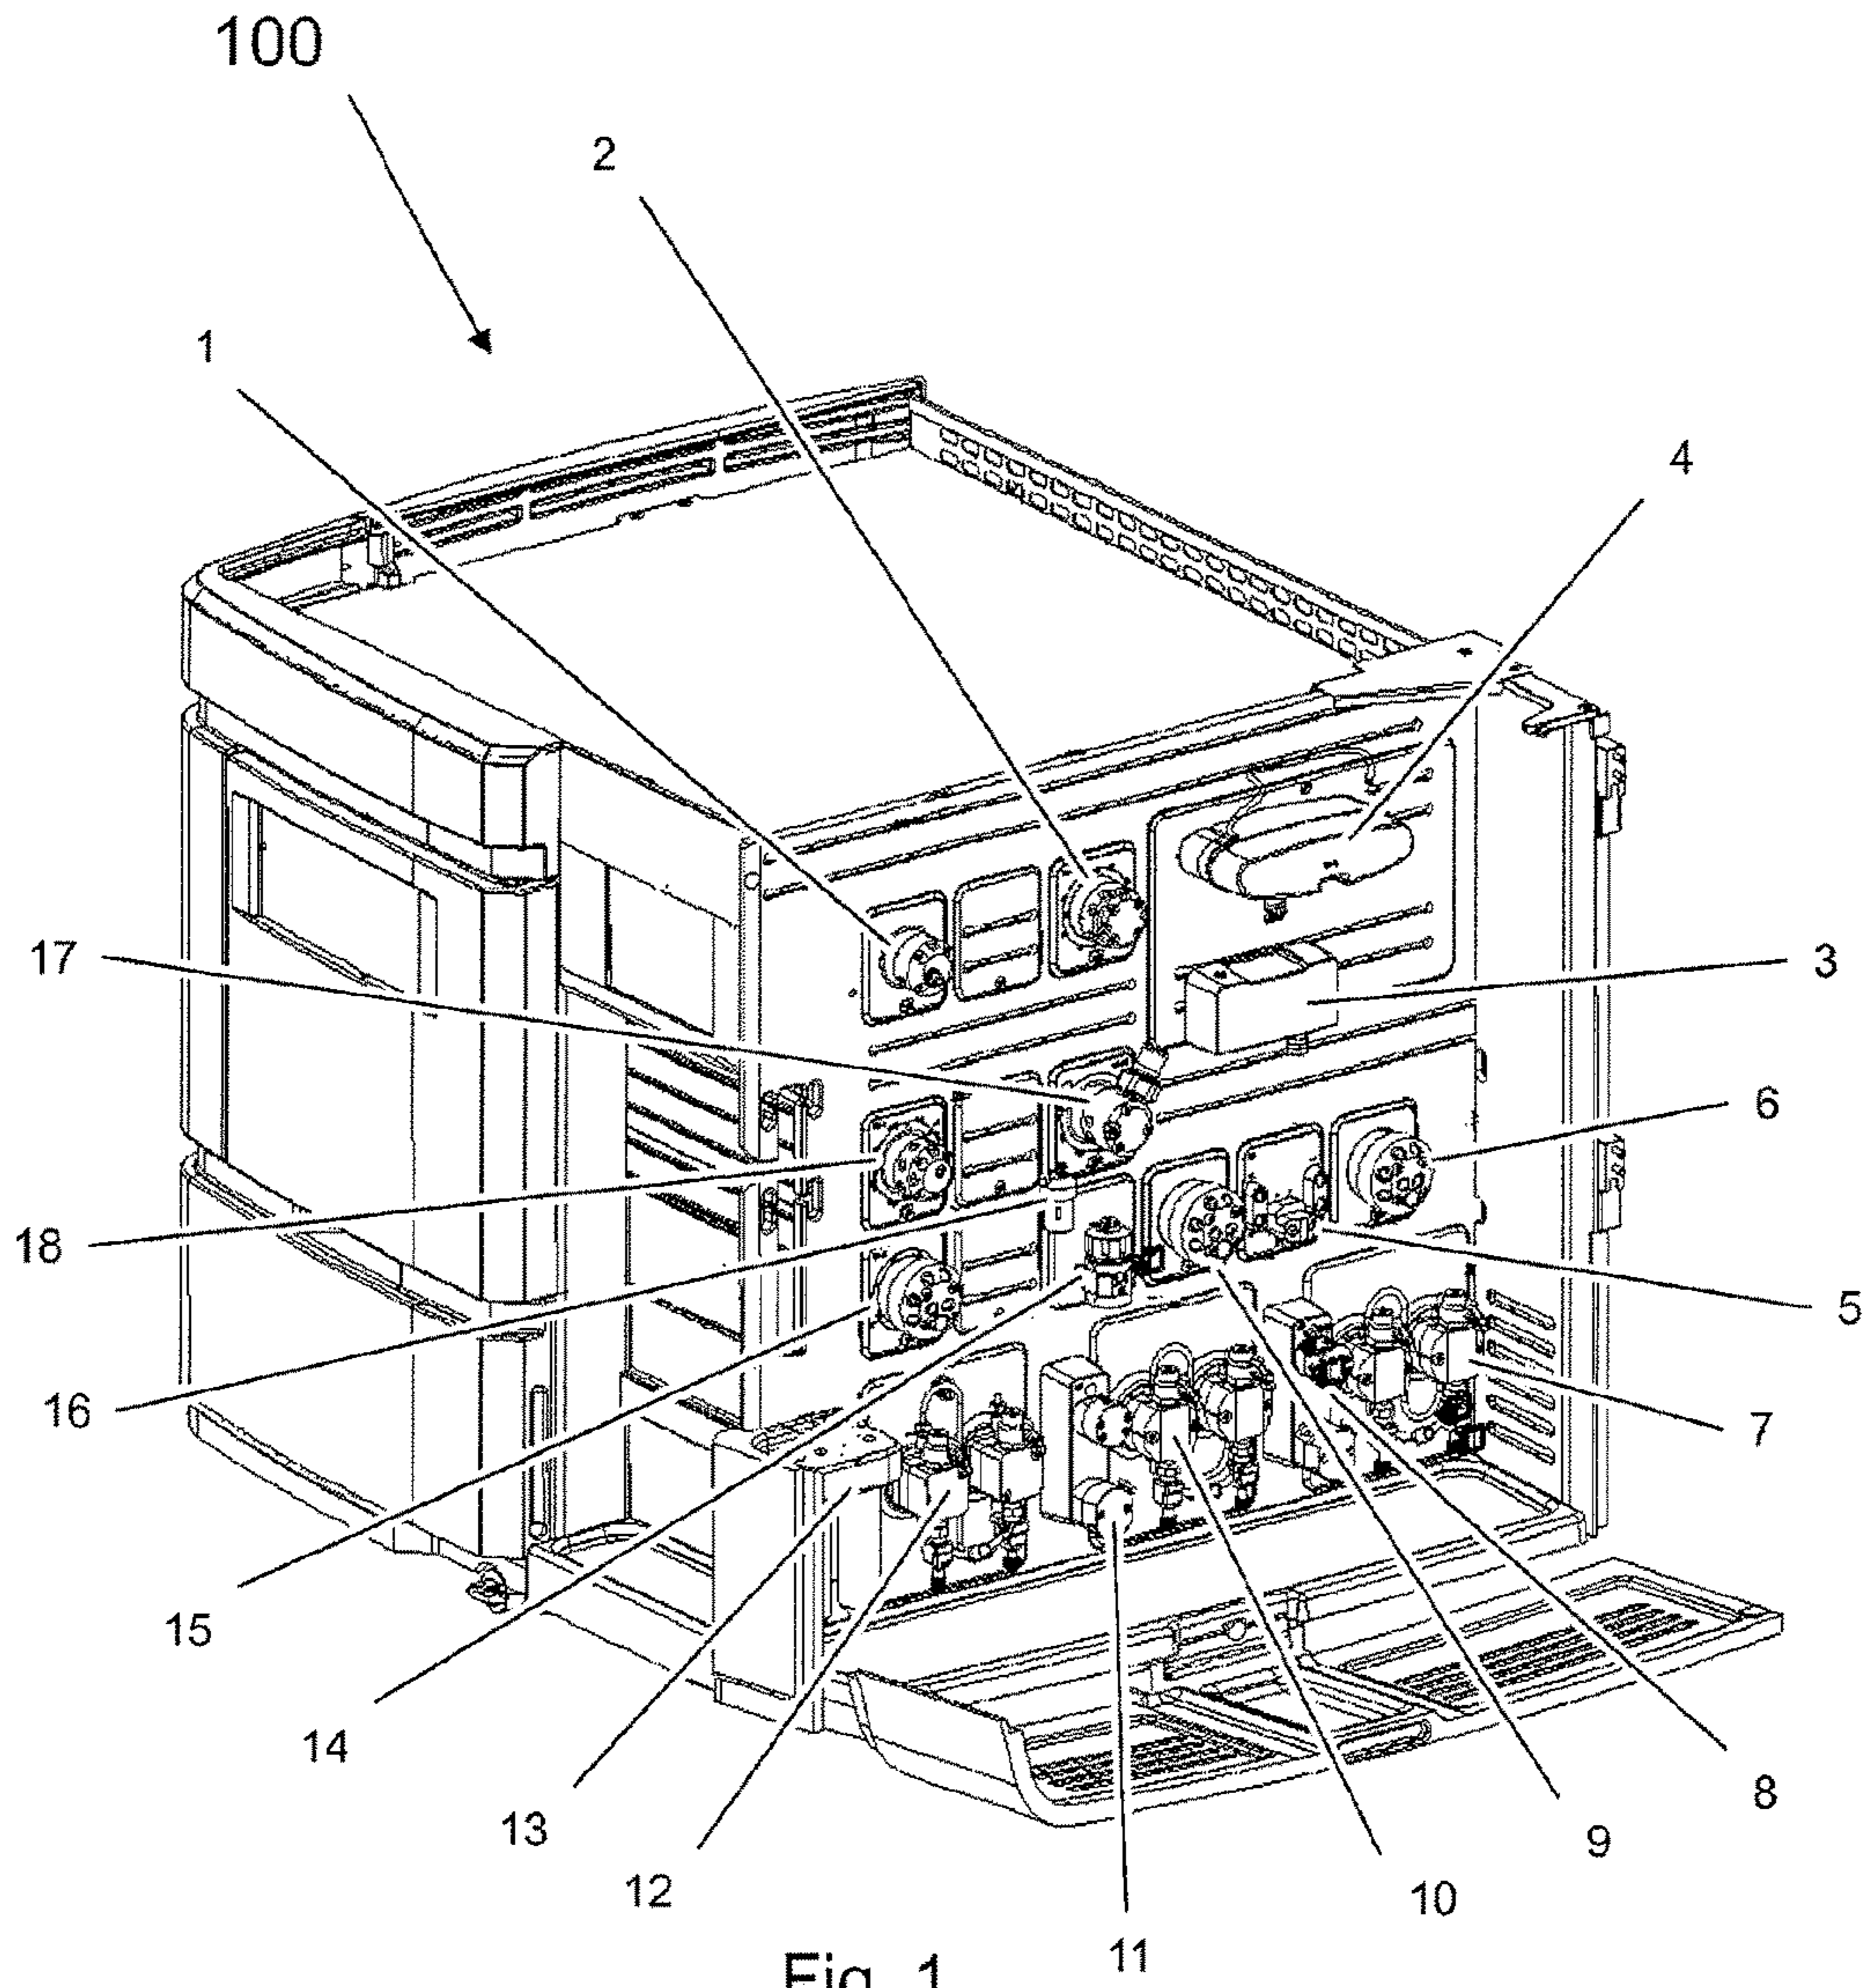


Fig. 1

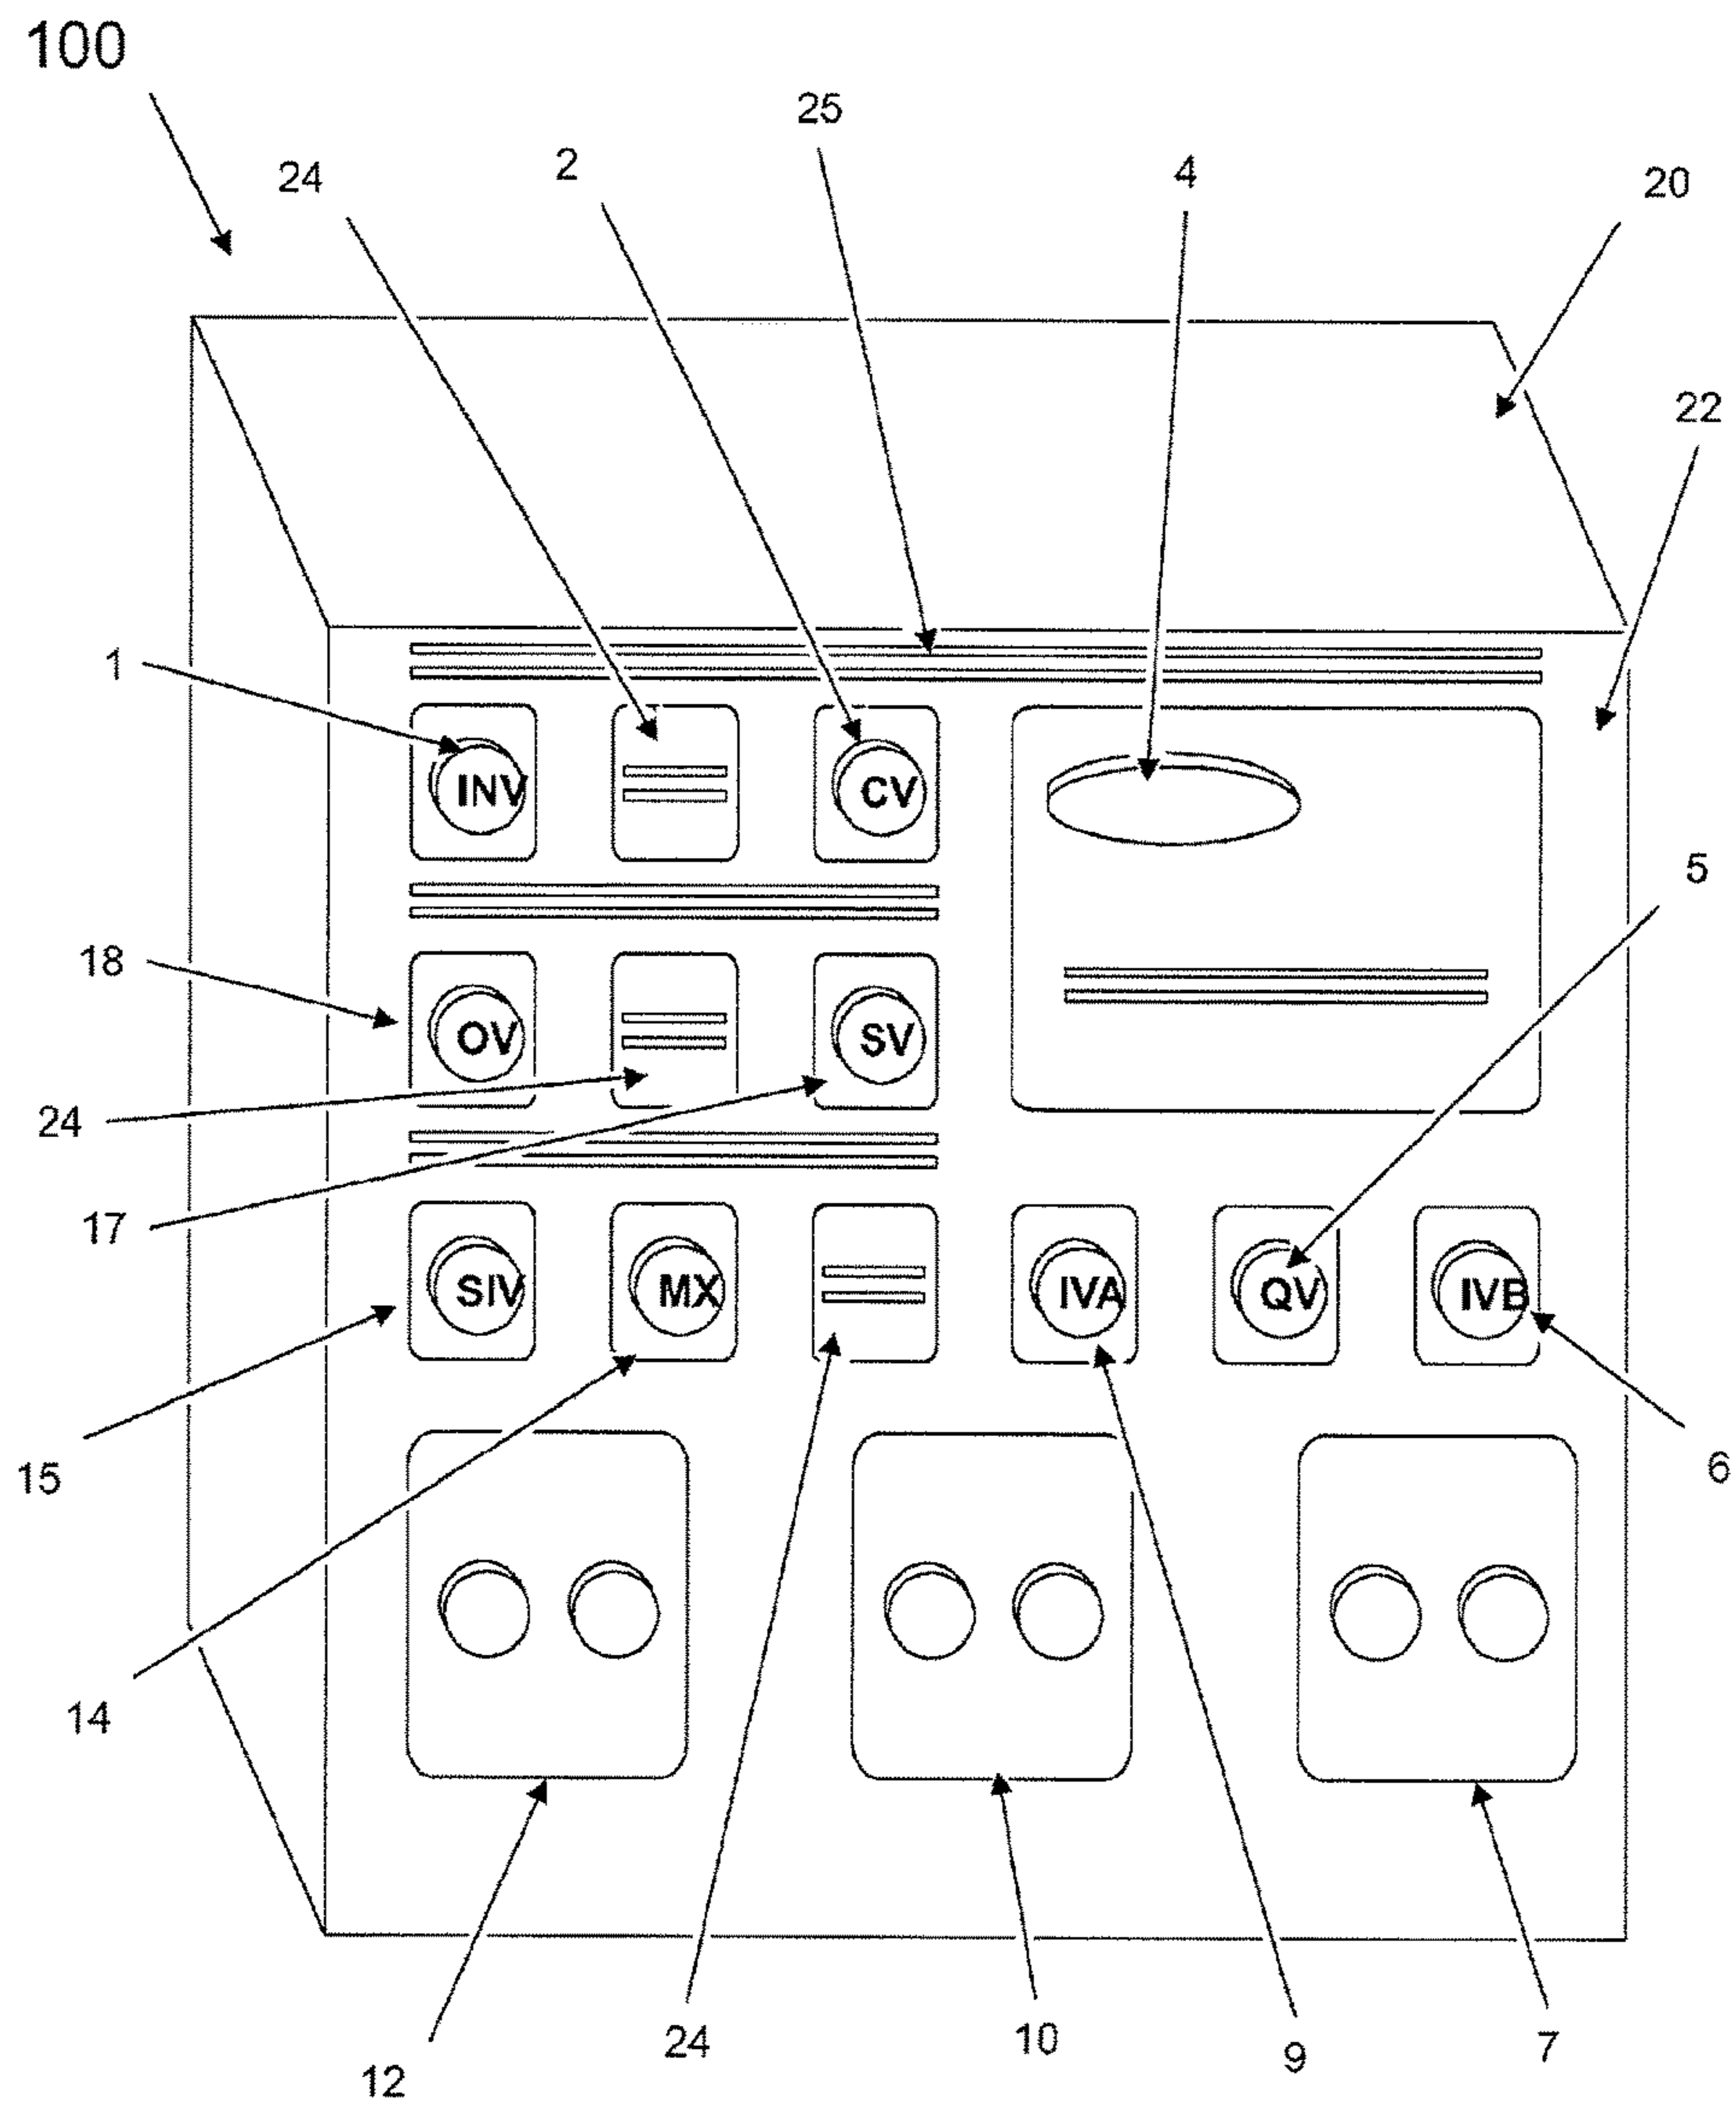


Fig. 2

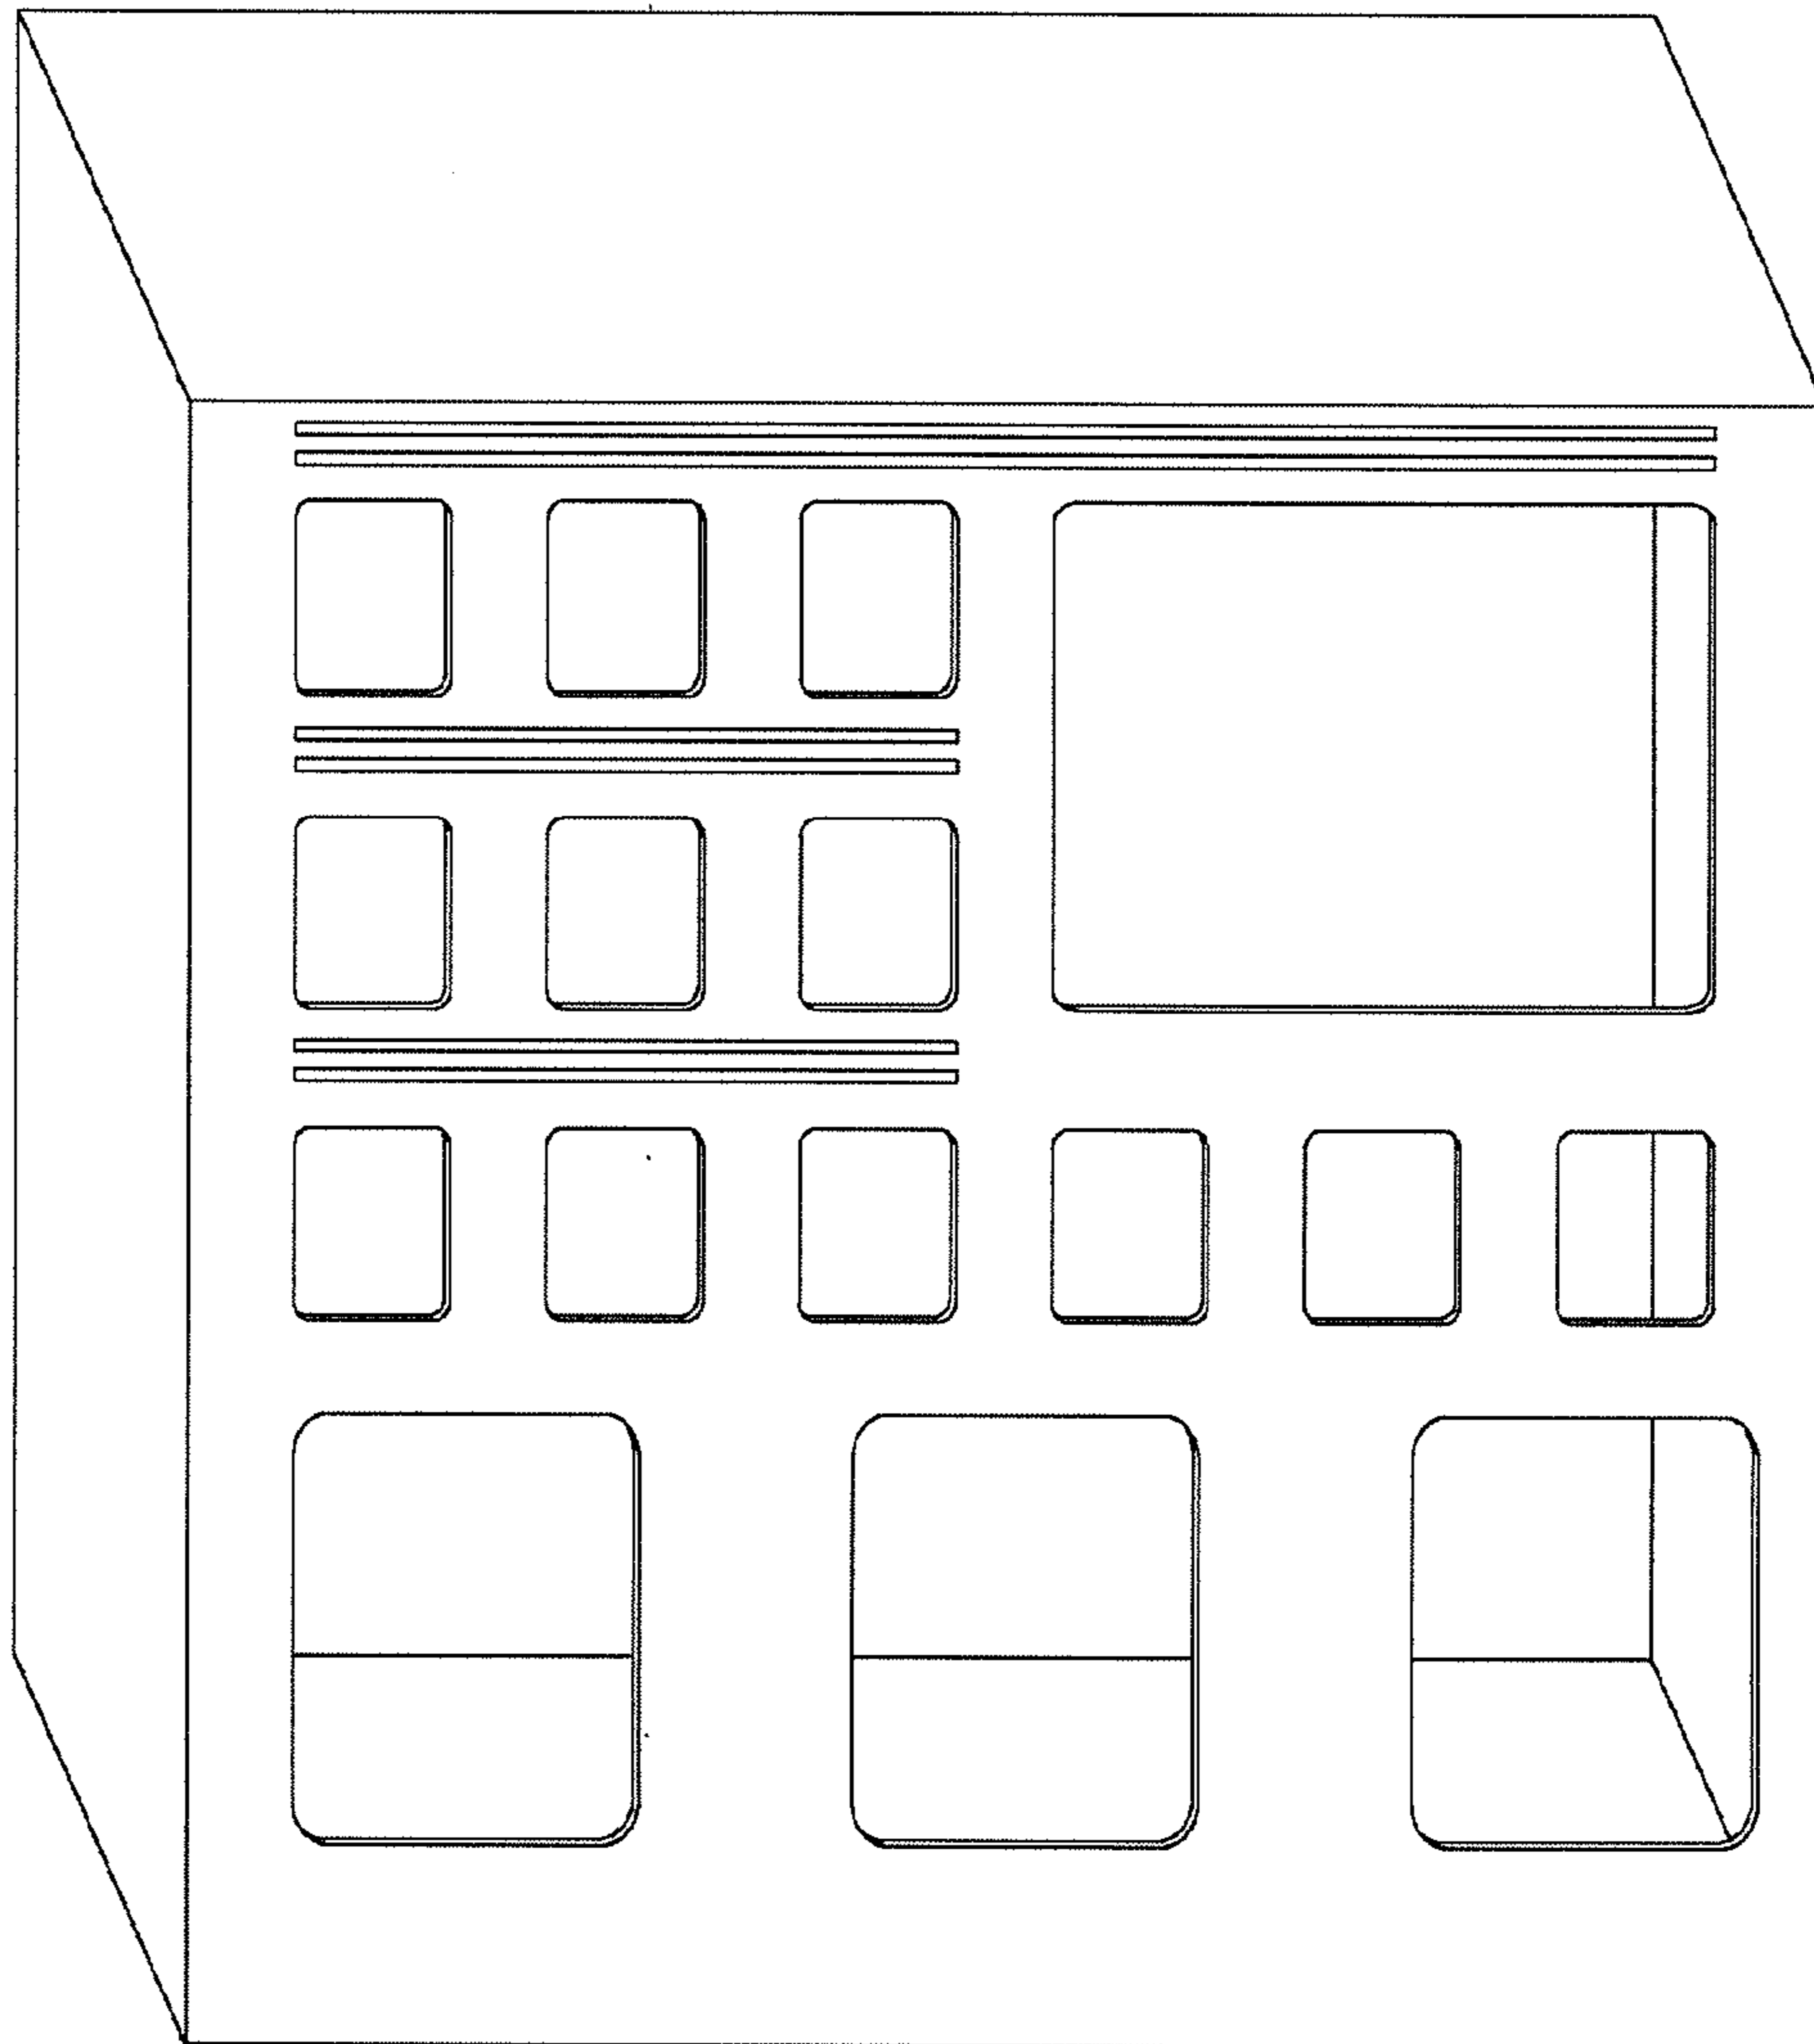


Fig. 3

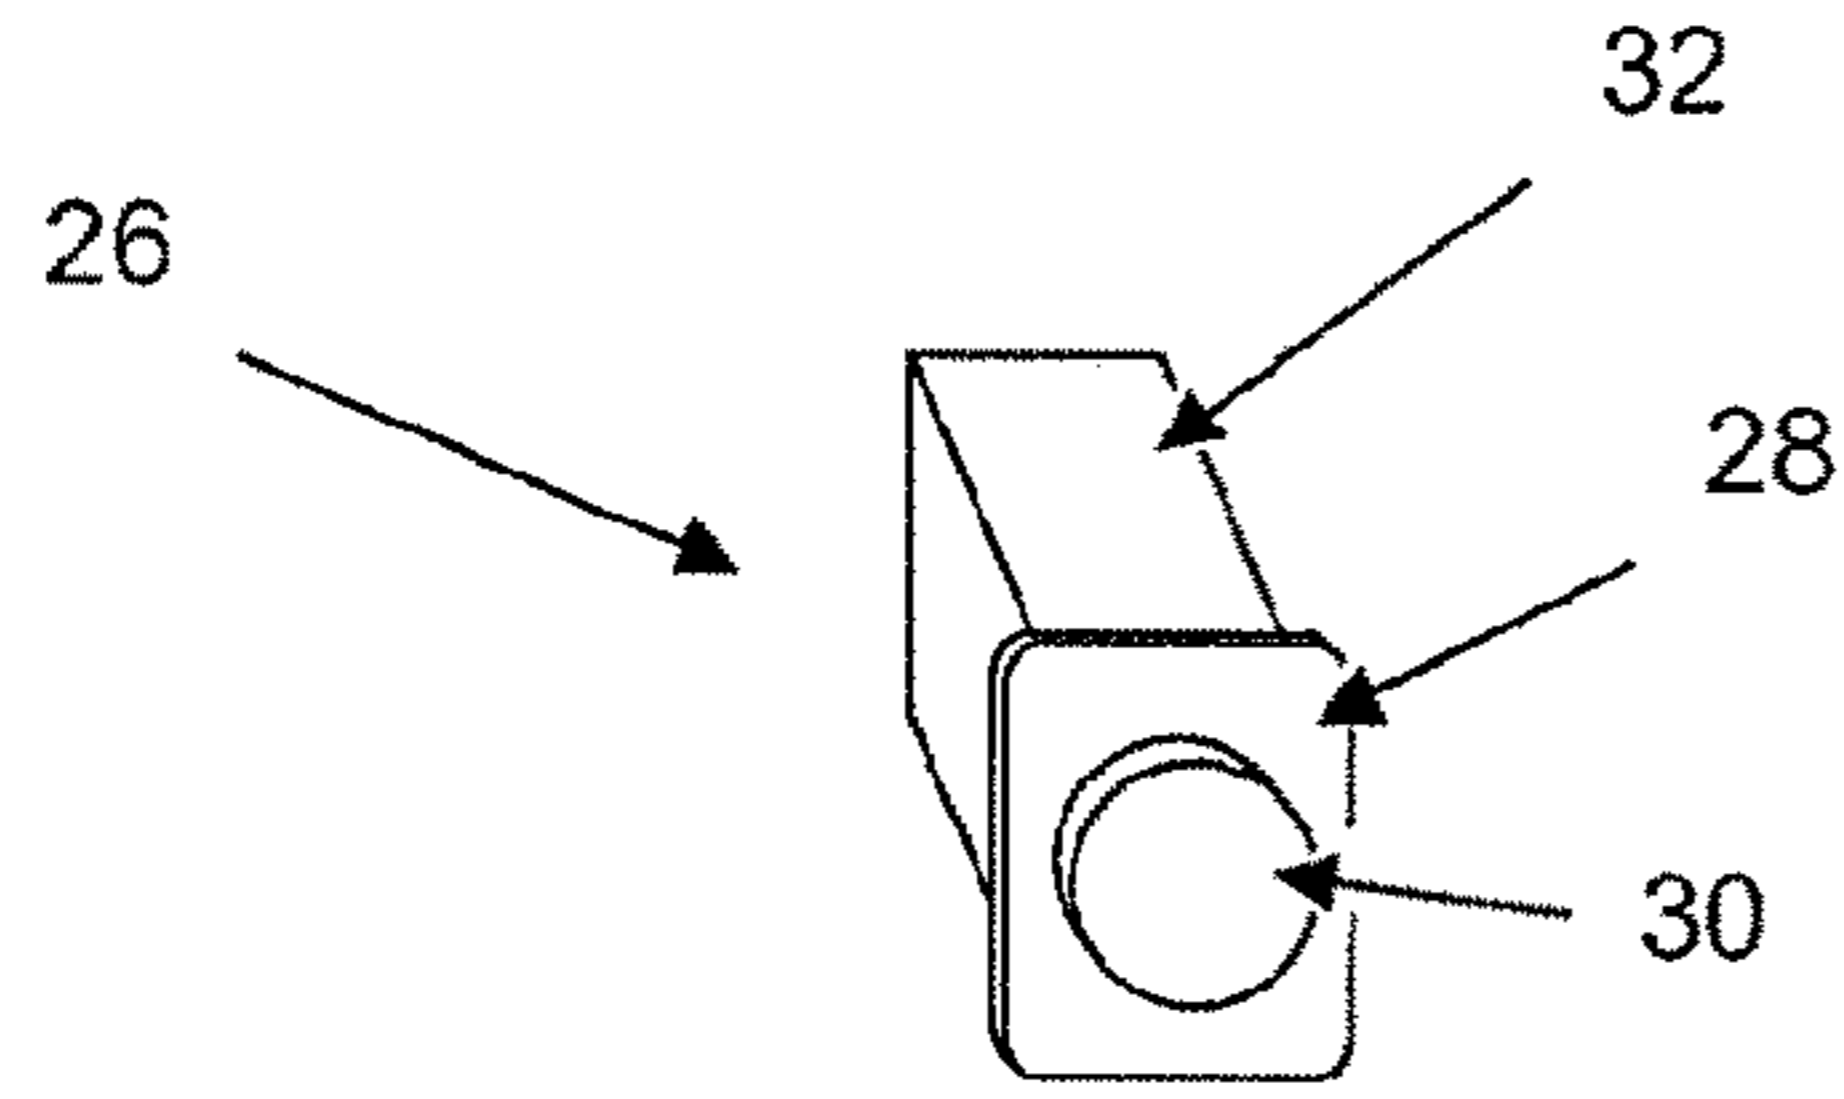


Fig. 4a

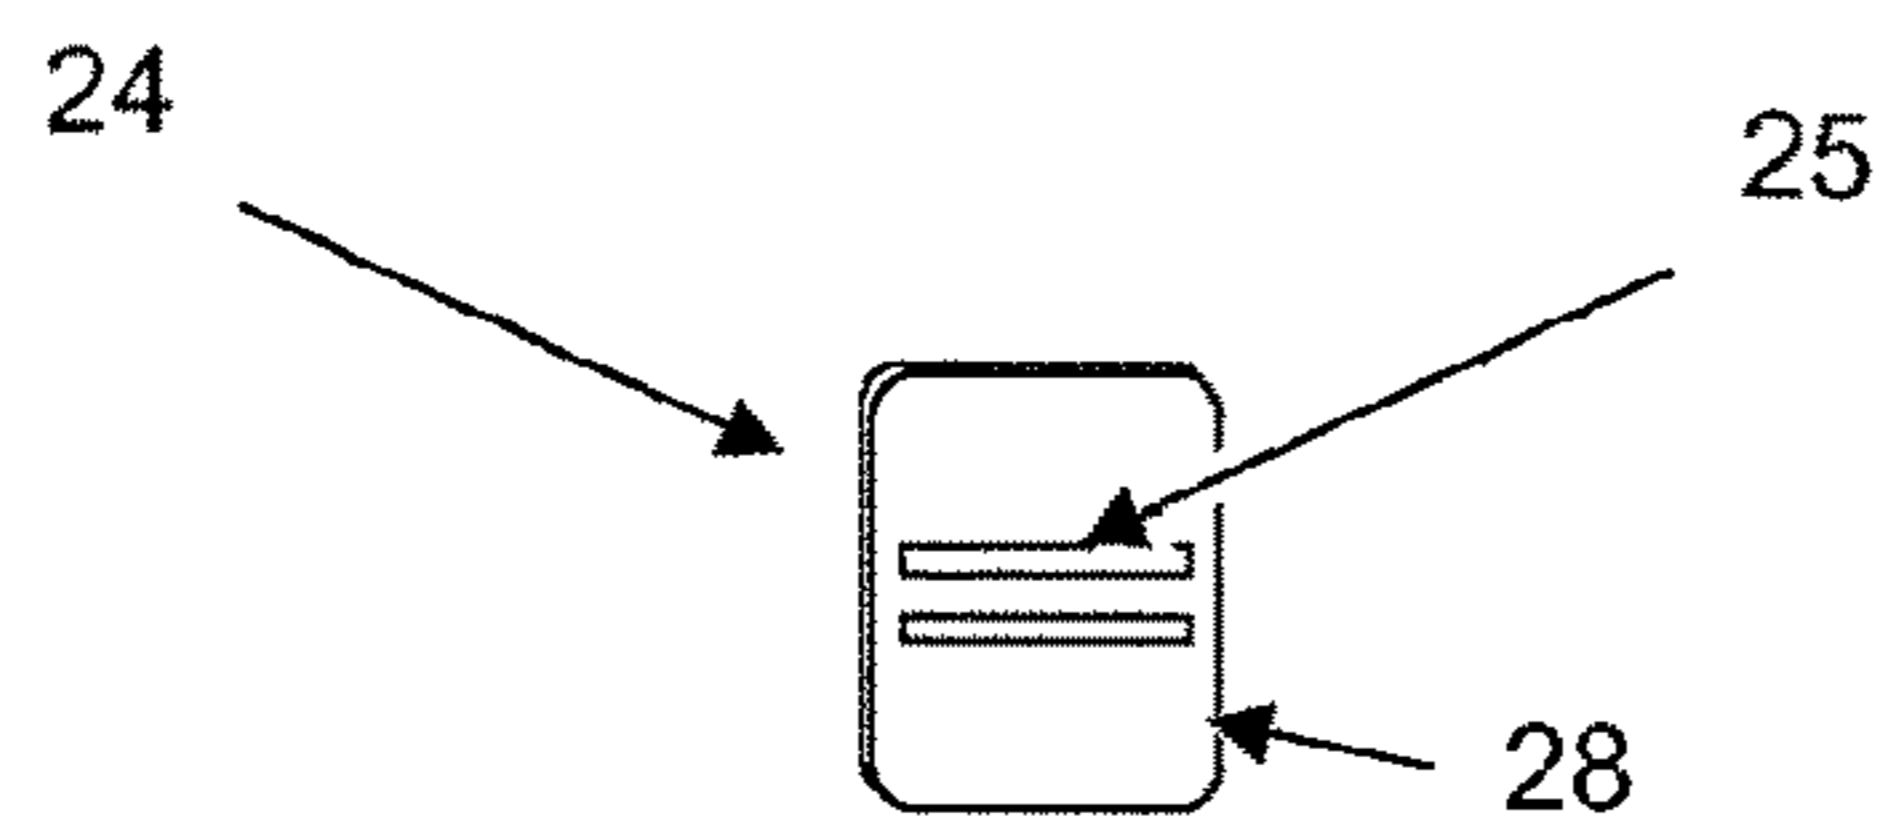


Fig. 4b

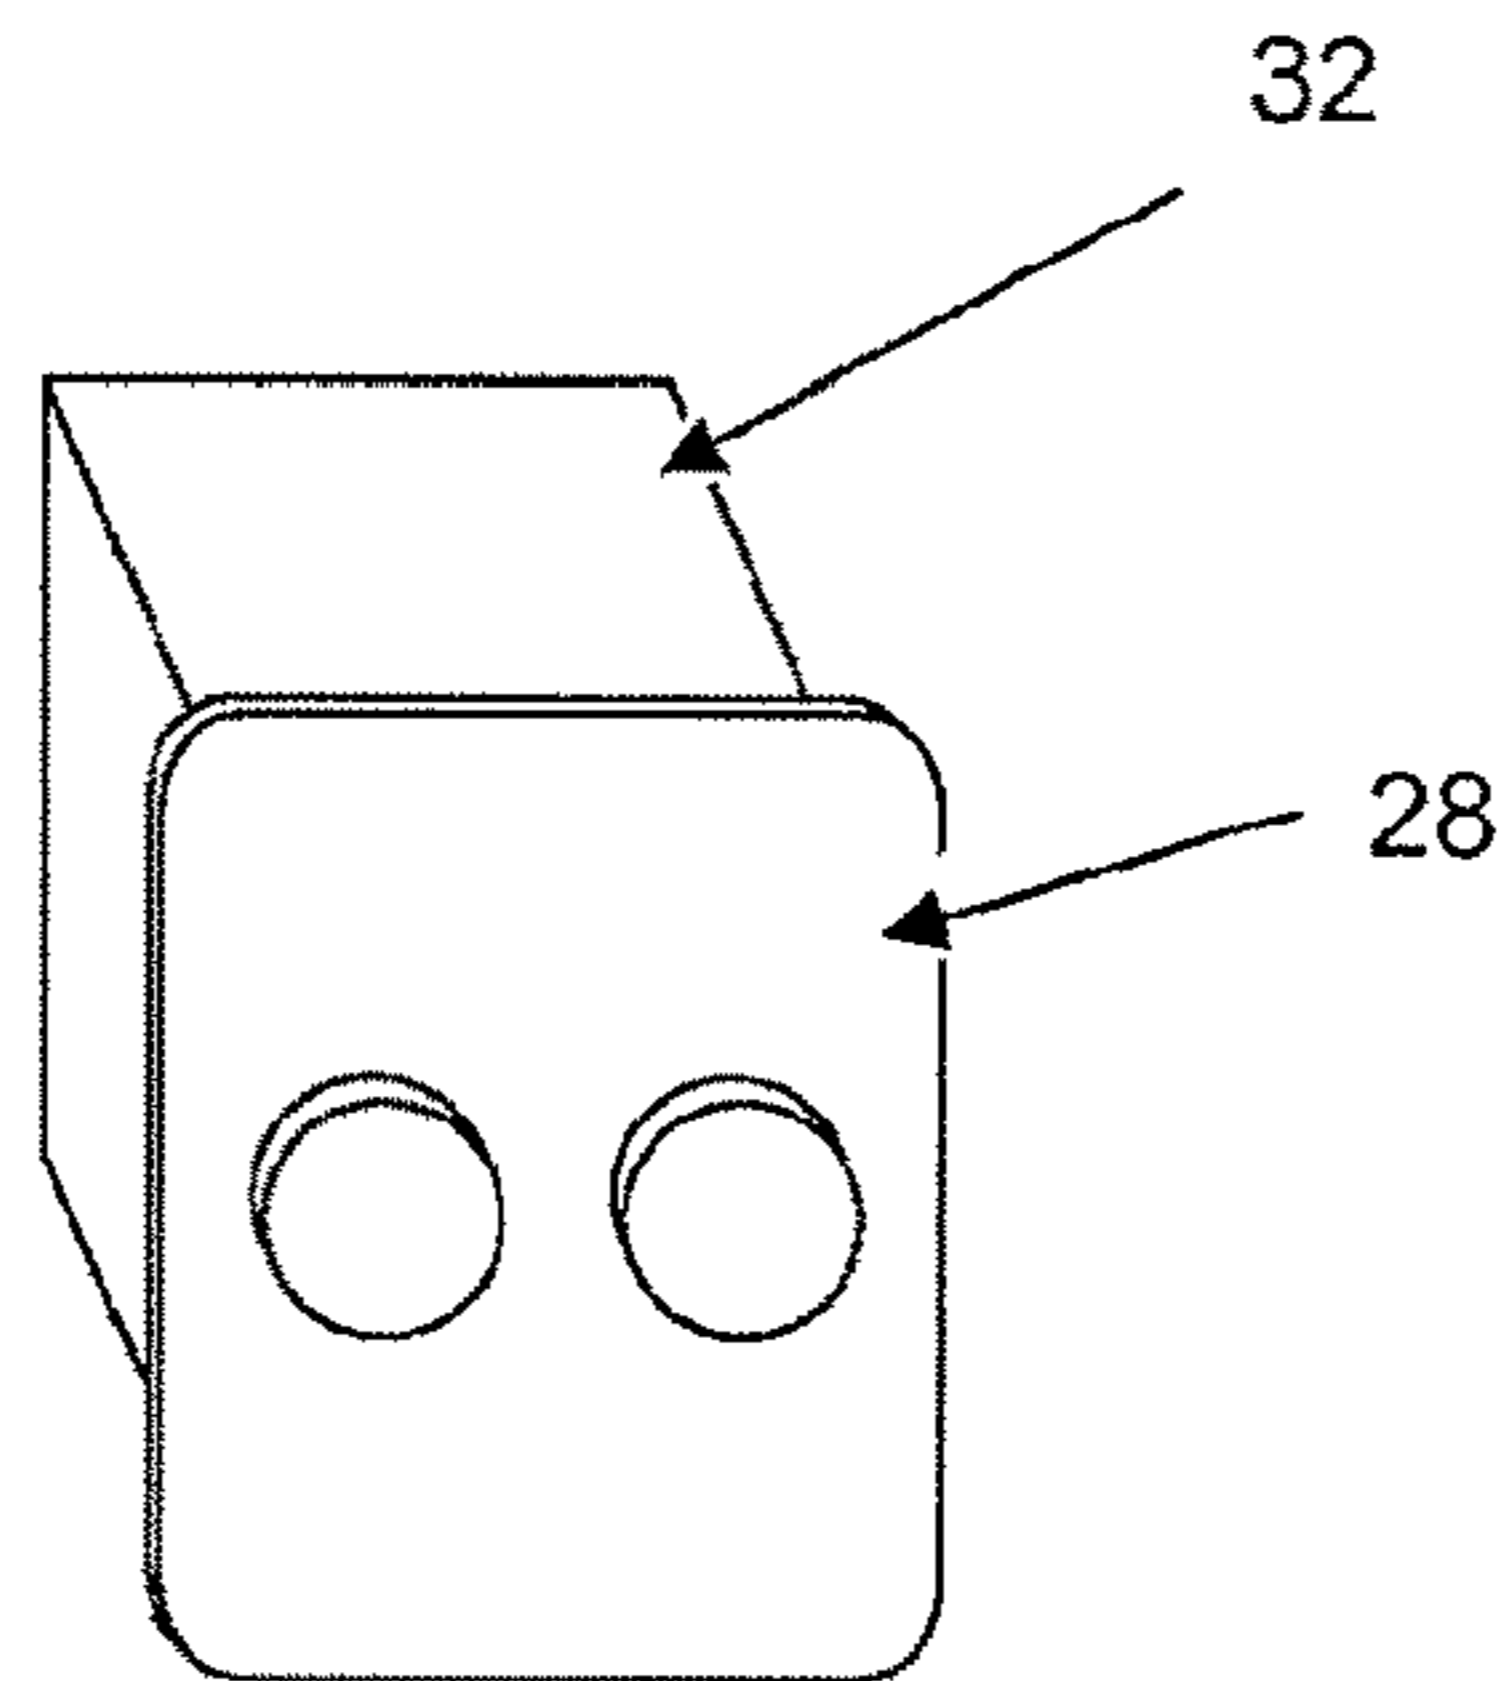


Fig. 4c

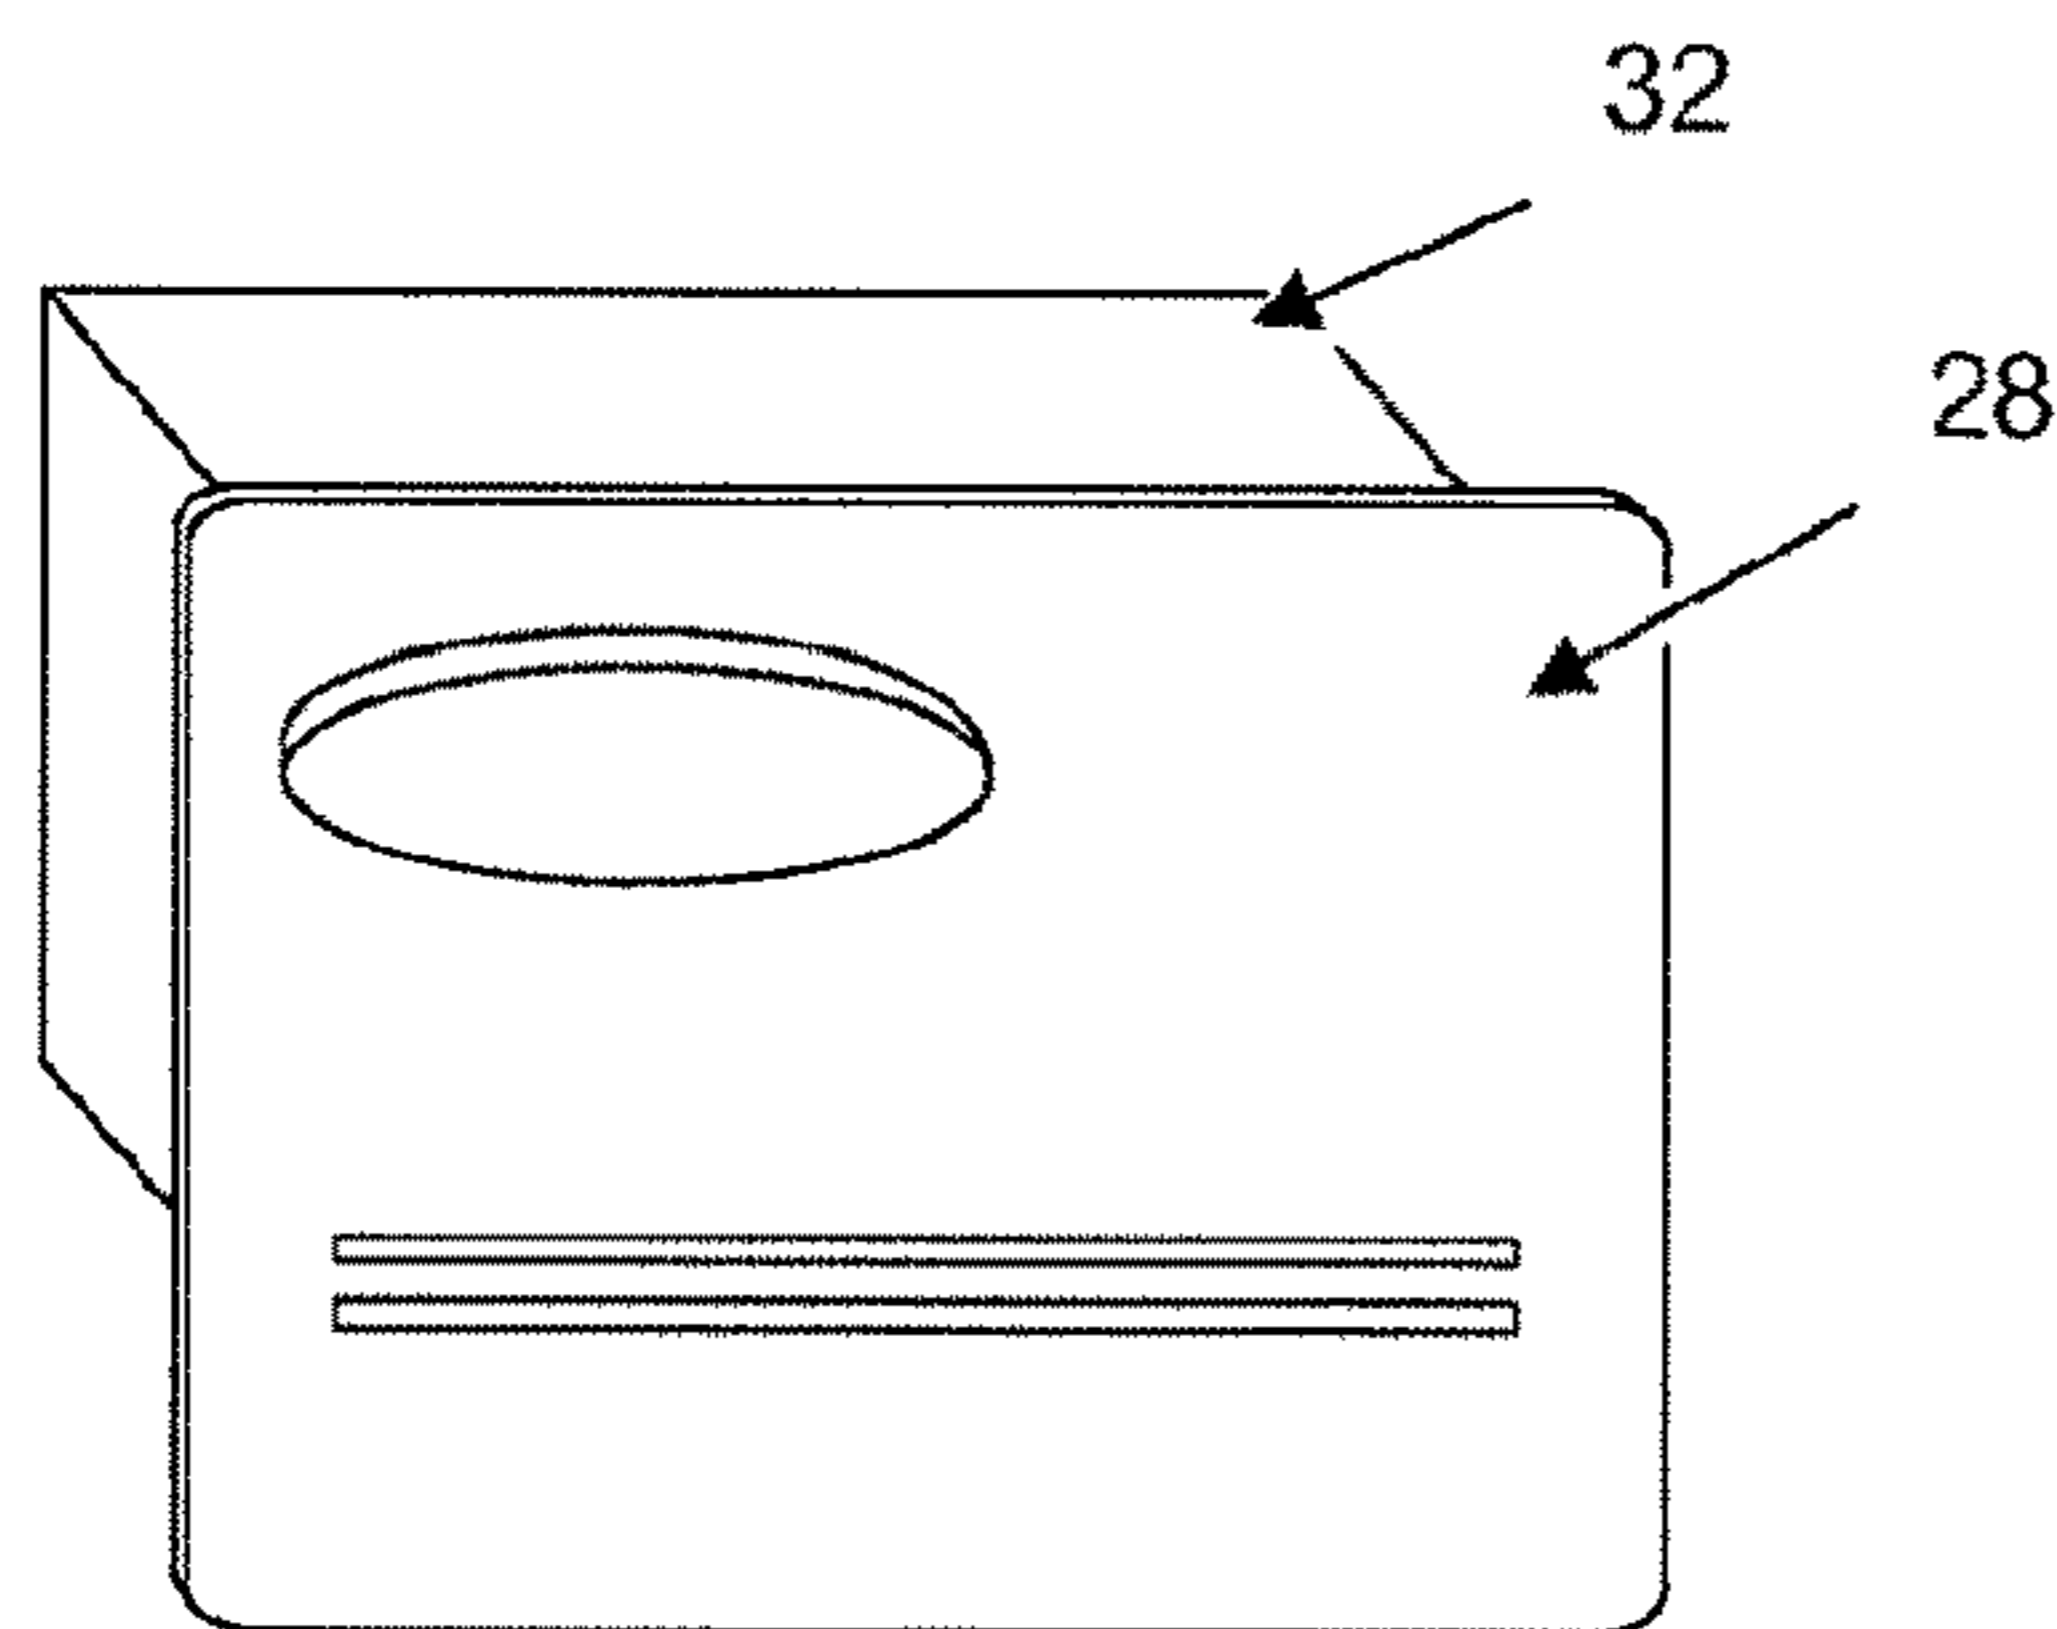


Fig. 4d

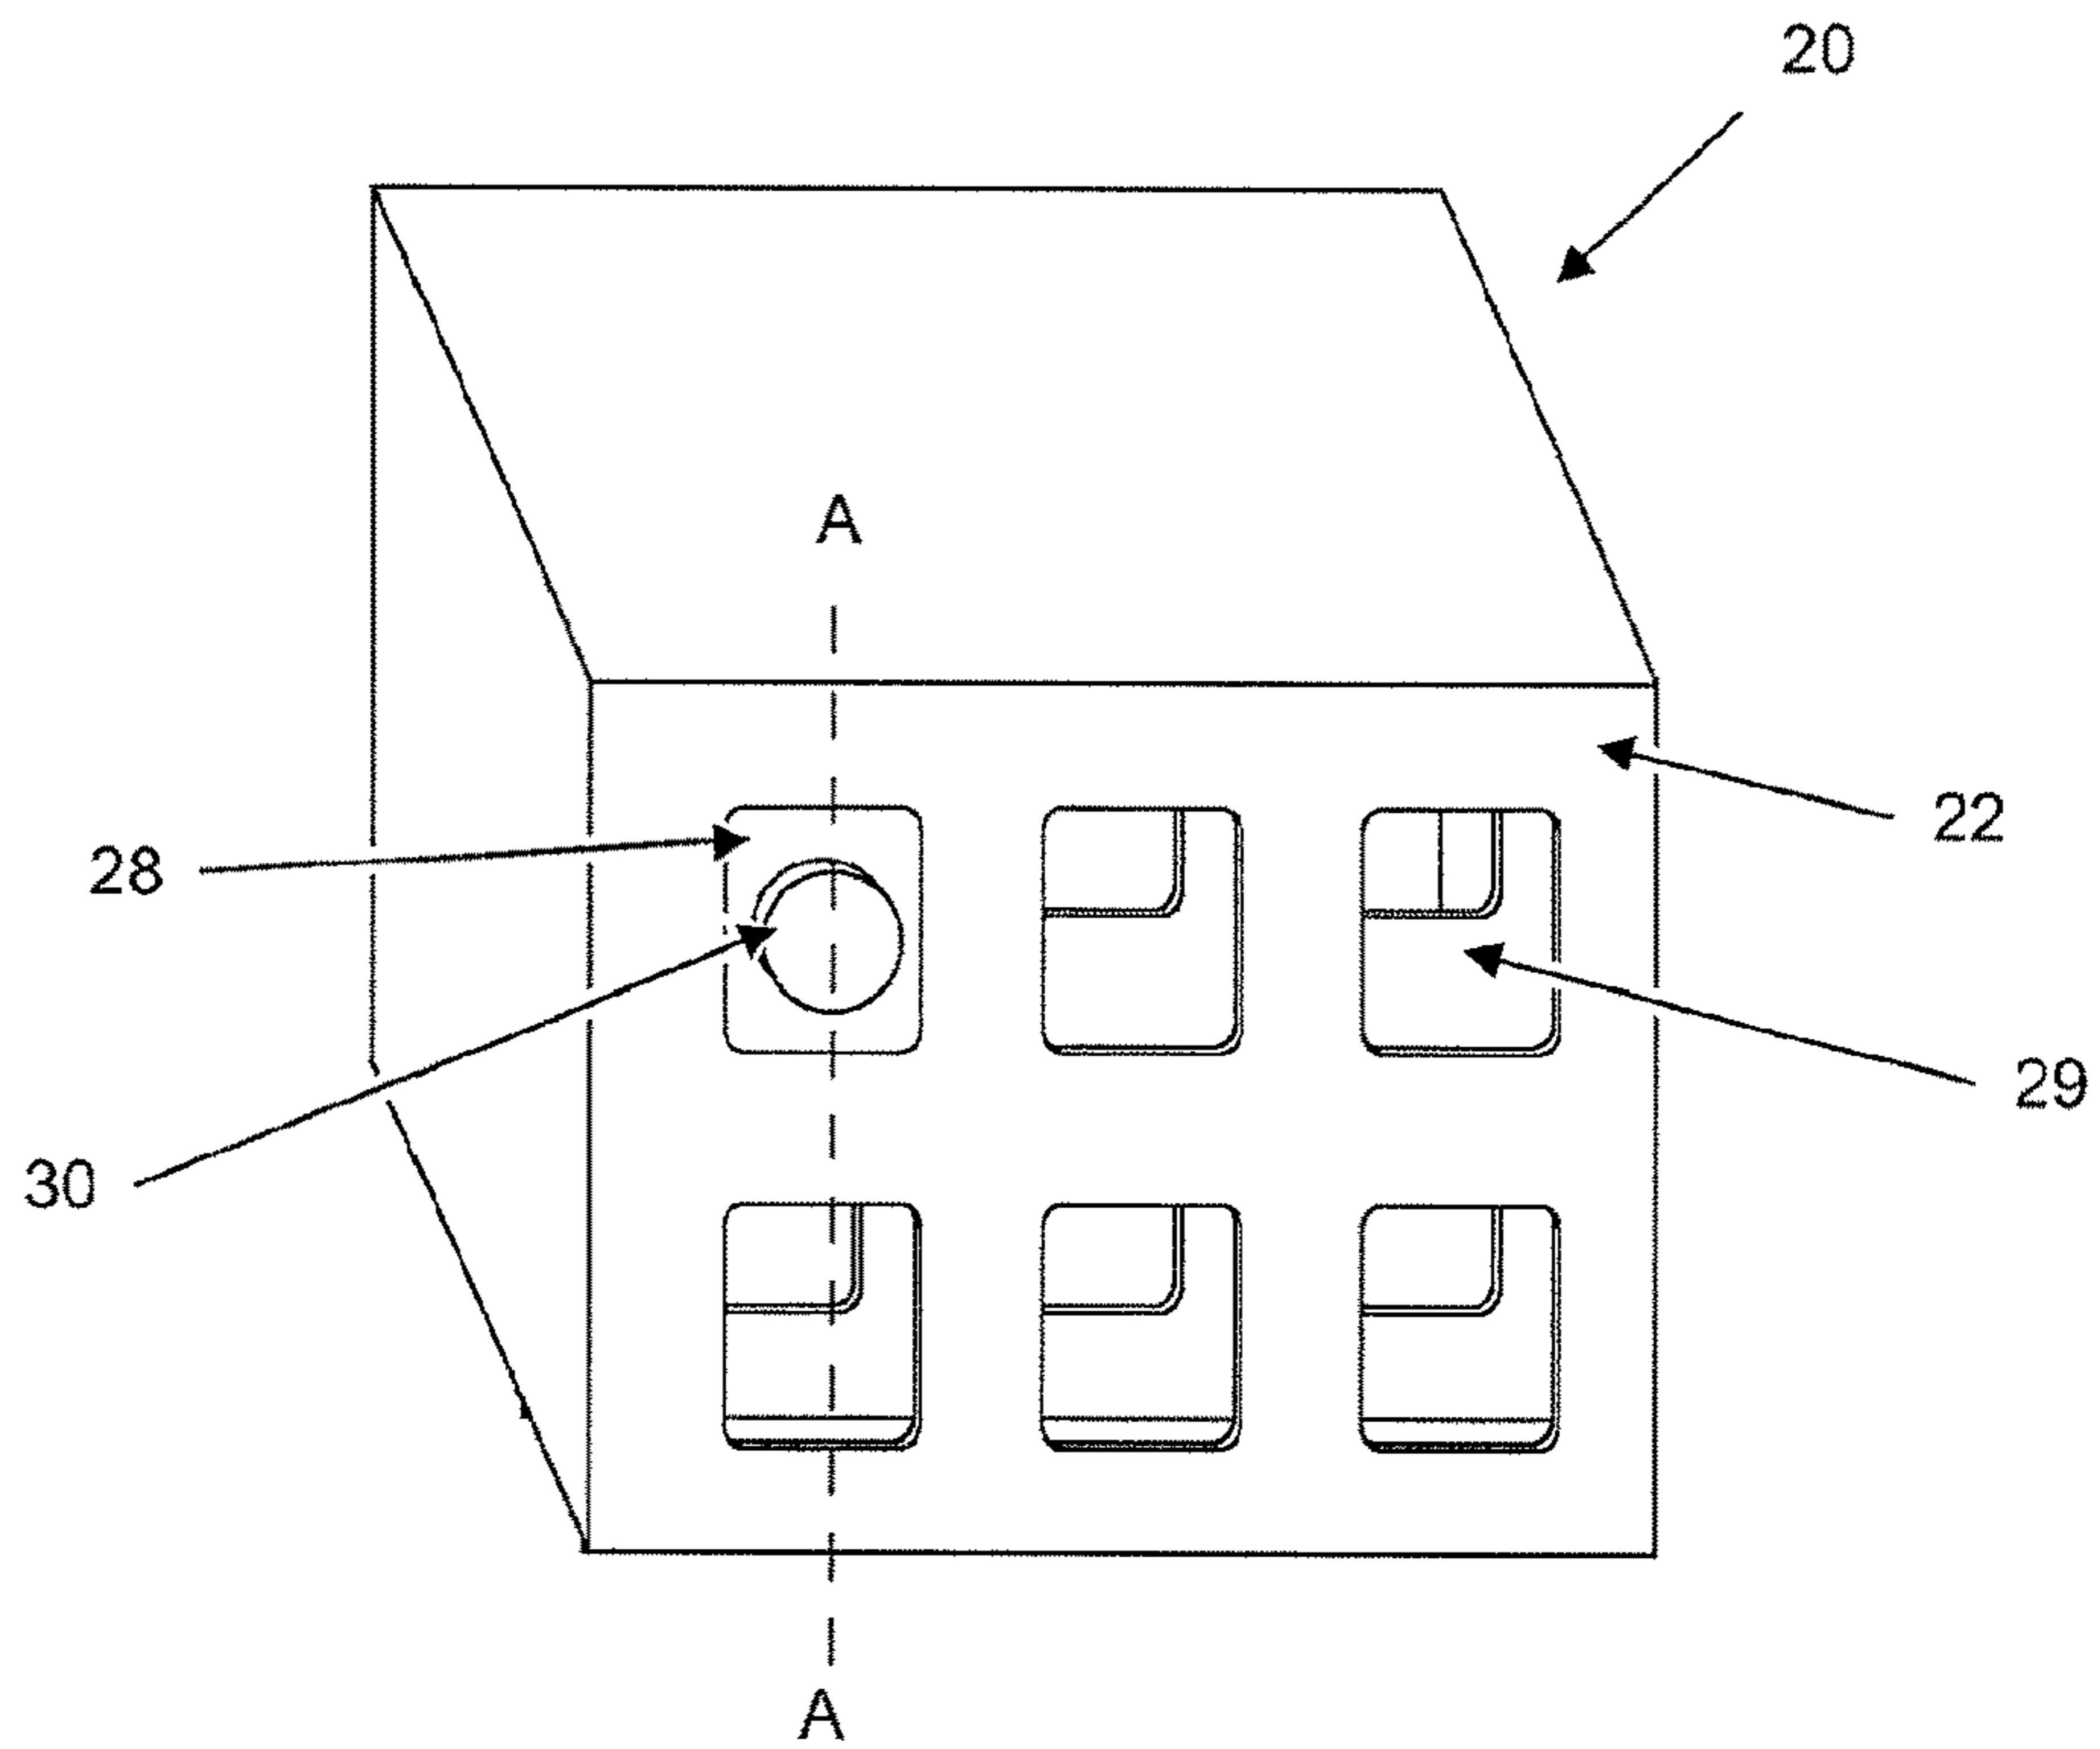


Fig. 5a

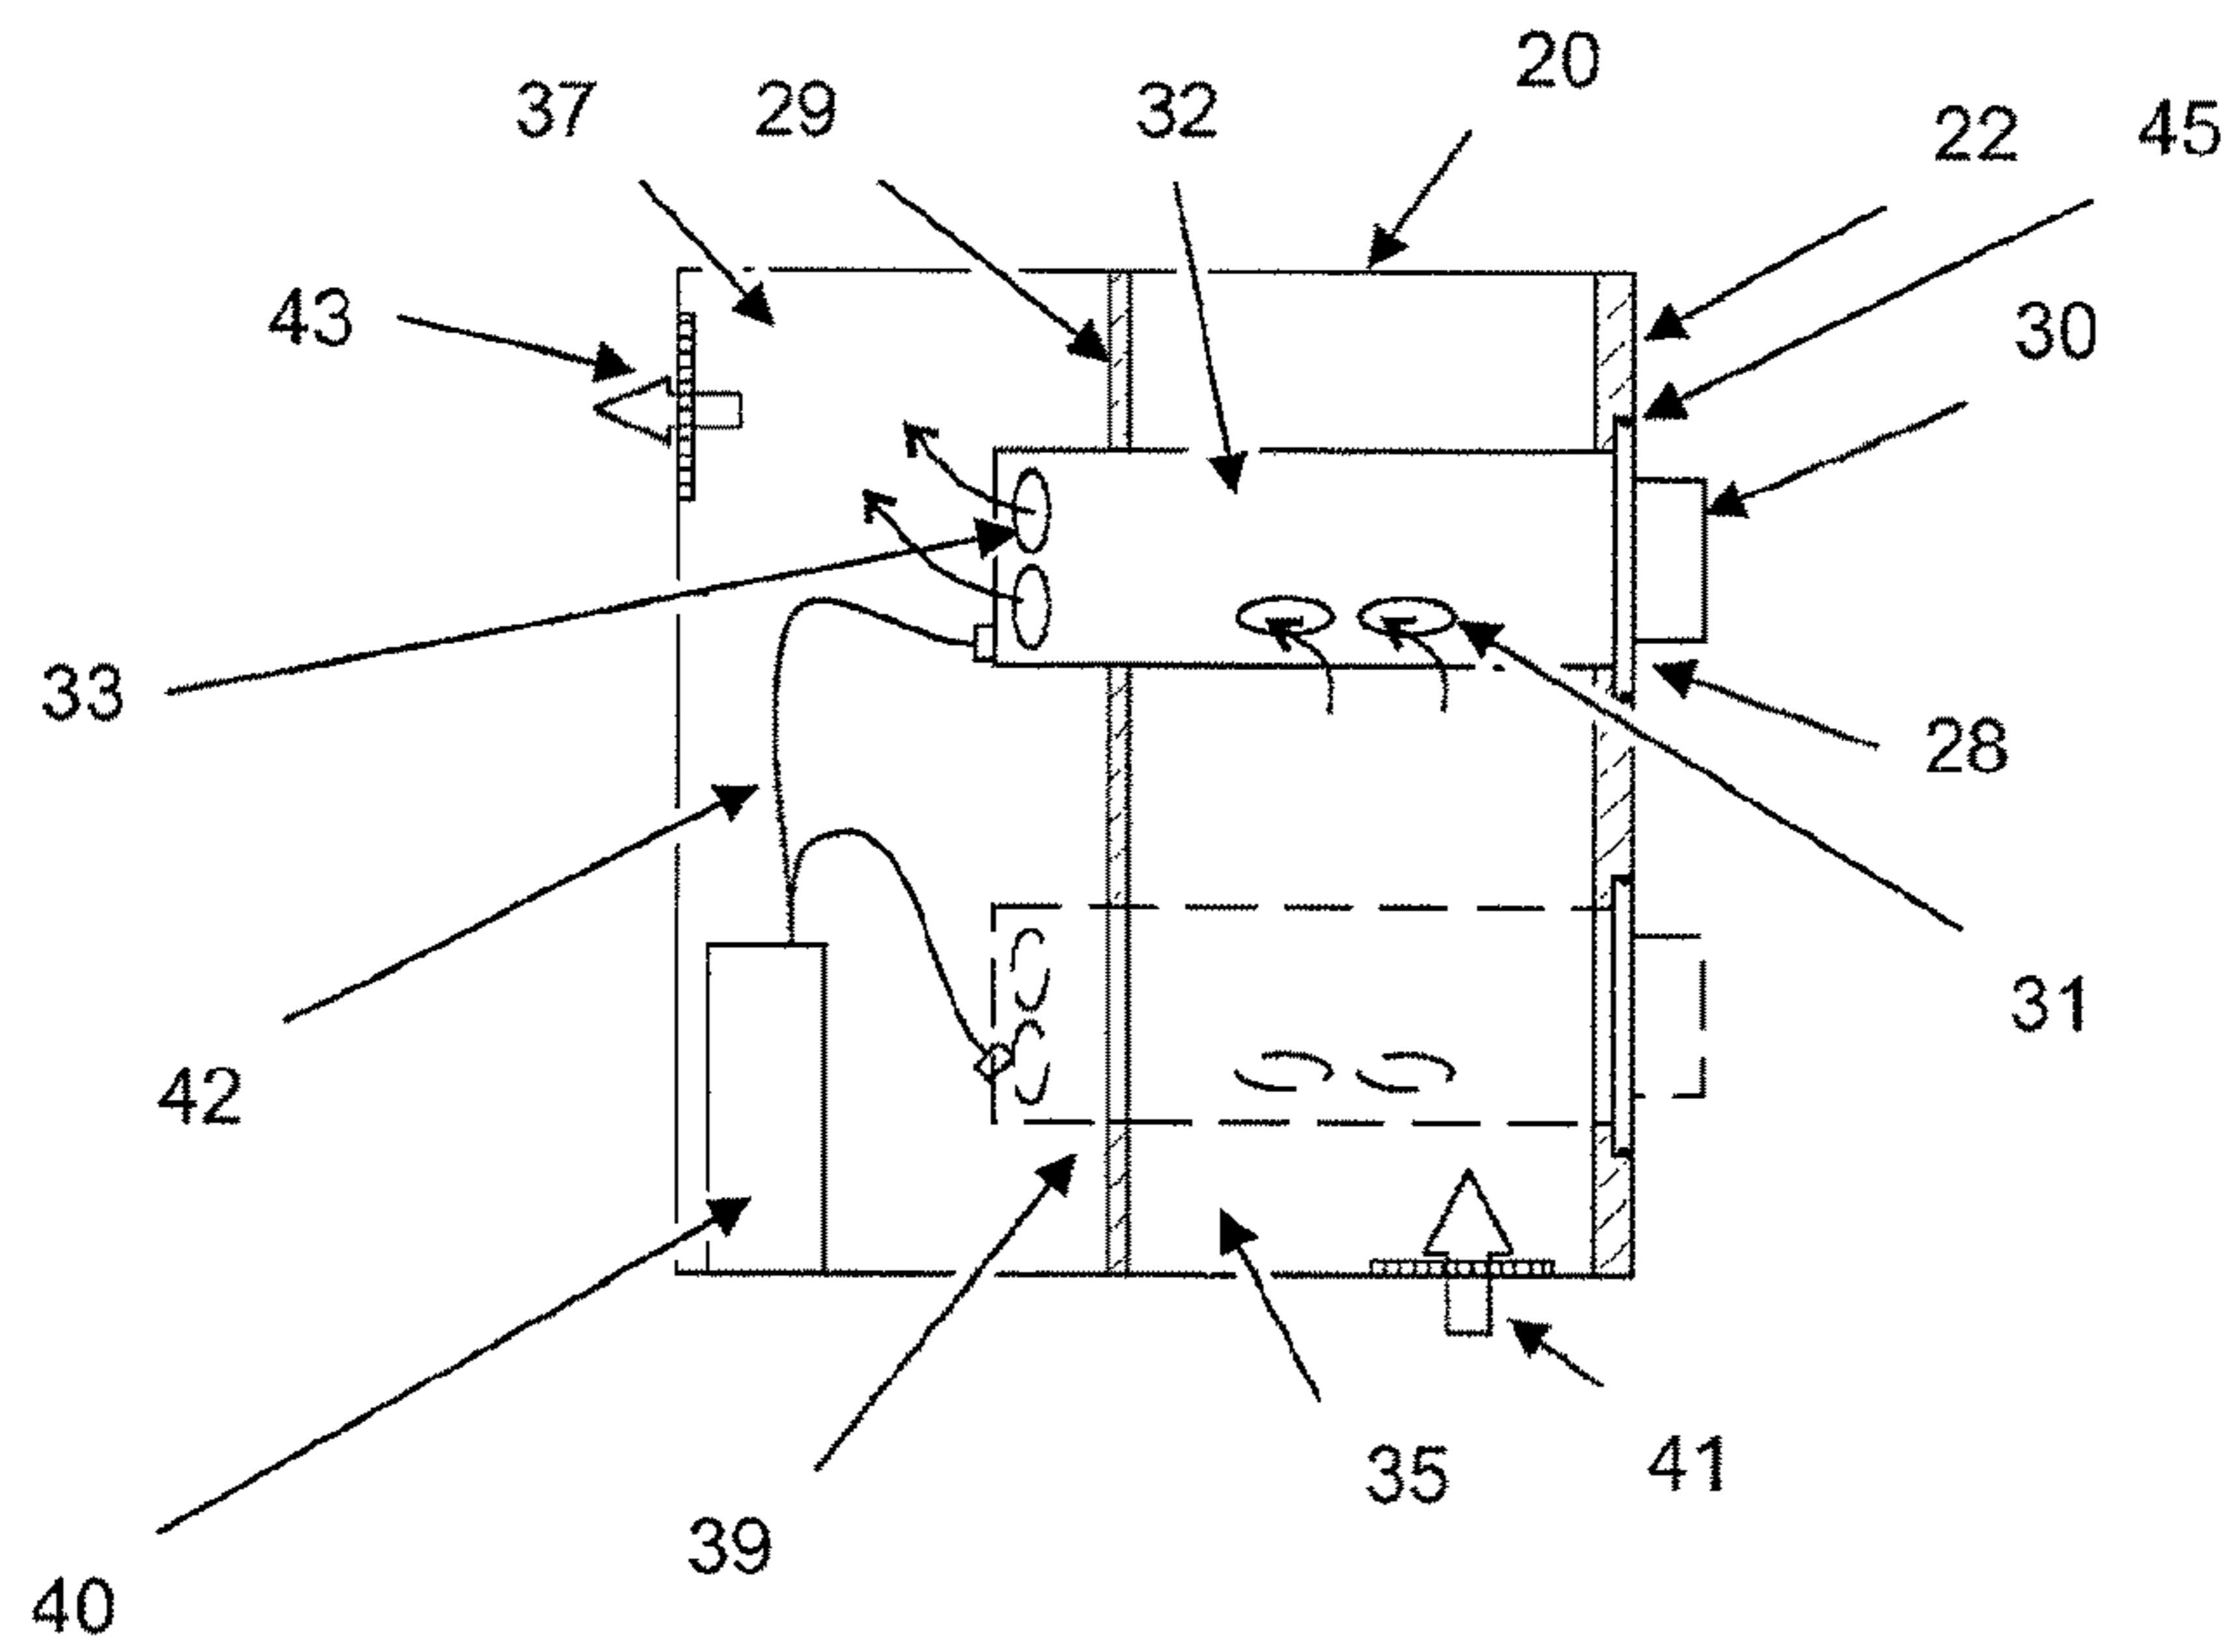


Fig. 5b



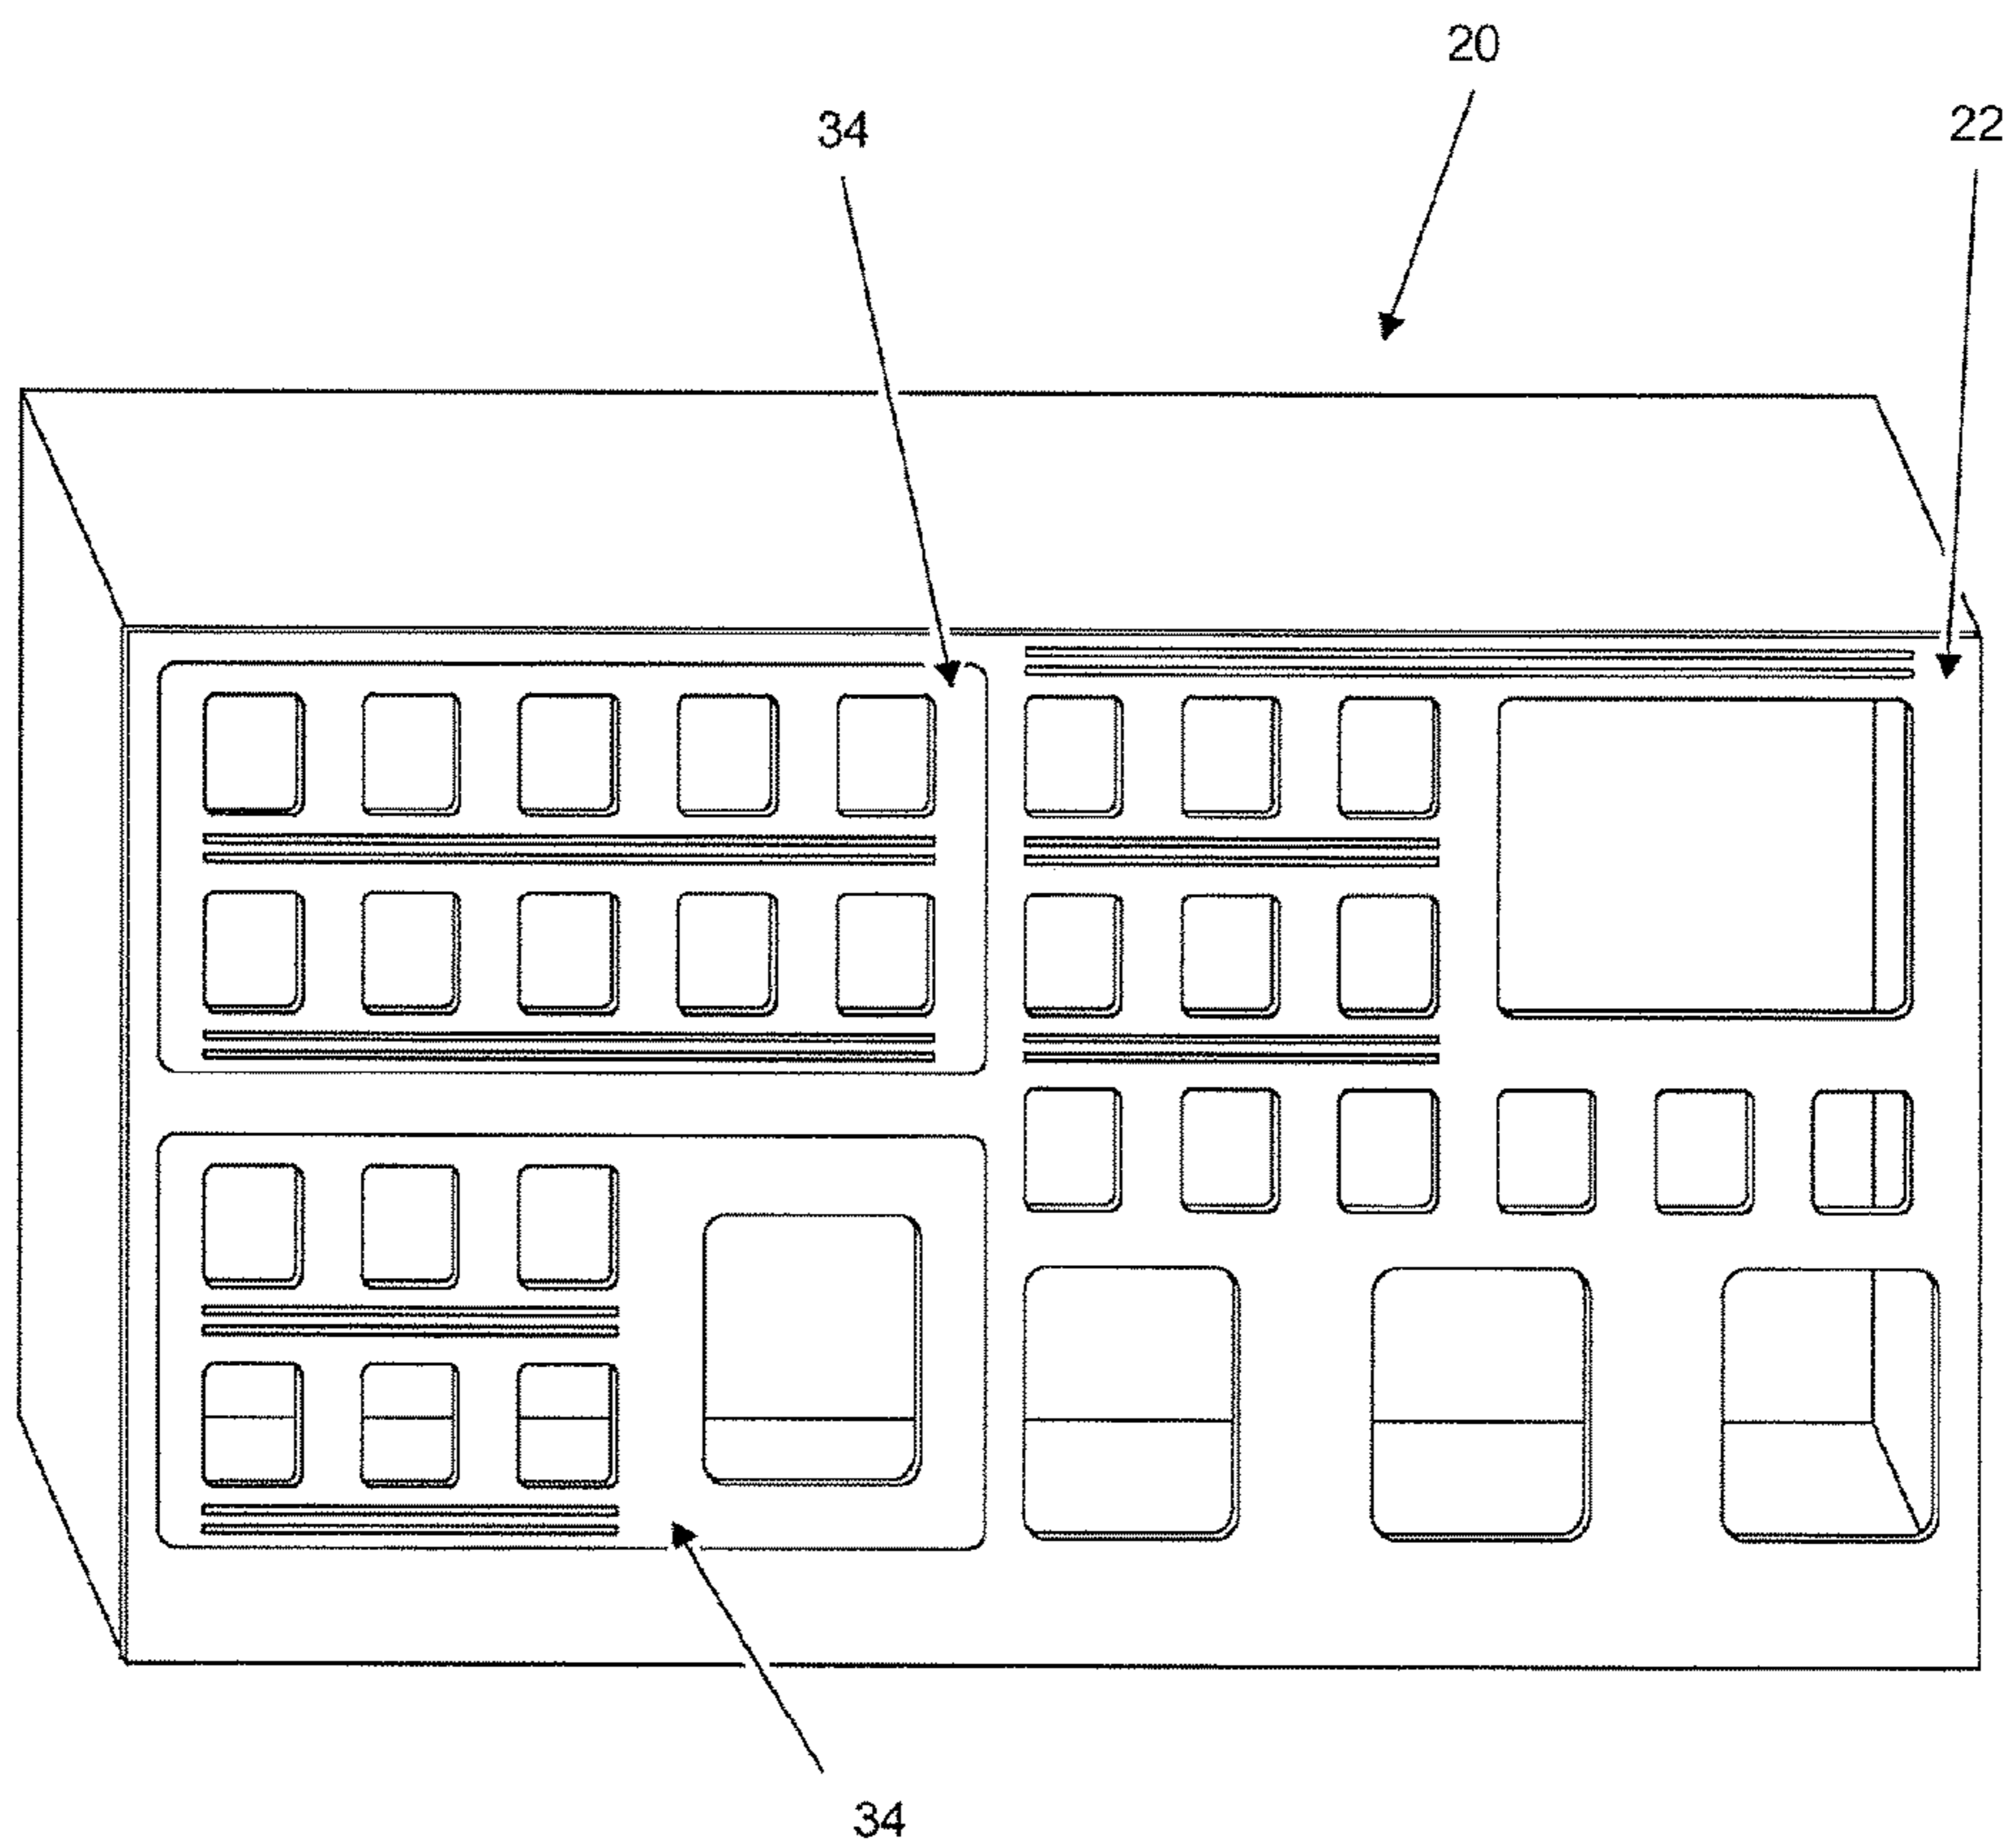


Fig. 6

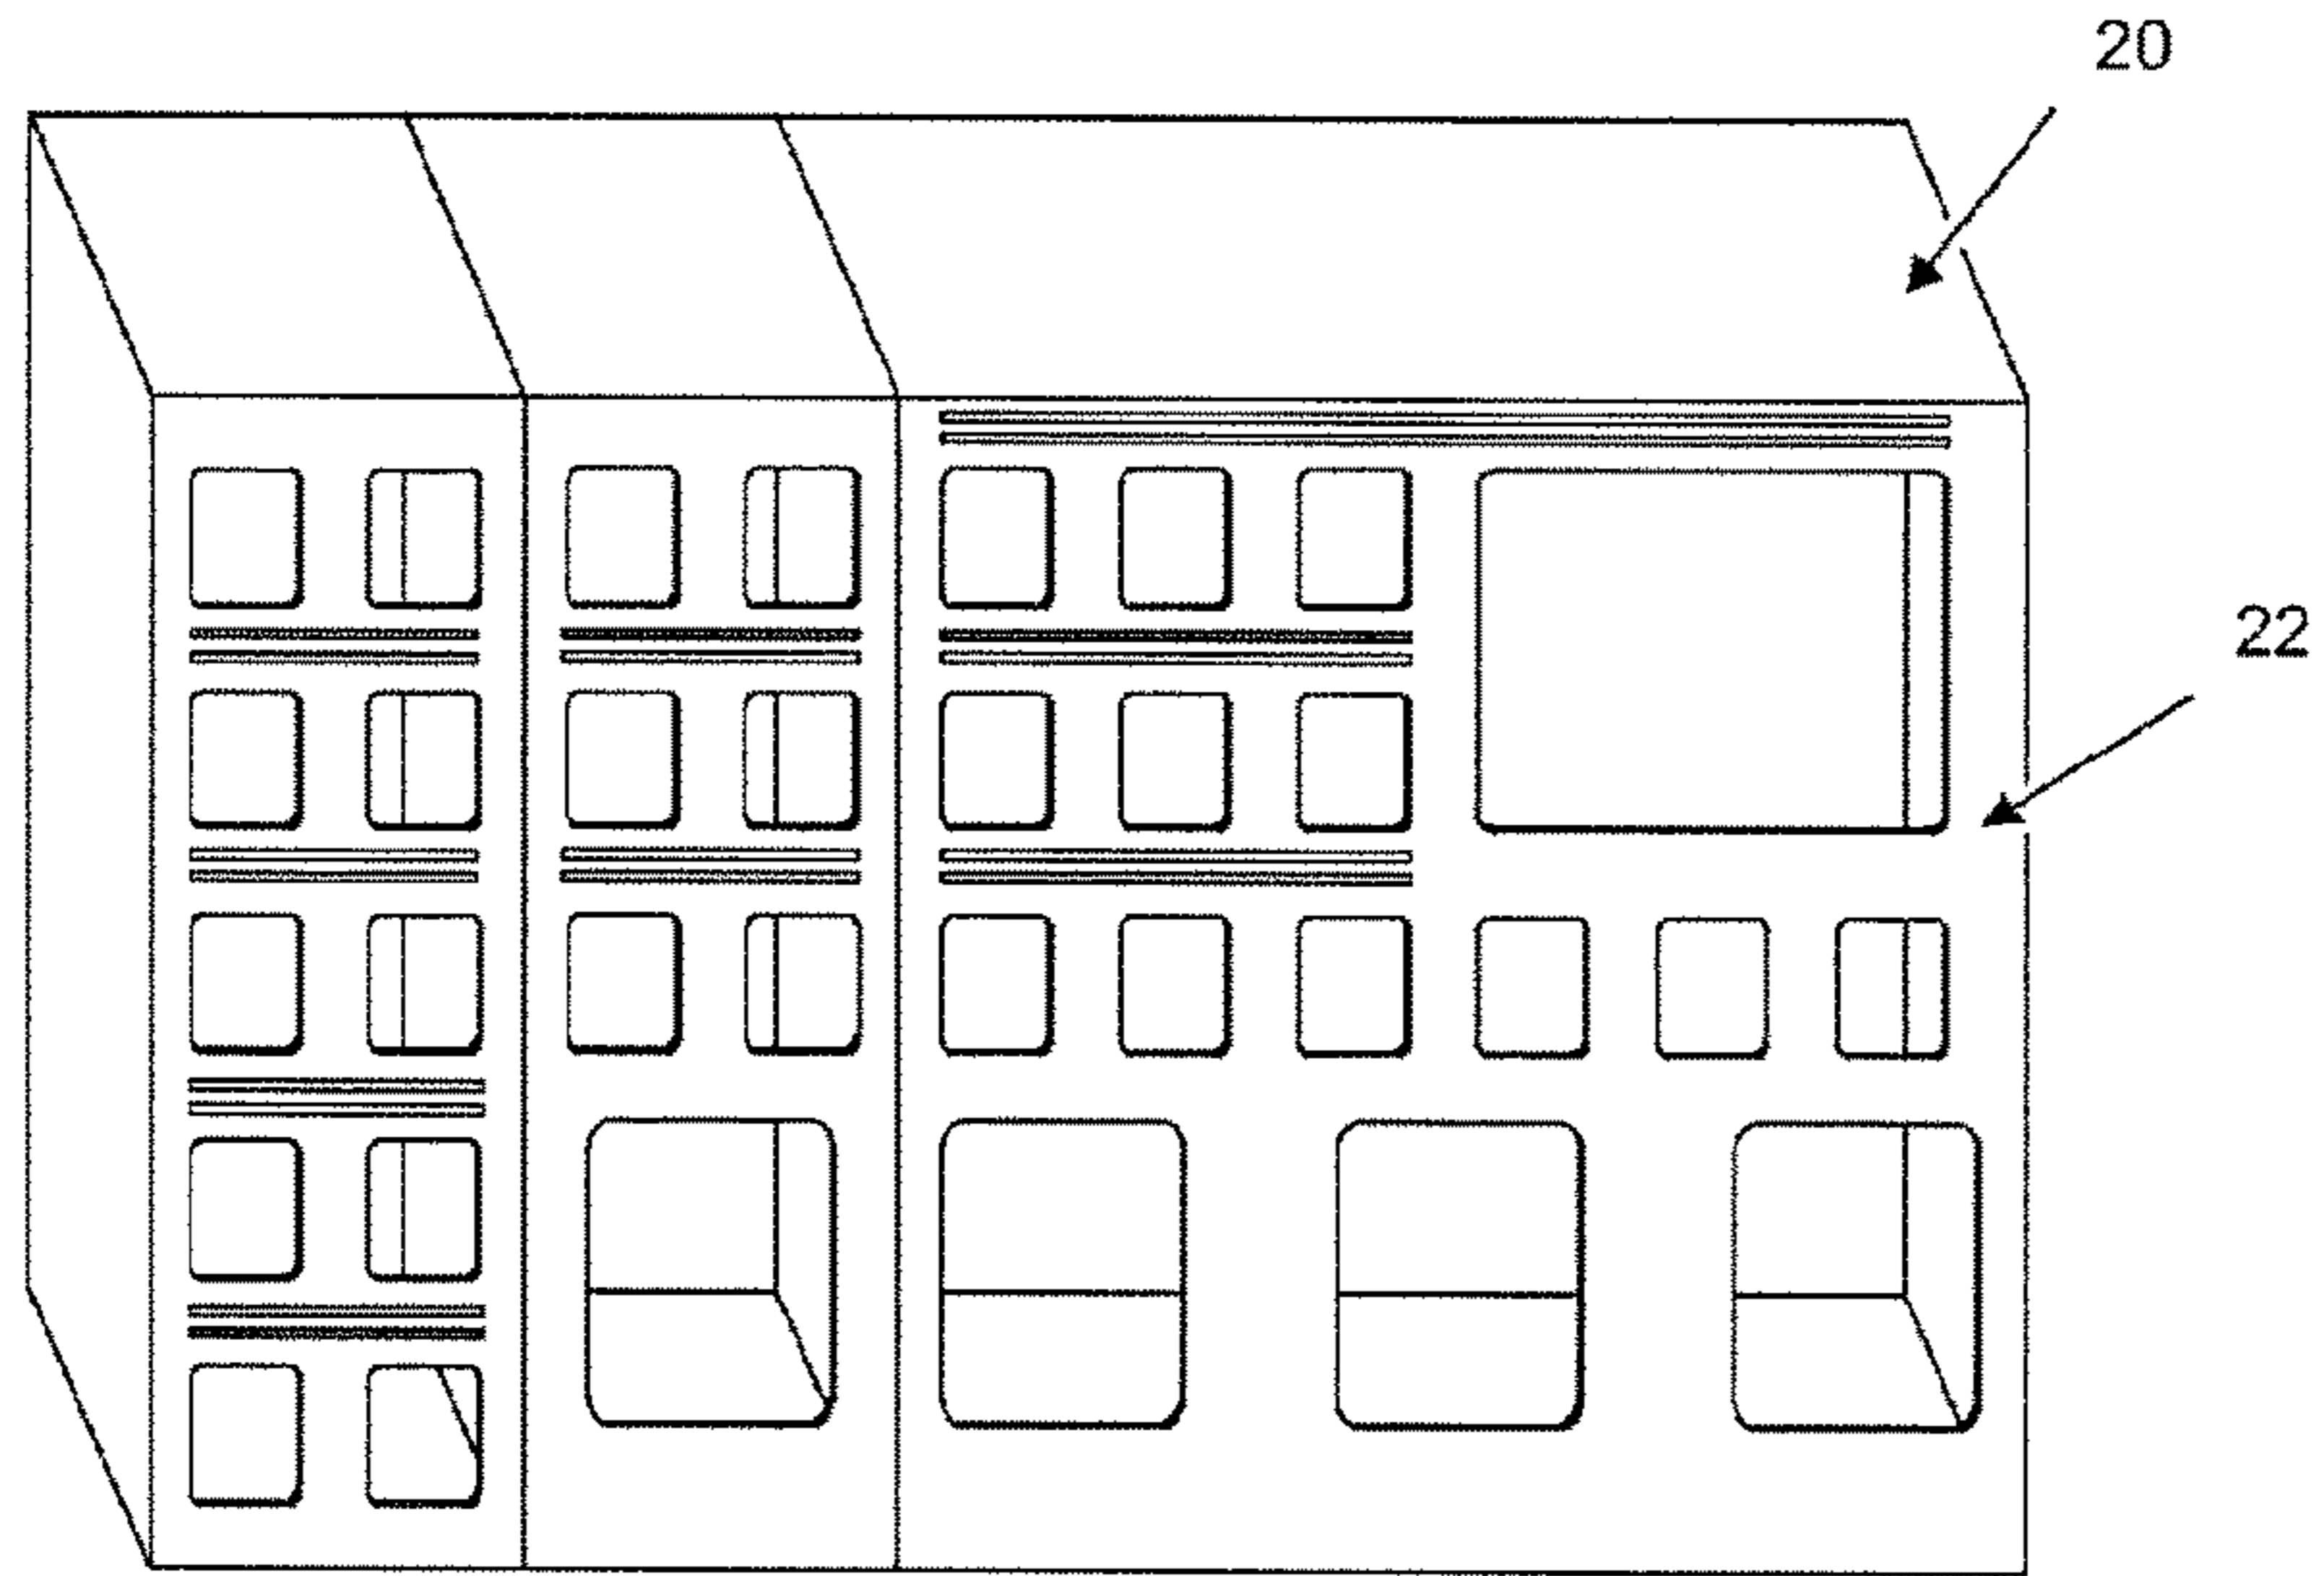


Fig. 7a

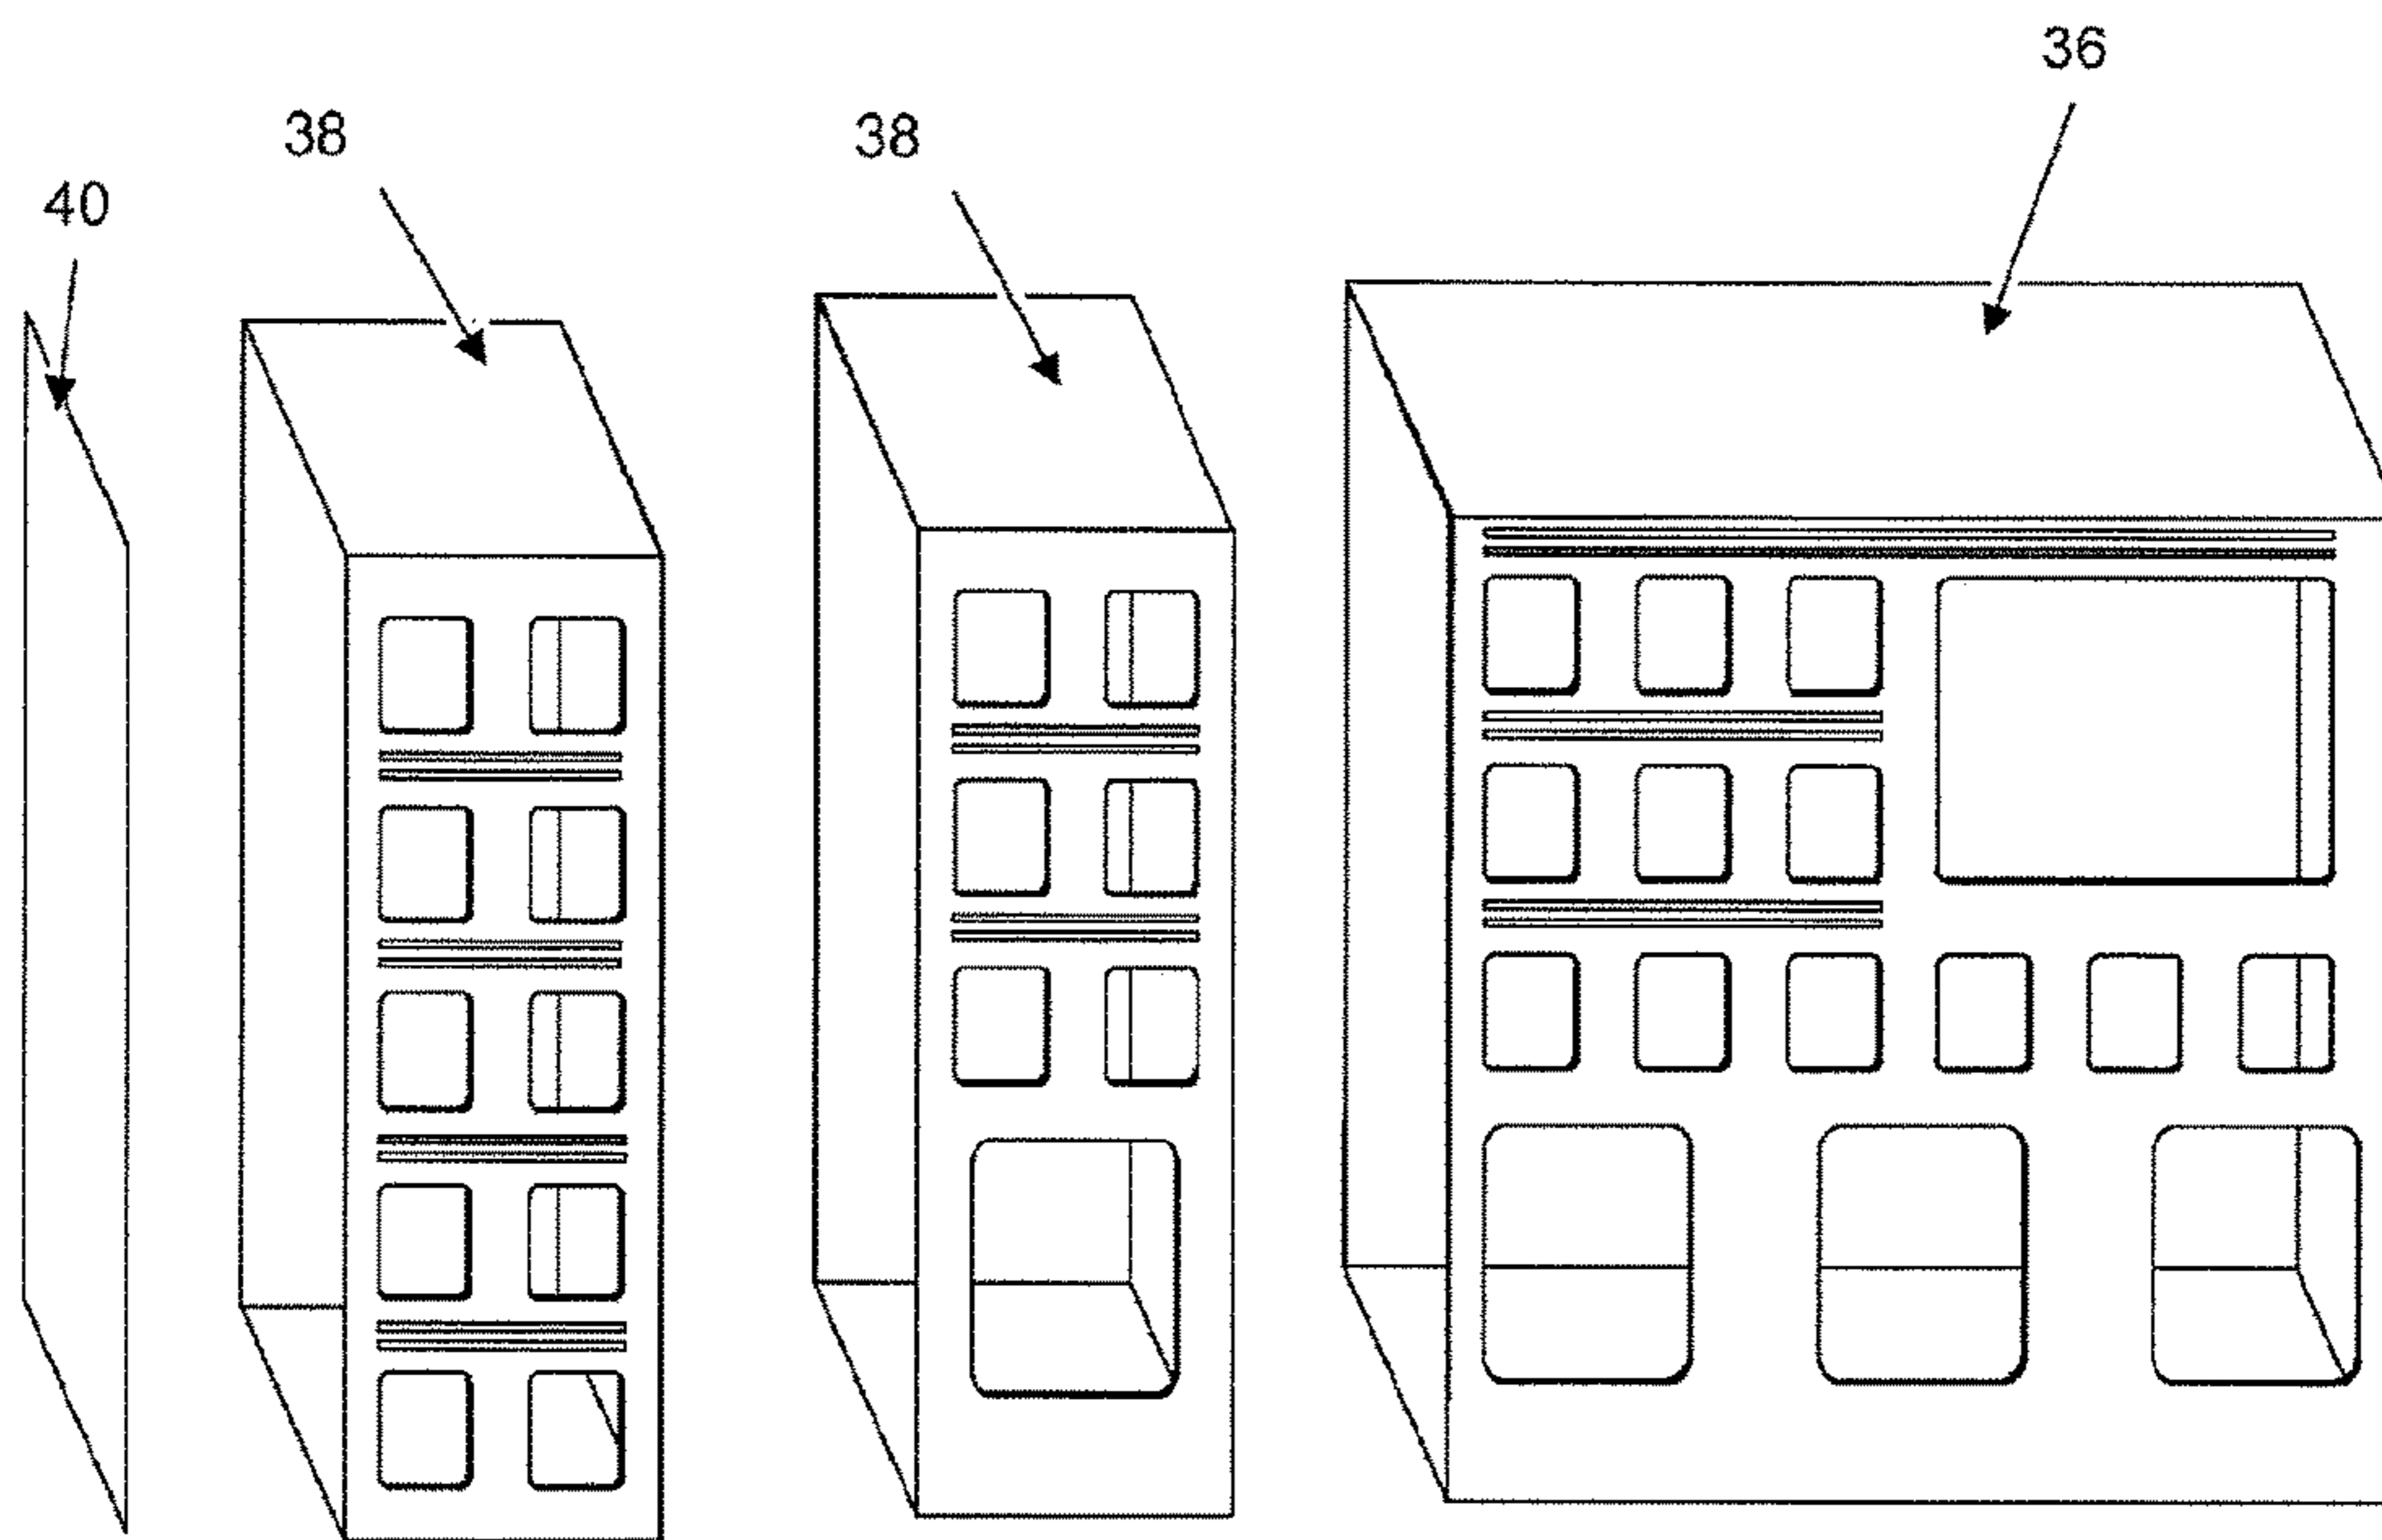
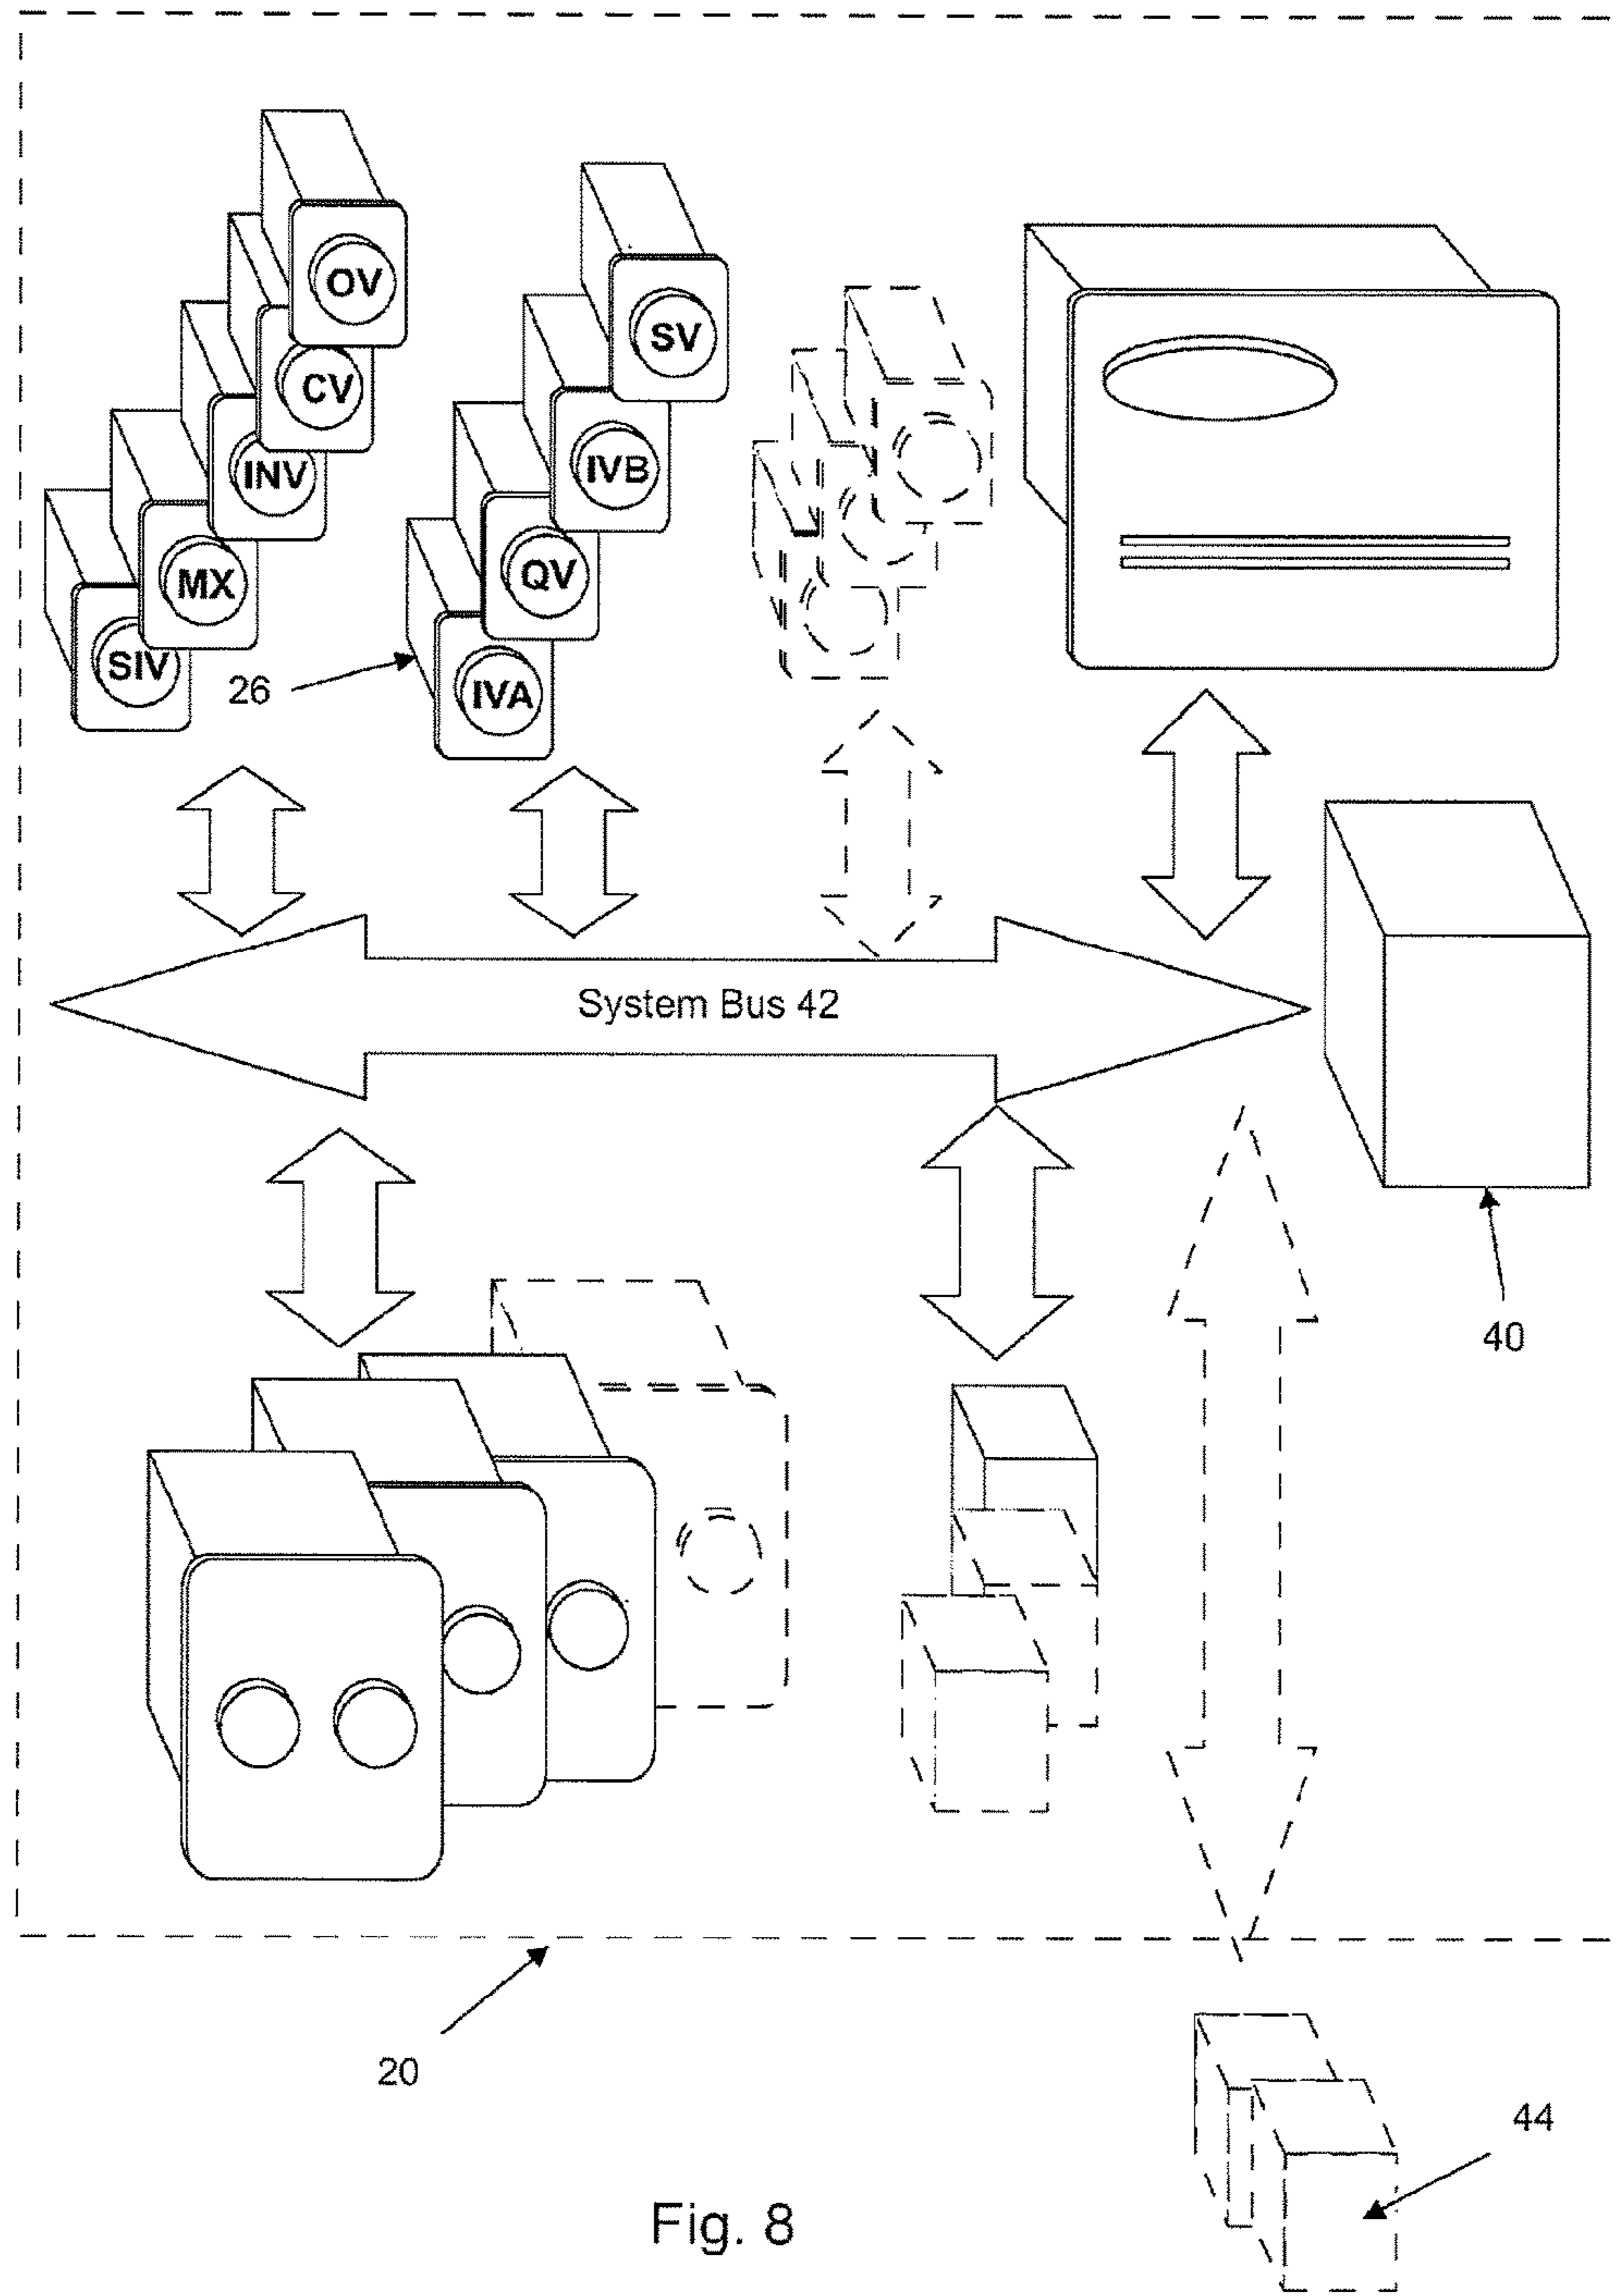


Fig. 7b



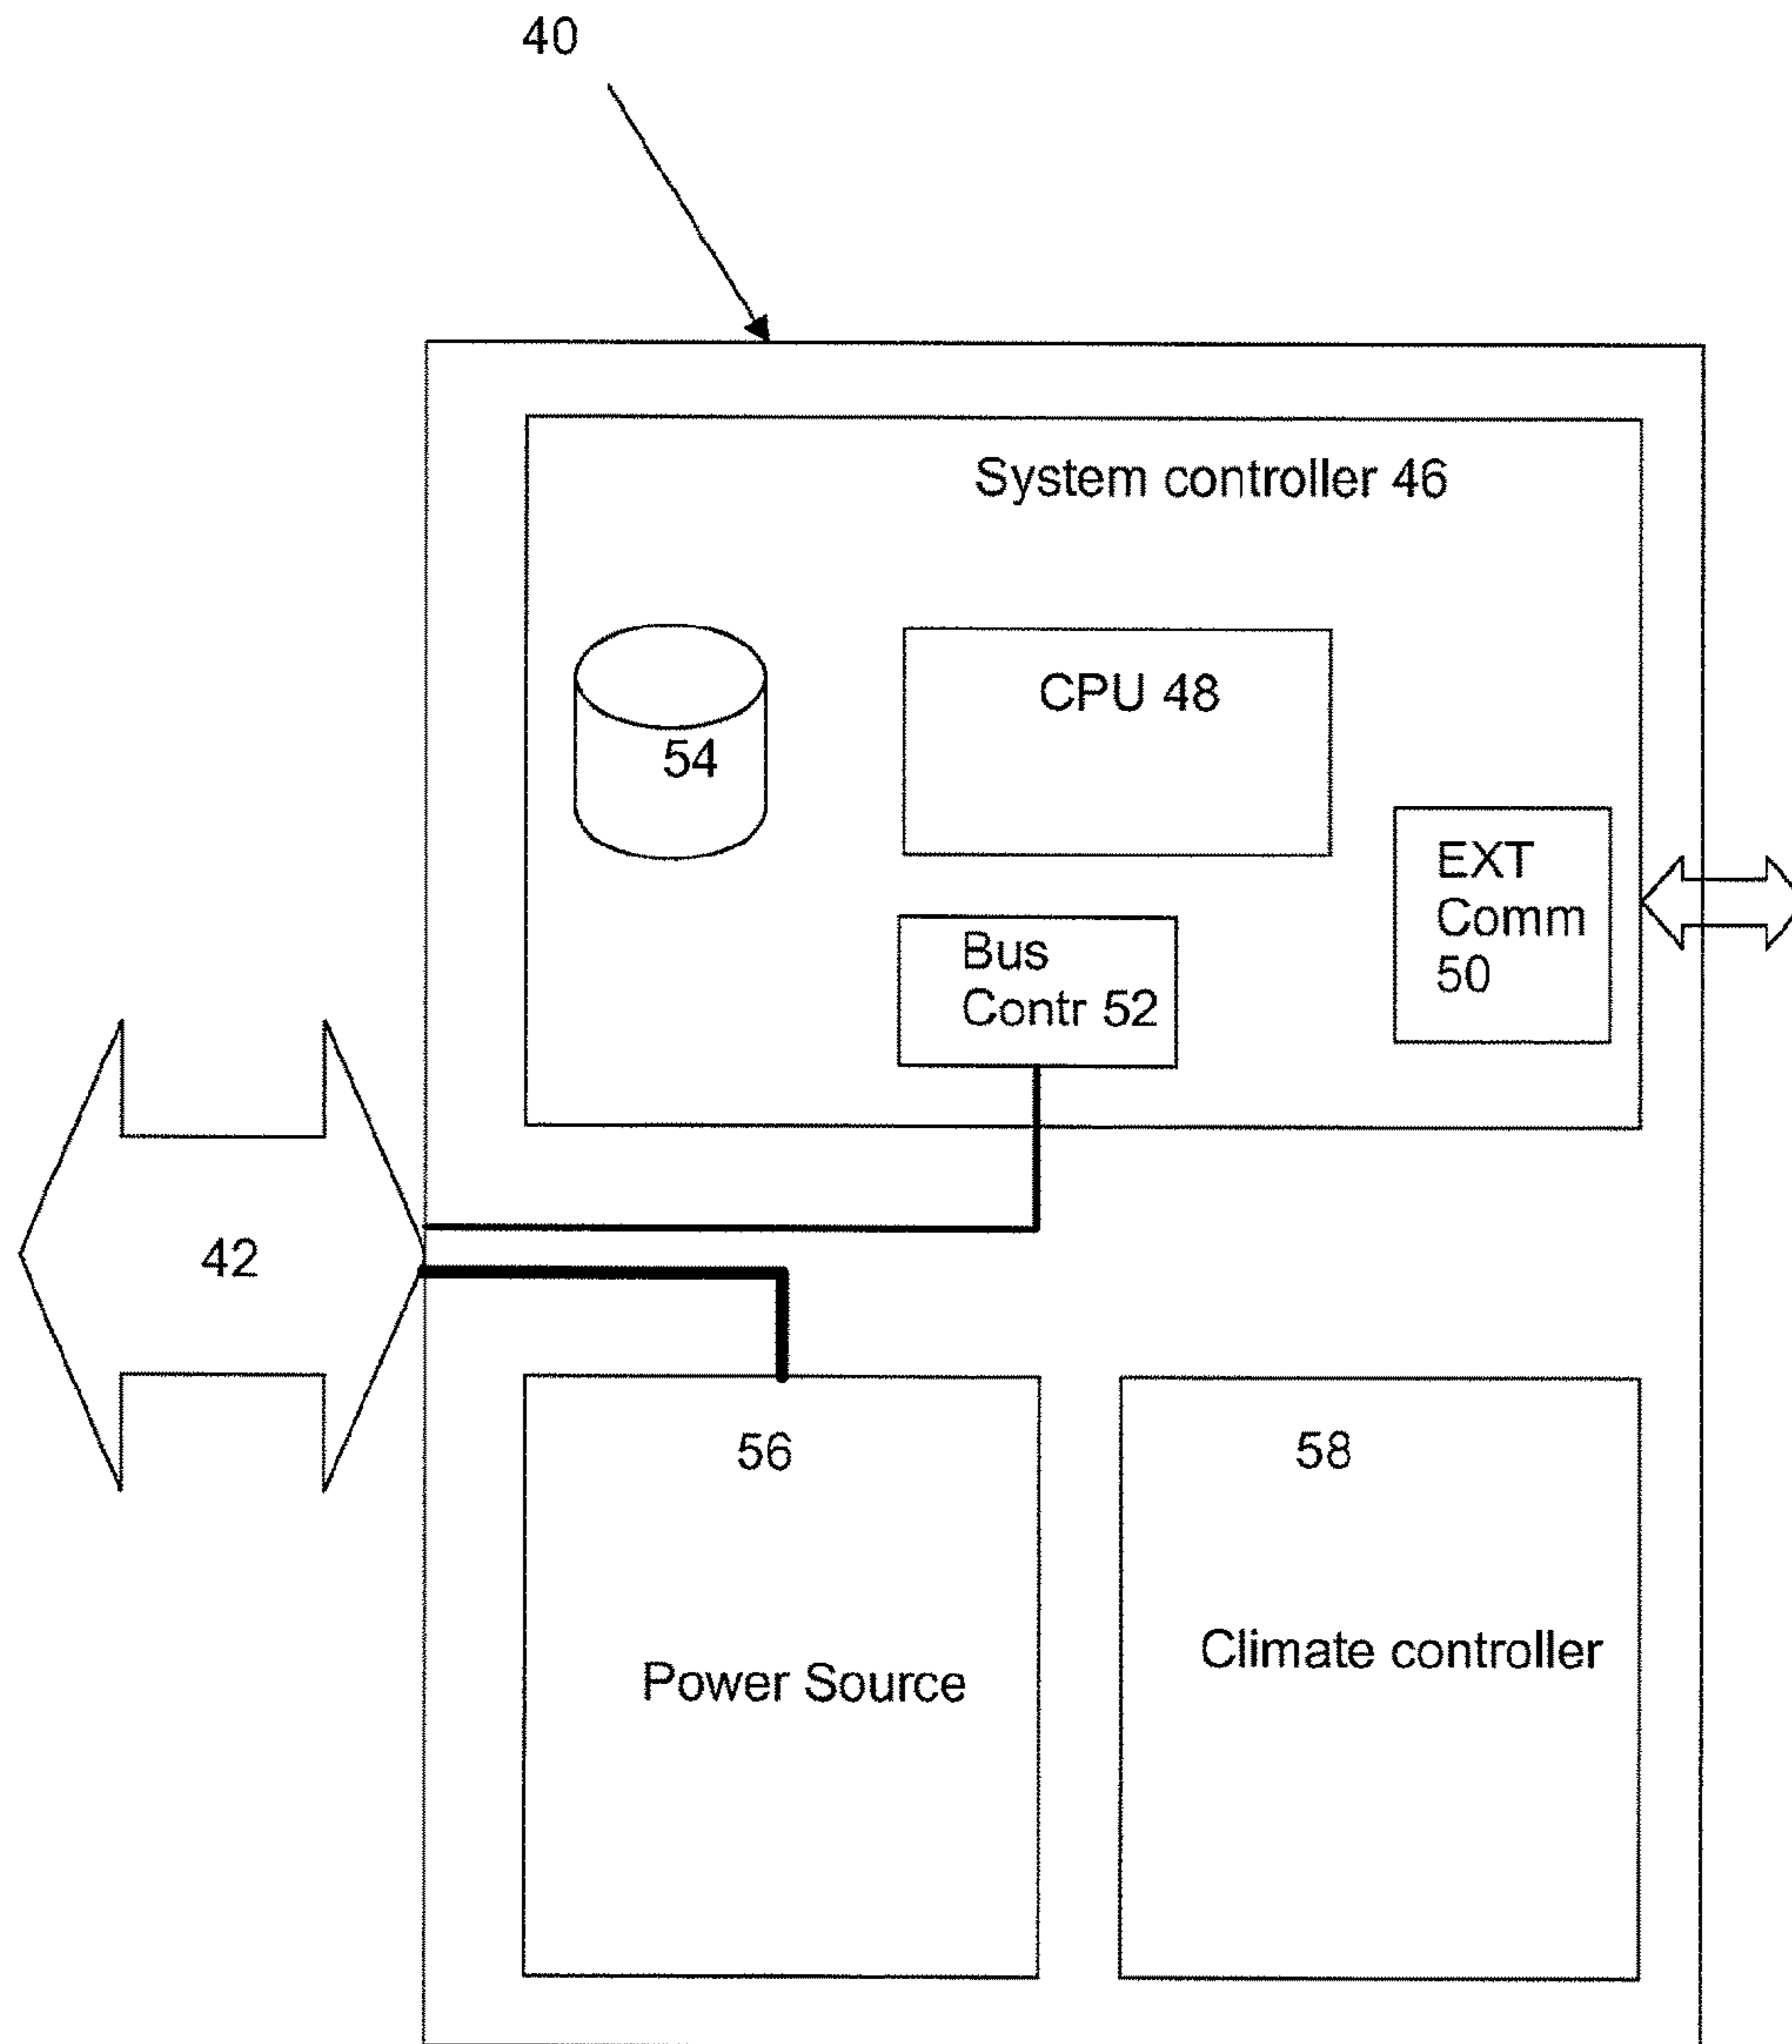


Fig. 9

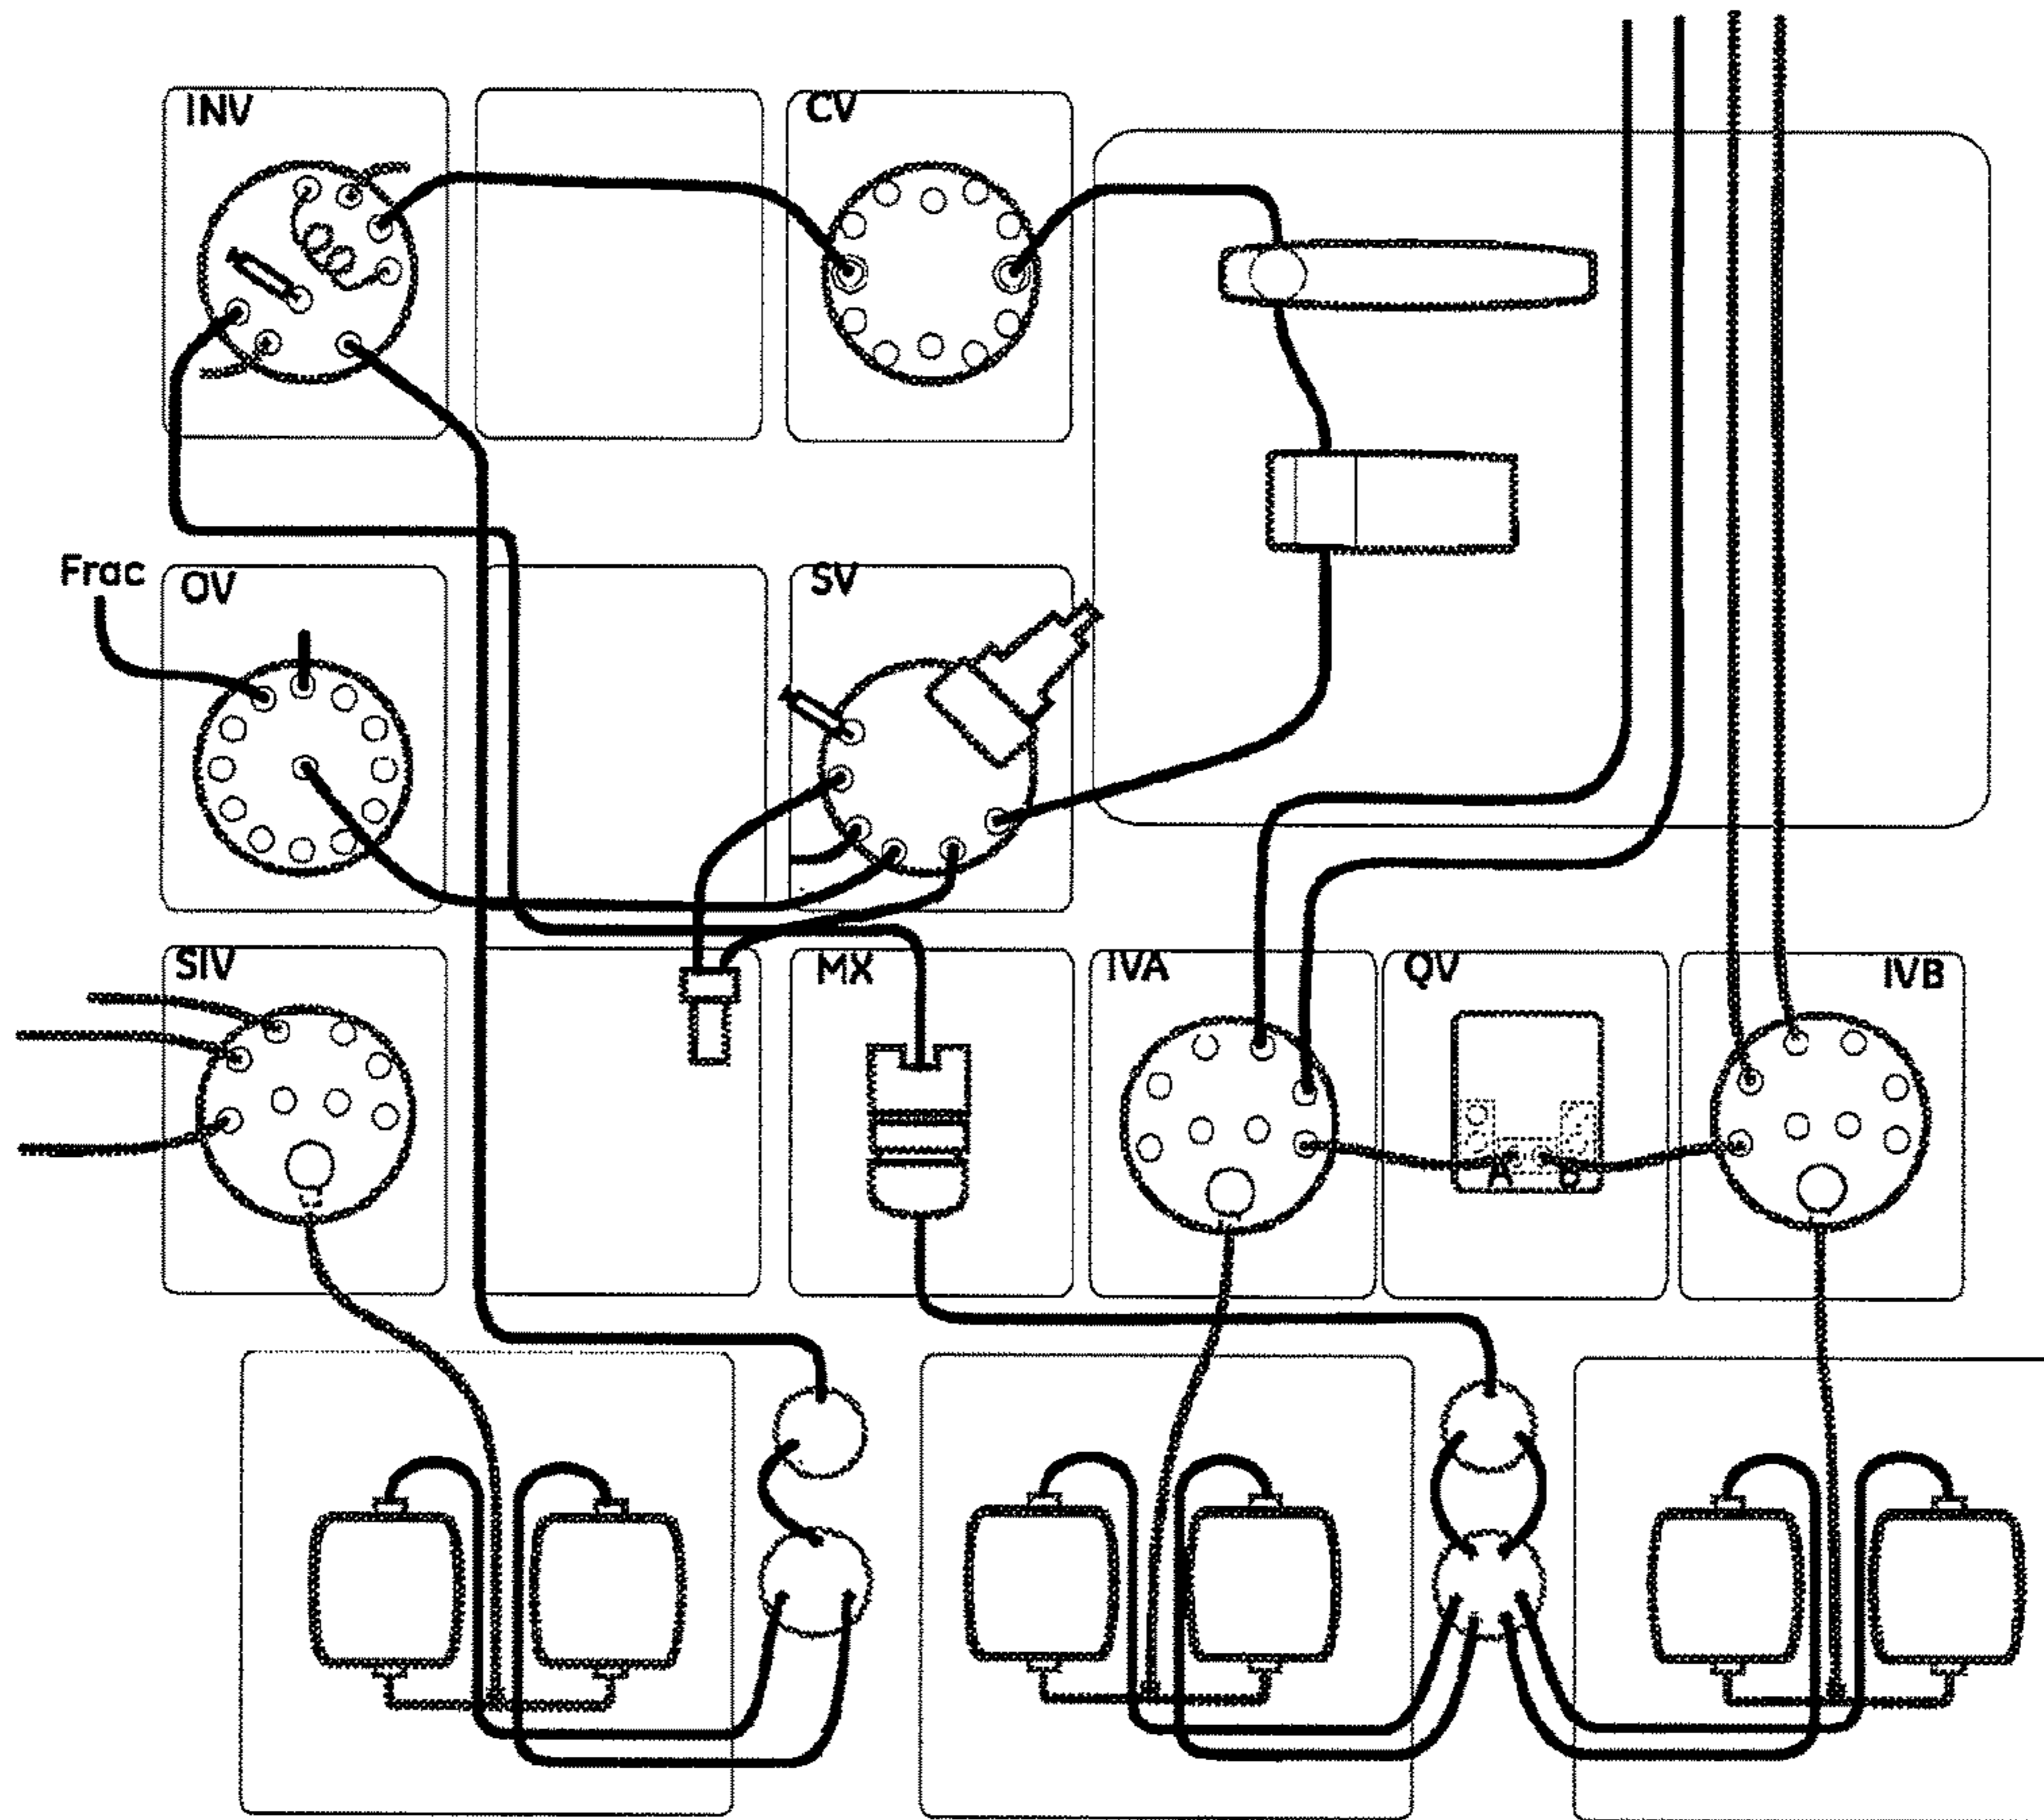


Fig. 10

## AUTOMATED FLUID HANDLING SYSTEM

**Matter enclosed in heavy brackets [ ] appears in the original patent but forms no part of this reissue specification; matter printed in italics indicates the additions made by reissue; a claim printed with strikethrough indicates that the claim was canceled, disclaimed, or held invalid by a prior post-patent action or proceeding.**

## CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a filing under 35 U.S.C. §371 and claims priority to international patent application number PCT/SE2010/050624 filed Jun. 4, 2010, published on Dec. 16, 2010 as WO 2010/144037, which claims priority to application number 0950431-7 filed in Sweden on Jun. 9, 2009.

## BACKGROUND OF THE INVENTION

The present invention relates to the art of fluid handling system systems, and in particular to an automated fluid handling system that is highly flexible and configurable. The fluid handling system may e.g. be a liquid chromatography system, a filtration system, a chemical synthesis system or the like.

There is a large range of fluid handling systems e.g. in laboratories. Such systems comprise a number of fluid handling units, e.g. one or more pumps, valves, mixers, sensor units etc of different types. Said fluid handling units are interconnected by fluid conduits in the form of, rigid or flexible tubes or the like. Even though some systems may be designed for a specific type of application with a specific flow path, there often exists a need for flexibility and ability to alter or optimize the fluid flow path of the system. Moreover, upgrading is often restricted to specific kits provided by the manufacturer, and upgrade kits often is supplied as external add-on equipment to be arranged besides the original system, thus enlarging the foot print of the system and that need to be connected to the system both fluidically and electrically (i.e. to a system control bus or the like). Moreover, replacement of defect fluid handling units is a time consuming and delicate task.

One type of liquid handling system is liquid chromatography systems which is a standard method in laboratories, and there are a broad range of liquid chromatography systems available on the market. Common to most of the present systems is the lack of flexibility in adapting the instrument to a variety of different applications.

## SUMMARY OF THE INVENTION

The object of the invention is to provide a new fluid handling system, which system overcomes one or more drawbacks of the prior art. This is achieved by the fluid handling system as defined in the independent claims.

One advantage with such a fluid handling systems is that the system may easily be upgraded without need for add-on equipment, and that the flow path may be easily optimized for new experimental setups.

Embodiments of the invention are defined in the dependent claims.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows one embodiment of a fluid handling system in the form of a liquid chromatography system, according to the present invention.

FIG. 2 is a schematic illustration of a housing with a liquid handling panel of the fluid handling system of FIG. 1.

FIG. 3 is a schematic illustration of the housing with the liquid handling panel of FIG. 2 with the modular components of the fluid handling system removed.

FIGS. 4a to 4d are schematic illustrations of examples of component modules of the fluid handling system removed.

FIGS. 5a and 5b show a schematic embodiment of an automated fluid handling system.

FIG. 6 is a schematic illustration of an embodiment of a housing with a modular liquid handling panel with the modular components of the fluid handling system removed.

FIGS. 7a and 7b are schematic illustrations of an embodiment of a modular housing with a liquid handling panel with the modular components of the fluid handling system removed.

FIG. 8 is a schematic illustration of an embodiment of the system architecture of one embodiment of a fluid handling system according to the present invention.

FIG. 9 is a schematic illustration of an embodiment of a master control unit of one embodiment of a fluid handling system according to the present invention.

FIG. 10 is a schematic illustration of one embodiment of a fluidic interconnection arrangement between the modular components of the liquid handling panel for the liquid chromatography system of FIG. 1.

## DETAILED DESCRIPTION OF THE INVENTION

According to one embodiment, there is provided an automated fluid handling system comprising a housing and two or more fluid handling units arranged as interchangeable modular components with an external fluidics section and an internal non fluidics section, and wherein the housing comprises a liquid handling panel with two or more of component positions for receiving said interchangeable modular components such that the external fluidics section is separated from the non fluidics section by the liquid handling panel.

According to another embodiment, there is provided a fluid handling system in the form of a liquid chromatography system comprising a housing, two or more high pressure pumps, at least one sensor unit and a plurality of fluid control valves of at least two different configurations, wherein at least the fluid control valves are arranged as interchangeable modular components and the housing comprises a liquid handling panel with a plurality of component positions for receiving said modular components.

FIG. 1 shows one embodiment of an automated fluid handling system modular in the form of a liquid chromatography system, with a plurality of interchangeable modular components arranged in a liquid handling panel wherein the reference numbers denotes:

1. Injection valve
2. Column valve with integrated pressure sensors
3. Conductivity monitor
4. UV monitor
5. Quaternary valve
6. Inlet valve B with integrated air sensor
7. System pump
8. Pressure monitor, system pump
9. Inlet valve A with integrated air sensor
10. System pump
11. Pressure monitor, sample pump
12. Sample pump
13. Rinsing system

- 14. Mixer with online filter
- 15. Sample inlet valve with integrated air sensor
- 16. Flow restrictor
- 17. pH valve
- 18. Outlet valve

The disclosed embodiment is supplied with three high precision pumps **7**, **10**, **12**. There are two System pumps **7**, **10**, System pump A **10** and System pump B **7**, and one Sample pump **12**. The System pumps **7**, **10** may be used individually, or in combination to generate isocratic or gradient elution in purification methods. The Sample pump **12** is dedicated for direct loading of sample onto a column, or for filling of sample loops.

Function of the Pumps:

Each pump module consists of two pump heads (not shown). The individual heads are identical but actuated in opposite phase to each other by individual stepper motors, controlled by a microprocessor. The two pistons and pump heads work alternately to give a continuous, low pulsation, liquid delivery. The flow rate of the two System pumps may be varied between about 0.001 ml/min and 25.000 ml/min and the maximum operating pressure is about 20 MPa. The flow rate of the Sample pump may e.g. be varied between 0.01 and 25 ml/min and according to one embodiment the maximum operating pressure is 10 MPa.

According to one embodiment, the plurality of fluid control valves of at least two different configurations are valves of rotary type. Such a motorized rotary valve may consist of a Valve head with a number of defined bores with channels to the inlet and outlet ports of the valve. The Rotary disc, mounted on the motor, has a number of defined channels. The pattern of channels of the Rotary disc together with the pattern and location of the ports of the Valve head, define the flow path and function of each type of valve. When the Rotary disc turns, the flow path in the valve changes.

One embodiment of fluid control valves are Inlet valves A and B (**9**, **6** respectively) that are used to select which buffers or samples to use in a run, and Sample inlet valve **15** that is located before Sample pump **12**. Inlet valve A **9** **1** is located before System pump A **10**, inlet valve B **6** is located before System pump B **10**, and Sample inlet valve **15** is located before Sample pump **12**. Inlet valve A and Inlet valve B are connected to another embodiment of a fluid control valve in the form of a Quaternary valve **5**. The Quaternary valve is used for automatic buffer preparation, and for formation of quaternary gradients. The number of inlets can be increased by installing component modules with extra inlet valves. Inlet valve A and Inlet valve B enable automatic changing between different buffers and wash solutions, and can be used to generate gradients by mixing buffer A and buffer B. The air sensors integrated in Inlet valve A and Inlet valve B can be used to prevent introduction of air into the pumps and columns.

The Quaternary valve is used for automatic mixing of four different solutions. The Quaternary valve opens one inlet port at a time, and the different solutions are mixed in a Mixer **14** to form the desired buffer. The opening time in the switching valve is controlled by the system. The volume for each inlet port opening increases stepwise when the flow increases. To obtain a homogeneous buffer composition, one has to make sure to use a mixer chamber volume suitable for the flow rate of the method.

The Quaternary valve can be used to create a gradient using four different solutions simultaneously in any combination. The percentage of each solution is controlled by instructions in the method. It is possible to form gradients

that changes the percentage of two, three or four solutions linearly over time. This is useful when advanced methods are developed.

The Sample inlet valve **15** enables automatic loading of different samples when using the Sample pump **12** to inject sample directly onto the column or to fill a sample loop. The Sample inlet valve has an inlet dedicated for buffer. This Buffer inlet is used in methods to fill the Sample pump with solution before sample is introduced. The Buffer inlet is also used to wash the Sample pump with buffer between runs. The air sensor integrated in the Sample inlet valve is e.g. used when sample is applied from a vessel onto a column by selecting Inject all sample using air sensor in the Sample application phase of a method. This function uses the Buffer inlet is used to finalize sample injection and to remove air from the Sample pump.

Still another embodiment of fluid control valve may be an Injection valve **1**, which is used to direct sample onto the column. The valve enables usage of a number of different sample application techniques. A sample loop can be connected to the Injection valve and filled either automatically using the Sample pump or manually using a syringe. The sample can also be injected directly onto the column using the Sample pump.

Still another embodiment of fluid control valve may be a Column valve **2** that is used for connection of columns to the system, and to direct the flow onto the column. Up to five columns can be connected to the disclosed embodiment of said valve simultaneously. The valve also has a built-in bypass capillary that enables bypassing of connected columns.

The number of column positions can be increased by installing an extra Column valve. Both top and bottom of each column shall be connected to the Column valve. The top of the column shall be connected to one of the A ports (e.g., **1A**), and the bottom of the column shall be connected to the corresponding B port (e.g., **1B**). The flow direction can be set either from the top of the column to the bottom of the column, Down flow, or from the bottom of the column to the top of the column, Up flow. In the default flow path of the Column valve the columns are bypassed. Pressure monitors that measures the actual pressure over the column are integrated into the inlet and outlet ports of the Column valve.

Still another embodiment of fluid control valve may be a pH valve **17** that has an integrated flow cell where a pH electrode can be installed. This enables in-line monitoring of pH during the run. A flow restrictor is connected to the pH valve and can be included in the flow path to generate a backpressure high enough to prevent formation of air bubbles in the UV flow cell. The pH valve is used to direct the flow to the pH electrode and to the flow restrictor, or to bypass one or both.

Still another embodiment of fluid control valve may be an Outlet valve **18** that is used to direct the flow to a Fraction collector (not shown), to any of e.g. 10 outlet ports, or to waste. The number of outlets can be increased by installing an extra Outlet valve.

A Mixer **14** may e.g. be located after System pump A and System pump B and before the Injection valve. The purpose of the Mixer is to make sure that the buffers from the System pumps are mixed to give a homogenous buffer composition. The Mixer has a built-in filter that prevents impurities from entering the flow path.

To fulfil a desired purpose, with the disclosed liquid chromatography system it is possible to adapt and extend the flow path in a simple and a flexible way. Up to three extra

## 5

fluid control valves or the like can be installed using the free valve positions. Dummy modules are installed in these positions at delivery. To obtain an optional flow path, it is also possible to move the standard fluid control valves to other positions. There are also two types of extra air sensors available which can be installed before Sample inlet valve or after Injection valve.

In the configuration disclosed in FIG. 1, 7 inlets are available for each inlet valve. To increase the number of inlets, an extra inlet valve can be installed which increases the number of inlets to 14 for one of the valves. This optional configuration can be convenient for example when a larger number of samples will be used. There is also a general type of inlet valve, Valve X, which can be used to increase the number of inlets to for example the Quaternary valve.

In the configuration disclosed in FIG. 1 with one column valve, 5 column positions are available. To increase the number of column positions to 10, an additional column valve can be installed in the instrument. An application can be to evaluate a number of different columns in method optimization.

In the configuration disclosed in FIG. 1 with one outlet valve, 10 outlet positions are available. To increase the number of outlets, one or two extra outlet valves can be connected, adding up to a total of 21 or 32 outlet positions. This optional configuration is convenient when collecting a number of large fractions outside the fraction collector.

Optional modules are easy to install in the disclosed modular liquid chromatography system. The dummy module is removed with a hexagon wrench and a bus cable is disconnected. The bus cable is connected to the optional fluid control valve or the like which is assembled in the instrument. The module is then added to the System properties in the control software. The available optional modules may e.g. be pre-configured to give the desired function. However, the function of a valve may e.g. be changed by changing the Node ID.

FIG. 2 is a schematic illustration of a housing 20 with a liquid handling panel 22 of the fluid handling system in the form of a modular liquid chromatography system 100 of FIG. 1. In FIG. 2 some components have been removed for clarity reasons. In the disclosed configuration, as disclosed in detail above, the modular liquid chromatography system 100 comprises a plurality of fluid control valves in the form of: Injection valve 1, Column valve 2, Quaternary valve 5, Inlet valve B 6, Inlet valve A 9, Sample inlet valve 15, pH valve 17, and Outlet valve 18. The chromatography system 100 further comprises UV monitor 4, System pump B 7, System pump A 10, Sample pump 12, Mixer 14, and three Dummy modules 24. According to one embodiment, all liquid handling components and sensors arranged at the liquid handling panel 22 are designed to be readily interchangeable. The interchangeability provides improved service and upgrade possibilities and also a possibility to customize the positions of the respective liquid handling components, such as the fluid control valves, e.g. in order to optimize the fluid path for a specific experimental setup. As is illustrated in FIG. 2, there are three large component positions e.g. for pump modules, one UV-sensor position and 9 standard component positions, e.g. for fluid control valves or the like. The component positions are given a standardized size and shape to provide simple interchangeability. According to one embodiment, each modular component is retained in a mating component position by a single screw, and it is connected to the master control unit by a single bus cable providing both communication and system power to each component. FIG. 3 is a schematic

## 6

illustration of the housing with the liquid handling panel of FIG. 2 with the modular components of the liquid chromatography system removed.

FIGS. 4a to 4d are schematic illustrations of examples of fluid handling units in the form of modular component of the fluid handling system removed. FIG. 4a shows a standard interchangeable modular component 26, e.g. a fluid control valve or the like. The standard component module 26 comprises a panel member 28, an external fluidics section 30 and an internal non-fluidics section 32. According to one embodiment, the panel member 28 essentially separates the fluidics in the external fluidics section 30 from electronics and control means in the internal non-fluidics section 32.

FIG. 4b shows a Dummy module 24, which is intended to be placed in non used standard component positions. In the disclosed embodiment, the Dummy modules are provided with mounting grooves for attachment of accessories to the system. In the disclosed embodiment the dummy module is shown as a panel member 28 without any internal section FIGS. 4c and 4d shows a pump module and an UV-module, respectively, each having an external fluidics section 30 and an internal non-fluidics section 32.

As is disclosed in FIGS. 4a to 4d, the interchangeable modular components 26 comprises a panel member arranged to separate the fluidics section from the non fluidics section and for attachment to a component position in the liquid handling panel. Said panel attachment member may be arranged so that all fluid connections of said modular component are arranged on a wet side of the panel attachment member separating them from electrical components that are arranged on a dry side thereof, hence providing a high degree of liquid resistance at the external part of the fluid handling panel, and so that the liquid resistance requirements for the internal sections may be somewhat lightened. According to one embodiment, the interchangeable modular components are sealed against the liquid handling panel by a sealing member. According to another embodiment, not shown, the modular component does not comprise any panel member, but there is provided a suitable sealing arrangement between the component position openings of the liquid handling panel and the external surface of the interchangeable modular components 26. In the disclosed embodiments, the component position openings of the liquid handling panel and the interchangeable modular components 26 are shown to have an essentially rectangular cross sectional shape, but other shapes may be equally applicable.

According to one embodiment, there is provided a general fluid handling system comprising a housing and two or more fluid handling units arranged as interchangeable modular components as is schematically disclosed in FIG. 5a. As discussed above such a system may be configured for essentially any type of automated liquid handling operations provided that suitable fluid handling units are provided as interchangeable modular components for the system. According to one embodiment there is provided an automated fluid handling system comprising at least one fluid pump, at least one sensor unit and two or more fluid control valves of at least two different configurations, wherein at least the fluid control valves are arranged as interchangeable modular components.

The liquid handling panel 22 of the fluid handling system may e.g. be designed in any suitable manner to allow the modular components to be arranged in an efficient manner. FIGS. 5a and 5b shows a schematic embodiment of an automated fluid handling system wherein the housing 20 comprises an internal climate panel 29 arranged at a distance



behind the liquid handling panel 22 defining an air inlet compartment 35 and air outlet compartment 37 in the housing 20, the climate panel 29 being provided with complementary component positions 39 for receiving the internal non fluidics section 32 of the interchangeable modular components 26, and wherein the non-fluidics section 32 of at least one interchangeable modular component is provided with one or more air inlet openings 31 located in the air inlet compartment 35 and one or more air outlet openings 33 located in the air outlet compartment 37 when the interchangeable modular component arranged in position in the component position. FIG. 5b shows the fluid handling system of FIG. 5a in a schematic cross sectional view. As is indicated by inlet vent 41 and outlet vent 43, air for cooling interchangeable modular components 26 provided with air inlet and outlet openings 31, 33 is preferably arranged to enter the air inlet compartment 35 at a distance from the outlet vent 43 in order to avoid recirculation of air. The air circulation in the system may be achieved by a system cooling unit (not shown) providing a flow of air from the air inlet compartment 35 to the air outlet compartment 37, through the at least one interchangeable modular component 26. Alternatively, the at least one interchangeable modular component 26 is provided with a local cooling unit (not shown) providing a flow of air from the air inlet compartment 35 to the air outlet compartment 37. As is indicated, the complementary component positions 39 are arranged to provide a relatively air flow tight fit with respect to the internal non fluidics section 32 of the interchangeable modular components 26, and according to one embodiment, this may be achieved by a sealing arrangement. In FIG. 5b, there is shown a sealing member 45 for sealing the interchangeable modular components 26 with respect to the liquid handling panel 22, as discussed above. Other sealing member arrangements may be envisaged by a person skilled in the art. According to one embodiment, fluids are strictly restricted to the fluidics section 30 of the interchangeable modular component 26, but in alternative embodiments, only fluid connections are restricted to the fluidics section 30 allowing fluid to "cross" the fluid handling panel inside the non-fluidics section 30 of the interchangeable modular component 26.

In FIG. 5b there is further shown a master control unit 40 and buss connectors 42 for connecting the interchangeable modular components 26 to the master control unit 40. According to one embodiment, the component positions including the buss connectors 42 and the interchangeable modular components 26 are of plug and play configuration with respect to each other.

FIG. 6 is a schematic illustration of an embodiment of a housing 20 with a modular liquid handling panel 22 with the modular components of the liquid chromatography system removed. In the disclosed embodiment, also the layout of the liquid handling panel 22 is configurable by means of two interchangeable panel sections 34 which may be selected in accordance with the desired layout of the system. In FIG. 6 two different layouts of the interchangeable panel sections are disclosed, but the layout may include any suitable configuration.

FIGS. 7a and 7b are schematic illustrations of an embodiment of a modular housing with a liquid handling panel with the modular components of the liquid chromatography system removed. In the disclosed embodiment, the modular housing is comprised of a main housing 36 that comprises the master control unit including power supply and climate control for the whole housing, two expansion housing modules 38 and a side member 40. This approach provides very

flexible expansion possibilities for the chromatography system, while preserving the benefits of a single master control unit including power supply and climate control.

FIG. 8 is a schematic illustration of an embodiment of the system architecture of one embodiment of a modular liquid chromatography system according to the present invention. As mentioned above, the chromatography system may comprise a master control unit 40 arranged to communicate with all modular components e.g. 1-26, over a system bus 42 such as a CAN-bus or the like. In one embodiment, each modular component is provided with a dedicated CPU unit allowing the component to independently perform operations in response to instructions over the BUS 42. In order to minimize the number of connectors to be attached to each modular component, the bus 42 further comprises power feed for the modular components. The Bus 42 may be connected to any suitable number of modular components arranged in the housing 20, but also to one or more modular components 44 outside of the housing 20 or the like. As is mentioned briefly above, the master control unit may further be arranged to control the climate in the housing. In addition to the disclosed modular components, other components of the chromatography system, e.g. a fraction collector or the like, may be arranged in the housing and the controlled climate therein.

According to one embodiment, different component modules are automatically identified by the master control unit, whereby they may be moved essentially freely between different positions. Moreover, the master control unit may be arranged to provide said information to Chromatography control software whereby experimental setup and planning may be performed. In one embodiment, the control system may be arranged to provide an optimized layout of the component modules with respect to the present layout of the liquid handling panel and available component modules for a specific experimental setup.

According to one embodiment, the interchangeable panel sections 34 of FIG. [5] 6 and the expansion housing modules 38 of FIGS. [6a] 7a and [6b] 7b may be provided with means for automatic detection of the same to allow automatic configuration of the system by the master control unit 40. In one embodiment, each interchangeable panel section 34 and expansion housing module 38 comprises a hub (not shown) for connection to the system bus 42 in order to expand the system bus 42 network to the number of component modules in each interchangeable panel section 34 or expansion housing module 38.

FIG. 9 is a schematic illustration of an embodiment of a master control unit of one embodiment of a modular liquid chromatography system according to the present invention. The master control unit 40 comprises a system controller 46 for communicating with internal and external components and control computers (not shown) etc. According to one embodiment, the system controller comprises a suitable CPU 48, a bus controller 52, an external communications controller 50, such as a LAN unit, and a storage device 54. The bus controller 52 is providing communication with the component modules. The master control unit may further comprise a Power supply 56 and a climate controller 58 arranged to keep the internal climate in the housing 20 at a predetermined level as discussed above.

FIG. 10 is a schematic illustration of one embodiment of a fluidic interconnection arrangement between the modular components of the liquid handling panel. Taking into account the complexity of the disclosed interconnection arrangement, the benefit of optimizing the fluid paths in alternative configurations of the system becomes evident.

The task of optimizing the fluid paths may e.g. be performed to reduce the total length/volume of the fluid paths/tubing arranged to interconnect the different component modules in the system. Alternatively the optimization may be performed to minimize the length/volume of one or more specific fluid paths, such as the sample output path from the column to the fraction collector, in order to minimize dispersion of the fractionized sample.

The invention being thus described, it will be obvious that the same may be varied in many ways. Such variations are not to be regarded as a departure from the spirit and scope of the invention, and all such modifications as would be obvious to one skilled in the art are intended to be included within the scope of the following claims.

What is claimed is:

**[1.** Automated fluid handling system comprising a housing and two or more interchangeable fluid handling units the housing comprising a liquid handling panel including two or more component positions for receiving said interchangeable units, wherein said units are arranged as interchangeable modular components, and include:

- a fluidics section;
- a non fluidics section comprising electronics or electrical components or control means; and
- a panel member arranged to separate the fluidics section from the non fluidics section and for attachment of the modular component to a component position of the liquid handling panel,

and wherein the two or more component positions of the liquid handling panel are arranged for attachment of the panel members such that said respective fluidics sections are external to the housing and said respective non fluidics sections are internal to the housing.]

**[2.** The fluid handling system of claim 1, wherein the interchangeable modular components are sealed against the liquid handling panel by a sealing member.]

**[3.** The fluid handling system of claim 1, comprising a master control unit wherein the interchangeable modular components are connected to the master control unit by a system bus providing electrical communication to each interchangeable modular component.]

**[4.** The fluid handling system of claim 1, wherein all interchangeable modular components are of same size.]

**[5.** The fluid handling system of claim 1, wherein the interchangeable modular components are of two or more sizes.]

**[6.** The fluid handling system of claim 1, comprising at least one fluid pump, at least one sensor unit and two or more fluid control valves of at least two different configurations, wherein at least the fluid control valves comprise said interchangeable modular components.]

**[7.** The fluid handling system of claim 3, wherein the master control unit comprises a system climate controller for controlling the climate in the housing and the interchangeable modular components.]

**[8.** The fluid handling system of claim 1, wherein the housing comprises an internal climate panel arranged spaced from the liquid handling panel within the housing, said internal climate panel defining on one side an air inlet compartment and defining on an opposing side an air outlet compartment in the housing, the climate panel being provided with complementary component positions for receiving the internal non fluidics section of the interchangeable modular components, and wherein the non-fluidics section of at least one interchangeable modular component is provided with one or more air inlet openings located in the air inlet compartment and one or more air outlet openings

located in the air outlet compartment when the interchangeable modular component is arranged in position in the component position.]

**[9.** The fluid handling system of claim 8, further comprising a system cooling unit providing a flow of air from the air inlet compartment to the air outlet compartment, through said at least one interchangeable modular component.]

**[10.** The fluid handling system of claim 8, wherein said at least one interchangeable modular component is provided with a local cooling unit providing a flow of air from the air inlet compartment to the air outlet compartment.]

**[11.** The fluid handling system of claim 1, wherein the system is a liquid chromatography system arranged to provide a controlled fluid flow through a chromatography column.]

**[12.** The fluid handling system of claim 1, wherein the system is a liquid filtration system.]

**[13.** The fluid handling system of claim 1, wherein the system is a chemical synthesis system.]

**[14.** The fluid handling system according to claim 1 wherein the system further comprises at least one expansion housing module for accommodating additional interchangeable modular components.]

**[15.** The fluid handling system according to claim 14, further including means for automatic detection of said module to allow automatic configuration of the system by a master control unit.]

**16.** A liquid chromatography system arranged to provide a controlled fluid flow through a chromatography column, the system comprising a housing and two or more interchangeable fluid handling units, the housing comprising a liquid handling panel including two or more component positions for receiving said interchangeable units, wherein said units are arranged as interchangeable modular components, and include:

- a fluidics section;
- a non fluidics section in turn comprising electronics or electrical components or control means; and
- a panel member arranged to separate the fluidics section from the non fluidics section and for attachment of the modular component to a component position of the liquid handling panel,

and wherein the liquid handling panel of the housing and the panel members are arranged such that the fluidics sections are external to the housing and respective non fluidics sections are internal to the housing.

**17.** The liquid chromatography system according to claim 16, wherein the interchangeable modular components include at least **[one]** *two* of: an injection valve; a column valve with integrated pressure sensors; a conductivity monitor; a UV monitor; a quaternary valve; an inlet valve with integrated air sensor; a system pump; a pump pressure monitor; **[an inlet valve with integrated air sensor]**; a rising valve; a mixer; a filter; a sample inlet valve; a flow restrictor; a pH valve; an outlet valve; **[and]** *or* a dummy component.

**18.** The liquid chromatography system according to claim 17, wherein said modular components are interconnected fluidically on the external side of the panel.

**19.** *The liquid chromatography system of claim 16, wherein the interchangeable modular components are sealed against the liquid handling panel by a sealing member.*

**20.** *The liquid chromatography system of claim 16, comprising a master control unit wherein the interchangeable modular components are connected to the master control unit by a system bus providing electrical communication to each interchangeable modular component, and wherein*

each of the interchangeable modular components includes a dedicated CPU unit allowing each of the interchangeable modular components to independently perform operations in response to instructions over the bus.

21. The liquid chromatography system of claim 16, wherein all interchangeable modular components are of same size.

22. The liquid chromatography system of claim 16, wherein the interchangeable modular components are of two or more sizes.

23. The liquid chromatography system of claim 16, comprising at least one fluid pump, at least one sensor unit and two or more fluid control valves of at least two different configurations, wherein at least the fluid control valves are arranged as interchangeable modular components.

24. The liquid chromatography system of claim 20, comprising at least one fluid pump, at least one sensor unit and two or more fluid control valves of at least two different configurations, wherein at least the fluid control valves are arranged as interchangeable modular components.

25. The liquid chromatography system of claim 16 wherein the system further comprises at least one expansion housing module for accommodating additional interchangeable modular components at the liquid handling panel.

26. The liquid chromatography system of claim 16, wherein the housing includes at least four component positions.

27. The liquid chromatography system of claim 26, wherein the at least four component positions are arranged in a two dimensional array.

28. The liquid chromatography system of claim 16, comprising  
two double piston pumps,  
one injection valve for injecting sample onto a column  
connecting to the flow path of the liquid chromatography system,  
a UV monitor, and  
a mixer.

29. The liquid chromatography system of claim 28, wherein the pump, valve, monitor, and mixer are interchangeable modular components.

30. The liquid chromatography system of claim 28, wherein the system further includes  
a pH-valve with an integrated flow cell for in-line monitoring of pH levels, and  
a quaternary valve for automatic buffer preparation and formation of quaternary gradients.

31. The liquid chromatography system of claim 25, wherein the expansion housing module is attached to the housing and comprises two or more component positions adapted to receive additional interchangeable modular components at the liquid handling panel.

32. The liquid chromatography system of claim 31, wherein the component positions of the expansion housing module are arranged to receive interchangeable modules of the same size.

33. The liquid chromatography system of claim 31, wherein the component positions of the expansion housing module are arranged to receive interchangeable modules of two or more sizes.

34. The liquid chromatography system of claim 31, wherein the component positions of the expansion housing module comprise at least four component positions.

35. The liquid chromatography system of claim 16, wherein the fluidics section comprises one or more fluid connectors for connecting the interchangeable fluid handling unit to a fluid flow path of the liquid chro-

matography system, and the non fluidics section comprises an enclosure housing the with one or more air inlet openings.

36. The liquid chromatography system of claim 20, wherein the internal fluidics section comprises a bus connector for directly connecting the interchangeable modular component with the system bus, and each component position includes a complementary connector for connecting the bus connector of the interchangeable modular component inserted therein to said system bus.

37. The liquid chromatography system of claim 16, wherein said housing is adapted to accommodate at least one pump, at least one sensor unit and at least two fluid control valves of different configurations, of which at least two are interchangeable modular components.

38. A liquid chromatography system arranged to provide a controlled fluid flow through a chromatography column, the system comprising a housing, a master control unit connected to a system bus, two double piston pumps, and two or more interchangeable fluid handling units, the housing comprising a liquid handling panel including two or more component positions for receiving said interchangeable units, wherein said units are arranged as interchangeable modular components, and include:

a fluidics section;  
a non fluidics section in turn comprising electronics or electrical components or control means, and including a bus connector for directly connecting the interchangeable modular component with the system bus;  
and

a panel member arranged to separate the fluidics section from the non fluidics section and for attachment of the interchangeable modular component to a component position of the liquid handling panel,

wherein the liquid handling panel of the housing and the panel members are arranged such that the fluidics sections are external to the housing and respective non fluidics sections are internal to the housing,

wherein each component position includes a complementary connector for connecting the bus connector of the interchangeable modular component inserted therein to said system bus,

wherein each interchangeable modular component includes a dedicated CPU unit allowing the interchangeable modular component to independently perform operations in response to instructions over the system bus,

wherein the master control unit is arranged to automatically identify interchangeable modular components, wherein the system includes at least a valve and a mixer as interchangeable modular components, wherein the system is capable of performing automated liquid chromatography.

39. The liquid chromatography system according to claim 38, wherein said interchangeable modular components are interconnected fluidically on the external side of the panel.

40. The liquid chromatography system of claim 38, wherein the interchangeable modular components are sealed against the liquid handling panel by a sealing member.

41. The liquid chromatography system of claim 38, wherein the housing includes at least four component positions arranged in a two dimensional array.

42. The liquid chromatography system of claim 38, wherein the system further comprises at least one expansion housing module for accommodating additional interchangeable modular components at the liquid handling panel.

43. The liquid chromatography system of claim 38, wherein said housing is further adapted to include at least one sensor unit and at least two fluid control valves of different configurations, of which at least the sensor unit, and the fluid control valves are interchangeable modular 5 components.

44. The liquid chromatography system of claim 38, wherein the fluidics section comprises one or more fluid connectors for connecting the interchangeable fluid handling unit to a fluid flow path of the liquid chromatography 10 system, and the non fluidics section comprises an enclosure housing the with one or more air inlet openings.

\* \* \* \* \*